



(11) **EP 3 422 936 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:

03.04.2019 Bulletin 2019/14

(21) Application number: **17818598.9**

(22) Date of filing: **08.11.2017**

(51) Int Cl.:

A61B 5/05 (2006.01) **A61B 5/15** (2006.01)
A61B 5/145 (2006.01) **A61B 5/1477** (2006.01)
A61B 5/151 (2006.01) **A61B 5/157** (2006.01)
A61B 5/00 (2006.01)

(86) International application number:

PCT/FI2017/050767

(87) International publication number:

WO 2018/091771 (24.05.2018 Gazette 2018/21)

(54) **DEVICE FOR SAMPLING ONE OR MORE ANALYTES**

VORRICHTUNG ZUR ENTNAHME EINES ODER MEHRERE ANALYTE

DISPOSITIF D'ÉCHANTILLONNAGE D'UN OU PLUSIEURS ANALYTES

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **21.11.2016 FI 20165876**

(43) Date of publication of application:

09.01.2019 Bulletin 2019/02

(73) Proprietor: **GlucModicum Oy**

00560 Helsinki (FI)

(72) Inventors:

- **GARCIA PEREZ, Alejandro**
00710 Helsinki (FI)

• **NIEMINEN, Heikki**

00170 Helsinki (FI)

• **HAEGGSTRÖM, Edward**

00140 Helsinki (FI)

(74) Representative: **Finnpatent Oy**

Smart Chemistry Park

Raisio Kaari 55

21200 Raisio (FI)

(56) References cited:

WO-A1-2017/021585 WO-A2-2010/001122

US-A1- 2002 002 328 US-A1- 2011 037 325

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

FIELD

[0001] This invention relates to devices based on magneto-hydrodynamics (MHD) to extract fluid comprising one or more analytes from a target, in particular, interstitial fluid from skin.

BACKGROUND

[0002] Interstitial fluid (IF) is an aqueous solution that serves as a transport medium for e.g. glucose and electrolytes between the cells and the circulatory system. Therefore, the concentration of different solutes, such as glucose and lactic acid, in IF and in blood exhibits a substantial correlation. This makes the analysis of IF relevant to many developing fields, including, medical diagnosis, early disease detection, pharmacokinetics, and smart wearable technologies. Furthermore, a strong commercial and scientific interest promotes research on painless and non-invasive IF sampling methods.

[0003] US2002/0002328A1 discloses a noninvasive IF device and method for sampling substances such as glucose through skin by reverse iontophoresis. The device is designed to monitor blood glucose levels in people with diabetes. The device is not considered a replacement, but an addition to conventional invasive blood glucose monitoring.

[0004] WO2010001122A2 discloses a patch for sampling one or more analytes through the skin of a patient. The patch comprises an electrode layer that is positioned adjacent to the skin of a patient, and means for actuating an electrode layer to induce the withdrawal of analyte through the skin by reverse iontophoresis. The patch comprises reservoir chambers containing an electrically conducting medium to induce the process of iontophoresis.

[0005] According to the document, the presence of an electrolyte in liquid form ensures good conductivity between the electrodes and the skin, which enhances the effectiveness of the reverse iontophoresis process.

[0006] The state-of-the-art devices discussed above for noninvasive glucose monitoring are based on the harnessing of osmotic flow or electrophoresis. In these devices, the extraction occurs locally at the electrode-skin interface. Accordingly, a limited volume of fluid can be extracted and analyzed, which in turn requires sensitive detection and analysis techniques.

[0007] Thus, there is still need for further devices for sampling analytes through skin with improved efficacy and extraction rate.

SUMMARY

[0008] The present invention is based on the observation that at least some of the state-of-the-art problems related to sampling of one or more analytes from skin

can be solved or at least alleviated by exploiting the magneto-hydrodynamic (MHD) phenomenon.

[0009] Accordingly, it is an object of the present invention to provide a device for sampling interstitial fluid comprising one or more analytes from dermis to skin surface in a non-invasive manner, the device comprising

- a first electrode and a second electrode adapted to be positioned adjacent to the skin surface, the first electrode separated from the second electrode by a distance,
- a power source adapted to induce electric current through the first electrode, the interstitial fluid and the second electrode, and
- one or more magnets adapted to induce magnetic field to the interstitial fluid.

[0010] According to the device of the present invention direction of the magnetic field produced by the one or more magnets, and direction of the electric current produced by the power source is adapted to be such that Lorentz force produced by the magnetic field and the electric current is adapted to drive the interstitial fluid from the dermis substantially towards the skin surface.

[0011] According to the device of the present invention, the IF can be sampled from the skin not only locally at the electrode-skin interface as in the state of the art, but also between the electrodes, where a further volume of IF is available. Furthermore, MHD adds a force component that increases the extraction rate under a negative electrode.

[0012] Further objects of the present invention are described in the accompanying dependent claims.

[0013] Exemplifying and non-limiting embodiments of the invention, both as to constructions and to methods of operation, together with additional objects and advantages thereof, are best understood from the following description of specific exemplifying embodiments when read in connection with the accompanying drawings.

[0014] The verbs "to comprise" and "to include" are used in this document as open limitations that neither exclude nor require the existence of un-recited features. The features recited in the accompanied depending claims are mutually freely combinable unless otherwise explicitly stated. Furthermore, it is to be understood that the use of "a" or "an", i.e. a singular form, throughout this document does not exclude a plurality.

BRIEF DESCRIPTION OF THE DRAWINGS

[0015]

Figure 1 illustrates the principle of the device according to the present invention for sampling e.g. extracting an analyte such as glucose (black dots) from skin; (+): the first electrode; (-): the second electrode; dot-

ted arrow: direction of electric current; (B): magnetic field; upper layer: the epidermis; middle layer: dermis; lower layer: hypodermis; white arrows: fluid displacement in the direction of the Lorentz force; black arrows: direction of electrophoresis,

figure 2 illustrates an exemplary non-limiting device according to the present invention,

figure 3 illustrates exemplary non-limiting electrode shapes,

figure 4 illustrates an exemplary magnet array suitable for use in the device according to the present invention,

figure 5 illustrates a schematic view of a non-limiting exemplary device in form of a wristband according to the present invention, and

figure 6 illustrates result of treatment of a skin sample using an exemplary device of the present invention (MHD to the left) and by using a device according to state of the art (electrophoresis to the right).

DESCRIPTION

[0016] According to one embodiment, the present invention concerns a device for sampling IF in a non-invasive manner. The IF comprises one or more analytes to be analyzed. According to the invention, the IF is extracted from the skin by exploiting the MHD phenomenon.

[0017] Figure 1 shows the working principle of the present invention. In the figure, the device serves to extract IF from skin. Accordingly, an electric current produced by a power source is established through a pair of electrodes (marked with + and -) and the skin. The magnetic field (B) is produced by a magnet. The current density in the middle skin layer (dermis) is substantially higher than in the inner (hypodermis) or outer (epidermis) skin layers because the higher content of IF in the dermis offers a lower impedance electric path. When the device is in operation, the direction of the magnetic field is substantially perpendicular to the skin surface, particularly within the distance and at the location of the electrodes, and substantially perpendicular to desired direction of fluid displacement from the dermis to the skin surface. Therefore, the current-carrying fluid in the magnetic field experiences a Lorentz force towards the skin surface. This force serves to drive IF out of the skin. The driving force exerted in the fluid is described by the equation $F = J \times B$; where F, J, and B are the force, current density, and magnetic field vectors respectively, and $\times$ indicates a cross product. Based on this equation, the vectors of Lorentz force, electric current, and magnetic field are all perpendicular to each other. Also, the force distribution is defined by the distribution of the electric current and the magnetic field. The distribution of Lorentz force in the

current carrying fluid permits directional driving of the IF out of the skin along the whole/entire current path i.e. along the distance between the electrodes. The fluid displacement in the direction of the Lorentz force is indicated with white big arrows. The IF containing relevant analytes, such as glucose, shown as black dots in the figure, is extracted also along the distance between the electrodes and not only under the negative electrode wherein also electrophoresis (black small arrows) promotes movement of fluid towards the electrode-skin interface.

[0018] An exemplary device according to the present invention is shown in figure 2. Accordingly, a device 100 for sampling IF comprising one or more analytes from dermis 101a to skin surface 101b comprises

- a first electrode and a second electrode adapted to be positioned adjacent to the skin surface, the first electrode separated from the second electrode by a distance 103,
- a power source 104 adapted to induce an electric current through the first electrode, the interstitial fluid and the second electrode, and
- a magnet 105 adapted to induce a magnetic field to the interstitial fluid, wherein direction of the magnetic field produced by the magnet and direction of the electric current produced by the power source is such that that Lorentz force is adapted to drive the interstitial fluid from the dermis substantially towards the skin surface along the entire current path, in particular within the distance and the (-)-electrode.

[0019] When the device is in operation, the electric current flows substantially in three different directions as described by the dotted arrow in figure 2: initially from the first electrode towards the skin, in particular towards the dermis comprising the IF, then within the distance between the electrodes, substantially parallel to the skin surface, and finally from the dermis towards the second electrode (i.e. the (-)-electrode), i.e. in -y-, x- and y-directions, respectively of the coordinate system 199 of figure 2. Accordingly, the electric current contributes to driving a certain volume of IF towards the second electrode.

[0020] In order to produce a Lorentz force in the current-carrying IF in the skin towards the skin surface, the magnet should produce a magnetic field that is substantially in z-direction of the coordinate system 199. Accordingly, the MHD effect produced by the magnetic field and the electric current drives the IF comprising the one or more analytes from the dermis substantially towards the skin surface within the distance and below the (-)-electrode 102b. Accordingly, the direction of the flow of the IF is substantially in y-direction of the coordinate system 199.

[0021] According to an exemplary embodiment the first electrode, and the second electrode is a silver-silver chloride (Ag-AgCl) electrode to avoid electrolysis of water and pH drifts. However, other inert and non-ferromagnetic materials are also suitable. Exemplary further ma-

materials are carbon, gold, and platinum.

[0022] The electrodes can be coated with different materials, for instance, enzymes and catalysts such as glucose oxidase, dehydrogenase and Prussian blue. Furthermore, different materials or combination of materials can be used as an interface between the electrodes and the skin for instance to reduce the electric impedance, to protect the electrode coating and to facilitate the analysis of the extracted IF samples. Suitable materials for this purpose include biocompatible membranes (*i.e.* permeable or semipermeable) made of regenerated cellulose, silicone and monofilament fabric of polyamide.

[0023] The interface serves to maintain a low electric impedance between the electrodes and the skin, to facilitate the transport of analytes towards the device, to preserve electrochemical conditions (*e.g.* pH) and activity of the enzyme. In one embodiment, the electrode skin interface is preferable a gel or hydrogel. In another preferred embodiment, the electrode skin interface is a membrane which is permeable or semipermeable, electrically conductive, and hypoallergenic. Exemplary materials suitable for this purpose include biocompatible membranes (*i.e.* permeable or semipermeable) made of regenerated cellulose, silicone and monofilament fabric of polyamide. These membranes can be treated with agents that work as humectants (*i.e.* glycerol, agarose gel and phosphate buffered saline) to help maintain the desired pose structure and to increase its electric conductivity. The membranes can also be loaded with agents, such as corticosteroids and other drugs, to prevent or reduce potential skin reactions induced by the extraction procedure.

[0024] According to the exemplary embodiment shown in figure 2, the first electrode 102a is acting as a positive electrode and the second electrode 102b is acting as a negative electrode. It is to be understood that the polarity of the electrodes can be flipped and that other configurations are possible. The first electrode and the second electrode are preferably substantially parallel to each other. The device may include plurality of first electrodes and plurality of second electrodes. The electrodes can be same of different.

[0025] The first electrode and the second electrode comprise a contact surface. The contact surfaces are shown in figure 2 with reference numbers 106a and 106b for the first electrode and the second electrode, respectively. According to one exemplary embodiment, the contact surface of the electrodes is flat and either circular *e.g.* disk-shaped, rectangular, elliptical or pyramidal. According to another embodiment the contact surface is adapted to the shape of the skin surface. For example, if the skin is in a finger or in the wrist, the contact surface may be substantially curved to allow maximal mechanical and electric contact with the skin. The contact surface may comprise extrusions and/or protrusions to facilitate maximal adherence to the skin surface.

[0026] The area of the contact surface of each electrode is preferably between 0.01 cm^2 and 9 cm^2 , and

most preferably between 0.15 cm^2 and 1 cm^2 . The distance between the first electrode and the second electrode is preferably between 1 mm and 5 cm, and most preferably between 5 mm and 3 cm. According to an exemplary embodiment the distance is 1 cm.

[0027] According to one embodiment, the shape of the contact surface of the electrodes is elliptical, and the major axis of the ellipsis is substantially larger than the minor axis. This allows to set a larger current density through the dermis without increasing the current density at the electrode-skin interface. Exemplary electrode shapes are shown in figure 3. This figure depicts five cases illustrating different electrode configurations (first electrode to the left, and second electrode to the right). The current density through the target such as skin can be different in all cases even if the contact area of the electrodes is the same. The electrode shape can alter the distribution of electric current in the skin, and therefore, the local current density to increase the Lorentz force and the extraction rate of IF. For this reason, the elliptical electrode shapes illustrated in case 3 are preferable.

[0028] The power source 104 can be a direct current (DC) power source and/or an alternating current (AC) power source that limits and regulates the energy *i.e.* the intensity of the electric current and/or voltage delivered through the electrodes. According to an exemplary embodiment, the power source is a floating current source that provides means to establish a direct electric current preferably in the range of $10 \text{ }\mu\text{A}$ to 10 mA, and more preferably in the range 0.1 mA to 1 mA. The current density at the electrode-target, such as skin interface is preferably between $1 \text{ }\mu\text{A}/\text{cm}^2$ and $10 \text{ mA}/\text{cm}^2$, and most preferably between $0.1 \text{ mA}/\text{cm}^2$ and $1 \text{ mA}/\text{cm}^2$. The voltage provided by the current source is preferable between 1 and 100 V.

[0029] In a particular embodiment, the electric current established by the floating current source exhibits a unipolar (unidirectional) or bipolar (*e.g.* bidirectional or alternating) waveform. The frequency of the electric signal is preferably between 0.1 Hz and 100 kHz, and more preferably between 10 Hz and 10 kHz. The electric signal can be modulated in amplitude and/or frequency, and can have different waveforms, for instance, sine, square, pulsed (*e.g.* rectangular), triangle, and saw tooth. Also, the signal can be burst- and/or duty-cycle-modulated.

[0030] The magnet 105 can be a permanent magnet or an electromagnet. The intensity of the magnetic field at the surface of the magnet is preferably between 0.01 mT and 2 T, and most preferably between 0.1 mT and 500 mT. The distance between the magnet and the electrodes is preferably less than 5 cm, more preferably less than 3 cm, and most preferably less than 1 cm. According to an exemplary embodiment, the magnetic field is provided by a neodymium magnet located 0.5 cm apart from the skin surface when the device is at its operational position. Also, when the device is at its operational position, the direction of the magnetic field is substantially perpendicular to the skin surface within the distance and sub-

stantially perpendicular to desired direction of fluid displacement from the dermis to the skin surface. Consequently, the dermal IF is driven towards the surface of the skin.

[0031] According to another embodiment the device comprises plurality of magnets. According to an exemplary embodiment, the magnetic field is provided by an array of magnets or electromagnets. An exemplary array is a Halbach array 211 shown in Figure 4. Two of the magnets are shown with the reference numbers 205a and 205b. The overlapping magnetic fields of the magnets in the array combine to produce a resultant magnetic field acting in one direction marked with the letter B. The electrodes (not shown) are positioned inside the array so that the electric field E is as shown in the coordinate system 299. Accordingly, the direction of IF extraction can be adapted to be towards the skin surface.

[0032] The use of arrays of magnets allows to modulate (i.e. to augment, decrease or cancel) the magnetic field directionally or locally. For instance, a circular Halbach array consisting on a cylinder composed of neodymium magnets can be used to produce an intense magnetic field confined within the cylinder. Moreover, the array of magnets can be positioned wrapping the electrode and the extraction site, for instance in a ring or wristband, where the electrodes are arranged inside the cylinder. This allows having a strong magnetic field at the extraction site while keeping a weak magnetic field elsewhere.

[0033] According to one embodiment the device comprises means 107 adapted to store (e.g. to collect) and/or means 108 adapted to analyze the IF comprising one or more analytes extracted from the skin. According to an exemplary embodiment, the storing means comprises one or more capillaries located within the distance 103. The one or more capillaries are preferably coaxial with the electrodes, and one end of the capillaries is located so that the IF extracted from the skin moves into the one or more capillaries. According to a particular embodiment, the means adapted to store the fluid, such as the one or more capillaries or a reservoir, act also as means adapted to transfer the fluid to means 108 adapted to analyze the one or more analytes. Alternatively, the means 108 is adapted to record one or more signals derived from the one or more analytes and to send the one or more signals to means adapted to analyze them. According to an exemplary embodiment, the means 107 and/or 108 comprises medium such as gel or liquid comprising glucose oxidase adapted to form hydrogen peroxide, the concentration of which is determined electrochemically and/or optically. The means 107 and 108 are preferably located within the distance and/or under one or more electrodes. According to another embodiment, the device comprises means for storing and analyzing interstitial fluid. According to still another embodiment, the analyzing means is separated from the device.

[0034] According to an exemplary embodiment, the device comprises a frame 109 adapted to position the

electrodes, the power source, and the magnet, and any further means of the device such as the energy storing means (such as a battery), the IF storing means and the IF analyzing means. The contact surface of the first electrode, the contact surface of the second electrode, and preferably also the means adapted to store and/or analyze the one or more analytes are on the surface of the frame adapted to be in direct or indirect contact with the skin surface.

[0035] According to another embodiment the frame of the device is of pocket size.

[0036] According to an exemplary embodiment, the MHD device of the present invention is combined with other approaches, such as sonoporation, laserporation, electroporation and hydraulic pressure, to increase the permeability of the skin. The different permeability-enhancing approaches can be used to disrupt the mechanical properties of the upper layer of the skin (e.g. the stratum corneum) temporarily or permanently. This can facilitate the IF extraction. For instance, sonoporation can be applied before or during IF extraction with the device of the present invention (e.g. constantly or recurrently). Accordingly, the device of the present invention may comprise one or more means 110 selected from ultrasound generating means, laser light generating means, electroporation generating means, hydraulic pressure generating means.

[0037] Another exemplary non-limiting device 300 according to the present invention is shown in figure 5. Frame of the device is in form of a wristband 309. The device shown therein comprises a first electrode 302a and a second electrode 302b adapted to be positioned adjacent to skin surface. The first electrode and the second electrode are separated by a distance 303. The device comprises also a power source 304 adapted to induce an electric current through the first electrode, interstitial fluid and the second electrode when the device is at its operational position. The device comprises also a magnet 305 adapted to induce a magnetic field to the IF. Direction of the magnetic field and direction of the electric current is such that Lorentz force is adapted to drive the IF from dermis substantially towards the skin surface. The magnetic field can also be produced by a plurality of magnets, such as an array of magnets as shown in figure 4.

[0038] In order to produce Lorentz force in the current-carrying IF in the skin within the distance and below the negative electrode towards the skin surface, the magnet 305 should produce a magnetic field that is substantially in z-direction of the coordinate system 399. Accordingly, the MHD effect generated by the magnetic field produced by the magnet 305 or plurality of magnets and the electric current established by the power source 304 drives the IF comprising the one or more analytes from dermis substantially towards the skin surface. Accordingly, the direction of the flow of the IF is substantially in y-direction of the coordinate system 399. The location of the power source and the magnet in figure 5 are only illustrative.

[0039] The advantages of this embodiment are that the wristband can offer means to position the first electrode and the second electrode in contact with the skin, for instance, by using adhesive materials, pneumatic force and/or mechanical pressure. According to the embodiment shown in the figure, a permanent magnet is arranged in the wristband close to target site of interstitial fluid extraction, so that the magnetic field is substantially perpendicular to the skin surface within the distance and substantially perpendicular to the direction of fluid from the dermis to the skin surface. To accomplish this, the wristband may have movable parts such as a retractable magnet holder. Furthermore, the wristband can offer means to collect, transport, store and/or analyze the interstitial fluid sample (not shown in figure 5). Also, the wristband can be provided with an electronic or electro-mechanical user interface comprising, for instance, a display 310, such as a touch screen display, push buttons, and mechanical, visual and/or audio indicators (e.g. light emitting diodes, loudspeaker and vibrating alarms). Furthermore, the wristband may have means to store data such as an electronic circuit and means to send data, preferably wirelessly, to another electronic device such as a cellphone, a tablet, a computer or an insulin pump. Also, the device may have means to connect to Internet. An electronic circuit in the wristband can also serve to monitor the electric current and/or voltage applied to the skin to assess the electrode-skin electric contact. The energy required for the operation of the electronic circuit can be provided by, for instance, a rechargeable battery adapted in the wristband. In one particular embodiment of the invention, the wristband encompasses one or more capillaries made of organic or inorganic materials (e.g. polyfluorocarbon, polyethylene, polyvinyl chloride, and borosilicate glass) to collect the interstitial fluid sample. The tip of the capillaries is arranged close to, or in contact with, the extraction site. For instance, they can be arranged in the electrode gap and/or integrated in the first electrode and/or in the second electrode. Other suitable elements to collect the extracted IF samples or compounds in the IF samples include electrically and/or magnetically charged materials, hydrophobic and/or hydrophilic materials, and absorbent materials. In another particular embodiment of the invention, the electrodes are coated with a substance or mixture that reacts (e.g. chemically or physically) or that binds to one or more constituents of the IF sample. Exemplary electrode coatings include gels, such as hydrogels and polymeric gels, where the gels can be further loaded with reagents such as enzymes, for instance, glucose oxidase. The electrode coating can serve to collect the sample of interstitial fluid or particular components of the sample and to allow further sample analysis, for instance, to measure the content of glucose, lactic acid or other compounds in the IF sample by applying current technologies or technologies developed in the future. Also, in humans, this invention can also be implemented in different parts of the body, including (but not limiting to) the head, earlobe, eyes,

neck, nose, mouth, chest, abdomen, arms, forearms, legs, fingers (e.g. as in a ring), feet, and toes. Furthermore, the invention can be used in any living or dead biological organism, including but not limiting humans and animals (e.g. in the ears, legs, or in the tail of dogs or rats).

[0040] The device of the present invention is suitable for sampling one or more analytes that can be withdrawn from skin by using the MHD phenomenon. Exemplary non-limiting analytes comprise amino acids, sugars, fatty acids, co-enzymes, hormones, neurotransmitters, lactic acid, and drugs. A particular analyte is glucose. Another particular analyte is lactic acid.

15 EXAMPLES

Example 1

[0041] The efficacy of the device according to the present invention to extract dermal IF was compared to electrophoresis. Postmortem abdominal porcine skin samples (3 cm × 3 cm) dissected from adjacent tissue were treated with 1) the device according to the present invention and 2) the device according to the present invention but omitting the magnetic field. Accordingly, in experiment 1) and experiment 2) the sampling was performed by MHD and electrophoresis, respectively.

[0042] The two experiments were run simultaneously and applying the same parametrization and electrode configuration. In each case, the first electrode and the second electrode were made of graphite. The contact surface of all the electrodes was flat and round (diameter = 7 mm). A single current source was used to establish a 0.4 mA direct electric current serially in the two treatments. The estimated current density at the electrode-skin interface was 1 mA/cm². The separation between the first electrode and the second electrode in both experiments was 1 cm. For the device according to the present invention exclusively, a permanent neodymium magnet with a 0.8 T magnetic field at its surface was arranged at distance of 1 cm from the extraction site. The magnet was arranged in such a way that the magnetic field was established in a direction substantially perpendicular to the skin surface within the distance and substantially perpendicular to desired direction of fluid displacement from the dermis to the skin surface. Consequently, a Lorentz force was generated towards the skin surface in the current-carrying fluid in the skin. An exposure-to-treatment time of 1 hour revealed a clear difference in the volume of dermal IF extracted by the two methods. As seen in figure 6, the fluid extracted with the device according to the present invention forms a drop (marked with an arrow in figure 6, left) that can be seen by the naked eye and whose volume is substantially larger than the volume of fluid extracted by electrophoresis, which is not sufficiently large to be distinguished by the naked eye. Considering that the extracted fluid is subject to evaporation, the accumulation of fluid observed in the

sample treated with the device according to the present invention is a strong indicator that this method is substantially faster than electrophoresis.

Example 2

[0043] The concentration of glucose in intestinal fluid and blood was measured by using a device according to the present invention and by using a conventional fingertip pricking instrument in a group of healthy adult humans (n = 11).

[0044] For each measurement, paired samples of interstitial fluid and blood were concurrently obtained using either the device according to the present invention or conventional fingertip pricking instrument (CareSensT-MN; model GM505PAD, i-SENSm inc, Seoul, Korea), respectively. The concentration of glucose in the samples of interstitial fluid was measured using a commercial assay kit (AB65333, Abcam Cambridge, UK). The results showed a direct relationship between the concentration of glucose in the samples of interstitial fluid and blood. The results confirm that the concentration of glucose in the samples extracted with a device according to the present invention can be used to estimate blood glucose. Furthermore, no pain, skin reactions, or evident sample disruption was induced by the extraction procedure.

[0045] The concentration of glucose in interstitial fluid correlates with the concentration of glucose in blood. In one preferred embodiment, once the concentration of glucose in the sample of interstitial fluid is measured, a mathematical algorithm or mathematical model can be used to estimate the corresponding level of blood glucose. This mathematical algorithm can consist of arithmetic operations, statistical functions and even artificial intelligence algorithms.

[0046] The specific examples provided in the description given above should not be construed as limiting the scope and/or the applicability of the appended claims.

Claims

1. A device (100, 300) for sampling interstitial fluid comprising one or more analytes from dermis (101a) to skin surface (101b), the device comprising
 - a first electrode (102a, 302a) and a second electrode (102a, 302b) adapted to be positioned adjacent to the skin surface, the first electrode separated from the second electrode by a distance (103, 303),
 - a power source (104, 304) adapted to induce an electric current through the first electrode, the interstitial fluid and the second electrode, **characterized in that** the device further comprising
 - one or more magnets (105, 205a,b, 305) adapted to induce magnetic field to the interstitial fluid,

and in that direction of the magnetic field produced by the one or more magnets, and direction of the electric current produced by the power source are adapted to be such that Lorentz force produced by the magnetic field and the electric current is adapted to drive the interstitial fluid from the dermis substantially towards the skin surface.

2. The device according to claim 1, wherein the magnetic field is adapted to be substantially in z-direction, the electric field is adapted to be substantially in x-direction, and the skin surface is adapted to be substantially perpendicular to y-direction of coordinate system (199, 399), within the distance, the first electrode and the second electrode, when the device is at its operational position.
3. The device according to claim 1 or 2 comprising a frame (109, 309) adapted to position the first electrode, the second electrode, the power source and the one or more magnets.
4. The device according to any of claims 1-3, wherein the first electrode and the second electrode are adapted to be substantially perpendicular to the skin surface when the device is at its operational position.
5. The device according to any of claims 1-4, wherein the distance is 1 mm - 5 cm, preferably 5 mm - 3 cm.
6. The device according to any of claims 1-5, wherein the device comprises means (107) adapted to collect and/or store the one or more analytes sampled from the dermis.
7. The device according to any of claims 1-6 wherein the device comprises means (108) adapted to analyze the one or more analytes.
8. The device according to any of claims 1-7 wherein contact surface (106a) of the first electrode and/or contact surface (106b) of the second electrode is elliptical.
9. The device according to any of claims 1-8, wherein contact surface (106a) of the first electrode and/or contact surface (106b) of the second electrode comprises extrusions and/or protrusions.
10. The device according to claim 3, wherein the frame is in form of wristband, ring.
11. The device according to claim 10, wherein the frame is in form of wristband, and the wristband comprises one or more of: user interface, means adapted to store data, means adapted to send and receive data, means adapted to provide energy to the power

source.

12. The device according to any of claims 1-11, comprising means (110) selected from one or more of: ultrasound generating means, laser light generating means, electroporation generating means, and hydraulic pressure generating means.
13. The device according to any of claims 3, 10 or 11 wherein the frame comprises adhesive material adapted to be positioned in contact with the skin.
14. The device according to any of claims 1-13, wherein the first electrode and/or the second electrode is/are coated with one or more enzymes and/or one or more catalysts.
15. The device according to any of claims 1-14, wherein the device comprises a membrane and/or electrically conducting material adapted to be positioned between the first electrode and the skin, and between the second electrode and the skin.

Patentansprüche

1. Vorrichtung (100, 300) zum Entnehmen von interstitiellem Fluid, umfassend einen oder mehrere Analyte von der Dermis (101a) zu der Hautoberfläche (101b), wobei die Vorrichtung umfasst
 - eine erste Elektrode (102a, 302a) und eine zweite Elektrode (102a, 302b), die eingerichtet sind, benachbart zur Hautoberfläche positioniert zu werden, wobei die erste Elektrode von der zweiten Elektrode durch einen Abstand (103, 303) getrennt ist,
 - eine Energiequelle (104, 304), die eingerichtet ist, um einen elektrischen Strom durch die erste Elektrode, das interstitielle Fluid und die zweite Elektrode zu induzieren, **dadurch gekennzeichnet, dass** die Vorrichtung ferner umfasst
 - einen oder mehrere Magnete (105, 205a, b, 305), die eingerichtet sind, um ein Magnetfeld in dem interstitiellen Fluid zu induzieren, und dadurch, dass die Richtung des von dem einen oder den mehreren Magneten erzeugten Magnetfeld und die Richtung des von der Energiequelle erzeugten elektrischen Stroms derart eingerichtet sind, dass die Lorentzkraft, die durch das Magnetfeld und den elektrischen Strom erzeugt wurde, eingerichtet ist, dass sie das interstitielle Fluid aus der Dermis im Wesentlichen in Richtung der Hautoberfläche treibt.
2. Vorrichtung nach Anspruch 1, wobei das Magnetfeld so eingerichtet ist, dass es im Wesentlichen in z-Richtung ist, das elektrische Feld so eingerichtet ist,

dass es im Wesentlichen in x-Richtung ist, und die Hautoberfläche so eingerichtet ist, dass sie im Wesentlichen senkrecht zur y-Richtung des Koordinatensystems (199, 399) innerhalb des Abstands der ersten Elektrode und der zweiten Elektrode ist, wenn die Vorrichtung in ihrer Betriebsposition ist.

3. Vorrichtung nach Anspruch 1 oder 2, umfassend einen Rahmen (109, 309), der eingerichtet ist, die erste Elektrode, die zweite Elektrode, die Energiequelle und den einen oder die mehreren Magnete zu positionieren.
4. Vorrichtung nach einem der Ansprüche 1 bis 3, wobei die erste Elektrode und die zweite Elektrode eingerichtet sind, dass sie im Wesentlichen senkrecht zur Hautoberfläche sind, wenn die Vorrichtung in ihrer Betriebsposition ist.
5. Vorrichtung nach einem der Ansprüche 1 bis 4, wobei der Abstand 1 mm - 5 cm, vorzugsweise 5 mm - 3 cm beträgt.
6. Vorrichtung nach einem der Ansprüche 1 bis 5, wobei die Vorrichtung Mittel (107) umfasst, die zum Sammeln und/oder Speichern des einen oder der mehreren Analyte, die aus der Dermis als Probe entnommen wurden, eingerichtet sind.
7. Vorrichtung nach einem der Ansprüche 1 bis 6, wobei die Vorrichtung Mittel (108) umfasst, die zum Analysieren des einen oder der mehreren Analyte eingerichtet sind.
8. Vorrichtung nach einem der Ansprüche 1 bis 7, wobei die Kontaktfläche (106a) der ersten Elektrode und/oder die Kontaktfläche (106b) der zweiten Elektrode elliptisch sind.
9. Vorrichtung nach einem der Ansprüche 1 bis 8, wobei die Kontaktfläche (106a) der ersten Elektrode und/oder die Kontaktfläche (106b) der zweiten Elektrode Extrusionen und/oder Vorsprünge umfassen.
10. Vorrichtung nach Anspruch 3, wobei der Rahmen in Form eines Armbandes, eines Rings ausgebildet ist.
11. Vorrichtung nach Anspruch 10, wobei der Rahmen in der Form eines Armbandes ausgebildet ist und das Armband eines oder mehrere umfasst von: Benutzerschnittstelle, Mittel, die zum Speichern von Daten eingerichtet sind, Mittel, die zum Senden und Empfangen von Daten eingerichtet sind, Mittel, die zum Bereitstellen von Energie für die Energiequelle eingerichtet sind.
12. Vorrichtung nach einem der Ansprüche 1 bis 11, umfassend Mittel (110), die ausgewählt sind aus einem

oder mehreren von: Ultraschall erzeugenden Mitteln, Laserlicht erzeugenden Mitteln, Elektroporation erzeugenden Mitteln und hydraulischen Druck erzeugenden Mitteln.

13. Vorrichtung nach einem der Ansprüche 3, 10 oder 11, wobei der Rahmen ein Klebematerial umfasst, das eingerichtet ist, in Kontakt mit der Haut positioniert zu werden.
14. Vorrichtung nach einem der Ansprüche 1 bis 13, wobei die erste Elektrode und/oder die zweite Elektrode mit einem oder mehreren Enzymen und/oder einem oder mehreren Katalysatoren beschichtet ist/sind.
15. Vorrichtung nach einem der Ansprüche 1 bis 14, wobei die Vorrichtung eine Membran und/oder ein elektrisch leitfähiges Material umfasst, das eingerichtet ist, zwischen der ersten Elektrode und der Haut und zwischen der zweiten Elektrode und der Haut positioniert zu werden.

Revendications

1. Dispositif (100, 300) pour échantillonner un liquide interstitiel, comprenant un ou plusieurs analytes, du derme (101a) vers la surface de la peau (101b), le dispositif comprenant
- une première électrode (102a, 302a) et une deuxième électrode (102a, 302b) adaptées pour être positionnées de manière adjacente à la surface de la peau, la première électrode étant séparée de la deuxième électrode de l'ordre d'une distance (103, 303),
 - une source d'alimentation (104, 304) adaptée pour induire un courant électrique à travers la première électrode, le liquide interstitiel et la deuxième électrode, **caractérisé en ce que** le dispositif comprend en outre
 - un ou plusieurs aimants (105, 205a, b, 305) adaptés pour induire un champ magnétique pour le liquide interstitiel, et **en ce que** la direction du champ magnétique produite par ce ou ces aimants, et une direction du courant électrique produit par la source d'alimentation sont adaptées pour être telles, qu'une force de Lorentz produite par le champ magnétique et le courant électrique est adaptée pour entraîner le liquide interstitiel du derme sensiblement vers la surface de la peau.
2. Dispositif selon la revendication 1, dans lequel le champ magnétique est adapté pour être sensiblement en direction z, le champ électrique est adapté pour être sensiblement en direction x, et la surface de la peau est adaptée pour être sensiblement per-

pendiculaire à la direction y d'un système de coordonnées (199, 399), dans les limites de la distance, de la première et la deuxième électrode, lorsque le dispositif est dans sa position de fonctionnement.

3. Dispositif selon la revendication 1 ou 2, comprenant un cadre (109, 309) adapté pour positionner la première électrode, la deuxième électrode, la source d'alimentation et ce ou ces aimants.
4. Dispositif selon l'une quelconque des revendications 1-3, dans lequel la première électrode et la deuxième électrode sont adaptées pour être sensiblement perpendiculaires à la surface de la peau lorsque le dispositif est dans sa position de fonctionnement.
5. Dispositif selon l'une quelconque des revendications 1-4, dans lequel la distance est de 1 mm - 5 cm, de préférence de 5 mm - 3 cm.
6. Dispositif selon l'une quelconque des revendications 1-5, dans lequel le dispositif comprend un moyen (107) adapté pour collecter et/ou stocker ce ou ces analytes échantillonnés à partir du derme.
7. Dispositif selon l'une quelconque des revendications 1-6, dans lequel le dispositif comprend un moyen (108) adapté pour analyser ce ou ces analytes.
8. Dispositif selon l'une quelconque des revendications 1-7, dans lequel une surface de contact (106a) de la première électrode et/ou une surface de contact (106b) de la deuxième électrode est elliptique.
9. Dispositif selon l'une quelconque des revendications 1-8, dans lequel une surface de contact (106a) de la première électrode et/ou une surface de contact (106b) de la deuxième électrode comprennent des extrusions et/ou saillies.
10. Dispositif selon la revendication 3, dans lequel le cadre est en forme de bracelet, de bague.
11. Dispositif selon la revendication 10, dans lequel le cadre est en forme de bracelet, et le bracelet comprend un(e) ou plusieurs parmi : une interface utilisateur, un moyen adapté pour stocker des données, un moyen adapté pour envoyer et recevoir des données, un moyen adapté pour fournir de l'énergie à la source d'alimentation.
12. Dispositif selon l'une quelconque des revendications 1-11, comprenant un moyen (110) sélectionné à partir d'un ou plusieurs parmi : un moyen de génération d'ultrasons, un moyen de génération de lumière laser, un moyen de génération d'électroporation, et un moyen de génération de pression hydraulique.

13. Dispositif selon l'une quelconque des revendications 3, 10 ou 11, dans lequel le cadre comprend une matière adhésive adaptée pour être positionnée en contact avec la peau.

5

14. Dispositif selon l'une quelconque des revendications 1-13, dans lequel la première électrode et/ou la deuxième électrode est/sont revêtue(s) avec un ou plusieurs enzymes et/ou un ou plusieurs catalyseurs.

10

15. Dispositif selon l'une quelconque des revendications 1-14, dans lequel le dispositif comprend une membrane et/ou un matériau électroconducteur adapté pour être positionné entre la première électrode et la peau, et entre la deuxième électrode et la peau.

15

20

25

30

35

40

45

50

55

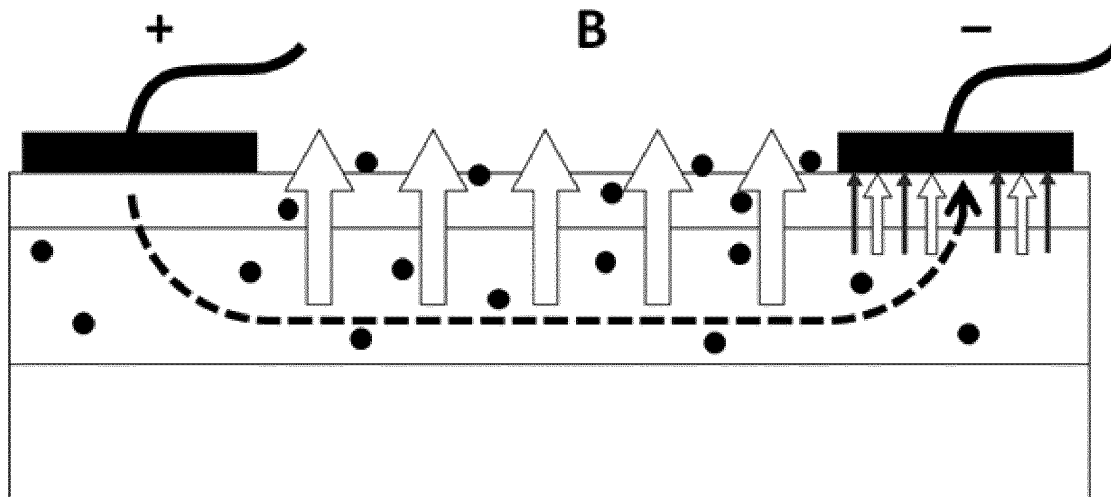


Figure 1

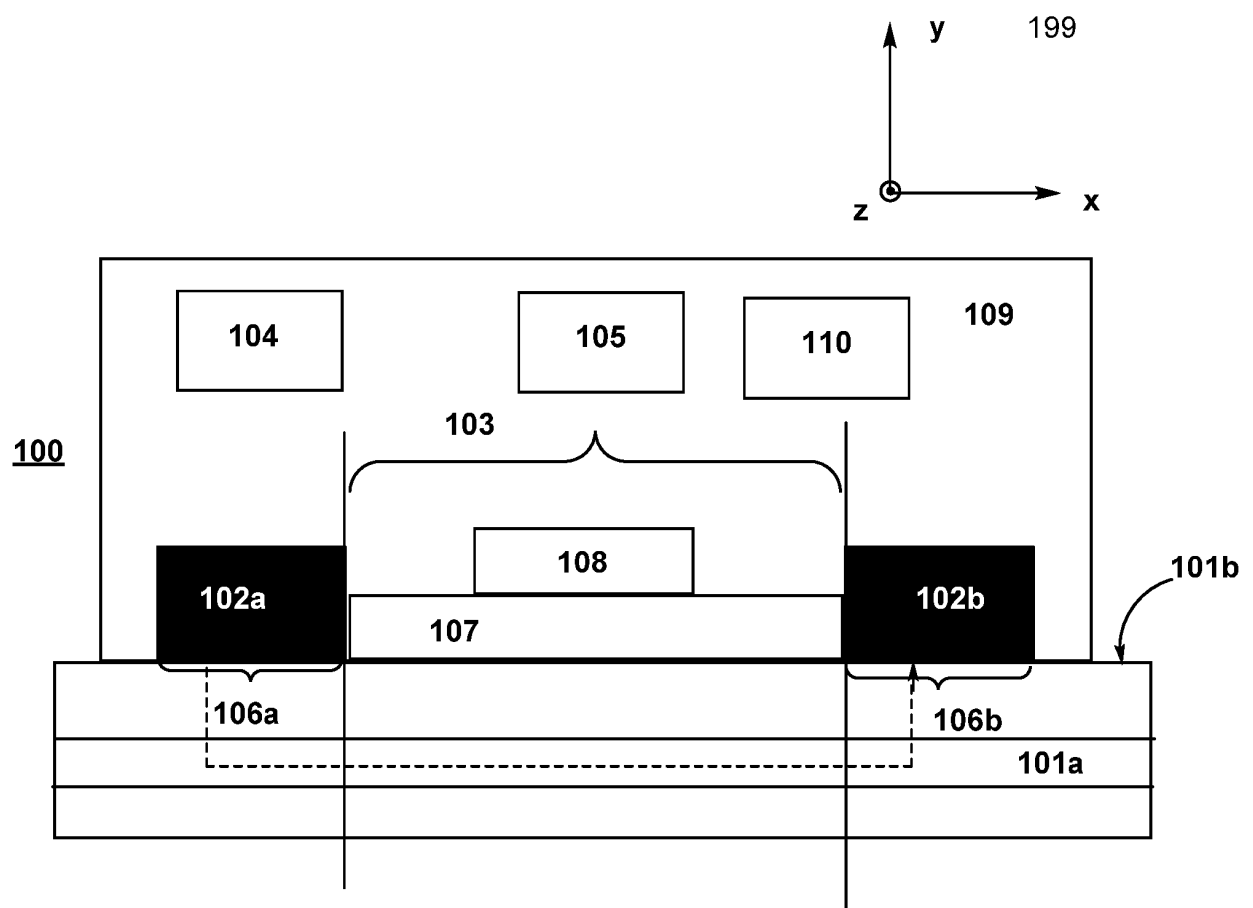


Figure 2

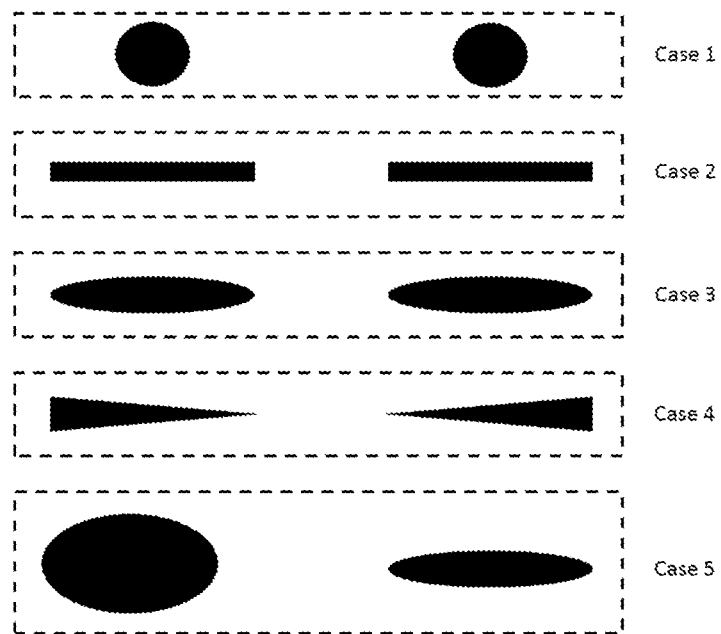


Figure 3

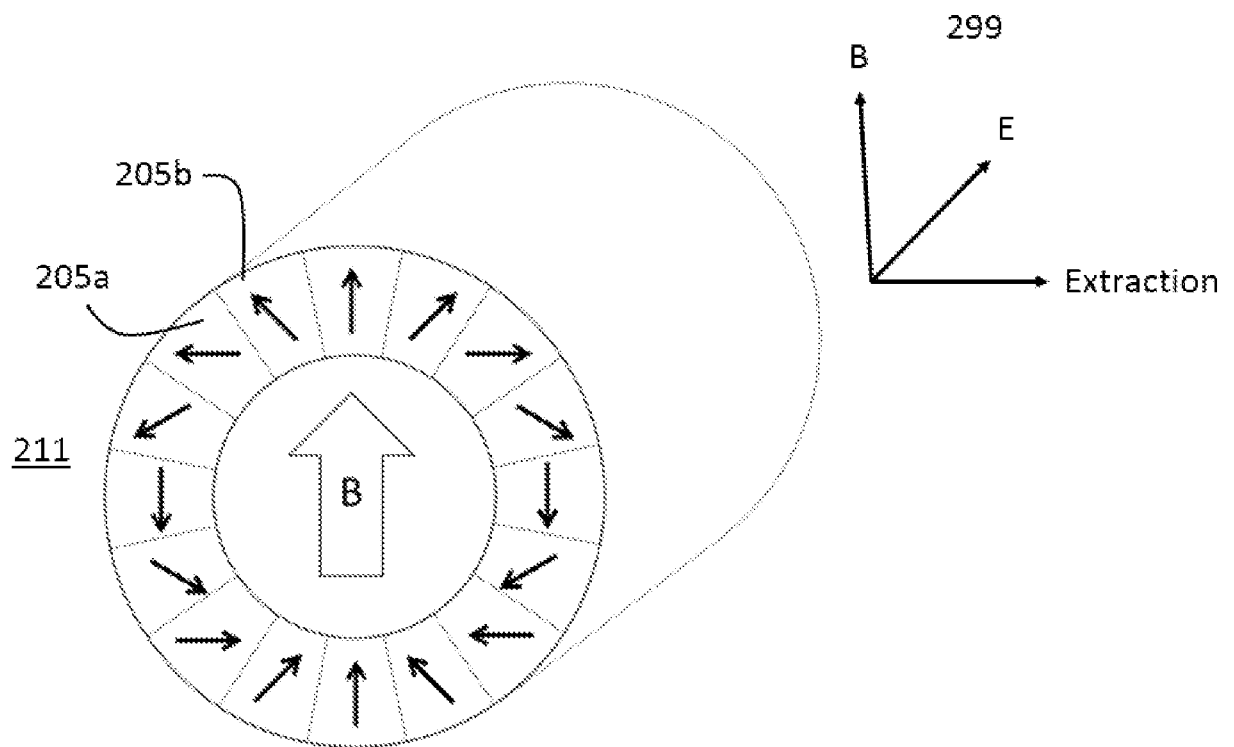


Figure 4

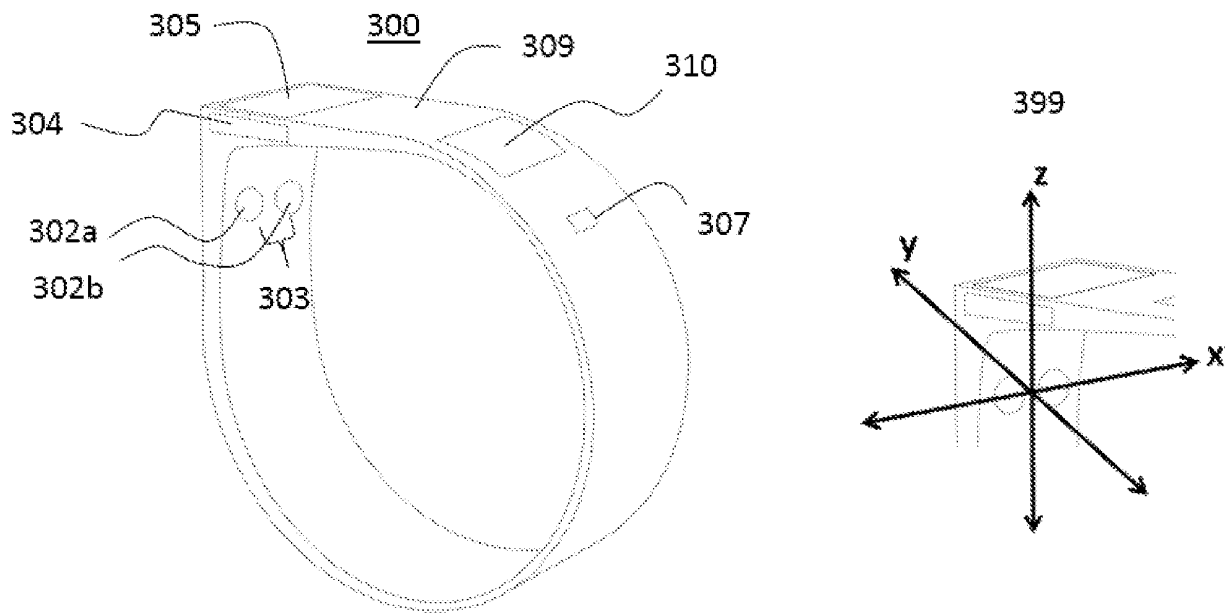


Figure 5

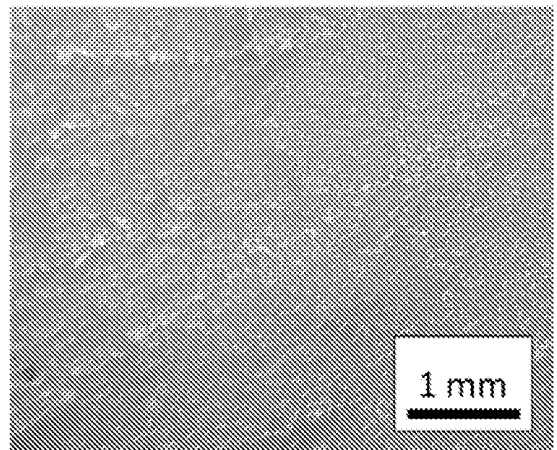
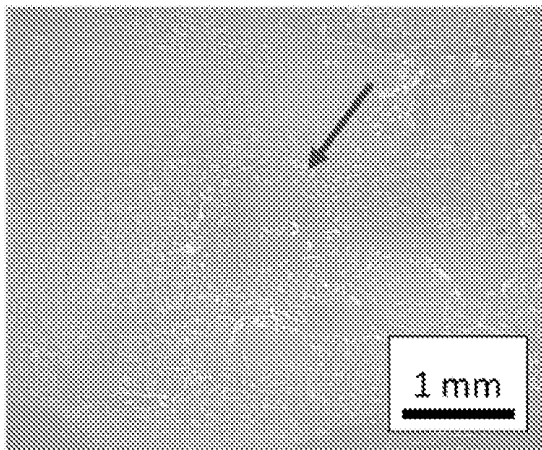


Figure 6

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 20020002328 A1 [0003]
- WO 2010001122 A2 [0004]

专利名称(译)	用于取样一种或多种分析物的装置		
公开(公告)号	EP3422936A1	公开(公告)日	2019-01-09
申请号	EP2017818598	申请日	2017-11-08
[标]发明人	GARCIA PEREZ ALEJANDRO NIEMINEN HEIKKI HAEGGSTROM EDWARD		
发明人	GARCIA PEREZ, ALEJANDRO NIEMINEN, HEIKKI HAEGGSTROM, EDWARD		
IPC分类号	A61B5/05 A61B5/15 A61B5/145 A61B5/1477 A61B5/151 A61B5/157 A61B5/00		
CPC分类号	A61B5/14514 A61B5/14532 A61B5/14546 A61B5/1477 A61B5/150022 A61B5/150091 A61B5/150343 A61B5/15134 A61B5/157 A61B5/681 A61B5/15 A61B5/0002 A61B5/1486 A61B5/6832 A61B5/7475 A61B2560/0214 A61B2560/0475 G01N33/66		
优先权	2016005876 2016-11-21 FI		
其他公开文献	EP3422936B1		
外部链接	Espacenet		

摘要(译)

本申请涉及一种用于非侵入性地采样组织间液的装置 (100) , 其包括通过使用磁流体动力学效应从真皮 (101a) 到皮肤表面 (101b) 的一种或多种分析物。该装置包括第一电极 (102a) 和第二电极 (102b) , 其适于邻近皮肤表面定位, 第一电极与第二电极分开一距离 (103) , 电源 (104) 适于诱导通过第一电极, 组织间液和第二电极的电流, 以及适于向组织间液产生磁场的磁体 (105) 。磁场的方向和由磁体和电源产生的电流的方向分别使得洛伦兹力驱动流体从真皮朝向皮肤表面。