



(11) **EP 1 356 250 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
22.07.2009 Bulletin 2009/30

(51) Int Cl.:
G01B 9/02 ^(2006.01) **A61B 6/02** ^(2006.01)
G01M 11/00 ^(2006.01)

(21) Application number: **01980204.0**

(86) International application number:
PCT/DK2001/000721

(22) Date of filing: **31.10.2001**

(87) International publication number:
WO 2002/037075 (10.05.2002 Gazette 2002/19)

(54) **OPTICAL AMPLIFICATION IN COHERENT OPTICAL FREQUENCY MODULATED CONTINUOUS WAVE REFLECTOMETRY**

OPTISCHE VERSTÄRKUNG BEI DER KOHÄRENTEN OPTISCHEN FREQUENZMODULIERTEN DAUER-REFLEKTOMETRIE

AMPLIFICATION OPTIQUE EN REFLECTOMETRIE PAR COHERENCE OPTIQUE A ONDES ENTRETENUES MODULEES EN FREQUENCE

(84) Designated Contracting States:
AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU MC NL PT SE TR

- **BJARKLEV, Anders**
DK-4000 Roskilde (DK)
- **TYCHO, Andreas**
DK-2100 København Oe (DK)

(30) Priority: **31.10.2000 DK 200001637**

(43) Date of publication of application:
29.10.2003 Bulletin 2003/44

(74) Representative: **HOEIBERG A/S**
European Patent & Trademark Attorneys
Store Kongensgade 59 A
1264 Copenhagen K (DK)

(73) Proprietor: **Danmarks Tekniske Universitet**
2800 Lyngby (DK)

(56) References cited:
EP-A2- 0 578 400 **WO-A1-00/45153**
US-A- 5 268 741 **US-A- 5 365 335**
US-A- 5 459 570 **US-A- 6 015 969**

(72) Inventors:
• **ANDERSEN, Peter, E.**
DK-4340 Tølløse (DK)

EP 1 356 250 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The present invention relates to an apparatus for optical coherence reflectometry, in particular for optical coherence tomography.

Background

[0002] Optical low-coherence reflectometry (OLCR) is used for example for analyzing inhomogeneities in optical waveguides and optical devices. In this method light is transmitted down the optical fibre and light resulting from the interaction with an inhomogeneity in the optical fibre is back-scattered. The light is split into two arms, a sample arm and a reference arm. When the optical pathlength in the sample arm matches time delay in the reference arm coherent interference occurs and the distance the light has travelled in the sample arm may be determined.

[0003] Most known devices, use broadband light sources eg. superluminescent diodes, with a short coherence time, and they need a scanning mirror to record the depth resolved backscattered signal. In other systems a tunable laser is used as the light source, whereby, instead of moving the mirror, the wavelength of the laser can be varied to record the backscattered signal. This principle is discussed in Haberland, U.H.P. et al., "Chirp Optical Coherence Tomography of Layered Scattering Media" as well as in US 5,956,355 (Swanson et al.). The method is often referred to as coherent optical frequency modulated continuous wave (FMCW) reflectometry.

[0004] OLCR can be extended through the use of polarized light. The light field towards the reference and sample is then polarized. After combining the light field reflected from the reference and the sample, the combined light field is split up again into two new light fields with perpendicular polarization states. Through this method the birefringent properties of the sample can be investigated in addition to the information obtainable with ordinary OLCR adding to the systems ability to discriminate between certain types of materials within the sample. This method also applies to OCT often referred to as polarization sensitive OCT (PS-OCT), as well as coherent optical FMCW reflectometry.

[0005] Optical low-coherence reflectometry is also used in the imaging of 2-dimensional and 3 dimensional structures, eg. biological tissues, in this respect often referred to as optical coherence tomography (OCT). OCT can be used to perform high-resolution cross-sectional *in vivo* and *in situ* imaging of microstructures, such as in transparent as well as non-transparent biological tissue or other absorbing and/or random media in general. There are a number of applications for OCT, such as non-invasive medical diagnostic tests also called optical biopsies. For example cancer tissue and healthy tissue can be distinguished by means of different optical properties. Coherent optical FMCW reflectometry also applies to the above-mentioned cases.

[0006] In order to optimize optical low-coherence reflectometry measurements and imaging various suggestions to increase signal-to-noise ratio (SNR) have been discussed in the art.

[0007] US 5,291,267 (Sorin et al.) discloses optical reflectometry for analyzing inhomogeneities in optical fibres. In US 5,291,267 amplification of the light reflected from the optical fibre is conducted. In particular US 5,291,267 suggests to use the light source as an amplifier in order to save costs.

[0008] WO 99/46557 (Optical Biopsies Technologies) discusses SNR in a system wherein a reference beam is routed into a long arm of an interferometer by a polarizing beamsplitter. In general the reference suggest to include an attenuator in the reference arm to increase SNR. In a balanced setup the reference on the other hand suggests to increase the power of the reference arm in order to increase SNR.

[0009] In "Unbalanced versus balanced operation in an optical coherence tomography system" Podoleanu, A.G., Vol. 39, No. 1, Applied optics, discussed various methods of increasing SNR in unbalanced and balanced systems, respectively. Reduction of power in the reference arm was suggested as well as reduction of fibre end reflections to increase the SNR.

[0010] Optical low-coherence tomography reflectometry and coherent optical FMCW reflectometry obtain the same information about the sample being investigated, and, in this respect, they may be considered similar.

[0011] The present invention relates to an optimisation coherent optical FMCW reflectometry whereby an increase of the SNR is obtained leading to a better result of the measurements, in particular in relation to penetration depth of the system, so that the penetration depth increases, when the SNR increases.

Summary of the invention

[0012] Thus, the present invention relates to an apparatus for optical coherence reflectometry comprising

- a wavelength scanning laser source for providing a light signal
- splitting means for dividing said light signal into a first light field and a second light field,

EP 1 356 250 B1

- 5 - means for directing the first light field to a sample, and means for directing a first reflected light field from the sample, wherein an optical amplifier is inserted in the first reflected light field, said optical amplifier being different from the light source, and means for directing the amplified first reflected light field to a combining means, so that the amplified first reflected light field is directed to the combining means through another route than a route through the splitting means for dividing the light signal,
- means for directing the second light field to the combining means,
- 10 - combining means for receiving said amplified first reflected light field and said second light field to generate a combined light signal, and
- at least one detecting means for detecting the combined light signal and outputting detection signals.

15 **[0013]** In the present context the term "optical coherence reflectometry" is used in its normal meaning, and in particular the term means optical coherence FMCW reflectometry.

[0014] Furthermore, the term "wavelength scanning laser source" means a frequency-tuned laser having a tunable longitudinal cavity mode and a center tunable wavelength, for example as described in US 5,956,355.

20 **[0015]** The present apparatus offers a better signal-to-noise ratio (SNR) whereby an increase of the maximal penetration depth is obtained. Thereby, the apparatus according to the present invention is especially useful for obtaining optical biopsies of transparent as well as non-transparent tissues.

[0016] In particular a combination of the arrangement of amplification discussed above and reduction of fibre end reflections increases the signal-to-noise ratio leading to an improved system.

25 **[0017]** The term "sample path" or "sample arm" is used to define the route travelled by the light from the light source to the sample and reflected from the sample to the combining means. In the present context the light field and routes relating to the sample arm is denoted the first light field and the first light route, respectively.

30 **[0018]** Correspondingly the term "reference path" or "reference arm" is used to define the route travelled by the light from the light source to the combining means. In the present context the light field and routes relating to the reference arm is denoted the second light field and the second light route, respectively. It is often convenient to be able to alter the optical length of the second light route. This may be accomplished by insertion of reflection means where the position of these may be scanned or by using a so-called fiber-stretcher well known in the art.

[0019] In another aspect the present invention relates to a method for providing a result of a sample comprising

- 35 - establishing a wavelength scanning laser source for providing a light signal,
- splitting said light signal into a first light field and a second light field,
- directing the first light field to the sample, and the second light field to a reference path,
- receiving a first reflected light field from the sample, optically amplifying the first reflected light field, and directing the first reflected light field in a combining " means,
- 40 - receiving the second light field,
- combining said amplified first reflected light field and said second light field to generate a combined light signal,
- 45 - detecting the combined light signal obtaining detection signals, and
- processing the detection signals obtaining the result of the sample.

50 **[0020]** In the present context the term "result of the sample" may refer in coherent optical FMCW reflectometry to the image of the sample obtained. When using the present invention in coherent optical FMCW reflectometry in optical fibres used for example in the communication technology the result relates to the signal obtained, such as a signal relating to the distance to an inhomogeneity in the device under test.

55 Drawings

[0021]

Fig. 1 shows an unbalanced conventional coherent optical FMCW reflectometry system according to prior art, wherein an attenuator has been inserted in the reference arm.

5 Fig. 2 shows a balanced apparatus according to the invention, wherein the amplified first reflected light field is directed to the combining means through another route than a route through the splitting means. A y-coupler is inserted in the sample arm to receive the reflected light field from the sample.

Fig 3 shows the balanced detection means of Fig. 2 in detail.

10 Fig. 4 shows a balanced apparatus as in Fig. 2 wherein an optical circulator has been inserted instead of the beam splitting means in the sample.

15 Fig. 5 shows a balanced system chosen as reference system. The system is similar to the system shown in Fig. (2) except for omission of the optical amplifier and the y-coupler in the sample part. The y-coupler is omitted since it is no longer necessary for the light to follow a different path to and from the sample.

20 Fig. 6 shows the optimum splitter ratio for the system shown in Fig. (2) investigated in the absence of an optical amplifier, i.e. the amplification factor is set to 1 and the optical noise added from the amplifier is set to zero. The SNR of the system is compared to the reference system, where both systems are used in the uncoated case.

Fig. 7 shows the optimum splitter ratio for the system shown in Fig. (2) investigated in the absence of an optical amplifier, i.e. the amplification factor is set to 1 and the optical noise added from the amplifier is set to zero. The SNR of the system is compared to the reference system, where both systems are used in the coated case.

25 Fig. 8 shows the effect of including an optical amplifier on the novel system shown in Fig. (2). The SNR of the novel system is compared to that of the reference system Fig(5), i.e. $SNR_{\text{novel}} / SNR_{\text{reference}}$, where both systems are used in the uncoated case.

30 Fig. 9 shows the effect of including an optical amplifier on the novel system shown in Fig. (2). The SNR of the novel system is compared to that of the reference system Fig(5), i.e. $SNR_{\text{novel}} / SNR_{\text{reference}}$, where both systems are used in the coated case.

35 Fig. 10 shows the optimum splitting ratio for the novel system shown in Fig. (2), with the optical amplifier set at a fixed amplification factor of 20dB. The SNR of the novel system is compared to the reference system Fig(5), where both systems are used in the uncoated case.

40 Fig. 11 shows the optimum splitting ratio for the novel system shown in Fig. (2), with the optical amplifier set at a fixed amplification factor of 20dB. The SNR of the novel system is compared to the reference system Fig(5), where both systems are used in the coated case.

Fig. 12 shows the relative SNR shown as function of the thermal noise for the system shown in Fig. (4), where the splitting ratio is set to the optimum setting and r_{und} is taken as the coated case.

45 Fig. 13 shows a balanced apparatus according to the invention, wherein only the first reflected light field is amplified by the optical amplifier and hereafter directed to the combining means.

50 Fig. 14 shows the optimum splitter ratio for the system shown in Fig. (13) investigated in the absence of an optical amplifier, i.e. the amplification factor is set to 1 and the optical noise added from the amplifier is set to zero. The SNR of the system is compared to the reference system, where both systems are used in the uncoated case.

Fig. 15 shows the optimum splitter ratio for the system shown in Fig. (13) investigated in the absence of an optical amplifier, i.e. the amplification factor is set to 1 and the optical noise added from the amplifier is set to zero. The SNR of the system is compared to the reference system, where both systems are used in the coated case

55 Fig. 16 shows the effect of including an optical amplifier on the novel system shown in Fig. (13). The SNR of the novel system is compared to that of the reference system Fig(5), i.e. $SNR_{\text{novel}} / SNR_{\text{reference}}$, where both systems are used in the uncoated case.

Fig. 17 shows the effect of including an optical amplifier on the novel system shown in Fig. (13). The SNR of the novel system is compared to that of the reference system Fig(5), i.e. $SNR_{\text{novel}} / SNR_{\text{reference}}$, where both systems are used in the coated case.

5 Fig. 18 shows the optimum splitting ratio for the novel system shown in Fig. (13), with the optical amplifier set at a fixed amplification factor of 20dB. The SNR of the novel system is compared to the reference system Fig(5), where both systems are used in the uncoated case.

10 Fig. 19 shows the optimum splitting ratio for the novel system shown in Fig. (13), with the optical amplifier set at a fixed amplification factor of 20dB. The SNR of the novel system is compared to the reference system Fig(5), where both systems are used in the coated case.

15 Fig. 20 shows the SNR of the novel system shown in Fig. (4), relative to the optimum reference system, as a function of the splitting ratio $x/(1-x)$ in the uncoated case. The optical amplifier is set at a fixed amplification factor of 20 dB. The optimum splitting ratio for the set of parameter values chosen as an example is found to be 75.21/24.79.

20 Fig. 21 shows the SNR of the novel system shown in Fig. (4), relative to the optimum reference system, as a function of the splitting ratio $x/(1-x)$ in the coated case. The optical amplifier is set at a fixed amplification factor of 20 dB. The optimum splitting ratio for the set of parameter values chosen as an example is found to be 75,59/24.41.

Description of the drawings

[0022] In Fig. 1 an unbalanced detection scheme, not according to the invention, is shown for comparison reasons. The optical coherence system is denoted 1. A light source 2 provides a light signal that is directed to a splitting means 3 for dividing said light signal into a first light field 4 and a second light field 5. The splitting ratio in Fig. 1 is set to 50/50. The first reflected light 9 and the second light 10 is combined by the splitter means 3 and a combined signal is directed to the detector 8. The second light field reflected from the reflection means 6 is attenuated by attenuator 7.

[0023] In Fig. 2 a detection scheme according to the invention is depicted. The optical coherence system is denoted 1. A light source 2 provides a light signal that is directed to a splitting means 3 for dividing said light signal into a first light field 4 and a second light field 5. The splitting ratio may be set to any suitable ratio, exemplified by the ratio $x/1-x$. The first reflected light field 9 is directed back through another route than to the splitting means 3, and amplified in the optical amplifier 12, and thereafter directed to the balanced detection means 11 comprising a combining means. The second light field 10 reflected from the reflection means 6 is also directed to the balanced detection means 11. The reflection means 6 is shown as a so-called corner cube configuration.

[0024] The balanced detection means 11 is shown in detail in Fig. 3 comprising a combining means 13, exemplified by a splitter having a splitting ratio of 50/50, capable of splitting the combined signal into first split signal 14 and second split signal 14'. The split signals 14, 14' are directed to the detectors 8, 8' respectively. The two detected split signals are subtracted to obtain an output signal. The output signal may be output via 15 to a printing means, a display and/or a storage means.

[0025] In Fig. 4, a refinement of the system 1 shown in Fig. 2 is shown. To avoid the reduction of the first reflected light field 9 by the splitting means 3, an optical circulator 16 is inserted to direct substantially all the light power in the first reflected light field 9 to the optical amplifier 12.

[0026] In Fig. 13 a preferred detection scheme according to the invention is depicted. The optical coherence system is denoted 1. A light source 2 provides a light signal that is directed to a splitting means 3 for dividing said light signal into a first light field 4 and a second light field 5. The splitting ratio may be set to any suitable ratio, exemplified by the ratio $x/1-x$. The first reflected light field 9 is directed back to the splitting means 3. After the splitter, the first reflected light field 9 is - due to the nature of the splitter used - reduced by the factor $(1-x)$ and directed to the optical amplifier 12, and thereafter to the balanced detection means 11 comprising a combining means. The second light field 10 reflected from the reflection means 6 is also directed to the balanced detection means 11. The reflection means 6 is shown as a so-called corner cube configuration.

Detailed description

[0027] The present invention relates to an apparatus for coherent optical FMCW reflectometry, in particular optical coherence tomography.

[0028] One important aspect of the present invention is the route of the light field in the sample arm. The first reflected light field is amplified before being received by a combining means, said combining means being capable of receiving the first reflected light field from the sample arm as well as the second light field from the reference arm. The amplified

first reflected light field is directed to the combining means through another route than a route through the splitting means for dividing the light signal from the light source into the sample arm and the reference arm, respectively. Thereby, it is possible to direct substantially all light energy from the first reflected light field to the combining means, and to obtain fully the utilisation of the amplification of the first reflected light field. In other words by the present invention the amplified first reflected light field is directed to the combining means, so that only the reflected light field is amplified by the optical amplifier.

[0029] Another important aspect of the invention is that the optical amplifier inserted in the first reflected light field is different from the light source so that the effect of the light source may be regulated independent of the degree of amplification. In particular when using the apparatus in coherent optical FMCW reflectometry certain safety regulations for the power density towards the sample has to be observed to reduce the risk of damages to the sample under examination, such as biological tissue.

Light Source

[0030] The wavelength scanning laser source provides the light signal for use in the method and system.

[0031] The wavelengths scanned are adjusted to the purpose of the analysis performed with the apparatus. The wavelengths are mostly selected in the range from 500 nm to 2000 nm. For non-transparent solid tissue the wavelength is normally selected in the range from 1250 nm to 2000 nm.

[0032] For retinal examinations the wavelength is mostly selected in the range from 600 nm to 1100 nm.

Balanced/unbalanced system

[0033] In general the system or apparatus according to the invention may be constructed as either an unbalanced system or a balanced system. The terms unbalanced and balanced are used in the normal meaning, ie. an unbalanced system refers to a system having one detecting means, whereas a balanced system refers to a system having two detecting means, wherein each detector receives signals from the sample arm as well as from the reference arm. In a balanced system the signals from the two detectors are subtracted from each other in order to obtain the result

[0034] Also a double balanced system may be used in the apparatus according to the invention, a double balanced system referring to a system comprising four detecting means.

Noise

[0035] The noise in the apparatus or system according to the invention is the total sum of noise sources in the following parts:

- Optical noise, such as noise from the light source and noise from the optical amplifier.
- Receiver noise, such as thermal fluctuations in the electronic parts and shot noise.

[0036] The optical noise from the light source is manifested as the phase noise relating to the first reflected light and phase noise relating to the second light as well as phase noise from a mixture of both.

[0037] In the following calculations, a specific configuration for the balanced detection scheme applied to low coherent reflectometry has been chosen. However, the added benefit of introducing an optical amplifier with respect to the signal-to-noise-ratio also applies to other realizations of balanced detection and double balanced detection schemes.

[0038] For the following calculation a balanced detector system is assumed comprising of two detectors and a fiber-optic splitter as shown in Fig. 3.

[0039] The receiving device is assumed to receive two light fields, see Fig. 3: From the reference arm the field is $E_{ref}(t)$ having the intensity $I_{ref}(t)$ from the sample the field is $E_{sam}(t)$ with intensity $I_{sam}(t)$.

[0040] Assuming that the coupler used in the balanced detector, see Fig. 3, is symmetric, the field incident on each detector 1 and detector 2 respectively can be written as

$$\begin{bmatrix} E_1(t) \\ E_2(t) \end{bmatrix} = e^{i\varphi} \begin{bmatrix} a & be^{i\varphi} \\ be^{i\varphi} & a \end{bmatrix} \begin{bmatrix} E_{sam}(t) \\ E_{ref}(t) \end{bmatrix},$$

(1)

where φ_r and φ expresses phase changes due to the coupler, t the time, $j = \sqrt{-1}$ and a and b are coupling constants. It is known from the art that if the coupler is assumed lossless this constraint will mean that $a^2 + b^2 = 1$ and $\varphi = \pm\pi/2$. For a 50/50 coupler $a = b = 1/\sqrt{2}$. Thus for the balanced detector the incident fields are:

$$\begin{bmatrix} E_1(t) \\ E_2(t) \end{bmatrix} = \frac{1}{\sqrt{2}} \begin{bmatrix} 1 & e^{i\pi/2} \\ e^{i\pi/2} & 1 \end{bmatrix} \begin{bmatrix} E_{sam}(t) \\ E_{ref}(t) \end{bmatrix}, \quad (2)$$

where the common phase change φ_r has been assumed zero without loss of generality. Using this it is straight forward to calculate the electrical current i_1 and i_2 in each detector due to a square law detection of the incident light power:

$$\begin{bmatrix} i_1(t) \\ i_2(t) \end{bmatrix} = \frac{1}{2} \alpha \begin{bmatrix} I_{sam}(t) + I_{ref}(t) + E_{sam}(t)E_{ref}^*(t)e^{-i\pi/2} + E_{sam}^*(t)E_{ref}(t)e^{i\pi/2} \\ I_{sam}(t) + I_{ref}(t) + E_{sam}(t)E_{ref}^*(t)e^{i\pi/2} + E_{sam}^*(t)E_{ref}(t)e^{-i\pi/2} \end{bmatrix}. \quad (3)$$

$a = \eta e/h\nu$ is the responsivity of the photodetectors used in a balanced system setup where e is the electron charge, h Planck's constant, ν the average wavelength of the light source, η the quantum efficiency of the photodetectors. Since the balanced detector detects the difference between the two currents, the received electrical signal $i(t)$ becomes:

$$i(t) = -\alpha i (E_{sam}(t)E_{ref}^*(t) - E_{sam}^*(t)E_{ref}(t)) \quad (4)$$

FMCW spectrum

[0041] The signal in a FMCW system is obtained through a narrow line width light source where the frequency is scanned, and the resulting signal current is Fourier-transformed to obtain the desired information. If the optical frequency is scanned linearly and the source is assumed to only exhibit phase noise, the field from the source can be written as

$$\begin{aligned} E_{source}(t') &= E_0 \exp[j(\omega(t')t' + \varphi_r)] \\ &= E_0 \exp[j(\omega_0 t' + \pi\gamma t'^2 + \varphi_r)] \end{aligned} \quad (5)$$

where $\omega(t)$ is the angular frequency as a function of time, ω_0 the angular frequency offset, γ the frequency scan speed E_0 is the amplitude and φ_r is the random fluctuation phase at time t' . The reference field and the field from the sample arm originate from the same source and can be written as:

$$E_{ref}(t) = E_r \exp[j(\omega_0 t + \pi \gamma t^2 + \varphi_r)]$$

(6)

$$E_{sam}(t) = \int_{-\infty}^{\infty} \sqrt{r(\tau_0)} E_s \exp[j(\omega_0(t + \tau_0) + \pi \gamma(t + \tau_0)^2 + \varphi_{s+\tau_0})] d\tau_0$$

(7)

where τ_0 is the time delay due to difference in optical path length between the sample and reference arm, E_r and E_s the respective amplitudes and $r(\tau_0)$ is a function describing the intensity reflectivity profile of the sample arm. This reflectivity profile includes the reflectivity profile of the sample and any undesired reflections in the sample arm e.g. from lenses, fiber ends, etc. Next, we investigate the received signal due to a single reflection in the sample arm i.e. the case where $r(\tau_0) = \delta(\tau_0)$, where δ is the Dirac delta function. Adapting the calculation of the spectrum of the received photocurrent given by S. Venkatesh and W. Sorin ("Phase Noise Considerations in Coherent Optical FMCW Reflectometry", J. of Lightw. Tech., VOL 11, No. 10, 1993) to a balanced system the single sided spectrum of the signal current is found to be

$$\frac{S(f)}{\alpha^2 E_r^2 E_s^2} = 2 \exp\left[-\frac{|f|}{\tau_c \gamma}\right] \delta(f - f_b) + \frac{4\tau_c}{1 + (2\pi|\tau_0|(f - f_b))^2} \left(1 - \exp\left[-\frac{\tau_0}{\tau_c}\right] \left(\cos(2\pi|\tau_0|(f - f_b)) + \frac{\sin(2\pi|\tau_0|(f - f_b))}{2\pi\tau_c(f - f_b)}\right)\right)$$

(8)

where $f_b = \gamma\tau_0$ is the beat frequency due to path length difference between the reference and sample fields, $\tau_c = 1/2\phi\Delta\gamma$ is the coherence time of the light source and $\Delta\gamma$ is the full width half max (FWHM) of the line width of the source.

[0042] The first term of Eq.(8) is the signal due to the reflection in the sample arm, and the second term is a broadband noise contribution due to the phase noise of the light source. Inspecting Eq.(4) it is clear that since there is no mixing terms of the sample field with itself the current resulting from multiple reflections in the sample will be a superposition of the current resulting from each reflection had it been alone. Thus, the single sided spectrum of the signal current is found to be

$$\frac{S(f)}{\alpha^2 E_r^2 E_s^2} = 2 \exp\left[-\frac{|f|}{\tau_c \gamma}\right] r\left(\frac{f}{\gamma}\right) + \int_{-\infty}^{\infty} \frac{4\tau_c r(\tau_0)}{1 + (2\pi|\tau_0|(f - f_b))^2} \left(1 - \exp\left[-\frac{\tau_0}{\tau_c}\right] \left(\cos(2\pi|\tau_0|(f - f_b)) + \frac{\sin(2\pi|\tau_0|(f - f_b))}{2\pi\tau_c(f - f_b)}\right)\right) d\tau_0$$

(9)

Optical Amplification

[0043] In this calculation an optical amplifier is modeled to amplify the incoming light and add optical noise due to intrinsic amplifier noise. Hence, the light intensity emitted from an optical amplifier is given by

$$\langle I_{out} \rangle = G \langle I_{in} \rangle + \langle I_{noise} \rangle,$$

(10)

where G is the amplification factor, I_{in} the intensity of the incident light, and I_{noise} the intensity due to intrinsic amplifier noise. [0044] The term I_{noise} added by the optical amplifier contributes to the system noise in two ways. Firstly, through a mixing term with the reference field in the art known as signal-local oscillator noise, and secondly through adding to the shot noise. According to the art (see e.g. N.A. Olsson, "Lightwave Systems with optical Amplifiers", AT&T Bell Laboratories, J. of Lightwave Tech., Vol. 7, No. 7, 1983) the optical noise power emitted by the optical amplifier is given by

$$\langle I_{noise} \rangle = N_{sp} (G - 1) h \nu B_o,$$

(11)

where N_{sp} is the spontaneous emission factor, ν the center frequency of the optical bandwidth of the amplifier B_o , and h Planck's constant. The bandwidth B_o should be chosen to span over the wavelengths scanned by the light source.

Noise Contributions

[0045] The noise contributions are all expressed as the received noise power after electrical subtraction of the two signals received by each photodetector per unit bandwidth.

Phase noise

[0046] In Eq.(9) the second term represents the noise contribution due to phase noise. To estimate this contribution a realistic reflectivity profile, $r(\tau_0)$, of the sample arm is constructed where the sample is, without loss of generality, chosen to be a highly scattering tissue. This profile consists of three elements: an undesired reflection from the optics before the sample e.g. a fiber end or a lens, the desired reflections inside the sample and a distributed reflectivity exponentially decreasing due to backscattering within the highly scattering tissue. $r(\tau_0)$ is written as

$$r(\tau_0) = r_{und} \delta(\tau_0 - \tau_{und}) + \sum_i r_i \exp[-2\mu\tau_i] \delta(\tau_0 - \tau_i) + r_b \exp[-2\mu\tau_0]$$

(12)

where μ is the damping coefficient of the medium, r_{und} is the reflectivity of the undesired reflection, r_i is the reflectivity of the respective discrete reflection, and r_b is the fraction of the light lost due to damping which goes to backscattering. The noise contribution from phase noise is thus

$$\langle \Delta i_{phase}^2 \rangle = \alpha^2 E_r^2 E_s^2 S_n(f),$$

(13)

where $S_n(f)$ is given by

$$S_n(f) = \int_{-\infty}^{\infty} \frac{4\tau_c r(\tau_0)}{1 + (2\pi|\tau_0|(f - f_b))^2} \left(1 - \exp\left[-\frac{\tau_0}{\tau_c}\right] \left(\cos(2\pi|\tau_0|(f - f_b)) + \frac{\sin(2\pi|\tau_0|(f - f_b))}{2\pi\tau_c(f - f_b)} \right) \right) d\tau_0. \quad (14)$$

5

10 Amplifier noise

[0047] Since the system utilizes a balanced detection scheme the noise emitted by the amplifier, I_{noise} , can only contribute to the noise of the system through mixing with the reference field. This contribution is given by (see e.g. N.A. Olsson, "Lightwave Systems with optical Amplifiers", AT&T Bell Laboratories, J. of Lightwave Tech., Vol. 7, No. 7, 1983):

15

$$\langle \Delta i_{noise}^2 \rangle = 4\alpha^2 h\nu \langle I_{ref} \rangle N_{sp} (G - 1).$$

20

(15)

Shot noise

[0048] It is common knowledge within the art that the so-called shot-noise due to the particle nature of the photon-to-electron conversion in the photodetectors is given by

30

$$\begin{aligned} \langle \Delta i_{shot}^2 \rangle &= 2e\alpha \langle I_{total} \rangle \\ &= 2e\alpha (G \langle I_{sam} \rangle + \langle I_{ref} \rangle + \langle I_{noise} \rangle) \end{aligned}$$

(16)

35

where I_{total} is the total light intensity entering the splitter of the balanced detector (see Fig. (3)).

Receiver noise

[0049] The photodetectors also have an inherent noise contribution, which is independent of the incident light power. There are two contributions to this noise: Thermal noise in the electrical circuit of the detectors and shot-noise due to dark current in photodetector. The receiver noise is:

45

(17)

$$\langle \Delta i_{receiver}^2 \rangle = \langle \Delta i_{thermal}^2 \rangle + \langle \Delta i_{dark}^2 \rangle = 2 \left(\frac{4k_B T}{R} F_n + 2e \langle i_{dark} \rangle \right)$$

50

where k_B is Boltzman's constant, R the load resistance of each of the detectors, T the temperature, F_n the noise figure of the electrical circuit of the detectors normally dominated by the preamplifier, (i_{dark}) the dark current in each detector and the factor of 2 is due to having two independent detectors. However, this receiver noise, independent of the incident light, is often more conveniently measured experimentally.

55

[0050] Thermal fluctuations in the electronic parts are independent of the amount of light used, and furthermore, the thermal fluctuations may be reduced by cooling of the detectors, and also by optimising the construction.

[0051] Shot noise relates to the particle nature of the light. The shot noise is proportional to the amount of light received.

[0052] When inserting an optical amplifier in the apparatus it is inherent that in addition to the amplification of the signal desired the optical noise will inevitably also be amplified.

Received signal power

[0053] From Eq.(8) it can be seen that the signal power due to a single reflection with the time delay to the reference τ_0 is given by

$$\langle i_{signal}^2 \rangle = \exp\left[-\frac{\tau_0}{\tau_c}\right] \alpha^2 E_r^2 E_s^2 \int_{\tau_0}^{\tau_0+\gamma} r(\tau_0) d\tau_0,$$

(18)

when one measures the signal over a finite bandwidth: $\gamma(\tau_0^+-\tau_0^-)$.

Signal-to-Noise Ratio

[0054] Using the above equations it is straightforward to derive the signal-to-noise ratio (SNR):

$$SNR = \frac{\langle i_{signal}^2 \rangle}{B(\langle \Delta i_{receiver}^2 \rangle + \langle \Delta i_{shot}^2 \rangle + \langle \Delta i_{amp}^2 \rangle + \langle \Delta i_{phase}^2 \rangle)},$$

(19)

where B is the bandwidth over which a signal is detected i.e. the resolution of the Fourier-transform of the signal current. However, as the light source is scanned over a finite interval, a time window is imposed upon the signal current leading to a convolution of the signal spectrum with the Fourier-transform of the this time window. The width of this transform determines the resolution of the system together with the bandwidth of the detection system, which determines the smallest frequency increment detectable. Notice, that this bandwidth is decided by the scanning of the light source and the electrical detection system, so in a comparison of the performance of different systems, which uses the same light source and electrical detector system, the bandwidth involved will be a common factor, and is thus ignored for the rest of this analysis.

[0055] For a given light source, sample and electrical detector system the field amplitudes E_r and E_s must be found according to the chosen system configuration. For this analysis the system shown in Fig.(2) has been chosen. From inspection it is straightforward to see that if the light source emits the light intensity I_{source} is then

$$E_r = \sqrt{(1-x)\beta \langle I_{source} \rangle}$$

(20)

and

$$E_s = \sqrt{\frac{1}{4}x\langle I_{source} \rangle}$$

(21)

where x is the coupling ratio towards the sample of the first coupler from the source, and β is a factor describing the loss of power due to an inserted device for altering the optical path length of the second light field, such as a mirror, retro-reflector or fiber-stretcher. For simplicity, and without loss of generality, the factor β is set to unity. This leads to the light intensities

$$\langle I_{ref} \rangle = (1-x)\beta\langle I_{source} \rangle$$

(22)

and

$$\langle I_{sam} \rangle = \frac{1}{4}x\langle I_{source} \rangle \int_{-\infty}^{\infty} r^2(\tau_0) d\tau_0$$

(23)

[0056] Combining Eq.(20), Eq. (21), Eq. (22), and Eq.(23) with Eq. (13), Eq.(15), Eq. (16), Eq. (17) and Eq.(18) it is straight forward to calculate Eq.(19) which can be used for comparison of system performance between different configurations.

[0057] In analogy with this derivation, the SNR can be derived for a wide variety of low-coherent reflectometer systems with balanced detection and thus the performance of such systems can be easily compared.

Splitting means

[0058] The general principle of coherent optical FMCW reflectometry is that distance travelled by the light in the sample arm is correlated to the distance travelled by the light in reference arm.

[0059] The light is emitted from a light source as discussed above and divided into a first light field and a second light field by a splitting means. The splitting means may be any means suitable for splitting a light signal into two light fields. The splitting means may be selected from any suitable splitting means, such as a bulk optic splitting means, a fibre optic splitting means, a holographic optical element or a diffractive optical element.

[0060] In one embodiment the apparatus according to the invention comprises a splitting means capable of dividing the light signal into the sample arm and the reference arm with a splitting ratio of the splitting means being substantially 50%/50%.

[0061] However the present inventors have found due to the location of the amplifier as well as the route of the first reflected light field that a further increase in SNR may be obtained when using a changeable splitting ratio, so that from 1% to 99% of the light energy from the light source is directed to the sample arm. It is preferred that more than 50% of the light energy is directed to the sample, such as from 50% to 99% of the light energy from the light source is directed to the sample arm, such as from 55% to 90% of the light energy from the light source is directed to the sample arm, such as from 60% to 85% of the light energy from the light source is directed to the sample arm, such as from 65% to 85% of the light energy from the light source is directed to the sample arm.

[0062] In another embodiment it is more preferred that from 1% to 60% of the light energy from the light source is directed to the sample arm, such as from 20% to 55% of the light energy from the light source is directed to the sample arm, such as from 30% to 50% of the light energy from the light source is directed to the sample arm, such as from 40

% to 50 % of the light energy from the light source is directed to the sample arm.

Sample arm - first light field route

5 **[0063]** The apparatus according to the invention comprises means for directing the first light field to the sample. In a preferred embodiment at least a part of the means for directing the first light field to the sample comprises an optical fibre, so that the means in total comprises an optical fibre and an optical system. An optical system may be included for focusing the first light field to the sample. The optical system for example being one or more lenses.

10 **[0064]** It is preferred that the first light field is directed to the sample without being amplified. Thereby the intensity of the first light field onto the sample is exclusively determined by the light source. This leads to a better control of the light intensity in the sample arm, since the light directed to the sample conforms to the practical limits for sample light, such as an upper limit for the intensity to avoid damages to the sample, and the light reflected from the sample may be amplified to the degree necessary for the SNR to be suitably increased. Thus, the amplifier is preferably located in a part of the sample arm by which only the reflected light is travelling. This may be accomplished by inserting a splitting means or a circulator to receive the reflected first light field from the sample, or by inserting the optical amplifier after the first reflected light field has passed the splitting means used to split the light into the first and second light fields.

15 **[0065]** In a preferred embodiment a circulator is inserted whereby substantially all light energy reflected from the sample is directed as the first reflected light field to the optical amplifier.

20 **[0066]** The term light field as used herein means light field as normally used for the light in optical fibres, but does also include a light beam as normally used in bulk systems and in the optical system.

Scanning head

25 **[0067]** The sample is scanned by means known in the art, such as galvanometer scanners, polygon mirrors, resonant scanners, a scanning head.

Amplifier

30 **[0068]** Any optical amplifier suitable for amplifying the reflected first light field may be interposed in the light route from the sample to the combining means. The amplifier may thus be a semiconductor, a resonant amplifier or a fibre and/or Raman amplifier. The amplification factor may be in the range from 1.5 to 1,000,000 times, such as from 20 to 500,000 times, for example from 20 to 100,000 times, such as from 20 to 50,000 times, such as from 20 to 10,000 times, such as from 20 to 1000 times, such as from 20 to 100 times.

Reference arm - second light route

35 **[0069]** The apparatus according to the invention also comprises means for directing the second light field to the combining means. In a preferred embodiment a device is included so that the optical path length of the second light route may be altered. In a preferred embodiment hereof at least a part of the directing means is comprised of an optical fiber and an optical fiber stretcher. In another preferred embodiment the device is a reflecting means such as a mirror setup. In this embodiment at least a part of the means for directing the second light field to the reflecting means comprises an optical fibre, so that the directing means in total comprises an optical fibre and an optical system. The optical system may be used for directing the second light field to the reflecting means, such as any kind of lenses, gratings etc. known to the person skilled in the art.

40 **[0070]** Attenuation of the reflected second light field may be useful when using an unbalanced system, whereas attenuation of the reference arm does not add anything further to the SNR in a balanced system.

45 **[0071]** In a preferred embodiment the reflected second light field does not pass any splitting means for dividing the light signal when travelling towards the combining means. It is an advantage to maintain as much as possible of the second light field on the route to the combining means. This may be accomplished by directing the second light field from the splitting means to the combining means in an optical fiber and if it is desired to alter the optical path length of the second light route to modulate the properties of the fiber. This may be done through a fiber stretcher to modulate the physical length of the fiber or by e.g. applying heat to alter the refractive index of the fiber. If a reflecting means is applied to alter the optical path length the light power may substantially be preserved by inserting a circulator to receive the second light field from the reflection means to direct the second light field directly to the combining means.

50 **[0072]** In a preferred embodiment a circulator is inserted to receive the second light field whereby substantially all light energy reflected from the reflecting means is directed as the second light field to the combining means.

55 **[0073]** In another preferred embodiment a fiber stretcher is inserted as described above.

[0074] The reflecting means may be any means suitable for reflecting the light in the reference arm. The reflecting

means may be a mirror or another structure having reflective properties.

Combining means

5 [0075] The combining means is any suitable means capable of receiving two light fields and combining the light fields into at least one light signal. In a preferred embodiment the combining means is a coupler.

[0076] In an unbalanced system the combining means may be identical to the detecting means.

Detecting means

10 [0077] The system comprises conventional detecting means. The detecting means is essentially a photodetector chosen accordingly to match the source wavelength, a combination of photodetectors arranged to make up a balanced scheme, or a combination of photodetectors arranged to make up a double-balanced scheme.

15 Furthermore, the detecting means may be a linear array of photodetectors without or combined with a dispersive element arranged so that the array provides depth and spectral information. The detecting means may also be a linear charge-coupled device (CCD) array without or combined with a dispersive element arranged so that the array provides depth and spectral information.

20 Finally, the detecting means may be a two-dimensional array of photodetectors without or combined with a dispersive element arranged so that the array provides depth and spectral information. The detecting means may also be a two-dimensional CCD array without or combined with a dispersive element arranged so that the array provides depth and spectral information.

For example, the dispersive element may be a diffraction grating (reflection or transmission), a prism or a combination of prisms.

25 End reflections

[0078] In a preferred embodiment the SNR is further increased by reducing non-sample reflections, such as the fibre end reflections in the sample arm. By reducing the non-sample reflections in combination with amplification of the first light field an increase of the relative SNR is increased up to for example about 10 dB, such as up to about 15 dB, for example up to about 20 dB. It has been shown that the amplification of the light field in the sample arm is improved additionally when reducing reflections.

30 [0079] The end reflections may be reduced by anti-reflex coating the fibre ends of the fibres in one or both of the arms.

[0080] Also the fibre ends may be cleaved at an angle to reduce reflections, such an angle being at least 5 degrees, such as preferably at least 7 degrees.

35 [0081] The anti-reflex coating and the cleaving of the fibre ends may be used as alternatives or in combination.

Processing/displaying

40 [0082] The result obtained may be further processed to obtain relevant information based on the detection signal relating to the distance/coherence. In one embodiment the detection signal is sent to a computer for analysis. Depending on the object scanned, the computer may provide an image relating to for example the tissue scanned.

[0083] In relation to detection of inhomogeneities in for example optical waveguides, the computer may provide information relating to the distance to the inhomogeneity and for example also an image of the inhomogeneity.

45 [0084] The result may be sent from the computer to a display and/or a printer and/or stored in a storage means.

Penetration depth

[0085] The parameters that govern coherent optical FMCW reflectometry performance are longitudinal and transverse resolution, dynamic range, measurement speed, and the centre wavelength of the light source.

50 [0086] The depth to which an illumination field of light penetrates within turbid media, such biological tissue or the like, is determined by the amount of scattering and absorption present in the media.

[0087] In tissue scattering diminishes rapidly with increasing wavelength throughout the visible and infrared wavelength regions. Absorption in tissue is dominated by resonant absorption features, and no simple scaling can be assumed. For near-infrared light ($\sim 0.8 \mu\text{m}$), where absorption is relatively weak, scattering is the dominant mechanism of attenuation. At longer wavelengths, such as $1.3 \mu\text{m}$, $1.55 \mu\text{m}$ or $1.9 \mu\text{m}$, scattering is minimal, and water absorption becomes increasingly important

55 [0088] The longitudinal resolution governed by the coherence length is inversely proportional to the optical bandwidth of the light source.

[0089] By the present invention the penetration depths may be increased or even doubled due to the increased SNR depending on the optical properties of the medium.

[0090] The transversal resolution is essentially given by the well-known diffraction limit, i.e. the minimum focal spot, which is the resolving power. The diffraction limit is determined by the wavelength, the effective aperture of the beam and the focal length of the lens as known from the art.

[0091] The measurement speed, i.e. the time to perform a single a-scan and capture the interference signal, may be defined in different ways, and therefore a unique measure for this quantity cannot be given. However, increasing the scan speed implies increasing the electrical bandwidth of the detecting means and this may ultimately lead to an increase of the receiver noise. As shown by the analysis above, the introduction of the optical amplifier amplifying the reflected light from the sample may be even more advantageous if the noise in the detecting means increases. In other words, the optical amplifier may to a certain extent aid to overcome receiver noise.

[0092] Thus, due to the amplification system according to the present invention it is possible to conduct a faster scanning than with state-of-the-art systems.

Transverse scanning

[0093] The light path preferably includes a transverse scanning mechanism for scanning the probe beam within the sample, for example an actuator for moving the apparatus in a direction substantially perpendicular to the sample. Such a scanning mechanism can have a micro-machined scanning mirror. A longitudinal scanning mechanism can also be provided to scan in a direction parallel to the probe beam. Scanning allows the apparatus to create images. Longitudinal scanning in the direction of the probe beam axis, along with scanning in a direction perpendicular to the axis, provides the possibility of obtaining an image of a vertical cross section of the sample.

[0094] It is of course understood that although it is preferred to scan the sample apparatus in relation to the sample, the sample may also be scanned with respect to a stationary sample probe or a combination of these.

Applications

[0095] The apparatus and method according to the present invention may be used in any application normally applying OCT scanning as well new technical fields wherein the increased SNR allows the use of the present apparatus. Thus, the apparatus may be used for so-called optical biopsies, wherein a segment of tissue, such as the skin, mucosa or any other solid tissue is examined by OCT to diagnose any cellular abnormalities, such as cancer or cancer in situ. Furthermore, any malignant growth may be detected by the present apparatus.

[0096] Due to the optical amplification conducted as discussed herein it is possible to increase the relative SNR, for example up to about 20 dB, such as about 17 dB, such as about 14 dB, drastically increasing the penetration depth of the system. Thus, malignancies in the skin or mucosa may be detected directly by using the present invention. Furthermore, the apparatus may be coupled to catheters or the like to scan internal body parts, such as the gastro-intestinal tract, a vessel or the heart or any body cavity. Also, the apparatus may be used for scanning during a surgical operation.

[0097] Also, the present apparatus has improved the use of OCT in ophthalmic application due to the increased penetration depth, such as in corneal topography measurements and as an aid in ophthalmic surgery, for example for focusing on the posterior intraocular lens capsule for use in cataract surgery.

[0098] The present invention may also be applied in conventional OLCR applications, such as detection or imaging of inhomogeneities in optical waveguides or devices, i.e. wherein the sample is an optical waveguide or an integrated optical device.

[0099] In another embodiment the sample may be a polymer or like structure.

[0100] In yet another embodiment the sample may be silicon-based integrated circuit.

Examples

[0101] Here follows a comparison of a coherent optical FMCW reflectometry system according to prior art and two coherent optical FMCW reflectometry systems according to the present invention exemplifying the added benefit of introducing an optical amplifier. The effect of using a system where all undesired reflections has been reduced as much as possible e.g. through coating of all surfaces, as well as the effect of changing the splitting ratio on the splitter from the source, is demonstrated. The former case in which all surfaces are coated is referred to as the coated case, whereas not coating the surfaces is referred to as the uncoated case.

[0102] The system parameters used are

$$\langle I_{source} \rangle = 10 \text{ mW}$$

Scan length of the light source = 100 nm

$$\Delta\gamma = \frac{1}{2\pi\tau_c} = 20 \text{ MHz}$$

$$\text{Center wavelength} = \frac{c}{\nu} = 1050 \text{ nm}$$

$$\gamma = 2.72727 \cdot 10^{18} \text{ Hz/s}$$

$$B_o = \nu_{\max} - \nu_{\min} = 27.2727 \text{ THz}$$

$$N_{sp} = 2$$

$$q = 0.8$$

Receiver noise density = -155 dBm/Hz

and the reflectivity profile of the sample arm is chosen to be

$$r(\tau_0) = r_{und} \delta(\tau_0 - \tau_{und}) + \sum_{i=1}^4 r_i \exp[-2\mu\tau_i] \delta(\tau_0 - \tau_i) + r_b \exp[-2\mu\tau_0] \quad (24)$$

where

$$r_{und} = \begin{cases} 0.04 & \text{in the uncoated case} \\ 10^{-5} & \text{in the coated case} \end{cases}$$

$$r_1 = 0.001 \text{ and } \tau_1 = 0$$

$$r_2 = 0.004 \text{ and } \tau_1 = \frac{c}{(n \cdot 0.5 \text{ mm})}$$

$$r_3 = 0.004 \text{ and } \tau_1 = \frac{c}{(n \cdot 1 \text{ mm})}$$

$$r_4 = 0.004 \text{ and } \tau_1 = \frac{c}{(n \cdot 1.5 \text{ mm})}$$

$$r_b = 10^{-6} \text{ and } \mu = 5 \text{ mm}^{-1}$$

and the Signal-to-noise ratio is inspected for the measurement of the reflectivity r_3 and position τ_3 . Here an attenuation coefficient $\mu_t = 5 \text{ mm}^{-1}$, a probing depth $z = 2 \text{ mm}$, and a reflection coefficient within the sample of 0.4% have been chosen.

Example 1a

a) Choice of reference system

[0103] First, a reference system against which to compare the performance is decided. This system can be seen in Fig. 5. Through a similar analysis as to the one used to derive Eq. (19), the SNR of the reference system may be found. By doing so, it is found that the optimum splitting ratio toward the sample is approximately 35% and 65% towards the reference both for a system with and without coated surfaces. A system with this splitting ratio is chosen as reference

system. This is shown in Fig. 14 and 15 where r_{und} is in the uncoated and coated case, respectively. A system with this splitting ratio is chosen as reference system.

[0104] In the graphs in Fig. 6 - Fig. 11, relative SNR implies that the system under investigation is compared to the corresponding reference system, which experiences the same conditions in terms of reflectivity, receiver noise etc. The novel system in Fig. 2 is compared to the reference system.

b) Optimum splitting ratio in the absence of amplification

[0105] First, the splitting ratio x is investigated in the absence of an amplifier for both the coated and uncoated case. The SNR for this system is found from Eq. (19) by letting $G=1$ and $N_{sp}=0$. Figures 6 and 7 shows the SNR of the system shown in Fig. 2 as a function of the splitter ratio x relative to the reference system Fig. 3 when r_{und} is in the uncoated and coated case, respectively.

[0106] From figures 6 and 7 it is concluded that when an optical amplifier is not present in the system adjusting the splitting ratio away from 50/50 is a disadvantage.

c) Effect of amplification for a constant splitting ratio

[0107] Next, the effect of the amplifier is investigated over a wide range of amplification factors and the splitting ratio is set to 50/50. Fig. 8 shows the increase in SNR due to the use of an optical amplifier in the novel system shown in Fig. 2 for the uncoated case and Fig. 9 shows the increase in SNR in the coated case. It is noted that the relative SNR is less than unity for low amplification factors. This is due to the amplifier having to compensate for the loss of optical signal power due to the extra coupler in the system under investigation and added amplifier noise.

d) Optimum splitting ratio for a fixed amplification

[0108] A conservative amplification factor of 100 (20 dB) is chosen and the effect of choosing a different splitting ratio than 50/50 is investigated again. Fig. 10 and Fig. 11 shows the uncoated and the coated case, respectively. These graphs demonstrate that in both cases it is an advantage to select a different splitting ratio than 50/50 for a system using optical amplification, and that the advantage of doing this is highest in the coated case. In this case the SNR is improved with about 9 dB.

e) Optical circulators and fixed amplification

[0109] Another realization of the novel coherent optical FMCW reflectometry system is shown in Fig. 4, where the γ -coupler in the sample part has been replaced with a so-called optical circulator known from the art. Obviously, the signal light power is increased by a factor of four. Using the same parameters as above in d) for the coated case, the improvement in relative SNR for the realization in Fig. 4 is 31 compared to 10 for the realization in Fig. 2 when both realizations are compared to the same reference system.

[0110] Finally, in Fig. 12 the sensitivity of the relative SNR on the receiver noise is demonstrated for the realization in Fig. 4. For a low thermal noise the optical amplifier may be a disadvantage since the noise is dominated by the noise added by the optical amplifier. As the thermal noise in the receiver is increased the optical amplifier becomes an increased advantage because the optical noise added is gradually masked by the thermal noise. For high values of the thermal noise the advantage of the optical amplifier is constant since the thermal noise is the dominant noise term.

Example 1b

a) Choice of reference system

[0111] The reference system chosen for this example is identical to that of example 1a.

[0112] In the graphs in Fig. 16 - Fig. 21, relative SNR implies that the system under investigation is compared to the corresponding reference system, which experiences the same conditions in terms of reflectivity, receiver noise etc. The novel system in Fig. 13 is compared to the reference system. The SNR for the system shown in Fig. 13 is easily found by replacing Eq. 21 and Eq. 23 in the substitution into Eq. 19 with

$$E_s = \sqrt{(1-x)x\langle I_{source} \rangle}$$

(25)

and

$$\langle I_{sam} \rangle = (1-x)x\langle I_{source} \rangle \int_{-\infty}^{\infty} r^2(\tau_0) d\tau_0 ,$$

(26)

respectively.

c) Effect of amplification for a constant splitting ratio

[0113] Next, the effect of the amplifier is investigated over a wide range of amplification factors and the splitting ratio is set to 50/50. Fig. 16 shows the modest increase in SNR due to the use of the optical amplifier in the uncoated case. This is due to the increase in amplifier noise through mixing of the light due to the undesired reflection r_{und} and the spontaneous noise power emitted by the amplifier. Fig. 17 show the increase in SNR due to the use of the optical amplifier in the coated case. For both cases it is noted that the relative SNR is less than unity for very low amplification factors. This is due to the amplifier having to compensate for the extra noise added by the amplifier.

d) Optimum splitting ratio for a fixed amplification

[0114] A conservative amplification factor of 100 (20 dB) is chosen and the effect of choosing a different splitting ratio than 50/50 is investigated again. Fig. 18 and Fig. 19 shows the uncoated and coated case, respectively. These graphs demonstrate that in both cases it is an advantage to select a different splitting ratio than 50/50 for a system using optical amplification although for chosen system parameters, the advantage is only slight and the optimum splitting ratio is 45/55. It is seen that the relative increase in SNR by inclusion of an optical amplifier is approximately a factor 25 higher in the coated case compared to the uncoated case, and there is little advantage in the uncoated case.

[0115] The system realisations analyzed above should be considered typical examples. However, the advantage of introducing an optical amplifier is clearly pointed out. Firstly, it is demonstrated that the optical amplifier may aid to overcome receiver noise leading to improved system performance in terms increased SNR. The impact of optical amplification on a coherent optical FMCW reflectometry system is highly dependent on the noise contribution from the receiving system, which comprises all components involved in obtaining an electrical signal from the optical output e.g. electrical amplifiers, computer data collection system etc. This sensitivity is illustrated through Fig. 12, where the system with optical amplifier and optical circulator (shown in Fig. 4) is compared to the reference system in the coated case. Secondly, an optimum splitting ratio different from 50/50 has been demonstrated. Finally, adding an optical amplifier will be an increased advantage as the electrical bandwidth of the receiver is increased, which may lead to an increase of the receiver noise. In other words, the optical amplifier may to a certain extent aid to overcome the increase in receiver noise. An increase in electrical detection bandwidth is necessary when fast acquisition of measurement data desired e.g. for real-time imaging.

Claims

1. An apparatus for optical coherence reflectometry comprising

- a wavelength scanning laser source (2) for providing a light signal
- splitting means (3) for dividing said light signal into a first light field (4) and a second light field (5),
- means for directing the first light field to a sample (5), and means for directing a first reflected light field (9) from the sample, wherein an optical amplifier (12) is inserted in the first reflected light field, said optical amplifier being different from the light source, and means for directing the amplified first reflected light field to a combining means (13), so that the amplified first reflected light field is directed to the combining means through another

route than a route through the splitting means for dividing the light signal,

- means for directing the second light field to the combining means,

- combining means for receiving said amplified first reflected light field and said second light field to generate a combined light signal, and

- at least one detecting means (11) for detecting the combined light signal and outputting detection signals.

2. The apparatus according to claim 1, wherein the wavelength scanning laser source is an external-cavity frequency-tuned laser.

3. The apparatus according to claim 1 or 2, wherein the optical amplifier is a semiconductor resonator, amplifier, resonant amplifier, fibre and/or Raman amplifier.

4. The apparatus according to any of the preceding claims, wherein the first light field is directed to the sample without being amplified.

5. The apparatus according to any of the preceding claims, wherein substantially all light energy from the first reflected light field is directed to the combining means.

6. The apparatus according to any of the preceding claims, wherein substantially all light energy from the second light field is directed to the combining means.

7. The apparatus according to any of the preceding claims, wherein the optical path of the second light field comprises a reflecting means, such as a mirror or a retroreflector.

8. The apparatus according to any of the preceding claims, comprising means for altering the optical length of the reference path with the purpose of inducing a frequency shift in the detected signal, such as an optical modulator, for an electro-optic modulator or a fibre stretcher.

9. The apparatus according to any of the preceding claims, wherein the splitting means is bulk-optic, fibre optic or a hologram.

10. The apparatus according to any of the preceding claims, wherein the splitting ratio of the splitting means is substantially 50 %/50 %.

11. The apparatus according to any of the preceding claims 1-9, wherein the splitting ratio of the splitting means is changeable, so that from 1 % to 99 % of the light energy from the light source is directed to a sample arm.

12. The apparatus according to claim 11, wherein less than 50 % of the light energy is directed to the sample arm.

13. The apparatus according to any of the preceding claims, wherein two detecting means are arranged to obtain a balanced detection signal.

14. The apparatus according to any of the preceding claims, wherein at least one CCD camera is arranged as a part of the detecting means to detect a part of the first reflected light field.

15. The apparatus according to any of the preceding claims, wherein at least a part of the means for directing the first light field is an optical fibre.

16. The apparatus according to claim 15, further comprising means for reducing non-sample reflection(s), such as fibre-end reflection(s).

17. The apparatus according to claim 16, wherein the fibre-ends are anti-reflection coated.

18. The apparatus according to claim 16 or 17, wherein the fibre-ends are cleaved at an angle.

19. The apparatus according to claim 18, wherein the angle is at least 5 degrees, such as at least 7 degrees.

20. The apparatus according to any of the preceding claims, further comprising an actuator means for moving the

apparatus in a direction substantially parallel to the sample.

5 21. The apparatus according to any of the preceding claims, further comprising an actuator means for moving the apparatus in a direction substantially perpendicular to the sample.

22. The apparatus according to any of the preceding claims, further comprising processing means for providing a result of the detection signals.

10 23. The apparatus according to claim 22, further comprising a display device displaying the result from the processed detection signals.

24. A method for providing a result of a sample (S) comprising

- 15
- establishing a wavelength scanning laser source (2) for providing a light signal,
 - splitting said light signal into a first light field (4) and a second light field (5),
 - directing the first light field to the sample, and the second light field to a reference path,
 - receiving a first reflected light field (9) from the sample,
 - optically amplifying the first reflected light field,
 - receiving the second light field,

20

 - combining said amplified first reflected light field and said second light field to generate a combined light signal,
 - detecting the combined light signal obtaining detection signals, and
 - processing the detection signals obtaining the result image of the sample.

25 25. The method according to claim 24, wherein the sample is skin or mucosa.

26. The method according to claim 24, wherein the sample is retina.

27. The method according to claim 24, wherein the sample is a vessel or heart:

30 28. The method according to claim 24, applied during a surgical operation.

29. The method according to claim 24, wherein the wavelength scanning laser source is an external-cavity frequency tuned laser.

35 30. The method according to claim 24, wherein the optical amplifier is a semiconductor resonator, an amplifier, a resonant amplifier, fibre and/or Raman amplifier.

40 31. The method according to any of the preceding claims 24-30, wherein the first light field is directed to the sample without being amplified.

32. The method according to any of the preceding claims 24-31, wherein substantially all light energy from the first reflected light field is directed to the combining means.

45 33. The method according to any of the preceding claims 24-32, wherein substantially all light energy from the second light field is directed to the combining means.

34. The method according to any of the preceding claims 24-33, wherein the optical path of the second light field comprises a reflecting means, such as a mirror or a retroreflector.

50 35. The method according to any of the preceding claims 24-34, wherein the splitting means is bulk-optic, fibre optic or a hologram.

55 36. The method according to any of the preceding claims 24-35, wherein the splitting ratio of the splitting means is substantially 50 %/50 %.

37. The method according to any of the preceding claims 24-36, wherein the splitting ratio of the splitting means is changeable, so that from 1% to 99 % of the light energy from the light source is directed to the sample arm.

38. The method according to claim 37, wherein less than 50 % of the light energy is directed to the sample arm.
39. The method according to any of the preceding claims 24-38, wherein two detecting means are arranged to obtain a balanced detection signal.
- 5 40. The method according to any of the preceding claims 24-39, wherein at least a part of the means for directing the first light field is an optical fibre.
- 10 41. The method according to claim 40, further comprising means for reducing non-sample reflection(s), such as fibre-end reflection(s).
42. The method according to claim 41, wherein the fibre-ends are anti-reflection coated.
43. The method according to claim 41 or 42, wherein the fibre-ends are cleaved at an angle.
- 15 44. The method according to claim 43, wherein the angle is at least 5 degrees, such as at least 7 degrees.
45. The method according to any of the preceding claims 24-44, further comprising an actuator means for moving the first light field in a direction substantially parallel to the sample.
- 20 46. The method according to any of the preceding claims 24-45, further comprising an actuator means for moving the first light field in a direction substantially perpendicular to the sample.
47. The method according to claim 24, wherein the wavelength of the light source is in the range from 500 nm to 2000 nm.
- 25 48. The method according to claim 25 or 27, wherein the wavelength of the light source is in the range from 1250 nm to 2000 nm.
- 30 49. The method according to claim 26, wherein the wavelength of the light source is in the range from 600 nm to 1100 nm.

Patentansprüche

1. Vorrichtung für die optische Kohärenzreflektometrie, umfassend:

- 35 - eine Wellenlängen-Abtastlaserquelle (2) zum Bereitstellen eines Lichtsignals
- ein Spaltmittel (3) zum Teilen des Lichtsignals in ein erstes Lichtfeld (4) und ein zweites Lichtfeld (5),
- Mittel zum Lenken des ersten Lichtfelds zu einer Probe (5), und Mittel zum Lenken eines ersten reflektierten Lichtfelds (9) von der Probe, wobei ein optischer Verstärker (12) in das erste reflektierte Lichtfeld eingefügt ist,
40 wobei der optische Verstärker von der Lichtquelle verschieden ist, sowie Mittel zum Lenken des verstärkten, ersten reflektierten Lichtfelds zu einem Kombiniermittel (13), so daß das verstärkte, erste reflektierte Lichtfeld über eine andere Strecke als eine Strecke durch das Spaltmittel zum Trennen des Lichtsignals zu dem Kombiniermittel gelenkt wird,
- Mittel zum Lenken des zweiten Lichtfelds zu dem Kombiniermittel,
45 - ein Kombiniermittel zum Empfangen des verstärkten, ersten reflektierten Lichtfelds und des zweiten Lichtfelds, um ein kombiniertes Lichtsignal zu erzeugen, und
- wenigstens ein Detektiermittel (11) zum Detektieren des kombinierten Lichtsignals und zum Ausgeben von Detektionssignalen.

50 2. Vorrichtung nach Anspruch 1, wobei es sich bei der Wellenlängen-Abtastlaserquelle um einen frequenznachgesteuerten External-Cavity-Laser handelt.

3. Vorrichtung nach Anspruch 1 oder 2, wobei es sich bei dem optischen Verstärker um einen Halbleiterresonator, einen Verstärker, einen Resonanzverstärker, einen Faser- und/oder Raman-Verstärker handelt.

55 4. Vorrichtung nach einem der vorangegangenen Ansprüche, wobei das erste Lichtfeld unverstärkt zu der Probe gelenkt wird.

EP 1 356 250 B1

5. Vorrichtung nach einem der vorangegangenen Ansprüche, wobei im wesentlichen die gesamte Lichtenergie von dem ersten reflektierten Lichtfeld zu dem Kombiniermittel gelenkt wird.
- 5 6. Vorrichtung nach einem der vorangegangenen Ansprüche, wobei im wesentlichen die gesamte Lichtenergie von dem zweiten Lichtfeld zu dem Kombiniermittel gelenkt wird.
7. Vorrichtung nach einem der vorangegangenen Ansprüche, wobei der optische Weg des zweiten Lichtfelds ein Reflexionsmittel, wie beispielsweise einen Spiegel oder einen Retro-Reflektor umfaßt.
- 10 8. Vorrichtung nach einem der vorangegangenen Ansprüche, umfassend Mittel zum Abändern der optischen Länge des Referenzwegs, mit dem Zweck, eine Frequenzverschiebung bei dem detektierten Signal herbeizuführen, wie beispielsweise einen optischen Modulator, oder einen elektrooptischen Modulator oder eine Faserstreckvorrichtung.
- 15 9. Vorrichtung nach einem der vorangegangenen Ansprüche, wobei das Spaltmittel massivoptisch, faseroptisch oder ein Hologramm ist.
10. Vorrichtung nach einem der vorangegangenen Ansprüche, wobei das Spaltverhältnis im wesentlichen 50 % : 50 % beträgt.
- 20 11. Vorrichtung nach einem der vorangegangenen Ansprüche 1 - 9, wobei das Spaltverhältnis des Spaltmittels veränderbar ist, so daß von 1 % bis 99 % der Lichtenergie von der Lichtquelle zu einem Probenarm gelenkt werden.
12. Vorrichtung nach Anspruch 11, wobei weniger als 50 % der Lichtenergie zu dem Probenarm gelenkt werden.
- 25 13. Vorrichtung nach einem der vorangegangenen Ansprüche, wobei zwei Detektiermittel eingerichtet sind, um ein symmetrisches Detektionssignal zu gewinnen.
14. Vorrichtung nach einem der vorangegangenen Ansprüche, wobei wenigstens eine ladungsgekoppelte Kamera als Teil des Detektiermittels eingerichtet ist, um einen Teil des ersten reflektierten Lichtfelds zu detektieren.
- 30 15. Vorrichtung nach einem der vorangegangenen Ansprüche, wobei wenigstens ein Teil des Mittels zum Lenken des ersten Lichtfelds eine Lichtleitfaser ist.
16. Vorrichtung nach Anspruch 15, welche ferner Mittel zum Reduzieren nichtprobenrelevanter Reflexion bzw. nichtprobenrelevanten Reflexionen, wie beispielsweise Faserend-Reflexion(en), umfaßt.
- 35 17. Vorrichtung nach Anspruch 16, wobei die Faserenden antireflexionsbeschichtet sind.
18. Vorrichtung nach Anspruch 16 oder 17, wobei die Faserenden in einem Winkel gespalten sind.
- 40 19. Vorrichtung nach Anspruch 18, wobei der Winkel wenigstens 5 Grad, beispielsweise wenigstens 7 Grad beträgt.
20. Vorrichtung nach einem der vorangegangenen Ansprüche, ferner umfassend ein Betätigungsmittel, um die Vorrichtung in eine im wesentlichen parallel zu der Probe verlaufende Richtung zu bewegen.
- 45 21. Vorrichtung nach einem der vorangegangenen Ansprüche, ferner umfassend ein Betätigungsmittel, um die Vorrichtung in eine im wesentlichen senkrecht zu der Probe verlaufende Richtung zu bewegen.
22. Vorrichtung nach einem der vorangegangenen Ansprüche, ferner umfassend ein Verarbeitungsmittel, um ein Ergebnis aus den Detektionssignalen bereitzustellen.
- 50 23. Vorrichtung nach Anspruch 22, welche ferner eine Anzeigeeinrichtung umfaßt, die das Ergebnis aus den verarbeiteten Detektionssignalen anzeigt.
- 55 24. Verfahren zum Bereitstellen eines Ergebnisses einer Probe (S), umfassend:
- Einrichten einer Wellenlängen-Abtastlaserquelle (2) zum Bereitstellen eines Lichtsignals,
 - Spalten des Lichtsignals in ein erstes Lichtfeld (4) und ein zweites Lichtfeld (5),

EP 1 356 250 B1

- Lenken des ersten Lichtfelds zu der Probe und des zweiten Lichtfelds zu einem Referenzweg,
 - Empfangen eines ersten reflektierten Lichtfeldes (9) von der Probe,
 - optisches Verstärken des ersten reflektierten Lichtfeldes,
 - Empfang des zweiten Lichtfeldes,
 - Kombinieren des verstärkten ersten reflektierten Lichtfeldes und des zweiten Lichtfeldes, um ein kombiniertes Lichtsignal zu erzeugen,
 - Detektieren des kombinierten Lichtsignals, wobei Detektionssignale gewonnen werden, und
 - Verarbeiten der Detektionssignale, wobei das Ergebnisbild der Probe gewonnen wird.
- 5
- 10 **25.** Verfahren nach Anspruch 24, wobei es sich bei der Probe um Haut oder Schleimhaut handelt.
- 26.** Verfahren nach Anspruch 24, wobei es sich bei der Probe um Netzhaut handelt.
- 27.** Verfahren nach Anspruch 24, wobei es sich bei der Probe um ein Gefäß oder Herz handelt.
- 15 **28.** Verfahren nach Anspruch 24, angewandt während eines chirurgischen Eingriffs.
- 29.** Verfahren nach Anspruch 24, wobei es sich bei der Wellenlängen-Abtastlaserquelle um einen frequenznachgesteuerten External-Cavity-Laser handelt.
- 20 **30.** Verfahren nach Anspruch 24, wobei es sich bei dem optischen Verstärker um einen Halbleiterresonator, einen Verstärker, einen Resonanzverstärker, einen Faser- und/oder Raman-Verstärker handelt.
- 31.** Verfahren nach einem der vorangegangenen Ansprüche 24 - 30, wobei das erste Lichtfeld unverstärkt zu der Probe gelenkt wird.
- 25 **32.** Verfahren nach einem der vorangegangenen Ansprüche 24 - 31, wobei im wesentlichen die gesamte Lichtenergie von dem ersten reflektierten Lichtfeld zu dem Kombiniermittel gelenkt wird.
- 33.** Verfahren nach einem der vorangegangenen Ansprüche 24 - 32, wobei im wesentlichen die gesamte Lichtenergie von dem zweiten Lichtfeld zu dem Kombiniermittel gelenkt wird.
- 30 **34.** Verfahren nach einem der vorangegangenen Ansprüche 24 - 33, wobei der optische Weg des zweiten Lichtfelds ein Reflexionsmittel, wie beispielsweise einen Spiegel oder einen Retro-Reflektor umfaßt.
- 35 **35.** Verfahren nach einem der vorangegangenen Ansprüche 24 -34, wobei das Spaltmittel massivoptisch, faseroptisch oder ein Hologramm ist.
- 36.** Verfahren nach einem der vorangegangenen Ansprüche 24 - 35, wobei das Spaltverhältnis des Spaltmittels im wesentlichen 50 % : 50 % beträgt.
- 40 **37.** Verfahren nach einem der vorangegangenen Ansprüche 24-36, wobei das Spaltverhältnis des Spaltmittels veränderbar ist, so daß von 1 % bis 99 % der Lichtenergie von der Lichtquelle zu dem Probenarm gelenkt werden.
- 38.** Verfahren nach Anspruch 37, wobei weniger als 50 % der Lichtenergie zu dem Probenarm gelenkt werden.
- 45 **39.** Verfahren nach einem der vorangegangenen Ansprüche 24 - 38, wobei zwei Detektiermittel eingerichtet sind, um ein symmetrisches Detektionssignal zu gewinnen.
- 40.** Verfahren nach einem der vorangegangenen Ansprüche 24 - 39, wobei wenigstens ein Teil des Mittels zum Lenken des ersten Lichtfelds eine Lichtleitfaser ist.
- 50 **41.** Verfahren nach Anspruch 40, welches ferner Mittel zum Reduzieren von nichtprobenrelevanter Reflexion bzw. nichtprobenrelevanten Reflexionen, wie beispielsweise Faserend-Reflexion(en), umfaßt.
- 55 **42.** Verfahren nach Anspruch 41, wobei die Faserenden antireflexionsbeschichtet sind.
- 43.** Verfahren nach Anspruch 41 oder 42, wobei die Faserenden in einem Winkel gespalten sind.

EP 1 356 250 B1

44. Verfahren nach Anspruch 43, wobei der Winkel wenigstens 5 Grad, beispielsweise wenigstens 7 Grad beträgt.
45. Verfahren nach einem der vorangegangenen Ansprüche 24 - 44, ferner umfassend ein Betätigungsmittel, um das erste Lichtfeld in eine im wesentlichen parallel zu der Probe verlaufende Richtung zu bewegen.
46. Verfahren nach einem der vorangegangenen Ansprüche 24 - 45, ferner umfassend ein Betätigungsmittel, um das erste Lichtfeld in eine im wesentlichen senkrecht zu der Probe verlaufende Richtung zu bewegen.
47. Verfahren nach Anspruch 24, wobei die Wellenlänge der Lichtquelle in dem Bereich von 500 nm bis 2000 nm liegt.
48. Verfahren nach Anspruch 25 oder 27, wobei die Wellenlänge der Lichtquelle in dem Bereich von 1250 nm bis 2000 nm liegt.
49. Verfahren nach Anspruch 26, wobei die Wellenlänge der Lichtquelle in dem Bereich von 600 nm bis 1100 nm gelegen ist.

Revendications

1. Appareil pour réflectométrie par cohérence optique comprenant :
- une source laser à balayage de longueur d'onde (2) pour fournir un signal lumineux
 - des moyens diviseurs (3) pour diviser ledit signal lumineux en un premier champ lumineux (4) et un second champ lumineux (5),
 - des moyens pour diriger le premier champ lumineux jusqu'à un échantillon (5), et des moyens pour diriger un premier champ lumineux réfléchi (9) à partir de l'échantillon, dans lequel un amplificateur optique (12) est inséré dans le premier champ lumineux réfléchi, ledit amplificateur optique étant différent de la source lumineuse, et des moyens pour diriger le premier champ lumineux réfléchi amplifié jusqu'à des moyens de combinaison (13), de sorte que le premier champ lumineux réfléchi amplifié soit dirigé jusqu'aux moyens de combinaison à travers un autre chemin qu'un chemin à travers les moyens diviseurs pour diviser le signal lumineux,
 - des moyens pour diriger le second champ lumineux jusqu'aux moyens de combinaison,
 - des moyens de combinaison pour recevoir ledit premier champ lumineux réfléchi amplifié et ledit second champ lumineux pour générer un signal lumineux combiné, et
 - au moins un premier ensemble de moyens de détection (11) pour détecter le signal lumineux combiné et envoyer des signaux de détection.
2. Appareil selon la revendication 1, dans lequel la source laser à balayage de longueur d'onde est un laser accordé en fréquence à cavité externe.
3. Appareil selon la revendication 1 ou 2, dans lequel l'amplificateur optique est un résonateur à semi-conducteur, amplificateur, amplificateur résonant, fibre et/ou amplificateur Raman.
4. Appareil selon une quelconque des revendications précédentes, dans lequel le premier champ lumineux est dirigé jusqu'à l'échantillon sans être amplifié.
5. Appareil selon une quelconque des revendications précédentes, dans lequel sensiblement toute l'énergie lumineuse à partir du premier champ lumineux réfléchi est dirigée jusqu'aux moyens de combinaison.
6. Appareil selon une quelconque des revendications précédentes, dans lequel sensiblement toute l'énergie lumineuse à partir du second champ lumineux est dirigée jusqu'aux moyens de combinaison.
7. Appareil selon une quelconque des revendications précédentes, dans lequel le chemin optique du second champ lumineux comprend des moyens réfléchissants, tels qu'un miroir ou un rétro-rélecteur.
8. Appareil selon une quelconque des revendications précédentes, comprenant des moyens pour modifier la longueur optique du chemin de référence dans le but de provoquer un glissement de fréquence dans le signal détecté, tels qu'un modulateur optique, pour un modulateur électro-optique ou un allongeur de fibre.

EP 1 356 250 B1

9. Appareil selon une quelconque des revendications précédentes, dans lequel les moyens diviseurs sont un élément optique volumineux, une fibre optique ou un hologramme.
- 5 10. Appareil selon une quelconque des revendications précédentes, dans lequel le rapport de division des moyens diviseurs est sensiblement 50 %/50 %.
- 10 11. Appareil selon une quelconque des revendications précédentes 1 à 9, dans lequel le rapport de division des moyens diviseurs peut être changé, de sorte que d'1 % à 99 % de l'énergie lumineuse à partir de la source lumineuse soit dirigé jusqu'à un bras d'échantillon.
12. Appareil selon la revendication 11, dans lequel moins de 50 % de l'énergie lumineuse est dirigé jusqu'au bras d'échantillon.
- 15 13. Appareil selon une quelconque des revendications précédentes, dans lequel deux ensembles de moyens de détection sont agencés pour obtenir un signal de détection équilibré.
- 20 14. Appareil selon une quelconque des revendications précédentes, dans lequel au moins une caméra à dispositif à transfert de charge (« CCD ») est agencée en tant que partie des moyens de détection pour détecter une partie du premier champ lumineux réfléchi.
- 25 15. Appareil selon une quelconque des revendications précédentes, dans lequel au moins une partie des moyens pour diriger le premier champ lumineux est une fibre optique.
16. Appareil selon la revendication 15, comprenant en outre des moyens pour réduire des réflexion(s) de non-échantillon, telles que des réflexion(s) d'extrémité de fibre.
17. Appareil selon la revendication 16, dans lequel les extrémités de fibre sont enduites de revêtement anti-réflexion.
- 30 18. Appareil selon la revendication 16 ou 17, dans lequel les extrémités de fibre sont coupées à un angle.
19. Appareil selon la revendication 18, dans lequel l'angle est au moins 5 degrés, tel qu'au moins 7 degrés.
- 35 20. Appareil selon une quelconque des revendications précédentes, comprenant en outre des moyens actionneurs pour déplacer l'appareil dans une direction sensiblement parallèle à l'échantillon.
21. Appareil selon une quelconque des revendications précédentes, comprenant en outre des moyens actionneurs pour déplacer l'appareil dans une direction sensiblement perpendiculaire à l'échantillon.
- 40 22. Appareil selon une quelconque des revendications précédentes, comprenant en outre des moyens de traitement pour fournir un résultat des signaux de détection.
23. Appareil selon la revendication 22, comprenant en outre un dispositif d'affichage affichant le résultat à partir des signaux de détection traités.
- 45 24. Procédé pour fournir un résultat d'un échantillon (5) comprenant les étapes consistant à :
- établir une source laser à balayage de longueur d'onde (2) pour fournir un signal lumineux,
 - diviser ledit signal lumineux en un premier champ lumineux (4) et un second champ lumineux (5),
 - diriger le premier champ lumineux jusqu'à l'échantillon, et le second champ lumineux jusqu'à un chemin de
 - 50 référence,
 - recevoir un premier champ lumineux réfléchi (9) à partir de l'échantillon,
 - amplifier optiquement le premier champ lumineux réfléchi,
 - recevoir le second champ lumineux,
 - combiner ledit premier champ lumineux réfléchi amplifié et ledit second champ lumineux pour générer un
 - 55 signal lumineux combiné,
 - détecter le signal lumineux combiné obtenant des signaux de détection, et
 - traiter les signaux de détection obtenant le résultat image de l'échantillon.

EP 1 356 250 B1

25. Procédé selon la revendication 24, dans lequel l'échantillon est de la peau ou muqueuse.
26. Procédé selon la revendication 24, dans lequel l'échantillon est une rétine.
- 5 27. Procédé selon la revendication 24, dans lequel l'échantillon est un vaisseau ou coeur.
28. Procédé selon la revendication 24, appliqué au cours d'une opération chirurgicale.
29. Procédé selon la revendication 24, dans lequel la source laser à balayage de longueur d'onde est un laser accordé
10 en fréquence à cavité externe.
30. Procédé selon la revendication 24, dans lequel l'amplificateur optique est un résonateur à semi-conducteur, un amplificateur, un amplificateur résonant, fibre et/ou amplificateur Raman.
- 15 31. Procédé selon une quelconque des revendications précédentes 24 à 30, dans lequel le premier champ lumineux est dirigé jusqu'à l'échantillon sans être amplifié.
32. Procédé selon une quelconque des revendications précédentes 24 à 31, dans lequel sensiblement toute l'énergie
20 lumineuse à partir du premier champ lumineux réfléchi est dirigée jusqu'aux moyens de combinaison.
33. Procédé selon une quelconque des revendications précédentes 24 à 32, dans lequel sensiblement toute l'énergie lumineuse à partir du second champ lumineux est dirigée jusqu'aux moyens de combinaison.
34. Procédé selon une quelconque des revendications précédentes 24 à 33, dans lequel le chemin optique du second
25 champ lumineux comprend des moyens réfléchissants, tels qu'un miroir ou un rétro-rélecteur.
35. Procédé selon une quelconque des revendications précédentes 24 à 34, dans lequel les moyens de division sont un élément optique volumineux, une fibre optique ou un hologramme.
- 30 36. Procédé selon une quelconque des revendications précédentes 24 à 35, dans lequel le rapport de division des moyens diviseurs est sensiblement 50 %/50 %.
37. Procédé selon une quelconque des revendications précédentes 24 à 36, dans lequel le rapport de division des
35 moyens diviseurs peut être changé, de sorte que d'1 % à 99 % de l'énergie lumineuse à partir de la source lumineuse soit dirigé jusqu'au bras d'échantillon.
38. Procédé selon la revendication 37, dans lequel moins de 50 % de l'énergie lumineuse est dirigé jusqu'au bras d'échantillon.
- 40 39. Procédé selon une quelconque des revendications précédentes 24 à 38, dans lequel deux ensembles de moyens de détection sont agencés pour obtenir un signal de détection équilibré.
40. Procédé selon une quelconque des revendications précédentes 24 à 39, dans lequel au moins une partie des
45 moyens pour diriger le premier champ lumineux est une fibre optique.
41. Procédé selon la revendication 40, comprenant en outre des moyens pour réduire des réflexion(s) de non-échantillon, telles que des réflexion(s) d'extrémité de fibre.
42. Procédé selon la revendication 41, dans lequel les extrémités de fibre sont enduites de revêtement anti-réflexion.
- 50 43. Procédé selon la revendication 41 ou 42, dans lequel les extrémités de fibre sont coupées à un angle.
44. Procédé selon la revendication 43, dans lequel l'angle est au moins 5 degrés, tel qu'au moins 7 degrés.
- 55 45. Procédé selon une quelconque des revendications précédentes 24 à 44, comprenant en outre des moyens actionneurs pour déplacer le premier champ lumineux dans une direction sensiblement parallèle à l'échantillon.
46. Procédé selon une quelconque des revendications précédentes 24 à 45, comprenant en outre des moyens action-

EP 1 356 250 B1

neurs pour déplacer le premier champ lumineux dans une direction sensiblement perpendiculaire à l'échantillon.

5 47. Procédé selon la revendication 24, dans lequel la longueur d'onde de la source lumineuse est dans la plage de 500 nm à 2000 nm.

10 48. Procédé selon la revendication 25 ou 27, dans lequel la longueur d'onde de la source lumineuse est dans la plage de 1250 nm à 2000 nm.

15 49. Procédé selon la revendication 26, dans lequel la longueur d'onde de la source lumineuse est dans la plage de 600 nm à 1100 nm.

20

25

30

35


40


45

50

55

Fig. 1

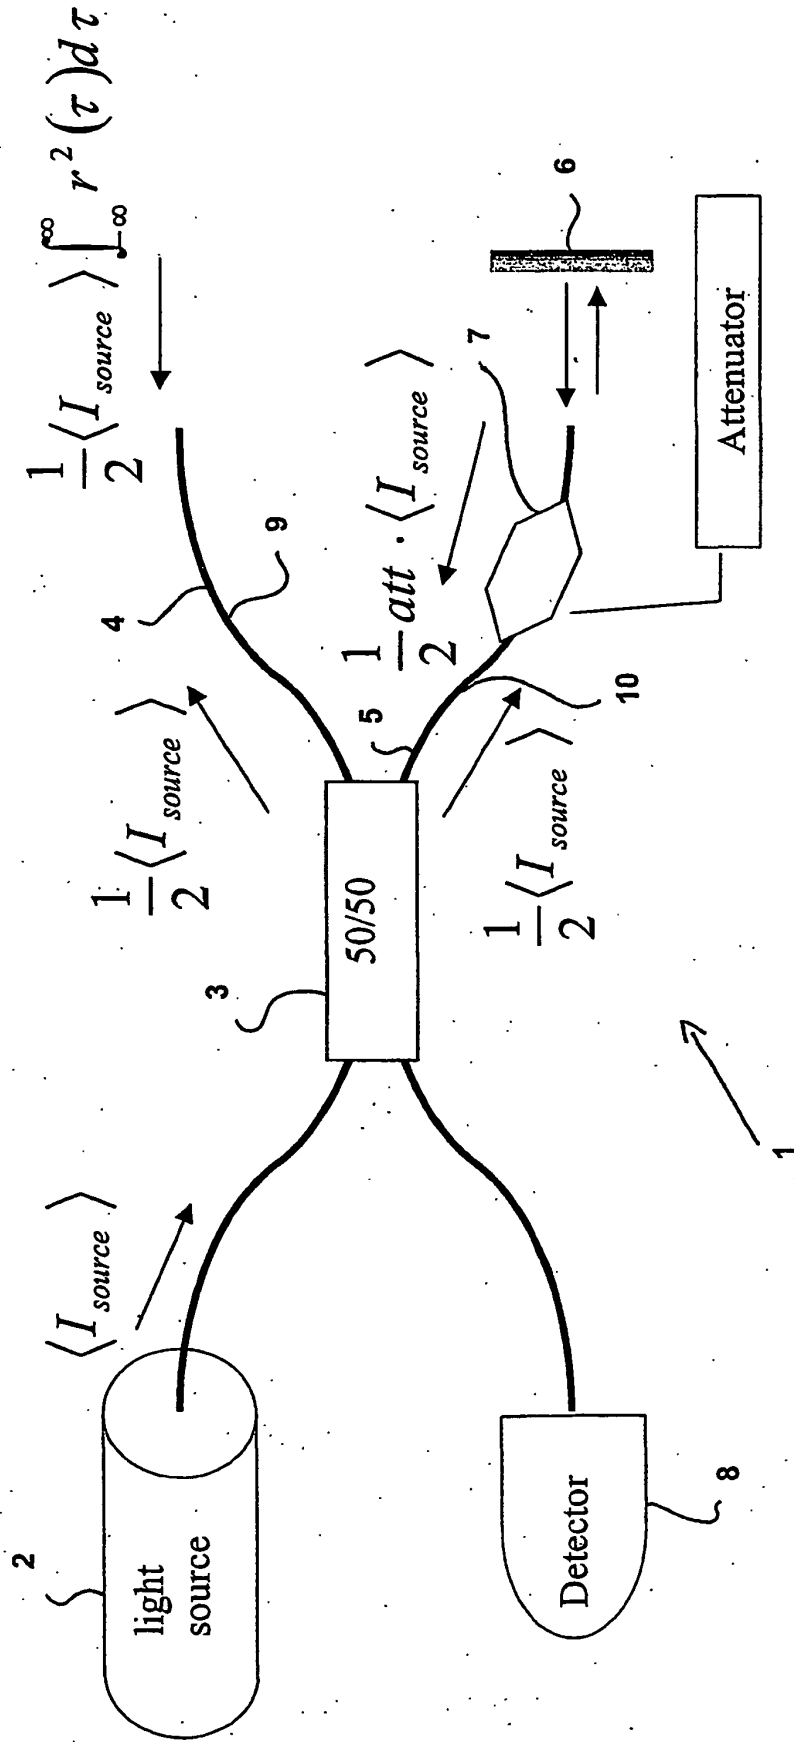

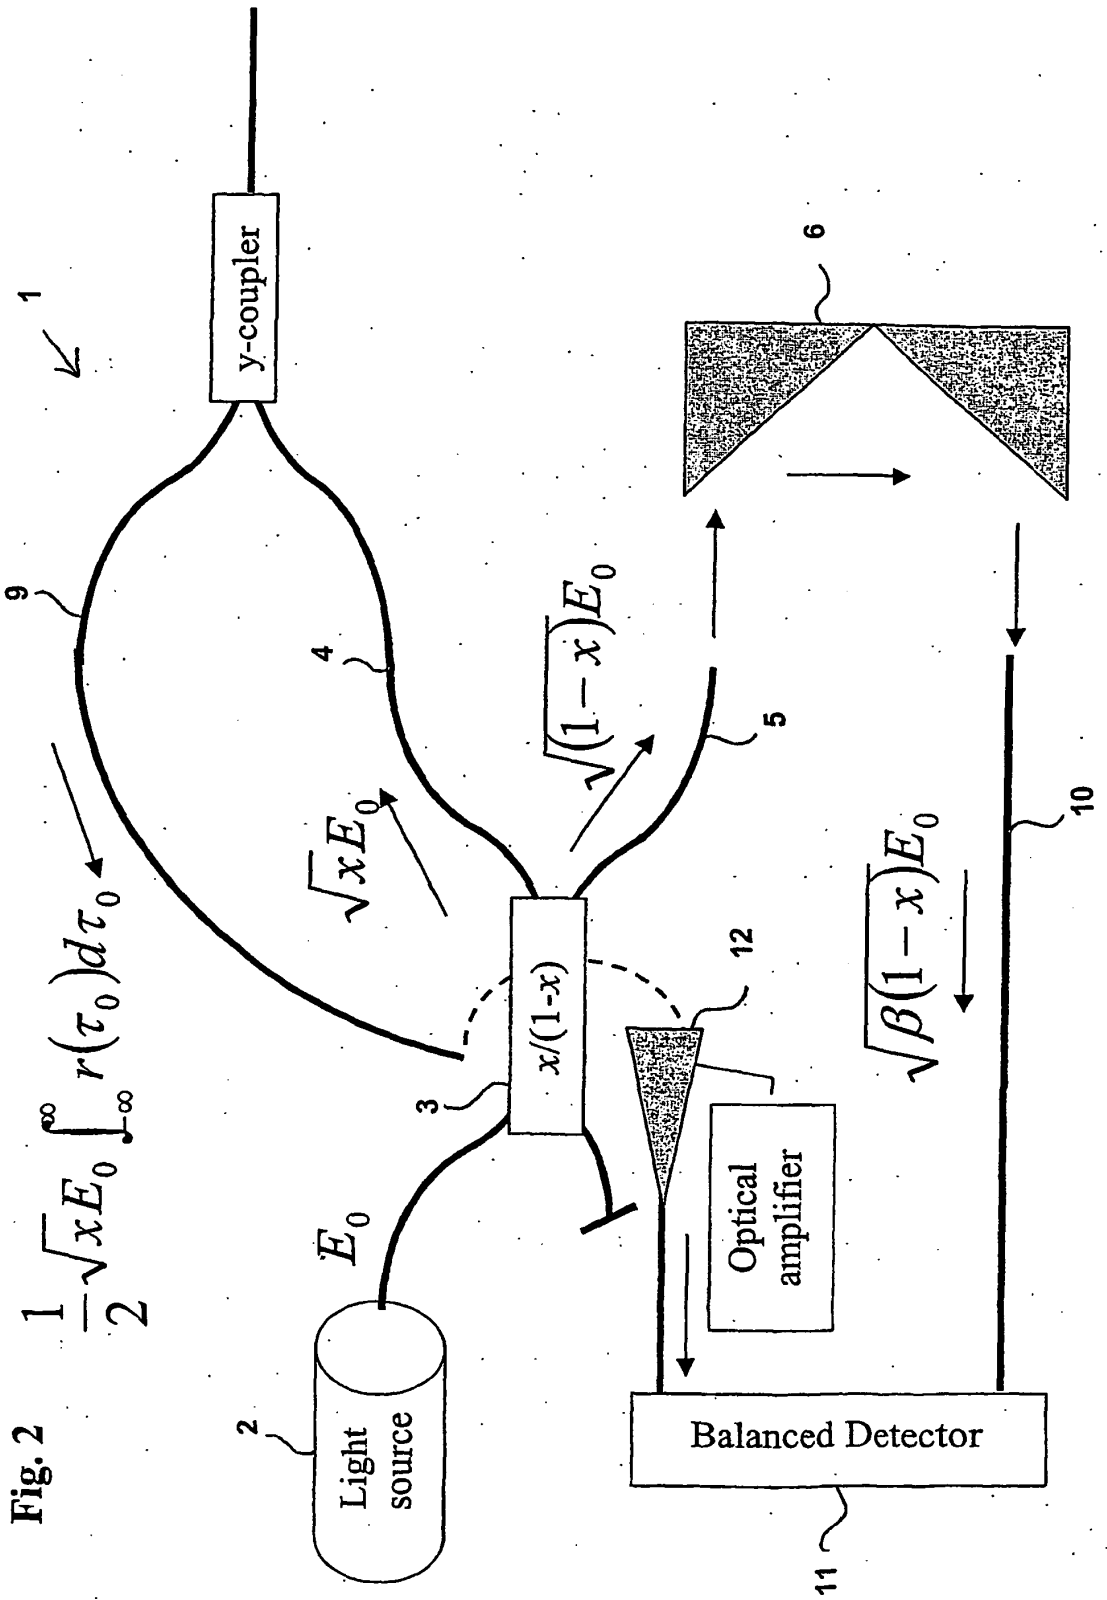

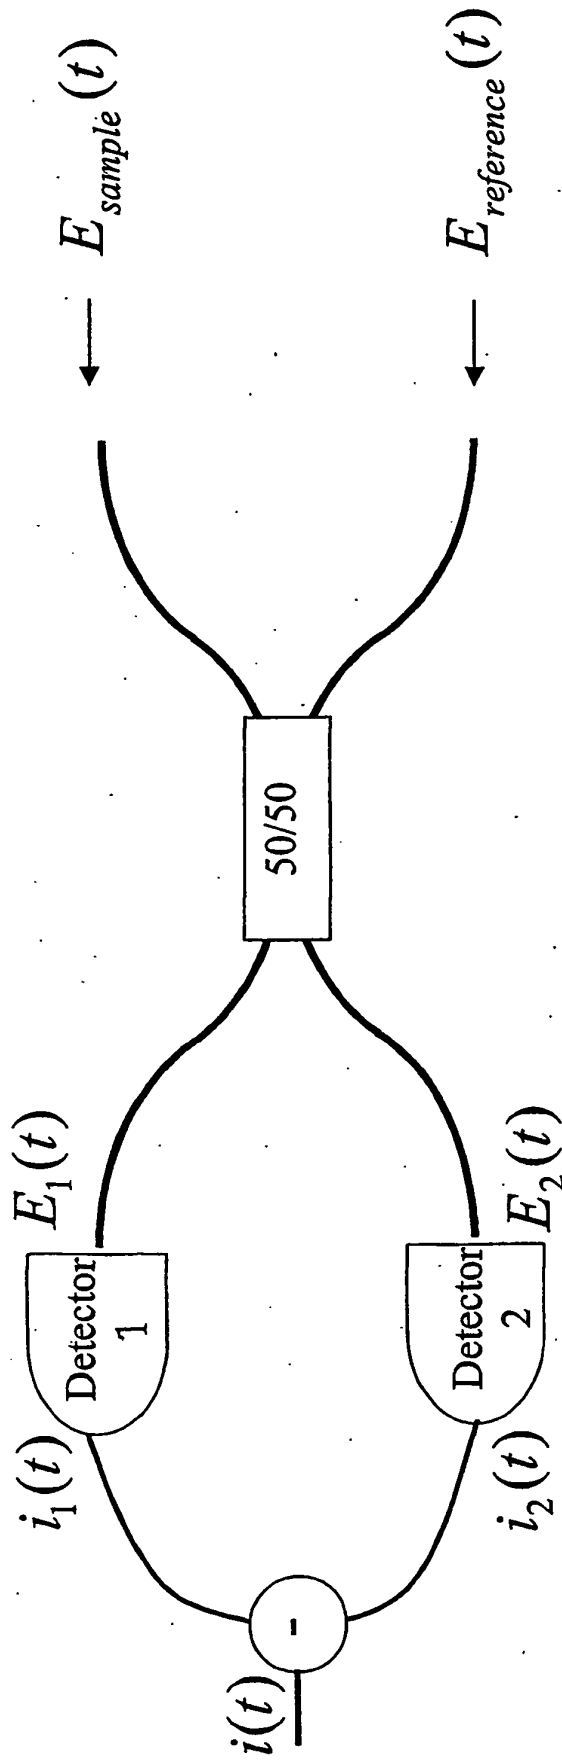
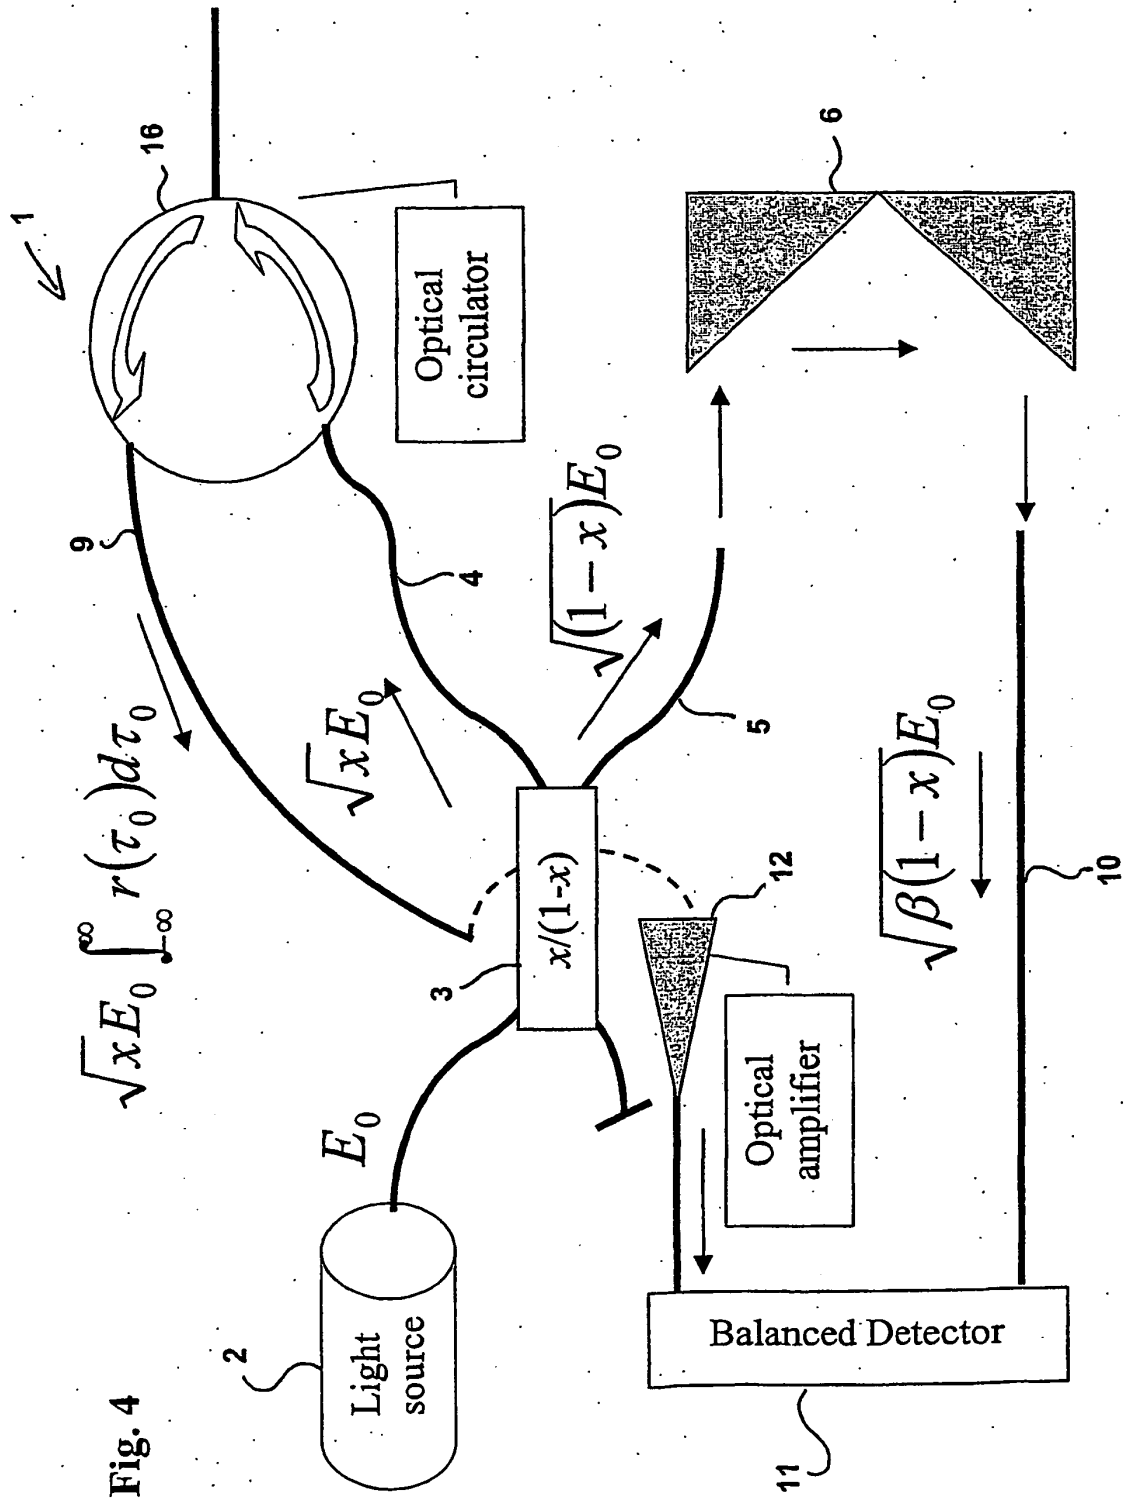
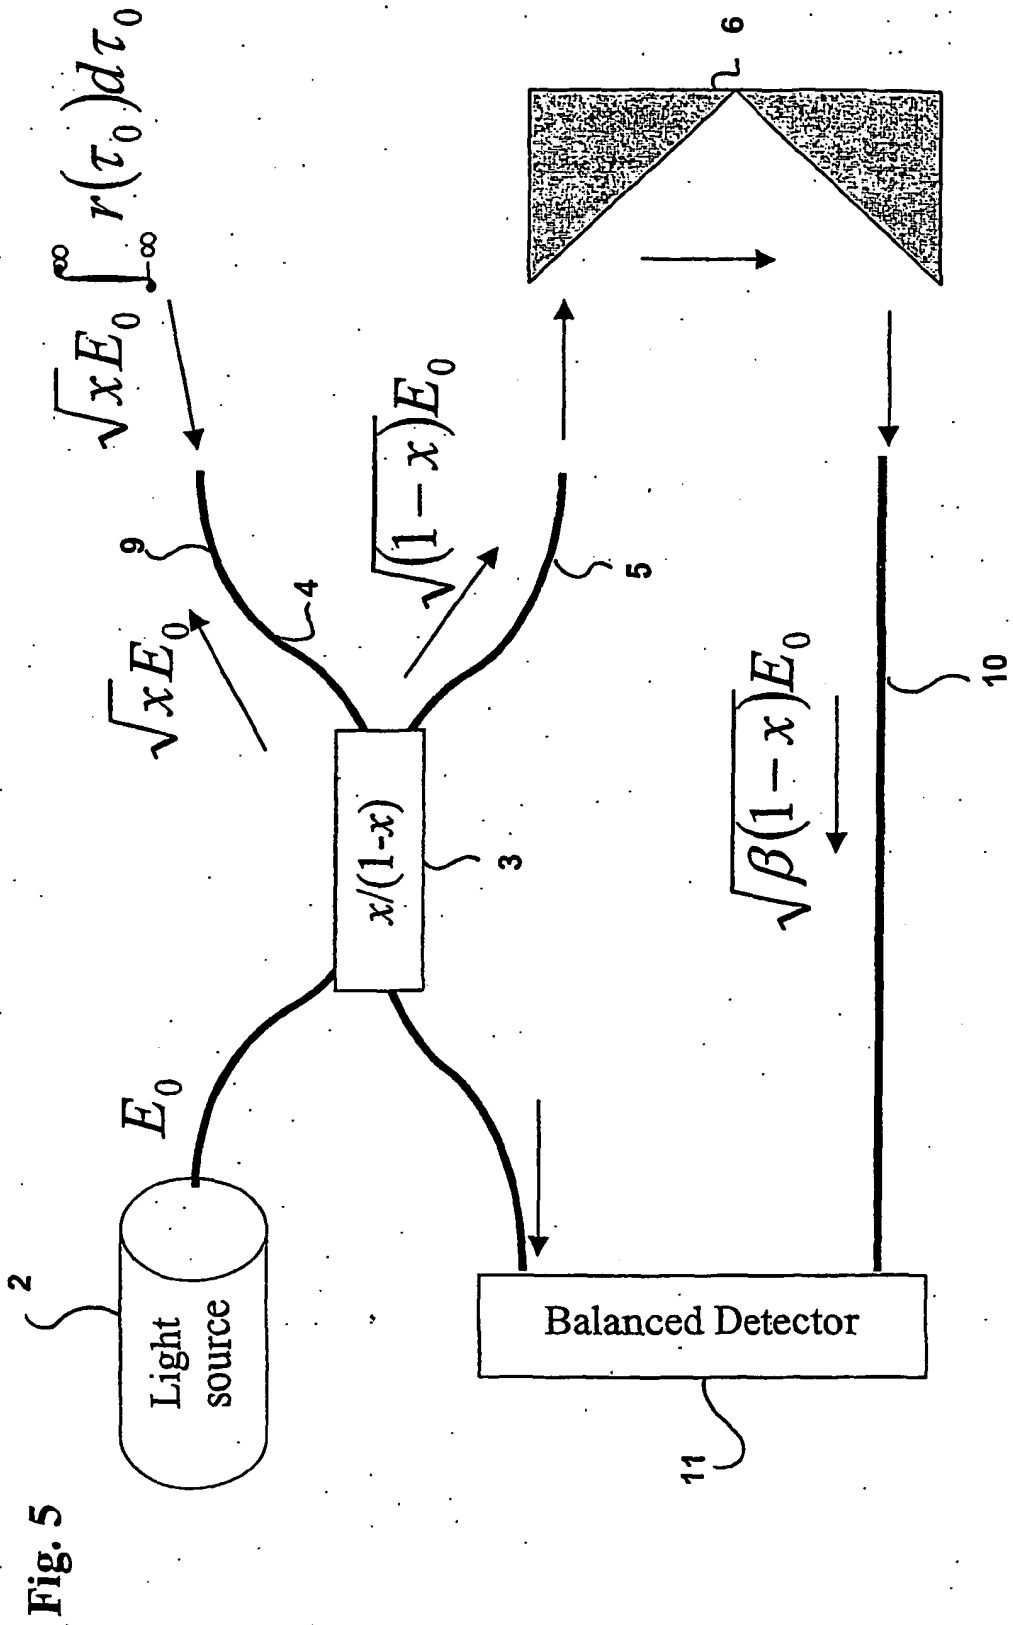


Fig. 3





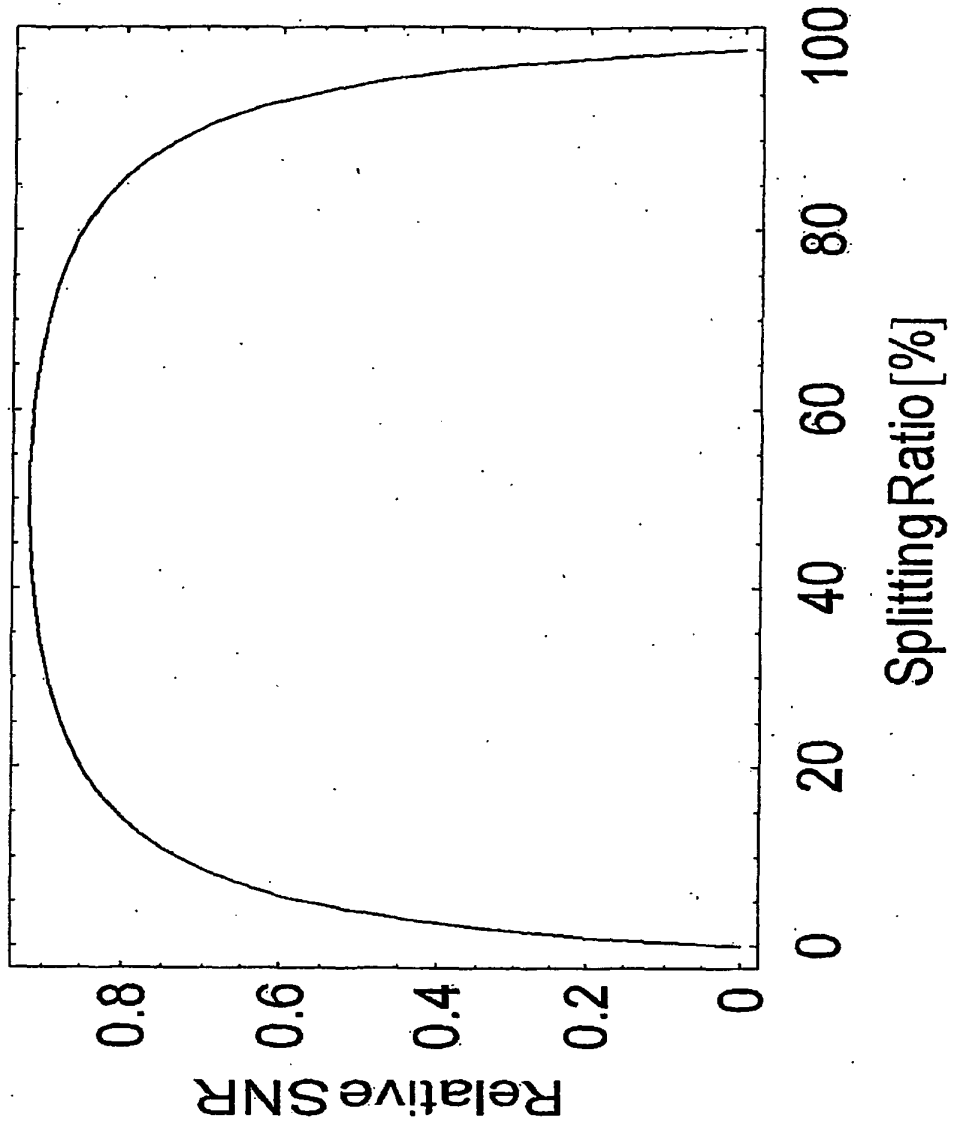


Fig. 6

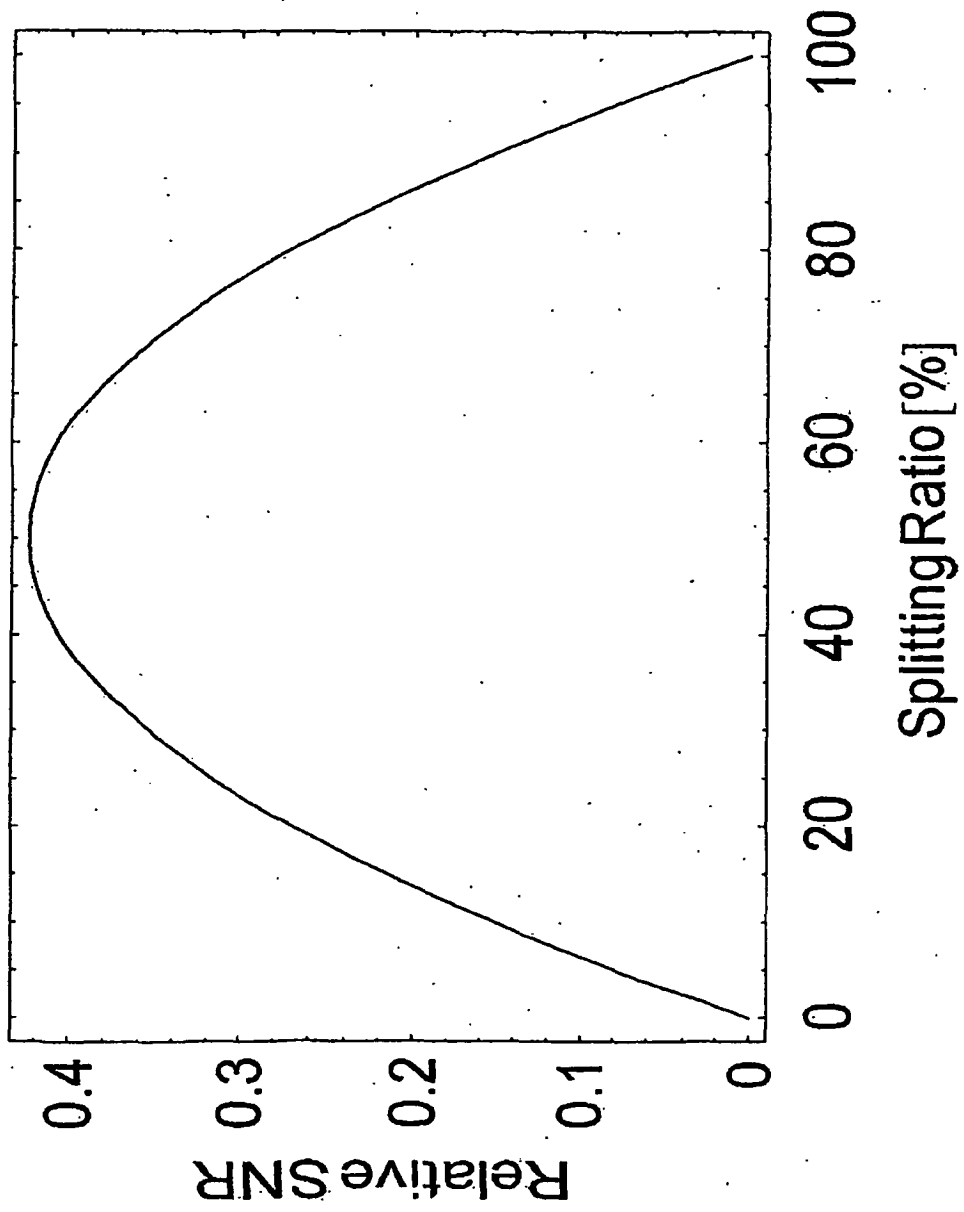
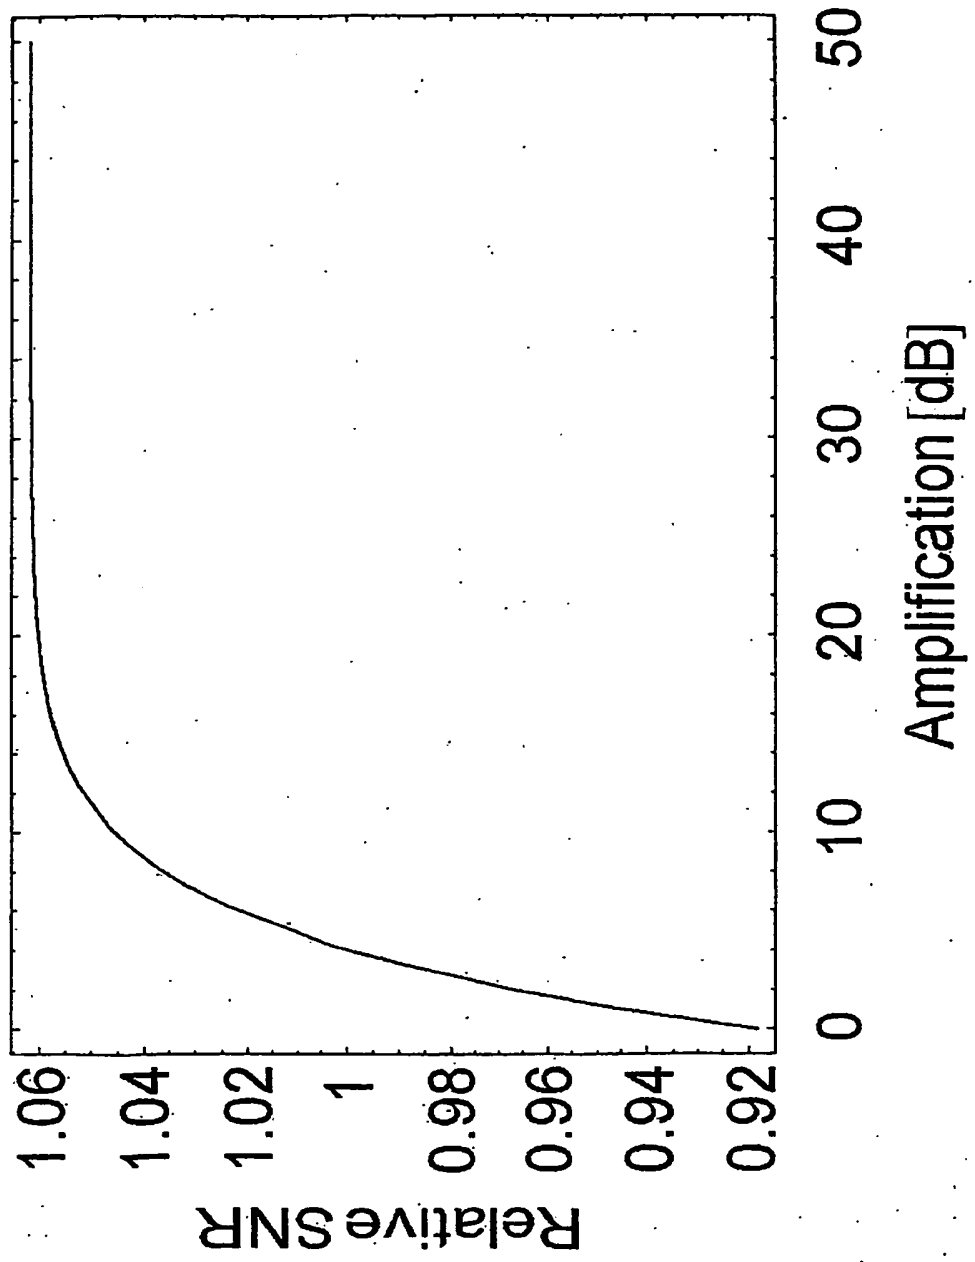


Fig. 7

Fig. 8



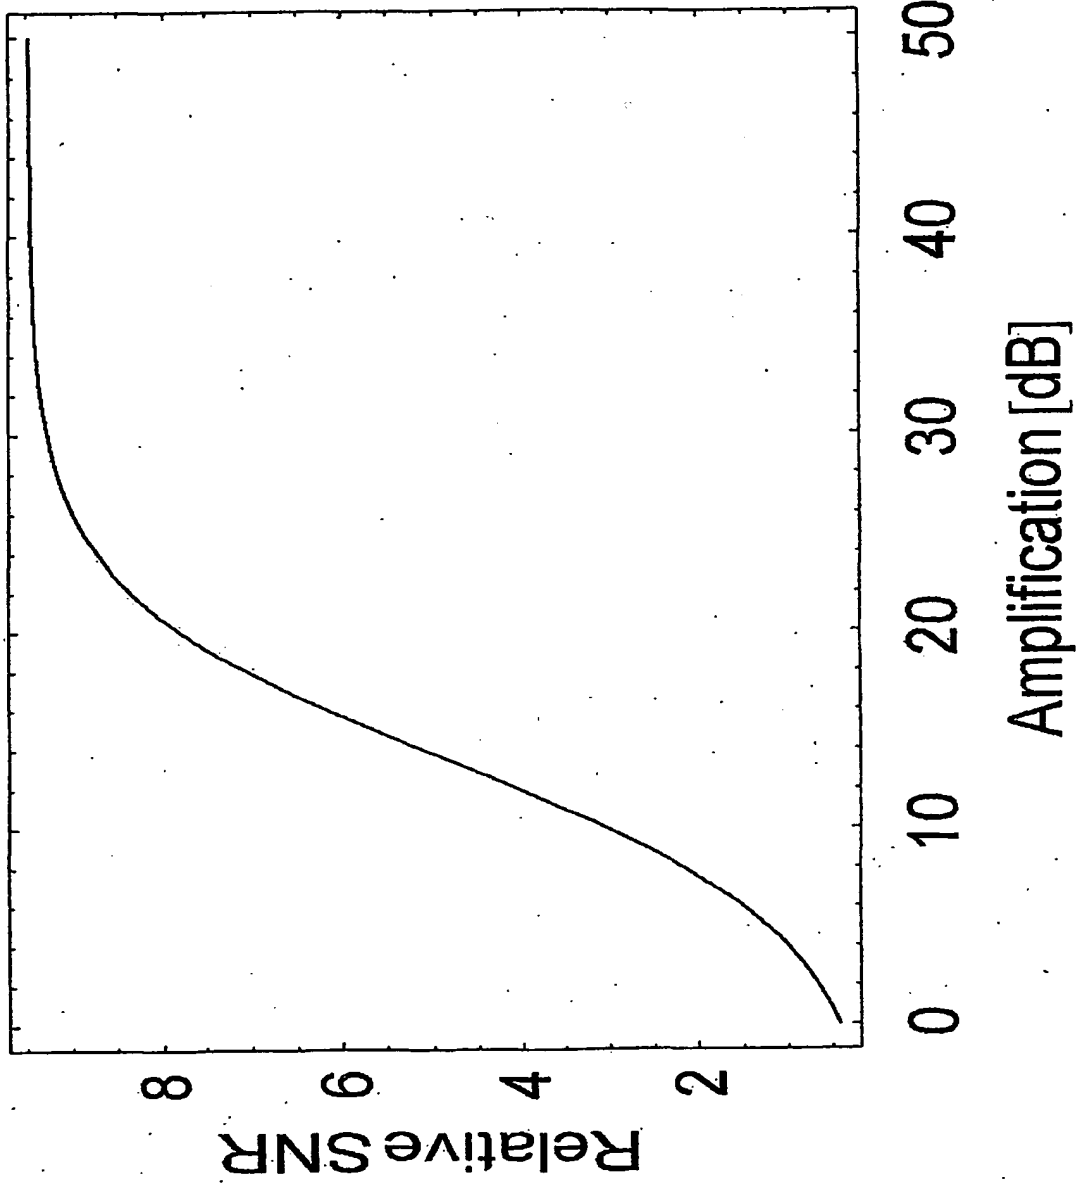


Fig. 9

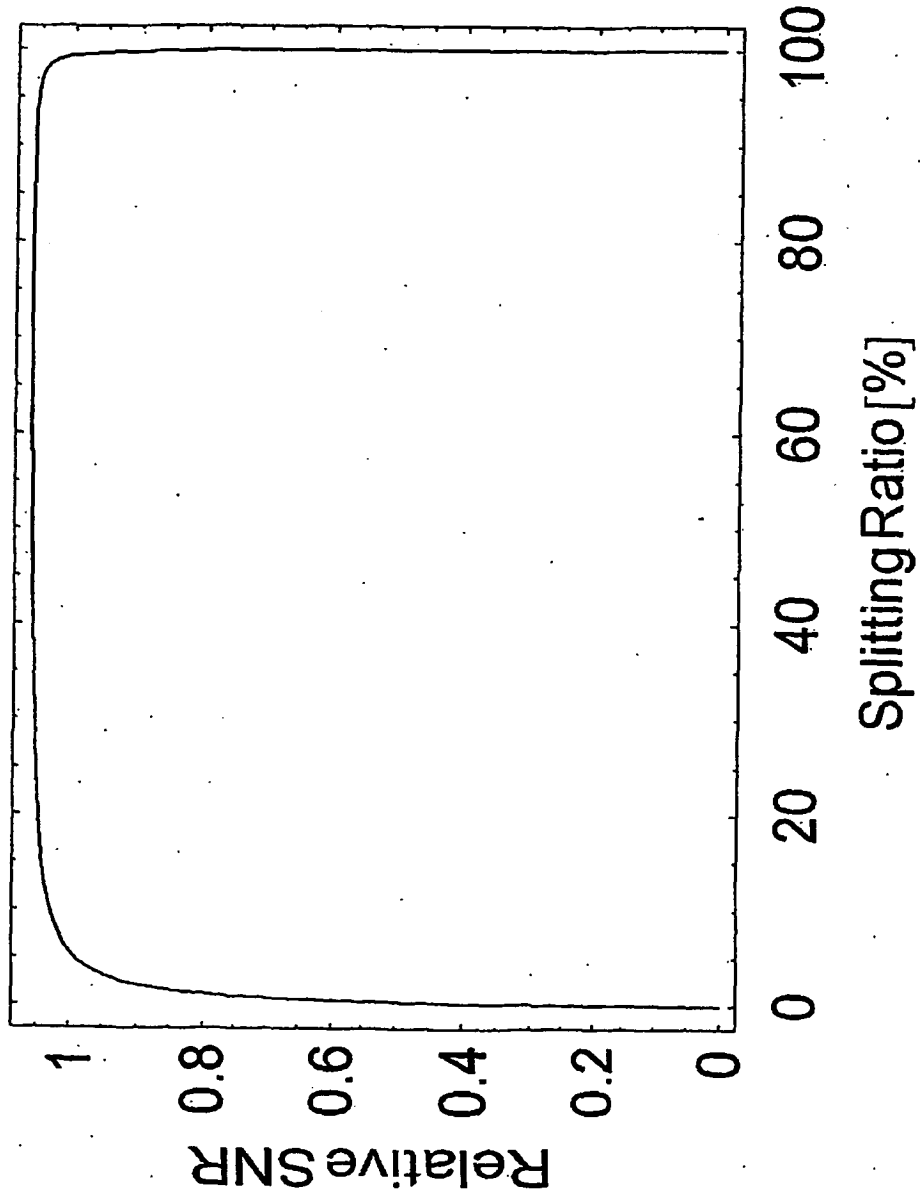


Fig. 10

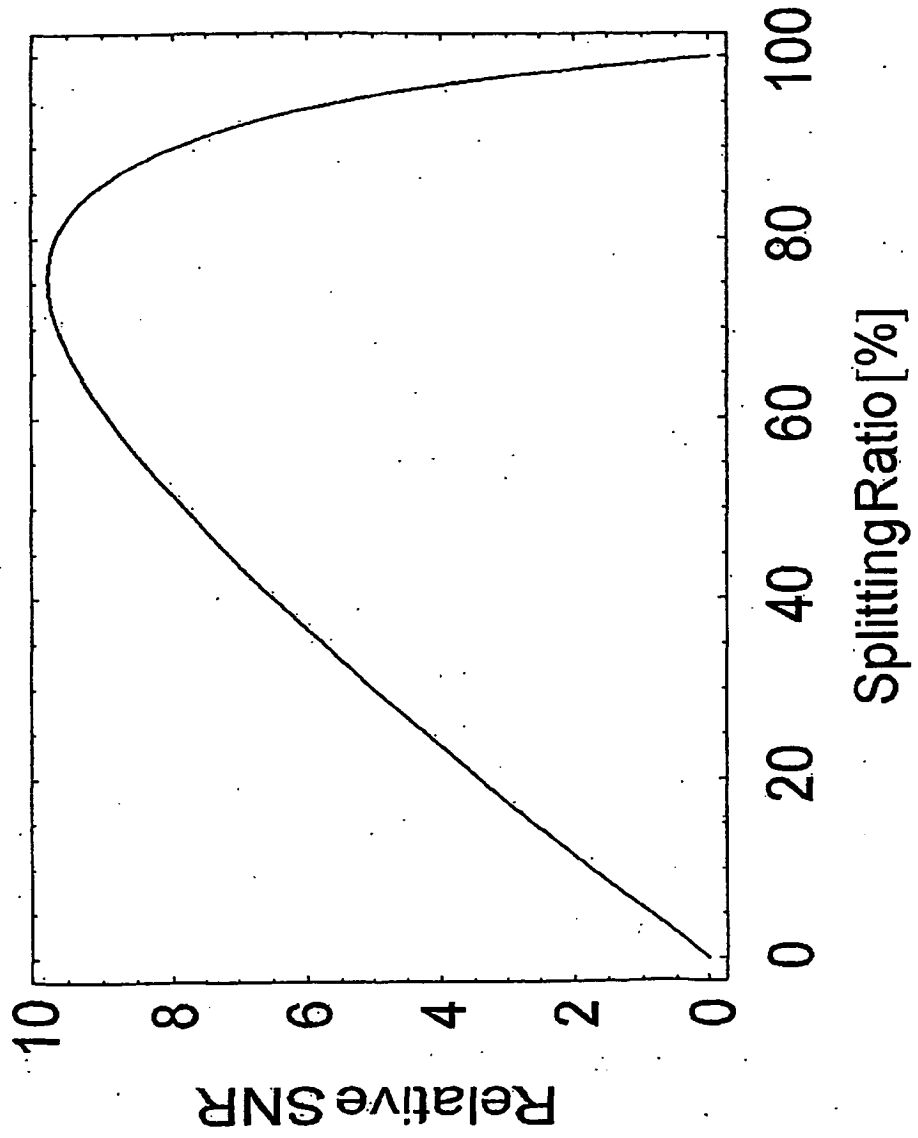


Fig. 11

Fig. 12

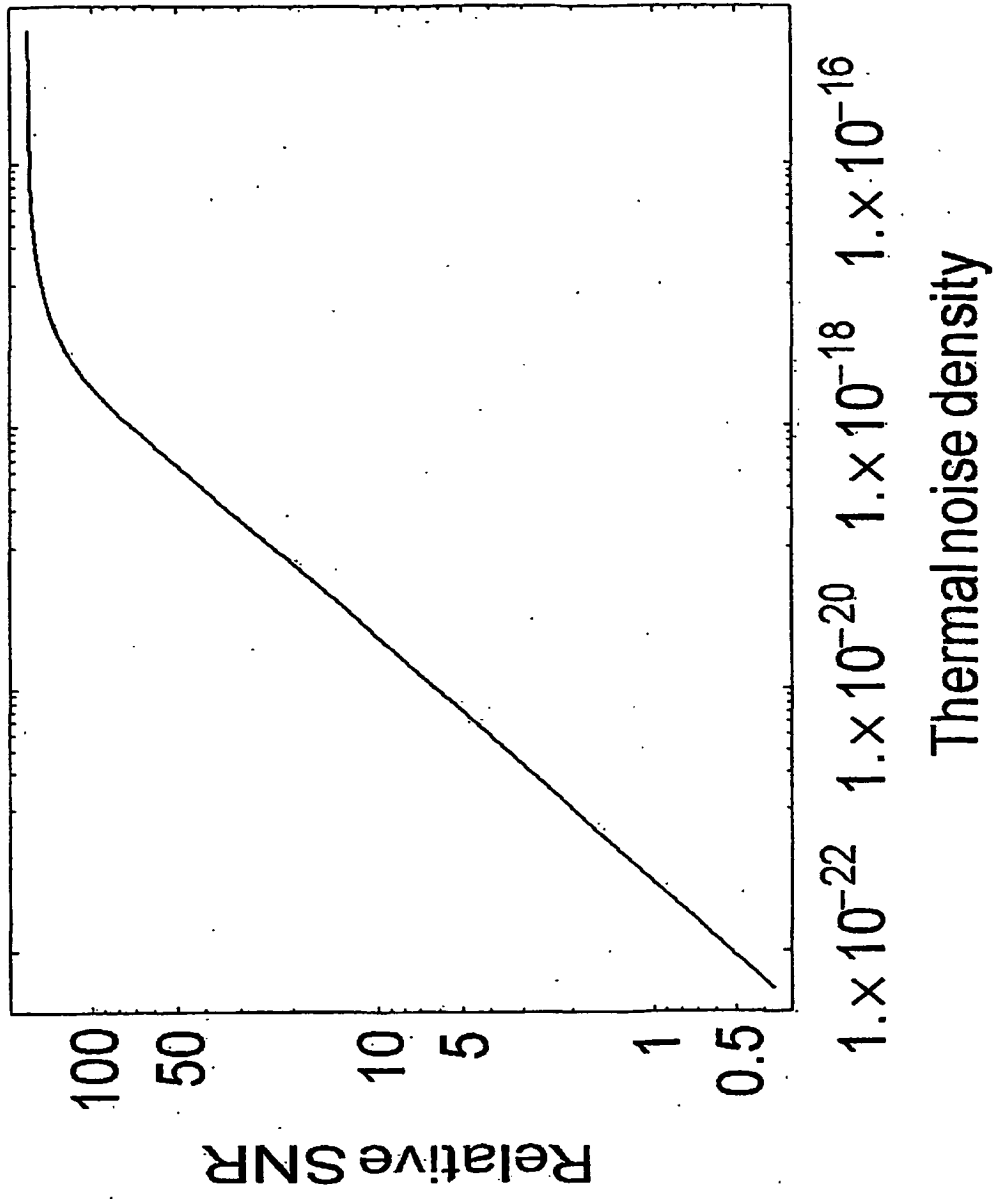
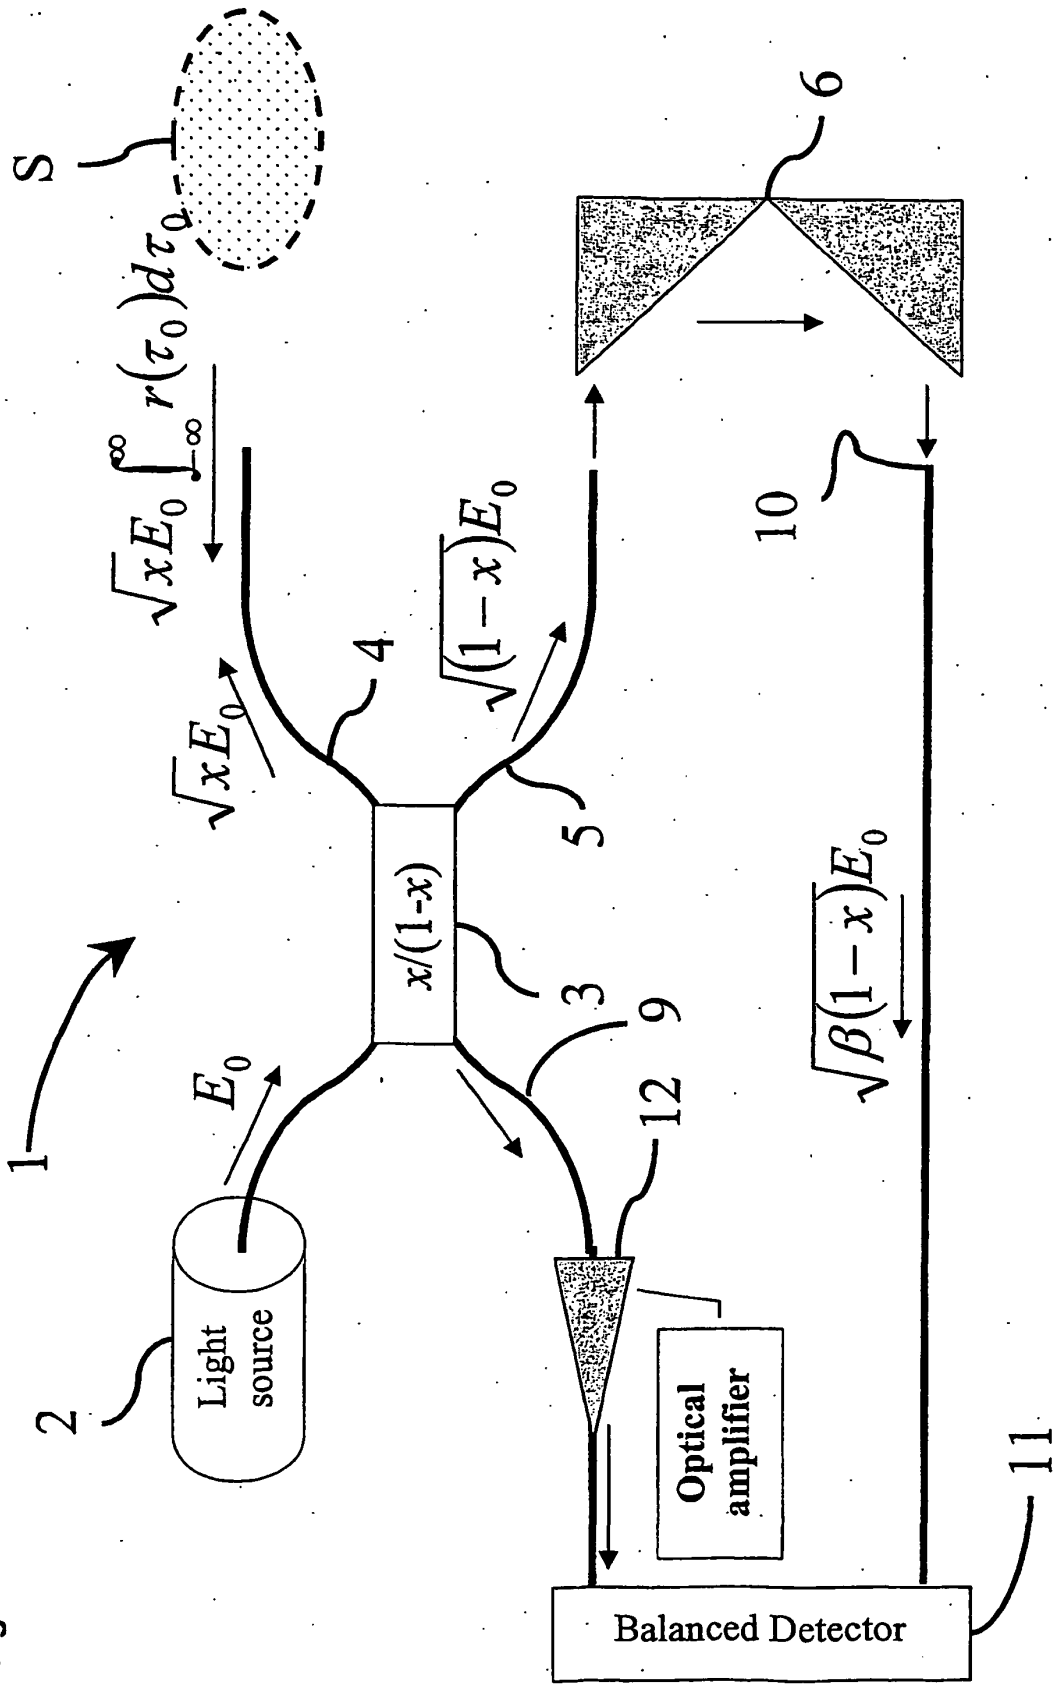


Fig. 13



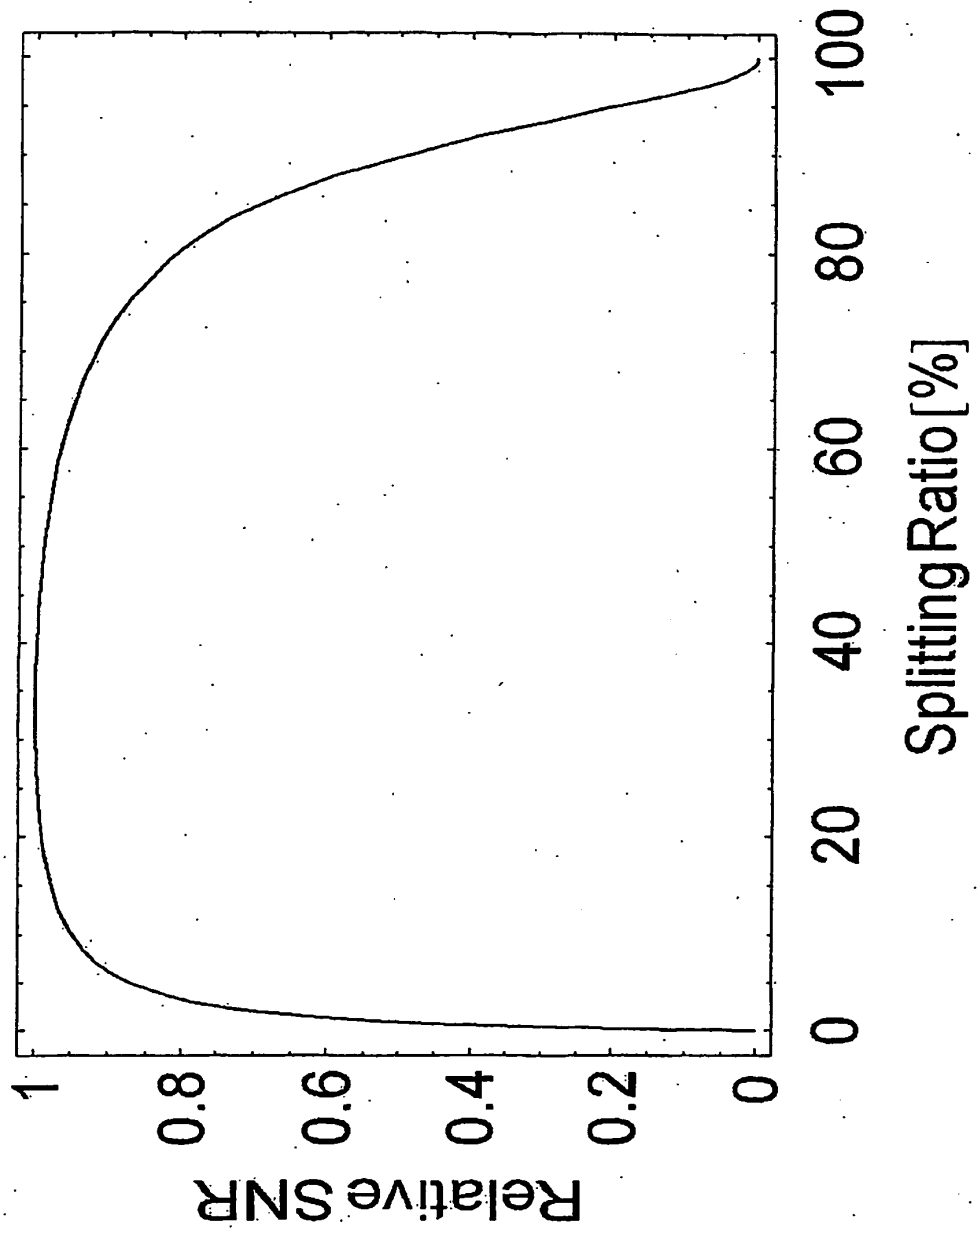


Fig. 14

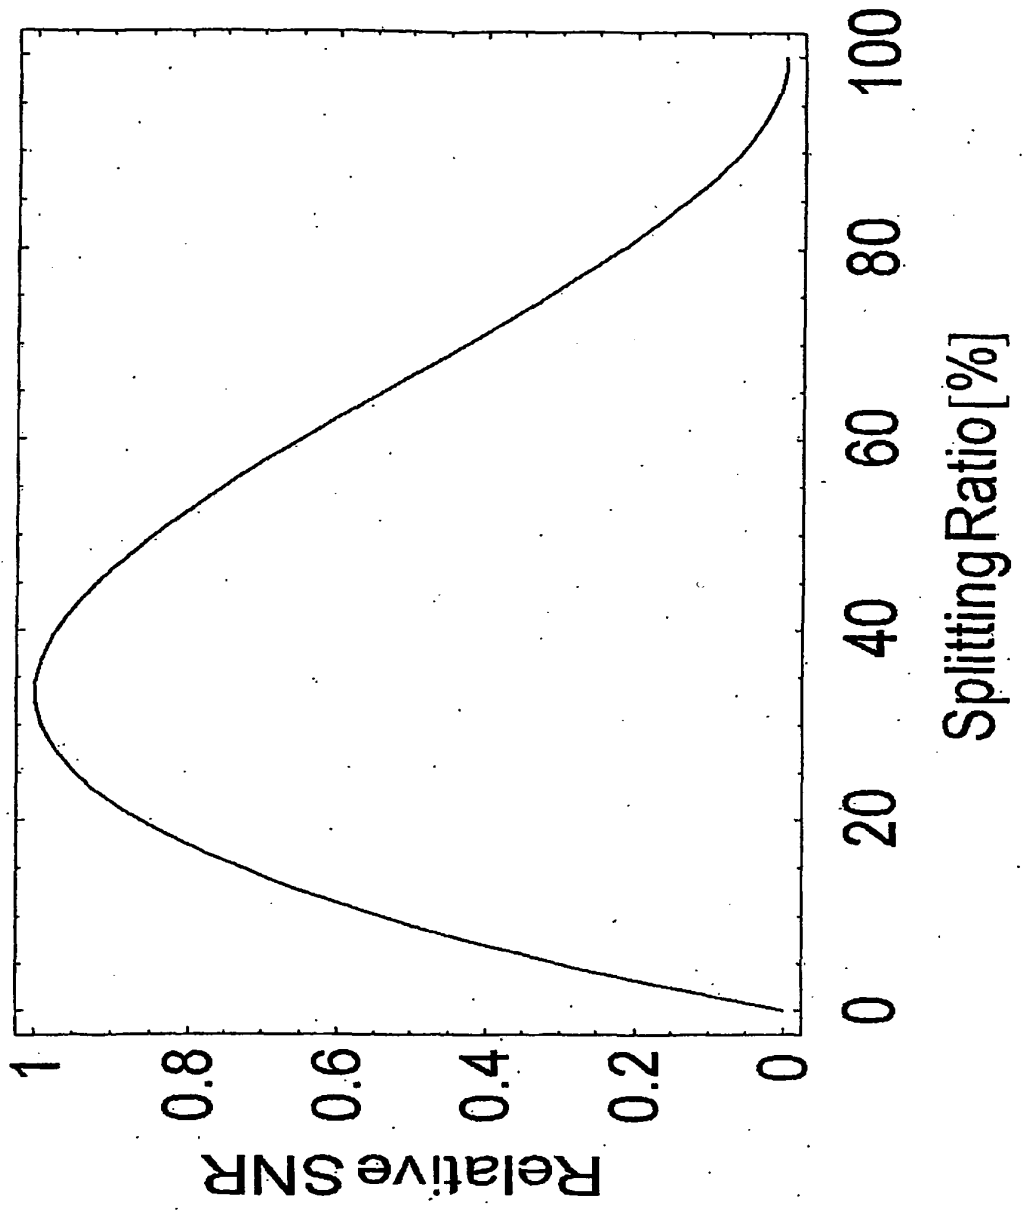


Fig. 15

Fig. 16

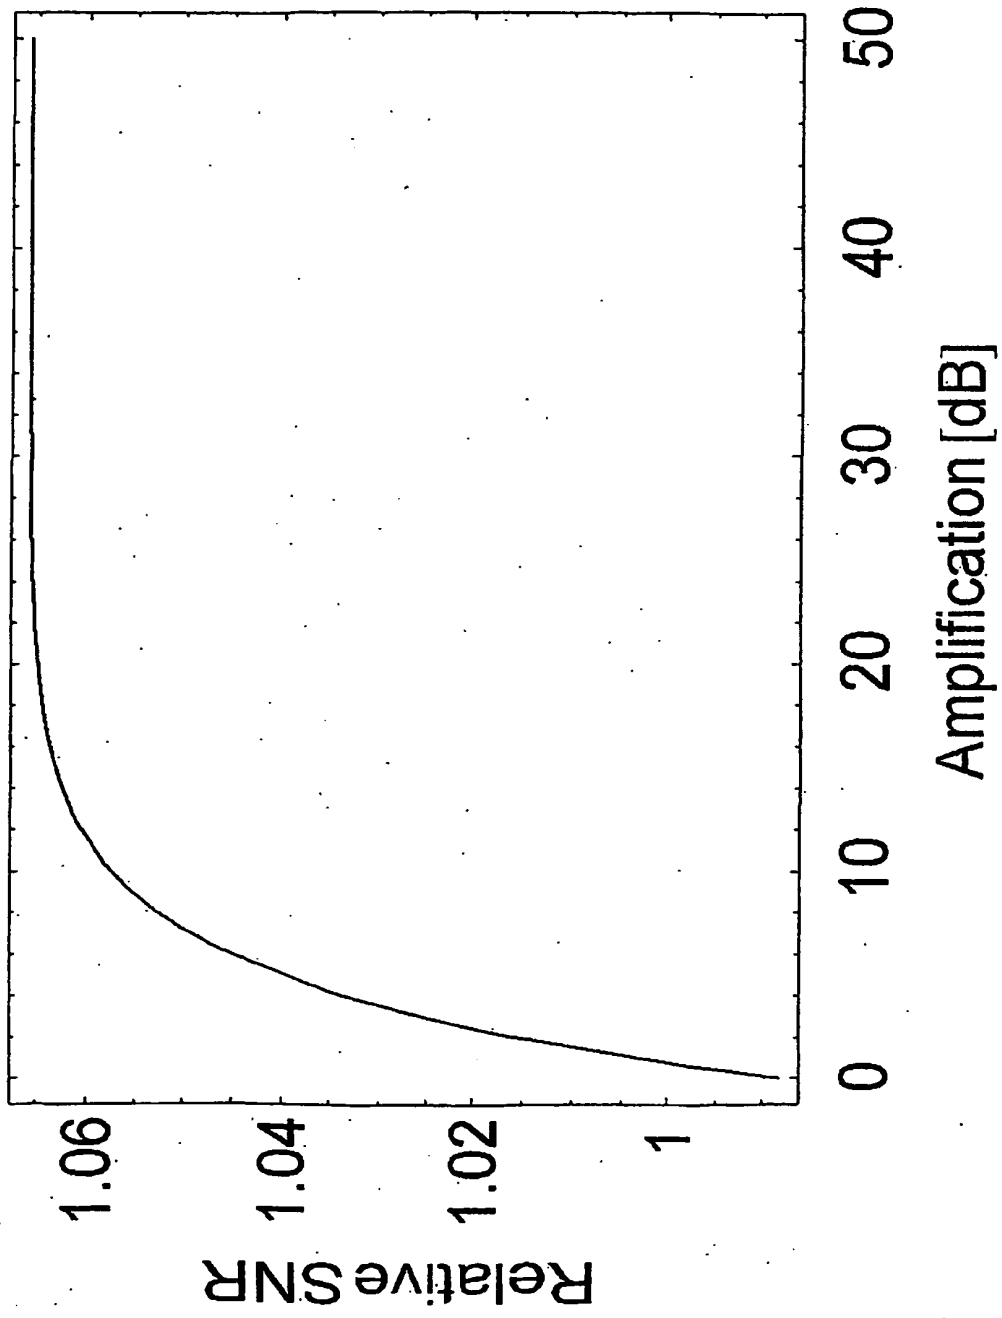


Fig. 17

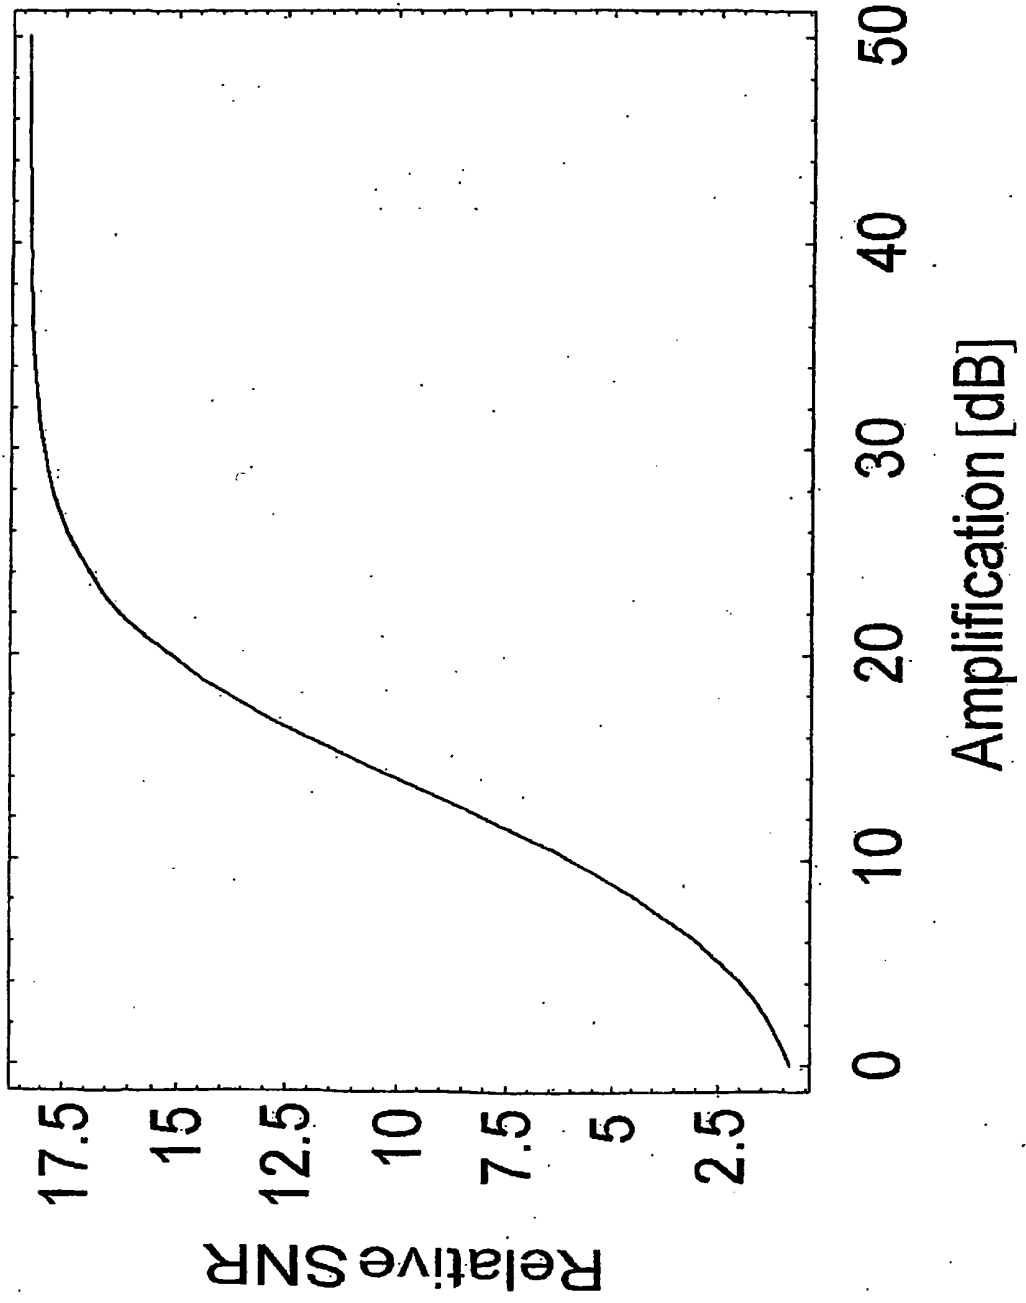
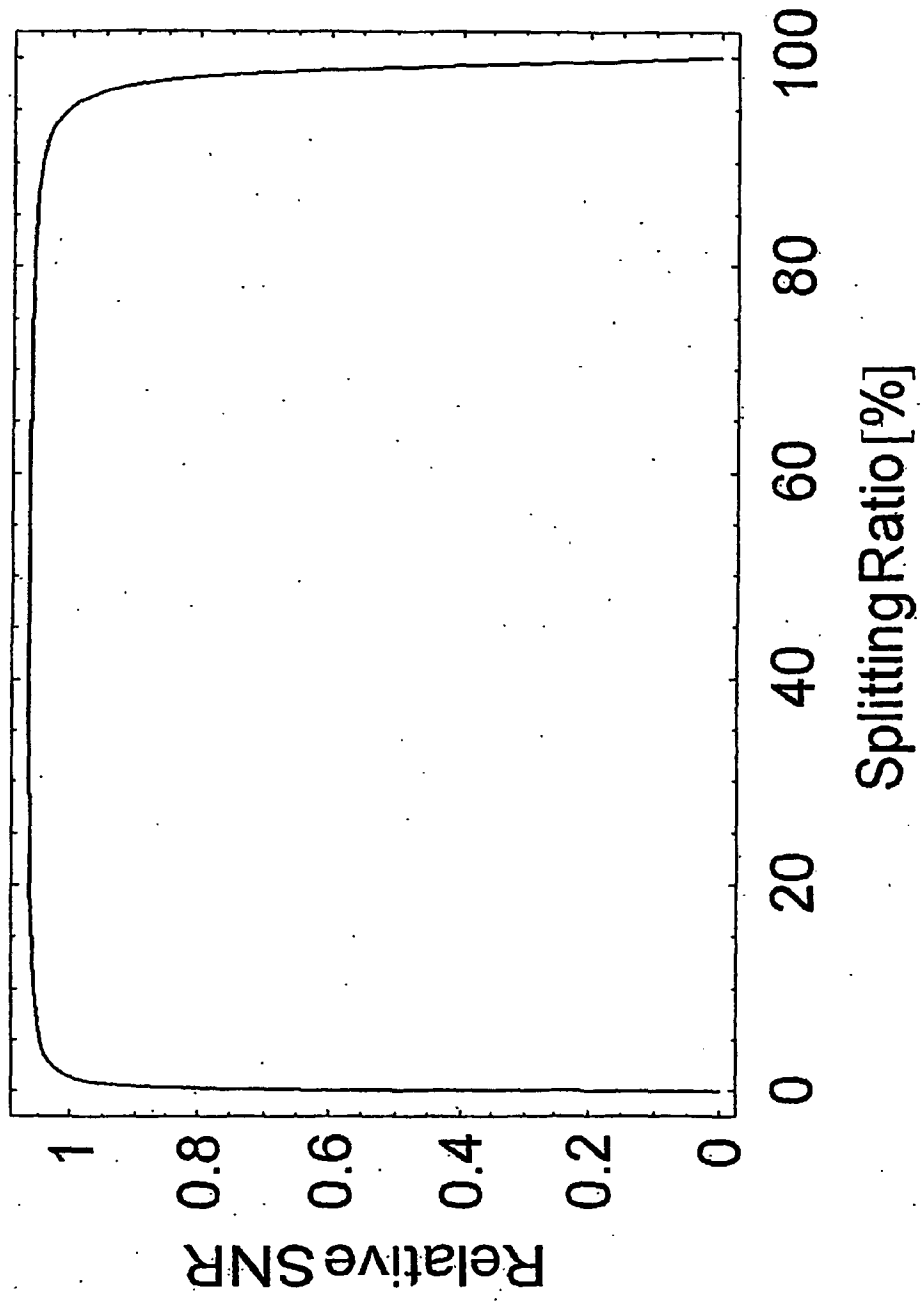


Fig. 18



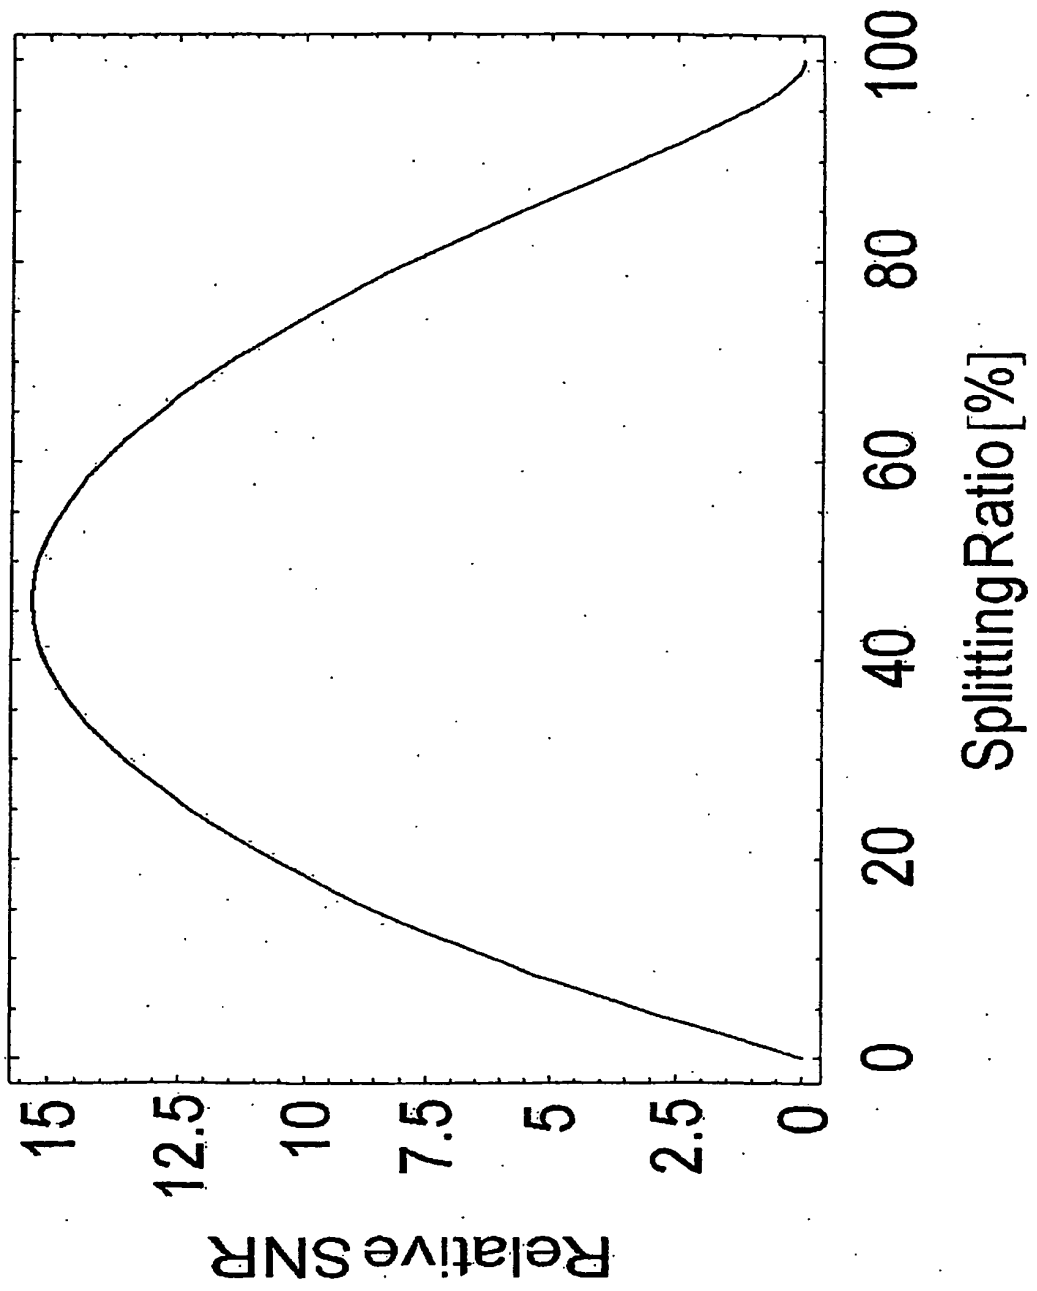
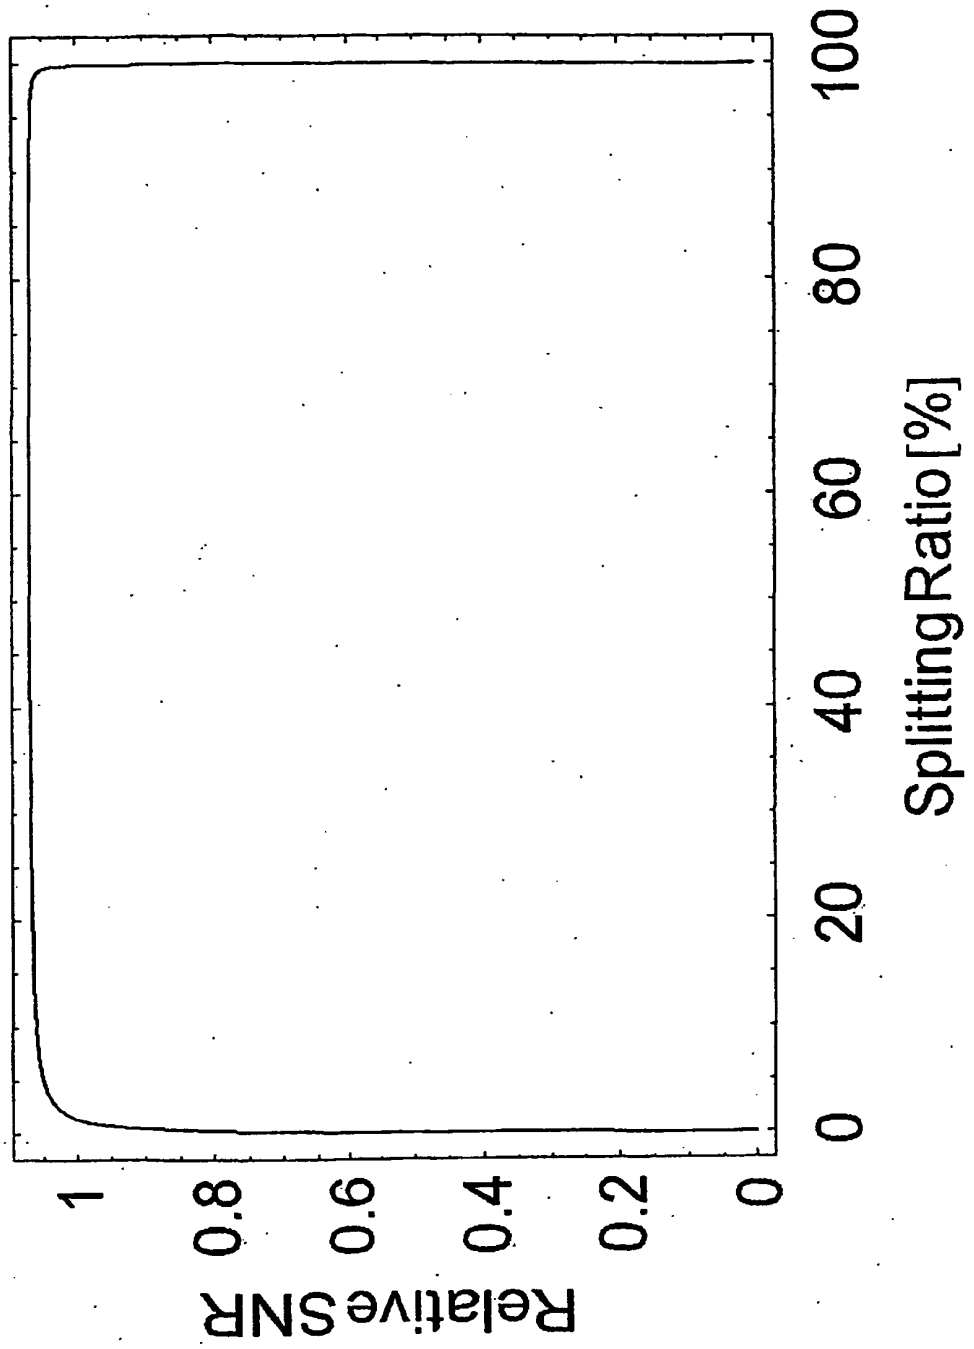


Fig. 19

Fig. 20



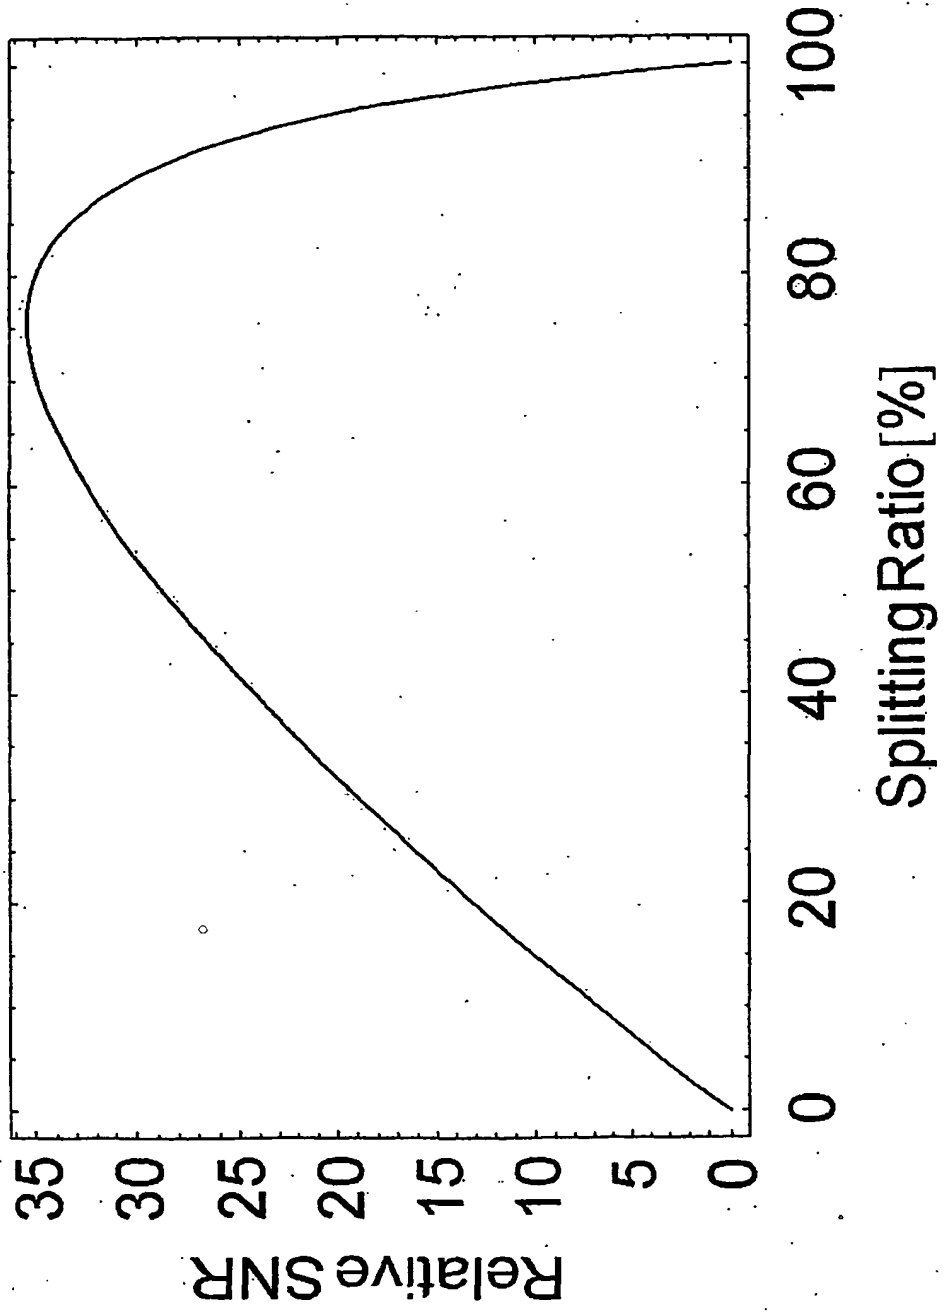


Fig. 21

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5956355 A, Swanson [0003] [0014]
- US 5291267 A [0007] [0007] [0007]
- WO 9946557 A [0008]

Non-patent literature cited in the description

- **Podoleanu, A.G.** Unbalanced versus balanced operation in an optical coherence tomography system. *Applied optics*, vol. 39 (1 [0009])
- **S. Venkatesh ; W. Sorin.** Phase Noise Considerations in Coherent Optical FMCW Reflectometry. *J. of Lightw. Tech.*, 1993, vol. 11 (10 [0041])
- **N.A. Olsson.** Lightwave Systems with optical Amplifiers. *AT&T Bell Laboratories, J. of Lightwave Tech.*, 1983, vol. 7 (7 [0044])
- **N.A. Olsson.** Lightwave Systems with optical Amplifiers. *AT&T Bell Laboratories, J. of Lightwave Tech.*, 1983, vol. 7 (7 [0047])

专利名称(译)	相干光调频连续波反射仪中的光放大		
公开(公告)号	EP1356250B1	公开(公告)日	2009-07-22
申请号	EP2001980204	申请日	2001-10-31
[标]申请(专利权)人(译)	里索国家实验室 丹麦技术大学		
申请(专利权)人(译)	Forskningscenter RISO 丹麦技术大学 (DTU)		
当前申请(专利权)人(译)	马尔克斯TEKNISKE UNIVERSITET		
[标]发明人	ANDERSEN PETER E BJARKLEV ANDERS TYCHO ANDREAS		
发明人	ANDERSEN, PETER, E. BJARKLEV, ANDERS TYCHO, ANDREAS		
IPC分类号	G01B9/02 A61B6/02 G01M11/00 A61B5/00 G01N21/47		
CPC分类号	G01N21/4795 A61B5/0059 A61B5/0066 G01B9/02004 G01B9/02091 G01M11/3127 G01M11/3172		
优先权	200001637 2000-10-31 DK		
其他公开文献	EP1356250A2		
外部链接	Espacenet		

摘要(译)

用于光学相干测量的装置技术领域本发明涉及一种用于光学相干测量的装置，特别是用于光学相干断层扫描的装置，其中用于光学相干测量的装置包括用于提供光信号的波长扫描激光源，以及用于将所述光信号分成样品光的分离装置场和参考光场，其中样品光场指向被测样品，并且从样品反射的光被放大而不相应地放大在参考光场中反射的光。因此，可以将来自第一反射光场的基本上所有光能引导到检测器，并且完全利用第一反射光场的放大。插入样本反射光场的光放大器与光源不同，因此可以独立于放大程度调节光源的效果。特别是当在相干光学FMCW反射计中使用该装置时，必须遵守对样品的功率密度的某些安全规定，以降低对检查中的样品（例如生物组织）造成损害的风险。该装置可用于各种目的，特别是用于获得透明组织和非透明组织的光学活组织检查。

$$\begin{bmatrix} E_1(t) \\ E_2(t) \end{bmatrix} = e^{i\phi} \begin{bmatrix} a & be^{i\phi} \\ be^{i\phi} & a \end{bmatrix} \begin{bmatrix} E_{sam}(t) \\ E_{ref}(t) \end{bmatrix},$$

(1)