

(19)



(11)

**EP 2 938 249 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**23.10.2019 Bulletin 2019/43**

(51) Int Cl.:  
**A61B 5/00 (2006.01)**

(21) Application number: **13868464.2**

(86) International application number:  
**PCT/US2013/078103**

(22) Date of filing: **27.12.2013**

(87) International publication number:  
**WO 2014/106117 (03.07.2014 Gazette 2014/27)**

(54) **ANALYTE PERMEABLE MEMBRANE SYSTEMS FOR OXIDATIVE AND OPTICAL STABILITY**  
 ANALYTDURCHLÄSSIGE MEMBRANSYSTEME FÜR OXIDATIVE UND OPTISCHE STABILITÄT  
 SYSTÈMES DE MEMBRANE PERMÉABLES À DES ANALYTES POUR UNE STABILITÉ À L'OXYDATION ET OPTIQUE

(84) Designated Contracting States:  
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR**

- **HUFFSTETLER, Philip**  
Germantown, MD 20876 (US)
- **WHITEHURST, Todd**  
Germantown, MD 20876 (US)

(30) Priority: **28.12.2012 US 201261746790 P**  
**18.07.2013 US 201361847881 P**

(74) Representative: **Elkington and Fife LLP**  
**Prospect House**  
**8 Pembroke Road**  
**Sevenoaks, Kent TN13 1XR (GB)**

(43) Date of publication of application:  
**04.11.2015 Bulletin 2015/45**

(73) Proprietor: **Senseonics, Incorporated**  
**Germantown, MD 20876-7005 (US)**

(56) References cited:  
**WO-A1-2010/119916 WO-A1-2010/123972**  
**WO-A1-2014/043204 US-A1- 2005 031 689**  
**US-A1- 2007 235 331 US-A1- 2012 238 842**  
**US-B1- 6 330 464 US-B1- 6 405 066**  
**US-B2- 8 126 554**

(72) Inventors:  
• **EMKEN, Jeremy**  
**Germantown, MD 20876 (US)**

**EP 2 938 249 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

### CROSS-REFERENCE TO RELATED APPLICATIONS

**[0001]** The present application claims the benefit of priority to U.S. Provisional Application Serial No. 61/746,790, filed on December 28, 2012, and U.S. Provisional Application Serial No. 61/847,881, filed on July 18, 2013.

### BACKGROUND

#### Field of Invention

**[0002]** The present invention relates generally to sensors for implantation or insertion within a living animal and measurement of a concentration of an analyte in a medium within the living animal. Specifically, the present invention relates to sensors having a membrane over an indicator element on the surface of the sensor body.

#### Discussion of the Background

**[0003]** A sensor may include an indicator element, such as, for example, indicator molecules embedded or polymerized in or onto a polymer graft (*i.e.*, layer or matrix). For example, in an implantable fluorescence-based glucose sensor, fluorescent indicator molecules may reversibly bind glucose and, when illuminated with excitation light (*e.g.*, light having a wavelength of approximately 378 nm), emit an amount of light (*e.g.*, light in the range of 400 to 500 nm) that depends on whether glucose is bound to the indicator molecule.

**[0004]** If a sensor is implanted in the body of a living animal, the animal's immune system begins to attack the sensor. For instance, if a sensor is implanted in a human, white blood cells attack the sensor as a foreign body, and, in the initial immune system onslaught, neutrophils are the primary white blood cells attacking the sensor. Macrophages and giant cells may further attack the sensor. The defense mechanism of neutrophils and other white blood cells includes the release of highly oxidative substances known as reactive oxygen species (ROS), such as hydrogen peroxide (H<sub>2</sub>O<sub>2</sub>), hydroxyl radical (OH<sup>•</sup>), hypochlorite (OCl<sup>-</sup>), peroxynitrite (OONO<sup>-</sup>), and superoxide (O<sub>2</sub><sup>-</sup>).

**[0005]** ROS, such as hydrogen peroxide, may degrade indicator molecules. For instance, in indicator molecules having a boronate group, hydrogen peroxide may degrade the indicator molecules by oxidizing the boronate group, thus disabling the ability of the indicator molecule to bind glucose.

**[0006]** In addition, if the sensor is an optical sensor, light (*e.g.*, excitation light, fluorescent light emitted by the indicator molecules) from the sensor may pass through the indicator element or other transparent portions of the sensor. If the sensor has been implanted in animal tissue, the light may be reflected by the tissue or may cause the

tissue to fluoresce and return light at a different wavelength. The reflected and fluoresced light from the tissue may return through the indicator element or other transparent part of the sensor and may be received by one or more light detectors (*e.g.*, photodiodes) of the sensor. This results in noise in the signals received by the light detectors.

**[0007]** Moreover, if the animal (*e.g.*, a human patient) is in a brightly lit area, then the light may pass through the patient's skin and be received by the light detectors of the sensor. This could also introduce noise into the signals received by the light detectors. Thus, erroneous sensor readings may occur because light detectors in an implanted sensor may receive additional signals unrelated to the analyte concentration.

**[0008]** US 2012/0238842 A1 and WO 2014/043204 A1 each disclose an implantable device at least partially surrounded by a protective material, structure, and/or a coating that prevents damage to the device from any inflammation reactions, *e.g.* a biocompatible metal, preferably silver, platinum, palladium, gold, manganese, or alloys or oxides thereof that decomposes reactive oxygen species (ROS), such as hydrogen peroxide, and prevents ROS from oxidizing molecules on the surface of or within the device.

**[0009]** US 8,126,554 B2 discloses an implantable medical device with a pulse generator and a chemical sensor in communication with the pulse generator, the chemical sensor configured to detect an ion concentration in a bodily fluid.

**[0010]** WO 2010/123972 A1 discloses an implantable device encapsulated by a protective coating that prevents damage to the device from any inflammation reactions and designed to persist for a set period of time.

**[0011]** There is presently a need in the art for improvements in optical sensor isolation and reducing indicator element degradation.

### SUMMARY

**[0012]** The present invention overcomes the disadvantages of prior systems by providing, among other advantages, improved optical isolation and/or reduced indicator element degradation while still allowing an analyte of interest to reach the indicator element.

**[0013]** The present invention provides a sensor that may be used for *in vivo* detection of the presence, amount, and/or concentration of an analyte in a medium within a living animal as defined in claim 1.

**[0014]** The indicator element may include indicator molecules.

**[0015]** In some embodiments, the membrane may have pores configured to substantially prevent white blood cells from passing through the membrane but to permit the analyte to pass through the membrane. The membrane is opaque. The membrane catalyzes degradation of ROS, such as hydrogen peroxide, and reduce deterioration of the indicator element. The membrane

may comprise a hydrophilic or hydrophobic membrane material.

**[0016]** In some embodiments, the membrane is a porous, opaque diffusion membrane covering at least a portion of the housing and the graft, and the membrane may be configured to substantially prevent white blood cells from passing through the membrane and permit an analyte of interest to pass through the membrane to the indicator element and to substantially prevent transmission of light of at least a specified wavelength or range of wavelengths through the membrane. The diffusion membrane may comprise an opaque or light absorbing colorant.

**[0017]** Further variations encompassed within the systems and methods are described in the detailed description of the invention below.

### BRIEF DESCRIPTION OF THE DRAWINGS

**[0018]** The accompanying drawings, which are incorporated herein and form part of the specification, illustrate various, non-limiting embodiments of the present invention. In the drawings, like reference numbers indicate identical or functionally similar elements.

FIG. 1 is a schematic view of a sensor system, which includes an implantable sensor and a sensor reader, embodying aspects of the present invention.

FIG. 2 illustrates a perspective view of a sensor embodying aspects of the present invention.

FIG. 3 illustrates an exploded view of a sensor embodying aspects of the present invention.

FIGS. 4 and 5 illustrate perspective views of sensor components within the sensor body/shell/capsule of a sensor embodying aspects of the present invention.

FIG. 6 illustrates a side view of a sensor embodying aspects of the present invention.

FIG. 7 illustrates a cross-sectional end view of a sensor embodying aspects of the present invention.

FIG. 8 illustrates a cross-sectional side view of a sensor in operation in accordance with an embodiment of the present invention.

FIGS. 9 and 10 illustrate a side view of a sensor, without and with a membrane over the indicator element, respectively, in accordance with an embodiment of the present invention.

FIGS. 11 and 12 illustrate a cross-sectional view of a sensor in accordance with an embodiment of the present invention.

FIG. 13 is a perspective view of an alternate embodiment of a sensor embodying aspects of the present invention and comprising an opaque diffusion membrane substantially, or totally, covering the housing of a sensor.

FIG. 14 is a transverse cross-section of the sensor and opaque diffusion membrane along the line XIV-XIV in FIG. 13.

FIG. 15 is an alternate embodiment of a sensor covered with an opaque diffusion membrane.

### DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

**[0019]** This description may use relative spatial and/or orientation terms in describing the position and/or orientation of a component, apparatus, location, feature, or a portion thereof. Unless specifically stated, or otherwise dictated by the context of the description, such terms, including, without limitation, top, bottom, above, below, under, on top of, upper, lower, left of, right of, inside, outside, inner, outer, proximal, distal, in front of, behind, next to, adjacent, between, horizontal, vertical, diagonal, longitudinal, transverse, etc., are used for convenience in referring to such component, apparatus, location, feature, or a portion thereof in the drawings and are not intended to be limiting.

**[0020]** FIG. 1 is a schematic view of a sensor system embodying aspects of the present invention. In one non-limiting embodiment, the system includes a sensor 100 and an external transceiver 101. In the embodiment shown in FIG. 1, the sensor 100 is implanted in a living animal (e.g., a living human). The sensor 100 may be implanted, for example, in a living animal's arm, wrist, leg, abdomen, or other region of the living animal suitable for sensor implantation. For example, as shown in FIG. 1, in one non-limiting embodiment, the sensor 100 may be implanted between the skin 109 and subcutaneous tissues 111. In some embodiments, the sensor 100 may be an optical sensor. In some embodiments, the sensor 100 may be a chemical or biochemical sensor.

**[0021]** A transceiver 101 may be an electronic device that communicates with the sensor 100 to power the sensor 100 and/or obtain analyte (e.g., glucose) readings from the sensor 100. In non-limiting embodiments, the transceiver 101 may be a handheld reader, a wristwatch, waistband, or an armband. In other non-limiting embodiments, the transceiver 101 may be held on a user's body by adhesive (e.g., as part of a biocompatible patch). In one embodiment, positioning (*i.e.*, hovering or swiping/waiving/passing) the transceiver 101 within range over the sensor implant site (*i.e.*, within proximity of the sensor 100) will cause the transceiver 101 to automatically convey a measurement command to the sensor 100 and receive a reading from the sensor 100.

**[0022]** In some embodiments, the transceiver 101 may include an antenna 103, a processor 105 and/or a user interface 107. In one non-limiting embodiment, the user interface 107 may include a liquid crystal display (LCD), but, in other embodiments, different types of displays may be used.

**[0023]** In some embodiments, the antenna 103 may include an inductive element, such as, for example, a coil. The antenna 103 may generate an electromagnetic wave or electrodynamic field (e.g., by using a coil) to induce a current in an inductive element (e.g., inductive

element 114 of FIGS. 3-8) of the sensor 100, which powers the sensor 100. The antenna 103 may also convey data (e.g., commands) to the sensor 100. For example, in a non-limiting embodiment, the antenna 103 may convey data by modulating the electromagnetic wave used to power the sensor 100 (e.g., by modulating the current flowing through a coil of the antenna 103). The modulation in the electromagnetic wave generated by the transceiver 101 may be detected/extracted by the sensor 100. Moreover, the antenna 103 may receive data (e.g., measurement information) from the sensor 100. For example, in a non-limiting embodiment, the antenna 103 may receive data by detecting modulations in the electromagnetic wave generated by the sensor 100, e.g., by detecting modulations in the current flowing through the coil of the antenna 103.

**[0024]** The inductive element of the antenna 103 and the inductive element (e.g., inductive element 114 of FIGS. 3-8) of the sensor 100 may be in any configuration that permits adequate field strength to be achieved when the two inductive elements are brought within adequate physical proximity.

**[0025]** In some embodiments, the processor 105 may calculate one or more analyte concentrations based on the analyte readings received from the sensor 100. In some embodiments, the processor 105 may also generate one or more alerts and/or alarms based on the calculated analyte concentrations (e.g., if the calculated analyte concentration exceeds or falls below one or more thresholds). The calculated analyte concentrations, alerts, and/or alarms may be displayed via the user interface 107.

**[0026]** In some embodiments, the transceiver 101 may communicate (e.g., using a wireless communication standard, such as, for example, Bluetooth) with a remote device (e.g., a smartphone, personal data assistant, handheld device, or laptop computer). The remote device may receive calculated analyte concentrations, alerts, and/or alarms from the transceiver 101 and display them. Display by the remote device may be in addition to, or in the alternative to, display by the user interface 107 of the transceiver 101. For example, in some embodiments, as illustrated in FIG. 1, the transceiver 101 may include a user interface 107, but this is not required. In some alternative embodiments, the transceiver 101 may not have a user interface 107, and calculated analyte concentrations, alerts, and/or alarms may instead be displayed by a remote device.

**[0027]** In some non-limiting embodiments, the transceiver 101 may have some or all of the structure described in U.S. Patent Application No. 13/937,871 with particular reference to FIGS. 1 and 9.

**[0028]** FIGS. 2-8 illustrate a non-limiting embodiment of a sensor 100 embodying aspects of the present invention that may be used in the sensor system illustrated in FIG. 1. In some embodiments, the sensor 100 may be an optical sensor. In one non-limiting embodiment, sensor 100 includes a sensor housing 102 (i.e., body, shell,

or capsule). In exemplary embodiments, sensor housing 102 may be formed from a suitable, optically transmissive polymeric material, such as, for example, acrylic polymers (e.g., polymethylmethacrylate (PMMA)).

**[0029]** In the embodiment illustrated in FIGS. 2-8, the sensor 100 includes indicator molecules 104 (see, e.g., FIGS. 7 and 8). Indicator molecules 104 may be fluorescent indicator molecules or absorption indicator molecules. In some non-limiting embodiments, the indicator molecules 104 may be as described in U.S. Patent No. 6,344,360 or U.S. Patent Application No. 13/937,871. In some non-limiting embodiments, sensor 100 may include an indicator element 106. In some non-limiting embodiments, the indicator element 106 may be a polymer graft (i.e., matrix layer or gel) coated or embedded on at least a portion of the exterior surface of the sensor housing 102, with the indicator molecules 104 distributed throughout the graft. The indicator element 106 may be embedded within the sensor housing 102 and/or cover the entire surface of sensor housing 102 or only one or more portions of the surface of housing 102. Similarly, the indicator molecules 104 may be distributed throughout the entire indicator element 106 or only throughout one or more portions of the indicator element 106.

**[0030]** In the illustrated embodiment, the sensor 100 includes a light source 108, which may be, for example, a light emitting diode (LED) or other light source that emits light over a range of wavelengths that interact with the indicator molecules 104.

**[0031]** In the illustrated embodiment, sensor 100 also includes one or more photodetectors 110 (e.g., photodiodes, phototransistors, photoresistors, or other photosensitive elements) which, in the case of a fluorescence-based sensor, is sensitive to fluorescent light emitted by the indicator molecules 104 such that a signal is generated by the photodetector 110 in response thereto that is indicative of the level of fluorescence of the indicator molecules and, thus, the amount of analyte of interest (e.g., glucose).

**[0032]** As illustrated in FIG. 8, some embodiments of sensor 100 include one or more optical filters 112, such as high pass or band pass filters, that may cover a photosensitive side of the one or more photodetectors 110.

**[0033]** As shown in FIG. 8, in some embodiments, sensor 100 may be wholly self-contained. In other words, the sensor may be constructed in such a way that no electrical leads extend into or out of the sensor housing 102 to supply power to the sensor (e.g., for driving the light source 108) or to convey signals from the sensor 100. Instead, in one embodiment, sensor 100 may be powered by an external power source (e.g., external transceiver 101). For example, the external power source may generate a magnetic field to induce a current in an inductive element 114 (e.g., a coil or other inductive element). Additionally, the sensor 100 may use the inductive element 114 to communicate information to an external sensor reader (e.g., transceiver 101). In some embodiments, the external power source and data reader

may be the same device (e.g., transceiver 101). Although, in FIG. 8, antenna 103 of transceiver 101 is illustrated as a coil that wraps around the sensor 100, this is not required. In some alternative embodiments, the sensor may have a different configuration, such as, for example, those described in U.S. Patent Application No. 13/650,016, with particular reference to FIGS. 2A-2C, or those described in U.S. Patent Application No. 13/937,871.

**[0034]** In some embodiments, sensor 100 may include a semiconductor substrate 116 and circuitry may be fabricated in the semiconductor substrate 116. The circuitry may include analog and/or digital circuitry. In some embodiments, the circuitry may incorporate some or all of the structure described in U.S. Patent Application No. 13/650,016, with particular reference to FIG. 11D. Also, although in some preferred embodiments the circuitry is fabricated in the semiconductor substrate 116, in alternative embodiments, a portion or all of the circuitry may be mounted or otherwise attached to the semiconductor substrate 116. In other words, in alternative embodiments, a portion or all of the circuitry may include discrete circuit elements, an integrated circuit (e.g., an application specific integrated circuit (ASIC)) and/or other electronic components discrete and may be secured to the semiconductor substrate 116, which may provide communication paths between the various secured components.

**[0035]** In some embodiments, the one or more photodetectors 110 may be mounted on the semiconductor substrate 116, but, in some preferred embodiments, the one or more photodetectors 110 may be fabricated in the semiconductor substrate 116. In some embodiments, the light source 108 may be mounted on the semiconductor substrate 116. For example, in a non-limiting embodiment, the light source 108 may be flip-chip mounted on the semiconductor substrate 116. However, in some embodiments, the light source 108 may be fabricated in the semiconductor substrate 116.

**[0036]** In some embodiments, the sensor 100 may include one or more capacitors 118. The one or more capacitors 118 may be, for example, one or more tuning capacitors and/or one or more regulation capacitors. Further, the one or more capacitors 118 may be in addition to one or more capacitors fabricated in the semiconductor substrate 116.

**[0037]** In some embodiments, the sensor 100 may include a reflector 119 (i.e., mirror). Reflector 119 may be attached to the semiconductor substrate 116 at an end thereof (see, FIG. 3). In a non-limiting embodiment, reflector 119 may be attached to the semiconductor substrate 116 so that a face portion 121 of reflector 119 is generally perpendicular to a top side of the semiconductor substrate 116 (i.e., the side of semiconductor substrate 116 on or in which the light source 108 and one or more photodetectors 110 are mounted or fabricated) and faces the light source 108. The face 121 of the reflector 119 may reflect radiation emitted by light source 108. In other words, the reflector 119 may block radiation emitted

by light source 108 from reaching the axial end of the sensor 100.

**[0038]** According to one aspect of the invention, an application for which the sensor 100 was developed (although by no means the only application for which it is suitable) is measuring various biological analytes in the living body of an animal (including a human). For example, sensor 100 may be used to measure glucose, oxygen toxins, pharmaceuticals or other drugs, hormones, and other metabolic analytes in, for example, the human body. The specific composition of the indicator element 106 and the indicator molecules 104 therein may vary depending on the particular analyte the sensor is to be used to detect and/or where the sensor is to be used to detect the analyte (i.e., in interstitial fluid). Preferably, however, indicator element 106 should facilitate exposure of the indicator molecules to the analyte. Also, it is preferred that the optical characteristics of the indicator molecules (e.g., the level of fluorescence of fluorescent indicator molecules) be a function of the concentration of the specific analyte to which the indicator molecules are exposed.

**[0039]** FIGS. 4 and 5 illustrate perspective views of the sensor 100. In FIGS. 4 and 5, the sensor housing 102, filters 112, and the reflector 119, which may be included in some embodiments of the sensor 100, are not illustrated. As shown in the illustrated embodiment, the inductive element 114 may comprise a coil 220. In one embodiment, coil 220 may be a copper coil but other conductive materials, such as, for example, screen printed gold, may alternatively be used. In some embodiments, the coil 220 is formed around a ferrite core 222. Although core 222 is ferrite in some embodiments, in other embodiments, other core materials may alternatively be used. In some embodiments, coil 220 is not formed around a core. Although coil 220 is illustrated as a cylindrical coil in FIGS. 4 and 5, in other embodiments, coil 220 may be a different type of coil, such as, for example, a flat coil.

**[0040]** In some embodiments, coil 220 is formed on ferrite core 222 by printing the coil 220 around the ferrite core 222 such that the major axis of the coil 220 (magnetically) is parallel to the longitudinal axis of the ferrite core 222. A non-limiting example of a coil printed on a ferrite core is described in U.S. Patent No. 7,800,078. In an alternative embodiment, coil 220 may be a wire-wound coil. However, embodiments in which coil 220 is a printed coil as opposed to a wire-wound coil are preferred because each wire-wound coil is slightly different in characteristics due to manufacturing tolerances, and it may be necessary to individually tune each sensor that uses a wire-wound coil to properly match the frequency of operation with the associated antenna. Printed coils, by contrast, may be manufactured using automated techniques that provide a high degree of reproducibility and homogeneity in physical characteristics, as well as reliability, which is important for implant applications, and increases cost-effectiveness in manufacturing.

**[0041]** In some embodiments, a dielectric layer may be printed on top of the coil 220. The dielectric layer may be, in a non-limiting embodiment, a glass based insulator that is screen printed and fired onto the coil 220. In an exemplary embodiment, the one or more capacitors 118 and the semiconductor substrate 116 may be mounted on vias through the dielectric.

**[0042]** In the illustrated embodiment, the one or more photodetectors 110 include a first photodetector 224 and a second photodetector 226. First and second photodetectors 224 and 226 may be mounted on or fabricated in the semiconductor substrate 116.

**[0043]** FIGS. 6 and 7 illustrate side and cross-sectional views, respectively, of the sensor 100 according to one embodiment. As illustrated in FIGS. 6 and 7, the light source 108 may be positioned to emit light that travels within the sensor housing 102 and reaches the indicator molecules 104 of the indicator element 106, and the photodetectors 110, which may be located beneath filters 112, may be positioned to receive light from the indicator molecules 104 of the indicator element 106.

**[0044]** In operation, as shown in FIG. 8, the light source 108 (e.g., an LED) may emit excitation light 329 that travels within the sensor housing 102 and reaches the indicator molecules 104 of the indicator element 106. In a non-limiting embodiment, the excitation light 329 may cause the indicator molecules 104 distributed in indicator element 106 to fluoresce. As the indicator element 106 may be permeable to the analyte (e.g., glucose) in the medium (e.g., blood or interstitial fluid) into which the sensor 100 is implanted, the indicator molecules 104 in the indicator element 106 may interact with the analyte in the medium and, when irradiated by the excitation light 329, may emit indicator fluorescent light 331 indicative of the presence and/or concentration of the analyte in the medium.

**[0045]** The photodetectors 224 and 226 are used to receive light (see FIG. 3). Each photodetector 224 and 226 may be covered by a filter 112 that allows only a certain subset of wavelengths of light to pass through (see FIG. 3). The filters 112 may be thin film (e.g., dichroic) filters deposited on glass, and the filters 112 may pass only a narrow band of wavelengths and otherwise reflect the received light. The filters 112 may be identical (e.g., both filters 112 may allow signal light to pass) or different (e.g., one filter 112 may allow signal light to pass, and the other filter 112 may allow reference light to pass).

**[0046]** Photodetector 226 may be a reference photodetector, and the filter 112 may pass light at the same wavelength as the wavelength of the excitation light 329 emitted from the light source 108 (e.g., 378 nm). Photodetector 224 may be a signal photodetector that detects the amount of fluoresced light 331 that is emitted from the indicator molecules 104 in the indicator element 106. In some non-limiting embodiments, the signal filter 112 (i.e., the filter 112 covering photodetector 224) may pass light in the range of about 400 nm to 500 nm. Higher analyte levels may correspond to a greater amount of

fluorescence of the molecules 104 in the indicator element 106, and therefore, a greater amount of photons striking the signal photodetector 224.

**[0047]** Embodiments of the present invention may include one or more of several possible solutions to the light-blocking and/or indicator element deterioration problems described above.

**[0048]** FIGS. 9 and 10 illustrate a sensor 100 having a membrane 808 in accordance with an embodiment of the present invention. FIG. 9 shows the sensor 100 without the membrane 808, and FIG. 10 shows the sensor 100 with the membrane 808. In some non-limiting embodiments, the sensor 100 may have a sensor housing/shell 102 and an indicator element 106 embedded within and/or covering at least a portion of the housing 102. The indicator element 106 may include indicator molecules 104.

**[0049]** In regard to indicator element deterioration, as explained above, white blood cells, including neutrophils, may attack an implanted sensor 100. The neutrophils release, *inter alia*, hydrogen peroxide, which may degrade indicator molecules 104 (e.g., by oxidizing a boronate group of an indicator molecule and disabling the ability of the indicator molecule to bind glucose).

**[0050]** As illustrated in FIGS. 9 and 10, according to the present invention, the indicator element 106 has a thin layer (e.g., 10 nm) on the outside of the indicator element 106. The thin layer protects against indicator molecule degradation. The thin layer may be platinum, and the platinum may be sputtered onto the outside surface of the indicator element 106, which includes the indicator molecules 104. Platinum rapidly catalyzes the conversion of hydrogen peroxide into water and oxygen, which are harmless to the sensor. The rate of this reaction is much faster than the boronate oxidation; thus, the platinum provides some protection against oxidation by reactive oxygen species. Although platinum is the catalyst of the conversion of hydrogen peroxide into water and oxygen in some embodiments, in alternative embodiments, other catalysts of this reaction, such as, for example, palladium or catalase, may be used for the thin layer instead of or in addition to platinum.

**[0051]** As illustrated in FIG. 10, the sensor 100 has a membrane 808 over the indicator element 106 (and over the thin layer/film on the outside of the indicator element 106). The membrane 808 is opaque and, therefore, perform a light-blocking function. In other words, the opaque nature of the membrane may serve the function of effectively blocking extraneous light. In some non-limiting embodiments, only the opaque membrane 808 is used to block light, and, in these embodiments, the sensor 100 does not include an additional layer, such as the layer 810 illustrated in FIG. 11, over the membrane 808. However, in other embodiments, the sensor 100 may include both a membrane 808 that is opaque and an additional layer, such as layer 810 illustrated in FIG. 11, over the membrane 808.

**[0052]** In some non-limiting embodiments, the opaque

membrane 808 may be physically attached over the indicator element 106 after boring an additional, smaller well into the capsule/housing 102. In some non-limiting embodiments, the membrane 808 may be made of a mesh material, such as, for example, as a woven, non-woven, sintered, precipitated, or electrospun nylon. However, this is not required, and, in some alternative embodiments, the membrane 808 may be made of another material, such as, for example, cellulose acetate, polytetrafluoroethylene, polyethylene terephthalate, polypropylene, polyvinyl alcohol, polybutylene terephthalate, polyether ether ketone, polyanhydride, polyamide, polyvinylchloride, polyethersulfone, polyvinylidene difluoride, polycarbonate, or derivatives thereof.

**[0053]** In some embodiments, the membrane 808 may be porous. In other words, the membrane 808 may be structured so that it channels one or more analytes (e.g., glucose) to the indicator element 106. For example, in one non-limiting embodiment, the membrane 808 has small pores (e.g., pores having a pore size of microns or less) that block the passage of white blood cells (e.g., neutrophils), which are between 6 and 12 microns in diameter, from reaching the underlying indicator element 106 to attack it. The small pores, however, would at the same time be large enough to allow the analyte to reach the indicator element 106. In this way, a porous membrane 808 having small pores would increase sensor longevity while not affecting the ability of the sensor 100 to measure the concentration of an analyte. In some embodiments, polymers that control or reduce the body's response to an implant (i.e., the foreign body response) such as polyethylene oxides (PEO), hydroxy acrylates (HEMA), or fluoropolymers could be coated onto any of the membranes 808 (e.g., polytetrafluoroethylene (PTFE) coated onto polyethylene terephthalate (PET) or PEO coated onto nylon).

**[0054]** In some embodiments, the opaque membrane 808 may be made from a material that does not react adversely to the body's defenses. In non-limiting embodiments, the material from which the opaque membrane 808 is made may additionally be both porous (e.g., to allow and analyte, such as glucose, to flow through it) and opaque (e.g., to prevent light from traveling through it). For example, in some embodiments, the membrane material may be a hydrophilic material, such as, for example, nylon or cellulose acetate. In other embodiments, the membrane material may be a hydrophobic material, such as, for example, polyethylene terephthalate or polytetrafluoroethylene.

**[0055]** FIGS. 11 and 12 illustrate a cross-sectional view of a sensor 100 having a membrane 808 in accordance with another embodiment of the present invention. As illustrated in FIGS. 11 and 12, the indicator element 106 of sensor 100 may be covered by a membrane 808, and the sensor 100 may additionally include a thin layer 810, which may also block light. For example, in some embodiments, the layer 810 may prevent excitation light 329 from the light source 108 from escaping the sensor hous-

ing/capsule 102 and prevent undesirable light entering the sensor housing/capsule 102. This undesirable light may be from outside the body and/or may be reflected or fluoresced excitation light being returned from body tissue. Reduction of each type of undesirable light would improve sensor accuracy. In one non-limiting embodiment, the layer 810 may be a mirror. In one non-limiting embodiment, an additional smaller well may be bored into the capsule/housing 102, a membrane 108 may be physically attached over the indicator element 106, and an additional blocking layer 810 may then be attached.

**[0056]** In some embodiments, the membrane 808 may channel an analyte to the indicator element 106, while the layer 810 and/or membrane 808 simultaneously block any errant light.

**[0057]** The membrane 808 may be porous such that it does not physically block the analyte (e.g., glucose) from reaching the indicator element 106. Furthermore, the membrane 808 may have channels small enough to block white blood cells from reaching the indicator element 106, but large enough to allow for the passage of red blood cells and glucose molecules.

**[0058]** In some non-limiting embodiments, the layer 810 may be a material that does not adversely react to the body's defenses. In one non-limiting embodiment, platinum may serve as both the material for the membrane 808 and as the material for the layer 810 because platinum catalyzes hydrogen peroxide species and reduces the deterioration of the indicator element 106 that would otherwise occur, while also blocking extraneous light from over stimulating the indicator element 106. With a platinum membrane 808 in place, hydrogen peroxide, which is produced by a patient's white blood cells through the disproportionation of superoxide ( $O_2^-$ ), would quickly be catalyzed to water and oxygen, which are harmless to the transceiver 101. Thus, a platinum membrane 808 may increase the lifetime of the sensor 100 in the body.

**[0059]** In some alternative embodiments, polymers, such as, for example, nylon, cellulose acetate, polytetrafluoroethylene (PTFE), polyethylene terephthalate (PET), polypropylene (PP), polyvinyl alcohol (PVA), polybutylene terephthalate (PBT), polyether ether ketone (PEEK), polyanhydride, polyamide, polyvinylchloride (PVC), polyethersulfone (PES), polyvinylidene difluoride (PVDF), or polycarbonate may additionally or alternatively be used as the membrane material.

**[0060]** Platinum may not, however, offer complete protection from the *in vivo* oxidation in all cases.

**[0061]** An alternative solution to the light blocking and immune response issues is an opaque diffusion membrane that is configured to both block light from entering or exiting the sensor housing and prevent reactive oxygen species-generating cells from direct tissue contact with the indicator element. A sensor assembly embodying aspects of the invention of this alternative solution is represented by reference number 300 in FIG. 13, which is a perspective view of the sensor assembly. Sensor assembly 300 comprises an implantable sensor, such as

sensor 100 described above, covered or substantially covered by an opaque diffusion membrane 320.

**[0062]** FIG. 14 is a transverse cross-section of the sensor assembly 300. For simplicity of the figure, the internal components of the sensor, such as the light source, filters, antennae, etc., are not shown in FIG. 14. The sensor assembly 300 may comprise a sensor housing 102 which, as described above, may comprise a suitable, optically transmissive polymer material, such as PMMA. Further, as described above, the sensor may include an indicator element 106 coated on or embedded in at least a portion of the exterior surface of the housing 102. The diffusion membrane 320 is disposed over the sensor housing 102 and indicator element 106. It should be noted that the relative thicknesses of the various layers of the sensor assembly 300 shown in FIG. 14 are for clarity of illustration and should not be viewed as limiting.

**[0063]** Preferably, the diffusion membrane 320 is made of a material that does not react adversely to the body's defenses but can also be effectively manipulated to be both porous to allow an analyte (e.g., glucose) to flow through the membrane and opaque to substantially prevent light transmission through the membrane. Suitable materials include, for example, nylon or cellulose acetate because such materials are hydrophilic and can therefore be expected to allow an analyte solution (e.g., a glucose solution) to pass through pores formed in the material. Ready passage of the analyte solution through the membrane pores will facilitate analyte readings with less of a time lag. In addition, porous membranes formed from hydrophobic materials, such as polypropylene, polyethylene terephthalate ("PET"), and polytetrafluoroethylene ("PTFE"), can be made hydrophilic by known surface treatments methods, such as oxygen plasma treatment or chemical treatments to generate hydrophilic surface moieties or by grafting of hydrophilic polymers onto the surface of hydrophobic materials, and thus allow facile diffusion of analyte solutions.

**[0064]** One example of an opaque diffusion membrane embodying aspects of the invention may comprise a porous PET tube loaded with an opaque colorant (e.g., TiO<sub>2</sub>, carbon black). The total amount of colorant added to the PET may be altered such that no measurable light transmission through the diffusion membrane can be detected at the wavelengths of interest. For example, the amount of colorant added to the diffusion membrane material may be increased to a point at which no measurable light is transmitted through the PET (or other membrane material) layer.

**[0065]** Preferably, in one embodiment, the opaque diffusion membrane 320 extends over the entire sensor housing 102 covering substantially any and all light paths into or out of the sensor housing. Preferably, the membrane would include end covers with or without wrapped ends.

**[0066]** A goal is to match light-blocking ability of the membrane 320 with the porosity of the membrane material. Accordingly, the percent open area of the mem-

brane material is preferably sufficiently small (e.g., 6-25%) to block light, but still has sufficient porosity to allow diffusion. In one exemplary embodiment, PET membrane material could be tracked, etched, or laser drilled to add pores. In some non-limiting embodiments, the pores added to the PET membrane material may have a size at the exit that prevents leukocytes (white blood cells), which have a size of approximately 7-80 microns, from passing through the pores. For example, in one non-limiting embodiment, the pores may have a size of approximately 5-7 microns at the exit.

**[0067]** Another important characteristic of the diffusion membrane 320 is to provide maximum distance between the white blood cells and the indicator element 106. Thus, in one embodiment of a diffusion membrane 320 embodying aspects of the invention, the membrane 320 comprises a PET layer having a thickness of approximately 25 to 50 microns to keep immune cells (e.g., white blood cells) at a sufficient distance away from the indicator element 106.

**[0068]** As shown in FIG. 15, another embodiment of a diffusion membrane embodying aspects of the invention is configured to maintain a sufficient distance between white blood cells and the indicator element 106 and employs a combination of materials comprising a relatively thick (e.g., 50-200 micron) porous, torturous path material 330 disposed either beneath or on top of the porous PET (or other material) layer 320 to provide an additional optically isolating layer and to further increase the distance between the immune cell (e.g., white blood cells) and the indicator element 106. A suitable material for the torturous path layer includes nylon. The torturous path material 330 provides a longer path through which ROS produced by the white blood cells would need to travel before reaching analyte-sensing indicator element 106 and thereby increases the degree to which the ROS are diluted and/or degraded. Accordingly, the tortuous path material 330 enhances the white blood cell-blocking capability of such a multi-layer diffusion membrane comprising layers 320 and 330.

**[0069]** In some embodiments, the sensor 100 may include a plurality of membranes. For example, in some non-limiting embodiments, the sensor 100 may include one or more catalytic membranes, one or more porous immune response blocking membranes, and/or one or more light blocking membranes. In one non-limiting embodiment, the sensor 100 may include a catalytic membrane on top of the indicator element 106, a porous immune response blocking membrane on top of the catalytic membrane, and a light blocking membrane on top of the porous immune response blocking membrane. In another non-limiting embodiment, the membranes may be arranged over the indicator element 106 in a different order. In yet another non-limiting embodiment, one or more of the plurality of membranes may have one or more functions (e.g., a sensor 100 may include membrane having catalytic membrane and a membrane that blocks both light and immune response).

**[0070]** Embodiments of the present invention have been fully described above with reference to the drawing figures. Although the invention has been described based upon these preferred embodiments, it would be apparent to those of skill in the art that certain modifications, variations, and alternative constructions could be made to the described embodiments within the scope of the invention. For example, in some embodiments, the sensor 100 is a subcutaneous electrooptical sensor, but this is not required, and, in other embodiments, the sensor 100 may be a transcutaneous and/or electrochemical sensor. Also, circuitry of the sensor 100 and reader 101 may be implemented in hardware, software, or a combination of hardware and software. The software may be implemented as computer executable instructions that, when executed by a processor, cause the processor to perform one or more functions.

### Claims

1. A sensor (100, 300) for in vivo detection of the presence, amount, and/or concentration of an analyte in a medium within a living animal, the sensor comprising:

a sensor housing (102);  
 an indicator element (106) embedded within and/or covering at least a portion of the sensor housing;  
**characterized in that** the sensor further comprises:

a membrane (808, 320) over at least a portion of the indicator element, wherein the membrane is opaque and reduces deterioration of the indicator element by catalyzing degradation of reactive oxygen species (ROS); and  
 a layer between the indicator element and the membrane, wherein the layer is on the outside of the indicator element and reduces deterioration of the indicator element by catalyzing degradation of ROS.

2. The sensor of claim 1, wherein the membrane has pores configured to substantially prevent white blood cells from passing through the membrane but to permit the analyte to pass through the membrane, and the analyte is preferably glucose.
3. The sensor of claim 1, wherein the membrane comprises one or more of:

(i) nylon, cellulose acetate, polytetrafluoroethylene, polyethylene terephthalate, polypropylene, polyvinyl alcohol, polybutylene terephthalate, polyether ether ketone, polyanhydride, polyamide, polyvinylchloride, polyethersulfone, polyethylene terephthalate, polyvinylidene difluoride, polytetrafluoroethylene, nitrocellulose, acrylate, poly(methyl methacrylate), polyacrylate homo- or copolymers, polycarbonate, or combinations or derivatives thereof; and  
 (ii) platinum.

4. The sensor of claim 1, wherein the layer comprises platinum.

5. The sensor of claim 1, wherein the layer is a thin layer sputtered on the outside of the indicator element, and the membrane is preferably wrapped around the indicator element and layer.

6. The sensor of claim 1, further comprising one or more of the following features:

(i) wherein the membrane is wrapped around the indicator element;  
 (ii) wherein the membrane comprises a hydrophilic or hydrophobic membrane material; and  
 (iii) wherein the membrane comprises a mesh material.

7. The sensor of claim 1, further comprising one or more of the following features:

(i) wherein the indicator element is a polymer graft including indicator molecules; and  
 (ii) wherein the sensor housing includes a light source (108) and a light detector (224, 226);  
 (iii) wherein the living animal is a human;  
 (iv) wherein the medium is interstitial fluid;  
 (v) wherein the indicator element comprises a fluorescent indicator element;  
 (vi) wherein the sensor housing comprises an optically transmissive polymer material; and  
 (vii) wherein the sensor housing is a shell or capsule.

8. The sensor of claim 1, wherein membrane is a porous, opaque diffusion membrane covering at least a portion of the housing and the indicator element, wherein the membrane is configured to substantially prevent white blood cells from passing through the membrane and permit an analyte of interest to pass through the membrane to the indicator element and to substantially prevent transmission of light of at least a specified wavelength or range of wavelengths through the membrane.

9. The sensor of claim 8, wherein the diffusion membrane has pores configured to substantially prevent white blood cells from passing through the membrane but to permit glucose to pass through the mem-

brane, the diffusion membrane preferably has a porosity of 3-60%, and pores formed through the diffusion membrane preferably have a size of 0.45-6 microns.

10. The sensor of claim 8, wherein the diffusion membrane comprises a layer of hydrophilic material, and the hydrophilic layer preferably has a thickness of 10 - 200 microns.
11. The sensor of claim 10, wherein the diffusion membrane further comprises a layer of torturous path material disposed over or under the layer of hydrophilic material, the torturous path material preferably comprises nylon, and the torturous path layer preferably has a thickness of 50 - 200 microns.
12. The sensor of claim 8, further comprising one or more of the following features:

- (i) wherein the diffusion membrane comprises a layer of material selected from the group consisting of nylon, cellulose acetate, polytetrafluoroethylene, polyethylene terephthalate, polypropylene, polyvinyl alcohol, polybutylene terephthalate, polyether ether ketone, polyanhydride, polyamide, polyvinylchloride, polyethersulfone, polyethylene terephthalate, polyvinylidene difluoride, polytetrafluoroethylene, nitrocellulose, acrylate, poly(methyl methacrylate), polyacrylate homo- or copolymers, polycarbonate, derivatives thereof, and combinations thereof;
- (ii) wherein the diffusion membrane has a thickness of 10 - 200 microns; and
- (iii) wherein the diffusion membrane comprises an amount of opaque or light absorbing colorant such that light transmission through the diffusion membrane is reduced.

13. The sensor of claim 8, wherein the diffusion membrane comprises an opaque or light absorbing colorant, and, preferably, the opaque or light absorbing colorant comprises TiO<sub>2</sub> or carbon black.
14. The sensor of claim 1, wherein the layer is configured to block (i) external light from reaching the indicator element and (ii) light from the sensor housing that has passed through the indicator element from reaching bodily tissue of the living animal.

#### Patentansprüche

1. Sensor (100, 300) zum in-vivo-Nachweis des Vorhandenseins, der Menge und/oder der Konzentration eines Analyts in einem Medium in einem lebenden Tier, wobei der Sensor folgendes umfasst:

ein Sensorgehäuse (102);  
ein Indikatorelement (106), das in wenigstens einen Teil des Sensorgehäuses eingebettet ist oder diesen bedeckt;

**dadurch gekennzeichnet, dass** der Sensor ferner folgendes umfasst:

eine Membran (808, 320) über wenigstens einem Teil des Indikatorelements, wobei die Membran opak ist und den Abbau des Indikators durch katalysierenden Abbau reaktiver Sauerstoffspezies (ROS) verringert; und  
eine Schicht zwischen dem Indikatorelement und der Membran, wobei sich die Schicht auf der Außenseite des Indikatorelements befindet und den Abbau des Indikators durch katalysierenden Abbau von ROS verringert.

2. Sensor nach Anspruch 1, wobei die Membran Poren aufweist, die so gestaltet sind, dass sie es im Wesentlichen verhindern, dass weiße Blutkörperchen durch die Membran treten, um es zu erlauben, dass der Analyt durch die Membran tritt, und wobei der Analyt vorzugsweise Glukose ist.

3. Sensor nach Anspruch 1, wobei die Membran eines oder mehrerer der folgenden umfasst:

- (i) Nylon, Celluloseacetat, Polytetrafluorethylen, Polyethylenteraphthalat, Polypropylen, Polyvinylalkohol, Polybutylenteraphthalat, Polyetheretherketon, Polyanhydrid, Polyamid, Polyvinylchlorid, Polyethersulfon, Polyethylenteraphthalat, Polyvinylidendifluorid, Polytetrafluorethylen, Nitrocellulose, Acrylat, Polymethylmethacrylat, Polyacrylat-Homopolymere oder -Copolymere, Polycarbonat oder Kombinationen oder Derivate davon; und  
(ii) Platin.

4. Sensor nach Anspruch 1, wobei die Schicht Platin umfasst.

5. Sensor nach Anspruch 1, wobei die Schicht eine dünne Schicht ist, die auf die Außenseite des Indikatorelements aufgesprüht ist, und wobei die Membran vorzugsweise um das Indikatorelement und die Schicht gewickelt ist.

6. Sensor nach Anspruch 1, ferner eines oder mehrere der folgenden Merkmale umfassend:

- (i) wobei die Membran um das Indikatorelement gewickelt ist;  
(ii) wobei die Membran ein hydrophiles oder hydrophobes Membranmaterial umfasst; und

- (iii) wobei die Membran ein Netzmaterial umfasst.
7. Sensor nach Anspruch 1, ferner eines oder mehrere der folgenden Merkmale umfassend:
- (i) wobei das Indikatorelement ein Polymerpropf ist, der Indikatormoleküle aufweist; und
- (ii) wobei das Sensorgehäuse eine Lichtquelle (108) und einen Lichtdetektor (224, 226) aufweist;
- (iii) wobei das lebende Tier ein Mensch ist;
- (iv) wobei das Medium interstitielles Fluid ist;
- (v) wobei das Indikatorelement ein fluoreszierendes Indikatorelement ist;
- (vi) wobei das Sensorgehäuse ein lichtdurchlässiges Polymermaterial ist; und
- (vii) wobei das Sensorgehäuse eine Schale oder Kapsel ist.
8. Sensor nach Anspruch 1, wobei die Membran eine poröse, opake Diffusionsmembran ist, die wenigstens einen Teil des Gehäuses und das Indikatorelement bedeckt, wobei die Membran so gestaltet ist, dass sie es im Wesentlichen verhindert, dass weiße Blutkörperchen durch die Membran treten, und dass sie es erlaubt, dass ein relevanter Analyt durch die Membran zu dem Indikatorelement tritt, und dass sie im Wesentlichen die Übertragung von Licht mit mindestens einer spezifizierten Wellenlänge oder einem Wellenlängenbereich durch die Membran verhindert.
9. Sensor nach Anspruch 8, wobei die Diffusionsmembran Poren aufweist, die so gestaltet sind, dass sie es im Wesentlichen verhindern, dass weiße Blutkörperchen durch die Membran treten, wobei sie es aber erlaubt, dass Glukose durch die Membran tritt, wobei die Diffusionsmembran vorzugsweise eine Porosität von 3 bis 60% aufweist, und wobei die durch die Diffusionsmembran ausgebildeten Poren vorzugsweise eine Größe von 0,45 bis 6 Mikron aufweisen.
10. Sensor nach Anspruch 8, wobei die Diffusionsmembran eine Schicht aus einem hydrophilen Material umfasst, und wobei die hydrophile Schicht vorzugsweise eine Dicke von 10 bis 200 Mikron aufweist.
11. Sensor nach Anspruch 10, wobei die Diffusionsmembran ferner eine Schicht aus einem Material mit gewundenem Pfad umfasst, die sich über oder unter der Schicht aus hydrophilem Material befindet, wobei das Material mit gewundenem Pfad vorzugsweise Nylon umfasst, und wobei die Schicht mit gewundenem Pfad vorzugsweise eine Dicke von 50 bis 200 Mikron aufweist.
12. Sensor nach Anspruch 8, ferner eines oder mehrere der folgenden Merkmale umfassend:
- (i) wobei die Diffusionsmembran eine Schicht aus einem Material umfasst, das ausgewählt ist aus der Gruppe bestehend aus Nylon, Celluloseacetat, Polytetrafluorethylen, Polyethylenterephthalat, Polypropylen, Polyvinylalkohol, Polybutylenterephthalat, Polyetheretherketon, Polyanhydrid, Polyamid, Polyvinylchlorid, Polyethersulfon, Polyethylenterephthalat, Polyvinylidendifluorid, Polytetrafluorethylen, Nitrocellulose, Acrylat, Polymethylmethacrylat, Polyacrylat-Homopolymeren oder-Copolymeren, Polycarbonat, Derivaten davon und Kombinationen davon;
- (ii) wobei die Diffusionsmembran eine Dicke von 10 bis 200 Mikron aufweist; und
- (iii) wobei die Diffusionsmembran eine Menge an opakem oder lichtabsorbierendem Farbstoff umfasst, so dass die Lichtdurchlässigkeit durch die durch die Diffusionsmembran reduziert ist.
13. Sensor nach Anspruch 8, wobei die Diffusionsmembran einen opaken oder lichtabsorbierenden Farbstoff umfasst, und wobei der opake oder lichtabsorbierende Farbstoff TiO<sub>2</sub> oder Carbon Black umfasst.
14. Sensor nach Anspruch 1, wobei die Schicht so gestaltet ist, dass sie folgendes blockiert: (i) dass externes Licht das Indikatorelement erreicht, und (ii) dass Licht von dem Sensorgehäuse, das durch das Indikatorelement getreten ist, Körpergewebe des lebenden Tieres erreicht.

### Revendications

1. Capteur (100, 300) pour la détection in vivo de la présence, de la quantité et/ou de la concentration d'un analyte dans un milieu à l'intérieur d'un animal vivant, le capteur comprenant :

un boîtier de capteur (102) ;

un élément indicateur (106) intégré dans et/ou couvrant au moins une partie du boîtier de capteur ;

**caractérisé en ce que** le capteur comprend en outre :

une membrane (808, 320) sur au moins une partie de l'élément indicateur, la membrane étant opaque et réduisant la détérioration de l'élément indicateur en catalysant la dégradation des dérivés réactifs de l'oxygène (DRO) ; et

une couche entre l'élément indicateur et la membrane, la couche se trouvant sur l'ex-

- térieur de l'élément indicateur et réduisant la détérioration de l'élément indicateur en catalysant la dégradation des DRO.
2. Capteur selon la revendication 1, la membrane ayant des pores conçus pour empêcher sensiblement les leucocytes de passer à travers la membrane mais pour permettre à l'analyte de passer à travers la membrane, et l'analyte étant de préférence du glucose.
3. Capteur selon la revendication 1, la membrane comprenant en outre un ou plusieurs éléments parmi :
- (i) nylon, acétate de cellulose, polytétrafluoroéthylène, poly(téréphtalate d'éthylène), polypropylène, alcool polyvinylique, téréphtalate de polybutylène, polyéther éther cétone, polyanhydride, polyamide, poly(chlorure de vinyle), polyéthersulfone, poly(téréphtalate d'éthylène), difluorure de polyvinylidène, polytétrafluoroéthylène, nitrocellulose, acrylate, poly(méthacrylate de méthyle), homo- ou copolymères de polyacrylate, polycarbonate ou leurs combinaisons ou dérivés ; et
- (ii) platine.
4. Capteur selon la revendication 1, la couche comprenant du platine.
5. Capteur selon la revendication 1, la couche étant une couche mince pulvérisée sur l'extérieur de l'élément indicateur, et la membrane étant de préférence enroulée autour de l'élément indicateur et de la couche.
6. Capteur selon la revendication 1, comprenant en outre une ou plusieurs des caractéristiques suivantes :
- (i) la membrane étant enroulée autour de l'élément indicateur ;
- (ii) la membrane comprenant un matériau de membrane hydrophile ou hydrophobe ; et
- (iii) la membrane comprenant un matériau en maille.
7. Capteur selon la revendication 1, comprenant en outre une ou plusieurs des caractéristiques suivantes :
- (i) l'élément indicateur étant un greffon de polymère comprenant des molécules indicatrices ; et
- (ii) le boîtier de capteur comprenant une source lumineuse (108) et un détecteur de lumière (224, 226) ;
- (iii) l'animal vivant étant un être humain ;
- (iv) le milieu étant un fluide interstitiel ;
- (v) l'élément indicateur comprenant un élément indicateur fluorescent ;
- (vi) le boîtier de capteur comprenant un matériau polymère optiquement transmissif ; et
- (vii) le boîtier de capteur étant une coque ou une capsule.
8. Capteur selon la revendication 1, la membrane étant une membrane de diffusion poreuse et opaque couvrant au moins une partie du boîtier et de l'élément indicateur, la membrane étant conçue pour empêcher sensiblement les leucocytes de passer à travers la membrane et permettre à un analyte d'intérêt de passer à travers la membrane vers l'élément indicateur et pour empêcher sensiblement la transmission de lumière d'au moins une longueur d'onde ou plage de longueurs d'onde spécifiée à travers la membrane.
9. Capteur selon la revendication 8, la membrane de diffusion ayant des pores conçus pour empêcher sensiblement les leucocytes de passer à travers la membrane mais pour permettre au glucose de passer à travers la membrane, la membrane de diffusion ayant de préférence une porosité de 3 à 60 % et les pores formés à travers la membrane de diffusion ayant de préférence une taille de 0,45 à 6 microns.
10. Capteur selon la revendication 8, la membrane de diffusion comprenant une couche de matériau hydrophile, et la couche hydrophile ayant de préférence une épaisseur de 10 à 200 microns.
11. Capteur selon la revendication 10, la membrane de diffusion comprenant en outre une couche de matériau à trajet sinueux disposée sur ou sous la couche de matériau hydrophile, le matériau à trajet sinueux comprenant de préférence du nylon, et la couche à trajet sinueux ayant de préférence une épaisseur de 50 à 200 microns.
12. Capteur selon la revendication 8, comprenant en outre une ou plusieurs des caractéristiques suivantes :
- (i) la membrane de diffusion comprenant une couche de matériau choisi dans le groupe constitué par le nylon, l'acétate de cellulose, le polytétrafluoroéthylène, le poly(téréphtalate d'éthylène), le polypropylène, l'alcool polyvinylique, le téréphtalate de polybutylène, le polyéther éther cétone, le polyanhydride, le polyamide, le poly(chlorure de vinyle), le polyéthersulfone, le poly(téréphtalate d'éthylène), le difluorure de polyvinylidène, le polytétrafluoroéthylène, la nitrocellulose, l'acrylate, le poly(méthacrylate de méthyle), les homo- ou copolymères de polyacryla-

te, le polycarbonate, leurs dérivés et leurs combinaisons ;

(ii) la membrane de diffusion ayant une épaisseur de 10 à 200 microns ; et

(iii) la membrane de diffusion comprenant une quantité de colorant opaque ou absorbant la lumière de sorte que la transmission de lumière à travers la membrane de diffusion soit réduite. 5

**13.** Capteur selon la revendication 8, la membrane de diffusion comprenant un colorant opaque ou absorbant la lumière et, de préférence, le colorant opaque ou absorbant la lumière comprenant du TiO<sub>2</sub> ou du noir de carbone. 10

**14.** Capteur selon la revendication 1, la couche étant conçue pour empêcher (i) la lumière extérieure d'atteindre l'élément indicateur et (ii) la lumière provenant du boîtier de capteur qui est passée à travers l'élément indicateur d'atteindre le tissu corporel de l'animal vivant. 15  
20

25

30

35

40

45

50

55

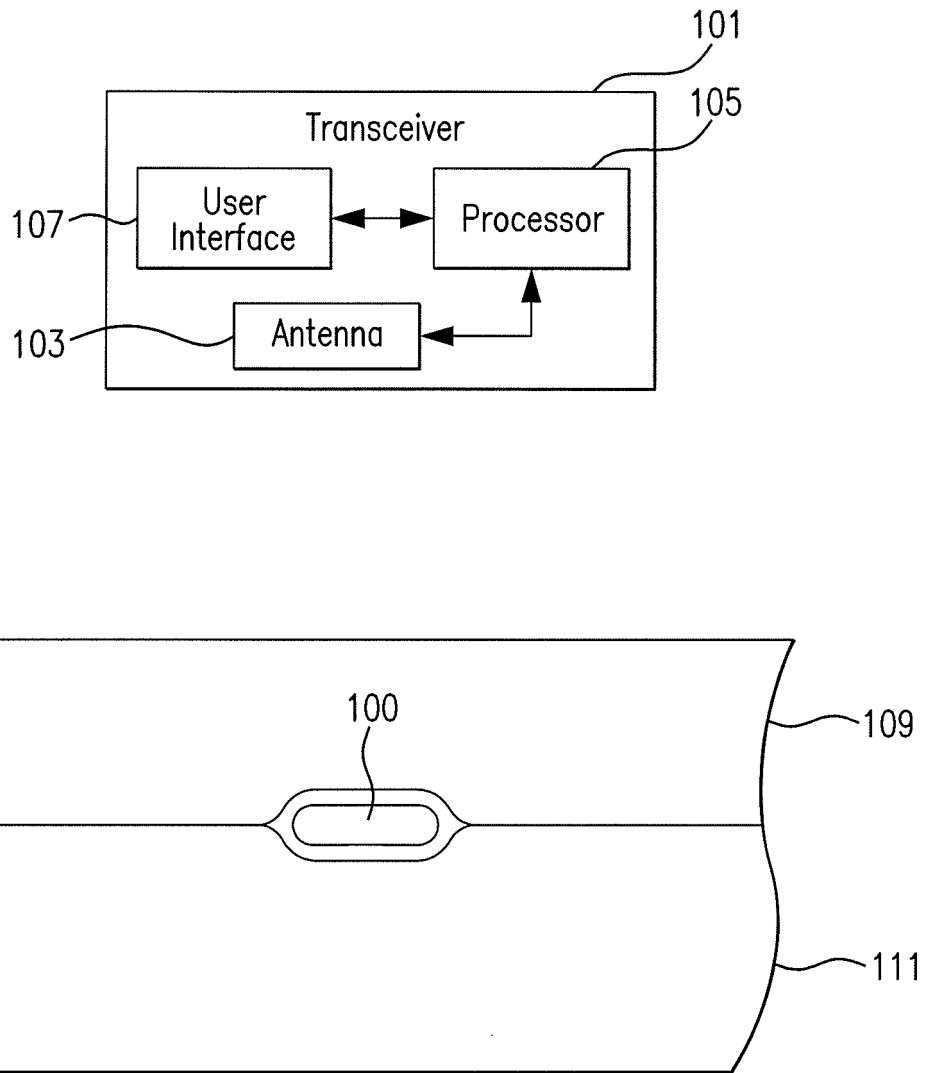


FIG. 1

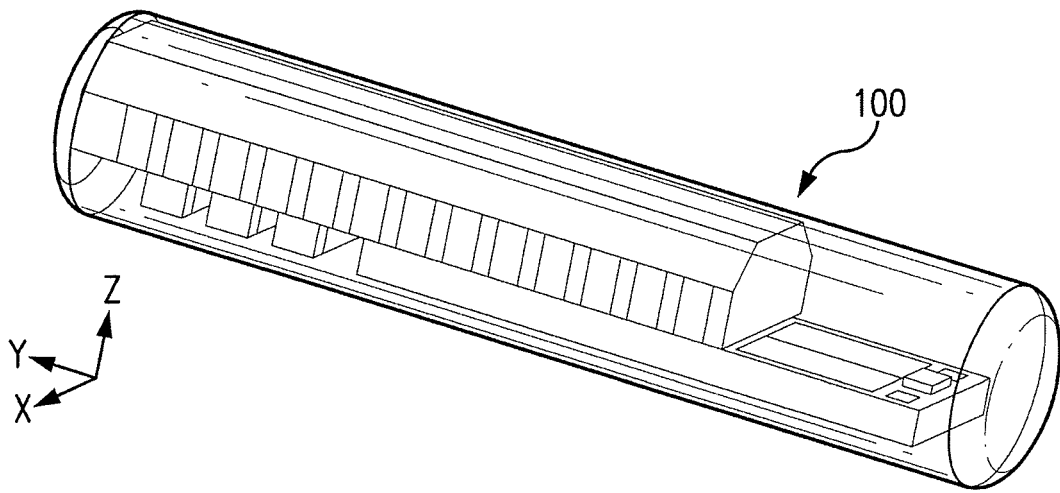


FIG. 2

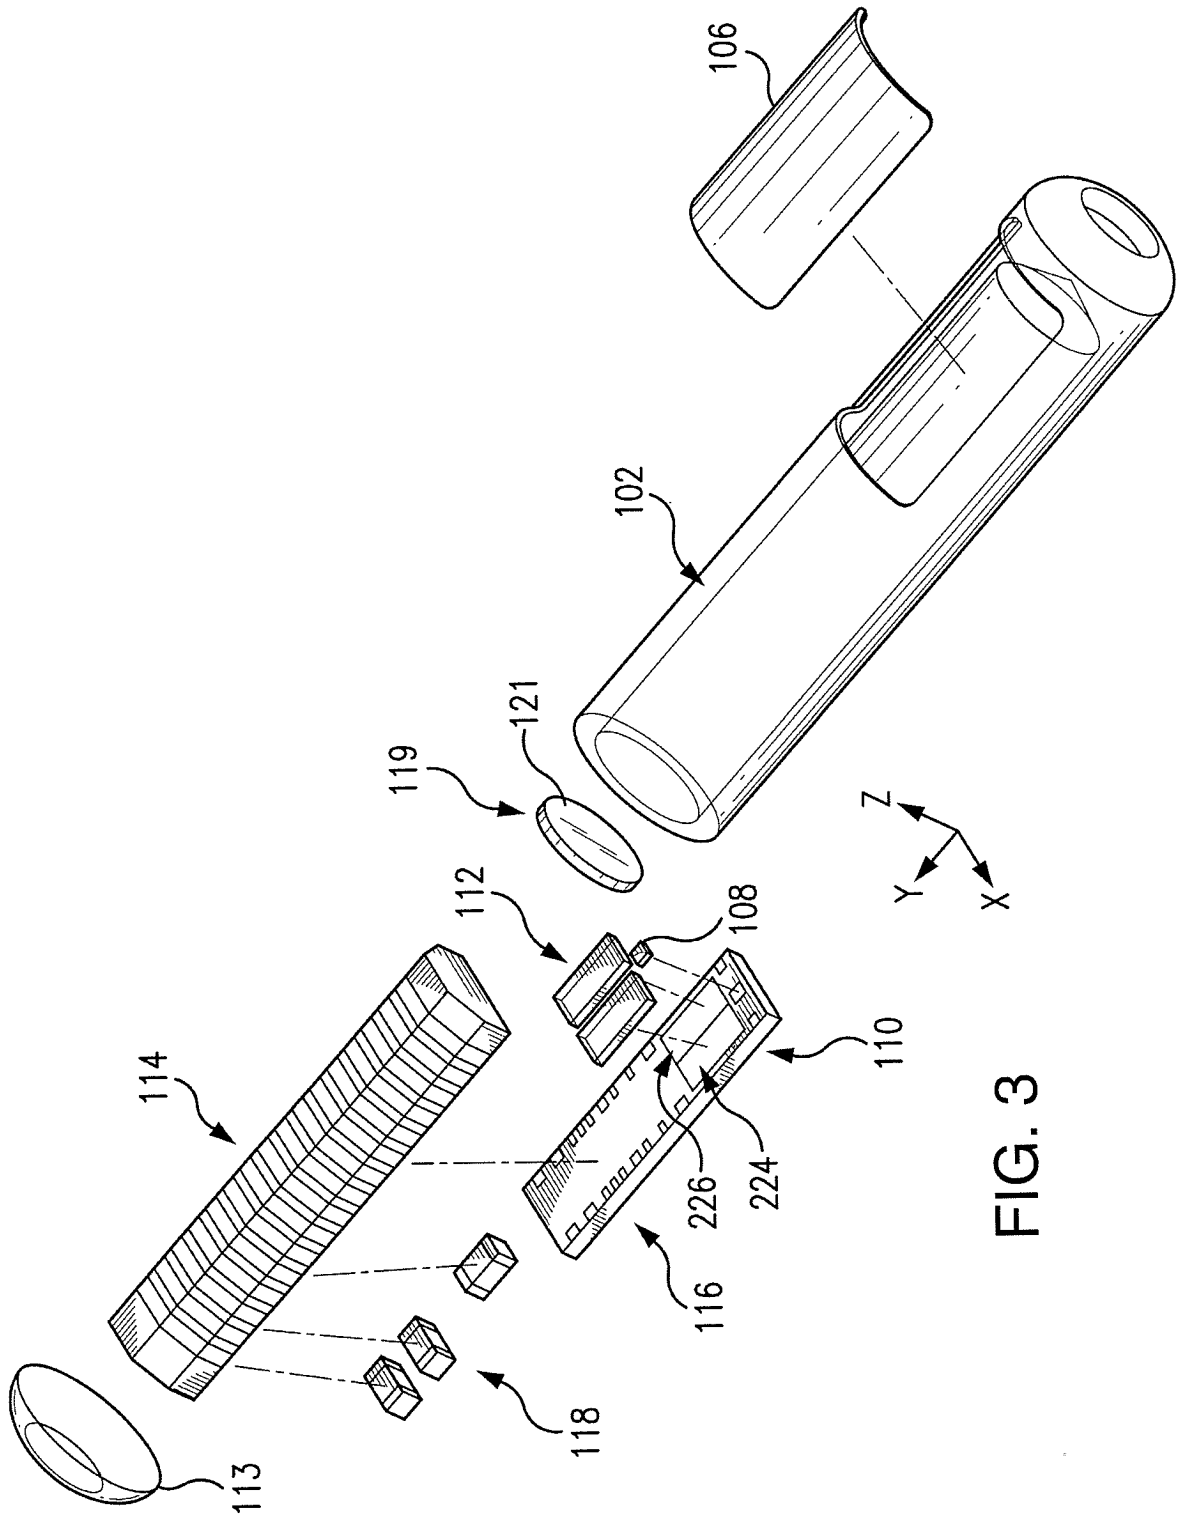


FIG. 3

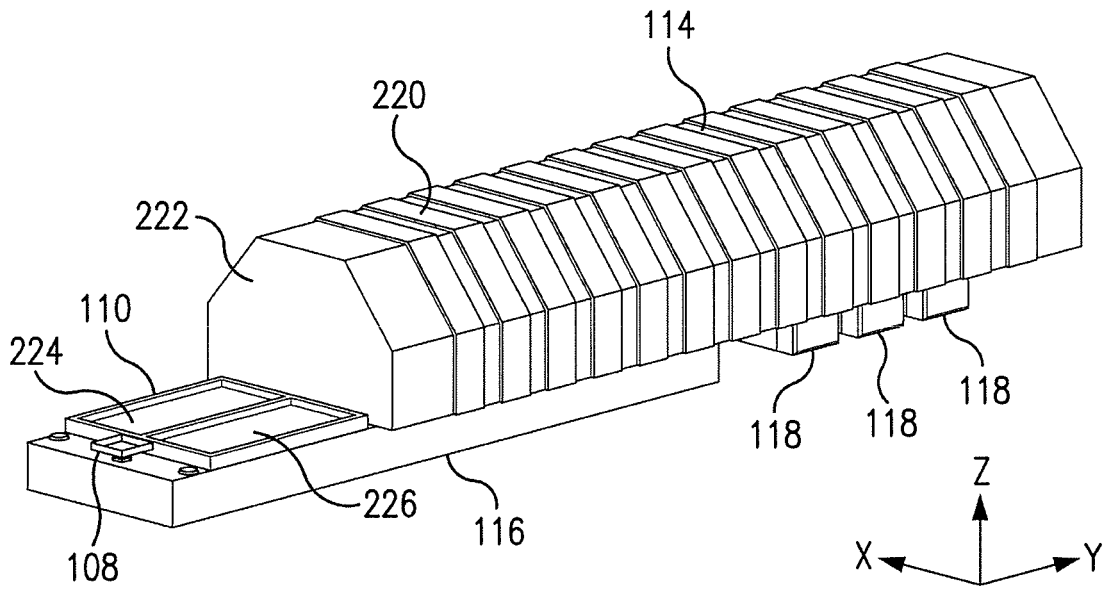


FIG. 4

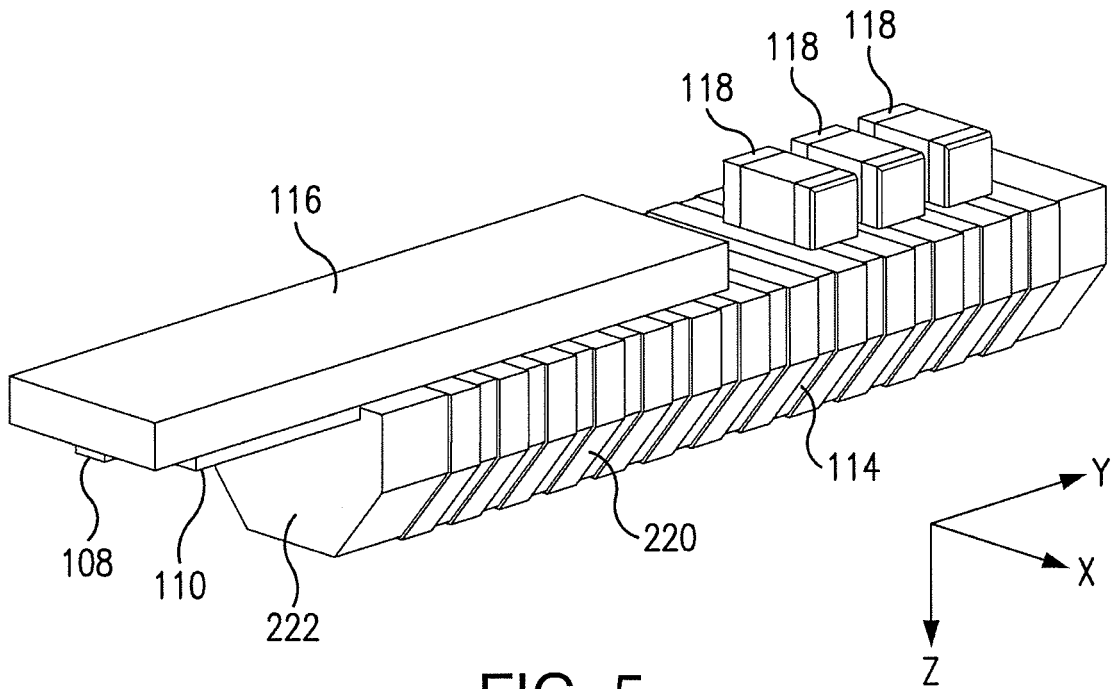


FIG. 5

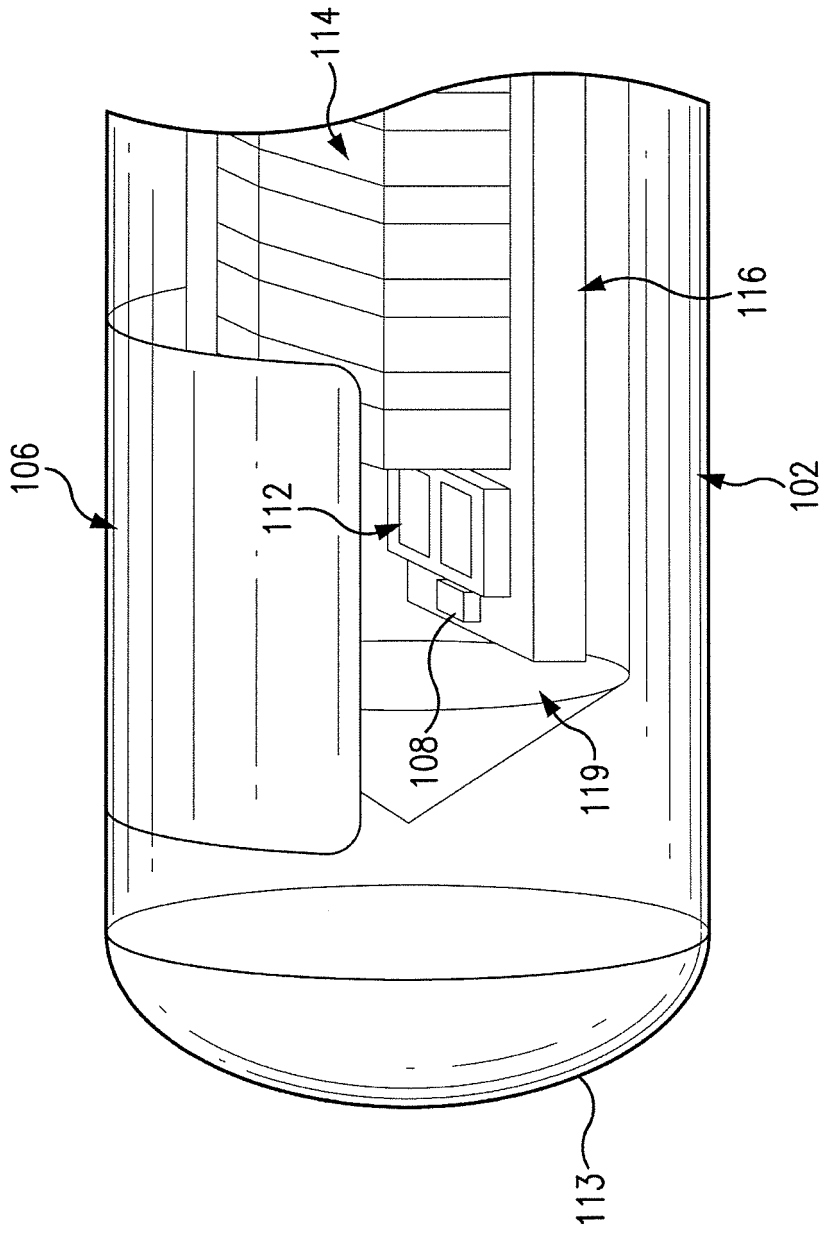


FIG. 6

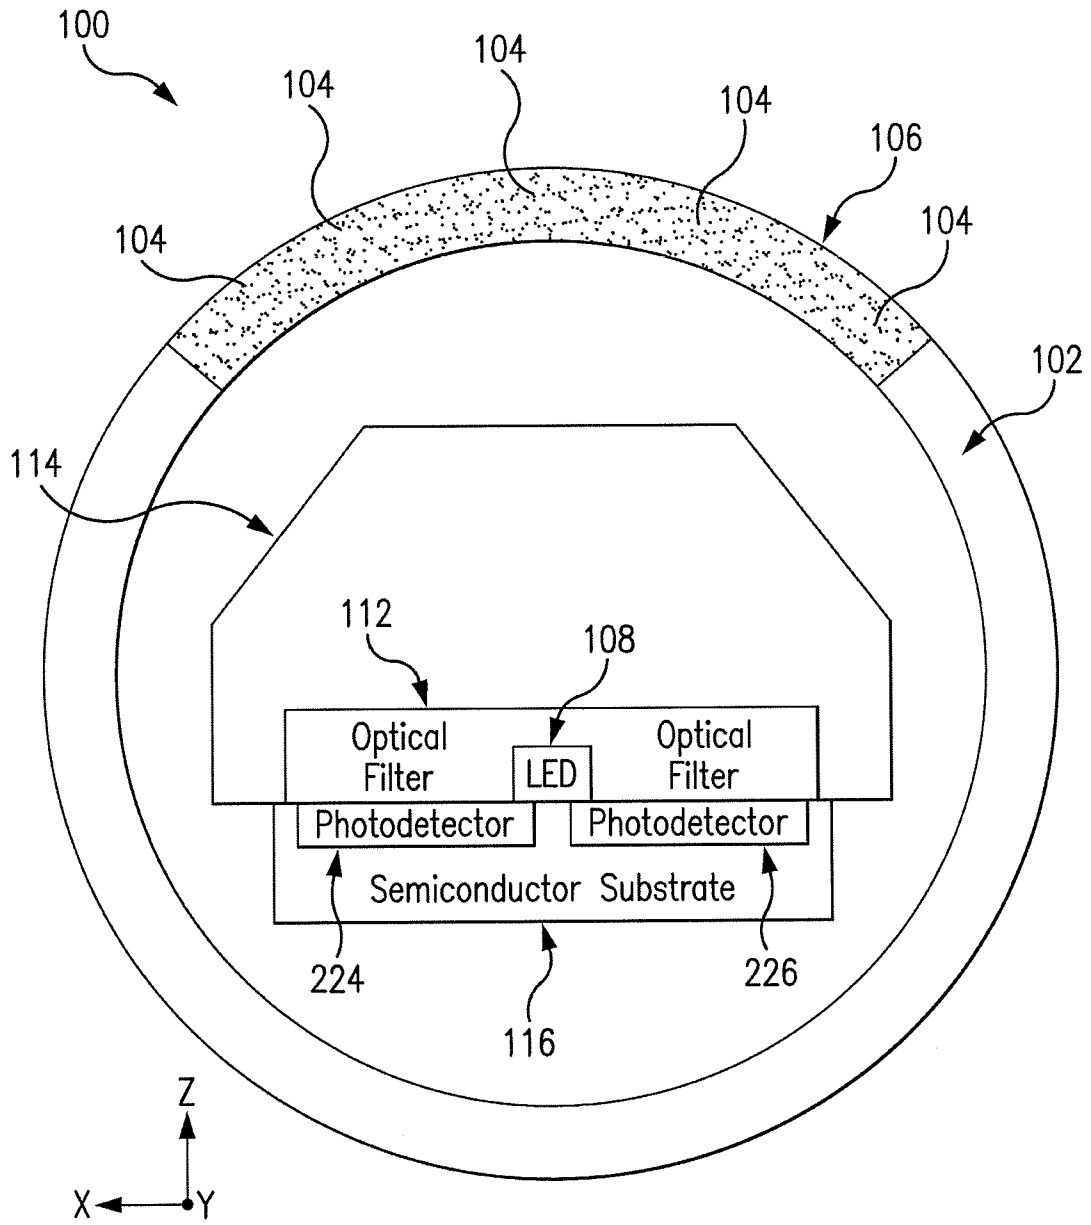


FIG. 7

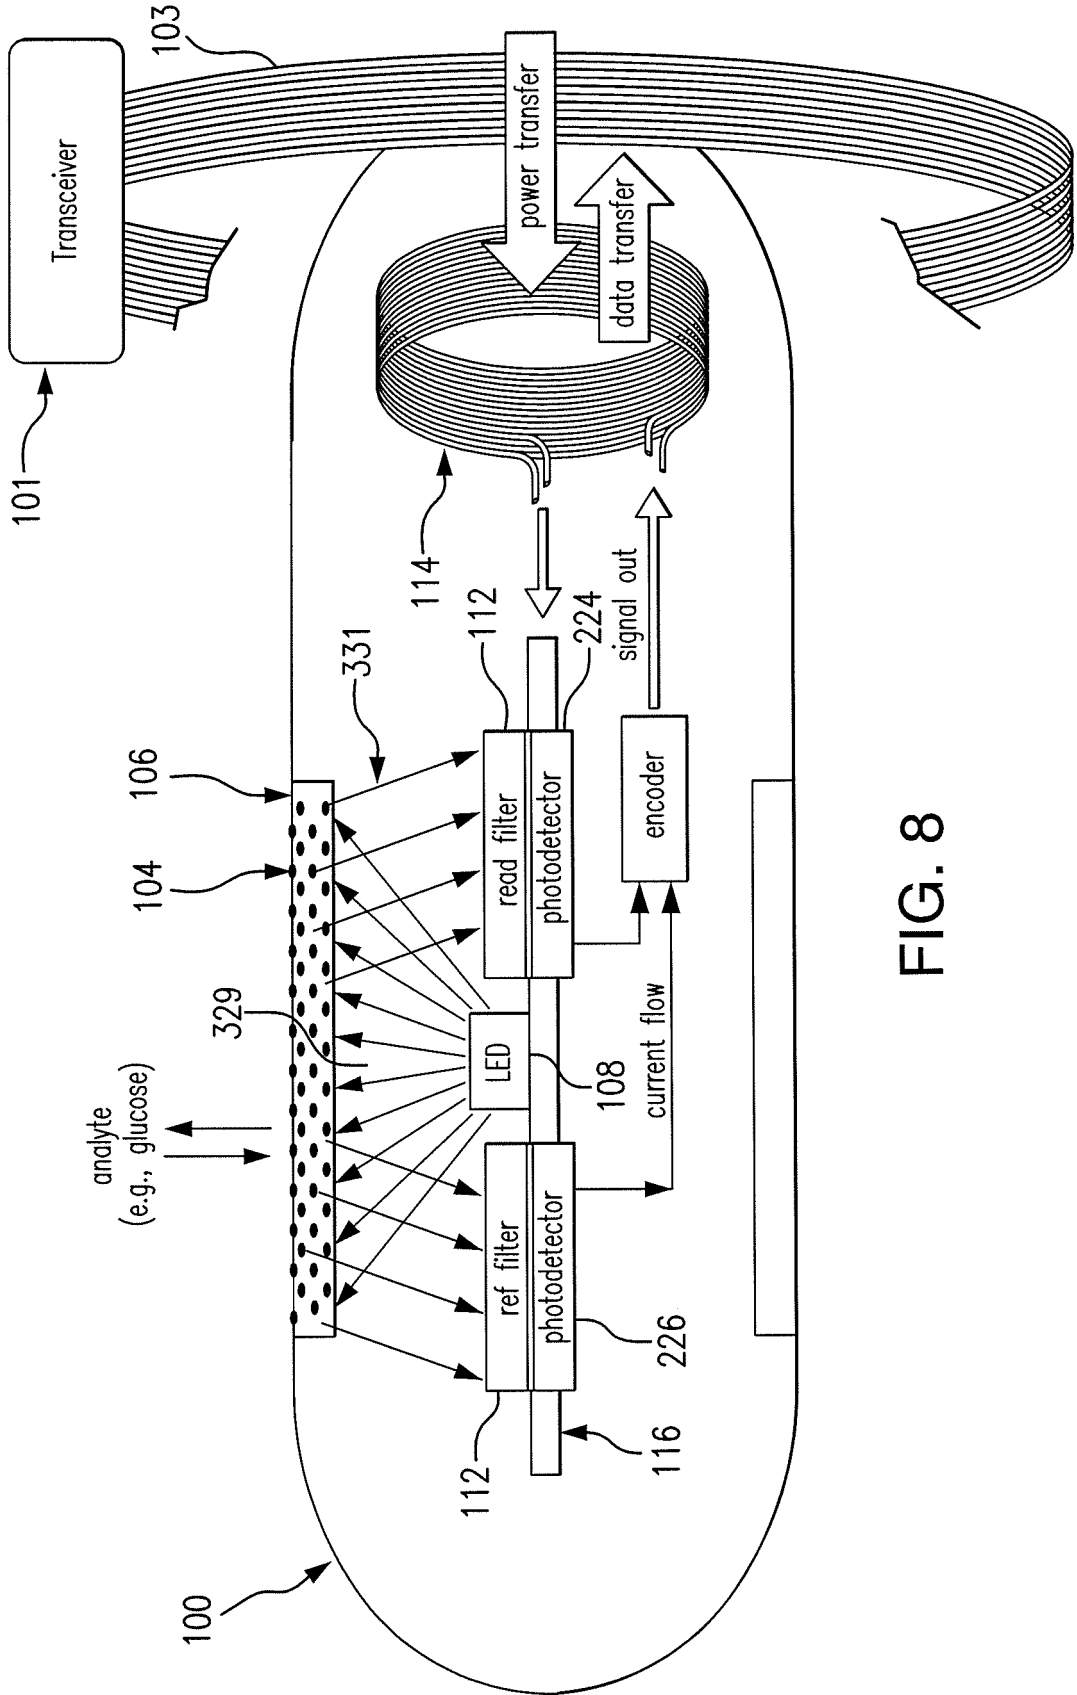


FIG. 8

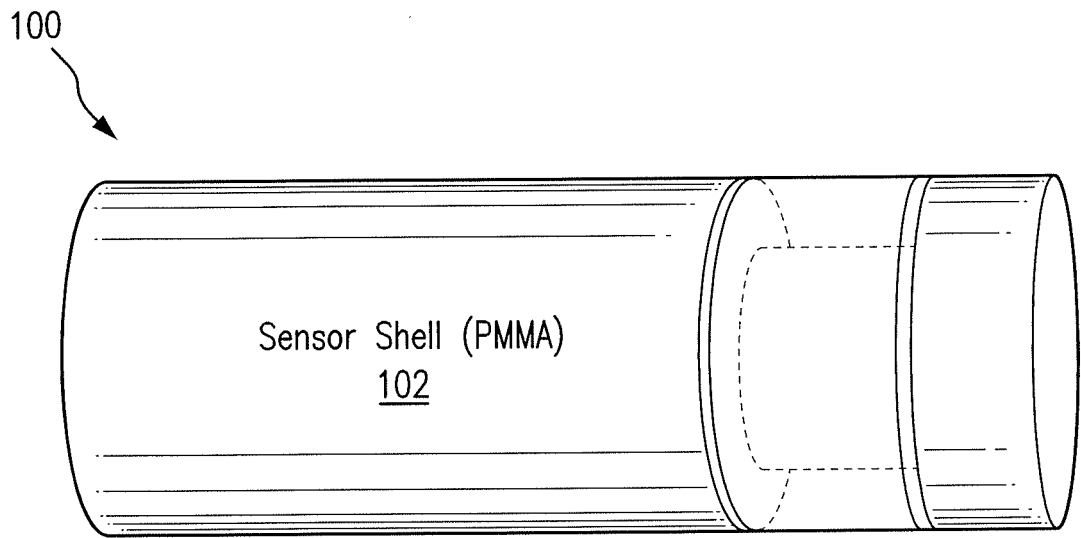


FIG. 9

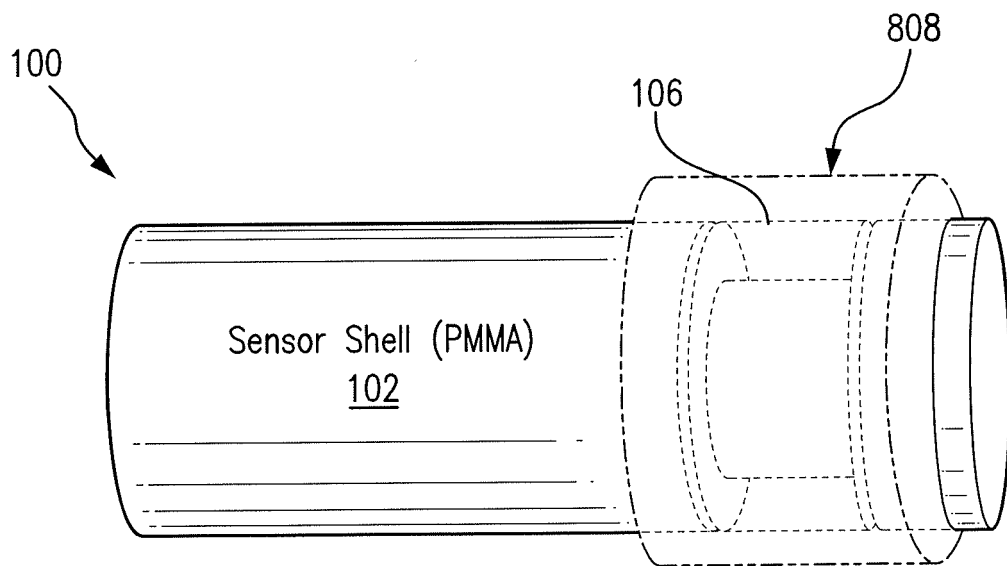


FIG. 10

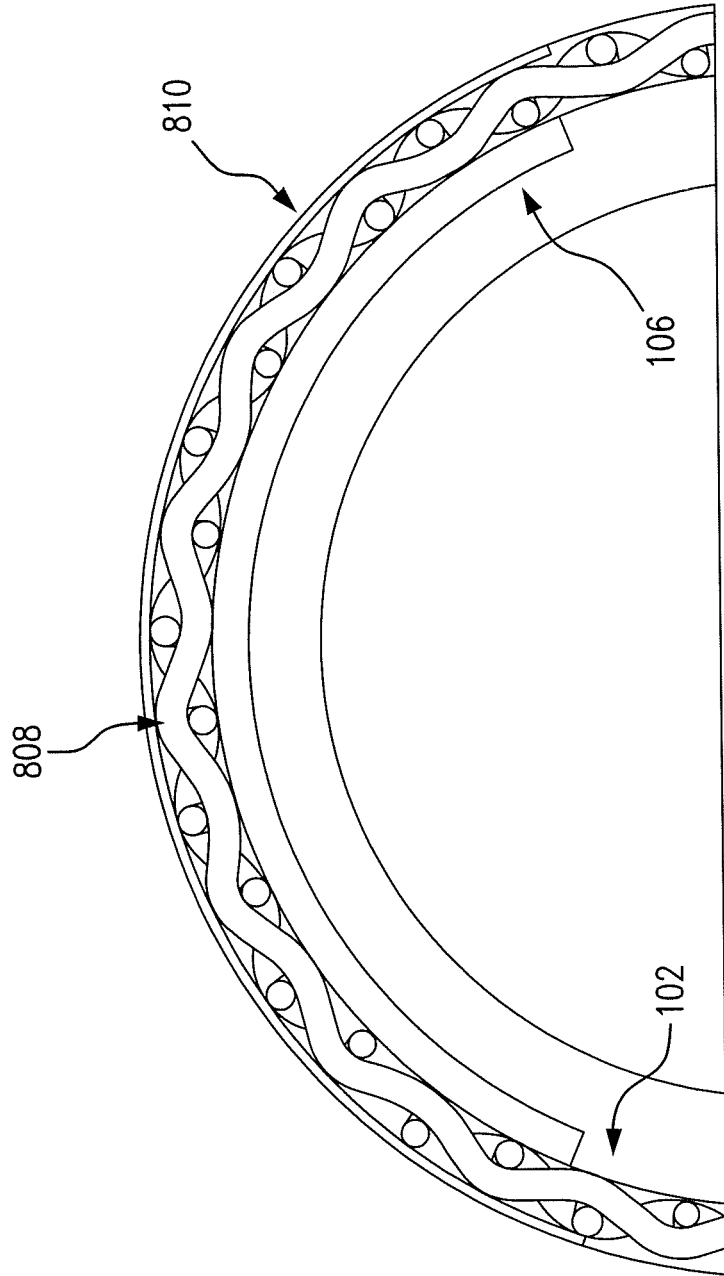


FIG. 11

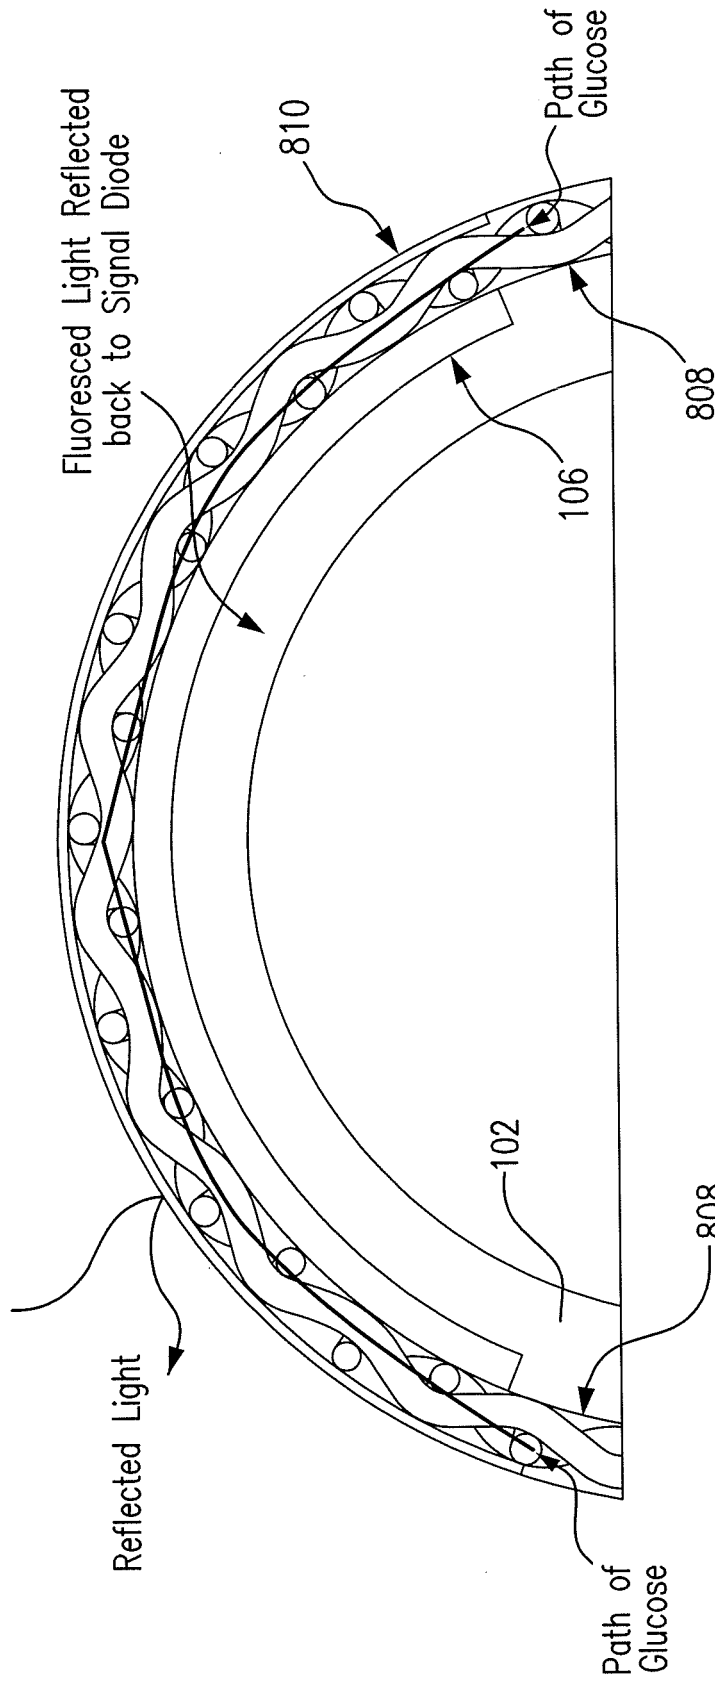


FIG. 12

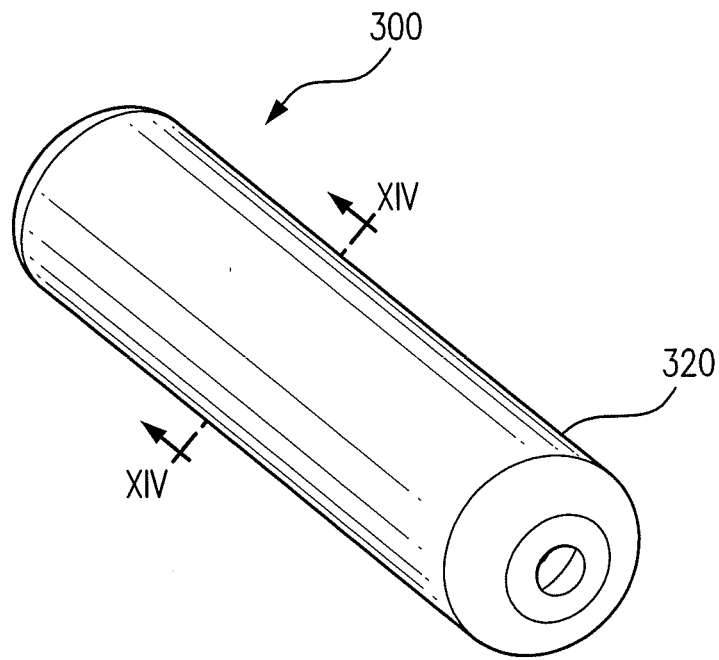


FIG. 13

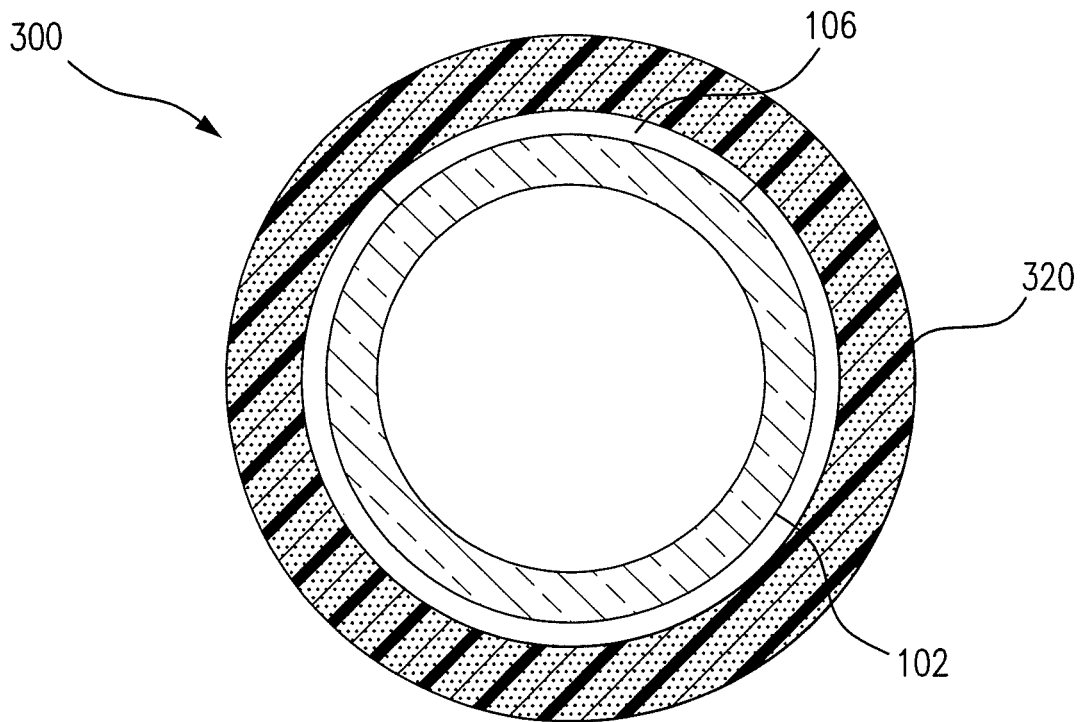


FIG. 14

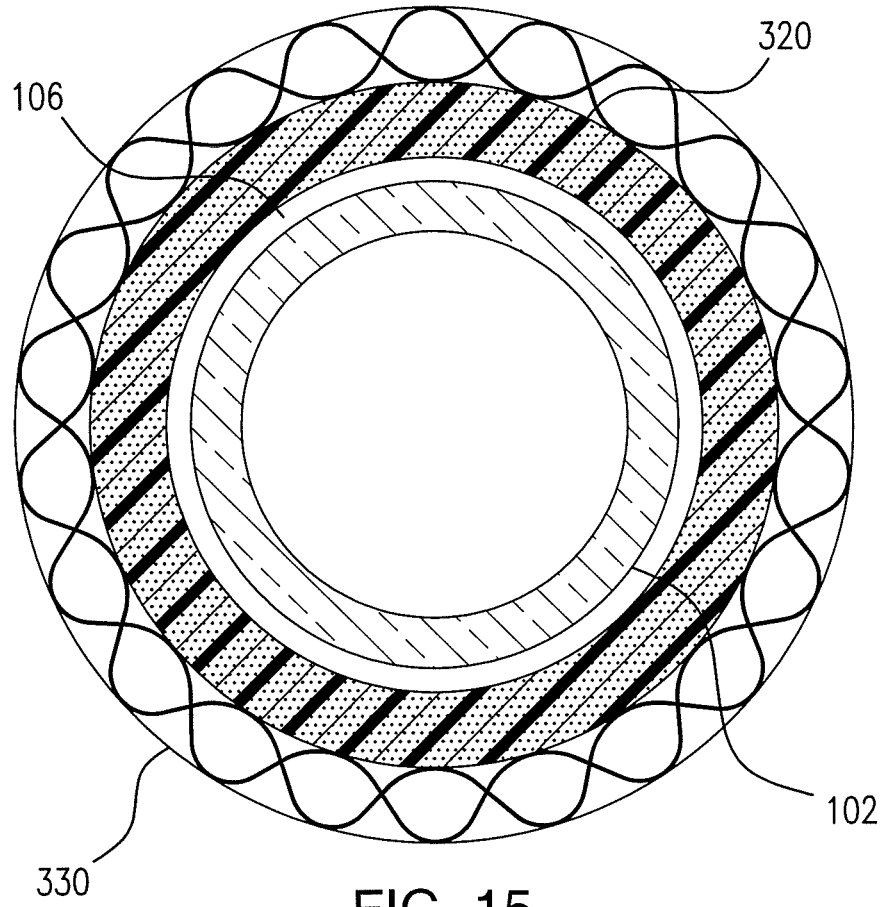


FIG. 15

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 61746790 A [0001]
- US 61847881 A [0001]
- US 20120238842 A1 [0008]
- WO 2014043204 A1 [0008]
- US 8126554 B2 [0009]
- WO 2010123972 A1 [0010]
- US 937871 A [0027]
- US 6344360 B [0029]
- US 937871 [0029] [0033]
- US 650016 A [0033] [0034]
- US 7800078 B [0040]

专利名称(译)	用于氧化和光学稳定性的分析物渗透膜系统		
公开(公告)号	<a href="#">EP2938249A4</a>	公开(公告)日	2016-08-31
申请号	EP2013868464	申请日	2013-12-27
申请(专利权)人(译)	SENSEONICS注册成立		
当前申请(专利权)人(译)	SENSEONICS INCORPORATED		
[标]发明人	EMKEN JEREMY HUFFSTETLER PHILIP WHITEHURST TODD		
发明人	EMKEN, JEREMY HUFFSTETLER, PHILIP WHITEHURST, TODD		
IPC分类号	A61B5/00		
代理机构(译)	泽吉尔斯达, ROBERT WIEBO JOHAN		
优先权	61/746790 2012-12-28 US 61/847881 2013-07-18 US		
其他公开文献	EP2938249B1 EP2938249A2		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

可用于检测动物体内培养基中分析物的存在, 量和/或浓度的传感器。传感器可包括传感器壳体, 嵌入传感器壳体的至少一部分内和/或覆盖传感器壳体的至少一部分的指示器元件, 以及指示器元件上方的膜。膜可以通过防止诸如白细胞的免疫细胞接触指示元件来减少指示元素的劣化, 基本上防止至少特定波长或波长范围的光透过膜, 和/或允许分析物传递给指示元素。膜可以是不透明的扩散膜。传感器可包括箔。箔可以阻挡光和/或减少指示元件劣化。膜可以减少指示元素的氧化。