

(19)



(11)

EP 3 228 237 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:

25.12.2019 Bulletin 2019/52

(51) Int Cl.:

A61B 3/028 ^(2006.01) **A61B 3/09** ^(2006.01)
A61B 3/103 ^(2006.01) **A61B 5/00** ^(2006.01)
A61B 5/06 ^(2006.01) **A61B 5/107** ^(2006.01)
A61B 5/11 ^(2006.01)

(21) Application number: **16164472.9**

(22) Date of filing: **08.04.2016**

(54) A DEVICE AND METHOD FOR MEASURING DISTANCES

VORRICHTUNG UND VERFAHREN ZUM MESSEN VON ENTFERNUNGEN

DISPOSITIF ET PROCÉDÉ DE MESURE DE DISTANCE

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(43) Date of publication of application:

11.10.2017 Bulletin 2017/41

(73) Proprietor: **Vivior AG**

8005 Zürich (CH)

(72) Inventors:

• **Zakharov, Pavel**
8604 Volketswil (CH)

• **Mrochen, Michael**
8193 Eglisau (CH)

(74) Representative: **Frenkel, Matthias Alexander**

Wuesthoff & Wuesthoff
Patentanwälte PartG mbB
Schweigerstrasse 2
81541 München (DE)

(56) References cited:

WO-A1-2014/126307 US-A1- 2003 218 721
US-A1- 2011 249 237

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 3 228 237 B1

Description

[0001] The present invention is directed to a distance measuring system and a method for measuring viewing distances between a subject, e.g. a user, and one or more objects in the subject's viewing direction. The device and method allow a determination of a statistical distribution of the measured viewing distances.

[0002] In ophthalmology, it is important to characterise and understand patient's vision requirements in order to customise a therapy to achieve best clinical outcome and a patient's satisfaction.

[0003] This is, for example, the case in the cataract surgery, when a natural crystalline lens is replaced by an artificial intraocular lens (IOL). Due to the limitations of the current technology, IOL lacks the ability to accommodate to different distances. Thus, the implanted monofocal artificial lens is set to a specific viewing distance defined by a refractive target. As a result the eye of the patient is fixed to a specific viewing distance and the patient has to use refraction correction means (such as glasses) to see sharp in other distances. Alternatively, a surgeon might suggest a premium refractive solution that can be a multifocal and aspheric IOL or a cataract surgery in combination with a corneal refractive surgery, which allows the patient to retain acceptable visual performance at a set of viewing distances. The refractive solution and refractive targets which are derived from the patient's viewing distance needs are chosen before surgery during an interview with the surgeon based on the patient's preferences. The patient consults the surgeon and explains his or her requirements based on personal habits, occupation, lifestyle and preferences. Thus, the decision is based on the patient's subjective perception of his or her habits and requirements, which may reflect misperceived vision needs. The consecutive choice of a refractive correction for an artificial lens may neglect required everyday accommodation needs.

[0004] For the laser refractive correction surgery, when presbyopia of the patient is taken into account (for example in presbyopia treatment), surgery has to be adjusted for the optimisation of visual performance for the specific viewing distances. Viewing distances outside of the optimised range would be compromised. Thus, during the surgery planning, a medical professional has to be able to understand the patient's visual requirements in order to better adjust the range of optimised vision performance for a specific patient. Any ophthalmic treatment or procedure which has to take into account limited accommodating performance of the eye irrespectively if it is induced by this procedure or by other factors would benefit from objective characterisation of the patient's visual habits and requirements.

[0005] Since the patient is subject to his own subjective perception, there is a need for a technique supporting a more objective decision for the selection of an artificial lens.

[0006] Document WO-A-2014/179 857 discloses a dis-

tance measuring system adapted to be mounted on glasses, spectacles' frame and/or adapted to be attached to a subject's head comprising a distance measuring sensor adapted and arranged to measure viewing distances between eyes of a subject and one or more objects, a memory unit and a processing unit.

[0007] According to a first aspect of the present invention, a viewing distance measuring system according to claim 1 is disclosed, which comprises a distance measuring sensor, a memory unit and a processing unit. The distance measuring sensor is adapted and arranged to measure viewing distances between eyes of a subject, e.g. eyes of a user, and one or more objects. The viewing distances may be measured between the eyes of the subject and the one or more objects in the distance measuring sensor's viewing direction. The memory unit is adapted to store the measured viewing distances in a set of measured viewing distances. The processing unit is adapted to determine a statistical distribution of the measured viewing distances from the set of measured viewing distances.

[0008] The memory unit may be a storage unit, arranged in the distance measuring system, for example in a distance measuring device of the distance measuring system, on a connected mobile device, mobile or desktop personal computer. The memory unit may also be or be part of a cloud storage. That is, the memory unit may be part of the same device as the distance measuring sensor, e.g. part of the distance measuring device, or may be part of a different device than the distance measuring sensor. Similarly, the processing unit may be part of the same device as the distance measuring sensor and/or the memory unit, e.g. may be part of the distance measuring device, or may be part of a different device than the distance measuring sensor and/or the memory unit.

[0009] Activities and context recognition can be performed based on the statistical distribution derived from a history of measurements of a particular subject or multiple subjects. For example, an activity can have a similar signature in signals of various subjects and thus an algorithm can be trained to recognise the activity automatically.

[0010] The distance measuring sensor's viewing direction can be understood as the sensitivity of the distance measuring sensor or the subject's common or normal viewing direction. In such common or normal viewing direction, the subject's head can be turned into a direction of the one or more objects and the distance measuring sensor's viewing direction may be oriented into the subject's viewing direction. The subject may be understood as the person wearing a device including the distance measuring sensor, e.g. wearing the distance measuring device, e.g. a patient. The user may be understood as the person evaluating the statistical distribution, e.g. a medical professional such as a doctor.

[0011] The distance measuring sensor can be an optical, acoustical or an electromagnetic sensor, for example a LASER, SONAR, LIDAR or RADAR. The distance

measuring sensor can be a time-of-flight optical sensor. Further, the distance measuring sensor can be an imaging sensor. The distance measuring system may contain two or more distance measuring sensors being able to obtain distances of multiple objects at the same time. For example, the two distance measuring sensors can be located on the left and right side of the subject's head, glasses or spectacles' frame. The distance measuring sensor can also be an imaging sensor, for example a camera, capable to acquire or derive three-dimensional scenes, for example a stereo image sensor in a double camera system, time-of-flight sensor or imaging sensor with a structured illumination.

[0012] The statistical distribution may indicate average and/or overall viewing distances viewed by the subject, e.g. a patient, over a certain period of time. The certain period of time may be one or more hours or one or more days. The statistical distribution can be in a form of histogram where viewing distances can be weighted. For example, the viewing distances can be weighted based on the frequency of their occurrence. The statistical distribution can be in a form of a histogram where viewing distances can be weighted based on the subject's feedback. Important periods may be elevated. Unimportant periods may be reduced. The subject can highlight or elevate a significant or an important time period or reduce an insignificant or unimportant time period.

[0013] The statistical distribution can be stratified based on the subject's activities and context and presented separately for each activity and context. Context-aware statistics might also include time spent in specific activities and context. If the data is used for a cataract surgery planning, the statistical distribution allows a medical professional to more objectively choose the right refractive power of an artificial lens to be implanted into the patient's eye. The context-aware statistics can allow the medical professional to choose a refractive solution based on the importance of a specific context to the patient.

[0014] In other words, the statistical distribution forms a more objective basis of decision-making for the medical professional.

[0015] The distance measuring system may further comprise an eye monitoring unit. The eye monitoring unit is adapted and arranged to detect the subject's eye direction relative to the distance measuring sensor's viewing direction. The processing unit may be further adapted to statistically weight, select or discard the measured viewing distances from the set of measured viewing distances based on the subject's eye direction relative to the distance measuring sensor's viewing direction. Eye monitoring measurements can be stored for further retrospective analysis. Discarded measured viewing distances may be neglected for determining the statistical distribution and thus not considered for determining the statistical distribution of the measured viewing distances. Selected measured viewing distances can be the most valuable viewing distances for a specific acquisition time

or the only measured viewing distances to be measured during a subject's favourite activity. These selected measured viewing distances may be the only measured viewing distances considered for storing in the set of measured viewing distances and the only measured viewing distances considered for the statistical distribution. In one specific example, the subject's eye direction may be considered to be substantially different to the distance measuring sensor's viewing direction if the subject's eye direction is not parallel to the distance measuring sensor's viewing direction. The subject's eye direction may be defined as the direction of one of the subject's eyes, but may be defined as the direction of both of the subject's eyes.

[0016] Statistically weighting, selecting or discarding the measured viewing distances when the subject's eye direction is substantially different to the distance measuring sensor's viewing direction has the advantage to better indicate where the subject's (here a patient's) viewing distances are the most likely to occur. For example, viewing distances that only occur for a number of times that is below a predetermined threshold are not or at least less considered for determining the statistical distribution.

[0017] The distance measuring sensor can be a sensor array or an imaging sensor adapted to acquire distances of multiple objects at the same time. The processing unit can statistically weight, select or discard the measured viewing distances from the set of measured viewing distances simultaneously acquired from multiple objects based on the subject's eye direction relative to the distance measuring sensor's viewing direction.

[0018] In one or more embodiments, the eye monitoring unit may comprise any eye tracking functionality. Eye tracking is normally understood as the process of measuring either the point of gaze (where one is looking) or the motion of an eye relative to the head. An eye tracker is thus normally a device for measuring eye positions and eye movement.

[0019] The eye monitoring unit can further be adapted and arranged to detect the subject's eye blinks, the subject's eye motion, the subject's eye pupil size and/or crystalline lens accommodation. The subject's eye blinks, eye motion, pupil size and variations indicate whether the subject is paying attention to the viewed object or not. The subject's pupil variations under stable lighting conditions and the subject's eye direction can serve as an indirect sign of accommodative efforts and indicates importance of the object or scene for the subject. Pupil size, while viewing an object or scene, can also be taken into account as a weighting factor for visual requirements. Constricted pupils increase the depth of field and thus increase the visual tolerance of a refractive error, which can be accounted in the data analysis of the statistical distribution.

[0020] Direct measure of lens accommodation effort in the stable viewing direction serves as an indication of importance of the viewed object scene and thus also can

be taken into account.

[0021] Further, the eye monitoring unit can be adapted and arranged to detect light reflections from an optical surface of the subject's eye. This light can be from an external (ambient) source or from a light source mounted on the device carrying the eye monitoring unit, e.g. the distance measuring device. The reflection from a corneal front surface as well as from a lens' surface allows for more precisely determining eye movements. At the same time, reflections from the lens' surface can be used for the measurements of the lens' accommodative changes. The eye monitoring unit can also determine the blinking and open and/or closure timing for the processing unit to derive the subject's mental state, wakefulness and drowsiness.

[0022] One or more, e.g. all, of the above-mentioned factors can be taken into account for determining the statistical distribution. In this respect, the processing unit can further be adapted to weight or to discard the measured viewing distances based on the subject's eye blinks, the subject's eye motion, the subject's pupil size and/or variation. For example, the processing unit can be adapted to weight, with a weighting factor smaller than one, or to discard the measured viewing distances that have been measured while / when the number of blinks of the subject's eye is higher than a predetermined threshold or for example when the subject is sleeping. Alternatively or additionally, the processing unit can be adapted to weight, with a weighting factor smaller than one, or to discard the measured viewing distances that have been measured while / when the motion of the subject's eye is higher than a predetermined threshold. Additionally, the subject's pupil variations under stable light conditions as indication of accommodative effort can be taken into account in the statistics. In this way, the attention the subject pays to the specific object /scene can be taken into account for determining the statistical distribution.

[0023] In one case, measurements of viewing distance can be discarded when subject's eyes are closed, for example during a blink, or during sleep.

[0024] Weighting the measured viewing distances comprises prioritizing or deprioritizing measured viewing distances by weighting the measured viewing distances with values smaller than one, e.g. equal to or close to zero, for deprioritizing and values higher than one for prioritizing.

[0025] The distance measuring system further comprises a movement sensor. The movement sensor may be for example an accelerometer, a gyroscope, a magnetometer, an altimeter, a pedometer and/or a geopositioning device, or a combination thereof. The movement sensor can be adapted and arranged to measure movements of the subject's body, for example the subject's head. The processing unit can further be adapted to statistically weight, select or discard the measured viewing distances from the set of measured viewing distances based on the measured movements.

[0026] The distance measuring system can further

comprise an ambient light sensor. The ambient light sensor can be adapted and arranged to measure ambient light, light intensity and/or spectral content in the distance measuring sensor's viewing direction. The processing unit can further be adapted to statistically weight, select or discard the measured viewing distances from the set of measured viewing distances based on the measured ambient light, light intensity and/or spectral content.

[0027] The ambient light sensor can further measure total integrated light intensity, specific spectral components and/or hue.

[0028] The distance measuring system can further comprise a proximity sensor. The proximity sensor can be used to detect if the device including the distance measuring sensor, e.g. the distance measuring device, is worn on the body and can control this device accordingly, for example, start measurement automatically, when this device is placed on or at the body.

[0029] The distance measuring system can further comprise a temperature and/or a humidity sensor. The temperature and/or humidity sensor can be used to identify an environment the subject is exposed to on a daily basis, the attention of the subject and the activities he or she is doing regularly. The environment can also be referred to as context or context information.

[0030] The distance measuring system can further comprise a user interface. The user interface can be adapted to receive a user input. The processing unit can further be adapted to weight, select or discard the measured viewing distances from the set of measured viewing distances based on the user input. The user interface can be for example a touch display, a button, a trigger, a proximity sensor, microphone and/or a tap detector. The user input can further be a head shake, an eye blink, an eye squint, eye movement, a hand gesture and/or voice command, wherein the user interface may comprise or be replaced by or be configured as the movement sensor or the eye monitor unit.

[0031] The user interface may be further adapted to generate a feedback signal for the subject. This feedback signal may be based on the measured distance and may be in the form of an acoustic, visual or haptic indicator. For example, the user interface may generate an alarm for the subject by a vibration of the distance measuring system or a connected cell phone when the subject is reading a book too close under inadequate lightning conditions.

[0032] The user input provides the advantage of getting feedback from the patient and assessing an activity he or she deems important or unimportant throughout the day.

[0033] Further, the distance measuring system can comprise a intermittent (triggered) measurement mode to be used by the subject. The user input can be used to initiate measuring viewing distances by the distance measuring system if the intermittent (triggered) measurement mode is used. For example, the distance measuring system might only perform measurements when

the measurements are initiated by the subject (spot-measurements).

[0034] The distance measuring system is further adapted to be mounted on glasses, spectacles' frame and/or adapted to be attached to the subject's head. The distance measuring system can be integrated in or arranged at or on glasses and/or a spectacles' frame respectively. Further, the distance measuring system could be attached to the subject's head by straps, to a helmet, to a headset, to hearing aid or headphones. The distance measuring system may be configured as or attached to a wearable device.

[0035] The processing unit can further be adapted to calculate one or more refraction requirements from the viewing distances. The former can be expressed in diopters (D) being reciprocal to the latter, which is expressed in meters.

[0036] The processing unit can further be adapted to calculate a target refraction by applying a statistical method to the statistical distribution of the measured viewing distances. The measured viewing distances can indicate the required refraction needs. The statistical method can be or include a mean, a variance, a standard deviation, a median or a maximum which allows for a surgeon to select an overall best fitting refractive correction for an artificial lens.

[0037] The distance measuring system according to the first aspect can be used before the subject's cataract surgery. The subject can wear the distance measuring system in order to gather information and extract a statistical distribution determined by the processing unit. The determined statistical distribution considers the needs of the subject and provides information for a selection and adjustment of an artificial lens type and parameters to be implanted into the subject's eye.

[0038] One exemplary implementation of the distance measuring system can be that the subject, in this case a cataract patient is provided with the device by the user, in this case a cataract surgeon or a supporting member of a medical staff, who may initialise the device for the patient. The Patient may wear the device for a required amount of time, which could be several days. Wearing of the device may be recognised by a proximity sensor and/or by a motion sensor detecting motion. The distance measuring sensor may perform continuous measurements when the patient wears a distance measuring device of the distance measuring system and may store viewing distances in the internal or external memory unit. At the next visit the patient returns the device to the user, who may download the data from the memory unit to allow processing by the processing unit. The statistical distribution may then be used to find the optimal individual refractive solution. In another exemplary implementation, the patient may perform triggered measurements under specific conditions or specific activities.

[0039] According to a second aspect of the present invention, the distance measuring system according to the first aspect can be used for selection and customisa-

tion of a refractive solution in cataract surgery. The data gathered from and determined by the distance measuring system according to the first aspect e.g. presented as statistics of refraction needs can be used to select the optimal lens or combination of lenses (refractive solution) based on the optical properties of lenses available in the database. The refractive solution can be two lenses (monofocal or multifocal) of a single type implanted in both eyes which fits the statistics of refraction needs, or two lenses with two different optical profiles which being implanted in eyes create a vision solution through binocular fusion (monovision).

[0040] With the same method customisation can be done by adjusting optical profiles of artificial lenses or manufacturing artificial lenses with required optical profiles.

[0041] According to a third aspect of the present invention, a distance measuring method according to claim 8 is provided. The method comprises the steps of measuring viewing distances, by a distance measuring sensor of a distance measuring system, between eyes of a subject, e.g. eyes of a user, and one or more objects. The viewing distances may be measured between the eyes of the subject and the one or more objects in the distance measuring sensor's viewing direction. The method further comprises storing, by a memory unit of the distance measuring system, the measured viewing distances in a set of measured viewing distances. The method further comprises determining, by a processing unit of the distance measuring system, a statistical distribution of the measured viewing distances from the set of measured viewing distances.

[0042] The method can further comprise detecting, by an eye monitoring unit, the subject's eye direction relative to the distance measuring sensor's viewing direction. and the method may further comprise statistically weighting, selecting or discarding, by the processing unit, the measured viewing distances from the set of measured viewing distances based on the subject's eye direction relative to the distance measuring sensor's viewing direction.

[0043] The method further comprises measuring, by a movement sensor, movements of the subject's body, for example the subject's head. The method may further comprise statistically weighting, selecting or discarding, by the processing unit, the measured viewing distances from the set of measured viewing distances based on the measured movements.

[0044] The method can further comprise measuring, by an ambient light sensor of the distance measuring system, ambient light, light intensity and/or spectral content in the distance measuring sensor's viewing direction. The method may further comprise statistically weighting, selecting or discarding, by the processing unit, the measured viewing distances from the set of measured viewing distances based on the measured ambient light, light intensity and/or spectral content.

[0045] The method can further comprise receiving, by a user interface of the distance measuring system, a user

input. The method may further comprise weighting, selecting or discarding, by the processing unit, the measured viewing distances from the set of measured viewing distances based on the user input.

[0046] The method can further comprise calculating, by the processing unit, a target refraction by applying a statistical method to the statistical distribution of the measured viewing distances.

[0047] The method or parts of the method may be implemented by a computer program. The computer program may comprise program code portions for causing the steps of any one of the method aspects described herein to be performed, when the computer program is run on a computer system or on one or more computing devices, e.g. an apparatus, like the distance measuring system. The computer program may be stored on a computer-readable recording medium or may be downloadable as a signal.

[0048] The method according to the third aspect may be performed before or after cataract surgery. Alternatively, the method may be performed before, during or after contact lens or spectacle fitting.

[0049] In general, the steps of any one of the method aspects described herein may equally be embodied in one or more suitable components, devices or units, e.g. in suitable components of the distance measuring system. Likewise, any of the details described with respect to the distance measuring system may be embodied as a method and/or as a computer program carrying out the method.

[0050] In the following, the present invention will further be described with reference to exemplary embodiments illustrated in the Figures, in which:

- Figure 1 schematically illustrates an embodiment of the distance measuring system according to the present invention;
- Figure 2 schematically illustrates an embodiment of a distance measuring method according to the present invention;
- Figure 3 schematically illustrates occurrences over distance and corresponding refraction respectively;
- Figure 4 schematically illustrates a two-dimensional distance mapping diagram and the underlying ambient light intensity distribution; dimensions on the mapping are in centimeters, half-circles indicates boundaries of the near vision zone (<50 cm), intermediate zone (between 50 and 100 cm) and far zone (above 100 cm);
- Figure 5 schematically illustrates two dimensional diagrams with respect to viewing preferences of a subject;

Figure 6 schematically illustrates a distribution of an ambient light intensity;

Figure 7 schematically illustrates the use of the embodiment of the distance measuring system of Figure 1 arranged on glasses;

Figure 8 schematically illustrates a time history of refraction requirements distribution and ambient light;

Figure 9 schematically illustrates examples of statistical distributions of refraction requirements calculated by the embodiment of the distance measuring system for different activities;

Figure 10 schematically illustrates distributions of refraction requirements and mean light intensities associated with specific requirements;

Figure 11 schematically illustrates possible solutions for a realization of optimal refraction requirements distribution; and

Figure 12 schematically illustrates a prioritization mechanism of prioritized viewing distances.

[0051] In the following description, for purposes of explanation and not limitation, specific details are set forth, such as processing details and steps, in order to provide a thorough understanding of the present invention. It will be apparent to one skilled in the art that the present invention may be practiced in other embodiments that depart from these specific details.

[0052] Those skilled in the art will further appreciate that functions explained herein below may be implemented using individual hardware circuitry, using software functioning in conjunction with one or more processors, e.g. a programmed microprocessor or a general purpose computer, using an Application Specific Integrated Circuit (ASIC) and/or using one or more Digital Signal Processors (DSPs). It will also be appreciated that when the present disclosure is described as a method, it may also be embodied in a computer processor arrangement and a memory arrangement coupled to a processor arrangement, wherein the memory arrangement is encoded with or stores one or more programs or corresponding code to cause the processor arrangement to perform or control the methods disclosed herein when executed by the processor arrangement.

[0053] Figure 1 schematically illustrates the distance measuring system 1 according to an embodiment of the present invention. The distance measuring system 1 comprises a distance measuring sensor 5, a memory unit 7 and a processing unit 10. Optionally, the distance

measuring system 1 comprises an eye monitor unit 15, a movement sensor 20, an ambient light sensor and/or a user interface 30. The different units 5, 7, 10, 15, 20, 25 of the distance measuring system 1 can be realised in one and the same device 1 as illustrated in Figure 1 or can be distributed in two or more separate devices to form the distance measuring system 1. Further details of the distance measuring system 1 will now be described with respect to Figure 2.

[0054] Figure 2 schematically illustrates a method embodiment of the present invention that can be implemented by the distance measuring system of Figure 1. First, distance measuring sensor 5 measures one or more viewing distances in step S10. These distances are distances between a subject and one or more objects in the subject's viewing direction. Second, in step S7, the memory unit 7 stores the measured viewing distances in a set of measured viewing distances. Third, in step S11, the processing unit 10 determines a statistical distribution of the measured viewing distances from the set of measured viewing distances.

[0055] In the following, some steps shown in Figure 2 will be described. These optional steps usually lead to an improved, e.g. more precise, evaluation. For example, eye monitoring unit 15 detects, in optional step S15, the subject's eye direction relative to the distance measuring sensor's direction, e.g. viewing direction. In optional step S16, the processing unit 10 statistically weights, selects or discards the measured viewing distances from the set of measured viewing distances based on the subject's eye direction relative to the distance measuring sensor's direction, e.g. viewing direction. Instead of discarding the measured viewing distances, the processing unit 10 may select specific viewing distances regarded valuable or select subject preferred viewing distances or weight the measured viewing distances with a weighting factor smaller or higher than one. In step S20, a movement sensor 20 measures S20 movements of the subject's body. In the present example, the movement sensor 20 comprises an accelerometer and a gyroscope, but may further comprise different sensors like for example a magnetometer, an altimeter, a pedometer or a geopositioning device. In optional step S21, the processing unit 10 statistically weights, selects or discards the measured viewing distances from the set of measured viewing distances based on the measured movements. If a subject's head is at least substantially steadily pointed to a measured object, the object is measured in distance and weighted by a factor of one or higher than one. If the subject's attention is distracted, e.g. when a subject's head is moving at least substantially constantly around an object, the measured distance is weighted by a factor smaller than 1 or discarded and therefore not considered in the overall statistical distribution.

[0056] Ambient light sensor 25, which may also be extended by using an additional colour sensor, measures ambient light and/or light intensity and/or spectral content in the subject's viewing direction in optional step S25.

The processing unit 10 statistically weights, selects or discards the measured viewing distances from the set of measured viewing distances based on the measured ambient light, light intensity and/or spectral content in optional step S26. The ambient light affects the subject's eye accommodation and depth-of-focus. Under bright illumination, when the pupil of the subject is constricted and subject's depth-of-focus is significantly increased, the measured viewing distances are deprioritized and weighted by values lower one. When considering dim light, for example when the subject is reading a book and the subject's pupils are dilated, which corresponds to ambient light associated with dim illumination, the measured viewing distances are prioritized and weighted by values higher than one.

[0057] In optional step S30, a user interface 30 receives a user input. In optional step S31, the processing unit 10 weights, selects or discards the measured viewing distances from the set of measured viewing distances based on the user input. The subject may use a tap on the distance measuring system 1, on attached devices or on glasses which comprise the distance measuring system 1, in order to weight, select or discard the measured viewing distances. The subject's input can further be head gestures like nodding or shaking, detected by head motion sensor, subject or eye movement, detected by the eye monitoring device. For example, a subject might discard measured viewing distances by looking aside from the object to be measured, directly leading to discarded measuring results, because of the so adjusted eye monitoring device. Another example might be a subject putting his or her hands in front of the sensor with a waving hand gesture or keeping his or her hand in front of the distance measuring system 1 for a few seconds to discard or weight measured viewing distances.

[0058] One or more, e.g. all of the aforementioned weighting or discarding steps may be performed independently from each other or together in a common processing step.

[0059] Finally, the processing unit 10 calculates, in optional step S35, a target refraction by applying a statistical method to the statistical distribution of the measured viewing distances from the set of measured viewing distances. The target refraction, respectively the refractive corrections for an artificial lens, is derived from refractive target diagrams described as refractive requirements diagram in Figure 8 below. These diagrams directly correlate with the distance occurrence measurement results from a distance occurrence diagram exemplarily described in Figure 3 below.

[0060] Figure 3 shows a distance occurrence diagram over distance in centimetres (cm). The diagram of Figure 3 serves an example for distance occurrences that can be obtained by the distance measuring system 1 of Figure 1 with the method steps of Figure 2. The occurrence diagram shows the probability of distance occurrences over specific distances based on actual measurements. By converting distance to refraction the refraction statis-

tics can be obtained. By analysing the refraction statistics (distribution) in Figure 3, the surgeon is able to derive the target refraction or required depth-of-focus from the refractive requirements diagram for one or both eyes. In consequence the surgeon can obtain a statistically best fitting IOL as e.g. characterised by a specific thought-focus-curve (visual acuity or optical quality as a function of viewing distance or refractive addition) for a patient, who used or was wearing the distance measuring system 1 for a certain amount of time. The certain amount of time can be several hours or even several days and is shown to be 30.9 hours in the illustrated scenario of Figure 3. The 30.9 hours lead to 1114K samples of distances for a patient. This duration may be considered as an example mean time for use of / wearing of such a device by a patient.

[0061] Figure 4 illustrates two dimensional maps of viewing range distributions of a person wearing the distance measuring system 1 of Figure 1. The two dimensional maps comprise a vertical viewing distance and horizontal viewing distance. The diagrams indicate horizontal distances from 0 to 600 cm in horizontal direction and 0 to 300 cm in vertical direction. Underlying measurements are shown in the lower plot, which illustrates occurrences of specific ambient light intensities. Darker colors in the upper plot indicate a higher occurrence rate. It is shown a subject body and head being scaled to the dimensions of the two upper plots. Highlighted zones (dashed ovals) in the plots are shown starting from the left: a laptop area and a television screen. The zoomed-in diagram on the right-hand-side illustrates further results of the patient and his preferred activities during an office day. As can be seen therefrom, the most occurrences happened within a short range of viewing distances and thus in near vision, for example when the patient was using his laptop or the like. In the specific example of Figure 4, 41% of the occurrences happened in near vision. Less occurrences happened in an intermediate range (intermediate vision), for example when the patient had conversations with others, and the least occurrences happened in a far range (far vision), for example when the patient was looking out of a window in front.

[0062] The occurrence diagram down below schematically illustrates occurrences of specific ambient light during the activities of using a laptop and watching TV. The distance map and the occurrences diagram build the foundation for the illustrated results shown in figures 11 and 12.

[0063] Figure 5 schematically illustrates another two dimensional distance distribution when the patient was wearing the distance measuring system 1 of Figure 1 at home. The left diagram illustrates distances in horizontal direction from 0 to 600 cm and 0 to 300 cm in vertical direction. The right diagram illustrates a zoomed-in diagram with preferred activities of the patient shown with dashed ovals. From left to right areas correspond to desktop work, reading and computer screen, respectively. The probability of tasks performed often is highlighted in

a darker black colour, wherein light colour indicates tasks performed less often.

[0064] Figure 6 schematically illustrates distance occurrences over ambient light obtained by the distance measuring system 1 with the optional ambient light sensor 25 according to Figure 1. Information about the ambient light can be considered to weight distance occurrences. Illumination conditions, e.g. the ambient light and/or light intensities occurring during different activities, in different times of day can influence the size of the pupil and thus modify the vision requirements. Moreover, the information about the ambient light can be used for weighting or discarding measured viewing distances to get a more profound analysis of the statistical distribution of measured viewing distances. The subject's activities reflect daily exposures to different ambient lights in association with the measured viewing distances. This additional measurement provides a more robust objective solution to a patient's daily accommodation needs. For example, two patients may need the same distance accommodation, but are exposed by different ambient light throughout a daily routine, which will lead to different overall refractive requirements for both patients.

[0065] Figure 7 schematically illustrates a scenario of a patient wearing glasses to which the distance measuring system 1 of Figure 1 is attached or which comprise the distance measuring system 1 of Figure 1. The distance measuring system 1 may be implemented as a distance measuring device having a range distance sensor in Figure 7. The patient looks in a gaze direction, wherein the sensor is sensitive to this gaze direction. This is illustrated in a top view and a side view illustrating the sensor sensitivity in a direction of the sensing area corresponding to the patient's viewing direction. The distance measuring device having the distance measuring sensor moves with the movement of the patient's head. Thus, every distance in the line of the patient's head direction can be sampled. Additional sensors comprised in the distance measuring system 1 help to concentrate the gathered information about the measured viewing distances to only the most important distances, which are to be considered in the final statistical distribution. The final statistical distribution indicates the measured viewing distances which occurred most often and neglects measured viewing distances which were found to be negligible. Therefore, a surgeon is able to make a profound choice of a refractive correction applied to an artificial lens together with the patient.

[0066] Figure 8 schematically shows an illustration of the time history of a refraction requirements distribution (upper plot) and ambient light distribution (lower plot) in accordance with the acquired data of figure 3, which was acquired over time, whereby figure 8 illustrates data over a time axis. Darker colors indicate a higher occurrence rate. Typical office time is shown. Periods of the desktop monitor with refraction between -2 and -1 diopters are shown. Lunch time between 12:45 and 13:30 shows broader distribution of larger distances (smaller refrac-

tion). Desktop work (16:20 till 17:15) is observed as period with shorter distances (larger refraction).

[0067] Figure 9 illustrates four different exemplary refractive requirements diagrams derived by way of the distance measuring system 1 of Figure 1. The different exemplary refractive requirements diagrams are assigned to specific contexts. For example, when a patient uses a PC, the refraction requirement is lower in magnitude than the refraction requirement for reading, but higher than the refraction requirement for watching TV or playing golf. The refraction requirements of the specific activities can then be integrated into a combined diagram based on the patient's individual preferences, wishes and/or time spent in specific activities. In this way the patient is able to prioritise or deprioritise certain activities and with this feature he is able to adjust a weight of contribution to the overall statistics. For example, the patient might prefer to elevate activities, where dependence on glasses would be a higher burden, for example, when it is accompanied by a physical activity. In contrast, the patient might be willing to depreciate activities, where vision quality is not critical, even when he or she is spending significant amount of time in this activity. The refractive target can be individualised in such manner according to an interview between the patient and the doctor before the surgery and then be used for the selection of an IOL type and specific parameters. Such individual tuning is not possible when the overall statistics are estimated purely on the time basis and thus without stratification of data based on the activities.

[0068] Figure 10 schematically illustrates refraction requirements and mean light intensities associated with refraction, calculated from the distance measurements illustrated on figure 4. The peak at refraction -2D corresponds to usage of a laptop computer, which might be considered the most preferred distance of this specific subject.

[0069] Further considerations for manufacturing an artificial lens may be extracted by using the following diagrams of figure 11.

[0070] Figure 11 schematically illustrates possible solutions for a realization of optimal refraction requirements extracted from figure 4 and 10 respectively. This realisation of optimal refraction requirements curves are based on the through-focus curves (TFC) of intraocular lenses, which are shown from Left-to-right. The first diagram on the left below illustrates a diagram for a multifocal IOL, whereby both eyes (OD and OS) are getting an implant which considers both maximum refractive corrections of -2D and 0D. The second diagram in the middle below illustrates a diagram for two monofocal lenses, wherein one eye (OD) is getting an implant of a monofocal lens matching the -2D target, while the other (OS) is getting an implant of a monofocal lens matching the 0D target. The 0D target corresponds to a plano lens with 0 diopters to match distance vision, the so called monovision. The third diagram on the right below illustrates a diagram for two monofocal lenses, wherein one eye (OD) is getting

an implant of a monofocal lens as in the second diagram, while the other eye (OS) is getting an implant of a lens with an extended depth of field between -2 and 0 diopters. The statistical distribution determined herein enables a medical professional to determine a well-suited monofocal IOL or an even better suited multifocal IOL.

[0071] Figure 12 schematically illustrates a prioritization mechanism of prioritized viewing distances. An occurrence diagram, a priority diagram and a refraction need diagram are shown. The refraction need diagram is derived from the combination of the priority diagram and the refraction need diagram. In the occurrence diagram the peak around -2D (reading) is elevated based on a prioritization feedback shown in the refraction need diagram below the occurrence diagram, while a peak around -0.7D (TV), which was deprioritized based on the patient feedback, is reduced in the final refraction need diagram. Therefore, a better solution for an artificial lens can be found by introduction of a specific prioritization, wherein the circumstances for prioritization can be different for each individual.

[0072] By way of the technique described herein, customised ablation profiles can be determined. Current refractive lasers are considering current refractive power (and/or the corneal radius of curvature - corneal power and/or total wavefront aberrations of the eye) and target refractive power and estimate the ablation profile based on the difference. The technique described herein enables to calculate a customised ablation profile in order to realise the desired vision performance of the eye. For example, this could be an extended depth of field. Thus, the measurements described herein can serve as an input to the calculation of ablation profiles to realise required optical power and depth of field.

Claims

1. A distance measuring system (1) adapted to be mounted on glasses, spectacles' frame and/or adapted to be attached to a subject's head comprising:

a distance measuring sensor (5) adapted and arranged to measure viewing distances between eyes of the subject and one or more objects;

a memory unit (7) adapted to store the measured viewing distances in a set of measured viewing distances;

a movement sensor (20) adapted and arranged to measure movements of the subject's head, and a processing unit (10) adapted to determine a statistical distribution of the measured viewing distances from the set of measured viewing distances, and wherein the processing unit is further adapted to statistically weight, select or discard the measured viewing distances from the

set of measured viewing distances based on the measured movements.

2. The distance measuring system (1) according to claim 1, further comprising:
an eye monitoring unit (15) adapted and arranged to detect the subject's eye direction relative to the distance measuring sensor's (5) viewing direction, wherein the processing unit (10) is further adapted to statistically weight, select or discard the measured viewing distances from the set of measured viewing distances based on the subject's eye direction relative to the distance measuring sensor's (5) viewing direction. 5
3. The distance measuring system (1) according to claims 1 or 2, wherein the movement sensor (20) is an accelerometer, a gyroscope or a magnetometer. 10
4. The distance measuring system (1) according to any of claims 1 to 3, further comprising:
an ambient light sensor (25) adapted and arranged to measure ambient light, light intensity and/or spectral content in the distance measuring sensor's (5) viewing direction, wherein the processing unit (10) is further adapted to statistically weight, select or discard the measured viewing distances from the set of measured viewing distances based on the measured ambient light, light intensity and/or spectral content. 15
5. The distance measuring system (1) according to any of claims 1 to 4, further comprising:
a user interface (30) adapted to receive a user input, wherein the processing unit (10) is further adapted to weight, select or discard the measured viewing distances from the set of measured viewing distances based on the user input. 20
6. The distance measuring system (1) according to any of claims 1 to 5, wherein the processing unit (10) is further adapted to calculate a target refraction by applying a statistical method to the statistical distribution of the measured viewing distances. 25
7. Use of the distance measuring system (1) according to any of claims 1 to 6 for selection and customisation of a refractive solution. 30
8. A distance measuring method comprising the steps of: 35

measuring (S10) viewing distances, by a distance measuring sensor (5) of a distance measuring system (1), between eyes of a subject and one or more objects, wherein the distance measuring system (1) is adapted to be mounted on glasses, spectacles' frame and/or adapted to be 40

attached to the subject's head;
storing (S7), by a memory unit (7), the measured viewing distances in a set of measured viewing distances;
measuring (S20), by a movement sensor (20) of the distance measuring system (1), movements of the subject's head;
statistically weighting, selecting or discarding (S21), by a processing unit (10), the measured viewing distances from the set of measured viewing distances based on the measured movements; and
determining (S11), by the processing unit (10) of the distance measuring system (1), a statistical distribution of the measured viewing distances from the set of measured viewing distances. 45

9. The method according to claim 8, further comprising:

detecting (S15), by an eye monitoring unit (15) of the distance measuring system (1), the subject's eye viewing direction relative to the distance measuring sensor's (5) viewing direction; and
statistically weighting, selecting or discarding (S16), by the processing unit (10), the measured viewing distances from the set of measured viewing distances based on the subject's eye direction relative to the distance measuring sensor's (5) viewing direction. 50

10. The method according to any of claims 8 to 9, further comprising:

measuring (S25), by an ambient light sensor (25), ambient light, light intensity and/or spectral content in the distance measuring sensor's (5) viewing direction; and
statistically weighting, selecting or discarding (S26), by the processing unit (10), the measured viewing distances from the set of measured viewing distances based on the measured ambient light, light intensity and/or spectral content. 55

11. The method according to any of claims 8 to 10, further comprising:

receiving (S30), by a user interface (30) of the distance measuring system (1), a user input; and
weighting, selecting or discarding (S31), by the processing unit (10), the measured viewing distances from the set of measured viewing distances based on the user input. 60

12. The method according to any of claims 8 to 11, further comprising:
calculating (S35), by the processing unit (10), a tar-

get refraction by applying a statistical method to the statistical distribution of the measured viewing distances.

13. The method according to any of claims 8 to 12, wherein the method is performed before or after cataract or refractive surgery, or before, during or after contact lens or spectacle fitting.

Patentansprüche

1. Entfernungsmesssystem (1), das an einer Brille, einem Brillengestell und/oder an einem Kopf eines Probanden anbringbar ist, und folgendes umfasst:

einen Entfernungsmesssensor (5), der ausgebildet und angeordnet ist, Betrachtungsentfernungen zwischen Augen des Probanden und einem oder mehreren Objekten zu messen;
eine Speichereinheit (7), die ausgebildet ist, die gemessenen Betrachtungsentfernungen in einem Satz gemessener Betrachtungsentfernungen zu speichern;
einen Bewegungssensor (20), der ausgebildet und angeordnet ist, Bewegungen des Kopfes des Probanden zu messen; und
eine Verarbeitungseinheit (10), die ausgebildet ist, eine statistische Verteilung der gemessenen Betrachtungsentfernungen von dem Satz gemessener Betrachtungsentfernungen zu bestimmen, und wobei die Verarbeitungseinheit ferner ausgebildet ist, die gemessenen Betrachtungsentfernungen von dem Satz gemessener Betrachtungsentfernungen basierend auf den gemessenen Bewegungen statistisch zu gewichten, auszuwählen oder zu verwerfen.

2. Entfernungsmesssystem (1) nach Anspruch 1, ferner umfassend:

eine Augenüberwachungseinheit (15), die ausgebildet und angeordnet ist, die Blickrichtung des Probanden relativ zur Betrachtungsrichtung des Entfernungsmesssensors (5) zu erfassen, wobei die Verarbeitungseinheit (10) ferner ausgebildet ist, die gemessenen Betrachtungsentfernungen von dem Satz gemessener Betrachtungsentfernungen basierend auf der Blickrichtung des Probanden relativ zur Betrachtungsrichtung des Entfernungsmesssensors (5) statistisch zu gewichten, auszuwählen oder zu verwerfen.

3. Entfernungsmesssystem (1) nach Anspruch 1 oder 2, wobei der Bewegungssensor (20) ein Beschleunigungsmesser, ein Kreisel oder ein Magnetometer ist.

4. Entfernungsmesssystem (1) nach einem der An-

sprüche 1 bis 3, ferner umfassend:

einen Umgebungslichtsensor (25), der ausgebildet und angeordnet ist, Umgebungslicht, Lichtintensität und/oder Spektralgehalt in Betrachtungsrichtung des Entfernungsmesssensors (5) zu messen, wobei die Verarbeitungseinheit (10) ferner ausgebildet ist, die gemessenen Betrachtungsentfernungen von dem Satz gemessener Betrachtungsentfernungen basierend auf dem gemessenen Umgebungslicht, der Lichtintensität und/oder dem Spektralgehalt statistisch zu gewichten, auszuwählen oder zu verwerfen.

5. Entfernungsmesssystem (1) nach einem der Ansprüche 1 bis 4, ferner mit:

eine Benutzerschnittstelle (30), die ausgebildet ist, eine Benutzereingabe zu empfangen, wobei die Verarbeitungseinheit (10) ferner ausgebildet ist, die gemessenen Betrachtungsentfernungen aus dem Satz gemessener Betrachtungsentfernungen basierend auf der Benutzereingabe zu gewichten, auszuwählen oder zu verwerfen.

6. Entfernungsmesssystem (1) nach einem der Ansprüche 1 bis 5, wobei die Verarbeitungseinheit (10) ferner ausgebildet ist, eine Zielrefraktion zu berechnen, indem eine statistische Methode auf die statistische Verteilung der gemessenen Betrachtungsentfernungen angewendet wird.

7. Verwendung des Entfernungsmesssystems (1) nach einem der Ansprüche 1 bis 6 zur Auswahl und Anpassung einer refraktiven Lösung.

8. Entfernungsmessverfahren, umfassend die Schritte:

Messen (S10) von Betrachtungsentfernungen, durch einen Entfernungsmesssensor (5) eines Entfernungsmesssystems (1), zwischen Augen eines Probanden und einem oder mehreren Objekten, wobei das Entfernungsmesssystem (1) an einer Brille, einem Brillengestell und/oder an einem Kopf eines Probanden anbringbar ist;
Speichern (S7), durch eine Speichereinheit (7), der gemessenen Betrachtungsentfernungen in einem Satz gemessener Betrachtungsentfernungen;
Messen (S20), durch einen Bewegungssensor (20) des Entfernungsmesssystems (1), von Bewegungen eines Kopfes des Probanden;
statistisches Gewichten, Auswählen oder Verwerfen (S21), durch eine Verarbeitungseinheit (10), der gemessenen Betrachtungsentfernungen von dem Satz gemessener Betrachtungsentfernungen basierend auf den gemessenen Bewegungen; und

Bestimmen (S11), durch die Verarbeitungseinheit (10) des Entfernungsmesssystems (1), einer statistischen Verteilung der gemessenen Betrachtungsentfernungen von dem Satz gemessener Betrachtungsentfernungen.

9. Verfahren nach Anspruch 8, ferner umfassend:

Ermitteln (S15), durch eine Augenüberwachungseinheit (15) des Entfernungsmesssystems (1), der Blickrichtung des Probanden relativ zur Betrachtungsrichtung des Entfernungsmessensors (5); und
Statistisches Gewichten, Auswählen oder Verwerfen (S16), durch die Verarbeitungseinheit (10), der gemessenen Betrachtungsentfernungen von dem Satz gemessener Betrachtungsentfernungen basierend auf der Blickrichtung des Probanden relativ zur Betrachtungsrichtung des Entfernungsmessensors (5).

10. Verfahren nach einem der Ansprüche 8 bis 9, ferner umfassend:

Messen (S25), durch einen Umgebungslichtsensor (25), von Umgebungslicht, Lichtintensität und/oder Spektralgehalt in Betrachtungsrichtung des Entfernungsmessensors (5); und
statistisches Gewichten, Auswählen oder Verwerfen (S26), durch die Verarbeitungseinheit (10), der gemessenen Betrachtungsentfernungen von dem Satz gemessener Betrachtungsentfernungen basierend auf dem gemessenen Umgebungslicht, der Lichtintensität und/oder des Spektralgehalts.

11. Verfahren nach einem der Ansprüche 8 bis 10, ferner umfassend:

Empfangen (S30), durch eine Benutzerschnittstelle (30) des Entfernungsmesssystems (1), einer Benutzereingabe; und
Gewichten, Auswählen oder Verwerfen (S31), durch die Verarbeitungseinheit (10), der gemessenen Betrachtungsentfernungen von dem Satz gemessener Betrachtungsentfernungen basierend auf der Benutzereingabe.

12. Verfahren nach einem der Ansprüche 8 bis 11, ferner umfassend:

Berechnen (S35) durch die Verarbeitungseinheit (10) einer Zielrefraktion durch Anwenden eines statistischen Verfahrens auf die statistische Verteilung der gemessenen Betrachtungsentfernungen.

13. Verfahren nach einem der Ansprüche 8 bis 12, wobei das Verfahren vor oder nach einer Katarakt- oder refraktiven Operation oder vor, während oder nach

einer Kontaktlinsen- oder Brillenanpassung durchgeführt wird.

5 Revendications

1. Système de mesure de distance (1) adapté pour être monté sur des lunettes, une monture de lunettes et/ou adapté pour être fixé à la tête d'un sujet comprenant :

un capteur de mesure de distance (5) adapté et agencé pour mesurer des distances de visualisation entre les yeux du sujet et un ou plusieurs objets ;
une unité de mémoire (7) adaptée pour stocker les distances de visualisation mesurées dans un ensemble de distances de visualisation mesurées ;
un capteur de mouvement (20) adapté et agencé pour mesurer des mouvements de la tête du sujet, et une unité de traitement (10) adaptée pour déterminer une distribution statistique des distances de visualisation mesurées à partir de l'ensemble de visualisations mesurées, et dans lequel l'unité de traitement est en outre adaptée pour statistiquement pondérer, sélectionner ou éliminer les distances de visualisation mesurées à partir de l'ensemble de distances de visualisation mesurées sur la base des mouvements mesurés.

2. Système de mesure de distance (1) selon la revendication 1, comprenant en outre :

une unité de surveillance d'oeil (15) adaptée et agencée pour détecter la direction de l'œil du sujet par rapport à la direction de visualisation du capteur de mesure de distance (5), dans lequel l'unité de traitement (10) est en outre adaptée pour statistiquement pondérer, sélectionner ou éliminer les distances de visualisation mesurées à partir de l'ensemble de distances de visualisation mesurées sur la base de la direction de l'œil du sujet par rapport à la direction de visualisation du capteur de mesure de distance (5).

3. Système de mesure de distance (1) selon les revendications 1 ou 2, dans lequel le capteur de mouvement (20) est un accéléromètre, un gyroscope ou un magnétomètre.

4. Système de mesure de distance (1) selon l'une quelconque des revendications 1 à 3, comprenant en outre :

un capteur de lumière ambiante (25) adapté et agencé pour mesurer la lumière ambiante, l'intensité lumineuse et/ou le contenu spectral dans la direction de visualisation du capteur de mesure de distance

(5), dans lequel l'unité de traitement (10) est en outre adaptée pour statistiquement pondérer, sélectionner ou éliminer les distances de visualisation mesurées à partir de l'ensemble de distances de visualisation mesurées sur la base de la lumière ambiante, de l'intensité lumineuse et/ou du contenu spectral mesurés.

5. Système de mesure de distance (1) selon l'une quelconque des revendications 1 à 4, comprenant en outre :

une interface utilisateur (30) adaptée pour recevoir une entrée utilisateur, dans lequel l'unité de traitement (10) est en outre adaptée pour pondérer, sélectionner ou éliminer les distances de visualisation mesurées à partir de l'ensemble de distances de visualisation mesurées sur la base de l'entrée utilisateur.

6. Système de mesure de distance (1) selon l'une quelconque des revendications 1 à 5, dans lequel l'unité de traitement (10) est en outre adaptée pour calculer une réfraction cible en appliquant un procédé statistique à la distribution statistique des distances de visualisation mesurées.

7. Utilisation du système de mesure de distance (1) selon l'une quelconque des revendications 1 à 6 pour la sélection et la personnalisation d'une solution de réfraction.

8. Procédé de mesure de distance comprenant les étapes consistant à :

mesurer (S10) des distances de visualisation, par un capteur de mesure de distance (5) d'un système de mesure de distance (1), entre les yeux d'un sujet et un ou plusieurs objets, dans lequel le système de mesure de distance (1) est adapté pour être monté sur des lunettes, une monture de lunettes et/ou adapté pour être fixé à la tête du sujet ;

stocker (S7), par une unité de mémoire (7), les distances de visualisation mesurées dans un ensemble de distances de visualisation mesurées ;

mesurer (S20), par un capteur de mouvement (20) du système de mesure de distance (1), des mouvements de la tête du sujet ;

statistiquement pondérer, sélectionner ou éliminer (S21), par une unité de traitement (10), les distances de visualisation mesurées à partir de l'ensemble de distances de visualisation mesurées sur la base des mouvements mesurés ; et déterminer (S11), par l'unité de traitement (10) du système de mesure de distance (1), une distribution statistique des distances de visualisation mesurées à partir de l'ensemble de distances de visualisation mesurées.

ces de visualisation mesurées.

9. Procédé selon la revendication 8, comprenant en outre les étapes consistant à :

détecter (S15), par une unité de surveillance de l'œil (15) du système de mesure de distance (1), la direction de visualisation de l'œil du sujet par rapport à la direction de visualisation du capteur de mesure de distance (5) ; et statistiquement pondérer, sélectionner ou éliminer (S16), par l'unité de traitement (10), les distances de visualisation mesurées à partir de l'ensemble de distances de visualisation mesurées sur la base de la direction de l'œil du sujet par rapport à la direction de visualisation du capteur de mesure de distance (5).

10. Procédé selon l'une quelconque des revendications 8 à 9, comprenant en outre les étapes consistant à :

mesurer (S25), par un capteur de lumière ambiante (25), la lumière ambiante, l'intensité lumineuse et/ou le contenu spectral dans la direction de visualisation du capteur de mesure de distance (5) ; et statistiquement pondérer, sélectionner ou éliminer (S26), par l'unité de traitement (10), les distances de visualisation mesurées à partir de l'ensemble de distances de visualisation mesurées sur la base de la lumière ambiante, de l'intensité lumineuse et/ou du contenu spectral mesurés.

11. Procédé selon l'une quelconque des revendications 8 à 10, comprenant en outre les étapes consistant à :

recevoir (S30), par une interface utilisateur (30) du système de mesure de distance (1), une entrée utilisateur ; et pondérer, sélectionner ou éliminer (S31), par l'unité de traitement (10), les distances de visualisation mesurées à partir de l'ensemble de distances de visualisation mesurées sur la base de l'entrée utilisateur.

12. Procédé selon l'une quelconque des revendications 8 à 11, comprenant en outre l'étape consistant à : calculer (S35), par l'unité de traitement (10), une réfraction cible en appliquant un procédé statistique à la distribution statistique des distances de visualisation mesurées.

13. Procédé selon l'une quelconque des revendications 8 à 12, dans lequel le procédé est réalisé avant ou après une chirurgie de la cataracte ou réfractive, ou avant, pendant ou après l'ajustement de lentilles de contact ou d'une monture de lunettes.

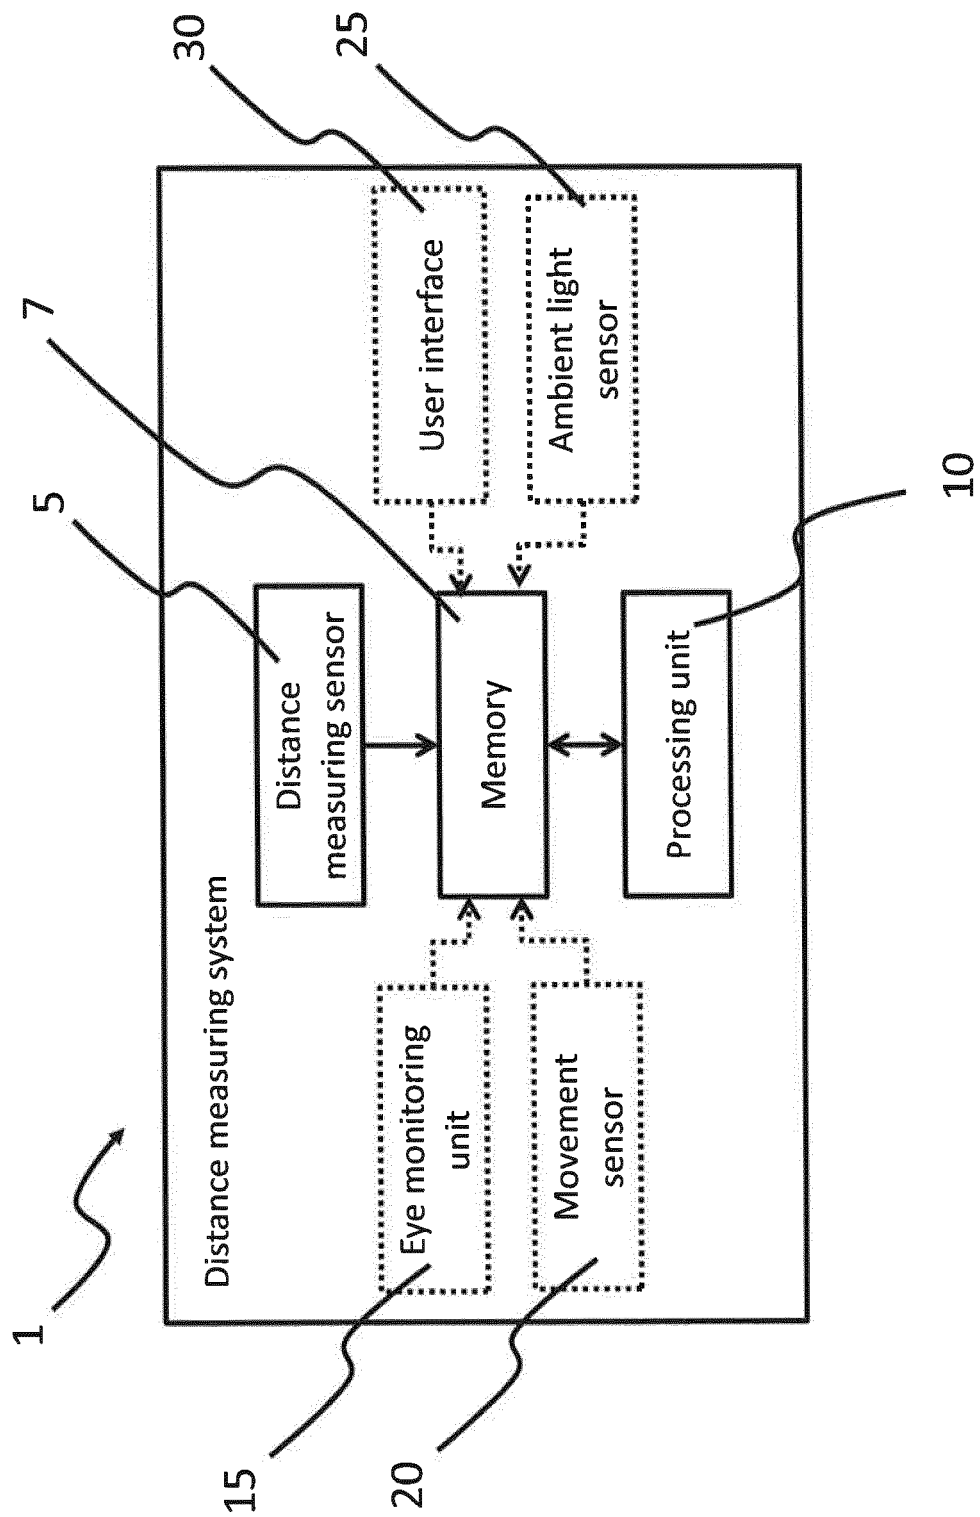


Fig.1

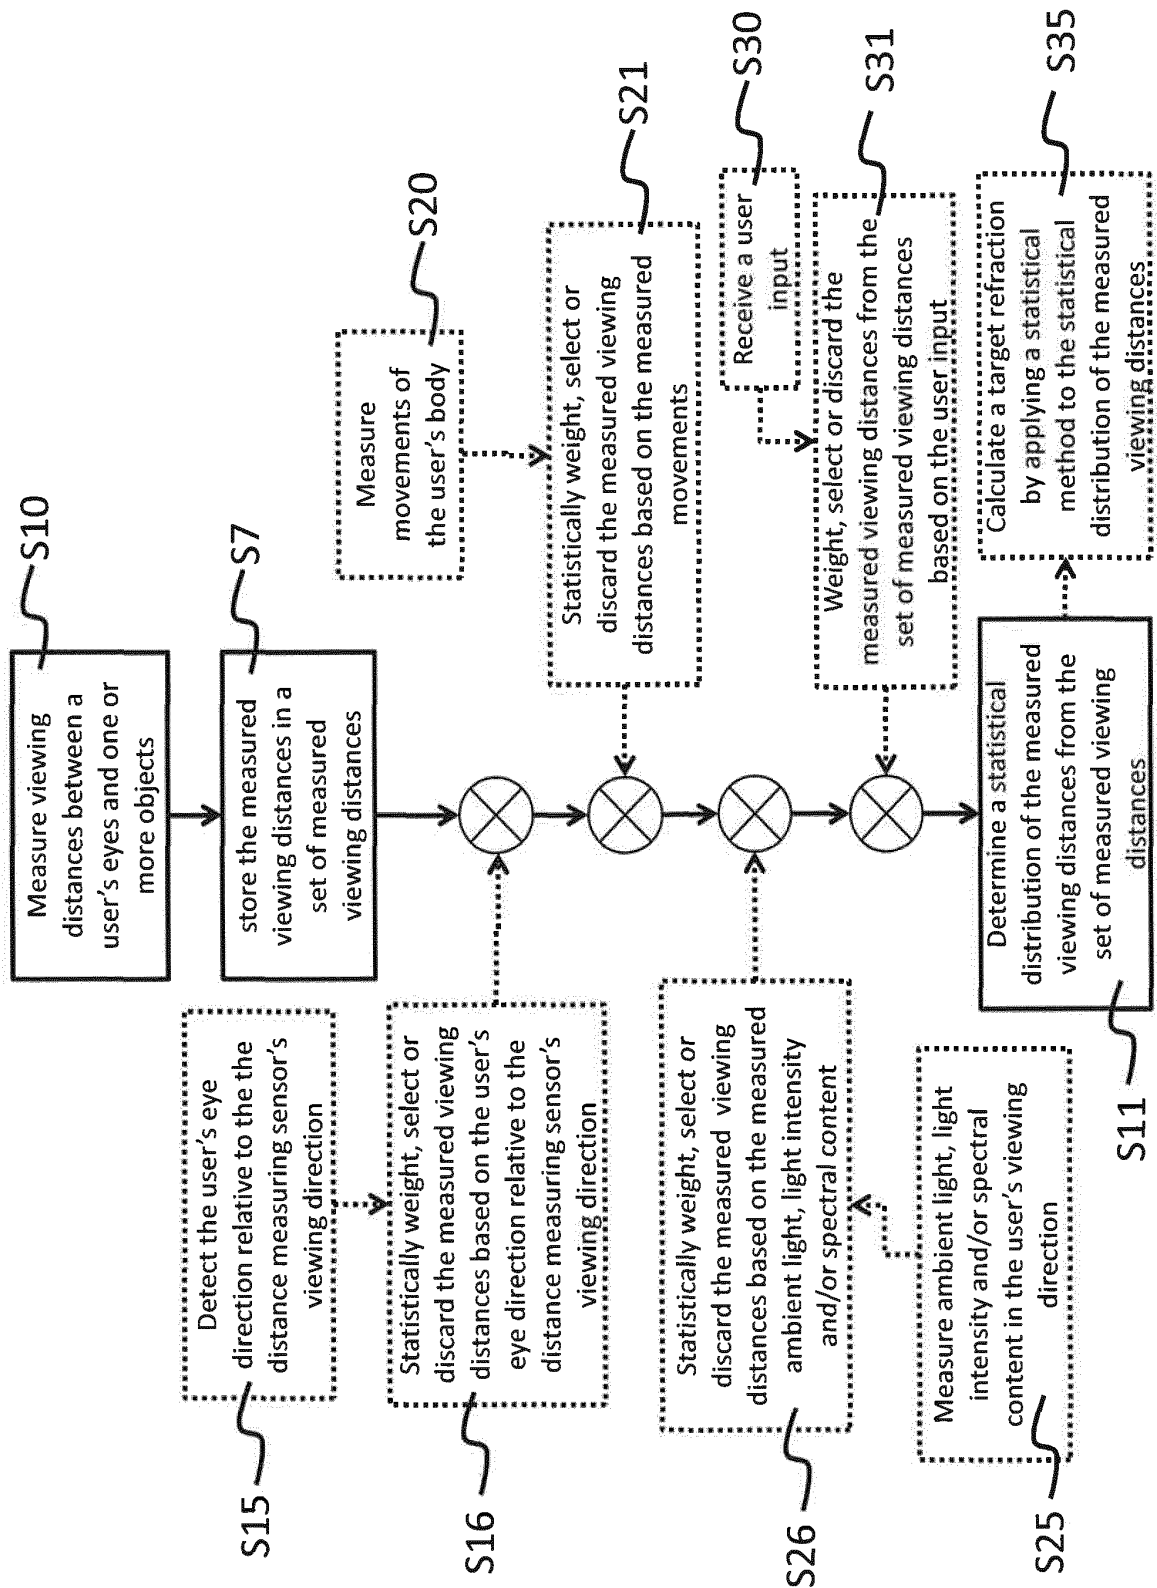


Fig.2

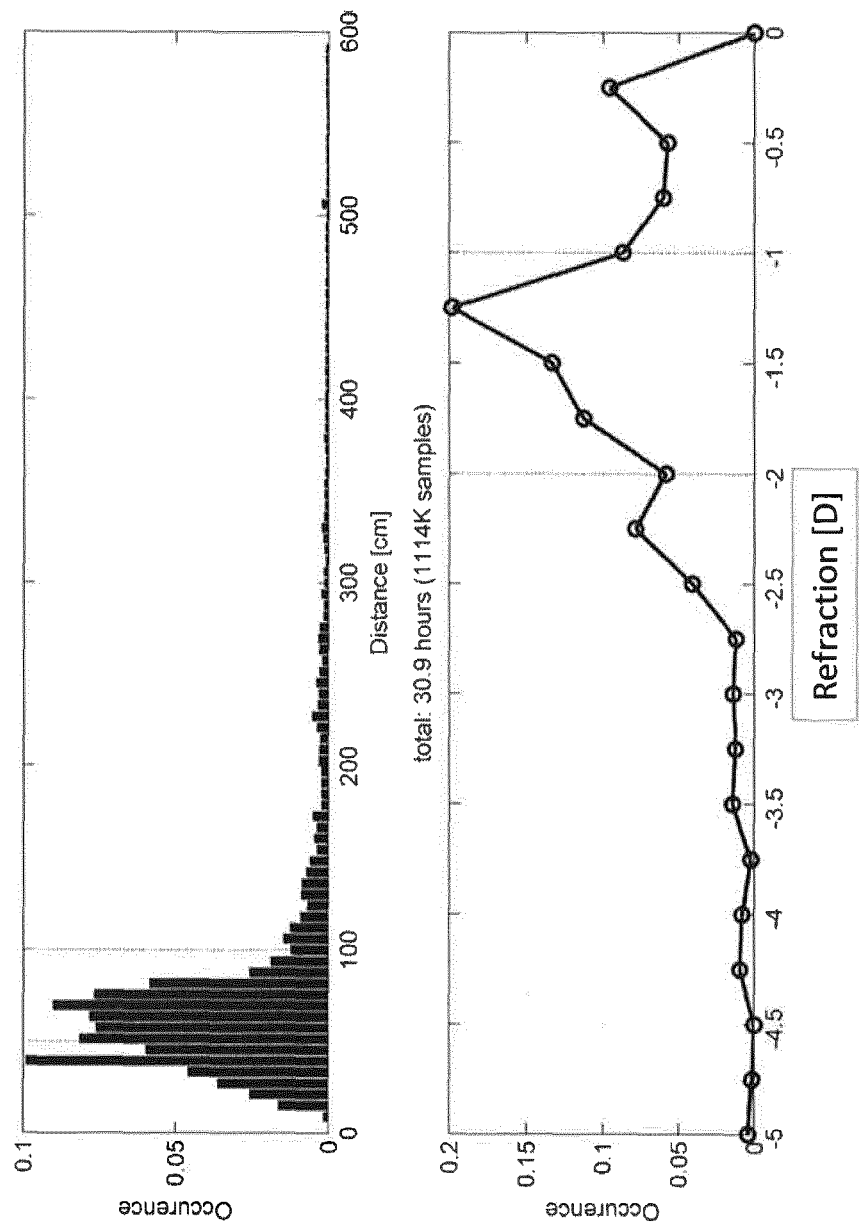


Fig.3

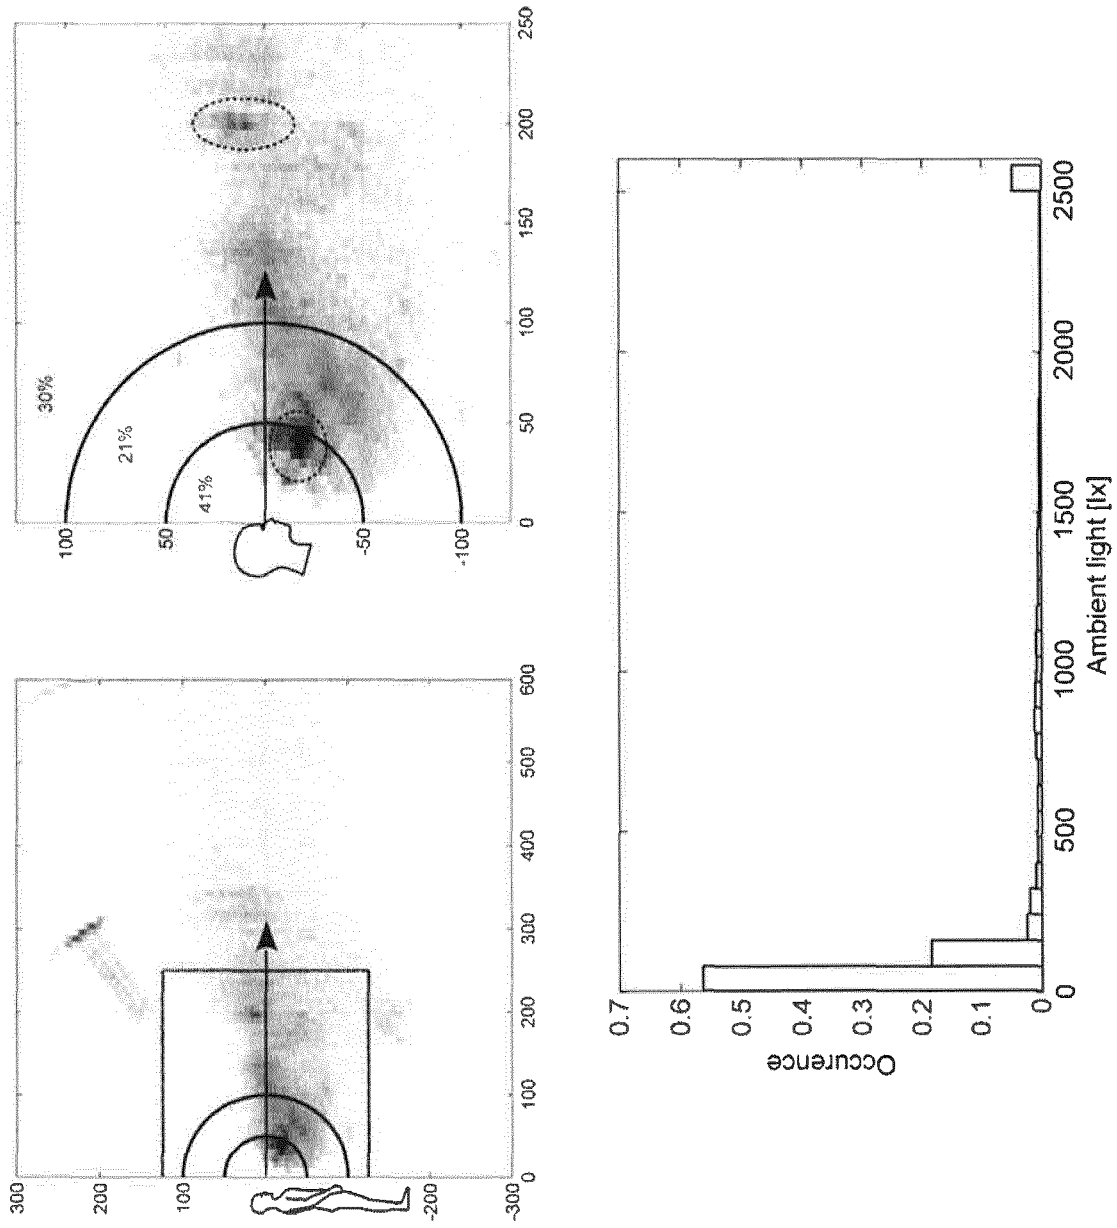


Fig.4

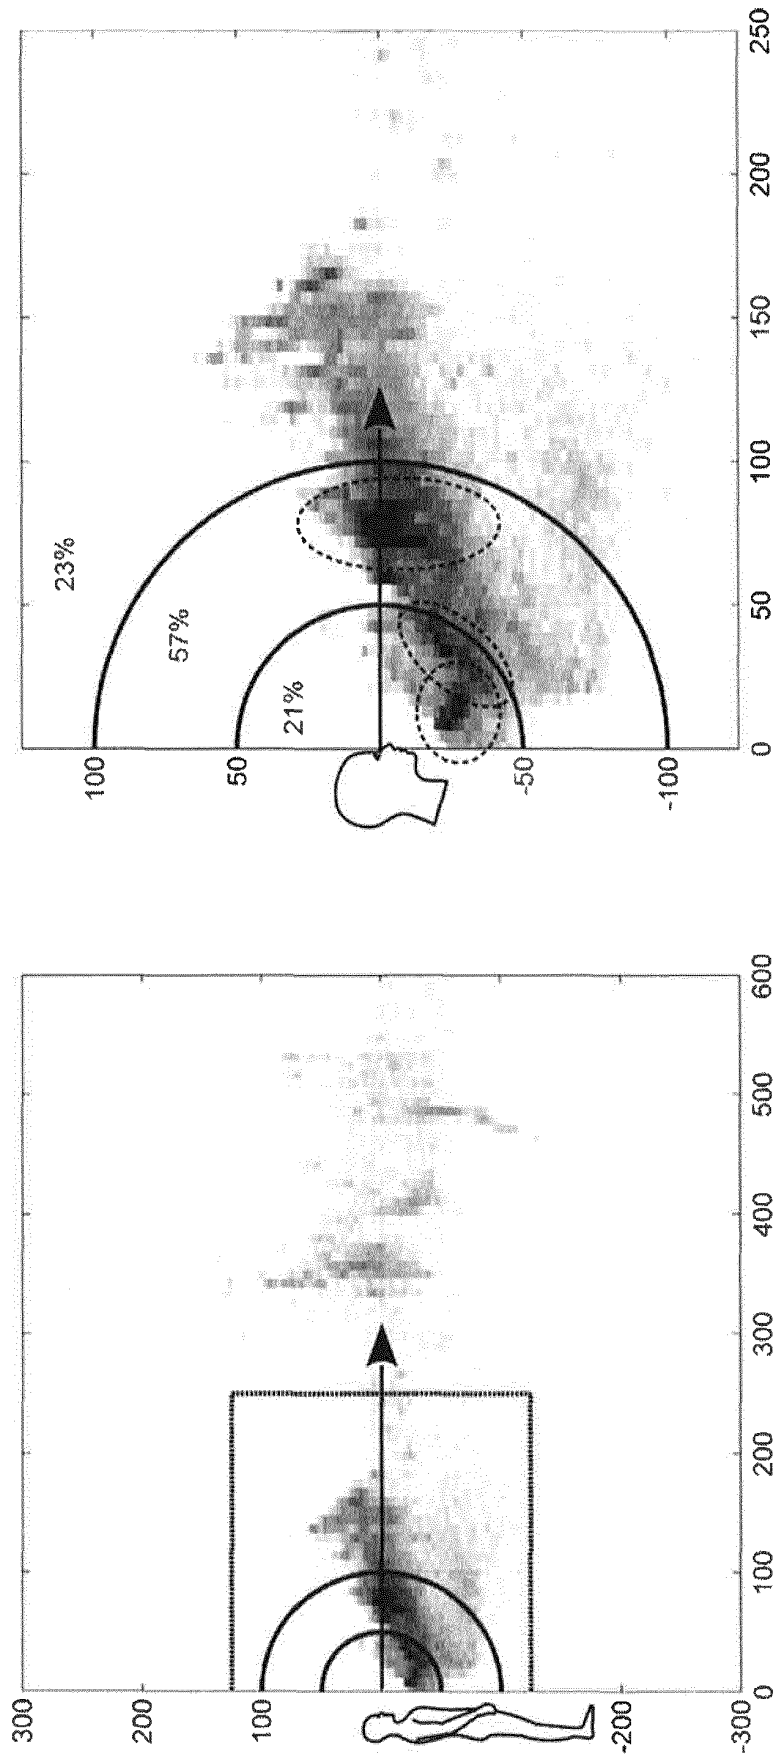


Fig.5

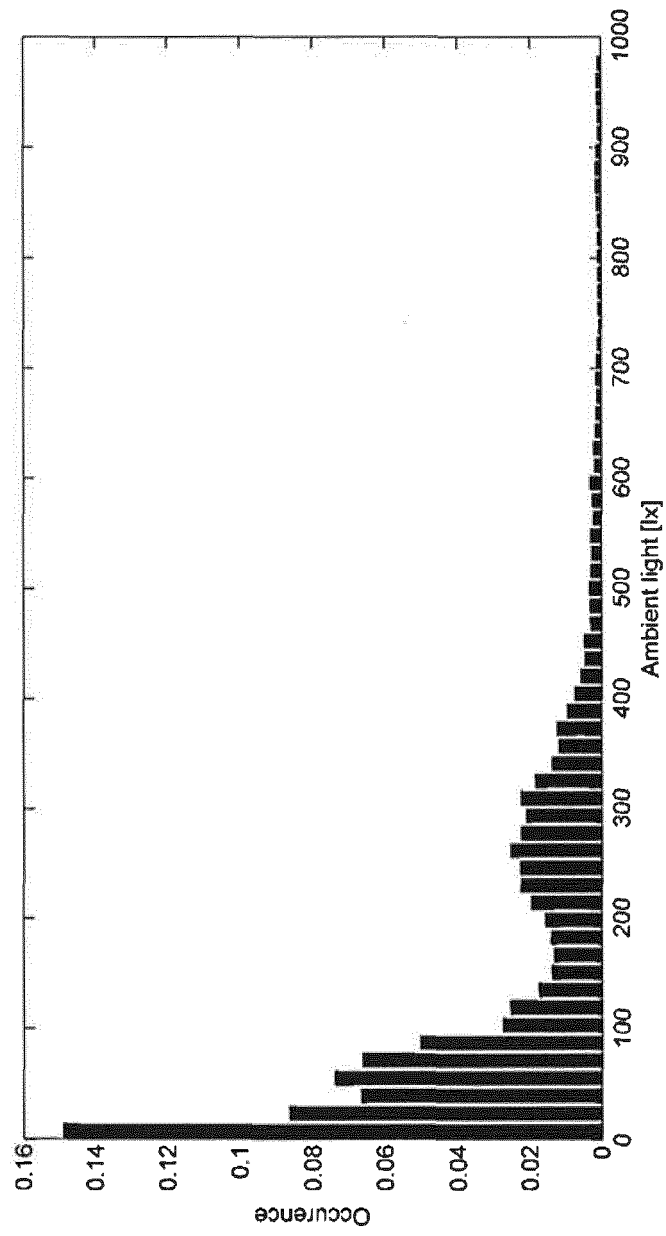


Fig.6

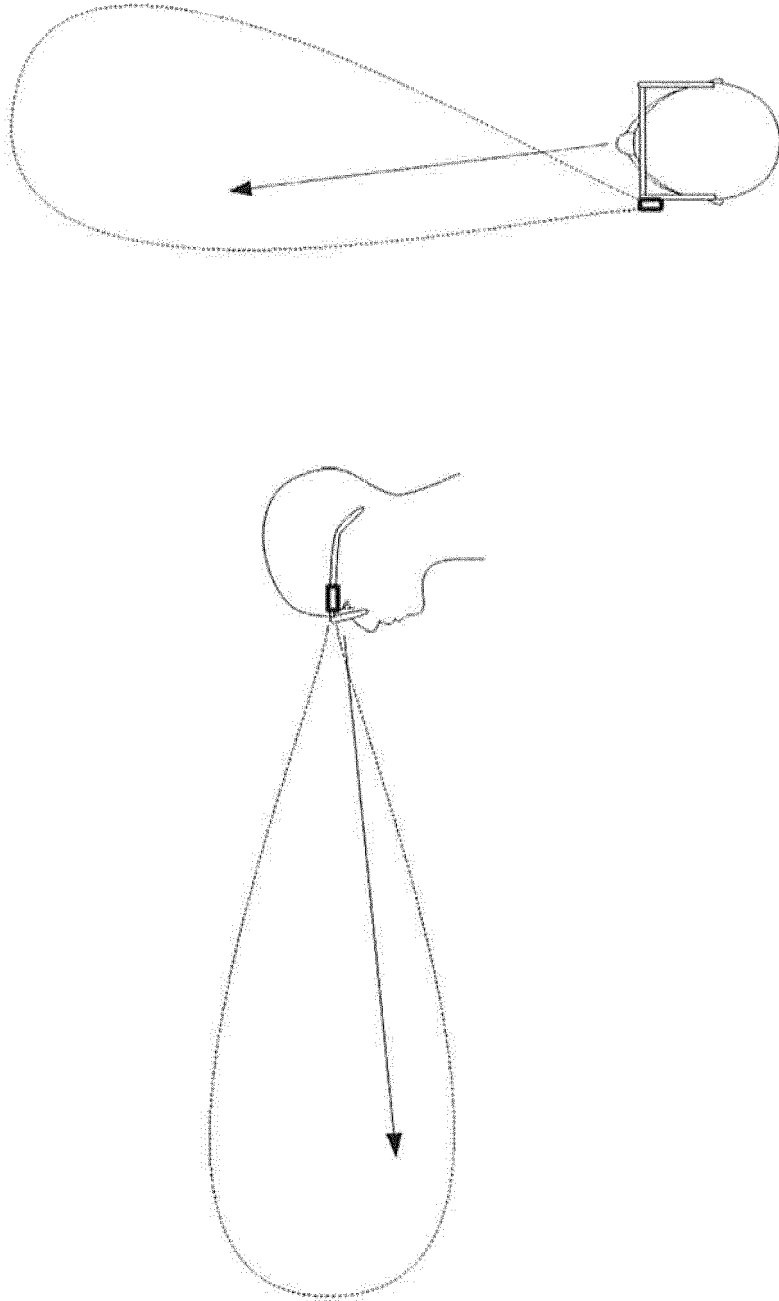


Fig.7

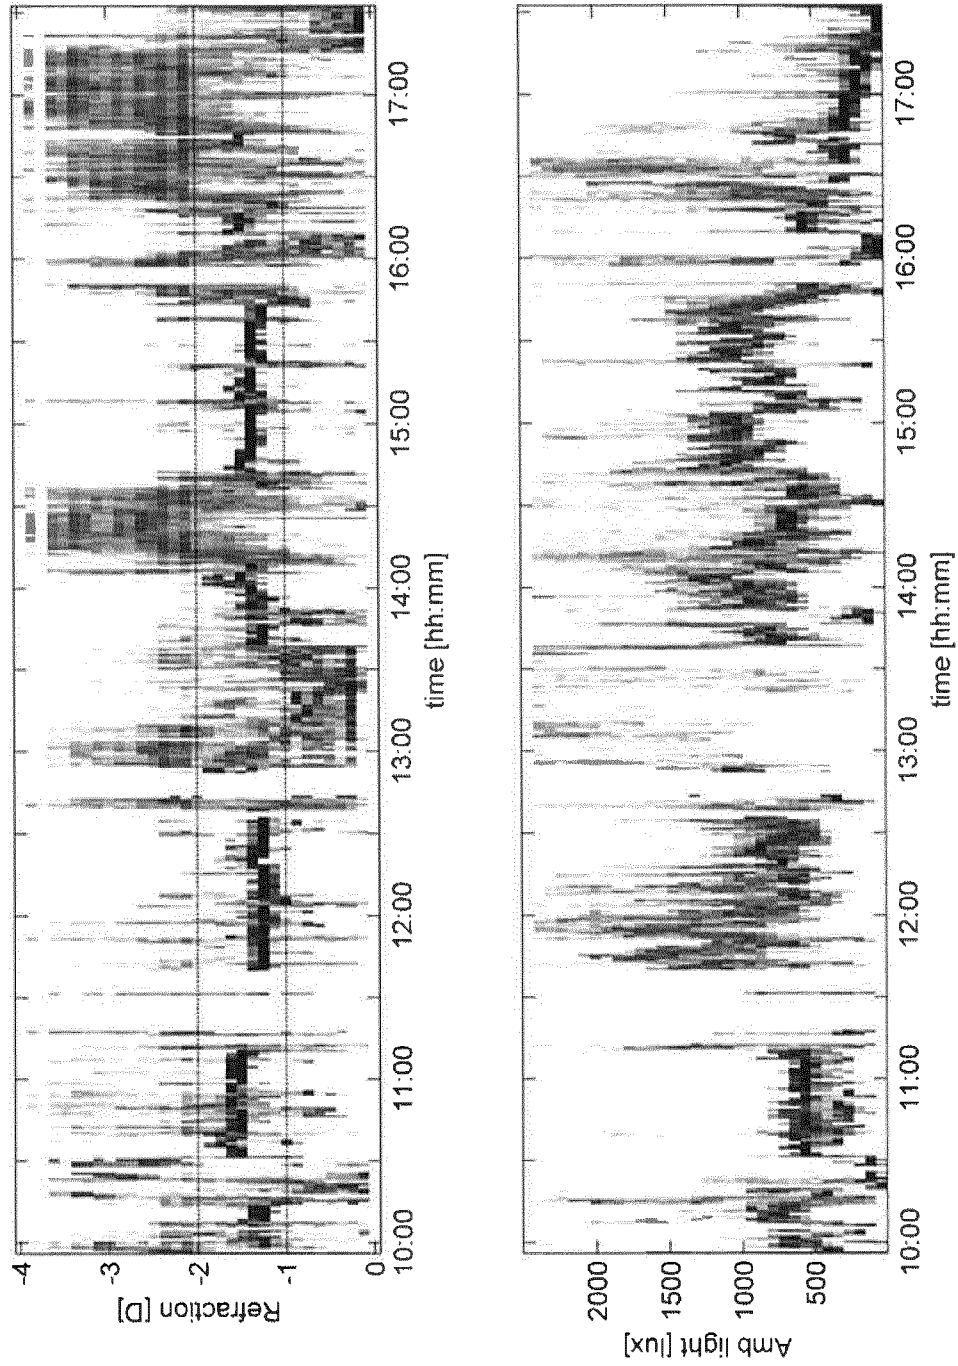


Fig.8

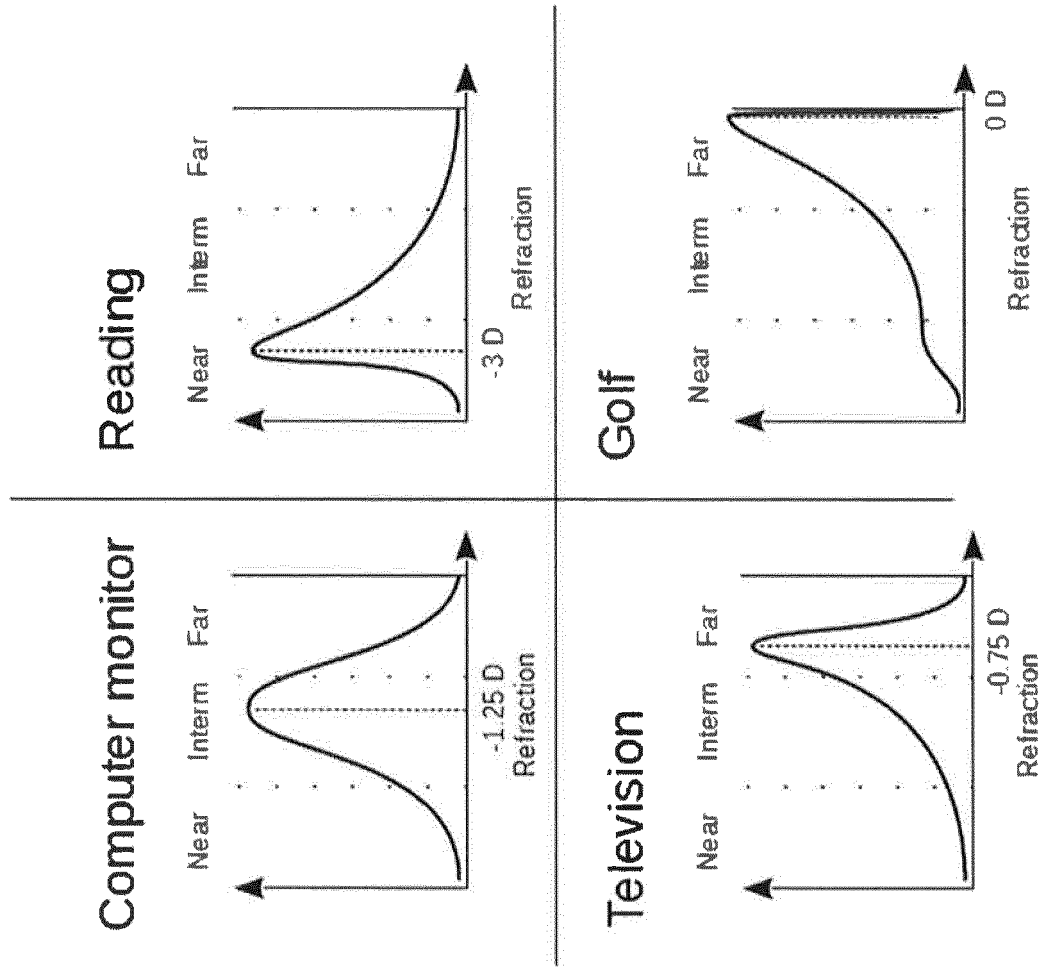


Fig.9

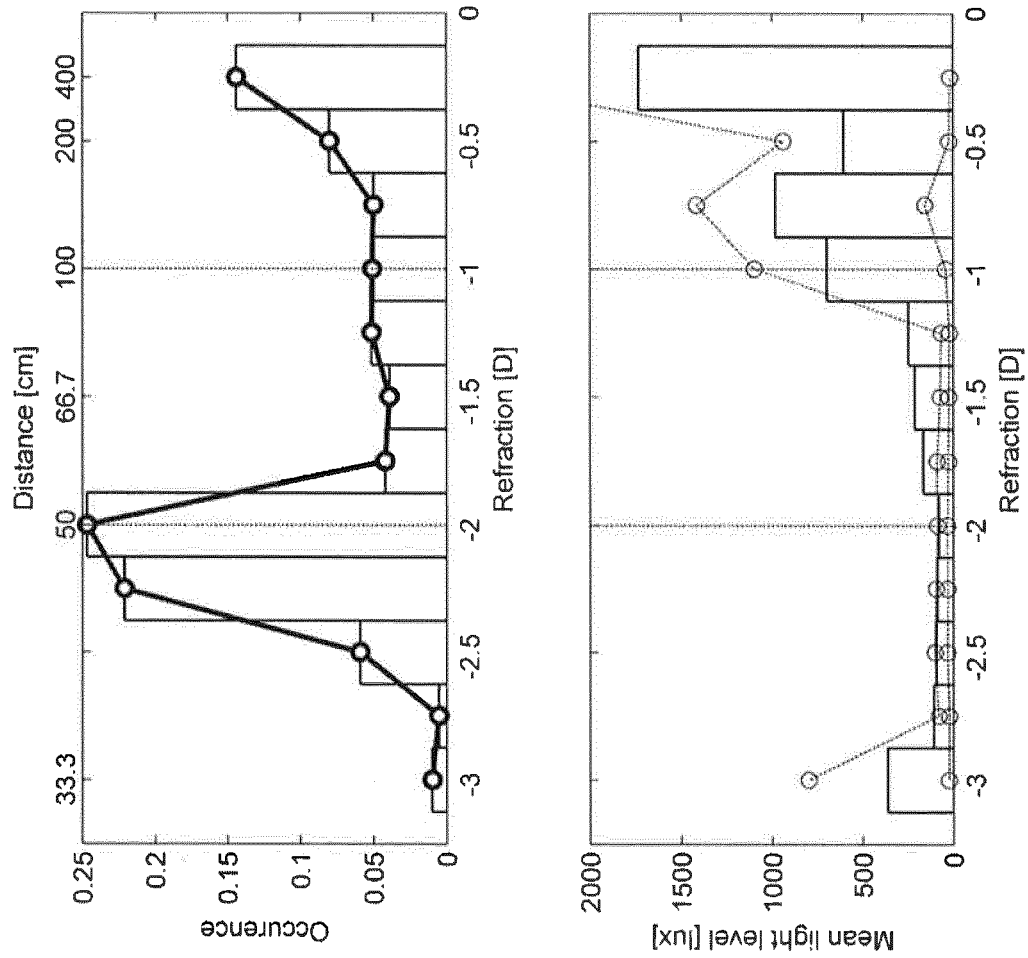


Fig.10

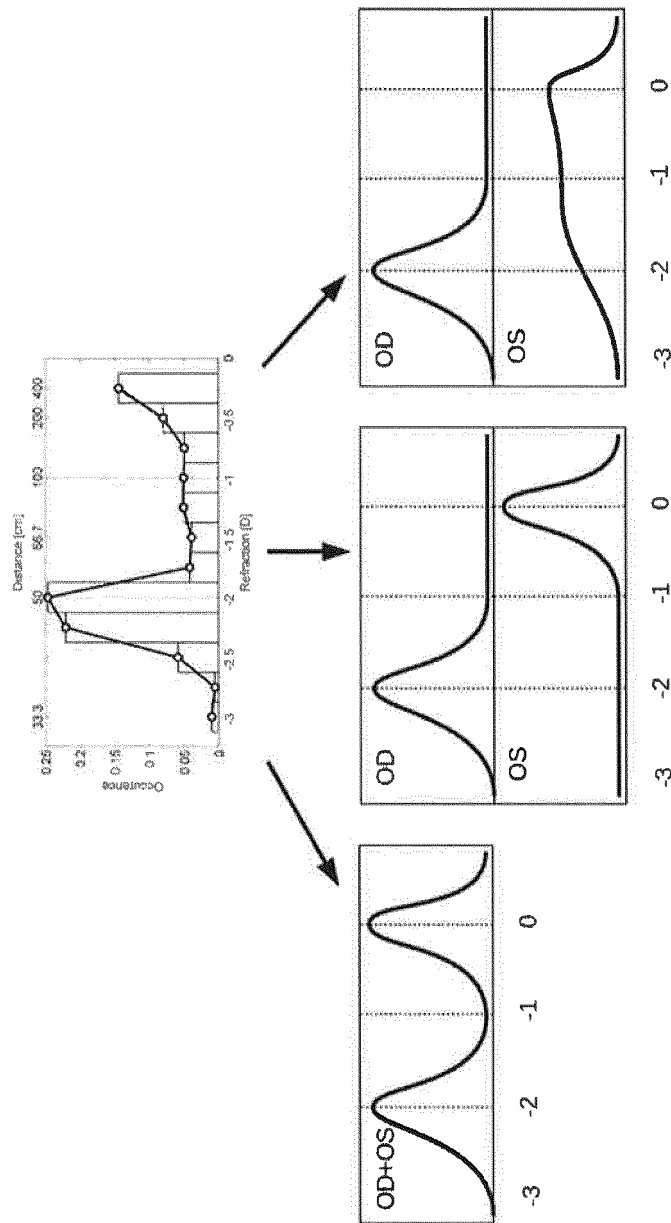


Fig.11

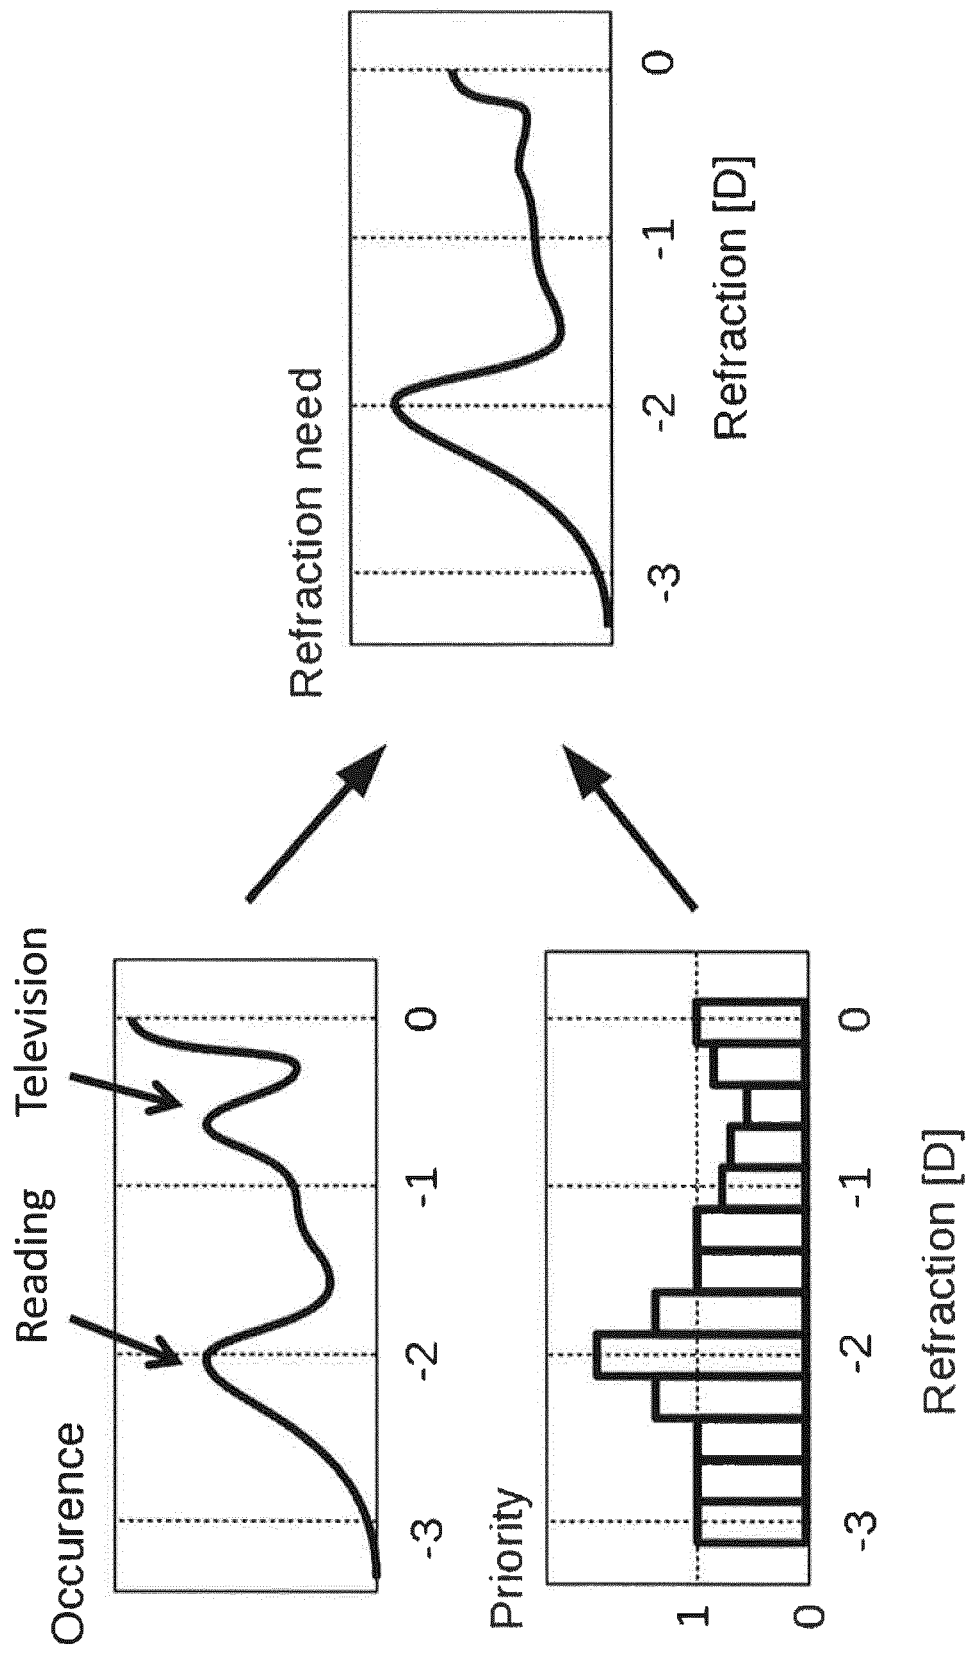


Fig.12

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- WO 2014179857 A [0006]

专利名称(译)	测量距离的装置和方法		
公开(公告)号	EP3228237B1	公开(公告)日	2019-12-25
申请号	EP2016164472	申请日	2016-04-08
[标]发明人	ZAKHAROV PAVEL MROCHEN MICHAEL		
发明人	ZAKHAROV, PAVEL MROCHEN, MICHAEL		
IPC分类号	A61B3/028 A61B3/09 A61B3/103 A61B5/00 A61B5/06 A61B5/107 A61B5/11		
CPC分类号	A61B3/028 A61B3/09 A61B3/103 A61B5/0002 A61B5/06 A61B5/1072 A61B5/1114 A61B5/163 A61B5/168 A61B5/6803 G02C13/005		
其他公开文献	EP3228237A1		
外部链接	Espacenet		

摘要(译)

测距系统技术领域本发明涉及测距系统。测距系统包括测距传感器，存储单元和处理单元。距离测量传感器适于并布置成测量对象的眼睛与一个或多个对象之间的观看距离。所述存储单元适于将所测量的观看距离存储在一组所测量的观看距离中。所述处理单元适于从所述一组测量距离确定所述测量观看距离的统计分布。

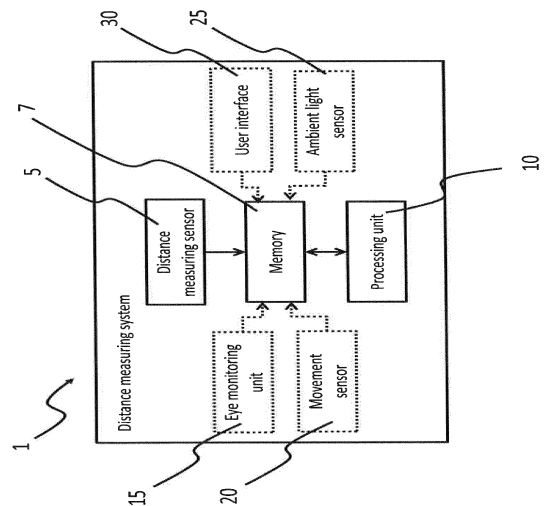


Fig. 1