



(11) **EP 1 389 443 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
05.10.2011 Bulletin 2011/40

(51) Int Cl.:
A61B 5/15^(2006.01)

(21) Application number: **03018219.0**

(22) Date of filing: **11.08.2003**

(54) **Fluid Collecting and Monitoring Device**

Vorrichtung zur Abnahme und Überwachung von Körperflüssigkeiten

Appareil pour recueillir et contrôler des liquides

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IT LI LU MC NL PT RO SE SI SK TR

(30) Priority: **12.08.2002 US 216597**

(43) Date of publication of application:
18.02.2004 Bulletin 2004/08

(73) Proprietor: **Bayer HealthCare LLC**
Tarrytown, NY 10591 (US)

(72) Inventors:
• **Pollock, Neil**
Royston,
Hertfordshire SG8 7DW (GB)
• **Van Rensburg, Richard Wilhelm Janse**
Longstanton,
Cambridge CB4 5BW (GB)

(74) Representative: **Linhart, Angela**
Bayer HealthCare AG
CAO Law & Patents,
Patents & Licensing
51368 Leverkusen (DE)

(56) References cited:
WO-A-01/36954 US-A1- 2002 009 387

- **PATENT ABSTRACTS OF JAPAN vol. 1997, no. 09, 30 September 1997 (1997-09-30) & JP 09 133673 A (KDK CORP), 20 May 1997 (1997-05-20)**
- **PATENT ABSTRACTS OF JAPAN vol. 1996, no. 10, 31 October 1996 (1996-10-31) & JP 08 145980 A (OTAX KK;NITTO DENKO CORP), 7 June 1996 (1996-06-07)**

EP 1 389 443 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The present invention relates generally to fluid collecting and monitoring devices and, more particularly, to a device for obtaining a sample of body fluid, such as blood.

[0002] There are a number of problems with the devices available in the prior art. One such piece of prior art is disclosed in Glenn Purcell's US 2003007893 A entitled "Volume metre testing device". This document discloses a device for collecting and testing blood samples. One problem that is recognised in this document is that of air contaminating the sample and resulting in an inaccurate reading. The prior art device sets about solving this problem by forming a read area that is open sided, that is, one having no side walls. The test fluid arrives in the read area from a transfer area via a capillary gap that has no ceiling or floor and the transfer area itself is fully enclosed. This is a complex structure and requires a high level of dimensional accuracy in the various areas.

[0003] JP 9 133 673 A discloses an instrument and method for measuring liquid sample. The instrument comprises a substrate (3) which can be bent in a U-shape manner. The U-shape comprises a reagent layer (4) and a section (12) separate from the reagent layer (4) forming a system of capillary channels between the facing surfaces (3a and 3b) of substrate (3). The open end of the U-shape forms a sample supplying section. The volume between the section (12) and the opposing surface (3a) of the substrate (3) forms a first channel having a depth t_1 . The volume between the surface of the reagent layer (4) and the opposing surface (3a) of the substrate (3) forms a second channel having a depth t_2 which is smaller than depth t_1 . The volume surrounding section (12) and the reagent layer (4) forms side channels and a rear channel having a depth t_3 which is larger than depths t_1 or t_2 . There is also a gap of depth t_3 between section (12) and reagent layer (4).

[0004] Test devices available in the prior art generally work by making a puncture wound in the skin, placing a vacuum device over the puncture, and applying the vacuum until a bead of blood is formed. The vacuum device is then removed and a test device is brought into contact with the bead to collect a sample.

[0005] A major disadvantage of this system is that the size of blood bead generated by the vacuum stage is variable. If the blood bead is too small then the test device will not collect enough blood and the vacuum has to be re-applied to draw extra blood from the skin. This is a problem for most amperometric devices, where it is important that the test volume is filled in one attempt. If the blood bead is too small and the test device is not completely filled, the test usually has to be repeated causing more pain and inconvenience to the user.

[0006] One of the aspects on which the prior art remains silent is the issue of blood left on the skin. The main aim of the prior art is in regard to picking up a sufficient quantity of blood to perform an accurate test and

it is specifically stated that once the pick up area is full and there is sufficient blood in the device to perform an accurate reading, then the device can be removed from contact with the skin. However, if the blood drop has a volume greater than that required to perform the test then this blood will be left on the skin and the present invention aims to enable enough blood to be obtained to perform the test whilst leaving the skin clean by continuing take up of fluid beyond that strictly necessary to perform the test.

[0007] The choice of material from which the device of the present invention is made is influenced by the surface energies of the fluids under test. As the device operates by capillary action the fluid must have an internal contact angle between the bead of fluid and the surface of less than 90° . For this to occur the surface energy of the surface is more than, or similar to, the surface energy of the fluid. The surface energy is determined by the surface chemistry of the materials and also the surface roughness. The smaller the angle between the surface of a bead of fluid and the surface, the faster the fluid will move through the device.

[0008] The present invention aims to overcome the problems associated with the prior art and accordingly there is provided a device for sampling a fluid in accordance with claim 1.

[0009] Preferably, the device further comprises a step between the first and second channels.

[0010] Vent channels may be provided that surround the first and second open-sided channels.

[0011] The open sides of the channels may be small in comparison to the width of the channels.

[0012] The device may further comprise a vent through which air can be removed from the vent channels. This vent may be situated beyond the second channel.

[0013] The volumetric space within the first channel is preferably 0.4-1.3 μ l and the volumetric space within the second channel is preferably 0.4-1.0 μ l.

[0014] The first and second channels may be aligned to form a substantially straight passageway.

[0015] The lid and base may be bonded together to contain the channels.

[0016] Preferably, a surface of the second channel is coated with a reagent.

[0017] The lid of the device may be translucent or transparent such that a colour change in the reagent may be analysed externally.

[0018] The device may further comprise a pair of electrodes disposed within the second channel to enable measurement of a change in current flowing between the electrodes.

[0019] There is also provided a method of collecting a fluid sample using a device according to the present invention in accordance with claim 2.

[0020] The fluid collected in the first channel is transferred to the second channel by capillary action.

[0021] Alternatively the fluid may continue to be collected by the first channel after the transfer to the second

channel has commenced.

[0022] The fluid may be collected from multiple beads of fluid from different surfaces.

[0023] The method may further comprise placing the device adjacent to a fluid drop such that the lid is closer to the drop than the base and allowing capillary action to collect the fluid into the device. The present invention has a number of advantages over the prior art. Firstly the simplicity of the structure with two open sided capillary channels surrounded by vent channels allows a very high efficiency of fluid transfer between the two capillary channels. This simplicity also has the advantage that the device is comparatively simple to manufacture and construct. The device can be manufactured in two parts: a base and a lid. Each of these may be injection moulded, cast or thermoformed or processed in sheet form and then stamped out. It is therefore easy to assemble the device by joining these two parts together. The movement of the fluid into the device takes place by capillary action encouraged by the provision of side and rear vent channels that allow air to be displaced from the device. This results in a high efficiency of collection from a surface.

[0024] The vent channels render the device robust to the effects of air inclusions and the relative lengths of the capillary and vent channels compared to their widths minimises the evaporation from the device. This means that the lid only has to span the comparatively small combined width of the vent and capillary channels. This has two advantages. Firstly, it is easier to get a tighter tolerance of the heights of the capillary gaps because the smaller span reduces the extent to which the centre can sag and reduce the gap thickness. Secondly, the lid can be made thinner and the device can then be inverted in use so that the lid is in contact with the collection surface where a much smaller bead of blood can bridge the thickness of the lid and be drawn into the capillary structure. This results in a high collection efficiency and also minimised waste. Furthermore, it minimises the amount of fluid left on the front of the device and thereby reduces the risk of contamination. The device has a minimum contact area with the skin resulting in very efficient collection and therefore very little fluid will be left on the surface. The device is able to collect a very small volume of fluid very accurately.

[0025] A number of devices according to the present invention may be formed side-by-side to form a frangible strip. If this is the case then one device may then be removed from the strip whenever it is needed. Alternatively, the devices may be manufactured in the form of a frangible strip but they may subsequently be separated for discrete packaging before they are distributed to the end user.

[0026] Examples of devices according to the present invention will now be described with reference to the drawings, in which:

Figure 1 is a planar section of the device;

Figure 2 is a schematic longitudinal sectional view through the device;

Figure 3 is an exploded isometric view of the device;

Figure 4 is a partially sectioned side view of the device shown in use in the collection of a blood sample.

Figure 5 is a plan view of the facing surfaces of a base and lid which includes electrodes;

Figure 6 is a plan view of the device of Figure 5, after assembly, showing hidden detail; and

Figure 7 is a longitudinal section through the device of Figure 6.

[0027] The device 11 shown in the figures is a blood sampling device and has a base 1 and a lid 2 bonded to the base to form internal volumes which are used to collect and transfer small volumes of blood as described below.

[0028] The device 11 has a fluid collection point 3 at one end provided by the open end of a first channel 17 of depth (capillary gap) t_1 defined, between the base 1 and the underside of the lid 2, by a collection island 4 and the lid 2, and a second channel 18 of depth t_2 defined by a read island 7 and the underside of the lid 2. Side channels 5 and a rear channel 8 surround the islands 4, 7. The side channels 5 and rear channels have a greater depth (larger capillary gap) t_3 and the side channels are located one on each side of the islands 4 and 7. The device 11 also has a vent passage 9 communicating with the rear channels and a pin hole vent 10 communicating with the vent passage 9 to provide for venting of air from any of the channels 5, 8, 17 and 18.

[0029] In one embodiment, the base 1 and the lid 2 are manufactured from transparent materials and a reagent on the read island 7 is arranged to cause a colour change that can be analysed by an external photo-metric unit in use.

[0030] The fluid collection point 3 of the device 11 is placed in contact with the skin 12, typically within 0.5mm of the puncture site 15. The device 11 is used in an inverted position such that the lid 2 is closer to the skin 12 than the base 1. The lid 2 is thinner in section than the base 1 so that the bead of blood only needs to grow enough in height to bridge the thickness of the lid 2 and the gap t_1 (see fig. 2) at the fluid collection point 3. This minimises the volume of blood that is left on the skin 12 after the device has been removed.

[0031] The device can be used to collect blood from the surface of skin as shown in Figure 4 by means of a needle 14 which produces a small puncture 15 in the skin 12. A bead of blood is caused to flow from the puncture wound 15, for example by the application of an area of reduced pressure in the volume of air 13 directly above the skin 12, the volume of air 13 above the skin being defined by an appropriate structure 16. The absolute pressure in this area may be 0.1 to 0.7 bars and preferably 0.3 to 0.5 bars. An advantage of the present invention is that the read island 7 and collection island 4 can be stationary throughout the blood collection process. The de-

vice needs to be enclosed in the vacuum to prevent air leaking via the vent hole 10. The first channel 17 is kept in a known position relative to the puncture site. This means that the internal volume of the device can be smaller and the side channel can also be smaller and therefore the bead of blood required is smaller. This means, in turn, that the puncture in the skin required to extract sufficient blood to fill the device will be smaller and less painful.

[0032] The device 11 is held by the user at an angle relative to the surface of the skin 12 at the puncture site 15. The angle (typically between 30 degrees and 60 degrees) ensures that the contact area between the lid 2 and the skin 12 is minimised, which also reduces the volume of blood left on the surface of the test device and the skin when the test has been completed and the device 11 has been removed.

[0033] In use, the blood bead grows to bridge the gap t_1 between the lid 2 and the collection island 4 as mentioned above.. Blood fills the channel 17 above the collection island 4 by capillary action until the fluid front of the blood contacts a step 6 at the front edge of the read island 7. The shape of the blood volume in the channel 17 above the collection island 4 is defined by the edge of the collection island 4 as there are no side walls. Once the blood volume has reached the step 6, the blood is in communication with the channel 18 (which has a gap t_2 above the read island 7). The majority of the volume of blood on the collection island 4 is then transferred onto the read island 7 by capillary action. Blood will not flow into the side channels 5 or the rear channel 8 because the gap t_3 between the base 1 and lid 2 at the side channels 5 and the rear channel 8 is significantly larger than the gaps t_1 and t_2 above the collection island 4 and the read island 7, respectively. Once the blood is transferred to the read island 7 the blood is exposed to a reagent previously coated onto either the area of the lid 2 opposite the read island 7 or onto the surface of the read island 7. The reagent reacts with an analyte in the blood to produce either a colour change or an electrical current (as described below).

[0034] Although The area of the read island 7 is slightly larger than the area of the collection island 4 the channel 17 associated with the collection island is deeper and therefore the overall volume of the collection island 4 is greater than that of the read island 7. This ensures that the read island 7 is completely filled when the blood transfers between islands. By having the collection volume larger than the read volume an incomplete fill of the read area is eliminated. The majority of the volume of the blood on the collection island 4 is transferred since the blood is only in contact (and pinned) at the two edges at the front of the collection island 4 and the lid 2 at the fluid collection point 3. The amount of blood left in the collection island 4 is the difference in volume between the collection 4 and read 7 islands. The difference in the size of the gaps t_1 and t_2 at the step 6 is sufficient to unpin the blood from these edges. The high efficiency transfer

of blood between the islands means that the device is very efficient. Typically, the transfer efficiency between the collection island 4 and the read island 7 may be between 75% and 100%. The small volume of waste in the collection and transfer mechanisms also means that the initial volume of blood in the blood bead on the surface of the skin 12 can be very small. In a preferred example, the volume of blood on the skin collected and transferred to fill the read island 7 can be between 0.5 μl and 1.5 μl .

[0035] One advantage of the step 6 and the relative heights of the two channels 17, 18 is that the collection of blood will continue as blood moves by capillary action from the first channel 17 to the second channel 18 leaving the first channel 17 available to collect more blood from the surface of the skin 12. The transfer of the blood volume between the collection island 4 and the read island 7 can, however, occur rapidly if the surface energies of the islands and the lid as well as the sizes of the gaps t_1 and t_2 are controlled. This feature is an advantage if the method of analysing the analyte in the blood on the read island 7 is time-dependant. Blood will preferentially be picked up by the smaller capillary gap t_1 on the collection island 4 at, or near, the fluid collection point 3.

[0036] If the bead of blood is large enough, the device 11 can be used to collect an initially larger bead of blood, such that the larger initial volume and size of the blood bead blocks both side channels 5 and the collection island 4. In this case, the device will still operate since the air above the collection island 4 and the read island 7 can be displaced out of the device 11 through the vent 9 and the pin hole vent 10.

[0037] The widths of the side channels and collection islands are minimised as far as practicable so that the lid 2 can be made to be as thin as possible without compromising the assembly tolerances of the gaps t_1 and t_3 . The thickness of the lid 2 is made as low as possible in order to minimise the size of the blood bead that can be collected from the surface of the skin. Another advantage of reducing the width of the collection island 4 is to control the position of the fluid front of the blood more accurately as it flows to the step 6. There is also an advantage to maximising the length of both islands 4, 7 as this maximises the length of the air diffusion path between the blood volume and the air outside the device 11. This minimises the effects of evaporation which in turn may affect the concentration of the analyte within the blood sample.

[0038] When the blood volume in the collection island 4 is transferred to the read island 7, the collection island is nearly emptied of blood. This has two potential advantages. Firstly, if blood continues to flow from the puncture site 15, the device will continue to collect blood onto the collection island 4 i.e. 'mopping' up excess blood from the skin 12. Secondly, if the device 11 is removed from the surface of the skin at the moment of blood transfer to the collection island 4 (this movement may be triggered by the appearance of blood on the read island 7), then there will be little or no blood left on the collection island 4 and the blood sample will be isolated inside the device

11 on the read island 7. This may reduce the risks of blood contamination.

[0039] In an alternative embodiment, illustrated in figures 5, 6 and 7, two electrodes are formed onto the underside of the lid 2: a working electrode 19 and a reference electrode 20. Both electrodes are then coated with an insulating layer 23 over the area which will contact the base 1, and two small windows are left in the insulating layer to provide a working electrode window 21 and a reference electrode window 22 on the lid 2 opposite the read island 7. A chemical reagent is coated on to the read island 7.

[0040] When blood is transferred from the collection island 4 to the read island 7, the reagent dissolves in the blood and a reaction takes place that creates a small current which is related to the amount of glucose in the blood. The current creates a potential difference between the reference electrode 20 and the working electrode 19. The location and exposed area of the electrode windows 21 and 22 is very important. The area of the read island 7 and hence the volume of the initial blood sample can be reduced by minimising the exposed area of the electrodes 21 and 22 and also by their positional accuracy.

Claims

1. A device (11) for sampling a fluid comprising:

a base (1);
 a lid (2);
 and, between the base (1) and the lid (2),
 an opening (3),
 a first open-sided channel (17) extending from the opening (3) to a second open-sided channel (18), and
 side channels (5) and rear channel (8) surrounding the first open-sided channel (17) and the second open-sided channel (18),
 wherein the first open-sided channel (17) has a depth t_1 defined by a collection island (4) and the underside of the lid (2),
 wherein a depth t_2 of the second open-sided channel (18) defined by a read island (7) and the underside of the lid (2) is smaller than the depth t_1 of the first open-sided channel (17),
 wherein the depth t_3 of the side channels (5) and the rear channel (8) defined between the underside of the lid (2) and the base (1) is greater than the depth t_1 of the first open-sided channel (17) and the depth t_2 of second open-sided channel (18).

2. A device (11) according to claim 1, further comprising a step (6) between the first and second channels (17, 18).

3. A device (11) according to claim 1 or claim 2, wherein

the open sides of the first and second channels (17, 18) are small in comparison to the width of the channels (17, 18).

4. A device (11) according to one of the claims 1 to 3, further comprising a vent (9, 10) through which air can be removed from the first, second, side and rear channels (17, 18, 5, 8).

5. A device (11) according to claim 4, wherein the vent (9, 10) is situated beyond the second channel (18).

6. A device (11) according to one of the claims 1 to 5, wherein the volumetric space within the first channel (17) is 0.4 - 1.3 μl and the volumetric space within the second channel (18) is 0.4 - 1.0 μl .

7. A device (11) according to one of the claims 1 to 6, wherein the first (17) and second (18) channels are aligned to form a substantially straight passageway.

8. A device (11) according to one of the claims 1 to 7, wherein the lid (2) and the base (1) are bonded together to contain the channels (17, 18, 5, 8).

9. A device (11) according to one of the claims 1 to 8, wherein a surface of the second channel (18) is coated with a reagent.

10. A device (11) according to claim 9, wherein the lid (2) of the device (11) is translucent or transparent such that a colour change in the reagent may be analysed externally.

11. A device (11) according to claim 9, further comprising a pair of electrodes (19, 20) disposed within the second channel (18) to enable measurement of a change in current flowing between the electrodes (19, 20).

12. A method of collecting a fluid sample using a device (11) according to claim 1, the method comprising; placing the device (11) adjacent to a fluid drop (15) and allowing capillary action to collect the fluid into the device (11), wherein the fluid collected in the first channel (17) is transferred to the second channel (18) by capillary action, and wherein the fluid collected in the first channel (17) is not transferred into the side channels (5) and the rear channel (8).

13. A method according to claim 12, wherein fluid continues to be collected by the first channel (17) after the transfer to the second channel (18) has commenced.

14. A method according to claim 12 or 13, wherein the fluid is collected from multiple beads of fluid from different surfaces.
15. A method of collecting a fluid sample according to claim 12, the method comprising;
placing the device adjacent to a fluid drop such that the lid is closer to the drop than the base and allowing capillary action to collect the fluid into the device.

Patentansprüche

1. Vorrichtung (11) zur Entnahme einer Probe einer Flüssigkeit, die Folgendes umfasst: einen Boden (1); einen Deckel (2); und zwischen dem Boden (1) und dem Deckel (2) eine Öffnung (3), wobei sich ein erster an der Seite offener Kanal (17) von der Öffnung (3) zu einem zweiten an der Seite offenen Kanal (18) erstreckt und wobei die seitlichen Kanäle (5) und ein hinterer Kanal (8) den ersten an der Seite offenen Kanal (17) und den zweiten an der Seite offenen Kanal (18) umgeben, worin der erste an der Seite offene Kanal (17) eine Tiefe t_1 aufweist, die durch eine Auffanginsel (4) und die Unterseite des Deckels (2) definiert wird, worin eine tiefe t_2 des zweiten an der Seite offenen Kanals (18), die von einer Ablesinsel (7) und der Unterseite des Deckels (2) definiert wird, kleiner ist als die Tiefe t_1 des ersten an der Seite offenen Kanals (17), worin die Tiefe t_3 der seitlichen Kanäle (5) und des hinteren Kanals (8), die zwischen der Unterseite des Deckels (2) und dem Boden (1) definiert wird, größer ist als die Tiefe t_1 des ersten an der Seite offenen Kanals (17) und die Tiefe t_2 des zweiten an der Seite offenen Kanals (18).
2. Vorrichtung (11) nach Anspruch 1, die ferner eine Stufe (6) zwischen den ersten und zweiten Kanälen (17, 18) umfasst.
3. Vorrichtung (11) nach Anspruch 1 oder Anspruch 2, worin die offenen Seiten der ersten und zweiten Kanäle (17, 18) im Vergleich zur Breite der Kanäle (17, 18) klein sind.
4. Vorrichtung (11) nach einem der Ansprüche 1 bis 3, die ferner eine Entlüftungsöffnung (9, 10) umfasst, durch die Luft aus den ersten, zweiten, seitlichen und hinteren Kanälen (17, 18, 5, 8) entfernt werden kann.
5. Vorrichtung (11) nach Anspruch 4, worin die Entlüftungsöffnung (9, 10) hinter dem zweiten Kanal (18) angeordnet ist.
6. Vorrichtung (11) nach einem der Ansprüche 1 bis 5, worin der volumetrische Raum im ersten Kanal (17)

0,4 - 1,3 μl beträgt und der volumetrische Raum im zweiten Kanal (8) 0,4 - 1,0 μl beträgt.

7. Vorrichtung (11) nach einem der Ansprüche 1 bis 6, worin die ersten (17) und zweiten (18) Kanäle so ausgerichtet sind, dass sie einen im Wesentlichen geraden Durchgang formen.
8. Vorrichtung (11) nach einem der Ansprüche 1 bis 7, worin der Deckel (2) und der Boden (1) miteinander verbunden sind, um die Kanäle (17, 18, 5, 8) aufzunehmen.
9. Vorrichtung (11) nach einem der Ansprüche 1 bis 8, worin eine Oberfläche des zweiten Kanals (18) mit einem Reagenz beschichtet ist.
10. Vorrichtung (11) nach Anspruch 9, worin der Deckel (2) der Vorrichtung (11) durchscheinend oder durchsichtig ist, so dass eine Farbveränderung des Reagenz von außen analysiert werden kann.
11. Vorrichtung (11) nach Anspruch 9, die ferner ein im zweiten Kanal (18) angeordnetes Elektrodenpaar (19, 20) zur Messung einer Veränderung des zwischen den Elektroden (19, 20) fließenden Stroms umfasst.
12. Verfahren zur Entnahme einer Flüssigkeitsprobe mit einer Vorrichtung (11) nach Anspruch 1, wobei das Verfahren Folgendes umfasst: Platzierung der Vorrichtung (11) neben einem Flüssigkeitstropfen (15) und Auffangen der Flüssigkeit durch Kapillarwirkung in der Vorrichtung (11), worin die im ersten Kanal (17) aufgefangene Flüssigkeit durch Kapillarwirkung zum zweiten Kanal (18) überführt wird und worin die im ersten Kanal (17) aufgefangene Flüssigkeit nicht in die seitlichen Kanäle (5) und den hinteren Kanal (8) überführt wird.
13. Verfahren nach Anspruch 12, worin vom ersten Kanal (17) weiter Flüssigkeit aufgefangen wird, nachdem die Überführung zum zweiten Kanal (18) begonnen hat.
14. Verfahren nach Anspruch 12 oder 13, worin die Flüssigkeit von mehreren Flüssigkeitsperlen von unterschiedlichen Oberflächen gesammelt wird.
15. Verfahren zur Entnahme einer Flüssigkeitsprobe nach Anspruch 12, wobei das Verfahren Folgendes umfasst: Platzierung der Vorrichtung neben einem Flüssigkeitstropfen, so dass der Deckel näher am Tropfen als am Boden ist, und Auffangen der Flüssigkeit durch Kapillarwirkung in der Vorrichtung.

Revendications

1. Dispositif (11) pour échantillonner un fluide, comprenant:
 - une base (1);
 - un couvercle (2);
 - et, entre la base (1) et le couvercle (2);
 - une ouverture (3);
 - un premier canal à côtés ouverts (17) qui s'étend à partir de l'ouverture (3) jusqu'à un deuxième canal à côtés ouverts (18); et
 - des canaux latéraux (5) et un canal arrière (8) qui entourent le premier canal à côtés ouverts (17) et le deuxième canal à côtés ouverts (18), dans lequel le premier canal à côtés ouverts (17) a une profondeur t_1 qui est définie par un îlot de collecte (4) et la face inférieure du couvercle (2), dans lequel une profondeur t_2 du deuxième canal à côtés ouverts (18) qui est défini par un îlot de lecture et la face inférieure du couvercle (2) est plus petite que la profondeur t_1 du premier canal à côtés ouverts (17), dans lequel la profondeur t_3 des canaux latéraux (5) et du canal arrière (8) qui sont définis entre la face inférieure du couvercle (2) et la base (1) est plus grande que la profondeur t_1 du premier canal à côtés ouverts (17) et que la profondeur t_2 du deuxième canal à côtés ouverts (18).
2. Dispositif (11) selon la revendication 1, comprenant en outre un gradin (6) entre les premier et deuxième canaux (17, 18).
3. Dispositif (11) selon la revendication 1 ou la revendication 2, dans lequel les côtés ouverts des premier et deuxième canaux (17, 18) sont petits en comparaison avec la largeur des canaux (17, 18).
4. Dispositif (11) selon l'une quelconque des revendications 1 à 3, comprenant en outre un évent (9, 10) à travers lequel l'air peut être évacué à partir des premier et deuxième canaux (17, 18), des canaux latéraux (5) et du canal arrière (8).
5. Dispositif (11) selon la revendication 4, dans lequel l'évent (9, 10) est situé au-delà du deuxième canal (18).
6. Dispositif (11) selon l'une quelconque des revendications 1 à 5, dans lequel l'espace volumétrique à l'intérieur du premier canal (17) est compris entre 0,4 μl et 1,3 μl , et l'espace volumétrique à l'intérieur du deuxième canal (18) est compris entre 0,4 μl et 1,0 μl .
7. Dispositif (11) selon l'une quelconque des revendications 1 à 6, dans lequel le premier canal (17) et le deuxième canal (18) sont alignés de manière à former un passage sensiblement droit.
8. Dispositif (11) selon l'une quelconque des revendications 1 à 7, dans lequel le couvercle (2) et la base (1) sont assemblés l'un à l'autre pour contenir les canaux (17, 18, 5, 8).
9. Dispositif (11) selon l'une quelconque des revendications 1 à 8, dans lequel une surface du deuxième canal (18) est revêtue d'un réactif.
10. Dispositif (11) selon la revendication 9, dans lequel le couvercle (2) du dispositif (11) est translucide ou transparent, de telle sorte qu'un changement de couleur dans le réactif puisse être analysé depuis l'extérieur.
11. Dispositif (11) selon la revendication 9, comprenant en outre une paire d'électrodes (19, 20) qui sont disposées à l'intérieur du deuxième canal (18) de manière à permettre la mesure d'un chargement dans un courant qui s'écoule entre les électrodes (19, 20).
12. Procédé de collecte d'un échantillon de fluide en utilisant un dispositif (11) selon la revendication 1, le procédé comprenant les étapes suivantes:
 - placer le dispositif (11) à proximité d'une chute de fluide (15); et
 - laisser le fluide être collecté dans le dispositif (11) par capillarité, dans lequel le fluide collecté dans le premier canal (17) est transféré vers le deuxième canal (18) par capillarité, et dans lequel le fluide collecté dans le premier canal (17) n'est pas transféré dans les canaux latéraux (5) et le canal arrière (8).
13. Procédé selon la revendication 12, dans lequel le fluide continue à être collecté par le premier canal (17) après que le transfert vers le deuxième canal (18) ait commencé.
14. Procédé selon la revendication 12 ou 13, dans lequel le fluide est collecté à partir de multiples perles de fluide à partir de différentes surfaces.
15. Procédé de collecte d'un échantillon de fluide selon la revendication 12, le procédé comprenant les étapes suivantes:
 - placer le dispositif à proximité d'une chute de fluide de telle sorte que le couvercle soit plus proche de la chute que la base; et
 - laisser le fluide être collecté dans le dispositif par capillarité.

FIG. 1

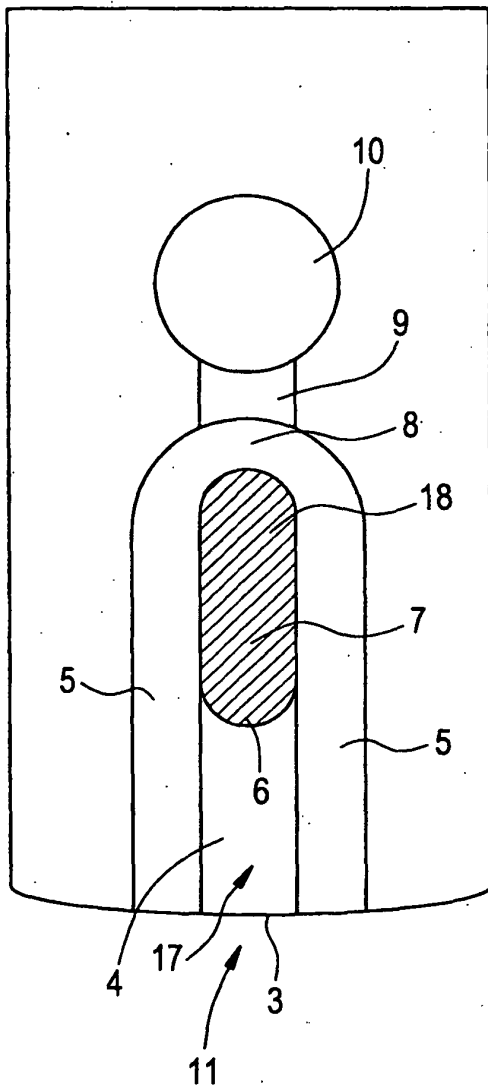


FIG. 2

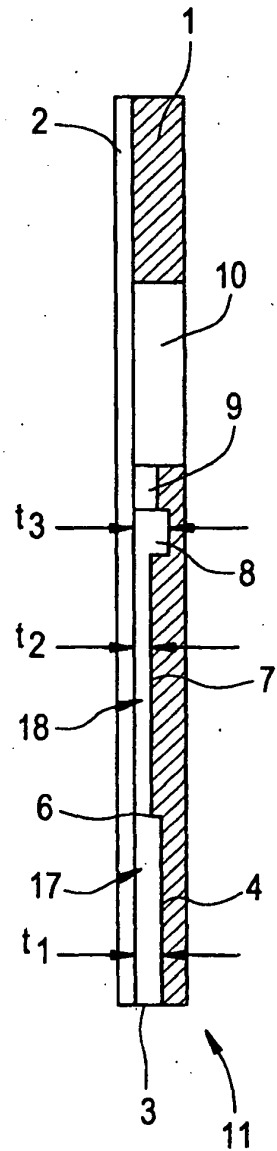


FIG. 3

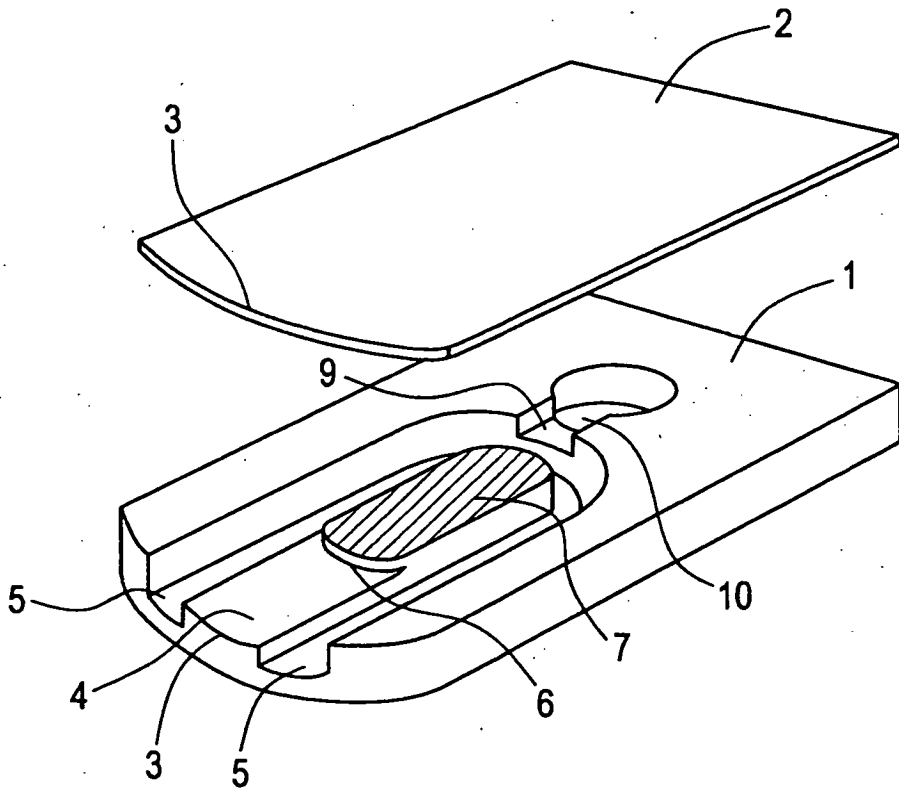


FIG. 4

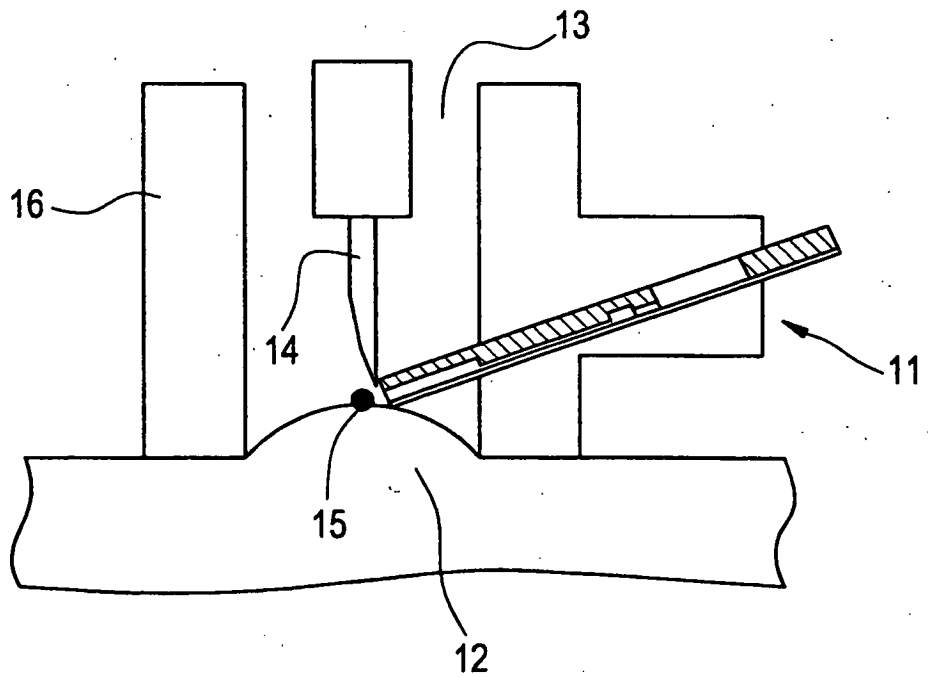


FIG. 5

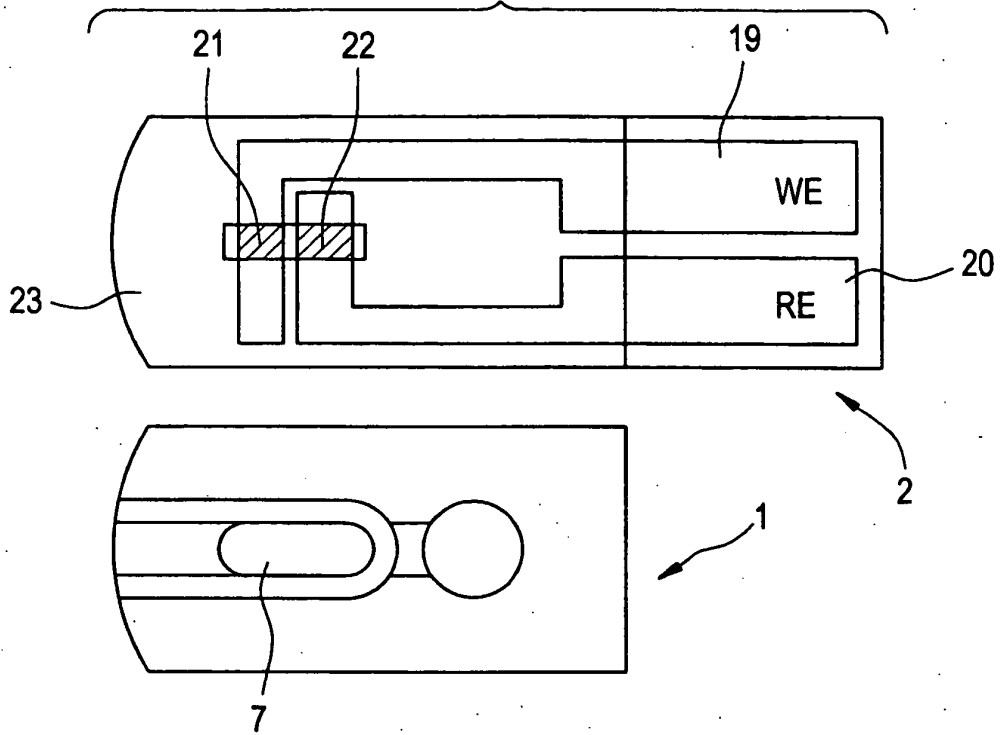


FIG. 6


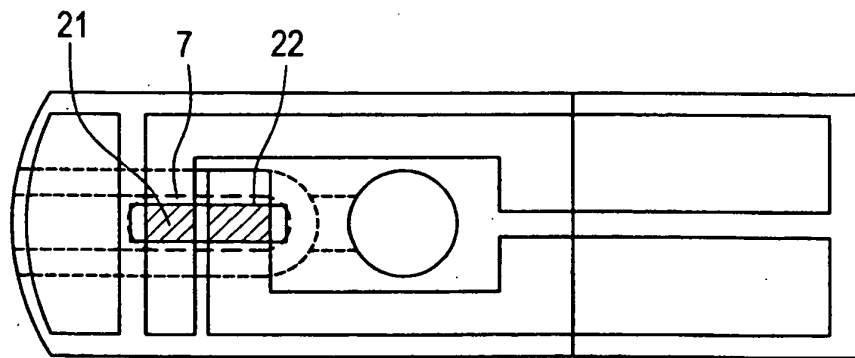


FIG. 7

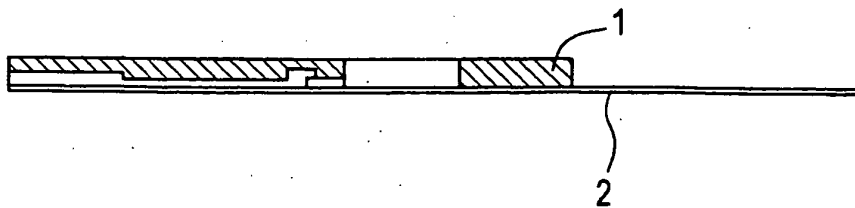

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 2003007893 A [0002]
- JP 9133673 A [0003]

专利名称(译)	流体收集和监测装置		
公开(公告)号	EP1389443B1	公开(公告)日	2011-10-05
申请号	EP2003018219	申请日	2003-08-11
[标]申请(专利权)人(译)	拜尔健康护理有限责任公司		
申请(专利权)人(译)	拜耳医药保健, LLC		
当前申请(专利权)人(译)	拜耳医药保健有限责任公司		
[标]发明人	POLLOCK NEIL VAN RENSBURG RICHARD WILHELM JANSE		
发明人	POLLOCK, NEIL VAN RENSBURG, RICHARD WILHELM JANSE		
IPC分类号	A61B5/15 G01N1/10 A61B5/00 A61B5/151 G01N27/327		
CPC分类号	A61B5/150358 A61B5/14532 A61B5/150022 A61B5/150213 A61B2562/0295 Y10T436/2575		
优先权	10/216597 2002-08-12 US		
其他公开文献	EP1389443A1		
外部链接	Espacenet		

摘要(译)

一种用于流体取样的装置，包括底座（1）和盖子（2）。在底座和盖子之间设置有开口和从开口延伸到第二开口侧通道（7）的第一开口侧通道（4），用于在其中收集流体。第二通道的深度小于第一通道的深度。

FIG. 1

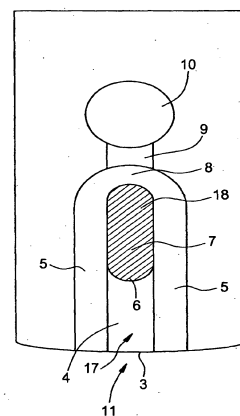


FIG. 2

