



(11) **EP 1 664 745 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
10.01.2007 Bulletin 2007/02

(21) Application number: **04774960.1**

(22) Date of filing: **22.09.2004**

(51) Int Cl.:
G01N 21/49 (2006.01) A61B 5/00 (2006.01)

(86) International application number:
PCT/NL2004/000657

(87) International publication number:
WO 2005/029051 (31.03.2005 Gazette 2005/13)

(54) **METHOD AND APPARATUS FOR BACKSCATTER SPECTROSCOPY**

VERFAHREN UND VORRICHTUNG ZUR RÜCKSTREUSPEKTROSKOPIE

PROCEDE ET DISPOSITIF POUR LA SPECTROSCOPIE DE RETRODIFFUSION

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IT LI LU MC NL PL PT RO SE SI SK TR

(30) Priority: **23.09.2003 EP 03078010**

(43) Date of publication of application:
07.06.2006 Bulletin 2006/23

(73) Proprietor: **Stichting voor de Technische Wetenschappen**
3527 EP Utrecht (NL)

(72) Inventors:
• **AMELINK, Arjen**
NL-2803 CB Gouda (NL)

• **STERENBORG, Henricus, Josephus, Cornelis, Maria**
NL-2901 RC Capelle Aan Den IJssel (NL)

(74) Representative: **van Westenbrugge, Andries**
Nederlandsch Octrooibureau
Postbus 29720
2502 LS Den Haag (NL)

(56) References cited:
US-A1- 2002 171 831 US-B1- 6 381 018

• **AMELINK A ET AL: "Single-scattering spectroscopy for the endoscopic analysis of particle size in superficial layers of turbid media"**
APPLIED OPTICS, vol. 42, no. 19, July 2003 (2003-07), pages 4095-4101, XP002266905 cited in the application

EP 1 664 745 B1

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The present invention relates to a method of determining of a physical feature of a medium, comprising:

- 5 - producing radiation with a light source;
- placing a probe on a sample of said medium, the probe comprising a first optical fiber having a first diameter, and at least a second optical fiber having a second diameter;
- sending light coming from the light source, through the first optical fiber;
- 10 - collecting first backscattered radiation through the first optical fiber and second backscattered radiation through the second optical fiber;
- producing a first signal based on the first backscattered radiation, and a second signal based on the second backscattered radiation;
- determine a measured differential backscatter signal as a function of wavelength using the first and second signals.

15 **[0002]** Such a method is known from Amelink et al [1]. There, a special device is used to determine particle sizes in superficial layers. The device is suitable for measuring particle sizes in for example an aqueous suspension with polystyrene spheres, but is not fitted to accurately measure particle sizes in living tissue. So, determining whether living tissue is normal or precancerous, by way of measuring particle sizes in living tissue is not very promising.

20 **[0003]** In Doornbos et al [2] the optical properties of human tissue are determined in vivo using a spectroscopic arrangement with ten optical fibers. One of the fibers is used to irradiate a sample, and nine other fibers collect the reflected light. By using a multitude of fibers to collect the reflected light, it is possible to calculate scattering and absorption coefficients of the sample. However, the method is not suitable for locally measuring the optical properties of the tissue. In particular, only mean values of the absorption coefficient of a relatively large part of the sample can be determined.

25 **[0004]** It is an object of the present invention to locally measure a physical feature, such as a concentration, of a substance in a medium.

[0005] The object is achieved by a method as described above, characterized by

- 30 - calculating the physical feature by curve fitting said measured differential backscatter signal to a backscatter function, in which the backscatter function is a function of an average path-length travelled by detected scattered photons, wherein the average path-length is independent from an absorption coefficient of the medium, and from a scattering coefficient of the medium. Contrary to methods using diffusely scattered photons such as Doornbos et al [2], in the method according to the invention, the local absorption coefficient of the sample is measured in an absolute way, independent of the magnitude of the local scattering and absorption coefficients. This facilitates the measurement of absolute concentrations of absorbing molecules in a sample without requiring prior knowledge of the magnitude of the scattering and absorption coefficients of the medium.

35 **[0006]** In an embodiment, the average path-length is proportional to the first fiber diameter. This has as additional advantage that the average path-length and thereby the average penetration depth into the sample of the photons that contribute to the differential backscatter signal can be controlled by choosing the fiber diameter. As a result, the sampling volume can be controlled by adjusting the fiber diameter. Hence, the fiberoptic probe can be engineered to match the relevant dimensions of the medium under investigation.

40 **[0007]** In a particular embodiment, the physical feature is a concentration of at least one substance in the medium.

[0008] The invention also relates to a device for determining a physical feature of a medium, comprising:

- 45 - a light source for producing radiation;
- a probe with at least a first and a second optical fiber, the first optical fiber having a first diameter and being arranged to deliver the radiation on a sample of said medium and to collect first backscattered radiation from said sample, the second optical fiber having a second diameter and being arranged to collect second backscattered radiation, wherein the second optical fiber is positioned alongside the first optical fiber;
- 50 - a spectrometer for producing a first signal based on the first backscattered radiation, and for producing a second signal based on the second backscattered radiation;
- a processor arranged to determine a measured differential backscatter signal as a function of wavelength using the first and second signals,

55 characterized in that the processor is arranged to calculate the physical feature by curve fitting the measured differential backscatter signal to a backscatter function, in which the backscatter function is a function of an average path-length travelled by detected scattered photons, the average path-length being independent from an absorption coefficient of the medium, and from a scattering coefficient of the medium.

[0009] Furthermore, the invention relates to a computer program according to claim 8 and to a data carrier according to claim 9.

[0010] In another aspect of the invention, the invention relates to a method of determining a physical feature of a medium, comprising:

- 5
- producing radiation with a light source;
 - placing a probe on a sample of the medium, the probe comprising a first optical fiber having a first diameter, and at least a second optical fiber having a second diameter;
 - sending light coming from the light source, through the first optical fiber;
 - 10 - collecting first backscattered radiation through the first optical fiber and second backscattered radiation through the second optical fiber;
 - producing a first signal based on the first backscattered radiation; and a second signal based on the second backscattered radiation;
 - determining a measured differential backscatter signal as a function of wavelength using the first and second signals,

15 characterized by

- calculating the physical feature by curve fitting the measured differential backscatter signal to a backscatter function, in which the backscatter function is a function of a mean free path of photons. In this method, it is assumed that only singly scattered photons contribute to the differential backscatter signal and as a result the backscatter function can be easily derived analytically.
- 20

[0011] In an embodiment, the physical feature is a concentration of at least one substance in the medium.

[0012] The invention also relates to a device according to claim 13.

25 **[0013]** Furthermore, the invention relates to a computer program according to claim 14 and to a data carrier according to claim 15.

[0014] Finally, the invention relates to a method according to claim 16.

[0015] The present invention will be described below with reference to exemplary embodiments and the accompanying schematic drawings, in which:

30 Fig. 1 is a schematic diagram of a measuring device according to a preferred embodiment;

Fig. 2a and 2b show cross sections of a sample and two fiber tips in the situation wherein the mean free path of the photons is much larger than the diameter of the fibers;

Fig. 3 shows the results of Monte Carlo simulations for a homogeneous medium;

35 Fig. 4 a differential backscatter signal normalized at zero absorption for several scattering coefficients;

Fig. 5 shows a differential backscatter signal of a dilute suspension of 0.2 μm polystyrene spheres

Fig. 6 shows the total differential backscatter signal as a function of the reflection coefficient $\mu_s(\lambda)$ in the range of 10-100 mm^{-1} ;

Fig. 7 shows the measured and calculated average path length τ as a function of the average scattering coefficient;

40 Fig. 8 is a graph of measurement results for three different absorption coefficients μ_a showing the dc-fiber signal I , the c-fiber signal J and the differential backscatter signal R_{bs} as a function of wavelength;

Fig. 9 shows a typical spectrum of an absorption curve A along with the specific absorption coefficient of Evans Blue dye;

Fig. 10 shows a measured A^* as a function of the absorption coefficient μ_a at $\lambda = 600 \text{ nm}$;

45 Fig. 11 shows typical spectra measured in a suspension of 1.0 μm polystyrene spheres with and without Evans Blue dye;

Fig. 12 graphically shows a molar extinction coefficient as a function of wavelength;

Fig. 13 shows in vivo measurements and a fit of the differential backscatter signal R_{bs} in a human trachea realized using a fiber diameter of 400 μm , and

50 Fig. 14 shows in vivo measurements and a fit of the differential backscatter signal R_{bs} in a human trachea showing very low oxygenation indicative for lung tumor.

[0016] A schematic diagram of a preferred embodiment according to the invention is shown in figure 1. The setup consists of a set of optical fibers for the delivery and collection of light to and from a sample 1 under investigation. Light from a light source 2, for example a Tungsten Halogen lamp (Avantes HL-2000-FHSA), is led through a first arm 3 of a bifurcated optical fiber. The bifurcated optical fiber is at a distal end 4 coupled to a first distal end of a delivery- and-collection fiber 5 (in the following referred to as dc-fiber 5) which is small enough to be fit through a working channel of a clinical endoscope, not shown. A second distal end of the delivery- and-collection fiber 5 contacts the sample 1.

55

Alongside the dc-fiber 5, a collection fiber 6 is arranged to collect light reflected by the sample 1. The collection fiber 6 (referred to as c-fiber 6) is connected to a slave channel of a dual-channel spectrometer 7, for example an Avantes SD2000. Preferably, the dc-fiber 5 is polished at a small angle to reduce specular reflections.

[0017] Light reflected back from the sample 1 into the c-fiber 6 is led directly into the slave channel of the dual-channel spectrometer 7. A second arm 8 of the bifurcated fiber is connected to a master channel of the dual-channel spectrometer 7. Light reflected into the dc-fiber 5 is coupled back into the bifurcated fiber, and reaches the dual-channel spectrometer 7 via the second arm 8 of the bifurcated fiber. An output of the spectrometer 7 is connected to an input of a processor 9 which is arranged to analyze signals from the spectrometer 7.

[0018] If only the dc-fiber 5 would be used to deliver and collect light to and from the sample 1, a large fraction of collected light is due to single backscattering from small sample depths, see [1]. A single to multiple scattering ratio depends on the scattering coefficient and phase function of the sample 1 and on a diameter of the dc-fiber 5. The contribution of multiply scattered light to the signal of the dc-fiber 5 can be approximately determined by combining the signal of the dc-fiber 5 with a signal coming from an additional fiber, i.e. the c-fiber 6 mentioned above.

[0019] In [4] a differential backscatter signal R_{bs} as a function of the wavelength λ is determined using a formula like

$$R_{bs}(\lambda) = c \cdot \left(\frac{(I(\lambda) - I_n(\lambda))}{(I_{white}(\lambda) - I_{black}(\lambda))} - \frac{J(\lambda)}{J_{white}(\lambda) - J_{black}(\lambda)} \right) \quad (1)$$

where $I(\lambda)$ is the signal from the dc-fiber 5 in contact with the sample 1, $I_n(\lambda)$ is the signal from the dc-fiber 5 submersed in a fluid with an appropriate refractive index (for tissue: water would be appropriate), $I_{white}(\lambda)$ is the signal from the dc-fiber 5 with the probe-tip at a specific distance from a diffuse reflecting reference material with a large, preferably wavelength-independent reflectance coefficient (white spectralon) and $I_{black}(\lambda)$ is the signal from the dc-fiber 5 with the probe-tip at that same specific distance from a diffuse reflecting reference material with a small, preferably wavelength-independent reflectance coefficient (black spectralon). Furthermore, $J(\lambda)$ is the signal from the c-fiber 6 in contact with the sample 1 and $J_{white/black}(\lambda)$ is the signal from the c-fiber 6 with the probe-tip at the previously mentioned specific distance from the white/black spectralon. Finally, c is a calibration constant that depends on the distance between the probe-tip and the reference materials.

[0020] According to the invention, the processor 9 is arranged to calculate the physical feature using a predefined mathematical model, the differential backscatter signal (R_{bs}) and a curve fitting mechanism. In an embodiment, the diameters of the fibers 5, 6 are selected depending on a mean free path (mfp) of photons sent into the sample 1. It is noted that if the mean free path can not be estimated before selecting a fiber diameter, initially two arbitrary fiber diameters may be selected. After curve fitting the measuring results using two different mathematical models, it will show which model applies.

[0021] Figures 2a and 2b depict fiber tips of the dc-fiber 5 and the c-fiber 6 in the situation wherein the mean free path (mfp) of photons coming out of the dc-fiber 5, is much larger than a diameter d_{fiber} of the fibers 5, 6. In an embodiment, the diameters of both fibers 5, 6 are of equal size, however it should be understood that other selections are possible. In figure 2a, lines 21 and 22 show an example of a path traveled by a detectable singly scattered photon. In figure 2b, lines 23, 24, 25 and lines 23, 24, 26 show two possible paths of detectable multiply scattered photons. All multiple scattering events occur at such large distances from the fiber tip of the fibers 5, 6, that the probability of detection of multiply scattered photons is roughly equal for the dc-fiber 5 and the c-fiber 6. The differential backscatter signal $R_{bs}(\lambda)$ will now purely be determined by singly scattered photons.

[0022] In an embodiment, the diameter of the fibers 5, 6 are selected so that $mfp > d_{fiber}$. In the predefined mathematical model of this embodiment, the differential backscatter signal $R_{bs}(\lambda)$ is an exponential function of two times the mean free path. Below, an explanation for this model is given.

[0023] In the absence of absorbers, the differential backscatter signal $R_{bs}(\lambda)$ is proportional to the local, superficial scattering coefficient $\mu_s(\lambda) = Q_{sca}(\lambda) \cdot \rho \cdot A_s$:

$$R_{bs}(\lambda) = C_{app} \cdot \frac{1}{4\pi} \cdot \int_{\Omega_{NA}} d\Omega \cdot p(\lambda, \Omega) \cdot Q_{sca}(\lambda) \cdot \rho \cdot A_s \quad (2)$$

where C_{app} is an apparatus constant that depends amongst others on the distance between the probe tip and the reference materials (black and white spectralon), $p(\lambda, \Omega)$ is a function called the phase function where Ω is the scattering

angle, $Q_{sca}(\lambda)$ the scattering efficiency, ρ the concentration of substances present in the sample 1, and A the area of a scattering particle. For example, using a fused silica fiber with numerical aperture $NA=0.22$, the differential backscatter signal $R_{bs}(\lambda)$ can be approximated by

$$R_{bs}(\lambda) \approx C_{app} \cdot \frac{1}{4\pi} \cdot \int_0^{2\pi} d\varphi \cdot \int_{170}^{180} d\theta \cdot \sin(\theta) \cdot p(\lambda, 180) \cdot \mu_s(\lambda) = C_{app}' \cdot p(\lambda, 180) \cdot \mu_s(\lambda) \quad (3)$$

where φ is the azimuthal angle and θ is the polar angle.

[0024] Figure 3 shows the differential backscatter signal $R_{bs}(\lambda)$ of measurements (see dots) of a dilute suspension of 0.2 μm polystyrene spheres along with a calculation (see curve 32) according to Eq. (3). In figure 3 $R_{bs}(\lambda)$ is shown using arbitrary units (a.u.). Also a value of Q_{radar} where $Q_{radar} = 4\pi \cdot \rho(\lambda, 180) \cdot Q_{sca}(\lambda)$, is indicated in the figure. Figure 3 shows excellent agreement between the measurement (i.e. the dots) and the calculation, which indicates that if $mfp > d_{fiber}$, the single scattering is indeed the dominant contributor to the differential backscatter signal $R_{bs}(\lambda)$ as defined in Eq. (1).

[0025] A singly scattered photon first travels from the tip of the dc-fiber 5 to a particle, and then (the same distance) back from the particle to the tip of the de-fiber 5 (or tip of c-fiber 6), see also figure 2a. So an average path length $\tau(\lambda)$ traveled by the measured single scattered photons is equal to two times the mean free path $mfp(\lambda)$, i.e.

$$\tau(\lambda) = 2 \cdot mfp(\lambda) \quad (4)$$

In the presence of n absorbing species with specific absorption coefficients $\mu_a^{spec,i}(\lambda)$, the differential backscatter signal becomes

$$\begin{aligned} R_{bs}(\lambda) &= C_{app}' \cdot p(\lambda, 180) \cdot \mu_s(\lambda) \cdot \exp(-\tau(\lambda)) \cdot \sum_{i=1}^n \rho_i \cdot \mu_a^{spec,i}(\lambda) \\ &= C_{app}' \cdot p(\lambda, 180) \cdot \mu_s(\lambda) \cdot \exp(-2 \cdot mfp(\lambda)) \cdot \sum_{i=1}^n \rho_i \cdot \mu_a^{spec,i}(\lambda) \end{aligned} \quad (5)$$

where C_{app}' is an apparatus constant, $p(\lambda, 180)$ is the phase function, $\mu_s(\lambda)$ is the scattering coefficient of the medium, λ is the wavelength of the first and second backscattered radiation, $mfp(\lambda)$ is the mean free path as a function of the wavelength, n is the number of substances in the sample 1, ρ_i is the concentration of absorber i present in a detection volume of the sample 1, and $\mu_a^{spec,i}(\lambda)$ is the absorption coefficient of absorber i as a function of the wavelength.

[0026] It is noted that in Eq. (5) the assumption is made that absorbers are homogeneously distributed and do not influence each other. The Eq. (5) may be corrected for non-linear phenomena such as an inhomogeneous distribution of absorbers, see e.g. [8].

[0027] According to an embodiment, the specific absorption coefficients of the absorbers, the wavelength dependency of the scattering coefficient μ_s and the phase function p , together with Eq. (5) are used in order to calculate the concentrations of all the absorbing substances present in the detection volume of the sample 1. Since the detection volume is typically very small in the present invention, the extracted concentrations are highly spatially resolved. This is not possible with the known methods that are based on diffuse reflectance, and wherein the obtained concentrations are averages over large sample volumes, see e.g. [2].

[0028] The apparatus constant C_{app}' (Eq. 3) can be determined for a specific distance between the tip of the dc-fiber 5 and the reference materials (black and white spectralon). For a suspension of monodisperse polystyrene spheres of known size and concentration, the scattering coefficient μ_s and the phase function $p(180)$ can be calculated using Mie theory [4]. The apparatus constant C_{app}' simply follows from Eq. (3). In terms of the volume fraction f of the suspension, the radius of the spheres a and the radar efficiency coefficient $Q_{radar}(\lambda) = 4\pi \cdot \rho(\lambda, 180) \cdot Q_{sca}(\lambda)$ the apparatus constant is determined by

$$R_{bs}(\lambda) \approx C_{app} \cdot p(\lambda, 180) \cdot \mu_s(\lambda) = C_{app} \cdot 0.05968 \cdot \frac{f}{a} \cdot Q_{radar}(\lambda) \quad (6)$$

5 [0029] According to another embodiment, the selected diameter d_{fiber} is chosen so that the mean free path is smaller than d_{fiber} . In this embodiment, the differential backscatter signal R_{bs} is a function of the fiber diameter d_{fiber} . This will be discussed in more detail below.

10 [0030] When the mean free path of the photons is smaller than the selected fiber diameter (i.e. $mfp(\lambda) < d_{fiber}$), the contribution of multiply scattered light to the differential backscatter signal $R_{bs}(\lambda)$ of the single dc-fiber 5 cannot completely be removed using Eq. (1). In this case, it appears that the average path length of the photons contributing to the signal $R_{bs}(\lambda)$ becomes nearly independent of the optical properties of the sample 1. In this situation, multiple scattering events already occur at small distances from the tip of the dc-fiber 5. An analytical expression for the backscatter signal $R_{bs}(\lambda)$ is not available for this situation and Monte Carlo simulations were used to model the behaviour of $R_{bs}(\lambda)$ as a function of the diameter of the fibers 5, 6 and of the optical properties of the sample 1. Figure 4 shows the results of Monte Carlo simulations using the MCML-code (Monte Carlo for Multi-Layered media) of Wang et al [6,7] for a homogeneous medium with an anisotropy value $g=0.9$. A flat circular incident beam with diameter d_{fiber} is directed onto the sample 1, and the differential backscatter signal R_{bs} is calculated by subtracting the total reflectance in the c-fiber 6 (with diameter d_{fiber} and center located at a distance d_{fiber} from the center of the incident beam) from the total reflectance in the dc-fiber 5 (with diameter d_{fiber} overlapping the incident beam). Simulations were performed for sets of four different scattering coefficients ($\mu_s=15, 25, 50$ and 80 mm^{-1}), four different fiber diameters ($d_{fiber}=200, 400, 600$ and $800 \mu\text{m}$) and five different absorption coefficients ($\mu_a=0, 0.2, 0.4, 0.6$ and 0.8 mm^{-1}).

15 [0031] Figure 4 shows R_{bs} as a function of absorption coefficient μ_a where the open circles/dashed lines correspond to $d_{fiber}=200 \mu\text{m}$, the filled circles/dotted lines correspond to $d_{fiber}=400 \mu\text{m}$, the open squares/solid lines correspond to $d_{fiber}=600 \mu\text{m}$ and the filled squares/dash-dotted lines correspond to $d_{fiber}=800 \mu\text{m}$. The differential backscatter signal R_{bs} for each scattering coefficient μ_s was normalized to the ($d_{fiber}=200 \mu\text{m}$, $\mu_a=0 \text{ mm}^{-1}$) case. Figure 4 shows that in the absence of absorption, i.e. $\mu_a = 0$, the differential backscatter signal R_{bs} depends linearly on the scattering coefficient μ_s . Furthermore, the slope of the straight lines (signifying the relation between R_{bs} and μ_a) depends only on the fiber diameter and is independent of the scattering coefficient μ_s . The latter is more clearly demonstrated in figure 5, where the differential backscatter signal R_{bs} is normalized to unity at zero absorption for all scattering coefficients μ_s . The open circles correspond to $d_{fiber}=200 \mu\text{m}$ and the filled squares correspond to $d_{fiber}=800 \mu\text{m}$. These Monte Carlo simulations therefore suggest that in the situation where $mfp < d_{fiber}$, the diameter of the fibers 5, 6 determines the average path length τ of the measured photons. The backscatter signal R_{bs} for this range of parameters can thus be written as

$$R_{bs}(\lambda) = C_1 \cdot \mu_s \cdot \exp(-\tau \cdot \mu_a) = C_1 \cdot \mu_s \cdot \exp(-C_2 \cdot d_{fiber} \cdot \mu_a) \quad (7)$$

20 where C_1 and C_2 are constants, τ is the average path length, μ_a is the absorption coefficient, μ_s is the scattering coefficient and d_{fiber} is the fiber diameter of the fibers 5, 6.

25 [0032] An exact analytical expression for $R_{bs}(\lambda)$ is not available due to the large contribution of multiple scattering events to the signal. Measurements were done for determining a total integrated backscatter signal R_{tot} for a range of λ between 400-900 nm, using the formula

$$R_{tot}(\mu_s) = \int_{400\text{nm}}^{900\text{nm}} d\lambda R_{bs}(\lambda, \mu_s) \quad (8)$$

30 Figure 6 shows that the integrated total backscatter signal $R_{tot}(\mu_s)$ is proportional to $\mu_s(\lambda)$ in the relevant range of μ_s between 10-100 mm^{-1} . Therefore, in the absence of absorbers, it follows that

$$R_{bs}(\lambda) = C_{app} \cdot \mu_s(\lambda) \quad (9)$$

35 which is in agreement with the Monte Carlo simulations.

[0033] In the presence of n absorbing substances in a suspension, with specific absorption coefficients $\mu_a^{spec,i}(\lambda)$, the differential backscatter signal becomes

$$R_{bs}(\lambda) = C_{app} \cdot \mu_s(\lambda) \cdot \exp(-\tau \cdot \sum_{i=1}^n \rho_i \cdot \mu_a^{spec,i}(\lambda)) \quad (10)$$

where τ is the average path length of the detected backscattered photons and ρ_i is the concentration of the substance i .

[0034] Non-linear phenomena such as an inhomogeneous distribution of absorbers are not incorporated in Eq. (10), but can be added by the skilled person, see e.g. [8].

[0035] Figure 7 shows the measured and calculated average path length τ as a function of the average scattering coefficient $\langle \mu_s(\lambda) \rangle$ (with $500 \text{ nm} < \lambda < 700 \text{ nm}$) for $d_{fiber} = 0.4 \text{ mm}$ and for absorption coefficient $\mu_a(\lambda) = 2.0 \text{ mm}^{-1}$ at $\lambda = 600 \text{ nm}$. In figure 7 measurement are indicated by dots, the $\tau = 2 \cdot \text{mfp}$ curve is indicated by a line 71 and Monte Carlo simulations are depicted by dashed lines. Identical results were obtained for suspensions with an absorption coefficient of $\mu_a = 1.0 \text{ mm}^{-1}$ at 600 nm . The average path length τ was determined using suspensions of polystyrene spheres with different sizes and concentrations to vary the scattering coefficient $\mu_s(\lambda)$. The anisotropy g of these suspensions was in the range of 0.8-0.9. Evans Blue dye was added as an absorber, and the average path length τ was calculated from Eqs. (9) and (10) and knowledge of the concentrations and specific absorption coefficient of Evans Blue, as will be known to the skilled person.

[0036] Looking at the measured average path lengths of figure 7, it clearly shows that for large scattering coefficients ($\mu_s = 10\text{-}100 \text{ mm}^{-1}$, the range relevant for tissue) the average path length τ is independent of the scattering coefficient μ_s to within 10% and approximately equal to half the fiber diameter ($\tau \approx 0.24 \text{ mm}$ while $d_{fiber} = 0.40 \text{ mm}$), in agreement with the Monte Carlo simulations (the dashed lines correspond to Monte Carlo calculations for $d_{fiber} = 0.2, 0.4, 0.6$ and 0.8 mm). For small scattering coefficients (e.g. $\mu_s < 5 \text{ mm}^{-1}$) the average path length τ is well described by $\tau = 2 \cdot \text{mfp}$, according to Eq.(4), see line 71. Figure 7 also clearly demonstrates that the transition from the 'single scattering regime' to the 'constant path length regime' occurs for mean free paths of the order of the fiber diameter. It is therefore expected that single scattering will prevail over a larger range of scattering coefficients for fiber diameters smaller than $400 \mu\text{m}$.

[0037] In the following, the effect of absorption on the average path length τ will be examined in more detail. Various concentrations of Evans Blue dye were added to a suspension of polystyrene spheres with scattering coefficients μ_s of 35 mm^{-1} . The concentrations of Evans Blue (EB) dye were varied such that the absorption coefficient μ_a at 600 nm was in the range of 0 to 2 mm^{-1} . Typical results of the differential backscatter signal R_{bs} for three different absorption coefficients μ_a are shown in figure 8. Note that the signal I of the dc-fiber 5 is plotted on a different vertical scale than the signal J of the c-fiber 6 and the differential backscatter signal R_{bs} .

The spectra with Evans Blue R^{EB} present in the suspension were divided by the spectrum with no Evans Blue present R^0 and the negative natural logarithm of the ratio R^{EB}/R^0 was determined:

$$A = -\ln(R^{EB}/R^0) = \tau \cdot \rho \cdot \mu_a^{spec,EB} \quad (11)$$

where ρ is the concentration of Evans Blue, and $\mu_a^{spec,EB}$ is the specific absorption coefficient of Evans Blue.

[0038] Figure 9 shows a typical spectrum of an absorption curve 92, along with the specific absorption coefficient $\mu_a^{spec,EB}$ of Evans Blue dye, see curve 94.

[0039] For all concentrations, an area A^* under the absorption curve 92 was determined in the wavelength range λ between 500 and 650 nm . From Eq. (11) it follows that if the average path length τ is independent of the absorption coefficient μ_a^{spec} , area A^* should depend linearly on the concentration ρ of the species in the suspension.

[0040] Figure 10 shows a measured A^* as a function of the absorption coefficient μ_a at 600 nm . A curve fitting is done, resulting in a line for $\mu_s(\lambda) = 35 \text{ mm}^{-1}$. Figure 10 shows that the average path length τ is indeed independent of the absorption coefficient μ_a in the range $0\text{-}2 \text{ mm}^{-1}$.

[0041] From the previous results of figure 4 to 10, it shows that for $\text{mfp} < d_{fiber}$, the differential backscatter signal R_{bs} is described by Eq. (7) with $C_2 \approx 0.6$. Figure 11 shows typical spectra measured in a suspension of $1.0 \mu\text{m}$ polystyrene spheres with and without Evans Blue dye ($\mu_a = 2$ and 0 mm^{-1} at 600 nm , respectively). From Eq. (7) and figure 7, the relation between the differential backscatter signals with and without absorber is given by

$$R_{bs}(\lambda, \mu_a) = R_{bs}(\lambda, 0) \cdot \exp(-0.24 \cdot \mu_a) \quad (12)$$

5 **[0042]** The calculated spectrum according to Eq. (12) is plotted as a dashed line 110 in figure 11 and shows excellent agreement with the measured $R_{bs}(\lambda, \mu_a)$, see line 111. In figure 11, line 112 depicts $R_{bs}(\lambda, 0)$.

[0043] In short, the average path length τ of photons measured when subtracting the signals of the c-fiber 6 from the dc-fiber 5 using Eq. (1), is independent of the optical properties of the sample 1 and approximately equal to half the diameter of the fibers 5, 6 used, as long as the fiber diameter is larger than the mfp.

10 **[0044]** In a specific embodiment, the device according to the invention is arranged to determine concentrations of oxygenated blood in tissue. Since the scattering coefficient of tissue μ_s^{tissue} is in the range of 10-100 mm⁻¹, the fiber diameter should be smaller than a certain maximum diameter d_{max} where d_{max} is between 10 and 100 μm , so for example smaller than 50 nm, in order to measure predominantly single scattering in tissue. In this case, Eq. (5) holds. For fibers 15 5, 6 with much larger diameters (e.g. 200 or 400 μm), the differential backscatter signal $R_{bs}(\lambda)$ is described by Eq. (10) with $\tau \approx 0.6 \cdot d_{fiber}$.

[0045] It is presently known that the wavelength dependence of the scattering coefficient in tissue μ_s^{tissue} can be adequately described by an empirical power-law function, see also [3], [4], [5].

$$20 \mu_s^{tissue}(\lambda) = a \cdot \lambda^{-b} \quad (13)$$

25 with a and b constants that depend on the size, concentration and relative refractive index of the scatterers (i.e. substances) present in the detection volume.

The dominant absorbers in tissue in the visible wavelength range are oxygenated and deoxygenated blood. Thus in tissue Eq. (10) becomes

$$30 R_{bs}(\lambda) = C_{app} \cdot a \lambda^{-b} \cdot \exp(-0.6 \cdot d_{fiber} \cdot \rho_{blood} \cdot (S_{O_2} \cdot \mu_a^{spec,ox} + (1-S_{O_2}) \cdot \mu_a^{spec,deox}))$$

$$35 = C'_{app} \cdot \lambda^{-b} \cdot \exp(-0.6 \cdot d_{fiber} \cdot \rho_{blood} \cdot (S_{O_2} \cdot \mu_a^{spec,ox} + (1-S_{O_2}) \cdot \mu_a^{spec,deox})) \quad (14)$$

40 where ρ_{blood} is the concentration of blood, S_{O_2} is the blood oxygenation (percentage oxygen saturation) in a certain detection volume, C_{app} is a constant that depends on the calibration constant c , C'_{app} is $C_{app} \cdot a$, λ is the wavelength,

b is the slope of the scattering coefficient defined in Eq. 13, $\mu_a^{spec,ox}$ is the specific absorption coefficients of fully oxygenated blood, $\mu_a^{spec,deox}$ is the specific absorption coefficients of fully deoxygenated blood.

45 **[0046]** Non-linear phenomena such as an inhomogeneous distribution of absorbers are not incorporated in Eq. (14), but can be added by the skilled person, see e.g. [8].

[0047] Since the specific absorption coefficients of fully oxygenated ($\mu_a^{spec,ox}$) and fully deoxygenated ($\mu_a^{spec,deox}$) blood are well known, see figure 12, Eq. (14) can be fitted to the measured data to yield the slope b of the scattering

50 coefficient μ_s^{tissue} , the concentration ρ_{blood} and the oxygen saturation S_{O_2} of the blood present in the detection volume. When a correction is made for the inhomogeneous distribution of blood in the vessels, a vessel diameter D may be determined as well. Since the average detection depth is small (e.g. 0.1 mm), the blood present in the detection volume when measuring non-invasively is located in capillaries.

55 **[0048]** In figure 13, in vivo measurements of backscattering in a human trachea together with a fit using Eq. (14) are shown. The measurements are realized using a fiber diameter of 400 μm . The dots depict the measurements and curve 130 is a fitting curve. In figure 13, $b = -0.94$ and the oxygenation $S_{O_2} = 95\%$.

[0049] The present invention can be used for tumor detection. Tumor growth may, due to its excessive oxygen con-

sumption, be accompanied by a low capillary oxygen saturation, which can only be assessed using a very localized measurement. Since (pre-)cancerous tissue is generally more heterogeneous than normal tissue, the standard deviation of multiple measurements is likely to be larger for (pre-)cancerous tissue than for normal tissue. Standard deviations in the measurements can be calculated for the oxygen saturation, the blood concentration, the blood vessel diameter, and

the slope b of the scattering coefficient μ_s^{tissue} . It is noted that the invention is by no means restricted to determine a concentration of a substance as the physical feature. All features, mentioned in the previous phrase can be regarded as physical features.

[0050] An example of a measurement of a lung tumor is shown in figure 14. The shape of the dip in the wavelength range of 500-600 nm in this figure demonstrates the depletion of oxygen from the capillaries of this tumor due to its excessive oxygen consumption.

[0051] When a needle-probe is used, the local oxygenation and scattering coefficient μ_s^{tissue} can be measured invasively. This could be helpful in determining tumor-margins intra-operatively in real-time, for instance during resection of a breast-tumor.

[0052] According to an embodiment, the device comprises multiple probes and a multichannel spectrometer for multiple simultaneous measurements on different locations of the sample 1. Using this device, multiple measurements can be made simultaneously on different locations of for example a suspicious lesion.

[0053] In yet another embodiment, the device comprises at least two pairs of fibers, having different fiber diameters. For example, when a pair of fibers with 100 μm , a pair of fibers with a diameter of 200 μm and a pair of fibers with a diameter of 400 μm are used, information from different depths in the sample 1 can be obtained as the average path length increases with increasing fiber diameter.

[0054] The method and apparatus according to the invention can also be used to analyze local drug concentrations. From Eq. (10) it follows that if the specific absorption coefficient of a certain drug is known, the local concentration ρ of that substance can be determined using the invention.

[0055] Another possibility of the present invention is to monitor glucose concentrations. The scattering coefficient μ_s^{tissue} depends among others on the relative refractive index of the scatterers with respect to the surrounding medium (in tissue: cytoplasm). The refractive index of the surrounding cytoplasm is likely to depend on the concentration of glucose. A change in the glucose concentration will therefore likely affect the slope b of the scattering coefficient μ_s^{tissue} , see Eq. (13).

[0056] Whilst specific embodiments of the invention have been described above, it will be appreciated that the invention may be practiced otherwise than as described. For example, a concentration of a substance in polluted water may be calculated. The description is not intended to limit the scope of the invention as defined by the claims.

Reference

[0057]

1. A. Amelink, M.P.L. Bard, J.A. Burgers and H.J.C.M. Sterenberg, "Single scattering spectroscopy for the endoscopic analysis of particle size in superficial layers of turbid media", *Applied Optics* 42, page 4095-4101 (2003).
2. R.M.P. Doornbos, R Lang, M.C. Aalders, F.W.Cross and H.J.C.M. Sterenberg, "The determination of in vivo human tissue optical properties and absolute chromophore concentrations using spatially resolved steady-state diffuse reflectance spectroscopy", *Phys. Med. Biol.* 44 (1999) page 967-981.
3. A. Angstrom, "On the atmospheric transmission of sun radiation and on dust in the air", *Geograf. Ann. Deut.* 11, 156-166 (1929)
4. H.C. van de Hulst, "Light Scattering by Small Particles", Wiley, New York, 1957.
5. R. Graaff, J.G. Aarnoudse, J.R. Zijp, P.M.A. Sloop, F.F.M. de Mul, J. Greve, and M.H. Koelink, "Reduced light-scattering properties for mixtures of spherical particles: a simple approximation derived from Mie calculations", *Applied Optics.* 31, 1370-1376 (1992).
6. L-H Wang, S.L. Jacques, L-Q Zheng, "MCML - Monte Carlo modeling of photon transport in multi-layered tissues", *Computer Methods and Programs in Biomedicine* 47, 131-146 (1995).
7. L-H Wang, S.L. Jacques, L-Q Zheng, "CONV - Convolution for responses to a finite diameter photon beam incident on multi-layered tissues", *Computer Methods and Programs in Biomedicine* 54, 141-150 (1997).
8. R.L.P. van Veen, W. Verkrusse, and H.J.C.M. Sterenberg, "Diffuse reflectance spectroscopy from 500 to 1060 nm using correction for inhomogeneously distributed absorbers", *Opt. Lett.* 27, 246-248 (2002).

Claims

1. A method of determining of a physical feature of a medium, comprising:

- producing radiation with a light source (2);
- placing a probe on a sample (1) of said medium, said probe comprising a first optical fiber (5) having a first diameter, and at least a second optical fiber (6) having a second diameter;
- sending light coming from said light source, through said first optical fiber;
- collecting first backscattered radiation through said first optical fiber and second backscattered radiation through said second optical fiber;
- producing a first signal (I) based on said first backscattered radiation, and a second signal (J) based on said second backscattered radiation;
- determining a measured differential backscatter signal as a function of wavelength using said first and second signals (I, J),

characterized by

- calculating said physical feature by curve fitting said measured differential backscatter signal to a backscatter function, in which said backscatter function is a function of an average path-length (τ) travelled by detected scattered photons, said average path-length (τ) being independent from an absorption coefficient (μ_a) of said medium, and from a scattering coefficient (μ_s) of said medium.

2. Method according to claim 1, wherein said average path-length (τ) is also independent from a wavelength (λ) of said first and second backscattered radiation

3. Method according to claim 1, wherein said path-length (τ) is proportional to said first fiber diameter.

4. Method according to claim 1, wherein said backscatter function is given by:

$$R_{bs} = C1 \cdot \mu_s \cdot \exp(-\tau \cdot \mu_a)$$

with $\tau = C2 \cdot d_{fiber}$

where C1 and C2 are constants, μ_a = said absorption coefficient of said medium, μ_s = said scattering coefficient of said medium, and d_{fiber} = said first fiber diameter.

5. Method according to claim 4, wherein C2 is approximately 0.6.

6. Method according to any of claims 1-5, wherein said physical feature is a concentration of at least one substance in said medium.

7. A device for determining a physical feature of a medium, comprising:

- a light source (2) for producing radiation;
- a probe with at least a first and a second optical fiber (5, 6), said first optical fiber (5) having a first diameter and being arranged to deliver said radiation on a sample (1) of said medium and to collect first backscattered radiation from said sample (1), said second optical fiber (6) having a second diameter and being arranged to collect second backscattered radiation, wherein said second optical fiber (6) is positioned alongside said first optical fiber (5);
- a spectrometer (7) for producing a first signal (I) based on said first backscattered radiation, and for producing a second signal (J) based on said second backscattered radiation;
- a processor (9) arranged to determine a measured differential backscatter signal as a function of wavelength (λ) using said first and second signals (I, J),

characterized in that said processor is arranged to calculate said physical feature by curve fitting said measured differential backscatter signal to a backscatter function (R_{bs}), in which said backscatter function is a function of an average path-length (τ) travelled by detected scattered photons, said average path-length (τ) being independent

from an absorption coefficient (μ_a) of said medium, and from a scattering coefficient (μ_s) of said medium.

8. Computer program product to be loaded by a computer, said computer program product, after being loaded, providing said computer with the capacity to:

- receive a first signal (I) indicative of a collected radiation received from a first fiber (5) and a second signal (J) indicative of a collected radiation received from a second fiber (6);
- determine a measured differential backscatter signal (R_{bs}) as a function of wavelength (λ) of said collected radiation using said first and second signals (I, J);

characterized by the capacity to

- calculate a physical feature by curve fitting said measured differential backscatter signal to a backscatter function, in which said backscatter function is a function of an average path-length (τ) travelled by detected scattered photons, said average path-length (τ) being independent from an absorption coefficient (μ_a) of said medium, and from a scattering coefficient (μ_s) of said medium.

9. Data carrier provided with a computer program product according to claim 8.

10. A method of determining a physical feature of a medium, comprising:

- producing radiation with a light source (2);
- placing a probe on a sample (1) of said medium, said probe comprising a first optical fiber (5) having a first diameter, and at least a second optical fiber (6) having a second diameter;
- sending light coming from said light source, through said first optical fiber;
- collecting first backscattered radiation through said first optical fiber and second backscattered radiation through said second optical fiber;
- producing a first signal (I) based on said first backscattered radiation, and a second signal (J) based on said second backscattered radiation;
- determining a measured differential backscatter signal as a function of wavelength using said first and second signals (I, J),

characterized by

- calculating said physical feature by curve fitting said measured differential backscatter signal to a backscatter function, in which said backscatter function is a function of a mean free path of photons in the medium.

11. Method according to claim 10, wherein said backscatter function (R_{bs}) is defined by:

$$R_{bs}(\lambda) = C_{app}' \cdot p(\lambda, 180) \cdot \mu_s(\lambda) \cdot \exp(-2 \cdot mfp(\lambda)) \cdot \sum_{i=1}^n \rho_i \cdot \mu_a^{spec,i}(\lambda)$$

where C_{app}' is an apparatus constant, $p(\lambda, 180)$ is a phase function, $\mu_s(\lambda)$ is a scattering coefficient of said medium, λ is a wavelength of said first and second backscattered radiation, $mfp(\lambda)$ is said mean free path as a function of the wavelength, n is a number of substances in said medium, ρ_i is concentration of absorber i present in a detection volume of said sample (1), and $\mu_a^{spec,i}(\lambda)$ is an absorption coefficient of substance i as a function of the wavelength.

12. Method according to any of claims 10-11, wherein said physical feature is a concentration of at least one substance in said medium.

13. A device for determining a physical feature of a medium, comprising:

- a light source (2) for producing radiation;
- a probe with at least a first and a second optical fiber (5, 6), said first optical fiber (5) having a first diameter and being arranged to deliver said radiation on a sample (1) of said medium and to collect first backscattered radiation from said sample (1), said second optical fiber (6) having a second diameter and being arranged to

collect second backscattered radiation, wherein said second optical fiber (6) is positioned alongside said first optical fiber (5);

- a spectrometer (7) for producing a first signal (I) based on said first backscattered radiation, and for producing a second signal (J) based on said second backscattered radiation;

- a processor (9) arranged to determine a measured differential backscatter signal as a function of wavelength (λ) using said first and second signals (I, J),

characterized in that said processor is arranged to calculate said physical feature by curve fitting said measured differential backscatter signal to a backscatter function (R_{bs}), wherein said backscatter function is a function of a mean free path of photons.

14. Computer program product to be loaded by a computer, said computer program product, after being loaded, providing said computer with the capacity to:

- receive a first signal (I) indicative for a collected radiation received from a first fiber (5) and a second signal (J) indicative for a collected radiation received from a second fiber (6);

- determine a measured differential backscatter signal (R_{bs}) as a function of wavelength (λ) of said collected radiation using said first and second signals (I, J);

characterized by the capacity to

- calculate a physical feature by curve fitting said measured differential backscatter signal to a backscatter function, wherein said backscatter function is a function of a mean free path of photons.

15. Data carrier provided with a computer program product according to claim 14.

16. Method according to any of the claim 1-6, 10-12 wherein said method comprises:

- simultaneously measuring backscatter radiation on different locations of said sample (1);

- determining a physical feature for said different locations;

- calculating a standard deviation of said physical feature.

Patentansprüche

1. Verfahren

zur Bestimmung einer physikalischen Eigenschaft eines Mediums,
mit nachstehenden Verfahrensschritten:

- mit Hilfe einer Lichtquelle (2) wird Lichtstrahlung erzeugt;

- eine Sonde wird an einer Probe (1) des Mediums angeordnet,

wobei diese Sonde eine erste Lichtleitfaser (5) mit einem ersten Durchmesser und wenigstens eine zweite Lichtleitfaser (6) mit einem zweiten Durchmesser aufweist;

- von der Lichtquelle stammendes Licht wird durch diese erste Lichtleitfaser geleitet;

- mit Hilfe der ersten Lichtleitfaser wird erste Rückstreustrahlung gesammelt, und mit Hilfe der zweiten Lichtleitfaser wird zweite Rückstreustrahlung gesammelt;

- es wird ein erstes Signal (I) erzeugt, das auf dieser ersten Rückstreustrahlung beruht, und es wird ein zweites Signal (J) erzeugt, das auf dieser zweiten Rückstreustrahlung beruht;

- als Funktion der in diesem ersten Signal (I) und in diesem zweiten Signal (J) verwendeten Wellenlänge wird ein gemessenes Differentialrückstreusignal bestimmt;

dadurch gekennzeichnet, dass

- diese physikalische Eigenschaft berechnet wird durch Kurvenanpassung dieses gemessenen Differentialrückstreusignals an eine Rückstreufunktion, wobei es sich bei dieser Rückstreufunktion um eine Funktion der mittleren Weglänge (τ) handelt, welche die erfassten gestreuten Photonen zurückgelegt haben,

wobei diese mittlere Weglänge (τ) unabhängig ist von einem Absorptionskoeffizienten (μ_a) dieses Mediums und

EP 1 664 745 B1

von einem Streukoeffizienten (μ_s) dieses Mediums.

2. Verfahren nach Anspruch 1,
wobei

5 diese mittlere Weglänge (τ) auch unabhängig ist von einer Wellenlänge (λ) dieser ersten Rückstreustrahlung und dieser zweiten Rückstreustrahlung.

3. Verfahren nach Anspruch 1,
wobei

10 diese Weglänge (T) proportional ist zum Durchmesser dieser ersten Lichtleitfaser.

4. Verfahren nach Anspruch 1,
wobei

15 diese Rückstrefunktion gegeben ist durch:

$$R_{bs} = C1 \cdot \mu_s \cdot \exp(-\tau \cdot \mu_a)$$

20 mit: $T = C2 \cdot d_{Faser}$
wobei:

C1 und C2 sind Konstanten;

μ_a = der Absorptionskoeffizient dieses Mediums;

25 μ_s = der Streukoeffizient dieses Mediums; und

d_{Faser} = der Durchmesser dieser ersten Lichtleitfaser.

5. Verfahren nach Anspruch 4,
wobei

30 C2 angenähert den Wert 0,6 hat.

6. Verfahren nach einem der Ansprüche 1 bis 5,
wobei

35 es sich bei dieser physikalischen Eigenschaft um die Konzentration von wenigstens einer Substanz handelt, die in diesem Medium enthalten ist.

7. Vorrichtung

zur Bestimmung einer physikalischen Eigenschaft eines Mediums,

mit:

- 40
- einer Lichtquelle (2) zur Erzeugung von Lichtstrahlung;
 - einer Sonde mit wenigstens einer ersten Lichtleitfaser (5) und mit wenigstens einer zweiten Lichtleitfaser (6), wobei diese erste Lichtleitfaser (5) einen ersten Durchmesser hat und so angeordnet und ausgebildet ist, dass sie diese Lichtstrahlung einer Probe (1) dieses Mediums zuführt, und dass sie die an dieser Probe (1) gestreute, erste Rückstreustrahlung sammelt, und
 - 45 wobei diese zweite Lichtleitfaser (6) einen zweiten Durchmesser hat und so angeordnet und ausgebildet ist, dass sie eine zweite Rückstreustrahlung sammelt, wobei diese zweite Lichtleitfaser (6) längs dieser ersten Lichtleitfaser (5) angeordnet ist;
 - einem Spektrometer (7), um ein, auf dieser ersten Rückstreustrahlung beruhendes erstes Signal (I) zu erzeugen, und um ein, auf dieser zweiten Rückstreustrahlung beruhendes zweites Signal (J) zu erzeugen;
 - 50 - einem Prozessor (9), der so angeordnet und ausgebildet ist, dass er als Funktion der in diesem ersten Signal (I) und in diesem zweiten Signal (J) verwendeten Wellenlänge ein gemessenes Differentialrückstreusignal bestimmt;

55 **dadurch gekennzeichnet, dass**

- dieser Prozessor so angeordnet und ausgebildet ist, dass er diese physikalische Eigenschaft berechnet durch Kurvenanpassung dieses gemessenen Differentialrückstreusignals an eine Rückstrefunktion (R_{bs}),

EP 1 664 745 B1

wobei es sich bei dieser Rückstreuungsfunktion um eine Funktion der mittleren Weglänge (T) handelt, die erfasste gestreute Photonen zurückgelegt haben,
wobei diese mittlere Weglänge (T) unabhängig ist von einem Absorptionskoeffizienten (μ_a) dieses Mediums und von einem Streukoeffizienten (μ_s) dieses Mediums.

- 5
8. Computerprogrammprodukt,
mit dem ein Computer geladen wird,
wobei dieses Computerprogrammprodukt - nach dem Ladevorgang - diesen Computer in die Lage versetzt:
- 10
- ein erstes Signal (I) zu empfangen, das die gesammelte Strahlung angibt, die von dieser ersten Lichtleitfaser (5) aufgenommen worden ist, und
 - ein zweites Signal (J) zu empfangen, das die gesammelte Strahlung angibt, die von einer zweiten Lichtleitfaser (6) aufgenommen worden ist;
 - ein gemessenes Differentialrückstreusignal (R_{bs}) zu bestimmen als Funktion der Wellenlänge (λ) dieser gesammelten Strahlung, die bei diesem ersten Signal (I) und bei diesem zweiten Signal (J) verwendet worden ist;
- 15

dadurch gekennzeichnet, dass

der Computer in die Lage versetzt worden ist:

- 20
- eine physikalische Eigenschaft **dadurch** zu berechnen, dass eine Kurvenanpassung dieses gemessenen Differentialrückstreusignals an eine Rückstreuungsfunktion vorgenommen wird,

wobei es sich bei dieser Rückstreuungsfunktion um eine Funktion der mittleren Weglänge (T) handelt, die erfasste gestreute Photonen zurückgelegt haben,
wobei diese mittlere Weglänge (T) unabhängig ist von einem Absorptionskoeffizienten (μ_a) dieses Mediums und von einem Streukoeffizienten (μ_s) dieses Mediums.

25

9. Datenträger,
der mit einem Computerprogrammprodukt nach Anspruch 8 versehen ist.
- 30

10. Verfahren
zur Bestimmung einer physikalischen Eigenschaft eines Mediums,
mit nachstehenden Verfahrensschritten:

- 35
- mit Hilfe einer Lichtquelle (2) wird Lichtstrahlung erzeugt;
 - eine Sonde wird an einer Probe (1) des Mediums angeordnet,
wobei diese Sonde eine erste Lichtleitfaser (5) mit einem ersten Durchmesser und wenigstens eine zweite Lichtleitfaser (6) mit einem zweiten Durchmesser aufweist;
 - von der Lichtquelle stammendes Licht wird durch diese erste Lichtleitfaser geleitet;
- 40
- mit Hilfe der ersten Lichtleitfaser wird erste Rückstreustrahlung gesammelt, und mit Hilfe der zweiten Lichtleitfaser wird zweite Rückstreustrahlung gesammelt;
 - es wird ein erstes Signal (I) erzeugt, das auf dieser ersten Rückstreustrahlung beruht, und es wird ein zweites Signal (J) erzeugt, das auf dieser zweiten Rückstreustrahlung beruht;
 - als Funktion der in diesem ersten Signal (I) und in diesem zweiten Signal (J) verwendeten Wellenlänge wird ein gemessenes Differentialrückstreusignal bestimmt;
- 45

dadurch gekennzeichnet, dass

- 50
- diese physikalische Eigenschaft berechnet wird durch Kurvenanpassung dieses gemessenen Differentialrückstreusignals an eine Rückstreuungsfunktion,

wobei es sich bei dieser Rückstreuungsfunktion um eine Funktion der mittleren freien Weglänge der Photonen in diesem Medium handelt.

- 55
11. Verfahren nach Anspruch 10,
wobei
diese Rückstreuungsfunktion (R_{bs}) gegeben ist durch:

$$R_{bs}(\lambda) = C_{app}' \cdot p(\lambda, 180) \cdot \mu_s(\lambda) \cdot \exp(-2 \cdot mfp(\lambda)) \cdot \sum_{i=1}^n \rho_i \cdot \mu_a^{spec,i}(\lambda)$$

5

wobei:

C_{app}' ist eine Apparatekonstante;

$p(\lambda, 180)$ ist eine Phasenfunktion;

10

$\mu_s(\lambda)$ ist ein Streukoeffizient dieses Mediums;

λ ist eine Wellenlänge dieser ersten Rückstreustrahlung und dieser zweiten Rückstreustrahlung;

$mfp(\lambda)$ ist diese mittlere freie Weglänge als Funktion der Wellenlänge;

n bezeichnet die Anzahl der Substanzen, die in diesem Medium enthalten sind;

ρ_i ist die Konzentration eines Absorbers i , der in einem Erfassungsvolumen dieser Probe (1) vorhanden ist; und

15

$\mu_a^{spec,i}(\lambda)$ ist ein Absorptionskoeffizient der Substanz i als Funktion der Wellenlänge.

12. Verfahren nach einem der Ansprüche 10 oder 11,

wobei

es sich bei dieser physikalischen Eigenschaft um die Konzentration von wenigstens einer Substanz handelt, die in diesem Medium enthalten ist.

20

13. Vorrichtung

zur Bestimmung einer physikalischen Eigenschaft eines Mediums,

mit

25

- einer Lichtquelle (2) zur Erzeugung von Lichtstrahlung;

- einer Sonde mit wenigstens einer ersten Lichtleitfaser (5) und mit wenigstens einer zweiten Lichtleitfaser (6),

wobei diese erste Lichtleitfaser (5) einen ersten Durchmesser hat und so angeordnet und ausgebildet ist, dass sie diese Lichtstrahlung einer Probe (1) dieses Mediums zuführt; und dass sie die an dieser Probe (1) gestreute

30

erste Rückstreustrahlung sammelt, und

wobei diese zweite Lichtleitfaser (6) einen zweiten Durchmesser hat und so angeordnet und ausgebildet ist, dass sie eine zweite Rückstreustrahlung sammelt,

wobei diese zweite Lichtleitfaser (6) längs dieser ersten Lichtleitfaser (5) angeordnet ist;

- einem Spektrometer (7), um ein, auf dieser ersten Rückstreustrahlung beruhendes erstes Signal (I) zu erzeugen, und um ein, auf dieser zweiten Rückstreustrahlung beruhendes zweites Signal (J) zu erzeugen;

35

- einem Prozessor (9) der so angeordnet und ausgebildet ist, dass er als Funktion der in diesem ersten Signal (I) und in diesem zweiten Signal (J) verwendeten Wellenlänge ein gemessenes Differentialrückstreusignal

bestimmt;

40

dadurch gekennzeichnet, dass

- dieser Prozessor so angeordnet und ausgebildet ist, dass er diese physikalische Eigenschaft berechnet durch Kurvenanpassung dieses gemessenen Differentialrückstreusignals an eine Rückstreufunktion (R_{bs}),

45

wobei es sich bei dieser Rückstreufunktion (R_{bs}) um eine Funktion einer mittleren freien Weglänge (T) von Photonen handelt,

14. Computerprogrammprodukt,

mit dem ein Computer geladen wird,

50

wobei dieses Computerprogrammprodukt - nach dem Ladevorgang - diesen Computer in die Lage versetzt:

- ein erstes Signal (I) zu empfangen, das eine gesammelte Strahlung angibt, die von einer ersten Lichtleitfaser (5) aufgenommen worden ist, und

ein zweites Signal (J) zu empfangen, das die gesammelte Strahlung angibt, die von einer zweiten Lichtleitfaser (6) gesammelt worden ist;

55

- ein gemessenes Differentialrückstreusignal (R_{bs}) zu bestimmen, als Funktion der Wellenlänge (λ) dieser gesammelten Strahlung, die bei diesem ersten Signal (I) und bei diesem zweiten Signal (J) verwendet worden ist;

dadurch gekennzeichnet, dass

der Computer in die Lage versetzt worden ist:

- eine physikalische Eigenschaft **dadurch** zu berechnen, dass eine Kurvenanpassung dieses gemessenen Differentialrückstreusignals an eine Rückstreuungsfunktion vorgenommen wird,

wobei es sich bei dieser Rückstreuungsfunktion um eine Funktion der mittleren freien Weglänge von Photonen handelt.

15. Datenträger,

der mit einem Computerprogrammprodukt nach Anspruch 14 versehen ist.

16. Verfahren nach einem der Ansprüche 1 bis 6 und 10 bis 12,

wobei

dieses Verfahren nachstehende Verfahrensschritte aufweist:

- Rückstreustrahlung gleichzeitig an verschiedenen Orten dieser Probe (1) gemessen wird;
- eine physikalische Eigenschaft für diese verschiedenen Orte bestimmt wird; und
- eine Standardabweichung dieser physikalischen Eigenschaft berechnet wird.

Revendications

1. Procédé pour déterminer une caractéristique physique d'un support, comportant les étapes consistant à :

- produire une radiation avec une source lumineuse (2) ;
- placer une sonde sur un échantillon (1) dudit support, ladite sonde comportant une première fibre optique (5) présentant un premier diamètre, et au moins une seconde fibre optique (6) présentant un second diamètre ;
- envoyer de la lumière provenant de ladite source lumineuse, à travers ladite première fibre optique ;
- collecter une première radiation rétrodiffusée à travers ladite première fibre optique et une seconde radiation rétrodiffusée à travers ladite seconde fibre optique ;
- produire un premier signal (I) sur la base de ladite première radiation rétrodiffusée, et un second signal (J) sur la base de ladite seconde radiation rétrodiffusée ;
- déterminer un signal de rétrodiffusion différentielle mesuré en tant qu'une fonction de longueur d'onde utilisant lesdits premier et second signaux (I, J),

caractérisé par les étapes consistant à

- calculer ladite entité physique en lissant ledit signal de rétrodiffusion différentielle mesuré en une fonction de rétrodiffusion, dans lequel ladite fonction de rétrodiffusion est une fonction d'une longueur de cheminement moyenne (τ) utilisée par des photons diffusés détectés, ladite longueur de cheminement moyenne (τ) étant indépendante d'un coefficient d'absorption (μ_a) dudit support, et d'un coefficient de diffusion (μ_s) dudit support.

2. Procédé selon la revendication 1, dans lequel ladite longueur de cheminement moyenne (τ) est aussi indépendante de la longueur d'onde (λ) desdites première et seconde radiations rétrodiffusées.

3. Procédé selon la revendication 1, dans lequel ladite longueur de cheminement (τ) est proportionnelle audit premier diamètre de fibre.

4. Procédé selon la revendication 1, dans lequel ladite fonction de rétrodiffusion est donnée par :

$$R_{bs} = C1 * \mu_s * \exp(-\tau * \mu_a)$$

avec $\tau = C2 * d_{\text{fiber}}$

où C1 et C2 sont constants, μ_a = ledit coefficient d'absorption dudit support, μ_s = ledit coefficient de diffusion dudit support, et d_{fiber} = ledit diamètre de première fibre.

EP 1 664 745 B1

5. Procédé selon la revendication 4, dans lequel C2 vaut approximativement 0,6.
6. Procédé selon l'une quelconque des revendications 1 à 5, dans lequel ladite entité physique est une concentration d'au moins une substance dans ledit support.

5

7. Dispositif pour déterminer une entité physique d'un support, comportant :

- une source lumineuse (2) pour produire une radiation ;
- une sonde avec au moins une première et une seconde fibre optique (5, 6) ladite première fibre optique (5) présentant un premier diamètre et étant disposée pour délivrer ladite radiation à un échantillon (1) dudit support et pour collecter la première radiation rétrodiffusée dudit échantillon (1), ladite seconde fibre optique (6) présentant un second diamètre et étant disposée pour collecter une seconde radiation rétrodiffusée, dans lequel ladite seconde fibre optique (6) est positionnée le long de ladite première fibre optique (5) ;
- un spectromètre (7) pour générer un premier signal (I) sur la base de la première radiation rétrodiffusée, et pour générer un second signal (J) sur la base de la seconde radiation rétrodiffusée ;
- un processeur (9) disposé pour déterminer un signal de rétrodiffusion différentielle mesuré en tant qu'une fonction de longueur d'onde (λ) utilisant lesdits premier et second signaux (I, J),

10

15

caractérisé en ce que ledit processeur est disposé pour calculer ladite entité physique en lissant ledit signal de rétrodiffusion différentielle mesuré en une fonction de rétrodiffusion (R_{bs}), dans lequel ladite fonction de rétrodiffusion est une fonction d'une longueur de cheminement moyenne (τ) utilisée par des photons diffusés détectés, ladite longueur de cheminement moyenne (τ) étant indépendante d'un coefficient d'absorption (μ_a) dudit support, et d'un coefficient de diffusion (μ_s) dudit support.

20

- 25 8. Produit-programme informatique à charger sur un ordinateur, ledit produit-programme informatique, après avoir été chargé, délivrant audit ordinateur la capacité de :

- recevoir un premier signal (I) révélateur d'une radiation collectée reçue d'une première fibre (5) et un second signal (J) révélateur d'une radiation collectée reçue d'une seconde fibre (6) ;
- déterminer un signal de rétrodiffusion différentielle mesuré (R_{bs}) en tant qu'une fonction de longueur d'onde (λ) de ladite radiation collectée utilisant lesdits premier et second signaux (I, J).

30

caractérisé par la capacité de

- calculer une entité physique en lissant ledit signal de rétrodiffusion différentielle mesuré en une fonction de rétrodiffusion, dans laquelle ladite fonction de rétrodiffusion est une fonction d'une longueur de cheminement moyenne (τ) utilisée par des photons diffusés détectés, ladite longueur de cheminement moyenne (τ) étant indépendante d'un coefficient d'absorption (μ_a) dudit support, et d'un coefficient de diffusion (μ_s) dudit support.

35

- 40 9. Support de données délivré avec un produit-programme selon la revendication 8.

10. Procédé de détermination d'une entité physique d'un support, comportant les étapes consistant à :

- produire une radiation avec une source lumineuse (2) ;
- placer une sonde sur un échantillon (1) dudit support, ladite sonde comportant une première fibre optique (5) présentant un premier diamètre, et au moins une seconde fibre optique (6) présentant un second diamètre ;
- envoyer de la lumière provenant de ladite source lumineuse, à travers ladite première fibre optique ;
- collecter une première radiation rétrodiffusée à travers ladite première fibre optique et une seconde radiation rétrodiffusée à travers ladite seconde fibre optique ;
- produire un premier signal (I) sur la base de ladite première radiation rétrodiffusée, et un second signal (J) sur la base de ladite seconde radiation rétrodiffusée ;
- déterminer un signal de rétrodiffusion différentielle mesuré en tant qu'une fonction de longueur d'onde utilisant lesdits premier et second signaux (I, J),

45

50

caractérisé par les étapes consistant à

- calculer ladite entité physique en lissant ledit signal de rétrodiffusion différentielle mesuré en une fonction de rétrodiffusion, dans lequel ladite fonction de rétrodiffusion est une fonction d'un libre parcours moyen de photons

55

dans le support.

11. Procédé selon la revendication 10, dans lequel ladite fonction de rétrodiffusion (R_{bs}) est définie par :

5

$$R_{bs}(\lambda) = C_{app}' \cdot p(\lambda, 180) \cdot \mu_s(\lambda) \cdot \exp(-2 \cdot mfp(\lambda)) \cdot \sum_{i=1}^n \rho_i \cdot \mu_a^{spec,i}(\lambda)$$

10 ou C_{app}' est une constante de dispositif, $p(\lambda, 180)$ est une fonction de phase, $\mu_s(\lambda)$ est un coefficient de diffusion dudit support, λ est une longueur d'onde de ladite première et seconde radiation rétrodiffusée, $mfp(\lambda)$ est ledit parcours libre moyen en tant qu'une fonction de la longueur d'onde, n est un nombre de substances dans ledit support, ρ_i est une concentration d'absorbeur i présent dans un volume de détection dudit échantillon (1), et $\mu_a^{spec,i}(\lambda)$ est un coefficient d'absorption de substance i en tant que fonction de la longueur d'onde.

15

12. Procédé selon l'une quelconque des revendications 10 et 11, dans lequel ladite entité physique est une concentration d'au moins une substance dans ledit support.

13. Dispositif pour déterminer une entité physique d'un support, comportant :

20

- une source lumineuse (2) pour produire une radiation ;
- une sonde avec au moins une première et une seconde fibre optique (5, 6) ladite première fibre optique (5) présentant un premier diamètre et étant disposée pour délivrer ladite radiation à l'échantillon (1) dudit support et pour collecter la première radiation rétrodiffusée dudit échantillon (1), ladite seconde fibre optique (6) présentant un second diamètre et étant disposée pour collecter une seconde radiation rétrodiffusée, dans lequel ladite seconde fibre optique (6) est positionnée le long de ladite première fibre optique (5) ;
- un spectromètre (7) pour générer un premier signal (I) sur la base de la première radiation rétrodiffusée, et pour générer un second signal (J) sur la base de la seconde radiation rétrodiffusée ;
- un processeur (9) disposé pour déterminer un signal de rétrodiffusion différentielle mesuré en tant qu'une fonction de longueur d'onde (λ) utilisant lesdits premier et second signaux (I, J),
- **caractérisé en ce que** ledit processeur est disposé pour calculer ladite entité physique en lissant ledit signal de rétrodiffusion différentielle mesuré en une fonction de rétrodiffusion (R_{bs}), dans lequel ladite fonction de rétrodiffusion est une fonction d'un parcours libre moyen de photons.

25

30

35

14. Produit-programme informatique à charger sur un ordinateur, ledit produit-programme informatique, après avoir été chargé, délivrant audit ordinateur la capacité de :

40

- recevoir un premier signal (I) révélateur d'une radiation collectée reçue d'une première fibre (5) et un second signal (J) révélateur d'une radiation collectée reçue d'une seconde fibre (6) ;
- déterminer un signal de rétrodiffusion différentielle mesuré (R_{bs}) en tant qu'une fonction de longueur d'onde (λ) de ladite radiation collectée utilisant lesdits premier et second signaux (I, J).

caractérisé par la capacité de

45

- calculer une entité physique en lissant ledit signal de rétrodiffusion différentielle mesuré en une fonction de rétrodiffusion, dans laquelle ladite fonction de rétrodiffusion est une fonction d'un parcours libre moyen de photons.

15. Support de données délivré avec un produit-programme selon la revendication 14.

50

16. Procédé selon l'une quelconque des revendications 1 à 6, 10 à 12 dans lequel ledit procédé comporte les étapes consistant à :

55

- mesurer simultanément une radiation de radiodiffusion à différents endroits dudit échantillon (1) ;
- déterminer une caractéristique physique pour lesdits différents emplacements.
- calculer une déviation standard de ladite caractéristique physique.

Fig 1

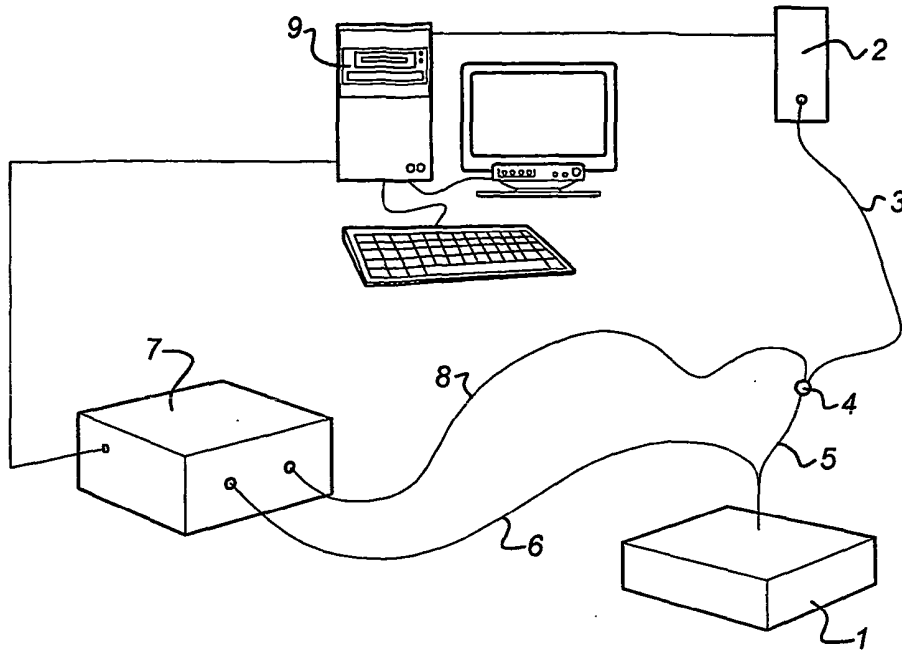


Fig 2a

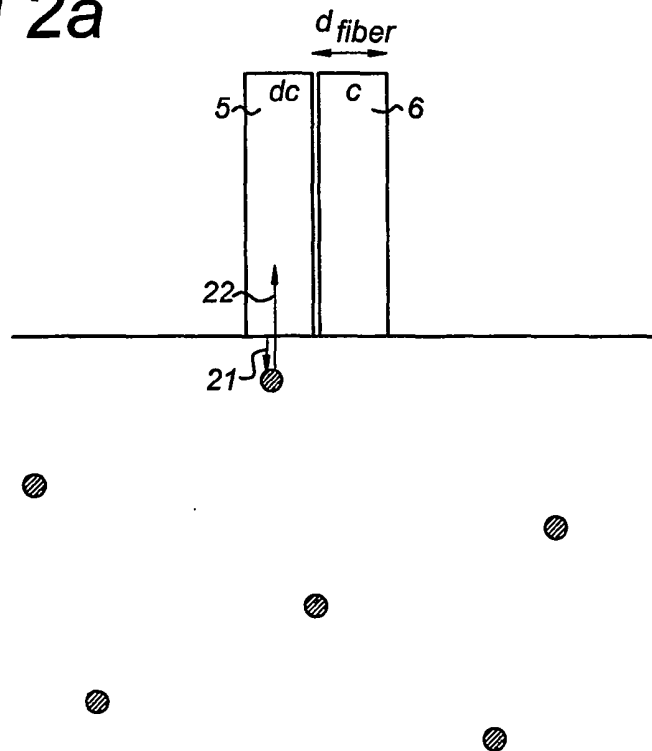


Fig 2b

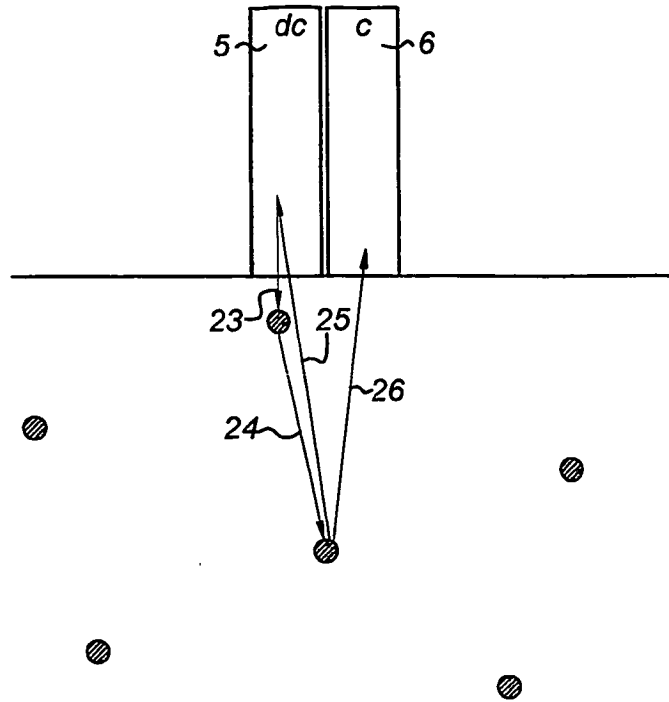
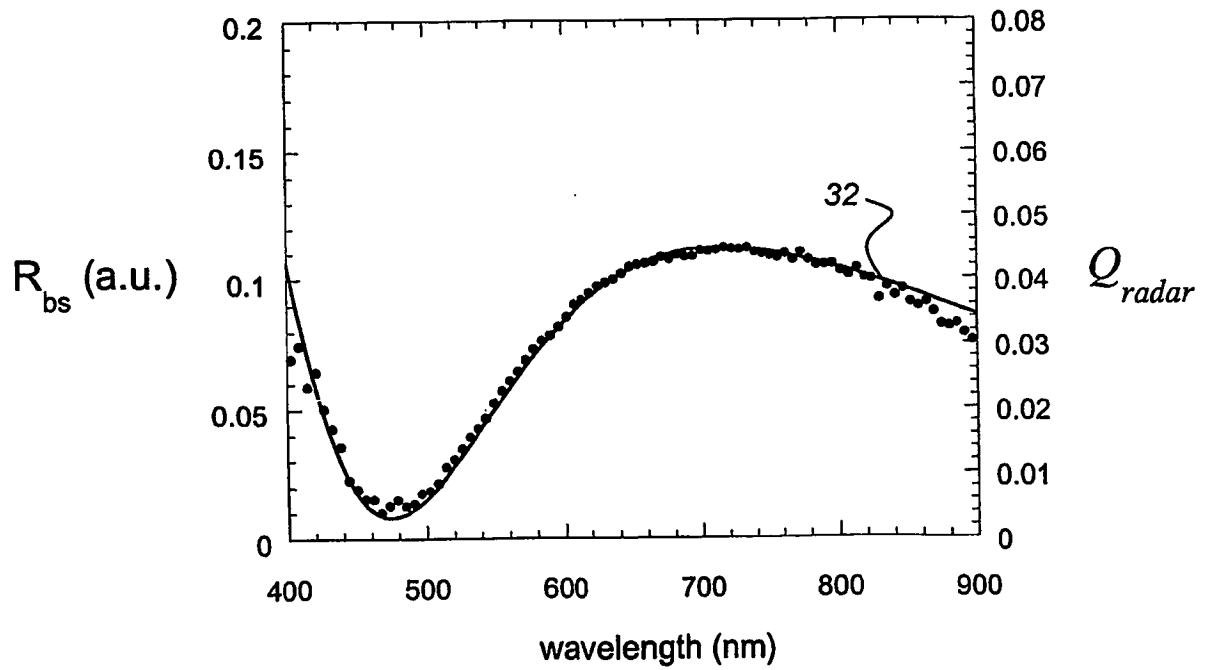


Fig 3



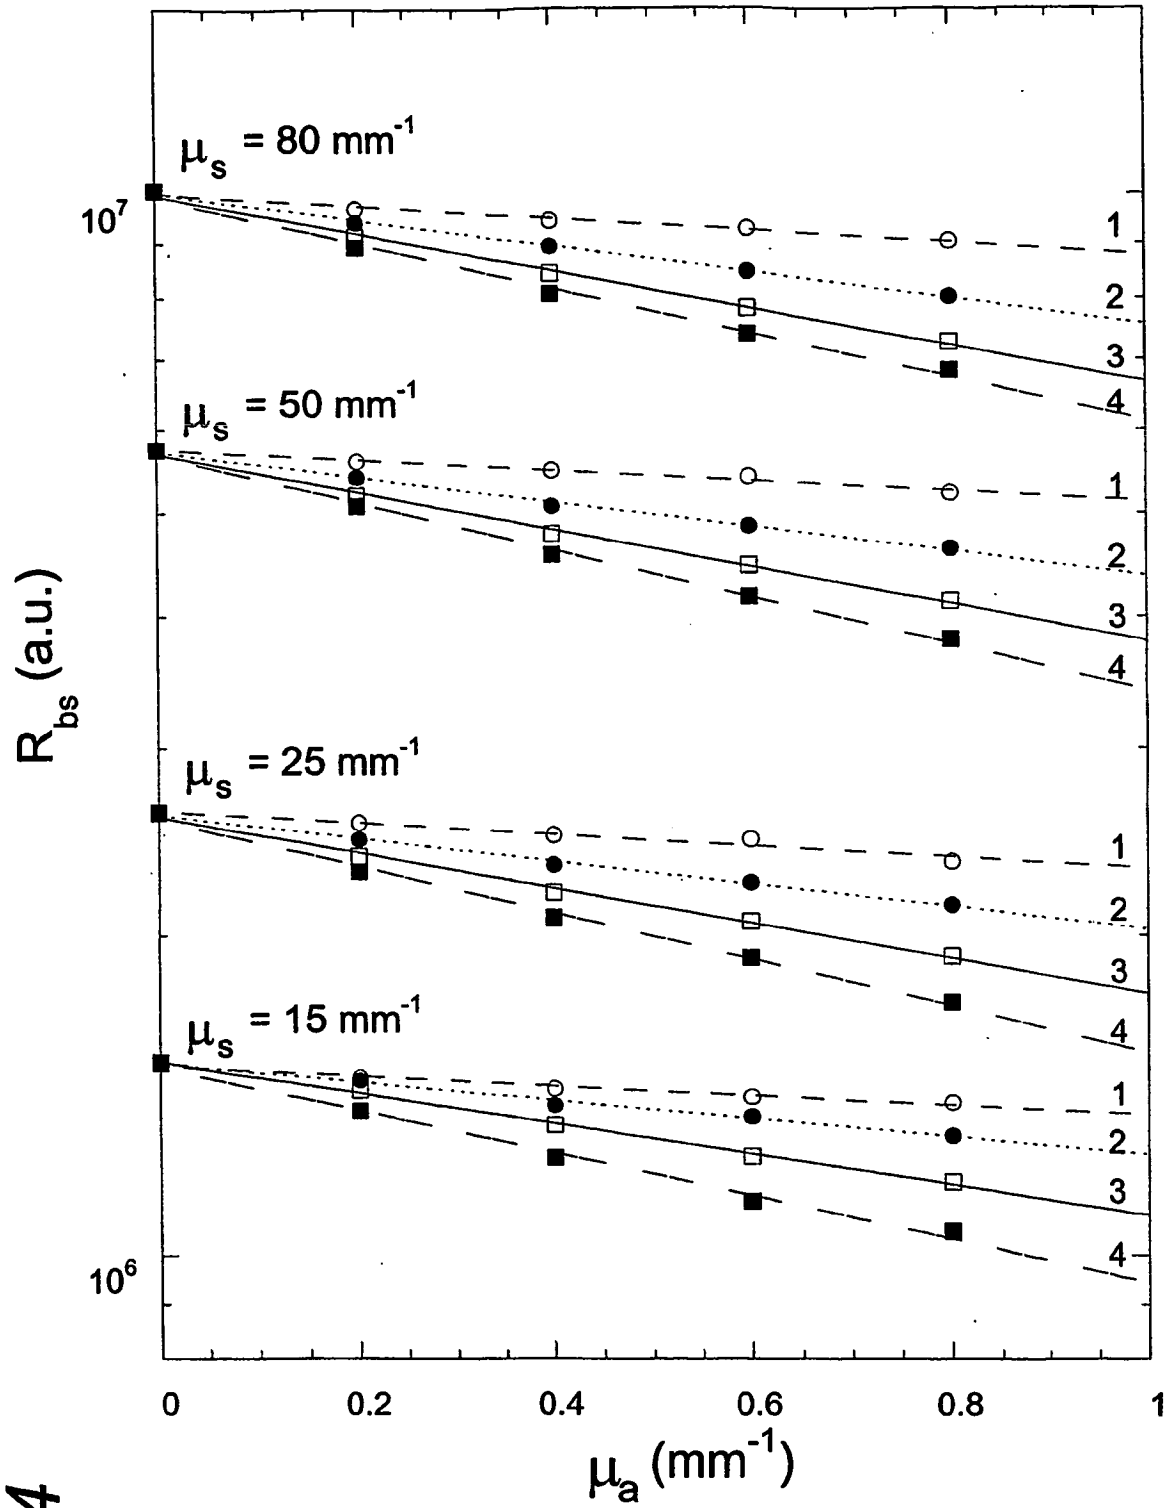


Fig 4

Fig 5

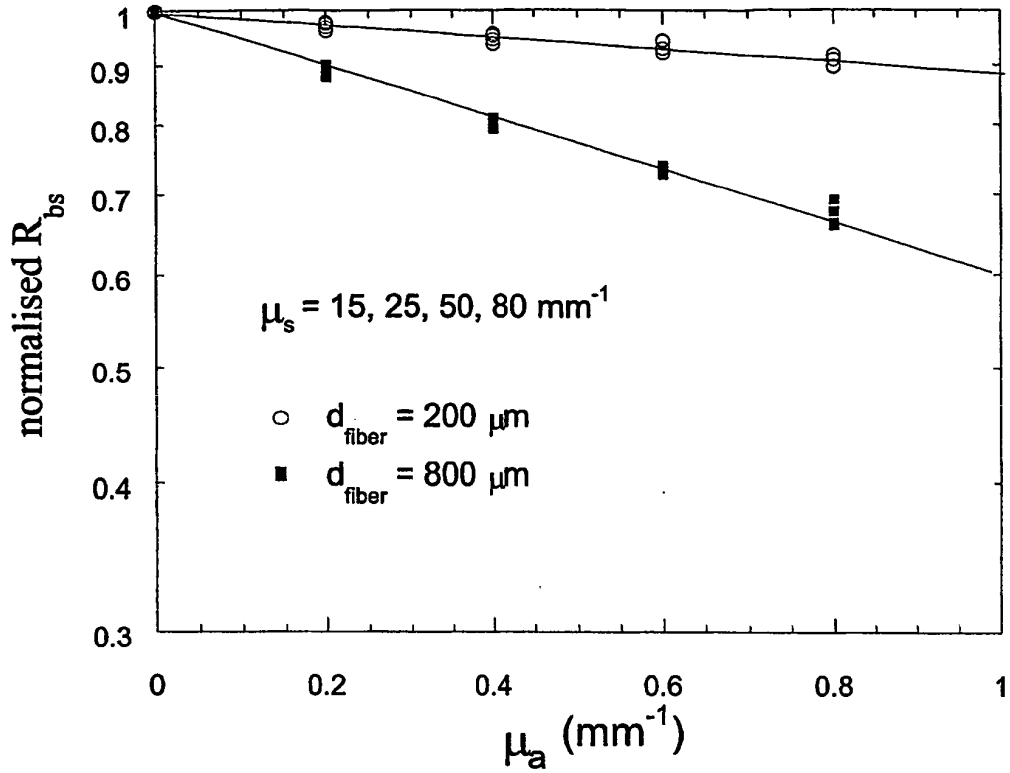


Fig 6

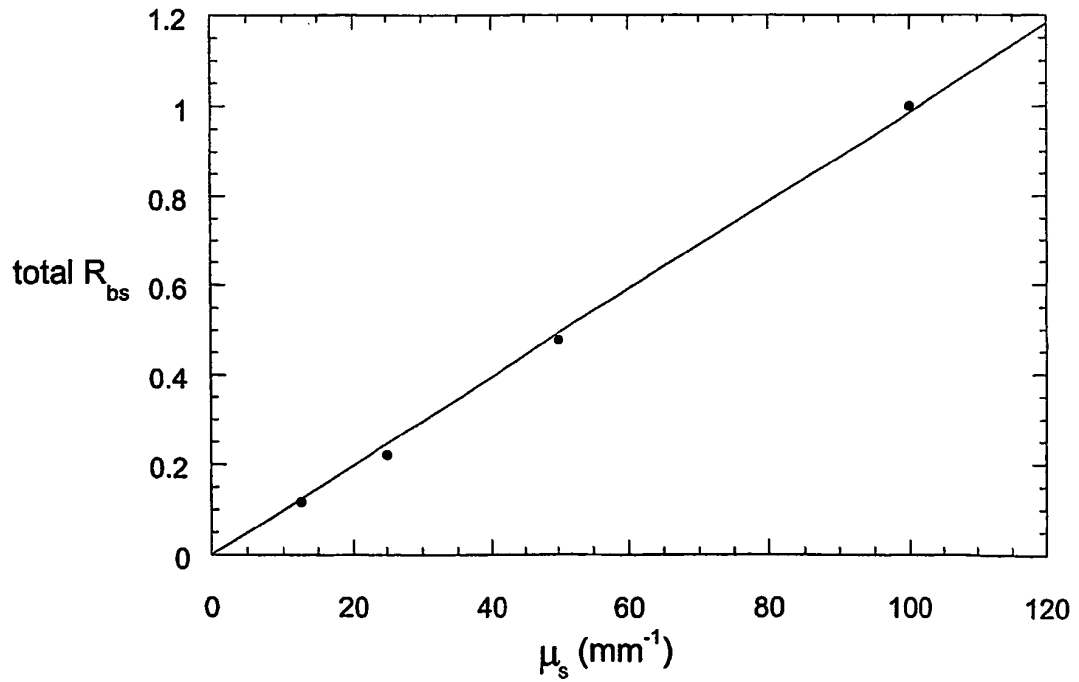


Fig 7

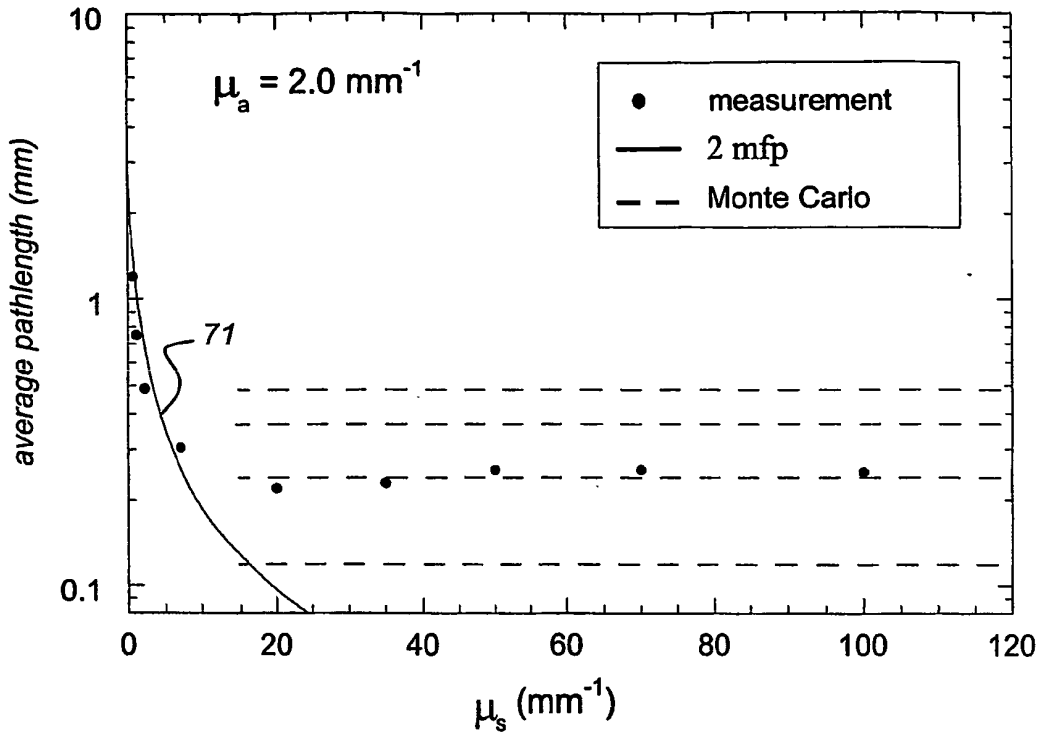


Fig 8

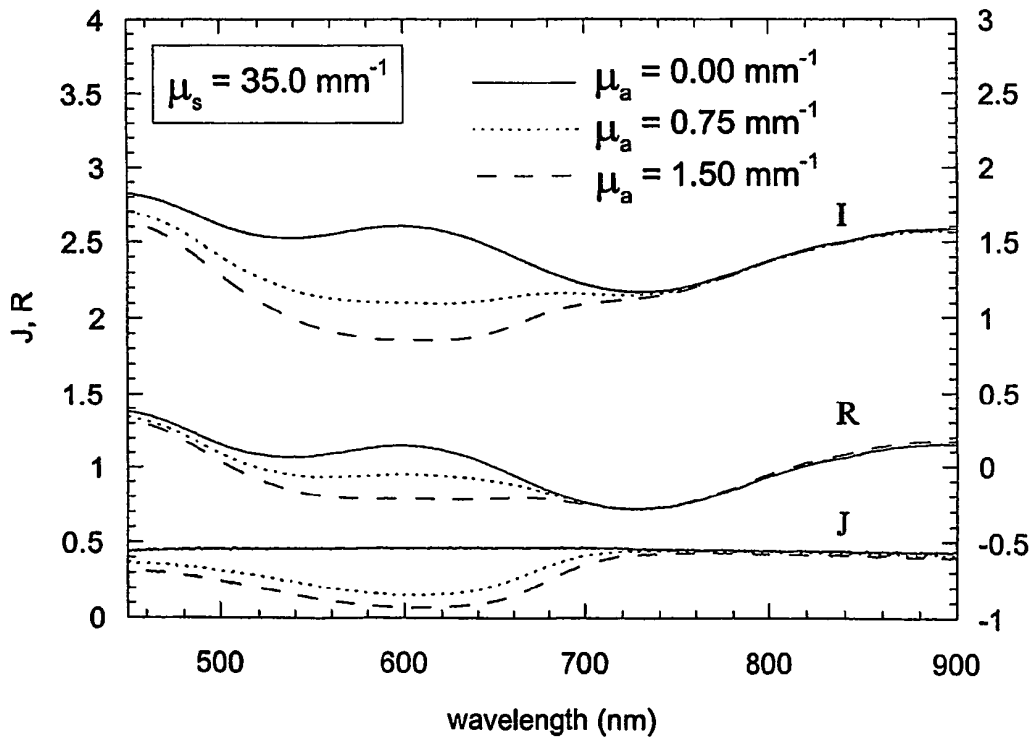


Fig 9

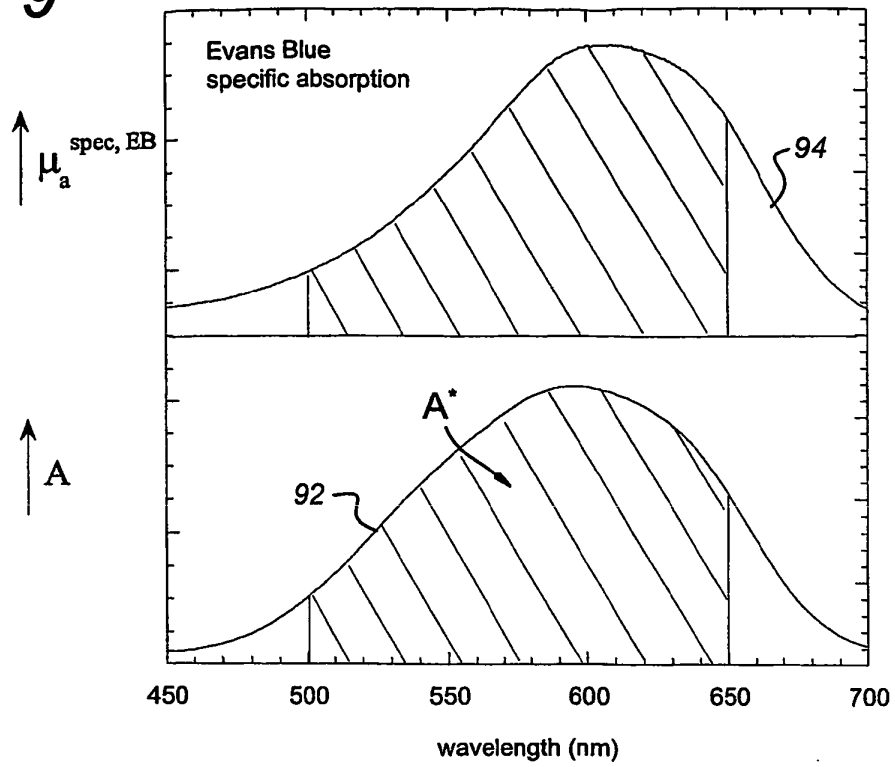


Fig 10

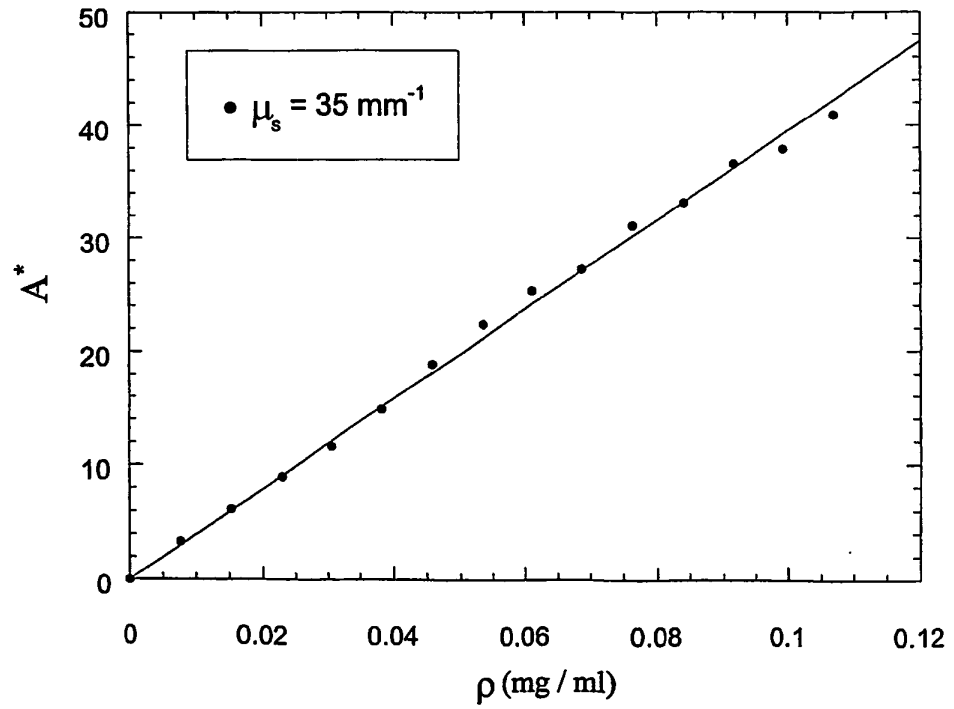


Fig 11

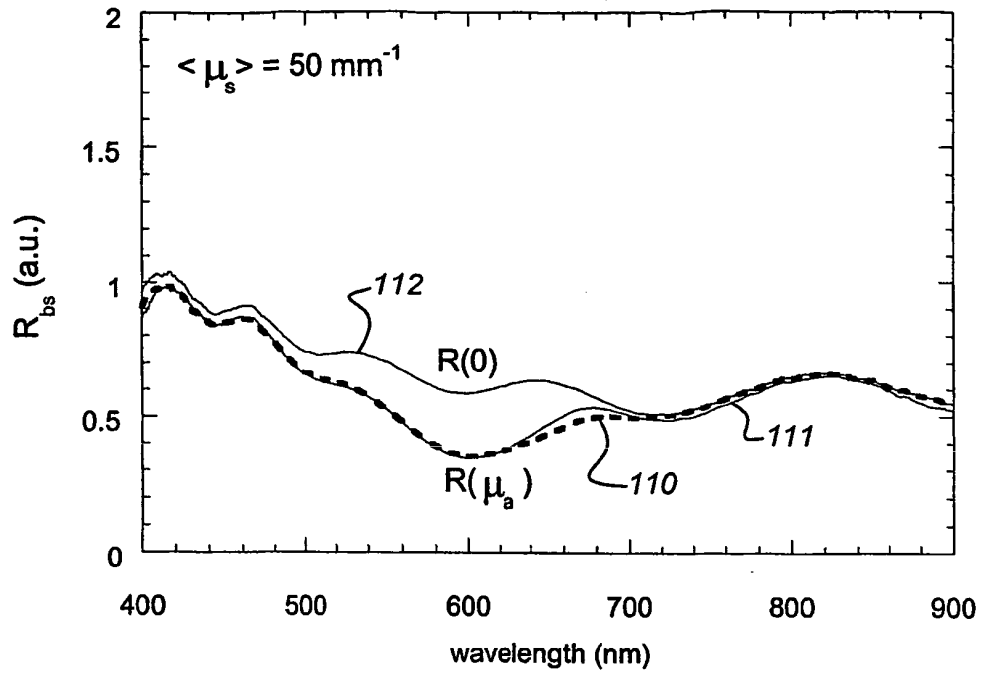


Fig 12

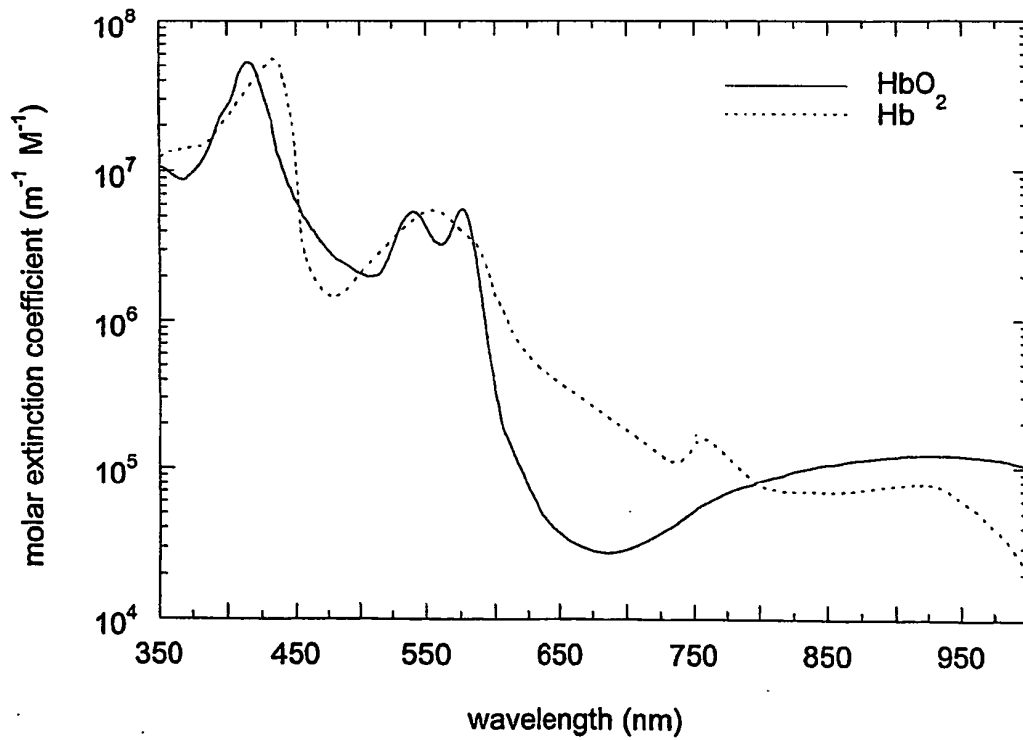


Fig 13


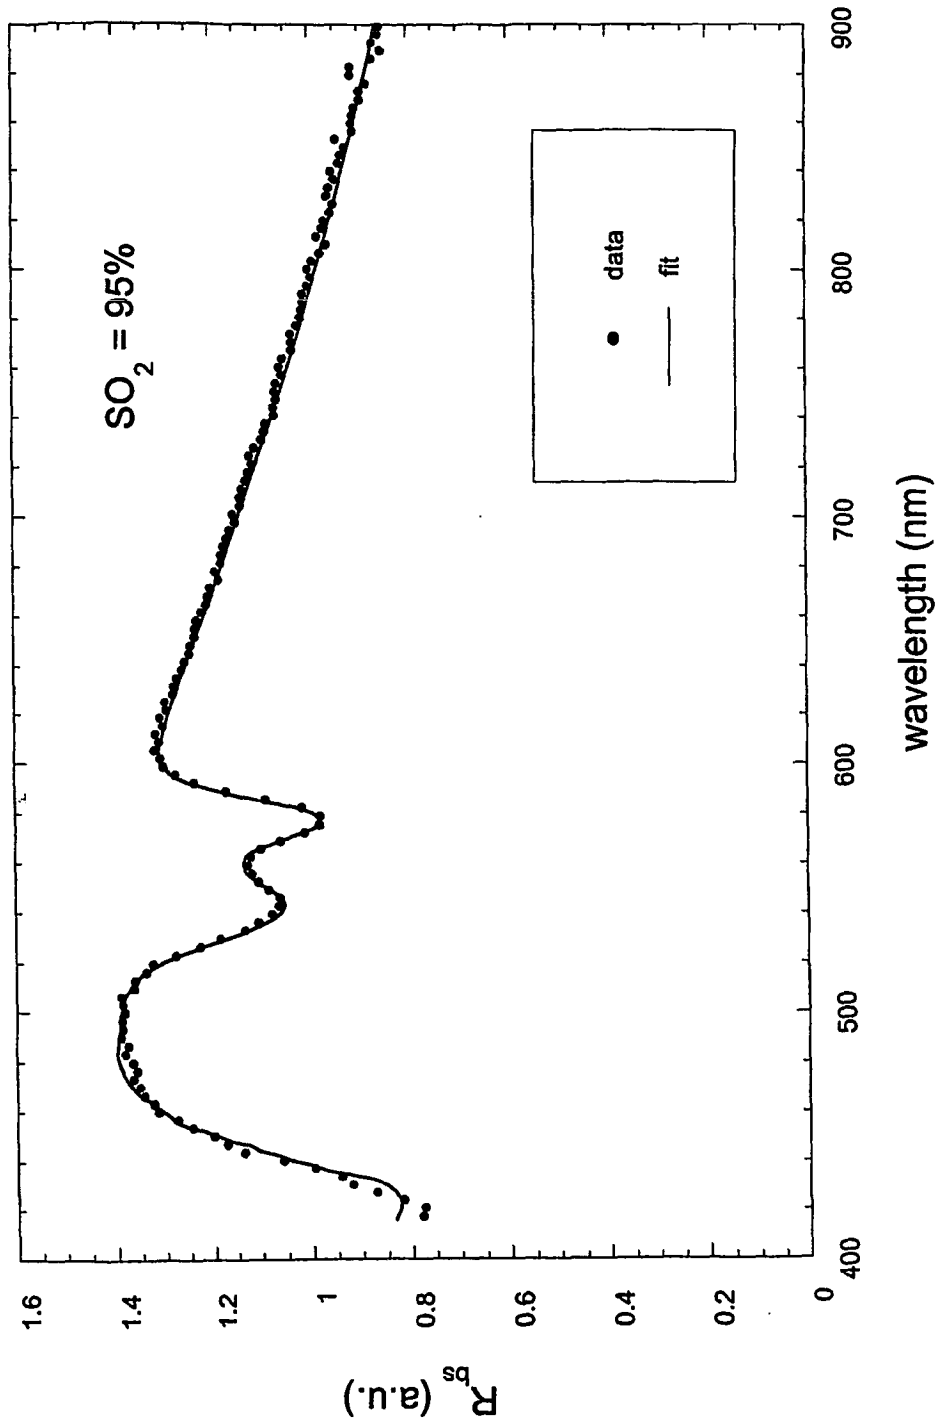


Fig 14

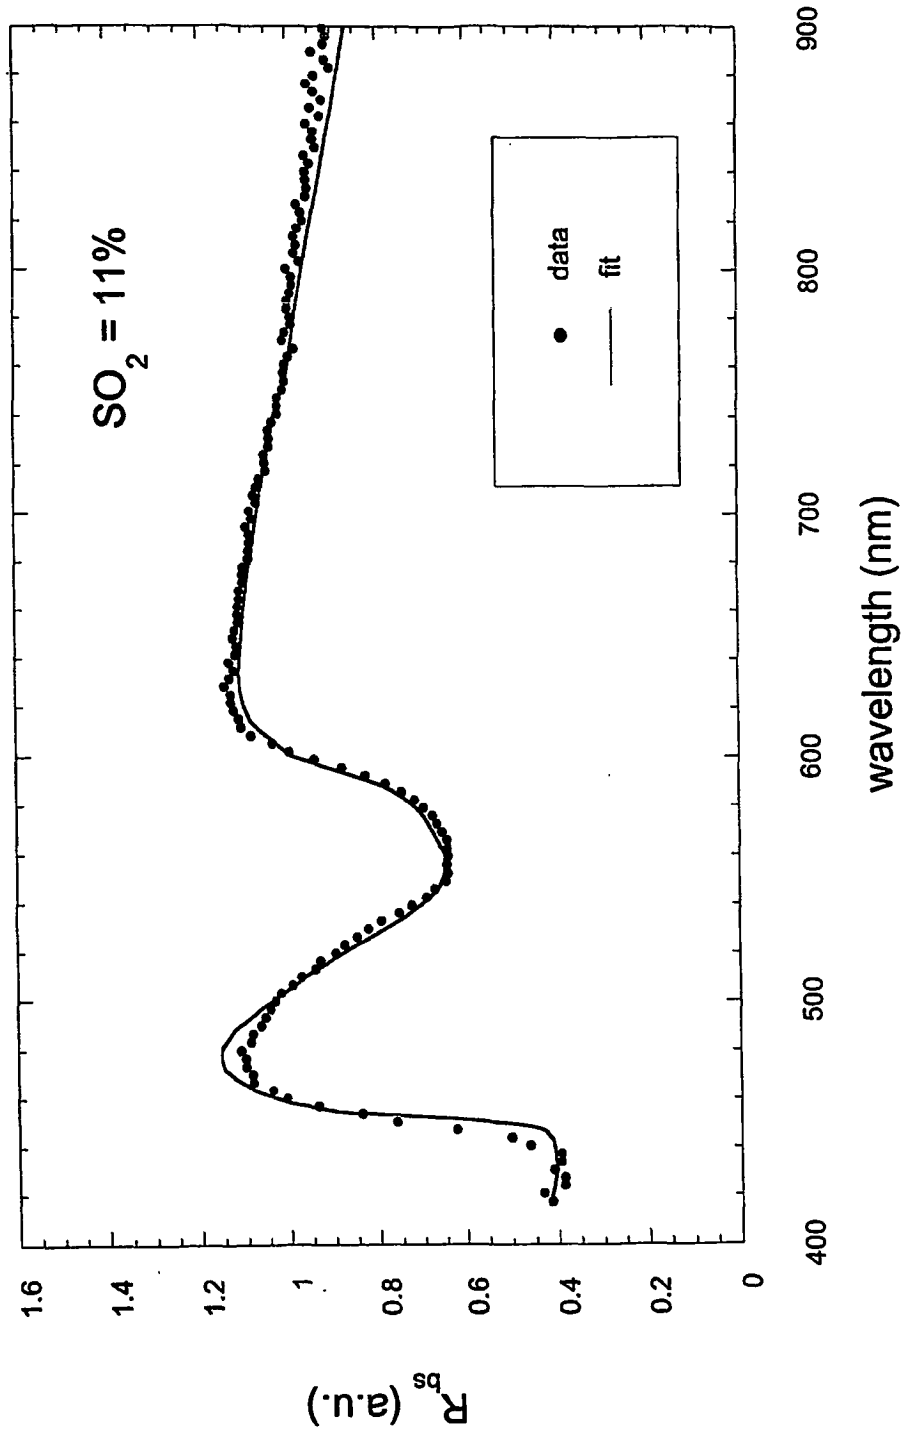

专利名称(译)	用于反向散射光谱的方法和装置		
公开(公告)号	EP1664745B1	公开(公告)日	2007-01-10
申请号	EP2004774960	申请日	2004-09-22
[标]申请(专利权)人(译)	技術科學基金會		
申请(专利权)人(译)	STICHTING VOOR DE TECHNISCHE WETENSCHAPPEN		
当前申请(专利权)人(译)	STICHTING VOOR DE TECHNISCHE WETENSCHAPPEN		
[标]发明人	AMELINK ARJEN STERENBORG HENRICUS JOSEPHUS CORNELIS MARIA		
发明人	AMELINK, ARJEN STERENBORG, HENRICUS, JOSEPHUS, CORNELIS, MARIA		
IPC分类号	G01N21/49 A61B5/00		
CPC分类号	A61B5/14551 A61B5/0059 G01N21/49 G01N2021/4709 G01N2021/4742		
优先权	2003078010 2003-09-23 EP		
其他公开文献	EP1664745A1		
外部链接	Espacenet		

摘要(译)

公开了一种用于确定介质的物理性质的方法和装置，例如介质中物质的浓度。该装置包括光源（2），具有至少第一和第二光纤（5,6）的探针，所述第一和第二光纤（5,6）彼此并排放置，所述第一光纤（5）设置成将来自光源的辐射传递给光源。样品（1）并从所述样品收集第一反向散射辐射，所述第二光纤（6）用于收集第二反向散射辐射，用于产生第一和第二反向散射辐射的光谱仪（7），用于首先产生的光谱仪（7）基于所述第一和第二反向散射辐射的第二和第二信号，以及适于从所述第一和第二信号确定差分反向散射信号并通过将所述测量的差分反向散射信号曲线拟合到反向散射函数来计算所述物理特性的处理器（9）。取决于光纤的直径是小于还是大于样品中光子的平均自由程，使用不同的反向散射功能。

