

(19)



(11)

**EP 2 627 238 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:

**17.08.2016 Bulletin 2016/33**

(51) Int Cl.:

**A61B 1/00** <sup>(2006.01)</sup>      **G02B 26/10** <sup>(2006.01)</sup>  
**A61B 1/005** <sup>(2006.01)</sup>      **G02B 23/24** <sup>(2006.01)</sup>  
**A61B 5/00** <sup>(2006.01)</sup>

(21) Application number: **11831848.4**

(86) International application number:

**PCT/AU2011/001303**

(22) Date of filing: **12.10.2011**

(87) International publication number:

**WO 2012/048374 (19.04.2012 Gazette 2012/16)**

(54) **A SCANNER FOR AN ENDOSCOPE**

SCANNER FÜR EIN ENDOSKOP

SCANNER POUR UN ENDOSCOPE

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR**

(74) Representative: **Zimmermann, Tankred Klaus et al**

**Schoppe, Zimmermann, Stöckeler**  
**Zinkler, Schenk & Partner mbB**  
**Patentanwälte**  
**Radlkoferstrasse 2**  
**81373 München (DE)**

(30) Priority: **12.10.2010 AU 2010904552**

(43) Date of publication of application:

**21.08.2013 Bulletin 2013/34**

(56) References cited:

**WO-A1-00/44275**      **JP-A- S61 250 608**  
**US-A1- 2007 100 200**      **US-A1- 2007 249 908**  
**US-A1- 2009 177 042**      **US-A1- 2010 179 386**  
**US-A1- 2010 204 546**      **US-B2- 6 950 692**  
**US-B2- 6 950 692**

(73) Proprietor: **OPTISCAN PTY LTD**

**Notting Hill,**  
**Victoria 3168 (AU)**

• **PATENT ABSTRACTS OF JAPAN & JP 61 250608**

**A (OLYMPUS OPTICAL CO LTD) 07 November 1986**

(72) Inventors:

- **BYRNE, Christopher Gerard**  
**Berwick**  
**Victoria 3806 (AU)**
- **PATTIE, Robert Alan**  
**Nyora**  
**Victoria 3987 (AU)**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

**EP 2 627 238 B1**

**Description**Field

5 **[0001]** The invention relates to a flexible scanner suitable for probe based endomicroscopy

Background

10 **[0002]** The field of endomicroscopy has emerged over the past decade with several innovations enabling microscopic imaging of living tissues of humans and animals and other subjects without the previously required removal of tissue for physical sectioning into thin slices for examination under a bench microscope.

**[0003]** Various forms of optical sectioning microscopy have featured, including laser scanning confocal microscopy (us, MKT), multiphoton microscopy and other forms of nonlinear scanning microscopy.

15 **[0004]** Clinical evidence has amassed as to the clinical benefit of endomicroscopy, including increased sensitivity and specificity of disease detection and, if used to select sites for traditional biopsy sampling, achievement of higher diagnostic yield from a reduced number of biopsy sampling sites.

20 **[0005]** The most established systems in practical clinical use have been used most in gastroenterological endoscopy (GI endoscopy) and involve two main technical approaches to miniaturization of the confocal microscope sufficient for endoscopic use. Both these approaches involve the use of optical fibre technology to provide a flexible conduit that separates bulky laser source and detection components from the imaging components near the tissue.

25 **[0006]** Of the two commercially available instruments, the first uses a single optical fibre acting as both an illumination and detection aperture, and the fibre is physically scanned in a raster pattern and this occurs within the distal end of the device. A miniature objective lens couples the plane traversed by the scanning fibre tip to an objective imaging plane at or beneath the surface of the tissue in front of the device. This lens is used bidirectionally, forward coupling the illumination source from fibre to sample, and then collecting fluorescent or reflected light from the focal plane and projecting it back into the source optical fibre for transmission back to the proximal detection unit. A contact window at the tip of the device in front of said lens provides a reference plane of tissue contact, and an actuation mechanism included in the imaging head moves the focal plane of the optical system to different distances beyond the contact window (thus effecting optical sectioning at dynamically variable depth relative to the surface of the tissue contacting the window), either by moving part of the optical system to shift the focal plane, or by moving the whole scanning mechanism and lens system relative to the window. This has resulted in devices that yield subcellular, sub-micron resolution across a usable sub-millimetre field of view, with dynamic adjustment of imaging depth under control of the endoscopist.

30 **[0007]** Commercially available scanners exploiting this approach have reached dimensions of 5mm x 43mm as a rigid tip connected via a flexible umbilicus for integration with flexible and rigid endoscope devices. This is sufficiently small to allow integration into a modified gastrointestinal (GI) endoscope or surgical endoscope, the former requiring a slight rigidisation of a short length of the distal region of the endoscope to accommodate the rigid scanner components.

35 **[0008]** Variations on this approach have been proposed which include alternative scanning patterns (spiral fibre scanning, elliptical fibre scanning, lissajous pattern fibre scanning, and MEMS based mirror scanning) but at the dimensions required for endoscopy, none have yet been reported to produce the imaging performance or mechanical viability of the above approach.

40 **[0009]** The other of the commercially available instruments involves proximal scanning of a coherent imaging bundle of optical fibres, each acting in turn as a confocal illumination and detection aperture, sequentially. This approach removes the requirement for several of the moving parts required in the scanning fibre approach, and has facilitated more extreme miniaturization than the scanning fibre approach to date, allowing probes less than 3mm diameter down to sub millimeter devices. This comes at the expense of resolution, being limited by the packing density of fibres (which cannot approach the resel density of a continuously moving fibre core), and devices in use have a maximum fibre count of 30,000 elements at the larger diameters down to less than 10,000 pixels for the smaller devices (compared to a 1024x1024 pixels, or 1megapixel, associated with the scanned fibre devices). These devices also do not allow the dynamic adjustment of imaging depth, although lens systems have been developed which fix individual devices at specific imaging depths, which may be at or beneath the tissue surface (see MKT specifications). The great advantage of these probes is that they are small enough, and have a sufficiently short rigid length at the tip, and are sufficiently flexible in between, to allow insertion through working channels of existing endoscopes without modification or integration. To date, this has not been possible with the scanning fibre devices, due in part to diameter, but mostly to the rigid length resulting in the longitudinal arrangement of window, then objective lens, then fibre scanning region, fibre mount, and depth actuation mechanism.

55 **[0010]** Although further miniaturization of the scanned fibre approach has been demonstrated, the rigid length of the scanner, while shortened, still precludes insertion via working channels of unmodified GI endoscopes and still require integration into the endoscope. Sufficient further shortening of the rigid length of said scanner designs is limited little by

the ability to make smaller components but fundamentally by the physics dictating the required longitudinal arrangements. Although the diameter of the components in the above have approached the diameter required for insertion into flexible endoscope working channels, the rigid length remains too long to navigate the bends in the device, including the permanently angled insertion port typically configured to ensure that if a device can be inserted into the first part of the channel, it will subsequently be able to negotiate any path through the endoscope in normal use.

### Summary

**[0011]** The invention, which is defined in dependent claim 1 and the dependent claims, provides a scanner for an endoscope comprising:

a scanning mechanism comprising a light transmitter and arranged to move the light transmitter to perform a scan;  
 a lens system arranged to optically couple the light transmitter to a target during a scan;  
 a first housing which houses at least a first portion of the lens system;  
 a second housing which houses at least the fibre scanning mechanism; and  
 a bendable joint joining the first and second housings such that in a scanning configuration the bendable joint joins the first and second housings so that optical elements in the first and second housings are aligned at a working separation, the bendable joint arranged to bend in response to insertion forces applied to the scanner during insertion of the scanner and revert to the scanning configuration in the absence of insertion forces.

**[0012]** In an embodiment, the bendable joint is sufficiently rigid so as not to compress when the first housing is pressed against a surface during a scan.

**[0013]** In an embodiment, a second portion of the lens system is housed in the second housing.

**[0014]** In an embodiment, the lens system is housed in the first housing.

**[0015]** In an embodiment, the scanner comprises a third housing which houses a second portion of the lens system, and an additional bendable joint intermediate the first and third housings

**[0016]** In an embodiment, the flexible optical transmitter comprises an optical fibre or a bundle of optical fibres.

**[0017]** The invention also provides a probe for an endoscope comprising a scanner as described above and a flexible umbilicus carrying the light transmitter and adapted to connect the scanner mechanism to a host system.

**[0018]** Thus, embodiments of the present invention enables the components of a scanned fibre scanner to be transiently flexed to allow insertion through the working channel, and then conform to a linear configuration once at the distal for apposition to, and imaging of, the tissue in front of the distal tip of the endoscope.

**[0019]** Advantageously, the embodiments enable sufficient miniaturisation and flexibility of a fibre scanning type scanner to allow insertion into common endoscope working channels regardless of make, thus enabling true fibre scanning and associated resolution and field of view comparable integrated approaches and far exceeding the resolution compromises of fibre bundle approaches previously used to access endoscope working channels and provision of features such as variable resolution and hardware (scan) zoom that are not achievable with fibre bundle approaches.

### Brief description of the drawings

**[0020]** Embodiments of the invention are described in connection with the following drawings in which:

Figure 1 is a schematic diagram of a scanner for an endoscope of a first embodiment;

Figure 2 is a schematic diagram of a scanner for an endoscope of a first embodiment; and

Figure 3 is an exemplary image of a fluorescent grid collected with the endoscope of Figure 1.

### Detailed description

**[0021]** Figure 1 shows a probe 100 for a confocal endoscope. The probe has a flexible umbilicus 110 of dimensions suitable for insertion through the working channel of an endoscope (e.g. 3.3mm diameter tubing) containing a flexible optical transmitter in the form of an optical fibre the optical fibre 122 and electrical conduits 111 to connect the scanner proximally to a host system (not shown) containing laser illumination, detection, scan control, and image display and acquisition components. In other embodiments, the flexible optical transmitter may be in the form of a bundle of optical fibres.

**[0022]** The distal end of the flexible umbilicus 110 is connected to a scanner 105. The scanner has a first short (typically <13mm) rigid tube 140 that provides a housing for a confocal projection/objective lens system 141 positioned at a prescribed distance behind an outer tissue contact window 150 that seals the tip of the tube 140.

**[0023]** The inner region of this more distal short rigid tube 140 includes a protective bush 123 around the tip of the

optical fibre 122 fabricated of a material that provides impact protection should the tip of the fibre contact the wall when scanning due to mechanical impact external to the scanner or bending during insertion into or withdrawal from the endoscope working channel. In other embodiments, protection may be provided by a coating material rather than bush 123.

**[0024]** A second short (typically <13mm) rigid tube 120 provides a housing for a distal fibre scanning mechanism and is mounted onto the distal end of the above flexible umbilical tube 110.

**[0025]** The dimensions of each of the two short sections of tube are chosen to fall within the limits of length versus diameter for the target channel through which the device is to be inserted and withdrawn. Example dimensions are set out in Table 1.

Table 1

Scanner Diameter	3.8mm Channel	4.2mm Channel
3mm	19mm Rigid length	21mm Rigid Length
3.5mm	17mm Rigid Length	18.5mm Rigid Length
4mm	-	16mm Rigid Length

**[0026]** Any suitable fibre scanning mechanism can be employed. In the embodiment, the scanning mechanism comprises a magnet 123, a fibre 122, and a fibre scanning mount and coils deployed within scanning mechanism housing 121. Examples of fibre scanning mechanism are described in US 2009/0177042, WO 2004/040267 and US 2009/001589. In figure 1, the fibre is shown as moving between different scanning positions 122A, 122B.

**[0027]** A bendable joint 130 between the two housing sections is provided by section of flexible sprung tubing 130 that joins the first short rigid tube 140 to the second short rigid tube 120 such that the fibre 122 is positioned at a working separation corresponding to the required distance from the projection/objective lens 141.

**[0028]** The entry into the endoscope through which a probe is introduced has "gate" port with a bend in it so as to prevent the insertion of probes which do not bend sufficiently and hence are at risk of breaking during insertion. Typically, the bend is 135 degrees.

**[0029]** The bendable joint 130 has properties that will allow it to bend sideways when a lateral force is exerted, thus allowing the two short sections to follow through a curved channel (such as the gate port) but then to "snap" back into co-axial alignment within a sufficiently small tolerance to restore the functional alignment of the optical components (that is to return to a scanning configuration where the optical elements are positioned relative to the desired optical axis at a separation where they will still work). In the embodiment of Figure 1, a working separation is maintained between the scanning fibre 122 to the scanning image plane of the projection/objective lens 141. The bendable joint may take a number of different forms. For example, a spring of closed configuration, with the wire cross section either cylindrical, flattened, rectangular or square. The spring is selected so as to allow small movements from straight to bent based on typical insertion forces applied to push devices through endoscope working channels. The spring of Figure 1 is a closed stack construction that is not compressible when straight by the forces normally needed to locate the window of the scanner against the surface of a target (such as tissue to be examined), but rather opens out to permit lateral flexing. This design can provide reliable return to a precise axial and lateral alignment of scanner components after flexing.

**[0030]** An advantage of the spring being not compressible in its re-aligned state is that it can withstand being pushed against the tissue without inducing any bends in the scanner.

**[0031]** In other embodiments, the bendable joint 130 may take the form of non-kinking flexible tubes such as shape memory alloy tubular structures. In some embodiments, the shape memory material may be subject to electrical actuation to move between "bendable" and "rigid" states for insertion and imaging (scanning) phases of use, respectively.

**[0032]** The bendable joint 130 of the scanner 105 is coated with an appropriately flexible glue or covered with an a rubber or plastic tube so as to seal this section from ingress of fluid, and to provide a surface suitable for disinfection or sterilization.

**[0033]** No active imaging depth adjustment is included in the present invention. However, a passive mechanism for adjusting imaging depth is provided may be constructed by inclusion of an short flexible walled region 160 in the distal short rigid tube between the fixture of the projection/objective lens 141 and the fixture of the imaging window 150. The compression spring constants of this material are selected so as allow the imaging window 150 to move a useful distance (axially to the device), thus effecting a manual imaging depth adjustment controlled by the pressure applied to the device in positioning it against the tissue. This allows quite intuitive adjustment of the observed image from the surface of the tissue (light touch of probe to tissue) through to the deepest tissue imaging afforded by tissue scattering (typical for confocal endomicroscopy) with firm pressure on the tissue.

**[0034]** Figure 3 shows an example of a fluorescent grid collected with a scanner made in accordance with the first

embodiment.

[0035] Figure 2 shows a probe 200 of a second embodiment with a different scanner 205 configuration. In this embodiment, there are three housings 120, 240, 260 joined by two bendable joints 130, 270. One of the bendable joints 270 is disposed between a first part 241 and a second part 261 of the lens system.

[0036] Persons skilled in the art will appreciate that in some embodiments, it is possible to modify the embodiment of Figure 1 along the lines of Figure 2 to provide a scanner with two housings where one part of the lens system is in the same housing as the scanning mechanism and another part of the lens system is in a separate housing.

[0037] Persons skilled in the art will appreciate that the scanner can be employed in microscope, an endoscope, an endomicroscope, an optical coherence tomograph, a confocal microscope, or a confocal multiphoton microscope or other image apparatus.

[0038] It will be understood to persons skilled in the art of the invention that many modifications may be made without departing from the scope of the invention, in particular it will be apparent that certain features of embodiments of the invention can be employed to form further embodiments.

[0039] It is to be understood that, if any prior art is referred to herein, such reference does not constitute an admission that the prior art forms a part of the common general knowledge in the art in any country.

[0040] In the claims which follow and in the preceding description of the invention, except where the context requires otherwise due to express language or necessary implication, the word "comprise" or variations such as "comprises" or "comprising" is used in an inclusive sense, i.e. to specify the presence of the stated features but not to preclude the presence or addition of further features in various embodiments of the invention.

## Claims

1. A scanner for a microscope, endoscope or endomicroscope, the scanner comprising:

a scanning mechanism (121, 122, 124) comprising a light transmitter (122) and arranged to move the light transmitter (122) to perform a scan;

a lens system (141) arranged to optically couple the light transmitter (122) to a target during a scan;

a first housing (140) which houses at least a first portion of the lens system (141); and

a second housing (120) which houses at least the scanning mechanism (121, 122, 124);

### characterized by

a bendable joint (130) joining the first and second housings (140, 120) such that in a scanning configuration the bendable joint (130) joins the first and second housings (140, 120) so that optical elements in the first and second housings (140, 120) are aligned at a working separation, the bendable joint (130) arranged to bend in response to insertion forces applied to the scanner (105; 205) during insertion of the scanner (105; 205) and revert to the scanning configuration in the absence of insertion forces.

2. The scanner of claim 1, wherein the bendable joint (130) is sufficiently rigid so as not to compress when the first housing (140) is pressed against a surface during a scan.

3. The scanner of claim 1 or claim 2, wherein a second portion of the lens system (141) is housed in the second housing.

4. The scanner of claim 1 or claim 2, wherein the lens system (141) is housed in the first housing (140).

5. The scanner of claim 1 or claim 2, comprising a third housing (260) which houses a second portion (261) of the lens system (141), and an additional bendable joint (270) intermediate the first and third housings (240, 261).

6. The scanner of any one of claims 1 to 5, wherein the light transmitter comprises an optical fibre or a bundle of optical fibres.

7. A probe for an endoscope comprising:

a scanner (105; 205) as claimed in any one of claims 1 to 6, and a flexible umbilicus (110) carrying the light transmitter (122) and adapted to connect the scanner (105; 205) to a host system.

8. An microscope, an endoscope, an endomicroscope, an optical coherence tomograph, a confocal microscope, or a confocal multiphoton microscope comprising the scanner (105; 205) of any one of claims 1 to 6.

9. An image apparatus comprising the scanner (105; 205) of any one of claims 1 to 6.

**Patentansprüche**

5

1. Eine Abtastvorrichtung für ein Mikroskop, Endoskop oder Endomikroskop, wobei die Abtastvorrichtung folgende Merkmale aufweist:

10

einen Abtastmechanismus (121, 122, 124), der ein Lichtübertragungselement (122) aufweist und angeordnet ist, um das Lichtübertragungselement (122) zu bewegen, um eine Abtastung durchzuführen; ein Linsensystem (141), das angeordnet ist, um das Lichtübertragungselement (122) optisch während einer Abtastung mit einem Ziel zu koppeln; ein erstes Gehäuse (140), das zumindest einen ersten Abschnitt des Linsensystems (141) häusst; und ein zweites Gehäuse (120), das zumindest den Abtastmechanismus (121, 122, 124) häusst;

15

**gekennzeichnet durch:**

20

ein biegbares Gelenk (130), das das erste und das zweite Gehäuse (140, 120) derart verbindet, dass in einer Abtastkonfiguration das biegbare Gelenk (130) das erste und das zweite Gehäuse (140, 120) so verbindet, dass optische Elemente in dem ersten und dem zweiten Gehäuse (140, 120) in einem Arbeitsabstand ausgerichtet sind, wobei das biegbare Gelenk (130) angeordnet ist, um sich ansprechend auf Einführkräfte, die auf die Abtastvorrichtung (105, 205) während einer Einführung der Abtastvorrichtung (105, 205) ausgeübt werden, zu biegen und in Abwesenheit der Einführkräfte in die Abtastkonfiguration zurückzukehren.

25

2. Die Abtastvorrichtung gemäß Anspruch 1, bei der das biegbare Gelenk (130) ausreichend starr ist, so dass dieses nicht komprimiert wird, wenn das erste Gehäuse (140) während einer Abtastung gegen eine Oberfläche gedrückt wird.

30

3. Die Abtastvorrichtung gemäß Anspruch 1 oder Anspruch 2, bei der ein zweiter Abschnitt des Linsensystems (141) in dem zweiten Gehäuse gehäust ist.

35

5. Die Abtastvorrichtung gemäß Anspruch 1 oder Anspruch 2, die ein drittes Gehäuse (260), das einen zweiten Abschnitt (261) des Linsensystems (141) häusst, und ein zusätzliches biegbares Gelenk (270) zwischen dem ersten und dem dritten Gehäuse (240, 261) aufweist.

40

6. Die Abtastvorrichtung gemäß einem der Ansprüche 1 bis 5, bei der das Lichtübertragungselement eine optische Faser oder ein Bündel optischer Fasern aufweist.

7. Eine Sonde für ein Endoskop, die folgendes Merkmal aufweist:

45

eine Abtastvorrichtung (105, 205) gemäß einem der Ansprüche 1 bis 6, sowie einen flexiblen Nabel (110), der das Lichtübertragungselement (122) trägt und angepasst ist, um die Abtastvorrichtung (105; 205) mit einem Host-System zu verbinden.

50

8. Ein Mikroskop, ein Endoskop, ein Endomikroskop, ein optischer Kohärenztomograph, ein konfokales Mikroskop oder ein konfokales Mehrphotonenmikroskop mit der Abtastvorrichtung (105; 205) gemäß einem der Ansprüche 1 bis 6.

9. Ein Bildgerät mit der Abtastvorrichtung (105; 205) gemäß einem der Ansprüche 1 bis 6.

55

**Revendications**

1. Scanner pour un microscope, endoscope ou endomicroscope, le scanner comprenant:

## EP 2 627 238 B1

un mécanisme de balayage (121, 122, 124) comprenant un émetteur de lumière (122) et aménagé pour déplacer l'émetteur de lumière (122) pour effectuer un balayage;  
un système de lentilles (141) aménagé pour coupler optiquement l'émetteur de lumière (122) à une cible pendant un balayage;  
5 un premier boîtier (140) qui abrite au moins une première partie du système de lentilles (141); et  
un deuxième boîtier (120) qui abrite au moins le mécanisme de balayage (121, 122, 124);

### caractérisé par

10 une articulation pliable (130) reliant les premier et deuxième boîtiers (140, 120) de sorte que, dans une configuration de balayage, l'articulation pliable (130) connecte les premier et deuxième boîtiers (140, 120) de sorte que les éléments optiques dans les premier et deuxième boîtiers (140, 120) soient alignés à une distance de travail, que l'articulation pliable (130) soit aménagée de manière à fléchir en réponse à des forces d'insertion appliquées au scanner (105; 205) pendant l'insertion du scanner (105; 205) et à retourner à la configuration de balayage en l'absence de forces d'insertion.

15 **2.** Scanner selon la revendication 1, dans lequel l'articulation pliable (130) est suffisamment rigide pour ne pas se comprimer lorsque le premier boîtier (140) est pressé contre une surface pendant un balayage.

20 **3.** Scanner selon la revendication 1 ou la revendication 2, dans lequel une deuxième partie du système de lentilles (141) est logé dans le deuxième boîtier.

**4.** Scanner selon la revendication 1 ou la revendication 2, dans lequel le système de lentilles (141) est logé dans le premier boîtier (140).

25 **5.** Scanner selon la revendication 1 ou la revendication 2, comprenant un troisième boîtier (260) qui abrite une deuxième partie (261) du système de lentilles (141), et une articulation pliable additionnelle (270) entre les premier et troisième boîtiers (240, 261).

30 **6.** Scanner selon l'une quelconque des revendications 1 à 5, dans lequel l'émetteur de lumière comprend une fibre optique ou un faisceau de fibres optiques.

**7.** Sonde pour un endoscope, comprenant:

35 un scanner (105; 205) selon l'une quelconque des revendications 1 à 6, et un ombilic flexible (110) portant l'émetteur de lumière (122) et adapté pour connecter le scanner (105; 205) à un système hôte.

**8.** Microscope, endoscope, endomicroscope, tomographe de cohérence optique, microscope confocal ou microscope multiphoton confocal comprenant le scanner (105; 205) selon l'une quelconque des revendications 1 à 6.

40 **9.** Dispositif d'image comprenant le scanner (105; 205) selon l'une quelconque des revendications 1 à 6.

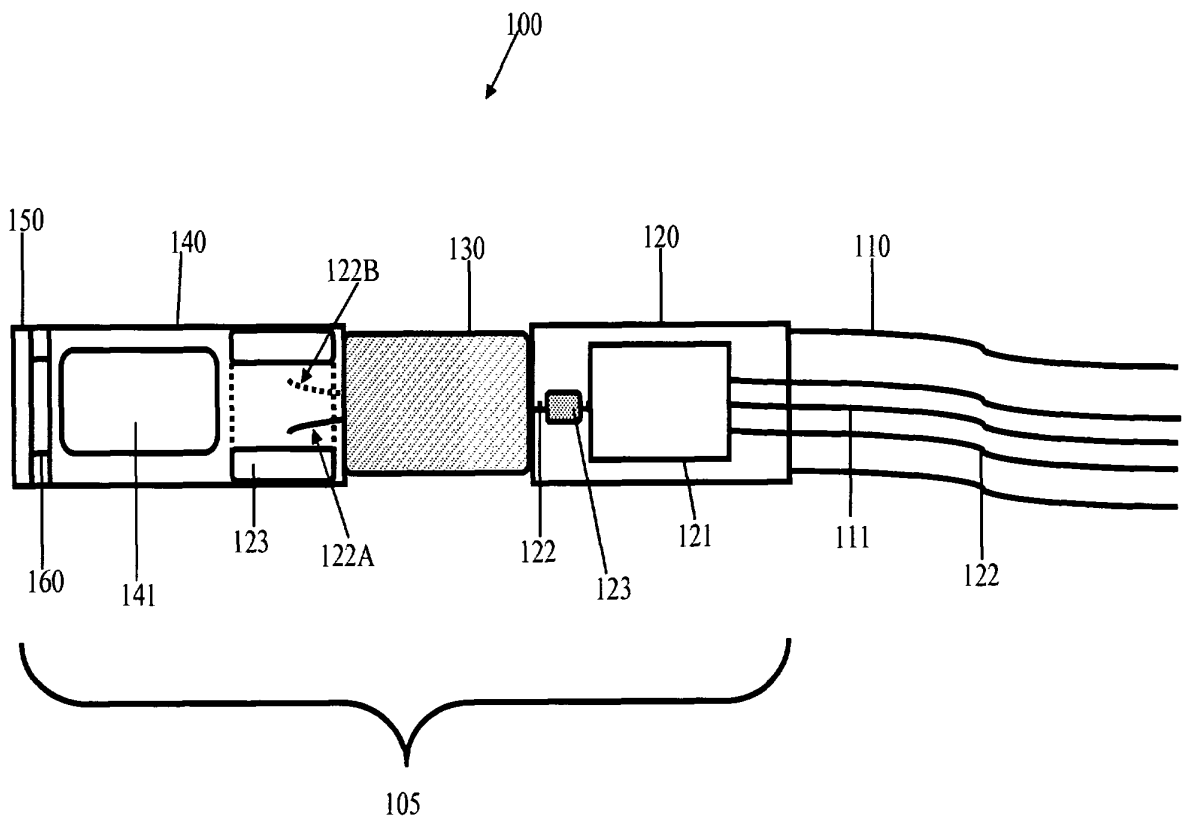


Figure 1

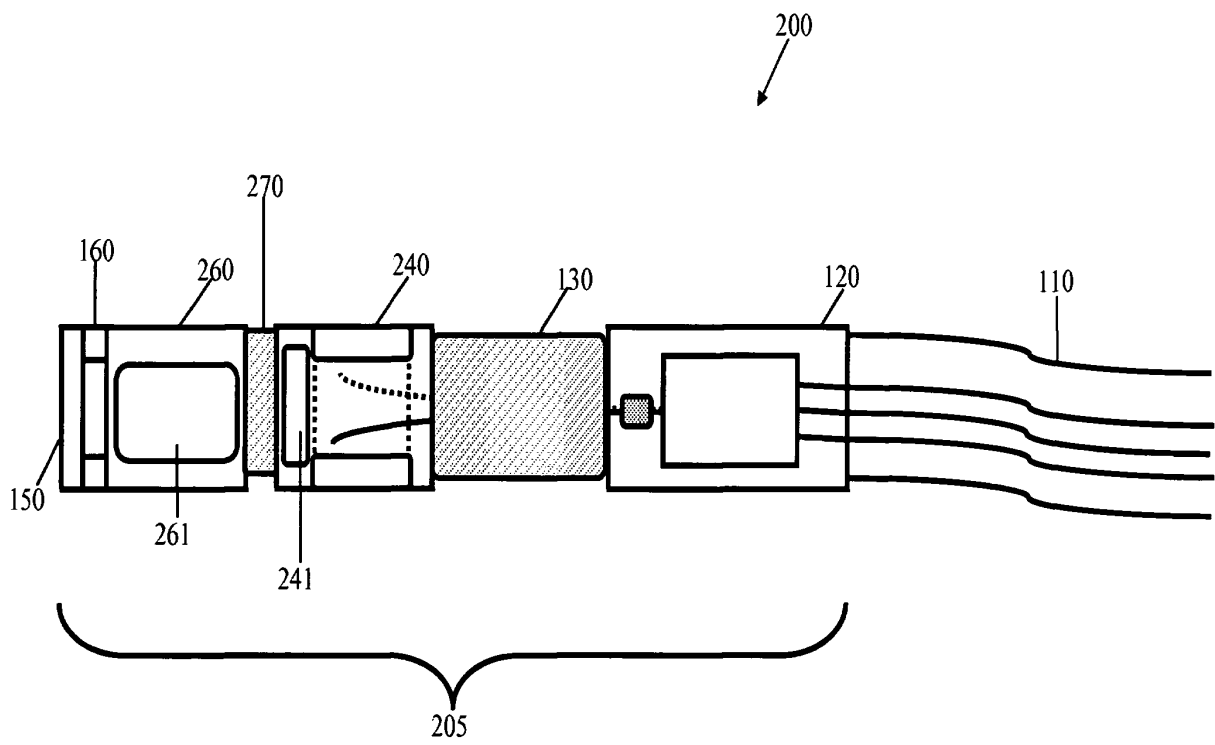


Figure 2

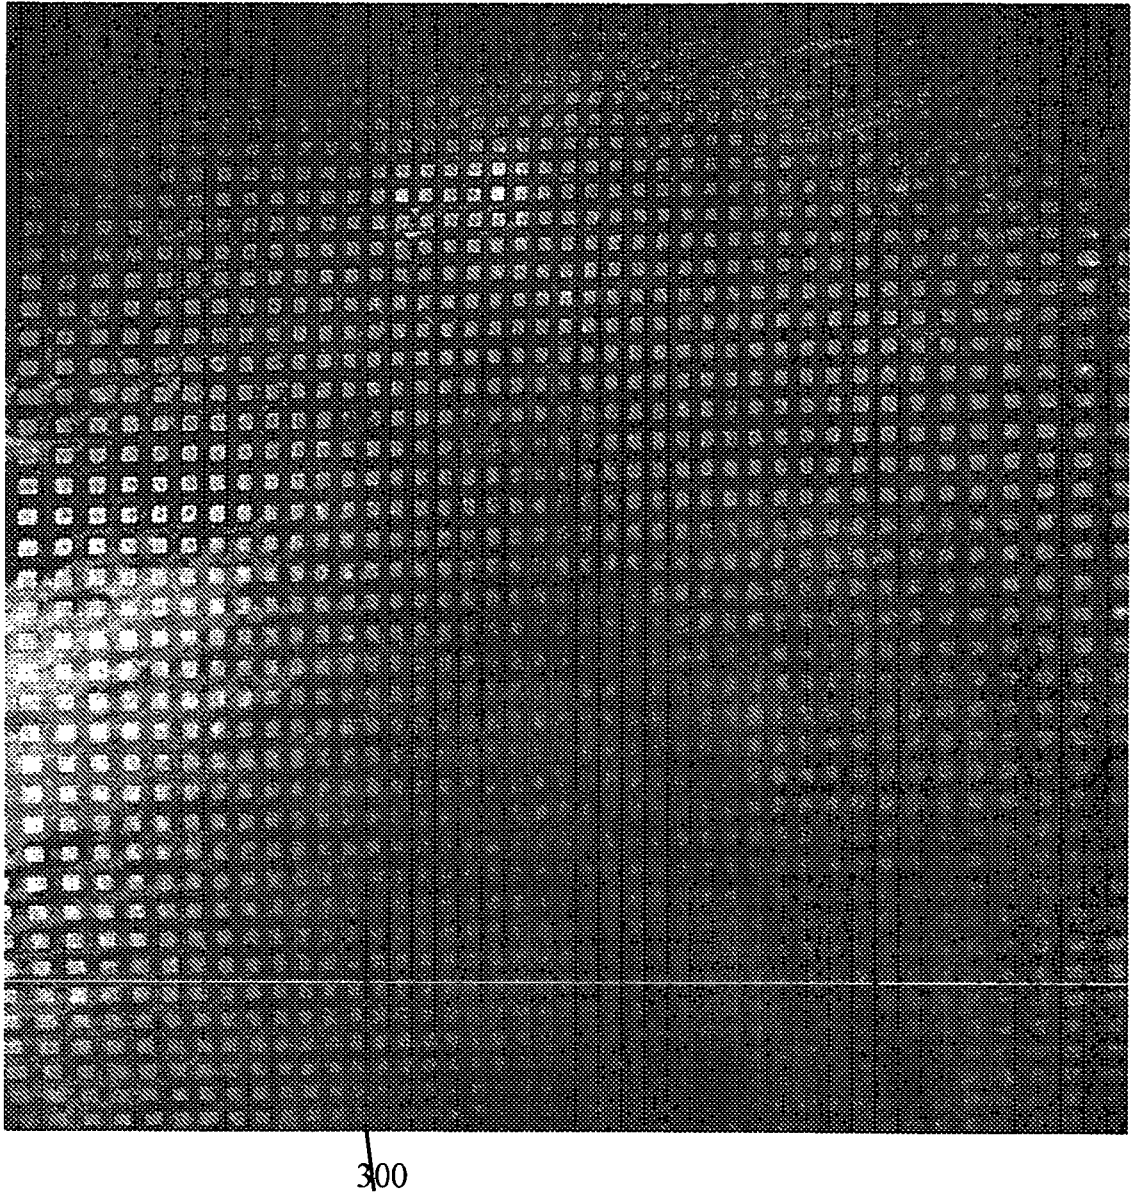


Figure 3

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 20090177042 A [0026]
- WO 2004040267 A [0026]
- US 2009001589 A [0026]

专利名称(译)	用于内窥镜的扫描仪		
公开(公告)号	<a href="#">EP2627238B1</a>	公开(公告)日	2016-08-17
申请号	EP2011831848	申请日	2011-10-12
[标]申请(专利权)人(译)	OPTISCAN		
申请(专利权)人(译)	OPTISCAN PTY LTD		
当前申请(专利权)人(译)	OPTISCAN PTY LTD		
[标]发明人	BYRNE CHRISTOPHER GERARD PATTIE ROBERT ALAN		
发明人	BYRNE, CHRISTOPHER GERARD PATTIE, ROBERT ALAN		
IPC分类号	A61B1/00 G02B26/10 A61B1/005 G02B23/24 A61B5/00		
CPC分类号	A61B1/00165 A61B1/00096 A61B1/00117 A61B1/00172 A61B1/005 A61B5/0066 A61B5/0068 A61B5/0084 G02B23/2469 G02B23/2476 G02B26/103		
优先权	2010904552 2010-10-12 AU		
其他公开文献	EP2627238A4 EP2627238A1		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

一种用于内窥镜的扫描仪，包括：扫描机构，包括光发射器，并设置成移动光发射器以执行扫描；透镜系统，设置成在扫描期间将光发射器光学耦合到目标；第一壳体，其至少容纳透镜系统的第一部分；第二壳体，至少容纳纤维扫描机构；连接第一和第二壳体的可弯曲接头使得在可扫描构造中，可弯曲接头连接第一和第二壳体，使得第一和第二壳体中的光学元件以工作间隔对准，可弯曲接头设置成弯曲以响应在插入扫描仪期间施加到扫描仪的插入力，并在没有插入力的情况下恢复到扫描配置。

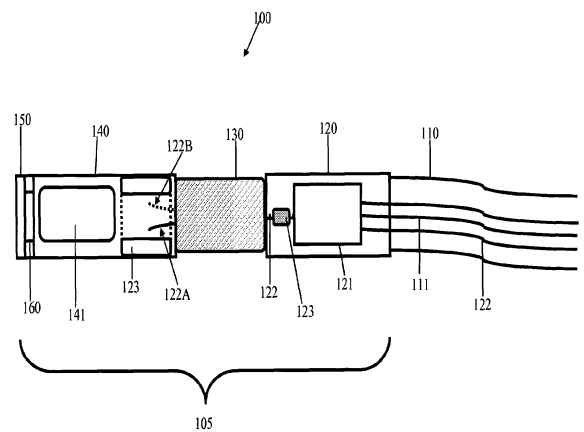


Figure 1