

(19)



(11)

EP 2 732 756 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
11.09.2019 Bulletin 2019/37

(51) Int Cl.:
A61B 5/00 ^(2006.01) **A61B 5/145** ^(2006.01)
G06T 11/00 ^(2006.01)

(21) Application number: **13190007.8**

(22) Date of filing: **24.10.2013**

(54) Object information acquisition apparatus

Objektinformationserfassungsvorrichtung

Appareil d'acquisition d'informations d'un objet

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **15.11.2012 JP 2012251317**

(43) Date of publication of application:
21.05.2014 Bulletin 2014/21

(73) Proprietor: **Canon Kabushiki Kaisha
Tokyo 146-8501 (JP)**

(72) Inventor: **Nanaumi, Ryuichi
Tokyo, Tokyo 146-8501 (JP)**

(74) Representative: **TBK
Bavariaring 4-6
80336 München (DE)**

(56) References cited:
**EP-A1- 2 345 364 WO-A1-2011/096551
WO-A1-2011/125468 WO-A1-2012/086842
WO-A1-2012/144395 JP-A- 2012 061 055
JP-A- 2012 085 965 US-A1- 2011 245 652**

EP 2 732 756 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description**BACKGROUND OF THE INVENTION**

Field of the Invention

[0001] The present invention relates to an object information acquisition apparatus.

Description of the Related Art

[0002] As one in vivo imaging technique using near-infrared light, there is photoacoustic tomography (PAT). In PAT, an object such as a biological body is irradiated with pulsed light generated from a light source, whereby light propagated and diffused within the object is absorbed by a light absorber to generate an elastic wave. This mechanism of elastic wave generation is called a photoacoustic effect. Since a tumor has a higher light energy absorption rate for near-infrared light than surrounding tissues, the tumor absorbs more light than the surrounding tissues. Thus, the tumor momentarily expands and generates an elastic wave.

[0003] In an apparatus described in Japanese Patent Application Laid-open No. 2011-245277, the elastic wave is detected with a detection element and converted to a received signal. Through signal processing (reconstruction) of the received signal, object information such as the space distribution of initial sound pressure of the elastic wave generated upon absorption of light energy within the object can be imaged. Since the space distribution of generated sound pressure relates to the absorption coefficient of light, diagnosis of an object using space distribution relating to the absorption coefficient of light has been studied.

[0004] Prior art which is related to this field of technology can be found e.g. in document JP 2012 061055 A disclosing photoacoustic imaging apparatus, and method for controlling the same, in document WO 2012/144395 A1 disclosing photoacoustic imaging apparatus and method therefor, in document JP 2012 085965 A disclosing mammographic measuring apparatus, in document EP 2 345 364 A1 disclosing subject information obtaining apparatus, subject information obtaining method, and program, in document WO 2012/086842 A1 disclosing subject information acquiring device and subject information acquiring method, in document WO 2011/125468 A1 disclosing photoacoustic imaging apparatus, photoacoustic imaging method, and program, in document US 2011/0245652 A1 disclosing imaging apparatus and imaging method, and in document WO 2011/096551 A1 disclosing photoacoustic apparatus and a method for its use to acquire biofunctional information.

SUMMARY OF THE INVENTION

[0005] The present invention in its one aspect provides an object information acquisition apparatus as specified in claims 1 to 15. Further features of the present invention will become apparent from the following description of exemplary embodiments with reference to the attached drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0006]

Fig. 1 is a diagram showing an overview of a photoacoustic imaging apparatus in a first embodiment;
 Fig. 2 is a diagram showing the details of a light intensity domain setting unit in the first embodiment;
 Fig. 3 is a diagram showing the flow of measurement in the first embodiment;
 Fig. 4 is a diagram showing an overview of a photoacoustic imaging apparatus in a second embodiment;
 Fig. 5 is a diagram showing the flow of measurement in the second embodiment;
 Fig. 6 is a diagram showing an overview of a photoacoustic imaging apparatus in a third embodiment;
 Fig. 7 is a diagram showing the flow of measurement in the third embodiment;
 Fig. 8 is a diagram showing an overview of a photoacoustic imaging apparatus in a fourth embodiment;
 Fig. 9 is a diagram showing the directivity range in the fourth embodiment;
 Fig. 10 is a diagram showing the details of a directivity range domain setting unit in the fourth embodiment;
 Fig. 11 is a diagram showing the details of a reconstruction unit in the fourth embodiment; and
 Fig. 12 is a diagram showing the flow of measurement in the fourth embodiment.

DESCRIPTION OF THE EMBODIMENTS

[0007] A preferred embodiment of the present invention will be described below with reference to the drawings. Note

that the dimension, material, and shape of components, the relative arrangement thereof, and the like described below should be changed appropriately depending on the configuration of an apparatus or various conditions to which the invention is applied and are not intended to limit the scope of this invention to the description below.

[0008] In the present invention, an acoustic wave includes an elastic wave called a sound wave, ultrasound wave, photoacoustic wave, or light-induced ultrasound wave. An object information acquisition apparatus of the present invention is an apparatus utilizing a photoacoustic effect in which an acoustic wave generated within an object by irradiating the object with light (electromagnetic wave) is received and characteristic information within the object is acquired.

[0009] Object information in the object information acquisition apparatus is the characteristic information reflecting the initial sound pressure of an acoustic wave caused by light irradiation, light energy absorption density derived from the initial sound pressure, absorption coefficient, concentration of a substance forming a tissue, or the like. The concentration of a substance is, for example, the concentration of oxygenated hemoglobin and reduced hemoglobin or oxygen saturation. The characteristic information may be distribution information of each position within an object instead of numerical data. That is, initial sound pressure distribution, absorption coefficient distribution, oxygen saturation distribution, or the like may be generated into image data.

[0010] The present invention can be understood as a control method upon receiving an acoustic wave with the object information acquisition apparatus. In the embodiments below, a photoacoustic imaging apparatus will be described as a specific example of the object information acquisition apparatus. In the respective drawings, the same components are basically denoted by the same reference numerals, and descriptions will be omitted.

<First embodiment>

[0011] First, the relationship of sound pressure of an elastic wave caused by a photoacoustic effect and light intensity within an object will be described. A sound pressure p_0 (Pa) of the elastic wave caused by the photoacoustic effect is represented by Formula (1).

[Math. 1]

$$p_0 = \mu_a \cdot \Gamma \cdot \Phi \quad \cdot \cdot \cdot (1)$$

In Formula (1), μ_a is the absorption coefficient (mm^{-1}) of a light absorber (tumor or the like), Γ is the Gruneisen coefficient, and Φ is the light intensity (J/mm^2) at a position of the light absorber. The Gruneisen coefficient Γ is a value for which a value of the volume expansion coefficient multiplied by the square of the speed of sound is divided by the constant pressure specific heat, and takes an approximately constant value in vivo.

[0012] As can be seen from Formula (1), the generated sound pressure is proportional to light intensity. In the case where a strong light scatterer such as a biological body is the object, the light intensity Φ decays exponentially in accordance with the distance from the position irradiated with light. Therefore, the light intensity decreases due to decay, and a domain where an elastic wave with sufficient sound pressure to be detected is not generated exists. Since it is difficult to acquire the object information with high precision even if reconstruction is performed with respect to such a domain where the light intensity is low, the inventor of the present invention has found that the significance of performing the reconstruction is small.

[0013] In a first embodiment, an optical characteristic value of the object is input to an apparatus, and a domain for which the object information is acquired is limited based on the light intensity distribution calculated from the optical characteristic value to shorten the time required for acquisition of the object information. As the optical characteristic value, the absorption coefficient that is an absorption characteristic value and the reduced scattering coefficient that is a scattering characteristic value are used.

(Apparatus configuration)

[0014] Fig. 1 is a diagram showing an overview of a photoacoustic imaging apparatus in this embodiment. The configuration for acquiring information of an object will be described below.

[0015] A light source of the present invention includes at least one coherent or incoherent pulsed light source. In order to generate a photoacoustic effect, the pulse width is preferably several hundred nanoseconds or less. In the case of measurement of a breast cancer or the like, light of a specific wavelength that is absorbed by a specific constituent (for example, hemoglobin) out of constituents forming a biological body is generated. Laser with which a large output can be obtained is preferable as the light source, but it is also possible to use a light-emitting diode or the like instead of the laser. As the laser, various lasers such as solid-state laser, gas laser, dye laser, or semiconductor laser may be used.

[0016] An irradiation unit 101 that is irradiating unit irradiates an object 100 with irradiation light from the light source with a method suitable for photoacoustic measurement. In order to increase the SN ratio of a received signal, not only

a part of surfaces but also a plurality of surfaces of the object may be irradiated with light. For example, the irradiation unit 101 may be provided not only on the side opposing a probe 103 with respect to the object but also on the same side. The irradiation unit 101 includes a mirror, a lens that collects, magnifies, or changes the shape of light, a prism that disperses, refracts, or reflects light, or an optical fiber. Any such optical part aside from those mentioned above may also be used as long as an object can be irradiated with light emitted from a light source with a desired method (irradiation direction, shape, or the like).

[0017] With a transducer 102 that is detecting unit, an elastic wave generated by the object 100 being irradiated with light is received and converted to an electrical signal that is the received signal. The transducer 102 is configured of a transducer using a piezoelectric phenomenon, a transducer using optical resonance, a transducer using capacity change, or the like. Any transducer with which an elastic wave can be received and converted to an electrical signal may be used. In this embodiment, a plurality of the transducers 102 are present in order to receive elastic waves in different positions. The plurality of transducers 102 are, for example, arranged one-dimensionally or two-dimensionally to form the probe 103. The probe 103 outputs the electrical signal generated by the plurality of transducers 102 to a reconstruction unit 109.

[0018] An optical characteristic value input unit 106 that is characteristic input unit includes an interface that accepts an input of the optical characteristic value (absorption coefficient and reduced scattering coefficient) of the object 100 performed by an operator. For example, in the case where the object 100 is a biological body, a general value for a biological body may be input or a known statistical value according to a characteristic, e.g., age, of the object 100 may be input as the absorption coefficient and the reduced scattering coefficient. Alternatively, it may be such that, when an input of age or sex is received, a value according thereto is set automatically.

[0019] An optical characteristic value setting unit 105 that is characteristic setting unit sets the absorption coefficient and the reduced scattering coefficient input to the optical characteristic value input unit 106 in a light intensity distribution calculation unit 107.

[0020] The light intensity distribution calculation unit 107 uses the absorption coefficient and the equivalent scattering coefficient set by the optical characteristic value setting unit 105 to calculate the light intensity distribution inside the object 100. The light intensity distribution calculation unit is distribution acquiring unit of the present invention. As a calculation method for the light intensity distribution, a numerical solution method of transport equations, a numerical solution method of diffusion approximation equations, a numerical solution method using a Monte Carlo method, or the like may be used. It is desirable that an intensity distribution pattern of irradiation light be reflected in the calculation of the light intensity distribution. Accordingly, the precision of calculation of the light intensity distribution can be improved. For example, it is recommended that the irradiation unit 101 be able to monitor the intensity distribution pattern of irradiation light and that the intensity distribution pattern be input to the light intensity distribution calculation unit.

[0021] With a light intensity domain setting unit 108 that is setting unit, a minimum block unit within a light intensity domain that is a domain having a light intensity of a predetermined threshold value or greater is extracted and set in the reconstruction unit 109. As the threshold value of light intensity, light intensity with which a minimum sound pressure detectable by the transducer 102 is generated can be utilized, for example.

[0022] The predetermined threshold value may differ for each minimum block unit. A calculation method therefor will be described below.

[0023] Formula (2) represents a decay compensation noise equivalent sound pressure value $p_{NEP_c}(r)$ described later. A threshold value $\Phi_{th}(r)$ of light intensity of the minimum block unit of a position vector r is represented by Formula (3) that is a deformation of Formula (1).

[Math. 2]

$$p_{NEP_c}(r) = p_{NEP} / A(\alpha, \max_i(|d_i - r|)) \quad \cdot \cdot \cdot \quad (2)$$

[Math. 3]

$$\Phi_{th}(r) = p_{NEP_c}(r) / \mu_{a_BG} \cdot \Gamma \quad \cdot \cdot \cdot \quad (3)$$

In Formula (2), p_{NEP} is the noise equivalent sound pressure for which the intensity of noise included in the electrical signal that is the received signal is divided by the conversion efficiency in the conversion of the sound pressure to the electrical signal by the transducer 102. The unit for the conversion efficiency is V/Pa in the case where the electrical

signal is a voltage. In Formula (2), $A(\alpha, \max(|d_i-r|))$ is the decay ratio of sound pressure upon propagation of an elastic wave between the transducer 102 of a position vector d_i (where i is a number showing each of the plurality of transducers 102) and the minimum block unit. The decay coefficient (mm^{-1}) of the object 100 and $\max|d_i-r|$ that is the greatest among distances $|d_i-r|$ of the i -th transducer 102 and the minimum block unit determine A . The decay of sound pressure includes distance-dependent decay by a decay coefficient α and distance-dependent decay due to energy dissipation in spherical wave propagation, cylindrical wave propagation, or the like.

[0024] The noise equivalent sound pressure p_{NEP} is divided and corrected by the decay ratio A for $p_{\text{NEP}_c}(r)$ that is the decay compensation noise equivalent sound pressure value. That is, if the minimum block unit of the position vector r has generated an elastic wave of a sound pressure of $p_{\text{NEP}_c}(r)$, the elastic wave is detected by the transducer 102. Thus, through correction using the decay ratio in the greatest distance $\max|d_i-r|$ in which the sound pressure decays most, it can be guaranteed that a transducer in a distance nearer than $\max|d_i-r|$ can detect the elastic wave.

[0025] The absorption coefficient of the object 100 set in the light intensity distribution calculation unit 107 by the optical characteristic value setting unit 105 is μ_{a_BG} . The absorption coefficient of tumor presumably has a value greater with respect to μ_{a_BG} that is an average coefficient of the object 100. This is because a tumor is rich in blood of a large absorption coefficient since new blood vessels are drawn in. From Formula (1), the sound pressure of the generated elastic wave is small when the absorption coefficient is small. Therefore, at least when $\Phi_{th}(r)$ obtained using μ_{a_BG} is the threshold value, an elastic wave caused by the tumor that is a target for imaging can be detected. In Formula (3), Γ is the Gruneisen coefficient, and it is recommended that a value typical for a biological body be input in the case where the object 100 is a biological body, for example.

[0026] The light intensity domain setting unit 108 calculates the threshold value of light intensity for each minimum block unit in a manner described above.

[0027] Next, the light intensity domain will be described. Fig. 2 is a diagram showing the details of the light intensity domain setting unit 108. Reference numeral 202 in the upper left in the drawing shows the light intensity distribution calculated by the light intensity distribution calculation unit 107. The intensity of the light is stronger when nearer the irradiation unit 101. The light intensity distribution 202 is output to the light intensity domain setting unit 108 as a light intensity distribution 203 for each minimum block unit 201.

[0028] In the light intensity domain setting unit 108 on the right side in the drawing, Φ_i shown in the light intensity distribution 203 for each minimum block unit shows the light intensity of the minimum block unit of the number i . When the position vector of the i -th minimum block unit is r_i , $\Phi_i = \Phi(r_i)$ (where $\Phi(r_i)$ is the light intensity of the minimum block unit of the position vector r_i). Reference numeral 204 denotes a threshold value of light intensity for each minimum block unit that is calculated for each minimum block unit by Formula (2) and Formula (3). The threshold value of light intensity of the minimum block unit of the number i is shown by Φ_{ti} shown in the threshold value 204 of light intensity for each minimum block unit. In a similar manner to reference numeral 203, $\Phi_{ti} = \Phi_{th}(r_i)$.

[0029] The light intensity domain setting unit 108 further includes a light intensity domain storage unit 205 that stores a value corresponding to each minimum block unit forming the object 100. The light intensity domain setting unit 108 compares Φ_i and Φ_{ti} of the same number i , and sets 1 in a storage area for the corresponding minimum block unit in the light intensity domain storage unit 205 if $\Phi_i \geq \Phi_{ti}$. The light intensity domain setting unit 108 sets 0 in a storage area other than for the corresponding minimum block unit. A domain of black minimum block units shown in the light intensity domain storage unit 205 is a light intensity domain. The light intensity domain setting unit 108 sets the minimum block unit within the light intensity domain in the reconstruction unit 109 by outputting a value in the light intensity domain storage unit 205 to the reconstruction unit 109.

[0030] The reconstruction unit 109 as generating unit generates (reconstructs) photoacoustic image data using a plurality of the electrical signals output from the probe 103. As a method of reconstruction, a back projection method or the like with time domain or Fourier domain that is normally used in a tomography technique may be used. The photoacoustic image data in the present invention, whether in two dimension or three dimension, refers to data showing information (biological information such as in vivo initial sound pressure distribution, light absorption coefficient distribution, or oxygen saturation) inside the object. The photoacoustic image data is configured as an arrangement of a plurality of pixels that are the minimum block units in a two-dimensional case, and is configured as an arrangement of a plurality of voxels that are the minimum block units in a three-dimensional case.

[0031] The reconstruction unit 109 selectively reconstructs the minimum block unit within the light intensity domain set by the light intensity domain setting unit 108 that is the setting unit out of the minimum block units forming the object 100, and generates data with which the inside of the object 100 is imaged.

[0032] The data with which the inside of the object 100 is imaged is transferred to a display unit 110 and displayed with respect to the operator.

[0033] The light intensity distribution calculation unit 107, the light intensity domain setting unit 108, and the reconstruction unit 109 described above may be a program installed in a computer or may be an electronic circuit.

[0034] The flow of measurement in this embodiment is shown in Fig. 3.

[0035] In step S301, the measurement is started.

[0036] In step S302 that is a characteristic setting step, the operator executes a characteristic inputting step of inputting the optical characteristic value (the absorption coefficient and the equivalent scattering coefficient) of the object 100 from the optical characteristic value input unit 106. The input absorption coefficient and equivalent scattering coefficient are set in the light intensity distribution calculation unit 107 and the light intensity domain setting unit 108.

[0037] In step S303 that is a detecting step, the object 100 irradiated with light from the irradiation unit 101, and the elastic wave generated in the object 100 by light irradiation is detected by the transducer 102. The detected elastic wave is output as the received signal from the probe 103.

[0038] In step S304 that is a distribution acquiring step, the light intensity distribution inside the object 100 is calculated in the light intensity distribution calculation unit 107 using the absorption coefficient and the equivalent scattering coefficient input in step S302.

[0039] In step S305 that is a setting step, the light intensity domain is calculated and the minimum block unit inside the light intensity domain is extracted by the light intensity domain setting unit 108 using the absorption coefficient input in step S302 and the light intensity distribution obtained in step S304. The extracted minimum block unit is set in the reconstruction unit 109.

[0040] In step S306 that is a generating step, the minimum block unit extracted and set in step S305 is reconstructed in the reconstruction unit 109 using the received signal obtained in step S303. Accordingly, image data of the inside of the object is obtained.

[0041] In step S307, the image data of the inside of the object obtained in step S306 is displayed in the display unit 110.

[0042] In step S308, the measurement is terminated.

[0043] In the first embodiment, the minimum block units to be reconstructed can be reduced and the time until acquisition of the object information can be shortened by selectively reconstructing the minimum block unit included in a domain having sufficient light intensity obtained from the input optical characteristic value of the object.

<Second embodiment>

[0044] In a second embodiment, an optical characteristic value of an object is actually measured and acquired, and a domain for which object information is acquired is limited based on the light intensity distribution calculated from the optical characteristic value to shorten the time required for the acquisition of the object information. As the optical characteristic value, the absorption coefficient that is an absorption characteristic value and the equivalent scattering coefficient that is a scattering characteristic value are measured.

(Apparatus configuration)

[0045] Fig. 4 is a diagram showing an overview of a photoacoustic imaging apparatus in a second embodiment of the present invention. In the second embodiment, when compared to the first embodiment, the optical characteristic value input unit is replaced with an optical characteristic value measurement unit 403, and a light source 401 and a light detection unit 402 are added. Since other components are the same as in the first embodiment, description is omitted regarding terms that are the same. Only configurations that differ from the first embodiment will be described below.

[0046] The light source 401 that is unit of light irradiation for optical characteristic value measurement irradiates the object 100 with light (optical characteristic value measurement light) for measuring the optical characteristic value (the absorption coefficient that is the absorption characteristic value and the equivalent scattering coefficient that is the scattering characteristic value) of the object 100. It is desirable that the wavelength of radiated light be close to the wavelength of light radiated by the irradiation unit 101. For the light source 401, a light source that generates either pulsed light or intensity-modulated light may be used. For example, a laser diode may be used. In the case of pulsed light, it is desirable that the pulse width be several to several hundreds of picoseconds (ps). In the case of intensity-modulated light, it is desirable that the frequency of intensity modulation be several to several hundreds of megahertz.

[0047] The light detection unit 402 that is unit of detecting light for optical characteristic value measurement detects the optical characteristic value measurement light that is radiated by the light source 401 and has propagated inside the object 100. A detector that responds quickly with respect to at least the pulse width or the frequency of intensity modulation is desirable. For example, a photomultiplier, an avalanche photodiode, a photodiode, or the like may be used. A detection light signal obtained through detection of the optical characteristic value measurement light is output to the optical characteristic value measurement unit 403 that is characteristic measuring unit.

[0048] The optical characteristic value measurement unit 403 calculates the absorption coefficient and the reduced scattering coefficient of the object 100 using the detection light signal output from the light detection unit 402. For calculation, an analytical solution or numerical solution method of transport equations, an analytical solution or numerical solution method of diffusion approximation equations, a numerical solution method using a Monte Carlo method, or the like may be used.

[0049] In the case where the light source 401 generates pulsed light, the absorption coefficient and the reduced

scattering coefficient are changed such that an analytical solution and the time waveform of the detection light signal match, and the absorption coefficient and the equivalent scattering coefficient at the time of a sufficient match is assumed as the absorption coefficient and the equivalent scattering coefficient of the object. In a similar manner, a numerical solution of the time waveform using a numerical solution method and the time waveform of the detection light signal may be caused to match.

[0050] In the case where the light source 401 generates intensity-modulated light, an analytical solution and the detection light signal are caused to match in the decay rate of intensity modulation amplitude (amplitude decay rate) of the detection light signal with respect to the intensity modulation amplitude at the time of incidence upon the object 100 and the phase delay of the intensity modulation of the detection light signal. The amplitude decay rate and the phase delay using a numerical solution method may also be used.

[0051] The absorption coefficient and the equivalent scattering coefficient of the object measured by the optical characteristic value measurement unit 403 in this manner is set in the light intensity distribution calculation unit 107 and the light intensity domain setting unit 108 by the optical characteristic value setting unit 404.

[0052] The flow of measurement in the second embodiment is shown in Fig. 5. For Fig. 5, description of steps in which the same processes as in Fig. 3 are performed will be omitted.

[0053] Step S501 is the same as step S301 in the first embodiment.

[0054] In step S502, the object 100 is irradiated with the optical characteristic value measurement light from an optical characteristic value measurement light irradiation light source 401.

[0055] In step S503, the optical characteristic value measurement light having propagated in the object 100 is detected by an optical characteristic value measurement light detector 402 to obtain the detection light signal.

[0056] In step S504, the absorption coefficient and the reduced scattering coefficient of the object 100 are calculated in the optical characteristic value measurement unit 403 using the detection light signal obtained in step S503.

[0057] Step S505 is the same as step S303 in the first embodiment.

[0058] In step S506 that is a distribution acquiring step, the light intensity distribution inside the object 100 is calculated in the light intensity distribution calculation unit 107 using the absorption coefficient and the reduced scattering coefficient obtained through measurement in step S503.

[0059] In step S507 that is a setting step, a light intensity domain is calculated and a minimum block unit inside the light intensity domain is extracted by the light intensity domain setting unit 108 using the absorption coefficient obtained through measurement in step S503 and the light intensity distribution obtained in step S506. The extracted minimum block unit is set in the reconstruction unit 109.

[0060] Step S508 is the same as step S306 in the first embodiment.

[0061] Step S509 is the same as step S307 in the first embodiment.

[0062] In step S510, the measurement is terminated.

[0063] In the second embodiment, the minimum block units to be reconstructed can be reduced and the time until acquisition of the object information can be shortened by selectively reconstructing the minimum block unit included in a domain having sufficient light intensity obtained from the optical characteristic value of the object obtained through measurement. By using the absorption coefficient and the reduced scattering coefficient of the object obtained through measurement, the domain with sufficient light intensity can be designated with higher precision.

<Third embodiment>

[0064] In a third embodiment, a domain to be imaged is limited based on the light intensity distribution inside an object prepared in advance. Accordingly, since the time of acquiring the light intensity distribution can be shortened compared to other embodiments, the time required for acquisition of object information can be shortened further.

[0065] Fig. 6 is a diagram showing an overview of a photoacoustic imaging apparatus in the third embodiment of the present invention. In the third embodiment, the light intensity distribution calculation unit 107 is replaced with a light intensity distribution storage unit 601 when compared to the first embodiment. Since other components are the same as in the first embodiment, description is omitted regarding terms that are the same. Only configurations that differ from the first embodiment will be described below.

[0066] The light intensity distribution storage unit 601 stores the light intensity distribution calculated in advance. For example, the light intensity distribution can be stored as volume data showing the inside of the object 100. As the light intensity distribution storage unit 601, a hard disk, a non-volatile memory, or the like may be used. The light intensity distribution to be stored can be calculated using a general optical characteristic value for a biological body. In calculating in advance the light intensity distribution to be stored, the intensity distribution pattern of irradiation light measured in advance can be reflected.

[0067] Note that the light intensity distribution storage unit 601 preferably can store a plurality of light intensity distributions. That is, a light intensity distribution corresponding to the optical characteristic value of the object set by the optical characteristic value setting unit 105 can be selected. Since there are endless patterns to the optical characteristic

value and it is difficult to store all of the corresponding light intensity distributions at this time, it is recommended that light intensity distributions for a limited number of patterns of the optical characteristic value be stored. In the case where a certain optical characteristic value is input, one that is closest to the optical characteristic value among the limited number of optical characteristic values is selected, and a light intensity distribution corresponding to the selected optical characteristic value is used.

[0068] Note that a general value for a biological body, a statistical value according to the characteristic of the object 100, a measured value obtained through measurement of the object 100, or the like may be used for the optical characteristic value to be set. Although the light intensity distribution is stored in the light intensity distribution storage unit 601 in this embodiment, the light intensity domain setting unit 108 may be included in the light intensity distribution storage unit 601 to store the light intensity distribution.

[0069] The flow of measurement in this embodiment is shown in Fig. 7. For Fig. 7, description of steps in which the same processes as in Fig. 3 are performed will be omitted.

[0070] Step S701 is the same as step S301.

[0071] In step S702 that is a characteristic setting step, an operator executes a characteristic inputting step of inputting an optical characteristic value (the absorption coefficient and the reduced scattering coefficient) of the object 100 from the optical characteristic value input unit 105. The input absorption coefficient and equivalent scattering coefficient are set in the light intensity distribution storage unit 601 and the light intensity domain setting unit 108. Alternatively, the optical characteristic value obtained through measurement of the object 100 is set in the light intensity distribution storage unit 601 and the light intensity distribution calculation unit 107.

[0072] In step S704 that is a distribution acquiring step, the light intensity distribution corresponding to the optical characteristic value set in step S703 is read from the light intensity distribution storage unit 601 to obtain the light intensity distribution inside the object 100. Alternatively, the light intensity domain is read in the case where the light intensity domain is stored in the light intensity distribution storage unit 601. In this case, calculation of the light intensity domain in step S705 is omitted.

[0073] Steps S705 to S708 are respectively the same as steps S305 to S308.

[0074] In the third embodiment, a minimum block unit included in a domain having sufficient light intensity acquired from the light intensity distribution calculated in advance is selectively reconstructed. Accordingly, since the number of minimum block units to be reconstructed can be reduced and the time required for acquisition of the light intensity distribution can be shortened, the time until acquisition of the object information can be shortened further.

<Fourth embodiment>

[0075] In a fourth embodiment, the number of minimum block units to be reconstructed can be reduced and the time until acquisition of object information can be shortened compared to other embodiments by selectively reconstructing the minimum block unit included in both a domain of the directivity range of a transducer and a domain having sufficient light intensity.

(Apparatus configuration)

[0076] Fig. 8 is a diagram showing an overview of a photoacoustic imaging apparatus in the fourth embodiment of the present invention. In the fourth embodiment, a directivity range domain setting unit 801 is added and the behavior of the reconstruction unit 109 differs when compared to the first embodiment. Since other components are the same as in the first embodiment, description is omitted regarding terms that are the same. Only configurations that differ from the first embodiment will be described below.

[0077] With the directivity range domain setting unit 801 that is directivity setting unit, the minimum block unit within the directivity range of the transducer 102 among the minimum block units forming the object 100 is extracted and set in the reconstruction unit 109. A directivity range is a domain determined by a directivity angle that is the angle in which the transducer 102 can receive an elastic wave. The directivity range will be described using Fig. 9.

[0078] In Fig. 9, reference numeral 901 denotes the directivity angle of one transducer 102. Herein, a case where the directivity angle is 20° is shown. An elastic wave generated in a range inside the directivity angle 901 can be detected by the transducer 102. Thus, an elastic wave generated in a range inside the directivity angle of any one of the plurality of transducers 102 forming the probe 103 can be output from the probe 103 as a received signal. That is, a portion shown in black in Fig. 2 among the minimum block units 201 can be reconstructed from the received signal. The domain shown in black is the directivity range. Note that the directivity angle can be specified in various ways according to the precision desired in the measurement or the characteristic of the transducer. For example, in the case where the receiving sensitivity is maximum in the normal direction of the transducer, the directivity angle may be a range of a half width that enables reception with intensity half the maximum sensitivity.

[0079] As shown in Fig. 10, the directivity range domain setting unit 801 includes a directivity range storage unit 1001

that stores a value corresponding to each minimum block unit forming the object 100. In the directivity range storage unit 1001, a storage area corresponding to the minimum block units within the directivity range is set to 1, and a storage area corresponding to other minimum block units is set to 0. The directivity range domain setting unit 801 sets, in the reconstruction unit 109, the minimum block unit that is present inside the directivity range by outputting a value of the

[0080] The reconstruction unit 109 selectively reconstructs the minimum block unit set in both the light intensity domain setting unit 108 that is setting unit and the directivity range domain setting unit 801 that is the directivity setting unit among the minimum block units forming the object 100. The details will be described below.

[0081] Fig. 11 is a diagram showing the details of the reconstruction unit 109. Reference numeral 1101 denotes data showing the minimum block unit within the light intensity domain set by the light intensity distribution calculation unit 107, and reference numeral 1102 denotes data showing the minimum block unit within the directivity range domain set by the directivity range domain setting unit 801. The reconstruction unit 109 performs a multiplication operation for each minimum block unit corresponding to reference numeral 1101 and reference numeral 1102. The result of the multiplication operation is stored in a storage area of the corresponding minimum block unit in a reconstruction domain storage unit 1103. A reconstruction processing unit 1104 performs reconstruction of the minimum block unit that is set to 1 by the reconstruction domain storage unit and generates data with which the inside of the object is imaged.

[0082] The flow of measurement in this embodiment is shown in Fig. 12. For Fig. 12, description of steps in which the same processes as in Fig. 3 are performed will be omitted.

[0083] Step S1201 to step S1205 are respectively the same as step S301 to step S305.

[0084] In step S1206 that is a directivity setting step, the minimum block unit included in the domain within the directivity range of the transducer 102 is extracted. The extracted minimum block unit is set in the reconstruction unit 109.

[0085] In step S1207 that is a generating step, the minimum block unit extracted and set in both step S1205 and step S1206 is reconstructed in the reconstruction unit 109 using the received signal obtained in step S1203. Accordingly, image data of the inside of the object is obtained.

[0086] Step S1208 and step S1209 are respectively the same as step S307 and step S308.

[0087] In the fourth embodiment above, the number of minimum block units to be reconstructed can be reduced and the time until acquisition of the object information can be shortened compared to other embodiments by selectively reconstructing the minimum block unit included in both the domain of the directivity range of the transducer and the domain having sufficient light intensity.

[0088] Note that the minimum block unit included in the domain of the directivity range of the transducer may be selectively reconstructed. That is, the minimum block unit not included in the domain of the range of the directivity of the transducer may be not reconstructed. Accordingly, the time until acquisition of the object information can be shortened.

[0089] With the present invention, as described above, a domain within an object to be reconstructed is set in consideration of the light intensity distribution within the object in photoacoustic imaging. Since a domain with light intensity that generates an elastic wave of sufficient sound pressure is selected and reconstructed as a result, the time until acquisition of object information can be shortened.

[0090] While the present invention has been described with reference to exemplary embodiments, it is to be understood that the invention is not limited to the disclosed exemplary embodiments. The scope of the following claims is to be accorded the broadest interpretation so as to encompass all such modifications and equivalent structures and functions.

Claims

1. An object information acquisition apparatus comprising:

an irradiating unit (101) configured to irradiate an object (100) with light;
a plurality of detecting units (102) configured to receive an elastic wave generated by irradiating the object (100) with light and convert the elastic wave to a signal;
a distribution acquiring unit (107, 601) configured to acquire a light intensity distribution within the object (100);
characterized by
a setting unit (108) configured to select a minimum block unit within a light intensity domain in which light intensity is greater than or equal to a predetermined threshold value, using the light intensity distribution; and
a generating unit (109) configured to generate image data representing object information in the object by selectively reconstructing the minimum block unit selected by the setting unit (108), using the signal.

2. The object information acquisition apparatus according to claim 1, further comprising a characteristic setting unit configured to set an optical characteristic value of the object, wherein the distribution acquiring unit is configured to acquire the light intensity distribution using the optical characteristic value set by the characteristic setting unit.

3. The object information acquisition apparatus according to claim 2, wherein the optical characteristic value is an absorption characteristic value showing an absorption characteristic of the object and a scattering characteristic value showing a scattering characteristic.
- 5 4. The object information acquisition apparatus according to claim 3, wherein the setting unit is configured to assume a value obtained by dividing a noise equivalent sound pressure of the signal by the absorption characteristic value and a Gruneisen coefficient of the object as the predetermined threshold value.
- 10 5. The object information acquisition apparatus according to claim 4, wherein the setting unit is configured to correct, upon calculating the predetermined threshold value for each of the minimum block units, the noise equivalent sound pressure with a decay ratio of sound pressure upon propagation of the elastic wave between that minimum block unit and the detecting unit.
- 15 6. The object information acquisition apparatus according to claim 3, wherein the setting unit is configured to set the predetermined threshold value such that an elastic wave generated from a minimum block unit of which the absorption characteristic value is greater than an average value of the object can be detected.
- 20 7. The object information acquisition apparatus according to claim 2, wherein the characteristic setting unit includes a characteristic input unit configured to input the optical characteristic value.
8. The object information acquisition apparatus according to claim 7, wherein the characteristic input unit is configured to accept an input of the optical characteristic value performed by an operator.
- 25 9. The object information acquisition apparatus according to claim 2, wherein the characteristic setting unit includes a characteristic measuring unit configured to measure the optical characteristic value.
- 30 10. The object information acquisition apparatus according to claim 9, wherein the characteristic measuring unit includes a unit configured to irradiate the object with optical characteristic value measurement light for measuring the optical characteristic value, and a unit configured to detect light resulting from the optical characteristic value measurement light having propagated through the object.
- 35 11. The object information acquisition apparatus according to claim 1, further comprising a distribution storage unit configured to store a light intensity distribution acquired in advance, wherein the distribution acquiring unit is configured to acquire the light intensity distribution from the distribution storage unit.
- 40 12. The object information acquisition apparatus according to claim 11, further comprising a characteristic setting unit configured to set an optical characteristic value of the object, wherein the distribution acquiring unit is configured to select a light intensity distribution corresponding to the optical characteristic value set by the characteristic setting unit from a plurality of the light intensity distributions stored in the distribution storage unit.
- 45 13. The object information acquisition apparatus according to any one of claims 1 to 12, further comprising a directivity setting unit configured to select a minimum block unit included in a directivity range domain determined by a directivity angle of the detecting unit, wherein the generating unit is configured to reconstruct a minimum block unit included in both the minimum block unit selected by the setting unit and the minimum block unit selected by the directivity setting unit.
- 50 14. The object information acquisition apparatus according to any one of claims 1 to 12, wherein the generating unit is configured not to reconstruct a minimum block other than the minimum block unit selected by the setting unit.
- 55 15. The object information acquisition apparatus according to claim 13, wherein the generating unit is configured not to reconstruct a minimum block unit other than the minimum block unit included in both the minimum block unit selected by the setting unit and the minimum block unit selected by the directivity setting unit.

Patentansprüche

1. Objektinformationserhaltevorrichtung mit:

einer Bestrahlungseinheit (101), die konfiguriert ist, ein Objekt (100) mit Licht zu bestrahlen;
 einer Vielzahl von Erfassungseinheiten (102), die konfiguriert sind, eine elastische Welle, die durch Bestrahlen
 des Objekts (100) mit Licht erzeugt wird, zu empfangen und die elastische Welle in ein Signal umzuwandeln;
 eine Verteilungserhalteinheit (107, 601), die konfiguriert ist, eine Lichtintensitätsverteilung innerhalb des Ob-
 jekts (100) zu erhalten;

gekennzeichnet durch

eine Einstelleinheit (108), die konfiguriert ist, eine minimale Blockeinheit innerhalb einer Lichtintensitätsdomäne,
 in der eine Lichtintensität größer als oder gleich einem vorbestimmten Schwellenwert ist, unter Verwendung
 der Lichtintensitätsverteilung auszuwählen; und

eine Erzeugungseinheit (109), die konfiguriert ist, Bilddaten, die eine Objektinformation in dem Objekt reprä-
 sentieren, durch selektives Rekonstruieren der minimalen Blockeinheit, die durch die Einstelleinheit (108) aus-
 gewählt ist, unter Verwendung des Signals zu rekonstruieren.

2. Objektinformationserhaltevorrichtung nach Anspruch 1, ferner mit einer Charakteristikeinstelleinheit, die konfiguriert
 ist, einen optischen charakteristischen Wert des Objekts einzustellen, wobei die Verteilungserhalteinheit konfigu-
 riert ist, die Lichtintensitätsverteilung unter Verwendung des optischen charakteristischen Werts, der durch die
 Charakteristikeinstelleinheit eingestellt ist, zu erhalten.
3. Objektinformationserhaltevorrichtung nach Anspruch 2, wobei der optische charakteristische Wert ein charakteris-
 tischer Absorptionswert, der eine Absorptionscharakteristik des Objekts zeigt, und ein charakteristischer Streuungs-
 wert, der eine Streucharakteristik zeigt, ist.
4. Objektinformationserhaltevorrichtung nach Anspruch 3, wobei die Einstelleinheit konfiguriert ist, einen Wert, der
 durch Teilen eines Rauschäquivalenzschalldrucks des Signals durch den charakteristischen Absorptionswert er-
 halten wird, und einen Grüneisenkoeffizienten des Objekts als den vorbestimmten Schwellenwert anzunehmen.
5. Objektinformationserhaltevorrichtung nach Anspruch 4, wobei die Einstelleinheit konfiguriert ist, beim Berechnen
 des vorbestimmten Schwellenwerts für jede der minimalen Blockeinheiten den rauschäquivalenten Schalldruck mit
 einer Abfallrate des Schalldrucks bei einer Propagation der elastischen Welle zwischen der minimalen Blockeinheit
 und der Erfassungseinheit zu korrigieren.
6. Objektinformationserhaltevorrichtung nach Anspruch 3, wobei die Einstelleinheit konfiguriert ist, den vorbestimmten
 Schwellenwert so einzustellen, dass eine elastische Welle, die von einer minimalen Blockeinheit, von der der cha-
 rakteristische Absorptionswert größer als ein Durchschnittswert des Objekts ist, erfasst werden kann.
7. Objektinformationserhaltevorrichtung nach Anspruch 2, wobei die Charakteristikeinstelleinheit eine Charakteristi-
 keingabeeinheit enthält, die konfiguriert ist, den optischen charakteristischen Wert einzugeben.
8. Objektinformationserhaltevorrichtung nach Anspruch 7, wobei die Charakteristikeingabeeinheit konfiguriert ist, eine
 Eingabe des optischen charakteristischen Werts, die durch einen Operator durchgeführt wird, zu akzeptieren.
9. Objektinformationserhaltevorrichtung nach Anspruch 2, wobei die Charakteristikeinstelleinheit eine Charakteristik-
 messeinheit enthält, die konfiguriert ist, den optischen charakteristischen Wert zu messen.
10. Objektinformationserhaltevorrichtung nach Anspruch 9, wobei die Charakteristikmesseinheit eine Einheit, die kon-
 figuriert ist, das Objekt mit einem optischen Charakteristikwertmesslicht zum Messen des optischen charakteristi-
 schen Werts zu bestrahlen, und eine Einheit, die konfiguriert ist, Licht, das von dem optischen Charakteristikwert-
 messlicht resultiert, das durch das Objekt propagiert ist, zu erfassen, enthält.
11. Objektinformationserhaltevorrichtung nach Anspruch 1, ferner mit einer Verteilungsspeichereinheit, die konfiguriert
 ist, eine Lichtintensitätsverteilung, die im Voraus erhalten wurde, zu speichern, wobei die Verteilungserhalteinheit
 konfiguriert ist, die Lichtintensitätsverteilung von der Verteilungsspeichereinheit zu erhalten.
12. Objektinformationserhaltevorrichtung nach Anspruch 11, ferner mit einer Charakteristikeinstelleinheit, die konfigu-
 riert ist, einen optischen charakteristischen Wert des Objekts einzustellen, wobei die Verteilungserhalteinheit kon-
 figuriert ist, eine Lichtintensitätsverteilung entsprechend dem optischen charakteristischen Wert, der durch die Cha-
 rakteristikeinstelleinheit eingestellt ist, aus einer Vielzahl der Lichtintensitätsverteilungen, die in der Verteilungsspei-
 chereinheit gespeichert sind, auszuwählen.

13. Objektinformationserhaltevorrichtung nach einem der Ansprüche 1 bis 12, ferner mit einer Direktivitätseinstelleinheit, die konfiguriert ist, eine minimale Blockeinheit, die in einer Direktivitätsbereichsdomäne, die durch einen Direktivitätswinkel der Erfassungseinheit bestimmt wird, enthalten ist, auszuwählen, wobei die Erzeugungseinheit konfiguriert ist, eine minimale Blockeinheit, die sowohl in der minimalen Blockeinheit, die durch die Einstelleinheit ausgewählt ist, und die minimale Blockeinheit, die durch die Direktivitätseinstelleinheit ausgewählt ist, zu rekonstruieren.
14. Objektinformationserhaltevorrichtung nach einem der Ansprüche 1 bis 12, wobei die Erzeugungseinheit konfiguriert ist, keine andere minimale Blockeinheit als die minimale Blockeinheit, die durch die Einstelleinheit ausgewählt ist, zu rekonstruieren.
15. Objektinformationserhaltevorrichtung nach Anspruch 13, wobei die Erzeugungseinheit konfiguriert ist, keine andere minimale Blockeinheit als die minimale Blockeinheit, die sowohl in der minimalen Blockeinheit, die durch die Einstelleinheit ausgewählt ist, als auch in der minimalen Blockeinheit, die durch die Direktivitätseinstelleinheit ausgewählt ist, enthalten ist, zu rekonstruieren.

Revendications

1. Appareil d'acquisition d'informations d'objet, comprenant :

une unité d'exposition à un rayonnement (101) configurée pour exposer un objet (100) à un rayonnement de lumière ;
 une pluralité d'unités de détection (102) configurées pour recevoir une onde élastique générée par l'exposition de l'objet (100) à un rayonnement de lumière et pour convertir l'onde élastique en un signal ;
 une unité d'acquisition de distribution (107, 601) configurée pour acquérir une distribution d'intensité de lumière à l'intérieur de l'objet (100) ;

caractérisé par

une unité de définition (108) configurée pour sélectionner une unité minimale de bloc dans un domaine d'intensité de lumière dans lequel l'intensité de lumière est supérieure ou égale à une valeur seuil prédéterminée, au moyen de la distribution d'intensité de lumière ; et
 une unité de génération (109) configurée pour générer des données d'image représentant des informations d'objet dans l'objet par une reconstruction sélective de l'unité minimale de bloc sélectionnée par l'unité de définition (108), au moyen du signal.

2. Appareil d'acquisition d'informations d'objet selon la revendication 1, comprenant en outre une unité de définition de caractéristique configurée pour définir une valeur de caractéristique optique de l'objet, dans lequel l'unité d'acquisition de distribution est configurée pour acquérir la distribution d'intensité de lumière au moyen de la valeur de caractéristique optique définie par l'unité de définition de caractéristique.
3. Appareil d'acquisition d'informations d'objet selon la revendication 2, dans lequel la valeur de caractéristique optique est une valeur de caractéristique d'absorption montrant une caractéristique d'absorption de l'objet et une valeur de caractéristique de diffusion montrant une caractéristique de diffusion.
4. Appareil d'acquisition d'informations d'objet selon la revendication 3, dans lequel l'unité de définition est configurée pour prendre une valeur obtenue par une division d'une pression sonore équivalant à du bruit du signal par la valeur de caractéristique d'absorption et d'un coefficient de Gruneisen de l'objet en tant que la valeur seuil prédéterminée.
5. Appareil d'acquisition d'informations d'objet selon la revendication 4, dans lequel l'unité de définition est configurée pour corriger, lors d'un calcul de la valeur seuil prédéterminée de chaque unité des unités minimales de bloc, la pression sonore équivalant à du bruit à l'aide d'un taux de décroissance de pression sonore lors de la propagation de l'onde élastique entre ladite unité minimale de bloc et l'unité de détection.
6. Appareil d'acquisition d'informations d'objet selon la revendication 3, dans lequel l'unité de définition est configurée pour définir la valeur seuil prédéterminée de façon qu'une onde élastique générée à partir d'une unité minimale de bloc dont la valeur de caractéristique d'absorption est supérieure à une valeur moyenne de l'objet, puisse être détectée.
7. Appareil d'acquisition d'informations d'objet selon la revendication 2, dans lequel l'unité de définition de caractéris-

tique comprend une unité d'entrée de caractéristique configurée pour entrer la valeur de caractéristique optique.

8. Appareil d'acquisition d'informations d'objet selon la revendication 7, dans lequel l'unité d'entrée de caractéristique est configurée pour accepter une entrée de la valeur de caractéristique optique effectuée par un opérateur.

9. Appareil d'acquisition d'informations d'objet selon la revendication 2, dans lequel l'unité de définition de caractéristique comprend une unité de mesure de caractéristique configurée pour mesurer la valeur de caractéristique optique.

10. Appareil d'acquisition d'informations d'objet selon la revendication 9, dans lequel l'unité de mesure de caractéristique comprend une unité configurée pour exposer l'objet à un rayonnement de lumière de mesure de valeur de caractéristique optique afin de mesurer la valeur de caractéristique optique, et une unité configurée pour détecter la lumière obtenue à partir de la lumière de mesure de valeur de caractéristique optique qui s'est propagée à travers l'objet.

11. Appareil d'acquisition d'informations d'objet selon la revendication 1, comprenant en outre une unité d'enregistrement de distribution configurée pour enregistrer une distribution d'intensité de lumière acquise à l'avance, dans lequel l'unité d'acquisition de distribution est configurée pour acquérir la distribution d'intensité de lumière à partir de l'unité d'enregistrement de distribution.

12. Appareil d'acquisition d'informations d'objet selon la revendication 11, comprenant en outre une unité de définition de caractéristique configurée pour définir une valeur de caractéristique optique de l'objet, dans lequel l'unité d'acquisition de distribution est configurée pour sélectionner une distribution d'intensité de lumière correspondant à la valeur de caractéristique optique définie par l'unité de définition de caractéristique parmi une pluralité de distributions d'intensité de lumière enregistrées dans l'unité d'enregistrement de distribution.

13. Appareil d'acquisition d'informations d'objet selon l'une quelconque des revendications 1 à 12, comprenant en outre une unité de définition de directivité configurée pour sélectionner une unité minimale de bloc comprise dans un domaine de plage de directivité déterminé par un angle de directivité de l'unité de détection, dans lequel l'unité de génération est configurée pour reconstruire une unité minimale de bloc comprise à la fois dans l'unité minimale de bloc sélectionnée par l'unité de définition et dans l'unité minimale de bloc sélectionnée par l'unité de définition de directivité.

14. Appareil d'acquisition d'informations d'objet selon l'une quelconque des revendications 1 à 12, dans lequel l'unité de génération est configurée pour ne pas reconstruire une unité minimale de bloc autre que l'unité minimale de bloc sélectionnée par l'unité de définition.

15. Appareil d'acquisition d'informations d'objet selon la revendication 13, dans lequel l'unité de génération est configurée pour ne pas reconstruire une unité minimale de bloc autre que l'unité minimale de bloc comprise à la fois dans l'unité minimale de bloc sélectionnée par l'unité de définition et dans l'unité minimale de bloc sélectionnée par l'unité de définition de directivité.

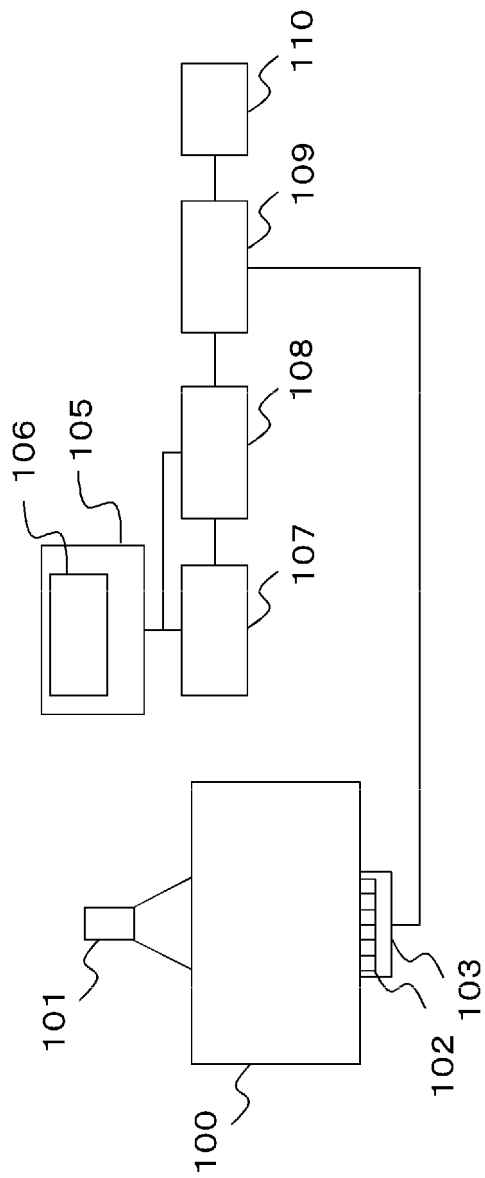


FIG. 1

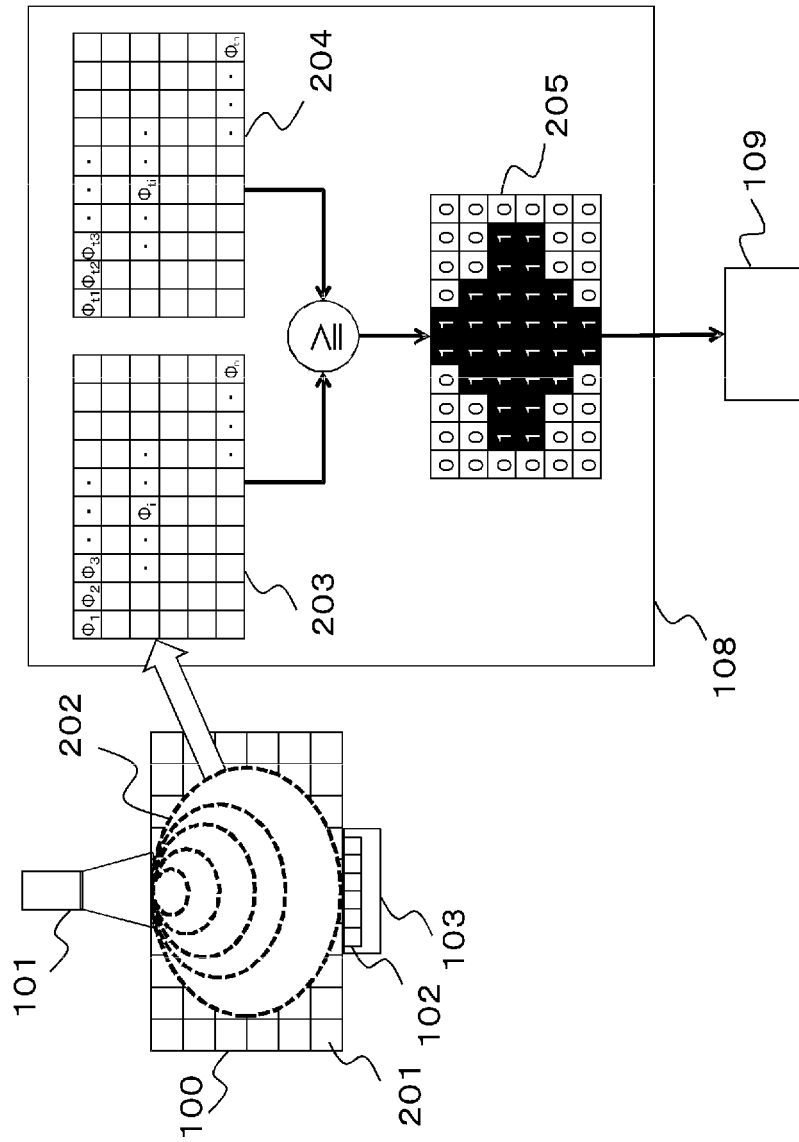


FIG. 2

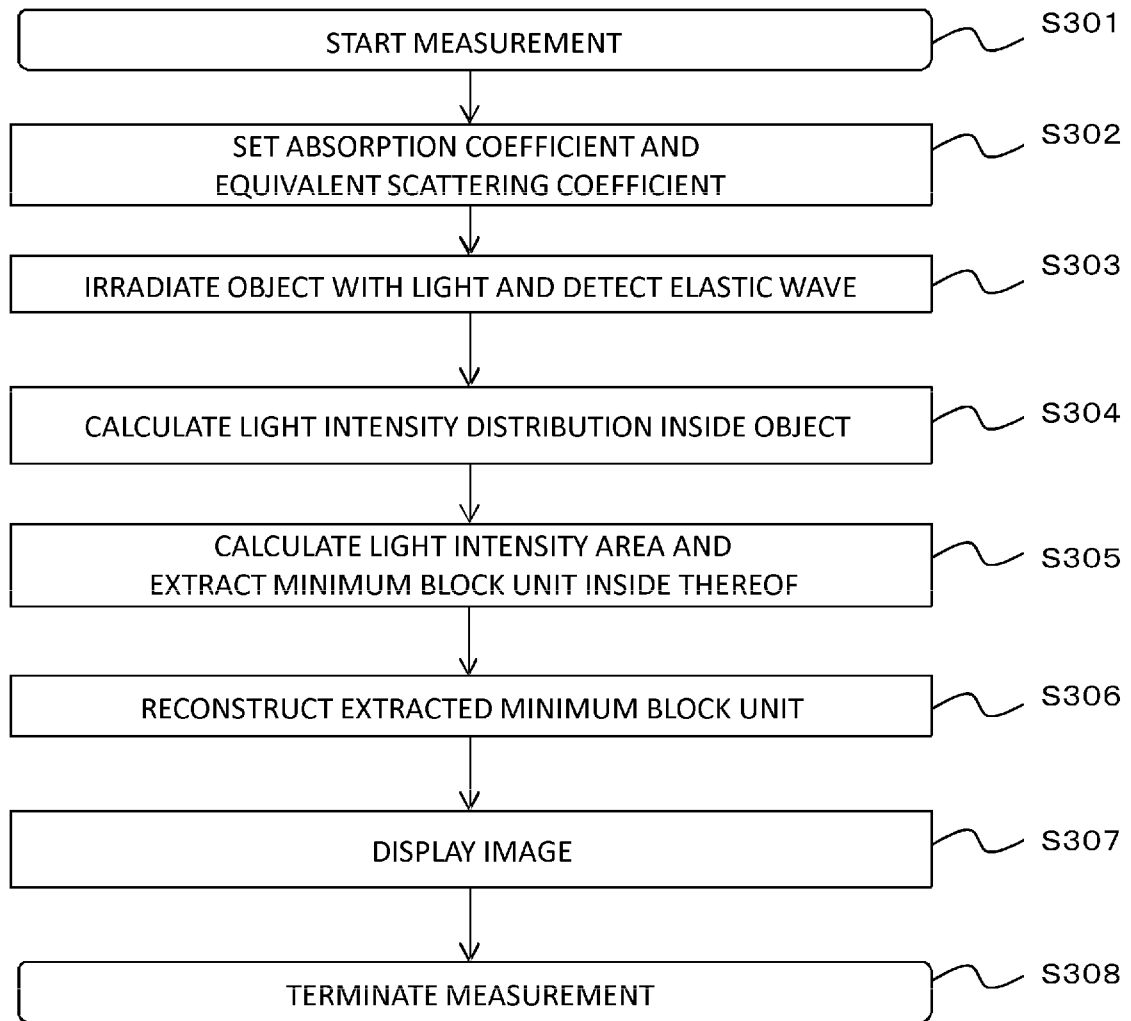


FIG. 3

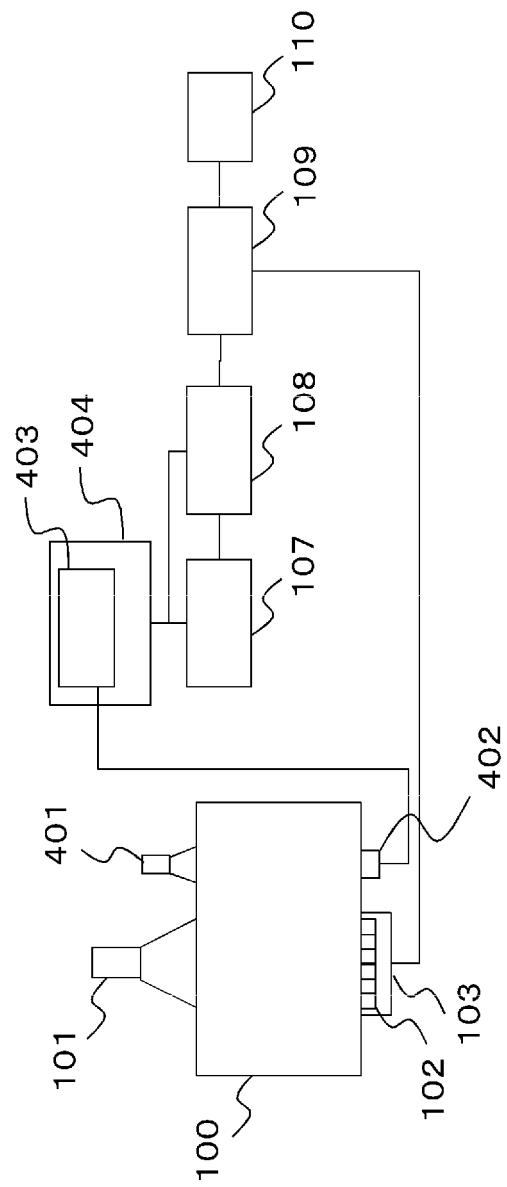


FIG. 4

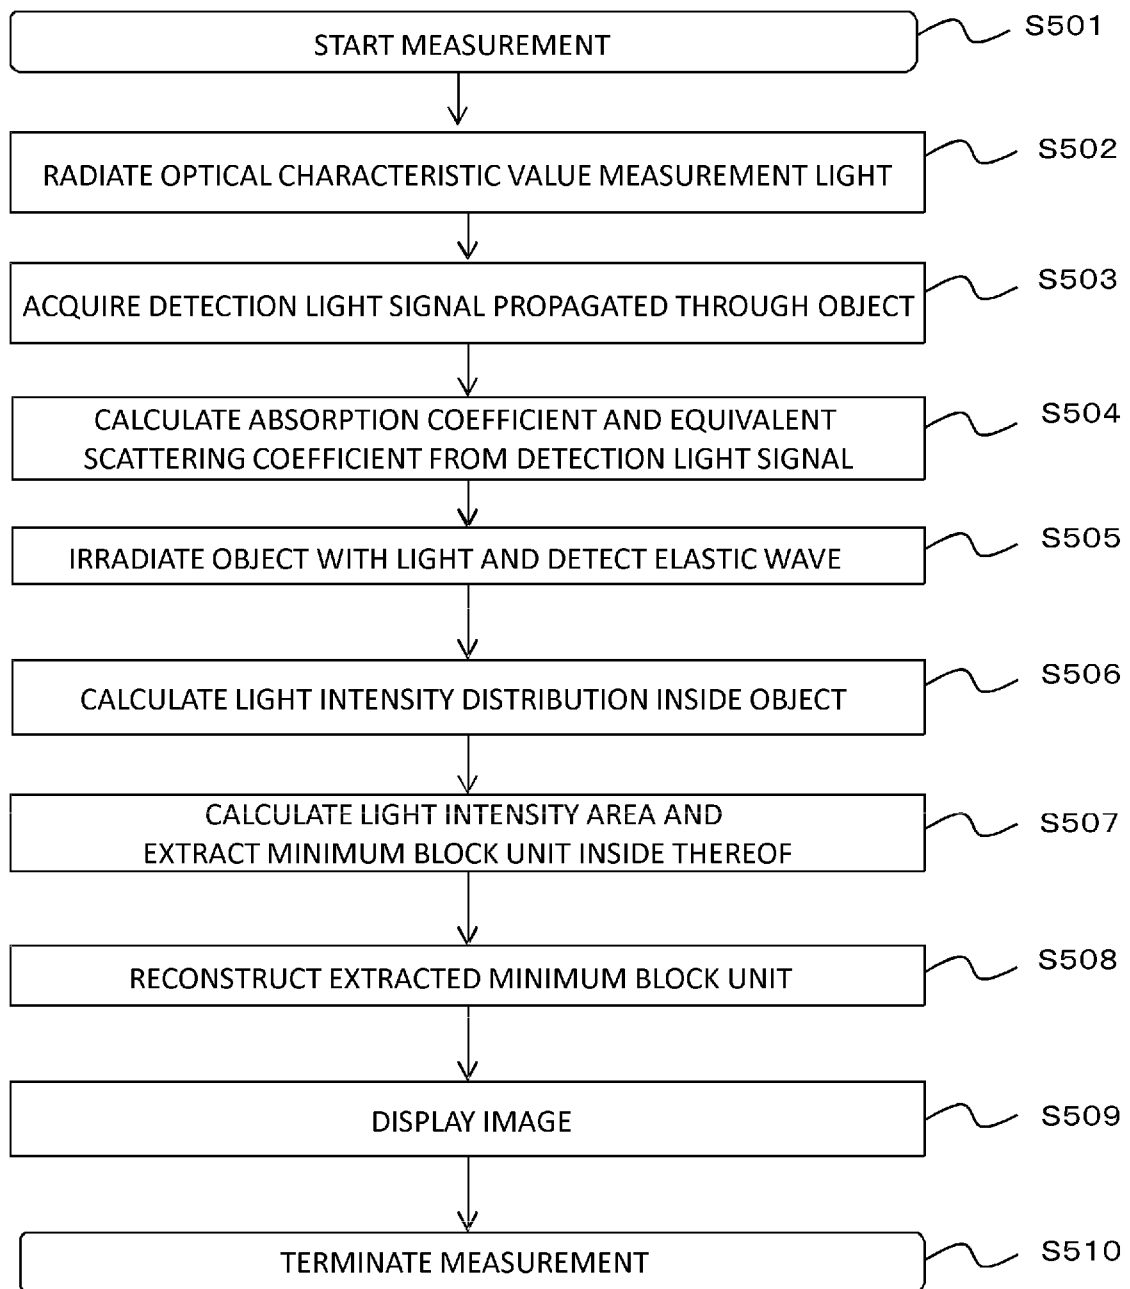


FIG. 5

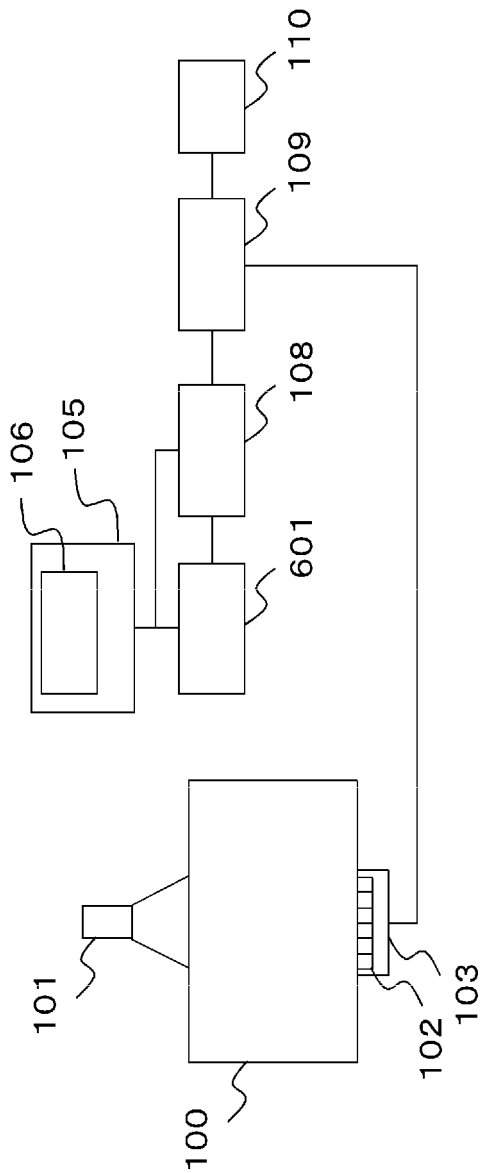


FIG. 6

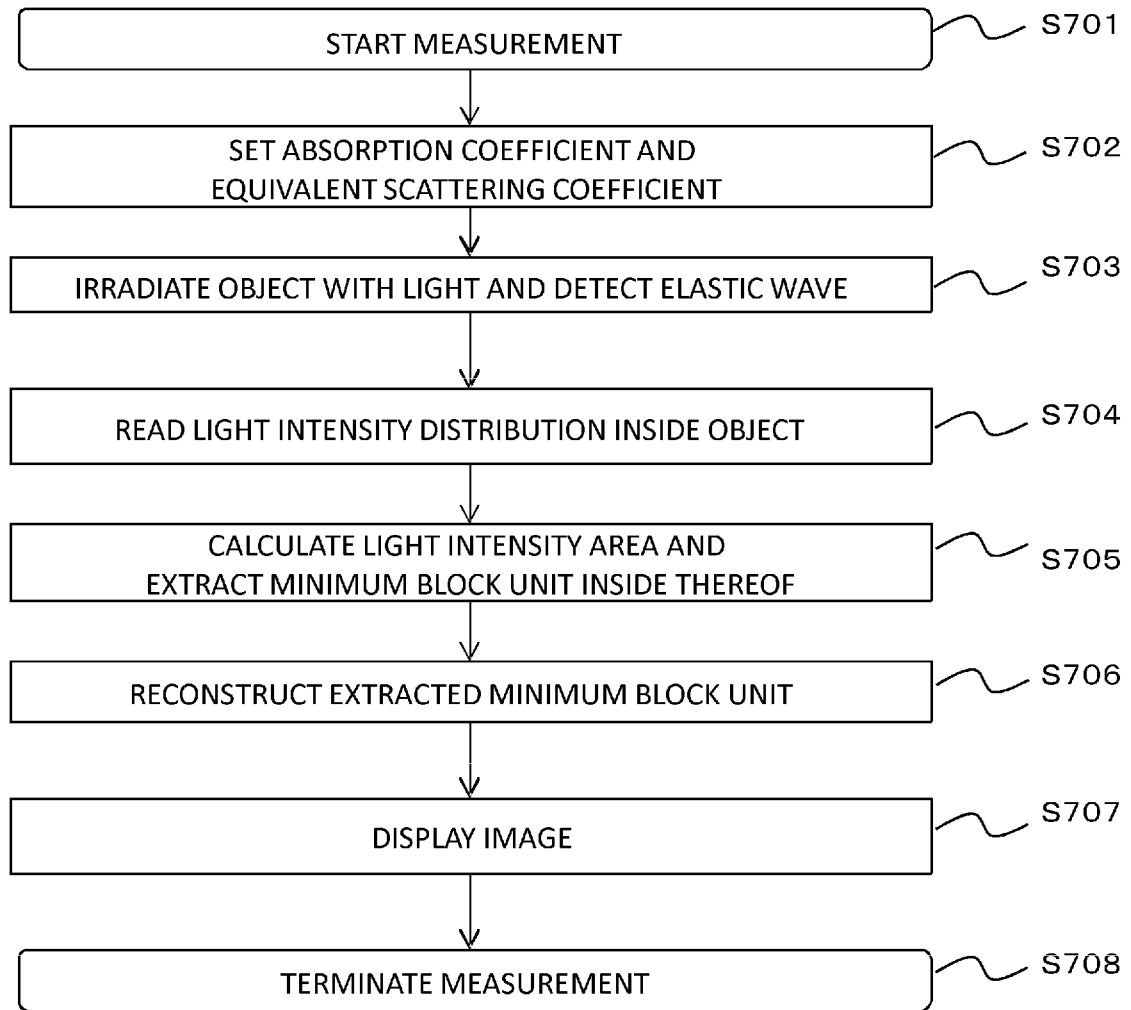


FIG. 7

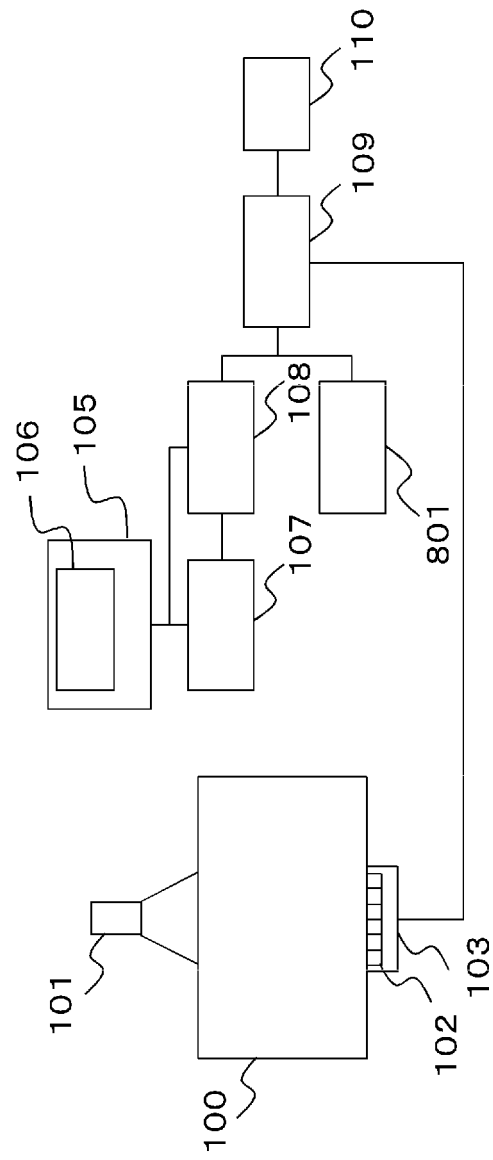


FIG. 8

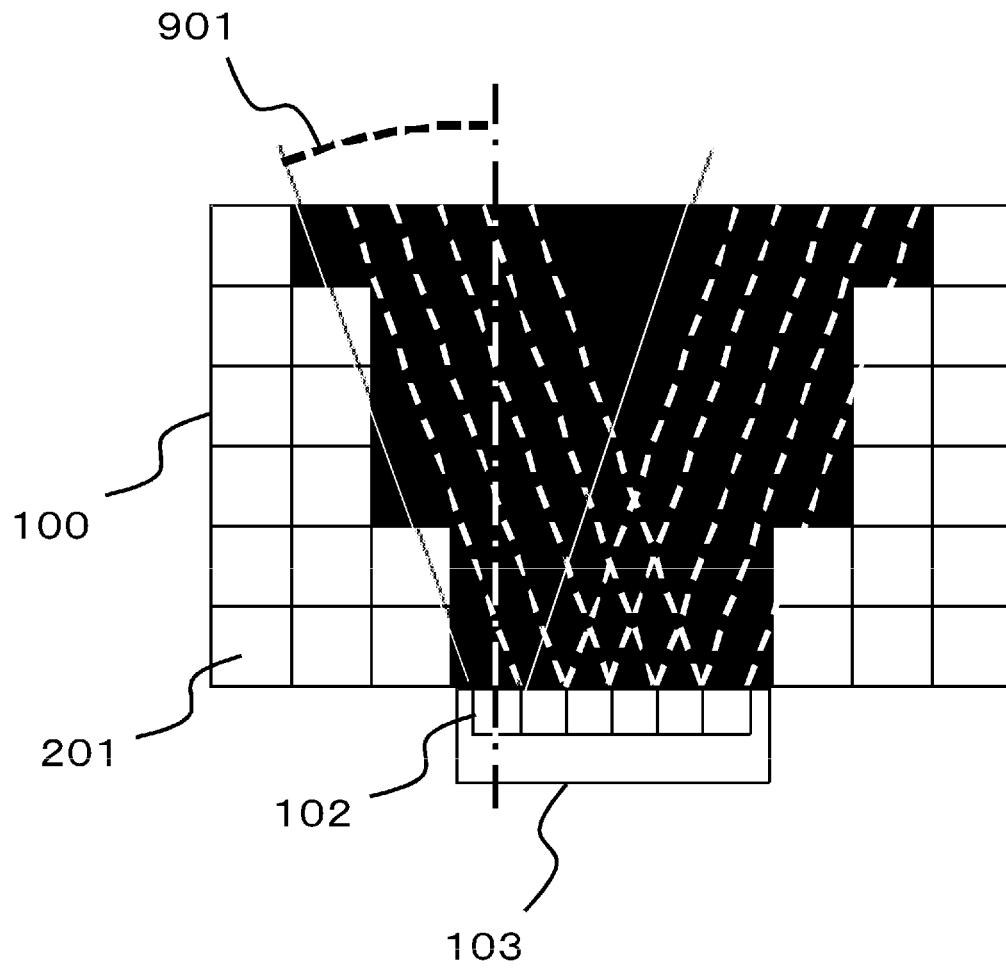


FIG. 9

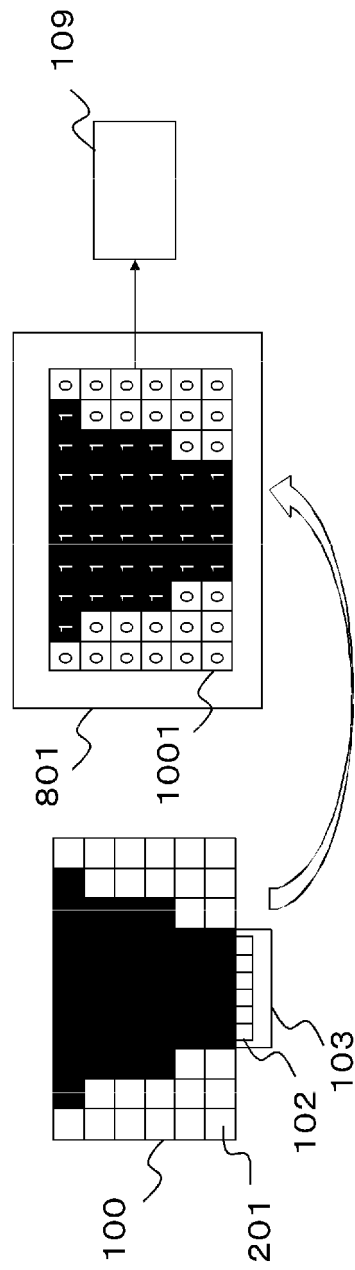


FIG. 10

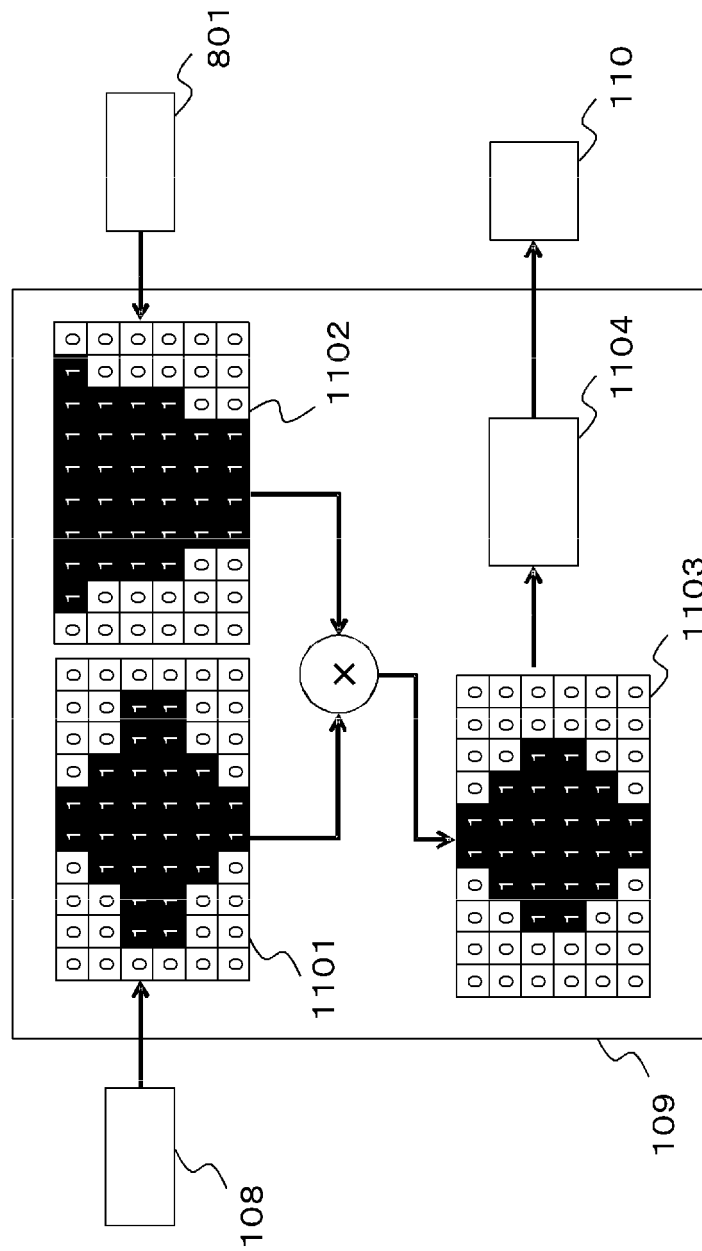


FIG. 11

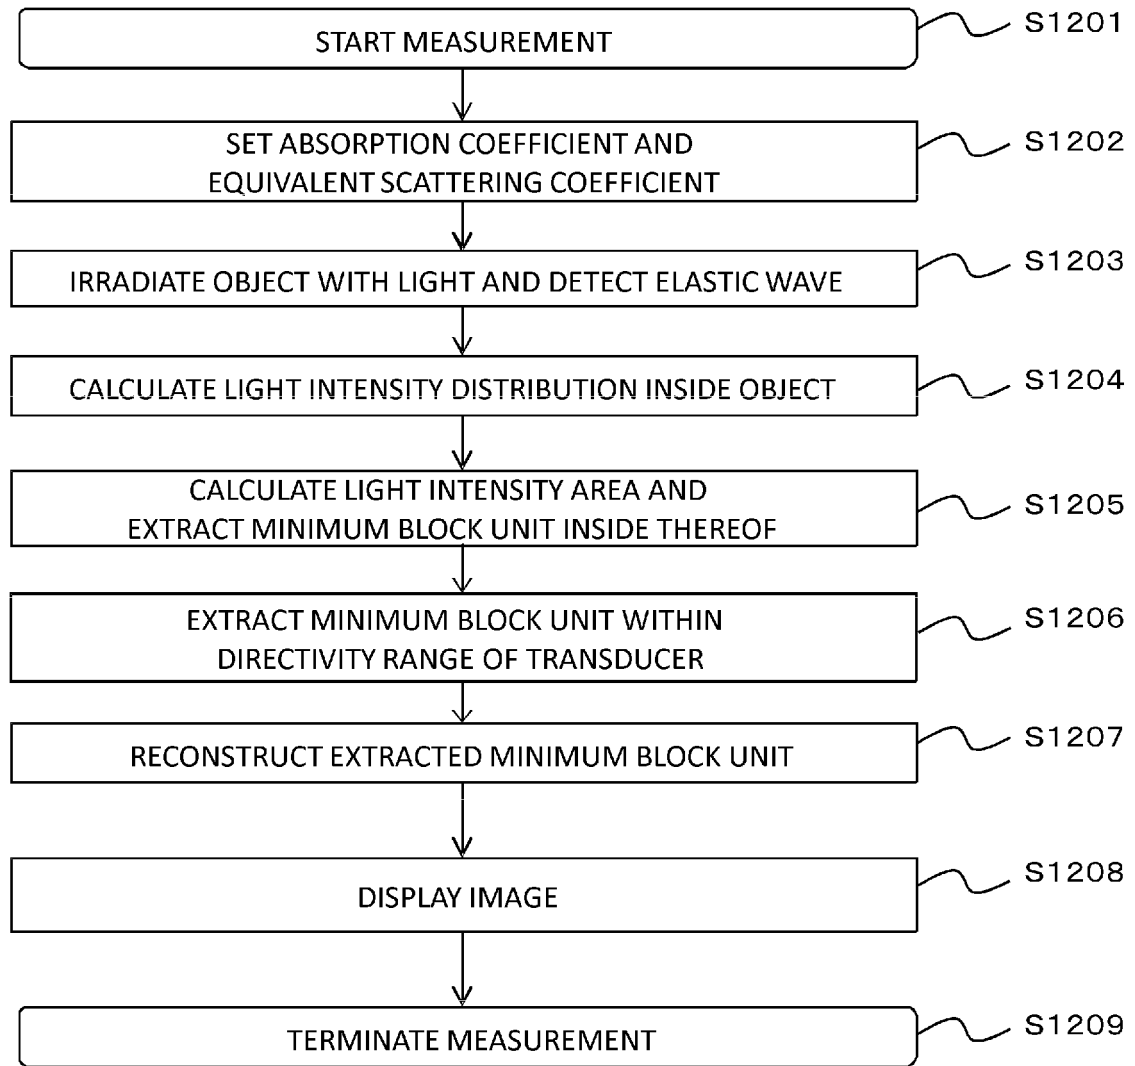


FIG. 12

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 2011245277 A [0003]
- JP 2012061055 A [0004]
- WO 2012144395 A1 [0004]
- JP 2012085965 A [0004]
- EP 2345364 A1 [0004]
- WO 2012086842 A1 [0004]
- WO 2011125468 A1 [0004]
- US 20110245652 A1 [0004]
- WO 2011096551 A1 [0004]

专利名称(译)	对象信息获取装置		
公开(公告)号	EP2732756B1	公开(公告)日	2019-09-11
申请号	EP2013190007	申请日	2013-10-24
[标]申请(专利权)人(译)	佳能株式会社		
申请(专利权)人(译)	佳能株式会社		
当前申请(专利权)人(译)	佳能株式会社		
[标]发明人	NANAUMI RYUICHI		
发明人	NANAUMI, RYUICHI		
IPC分类号	A61B5/00 A61B5/145 G06T11/00		
CPC分类号	A61B5/0095 A61B5/14542 A61B5/4312		
代理机构(译)	TBK		
优先权	2012251317 2012-11-15 JP		
其他公开文献	EP2732756A1		
外部链接	Espacenet		

摘要(译)

物体信息获取装置包括照射单元，该照射单元被配置为用光照射物体；多个检测单元，用于接收在被光照射的物体内部产生的弹性波，并将弹性波转换为接收信号；分布获取单元，被配置为获取被光照射的对象内的光强度分布；设置单元，被配置为使用光强度分布选择光强度大于或等于预定阈值的最小块单元；生成单元，被配置为使用所接收的信号生成由设置单元选择的最小块单元的对象信息。

