

(19)



(11)

EP 2 945 561 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
27.09.2017 Bulletin 2017/39

(51) Int Cl.:
A61B 90/00 ^(2016.01) **A61B 5/00** ^(2006.01)
A61B 18/14 ^(2006.01) **A61B 5/042** ^(2006.01)

(21) Application number: **14720414.3**

(86) International application number:
PCT/US2014/030702

(22) Date of filing: **17.03.2014**

(87) International publication number:
WO 2014/145866 (18.09.2014 Gazette 2014/38)

(54) **ELECTRODE CONTACT FEEDBACK SYSTEM**

ELEKTRODENKONTAKTRÜCKKOPPLUNGSSYSTEM

SYSTÈME DE RÉTROACTION DE CONTACT D'ÉLECTRODE

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

(30) Priority: **15.03.2013 US 201361798138 P**

(43) Date of publication of application:
25.11.2015 Bulletin 2015/48

(60) Divisional application:
17185963.0

(73) Proprietor: **St. Jude Medical, Atrial Fibrillation Division, Inc. St. Paul, Minnesota 55117-9913 (US)**

(72) Inventors:
• **SCHWEITZER, Jeffrey, A. St. Paul, MN 55108 (US)**
• **CHRISTIAN, Steven, C. New Brighton, MN 55112 (US)**
• **HILL, Anthony, D. Minneapolis, MN 55407 (US)**

(74) Representative: **Kramer Barske Schmidtchen Patentanwälte PartG mbB European Patent Attorneys Landsberger Strasse 300 80687 München (DE)**

(56) References cited:
EP-A1- 2 138 123 EP-A1- 2 742 886
US-A- 5 911 694 US-A1- 2012 065 506

EP 2 945 561 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

BACKGROUND

a. Field of the Disclosure

[0001] This disclosure relates to medical devices, including a catheter configured to provide an indication of contact between the catheter and tissue in a body.

b. Background Art

[0002] US 2012/0065506 A1 is directed to methods for assessing one or more mechanical properties of tissue of the body of a patient.

[0003] US 5,911,694 relates to an apparatus for detecting a change in a resonance state caused when an organic tissue as an object of measurement is touched by a body vibrating in a resonant state.

[0004] EP 2 138 123 A1 does not disclose to use a resonance frequency of an electrode tip for sensing contact with an object.

[0005] EP 2 742 886 A1, which is prior art according to Article 54(3) EPC, discloses an ultrasound apparatus that generates an ultrasound signal to supply ultrasound energy to a treatment section, wherein a fundamental frequency of the ultrasound signal is changed in response to a change of a resonance frequency of the ultrasound transducer, wherein the resonance frequency relates to the ultrasound transducer and not to a resonance frequency of an electrode tip which depends on a mechanical structure of the electrode.

[0006] Catheters are used to perform a variety of tasks within human bodies and other bodies including the delivery of medicine and fluids, the removal of bodily fluids, and the transport of surgical tools and instruments. In the diagnosis and treatment of atrial fibrillation, for example, electrodes may be added to catheters for electrophysiological mapping of the surface of the heart and to deliver ablative energy to the surface, among other tasks. Catheters are typically routed to a region of interest through the vascular system. In a conventional approach, an introducer is inserted through the skin surface and a sheath having an inner diameter greater than the outer diameter of the catheter is threaded through the vasculature to a region of interest. The catheter is then moved longitudinally through the sheath to the region of interest either manually or through the use of various types of robotic controls such as electromechanical drive systems.

[0007] In the case of an electrophysiological mapping catheter, electrode-to-tissue contact facilitates meaningful electrograms and accurate mapping of the heart. In the case of ablation catheters, sufficient contact may be required for effective formation of ablative lesions in the tissue. A variety of mechanisms and techniques have been employed to determine contact between catheters and tissue, but these are either complex and require additional components that increase the cost, size, and

complexity of the catheter, or they are non-specific and difficult to interpret.

[0008] The disclosure herein has recognized a desire for a catheter that will minimize and/or eliminate one or more of the above-identified deficiencies.

BRIEF SUMMARY

[0009] The present invention generally relates to contact feedback mechanisms. Among other things, the present disclosure relates to contact feedback mechanisms used in conjunction with catheters during cardiac ablation or diagnostic procedures.

[0010] The disclosure is directed to contact feedback mechanisms, embodiments of which are described in detail herein that include systems providing angular displacement on a spherical joint between an electrode body and its mounting structure. In one embodiment, adjacent to the spherical joint are compliant members, such as silicone, that are compressed axially under load. The axial load creates a lateral or radial expansion of the compliant members. One or more of these compliant members are fitted with strain gauges or other sensor(s) that respond to the displacement of the material with a change in resistance. With appropriate electronics, this change in resistance can be used as a signal or output to control an audible, visual, tactile (e.g., vibratory), and/or other perceptible output system mounted in the catheter handle or displayed on a monitor or other display device.

[0011] Further, the output could be tuned to respond to the magnitude of the load applied to the electrode. For example, if the output is used to drive a handle-mounted transducer that vibrates with an input signal, a frequency, amplitude, phase, and/or magnitude of this output might change to represent the relative displacement or force applied to the electrode. Or, in a similar fashion, an LED mounted in the handle might change color or intensity as the electrode contact increases.

[0012] The disclosure further relates to contact feedback mechanisms in which the compliant members and strain gauges are replaced with piezoelectric transducers that are configured to respond to input forces from any electrode deflection. In addition, the input on the piezoelectric transducer can be amplified or concentrated with small evenly spaced risers on the interface between the electrode and transducer.

[0013] The disclosure further relates to a contact sensing assembly of a medical device that may comprise a catheter including an elongate tubular body having at least a distal end, an electrode, a transducer, and a sensor. The electrode may be connected to the elongate tubular body. The transducer may be driven by an electrical signal to vibrate the electrode at a defined frequency, such as a resonant frequency, which depends on the mechanical structure of the electrode. When the electrode contacts an object, the amplitude, phase, and/or frequency of the resonant vibrations of the electrode may be dampened, and the dampening may be sensed either

through the electrical drive signal or through a second independent transducer located near the vibrating electrode.

[0014] The present disclosure further relates to a contact sensing assembly for a medical device that may comprise a catheter including an elongate body having a distal end, an electrode, an elastic or deformable member, and a sensor. The electrode may have an electrode tip and an electrode base. The electrode base may be connected to a distal end of the elongate body. The electrode tip may be connected to the electrode base via a spherical joint. The spherical joint may allow the electrode tip to move relative to the electrode base. The elastic or deformable member may be in contact with both the electrode tip and the electrode base and may be configured to elastically deform upon movement of said electrode tip relative to electrode base. The sensor may be located on the member. The sensor may be configured for measuring deformation of the member, where a magnitude of the measured deformation of the member may be correlated to a contact between the electrode tip and the object.

[0015] Additional embodiments are described and shown in detail herein. One mechanism to recognize tissue contact in this system is movement or displacement of the electrode relative to a catheter body interface. Upon such occurrence, an output signal can be generated to allow for audible, visual tactile, and/or other user feedback when a desired contact has been achieved between the electrode and the tissue, possibly above a predetermined threshold. This feedback, which may be varied, is provided through loads applied to sensors, including strain and pressure gauges, piezoelectric transducers, microelectromechanical systems (MEMS), optical or laser displacement transducers, linear voltage displacement transducers, microphones, among other devices.

[0016] The foregoing and other aspects, features, details, utilities, and advantages of the present invention will be apparent from reading the following description and claims, and from reviewing the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0017]

Figure 1 is a schematic and block diagram view of a system incorporating an embodiment of a medical device having a contact sensing electrode assembly.

Figure 2 is a cross-sectional view of an embodiment of the electrode assembly of the medical device of Figure 1 configured to use vibration and deflection sensing to sense contact.

Figures 3 and 4 are cross-sectional views of other embodiments of the electrode assembly of the medical device of Figure 1 configured to use deflection

sensing to sense contact.

Figure 5 is a cross-sectional view of another embodiment of the electrode assembly of the medical device of Figure 1 configured to use vibration and deflection sensing to sense contact.

Figures 6-9B are cross-sectional views of other embodiments of the electrode assembly of the medical device of Figure 1 configured to use deflection sensing to sense contact.

Figure 9C is an exemplary layout for transducers in the embodiment of the electrode assembly of the medical device of Figure 9A and 9B for deflection sensing.

Figures 10-11D are cross-sectional views of other embodiments of the electrode assembly of the medical device of Figure 1 configured to use deflection sensing to sense contact.

DETAILED DESCRIPTION

[0018] Referring now to the drawings wherein like reference numerals are used to identify identical components in the various views, Figure 1 generally illustrates a system 10 having a catheter electrode assembly 11 configured to be used in the body for medical procedures. The electrode assembly 11 is included as part of a medical device such as a catheter 19 and may be used for diagnosis, visualization, and/or treatment of tissue 13 (such as cardiac or other tissue) in the body. For example, the electrode assembly 11 may be used for ablation therapy of tissue 13 or mapping purposes in a patient's body 14. Figure 1 further shows various sub-systems included in the overall system 10. The system 10 may include a main computer system 15 (including an electronic control unit 16 and data storage 17, e.g., memory). The computer system 15 may further include conventional interface components, such as various user input/output mechanisms 18a and a display 18b, among other components. Information provided by the electrode assembly 11 may be processed by the computer system 15 and may provide data to the clinician via the input/output mechanisms 18a and/or the display 18b, or in other ways as described herein.

[0019] In the illustrative embodiment, the catheter 19 may include a cable connector or interface 20, a handle 21, a tubular body or shaft 22 having a proximal end 23 and a distal end 24. The catheter 19 may also include other conventional components not illustrated herein such as a temperature sensor, additional electrodes, and corresponding conductors or leads. The connector 20 may provide mechanical, fluid and/or electrical connections for cables 25, 26 extending from a fluid reservoir 12 and a pump 27 and the computer system 15, respectively. The connector 20 may comprise conventional

components known in the art and, as shown, may be disposed at the proximal end of the catheter 19.

[0020] The handle 21 provides a portion for a user to grasp or hold the catheter 19 and may further provide a mechanism for steering or guiding the shaft 22 within the patient's body 14. For example, the handle 21 may include a mechanism configured to change the tension on a pull-wire extending through the catheter 19 to the distal end 24 of the shaft 22 or some other mechanism to steer the shaft 22. The handle 21 may be conventional in the art, and it will be understood that the configuration of the handle 21 may vary. In an embodiment, the handle 21 may be configured to provide visual, auditory, tactile and/or other feedback to a user based on information received from the electrode assembly 11. For example, if contact to tissue 13 is made by the electrode assembly 11, the handle 21 may include light-emitting-diodes, a tone generator, a vibrating mechanical transducer, and/or other indicator(s), the outputs of which could vary in proportion to the signal sensed at the electrode assembly.

[0021] Referring to Figure 2, a cross-sectional view of an embodiment of a distal portion of a catheter 19 having an electrode assembly 11^A is generally illustrated. The electrode assembly 11^A may be connected to the tubular body 22^A of the catheter 19 and located distal from an end of the tubular body 22^A. The tubular body 22^A can be an elongate tubular body, in some examples. The electrode assembly 11^A may comprise an electrode 31^A, a vibration element 32, a deformable member 35^A, and a deflection measuring sensor 33^A.

[0022] The electrode 31^A may include an electrode tip 34^A and an electrode base 36^A, which can form a single, integral component. In some embodiments, the electrode tip 34^A may be configured to contact an object. The object can include, for example, tissue 13 of a patient. In some embodiments, the electrode tip 34^A can be configured to contact a medium. The medium can include, for example, blood of a patient or a saline solution. As used herein, the terms "object" and "medium" are meant to include both items in which the catheter tip may be immersed, as well as items against which the catheter tip may be touched and exert a force.

[0023] The vibration element 32 may be driven by an electrical signal to vibrate the electrode 31^A with a vibration inducing signal to induce vibration of the electrode 31^A. The electrode 31^A can be vibrated by the vibration element 32 at a frequency, for example, a resonant frequency of the electrode tip 34^A, which depends on the mechanical structure of the electrode 31^A. The vibration element 32 can also be configured to vibrate the electrode 31^A at a particular amplitude and/or phase. In an example, the vibration element 32 can be a transducer that converts the electrical signal into mechanical energy (e.g., vibrations).

[0024] When the electrode tip 34^A comes into contact with the object and/or medium, the frequency, amplitude, and/or phase of the resonant vibration of the electrode

tip 34^A may be changed (e.g., dampened). For example, prior to contact occurring between the electrode tip 34^A and the object and/or medium, the electrode assembly 11^A can vibrate at a particular frequency, amplitude, and/or phase. However, upon contact between the electrode tip 34^A and the object and/or medium, energy can be imparted from the electrode tip 34^A to the object in the form of vibrations, thus changing the particular frequency, amplitude and/or phase at which the electrode tip 34^A is vibrating. In addition, as a force between the object and the electrode tip 34^A is increased, more vibrations can be absorbed by the object, thus dampening vibration of the electrode and causing a perturbation. Increasing the force between the object and the electrode tip 34^A can place a larger surface area of the electrode tip 34^A in contact with the object, thus increasing an amount of vibrations that are absorbed by the object.

[0025] The perturbation (e.g., changed frequency, amplitude, phase at which the electrode tip 34^A is vibrating, electrical drive signal) may be sensed either through the electrical drive signal or through a second sensor (not shown) located near the vibrating electrode 31. The second sensor can be configured to monitor the electrode 31^A for a perturbation in the induced vibration of the electrode 31^A. For example, the second sensor can be configured to sense a change in the frequency, amplitude, and/or phase at which the electrode tip 34^A is vibrating at before contact with the object and/or medium and after contact with the object and/or medium. In addition, upon contact of the electrode tip 34^A with the object and/or medium, the electrical drive signal may change. For example, upon contact of the electrode tip 34^A with the object and/or medium, a change in energy used to drive the electrode tip 34^A may occur, as a result of energy being imparted from the electrode tip 34^A to the object and/or medium. As such, the change in energy may be reflected by a change in current and/or voltage used to vibrate the electrode tip 34^A, which can be sensed.

[0026] The frequency, amplitude, and/or phase of vibration of the electrode tip can be dampened by different amounts, depending on what type of object and/or medium the electrode tip 34^A contacts. For example, as discussed herein, when the electrode tip 34^A contacts tissue 13, a particular amount of energy can be imparted to the tissue 13 from the electrode tip 34^A, thus dampening the vibration of the electrode tip 34^A. The amount of energy imparted to the tissue 13, however, can be different than an amount of energy imparted to blood or another type of medium that the electrode tip 34^A contacts in route to a targeted site within the body. For example, a mechanical property (e.g., density) of air is different than a mechanical property of saline solution, which is different than a mechanical property of blood, which is different than a mechanical property of tissue 13. These different mechanical properties can lead to a different change in vibration of the electrode tip 34^A, as the electrode tip 34^A comes into contact with different regions of a patient's vasculature and/or anatomy.

[0027] In some embodiments, when the electrode tip 34^A comes into contact with different types of objects and/or media (e.g., tissue 13, blood, saline solution, air), a change in vibration that occurs when crossing from one type of medium to the next may be reproducible. For example, when the electrode tip 34^A crosses an air-blood interface, blood-tissue interface, or air-tissue interface, for example, the vibration of the electrode tip 34^A may be reduced by a particular amount that is reproducible. Particular devices can be calibrated to factor in what type of interfaces (e.g., air-blood, blood-tissue, air-tissue) that the device will be operating in. As such, if in a particular procedure, the electrode assembly 11^A will be crossing a blood-tissue interface, the electrode assembly 11^A can be calibrated for this and can accurately correlate a dampening of the vibration to contact with the tissue 13. Alternatively, if in a particular procedure, the electrode assembly 11^A will be crossing an air-tissue interface, the electrode assembly 11^A can be appropriately calibrated for this and can accurately correlate a dampening of the vibration to contact with the tissue 13.

[0028] In some embodiments, the vibration element 32 can be configured to maintain the induced vibration after contact between the electrode 31^A and the object and/or medium. For example, the vibration element 32 can be configured to maintain a particular frequency, particular amplitude, and/or particular phase of the vibration inducing signal upon contact between the electrode 31^A and the object and/or medium. The particular frequency, particular amplitude, and/or particular phase can be maintained by varying an electrical drive signal of the vibration element 32. Increasing contact (e.g., magnitude of force) between the electrode 31^A and the object can result in changing (e.g., increasing) the electrical drive signal to maintain a substantially-steady-state vibration of the electrode 31^A. The change to the electrical drive signal can be monitored with a sensor, for example, a current sensor.

[0029] The magnitude of change of the dampened frequency, amplitude, and/or phase of the vibration and/or change in electrical drive signal may be used to determine whether contact has occurred between the electrode tip 34^A and tissue 13. As used herein, contact can be defined as contact between the electrode tip 34^A and tissue 13, a magnitude of force applied between the electrode tip 34^A and tissue 13, and/or a vector of force applied to the electrode tip 34^A as a result of contact between the electrode tip 34^A and tissue 13. For example, in response to the frequency, amplitude, and/or phase changing by a defined amount, a determination that contact has occurred can be made (e.g., yes or no). Alternatively, the magnitude of change of the dampened frequency, amplitude, and/or phase of the vibration and/or the change in the electrical drive signal may be correlated to a magnitude of force applied between the electrode tip 34^A and tissue 13. As described more fully below, the vibration element 32 may be driven at any predetermined frequency, and not necessarily at a resonant frequency,

where vibrations sensed by the second sensor may exhibit discernible differences in responsive vibration characteristics (e.g., frequency, amplitude, and/or phase) upon contact between the electrode 31^A and tissue 13, which can be analyzed to determine contact (e.g., whether contact has occurred, magnitude of force corresponding to contact).

[0030] In an example, as pressure is applied to the handle 21, increasing contact (e.g., magnitude of force) between the electrode tip 34^A and the tissue 13, vibrations produced by the vibration element 32 can be absorbed by the tissue 13. As such, the frequency, amplitude, and/or phase at which the electrode tip 34^A is vibrating, can be reduced. Alternatively, as pressure applied to the handle 21 is decreased, decreasing contact (e.g., magnitude of force) between the electrode tip 34^A and the tissue 13, vibrations can be less absorbed by the tissue 13. Therefore, the frequency, amplitude, and/or phase may be reduced less.

[0031] The electrode tip 34^A may be configured for axial movement M_A and lateral movement M_L relative to the electrode base 36^A. A clearance gap 38 may exist between a portion of the electrode tip 34^A and the electrode base 36^A to accommodate any axial and lateral movements M_A , M_L of the electrode tip 34^A relative to the electrode base 36^A. The electrode base 36^A may be configured to securely connect to a distal end of the tubular body 22 of the catheter 19. A portion of the electrode base 36^A may be inserted into the tubular body 22.

[0032] The electrode tip 34^A may also have a channel 37^A (or a plurality of channels as shown in Figure 5) configured to allow a fluid to flow through or adjacent to the electrode tip 34^A, such as for irrigation purposes. The electrode base 36^A may further include a channel 39 configured to allow a fluid to flow from a lumen in the tubular body 22, through the electrode base 36^A, and to the electrode tip 34^A, and may be used for irrigation purposes. The channel 37^A can line up with the channel 39 to some degree at all lateral movements of the electrode tip 34^A relative to the electrode base 36^A.

[0033] The electrode tip 34^A may be connected to the electrode base 36^A via a spherical joint 40^A. The spherical joint 40^A may comprise a spherical knuckle 41^A located in a pocket 42^A. The pocket 42^A may be substantially cylindrical in shape. In an embodiment, the knuckle 41^A may be a portion of the electrode base 36^A and the pocket 42^A may be a cavity located in the electrode tip 34^A. In another embodiment (as generally illustrated in Figure 3), the knuckle 41^A may be a portion of the electrode tip 34^A and the pocket 42^A may be a cavity located in the electrode base 36^A.

[0034] The vibration element 32 may be configured to vibrate the electrode tip 34^A at a defined frequency, amplitude, and/or phase of vibration. The vibration element 32 may be fixedly or rigidly connected to the electrode tip 34^A, such that vibrations produced by the vibration element 32 are transferred to the electrode tip 34^A via a contact point between the vibration element 32 and the

electrode tip 34^A. In some embodiments, the vibration element 32 may be located in the pocket 42^A. The vibration element 32 may be annular and may be substantially similar in diameter to the pocket 42^A. The vibration element 32 may include an aperture located in the center of the vibration element 32. The aperture may be used to allow fluid to pass through the vibration element 32. The aperture may be substantially the same diameter as the channel 37^A located in the electrode tip 34^A. The vibration element 32 may be located in the pocket in the electrode tip 34^A, at a distal position relative to the knuckle 41^A. Alternatively, the vibration element 32 may be located in the pocket 42^A in the electrode base 36^A, at a proximal position relative to the knuckle 41^A (as generally illustrated in Figure 3). While a detailed embodiment of a vibration element is provided, it will be appreciated that this disclosure is not limited to the illustrated embodiments. Rather, other types and forms of vibration inducing transducers, including those known to those with skill in the art, may be used.

[0035] In embodiments, the second sensor may be configured to measure the frequency, amplitude, and/or phase of the vibration of the electrode tip 34^A. When the electrode tip 34^A is not in contact with tissue 13, the second sensor may detect a frequency, amplitude, and/or phase substantially equal to a frequency (which may be predefined or predetermined), amplitude, and/or phase imparted to the electrode tip 34^A by the vibration element 32. When the electrode tip 34^A is in contact with tissue 13, the second sensor may detect changes in frequency, amplitude, and/or phase. The changes might be positive or negative depending on the specific design of the resonating structure, but the magnitude of the change will be proportional to a magnitude of force applied between the electrode tip 34^A and tissue 13.

[0036] In some examples, the second sensor can be annular in shape. The second sensor can be located on the electrode tip 34^A; located distally with respect to the spherical knuckle 41^A in a pocket of the electrode tip 34^A; or located proximally with respect to the spherical knuckle 41^B in the pocket of the electrode base 36^B, as shown in Figure 3.

[0037] In an embodiment, the system 10 may be programmed to determine whether contact between the electrode tip 34^A and tissue 13 has occurred. For example, a determination that contact has occurred between the electrode tip 34^A and the tissue 13 can be made in response to a differential between a first and second frequency, amplitude, and/or phase of vibration being exceeded. The first frequency, amplitude, and/or phase of vibration can be a frequency, amplitude, and/or phase that exists when the electrode tip 34^A is not in contact with tissue 13 and the second frequency, amplitude, and/or phase of vibration can be a frequency, amplitude, and/or phase that exists when the electrode tip 34^A is in contact with tissue 13. In some embodiments, the first and second frequency, amplitude, and/or phase can be correlated with a first and second magnitude of force ap-

plied between the electrode tip 34^A and tissue 13.

[0038] This allows the system 10 to be adjustable for determining the amount of force between the electrode tip 34^A and tissue 13 that must occur before the system acknowledges that contact with tissue 13 has occurred. For example, if the differential between the first and second frequency, amplitude, and/or phase of vibration is set high, then the magnitude of force applied between the electrode tip 34^A and tissue 13e to sufficiently determine that contact has been made may be high in magnitude. Additionally, if the differential between the first and second frequency, amplitude, and/or phase of vibration is set low, then the amount of contact force to sufficiently determine that contact has been made may be low in magnitude.

[0039] In some embodiments, the electrode assembly 11^A can include a deformable member 35^A and a deflection measuring sensor 33^A, as further discussed in relation to Figure 3. The deformable member 35^A and the deflection measuring sensor 33^A can be configured to measure a lateral displacement M_L (e.g., angular) and axial displacement M_A of the electrode tip 34^A relative to the electrode base 36^A.

[0040] The deflection measuring sensor 33^A and/or the deformable member 35^A may be annular in shape and may be provided in the pocket 42^A in the electrode tip 34^A. The deflection measuring sensor 33^A and/or the deformable member 35^A may be provided at a position distal to the knuckle 41^A. In another embodiment (as generally illustrated in Figure 3), the deflection measuring sensor 33^A and/or the deformable member 35^A may be located proximal to the knuckle 41 in the pocket 42^B in the electrode base 36^B. In yet another embodiment, the deflection measuring sensor 33^A may be a piezoelectric transducer.

[0041] In some embodiments, the deflection measuring sensor 33^A and/or the second sensor may send a signal to the handle 21 and/or control unit 16, upon determining that contact has been made between the electrode tip 34^A and the tissue 13, or when the magnitude of force applied between the electrode tip 34^A and tissue 13 is greater than a defined amount. The signal to the handle 21 may be used to provide a required amount of haptic or visual feedback via the handle 21 (which may have been configured as previously described). The signal to the control unit 16 may be used to provide information to the user, such as through the various input/output devices 18a or the display 18b of the system 10.

[0042] As generally shown in Figure 3, an embodiment of an electrode assembly 11^B may also be configured to measure lateral displacement M_L (e.g., angular) and axial displacement M_A of the electrode tip 34^B relative to an electrode base 36^B. The magnitude of the displacements M_L , M_A may be used to determine contact between the electrode tip 34^B and tissue 13, a magnitude of force applied between the electrode tip 34^B and tissue 13, and/or a vector of force applied to the electrode tip 34^B as a result of contact between the electrode tip 34^B and

tissue 13. In an embodiment, the electrode assembly 11^B may comprise the electrode 31^B having the electrode tip 34^B and the electrode base 36^B, a deformable member 35^B, and a deflection measuring sensor 33^A.

[0043] The deformable member 35^B is configured to deform when a force is applied between the electrode tip 34^B and tissue 13. The deformable member 35^B may be located adjacent to a flat portion of the knuckle 42^B. As the electrode tip 34^B makes contact with tissue 13, the electrode tip 34^B will move relative to the electrode base 36^B. Depending on the angle at which the electrode tip 34^B contacts the tissue 13, the electrode tip 34^B may move either axially M_A and/or laterally M_L relative to the electrode base 36^B. When the electrode tip 34^B moves axially M_A and/or laterally M_L by pivoting about the spherical joint 40^B, the deformable member 35^B may be squeezed against the flat portion of the knuckle 41^B and a rigid surface, such as a wall 45 of the electrode base 36^B (as shown in Figure 3) or a surface of the vibration element 32 (as shown in Figure 2). In some embodiments, the deformable member 35^B can expand radially outward. When the electrode tip 34^B is no longer in contact with tissue 13, the deformable member 35^B can elastically return to its initial form. The deformable member 35^B may be annular in shape and may have an aperture located at the center of the deformable member 35^B which may allow fluid to pass through the deformable member 35^B. The deformable member 35^B may be provided or positioned in the pocket 42^B of the electrode tip 34^B between the knuckle 41^B and the electrode base 36^B.

[0044] In another embodiment, shown in Figure 3, the deformable member 35^B may be provided or positioned in the pocket 42^B of the electrode base 42^B between the knuckle 41^B and the wall 45 of the electrode base 36^B. The amount of force necessary to deform the deformable member 35^B may be set or determined based on a selection of a material used for the deformable member 35^B. For example, as the selected material of the deformable member 35^B becomes stiffer and more difficult to deform, the amount of force necessary to deflect the electrode tip 34^B may also increase. This may be useful, for example, in setting or determining the range of forces to be measured. In embodiments, the deformable member 35^B may comprise silicon, rubber, or other natural and manmade elastomeric materials. A wide variety of other elastically deformable materials may be used as known to those with skill in the art.

[0045] The deflection measuring sensor 33^B may be configured to measure the deformation of the member 35^B. As the deformable member deforms (e.g., expands radially), the deflection measuring sensor 33^B may detect the deformation of the deformable member 35^B. The deflection measuring sensor 33^B may be located on the deformable member 35^B and may be coaxial with the deformable member 35^B and surround the deformable member 35^B. The deflection measuring sensor 33^B may be annular in shape. In an embodiment, the deflection

measuring sensor 33^B may be a piezoelectric transducer configured for measuring strain. The magnitude of deformation of the deformable member 35^B detected by the deflection measuring sensor 33^B may correlate to a vector of force applied to the electrode tip 34^B as a result of contact between the electrode tip 34^B and tissue 13. The deflection measuring sensor 33^B may send a signal to the handle 21 and/or the control unit 16. The signal to the handle 21 may be used to provide a set or required amount of haptic or visual feedback for which the handle 21 may be configured to produce. The signal to the control unit 16 may be used to provide information to a user, such as through the various input/output devices 18a or the display 18b of the system 10.

[0046] The deformable member 35^C may have various shapes. For example, as generally illustrated in Figure 4, the deformable member 35^C may be a beam that is generally linear shaped, such as substantially cylindrical shaped or substantially rectangular shaped. The deformable member 35^C may be provided or positioned distally of the knuckle 41^C and provided or positioned in the pocket 42^C. One end of the deformable member 35^C may be connected to the knuckle 41^C and the opposing end of the member may be connected to the electrode tip 34^C. The deformable member 35^C can be longitudinally arranged along a longitudinal centerline of the catheter 19, extending from a distal end of the knuckle 41^C to a distal end of the pocket 42^C. The electrode tip 34^C can be deflected axially M_A or laterally M_L , causing deformation of the deformable member 35^C. The deflection measuring sensor 33^C, provided or positioned on deformable member 35^C may measure the deformation of the deformable member 35^C.

[0047] In an embodiment, and as generally illustrated in Figure 5, an electrode assembly 11^D may comprise an electrode 31^D having an electrode tip 34^D and an electrode base 36^D, a deformable member 35^D, a deflection measuring sensor 33^D, a vibration element 32^D and a vibration measuring sensor 49.

[0048] The electrode assembly 11^D may be configured to determine contact between the electrode tip 34^D and tissue 13, a magnitude of force applied between the electrode tip 34^D and tissue 13, and/or a vector of force applied to the electrode tip 34^D as a result of contact between the electrode tip 34^D and tissue 13 by both vibration dampening sensing of the electrode tip 34^D and strain deflection measurements of the deformable member 35^D, such as generally described with reference to Figures 2 and 3. By using both vibration dampening sensing of the electrode tip 34^D and strain deflection measurements of the deformable member 35^D, the accuracy and/or range of measurements associated with determining contact between the electrode tip 34^D and tissue 13, magnitude of force applied between the electrode tip 34^D and tissue 13, and/or the vector of force applied between the electrode tip 34^D and tissue 13 may be increased. For example, the vibration measuring sensor 49 may be configured to measure small magnitudes of

force applied between the electrode tip 34^D and tissue 13, while the deflection measuring sensor 33^D may be configured to measure larger magnitudes of force applied between the electrode tip 34^D and tissue 13. The vibration measuring sensor 49 may be provided or positioned directly on the electrode tip 34^D. The deflection measuring sensor 33^D may be located directly on the deformable member 35^D.

[0049] In yet another embodiment illustrated in Figure 6, an electrode assembly 11^E may comprise electrode 31^E having an electrode tip 34^E and an electrode base 36^E. The electrode assembly 11^E may further comprise a spherical joint 53, a beam 54 positioned distally of the spherical joint 53, one or more strain gauges 55 and a cavity 56. As shown, one end of the beam 54 may be connected to the spherical joint 53 and the other end of the beam 54 may be connected to the electrode 31^E at or near the electrode tip 34^E.

[0050] The electrode assembly 11^E may be configured to measure contact between the electrode tip 34^E and tissue 13, a magnitude of force applied between the electrode tip 34^E and tissue 13, and/or a vector of force applied to the electrode tip 34^E as a result of contact between the electrode tip 34 and tissue 13 since any applied force on the electrode tip 34^E causes deflection in the beam 54, which generates feedback through the one or more strain gauges 55. Based on this embodiment, a determination can be made whether the force applied between the electrode tip 34^E and the tissue 13 is an axial force or a lateral force. Further, the one or more strain gauges 55 may be replaced with piezoelectric transducers, or other sensors to determine the contact between the electrode tip 34^E and tissue 13, the magnitude of force applied between the electrode tip 34^E and tissue 13, and/or the vector of force applied to the electrode tip 34^E as a result of contact between the electrode tip 34^E and tissue 13.

[0051] In yet another embodiment illustrated in Figure 7, an electrode assembly 11^F may comprise electrode 31^F having an electrode tip 34^F, an electrode base 36^F, a standoff 58, a first piezoelectric transducer 59, a second piezoelectric transducer 60, a seal 61, and a cavity 62. The electrode tip 34^F can move laterally with respect to the electrode base 36^F at a center of rotation 63. The electrode 31^F is connected to the electrode base 36^F at the standoff 58 and the seal 61, such that when a force is applied to the electrode tip 34^F, either an axial force or a lateral force, the standoff impinges on the first piezoelectric transducer 59.

[0052] In operation, the second piezoelectric transducer 60 is electrically driven at a known frequency and the first piezoelectric transducer 59 is set up to recognize the output of the second piezoelectric transducer 60. When the electrode tip 34^F is in contact with the tissue 13, the response output of the first piezoelectric transducer 59 will change with the applied load or tone of the tissue as a lesion is developed. The output of the first piezoelectric transducer 59 may be used to provide a signal for audible,

visual, tactile, and/or other feedback to the user as described above. In some embodiments, the first piezoelectric transducer 59 can be configured to recognize an output of the second piezoelectric transducer 60. The output recognized by the first piezoelectric transducer 59 can be correlated to the magnitude of the contact force applied to the electrode tip 34^F. Further, the second piezoelectric transducer 60 may be optional and the first piezoelectric transducer 59 may be replaced with a strain gauge.

[0053] In yet another embodiment, illustrated in Figure 8, an electrode assembly 11^G may comprise electrode 31^G having an electrode tip 34^G, and an electrode base 36^G, a seal 65, a fluid or gel 66, a strain gauge 67, and a cavity 68. The space between the electrode tip 34^G and the electrode base 36^G is filled with the fluid 66, which is retained in the cavity 68 by the seal 65. The fluid 66 has significant electrical resistance or impedance such that the closer the electrode tip 34^G comes to the electrode base 36^G, the lower the resistance. Depending on where contact occurs between the electrode tip 34^G and the tissue 13, a distance between the electrode tip 34^G and the electrode base 36^G can decrease, thus reducing the amount of fluid 66 and electrical resistance or impedance between a particular point of the electrode tip 34^G and the base. A number of sensors (e.g., current sensors) can be placed on the electrode base 36^G, which can detect changes in current resultant from the varying distance between the electrode tip 34^G and the electrode base 36^G. The detected changes in current can be correlated with measurements of contact between the electrode tip 34^G and tissue 13, a magnitude of force applied between the electrode tip 34^G and tissue 13, and/or a vector of force applied to the electrode tip 34^G. As discussed herein, the measurement can be based on capacitance and/or impedance associated with the fluid 66.

[0054] Further, the strain gauge 67 may measure the force on the electrode base 36^G (or on the electrode tip 34^G) as the distance or thickness of space between the electrode tip 34^G and the electrode base 36^G changes. A number of strain gauges 67 can be placed on the electrode base 36^G in the cavity 68. In an example, as force is applied to the electrode tip 34^G, a pressure in the cavity 68 can increase and can be registered by one of the number of strain gauges 67 and correlated with a magnitude of force and/or a vector of force applied to the electrode tip 34^G. Depending on where the force is applied to the electrode tip 34^G, one strain gauge 67 may register a greater pressure increase than another, providing for omni-directional measurement of force on the electrode tip 34^G.

[0055] As described above, when the electrode tip 34^G is in contact with the tissue 13, the response output will change with the applied load or tone of the tissue as a lesion is developed. As with the embodiments described herein, the principles can be used for measuring changes in tissue tone as a means for assessing lesion development. Given that the mechanical characteristics of the

tissue changes during and following RF ablation, the described embodiments could also be used to monitor the extent (e.g., size) of a lesion by recognizing changes in the feedback thru the transducers, strain gauges, or the like.

[0056] In yet another embodiment illustrated in Figure 9A, an electrode assembly 11^H may comprise electrode 31^H having an electrode tip 34^H and an electrode base 36^H. Similar to the embodiments shown in Figures 3 and 5, a knuckle 72 is incorporated along with a gap 73^A between the electrode tip 34^H and the electrode base 36^H. As further shown in Figure 9B, a strain gauge 74 is located in the gap 73^B between the electrode tip 34^I and the electrode base 36^I. Lateral movement of the electrode tip 34^I relative to the base 36^I can change a size of the gap 73^B, which can be registered by the strain gauge 74. In some embodiments, multiple strain gauges 74 can be located in the gap 73^B in a radial configuration. For example, strain gauges 74 can be located in one of three places, each 120° from each other, as shown in the layout in Figure 9C. Other configurations using more or fewer than three transducers may be utilized with similar results. As described herein, the strain gauges 74 may be replaced with piezoelectric transducers, or various other types of sensors MEMS, LVDT, optical, laser, etc., configured to measure an increase or decrease in a size of the gap 73^B. Upon contact between the electrode tip 34^H and the tissue 13, the strain gauges 74 (or transducers) will provide a signal for audible, visual, tactile and/or other feedback to the user as described above.

[0057] In yet another embodiment illustrated in Figure 10, an electrode assembly 11^J may comprise electrode 31^J having an electrode tip 34^J, and an electrode base 36^J. The electrode tip 34^J can have a first diameter and can be connected to a beam 81 of a second diameter at a proximal end of the electrode tip 34^J. The electrode base 36^J includes an opening of a varying diameter passing from a proximal end to a distal end of the electrode base 36^J. The diameter of the opening at the distal end of the electrode base 34^J can be smaller than the first diameter of the electrode tip 34^J and larger than the second diameter of the beam 81. The beam 81 can be inserted into the opening of the distal end of the electrode base 36^J.

[0058] The electrode assembly 11^J further comprises a transducer 78, which can be annular in shape, a compliant or deformable member 79, and a tensioned assembly 80. The tensioned assembly may be made up of the beam 81, similar to the beam in Figure 6 and a band 82 stretched between the beam 81 and an end piece 83. The transducer 78 may be of any type of transducer that can sense a change in tension in the band 82, such as a strain gauge, piezoelectric, MEMS, LVDT, optical, laser, etc. Upon contact between the electrode tip 34^J (or the electrode 31^J) and the tissue 13, the deformable member 79 can deform causing the tensioned assembly 80 to increase or decrease the amount of tension on the band 82. The transducer 78 will sense the change in ten-

sion and provide an output signal 84 for audible, visual, tactile and/or other feedback to the user as described above. For example, an increase or decrease in the amount of tension on the band 82 can pull the end piece 83 towards a distal end of the electrode tip 34^J, causing the end piece 82 to exert an increase or decrease in amount of force applied to the transducer 78. The transducer 78 can sense the increase or decrease in the amount of force applied on the transducer 78 and/or can sense the change in tension in the band 82, which can be used to determine contact between the electrode tip 34^J and tissue 13, a magnitude of force applied between the electrode tip 34^J and tissue 13, and/or a vector of force applied to the electrode tip 34^J.

[0059] In yet another embodiment illustrated in Figure 11A, an electrode assembly 11^K may comprise electrode 31^K having an electrode tip 34^K of a first diameter, and an electrode shaft 88 of a second diameter. Electrode assembly 11^K may further comprise a compliant or soft material 89, such as silicone, a piezoelectric receiver transducer 90^A, and a piezoelectric transmitter transducer 91^A. The electrode shaft 88 can be connected to the electrode tip 34^K. In addition, the piezoelectric receiver transducer 90^A can be attached to a proximal end of the electrode shaft 88. The electrode shaft 88 and the piezoelectric receiver transducer 90^A can be inserted into an opening at a distal end of an electrode base 94. In an example, the diameter of the opening at the distal end of the electrode base 94 can be smaller than the first diameter of the electrode tip 34^K and larger than the second diameter of the electrode shaft 88.

[0060] An application of force to the electrode tip 34^K can move the electrode tip 34^K, the electrode shaft 88, and the piezoelectric receiver transducer 90^A proximally towards the piezoelectric transmitter transducer 91^A, such that the transducers contact one another, creating a signal which can be correlated with the application of force to the electrode tip 34^K.

[0061] The piezoelectric receiver transducer 90^B and piezoelectric transmitter transducer 91^B are represented schematically in Figure 11B along with the connections for the signal into the transmitter 92 and the signal out from the receiver 93. Additional embodiments are shown in Figure 11C (indicating a pressure amplification due to a small contact area) and Figure 11D (alternative transducer arrangements). For example, as the piezoelectric receiver transducer 90^C moves towards and contacts the piezoelectric transmitter transducer 91^C, the piezoelectric receiver transducer 90^C can contact the piezoelectric transmitter transducer 91^C with a reduced contact area, leading to a pressure amplification between the point of the piezoelectric receiver transducer 90^C and the piezoelectric transmitter transducer 91^C. The pressure amplification between the piezoelectric receiver transducer 90^C and the piezoelectric transmitter transducer 91^C can provide an increase in sensitivity. In some embodiments, the piezoelectric receiver transducer 90^D can have a female contact face and the piezoelectric transmitter trans-

ducer 91^D can have a male contact face. Alternatively, the piezoelectric receiver transducer 90^E can have a female contact face and the piezoelectric transmitter transducer 91^E can have a male contact face. In an example, the alternative transducer configurations in Figure 11D can provide for a different sensitivities. As also described herein, the piezoelectric transducers 90^A, 91^A may be replaced with strain gauges, MEMS microphones, LVDT, optical, laser, etc. Upon contact between the electrode tip 34^K and the tissue 13, the electrode shaft 88 will move accordingly, such movement will be picked-up by the transducers, which will generate a signal as described above.

[0062] In yet another embodiment illustrated in Figure 12, an electrode assembly 11^L can include an electrode 31^L having an electrode tip 34^L, an electrode base 96, a beam 98, swivel joint 99, and strain gauges 97. The electrode 31^L can be connected to the beam 98 at a proximal end of the electrode 31^L. The beam 98 can extend through a portion of a length of the electrode base 96. In some embodiments, the electrode base 98 can be cylindrical and can have tapered inner walls, such that a distal opening of the electrode base 96 is substantially the same size as the beam 98 and a proximal opening of the electrode base 96 is larger than the distal opening. This can allow for movement of the beam 98 when deflection of the electrode tip 34^L occurs. The electrode base 96 can be in contact with the electrode 31^L via a swivel joint 99. Movement of the beam 98 can be detected by strain gauges 97 in contact with the beam 98 and the electrode base 96. For example, lateral movement of the electrode tip 34^L caused by contact with tissue 13 can also cause movement of the beam 98, which can be detected by sensors 97. An output of the sensors 97 can be used to determine contact between the electrode tip 34^L and tissue 101, a magnitude of force applied between the electrode tip 34^L and tissue 101, and/or a vector of force applied to the electrode tip 34^L.

[0063] As discussed herein, the amount of energy imparted to the tissue 101 can be different than an amount of energy imparted to medium 100 (e.g., blood) that the electrode tip 34^L contacts in route to a targeted site within the body. In an example, the electrode tip 34^L can penetrate medium 100 to contact tissue 101. Mechanical properties of the tissue 101 and medium 100 can lead to a different change in vibration of the electrode tip 34^L, as the electrode tip 34^L comes into contact with different regions of a patient's vasculature. Accordingly, the electrode assembly 11^L can be calibrated to account for different types of media that the electrode tip 34^L will contact, as discussed in relation to Figure 2.

[0064] The scope of the invention is defined by attached independent claim 1. Preferred embodiments are given in the dependent claims. It will be appreciated that the terms "proximal" and "distal" may be used throughout the specification with reference to a clinician manipulating one end of a medical device or instrument used to treat a patient. The term "proximal" refers to the portion

of the device closest to the clinician and the term "distal" refers to the portion located furthest from the clinician. It will be further appreciated that for conciseness and clarity, spatial terms such as "vertical," "horizontal," "up," and "down" may be used herein with respect to the illustrated embodiments. However, medical devices may be used in many orientations and positions, and these terms are not intended to be limiting or absolute.

[0065] Although only certain embodiments have been described above with a certain degree of particularity, those skilled in the art could make numerous alterations to the disclosed embodiments without departing from the scope of this disclosure. Joinder references (e.g., attached, coupled, connected, and the like) are to be construed broadly and may include intermediate members between a connection of elements and relative movement between elements. As such, joinder references do not necessarily infer that two elements are directly connected/coupled and in fixed relation to each other. Additionally, the terms "electrically connected" and "in communication" are meant to be construed broadly to encompass both wired and wireless connections and communications. It is intended that all matter contained in the above description or shown in the accompanying drawings shall be interpreted as illustrative only and not limiting. Changes in detail or structure may be made without departing from the invention as defined in the appended claims.

Claims

1. A sensing assembly (11) for sensing contact with an object, the assembly (11) comprising the following:
 - an elongate tubular body (22);
 - an electrode (31) connected to the elongate tubular body;
 - a vibration element (32) operatively connected with the electrode (31) and configured to deliver a vibration-inducing signal to induce vibration of the electrode (31); and
 - a sensor configured to monitor the electrode (31) for a perturbation in the induced vibration, wherein the perturbation results from contact between the electrode (31) and the object, **characterised in that** the electrode (31) includes an electrode tip (34) for contacting the object, and the vibration-inducing signal is selected to vibrate the electrode (31) at a resonant frequency of the electrode tip (34), which depends on the mechanical structure of the electrode (31).
2. The sensing assembly of claim 1, wherein the electrode includes an electrode base (36) connected to the elongate tubular body (22) and an electrode tip (34) connected to the electrode base (36).

3. The sensing assembly of claim 2, wherein the vibration element (32) is located in a pocket of the electrode tip (34).
4. The sensing assembly of any one of claims 1 to 3 further configured to correlate the monitored perturbation to a force applied to the electrode (31).
5. The sensing assembly of any one of claims 1 to 4, wherein the vibration element (32) is configured to maintain at least one of the particular frequency, the particular amplitude, and the particular phase of the vibration inducing signal upon contact between the electrode (31) and the object.
6. The sensing assembly of claim 5, wherein the perturbation includes a change in the electrical drive signal of the vibration element (32).
7. The sensing assembly of claim 6, wherein the perturbation corresponding to the vibration-inducing signal is determined based on the change in the electrical drive signal of the vibration element (32).
8. The sensing assembly according to claim 1, wherein the elongate tubular body (22) comprises a distal end; the electrode (31) comprising (a) an electrode base (36) connected to the distal end of the elongate tubular body (22) and (b) an electrode tip (34) connected to the electrode base; the vibration element (32) is operatively connected to the electrode tip (34) and configured to deliver the vibration-inducing drive signal to induce vibration of the electrode tip (34), wherein the vibration element (32) is configured to maintain the induced vibration after contact between the electrode (31) and tissue (13); and the sensor is configured to monitor a change in the drive signal of the vibration element (32), wherein contact between the electrode (31) and tissue (13) causes a change in the drive signal.
9. The sensing assembly of claim 8, wherein the induced vibration of the tip is a substantially-steady-state vibration.
10. The sensing assembly of claim 8, wherein the electrode (31) further comprises at least one channel configured for fluid delivery.
11. The sensing assembly of claim 8, wherein the change in the electrical drive signal is correlated with a magnitude of force applied between the electrode (31) and tissue (13).
12. The sensing assembly of claim 11, further comprising a handle (21) configured to provide feedback based on the magnitude of force applied between the electrode (31) and tissue (13).
13. The sensing assembly of claim 8, wherein the electrode base (36) and the electrode tip (34) comprise a single, integral component.
14. The sensing assembly according to claim 1, wherein the electrode (31) comprises an electrode tip (34) connected to an electrode base via a spherical joint configured to allow relative movement between the electrode tip (34) and the electrode base (36); the vibration element (32) operatively connected to a vibrating tip component comprising at least one of (a) the electrode tip (34) and (b) the electrode base (36), the vibration element (32) being thereby configured to deliver the vibration-inducing signal to the vibrating tip component; and a perceptible output system configured to provide perceptible output in response to the monitored perturbation in the induced vibration, wherein the perceptible output is selected from the group consisting of an audible output, a visual output, and a tactile output.
15. The sensing assembly of claim 14, further comprising a deformable member in contact with the electrode base (36) and the electrode tip (34) and configured to deform in response to the relative movement between the electrode tip (34) and the electrode base (36).
16. The sensing assembly of claim 15, further comprising a deflection measuring sensor in contact with the deformable member and configured to measure a deflection of the deformable member.
17. The sensing assembly of claim 14, wherein a clearance gap exists between at least a portion of the electrode tip (34) and the electrode base (36), the gap being configured to accommodate at least one of axial and lateral movement of the electrode tip (34) relative to the electrode base (36).
18. The sensing assembly of claim 14, wherein the sensor is located on the electrode tip (34).

Patentansprüche

1. Erfassungsanordnung (11) zum Erfassen eines Kontakts mit einem Objekt, wobei die Anordnung (11) folgendes aufweist:
- einen länglichen Röhrenkörper (22);
eine Elektrode (31), die mit dem länglichen Röhrenkörper verbunden ist;
ein Vibrationselement (32), das operativ mit der

- Elektrode (31) verbunden und konfiguriert ist zum Liefern eines vibrationsinduzierten Signals, um Vibration der Elektrode (31) zu induzieren; und
einen Sensor, der konfiguriert ist zum Überwachen der Elektrode (31) hinsichtlich einer Störung in der induzierten Vibration, wobei die Störung von dem Kontakt zwischen der Elektrode (31) und dem Objekt her resultiert, **dadurch gekennzeichnet, dass** die Elektrode (31) eine Elektrodenspitze (34) zum Kontaktieren des Objekts aufweist, und
das vibrationsinduzierte Signal ausgewählt ist, damit die Elektrode (31) bei einer Resonanzfrequenz der Elektrodenspitze (34) vibriert, die von einer mechanischen Struktur der Elektrode (31) abhängig ist.
2. Erfassungsanordnung nach Anspruch 1, bei der die Elektrode eine Elektrodenbasis (36) aufweist, die mit dem länglichen Röhrenkörper (22) verbunden ist, und eine Elektrodenspitze (34), die mit der Elektrodenbasis (36) verbunden ist.
 3. Erfassungsanordnung nach Anspruch 2, bei der das Vibrationselement (32) sich in einer Aussparung der Elektrodenspitze (34) befindet.
 4. Erfassungsanordnung nach einem der Ansprüche 1 bis 3, die ferner konfiguriert ist zum Korrelieren der überwachten Störung mit einer an die Elektrode (31) angelegten Kraft.
 5. Erfassungsanordnung nach einem der Ansprüche 1 bis 4, bei der das Vibrationselement (32) konfiguriert ist, um mindestens eine von der bestimmten Frequenz, der bestimmten Amplitude und der bestimmten Phase des vibrationsinduzierten Signals bei Kontakt zwischen der Elektrode (31) und dem Objekt aufrechtzuerhalten.
 6. Erfassungsanordnung nach Anspruch 5, bei der die Störung eine Änderung in dem elektrischen Antriebssignal des Vibrationselements (32) aufweist.
 7. Erfassungsanordnung nach Anspruch 6, bei der die Störung, die dem vibrationsinduzierten Signal entspricht, bestimmt wird basierend auf einer Änderung des elektrischen Antriebssignals des Vibrationselements (32).
 8. Erfassungsanordnung nach Anspruch 1, bei der der längliche Röhrenkörper (22) ein distales Ende aufweist;
die Elektrode (31) (a) eine Elektrodenbasis (36), die mit dem distalen Ende des länglichen Röhrenkörpers (22) verbunden ist, und (b) eine Elektrodenspitze (34), die mit der Elektrodenbasis verbunden ist,
aufweist;
das Vibrationselement (32) operativ mit der Elektrodenspitze (34) verbunden und konfiguriert ist zum Liefern des vibrationsinduzierten Antriebssignals, um eine Vibration der Elektrodenspitze (34) zu induzieren, wobei das Vibrationselement (32) konfiguriert ist zum Aufrechterhalten der induzierten Vibration nach einem Kontakt zwischen der Elektrode (31) und dem Gewebe (13); und
der Sensor konfiguriert ist zum Überwachen einer Änderung des Antriebssignals des Vibrationselements (32), wobei ein Kontakt zwischen der Elektrode (31) und dem Gewebe (13) eine Änderung des Antriebssignals verursacht.
 9. Erfassungsanordnung nach Anspruch 8, bei der die induzierte Vibration der Spitze eine im Wesentlichen stabile Vibration ist.
 10. Erfassungsanordnung nach Anspruch 8, bei der die Elektrode (31) ferner mindestens einen Kanal aufweist, der zur Fluidlieferung konfiguriert ist.
 11. Erfassungsanordnung nach Anspruch 8, bei der die Änderung des elektrischen Antriebssignals mit einer Größe einer Kraft korreliert, die zwischen der Elektrode (31) und dem Gewebe (13) anliegt.
 12. Erfassungsanordnung nach Anspruch 11, ferner mit einem Griff (21), der konfiguriert ist zum Bereitstellen einer Rückmeldung basierend auf der Größe der Kraft, die zwischen der Elektrode (31) und dem Gewebe (13) wirkt.
 13. Erfassungsanordnung nach Anspruch 8, bei der die Elektrodenbasis (36) und die Elektrodenspitze (34) eine einzelne, integrale Komponente aufweisen.
 14. Erfassungsanordnung nach Anspruch 1, bei der die Elektrode (31) eine Elektrodenspitze (34) aufweist, die mit einer Elektrodenbasis verbunden ist über eine kugelförmige Verbindung, die konfiguriert ist, damit eine relative Bewegung zwischen der Elektrodenspitze (34) und der Elektrodenbasis (36) möglich ist;
das Vibrationselement (32) operativ mit einer Vibrationsspitzenkomponente operativ verbunden ist, die mindestens (a) die Elektrodenspitze (34) und (b) die Elektrodenbasis (36) aufweist, wobei das Vibrationselement (32) dadurch konfiguriert wird zum Liefern des vibrationsinduzierten Signals an die Vibrationsspitzenkomponente; und
ein Wahrnehmungsausgabesystem konfiguriert ist zum Bereitstellen der Wahrnehmungsausgabe in Antwort auf die überwachte Störung in der induzierten Vibration, wobei die Wahrnehmungsausgabe ausgewählt ist aus der Gruppe, die eine Audioausgabe, visuelle Ausgabe und eine taktile Ausgabe

aufweist.

15. Erfassungsanordnung nach Anspruch 14, ferner mit einem verformbaren Bauteil, das in Kontakt mit der Elektrodenbasis (36) und der Elektrodenspitze (34) und konfiguriert ist, um in Antwort auf die relative Bewegung zwischen der Elektrodenspitze (34) und der Elektrodenbasis (36) sich zu verformen.
16. Erfassungsanordnung nach Anspruch 15, ferner mit einem Abweichungsmesssensor, der in Kontakt ist mit dem verformbaren Bauteil und konfiguriert ist zum Messen einer Verformung des verformbaren Bauteils.
17. Erfassungsanordnung nach Anspruch 14, bei der ein Spalt existiert zwischen mindestens einem Bereich der Elektrodenspitze (34) und der Elektrodenbasis (36), wobei der Spalt konfiguriert ist zum Aufnehmen von mindestens einer axialen und lateralen Bewegung der Elektrodenspitze (34) relativ zu der Elektrodenbasis (36).
18. Erfassungsanordnung nach Anspruch 14, bei der der Sensor sich auf der Elektrodenspitze (34) befindet.

Revendications

1. Ensemble de détection (11) pour détecter un contact avec un objet, l'ensemble (11) comprenant les éléments suivantes :
- un corps tubulaire allongé (22) ;
 - une électrode (31) connectée au corps tubulaire allongé ;
 - un élément de vibration (32) connecté opérationnellement à l'électrode (31) et configuré pour délivrer un signal induisant une vibration pour induire une vibration de l'électrode (31) ; et
 - un capteur configuré pour surveiller l'électrode (31) quant à une perturbation dans la vibration induite, dans lequel la perturbation résulte d'un contact entre l'électrode (31) et l'objet,
- caractérisé en ce que** l'électrode (31) inclut un embout d'électrode (34) pour venir en contact avec l'objet, et le signal induisant une vibration est sélectionné pour faire vibrer l'électrode (31) à une fréquence de résonance de l'embout d'électrode (34), qui dépend de la structure mécanique de l'électrode (31).
2. Ensemble de détection selon la revendication 1, dans lequel l'électrode inclut une base d'électrode (36) connectée au corps tubulaire allongé (22) et un embout d'électrode (34) connecté à la base d'électrode (36).
3. Ensemble de détection selon la revendication 2, dans lequel l'élément de vibration (32) est situé dans une poche de l'embout d'électrode (34).
4. Ensemble de détection selon l'une quelconque des revendications 1 à 3, configuré en outre pour corrélérer la perturbation surveillée à une force appliquée à l'électrode (31).
5. Ensemble de détection selon l'une quelconque des revendications 1 à 4, dans lequel l'élément de vibration (32) est configuré pour maintenir au moins l'une parmi la fréquence particulière, l'amplitude particulière, et la phase particulière du signal induisant une vibration lors d'un contact entre l'électrode (31) et l'objet.
6. Ensemble de détection selon la revendication 5, dans lequel la perturbation inclut un changement dans le signal d'attaque électrique de l'élément de vibration (32) .
7. Ensemble de détection selon la revendication 6, dans lequel la perturbation correspondant au signal induisant une vibration est déterminée en se basant sur le changement dans le signal d'attaque électrique de l'élément de vibration (32).
8. Ensemble de détection selon la revendication 1, dans lequel le corps tubulaire allongé (22) comprend une extrémité distale ; l'électrode (31) comprenant (a) une base d'électrode (36) connectée à l'extrémité distale du corps tubulaire allongé (22) et (b) un embout d'électrode (34) connecté à la base d'électrode ; l'élément de vibration (32) est connecté opérationnellement à l'embout d'électrode (34) et configuré pour délivrer le signal d'attaque induisant une vibration pour induire une vibration de l'embout d'électrode (34), dans lequel l'élément de vibration (32) est configuré pour maintenir la vibration induite après contact entre l'électrode (31) et un tissu (13) ; et le capteur est configuré pour surveiller un changement dans le signal d'attaque de l'élément de vibration (32), dans lequel un contact entre l'électrode (31) et un tissu (13) entraîne un changement dans le signal d'attaque.
9. Ensemble de détection selon la revendication 8, dans lequel la vibration induite de l'embout est une vibration sensiblement en régime permanent.
10. Ensemble de détection selon la revendication 8, dans lequel l'électrode (31) comprend en outre au moins un canal configuré pour un apport de fluide.
11. Ensemble de détection selon la revendication 8,

dans lequel le changement dans le signal d'attaque électrique est corrélé à une grandeur d'une force appliquée entre l'électrode (31) et un tissu (13).

12. Ensemble de détection selon la revendication 11, 5
comprenant en outre un manche (21) configuré pour apporter un retour basé sur la grandeur d'une force appliquée entre l'électrode (31) et un tissu (13).
13. Ensemble de détection selon la revendication 8, 10
dans lequel la base d'électrode (36) et l'embout d'électrode (34) comprennent un composant unique d'un seul tenant.
14. Ensemble de détection selon la revendication 1, 15
dans lequel
l'électrode (31) comprend un embout d'électrode (34) connecté à une base d'électrode via un joint sphérique configuré pour permettre un mouvement relatif entre l'embout d'électrode (34) et la base d'électrode (36) ; l'élément de vibration (32) connecté opérationnellement à un composant d'embout vibrant comprenant au moins l'un parmi (a) l'embout d'électrode (34) et (b) la base d'électrode (36), l'élément de vibration (32) étant ainsi configuré pour délivrer le signal induisant une vibration au composant d'embout vibrant ; et 20
un système de sortie perceptible configuré pour fournir une sortie perceptible en réponse à la perturbation surveillée dans la vibration induite, dans lequel la sortie perceptible est choisie dans le groupe consistant en une sortie audible, une sortie visuelle et une sortie tactile. 25 30
15. Ensemble de détection selon la revendication 14, 35
comprenant en outre un organe déformable en contact avec la base d'électrode (36) et l'embout d'électrode (34) et configuré pour se déformer en réponse au mouvement relatif entre l'embout d'électrode (34) et la base d'électrode (36). 40
16. Ensemble de détection selon la revendication 15, 45
comprenant en outre un capteur de mesure de déflexion en contact avec l'organe déformable et configuré pour mesurer une déflexion de l'organe déformable.
17. Ensemble de détection selon la revendication 14, 50
dans lequel il existe un espace de débattement entre au moins une portion de l'embout d'électrode (34) et la base d'électrode (36), l'espace étant configuré pour accueillir au moins l'un parmi un mouvement axial et un mouvement latéral de l'embout d'électrode (34) par rapport à la base d'électrode (36). 55
18. Ensemble de détection selon la revendication 14, dans lequel le capteur est situé sur l'embout d'électrode (34).

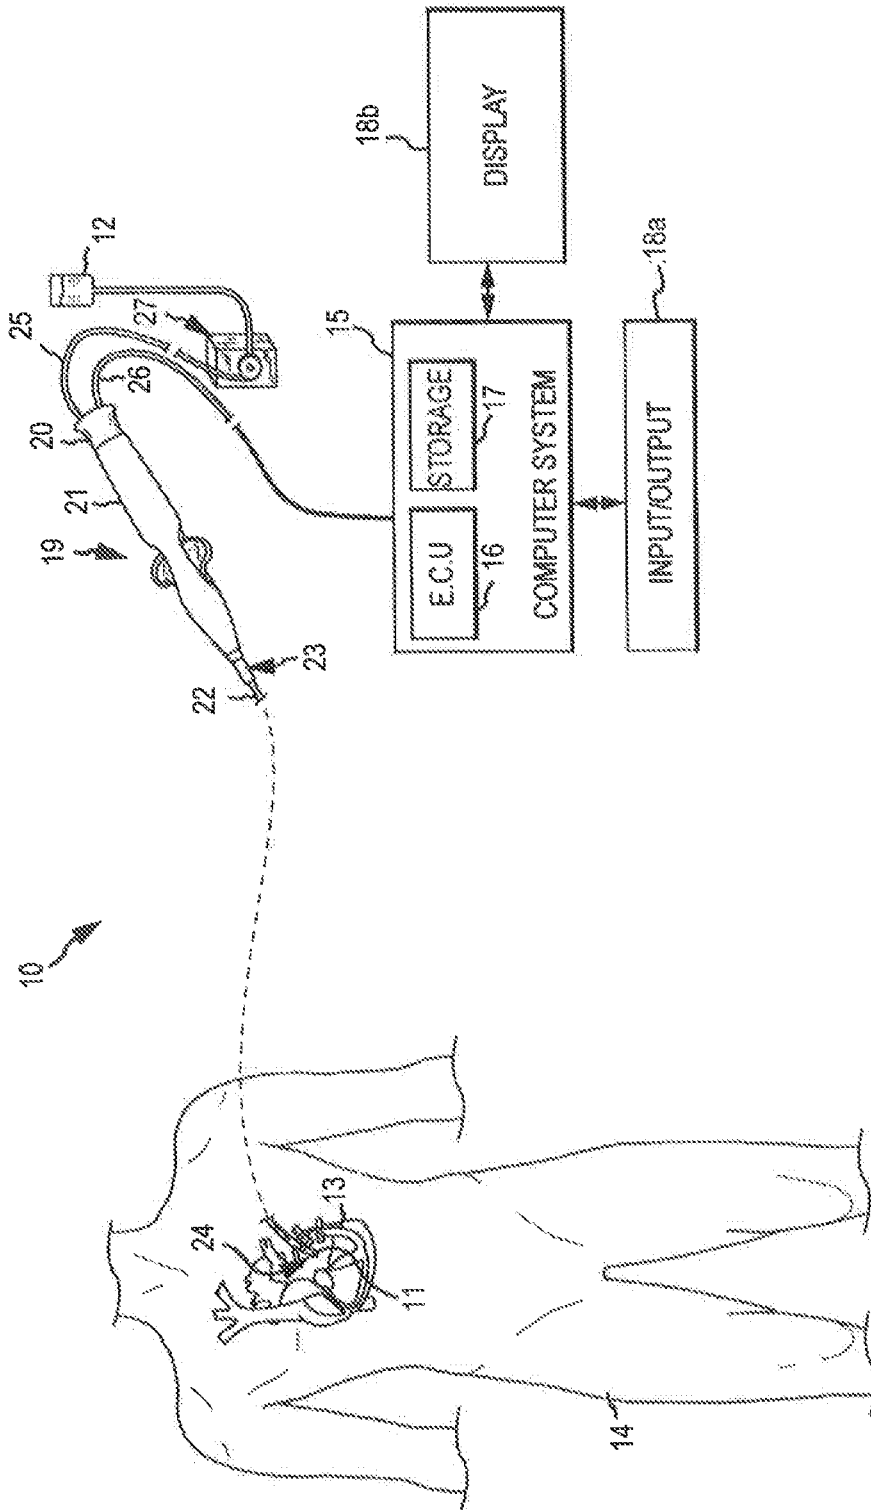


FIG.1

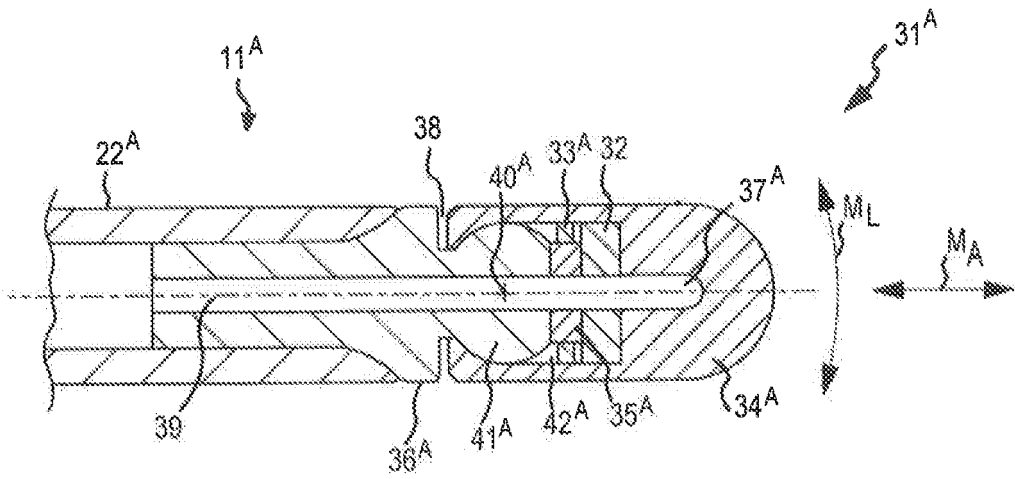


FIG. 2

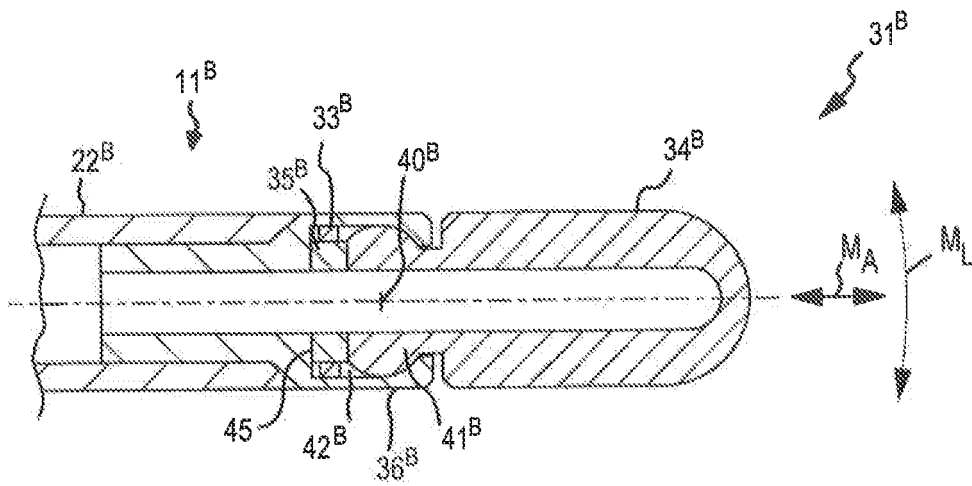


FIG. 3

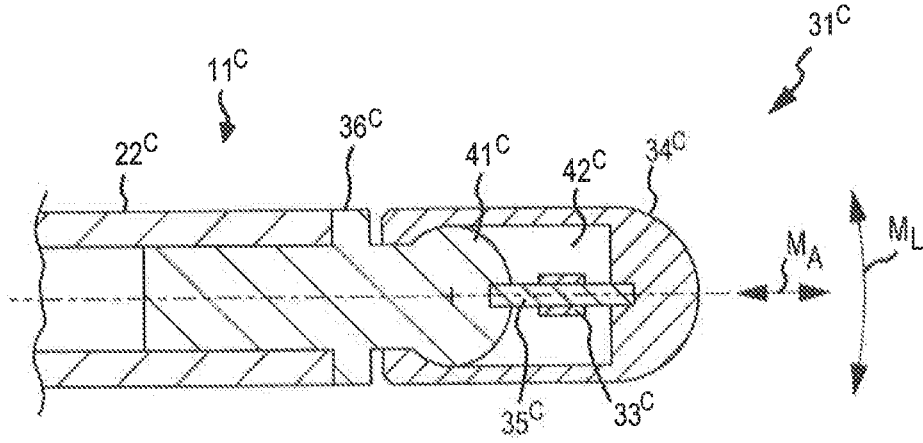


FIG. 4

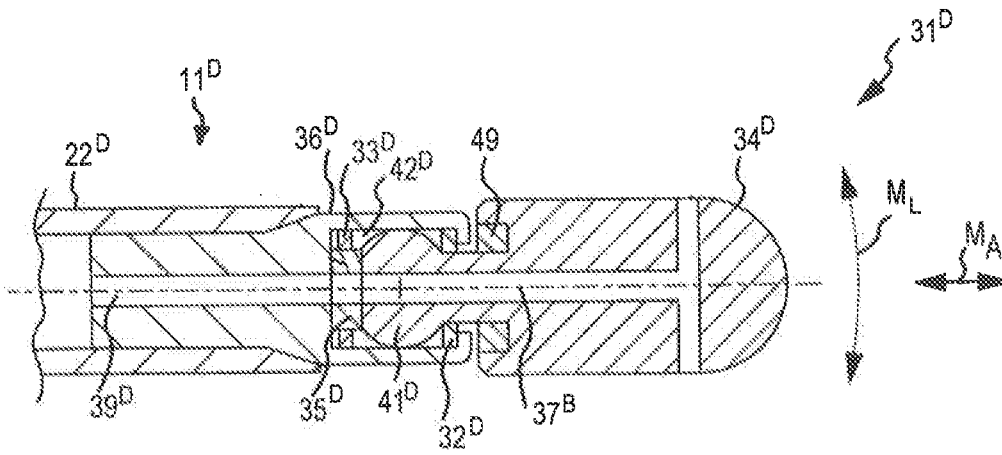


FIG. 5

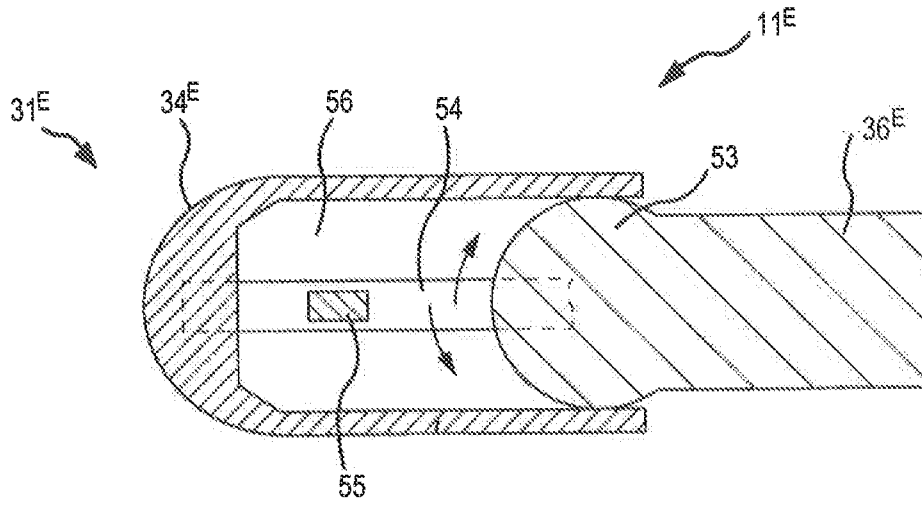


FIG. 6

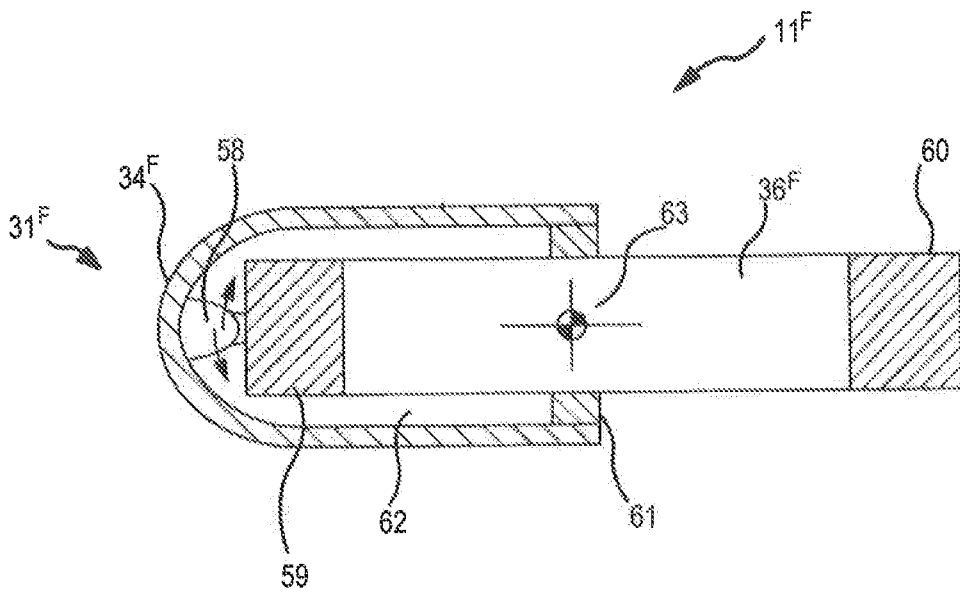


FIG. 7

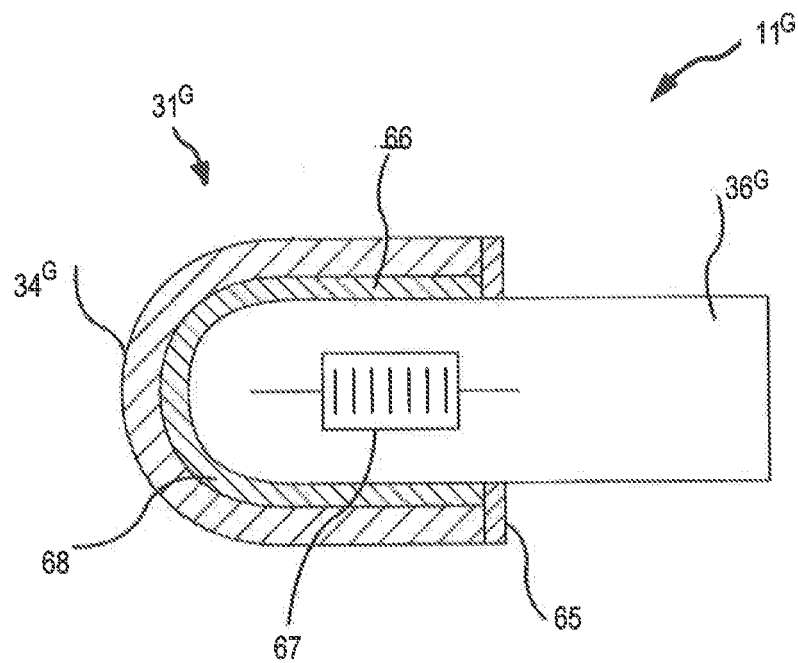


FIG.8

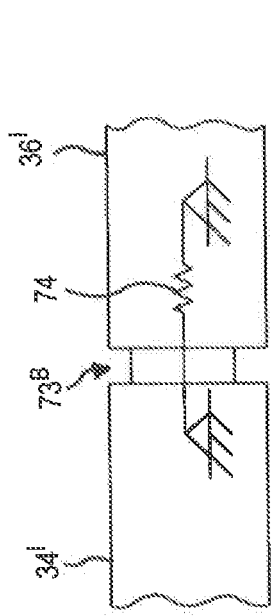


FIG.9B

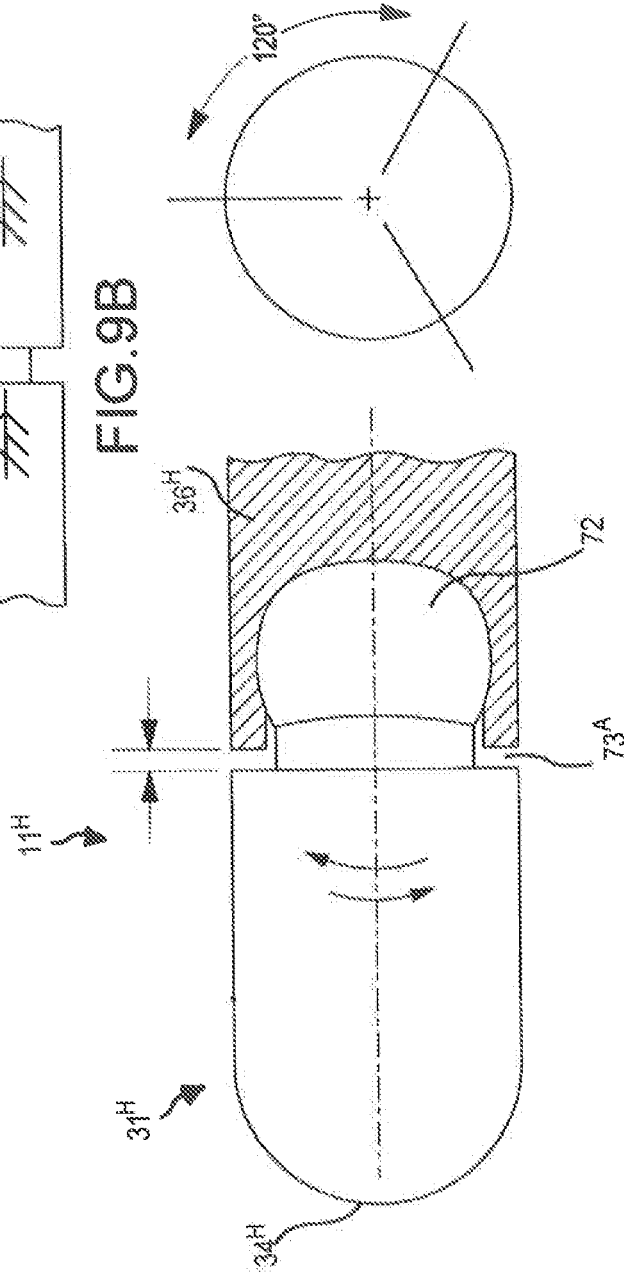
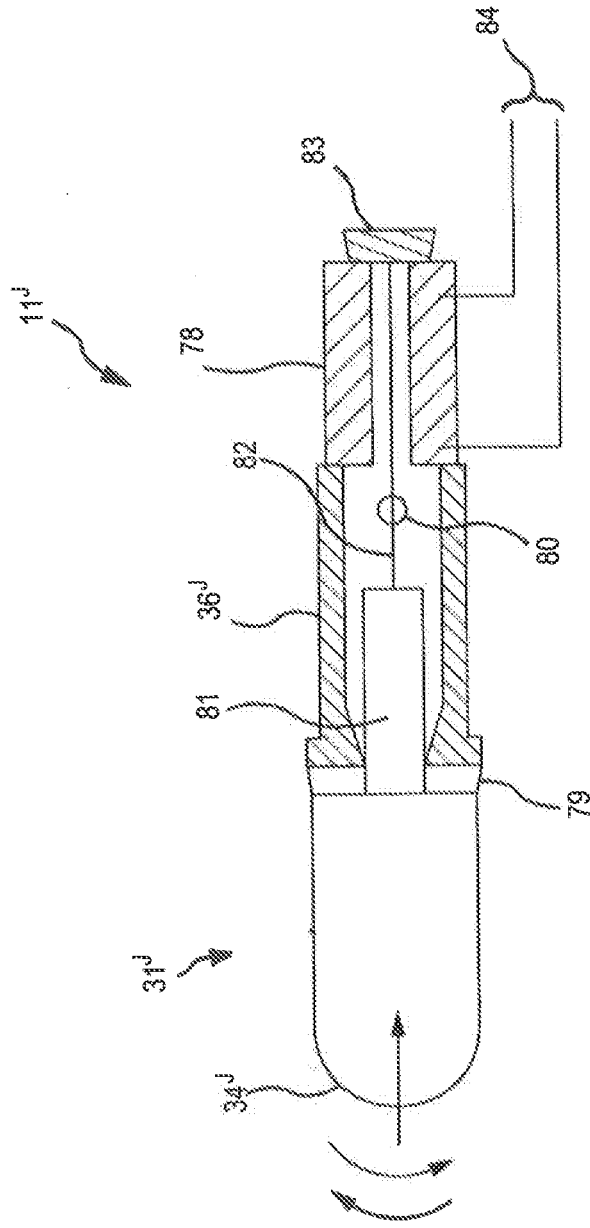


FIG.9C

FIG.9A



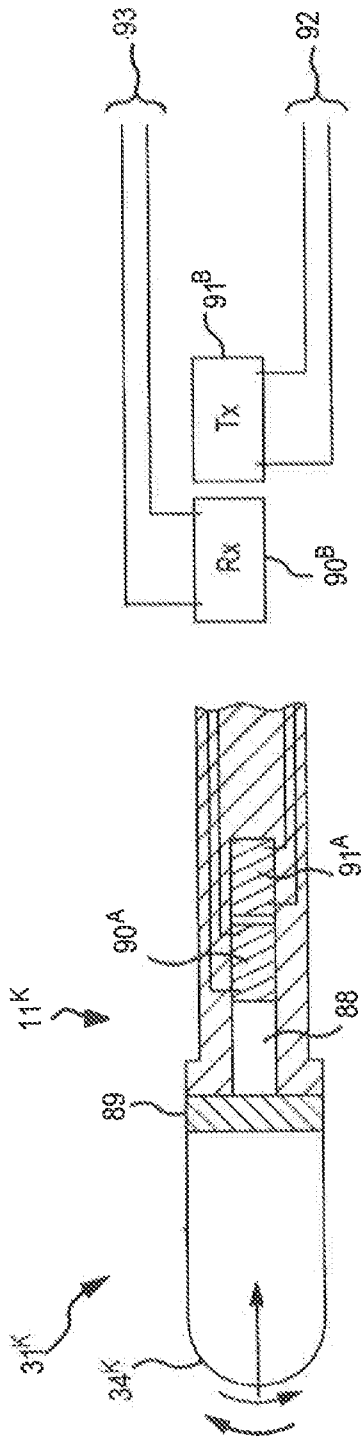


FIG. 11A

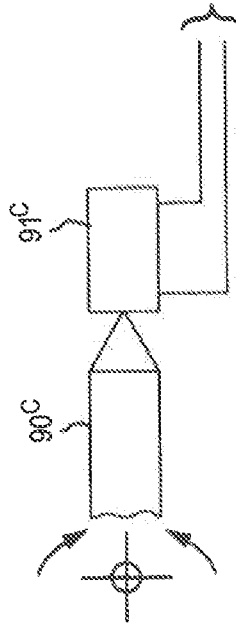


FIG. 11C

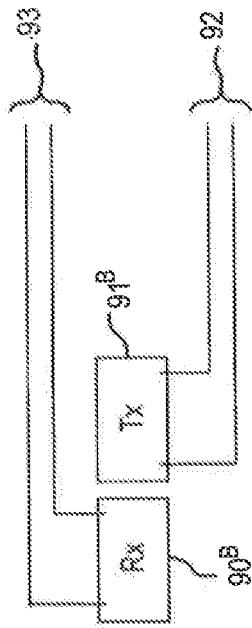


FIG. 11B

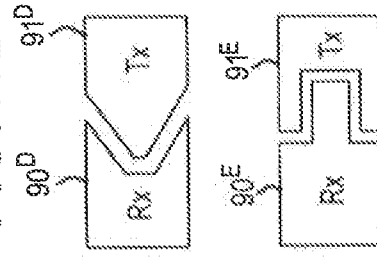


FIG. 11D

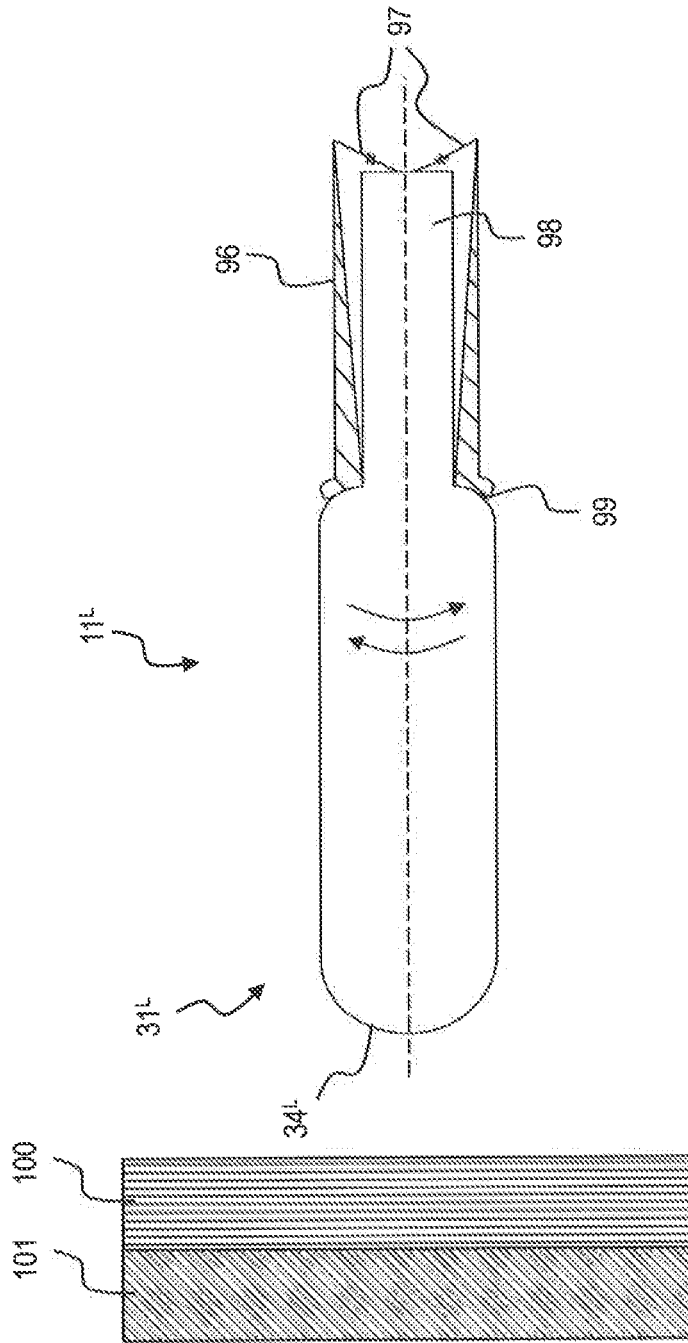


FIG. 12

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 20120065506 A1 [0002]
- US 5911694 A [0003]
- EP 2138123 A1 [0004]
- EP 2742886 A1 [0005]

专利名称(译)	电极接触反馈系统		
公开(公告)号	EP2945561B1	公开(公告)日	2017-09-27
申请号	EP2014720414	申请日	2014-03-17
[标]申请(专利权)人(译)	圣犹达医疗用品电生理部门有限公司		
申请(专利权)人(译)	ST.犹达医疗心房颤动DIVISION INC.		
当前申请(专利权)人(译)	ST.犹达医疗用品, 房颤DIVISION, INC.		
[标]发明人	SCHWEITZER JEFFREY A CHRISTIAN STEVEN C HILL ANTHONY D		
发明人	SCHWEITZER, JEFFREY, A. CHRISTIAN, STEVEN, C. HILL, ANTHONY, D.		
IPC分类号	A61B90/00 A61B5/00 A61B18/14 A61B5/042		
CPC分类号	A61B5/042 A61B5/6885 A61B5/6886 A61B18/1492 A61B2018/0019 A61B2018/00297 A61B2018/00351 A61B2018/0088 A61B2090/065 A61B5/0408 A61B5/6852 A61B90/06 A61B2018/00303		
优先权	61/798138 2013-03-15 US		
其他公开文献	EP2945561A2		
外部链接	Espacenet		

摘要(译)

公开了一种用于感测与物体接触的传感组件。接触感测组件可包括细长管状主体 (22A)。电极 (31A) 可以连接到细长管状主体 (22A)。振动元件 (32) 与电极 (31A) 可操作地连接, 并配置成传递振动诱导信号以引起电极 (31A) 的振动。传感器配置成监测电极 (31A) 以引起诱发振动的扰动。扰动是由电极 (31A) 与物体之间的接触引起的。

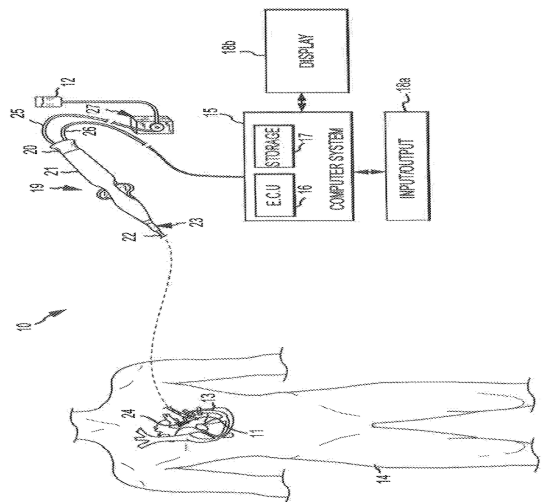


FIG.1