



(11) **EP 2 949 259 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
27.06.2018 Bulletin 2018/26

(51) Int Cl.:
A61B 1/00 (2006.01) **A61B 5/00** (2006.01)
A61B 5/02 (2006.01) **G06T 7/00** (2017.01)
G06T 11/00 (2006.01)

(21) Application number: **13873103.9**

(86) International application number:
PCT/JP2013/000327

(22) Date of filing: **23.01.2013**

(87) International publication number:
WO 2014/115182 (31.07.2014 Gazette 2014/31)

(54) **IMAGE DIAGNOSTIC DEVICE AND INFORMATION PROCESSING DEVICE**

BILDDIAGNOSEVORRICHTUNG UND INFORMATIONSVERRICHTUNG
DISPOSITIF DE DIAGNOSTIC PAR L'IMAGE ET DISPOSITIF DE TRAITEMENT DES
INFORMATIONS

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(43) Date of publication of application:
02.12.2015 Bulletin 2015/49

(73) Proprietor: **Terumo Kabushiki Kaisha**
Tokyo 151-0072 (JP)

(72) Inventors:
• **FURUICHI, Junya**
Ashigarakami-gun
Kanagawa 259-0151 (JP)

• **INOUE, Kouichi**
Ashigarakami-gun
Kanagawa 259-0151 (JP)
• **ETOU, Hijiri**
Ashigarakami-gun
Kanagawa 259-0151 (JP)

(74) Representative: **Casalonga**
Casalonga & Partners
Bayerstraße 71/73
80335 München (DE)

(56) References cited:
JP-A- 2012 505 669 US-A1- 2010 094 127
US-A1- 2012 075 638

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 2 949 259 B1

Description

Technical Field

[0001] The present invention relates to a technique for generating a tomographic image of biological tissues by using light.

Background Art

[0002] Intravascular treatment has been carried out by using a highly functional catheter such as a balloon catheter, a stent or the like. An imaging apparatus for diagnosis such as an optical coherence tomography (OCT) apparatus or the like has been generally used in order to perform preoperative diagnosis or to check postoperative progress.

[0003] The optical coherence tomography apparatus includes a built-in optical fiber, to a distal end of which an imaging core having an optical lens and an optical mirror is attached. At least a distal end portion thereof has a transparent sheath. Then, the sheath is inserted into a blood vessel of a patient. While the imaging core is rotated, light is emitted to an intravascular wall via the optical mirror. The reflection light from the blood vessel is received again via the optical mirror, and radial scanning is performed, thereby configuring a cross-sectional image of the blood vessel, based on the obtained reflection light. Then, while the optical fiber is rotated, a pulling operation (generally called pull-back) is performed at a predetermined speed, thereby forming a three-dimensional image of an inner wall in the longitudinal direction of the blood vessel (refer to PTL 1). In addition, as an improved OCT type, a swept-source optical coherence tomography (SS-OCT) apparatus utilizing wavelength sweeping has also been developed. Document US 2010/094127 A1 discloses an imaging apparatus according to the preamble of claim 1.

Citation List

Patent Literature

[0004] PTL 1: JP-A-2007-267867

Summary of Invention

Technical Problem

[0005] An important point in examining the postoperative progress after the stent indwells the blood vessel is to check how closely a vascular lumen surface is in contact (familiar) with the stent. However, when the three-dimensional image is used to display the postoperative progress, a diagnostician has to check the three-dimensional image by setting various viewpoint positions, thereby causing a complicated operation. In addition, whenever the viewpoint position is changed, the di-

agnostician has to perform a huge amount of calculation for generating the three-dimensional image which can be observed from the changed viewpoint position. Consequently, a high-level response to a user's operation cannot be expected.

[0006] A technique which enables a user to easily check postoperative progress without a need to perform a complicated operation after a stent indwells is applied to the present description.

Solution to Problem

[0007] In order to solve the above-described problem, the present description provides an imaging apparatus for diagnosis as defined in claim 1.

Advantageous Effects of Invention

[0008] According to the present description, it is possible to easily check postoperative progress without a need to perform a complicated operation after a stent indwells.

Brief Description of Drawings

[0009]

[Fig. 1] Fig. 1 is a view illustrating an external configuration of an imaging apparatus for diagnosis according to the present embodiment.

[Fig. 2] Fig. 2 is a view illustrating an overall configuration of a probe unit and a cross-sectional configuration of a distal end portion.

[Fig. 3] Fig. 3 is a diagram illustrating a functional configuration of the imaging apparatus for diagnosis.

[Fig. 4] Fig. 4 is a view for illustrating reconfiguration processing of a cross-sectional image.

[Fig. 5] Fig. 5 is a view illustrating an example of three-dimensional model data of a blood vessel which is reconfigured.

[Fig. 6] Fig. 6 is a view for illustrating an example of volume data when a two-dimensional image is generated according to the embodiment.

[Fig. 7] Fig. 7 is a view illustrating an example of an opacity conversion curve.

[Fig. 8] Fig. 8 is a view illustrating a relationship between a stent and a vascular lumen surface, and an example of a cross-sectional image orthogonal to a blood vessel axis.

[Fig. 9] Fig. 9 is a view illustrating an example of the two-dimensional image generated for a progress examination of the stent according to the embodiment.

[Fig. 10] Fig. 10 is a flowchart illustrating a processing procedure according to the embodiment.

[Fig. 11] Fig. 11 is a view illustrating an example of a user interface displayed on a display screen of the imaging apparatus for diagnosis according to the embodiment.

Description of Embodiments

[0010] Hereinafter, an embodiment according to the present invention will be described in detail with reference to the accompanying drawings.

1. External Configuration of Imaging Apparatus for Diagnosis

[0011] Fig. 1 is a view illustrating an external configuration of an imaging apparatus for diagnosis 100 according to an embodiment of the present invention.

[0012] As illustrated in Fig. 1, the imaging apparatus for diagnosis 100 comprises a probe unit 101, a scanner and pull-back unit 102, and an operation control device 103. The scanner and pull-back unit 102 and the operation control device 103 are connected to each other by a signal line 104 so that various signals can be transmitted.

[0013] The probe unit 101 has an internally inserted imaging core which is directly inserted into a blood vessel and comprises an optical transceiver which continuously transmits transmitted light (measurement light) into the blood vessel and which continuously receives reflected light from the inside of the blood vessel. The imaging apparatus for diagnosis 100 measures an intravascular state by using the imaging core.

[0014] The probe unit 101 is detachably attached to the scanner and pull-back unit 102. A motor incorporated in the scanner and pull-back unit 102 is driven, thereby regulating an intravascular operation in the axial direction and an intravascular operation in the rotation direction of the imaging core which is internally inserted into the probe unit 101.

[0015] The operation control device 103 comprises a function for inputting various setting values upon each measurement, and a function for processing data obtained by the measurement and for displaying various blood vessel images.

[0016] In the operation control device 103, the reference numeral 111 represents a main body control unit. The main body control unit 111 generates interference light data by causing reflected light obtained by the measurement to interfere with reference light obtained by separating the light from a light source, and generates an optical cross-sectional image by processing line data generated based on the interference light data.

[0017] The reference numeral 111-1 represents a printer and DVD recorder, which prints a processing result in the main body control unit 111 or stores the processing result as data. The reference numeral 112 represents an operation panel, and a user inputs various setting values and instructions via the operation panel 112. The reference numeral 113 represents an LCD monitor as a display device, which displays a cross-sectional image generated in the main body control unit 111. The reference numeral 114 represents a mouse serving as a pointing device (coordinate input device).

2. Overall Configuration of Probe Unit and Cross-Sectional Configuration of Distal End Portion

[0018] Next, an overall configuration of the probe unit 101 and a cross-sectional configuration of a distal end portion will be described with reference to Fig. 2. As illustrated in Fig. 2, the probe unit 101 is configured to include a long catheter sheath 201 to be inserted into the blood vessel and a connector unit 202 to be arranged on the front side of a user so as to be operated by the user without being inserted into the blood vessel. A guidewire lumen tube 203 which fixes a guidewire 250 for guiding the probe unit 101 to a position of a diagnosis-targeted blood vessel is disposed in the distal end of the catheter sheath 201. The catheter sheath 201 has a lumen which is continuously formed from a connection portion with the guidewire lumen tube 203 to a connection portion with the connector unit 202.

[0019] An imaging core 220 which internally comprises a transceiver 221 in which the optical transceiver for transmitting and receiving the light is arranged and which comprises a coil-shaped drive shaft 222 internally comprising an optical fiber cable and transmitting rotary drive power for rotating the transceiver 221 is inserted into the lumen of the catheter sheath 201 over substantially the entire length of the catheter sheath 201.

[0020] The connector unit 202 comprises a sheath connector 202a configured to be integral with a proximal end of the catheter sheath 201, and a drive shaft connector 202b which is configured to rotatably fix the drive shaft 222 to the proximal end of the drive shaft 222.

[0021] An anti-kink protector 211 is disposed in a boundary section between the sheath connector 202a and the catheter sheath 201. This can maintain predetermined rigidity, and can prevent bending (kink) caused by a rapid change in physical properties.

[0022] The proximal end of the drive shaft connector 202b is detachably attached to the scanner and pull-back unit 102.

[0023] A housing 223 has a shape in which a short cylindrical metal pipe partially has a cutout portion, and is formed by being cut out from a metal ingot, or is molded by means of metal powder injection molding (MIM) or the like. In addition, an elastic member 231 having a short coil shape is disposed on the distal end side.

[0024] The elastic member 231 is obtained by forming a stainless steel wire into a coil shape. The elastic member 231 is arranged on the distal end side, thereby preventing the imaging core 220 from being caught on the inside of the catheter sheath 201 when the imaging core 220 is moved forward and rearward.

[0025] The reference numeral 232 represents a reinforcement coil which is disposed in order to prevent rapid bending of the distal end portion of the catheter sheath 201.

[0026] The guidewire lumen tube 203 has a guidewire lumen into which a guidewire 250 can be inserted. The guidewire 250 is used in guiding the distal end of the

catheter sheath 201b to a lesion.

3. Functional Configuration of Imaging Apparatus for Diagnosis

[0027] Next, a functional configuration of the imaging apparatus for diagnosis 100 will be described. Fig. 3 is a diagram illustrating the functional configuration of the imaging apparatus for diagnosis 100 which includes an OCT function (here, a swept source OCT as an example). Hereinafter, the functional configuration of the swept source OCT will be described with reference to the same drawings.

[0028] In the drawing, the reference numeral 408 represents a wavelength swept light source (swept laser), and is one type of an extended-cavity laser which includes an optical fiber 416 which is coupled to a semiconductor optical amplifier (SOA) 415 in a ring shape and a polygon scanning filter (408b).

[0029] Light output from the SOA 415 proceeds to the optical fiber 416, and enters the polygon scanning filter 408b. The light whose wavelength is selected here is amplified by the SOA 415, and is finally output from a coupler 414.

[0030] The polygon scanning filter 408b selects the wavelength in combination with a diffraction grating 412 for diffracting the light and a polygon mirror 409. Specifically, the light diffracted by the diffraction grating 412 is concentrated on a surface of the polygon mirror 409 by two lenses (410 and 411). In this manner, only the light having a wavelength orthogonal to the polygon mirror 409 returns through the same optical path, and is output from the polygon scanning filter 408b. That is, time sweeping of the wavelength can be performed by rotating the polygon mirror 409.

[0031] For example, a 32-sided mirror is used for the polygon mirror 409 whose rotation speed is approximately 50000 rpm. A wavelength swept system in which the polygon mirror 409 and the diffraction grating 412 are combined with each other enables high speed and high output wavelength sweeping.

[0032] The light of a wavelength swept light source 408 which is output from the coupler 414 is incident on one end of a first single mode fiber 440, and is transmitted to the distal end side. The first single mode fiber 440 is optically coupled to a second single mode fiber 445 and a third single mode fiber 444 in an optical coupler 441 located in the middle therebetween.

[0033] On the further distal end side than the optical coupler 441 of the first single mode fiber 440, an optical rotary joint (optical coupling unit) 403 which transmits the light by coupling a non-rotating part (fixed portion) and a rotating part (rotary drive unit) to each other is disposed inside the rotary drive device 404.

[0034] Furthermore, a fifth single mode fiber 443 of the probe unit 101 is detachably connected via the adapter 402 to the distal end side of a fourth single mode fiber 442 inside the optical rotary joint (optical coupling unit)

403. In this manner, the light from the wavelength swept light source 408 is transmitted to the fifth single mode fiber 443 which is inserted into the imaging core 220 and can be rotatably driven.

[0035] The transmitted light is emitted from the optical transceiver 221 of the imaging core 220 to the biological tissues inside the blood vessel while a rotary operation and an axial operation are performed. Then, the reflected light scattered on a surface or inside the biological tissues is partially captured by the optical transceiver 320 of the imaging core 220, and returns to the first single mode fiber 440 side through a rearward optical path. Furthermore, the light is partially transferred to the second single mode fiber 445 side by the optical coupler 441, and is emitted from one end of the second single mode fiber 445. Thereafter, the light is received by an optical detector (for example, a photodiode 424).

[0036] The rotary drive unit side of the optical rotary joint 403 is rotatably driven by the radial scanning motor 405 of the rotary drive device 404.

[0037] On the other hand, an optical path length variable mechanism 432 for finely adjusting an optical path length of reference light is disposed in the distal end opposite to the optical coupler 441 of the third single mode fiber 444.

[0038] In order for variations in the length of an individual probe unit 101 to be absorbed when the probe unit 101 is replaced and newly used, this optical path length variable mechanism 432 comprises optical path length changing means for changing an optical path length corresponding to the variations in the length.

[0039] The third single mode fiber 444 and a collimating lens 418 are disposed on a one-axis stage 422 which is movable in an optical axis direction thereof as illustrated by an arrow 423, thereby forming the optical path length changing means.

[0040] Specifically, the one-axis stage 422 functions as the optical path length changing means having a variable enough range of the optical path length to absorb the variations in the optical path length of the probe unit 101 when the probe unit 101 is replaced. Furthermore, the one-axis stage 422 also comprises a function as adjusting means for adjusting an offset. For example, even when the distal end of the probe unit 101 is not in close contact with the surface of the biological tissues, the one-axis stage finely changes the optical path length. In this manner, it is possible to set the optical path length in a state of interfering with the reflected light from the surface position of the biological tissues.

[0041] The optical path length is finely adjusted by the one-axis stage 422. The light reflected on a mirror 421 via a grating 419 and a lens 420 is mixed with the light obtained from the first single mode fiber 440 side by the optical coupler 441 disposed in the middle of the third single mode fiber 444, and then is received by the photodiode 424.

[0042] Interference light received by the photodiode 424 in this way is photoelectrically converted, and is input

to a demodulator 426 after being amplified by the amplifier 425. The demodulator 426 performs demodulation processing for extracting only a signal portion of the interference light, and an output therefrom is input to the A/D converter 427 as an interference light signal.

[0043] The A/D converter 427 performs sampling on the interference light signal, for example, at 90 MHz by an amount of 2048 points, and generates digital data (interference light data) of one line. The reason for setting the sampling frequency to 90 MHz is on the assumption that approximately 90% of wavelength swept cycles (12.5 μ sec) is extracted as the digital data of 2048 points, when a repetition frequency of the wavelength sweeping is set to 40 kHz. However, the sampling frequency is not particularly limited thereto.

[0044] The interference light data in the units of lines which is generated by the A/D converter 427 is input to the signal processing unit 428. The signal processing unit 428 generates data in a depth direction (line data) by performing frequency resolution on the interference light data using the fast Fourier transform (FFT), and the data is subjected to coordinate transformation. In this manner, an optical cross-sectional image is constructed at each intravascular position, and is output to the LCD monitor 113.

[0045] The signal processing unit 428 is further connected to a control device of optical path length adjusting means 430. The signal processing unit 428 controls a position of the one-axis stage 422 via the control device of optical path length adjusting means 430.

[0046] The processing in the signal processing unit 428 is also realized in such a way that a predetermined program causes a computer to execute the processing.

4. Image Reconfiguration Processing

[0047] In the above-described configuration, if a user operates the operation control device 103 and inputs an instruction to start scanning, the signal processing unit 428 controls the scanner and pull-back unit 102 so as to rotate the imaging core 220 and pull the imaging core 220 at a predetermined speed so as to move in the longitudinal direction of the blood vessel. At this time, generally, a transparent flush solution is caused to flow into the blood vessel until light emitting and light receiving performed by the imaging core 220 is prevented from being obstructed by the blood. Based on the above-described result, as described above, the A/D converter 427 comes to output the digital interference light data. Accordingly, the signal processing unit 428 continuously builds an optical cross-sectional image at each position along the movement direction of the imaging core 220, in a memory 428a belonging to the signal processing unit 428.

[0048] Here, processing for generating one sheet of the optical cross-sectional image will be described with reference to Fig. 4. Fig. 4 is a view for illustrating reconfiguration processing of the cross-sectional image of a

blood vessel 401 in which the imaging core 220 is located. While the imaging core 220 is rotated once (rotation of 360 degrees), the measurement light is transmitted and received many times. The light transmitted and received once can obtain data of one line in a light-emitted direction. Accordingly, during one rotation, it is possible to obtain 512 items of the line data radially extending from the rotation center 402 by transmitting and receiving the light 512 times, for example. The line data is calculated by means of a known method, thereby continuously generating three-dimensional model data extending in the radial direction (direction r) from the rotation center position. One line in this model data is configured to include 1024 luminance values 10 to 11023. The luminance value 10 represents the rotation center position, and the luminance value 11023 represents a luminance value at a position farthest from the rotation center position.

[0049] In the above-described manner, 512 items of line data are continuously built. However, the items become closer to each other in the vicinity of the rotation center position, and become isolated from each other as the items are separated from the rotation center position. Accordingly, a pixel present in an empty space between the respective lines is continuously generated by performing known interpolation thereon so as to generate a cross-sectional image visible to humans. It should be noted that the center position of the cross-sectional image coincides with the rotation center position of the imaging core 220 and does not represent the center position of the blood vessel cross section.

[0050] When the light is transmitted and received, the light is also reflected from the catheter sheath 201 itself. Accordingly, as illustrated in the drawing, a shadow 403 of the catheter sheath 201 is formed on the cross-sectional image. In addition, the reference numeral 404 illustrated in the drawing is the shadow of the guidewire 250. In practice, the guidewire 250 is made of metal and the light is not transmitted therethrough. Thus, it is not possible to obtain an image of a rear side portion of the guidewire 250 when viewed from the rotation center position. The illustration is to be recognized as a merely conceptual diagram.

[0051] If a user operates the operation control device 103 and inputs an instruction to start scanning, the signal processing unit 428 controls the scanner and pull-back unit 102 so as to rotate the imaging core 220 and pull the imaging core 220 at a predetermined speed so as to move in the longitudinal direction of the blood vessel (pull-back processing). As a result, the signal processing unit 428 continuously builds multiple cross-sectional images taken along the pulling direction of the image core 220, in its own memory 428a.

[0052] The reference numeral 500 in Fig. 5 illustrates a conceptual diagram of three-dimensional image data generated by connecting the multiple cross-sectional images built in the memory 428a to one another in the pull-back processing. The z axis illustrated in the drawing represents a pull-back direction (longitudinal direction of

the blood vessel). As is well known, if the thrombus or the like is present, a passage through which the blood flows is locally narrowed. A broken line illustrated in the drawing represents a boundary surface with the blood in the blood vessel. Hereinafter, the boundary surface is referred to as a vascular lumen surface. That is, it should be understood that the vascular lumen surface includes not only a blood vessel inner wall but also the thrombus.

[0053] A case may be considered where the stent is arranged. In this case, the three-dimensional image as illustrated in Fig. 5 can be obtained. However, it is necessary to set various viewpoint positions in order to recognize which portion of the stent has a gap with the vascular lumen surface, and which portion is in contact with the vascular lumen surface. However, this causes the operation to be complicated. Above all, processing for reconfiguring the three-dimensional image needs a huge amount of calculation. Accordingly, it is impractical to perform the reconfiguration processing of the three-dimensional image each time in response to a user's instruction to change the viewpoint position. Consequently, a high-level response to the user's operation cannot be expected.

[0054] In the present embodiment, instead of displaying a positional relationship between the stent and the vascular lumen surface as a three-dimensional image, the positional relationship is displayed as a two-dimensional image which does not require a change in the viewpoint position. Hereinafter, a principle thereof will be described with reference to Figs. 6 to 9.

[0055] As described above, when the positional relationship between the stent and the vascular lumen surface is observed, a point which a user wants to recognize most is which portion of the stent has a gap with the vascular lumen surface, and which portion is in contact with the vascular lumen surface. In the present embodiment, the two-dimensional image which enables the user to easily recognize the related point is generated. In addition, if the stent becomes familiar with the vascular lumen surface to some extent, even the lumen surface of the stent is covered with vascular tissues. Therefore, the two-dimensional image according to the present embodiment also enables the user to easily observe the related point.

[0056] One line data 450 illustrated in Fig. 4 can be specified by a position in the longitudinal direction (z axis) of the blood vessel and a rotation angle θ . Then, one of 1024 luminance values in the line data 450 can be specified by a distance r (r is any one of 0, 1, 2, to 1023) from the rotation center position. Accordingly, it can be understood that any optional pixel value in the line data obtained by the pull-back processing can be specified in the space having three axes $\{z, \theta, \text{ and } r\}$.

[0057] Fig. 6 illustrates a three-dimensional space defined by the three axes z, θ , and r . The reference numeral 601 illustrated in the drawing indicates the line data specified by an angle θ_1 in a cross section of $z=0$. However, as described with reference to Fig. 4, data I_0 to I_{n-1} (ref-

erence numeral 403 in Fig. 4) from the rotation center position to the surface of the catheter sheath 220 in one line data is data having no relationship with the blood vessel. Accordingly, the corresponding portion is cut away so as to handle the remaining luminance I_n to I_{1023} as valid data. In the three-dimensional space in Fig. 6, as a position has a smaller value of r , it is illustrated that the position is closer to the rotation center. The reference numeral n illustrated here represents a known value including an outer diameter of the catheter sheath 201.

[0058] In the present embodiment, the "two-dimensional image" obtained when a direction having a positive value of r is viewed from a position having a negative value of r is rebuilt in the three-dimensional space in Fig. 6. In short, the two-dimensional image of $[\theta-z]$ obtained when viewed from the rotation center position is reconfigured. The two-dimensional image is an image shown in a coordinate space between θ and z . Accordingly, a pixel value in the two-dimensional image can be expressed by $P(z, \theta)$. Therefore, hereinafter, a calculation method of the pixel value $P(z, \theta)$ will be described.

[0059] In the present embodiment, as illustrated in Fig. 7, each luminance value I_m (m is any one of n to 1023) is converted into opacity by setting a conversion curve f which is shown by the luminance value and the opacity and is represented by the reference numeral 700. In the conversion curve f , when the luminance value is equal to or smaller than I_L , the opacity has the minimum value $a_{\min}$ (in the embodiment, $a_{\min}=0$), that is, the transparency is maximized. In contrast, when the luminance value is equal to or greater than I_H , the opacity has the maximum value $a_{\max}$, that is, the transparency is minimized. Then, a portion between the luminance values I_L and I_H has a linear shape. A user can freely move the conversion curve 700 in parallel along the z axis, and the meaning will be described later. By default, the opacity of the surface tissues on the vascular lumen surface which is obtained statistically is set to have a value greater than the minimum value $a_{\min}$.

[0060] In the present embodiment, in a relationship with a preset threshold value Th (in the embodiment, threshold value $Th=1$), the minimum value m satisfying the following equation is obtained.

$$f(I_n) + f(I_{n+1}) + \dots + f(I_m) \geq Th$$

Then, the minimum value m is utilized, and a representative pixel value $P(z, \theta)$ representing the targeted line data is calculated by using the following equation. When the representative pixel value of the targeted line data in the coordinates (θ, z) is calculated, instead of referring to the other line data, the representative pixel value is expressed as a function of only the position in the targeted line data as in the following equation. $P(z, \theta) = P_i = f(I_i) * I_i + (1 - f(I_i)) * P_{i-1}$

Here, i is the index number of data points and rows in

the direction r , and the relationship is expressed by $n \leq m$.

[0061] As described above, the above-described processing is to describe image generation of the "two-dimensional image" obtained when the direction having the positive value of r is viewed from the position having the negative value of r in the r axis in Fig. 6. However, without being limited to the related two-dimensional image, the viewpoint direction may be optionally rotated and moved in parallel by a user. When the viewpoint direction is rotated, the two-dimensional image to be displayed is displayed as a positive projection image in the viewing direction of the three-dimensional space illustrated in Fig. 6. As described above, in the processing content, a data group of $\{In \text{ to } Im\}$ may be calculated by being replaced with a data group having the luminance values arrayed on the line of sight in Fig. 6. In this case, m can take a value greater than 1023.

[0062] The luminance value from the catheter sheath 201 to the vascular lumen surface is small due to an action of a flush solution. Therefore, the opacity therebetween is equal to or close to the minimum $a_{\max}$ (maximum transparency). Then, if the stent reaches a surface of the vascular lumen surface, the opacity gradually increases along the depth direction. Accordingly, it can be described that the pixel value $P(z, \theta)$ represents a result of adding the opacity in the depth direction to some extent from the vascular lumen surface.

[0063] In contrast, the stent is configured to have metal, and thus has very high luminance (high reflection intensity). The high luminance representing the stent has a sufficiently greater value as compared to the vascular tissues. Accordingly, it is convenient to distinguish the stent from the vascular lumen surface. The pixel value $P(z, \theta)$ obtained by the above-described calculation becomes a greater value as compared to the pixel value of the vascular lumen surface.

[0064] In addition, in a state where the stent is covered with the vascular tissues when viewed from the inner side of the stent, the opacity exceeding the minimum value $a_{\min}$ of the vascular tissues is added to some extent in the above-described calculation process. Thereafter, the opacity representing the stent is added thereto. The pixel value $P(z, \theta)$ obtained as a result becomes a much greater value as compared to that in a case where the stent is exposed. That is, it is possible to discriminate a case where the stent is exposed on the blood flow surface and a case where the stent is covered with the vascular tissues from each other.

[0065] According to the two-dimensional image represented by the pixel $P(z, \theta)$ generated as described above, it is not possible to recognize whether the rear surface of the stent is in contact with the vascular lumen surface, or whether there is a gap from the rear surface to the vascular lumen surface. Therefore, interpolation processing is performed on the two-dimensional image according to the present embodiment so that the related point can be discriminated.

[0066] Here, a principle of detecting a gap between the rear surface of the stent and the vascular lumen surface will be described with reference to Fig. 8.

[0067] The drawing is a perspective conceptual view when a blood vessel 800 is viewed from a position orthogonal to the longitudinal direction of the blood vessel 800. The reference numeral 850 illustrated in the drawing represents the stent. As previously described, the reference numeral 201 represents the catheter sheath, and the reference numeral 250 represents the guidewire.

[0068] The lower part of Fig. 8 illustrates respective cross-sectional views at a position A-A' and a position B-B' of the blood vessel 800.

[0069] In general, the stent 850 expands its diameter after indwelling a targeted vascular position. Thus, the stent 850 has a mesh structure. Accordingly, as illustrated in the cross-sectional view A-A' and the cross-sectional view B-B', the stent 850 is detected in a state of being scattered at discrete positions on the cross-sectional image obtained by one rotation viewed from the imaging core 220.

[0070] The cross-sectional image A-A' indicates that a gap is present over an entire angular range between the stent and a vascular lumen surface 801. In addition, the cross-sectional image B-B' indicates a state where a portion of the stent is covered with the vascular tissues. In addition, the stent 850 and the guidewire 250 are generally made of metal. Thus, the reflectivity of the light is very high and thus the light is not transmitted there-through. Accordingly, it is not possible to obtain an image on the rear side of the stent 850 and the guidewire 250 when viewed from the imaging core 220. It should be noted that the illustration is merely a conceptual view. Although details will be described later, a method of discriminating the guidewire and the stent from each other will be described later.

[0071] Based on the cross-sectional view, it is possible to easily calculate a distance $L0$ from the rotation center position of the imaging core 220 to the surface of the stent. In addition, as described above, since the stent is made of metal, it is not possible to obtain an image of the vascular lumen surface on the rear surface of the stent. However, a distance $L1$ to the vascular lumen surface when it is assumed that the stent is not present may be calculated by respectively coming into contact with both ends of the stent and setting an average value between two lines L' and L'' where the stent is not detected to the distance $L1$.

$$L1 = (L' + L'') / 2$$

[0072] In addition, the cross-sectional image A-A' in Fig. 8 is displayed, a point which a user regards as the vascular lumen surface is indicated at multiple locations, and the multiple points are interpolated in a cubic spline. In this manner, the distance $L1$ may be obtained by gen-

erating a closed curve representing a virtual vascular lumen surface and referring to the generated closed curve.

[0073] Here, a thickness d of the stent is known depending on a type of the stent, and is set in advance. Accordingly, a gap (in general, called a malapposition) MP between the rear surface of the stent 850 and the vascular lumen surface 801 can be obtained by using the following equation.

$$MP = L1 - \{L0 + d\}$$

Here, when the malapposition MP is greater than zero, an indication that "the malapposition is present" between the stent 850 and the vascular lumen surface 801 is shown. In order to allow some error, a predetermined non-negative threshold value TH_{mp1} is set in the embodiment. When a relationship satisfies $MP > TH_{mp1}$, it is determined that the malapposition is present. A pixel for determining the presence or absence of the malapposition may be set to a pixel which is adjacent to a pixel determined to belong to the stent and is determined to belong to the vascular lumen surface.

[0074] In addition, a case of $L1 < L0$ indicates a state where the stent is covered with the vascular tissues. However, a non-negative threshold value TH_{mp2} is set in order to allow some errors. When a case where the relationship satisfies $L0 - L1 < TH_{mp2}$ indicates the state where the stent is covered with the vascular tissues. A determination-targeted pixel is set to be the same as that of the malapposition.

[0075] Next, distinction between the guidewire 250 and the stent 850 will be described. As previously described, the guidewire 250 is made of metal similarly to the stent 850. Accordingly, luminance distribution of the line data in which the stent is present resembles luminance distribution of the guidewire 250. The guidewire 250 is not always disposed by keeping a suitable distance from the inner surface of the stent 850, and may be disposed by being in contact with the inner surface of the stent 850. Accordingly, it is difficult to distinguish the guidewire and the stent from each other on one cross-sectional image.

[0076] However, the present inventors focus on a fact that the stent 850 is caused to indwell only a treatment-targeted region and the pull-back processing is performed by including an outside region of the treatment-targeted region in order to observe the entire treatment-targeted region. That is, the guidewire 250 is detected throughout the pull-back region, and the stent or the like appears in only a specified region where the pull-back processing is performed. By utilizing this characteristic, the guidewire and the stent are distinguished from each other as follows.

[0077] First, a direction of an angle θ where the line data having a high luminance pixel detected is present is determined as a candidate point of the stent for a single tomographic image of an end portion in the pull-back

processing. Then, the stent candidate is also similarly obtained for the adjacent tomographic image, and the candidate point having the angle closest to the candidate point on the adjacent tomographic image is detected, thereby performing grouping. This processing is performed for the other end portion of the pull-back processing, thereby calculating a group of one candidate point continuous throughout the entire region of the pull-back processing. The candidate point configuring one group is recognized as the guidewire 250.

[0078] Hitherto, the processing in the embodiment has been described. However, the outline is as follows.

[0079] Based on the line data obtained by the pull-back processing, the signal processing unit 428 builds each cross-sectional tomographic image along the z axis which serves as a three-dimensional tomographic image as usual, that is, builds three-dimensional volume data (refer to Fig. 5). Then, the signal processing unit 428 converts the luminance value in each line data in accordance with the opacity conversion curve f . In accordance with the previously described principle, the signal processing unit 428 calculates each pixel value $P(z, \theta)$ configuring the two-dimensional image which is fundamental to θ - z in the embodiment. At this time, discrimination processing of the stent and the guidewire is also performed. According to the processing till now, each pixel of the two-dimensional image is determined to belong to any one of the stent, the guidewire, and the vascular lumen surface.

[0080] Next, the signal processing unit 428 obtains the distance $L0$ between a pixel $P1$ which belongs to the stent and is adjacent to the pixel of the vascular lumen and the rotation center position on the tomographic image. In addition, the signal processing unit 428 obtains the distance $L1$ between a pixel $P2$ which belongs to the vascular lumen and is adjacent to the pixel $P1$ of the stent and the rotation center position on the tomographic image. Then, based on the preset thickness d of the stent, and the distances $L0$ and $L1$, the signal processing unit 428 determines whether or not the pixel $P2$ (or $P1$) configures the malapposition, or determines whether or not the stent is covered with the tissues of the vascular lumen, and adds correction to the determination result in order to perform emphasis processing of the pixel value $P2$. In the embodiment, as the correction processing, correction of the pixel value is added so as to become a line segment of a broken thick line, a solid line, and a broken normal line along the pixel $P2$.

[0081] Fig. 9 illustrates an example of the two-dimensional image generated by adding the above-described correction processing. In Fig. 9, the vertical axis is θ , and the horizontal axis is the direction z (longitudinal direction of the blood vessel = pull-back direction). Fig. 9 illustrates the two-dimensional image of θ - z , and thus the image comes to have a rectangular shape.

[0082] The reference numeral 900 which forms the illustrated mesh represents an image of the stent. A broken thick line 901 indicates that the stent in which the

thick broken line serves as a boundary line on both sides configures the malapposition (that a gap is present between the rear surface of the stent and the vascular lumen surface). In addition, a broken thin line 902 indicates that the stent is covered with the tissues of the vascular lumen at the portion. A curve 250 indicates the guidewire. However, as described above, the discrimination of the guidewire from the stent is performed. Thus, an edge of the curve 250 is not a display target for indicating the malapposition or that the stent is covered with the vascular lumen tissues.

[0083] According to the two-dimensional image in Fig. 9, it is possible to obviously understand a stabilized state where the malapposition is formed in an entire angular range on the left side of the stent, and where the entire angular region on the right side of the stent is covered with the vascular tissues.

5. Description of Processing Procedure

[0084] The signal processing unit 428 which has completed the pull-back processing may consequently generate each cross-sectional image according to the flowchart in Fig. 10. Hereinafter, processing of the signal processing unit 428 will be described with reference to the drawing. In practice, a processing procedure according to the flowchart in the drawing is stored in a hard disk device or the like, as a program executed by the signal processing unit.

[0085] First, in Step S1001, line data acquired by the pull-back processing is received and stored in the memory 428a. Next, in Step S1002, the signal processing unit 429 reconfigures each cross-sectional image, and generates three-dimensional volume data (refer to Fig. 5). The generation processing is known, and thus description thereof will be omitted here.

[0086] In subsequent Step S1003, the signal processing unit 428 calculates each pixel value $P(z, \theta)$ of the two-dimensional image which is fundamental. Thereafter, in Step S1004, the signal processing unit 428 performs processing for discriminating whether each pixel unit belongs to any one of the stent, the guidewire, and the vascular lumen. Although details have been described above, as an initial value, the signal processing unit 428 may determine all pixels belong to the vascular lumen. Thereafter, the signal processing unit 428 may determine that the pixel P having high reflectivity belongs to the guidewire and the stent.

[0087] In Step S1005, the signal processing unit 428 refers to the volume data, and determines whether or not the pixel adjacent to the stent among the pixels belonging to the vascular lumen configures the malapposition, or whether or not the stent is covered with the vascular tissues. Based on the determination result, the signal processing unit 428 performs emphasis processing so that both of these can be distinguished from each other. In Fig. 9, a pixel value is corrected so that the pixel belonging to the malapposition is illustrated by the broken

thick line, the portion covered with the vascular tissues is illustrated by the broken line, and the others (state where the rear surface of the stent is in contact with the vascular lumen surface) are illustrated by the solid line.

In Step S1006, the signal processing unit 428 generates the two-dimensional image for display together with various user interface components. Then, in Step S1007, the signal processing unit 428 displays the generated two-dimensional image of θ - z and the generated user interface components, on the LCD monitor 113.

[0088] Here, Fig. 11 illustrates an example of a user interface displayed on a screen of the LCD 113, and the example will be described as follows.

[0089] The reference numeral 1101 illustrated in the drawing represents a window displayed on the screen of the LCD 113. The window 1101 has a region 1102 for displaying the two-dimensional image of the space θ - z , a state region for visually displaying a degree of the malapposition along the z axis and a degree where the stent is covered with vascular tissues, a scroll bar 1104 for scrolling in the z axis direction (in order to deal with a case where the distance of the pull-back processing exceeds the width of the screen), a button 1105 for instructing a change in the opacity conversion curve, an area calculation button 1106, and a distance calculation button 1107.

[0090] It is not necessary to describe the region 1102. The region 1103 displays an occurrence degree of the malapposition along the z axis direction on the two-dimensional image displayed in the region 1102 and the degree where the stent is covered with vascular tissues, and is disposed in order to display the degrees in a one-dimensional manner through multiple stages.

[0091] A degree D of the malapposition is calculated according to the following equation, for example, when as illustrated in Fig. 9, a horizontal direction is set to W , the number of all pixels within a rectangular region 950 defined in all angular regions in a vertical direction is set to N , the number of pixels determined to have the malapposition within the region is set to N_m , and a preset multiplication factor is set to α .

$$D = \alpha \cdot N_m / N$$

In addition, a ratio where the stent is covered with the vascular tissues may be calculated similarly.

[0092] If the opacity conversion curve 1105 is clicked by the mouse 114, the signal processing unit 428 displays a GUI for moving the conversion curve illustrated in Fig. 7 in parallel along the luminance axis in the horizontal direction, thereby enabling a user to freely change the position of the conversion curve. Then, the signal processing unit 428 recalculates and displays the two-dimensional image of θ - z in accordance with the changed conversion curve. For example, when the conversion curve 700 in Fig. 7 is moved in parallel to the right side,

the opacity from the vascular lumen surface to a certain degree depth is set to a_{min} . Accordingly, a deeper layer is displayed as the vascular lumen surface.

[0093] The area calculation button 1106 is disposed in order to calculate an actual area of the vascular lumen surface when a user draws a closed curve within the illustrated region 1102. In the embodiment, the vertical axis is θ , which is different from an axis in the three-dimensional space visible to humans. Accordingly, even when the closed curve is drawn within the region 1102 by the mouse 114, it is difficult to estimate the actual area of the vascular lumen surface, based on the drawn result. Therefore, in the embodiment, after the button 1106 is clicked, the signal processing unit 428 obtains an actual three-dimensional position by projecting each pixel value connecting line segments when the closed curve including any optional position in the region 1102 is drawn, to a three-dimensional model. This processing is performed for each pixel position so as to determine multiple pixel positions for defining the closed curve in the actual three-dimensional space. Thereafter, the signal processing unit 428 calculates the area, and displays the result on the screen.

[0094] The distance calculation button 1107 is disposed to display a distance in such a way that a user designates two desired points within the illustrated region 1102, the two points are projected to the three-dimensional model representing the actual vascular lumen surface, and the distance between the two projected points is calculated.

[0095] Hitherto, the embodiment has been described. However, the present invention is not limited to the above-described embodiment. For example, in the embodiment, the pixel value representing the vascular tissues is corrected so as to visually display the presence or absence of the malapposition, whether or not the stent is covered with the vascular tissues. However, a correction-targeted pixel may be a pixel belonging to the stent. In addition, without being limited to the broken thick line, the solid line, and broken thin line, display forms may be displayed by colors. In addition, in particular, the malapposition may be displayed at multiple stage levels depending on the distance between the rear surface of the stent and the vascular lumen surface. In a case of the multiple stage display, a degree of the malapposition may be displayed by using a color density. The thickness when the stent is covered with the vascular tissues may also be displayed in this manner.

[0096] As is understood from the above-described embodiment, processing for the reconfiguration of the cross-sectional image and the two-dimensional reconfiguration are performed by the signal processing unit 428 configured to have a microprocessor. The microprocessor executes a program so as to realize a function thereof. Accordingly, the program is also included within the scope of the present invention, as a matter of course. In addition, the program is generally stored in a computer-readable storage medium such as a CD-ROM, a DVD-ROM, or

the like. The computer-readable storage medium is set in a reading device (CD-ROM drive or the like) included in a computer. The program can be executed by being copied to or installed in a system. Therefore, it is apparent that the related computer-readable storage medium is also included within the scope of the present invention.

[0097] Without being limited to the above-described embodiment, the present invention can be changed and modified in various ways without departing from the scope of the present invention as defined in the claims.

Claims

1. An imaging apparatus for diagnosis (100) adapted to reconfigure a three-dimensional image of a blood vessel including a probe (101) adapted to emit light toward a vascular lumen surface, said probe (101) accommodating an imaging core (220) adapted to detect reflection light therefrom, to move the imaging core (220) along the probe (101) at a predetermined speed while the imaging core (220) is rotated, the apparatus comprising:

deriving means adapted to derive line data configured to include multiple luminance values arrayed side by side in a radial direction from the rotation center of the imaging core (220) per each rotation angle (θ) in the rotation, based on data obtained by the imaging core (220) during a period while the imaging core (220) is rotated and moved;

calculation means adapted to calculate a two-dimensional image data in which θ , z are set to two axes, by calculating a representative pixel value $P(\theta, z)$ in a viewing direction toward the radial direction from the rotation center of the imaging core (220) in each line data $L(\theta, z)$, when the rotation angle (θ) of the imaging core (220) is defined as θ and the line data at a movement position z in the movement is defined as $L(\theta, z)$; and

display means adapted to display the calculated two-dimensional image data, the calculation means further including: generation means adapted to generate three-dimensional model data of the blood vessel, based on each line data obtained by the deriving means;

discrimination means adapted to discriminate whether or not each line data obtained by the deriving means is line data indicating a stent indwelling the blood vessel; **characterized in that** the calculation means further includes:

specifying means adapted to specify a portion where a malapposition having a predetermined threshold value or greater is present between a vascular lumen surface and a surface of the stent opposing the vascular lumen surface,

- based on the discrimination result obtained by the discrimination means, the three-dimensional model data obtained by the generation means, and a preset thickness d of the stent; representative pixel value calculation means adapted to calculate the representative pixel value of the line data by converting a luminance value of each line data into a value indicating opacity using a preset conversion function, and by continuously adding the value indicating the opacity of a luminance value along the radial direction from the center position of the rotation; and correction means adapted to correct a pixel value corresponding to a portion specified by the specifying means within image data configured to have the representative pixel value calculated by the representative pixel value calculation means, and to generate the two-dimensional image data for highlighting the portion where the malapposition is present.
2. The imaging apparatus for diagnosis (100) according to Claim 1, wherein the conversion function is a function which has a conversion curve in a shape of linearly connecting the minimum opacity in a case of two preset luminance values IL or smaller, the maximum opacity in a case of a luminance value IH greater than the luminance value IL or greater, and the minimum opacity and the maximum opacity between the luminance values IL and IH .
 3. The imaging apparatus for diagnosis (100) according to Claim 2, further comprising: means for moving the conversion curve in parallel along the luminance axis in response to a user's instruction.
 4. The imaging apparatus for diagnosis (100) according to any one of Claims 1 to 3, wherein the specifying means further specifies a portion where the stent is covered with vascular tissues, and in which a relationship satisfies $L0 > L1$ between a distance $L0$ between the imaging core (220) and the surface of the stent and a distance $L1$ between the imaging core (220) in the vicinity of a measurement position of the distance $L0$ and the vascular lumen surface, based on the discrimination result obtained by the discrimination means, and the correction means corrects a pixel of the portion where the stent is covered with the vascular tissues specified by the specifying means within the image data configured to have the representative pixel value calculated by the representative pixel value calculation means.
 5. The imaging apparatus for diagnosis (100) accord-

ing to Claim 4, further comprising:

means for generating a guide image indicating a ratio of the malapposition present at each position in the z axis of the two-dimensional image, and a ratio of the stent covered with the vascular tissues, wherein the display means displays the two-dimensional image data and the guide image in parallel with each other along the z axis.

6. The imaging apparatus for diagnosis (100) according to any one of Claims 1 to 5, further including an information processing apparatus that generates a three-dimensional image, based on data transmitted from the imaging core (220).

Patentansprüche

1. Bildgebungs Vorrichtung zur Diagnose (100), die zum Rekonfigurieren eines dreidimensionalen Bildes eines Blutgefäßes eingerichtet ist, umfassend eine Sonde (101), die zum Emittieren von Licht in Richtung einer Gefäßlumenfläche eingerichtet ist, wobei die Sonde (101) einen Bildgebungskern (220) aufnimmt, der zum Erfassen von Reflexionslicht von dieser eingerichtet ist, um den Bildgebungskern (220) entlang der Sonde (101) mit einer vorbestimmten Geschwindigkeit zu bewegen, während der Bildgebungskern (220) gedreht wird, wobei die Vorrichtung aufweist:

eine Ableitungseinrichtung, die eingerichtet ist, um Liniendaten abzuleiten, welche konfiguriert sind, um mehrere Luminanzwerte zu umfassen, die Seite an Seite in einer radialen Richtung von dem Rotationszentrum des Bildgebungskerns (220) pro Rotationswinkel (θ) bei der Rotation angeordnet sind, basierend auf den durch den Bildgebungskern (220) während einer Zeitspanne erhaltenen Daten, während der Bildgebungskern (220) gedreht und bewegt wird;

eine Berechnungseinrichtung, die zum Berechnen zweidimensionaler Bilddaten eingerichtet ist, in denen θ, z für zwei Achsen festgelegt sind, durch Berechnen eines repräsentativen Pixelwerts $P(\theta, z)$ in einer Betrachtungsrichtung in Richtung auf die radiale Richtung von dem Rotationszentrum des Bildgebungskerns (220) in jeden Liniendaten $L(\theta, z)$, wenn der Rotationswinkel (θ) des Bildgebungskerns (220) als θ definiert ist und die Liniendaten an einer Bewegungsposition z in der Bewegung als $L(\theta, z)$ definiert sind; und

eine Anzeigeeinrichtung, die eingerichtet ist, um die berechneten zweidimensionalen Bilddaten anzuzeigen,

wobei die Berechnungseinrichtung ferner umfasst:

eine Erzeugungseinrichtung, die eingerichtet ist, um dreidimensionale Modelldaten des Blutgefäßes basierend auf jeden durch die Ableitungseinrichtung erhaltenen Liniendaten zu erzeugen;
eine Unterscheidungseinrichtung, die eingerichtet ist, um zu unterscheiden, ob oder ob nicht jede Liniendaten, die durch die Ableitungseinrichtung erhalten werden, Liniendaten sind, die einen Stent anzeigen, der in dem Blutgefäß verweilt;

dadurch gekennzeichnet, dass die Berechnungseinrichtung ferner umfasst:

eine Spezifizierungseinrichtung, die eingerichtet ist, um einen Abschnitt zu spezifizieren, wo eine Malapposition mit einem vorbestimmten Schwellenwert oder größer zwischen einer Gefäßlumenfläche und einer Oberfläche des Stents, die der Gefäßlumenfläche gegenüberliegt, vorliegt, basierend auf dem Unterscheidungsergebnis, das durch die Unterscheidungseinrichtung erhalten wird, den dreidimensionalen Modelldaten, die durch die Erzeugungseinrichtung erhalten werden, und einer voreingestellten Dicke d des Stents;
eine Berechnungseinrichtung für repräsentative Pixelwerte, die eingerichtet ist zum Berechnen des repräsentativen Pixelwerts der Liniendaten durch Umwandeln eines Luminanzwertes von jeden Liniendaten in einen Wert, der eine Opazität anzeigt, unter Verwendung einer voreingestellten Konvertierungsfunktion und durch kontinuierliches Addieren des Wertes, der die Opazität eines Luminanzwertes entlang der radialen Richtung von der zentralen Position der Rotation anzeigt; und
eine Korrekturereinrichtung, die zum Korrigieren eines Pixelwerts eingerichtet ist, der einem durch die Spezifizierungseinrichtung innerhalb der Bilddaten spezifizierten Abschnitt entspricht, die konfiguriert ist, den durch die Berechnungseinrichtung für repräsentative Pixelwerte berechneten repräsentativen Pixelwert aufzuweisen und die zweidimensionalen Bilddaten zum Hervorheben des Abschnitts, wo die Malapposition vorhanden ist, zu erzeugen.

2. Bildgebungsvorrichtung zur Diagnose (100) nach Anspruch 1, wobei die Umwandlungsfunktion eine Funktion ist, die eine

Konversionskurve in einer Form aufweist, in der die minimale Opazität in einem Fall von zwei voreingestellten Luminanzwerten IL oder kleiner, die maximale Opazität in einem Fall eines Luminanzwerts IH größer als der Luminanzwert IL oder größer und die minimale Opazität und die maximale Opazität zwischen den Luminanzwerten IL und IH linear verbunden sind.

3. Bildgebungsvorrichtung zur Diagnose (100) nach Anspruch 2, ferner umfassend:
eine Einrichtung zum parallelen Bewegen der Konversionskurve entlang der Luminanzachse als Antwort auf eine Benutzeranweisung.
4. Bildgebungsvorrichtung zur Diagnose (100) nach einem der Ansprüche 1 bis 3, wobei die Spezifizierungseinrichtung ferner einen Abschnitt spezifiziert, in dem der Stent mit vaskulärem Gewebe bedeckt ist und in dem eine Beziehung $L0 > L1$ zwischen einem Abstand $L0$ zwischen dem Bildgebungskern (220) und der Oberfläche des Stents und einem Abstand $L1$ zwischen dem Bildgebungskern (220) in der Nähe einer Messposition des Abstandes $L0$ und der Oberfläche des Gefäßlumens erfüllt ist, basierend auf dem Unterscheidungsergebnis, das durch die Unterscheidungseinrichtung erhalten wird, und die Korrekturereinrichtung ein Pixel des Abschnitts korrigiert, in welchem der Stent mit dem durch die Spezifizierungseinrichtung innerhalb der Bilddaten spezifizierten vaskulären Gewebe bedeckt ist, die so konfiguriert ist, dass sie den repräsentativen Pixelwert aufweist, der von der Berechnungseinrichtung für repräsentative Pixelwerte berechnet wurde.
5. Bildgebungsvorrichtung zur Diagnose (100) nach Anspruch 4, ferner umfassend:
eine Einrichtung zum Erzeugen eines Führungsbildes, das einen Anteil der Malapposition, die an jeder Position in der z-Achse des zweidimensionalen Bildes vorhanden ist, und einen Anteil des Stents, der mit dem vaskulären Gewebe bedeckt ist, anzeigt, wobei die Anzeigeeinrichtung die zweidimensionalen Bilddaten und das Führungsbild parallel zueinander entlang der z-Achse anzeigt.
6. Bildgebungsvorrichtung zur Diagnose (100) nach einem der Ansprüche 1 bis 5, ferner umfassend eine Informationsverarbeitungsvorrichtung, die ein dreidimensionales Bild basierend auf Daten erzeugt, die von dem Kern (220) übertragen werden.

Revendications

1. Appareil d'imagerie diagnostique (100) conçu pour

reconfigurer une image tridimensionnelle d'un vaisseau sanguin, comportant une sonde (101) conçue pour émettre de la lumière vers une surface de lumen vasculaire, ladite sonde (101) logeant un coeur d'imagerie (220) conçu pour détecter de la lumière réfléchiée par ladite surface, pouvant déplacer le coeur d'imagerie (220) le long de la sonde (101) à une vitesse prédéterminée tout en mettant le coeur d'imagerie (220) en rotation, l'appareil comprenant :

un moyen de dérivation conçu pour dériver des données de lignes configurées pour comprendre de multiples valeurs de luminance alignées côte à côte dans une direction radiale à partir du centre de rotation du coeur d'imagerie (220) pour chaque angle de rotation (θ) au cours de la rotation, sur la base de données obtenues par le coeur d'imagerie (220) durant une période pendant laquelle le coeur d'imagerie (220) est mis en rotation et déplacé ;

un moyen de calcul conçu pour calculer des données d'une image bidimensionnelle dans laquelle θ , z sont reportés sur deux axes, par calcul d'une valeur de pixel représentative $P(\theta, z)$ dans une direction de visualisation dans la direction radiale à partir du centre de rotation du coeur d'imagerie (220) dans les données $L(\theta, z)$ de chaque ligne, quand l'angle de rotation (θ) du coeur d'imagerie (220) est noté θ et les données d'une ligne au niveau d'une position de déplacement z dans le déplacement sont notées $L(\theta, z)$; et

un moyen d'affichage conçu pour afficher les données de l'image bidimensionnelle calculées, le moyen de calcul comprenant en outre :

un moyen de génération conçu pour générer des données de modèle tridimensionnel du vaisseau sanguin, sur la base des données de chaque ligne obtenues par le moyen de dérivation ;

un moyen de distinction conçu pour distinguer si les données de chaque ligne obtenues par le moyen de dérivation sont ou ne sont pas des données de ligne indiquant un stent à demeure dans le vaisseau sanguin ;

caractérisé en ce que le moyen de calcul comprend en outre :

un moyen de spécification conçu pour spécifier une partie où une malapposition ayant une valeur seuil prédéterminée ou plus est présente entre une surface de lumen vasculaire et une surface du stent en regard de la surface de lumen vasculaire, sur la base du résultat de distinction obtenu par le moyen de distinction, des données de mo-

dèle tridimensionnel obtenues par le moyen de génération, et d'une épaisseur prédéfinie d du stent ;

un moyen de calcul de valeur de pixel représentative conçu pour calculer la valeur de pixel représentative des données de ligne par conversion d'une valeur de luminance des données de chaque ligne en une valeur indiquant une opacité à l'aide d'une fonction de conversion prédéfinie, et par somme continue de la valeur indiquant l'opacité d'une valeur de luminance le long de la direction radiale à partir de la position du centre de rotation ; et

un moyen de correction conçu pour corriger une valeur de pixel correspondant à une partie spécifiée par le moyen de spécification dans des données d'image configurées pour avoir la valeur de pixel représentative calculée par le moyen de calcul de valeur de pixel représentative, et pour générer les données de l'image bidimensionnelle de manière à mettre en évidence la partie où la malapposition est présente.

2. Appareil d'imagerie diagnostique (100) selon la revendication 1, dans lequel :

la fonction de conversion est une fonction qui a une courbe de conversion dont la forme relie linéairement l'opacité minimale dans le cas de deux valeurs de luminance prédéfinies IL ou moins, l'opacité maximale dans le cas d'une valeur de luminance IH supérieure à la valeur de luminance IL ou plus, et l'opacité minimale et l'opacité maximale entre les valeurs de luminance IL et IH .

3. Appareil d'imagerie diagnostique (100) selon la revendication 2, comprenant en outre :

un moyen pour déplacer la courbe de conversion parallèlement le long de l'axe de luminance en réponse à une instruction de l'utilisateur.

4. Appareil d'imagerie diagnostique (100) selon l'une quelconque des revendications 1 à 3, dans lequel :

le moyen de spécification spécifie en outre une partie où le stent est couvert par des tissus vasculaires, et dans laquelle une relation $L0 > L1$ est satisfaite entre une distance $L0$ entre le coeur d'imagerie (220) et la surface du stent et une distance $L1$ entre le coeur d'imagerie (220) au voisinage d'une position de mesure de la distance $L0$ et la surface de lumen vasculaire, sur la base du résultat de distinction obtenu par le moyen de distinction, et

le moyen de correction corrige un pixel de la partie où le stent est couvert par les tissus vasculaires, spécifiée par le moyen de spécification,

dans les données d'image configurées pour avoir la valeur de pixel représentative calculée par le moyen de calcul de valeur de pixel représentative.

5

5. Appareil d'imagerie diagnostique (100) selon la revendication 4, comprenant en outre :

un moyen pour générer une image de guidage indiquant une proportion de la malapposition présente à chaque position suivant l'axe z de l'image bidimensionnelle, et une proportion du stent couvert par les tissus vasculaires, dans lequel

10

le moyen d'affichage affiche les données de l'image bidimensionnelle et l'image de guidage en parallèle le long de l'axe z.

15

6. Appareil d'imagerie diagnostique (100) selon l'une quelconque des revendications 1 à 5, comprenant en outre un appareil de traitement d'informations qui génère une image tridimensionnelle, sur la base de données transmises à partir du coeur d'imagerie (220).

20

25

30

35

40

45

50

55

FIG. 1

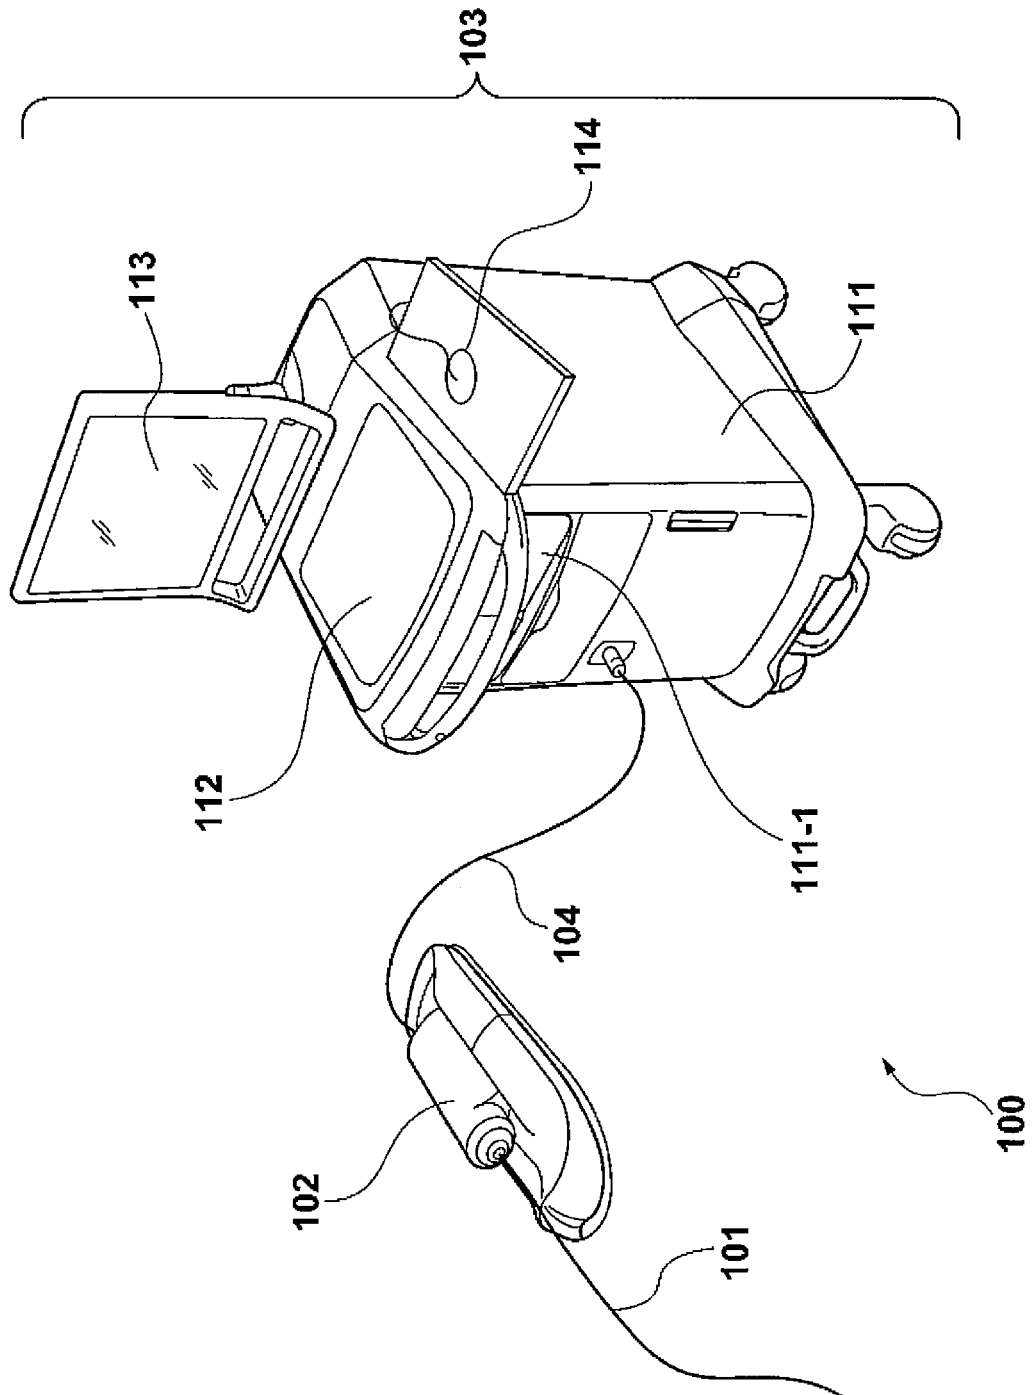


FIG. 2

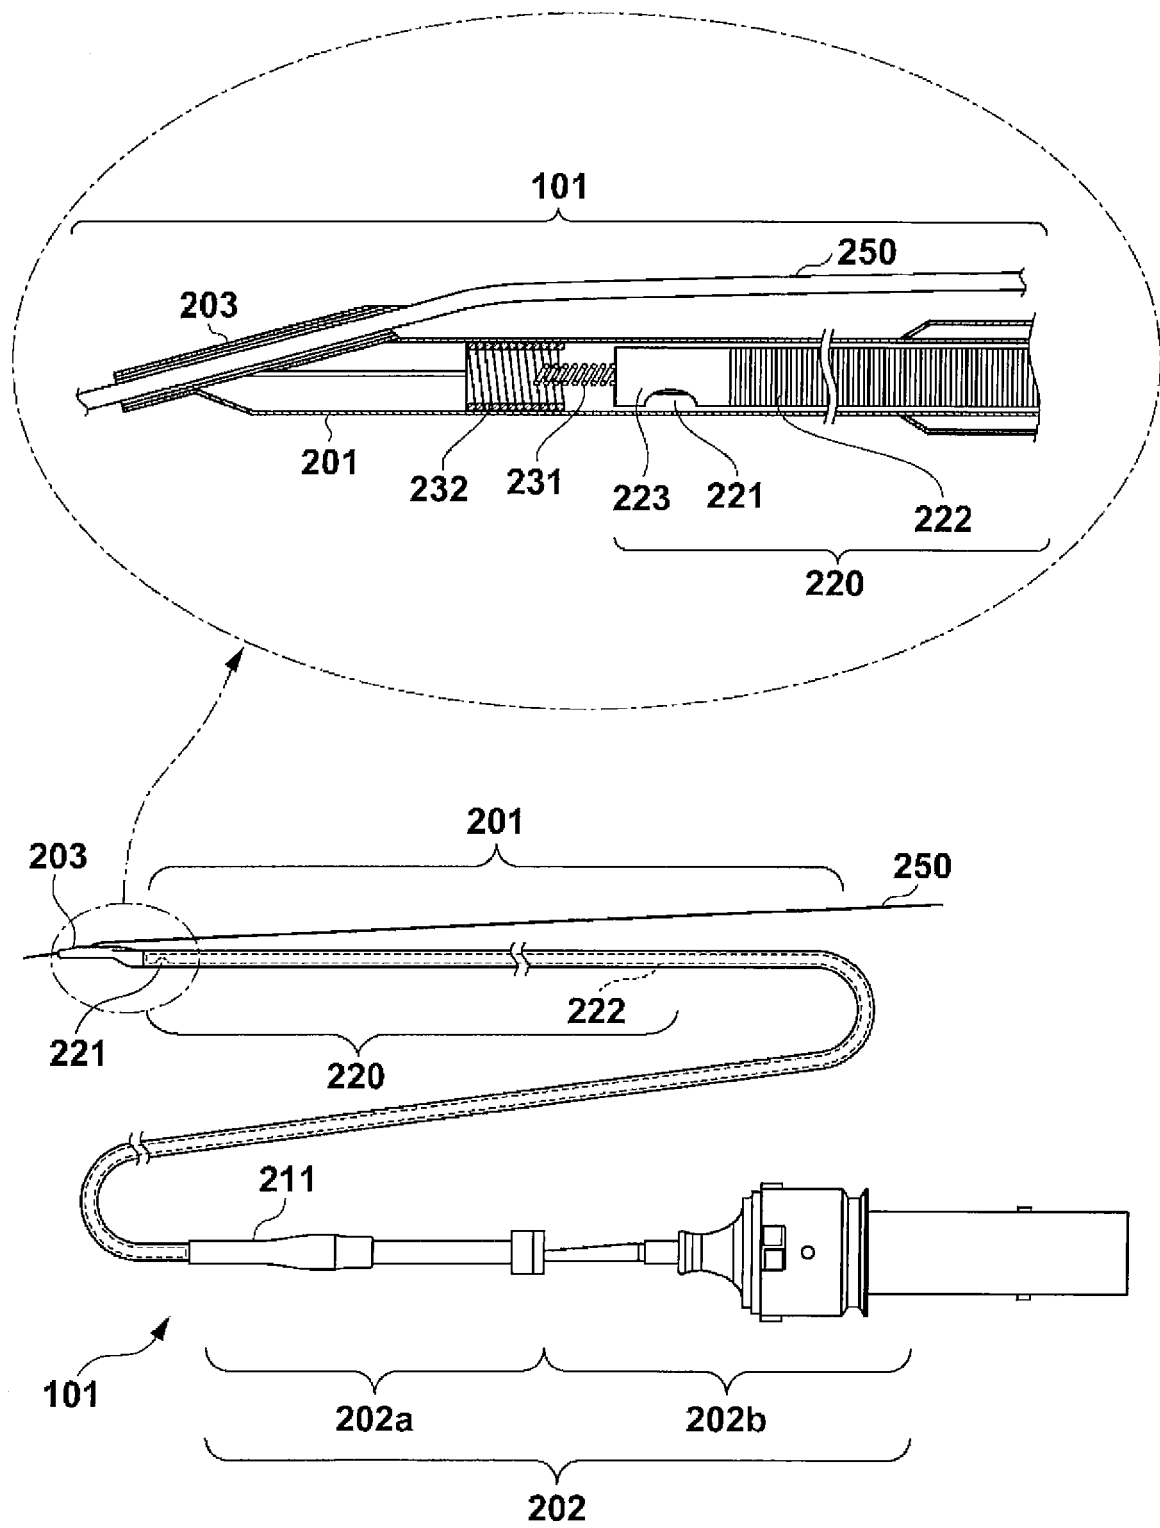


FIG. 3

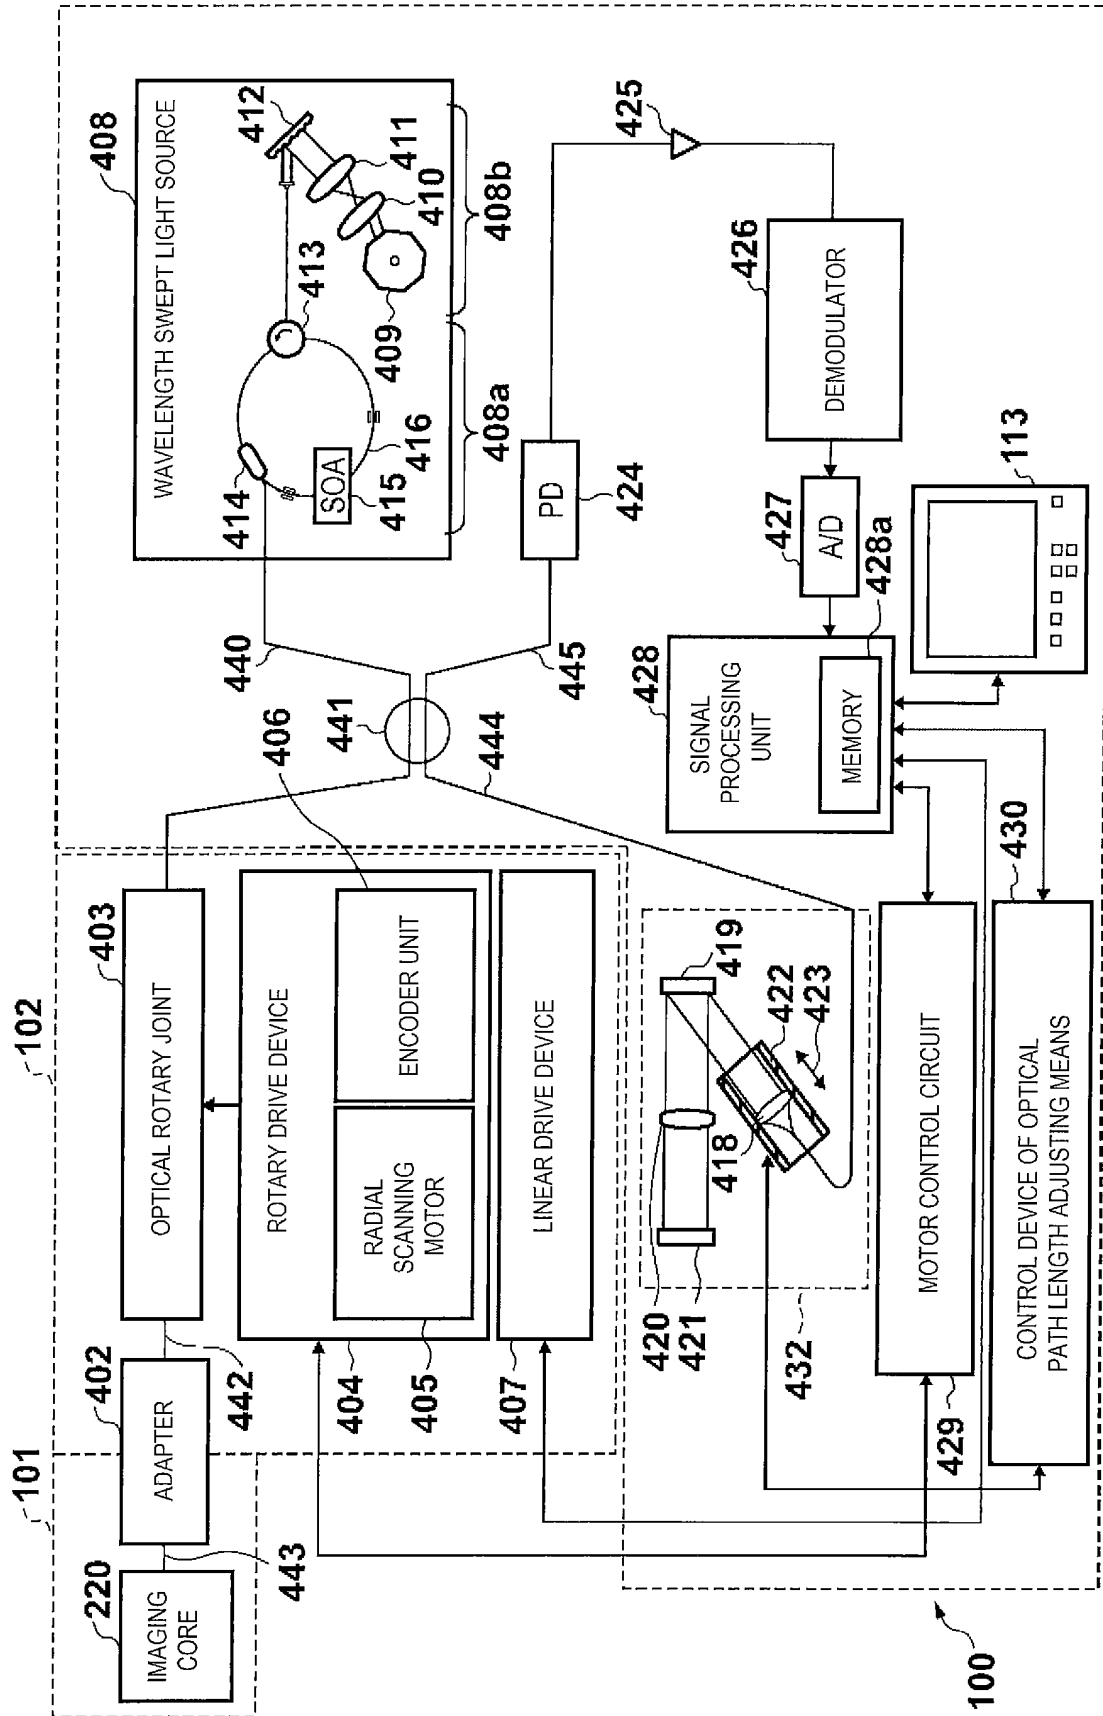


FIG. 4

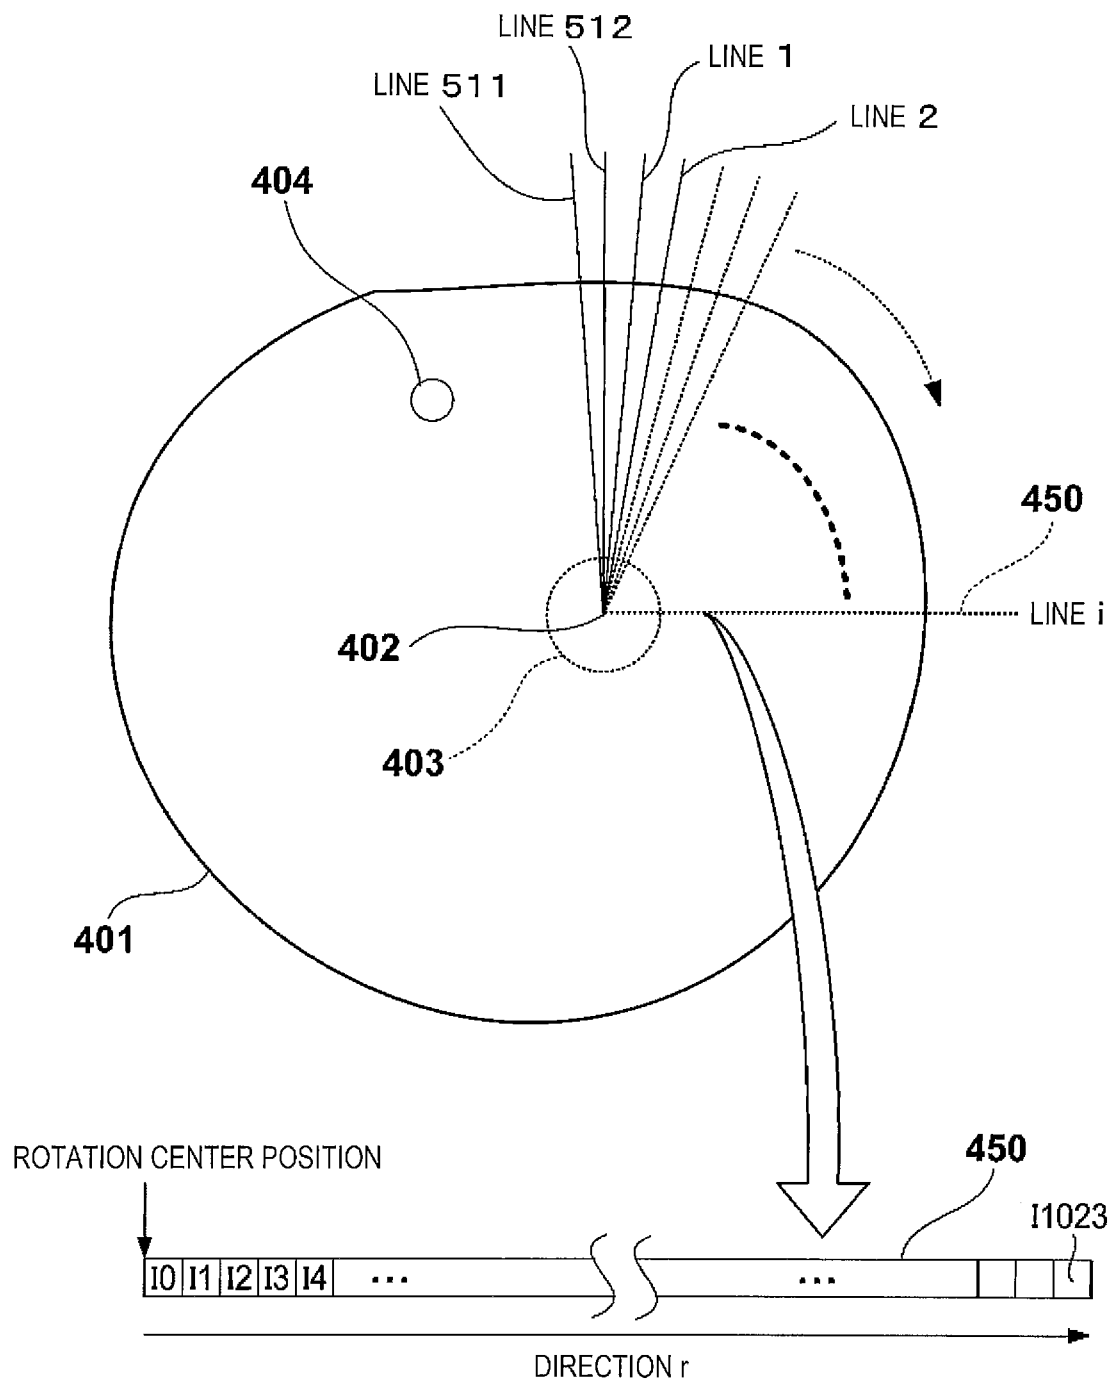


FIG. 5

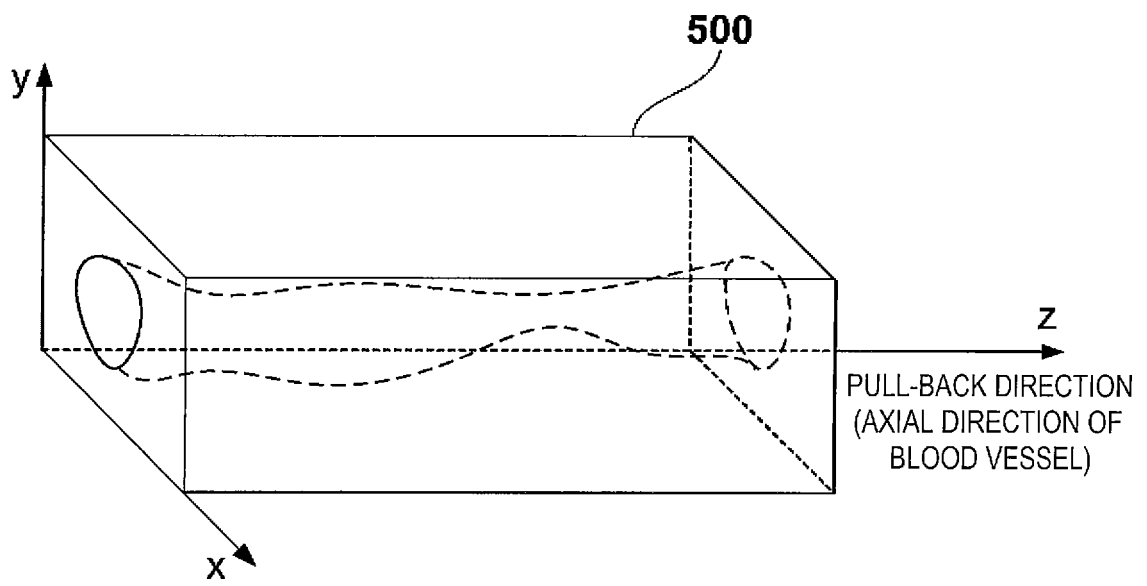


FIG. 6

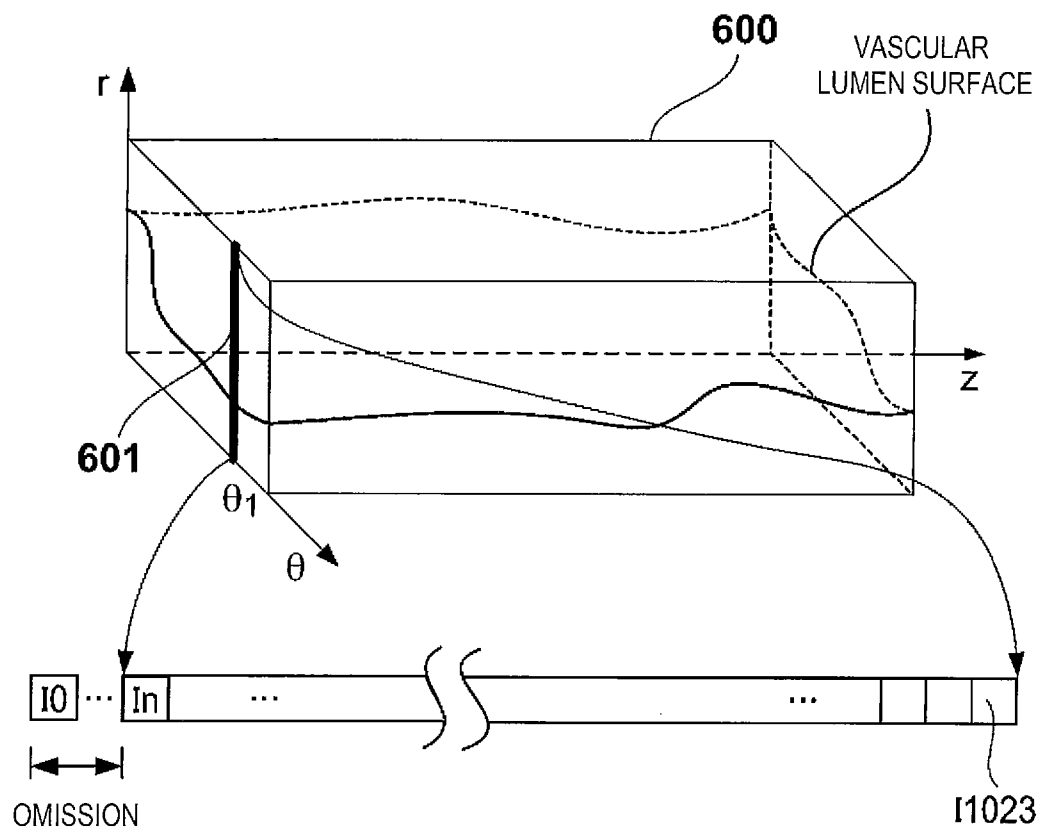


FIG. 7

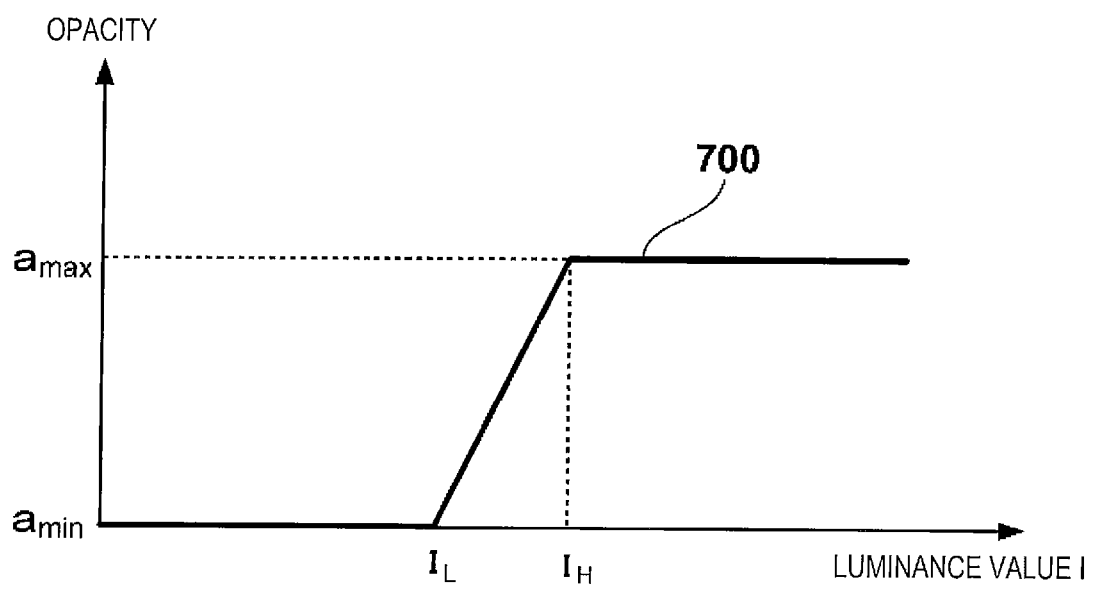


FIG. 8

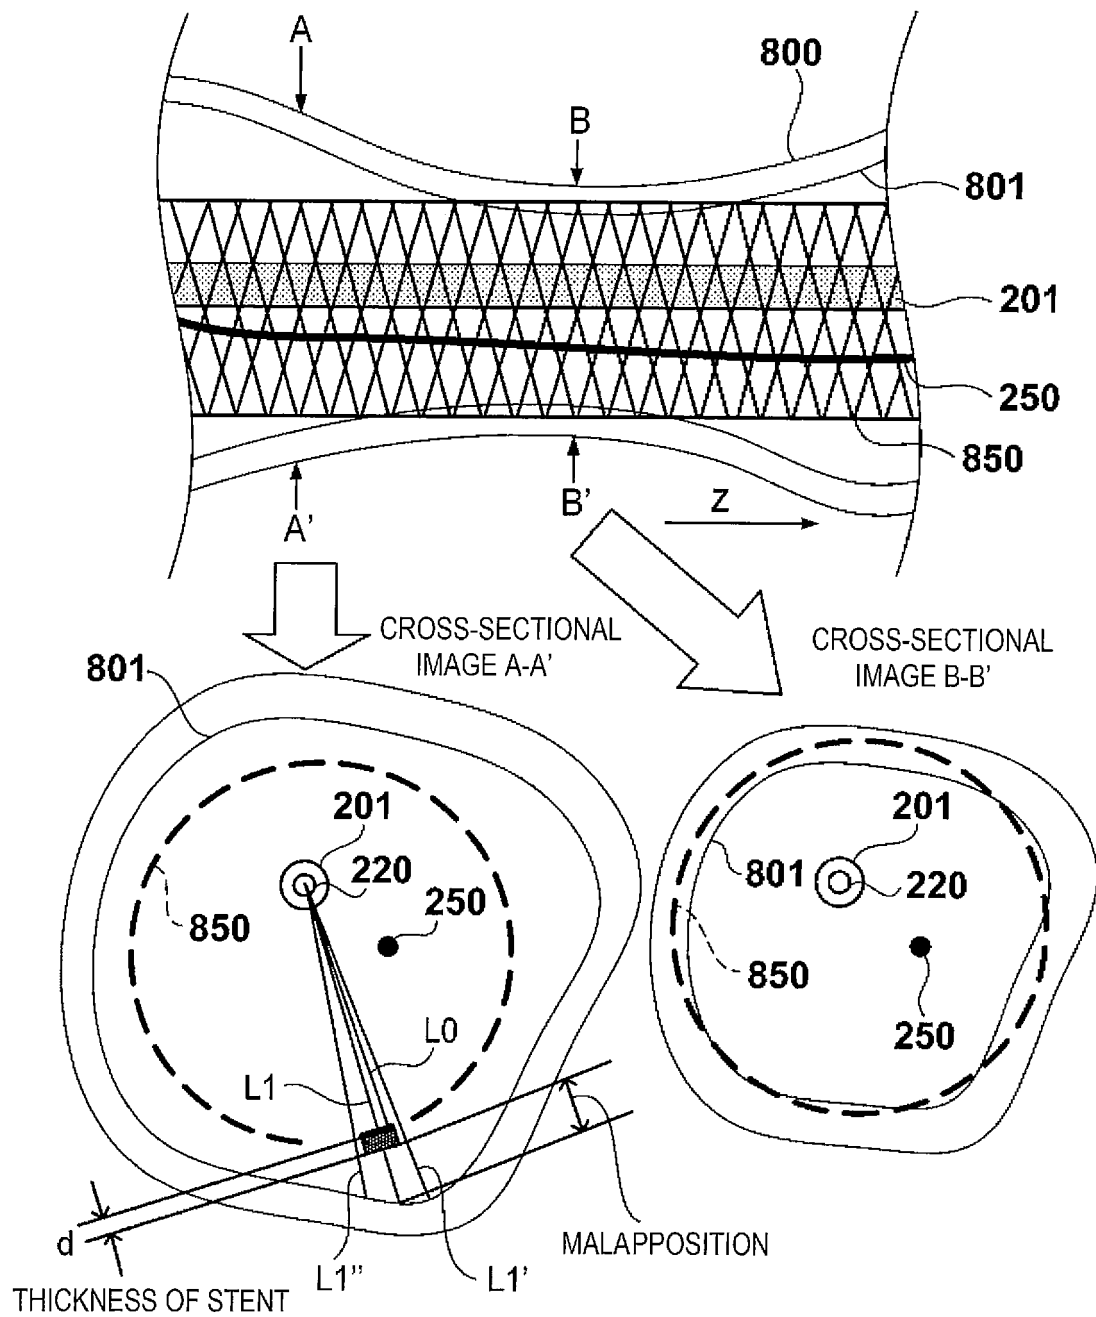


FIG. 9

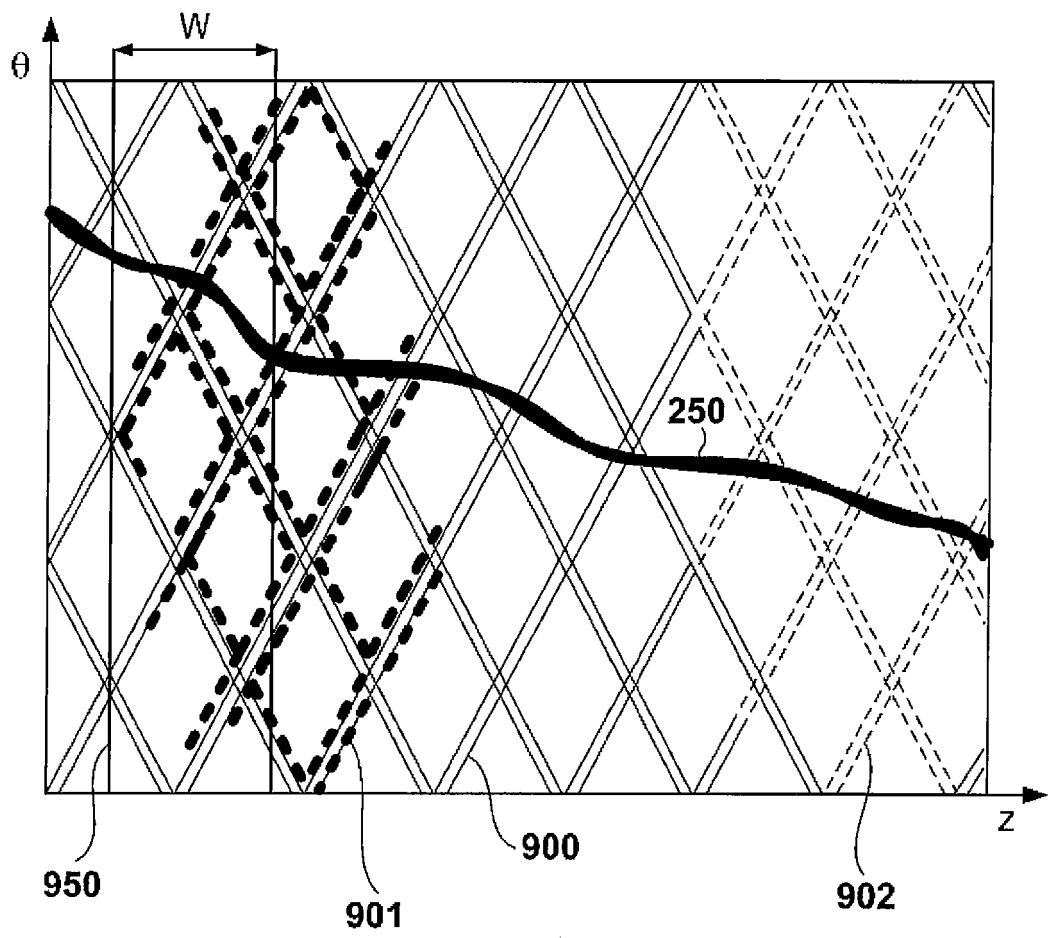


FIG. 10


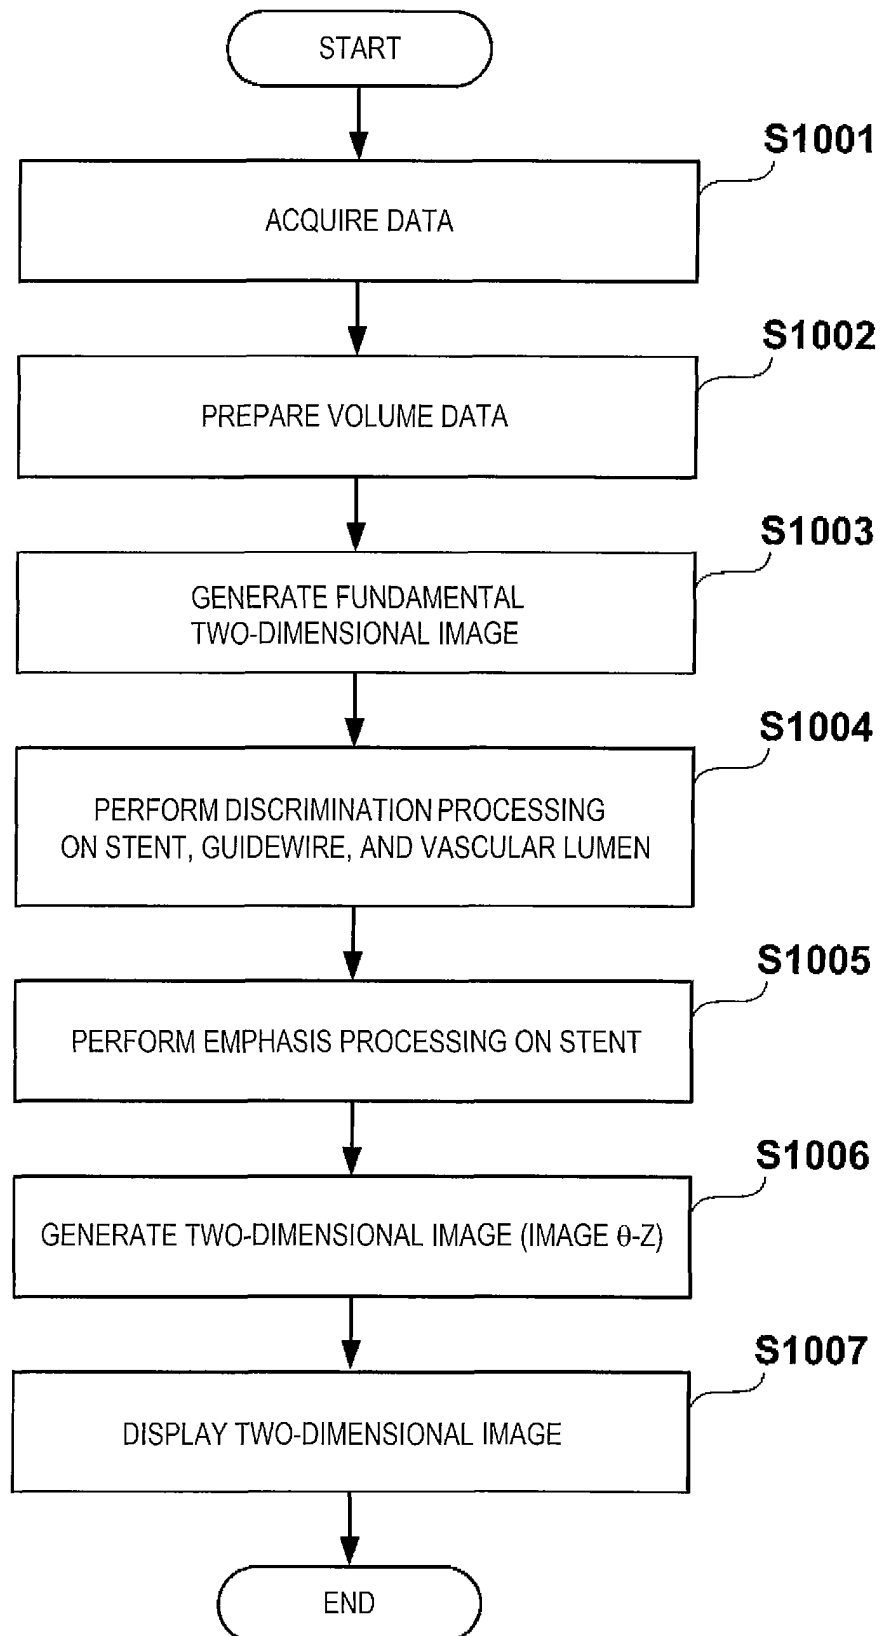


FIG. 11

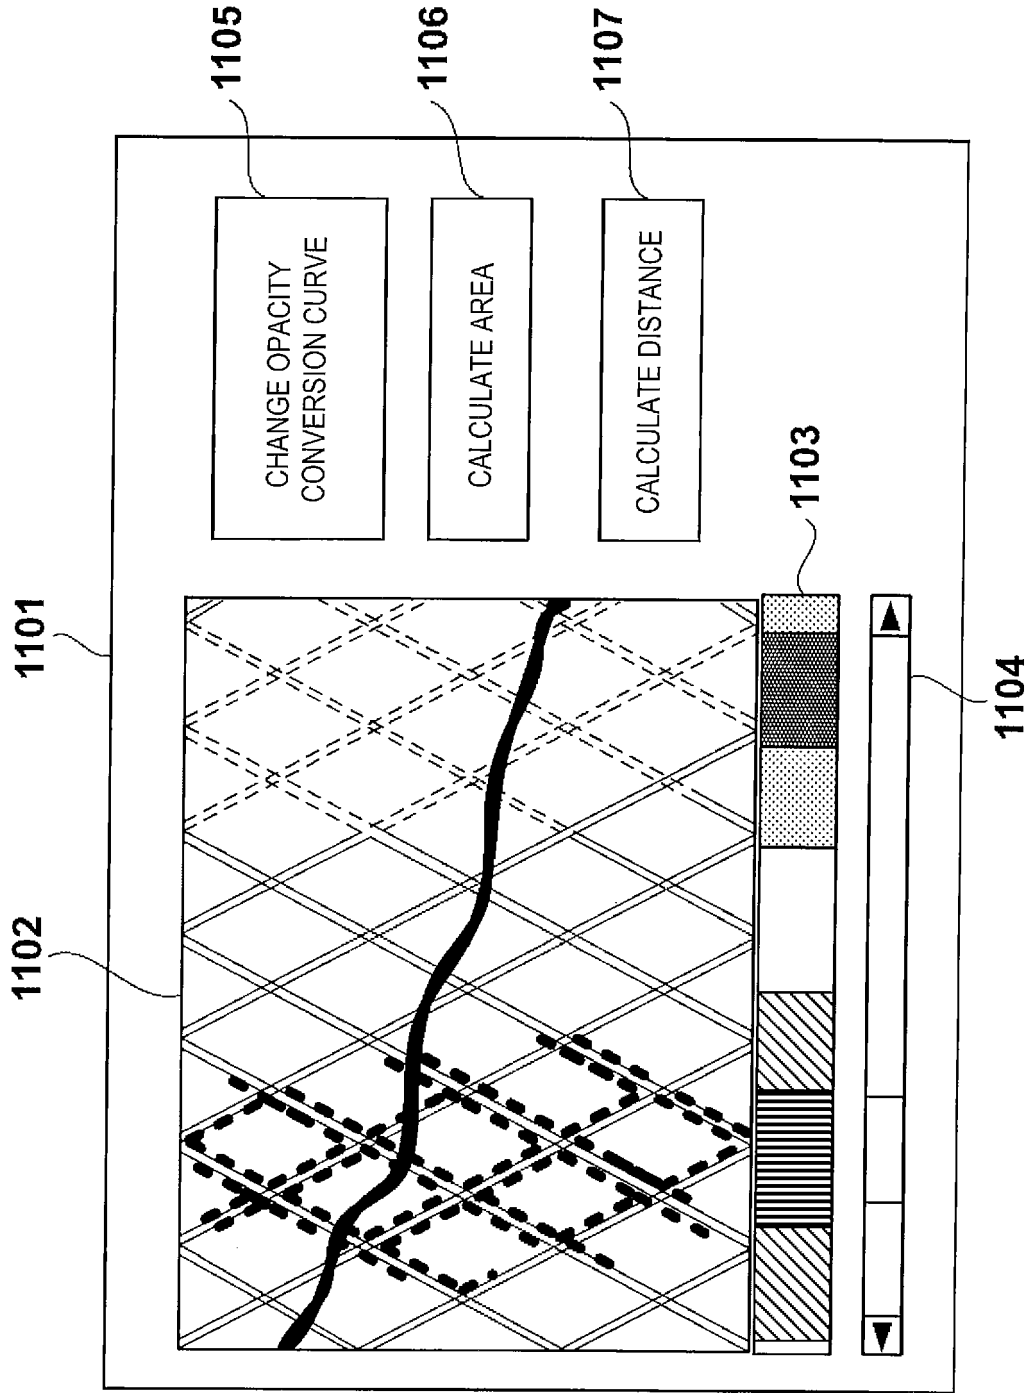

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 2010094127 A1 [0003]
- JP 2007267867 A [0004]

专利名称(译)	图像诊断装置和信息处理装置		
公开(公告)号	EP2949259B1	公开(公告)日	2018-06-27
申请号	EP2013873103	申请日	2013-01-23
[标]申请(专利权)人(译)	泰尔茂株式会社		
申请(专利权)人(译)	泰尔茂株式会社		
当前申请(专利权)人(译)	泰尔茂株式会社		
[标]发明人	FURUICHI JUNYA INOUE KOUICHI ETOU HIJIRI		
发明人	FURUICHI, JUNYA INOUE, KOUICHI ETOU, HIJIRI		
IPC分类号	A61B1/00 A61B5/00 A61B5/02 G06T7/00 G06T11/00		
CPC分类号	A61B1/00009 A61B5/0066 A61B5/0084 A61B5/06 A61B2576/02 G16H30/40 A61B5/02007 A61B5/6852 A61B5/742 G06T7/0002 G06T11/003 G06T2207/10072 G06T2207/30101 G06T2211/40		
其他公开文献	EP2949259A1 EP2949259A4		
外部链接	Espacenet		

摘要(译)

本发明从成像芯的旋转中心位置获取由径向方向上的多个亮度值表示的线数据，所述旋转中心位置是由成像芯的旋转位置和移动导出的。然后，基于所获取的线数据，生成并显示二维空间的图像，在该二维空间中，表示旋转角度的 θ 和表示移动方向上的位置的 z 被设置为两个轴。

