

(19)



(11)

EP 3 111 840 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
19.06.2019 Bulletin 2019/25

(21) Application number: **15755345.4**

(22) Date of filing: **27.02.2015**

(51) Int Cl.:
A61B 5/11 (2006.01) A61B 5/00 (2006.01)

(86) International application number:
PCT/JP2015/055928

(87) International publication number:
WO 2015/129883 (03.09.2015 Gazette 2015/35)

(54) **DEVICE FOR DETECTING AMBULATORY STATUS**

VORRICHTUNG ZUR ERKENNUNG EINES AMBULANTEN ZUSTANDS

DISPOSITIF DE DÉTECTION D'ÉTAT AMBULATOIRE

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

(30) Priority: **28.02.2014 JP 2014039341**

(43) Date of publication of application:
04.01.2017 Bulletin 2017/01

(73) Proprietors:
• **MicroStone Corporation**
Nagano 389-0202 (JP)
• **Ichikawa, Akira**
Saku-shi, Nagano 385-0016 (JP)

(72) Inventors:
• **ICHIKAWA, Akira**
Saku-shi
Nagano 385-0016 (JP)
• **SHIRATORI, Norihiko**
Saku-shi
Nagano 385-0007 (JP)
• **OKADA, Shigeya**
Saku-shi
Nagano 385-0007 (JP)
• **NOZAWA, Hidetaka**
Saku-shi
Nagano 385-0007 (JP)

(74) Representative: **Mewburn Ellis LLP**
City Tower
40 Basinghall Street
London EC2V 5DE (GB)

(56) References cited:
JP-A- 2008 307 207 JP-A- 2009 106 377
JP-A- 2009 106 391 JP-A- 2010 193 977
JP-A- 2012 024 449 JP-A- 2014 504 932
US-A- 5 146 929 US-A1- 2009 030 345
US-A1- 2012 101 771

- **SMEATHERS ET AL: "Measurement of transmissibility for the human spine during walking and running", CLINICAL BIOMECHANICS, BUTTERWORTH SCIENTIFIC LTD, GUILDFORD, GB, vol. 4, no. 1, 1 February 1989 (1989-02-01), pages 34-40, XP026177986, ISSN: 0268-0033, DOI: 10.1016/0268-0033(89)90065-X [retrieved on 1989-02-01]**
- **JUNG KEUN LEE ET AL: "3D spinal motion analysis during staircase walking using an ambulatory inertial and magnetic sensing system", MEDICAL & BIOLOGICAL ENGINEERING & COMPUTING, SPRINGER, BERLIN, DE, vol. 49, no. 7, 27 January 2011 (2011-01-27), pages 755-764, XP019919631, ISSN: 1741-0444, DOI: 10.1007/S11517-011-0738-Y**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 3 111 840 B1

Description**FIELD OF TECHNOLOGY**

[0001] The present invention relates to a device for detecting an ambulatory status of a subject.

BACKGROUND TECHNOLOGY

[0002] In case of analyzing an ambulatory status, moving images, which have been photographed by a high speed camera, etc., are usually analyzed.

[0003] However, there are some problems, e.g., the high speed camera being expensive, a measuring range being limited within several meters square, a method for analyzing moving images being complex.

[0004] On the other hand, another conventional method for analyzing an ambulatory status by using motion sensors, e.g., acceleration sensors, without photographing moving images, has been developed.

[0005] For example, in a method for analyzing an ambulatory status disclosed in Patent Document 1, a plurality of sensors are provided to a hip joint between both feet and provided to knee joints and foot joints in a state where the joints are pinched between the sensors, so that walking data, e.g., joint angles, of a subject can be obtained on the basis of data from the sensors.

[0006] Further, in a walking evaluation device disclosed in Patent Document 2, acceleration sensors are attached to ankle parts of a subject, and frequency spectra of acceleration signals are analyzed on the basis of the acceleration data of the ankle parts measured by the acceleration sensors, so that ambulatory statuses, e.g., shuffling, sliding, can be evaluated.

[0007] Further, in a walking posture determination apparatus disclosed in Patent Document 3, acceleration sensors are used to monitor ambulatory status of a patient.

PRIOR ART DOCUMENT**PATENT DOCUMENT****[0008]**

Patent Document 1: Japanese Laid-open Patent Publication No. 2012-343

Patent Document 2: Japanese Laid-open Patent Publication No. 2013-59489

Patent Document 3: US 2012/101771

DISCLOSURE OF THE INVENTION**PROBLEMS TO BE SOLVED BY THE INVENTION**

[0009] In the above described conventional analyzing method and device, number of steps and walking cycles (walking pitches) can be easily measured. However, con-

ditions of movement of a trunk of the subject while walking cannot be precisely analyzed.

[0010] Note that, in a rehabilitation facility, a physical therapist visually observes an ambulatory status of a subject and instructs the subject on the basis of the ambulatory status. When instructing the subject, the physical therapist attentions not only a lower body trunk, e.g., lower lumbar vertebrae, near sacral bone, but also magnitude and balance of the movement.

[0011] However, the physical therapist needs a lot of experiences to analyze the ambulatory status on the basis of not only movements of limbs but also movements of the upper and lower body trunks, so it is difficult to perform such analysis. Therefore, there is a problem of providing a method and a device for easily analyzing an ambulatory status including a movement of an upper body.

[0012] Thus, the present invention is invented to solve the above described problems, and an object of the present invention is to provide a device for easily detecting an ambulatory status including a movement of an upper body, without complex operation of equipment, in a medical facility, e.g., rehabilitation facility.

MEANS FOR SOLVING THE PROBLEMS

[0013] To achieve the above described object, the present invention has the following structures.

[0014] The device for detecting ambulatory status of the present invention comprises: a monitor; motion sensors being respectively provided to two places of a subject, i.e., a lumbar area and a thoracodorsal area; means for calculating conditions of movement in said two places on the basis of data measured by the motion sensors; and means for superposing the conditions of movement in said two places, which have been calculated by the calculating means, and displaying the superposed conditions on the monitor.

[0015] With this structure, the conditions of movement of the lumbar area and the thoracodorsal area can be visually observed, so that a proper judgement can be performed without gaining many actual experiences in, for example, a rehabilitation facility.

[0016] In the device, each of the motion sensors is an acceleration sensor and an angular speed sensor.

[0017] In case that the motions sensors are acceleration sensors, the calculating means may extract only vibration components by filtering the data detected by the acceleration sensors, and the extracted vibration components may be integrated so as to calculate any of rocking accelerations, rocking speeds and rocking amounts.

[0018] By extracting only the vibration components from the data detected by the acceleration sensors, walking displacement in a walking direction can be removed, so that the correct ambulatory status can be known.

[0019] In case that the motions sensors are angular speed sensors, the calculating means may extract only vibration components by filtering the data detected by

the angular speed sensors, and the extracted vibration components may be integrated so as to calculate any of rocking accelerations, rocking speeds and rocking amounts.

[0020] By extracting only the vibration components from the data detected by the angular speed sensors, walking displacement in a walking direction can be removed, so that the correct ambulatory status can be known.

[0021] In case that the motions sensors are angular speed sensors, the calculating means may calculate angular speeds from the data detected by the angular speed sensors, or may calculate angles by integrating the data detected by the angular sensors.

[0022] In case that the motions sensors are magnetic sensors, the calculating means may calculate angles from the data detected by the magnetic sensors.

[0023] Further, in the device, the displaying means makes Lissajous figures of said two places, in a horizontal plane, on the basis of any of rocking accelerations, rocking speeds and rocking amounts calculated by the calculating means, and superposes the Lissajous figures of said two places and displays the superposed figures on the monitor.

[0024] With this structure, the ambulatory status of the subject, especially the lumber area and the thoracodorsal area, can be visually confirmed as a highly clear image.

[0025] In the device, each of the motion sensors is constituted by a three-axis acceleration sensor and a three-axis angular speed sensor, the calculating means detects the gravity direction on the basis of the data detected by the three-axis acceleration sensor and calculates angular speeds or angles in the three-dimensional orthogonal coordinate system, i.e., in the gravity direction, a walking direction in a horizontal plane and a left/right direction in the horizontal plane, on the basis of the detected gravity direction, from the data detected by the three-axis acceleration sensors, and the displaying means makes Lissajous figures on the basis of the angular speeds or angles in the gravity direction, the walking direction in the horizontal plane and the left/right direction in the horizontal plane, superposes the Lissajous figures of the motion sensors of said two places in the walking direction in the horizontal plane and the left/right direction in the horizontal plane respectively, and displays the superposed figures on the monitor.

[0026] With this structure, the ambulatory status can be further correctly confirmed.

[0027] In the device, the calculating means may calculate conditions of movement in said two places from a reference posture of the subject being stationary to an ordinary posture of the subject being stationary, and the displaying means may correct the conditions of movement in said two places from the reference posture of the subject to the ordinary posture of the subject being stationary, which have been calculated by the calculating means, and may display the corrected conditions on the monitor when superposing the conditions of movement

in said two places, which have been measured by the motion sensors on the basis of the measured data, and displaying the superposed conditions on the monitor.

[0028] With this structure, a positional relationship between the motion sensors (e.g., position shift, inclination, twisting) can be calculated, so that physical features of the subject other than walking, e.g., shoulder lowering, round shoulders, can be judged. When displaying the conditions of movement while walking, proper judgement for rehabilitation can be performed by further displaying the above described physical features on the monitor.

[0029] Note that, the reference posture means a posture in a state where the two motion sensors are provided on a vertical axial line of the subject, which is located at near the left right center of the subject, and axial directions of the two motion sensors are coincided.

[0030] In the device, the calculating means may calculate positions of the motion sensors with respect to a center axis of the subject along the vertical direction while walking, and the displaying means may correct the positions of the motion sensors, which have been calculated by the calculating means, and may display the corrected positions on the monitor when superposing the conditions of movement in said two places, which have been measured by the motion sensors on the basis of the measured data, and displaying the superposed conditions on the monitor.

[0031] With this structure, the positional relationship between the motion sensors while walking (e.g., position shift, inclination, twisting) can be calculated, so that the physical features of the subject other than walking, e.g., shoulder lowering, round shoulders, can be judged. When displaying the conditions of movement while walking, proper judgement for rehabilitation can be performed by further displaying the above described physical features on the monitor.

[0032] In the device, the displaying means may display a connection line, which connects same time points in the Lissajous figures of the motion sensors of said two places to each other, and may move the connection line with the lapse of time.

[0033] With this structure, linked movement of the lumber area and the thoracodorsal area can be displayed and easily understood.

[0034] In the device, the displaying means may display images of soles of both feet of the subject on the monitor and specified places of the soles of the both feet, the calculating means may calculate impact values applied to the specified places, and the displaying means may display the calculated impact values on the monitor.

[0035] With this structure, the impact values applied to the both feet can be known, so that the ambulatory status can be further correctly confirmed.

EFFECTS OF THE INVENTION

[0036] In the device for detecting ambulatory state of the present invention, a proper judgement can be per-

formed without gaining many actual experiences in, for example, a rehabilitation facility.

BRIEF DESCRIPTION OF THE DRAWINGS

[0037]

[Fig. 1] is an explanation view of a subject whose ambulatory status is detected by the method for detecting an ambulatory status.

[Fig. 2] is an explanation view of a first embodiment of the device for detecting an ambulatory status.

[Fig. 3] is an explanation view of the device for detecting an ambulatory status which has a radio communication function.

[Fig. 4] is an explanation view of another example of the device for detecting an ambulatory status which has a radio communication function.

[Fig. 5] is a schematic view of Lissajous figures displayed by the detecting device of the first embodiment.

[Fig. 6] is a schematic view of Lissajous figures displayed by the detecting device of the first embodiment.

[Fig. 7] is a schematic view of Lissajous figures displayed by the detecting device of the first embodiment.

[Fig. 8] is an explanation view of a second embodiment of the device for detecting an ambulatory status.

[Fig. 9] is an example of a screen displayed on the basis of angular speed data.

[Fig. 10] is an example of a screen displayed on the basis of angle data.

[Fig. 11] is an explanation view of a third embodiment of the device for detecting an ambulatory status.

[Fig. 12] is an explanation view of a fourth embodiment of the device for detecting an ambulatory status.

[Fig. 13] is an explanation view of a setting screen for setting each of motion sensors, which is displayed by the detecting device of the fourth embodiment.

[Fig. 14] is an explanation view of a screen showing data measured by the motion sensors of the detecting device of the fourth embodiment.

[Fig. 15] is an explanation view of a screen for analyzing data from each of the motion sensors and showing the analyzed data, which is displayed by the detecting device of the fourth embodiment.

[Fig. 16] is an explanation view of a screen showing comparison results of the analyzed data shown in Fig. 15, which is displayed by the detecting device of the fourth embodiment.

[Fig. 17] is an explanation view of a fifth embodiment of the device for detecting an ambulatory status.

EMBODIMENTS OF THE INVENTION

(First Embodiment)

5 [0038] An embodiment of the present invention will now be described in detail with reference to the accompanying drawings.

[0039] Fig. 1 is an explanation view of a subject 10 whose ambulatory status will be detected. Fig. 2 is a schematic explanation view of the device for detecting the ambulatory status.

[0040] In the present embodiment, conditions of movement of the subject are measured in two places, i.e., a lumber area 12 and a thoracodorsal area 14. A concrete example of the lumber area 12 is near a sacral bone from lower lumber vertebrae. The sacral bone locates in a lower part of vertebra and constitutes pelvis. The thoracodorsal area 14 is near an apex of a posterior curve of thoracic vertebrae. The thoracic vertebra is a part of the vertebra and locates near scapulars. Note that, the conditions of movement must be measured at said two places, but the conditions of movement may be further measured in three places or more, e.g., head part.

[0041] In case of detecting an ambulatory status, movement of, especially, an upper body trunk can be easily known by measuring conditions of movement of the lumber area and the thoracodorsal area, not legs, so that the ambulatory status can be correctly known.

[0042] In the present embodiment, the device 30 for detecting an ambulatory status has: motions sensors 18 and 20, which are respectively provided to the lumber area 12 and the thoracodorsal area 14 of the subject; a main device section 31; and a monitor 32.

[0043] In the present embodiment, three-axis acceleration sensors 18 and 20 are provided to the lumber area 12 and the thoracodorsal area 14, as examples of the motion sensors, so as to measure the conditions of movement in the lumber area 12 and the thoracodorsal area 14.

[0044] Accelerations of three axes, i.e., an x-axis which is a left/right direction in a horizontal plane, a y-direction which is a walking direction in the horizontal plane and a z-direction which is the vertical direction, can be measured in said places.

[0045] The two three-axis acceleration sensors 18 and 20 are connected to the main device section 31 of the device 30 for detecting an ambulatory status and capable of data-communicating therewith. The three-axis acceleration sensors 18 and 20 are connected to the main device section 31 by, for example, data communication cables 33, so that data communication can be performed.

[0046] Next, a concrete example of the main device section 31 of the device 30 for detecting an ambulatory status will be explained.

[0047] The main device section 31 may be an ordinary computer.

[0048] The computer 31 has a control section 42 which runs on the basis of control programs. The control section

42 is constituted by a CPU, ROMs, RAMs, etc., not shown. The control section 42 is connected to a storing unit 44, e.g., hard disk drive unit, via an inner bus 43. Note that, the storing device 44 is not limited to the hard disk drive unit.

[0049] Note that, a key board and a pointing device, e.g., a mouse 48, which act as input units, are connected to the control section 42 via the inner bus 43.

[0050] The control section 42 calculates conditions of movement in said two places, on the basis of data sent from the three-axis acceleration sensors 18 and 20, so as to realize calculating means 34.

[0051] Further, the control section 42 superposes the conditions of movement, which have been calculated by the calculating means 34, and displays the superposed conditions on the monitor 32, so as to realize displaying means 36.

[0052] Acceleration data of the two three-axis acceleration sensors 18 and 20 are inputted to the calculating means 34.

[0053] The calculating means 34 includes a high-pass filter 35, which filters the acceleration data measured in said two places. Low frequency components of the acceleration data are removed by the high-pass filter 35, so that only high frequency components thereof are obtained.

[0054] A reason of performing the filtering process will be explained. In case of using the acceleration data, walking displacements are included, so the ambulatory status should be judged on the basis of the data excluding the walking displacements. Therefore, in the calculating means 34, the high-pass filter 35 removes the walking displacements, which correspond to the low frequency components, so that only vibration components, which are high frequency components, can be extracted.

[0055] Note that, in the calculating means 34, the filtering means for removing the walking displacements, i.e., low frequency components, is not limited to the high-pass filter, and other filtering means together using angular speeds and signals from magnetic sensors may be employed.

[0056] Further, the calculating means 34 has an integrator 37 for integrating vibration components extracted in the filtering process.

[0057] Note that, in the specification and claims of the present invention, the vibration components of the acceleration data (not integrated) indicate a rocking acceleration; the vibration components of the acceleration data integrated once indicate a rocking speed; and the vibration components of the acceleration data integrated twice indicate a rocking amount.

[0058] The displaying means 36 of the present embodiment makes Lissajous figures of said two places, in a horizontal plane, on the basis of the rocking accelerations, the rocking speeds or the rocking amounts calculated by the calculating means 34, superposes the Lissajous figures of said two places and displays the superposed figures on the monitor 32.

[0059] The Lissajous figure is a curved line drawn by mutually combining single vibrations in the vertical direction.

[0060] In the present embodiment, the vibration components are extracted by the calculating means 34 as described above, so the Lissajous figures can be made.

[0061] Other embodiments of the detecting device of the preset invention are schematically shown in Figs. 3 and 4. Note that, the structural elements shown in Fig. 2 are assigned the same symbols and explanation will be omitted.

[0062] In Fig. 3, the three-axis acceleration sensors 18 and 20 are data-communicated with the main device section 31 by radio communication means, not by communication cables, etc.

[0063] The three-axis acceleration sensors 18 and 20 respectively have data transmitting sections 22 and 24, so that the detected acceleration data can be radio-transmitted. Further, the main device section 31 has a data receiving section 29, which receives the acceleration data radio-transmitted from the data transmitting sections 22 and 24.

[0064] For example, Bluetooth (registered trademark) may be employed as the radio communication means.

[0065] In Fig. 4 too, the three-axis acceleration sensors 18 and 20 can be radio-communicated with the main device section 31 so as to transmit and receive the data, but the three-axis acceleration sensors 18 and 20 are connected to one data transmitting section 25, so the data from the two three-axis acceleration sensors 18 and 20 can be transmitted from the one data transmitting section 25.

[0066] The main device section 31 has the data receiving section 29, which receives the acceleration data radio-transmitted from the data transmitting section 25.

[0067] The Lissajous figures made by the displaying means 36 are schematically shown in Figs. 5-7.

[0068] In each of the Lissajous figures of the present embodiment, a horizontal axis indicates a left/right direction in a horizontal plane and a vertical axis indicates a walking direction, and the figures show rocking amounts of the lumber area 12 (near the sacral bone) and the thoracodorsal area 14 (near the sixth thoracic vertebrae).

[0069] In Fig. 5, the rocking amounts of the lumber area 12 (near the sacral bone) and the thoracodorsal area 14 (near the sixth thoracic vertebrae) are shown as ellipse circles of the same size. The two ellipse circles are almost not shifted to each other and located at a position near the same. The ellipse circle of the lumber area 12 (near the sacral bone) is located slightly forward and the ellipse circle of the thoracodorsal area 14 (near the sixth thoracic vertebrae) is located slightly backward with respect to the walking direction.

[0070] In case that the rocking amounts of the lumber area 12 (near the sacral bone) and the thoracodorsal area 14 (near the sixth thoracic vertebrae) are almost same and they are almost not shifted in the left/right direction, the ambulatory status is judged as a good status.

[0071] In Fig. 6, the rocking amount of the lumber area 12 (near the sacral bone) is shown as a slightly small ellipse circle. The rocking amount of the thoracodorsal area 14 (near the sixth thoracic vertebrae) is shown as a large ellipse circle, which includes the rocking amount of the lumber area 12 (near the sacral bone) inside. The rocking amount of the thoracodorsal area 14 (near the sixth thoracic vertebrae) largely expands leftward with respect to the rocking amount of the lumber area 12 (near the sacral bone).

[0072] In case that such Lissajous figures are made, a displacement of near the thoracic vertebrae is shifted leftward, so it is assumed that an upper body is largely inclined leftward when a left foot contacts the ground. Therefore, it is judged that there is a problem in a standing period of the left foot (a period while the left foot contacts the ground).

[0073] In Fig. 7, the rocking amount of the lumber area 12 (near the sacral bone) is shown as a slightly small ellipse circle. The rocking amount of the thoracodorsal area 14 (near the sixth thoracic vertebrae) is shown as a large ellipse circle, which includes the rocking amount of the lumber area 12 (near the sacral bone) inside, and largely expands in the left/right direction. Unlike the example shown in Fig. 6, the both rocking amounts are not shifted in the left/right direction.

[0074] In case that such Lissajous figures are made, it is known that a displacement of near the thoracic vertebrae is extremely large (especially in the left/right direction). Therefore, it is assumed that muscles of the lower body trunk are weakened and a driving force of walking is generated by largely swinging the upper body.

[0075] Note that, the Lissajous figures of Fig. 5-7 show the rocking amounts (the values obtained by integrating the vibration components obtained by filtering the acceleration data twice), and the above described rocking accelerations and rocking speeds can be shown as Lissajous figures.

(Second Embodiment)

[0076] In the above described First Embodiment, the three-axis acceleration sensors are employed as the motion sensors. The present embodiment, in which three-axis angular speed sensors are employed as the motion sensors, will be explained with reference to Fig. 8.

[0077] Note that, the structural elements described in the former embodiment are assigned the same symbols and explanation will be omitted.

[0078] In case of employing the three-axis angular speed sensors as the motion sensors, the motion sensors are respectively provided to the lumber area 12 and the thoracodorsal area 14, and detected angular speed data are sent to the calculating means 34.

[0079] The angular speed data of the three-axis angular speed sensors 38 and 40 provided in said two places are inputted to the calculating means 34.

[0080] The calculating means 34 includes the high-

pass filter 35, which filters the angular speed data measured in said two places. Low frequency components of the angular speed data are removed by the high-pass filter 35, so that only high frequency components thereof are obtained.

[0081] Further, the calculating means 34 has the integrator 37 for integrating vibration components extracted in the filtering process.

[0082] Note that, in the specification and claims of the present invention, the vibration components of the angular speed data (not integrated) indicate a rocking angular speed; and the vibration components of the angular speed data integrated once indicate a rocking angle.

[0083] Note that, the three-axis angular speed sensors 38 and 40 may be data-communicated with the main device section 31 by radio communication means, not by a communication cables, etc. In this case, the structure shown in Fig. 3 or 4 may be employed, so explanation will be omitted.

[0084] The displaying means 36 of the present embodiment makes Lissajous figures of said two places, in the horizontal plane, on the basis of the rocking angular speeds and the rocking angles calculated by the calculating means 34, superposes the Lissajous figures of said two places and displays the superposed figures on the monitor 32.

[0085] Note that, examples of the Lissajous figures are not shown, but they are similar to those of the First Embodiment which are shown in Figs. 5-7.

[0086] In comparison with the acceleration data, the angular speed data are sometimes less influenced by walking displacements.

[0087] Therefore, the displaying means 36 may superpose the angular speed data of said two places and display the superposed data on the monitor 32 without filtering or integrating the angular speed data by the calculating means 34.

[0088] Note that, in this case, the calculating means 34 in the control section 42 may be omitted.

[0089] An example of a display screen of the monitor, in which the angular speed data without being filtered and integrated are displayed, is shown in Fig. 9.

[0090] In Fig. 9, the horizontal axis of the graph indicates "time (sec.)" and the vertical axis thereof indicates "angular speed (degrees/sec.)".

[0091] There are four high peaks in the graph. The peak appears when taking one step, so the graph shows that the subject has walked four steps.

[0092] In this example, the angular speed near the sacral bone is slow, so it is judged that at least the lumber area is not twisted; but turn near the thoracic vertebrae is large, so it is judged that the subject walks with twisting the upper body trunk.

[0093] Further, the calculating means 34, to which the angular speed data have been inputted, may integrate the data once, without filtering the data, to obtain the angle data, and may display conditions of movement, on the basis of the angle data, on the monitor 32.

[0094] An example of the screen of the monitor, in which the angle data obtained by integrating once, without being filtered, are displayed, is shown in Fig. 10.

[0095] In Fig. 10, four hands indicating right and left directions are extended from a center of a circle, an upper side of the drawing is a walking direction, and scales of 30 degrees, 60 degrees and 90 degrees, with respect to the center of the circle, are provided on the right and left sides.

[0096] Two hands of the four indicate angles of the lumber area, and the rest hands indicate angles of the thoracodorsal area. The two hands of the lumber area or the thoracodorsal area respectively indicate maximum angles in the right direction and the left direction.

[0097] With this method, twist of the upper body while walking can be judged.

(Third Embodiment)

[0098] An embodiment, in which three-axis magnetic sensors are employed as the motion sensors, will be explained with reference to Fig. 11.

[0099] Note that, the structural elements described in the former embodiments are assigned the same symbols and explanation will be omitted.

[0100] Magnetic sensors can detect angle components of moving parts by using the fact that magnetic field of earth magnetism is greater. Therefore, in the present embodiment too, the three-axis magnetic sensors detect angle data.

[0101] In case that the three-axis magnetic sensors 39 and 41 are employed as the motion sensors too, the sensors are respectively provided in the lumber area 12 and the thoracodorsal area 14, and the detected angle data are sent to the control section 42.

[0102] In the present embodiment, the angler data may be used without being processed, and the displaying means 36 may superpose the angle data of said two places and may display them on the monitor 32.

[0103] In this case, the calculating means 34 for filtering and integrating the data may be omitted.

[0104] Note that, the three-axis magnetic sensors 39 and 41 may be data-communicated with the main device section 31 by radio communication means, not by communication cables, etc. In this case, the structure shown in Fig. 3 or 4 may be employed, so explanation will be omitted.

[0105] The screen of the monitor indicating the angle data may be similar to the example shown in Fig. 10, so explanation will be omitted.

(Fourth Embodiment)

[0106] An embodiment, in which three-axis acceleration sensors and three-axis angular speed sensors are employed as the motion sensors, will be explained.

[0107] Namely, a motion sensor 56 is constituted by the three-axis acceleration sensor and the three-axis an-

gular speed sensor, and provided to near the sacral bone; and a motion sensor 58 is also constituted by the three-axis acceleration sensor and the three-axis angular speed sensor, and provided to near the thoracic vertebrae.

[0108] The device for detecting an ambulatory status of the present embodiment is shown in Fig. 12.

[0109] Note that, the structural elements described in the former embodiments are assigned the same symbols and explanation will be omitted.

[0110] The motion sensors 56 and 58 respectively have the data transmitting sections 22 and 24, so that the detected acceleration data can be radio-transmitted. Further, the main device section 31 has the data receiving section 29, which receives the acceleration data transmitted from the data transmitting sections 22 and 24. For example, Bluetooth (registered trademark) may be employed as the radio communication means.

[0111] The main device section 31 may be an ordinary computer.

[0112] The computer 31 has the control section 42 which runs on the basis of the control programs.

[0113] By starting the control program previously stored in the control section 42, an operation screen shown in Fig. 13 is displayed on the monitor 32. The operation screen is used to set and correct the motion sensors 56 and 58.

[0114] By pushing a connecting/setting button 60 shown in an upper-left part of the screen shown in Fig. 13 with, for example, the mouse 48, the control section 42 connects and sets the motion sensors 56 and 58.

[0115] A sensor turn-off button 61 is provided to near the connecting/setting button 60.

[0116] Instructions for correction are shown in a right part of the screen shown in Fig. 13.

[0117] A purpose of the instructions is to securely detect the gravity direction and the horizontal direction perpendicular to the gravity direction, and an operator can select a simple correction manner or a standard correction manner.

[0118] In each of the simple correction manner and the standard correction manner, the motion sensors 56 and 58 are mounted on a horizontal plane so as to detect the gravity direction. By pushing a correction button 62 with the mouse 48, etc., the control section 42 executes the correction. Corrected data collection lamps, which respectively correspond to the motion sensors 56 and 58, are provided to near the correction button 62.

[0119] Next, the actual detecting actions will be explained.

[0120] The motion sensor 56 is provided to near the sacral bone of the subject, the motion sensor 58 is provided to near the sixth thoracic vertebrae thereof, and the control section 42 automatically collects walking data of a prescribed time period when the subject walks.

[0121] Note that, when the motion sensors 56 and 58 are attached to the subject, the motion sensors 56 and 58 must be directed in the assigned directions. For ex-

ample, in the motion sensors 56 and 58, the attaching directions are indicated as follows: X-direction being a right direction; Y-direction being an upper direction; and Z-direction being a walking direction.

[0122] Acceleration data in the X-direction, acceleration data in the Y-direction and acceleration data in the Z-direction, angular speed data in the X-direction, angular speed data in the Y-direction and angular speed data in the Z-direction are transmitted from the motion sensor 56 provided to near the sacral bone, at regular time intervals (e.g., 5 milliseconds), to the data receiving section 29.

[0123] Similarly, acceleration data in the X-direction, acceleration data in the Y-direction and acceleration data in the Z-direction, angular speed data in the X-direction, angular speed data in the Y-direction and angular speed data in the Z-direction are transmitted from the motion sensor 58 provided to near the sixth thoracic vertebrae, at regular time intervals (e.g., 5 milliseconds), to the data receiving section 29.

[0124] The data received by the data receiving section 29 are displayed, without being processed, by the displaying means 36.

[0125] An example of displaying the detected data is shown in Fig. 14.

[0126] In Fig. 14, a graph 64 shows an acceleration A_x in the X-direction, an acceleration A_y in the Y-direction and an acceleration A_z in the Z-direction measured by the acceleration sensors included in the motion sensor 56 provided to near the sacral bone, the horizon axis indicates "time (sec.)" and the vertical axis indicates "accelerations ($m/sec.^2$)".

[0127] A graph 65 shows an angular speed W_x in the X-direction, an angular speed W_y in the Y-direction and an angular speed W_z in the Z-direction measured by the angular speed sensors included in the motion sensor 56 provided to near the sacral bone, the horizon axis indicates "time (sec.)" and the vertical axis indicates "angular speed ($rad/sec.^2$)".

[0128] A graph 66 shows an acceleration A_x in the X-direction, an acceleration A_y in the Y-direction and an acceleration A_z in the Z-direction measured by the acceleration sensors included in the motion sensor 58 provided to near the sixth thoracic vertebrae, the horizon axis indicates "time (sec.)" and the vertical axis indicates "accelerations ($m/sec.^2$)".

[0129] A graph 67 shows an angular speed W_x in the X-direction, an angular speed W_y in the Y-direction and an angular speed W_z in the Z-direction measured by the angular speed sensors included in the motion sensor 58 provided to near the sixth thoracic vertebrae, the horizon axis indicates "time (sec.)" and the vertical axis indicates "angular speed ($rad/sec.^2$)".

[0130] In Fig. 14, a setting part 68 for setting a measuring timer period is provided on the right side of the graphs. An indicating part 69 for indicating a remaining period of measurement is provided under the setting part 68. Further, a start/stop button 70 for starting or stopping

the measurement is provided.

[0131] Note that, as to the data shown in Fig. 14, the data being measured can be displayed in real time, and the data which have been previously measured can be displayed, too. In case of storing the measured data (the data previously measured and stored), the measured data can be read and the graphs 64-67 can be displayed by pushing a stored data button 71.

[0132] Fig. 15 shows a screen displaying the results of analyzing the data shown in Fig. 14.

[0133] The calculating means 34 removes low frequency components from the accelerations A_x in the X-direction, the accelerations A_y in the Y-direction and the accelerations A_z in the Z-direction by the high-pass filter. The integrator 37 of the calculating means 34 integrates the rocking accelerations, which have been extracted in the filtering process, once to calculate rocking speeds and integrates the same twice to calculate rocking amounts.

[0134] A graph 72 in an upper-left part of Fig. 15 shows displacements of the motion sensor 56 provided to near the sacral bone in the X-, Y- and Z-directions respectively. The horizontal axis of the graph 72 indicates "displacement (mm)", and the vertical axis thereof indicates "time (sec.)".

[0135] In the graph 72, the displacements in the three directions indicated by the vertical axis are distances from a reference stop position (0).

[0136] A graph 74 in a lower-left part of Fig. 15 shows Lissajous figures of the displacement of the motion sensor 56 provided to near the sacral bone, the vertical axis indicates "displacement (mm)" in the vertical direction, and the horizontal axis indicates "displacement (mm)" in the left/right direction.

[0137] A graph 76 in an upper-right part of Fig. 15 shows Lissajous figures of the displacement of the motion sensor 58 provided to near sixth thoracic vertebrae in the X-, Y- and Z-directions respectively, the vertical axis indicates "displacement (mm)" in the vertical direction, and the horizontal axis indicates "displacement (mm)" in the left/right direction. The horizontal axis of the graph 76 indicates "displacement (mm)", and the vertical axis thereof indicates "time (sec.)".

[0138] In the graph 76, the displacements in the three directions indicated by the vertical axis are distances from the reference stop position (0).

[0139] A graph 76 in a lower-right part of Fig. 15 shows Lissajous figures of the displacement of the motion sensor 58 provided to near sixth thoracic vertebrae, the vertical axis indicates "displacement (mm)" in the vertical direction, and the horizontal axis indicates "displacement (mm)" in the left/right direction.

[0140] As to the track graphs 74 and 78 of Fig. 15 showing the Lissajous figures, the graphs in the X-Y plane, Y-Z plane of X-Z plane can be selectively displayed by pushing a select button 79. In Fig. 15, the X-Y plane is displayed as a frontal plane, and the Y-Z plane a sagittal plane or the X-Z plane (the horizontal plane) can be fur-

ther displayed by pushing the select button 79.

[0141] As to the displayed data of the track graphs 74 and 78 shown in Fig. 15, a walking cycle of a selected time period to be displayed can be optionally selected from walking cycles which have been actually measured. Selecting the walking cycle can be performed in a select screen 80. In Fig. 15, a first walking and a second walking cycle are displayed, but it is preferable to select a middle part of the cycles during stable walking. The range of the walking cycle selected in the select screen 80 is displayed by two thick lines 81 in the graphs 72 and 76 showing the displacements of the motion sensors 56 and 58.

[0142] The calculating means 34 is capable of calculating a walking pitch on the basis of the rocking amounts, which have been obtained from the data measured by the motion sensors 56 and 58. One walking pitch is from putting one foot on the ground to nextly putting the same foot on the ground.

[0143] The calculated walking pitch is displayed in an extraction window 83. Further, the calculating means 34 is capable of calculating the walking pitch within a maximum limit, which can be set, by the operator, in a maximum limit setting window 85.

[0144] The measured data of the graphs shown in Fig. 15 and analyzing conditions can be stored in the storing device 44 by pushing a storing button 96.

[0145] The measured data and the analyzing conditions can be store as, for example, CSV files.

[0146] The displaying means finally makes a screen shown in Fig. 16, which will be provided to the subject.

[0147] Fig. 16 is characterized in that the Lissajous figures of the displacements of the places near the sacral bone and near the sixth thoracic vertebrae, which are detected by the motion sensors 56 and 58, in the Y-A plane the saggital plane 100, the X-Y plane (the frontal plane) and the X-Z plane (the horizontal plane) are simultaneously displayed.

[0148] Note that, in Fig. 16, the three Lissajous figures correspond to the two kinds of data are disposed on right and left to compare with each other, but the figures correspond to one kind of the two may be displayed.

[0149] The displaying means 36 is capable of displaying connection lines 82, each of which connects same time points in the Lissajous figures of the motion sensors 56 and 58 of said two places to each other, and moves the connection lines 82 with the lapse of time.

[0150] When the operator pushes a phase button 89 which is located in the right part of the screen, the displaying means 36 displays the connection lines 82. A playback button 92 is provided under the phase button 89. By pushing the playback button 92, the displaying means 36 displays and moves the connection lines with the lapse of time. A playback speed of displaying the connection lines 82 can be changed by changing a number in a playback speed window 93. When the number in the playback speed window 93 is 1.0, the playback is performed in a normal time; when the number therein is 0.5, the playback can be performed in a half of

the normal time.

[0151] Indication parts 105, in each of which rocking widths and track lengths of each Lissajous figure are indicated, are respectively disposed adjacent to the Lissajous figures of the Y-Z plane the saggital plane 100, the X-Y plane (the frontal plane) 102 and the X-Z plane (the horizontal plane) 104.

[0152] The displaying means 36 calculates front-to-rear widths (mm), vertical widths (mm) and track lengths (mm) relating to the Y-Z plane the saggital plane 100 and displays them in the indication parts 105.

[0153] The displaying means 36 calculates left and right widths (mm), vertical widths (mm) and track lengths (mm) relating to the X-Y plane (the frontal plane) 102 and displays them in the indication parts 105.

[0154] The displaying means 36 calculates left and right widths (mm), front-to-rear widths (mm) and track lengths (mm) relating to the X-Z plane (the horizontal plane) 104 and displays them in the indication parts 105.

[0155] Images of soles 84a and 84b of the left foot and the right foot are shown under the Lissajous figures, and impact values applied to specified places in the soles are displayed in impact value windows 86a and 86b. Instruction bars 87a and 87b, which are used to optionally specify the places in the soles, are located near the images of the soles 84a and 84b, and the operator can optionally specify the places in the soles by operating the instruction bars 87a and 87b.

[0156] When the operator operates the instruction bars 87a and 87b, the calculating means 34 calculates vertical accelerations in the specified places detected by the motion sensor 56, and the displaying means 36 displays the calculated accelerations in the impact value windows 86a and 86b as the impact values.

[0157] Note that, in case that a rearmost part of the Lissajous figure (formed like "oo") of the X-Z plane (the horizontal plane) relating to the motion sensor 56 is regarded as a time point when a heel contacts the ground and that a frontmost part thereof is regarded as a time point when a toe leaves the ground, the places in each of the soles can be known.

[0158] The analysis results shown in Fig. 16 can be stored in the storing device 44 by pushing a storing button 95. The analysis results can be store as, for example, a CSV file.

[0159] Further, scales of the Lissajous figures can be changed by changing a number displayed in a scale window 97.

[0160] Note that, the displaying means 36 is capable of making video images (animations) of three dimensional movement of the subject on the basis of the displacements of the place near the sacral bone and the place near sixth thoracic vertebrae in the Y-Z plane the saggital plane

, the X-Y plane (the frontal plane) and the X-Z plane (the horizontal plane) detected by the motion sensors 56 and 58.

[0161] Note that, in each of the former embodiments

too, the places of the motion sensors may be measured, and Lissajous figures may be corrected on the basis of the positional relationship between the motion sensors.

[0162] For example, the subject is compulsorily taken a reference position when the subject is in a stationary state. To take the reference position, an assistant may correct the posture or a posture correcting member may be attached to the subject. Then, the subject is made relax and made take an easy posture. In this action, a rocking amount from the reference posture to an original posture or ordinary posture of the subject (physical feature) is calculated by the calculating means 34. Namely, positional displacement, inclination and twist between the motion sensors of the lumber area and the thoracodorsal area can be known. For example, in case that a right shoulder of the subject is originally lowered, the motion sensor of the thoracodorsal area is inclined rightward more than the motion sensor of the lumber area; in case that the subject is round-shouldered, the motion sensor of the thoracodorsal area is inclined forward more than the motion sensor of the lumber area.

[0163] For example, when it is known that the motion sensor of the thoracodorsal area is rightwardly shifted 1 cm from the motion sensor of the lumber area on the basis of the rocking amounts calculated by the calculating means 34, the displaying means 36 corrects to rightwardly shift the Lissajous figure of the rocking amount of the thoracodorsal area 1 cm.

[0164] By this action, the original physical features can be confirmed, from the Lissajous figures, even in the walking state.

[0165] The Lissajous figures may be displayed with considering physical features of the subject while walking, not physical features of the stationary state. Some subjects can take the reference postures, but they will sometimes take bad postures or good postures while walking.

[0166] In such case, the calculating means 34 calculates positional displacements of the motion sensors attached to the walking subject, in orthogonal coordinate systems, so as to calculate physical features of the subject while walking.

[0167] Then, the displaying means 36 corrects the Lissajous figures of the rocking amounts on the basis of the physical features. With this manner, the physical features while walking too can be confirmed.

(Fifth Embodiment)

[0168] An embodiment, in which conditions of movement are measured on the basis of images photographed by high speed cameras without using motion sensors, will be explained with reference to Fig. 17.

[0169] Note that, the structural elements described in the former embodiments are assigned the same symbols and explanation will be omitted.

[0170] High speed cameras 55 are publicly known cameras which are capable of photographing several

dozens of frames a second. A plurality of the high speed cameras 55, which are disposed at different positions, are provided so as to improve a measuring accuracy.

[0171] Markers 50 and 52 are respectively attached in the lumber area 12 and the thoracodorsal area 14. The high speed cameras 55 photograph the markers 50 and 52.

[0172] Photographed image data are inputted to the main device section 31.

[0173] In the main device section 31, the displaying means 36 realized by the control section 42 displays the conditions of movement of the markers 50 and 52, on the basis of the image data, on the monitor 32. At this time, the image data photographed by the high speed cameras 55 located at different positions are inputted to the main device section 31, so it is preferable to display three dimensional movements of the markers 50 and 52, i.e., moving tracks of the markers 50 and 52 (not shown).

[0174] Note that, in the present embodiment, the motion sensors described in the former embodiments may be provided to the places of the markers 50 and 52, and means for calculating conditions of movement of said two places on the basis of data measured by the motion sensors may be further provided (not shown).

[0175] In this case, the displaying means 36 superposes the moving tracks of the markers 50 and 52, which have been photographed by the high speed cameras 55, and displays the superposed tracks on the monitor 32, further the displaying means can superpose the conditions of movement of said two places and can display the superposed conditions on the monitor 32.

[0176] Further, a positional relationship between the motion sensors attached to the subject in the stationary state may be measured by using the high speed cameras 55. The positional relationship between the motion sensors are, for example, positional displacement, inclination and twist between the motion sensors of the lumber area and the thoracodorsal area. For example, in case that a right shoulder of the subject is originally lowered, the motion sensor of the thoracodorsal area is inclined rightward more than the motion sensor of the lumber area; in case that the subject is round-shouldered, the motion sensor of the thoracodorsal area is inclined forward more than the motion sensor of the lumber area.

[0177] By photographing the positions of the motion sensors of the subject being stationary with the high speed cameras 55, the above described positional relationships can be known. The displaying means 36 is capable of correcting the Lissajous figures of the rocking amounts measured by the motion sensors on the basis of the positional relationship between the motion sensors and displaying the corrected figures on the monitor 32. For example, when it is known that the motion sensor of the thoracodorsal area is rightwardly shifted 1 cm from the motion sensor of the lumber area on the basis of the rocking amounts calculated by the calculating means 34, the displaying means 36 corrects to rightwardly shift the Lissajous figure of the rocking amount of the thoracodorsal

sal area 1 cm.

[0178] By this action, the original physical features of the subject can be confirmed, from the Lissajous figures, even in the walking state.

[0179] In the above described embodiments, the conditions of movement of the subject 10 are measured in the two places, i.e., the lumber area 12 and the thoracodorsal area 14, but the conditions of movement may be measured in three places or more, e.g., head.

[0180] Note that, in the above described embodiments, the motion sensors are the acceleration sensors only, the angular speed sensors only or the magnetic sensors only, but a combination or combinations of the acceleration sensor, the angular speed sensor and the magnetic sensor may be employed.

[0181] In such case, a combination or combinations of accelerations, speeds, positions, angular speeds and angles can be measured.

[0182] In each of the above described embodiments, a large-sizes monitor may be employed as the monitor 32, and the subject may walk with watching his own posture displayed on the monitor.

[0183] In this case, the subject can walk with correcting his posture, so a feedback effect can be obtained.

[0184] Further, the displaying means 36 is capable of making personified images, e.g., computer graphics, animations, on the basis of the analysis results of Lissajous figures, and the displaying means may display the personified images on the monitor 32. With this manner, the subject can easily understand the analysis results.

(Use of Device for Detecting Ambulatory Status)

[0185] The conditions of movement of the lumber area and the thoracodorsal area can be known by the above described device for detecting the ambulatory status, so effects of an insole of a shoe can be confirmed.

[0186] These days, manufacturers have developed insoles of many kinds of shoes, e.g., running shoes, climbing shoes, winter sports shoes, and the insoles are composed of suitable materials and formed into suitable shapes on the basis of uses.

[0187] In Fig. 16, the two kinds of data are displayed on right and left, and the data can be changed by pushing a read button 90. Therefore, by attaching no insoles to shoes, attaching insoles to the shoes and changing insoles, the operator can collect a plurality of sets of data of the motion sensors and display the two kinds of data under different conditions on the monitor 32.

[0188] By displaying the data collected under different conditions on one screen as shown in Fig. 16, the ambulatory statuses under different conditions can be easily known.

[0189] As to the example shown in Fig. 16, Data 2 on the right side indicate existence of walking deviations in the three directions, i.e., forth/back direction, left/right direction and vertical direction; on the other hand, Data 1 on the left side indicate the good ambulatory state.

[0190] Conventionally, effects of insoles, e.g., walking ease, are subjectively judged by a subject only, but the effects can be easily objectively judged by the device for detecting an ambulatory status.

(Other Uses of Device)

[0191] The device for detecting an ambulatory status can be used for not only confirming effects of insoles but also confirming whether shoes are good or bad. By changing shoes, the operator can collect data of the motion sensors a plurality of times, so that suitable shoes capable of producing a good ambulatory status can be easily objectively judged.

[0192] Further, the device for detecting ambulatory status is capable of confirming effects of rehabilitation. By collecting data of the motion sensors before and after performing rehabilitation, the operator can easily objectively judge whether the rehabilitation improves the ambulatory status or not.

[0193] The device for detecting ambulatory status is capable of confirming effects of physical training and stretching exercise. By collecting data of the motion sensors before and after performing physical training or stretching exercise, the operator can easily objectively judge whether the physical training or stretching exercise effectively improves the ambulatory status or not.

[0194] The preferred embodiments of the present have been explained above, but the present invention is not limited to the embodiments but is solely limited by the scope of the claims.

Claims

1. A device for detecting an ambulatory status, comprising:

a monitor;
 motion sensors being respectively provided to two places of a subject, i.e., a lumber area and a thoracodorsal area;
 means for calculating conditions of movement in said two places on the basis of data measured by the motion sensors; and
 means for superposing the conditions of movement in said two places, which have been calculated by the calculating means, and displaying the superposed conditions on the monitor;
characterized in that each of the motion sensors is constituted by a three-axis acceleration sensor and a three-axis angular speed sensor, the calculating means is configured to detect the gravity direction on the basis of the data detected by the three-axis acceleration sensor and calculate angular speeds or angles in the three-dimensional orthogonal coordinate system, i.e., in the gravity direction, a walking direction in a

horizontal plane and a left/right direction in the horizontal plane, on the basis of the detected gravity direction, from the data detected by the three-axis acceleration sensors, and the displaying means is configured to make Lissajous figures on the basis of the angular speeds or angles in the gravity direction, the walking direction in the horizontal plane and the left/right direction in the horizontal plane, superpose the Lissajous figures of the motion sensors of said two places in the walking direction in the horizontal plane and the left/right direction in the horizontal plane respectively, and display the superposed figures on the monitor.

2. The device for detecting an ambulatory status according to claim 1, wherein the calculating means is configured to calculate conditions of movement in said two places from a reference posture of the subject being stationary to an ordinary posture of the subject being stationary, and the displaying means is configured to correct the conditions of movement in said two places from the reference posture of the subject to the ordinary posture of the subject being stationary, which have been calculated by the calculating means, and display the corrected conditions on the monitor when superposing the conditions of movement in said two places, which have been measured by the motion sensors on the basis of the measured data, and displaying the superposed conditions on the monitor.
3. The device for detecting an ambulatory status according to claim 1 or 2, wherein the calculating means is configured to calculate positions of the motion sensors with respect to a center axis of the subject along the vertical direction while walking, and the displaying means is configured to correct the positions of the motion sensors, which are calculated by the calculating means, and display the corrected positions on the monitor when superposing the conditions of movement in said two places, which are measured by the motion sensors on the basis of the measured data, and display the superposed conditions on the monitor.
4. The device for detecting an ambulatory status according to any one of claims 1 to 3, wherein the displaying means is configured to display a connection line, which connects same time points in the Lissajous figures of the motion sensors of said two places to each other, and move the connection line with the lapse of time.
5. The device for detecting an ambulatory status according to any one of claims 1 to 4, wherein

the displaying means is configured to display

images of soles of both feet of the subject on the monitor and specified places of the soles of the both feet, the calculating means is configured to calculate impact values applied to the specified places, and the displaying means is configured to display the calculated impact values on the monitor.

Patentansprüche

1. Vorrichtung zur Detektion eines ambulanten Zustands, die Folgendes umfasst:

einen Monitor;
Bewegungssensoren, die jeweils an zwei Stellen eines Individuums bereitgestellt sind, d.h. einem Lendenbereich und einem Brustkorb-Rücken-Bereich;
Mittel zur Berechnung von Bewegungsbedingungen an diesen zwei Stellen auf Basis der Daten, die von den Bewegungssensoren gemessen wurden; und
Mittel zum Überlagern der Bewegungsbedingungen an diesen zwei Stellen, die vom Berechnungsmittel berechnet wurden, und das Anzeigen der überlagerten Bedingungen auf dem Monitor;

dadurch gekennzeichnet, dass

jeder der Bewegungssensoren aus einem dreiaxigen Beschleunigungssensor und einem dreiaxigen Winkelgeschwindigkeitssensor besteht,
das Berechnungsmittel ausgebildet ist, um die Gravitationsrichtung auf Basis der vom dreiaxigen Beschleunigungssensor detektierten Daten zu detektieren, und Winkelgeschwindigkeiten oder Winkel im dreidimensionalen orthogonalen Koordinatensystem zu berechnen, d.h. in der Gravitationsrichtung, einer Gehrichtung auf einer horizontalen Ebene und einer Links/Rechts-Richtung auf der horizontalen Ebene auf Basis der detektierten Gravitationsrichtung von den Daten, die von den dreiaxigen Beschleunigungssensoren detektiert wurden, und
das Anzeigemittel ausgebildet ist, um Lissajous-Figuren auf Basis der Winkelgeschwindigkeiten oder Winkel in die Gravitationsrichtung, der Gehrichtung auf der horizontalen Ebene und der Links/Rechts-Richtung auf der horizontalen Ebene zu erzeugen, die Lissajous-Figuren der Bewegungssensoren von diesen zwei Stellen in die Gehrichtung auf der horizontalen Ebene bzw. der Links/Rechts-Richtung auf der horizontalen Ebene zu überlagern und die überlagerten Figuren auf dem Monitor anzuzeigen.

2. Vorrichtung zu Detektion eines ambulanten Zustands nach Anspruch 1, wobei das Berechnungsmittel ausgebildet ist, um Bewegungsbedingungen an diesen beiden Stellen aus einer Referenzhaltung des ruhig stehenden Individuums zu einer Normalhaltung des ruhig stehenden Individuums zu berechnen, und
das Anzeigemittel ausgebildet ist, um die Bewegungsbedingungen an diesen zwei Stellen von der Referenzhaltung des Individuums zur Normalhaltung des Individuums, das stationär ist, die vom Berechnungsmittel berechnet wurden, zu korrigieren, und die korrigierten Bedingungen auf dem Monitor anzuzeigen, wenn die Bewegungsbedingungen an diesen zwei Stellen überlagert werden, die von den Bewegungssensoren auf Basis der gemessenen Daten gemessen wurden, und die überlagerten Bedingungen auf dem Monitor anzuzeigen. 10
3. Vorrichtung zur Detektion eines ambulanten Zustands nach Anspruch 1 oder 2, wobei das Berechnungsmittel ausgebildet ist, um Positionen der Bewegungssensoren in Bezug auf eine Mittelachse des Individuums entlang der vertikalen Richtung während des Gehens zu berechnen, und
das Anzeigemittel ausgebildet ist, um die Positionen der Bewegungssensoren, die vom Berechnungsmittel berechnet werden, zu korrigieren, und die korrigierten Positionen auf dem Monitor anzuzeigen, wenn die Bewegungsbedingungen an diesen zwei Stellen überlagert werden, die von den Bewegungssensoren auf Basis der gemessenen Daten gemessen werden, und die überlagerten Bedingungen auf dem Monitor anzuzeigen. 20 25 30
4. Vorrichtung zur Detektion eines ambulanten Zustands nach einem der Ansprüche 1 bis 3, wobei das Anzeigemittel ausgebildet ist, um eine Verbindungslinie anzuzeigen, die die gleichen Punkte auf den Lissajous-Figuren der Bewegungssensoren der zwei Stellen miteinander verbindet und die Verbindungslinie mit dem Zeitverlauf verschiebt. 35 40
5. Vorrichtung zur Detektion eines ambulanten Zustands nach einem der Ansprüche 1 bis 4, wobei das Anzeigemittel ausgebildet ist, um Bilder von Sohlen beider Füße des Individuums, und spezifizierte Stellen der Sohlen der beiden Füße auf dem Monitor anzuzeigen, und
das Berechnungsmittel ausgebildet ist, um die Belastungswerte, die auf die spezifizierten Stellen angewendet werden, zu berechnen, und
das Anzeigemittel ausgebildet ist, um die berechneten Belastungswerte auf dem Monitor anzuzeigen. 45 50 55

Revendications

1. Dispositif destiné à détecter un état ambulator, comprenant :
un moniteur ;

des capteurs de mouvement qui sont respectivement fournis à deux endroits d'un sujet, à savoir au niveau d'une zone lombaire et d'une zone thoraco-dorsale ;

un moyen pour calculer des conditions de déplacement dans lesdits deux endroits sur la base de données mesurées par les capteurs de mouvement ; et

un moyen pour superposer les conditions de déplacement dans lesdits deux endroits, lesquelles ont été calculées par le moyen de calcul, et pour afficher les conditions superposées sur le moniteur ;

caractérisé en ce que chacun des capteurs de mouvement est constitué par un capteur d'accélération à trois axes et un capteur de vitesse angulaire à trois axes ;

le moyen de calcul est configuré de manière à détecter la direction de gravité sur la base des données détectées par le capteur d'accélération à trois axes et à calculer des vitesses angulaires ou des angles dans le système de coordonnées orthogonales tridimensionnelles, à savoir dans la direction de gravité, dans une direction de marche dans un plan horizontal et dans une direction gauche/droite dans le plan horizontal, sur la base de la direction de gravité détectée, à partir des données détectées par les capteurs d'accélération à trois axes ; et

le moyen d'affichage est configuré de manière à réaliser des figures de Lissajous sur la base des vitesses angulaires ou des angles dans la direction de gravité, dans la direction de marche dans le plan horizontal et dans la direction gauche/droite dans le plan horizontal, à superposer les figures de Lissajous des capteurs de mouvement desdits deux endroits dans la direction de marche dans le plan horizontal et dans la direction gauche/droite dans le plan horizontal, et à afficher les figures superposées sur le moniteur.

2. Dispositif destiné à détecter un état ambulator selon la revendication 1, dans lequel le moyen de calcul est configuré de manière à calculer des conditions de déplacement dans lesdits deux endroits, d'une posture de référence du sujet qui est stationnaire à une posture ordinaire du sujet qui est stationnaire ; et le moyen d'affichage est configuré de manière à corriger les conditions de déplacement dans lesdits deux endroits, de la posture de référence du sujet à la posture ordinaire du sujet qui est stationnaire, les-

quelles ont été calculées par le moyen de calcul, et à afficher les conditions corrigées sur le moniteur lors de la superposition des conditions de déplacement dans lesdits deux endroits, lesquelles ont été mesurées par les capteurs de mouvement sur la base des données mesurées, et à afficher les conditions superposées sur le moniteur. 5

3. Dispositif destiné à détecter un état ambulaire selon la revendication 1 ou 2, dans lequel le moyen de calcul est configuré de manière à calculer des positions des capteurs de mouvement par rapport à un axe central du sujet le long de la direction verticale au cours de la marche ; et 10
- le moyen d'affichage est configuré de manière à corriger les positions des capteurs de mouvement, lesquelles sont calculées par le moyen de calcul, et à afficher les positions corrigées sur le moniteur lors de la superposition des conditions de déplacement dans lesdits deux endroits, lesquelles sont mesurées par les capteurs de mouvement sur la base des données mesurées, et à afficher les conditions superposées sur le moniteur. 15 20

4. Dispositif destiné à détecter un état ambulaire selon l'une quelconque des revendications 1 à 3, dans lequel le moyen d'affichage est configuré de manière à afficher une ligne de connexion, qui relie entre eux des mêmes instants dans les figures de Lissajous des capteurs de mouvement desdits deux endroits, et à déplacer la ligne de connexion au fil du temps. 25 30

5. Dispositif destiné à détecter un état ambulaire selon l'une quelconque des revendications 1 à 4, dans lequel : 35

le moyen d'affichage est configuré de manière à afficher des images des semelles des deux pieds du sujet sur le moniteur, et des endroits spécifiés des semelles des deux pieds ; 40

le moyen de calcul est configuré de manière à calculer des valeurs d'impact appliquées aux endroits spécifiés ; et

le moyen d'affichage est configuré de manière à afficher les valeurs d'impact calculées sur le moniteur. 45

50

55

FIG.1

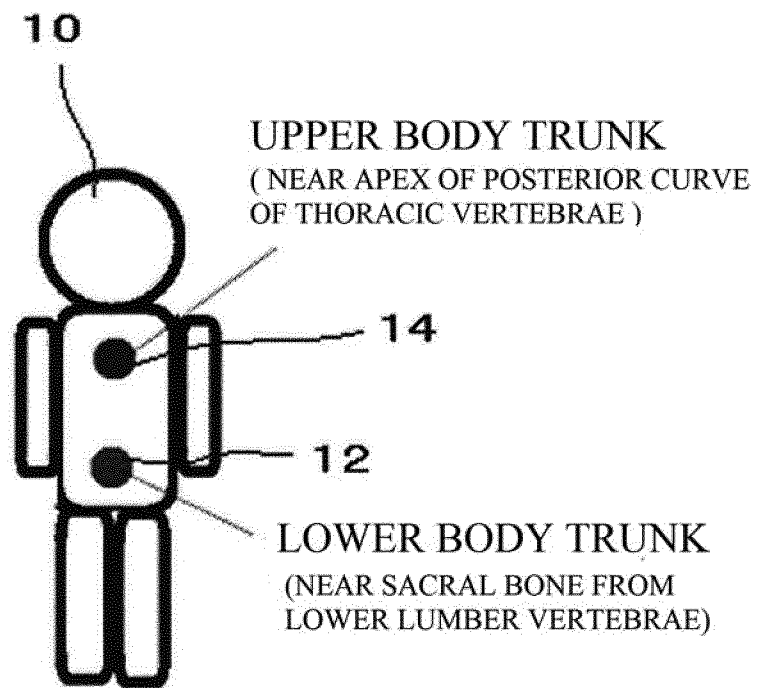


FIG.2

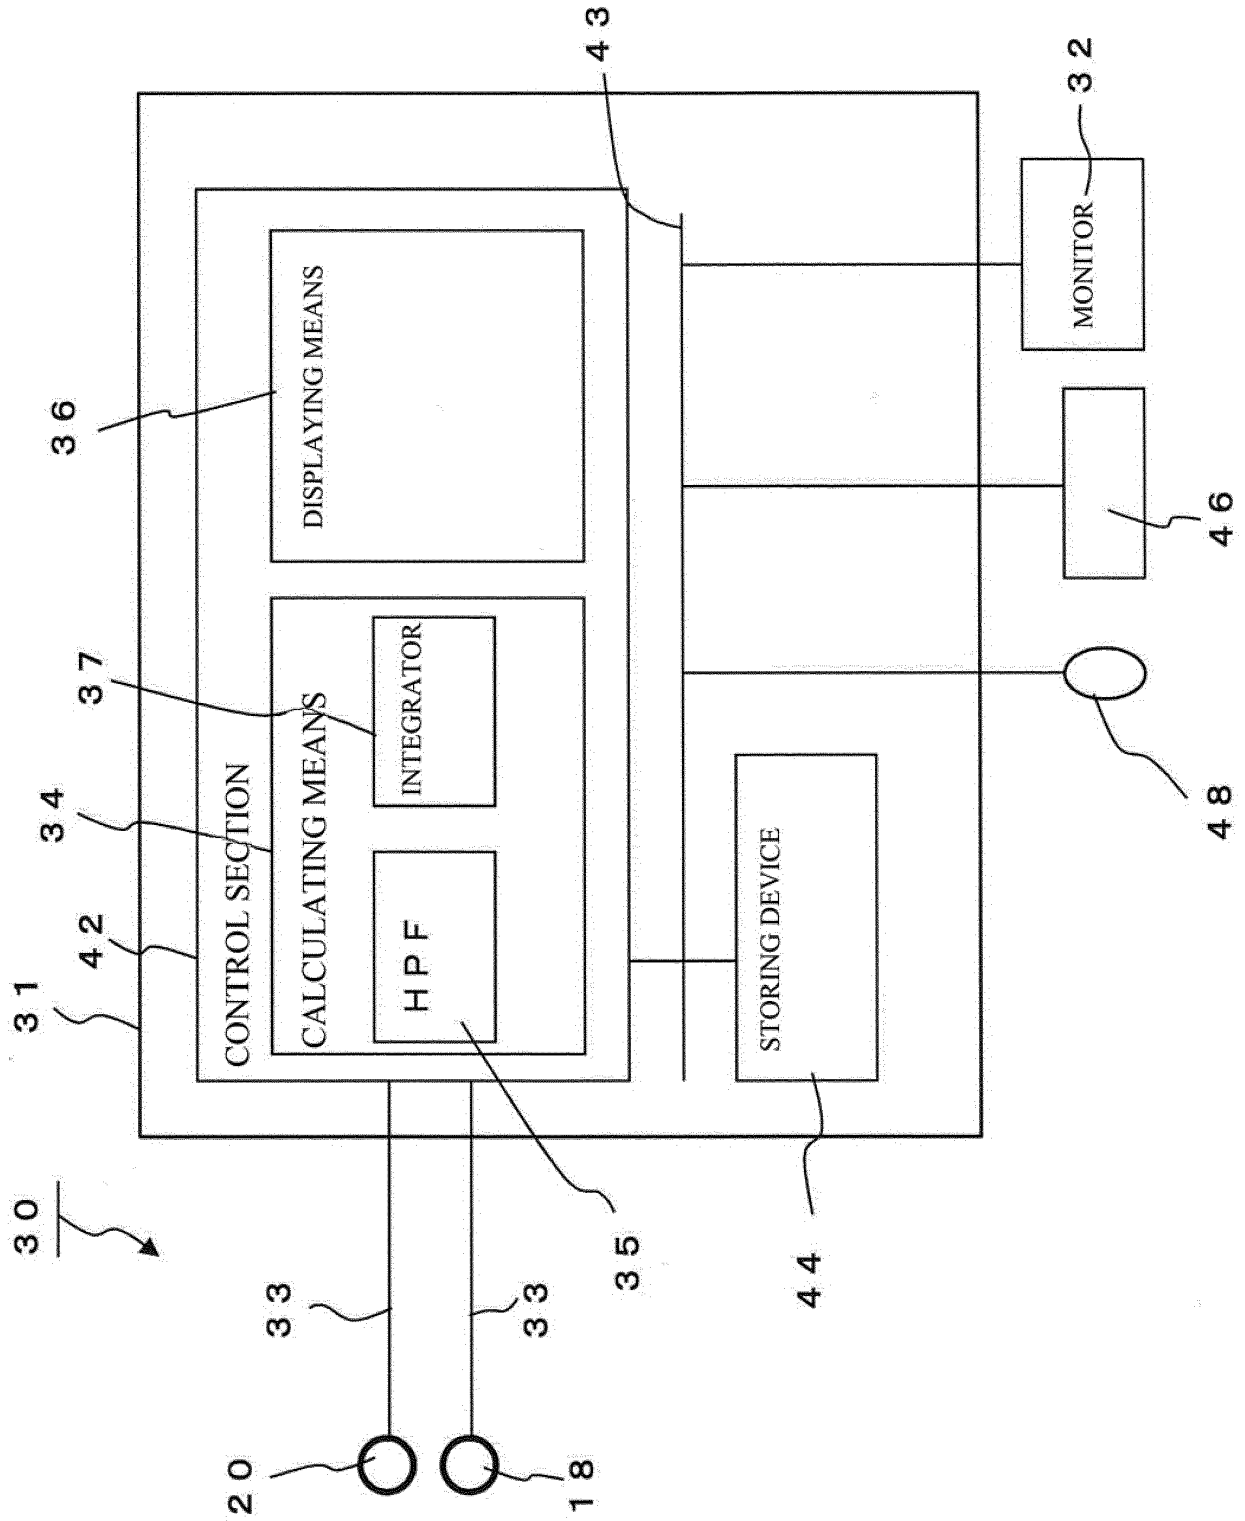


FIG.3

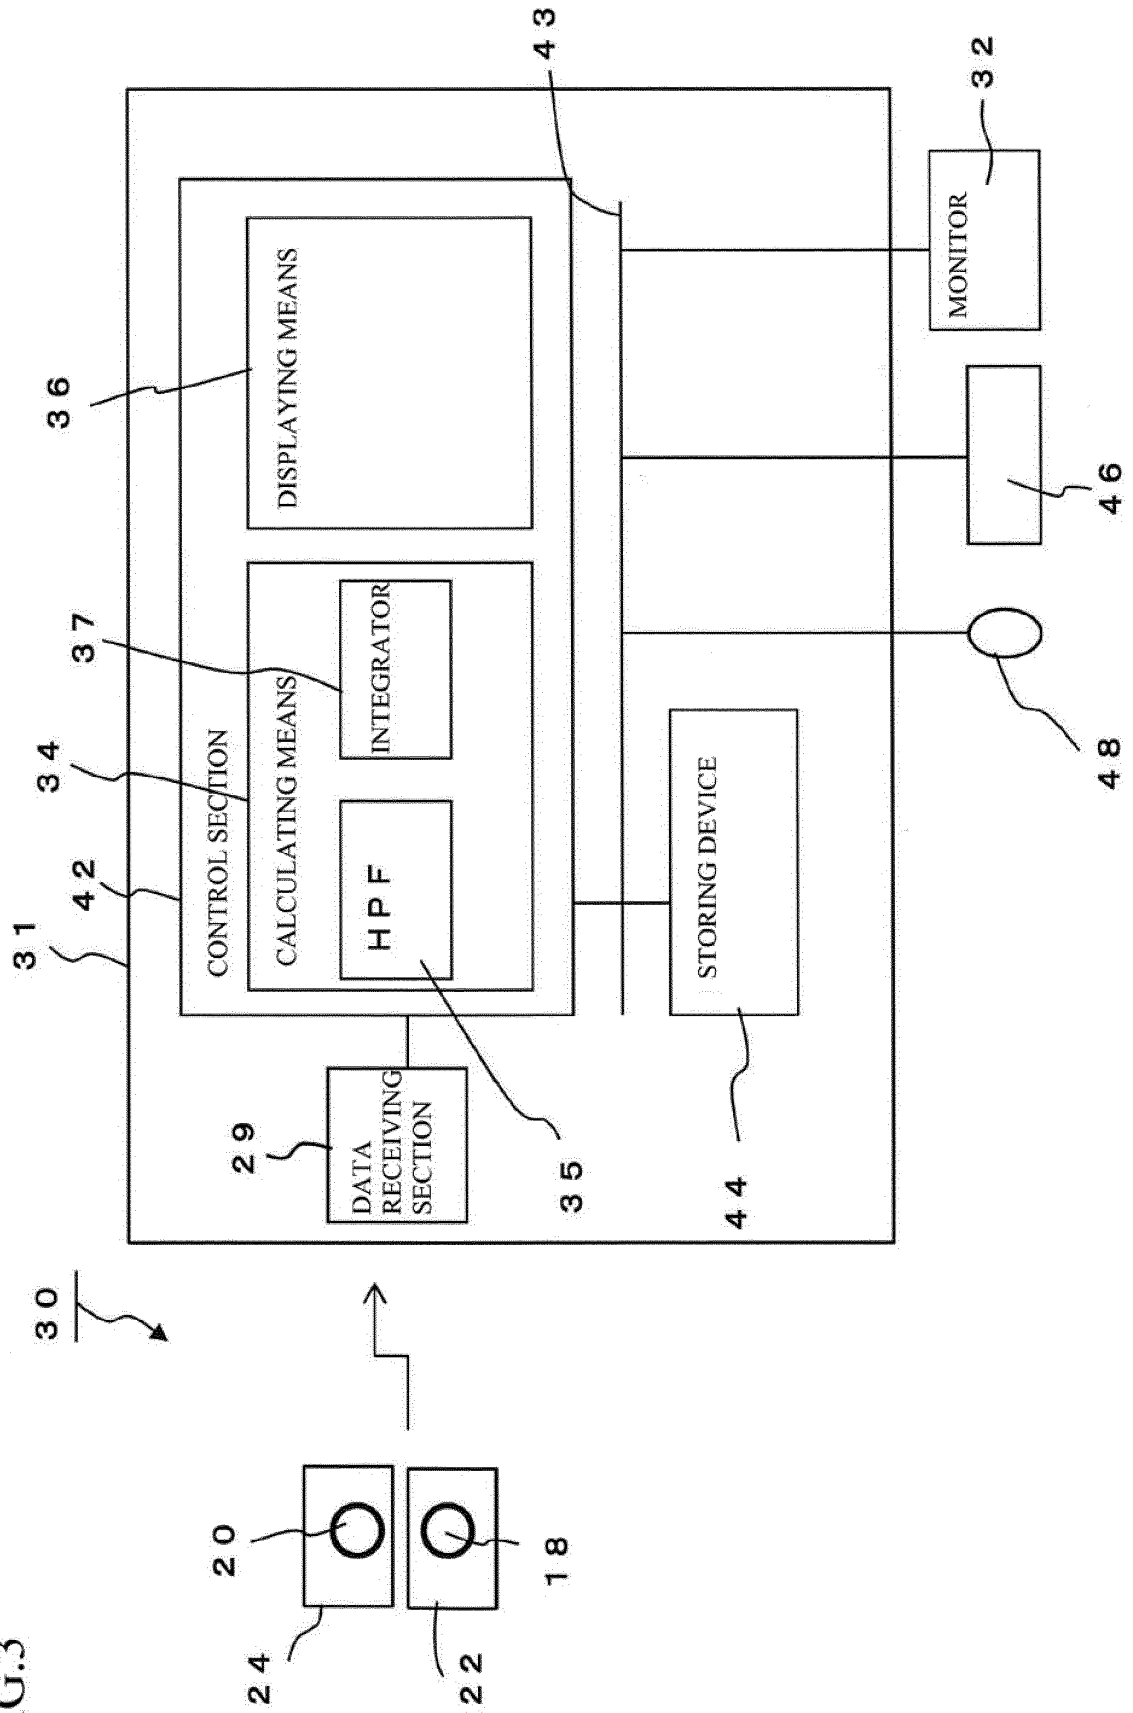


FIG.4

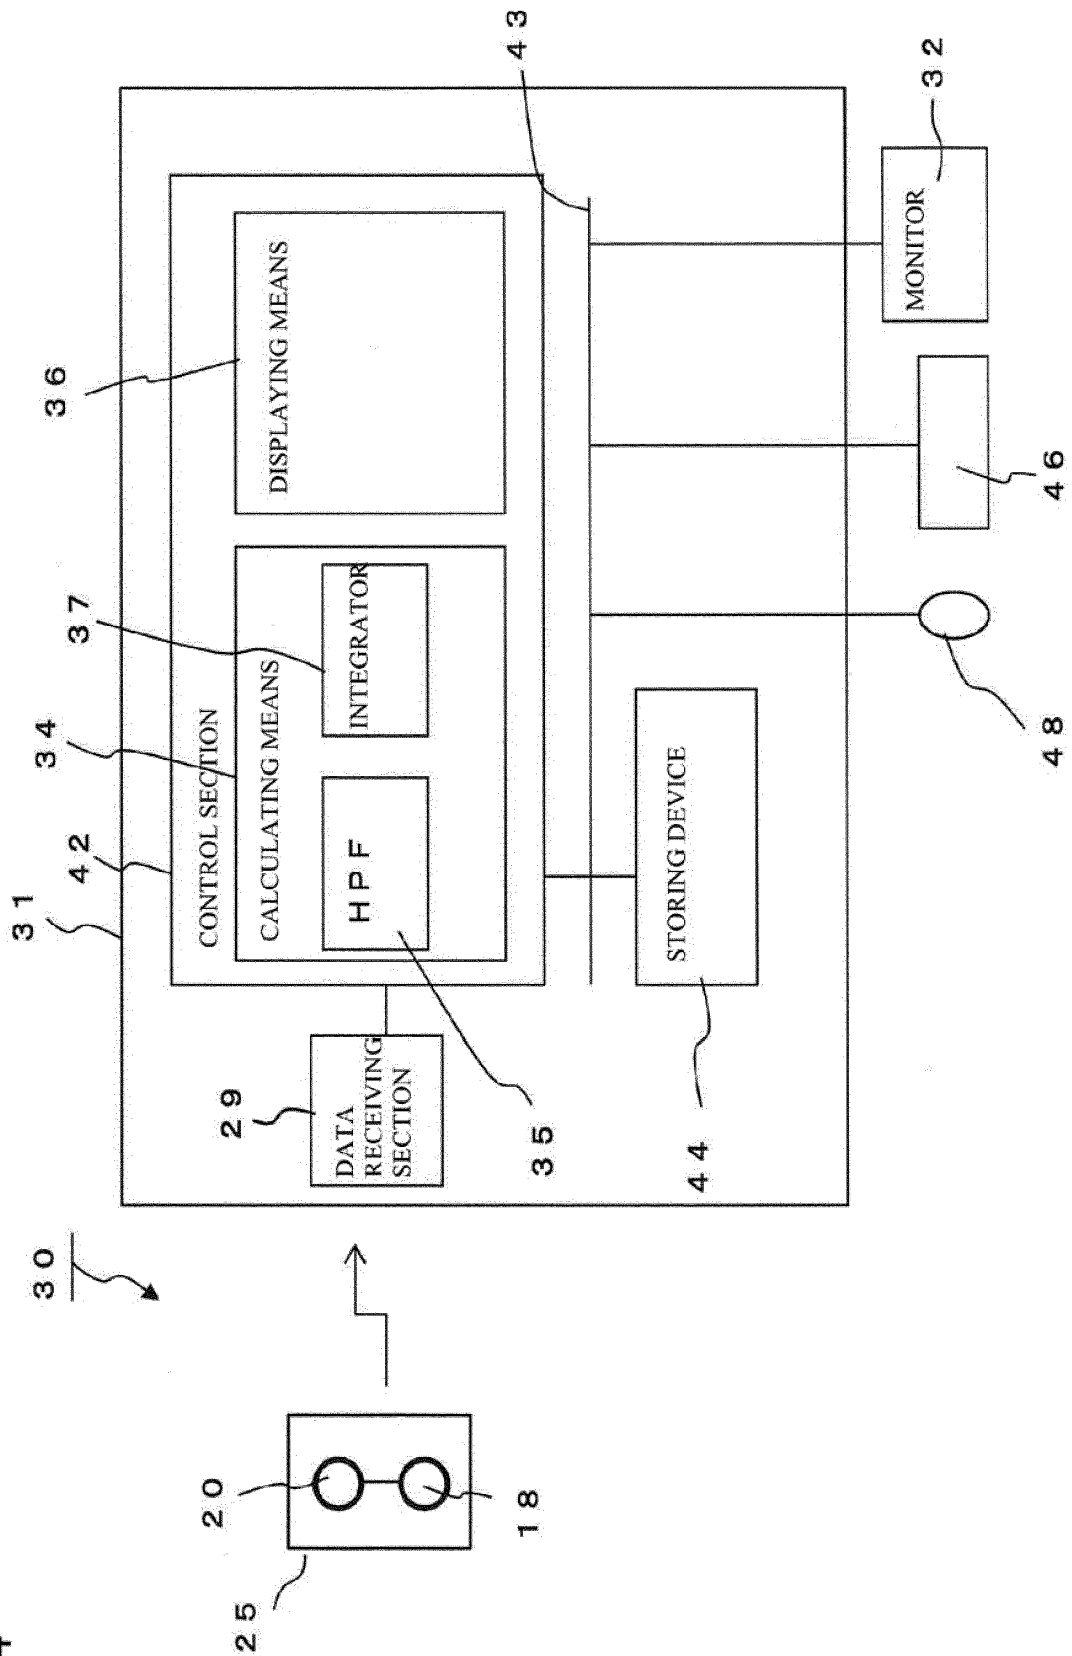


FIG.5

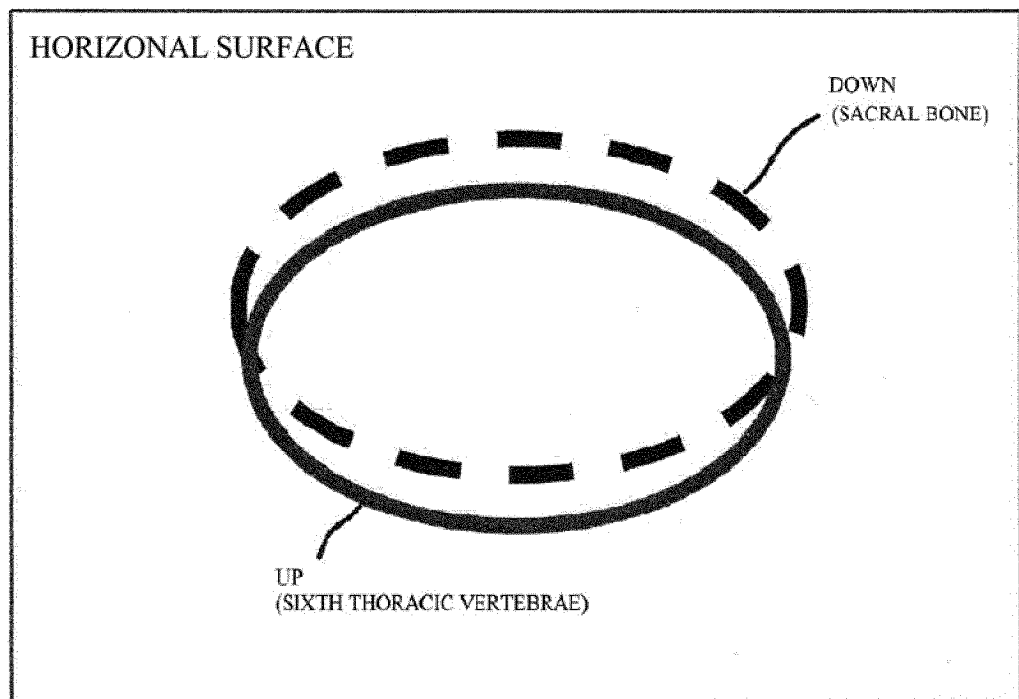


FIG.6

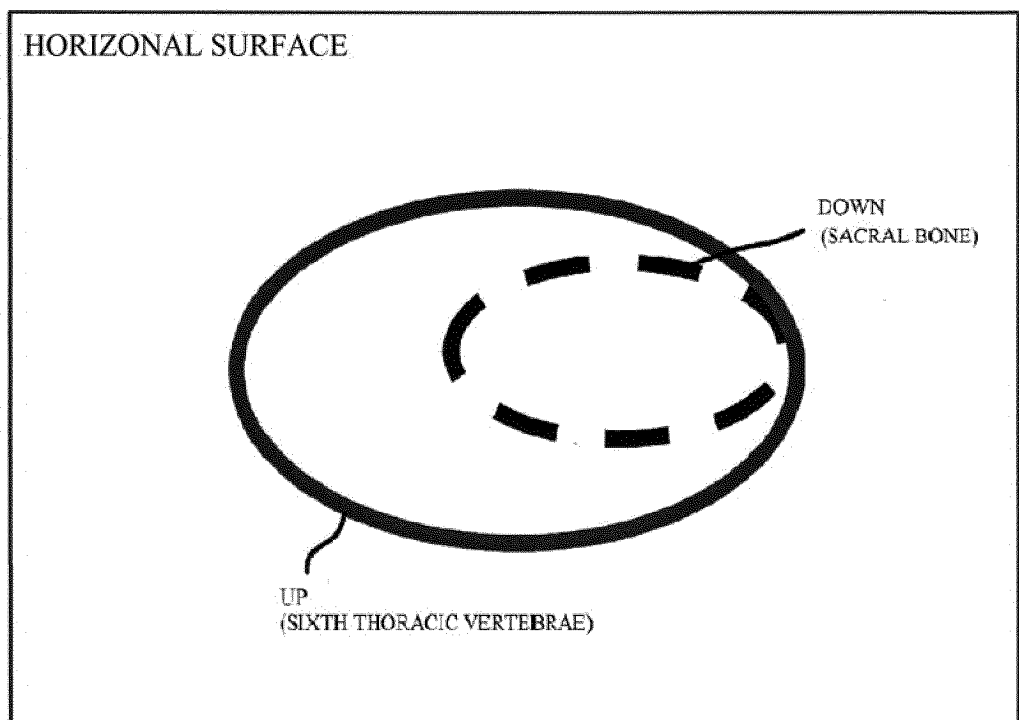


FIG.7

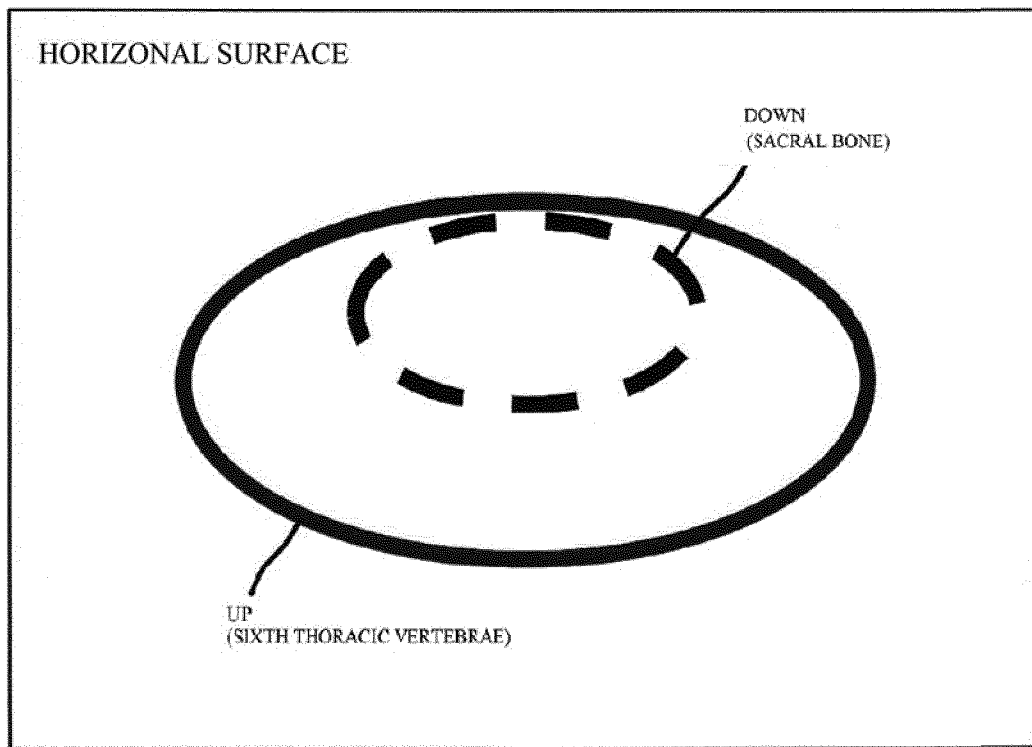


FIG.8

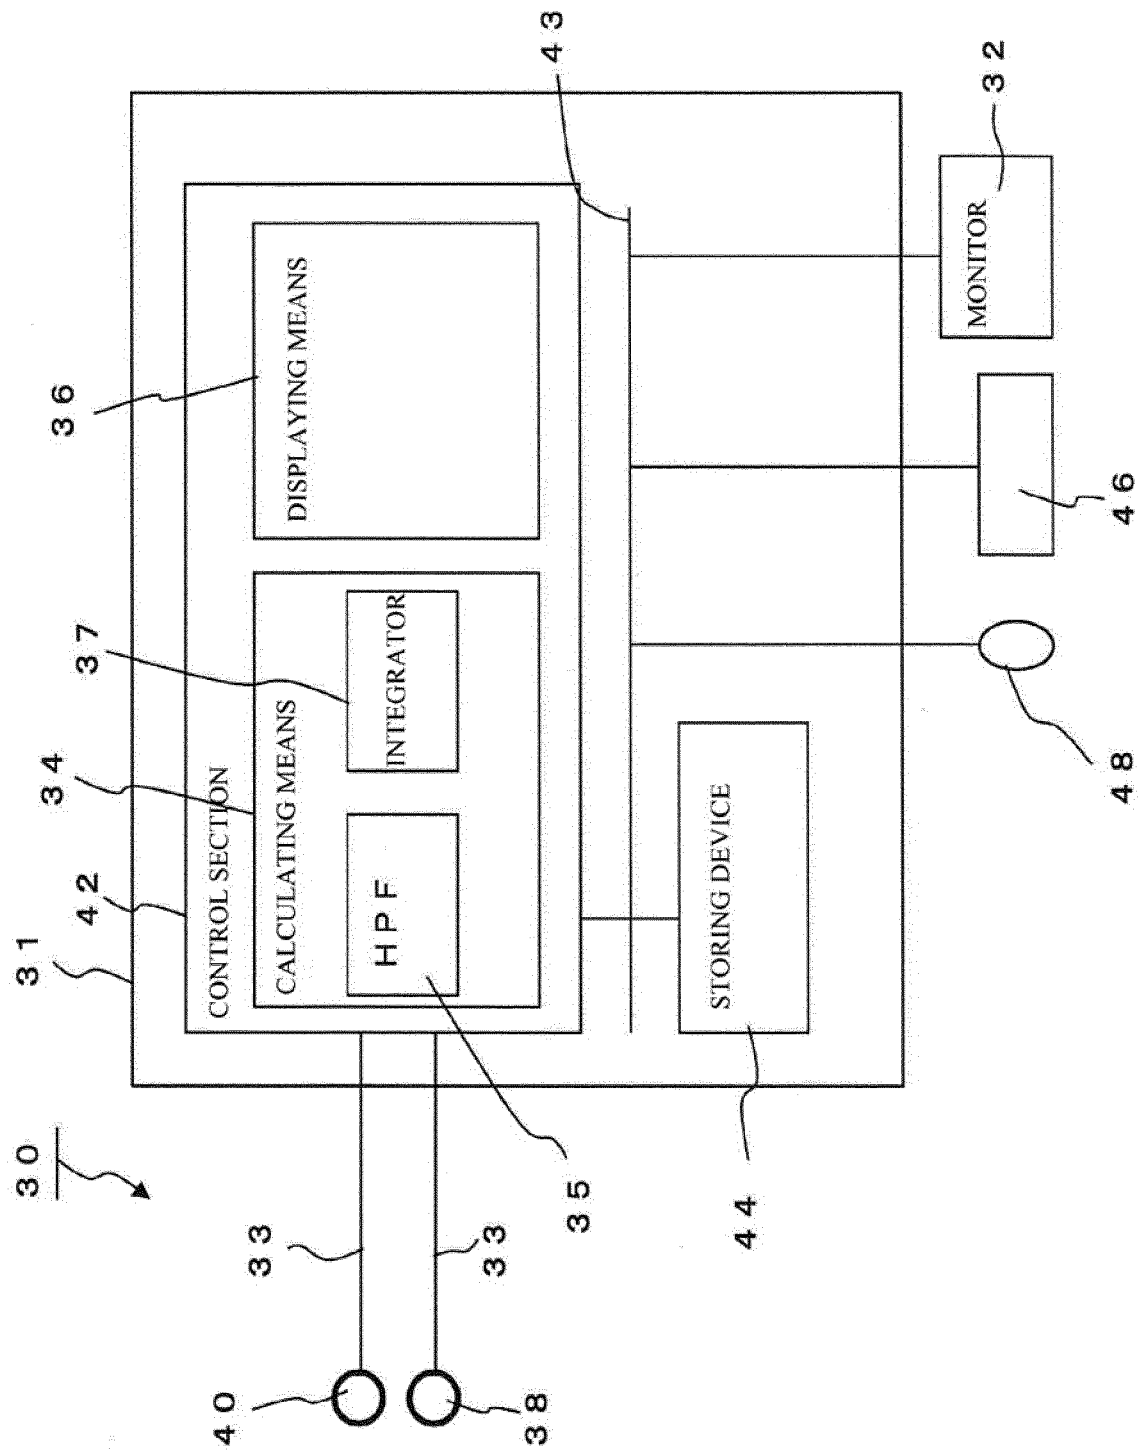


FIG.9

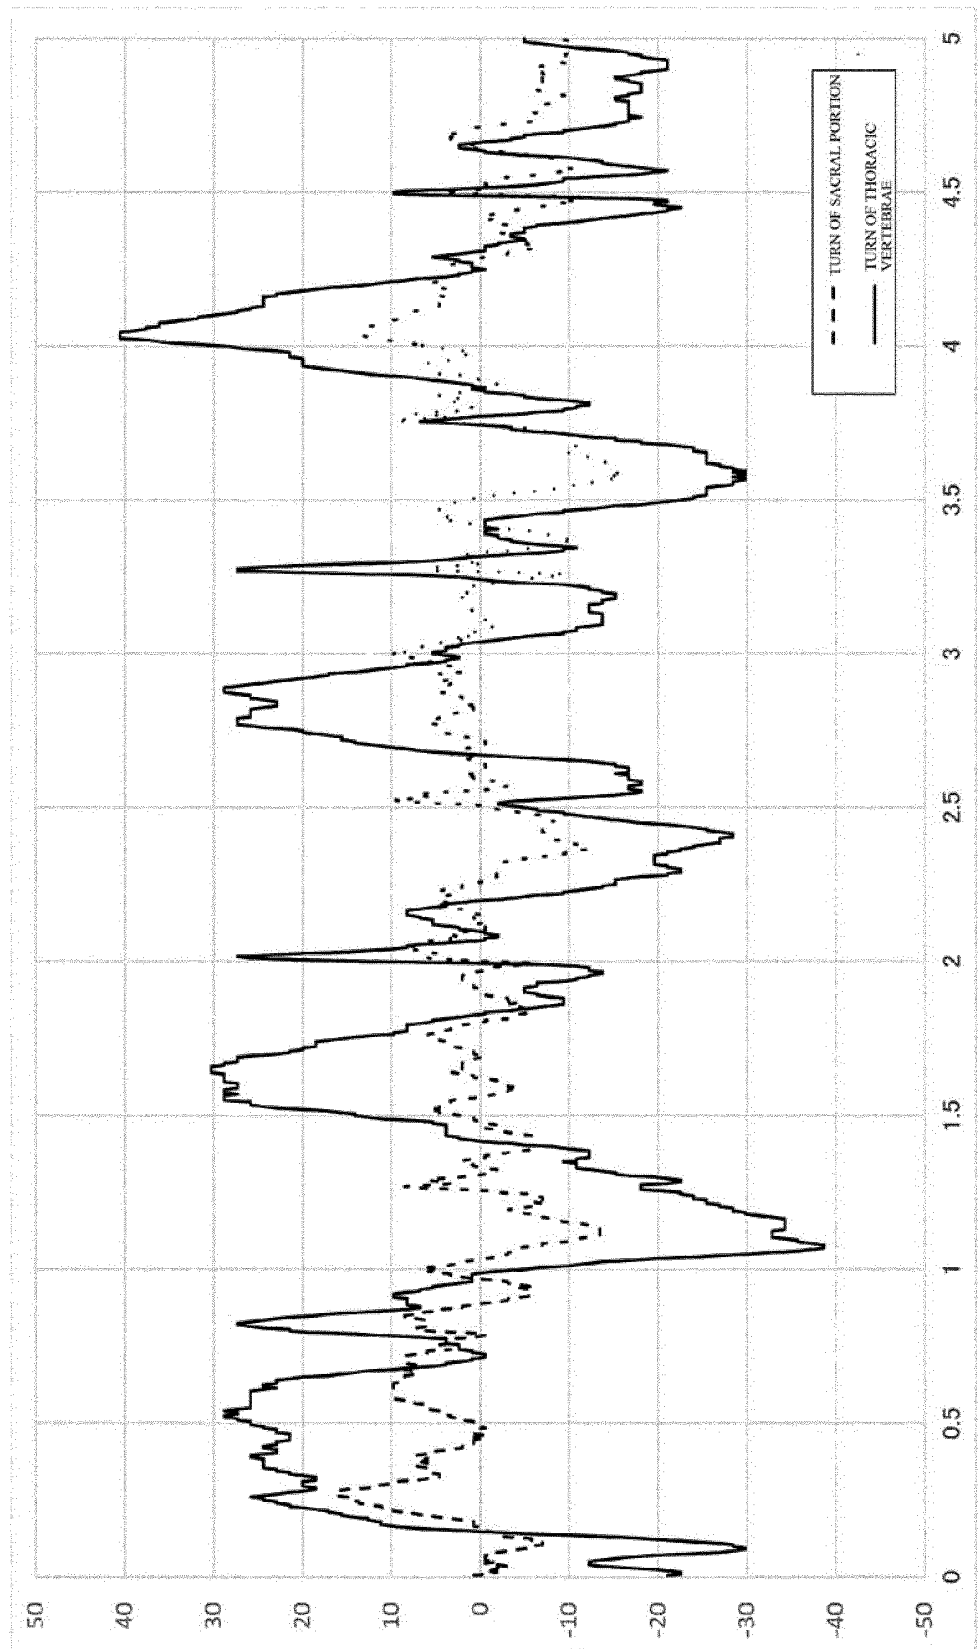


FIG.10

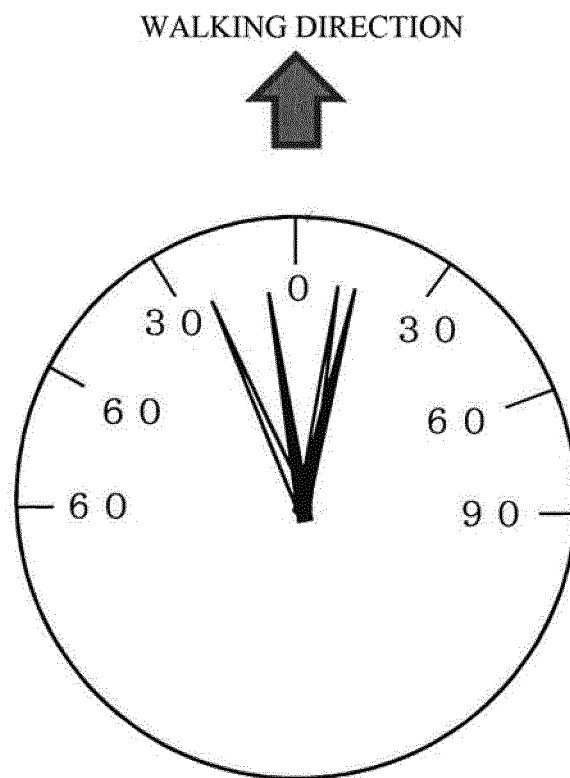


FIG.11

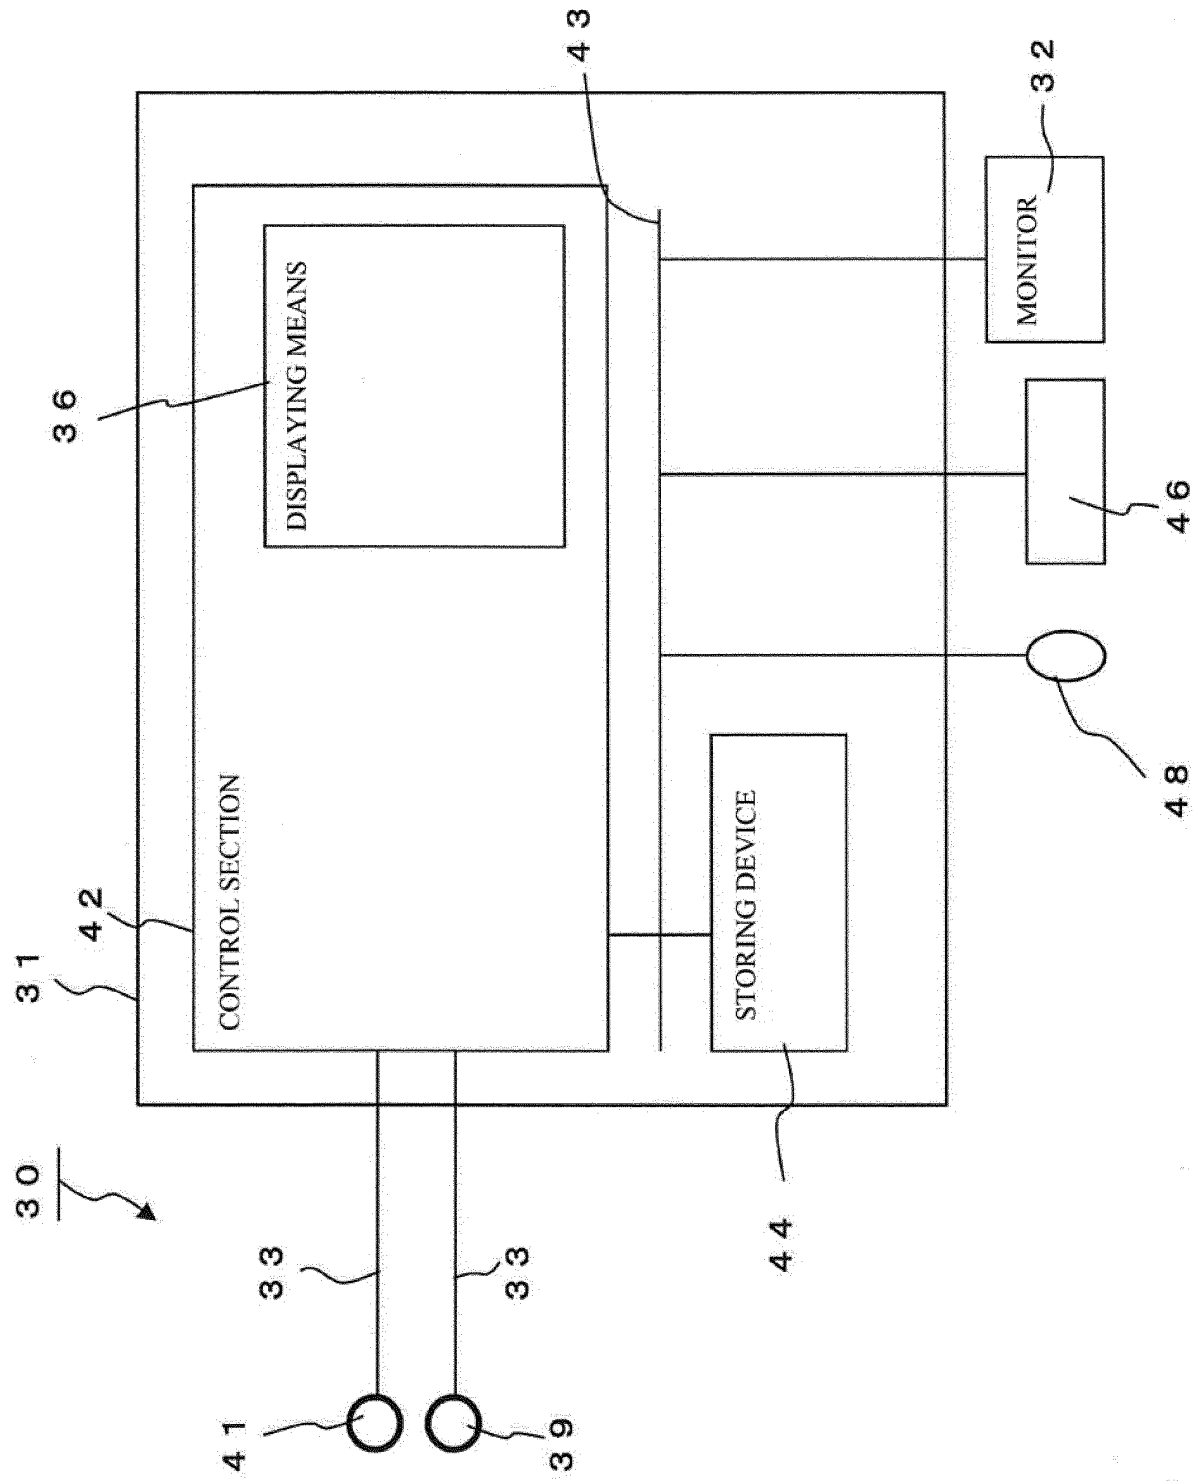


FIG.12

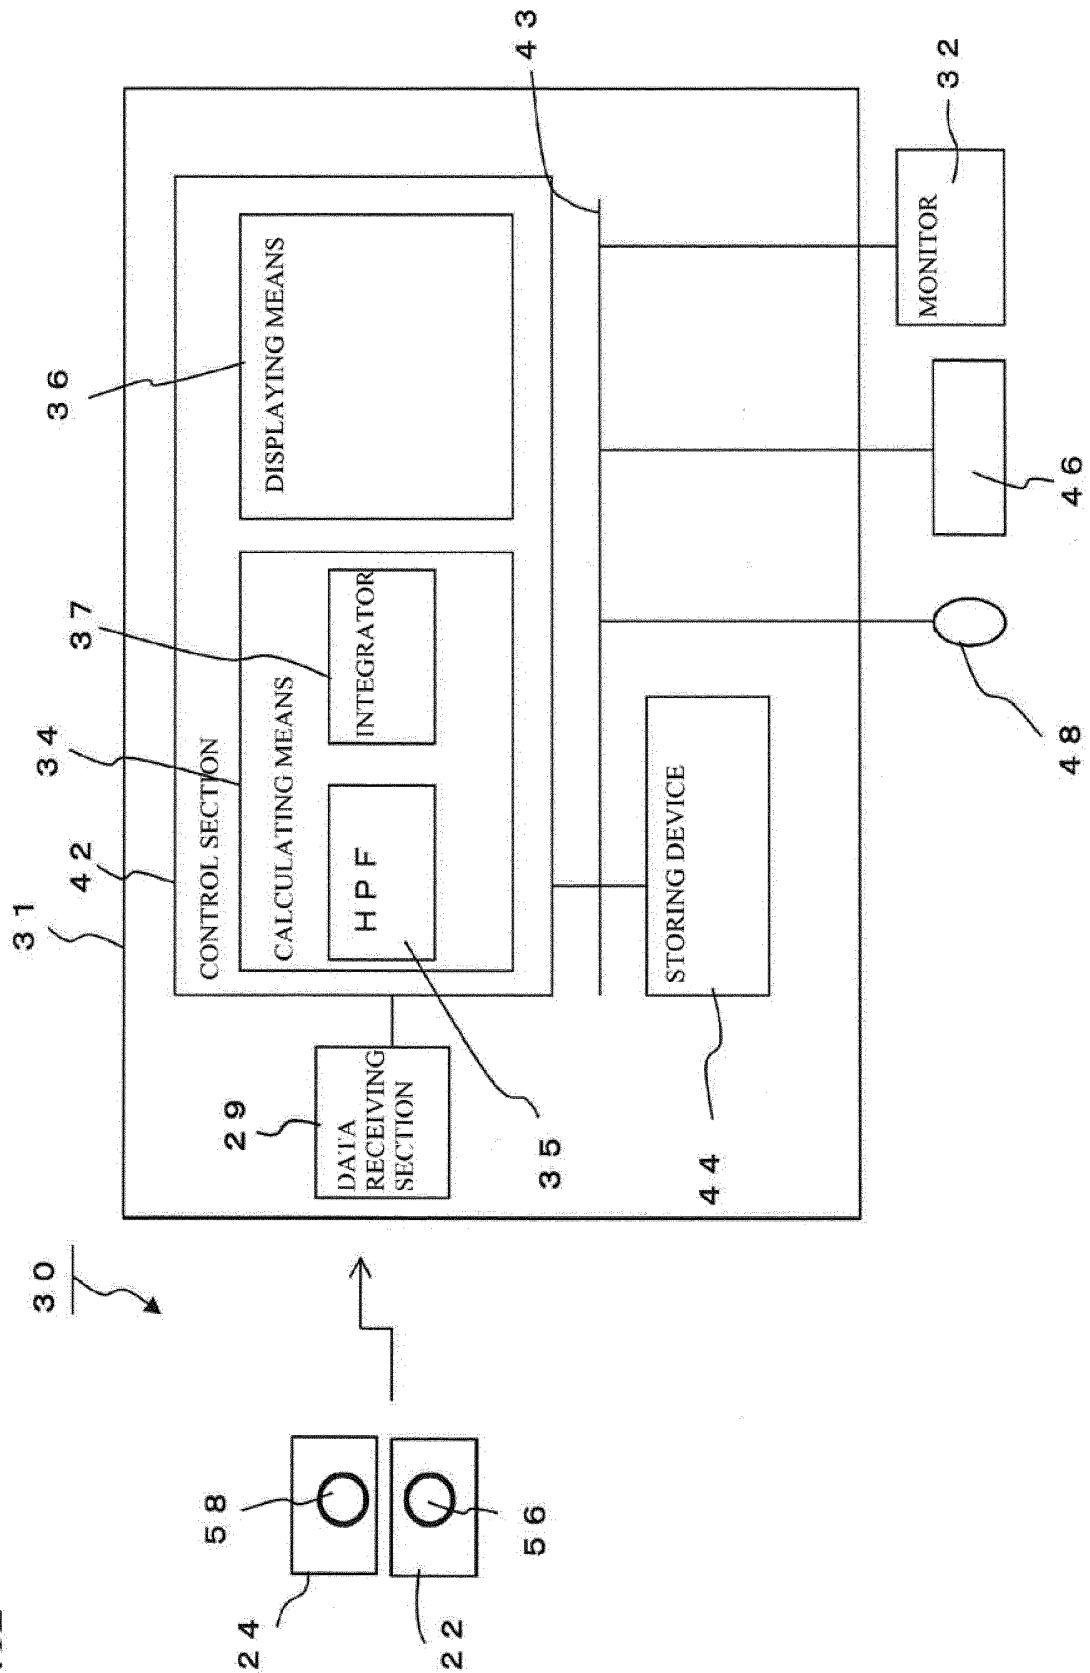


FIG.13

MicroStone®

Setup/Calibration Measure/Load Analysis/Save 2-Point Gait Oscillometer MVP-WS2-S Ver.1.1.2E

Connection/Setup

Sensor A (sacrum) COM35 Sensor B (dorsal vertebrae) COM34

Com.port COM35 %

Sensor setting 2G/2000dps ▾

60 Connection/Setup 61 Disconnect

* Attach the sensor unit to a power source and check that the LED is flashing red before connecting.

Calibration

Gravity calibration switch

☒ Simple Calibration ☐ Standard Calibration

Simple Calibration :
Fine-tunes the acceleration sensor offset and the gyroscope sensor offset from the sensor output when placed on a horizontal surface with the label side (+Z) uppermost.

Standard Calibration (Recommended) :
Fine-tunes the acceleration sensor offset, the gyroscope sensor offset and the sensitivity of the accelerometer sensor from the sensor output when each of the sensor's 6 sides are placed uppermost on a horizontal surface.

Calibration data collection

+X	-X	+Y	-Y	+Z	-Z
+X	-X	+Y	-Y	+Z	-Z

OK Sensor A OK Sensor B

62 Calibrate

* During calibration, only stable data is collected. Make sure that the sensor is horizontal and not subject to vibration (noise). (Calibration will time-out after 60 seconds.)

Gyroscope recalibration:
Repeats the fine-tuning of the gyroscope sensor offset only. The position of the sensor is not important, so long as it is stationary. To obtain measurements with a high degree of accuracy, it is recommended that fine-tuning be repeated every 15 minutes.

Gyroscope recalibration

Save calibration values Load calibration values

Sensor Information

Completed

Sensor A (sacrum) ID 0009E7024BF8 Sensor B (dorsal vertebrae) ID 0009E70254A2

Battery level 50~100% 50~100%

FIG.14

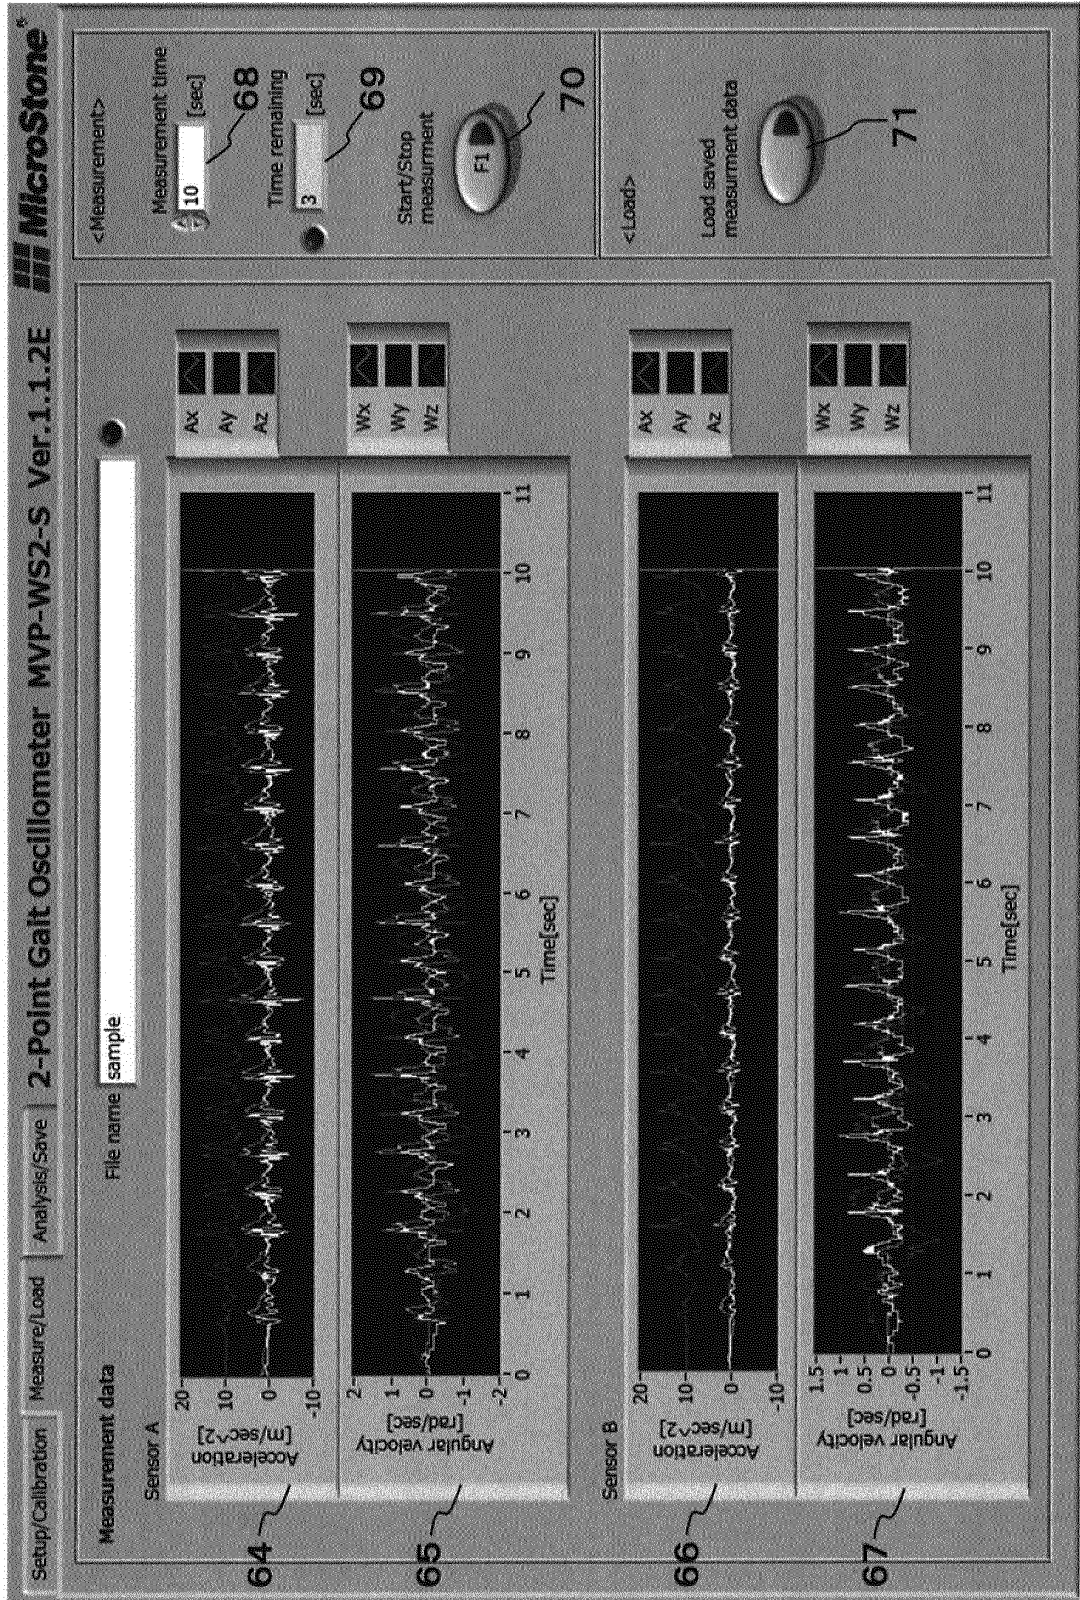


FIG.15

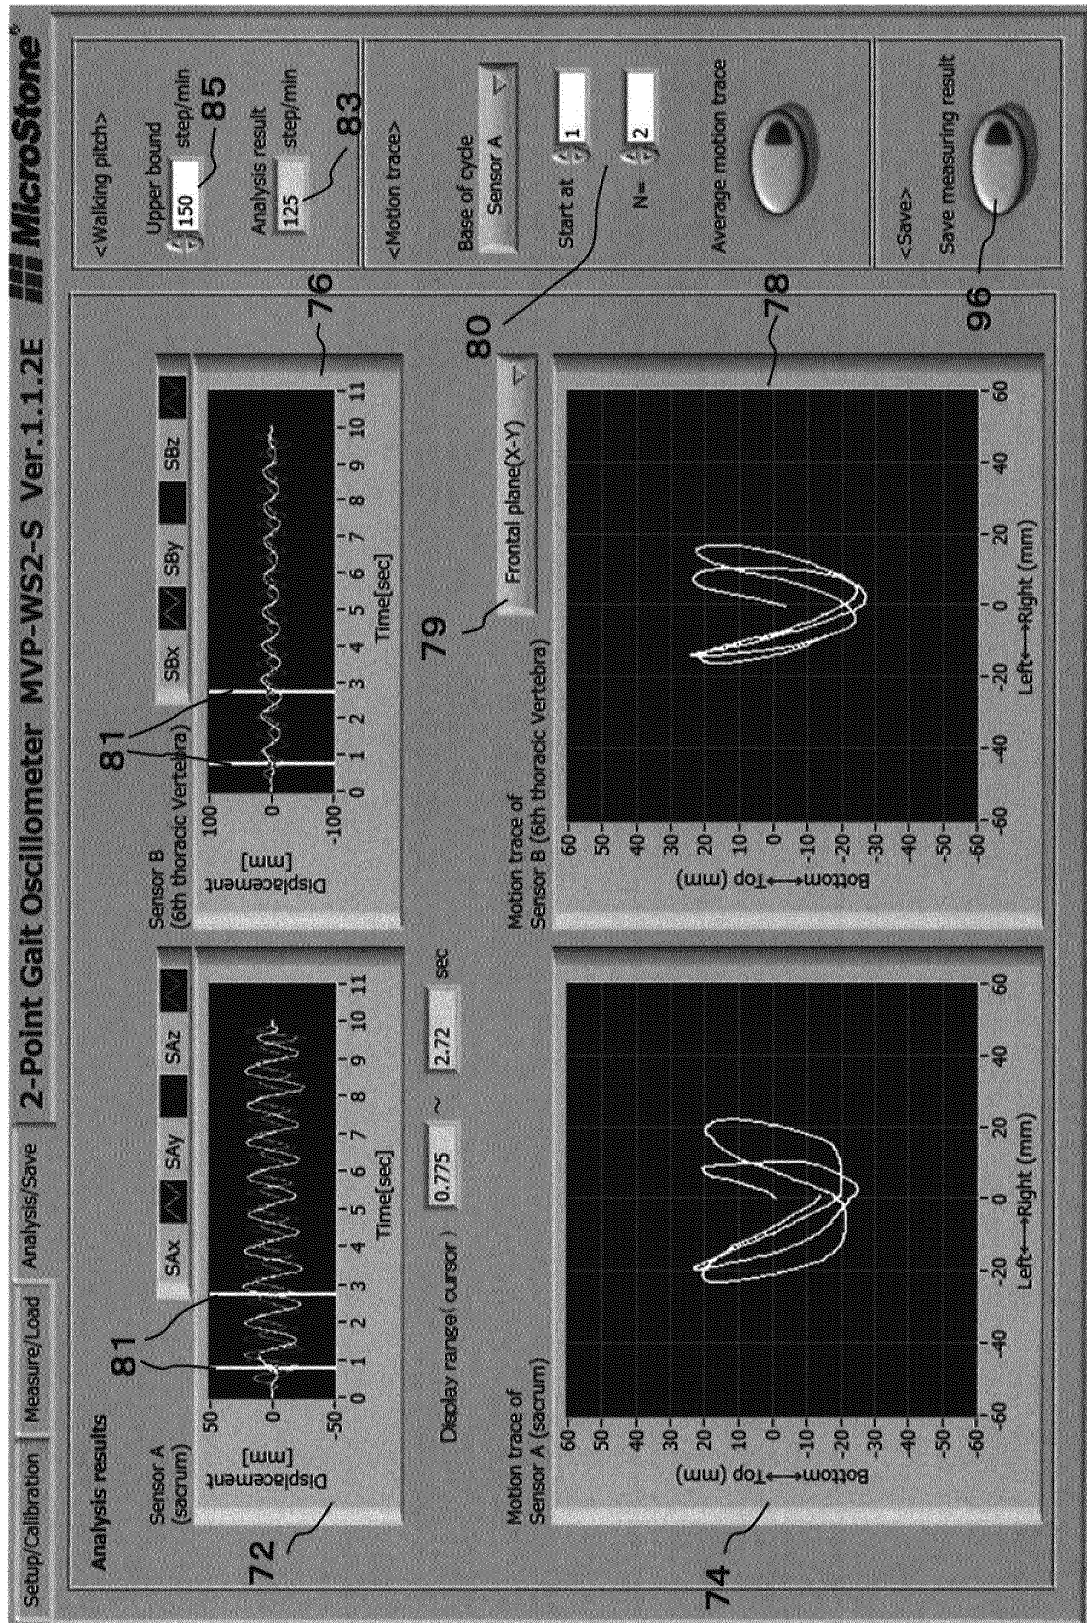


FIG.16


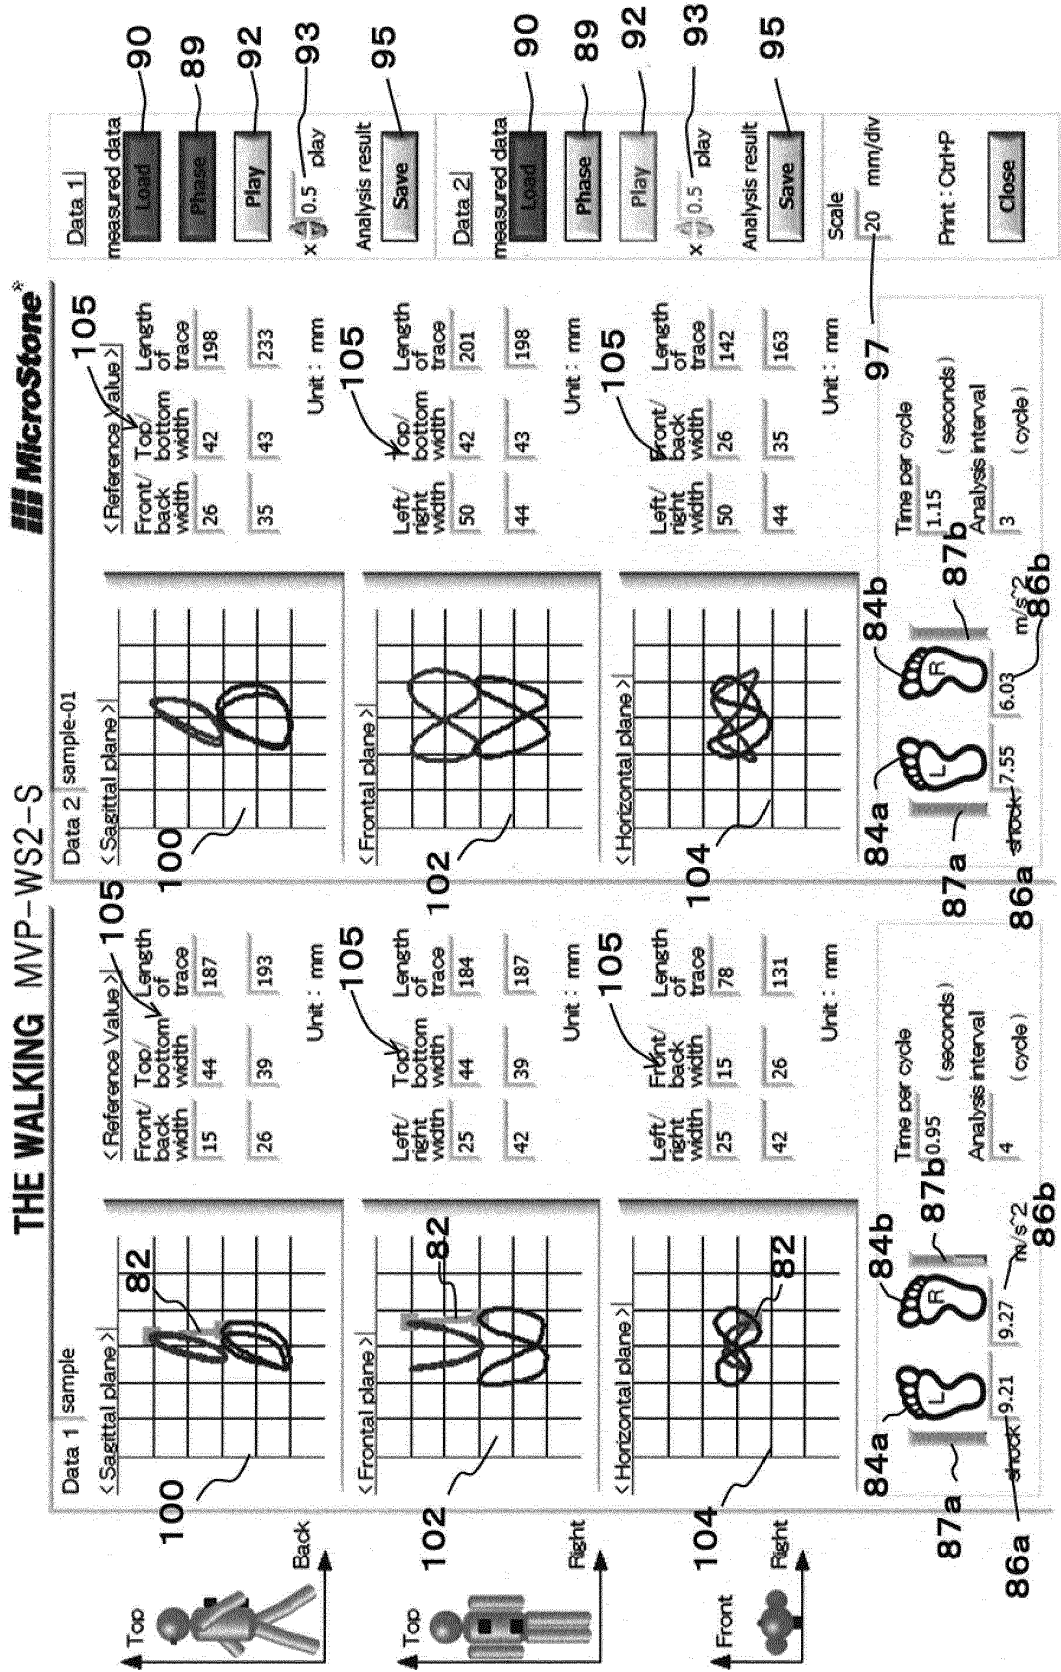


FIG.17

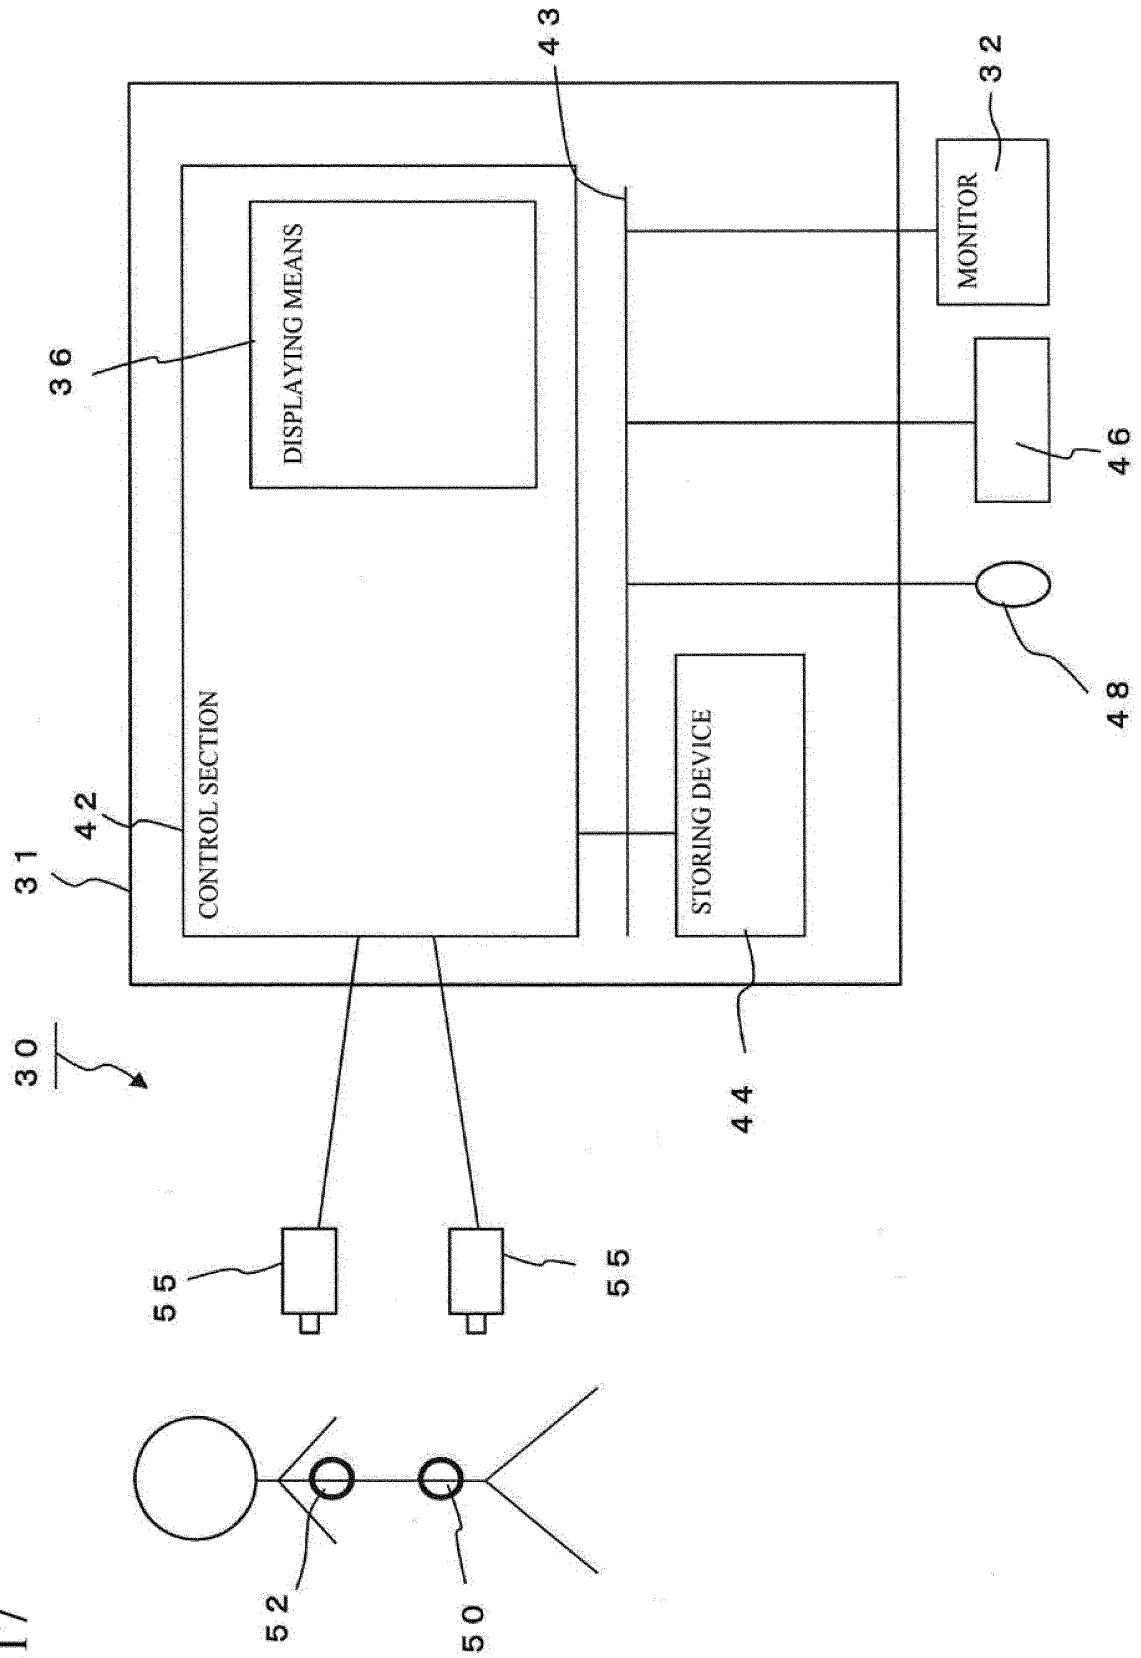

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 2012000343 A [0008]
- JP 2013059489 A [0008]
- US 2012101771 A [0008]

专利名称(译)	用于检测走动状态的装置		
公开(公告)号	EP3111840B1	公开(公告)日	2019-06-19
申请号	EP2015755345	申请日	2015-02-27
[标]申请(专利权)人(译)	微石有限公司 导演阿基拉		
申请(专利权)人(译)	MICROSTONE CORPORATION ICHIKAWA , AKIRA		
当前申请(专利权)人(译)	MICROSTONE CORPORATION ICHIKAWA , AKIRA		
[标]发明人	ICHIKAWA AKIRA SHIRATORI NORIHIKO OKADA SHIGEYA NOZAWA HIDETAKA		
发明人	ICHIKAWA, AKIRA SHIRATORI, NORIHIKO OKADA, SHIGEYA NOZAWA, HIDETAKA		
IPC分类号	A61B5/11 A61B5/00		
CPC分类号	A61B5/1127 A61B5/0024 A61B5/0077 A61B5/1116 A61B5/112 A61B5/1121 A61B5/1122 A61B5/1123 A61B5/1124 A61B5/6814 A61B5/6823 A61B5/6828 A61B5/7207 A61B5/725 A61B5/743 A61B5/7435 A61B2505/09 A61B2562/0219 A61B2562/0223		
代理机构(译)	MEWBURN ELLIS LLP		
优先权	2014039341 2014-02-28 JP		
其他公开文献	EP3111840A4 EP3111840A1		
外部链接	Espacenet		

摘要(译)

本发明解决了提供一种方法和装置的问题，利用该方法和装置，可以容易地检测包括上身运动的走动状态，而不需要在用于康复的医疗设施等中使用所用设备的复杂操作。在检测到受试者的走动状态的情况下（10），通过测量至少两个地方（特别是木材区域（12）和胸背区域）的运动条件来检测受试者的走动状态来解决该问题。14）主题。

FIG.1

