



Europäisches Patentamt
European Patent Office
Office européen des brevets



(11) **EP 1 174 083 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
15.11.2006 Bulletin 2006/46

(51) Int Cl.:
A61B 5/15^(2006.01)

(21) Application number: **01115603.1**

(22) Date of filing: **02.07.2001**

(54) **Thin lancet for test sensor**

Dünne Lanzette für Prüfsonde

Lance mince pour capteur de test

(84) Designated Contracting States:
**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE TR**

(30) Priority: **10.07.2000 US 216972 P**

(43) Date of publication of application:
23.01.2002 Bulletin 2002/04

(60) Divisional application:
04001740.2 / 1 417 929

(73) Proprietor: **BAYER CORPORATION
Pittsburgh, PA 15205-9741 (US)**

(72) Inventor: **Whitson, Robert C.
Goshen,
Indiana 46528 (US)**

(74) Representative: **Linhart, Angela
Bayer HealthCare AG
CAO Law & Patents,
Patents & Licensing
51368 Leverkusen (DE)**

(56) References cited:
**EP-A- 0 747 006 US-A- 3 659 608
US-A- 5 643 306**

EP 1 174 083 B1

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

FIELD OF THE INVENTION

[0001] The present invention relates to a thin lancet for obtaining a sample of blood.

BACKGROUND OF THE INVENTION

[0002] It is often necessary to quickly obtain a sample of blood and perform an analysis of the blood sample. One example of a need for painlessly obtaining a sample of blood is in connection with a blood glucose monitoring system where a user must frequently use the system to monitor the user's blood glucose level.

[0003] Those who have irregular blood glucose concentration levels are medically required to regularly self-monitor their blood glucose concentration level. An irregular blood glucose level can be brought on by a variety of reasons including illness such as diabetes. The purpose of monitoring the blood glucose concentration level is to determine the blood glucose concentration level and then to take corrective action, based upon whether the level is too high or too low, to bring the level back within a normal range. The failure to take corrective action can have serious implications. When blood glucose levels drop too low - a condition known as hypoglycemia - a person can become nervous, shaky, and confused. That person's judgment may become impaired and that person may eventually pass out. A person can also become very ill if their blood glucose level becomes too high - a condition known as hyperglycemia. Both conditions, hypoglycemia and hyperglycemia, are both potentially life-threatening emergencies.

[0004] One method of monitoring a person's blood glucose level is with a portable, hand-held blood glucose testing device. A prior art blood glucose testing device 100 is illustrated in FIG. 1. The portable nature of these devices 100 enables the users to conveniently test their blood glucose levels wherever the user may be. The glucose testing device contains a test sensor 102 to harvest the blood for analysis. The device 100 contains a switch 104 to activate the device 100 and a display 106 to display the blood glucose analysis results. In order to check the blood glucose level, a drop of blood is obtained from the fingertip using a lancing device. A prior art lancing device 120 is illustrated in FIG. 2. The lancing device 120 contains a needle lancet 122 to puncture the skin. Some lancing devices implement a vacuum to facilitate the drawing of blood. Once the requisite amount of blood is produced on the fingertip, the blood is harvested using the test sensor 102. The test sensor 102, which is inserted into a testing unit 100, is brought into contact with the blood drop. The test sensor 102 draws the blood to the inside of the test unit 100 which then determines the concentration of glucose in the blood. Once the results of the test are displayed on the display 106 of the test unit 100, the test sensor 102 is discarded. Each new test re-

quires a new test sensor 102.

[0005] One problem associated with some conventional lancing devices is that the user who regularly self-tests is required to carry at least two instruments - a lancet and a test unit. This places a greater burden on the user to remember to carry as well as to maintain two separate devices. Further, a greater amount of space is occupied on the user's person. There can also be an increased expense associated with two separate units.

[0006] Another problem associated with some conventional blood glucose monitoring devices is that the user's blood physically contacts the elements within the testing unit. Cross-contamination can be a problem if the monitoring device is used by more than one user such as in a doctor's office or other clinical setting.

[0007] EP 0 747 006 A1 discloses a lancet structure comprising a lancet member and an ejector. The lancet member includes a pricking member such as a blade or a needle and a lancet body having a pair of cantilevered arms. The ejector includes a compressible spring member and a U-shaped actuator the U-shaped actuator includes a base portion to which the compressible spring member is coupled and upstanding actuator arms are positioned pendicularly at both ends thereof. The opposite end of the spring member is attached to the lancet body. The lancet structure excluding the pricking member is made of a polymer. The pricking member is formed from stainless steel for like.

[0008] US 3,659,608 disclose a snap-acting surgical lancet which has a spring urging the forward ends of two opposed arms apart. A lower of the two arms carries a downwardly protruding lancing blade. Latching elements on the two arms hold them cocked with their front ends close together, and are releasable to allow the spring to snap the end of the lower arm downward, carrying the blade downward to lance the skin. A stop carried on one arm engages the other arm to limit this snap-apart travel of the arm ends. A single piece of spring material is readily formed to provide all of the foregoing structure, thereby providing a one-piece lancet.

[0009] US 5,643,306 disclose a single use disposable lancet device comprising housing and a spring mechanism pivotally mounted to the housing. The spring mechanism includes a sharpened end. The spring mechanism is mounted within the housing in a substantially unbiased state prior to use. An actuator for biasing the spring mechanism is movable, with respect to the housing, from an initial position to a biasing position to a locked position, in that order.

SUMMARY OF THE INVENTION

[0010] A lancet is provided for puncturing skin and producing a sample of blood. The lancet comprises a spring having a first end and a second end disposed between a U-shaped body with a needle and a base wherein the first end of integral spring is coupled to the base and the second end of the spring is coupled to the interior edge

of the U-shaped body and the needle is coupled to the exterior edge of the U-shaped body. The base, the spring, the U-shaped body and the needle are made out of a single piece of metal.

[0011] Additional features and benefits of the present invention will become apparent from the detailed description, figures, and claims set forth below.

BRIEF DESCRIPTION OF THE DRAWINGS

[0012] Other objects and advantages of the invention will become apparent upon reading the following detailed description in conjunction with the drawings in which

FIG. 1 is a top view of a prior art blood glucose testing device-;

FIG. 2 is a perspective view of a prior art lancet-;

FIG. 3 is a perspective view of a test sensor having a thin lancet according to one embodiment of the present invention;

FIG. 4 is front view of a thin lancet according to one embodiment of the present invention"

FIG. 5 is a perspective view of test sensor according to one embodiment of the present invention,

FIG. 6 is a cross-sectional view of the test sensor illustrated in FIG. 5;

FIG. 7 is an embodiment of a blood glucose monitoring system for use in conjunction with a test sensor having a thin lancet according to an alternative embodiment of the present invention"

FIG. 8 is a prospective view of an end cap and a blood glucose monitoring system for use in conjunction with a test sensor having a thin lancet according to a second alternative embodiment of the present invention;

FIG. 9a is a cross-sectional view of the end cap illustrated in FIG. 8; and

FIG. 9b is a cross-sectional view of the end cap illustrated in FIG. 8 with the thin lancet extended.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0013] Referring now to FIG. 3, a test sensor having a thin sensor and lancet ("sensor/lancet") 200 according to one embodiment of the present invention is illustrated. The sensor/lancet 200 includes a thin test sensor 202 and a thin lancet 203. The thin lancet 203 has a base 204 which is coupled to the test sensor 202. The remainder of the thin lancet 203 is movable allowing a thin needle 206 to travel downward to puncture a user's skin in order to produce a drop of the user's blood. The test sensor 202 has an inlet 208 through which blood is moved by capillary action into the test sensor 202. The test sensor 202 and the lancet 203 are generally thin and flat and each have a thickness of approximately 0.015 cm (0.006 inch).

[0014] Referring also to FIG. 4, the thin lancet 203 of

the sensor/lancet 200 will be described in greater detail. The thin lancet 203 is formed out of a single piece of metal. A thin spring 212 couples the base 204 to a U-shaped member 216. The spring 212 has a first end 218 and a second end 220, the first end 218 of which is coupled to the base 204 and the second end is coupled to an interior 222 of the U-shaped member 216. The thin needle 206 is formed on an exterior 224 of the U-shaped member. The two sides of the U-shaped member are force receiving members 232,234 for providing movement to the thin needle 206.

[0015] In operation, when a user is testing the glucose concentration of blood, the test sensor 202 remains stationary within a testing device while a force is imparted on to a top portion 236,238 of each force receiving member 232,234. The force receiving members 232,234 are driven downward thus forcing the needle 206 downward into the user's skin. Once the force is removed from the force receiving members 232,234, the spring 212 retracts the needle 206 from the user's skin.

[0016] Referring also to FIGS. 5 and 6, the thin test sensor 202 will be described in greater detail. The test sensor 202 comprises a test chamber having a test area 240 disposed between a front panel 242 and a rear panel 244. The test area 240 is designed to allow blood to move from the inlet 208 up the test area 240 via capillary action. An adhesive 246 is disposed on the front panel 242 to adhere the base 204 of the thin lancet 203 to the front panel 240.

[0017] A reagent is incorporated into the test sensor 202. The reagent is designed to react with the glucose in the blood which moves up the test area 240. The reaction produces a detectable signal which is indicative of the glucose concentration in the sample of blood. That signal is then measured by a sensor which can measure the concentration of the glucose in the blood based on the signal. The specific reagent incorporated into the test sensor 202 is a function of the type of sensing employed to determine the concentration of glucose in the blood. In the illustrated embodiment of the test sensor 202, electrochemical sensing is employed. The test sensor 202 includes a pair of electrodes 250 (FIG. 6). In electrochemical analysis, the change in current across the electrodes 250 caused by the reaction of the glucose and the reagent is indicative of the concentration of the glucose in the blood. The reaction of the glucose and the reagent creates an oxidation current at the electrodes 250 which is directly proportional to the user's blood glucose concentration. This current can be measured by an appropriate sensor coupled to a pair of terminals 252 corresponding to the electrodes 250 implemented in a glucose monitoring device for use with the sensor/lancet 200. The glucose monitoring device can then communicate to the user the blood glucose concentration. An example of an electrochemical testing system is described in detail by commonly-owned U.S. Patent No. 5,723,284 entitled "Control Solution and Method for Testing the Performance of an Electrochemical Device for Determining the

Concentration of an Analyte in Blood".

[0018] Referring now to FIG. 7, an application of the sensor/lancet 200 is in an integrated blood glucose monitoring system 300 which integrates the lancing, the blood harvesting, and a blood glucose analyzer into a single instrument. The integrated blood glucose monitoring system 300 contains a plurality of sensors/lancets 200 for use in a plurality of blood glucose self-tests. In operation, a user would activate the system 300 with a switch 304. A new thin sensor/lancet 200 is advanced to the test end 302 of the system 300. The user would then press the test end 302 of the system against the user's skin and depress a trigger 306 causing a spring loaded member (not shown) to apply a force to the force receiving members 232,234 of the thin lancet 203. The needle 206 would then extend through an opening 308 in the test end 302 of the system 300 to puncture the user's skin. After the needle 206 is fully extended out of the opening 308, the spring 214 would withdraw the needle from the laceration created in the user's skin through the opening 308. Blood emerging from the laceration created in the user's skin is moved from the inlet 208 by capillary action into the test sensor 202. Once the requisite blood sample has been obtained and the requisite time has elapsed for the reaction in the test sensor 202 to take place, the blood glucose monitoring system 300 measures the signal produced by the reaction and determines the blood glucose concentration of the blood sample. The results of the analysis are communicated to the user via a display 310. The sensor/lancet 200 is then ejected from the system 300 and discarded.

[0019] Referring now to FIGS. 8, 9a, and 9b, another application of the sensor/lancet 200 is in a disposable, protective end cap 350. In a clinical setting, such as a medical doctor's office where the user is a doctor, nurse, or technician seeing multiple patients, cross contamination is a serious concern. Obviously, components of medical devices which come into contact with one patient's blood can not come into contact with the user or another patient. The end cap 350 protects those who handle the end cap 350 from coming into contact with the needle 206 and any blood disposed thereon after the sensor/lancet 200 within the end cap 350 have been used. Only when actuated (during testing), does the needle 206 extend beyond the area bounded by the end cap 350. Accordingly, a user (doctor, nurse, technician) is protected from being punctured with the needle 206 when connecting the end cap 350 to or removing the end cap 350 from the sensor/lancet 200.

[0020] A blood glucose monitoring system 360 for use with the disposable end cap 350 having a sensor/lancet 200 disposed therein is also illustrated in FIG. 8. The device 360 contains a switch 362 to activate the device 360. A trigger 364 is provided to fire a spring loaded plunger 366 to contact the force receiving members 232,234 which in turn provide movement to the needle 206. The when actuated, the spring loaded plunger 366 rapidly moves downward a predetermined distance to

move the force receiving members 232,234 and in turn the needle 206 a predetermined distance causing the needle 206 to extend beyond a test end 352 of the end cap 350 a distance about equal to the needle 206 penetration depth. The distance that the needle 206 extends beyond the test end 352 of the end cap 350 is preferably a distance sufficient to draw a sample of blood for analysis. Once the plunger forces the needle downward, the spring loaded plunger 366 retracts a distance allowing the needle 206 to retract back within the bounds of the disposable end cap 350. Meanwhile, the sample of blood moves through the inlet 208 disposed adjacent to the test end 352 of the end cap 350) of the test sensor 202. Once the requisite blood sample has been obtained and the requisite time has elapsed for the reaction in the test sensor 202, the blood glucose monitoring system 360 measures the signal produced by the reaction and determines the blood glucose concentration of the blood sample. The results of the analysis are communicated to the user via a display 368. The end cap 350 containing the used sensor/lancet 200 is then removed from the system 300 and discarded. The end cap 350 and the blood glucose monitoring system 360 have suitable connectors 370, 372 for mating the end cap 350 with the blood glucose monitoring system 360.

[0021] Thus far, only electrochemical analysis to determine the glucose concentration of a blood sample has been discussed in conjunction with the present invention. However, the thin sensor/lancet 200 of the present invention can be used with other types of blood glucose testing methods. For example, colorimetric testing may be implemented in the test sensor in conjunction with an alternative embodiment of the present invention. Colorimetric testing is described in commonly-owned U.S. Patent No. 5,723,284 entitled "Control Solution and Method for Testing the Performance of an Electrochemical Device for Determining the Concentration of an Analyte in Blood".

[0022] While the invention is susceptible to various modifications and alternative forms, specific embodiments thereof have been shown by way of example in the drawings and will be described in detail herein. It should be understood, however, that it is not intended to limit the invention to the particular forms disclosed, but, to the contrary, the intention is to cover all modifications, equivalents and alternatives falling within the scope of the invention as defined by the appended claims.

Claims

1. A lancet (203) comprising:

- a base (204),
- a spring (212) having a first end and a second end, the first end of the spring (212) coupled to the base (204),
- a needle (206) coupled to the second end (220)

of the spring (212), and
a U-shaped body (216) disposed between the
second end (220) of the spring (212) and the
needle (206), the U-shaped body (216) having
an interior edge (222) and an exterior edge (224),
the second end (220) of the spring (212) being
coupled to the interior edge (222), the needle
(206) being coupled to the exterior edge (224),

characterized in that

the base (204), the spring (212), the U-shaped body
(216), and the needle (212) are made out of a single
piece of metal.

2. The lancet (203) of claim 1 wherein the base (204),
the spring (212), the U-shaped body (216), and the
needle (206) are generally flat.
3. The lancet (203) of claim 1 or 2 wherein lancet (203)
has a thickness of about 0,015 cm (0,006 inch).
4. The lancet (203) of one of the claims 1 to 3 further
comprising a test sensor (202) for use in the deter-
mination of the concentration of a chemical in blood,
the base (204) being attached to the test sensor
(202) such that an inlet (208) of the test sensor (202)
is disposed proximate the needle (206).

Patentansprüche

1. Lanzette (203), umfassend:

eine Basis (204),
eine Feder (212) mit einem ersten Ende und ei-
nem zweiten Ende, wobei das erste Ende der
Feder (212) mit der Basis (204) verbunden ist,
eine Nadel (206), die mit dem zweiten Ende
(220) der Feder (212) verbunden ist, und
einen U-förmigen Körper (216), der zwischen
dem zweiten Ende (220) der Feder (212) und
der Nadel (206) angeordnet ist, wobei der U-
förmige Körper (216) einen inneren Rand (222)
und einen äußeren Rand (224) aufweist, worin
das zweite Ende (220) der Feder (212) mit dem
inneren Rand (222) verbunden ist und die Nadel
(206) mit dem äußeren Rand (224) verbunden
ist,

dadurch gekennzeichnet, dass

die Basis (204), die Feder (212), der U-förmige Kör-
per (216) und die Nadel (212) aus einem einzigen
Stück Metall bestehen.

2. Lanzette (203) nach Anspruch 1, worin die Basis
(204), die Feder (212), der U-förmige Körper (216)
und die Nadel (206) im Allgemeinen flach sind.

3. Lanzette (203) nach Anspruch 1 oder 2, worin die
Lanzette (203) eine Dicke von etwa 0,015 cm (0,006
Zoll) aufweist.

4. Lanzette (203) nach einem der Ansprüche 1 bis 3,
die weiters einen Testsensor (202) zur Verwendung
bei der Bestimmung der Konzentration einer Chemi-
kalie in Blut umfasst, wobei die Basis (204) am Test-
sensor (202) befestigt ist, sodass ein Einlass (208)
des Testsensors (202) sehr nahe an der Nadel (206)
angeordnet ist.

Revendications

1. Lancette (203) comprenant :

une base (204),
un ressort (212) ayant une première extrémité
et une seconde extrémité, la première extrémité
du ressort (212) étant couplée à la base (204),
une aiguille (206) couplée à la seconde extré-
mité (220) du ressort (212), et
un corps en forme de U (216) disposé entre la
seconde extrémité (220) du ressort (212) et
l'aiguille (206), le corps en forme de U (216)
ayant un bord intérieur (222) et un bord extérieur
(224), la seconde extrémité (220) du ressort
(212) étant couplée au bord intérieur (222),
l'aiguille (206) étant couplée au bord extérieur
(224),

caractérisée en ce que

la base (204), le ressort (212), le corps en forme de
U (216), et l'aiguille (212) sont réalisés à partir d'un
seul morceau de métal.

2. Lancette (203) selon la revendication 1, dans laquel-
le la base (204), le ressort (212), le corps en forme
de U (216) et l'aiguille (206) sont généralement plats.
3. Lancette (203) selon la revendication 1 ou 2, dans
laquelle la lancette (203) présente une épaisseur
d'environ 0,015 cm (0,006 pouce).
4. Lancette (203) selon l'une des revendications 1 à 3,
comprenant en outre un capteur de test (202) à uti-
liser pour la détermination de la concentration d'une
espèce chimique dans le sang, la base (204) étant
fixée au capteur de test (202), de sorte qu'une entrée
(208) du capteur de test (202) soit disposée à proxi-
mité de l'aiguille (206).

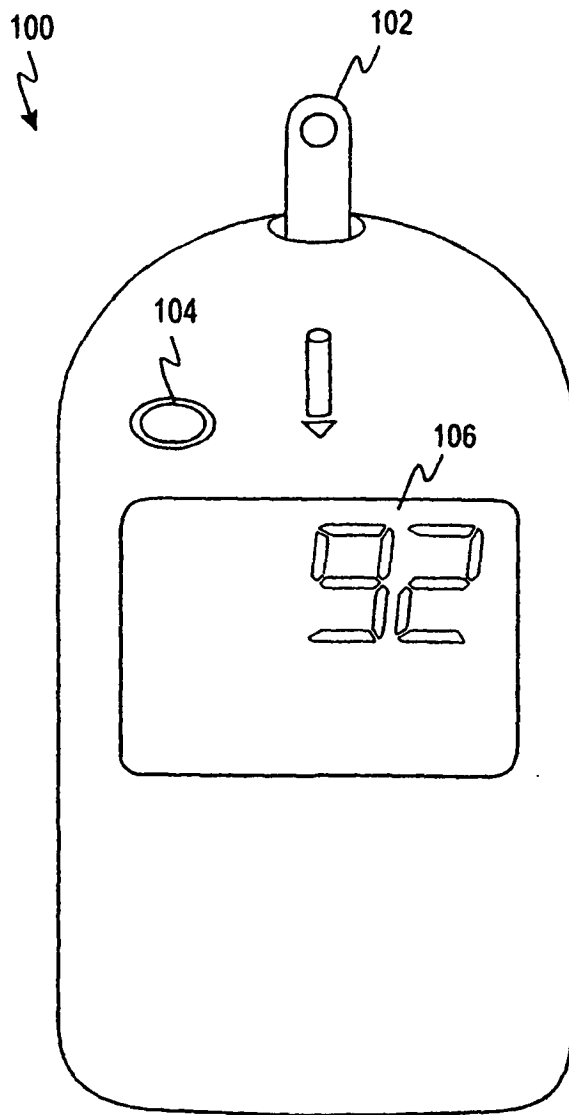


FIG. 1
(Prior Art)

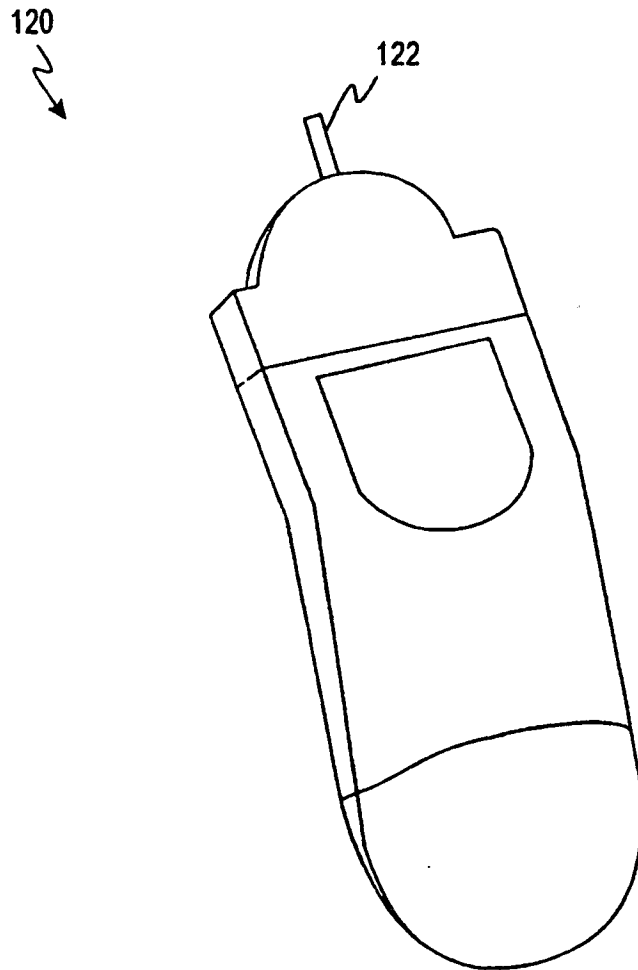
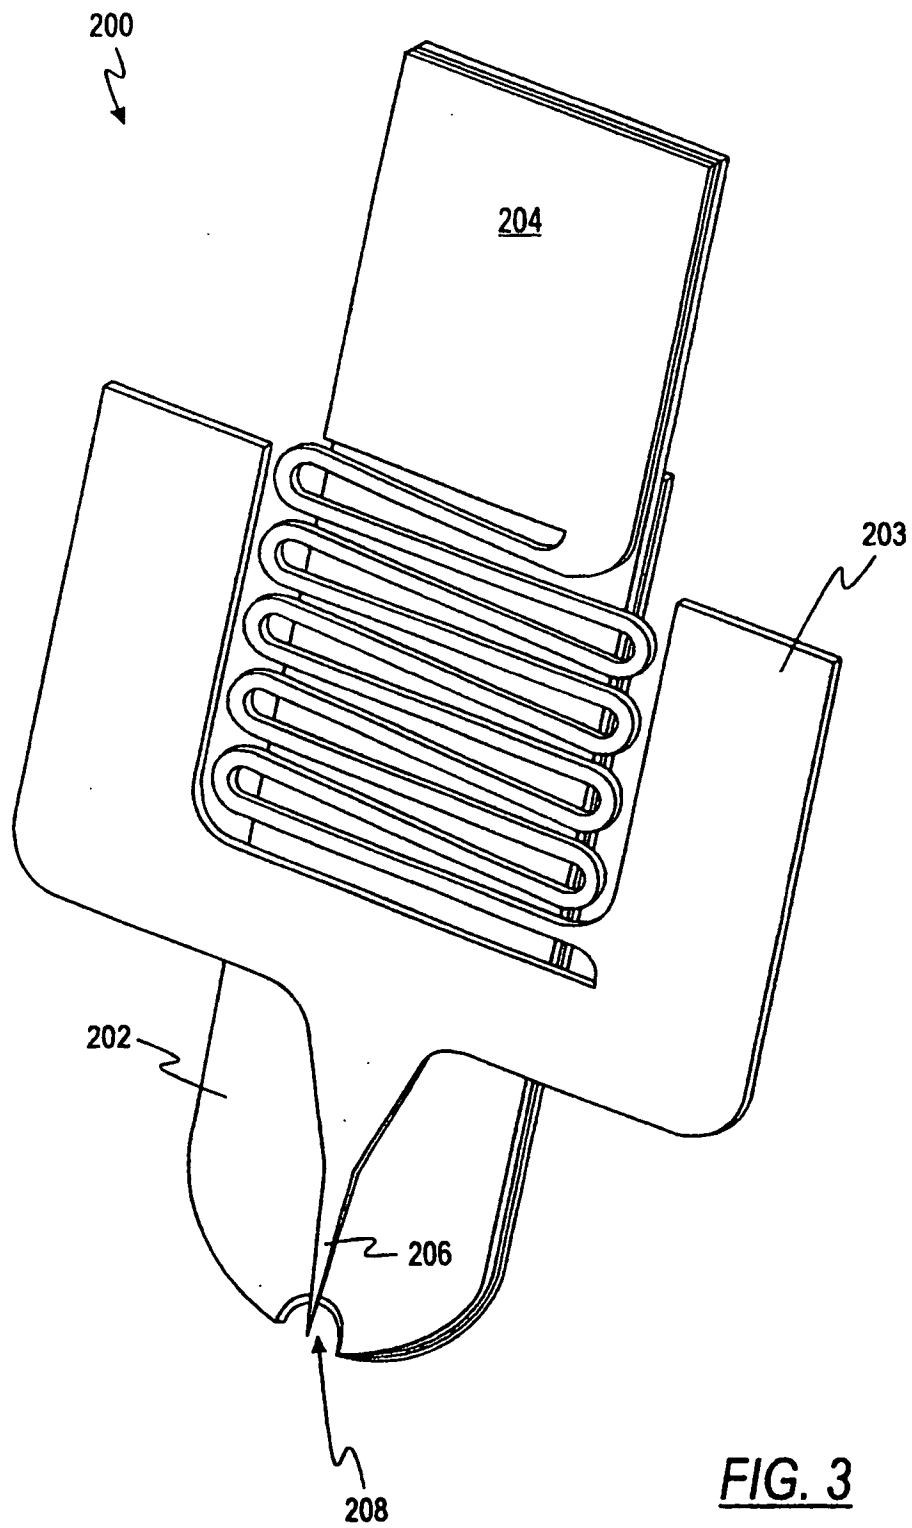


FIG. 2
(Prior Art)



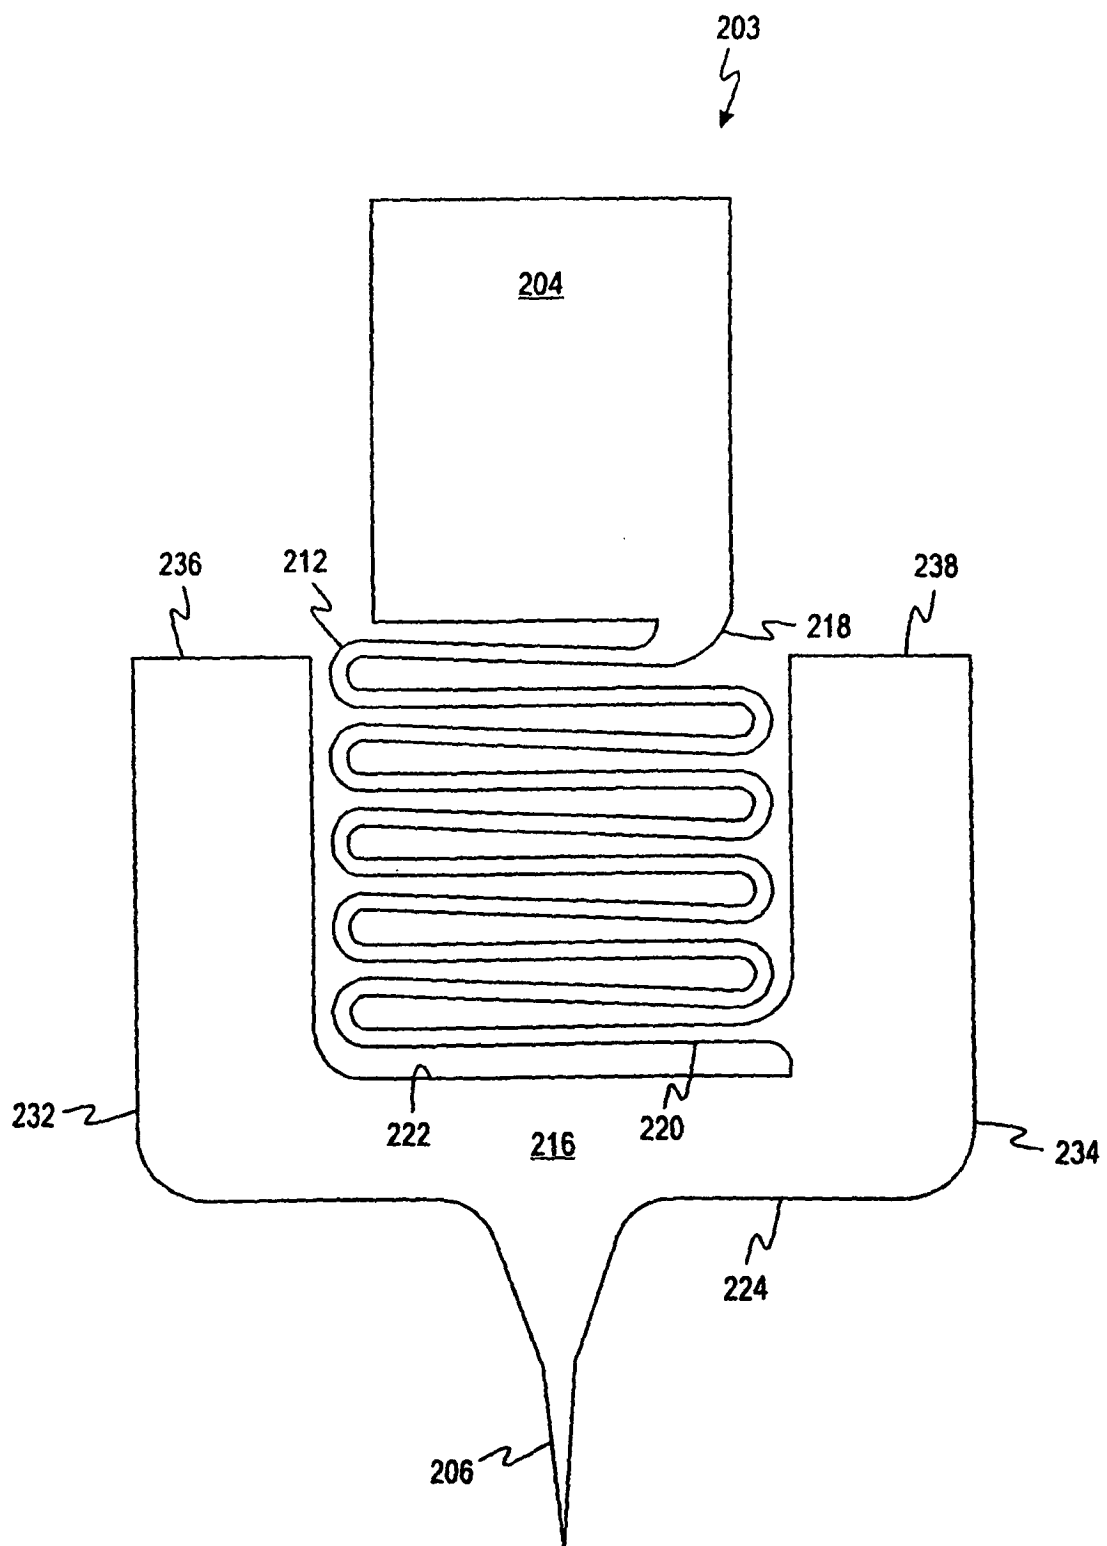


FIG. 4

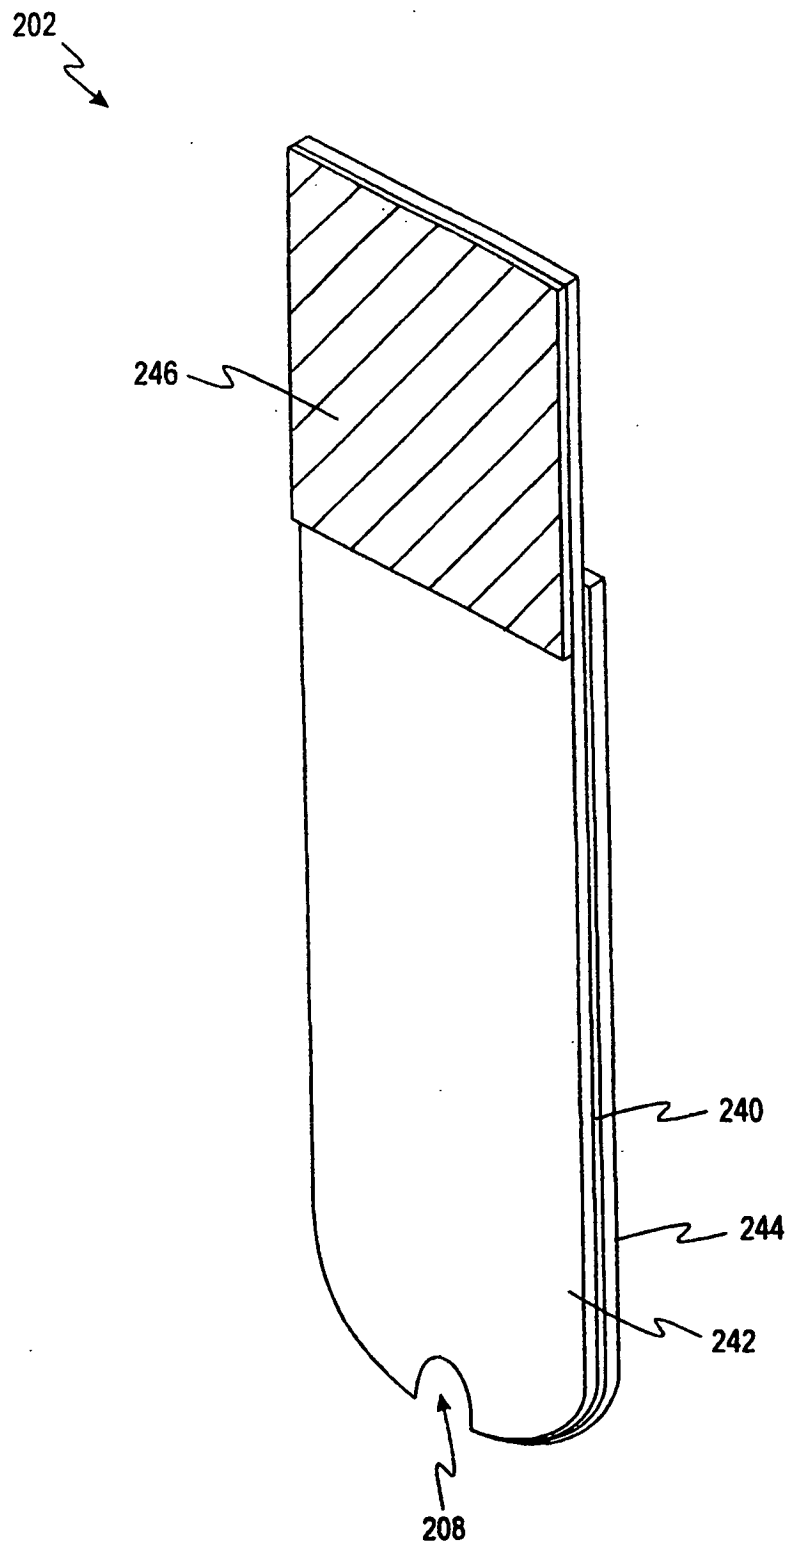


FIG. 5

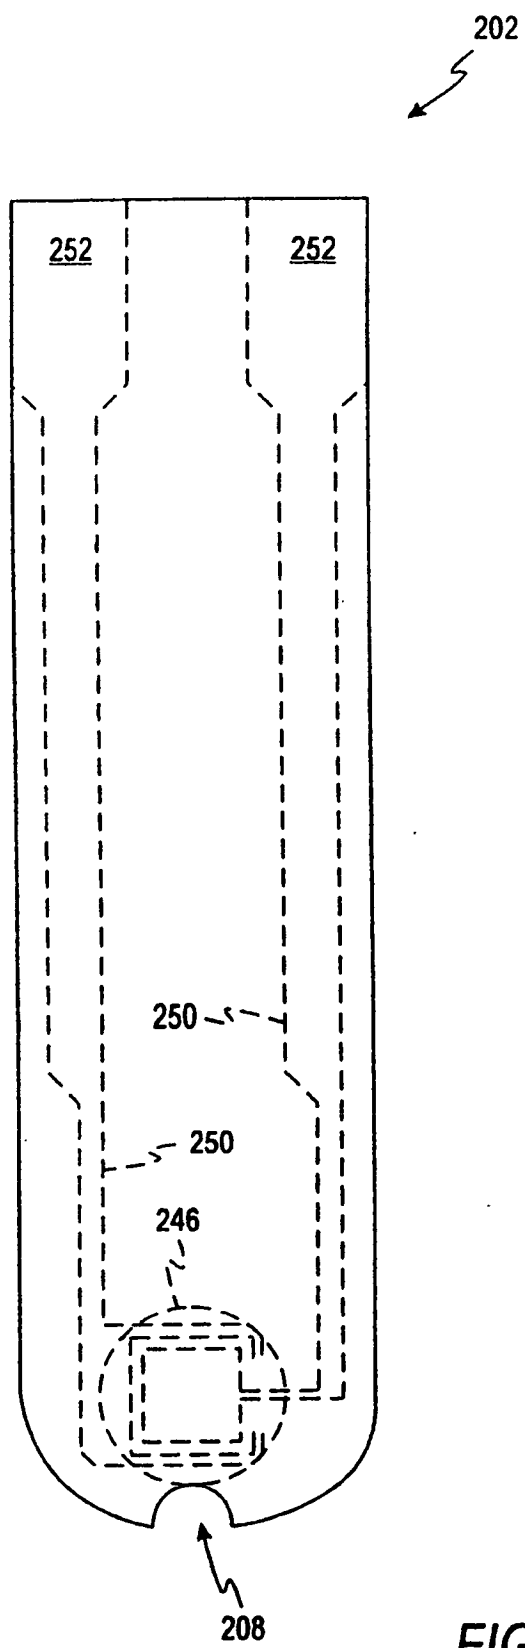


FIG. 6

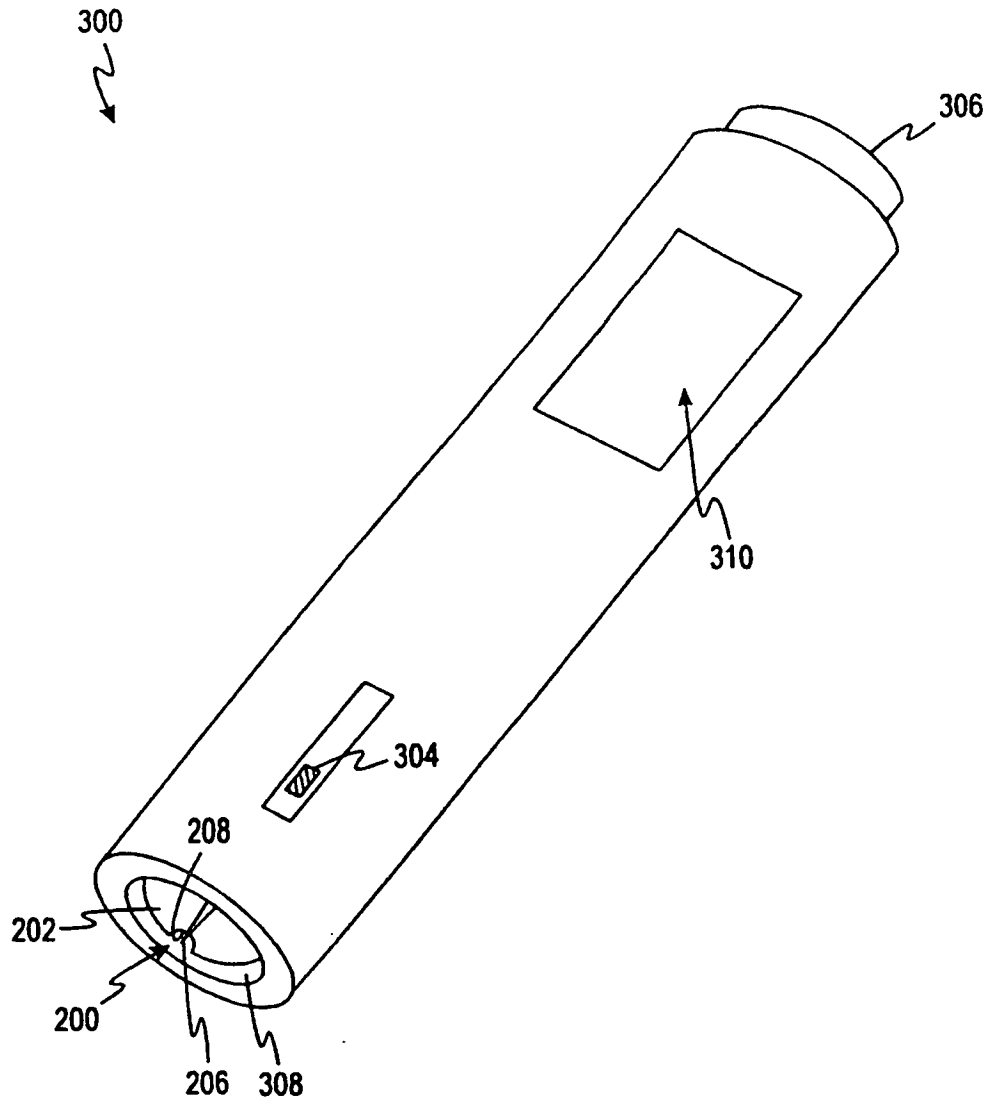


FIG. 7

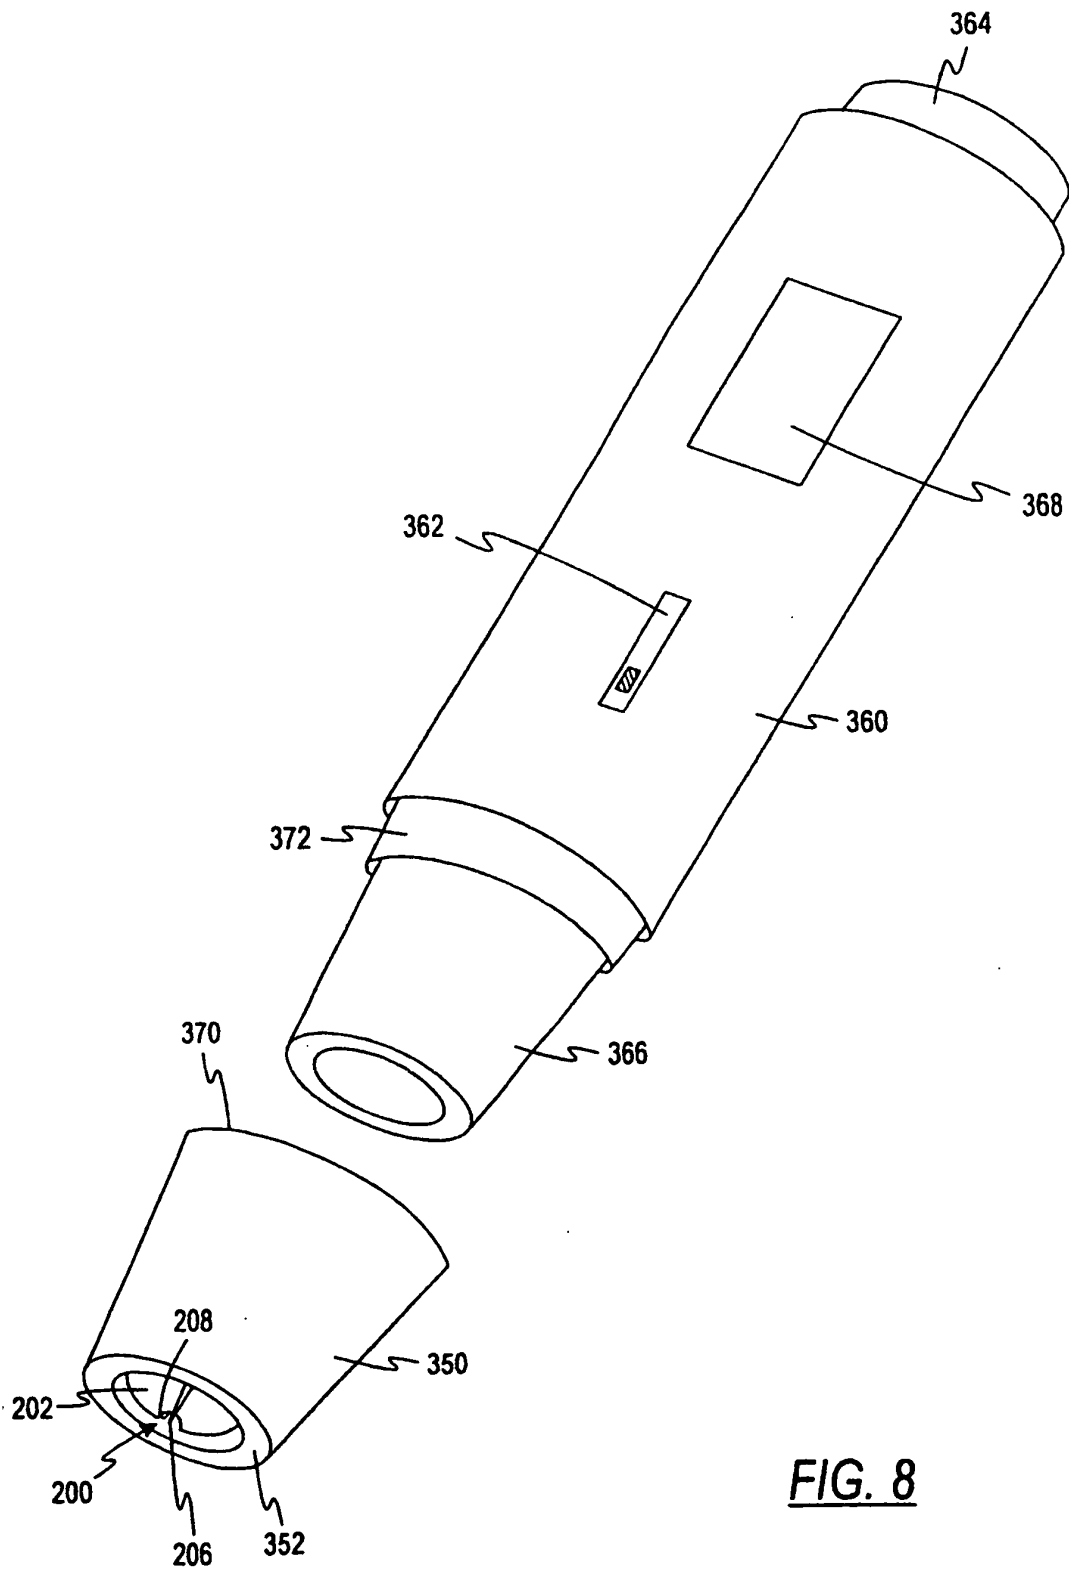


FIG. 8

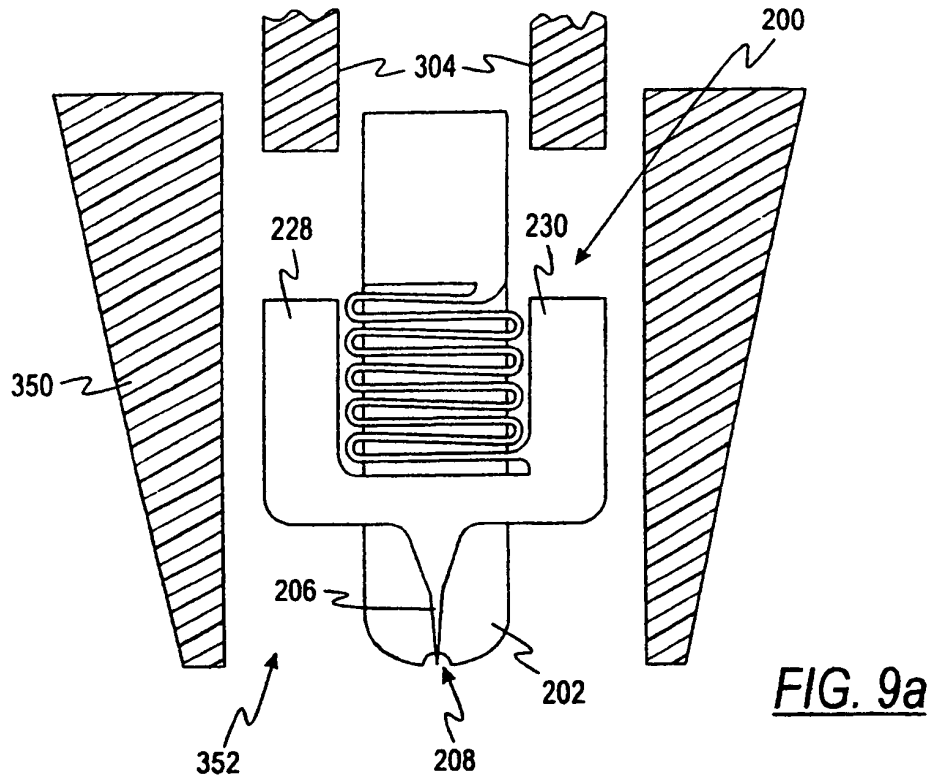


FIG. 9a

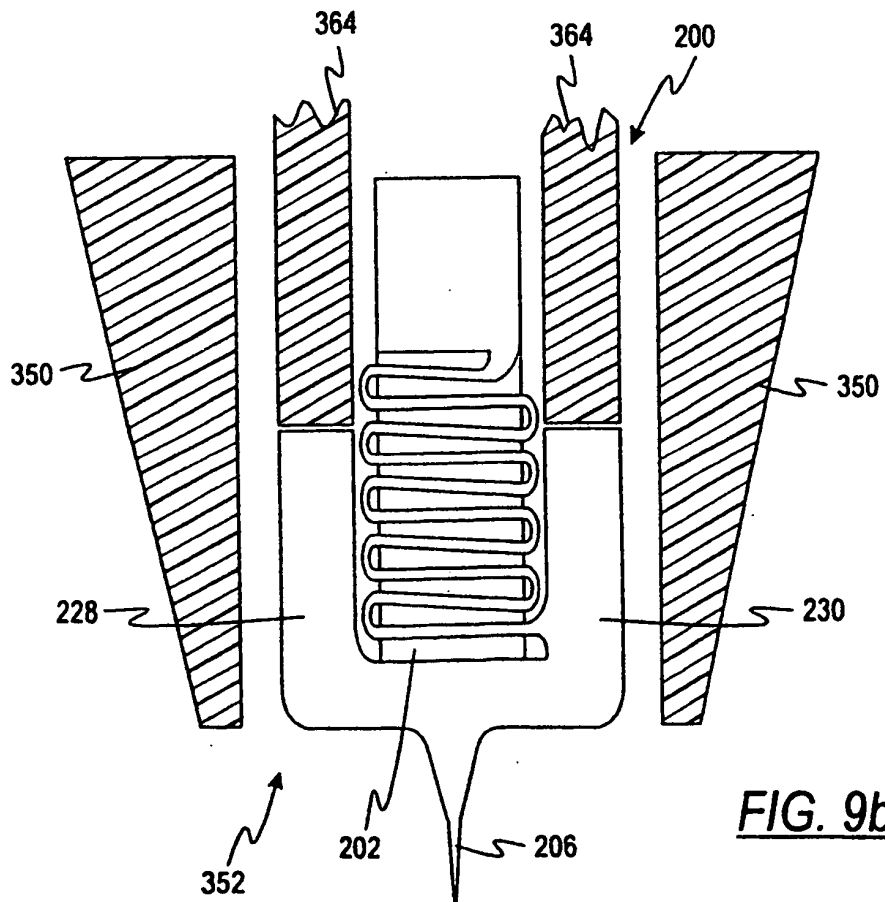


FIG. 9b

专利名称(译)	用于测试传感器的薄柳叶刀		
公开(公告)号	EP1174083B1	公开(公告)日	2006-11-15
申请号	EP2001115603	申请日	2001-07-02
[标]申请(专利权)人(译)	拜尔公司		
申请(专利权)人(译)	拜耳公司		
当前申请(专利权)人(译)	拜耳公司		
[标]发明人	WHITSON ROBERT C		
发明人	WHITSON, ROBERT C.		
IPC分类号	A61B5/15 G01N33/48 A61B5/00 A61B5/145 A61B5/1473 A61B5/151 A61B5/157 G01N33/49 G01N33/66		
CPC分类号	A61B5/15186 A61B5/14532 A61B5/150022 A61B5/150358 A61B5/150435 A61B5/150503 A61B5/15113 A61B5/15117 A61B5/1519 A61B5/15194 A61B5/157 A61B2562/0295		
优先权	60/216972 2000-07-10 US		
其他公开文献	EP1174083A3 EP1174083A2		
外部链接	Espacenet		

摘要(译)

提供喷枪 (203) 用于刺穿皮肤并产生血液样本。喷枪包括弹簧 (212) , 弹簧 (212) 具有第一端 (218) 和设置在针 (206) 和基部 (204) 之间的第二端 (220) , 其中弹簧的第一端连接到基座和第二端弹簧的一部分与针连接。

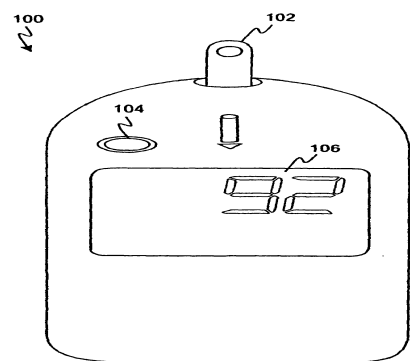


FIG. 1
(Prior Art)