



(11) **EP 2 436 307 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
21.10.2015 Bulletin 2015/43

(51) Int Cl.:
A61B 5/00 (2006.01) **G01N 21/47** (2006.01)
G02B 27/48 (2006.01) **G01B 9/02** (2006.01)

(21) Application number: **11188120.7**

(22) Date of filing: **31.03.2004**

(54) **Speckle reduction in optical coherence tomography by path length encoded angular compounding**

Fleckenreduzierung bei der optischen Kohärenztomografie durch pfadlängencodierte Winkelmischung

Réduction des taches dans la tomographie de cohérence optique par combinaison angulaire codée pour la longueur de chemin

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IT LI LU MC NL PL PT RO SE SI SK TR

(30) Priority: **31.03.2003 US 459543 P**
06.06.2003 US 476600 P
27.10.2003 US 514769 P

(43) Date of publication of application:
04.04.2012 Bulletin 2012/14

(62) Document number(s) of the earlier application(s) in accordance with Art. 76 EPC:
04749658.3 / 1 611 470

(73) Proprietor: **The General Hospital Corporation**
Boston, MA 02114 (US)

(72) Inventors:
• **Tearney, Guillermo, J.**
Cambridge, MA 02139 (US)
• **Iftimia, Nicusor**
North Chelmsford, MA 01863 (US)
• **Bouma, Brett, E.**
Quincy, MA 02171 (US)

(74) Representative: **Maiwald Patentanwalts GmbH**
Elisenhof
Elisenstrasse 3
80335 München (DE)

(56) References cited:
WO-A1-01/38820 WO-A2-03/012405
US-A- 6 037 579

- **BASHKANSKY M ET AL: "Statistics and reduction of speckle in optical tomography", OPTICS LETTERS, OSA, OPTICAL SOCIETY OF AMERICA, WASHINGTON, DC, US, vol. 25, no. 8, 1 April 2000 (2000-04-01), pages 545-547, XP002363428, ISSN: 0146-9592, DOI: 10.1364/OL.25.000545**
- **SCHMITT J M: "ARRAY DETECTION FOR SPECKLE REDUCTION IN OPTICAL COHERENCE MICROSCOPY", PHYSICS IN MEDICINE AND BIOLOGY, TAYLOR AND FRANCIS LTD. LONDON, GB, vol. 42, no. 7, 1 July 1997 (1997-07-01), pages 1427-1439, XP000656596, ISSN: 0031-9155, DOI: 10.1088/0031-9155/42/7/015**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 2 436 307 B1

DescriptionFIELD OF THE INVENTION

5 **[0001]** The present invention relates to optical imaging methods and apparatus useful in medical diagnosis and imaging. In particular, the present invention relates to a high speed method for implementing angular compounding, e.g., angular compounding by path length encoding ("ACPE") for reducing speckle in optical coherence tomography images.

BACKGROUND INFORMATION

10 **[0002]** Optical coherence tomography ("OCT") is a technique for obtaining high resolution cross-sectional images of biological tissues. Clinical OCT studies conducted in the gastrointestinal tract and cardiovascular system have shown that OCT is capable of providing images of the architectural ($>20\mu\text{m}$) microanatomy of a variety of epithelial tissues, including the layered structure of squamous epithelium and arterial vessels. However, for certain medical applications, such as the early detection of high-grade dysplasia in Barrett's esophagus and the identification of inflammation within atherosclerotic plaques, visualization of structures that are on a size scale of $< 20 \mu\text{m}$ may be preferable. OCT systems, with typical axial resolutions ranging from 8 - 12 μm , have the potential to resolve many of these structures, including nuclei, individual glands, and macrophages. Unfortunately, speckle, which occurs on the same size scale as these features, may prohibit unambiguous including nuclei, individual glands, and macrophages. Unfortunately, speckle, which occurs on the same size scale as these features, may prohibit unambiguous identification of the cellular and subcellular tissue components required for widespread clinical utilization of such technology.

20 **[0003]** Catheter or endoscope access and imaging is used in order to perform OCT in the internal organs of patients. In order to minimize diameter, most catheter-based OCT probes employ a single optical fiber to illuminate the sample and detect the signal from the tissue. High frame rates (typically 4-10 frames per second) are preferred for performing OCT imaging while minimizing artifacts caused by patient motion. A way to reduce speckle in OCT images that does not significantly increase the complexity of single optical fiber probe designs while maintaining high frame rates may be beneficial for applying OCT to accurately detect and quantify key microscopic tissue structures in patients.

25 **[0004]** The reduction of speckle in the OCT images speckle has been previously described. A publication by J. M. Schmitt, "Array Detection for Speckle Reduction in Optical Coherence Microscopy," Phys. Med. Biol. 42, 1427-1429, 1997, describes a procedure for a speckle reduction by averaging multiple images acquired at different angles, known as angular compounding. In this publication, multiple (N) detectors receive images that have been acquired from different angles. The images are averaged incoherently, providing an improvement (square root of N) in the signal to noise ratio ("SNR"). While this technique may be performed in real-time, the experimental apparatus as described therein would not be compatible with a single fiber optic catheter.

30 **[0005]** Another publication, M. Bashkansky and J. Reintjes, "Statistics and reduction of Speckle in Optical Coherence Tomography," Opt. Lett. 25, 545-547, 2000, describes an alternative technique for angular compounding to reduce speckle. In this method, a retroreflector apparatus is translated in front of the objective lens to change the angle of the incident beam on the tissue. N successive images are acquired and added incoherently to reduce speckle, again improving the SNR by a factor of square root of N. While this method may be less complex than the use of multiple detectors, the time needed thereby to acquire the images is increased by N. In addition, the implementation of this method within the confines of a small diameter catheter or endoscope could be difficult or impossible and may cause other disadvantage limitations.

SUMMARY OF THE INVENTION

45 **[0006]** The object of the present invention may be seen as to provide for a for an improved sample irradiation.

[0007] The object of the present invention is solved by the subject-matter of the independent claim. Further embodiments and advantages of the invention are incorporated in the dependent claims.

50 **[0008]** The described embodiments herein similarly pertain to the method for irradiating and the apparatus for irradiating a sample. Especially, the embodiments of the method described herein are related to an correspondingly configured apparatus of the present invention. Synergetic effects may arise from different combinations of the embodiments although they might not be described in detail. Further on, it shall be noted that all embodiments of the present invention concerning a method, might be carried out with the order of the steps as described, nevertheless this has not to be the only and essential order of the steps of the method. All different orders and combinations of the method steps are herewith described.

55 **[0009]** According to one exemplary embodiment of the present invention, an apparatus and a method for performing angular compounding to reduce speckle within OCT images are provided, which may use angular compounding by path length encoding ("ACPE"). With ACPE, a high-speed acquisition can be maintained, and modifications to standard OCT

catheter optics are likely to be minimal.

[0010] Accordingly, an apparatus for irradiating a sample, an apparatus probe catheter and a method according to exemplary embodiments of the present invention are provided for irradiating the sample. In particular, an interferometer may forward forwarding an electromagnetic radiation. In addition, a sample arm may receive the electromagnetic radiation, and can include an arrangement which facilitates a production of at least two radiations from the electromagnetic radiation so as to irradiate the sample. Such arrangement can be configured to delay a first radiation of the at least two radiations with respect to a second radiation of the at least two radiations.

[0011] In other words, an apparatus for irradiating a sample is provided which comprises an interferometer configured to forward an electromagnetic radiation and a sample arm configured to receive the electromagnetic radiation. Therein the sample arm includes an arrangement which is configured to produce at least two radiations from the electromagnetic radiation so as to irradiate the sample, and to delay a first radiation of the at least two radiations with respect to a second radiation of the at least two radiations. Furthermore the arrangement has at least one of a first optical section with a refractive index of at least 1.5, the first section being structured to propagate the at least two radiations, and a second section which has silicon, the second section being structured to propagate the at least two radiations. The apparatus of said embodiment may be configured to use angular compounding by path length encoding. The advantageous of this exemplary embodiment of the invention will become elucidated in the following description.

[0012] According to another exemplary embodiment the refractive index of the first optical section is at least 3.0.

[0013] According to another exemplary embodiment at least one of the first section or the second section comprises an anti-reflection-coated BK 7 glass.

[0014] According to another exemplary embodiment the glass has a thickness of from about 1.6 mm to about 7.7 mm.

[0015] According to another exemplary embodiment the at least one of the first section or the second section comprises an anti-reflection-coated glass that has a refractive index of from about 1.51 to about 3.5.

[0016] According to another exemplary embodiment of the present invention, a reference arm provides a further electromagnetic radiation. In particular, the interferometer receives the first, second and further radiations, and forms a resultant signal based on the first, second and further radiations. A processing arrangement may also be provided for generating a first image based on the first radiation and a second image based on the second radiation, such that the first and second images are different from one another. The further image may be generated based on the first and second images. In addition, the further image may have a noise that is smaller than a noise of the first image and a noise of the second image. Also, the further image may have a signal to noise ratio that is improved according to the equation:

$$SNR_{ACPE} = \frac{\langle S_{OCT} \rangle}{\sqrt{\text{var}[S_{OCT}]}} \propto \frac{\sum_{i=1}^N u_i}{\sqrt{\sum_{i=1}^N u_i^2}},$$

where SNR_{ACPE} is the signal to noise ratio, S_{OCT} is an amplitude of a high-pass filtered OCT signal, m is a thickness of the arrangement, u_i is an amplitude of a demodulated OCT signal at a spatial location, and N = 2m - 1. Further, m=2 and N=3 images associated with the at least two radiations may be obtained. The further image may also be generated based on a mathematical combination of the first and second images.

[0017] According to yet another exemplary embodiment of the present invention, the sample can be irradiated by the first irradiation at a first angle, and by the second radiation at a second angle, such that the first and second angles different from one another. For example, the first and second angle may be different from one another based on the delay and at least one of a phase and a incident angle of each of the first and second radiations. It is also possible to utilize a detector which detects the first electromagnetic energy, and forwards the detected energy to the processing arrangement.

[0018] In still another exemplary embodiment of the present invention, the arrangement can include two sections, each being configured to delay a respective one of the first and second radiations. In particular, in a further embodiment a delay of the first radiation is preferably greater than a delay of the second radiation. In addition and if desired, the delay of a path of the first radiation compared to a path of the second radiation is at least 500µm in air. In a further embodiment, the delay of a path of the first radiation compared to a path of the second radiation is at least 1mm in air. The arrangement may have a refractive index of at least 1.5 or at least 3.0. The arrangement can include silicon and/or an anti-reflective coating on at least one surface thereof. Such arrangement can be an anti-reflection-coated BK 7 glass. The glass may have a thickness of from about 1.6 mm to about 7.7 mm, and a refractive index of from about 1.51 to about 3.5.

5 [0019] According to yet another exemplary embodiment of the present invention, an apparatus for imaging is provided. The apparatus includes a sample arm that receive an electromagnetic radiation. The sample arm includes an arrangement which facilitates a production of at least two radiations from the electromagnetic radiation so as to irradiate a sample. The arrangement is configured to delay a first radiation of the at least two radiations with respect to a second radiation of the at least two radiations. The apparatus also includes a device for receiving the first and second radiations from the sample arm and at least one third radiation from a reference arm, such that the first and second radiations interfere with the third radiation. Further, the apparatus includes at least one of spectral separating unit which separates spectrum of at least one of the first, second and third radiations into frequency components, and at least one detection arrangement including a plurality of detectors. Each detector is capable of detecting at least a portion of at least one of the frequency components.

10 [0020] In a further exemplary embodiment of the present invention, an apparatus is provided. Such apparatus includes at least one first arrangement that provides at least one first electro-magnetic radiation to a sample arm and at least one second electro-magnetic radiation to a non-reflective reference arm. A frequency of radiation provided by the first arrangement varies over time. The sample arm receives the first electromagnetic radiation, and includes an arrangement which facilitates a production of at least two radiations from the electromagnetic radiation so as to irradiate a sample. The arrangement is configured to delay a first radiation of the at least two radiations with respect to a second radiation of the at least two radiations. The apparatus also includes at least one second arrangement detecting an interference between the first and second radiations generated at the sample arm and the second electro-magnetic radiations generated at the reference.

15 [0021] In still another exemplary embodiment of the present invention, an apparatus is provided. The apparatus includes a. at least one first arrangement providing at least one first electro-magnetic radiation to a sample arm and at least one second electro-magnetic radiation to a reference arm. The first and/or second electromagnetic radiation have a spectrum which changes over time. The spectrum contains multiple frequencies at a particular time. The sample arm receives the first electromagnetic radiation, and includes an arrangement which facilitates a production of at least two radiations from the electromagnetic radiation so as to irradiate a sample. The arrangement is configured to delay a first radiation of the at least two radiations with respect to a second radiation of the at least two radiations. The apparatus also includes at least one second arrangement detecting an interference between the first and second radiations generated at the sample arm and the second electro-magnetic radiations generated at the reference.

20 [0022] Other features and advantages of the present invention will become apparent upon reading the following aspects and the following detailed description of embodiments of the invention, when taken in conjunction with the appended claims.

25 [0023] According to a first aspect of the present invention an apparatus for irradiating a sample, comprises

- 30 a) an interferometer forwarding an electromagnetic radiation; and
35 b) a sample arm receiving the electromagnetic radiation, the sample arm including an arrangement which facilitates a production of at least two radiations from the electromagnetic radiation so as to irradiate the sample, the arrangement being configured to delay a first radiation of the at least two radiations with respect to a second radiation of the at least two radiations.

40 [0024] According to a second aspect of the present invention the apparatus of the first aspect further comprises

- c) a reference arm providing a further electromagnetic radiation, wherein the interferometer receives the first, second and further radiations, and forms a resultant signal based on the first, second and further radiations; and
45 d) a processing arrangement generating a first image based on the first radiation and a second image based on the second radiation, wherein the first and second images are different from one another.

[0025] According to a third aspect of the present invention in the apparatus of the second aspect the processing arrangement generates a further image based on the first and second images.

50 [0026] According to a forth aspect of the present invention in the apparatus of the third aspect the further image has a noise that is smaller than a noise of the first image and a noise of the second image.

[0027] According to a fifth aspect of the present invention in the apparatus of the fourth aspect the further image has a signal to noise ratio that is improved according to the equation:

5

$$SNR_{ACPE} = \frac{\langle S_{OCT} \rangle}{\sqrt{\text{var}[S_{OCT}]}} \propto \frac{\sum_{i=1}^N u_i}{\sqrt{\sum_{i=1}^N u_i^2}},$$

10

wherein SNR_{ACPE} is the signal to noise ratio, S_{OCT} is an amplitude of a high-pass filtered OCT signal, m is a thickness of the arrangement, u_i is an amplitude of a demodulated OCT signal at a spatial location, and $N = 2m - 1$.

[0028] According to a sixth aspect of the present invention in the apparatus of the fifth aspect $m=2$ and $N=3$ images associated with the at least two radiations are obtained.

15 **[0029]** According to a seventh aspect of the present invention in the apparatus of the third aspect the further image is generated based on a mathematical combination of the first and second images.

[0030] According to an eighth aspect of the present invention in the apparatus of the second aspect the sample is irradiated by the first irradiation at a first angle, wherein the sample is irradiated by the second radiation at a second angle, the first and second angles different from one another.

20 **[0031]** According to a ninth aspect of the present invention in the apparatus of the eighth aspect the first and second angle are different from one another based on the delay and at least one of a phase and a incident angle of each of the first and second radiations.

[0032] According to a tenth aspect of the present invention the apparatus of the second aspect, further comprising a detector which detects the first electromagnetic energy, and forwards the detected energy to the processing arrangement.

25 **[0033]** According to an eleventh aspect of the present invention in the apparatus of the first aspect, the arrangement includes two sections, each being configured to delay a respective one of the first and second radiations, and wherein a delay of the first radiation is greater than a delay of the second radiation.

[0034] According to a twelfth aspect of the present invention in the apparatus of the first aspect the delay of a path of the first radiation compared to a path of the second radiation is at least $500\mu\text{m}$ in air.

30 **[0035]** According to a thirteenth aspect of the present invention in the apparatus of the first aspect the delay of a path of the first radiation compared to a path of the second radiation is at least 1mm in air.

[0036] According to a fourteenth aspect of the present invention in the apparatus of the first aspect the arrangement has a refractive index of at least 1.5.

35 **[0037]** According to a fifteenth aspect of the present invention in the apparatus of the first aspect the arrangement has a refractive index of at least 3.0.

[0038] According to a sixteenth aspect of the present invention in the apparatus of the first aspect the arrangement includes silicon.

[0039] According to a seventeenth aspect of the present invention in the apparatus of the first aspect the arrangement includes an anti-reflective coating on at least one surface thereof.

40 **[0040]** According to an eighteenth aspect of the present invention in the apparatus of the first aspect the arrangement comprises an anti-reflection-coated BK 7 glass.

[0041] According to a nineteenth aspect of the present invention in the apparatus of the sixteenth aspect the glass has a thickness of from about 1.6mm to about 7.7mm .

45 **[0042]** According to a twentieth aspect of the present invention in the apparatus of the sixteenth aspect the glass has a refractive index of from about 1.51 to about 3.5.

[0043] According to aspect 21 of the present invention a catheter is presented which comprises

- a) an interferometer forwarding an electromagnetic radiation; and
- b) a sample arm receiving the electromagnetic radiation, the sample arm including an arrangement which facilitates a production of at least two radiations from the electromagnetic radiation so as to irradiate the sample, the arrangement being configured to delay a first radiation of the at least two radiations with respect to a second radiation of the at least two radiations.

50

[0044] According to aspect 22 of the present invention a catheter is presented which comprises

55

- a. an interferometer forwarding an electromagnetic radiation; and
- b. a sample arm receiving the electromagnetic radiation, the sample arm including an arrangement which facilitates a production of at least two radiations from the electromagnetic radiation so as to irradiate a sample, the arrangement

being configured to delay a first radiation of the at least two radiations with respect to a second radiation of the at least two radiations.

5 [0045] According to aspect 23 of the present invention method for irradiating a sample is presented comprising the steps of:

- 10 a. providing an electromagnetic radiation from an interferometer; and
b. in a sample arm, facilitating production of at least two radiations from the electromagnetic radiation so as to irradiate the sample, a first radiation of the at least two radiations being delayed with respect to a second radiation of the at least two radiations.

[0046] According to aspect 24 of the present invention an apparatus is presented which comprises

- 15 a. a sample arm receiving an electromagnetic radiation, the sample arm including an arrangement which facilitates a production of at least two radiations from the electromagnetic radiation so as to irradiate a sample, the arrangement being configured to delay a first radiation of the at least two radiations with respect to a second radiation of the at least two radiations;
b. a device receiving the first and second radiations from the sample arm and at least one third radiation from a reference arm, wherein the first and second radiations interfere with the third radiation;
20 c. at least one of spectral separating unit which separates spectrum of at least one of the first, second and third radiations into frequency components; and
d. at least one detection arrangement including a plurality of detectors, each detector capable of detecting at least a portion of at least one of the frequency components.

25 [0047] According to aspect 25 of the present invention an apparatus is presented which comprises

- 30 a. at least one first arrangement providing at least one first electromagnetic radiation to a sample arm and at least one second electro-magnetic radiation to a non-reflective reference arm, wherein a frequency of radiation provided by the first arrangement varies over time, wherein the sample arm receives the first electromagnetic radiation, the sample arm including an arrangement which facilitates a production of at least two radiations from the electromagnetic radiation so as to irradiate a sample, the arrangement being configured to delay a first radiation of the at least two radiations with respect to a second radiation of the at least two radiations; and b. at least one second arrangement detecting an interference between the first and second radiations generated at the sample arm and the second electromagnetic radiations generated at the reference.

35 [0048] According to aspect 26 of the present invention an apparatus is presented which comprises

- 40 a. at least one first arrangement providing at least one first electromagnetic radiation to a sample arm and at least one second electro-magnetic radiation to a reference arm, wherein at least one of the first and second electro-magnetic radiation has a spectrum which changes over time, the spectrum containing multiple frequencies at a particular time, wherein the sample arm receives the first electromagnetic radiation, the sample arm including an arrangement which facilitates a production of at least two radiations from the electromagnetic radiation so as to irradiate a sample, the arrangement being configured to delay a first radiation of the at least two radiations with respect to a second radiation of the at least two radiations; and b. at least one second arrangement detecting an interference between the first and second radiations generated at the sample arm and the second electromagnetic radiations generated at the reference.

BRIEF DESCRIPTION OF THE DRAWINGS

50 [0049] The invention is illustrated in the drawings in which like reference characters designate the same or similar parts throughout the figures of which:

Fig. 1A is a schematic diagram of an exemplary embodiment of an ACPE-OCT apparatus according to the present invention.

55 Fig. 2A is a schematic diagram of an exemplary embodiment of an Intralipid-Agar phantom according to the present invention.

Fig. 2B is an exemplary OCT image of the phantom of Fig. 2A without the insertion of a BK7 ACPE element.

Fig. 2C is an illustration of exemplary ACPE OCT images obtained by splitting a sample beam in two parts using

an exemplary 3.1 mm BK7 glass element.

Fig. 3A is an exemplary OCT image of a ventral forearm obtained in vivo prior to the insertion of the BK7 ACPE element.

Fig. 3B is an exemplary compounded ACPE OCT image of the skin acquired at the same location as that in Fig. 3A.

5 DETAILED DESCRIPTION

I. Materials and Methods

[0050] Fig. 1A shows an exemplary embodiment of an apparatus according to the present invention which uses ACPE. An optical glass 20 is placed in an imaging path 10 of a conventional OCT imaging apparatus 5, splitting the incident field into two beamlets 1 and 2 which are provided on beam paths 30 and 40, respectively. For the purpose of the present discussion, a beamlet can be defined as a portion of a beam. An optical element (e.g., the optical glass 20) causes a portion of the incident beam (beamlet 2) to experience a greater path length delay than beamlet 1. In addition, beamlet 2 illuminates the sample at a different angle than beamlet 1. A lens may be provided to converge the beamlets 1 and 2 onto the sample (e.g., a tissue). As a result, multiple OCT images of a specimen in or on the sample, each acquired at a different angle, can appear simultaneously on the OCT display (see Fig. 1B), in particular, Fig. 1B shows that the top image (i.e., labeled as 1 + 1) corresponds to the image formed from path 1 (i.e., incident and reflected), the middle image (i.e., labeled as 1 + 2, 2 + 1) corresponds to the image formed from path 1 incident, path 2 reflected and path 2 incident, path 1 reflected. Further, the bottom image (i.e., 2 + 2) of Fig. 1B corresponds to the image formed from path 2 (incident and reflected).

[0051] These beamlets 1 and 2, thus encoded by optical path length, also illuminate the sample at different angles. As a result, multiple OCT images, each acquired at different angles, are preferably present in a single OCT frame (as shown in Fig. 1B). For example, when the optical element contains m distinct thicknesses of glass, with each optical thickness a multiple of the others, 2m - 1 OCT images can be obtained in one OCT frame. Each image may be separated by a group delay of D(n - 1)/2, where D is the thickness and n is the refractive index of the optical material. The distinct OCT images are then averaged to produce a composite OCT image with significantly reduced speckle. Since all of the images are acquired in one OCT frame, single frame acquisition time can be maintained, in addition, the modifications to the OCT probe may involve only the insertion of at least one small optical element in the beam path of the distal optics. These advantages of ACPE allow speckle averaging to be performed within the confines of a small diameter catheter or endoscope, and without compromising the acquisition speed.

[0052] Previous attempts of utilizing OCT speckle reduction by image compounding has shown that the addition of N images of the same intensity provides an SNR increase by a factor of N. For example, the Bashkansky publication described above describes that the speckle distribution in OCT takes the form of the probability density function:

$$p(S_{OCT}) = \frac{1}{\sqrt{2\pi K}} \exp\left(\frac{-S_{OCT}^2}{2K^2}\right)$$

where K = 2ARσ, with AR is the amplitude of the reference field, Socris the amplitude of the high-pass filtered OCT signal, and σ is its standard deviation. For this probability density function, it can be demonstrated that the SNR improvement obtained by averaging N images of the same amplitude is also a factor of √N, a result that has been experimentally described in the Schmitt and Bashkansky publications. For ACPE, the distinct OCT subimages generally may not have equal amplitudes. However, with the assumption of isotropic backscattering, these subimages are related to the original OCT image, S_{OCT} by β n₂, where P is the number of path length combinations that contribute to a distinct subimage. As a result, the SNR for ACPE may be defined as

$$SNR_{ACPE} = \frac{\langle S_{OCT} \rangle}{\sqrt{\text{var}[S_{OCT}]}} \propto \frac{\sum_{i=1}^N u_i}{\sqrt{\sum_{i=1}^N u_i^2}},$$

where w_i is the amplitude of the demodulated OCT signal at a spatial location, and N = 2m - J. In the case of m=2, N=

3 images are obtained and the relationships between the amplitudes of the ACPE OCT subimages are $SIQCT = S3_{OCT} = \frac{1}{4} S0_{OCT}$
 $mL \text{ } \$ QCT - 2SIQCT = \frac{1}{2} S0_{OCT}$. The potential SNR improvement of the compounded $m = 2$ ACPE image can then become $SNR_{ACPE} / SNR_0 = 1.63$, where SNR_0 is the signal to noise ratio of $S0_{OCT}$.

5 [0053] If desired the apparatus of Fig. 1A may be provided in a different form according to the present invention such that the following apparatus for irradiating a sample is provided. Said apparatus comprises an interferometer configured to forward an electromagnetic radiation and a sample arm configured to receive the electromagnetic radiation. Therein the sample arm includes an arrangement which is configured to produce at least two radiations from the electromagnetic radiation so as to irradiate the sample, and to delay a first radiation of the at least two radiations with respect to a second radiation of the at least two radiations. Furthermore the arrangement has at least one of a first optical section with a refractive index of at least 1.5, the first section being structured to propagate the at least two radiations, and a second section which has silicon, the second section being structured to propagate the at least two radiations. If desired the refractive index of the first optical section is at least 3.0 in said apparatus. If desired the first section or the second section comprises an anti-reflection-coated BK 7 glass in said apparatus. If further desired the glass has a thickness of from about 1.6 mm to about 7.7 mm in said apparatus. Furthermore, if desired the at least one of the first section or the second section comprises an anti-reflection-coated glass that has a refractive index of from about 1.51 to about 3.5 in said apparatus. All the herein cited features of said apparatus may be combined in any desired way to provide for specific advantageous effects.

20 **EXAMPLES**

II. Example 1

25 [0054] An exemplary polarization-diverse OCT system according to the present invention can be utilized for the exemplary apparatus (e.g., as shown in Fig. 1 A) that implements ACPE. Using such exemplary system according to the present invention, OCT images may be acquired at 2 frames per second (e.g., 500 axial pixels x 500 transverse pixels), which may be displayed with an inverse gray-scale lookup table, and digitally archived. The optical source which can be used in such exemplary OCT system may have a center wavelength of 1310 nm and a bandwidth of 70 nm, and thus providing an axial resolution of approximately 8 μm in the tissue.

30 [0055] A modified hand-held galvanometer probe (e.g., the apparatus of Fig. 1A) can be inserted in the sample arm of the OCT system 5. The objective lens 50 may have a focal length of 25 mm and a numerical aperture (NA) of 0.11, providing a measured $1/e^2$ focal spot diameter of 23 μm . A square, antireflection-coated $D = 3.1$ mm BK7 glass ($n = 1.51$) (e.g., the optical glass 20, may be inserted between the optical fiber collimator and the objective lens 50 (see Fig. 1 A) so that overlaps with half of the illuminating beam. With this exemplary configuration, an OCT image separation of approximately 800 μm can be achieved. When the glass plate is inserted, the spot diameter perpendicular to the glass edge may increase by a factor of two (46 μm). In the plane of the OCT image, however, the transverse resolution is likely preserved.

40 **III. Example 2**

[0056] A solid phantom consisting of 1 % Intralipid solution and Agar can be used to measure a reduction in speckle provided by ACPE. For example, four (4) hairs can be embedded in the Intralipid- Agar gel at different transverse positions and depths. A schematic of the phantom is depicted in Fig. 2A. The corresponding OCT images with and without the BK7 glass plate are shown in Figs. 2B and 2C, respectively. ROI's labeled 1-5 represent exemplary locations where the SNR improvement by ACPE is preferably measured. The insertion of the BK7 glass plate 20 (with a 3.1 mm BK7 glass element) in the sample arm can produce three copies of the original OCT image (see Fig. 2C), with each image being acquired at a different illumination angles and separated by group delay increments of, e.g., 800 μm . The amplitudes of the signals in the top and bottom images of Fig. 2C can be approximately half of the center image ($SIQCTI \ S20_{ct} = S3Q_{ct} \ S20_{ct} = 1:2$). The compounded ACPE image shown in Fig. 2D can be obtained by incoherently averaging the three images that are shown in Fig. 2C. A substantial reduction of speckle in the compounded image can be visualized in Fig. 2D. Compared to the original OCT image, the average ACPE SNR improvement for the five regions depicted in Fig. 2B is preferably 1.54 ± 0.12 (mean \pm standard deviation).

55 **IV. Example 3**

[0057] In order to demonstrate SNR improvement in vivo, ACPE OCT imaging can be performed on a ventral forearm of a subject. Figs. 3A and 3B shows one representative set of images. Fig. 3A shows an exemplary OCT image of the ventral forearm obtained in vivo prior to the insertion of the BK7 ACPE element. Visual assessment of these pictures

demonstrates a qualitative improvement in the compounded ACPE image (Fig. 3B). The boundary between the epidermis (E) and dermis (D) is more clearly demarcated with ACPE as shown in Fig. 3B. In addition, horizontal structures consistent with dermal vasculature are more readily identified in the ACPE image of Fig. 3B. The SNR can be measured for the ACPE and original OCT images in Fig. 3B, providing an exemplary SNR improvement of 1.56.

5 [0058] The apparatus and method according to the exemplary embodiments of the present invention are provide to reduce speckle in OCT images that does not decrease the OCT frame rate and requires only minor modifications to the OCT probe. The implementation of ACPE, implements potential compromises between speckle reduction and three other OCT system parameters: a) sample arm transverse resolution, b) total reference arm path length, and c) OCT image sensitivity. In particular, for any given objective lens, ACPE may compromise the transverse resolution in one dimension by underfilling the lens aperture for each individual beamlet. In most cases, increasing the numerical aperture (NA) of the objective can compensate for this resolution loss.

10 [0059] Speckle averaged ACPE-OCT images can be obtained at the same rate as conventional OCT images by scanning an increased reference arm path length delay at substantially the same frequency. In order to acquire each of the individual OCT subimages, the new scan length of the ACPE-OCT system can preferably be $L(2m - 1)$, where L is the original scan length of the OCT system. Using phase control RSOD lines, scan ranges up to 10 mm are possible, thus enabling $m = 3$, $L = 2$ mm, and a maximum predicted SNR improvement of ~ 2.1 .

15 [0060] Increasing the reference arm path length scan range while maintaining the scan rate, may increase the electronic bandwidth and decrease the sensitivity of the OCT system. Also, because ACPE splits the sample arm power into $2m - 1$ subimages, each subimage contains a fraction of the original sample arm power. When imaging a human tissue, these losses may primarily affect the penetration depth of the OCT image. Since many features of clinical relevance, such as nuclei in patients with Barrett's esophagus or macrophages in atherosclerotic plaques, may be present at tissue surfaces, for modest m, the improvements in image quality provided by ACPE likely outweigh sensitivity losses. Moreover, ongoing technical developments towards more efficient interferometer designs and higher power, clinically viable OCT sources may render ACPE sensitivity losses a non-issue. The thickness of the path length encoding optical element described herein in the above-referenced Examples (3.1 mm BK7) may not be sufficient for OCT imaging in some tissues since they provide 800 nm separation between individual subimages. Increasing the thickness of the BK7 glass to 7.7 mm may allow a path length separation of 2 mm. This thickness may be adequate for a free-space, handheld OCT probes, but can be problematic in small diameter, flexible catheters, where minimizing the rigid length can be important. In order to increase the optical thickness of the path length encoding element, a higher refractive index material such as silicon ($n = 3.5$) may be used. To create a 2 mm delay with silicon, preferably approximately 1.6 mm of the material can be used. When using high refractive index glass, dispersion imbalances between the reference and sample arms should be considered. For high-resolution OCT imaging ($\Delta\lambda/\lambda > 10\%$), appropriate selection of the optical material used for path length encoding will depend on the center wavelength and bandwidth of the source.

25 [0061] Advantages of the exemplary embodiment of the method and apparatus according to the present invention may include the fact that the OCT frame rate is not increased, and the addition of only a single passive element in the OCT probe should be implemented. These features of ACPE make the system and method of the present invention compatible with OCT imaging in internal organ systems in patients. While implementation of ACPE may facilitate tradeoffs between speckle reduction and system sensitivity, the problems caused by speckle noise are likely more significant for clinical diagnosis than the penetration depth of modern OCT systems, especially at 1300 nm. Since difficulties in interpreting features on the size scale of 20 μm or less is in part a result of speckle noise in OCT images, ACPE would likely significantly improve the capabilities of OCT for the diagnosis of important diseases such as, but not limited to, dysplasia and inflammation in atherosclerosis.

30 [0062] Although only particular exemplary embodiments of the present invention have been described in detail herein above, those skilled in the art will readily appreciate and understand that many modifications are possible in the exemplary embodiments without materially departing from the novel teachings and advantages of this invention. Accordingly, all such modifications are intended to be included within the scope of the present invention as defined in the following claims.

35 [0063] Other variations to the disclosed embodiments can be understood and effected by those skilled in the art in practising the claimed invention, from the study of the drawings, the disclosure, and the appended claims. In the claims the word "comprising" does not exclude other elements or steps and the indefinite article "a" or "an" does not exclude a plurality. A single processor or other unit may fulfil the functions of several items or steps recited in the claims. The mere fact that certain measures are recited in mutually different dependent claims does not indicate that a combination of these measures cannot be used to advantage. A computer program may be stored/distributed on a suitable medium such as an optical storage medium or a solid-state medium supplied together with or as part of other hardware, but may also be distributed in other forms, such as via the Internet or other wired or wireless telecommunication systems. Any reference signs in the claims should not be construed as limiting the scope of the claims.

Claims

1. An optical coherence tomography (5) apparatus for irradiating a sample, comprising:

5 a) an interferometer in a backscattering configuration forwarding an electromagnetic radiation; the interferometer comprising

10 a sample arm receiving the electromagnetic radiation, the sample arm including an arrangement which is configured to separate at least two beamlets (1,2) from the electromagnetic radiation so as to irradiate the sample, and the arrangement is configured to delay a first beamlet (1) of the at least two beamlets with respect to a second beamlet (2) of the at least two beamlets, wherein the delay is a difference in an optical path length, and

15 a reference arm providing a further electromagnetic radiation, wherein the interferometer receives the first beamlet (1), the second beam let (2) and the further radiation, and forms a resultant signal based on the first and second beamlets and the further radiation;

20 b) a processing arrangement configured for generating a first image based on the first beamlet (1), a second image based on the second beamlet (2), and a further image based on the first and second images, wherein the first and second images are different from one another, wherein the further image is generated based on an incoherent mathematical combination of the first and second images so as to reduce speckle, and

wherein the arrangement has:

- 25 a first configuration with a refractive index of at least 1.5, and propagates one of the at least two beamlets, or
 a second configuration which has silicon, and propagates one of the at least two beamlets.

2. The apparatus according to claim 1, wherein the refractive index of the first optical configuration is at least 3.0,

30 3. The apparatus according to claim 1, wherein at least one of the first configuration or the second configuration comprises an anti-reflection-coated BK 7 glass.

4. The apparatus according to claim 3, wherein the glass has a thickness of from about 1.6 mm to about 7.7 mm.

35 5. The apparatus according to claim 1, wherein at least one of the first configuration or the second configuration comprises an anti-reflection-coated glass that has a refractive index of from about 1.51 to about 3.5.

Patentansprüche

40 1. Optische Kohärenztomografievorrichtung (5) zum Bestrahlen einer Probe, Folgendes umfassend:

a) ein Interferometer in einer Rückstreuungskonfiguration, welches eine elektromagnetische Strahlung weitergibt; wobei das Interferometer Folgendes umfasst:

45 einen Probenarm, der die elektromagnetische Strahlung empfängt, wobei der Probenarm eine Anordnung einschließt, die konfiguriert ist, wenigstens zwei Teilstrahlen (1, 2) aus der elektromagnetischen Strahlung abzutheilen, um die Probe zu bestrahlen, und die Anordnung konfiguriert ist, einen ersten Teilstrahl (1) der wenigstens zwei Teilstrahlen bezogen auf einen zweiten Teilstrahl (2) der wenigstens zwei Teilstrahlen zu verzögern, wobei die Verzögerung eine Veränderung einer Länge des optischen Pfads ist; und

50 einen Referenzarm, der eine weitere elektromagnetische Strahlung bereitstellt, wobei das Interferometer den ersten Teilstrahl (1), den zweiten Teilstrahl (2) und die weitere Strahlung empfängt und ein Ergebnis-signal auf der Grundlage des ersten und des zweiten Teilstrahls und der weiteren Strahlung ausbildet;

55 b) eine Verarbeitungsanordnung, konfiguriert, ein erstes Bild auf der Grundlage des ersten Teilstrahls (1), ein zweites Bild auf der Grundlage des zweiten Teilstrahls (2) und ein weiteres Bild auf der Grundlage des ersten und des zweiten Bildes zu erzeugen, wobei sich das erste und das zweite Bild voneinander unterscheiden, wobei das weitere Bild auf der Grundlage einer inkohärenten mathematischen Kombination des ersten und des zweiten Bildes erzeugt wird, um Speckle zu verringern; und

wobei die Anordnung Folgendes aufweist:

- eine erste Konfiguration mit einem Brechungsindex von wenigstens 1,5, in der sich einer der wenigstens zwei Teilstrahlen ausbreitet, oder
 - eine zweite Konfiguration, die Silicium aufweist und in der sich einer der wenigstens zwei Teilstrahlen ausbreitet.
2. Vorrichtung nach Anspruch 1, wobei der Brechungsindex der ersten optischen Konfiguration wenigstens 3,0 beträgt.
 3. Vorrichtung nach Anspruch 1, wobei die erste Konfiguration und/oder die zweite Konfiguration ein antireflexionsbeschichtetes BK 7 Glas umfasst.
 4. Vorrichtung nach Anspruch 3, wobei das Glas eine Dicke von etwa 1,6 mm bis etwa 7,7 mm hat.
 5. Vorrichtung nach Anspruch 1, wobei die erste Konfiguration und/oder die zweite Konfiguration ein antireflexionsbeschichtetes Glas mit einem Brechungsindex von etwa 1,51 bis etwa 3,5 umfasst.

Revendications

1. Appareil de tomographie par cohérence optique (5) pour irradier un échantillon, comportant :
 - a) un interféromètre dans une configuration de rétrodiffusion acheminant un rayonnement électromagnétique ; l'interféromètre comportant :
 - un bras à échantillon recevant le rayonnement électromagnétique, le bras à échantillon comprenant un dispositif configuré pour séparer au moins deux faisceaux (1, 2) du rayonnement électromagnétique de manière à irradier l'échantillon, et le dispositif étant configuré pour retarder un premier faisceau (1) des au moins deux faisceaux par rapport à un second faisceau (2) des au moins deux faisceaux, dans lequel le retard est une différence dans une longueur de trajet optique, et
 - un bras de référence fournissant un rayonnement électromagnétique supplémentaire, dans lequel l'interféromètre reçoit le premier faisceau (1), le second faisceau (2) et le rayonnement supplémentaire, et forme un signal résultant, basé sur les premier et second faisceaux et sur le rayonnement supplémentaire ;
 - b) un dispositif de traitement configuré pour générer une première image basée sur le premier faisceau (1), une seconde image basée sur le second faisceau (2), et une image supplémentaire basée sur les première et seconde images, dans lequel les première et seconde images sont différentes l'une de l'autre, dans lequel l'image supplémentaire est générée sur la base d'une combinaison mathématique incohérente des première et seconde images de manière à réduire la granularité une, et
- dans lequel le dispositif a :
 - une première configuration ayant un indice de réfraction d'au moins 1,5, et propageant l'un des au moins deux faisceaux, ou
 - une seconde configuration comportant du silicium, et propageant l'un des au moins deux faisceaux.
2. Appareil selon la revendication 1, dans lequel l'indice de réfraction de la première configuration optique est d'au moins 3,0.
3. Appareil selon la revendication 1, dans lequel au moins l'une de la première configuration ou de la seconde configuration comporte un verre BK7 avec un revêtement anti-reflet.
4. Appareil selon la revendication 3, dans lequel le verre a une épaisseur d'environ 1,6 mm à environ 7,7 mm.
5. Appareil selon la revendication 1, dans lequel au moins l'une de la première configuration ou de la seconde configuration comporte un verre avec un revêtement anti-reflet ayant un indice de réfraction allant d'environ 1,51 à environ 3,5.

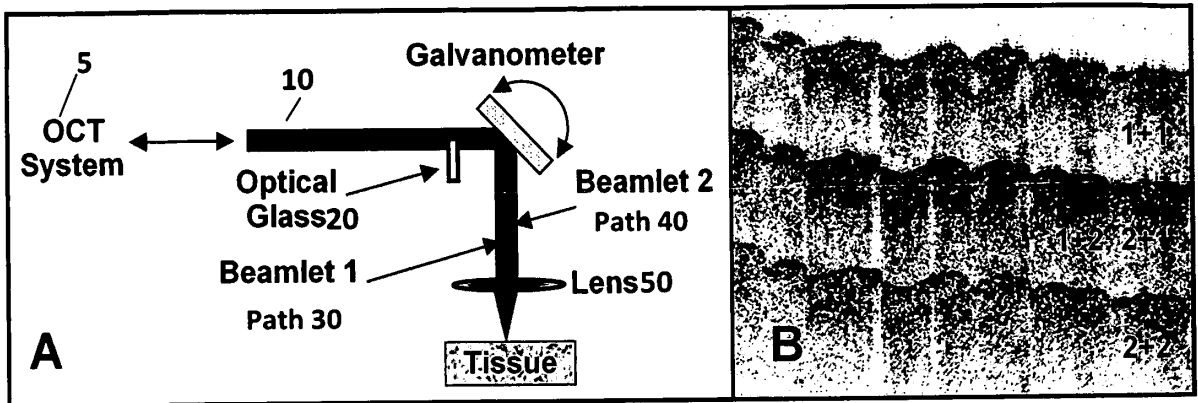


Fig. 1

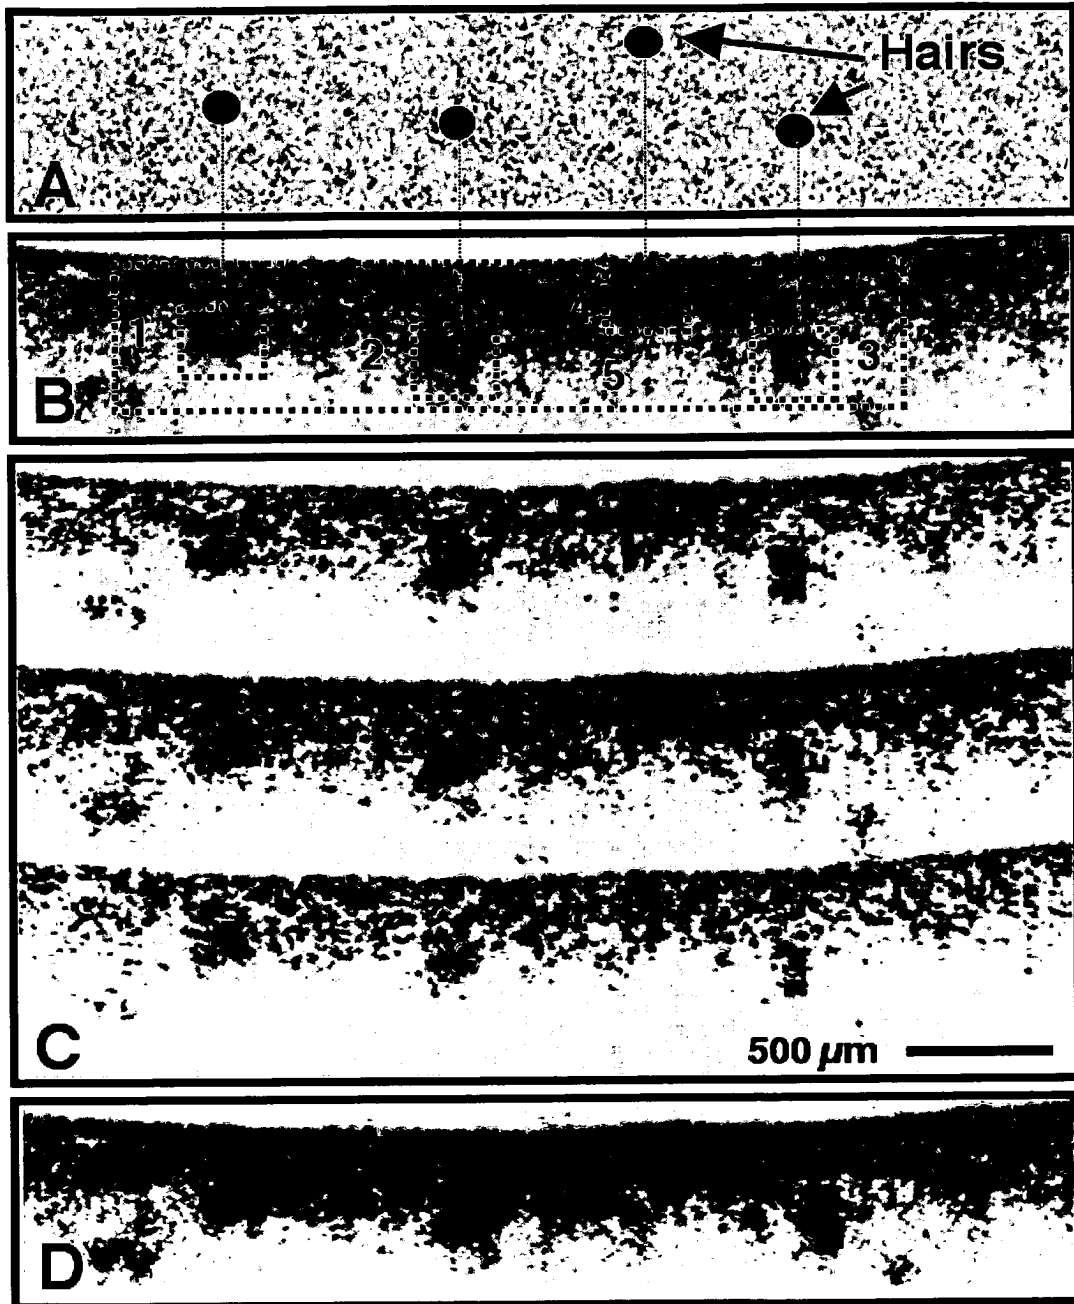


Fig. 2

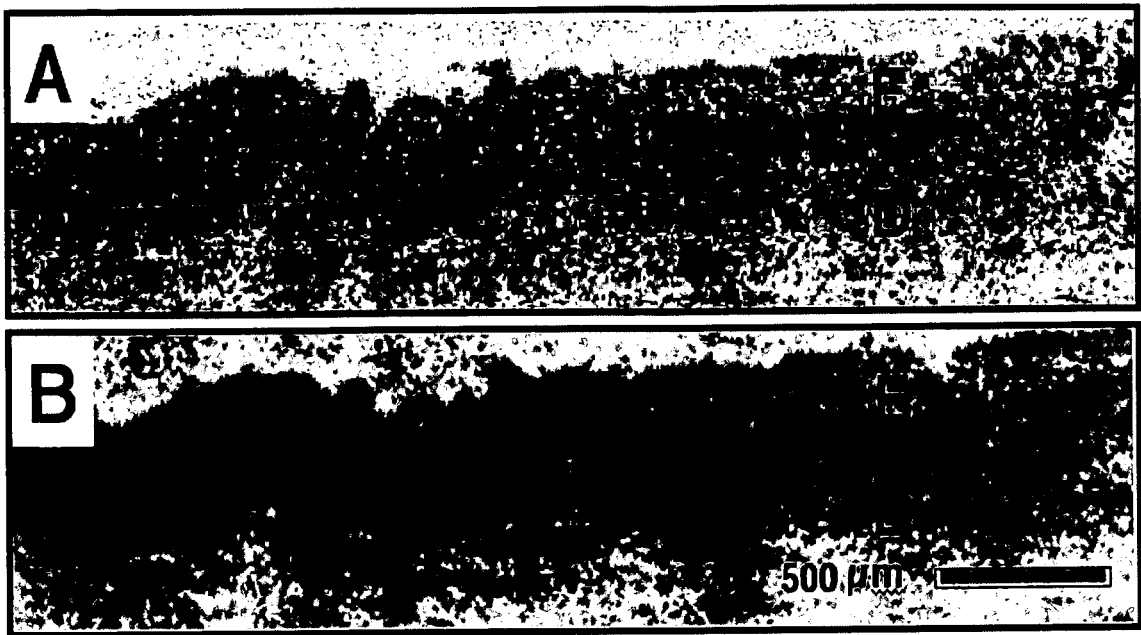


Fig. 3

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Non-patent literature cited in the description

- **J. M. SCHMITT.** Array Detection for Speckle Reduction in Optical Coherence Microscopy. *Phys. Med. Biol.*, 1997, vol. 42, 1427-1429 **[0004]**
- **M. BASHKANSKY ; J. REINTJES.** Statistics and reduction of Speckle in Optical Coherence Tomography. *Opt. Lett.*, 2000, vol. 25, 545-547 **[0005]**

专利名称(译)	通过路径长度编码角度复合的光学相干断层扫描中的斑点减少		
公开(公告)号	EP2436307B1	公开(公告)日	2015-10-21
申请号	EP2011188120	申请日	2004-03-31
[标]申请(专利权)人(译)	通用医疗公司		
申请(专利权)人(译)	总医院CORPORATION		
当前申请(专利权)人(译)	总医院CORPORATION		
[标]发明人	TEARNEY GUILLERMO J IFTIMIA NICUSOR BOUMA BRETT E		
发明人	TEARNEY, GUILLERMO, J. IFTIMIA, NICUSOR BOUMA, BRETT, E.		
IPC分类号	A61B5/00 G01N21/47 G02B27/48 G01B9/02 G01J9/02		
CPC分类号	A61B5/0066 A61B5/0059 A61B5/6852 G01B9/02028 G01B9/02082 G01B9/02087 G01B9/02091 G01J9/0215 G01N21/4795 G02B26/105 G02B27/48		
代理机构(译)	MAIWALD专利ADVOCATE GMBH		
优先权	60/476600 2003-06-06 US 60/514769 2003-10-27 US 60/459543 2003-03-31 US		
其他公开文献	EP2436307A1		
外部链接	Espacenet		

摘要(译)

用于照射样品的装置，包括转发电磁辐射的干涉仪和接收电磁辐射的样品臂，其中样品臂包括配置成从电磁辐射产生至少两个辐射以便照射样品的装置，和延迟相对于至少两个辐射的第二辐射的至少两个辐射的第一辐射。

$$SNR_{ACPE} = \frac{\langle S_{OCT} \rangle}{\sqrt{\text{var}[S_{OCT}]}} \propto \frac{\sum_{i=1}^N u_i}{\sqrt{\sum_{i=1}^N u_i^2}},$$