



(11) **EP 2 554 118 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:

08.10.2014 Bulletin 2014/41

(21) Application number: **11762715.8**

(22) Date of filing: **25.03.2011**

(51) Int Cl.:

A61B 5/15 (2006.01) **A61B 5/151** (2006.01)
A61M 5/00 (2006.01) **A61M 5/178** (2006.01)
A61B 5/00 (2006.01) **A61B 5/153** (2006.01)
A61M 5/42 (2006.01)

(86) International application number:

PCT/JP2011/057410

(87) International publication number:

WO 2011/122484 (06.10.2011 Gazette 2011/40)

(54) **BLOOD SAMPLING DEVICE**

VORRICHTUNG FÜR BLUTABNAHME

DISPOSITIF DE PRÉLÈVEMENT DE SANG

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **27.03.2010 JP 2010073947**

(43) Date of publication of application:

06.02.2013 Bulletin 2013/06

(73) Proprietors:

- **NIPRO CORPORATION**
Osaka-shi, Osaka 531-8510 (JP)
- **The Ritsumeikan Trust**
Kyoto-shi, Kyoto 604-8520 (JP)

(72) Inventors:

- **KONISHI, Satoshi**
Kusatsu-shi
Shiga 525-8577 (JP)
- **KOBAYASHI, Taizo**
Horono-cho, Uji-shi
Kyoto 611-0031 (JP)

- **YOSHIDA, Hiroshi**
Osaka-shi
Osaka 531-8510 (JP)
- **WADA, Takashi**
Kobe-shi
Hyogo 650-0022 (JP)
- **HAGIWARA, Fumihiro**
Kobe-shi
Hyogo 650-0022 (JP)
- **TAKEYAMA, Norihide**
Mitaka-shi
Tokyo 181-0013 (JP)

(74) Representative: **Bertsch, Florian Oliver**

Kraus & Weisert
Patentanwälte PartGmbB
Thomas-Wimmer-Ring 15
80539 München (DE)

(56) References cited:

JP-A- 2006 102 360 JP-A- 2007 125 324
JP-A- 2009 064 455

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

Technical Field

[0001] The present invention relates to a blood sampling device which samples blood from subcutaneous blood vessels, and particularly relates to one which specifies the position of blood vessels using near-infrared rays.

Background Art

[0002] A blood vessel position presenting apparatus which is one of former blood position specifying devices is described with reference to Fig. 11. The blood vessel position presenting apparatus is a device capable of confirming the position and the direction of blood vessels.

[0003] The blood vessel position presenting apparatus of Fig. 11 is constituted including an image pick-up unit 101, an image processing unit 102, an illuminating unit 103, a display unit 104, a mark control unit 105, and a mark illuminating unit 106.

[0004] The illuminating unit 103 irradiates a living body with a near-infrared illumination light beam 127 which is an illumination light beam of a near-infrared wavelength region and is constituted including a near-infrared LED.

[0005] The image pick-up unit 101 takes a photograph of a living body and is, for example, a monochrome CCD camera or a monochrome CMOS camera having high spectral sensitivity from visible wavelength to near infrared wavelength region. The image pick-up information obtained from a reflected light beam 129 from a living body is transferred to the image processing unit 102 as a living body image information 121. The image pick-up unit 101 obtains a near-infrared image information which is living body image information when emitting the illumination light beam and a non-light image information which is living body image information when not emitting the illumination light beam, and then transfers the same to the image processing unit.

[0006] The display unit 104 displays an image based on an image information 124 output from the image processing unit 102 with a liquid crystal display or the like.

[0007] The mark illuminating unit 106 emits a puncture mark projecting light beam 128 for projecting a puncture mark showing a puncture position to the surface of a living body and is constituted including a visible light laser. The mark illuminating unit 106 emits the puncture mark projecting light beam 128 at an illumination timing and in an illumination direction based on a drive signal 126 from the mark control unit 105.

[0008] The mark control unit 105 generates the drive signal 126 based on an instruction signal 122 from the image processing unit 102. The instruction signal 122 contains a deviation information of the display position of the puncture mark included in an image displayed on the display unit 104 and the target position of the puncture mark input from the outside.

[0009] The mark control unit 105 generates the drive signal 126 for matching the display position of the puncture mark with the target position of the puncture mark utilizing this deviation information.

5 **[0010]** The image processing unit 102 generates a processed near-infrared image information in which a blood vessel image and an injection needle image are emphasized based on the near-infrared image information which is a living body image information when emitting an illumination light beam, and generates a processed non-light image information in which a puncture mark image is emphasized based on the non-light image information which is a living body image information when not emitting an illumination light beam. Then, the processed near-infrared image information and the processed non-light image information are synthesized to obtain a display image information.

10 **[0011]** The elements illustrated in Fig. 11 are stored in a predetermined case, and are disposed at a predetermined positional relationship with a living body whose blood vessel position is to be detected for use.

15 **[0012]** Fig. 12 illustrates a general view of an example of the blood vessel position presenting apparatus. Fig. 12 illustrates an example in which the blood vessel position presenting apparatus and a living body are not fixed, and a case 202 is supported by scaffolds 209 and 210. The scaffolds 209 and 210 stabilize the case 202 and an arm 201 whose blood vessel position is to be detected in a state where the case 202 and the arm 201 are separated at a predetermined interval and the apparatus is disposed in such a manner that the case 202 and the scaffolds 209 and 210 surround the arm 201.

20 **[0013]** The case 202 is provided, on the upper surface, with a liquid crystal display portion 203 constituting the display unit 104, a trackball 204 which moves a cursor 207 displayed on the liquid crystal display portion 203, and an input button 208 for setting the position of the cursor 207 as a target position of a puncture mark. On the liquid crystal display portion 203 of Fig. 2, blood vessels 206 and the cursor 207 are displayed. Onto the surface of the arm 201, a puncture mark 205 in the shape of a spot is projected.

25 **[0014]** When using the blood vessel position presenting apparatus of Fig. 12, a doctor and a nurse move the cursor 207 for setting the target position of the puncture mark using the trackball 204 on the screen of the liquid crystal display portion 203, and then pushing the input button 208 to thereby fix the position indicated by the cursor 207 as the target position of the puncture mark. 30 The puncture mark 205 is a mark projected by the mark illuminating unit 106, and looks red to the naked eye. The puncture mark 205 indicates an arbitrary portion on the surface of the arm 201 in the initial state. When the target position is fixed by the cursor 207, a red visible light laser of the mark illuminating unit 106 changes the direction in such a manner that the position of the puncture mark 205 and the target position (the position of the cursor at this time) are matched on an image taken by the image pick- 35 40 45 50 55

up unit 101.

[0015] The image processing unit 102 receives the near-infrared image information obtained when the illumination unit 103 emits a near-infrared light beam and the non-light image information obtained when the illumination unit 103 does not emit a light beam as a living body image information 121 from the image pick-up unit 101. As an example, the two kinds of image information are alternately input in time division. Since the venous blood has high absorptivity of a near-infrared light beam, a blood vessel portion appears in black and an injection needle appears in white on the image based on the near-infrared image information. On an image based on the non-light image information, the puncture mark projected onto the arm 201 by a puncture mark projecting light beam 128 which is a visible light beam appears.

Citation List

[Patent Documents]

[0016] [Patent Document 1] Japanese Unexamined Patent Application Publication No. 2006-102110

Summary of Invention

Problems to be Solved by the Invention

[0017] The above-described blood vessel position presenting apparatus needs to be improved as described below. In the blood vessel position presenting apparatus, the image processing unit 102 synthesizes a processed near-infrared image information and a processed non-light image information to generate a display image information. Moreover, the image processing unit 102 generates a processed near-infrared image information in which a blood vessel image and an injection needle image are emphasized based on the near-infrared image information. Furthermore, the image processing unit 102 generates a processed non-light image information in which an image of a puncture mark is emphasized based on non-light image information.

[0018] Thus, the former blood vessel position presenting apparatus presents a blood vessel position by processing a predetermined image information. Therefore, an image processing unit having high processing capability is required.

[0019] In order to treat image information, a display unit 104, such as a liquid crystal display for displaying the image information, is required. Furthermore, a mark illuminating unit 106 is required which emits a puncture mark projecting light beam 128 for projecting a puncture mark for indicating a puncture position on the surface of a living body.

[0020] Thus, since the former blood vessel position presenting apparatus requires a large number of components, the device itself becomes large. Thus, the device needs to be improved in that and it is difficult to use

the device regardless of time or place, for example during going out.

[0021] Moreover, since the former blood vessel position presenting apparatus requires a large number of components and also requires expensive components, the device needs to be improved in that the device is difficult for an individual to own.

[0022] Then, the present invention aims at providing a blood vessel position specifying device capable of easily specifying the position of blood vessels.

Effects of the Invention

[0023] Means for solving the problems to be solved in the invention and the effects of the invention are described below.

[0024] The blood vessel position specifying device according to the invention is a blood vessel position specifying device which specifies the position of blood vessels present under the skin. The blood vessel position specifying device has: a light projection unit which has a light projection axis having a predetermined angle to the normal line of a predetermined irradiated surface and which projects a near-infrared ray toward the intersection of the light projection axis and the normal line; a spectral lens which is located at the same side as the side where the light projection unit is located relative to the irradiated surface, which receives the reflected light beam of the near-infrared ray projected by the light projection unit, which disperses the reflected light beam, and which has an optical axis having a predetermined angle to the normal line of the irradiated surface; a light receiving unit having a light receiving surface which receives the dispersed reflected light beam; and a blood vessel position calculation unit which calculates the position of the blood vessel based on the brightness of the reflected light beam on the light receiving surface, in which the intersection of the light projection axis and the optical axis of the spectral lens is located at the side opposite to the side where the light projection unit and the spectral lens are located relative to the irradiated surface.

[0025] When near-infrared rays are projected to the skin, the near-infrared rays are absorbed, at a position where a blood vessel is present under the skin, by the blood vessel. In contrast, at a position where a blood vessel is not present, the rays are diffused on the skin surface and in the skin, and some rays become reflected light beams heading to the outside of the skin. Therefore, by receiving the reflected light beams of the near-infrared rays projected to the skin, and then dispersing the same relative to the normal line direction of the irradiated surface to analyze a change in the brightness of the reflected light beams, the position of the blood vessel can be specified.

[0026] Thus, the blood vessel position specifying device according to the invention can easily specify the position of a blood vessel based on the change in the brightness of reflected light beams of near-infrared light beams.

[0027] In the blood vessel position specifying device according to the invention, the light receiving unit is disposed in such a manner that the light receiving surface inclines to the optical axis.

[0028] Thus, the image formation position at the light receiving surface of the dispersed reflected light beams can be changed according to the depth in the normal line direction of the irradiated surface. Therefore, the blood vessel position specifying device according to the invention can easily specify the position of blood vessels based on a change in the brightness of the reflected light beams of near-infrared light beams.

[0029] In the blood vessel position specifying device according to the invention, the light projection axis of the light projection unit and the optical axis of the spectral lens are present in the same plane.

[0030] Thus, the position of a blood vessel present in parallel to the plane where the light projection axis of the light projection unit and the optical axis of the spectral lens are present can be specified with good accuracy.

[0031] In the blood vessel position specifying device according to the invention, the plane including the light projection axis of the light projection unit and the normal line of the irradiated surface and the plane including the optical axis of the spectral lens and the normal line of the irradiated surface are disposed at a predetermined angle.

[0032] Thus, the position of a blood vessel present at a predetermined angle to the plane where the light projection axis of the light projection unit and the optical axis of the spectral lens are present can be specified with good accuracy.

[0033] In the blood vessel position specifying device according to the invention, the plane including the light projection axis of the light projection unit and the normal line of the irradiated surface and the plane including the optical axis of the spectral lens and the normal line of the irradiated surface are disposed at 90°.

[0034] Thus, the position of a blood vessel present at 90° to the plane where the light projection axis of the light projection unit and the optical axis of the spectral lens are present can be specified with good accuracy. By disposing the plane including the light projection axis of the light projection unit and the normal line of the irradiated surface in such a manner as to be orthogonal to each other, the position of blood vessels from a blood vessel present in parallel to the plane where the light projection axis of the light projection unit and the optical axis of the spectral lens are present to a blood vessel present at 90° to the plane where the light projection axis of the light projection unit and the optical axis of the spectral lens are present can be specified with good accuracy.

[0035] In the blood vessel position specifying device according to the invention, the spectral lens is an aspherical lens. Thus, reflected light beams can be dispersed with good accuracy.

[0036] A blood sampling device according to the invention is a blood sampling device which samples blood from a blood vessel present under the skin and has the blood

vessel position specifying device according to any one of Claims 1 to Claim 6 and a needle projecting unit having a needle for use in blood sampling and projecting the needle to the calculated blood vessel position.

[0037] Thus, a user can certainly and easily sample blood without failing in sampling of blood.

Brief Description of Drawings

[0038]

[Fig. 1] Fig. 1 is an outside view of a blood sampling device 100 containing a blood vessel position specifying device 111 according to the invention.

[Fig. 2] Fig. 2 is an outside view of the blood sampling device 100 containing the blood vessel position specifying device 111 according to the invention.

[Fig. 3] Fig. 3 is an upper surface view of the blood sampling device 100.

[Fig. 4] Fig. 4 is a cross sectional view of the X-X cross section in Fig. 3.

[Fig. 5] Fig. 5 is a cross sectional view of the Y-Y cross section in Fig. 3.

[Fig. 6] Fig. 6 is a view for explaining the principle of a method for specifying a blood vessel position.

[Fig. 7] Fig. 7 is a view illustrating the conditions of simulation.

[Fig. 8] Fig. 8 is a view illustrating simulation results.

[Fig. 9] Fig. 9 is a view illustrating simulation results.

[Fig. 10] Fig. 10 is a view illustrating simulation results.

[Fig. 11] Fig. 11 is a view illustrating an example of a former blood vessel position specifying device.

[Fig. 12] Fig. 12 is a view illustrating an example of a former blood vessel position specifying device.

Modes for Carrying out the Invention

[0039] Hereinafter, embodiments of the invention are described in detail with reference to the drawings.

[Embodiment 1]

1. Configuration

1. Configuration of blood sampling device 100

[0040] A blood sampling device 100 according to the invention is described with reference to Fig. 1. Fig. 1 illustrates a perspective view of the blood sampling device 100 as viewed from an obliquely upper side. The blood sampling device 100 has a blood vessel position specifying device 111 and a puncture device 113. The puncture device 113 is a device which inserts an injection needle into a blood vessel from the outside of the body to sample blood. The blood vessel position specifying device 111 is a device which specifies the position of a blood vessel from which blood is sampled.

[0041] The puncture device 113 can be attached to and detached from the blood vessel position specifying device 111. The puncture device 113 has a puncture needle 113b (Fig. 2) therein. The puncture device 113 is provided with a puncture button B113 at the side surface. The puncture device 113 projects the puncture needle 113b disposed inside to the outside when the puncture button B113 is pushed.

[0042] Fig. 2 illustrates a perspective view of the blood sampling device 100 as viewed from an obliquely lower side. In the blood sampling device 100, the blood vessel position specifying device 111 has a puncture aperture 111a and a close contact surface 111s at the bottom. The close contact surface 111s is disposed around the puncture aperture 111a. The puncture needle 113b of the puncture device 113 is projected to the outside from the puncture aperture 111a.

[0043] A user of the blood sampling device 100 attaches the puncture device 113 to the blood vessel position specifying device 111. The user disposes the puncture device 113 in such a manner that the skin from which blood is to be sampled is brought into close contact with the close contact surface 111s. At this time, an irradiated surface is formed by the skin located at the position of the puncture aperture 111a of the blood vessel position specifying device 111.

[0044] After disposing the blood vessel position specifying device 111, the puncture button B113 is pushed. Thus, the puncture needle 113b is projected from the tip of the puncture device 113 to be inserted into the body.

2. Configuration of blood vessel position specifying device 111

[0045] The configuration of the blood vessel position specifying device 111 is described with reference to Figs. 3, 4, and 5. Fig. 3 illustrates the top view of the blood sampling device 100. Fig. 4 illustrates the X-X cross section of the blood sampling device 100 illustrated in Fig. 3 and Fig. 5 illustrates the Y-Y cross section thereof. Figs. 4 and 5 illustrate a state where the blood sampling device 100 is disposed at a predetermined position of a target person. Fig. 4 also illustrates a partial cross sectional view of the blood sampling device 100.

[0046] As illustrated in Fig. 4, the blood vessel position specifying device 111 has a near-infrared light emitting unit 121, a reflected light receiving unit 123, and a case 125. The near-infrared light emitting unit 121 and the reflected light receiving unit 123 are attached to predetermined positions of the case 125.

[0047] The near-infrared light emitting unit 121 has a near-infrared light emitting diode 121d, a light emission side lens 121c, and a case 121k. The near-infrared light emitting unit 121 has an optical axis J121 (hereinafter referred to as a light emitting unit optical axis J121). The near-infrared light emitting diode 121d is fixed to a predetermined position of the case 121k in such a manner that the central axis is in agreement with the light emitting

unit optical axis J121. The light emission side lens 121c is fixed to a predetermined position of the case 121k in such a manner that the optical axis is in agreement with the light emitting unit optical axis J121.

[0048] The light emitting unit optical axis J121 of the near-infrared light emitting unit 121 has an angle α to a normal line N1 of an irradiated surface P1. The near-infrared light emitting unit 121 projects near-infrared rays toward an intersection Q1 of the light emitting unit optical axis J121 and a normal line N1 of the irradiated surface P1 (light projection direction).

[0049] The near-infrared light emitting diode 121d emits near-infrared light beams with a wavelength of 700 nm to 3000 nm between visible light and infrared light. It is known that the near-infrared light beam is absorbed by the hemoglobin of blood. The near-infrared light emitting diode 121d is connected to a predetermined control portion and a power supply portion through a connection line 1211.

[0050] The reflected light receiving unit 123 has a light receiving side lens 123c, a photodiode array 123f, and a case 123k. The light receiving side lens 123c is an aspherical lens. The light receiving side lens 123c disperses reflected light beams of near-infrared rays projected by the near-infrared light emitting unit 121. The optical axis J123 of the light receiving side lens 123c has an angle β to the normal line direction N1 of the irradiated surface P1. The light receiving side lens 123c is fixed to a predetermined position of the case 123k.

[0051] The photodiode array 123f is one in which a plurality of photodiodes are arranged in a predetermined shape. The photodiode array 123f receives the reflected light beams dispersed by the light receiving side lens 123c with the front surface as a light receiving surface P3. The light receiving surface P3 of the photodiode array 123 has an angle γ to the light receiving unit optical axis J123. Thus, by disposing the photodiode array 123 in such a manner that the light receiving surface P3 inclines to the light receiving unit optical axis J123, a change in a substance in the normal line direction N1 of the incidence plane P1 can be obtained as a change in the illumination of the reflected light beams at the light receiving surface P3.

[0052] The photodiode array 123f is connected to an analysis circuit (not illustrated) and the like through the connection line 1231.

[0053] The light emitting unit optical axis J121 and the optical axis of the light receiving side lens 123c are present in the same plane. The light emitting unit optical axis J121 and the optical axis J123 of the light receiving side lens 123c are disposed in such a manner as to cross at a position with a distance d from the irradiated surface P1 to the inside of the body. The blood vessel position specifying device 111 detects whether or not a blood vessel is present at the intersection of the light emitting unit optical axis J121 and the optical axis J123c.

[0054] By selecting as appropriate, on the basis of the used conditions and components utilized, the angle α

between the light emitting unit optical axis J121 of the near-infrared light emitting unit 121 and the normal line N1 of the irradiated surface P1, the angle β between the optical axis J123 of the light receiving side lens 123c and the normal line direction N1 of the irradiated surface P1, and the angle γ between the light receiving surface P3 of the photodiode array 123 and the light receiving unit optical axis J123, the blood vessel position can be more appropriately specified.

[0055] The analysis circuit is connected to the photodiode array 123f. The analysis circuit calculates the illumination in the depth direction of the normal line N1 of the irradiated surface P1 from light receiving results of the photodiode array 123f.

[0056] As illustrated in Fig. 5, the blood vessel position specifying device 111 further has another near-infrared light emitting unit 127. The configuration of the near-infrared light emitting unit 127 is the same as that of the near-infrared light emitting unit 121. The plane including the light emitting unit optical axis J127 of the near-infrared light emitting unit 127 and the normal line N1 of the irradiated surface P1 and the plane including the optical axis J123 of the light receiving side lens 123c and the normal line N1 of the irradiated surface P1 are disposed at 90°.

[0057] Thus, by disposing a plurality of near-infrared light emitting units at different positions to the reflected light receiving unit 123, the position of blood vessels can be specified irrespective of the arrangement state of blood vessels.

[0058] The case 125 has the near-infrared light emitting units 121 and 127 and the reflected light receiving unit 123 therein. The case 125 has the close contact surface 111s contacting the skin surface on the bottom. The case 125 further has the puncture aperture 111a in the close contact surface 111s. The surface where the puncture aperture 111a opens forms the irradiated surface P1. While the puncture aperture 111a allows near-infrared rays projected by the infrared light emitting units 121 and 127 to pass to the outside and allows only reflected light beams required for specifying the position of blood vessels to pass to the inside, the puncture aperture 111a prevents passage of unnecessary reflected light beams, such as a disturbance light beam.

[0059] The blood vessel position specifying device 111 starts to specify the position of blood vessels when a measurement starting button (not illustrated) provided at the case 125 is operated.

2. Principle for specifying blood vessel position and simulation results

[0060] The principle of the method for specifying a blood vessel position in the blood vessel position specifying device 111 is described with reference to Fig. 6. Near-infrared light beams R1 projected from the near-infrared light emitting diode 121d enter the skin through the light emission side lens 121c. Some of the near-infrared light beams R1 entering the skin become reflected

light beams R3 on the skin surface. The other near-infrared light beams R1 enter the inside of the skin. The near-infrared light beams entering the inside of the skin repeats diffused reflection in the skin, and some light beams become reflected light beams R5 from the inside of the skin to go out to the outside from the skin surface.

[0061] A near-infrared light R7 which has reached a blood vessel among the near-infrared light beams entering the inside of the skin is absorbed by hemoglobin in the blood vessel.

[0062] Thus, the near-infrared light R7 absorbed into blood is not contained in the reflected light beams of the near-infrared light beams R1 projected by the near-infrared light emitting unit 121d. Therefore, by analyzing the reflected light beams of the near-infrared light beams R1, the position where blood is present, i.e., the position of blood vessels, can be specified.

[0063] Figs. 7 to 10 show experimental results of specifying the position of a blood vessel by the blood vessel position specifying device 111. Figs. 7 to 10 show the results of simulating, by a computer, a course of the near-infrared light beams R1 projected by the near-infrared light emitting unit 121d.

[0064] Fig. 7 shows conditions of a model built in the simulation. As illustrated in Fig. 7, in this simulation, a blood vessel is dealt as a Mie scattering body. Therefore, the near-infrared light beam which has reached the blood vessel is not absorbed into the blood in the blood vessel but is reflected by the blood vessel. Therefore, when the reflected light beams are actually analyzed by the blood vessel position specifying device 111, the intensity of the reflected light beams becomes lower depending on the depth where the blood vessel is present. However, in the simulation, the intensity of the reflected light beams becomes higher depending on the depth where the blood vessel is present.

[0065] Fig. 8 illustrates the results of simulation in the case where two blood vessels are vertically present in parallel to each other under the skin orthogonal to the incidence plane of near-infrared light beams. The blood vessels are made to be present at depths of 1 mm and 5 mm from the skin surface, respectively, as illustrated in the left of Fig. 8.

[0066] In this case, as shown by the illumination distribution on the detection plane illustrated in the right of Fig. 8, the illumination becomes high around a depth of 1 mm and around a depth of 5 mm. More specifically, the blood vessel position specifying device 111 can specify that the blood vessels orthogonal to the incidence plane of near-infrared light beams are present at the depths of 1 mm and 5 mm from the skin surface.

[0067] Fig. 9 shows the results of simulation in a case where one blood vessel is orthogonal to the incidence plane of near-infrared light beams under the skin. As shown in the left of Fig. 9, the blood vessel is made to be present at a depth of 3 mm from the skin surface.

[0068] In this case, as shown by the illumination distribution on the detection surface shown in the right of Fig.

9, the illumination becomes high around a depth of 3 mm. More specifically, the blood vessel position specifying device 111 can specify that the blood vessel orthogonal to the incidence plane of near-infrared light beams is present at a depth of 3 mm from the skin surface.

[0069] Fig. 10 illustrates the results of simulation in a case where one blood vessel is present in parallel to the incidence plane of near-infrared light beams under the skin. As illustrated in the left of Fig. 10, the blood vessel is made to be present at a depth of 3 mm from the skin surface.

[0070] In this case, as shown by the illumination distribution on the detection surface shown in the right of Fig. 10, the illumination becomes higher at a position deeper than a depth of 3 mm. More specifically, the blood vessel position specifying device 111 specifies that the blood vessel present at a depth of 3 mm from the skin surface is present at a position deeper than a depth of 3 mm.

[0071] From the simulation results of Fig. 9 and Fig. 10, the blood vessel position specifying device 111a can more appropriately specify the depth in the case where a blood vessel is orthogonal to the incidence plane of near-infrared light beams rather than the case where a blood vessel is present in parallel to the incidence plane of near-infrared light beams. Therefore, in the blood vessel position specifying device 111, the two near-infrared light emitting units 121 are disposed in such a manner that the incidence planes of near-infrared light beams are orthogonal to each other. This allows more appropriate specification of the position of blood vessels.

[Other embodiments]

(1) Configuration of blood sampling device 100:

[0072] In Embodiment 1 described above, the blood sampling device 100 is constituted by the blood vessel position specifying device 111 and the puncture device 113 which can be detached from each other. However, the blood sampling device 100 may be integrally constituted by the blood vessel position specifying device 111 and the puncture device 113 which cannot be detached from each other.

(2) Arrangement of near-infrared light emitting units:

[0073] Although the two near-infrared light emitting units 121 and 127 are disposed at positions orthogonal to the reflected light receiving unit 123 in Embodiment 1 described above, the position is not limited to the example above insofar as the two near-infrared light emitting units 121 and 127 are disposed at different positions.

[0074] Alternatively, only one near-infrared light emitting unit 121 may be disposed in the blood sampling device 100. Furthermore, three or more near-infrared light emitting units may be disposed at different positions relative to the reflected light receiving unit 123.

(3) Light receiving side lens 123c:

[0075] Although the light receiving side lens 123c is an aspherical lens in Embodiment 1 described above, the lens is not limited to the example above insofar as the lens is a lens capable of dispersing a reflected light beam. For example, a spherical lens may be used.

(4) Photodiode array 123f:

[0076] Although the photodiode array 123f is mentioned as one obtaining the brightness of a reflected light beam in Embodiment 1 described above, the photodiode array 123f is not limited to the example above insofar as the brightness of a reflected light beam can be obtained.

[Industrial availability]

[0077] The blood vessel position specifying device according to the invention can be used for a blood sampling device which samples blood required in a blood test, for example.

Description of Reference Numerals

[0078]

100 Blood sampling device
111 Blood vessel position specifying device
121 Near-infrared light emitting unit
121d Near-infrared light emitting diode
121c Light emission side lens
123 Reflected light receiving unit
123c Light receiving side lens
123f Photodiode array
113 Puncture device
113b Puncture needle

Claims

1. A blood vessel position specifying device (111) which specifies a position of a blood vessel present under skin, the blood vessel position specifying device, comprising:

a light projection unit (121) which has a light projection axis having a predetermined angle to a normal line of a predetermined irradiated surface and which projects a near-infrared ray in a direction of an intersection of the light projection axis (J121) and the normal line (N1) ;
a spectral lens (123c) which is located at the same side as a side where the light projection unit (121) is located relative to the irradiated surface, which receives a reflected light beam of the near-infrared ray projected by the light projection unit (121), which disperses the reflected

- light beam, and which has an optical axis having a predetermined angle to the normal line of the irradiated surface;
 a light receiving unit (123) having a light receiving surface (P3) which receives the dispersed reflected light beam; and
 a blood vessel position calculation unit which calculates a position of the blood vessel based on brightness of the reflected light beam on the light receiving surface,
 the intersection of the light projection axis and the optical axis of the spectral lens being located at a side opposite to the side where the light projection unit and the spectral lens are located relative to the irradiated surface.
2. The blood vessel position specifying device (111) according to Claim 1, wherein the light receiving unit (123) is disposed in such a manner that the light receiving surface inclines to the optical axis.
 3. The blood vessel position specifying device according to Claim 1 or 2, wherein the light projection axis (J121) of the light projection unit (121) and the optical axis of the spectral lens are present in the same plane.
 4. The blood vessel position specifying device according to Claim 1 or 2, wherein a plane including the light projection axis (J121) of the light projection unit (121) and the normal line of the irradiated surface and a plane including the optical axis of the spectral lens (123c) and the normal line of the irradiated surface are disposed at a predetermined angle.
 5. The blood vessel position specifying device according to Claim 4, wherein the plane including the light projection axis (J121) of the light projection unit (121) and the normal line of the irradiated surface and the plane including the optical axis of the spectral lens and the normal line of the irradiated surface are disposed at 90°.
 6. The blood vessel position specifying device according to any one of Claims 1 to 6, wherein the spectral lens (123c) is an aspherical lens.
 7. A blood sampling device (100), which samples blood from a blood vessel present under skin, the blood sampling device, comprising:

the blood vessel position specifying device (111) according to any one of Claims 1 to Claim 6; and
 a needle projecting unit having a needle for use in blood sampling and projecting the needle to the calculated blood vessel position.

8. A blood sampling method for sampling blood from a blood vessel present under skin, the blood sampling method, comprising:

projecting a near-infrared ray while defining a direction having a predetermined angle to a normal line direction of a predetermined irradiated surface as a light projection direction;
 dispersing a reflected light beam of the near-infrared ray projected by the light projection unit using a spectral lens located at the same side as a side where the light projection unit is located relative to the irradiated surface and having a predetermined angle to the normal line direction of the irradiated surface as an optical axis direction;
 receiving the dispersed reflected light beam on a light receiving surface;
 calculating a position of the blood vessel based on brightness of the reflected light beam on the light receiving surface; and
 projecting a needle for use in blood sampling to the calculated blood vessel position.

Patentansprüche

1. Vorrichtung (111) zur Spezifizierung einer Position eines Blutgefäßes, welche eine Position eines Blutgefäßes, welches unter einer Haut vorhanden ist, spezifiziert, wobei die Vorrichtung zur Spezifizierung einer Position eines Blutgefäßes umfasst:

eine Lichtprojektionseinheit (121), welche eine Lichtprojektionsachse aufweist, die einen vorbestimmten Winkel zu einer Normalen einer vorbestimmten bestrahlten Fläche aufweist, und welche einen Infrarotstrahl in einer Richtung eines Schnittpunkts der Lichtprojektionsachse (J121) und der Normalen (N1) projiziert;
 eine Spektrallinse (123c), welche relativ zu der bestrahlten Fläche an derselben Seite wie eine Seite angeordnet ist, wo die Lichtprojektionseinheit (121) angeordnet ist, welche einen reflektierten Lichtstrahl des Infrarotstrahls, welcher durch die Lichtprojektionseinheit (121) projiziert wird, empfängt, welche den reflektierten Lichtstrahl streut und welche eine optische Achse aufweist, die einen vorbestimmten Winkel zu der Normalen der bestrahlten Fläche aufweist;
 eine Lichtempfangseinheit (123), welche eine Lichtempfangsfläche (P3) aufweist, die den gestreuten reflektierten Lichtstrahl empfängt; und
 eine Einheit zur Berechnung einer Position eines Blutgefäßes, welche eine Position des Blutgefäßes abhängig von einer Helligkeit des reflektierten Lichtstrahls auf der Lichtempfangsfläche berechnet,

wobei der Schnittpunkt der Lichtprojektionsachse und der optischen Achse der Spektrallinse an einer Seite gegenüber der Seite angeordnet ist, wo die Lichtprojektionseinheit und die Spektrallinse relativ zu der bestrahlten Fläche angeordnet sind.

2. Vorrichtung (111) zur Spezifizierung einer Position eines Blutgefäßes nach Anspruch 1, wobei die Lichtempfangseinheit (123) in solch einer Weise angeordnet ist, dass die Lichtempfangseinheit schräg zu der optischen Achse angeordnet ist. 10
3. Vorrichtung zur Spezifizierung einer Position eines Blutgefäßes nach Anspruch 1 oder 2, wobei die Lichtprojektionsachse (J121) der Lichtprojektionseinheit (121) und die optische Achse der Spektrallinse in derselben Ebene liegen. 15
4. Vorrichtung zur Spezifizierung einer Position eines Blutgefäßes nach Anspruch 1 oder 2, wobei eine Ebene, welche die Lichtprojektionsachse (J121) der Lichtprojektionseinheit (121) und die Normale der bestrahlten Fläche aufweist, und eine Ebene, welche die optische Achse der Spektrallinse (123c) und die Normale der bestrahlten Fläche aufweist, in einem vorbestimmten Winkel angeordnet sind. 20 25
5. Vorrichtung zur Spezifizierung einer Position eines Blutgefäßes nach Anspruch 4, wobei die Ebene, welche die Lichtprojektionsachse (J121) der Lichtprojektionseinheit (121) und die Normale der bestrahlten Fläche aufweist, und die Ebene, welche die optische Achse der Spektrallinse und die Normale der bestrahlten Fläche aufweist, mit 90° angeordnet sind. 30 35
6. Vorrichtung zur Spezifizierung einer Position eines Blutgefäßes nach einem der Ansprüche 1 bis 6, wobei die Spektrallinse (123c) eine asphärische Linse ist. 40
7. Blutsammelvorrichtung (100), welche Blut von einem Blutgefäß, welches unter einer Haut vorhanden ist, sammelt, wobei die Blutsammelvorrichtung umfasst: 45
 - die Vorrichtung (111) zur Spezifizierung einer Position eines Blutgefäßes nach einem der Ansprüche 1 bis 6; und
 - eine Nadelführungseinheit, welche eine Nadel zum Einsatz beim Blutsammeln aufweist und die Nadel zu der berechneten Position des Blutgefäßes führt. 50 55
8. Verfahren zum Blutsammeln von einem Blutgefäß, welches unter einer Haut vorhanden ist, wobei das

Verfahren zum Blutsammeln umfasst:

Projizieren eines Infrarotstrahls während er eine Richtung, welche einen vorbestimmten Winkel zu einer Normalenrichtung einer vorbestimmten bestrahlten Fläche aufweist, als eine Lichtprojektionsrichtung definiert;
 Streuen eines reflektierten Lichtstrahls des Infrarotstrahls, welcher durch die Lichtprojektionseinheit projiziert wird, mittels einer Spektrallinse, welche relativ zu der bestrahlten Fläche an derselben Seite wie eine Seite angeordnet ist, wo die Lichtprojektionseinheit angeordnet ist, und einen vorbestimmten Winkel zu der Normalenrichtung der bestrahlten Fläche als eine Richtung einer optischen Achse aufweist;
 Empfangen des gestreuten reflektierten Lichtstrahls auf einer Lichtempfangsfläche;
 Berechnen einer Position des Blutgefäßes abhängig von einer Helligkeit des reflektierten Lichtstrahls auf der Lichtempfangsfläche; und
 Führen einer Nadel zum Einsatz beim Blutsammeln zu der berechneten Position des Blutgefäßes.

Revendications

1. Dispositif de spécification de position de vaisseau sanguin (111) qui spécifie une position d'un vaisseau sanguin présent sous la peau, le dispositif de spécification de position de vaisseau sanguin comprenant :

une unité de projection de lumière (121) qui a un axe de projection de lumière ayant un angle prédéterminé par rapport à une ligne verticale d'une surface rayonnée prédéterminée et qui projette un rayon infrarouge proche dans une direction d'une intersection de l'axe de projection de lumière (J121) et de la ligne verticale (N1) ;

une lentille spectrale (123c) qui est positionnée du même côté qu'un côté où l'unité de projection de lumière (121) est positionnée par rapport à la surface rayonnée, qui reçoit un faisceau de lumière reflété du rayon infrarouge proche projeté par l'unité de projection de lumière (121), qui disperse le faisceau de lumière reflété, et qui a un axe optique ayant un angle prédéterminé par rapport à la ligne verticale de la surface rayonnée ;

une unité de réception de lumière (123) ayant une surface de réception de lumière (P3) qui reçoit le faisceau lumineux reflété dispersé ; et une unité de calcul de position de vaisseau sanguin qui calcule une position du vaisseau sanguin en fonction de la brillance du faisceau lu-

- mineux reflété sur la surface de réception de lumière,
l'intersection de l'axe de projection de lumière et de l'axe optique de la lentille spectrale étant positionnée d'un côté opposé au côté où l'unité de projection de lumière et la lentille spectrale sont positionnées par rapport à la surface rayonnée. 5
2. Dispositif de spécification de position de vaisseau sanguin (111) selon la revendication 1, dans lequel : 10
- l'unité de réception de lumière (123) est disposée de sorte que la surface de réception de lumière s'incline par rapport à l'axe optique. 15
3. Dispositif de spécification de position de vaisseau sanguin selon la revendication 1 ou 2, dans lequel :
- l'axe de projection de lumière (J121) de l'unité de projection de lumière (121) et l'axe optique de la lentille spectrale sont présents dans le même plan. 20
4. Dispositif de spécification de position de vaisseau sanguin selon la revendication 1 ou 2, dans lequel : 25
- un plan comprenant l'axe de projection de lumière (J121) de l'unité de projection de lumière (121) et la ligne verticale de la surface rayonnée et un plan comprenant l'axe optique de la lentille spectrale (123c) et la ligne verticale de la surface rayonnée sont disposés à un angle prédéterminé. 30
5. Dispositif de spécification de position de vaisseau sanguin selon la revendication 4, dans lequel : 35
- le plan comprenant l'axe de projection de lumière (J121) de l'unité de projection de lumière (121) et la ligne verticale de la surface rayonnée et le plan comprenant l'axe optique de la lentille spectrale et la ligne verticale de la surface rayonnée sont disposés à 90°. 40
6. Dispositif de spécification de position de vaisseau sanguin selon l'une quelconque des revendications 1 à 6, dans lequel : 45
- la lentille spectrale (123c) est une lentille asphérique. 50
7. Dispositif de prélèvement de sang (100), qui prélève du sang d'un vaisseau sanguin présent sous la peau, le dispositif de prélèvement de sang comprenant : 55
- le dispositif de spécification de position de vaisseau sanguin (111) selon l'une quelconque des


revendications 1 à 6 ; et

une unité de projection d'aiguille ayant une aiguille destinée à être utilisée pour le prélèvement de sang et faisant faire saillie à l'aiguille dans la position de vaisseau sanguin calculée.


8. Procédé de prélèvement de sang pour prélever du sang d'un vaisseau sanguin présent sous la peau, le procédé de prélèvement de sang comprenant les étapes consistant à :

projeter un rayon infrarouge proche tout en définissant une direction ayant un angle prédéterminé par rapport à une direction de ligne verticale d'une surface rayonnée prédéterminée en tant que direction de projection de lumière ;
dispenser un faisceau lumineux reflété du rayon infrarouge proche projeté par l'unité de projection de lumière à l'aide d'une lentille spectrale positionnée du même côté qu'un côté où l'unité de projection de lumière est positionnée par rapport à la surface rayonnée et ayant un angle prédéterminé par rapport à la direction de ligne verticale de la surface rayonnée en tant que direction d'axe optique ;
recevoir le faisceau lumineux reflété dispersé sur une surface de réception de lumière ;
calculer une position du vaisseau sanguin en fonction de la brillance du faisceau lumineux reflété sur la surface de réception de lumière ; et
faire faire saillie à une aiguille destinée à être utilisée pour prélever du sang dans la position de vaisseau sanguin calculée.


[Fig. 1]

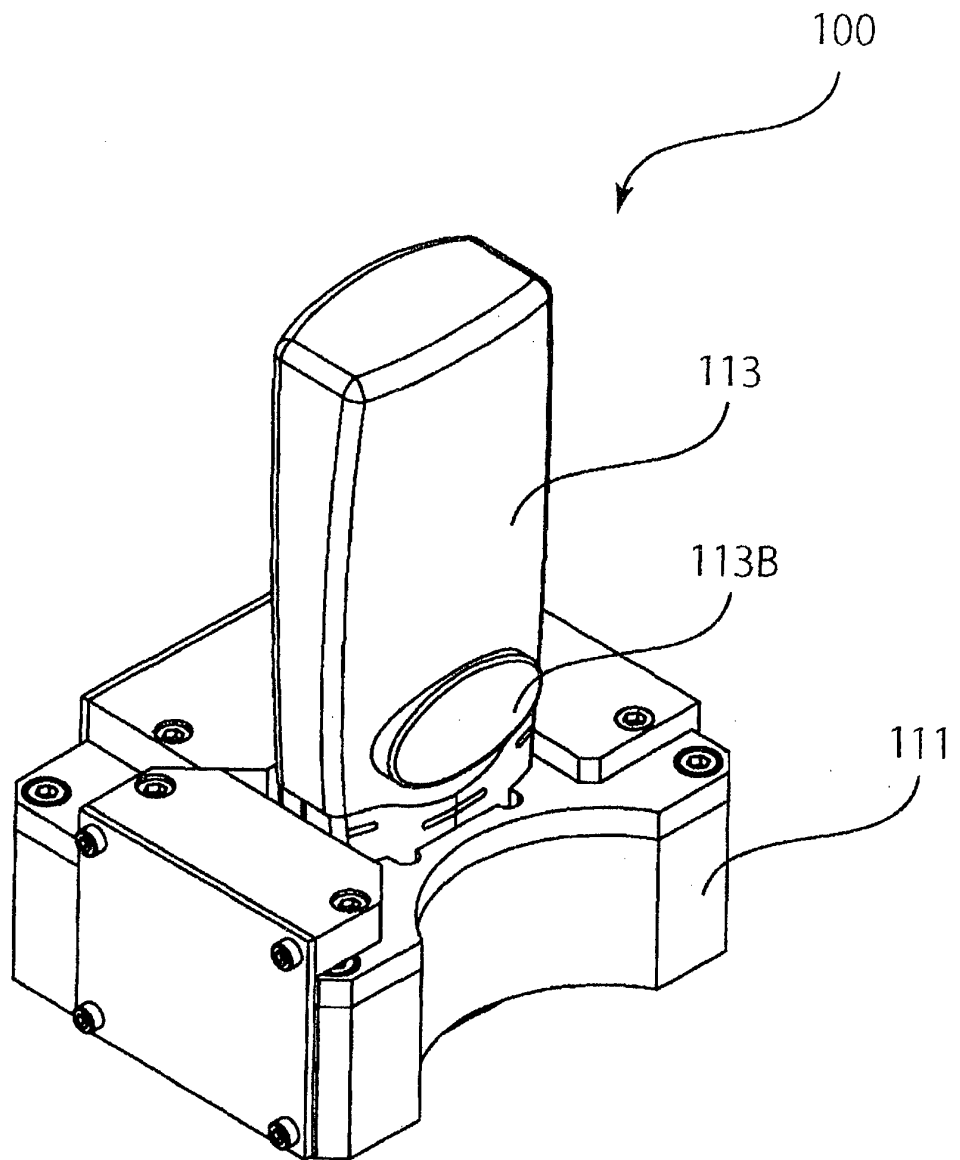


[Fig. 2]

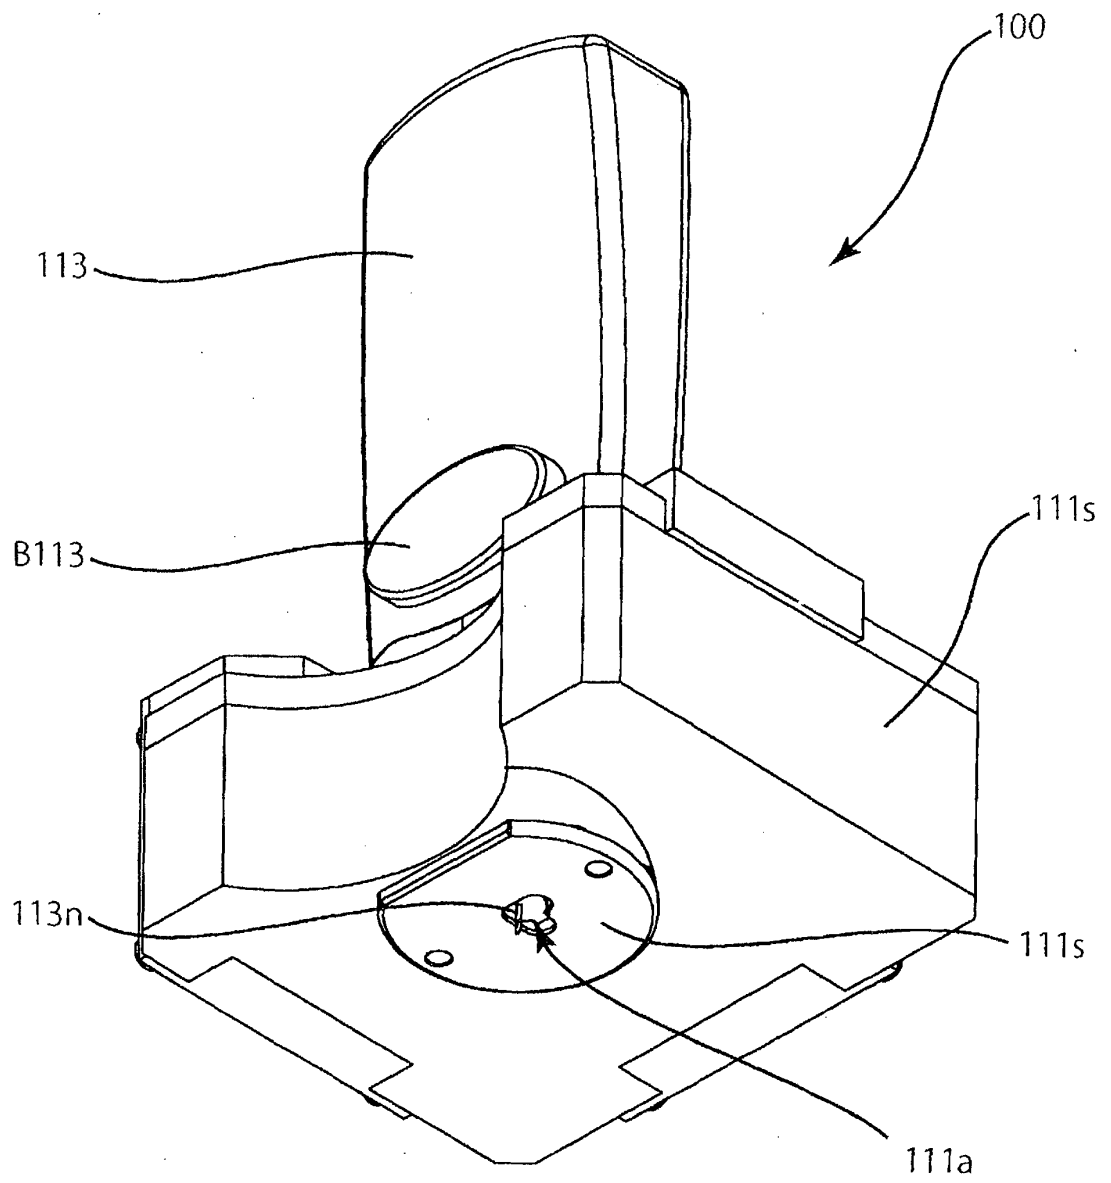


[Fig. 3]

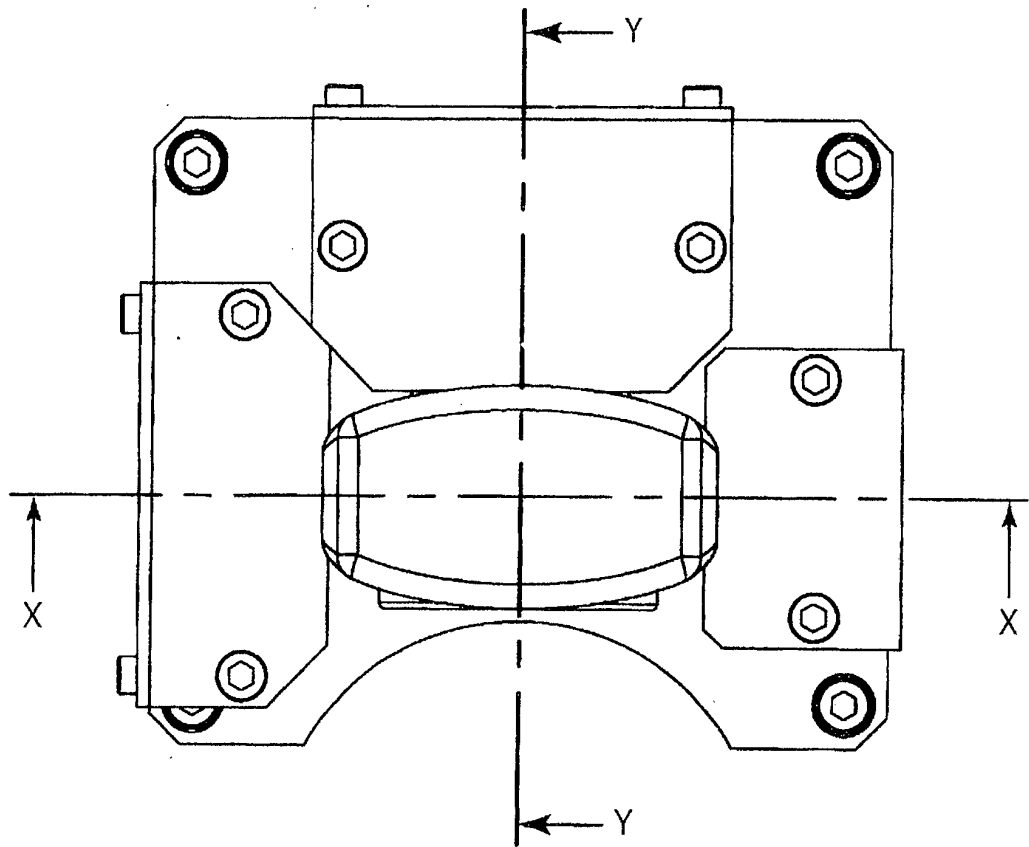


[Fig. 4]

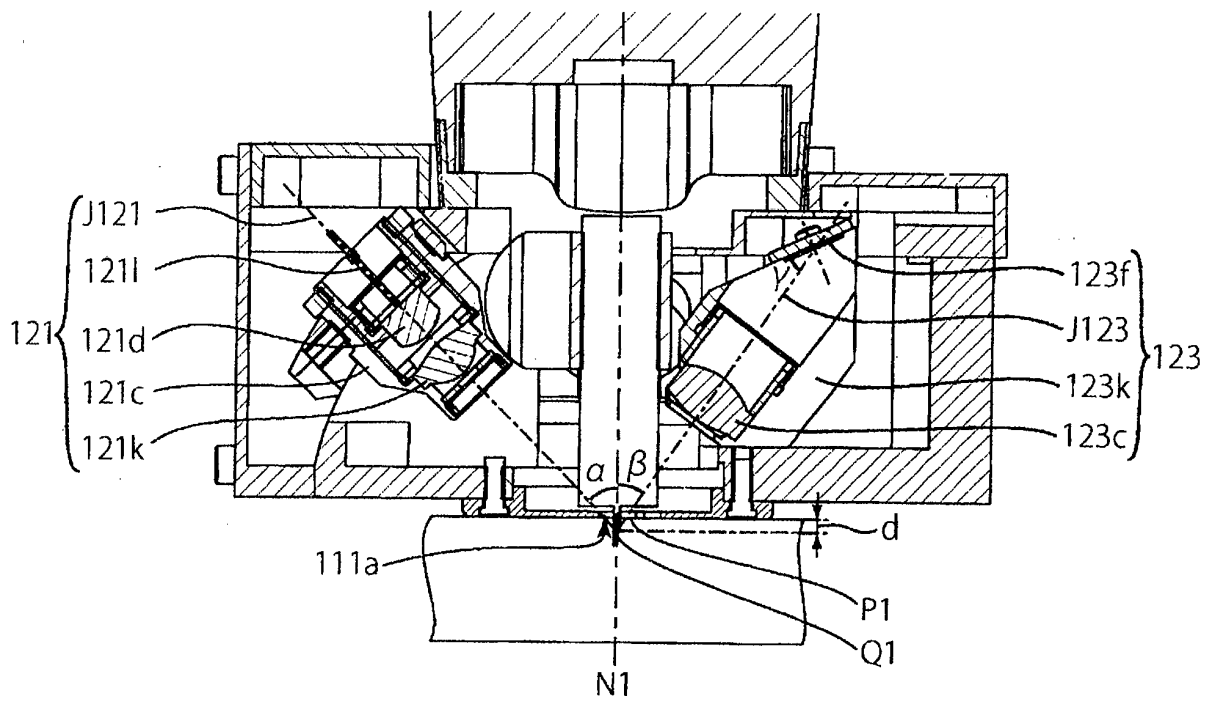


[Fig. 5]

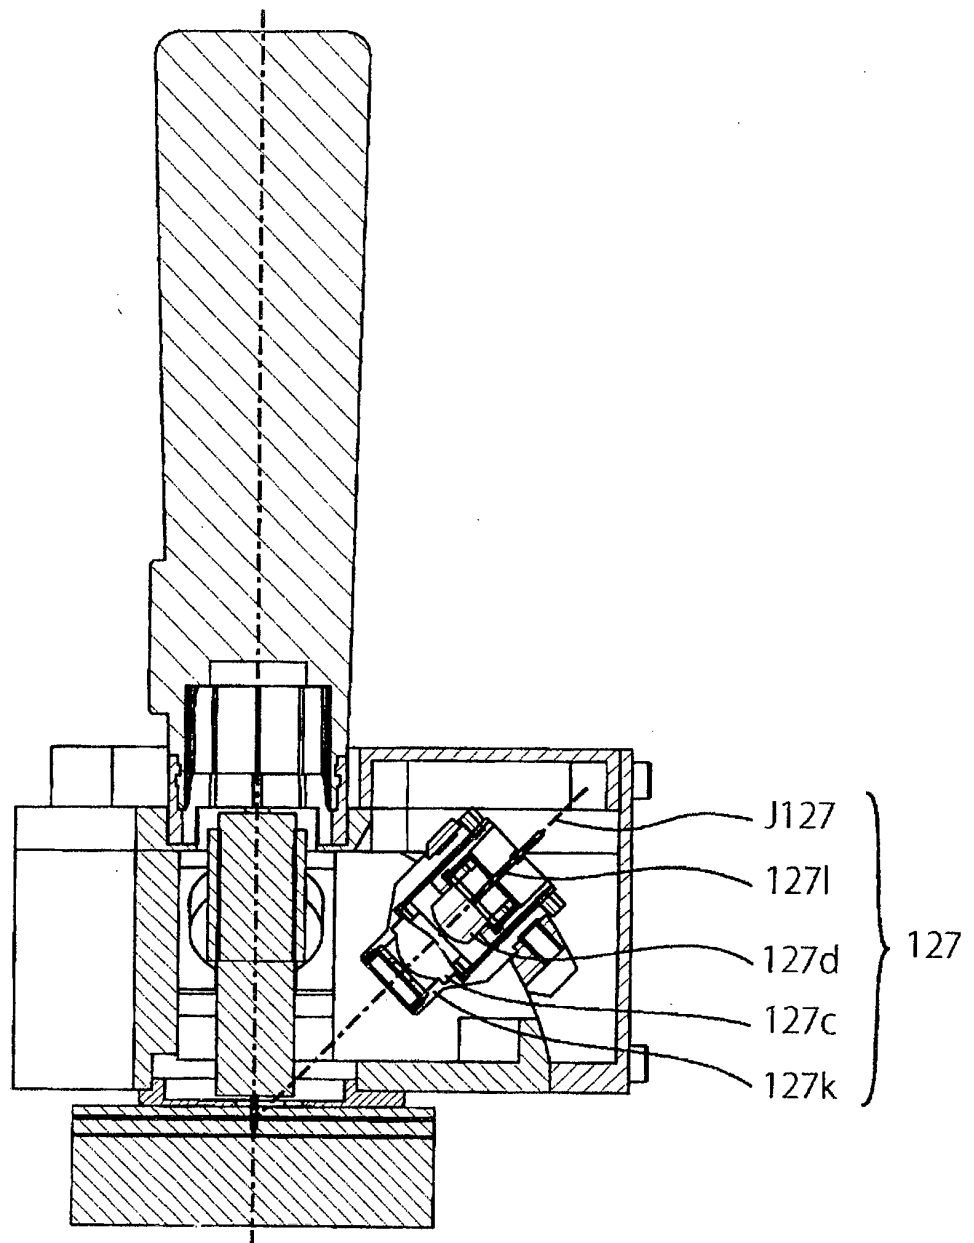


[Fig. 6]

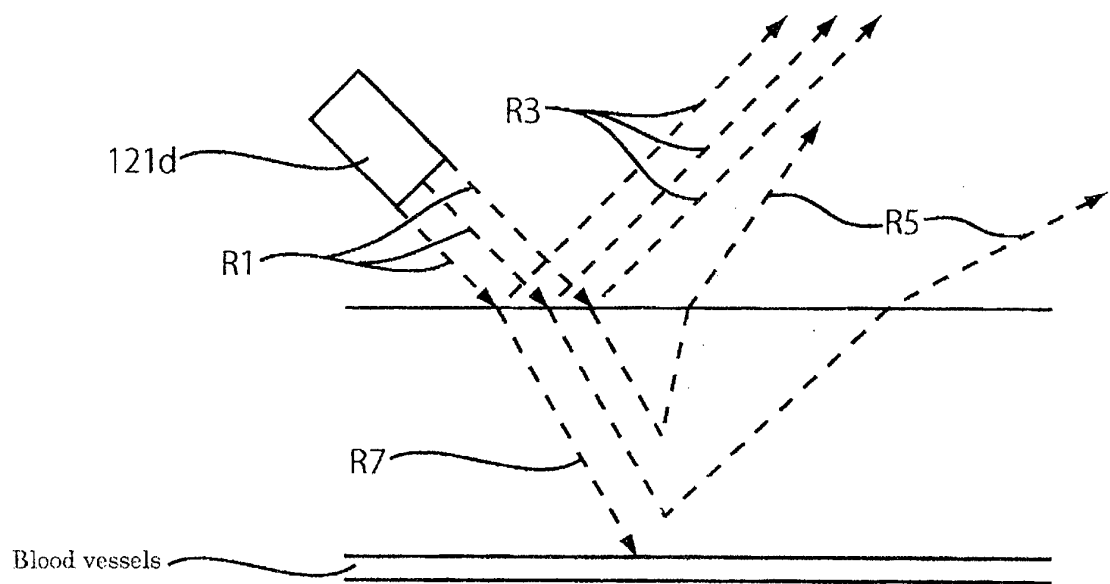


[Fig. 7]

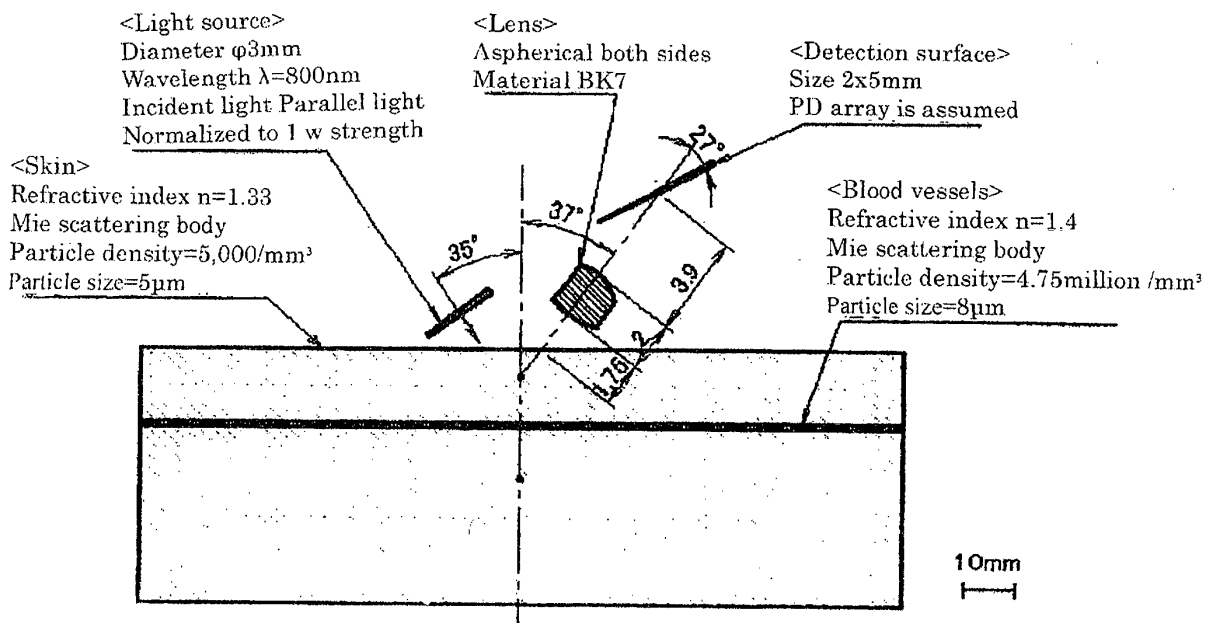


[Fig. 8]

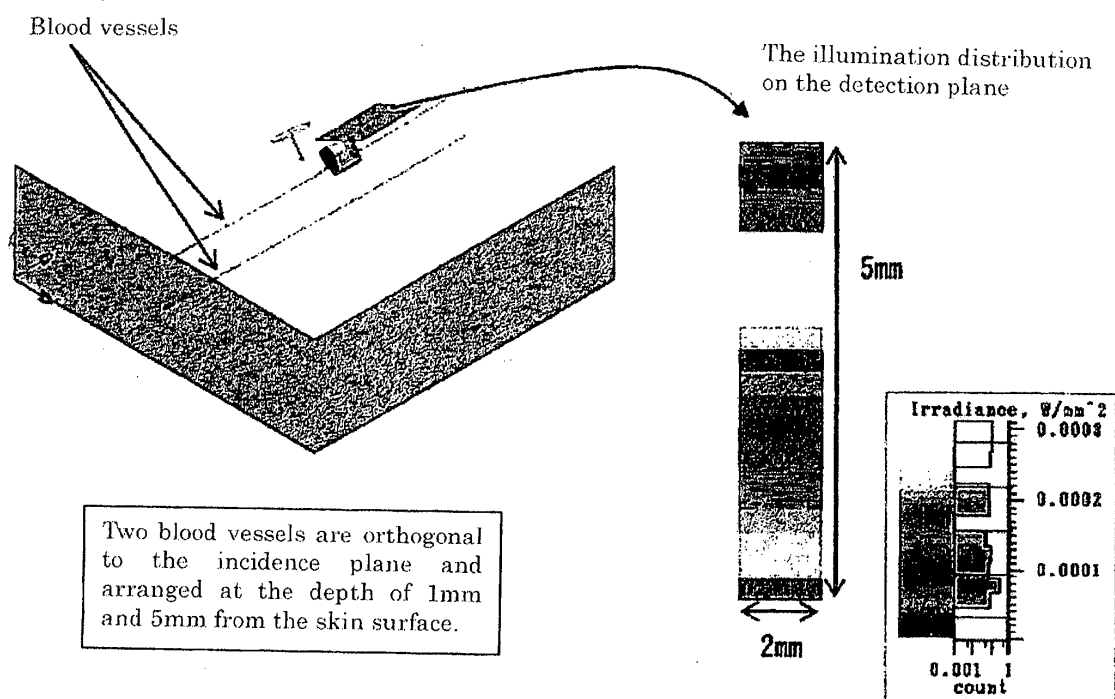

[Fig. 9]

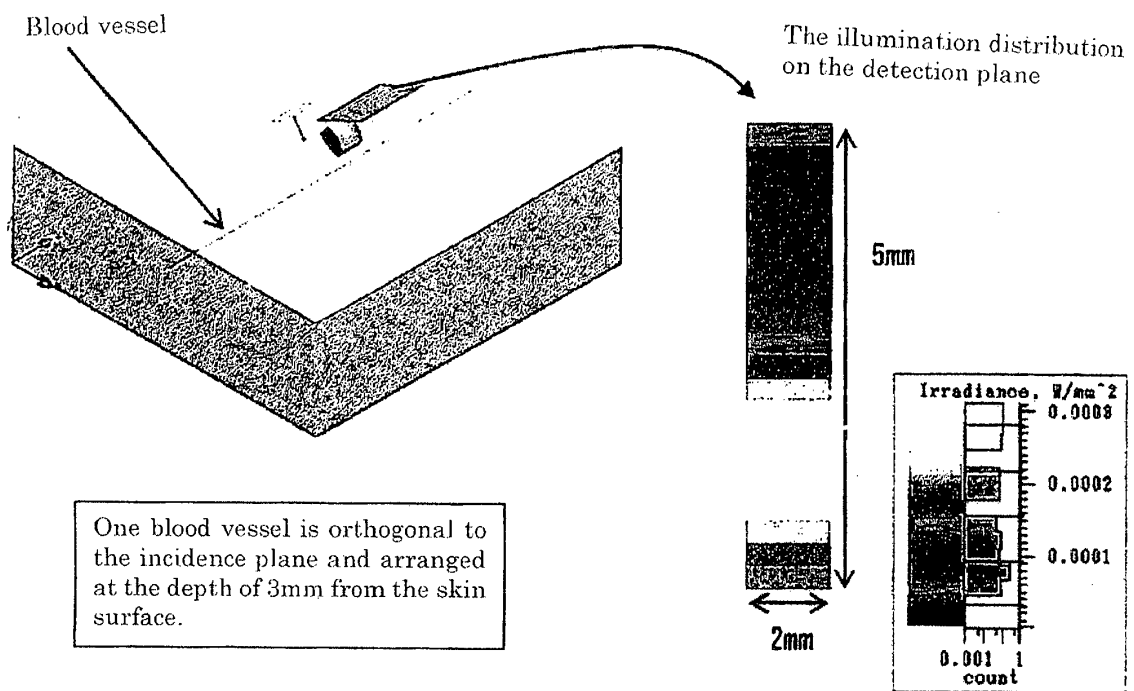


[Fig. 10]

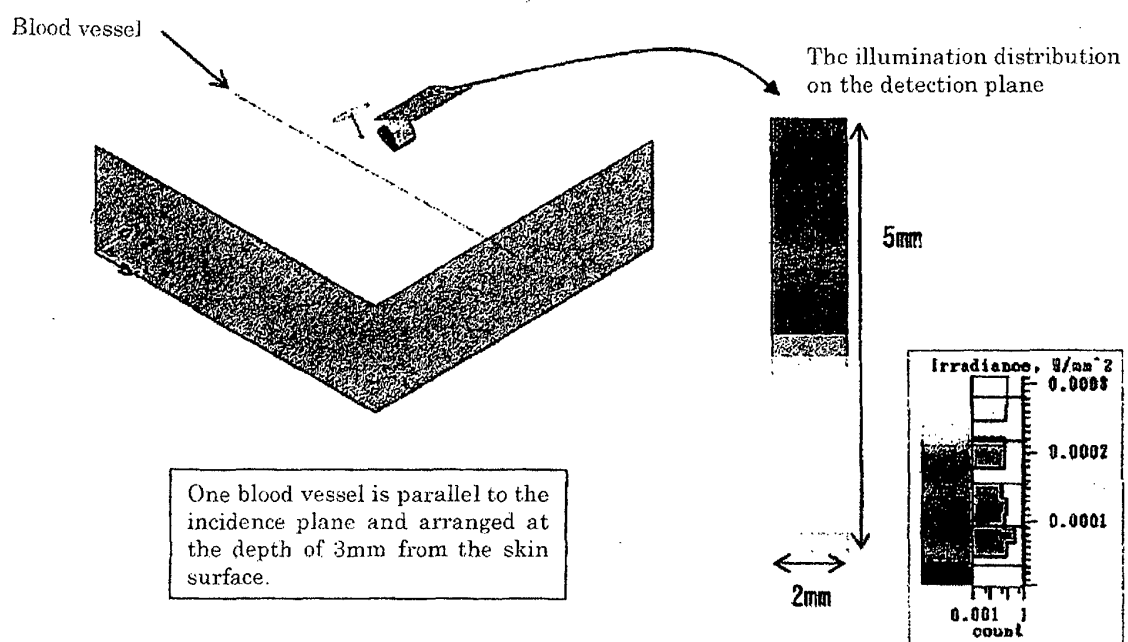


[Fig. 11]

< Prior art >

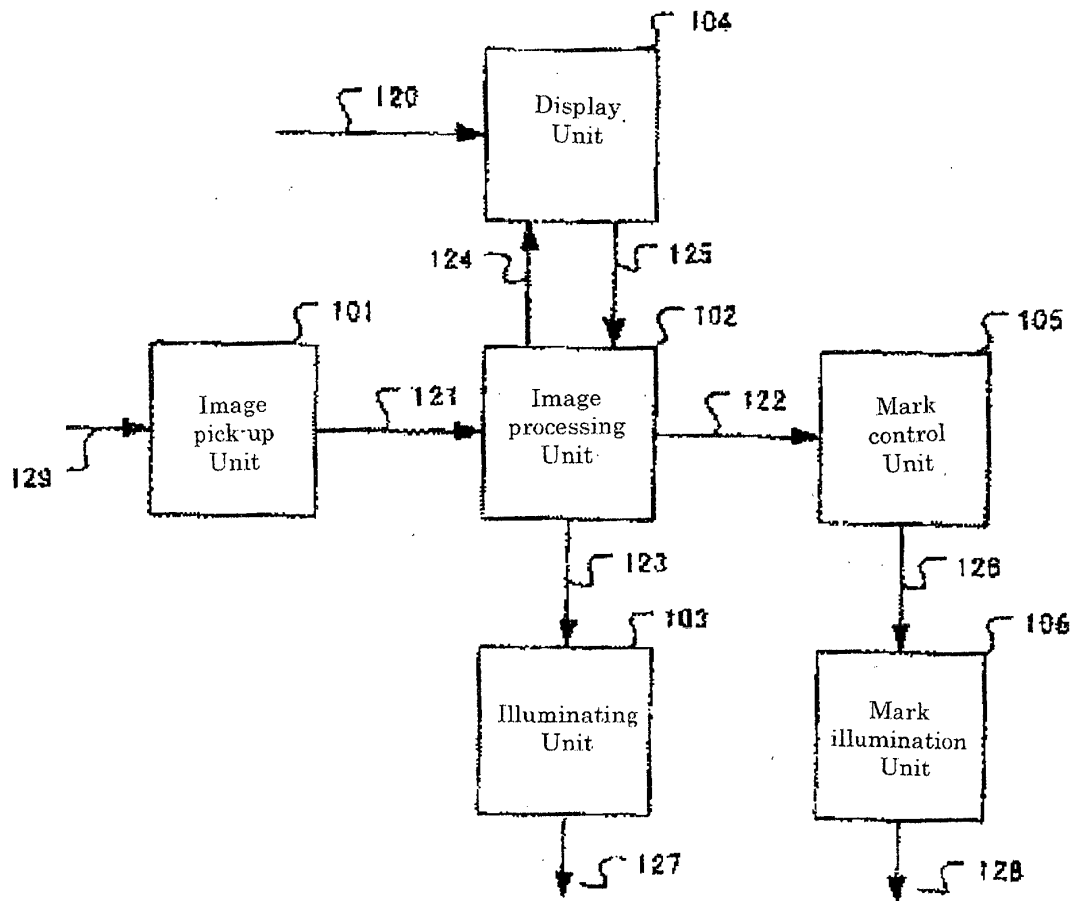

[Fig. 12]

< Prior art >

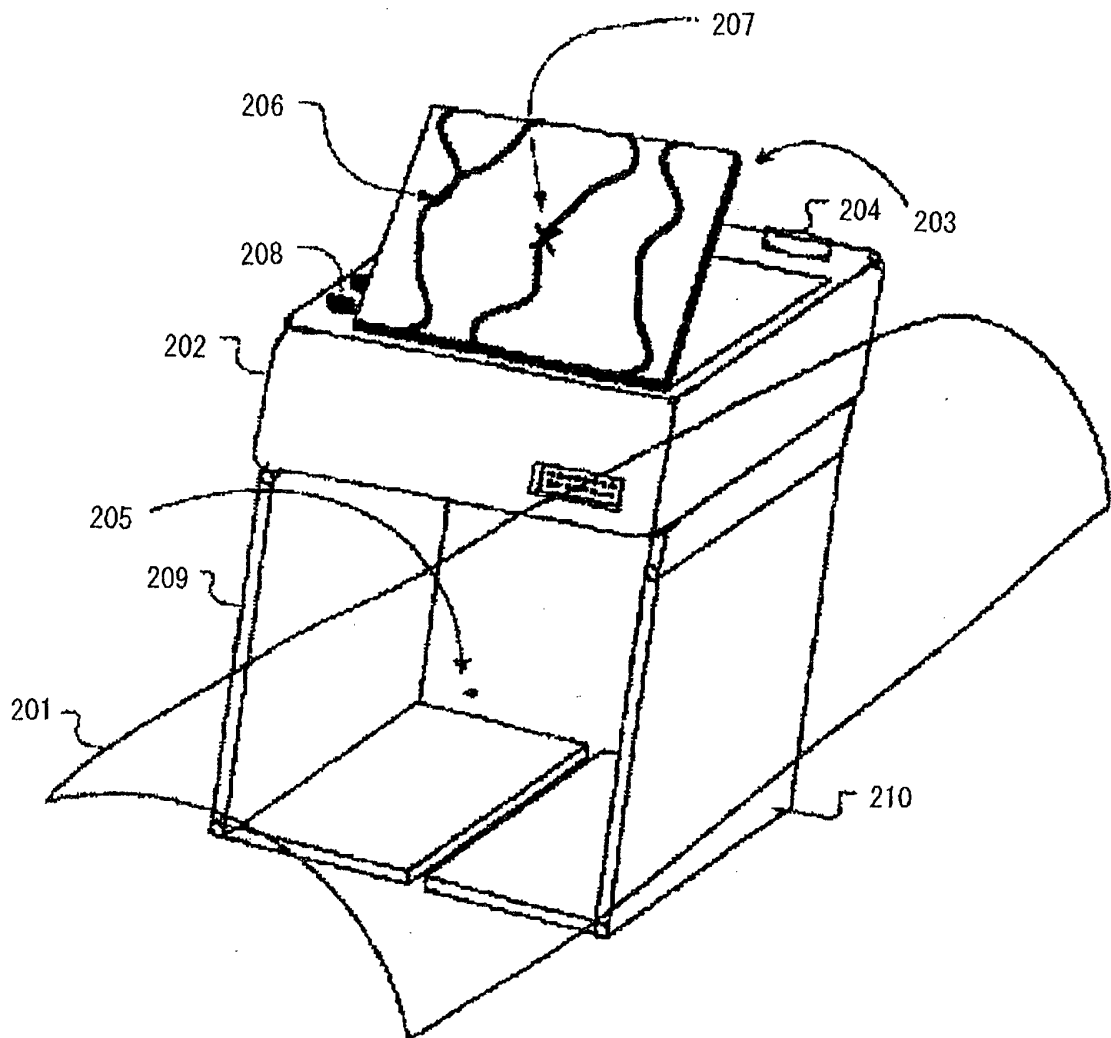

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 2006102110 A [0016]

专利名称(译)	采血装置		
公开(公告)号	EP2554118B1	公开(公告)日	2014-10-08
申请号	EP2011762715	申请日	2011-03-25
[标]申请(专利权)人(译)	尼普洛株式会社 学校法人立命馆		
申请(专利权)人(译)	尼普洛株式会社 立命馆TRUST		
当前申请(专利权)人(译)	尼普洛株式会社 立命馆TRUST		
[标]发明人	KONISHI SATOSHI KOBAYASHI TAIZO YOSHIDA HIROSHI WADA TAKASHI HAGIWARA FUMIHIRO TAKEYAMA NORIHIRO		
发明人	KONISHI, SATOSHI KOBAYASHI, TAIZO YOSHIDA, HIROSHI WADA, TAKASHI HAGIWARA, FUMIHIRO TAKEYAMA, NORIHIRO		
IPC分类号	A61B5/15 A61B5/151 A61M5/00 A61M5/178 A61B5/00 A61B5/153 A61M5/42		
CPC分类号	A61B5/0082 A61B1/0638 A61B5/0059 A61B5/0095 A61B5/1455 A61B5/15003 A61B5/150175 A61B5/150267 A61B5/150389 A61B5/150748 A61B5/153 A61B5/489 A61B5/72 A61B2017/00057 A61M5/427		
优先权	2010073947 2010-03-27 JP		
其他公开文献	EP2554118A1 EP2554118A4		
外部链接	Espacenet		

摘要(译)

通过基于所使用的条件和组件适当地选择近红外光发射单元121的发光单元光轴J121与法线之间的角度 α ，可以更适当地指定血管的位置。照射表面P1的N1，光接收侧透镜123c的光轴J123与照射表面P1的法线N1之间的角度 β ，以及光电二极管阵列123的光接收表面P3与光电二极管阵列123之间的角度 γ 。光接收单元光轴J123。因此，可以基于光电二极管阵列123f中的照明强度的变化来指定从照射表面P1沿法线N1方向的皮下血管深度。因此，可以容易地指定皮下血管的位置。

[Fig. 1]

