

(19)



(11)

EP 2 854 625 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:

04.10.2017 Bulletin 2017/40

(51) Int Cl.:

A61B 5/02 (2006.01) **A61M 5/142** (2006.01)
A61M 5/168 (2006.01) **A61M 5/145** (2006.01)
A61B 5/00 (2006.01)

(21) Application number: **13794119.1**

(86) International application number:

PCT/US2013/042388

(22) Date of filing: **23.05.2013**

(87) International publication number:

WO 2013/177379 (28.11.2013 Gazette 2013/48)

(54) **OCCLUSION DETECTION**

VERSTOPFUNGSERKENNUNG

DÉTECTION D'OCCLUSION

(84) Designated Contracting States:

AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

- **ADAMS, Grant, A.**
Rockland, MA 02370 (US)
- **LACY, Christopher, A.**
Rockland, MA 02370 (US)

(30) Priority: **25.05.2012 US 201261651860 P**

(74) Representative: **Harris, Oliver John Richard**

Novagraaf UK
Centrum
Norwich Research Park
Colney Lane
Norwich NR4 7UG (GB)

(43) Date of publication of application:

08.04.2015 Bulletin 2015/15

(73) Proprietor: **Smiths Medical ASD, Inc.**

Rockland, MA 02370 (US)

(72) Inventors:

- **WANDER, Jacob, A.**
Rockland, MA 02370 (US)

(56) References cited:

JP-A- H06 190 036 **JP-A- 2008 264 140**
US-A- 5 647 853 **US-A1- 2003 205 587**
US-A1- 2003 229 311 **US-A1- 2003 229 311**

EP 2 854 625 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

TECHNICAL FIELD

[0001] This disclosure relates generally to medical devices. More particularly, this disclosure relates to systems for, and methods of, occlusion detection.

BACKGROUND

[0002] In the medical arts, the term "occlusion" typically refers to the blocking or restriction of a normally open passage. In some instances, an occlusion is desired such as when a catheter is pinched off or temporarily collapsed into a closed state intentionally by a practitioner during a medical procedure. In other instances, an unintended occlusion could result in a potentially dangerous situation. For example, in the field of medication delivery devices and systems including so-called "syringe pumps", typically a pre-filled medication syringe is mechanically driven under microprocessor control to deliver a prescribed dose of medication at a controlled rate to a patient through an infusion line fluidly connected to the syringe. Syringe pumps typically include a motor that rotates a leadscrew. The leadscrew in turn activates a plunger driver which forwardly pushes a plunger within a barrel of the syringe. Pushing the plunger forward thus forces the dose of medication outwardly from the syringe, into the infusion line, and to the patient intravenously. Examples of syringe pumps are disclosed in, for example, U.S. Pat. No. 4,978,335 titled "Infusion Pump with Bar Code Input to Computer" and U.S. Pat. Applic. Pub. No. 2005/0096593 titled "Syringe Pump Rapid Occlusion Detection System". As used throughout this disclosure, the term "syringe pump" is intended to generally pertain to any device which acts on a syringe to controllably force fluid outwardly therefrom.

[0003] A further example of a system for occlusion detection is given in U.S. Pat. Applic. Pub. No. 2003/0229311 titled "Syringe Plunger Driver System"

[0004] In such devices, an occlusion might occur when the intended and commanded forward progression of the plunger longitudinally through the syringe barrel is blocked or otherwise impeded, as when for example the infusion line tubing is kinked or otherwise structurally blocked to some degree. If the occlusion is not noticed, the patient likely would not receive the prescribed medication leading to potentially serious consequences.

[0005] Attempts to sense or detect occlusions in medical devices such as syringe pumps have therefore been made. For example, some syringe pumps detect occlusions by use of a pressure sensor that senses a force exerted by the aforementioned syringe thumb-press on the plunger driver. When the force experienced by the pressure sensor exceeds a predetermined threshold force, a processor connected to the pressure sensor generates a signal indicating that an occlusion has possibly occurred or is possibly occurring. Since syringe pumps

are typically capable of accommodating a range of syringe diameters or sizes (e.g., 10 ml through 50 ml capacities) the plunger driver and pressure sensor may likely experience varying occlusion force vectors depending upon which particular size of syringe is being used in the syringe pump, leading to varying accuracy and responsiveness overall in the pump's occlusion sensing system. Since the occlusion force (F) is a function of pressure (P) exerted on the sensor over an area (A) experiencing the pressure (i.e., $P = F / A$) as the area decreases the pressure increases. Typically, therefore, smaller diameter syringes yield smaller sensed forces for given pressures upon occurrences of occlusions. Thus, known occlusion detection systems and methods have not been entirely satisfactory in sensing and signaling occlusions for relatively smaller diameter syringes.

[0006] Consequently, it would be useful and advantageous to provide systems for, and methods of, occlusion detection, particularly when using syringes of relatively small diameters in syringe pumps.

SUMMARY

[0007] This disclosure describes novel and inventive systems for, and methods of, occlusion detection. In accordance with the invention, a system for occlusion detection includes a syringe pump for a syringe containing a medication, wherein the syringe includes a plunger and the syringe pump includes a plunger driver. A bendable element is included within the plunger driver, preferably wherein the bendable element is integrally formed with said plunger driver, and a force sensor is integrally formed with the plunger driver. Upon occurrence of an occlusion, the plunger exerts a force backwardly against the bendable element, thereby deflecting the bendable element into contact with the force sensor to thereby generate a signal indicating the occurrence of the occlusion.

[0008] In another aspect, a system of occlusion detection could include a syringe pump for a syringe containing a medication, wherein the syringe includes a plunger and the syringe pump includes a plunger driver. A pivotable element could be connected to the plunger driver by a link. A force sensor could be integrally formed with the plunger driver. Upon occurrence of an occlusion, the plunger would exert a force backwardly against the pivotable element, thereby deflecting the pivotable element about the link into contact with the force sensor to thereby generate a signal indicating the occurrence of the occlusion.

[0009] In another aspect, a system of occlusion detection could include a syringe pump for a syringe containing a medication, wherein the syringe includes a plunger and the syringe pump includes a plunger driver. A pivotable sliding element having a spring-loaded slot could be connected to the plunger driver by a link residing within the spring-loaded slot. A force sensor could be integrally formed with the plunger driver. Upon occurrence of an occlusion, the plunger would exert a force backwardly

against the pivotable sliding element, thereby deflecting the pivotable sliding element about the link into contact with the force sensor to thereby generate a signal indicating the occurrence of the occlusion.

[0010] In another aspect, a system of occlusion detection could include a syringe pump for a syringe containing a medication, wherein the syringe includes a plunger and the syringe pump includes a plunger driver. A substantially unitary, combination component of a bendable element with a force sensor could be integrally formed with the plunger driver. Upon occurrence of an occlusion, the plunger would exert a force backwardly against the combination component, thereby deflecting the combination component such that a signal is thereby generated to indicate the occurrence of the occlusion.

[0011] In another aspect, a system for occlusion detection could include a syringe pump for a syringe containing a medication, wherein the syringe includes a plunger and the syringe pump includes a plunger driver. A bendable element could be integrally formed with the plunger driver, and a force sensor could also be integrally formed with the plunger driver. Upon occurrence of an occlusion, the plunger would exert a force backwardly against the bendable element, thereby deflecting the bendable element into contact with the force sensor to thereby generate a signal indicating the occurrence of the occlusion. The system for occlusion detection could be characterised in that forces exerted backwardly against the bendable element resulting from occurrences of occlusions, acting on the force sensor, increase in magnitude as syringe sizes decrease due to correspondingly greater moment arms on the bendable element.

[0012] In another aspect, a system of occlusion detection could include a syringe pump for a syringe containing a medication, wherein the syringe includes a plunger and the syringe pump includes a plunger driver. A pivotable element could be connected to the plunger driver by a link. A force sensor could be integrally formed with the plunger driver. Upon occurrence of an occlusion, the plunger would exert a force backwardly against the pivotable element, thereby deflecting the pivotable element about the link into contact with the force sensor to thereby generate a signal indicating the occurrence of the occlusion. The system of occlusion detection could be characterised in that forces exerted backwardly against the pivotable element resulting from occurrences of occlusions, acting on the force sensor, increase in magnitude as syringe sizes decrease due to correspondingly greater moment arms on the pivotable element.

[0013] In another aspect, a system of occlusion detection could include a syringe pump for a syringe containing a medication, wherein the syringe includes a plunger and the syringe pump includes a plunger driver. A pivotable sliding element having a spring-loaded slot could be connected to the plunger driver by a link residing within the spring-loaded slot. A force sensor could be integrally formed with the plunger driver. Upon occurrence of an occlusion, the plunger would exert a force backwardly

against the pivotable sliding element, thereby deflecting the pivotable sliding element about the link into contact with the force sensor to thereby generate a signal indicating the occurrence of the occlusion. The system of occlusion detection could be characterised in that forces exerted backwardly against the pivotable sliding element resulting from occurrences of occlusions, acting on the force sensor, increase in magnitude as syringe sizes decrease due to correspondingly greater moment arms on the pivotable sliding element.

[0014] In another aspect, a system of occlusion detection could include a syringe pump for a syringe containing a medication, wherein the syringe includes a plunger and the syringe pump includes a plunger driver. A substantially unitary, combination component of a bendable element with a force sensor could be integrally formed with the plunger driver. Upon occurrence of an occlusion, the plunger would exert a force backwardly against the combination component, thereby deflecting the combination component such that a signal is thereby generated to indicate the occurrence of the occlusion. The system for occlusion detection could be characterised in that forces exerted backwardly against the combination component resulting from occurrences of occlusions, acting on the combination component, increase in magnitude as syringe sizes decrease due to correspondingly greater moment arms on the combination component.

[0015] In accordance with the invention, a method of occlusion detection includes providing a syringe pump for a syringe containing a medication, wherein the syringe includes a plunger and the syringe pump includes (i) a plunger driver, (ii) an element within the plunger driver, the element being selected from a group consisting of a bendable element, and a pivotable sliding element, and (iii) a force sensor integrally formed with the plunger driver. Upon occurrence of an occlusion, the plunger exerts a force backwardly against the element, thereby deflecting the element into contact with the force sensor to thereby generate a signal indicating the occurrence of the occlusion. The medication is administered to an infusion line by way of the syringe pump, and the signal generated by the sensor is sent to medical staff upon the occurrence of the occlusion.

[0016] In another aspect, a method of occlusion detection could include providing a syringe pump for a syringe containing a medication, wherein the syringe includes a plunger and the syringe pump includes (i) a plunger driver and (ii) a substantially unitary, combination component of a bendable element with a force sensor, with the plunger driver. Upon occurrence of an occlusion, the plunger would exert a force backwardly against the combination component, thereby deflecting the combination component such that a signal is thereby generated to indicate the occurrence of the occlusion. The medication could be administered to a patient by way of the syringe pump, and the signal generated by the sensor could be sent to medical staff upon the occurrence of the occlusion.

BRIEF DESCRIPTION OF THE DRAWINGS

[0017] Systems for, and methods of, occlusion detection are illustrated by way of example and not limitation in the figures of the accompanying drawings in which:

Figure 1 is a schematic diagram of a system for occlusion detection, in use with a relatively large medication syringe.

Figure 1A is schematic diagram of the system shown in Figure 1, in use with a relatively small medication syringe.

Figure 2 is a schematic diagram of an alternative embodiment of a system for occlusion detection, in use with a relatively large medication syringe.

Figure 2A is schematic diagram of the system shown in Figure 2, in use with a relatively small medication syringe.

Figure 3 is a schematic diagram of an alternative embodiment of a system for occlusion detection, in use with a relatively large medication syringe.

Figure 3A is schematic diagram of the system shown in Figure 3, in use with a relatively small medication syringe.

Figure 4 is a schematic block diagram of a method for occlusion detection.

DETAILED DESCRIPTION

[0018] Occlusion detection systems and methods, that are described in greater detail by way of examples herein, make novel and inventive use of decreasing syringe diameters or sizes in syringe pumps to compensate for the aforementioned relatively smaller sensed occlusion forces that are otherwise generated by smaller diameter syringes. Such compensation advantageously results in more constant occlusion forces sensed for given pressures across varying ranges of syringe diameters or sizes used in syringe pumps; and better resolution and sensitivity in occlusion detection is achieved for smaller syringes that are used in, for example, neonatal care units when accuracy and precision in medication delivery are of paramount importance.

[0019] Generally, the aforementioned compensation is achieved by way of an element with a plunger driver of a syringe pump that is mechanically linked to a plunger of a syringe in the pump. The element is capable of bending, pivoting, or rotating about a point, upon displacement by an occlusion force acting backwardly on it as transmitted by the plunger. The element then bends, pivots, or rotates about the point, and thereby applies a force to a force sensor. The force sensor then outputs a signal indicative of an occurrence of an occlusion. As syringe diameter decreases, such as when, e.g., a 30 ml syringe is replaced in the pump by a 20 ml syringe, an occlusion force from the plunger of the smaller syringe acts on the element more distantly from the point about which the element bends, pivots, or rotates; and thus a relatively

larger moment arm results with a correspondingly higher force experienced by the force sensor.

[0020] Referring now to Figure 1, therein illustrated generally is an example of an embodiment of a system for occlusion detection 10. System 10 includes a syringe pump 100 for a syringe S having a plunger P. Syringe S is of a size or diameter (N) (e.g., a 30 ml syringe) that contains a medication to be delivered to a patient from pump 100 acting on syringe S by way of a plunger driver 110. Driver 110 includes an integrally formed bendable element 120. A force sensor 130 is also integrally formed with driver 110. As shown in Figure 1, upon occurrence of an occlusion plunger P would exert a force backwardly against bendable element 120, thereby deflecting element 120 (indicated by phantom line F) into contact with force sensor 130 to thereby generate a signal indicating the occurrence of the occlusion. With reference now to Figure 1A, it is to be appreciated and understood that upon occurrence of an occlusion with use of a syringe S of a size, or diameter, (N-) (e.g., a 20 ml syringe) plunger P would exert a force backwardly against bendable element 120, but at a greater distance downwardly along element 120 compared to Figure 1. Thereby, in Figure 1A, element 120 would be deflected (indicated by phantom line F(+)) with a greater moment arm and thus into more forceful contact with force sensor 130, compared to such contact from a relatively shorter moment arm shown in Figure 1 from the larger syringe size (N).

[0021] Another embodiment of an example of a system for occlusion detection 20 is illustrated generally in Figure 2. System 20 includes a syringe pump 200 for a syringe S having a plunger P. Syringe S is of a size or diameter (N) (e.g., a 30 ml syringe) that contains a medication to be delivered to a patient from pump 200 acting on syringe S by way of a plunger driver 210. A pivotable element 220 is connected to driver 210 by a link 225 (e.g., a pin through a corresponding hole in element 220). A force sensor 230 is integrally formed with driver 210. As shown in Figure 1, upon occurrence of an occlusion plunger P would exert a force backwardly against pivotable element 220, thereby deflecting element 220 about link 225 (indicated by phantom line F) into contact with force sensor 230 to thereby generate a signal indicating the occurrence of the occlusion. With reference now to Figure 2A, it is to be appreciated and understood that upon occurrence of an occlusion with use of a syringe S of a size or diameter (N-) (e.g., a 20 ml syringe) plunger P would exert a force backwardly against pivotable element 220, but at a greater distance downwardly along element 220 compared to Figure 2. Thereby, in Figure 2A, element 220 would be deflected (indicated by phantom line F(+)) with a greater moment arm and thus into more forceful contact with force sensor 230, compared to such contact from a relatively shorter moment arm shown in Figure 2 from the larger syringe size (N).

[0022] Another embodiment of an example of a system for occlusion detection 30 is illustrated generally in Figure 3. System 30 includes a syringe pump 300 for a syringe

S having a plunger P. Syringe S is of a size or diameter (N) (e.g., a 30 ml syringe) that contains a medication to be delivered to a patient from pump 300 acting on syringe S by way of a plunger driver 310. A pivotable sliding element 320 is connected to driver 310 by a link 325 (e.g., a pin in a spring-loaded slot 327 in element 320; details of the spring-loaded slot 327 have been omitted for clarity of the drawing). A force sensor 330 is integrally formed with driver 310. As shown in Figure 3, upon occurrence of an occlusion plunger P would exert a force backwardly against pivotable sliding element 320, thereby deflecting element 320 about link 325 (indicated by phantom line F) into contact with force sensor 330 to thereby generate a signal indicating the occurrence of the occlusion. With reference now to Figure 3A, it is to be appreciated and understood that upon occurrence of an occlusion with use of a syringe S of a size or diameter (N-) (e.g., a 20 ml syringe) plunger P would exert a force backwardly against pivotable sliding element 320, but at a greater distance downwardly along element 320 compared to Figure 3. Thereby, in Figure 3A, element 320 would be deflected (indicated by phantom line F(+)) with a greater moment arm and thus into more forceful contact with force sensor 330, compared to such contact from a relatively shorter moment arm shown in Figure 3 from the larger syringe size (N).

[0023] Referring now to Figure 4, therein illustrated generally is an example of a method for occlusion detection 400 in, e.g., a clinical setting having medical staff M. In this example, medical staff M would load a syringe S of a size (N) containing a selected medication for a patient into a syringe pump (e.g., the aforementioned pumps 100, 200, or 300). As described by example above, syringe S would include a plunger P. The syringe pump would include a plunger driver such as, e.g., the aforementioned drivers 110, 210, and 310. An element (e.g., the aforementioned bendable element 120, pivotable element 220, or pivotable sliding element 320) would be included with the plunger driver. A force sensor such as, e.g., the aforementioned sensors 130, 230, or 330, would be integrally formed with the plunger driver. The syringe pump would administer the medication to the patient (typically, e.g., through an intravenous line from the syringe to the patient). Upon occurrence of an occlusion, the plunger would exert a force backwardly against the element, thereby deflecting the element into contact with the force sensor. The force sensor would responsively generate a signal that would be sent to the medical staff alerting them to the occurrence of the occlusion as indicated by symbol 410 in the drawing.

[0024] Although not illustrated herein, another embodiment of an example of a system for occlusion detection could utilize a substantially unitary, combination component of a bendable element with a force sensor. I.e., the force sensor would respond to a bending moment by being incorporated with or into the bendable element itself, instead of separate bendable element and force sensor components as shown in, e.g., the various examples of

Figures 1, 2, and 3. In embodiments that have a substantially unitary, combination component of a bendable element with a force sensor - instead of separate components - a smaller syringe in the pump would, upon occurrence of an occlusion, apply a force closer to a free end of the combination component which would again, in turn, advantageously result in a greater moment arm and correspondingly higher force sensor output.

[0025] Regardless of particular components or modes of action, it is to be appreciated and understood that systems for, and methods of, occlusion detection such as have been described by example or otherwise contemplated herein could detect occlusions to enhance the safety and accuracy of delivery of medication from syringes to patients. As aforementioned, novel and inventive use is made of decreasing syringe diameters or sizes to compensate for the aforementioned otherwise relatively smaller sensed occlusion forces generated by smaller diameter syringes. That is, what heretofore had been a disadvantage in occlusion detection - decreasing syringe diameters or sizes - is now used to technical advantage as aforescribed, which may, for example, quite advantageously permit faster occlusion detection in small syringes.

[0026] It is also to be particularly appreciated and understood that any embodiment of systems for, and methods of, occlusion detection that have been described by example or otherwise contemplated herein could advantageously be used, or function in association, with principles of determining discrete force values. Such discrete force values could, in turn, determine whether relationships between them depart from expected relationships, etc., as disclosed in the aforesaid U.S. Pat. Applic. Pub. No. 2005/0096593. While systems for, and methods of, occlusion detection have been particularly shown and described with reference to the accompanying figures and specification, it should be understood however that other modifications thereto are of course possible; and all of them are intended to be within the scope of novel and inventive systems and methods described herein. Thus, configurations and designs of various features could be modified or altered depending upon particular embodiments.

[0027] Additionally, dimensioning and scaling of the drawings herein have been chosen to clearly show details of example embodiments. Thus, in some embodiments it is possible that spacing between various features might be visually imperceptible - e.g., the bendable, pivotable, and pivotable sliding elements; and the plunger driver. In any event, dimensioning and scaling could vary significantly across various embodiments of occlusion detection systems and methods.

[0028] It should also be appreciated that types, components, dimensions, fabrication processes, and other particulars and parameters of aforescribed example embodiments may be substituted for others as desired, or that accessories may be added thereto. For example, in one embodiment, the force sensor could comprise a

commercially available Honeywell 1865 Pressure Transducer.

[0029] It is also to be understood in general that any suitable alternatives may be employed to provide novel and inventive systems for, and methods of, occlusion detection described by example or otherwise contemplated herein. As such, although the bendable elements, force sensors, and combination components (collectively, regardless of particular constructions, "force components") described by example herein have been further described as being "integrally formed" with plunger drivers, it is to be appreciated and understood that this "integrally formed" terminology broadly includes constructions wherein (i) the force components are formed essentially as one with the plunger driver and also wherein (ii) the force components are physically separate from but attached to, connected to, or otherwise contained within, the plunger driver.

[0030] Lastly, compositions, sizes, and strengths of various aforementioned components of systems for, and methods of, occlusion detection described by example or otherwise contemplated herein are all a matter of design choice depending upon intended uses thereof.

[0031] Accordingly, these and other various changes or modifications in form and detail may also be made, without departing from the scope of systems for, and methods of, occlusion detection that may be defined by the appended claims.

Claims

1. A system for occlusion detection, comprising:

a syringe pump (100, 200, 300) for a syringe (S) containing a medication, wherein the syringe (S) includes a plunger (P) and said syringe pump (100, 200, 300) includes a plunger driver (110, 210, 310);

an element (120, 220, 320) within said plunger driver (110, 210, 310), said element (120, 220, 320) being selected from a group consisting of a bendable element (120) and a pivotable sliding element (320); and

a force sensor (130, 230, 330) integrally formed with said plunger driver (110, 210, 310), wherein upon occurrence of an occlusion, the plunger exerts a force backwardly against said element (120, 220, 320), thereby deflecting said element (120, 220, 320) into contact with said force sensor (130, 230, 330) to thereby generate a signal indicating the occurrence of the occlusion.

2. The system for occlusion detection according to claim 1, wherein the element (120, 220, 320) is a bendable element (120), and the bendable element (120) is integrally formed with said plunger driver (110, 210, 310).

3. The system for occlusion detection according to claim 1, wherein the element (120, 220, 320) is a pivotable sliding element (320), the pivotable sliding element (320) includes a spring-loaded slot (327), the pivotable sliding element (320) is connected to said plunger driver (310) by a link (325) residing within said spring-loaded slot (327), and the pivotable sliding element (320) is deflected about said link (325) into contact with said force sensor (330).

4. The system for occlusion detection of any one of the preceding claims **characterized in that** forces exerted backwardly against said element (120, 220, 320) resulting from occurrences of occlusions, acting on said force sensor (130, 230, 330), increase in magnitude as syringe sizes decrease due to correspondingly greater moment arms on said element (120, 220, 320).

5. The system for occlusion detection according to claim 1, wherein the element (120, 220, 320) is a bendable element (120) and the bendable element (120) and the force sensor (130) are combined in a substantially unitary, combination component, being integrally formed with said plunger driver (110), wherein upon occurrence of an occlusion, the plunger (P) exerts a force backwardly against said combination component, thereby deflecting said combination component such that a signal is thereby generated to indicate the occurrence of the occlusion.

6. The system for occlusion detection of claim 5, wherein in that forces exerted backwardly against said combination component resulting from occurrences of occlusions, acting on said combination component, increase in magnitude as syringe sizes decrease due to correspondingly greater moment arms on said combination component.

7. A method of occlusion detection, comprising:

providing a syringe pump (100, 200, 300) for a syringe (S) containing a medication, wherein the syringe includes a plunger (P) and said syringe pump (100, 200, 300) includes (i) a plunger driver (110, 210, 310), (ii) an element (120, 220, 320) within said plunger driver (110, 210, 310), said element (120, 220, 320) being selected from a group consisting of a bendable element (120) and a pivotable sliding element (320), and (iii) a force sensor (130, 230, 330) integrally formed with said plunger driver (110, 210, 310), wherein upon occurrence of an occlusion, the plunger (P) exerts a force backwardly against said element (120, 220, 320), thereby deflecting said element (120, 220, 320) into contact with said force sensor (130, 230, 330) to thereby generate a signal indicating the occurrence of the

occlusion;
 administering the medication to an infusion line
 by way of said syringe pump (100, 200, 300); and
 sending said signal generated by said sensor
 (130, 230, 330) to medical staff, upon an occur-
 rence of an occlusion.

8. The method of occlusion detection according to
 claim 7, wherein the element (120, 220, 330) is a
 bendable element (120) and the bendable element
 (120) and the force sensor (130) are combined in a
 substantially unitary, combination component, being
 integrally formed with said plunger driver (110, 210,
 310), wherein upon occurrence of an occlusion, the
 plunger (P) exerts a force backwardly against said
 combination component, thereby deflecting said
 combination component such that a signal is thereby
 generated to indicate the occurrence of the occlu-
 sion;
 administering the medication to an infusion line by
 way of said syringe pump (100, 200, 300); and
 sending said signal generated by said combination
 component to medical staff, upon an occurrence of
 an occlusion.

Patentansprüche

1. System zur Verstopfungserkennung, aufweisend:

eine Spritzenpumpe (100, 200, 300) für eine
 Spritze (S), die ein Medikament enthält, wobei
 die Spritze (S) einen Kolben (P) aufweist und
 die Spritzenpumpe (100, 200, 300) einen Kol-
 benantrieb (110, 210, 310) aufweist;
 ein Element (120, 220, 320) innerhalb des Kol-
 benantriebs (110, 210, 310), wobei das Element
 ausgewählt ist aus einer Gruppe bestehend aus
 einem biegsamen Element (120) und einem
 schwenkbar gleitenden Element (320); und
 einen Kraftaufnehmer (130, 230, 330), der ein-
 stückig mit dem Kolbenantrieb (110, 210, 310)
 ausgebildet ist, wobei bei Auftreten einer Ver-
 stopfung der Kolben eine rückwärts gerichtete
 Kraft gegen das Element (120, 220, 320) ausübt,
 wobei das Element (120, 220, 320) bis zum Kon-
 takt mit dem Kraftaufnehmer (130, 230, 330)
 ausgelenkt wird, um dadurch ein Signal zu er-
 zeugen, das das Auftreten der Verstopfung an-
 gibt.

2. System zur Verstopfungserkennung nach Anspruch
 1, wobei das Element (120, 220, 320) ein biegsames
 Element (120) ist und das biegsame Element (120)
 einstückig mit dem Kolbenantrieb (110, 210, 310)
 ausgebildet ist.

3. System zur Verstopfungserkennung nach Anspruch

1, wobei das Element (120, 220, 320) ein schwenk-
 bar gleitendes Element (320) ist, wobei das
 schwenkbar gleitende Element (320) einen federbe-
 lasteten Schlitz (327) aufweist, wobei das schwenk-
 bar gleitende Element (320) durch ein innerhalb des
 federbelasteten Schlitzes (327) angeordnetes Ge-
 lenk (325) mit dem Kolbenantrieb (310) verbunden
 ist und das schwenkbar gleitende Element (320) um
 das Gelenk (325) in Kontakt mit dem Kraftaufnehmer
 (330) ausgelenkt wird.

4. System zur Verstopfungserkennung nach einem der
 vorhergehenden Ansprüche, **dadurch gekenn-
 zeichnet, dass** Kräfte, die als Folge von Auftreten
 von Verstopfungen rückwärts gerichtet gegen das
 Element (120, 220, 320) ausgeübt werden, auf dem
 Kraftaufnehmer (130, 230, 330) wirken, an Größe
 zunehmen, wenn die Spritzengrößen aufgrund von
 entsprechend größeren Momentarmen auf dem Ele-
 ment (120, 220, 320) abnehmen.

5. System zur Verstopfungserkennung nach Anspruch
 1, wobei das Element (120, 220, 320) ein biegsames
 Element (120) ist und das biegsame Element (120)
 und der Kraftaufnehmer (130) in einer im Wesentli-
 chen einheitlichen Kombinationskomponente kom-
 biniert sind, die einstückig mit dem Kolbenantrieb
 (110) ausgebildet ist, wobei der Kolben (P) bei Auf-
 treten einer Verstopfung eine rückwärts gerichtete
 Kraft gegen die Kombinationskomponente ausübt
 und dabei die Kombinationskomponente so aus-
 lenkt, dass ein Signal erzeugt wird, das das Auftreten
 der Verstopfung anzeigt.

6. System zur Verstopfungserkennung nach Anspruch
 5, wobei Kräfte, die als Folge von Auftreten von Ver-
 stopfungen rückwärts gerichtet gegen die Kombina-
 tionskomponente ausgeübt werden, auf die Kombi-
 nationskomponente wirken, an Größe zunehmen,
 wenn die Spritzengrößen aufgrund von entspre-
 chend größeren Momentarmen auf der Kombinati-
 onskomponente abnehmen.

7. Verfahren zur Verstopfungserkennung, umfassend:

Bereitstellen einer Spritzenpumpe (100, 200,
 300) für eine Spritze (S), die ein Medikament
 enthält, wobei die Spritze einen Kolben (P) auf-
 weist und die Spritzenpumpe (100, 200, 300) (i)
 einen Kolbenantrieb (110, 210, 310) aufweist,
 (ii) ein Element (120, 220, 320) innerhalb des
 Kolbenantriebs (110, 210, 310) aufweist, wobei
 das Element (120, 220, 320) ausgewählt ist aus
 einer Gruppe bestehend aus einem biegsamen
 Element (120) und einem schwenkbar gleiten-
 den Element (320), und (iii) einen Kraftaufneh-
 mer (130, 230, 330) aufweist, der einstückig mit
 dem Kolbenantrieb (110, 210, 310) ausgebildet

ist, wobei bei Auftreten einer Verstopfung der Kolben (P) eine rückwärts gerichtete Kraft gegen das Element (120, 220, 320) ausübt, wobei das Element (120, 220, 320) in Kontakt mit dem Kraftaufnehmer (130, 230, 330) ausgelenkt wird, um dadurch ein Signal zu erzeugen, das das Auftreten der Verstopfung angibt; Verabreichen des Medikaments an eine Infusionsleitung mithilfe der Spritzenpumpe (100, 200, 300); und Senden des vom Kraftaufnehmer (130, 230, 330) erzeugten Signals an medizinisches Personal nach Auftreten einer Verstopfung.

8. Verfahren zur Verstopfungserkennung nach Anspruch 7, wobei das Element (120, 220, 320) ein biegsames Element (120) ist und das biegsame Element (120) und der Kraftaufnehmer (130) in einer im Wesentlichen einheitlichen Kombinationskomponente kombiniert sind, die einstückig mit dem Kolbenantrieb (110, 210, 310) ausgebildet ist, wobei der Kolben (P) bei Auftreten einer Verstopfung eine rückwärts gerichtete Kraft gegen die Kombinationskomponente ausübt und dabei die Kombinationskomponente so auslenkt, dass ein Signal erzeugt wird, das das Auftreten der Verstopfung anzeigt; Verabreichen des Medikaments an eine Infusionsleitung mithilfe der Spritzenpumpe (100, 200, 300); und Senden des von der Kombinationskomponente erzeugten Signals an medizinisches Personal nach Auftreten einer Verstopfung.

Revendications

1. Système de détection d'une occlusion, comprenant :

une pompe à seringue (100, 200, 300) pour une seringue (S) contenant un médicament, dans lequel la seringue (S) comprend un piston (P) et ladite pompe à seringue (100, 200, 300) comprend un dispositif d'entraînement de piston (110, 210, 310) ;
un élément (120, 220, 320) à l'intérieur dudit dispositif d'entraînement de piston (110, 210, 310), ledit élément (120, 220, 320) étant sélectionné parmi un groupe constitué d'un élément pliable (120) et d'un élément coulissant pivotant (320) ;
et
un détecteur de force (130, 230, 330) formé d'un seul tenant avec ledit dispositif d'entraînement de piston (110, 210, 310), dans lequel, quand une occlusion se manifeste, le piston exerce une force vers l'arrière contre ledit élément (120, 220, 320), faisant ainsi dévier ledit élément (120, 220, 320) en contact avec ledit détecteur de force (130, 230, 330) pour générer ainsi un signal

indiquant la manifestation d'une occlusion.

2. Système de détection d'une occlusion selon la revendication 1, dans lequel l'élément (120, 220, 320) est un élément pliable (120) et l'élément pliable (120) est formé d'un seul tenant avec ledit dispositif d'entraînement de piston (110, 210, 310).
3. Système de détection d'une occlusion selon la revendication 1, dans lequel l'élément (120, 220, 320) est un élément coulissant pivotant (320), l'élément coulissant pivotant (320) comprend une fente à ressort (327), l'élément coulissant pivotant (320) est relié au dit dispositif d'entraînement de piston (310) par une liaison (325) résidant à l'intérieur de ladite fente à ressort (327) et l'élément coulissant pivotant ((320) est dévié autour de ladite liaison (325) en contact avec ledit détecteur de force (330).
4. Système de détection d'une occlusion selon l'une quelconque des revendications précédentes, **caractérisé en ce que** l'amplitude des forces exercées vers l'arrière contre ledit élément (120, 220, 320), résultant de la manifestation des occlusions, agissant sur ledit détecteur de force (130, 230, 330), augmente au fur et à mesure que la taille de la seringue diminue en raison de bras avec un moment plus important de manière correspondante sur ledit élément (120, 220, 320) .
5. Système de détection d'une occlusion selon la revendication 1, dans lequel l'élément (120, 220, 320) est un élément pliable (120) et l'élément pliable (120) et le détecteur de force (130) sont combinés de façon essentiellement unitaire, le composant de combinaison étant formé d'un seul tenant avec ledit dispositif d'entraînement de piston (110), dans lequel, quand une occlusion se manifeste, le piston (P) exerce une force vers l'arrière contre ledit composant de combinaison, déviant ainsi ledit composant de combinaison de sorte qu'un signal est généré pour indiquer la manifestation de l'occlusion.
6. Système de détection d'une occlusion selon la revendication 5, dans lequel l'amplitude des forces exercées vers l'arrière contre ledit composant de combinaison résultant des manifestations d'occlusions, agissant sur ledit composant de combinaison, augmente au fur et à mesure que la taille de la seringue diminue en raison des bras avec un moment plus important de manière correspondante sur ledit composant de combinaison.
7. Procédé de détection d'une occlusion comprenant les étapes consistant à :
- fournir une pompe à seringue (100, 200, 300) pour une seringue (S) contenant un médica-

ment, dans lequel la seringue comprend un piston (P) et ladite pompe à seringue (100, 200, 300) comprend (i) un dispositif d'entraînement de piston (110, 210, 310), (ii) un élément (120, 220, 320) à l'intérieur dudit dispositif d'entraînement de piston (110, 210, 310), ledit élément (120, 220, 320) étant sélectionné parmi un groupe constitué d'un élément pliable (120) et d'un élément coulissant pivotant (320), et (iii) un détecteur de force (130, 230, 330) formé d'un seul tenant avec ledit dispositif d'entraînement de piston (110, 210, 310), dans lequel, quand une occlusion se manifeste, le piston exerce une force vers l'arrière contre ledit élément (120, 220, 320), faisant ainsi dévier ledit élément (120, 220, 320) en contact avec ledit détecteur de force (130, 230, 330) pour générer ainsi un signal indiquant la manifestation d'une occlusion ; administrer le médicament à une ligne de perfusion à l'aide de ladite pompe à seringue (100, 200, 300) ; et envoyer ledit signal généré par ledit détecteur (130, 230, 330) au personnel médical, dès qu'une occlusion se manifeste.

8. Procédé de détection d'une occlusion selon la revendication 7, dans lequel l'élément (120, 220, 330) est un élément pliable (120) et l'élément pliable (120) et le détecteur de force (130) sont combinés d'une manière essentiellement unitaire, le composant de combinaison étant formé d'un seul tenant avec ledit dispositif d'entraînement de piston (110, 210, 310), dans lequel, quand une occlusion se manifeste, le piston (P) exerce une force vers l'arrière contre ledit composant de combinaison, déviant ainsi ledit composant de combinaison de sorte qu'un signal soit généré pour indiquer la manifestation de l'occlusion ; administrer le médicament à une ligne de perfusion à l'aide d'une pompe à seringue (100, 200, 300) ; et envoyer ledit signal généré par ledit composant de combinaison au personnel médical, dès qu'une occlusion se manifeste.

Fig. 1

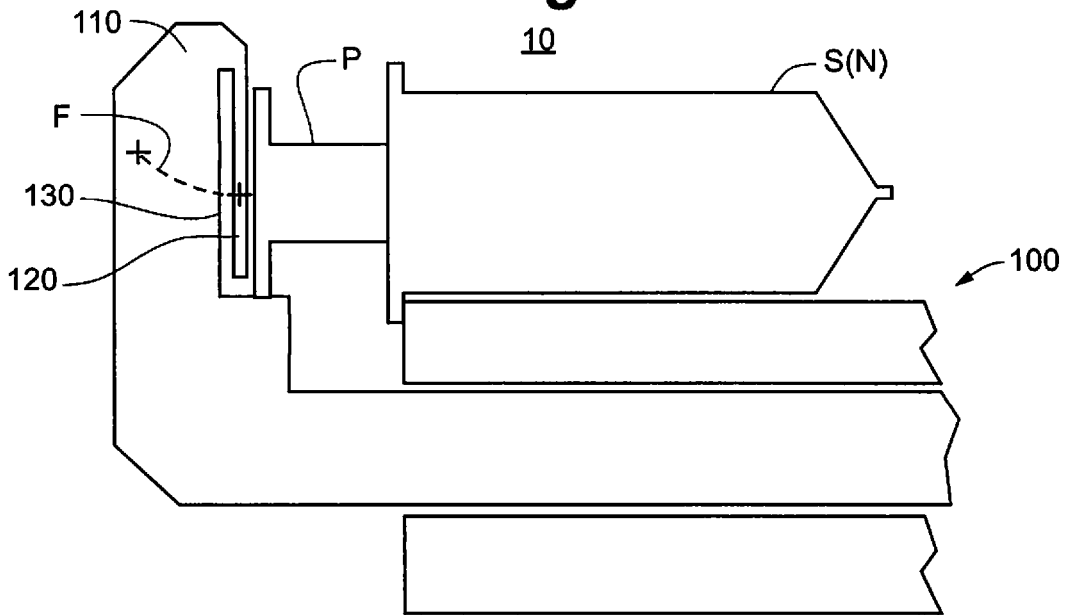


Fig. 1A

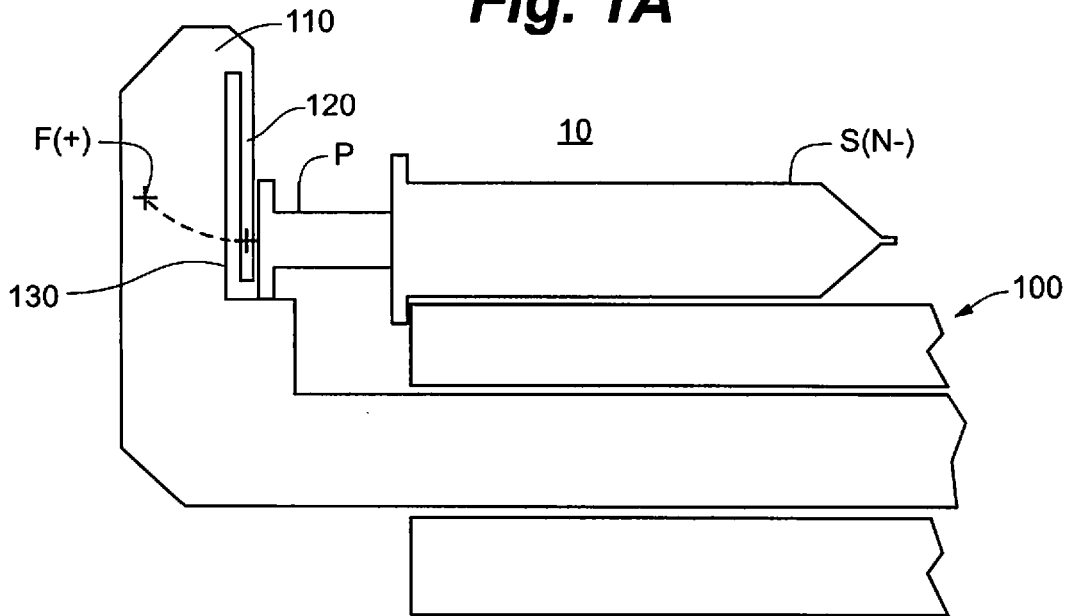


Fig. 2

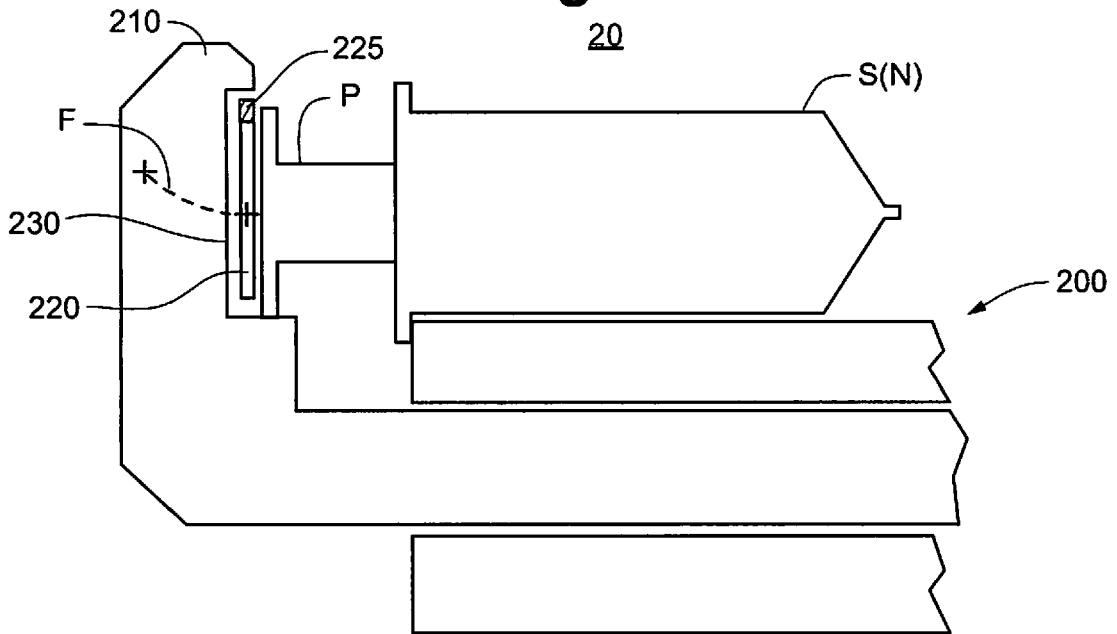


Fig. 2A

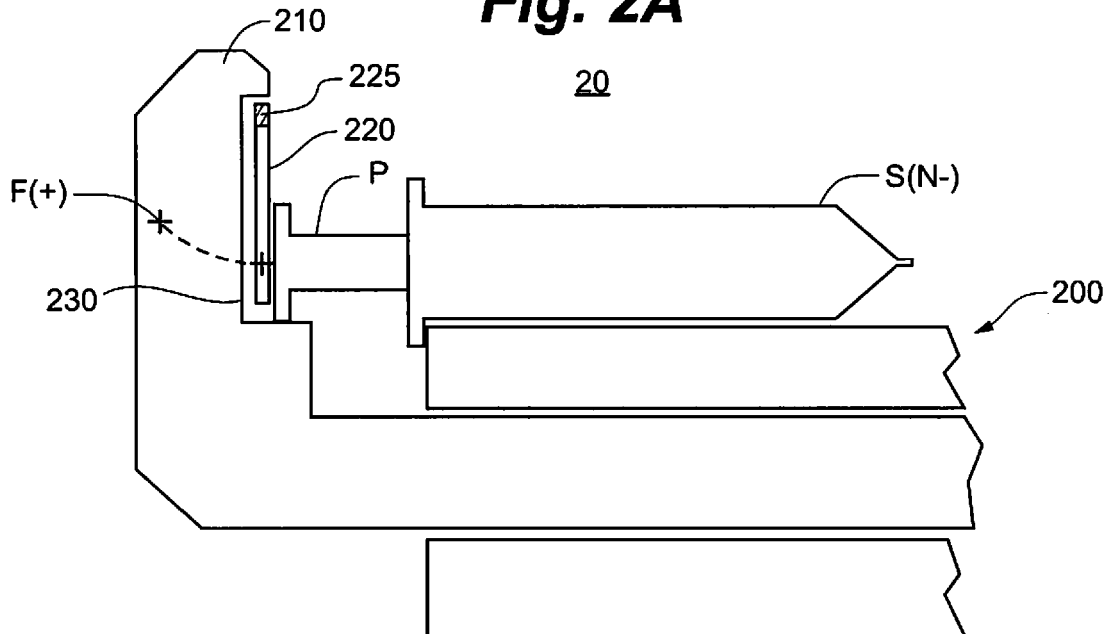


Fig. 3

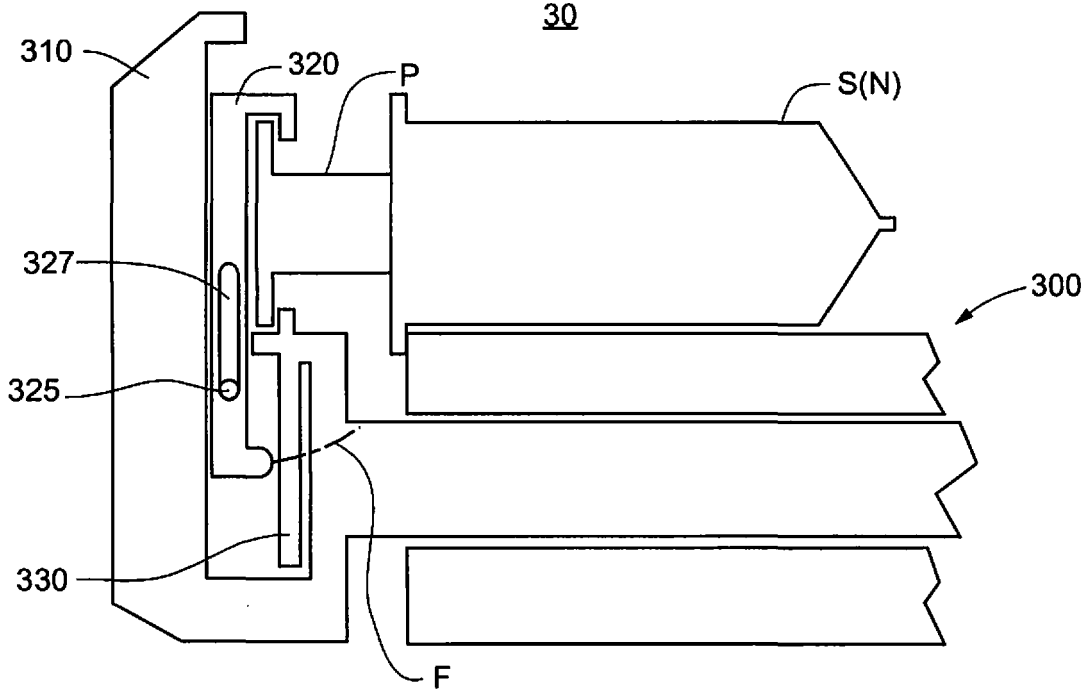


Fig. 3A


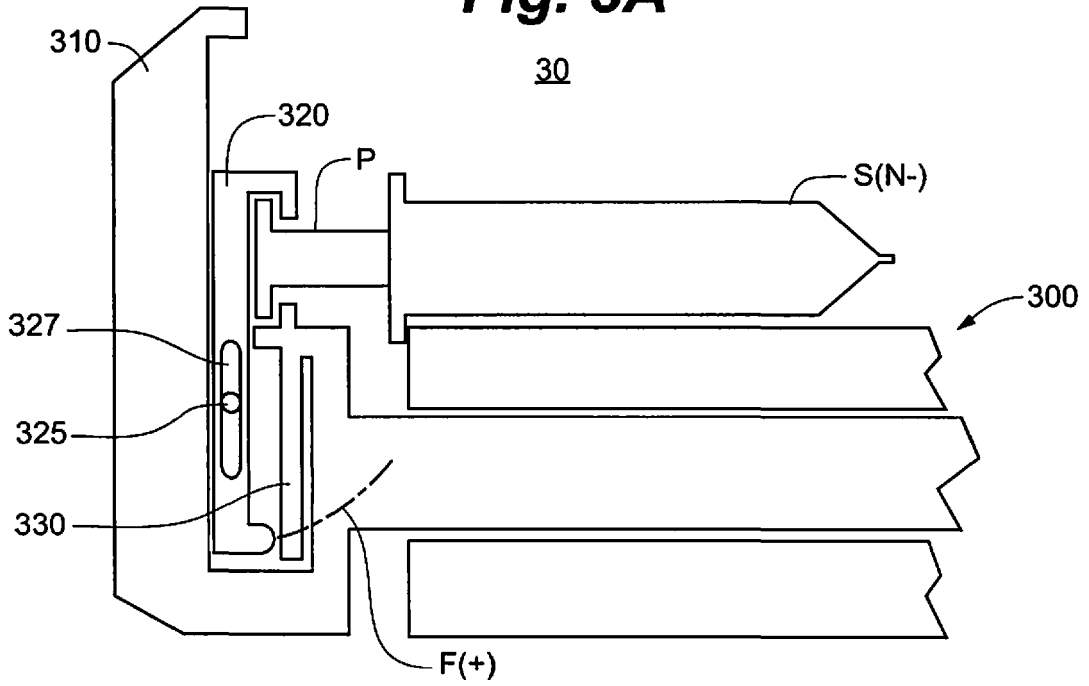


Fig. 4

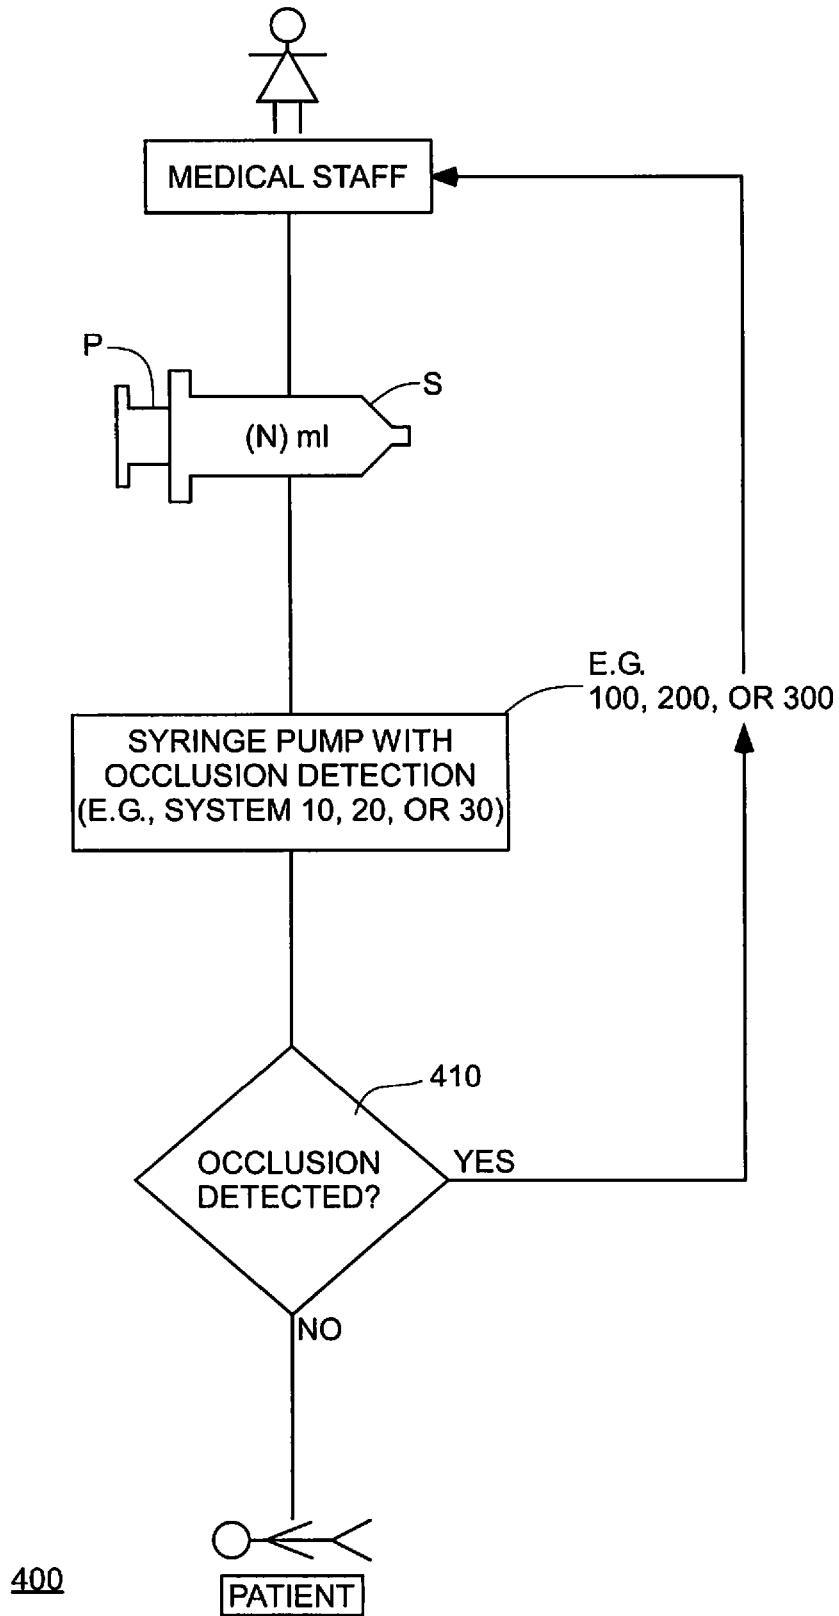

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 4978335 A [0002]
- US 20050096593 A [0002] [0026]
- US 20030229311 A [0003]

专利名称(译)	遮挡检测		
公开(公告)号	EP2854625A4	公开(公告)日	2015-11-18
申请号	EP2013794119	申请日	2013-05-23
[标]申请(专利权)人(译)	史密斯医疗ASD公司		
申请(专利权)人(译)	史密斯医疗ASD , INC.		
当前申请(专利权)人(译)	史密斯医疗ASD , INC.		
[标]发明人	WANDER JACOB A ADAMS GRANT A LACY CHRISTOPHER A		
发明人	WANDER, JACOB, A. ADAMS, GRANT, A. LACY, CHRISTOPHER, A.		
IPC分类号	A61B5/02 A61M5/142 A61B5/00 A61M5/145 A61M5/168		
CPC分类号	A61M5/16831 A61B5/4839 A61B2560/0266 A61M5/1456 A61M2005/16863 A61M2205/18 A61M2205/332 A61M2205/50		
优先权	61/651860 2012-05-25 US		
其他公开文献	EP2854625B8 EP2854625A1 EP2854625B1		
外部链接	Espacenet		

摘要(译)

用于闭塞检测的系统可包括用于包含药物的注射器的注射泵，其中注射器包括柱塞，并且注射泵包括柱塞驱动器。可弯曲元件可以与柱塞驱动器一体地形成，并且力传感器也可以与柱塞驱动器一体地形成。在发生闭塞时，柱塞将向后施加力抵靠可弯曲元件，从而使可弯曲元件偏转成与力传感器接触，从而产生指示闭塞发生的信号。