



(11) **EP 3 117 764 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
03.07.2019 Bulletin 2019/27

(51) Int Cl.:
A61B 5/00 ^(2006.01) **A61B 5/06** ^(2006.01)
A61F 13/12 ^(2006.01)

(21) Application number: **16179579.4**

(22) Date of filing: **14.07.2016**

(54) **A MAGNET-BASED MONITORING SYSTEM**

MAGNETBASIERTES ÜBERWACHUNGSSYSTEM

SYSTÈME DE SURVEILLANCE UTILISANT DES AIMANTS

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **14.07.2015 US 201562192062 P**
12.07.2016 US 201615207879

(43) Date of publication of application:
18.01.2017 Bulletin 2017/03

(73) Proprietor: **Getchell Technologies LLC**
Santa Cruz, CA 95060 (US)

(72) Inventors:
• **Readdie, Mark A.**
Santa Cruz, CA 95061-0320 (US)
• **Chatwin, Jeremy G.**
Santa Cruz, CA 95060 (US)
• **Nyong'o, Omondi L.**
San Francisco, CA 94102 (US)

(74) Representative: **Derry, Paul Stefan et al**
Venner Shipley LLP
200 Aldersgate
London EC1A 4HD (GB)

(56) References cited:
WO-A1-2013/050735 US-A- 5 879 292
US-A1- 2008 177 170 US-A1- 2010 322 859

- **KAIJANUSCHOWSKI ET AL: "Measuring wearing times of glasses and ocular patches using a thermosensor device from orthodontics", ACTA OPHTHALMOLOGICA: THE OPHTHALMOLOGICAL JOURNAL OF THE NORDIC COUNTRIES, vol. 91, no. 8, 1 December 2013 (2013-12-01), pages e635-e640, XP055246470, Denmark ISSN: 1755-375X, DOI: 10.1111/aos.12171**
- **YAROSLAVA CHOPOVSKA ET AL: "Electronic recording of occlusion treatment for amblyopia: potential of the new technology", GRAEFE'S ARCHIVE FOR CLINICAL AND EXPERIMENTAL OPHTHALMOLOGY ; INCORPORATING GERMAN JOURNAL OF OPHTHALMOLOGY, SPRINGER, BERLIN, DE, vol. 243, no. 6, 1 June 2005 (2005-06-01), pages 539-544, XP019342798, ISSN: 1435-702X, DOI: 10.1007/S00417-004-1067-8**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 3 117 764 B1

DescriptionFIELD

[0001] The present invention relates to using magnetometers, and more precisely to the determination of the disposition of an object using magnetometers.

BACKGROUND

[0002] Amblyopia is a vision disorder whereby information from one eye is not completely transmitted or not fully processed by the brain in favor of information from the other, "strong" eye. A common treatment modality for Amblyopia is the periodic occlusion of the "strong" eye for a prescribed duration over a specified time period. Occlusion may be achieved with an opaque "patch" that covers the eye by attachment to the face or by attachment to eyeglass lens or frame. This method of periodic occlusion is commonly referred to as "patching." Patching is also used as a treatment of strabismus and other vision disorders.

[0003] The most common method of tracking such treatment is asking the patient or caregiver to keep diaries or logs of patching without the use of any automation. The diary is reviewed when the patient next meets with their practitioner. This method relies on the patient or caregiver accurately recording these times. However, this may often be inaccurate.

[0004] A prior art apparatus uses two skin contact electrodes added to an adhesive patch and connected to electronics carried in a separate bag. The device seeks to use electrical resistance measurements between the electrodes as a sign of the patch being worn.

[0005] Another prior art apparatus attaches a small, self-contained device to a patch and monitors the temperature difference between the front and back of the device, as a signal for the wearing of the patch. This method does not rely on the patient or caregiver remembering to record timings but does require them to remember to transfer the sensor/microcontroller combination from patch to patch. Such devices are disclosed in "Measuring wearing times of glasses and ocular patches using a thermosensor device from orthodontics" from Kai Januschowski et al. (the ophthalmologic journal of the nordic countries, vol. 91, no. 8, 1.12.2013) or in "Electronic recording of occlusion treatment for amblyopia: potential of the new technology" from Yaroslava Chopovska et al. (Graefe's Archive for clinical and experimental ophthalmology, vol. 243, no. 6, 1.06.2005).

SUMMARY OF THE INVENTION

[0006] The scope of protection is defined by the claims.

BRIEF DESCRIPTION OF THE FIGURES

[0007] The present invention is illustrated by way of

example, and not by way of limitation, in the figures of the accompanying drawings and in which like reference numerals refer to similar elements and in which:

Figure 1 is a block diagram of one embodiment of an occlusion dosage monitor (ODM).

Figure 2A illustrates one embodiment of a top view of the user's face, showing glasses and logging device.

Figure 2B illustrates a cross-section of the logging device and one glass arm, showing the relative positions.

Figure 2C illustrates an embodiment of the logging device showing two sensors.

Figure 2D illustrates one embodiment of the logging device showing one sensor.

Figure 2E is a block diagram of one embodiment of the logging device.

Figure 2F is an exemplary circuit diagram of one embodiment of the logging device.

Figure 3A, 3C, and 3D illustrate embodiments of a top view of the user's face, showing glasses, patch, and logging device.

Figure 3B illustrates an exemplary patch, showing one embodiment of a relative location of the magnet.

Figure 4 is a flowchart of one embodiment of utilizing the system. Figure 5A illustrates an exemplary time-series output from an ODM with a single magnetometer, and a large magnet.

Figure 5B illustrates an exemplary time-series output from an ODM with a single magnetometer, and a small magnet.

Figure 5C illustrates an exemplary time-series output from an ODM with two magnetometers, and a small magnet.

DETAILED DESCRIPTION

[0008] Amblyopia is a vision disorder whereby information from one eye is not completely transmitted or not fully processed by the brain in favor of information from the other, "strong" eye. A common treatment modality for Amblyopia is the periodic occlusion of the "strong" eye for a prescribed duration over a specified time period. Occlusion may be achieved with an opaque "patch" that covers the eye or attaches to the eyeglass frame or lens. This method of periodic occlusion is commonly referred to as "patching". Patching is also used as a treatment of Strabismus and other vision disorders.

[0009] The system described in one embodiment utilizes a small magnet, in an eye patch such that the magnet is positioned on the side of the face in the region just behind the eye (or directly over the eye), or placed on or near where the lens and the leg of the spectacles meet (for the case of a patch on the lens), and one or more magnetometers to monitor compliance with the required wearing of the patch. This permits the use of a lightweight, simple, and cheap patch. It also permits adding a magnet

to an existing patch.

[0010] The presence or absence of the magnet is monitored by a device in close proximity to the magnet. In one embodiment, the logging device may be attached to the adjacent leg ("temple") of a pair of eyeglasses. The logging device makes and stores measurements of the magnetic field. Analysis of these measurements allows for a determination of those periods in time when the magnet is and is not present and further, when a magnet is present, it's disposition. In one embodiment, the distance from the nearest part of the device to the magnet may typically be less than 7,62 cm (3 inches). In other applications this distance can be longer, or shorter.

[0011] The detection of the magnet takes account of the sharp spatial drop-off in the magnetic field from the magnet; the presence of the background magnetic field of the Earth with respect to which the temple and magnetometer(s) change orientation as the eyeglasses move with their wearer; and the measurement errors of practical magnetometers.

[0012] The goal is to provide, after a period of operation of a device, a time-series of numbers which when graphed allow identification of those time periods during which the magnet was present (patch on) and absent (patch off). In addition, the data may be used to determine when the eyeglasses were stationary and deduce when the glasses were not being worn. This is of value quite apart from knowing when the patch was on.

[0013] In one embodiment, one magnetometer may be used to detect a large enough magnet. In another embodiment, two magnetometers are used in combination to detect smaller/weaker magnets. Because the magnet is worn, having a lower magnetic force, and smaller magnet is preferred, to minimize risks to health (swallowed magnets), electronic devices, and for comfort.

[0014] The below examples focus on an occlusion dosage monitor, but one of skill in the art would understand that the combination of magnet, magnetometer(s), and analysis described below may be applicable to other uses in which the disposition of an object may be monitored over time.

[0015] Figure 1 illustrates one embodiment of the ODM system. The system in one embodiment includes a Modified Eye-Patch (109) with a magnet (100), a Logging Device (101), a Base Station or interrogator (102), and a Data Processor (103). The modified eye-patch (109) may be attached to the eyeglass lens, stuck over the user's eye, or attached in some other way to occlude the selected eye. The Logging Device (101) is kept in close proximity to the patch.

[0016] The Logging Device (101) is mounted on a pair of eyeglasses (104) worn by the patient.

[0017] The Logging Device (101) communicates with a Base Station (102) via a communication link (105). The communication link (105) may utilize, but is not limited to, a wired or wireless or optical connection. In one embodiment, the Logging Device (101) is designed to have enough memory to log data until the user visits the med-

ical doctor, where the communication link (105) may be connected to the Logging Device (101), and the data may be downloaded. The communication link (105) may be a MicroUSB or other small form factor connector.

[0018] The Base Station (102) may connect to the Data Processor (103) for the purpose of data collation and analysis. To effect this connection, the Base Station (102) may have a connection (106) to the Internet (107). Similarly the Data Processor (103) may also have a connection (108) to the Internet (107). Alternatively the Base Station (102) and Data Processor (103) may communicate directly or via some other means. Alternatively, Base Station (102) may be within the same computing device as Data Processor (103) and they may communicate directly via an internal bus or similar communication mechanism.

[0019] The Logging Device (101) is mounted on the eyeglasses (104) as depicted in Figure 2A. The curvature (201) represents the user's facial contour, depicted from above, with the glasses (104) and the attached logging device (101) also shown. In one embodiment, the Logging Device is positioned along the eyeglasses leg with a preference to position it as far from the eye as possible, while still maintaining detection range. In one embodiment, as shown, the Logging Device (101) may be mounted on the outside of the left arm of the Patient's eyeglasses to monitor the occlusion dose of the left eye. In the case when the right eye is to be patched the Logging Device (101) may be mounted on the outside of the right arm of the Patient's eyeglasses. Other mounting configurations may also be used. For example the logging device (101) may be mounted on the inside of the eyeglass frame. The particular mounting configuration may depend upon the size and style of the patient's eyeglasses.

[0020] A modified eye patch (109) is shown in Figure 3B. In one embodiment, it is of the type commonly used for amblyopia treatment. In one embodiment, the eye patch (109) is one of: an adhesive bandage patch which is applied to the user's face to cover the eye, a patch for attaching to the eyeglasses in front of or behind the lens, and an eye patch over the eye which is held in place by an elastic band or string. The patch (109) is customized by the addition of a magnet (301). The magnet (301) may be built into the eye patch, stuck on the eye patch, enclosed in a cover which is adhered to the outside of the eye patch, or inserted within the patch during manufacture. A magnet is considered to be any device that creates a magnetic field. In one embodiment, instead of a permanent magnet, magnet (301) may be multiple smaller magnets, an electromagnet, or something else which generates a magnetic field. The magnet is small in size and lightweight, to minimize discomfort to the wearer. In one embodiment, the magnets also have low magnetic field strength. This is for patient safety and for minimal interference with other devices or cards with magnetic stripe.

[0021] The magnet (301) in one embodiment is attached securely to, or embedded within, the patch (109)

at a location on the outside edge of the patch. In one embodiment, the location of the magnet (301) is preferably in an area on or above the cheek. Generally patches are directional.

[0022] Figure 2B shows a cross section through the arm of the eyeglasses (104) and the Logging Device (101). The Logging Device is attached to the arm of the eyeglass by an attachment mechanism, such as heat shrink tubing, glue, epoxy, hook and loop fastener, screw, tension mount, clasp, etc. The logging device (101) should not move or shift with respect to the eyeglass leg. The attachment may be permanent or temporary. In one embodiment, the long axis of the Logging Device (101) is largely parallel with the eyeglasses leg (104), when attached. The same configuration may be used to monitor the left eye or the right eye. In one embodiment, rotation of the logging device (101) about this long axis, parallel with the eyeglass leg, allows mounting on the opposite eyeglass leg, enabling use of the same Logging Device (101) configuration, regardless of which site it is to be used for.

[0023] The preferred embodiment contains two magnetic sensors (202 & 203) as shown in Figure 2C.. An alternate embodiment with a single sensor is shown in Figure 2D. In one embodiment, as shown in Figure 2C the two sensors are aligned along the long axis of the logging device, and placed relatively far from each other. The two magnetometers are further aligned with respect to each other such that the X axis of the first magnetometer is substantially parallel to the X axis of the other magnetometer, and similarly with the Y and Z axes. The sensors may also be placed in any orientation with respect to the eyeglasses. In one embodiment, the separation between the sensors is maximized within the constraints of the logging device enclosure. In one embodiment, the positioning of the two magnetometers is such that the magnetic field detected by each from the magnet in the patch is different due to the magnet's dipole field. This enables use of the spatially variable field to detect a smaller magnet more accurately, and will be discussed below.

[0024] The magnetic sensors (202, 203) each measure the intensity and direction of the magnetic field passing through them. That is, they measure the magnetic field vector passing through them.

[0025] In the real world, magnetometers although sensitive can provide wildly inaccurate readings, due to large offset and differing axis gains which can drift over time. However, analysis can circumvent these issues. Prior art magnetometer systems either ignore offsets and gains, and assume that measurements are highly accurate as well as sensitive, or require intense calibration methods prior to measurements being conducted.

[0026] The output measure of each of the magnetometer's axis measurements can be modeled as a linear function of the component of the magnetic field present in the direction of the axis in question, with an offset, and a smaller cross-coupling contribution from off-axis com-

ponents of the magnetic field. We can approximate this mathematically, in vector form, as: $\underline{M} = \underline{A} + \underline{G} \cdot \underline{B} + \underline{\epsilon}$
Where

$\underline{M}$ is the measurement output 3-vector, with a component for each of the three axes.

$\underline{B}$ is the true 3-vector magnetic field being measured
 $\underline{A}$ provides the offset for each of the three axes.

$\underline{G}$ is a mostly diagonal 3x3 matrix multiplying each of the components of $\underline{B}$ along a given axis, to contribute a measured effect along the same axis. The off-diagonal terms couple the components of $\underline{B}$ with measured effects in magnetometer axes orthogonal to them.

$\underline{\epsilon}$ is a 3-vector representation of the small random errors due to thermal fluctuations and transient interference effects within the electronic circuitry. It will have a zero mean.

[0027] Calibration of a non-ideal magnetometer can be attempted by rotating the magnetometer in a constant magnetic field and taking measurements at many orientations, and then running a mathematical algorithm to best fit the measurements to an ellipsoid. The result of this fit yields values for a constant $\underline{A}$ and $\underline{G}$, and for the standard deviation of the random error, $\underline{\epsilon}$. Such calibration is not possible in the operation of a Logging Device and can be overcome through suitable analysis of the measurement output.

[0028] With a single magnetometer embodiment, in one embodiment, the process uses a shift in the range observed magnitude of $\underline{M}$ ($|\underline{M}|$) values to discern those time periods when a magnet is present. With the dual magnetometers, in one embodiment, a shift in the $|\underline{M}|$ level is used to discern the presence of the magnet.

[0029] Fig 5A shows modeled output of a single magnetometer with a relatively large magnet introduced and removed. The presence of the magnet can be clearly discerned by the jump in measured magnitude of the sensor's vector output. The period during which the magnet was present is designated by lines, beginning at time-point 93 and ending at time-point 231.

[0030] Fig. 5B shows the same single magnetometer and magnet disposition over time as in Fig. 5A but with a weaker magnet. It will be seen that the presence of the magnet cannot be reasonably discerned from the magnitude signal. This is because the magnet produces a field at the magnetometer which when added to the Earth's magnetic field cannot be distinguished from that of the Earth due to the inherent non-idealities of a practical magnetometer.

[0031] Fig 5C shows the results of an identical arrangement to that in Fig 5B, but with the addition of a second magnetometer. Fig 5C show the time plot of the difference in measured output of each magnetometer for each of the three aligned, orthogonal axes, X, Y and Z. The presence and absence of the magnet can now clearly be discerned.

[0032] These figures show that the operational regime of a single practical magnetometer will meet a limit at small magnet strength, and this limit can be surpassed by using a second magnetometer of same design, but using the difference vector.

[0033] Figure 2D illustrates the alternative embodiment not forming part of the present invention with a single magnetometer. The magnetometer may be positioned anywhere along the logging device. In one embodiment, the magnetometer is positioned along the portion of the logging device that is closest to the patch. In this embodiment the magnet must be sufficiently strong to make a contribution to the magnetic field at the single magnetometer sufficient to be detectable by the measurement process which combines the effects of offsets, different axis gains and the presence of the Earth's magnetic field. The small random errors, ϵ reduce the sensitivity but are small compared with typical offset and gain effects which greatly reduce the accuracy of M as a direct correlate of the magnetic field vector being measured. With this embodiment, the effects of other local fields such as telephones, headphones or other sources may be sufficient under certain circumstances to prevent a clear determination of the presence or absence of a magnet. The employment of operational rules adopted by the patient and care-giver limiting the presence of such magnetic field sources would allow full determination of the presence or absence of a magnet.

[0034] Figure 2E shows one embodiment of the Logging device (101), which includes one or more magnetometers (220), a microcontroller (222), non-volatile memory (224) such as a Flash memory, a battery or electrical power source (226), and a connection mechanism (228). In one embodiment, the battery (226) may be a small watch battery. In one embodiment, the battery (226) may be rechargeable. In one embodiment, the microcontroller (222) is an Atmel ATtiny85. In one embodiment, the magnetometers (220) are 3-Axis Digital Compass IC HMC5883L by HONEYWELL™.

[0035] The connection mechanism (228) provides a method to communicate the data stored in the Logging Device (101) to the base station (102) described above. In one embodiment, the connection mechanism (228) also provides a path for communication from the Base Station (102) to the Logging Device (101). In one embodiment, the raw data received by the magnetometers (220) is processed by microcontroller (222) and stored in memory (224). In another embodiment, the raw magnetometer data is stored in memory, and processing is done in data processor (103) or other computer system remote from the logging device (101). Once stored, the data is available for download/access. Figure 2F is an exemplary circuit diagram of one embodiment of the Logging Device.

[0036] One embodiment of the relative position of the magnet (301) and the magnetic sensors (202 & 203) is shown in Figure 3A. The user's eye area/facial curvature 201 is partially covered by patch 109, which includes a

small magnet 301. In one embodiment the patch adheres to the patient's face around the patch rim. The sensors (202 & 203) and magnet (301) need not be aligned. However in one embodiment the positioning of the logging device with respect to the magnet is optimized such that the magnetic field vector sensed by each magnetic sensor (202 & 203) is measurably different. This optimum position may depend on the shape and size of the patient's head and the configuration of the spectacles and patch.

[0037] When the magnet (301) is not present both magnetic sensors are subject to the Earth's magnetic field. The distance separating the magnetic sensors is small and so the Earth's magnetic field measured by the two sensors is assumed identical. When a strong dipole magnetic field, such as that generated by the magnet, is positioned relatively close to the logging device each magnetic sensor experiences a differing field vector. Since magnetic strength falls off at the cube of distance ($1/r^3$), even a small distance between the sensors will have a real impact on the magnetic field detected. In addition, if the magnet were equidistant from the two magnetometers, while the field strengths might be commensurate, their directions would differ. The foregoing may also be true for more complex fields, such as that from two or more magnets.

[0038] Therefore using a mathematical model of the dipole (or more complex) field, the relative position of the magnet with respect to the logging device may be inferred from the size and direction of the vector difference of the two sensors. Using this method, it is possible to infer if a patch is being worn or not. Other, local fields may be present temporarily, emanating from telephones, headphones, etc. - either while the eyeglasses are worn, stored or transported. Although such fields will also generate a vector difference in the magnetic fields of the two sensors, their size, orientation and variation in time will often be distinguishable from those of magnet on the patch when the Data Processor analyzes the measurements.

[0039] Figures 3C and 3D illustrate alternative patch configurations, in which the patch is attached to the eyeglasses either in front or behind the lens of the glasses, or is a freestanding or non-adhesive patch, secured with an elastic or similar attachment mechanism. The configuration of the patch is not limited, and merely requires a patch that can be modified with a magnet.

[0040] Figure 4 is a flowchart of one embodiment of utilizing the system. The process starts at block 410, when the system is initialized.

[0041] At block 420, instructions are received from the Logging Device microcontroller to measure the magnetic field. In one embodiment, this is detected as a three-dimensional vector quantity from each magnetometer. In one embodiment, this occurs periodically. The period may be invariant, on the order of seconds, or minutes. The period may be variable depending on anticipated activity levels or time of day. In one embodiment the pe-

riod is nominally invariant at one minute. In certain other embodiments the period may be controlled adaptively.

[0042] At block 430, these measurements may be examined by a program in the microcontroller to calculate derived information. In one embodiment, the derived information is a differential measurement between the two magnetometers to minimize the influence of earth's magnetic field. In other embodiments, this block is bypassed and the derived information may merely be the unchanged, raw measurements.

[0043] At block 440, the derived information is stored in memory. In one embodiment, the memory is non-volatile memory such as Flash memory. In one embodiment, the data is stored with time-stamp information. The derived information, together with the corresponding time-stamp information is collectively termed the "Data Log". In another embodiment, time stamp information is stored only on every N-th measurement, since the periodicity permits derivation of the actual time. In one embodiment, the time stamp information is stored only every 3 hours. In a further embodiment, no timestamp information is recorded, save for the time of the initiation of monitoring. The timestamps for each measurement are inferred by the position of the measurements in the data log, together with knowledge of the measurement period.

[0044] The data log, that is the time varying record of the two magnetic sensors measurements, may also be used to infer other useful data concerning the patient during the measurement period, in one embodiment. For example, variations in measured field over time indicate that the patient is awake, whereas a long period of non-movement indicates sleep. Periods during which the eyeglasses and sensors are being carried but not worn may be discernable by deducing their orientation with respect to the background magnetic field of the Earth. Knowing when the patient is wearing a patch whilst sleeping (which means the eyes are not being utilized) may be useful for the practitioner to make a more accurate assessment of the effective occlusion dosage.

[0045] At block 450, the data is communicated to a base station. The Logging Device includes a connection (105) which enables it to communicate with a Base Station. This connection may be used in both directions: for communication both to and from the Logging Device from and to the Base Station. One purpose of the connection is to download the Data Log stored in the Logging Device's memory to the Base Station. Another purpose of the connection may be to transfer diagnostic or other operating commands from the Base Station to the Logging Device. The connection (105) may be a wired connection such as USB/MicroUSB or wireless such as a Personal Area Network, for example a Bluetooth or NFC (Near-Field Communication) connection.

[0046] The Base Station (102) may be a personal computer, tablet, smart-phone, or customized device. The form of communication (105) between the Logging Device (101) and Base Station (102) may have different forms.

[0047] In addition, the Base Station has a connection to a Data Processor (103). This connection may be via the Internet (106, 107 & 108), a wired connection, an internal bus if the Base Station (102) resides on the same device as the Data Processor (103), or through an alternative mechanism.

[0048] In one embodiment, the Base Station (102) is used to regularly download the Data Log from the Logging Device (101). In one embodiment, the Base Station (102) may be at the office of a specialist treating the user. In another embodiment, the Base Station (102) may be the user's smart phone with an application enabling such a download. In one embodiment, a software program ("Client Software") on the Base Station is part of the preferred embodiment. The Client Software stores the downloaded Data Log on the Base Station's memory. In one embodiment, the connection may also be used to communicate status information, or updates, to the Logging Device.

[0049] At block 460, the data is provided to the Data Processor.

[0050] At block 470, the analysis of the captured Data is performed by the Data Processor (103). Analysis in one embodiment, processes the data and determines based on the data collected over a period of time, those sub-periods during which eyeglasses and a modified patch were worn together by the Patient. In one embodiment this analysis may be automated, in another it may be performed by a trained operator. In one embodiment, a second output of the analysis is a determination of those sub-periods during which the eyeglasses were worn but without a patch. In one embodiment, these determinations include a measure of confidence (a probable correctness of the determination.)

[0051] At block 480, the output of the analysis is provided to the Patient, his/her caregiver and to the physician. In one embodiment, the output may be provided via the Data Processor, the Base Station, another linked computer system or display system. In one embodiment, the output may be provided via email, text, application, or a website to authorized parties, including the patient. In one embodiment, the output is a chart of the times when the user was wearing the patch, and not wearing the patch. In one embodiment, a trained professional can then utilize this data to make recommendations, evaluate compliance, and potentially alert the patient's treatment plan based on the results.

[0052] In one embodiment, the system may alert the user, care-giver and/or physician's office of non-compliance. In one embodiment, an alert, may be sent. Some exemplary alerts may include: "To Doctor's office: Patient X has diverged from compliance please take a look." Or before that "To Caregiver: Patient is not patching the prescribed amount of time. Do you need any help?" Or potentially "To User: Please comply with the occlusion dosage prescribed."

[0053] The process then ends at block 490.

[0054] The magnetometer system may be used for oth-

er applications apart from occlusion monitoring, but these applications do not form part of the present invention. Exemplary applications include any application in which an object may include a magnet, and the object's disposition (positions and/or orientation) is relevant. The positions and/or orientation may be monitored with respect to rotational movements, translational movements, and combinations of rotational and translational movements. Examples of rotational movements include positions of a gate, door, lid, or any hinged object, where the monitoring may provide information about whether it is closed or ajar and to what degree. Other examples include a control dial or lever, actuator, spindle, wheel, faucet.

[0055] Examples of translational movements which can be monitored are sliding controls, doors, windows, drawers, lids & fluid levels. Furthermore, air movement may be detected by way of a small magnet suspended on a light fabric or vane. This method may determine whether a HVAC unit or a ceiling fan is active, for example. Alternatively it may be used to indicate the existence and direction of drafts within a room.

[0056] Applications combining rotational and translational motion may include monitoring of flexing members, eccentricity caused by bearing wear, weight scales, or a situation in which a deviation from any expected relative motion between objects occurs, such as an object which should be securely fastened during transportation. For example, flexure of a dog leash and therefore its use over a period of time can be monitored by attachment of a small magnet and the logging device to the leash.

[0057] In the foregoing specification, the invention has been described with reference to specific exemplary embodiments thereof. It will, however, be evident that various modifications and changes may be made thereto without departing from the scope of the appended claims. The description and drawings are, accordingly, to be regarded in an illustrative rather than a restrictive sense.

Claims

1. A magnetometer-based monitoring system comprising:
an eye patch (109) whose disposition is to be monitored; eyeglasses (104) adapted to be worn by a user; a processor (222) to determine the disposition of the eye patch (109); **characterised in that** a magnet (100) is integrated with the eye patch (109); a first magnetometer (202) and a second magnetometer (203) are integrated with a logging device (101), the logging device being attached to said eyeglasses such that the first magnetometer (202) is located in proximity to the eye patch and the second magnetometer (203) is located at a fixed distance from the first magnetometer in proximity to the eye patch; with the processor receiving data from the first magnetometer and the second magnetometer, and calculating a measurement vector to determine the dis-

position of the eye patch (109).

2. The magnetometer-based monitoring system of claim 1, wherein the eye patch comprises:

a covering portion to substantially cover one eye; and
the magnet is positioned on a side of the eye patch, such that the first magnetometer and the second magnetometer detect a magnetic field of the magnet, the presence of the magnet used to determine the compliance with a medical protocol.

3. The magnetometer-based monitoring system of claim 1, wherein the magnet is one of: built into the eye patch, enclosed in a cover which is adhered to the outside of the eye patch, stuck on the eye patch, or inserted within the eye patch during manufacture.

4. The magnetometer-based monitoring system of claim 1, wherein the logging device further comprises the processor, which is a microprocessor, and a memory.

5. The magnetometer-based monitoring system of claim 1, wherein the disposition of the object determines whether a user is wearing the eye patch including the magnet, to monitor compliance with a medical protocol.

6. The magnetometer-based monitoring system of claim 5, wherein the protocol is treatment of amblyopia.

7. The magnetometer-based monitoring system of claim 1, further comprising:

a memory to store data from the first magnetometer and the second magnetometer; and
a communication link to communicate data from the memory to the processor.

8. The magnetometer-based monitoring system of claim 7, further comprising:
a microprocessor to obtain the data from the first magnetometer and the second magnetometer, and store the data in the memory.

9. The magnetometer-based monitoring system of claims 1-8, wherein the first magnetometer and the second magnetometers are arranged to be in close proximity to the magnet in the eye patch, the magnetometers monitoring a magnetic field, generated by the magnet, earth, and proximate magnetic devices; and the magnetometer-based monitoring system further comprising:

- a memory to store data from the magnetometer;
and
a communication link to obtain the data from the memory, the data processed to show a pattern of wearing and not-wearing the eye patch, to monitor compliance with a medical prescription.
10. The magnetometer-based monitoring system of claim 11, further comprising:
the processor comprising a microcontroller to control a timing of measurements of the magnetic field, and storing of the data.
11. The magnetometer-based monitoring system of claim 11, further comprising:
a base station to receive data from the logging device, the base station comprising one of: a smart phone, a computer application, and a special purpose device.
12. The magnetometer-based monitoring system of claim 11, wherein the processor is
a data processor to process the data from the logging device, the data processor to determine the pattern of wearing and not-wearing the eye patch, to monitor compliance with a medical prescription.
13. The magnetometer-based monitoring system of claim 12, further comprising:
a communication system to inform one or more of the user, a medical professional, and a designated party of the pattern.

Patentansprüche

1. Magnetometerbasiertes Überwachungssystem, umfassend:
- eine Augenbinde (109), deren Anordnung zu überwachen ist; Augengläser (104), die angepasst sind, um von einem Nutzer getragen zu werden; einen Prozessor (222) zum Bestimmen der Anordnung der Augenbinde (109); **dadurch gekennzeichnet, dass** ein Magnet (100) in die Augenbinde (109) integriert ist;
ein erstes Magnetometer (202) und ein zweites Magnetometer (203) in einer Aufzeichnungsvorrichtung (101) integriert sind, wobei die Aufzeichnungsvorrichtung an die Augengläser angebracht ist, sodass sich das erste Magnetometer (202) in der Nähe zur Augenbinde befindet und sich der zweite Magnetometer (203) in einem festen Abstand von dem ersten Magnetometer in der Nähe zur Augenbinde befindet; wobei der Prozessor Daten vom ersten Magnetometer und vom zweiten Magnetometer empfängt; und Berechnen eines Messvektors, um

die Anordnung der Augenbinde (109) zu bestimmen.

2. Magnetometerbasiertes Überwachungssystem nach Anspruch 1, wobei die Augenbinde umfasst:
einen Abdeckungsabschnitt, um im Wesentlichen ein Auge abzudecken;
und wobei der Magnet an einer Seite der Augenbinde positioniert ist, sodass das erste Magnetometer und das zweite Magnetometer ein Magnetfeld des Magneten detektieren, wobei das Vorhandensein des Magneten verwendet wird, um die Einhaltung eines medizinischen Protokolls zu bestimmen.
3. Magnetometerbasiertes Überwachungssystem nach Anspruch 1, wobei der Magnet eines der folgenden ist: in die Augenbinde eingebaut, in einer Abdeckung umschlossen, die an die Außenseite der Augenbinde geklebt ist, auf die Augenbinde gesteckt oder während der Herstellung in die Augenbinde eingesetzt.
4. Magnetometerbasiertes Überwachungssystem nach Anspruch 1, wobei die Aufzeichnungsvorrichtung ferner einen Prozessor, bei dem es sich um einen Mikroprozessor handelt, und einen Speicher umfasst.
5. Magnetometerbasiertes Überwachungssystem nach Anspruch 1, wobei die Anordnung des Objekts bestimmt, ob ein Nutzer die den Magneten enthaltende Augenbinde trägt, um die Einhaltung eines medizinischen Protokolls zu überwachen.
6. Magnetometerbasiertes Überwachungssystem nach Anspruch 5, wobei das Protokoll eine Behandlung von Amblyopie ist.
7. Magnetometerbasiertes Überwachungssystem nach Anspruch 1, ferner umfassend:
einen Speicher zum Speichern von Daten vom ersten Magnetometer und zweiten Magnetometer;
und eine Kommunikationsstrecke, um Daten vom Speicher zum Prozessor zu kommunizieren.
8. Magnetometerbasiertes Überwachungssystem nach Anspruch 7, ferner umfassend:
einen Mikroprozessor, um die Daten vom ersten Magnetometer und vom zweiten Magnetometer zu erhalten und die Daten im Speicher zu speichern.
9. Magnetometerbasiertes Überwachungssystem nach den Ansprüchen 1 bis 8, wobei das erste Ma-

gnetometer und das zweite Magnetometer angeordnet sind, um sich in enger Nähe zum Magneten in der Augenbinde zu befinden, wobei die Magnetometer ein Magnetfeld, das vom Magneten erzeugt wird, Masse und nahegelegene Magnetvorrichtungen überwachen und wobei das magnetometerbasierte Überwachungssystem ferner umfasst:

einen Speicher zum Speichern von Daten vom Magnetometer;
und eine Kommunikationsstrecke, um die Daten vom Speicher zu erhalten, wobei die Daten verarbeitet werden, um ein Muster des Tragens und Nicht-Tragens der Augenbinde zu zeigen, um die Einhaltung einer medizinischen Verordnung zu überwachen.

10. Magnetometerbasiertes Überwachungssystem nach Anspruch 11, ferner umfassend:
den Prozessor, umfassend eine Mikrosteuerung, um eine Zeitgebung von Messungen des Magnetfelds zu steuern und die Daten zu speichern.

11. Magnetometerbasiertes Überwachungssystem nach Anspruch 11, ferner umfassend:
eine Basisstation zum Empfangen von Daten von der Aufzeichnungseinheit, wobei die Basisstation eines der folgenden umfasst: ein Smartphone, eine Computeranwendung und eine Spezialvorrichtung.

12. Magnetometerbasiertes Überwachungssystem nach Anspruch 11, wobei der Prozessor ein Datenprozessor zum Verarbeiten der Daten von der Aufzeichnungsvorrichtung ist, wobei der Datenprozessor dazu vorgesehen ist, das Muster des Tragens und Nicht-Tragens der Augenbinde zu bestimmen, um die Einhaltung einer medizinischen Verordnung zu überwachen.

13. Magnetometerbasiertes Überwachungssystem nach Anspruch 12, ferner umfassend:
ein Kommunikationssystem, um einen oder mehrere des Nutzers, einer medizinischen Fachkraft und einer ernannten Partei über das Muster zu informieren.

Revendications

1. Système de surveillance basé sur un magnétomètre, comprenant :

un cache-oeil (109) dont la disposition doit être surveillée ; des lunettes (104) adaptées pour être portées par un utilisateur ; un processeur (222) pour déterminer la disposition du cache-oeil (109) ; **caractérisé en ce qu'un** aimant (100) est intégré dans le cache-oeil (109) ; un premier magnétomètre (202) et un deuxième

magnétomètre (203) sont intégrés à un dispositif de journalisation (101), le dispositif de journalisation étant attaché auxdites lunettes de manière à ce que le premier magnétomètre (202) soit situé à proximité du cache-oeil et que le deuxième magnétomètre (203) soit situé à une distance fixe depuis le premier magnétomètre à proximité du cache-oeil ; avec le processeur recevant des données depuis le premier magnétomètre et le deuxième magnétomètre, et calculant un vecteur de mesure pour déterminer la disposition du cache-oeil (109).

2. Système de surveillance basé sur un magnétomètre selon la revendication 1, dans lequel le cache-oeil comprend :

une partie de recouvrement destinée à sensiblement recouvrir un oeil ;
et l'aimant est positionné sur un côté du cache-oeil, de manière à ce que le premier magnétomètre et le deuxième magnétomètre détectent un champ magnétique de l'aimant, la présence de l'aimant utilisée pour déterminer la conformité à un protocole médical.

3. Système de surveillance basé sur un magnétomètre selon la revendication 1, dans lequel l'aimant est au choix : intégré dans le cache-oeil, enfermé dans un capot qui est adhérent à l'extérieur du cache-oeil, collé sur le cache-oeil ou inséré à l'intérieur du cache-oeil pendant la fabrication.

4. Système de surveillance basé sur un magnétomètre selon la revendication 1, dans lequel le dispositif de journalisation comprend en outre un processeur, qui est un microprocesseur, et une mémoire.

5. Système de surveillance basé sur un magnétomètre selon la revendication 1, dans lequel la disposition de l'objet détermine si un utilisateur porte le cache-oeil incluant l'aimant, pour surveiller la conformité à un protocole médical.

6. Système de surveillance basé sur un magnétomètre selon la revendication 5, dans lequel le protocole est un traitement de l'amblyopie.

7. Système de surveillance basé sur un magnétomètre selon la revendication 1, comprenant en outre :

une mémoire pour stocker des données en provenance du premier magnétomètre et du deuxième magnétomètre ;
et une liaison de communication pour communiquer des données en provenance de la mémoire au processeur.

8. Système de surveillance basé sur un magnétomètre selon la revendication 7, comprenant en outre :
un microprocesseur pour obtenir les données en provenance du premier magnétomètre et du deuxième magnétomètre, et stocker les données dans la mémoire. 5
9. Système de surveillance basé sur un magnétomètre selon les revendications 1 à 8, dans lequel le premier magnétomètre et le deuxième magnétomètre sont agencés pour être en étroite proximité avec l'aimant dans le cache-oeil, les magnétomètres surveillant un champ magnétique, généré par l'aimant, la terre et des dispositifs magnétiques proches ; et le système de surveillance basé sur un magnétomètre comprenant en outre : 10
- une mémoire pour stocker des données en provenance du magnétomètre ;
et une liaison de communication pour obtenir les données en provenance de la mémoire, les données traitées pour montrer un schéma de port et de non-port du cache-oeil, pour surveiller la conformité à une prescription médicale. 15
- 25
10. Système de surveillance basé sur un magnétomètre selon la revendication 11, comprenant en outre :
le processeur comprenant un micro-contrôleur pour commander un minutage des mesures du champ magnétique, et le stockage des données. 30
11. Système de surveillance basé sur un magnétomètre selon la revendication 11, comprenant en outre :
une station de base pour recevoir des données en provenance du dispositif de journalisation, la station de base comprenant l'un parmi : un smartphone, une application informatique et un dispositif spécialisé. 35
12. Système de surveillance basé sur un magnétomètre selon la revendication 11, dans lequel le processeur est un processeur de données pour traiter les données en provenance du dispositif de journalisation, le processeur de données pour déterminer le schéma de port et non-port du cache-oeil, pour surveiller la conformité à une prescription médicale. 40
- 45
13. Système de surveillance basé sur un magnétomètre selon la revendication 12, comprenant en outre :
un système de communication pour informer un ou plusieurs parmi l'utilisateur, un professionnel médical et une partie désignée du schéma. 50
- 55

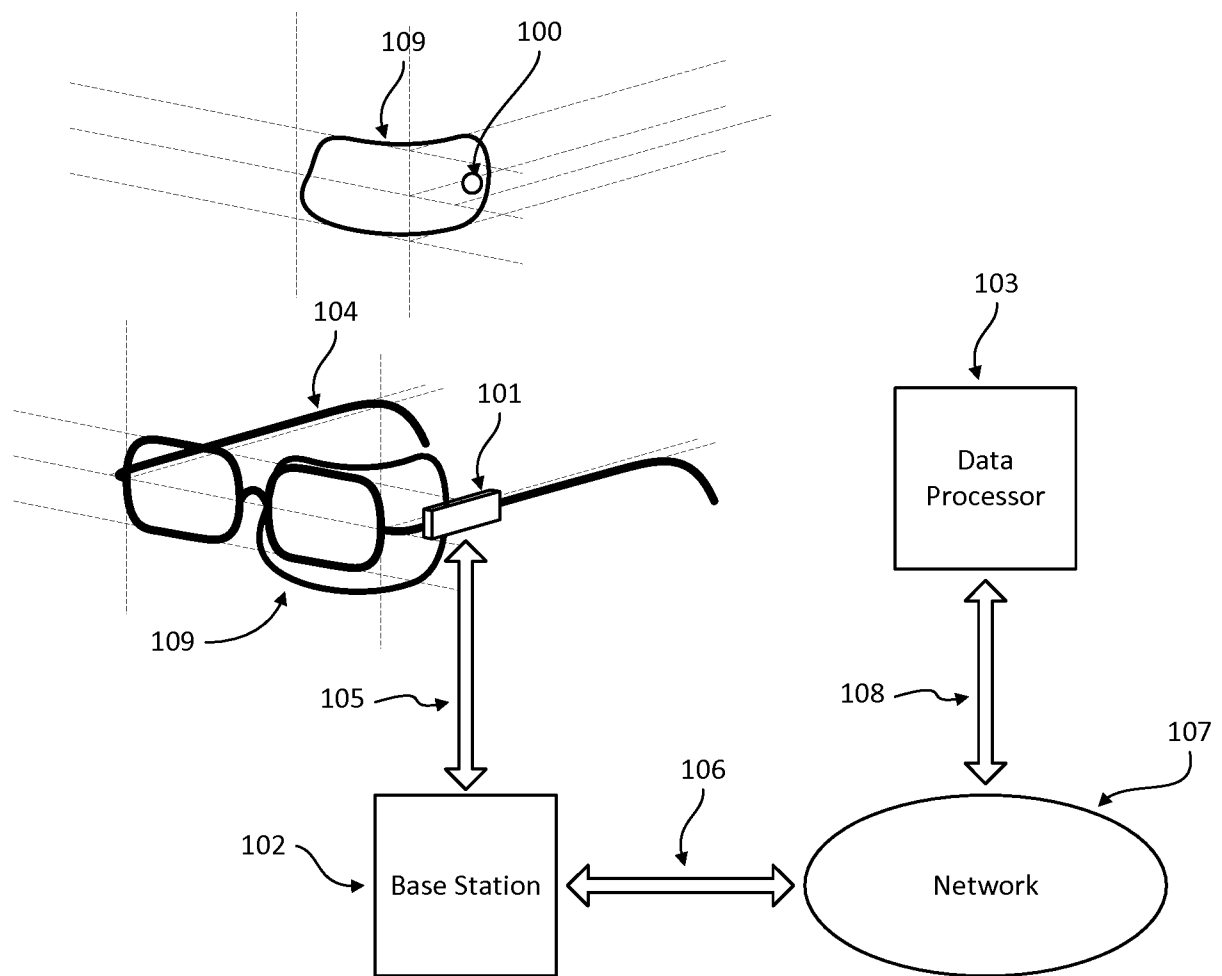


Fig. 1

Fig. 2A

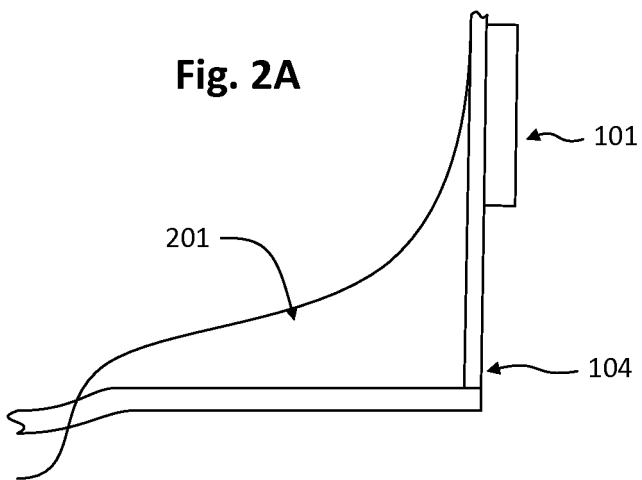


Fig. 2B




Fig. 2C

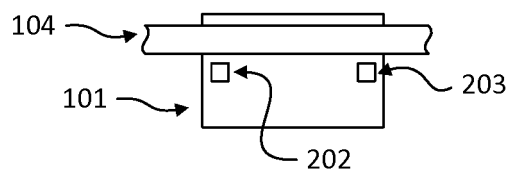
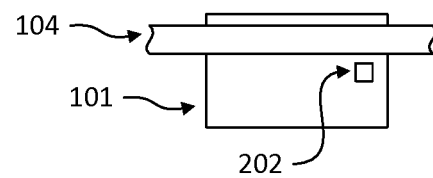


Fig. 2D



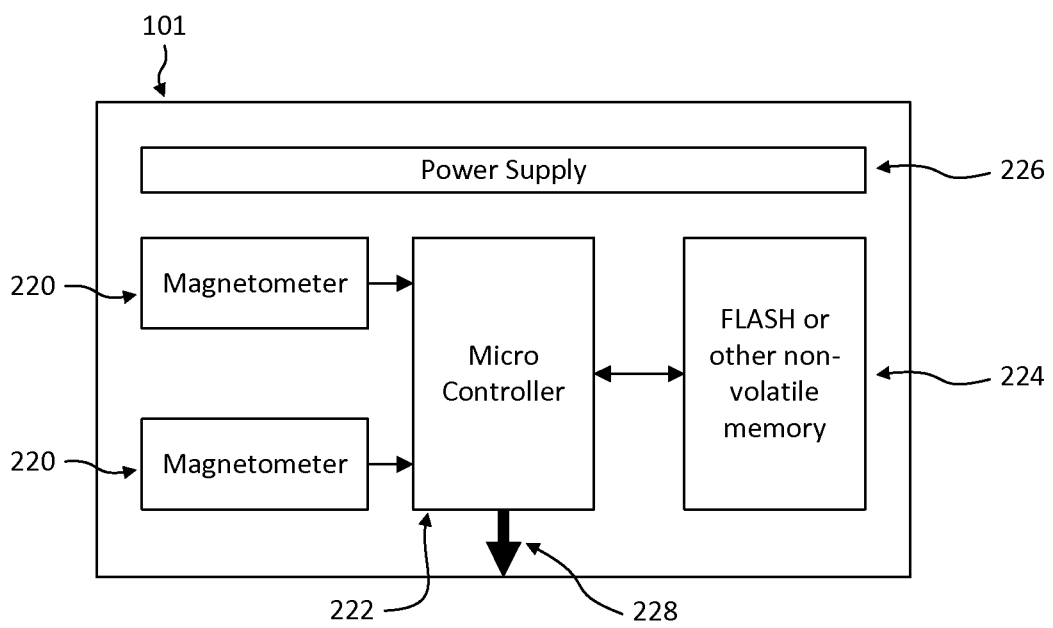


Fig. 2E

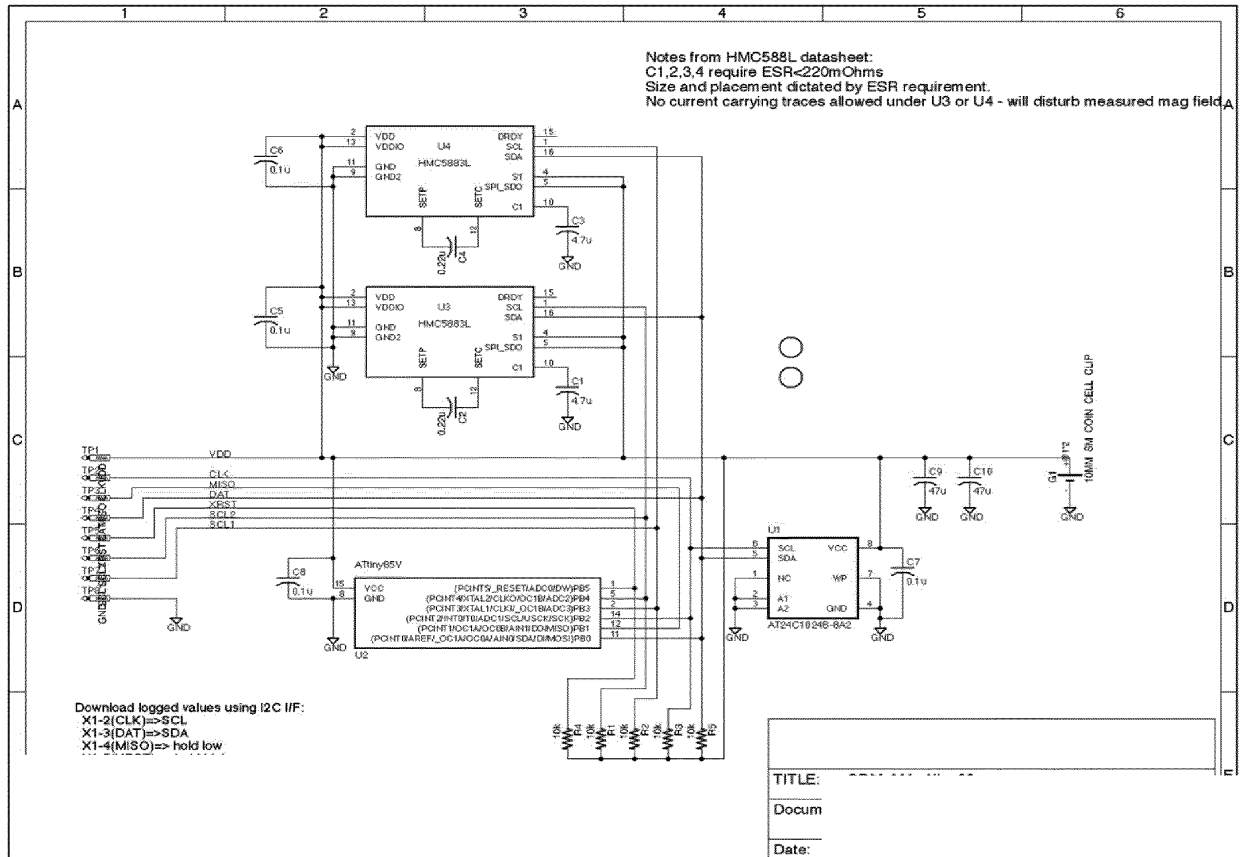
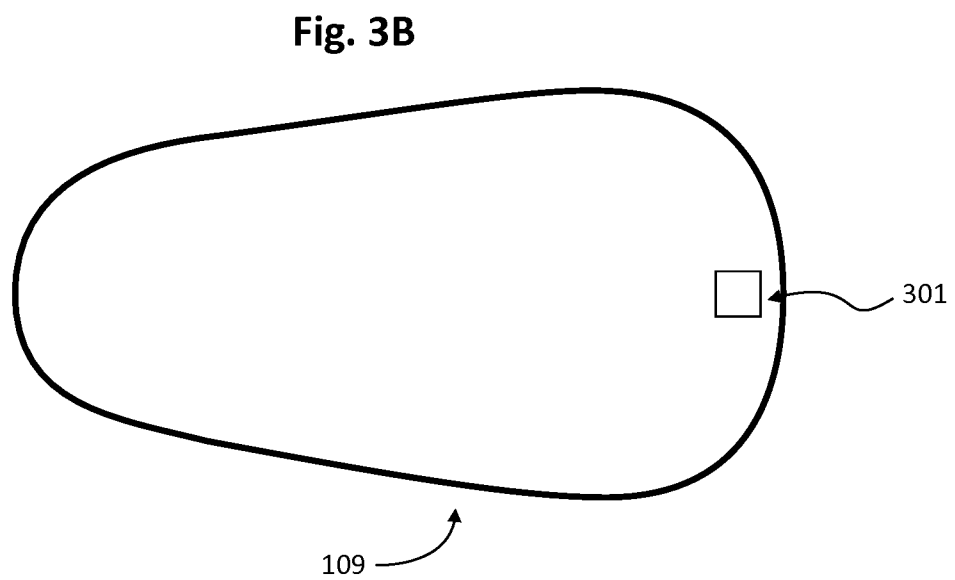
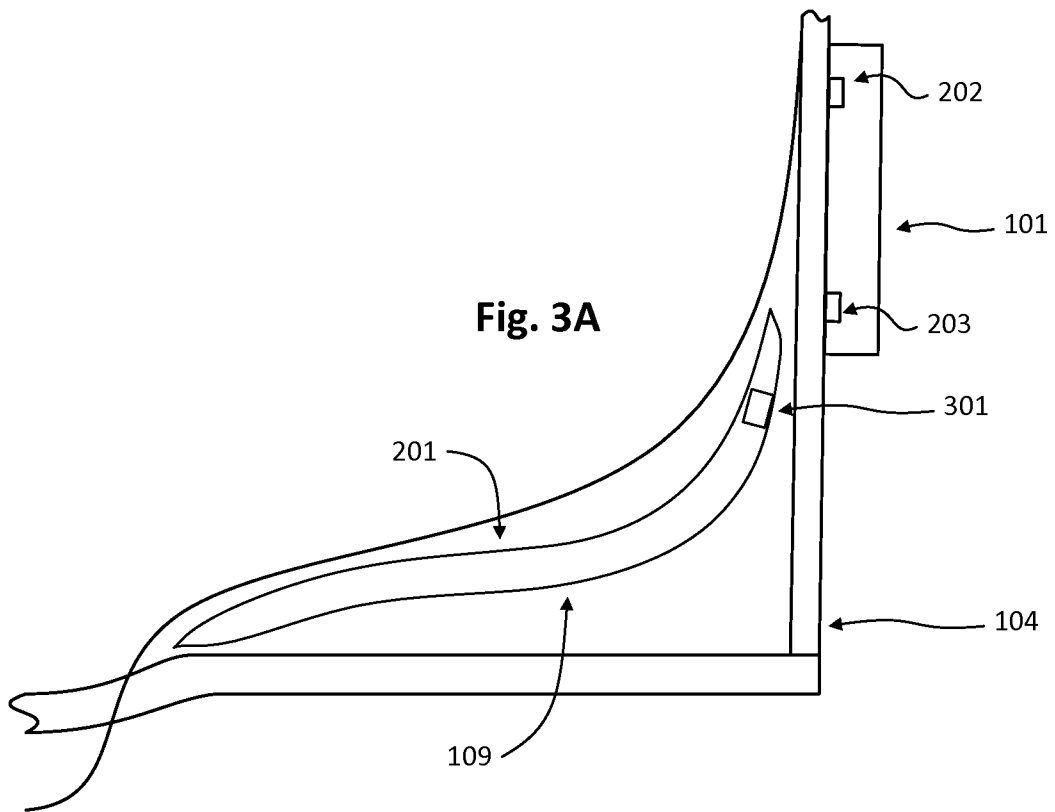
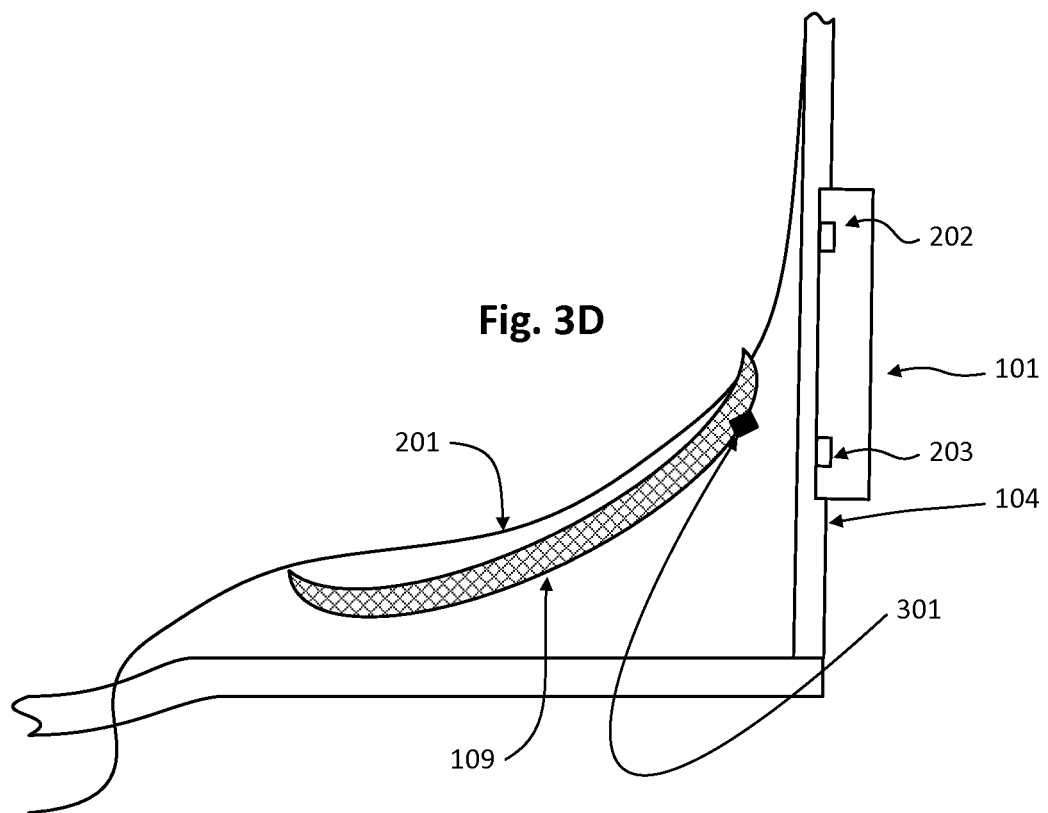
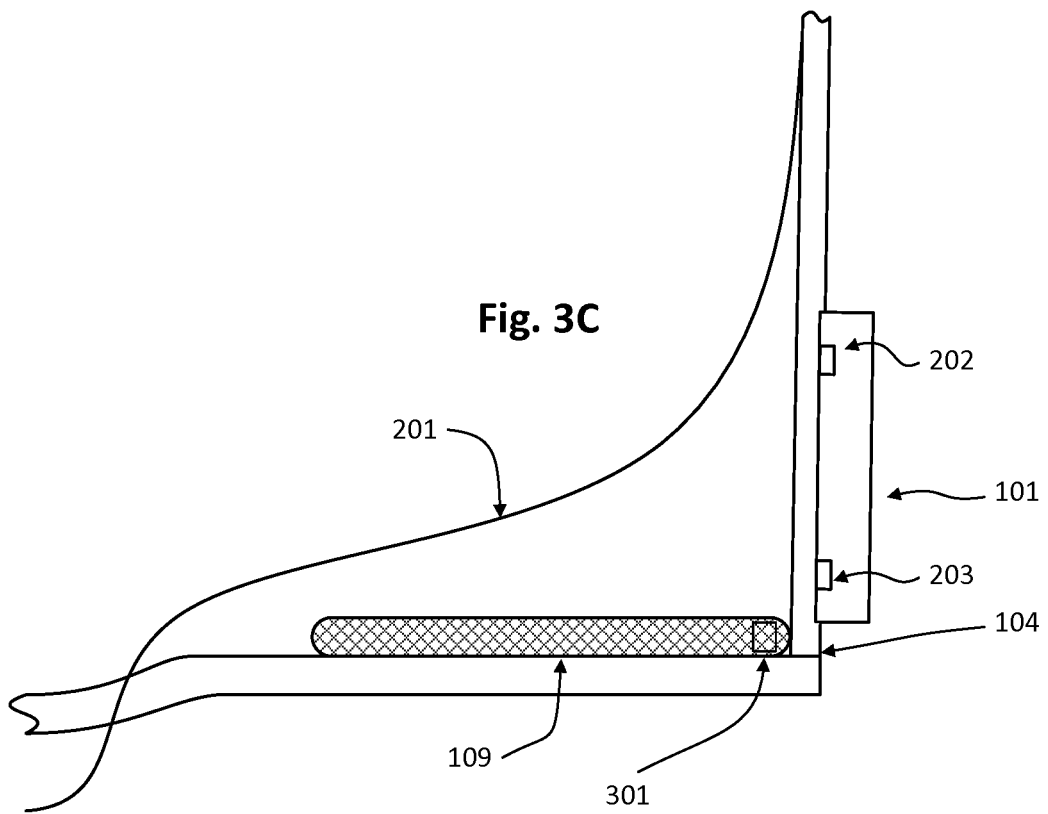


Fig. 2F





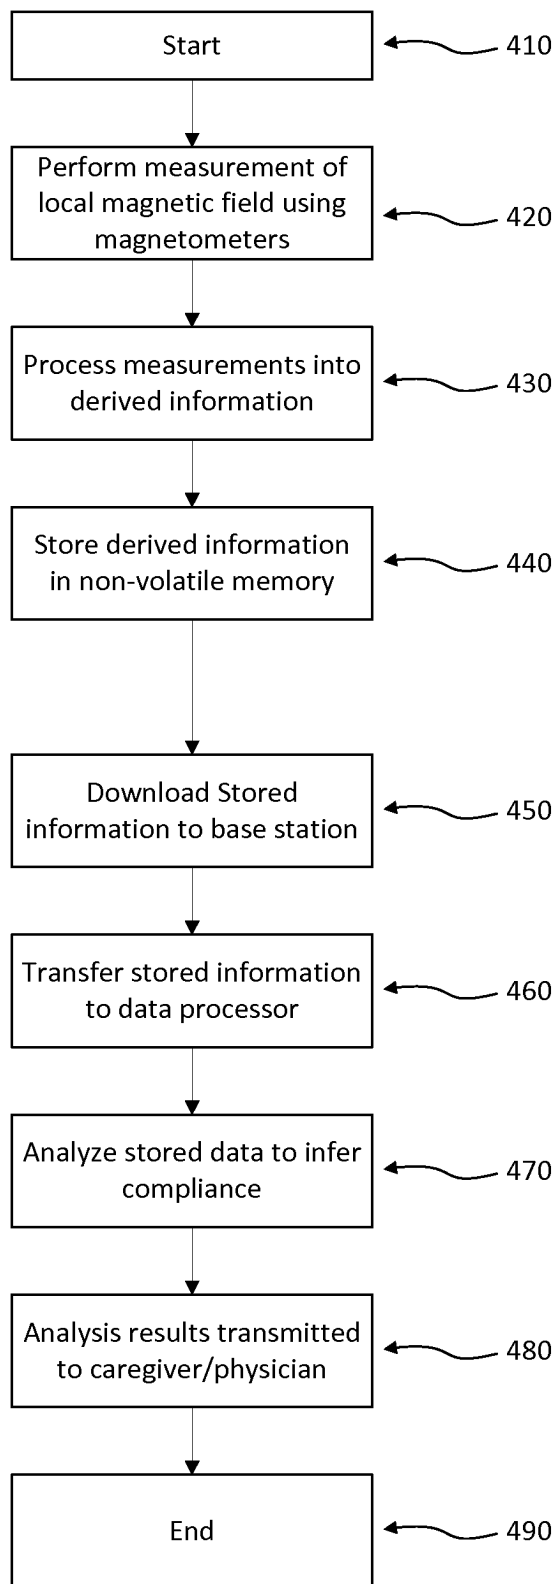
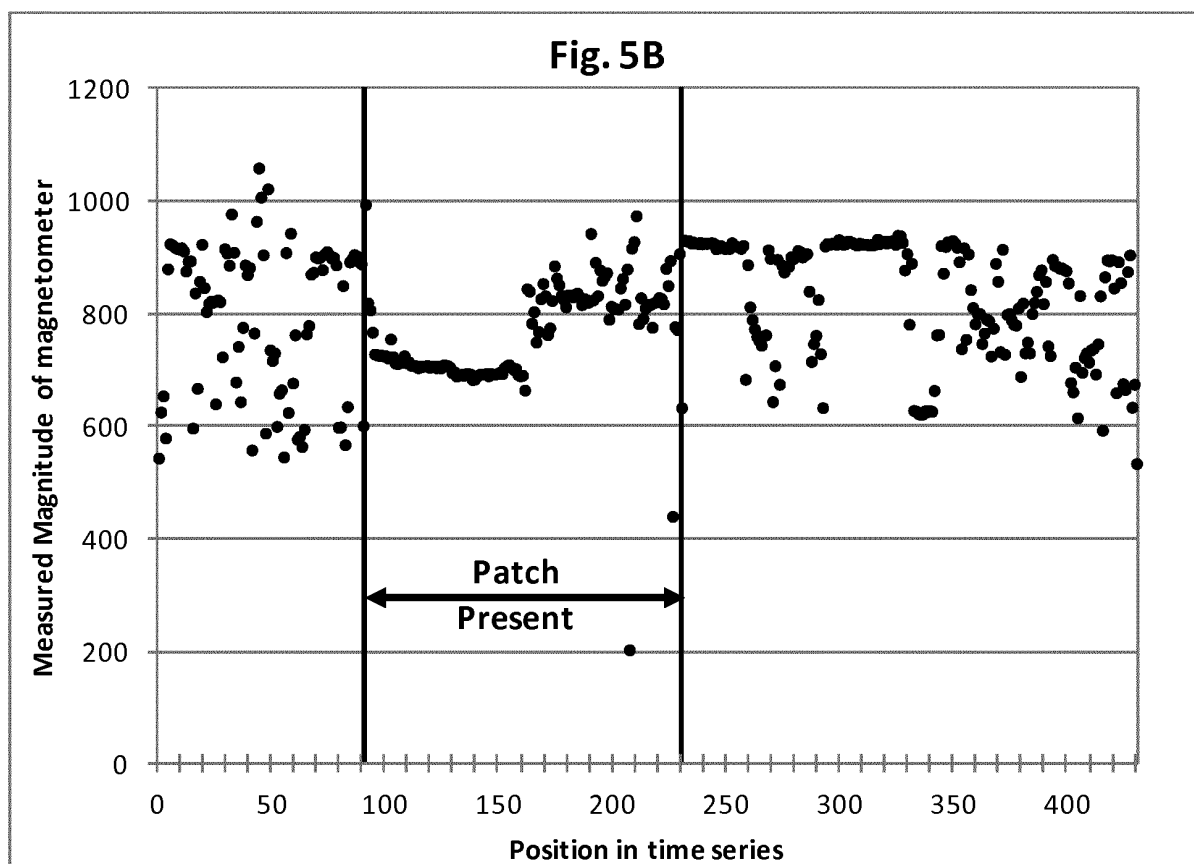
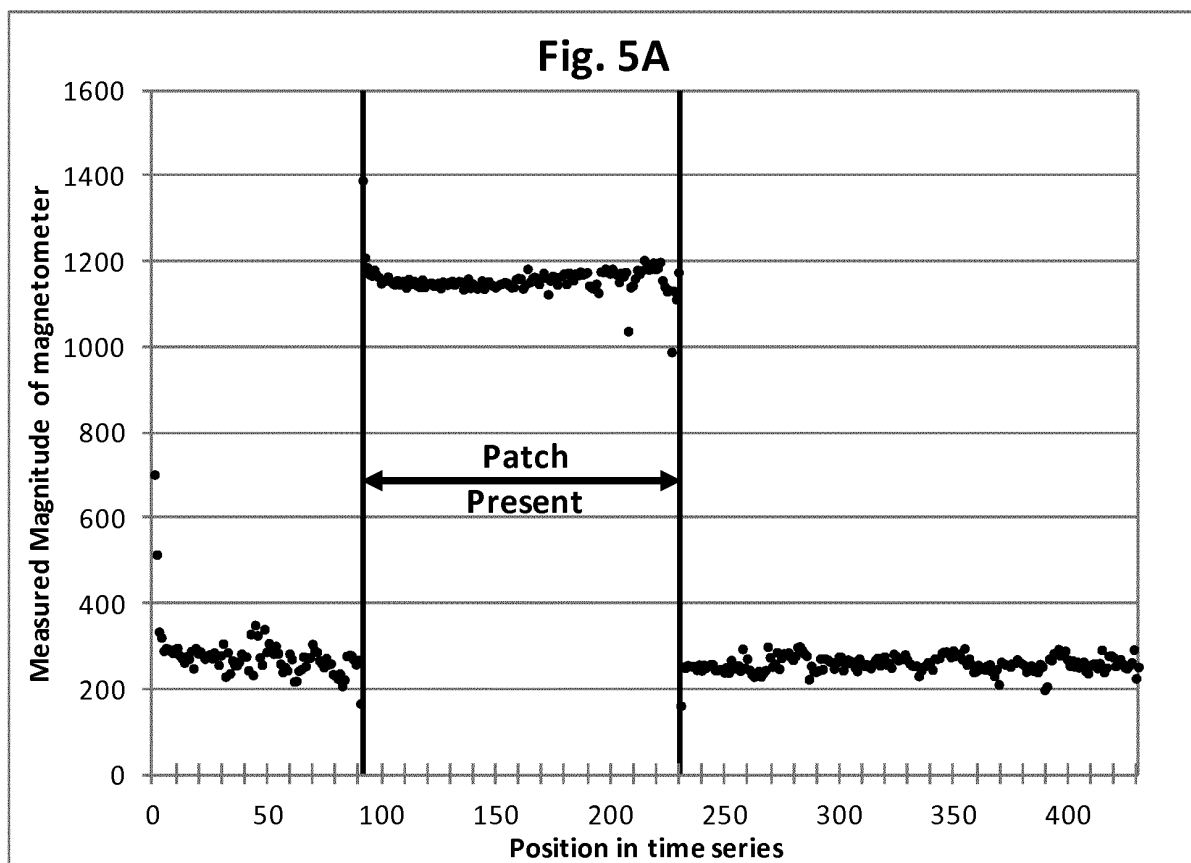


Fig. 4



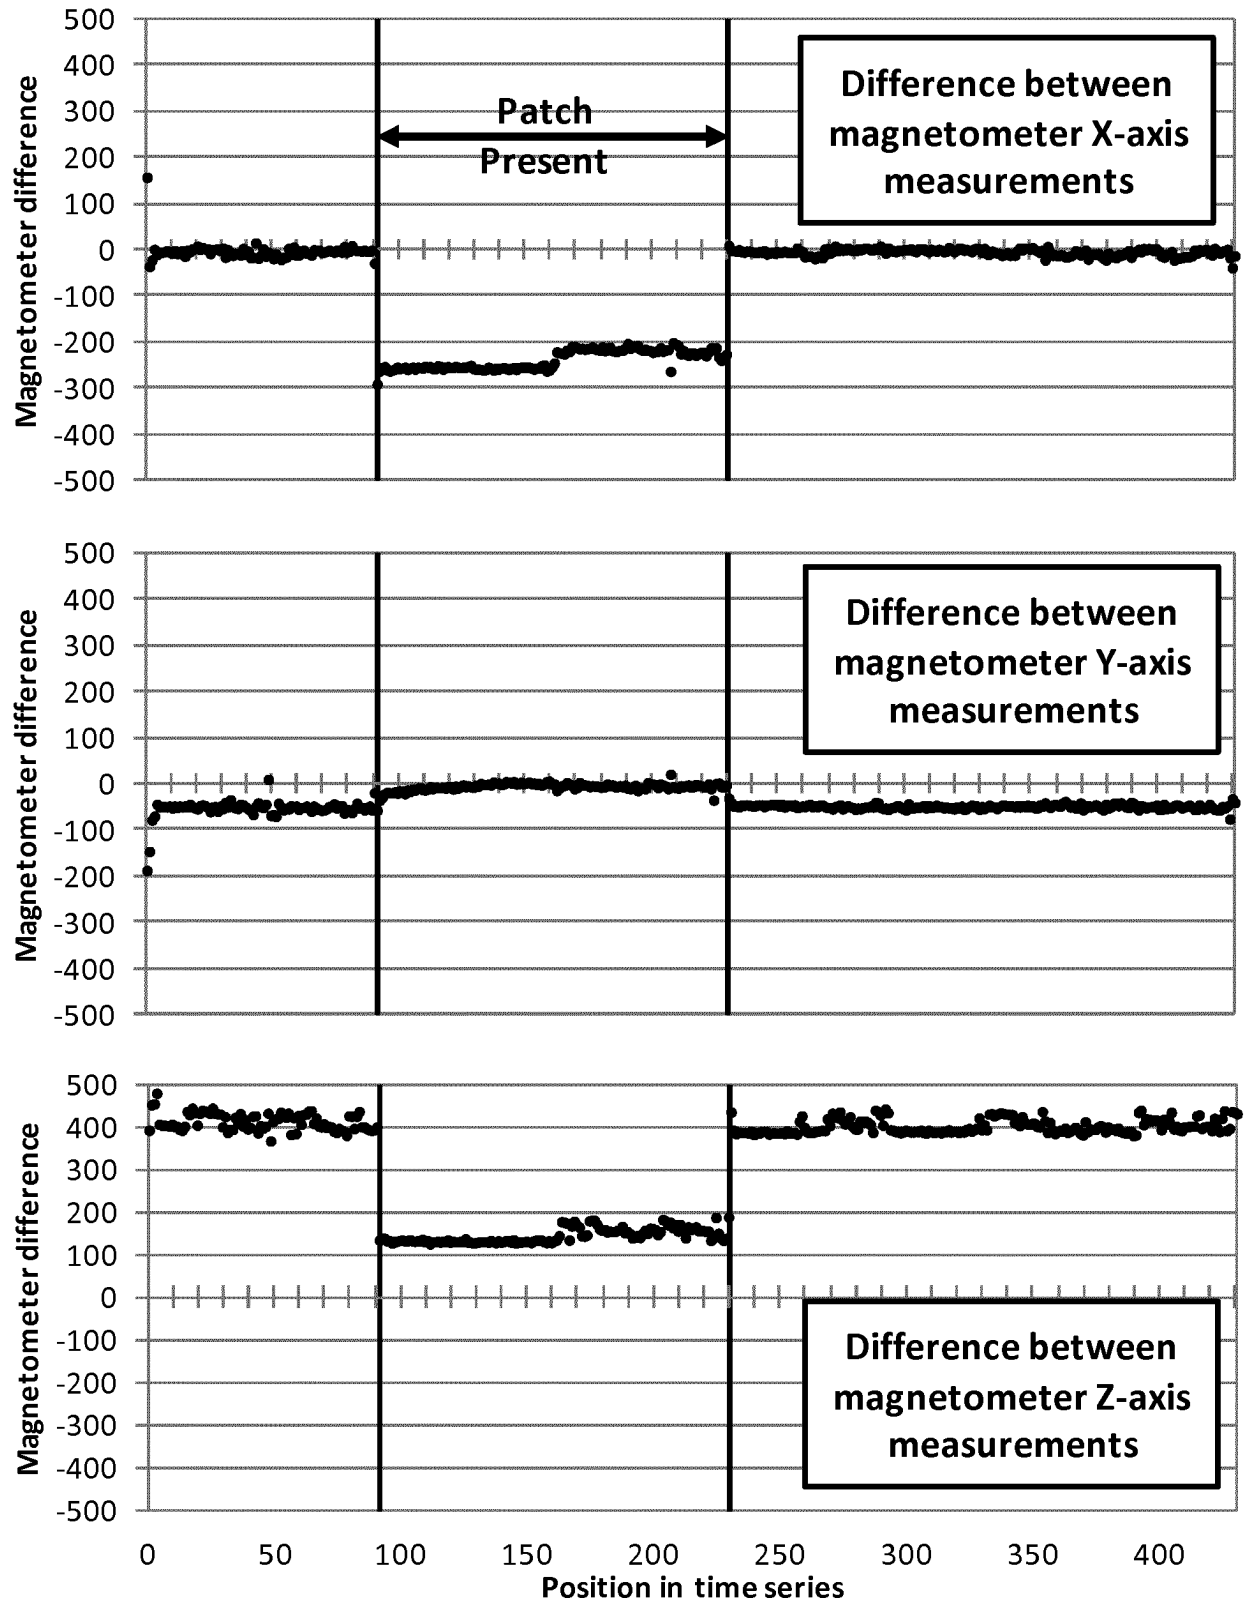


Fig. 5C

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Non-patent literature cited in the description

- **KAI JANUSCHOWSKI et al.** *the ophthalmologic journal of the nordic countries*, 01 December 2013, vol. 91 (8) [0005]
- **YAROSLAVA CHOPOVSKA.** *Electronic recording of occlusion treatment for amblyopia: potential of the new technology* [0005]
- *Graefe's Archive for clinical and experimental ophthalmology*, 01 June 2005, vol. 243 (6) [0005]

专利名称(译)	基于磁铁的监控系统		
公开(公告)号	EP3117764B1	公开(公告)日	2019-07-03
申请号	EP2016179579	申请日	2016-07-14
[标]申请(专利权)人(译)	雷迪标记 查特文杰瑞米 大号胆OMONDI		
申请(专利权)人(译)	雷迪, MARK A. 查特文, JEREMY G. Nyong'o, OMONDI L.		
[标]发明人	READDIE MARK A CHATWIN JEREMY G NYONGO OMONDI L		
发明人	READDIE, MARK A. CHATWIN, JEREMY G. NYONG'O, OMONDI L.		
IPC分类号	A61B5/00 A61B5/06 A61F13/12		
CPC分类号	A61B5/4833 A61B5/6803 A61B5/6821 A61B2562/0223 A61F9/04		
优先权	15/207879 2016-07-12 US 62/192062 2015-07-14 US		
其他公开文献	EP3117764A1		
外部链接	Espacenet		

摘要(译)

一种基于磁力计的监测系统，包括：磁体，其与待监测其布置的物体集成；第一磁力计，其固定在物体附近；以及第二磁力计，其固定在距离物体附近的第一磁力计的固定距离处。监视系统还包括处理器，用于从第一磁力计和第二磁力计接收数据，并计算测量矢量以确定物体的布置。

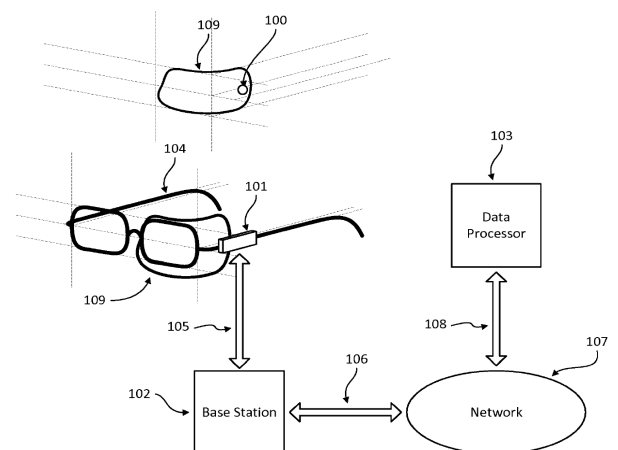


Fig. 1