

(19)



(11)

**EP 3 231 357 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**03.04.2019 Bulletin 2019/14**

(51) Int Cl.:  
**A61B 5/00** <sup>(2006.01)</sup> **A61B 5/0245** <sup>(2006.01)</sup>  
**A61B 5/0408** <sup>(2006.01)</sup>

(21) Application number: **17154739.1**

(22) Date of filing: **06.02.2017**

**(54) EMI PROTECTION FOR PHYSIOLOGICAL MEASUREMENTS**

EMI-SCHUTZ FÜR PHYSIOLOGISCHE MESSUNGEN

PROTECTION CONTRE LES INTERFÉRENCES ÉLECTROMAGNÉTIQUES POUR MESURES PHYSIOLOGIQUES

(84) Designated Contracting States:  
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR**

- **Lämsä, Kaisa**  
**90440 Kempele (FI)**
- **Pekonen, Elias**  
**90440 Kempele (FI)**

(43) Date of publication of application:  
**18.10.2017 Bulletin 2017/42**

(74) Representative: **Kolster Oy Ab**  
**(Salmisaarenaukio 1)**  
**P.O. Box 204**  
**00181 Helsinki (FI)**

(73) Proprietor: **Polar Electro Oy**  
**90440 Kempele (FI)**

(56) References cited:  
**EP-A1- 2 057 943 US-A- 4 478 225**  
**US-B1- 6 453 186**

(72) Inventors:  
 • **Korkala, Seppo**  
**90440 Kempele (FI)**

**EP 3 231 357 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

**Description**

## TECHNICAL FIELD

**[0001]** The present invention relates to a field of physiological or biometric measurements and, in particular, protecting a measurement component against electromagnetic interference.

## TECHNICAL BACKGROUND

**[0002]** Electrodes, signal lines and such components of a measurement circuitry are susceptible to electromagnetic interference (EMI). EMI typically corrupts a measurement signal such as an electrocardiogram or a bioimpedance signal and degrades measurement accuracy. Protection against EMI is advantageous.

**[0003]** EP 2 057 943 discloses a protective electrode structure that comprises a middle protective electrode which resides between an outer protective electrode and the skin electrodes during a measurement. The middle protective electrode and the outer protective electrode are insulated from each other. Additionally, the middle protective electrode may be coupled to a virtual ground of the user-specific performance monitor system.

## BRIEF DESCRIPTION

**[0004]** The present invention is defined by the subject matter of the independent claims.

**[0005]** Embodiments are defined in the dependent claims.

## BRIEF DESCRIPTION OF THE DRAWINGS

**[0006]** In the following the invention will be described in greater detail by means of preferred embodiments with reference to the attached [accompanying] drawings, in which

Figure 1 illustrates an apparel comprising a measurement circuitry;

Figures 2A and 2B illustrate an embodiment of shielding elements for providing electromagnetic interference (EMI) shielding for the measurement circuitry;

Figures 2C and 2D illustrate another configuration of the shielding elements of Figures 2A and 2B;

Figures 3A to 3D illustrate another embodiment of shielding elements for providing EMI shielding for the measurement circuitry;

Figures 3C and 3D illustrate another configuration of the shielding elements of Figures 3A and 3B;

Figure 4A and 4B illustrate an embodiment where the EMI shielding is formed by interlacing comb-shaped shielding elements;

Figures 4C and 4D illustrate another configuration of the shielding elements of Figures 4A and 4B;

Figures 5A and 5B illustrate an embodiment where the EMI shielding is formed by intertwining hook-shaped shielding elements;

Figures 5C and 5D illustrate another configuration of the shielding element of Figures 5A and 5B;

Figure 6 illustrates a perspective view of an embodiment of the comb-shaped shielding elements;

Figure 7 illustrates an embodiment where the EMI shielding elements form a mesh structure;

Figure 8 illustrates an embodiment where two layers of EMI shielding is provided;

Figure 9 illustrates an embodiment for providing EMI shielding for a signal line in the form of stitched EMI thread; and

Figure 10 illustrates a process for producing the EMI shielding of Figure 9 according to an embodiment of the invention.

## DETAILED DESCRIPTION OF THE INVENTION

**[0007]** The following embodiments are exemplifying. Although the specification may refer to "an", "one", or "some" embodiment(s) in several locations of the text, this does not necessarily mean that each reference is made to the same embodiment(s), or that a particular feature only applies to a single embodiment. Single features of different embodiments may also be combined to provide other embodiments.

**[0008]** Figure 1 illustrates an example of an apparatus to which embodiments of the invention may be applied. The apparatus may comprise a measurement circuitry or a part of a measurement circuitry configured to carry out electric physiological measurements such as measuring an electrocardiogram (ECG), electroencephalography (EMG), amperometry, bioimpedance. The apparatus may comprise a first layer comprising at least a first measurement electrode 102 and a second measurement electrode 104 disposed at a distance from one another, wherein the first measurement electrode 102 and second measurement electrode 104 are skin electrodes configured to measure an electric physiological property from a user's skin 120. The first layer is also denoted as an electrode layer in the description below. The first layer may be considered as a layer that is designed to contact the skin and it may form a bottom layer of the apparatus. Other layers may be provided on top of the first layer.

**[0009]** In an embodiment, the apparatus is or is comprised in an article of clothing, an apparel, or a garment such as a shirt 100. In another embodiment, the apparatus is or is comprised in a strap or another fixing structure that attaches the measurement electrodes 102, 104 to the skin.

**[0010]** The apparatus may further comprise a signal processing circuitry 110 provided in a casing. The signal processing circuitry 110 may be configured to process electric signals acquired from the skin by the electrodes 102, 104. The signal processing circuitry 110 may com-

prise a differential amplifier, a filter, an analog-to-digital (A/D) converter, and a digital signal processor. The casing may further house a wireless communication circuitry operating according to Bluetooth specifications, for example. The signal processing circuitry may use the wireless communication circuitry to wirelessly transmit processed measurement signals to another apparatus.

**[0011]** The apparatus may further comprise signal lines 106, 108 that connect the measurement electrodes 102, 104 to the signal processing circuitry 110. The signal processing circuitry 110 may be provided in a casing that has a shielding element against electromagnetic interference (EMI) radiating or induced from one or more sources outside the user's body. The measurement electrodes 102, 104 and the signal lines 106, 108 are, on the other hand, vulnerable to the EMI.

**[0012]** Embodiments of the invention provide the apparatus with a second layer 112 disposed on top of the first layer and comprising: a first shielding element which is electrically conductive and arranged to cover at least partially both the first measurement electrode 102 and second measurement electrode 104 so as to protect the first measurement electrode 102 and second measurement electrode 104 against the EMI, wherein the first shielding element is connected to a skin electrode; and a second shielding element which is electrically conductive, and arranged to cover at least partially both the first measurement electrode 102 and second measurement electrode 104 so as to protect the first measurement electrode 102 and second measurement electrode 104 against the EMI, wherein the second shielding element is connected to a skin electrode different from the skin electrode to which the first shielding element is connected. The first shielding element and the second shielding element extend adjacent with respect to one another between the first measurement electrode 102 and the second measurement electrode 104 on a plane defined by the second layer. The second shielding element is electrically isolated from the first shielding element.

**[0013]** By arranging each of the shielding elements to protect both measurement electrodes 102, 104 and in such a manner that shielding elements extend adjacent with respect to one another between measurement electrodes 102, 104 provides a technical effect where each shielding element absorbs EMI that affects each measurement electrode 102, 104 such that both shielding elements experience the same or similar EMI characteristics. In other words, the shielding elements absorb the EMI in a substantially similar manner. This reduces or eliminates a differential EMI component that could otherwise reach the signal processing circuitry 110. Common mode filtering employed by the signal processing circuitry 110 may then eliminate any residual EMI reaching the signal processing circuitry 110.

**[0014]** On the other hand, isolating the two shielding elements from one another eliminates differential interference components arising from poor or varying skin contacts between the skin electrodes and the skin. The

skin contact may vary during an exercise such as running, for example. Since each shielding element is "open-ended" when viewed from the skin electrode towards the shielding element, a signal modulated by electrical charges from the skin (a body potential) cannot cause a current through the shielding element and a differential interference component to the measurement electrodes.

**[0015]** In an embodiment, the skin electrodes ground the EMI absorbed by the shielding elements.

**[0016]** In an embodiment, the shielding elements are arranged at a proximity of both measurement electrodes. The proximity between the shielding element and the measurement electrodes may be defined such that the shielding element is provided so close to the measurement electrodes that it is capable of absorbing EMI that would otherwise be induced to the measurement electrodes. In some embodiments, the shielding element may be arranged on top of the measurement electrodes contrary to other examples where the shielding element may be arranged at the proximity with the measurement electrodes such that it is not on top of at least one of the measurement electrodes but still close enough to protect the at least one of the measurement electrodes against the EMI.

**[0017]** As disclosed in the embodiments below, the shielding elements extend adjacent with respect to one another between the first measurement electrode 102 and the second measurement electrode such that the shielding elements are arranged to extend in parallel at a section of the second layer that is between the measurement electrodes, when viewed from a top or bottom (see Figures 2A, 3A, 4A, 5A). From another perspective, the shielding elements extend adjacent with respect to one another between the first measurement electrode 102 and the second measurement electrode such that the shielding elements are arranged to extend in parallel at a section of the second layer that is between the measurement electrodes, when viewed from a source of the EMI. The source of the EMI is typically outside the user's skin and radiates EMI towards the user's skin to which the apparatus is positioned in use. In use, the first and second layer may be aligned with the skin. In such a case, the source of the EMI may be considered as a point that is at a distance from the plane formed by the skin as well as the first and second layer.

**[0018]** In some applications, it may not be necessary to arrange the shielding elements to extend as adjacent with respect to one another. For example, if the electrodes and the shielding elements are arranged in an apparel and the EMI characteristics are substantially similar in a large area of the apparel, e.g. on a front side of a shirt, the shielding elements may travel between the measurement electrodes via substantially different routes such that they do not extend as adjacent with respect to one another.

**[0019]** Let us now describe some embodiments for arranging the shielding elements. Figures 2A and 2B illustrate an embodiment where the shielding elements 200,

202 are each formed by a signal line forming a loop. The signal line 200 is connected to the measurement electrode 102 at both ends, and the signal line 202 is connected to the measurement electrode 104 at both ends. The signal line 200 may first extend vertically from the first measurement electrode 102 on the electrode layer 210 to the second layer now called an EMI layer 112 and then horizontally from a position of the first measurement electrode 102 towards the second measurement electrode 104. At a proximity of the second measurement electrode 104 in an example or above the second measurement electrode 104 in an embodiment, the signal line 200 takes a U-turn and extends back towards the first measurement electrode and, on top of the first measurement electrode 102, the signal line may extend vertically to connect to the first measurement electrode 102. In a similar manner, the signal line 202 may first extend vertically from the second measurement electrode 102 on the electrode layer 210 to the EMI layer 112 and then horizontally, adjacent to the signal line 200, from a position of the second measurement electrode 104 towards the first measurement electrode 102. At a proximity of the first measurement electrode 102 in an example or above the first measurement electrode 102 in an embodiment, the signal line 202 takes a U-turn and extends back towards the first measurement electrode and, on top of the first measurement electrode 102, the signal line 202 may extend vertically to connect to the second measurement electrode 104. In this embodiment, the signal lines 200, 202 extend to opposite directions on the same plane defined by the EMI layer 112 as adjacent to one another.

**[0020]** Figure 2B illustrates a side view of Figure 2A. A lining indicates an area where the signal lines 200, 202 overlap from this viewpoint. Figure 2B also illustrates how the signal lines 200, 202 extend vertically between the layers 210, 112 and connect to the respective measurement electrodes 102, 104.

**[0021]** In the embodiment of Figures 2A and 2B, the shielding elements 200, 202 are connected to the measurement electrodes 102, 104. Figures 2C and 2D illustrate an embodiment where the skin electrodes 220, 222 to which the shielding elements 200, 202 connect are other skin electrodes, e.g. grounding electrodes. In this embodiment, the measurement electrodes 102, 104 may be provided such that both shielding elements 200, 202 cover both measurement electrodes 102, 104. For example, the measurement electrodes 102, 104 may be provided between the grounding electrodes 220, 222. In another embodiment, the grounding electrodes 220, 222 are disposed between the measurement electrodes 102, 104, and the shielding elements 200, 202 may extend to over the grounding electrodes 220, 222 to cover the measurement electrodes at least partly. The grounding electrodes 220, 222 may be provided on the electrode layer 210.

**[0022]** Figures 3A to 3D illustrate an embodiment where the shielding elements are formed by open-ended

strips or signal lines extending from a skin electrode. Referring to Figures 3A and 3B, each shielding element 300, 302 may comprise a plurality of open-ended strips or signal lines extending from a respective measurement electrode 102, 104. The signal lines of the shielding element 300 may extend from the measurement electrode 102 and from the electrode layer 210 to the EMI layer 112 and then on the EMI layer 112 towards the second measurement electrode 104. The signal lines may extend to the proximity of the second measurement electrode 104 in an example or over the second measurement electrode 104 in an embodiment so as to protect both measurement electrodes against the EMI. Similarly, the signal lines of the shielding element 302 may extend from the measurement electrode 104 and from the electrode layer 210 to the EMI layer 112 and then on the EMI layer 112 towards the first measurement electrode 102. The signal lines may extend to the proximity of the first measurement electrode 102 in an example or over the first measurement electrode 102 in an embodiment so as to protect both measurement electrodes against the EMI.

**[0023]** In the embodiment of Figures 3A to 3D, the signal lines of the shielding elements 300, 302 are interlaced with respect to one another such that they are arranged in an alternating manner, as illustrated in the top/bottom view of Figure 3A. The signal lines may be provided in the same plane, as illustrated in the side view of Figure 3B.

**[0024]** Figures 3C and 3D illustrate an embodiment where the shielding elements 300, 302 are connected to the grounding electrodes 220, 222 other than the measurement electrodes 102, 104. In this embodiment, the measurement electrodes 102, 104 may be provided such that both shielding elements 300, 302 cover both measurement electrodes 102, 104. For example, the measurement electrodes 102, 104 may be provided between the grounding electrodes 220, 222. In another embodiment, the grounding electrodes 220, 222 are disposed between the measurement electrodes 102, 104, and the shielding elements 300, 302 may extend to over the grounding electrodes 220, 222 to cover the measurement electrodes at least partly. The grounding electrodes 220, 222 may be provided on the electrode layer 210.

**[0025]** In the embodiment of Figures 3A to 3D, the shielding elements are formed by straight signal lines. In another embodiment, the signal lines may form curves or a pattern other than an assembly of straight lines. Each signal line may form a uniform curve.

**[0026]** Figures 4A to 4D illustrate an embodiment where the shielding elements 400, 402 have a comb-shape. Referring to Figures 4A and 4B, a shielding element 400 may connect to the measurement electrode 102 and have a base line that extends from the measurement electrode 102 to the EMI layer 112 and on the EMI layer 112 towards the measurement electrode 104. The base line may extend to the proximity of the measurement electrode 104 in an example or over the measurement electrode 104 in an embodiment to cover the

measurement electrode 104. Comb peaks may extend from the base line as perpendicular to the base line and on the plane defined by the EMI layer 112, as illustrated in the top/bottom view of Figure 4A. In a similar manner, a shielding element 402 may connect to the measurement electrode 104 and have a base line that extends from the measurement electrode 104 to the EMI layer 112 and on the EMI layer 112 towards the measurement electrode 102. The base line may extend to the proximity of the measurement electrode 102 in an example or over the measurement electrode 102 in an embodiment to cover the measurement electrode 102. Comb peaks may extend from the base line as perpendicular to the base line and on the plane defined by the EMI layer 112, as illustrated in the top/bottom view of Figure 4A.

**[0027]** The comb peaks of the shielding element 400 may extend towards the base line of the shielding element 402, and the comb peaks of the shielding element 400 may extend towards the base line of the shielding element 402, as illustrated in Figure 4A. The comb peaks and the base lines of the shielding elements may extend in the same plane defined by the EMI layer 112, as illustrated in the side view of Figure 4B.

**[0028]** In the embodiment of Figures 4A to 4D, the comb peaks of the shielding elements 400, 402 are interlaced with respect to one another such that they are arranged in an alternating manner, as illustrated in the top/bottom view of Figure 4A. In other words, the combs may be facing one another at such proximity that comb peaks of one shielding element are provided between comb peaks of another shielding element.

**[0029]** In the embodiment of Figures 4A to 4D, the comb peaks extend perpendicularly from the base line, i.e. the angle between the comb peaks and the base line is 90 degrees. In another embodiment, the angle may be another, e.g. 45 degrees, 135 degrees, or at any angle between 10 and 170 degrees. In an embodiment, the angle may be the same for both shielding elements to enable the interlacing efficiently. In another embodiment, the angles of the peaks with respect to the base lines may be different for the shielding elements 400, 402, and the interlacing may still be achieved, if the spacing between the peaks is sufficiently large. In general, the angle(s) may be arbitrary as long as the comb peaks of the different shielding elements 400, 402 can be interlaced.

**[0030]** Figures 4C and 4D illustrate an embodiment where the shielding elements 400, 402 are connected to the grounding electrodes 220, 222 other than the measurement electrodes 102, 104. In this embodiment, the measurement electrodes 102, 104 may be provided such that both shielding elements 400, 402 cover both measurement electrodes 102, 104. For example, the measurement electrodes 102, 104 may be provided between the grounding electrodes 220, 222. In another embodiment, the grounding electrodes 220, 222 are disposed between the measurement electrodes 102, 104, and the shielding elements 400, 402 may extend to over the grounding electrodes 220, 222 to cover the measurement

electrodes at least partly. The grounding electrodes 220, 222 may be provided on the electrode layer 210.

**[0031]** In the embodiments of Figures 2A to 4D, the shielding elements are disposed symmetrically with respect to one another such that the axis of symmetry is an axis that extends between the shielding elements and between the skin electrodes, when viewed from the top/bottom.

**[0032]** Figures 5A to 5D illustrate an embodiment where the shielding elements 400, 402 have a hook-shape. Referring to Figures 5A and 5B, a shielding element 500 may connect to the measurement electrode 102 and have a base line that extends from the measurement electrode 102 to the EMI layer 112 and on the EMI layer 112 towards the measurement electrode 104. The base line may extend to the proximity of the measurement electrode 104 in an example or over the measurement electrode 104 in an embodiment to cover the measurement electrode 104. Hook-shaped signal lines may extend from the base line on the plane defined by the EMI layer 112, as illustrated in the top/bottom view of Figure 4A. In a similar manner, a shielding element 502 may connect to the measurement electrode 104 and have a base line that extends from the measurement electrode 104 to the EMI layer 112 and on the EMI layer 112 towards the measurement electrode 102. The base line may extend to the proximity of the measurement electrode 102 in an example or over the measurement electrode 102 in an embodiment to cover the measurement electrode 102. Hook-shaped signal lines may extend from the base line on the plane defined by the EMI layer 112, as illustrated in the top/bottom view of Figure 5A.

**[0033]** The hooks of the shielding element 500 may extend towards the base line of the shielding element 502, and the hooks of the shielding element 502 may extend towards the base line of the shielding element 500. The hooks of the shielding element 500 may intertwine with hooks of the shielding element 502 without connecting one another, as illustrated in Figure 5A. The shielding elements 500, 502 may have the same form and the same dimensions, and they may be arranged such that the hooks intertwine in the illustrated manner.

**[0034]** Figures 5C and 5D illustrate an embodiment where the shielding elements 500, 502 are connected to the grounding electrodes 220, 222 other than the measurement electrodes 102, 104. In this embodiment, the measurement electrodes 102, 104 may be provided such that both shielding elements 500, 502 cover both measurement electrodes 102, 104. For example, the measurement electrodes 102, 104 may be provided between the grounding electrodes 220, 222. In another embodiment, the grounding electrodes 220, 222 are disposed between the measurement electrodes 102, 104, and the shielding elements 500, 502 may extend to over the grounding electrodes 220, 222 to cover the measurement electrodes at least partly. The grounding electrodes 220, 222 may be provided on the electrode layer 210.

**[0035]** Let us now elaborate the positioning of the

shielding elements of the above-described embodiments on a general level with reference to Figure 6. Figure 6 illustrates a perspective view of the embodiment of Figure 4A and 4B where the comb-shaped shielding elements extend to cover the measurement electrodes 102, 104. The shielding elements may be connected to the measurement electrodes 102, 104 through signal lines 106, 108 that connect the measurement electrodes 102, 104 to the signal processing circuitry 110, for example. As illustrated in Figure 6, the electrode layer 210 comprising the measurement electrodes 102, 104 defines a first plane 602 that substantially conforms with the skin when the apparatus is in use and attached to the user. On top of the first plane, the EMI layer 112 comprising the shielding elements defines a second plane 600 that substantially conforms to the first plane and, the skin when the apparatus is in use.

**[0036]** In the embodiments of Figures 2A to 3D, the shielding elements are configured to extend as adjacent with respect to one another in only one dimension of the second plane 600.

**[0037]** In the embodiments of Figures 4A to 5D, the shielding elements are configured to extend as adjacent with respect to one another in two dimensions of the second plane 600.

**[0038]** In the embodiment of Figure 7, the EMI layer 112 is a mesh layer 700 where the shielding elements are configured to intertwine in three dimensions to form a mesh structure. As in other embodiments, the shielding elements may be isolated from one another and connect to different electrodes, e.g. the measurement electrodes 102, 104 or the grounding electrodes 220, 222.

**[0039]** In an embodiment, an electromagnetic absorption area covered by the first shielding element towards a source of the electromagnetic interference is substantially equal to an electromagnetic absorption area covered by the second shielding element towards a source of the electromagnetic interference. This provides a technical effect that the shielding elements are capable of absorbing a substantially equal amount of EMI, thus reducing differential mode interference.

**[0040]** In an embodiment, the first shielding element is arranged in a symmetric manner with respect to the second shielding element. In an embodiment, the first shielding element extends from a position (on top) of the first measurement electrode towards the second measurement electrode in an identical manner as the second shielding element extends from a position (on top) of the second measurement electrode towards the first measurement electrode.

**[0041]** In general, the shielding elements may be arranged to protect the measurement electrodes 102, 104 such that they both experience a substantially identical electromagnetic interference field. This may be achieved by arranging the shielding elements to extend as adjacent to one another, providing the shielding elements with the same absorption area towards the source of the EMI, and/or arranging the shielding elements in a symmetric

manner.

**[0042]** In all embodiment described above, the number of shielding elements is two but the number of shielding elements may be higher than two, and the number of shielding elements may be computed as how many shielding elements are isolated from one another.

**[0043]** Figure 8 illustrates an embodiment which combines the embodiments of Figures 4A/B and 4C/D. As illustrated in Figure 8, the EMI layer 112 may comprise at least two sub-layers, each sub-layer comprising an EMI shield provided by at least two shielding elements. Referring to Figure 8, a first sub-layer may be provided on top of the electrode layer 210 and it may comprise a first shielding element 806 which is electrically conductive and arranged at a proximity of both the first measurement electrode 102 and second measurement electrode 104 so as to protect the first measurement electrode 102 and second measurement electrode 104 against electromagnetic interference, wherein the first shielding element is connected to a skin electrode (the measurement electrode 104 in this example). The first sub-layer may further comprise a second shielding element 808 which is electrically conductive, and arranged at a proximity of both the first measurement electrode 102 and second measurement electrode 104 so as to protect the first measurement electrode 102 and second measurement electrode 104 against the electromagnetic interference, wherein the second shielding element is connected to a skin electrode different from the skin electrode to which the first shielding element is connected (the measurement electrode 102 in this example). The first and second shielding element extend adjacent with respect to one another between the measurement electrodes 102, 104 on a plane defined by the first sub-layer.

**[0044]** On top of the first sub-layer, there is provided a second sub-layer that comprises a third shielding element 800 which is electrically conductive and arranged at a proximity of both the first measurement electrode 102 and second measurement electrode 104 so as to protect the first measurement electrode 102 and second measurement electrode 104 against electromagnetic interference, wherein the third shielding element is connected to a skin electrode (the grounding electrode 220 in this example). The second sub-layer may further comprise a fourth shielding element 802 which is electrically conductive, and arranged at a proximity of both the first measurement electrode 102 and second measurement electrode 104 so as to protect the first measurement electrode 102 and second measurement electrode 104 against the electromagnetic interference, wherein the fourth shielding element is connected to a skin electrode different from the skin electrodes to which the other shielding elements are connected (the grounding electrode 222 in this example). The third and fourth shielding element 800, 802 extend adjacent with respect to one another between the measurement electrodes 102, 104 on a plane defined by the second sub-layer on top of the plane defined by the first sub-layer.

**[0045]** Figure 8 illustrates an embodiment where the shielding elements 800 to 808 have the comb-shaped form, but the shape of the shielding elements may be any one of the other embodiments described herein, e.g. any one of Figures 2A, 3A, and 5A, or another shape.

**[0046]** In another embodiment, the shielding elements 806, 808 are connected to the respective grounding electrodes 220, 222 while the shielding elements 800, 802 are connected to the respective measurement electrodes 102, 104. In another embodiment, all the shielding elements 800 to 808 are connected to different grounding electrodes.

**[0047]** In an embodiment, a substrate layer may be provided between the electrode layer and the EMI layer. The electrodes may be attached to the substrate on a side that contacts the skin, and the EMI layer may be provided on an opposite side of the substrate. The substrate layer may be a textile layer, for example.

**[0048]** In the embodiments described above, the shielding elements may be produced by using one of the following techniques: conductive threading stitched or sewn on top of the electrode layer, conductive fabric weaved on top of the electrode layer, conductive plastic attached on top of the electrode layer, conductive ink printed on top of the electrode layer, or printed electronics printed on top of the electrode layer.

**[0049]** Figures 9 and 10 relate to embodiments where the EMI shielding is provided for the signal lines 106, 108 of the apparatus. The apparatus according to these embodiments may thus comprise any signal lines that conduct electric signals and are susceptible to the EMI. Referring to Figure 9, the signal line 106 may comprise an electric conductor that may be formed by an electrically conductive thread or threading in an article of clothing, an apparel or a garment. The electric conductor may be isolated by an isolation layer 900 protecting the electric conductor and isolating the electric conductor. On top of the electric conductor, the EMI shielding may be provided by arranging a conductive threading to cover the electric conductor. The conductive threading may be arranged on top of the electric conductor by stitching or sewing the conductive threading with a sewing machine. The conductive threading may be formed by using zigzag stitching such that the zigzag pattern covers the signal line without penetrating the isolation layer 900. The conductive threading may be sewn through a substrate in which the signal line 106 is provided, e.g. a textile or a garment. When used in an application where the substrate is in contact with the user's skin, the conductive threading thus engages the user's skin and operates as a skin electrode for grounding the EMI.

**[0050]** Figure 9 illustrates both a top view and a side view of the threading. The top view illustrates that both the threading 902 on top of the substrate and a bobbin threading 904 form the zigzag pattern, the top threading travelling in parallel and on top of the bobbin threading. The side view illustrates how the two threadings 902, 904 intertwine through the substrate and around the signal

line 902.

**[0051]** In an embodiment, only the threading 902 forming a pattern on top of the substrate in the sewing process is conductive. In an embodiment, all threading included in the sewing process is conductive, including bobbin threading 904. Accordingly, the threadings 902, 904 together surround the signal line, thus shielding the signal line against the EMI from all directions. The conductive threadings 902, 904 may form a caging such as a Faraday cage for the signal line 106. In such an embodiment, stitches of the threadings 902, 904 may or ground to or contact with the user's skin in use. In an embodiment where the garment comprising the signal line and the stitched threadings 902, 904 is not arranged to contact the user's skin, separate grounding points may be arranged to ground the conductive threading(s) 902, 904.

**[0052]** Figure 10 illustrates a process for producing the EMI shielding of Figure 9 described above. Referring to Figure 10, the process comprises arranging at least one insulated conductive threading as a signal line in an apparel (block 1000). In block 1002, another conductive threading is stitched or sewn over the insulated signal lines to form the EMI shielding. By using the conductive threading stitched over the signal line, the EMI shielding may be provided in an inconspicuous manner and still produced by using conventional means used in textile industry. No separate industrial process is required to generate the EMI layer on top of the signal line.

**[0053]** It will be obvious to a person skilled in the art that, as the technology advances, the inventive concept can be implemented in various ways. The invention and its embodiments are not limited to the examples described above but may vary within the scope of the claims.

## Claims

### 1. An apparatus comprising:

a first layer (210) comprising at least a first measurement electrode (102) and a second measurement electrode (104) disposed at a distance from one another, wherein the first measurement electrode and second measurement electrode are skin electrodes configured to measure an electric physiological property from a skin; a second layer (112) disposed on top of the first layer and comprising:

a first shielding element (200, 300, 400, 500) which is electrically conductive and arranged to cover at least partially both the first measurement electrode and second measurement electrode so as to protect the first measurement electrode and second measurement electrode against electromagnetic interference, wherein the first

shielding element is connected to a skin electrode (102, 220); and a second shielding element (202, 302, 402, 502) which is electrically conductive, and arranged to cover at least partially both the first measurement electrode and second measurement electrode so as to protect the first measurement electrode and second measurement electrode against electromagnetic interference, wherein the second shielding element is connected to a skin electrode (104, 222) different from the skin electrode to which the first shielding element is connected,

**characterized in that** the first shielding element and the second shielding element extend adjacent with respect to one another between the first measurement electrode and the second measurement electrode on a plane defined by the second layer, and wherein the second shielding element is electrically isolated from the first shielding element.

2. The apparatus of claim 1, wherein the first shielding element and second shielding element are configured to extend as adjacent with respect to one another in only one dimension of the plane.
3. The apparatus of claim 1, wherein the first shielding element and second shielding element are configured to extend as adjacent with respect to one another in two dimensions of the plane.
4. The apparatus of claim 1 or 3, wherein the second layer is a mesh layer (700) where the first shielding element and second shielding element are configured to intertwine in three dimensions.
5. The apparatus of claim 1 or 3, wherein each of the first shielding element (400) and the second shielding element (402) forms a comb structure where comb peaks of the different shielding elements are interlaced.
6. The apparatus of any preceding claim, wherein an electromagnetic absorption area covered by the first shielding element towards a source of the electromagnetic interference is substantially equal to an electromagnetic absorption area covered by the second shielding element towards a source of the electromagnetic interference.
7. The apparatus of any preceding claim, wherein the first shielding element is arranged in a symmetric manner with respect to the second shielding element.
8. The apparatus of claim 7, wherein the first shielding element extends from a position of the first measurement electrode towards the second measurement electrode in an identical manner as the second shielding element extends from a position of the second measurement electrode towards the first measurement electrode.
9. The apparatus of any preceding claim, wherein the first shielding element and the second shielding element are arranged such that they both experience a substantially identical electromagnetic interference field.
10. The apparatus of any preceding claim, wherein each of the first shielding element and the second shielding element is connected to a skin electrode (220, 222) that is not a measurement electrode.
11. The apparatus of any preceding claim 1 to 9, wherein the first shielding element is connected to the first measurement electrode and the second shielding element is connected to the second measurement electrode.
12. The apparatus of any preceding claim, further comprising a third layer disposed on top of the second layer or between the first layer and the second layer, comprising:
  - a third shielding element which is electrically conductive and arranged at a proximity of both the first measurement electrode and second measurement electrode so as to protect the first measurement electrode and second measurement electrode against electromagnetic interference, wherein the third shielding element is connected to a skin electrode; and
  - a fourth shielding element which is electrically conductive, and arranged at a proximity of both the first measurement electrode and second measurement electrode so as to protect the first measurement electrode and second measurement electrode against electromagnetic interference, wherein the fourth shielding element is connected to a skin electrode different from the skin electrode to which the third shielding element is connected, wherein the third shielding element and the fourth shielding element extend adjacent with respect to one another between the first measurement electrode and the second measurement electrode on a plane defined by the second layer, and wherein all the shielding elements are electrically isolated from one another.
13. The apparatus of claim 12, wherein the first shielding element is connected to the first measurement elec-

trode and the second shielding element is connected to the second measurement electrode, and each of the third shielding element and the fourth shielding element is connected to a skin electrode that is not a measurement electrode.

14. The apparatus of any preceding claim, wherein the apparatus is an article of clothing.

#### Patentansprüche

1. Vorrichtung, die umfasst:

eine erste Schicht (210), die wenigstens eine erste Mess-Elektrode (102) und eine zweite Mess-Elektrode (104) umfasst, die in einem Abstand zueinander angeordnet sind, wobei die erste Mess-Elektrode und die zweite Mess-Elektrode Haut-Elektroden sind, die zum Messen einer elektrischen physiologischen Eigenschaft einer Haut eingerichtet sind;  
eine zweite Schicht (112), die über der ersten Schicht angeordnet ist und umfasst:

ein erstes Abschirm-Element (200, 300, 400, 500), das elektrisch leitend ist und so angeordnet ist, dass es sowohl die erste Mess-Elektrode als auch die zweite Mess-Elektrode wenigstens teilweise abdeckt, um die erste Mess-Elektrode und die zweite Mess-Elektrode vor elektromagnetischer Interferenz zu schützen, wobei das erste Abschirm-Element mit einer Haut-Elektrode (102, 220) verbunden ist; sowie ein zweites Abschirm-Element (202, 302, 402, 502), das elektrisch leitend ist und so angeordnet ist, dass es sowohl die erste Mess-Elektrode als auch die zweite Mess-Elektrode wenigstens teilweise abdeckt, um die erste Mess-Elektrode und die zweite Mess-Elektrode vor elektromagnetischer Interferenz zu schützen, wobei das zweite Abschirm-Element mit einer anderen Haut-Elektrode (104, 222) als der Haut-Elektrode verbunden ist, mit der das erste Abschirm-Element verbunden ist,

**dadurch gekennzeichnet, dass**

das erste Abschirm-Element und das zweite Abschirm-Element sich aneinander angrenzend zwischen der ersten Mess-Elektrode und der zweiten Mess-Elektrode auf einer Ebene erstrecken, die durch die zweite Schicht gebildet wird, und das zweite Abschirm-Element elektrisch von dem ersten Abschirm-Element isoliert ist.

2. Vorrichtung nach Anspruch 1, wobei das erste Ab-

schirm-Element und das zweite Abschirm-Element so eingerichtet sind, dass sie sich in nur einer Dimension der Ebene aneinander angrenzend erstrecken.

3. Vorrichtung nach Anspruch 1, wobei das erste Abschirm-Element und das zweite Abschirm-Element so eingerichtet sind, dass sie sich in zwei Dimensionen der Ebene aneinander angrenzend erstrecken.

4. Vorrichtung nach Anspruch 1 oder 3, wobei die zweite Schicht eine Netz-Schicht (700) ist, und das erste Abschirm-Element und das zweite Abschirm-Element so eingerichtet sind, dass sie in drei Dimensionen verwebt sind.

5. Vorrichtung nach Anspruch 1 oder 3, wobei das erste Abschirm-Element (400) und das zweite Abschirm-Element (402) eine Kamm-Struktur bilden und Kamm-Spitzen der verschiedenen Abschirm-Elemente verflochten sind.

6. Vorrichtung nach einem der vorangehenden Ansprüche, wobei ein Bereich elektromagnetischer Absorption, der durch das erste Abschirm-Element in Richtung einer Quelle der elektromagnetischen Interferenz abgedeckt wird, im Wesentlichen einem Bereich elektromagnetischer Absorption gleich ist, der durch das zweite Abschirm-Element in Richtung einer Quelle der elektromagnetischen Interferenz abgedeckt wird.

7. Vorrichtung nach einem der vorangehenden Ansprüche, wobei das erste Abschirm-Element symmetrisch in Bezug auf das zweite Abschirm-Element angeordnet ist.

8. Vorrichtung nach Anspruch 7, wobei sich das erste Abschirm-Element auf die gleiche Weise von einer Position der ersten Mess-Elektrode auf die zweite Mess-Elektrode zu erstreckt, auf die sich das zweite Abschirm-Element von einer Position der zweiten Mess-Elektrode auf die erste Mess-Elektrode zu erstreckt.

9. Vorrichtung nach einem der vorangehenden Ansprüche, wobei das erste Abschirm-Element und das zweite Abschirm-Element so angeordnet sind, dass beide einem im Wesentlichen identischen Feld elektromagnetischer Interferenz ausgesetzt sind.

10. Vorrichtung nach einem der vorangehenden Ansprüche, wobei das erste Abschirm-Element und das zweite Abschirm-Element jeweils mit einer Haut-Elektrode (220, 222) verbunden sind, die keine Mess-Elektrode ist.

11. Vorrichtung nach einem der vorangehenden An-

sprüche 1 bis 9, wobei das erste Abschirm-Element mit der ersten Mess-Elektrode verbunden ist und das zweite Abschirm-Element mit der zweiten Mess-Elektrode verbunden ist.

12. Vorrichtung nach einem der vorangehenden Ansprüche, die des Weiteren eine dritte Schicht umfasst, die über der zweiten Schicht oder zwischen der ersten Schicht und der zweiten Schicht angeordnet ist, wobei sie umfasst:

ein drittes Abschirm-Element, das elektrisch leitend ist und in der Nähe sowohl der ersten Mess-Elektrode als auch der zweiten Mess-Elektrode angeordnet ist, um die erste Mess-Elektrode und die zweite Mess-Elektrode vor elektromagnetischer Interferenz zu schützen, wobei das dritte Abschirm-Element mit einer Haut-Elektrode verbunden ist; sowie

ein viertes Abschirm-Element, das elektrisch leitend ist und in der Nähe sowohl der ersten Mess-Elektrode als auch der zweiten Mess-Elektrode angeordnet ist, um die erste Mess-Elektrode und die zweite Mess-Elektrode vor elektromagnetischer Interferenz zu schützen, wobei das vierte Abschirm-Element mit einer anderen Haut-Elektrode als der Haut-Elektrode verbunden ist, mit der das dritte Abschirm-Element verbunden ist,

wobei das dritte Abschirm-Element und das vierte Abschirm-Element sich aneinander angrenzend zwischen der ersten Mess-Elektrode und der zweiten Mess-Elektrode auf einer Ebene erstrecken, die durch die zweite Schicht gebildet wird, und alle der Abschirm-Elemente elektrisch voneinander isoliert sind.

13. Vorrichtung nach Anspruch 12, wobei das erste Abschirm-Element mit der ersten Mess-Elektrode verbunden ist und das zweite Abschirm-Element mit der zweiten Mess-Elektrode verbunden ist und das dritte Abschirm-Element und das vierte Abschirm-Element jeweils mit einer Haut-Elektrode verbunden sind, die keine Mess-Elektrode ist.

14. Vorrichtung nach einem der vorangehenden Ansprüche, wobei die Vorrichtung ein Kleidungsstück ist.

## Revendications

1. Appareil comprenant :

une première couche (210) comprenant au moins une première électrode de mesure (102) et une seconde électrode de mesure (104) disposées à une distance l'une de l'autre, la pre-

mière électrode de mesure et la seconde électrode de mesure étant des électrodes de peau configurées pour mesurer une propriété physiologique électrique à partir d'une peau ;  
une seconde couche (112) disposée sur le dessus de la première couche et comprenant :

un premier élément de blindage (200, 300, 400, 500) qui est électriquement conducteur et disposé pour recouvrir au moins partiellement à la fois la première électrode de mesure et la seconde électrode de mesure afin de protéger la première électrode de mesure et la seconde électrode de mesure de l'interférence électromagnétique, le premier élément de blindage étant relié à une électrode de peau (102, 220) ; et  
un second élément de blindage (202, 302, 402, 502) qui est électriquement conducteur, et disposé pour recouvrir au moins partiellement à la fois la première électrode de mesure et la seconde électrode de mesure afin de protéger la première électrode de mesure et la seconde électrode de mesure contre l'interférence électromagnétique, le second élément de blindage étant relié à une électrode de peau (104, 222) différente de l'électrode de peau à laquelle le premier élément de blindage est relié,

### caractérisé en ce que

le premier élément de blindage et le second élément de blindage s'étendent adjacents l'un par rapport à l'autre entre la première électrode de mesure et la seconde électrode de mesure sur un plan défini par la seconde couche, et le second élément de blindage est électriquement isolé du premier élément de blindage.

2. Appareil selon la revendication 1, le premier élément de blindage et le second élément de blindage étant configurés pour s'étendre comme adjacents l'un par rapport à l'autre dans uniquement une dimension du plan.

3. Appareil selon la revendication 1, le premier élément de blindage et le second élément de blindage étant configurés pour s'étendre en étant adjacents l'un par rapport à l'autre en deux dimensions du plan.

4. Appareil selon la revendication 1 ou 3, la seconde couche étant une couche maillée (700) où le premier élément de blindage et le second élément de blindage sont configurés pour être enchevêtrés en trois dimensions.

5. Appareil selon la revendication 1 ou 3, chacun du premier élément de blindage (400) et du second élé-

ment de blindage (402) forme une structure en peigne où les pics de peigne des différents éléments de blindage sont entrelacés.

6. Appareil selon l'une quelconque des revendications précédentes, une zone d'absorption électromagnétique recouverte par le premier élément de blindage vers une source de l'interférence électromagnétique étant sensiblement égale à une zone d'absorption électromagnétique recouverte du second élément de blindage vers une source de l'interférence électromagnétique. 5
7. Appareil selon l'une quelconque des revendications précédentes, le premier élément de blindage étant disposé d'une manière symétrique par rapport au second élément de blindage. 10
8. Appareil selon la revendication 7, le premier élément de blindage s'étendant depuis une position de la première électrode de mesure vers la seconde électrode de mesure d'une manière identique à celle du second élément de blindage qui s'étend depuis une position de la seconde électrode de mesure vers la première électrode de mesure. 15
9. Appareil selon l'une quelconque des revendications précédentes, le premier élément de blindage et le second élément de blindage étant disposés de sorte qu'ils font preuve tous deux d'un champ d'interférence électromagnétique sensiblement identique. 20
10. Appareil selon l'une quelconque des revendications précédentes, chacun du premier élément de blindage et du second élément de blindage étant reliés à une électrode de peau (220, 222) qui n'est pas une électrode de mesure. 25
11. Appareil selon l'une quelconque des revendications précédentes 1 à 9, le premier élément de blindage étant relié à la première électrode de mesure et le second élément de blindage étant relié à la seconde électrode de mesure. 30
12. Appareil selon l'une quelconque des revendications précédentes, comprenant en outre une troisième couche disposée sur le dessus de la seconde couche ou entre la première couche et la seconde couche, comprenant : 35
- un troisième élément de blindage qui est électriquement conducteur et disposé à une proximité à la fois de la première électrode de mesure et de la seconde électrode de mesure afin de protéger la première électrode de mesure et la seconde électrode de mesure contre l'interférence électromagnétique, le troisième élément de blindage étant relié à une électrode de peau ; 40
- 45
- 50
- 55

et

un quatrième élément de blindage qui est électriquement conducteur, et disposé à une proximité à la fois de la première électrode de mesure et de la seconde électrode de mesure afin de protéger la première électrode de mesure et la seconde électrode de mesure de l'interférence électromagnétique, le quatrième élément de blindage étant relié à une électrode de peau différente de l'électrode de peau à laquelle le troisième élément de blindage est relié, le troisième élément de blindage et le quatrième élément de blindage s'étendant adjacents l'un par rapport à l'autre entre la première électrode de mesure et la seconde électrode de mesure sur un plan défini par la seconde couche, et tous les éléments de blindage étant électriquement isolés l'un de l'autre.

13. Appareil selon la revendication 12, le premier élément de blindage étant relié à la première électrode de mesure et le second élément de blindage étant relié à la seconde électrode de mesure, et chacun du troisième élément de blindage et du quatrième élément de blindage étant relié à une électrode de peau qui n'est pas une électrode de mesure. 20
- 25

14. Appareil selon l'une quelconque des revendications précédentes, l'appareil étant un article vestimentaire. 30

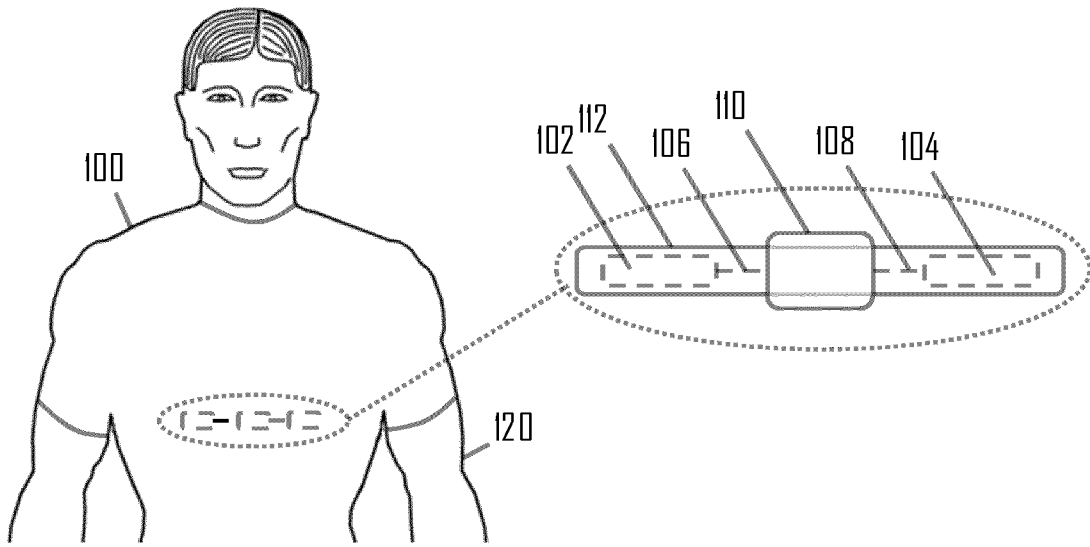


Fig 1



Fig 2A

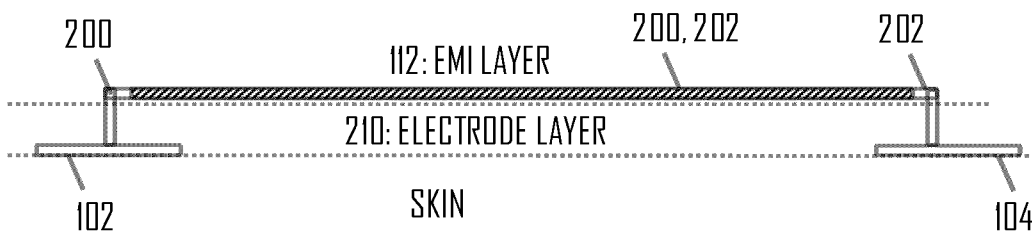


Fig 2B

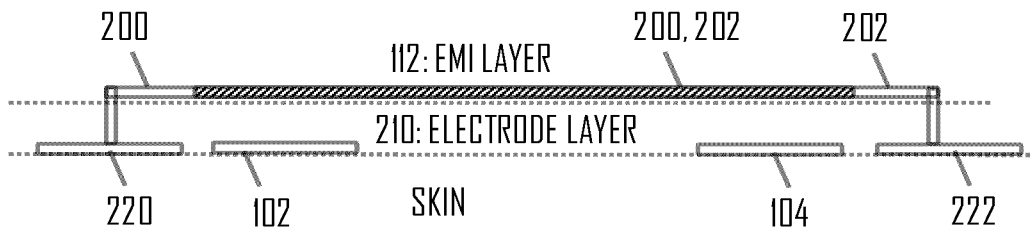
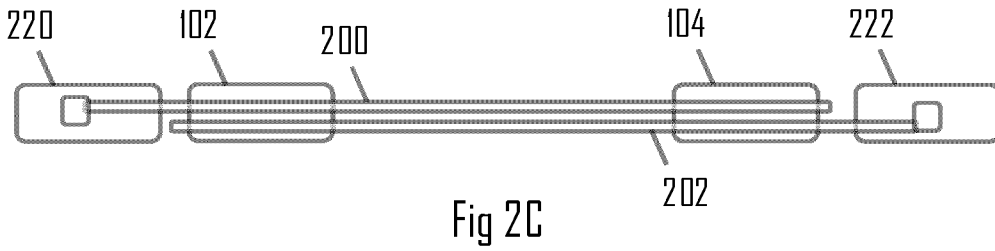


Fig 2D

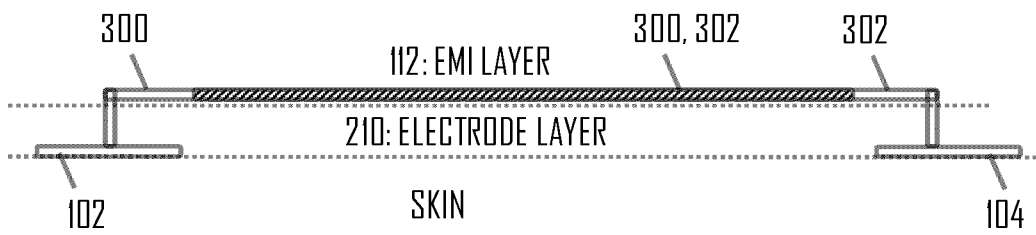
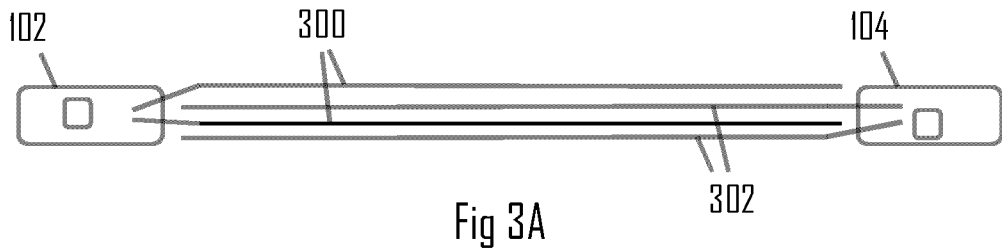


Fig 3B

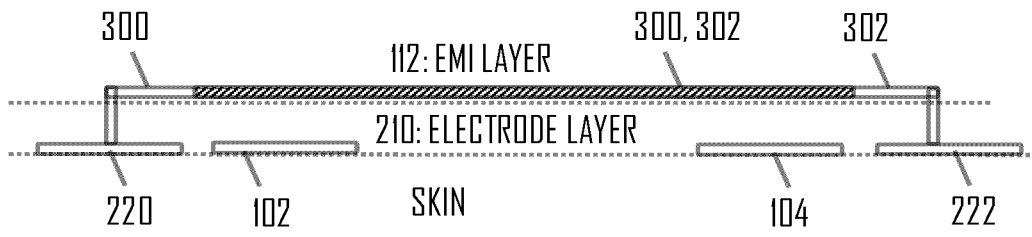
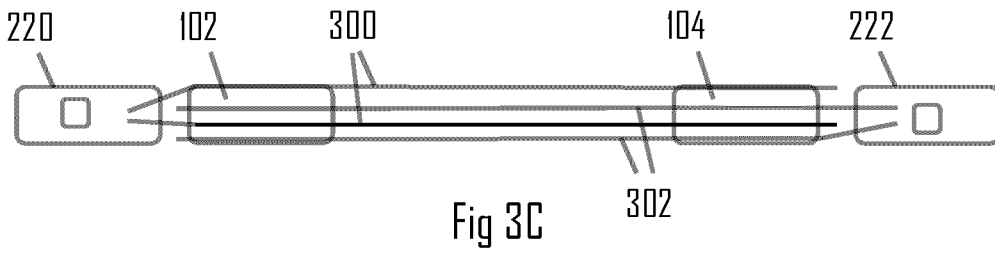


Fig 3D

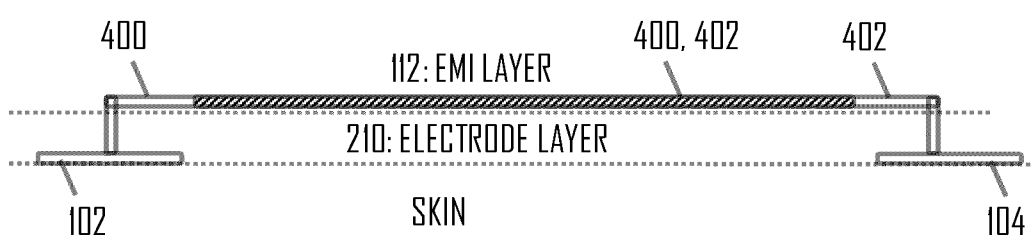
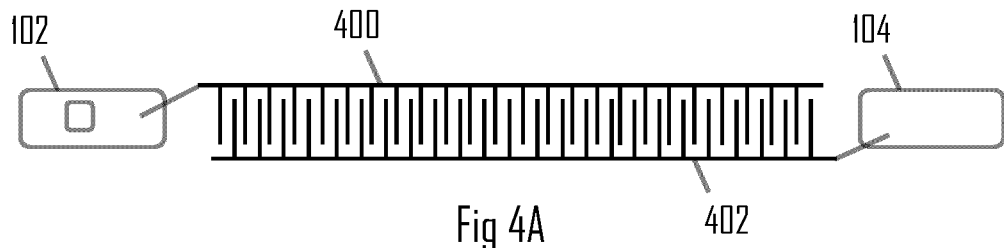


Fig 4B

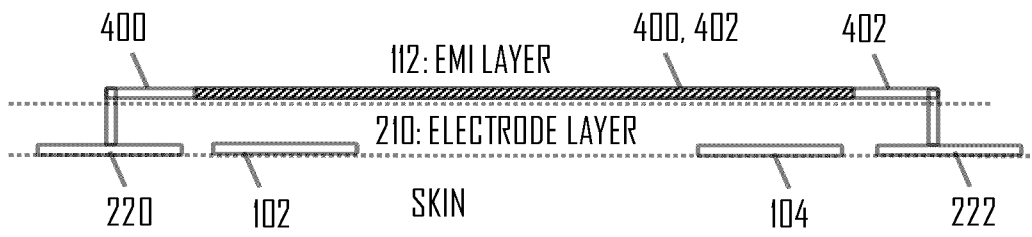
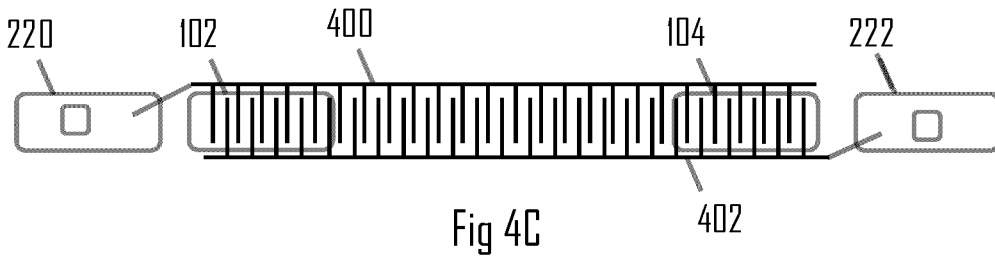


Fig 4D

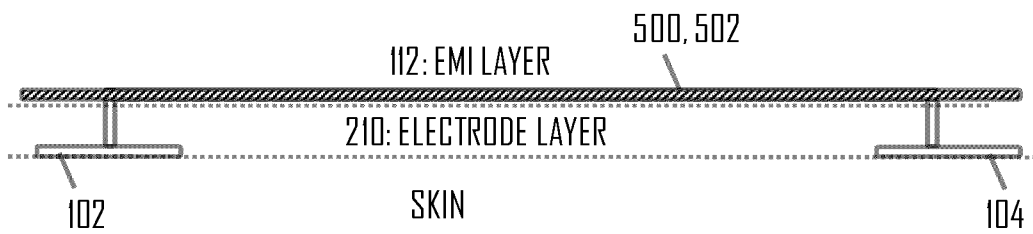
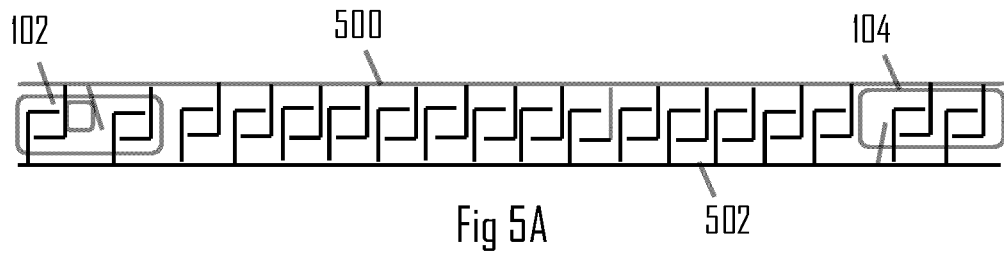
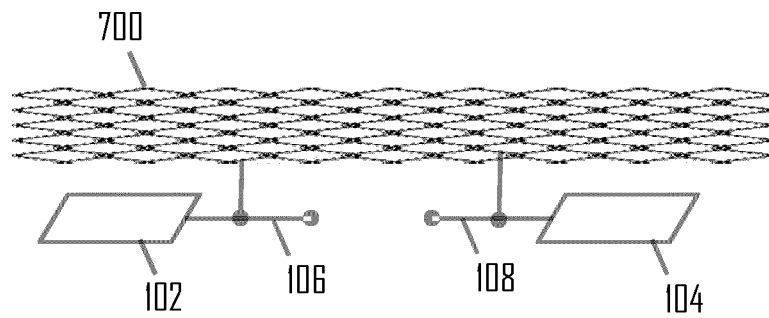
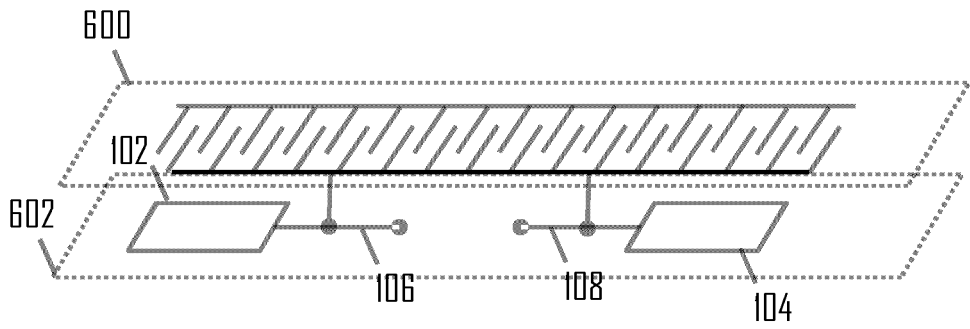
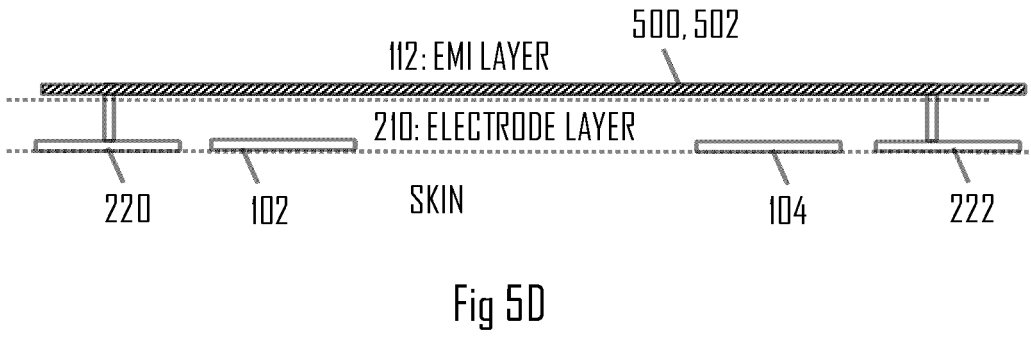
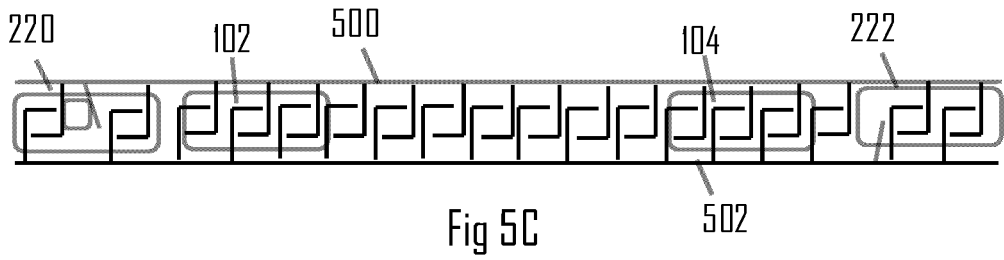


Fig 5B



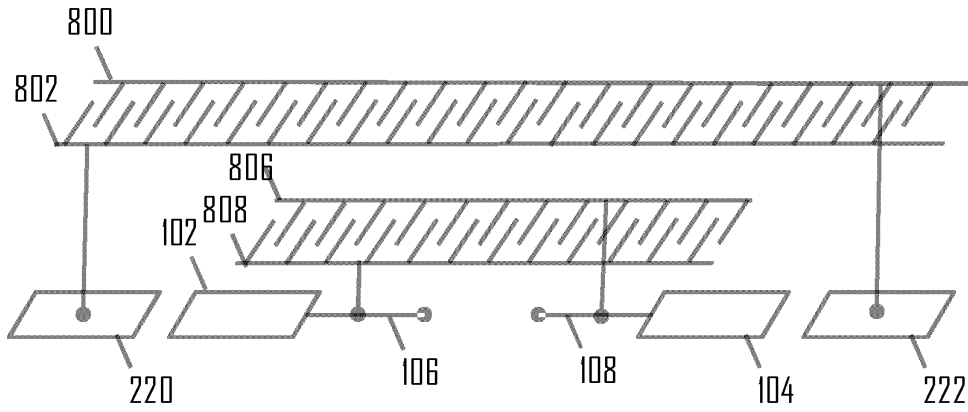


Fig 8

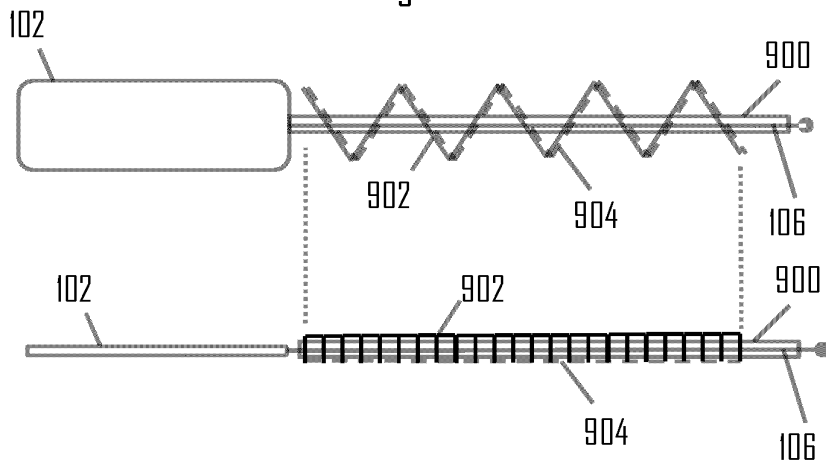


Fig 9

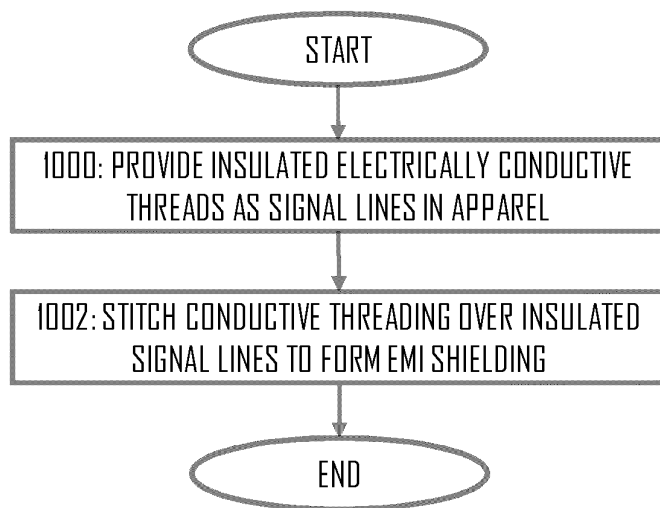


Fig 10

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- EP 2057943 A [0003]

专利名称(译)	用于生理测量的EMI保护		
公开(公告)号	<a href="#">EP3231357B1</a>	公开(公告)日	2019-04-03
申请号	EP2017154739	申请日	2017-02-06
[标]申请(专利权)人(译)	博能电子公司		
申请(专利权)人(译)	Polar Electro Oy公司		
当前申请(专利权)人(译)	Polar Electro Oy公司		
[标]发明人	KORKALA SEPPO LAMSA KAISA PEKONEN ELIAS		
发明人	KORKALA, SEPPO LÄMSÄ, KAISA PEKONEN, ELIAS		
IPC分类号	A61B5/00 A61B5/0245 A61B5/0408		
CPC分类号	A61B5/0478 A61B5/0245 A61B5/04 A61B5/0408 A61B5/04085 A61B5/0424 A61B5/6831 A61B2562/164 A61B2562/182 H05K9/0081		
代理机构(译)	KOLSTER OY AB		
其他公开文献	EP3231357A1		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

本发明公开了一种装置，包括：第一层，包括至少第一测量电极（102）和第二测量电极（104），所述第一测量电极和第二测量电极彼此隔开一定距离设置，其中所述第一测量电极和第二测量电极是配置的皮肤电极测量皮肤的电生理特性；第二层设置在第一层的顶部上并且包括：第一和第二屏蔽元件（200,202），其是导电的并且布置成至少部分地覆盖第一测量电极和第二测量电极，以便保护第一测量电极和第二测量电极。第一测量电极和第二测量电极抵抗电磁干扰，其中每个屏蔽元件连接到皮肤电极（102,104,220,222），其中第一屏蔽元件和第二屏蔽元件相对于彼此相邻地延伸第一测量电极和第二测量电极之间在由第二层限定的平面上，并且其中第二屏蔽元件与第一屏蔽元件电隔离。

