

(19)



(11)

**EP 3 492 133 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**10.06.2020 Bulletin 2020/24**

(51) Int Cl.:  
**A61M 25/00** (2006.01)      **A61B 5/00** (2006.01)  
**A61B 5/021** (2006.01)      **A61M 1/36** (2006.01)  
**A61B 5/0215** (2006.01)

(21) Application number: **19150583.3**

(22) Date of filing: **04.04.2012**

(54) **BI-DIRECTIONAL PERFUSION CANNULA**  
BIDIREKTIONALE PERFUSIONSKANÜLE  
CANULE DE PERFUSION BIDIRECTIONNELLE

(84) Designated Contracting States:  
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR**

(30) Priority: **05.04.2011 AU 2011901258**  
**03.06.2011 AU 2011902210**

(43) Date of publication of application:  
**05.06.2019 Bulletin 2019/23**

(62) Document number(s) of the earlier application(s) in accordance with Art. 76 EPC:  
**12767449.7 / 2 694 148**

(73) Proprietor: **Sorin Group Italia S.r.l.**  
**41037 Mirandola (MO) (IT)**

(72) Inventors:  
• **MOSHINSKY, Randall**  
**Melbourne, Victoria 3144 (AU)**  
• **MCMILLAN, James**  
**Melbourne, 3195 (AU)**  
• **TUTUNGI, Elli**  
**Melbourne, 3150 (AU)**

(74) Representative: **De Bonis, Paolo**  
**Buzzi, Notaro & Antonielli d'Oulx S.p.A.**  
**Corso Vittorio Emanuele II, 6**  
**10123 Torino (IT)**

(56) References cited:  
**WO-A2-2005/037345 US-A- 4 114 618**  
**US-A- 5 171 218**

**EP 3 492 133 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

### FIELD

**[0001]** The present disclosure relates to a bi-directional perfusion cannula. Bi-directional perfusion cannulae are known, e.g., from US 4,114,618, US 5,171,218, and WO 2005/037345 A1.

### BACKGROUND

**[0002]** This section provides background information related to the present disclosure which is not necessarily prior art.

**[0003]** Some cardiac surgery procedures require peripheral artery cannulation for cardiopulmonary bypass. Also, some disease states require mechanical cardiopulmonary support via peripheral artery cannulation. This peripheral artery is often, but not always, the femoral artery. Insertion into the femoral artery of an arterial cannula of sufficient size to support the patient with cardiopulmonary bypass often leads to compromised blood flow to the lower limb which can lead to ischemia and tissue necrosis during prolonged procedures.

**[0004]** Previously proposed methods of providing perfusion to the body while maintaining perfusion to the lower limb are generally inconvenient and often do not provide a satisfactory solution.

**[0005]** It has previously been proposed to use an undersized cannula, based on the assumption that the smaller cannula will allow blood flow back over the body of the cannula between the cannula body and the arterial wall. In practice it is difficult to achieve adequate perfusion to the lower limb and using a cannula of a smaller size than what is actually required compromises perfusion to the body and increases line pressures, thus increasing the risk of red blood cell haemolysis, increased backpressure to the membrane oxygenator and the perfusion pump and the increased risk of damage to these vital pieces of equipment.

**[0006]** It has also been previously proposed to insert a further perfusion cannula downstream of a first, main perfusion cannula. Inserting a downstream cannula can be technically difficult and a percutaneous approach often requires ultrasound guidance to allow accurate placement. This technique requires an extra cannula and an extra perfusion line that must be connected into the arterial side of the perfusion circuit and can be time consuming. It also results in extra hardware being disposed in the groin incision area, an area that is already compromised for space with the femoral arterial and femoral venous lines already in place. The downstream cannula would typically be a small cannula which is more susceptible to positional changes, resulting in less reliable downstream flow.

**[0007]** It has also been previously proposed to sew a side graft to the artery when using femoral artery cannulation. In this technique, surgeons sew on a Dacron graft

to the side of the femoral artery as an end to side anastomosis and a cannula is inserted into the graft. This technique is time consuming, taking approximately 30 minutes to sew on the graft and cannulate it, compared with approximately 2 minutes to insert a bidirectional femoral cannula. Furthermore, this technique requires an open surgical procedure which can be difficult in an ICU setting. Bleeding can also be a problem in patients requiring extended periods of support and when support ceases, the base of the Dacron graft may be left in situ with this technique, creating a potential source for thrombus formation and infection.

**[0008]** It is desirable to provide a single cannula that provides adequate perfusion to the lower limb. However, as will be discussed below, previously proposed cannulae suffer a number of drawbacks.

**[0009]** It has been previously proposed to provide a conventional cannula with side perfusion holes through which blood can flow toward the lower limb. Such arrangements have been disclosed in WO03/068303 to Laksen et al. and in "A Novel Femoral Arterial Cannula to Prevent Limb Ischemia During Cardiopulmonary Support: Preliminary Report of Experimental and Clinical Experiences" by Matsui et al. in *Artif Organs*, Vol. 30, No. 7 2006. In arrangements having side perfusion holes, the cannula must be correctly positioned in the artery so that the holes are not occluded, and maintained in that position. In these arrangements, no tactile feedback is available to assist with positioning of the holes and assistance in maintaining the holes in correct position is not provided. If the cannula migrates distally the holes will be occluded by wall of artery. If the cannula migrates proximally then the holes may move outside of the artery and cause bleeding. If the side holes are at level of the arteriotomy, perfusion into the wall of the artery may cause a dissection.

**[0010]** To prevent occlusion of side holes provided in a conventional cannula, it has been proposed to provide rails adjacent the holes to prevent occlusion of the holes. Such an arrangement has been disclosed in "A femoral artery cannula that allows distal blood flow" by Magovern, J. et al. (*The Journal of Thoracic and Cardiovascular Surgery*, September 2005). The configuration of the rails can be complicated and difficulties will be encountered with their insertion and removal through the wall of the artery. The rails also create a ridged cross section which creates a potential for bleeding during insertion and removal. Furthermore, blood passing through the side holes is not efficiently communicated as it is directed against the wall of artery.

**[0011]** Alternative rail configurations have also been proposed to facilitate insertion of the cannula into the artery while attempting to prevent occlusion of side holes. Documents US 5,171,218 and US 5,330,433 by Fonger, J. et al, each disclose an arrangement in which the rails are in the form of forward pointing barbs between which a slanted elongate hole located in a depression on the exterior of the wall of the cannula is disposed. The de-

pression impinges into the main lumen to act as a scoop to divert blood toward the lower limb.

**[0012]** As with previous proposals, difficulties will be encountered with insertion and removal due to the cross sectional shape of the barbs, which, as can be seen in Figure 5 of each of the documents, is ridged in the region of the barbs/rails and will require the artery to stretch during insertion and removal. As this region passes through the artery wall, this ridged cross section may also create channels between the ridges that may result in bleeding during insertion and removal.

**[0013]** Furthermore, the main lumen is narrowed by the side hole depression, thereby reducing flow capability. The most important determinant of flow through a cannula, as determined by the Poiseuille-Hagen equation, is cannula radius. Decreasing radius by half causes a decrease in flow of sixteen times. Reducing the radius in a femoral cannula that is already being pushed to achieve maximal flow rates is a major compromise in the primary function, that is, providing flow equal to systemic cardiac output.

**[0014]** Due to the configuration of the barbs and the side aperture, this arrangement may be difficult to manufacture. Furthermore, flow from the side aperture does not have an open area of artery to flow into, thereby reducing flow efficiency and creating an area of turbulent flow.

**[0015]** As discussed above, each of the previously proposed bidirectional cannulae have suffered from a number of problems. Furthermore, general poor performance has been observed due to issues with occlusion of side facing holes/apertures. The Inventors have found that the previous poor performance can at least partially be attributed to two factors, arterial spasm and downstream compression.

**[0016]** Arterial Spasm relates to the normal physiological response of contraction of arterial smooth muscle to stretch or local trauma. Arterial spasm around the body of the cannula will result in a reduction of blood flow back around the cannula and down the leg. This can even occur around undersized cannula.

**[0017]** Downstream Compression, as illustrated in Figure 1, is a mechanism that has not been previously acknowledged. The body of a standard femoral cannula causes a distortion of the arterial wall around the point of insertion. As the cannula tends to lie in the orientation of the artery, the body of the cannula causes a downward displacement of the distal edge of the arteriotomy, and compression of the artery just distal to the arteriotomy. Obstruction of flow downstream to the arteriotomy has to be overcome if reliable downstream flow is to be provided.

**[0018]** The issues of arterial spasm and downstream compression have not been acknowledged or addressed in the previous proposals.

**[0019]** Examples of the invention seek to solve, or at least ameliorate, one or more disadvantages of previous cannulae.

## SUMMARY

**[0020]** This section provides a general summary of the disclosure, and is not a comprehensive disclosure of its full scope or all of its features.

**[0021]** According to the present invention, there is provided a bidirectional perfusion cannula comprising an elongate tube for insertion into an artery, the elongate tube comprising: a first aperture at a distal end of the tube which is forward during insertion, the first aperture being configured so that blood can flow into the artery in the direction of insertion; an elbow formed in the elongate tube; and a second aperture, the second aperture being formed in or slightly rearward of the elbow and configured for supplying blood into the artery in a second direction which is generally opposite to the insertion direction.

**[0022]** Preferably, the elbow is performed in the elongate tube such that in a relaxed state prior to insertion the cannula has an elbow bend formed in it, preferably in the range of 90 to 180 degrees.

**[0023]** The elongate tube has a protuberance at least partially formed on the elbow, the protuberance being configured to facilitate positioning of the cannula in the artery. Preferably, the protuberance and elbow form a transition zone which splints open the artery. In one embodiment, the transition zone is inflatable. Preferably, the protuberance can taper in the insertion direction to allow insertion of the cannula in the artery.

**[0024]** Preferably, a rearward portion of the protuberance tapers at a greater rate than it does in the insertion direction so as to provide greater resistance during removal than during insertion.

**[0025]** A side profile of the protuberance can have the form of a shoulder, preferably a rounded shoulder.

**[0026]** According to the invention, the protuberance is ovoid in cross section. The protuberance can extend generally along an outer surface of the elbow. Preferably, the second aperture extends through the protuberance. Preferably, the second aperture extends in a direction generally away from the forward end of the tube.

**[0027]** The elongate tube can terminate at the first aperture. The elongate tube can be configured to receive an elongate introducer therethrough to aid in insertion of the cannula and prevent blood flow through the first aperture whilst the elongate tube and introducer are inserted into an artery.

**[0028]** The elongate tube can be configured so that an internal diameter of the elongate tube, in a region around the second aperture, is greater than a diameter of a corresponding portion of the elongate introducer when received therethrough so that blood can pass into the elongate tube through the second aperture to indicate that the second aperture has passed into the artery. Preferably, the internal diameter of the elongate tube is generally constant along a length of the tube.

**[0029]** Preferably, the elbow bends through an angle of approximately 130 degrees. The elongate tube can be formed of flexible material so as to at least partially

straighten when an introducer is inserted into the cannula. The elongate tube can be formed of a wire-reinforced flexible polyurethane material.

**[0030]** Preferably, the cannula is configured to be inserted into a femoral artery. The cannula can also be configured to be inserted into a subclavian or axillary artery.

**[0031]** The cannula can further include a manometer tube in communication with a pressure transducer, the manometer tube configured for measuring the pressure of blood flowing in the second direction.

**[0032]** According to the present disclosure, there is also provided, in combination, a bi-directional perfusion cannula of the above described type and a tapered introducer received through the elongate tube.

**[0033]** According to the present disclosure, there is also provided a method of inserting into an artery a bi-directional perfusion cannula, whereby the method is not part of the present invention, comprising an elongate tube having a first aperture at a distal end for supplying blood into the artery in a direction of insertion, an elbow formed in the elongate tube, a protuberance formed at least partially on the elbow and a second aperture formed in the protuberance for supplying blood into the artery away from the insertion direction, the method comprising the steps of: feeding the distal end of the elongate tube into the artery until an increase in resistance to insertion is felt to indicate that the protuberance is entering the artery; easing the elongate tube into the artery until the elbow and the protuberance have passed into the artery and the amount of resistance reduces; and retracting the elongate tube until an increase in resistance to retraction is felt to indicate that the protuberance is abutting the artery wall and the cannula is in position.

**[0034]** Preferably, blood flows into the elongate tube through the second aperture after the second aperture has been eased into the artery.

**[0035]** Preferably, after treatment the cannula is retracted by easing the protuberance through a wall of the artery, whereby an opening formed in the artery wall is gradually enlarged by the increasing cross sectional size of the protuberance so that the elongate tube can be removed generally without causing further trauma to the artery.

**[0036]** According to the present disclosure, there is also provided a method of providing perfusion to a limb during peripheral artery cannulation, whereby the method is not part of the invention, the method including the steps of: inserting a cannula of the above described type into an artery; pumping blood through the cannula to the artery; and monitoring the pressure measured by the pressure transducer to ensure that an adequate level of blood flow to the limb is provided.

**[0037]** According to preferred examples, the pressure of blood flowing in the second direction is constantly monitored and maintained in a range which is close to a pressure level in the second direction determined at the commencement of flow.

**[0038]** Further areas of applicability will become apparent from the description provided herein. The description and specific examples in this summary are intended for purposes of illustration only and are not intended to limit the scope of the present disclosure.

## DRAWINGS

**[0039]** The drawings described herein are for illustrative purposes only of selected embodiments and not all possible implementations, and are not intended to limit the scope of the present disclosure.

**[0040]** The invention will be further described, by way of nonlimiting example only, with reference to the accompanying drawings in which:

Figure 1 is a sectional side view of a conventional cannula inserted into an artery;

Figure 2 is a side view of a bi-directional perfusion cannula of one embodiment of the invention, with an introducer received therein;

Figure 3 is a sectional view of the cannula along line A-A of Figure 4;

Figure 4 is a front view of the cannula with wire reinforcement removed for clarity;

Figure 5 is a side view of the bi-directional perfusion cannula of Figure 4;

Figures 6A, 6B and 6C are sectional views of the cannula of Figure 5, the sections being taken along lines C-C, D-D and E-E of Figure 5 respectively;

Figure 7 is a sectional view of the cannula inserted into an artery;

Figure 8A is a rear perspective view of the cannula with a manometer tube affixed thereto; and

Figure 8B is a close rear view of the manometer tube.

**[0041]** Corresponding reference numerals indicate corresponding parts throughout the several views of the drawings.

## DETAILED DESCRIPTION

**[0042]** Example embodiments will now be described more fully with reference to the accompanying drawings.

**[0043]** References to "embodiments" throughout the description which are not under the scope of the appended claims represent possible examples and are therefore not part of the present invention, unless the context clearly dictates otherwise. The invention is defined by the appended claims.

**[0044]** With reference to Figure 2, there is shown a bi-directional perfusion cannula 10 comprising an elongate tube 12 configured for insertion into an artery. The elongate tube 12 comprises a first aperture 14 at a distal end of the elongate tube 12 which is forward during insertion of the cannula into an artery. The first aperture 14 is configured so that blood can flow into the artery in the direction of insertion and towards the arterial circulation of the

patient.

**[0045]** The elongate tube 12 also comprises an elbow 16 which is formed in the elongate tube. The elbow 16 is preformed such that in a relaxed state prior to insertion the cannula has an elbow bend in it. In the example shown, the elbow bends through an angle of 130 degrees, which has been found to be the angle that best alleviates the downstream compression of the artery distal to the arteriotomy and allows the cannula to achieve a suitable lie outside the artery. It will be appreciated that other angles, such as 120 degrees, and particularly those in the range of 90 to 180 degrees may also be suitable. Angles outside of this range may not be effective at alleviating downstream compression or allowing the intravascular and extra vascular sections of the cannula to achieve a suitable lie. The elbow 16 allows the elongate tube 12 to transition a suitable amount so that a second aperture 18, in the form of a rearward facing aperture can be provided for bi-directional perfusion.

**[0046]** Previously proposed arrangements, such as those disclosed in Fonger et al, do not include an elbow so that a rearward facing aperture directing blood into the artery and not into the artery wall can be provided. The inventors have found that, in use, an artery which is naturally flexible, and less rigid than a conventional cannula, tends to bend around a straight cannula when inserted in the artery, thereby acting to close the artery in the manner shown in Figure 1. Arrangements having side facing holes are particularly susceptible to this problem. By providing an elbow and a rearward facing aperture, it is possible to avoid obstruction or covering of the aperture by the artery wall, as illustrated in Figure 7, thus increasing the effectiveness of the cannula. In particular, the problems discussed above in relation to arterial spasm and downstream compression can be alleviated as the rearward facing aperture is away from the artery wall.

**[0047]** The elbow 16 also assists in positioning of the cannula 10 as it passes from the femoral artery to the surface of the leg. The angle used for the elbow 16 is selected so as to reduce the amount of downstream or distal artery compression.

**[0048]** As illustrated, the second aperture 18 is formed in or slightly rearward, i.e. away from the insertion or forward direction, of the elbow 16. The second aperture 18 faces rearward and is configured for supplying blood into the artery in a second direction which is generally opposite to the forward or insertion direction so as to achieve bi-directional perfusion in the artery. In the examples shown, the second aperture 18 is formed in the elbow, though it may be formed slightly rearward of the elbow and still provide adequate bi-directional perfusion in the artery. Forming the second aperture 18 in or slightly rearward of the elbow 16 allows a second path for blood flow to be provided without impinging on or narrowing the lumen of the elongate tube 12, thereby avoiding a reduction in blood flow through the cannula 10. The configuration of the elbow 16 and the second aperture 18 is such that when the cannula 10 is inserted into the artery, the sec-

ond aperture 18 is correctly orientated within the artery.

**[0049]** The elongate tube 12 has a protuberance 20 which is formed on the elbow 16 and is configured to facilitate insertion and positioning of the cannula 10 in the artery. The protuberance 20 is formed on and extends along an outer surface of the elbow 16. As can be seen in Figures 6A to 6C, the extent of the protuberance 20 is generally limited to a lower one half of the cross section and is not visible when viewed from in-front (Figure 4) or above the cannula 10.

**[0050]** The protuberance 20 tapers in the insertion direction to allow insertion of the cannula into the artery with minimal trauma. In this regard, the taper is gradual so as to allow the artery wall to gradually expand as the cannula 10 is inserted. The angle of the taper is between approximately 3 to 25 degrees. For differently sized cannulae, the taper angle will be the same, though the maximum thickness of the protuberance will depend on the size of the cannula. For example, a 20F cannula will have a protuberance with a maximum thickness, excluding the thickness of the elongate tube on which it is formed, of approximately 1.5mm. It will be appreciated that the size of the protuberance formed on smaller cannulae will be scaled down and smaller.

**[0051]** The size of the protuberance 20 is small enough so as to allow insertion of the cannula 10 into the artery with minimal trauma, though large enough to prevent accidental dislodgement of the cannula 10. The size of the protuberance 20 is also sufficient so that the second aperture 18 can be positioned within the protuberance 20 so as to orientate the second aperture 18 within the artery.

**[0052]** The protuberance 20 and elbow 16 together form a transition zone 28 where a cross sectional size of the elongate tube 12 gradually increases and then decreases so that it can be inserted into the artery with minimal trauma inflicted on the artery wall. In the embodiments shown, the protuberance 20 is generally ovoid in cross section, as can be seen in Figures 6A, 6B and 6C, though other shapes may also be used.

**[0053]** The transition zone 28 acts to splint open the artery so that the artery is not compressed by the body of the cannula and allows unimpeded flow in the second direction. The transition zone 28 acts to support the artery wall away from the second aperture 18 so that the artery is held open and does not block the flow of blood from the cannula 10 into the artery. The transition zone 28 also acts to provide stability to the cannula 10 when inserted in an artery so as to maintain the cannula 10 in position.

**[0054]** A rearward portion of the protuberance 20 tapers at a greater rate than it does in the insertion direction so as to provide greater resistance during removal than during insertion. The rearward portion of the protuberance 20 tapers more sharply so that a side profile of the protuberance 20 generally has the form of a rounded shoulder.

**[0055]** The inventors have found that by providing a

protuberance in the form of a rounded shoulder, a good balance between minimising arterial trauma during removal and resistance to removal can be achieved. The protuberance also provides a self-locating mechanism. In this regard, the increased resistance provided against removal of the cannula allows a surgeon to insert the cannula 10 under slight resistance to a predetermined depth at which the resistance will reduce. The cannula 10 can then be retracted slightly until increased resistance is felt, providing direct tactile feedback to indicate that the cannula is correctly placed in the artery. The increased resistance provided against removal also prevents accidental or unintentional withdrawal of the cannula 10 from the artery. This is important because if the second aperture 18 moves outside the artery, blood may flow from the cannula outside the artery causing bleeding.

**[0056]** By providing a protuberance in the form of a rounded shoulder, ridges, rails or barbs which can create channels for bleeding during insertion and removal are avoided.

**[0057]** The rearward portion of the protuberance 20 is disposed at a predetermined distance from the second aperture 18 so that when the cannula 10 is placed in a desired position in an artery, the second aperture 18 is positioned well within the artery.

**[0058]** The rearward portion of the protuberance 20 lies against the arteriotomy to act as a scaffold, effectively stenting open the downstream artery, which would otherwise move to conform with the shape of the cannula and compress the downstream artery potentially occlude flow from a side perfusion hole down the artery. By stenting open the artery, the protuberance maintains a channel through which blood can flow unobstructed down the leg.

**[0059]** In the examples shown, the second aperture 18 extends through the protuberance 20 and in a direction generally away from the forward end of the tube, as can be seen in Figure 3, so as to provide flow to a lower limb which is generally unimpeded. Due to the size of the cannula and the artery into which it is intended to be received, the protuberance generally surrounds the second aperture 18 so that the second aperture 18 is well placed within the artery when the cannula is positioned within the artery.

**[0060]** As can be seen in Figure 2, an innermost portion of the second aperture 18 which is inside the lumen of the elongate tube 12 is generally funnel shaped to minimise turbulence of blood flowing within the elongate tube 12 and through the second aperture 18. The size of the second aperture 18 may be varied in accordance with differently sized elongate tubes to achieve different proportions of flow to the lower limb. In the example shown, the diameter of the second aperture 18 is 2.0mm.

**[0061]** As can be seen in Figure 2, the elongate tube 12 terminates at the first aperture 14. It can also be seen that the elongate tube 12 tapers at the forward end in a region proximal the first aperture 14. A flexible elongate

introducer 22 can be received through the elongate tube 12 with its tip passing out of the first aperture 14. The introducer 22 aids insertion into the artery by providing a tapered end protruding out of the first aperture 14. The introducer also prevents blood flowing back from the first aperture 14. The first aperture 14 is configured to engage the introducer 22 which is received through the elongate tube 12 to prevent blood flow through the first aperture 14 and into the elongate tube 12 whilst an introducer 22 is received in the elongate tube 12.

**[0062]** As can be seen in Figure 7, the elongate tube 12 can be configured so that an internal diameter of the elongate tube 12, in a region around the second aperture 18, is greater than a diameter of a corresponding portion of the elongate introducer 22 when received therethrough so that blood can pass into the elongate tube 12 through the second aperture 18 to indicate that the second aperture 18 has passed into the artery 21. In this regard, the elongate introducer 22, when inserted in the elongate tube, narrows in the region of the second aperture 18 to allow entry of blood into the elongate tube 12. The internal diameter of the elongate tube 12 is generally constant along a length of the elongate tube 12.

**[0063]** The resulting flash of blood entering the elongate tube 12 as the second aperture 18 passes into the artery provides a physician with a visual indication that the cannula 10 is almost in position. This flash of blood is particularly helpful during percutaneous insertion. Inserting the cannula 10 a little further into the artery 21 from this position allows a rearward portion of the protuberance 20 to pass into the artery. Once this rearward portion has passed into the artery 21, the sharper taper of the rearward portion of the protuberance 20 works to prevent accidental or unintentional withdrawal.

**[0064]** As can be seen in Figure 6A, forward of the protuberance 20 and rearward of the taper proximal the first aperture 14, the external diameter of the elongate tube 12 is generally constant before transitioning into the protuberance 20 (Figure 6B). The diameter of the elongate tube 12 transitions back or returns to this constant value rearward of the protuberance 20, as can be seen in Figure 6C. The size of the elongate tube 12 is selected to provide adequate blood flow to the patient and an external diameter of the elongate tube may be between approximately 3mm and approximately 8mm. Depending on the size of the patient and the elongate tube used, obstruction of flow around the body of the cannula may occur.

**[0065]** The elongate tube 12 is formed of flexible material so as to at least partially straighten out when an introducer 22 is inserted into the cannula 10 to facilitate insertion of the cannula 10 into an artery. Once the introducer 22 is removed, the elongate tube 12 will return to its natural shape so as to splint open the artery, as discussed above. The elongate tube 12 may become almost completely straight when an introducer 22 is inserted into the cannula 10. As can be seen in Figure 2, the elongate tube 12 is formed of a wire-reinforced material. In the

described example, the elongate tube is formed of a flexible polyurethane material which is generally transparent, though it will be appreciated that other materials, such as silicone may also be used.

**[0066]** In some examples, different sections of the cannula 10 may be made from different materials. For example, the elbow 16 may be formed from a different material than the elongate tube 12. Furthermore, the elbow 16 may be formed of a flexible material such as PVC, polyurethane, silicone or rubber and configured so as to be inflatable. An inflatable elbow may be configured for manual inflation or configured to be self inflating. In such an example, the elbow 16 may remain in an uninflated or partially inflated state during insertion then become inflated to a form generally in accordance with that previously described ready for use. In this regard, when in position and inflated, the inflatable elbow provides a protuberance 20 and houses the second aperture 18 so that bi-directional perfusion can be achieved. The inflatable elbow may be configured to expand against the inner wall of the artery to hold the cannula in place and to keep the wall spaced from the second aperture 18.

**[0067]** A proximal end 24 of the cannula 10 is shown with a standard 3/8" connector. Such a generic fitting may be used, or other commercially available fittings may be substituted to allow the cannula 10 to be used with different perfusion tubing.

**[0068]** The previously described embodiments have been described in relation to generally inserting the cannula 10 into an artery. It will be appreciated that the cannula 10 is suitable for direct insertion into the artery with open surgical exposure and also suitable for percutaneous use.

**[0069]** During percutaneous use, which may continue for a number of days, it is desirable to ensure that the cannula remains correctly placed in the artery so that adequate perfusion is maintained. To ensure that adequate perfusion is maintained, the pressure of blood flowing into the artery behind the cannula and toward a limb, i.e. the perfusion blood which is flowing away from the arterial circulation of the patient, may be monitored.

**[0070]** Figures 8A and 8B illustrate an example of an arrangement for monitoring a pressure of perfusion blood flowing toward a limb, so as to indicate adequacy of downstream flow and position of the cannula 10. In the illustrated example, a manometer tube 30 extends adjacent to the elongate tube 12. The manometer tube 30 passes through a wall of the elongate tube at a location behind the protuberance 20 in the insertion direction. This location is such that its position will be outside the patient in use. It will be appreciated that the manometer tube 30 may pass through the wall of the elongate tube at other locations behind the protuberance 20 and still provide the required communication between the manometer tube 30 and a pressure transducer. The manometer tube 30 passes through the elongate tube 12 and terminates at aperture 32 which is adjacent the second aperture 18. The position of the aperture 32 is such that the pressure

of blood flowing toward the limb may be monitored.

**[0071]** The manometer tube 30 is configured to accept a connector 34 to allow connection between the manometer tube 30 and a pressure transducer (not shown). In use, when the cannula 10 is inserted in the artery, blood will flow through the aperture 18 and into an artery of the patient toward a limb. The pressure transducer will measure the pressure of this blood flowing toward the limb so that it may be determined if there is sufficient flow toward the limb. A reading from the pressure transducer may thus be used to indicate if the cannula is placed correctly in the artery. In this regard, when the cannula is placed correctly in the artery, the pressure reading will initially demonstrate pulsatile flow transmitted through the elongate tube from aperture 14. Once non-pulsatile flow commences through the elongate tube, monitoring the trend in pressure as well as the absolute pressure, will indicate any changes in perfusion towards the limb. Incorrect placement may involve the cannula being inserted too far into the artery, in which case the second aperture may become covered, or not being inserted far enough, in which case the second aperture would not be located within the artery and there would be little or no flow into the artery.

**[0072]** The pressure transducer may also be used to confirm that an initial placement of the cannula 10 is correct.

**[0073]** The use of a pressure transducer may be beneficial in environments where prolonged perfusion is common, such as Extra Corporeal Membrane Oxygenation (ECMO) units and in Intensive Care Units.

**[0074]** To allow insertion of the cannula 10 and tapered introducer 22 into an artery, known guide wire techniques are used.

**[0075]** A method of inserting the bi-directional perfusion cannula 10 into an artery comprises the steps of feeding the distal end of the elongate tube 12 with introducer 22 received therethrough into the artery (over a guide wire after predilating the artery with dilators) until an increase in resistance to insertion is felt to indicate that the protuberance 20 is entering the artery. The elongate tube 12 is then eased into the artery until the elbow 16 and the protuberance 20 have passed into the artery and the amount of resistance reduces. The elongate tube 12 is then retracted until an increase in resistance to retraction is felt to indicate that the protuberance 20 is abutting the artery wall and the cannula 10 is in position.

**[0076]** Once the cannula is in position, the introducer 22 may be removed so that the cannula 10 can be connected to suitable perfusion equipment.

**[0077]** After treatment, the cannula 10 is retracted by easing the protuberance 20 through a wall of the artery, whereby an opening formed in the artery wall is gradually enlarged by the increasing cross sectional size of the protuberance 20 so that the elongate tube 12 can be removed generally without causing further trauma to the artery. Pressure may be applied to the femoral artery at a distal location to assist in passing of the protuberance

through the artery wall so that the elongate tube can be withdrawn.

**[0078]** The foregoing description of the embodiments has been provided for purposes of illustration and description. It is not intended to be exhaustive or to limit the disclosure. Individual elements or features of a particular embodiment are generally not limited to that particular embodiment, but, where applicable, are interchangeable and can be used in a selected embodiment, even if not specifically shown or described. The same may also be varied in many ways. Such variations are not to be regarded as a departure from the disclosure, and all such modifications are intended to be included within the scope of the disclosure.

### Claims

1. A bi-directional perfusion cannula (10) comprising an elongate tube (12) for insertion into an artery, the elongate tube (12) comprising:

a first aperture (14) at a distal end of the elongate tube (12) which is forward during insertion, the first aperture (14) being configured so that blood can flow into the artery (21) in the direction of insertion;

an elbow (16) preformed in the elongate tube (12); and

a second aperture (18), the second aperture (18) being formed in or slightly rearward of the elbow (16) and configured for supplying blood into the artery in a second direction which is generally opposite to the insertion direction, wherein the elbow (16) is preformed in the elongate tube such that in a relaxed state prior to insertion the cannula has an elbow bend formed in it, preferably in the range of 90 to 180 degrees, and

wherein said elongate tube (12) has a protuberance at least partially formed on the elbow (16), the bi-directional perfusion cannula (10) being **characterized in that** the protuberance is ovoid in cross section.

2. The bi-directional perfusion cannula (10) according to claim 1, wherein said elbow bend is 180 degrees.
3. The bi-directional perfusion cannula (10) according to Claim 1, wherein the protuberance extends along an outer surface of the elbow (16).
4. The bi-directional perfusion cannula (10) according to any of Claims 1 and 3, wherein the second aperture (18) extends through the protuberance.
5. The bi-directional perfusion cannula (10) according to any of Claims 1 and 3, 4, wherein the second ap-

erture (18) extends in a direction generally away from the forward end of the elongated tube (12).

6. A bi-directional perfusion cannula (10) according to any of Claims 1 and 3 to 5, wherein the protuberance (20) and elbow (16) form a transition zone which splints open the artery.
7. A bi-directional perfusion cannula (10) according to Claim 6, wherein the transition zone is inflatable.
8. A bi-directional perfusion cannula (10) according to any of Claims 1 and 3 to 7, wherein the protuberance (20) tapers in the insertion direction to allow insertion of the cannula (10) in the artery (21).
9. A bi-directional perfusion cannula (10) according to Claim 1, wherein the elongate tube (12) is configured to receive an elongate introducer (22) therethrough to aid in insertion of the cannula (10) and prevent blood flow through the first aperture (14) whilst the elongate tube (12) and introducer (22) are inserted into an artery (21).

### Patentansprüche

1. Bidirektionale Perfusionskanüle (10) mit einem länglichen Schlauch (12) zum Einführen in eine Arterie, wobei der längliche Schlauch (12) aufweist:

eine erste Öffnung (14), die an einem distalen Ende des länglichen Schlauchs (12) ausgebildet ist und welche während des Einführens nach vorne gerichtet ist, wobei die erste Öffnung (14) derartig ausgebildet ist, dass Blut in der Einführungsrichtung in die Arterie (21) fließen kann; ein Winkelabschnitt (16), der in dem länglichen Schlauch (12) vorgeformt ist; und eine zweite Öffnung (18), wobei die zweite Öffnung (18) in oder leicht hinter dem Winkelabschnitt (16) ausgebildet und dazu ausgestaltet ist, Blut in einer zweiten Richtung, die im Allgemeinen entgegengesetzt zur Einführungsrichtung ist, in die Arterie zuzuführen,

wobei der Winkelabschnitt (16) in dem länglichen Schlauch derartig vorgeformt ist, dass die Kanüle in einem entspannten Zustand vor der Einführung mit einer Winkelabschnittbiegung ausgebildet ist, die vorzugsweise im Bereich von 90 - 180° liegt, und wobei der längliche Schlauch (12) einen Vorsprung aufweist, der zumindest abschnittsweise an dem Winkelabschnitt (16) ausgebildet ist, wobei die bidirektionale Perfusionskanüle (10) **dadurch gekennzeichnet ist, dass** der Vorsprung im Querschnitt eiförmig ausgebildet ist.

2. Bidirektionale Perfusionskanüle (10) nach Anspruch 1, **dadurch gekennzeichnet, dass** die Winkelabschnittsbiegung 180° beträgt.
3. Bidirektionale Perfusionskanüle (10) nach Anspruch 1, **dadurch gekennzeichnet, dass** sich der Vorsprung entlang einer Außenfläche des Winkelabschnitts (16) erstreckt. 5
4. Bidirektionale Perfusionskanüle (10) nach einem der Ansprüche 1 oder 3, **dadurch gekennzeichnet, dass** sich die zweite Öffnung (18) durch den Vorsprung erstreckt. 10
5. Bidirektionale Perfusionskanüle (10) nach einem der Ansprüche 1, 3 oder 4, **dadurch gekennzeichnet, dass** sich die zweite Öffnung (18) in eine Richtung erstreckt, die im Wesentlichen weg vom vorderen Ende des länglichen Schlauchs (12) weist. 15
6. Bidirektionale Perfusionskanüle (10) nach einem der Ansprüche 1 und 3 bis 5, **dadurch gekennzeichnet, dass** der Vorsprung (20) und der Winkelabschnitt (16) eine Übergangzone bilden, die die Arterie offenhält. 20
7. Bidirektionale Perfusionskanüle (10) nach Anspruch 6, **dadurch gekennzeichnet, dass** die Übergangzone aufblasbar ist. 25
8. Bidirektionale Perfusionskanüle (10) nach einem der Ansprüche 1 oder 3 bis 7, **dadurch gekennzeichnet, dass** der Vorsprung (20) sich in die Einführungsrichtung verjüngt, um die Einführung der Kanüle (10) in die Arterie (21) zu ermöglichen. 30
9. Bidirektionale Perfusionskanüle (10) nach Anspruch 1, **dadurch gekennzeichnet, dass** der längliche Schlauch (12) dazu ausgestaltet ist, eine längliche Einführeinrichtung (22) aufzunehmen, um das Einführen der Kanüle (10) zu unterstützen und um einen Blutfluss durch die erste Öffnung (14) zu verhindern, während der längliche Schlauch (12) und die Einführeinrichtung (22) in die Arterie (21) eingeführt werden. 35 40 45

## Revendications

1. Canule de perfusion bidirectionnelle (10) comprenant un tube allongé (12) à insérer dans une artère, le tube allongé (12) comprenant :
- une première ouverture (14) au niveau d'une extrémité distale du tube allongé (12) qui se trouve en avant pendant l'insertion, la première ouverture (14) étant configurée de sorte que le sang puisse s'écouler dans l'artère (21) dans le sens de l'insertion ; un coude (16) préformé dans le tube allongé (12) ; et une deuxième ouverture (18), la deuxième ouverture (18) étant formée dans ou légèrement en arrière du coude (16) et configurée pour amener du sang dans l'artère dans une deuxième direction qui est généralement opposée à la direction d'insertion, dans laquelle le coude (16) est préformé dans le tube allongé de sorte que dans un état détendu avant l'insertion, la canule ait une courbure de coude formée dans celle-ci, de préférence comprise dans la plage allant de 90 à 180 degrés, et dans laquelle ledit tube allongé (12) a une protubérance formée au moins partiellement sur le coude (16), la canule de perfusion bidirectionnelle (10) étant **caractérisée en ce que** la protubérance est de section ovoïde.
2. Canule de perfusion bidirectionnelle (10) selon la revendication 1, dans laquelle ladite courbure de coude est de 180 degrés.
3. Canule de perfusion bidirectionnelle (10) selon la revendication 1, dans laquelle la protubérance s'étend le long d'une surface externe du coude (16).
4. Canule de perfusion bidirectionnelle (10) selon l'une des revendications 1 et 3, dans laquelle la deuxième ouverture (18) s'étend à travers la protubérance.
5. Canule de perfusion bidirectionnelle (10) selon l'une des revendications 1, 3 et 4, dans laquelle la deuxième ouverture (18) s'étend dans une direction généralement éloignée de l'extrémité avant du tube allongé (12).
6. Canule de perfusion bidirectionnelle (10) selon l'une des revendications 1 et 3 à 5, dans laquelle la protubérance (20) et le coude (16) forment une zone de transition qui ouvre l'artère à l'aide d'attelle.
7. Canule de perfusion bidirectionnelle (10) selon la revendication 6, dans laquelle la zone de transition est gonflable.
8. Canule de perfusion bidirectionnelle (10) selon l'une des revendications 1 et 3 à 7, dans laquelle la protubérance (20) se rétrécit dans la direction d'insertion pour permettre l'insertion de la canule (10) dans l'artère (21).
9. Canule de perfusion bidirectionnelle (10) selon la revendication 1, dans laquelle le tube allongé (12) est configuré pour recevoir un dispositif d'introduction

allongé (22) à travers celui-ci pour faciliter l'insertion de la canule (10) et empêcher un écoulement de sang à travers la première ouverture (14) lorsque le tube allongé (12) et le dispositif d'introduction (22) sont insérés dans une artère (21).

5

10

15

20

25

30

35

40

45

50

55

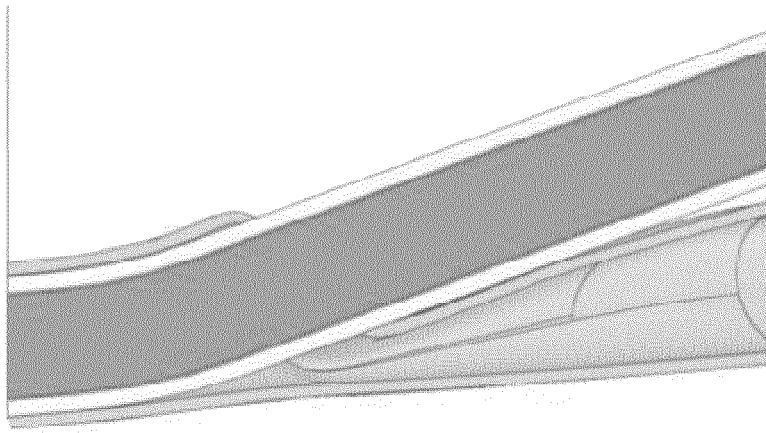


Figure 1

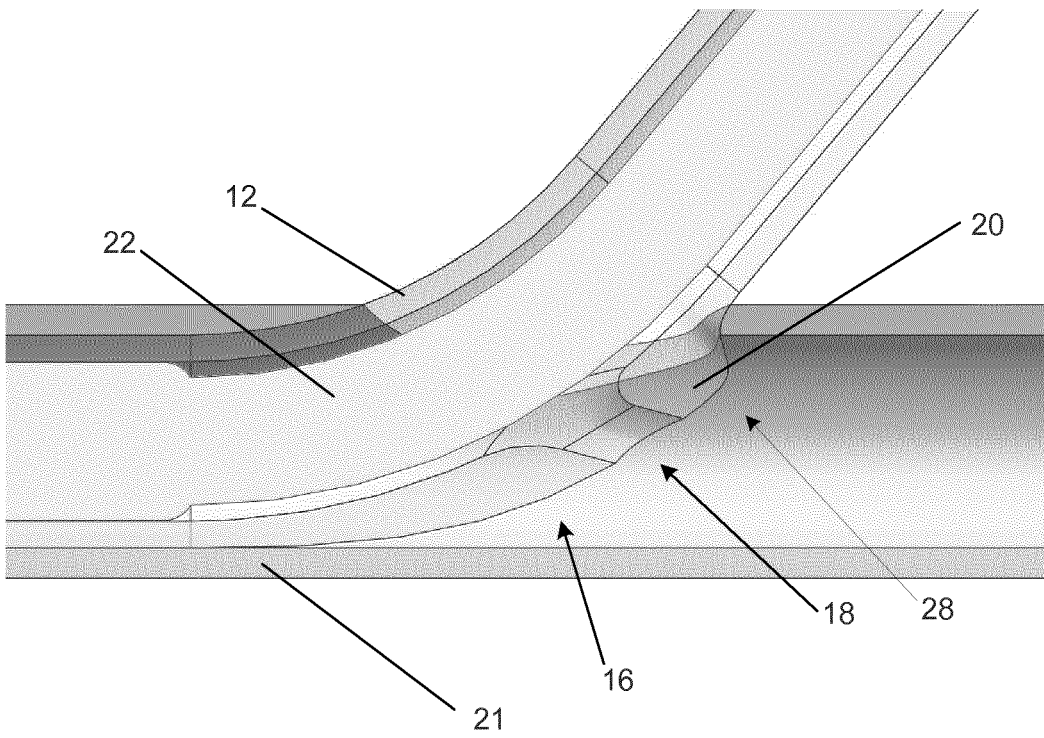


Figure 7

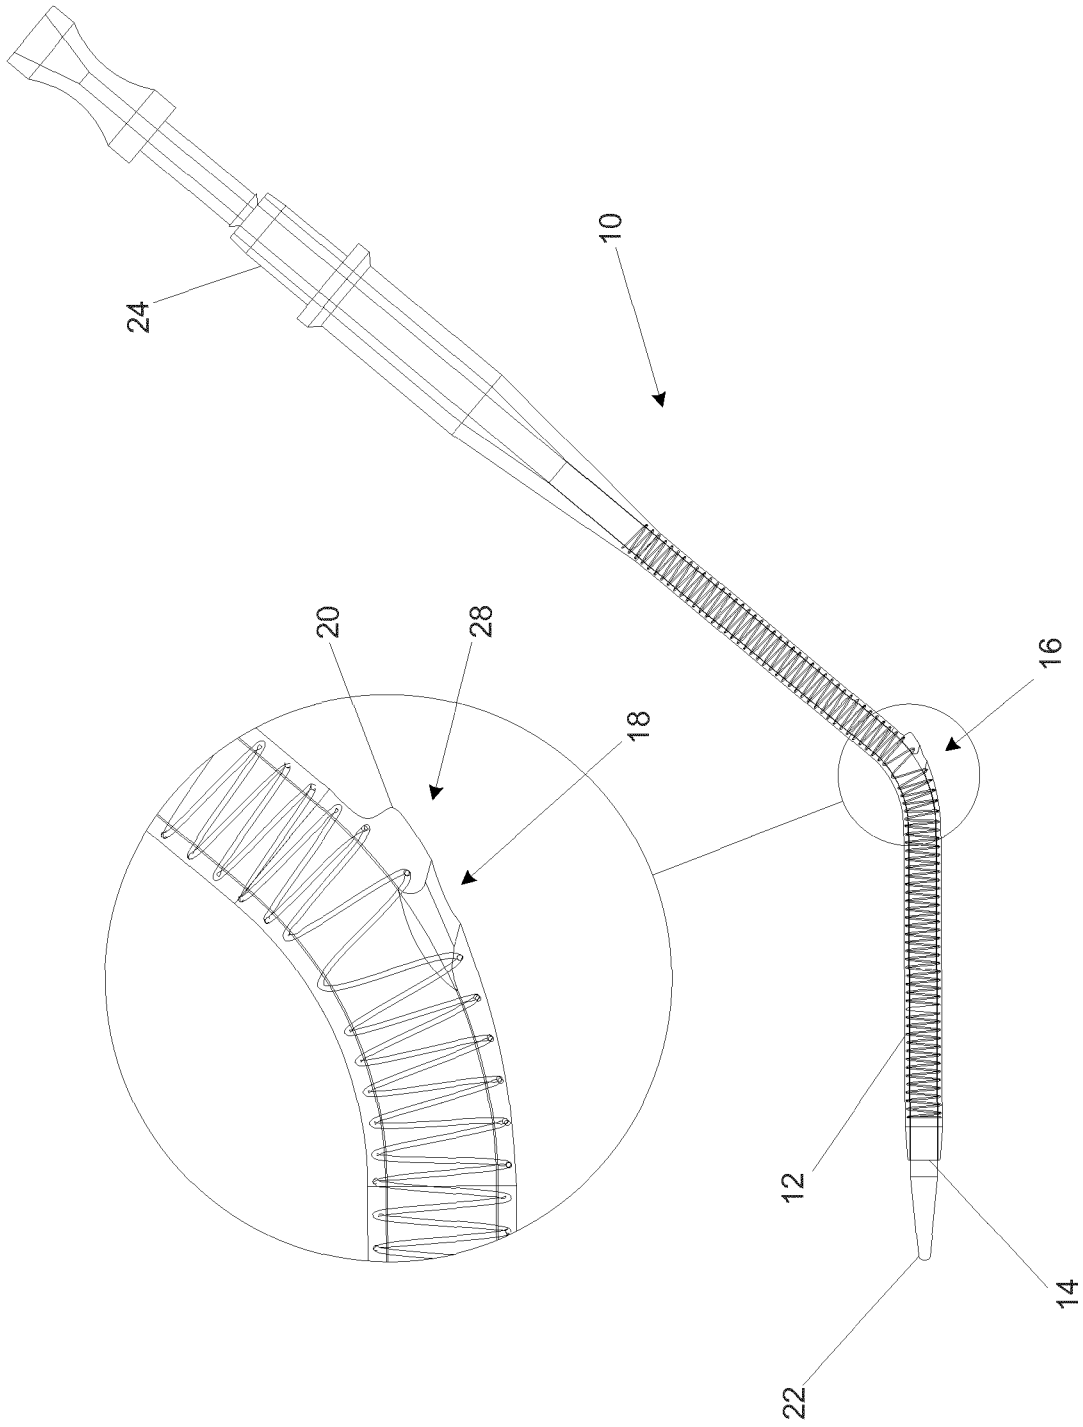
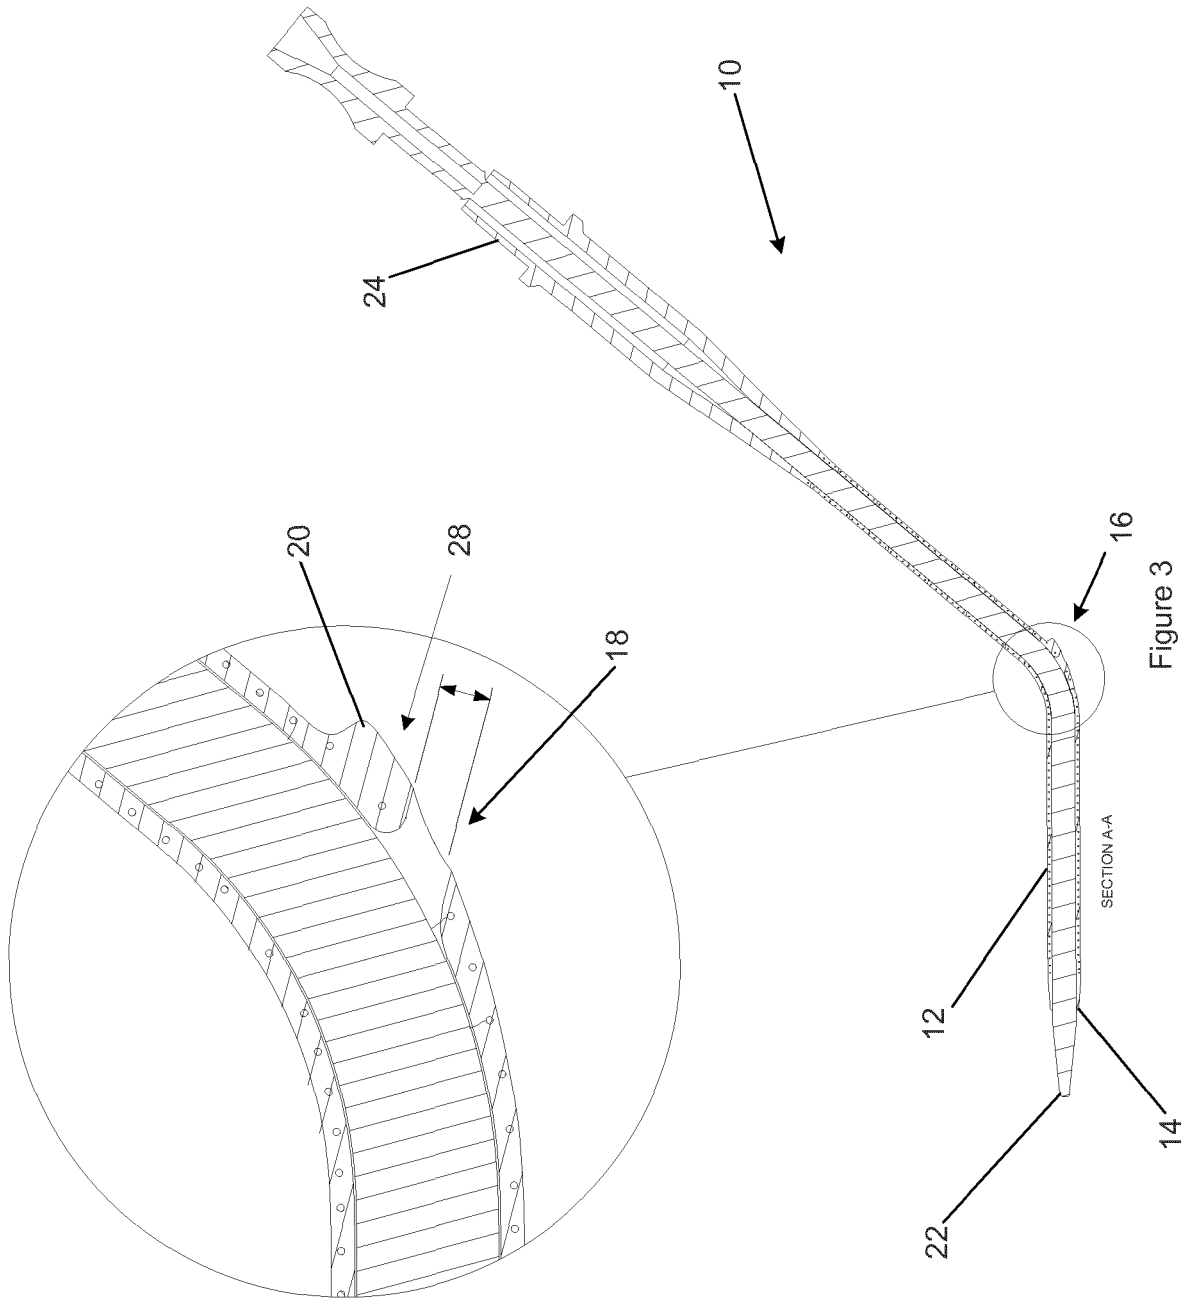


Figure 2



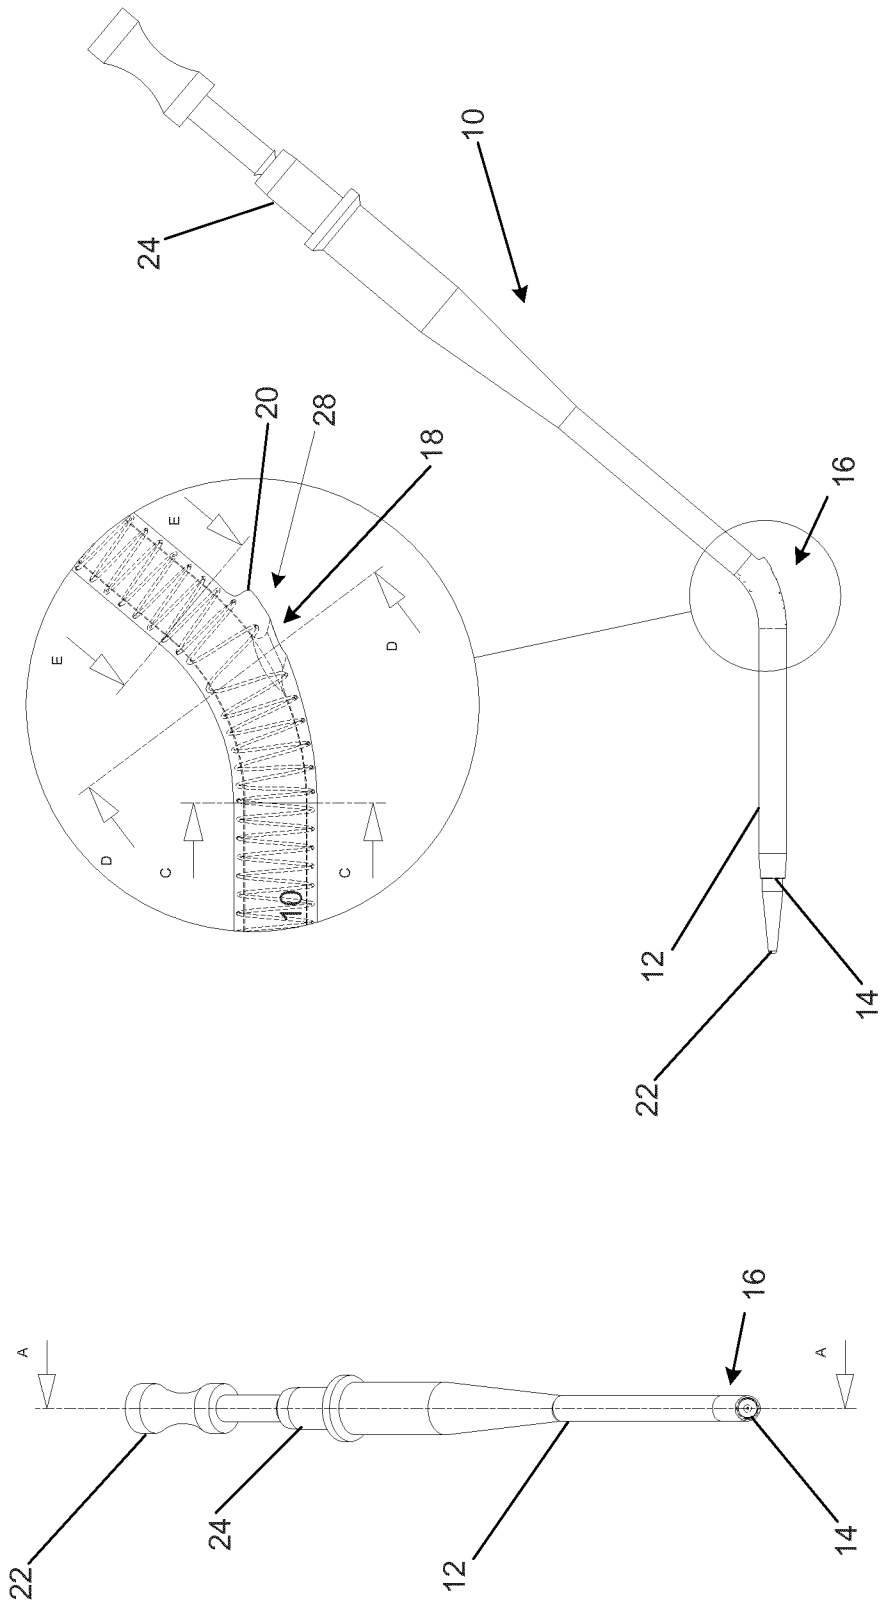


Figure 5

Figure 4

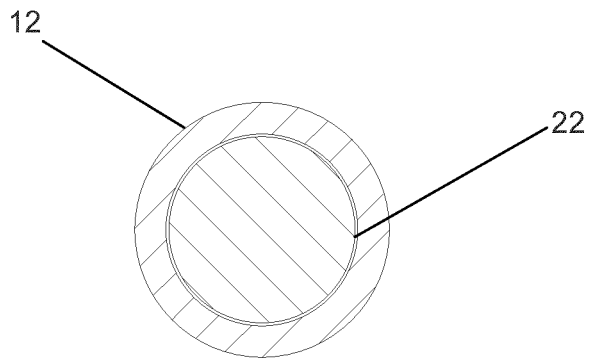


Figure 6A  
Section C-C

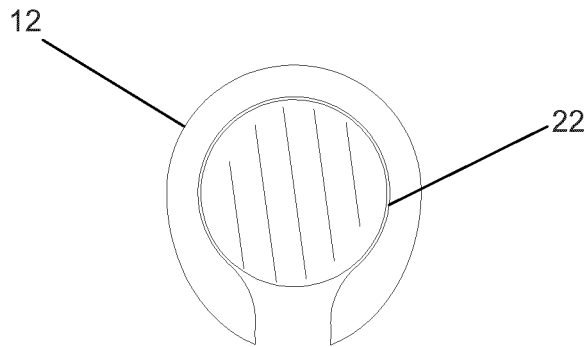


Figure 6B  
Section D-D

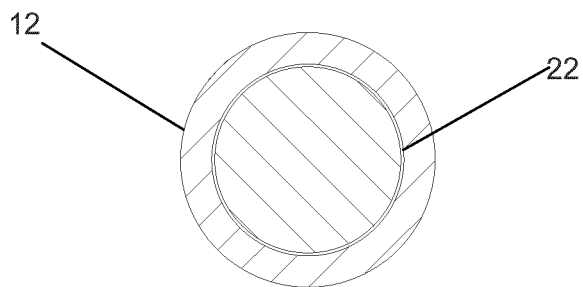


Figure 6C  
Section E-E

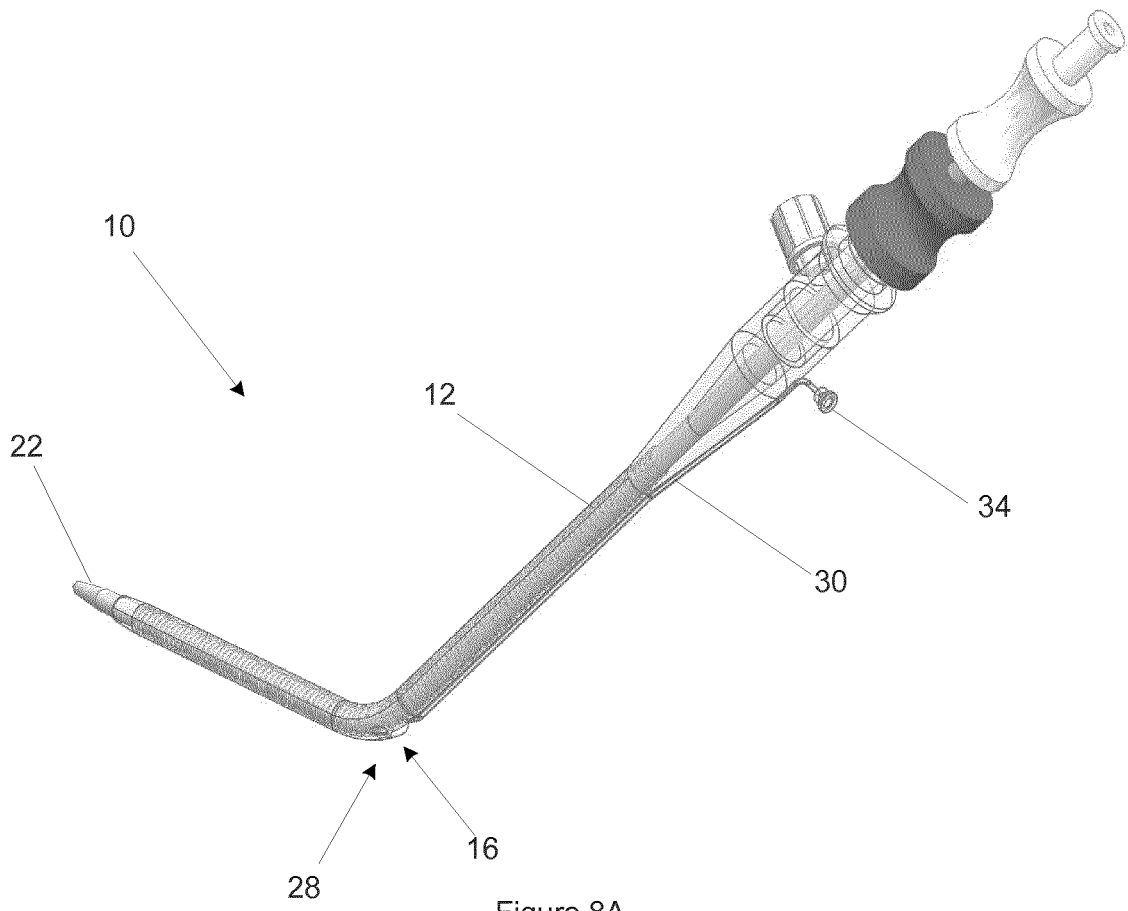


Figure 8A

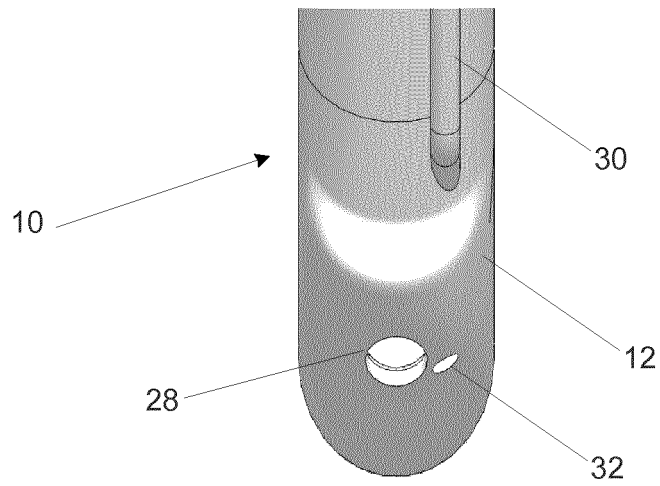


Figure 8B

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 4114618 A [0001]
- US 5171218 A [0001] [0011]
- WO 2005037345 A1 [0001]
- WO 03068303 A, Laksen [0009]
- US 5330433 A, Fonger, J. [0011]

**Non-patent literature cited in the description**

- **MATSUI et al.** A Novel Femoral Arterial Cannula to Prevent Limb Ischemia During Cardiopulmonary Support: Preliminary Report of Experimental and Clinical Experiences. *Artif Organs*, 2006, vol. 30 (7) [0009]
- **MAGOVERN, J. et al.** A femoral artery cannula that allows distal blood flow. *The Journal of Thoracic and Cardiovascular Surgery*, September 2005 [0010]

|                |   |         |            |
|----------------|---|---------|------------|
| 专利名称(译)        | 双向灌注插管  |         |            |
| 公开(公告)号        | <a href="#">EP3492133B1</a>   | 公开(公告)日 | 2020-06-10 |
| 申请号            | EP2019150583  | 申请日     | 2012-04-04 |
| [标]申请(专利权)人(译) | 索林集团意大利有限责任公司   |         |            |
| 申请(专利权)人(译)    | 索林集团ITALIA S.R.L.   |         |            |
| 当前申请(专利权)人(译)  | 索林集团ITALIA S.R.L.   |         |            |
| [标]发明人         | MOSHINSKY RANDALL<br>MCMILLAN JAMES<br>TUTUNGI ELLI   |         |            |
| 发明人            | MOSHINSKY, RANDALL<br>MCMILLAN, JAMES<br>TUTUNGI, ELLI  |         |            |
| IPC分类号         | A61M25/00 A61B5/00 A61B5/021 A61M1/36 A61B5/0215  |         |            |
| CPC分类号         | A61B5/02141 A61B5/0215 A61B5/6847 A61M25/0041 A61M25/0043 A61M25/007 A61M2025/006 F04C2270/041 A61M1/3659 |         |            |
| 优先权            | 2011901258 2011-04-05 AU<br>2011902210 2011-06-03 AU<br>PCT/AU2012/000347 2012-04-04 WO                   |         |            |
| 其他公开文献         | EP3492133A1   |         |            |
| 外部链接           | <a href="#">Espacenet</a>   |         |            |

摘要(译)

本文公开了一种包括用于插入动脉中的细长管 ( 12 ) 的双向灌注套管 ( 10 ) , 该细长管 ( 12 ) 在细长管的远端处包括第一孔 ( 14 ) , 该第一孔在该过程中是向前的。插入, 第一孔被构造使得血液可以在插入方向上流入动脉 ( 21 ) ; 在细长管中形成的肘部 ( 16 ) ; 第二孔 ( 18 ) , 该第二孔形成在肘部中或稍稍向后, 并构造用于沿与插入方向大致相反的第二方向向动脉供血, 其中, 肘部在细长管中预形成 因此, 在插入之前, 在松弛状态下, 插管具有弯头。

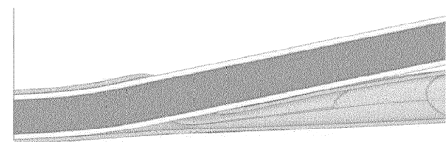


Figure 1

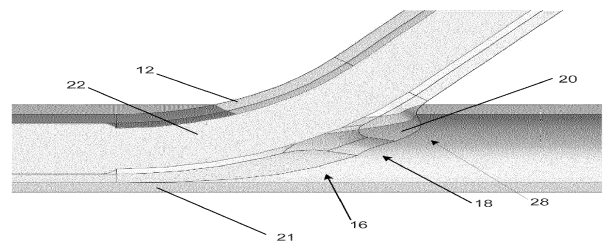


Figure 7