



(11) **EP 1 693 000 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
08.05.2013 Bulletin 2013/19

(51) Int Cl.:
A61B 5/00 (2006.01) **A61B 1/05** (2006.01)
H04L 25/03 (2006.01)

(21) Application number: **06010954.3**

(22) Date of filing: **08.03.2001**

(54) **A device for in vivo imaging**

Vorrichtung zur Invivo-Bildgebung

Dispositif d'imagerie in vivo

(84) Designated Contracting States:
**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE TR**

(30) Priority: **08.03.2000 US 187883 P**

(43) Date of publication of application:
23.08.2006 Bulletin 2006/34

(62) Document number(s) of the earlier application(s) in
accordance with Art. 76 EPC:
01912088.0 / 1 263 318

(73) Proprietor: **Given Imaging Ltd.**
20692 Yoqneam (IL)

(72) Inventors:
• **Iddan, Gavriel**
34602 Haifa (IL)
• **Avni, Dov**
34525 Haifa (IL)
• **Glukhovsky, Arkady**
36790 Neshet (IL)
• **Meron, Gavriel**
49556 Kfar Ganim
Petach Tikva (IL)

(74) Representative: **HOFFMANN EITLE**
Patent- und Rechtsanwälte
Arabellastrasse 4
81925 München (DE)

(56) References cited:
EP-A- 0 677 272 DE-A1- 3 440 177
US-A- 4 278 077 US-A- 4 416 283
US-A- 5 749 367

- **ZIAIE B ET AL: "A low-power miniature transmitter using a low-loss silicon platform for biotelemetry" PROCEEDINGS OF THE 19TH ANNUAL INTERNATIONAL CONFERENCE OF THE IEEE ENGINEERING IN MEDICINE AND BIOLOGY SOCIETY. MAGNIFICENT MILESTONES AND EMERGING OPPORTUNITIES IN MEDICAL ENGINEERING' (CAT. NO. 97CH36136) IEEE PISCATAWAY, NJ, USA, vol. 5, 1997, pages 2221-2224 vol., XP002389551 ISBN: 0-7803-4262-3**
- **HEUBERGER A ET AL: "Integrated RF transmitter based on SAW oscillator" SOLID-STATE CIRCUITS CONFERENCE, 1997. ESSCIRC '97. PROCEEDINGS OF THE 23RD EUROPEAN SOUTHAMPTON, UK 16-18 SEPT. 1997, PISCATAWAY, NJ, USA, IEEE, 16 September 1997 (1997-09-16), pages 344-347, XP010823381 ISBN: 2-86332-220-6**
- **SWAIN P ET AL: "Wireless capsule endoscopy of the small-bowel. Development, testing and first human trials", PROCEEDINGS OF SPIE - THE INTERNATIONAL SOCIETY FOR OPTICAL ENGINEERING 2001 SPIE US, vol. 4158, 5 July 2000 (2000-07-05), pages 19-23, DOI: DOI: 10.1117/12.413789**
- **GONG F ET AL: "Wireless endoscopy.", GASTROINTESTINAL ENDOSCOPY JUN 2000 LNKD- PUBMED:10840312, vol. 51, no. 6, June 2000 (2000-06), pages 725-729, ISSN: 0016-5107**
- **FOSSUM E R: "CMOS image sensors: electronic camera-on-a-chip", IEEE TRANSACTIONS ON ELECTRON DEVICES IEEE USA, vol. 44, no. 10, October 1997 (1997-10), pages 1689-1698, ISSN: 0018-9383**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 1 693 000 B1

Description

FIELD OF THE INVENTION

[0001] The present invention relates to a transmitter in an in vivo imaging device such as for imaging the digestive tract.

BACKGROUND OF THE INVENTION

[0002] Among known in vivo measuring systems are endoscopes, which are often utilized to provide images of the upper or lower gastro-intestinal tract. However, endoscopes do not provide views of the entire length of the small intestines. Additionally, they are uncomfortable, may cause damage to the patient and are complex to operate.

[0003] Swallowable electronic capsules which are moved through the digestive tract through the action of digestion and which collect data and transmit the data to a receiver system are known, one such example is the "Heidelberg" capsule. Yet another example is a capsule disclosed in US 5,604,531. These capsules may be utilized to measure pH, temperature and pressure throughout the intestines.

[0004] "A low-power miniature transmitter using a low-loss silicon platform for biotelemetry" by Babak Ziaie et al, Proceedings/19th International Conference-IEEE/EMBS October 30/November 2, 1997, Chicago, Illinois, USA (XP-002389551) describes a low-loss transmitter that can be used in a small, totally implantable system in laboratory animals, and can transmit for several months.

[0005] "Integrated RF transmitter based on SAW oscillator" by A. Heuberger et al, XP010823381 describes a low power and low cost RF transmitter that can operate at 433 MHz.

[0006] US-5,749,367 describes a heart monitoring apparatus and method that can transmit at 433 or 458 MHz.

[0007] US-5,833,603 describes in one embodiment an implantable biosensing transponder that is capsule shaped, having a lens formed on one end and a CMOS imager. After implantation, the external environment is externally illuminated with an optical source operating at a wavelength that readily penetrates tissue. Optical energy reflected from tissue in the external environment will then be focussed onto the imager by the lens. In a different embodiment, US-5,833,603 describes an implantable biosensing transponder that comprises optical emitters and a photosensor.

Summary of the invention

[0008] The present invention relates to a swallowable capsule for in vivo imaging as described in claim 1. Advantageous embodiments are described in the dependent claims.

[0009] The device of the invention can be used for obtaining in vivo images from within body lumens or cavities,

such as images of the entire length of the gastrointestinal (GI) tract. The device contains an imaging system that includes a complementary metal oxide semiconductor (CMOS) imaging camera. The transmitter can be an ultra low power radio frequency (RF) transmitter for transmitting signals from the CMOS imaging camera to a receiving system.

[0010] The CMOS imaging camera is an ultra low power imager, has low sensitivity to the red spectrum and is provided in chip scale packaging (CSP). The transmitter is an ultra low power RF transmitter with high bandwidth input, possibly provided in chip scale packaging.

[0011] The high integration and low power consumption achieved by the imaging system of the device were unobtainable prior to the advances in CMOS technology. Further, the ultra low power, high bandwidth input transmitter for video signals is unknown in the art. Also, an RF product in CSP has not been previously disclosed in the art.

[0012] Further, the imaging system may utilize a white light emitting diode (LED) as a light source rather than a reddish incandescence miniature bulb or an RGB LED presently used in the art. The white LED enables to produce a higher quality and more pleasant to the eye image.

[0013] There is therefore provided, an in vivo imaging device. The device consists of at least one imaging system for producing video output, preferably digital output, and a transmitter which transmits the video output to a receiving system.

[0014] The imaging system includes a CMOS imaging camera, at least one illumination source for illuminating an in vivo site and an optical system for imaging the in vivo site onto the CMOS imaging camera.

[0015] The illumination source may be a white LED. The term "white LED" as referred to herein relates to a combination of a blue LED chip (emitting light in the blue spectrum range) and a refracting crystal. The blue LED chip is encapsulated within the refracting crystal such that blue light incident on the crystal is emitted in different spectrums, resulting in white light. The white light emitted from the refracting crystal has a small fraction of red light and an even smaller, almost nonexistent, fraction of infra red (IR) light.

[0016] The illumination source may be a specific integrated light source in which a refracting crystal matrix has a plurality of blue LED chips integrated therein.

[0017] The components of the device are harbored in a housing having an optical window. The housing is configured for being inserted and passing through body lumens or cavities.

[0018] Also provided, is a system for in vivo imaging, which includes an imaging system producing video output, preferably digital output, a transmitter which transmits the video output of the imaging system and a receiving system for receiving the transmitted video output. The imaging system consists of a CMOS imaging camera, an illumination source for illuminating an in vivo site and an optical system for imaging the in vivo site onto the CMOS

imaging camera.

[0019] The system may further comprise an antenna array capable of surrounding a body and comprising one or a plurality of antennas for receiving the transmitted video output and for producing a plurality of received signals. Also the system may include a demodulator capable of transforming the plurality of received video signals into a single video datastream. The system may also comprise a data processing system which generates tracking and video data from the single datastream.

[0020] The receiving system and data processor are typically located outside a patient.

[0021] Optionally, the system can also include an apparatus for operating the transmitter intermittently.

[0022] The imaging system consists of a CMOS imaging camera, a white LED and a lens for imaging a GI tract site onto the CMOS imaging camera. The swallowable capsule also includes a contained energy source for providing energy the entirety of the electrical elements of the capsule.

[0023] Also provided is a transmitter for transmitting signals on RF to a receiving system. The transmitter, which is controlled by a normally opened (NO) switch, includes a control block for controlling the illumination and imager of the device of the invention.

[0024] The NO switch is controlled by an external magnet that keeps the switch closed while it is in proximity to the switch. However, an internal block maintains the logistics of an open switch, so as to keep the transmitter circuits and all capsule main subsystems inactive while the external magnet is present. Removal of the external magnet causes the switch to open and the internal block to close, thereby allowing the transmitter circuits and capsule main subsystems to be activated.

[0025] Further provided is a method for obtaining images in vivo. The method includes the steps of: illuminating a site in vivo; collecting remitted light onto pixels of a CMOS imaging camera, thereby generating an analog signal; processing and converting the analog signal to a digital signal; randomizing the digital signal; transmitting the digital signal to a receiving system; and processing the transmitted signals to obtain images of the in vivo site.

BRIEF DESCRIPTION OF THE DRAWINGS

[0026] The present invention will be understood and appreciated more fully from the following detailed description taken in conjunction with the drawings in which:

Figure 1 is a schematic longitudinal cross section illustration of an in vivo imaging device;

Figure 2 is a schematic presentation of the CMOS imaging camera;

Figure 3 is a cross section schematic illustration of a device, including a specific integrated illumination source;

Figure 4 is a block diagram of the transmitter in accordance with an embodiment of the invention; and

Figure 5 is a block diagram presentation of a method for obtaining images.

DETAILED DESCRIPTION OF THE INVENTION

[0027] The device and system to be described are utilized for viewing inside body lumens and cavities and for transmitting at least video data.

[0028] Reference is now made to Fig.1 which illustrates the device and its components. The device 10 typically comprises an optical window 21 and an imaging system for obtaining images from inside a body lumen, such as the GI tract. The imaging system includes an illumination source 23, such as a white LED, a CMOS imaging camera 24, which detects the images and an optical system 22 which focuses the images onto the CMOS imaging camera 24. The illumination source 23 illuminates the inner portions of the body lumen through optical window 21. Device 10 further includes a transmitter 26 and an antenna 27 for transmitting the video signal of the CMOS imaging camera 24, and a power source 25, such as a silver oxide battery, that provides power to the electrical elements of the device 10.

[0029] It will be appreciated that a plurality of CMOS imaging cameras may be used in the device and system. Each CMOS imaging camera may include its own optical system and either one or more illumination sources, in accordance with specific requirements of the device or system.

[0030] Images obtained by the CMOS camera 24 are transmitted to a receiving system (not shown), which may also include a data processing unit. The receiving system and data processing unit are typically located outside a patient.

[0031] The device 10 is capsule shaped, can be easily swallowed and may passively pass through the entire GI tract, pushed along by natural peristalsis.

[0032] Nonetheless, it should be appreciated that the device may be of any shape suitable for being inserted into and passing through a body lumen or cavity. Furthermore, the device may be attached or affixed on to an instrument that is inserted into body lumens and cavities, such as on an endoscope, laparoscope, stent, needle, catheter etc.

[0033] Thus, the device may be introduced into a body lumen or cavity by swallowing, by using an endoscopic device, by surgery and so on.

[0034] A suitable CMOS imaging camera 24 is, for example, a "camera on a chip" type CMOS imager specified by Given Imaging Ltd. of Yokneam, Israel and designed by Photobit Corporation of California, USA, with integrated active pixel and post processing circuitry (as will be further described with reference to Fig. 2). The single chip camera can provide either black and white or color signals.

[0035] The CMOS imaging camera 24 is designed such that it is less sensitive to light in the red spectrum than known CMOS cameras.

[0036] The optical system 22 comprises at least one lens and optionally mirrors and/or prisms for collecting and collimating remitted light on to the pixels of the CMOS imaging camera 24. Typically, the optical system comprises an aspherical focussing lens. A suitable lens is, for example, the lens designed by Given Imaging Ltd. of Yokneam, Israel, in accordance with specific object plane, distortion and resolution parameters.

[0037] Illumination source 23, transmits illumination to the walls of the body lumen via the optical window 21. The lens of the optical system 22 then focuses remittent light onto the pixels of the CMOS imaging camera 24.

[0038] A single or plurality of light sources or a specific integrated light source may be used and positioned in accordance with specific imaging requirements, such as to avoid stray light etc. Also, the optical window 21 may be positioned and shaped according to the device shape and according to specific imaging requirements. For example, optimized imaging conditions can be obtained when optical window 21 is formed to define an ellipsoid shaped dome and the CMOS imaging chip camera system 24 and illumination sources 23 are positioned in the proximity of the focal plane of the shape defined by the optical dome. Obtaining the above imaging conditions is described in WO 00/76391.

[0039] The in vivo sites imaged are usually very close to the imager. For example, an 11 x 30mm capsule passing through and imaging the small intestine, images the intestine walls from a very short distance. It is therefore possible to satisfy the illumination requirements of the imaging process utilizing solid state illumination sources, such as LEDs.

[0040] In an example the illumination source is a white LED. The white light emitted from the white LED has a small fraction of red light and even smaller fraction of IR light. Hence, a white LED is beneficial for use with silicone based image sensors (such as CMOS imaging cameras) because of the silicone sensitivity to red and IR light.

[0041] In a system which includes the CMOS imaging camera with its reduced sensitivity to light in the red spectrum and a white LED illumination source, no IR reject filters (photopic filters) are needed.

[0042] A suitable transmitter may comprise a modulator which receives the video signal (either digital or analog) from the CMOS imaging camera, a radio frequency (RF) amplifier, an impedance matcher and an antenna. A transmitter will be further illustrated in Fig. 4.

[0043] Other optional parts of the system as well as the method for localization of a capsule containing the system within the digestive system may be similar to those described in US 5,604,531 (which is assigned to the common assignees of the present invention and which is hereby incorporated in its entirety by reference).

[0044] Device 10 can additionally include sensor elements for measuring pH, temperature, pressure, etc. These sensor elements, some of which are described in the prior art, may be any element suitable for measuring conditions prevailing in the body lumen (for example, the

digestive system) and that are capable of being appended to or included in the device.

[0045] Reference is now made to Fig. 2, in which a schematic layout of the CMOS imaging camera is presented. The CMOS imaging camera 200 comprises active pixel and post processing circuitry on a single chip. The CMOS imaging camera 200 includes photo cell 202 (the pixels of the CMOS imaging camera), correlated double sampler (CDS) 204, analog to digital (A/D) converter 206, encoding and randomizing unit 208 and timing generator 210 for control and synchronization of the circuitry elements.

[0046] Light collected by an optical system is directed onto CMOS imaging camera 200 and photons are converted to electrons as the light is absorbed by photo cell 202. Electrons are converted to electrical current and an analog signal is produced by the active pixel circuitry. The analog signal is conveyed for further processing by on-chip post processing circuitry. The signal is further processed by CDS 204. CDS 204 performs correlated double sampling, for canceling noise and signal shaping before conveying the signal to the A/D converter 206. The A/D converter 206 is a serial output A/D converted which enables serial, low power transmission of signals.

The signal is converted into a digital signal and is further conveyed to encoding and randomizing unit 208 for defining frame and row parameters (encoding) and for priming the signals for transmission (randomizing). The encoding and randomizing unit 208 randomizes the occurrence of the digital "0" and "1" signals such that transmission is not impeded by a reoccurring signal of one type.

[0047] The CMOS imaging camera 200 is specified by Given Imaging Ltd. of Yokneam, Israel and designed by Photobit Corporation of California, USA, according to a specification adjusted to in vivo imaging. The CMOS imaging chip has ultra low power requirements (less than 3 milliwatts). The dynamics of the increase of dark current generated by the imaging camera, as a function of temperature, is less than that of solid state devices known in the art, such that at 37°C a low fraction of the out put video signal is dark current. Further, as discussed above, the imaging camera has reduced sensitivity to light in the red spectrum, abating the need for photopic filters.

[0048] Reference is now made to Fig. 3 in which a device for in vivo imaging comprising a specific integrated light source is illustrated. Device 300 comprises CMOS imaging camera 302, an optical system (not shown) for imaging in vivo images onto the CMOS imaging camera 302 and an integrated light source 304 for illuminating a site in vivo. The device 300 further includes a transmitter 305 for transmitting video data from the imaging camera 302 to a receiver (not shown). The transmitter 305 generates a high voltage and current source for the light source 304. The integrated light source 304 is connected to the transmitter 305 through connective wires 301. The electrical components of the device are powered by a battery contained within the device (not shown).

[0049] The integrated light source 304 comprises a strip 306 of a refracting crystal matrix encircling the CMOS imaging camera 302. Blue LED chips 308, encapsulated within the refracting crystal matrix of strip 306, are positioned along the strip 306 such that illumination is provided in a ring around the CMOS imaging camera 302.

[0050] Blue LED chips 308 can also be sprinkled throughout the strip 306 such that the whole strip 306 emits light.

[0051] Reference is now made to Fig. 4 in which a block diagram of the transmitter is shown. The transmitter 400, an ASIC (application specific integrated circuit) designed to fulfill international communication standards (such as the FCC) standards, operates on a minimum shift keying (MSK) modulation system to effect transmitting of digital signals through antenna 426 and 427 on radio frequencies to a receiving system. The transmitter 400 also controls the illumination and imager of the device of the invention and the logical conversion of the switch (as described above). The transmitter 400 includes a one time programming unit 408 in communication with external programming input 428, a control logic block 401 for communicating with the imager, a phase lock loop (PLL) 402 in communication with modulator 425, optionally, a LED power and control block 403 for controlling the illumination, a main oscillator 404 and a switch 405 which controls an internal electronic switch 406.

[0052] The control logic block 401 communicates with the imager, reads preprogrammed parameters and performs the interface to the "outside" world in the programming mode. Control logic block 401 maintains a master clock, is synchronized by bit rate data 412 and frame rate 413, and through control 411, which is generated by the imager, triggers LED power and control block 403. Control logic block 401 further controls the master clock 414 and the imager shutdown 415.

[0053] During shutdown the transmitter sends out beacon signals only. The shutdown enables economic use of the device's power supply. For example, in a device designed for imaging the small intestine, the transmitter 400 may be programmed to include a two hour delay, during which period shutdown of the imager and other device electronics is effected. Two hours is approximately the time it takes a swallowable device to pass the stomach and enter the small intestine, in particular patients. Thus, in those patients, the device will utilize power from the battery, for collecting images, only when the device has reached the small intestine.

[0054] The PLL 402 is a feedback system intended to automatically correct drifts in the transmitted frequency. PLL 402 includes a pre-scaler 424 for fast frequency dividing that is not dependant on the channel frequency. The pre-scaler 424 is in communication with a divider 421 that divides the frequency of the oscillator 404 to perform the reference frequency for the PLL. The division value is channel dependant. The PLL 402 also includes a phase frequency detector (PFD) 422 for per-

forming the frequency comparison and the phase comparison of the PLL, and a charge pump 423 for performing the shape of the loop transmission of the whole loop.

[0055] LED power and control block 403 includes a high voltage source 432 that is controlled by the external capacitor 431. LED power and control block 403 also includes a high current source 433 and the peak current value of the LEDs is controlled by the resistor which is connected to LedRes 435.

[0056] The transmitter 400 is controlled by an external magnetic switch 405. The switch 405 is a normally opened (NO) switch that is kept closed by an external magnet, as described above. Switch 405 controls an internal electronic switch 406 that controls all the device electronics. Electronic switch 406 includes a low leakage circuitry to convert the logic of the NO switch 405 to "normally closed" (NC) logic, such that although switch 405 is a NO switch it will keep the transmitter inactive while it is closed.

[0057] The low leakage circuit only uses 1% - 3% of the battery power per year, so that the internal electronic switch 406 is not a significant factor in the power regimen of the device.

[0058] In an embodiment of the invention the device swallowable capsule having an optical window and comprising a CMOS imaging camera, white LEDs, an optical system, a transmitter and battery. The swallowable capsule is kept inactive while contained in a package having a magnet, such as the magnetic packaging described in PCT application IL00/00752. Just prior to use the package having the magnet is removed enabling the switch 405 to be opened, thereby activating the transmitter and with it, initiating imager and illumination operation.

[0059] The input bandwidth of the information in the transmitter 400 is over 1.35Megabit per second. Such a low powered high input bandwidth transmitter for transmitting video data, has not yet been shown in the art.

[0060] Reference is now made to Fig. 5 in which a block diagram of an image obtaining method is illustrated. The method for in vivo imaging includes the following steps: illuminating a site in vivo (502); collecting remitted light onto pixels of a CMOS imaging camera, thereby generating an analog signal (504); converting the analog signal to a digital signal (506); randomizing the digital signal (508); transmitting the digital signal to a receiving system (510) and processing the transmitted signals to obtain images of the in vivo site (512).

[0061] The step of illumination (502) is preferably carried out by employing white LEDs to illuminate the site in vivo. Illumination may be continuous or alternating in accordance with specific requirements of the system.

[0062] Collecting light remitted from the site in vivo (504) and directing it on to the pixels of a CMOS imaging chip is achieved by employing an optical system which comprises a lens and which may further comprise any suitable collimator.

[0063] Conversion of the analog signal to a digital signal (506) is preferably effected in a serial manner.

[0064] Randomizing the digital signal (508), namely randomizing the occurrence of the digital signals ("0" and "1"), is performed so that transmission is not impeded by a reoccurring signal of one type.

[0065] Transmission of the signal (510) is accomplished using radio frequencies (approximately 432 - 434 Mhz) at a rate of two to eight frames per second to an array of antennas attached to a patient's body. The antennas allow image capture and are also used to calculate and indicate the position of the imager in the patient's body. An example of the calculation and indication the position of the imager in the patient's body is provided in the above mentioned US 5,604,531.

[0066] Processing of signals (512) can be carried out by employing suitable processors and software. For example, the RAPID software (propriety software developed and owned by Given Imaging Ltd. of Yokneam, Israel) is used to obtain a video clip of images captured from within the GI tract. The video clip can be synchronized with the trajectory of the imaging device as it passes through the GI tract to enable localization of the device in the GI tract.

[0067] Additionally, a plurality of receiving antennas can be used which can be moved to the location enabling best receiving conditions.

[0068] The images can be stored on a small portable recorder carried on a belt and subsequently downloaded for analysis and retrieval. Additionally, the receiver can be connected directly to a stationary data recorder.

[0069] Experiments were carried out with an 11 x 30 mm capsule comprising a CMOS imaging chip and miniature processor, white LED light sources, a short focal length lens and a miniature transmitter and antenna. The capsule, powered by silver oxide batteries, was swallowed and more than 5 hours of continuous recording of images from the gastrointestinal tract were achieved.

[0070] Live transmission of good quality video images were obtained for up to 6 hour periods in ambulatory dogs.

[0071] With ethical committee approval a human volunteer study was performed. The capsule was easily swallowed. Moving images were obtained from the stomach and small intestine. No discomfort was experienced. The optical window remained clear throughout the whole transmission.

[0072] Trigonometric analysis of signal strength allowed continuous monitoring of the capsule position. Imaging of the small bowel was successfully completed in 2 hours.

[0073] It will be appreciated by persons skilled in the art that the present invention is not limited to what has been particularly shown and described hereinabove. Rather the scope of the present invention is defined only by the claims which follow:

Claims

1. A swallowable capsule for in vivo imaging of the gastrointestinal tract said capsule having an optical window and comprising a CMOS imaging camera, at least one illumination source for illuminating a gastrointestinal tract site, an optical system for focussing images of the gastrointestinal tract site onto the CMOS imaging camera, and
a transmitter for transmitting video output of the CMOS imaging camera and **characterised in** the transmitter being arranged for transmitting on radio frequency and at a rate of two image frames per second.
2. The swallowable capsule of claim 1, **characterized in that** the transmitter is arranged to operate at frequencies of 432 to 434 MHz.
3. The swallowable capsule of claim 1 or 2, **characterized in that** the transmitter has an input bandwidth of more than 1.35 Megabit per second.

25 Patentansprüche

1. Verschluckbare Kapsel zur In-vivo-Bildgebung des Magen-Darm-Traktes, wobei die Kapsel ein optisches Fenster aufweist und eine CMOS-Bildgebungskamera, mindestens eine Beleuchtungsquelle zum Beleuchten einer Stelle im Magen-Darm-Trakt, ein optisches System zum Fokussieren von Bildern der Stelle des Magen-Darm-Traktes auf die CMOS-Bildgebungskamera, und
einen Transmitter zum Übertragen des Videoausgangs der CMOS-Bildgebungskamera umfasst, und **dadurch gekennzeichnet, dass** der Transmitter zum Übertragen auf Funkfrequenz und mit einer Geschwindigkeit von zwei Bildrahmen pro Sekunde geeignet ist.
2. Verschluckbare Kapsel nach Anspruch 1, **dadurch gekennzeichnet, dass** der Transmitter zum Betrieb bei Frequenzen von 432 bis 434 MHz geeignet ist.
3. Verschluckbare Kapsel nach Anspruch 1 oder 2, **dadurch gekennzeichnet, dass** der Transmitter eine Eingangsbandbreite von mehr als 1,35 Megabit pro Sekunde aufweist.

Revendications

1. Capsule endoscopique destinée à l'imagerie in vivo du tractus gastro-intestinal, ladite capsule ayant une fenêtre optique et comprenant une caméra d'imagerie CMOS, au moins une source d'éclairage destinée à éclairer un site du tractus gastro-intestinal, un sys-

tème optique destiné à mettre au point des images du site de tractus gastro-intestinal sur la caméra d'imagerie CMOS, et un émetteur destiné à émettre une prise de sortie vidéo de la caméra d'imagerie CMOS et **caractérisé en ce que** l'émetteur étant agencé pour l'émission sur une radiofréquence et à un taux de deux trames d'image par seconde.

5

2. Capsule endoscopique de la revendication 1, **caractérisée en ce que** l'émetteur est agencé pour fonctionner à des fréquences allant de 432 à 434 MHz. 10
3. Capsule endoscopique de la revendication 1 ou 2, **caractérisée en ce que** l'émetteur présente une largeur de bande à l'entrée supérieure à 1,35 Mégabits par seconde. 15

20

25

30

35

40

45

50

55

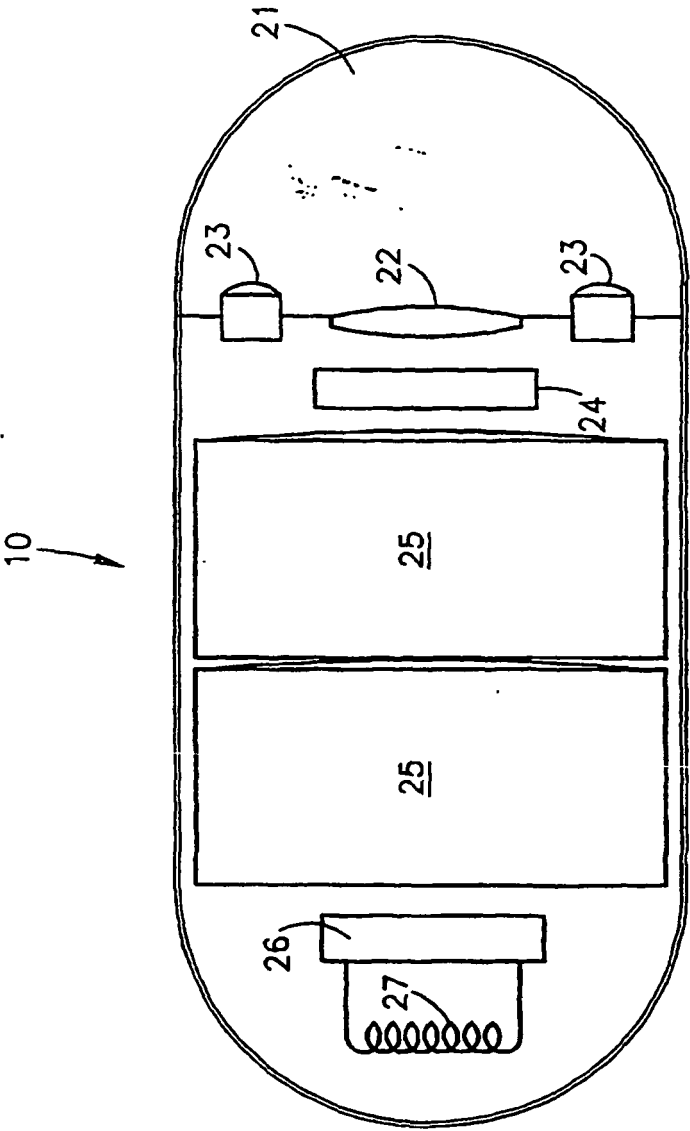


FIG.1

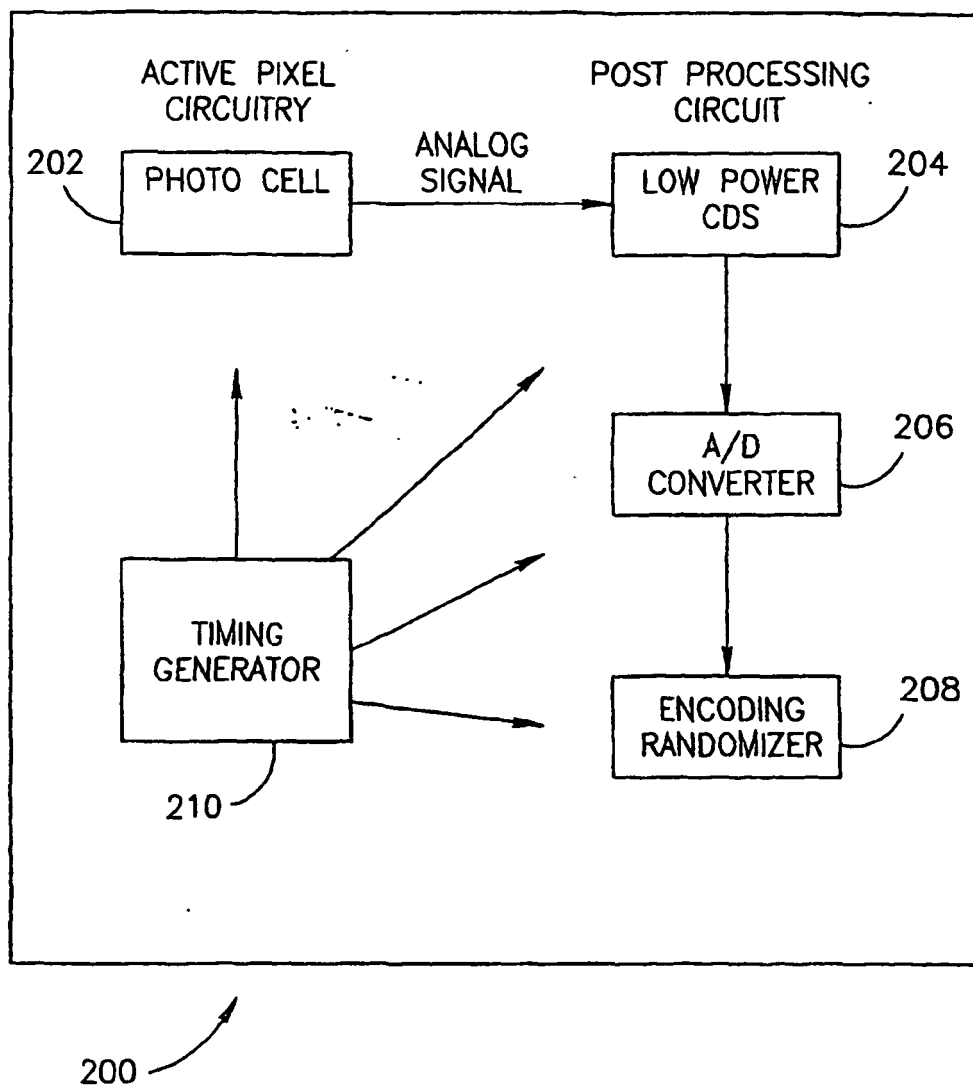


FIG.2

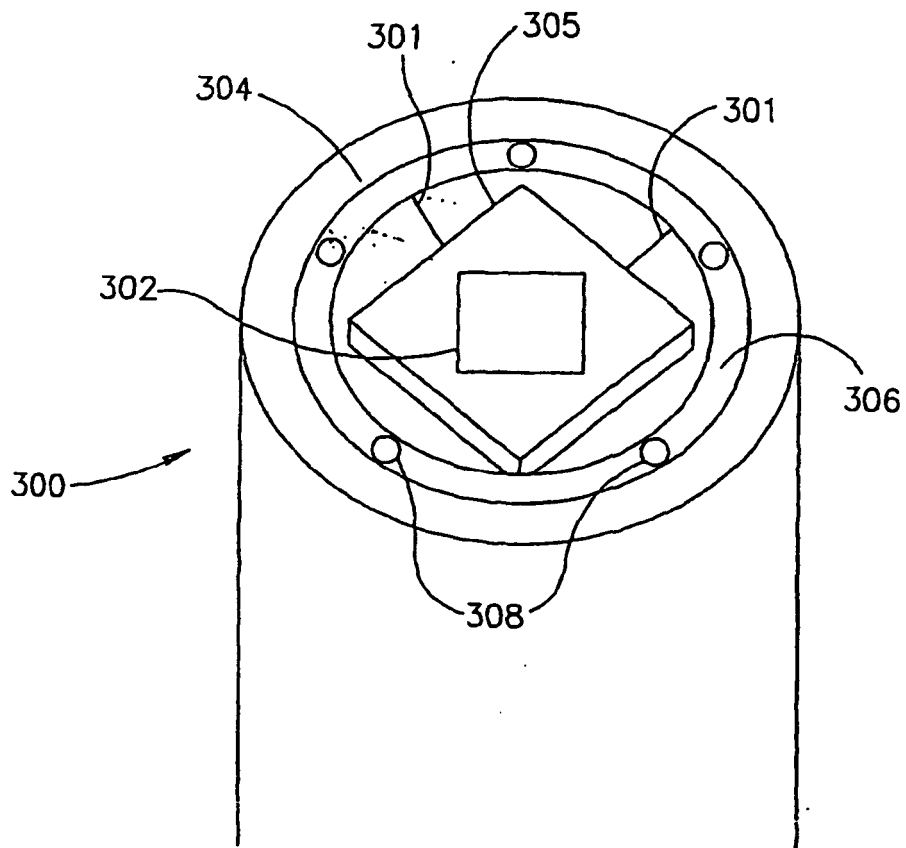


FIG.3

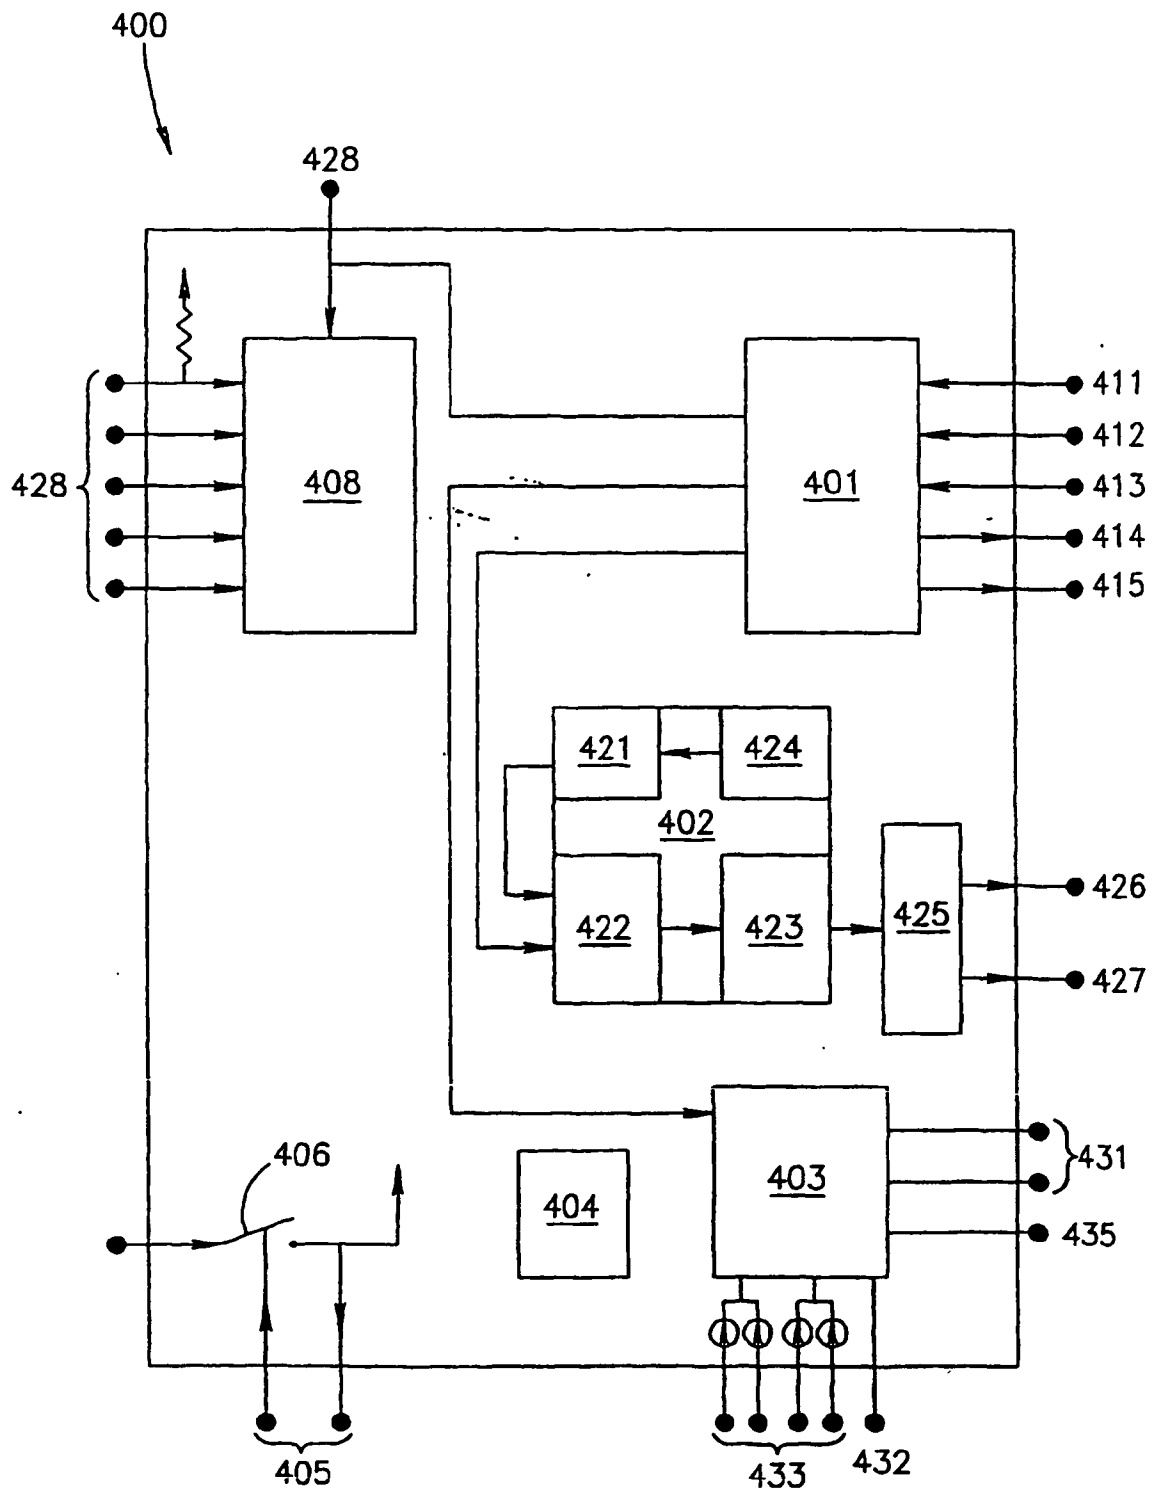


FIG.4

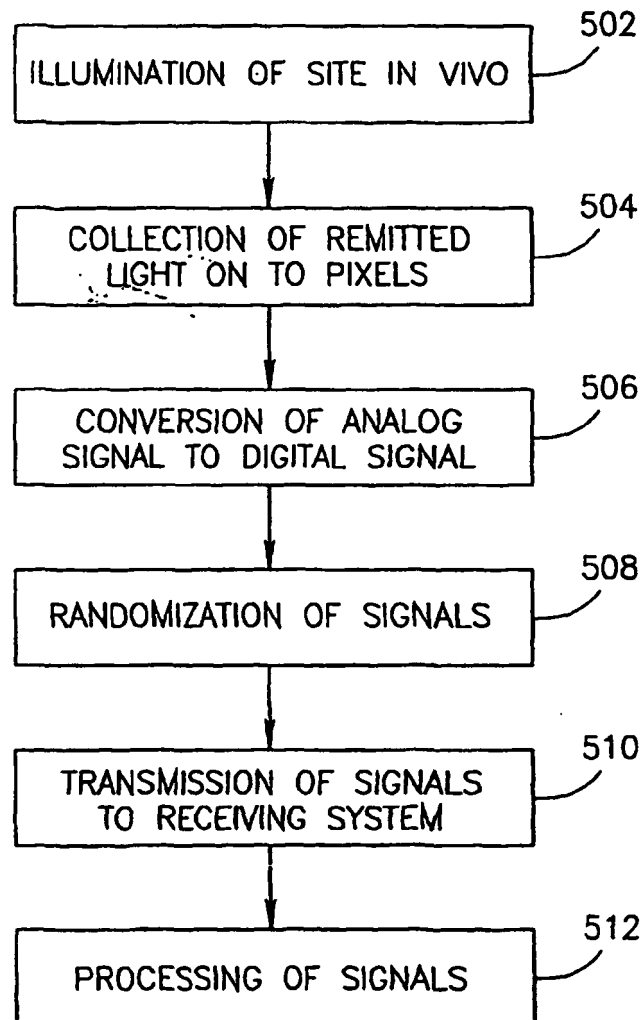


FIG.5

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5604531 A [0003] [0043] [0065]
- US 5749367 A [0006]
- US 5833603 A [0007]
- WO 0076391 A [0038]
- IL 0000752 W [0058]

Non-patent literature cited in the description

- **BABAK ZIAIE et al.** A low-power miniature transmitter using a low-loss silicon platform for biotelemetry. *Proceedings/19th International Conference-IEEE/EMBS*, 30 October 1997 [0004]
- **A. HEUBERGER.** *Integrated RF transmitter based on SAW oscillator* [0005]

专利名称(译)	一种用于体内成像的装置		
公开(公告)号	EP1693000B1	公开(公告)日	2013-05-08
申请号	EP2006010954	申请日	2001-03-08
[标]申请(专利权)人(译)	基文影像公司		
申请(专利权)人(译)	基文影像有限公司.		
当前申请(专利权)人(译)	基文影像有限公司.		
[标]发明人	IDDAN GAVRIEL AVNI DOV GLUKHOVSKY ARKADY MERON GAVRIEL		
发明人	IDDAN, GAVRIEL AVNI, DOV GLUKHOVSKY, ARKADY MERON, GAVRIEL		
IPC分类号	A61B5/00 A61B1/05 H04L25/03 G03B15/00 A61B1/00 A61B1/04 A61B1/273 A61B1/31 A61B5/07 G03B15/02 H04N5/225 H04N7/18		
CPC分类号	H04N5/2256 A61B1/00016 A61B1/00032 A61B1/00036 A61B1/0016 A61B1/041 A61B1/0607 A61B1/ /0676 A61B1/0684 A61B1/2733 A61B1/2736 A61B1/31 A61B5/0031 A61B5/073 A61B5/14539 A61B2560/0209 H04L25/03866 H04N5/2251 H04N5/2252 H04N5/23203 H04N7/185 H04N2005/2255		
优先权	60/187883 2000-03-08 US		
其他公开文献	EP1693000A2 EP1693000A3		
外部链接	Espacenet		

摘要(译)

一种用于可吞咽体内成像胶囊的发射器 (26; 305; 400) , 适用于将图像信号从所述胶囊传输到连接到患者身体的天线阵列, 所述发射器 (26; 305; 400) 包括天线 (27) ; 426,427) 并且被安排为以每秒2到8帧的速率发送。

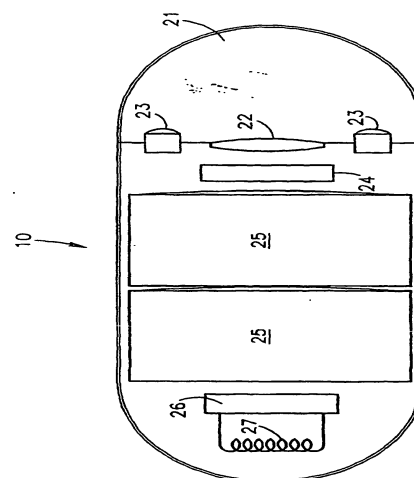


FIG.1