



(11)

EP 2 839 785 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
30.11.2016 Bulletin 2016/48

(51) Int Cl.:
A61B 5/00 (2006.01) A61B 10/00 (2006.01)
G01N 21/47 (2006.01)

(21) Application number: **13775158.2**

(86) International application number:
PCT/JP2013/060282

(22) Date of filing: **04.04.2013**

(87) International publication number:
WO 2013/154012 (17.10.2013 Gazette 2013/42)

(54) OBJECT OBSERVATION DEVICE AND OBJECT OBSERVATION METHOD

OBJEKTBEOBSACHTUNGSVORRICHTUNG UND OBJEKTBEOBSACHTUNGSVERFAHREN
DISPOSITIF D'OBSERVATION D'OBJET ET PROCÉDÉ D'OBSERVATION D'OBJET

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR

(74) Representative: **Müller Hoffmann & Partner**
Patentanwälte mbB
St.-Martin-Strasse 58
81541 München (DE)

(30) Priority: **10.04.2012 JP 2012088924**

(56) References cited:
EP-A2- 2 067 432 JP-A- 2005 328 916
JP-A- 2008 178 546 US-A1- 2009 244 546

(43) Date of publication of application:
25.02.2015 Bulletin 2015/09

(73) Proprietor: **Advanced Telecommunications**
Research Institute
International
Soraku-gun
Kyoto 619-0288 (JP)

- **CHRISTINA HABERMEHL ET AL:**
"Somatosensory activation of two fingers can be discriminated with ultrahigh-density diffuse optical tomography", **NEUROIMAGE, ACADEMIC PRESS, ORLANDO, FL, US, vol. 59, no. 4, 21 November 2011 (2011-11-21), pages 3201-3211, XP028456578, ISSN: 1053-8119, DOI: 10.1016/J.NEUROIMAGE.2011.11.062 [retrieved on 2011-12-01]**
- **NIU H ET AL:** "Development of a compensation algorithm for accurate depth localization in diffuse optical tomography", **OPTICS LETTERS, OPTICAL SOCIETY OF AMERICA, US, vol. 35, no. 3, 1 February 2010 (2010-02-01), pages 429-431, XP001551658, ISSN: 0146-9592, DOI: 10.1364/OL.35.000429**
- **ATSUSHIMIYAMOTO ET AL.:** 'Hierarchical Bayes method for NIRS-DOT inverse problem and its phase diagrams' **IEICE TECHNICAL REPORT. NC, NEUROCOMPUTING vol. 110, no. 149, 20 July 2010, pages 51 - 56, XP008175162**

(72) Inventors:

- **SHIMOKAWA, Takeaki**
Soraku-gun
Kyoto 619-0288 (JP)
- **KOSAKA, Takashi**
Soraku-gun
Kyoto 619-0288 (JP)
- **YAMASHITA, Okito**
Soraku-gun
Kyoto 619-0288 (JP)
- **SATO, Masaaki**
Soraku-gun
Kyoto 619-0288 (JP)

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 2 839 785 B1

Description

Technical Field

5 **[0001]** The present application relates to an object observing apparatus and the like for outputting three-dimensional information indicating a local optical characteristic-changed region inside an object.

Background Art

10 **[0002]** Since measurement using near-infrared light is simple and safe, it is used for non-invasive measurement of the brain functions (see Non-Patent Document 1) and detection of breast cancer (see Non-Patent Document 2). Diffuse optical tomography (DOT) is an attempt to reconstruct an optical characteristic change or the structure inside a living body from observation data, by calculating a diffusion process of near-infrared light, which is extensively scattered inside a living body. Examples of such near-infrared measurement include continuous-light measurement, time-resolved measurement, and frequency-resolved measurement. Continuous-light measurement is characterized in that the amount of information that can be obtained is small, but the cost is low, the measurement is robust to noise because a large amount of light is irradiated, and the sampling frequency is high. On the other hand, time-resolved measurement and frequency-resolved measurement are characterized in that the amount of information that can be obtained is large, but the measurement is significantly affected by noise, and the cost is high.

20 **[0003]** In many cases, near-infrared light does not penetrate a living body because it is extensively scattered inside the living body. Thus, for example, in measurement of the brain functions, reflection-type measurement is performed in which light-transmitting probes are arranged on the head surface, and light reflected by diffusion is observed using light-receiving probes also arranged on the head surface. In the measurement of the brain functions, simultaneous measurement using a large number of probes is necessary in order to cover the activity region, and, thus, continuous-light measurement is usually used.

25 **[0004]** Conventionally, probes are arranged at intervals of approximately 3 cm, which is considered to be suitable for measurement of the brain functions, and the observation result is obtained as topographic data (see Non-Patent Document 3). Meanwhile, in recent measurement of the brain functions, there have been many attempts to increase the number of probes per unit area, thereby performing DOT at high density. Accordingly, it becomes possible to discriminate multiple cortical activity regions in the visual area and the somatosensory area (see Non-Patent

30 **[0005]** Documents 4 and 5). In Non-Patent Document 6, a depth compensation algorithm (DCA) is applied, in which a sensitivity matrix is directly modified to compensate for a change in a sensitivity due to an increased depth. Non-Patent Document 7 and Patent Documents 1 and 2 describe near-infrared spectroscopy (NIRS). In particular, Non-Patent Document 7 describes a solving inverse problem of NIRS—diffusion optical tomography (NIRS—DOT) using a hierarchical Bayesian method. In Patent Document 3 a compensation table generation method is described, the compensation table being used when generating an optical tomography image by OCT (Optical Coherence Tomography). The compensation table is obtained by measuring an interference signal of a reference light and a reflection light. In Patent Document 4 describes an image processing system that is configured to correct an image of an object inside a physical body.

40

Citation List

Non-Patent Document

45 **[0006]**

[Non-Patent Document 1] Y. Hoshi and M. Tamura, "Detection of dynamic changes in cerebral oxygenation coupled to neuronal function during mental work in man," *Neurosci. Lett.* 150 (1993) 5-8.

50 [Non-Patent Document 2] Daisuke Yamashita, Motoki Oda, Hiroaki Suzuki, Takeshi Yamanaka, Toshihiko Suzuki, Yukio Ueda, Kazuyoshi Ohta, Mitsuharu Miwa, Yutaka Hasegawa, Hiroyuki Kyushima, and Yutaka Yamashita, "Development of Multi Channel Time Resolved Spectroscopy System and Application to Optical Mammography System," *J Jpn Coll Angiol.* 47 (2007) 11-16.

[Non-Patent Document 3] A. Maki, Y. Yamashita, Y. Ito, E. Watanabe, Y. Mayanagi, and H. Koizumi, "Spatial and temporal analysis of human motor activity using noninvasive NIR topography," *Med. Phys.* 22 (1995) 1997-2005.

55 [Non-Patent Document 4] B. W. Zeff, B. R. White, H. Dehghani, B. L. Schlaggar, and J. P. Culver, "Retinotopic mapping of adult human visual cortex with high-density diffuse optical tomography," *Proc. Natl. Acad. Sci. U.S.A.* 104 (2007) 12169-12174.

[Non-Patent Document 5] C. Habermehl, S. Holtze, J. Steinbrink, S. P. Koch, H. Obrig, J. Mehnert, and C. H. Schmitz,

"Somatosensory activation of two fingers can be discriminated with ultrahigh-density diffuse optical tomography," NeuroImage 59 (2011) 3201-3211.

[Non-Patent Document 6] H. Niu, F. Tian, Z.-J. Lin and H. Liu, "Development of a compensation algorithm for accurate depth localization in diffuse optical tomography", Optics Letter, Vol. 35, No. 3, 429-431.

[Non-Patent Document 7] MIYAMOTO, Atsushi et al., "Hierarchical Bayes method for NIRS—DOT inverse problem and its phase diagrams", IEICE Technical Report. NC, Neurocomputing, 20 July 2010, 110(149), 51-56.

Patent Documents

[0007]

[Patent Document 1] JP 2008-178546 A

[Patent Document 2] JP 2005-328916 A

[Patent Document 3] US 2009/0244546 A1

[Patent Document 4] EP 2 067 432 A2

Summary of Invention

Technical Problem

[0008] However, the above-described reflection-type continuous-light measurement provides the smallest amount of information among DOT, and, thus, ill-posed problems frequently occurs in estimating an activity source, and the estimation is difficult. The reflection-type continuous-light DOT has two main problems, which will be described below.

[0009] Firstly, in the reflection-type continuous-light DOT, which is of the reflection-type, since probes can be arranged only on the surface, and the sensitivity is exponentially attenuated in accordance with the depth as light is diffused, it is difficult to specify the depth of an activity source.

[0010] Secondly, in the reflection-type continuous-light DOT, since light is diffused in an object, spatial blurring occurs, which makes it difficult to improve the space resolution.

[0011] That is to say, conventional object observing systems cannot accurately estimate, as three-dimensional information, a local optical characteristic-changed region inside an object such as the brain.

Solution to Problem

[0012] The above objects are solved by the claimed matter according to the independent claims.

[0013] For the first problem, an object observing apparatus of the present application performs correction according to sensitivity attenuation in accordance with the depth. Furthermore, for the second problem, sparse estimation is performed as a method for improving the space resolution. The object observing apparatus of the present application combines these two countermeasures, thereby realizing accurate three-dimensional DOT including the depth direction.

[0014] More specifically, a first aspect of the present application is directed to an object observing apparatus, including: a reference light intensity information storage unit in which reference light intensity information, which is information regarding a light intensity at each light-receiving probe, and is information used as a reference, is stored; a light intensity information acquiring unit that, using a near-infrared measurement apparatus having at least one probe set consisting of a pair of a light-transmitting probe for transmitting light to an object that is to be observed and a light-receiving probe for receiving light, acquires light intensity information, which is information regarding a light intensity of light received by each light-receiving probe, in a case where light with a certain light intensity is transmitted from each light-transmitting probe forming each probe set to the object; a light intensity change information acquiring unit that acquires, for each probe set, light intensity change information, which is information regarding a light intensity change, from the reference light intensity information in the reference light intensity information storage unit and the light intensity information acquired by the light intensity information acquiring unit; an estimating unit that acquires optical characteristic-changed region information, which is three-dimensional information regarding a position with a light absorbance change inside the object, using the light intensity change information for each probe set; and an output unit that outputs the optical characteristic-changed region information acquired by the estimating unit; wherein the estimating unit includes: a sensitivity information storage part in which sensitivity information, which is information indicating a relationship between an optical characteristic change and a light intensity change, can be stored; a correcting part that performs correction according to sensitivity attenuation in accordance with a depth, using the sensitivity information; and a sparseness applying part that introduces sparseness for improving a space resolution, thereby acquiring the optical characteristic-changed region information. Note that the estimating unit may simultaneously perform the correction according to the sensitivity attenuation and the application of the sparseness for improving the space resolution.

[0015] With this configuration, it is possible to accurately estimate, as three-dimensional information, a local optical characteristic-changed region inside an object.

[0016] Furthermore, a second aspect of the present application is directed to the object observing apparatus according to the first aspect, wherein the estimating unit further includes an arithmetic expression storage part, in which a first arithmetic expression, which is an arithmetic expression used for acquiring the optical characteristic-changed region information, is an arithmetic expression for calculating a solution of an inverse problem, and is a cost function for performing correction according to the sensitivity information, can be stored, the correcting part substitutes the sensitivity information for the first arithmetic expression, thereby acquiring first optical characteristic-changed region information, the sparseness applying part acquires final optical characteristic-changed region information using the sparseness for improving the space resolution, using the first optical characteristic-changed region information, and the output unit outputs the optical characteristic-changed region information acquired by the sparseness applying part.

[0017] With this configuration, it is possible to accurately estimate, as three-dimensional information, a local optical characteristic-changed region inside an object.

[0018] Furthermore, a third aspect of the present application is directed to the object observing apparatus according to the second aspect, wherein, in the arithmetic expression storage part, a second arithmetic expression for performing hierarchical Bayesian estimation on an initial value is also stored, and the sparseness applying part substitutes the first optical characteristic-changed region information as an initial value for the second arithmetic expression, and executes the second arithmetic expression to perform hierarchical Bayesian estimation, thereby acquiring final optical characteristic-changed region information.

[0019] With this configuration, it is possible to accurately estimate, as three-dimensional information, a local optical characteristic-changed region inside an object.

[0020] Furthermore, a fourth aspect of the present application is directed to the object observing apparatus according to any one of the first to third aspects, for use in observation of a brain function of a living body, wherein the object that is to be observed is the brain of the living body, and the reference light intensity information is information regarding a light intensity at each light-receiving probe measured at rest.

[0021] With this configuration, it is possible to accurately and easily estimate the brain activity.

[0022] Furthermore, a fifth aspect of the present application is directed to the object observing apparatus according to any one of the first to third aspects, for use in screening of breast cancer, wherein the object that is to be observed is a breast, and the reference light intensity information is information regarding a light intensity at each light-receiving probe from a breast with normal cells.

[0023] With this configuration, it is possible to accurately and easily detect breast cancer.

[0024] Furthermore, a sixth aspect of the present application is directed to the object observing apparatus according to any one of the first to fifth aspects, wherein each interval between the light-transmitting and light-receiving probes is not greater than 20 mm.

[0025] With this configuration, it is possible to more accurately estimate, as three-dimensional information, a local optical characteristic-changed region inside an object.

Advantageous Effects of Invention

[0026] The object observing system according to the present application can accurately estimate, as three-dimensional information, a local optical characteristic-changed region inside an object.

Brief Description of Drawings

[0027]

FIG. 1 is a block diagram of an object observing system in Embodiment 1.

FIG. 2 is a flowchart illustrating an operation of an object observing apparatus in this embodiment.

FIG. 3 is a flowchart illustrating an operation of estimation processing in this embodiment.

FIG. 4 is a schematic diagram of an experiment using the object observing system in this embodiment.

FIG. 5 is a diagram illustrating positions of light-transmitting probes and light-receiving probes in a phantom experiment in this embodiment.

FIG. 6 is a diagram illustrating an environment of Experiment 1 in this embodiment.

FIG. 7 is a diagram showing an estimation result using a Tikhonov regularization method in a case where a regularization term is not normalized with the sensitivity in this embodiment.

FIG. 8 is a diagram showing an estimation result in a case where the regularization term is normalized with the sensitivity in this embodiment.

FIG. 9 is a diagram showing an estimation result in a case where application is made to a hierarchical Bayesian

method in this embodiment.

FIG. 10 shows diagrams of a result of estimation performed while changing the probe interval and the depth position of a light absorbing member in this embodiment.

FIG. 11 is a diagram illustrating expressing a three-dimensional estimation diagram in two dimensions in this embodiment.

FIG. 12 shows graphs of a result of Experiment 2 in this embodiment.

FIG. 13 shows a table of a result of Experiment 2 in this embodiment.

FIG. 14 shows diagrams of a result of Experiment 3 in this embodiment.

FIG. 15 shows a table of a result of Experiment 3 in this embodiment.

FIG. 16 shows diagrams of a result of Experiment 4 in this embodiment.

FIG. 17 shows a table of a result of Experiment 4 in this embodiment.

FIG. 18 is a schematic view of a computer system in this embodiment.

FIG. 19 is a block diagram of the computer system in this embodiment.

Description of Embodiment

[0028] Hereinafter, an embodiment of an object observing system and the like will be described with reference to the drawings. Note that constituent elements denoted by the same reference numerals perform the same operations in the embodiments, and, thus, a description thereof may not be repeated.

Embodiment 1

[0029] In this embodiment, an object observing system will be described that transmits near-infrared light to an object, receives light scattered inside the object, and outputs three-dimensional information indicating a local optical characteristic-changed region inside the object. In this case, the light typically received and used by an object observing apparatus forming the object observing system is not light that has penetrated an object, but backscattered light from the inside of an object.

[0030] FIG. 1 is a block diagram of an object observing system in this embodiment. The object observing system includes a near-infrared measurement apparatus 1 and an object observing apparatus 2.

[0031] The near-infrared measurement apparatus 1 includes light-transmitting probes 11, light-receiving probes 12, an accepting unit 13, and a control unit 14. The near-infrared measurement apparatus 1 has at least one probe set (also referred to as a channel) consisting of a pair of a light-transmitting probe 11 and a light-receiving probe 12. Note that the near-infrared measurement apparatus 1 typically has multiple probe sets.

[0032] The object observing apparatus 2 includes a reference light intensity information storage unit 21, a light intensity information acquiring unit 22, a light intensity change information acquiring unit 23, an estimating unit 24, and an output unit 25. Furthermore, the estimating unit 24 includes a sensitivity information storage part 241, an arithmetic expression storage part 242, a correcting part 243, and a sparseness applying part 244.

[0033] The light-transmitting probes 11 forming the near-infrared measurement apparatus 1 irradiate near-infrared light on an object (e.g., a head, a breast, or the like of a living body, in this example).

[0034] The light-receiving probes 12 typically receive light that has been absorbed or scattered inside an object and exits from the object. The probe arrangement density is more preferably 20 mm or less, extremely preferably 1.5 cm or less. The probe arrangement density refers to intervals between a light-transmitting probe 11 and a light-receiving probe 12. The higher the density at which the probes are arranged is, the better the configuration becomes. The reason for this is that, for example, the number of channels for detecting a state inside an object increases.

[0035] The light-transmitting probes 11 transmit light from one direction to an object that is to be observed. Furthermore, the light-receiving probes 12 typically receive light from the same direction as the one direction. Note that the same direction in this example is not limited to directions that exactly match each other, and there may be an angular difference therebetween (e.g., a large difference such as 30 degrees or 45 degrees). The same direction typically refers to a state in which a side from which the light-transmitting probes 11 transmit light and a side on which the light-receiving probes 12 receive light are on the same side of an object.

[0036] The accepting unit 13 accepts an instruction from the outside. This instruction is, for example, an irradiation instruction to irradiate near-infrared light on a living body.

[0037] If the accepting unit 13 accepts an irradiation instruction, the control unit 14 instructs the light-transmitting probes 11 to irradiate near-infrared light. Typically, if the light-transmitting probes 11 accept an irradiation instruction from the control unit 14, the light-transmitting probes 11 irradiate near-infrared light on an object.

[0038] In the reference light intensity information storage unit 21 forming the object observing apparatus 2, reference light intensity information is stored. The reference light intensity information is information regarding a light intensity at each light-receiving probe, and is information used as a reference. For example, in the case where the object observing

apparatus 2 observes a brain activity, the reference light intensity information is information regarding a light intensity at each light-receiving probe 12 measured at rest. In the case of detecting breast cancer, the reference light intensity information is information regarding a light intensity at each light-receiving probe 12 from normal cells. There is no limitation on the procedure in which the reference light intensity information is stored in the reference light intensity information storage unit 21. The reference light intensity information and light intensity information, which will be described later, may be acquired in the same period.

[0039] The light intensity information acquiring unit 22 acquires light intensity information, using the near-infrared measurement apparatus 1 having at least one probe set consisting of a pair of a light-transmitting probe 11 for transmitting light to an object that is to be observed and a light-receiving probe 12 for receiving light. The light intensity information is information regarding a light intensity of light received by each light-receiving probe, in a case where light with a certain light intensity is transmitted from each light-transmitting probe 11 forming each probe set to the object. Note that the object that is to be observed is, for example, a brain, a breast, or the like of a living body.

[0040] The light intensity change information acquiring unit 23 acquires, for each probe set, light intensity change information, which is information regarding a light intensity change, from the reference light intensity information in the reference light intensity information storage unit 21 and the light intensity information acquired by the light intensity information acquiring unit 22.

[0041] The estimating unit 24 acquires optical characteristic-changed region information, using the light intensity change information for each probe set. The light intensity change information is the information acquired by the light intensity change information acquiring unit 23. Furthermore, the optical characteristic-changed region information is three-dimensional information regarding a position with a light absorbance change inside an object. Furthermore, the optical characteristic-changed region information also may be referred to as information regarding the amount of light absorbance change inside an object.

[0042] In the sensitivity information storage part 241 forming the estimating unit 24, sensitivity information can be stored. The sensitivity information is information indicating a relationship between an optical characteristic change (e.g., corresponding to X (described later)) and a light intensity change (e.g., corresponding to Y (described later)). The sensitivity information is, for example, a sensitivity matrix, which will be described later.

[0043] In the arithmetic expression storage part 242, arithmetic expressions used by the object observing apparatus 2 can be stored. In the arithmetic expression storage part 242, for example, a first arithmetic expression or a second arithmetic expression can be stored. The first arithmetic expression is, for example, an arithmetic expression used for acquiring the optical characteristic-changed region information, is an arithmetic expression for calculating a solution of an inverse problem, and is a cost function for performing correction according to the sensitivity information. Furthermore, the second arithmetic expression is, for example, an arithmetic expression for performing hierarchical Bayesian estimation on an initial value. The second arithmetic expression may be, for example, an L1 norm arithmetic expression.

[0044] The correcting part 243 performs correction according to sensitivity attenuation in accordance with the depth, using the sensitivity information in the sensitivity information storage part 241. More specifically, the correcting part 243 substitutes the sensitivity information for the first arithmetic expression, thereby acquiring first optical characteristic-changed region information. There is no limitation on the arithmetic expression for performing correction according to sensitivity attenuation in accordance with the depth.

[0045] The sparseness applying part 244 introduces sparseness for improving the space resolution, thereby acquiring optical characteristic-changed region information. Specifically, the sparseness applying part 244 acquires final optical characteristic-changed region information using the sparseness for improving the space resolution, using the first optical characteristic-changed region information as input. More specifically, the sparseness applying part 244 substitutes the first optical characteristic-changed region information as an initial value for the second arithmetic expression, and executes the second arithmetic expression to perform hierarchical Bayesian estimation, thereby acquiring final optical characteristic-changed region information. Note that the sparseness is preferably introduced through hierarchical Bayesian estimation, but an L1 norm also may be used. There is no limitation on the algorithm for introducing the sparseness. Furthermore, in the algorithm, the correcting part 243 and the sparseness applying part 244 may simultaneously operate.

[0046] More specifically, the estimating unit 24 operates as follows. That is to say, the estimating unit 24 reconstructs a three-dimensional light absorbance change map, from light intensity change information, which is a value indicating a change between the two amounts of light consisting of reference light intensity information, which is information regarding the amount of light measured on the base line, and information (light intensity information) regarding the amount of light measured when there is a light absorbance change.

[0047] In order to perform the reconstruction, the estimating unit 24 executes two steps consisting of a direct problem solving step and an inverse problem solving step. Firstly, in the direct problem solving step, the estimating unit 24 acquires a relationship between a light absorbance change and an observed light intensity change. Next, in the inverse problem solving step, the estimating unit 24 estimates the light absorbance change, from the relationship obtained in the direct problem solving step and the observed light intensity change. Note that a problem, in a case of estimating and acquiring values (e.g., X), using observed values (e.g., Y) in a number smaller than the number of values (e.g., X) that

are to be estimated, is referred to as an ill-posed problem among inverse problems, and some sort of efforts such as regularization are necessary for solving the problem.

[0048] The object observing apparatus 2 uses the Rytov approximation in the direct problem solving step. The Rytov approximation is a known art, and, thus, a detailed description thereof has been omitted. According to the Rytov approximation, assuming that the amount of light $\Phi_0(r_s, r_d)$ transmitted from a source (the light-transmitting probe 11) at a position r_s and reaching a detector (the light-receiving probe 12) at a position r_d , on the base line, becomes $\Phi(r_s, r_d)$ due to a light absorbance change inside an object by $\delta\mu_a$, the amount of light change generated $\Phi_{\text{pert}}(r_s, r_d) = \ln(\Phi_0(r_s, r_d)/\Phi(r_s, r_d))$ is represented by Equation 1 below. That is to say, Equation 1 represents the Rytov approximation.

$$\Phi_{\text{pert}}(r_s, r_d) = \int dr \frac{\Phi_0(r_s, r) \Phi_0(r, r_d)}{\Phi_0(r_s, r_d)} \delta\mu_a(r). \quad (1)$$

[0049] In this embodiment, the object observing apparatus 2 discretizes a region into voxels of "2.5 mm x 2.5 mm x 2.5 mm". Assuming that a voxel index is i , a channel index is j , and " $Y_j = \Phi_{\text{pert}}(r_{s(j)}, r_{d(j)})$ ", $X_i = \delta\mu_a(r_i)$, $A_{j,i} = \Phi(r_{s(j)}, r_i) \Phi_0(r_i, r_{d(j)}) / \Phi_0(r_{s(j)}, r_{d(j)})$ ", the Rytov approximation expression in Equation 1 is represented by a linear equation " $Y = AX$ ". Note that " $Y = (Y_1, \dots, Y_M)^T$ " is an observed light intensity change in all channels, " $X = (X_1, \dots, X_N)^T$ " is a light absorbance change in all voxels, and A is a sensitivity matrix (exemplary sensitivity information) having $A_{j,i}$ as an element. The sensitivity matrix is stored in the sensitivity information storage part 241. Furthermore, the Rytov approximation expression or " $Y = AX$ " may be stored in the arithmetic expression storage part 242. Hereinafter, it is assumed that the number of voxels is N and the number of channels is M as appropriate.

[0050] The value of Φ_0 can be obtained using photon Monte Carlo simulation (see "Q. Fang and D. A. Boas, "Monte Carlo simulation of photon migration in 3D turbid media accelerated by graphics processing units," Opt. Express 17 (2009) 20178-20190."). Furthermore, depending on the shape of a medium, an approximate value of Φ_0 can be preferably obtained using analytic solution with diffusion approximation (see "R. C. Haskell, L. O. Svaasand, T. T. Tsay, T. C. Feng, M. S. McAdams, and B. J. Tromberg, "Boundary conditions for the diffusion equation in radiative transfer," J. Opt. Soc. Am. A 11 (1994) 2727-2741.).

[0051] Next, the estimating unit 24 solves the inverse problem as follows. That is to say, the correcting part 243 forming the estimating unit 24 obtains an estimated solution using a Tikhonov regularization method in a case where a regularization term is normalized with a sensitivity term. Next, the sparseness applying part 244 performs hierarchical Bayesian estimation in which the value obtained by the correcting part 243 is used as an initial value.

[0052] Firstly, an operation of the correcting part 243 will be described in detail. In the arithmetic expression storage part 242, a cost function shown in Equation 2 below is stored. The correcting part 243 obtains a solution " $X^{\wedge}_R = \arg\min_x C_R(X; \lambda)$ ", which minimizes the cost function. Note that " $\wedge$ " of " $X^{\wedge}$ " is positioned directly above X .

$$C_R(X; \lambda) = || \Sigma_y^{-\frac{1}{2}} (Y - AX) ||^2 + \lambda || D^{\frac{1}{2}} X ||^2. \quad (2)$$

[0053] In Equation 2, the first term is an observation error term, and the second term is an L2 regularization term for preventing overfitting. The overfitting refers to excessive optimization of parameters to observation data. Furthermore, in Equation 2, λ is a parameter for determining a regularization level. An optimum λ value is determined by ABIC minimization, which is one of the information criteria, and is stored in the arithmetic expression storage part 242 (see "H. Akaike, "Likelihood and the Bayes procedure," In Bayesian Statistics (eds J. M. Bernardo et al., Univ. Press, Valencia) 143-166 (1980)."). Furthermore, Σ_y is an observation noise covariance matrix of an observed value Y .

[0054] In Equation 2, D is a normalization term according to the sensitivity. The value of a sensitivity matrix A is exponentially attenuated in accordance with the depth. Thus, spatially uniform regularization may cause a bias in the estimation result. In order to prevent this problem, the normalization term causes the level of the regularization term at each location to match the level of the sensitivity. Note that D in Equation 2 is represented by Equation 3 below.

$$D = \text{diag}(A^T \Sigma_y^{-1} A + \beta I). \quad (3)$$

[0055] In Equation 3, diag represents a matrix constituted by diagonal components, and T in the upper right corner represents transposition of a matrix. Furthermore, I is an identity matrix, and β is a sensitivity threshold for performing normalization. In this embodiment, it is assumed that the value of β in all of the following analyses is, for example, a maximum value of the sensitivity at a voxel located at a depth of 22.5 mm or more from a probe surface, that is, " $\beta = \max_{z \geq 22.5 \text{ mm}} [\text{diag}(A^T \Sigma_y^{-1} A)]$ ". Furthermore, if the regularization term is in the form of an L2 norm, an estimated solution $X_R^\wedge$ (where $\wedge$ is positioned directly above X) can be analytically obtained as shown in Equation 4. That is to say, Equation 4 is stored in the arithmetic expression storage part 242. The correcting part 243 obtains an estimated solution $X_R^\wedge$ using Equation 4.

$$\hat{X}_R = (A^T \Sigma_y^{-1} A + \lambda D)^{-1} A^T \Sigma_y^{-1} Y.$$

(4)

[0056] Next, an operation of the sparseness applying part 244 will be described in detail. Note that an estimated solution $X_R^\wedge$ using a Tikhonov regularization method in a case where a regularization term is normalized with a sensitivity term has some problems. That is, there are problems in which correction according to the sensitivity significantly acts on a portion not requiring the correction because a solution cannot be localized, resulting in a significant error in the estimated position, and in which the space resolution is low. Thus, in order to further improve the solution, the sparseness applying part 244 performs hierarchical Bayesian estimation in which the estimated solution $X_R^\wedge$ is used as an initial value. That is to say, the sparseness applying part 244 introduces "sparseness" where the estimated solution is represented in the minimum region. It narrows down results obtained by the operation of the correcting part 243 correcting the sensitivity to an important location, thereby realizing a high space resolution. With this operation, the depth is also more correctly estimated.

[0057] The hierarchical Bayesian estimation represents not only the generation of observation values but also the regularization as a hierarchical probability model as follows. Firstly, an observation model of an observed light intensity change Y at an internal light absorbance change X is represented by Equation 5 below.

$$P(Y|X) = N(Y|AX, \Sigma_y), \quad (5)$$

[0058] In Equation 5, a normal distribution of an average μ and a covariance matrix Σ is $N(x|\mu, \Sigma)$. Σ_y is an observation noise covariance matrix of an observed value Y. Secondly, it is assumed that a solution X is given by normal distribution with a zero mean vector and a diagonal covariance matrix $\Lambda = \text{diag}(\lambda_1, \lambda_2, \dots, \lambda_N)$ whose diagonal elements are adjustable parameters.

$$P(X|\Lambda) = N(X|0, \Lambda^{-1}). \quad (6)$$

[0059] This sort of prior distribution is referred to as automatic relevance determination (ARD) prior distribution. Furthermore, A is obtained from a probability distribution shown in Equation 7 below.

$$P(\Lambda) = \prod_{i=1}^N \Gamma(\lambda_i | \lambda_{pi}, \gamma_{pi}), \quad (7)$$

[0060] In Equation 7, a gamma distribution with the average μ and the shape parameter γ is $\Gamma(x|\mu, \gamma)$. Furthermore,

λ_{pi} is an average of the prior distribution, and γ_{pi} is a reliability parameter thereof. For example, it is assumed that " $\gamma_{pi} = 0$ ". If " $\gamma_{pi} = 0$ ", Equation 7 is non-informative prior distribution, and γ_{pi} does not affect the probability model.

[0061] According to the Bayesian method, a posterior distribution $P(X, \Lambda | Y)$ of X and Λ in a state where an observed value Y is given is obtained (see Equation 8).

$$P(X, \Lambda | Y) = \frac{P(X | \Lambda) P(\Lambda)}{P(Y)} \quad (8)$$

[0062] However, a posterior distribution cannot be analytically obtained. Calculation of the posterior distribution can be considered as maximization of free energy using a variational Bayesian method as described later. The free energy is represented by Equation 9 below. In Equation 9, $f(\Lambda)$ is a prior distribution term. The free energy can be maximized by iterative calculation as described later.

$$F = -\frac{1}{2} \left[|| \Sigma_y^{-\frac{1}{2}} (Y - AX) ||^2 + || \Lambda^{\frac{1}{2}} X ||^2 + f(\Lambda) \right] \quad (9)$$

[0063] According to Equation 2 of the Tikhonov regularization method, a regularization parameter λ common to all internal states X_i is used and a uniform penalty is applied, so that a smoothed solution is obtained. On the other hand, according to Equation 9 of the hierarchical Bayesian estimation, a regularization parameter $\Lambda = \text{diag}(\lambda_1, \dots, \lambda_N)$ that varies for each voxel is used and is applied to data, so that a sparseness effect can be obtained (see "A. C. Faul and M. E. Tipping, "Analysis of sparse Bayesian learning," Adv. Neural Inf. Process. Syst. 14 (2002) 383-389."). The sparseness applying part 244 substitutes the estimated solution $X^{\wedge}_R$ obtained using the Tikhonov regularization method for an initial value λ_{0i} of iterative calculation (described later), and performs estimation. Exactly speaking, the sparseness applying part 244 performs scale correction of a noise term in Equation 5 and introduction of a smoothing filter in Equation 6, which will be described later.

[0064] Above, the outline of the hierarchical Bayesian estimation method has been described. Hereinafter, detailed settings will be described. Firstly, T time sample data sets are obtained in the measurement. Thus, extension is performed such that " $Y = (Y(1), \dots, Y(t), \dots, Y(T))$ ", and the light absorbance change is accordingly extended such that " $X = (X(1), \dots, X(t), \dots, X(T))$ " in accordance with the time. Furthermore, the observation noise covariance matrix is set to a constant multiple of the noise covariance matrix measured on the base line " $\Sigma_y = \sigma^{-1} \Sigma_{y0}$ ", a prior distribution is given to its coefficient σ , and its value is determined by estimation (see Equation 10).

$$P(Y | X, \sigma) = N(Y | AX, \sigma^{-1} \Sigma_{y0}), P(\sigma) \propto \sigma^{-1}, \quad (10)$$

[0065] Furthermore, if the non-linear effect is high, for example, if the probe interval is 13 mm, this aspect is incorporated as noise, and a term proportional to a square value Y^2 of the observed value is added to the diagonal terms of the observation noise Σ_y . Furthermore, in order to prevent the solution from being too sparse, the solution X is obtained as " $X = WZ$ " by multiplying a smoothing filter W by a sparse representation Z of the solution, and an ARD prior distribution is applied to Z . Accordingly, the probability distribution X is given as follows.

$$P(X | \Lambda) = N(X | 0, W \Lambda^{-1} W^T) \quad (11)$$

[0066] Equation 11 is obtained by extending Equation 6 in a more suitable form. Note that, for example, W is a Gaussian filter having a full width at half maximum of 5 mm. In this case, the posterior distribution is given as Equations 12 and 13 below.

$$P(X, \Lambda, \sigma | Y) = \frac{P(Y, X, \Lambda, \sigma)}{P(Y)}, \quad (12)$$

$$\begin{aligned} \log P(Y, X, \Lambda, \sigma) &= \log P(Y|X, \sigma) + \log P(X|\Lambda) + \log P(\Lambda) + \log P(\sigma) \\ &= -\frac{1}{2} \sum_{t=1}^T [(Y(t) - AX(t))^T \sigma \Sigma_{y0}^{-1} (Y(t) - AX(t)) + X(t)^T W^{-1T} \Lambda W^{-1} X(t)] \\ &\quad - \sum_{i=1}^N \gamma_{pi} \lambda_{pi}^{-1} \lambda_i + \sum_{i=1}^N (\gamma_{pi} + \frac{T}{2} - 1) \log \lambda_i + (\frac{MT}{2} - 1) \log \sigma + \text{const.} \end{aligned} \quad (13)$$

[0067] Since the posterior distribution cannot be analytically obtained, a variational Bayesian method is used. In the variational Bayesian method, instead of directly calculating the posterior distribution, a trial posterior distribution $Q(X, \Lambda, \sigma)$ is prepared, and approximation of true posterior distribution $P(X, \Lambda, \sigma | Y)$ is performed. This approximation is performed by maximizing a free energy $F(Q)$ defined by Equations 14 and 15 below.

$$F(Q) = \int dX d\Lambda d\sigma Q(X, \Lambda, \sigma) \log \frac{P(Y, X, \Lambda, \sigma)}{Q(X, \Lambda, \sigma)}, \quad (14)$$

$$F(Q) = \log P(Y) - \text{KL}[Q(X, \Lambda, \sigma) || P(X, \Lambda, \sigma | Y)]. \quad (15)$$

[0068] Equation 15 is obtained by rewriting Equation 14. In Equation 15, KL is a Kullback-Leibler distance. The first term in Equation 15 does not depend on Q , and, thus, the maximizing the free energy is equivalent to the minimizing the Kullback-Leibler distance between the true posterior distribution and the trial posterior distribution in the second term.

[0069] In this case, if an factorization assumption is placed between X and Λ, σ in the trial posterior distribution, the calculation can be easily performed (see Equation 16).

$$Q(X, \Lambda, \sigma) = Q_X(X) Q_{\Lambda}(\Lambda, \sigma). \quad (16)$$

[0070] With this assumption, the free energy can be maximized by alternately repeating an "X maximizing step" of maximizing $F(Q)$ regarding Q_X and a " Λ, σ maximizing step" of maximizing $F(Q)$ regarding Q_{Λ} .

[0071] In this case, the free energy is represented by Equation 17 below.

$$\begin{aligned} F &= -\frac{1}{2} \sum_{t=1}^T [(Y(t) - AX(t))^T \sigma \Sigma_{y0}^{-1} (Y(t) - AX(t)) + X(t)^T W^{-1T} \Lambda W^{-1} X(t)] \\ &\quad - \frac{T}{2} \log |\Lambda W \Lambda^{-1} W^T A^T + \sigma^{-1} \Sigma_{y0}| + \sum_{i=1}^N \gamma_{pi} [\log(\lambda_i / \lambda_{pi}) - \lambda_i / \lambda_{pi} + 1] \\ &= -\frac{1}{2} [\sigma || \Sigma_{y0}^{-1} (Y - AX) ||^2 + || \Lambda^{\frac{1}{2}} W^{-1} X ||^2 + f(\Lambda, \sigma)]. \end{aligned} \quad (17)$$

[0072] Equation 9 is obtained by simplifying Equation 17. In Equation 17, X, Λ , and σ represent an expected value of the distribution.

[0073] Next, an algorithm of the hierarchical Bayesian estimation performed by the sparseness applying part 244 will be described.

[0074] The sparseness applying part 244 repeats "X maximizing step" and " Λ, σ maximizing step" K times (e.g., K = 1000) with an initial value $\lambda_{0i} = (10 \cdot X_{Ri})^{-2}$ and $\sigma_0 = 1$.

[0075] Note that the "X maximizing step" is represented by Equations 18 to 20 below, and the " Λ, σ maximizing step" is represented by Equation 21 to 24 below.

[0076] Lastly, the sparseness applying part 244 performs the "X maximizing step", thereby obtaining a solution $X_B^\wedge$ (see Equation 25).

$$\Sigma_k = \sigma_{k-1}^{-1} \Sigma_{y0} + AW \Lambda_{k-1}^{-1} W^T A^T, \quad (18)$$

$$H_k = \text{diag}[\Lambda_{k-1}^{-1} W^T A^T \Sigma_k^{-1} Y Y^T \Sigma_k^{-1} AW + T(1 - \Lambda_{k-1}^{-1} W^T A^T \Sigma_k^{-1} AW)], \quad (19)$$

$$I_k = \text{tr}[\sigma_{k-1}^{-1} \Sigma_{y0} \Sigma_k^{-1} Y Y^T \Sigma_k^{-1} + T \Lambda_{k-1}^{-1} W^T A^T \Sigma_k^{-1} AW]. \quad (20)$$

$$r_{k,i} = r_{pi} + \frac{T}{2} \quad (21)$$

$$r_{k,i} \lambda_{k,i}^{-1} = r_{pi} \lambda_{pi}^{-1} + \frac{1}{2} H_{k,i,i} \lambda_{k-1,i}^{-1} \quad (22)$$

$$r_{\sigma k} = \frac{1}{2} MT \quad (23)$$

$$r_{\sigma k} \sigma_k^{-1} = \frac{1}{2} I_k \sigma_{k-1}^{-1} \quad (24)$$

$$\hat{X}_B = W \Lambda_{K-1}^{-1} W^T A^T \Sigma_K^{-1} Y \quad (25)$$

In Equations 21 and 23, T is the number of time sample data sets. In Equation 23, M is the number of channels.

[0077] The output unit 25 outputs the optical characteristic-changed region information acquired by the sparseness applying part 244. Typically, the output unit 25 graphically outputs the optical characteristic-changed region information. However, there is no limitation on the output mode of the optical characteristic-changed region information.

[0078] The output is a concept that encompasses display on a display screen, projection using a projector, printing in a printer, output of a sound, transmission to an external apparatus, accumulation in a storage medium, and delivery of a processing result to another processing apparatus or another program.

[0079] The reference light intensity information storage unit 21, the sensitivity information storage part 241, and the

arithmetic expression storage part 242 are preferably a non-volatile storage medium, but may be realized also by a volatile storage medium.

[0080] There is no limitation on the procedure in which the reference light intensity information and the like are stored in the reference light intensity information storage unit 21 and the like. For example, the reference light intensity information and the like may be stored in the reference light intensity information storage unit 21 and the like via a storage medium, the reference light intensity information and the like transmitted via a communication line or the like may be stored in the reference light intensity information storage unit 21 and the like, or the reference light intensity information and the like input via an input device may be stored in the reference light intensity information storage unit 21 and the like.

[0081] The light intensity information acquiring unit 22, the light intensity change information acquiring unit 23, the estimating unit 24, the correcting part 243, and the sparseness applying part 244 may be realized typically by a CPU, a memory, or the like. Typically, the processing procedure of the light intensity information acquiring unit 22 and the like is realized by software, and the software is stored in a storage medium such as a ROM. Note that the processing procedure may be realized also by hardware (a dedicated circuit).

[0082] The output unit 25 may be considered to include or not to include an output device such as a display screen. The output unit 25 may be realized, for example, by driver software for an output device, a combination of driver software for an output device and the output device, or the like.

[0083] Next, an operation of the object observing apparatus 2 will be described with reference to the flowchart in FIG. 2.

[0084] (Step S201) The light intensity information acquiring unit 22 acquires light intensity information, which is information regarding a light intensity of light received by each light-receiving probe, in a case where light with a certain light intensity is transmitted from each light-transmitting probe forming each probe set to an object.

[0085] (Step S202) The light intensity change information acquiring unit 23 reads reference light intensity information from the reference light intensity information storage unit 21.

[0086] (Step S203) The light intensity change information acquiring unit 23 calculates light intensity change information from the light intensity information acquired in step S201 and the reference light intensity information read in step S202.

[0087] (Step S204) The estimating unit 24 reads an arithmetic expression from the arithmetic expression storage part 242.

[0088] (Step S205) The estimating unit 24 reads sensitivity information from the sensitivity information storage part 241. For example, the sensitivity information is calculated in advance by the estimating unit 24 and is stored in the sensitivity information storage part 241.

[0089] (Step S206) The estimating unit 24 estimates optical characteristic-changed region information using the light intensity change information. This processing is referred to as estimation processing. Hereinafter, the estimation processing will be described with reference to the flowchart in FIG. 3.

[0090] (Step S207) The output unit 25 outputs the optical characteristic-changed region information acquired by the sparseness applying part 244. The procedure returns to step S201.

[0091] Note that the process is terminated by powering off or an interruption at completion of the process in the flowchart in FIG. 2.

[0092] Next, the estimation processing in step S206 will be described with reference to the flowchart in FIG. 3.

[0093] (Step S301) The correcting part 243 performs correction according to sensitivity attenuation in accordance with the depth, using the sensitivity information in the sensitivity information storage part 241. That is to say, the correcting part 243 substitutes the sensitivity information for the first arithmetic expression (arithmetic expression for performing estimation processing of optical characteristic-changed region information with correction according to the sensitivity), thereby acquiring first optical characteristic-changed region information.

[0094] (Step S302) The sparseness applying part 244 introduces sparseness for improving the space resolution, using the first optical characteristic-changed region information acquired in step S301 as input, thereby acquiring final optical characteristic-changed region information.

[0095] Hereinafter, experiments using the object observing system in this embodiment will be described. FIG. 4 is a schematic diagram of an experiment (phantom experiment) using the object observing system. In this phantom experiment, near-infrared light was transmitted from one direction to an object, and backscattered light was received from the same direction as the one direction. Furthermore, in this experiment, a tank phantom was used to obtain data for examining the estimation method realized by the object observing apparatus 2.

[0096] In this experiment, near-infrared light was transmitted and received by the light-transmitting probes 11 and the light-receiving probes 12 at a bottom face of the phantom tank. FIG. 5 is a diagram illustrating positions of the light-transmitting probes 11 and the light-receiving probes 12 and positions of light absorbing members. In FIG. 5, gray circles represent the light-transmitting probes 11, and white circles represent the light-receiving probes 12. The probes are arranged at intervals of l . Hereinafter, the positions at which the light absorbing members were placed will be described. In FIG. 5, (a) is the center (coordinate values $(0, 0)$), (b) is a middle point $(-1/2, 0)$, (c) is the position of one source (the light-transmitting probe 11) $(-1/2, -1/2)$, (d) is the position of one detector (the light-receiving probe 12) $(-1/2, +1/2)$, and (e) is the position of a second light absorbing member $(-1/2+d, 0)$. In the diagram, the horizontal distance between two

light absorbing members is d.

[0097] In this experiment, the tank was filled with 1.4% Intralipid and ink mixture liquid so as to realize the optical characteristics similar to those of the grey matter of the cerebral cortex. The estimated values of the optical parameters based on measurement using a spectrophotometer and a near-infrared imaging device were as follows: absorption coefficient $\mu_a = 0.019 \text{ mm}^{-1}$; and reduced scattering coefficient $\mu'_s = 1.1 \text{ mm}^{-1}$.

[0098] A light absorbance change was measured using a near-infrared imaging device (FOIRE-3000, Shimadzu Corporation). In this experiment, only a wavelength of 805 nm was used for measurement. Near-infrared light was irradiated in a time-divided manner from the light-transmitting probes 11 arranged on a square grid on the bottom face "z = 0" of the tank, and was received by the light-receiving probes 12. The sampling rate was set to 130 ms, and the measurement was performed for 20 seconds/each. The experiment was performed with three types of probe intervals, namely 13 mm, 18.4 mm (= 13 mm $\times \sqrt{2}$), and 26 mm (= 13 mm $\times 2$).

[0099] Furthermore, in the experiment, one or two spherical light absorbing members each having a diameter of 5 mm were arranged in the liquid. In the experiment with one light absorbing member, measurement was performed for four points, namely (a) the center, (b) the middle point between the light-transmitting probe 11 and the light-receiving probe 12, (c) the position directly below the light-transmitting probe 11, and (d) the position directly below the light-receiving probe 12 (see FIG. 5). In the experiment with two light absorbing members, measurement was performed while arranging the light absorbing members at (b) and (e), which was apart from (b) by d.

Experiment 1

[0100] Hereinafter, a three-dimensional reconstruction method using observation data in an actual phantom experiment will be described. In Experiment 1, the data measurement condition was such that the light-transmitting probes 11 and the light-receiving probes 12 arranged on the plane with z = 0 were used for measurement (see FIG. 6). The probe interval in Experiment 1 was set to 18.4 mm. Two spherical light absorbing members each having a diameter of 5 mm were arranged to cause light absorbance changes. The center coordinates (x, y, z) of the two light absorbing members were respectively (-9.2 mm, 0 mm, 10 mm) and (3.3 mm, 0 mm, 15 mm), that is, they were apart from each other by 12.5 mm in the horizontal direction and 5 mm in the vertical direction, which were distances shorter than the probe interval. Note that the coordinate system in FIG. 6 is obtained by turning that in FIG. 4 upside down. The reason for this is to make the coordinate system correspond to that in measurement of the brain functions where the probe plane is typically positioned on the upper side.

[0101] FIG. 7 is an estimation result using the Tikhonov regularization method in a case where D was taken as an identity matrix. Note that taking D as an identity matrix means not performing correction of the regularization term according to the sensitivity attenuation. As shown in FIG. 7, the position obtained as a solution was closer to the probe plane than the actual position was because the sensitivity was exponentially attenuated in accordance with the depth. Furthermore, as shown in FIG. 7, two light absorbance changes were not separated from each other.

[0102] FIG. 8 is an estimation result in a case where the regularization term is normalized with the sensitivity FIG. 8 shows a result that conversely seems to be biased in the depth direction, which is meaningful. Shallow and weak activities and deep and strong activities provide similar observed values, and the Tikhonov regularization method cannot localize the solution, and, thus, the estimation result is obtained as an overlap (coexistence) state thereof. It seems that, since deep and strong activities are more outstanding, the estimation result seems to be biased in the depth direction.

[0103] FIG. 9 is obtained by performing estimation, using the result in FIG. 8 as an initial value " $\lambda_{oi} = (10 \cdot X_{Ri})^{-2}$ " in the hierarchical Bayesian method. That is to say, FIG. 9 shows an estimation result (acquisition result of the optical characteristic-changed region information) by the object observing apparatus 2. Since the estimation result of the Tikhonov regularization method is excessively smoothed, a value obtained by multiplying ten by the estimated value was used as an initial value (the same is applied to other experiments below). The sparseness applying part 244 of the estimating unit 24 uses the hierarchical Bayesian algorithm to select an appropriate state from among various solution overlap states obtained in FIG. 8. Accordingly, the sparseness applying part 244 obtains a more accurate estimation result. In Experiment 1, each position of the two light absorbing members was identified, and a difference from the actual positions was one voxel or smaller.

Experiment 2

[0104] In Experiment 2, it was examined whether or not the depth was correctly estimated by placing the light absorbing member at the center position ((a) in FIG. 5) and changing the depth by 2.5 mm each time. The measurement was performed with three types of probe intervals, namely 26 mm, 18.4 mm, and 13 mm.

[0105] FIG. 10 shows a result of estimation performed by the object observing apparatus 2 while changing the probe interval and the depth position of the light absorbing member (exemplary output of the optical characteristic-changed region information by the output unit 25). In order to express a three-dimensional estimation diagram in two dimensions,

the estimation result is shown such that only the maximum values of three voxels in the vicinity of the center containing the light absorbing member in the y direction are projected on the respective x-z planes as shown in FIG. 11. In FIG. 10, estimation results are shown with a probe interval $l = 26$ mm, 18.4 mm, and 13 mm sequentially from above, and with a true depth z at the center of the light absorbing member = 7.5 mm, 10 mm, 12.5 mm, 15 mm, 17.5 mm, 20 mm, and 22.5 mm sequentially from the left. In FIG. 10, white circles represent the true position of the light absorbing member. If a positional error of the estimation result on each of the x, y, and z axes was one voxel or smaller (2.5 mm or less) and an estimated maximum value was 0.025 mm^{-1} or more, it is considered that the estimation was performed, and the corresponding graph is enclosed by a heavy line.

[0106] In the uppermost line (result with a probe interval of 26 mm) in FIG. 10, the estimation results indicate the same depth in the case where the true depth z of the light absorbing member was 7.5 mm to 15 mm (see the left graph in FIG. 12). This result indicates that it was not substantially possible to estimate the depth. Furthermore, it was not possible to perform the estimation in the case where z was 17.5 mm or more.

[0107] In the middle line (result with a probe interval of 18.4 mm) in FIG. 10, in the case where the true depth z of the light absorbing member was 7.5 mm to 20 mm, the estimation was possible and the true depth and the estimated depth matched each other within an error of one voxel or smaller (see the middle graph in FIG. 12).

[0108] In the lowermost line (result with a probe interval of 13 mm) in FIG. 10, in the case where the true depth z of the light absorbing member was 7.5 mm to 22.5 mm, the estimation was possible and the true depth and the estimated depth matched each other within an error of one voxel or smaller (see the right graph in FIG. 12). It was seen that the depth of a region with a light absorbance change can be accurately estimated in this manner according to high density measurement with a probe interval of 18.4 mm or 13 mm, for example.

[0109] Next, in order to investigate the degree of the estimation result depending on the probe relative position, the limit depth was checked at which a positional error of the estimation result on each of the x, y, and z axes was one voxel or smaller and an estimated maximum value was 0.025 mm^{-1} or more, by placing the light absorbing member at one of the four locations, namely (a) the center, (b) the middle point, (c) the position of the light-transmitting probe 11, and (d) the position of the light-receiving probe 12 in FIG. 5, and increasing the depth by 2.5 mm each time. FIG. 13 shows the result. Note that, in the case where the probe interval was 26 mm, estimation of the depth was not possible, and, thus, correct values of only x and y were regarded as sufficient. It is seen that, with high density measurement, the estimation can be accurately performed without so much depending on the position of the light absorbing member. Furthermore, it is seen that the depth that can be estimated increases as the probe interval is shorter.

Experiment 3

[0110] In Experiment 3, in order to check the space resolution according to the hierarchical Bayesian method used by the object observing apparatus 2, the number of light absorbing members was increased to two, and the experiment was performed. The x, y coordinates of the light absorbing members were respectively set to $(-1/2, 0)$ and $(-1/2+d, 0)$ ((b) and (e) in FIG. 5), and the horizontal distance between the centers was indicated as d .

[0111] Experiment 3 was carried out only with two types of probe intervals, namely 18.4 mm and 13 mm. Since Experiment 2 shows that three-dimensional reconstruction is not possible in the case where the probe interval is 26 mm, this probe interval was not applied to Experiments 3 and 4.

[0112] FIG. 14 shows an output result (estimation result) of the object observing apparatus 2 at a probe interval of 18.4 mm. This experiment was performed while changing the horizontal distance d and the depth z of the two light absorbing members by 2.5 mm each time. In order to express a three-dimensional estimation diagram in two dimensions as in FIG. 10, the estimation result is shown such that only the maximum values of three voxels in the vicinity of the center containing the light absorbing members in the y direction are projected on the respective x-z planes as shown in FIG. 11. In FIG. 14, estimation results are shown with a horizontal distance $d = 17.5$ mm, 15 mm, 12.5 mm, and 10 mm sequentially from above, and with a true depth z at the center of the light absorbing members = 12.5 mm, 15 mm, 17.5 mm, and 20 mm sequentially from the left.

[0113] If the two light absorbing members were apart from each other by a distance similar to the probe interval as in the case of " $d = 17.5$ mm, $z = 17.5$ mm" shown in FIG. 14, the positions of the two light absorbing members were accurately estimated up to a depth $z = 17.5$ mm.

[0114] Furthermore, the estimation was possible also in a case where the distance between the two light absorbing members was shorter than the probe interval. In particular, in the case where the probe interval was 18.4 mm, it was possible to identify the two light absorbing members located such that the distance d between their centers was 10 mm (distance between the outside edges of 5-mm spheres was 5 mm), that is, such that they were apart from each other by a distance approximately half the probe interval (see the diagram with " $d = 10$ mm, $z = 15$ mm" in FIG. 14).

[0115] FIG. 15 is a table showing the limit depths at which, in both of the two light absorbing members, a positional error of the estimation result on each of the x, y, and z axes was one voxel or smaller and an estimated absorption coefficient change was 0.025 mm^{-1} or more, obtained through the experiment setting the probe interval to two types,

namely 18.4 mm and 13 mm and the horizontal distance d between the two light absorbing members to 15 mm, 12.5 mm, 10 mm, and increasing the depth z of the light absorbing members by 2.5 mm each time.

Experiment 4

[0116] In order to see whether or not three-dimensional estimation including the depth is possible even under complex conditions, Experiment 4 was carried out. Experiment 4 was carried out with two light absorbing members located at depths different from each other by 5 mm. As in Experiment 3, the x , y coordinates of the light absorbing members were respectively set to $(-1/2, 0)$ and $(-1/2+d, 0)$ ((b) and (e) in FIG. 5), and the horizontal distance between the centers was indicated as d . Furthermore, the light absorbing member at (b) was placed at a position shallower than the light absorbing member at (e) by 5 mm. Experiment 4 was carried out only with two types of probe intervals at which the depth estimation was possible, namely 18.4 mm and 13 mm.

[0117] FIG. 16 shows an estimation result at a probe interval of 18.4 mm. Experiment 4 was performed while changing the horizontal distance d and the depth z of the two light absorbing members by 2.5 mm each time. In order to express a three-dimensional estimation diagram in two dimensions as in FIG. 10, the estimation result is shown such that only the maximum values of three voxels in the vicinity of the center containing the light absorbing members in the y direction are projected on the respective x - z planes.

[0118] As seen from FIG. 16, if the two light absorbing members were apart from each other by a distance similar to the probe interval as in the case of " $d = 17.5$ mm, $z = 15$ & 20 mm" shown in FIG. 16, the position of one light absorbing member at an estimation limit depth $z = 20$ mm was accurately estimated without being interrupted by the other light absorbing member located at a shallower position.

[0119] Furthermore, the estimation was possible also in a case where the distance between the two light absorbing members was shorter than the probe interval. It seems that, even if there are multiple light absorbing members located at different depths, high space resolution can be obtained according to the estimation method used by the object observing apparatus 2.

[0120] FIG. 17 is a table showing the limit depths at which, in both of the two light absorbing members, a positional error of the estimation result on each of the x , y , and z axes was one voxel or smaller and an estimated absorption coefficient change was 0.025 mm^{-1} or more, obtained through the experiment setting the probe interval to two types, namely 18.4 mm and 13 mm and the horizontal distance d between the two light absorbing members to 15 mm, 12.5 mm, 10 mm, and increasing the depth z of the light absorbing members by 2.5 mm each time.

[0121] As described above, this embodiment can accurately estimate, as three-dimensional information, a local optical characteristic-changed region inside an object. More specifically, a local optical characteristic-changed region inside an object can be accurately estimated as three-dimensional information by the high-accuracy three-dimensional reconstruction algorithm including the depth direction, used by this object observing system. Note that the reconstruction algorithm used by the object observing system includes two steps below. Firstly, estimation is performed using the Tikhonov regularization method in which the regularization term is normalized with the sensitivity, so that spatially extended solution candidates are obtained. Secondly, hierarchical Bayesian estimation is performed using the estimation result as an initial value, so that solution candidates are narrowed down to a more appropriate solution.

[0122] According to the phantom experiments in this embodiment, in the case where the probe interval was 26 mm, it was not possible for the reconstruction algorithm to operate well due to a lack of observation information, whereas, in the case where the probe interval was 18.4 mm and 13 mm, it was possible to accurately estimate the depth and to identify the two light absorbing members apart from each other by a distance shorter than the probe interval. In particular, in the case where the probe interval was 18.4 mm, it was possible to identify the two light absorbing members located such that the distance between their centers was 10 mm, that is, such that they were apart from each other by a distance approximately half the probe interval.

[0123] Furthermore, according to this embodiment, the object observing apparatus 2 introduces sparseness using the hierarchical Bayesian method. However, in this embodiment, it is also possible to introduce sparseness, using an L1 norm. For example, if the second power of the regularization term in Equation 2 is changed to the first power, normalization with the sensitivity and introduction of the sparseness can be simultaneously performed.

[0124] Note that estimation using L1 regularization was also actually performed. Also with L1 regularization, the solution becomes sparse, and, thus, a smoothing filter W was introduced in this experiment under the same conditions as those in the case of using the hierarchical Bayesian method. As a result of application to the experimental data, it was found that, if an appropriate regularization parameter λ is selected, the estimation can be performed at approximately the same level of precision as the hierarchical Bayesian method. Note that it was seen from this experiment that the correction with the sensitivity and the application of the sparseness can be simultaneously performed. That is to say, the estimating unit, in which sensitivity information, which is information indicating a relationship between an optical characteristic change and a light intensity change, is stored, may perform correction according to sensitivity attenuation in accordance with a depth, using the sensitivity information, and introduce sparseness for improving a space resolution, thereby

acquiring optical characteristic-changed region information, wherein the correction with the sensitivity and the application of the sparseness may be simultaneously performed or may be sequentially performed.

[0125] Furthermore, the processing in this embodiment may be realized using software. The software may be distributed by software download or the like. Furthermore, the software may be distributed in a form where the software is stored in a storage medium such as a CD-ROM. Note that the same is applied to other embodiments described in this specification. The software that realizes the object observing apparatus 2 in this embodiment may be the following sort of program. Specifically, this program is a program using a storage medium in which reference light intensity information, which is information regarding a light intensity at each light-receiving probe, and is information used as a reference, is stored, the program causing a computer to function as: a light intensity information acquiring unit that, using a near-infrared measurement apparatus having at least one probe set consisting of a pair of a light-transmitting probe for transmitting light to an object that is to be observed and a light-receiving probe for receiving light, acquires light intensity information, which is information regarding a light intensity of light received by each light-receiving probe, in a case where light with a certain light intensity is transmitted from each light-transmitting probe forming each probe set to the object; a light intensity change information acquiring unit that acquires, for each probe set, light intensity change information, which is information regarding a light intensity change, from the reference light intensity information in the storage medium and the light intensity information acquired by the light intensity information acquiring unit; an estimating unit that acquires optical characteristic-changed region information, which is three-dimensional information regarding a position with a light absorbance change inside the object, using the light intensity change information for each probe set; and an output unit that outputs the optical characteristic-changed region information acquired by the estimating unit; wherein the estimating unit includes: a correcting part that performs correction according to sensitivity attenuation in accordance with a depth, using sensitivity information, which is information indicating a relationship between an optical characteristic change and a light intensity change; and a sparseness applying part that introduces sparseness for improving a space resolution, thereby acquiring the optical characteristic-changed region information.

[0126] Furthermore, in this program, it is preferable that the computer is caused to function such that the estimating unit further includes an arithmetic expression storage part, in which a first arithmetic expression, which is an arithmetic expression used for acquiring the optical characteristic-changed region information, is an arithmetic expression for calculating a solution of an inverse problem, and is a cost function for performing correction according to the sensitivity information, can be stored, the correcting part substitutes the sensitivity information for the first arithmetic expression, thereby acquiring first optical characteristic-changed region information, the sparseness applying part acquires final optical characteristic-changed region information using the sparseness for improving the space resolution, using the first optical characteristic-changed region information, and the output unit outputs the optical characteristic-changed region information acquired by the sparseness applying part.

[0127] Furthermore, in this program, it is preferable that the computer is caused to function such that, in the arithmetic expression storage part, a second arithmetic expression for performing hierarchical Bayesian estimation on an initial value is also stored, and the sparseness applying part substitutes the first optical characteristic-changed region information as an initial value for the second arithmetic expression, and executes the second arithmetic expression to perform hierarchical Bayesian estimation, thereby acquiring final optical characteristic-changed region information.

[0128] Furthermore, in this program, it is preferable that the computer is caused to function for observing a brain function of a living body, wherein the object that is to be observed is the brain of the living body, and the reference light intensity information is information regarding a light intensity at each light-receiving probe measured at rest.

[0129] Furthermore, in this program, it is preferable that the computer is caused to function for screening of breast cancer, wherein the object that is to be observed is a breast, and the reference light intensity information is information regarding a light intensity at each light-receiving probe from a breast with normal cells.

[0130] Furthermore, in this program, it is preferable that the computer is caused to function such that each interval between the light-transmitting and light-receiving probes is not greater than 20 mm.

[0131] FIG. 18 shows the external appearance of a computer that executes the programs described in this specification to realize the object observing apparatus 2 and the like in the foregoing embodiments. The foregoing embodiments may be realized using computer hardware and a computer program executed thereon. FIG. 18 is a schematic view of the computer system. FIG. 19 is a block diagram of the computer system.

[0132] In FIG. 18, the computer system 340 includes a computer 341 including an FD drive and a CD-ROM drive, a keyboard 342, a mouse 343, and a monitor 344.

[0133] In FIG. 19, the computer 341 includes not only the FD drive 3411 and the CD-ROM drive 3412, but also a CPU 3413, a bus 3414 that is connected to the CD-ROM drive 3412 and the FD drive 3411, a RAM 3416 in which a command of an application program is temporarily stored and a temporary storage area is to be provided, and that is connected to a ROM 3415 in which a program such as a boot up program is to be stored, and a hard disk 3417 in which an application program, a system program, and data are to be stored. Although not shown, the computer 341 may further include a network card that provides connection to a LAN.

[0134] The program for causing the computer system 340 to execute the functions of the object observing apparatus

and the like in the foregoing embodiments may be stored in a CD-ROM 3501 or an FD 3502, inserted into the CD-ROM drive 3412 or the FD drive 3411, and transmitted to the hard disk 3417. Alternatively, the program may be transmitted via an unshown network to the computer 341 and stored in the hard disk 3417. At the time of execution, the program is loaded into the RAM 3416. The program may be loaded from the CD-ROM 3501 or the FD 3502, or directly from a network.

[0135] The program does not necessarily have to include, for example, an operating system (OS) or a third party program to cause the computer 341 to execute the functions of the object observing apparatus and the like in the foregoing embodiments. The program may only include a command portion to call an appropriate function (module) in a controlled mode and obtain the desired results. The manner in which the computer system 340 operates is well known, and, thus, a detailed description thereof has been omitted.

[0136] Furthermore, the computer that executes this program may be a single computer, or may be multiple computers. More specifically, centralized processing may be performed, or distributed processing may be performed.

[0137] Furthermore, in the foregoing embodiments, each process (each function) may be realized as an integrated process using a single apparatus (system), or may be realized as a distributed process using multiple apparatuses.

[0138] It will be appreciated that the present invention is not limited to the embodiments set forth herein, and various modifications are possible within the scope of the present invention, which is defined by the appended claims.

Industrial Applicability

[0139] As described above, the object observing system according to the present invention has an effect that this system can accurately estimate, as three-dimensional information, a local optical characteristic-changed region inside an object, and, thus, this system is useful as a brain function observing system and the like.

Claims

1. An object observing apparatus (2), comprising:

a reference light intensity information storage unit (21) configured to store reference light intensity information, which is information regarding a light intensity at each light-receiving probe, and is information used as a reference;

a light intensity information acquiring unit (22) that, using a near-infrared measurement apparatus (1) having at least one probe set consisting of a pair of a light-transmitting probe (11) for transmitting light to an object that is to be observed and a light-receiving probe (12) for receiving light, is configured to acquire light intensity information, which is information regarding a light intensity of light received by each light-receiving probe (12), in a case where light with a certain light intensity is transmitted from each light-transmitting probe (11) forming each probe set to the object;

a light intensity change information acquiring unit (23) that is configured to acquire, for each probe set, light intensity change information, which is information regarding a light intensity change, from the reference light intensity information in the reference light intensity information storage unit (21) and the light intensity information acquired by the light intensity information acquiring unit (22);

an estimating unit (24) that is configured to acquire optical characteristic-changed region information, which is three-dimensional information regarding a position with a light absorbance change inside the object, using the light intensity change information for each probe set; and

an output unit (25) that is configured to output the optical characteristic-changed region information acquired by the estimating unit (24);

wherein the estimating unit (24), in which sensitivity information, which is information indicating a relationship between an optical characteristic change and a light intensity change, is stored, is configured to perform correction according to sensitivity attenuation in accordance with a depth, using the sensitivity information, and to introduce sparseness for improving a space resolution, thereby acquiring the optical characteristic-changed region information.

2. The object observing apparatus (2) according to claim 1, wherein the estimating unit (24) includes:

a sensitivity information storage part (241) configured to store sensitivity information, which is information indicating a relationship between an optical characteristic change and a light intensity change;

a correcting part (243) that is configured to perform correction according to sensitivity attenuation in accordance with a depth, using the sensitivity information; and

a sparseness applying part (244) that is configured to introduce sparseness for improving the space resolution,

thereby acquiring the optical characteristic-changed region information.

3. The object observing apparatus (2) according to claim 2,
 wherein the estimating unit (24) further includes an arithmetic expression storage part (242), in which a first arithmetic
 expression, which is an arithmetic expression used for acquiring the optical characteristic-changed region informa-
 tion, is an arithmetic expression for calculating a solution of an inverse problem, and is a cost function for performing
 correction according to the sensitivity information, can be stored,
 the correcting part (243) is configured to substitute the sensitivity information for the first arithmetic expression,
 thereby acquiring first optical characteristic-changed region information,
 the sparseness applying part (244) is configured to acquire final optical characteristic-changed region information
 using the sparseness for improving the space resolution, using the first optical characteristic-changed region infor-
 mation, and
 the output unit (25) is configured to output the optical characteristic-changed region information acquired by the
 sparseness applying part (244).
4. The object observing apparatus (2) according to claim 3,
 wherein, in the arithmetic expression storage part (242), a second arithmetic expression for performing hierarchical
 Bayesian estimation on an initial value is also stored, and
 the sparseness applying part (244) is configured to substitute the first optical characteristic-changed region infor-
 mation as an initial value for the second arithmetic expression, and to execute the second arithmetic expression to
 perform hierarchical Bayesian estimation, thereby acquiring final optical characteristic-changed region information.
5. The object observing apparatus (2) according to claim 1, for use in observation of a brain function of a living body,
 wherein the object that is to be observed is the brain of the living body, and
 the reference light intensity information is information regarding a light intensity at each light-receiving probe meas-
 ured at rest.
6. The object observing apparatus (2) according to claim 1, for use in screening of breast cancer,
 wherein the object that is to be observed is a breast, and
 the reference light intensity information is information regarding a light intensity at each light-receiving probe from
 a breast with normal cells.
7. The object observing apparatus (2) according to any one of claims 1 to 6, wherein each interval between the light-
 transmitting and light-receiving probes (11, 12) is not greater than 20 mm.
8. An object observing method using a storage medium in which reference light intensity information, which is information
 regarding a light intensity at each light-receiving probe (12), and is information used as a reference, is stored, and
 realized with a light intensity information acquiring unit (22), a light intensity change information acquiring unit (23),
 an estimating unit (24), and an output unit (25), the object observing method comprising:
 a light intensity information acquiring step of the light intensity information acquiring unit (22), using a near-
 infrared measurement apparatus (1) having at least one probe set consisting of a pair of a light-transmitting
 probe (11) for transmitting light to an object that is to be observed and a light-receiving probe (12) for receiving
 light, acquiring light intensity information, which is information regarding a light intensity of light received by
 each light-receiving probe (12), in a case where light with a certain light intensity is transmitted from each light-
 transmitting probe (11) forming each probe set to the object;
 a light intensity change information acquiring step of the light intensity change information acquiring unit (23)
 acquiring, for each probe set, light intensity change information, which is information regarding a light intensity
 change, from the reference light intensity information in the storage medium and the light intensity information
 acquired in the light intensity information acquiring step;
 an estimating step of the estimating unit (24) acquiring optical characteristic-changed region information, which
 is three-dimensional information regarding a position with a light absorbance change inside the object, using
 the light intensity change information for each probe set; and
 an output step of the output unit (25) outputting the optical characteristic-changed region information acquired
 in the estimating step;

wherein, in the estimating step, correction is performed according to sensitivity attenuation in accordance with a
 depth, using sensitivity information, which is information indicating a relationship between an optical characteristic

change and a light intensity change, and sparseness is introduced for improving a space resolution, so that the optical characteristic-changed region information is acquired.

Patentansprüche

1. Objektbeobachtungsapparatur (2), umfassend:

eine Referenzlichtintensitätsinformation-Speichereinheit (21), die dafür eingerichtet ist, Referenzlichtintensitätsinformation zu speichern, welche eine Information bezüglich einer Lichtintensität bei jeder lichtempfangenden Sonde ist und eine als eine Referenz genutzte Information ist;
 eine Lichtintensitätsinformation gewinnende Einheit (22), die unter Verwendung einer Nahinfrarot-Messvorrichtung (1) mit zumindest einem Sondensatz, der aus einem Paar einer lichtsendenden Sonde (11) zum Senden von Licht zu einem Objekt, das beobachtet werden soll, und einer lichtempfangenden Sonde (12) zum Empfangen von Licht besteht, dafür eingerichtet ist, Lichtintensitätsinformation zu gewinnen, welche eine Information bezüglich einer Lichtintensität von durch jede lichtempfangende Sonde (12) empfangenem Licht ist, falls Licht mit einer bestimmten Lichtintensität von jeder lichtsendenden Sonde (11), die jeden Sondensatz bildet, zum Objekt gesendet wird;
 eine Lichtintensitätsänderungsinformation gewinnende Einheit (23), die dafür eingerichtet ist, für jeden Sondensatz eine Lichtintensitätsänderungsinformation, welche eine Information bezüglich einer Lichtintensitätsänderung ist, aus der Referenzlichtintensitätsinformation in der Referenzlichtintensitätsinformation-Speichereinheit (21) und der Lichtintensitätsinformation zu gewinnen, die durch die Lichtintensitätsinformation gewinnende Einheit (22) gewonnen wurde;
 eine Schätzeinheit (24), die dafür eingerichtet ist, eine Information über einen Bereich mit geänderter optischer Eigenschaft zu gewinnen, welche eine dreidimensionale Information bezüglich einer Position mit einer Änderung einer Lichtabsorbanz innerhalb des Objekts ist, wobei die Lichtintensitätsänderungsinformation für jeden Sondensatz genutzt wird; und
 eine Ausgabereinheit (25), die dafür eingerichtet ist, die durch die Schätzeinheit (24) gewonnene Information über einen Bereich mit geänderter optischer Eigenschaft auszugeben;

wobei die Schätzeinheit (24), in welcher eine Empfindlichkeitsinformation, welche eine Information ist, die eine Beziehung zwischen einer Änderung einer optischen Eigenschaft und einer Lichtintensitätsänderung angibt, gespeichert ist, dafür eingerichtet ist, eine Korrektur gemäß einer Empfindlichkeitsdämpfung entsprechend einer Tiefe durchzuführen, unter Verwendung der Empfindlichkeitsinformation, und Sparseness (engl. sparseness) zum Verbessern einer Raumaufklärung einzuführen, wodurch die Information über einen Bereich mit geänderter optischer Eigenschaft gewonnen wird.

2. Objektbeobachtungsapparatur (2) nach Anspruch 1, wobei die Schätzeinheit (24) umfasst:

einen Empfindlichkeitsinformation-Speicherteil (241), der dafür eingerichtet ist, Empfindlichkeitsinformation zu speichern, welche eine Information ist, die eine Beziehung zwischen einer Änderung einer optischen Eigenschaft und einer Lichtintensitätsänderung angibt;
 einen Korrekturteil (243), der dafür eingerichtet ist, eine Korrektur gemäß einer Empfindlichkeitsdämpfung entsprechend einer Tiefe durchzuführen, wobei die Empfindlichkeitsinformation genutzt wird; und
 einen Sparseness-Anwendungsteil (244), der dafür eingerichtet ist, Sparseness zum Verbessern der Raumaufklärung einzuführen, wodurch die Information über einen Bereich mit geänderter optischer Eigenschaft gewonnen wird.

3. Objektbeobachtungsapparatur (2) nach Anspruch 2,

wobei die Schätzeinheit (24) ferner einen Speicherteil (242) für arithmetische Ausdrücke umfasst, worin ein erster arithmetischer Ausdruck gespeichert werden kann, welcher ein arithmetischer Ausdruck ist, der zum Gewinnen der Information über einen Bereich mit geänderter optischer Eigenschaft genutzt wird, ein arithmetischer Ausdruck ist, um eine Lösung eines inversen Problems zu berechnen, und eine Kostenfunktion ist, um eine Korrektur gemäß der Empfindlichkeitsinformation durchzuführen,
 der Korrekturteil (243) dafür eingerichtet ist, die Empfindlichkeitsinformation für den ersten arithmetischen Ausdruck zu substituieren, wodurch eine erste Information über einen Bereich mit geänderter optischer Eigenschaft gewonnen wird,
 der Sparseness-Anwendungsteil (244) dafür eingerichtet ist, eine finale Information über einen Bereich mit geänderter optischer Eigenschaft zu gewinnen.

derter optischer Eigenschaft unter Verwendung der Sparseness zum Verbessern der Raumauflösung zu gewinnen, wobei die erste Information über einen Bereich mit geänderter optischer Eigenschaft genutzt wird, und die Ausgabeeinheit (25) dafür eingerichtet ist, die Information über einen Bereich mit geänderter optischer Eigenschaft, die durch den Sparseness-Anwendungsteil (244) gewonnen wurde, auszugeben.

4. Objektbeobachtungsanordnung (2) nach Anspruch 3, wobei im Speicherteil (242) für arithmetische Ausdrücke ein zweiter arithmetischer Ausdruck zum Durchführen einer hierarchischen Bayes-Schätzung an einem Anfangswert ebenfalls gespeichert ist, und der Sparseness-Anwendungsteil (244) dafür eingerichtet ist, die erste Information über einen Bereich mit geänderter optischer Eigenschaft als einen Anfangswert für den zweiten arithmetischen Ausdruck zu substituieren und den zweiten arithmetischen Ausdruck auszuführen, um eine hierarchische Bayes-Schätzung durchzuführen, wodurch eine finale Information über einen Bereich mit geänderter optischer Eigenschaft gewonnen wird.

5. Objektbeobachtungsanordnung (2) nach Anspruch 1, zur Verwendung bei einer Beobachtung einer Gehirnfunktion eines lebenden Körpers, wobei das Objekt, das beobachtet werden soll, das Gehirn des lebenden Körpers ist, und die Referenzlichtintensitätsinformation eine Information bezüglich einer Lichtintensität bei jeder lichtempfangenden Sonde, gemessen in Ruhe, ist.

6. Objektbeobachtungsanordnung (2) nach Anspruch 1, zur Verwendung bei der Früherkennung bzw. beim Screening von Brustkrebs, wobei das Objekt, das beobachtet werden soll, eine Brust ist, und die Referenzlichtintensitätsinformation eine Information bezüglich einer Lichtintensität bei jeder lichtempfangenden Sonde von einer Brust mit normalen Zellen ist.

7. Objektbeobachtungsanordnung (2) nach einem der Ansprüche 1 bis 6, wobei jedes Intervall zwischen den lichtsendenden und lichtempfangenden Sonden (11, 12) nicht größer als 20 mm ist.

8. Objektbeobachtungsverfahren, das ein Speichermedium nutzt, in welchem eine Referenzlichtintensitätsinformation, welche eine Information bezüglich einer Lichtintensität bei jeder lichtempfangenden Sonde (12) ist und eine als Referenz genutzte Information ist, gespeichert ist, und realisiert mit einer Lichtintensitätsinformation gewinnenden Einheit (22), einer Lichtintensitätsänderungsinformation gewinnenden Einheit (23), einer Schätzeinheit (24) und einer Ausgabeeinheit (25), wobei das Objektbeobachtungsverfahren umfasst:

einen Lichtintensitätsinformation gewinnenden Schritt der Lichtintensitätsinformation gewinnenden Einheit (22), die unter Verwendung einer Nahinfrarot-Messvorrichtung (1) mit zumindest einem SONDENSATZ, der aus einem Paar einer lichtsendenden Sonde (11) zum Senden von Licht zu einem Objekt, das beobachtet werden soll, und einer lichtempfangenden Sonde (12) zum Empfangen von Licht besteht, eine Lichtintensitätsinformation gewinnt, welche eine Information bezüglich einer Lichtintensität von durch jede lichtempfangende Sonde (12) empfangenem Licht ist, falls Licht mit einer bestimmten Lichtintensität von jeder lichtsendenden Sonde (11), die jeden SONDENSATZ bildet, zum Objekt gesendet wird;

einen Lichtintensitätsänderungsinformation gewinnenden Schritt der Lichtintensitätsänderungsinformation gewinnenden Einheit (23), die für jeden SONDENSATZ eine Lichtintensitätsänderungsinformation, welche eine Information bezüglich einer Lichtintensitätsänderung ist, aus der Referenzlichtintensitätsinformation im Speichermedium und der Lichtintensitätsinformation gewinnt, die im Lichtintensitätsinformation gewinnenden Schritt gewonnen wurde;

einen Schätzschrift der Schätzeinheit (24), die eine Information über einen Bereich mit geänderter optischer Eigenschaft gewinnt, welche eine dreidimensionale Information bezüglich einer Position mit einer Änderung einer Lichtabsorbanz innerhalb des Objekts ist, wobei die Lichtintensitätsänderungsinformation für jeden SONDENSATZ genutzt wird; und

einen Ausgabeschritt der Ausgabeeinheit (25), die die im Schätzschrift gewonnene Information über einen Bereich mit geänderter optischer Eigenschaft ausgibt;

wobei im Schätzschrift eine Korrektur gemäß einer Empfindlichkeitsdämpfung entsprechend einer Tiefe durchgeführt wird, unter Verwendung einer Empfindlichkeitsinformation, welche eine Information ist, die eine Beziehung zwischen einer Änderung einer optischen Eigenschaft und einer Lichtintensitätsänderung angibt, und Sparseness eingeführt wird, um eine Raumauflösung zu verbessern, so dass die Information über einen Bereich mit geänderter optischer Eigenschaft gewonnen wird.

Revendications

1. Appareil d'observation d'objet (2), comprenant :

- 5 une unité de stockage d'informations d'intensité lumineuse de référence (21) conçue pour stocker des informations d'intensité lumineuse de référence, qui sont des informations concernant une intensité lumineuse au niveau de chaque sonde de réception de lumière, et qui sont des informations utilisées comme référence ;
 une unité d'acquisition d'informations d'intensité lumineuse (22) qui, à l'aide d'un appareil de mesure de proche infrarouge (1) comportant au moins un ensemble de sondes constitué par une paire composée d'une sonde
 10 de transmission de lumière (11) pour transmettre la lumière à un objet à observer, et d'une sonde de réception de lumière (12) pour recevoir la lumière, est conçue pour acquérir des informations d'intensité lumineuse, qui sont des informations concernant une intensité lumineuse de la lumière reçue par chaque sonde de réception de lumière (12), dans un cas où la lumière avec une certaine intensité lumineuse est transmise, à partir de chaque sonde de transmission de lumière (11) formant chaque ensemble de sondes, à l'objet ;
 15 une unité d'acquisition d'informations de variation d'intensité lumineuse (23) qui est conçue pour acquérir pour chaque ensemble de sondes des informations de variation d'intensité lumineuse, qui sont des informations concernant une variation d'intensité lumineuse, à partir des informations d'intensité lumineuse de référence contenues dans l'unité de stockage d'informations d'intensité lumineuse de référence (21), et des informations d'intensité lumineuse acquises par l'unité d'acquisition d'informations d'intensité lumineuse (22) ;
 20 une unité d'estimation (24) qui est conçue pour acquérir des informations de zone de variation de caractéristique optique, qui sont des informations tridimensionnelles concernant une position avec une variation d'absorption de lumière à l'intérieur de l'objet, à l'aide des informations de variation d'intensité lumineuse pour chaque ensemble de sondes ; et
 25 une unité de sortie (25) qui est conçue pour sortir les informations de zone de variation de caractéristique optique acquises par l'unité d'estimation (24) ;

l'unité d'estimation (24), dans laquelle sont stockées des informations de sensibilité, qui sont des informations indiquant une relation entre une variation de caractéristique optique et une variation d'intensité lumineuse, étant conçue pour effectuer une correction suivant une atténuation de sensibilité selon une profondeur, à l'aide des
 30 informations de sensibilité, et pour introduire une dispersion afin d'améliorer une résolution spatiale, acquérant ainsi les informations de zone de variation de caractéristique optique.

2. Appareil d'observation d'objet (2) selon la revendication 1, dans lequel l'unité d'estimation (24) comprend :

- 35 une partie de stockage d'informations de sensibilité (241) conçue pour stocker des informations de sensibilité, qui sont des informations indiquant une relation entre une variation de caractéristique optique et une variation d'intensité lumineuse ;
 une partie de correction (243) qui est conçue pour effectuer une correction suivant une atténuation de sensibilité selon une profondeur, à l'aide des informations de sensibilité ; et
 40 une partie d'application de dispersion (244) qui est conçue pour introduire une dispersion afin d'améliorer la résolution spatiale, acquérant ainsi les informations de zone de variation de caractéristique optique.

3. Appareil d'observation d'objet (2) selon la revendication 2,

- dans lequel l'unité d'estimation (24) comprend également une partie de stockage d'expressions arithmétiques (242)
 45 dans laquelle peut être stockée une première expression arithmétique, qui est une expression arithmétique utilisée pour acquérir les informations de zone de variation de caractéristique optique, qui est une expression arithmétique pour calculer une solution d'un problème inverse, et qui est une fonction de coût pour effectuer une correction suivant les informations de sensibilité,
 la partie de correction (243) est conçue pour substituer les informations de sensibilité à la première expression arithmétique, acquérant ainsi des premières informations de zone de variation de caractéristique optique,
 50 la partie d'application de dispersion (244) est conçue pour acquérir des informations de zone de variation de caractéristique finale à l'aide de la dispersion, pour améliorer la résolution spatiale, à l'aide des premières informations de zone de variation de caractéristique optique, et
 l'unité de sortie (25) est conçue pour sortir les informations de zone de variation de caractéristique optique acquises
 55 par la partie d'application de dispersion (244).

4. Appareil d'observation d'objet (2) selon la revendication 3,

dans lequel dans la partie de stockage d'expressions arithmétiques (242) est également stockée une deuxième

expression arithmétique pour effectuer une estimation bayésienne hiérarchique sur une valeur initiale, et la partie d'application de dispersion (244) est conçue pour substituer les premières informations de zone de variation de caractéristique optique comme valeur initiale à la deuxième expression arithmétique, et pour exécuter la deuxième expression arithmétique afin d'effectuer une estimation bayésienne hiérarchique, acquérant ainsi des informations de zone de variation de caractéristique finale.

5 5. Appareil d'observation d'objet (2) selon la revendication 1, à utiliser dans l'observation d'une fonction cérébrale d'un corps vivant,
dans lequel l'objet qui doit être observé est le cerveau du corps vivant, et
10 les informations d'intensité lumineuse de référence sont des informations concernant une intensité lumineuse au niveau de chaque sonde de réception de lumière au repos.

15 6. Appareil d'observation d'objet (2) selon la revendication 1, à utiliser dans le dépistage du cancer du sein, dans lequel l'objet qui doit être observé est un sein, et
les informations d'intensité lumineuse de référence sont des informations concernant une intensité lumineuse au niveau de chaque sonde de réception de lumière à partir d'un sein avec des cellules normales.

20 7. Appareil d'observation d'objet (2) selon l'une quelconque des revendications 1 à 6, dans lequel chaque intervalle entre les sondes de transmission de lumière et de réception de lumière (11, 12) n'est pas supérieur à 20 mm.

25 8. Procédé d'observation d'objet utilisant un support de stockage dans lequel sont stockées des informations d'intensité lumineuse de référence, qui sont des informations concernant une intensité lumineuse au niveau de chaque sonde de réception de lumière (12), et qui sont des informations utilisées comme référence, et réalisé avec une unité d'acquisition d'informations d'intensité lumineuse (22), une unité d'acquisition d'informations de variation d'intensité lumineuse (23), une unité d'estimation (24) et une unité de sortie (25), le procédé d'observation d'objet comprenant :

30 une étape d'acquisition d'informations d'intensité lumineuse de l'unité d'acquisition d'informations d'intensité lumineuse (22), à l'aide d'un appareil de mesure de proche infrarouge (1) comportant au moins un ensemble de sondes constitué par une paire composée d'une sonde de transmission de lumière (11) pour transmettre la lumière à un objet à observer, et d'une sonde de réception de lumière (12) pour recevoir la lumière, qui acquiert des informations d'intensité lumineuse, qui sont des informations concernant une intensité lumineuse de la lumière reçue par chaque sonde de réception de lumière (12), dans un cas où la lumière avec une certaine intensité lumineuse est transmise, à partir de chaque sonde de transmission de lumière (11) formant chaque ensemble de sondes, à l'objet ;

35 une étape d'acquisition d'informations de variation d'intensité lumineuse de l'unité d'acquisition d'informations de variation d'intensité lumineuse (23), qui acquiert pour chaque ensemble de sondes des informations de variation d'intensité lumineuse, qui sont des informations concernant une variation d'intensité lumineuse, à partir des informations d'intensité lumineuse de référence contenues dans le support de stockage, et des informations d'intensité lumineuse acquises lors de l'étape d'acquisition d'informations d'intensité lumineuse (22) ;

40 une étape d'estimation de l'unité d'estimation (24), qui acquiert des informations de zone de variation de caractéristique optique, qui sont des informations tridimensionnelles concernant une position avec une variation d'absorption de lumière à l'intérieur de l'objet, à l'aide des informations de variation d'intensité lumineuse pour chaque ensemble de sondes ; et

45 une étape de sortie de l'unité de sortie (25), qui sort les informations de zone de variation de caractéristique optique acquises lors de l'étape d'estimation ;

50 une correction étant effectuée suivant une atténuation de sensibilité selon une profondeur, à l'aide des informations de sensibilité, qui sont des informations indiquant une relation entre une variation de caractéristique optique et une variation d'intensité lumineuse, et une dispersion étant introduite afin d'améliorer une résolution spatiale, de sorte que les informations de zone de variation de caractéristique optique sont acquises.

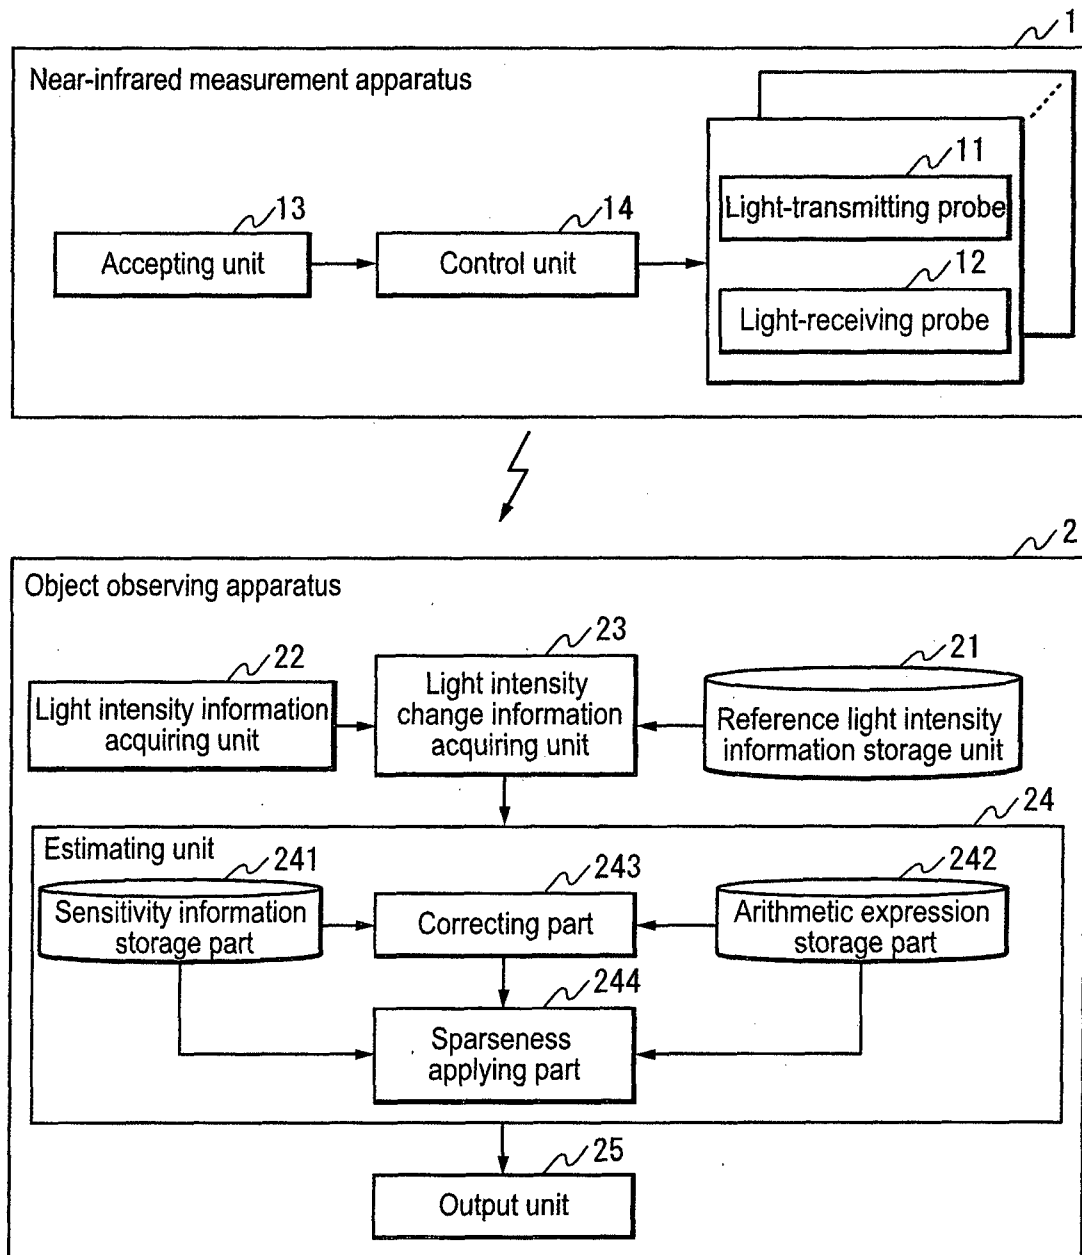
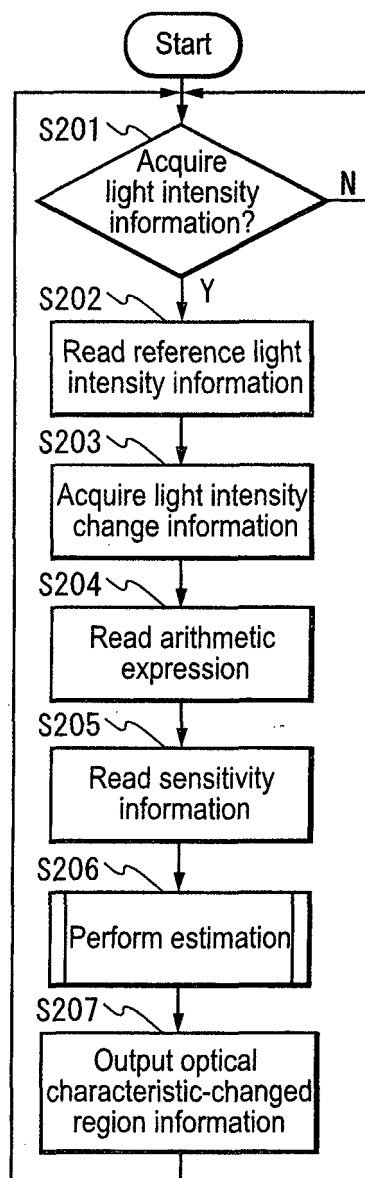


FIG.1

**FIG.2**

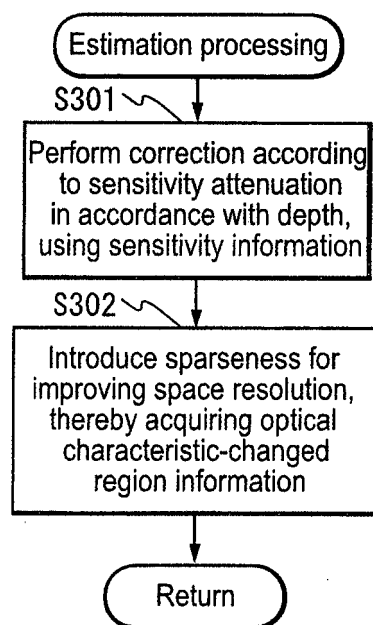


FIG.3

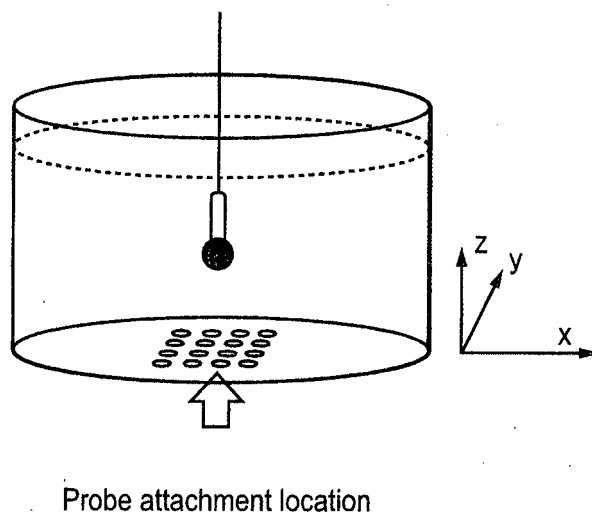


FIG.4

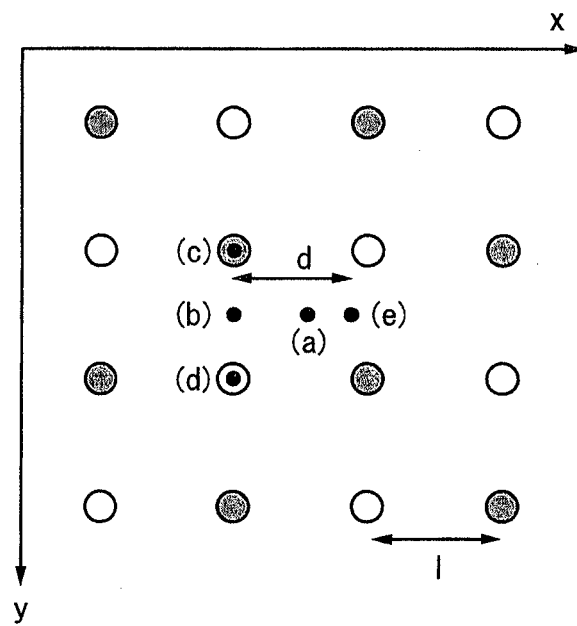


FIG.5

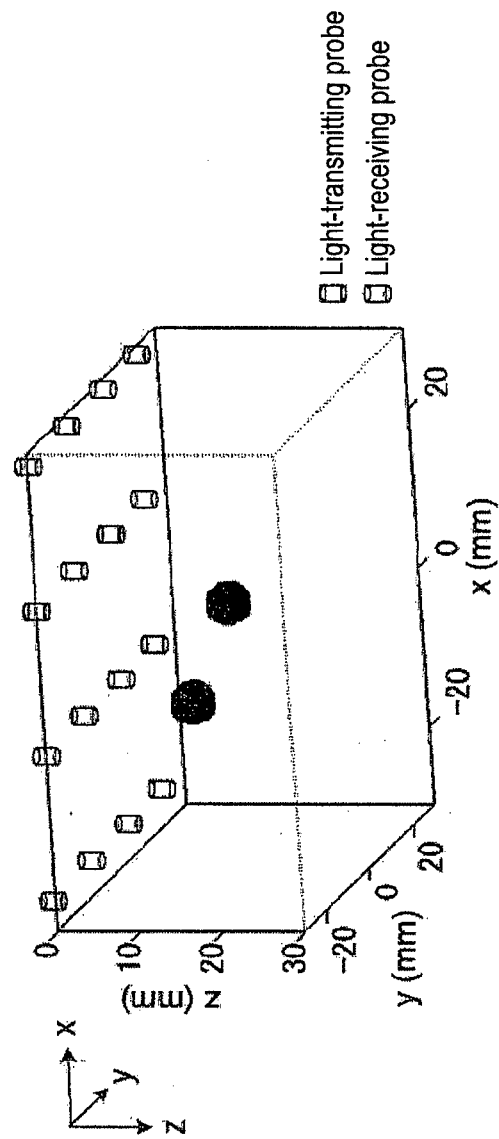


FIG.6

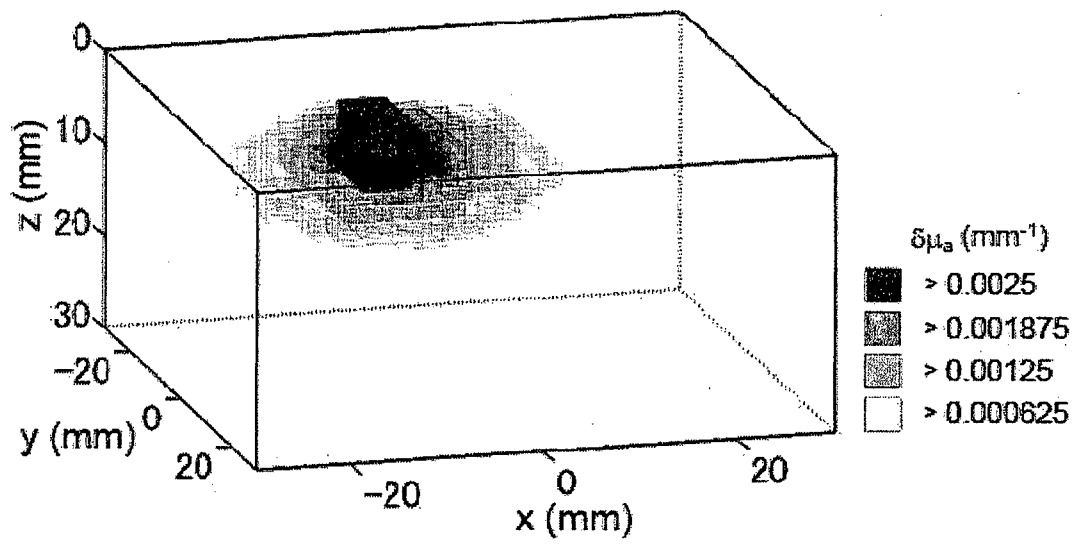


FIG.7

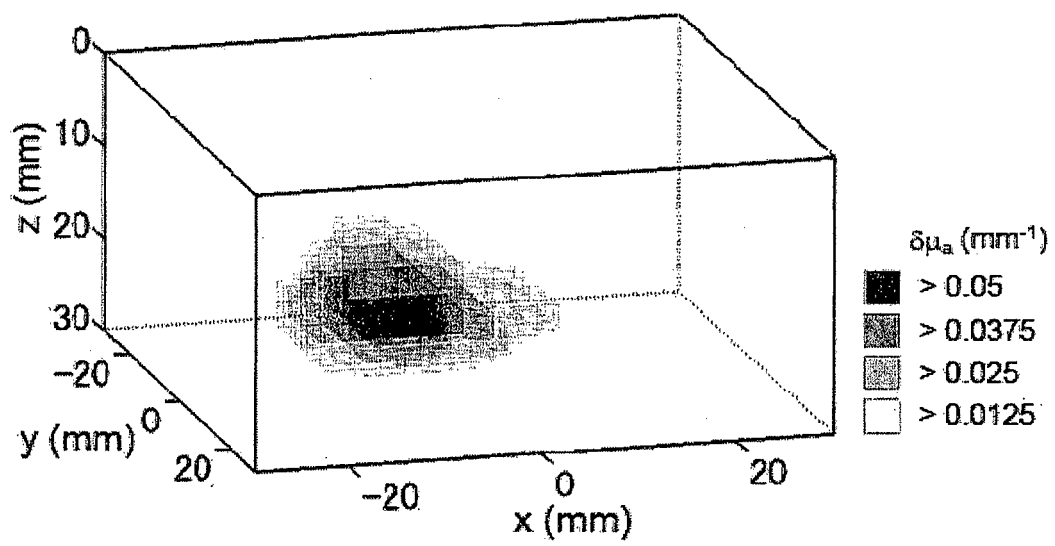


FIG.8

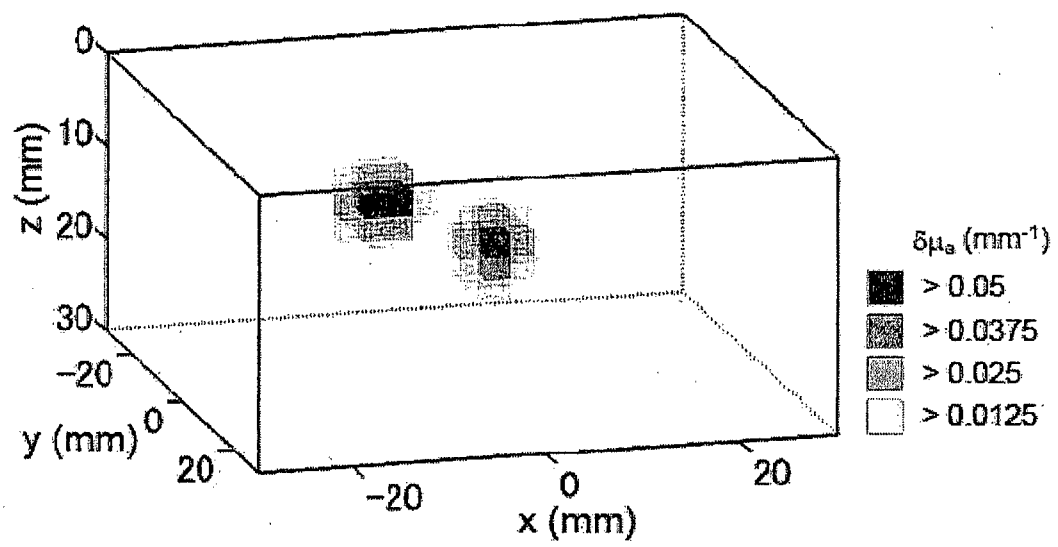
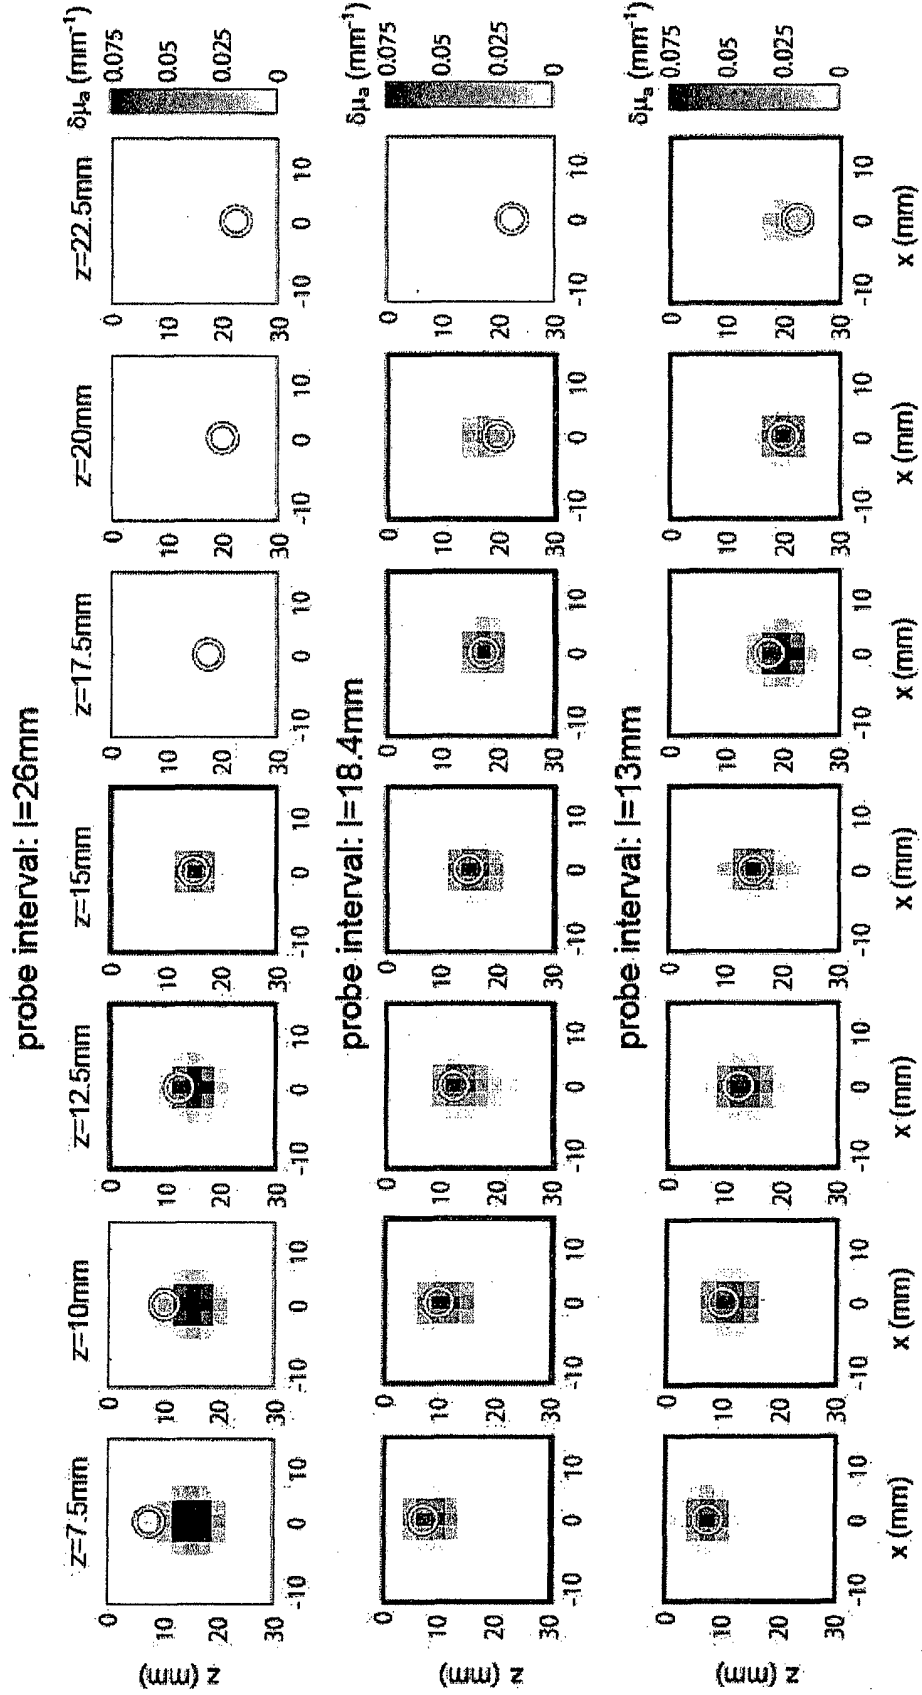


FIG.9

**FIG.10**

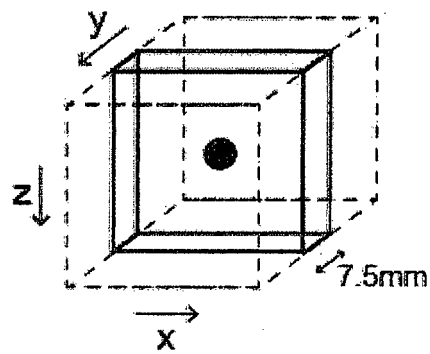


FIG.11

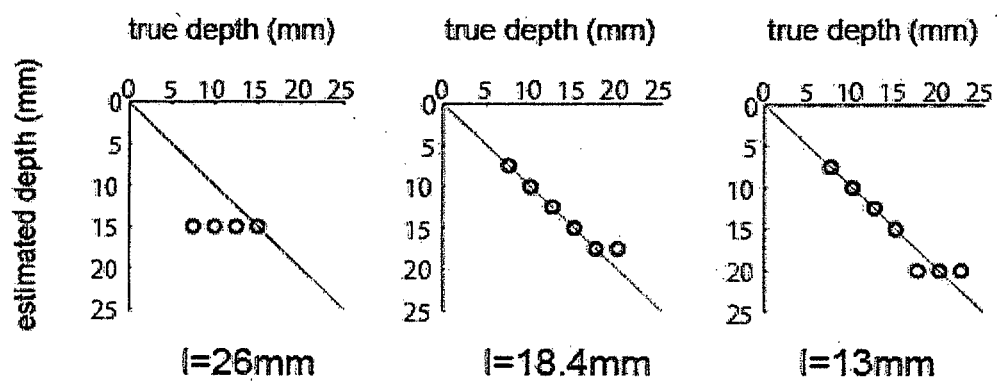
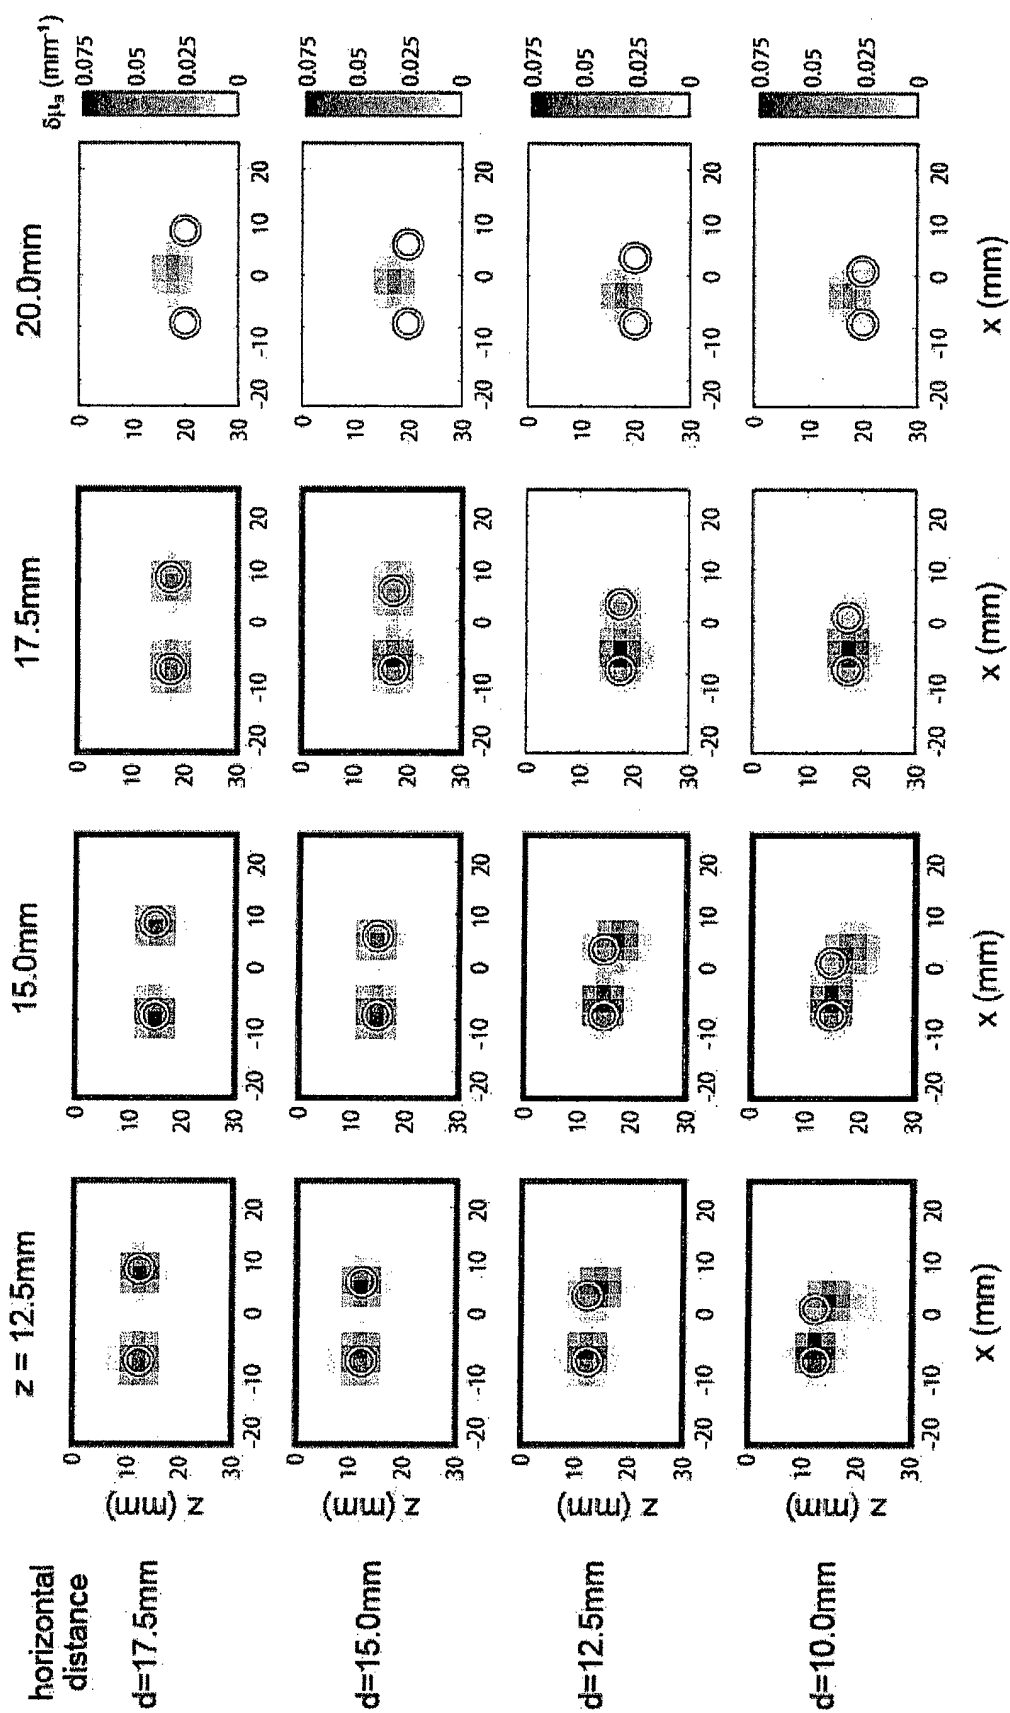


FIG.12

Probe interval	26mm	18. 4mm	13mm
Light absorbing member position	Estimation limit depth [mm]		
(a) Center	15. 0	20. 0	22. 5
(b) Middle point	17. 5	20. 0	22. 5
(c) Light-transmitting probe	17. 5	17. 5	20. 0
(d) Light-receiving probe	17. 5	17. 5	20. 0

FIG.13

**FIG.14**

Probe interval	18. 4mm	13mm
Horizontal distance [mm]	Estimation limit depth [mm]	
15. 0	17. 5	17. 5
12. 5	15. 0	17. 5
10. 0	15. 0	17. 5

FIG.15

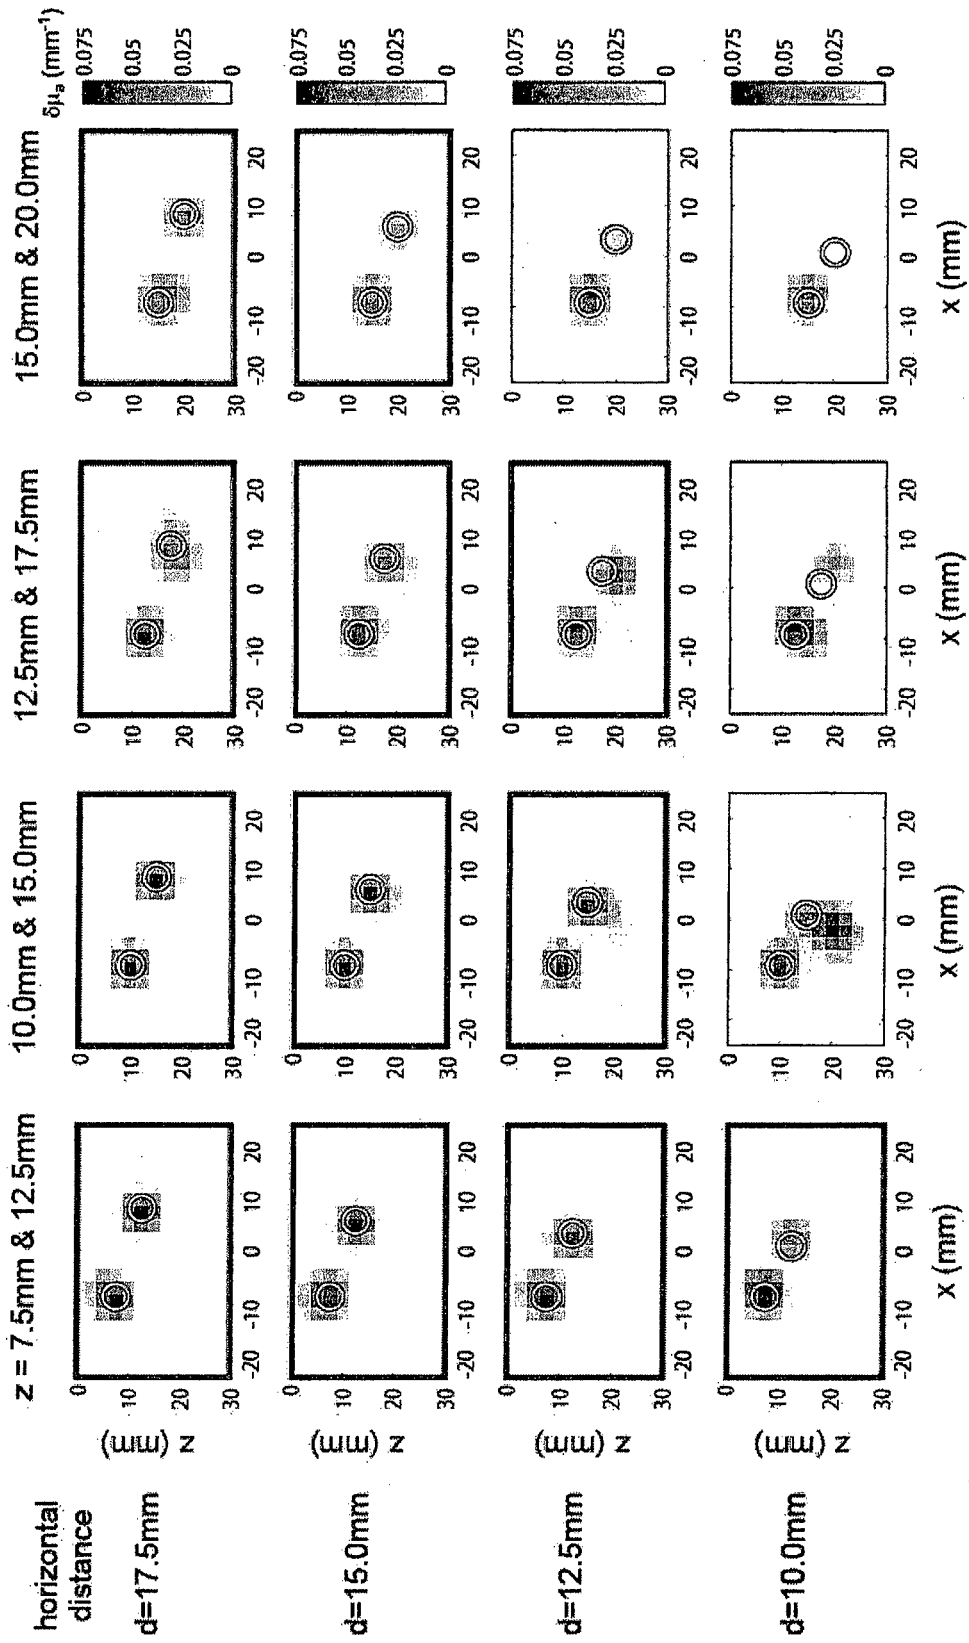


FIG.16

Probe interval	18. 4mm	13mm
Horizontal distance [mm]	Estimation limit depth [mm]	
15. 0	15. 0 & 20. 0	15. 0 & 20. 0
12. 5	12. 5 & 17. 5	12. 5 & 17. 5
10. 0	7. 5 & 12. 5	7. 5 & 12. 5

FIG.17

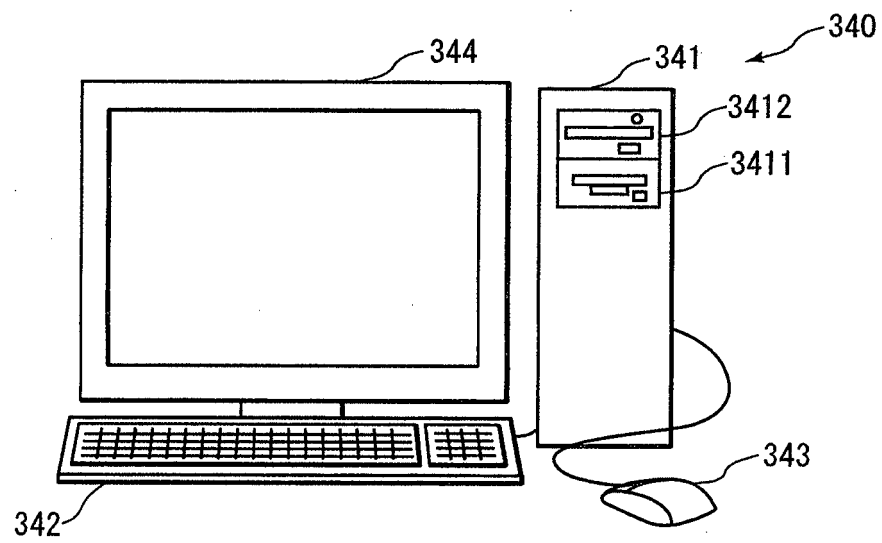


FIG.18

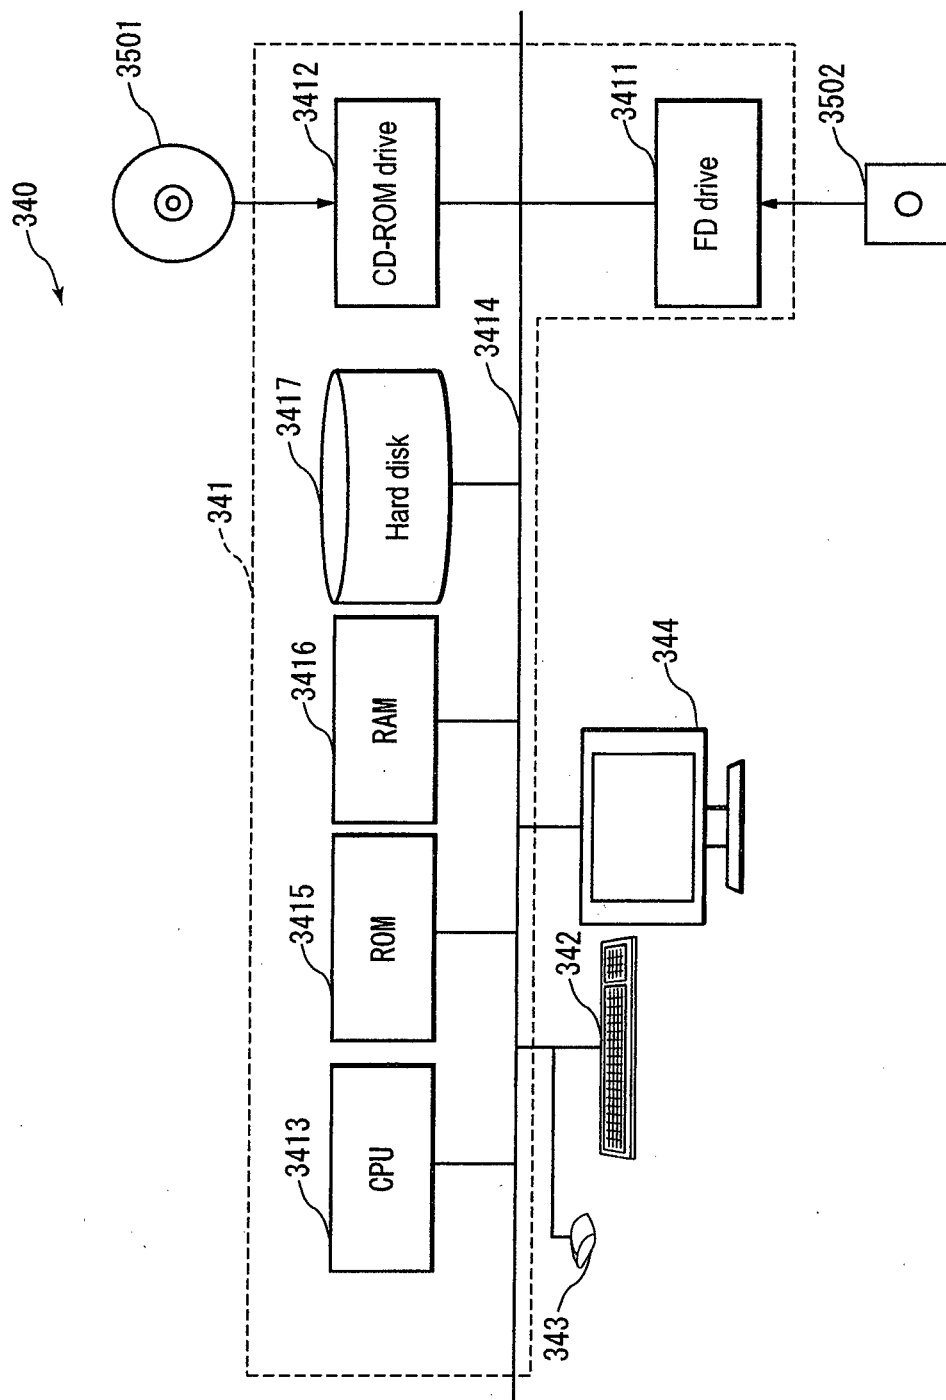


FIG.19

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 2008178546 A [0007]
- JP 2005328916 A [0007]
- US 20090244546 A1 [0007]
- EP 2067432 A2 [0007]

Non-patent literature cited in the description

- **Y. HOSHI ; M. TAMURA.** Detection of dynamic changes in cerebral oxygenation coupled to neuronal function during mental work in man. *Neurosci. Lett.*, 1993, vol. 150, 5-8 [0006]
- **DAISUKE YAMASHITA ; MOTOKI ODA ; HIROAKI SUZUKI ; TAKESHI YAMANAKA ; TOSHIHIKO SUZUKI ; YUKIO UEDA ; KAZUYOSHI OHTA ; MITSU HARU MIWA ; YUTAKA HASEGAWA ; HIROYUKI KYUSHIMA.** Development of Multi Channel Time Resolved Spectroscopy System and Application to Optical Mammography System. *J Jpn Coll Angiol*, 2007, vol. 47, 11-16 [0006]
- **A. MAKI ; Y. YAMASHITA ; Y. ITO ; E. WATANABE ; Y. MAYANAGI ; H. KOIZUMI.** Spatial and temporal analysis of human motor activity using noninvasive NIR topography. *Med. Phys.*, 1995, vol. 22, 1997-2005 [0006]
- **B. W. ZEFF ; B. R. WHITE ; H. DEGHANI ; B. L. SCHLAGGAR ; J. P. CULVER.** Retinotopic mapping of adult human visual cortex with high-density diffuse optical tomography. *Proc. Natl. Acad. Sci. U.S.A.*, 2007, vol. 104, 12169-12174 [0006]
- **C. HABERMEHL ; S. HOLTZE ; J. STEINBRINK ; S. P. KOCH ; H. OBRIG ; J. MEHNERT ; C. H. SCHMITZ.** Somatosensory activation of two fingers can be discriminated with ultrahigh-density diffuse optical tomography. *NeuroImage*, 2011, vol. 59, 3201-3211 [0006]
- **H. NIU ; F. TIAN ; Z.-J. LIN ; H. LIU.** Development of a compensation algorithm for accurate depth localization in diffuse optical tomography. *Optics Letter*, vol. 35 (3), 429-431 [0006]
- **MIYAMOTO, ATSUSHI et al.** Hierarchical Bayes method for NIRS—DOT inverse problem and its phase diagrams. *IEICE Technical Report. NC, Neurocomputing*, 20 July 2010, vol. 110 (149), 51-56 [0006]
- **Q. FANG ; D. A. BOAS.** Monte Carlo simulation of photon migration in 3D turbid media accelerated by graphics processing units. *Opt. Express*, 2009, vol. 17, 20178-20190 [0050]
- **R. C. HASKELL ; L. O. SVAASAND ; T. T. TSAY ; T. C. FENG ; M. S. MCADAMS ; B. J. TROMBERG.** Boundary conditions for the diffusion equation in radiative transfer. *J. Opt. Soc. Am. A*, 1994, vol. 11, 2727-2741 [0050]
- Likelihood and the Bayes procedure. **H. AKAIKE et al.** *Bayesian Statistics*. Univ. Press, 1980, 143-166 [0053]
- **A. C. FAUL ; M. E. TIPPING.** Analysis of sparse Bayesian learning. *Adv. Neural Inf. Process. Syst.*, 2002, vol. 14, 383-389 [0063]

专利名称(译)	物体观测装置和物体观测方法		
公开(公告)号	EP2839785B1	公开(公告)日	2016-11-30
申请号	EP2013775158	申请日	2013-04-04
申请(专利权)人(译)	高级电信研究院国际		
当前申请(专利权)人(译)	高级电信研究院国际		
[标]发明人	SHIMOKAWA TAKEAKI KOSAKA TAKASHI YAMASHITA OKITO SATO MASAACKI		
发明人	SHIMOKAWA, TAKEAKI KOSAKA, TAKASHI YAMASHITA, OKITO SATO, MASAACKI		
IPC分类号	A61B5/00 A61B10/00 G01N21/47		
CPC分类号	G01N21/4785 A61B5/0042 A61B5/0073 A61B5/0091 A61B10/0041 G01N2201/121 G01N2201/12753		
优先权	2012088924 2012-04-10 JP		
其他公开文献	EP2839785A1 EP2839785A4		
外部链接	Espacenet		

摘要(译)

为了解决不能精确估计物体内部的局部光学特性改变区域的问题，物体观测设备包括：光强度信息获取单元，其获取在每种光接收探头接收的光强度信息的情况下具有一定光强度的光从近红外测量装置的每个透光探头传输到物体；光强度变化信息获取单元，对于每个探针组，从参考光强度信息和光强度信息获取关于光强度变化的光强度变化信息；估计单元，使用光强度变化信息，获取关于物体内部具有光吸收变化的位置的三维光学特性改变区域信息；输出单元，输出光学特性变化区域信息；其中，估计单元包括：校正部分，使用灵敏度信息，根据深度根据灵敏度衰减进行校正；以及引入稀疏性以提高空间分辨率的稀疏度应用部分，从而获取光学特性改变的区域信息。因此，可以准确地估计对象内部的局部光学特性改变区域作为三维信息。

$$\Phi_{\text{pert}}(r, s, d) = \int dr \frac{\Phi_0(r, s, d) \Phi_0(r, r)}{\Phi_0(r, s, d)} \delta \mu_a(r). \quad (1)$$