



(19) **United States**

(12) **Patent Application Publication**
Brodnick et al.

(10) **Pub. No.: US 2005/0131282 A1**

(43) **Pub. Date: Jun. 16, 2005**

(54) **APPARATUS AND METHOD FOR ACQUIRING OXIMETRY AND ELECTROCARDIOGRAM SIGNALS**

Publication Classification

(51) **Int. Cl.⁷** A61B 5/00; A61B 5/04

(52) **U.S. Cl.** 600/323; 600/324; 600/509

(76) **Inventors:** Donald E. Brodnick, Cedarburg, WI (US); Paul S. Schluter, Whitefish Bay, WI (US); James M. Gray, Fox Point, WI (US); George M. Hutchinson, Milwaukee, WI (US)


(57) **ABSTRACT**

A method and apparatus for acquiring pulse oximetry and electrocardiogram signals from an appendage of a patient. The apparatus can include a substrate that can be attached to the appendage of the patient, an emitter coupled to the substrate, a detector coupled to the substrate, and an electrode coupled to the substrate. The apparatus can generate a blood oxygen saturation output signal based on radiation received by the detector. The apparatus can also generate a reference or non-reference electrocardiogram signal. The apparatus can include a neural-muscular transmission device.

Correspondence Address:
JOSEPH D. KUBORN
ANDRUS, SCEALES, STARKE & SAWALL
100 EAST WISCONSIN AVENUE
SUITE 1100
MILWAUKEE, WI 53202 (US)

(21) **Appl. No.:** 10/732,985

(22) **Filed:** Dec. 11, 2003

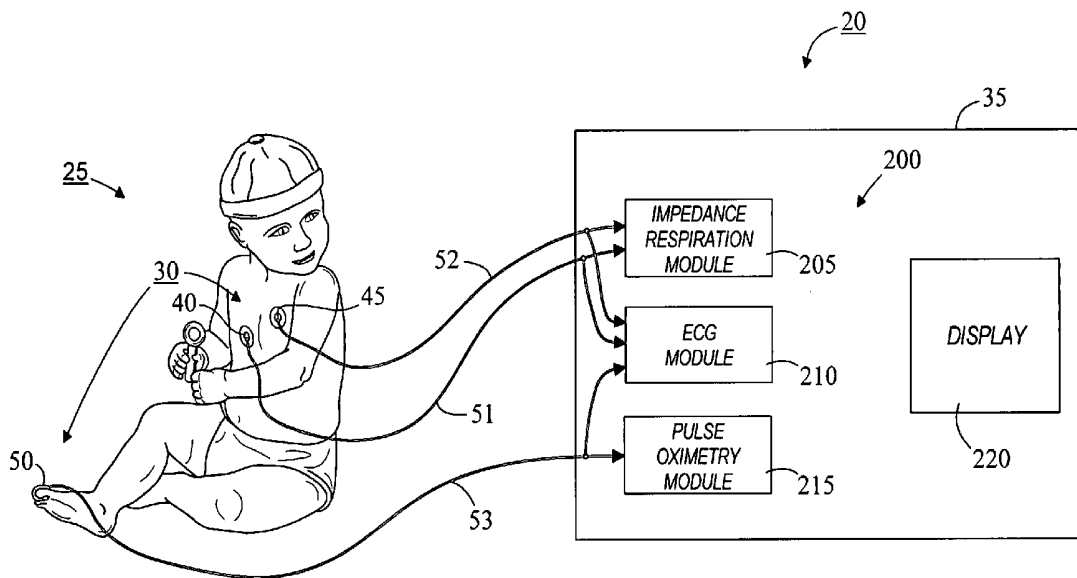

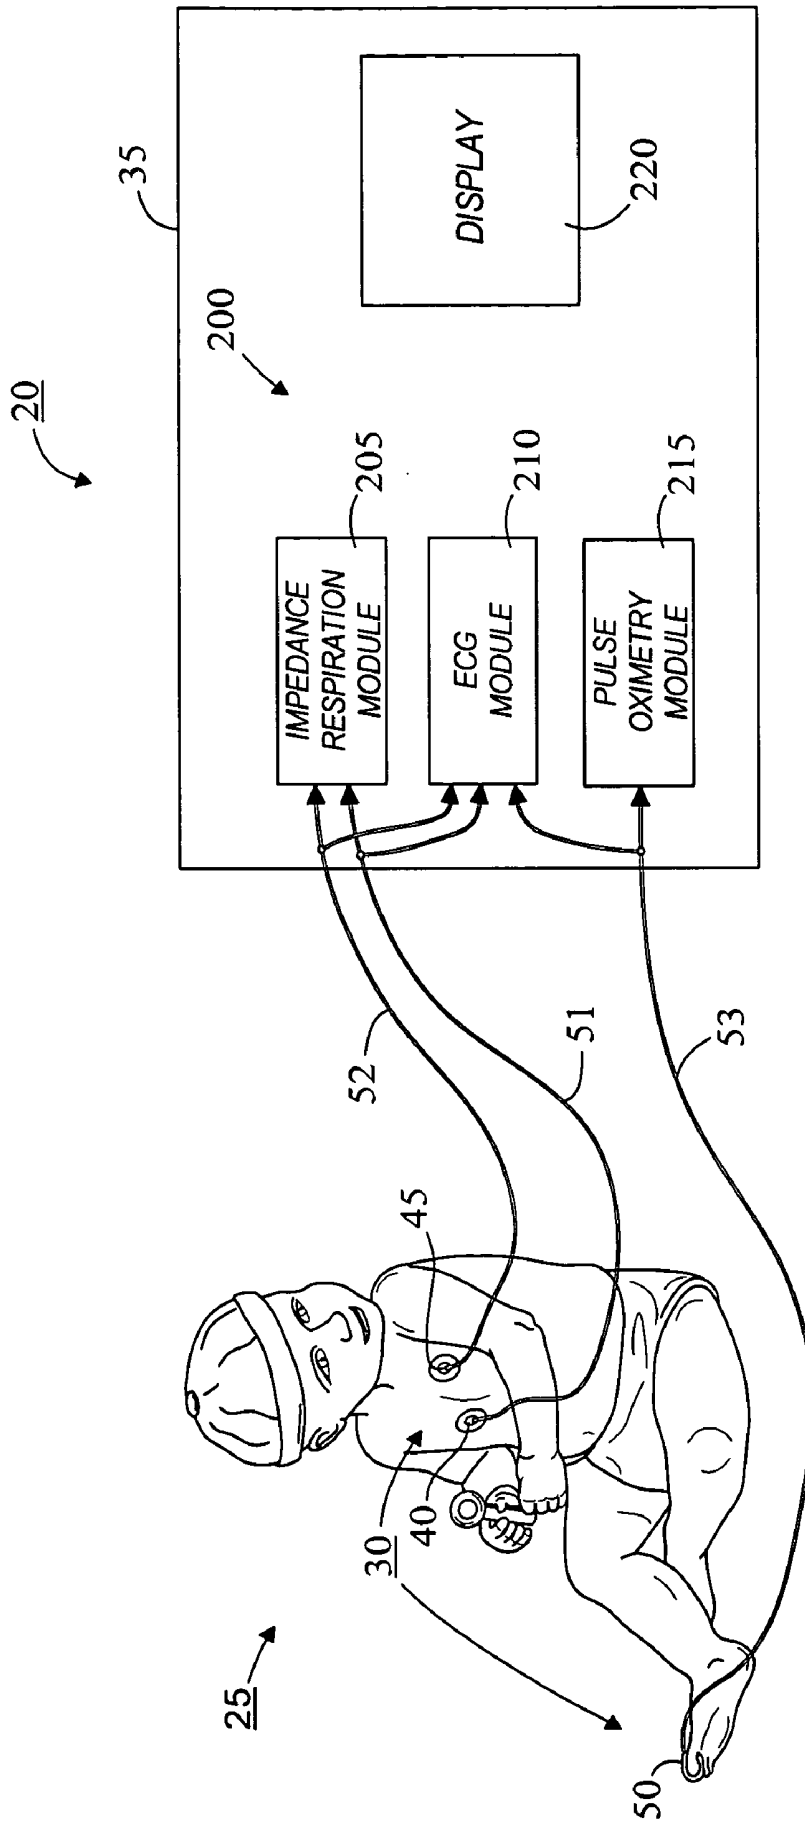


FIG. 1

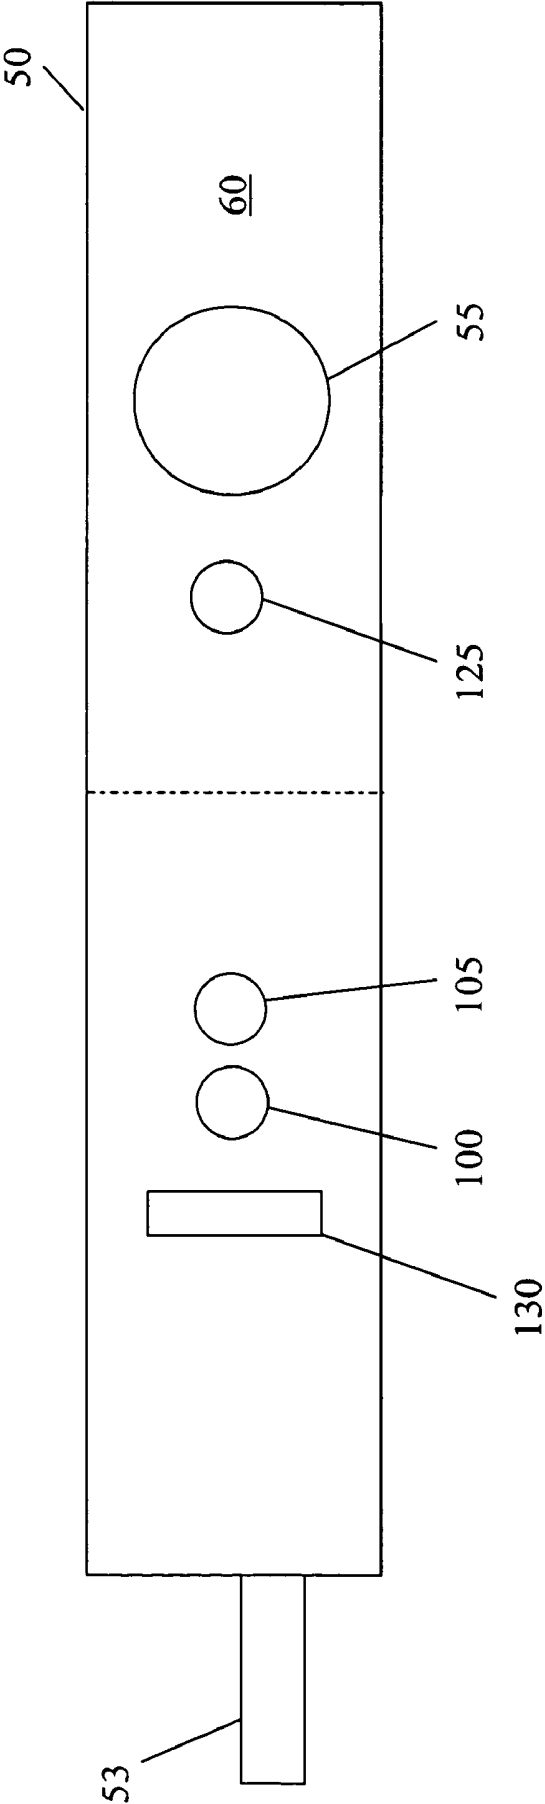


FIG. 2

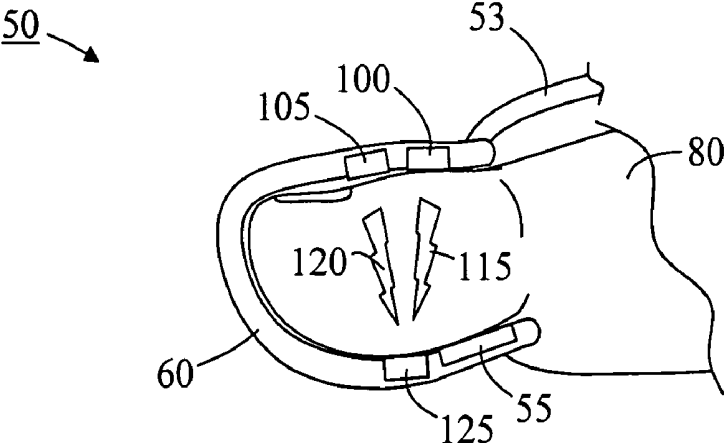


FIG. 3

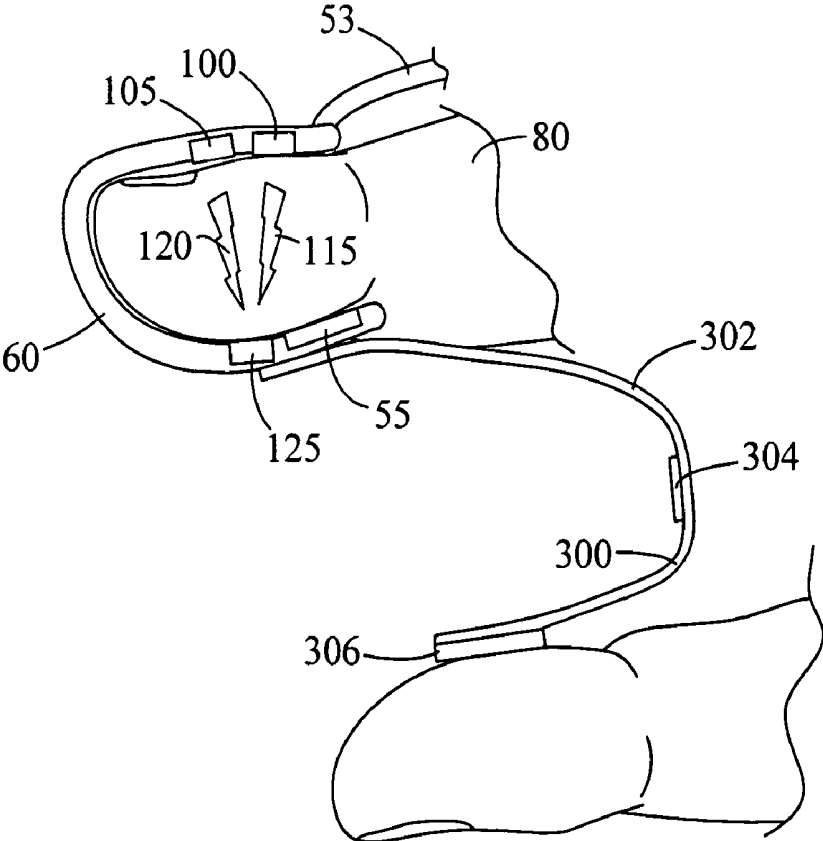


FIG. 6

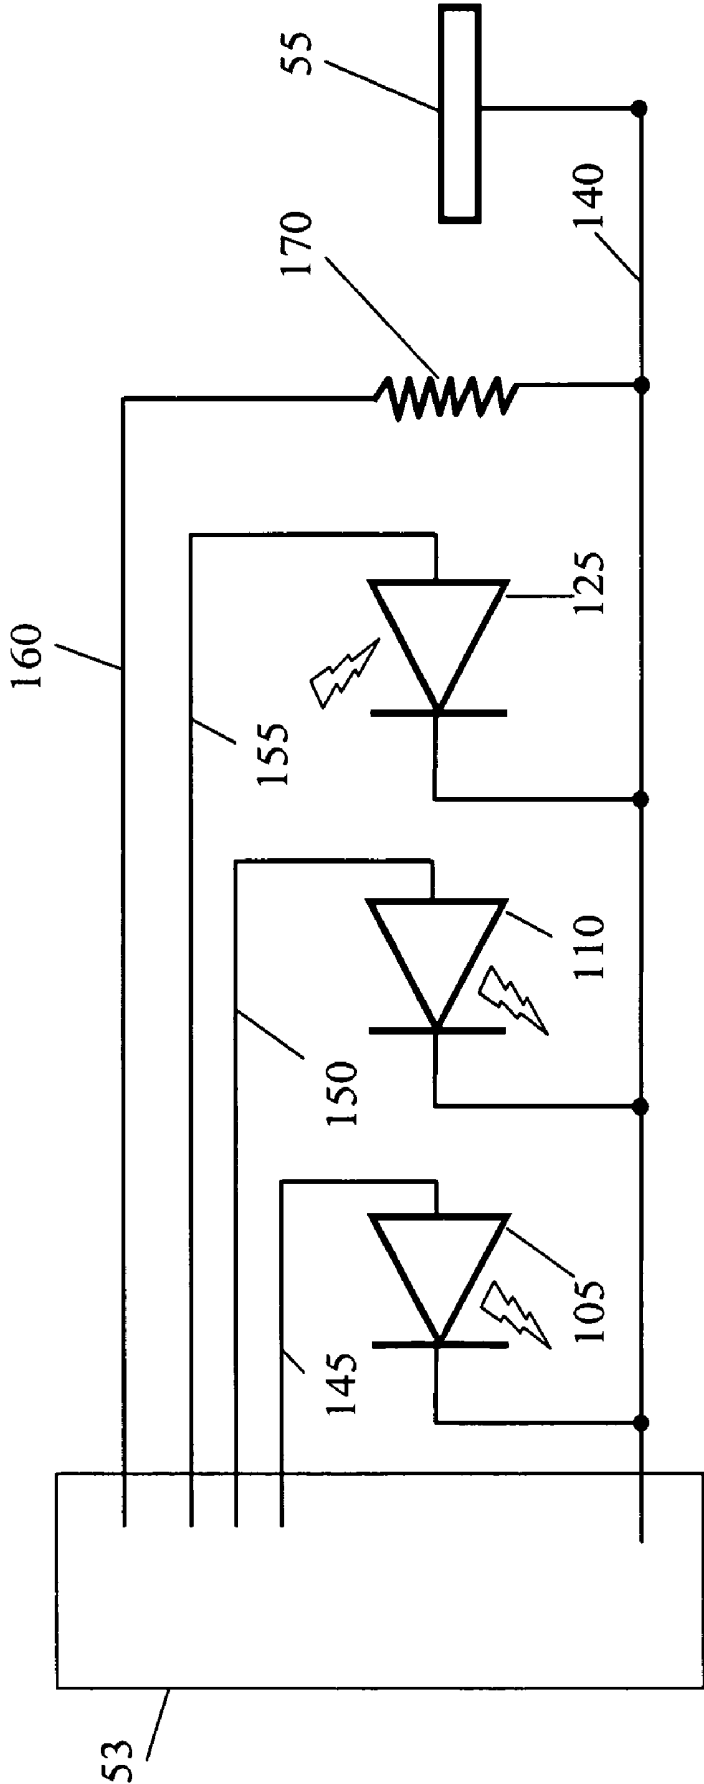


FIG. 4

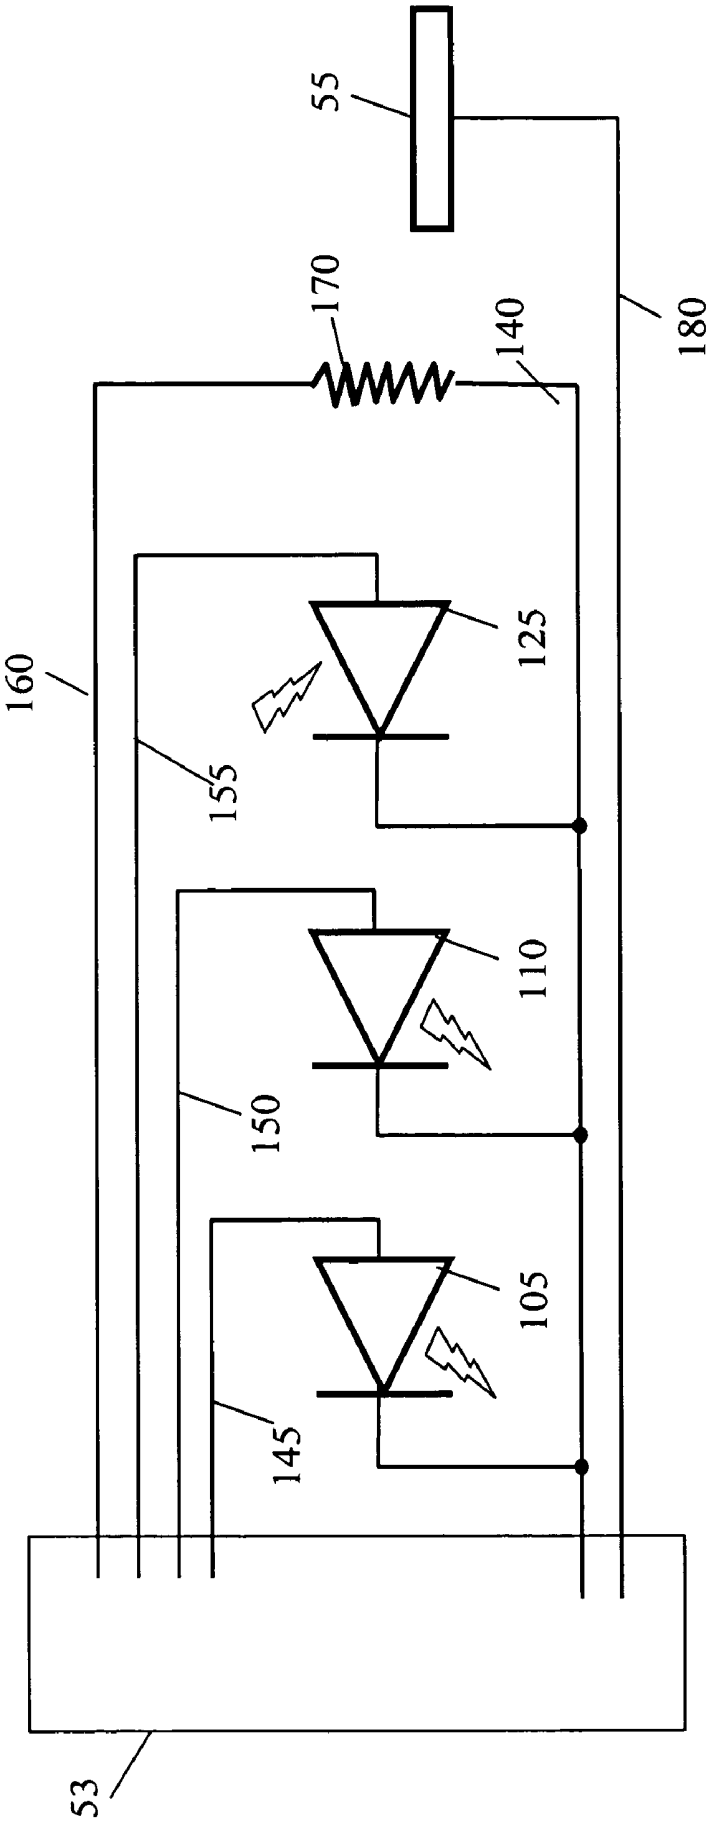


FIG. 5

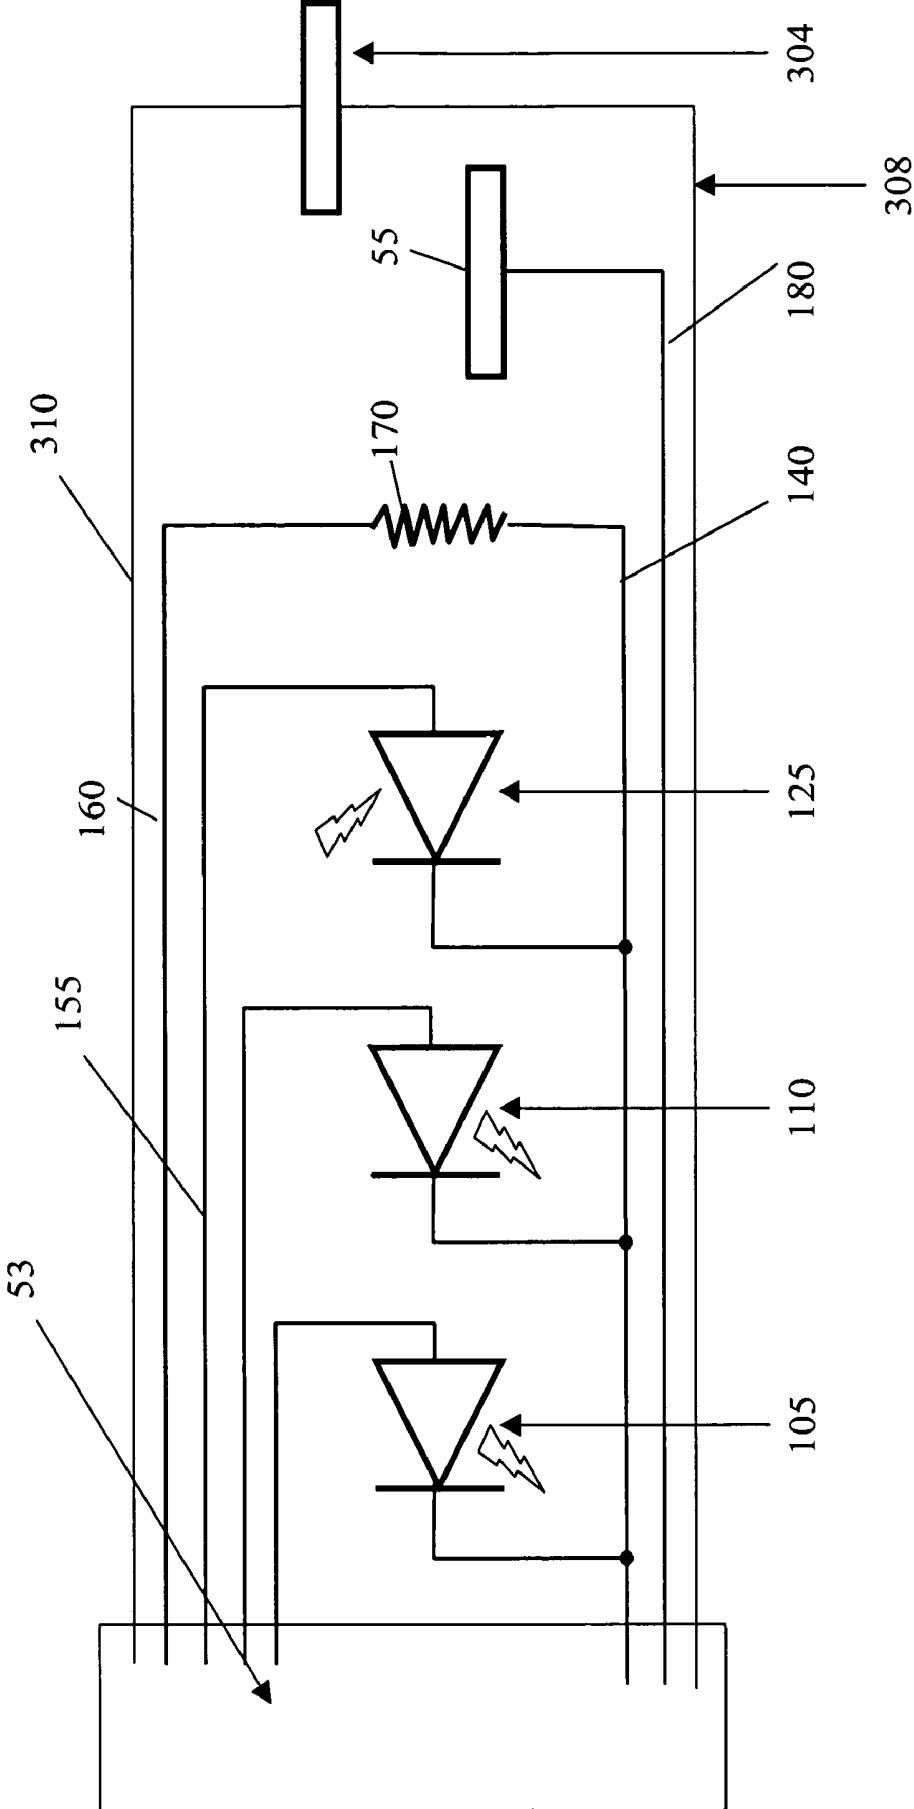


FIG. 7

APPARATUS AND METHOD FOR ACQUIRING OXIMETRY AND ELECTROCARDIOGRAM SIGNALS

BACKGROUND OF THE INVENTION

[0001] The present invention relates to patient monitoring, and more specifically to acquiring oximetry and electrocardiogram signals.

[0002] Conventional oximeter sensors are generally only capable of providing blood oxygen saturation data. However, oximeter sensors are often used at the same time that an electrocardiogram is being acquired. Electrocardiogram instruments require many design considerations, as described in more detail below. Conventionally, these design considerations are addressed with electrodes and an ECG instrument that are independent of the oximeter sensor.

[0003] As used herein, the term "ECG" refers to a standard ten-electrode, twelve-lead electrocardiogram or any non-standard electrocardiogram, as are known to one of ordinary skill in the art. The term "ECG signal" or "ECG output signal" refers to one or more leads or channels of data. The term "channel of ECG data" refers to a single lead or a single channel. The term "ECG instrument" refers to any acquisition, analysis, signal generation, and/or monitoring equipment that receives ECG signals from electrodes.

[0004] An ECG instrument measures voltage potentials between electrodes or combinations of electrodes attached to a patient. In a minimum configuration, one channel of ECG data is measured between two electrodes. To obtain more channels, additional electrodes are needed. Typically, the voltage between the electrodes (i.e., the differential voltage) is relatively low in amplitude (e.g., approximately one mV). Accordingly, high amplification is needed by the ECG instrument to raise the differential voltage. The body of the patient often has a common mode voltage that is very high in comparison to the differential voltage. It is understood by those of ordinary skill in the art that a high common mode rejection ratio ("CMRR") and a high input impedance are required for an ECG instrument to amplify a low differential voltage in the presence of large common mode voltages in order to acquire an ECG signal of adequate diagnostic quality [i.e., adequate voltage resolution, signal-to-noise ratio ("SNR"), and frequency bandwidth].

[0005] For applications in which an ECG signal of reduced quality is adequate (e.g., less than about eight bit resolution for a heart rate monitor in an exercise bicycle, a defibrillator, or an event recorder), the lower frequencies (e.g., less than approximately 0.6 Hz) and the higher frequencies (e.g., greater than approximately 40 Hz) can be filtered from the ECG signal. For these applications, the heart rate monitor may use only two electrodes and a relatively low-cost amplifier.

[0006] To avoid the high cost and difficult design of a high CMRR amplifier, an ECG instrument can include a third electrode with a low impedance path between the patient and the ECG instrument. The third electrode is generally referred to as the right leg ("RL") electrode, the common electrode, or the reference electrode. The reference electrode does not serve as a positive input or a negative input to the ECG amplifier(s). Only one reference electrode is necessary, even if many other electrodes are used to acquire several other

channels of ECG data. The reference electrode can be positioned on the patient's body in any suitable manner known in the art.

[0007] When monitoring infants, especially neonates, the application of many adhesive electrodes to the skin is particularly undesirable. The body surface of an infant is often so small that electrodes can cover relatively large areas of the infant's body. The skin of a neonate is extremely fragile and removing electrodes can easily tear the skin increasing infection risk and pain to the infant. Each electrode also requires a leadwire to connect the electrode to the ECG instrument. Additional electrodes and leadwires decrease the caregiver's ability to access the infant. Additional electrodes also add cost in materials and labor, and increase the time it takes to prepare an infant for monitoring.

[0008] Conventional patient monitors often acquire ECG signals, an impedance respiration signal, and a pulse oximeter signal from a patient. The combination of these three monitoring parameters is generally referred to as a cardio-respirogram ("CRG") signal or a pneumogram signal. The CRG signal is of special value in the care of a neonate. To acquire CRG signals, the patient monitor is generally connected to three electrodes for acquiring one channel of ECG data and an impedance respiration signal. A separate transducer, the pulse oximeter sensor, is often attached to an ear lobe, a finger, a toe or another body surface. The pulse oximeter sensor generally illuminates the skin with two colors of light (e.g., red and infra-red) and measures the reflected or transmitted light to determine the level of oxygen saturation of the blood.

BRIEF DESCRIPTION OF THE INVENTION

[0009] It is desired by caregivers to attach as few electrodes as possible to patients, especially infants. In one embodiment, the invention provides a method of acquiring pulse oximetry and ECG signals from a patient, including attaching a single transducer to a patient, acquiring a pulse oximetry signal with the single transducer, and acquiring a reference or non-reference ECG signal with the single transducer.

[0010] In some embodiments, the invention provides a device for acquiring pulse oximetry and ECG signals from an appendage of a patient. The device can include a substrate that can be attached to the appendage of the patient, at least one emitter coupled to the substrate, at least one detector coupled to the substrate, and an electrode coupled to the substrate. The emitter can be positioned to emit radiation through the appendage, and the electrode can generate a reference or non-reference ECG signal. The detector can be positioned to receive the radiation emitted through the appendage, and can generate a pulse oximetry signal based on the received radiation.

BRIEF DESCRIPTION OF THE DRAWINGS

[0011] FIG. 1 is a schematic illustration of a monitoring system embodying the invention.

[0012] FIG. 2 is a schematic illustration of a transducer for use in the monitoring system of FIG. 1.

[0013] FIG. 3 is a schematic illustration of the transducer of FIG. 2 attached to a patient's appendage.

[0014] FIG. 4 is an electrical schematic diagram of one embodiment of the transducer of FIG. 2.

[0015] FIG. 5 is an electrical schematic diagram of another embodiment of the transducer of FIG. 2.

[0016] FIG. 6 is a schematic illustration of a transducer attached to a patient's appendage according to another embodiment of the invention.

[0017] FIG. 7 is an electrical schematic diagram of one embodiment of the transducer of FIG. 6.

DETAILED DESCRIPTION OF THE INVENTION

[0018] Before any embodiments of the invention are explained in detail, it is to be understood that the invention is not limited in its application to the details of construction and the arrangement of components set forth in the following description or illustrated in the following drawings. The invention is capable of other embodiments and of being practiced or of being carried out in various ways. Also, it is to be understood that the phraseology and terminology used herein is for the purpose of description and should not be regarded as limited. The use of "including," "comprising" or "having" and variations thereof herein is meant to encompass the items listed thereafter and equivalents thereof as well as additional items. The terms "mounted," "connected" and "coupled" are used broadly and encompass both direct and indirect mounting, connecting and coupling. Further, "connected" and "coupled" are not restricted to physical or mechanical connections or couplings and can include electrical connections and couplings, whether direct or indirect.

[0019] In addition, it should be understood that embodiments of the invention include both hardware and electronic components or modules that, for purposes of discussion, may be illustrated and described as if the majority of the components were implemented solely in hardware. However, one of ordinary skill in the art, and based on a reading of this detailed description, would recognize that, in at least one embodiment, the electronic based aspects of the invention may be implemented in software. As such, it should be noted that a plurality of hardware and software based devices, as well as a plurality of different structural components may be utilized to implement the invention. Furthermore, and as described in subsequent paragraphs, the specific mechanical configurations illustrated in the drawings are intended to exemplify embodiments of the invention and that other alternative mechanical configurations are possible.

[0020] FIG. 1 illustrates a monitoring system 20 for monitoring a patient 25, such as an infant or neonate or any other patient, according to one embodiment of the invention. The monitoring system 20 can include several electrodes 30 for acquiring signals from the patient 25 and a monitoring instrument 35 for processing, analyzing, and/or displaying the signals acquired from the patient 25. In one embodiment, the monitoring system 20 can analyze, process, and/or display more than one signal from the patient 25, such as, for example, a single-channel of ECG data, multiple channels of ECG data, an impedance respiration signal, an oximeter signal, a pulse oximeter signal, a CRG signal, or any other suitable patient signal. In other embodiments, the monitoring system 20 can analyze, process, and/or display only one

signal from the patient 25, such as, for example, a CRG signal. In further embodiments, the monitoring system 20 can analyze, process, and/or display one or more signals from multiple patients (e.g., for monitoring more than one patient at a remote workstation or for monitoring a mother and a fetus).

[0021] The electrodes 30 are coupled to the patient 25 to acquire one or more signals. In one embodiment, the electrodes 30 can acquire at least two signals indicative of at least two patient parameters. For example, the electrodes 30 can acquire one or more channels of ECG data, an impedance respiration signal, a signal indicative of a level of oxygen saturation in the patient's blood, etc. In one embodiment, such as the embodiment illustrated in FIG. 1, the electrodes 30 can acquire a single channel of ECG data from the patient 25.

[0022] As shown in FIG. 1, the electrodes 30 include a first electrode 40, a second electrode 45, and a third electrode or transducer 50. The first electrode 40 can be attached to the upper-left portion of the patient's chest. The second electrode 45 can be attached to the upper-right portion of the patient's chest. The transducer 50 can be attached to an appendage of the patient 25 (such as, for example, an ear lobe, a finger, a toe, etc.). In other embodiments, the first electrode 40, the second electrode 45, and the transducer 50 can be arranged and attached to other suitable portions of the patient 25 as is known in the art. In one embodiment, one or more of the electrodes 30 (such as, for example, the first electrode 40 and the second electrode 45), can each include a conventional adhesive pad to attach to the skin of the patient 25.

[0023] As shown in FIG. 1, the first electrode 40 can be coupled to the monitoring instrument 35 via a first cable or leadwire 51, and the second electrode 45 can be coupled to the monitoring instrument 35 via a second cable or leadwire 52. Also, the transducer 50 can be coupled to the monitoring instrument 35 via a third cable or leadwire 53. In one embodiment, the first cable 51 and the second cable 52 can be single-wire cables, and the third cable 53 can be a multi-wire cable.

[0024] As shown in FIGS. 2 and 3, the transducer 50 can be a pulse oximeter transducer including an electrode 55 that functions as a reference or non-reference electrode for one or more ECG signals. In simplified instruments that forego the use of a reference electrode, the electrode 55 can act as any suitable terminal of an ECG lead. For example, the electrode 55 can act as a standard right arm electrode when attached to a finger on the patient's right hand. When attached to a toe of the left foot, the electrode 55 can act as a standard left leg or left foot electrode. When attached to a finger of the left hand, the electrode 55 can act as a standard left arm electrode. When attached to a forehead or ear lobe, the electrode 55 can act as a reference or non-reference electrode for the Frank lead system. The Frank lead system is an alternative set of eight electrode sites used to record three channels of XYZ ECG data (i.e., a vectorcardiogram). Thus, the transducer 50 can be used to acquire a signal indicative of a level of oxygen saturation in the patient's blood and a reference or non-reference ECG signal.

[0025] As shown in FIG. 2, the transducer 50 can include a substrate 60 that can be attached to the patient 25 or positioned at least partially on the patient 25. In some

embodiments, the substrate **60** can be flexible and can include a suitable adhesive. In another embodiment, the substrate **60** can be substantially rigid, such as in a reusable clam-shell design. In one embodiment, when the substrate **60** is attached to the patient **25** as shown in **FIG. 3**, the transducer **50** can be positioned at least partially on an appendage **80** of the patient **25** (such as, for example, a toe, a finger, an ear lobe, etc.).

[0026] As shown in **FIGS. 2 and 3**, the transducer **50** can include one or more “emitters” embodied by a first light-emitting diode (“LED”) **100** and a second LED **105**, each coupled to the substrate **60**. The first LED **100** and the second LED **105** can each emit a different wavelength of light **115** and **120** (as shown in **FIG. 3**) through the appendage **80** of the patient **25**. In one embodiment, the first LED **100** can emit a red wavelength **115** and the second LED **105** can emit an infra-red wavelength **120**. In other embodiments, the transducer **50** can include more or less LEDs than those shown in **FIGS. 2 and 3**. In other embodiments, the transducer **50** can include LEDs that each emit light having different wavelengths than those described with respect to **FIGS. 2 and 3**. Rather than LEDs, other suitable light-emitting devices can be used to emit light toward or through the patient **25**. Also, any suitable wavelength of light can be emitted toward or through the patient **25**. In one embodiment, the transducer **50** can include a photo plethysmograph (PPG) sensor (not shown) having a single LED. The PPG sensor is generally capable of sensing at least heart rate, blood pressure, and perfusion.

[0027] The transducer **50** can also include one or more light sensors or detectors **125** positioned to receive the different wavelengths of light **115** and **120** emitted from the first LED **100** and the second LED **105**, respectively. As shown in **FIG. 3**, the detector **125** can be positioned on the substrate **60** to receive wavelengths **115** and **120** that pass through the appendage **80** when the substrate **60** is properly attached to the patient **25**.

[0028] As noted above, the transducer **50** can include an electrode **55** that serves as an electrode when the monitoring system **20** acquires a single or multiple channels of ECG data. In one embodiment, the electrode **55** can be coupled, electrically and/or physically, to the detector **125**, as will be discussed below with respect to **FIG. 4**. In another embodiment, the electrode **55** can be isolated, electrically and/or physically, from the detector **125** and the additional components of the transducer **50**, as will be discussed below with respect to **FIG. 5**.

[0029] In one embodiment, as shown in **FIG. 4**, the electrode **55** can be electrically coupled to the detector **125** by a reference wire **140**. In this embodiment, the cable **53** coupling the transducer **50** to the monitoring instrument **35** can be a five-wire connection cable. The five-wire connection cable **53** can include a first wire **145**, a second wire **150**, a third wire **155**, a fourth wire **160**, and the reference wire **140**. The first LED **105** can be coupled between the first wire **145** and the reference wire **140**. The second LED **110** can be coupled between the second wire **150** and the reference wire **140**. The detector **125** can be coupled between the third wire **155** and the reference wire **140**. A resistor **170** can be coupled between the fourth wire **160** and the reference wire **140**.

[0030] In another embodiment, as shown in **FIG. 5**, the electrode **55** of the transducer **50** can be electrically isolated

from the detector **125** by being coupled to an isolated reference wire **180**. In one embodiment, the cable **53** coupling the transducer **50** to the monitoring instrument **35** can be a single connection cable including as many wires as necessary. The reference wire **140** can be a reference wire for the oximetry components, while the reference wire **180** can be a reference wire for the reference electrode **55** and the ECG signals.

[0031] As shown in **FIG. 1**, the monitoring instrument **35** can include one or more modules **200** for processing the signals acquired from the electrodes **30**. For example, the modules **200** can include an impedance respiration module **205** for determining the impedance respiration of the patient **25**. The modules **200** also can include an ECG module **210** for generating and analyzing a single or multiple channels of ECG data. In other embodiments, the ECG module can include more than one single-channel module (e.g., for monitoring more than one patient at a remote workstation or for monitoring a mother and a fetus). The modules **200** can further include a pulse oximetry module **215** for determining a level of oxygen saturation in the patient’s blood. The monitoring instrument **35** can also include modules in addition to those shown and described with respect to **FIG. 1**. However, the monitoring instrument **35** can include fewer modules than shown and described with respect to **FIG. 1**.

[0032] The monitoring instrument **35** can also include a display **220**. The display **220** can display one or more signals to a user or caregiver. The display **220** can display patient parameter signals such as one or more ECG signals, an impedance respiration signal, an cardio-respirogram, etc. In some embodiments, the display **220** can include a monitor for electronically displaying a signal. The display **220** in some embodiments can include a printer or an electrocardiograph for displaying a signal.

[0033] **FIG. 6** illustrates an alternative embodiment of the transducer **50**. In addition to the components of the transducer **50** shown in **FIGS. 2 and 3**, the alternative embodiment of the transducer **50** can include a neural-muscular transmission (NMT) device **300**. The NMT device **300** can include a support member **302** (e.g., a semi-rigid support member) and either a flexure sensor **304** or a pressure sensor **306**. The NMT device **300** can be connected to an NMT circuit (not shown) that can apply a stimulus to a peripheral motor nerve, such as the ulnar nerve at the patient’s wrist or elbow. Due to the stimulus, the patient’s adductor pollicis muscle can contract causing the patient’s thumb to twitch inward toward the patient’s fingers. The NMT device **300** can measure the strength of this muscle contraction between the support member **302** and the flexure sensor **304** (which can be located at a point of maximum bending on the support member **302**). Alternatively, the NMT device **300** can measure the strength of the muscle contraction between the support member **302** and the pressure sensor **306** (which can be located on the patient’s thumb). In some embodiments, the support member **302** can be fitted into the space between the patient’s index or middle finger and the patient’s thumb. In some embodiments, the support member **302** can include a channel (not shown) along its length to partially enclose the patient’s finger and thumb.

[0034] In some embodiments (unlike the embodiment shown in **FIG. 6**), the support member **302** does not extend over the electrode **55**. In some embodiments, the flexure

sensor **304** and/or the pressure sensor **306** can include a piezo-electric film or a strain gauge to perform the flexure or pressure sensing, respectively. In some embodiments, sensor **306** may be a motion sensor such as an accelerometer. One suitable NMT sensor is the S/5™ NeuroMuscular Transmission Module M-NMT manufactured by Datex-Ohmeda, Inc. (e.g., Part Number 888418 or 897439).

[0035] NMT is a measurement technology for monitoring the depth of muscle block, which is an important aspect of anesthesia. Although measuring SpO₂ by oximetry at a finger is made more difficult because of finger or hand motion, thumb motion is what is generated during anesthesia monitoring with NMT. Also, both oximetry and NMT measurement techniques are valuable at the same time in patients undergoing surgery or intubation. Although the SpO₂ measurement is not made at the thumb, thumb motion is likely to cause vibrations in the entire hand. As a result, the SpO₂ measurement is conventionally performed on a patient's right hand and the NMT measurement is conventionally performed on the patient's left hand. However, two separate measurements requires additional equipment and cable access to both sides of the patient, in addition to complicating the delivery of care. Also, if NMT and SpO₂ are measured with separate and independent devices, the NMT device often interferes electrically with the SpO₂ device.

[0036] In light of these problems, in one embodiment of the invention, the NMT device **300** and the transducer **50** can be connected to the monitoring system **20** by a single cable **53** in order to operate the NMT device **300** and the transducer **50** in a harmonious, non-interfering manner. Also, the NMT device **300** and the transducer **50** being connected to the monitoring system **20** by a single cable **53** further reduces the number of cables connected to the patient. By operating both devices from the same monitoring system **20**, the SpO₂ measurements can be disabled when the NMT device **300** is operating. The NMT device **300** may operate for about 2 to 5 seconds, but may only operate a few times each minute. Combining the NMT device **300** and the transducer **50** into a single unit also allows measurements to be taken on only one hand of the patient. Therefore, adaptive filtering techniques may be used, triggered or correlated to the activation of the NMT stimulation circuit or the response of the NMT sensor, to attenuate the consequent artifacts in the ECG signals and/or the SpO₂ signals.

[0037] In the alternative embodiment of the transducer **50**, as shown and described with respect to FIGS. 6 and 7, the reference wire **140** can be a reference wire for the oximetry components, the reference wire **180** can be a reference wire for the electrode **55** and the ECG signals, and an additional reference wire **308** (as shown in FIG. 7) can be a reference wire for the flexure sensor **304** of the NMT device **300**. However, in some embodiments, the NMT reference wire **308** can be combined with one or both of the reference wires **140** and **180**. The flexure sensor **304** can include a piezo-electric film that produces a voltage between the NMT reference wire **308** and an NMT sensing wire **310**.

[0038] In one embodiment of the method of the invention, a caregiver can attach the first electrode **40**, the second electrode **45**, and the transducer **50** to the patient **25** (such as, for example, an infant or neonate) in order to obtain an ECG signal and a signal indicative of a level of oxygen saturation.

In another embodiment of the method of the invention, a caregiver can attach the transducer **50** to a finger of the patient **25** and the NMT device **300** to the thumb of patient **25**. Thus, the monitoring system **20** can provide a reduction (with respect to conventional systems) in the total number of connections and lead wires attached to the patient **25**. It should be understood that although the appended claims refer to acts of the method of the invention in a particular order, the scope of the appended claims is not to be limited to any particular order. The acts specified in the appended claims can be performed in various different orders and still fall within the scope of the invention.

[0039] Various features and advantages of the invention are set forth in the following claims.

1. A method of acquiring pulse oximetry and electrocardiogram signals from a patient, the method comprising:

attaching a single transducer to a patient;

acquiring a pulse oximetry signal with the single transducer; and

acquiring an electrocardiogram signal with the single transducer.

2. The method of claim 1 and further comprising generating a blood oxygen saturation output signal based on the pulse oximetry signal.

3. The method of claim 1 and further comprising acquiring a reference electrocardiogram signal with the single transducer.

4. The method of claim 3 and further comprising attaching at least one additional electrode to the patient, and acquiring at least one non-reference electrocardiogram signal from the patient.

5. The method of claim 4 and further comprising generating at least one electrocardiogram output signal based on the reference electrocardiogram signal and the at least one non-reference electrocardiogram signal.

6. The method of claim 5 and further comprising acquiring an impedance respiration signal from the patient.

7. The method of claim 6 and further comprising generating a cardio-respirogram output signal based on the pulse oximetry signal, the reference electrocardiogram signal, the at least one non-reference electrocardiogram signal, and the impedance respiration signal.

8. The method of claim 4 and further comprising generating at least one channel of electrocardiogram output data based on the reference electrocardiogram signal and the at least one non-reference electrocardiogram signal.

9. The method of claim 1 and further comprising attaching the single transducer and at least two additional electrodes to the patient, and acquiring signals to generate a cardio-respirogram output signal.

10. The method of claim 1 and further comprising attaching a neural-muscular transmission device to the patient and acquiring a neural-muscular transmission signal.

11. The method of claim 10 and further comprising filtering at least one of the pulse oximetry signal and the electrocardiogram signal acquired when the neural-muscular transmission signal was being acquired.

12. The method of claim 10 and further comprising ignoring at least one of the pulse oximetry signal and the electrocardiogram signal acquired when the neural-muscular transmission signal was being acquired.

13. The method of claim 10 and further comprising using the neural-muscular transmission signal to monitor anesthesia.

14. The method of claim 1 and further comprising attaching a single transducer to the patient, the single transducer including an oximeter having at least two light-emitting diodes.

15. The method of claim 1 and further comprising attaching a single transducer to the patient, the single transducer including a photo plethysmograph sensor having at least one light-emitting diode.

16. A device for acquiring pulse oximetry and electrocardiogram signals from an appendage of a patient, the device comprising:

a substrate that can be attached to the appendage of the patient;

at least one emitter coupled to the substrate, the at least one emitter positioned to emit radiation through the appendage;

at least one detector coupled to the substrate, the at least one detector positioned to receive the radiation emitted through the appendage, the at least one detector generating a pulse oximetry signal based on the received radiation; and

an electrode coupled to the substrate, the electrode generating an electrocardiogram signal.

17. The device of claim 16 wherein the at least one emitter includes a first red light-emitting diode and a second infra-red light-emitting diode.

18. The device of claim 17 wherein the at least one detector includes a single detector to receive radiation emitted by the first red light-emitting diode and the second infra-red light-emitting diode.

19. The device of claim 16 and further comprising a common reference wire coupled to the electrode and the at least one detector.

20. The device of claim 16 and further comprising an electrocardiogram reference wire coupled to the electrode and an oximetry reference wire coupled to the at least one detector in order to isolate the electrode from the at least one detector.

21. The device of claim 16 and further comprising a multi-wire connector coupled to the at least one emitter, the at least one detector, and the electrode.

22. The device of claim 16 wherein the substrate is sized for attachment to an appendage of at least one of an infant and a neonate.

23. The device of claim 16 wherein the substrate includes an elongated portion adapted to be folded in half over the appendage in order to position the at least one emitter to emit radiation through a first side of the appendage and the at least one detector to receive the emitted radiation through a second side of the appendage.

24. The device of claim 16 and further comprising a neural-muscular transmission device coupled to the substrate, the neural-muscular transmission device generating a neural-muscular signal.

25. The device of claim 24 and further comprising a processor that filters at least one of the pulse oximetry signal and the electrocardiogram signal acquired when the neural-muscular transmission signal was being acquired.

26. The device of claim 24 and further comprising a processor that ignores at least one of the pulse oximetry signal and the electrocardiogram signal acquired when the neural-muscular transmission signal was being acquired.

27. The device of claim 16 wherein the electrode generates a reference electrocardiogram signal.

28. A system for monitoring pulse oximetry and electrocardiogram signals acquired from a patient, the system comprising:

a transducer including

a substrate that can be attached to an appendage of the patient,

at least one emitter coupled to the substrate, the at least one emitter positioned to emit radiation through the appendage,

at least one detector coupled to the substrate, the at least one detector positioned to receive the radiation emitted through the appendage, the at least one detector generating a pulse oximetry signal, and

a first electrode coupled to the substrate, the first electrode generating a reference electrocardiogram signal;

at least one second electrode attached to the patient, the at least one second electrode generating a non-reference electrocardiogram signal; and

a monitoring instrument that receives the pulse oximetry signal, the reference electrocardiogram signal, and the non-reference electrocardiogram signal, the monitoring instrument generating a blood oxygen saturation output signal and at least one electrocardiogram output signal.

29. The system of claim 28 wherein the monitoring instrument generates an impedance respiration signal from at least one of the first electrode and the at least one second electrode.

30. The system of claim 29 wherein the monitoring instrument generates a cardio-respirogram output signal based on the pulse oximetry signal, the reference electrocardiogram signal, the at least one non-reference electrocardiogram signal, and the impedance respiration signal.

31. The system of claim 28 wherein the monitoring instrument generates at least one channel of electrocardiogram output data based on the reference electrocardiogram signal and the at least one non-reference electrocardiogram signal.

32. The system of claim 28 wherein the at least one emitter includes a first red light-emitting diode and a second infra-red light-emitting diode.

33. The system of claim 32 wherein the at least one detector includes a single detector to receive radiation emitted by the first red light-emitting diode and the second infra-red light-emitting diode.

34. The system of claim 28 wherein the transducer includes a common reference wire coupled to the first electrode and the at least one detector.

35. The system of claim 28 wherein the transducer includes an electrocardiogram reference wire coupled to the first electrode and an oximetry reference wire coupled to the at least one detector in order to isolate the first electrode from the at least one detector.

36. The system of claim 35 wherein the transducer includes a multi-wire connector coupled to the at least one emitter, the at least one detector, and the first electrode.

37. The system of claim 28 wherein the substrate is sized for attachment to an appendage of at least one of an infant and a neonate.

38. The system of claim 28 wherein the substrate includes an elongated portion adapted to be folded in half over the appendage in order to position the at least one emitter to emit radiation through a first side of the appendage and the at least one detector to receive the emitted radiation through a second side of the appendage.

39. The system of claim 28 and further comprising a neural-muscular transmission device coupled to the substrate, the neural-muscular transmission device generating a neural-muscular transmission signal, the monitoring instrument generating a neural-muscular transmission output signal for monitoring anesthesia.

40. The device of claim 39 wherein the monitoring instrument filters at least one of the pulse oximetry signal and the electrocardiogram signal acquired when the neural-muscular transmission signal was being acquired.

41. The device of claim 39 wherein the monitoring instrument ignores at least one of the pulse oximetry signal and the electrocardiogram signal acquired when the neural-muscular transmission signal was being acquired.

42. A method of acquiring pulse oximetry and electrocardiogram signals from a patient, the method comprising:

attaching a transducer to an appendage of the patient, the transducer including at least one emitter, at least one detector, and a first electrode;

attaching at least one second electrode to the patient;

acquiring a pulse oximetry signal from the at least one detector;

acquiring a reference electrocardiogram signal from the first electrode;

acquiring at least one non-reference electrocardiogram signal from the at least one second electrode;

generating a blood oxygen saturation output signal based on the pulse oximetry signal; and

generating at least one electrocardiogram output signal based on the reference electrocardiogram signal and the at least one non-reference electrocardiogram signal.

43. The method of claim 42 and further comprising generating an impedance respiration signal based on the first electrode and the at least one second electrode.

44. The method of claim 43 and further comprising generating a cardio-respirogram output signal based on the pulse oximetry signal, the reference electrocardiogram signal, the at least one non-reference electrocardiogram signal, and the impedance respiration signal.

45. The method of claim 42 and further comprising generating at least one channel of electrocardiogram output data based on the reference electrocardiogram signal and the at least one non-reference electrocardiogram signal.

46. A method of acquiring pulse oximetry and electrocardiogram signals from an infant, the method comprising:

attaching a transducer to the infant, the transducer including at least one emitter, at least one detector, and a first electrode;

attaching at least two additional electrodes to the infant; acquiring a pulse oximetry signal from the detector, a reference electrocardiogram signal from the first electrode, and at least two non-reference electrocardiogram signals from the at least two additional electrodes; and

generating a blood oxygen saturation output signal based on the pulse oximetry signal and generating at least one electrocardiogram signal based on the reference electrocardiogram signal and the at least two non-reference electrocardiogram signals.

* * * * *

专利名称(译)	用于获取血氧测量和心电图信号的设备和方法		
公开(公告)号	US20050131282A1	公开(公告)日	2005-06-16
申请号	US10/732985	申请日	2003-12-11
[标]申请(专利权)人(译)	BRODNICK DONALD E SCHLÜTERPAUL 小号 GRAY JAMES 中号 哈金森 GEORGE 中号		
申请(专利权)人(译)	BRODNICK 唐纳德·E SCHLÜTERPAUL S. GRAY JAMES M. 哈金森 乔治·		
当前申请(专利权)人(译)	GE 医疗系统信息技术股份有限公司.		
[标]发明人	BRODNICK DONALD E SCHLUTER PAUL S GRAY JAMES M HUTCHINSON GEORGE M		
发明人	BRODNICK, DONALD E. SCHLUTER, PAUL S. GRAY, JAMES M. HUTCHINSON, GEORGE M.		
IPC 分类号	A61B5/00 A61B5/0402 A61B5/053 A61B5/08 A61B5/22 A61B5/04		
CPC 分类号	A61B5/0402 A61B5/0535 A61B5/0809 A61B5/6838 A61B5/224 A61B5/4821 A61B5/6826 A61B5/14552		
其他公开文献	US7305262		
外部链接	Espacenet USPTO		

摘要(译)

一种用于从患者的附肢获取脉搏血氧测量值和心电图信号的方法和设备。该装置可包括可附接到患者附肢的基板，耦合到基板的发射器，耦合到基板的检测器，以及耦合到基板的电极。该装置可以基于检测器接收的辐射产生血氧饱和度输出信号。该装置还可以产生参考或非参考心电图信号。该装置可包括神经肌肉传输装置。

