



US008078246B2

(12) **United States Patent**  
**Mannheimer et al.**

(10) **Patent No.:** **US 8,078,246 B2**  
 (45) **Date of Patent:** **\*Dec. 13, 2011**

(54) **PULSE OXIMETER SENSOR WITH  
 PIECE-WISE FUNCTION**

(56) **References Cited**

(75) Inventors: **Paul D. Mannheimer**, Danville, CA (US); **Michael E. Fein**, Mountain View, CA (US); **Marcia Fein**, legal representative, Mountain View, CA (US); **Charles E. Porges**, Orinda, CA (US)

(73) Assignee: **Nellcor Puritan Bennett LLC**, Boulder, CO (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1839 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **11/241,063**

(22) Filed: **Sep. 30, 2005**

(65) **Prior Publication Data**

US 2006/0030763 A1 Feb. 9, 2006

**Related U.S. Application Data**

(63) Continuation of application No. 10/798,596, filed on Mar. 10, 2004, now Pat. No. 7,689,259, which is a continuation of application No. 09/836,050, filed on Apr. 16, 2001, now Pat. No. 6,801,797.

(60) Provisional application No. 60/198,109, filed on Apr. 17, 2000.

(51) **Int. Cl.**  
**A61B 5/1455** (2006.01)

(52) **U.S. Cl.** ..... **600/323; 600/331**

(58) **Field of Classification Search** ..... **600/309-344**  
 See application file for complete search history.

**U.S. PATENT DOCUMENTS**

3,721,813 A	3/1973	Condon et al.
4,086,915 A	5/1978	Kofsky et al.
4,586,513 A	5/1986	Hamaguri
4,603,700 A	8/1986	Nichols et al.
4,621,643 A	11/1986	New, Jr. et al.
4,623,248 A	11/1986	Sperinde
4,653,498 A	3/1987	New, Jr. et al.
4,685,464 A	8/1987	Goldberger et al.
4,694,833 A	9/1987	Hamaguri

(Continued)

**FOREIGN PATENT DOCUMENTS**

EP	0 571 225 A2	11/1993
EP	0793942	3/1997
JP	3939782	7/1996
JP	10337282 A	12/1998
JP	2001-245871	3/2000
JP	4038280	11/2007
WO	WO 91/11137	8/1991
WO	WO 93/06775	4/1993
WO	WO 93/13706	7/1993
WO	WO 95/16387	6/1995
WO	WO 00/61000	10/2000

**OTHER PUBLICATIONS**

Such, Hans Olaf; "Optoelectronic Non-invasive Vascular Diagnostics Using multiple Wavelength and Imaging Approach," *Dissertation*, (1998).

*Primary Examiner* — Eric Winakur


*Assistant Examiner* — Chu Chuan (JJ) Liu

(74) *Attorney, Agent, or Firm* — Fletcher Yoder

(57) **ABSTRACT**

A memory in a sensor is used to store multiple coefficients for a physiological parameter. In one embodiment, not only are the sensor's specific calibration coefficients stored in a memory in the sensor for the formula to determine oxygen saturation, but multiple sets of coefficients are stored. The multiple sets apply to different ranges of saturation values to provide a better fit to occur by breaking the R to SpO<sub>2</sub> relationship up into different pieces, each described by a different function. The different functions can also be according to different formulas for determining oxygen saturation.

**17 Claims, 4 Drawing Sheets**

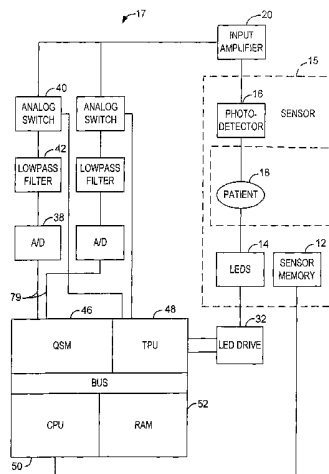

# US 8,078,246 B2

Page 2

## U.S. PATENT DOCUMENTS

4,697,593 A	10/1987	Evans et al.	5,125,403 A	6/1992	Culp
4,700,708 A	10/1987	New, Jr. et al.	5,127,406 A	7/1992	Yamaguchi
4,714,080 A	12/1987	Edgar, Jr. et al.	5,131,391 A	7/1992	Sakai et al.
4,714,341 A	12/1987	Hamaguri et al.	5,140,989 A	8/1992	Lewis et al.
4,759,369 A	7/1988	Taylor	5,152,296 A	10/1992	Simons
4,770,179 A	9/1988	New, Jr. et al.	5,154,175 A	10/1992	Gunther
4,773,422 A	9/1988	Isaacson et al.	5,158,082 A	10/1992	Jones
4,776,339 A	10/1988	Schreiber	5,170,786 A	12/1992	Thomas et al.
4,781,195 A	11/1988	Martin	5,188,108 A	2/1993	Secker et al.
4,796,636 A	1/1989	Branstetter et al.	5,190,038 A	3/1993	Polson et al.
4,800,495 A	1/1989	Smith	5,193,542 A	3/1993	Missanelli et al.
4,800,885 A	1/1989	Johnson	5,193,543 A	3/1993	Yelderman
4,802,486 A	2/1989	Goodman et al.	5,203,329 A	4/1993	Takatani et al.
4,805,623 A	2/1989	Jöbbsis	5,209,230 A	5/1993	Swedlow et al.
4,807,630 A	2/1989	Malinouskas	5,213,099 A	5/1993	Tripp et al.
4,807,631 A	2/1989	Hersh et al.	5,216,598 A	6/1993	Branstetter et al.
4,819,646 A	4/1989	Cheung et al.	5,217,012 A	6/1993	Young et al.
4,819,752 A	4/1989	Zelin	5,217,013 A	6/1993	Lewis et al.
4,824,242 A	4/1989	Frick et al.	5,218,962 A	6/1993	Mannheimer et al.
4,825,872 A	5/1989	Tan et al.	5,224,478 A	7/1993	Sakai et al.
4,825,879 A	5/1989	Tan et al.	5,226,417 A	7/1993	Swedlow et al.
4,830,014 A	5/1989	Goodman et al.	5,228,440 A	7/1993	Chung et al.
4,832,484 A	5/1989	Aoyagi et al.	5,237,994 A	8/1993	Goldberger
4,846,183 A	7/1989	Martin	5,239,185 A	8/1993	Ito et al.
4,848,901 A	7/1989	Hood, Jr.	5,246,002 A	9/1993	Prosser
4,854,699 A	8/1989	Edgar, Jr.	5,246,003 A	9/1993	DeLonzor
4,859,056 A	8/1989	Prosser et al.	5,247,931 A	9/1993	Norwood
4,859,057 A	8/1989	Taylor et al.	5,247,932 A	9/1993	Chung et al.
4,863,265 A	9/1989	Flower et al.	5,249,576 A	10/1993	Goldberger et al.
4,865,038 A	9/1989	Rich et al.	5,253,645 A	10/1993	Freidman et al.
4,867,557 A	9/1989	Takatani et al.	5,253,646 A	10/1993	Delpy et al.
4,869,253 A	9/1989	Craig, Jr. et al.	5,259,381 A	11/1993	Cheung et al.
4,869,254 A	9/1989	Stone et al.	5,259,761 A	11/1993	Schnettler et al.
4,880,304 A	11/1989	Jaeb et al.	5,263,244 A	11/1993	Centa et al.
4,883,055 A	11/1989	Merrick	5,267,562 A	12/1993	Ukawa et al.
4,883,353 A	11/1989	Hansmann et al.	5,267,563 A	12/1993	Swedlow et al.
4,890,619 A	1/1990	Hatschek	5,273,036 A	12/1993	Kronberg et al.
4,892,101 A	1/1990	Cheung et al.	5,275,159 A	1/1994	Griebel
4,901,238 A	2/1990	Suzuki et al.	5,279,295 A	1/1994	Martens et al.
4,908,762 A	3/1990	Suzuki et al.	5,285,783 A	2/1994	Secker
4,911,167 A	3/1990	Corenman et al.	5,285,784 A	2/1994	Seeker
4,913,150 A	4/1990	Cheung et al.	5,287,853 A	2/1994	Vester et al.
4,926,867 A	5/1990	Kanda et al.	5,291,884 A	3/1994	Heinemann et al.
4,927,264 A	5/1990	Shiga et al.	5,297,548 A	3/1994	Pologe
4,928,692 A	5/1990	Goodman et al.	5,299,120 A	3/1994	Kaestle
4,934,372 A	6/1990	Corenman et al.	5,299,570 A	4/1994	Hatschek
4,938,218 A	7/1990	Goodman et al.	5,309,908 A	5/1994	Freidman et al.
4,942,877 A	7/1990	Sakai et al.	5,311,865 A	5/1994	Mayeux
4,948,248 A	8/1990	Lehman	5,313,940 A	5/1994	Fuse et al.
4,955,379 A	9/1990	Hall	5,323,776 A	6/1994	Blakely et al.
4,960,126 A	10/1990	Conlon et al.	5,329,922 A	7/1994	Atlee, III
4,964,408 A	10/1990	Hink et al.	5,337,744 A	8/1994	Branigan
4,971,062 A	11/1990	Hasebe et al.	5,339,810 A	8/1994	Ivers et al.
4,974,591 A	12/1990	Awazu et al.	5,343,818 A	9/1994	McCarthy et al.
5,007,423 A	4/1991	Branstetter et al.	5,343,869 A	9/1994	Pross et al.
5,025,791 A	6/1991	Niwa	5,348,003 A	9/1994	Caro
RE33,643 E	7/1991	Isaacson et al.	5,348,004 A	9/1994	Hollub et al.
5,028,787 A	7/1991	Rosenthal et al.	5,348,005 A	9/1994	Merrick et al.
5,040,539 A	8/1991	Schmitt et al.	5,349,519 A	9/1994	Kaestle
5,054,488 A	10/1991	Muz	5,349,952 A	9/1994	McCarthy et al.
5,055,671 A	10/1991	Jones	5,349,953 A	9/1994	McCarthy et al.
5,058,588 A	10/1991	Kaestle	5,351,685 A	10/1994	Potratz
5,065,749 A	11/1991	Hasebe et al.	5,353,799 A	10/1994	Chance
5,066,859 A	11/1991	Karkar et al.	5,355,880 A	10/1994	Thomas et al.
5,069,213 A	12/1991	Polczynski	5,355,882 A	10/1994	Ukawa et al.
5,078,136 A	1/1992	Stone et al.	5,361,758 A	11/1994	Hall et al.
5,084,327 A	1/1992	Stengel	5,365,066 A	11/1994	Krueger, Jr. et al.
5,088,493 A	2/1992	Giannini et al.	5,368,025 A	11/1994	Young et al.
5,090,410 A	2/1992	Saper et al.	5,368,026 A	11/1994	Swedlow et al.
5,094,239 A	3/1992	Jaeb et al.	5,368,224 A	11/1994	Richardson et al.
5,094,240 A	3/1992	Muz	5,372,136 A	12/1994	Steuer et al.
5,099,841 A	3/1992	Heinonen et al.	5,377,675 A	1/1995	Ruskewicz et al.
5,099,842 A	3/1992	Mannheimer et al.	5,385,143 A	1/1995	Aoyagi
H1039 H	4/1992	Tripp et al.	5,386,827 A	2/1995	Chance et al.
5,104,623 A	4/1992	Miller	5,387,122 A	2/1995	Goldberger et al.
5,109,849 A	5/1992	Goodman et al.	5,390,670 A	2/1995	Centa et al.
5,111,817 A	5/1992	Clark et al.	5,392,777 A	2/1995	Swedlow et al.
5,113,861 A	5/1992	Rother	5,398,680 A	3/1995	Polson et al.
			5,400,267 A *	3/1995	Denen et al. .... 702/59

# US 8,078,246 B2

Page 3

5,402,777 A	4/1995	Warring et al.	5,673,693 A	10/1997	Solenberger
5,411,023 A	5/1995	Morris, Sr. et al.	5,676,139 A	10/1997	Goldberger et al.
5,411,024 A	5/1995	Thomas et al.	5,676,141 A	10/1997	Hollub
5,413,099 A	5/1995	Schmidt et al.	5,678,544 A	10/1997	DeLonzor et al.
5,413,100 A	5/1995	Barthelemy et al.	5,680,857 A	10/1997	Pelikan et al.
5,413,101 A	5/1995	Sugiura	5,685,299 A	11/1997	Diab et al.
5,413,102 A	5/1995	Schmidt et al.	5,685,301 A	11/1997	Klomhaus
5,417,207 A	5/1995	Young et al.	5,687,719 A	11/1997	Sato et al.
5,421,329 A	6/1995	Casciani et al.	5,687,722 A	11/1997	Tien et al.
5,425,360 A	6/1995	Nelson	5,692,503 A	12/1997	Kuenstner
5,425,362 A	6/1995	Siker et al.	5,692,505 A	12/1997	Fouts
5,427,093 A	6/1995	Ogawa et al.	5,709,205 A	1/1998	Bukta
5,429,128 A	7/1995	Cadell et al.	5,713,355 A	2/1998	Richardson et al.
5,429,129 A	7/1995	Lovejoy et al.	5,724,967 A	3/1998	Venkatachalam
5,431,159 A	7/1995	Baker et al.	5,727,547 A	3/1998	Levinson et al.
5,431,170 A	7/1995	Mathews	5,731,582 A	3/1998	West
5,437,275 A	8/1995	Amundsen et al.	D393,830 S	4/1998	Tobler et al.
5,438,986 A	8/1995	Disch et al.	5,743,260 A	4/1998	Chung et al.
5,448,991 A	9/1995	Polson et al.	5,743,263 A	4/1998	Baker, Jr.
5,452,717 A	9/1995	Branigan et al.	5,746,206 A	5/1998	Mannheimer
5,465,714 A	11/1995	Scheuing	5,746,697 A	5/1998	Swedlow et al.
5,469,845 A	11/1995	DeLonzor et al.	5,752,914 A	5/1998	DeLonzor et al.
RE35,122 E	12/1995	Corenman et al.	5,755,226 A	5/1998	Carim et al.
5,482,034 A	1/1996	Lewis et al.	5,758,644 A	6/1998	Diab et al.
5,482,036 A	1/1996	Diab et al.	5,760,910 A	6/1998	Lepper, Jr. et al.
5,483,646 A	1/1996	Uchikoga	5,766,125 A	6/1998	Aoyagi et al.
5,485,847 A	1/1996	Baker, Jr.	5,766,127 A	6/1998	Pologe et al.
5,490,505 A	2/1996	Diab et al.	5,769,785 A	6/1998	Diab et al.
5,490,523 A	2/1996	Isaacson et al.	5,772,587 A	6/1998	Gratton et al.
5,491,299 A	2/1996	Naylor et al.	5,774,213 A	6/1998	Trebino et al.
5,494,032 A	2/1996	Robinson et al.	5,776,058 A	7/1998	Levinson et al.
5,497,771 A	3/1996	Rosenheimer	5,776,059 A	7/1998	Kaestle et al.
5,499,627 A	3/1996	Steuer et al.	5,779,630 A	7/1998	Fein et al.
5,503,148 A	4/1996	Pologe et al.	5,779,631 A	7/1998	Chance
5,505,199 A	4/1996	Kim	5,782,237 A	7/1998	Casciani et al.
5,507,286 A	4/1996	Solenberger	5,782,756 A	7/1998	Mannheimer
5,517,988 A	5/1996	Gerhard	5,782,757 A	7/1998	Diab et al.
5,520,177 A	5/1996	Ogawa et al.	5,782,758 A	7/1998	Ausec et al.
5,521,851 A	5/1996	Wei et al.	5,783,821 A	7/1998	Costello, Jr.
5,522,388 A	6/1996	Ishikawa et al.	5,786,592 A	7/1998	Hök
5,524,617 A	6/1996	Mannheimer	5,790,729 A	8/1998	Pologe et al.
5,529,064 A	6/1996	Rall et al.	5,792,052 A	8/1998	Isaacson et al.
5,533,507 A	7/1996	Potratz	5,795,292 A	8/1998	Lewis et al.
5,551,423 A	9/1996	Sugiura	5,797,841 A	8/1998	DeLonzor et al.
5,551,424 A	9/1996	Morrison et al.	5,800,348 A	9/1998	Kaestle
5,553,614 A	9/1996	Chance	5,800,349 A	9/1998	Isaacson et al.
5,553,615 A	9/1996	Carim et al.	5,803,910 A	9/1998	Potratz
5,555,882 A	9/1996	Richardson et al.	5,807,246 A	9/1998	Sakaguchi et al.
5,558,096 A	9/1996	Palatnik	5,807,247 A	9/1998	Merchant et al.
5,560,355 A	10/1996	Merchant et al.	5,807,248 A	9/1998	Mills
5,564,417 A	10/1996	Chance	5,810,723 A	9/1998	Aldrich
5,575,284 A	11/1996	Athan et al.	5,810,724 A	9/1998	Gronvall
5,575,285 A	11/1996	Takanashi et al.	5,813,980 A	9/1998	Levinson et al.
5,577,500 A	11/1996	Potratz	5,817,008 A	10/1998	Rafert et al.
5,582,169 A	12/1996	Oda et al.	5,817,009 A	10/1998	Rosenheimer et al.
5,584,296 A	12/1996	Cui et al.	5,817,010 A	10/1998	Hibl
5,588,425 A	12/1996	Sackner et al.	5,818,985 A	10/1998	Merchant et al.
5,588,427 A	12/1996	Tien	5,820,550 A	10/1998	Polson et al.
5,590,652 A	1/1997	Inai	5,823,950 A	10/1998	Diab et al.
5,595,176 A	1/1997	Yamaura	5,823,952 A	10/1998	Levinson et al.
5,596,986 A	1/1997	Goldfarb	5,827,182 A	10/1998	Raley et al.
5,611,337 A	3/1997	Bukta	5,830,135 A	11/1998	Bosque et al.
5,617,852 A	4/1997	MacGregor	5,830,136 A	11/1998	DeLonzor et al.
5,619,992 A	4/1997	Guthrie et al.	5,830,137 A	11/1998	Scharf
5,626,140 A	5/1997	Feldman et al.	5,839,439 A	11/1998	Nierlich et al.
5,630,413 A	5/1997	Thomas et al.	RE36,000 E	12/1998	Swedlow et al.
5,632,272 A	5/1997	Diab et al.	5,842,979 A	12/1998	Jarman et al.
5,632,273 A	5/1997	Suzuki	5,842,981 A	12/1998	Larsen et al.
5,634,459 A	6/1997	Gardosi	5,842,982 A	12/1998	Mannheimer
5,638,593 A	6/1997	Gerhardt et al.	5,846,190 A	12/1998	Woehrle
5,638,818 A	6/1997	Diab et al.	5,851,178 A	12/1998	Aronow
5,645,060 A	7/1997	Yorkey	5,851,179 A	12/1998	Ritson et al.
5,645,440 A	7/1997	Tobler et al.	5,853,364 A	12/1998	Baker, Jr. et al.
5,660,567 A	8/1997	Nierlich et al.	5,860,919 A	1/1999	Kiani-Azarbayjany et al.
5,662,105 A	9/1997	Tien	5,865,736 A	2/1999	Baker, Jr. et al.
5,662,106 A	9/1997	Swedlow et al.	5,871,442 A	2/1999	Madarasz et al.
5,666,952 A	9/1997	Fuse et al.	5,879,294 A	3/1999	Anderson et al.
5,671,529 A	9/1997	Nelson	5,885,213 A	3/1999	Richardson et al.
5,673,692 A	10/1997	Schulze et al.	5,890,929 A	4/1999	Mills et al.

# US 8,078,246 B2

Page 4

5,891,021 A	4/1999	Dillon et al.	6,144,444 A	11/2000	Haworth et al.
5,891,022 A	4/1999	Pologe	6,144,867 A	11/2000	Walker et al.
5,891,024 A	4/1999	Jarman et al.	6,144,868 A	11/2000	Parker
5,891,025 A	4/1999	Buschmann et al.	6,149,481 A	11/2000	Wang et al.
5,891,026 A	4/1999	Wang et al.	6,150,951 A	11/2000	Olejniczak
5,902,235 A	5/1999	Lewis et al.	6,151,107 A	11/2000	Schöllermann et al.
5,910,108 A	6/1999	Solenberger	6,151,518 A	11/2000	Hayashi
5,911,690 A	6/1999	Rall	6,152,754 A	11/2000	Gerhardt et al.
5,912,656 A	6/1999	Tham et al.	6,154,667 A	11/2000	Miura et al.
5,913,819 A	6/1999	Taylor et al.	6,157,850 A	12/2000	Diab et al.
5,916,154 A	6/1999	Hobbs et al.	6,163,715 A	12/2000	Larsen et al.
5,916,155 A	6/1999	Levinson et al.	6,165,005 A	12/2000	Mills et al.
5,919,133 A	7/1999	Taylor et al.	6,173,196 B1	1/2001	Delonzor et al.
5,919,134 A	7/1999	Diab	6,178,343 B1	1/2001	Bindzus et al.
5,920,263 A	7/1999	Huttenhoff et al.	6,181,958 B1	1/2001	Steuer et al.
5,921,921 A	7/1999	Potratz et al.	6,181,959 B1	1/2001	Schöllermann et al.
5,922,607 A	7/1999	Bernreuter	6,184,521 B1	2/2001	Coffin, IV et al.
5,924,979 A	7/1999	Swedlow et al.	6,188,470 B1	2/2001	Grace
5,924,980 A	7/1999	Coetzee	6,192,260 B1	2/2001	Chance
5,924,982 A	7/1999	Chin	6,195,575 B1	2/2001	Levinson
5,924,985 A	7/1999	Jones	6,198,951 B1	3/2001	Kosuda et al.
5,934,277 A	8/1999	Mortz	6,206,830 B1	3/2001	Diab et al.
5,934,925 A	8/1999	Tobler et al.	6,213,952 B1	4/2001	Finarov et al.
5,940,182 A	8/1999	Lepper, Jr. et al.	6,217,523 B1	4/2001	Amano et al.
5,954,644 A	9/1999	Dettling et al.	6,222,189 B1	4/2001	Misner et al.
5,960,610 A	10/1999	Levinson et al.	6,226,539 B1	5/2001	Potratz
5,961,450 A	10/1999	Merchant et al.	6,226,540 B1	5/2001	Bernreuter
5,961,452 A	10/1999	Chung et al.	6,229,856 B1	5/2001	Diab et al.
5,964,701 A	10/1999	Asada et al.	6,230,035 B1	5/2001	Aoyagi et al.
5,971,930 A	10/1999	Elghazzawi	6,233,470 B1	5/2001	Tsuchiya
5,978,691 A	11/1999	Mills	6,236,871 B1	5/2001	Tsuchiya
5,978,693 A	11/1999	Hamilton et al.	6,236,872 B1	5/2001	Diab et al.
5,983,122 A	11/1999	Jarman et al.	6,240,305 B1	5/2001	Tsuchiya
5,987,343 A	11/1999	Kinast	6,253,097 B1	6/2001	Aronow et al.
5,991,648 A	11/1999	Levin	6,253,098 B1	6/2001	Walker et al.
5,995,855 A	11/1999	Kiani et al.	6,256,523 B1	7/2001	Diab et al.
5,995,856 A	11/1999	Mannheimer et al.	6,256,524 B1	7/2001	Walker et al.
5,995,858 A	11/1999	Kinast	6,261,236 B1	7/2001	Grimblatov
5,995,859 A	11/1999	Takahashi	6,263,221 B1	7/2001	Chance et al.
5,997,343 A	12/1999	Mills et al.	6,263,222 B1	7/2001	Diab et al.
5,999,834 A	12/1999	Wang et al.	6,263,223 B1	7/2001	Sheperd et al.
6,002,952 A	12/1999	Diab et al.	6,266,546 B1	7/2001	Steuer et al.
6,005,658 A	12/1999	Kaluza et al.	6,266,547 B1	7/2001	Walker et al.
6,006,120 A	12/1999	Levin	6,272,363 B1	8/2001	Casciani et al.
6,011,985 A	1/2000	Athan et al.	6,278,522 B1	8/2001	Lepper, Jr. et al.
6,011,986 A	1/2000	Diab et al.	6,280,213 B1	8/2001	Tobler et al.
6,014,576 A	1/2000	Raley et al.	6,280,381 B1	8/2001	Malin et al.
6,018,673 A	1/2000	Chin et al.	6,285,894 B1	9/2001	Oppelt et al.
6,018,674 A	1/2000	Aronow	6,285,895 B1	9/2001	Ristolainen et al.
6,022,321 A	2/2000	Amano et al.	6,285,896 B1	9/2001	Tobler et al.
6,023,541 A	2/2000	Merchant et al.	6,298,252 B1	10/2001	Kovach et al.
6,026,312 A	2/2000	Shemwell et al.	6,308,089 B1	10/2001	Von der Ruhr et al.
6,026,314 A	2/2000	Amerov et al.	6,321,100 B1	11/2001	Parker
6,031,603 A	2/2000	Fine et al.	6,330,468 B1	12/2001	Scharf
6,035,223 A	3/2000	Baker, Jr.	6,334,065 B1	12/2001	Al-Ali et al.
6,036,642 A	3/2000	Diab et al.	6,339,715 B1	1/2002	Bahr et al.
6,041,247 A	3/2000	Weckstrom et al.	6,343,223 B1	1/2002	Chin et al.
6,044,283 A	3/2000	Fein et al.	6,343,224 B1	1/2002	Parker
6,047,201 A	4/2000	Jackson, III	6,349,228 B1	2/2002	Kiani et al.
6,061,584 A	5/2000	Lovejoy et al.	6,351,658 B1	2/2002	Middleman et al.
6,064,898 A	5/2000	Aldrich	6,353,750 B1	3/2002	Kimura et al.
6,064,899 A	5/2000	Fein et al.	6,356,774 B1	3/2002	Bernstein et al.
6,067,462 A	5/2000	Diab et al.	6,360,113 B1	3/2002	Dettling
6,073,038 A	6/2000	Wang et al.	6,360,114 B1	3/2002	Diab et al.
6,078,833 A	6/2000	Hueber	6,361,501 B1	3/2002	Amano et al.
6,081,735 A	6/2000	Diab et al.	6,363,269 B1	3/2002	Hanna et al.
6,081,742 A	6/2000	Amano et al.	6,370,408 B1	4/2002	Merchant et al.
6,083,157 A	7/2000	Noller	6,370,409 B1	4/2002	Chung et al.
6,083,172 A	7/2000	Baker, Jr. et al.	6,374,129 B1	4/2002	Chin et al.
6,088,607 A	7/2000	Diab et al.	6,377,829 B1	4/2002	Al-Ali et al.
6,094,592 A	7/2000	Yorkey et al.	6,381,479 B1	4/2002	Norris
6,095,974 A	8/2000	Shemwell et al.	6,381,480 B1	4/2002	Stoddard et al.
6,104,938 A	8/2000	Huiku et al.	6,385,471 B1	5/2002	Mortz
6,112,107 A	8/2000	Hannula	6,385,821 B1	5/2002	Modgil et al.
6,113,541 A	9/2000	Dias et al.	6,388,240 B2	5/2002	Schulz et al.
6,115,621 A	9/2000	Chin	6,393,310 B1	5/2002	Kuenster
6,122,535 A	9/2000	Kaestle et al.	6,397,091 B2	5/2002	Diab et al.
6,133,994 A	10/2000	Mathews et al.	6,397,092 B1	5/2002	Norris et al.
6,135,952 A	10/2000	Coetzee	6,397,093 B1	5/2002	Aldrich

# US 8,078,246 B2

Page 5

6,400,971 B1	6/2002	Finarov et al.	6,793,654 B2	9/2004	Lemberg
6,400,972 B1	6/2002	Fine	6,801,797 B2	10/2004	Mannheimer et al.
6,402,690 B1	6/2002	Rhee et al.	6,810,277 B2	10/2004	Edgar, Jr. et al.
6,408,198 B1	6/2002	Hanna et al.	6,813,511 B2	11/2004	Diab et al.
6,411,832 B1	6/2002	Guthermann	6,816,741 B2	11/2004	Diab
6,411,833 B1	6/2002	Baker, Jr. et al.	6,826,419 B2	11/2004	Diab et al.
6,419,671 B1	7/2002	Lemberg	6,830,711 B2	12/2004	Mills et al.
6,421,549 B1	7/2002	Jacques	6,836,679 B2	12/2004	Baker, Jr. et al.
6,430,423 B2	8/2002	DeLonzor et al.	6,845,256 B2	1/2005	Chin et al.
6,430,513 B1	8/2002	Wang et al.	6,852,083 B2	2/2005	Caro et al.
6,438,399 B1	8/2002	Kurth	6,861,639 B2	3/2005	Al-Ali
6,453,183 B1	9/2002	Walker	6,898,452 B2	5/2005	Al-Ali et al.
6,463,310 B1 *	10/2002	Swedlow et al. .... 600/323	6,916,289 B2	7/2005	Schnall
6,463,311 B1	10/2002	Diab	6,939,307 B1	9/2005	Dunlop
6,466,808 B1	10/2002	Chin et al.	6,950,687 B2	9/2005	Al-Ali
6,470,200 B2	10/2002	Walker et al.	6,971,580 B2	12/2005	Zhu et al.
6,496,711 B1	12/2002	Athan et al.	6,979,812 B2	12/2005	Al-Ali
6,498,942 B1	12/2002	Esenaliev et al.	6,993,371 B2	1/2006	Kiani et al.
6,501,975 B2	12/2002	Diab et al.	6,996,427 B2	2/2006	Ali et al.
6,512,937 B2	1/2003	Blank et al.	7,003,339 B2	2/2006	Diab et al.
6,515,273 B2	2/2003	Al-Ali	7,006,855 B1	2/2006	Sarussi
6,519,486 B1	2/2003	Edgar, Jr. et al.	7,024,233 B2	4/2006	Ali et al.
6,519,487 B1	2/2003	Parker	7,035,697 B1	4/2006	Brown
6,525,386 B1	2/2003	Mills et al.	7,039,449 B2	5/2006	Al-Ali
6,526,300 B1	2/2003	Kiani et al.	7,043,289 B2	5/2006	Fine et al.
6,526,301 B2	2/2003	Larsen et al.	7,047,055 B2	5/2006	Boaz et al.
6,541,756 B2	4/2003	Schulz et al.	7,048,687 B1	5/2006	Reuss et al.
6,542,764 B1	4/2003	Al-Ali et al.	7,062,307 B2	6/2006	Norris et al.
6,549,284 B1	4/2003	Boas et al.	7,067,893 B2	6/2006	Mills et al.
6,553,242 B1	4/2003	Sarussi	7,072,702 B2	7/2006	Edgar, Jr. et al.
6,553,243 B2	4/2003	Gurley	RE39,268 E	9/2006	Merrick et al.
6,564,088 B1	5/2003	Soller et al.	7,130,671 B2	10/2006	Baker, Jr. et al.
6,574,491 B2	6/2003	Elghazzawi	7,132,641 B2	11/2006	Schulz et al.
6,580,086 B1	6/2003	Schulz et al.	7,198,778 B2	4/2007	Achilefu et al.
6,584,336 B1	6/2003	Ali et al.	7,215,984 B2	5/2007	Diab et al.
6,587,704 B1	7/2003	Fine et al.	7,254,433 B2	8/2007	Diab et al.
6,594,511 B2	7/2003	Stone et al.	7,272,425 B2	9/2007	Al-Ali
6,594,513 B1	7/2003	Jobsis et al.	7,315,753 B2	1/2008	Baker, Jr. et al.
6,597,933 B2	7/2003	Kiani et al.	7,428,432 B2	9/2008	Ali et al.
6,606,511 B1	8/2003	Ali et al.	7,457,652 B2	11/2008	Porges et al.
6,615,064 B1	9/2003	Aldrich	7,522,948 B2	4/2009	Chin
6,615,065 B1	9/2003	Barrett et al.	2001/0021803 A1	9/2001	Blank et al.
6,622,034 B1	9/2003	Gorski et al.	2002/0026109 A1	2/2002	Diab et al.
6,643,530 B2	11/2003	Diab et al.	2002/0028990 A1	3/2002	Sheperd et al.
6,647,280 B2	11/2003	Bahr et al.	2002/0103423 A1	8/2002	Chin et al.
6,650,917 B2	11/2003	Diab et al.	2002/0128544 A1	9/2002	Diab et al.
6,654,622 B1	11/2003	Eberhard et al.	2003/0018243 A1	1/2003	Gerhardt et al.
6,654,624 B2	11/2003	Diab et al.	2003/0045785 A1	3/2003	Diab et al.
6,658,276 B2	12/2003	Kianl et al.	2003/0132495 A1	7/2003	Mills et al.
6,662,033 B2	12/2003	Casciani et al.	2003/0135099 A1	7/2003	Al-Ali
6,671,526 B1	12/2003	Aoyagi et al.	2003/0162414 A1	8/2003	Schulz et al.
6,671,528 B2	12/2003	Steuer et al.	2003/0197679 A1	10/2003	Ali et al.
6,671,530 B2	12/2003	Chung et al.	2004/0059209 A1	3/2004	Al-Ali et al.
6,671,531 B2	12/2003	Al-Ali et al.	2004/0064020 A1	4/2004	Diab et al.
6,675,031 B1	1/2004	Porges et al.	2004/0068164 A1	4/2004	Diab et al.
6,678,543 B2	1/2004	Diab et al.	2004/0097797 A1	5/2004	Porges et al.
6,681,126 B2	1/2004	Solenberger	2004/0116789 A1	6/2004	Boas et al.
6,681,128 B2	1/2004	Steuer et al.	2004/0133087 A1	7/2004	Ali et al.
6,681,454 B2	1/2004	Modgil et al.	2004/0133088 A1	7/2004	Al-Ali et al.
6,684,090 B2	1/2004	Ali et al.	2004/0147823 A1	7/2004	Kiani et al.
6,684,091 B2	1/2004	Parker	2004/0147824 A1	7/2004	Diab et al.
6,694,160 B2	2/2004	Chin	2004/0152965 A1	8/2004	Diab et al.
RE38,476 E	3/2004	Diab et al.	2004/0158134 A1	8/2004	Diab et al.
6,699,194 B1	3/2004	Diab et al.	2004/0158135 A1	8/2004	Baker, Jr. et al.
6,708,049 B1	3/2004	Berson et al.	2004/0162472 A1	8/2004	Berson et al.
6,714,803 B1	3/2004	Mortz	2004/0176671 A1	9/2004	Fine et al.
6,714,804 B2	3/2004	Al-Ali et al.	2004/0181134 A1	9/2004	Baker, Jr. et al.
RE38,492 E	4/2004	Diab et al.	2004/0204636 A1	10/2004	Diab et al.
6,721,584 B2	4/2004	Baker, Jr. et al.	2004/0204637 A1	10/2004	Diab et al.
6,721,585 B1	4/2004	Parker	2004/0204638 A1	10/2004	Diab et al.
6,725,075 B2	4/2004	Al-Ali	2004/0204639 A1	10/2004	Casciani et al.
6,735,459 B2	5/2004	Parker	2004/0210146 A1	10/2004	Diab et al.
6,745,060 B2	6/2004	Diab et al.	2004/0236196 A1	11/2004	Diab et al.
6,748,253 B2	6/2004	Norris et al.	2005/0020894 A1	1/2005	Norris et al.
6,760,609 B2	7/2004	Jacques	2005/0033128 A1	2/2005	Ali et al.
6,763,255 B2	7/2004	DeLonzor et al.	2005/0033129 A1	2/2005	Edgar, Jr. et al.
6,770,028 B1	8/2004	Ali et al.	2005/0043600 A1	2/2005	Diab et al.
6,771,994 B2	8/2004	Kiani et al.	2005/0065417 A1	3/2005	Ali et al.
6,792,300 B1	9/2004	Diab et al.	2005/0283059 A1	12/2005	Iyer et al.

## US 8,078,246 B2

Page 6

---

2006/0030764 A1 2/2006 Porges et al.  
2006/0161054 A1 7/2006 Reuss et al.  
2006/0200018 A1 9/2006 Al-Ali  
2006/0224059 A1 10/2006 Swedlow et al.  
2006/0258926 A1 11/2006 Ali et al.

2007/0112260 A1 5/2007 Diab et al.  
2008/0039701 A1 2/2008 Ali et al.  
2008/0287757 A1 11/2008 Berson et al.

\* cited by examiner

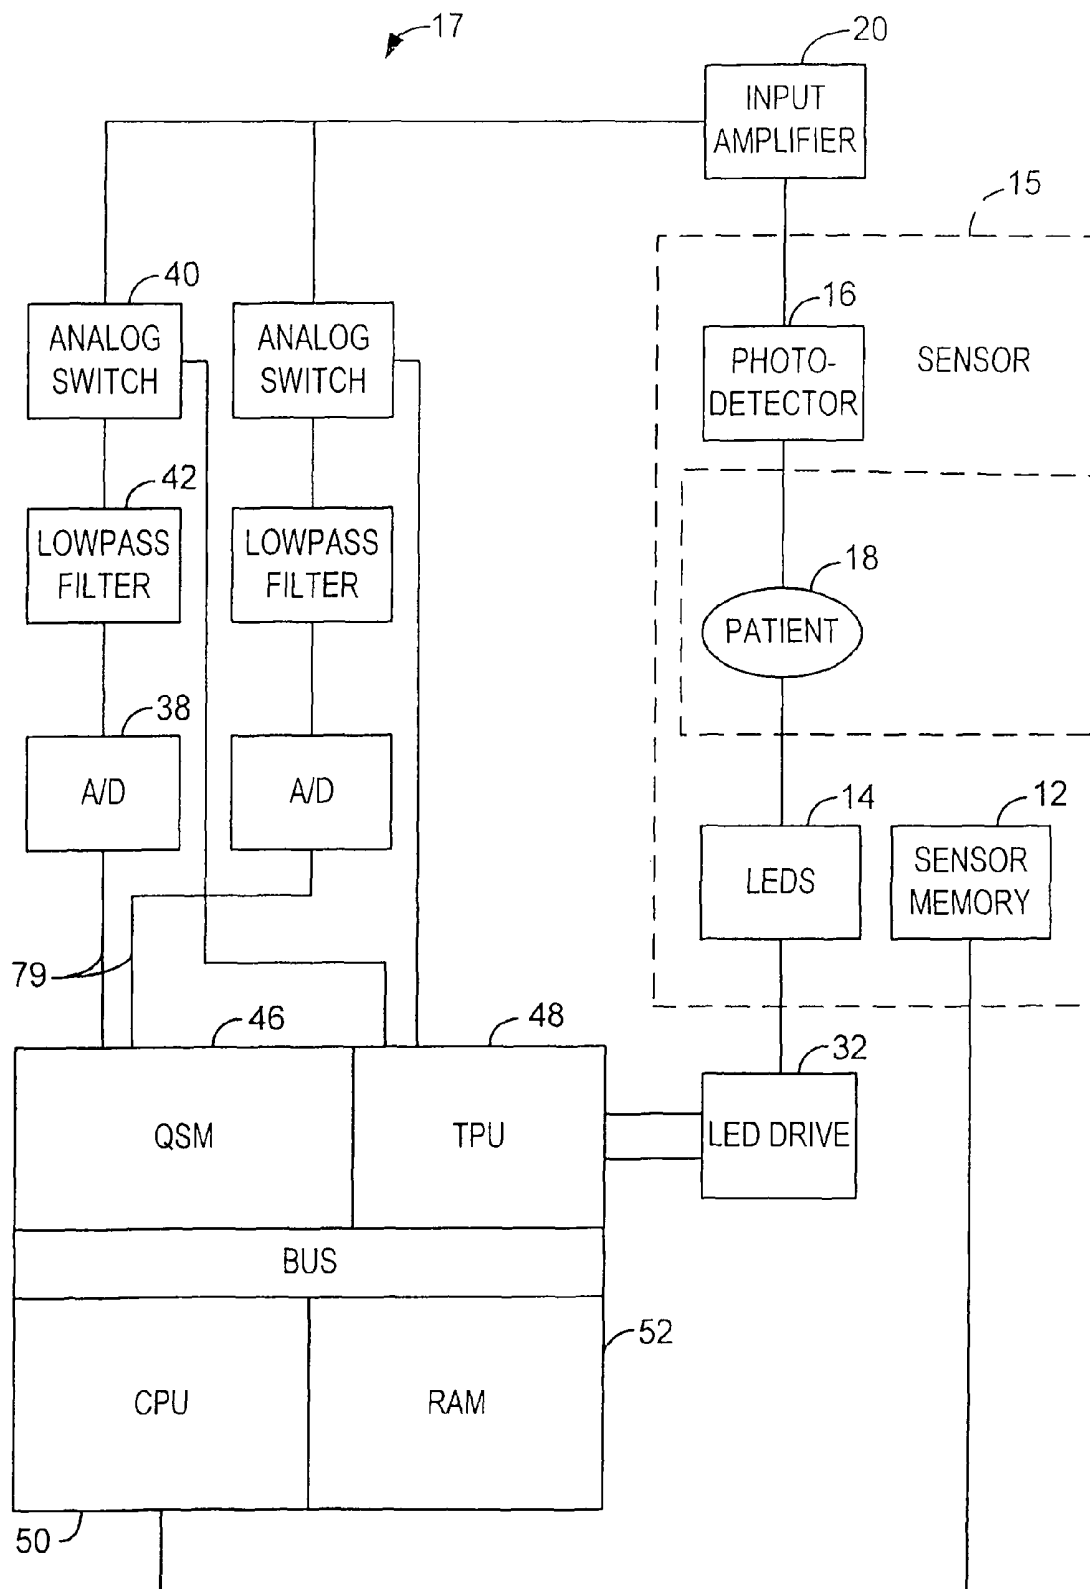
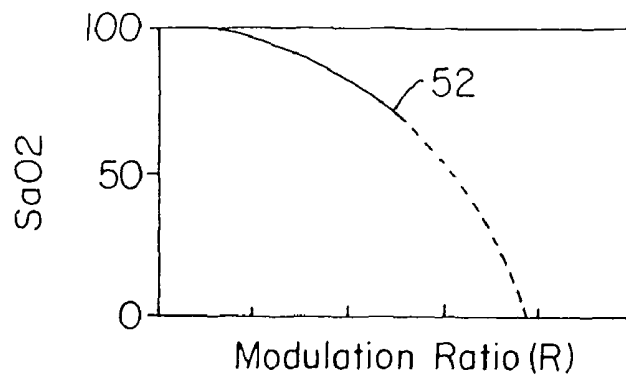
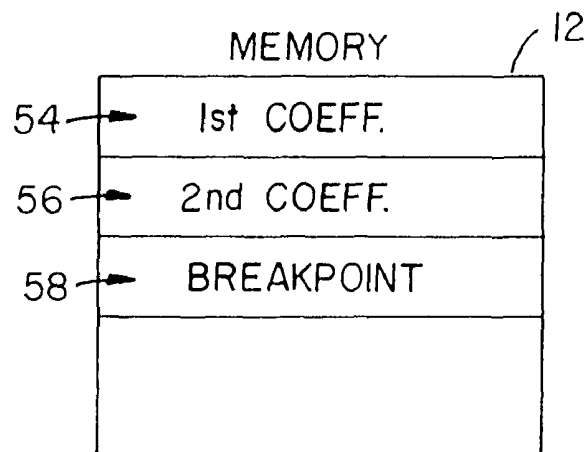
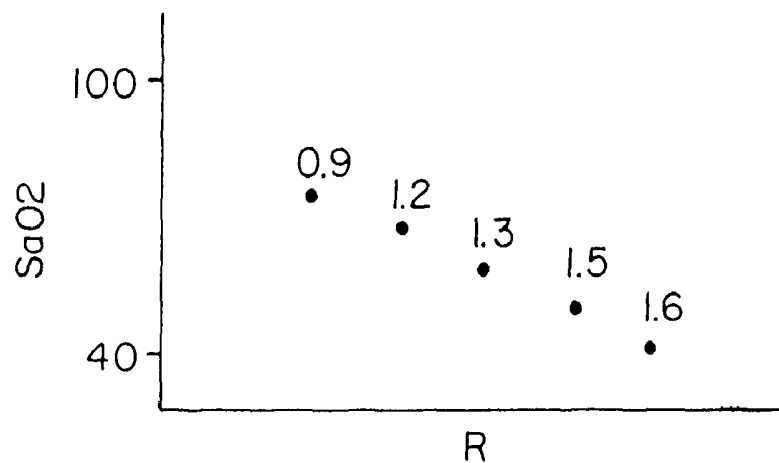


FIG. 1.

*FIG. 2.**FIG. 3.**FIG. 4.*



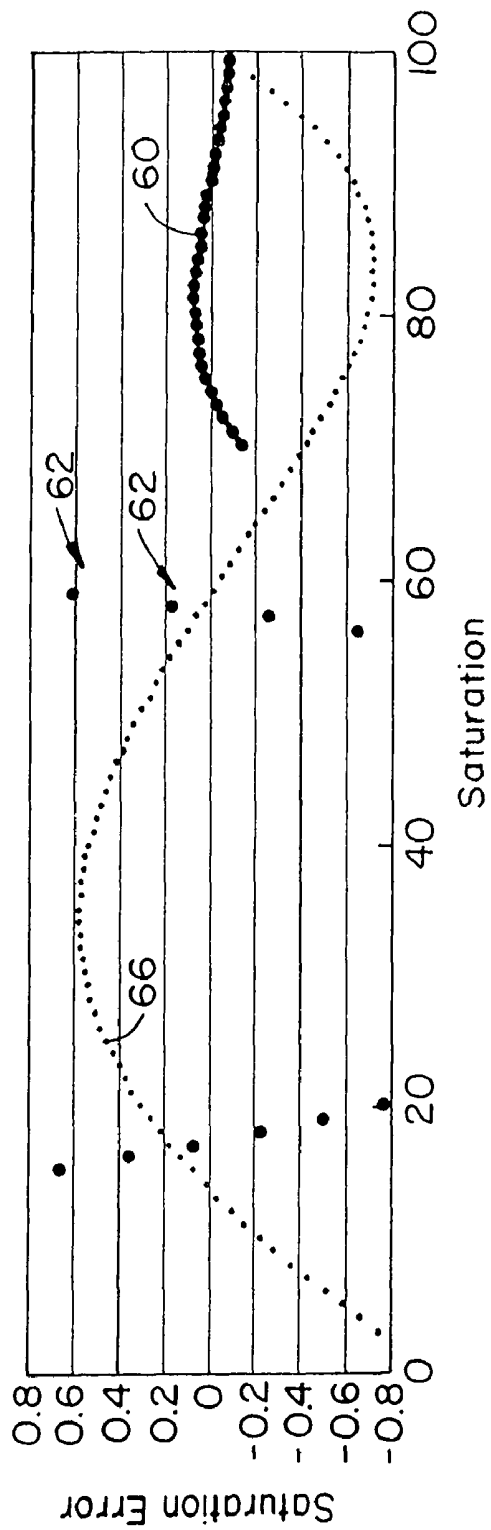


FIG. 5A.

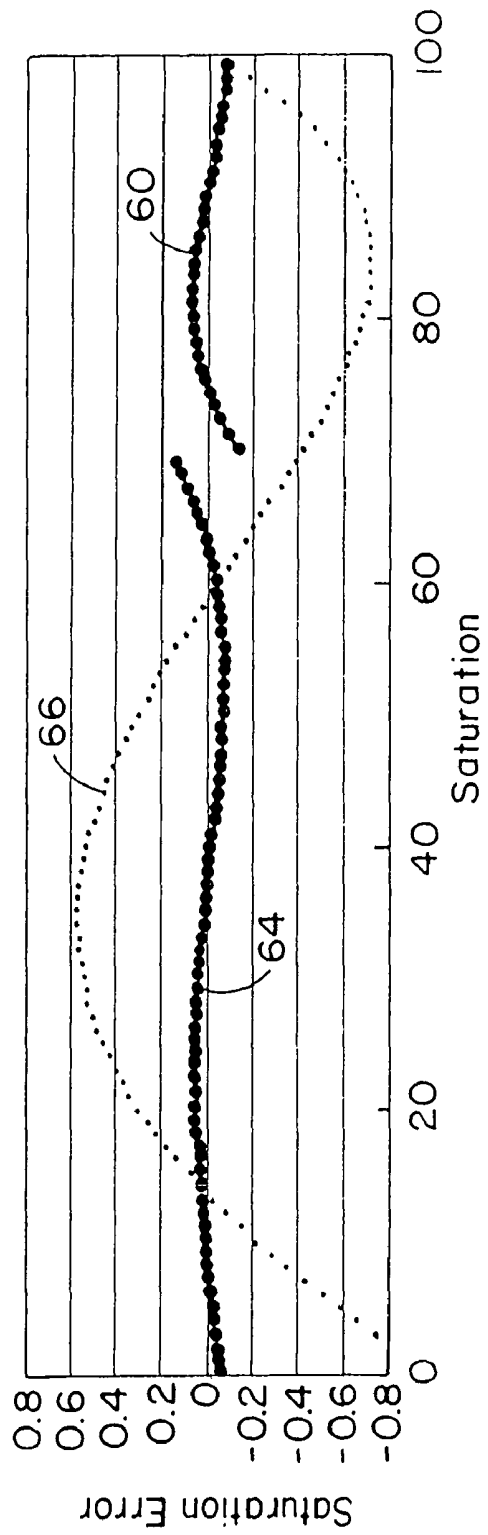


FIG. 5B.

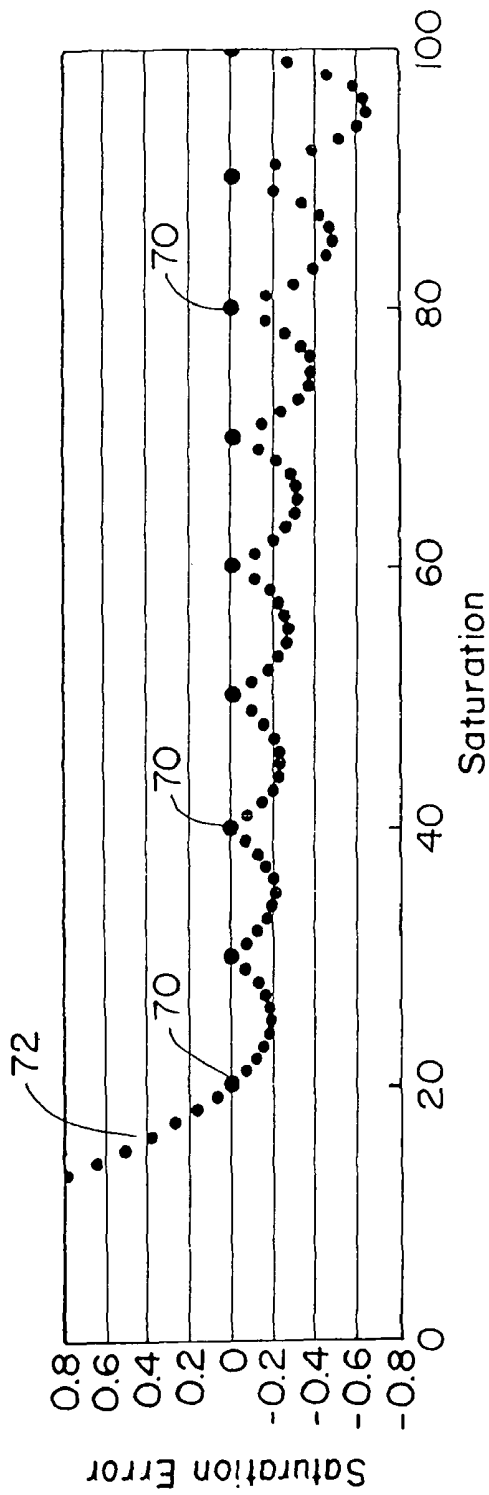


FIG. 6A.

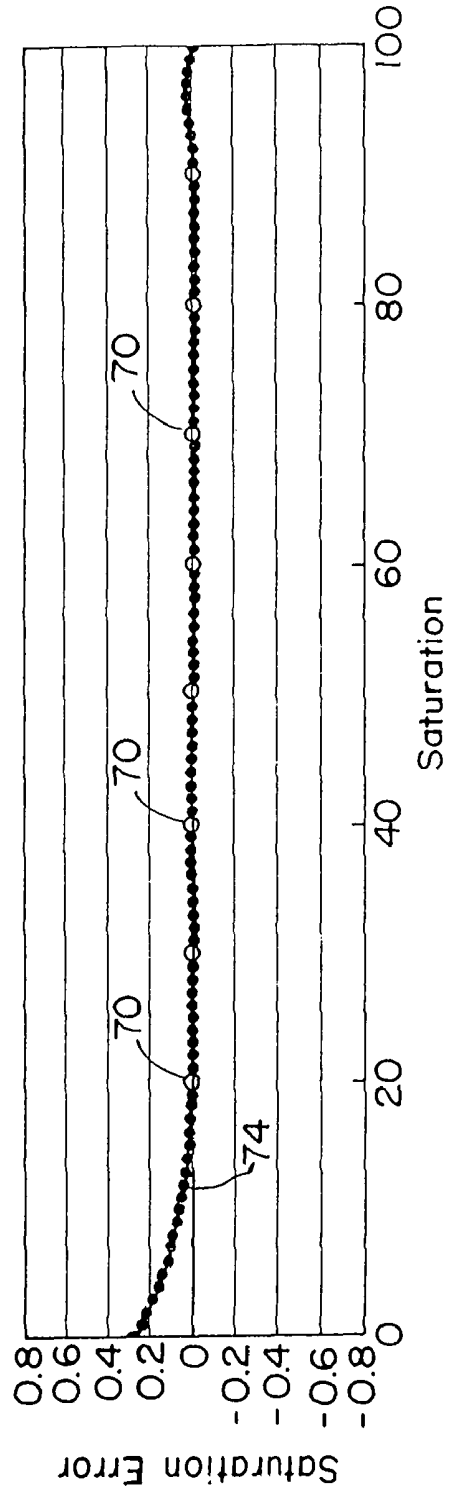


FIG. 6B.

1

# PULSE OXIMETER SENSOR WITH PIECE-WISE FUNCTION

## CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation of U.S. application Ser. No. 10/798,596, filed Mar. 10, 2004 now U.S. Pat. No. 7,689,259, which is a continuation U.S. application Ser. No. 09/836,050, filed Apr. 16, 2001, now U.S. Pat. No. 6,801,797, claims the benefit of U.S. Provisional Application No. 60/198,109, filed Apr. 17, 2000, the disclosures of which are hereby incorporated by reference.

## BACKGROUND OF THE INVENTION

The present invention relates to oximeter sensors having a memory.

Pulse oximetry is typically used to measure various blood flow characteristics including, but not limited to, the blood-oxygen saturation of hemoglobin in arterial blood, and the rate of blood pulsations corresponding to a heart rate of a patient. Measurement of these characteristics has been accomplished by use of a non-invasive sensor which passes light through a portion of the patient's tissue where blood perfuses the tissue, and photoelectrically senses the absorption of light in such tissue. The amount of light absorbed is then used to calculate the amount of blood constituent being measured.

The light passed through the tissue is selected to be of one or more wavelengths that are absorbed by the blood in an amount representative of the amount of the blood constituent present in the blood. The amount of transmitted or reflected light passed through the tissue will vary in accordance with the changing amount of blood constituent in the tissue and the related light absorption. For measuring blood oxygen level, such sensors have been provided with light sources and photodetectors that are adapted to operate at two different wavelengths, in accordance with known techniques for measuring blood oxygen saturation.

Various methods have been proposed in the past for coding information in sensors, including pulse oximeter sensors, to convey useful information to a monitor. For example, an encoding mechanism is shown in Nellcor U.S. Pat. No. 4,700,708. This mechanism relates to an optical oximeter probe which uses a pair of light emitting diodes (LEDs) to direct light through blood-perfused tissue, with a detector picking up light which has not been absorbed by the tissue. The operation depends upon knowing the wavelength of the LEDs. Since the wavelength of LEDs can vary from device-to-device, a coding resistor is placed in the sensor with the value of the resistor corresponding to the actual wavelength of at least one of the LEDs. When the oximeter instrument is turned on, it first determines the value of the resistor and thus appropriate saturation calculation coefficients for the value of the wavelengths of the LEDs in the probe.

Other coding mechanisms have also been proposed in U.S. Pat. Nos. 5,259,381; 4,942,877; 4,446,715; 3,790,910; 4,303,984; 4,621,643; 5,246,003; 3,720,177; 4,684,245; 5,645,059; 5,058,588; 4,858,615; and 4,942,877, the disclosures of which are all hereby incorporated by reference. The '877 patent in particular discloses storing a variety of data in a pulse oximetry sensor memory, including coefficients for a saturation equation for oximetry.

Nellcor pulse oximeter sensors are encoded with a resistor (RCAL) value that corresponds to the wavelength(s) of the LED(s) within the emitter, such as described in U.S. Pat. No.

2

4,700,708. Nellcor pulse oximeter instruments read this resistor coding value and use it as a pointer to a look-up table that holds the proper set of coefficients for that sensor for calculating arterial oxygen saturation ( $\text{SpO}_2$ ). The function that converts the measured red and IR signal modulation ratio  $1R$  (also known as the "ratio of ratios" or "rat-rat") to a calculated saturation value is derived from the basic form of the Lambert-Beer Law:

$$R = \frac{\ln(I_1 / I_2)_{\text{red}}}{\ln(I_1 / I_2)_{\text{ir}}} \quad (1)$$

$$= \frac{S \cdot \beta_{\text{O}_2\text{Hb}}^{\text{red}} + (1 - S) \cdot \beta_{\text{Hb}}^{\text{red}}}{S \cdot \beta_{\text{O}_2\text{Hb}}^{\text{ir}} + (1 - S) \cdot \beta_{\text{Hb}}^{\text{ir}}}$$

$$= \frac{S \cdot c_1 + (1 - S) \cdot c_2}{S \cdot c_3 + (1 - S) \cdot c_4}$$

where  $I_1$  and  $I_2$  refer to detected light signals at two different points in the cardiac cycle, and the  $\beta$ 's refer to the characteristic light absorption properties of oxygenated and deoxygenated hemoglobin. When solved for the saturation ( $S$ ), the result takes on the form:

$$\text{SpO}_2 = S \cdot 100 = \frac{c_2 - c_4 \cdot R}{(c_3 - c_4) \cdot R + (c_2 - c_1)} \cdot 100. \quad (2)$$

Equation 2 can be further simplified to require only three constants (by, for example, dividing each constant by  $c_2$ ), but will be used as shown for the remainder of this description. Although theoretically based, the four constants  $c_1$ - $c_4$  are empirically determined. Theoretical values for the constants are insufficient primarily due to the complexities of light scattering and sensor optics. The values of the sets of constants ( $c_1$  through  $c_4$ ) vary with each resistor coding bin (each "bin" corresponding to a range of different characterized LED wavelengths). Multiple sets of coefficients (bins) are provided within a lookup table in Nellcor oximeters. When calculated  $\text{SpO}_2$  values according to Eq. 2 are less than 70%, a revised value of  $\text{SpO}_2$  using a linear function is used:

$$\text{SpO}_2 = c_5 - c_6 \cdot R, \quad (3)$$

where both  $c_5$  and  $c_6$  vary with the resistor coding value. This linear function was found to better match  $\text{SpO}_2$  (arterial oxygen saturation as measured by a pulse oximeter) with  $\text{SaO}_2$  (the true value of arterial oxygen saturation, as measured directly on a blood sample) in observations made at low saturations.

A limitation of this method is that the proper calibration of the pulse oximetry sensor can be accomplished only if the relationship between the signal modulation ratio ( $R$ ) to blood  $\text{SaO}_2$  conforms to one of the pre-encoded sets of calibration coefficients.

A further limitation of this method is that the relationship between  $R$  and  $\text{SaO}_2$  of the pulse oximetry sensor may not be linear in a low-saturation region, or that the breakpoint may not optimally be located at 70%  $\text{SpO}_2$ .

A yet further limitation of this prior art method is that the functional relationship between the true arterial oxygen saturation and the measured signals may not fit a single function over the entire span of the measurement range.

## SUMMARY OF THE INVENTION

The present invention takes advantage of a memory in the sensor to provide enhanced performance. In one embodi-

ment, not only are the sensor's specific calibration coefficients stored in a memory in the sensor for the formula to determine oxygen saturation, but multiple sets of coefficients are stored. The multiple sets apply to different ranges of saturation values to provide a better fit to occur by breaking the R to SpO<sub>2</sub> relationship up into different pieces, each described by a different function. The different functions can also be according to different formulas for determining oxygen saturation.

In another aspect of the invention, the sensor can store a variable breakpoint between the two functions used for oxygen saturation. The two functions could either be separate formulas or the same formula with different coefficients. This allows optimization to a value other than the 70% breakpoint of the prior art.

In another aspect of the present invention, the sensor can store more than one breakpoint to create more than two functions describing the R to SpO<sub>2</sub> relationship.

In yet another aspect of the present invention, a spline function is used, breaking up the R to SpO<sub>2</sub> relationship into an arbitrary number of regions.

In one embodiment, the coefficients stored in the sensor memory correspond to a non-linear curve for low saturation values below 70% or some other breakpoint(s).

Each of the methods described here improve the fit between the chosen mathematical function and the arterial oxygen saturation by breaking the relationship into subsets of the full measured range and determining optimum coefficients for each range. Spline-fitting, in this context, similarly breaks the full measurement range into subsets to efficiently describe the numerical relational between the underlying tissue parameter of interest and the actual signals being used to estimate its value.

For a further understanding of the nature and advantages of the invention, reference should be made to the following description taken in conjunction with the accompanying drawings.

### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a block diagram of a pulse oximeter system incorporating the present invention.

FIG. 2 is a graph of R (signal modulation ratio) versus oxygen saturation (SaO<sub>2</sub>).

FIG. 3 is a diagram of the contents of a sensor memory according to the invention.

FIG. 4 is a graph of oxygen saturation versus R to illustrate the embodiment for spline or curve fitting to a predefined set of knots.

FIGS. 5A, 5B, 6A and 6B are graphs illustrating the improved curve fitting of the embodiments of the invention versus the prior art.

### DESCRIPTION OF THE SPECIFIC EMBODIMENTS

#### Sensor Reader/Monitor

FIG. 1 is a block diagram of one embodiment of the invention. FIG. 1 shows a pulse oximeter 17 (or sensor reader) which is connected to a non-invasive sensor 15 attached to patient tissue 18. Light from sensor LEDs 14 passes into the patient tissue 18, and after being transmitted through or reflected from tissue 18, the light is received by photosensor 16. Either two or more LEDs can be used depending upon the embodiment of the present invention. Photosensor 16 converts the received energy into an electrical signal, which is then fed to input amplifier 20.

Light sources other than LEDs can be used. For example, lasers could be used, or a white light source could be used with appropriate wavelength filters either at the transmitting or receiving ends.

Time Processing Unit (TPU) 48 sends control signals to the LED drive 32, to activate the LEDs, typically in alternation. Again, depending on the embodiment, the drive may control two or any additional desired number of LEDs.

The signal received from input amplifier 20 is passed through two different channels as shown in the embodiment of FIG. 1 for two different wavelengths. Alternately, three channels for three wavelengths could be used, or N channels for N wavelengths. Each channel includes an analog switch 40, a low pass filter 42, and an analog to digital (A/D) converter 38. Control lines from TPU 48 select the appropriate channel at the time the corresponding LED 14 is being driven, in synchronization. A queued serial module (QSM) 46 receives the digital data from each of the channels via data lines 79. CPU 50 transfers the data from QSM 46 into RAM 52 as QSM 46 periodically fills up. In one embodiment, QSM 46, TPU 48, CPU 50 and RAM 52 are part of one integrated circuit, such as a microcontroller.

#### Sensor Memory

Sensor 15, which includes photodetector 16 and LEDs 14, has a sensor memory 12 associated with it. Memory 12 is connected to CPU 50 in the sensor reader or monitor 17. The memory 12 could be packaged in a body of the sensor 15 or in an electrical plug connected to the sensor. Alternatively, the memory 12 could be packaged in a housing which is attachable to an external surface of the monitor or the memory 12 could be located anywhere in a signal path between the sensor body and the monitor. Specifically, according to some preferred embodiments, a content of the sensor memory 12 could be constant for all sensors associated with a particular sensor model. In this case, instead of putting an individual memory 12 on each sensor associated with this model, the memory 12 could instead be included in a reusable extension cable associated with the sensor model. If the sensor model is a disposable sensor, in this case a single memory 12 would be incorporated into a reusable extension cable. The reusable cable could then be used with multiple disposable sensors.

FIG. 2 is an example of a graph of the ratio of ratios (R) on the X axis versus oxygen saturation (SaO<sub>2</sub>) on the Y axis. Shown is a breakpoint 52. In the prior art, a breakpoint of 70% was pre-defined in the monitor software. To the right of the breakpoint (oxygen saturations between 70-100%) a formula was used with four coefficients. To the left of the breakpoint in the prior art, a linear equation was used with two coefficients. The present invention provides increased flexibility and accuracy by using a non-linear formula for the portion of the curve to the left of breakpoint 52. By using a memory chip in the sensor itself, it is possible to actually store these coefficients on the memory chip, as well as the separate coefficients for the higher saturation values.

In another embodiment of the invention, breakpoint 52 can be stored in the memory chip, and chosen to optimize the curve fitting for the two sets of coefficients. In other words, a better fit to the two curves may be obtained if the breakpoint is 68%, for example. In an alternate embodiment, multiple breakpoints and curves might be used. In addition, rather than using the same formula, different formulas could be used for different sections in another embodiment.

FIG. 3 illustrates the contents of sensor memory 12 of FIG. 1. As illustrated, in a first section of memory 54 are stored a first set of coefficients. A second portion of memory 56 stores a second set of coefficients. Finally, in a third section of memory 58, the breakpoint 52 is stored. Different combinations of these elements could be stored in different memories.

For example, the breakpoint could be left out of some, and in others a breakpoint may be provided with only one set of coefficients (with the other set of coefficients in the monitor). Alternately, a breakpoint might be implied from a sensor model number which is stored in the memory, or some other ID value.

$\beta$ -equation:

In one embodiment, an enhanced form of the curvilinear function is used. Instead of using Eq. 3 (linear) in the lower saturation region, Eq. 2 (non-linear) is used for both the upper and lower saturation regions. The breakpoint that defines when to switch coefficients from an upper-region set to a lower-region set is defined by another coefficient. The breakpoint can be programmed either as a value of R, or as a value of SpO<sub>2</sub>. With the breakpoint defined as a value of R, the algorithm becomes:

$$\text{SpO}_2 = \frac{b - d \cdot R}{(c - d) \cdot R + (b - a)} \cdot 100 \begin{cases} R \leq c_5: a = c_1, b = c_2, c = c_3, d = c_4 \\ R > c_5: a = c_6, b = c_7, c = c_8, d = c_9 \end{cases} \quad (4)$$

#### Curve Fitting

Curve fitting to multiple regions follows the same methodology as fitting to a single region. Simply put, the data is partitioned into separate regions and coefficients are determined for each region separately. Commercially available software programs are available, (for example, Mathcad, (Mathsoft, Inc., Cambridge, Mass.)). The process can also be found in, for example, Data Reduction and Error Analysis for the Physical Sciences (Philip Beviyton, McGraw-Hill, New York 1969, Ch. 11—Least squares fit to an arbitrary function).

#### Spline Fitting

An alternate embodiment uses either spline (curve) fitting, or linear or higher order interpolation to a predefined set of SpO<sub>2</sub> vs R values ("knots"). A "knot" is a term of art in spline fitting that refers to an x-y pair corresponding to a node on a line, with a number of such knots defining the line. Spline fitting is a technique for interpolation.

For instance, the values of R at specifically defined SpO<sub>2</sub> values would be stored in the sensor memory. An example of this looks like:

R =	a	b	c
SpO <sub>2</sub> =	100	95	90

Alternatively, though less preferably, the independent variable could be swapped:

R =	0.5	0.6	0.7
SpO <sub>2</sub> =	x	y	z

- Only the bold values (e.g., a, b and c) would need to be stored with fixed, pre-selected spaced values of SpO<sub>2</sub> (equally spaced or unequally spaced). Or, alternatively, preselected values of R.
- An alternative approach would store within the sensor memory the SpO<sub>2</sub>(minimum) and SpO<sub>2</sub>(maximum) values

of the spline range, the number of knots that will be defined, and the sequence of defined values of R for those knots.

- A further alternative approach could store both SpO<sub>2</sub> and the associated R value for each knot.

For each of these options, the instrument would use a spline-fitting algorithm, preferably a cubic spline, to determine the SpO<sub>2</sub> at the measured value of R according to the stored values (an alternative could be a linear or higher order interpolation algorithm).

FIG. 4 illustrates the cubic spline method. FIG. 4 is a graph of oxygen saturation vs. R for a particular sensor emitter. Thus, instead of storing the coefficients as in the prior art method, the actual R or oxygen saturation values are calculated and stored in the sensor memory for that particular sensor's characteristics (e.g., emitter wavelengths). When the oximeter measures the signal level of the light detector, it determines an oxygen saturation value by determining the point on the curve associated with the calculated R value between two of the sample points shown in FIG. 4.

There exists a trade-off in the number of knots defined and the amount of memory required to store them. Too few knots requires very little storage memory, but may not adequately describe the functional relationship; too many over-define the curve and consumes more memory. The inventors have found that knots spaced 5%-10% apart give adequate results. Cubic Spline Calculation:

The process for cubic spline interpolation is known to those skilled in the art. Intrinsic in using the spline method is that the value of R needs to be determined first before being translated to SpO<sub>2</sub>. The preferred process for spline interpolation can be accomplished using the functions provided in Mathcad, and treats the endpoints with cubic functions. Other references for cubic spline interpolations are available.

The process of finding the coordinates of the knots in empirical data with a significant amount of noise may require an additional step. Commercially available basic curve fitting programs may be used (sigmaPlot, or TableCurve, or Mathematical for instance) to determine a best-fit functional approximation to the data. Alternately, one can perform a least-squares fit of an arbitrarily chosen analytical function and pick the values of R at the knot locations (SaO<sub>2</sub> values). The analytical function can be an overlapping piece-wise polynomial (e.g., linear or parabolic), or the curvilinear equation of Eq. 1 or Eq. 4. Another approach is to perform a least-squares selection of the knots directly.

FIG. 5A shows the conventional curve fitting of the prior art, wherein a linear relationship is used below 70% saturation, with a curvilinear approach above 70%. The residual error due to an imperfect fit to the actual R to SaO<sub>2</sub> response for the curvilinear approach above 70% saturation is illustrated by curve 60, while the residual error of the linear interpolation approach below 70% is illustrated by dots 62. FIG. 5B illustrates the use of curvilinear fits in both regions, with a different curvilinear curve 64 being used below 70%. In this instance, a much improved fit is provided. In both figures, the smaller dotted line 66 corresponds to the use of a single curvilinear fit across both regions, which is also not as accurate, having a much higher error characteristic compared to the curves of the invention, 64 and 60 of FIG. 5B.

FIGS. 6A and 6B show a plurality of knots as circles 70 on the graphs. Dotted line 72 of FIG. 6A illustrates a linear interpolation fit to these knots, which shows a residual error prone result with multiple loops. In FIG. 6B, on the other hand, the present invention using a cubic spline fitting approach provides a dotted line 74 which is a more accurate fit to the knots 70.

As will be understood by those of skill in the art, the present invention may be embodied in other specific embodiments without departing from the essential characteristics thereof. For example, any function can be used for the formulas for determining oxygen saturation, not just the ones described. For a limited sensor memory, the function representation may be compressed. Any representation of a function could be used. Calibration coefficients may be based on more or different characteristics than the sensor's LED wavelength(s). For example, other LED emitter characteristics or sensor design characteristics can be factors in the sensor's calibration coefficients.

Additionally, the formula for calculating oxygen saturation may be a function of more than the ratio of ratios; for example, other input variables such as signal strength, light levels, and signals from multiple detectors could be used.

This methodology for piece-wise fitting is not limited to oximetry. This method is useful when the relationship between the measured signal and reference value observed during calibration is not adequately described by a single function or set of coefficients over the whole measurement range. The relationship may be broken into subsets, and a piece-wise continuous set of functions may be used to describe the relationship. For example, other blood or tissue constituents could be calculated, such as carboxyhemoglobin, methemoglobin, bilirubin, glucose, lactate, etc. Accordingly, the foregoing description is intended to be illustrative, but not limiting, of the scope of the invention which is set forth in the following claims.

What is claimed is:

1. A memory, comprising:
  - a memory body;
  - a memory disposed within the memory body, the memory storing at least one formula and coefficients for use in the at least one formula for determining oxygen saturation, the coefficients including at least a first set of coefficients and a second set of coefficients, wherein the first and second sets of coefficients are for use in the same formula, different linear formulas, or different nonlinear formulas, the memory also storing an indication of a saturation threshold to facilitate selection between the first set and the second set; and
  - a coupling configured to communicatively couple the memory to a sensor port on an oximeter monitor.
2. The memory of claim 1, wherein the memory body comprises a reusable extension cable having a first end communicatively coupleable to an oximeter sensor and a second end comprising the coupling.
3. A method of manufacturing memory, comprising:
  - providing a memory body;
  - providing a memory disposed within the memory body, the memory storing at least one formula and coefficients for use in the at least one formula for determining oxygen saturation, the coefficients including at least a first set of coefficients and a second set of coefficients, wherein the first and second sets of coefficients are for use in the same formula, different linear formulas, or different nonlinear formulas; and
  - providing a coupling configured to communicatively couple the memory to a sensor port on an oximeter monitor, wherein providing the memory body comprises providing a reusable extension cable having a first end communicatively coupleable to an oximeter sensor and a second end comprising the coupling.
4. A method of operating a memory, comprising:
  - transmitting an indication of saturation threshold, at least one formula, and coefficients from the memory to an

oximeter monitor via a coupling with a sensor port of the oximeter monitor, the coefficients for use in the at least one formula for determining oxygen saturation, the coefficients including at least a first set of coefficients and a second set of coefficients, wherein the first and second sets of coefficients are for use in the same formula, different linear formulas, or different nonlinear formulas, wherein the indication of saturation threshold facilitates selection between the first set and the second set.

5. The method of claim 4, comprising continuously transmitting data from an oximeter sensor to the memory and continuously transmitting the data from the memory to the oximeter monitor.

6. An oximeter system, comprising:

an oximeter sensor, comprising:

- a light emitting element configured to emit light into a patient;
- a light detector configured to detect the light from the patient; and an extension cable, comprising:
  - a first coupling configured to communicatively couple to the oximeter sensor;
  - a memory storing at least one formula and coefficients for use in the at least one formula for determining oxygen saturation, the coefficients including at least a first set of coefficients and a second set of coefficients, wherein the first and second sets of coefficients are for use in the same formula, different linear formulas, or different nonlinear formulas; and
  - a second coupling configured to communicatively couple the memory to a sensor port on an oximeter monitor

an oximeter monitor, comprising:

- a drive circuit configured to provide signals to the oximeter sensor via the sensor port; and
- a read circuit configured to read the at least one formula and the coefficients from the memory in the extension cable via the sensor port.

7. The system of claim 6, comprising a calculation mechanism storing the at least one formula and configured to use the coefficients to determine a blood oxygen saturation level in the patient.

8. An oximeter monitor, comprising:

- a drive circuit configured to provide signals to an oximeter sensor that is coupleable to a patient;
- a circuit configured to receive coefficients and a formula from a memory in a reusable extension cable coupleable with the oximeter sensor; and
- a calculation mechanism configured to utilize the coefficients in the formula to determine a blood oxygen saturation level of the patient.

9. A method of monitor operation, comprising:

- providing signals to an oximeter sensor that is coupleable to a patient;
- receiving information from a memory disposed within a reusable extension cable via the reusable extension cable, which is coupleable to the oximeter sensor, the information comprising coefficients and a formula; and
- utilizing the coefficients in the formula to determine a blood oxygen saturation level of the patient.

10. A method of manufacturing an oximeter sensor, comprising: providing a memory of the oximeter sensor having coefficients and at least one formula stored therein, the coefficients for use in the at least one formula for determining oxygen saturation, the coefficients including at least a first set

of coefficients and a second set of coefficients, wherein the first and second sets of coefficients are for use in the same formula.

11. A method of operating an oximeter sensor comprising: directing light at a patient with a light emitter; receiving light from the patient with a light detector; and transmitting coefficients and at least one formula from a memory of the oximeter sensor to a monitor, the coefficients for use in the at least one formula for determining oxygen saturation, the coefficients including at least a first set of coefficients and a second set of coefficients for the light emitter, wherein the first and second sets of coefficients are for use in the same formula.

12. An oximeter system, comprising:  
an oximeter sensor, comprising:  
a light emitter configured to direct light at a patient;  
a light detector configured to receive light from the patient; and  
a memory storing at least one formula and coefficients for use in the at least one formula for determining oxygen saturation, the coefficients including at least a first set of coefficients and a second set of coefficients for the light emitter, wherein the first and second sets of coefficients are for use in the same formula;  
an oximeter monitor, comprising:  
a drive circuit configured to provide signals to the oximeter sensor; and a read circuit configured to read the at least one formula and the coefficients from the memory of the oximeter sensor.

13. A method of manufacturing an oximeter sensor, comprising:  
providing a memory of the oximeter sensor having stored therein:  
a formula for determining oxygen saturation;  
coefficients for use in the formula for determining oxygen saturation, the coefficients including a first set of coefficients and a second set of coefficients; and  
an indication of a saturation threshold for use in selecting between the first and second sets of coefficients, wherein the first and second sets of coefficients are used in the same formula.

14. A method of operating an oximeter sensor comprising: directing light at a patient with a light emitter; receiving light from the patient with a light detector; and transmitting a formula for determining oxygen saturation and coefficients from a memory of the oximeter sensor to a monitor, the coefficients for use in the formula for determining oxygen saturation, the coefficients including a first set of coefficients and a second set of coefficients for the light emitter, wherein the first and second

sets of coefficients are used in the same formula, wherein selection between the first and second sets of coefficients is based on an indication of a saturation threshold stored in the memory.

15. An oximeter system, comprising:  
an oximeter sensor, comprising:  
a light emitter configured to direct light at a patient;  
a light detector configured to receive light from the patient; and  
a memory storing a formula for determining oxygen saturation and coefficients for use in the formula for determining oxygen saturation, the coefficients including a first set of coefficients and a second set of coefficients for the light emitter, wherein the first and second sets of coefficients are for use in the same formula, the memory further storing an indication of a saturation threshold for use in selecting between the first and second sets of coefficients; and

an oximeter monitor, comprising:  
a drive circuit configured to provide signals to the oximeter sensor; and  
a read circuit configured to read the formula and the coefficients from the memory of the oximeter sensor.

16. An oximeter monitor, comprising:  
a drive circuit configured to provide signals to an oximeter sensor that is coupleable to a patient;  
a read circuit configured to receive a formula and coefficients from a memory of the oximeter sensor, the coefficients including first and second sets of coefficients, the circuit also configured to receive an indication of a saturation threshold from the memory for use in selecting between the first and second sets of coefficients; and  
a calculation mechanism configured to utilize the first and second sets of coefficients in a same formula to determine a blood oxygen saturation level of the patient.

17. A method of monitor operation, comprising:  
providing signals to circuitry of an oximeter sensor that is coupleable to a patient;  
receiving information from a memory of the oximeter sensor, the information comprising a formula and first and second sets of coefficients for a light emitter of the oximeter sensor;  
selecting between the first and second set of coefficients based on an indication of saturation threshold stored in the memory; and  
utilizing the first and second sets of coefficients in a same formula to determine a blood oxygen saturation level of the patient.

\* \* \* \* \*

专利名称(译)	具有分段功能的脉搏血氧仪传感器		
公开(公告)号	<a href="#">US8078246</a>	公开(公告)日	2011-12-13
申请号	US11/241063	申请日	2005-09-30
[标]申请(专利权)人(译)	内尔科尔普里坦贝内特公司		
申请(专利权)人(译)	NELLCOR PURITAN BENNETT INCORPORATED		
当前申请(专利权)人(译)	NELLCOR PURITAN BENNETT LLC		
[标]发明人	MANNHEIMER PAUL D FEIN MICHAEL E FEIN LEGAL REPRESENTATIVE MARCIA PORGES CHARLES E		
发明人	MANNHEIMER, PAUL D. FEIN, MICHAEL E. FEIN, LEGAL REPRESENTATIVE, MARCIA PORGES, CHARLES E.		
IPC分类号	A61B5/1455 G01N21/27 A61B5/00 A61B5/145		
CPC分类号	A61B5/14551 A61B2562/085		
优先权	60/198109 2000-04-17 US		
其他公开文献	US20060030763A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

# 摘要(译)

传感器中的存储器用于存储生理参数的多个系数。在一个实施例中，不仅传感器的特定校准系数存储在传感器的存储器中，用于公式确定氧饱和度，而是存储多组系数。多组适用于不同的饱和度范围，以通过将R与SpO<sub>2</sub>关系分解成不同的片段来提供更好的拟合，每个片段由不同的函数描述。不同的功能也可以根据不同的公式来确定氧饱和度。

