



US 20090287069A1

(19) **United States**

(12) **Patent Application Publication**  
**Naghavi et al.**

(10) **Pub. No.: US 2009/0287069 A1**

(43) **Pub. Date: Nov. 19, 2009**

(54) **METHODS AND APPARATUS FOR REPEATED ISCHEMIC CONDITIONING TREATMENT OF HYPERTENSION AND OTHER MEDICAL CONDITIONS**

(60) Provisional application No. 60/989,946, filed on Nov. 25, 2007, provisional application No. 61/188,043, filed on Aug. 6, 2008.

(75) Inventors: **Morteza Naghavi**, Houston, TX (US); **Albert Andrew Yen**, Houston, TX (US); **Haider Hassan**, Houston, TX (US); **David Panthagani**, Houston, TX (US)

**Publication Classification**

(51) **Int. Cl.**  
*A61B 5/145* (2006.01)  
*A61B 17/135* (2006.01)  
*A61B 5/00* (2006.01)  
(52) **U.S. Cl.** ..... **600/309**; 606/202; 128/898

Correspondence Address:  
**WONG, CABELLO, LUTSCH, RUTHERFORD & BRUCCULERI, L.L.P.**  
**20333 SH 249 6th Floor**  
**HOUSTON, TX 77070 (US)**

(57) **ABSTRACT**

Methods for ischemic conditioning treatments of a chronic medical condition are provided. Baseline disease-related parameters of a patient with a chronic medical condition are measured. Ischemia is induced in the patient by occluding and releasing arterial flow in one or more extremities of the patient. Post-ischemia parameters in the patient are measured. The baseline and post-ischemia parameters are compared to provide an assessment of an ischemic conditioning treatment of a chronic medical condition. The repeated, scheduled delivery of ischemic conditioning provides a beneficial, therapeutic effect on the chronic medical condition. Also provided is a device for pulse oximetry during periods of absent or low pulsatile blood flow including an artificial pulse generator as well as the use of said device in assessment of ischemic conditioning.

(73) Assignee: **IC THERAPEUTICS**, Houston, TX (US)

(21) Appl. No.: **12/511,976**

(22) Filed: **Jul. 29, 2009**

**Related U.S. Application Data**

(63) Continuation-in-part of application No. 12/323,392, filed on Nov. 25, 2008.

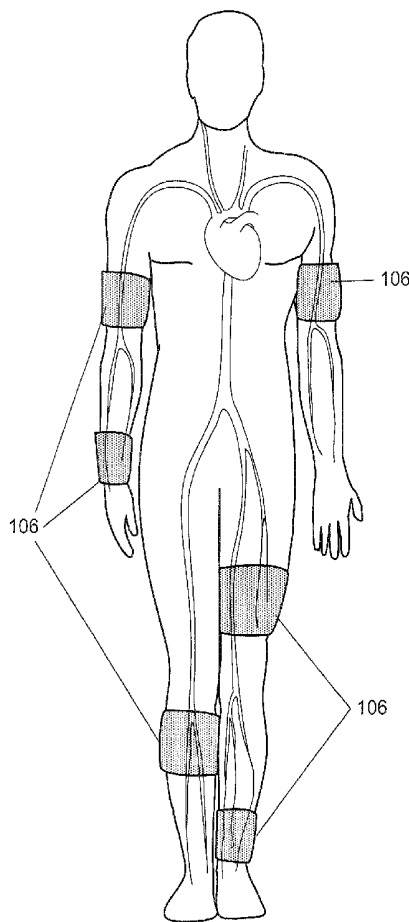


Figure 1

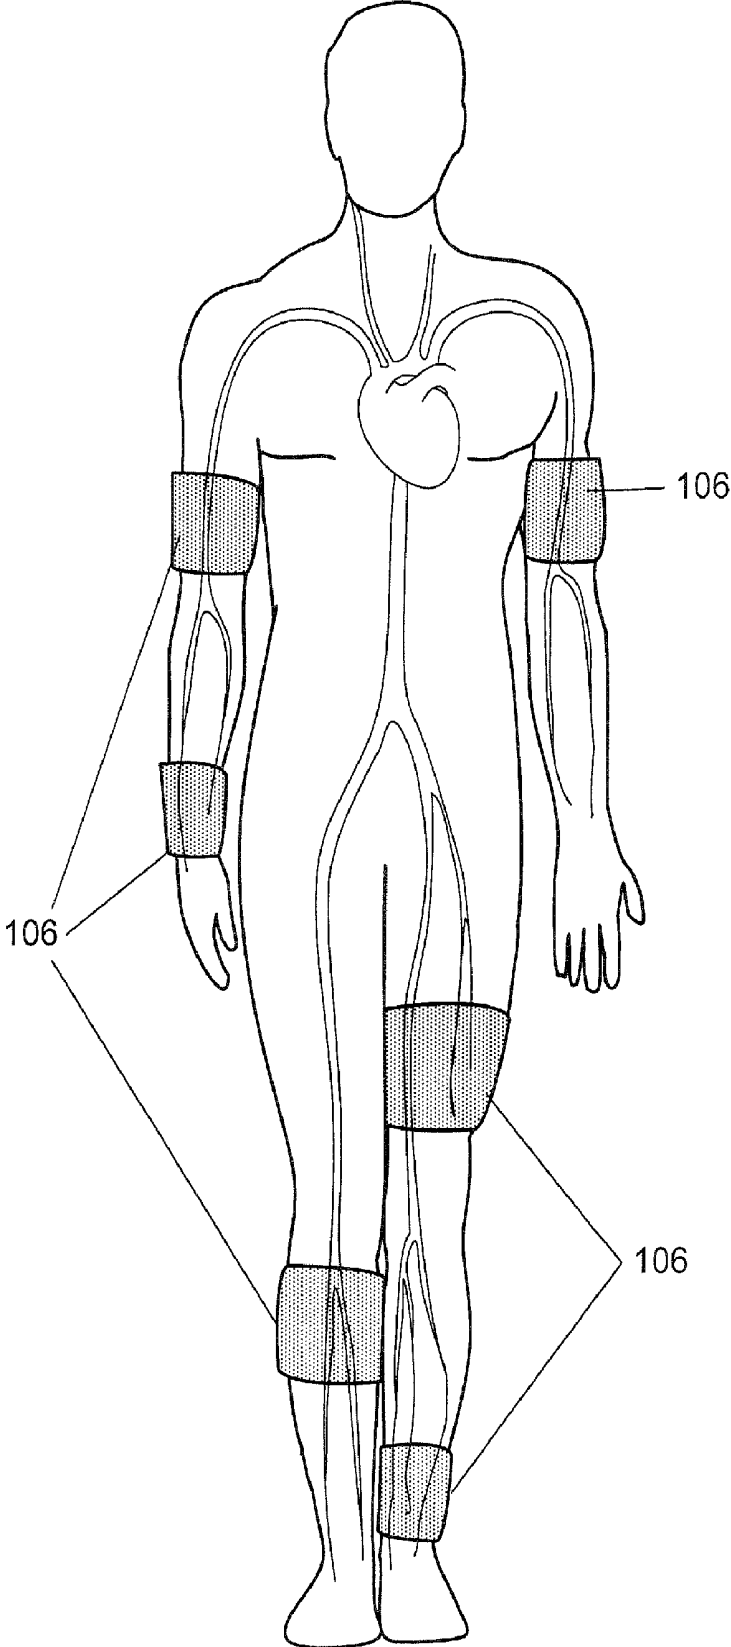


Figure 2

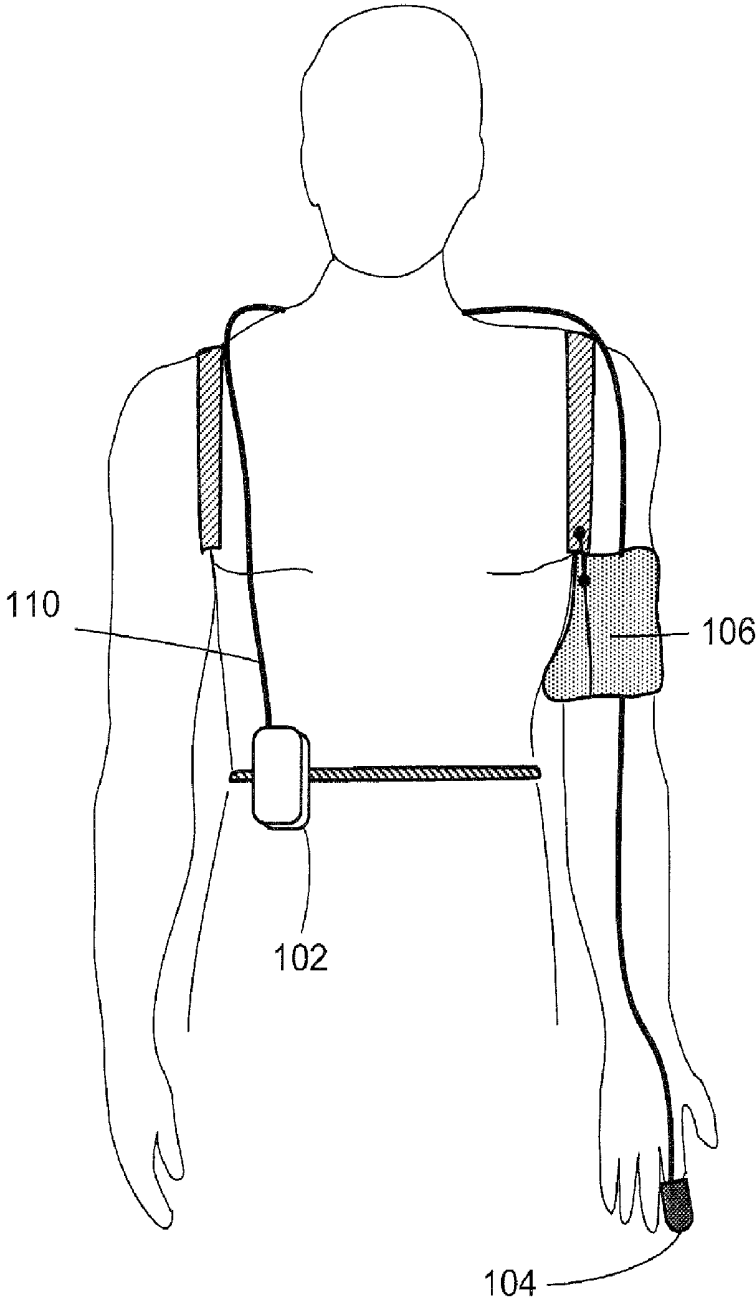


Figure 3a

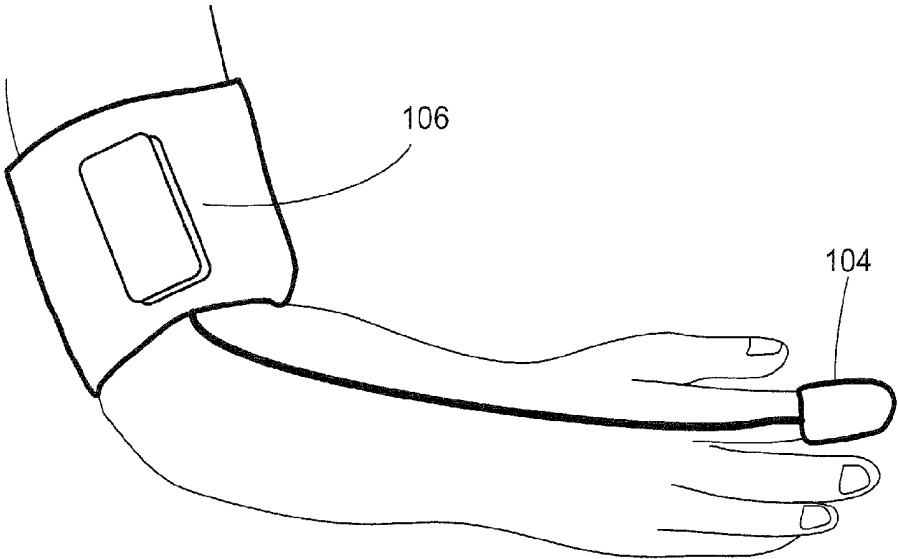


Figure 3b

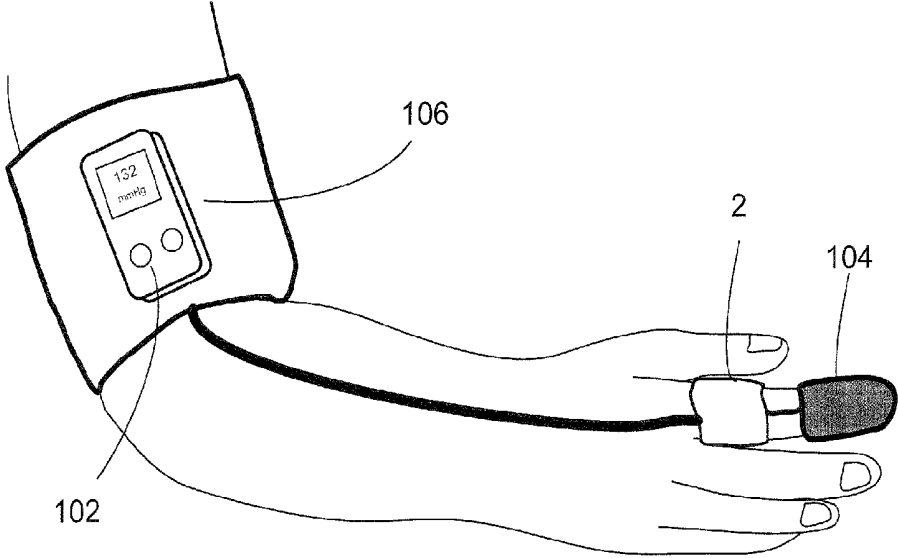


Figure 4a

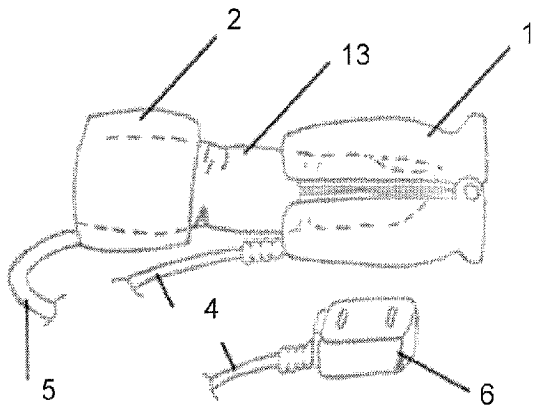


Figure 4c

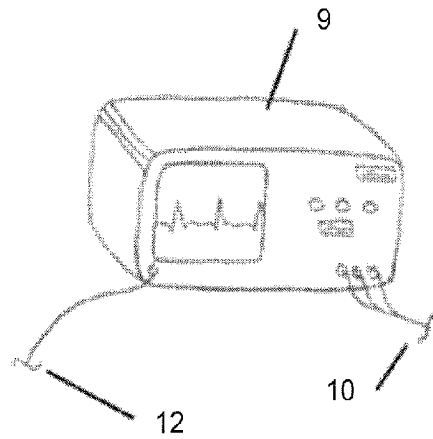


Figure 4b

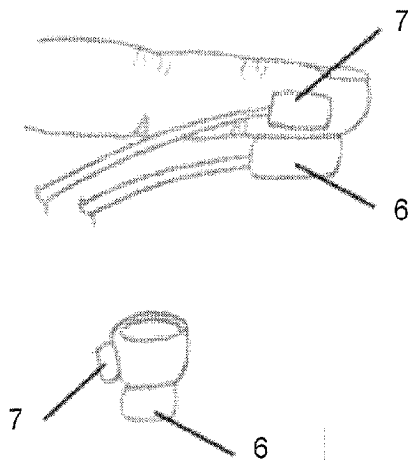


Figure 4d

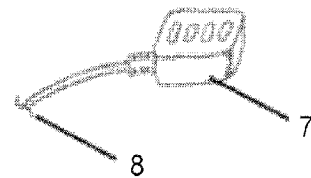


Figure 4e

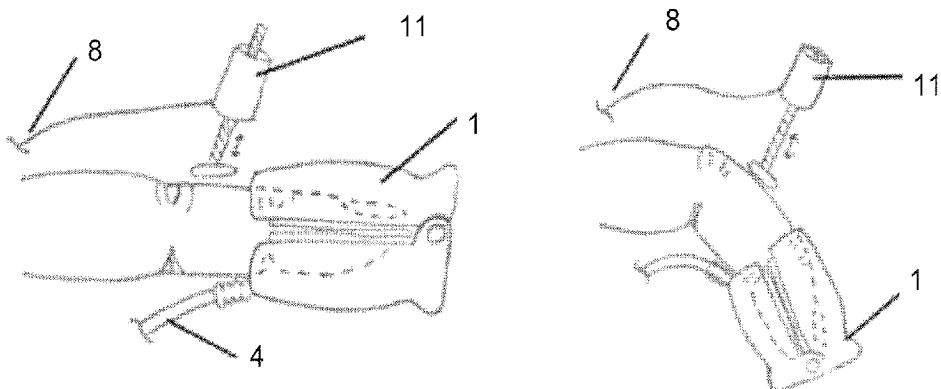


Figure 5a

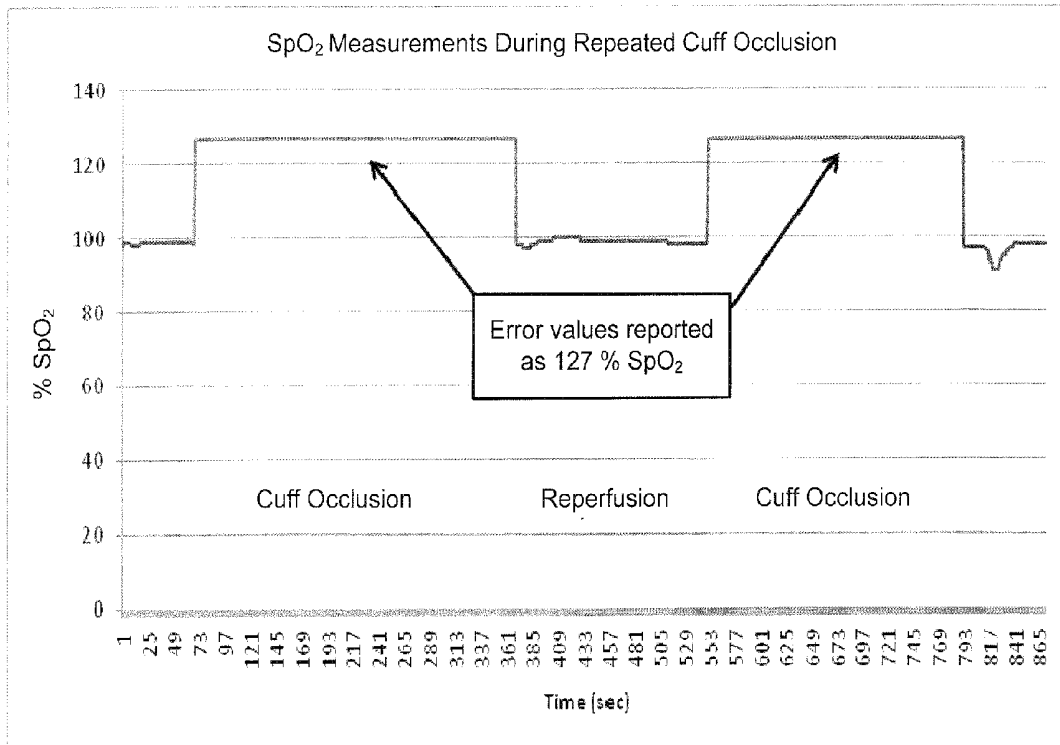


Figure 5b

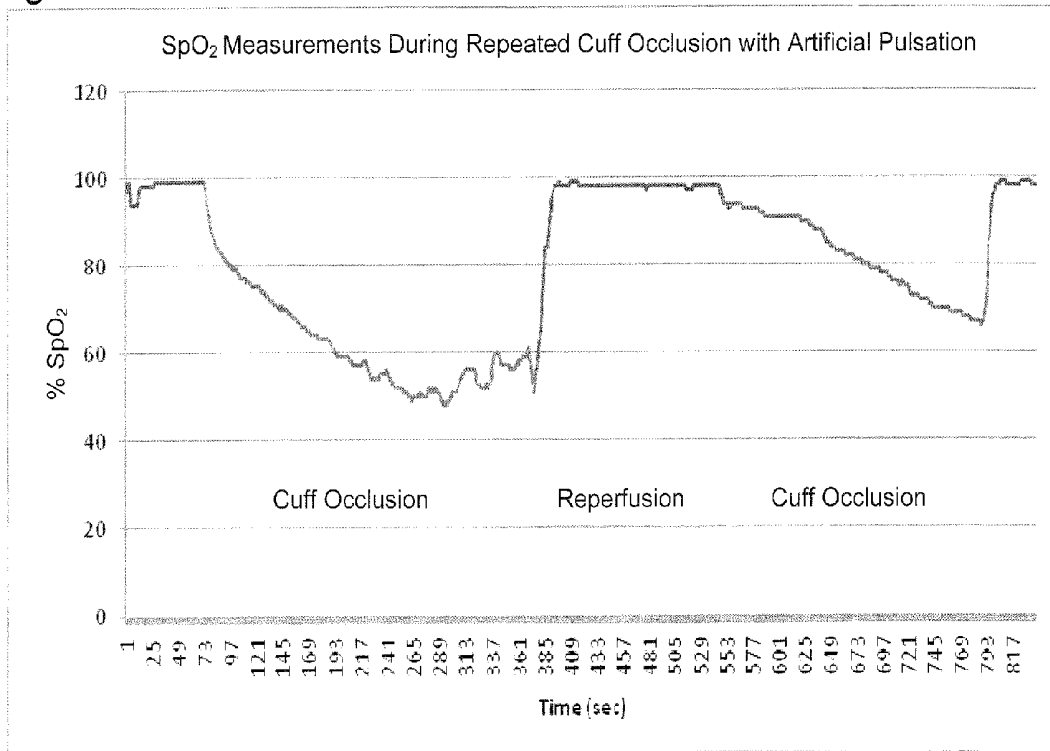


Figure 6a


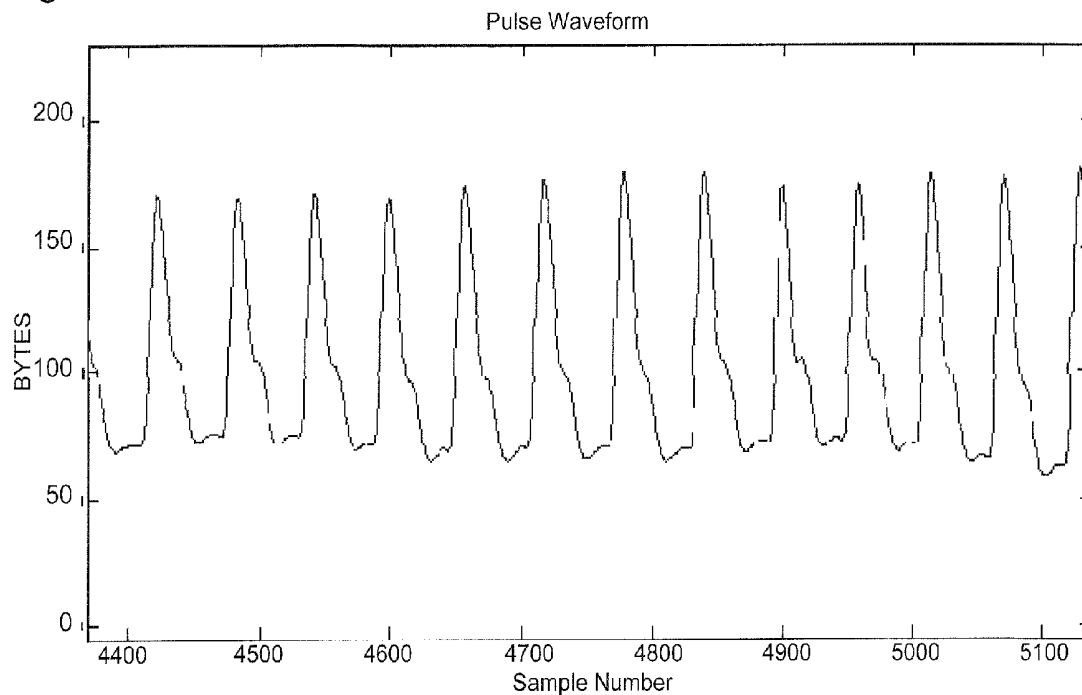


Figure 6b

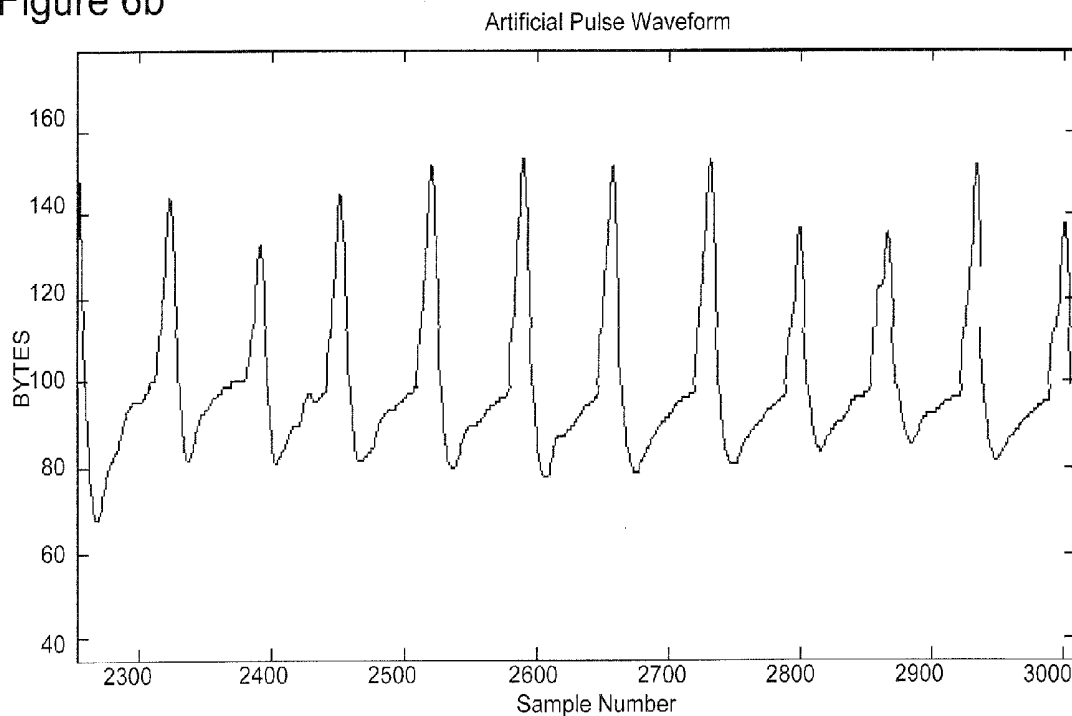

**METHODS AND APPARATUS FOR  
REPEATED ISCHEMIC CONDITIONING  
TREATMENT OF HYPERTENSION AND  
OTHER MEDICAL CONDITIONS**

**CROSS REFERENCE TO RELATED  
APPLICATIONS**

[0001] This application claims priority as a continuation-in-part application of U.S. patent application Ser. No. 12/323,392, Filed Nov. 25, 2008, which in turn claimed priority to U.S. Provisional Application No. 60/989,946 filed Nov. 25, 2007, the disclosures of which are incorporated herein by reference in their entireties. Priority is also claimed to U.S. Provisional Application No. 61/188,043, filed Aug. 6, 2008, entitled "Method and Apparatus for Measuring Blood Oxygen Saturation" and having M. Naghavi, A. Yen, H. Hassan, and D. Panthagani as inventors, the disclosure of which is incorporated herein by reference in its entirety.

**FIELD OF THE INVENTION**

[0002] This invention relates to methods and apparatus for ischemic conditioning to prevent, reduce, and/or treat certain chronic medical conditions, in particular, hypertension. Ischemic conditioning is implemented using noninvasive or invasive arterial occlusion and skin compression, and combinations thereof. More specifically, this invention relates to the treatment of high blood pressure (hypertension) using repeated ischemic conditioning.

**BACKGROUND OF THE INVENTION**

[0003] Without limiting the scope of the invention, its background is described in connection with treatment of hypertension and other chronic medical conditions including but not limited to peripheral arterial disease (PAD), Raynaud's syndrome, coronary heart disease (CHD), coronary artery disease (CAD), diabetes, pulmonary hypertension (PH), and connective tissue disorders.

[0004] By definition, chronic conditions are present when there is a persistent or lasting medical problem. For example, hypertension is considered to be present when there is persistent elevation of either systolic blood pressure or diastolic blood pressure, or when a patient has been placed on antihypertensive medication because of persistently elevated blood pressure (regardless of the current blood pressure level). The blood pressure level correlates directly with the magnitude of risk for clinical sequelae such as premature death, stroke, myocardial infarction, congestive heart failure, renal insufficiency, dementia, and peripheral vascular disease. As a result, numerous antihypertensive drugs have been developed to treat elevated blood pressure. Well known classes of prevalent anti-hypertensives include Angiotensin-Converting Enzyme (ACE) Inhibitors,  $\alpha_1$  Antagonists, Angiotensin II ( $AT_1$ ) Receptor Antagonists,  $\beta$ -Blockers, Calcium Antagonists, Central Adrenergic Inhibitors, Direct Vasodilators, and Diuretics.

[0005] Pharmacological blood pressure lowering reduces the risk of premature cardiovascular morbid and fatal events as well as all-cause mortality. Antihypertensive drug therapy has also been shown to prevent the gradual progression of mild hypertension to more severe elevations of blood pressure. The prevalence of pressure-related target-organ damage (i.e., elevated serum creatinine, left ventricular hypertrophy) is also greater at higher blood pressure levels. Hypertensives

(individuals with chronic hypertension) with pressure-related target-organ damage manifest a several-fold higher risk for pressure-related clinical complications at a given blood pressure level compared to hypertensives with similar levels of pressure without target-organ damage. Early treatment of hypertension favorably impacts long-term clinical risk, in part, by preventing the development of pressure-related target organ damage. However, hypertensive agents can cause hazardous side effects related to the dosage of medicine, the dangers of a rapidly decreasing blood pressure, and ischemic infarction of organ tissues (e.g. angina pectoris, myocardial infarction, transient ischemic attack, and stroke).

[0006] Similarly, other chronic conditions such as peripheral arterial disease and diabetes are also treated by pharmacological therapies. Several other important therapeutic principles are considered in treating patients of chronic conditions. In most cases, there is minimal to no value in rapid pharmacological control of a persistent or recurring condition. Rather, the goal for the vast majority is to prescribe a combination of appropriate lifestyle modifications (e.g. weight loss, dietary restriction, and increased physical activity) plus the lowest doses of drug(s) that allow for normalization over the long term. Further, many medications have dose-related side effects. Drug acquisition costs also usually increase at higher dose levels. In certain instances, cost is a major barrier to patient compliance with prescribed drug therapies. However, even the other noninvasive lifestyle approaches to chronic disease management can be tempered with side effects and ineffectiveness. For example, regular exercise is known to lower blood pressure in healthy individuals by inducing ischemia but also is problematic because it causes an increase in heart rate that may not be tolerated well by some individuals. Further, exercise, diet, and weight loss programs are all well known to suffer problems of compliance.

[0007] Accordingly, what are needed are further methods and apparatus for the management and treatment of chronic medical conditions, in particular hypertension, as well as methods and apparatus for applying ischemic conditioning to improved athletic performance.

**BRIEF SUMMARY OF THE INVENTION**

[0008] The present invention provides methods and apparatus for utilizing the protective effects of repeated, noninvasive applications of ischemic conditioning to treat long term chronic health conditions. In one embodiment of the invention, repeated ischemic conditioning is applied to confer pharmacologic-like and exercise-like therapeutic effects by increasing the vasodilative capacity of the vasculature in the limbs in order to positively affect a vascular condition.

[0009] In one embodiment of the invention, the patient is treated for hypertension, peripheral arterial disease, Raynaud's syndrome, coronary heart disease (CHD), coronary artery disease (CAD), heart failure, pulmonary hypertension (PH), diabetes, and/or connective tissue disorders. In one embodiment of the invention the vascular condition is a starting vascular condition of an athlete and the program of ischemic conditioning is administered on a repeated, scheduled basis adapted to improved endurance and athletic performance.

[0010] In one embodiment of the invention, treatment is effected using transient ischemia. In other embodiments, treatment is complemented using heat, including, for example, photo thermal energy.

**[0011]** In one embodiment, conditioning is effected by transiently and repeatedly administering the treatment to at least one limb, or part thereof, for treatment or prevention of hypertension. The ischemia conditioning treatment in one embodiment is transiently and repeatedly applied according to a schedule that is tailored to the medical and psychosocial needs of the individual patient. In accordance with one embodiment, the program of ischemic conditioning includes at least 1 cycle of from 1 to 20 minutes of occlusion on at least one extremity, at least 2-4 times per week. In one embodiment, the program of ischemic conditioning includes at least 1 cycle of from about 2 to about 5 minutes of occlusion. The program can be adapted to the patient by monitoring the relationship between different administration protocols and the blood pressure of the patient with a goal towards maximizing the lowering of blood pressure in the individual patient. In one version of the invention, the program of ischemic conditioning includes at least 2 cycles of about 2 to about 5 minutes of occlusion followed by about 2 to about 5 minutes of release of an extremity at least 2-4 times per week.

**[0012]** In one embodiment of the invention, the ischemic conditioning is applied to one or more extremities using an external cuff system for arterial occlusion. Alternatively or in addition, the ischemic conditioning is applied to one or more extremities using external pressure to the skin using a pressurizable garment.

**[0013]** In other embodiments, the ischemic conditioning includes a measurement aspect comprising one or more of determining a DTM response and a determination of blood oxygen saturation during ischemia using artificial pulse together with oximetry to improve the ischemic conditioning treatments. The artificial pulse may be generated by mechanical actuation. In some version of the invention, the mechanical actuation is effected by pulsating fluid pressure in a cuff to cause mechanical disturbance of arterial blood, repetitive, external electromechanical actuation, or repetitive, self-induced physical motion. Alternatively or in addition, the artificial pulse may be generated by external non-mechanical optical illumination utilized to imitate an absorption pattern of a pulsatile blood flow signal by oscillating an intensity of a light source of either a single or multiple wave length. Assessment of the progress of the ischemic conditioning treatment may include measuring one or more baseline hemodynamic parameters of a patient, applying an ischemic conditioning treatment in the patient by occluding and releasing arterial flow in one or more extremities of the patient on a scheduled, repeated basis, measuring post-ischemia parameters in the patient, and comparing the baseline and post-ischemia parameters to provide an assessment of the ischemic conditioning treatment over time.

**[0014]** In one embodiment wherein the ischemia conditioning treatment includes induced ischemia, the induced ischemia is sufficient to induce reactive hyperemia in the distal extremity including both hands, both feet, or both hands and feet, and/or portions thereof. The method may be complemented by instructing a schedule of hand and/or foot exercises to the patient.

**[0015]** In one embodiment wherein the ischemia conditioning treatment includes induced ischemia, continued monitoring by pulse oximetry of the induced ischemia, in the absence of pulsatile flow, is enabled by the creation of artificial pulsatile signals. The artificial pulsatile signals can be generated

by either external mechanical actuation that causes oscillatory displacement of blood or external non-mechanical optical illumination.

**[0016]** In one embodiment of the invention, a synergistic combination of physical exercise and ischemic conditioning is provided for prevention and treatment of hypertension. In another embodiment, methods and apparatus for treatment of intermittent claudication (a symptom of peripheral arterial disease) is provided using ischemic conditioning to increase dilative capacity and metabolic efficiency of conditioned areas. As a consequence, patients with intermittent claudication are enabled to walk longer distances and/or suffer less pain when walking the same distance.

**[0017]** In one embodiment employing induced ischemia as a conditioning treatment, the induced ischemia is transiently and repeatedly induced in at least one limb or portion thereof of a patient according to a schedule of vascular occlusions. Alternatively, or in addition to other conditioning treatments, in one embodiment, heat sufficient to induce vasodilation is applied to at least one distal extremity of the patient. In other embodiments, pharmacotherapy is initiated in conjunction with ischemic conditioning and/or heat treatments. The conditioning pharmacotherapy is effected by administration with one or more of the group of vasodilators, anti-oxidants, anti-inflammatory and anesthetic compounds and nitric oxide (NO) donors, precursors and agonists. In one embodiment, the pharmacotherapy is administered systemically.

**[0018]** In one embodiment, an apparatus is provided for transiently inducing ischemia in a peripheral vascular area of a patient, the apparatus including a plurality of releasable compressing elements, each adapted to reduce or occlude flow of blood to at least a portion of an extremity of the patient. The releasable compressing elements may comprise bands dimensioned to be tightened around at least one extremity such as an arm and/or leg to occlude flow of blood to at least a portion of the hands and/or feet. Alternatively, the releasable compressing elements may comprise inflatable compression suits, mittens, socks, stockings, gloves and/or full body suits.

**[0019]** In one embodiment of the invention, apparatus for transiently and repeatedly inducing ischemia in a peripheral vascular area of a patient includes use of a plurality of releasable bands, each adapted to occlude blood supply to at least a hand or foot of the patient when tightened or inflated. As used here, the term band includes cuffs such as inflatable blood pressure type cuffs. The apparatus may be manual in operation or may be automated such as with a control device for controlling compression and release of elements in accordance with a schedule. In one embodiment the apparatus includes a programmable computer for inducing ischemia in accordance with a schedule. In one embodiment the apparatus further includes a pump in operable communication with the releasable compressing elements, wherein the action of the pump results in tightening or inflation by filling of the releasable compressing elements. The apparatus may further include one or more heating mechanisms for intermittent heating at least one hand or foot.

**[0020]** One embodiment disclosed herein provides a device for monitoring blood oxygenation during periods of absent or low pulsatile blood flow by generating an artificial pulse that can be accurately read by a pulse oximeter. In some aspects the artificial pulse is generated by mechanical actuation including by pulsating fluid pressure in a cuff to cause mechanical disturbance of arterial blood, repetitive, external

electromechanical actuation, or repetitive, self-induced physical motion. In other aspects, the artificial pulse is generated by non-mechanical optical illumination utilized to imitate the absorption patterns of a pulsatile blood flow signal by oscillating the intensity of a light source of either a single or multiple wave length.

#### BRIEF DESCRIPTION OF THE DRAWINGS

**[0021]** FIG. 1 depicts several locations for placement of occlusive bands or cuffs for inducing transient intermittent ischemia.

**[0022]** FIG. 2 depicts a halter worn embodiment enabling the patient to wear one or more occlusive cuffs together with a pump and controlling unit for scheduled inflation of the cuff(s).

**[0023]** FIG. 3a depicts an occlusive arm band or cuff in which cuff inflation and deflation can be controlled by a device mounted externally on the cuff and includes a fingertip monitor of induced ischemia. FIG. 3b depicts a system for monitoring the induced ischemia by a fingertip probe that transmits information to the cuff control device and includes a finger mounted artificial pulse generator and pulse oximetry detector.

**[0024]** FIG. 4a depicts a conventional finger pulse oximeter and reflectance oximeter sensor. FIG. 4b depicts a method that involves using external optical illumination to imitate the absorption patterns of pulsatile blood. FIG. 4c depicts an embodiment of the external illumination source that takes its input from an external physiological signal detector such as the ECG device in FIG. 4d. FIG. 4e depicts an embodiment of the device that uses an external electromechanical actuator to cause oscillatory displacement of blood in the underlying blood vessels. These oscillations are detected by the SpO<sub>2</sub> sensor and reported during a low or no flow state.

**[0025]** FIG. 5a shows actual pulse oximetry data collected with a Nonin OEM III module without artificial pulsation during the occlusion periods. FIG. 5b shows actual pulse oximetry data collected with the same Nonin OEM III module as used to collect the data shown in FIG. 5a but with artificial pulsation used to simulate blood flow during the occlusion periods.

**[0026]** FIG. 6a shows a portion of the pulse waveform collected during the reperfusion section shown in FIG. 5a. FIG. 6b shows a portion of the artificial pulse waveform recorded during the cuff occlusion portion of the test case shown in FIG. 5b.

#### BRIEF DESCRIPTION OF THE INVENTION

**[0027]** Disclosed herein is a novel method of conditioning the vasculature of patients in order to reduce the potential for complications that occur with frequency as a consequence of chronic medical conditions, particularly hypertension, but also Raynaud's syndrome, coronary heart disease (CHD), coronary artery disease (CAD), peripheral arterial disease (PAD), diabetes, pulmonary hypertension (PH), and/or connective tissue disorders. In one embodiment, treatment of these chronic conditions is provided by repeated treatment or conditioning by using transient ischemia or hypoxia in order to increase the vasodilative capacity of the vasculature. In other embodiments, treatment is provided by application of heat at levels sufficient to induce peripheral vasodilatation and increase cardiac output and vasodilative capacity. Treatment may be augmented using pharmacologic interventions

including blood pressure lowering drugs. In effect, the methods and apparatus of the present invention emulate the positive effects of exercise on the vasculature in a population that has reduced capacity for exercise due to their chronic disease status.

**[0028]** The invention relies, at least in part, on physiologic reactions to ischemia. Brief periods of ischemia (a local shortage of oxygen-carrying blood supply) in biological tissue, render that tissue more resistant to subsequent ischemic insults through several mechanisms including through increased vasodilative capacity. Ischemic conditioning exerts protection and appears to be a ubiquitous endogenous protective mechanism at the cellular level that has been observed in the heart of humans and every animal species tested. This protection has also been seen in organs such as the liver, kidney, gut, skeletal tissue, urinary bladder and brain. See D M Yellon and J M Downey, "Preconditioning the myocardium: from cellular physiology to clinical cardiology" *Physiol Rev* 83 (2003) 1113-1151. In fact, ischemic conditioning can have an effect on any proliferative tissue, e.g. skin, hair, and bone marrow.

**[0029]** The therapeutic and protective effects of ischemic conditioning may be mediated by signal transduction changes to tissues. With respect to cardiac tissue, the current paradigm suggests that nonlethal episodes of pre-ischemia reduce the infarct size that results from subsequent total blockage of arterial blood supply. Ischemic conditioning has been found to lead to the release of certain substances, such as adenosine and bradykinin. These substances bind to their G-protein-coupled receptors and activate kinase signal transduction cascades. These kinases converge on the mitochondria, resulting in the opening of the ATP-dependent mitochondrial potassium channel. See Garlid K D et al. "Cardioprotective effect of diazoxide and its interaction with mitochondrial ATP-sensitive K<sup>+</sup> channels. Possible mechanism of cardioprotection" *Circ Res* 81 (1997) 1072-1082. Reactive oxygen species are then released. See Vanden Hoek T L et al., "Reactive oxygen species released from mitochondria during brief hypoxia induce preconditioning in cardiomyocytes" *J Biol Chem* 273 (1998) 18092-18098. Thus, additional protective signaling kinases can be activated, such as heat shock inducing protein kinase C.

**[0030]** Further, the signaling kinases mediate the transcription of protective distal mediators and effectors, such as inducible nitric oxide synthase, manganese superoxide dismutase, heat-stress proteins and cyclo-oxygenase 2, which manifest 24-72 hours after infarction to provide late protection. Suggested mechanisms of how these signaling transduction pathways mediate protection, and ultimately reduce infarct size, include maintenance of mitochondrial ATP generation, reduced mitochondrial calcium accumulation, reduced generation of oxidative stress, attenuated apoptotic signaling and inhibition of mitochondrial permeability transition-pore (mPTP) opening. See D M Yellon and J M Downey, "Preconditioning the myocardium: from cellular physiology to clinical cardiology" *Physiol Rev* 83 (2003) 1113-1151; Yellon D M, Hausenloy D J, "Realizing the clinical potential of ischemic preconditioning and postconditioning" *Nat Clin Pract Cardiovasc Med*. 2(11)(2005) 568-75. Alternative protective mechanisms of ischemic conditioning that are independent of signal transduction pathways, such as those mediated by antioxidant and anti-inflammatory mechanisms, may provide further protection.

**[0031]** Even further, formation of vascular collaterals is also induced by ischemia and hypoxia of blood vessels. Vascular endothelial growth factor (VEGF) production can be induced in cells that are not receiving enough oxygen. When a cell is deficient in oxygen, it produces the transcription factor Hypoxia Inducible Factor (HIF). HIF stimulates the release of VEGF among other functions including modulation of erythropoiesis. Circulating VEGF then binds to VEGF receptors on endothelial cells and triggers a tyrosine kinase pathway leading to angiogenesis.

**[0032]** Ischemic conditioning has been shown to produce tolerance to reperfusion damage from subsequent ischemic damage. One physiologic reaction to local ischemia in normal individuals is reactive hyperemia to the previously ischemic tissue. Arterial occlusion results in lack of oxygen (hypoxia) as well as an increase in vasoactive metabolites (including adenosine and prostaglandins) in the tissues downstream from the occlusion. Reduction in oxygen tension in the vascular smooth muscle cells surrounding the arterioles causes relaxation and dilation of the arterioles and thereby decreases vascular resistance. When the occlusion is released, blood flow is normally elevated as a consequence of the reduced vascular resistance.

**[0033]** Perfusion of downstream tissues is further augmented by flow-mediated dilation (FMD) of larger conduit arteries, which acts to prolong the period of increased blood flow. As a consequence of the elevated blood flow induced by reactive hyperemia, downstream conduit vessels undergo luminal shear stress. Endothelial cells lining the arteries are sensitive to shear stress and the stress induces in opening of calcium-activated potassium channels and hyperpolarization of the endothelial cells with resulting calcium entry into the endothelial cells, which then activates endothelial nitric oxide synthase (eNOS). Consequent nitric oxide (NO) elaboration results in vasodilation. Endothelium-derived hyperpolarizing factor (EDHF), which is synthesized by cytochrome epoxygenases and acts through calcium-activated potassium channels, has also been implicated in flow-mediated dilation. Endothelium derived prostaglandins are also thought to be involved in flow-mediated dilation.

**[0034]** The therapeutic effects of conditioning are mediated by changes to the vasculature and/or the neurovasculature, as well as anti-inflammatory effects. Nitric oxide (NO) bioavailability may be improved locally. Nitric oxide (NO) has been shown to be involved in cutaneous active vasodilation induced by systemic application of heat on the basis that local inhibition of NO synthase results in inhibition of cutaneous local perfusion while local perfusion of the NO donor, sodium nitroprusside, results in maximum local cutaneous perfusion. See DL Kellogg Jr., C G Crandall, Y Liu, N Charkoudian, and J M Johnson. "Nitric oxide and cutaneous active vasodilation during heat stress in humans" *J Appl Physiol* 85 (1998) 824-829. Similarly, it has been found that NO mediates vasodilation in response to local application of heat. See D L Kellogg Jr., Y Liu, I F Kosiba, and D. O'Donnell. "Role of nitric oxide in the vascular effects of local warming of the skin in humans" *J Appl Physiol* 86 (1999) 1185-1190. Conversely, local cooling induces cold-sensitive afferent nerves to activate sympathetic nerves to release norepinephrine, which leads to local cutaneous vasoconstriction. J M Johnson, T C Yen, K Zhao, and W A Kosiba. "Sympathetic, sensory, and nonneuronal contributions to the cutaneous vasoconstrictor response to local cooling" *J Physiol Heart Circ Physiol* 288 (2005) H1573-H1579.

**[0035]** Ischemia Preconditioning (IPC) has been found to have remote and systemic protective effects in both human and animal models. Transient limb ischemia (3 cycles of ischemia induced by cuff inflation and deflation) on a contralateral arm provides protection against ischemia-reperfusion (inflation of a 12-cm-wide blood pressure cuff around the upper arm to a pressure of 200 mm Hg for 20 minutes) induced endothelial dysfunction in humans and reduces the extent of myocardial infarction in experimental animals (four cycles of 5 minutes occlusion followed by 5 minutes rest, immediately before occlusion of the left anterior descending (LAD) artery). (Kharbanda R K, et al. *Circulation* 106 (2002) 2881-2883). This phenomenon suggests that ischemic conditioning creates natural therapeutic substances that can have desirable systemic effects.

**[0036]** Recent evidence in a skeletal muscle model has suggested that IPC results in increased functional capillary density, prevention of ischemia/reperfusion induced increases in leukocyte rolling, adhesion, and migration, as well as up-regulation of expression of nNOS, iNOS, and eNOS mRNA in ischemia reperfusion injured tissue. (Huang S S, Wei F C, Hung L M. "Ischemic preconditioning attenuates postischemic leukocyte-endothelial cell interactions: role of nitric oxide and protein kinase C" *Circulation Journal* 70 (8) (2006) 1070-5). Research has also shown that ischemic preconditioning can result in elevations of heat shock proteins, antioxidant enzymes, Mn-superoxide dismutase and glutathione peroxidase, all of which provide protection from free radical damage. (Chen Y S et al. "Protection 'outside the box' (skeletal remote preconditioning) in rat model is triggered by free radical pathway" *J. Surg. Res.* 126 (1) (2005) 92-101).

**[0037]** Although originally described as conferring protection against myocardial damage, preconditioned tissues have been shown to result in ischemia tolerance through reduced energy requirements, altered energy metabolism, better electrolyte homeostasis and genetic reorganization, as well as reperfusion tolerance due to less reactive oxygen species and activated neutrophils released, reduced apoptosis and better microcirculatory perfusion compared to non-preconditioned tissue. (Pasupathy S and Horner-Vanniasinkam S. "Ischaemic preconditioning protects against ischaemia/reperfusion injury: emerging concepts" *Eur. J. Vasc. Endovasc. Surg.* 29 (2) (2005) 106-15).

**[0038]** As used herein the term "ischemia" means lowering of baseline blood flow to a tissue. The term "hypoxia" means lowering of arterial PO<sub>2</sub>. Both ischemia and hypoxia in extremities can be induced by occluding the blood supply upstream of the extremity. By "extremity" it is meant the limbs (arms and legs). By "distal extremity" it is meant the hands and feet, including the digits of the hands and feet. By "regional or local" it is meant, administration to a defined area of the body as contrasted with systemic administration. One embodiment of the present invention employs transient, intermittent ischemia to condition and improve the vasculature of the extremities.

**[0039]** As used herein the phrase "compounds that increase the bioavailability of nitric oxide (NO)" include NO precursors, NO donors and NO agonists. An example of a NO precursor is the essential amino acid substrate L-arginine from which NO is synthesized by the action of nitric oxide synthase (NOS). NO donors, which generate NO via NOS independent processes, include both fast and slow release compounds that typically release NO by either oxidation or

reduction. Certain of the NO donor compounds such as nitroglycerin (an organic nitrate), which is enzymatically degraded to generate NO, have been utilized for over a century. Examples of NO donors (sometimes alternatively referred to in art as NO agonists) include the organic nitrates (e.g. glyceryl trinitrate, isosorbide dinitrate), sodium nitroprusside (SNP), sydnonimines (e.g. molsidomine, SIN-1), S-nitrosothiols (e.g. s-nitrosoglutathione), NONOates (e.g. Spermine-NONOate, DETA-NONOate), and hybrid donors such as the nitroaspirins and nicorandil. Certain other compounds that are considered herein to fall within the definition of compounds that increase the bioavailability of NO are compounds, and metabolites thereof, that include nitric oxide chemical structures and are considered to be NO agonists such as for example minoxidil (3-hydroxy-2-imino-6-(1-piperidyl)pyrimidin-4-amine). Such compounds are considered herein to be NO agonists if their action is the same as NO, such as for example, in opening of membrane potassium channels.

#### Transient Ischemia for Protection Against Chronic Medical Conditions

**[0040]** In one embodiment of the present invention, intermittent transient ischemia is induced in one or more limbs, or portions thereof, of a patient. The intermittent transient ischemia stimulates and conditions the downstream vasculature and thereby prevents or reduces symptoms of the chronic medical condition.

**[0041]** In accordance with the novel indication of the present invention, in one embodiment the body's own adaptive responses to induced ischemia or hypoxia are harnessed to provide protection against chronic medical conditions such as hypertension, Raynaud's syndrome, coronary heart disease (CHD), coronary artery disease (CAD), peripheral arterial disease, diabetes, pulmonary hypertension (PH), connective tissue disorders, and other chronic diseases involving the vasculature. In accordance with the method disclosed herein, a scheduled series of transient ischemic episodes is administered. The scheduled series of transient ischemic episodes provide protection against the incidence and severity of chronic medical conditions particularly by increasing the dilative capacity in the vasculature of the limbs. Additional beneficial effects include one or more of: increased scavenging of free radicals, reduction in inflammation, and increased functional capillary density.

**[0042]** In one embodiment of the invention, transient ischemia is implemented by cuffs or straps (106) that are secured around one or more of the limbs of the patient, as depicted in FIG. 1. As shown in FIG. 1, the occlusive cuffs or straps can be placed over one or more locations for compression sufficient to occlude blood flow to the hands and/or feet. For example, for occlusion of blood supply to the hands, compression can be applied to the upper arm over the brachial artery, the lower arm over the radial and ulnar arteries, or the wrist over the radial artery. For occlusion of blood supply to the feet, compression may be applied to the upper leg over the femoral and deep femoral arteries, or to the lower leg over the tibial arteries. In one embodiment, the cuffs are inflatable and inflation results in sufficient pressure around the circumference of the limb to result in occlusion of the arterial blood supply to the limb. In one embodiment, ischemic conditioning can be administered with cuffs on both arms and both legs.

**[0043]** The duration of ischemia varies by therapeutic targets, but is typically provided for a period from about 1 to

about 20 minutes, preferably from about 2 to about 5 minutes, followed by release of the occlusion. Occlusion and release (reactive hyperemia) procedures with different occlusion times are implemented depending on individual tolerance and response to therapy as well as the planned treatment schedule such that a desired distal and/or contralateral vascular/neuro/neurovascular function is obtained. Repeated cuff occlusion and release is tailored to improve vasoreactivity (increasing the vasodilative capacity) including by improving nitric oxide bioavailability (reducing destruction or increasing production). This effect can be seen in the same distal extremity as the cuff inflation but is also expected to have neurovascular mediated systemic vasodilation as well.

**[0044]** In one embodiment of the invention, a programmable cuff inflation and deflation device is employed to provide intermittent scheduled transient ischemia. The device can inflate one or more cuffs on one or more body parts at a time. The method induces reactive hyperemia and can mimic the effects of local exercise. The larger the area of ischemia the higher the hyperemia.

**[0045]** A portable form of the device is implemented for ambulatory use such as the embodiment depicted in part in FIG. 2. In the embodiment depicted in FIG. 2, one or more occlusive cuffs (106) are in electrical connection via cable (110) with programmable monitor (102) which may be worn anywhere on the body, such as for example on a waist band as depicted. The inclusive cuff can be inflated by an electric pump associated with the programmable monitor, which also can be adapted to record the pattern of occlusion. Alternatively, the cuff(s) can be manually inflated at intervals. In one embodiment, the cuff(s) are manually inflated in response to a signal given by a programmable monitor that instructs inflation and deflation of the inflatable cuff(s). In another embodiment, the monitor instructs manual tightening and loosening of one or more straps in accordance with a programmed schedule.

**[0046]** The duration of ischemia may not have a linear relationship with the effect. After 30 minutes the hyperemia plateaus and the biochemical imprint changes. Desired therapeutic effects are more expected in the first 20 minutes after which the potential harm from the ischemia would have to be weighed against benefits obtained by diminishing chronic complications. In an embodiment, by scheduling separate ischemic conditioning treatments apart from each other in a day (e.g. 3 times a day) can provide maximum therapeutic effect. In an embodiment, conducting ischemic conditioning treatments frequently over extended periods of time (e.g. a day, month, or year) can enhance therapeutic effect. In an embodiment, adjustments to ischemic conditioning regimens can be administered based on assessments of treatment resistance over a period of time and thereby customized to achieve optimal responsiveness in the individual patient. Longitudinal measurement of blood pressure provides a measure of efficacy in the treatment of hypertension.

**[0047]** In one embodiment of the invention, vascular and/or neurovascular and/or peripheral nerve function is determined on a distal extremity to aid in diagnosis, determination of progression and/or management of medical conditions as well as use in assessing the status of the preventive and remedial therapies disclosed herein. In one embodiment, vascular and/or neurovascular function is determined by measuring the vascular or neurovascular response induced by transient blood flow occlusion in the vasculature leading to a distal extremity. Vascular or neurovascular reactivity can be

monitored by any one of several methods that detect blood flow differences in response to transient blood flow occlusion including inherent skin temperature, clearance of induced skin temperature, tonometry, Doppler ultrasound, laser Doppler flowmetry (such as by a laser Doppler perfusion imaging (LDPI) instrument), plethysmography, iontophoresis, capillometry, and/or changes in magnetic or electromagnetic properties of the tissue.

**[0048]** Inherent skin temperature means the unaltered temperature of the skin. This is in contrast to an induced skin temperature measurement which measures perfusion by clearance or wash-out of heat induced on the skin. Various methods of recording of inherent skin temperature on a finger tip or palm distal to an occlusive cuff are disclosed in Naghavi et al., U.S. application Ser. No. 11/563,676 and PCT/US2005/018437 (published as WO2005/118516). The combination of occlusive means and skin temperature monitoring for determination of vascular reactivity has been termed Digital Temperature Monitoring (DTM) by certain of the present inventors. In one standard utilization, DTM employs a standard arm-cuff vascular reactivity procedure, which includes a temporary occlusion of blood flow in the arm. During the cuff occlusion, the lack of blood flow (ischemia) elicits a microvascular dilative response (opening small vessels). Upon releasing the cuff, blood flow rushes into the forearm and hand, not only restoring baseline flow but also resulting in an overshoot (reactive hyperemia). This overshoot causes shear stress in the larger (conduit) arteries, which stimulates these arteries (macro vessels) to dilate and accommodate the increased blood flow.

**[0049]** A sensitive fingertip temperature sensor monitors, records, and analyzes fingertip temperature during the above cuff occlusion and release procedure. Temperature changes serve as a surrogate marker of blood flow changes that result from vascular reactivity. In one embodiment of the DTM procedure, an automated procedure is initiated beginning with an automated blood pressure measurement, followed by cuff occlusion of the right arm. During the cuff occlusion (2 to 5 minutes), fingertip temperature in the right hand falls because of the absence of warm circulating blood. Once the cuff is released, blood flow rushes into the forearm and hand, causing a temperature rebound (TR) in the fingertip which is directly proportional to the vascular reactivity. The higher the temperature rebound (TR), the better the vascular reactivity.

**[0050]** FIGS. 2 and 3a depict use of fingertip monitor (104) in conjunction with a blood flow occlusive device (106) located on an upper or lower extremity. In the depicted embodiment of FIG. 3a, the fingertip monitor is a DTM that monitors fingertip temperature in conjunction with induced reactive hyperemia in order to provide a surrogate marker of vascular reactivity as a result of repeated ischemic conditioning. In the depicted embodiment of FIG. 3b, an artificial pulse generator (2) is included to provide an artificial pulse and fingertip monitor (104) is, or includes, a pulse oximeter. In one embodiment the pulse generator (2) effects mechanical actuation by pulsating fluid pressure in a cuff to cause mechanical disturbance of arterial blood. In other versions, repetitive, external electromechanical actuation provides the artificial pulse. In still other versions, the artificial pulse is generated by external non-mechanical optical illumination utilized to imitate the absorption patterns of a pulsatile blood flow signal by oscillating the intensity of a light source of either a single or multiple wave length. The optional extremity mounted monitor (102) is adapted to display one or more

of program parameters, ambient temperature, blood pressure, DTM parameters of fingertip temperature over time, and pulse oximetry data.

**[0051]** In one embodiment, the method for monitoring the vascular or neurovascular response further includes simultaneously measuring and recording additional physiologic parameters including pulse rate, blood pressure, galvanic response, sweating, core temperature, and/or skin temperature on a thoracic or truncal (abdominal) part.

**[0052]** In one alternative embodiment, local ischemia of the superficial skin layers is provided by an inflatable mitten, sock or glove that operates to provide compression against the skin and thus restrict normal blood flow to the superficial tissues. As with ischemia induced by blockage of blood flow by compression over an artery such as by inflation of a blood pressure cuff, the induction of superficial pressure can be implemented according to a schedule of transient induced pressure as the treatment or conditioning requires. Several other embodiments for inflatable compression are possible such as for example a full body suit that can be used to provide ischemia to the superficial skin layers.

#### Prevention and Treatment of Hypertension

**[0053]** Chronic medical conditions have various degrees of severity in different individuals including periods of partial remission and recrudescence. However, because each condition cannot be predicted and has variations for different patients, the ischemic conditioning therapy of the present invention can be modified to suit the unique parameters for the particular condition and patient. The present method of administering one or more transient ischemic episodes to one or more limbs according to a schedule is neither dangerous nor expensive and may be readily implemented in every patient. In one embodiment, cuffs are placed on both arms and legs for ischemic conditioning in the treatment of hypertension. The device can be implemented for either in-patient or, preferably, outpatient treatment. The transient ischemic episodes provide protection and treatment against chronic medical conditions by several mechanisms including without limitation: increased nitric oxide bioavailability, increased scavenging of free radicals and reduction of inflammation. If administered in a series of episodes over a sufficiently amount of time, the method is expected to increase vasodilative capacity including by increased arterial and smooth muscle flexibility, as well as increases in functional capillary density, and may be further expected to hasten wound healing.

**[0054]** In an embodiment of the invention, a scheduled series of transient ischemic episodes is applied as conditioning to prevent or manage chronic hypertension. Of the numerous compounds that are released following an ischemic episode as described herein, several are known to have anti-hypertensive effects. For example, increases in nitric oxide and adenosine bioavailability are known to occur after an ischemic episode. These compounds are frequently targeted by drug therapies and are well known to relax smooth muscle cells, decrease arterial stiffness, and improve hypertension over time.

**[0055]** In an embodiment, episodes of transient ischemic conditioning are employed to improve monitoring of stages of hypertension by vascular reactivity measurements. For example, since healthy individuals are expected to have an increase in vascular reactivity by vasodilation upon an ischemic episode, healthy patients can show a decrease in blood pressure following ischemic conditioning. Hyperten-

sive patients can be expected to have limited vasodilation capacity and thus have unchanged or even increased blood pressure after an ischemic conditioning treatment. In an embodiment, any vascular reactivity measurement that is suitable for the methods described herein can be used to determine stages of hypertension by ischemic conditioning. In an embodiment, utilizing ischemic conditioning to characterize stages of hypertension does not significantly affect heart rate of the patient. This creates an advantage over the increased heart rate problem faced by many exercise-induced ischemic vascular reactivity measures such as treadmill stress testing. Thus, ischemic conditioning is able to simulate ischemic effects of exercise but avoid associated problems.

**[0056]** In an embodiment, other chronic medical conditions can also benefit from scheduled ischemic conditioning and the resulting increase in perfusion, relaxation of smooth muscle cells, vasodilation, and elaboration of anti-inflammatory and anti-oxidant mediators. For example, microvascular dilative capacity is hindered and inflammation is increased in Raynaud's syndrome and several associated disorders such as scleroderma (a collagen-related immune disorder) and small vessel vasculitis (including vasculitis associated with anti-neutrophil cytoplasmic antibodies, or ANCA's). Further, diabetes, insulin resistance, high blood glucose, and several other metabolic dysregulations are well known to exacerbate inflammation and oxidation. Even further, patients with chronic coronary conditions that reduce ejection fractions and perfusion can benefit from the effects of ischemic conditioning. For example, chronic coronary heart disease patients, heart failure (especially the more severely symptomatic such as in Class III and IV patients), ischemic heart, and stable angina can exhibit chest pain upon exercise which limits the capacity for physical conditions. However, these patients can receive similar benefits of exercise by episodes of ischemic conditioning. Physical conditioning the extent tolerable is expected to increase the benefits of the ischemic conditioning provided herein.

**[0057]** In an embodiment, ischemic conditioning can allow for detection and management of subclinical diabetic neuropathy. Comparing nerve conduction differences before and after an episode of ischemic conditioning can provide information about existence and amounts of nerve damage due to diabetic microvascular injury. Any suitable nerve function measurement, such as needle electromyography (EMG), can be used.

#### Intermittent Heating for Protection and Treatment

**[0058]** In an alternative embodiment, increased blood flow, enhanced metabolic activity, and anti-oxidant capability is obtained by intermittent heating of the hands and/or feet, or digits thereof. Heat is employed to shift the sympathetic-parasympathetic balance, including through the induced increase in local production of nitric oxide, in order to induce vasodilation and reduced resistance to peripheral blood flow.

**[0059]** In certain embodiments, the heat is provided by a wearable appliance that includes a heating element, a heating controller connected to the heating element, and a source of power for the heating element. As used herein, the term "wearable appliance" includes heatable inserts or pads that are dimensioned for placement in desired anatomical locations, including stand-alone appliances, appliances disposed in garments, and appliances that are used in association with a garment. Appliances that are used in association with a garment include appliances that are worn inside and those that

are worn outside of the garment. As used herein, the term "non-wearable" appliance includes fixtures and/or portable devices that are not dimensioned to be attached or carried by an individual during ambulation.

**[0060]** In certain embodiments, a wearable treatment appliance is provided that is dimensioned to be worn as mittens, socks or booties, or gloves. The heating applied must be of sufficient magnitude to cause vasodilation. The optimal site for heating, as well as the intensity and duration of heating, can be readily determined for a given individual based on whether or not the desired vasodilation is obtained.

**[0061]** In one embodiment, local administration of heat is chronic, regular or periodic for a period prior to episodes of ischemic conditioning. For example, the individual patient may schedule a pattern of heating, such as for limited periods 2-10 times a day for a period preceding each round of ischemic conditioning. In another embodiment, heat is administered to the future site for a period prior to ischemic conditioning. Depending on responses desired and obtained in the individual patient, the intensity and duration of heat can be tuned for optimal responses.

**[0062]** In one embodiment of the invention, the heating is provided by Far Infrared Radiation (FIR). FIR is centered around a wavelength of 100  $\mu\text{m}$  on the electromagnetic spectrum. Commercially available versions of such elements able to provide heat to subcutaneous tissue include, for example, FIR Radiant Heating elements. (Challenge Carbon Technology Co., Taiwan). Such elements are suited for FIR heated clothing due to their flat form and foldable, durable and washable properties. The elements as provided for use in clothing include lithium-ion batteries, temperature controller and OCP (Over-Charge Protector) integrated in one controller that provides for rapid heat up according to set upper levels.

#### Combination Therapies

**[0063]** In one embodiment of the invention, at least one ischemic conditioning treatment of induced ischemia or hypoxia and/or application of heat is combined with pharmacotherapy including by administration of an anti-hypertensive agent, vasodilating agent, anti-oxidant, and/or anti-inflammatory agent. Multiple compounds are known in each of these categories. Existing vasodilators include for example hydralazine, ACE inhibitors (such as for example enalapril), alpha-beta blockers (such as for example carvedilol), minoxidil, and calcium channel blockers (such as for example nisoldipine, nifedipine, diltiazem and verapamil). New vasodilators such as, for example, oxdrilazine are being developed and may be equally suitable. Pharmacotherapy includes agents that increase the local bioavailability of NO. The pharmacotherapy can be administered systemically or locally, such as by iontophoresis.

**[0064]** In another embodiment, at least one ischemia conditioning treatment of induced ischemia or hypoxia, and/or application of heat, is combined with non-pharmacologic techniques for modulating the autonomic nervous system (ANS), mostly for regional and transient modulation based on anatomical reflex zones. These non-pharmacologic techniques may include non-invasive electric, magnetic, or electromagnetic neuromodulating devices used to increase local ANS activity. In another embodiment, transient intermittent

ischemia and or heating is combined with hand exercises to increase demand and thereby improve nitric oxide bioavailability in the target areas.

#### Improving Metabolic Endurance and Athletic Performance

**[0065]** In one embodiment of the invention, metabolic endurance and athletic performance can be improved by repeated, scheduled ischemic conditioning treatments. Such treatments provide a natural stimulus for the metabolic machinery (mitochondrial activity, intracellular genes, mRNA, proteins) of the ischemic tissue to better adapt itself to anaerobic conditions, such as those encountered during prolonged exercise and continuous, strenuous activity. Repeated ischemic conditioning treatments are expected to induce metabolic changes and adaptation similar to that induced by exercise conditioning. Ischemic conditioning modulates the supply component, whereas exercise conditioning modulates the demand component. The intracellular metabolic machinery responds to the balance between supply and demand for oxygen and other required nutrients. A decrease in supply (ischemia) or an increase in demand (exercise) will trigger a similar response.

#### Artificial Pulse Oximetry

**[0066]** Pulse oximetry is a non-invasive method allowing the monitoring of the oxygenation of a patient's hemoglobin. A sensor is placed on a thin part of the patient's anatomy, usually a fingertip or earlobe, and a light containing both red and infrared wavelengths is passed from one side to the other. Changing absorbance of each of the two wavelengths is measured, allowing determination of the absorbances due to the pulsing blood. Based upon the ratio of changing absorbance of the red and infrared light caused by the difference in color between oxygen-bound (bright red) and oxygen unbound (dark red or blue, in severe cases) blood hemoglobin, a measure of oxygenation (the percent of hemoglobin molecules bound with oxygen molecules) can be made.

**[0067]** During naturally occurring pulsatile blood flow, only arterial blood flow is primarily pulsatile, while the venous flow is relatively steady and constant due to the pressure loss across the capillary bed. Existing methods of pulse oximetry require a naturally occurring pulsatile signal in order to function. Standard pulse oximetry will not function correctly in the absence of pulsatile blood flow or during low perfusion states, such as during surgery, hypovolemic shock, cardiogenic shock, septic shock, etc. Thus, accurate measurement of oxygenation cannot be obtained using pulse oximetry under low or no flow conditions.

**[0068]** During pulsation induced by artificial external or internal actuation as disclosed herein, both the arterial and venous blood are caused to have oscillatory displacement. As a result, the disclosed method of pulse oximetry using artificial pulsation provides accurate measurement of tissue oxygenation and thus the monitoring of local ischemia in critical low flow conditions.

**[0069]** Measurement of blood oxygenation using artificial pulsation is more representative of tissue oxygenation because the artificial pulsation created by external or internal mechanical actuation causes blood movement in both the arterial and venous vessels. This measurement of blood oxygenation is useful in clinical conditions in which monitoring local tissue oxygenation is desirable. These clinical conditions include the monitoring of skin wounds.

**[0070]** In one embodiment of the invention, artificial pulse oximetry can be used to measure oxygen saturation of blood hemoglobin (% SpO<sub>2</sub>) in the absence of naturally occurring pulsatile blood flow (e.g., surgery with heart bypass pump, circulatory shock, occlusive arterial disorders, etc.) in humans and animals. Artificial pulses can simulate natural pulsatile blood flow in order to enable pulse oximetry devices to calculate arterial and capillary oxygen saturation. This method may also use physiological signals detected by devices such as electrocardiograms to simulate the natural pulsatile rhythm.

**[0071]** In one embodiment, the artificial pulsatile signals are generated by either external mechanical actuation that causes oscillatory displacement of blood or external non-mechanical optical illumination. Methods of generating an artificial pulsatile signal include, but are not limited to, the following:

**[0072]** Pulsating fluid pressure in a cuff to cause mechanical disturbance of arterial blood.

**[0073]** Repetitive, external electromechanical actuation

**[0074]** Repetitive, self-induced physical motion

**[0075]** Optical illumination to imitate the absorption patterns of a pulsatile blood flow signal by oscillating the intensity of a light source (single or multiple wave length).

**[0076]** In other embodiments, the artificial pulsatile signals are generated by internal mechanical actuation or internal non-mechanical optical illumination, and these methods include, but are not limited to, the following:

**[0077]** Repetitive, internal electromechanical actuation that causes mechanical disturbance of arterial blood.

**[0078]** Repetitive, internal balloon inflation and deflation

**[0079]** Optical illumination can be utilized to imitate the absorption patterns of a pulsatile blood flow signal by oscillating the intensity of a light source (single or multiple wave length).

**[0080]** FIG. 4a depicts a conventional finger pulse oximeter (1) and reflectance oximeter (6) sensor. A finger cuff (2) is placed on the proximal section of the finger and its pressure is increased to supra-systolic by monitoring when the pulse oximeter loses signal. Once at this supra-systolic level, its pressure is oscillated via the fluid tube (5) to create an artificial flow in the distal portion of the fingertip. This flow is detected by the pulse oximeter and reported to an interpreting device (8) which displays the saturated oxygen during an occluded or low flow state.

**[0081]** FIG. 4b depicts a method that involves using external optical illumination (7) to imitate the absorption patterns of pulsatile blood. The pulse oximeter sensor (6) is able to detect this pulsatile fluctuation in light intensity and report saturated oxygen in a low or no flow state. FIG. 4c depicts an embodiment of the external illumination source (7) that takes its input (8) from an external physiological signal detector such as the ECG device (9) in FIG. 4d. The ECG electrodes (10) attain the patient's heart rate, for example, and send an output signal (12) to the light source or any electromechanical actuator. FIG. 4e depicts an embodiment of the device that uses an external electromechanical actuator (11) to cause oscillatory displacement of blood in the underlying blood vessels. These oscillations are detected by the SpO<sub>2</sub> sensor (1) and reported during a low or no flow state.

**[0082]** FIG. 5a shows actual pulse oximetry data collected with a Nonin OEM III module. During the reperfusion peri-

ods, the module reports accurate values of oxygen saturation between 95% and 100%. However, during the cuff occlusion periods where arterial pulsation is not present due to lack of blood flow, the module reports an error value of 127% which is reported only when oxygen saturation cannot be computed by the module.

**[0083]** FIG. 5b shows actual pulse oximetry data collected with the same Nonin OEM III module as in FIG. 5a but with artificial pulsation provided during the cuff occlusion period. Similar to that of FIG. 5a, during the reperfusion periods the module reports accurate values for oxygen saturation between 95% and 100%. During the cuff occlusion periods, however, artificial pulsation was used to simulate blood flow in the occluded arteries. As a result of the artificial pulsation, the Nonin module was able to calculate and report actual values of oxygen saturation. As seen in the figures, the oxygen saturation for the occluded tissue continuously dropped during the five minute occlusion period. The error value of 127% was not reported for these periods.

**[0084]** FIG. 6a shows a portion of the pulse waveform collected during the reperfusion section shown in FIG. 5a. FIG. 6b shows a portion of the artificial pulse waveform recorded during the cuff occlusion portion of the test case shown in FIG. 5b.

**[0085]** In another embodiment, this method can also be used with existing pulse oximetry sensors during conditions of low pulse amplitude or non-pulsatile flow by programming the device to initiate artificial pulsations whenever pulsatile blood flow is absent. The artificial pulsations will create an interpretable signal and allow the pulse oximetry device to continue to measure blood oxygen saturation.

**[0086]** Although particular embodiments of the present invention have been shown and described, it should be understood that the above discussion is not intended to limit the present invention to these embodiments. One skilled in the art will readily appreciate that various changes and modifications may be made without departing from the spirit and scope of the present invention. Thus, the present invention is intended to cover alternatives, modifications, and equivalents that may fall within the spirit and scope of the present invention as defined by the claims.

We claim:

1. A method for modulating a vascular condition by administering a program of ischemic conditioning.

2. The method of claim 1, wherein the program of ischemic conditioning comprises at least 1 cycle of from 1 to 20 minutes of occlusion on at least one extremity, at least 2-4 times per week.

3. The method of claim 2, wherein the program of ischemic conditioning comprises at least 1 cycle of from about 2 to about 5 minutes of occlusion.

4. The method of claim 2, wherein the program of ischemic conditioning comprises plurality of cycles of occlusion followed by release according to a schedule implemented to maximize lowering of blood pressure in an individual patient.

5. The method of claim 1 wherein the program of ischemic conditioning comprises at least 2 cycles of about 2 to about 5 minutes of occlusion followed by about 2 to about 5 minutes of release of an extremity at least 2-4 times per week.

6. The method of claim 1, wherein the vascular condition is selected from the group consisting of: hypertension, Raynaud's syndrome, coronary heart disease (CHD), coro-

nary artery disease (CAD), peripheral arterial disease (PAD), diabetes, pulmonary hypertension (PH), and connective tissue disorders.

7. A method of claim 1, wherein the vascular condition is a starting vascular condition of an athlete and the program of ischemic conditioning is administered on a repeated, scheduled basis adapted to improved endurance and athletic performance.

8. The method of claim 1, wherein the ischemic conditioning is applied to one or more extremities using an external cuff system for arterial occlusion.

9. The method of claim 1, wherein the ischemic conditioning is applied to one or more extremities using external pressure to the skin using a pressurizable garment.

10. The method of claim 1, further comprising measurement of blood oxygen saturation during ischemia using artificial pulse together with oximetry to improve the ischemic conditioning treatments.

11. The method of claim 10, wherein the artificial pulse is generated by mechanical actuation.

12. The method of claim 11, wherein the mechanical actuation is effected by pulsating fluid pressure in a cuff to cause mechanical disturbance of arterial blood, repetitive, external electromechanical actuation, or repetitive, self-induced physical motion.

13. The method of claim 10, wherein the artificial pulse is generated by external non-mechanical optical illumination utilized to imitate an absorption pattern of a pulsatile blood flow signal by oscillating an intensity of a light source of either a single or multiple wave length.

14. A method for assessing an ischemic conditioning treatment comprising:

measuring one or more baseline hemodynamic parameters of a patient,

applying an ischemic conditioning treatment in the patient by occluding and releasing arterial flow in one or more extremities of the patient on a scheduled, repeated basis, measuring post-ischemia parameters in the patient, and comparing the baseline and post-ischemia parameters to provide an assessment of the ischemic conditioning treatment over time.

15. The method of claim 14, further comprising measuring blood oxygen saturation during ischemia using an artificial pulse together with oximetry to improve assessment of the ischemic conditioning treatments.

16. The method of claim 15, wherein the artificial pulse is generated by mechanical actuation.

17. The method of claim 16, wherein the mechanical actuation is effected by pulsating fluid pressure in a cuff to cause mechanical disturbance of arterial blood, repetitive, external electromechanical actuation, or repetitive, self-induced physical motion.

18. The method of claim 15, wherein the artificial pulse is generated by external non-mechanical optical illumination utilized to imitate the absorption patterns of a pulsatile blood flow signal by oscillating the intensity of a light source of either a single or multiple wave length.

19. The method of claim 14, wherein the treatment is for a condition selected from the group consisting of: hypertension, pulmonary hypertension (PH), Raynaud's syndrome, coronary heart disease (CHD), coronary artery disease (CAD), peripheral arterial disease (PAD), diabetes, and connective tissue disorders.

**20.** A device for monitoring blood oxygenation during periods of absent or low pulsatile blood flow comprising:

a pulse oximeter, and  
an artificial pulse generator, wherein the pulse oximeter is adapted to measure blood oxygenation in an artificial pulse created by the artificial pulse generator.

**21.** The device of claim **20**, wherein the artificial pulse is generated by mechanical actuation.

**22.** The device of claim **21**, wherein the mechanical actuation is effected by pulsating fluid pressure in a cuff to cause

mechanical disturbance of arterial blood, repetitive, external electromechanical actuation, or repetitive, self-induced physical motion.

**23.** The device of claim **20** wherein the artificial pulse is generated by external non-mechanical optical illumination utilized to imitate the absorption patterns of a pulsatile blood flow signal by oscillating the intensity of a light source of either a single or multiple wave length.

\* \* \* \* \*

专利名称(译)	用于高血压和其他医学病症的重复缺血性调理治疗的方法和装置		
公开(公告)号	<a href="#">US20090287069A1</a>	公开(公告)日	2009-11-19
申请号	US12/511976	申请日	2009-07-29
[标]申请(专利权)人(译)	IC THERAPEUTICS		
申请(专利权)人(译)	IC THERAPEUTICS		
当前申请(专利权)人(译)	IC THERAPEUTICS		
[标]发明人	NAGHAVI MORTEZA YEN ALBERT ANDREW HASSAN HAIDER PANTHAGANI DAVID		
发明人	NAGHAVI, MORTEZA YEN, ALBERT ANDREW HASSAN, HAIDER PANTHAGANI, DAVID		
IPC分类号	A61B5/145 A61B17/135 A61B5/00		
CPC分类号	A61B5/01 A61B5/022 A61B17/1355 A61B5/417 A61B17/135 A61B5/1455		
优先权	61/188043 2008-08-06 US 60/989946 2007-11-25 US		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

提供了用于慢性疾病的缺血性调理治疗的方法。测量患有慢性疾病的患者的基线疾病相关参数。通过阻塞和释放患者的一个或多个肢体中的动脉血流在患者中诱导缺血。测量患者的缺血后参数。比较基线和缺血后参数以提供对慢性疾病的缺血性调理治疗的评估。重复的，预定的缺血性调理递送为慢性疾病提供了有益的治疗效果。还提供了一种用于脉搏血氧测定的装置，其在缺失或低脉动血流期间包括人工脉冲发生器以及所述装置在评估缺血性调节中的用途。

