



US006595918B2

(12) **United States Patent**
Gopinathan et al.

(10) **Patent No.:** **US 6,595,918 B2**
(45) **Date of Patent:** ***Jul. 22, 2003**

- (54) **TELE-DIAGNOSTIC DEVICE**
- (75) Inventors: **Govindan Gopinathan**, Oradell, NJ (US); **Arthur R. Tilford**, Yorba Linda, CA (US)
- (73) Assignee: **inneedmd.com**, Great Neck, NY (US)
- (*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

- (21) Appl. No.: **09/884,371**
- (22) Filed: **Jun. 19, 2001**
- (65) **Prior Publication Data**
US 2001/0056227 A1 Dec. 27, 2001

Related U.S. Application Data

- (63) Continuation of application No. 09/188,971, filed on Nov. 10, 1998, now Pat. No. 6,248,064, which is a continuation-in-part of application No. 09/084,647, filed on May 26, 1998, now Pat. No. 6,224,548.
- (51) **Int. Cl.⁷** **A61B 5/00**
- (52) **U.S. Cl.** **600/300; 600/301; 600/309; 600/323; 600/485; 600/500; 600/503; 600/529; 600/481; 600/538; 600/549; 600/561; 600/587**
- (58) **Field of Search** **600/300, 301, 600/485, 500, 503, 504, 529, 481, 309, 322, 532, 538, 549, 561, 587, 595, 508**

(56) **References Cited**
U.S. PATENT DOCUMENTS

3,888,240 A	6/1975	Reinhold, Jr. et al.
4,016,868 A	4/1977	Allison
4,230,127 A	10/1980	Larson
4,381,012 A	4/1983	Russek
4,510,939 A	4/1985	Brenman et al.


4,583,547 A	4/1986	Granek et al.
4,608,987 A	9/1986	Mills
4,662,378 A	5/1987	Thomis
4,698,848 A	10/1987	Buckley
4,709,704 A	12/1987	Lukasiewicz
4,974,607 A	12/1990	Miwa
5,007,427 A	4/1991	Suzuki et al.
5,224,479 A	7/1993	Sekine
5,353,793 A	10/1994	Bornn
5,431,170 A	7/1995	Mathews
5,442,729 A	8/1995	Kramer et al.
5,465,727 A	11/1995	Reinhold, Jr.
5,511,546 A	4/1996	Hon
5,640,953 A	6/1997	Bishop et al.
5,666,404 A	9/1997	Ciccotelli et al.
5,670,944 A	9/1997	Myllymaki
5,687,738 A	11/1997	Shapiro et al.
5,704,364 A	1/1998	Saltzstein et al.
5,730,140 A	3/1998	Fitch
5,738,104 A	4/1998	Lo et al.
5,771,001 A	6/1998	Cobb
5,771,891 A	6/1998	Gozani
5,855,550 A	1/1999	Lai et al.
5,877,675 A	3/1999	Rebstock et al.
6,022,321 A	2/2000	Amano et al.
6,217,523 B1	4/2001	Amano et al.
6,224,548 B1	5/2001	Gopinathan et al.
6,248,064 B1	6/2001	Gopinathan et al.

Primary Examiner—Robert L. Nasser
(74) *Attorney, Agent, or Firm*—Brooks & Kushman P.C.

(57) **ABSTRACT**

A system (10) for collecting a plurality of diagnostic information and transmitting the diagnostic information to a remote location (18, 20, and 22a-22e) and for providing emergency treatment. The system (10) comprises, a first member (12a) adaptable to be worn on a person's first hand and a second member (12b) adaptable to be worn on a person's second hand. The members (12a and 12b) comprise a plurality of diagnostic devices and a defibrillator device. A transmitting unit for transmitting information to, and receiving information from, a remote location is provided.

64 Claims, 6 Drawing Sheets

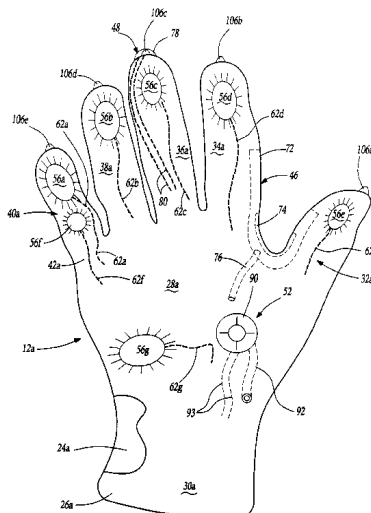

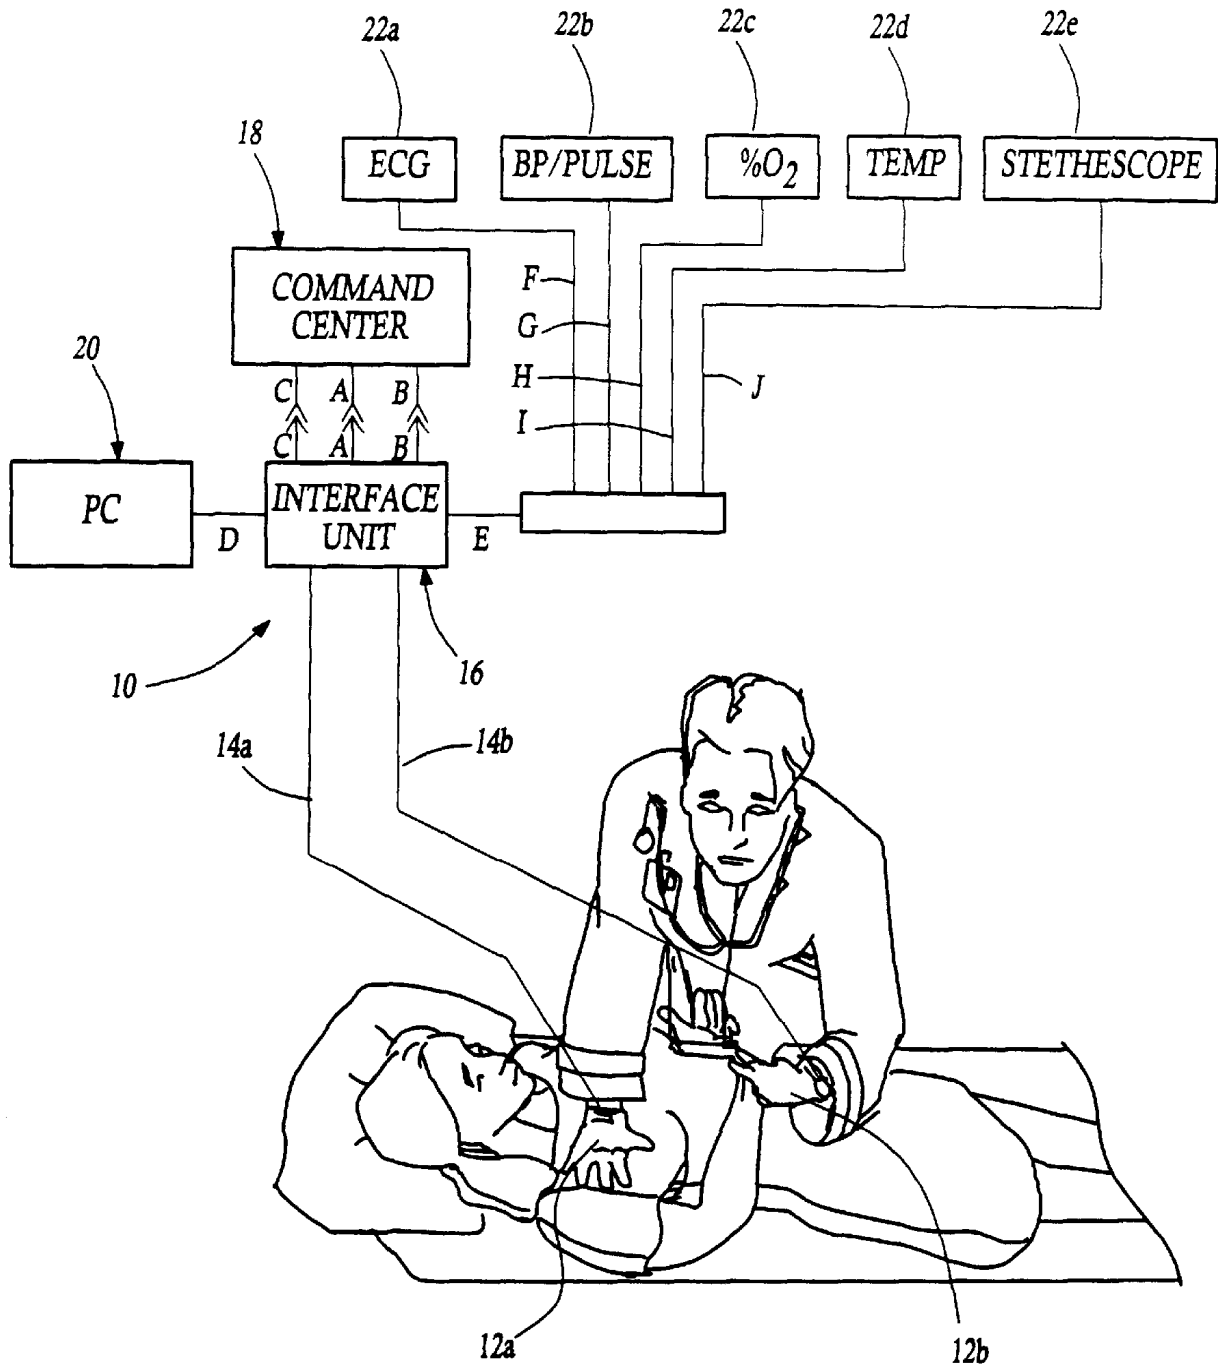


Fig-1

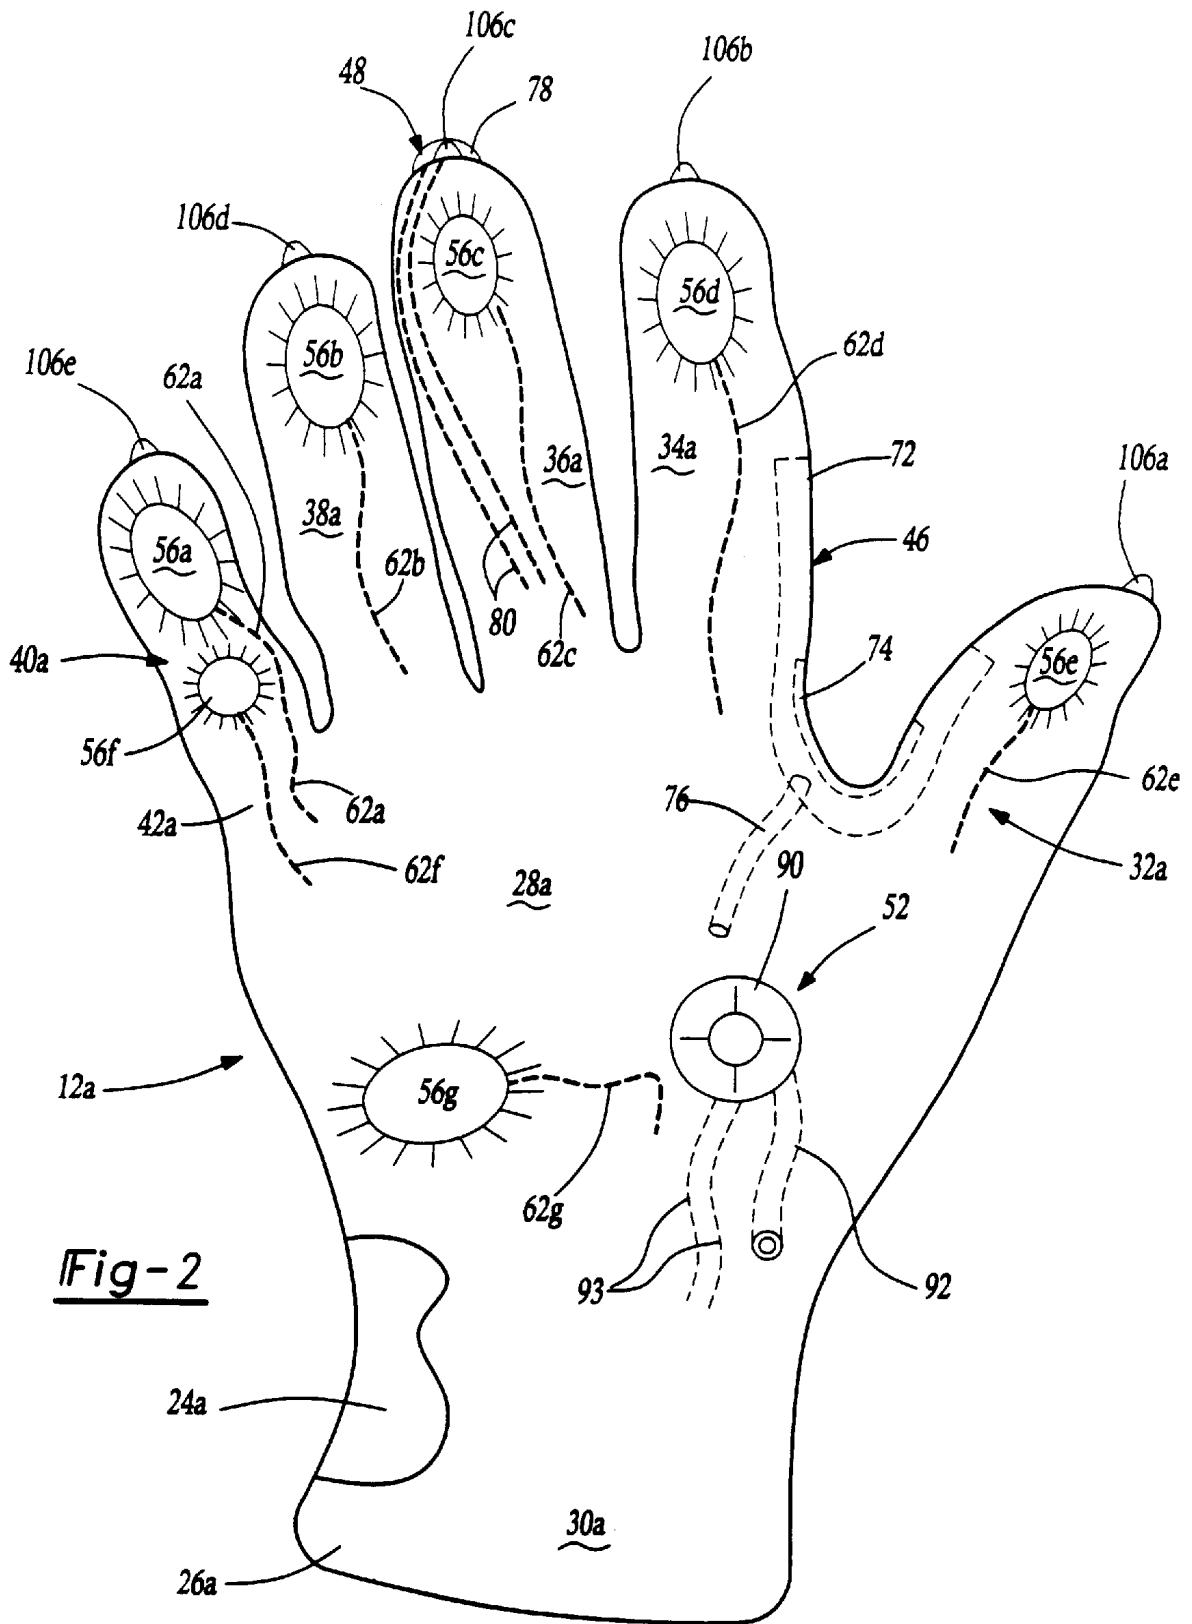


Fig-2

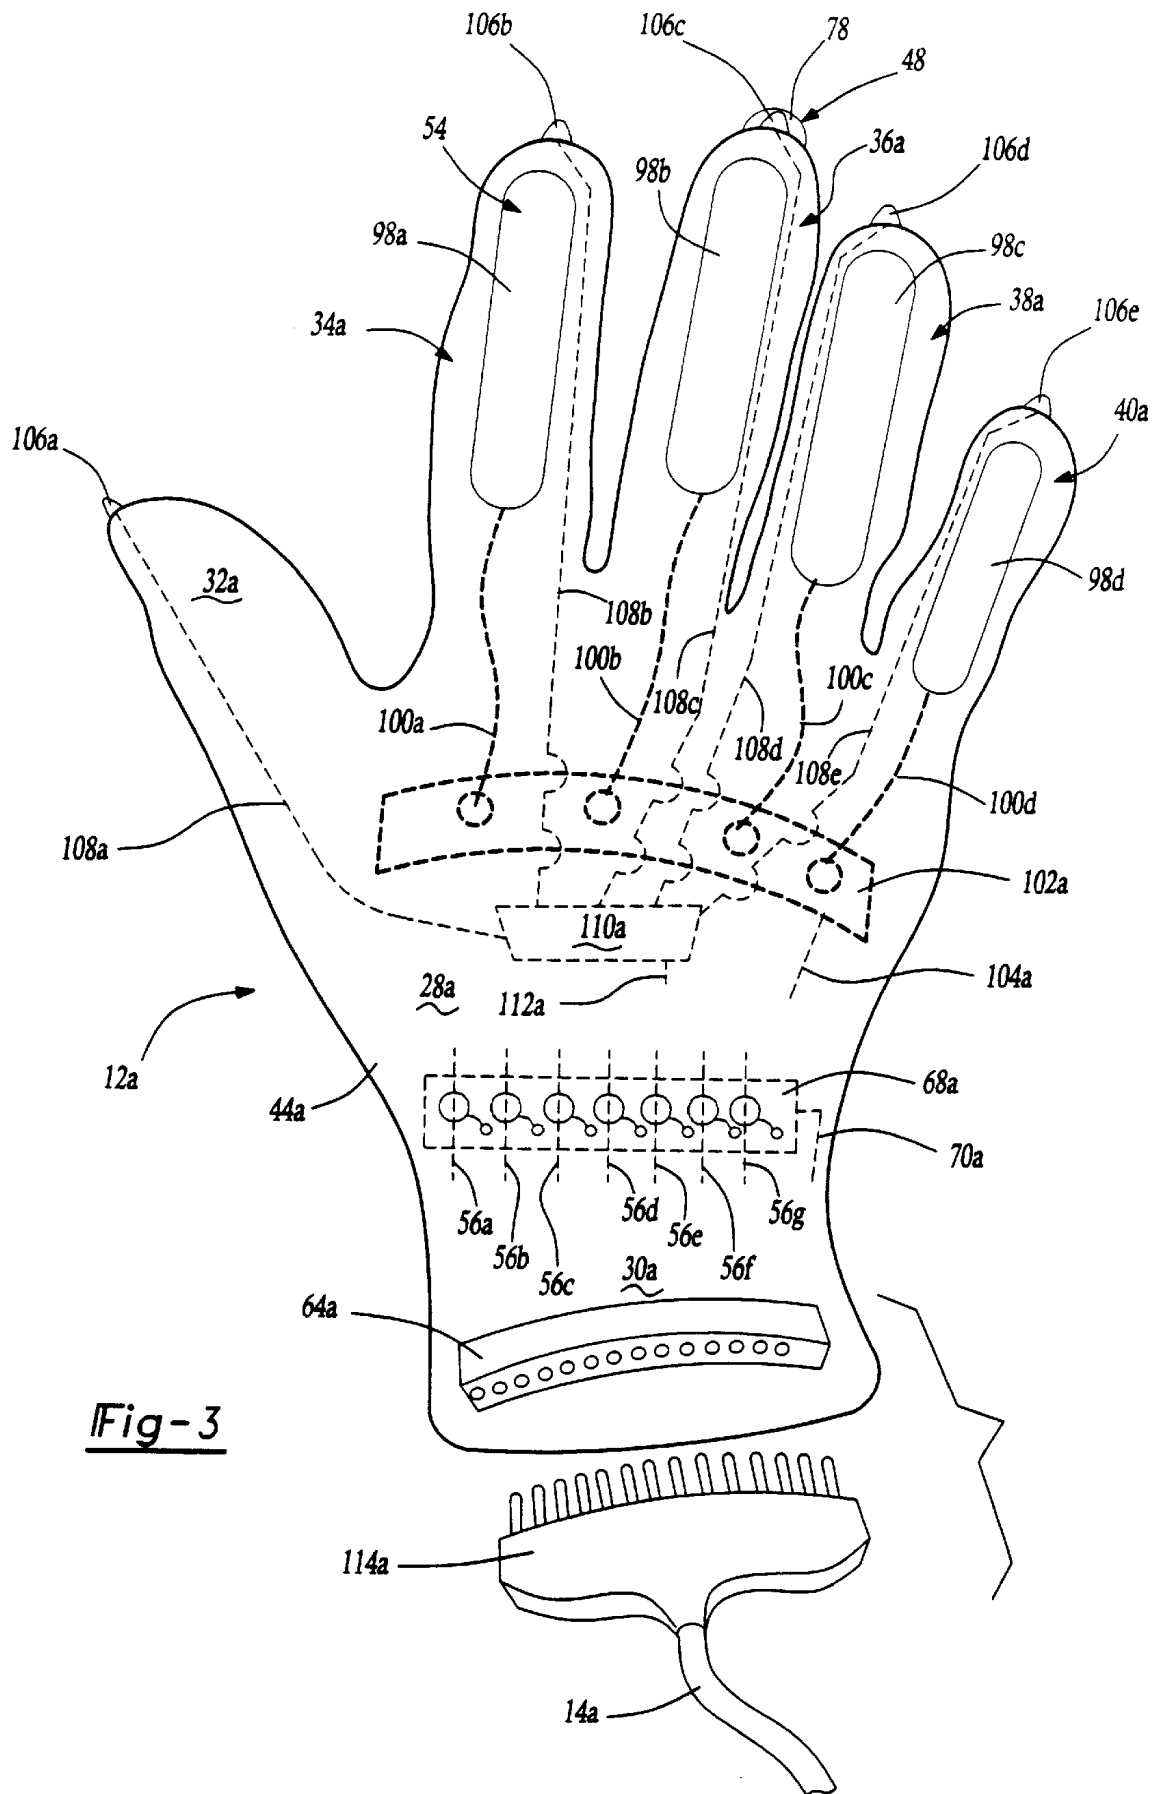


Fig-3

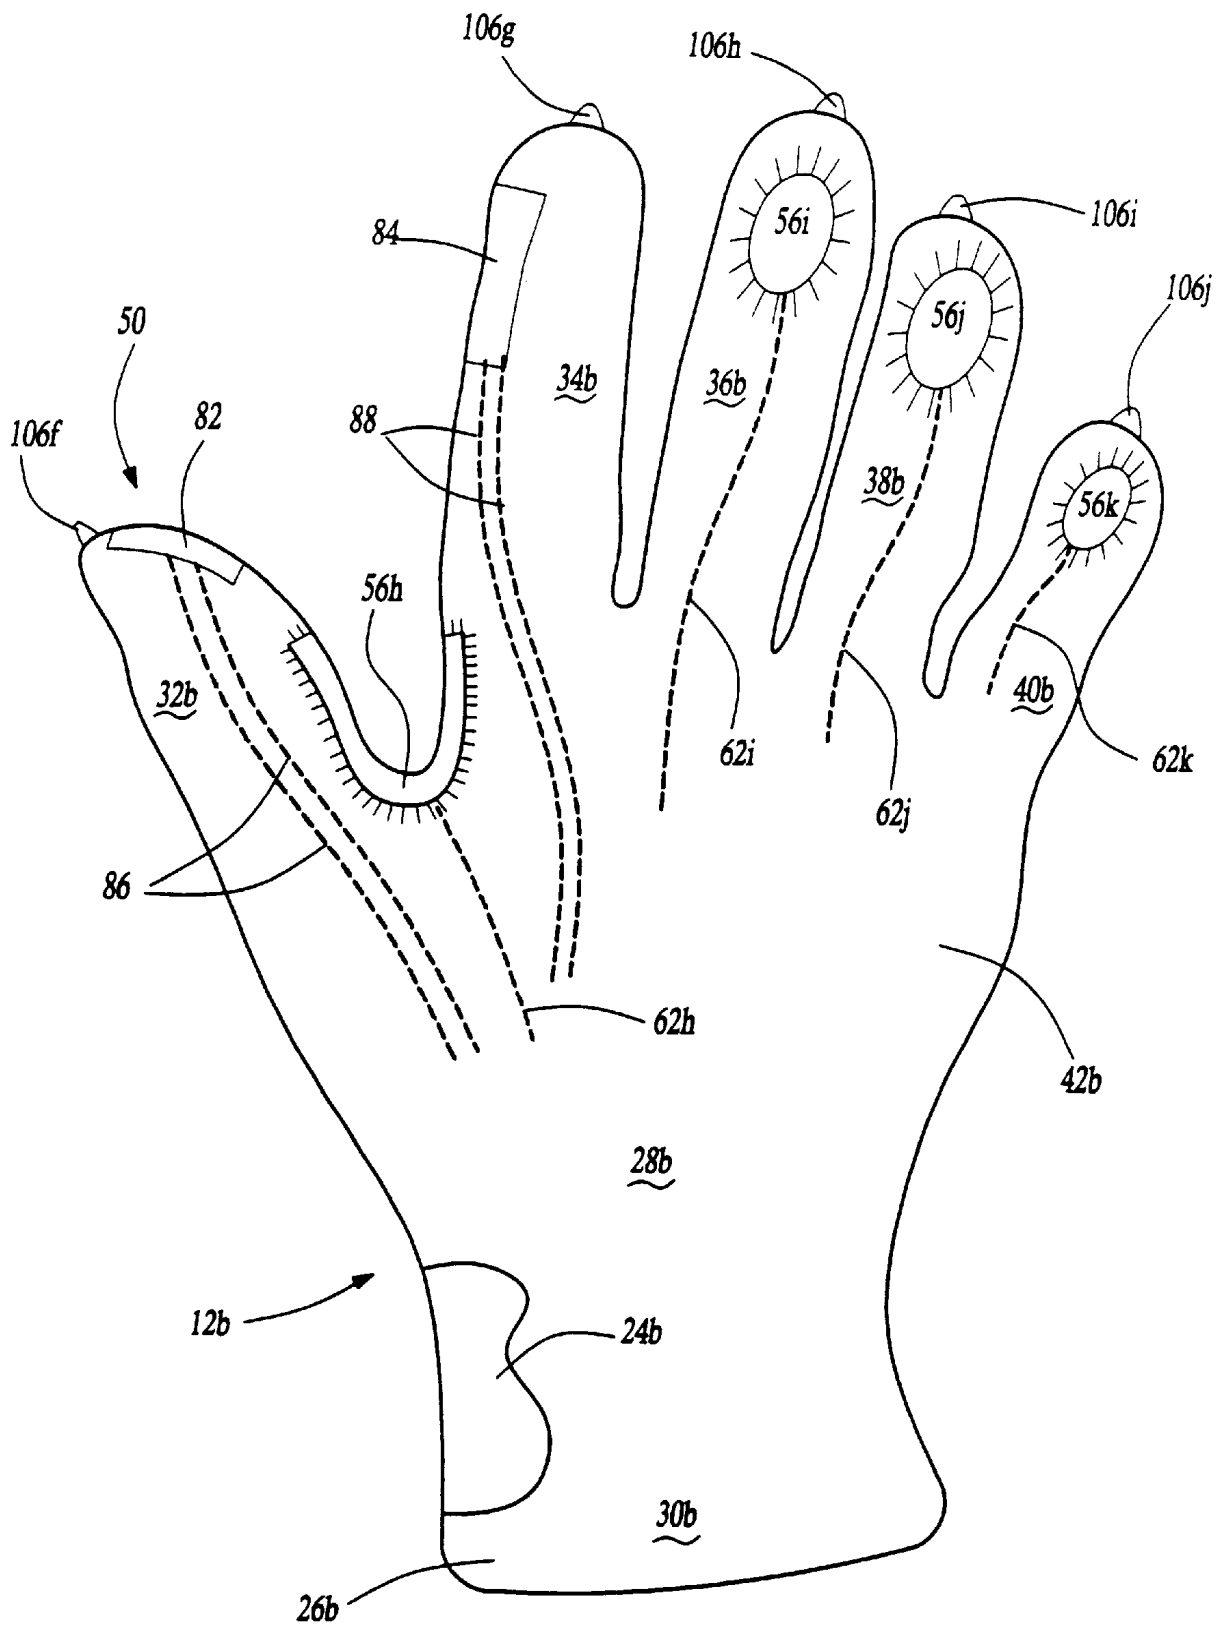


Fig-4

TELE-DIAGNOSTIC DEVICE

This application is a continuation of U.S. patent application Ser. No. 09/188,971, filed Nov. 10, 1998, now U.S. Pat. No. 6,248,064 which is a continuation-in-part of U.S. patent application Ser. No. 09/084,647, filed May 26, 1998, now U.S. Pat. No. 6,224,548, issued May 1, 2001, which are hereby incorporated by reference.

TECHNICAL FIELD

This invention relates to a system, and a device for use with the system, for obtaining a plurality of medical diagnostic information and for providing emergency treatment. In particular, the present invention relates to a system, and device for use with the system, for gathering cardiac-related diagnostic information and transmitting the information from a first, remote, location, to a second location, such as a medical monitoring command center, for providing medical management information from the first location to the second location, and for providing emergency treatment to the patient at the first location.

BACKGROUND

In a hospital setting, when a situation arises, where a person in distress (i.e., a "patient") requires emergency treatment (i.e., and "emergency"), the doctor attending the patient must first evaluate the patient and determine the cause of the emergency. To do so, the doctor typically examines the patient in a methodical manner: (i) observing the patient's appearance and actions, (ii) if the situation permits, asking the patient and/or others around the patient questions, to obtain an accurate history of the illness, and (iii) performing a number of diagnostic tests such as EKG, blood pressure, pulse, blood gas analysis etc. After conducting the examination, the doctor is able to diagnose the patient's illness and decide upon a course of action (i.e., the treatment), to alleviate the medical emergency the patient is suffering from.

However, emergencies rarely occur in a setting where a doctor is in close physical proximity to the patient. Not uncommonly, emergencies occur at remote locations. Usually a paramedic is the first medical professional to reach the patient. In addition to transporting the patient to a hospital where the patient can be treated by a doctor, the paramedic typically uses a plurality of independent medical diagnostic probes, such as a blood pressure apparatus, stethoscope, and EKG device to perform a quick evaluation of the patient. The paramedic then conveys this information to a doctor so that the doctor can (i) provide the paramedic with treatment instructions, and (ii) prepare the emergency room for the incoming patient. This routine, while being the commonly accepted practice, is somewhat inefficient in that it is relatively time consuming to manipulate all of the different diagnostic probes attached to the patient to generate vital information and accurately read the display and convey the information to the doctor. Usually this is done over a local radio transmitting system, from an ambulance.

Other emergency situations occur where the patient is in a location which is not easily accessible except to persons already in that location. Typically, such situations occur in a plane, a boat, or other remote locations like ski resorts. Often times, constraints, such as budgetary restrictions, or easy access to the location of the emergency situation, limit availability of medical diagnostic equipment. In other circumstances, lack of sufficient population does not merit satisfactory medical diagnostic facilities. If an emergency

situation occurs in a boat or plane, the vessel carrying the patient must reach a ground station so that the patient can be treated by a doctor at the base station or transported to a hospital by paramedics. In these cases, inevitably, more time passes before a doctor can evaluate the patient's medical condition and prescribe a course of action.

In most emergency situations, time is of the essence and is the key factor that determines the final outcome. As the passage of time before receiving treatment increases, the chances of successfully treating the patient decreases. Thus, it would be desirable to provide a device and system that could reduce the time element in the evaluation and treatment of the patient. Accordingly, a device and system which could reduce the time for evaluating a patient and transmitting the information gathered to a doctor would be desirable.

Also, it would be desirable to be able to provide a device and system which could be used by non-medical personnel (e.g., a flight attendant) which could enable a remotely located doctor to evaluate a patient and to provide emergency treatment without having to wait for a paramedic or caregiver to arrive.

During emergency situations, time is often expended adjusting the placement of EKG electrodes to take accurate EKG readings. Moreover, even in a non-emergency situation, it is often time consuming to correctly locate the proper placement of EKG electrodes. It would be desirable to provide a device which could be placed directly on the patient's chest and which could expedite the recording of accurate EKG tracings. It would also be desirable to provide a device which is capable of readily obtaining from the patient a plurality of diagnostic information and transmitting them in the shortest amount of time to help facilitate a doctor located far away from the patient to analyze the data and diagnose the emergency condition.

Accordingly, it would be desirable to provide an inexpensive and easy to use device which could (i) quickly and easily gather and transmit from a remote location a plurality of diagnostic information, which includes EKG, Blood Pressure, Pulse, temperature %O₂ saturation, and heart sound monitoring, (ii) provide the ability to allow oral communication with a remote location from a medical command center, (iii) provide emergency initial treatment, and (iv) expedite the eventual transfer of the patient to the nearest medical center.

It would also be desirable to provide a device and a system which could convey all the diagnostic information mentioned above, and have the capability to recognize life threatening heart irregularities and have the ability to instantaneously defibrillate a patient.

DISCLOSURE OF THE INVENTION

An object of the present invention is to provide an inexpensive and easy to use system for gathering and transmitting a plurality of diagnostic information to a remote location.

Another object is to provide an inexpensive and easy to use system for providing emergency medical treatment at a remote location.

Yet another object of the present invention is to provide an inexpensive and easy to use probe which could gather and transmit a plurality of diagnostic information to a remote location.

Yet still another object is to provide an inexpensive and easy to use device which could provide emergency medical treatment (e.g. defibrillation) at a remote location.

In carrying out the above and other objects, a system for collecting a plurality of diagnostic information and transmitting the diagnostic information to a remote location and for providing emergency treatment is provided. The system comprises a first member adaptable to be worn on a first hand of a person, a second member adaptable to be worn on a second hand of a person, and a means for transmitting information to, and receiving information from, a remote location. Each member comprises a glove member having a palm portion, a wrist portion and five phalange portions. The members further comprise an EKG diagnostic device, a blood pressure and pulse rate device, a temperature device and a defibrillator device. Also, the members could have a %O₂ device, as well as an auscultation device.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a schematic view of the system of the present invention;

FIG. 2 is a plan view of a first side of a first apparatus of the present invention;

FIG. 3 is a plan view of a second side of the first apparatus of the present invention;

FIG. 4 is a plan view of a first side of a second apparatus of the present invention;

FIG. 5 is a plan view of a second side of the second apparatus of the present invention;

FIG. 6 is a schematic diagram of the circuit of the interface unit shown in FIG. 1; and

FIG. 7 is an exploded view of an EKG sensor used in FIGS. 2-5.

BEST MODE FOR CARRYING OUT THE INVENTION

The present invention relates to a system, and a device for use with the system, for obtaining a plurality of medical diagnostic information from, and for providing emergency treatment at, a remote location. In particular, the present invention relates to a system, and diagnostic probe and emergency treatment members and an information transmission device for use with the system, for gathering cardiac related diagnostic information and transmitting the information from a remote location to another location, such as a medical monitoring command center, and for providing emergency treatment at the remote location.

As representative of the present invention, FIG. 1, illustrates a system 10 or gathering, and transmitting, from a remote location, a plurality of diagnostic information and for providing emergency treatment at the remote location. The system 10 includes a first glove member 12a and a second glove member 12b.

The first glove member 12a is adaptable to be worn over one of a person's hand. The second glove member 12b is adaptable to be worn over the other one of a person's hand. The glove members 12a and 12b include a plurality of medical diagnostic probes, which gather diagnostic signals, and emergency treatment devices, which provide emergency cardiac treatment, as will be explained in more detail below.

The glove members 12a and 12b are connected via a first cable 14a and a second cable 14b, respectively, to an interface unit 16 and, thus communicates with, and are capable of transmitting diagnostic signals, or information, from the medical diagnostic probes to the interface unit. In a preferred embodiment, the interface unit 16 communicates with a remote command center 18 via a telephone wire or fiber A, a satellite connection B, or a radio wave connection

C. The interface unit 16 can alternatively communicate with a personal computer (PC) 20 via an interface connection D. The PC 20 can be local or remote relative to the interface unit 16. The interface unit 16 may also communicate with a plurality of local or remote diagnostic readout apparatuses 22a, 22b, 22c, 22d, and 22e via a central interface connection E via a plurality of individual interface connections, F, G, H, I, and J, respectively. The diagnostic readout apparatuses 22a-e are preferably an electrocardiogram (EKG) readout; a blood pressure (BP) and pulse readout, a %O₂ oxygen readout, a temperature readout, and a stethoscope, respectively.

Referring to FIGS. 2 and 4, both the first glove member 12a and the second glove member 12b comprise a first glove layer 24a and 24b, respectfully, and a second glove layer 26a and 26b, respectively, secured to the first glove layer such that the second glove layer overlies a majority, and preferably almost all, of the first glove layer. Each of the first glove layers 24a and 24b is preferably made of a highly flexible natural or synthetic material, such as cotton flocked nitrile. Each of the second glove layers 26a and 26b is preferably made of a highly flexible material, such as nitrile.

Referring to FIG. 2, the first glove member 12a includes a palm portion 28a, a wrist portion 30a, a thumb phalange portion 32a, an index finger phalange portion 34a, a middle finger phalange portion 36a, a ring finger phalange portion 38a, and a pinky finger phalange portion 40a. The first glove member 12a further includes a palmar surface 42a (FIG. 2) and a dorsal surface 44a (FIG. 3).

Referring to FIG. 4, the second glove member 12b includes a palm portion 28b, a wrist portion 30b, a thumb phalange portion 32b, an index finger phalange portion 34b, a middle finger phalange portion 36b, a ring finger phalange portion 38b, and a pinky finger phalange portion 40b. The second glove member 12b further includes a palmar side 42b and a dorsal side 44b (FIG. 5).

As discussed previously, the glove members 12a and 12b contain a plurality of medical diagnostic devices and emergency treatment devices. In the embodiments shown in FIGS. 2-5, the glove members 12a and 12b contain an EKG diagnostic device, a blood pressure and pulse rate device 46 (FIG. 2), a temperature device 48, a %O₂ device 50 (FIG. 4), an auscultation device 52 (FIG. 2) and a defibrillator device 54 (FIGS. 3 and 5).

The EKG device is capable of measuring the EKG currents of the heart muscle and preferably includes a plurality of sensors 56a-56k located on the glove members 12a and 12b. Specifically, sensors 56a (FIG. 2), 56b, 56c, 56d, 56e, 56f, 56g are located on the first glove member 12a. Sensors 56h (FIG. 4), 56i, 56j, and 56k are located on the second glove member 12b. Sensors 56a-56g (FIG. 2) are secured to the first layer 24a of the first glove member 12a. Sensors 56h-56k (FIG. 4) are secured to the first layer 24b of the second glove member 12b. An exemplary sensor 56c is shown in FIG. 7. Each of the sensors 56a-56k preferably includes a stainless-steel screen 58 and an EKG jelly sponge 60, capable of supplying EKG conductive jelly, disposed between the screen and, preferably, the respective first layer 24a and 24b (FIGS. 2 and 4). Each sensor 56a-56k is provided on the palmar surface 42a and 42b, respectively, of one of the glove members 12a and 12b and, preferably, extends through each respective glove member so that the sensor is exposed to the environment.

More specifically, sensor 56a (FIG. 2) is positioned on the tip portion of the palmar surface 42a of the pinky finger phalange portion 40a of the first glove member 12a. Sensor

56b is positioned on the tip portion of the palmar surface **42a** of the ring finger phalange portion **38a** of the first glove member **12a**. Sensor **56c** is positioned on the tip portion of the palmar surface **42a** of the middle finger phalange portion **36a** of the first glove member **12a**. Sensor **56d** is positioned on the tip portion of the palmar surface **42a** of the index finger phalange portion **34a** of the first glove member **12a**. Sensor **56e** is positioned on the tip portion of the palmar surface **42a** of the thumb phalange portion **32a** of the first glove member **12a**. Sensor **56f** is positioned on the base portion of the palmar surface **42a** of the pinky finger phalange portion **40a** of the first glove member **12a**. Sensor **56g** is positioned on the left side, as viewed in FIG. 2, of the palmar surface **42a** of the palm portion **28a** of the first glove member **12a**.

Sensor **56h** (FIG. 4) is positioned on the palmar surface **42b** and the dorsal surface **44b** (FIG. 5) of the thumb phalange portion **32b** and the index finger phalange portion **34b** of the second glove member **12b**. The sensor **56h** extends from the base portion of the thumb phalange portion **32b** of the second glove member **12b** to the base portion of the index finger phalange portion **34b** of the second glove member. Sensor **56i** is positioned on the tip portion of the palmar surface **42b** of the middle finger phalange portion **36b** of the second glove member **12b**. Sensor **56j** is positioned on the tip portion of the palmar surface **42b** of the ring finger phalange portion **38b** of the second glove member **12b**. Sensor **56k** is positioned on the tip portion of the palmar surface **42b** of the pinky finger phalange portion **40b** of the second glove member **12b**.

Each of the sensors **56a–56g** (FIG. 2) is connected to a wire **62a–62g**, respectively, which extends between and electrically connects a respective one of the sensors **56a–56g** with a first female connection plug **64a** (FIG. 3), which is preferably provided on the dorsal surface **44a** of the first glove member **12a**. Each wire **62a–62g** is preferably disposed between the first and second layers **24a** and **26a** of the first glove member **12a**, and is preferably secured to the first layer **24a**. Each of the sensors **56h–56k** (FIG. 4) is connected to a wire **62h–62k**, respectively, which extends between and electrically connects a respective one of the sensors **56h–56k** with a second female connection plug **64b** (FIG. 5), which is preferably provided on the dorsal surface **44b** of the second glove member **12b**. Each wire **62h–62k** is preferably disposed between the first and second layers **24b** and **26b** of the second glove member **12b**, and is preferably secured to the first layer **30b**. Each wire **62a–62k** is preferably a highly flexible stranded No. 30 (or smaller) wire which is shielded and has a powdered-iron bead **66** (FIG. 7), such as Part No. T25-26 from Amidon Associates in Santa Ana, Calif., disposed adjacent to its respective sensors **56a–56k** to help prevent the detection of unwanted noise.

The first glove member **12a** includes a first ground strip **68a** (FIG. 3) which is preferably positioned on the dorsal surface **44a** of the palm portion **28a** between the first and second layers **24a** and **26a**, respectively. Each wire **62a–62g** is connected to the first ground strip **68a**, preferably, via each respective wire's shield. The first ground strip **68a** is connected to a wire **70a**, which extends between and electrically connects the first ground strip **68a** to the first female connection plug **64a**. The second glove member **12b** includes a second ground strip **68b** (FIG. 5) which is preferably positioned on the dorsal surface **44b** of the palm portion **28b** between the first and second layers **24b** and **26b**, respectively. Each wire **62i–62k** is connected to the second ground strip **68b**, preferably, via each respective wire's shield. The second ground strip **68b** is connected to a wire

70b, which extends between and electrically connects the second ground strip **68b** to the second female connection plug **64a**. The first and second ground strips **68a** and **68b**, respectively, are composed of highly flexible copper mesh or foil and function to bring existing electromagnetic forces (EMF) noise to a single electrical voltage point for removal.

The blood pressure device **46** (FIG. 2), which is capable of measuring systolic and diastolic blood pressure and pulse rate signals, is preferably secured to the first layer **24a** of the first glove member **12a** between the first layer **24a** and the second layer **26a** on the thumb phalange portion **32a** and the index finger phalange portion **34a** of the first glove member **12a**. The blood pressure device **46** preferably includes an expandable air bladder **72** defining a chamber for accommodating air or another suitable inflation fluid, an acoustical coupler **74** in the chamber and an air tube **76**. The air bladder **72** extends from the mid-portion of the thumb phalange portion **32a** of the first glove member **12a** to the mid-portion of the index finger phalange portion **34a**. The air tube **76** extends between and provides fluid and audio communication between the chamber of the air bladder **72** and the first female connection plug **64a** (FIG. 3). The acoustical coupler **74** (FIG. 2) is capable of collecting the sound waves in the air bladder **72** and directing the sound waves towards, and through, the air tube **76**. The blood pressure device **46** is preferably made of parts similar, or identical, to parts of the UB-302 Systolic/Diastolic (Pulse) Digital Blood Pressure monitor from A+D Engineering Inc., of Milpitas, Calif.

The temperature device **48** is capable of measuring temperature signals and preferably includes a thermistor **78**. The thermistor **78** is preferably positioned on the tip of the middle finger phalange portion **36a** of the first glove member **12a**. The thermistor **78** is preferably secured to the first layer **24a** of the first glove member **12a** and extends through the second layer **26a**. The temperature device **48** includes a pair of highly flexible No. 30 (or smaller) stranded and shielded wires **80** which extend between and electrically connect the thermistor **78** and the first female connection plug **64a** (FIG. 3). The temperature device **48** (FIG. 2) is preferably made of parts similar, or identical, to parts of the Cole-Parmer E-08402-00 thermometer and Generic thermistor E-08459-10 from Cole-Parmer Instrument Company of Vernon Hills, Ill.

The %O₂ device **50** (FIGS. 4 and 5) is capable of measuring the percent oxygen saturation in the blood (%O₂) signals and preferably includes a red (600–660 nm) and infra-red (880–1000 nm) LED emitter **82** and an LED (600–1000 nm) sensor **84** positioned on the second layer **26b** of the second glove member **12b**. The LED emitter **82** is preferably secured to the inner side of the thumb phalange portion **32b** of the second glove member **12b** and the LED sensor **84** is preferably secured to the side of the index finger phalange portion **34b** facing the thumb phalange portion **32b** of the second glove member **12b** such that the LED emitter **82** faces the LED sensor **84**. The LED emitter **82** is connected to a pair of highly flexible No. 30 (or smaller) stranded and shielded wires **86** which extend between and electrically connect the LED emitter and the second female connection plug **64b** (FIG. 5). The LED sensor **84** (FIG. 4) is connected to a pair of wires **88** which extend between and electrically connect the LED sensor and the second female connection plug **64b** (FIG. 5). The %O₂ device **50** (FIGS. 4 and 5) is preferably made of parts similar, or identical, to parts of the Nonin Onyx blood flow and oxygen % reader, model No. 8500M from Nonin Medical, Inc., of Plymouth, Minn.

The auscultation device **52** (FIG. 2) is capable of detecting the sound waves local to the patient's heart and lungs and preferably includes an acoustical coupler and microphone **90**, an air tube **92**, and a pair of highly flexible No. 30 (or smaller) stranded and shielded wires **93**. The acoustical coupler and microphone **90** is preferably secured to the right side of the palmar surface **42a** of the palm portion **28a** of the first glove member **12a**, preferably on the first layer **24a**. The acoustical coupler and microphone **90** is capable of collecting and amplifying sound waves which are in relative close proximity to the acoustical coupler and microphone. The air tube **92** extends between and provides audio communication between the acoustical coupler and microphone **90** and the first female connection plug **64a**, which is adaptable for connection with a stethoscope. The air tube **92**, thus when connected with a stethoscope, extends between and provides audio communication between the acoustical coupler and microphone **90** and the stethoscope. The pair of wires **93** extends between and electrically connects the acoustical coupler and microphone **90** and the first female connection plug **64a** (FIG. 3). The auscultation device **52** (FIG. 2) is preferably made of parts similar, or identical, to parts of the EG Company microphone 9445 from the Electrical Gold Co. Of Scottsdale, Ariz.

The defibrillator device **54** (FIGS. 3 and 5) is capable of providing an electrical shock to restore the rhythm of a ventrally fibrillating heart. The defibrillator device **54** includes a plurality of electrodes **98a–98h** located on the dorsal surfaces **44a** and **44b**, respectively, of the second layer **26a** and **26b**, respectively, of the first glove member **12a** and the second glove member **12b**, respectively,

More specifically, electrode **98a** (FIG. 3) is positioned on the dorsal surface **44a** of the index finger phalange portion **34a** of the first glove member **12a**. Electrode **98b** is positioned on the dorsal surface **44a** of the middle finger phalange portion **36a** of the first glove member **12a**. Electrode **98c** is positioned on the dorsal surface **44a** of the ring finger phalange portion **38a** of the first glove member **12a**. Electrode **98d** is positioned on the dorsal surface **44a** of the pinky finger phalange portion **40a** of the first glove member **12a**.

Electrode **98e** (FIG. 5) is positioned on the dorsal surface **44b** of the index finger phalange portion **34b** of the second glove member **12b**. Electrode **98f** is positioned on the dorsal surface **44b** of the middle finger phalange portion **36b** of the second glove member **12b**. Electrode **98g** is positioned on the dorsal surface **44b** of the ring finger phalange portion **38b** of the second glove member **12b**. Electrode **98h** is positioned on the dorsal surface **44b** of the pinky finger phalange portion **43b** of the second glove member **12b**.

Each of the electrodes **98a–98d** (FIG. 3) is connected to a wire **100a–100d**, respectively, that extends between and electrically connects a respective one of the electrodes **98a–98d** with a first defibrillator electrode combiner **102a**, which is preferably positioned on the dorsal surface **44a** of the first glove member **12a**. The first defibrillator electrode combiner **102a** is connected to a highly flexible No. 24 (or smaller) stranded high voltage insulated wire **104a** which extends between and electrically connects the first defibrillator electrode combiner **102a** to the first female connection plug **64a**.

Each of the electrodes **98e–98h** (FIG. 5) is connected to a highly flexible No. 24 (or smaller) stranded high voltage insulated wire **100e–100h**, respectively, that extends between and electrically connects a respective one of the electrodes **98a–98d** with a second defibrillator electrode

combiner **102b**, which is preferably positioned on the dorsal surface **44b** of the second glove member **12b**. The second defibrillator electrode combiner **102b** is connected to a highly flexible No. 24 (or smaller) stranded high voltage insulated wire **104b** which extends between and electrically connects the second defibrillator electrode combiner **102b** to the second female connection plug **64b**. The defibrillator device **54** is preferably made of parts similar, or identical, to parts of the Heartstream automatic defibrillator model "E" or "EM" of the Heartstream Co., of Seattle, Wash.

The glove members **12a** and **12b** preferably further comprise an acupuncture device for providing a voltage of sufficient potential to create electrical pin stimulations. The acupuncture device preferably includes a plurality of stainless steel electrodes **106a–106j** (FIGS. 3 and 4) positioned at the tip of, and extending away from, a respective phalange portion **32a–40a**, and **32b–40b**, respectively, on a respective glove member **12a** and **12b**. Each electrode **106a–106j** is essentially conical and has a base portion connected to a respective phalange portion **32a–40a** and **32b–40b**, respectively, and terminates in a head portion. Each of the electrodes **106a–106e** (FIG. 3) includes a wire **108a–108e**, respectively, that extends between and electrically connects a first acupuncture electrode combiner **110a** with a respective one of the electrodes **106a–106e**. The first acupuncture electrode combiner **110a** is connected to a wire **112a** which extends between and electrically connects the first acupuncture electrode combiner **110a** with the first female connection plug **64a**. Each of the electrodes **106f–106j** (FIG. 5) includes a wire **108f–108j**, respectively, that extends between and electrically connects a second acupuncture electrode combiner **110b** with a respective one of the electrodes **106f–106j**. The second acupuncture electrode combiner **110b** is connected to a wire **112b** which extends between and electrically connects the second acupuncture electrode combiner **110b** with the second female connection plug **64b**.

Each of the glove members **12a** and **12b** is preferably manufactured by securing, by any suitable means, the wires, sensors, electrodes and other components to a respective glove, preferably made of nitrile (i.e., the first layers **24a** and **24b**). It should be noted that the wires, sensors and/or electrodes could be made using flexible circuit technology, such as by using a conductive printable ink. The components of the glove member **12a** and **12b** which do not extend past the second layers **26a** and **26b**, such as the wires, are then covered by the respective second layer **26a** and **26b** in a suitable manner, such as by spraying or dip coating.

The first cable **14a** includes a first input plug **114a** (FIG. 3), which plugs into male receptors on the first female connection plug **64a** on the first glove member **12a**, and a first output plug **116a** (FIG. 6), which plugs into male receptors on a first female connection plug **118a** on the interface unit **16**. The second cable **14b** includes a first input plug **114b** (FIG. 5), which plugs into male receptors on the second female connection plug **64b** on the second glove member **12b**, and a second output plug **116b** (FIG. 6), which plugs into male receptors on a second female connection plug **118b** on the interface unit **16**. The first cable **14a** (FIG. 3) preferably includes a plurality of electrical wires and air tubes which extend between plugs **114a** and **116a** (FIG. 6) to provide electrical, audio, and fluid communication between the first glove member **12a** and the interface unit **16** when the plugs **114a** (FIG. 3) and **116a** (FIG. 6) are plugged into their respective female connection plugs **64a** (FIG. 3) and **118a** (FIG. 6). The second cable **14b** (FIG. 5) preferably includes a plurality of electrical wires which extend between

plugs **114b** and **116b** (FIG. 6) to provide electrical communication between the second glove member **12b** and the interface unit **16** when the plugs **114b** (FIG. 5) and **116b** (FIG. 6) are plugged into their respective female connection plugs **64b** (FIG. 5) and **118b** (FIG. 6).

The interface unit **16** (FIG. 6) preferably includes an EKG circuit board **120** for receiving EKG currents detected by the sensors **56a–56k** (FIGS. 2 and 4), a blood pressure circuit board **122** (FIG. 6) for receiving systolic and diastolic blood pressure and pulse rate signals from the blood pressure device **46** (FIG. 2), a temperature circuit board **124** (FIG. 6) for receiving temperature signals from the temperature device **48** (FIG. 2), a %O₂ circuit board **126** (FIG. 6) for receiving %O₂ signals from the %O₂ device **50** (FIG. 4) and an acupuncture/defibrillator circuit board **128** (FIG. 6) for controlling the delivery of electrical shock to the patient.

The EKG circuit board **120** is capable of amplifying the EKG currents from the sensors **56a–56k** and converting the EKG currents to at least a plurality of EKG analog outputs. The EKG circuit board **120** is preferably made of parts similar, or identical, to parts of the PC-ECG recorder unit from I.P.I. Medical Products of McLean, Va.

The blood pressure circuit board **122** is capable of (i) converting the systolic blood pressure signals to a systolic blood pressure analog output, (ii) the diastolic blood pressure signals to a diastolic blood pressure analog output, and (iii) the pulse rate signals to a pulse rate analog output. The blood pressure circuit board **122** includes a source of inflation fluid, such as an air pump **130** (FIG. 6), for supplying a source of inflation fluid for the air bladder **72**, and an acoustical sensor (not shown) for detecting the systolic and diastolic blood pressure and pulse rate signals. The pump **130** is in fluid communication with the air bladder **72** (FIG. 2) via the air tube **76**, cable **14a** (FIG. 1) and air conduit **131** (FIG. 6), which extends between and provides fluid and audio communication between the female connection plug **118a** of the interface unit **16** and the air pump **130** of the blood pressure circuit board **122**. The blood pressure circuit board **122** is preferably made of parts similar, or identical, to parts of the UB-302 Systolic/Diastolic (Pulse) Digital Blood Pressure monitor from A+D Engineering Inc., of Milpitas, Calif.

The temperature circuit board **124** is capable of converting the temperature signals to a temperature analog output. The temperature circuit board **124** is preferably made of parts similar, or identical, to parts of the Cole-Parmer E-08402-00 digital thermometer from Cole-Parmer, of Vernon Hills, Ill. The %O₂ circuit board **126** is capable of converting the %O₂ signals to a %O₂ analog output. The %O₂ circuit board **124** is preferably made of parts similar, or identical to parts of the Nonin Onyx blood flow and oxygen % reader, model No. 8500M from Nonin Medical, Inc., of Plymouth, Minn. The interface unit **16** also includes a first audio amp **132** for amplifying the sound waves received from the auscultation device **52** (FIG. 2). The acupuncture defibrillator circuit board **128** selectively regulates the amount of electrical energy supplied by the defibrillator device **54** (FIG. 3) and the acupuncture device. A high voltage source **134** is contained within the interface unit **16** which supplies power to the electrodes **98a–98k** to generate the electrical shock to be delivered to the patient and also supplies power to electrodes **106a–106j** (FIGS. 3 and 5).

The interface unit **16** further includes a first analog to digital converter **136** for converting the EKG analog outputs to an EKG digital data stream, a second analog to digital converter **138** for converting (i) the systolic blood pressure

analog output to a systolic blood pressure digital data stream, (ii) the diastolic blood pressure analog output to a diastolic blood pressure digital data stream, and (iii) the pulse rate analog output to a pulse rate digital data stream, a third analog to digital converter **140** for converting the temperature analog output to a temperature digital data stream, a fourth analog to digital converter **142** for converting the %O₂ analog output to a %O₂ digital data stream, and a fifth analog to digital converter **144** for converting the sound waves from the first audio amp **132** to a sound digital data stream.

The interface unit **16** further includes a multiplexer **146** for combining the digital data streams from the analog to digital converters **136–144** to a combined digital data stream. The combined digital data stream can then be conveyed to the PC **20** (FIG. 1) via a first port **148** (FIG. 6), or to the command center **18** (FIG. 1) by satellite connection B via a modem, or by radio wave connection C via the first port **148**, or to the command center **18** by telephone wire, or fiber A, via telephone modem **150** (FIG. 6) and a second port **152**. The digital data streams from the interface unit **16** are then converted or interpreted into readable diagnostic information in the command center **18** (FIG. 1) or the PC **20**. This circuitry enables the glove members **12a** and **12b** and the interface unit **16** to be provided at a reasonable cost. The multiplexer **146** (FIG. 6) also communicates with a control panel and indicator circuit board **154**.

The interface unit **16** further includes a speaker/microphone **156** (FIG. 6) which communicates with the multiplexer **146**, via a second audio amp **158** and a sixth analog to digital converter **160**, to enable a medical professional in the command center **18** (FIG. 1) to communicate orally with the persons in relative close proximity to the speaker/microphone **156** (FIG. 6).

The interface unit **16** includes a third port **164** for receiving and transmitting EKG currents detected by sensors **56a–56k** to an EKG readout apparatus **22a** (FIG. 1) where the EKG currents will be converted or interpreted into readable diagnostic information. The interface unit **16** (FIG. 6) further includes a fourth, fifth and sixth port **166**, **168** and **170**, respectively, for receiving and transmitting the analog outputs from the blood pressure circuit board **122**, the temperature circuit board **124** and the %O₂ circuit board **126**, respectively, to a blood pressure and pulse readout apparatus **22b** (FIG. 1), a temperature readout apparatus **22c**, and a %O₂ readout apparatus **22d**, respectively, where the analog outputs will be converted or interpreted into readable diagnostic information.

The interface unit **16** (FIG. 6) also includes a power supply **172** which supplies power, via power supply distributor **174**, to all of the components of the interface unit. The interface unit **16** also preferably includes a plurality of battery packs **176** and a battery charger port **178**.

The interface unit **16** further includes an optical isolator **180** for electrically isolating the entire interface unit **16** and glove members **12a** and **12b** from any destructive and damaging currents which might be encountered from external communication links.

The manner of operation of the system **10** (FIG. 1) will now be described. A person, other than the patient, places the glove probes **12a** and **12b** over his or her right and left hands, respectively, so that each of the person's fingers are received within a respective one of the phalange portions **32a–40a** and **32b–40b**, respectively. The glove members **12a** and **12b** are then connected to interface unit **16** by cables **14a** and **14b**, respectively.

EKG Diagnostic Information

To obtain EKG diagnostic information, the palmar sides **42a** and **42b** of the glove members **12a** and **12b** are placed over the patient. The sensors **56a–56g** are located at strategic positions on the glove members **12a** and **12b**, as described above, to enable a plurality of leadwire combinations to detect a plurality of standard leads when the glove members **12a** and **12b** are placed over the patient. Some exemplary leadwire combinations are as follows:

I. Single Lead Three-Leadwire Scenarios:

It is believed that at least the following ECG Leads are possible:

Lead 1:

Positive leadwire: Sensor **56c** on the tip portion of the index finger phalange portion **34a** of the first glove member **12a** is positioned above the patient's left breast at the left shoulder quadrant.

Negative leadwire: Sensor **56e** on the tip portion of the thumb phalange portion **32a** of the first glove member **12a** is positioned above and into the patient's right shoulder quadrant.

Ground leadwire: Sensor **56a** on the tip portion of the pinky finger phalange portion **40a** of the first glove member **12a** is positioned under the patient's left breast.

Lead 2:

Positive leadwire: Sensor **56a** on the tip portion of the pinky finger phalange portion **40a** of the first glove member **12a** is positioned under the patient's left breast towards the V6 position.

Negative leadwire: Sensor **56e** on the top portion of the thumb phalange portion **32a** of the first glove member **12a** is positioned above and into the patient's right shoulder quadrant.

Ground leadwire: Sensor **56a** on the tip portion of the pinky finger phalange portion **40a** of the first glove member **12a** is positioned under the patient's left breast.

Lead 3:

Positive leadwire: Sensor **56a** on the tip portion of the pinky finger phalange portion **40a** of the first glove member **12a** is positioned under the patient's left breast towards the V6 position.

Negative leadwire: Sensor **56c** on the tip portion of the index finger phalange portion **34a** of the first glove member **12a** is positioned above the patient's left breast at the left shoulder quadrant.

Ground leadwire: Sensor **56a** on the tip portion of the pinky finger phalange portion **40a** of the first glove member **12a** is positioned under the patient's left breast.

MCL1 (Modified Chest Lead) Lead:

Negative leadwire: Sensor **56c** on the tip portion of the index finger phalange portion **34a** of the first glove member **12a** is positioned above the patient's left breast at the left shoulder quadrant.

Positive leadwire: Sensor **56g** on the left side of the palm portion **28a** of the first glove member **12a** is positioned at the patient's right sternal border.

Ground leadwire: Sensor **56a** on the tip portion of the pinky finger phalange portion **40a** of the first glove member **12a** is positioned under the patient's left breast.

MCL4 Lead:

Negative leadwire: Sensor **56c** on the tip portion of the index finger phalange **34a** of the first glove member **12a** is positioned above the patient's left breast at the left shoulder quadrant.

Positive leadwire: Sensor **56a** on the tip portion of the pinky finger phalange portion **40a** of the first glove member **12a** is positioned at the patient's V4 position.

Ground leadwire: Sensor **56a** on the tip portion of the pinky finger phalange portion **40a** of the first glove member **12a** is positioned under the patient's left breast.

II. Five-Leadwire Scenario:

With the glove member **12a** placed over the patient's left breast and the second glove member **12b** placed over the patient's right wrist, it is believed that at least the following leadwires are possible:

LL acting leadwire: Sensor **56a** on the tip portion of the pinky finger phalange portion **40a** of the first glove member **12a** is positioned under the patient's left breast.

RL leadwire: Sensor **56i** on the tip portion of the middle finger phalange portion **36b** of the second glove member **12b** is positioned on the patient's right wrist.

LA acting lead: Sensor **56c** on the tip portion of the index finger phalange portion **34a** of the first glove member **12a** is positioned above the patient's left breast at the left shoulder quadrant.

RA acting leadwire: Sensor **56e** on the tip portion of the thumb phalange portion **32a** of the first glove member **12a** is positioned above and into the patient's right shoulder quadrant.

C leadwire: Sensor **56g** on the left side of the palm portion **28a** of the first glove member **12a** is positioned at the patient's right sternal border.

With the glove members **12a** and **12b** positioned in the five leadwire scenario, it is believed that the following lead readings are possible: Lead 1, Lead 2, Lead 3, AVR and AVL.

III. Seven-Leadwire Scenario:

With the glove member **12a** placed over the patient's left breast and the second glove member **12b** placed over the patient's right wrist, it is believed that at least the following leadwires are possible:

LL acting leadwire: Sensor **56a** on the tip portion of the pinky finger phalange portion **40a** of the first glove member **12a** is positioned under the patient's left breast.

V2 leadwire: Sensor **56f** on the base portion of the pinky finger phalange portion **40a** of the first glove member **12a** is positioned in the patient's V2 position.

RL leadwire: Sensor **56i** on the tip portion of the middle finger phalange portion **36b** of the second glove member **12b** is positioned on the patient's right wrist.

V4r leadwire: Sensor **56k** on the tip portion of the pinky finger phalange portion **40b** of the second glove member **12b** is positioned in the patient's V4r position.

LA acting leadwire: Sensor **56c** on the tip portion of the index finger phalange portion **34a** of the first glove member **12a** is positioned above the patient's left breast at the left shoulder quadrant.

RA acting leadwire: Sensor **56e** on the tip portion of the thumb phalange portion **32a** of the first glove member **12a** is positioned above and into the patient's right shoulder quadrant.

C leadwire: Sensor **56g** on the left side of the palm portion **28a** of the first glove member **12a** is positioned at the patient's right sternal border.

With the glove members **12a** and **12b** positioned in the seven leadwire scenario, it is believed that at least the following lead readings are possible: Lead 1, Lead 2, Lead 3, AVR, AVL, V2 and V4r.

IV. Modified Leadwire Scenarios.

Other EKG leadwire scenarios can be accomplished at the discretion of the command center and the person wearing the glove members **12a** and **12b**. Such options are available since the following glove member positions relate to electrical heart activity as below:

G (ground) leadwire:	patient's left side
+ (positive) leadwire:	patient's right chest (right sternal border)
- (negative) leadwire:	patient's left shoulder

It will be noted that the above relationships form a triangle. This triangle can be compressed or expanded, but always have the same relationships.

It should be noted that the glove members 12a and 12b of the present invention allow for a flexibility in EKG electrode positioning which has not been possible until now. With the glove members 12a and 12b positioned at the right and left shoulders, it is possible to slide a sensor 56i on the middle finger phalange portion 36b of the second glove member 12b across the patient's chest from V1 to V6 position to generate the V1-V6 leads as well as the points between the V1-V6 precordial leads. This enables one to see how the precordial electrical field changes and to determine with more accuracy the specific area of patient's heart where a possible abnormality may occur.

It should also be noted that, in the event that distortion of the EKG waveform occurs due to misplacement of the EKG sensors 56a-56k, correction of such can be accomplished using waveform modification circuits located at the command center 18. Such waveform modification circuitry accomplishes distortion correction utilizing waveshaping techniques which filter, compare, and re-shape into readable data.

V. Six-Leadwire Scenario

With the first glove member 12a placed over the patient's left breast and the second glove member 12b placed over the patient's right breast, it is believed that at least the following leadwires are possible:

6 Leadwire with Vr positions:	
Positive Leadwire:	Sensor 56c on the tip portion of the index finger phalange portion 34a of the first glove member 12a is positioned above the patient's left breast at the left shoulder quadrant.
Negative Leadwire:	Sensor 56e on the tip portion of the thumb phalange portion 32a of the first glove member 12a is positioned above and into the patient's right shoulder quadrant.
V3r Leadwire:	Sensor 56i on the middle finger phalange portion 36b of the second glove member 12b is positioned at the patient's right chest V3r position.
V4r Leadwire:	Sensor 56j on the ring finger phalange portion 38b of the second glove member 12b is positioned at the patient's right chest V4r position.
V5r Leadwire:	Sensor 56k on the pinky finger phalange portion 40b of the second glove member 12b is positioned at the patient's right chest V5r position.

A six leadwire scenario is especially useful in emergency settings to quickly evaluate risks in patients with acute inferior myocardial infraction.

With the glove members 12a and 12b positioned in the six leadwire scenario, it is believed that at least the following lead reading are possible: Lead 1, Lead 2, Lead 3, V4r, V5r and V6r. The above lead readings are important in diagnosing heart conditions in children, and especially infants.

As detailed above, the plurality of EKG sensors 56a-56g, being located together on two easily and quickly manipu-

latable glove members 12a and 12b, allows for a variety of EKG leads to be quickly and easily attained by manipulating the glove members 12a and 12b and the phalange portions 32a-40a and 32b-40b.

The EKG currents, or leads, detected from the sensors 56a-56k are transmitted to the first and second female connection plugs 64a and 64b, and through the cables 14a and 14b to the interface unit 16 where they can be sent to the command center 18 or PC 20 in a digital data stream, or to the EKG readout apparatus 22a, as discussed above.

Blood Pressure and Pulse Rate Diagnostic Information

To obtain blood pressure and pulse rate diagnostic information, the thumb phalange portion 32a (FIG. 2) and the index finger phalange portion 34a of the first glove member 12a is wrapped around one of the patient's wrist. In this position, the air bladder 72 is ready to accept air pressure from the pump 130 (FIG. 6) in the blood pressure circuit board 122. The air pump 130 then transmits inflation fluid, such as air, via the conduit 131, cable 14a and air tube 76 (FIG. 2), to the air bladder 72 to inflate the air bladder. Inflation of the air bladder 72 obliterates the radial artery. As the air bladder 72 releases the inflation fluid, pulse sound waves are acoustically picked-up by the acoustical coupler 74 and are sent over the air tube 76 to the first female connection plug 64a, and through the first cable 14a to the interface unit 16 (FIG. 1) where they can be sent to the command center 18 or PC 20 in a digital data stream, or to the blood pressure and pulse rate readout 22b, as discussed above.

Body Temperature Diagnostic Information

To obtain body temperature diagnostic information, the middle finger phalange portion 36a (FIG. 2) of the first glove member 12a is placed under the patient's tongue, or in a suitable orifice, for a period of time sufficient to receive temperature signals from the thermistor 78, preferably about one minute. The temperature signals from the temperature device 48 can be transmitted to the first female connection plug 64a, and through the first cable 14a to the interface unit 16 (FIG. 1) where they can be sent to the command center 18 or PC 20 in a digital data stream, or to the temperature readout apparatus 22d, as discussed above.

%O₂ Diagnostic Information

To obtain %O₂ diagnostic information, the thumb phalange portion 32b (FIG. 3) and the index finger phalange portion 34b of the second glove member 12b are pressed against one of the patient's finger tips. In this position, the red LED emitter 82 (FIG. 4) emits red and infra-red light toward the LED sensor 84. When the light from the LED emitter 84 is passed through the patient's finger (non-painted finger nails only) at the finger nail, the LED sensor 84 detects the color light waves present. These signals are translated from light intensity and color quality to oxygen levels. More oxygen yields a light red blood while less oxygen produces a darker red to purple blood. It should be noted that pulse rate can also be ascertained from these readings. As an alternative to the finger tips, the ear lobes could be used to measure the %O₂.

The %O₂ signals from the %O₂ device 50 are then sent to the second female connection plug 64b, and through the second cable 14b to the interface unit 16 (FIG. 1) where the %O₂ signals can be sent to the command center 18 or PC 20 in a digital data stream, or to the %O₂ readout apparatus 22c, as discussed above.

Auscultation Diagnostic Information

To listen to the heart and lungs of the patient, the first glove member 12a is moved over the patient's body to enable the acoustical coupler and microphone 90 to pick up,

or hear, sound waves from the patient's heart and lungs, much like a stethoscope would. The sound waves are then transmitted to the first female connection plug 64a, via the pair of wires 93, and then through the first cable 14a to the interface unit 16, where they can be sent to the command center 18 or PC 20, in a digital data stream as described above. Alternatively, the sound waves from the acoustical coupler of the acoustical coupler and microphone 90 could also be conducted via air tube 94 to a stethoscope 22e.

Oral Communication

To communicate orally with a remote location, such as the command center 18, the speaker/microphone 156 can transmit and receive sound waves as described above. It should be noted that the interface unit 16 may not be able to transmit or receive sound waves via the speaker/microphone 156 when processing diagnostic information from the EKG diagnostic device, the blood pressure device 46, the temperature device 48, the %O₂ device 50 and/or the auscultation device 52. The ability for a doctor to communicate with the patient, if alert, and people proximate to the patient, such as the person manipulating the glove members 12a and 12b, if such person is not the doctor, allows the doctor to instruct the person manipulating the glove members 12a and 12b to best obtain the diagnostic information and to instruct the person manipulating the glove members, or other near by the patient how to provide care/treatment to the patient.

Defibrillator Device

Once the diagnostic information from any, or all, of the EKG device, the blood pressure device 46, the temperature device 48, the %O₂ device 50, the auscultation device 52, and the oral information obtained via the speaker/microphone 156 has been received by a doctor in the command center 18 or accessible to the PC 20 or the readout apparatus 22a-22e, the doctor can decide on the best way to treat the patient. If the information obtained by the doctor indicates that the patient is in ventricular fibrillation (i.e., the heart beats in an uneven and inefficient fashion, virtually stopping the heart's ability to pump blood), the doctor instructs the person manipulating the glove to defibrillate the patient. Of course, if the doctor is with the patient and is manipulating the glove members 12a and 12b herself, then the doctor would defibrillate the patient herself.

To defibrillate the patient, the dorsal sides 44a and 44b of the first and second glove members 12a and 12b, respectively, are positioned on the patient's chest area so that the electrodes 98a-h contact the patient's chest area. The acupuncture/defibrillator circuit board 128 (FIG. 6) is activated to ready the high voltage source 134 to deliver a powerful electrical shock to the patient's heart. The high voltage source 134 delivers power, preferably about 130-300 Joules per shock, through the cables 14a and 14b to the electrodes 98a-k on the first and second glove members 12a and 12b to deliver the electric shock to the patient's heart to bring the patient out of ventricular fibrillation. The acupuncture/defibrillator circuit board 128 can be activated either by the command center 18 or by a person near the interface unit 16. In the event that the acupuncture/defibrillator circuit board 128 is to be activated by a person near the interface unit, such as the person manipulating the glove members, the delivery of power can be delayed for a period of time, preferably about five seconds, after activation of the circuit board 128 to enable proper placement of the electrodes 98a-h.

The delivery of electrical shock to the patient's heart can be repeated as necessary to bring the patient out of ventricular fibrillation to restore the patient's heartbeat to an even and efficient fashion (i.e., a regular rhythm). The glove

members 12a and 12b, having both an EKG device and a defibrillator device, enables the person manipulating the glove members to quickly and easily alternate between taking EKG readings, to monitor the condition of the patient's heart, and the defibrillator device with only a quick rotation of their hands.

Once the patient's heartbeat has been restored to a regular rhythm, the next step is to maintain the patient's heart in a regular rhythm. To do so, a first aid kit is preferably provided with the interface unit 16. The first aid kit would preferably include medications which would include an anti-arrhythmic drug, such as Lidocaine, for inhibiting the heart from falling back into ventricular fibrillation, a lactic acidosis neutralizer, such as sodium bicarbonate and pain relieving medications like demerol or morphine. These medications would preferably be preloaded in clearly marked and color coded syringes to enable quick administration. If the doctor were not near the patient and is operating out of the command center 18, the doctor can monitor the patient's condition via the glove members 12a and 12b and the interface unit 16 and can instruct the person manipulating the glove members 12a and 12b and/or persons near the patient to properly provide care/treatment for the patient.

Acupuncture Device

To provide electrical pin stimulations, the acupuncture/defibrillator circuit board 128 is activated to cause the high voltage source 134 to deliver power to the electrodes 106a-106j. The high voltage source 134 delivers power, preferably about 5 to 10 Joules per electrode 106a-106j, through the cables 14a and 14b to the electrodes 106a-106j on the first and second glove members 12a and 12b to enable the electrodes 106a-106j to provide electrical pin stimulation to the patient when the electrodes 106a-106j are moved over the patient's body.

The electrical pin stimulation from the electrodes 106a-106j can be used to alleviate pain, as is done via conventional acupuncture practice, albeit in a non-invasive manner. This glove mediated acupuncture technique obviates the need to insert needles into the body to deliver acupuncture and helps insure safety from needle transmitted diseases, such as HIV infection. The electrical pin stimulations can also be used to cauterize wounds on the patient.

Accordingly, the above-described present invention enables a plurality of diagnostic information to be quickly and accurately obtained, either by a doctor in close proximity to a patient, or by a doctor remote from the patient (i.e., when the doctor is in the command center 18), evaluate and/or monitor a patient's condition. The present invention also provides a means for quickly treating a patient (i.e., the defibrillator device 54 and the acupuncture device) under the care of a doctor who is accurately informed of the patient's condition even when the doctor is not near the patient.

While the best modes for carrying out the invention have been described in detail, those familiar with the art to which the invention relates will appreciate other ways of carrying out the invention defined by the following claims. For instance, the placement of the diagnostic devices on the glove members 12a and 12b and/or specific design of the diagnostic devices could vary from that described above. For instance, the EKG device could have more or fewer sensors or the sensors could be located differently than that described above.

What is claimed is:

1. A system for collecting and transmitting diagnostic information to a remote location and for providing emergency treatment, said system comprising:

a first member contoured to at least a portion of a first person's first hand and a second member contoured to

17

at least a portion of the first person's second hand, said members having at least one diagnostic device capable of sensing diagnostic signals from a second person, said members further comprising a defibrillator device; and

an interface unit for transmitting information to a remote location.

2. The system of claim 1 wherein said members have a shape that corresponds to at least a substantial portion of a person's hand such that each of said members is capable of being worn on a person's hand.

3. The system of claim 2 wherein said members have a portion shaped to contour to a person's palm.

4. The system of claim 3 further comprising electrical connection plugs capable of communicating with said devices and said interface unit, said members further comprising electrical circuitry providing electrical communication between said devices and said plug.

5. The system of claim 2 wherein said members have a portion shaped to contour to a person's finger.

6. The system of claim 5 wherein said members have a portion shaped to contour to a person's palm.

7. The system of claim 2 wherein said members comprise a wrist portion and a palm portion.

8. The system of claim 7 wherein said interface unit comprises a microphone.

9. The systems of claim 2 wherein said members comprise a palm portion and a phalange portion.

10. The system of claim 2 wherein each of said members have a palmar side, each of said members having at least one sensor on said palmar side of said member.

11. The system of claim 10 wherein said members have a dorsal side.

12. The system of claim 2 wherein the information that said interface unit is capable of transmitting comprises sound waves.

13. The system of claim 2 wherein said interface unit comprises a speaker.

14. The system of claim 2 wherein each of said members has a palmar side, said diagnostic device comprising at least one sensor located on said palmar side of one of said members.

15. The system of claim 14 wherein each of said members has a dorsal side, said defibrillator device comprising a plurality of defibrillator electrodes, at least one of the defibrillator electrodes being located on said dorsal side of said first member.

16. The system of claim 15 wherein said diagnostic device comprises an EKG diagnostic device and said sensor comprises a first EKG sensor.

17. The system of claim 14 wherein said diagnostic device comprises an EKG diagnostic device and said sensor comprises a first EKG sensor.

18. The system of claim 17 wherein each of said members comprises a palm portion.

19. The system of claim 18 wherein said first EKG sensor is located on said palm portion of said first member.

20. The system of claim 18 wherein said first member further comprises five phalange portions, said first EKG sensor being located on one of said phalange portions of said first member.

21. The system of claim 17 wherein said EKG device comprises a plurality of EKG sensors.

22. The system of claim 17 wherein said EKG diagnostic device includes at least seven EKG sensors.

23. The system of claim 1 wherein each of said members comprises a glove.

18

24. The system of claim 23 wherein each of said members comprises a palm portion, a wrist portion and five phalange portions.

25. The system of claim 1 wherein said members comprise a plurality of diagnostic devices.

26. The system of claim 25 wherein said plurality of diagnostic devices includes an EKG diagnostic device, a blood pressure and pulse diagnostic device and a temperature device.

27. The system of claim 26 wherein said plurality of diagnostic devices further includes a percent O₂ diagnostic device and an auscultation device.

28. The system of claim 27 wherein said members further include an acupuncture device having a plurality of electrodes located on said members.

29. The system of claim 25 wherein said plurality of diagnostic devices comprises at least two diagnostic devices selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, a percent O₂ device, and an auscultation device.

30. The system of claim 25 wherein said plurality of diagnostic devices comprises at least three diagnostic devices selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, a percent O₂ device, and an auscultation device.

31. The system of claim 25 wherein said plurality of diagnostic devices comprises at least four diagnostic devices selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, a percent O₂ device, and an auscultation device.

32. The system of claim 2 wherein said diagnostic device is selected from the group consisting of an EKG device, a blood pressure and pulse rate device, and a temperature device, a percent O₂ device.

33. The system of claim 2 wherein said diagnostic device is selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, a percent O₂ device, and an auscultation device.

34. A system for collecting and transmitting diagnostic information to a remote location and for providing emergency treatment, said system comprising:

a first member contoured to at least a portion of a first person's first hand and a second member contoured to at least a portion of the first person's second hand, said members having at least one diagnostic device capable of sensing diagnostic signals from a second person; and an interface unit for transmitting information to a remote location.

35. The system of claim 34 wherein said members have a shape that corresponds to at least a substantial portion of a person's hand such that each of said members is capable of being worn on a person's hand.

36. The system of claim 35 wherein said members have a portion shaped to contour to a person's palm.

37. The system of claim 35 wherein said members have a portion shaped to contour to a person's finger.

38. The system of claim 37 wherein said members have a portion shaped to contour to a person's palm.

39. The system of claim 35 wherein said members comprise a wrist portion and a palm portion.

40. The system of claim 35 wherein said members comprise a palm portion and a phalange portion.

41. The system of claim 35 wherein each of said members have a palmar side, each of said members having at least one sensor on said palmar side of said member.

42. The system of claim 41 wherein said members have a dorsal side.

19

43. The system of claim 35 wherein said members further comprise a defibrillator device.

44. The system of claim 43 wherein each of said members has a dorsal side, said defibrillator device comprising a plurality of defibrillator electrodes, at least of the defibrillator electrodes being located on said dorsal side of said first member.

45. The system of claim 35 wherein each of said members has a palmar side, said diagnostic device comprising at least one sensor located on said palmar side of one of said members.

46. The system of claim 45 wherein said diagnostic device comprises an EKG diagnostic device and said sensor comprises a first EKG sensor.

47. The system of claim 46 wherein said EKG device comprises a plurality of EKG sensors.

48. The system of claim 45 wherein said first member further comprises five phalange portions, said first EKG sensor being located on one of said phalange portions of said first member.

49. The system of claim 35 wherein each of said members comprises a glove.

50. The system of claim 35 wherein said members comprise a plurality of diagnostic devices.

51. The system of claim 50 wherein said plurality of diagnostic devices comprises at least two diagnostic devices selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, a percent O₂ device, and an auscultation device.

52. The system of claim 50 wherein said plurality of diagnostic devices comprises at least three diagnostic devices selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, a percent O₂ device, and an auscultation device.

53. The system of claim 50 wherein said plurality of diagnostic devices comprises at least four diagnostic devices selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, a percent O₂ device, and an auscultation device.

54. The system of claim 35 wherein each of said members comprises a palm portion, a wrist portion and five phalange portions.

55. The system of claim 35 wherein said diagnostic device is selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, a percent O₂ device, and an auscultation device.

20

56. The system of claim 35 wherein said diagnostic device is selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, and a percent O₂ device.

57. A system for collecting and transmitting diagnostic information to a remote location and for providing emergency treatment, said system comprising:
 a first member contoured to at least a portion of a first person's first hand and a second member contoured to at least a portion of the first person's second hand, each said members having a palmar side, a dorsal side, an inner surface and an outer surface, at least one of said members having at least one sensor on said palmar side and outer surface of said member; and
 an interface unit for transmitting information to a remote location.

58. The system of claim 57 wherein said members have a shape that corresponds to at least a substantial portion of a person's hand such that each of said members is capable of being worn on a person's hand.

59. The system of claim 57 wherein the members comprise at least one diagnostic device having at least one sensor, said sensor being the at least one sensor.

60. The system of claim 59 wherein said diagnostic device is selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, a percent O₂ device, and an auscultation device.

61. The system of claim 57 wherein the members comprise a plurality of diagnostic devices.

62. The system of claim 61 wherein said plurality of diagnostic devices comprises at least three diagnostic devices selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, a percent O₂ device, and an auscultation device.

63. The system of claim 61 wherein said plurality of diagnostic devices comprises at least four diagnostic devices selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, a percent O₂ device, and an auscultation device.

64. The system of claim 61 wherein said plurality of diagnostic devices comprises at least two diagnostic devices selected from the group consisting of an EKG device, a blood pressure and pulse rate device, a temperature device, a percent O₂ device, and an auscultation device.

* * * * *

专利名称(译)	远程诊断设备		
公开(公告)号	US6595918	公开(公告)日	2003-07-22
申请号	US09/884371	申请日	2001-06-19
[标]申请(专利权)人(译)	INEEDMD.COM		
申请(专利权)人(译)	INEEDMD.COM		
当前申请(专利权)人(译)	INEEDMD.COM		
[标]发明人	GOPINATHAN GOVINDAN TILFORD ARTHUR R		
发明人	GOPINATHAN, GOVINDAN TILFORD, ARTHUR R.		
IPC分类号	A61B5/0205 A61B5/00 A61B5/0408 A61B5/021 A61B5/024 A61B7/00 A61B7/04 G01N21/27 A61B5/01 A61B5/022 A61B5/0245 A61B5/04 A61B5/0402 A61B5/145 A61B5/1455 A61B19/00 G01N21/35		
CPC分类号	A61B5/0006 A61B5/02055 A61B5/04085 A61B5/6806 A61B5/0022 A61B5/0008 A61B5/021 A61B5 /022 A61B5/024 A61B5/02438 A61B5/1455 A61B7/003 A61B7/04 A61B2562/168 Y10S128/903 G16H40/67		
其他公开文献	US20010056227A1		
外部链接	Espacenet USPTO		

摘要(译)

一种系统 (10) , 用于收集多个诊断信息并将诊断信息发送到远程位置 (18,20和22a-22e) 并用于提供紧急治疗。该系统 (10) 包括 : 第一构件 (12a) , 其适于佩戴在人的第一只手上;以及第二构件 (12b) , 其适于佩戴在人的第二只手上。构件 (12a和12b) 包括多个诊断装置和除颤器装置。提供了一种用于向远程位置发送信息和从远程位置接收信息的发送单元。

