



US008308650B2

(12) **United States Patent**  
**Bardy**

(10) **Patent No.:** **US 8,308,650 B2**  
(45) **Date of Patent:** **\*Nov. 13, 2012**

(54) **SYSTEM AND METHOD FOR GENERATING  
BASELINE DATA FOR AUTOMATED  
MANAGEMENT OF CARDIOVASCULAR  
PRESSURE**

4,142,533 A 3/1979 Brownlee et al.  
4,197,856 A 4/1980 Northrop  
4,428,378 A 1/1984 Anderson et al.  
4,531,527 A 7/1985 Reinhold, Jr. et al.

(Continued)

(75) Inventor: **Gust H. Bardy**, Seattle, WA (US)

FOREIGN PATENT DOCUMENTS

(73) Assignee: **Cardiac Pacemakers, Inc.**, St. Paul, MN (US)

AU 759502 2/2001

(Continued)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

OTHER PUBLICATIONS

Partial File History (from Jul. 23, 2010 to Feb. 7, 2011) for co-pending U.S. Appl. No. 10/876,118, filed Jun. 24, 2004, "System and Method for Analyzing a Patient Status for Congestive Heart Failure for Use in Automated Patient", which is a parent application to the present U.S. Appl. No. 11/150,334 (40 pages).

(Continued)

(21) Appl. No.: **12/938,686**

(22) Filed: **Nov. 3, 2010**

(65) **Prior Publication Data**

US 2011/0046493 A1 Feb. 24, 2011

**Related U.S. Application Data**

(63) Continuation of application No. 11/635,205, filed on Dec. 6, 2006, now Pat. No. 7,837,629, which is a continuation of application No. 09/789,416, filed on Feb. 20, 2001, now Pat. No. 7,248,916, which is a continuation of application No. 09/361,332, filed on Jul. 26, 1999, now Pat. No. 6,221,011.

(51) **Int. Cl.**  
**A61B 5/02** (2006.01)

(52) **U.S. Cl.** ..... **600/508; 607/9; 600/300; 600/301**

(58) **Field of Classification Search** ..... **600/508, 600/301**

See application file for complete search history.

(56) **References Cited**


U.S. PATENT DOCUMENTS

3,832,339 A 8/1974 Aisenberg et al.  
3,837,339 A 9/1974 Aisenberg et al.

(57) **ABSTRACT**

A system and method for generating baseline data for automated management of cardiovascular pressure is disclosed. Collected device measures are accumulated to record raw physiometry for a patient, wherein the patient is regularly monitored by an implantable medical device, beginning with an initial observation period. Derived device measures are generated to provide derivative physiometry determined at least in part from the collected device measures. A patient status indicator is determined by analyzing the collected and derived device measures to diagnose a pathophysiology indicative of an absence, onset, progression, regression, and status quo in cardiovascular pressure, wherein the collected and derived device measures and the patient status indicator originating from the initial observation period include baseline data.

**18 Claims, 13 Drawing Sheets**

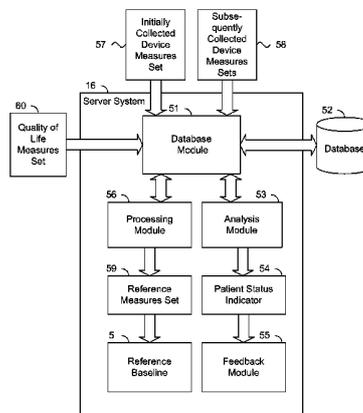

U.S. PATENT DOCUMENTS							
4,566,461	A	1/1986	Lubell et al.	6,004,276	A	12/1999	Wright et al.
4,686,999	A	8/1987	Snyder et al.	6,014,581	A	1/2000	Wayne et al.
4,803,625	A	2/1989	Fu et al.	6,024,699	A	2/2000	Surwit et al.
4,809,697	A	3/1989	Causey, III et al.	6,038,469	A	3/2000	Karlsson et al.
4,852,570	A	8/1989	Levine	6,047,203	A	4/2000	Sackner et al.
4,899,758	A	2/1990	Finkelstein et al.	6,050,940	A	4/2000	Braun
4,958,645	A	9/1990	Cadell et al.	6,063,028	A	5/2000	Luciano
4,974,607	A	12/1990	Miwa	6,067,466	A	5/2000	Selker
4,987,897	A	1/1991	Funke	6,073,046	A	6/2000	Patel
5,040,536	A	8/1991	Riff	6,080,106	A	6/2000	Lloyd et al.
5,113,859	A	5/1992	Funke	6,083,248	A	7/2000	Thompson
5,113,869	A	5/1992	Nappholz et al.	6,093,146	A	7/2000	Filangeri
5,133,346	A	7/1992	Kulkarni	6,095,985	A	8/2000	Raymond et al.
5,178,149	A	1/1993	Imburgia et al.	6,102,856	A	8/2000	Groff et al.
5,199,428	A	4/1993	Obel et al.	6,122,351	A	9/2000	Schlueter, Jr. et al.
5,301,105	A	4/1994	Cummings, Jr.	6,129,675	A	10/2000	Jay
5,307,263	A	4/1994	Brown	6,135,951	A	10/2000	Richardson et al.
5,309,919	A	5/1994	Snell et al.	6,139,494	A	10/2000	Cairnes
5,313,593	A	5/1994	Barakat et al.	6,152,882	A	11/2000	Prutchi
5,331,549	A	7/1994	Crawford, Jr.	6,155,267	A	12/2000	Nelson
5,336,245	A	8/1994	Adams et al.	6,166,563	A	12/2000	Volk et al.
5,355,889	A	10/1994	Nevo et al.	6,168,563	B1	1/2001	Brown
5,357,427	A	10/1994	Langen et al.	6,168,653	B1	1/2001	Myers
5,390,238	A	2/1995	Kirk et al.	6,171,237	B1	1/2001	Avitall et al.
5,416,695	A	5/1995	Stutman et al.	6,171,256	B1	1/2001	Joo et al.
5,421,343	A	6/1995	Feng	6,203,495	B1	3/2001	Bardy
5,437,278	A	8/1995	Wilk	6,211,011	B1	4/2001	Chen
5,438,983	A	8/1995	Falcone	6,221,011	B1	4/2001	Bardy
5,464,012	A	11/1995	Falcone	6,223,078	B1	4/2001	Marcovecchio
5,544,661	A	8/1996	Davis et al.	6,225,901	B1	5/2001	Kail, IV
5,553,609	A	9/1996	Chen et al.	6,234,964	B1	5/2001	Iliff
5,557,514	A	9/1996	Seare et al.	6,246,992	B1	6/2001	Brown
5,576,952	A	11/1996	Stutman et al.	6,249,705	B1	6/2001	Snell
5,584,868	A	12/1996	Salo et al.	6,250,309	B1	6/2001	Krichen et al.
5,591,215	A	1/1997	Greenhut et al.	6,261,230	B1	7/2001	Bardy
5,603,331	A	2/1997	Heemels et al.	6,263,245	B1	7/2001	Snell
5,660,183	A	8/1997	Chiang et al.	6,270,457	B1	8/2001	Bardy
5,673,691	A	10/1997	Abrams et al.	6,277,072	B1	8/2001	Bardy
5,687,734	A	11/1997	Dempsey et al.	6,280,380	B1	8/2001	Bardy
5,697,959	A	12/1997	Poore	6,283,923	B1	9/2001	Finkelstein et al.
5,704,345	A	1/1998	Berthon-Jones	6,287,252	B1	9/2001	Lugo
5,704,366	A	1/1998	Tacklind et al.	6,290,646	B1	9/2001	Cosentino et al.
5,711,297	A	1/1998	Iliff	6,302,844	B1	10/2001	Walker
5,712,580	A	1/1998	Baumgartner et al.	6,306,088	B1	10/2001	Krausman et al.
5,713,350	A	2/1998	Yokota et al.	6,312,378	B1	11/2001	Bardy
5,720,770	A	2/1998	Nappholz et al.	6,331,160	B1	12/2001	Bardy
5,720,771	A	2/1998	Snell	6,336,900	B1	1/2002	Alleckson
5,724,580	A	3/1998	Levi et al.	6,336,903	B1	1/2002	Bardy
5,724,983	A	3/1998	Selker et al.	6,361,501	B1	3/2002	Amano et al.
5,738,102	A	4/1998	Lemelson	6,363,282	B1	3/2002	Nichols et al.
5,743,267	A	4/1998	Nikolic	6,368,284	B1	4/2002	Bardy
5,749,907	A	5/1998	Mann	6,379,301	B1	4/2002	Worthington et al.
5,749,908	A	5/1998	Snell	6,398,728	B1	6/2002	Bardy
5,752,976	A	5/1998	Duffin et al.	6,411,840	B1	6/2002	Bardy
5,769,074	A	6/1998	Barnhill et al.	6,416,471	B1	7/2002	Kumar et al.
5,772,586	A	6/1998	Heinonen et al.	6,428,483	B1	8/2002	Carlebach
5,772,599	A	6/1998	Nevo et al.	6,440,066	B1	8/2002	Bardy
5,772,604	A	6/1998	Langberg et al.	6,442,432	B2	8/2002	Lee
5,778,882	A	7/1998	Raymond et al.	6,442,433	B1	8/2002	Linberg
5,785,650	A	7/1998	Akasaka et al.	6,454,705	B1	9/2002	Cosentino
5,785,660	A	7/1998	Van Lake et al.	6,454,707	B1	9/2002	Casscells, III et al.
5,788,640	A	8/1998	Peters	6,473,646	B2	10/2002	Sun et al.
5,788,643	A	8/1998	Feldman	6,477,424	B1	11/2002	Thompson et al.
5,792,062	A	8/1998	Poon et al.	6,478,737	B2	11/2002	Bardy
5,819,251	A	10/1998	Kremer et al.	6,480,745	B2	11/2002	Nelson et al.
5,855,593	A	1/1999	Olson et al.	6,497,655	B1	12/2002	Linberg et al.
5,860,918	A	1/1999	Schradi et al.	6,512,949	B1	1/2003	Combs et al.
5,876,353	A	3/1999	Riff	6,524,239	B1	2/2003	Reed et al.
5,879,375	A	3/1999	Larson, Jr. et al.	6,564,104	B2	5/2003	Nelson et al.
5,891,178	A	4/1999	Mann et al.	6,648,820	B1	11/2003	Sarel
5,897,493	A	4/1999	Brown	6,662,032	B1	12/2003	Gavish et al.
5,911,132	A	6/1999	Sloane	6,811,537	B2	11/2004	Bardy
5,931,857	A	8/1999	Prieve	6,827,670	B1	12/2004	Stark et al.
5,954,640	A	9/1999	Szabo	6,866,629	B2	3/2005	Bardy
5,957,861	A	9/1999	Combs et al.	6,887,201	B2	5/2005	Bardy
5,974,124	A	10/1999	Schlueter, Jr. et al.	6,893,397	B2	5/2005	Bardy
5,987,352	A	11/1999	Klein et al.	6,908,437	B2	6/2005	Bardy
5,993,386	A	11/1999	Ericsson	6,920,360	B2	7/2005	Lee et al.
				6,945,494	B2	9/2005	Bardy

6,945,934	B2	9/2005	Bardy	
6,960,167	B2	11/2005	Bardy	
7,104,955	B2	9/2006	Bardy	
7,134,996	B2	11/2006	Bardy	
7,147,600	B2	12/2006	Bardy	
7,248,916	B2	7/2007	Bardy	
7,837,629	B2 *	11/2010	Bardy	600/508
7,874,993	B2	1/2011	Bardy	
7,972,274	B2	7/2011	Bardy	
2001/0023360	A1	9/2001	Nelson et al.	
2001/0039375	A1	11/2001	Lee et al.	
2003/0055679	A1	3/2003	Soll et al.	
2004/0122486	A1	6/2004	Stahmann et al.	
2007/0179357	A1	8/2007	Bardy	
2007/0239741	A1	12/2007	Bardy	
2011/0172548	A1	7/2011	Bardy	
2011/0224563	A1	9/2011	Bardy	

FOREIGN PATENT DOCUMENTS

AU	759934	3/2001
AU	751467	8/2002
CA	2314517	1/2001
EP	0 34 2859	11/1989
EP	0 513 457	11/1992
EP	0 531 889 A2	3/1993
EP	0 711 531 A1	5/1996
EP	0 887 759	12/1998
EP	1057448	5/2000
EP	1107158	7/2000
WO	WO 97/39792	10/1997
WO	98/07142	2/1998
WO	WO 98/01742	2/1998
WO	WO 98/42103	9/1998
WO	WO-99/14882	3/1999
WO	WO 99/46718	9/1999
WO	WO 99/55226	11/1999
WO	03/027936	4/2003

OTHER PUBLICATIONS

Partial File History (from Jul. 23, 2010 to Feb. 7, 2011) for co-pending U.S. Appl. No. 11/894,514, filed Dec. 6, 2006, entitled "System and Method for Providing Baseline Data for Automated Patient Management", which claims priority to the same parent application (U.S. Appl. No. 09/361,332) as the present application (U.S. Appl. No. 11/894,514) (17 pages).

Partial File History (from Apr. 26, 2011 through Jun. 1, 2011) for co-pending U.S. Appl. No. 11/894,514, filed Dec. 6, 2006, entitled "System and Method for Providing Baseline Data for Automated Patient Management", which claims priority to the same parent application (U.S. Appl. No. 09/361,332) as the present application (U.S. Appl. No. 12/938,686) (31 pages).

Partial File History (from Feb. 8, 2011 through Jun. 2, 2011) for co-pending U.S. Appl. No. 10/876,118, filed Jun. 24, 2004, "System and Method for Analyzing a Patient Status for Congestive Heart Failure for Use in Automated Patient" (43 pages).

File History (as of Jun. 2, 2011) for co-pending U.S. Appl. No. 13/115,266, filed May 25, 2011, "System and Method for Analyzing a Patient Status for Congestive Heart Failure for Use in Automated Patient" (91 pages).

File History (as of Jun. 2, 2011) for co-pending U.S. Appl. No. 13/073,301, filed Mar. 28, 2011, "System and Method for Analyzing a Patient Status for Congestive Heart Failure for Use in Automated Patient" (96 pages).

Partial File History (from Sep. 25, 2010 through Jun. 2, 2011) for co-pending U.S. Appl. No. 11/635,364, filed Dec. 6, 2006, entitled "System and Method for Determining a Reference Baseline for Use in Heart Failure Assessment" (5 pages).

Partial File History (from Feb. 7, 2011 to Apr. 25, 2011) for co-pending U.S. Appl. No. 11/894,514, filed Dec. 6, 2006, entitled "System and Method for Providing Baseline Data for Automated Patient Management", which claims priority to the same parent application (U.S. Appl. No. 09/361,332) as the present application (U.S. Appl. No. 11/894,514) (11 pages).

Auer et al., "Paced Epimyocardial Electrograms for Noninvasive Rejection Monitoring After Heart Transplantation," *The Journal of Heart and Lung Transplantation*, vol. 15, No. 10, pp. 993-998 (Oct. 1996).

Belardinelli et al., "A Four-Minutes Submaximal Constant Work Rate Exercise Test to Assess Cardiovascular Functional Class in Chronic Heart Failure", *The American Journal of Cardiology*, 81:1210-1214 (1998).

Braunwald, "Heart Disease: A Textbook of Cardiovascular Medicine" 5th Ed., W.B. Saunders Co., vol. 1, pp. 451-455 (1997).

Office Actions, Responses, and Appeal-related documents for EP Patent Application No. 00650193.6, filed Nov. 16, 2000, which corresponds to U.S. Appl. No. 09/441,623, which is the parent application to co-pending application U.S. Appl. No. 10/876,118 (113 pages).

Office Actions, Responses, and Notice of Allowance for EP Patent Application No. 00202604.05, filed Jun. 20, 2000, which corresponds to U.S. Appl. No. 09/361,332, which is the parent application to the present application (40 pages).

Discovery® II Pacemaker System Guide Manual, Dec. 2003 (207 pages).

Discovery™ II Pacemaker Physician's Technical Manual, Oct. 1999 (6 pages).

Dunn et al., "Telemedicine Links Patients in Sioux Lookout with Doctors in Toronto," *CMA Journal*, vol. 122, pp. 484-487 (Feb. 23, 1980).

EP Search Report for EP Patent Application No. 00202604.05, dated Dec. 8, 2000, which corresponds to U.S. Appl. No. 09/361,332, which is the parent application to the present application (2 pages).

EP Search Report for EP Patent Application No. 00650193.6, dated Apr. 2, 2002, which corresponds to U.S. Appl. No. 09/441,623, which is the parent application to co-pending U.S. Appl. No. 10/876,118 (4 pages).

Examiner's First Report on AU Patent Application No. 2002302016, dated Jun. 22, 2005, which corresponds to U.S. Appl. No. 09/441,623, which is the parent application to co-pending U.S. Appl. No. 10/876,118 (2 pages).

File History for Canadian Patent Application No. 2325660 (abandoned), which corresponds to U.S. Appl. No. 09/441,623, filed Nov. 16, 1999, which is the parent application to co-pending U.S. Appl. No. 10/876,118 (17 pages).

File History for co-pending U.S. Appl. No. 11/150,334, filed Jun. 10, 2005, entitled "System and Method for Diagnosing and Monitoring Congestive Heart Failure" (393 pages).

File History for co-pending U.S. Appl. No. 10/876,118, filed Jun. 24, 2004, entitled "System and Method for Analyzing a Patient Status Failure for Congestive Heart Failure for use in Automated Patient Care" (418 pages).

File History for co-pending U.S. Appl. No. 11/880,754, filed Jul. 23, 2007, entitled "System and Method for Determining a Reference Baseline for Use in Cardiac Decompensation Assessment" (160 pages).

File History for co-pending U.S. Appl. No. 11/102,522, filed Apr. 8, 2005, entitled "System and Method for Determining a Reference Baseline for Use in Heart Failure Assessment" (427 pages).

File History for co-pending U.S. Appl. No. 11/635,364, filed Dec. 6, 2006, entitled "System and Method for Determining a Reference Baseline for Use in Heart Failure Assessment" (332 pages).

File History for co-pending U.S. Appl. No. 11/894,514, filed Aug. 20, 2007, entitled "System and Method for Determining a Reference Baseline for Use in Heart Failure Assessment" (223 pages).

Hutten et al., "Cardiac Telemonitoring by Integrating Pacemaker Telemetry within Worldwide Data Communication Systems," *Proceedings of 19th International Conference, IEEE/EMBS, Chicago, IL*, pp. 974-976 (Oct. 30-Nov. 2, 1997).

Long WJ, et al., "Differential Diagnosis Generation From a Causal Network With Probabilities," *Computers in Cardiology*, 1988, *Proceedings*, pp. 185-188, Washington DC, USA.

Magrabi et al., "Web Based Longitudinal ECG Monitoring," *Proceedings of 20th Annual International Conference of the IEEE Engineering in Medicine and Biology Society*, vol. 20, No. 3, pp. 1155-1158 (1998).

- Medtronic GEM® 7227Cx, 7227B, 7227D, 7227E Implantable Cardioverter Defibrillators, Sep. 2001 (313 pages).
- Medtronic GEM® II DR 7273 Dual Chamber Implantable Cardioverter Defibrillator 9964E Software, Jan. 2001 (402 pages).
- Merriam Webster Online and Dictionary.com definitions for “implantable” (Sep. 30, 2007).
- Moody, “Integration of Real-Time and Off-Line Clinical Data in the MIMIC Database,” *Computers in Cardiology* 1997 vol. 24, pp. 585-588, Cambridge, MA USA.
- Nelwan et al., “Ubiquitous Access to Real-Time Patient Monitoring Data,” *Computers in Cardiology*, vol. 24, pp. 271-274 (1997).
- PRM Portable Programmer Recorder Monitor, Model 2901, Operator’s Manual, Guidant Corporation (1999) (22 pages).
- Roberge et al., “Basic and Applied Biomedical Engineering Building Blocks for Health Care,” 1995 IEEE Engineering in Medicine and Biology 17th Annual Conference, vol. 1, Montreal-Canada, (Sep. 20-23, 1995).
- Schreier et al., “A Non-Invasive Rejection Monitoring System Based on Remote Analysis of Intramyocardial Electrograms from Heart Transplants,” *IEEE*, pp. 35-36 (1997).
- Vargas, “Home-Based Monitoring of Cardiac Patients,” Dept. of Electr. & Comput. Eng., South Carolina Univ., Columbia, SC, Information Technology Applications in Biomedicine, Proceedings., 1998 IEEE International Conference, pp. 133-136 (May 16-17, 1998).
- Partial File History (from Jun. 2, 2011 through Oct. 13, 2011) for co-pending U.S. Appl. No. 13/073,301, filed Mar. 28, 2011, “System and Method for Analyzing a Patient Status for Congestive Heart Failure for Use in Automated Patient” (38 pages).
- “File History of Office Actions and Responses for co-owned EP publication No. 1107158”, From Dec. 21, 2000 to Feb. 28, 2008, Entitled “System and Method for Determining a Reference Baseline of Individual Patient Status for Use in an Automated Collection and Analysis Patient Care System,” Filed on Jul. 20, 2000 (53 pages).
- “File History for co-pending U.S. Appl. No. 13/073,301”, from Oct. 14, 2011 to Feb. 20, 2012, Entitled “System and Method for Diagnosing and Monitoring Congestive Heart Failure,” Filed on Mar. 28, 2011 (16 pages).
- “File History for co-pending U.S. Appl. No. 13/115,266,” From Jun. 3, 2011 to Feb. 20, 2012, Entitled “System and Method for Diagnosing and Monitoring Congestive Heart Failure,” Filed on May 25, 2011 (50 pages).
- “File History for co-owned, co-pending EP publication No. 1102196 claiming priority to US patent 6,336,903”, From Nov. 2, 2010 to Feb. 20, 2012, Entitled “Automated Collection and Analysis Patient Care System and Method for Diagnosing and Monitoring Congestive Heart Failure and Outcomes Thereof,” Filed on Nov. 16, 2000 (125 pages).
- “File History for co-owned EP publication No. 1102199 claiming priority to US patent 6,336,903”, complete file history, Entitled “Automated Collection and Analysis Patient Care System and Method for Diagnosing and Monitoring Myocardial Ischemia and Outcomes Thereof,” Filed on Nov. 16, 2000 (288 pages).
- Dawant, Benoit M. et al., “SIMON: A Distributed Computer Architecture for Intelligent Patient Monitoring”, *Expert Systems With Applications* 1993, vol. 6, pp. 411-420.
- Degoulet, Patrice et al., “Introduction to Clinical Informatics”, *Computers in Health Care* 1996, 10: pp. 131-138.
- Nelson, Charlotte L. et al., “Relation of Clinical and Angiographic Factors to Functional Capacity as Measured by the Duke Activity Status Index”, *The American Journal of Cardiology*, Oct. 1, 1991, vol. 68, pp. 973-975.
- Puers, B. et al., “Patient Monitoring Systems”, *IEEE* 1989, pp. 1-6.
- Uckun, Serdar, “Intelligent systems in patient monitoring and therapy management”, *International Journal of Clinical Monitoring and Computing* 1994, 11: pp. 241-253.
- Van Bommel, J.H. et al., “Handbook of Medical Informatics”, *Handbook of Medical Informatics* 1997, 8: pp. 117-125.
- Benditt, DG et al., “Single-chamber cardiac pacing with activity-initiated chronotropic response: evaluation by cardiopulmonary exercise testing”, 9 Pgs.

\* cited by examiner

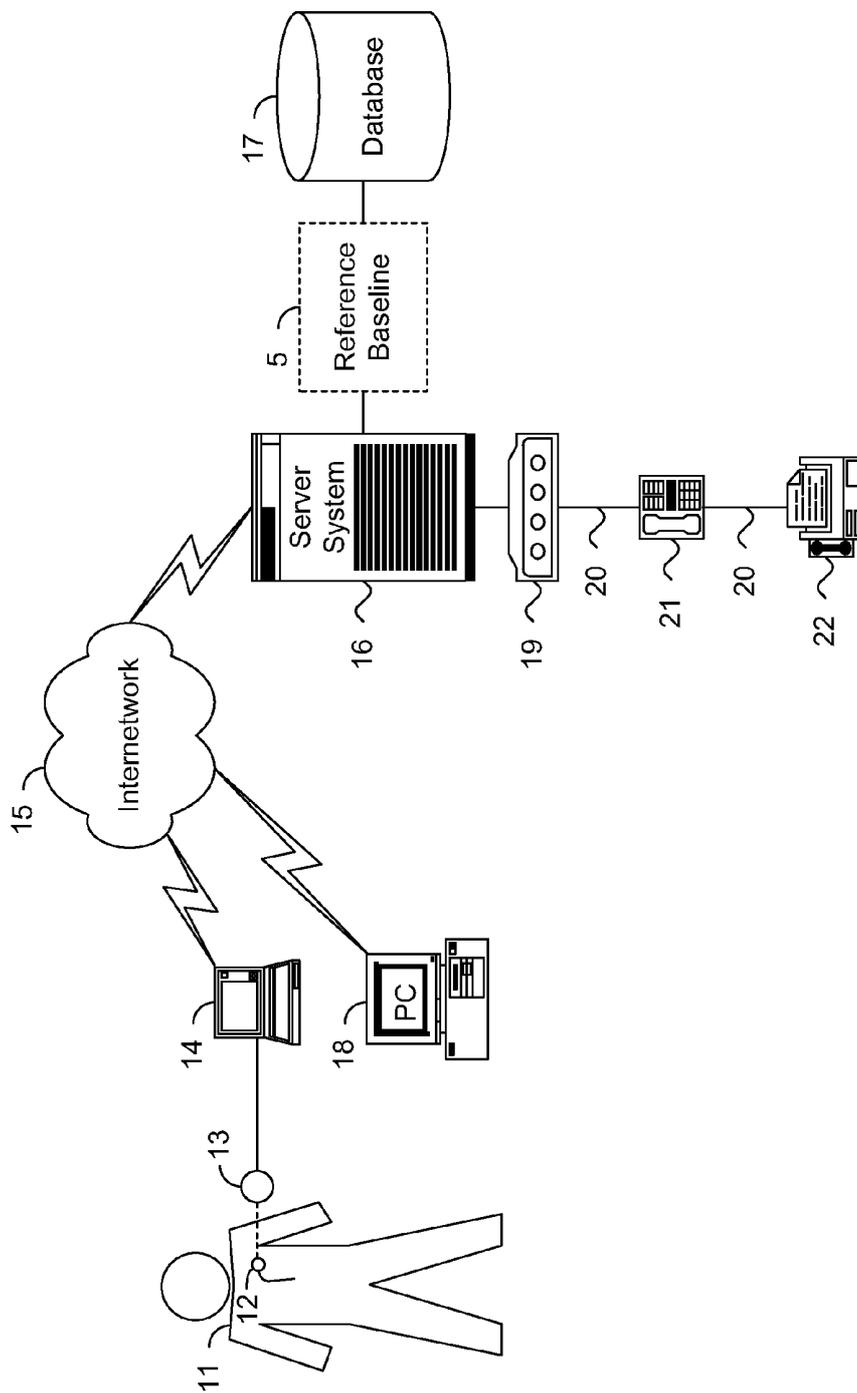


Fig. 1A.

10

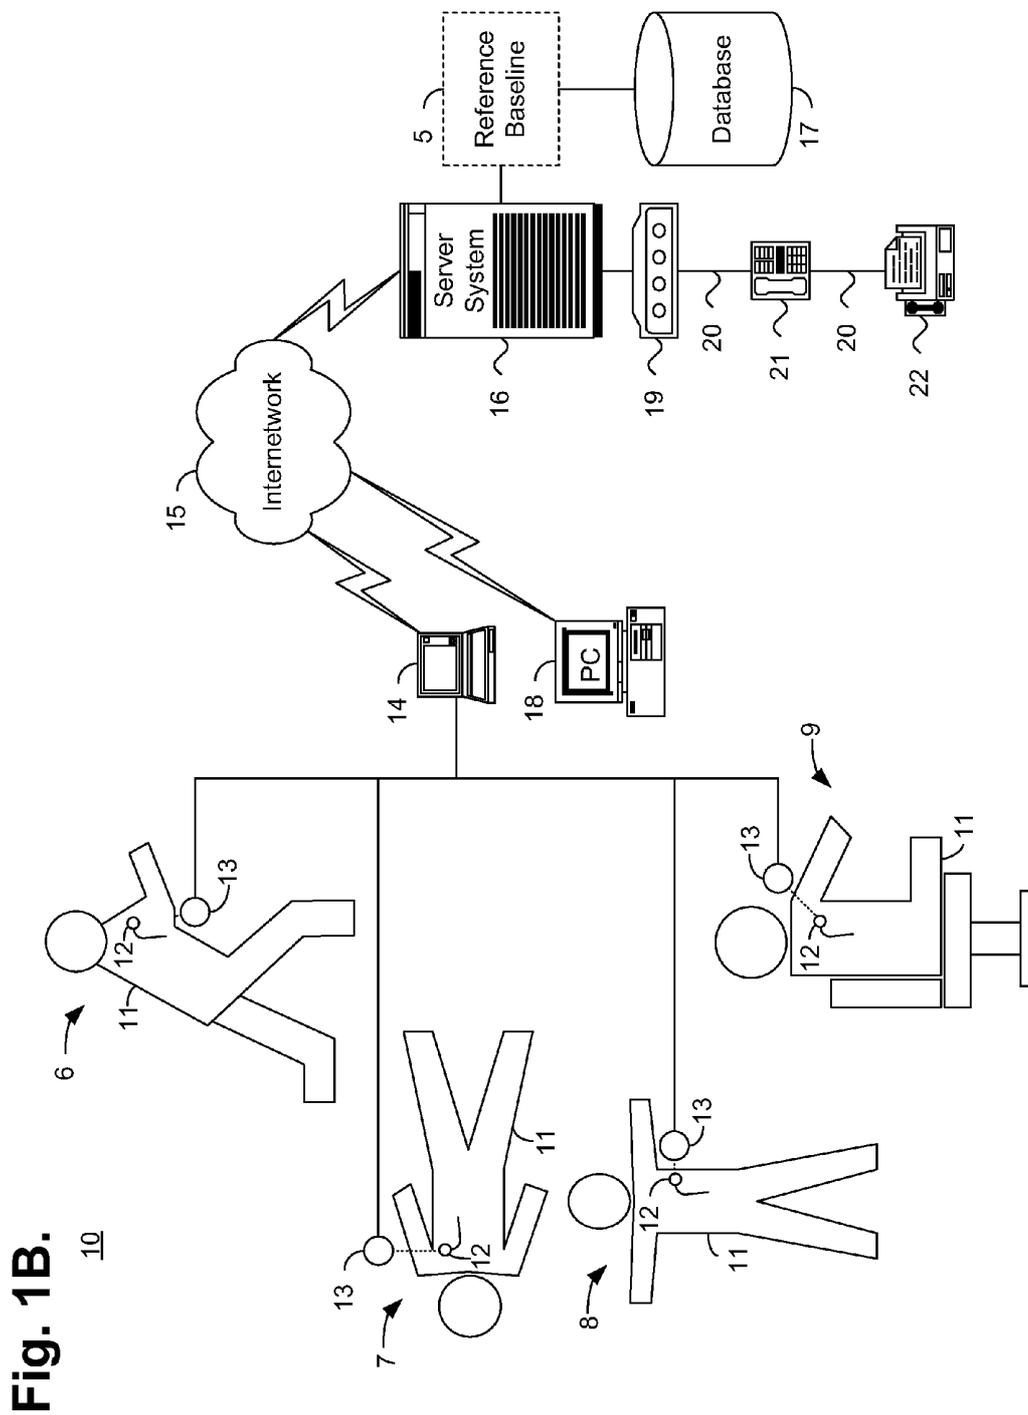


Fig. 2.

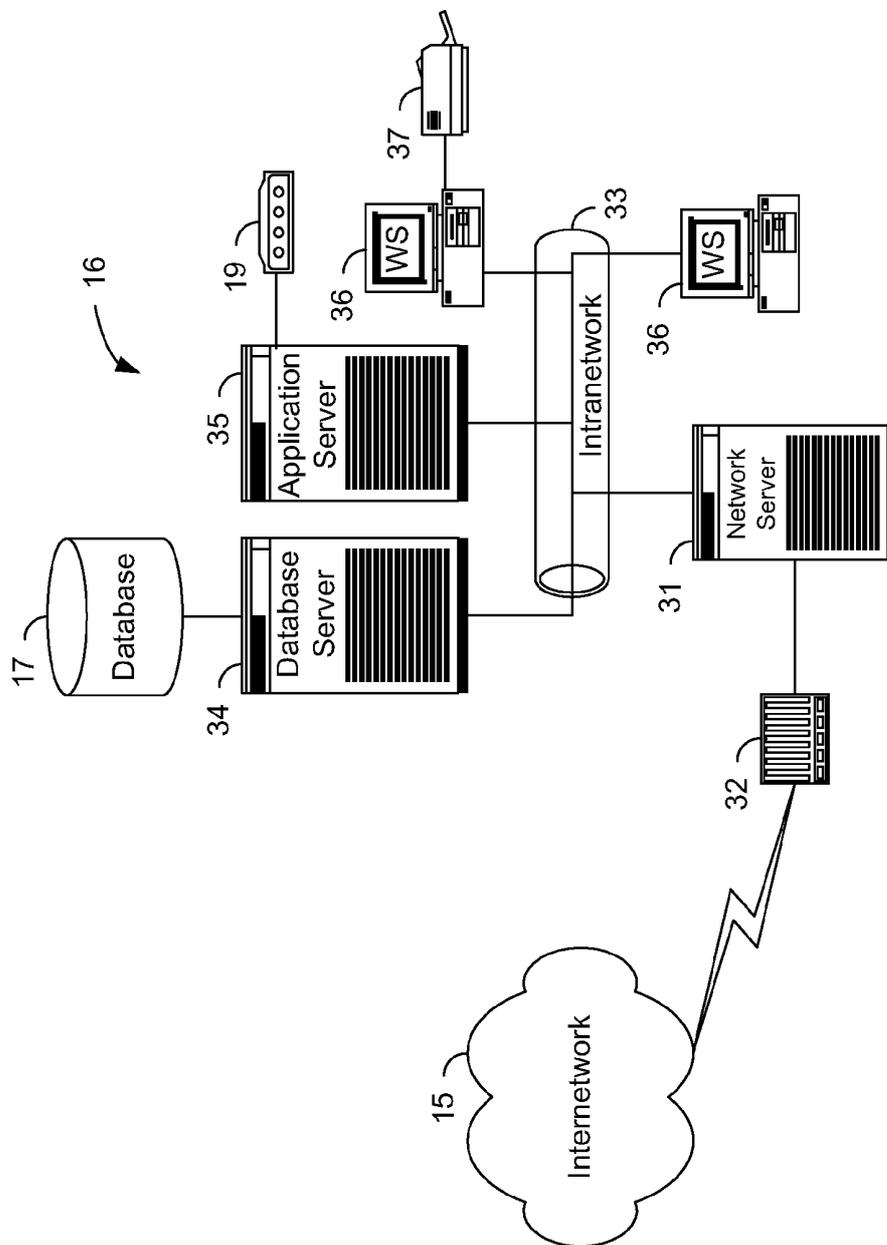


Fig. 3.

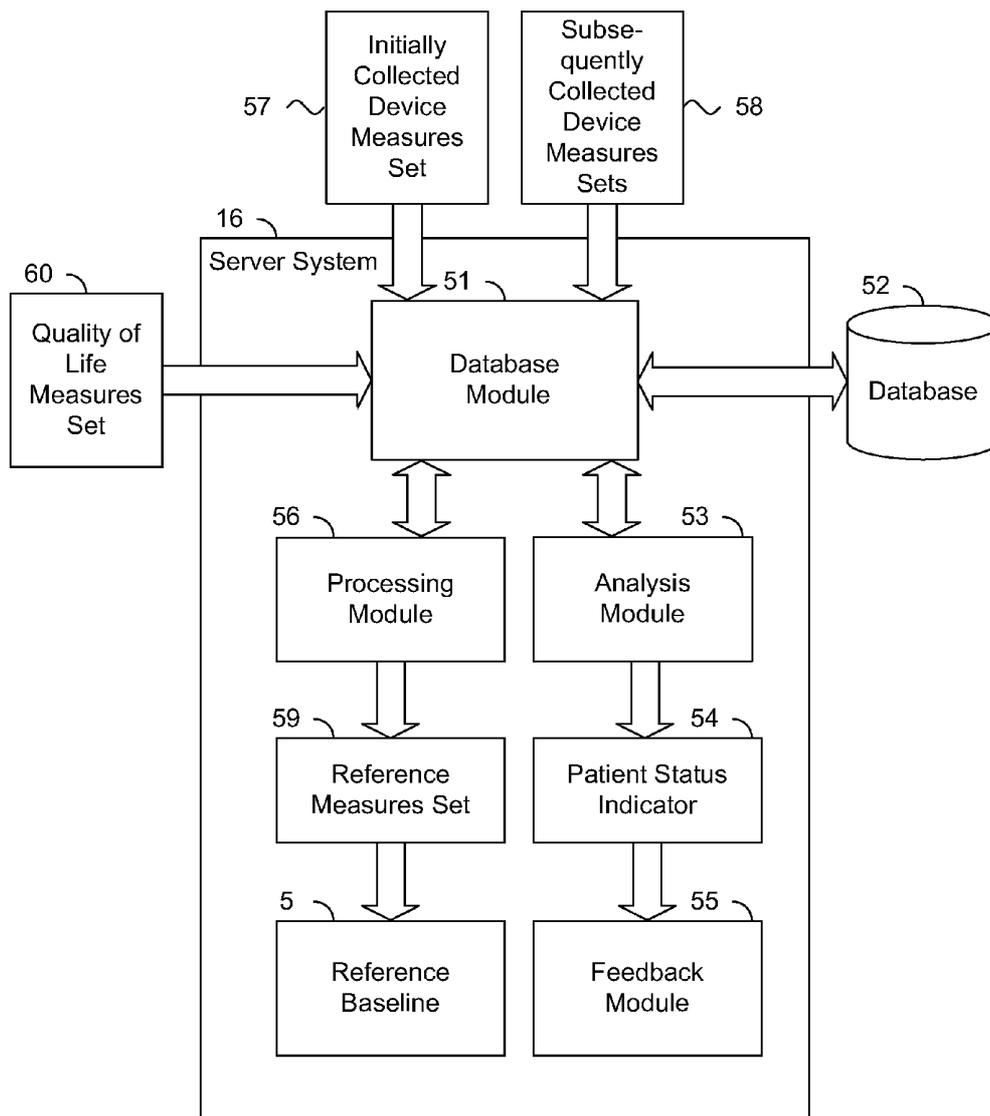


Fig. 4.

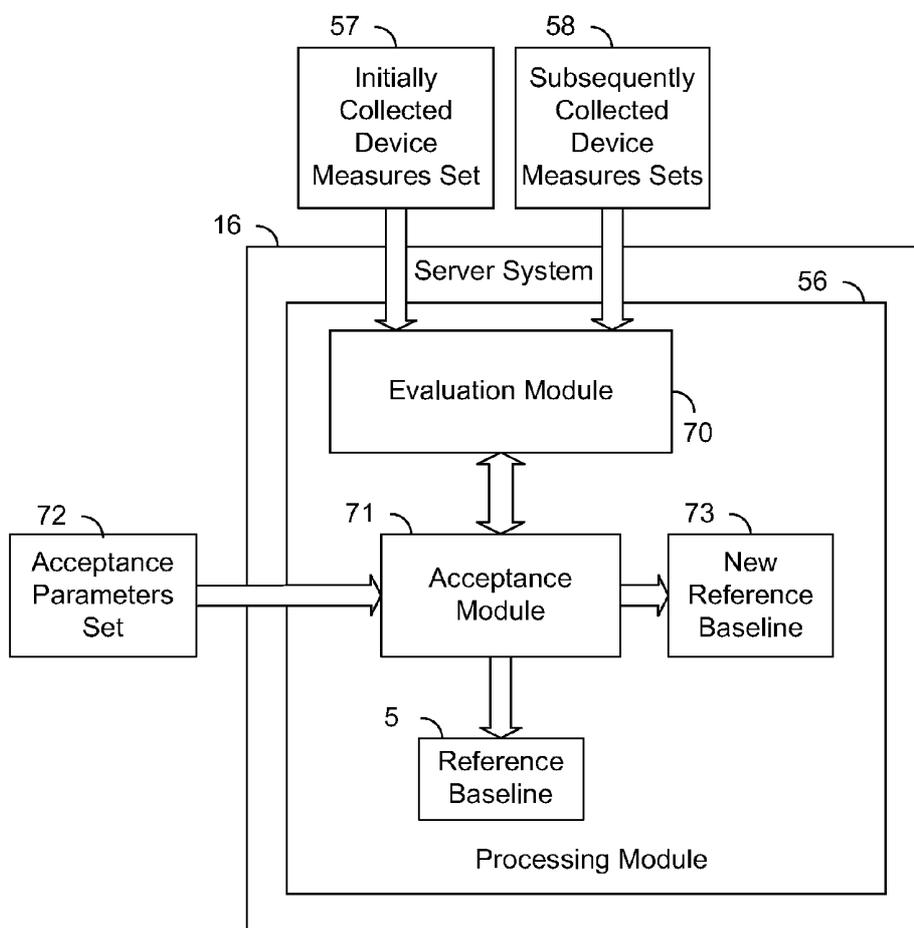


Fig. 5.

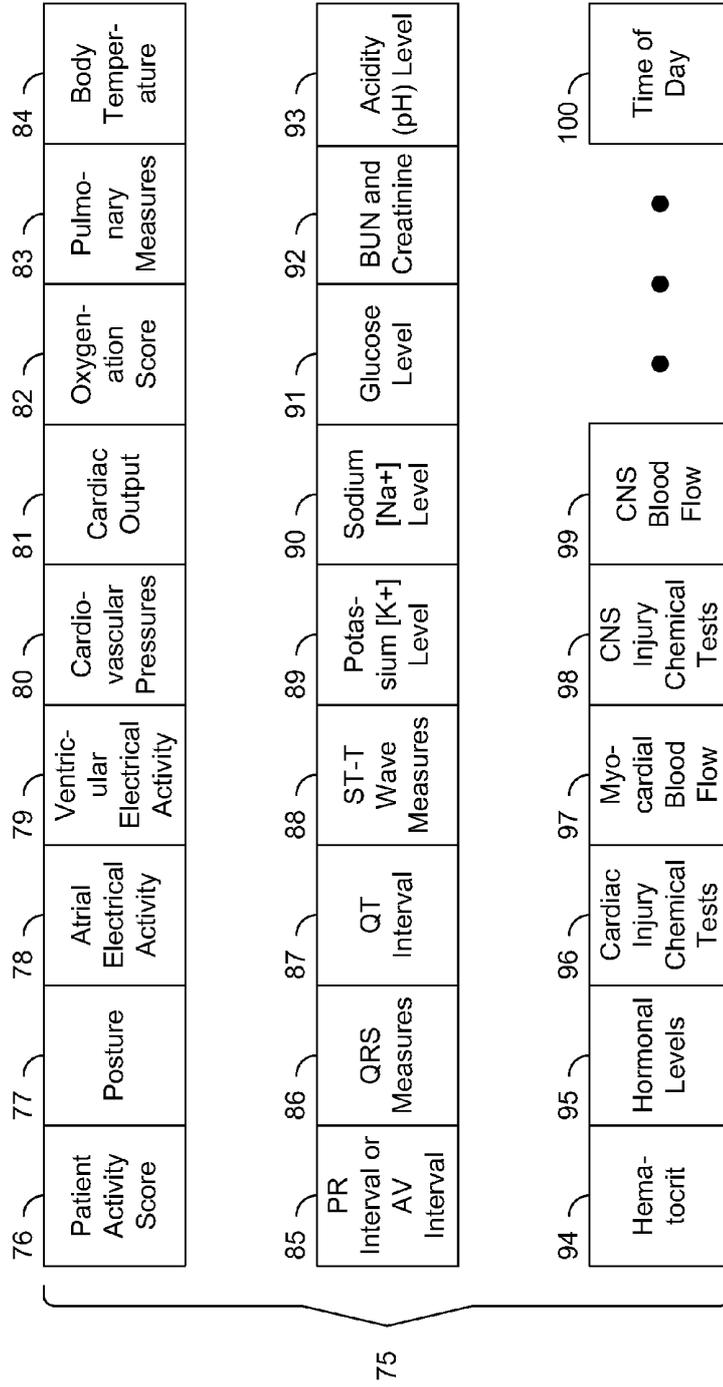


Fig. 6.

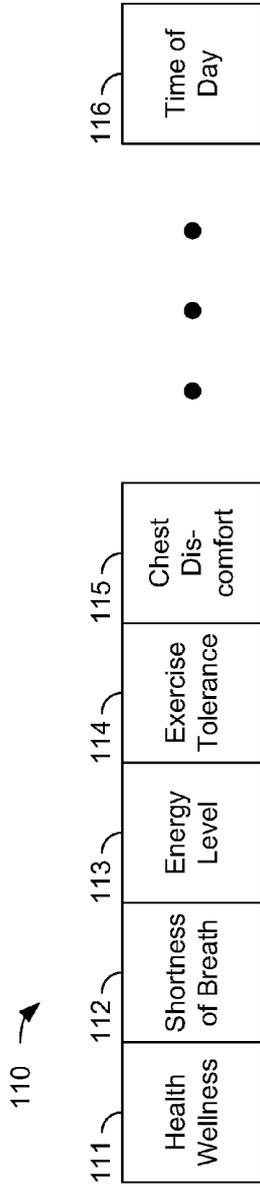


Fig. 7.

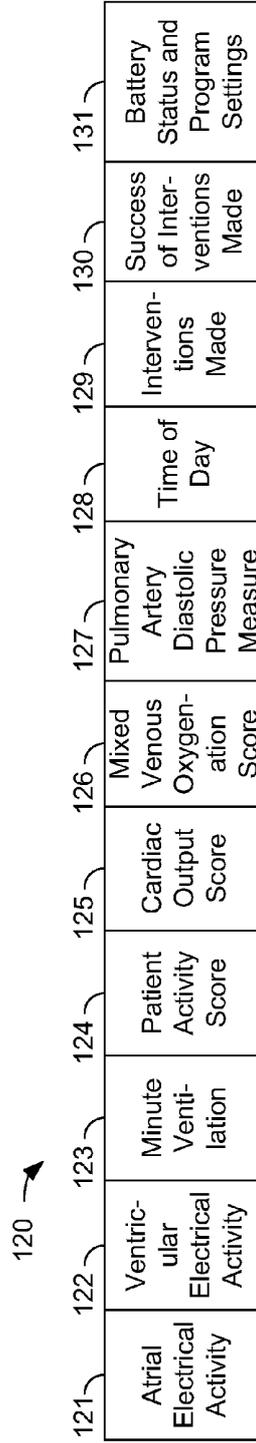


Fig. 8A.

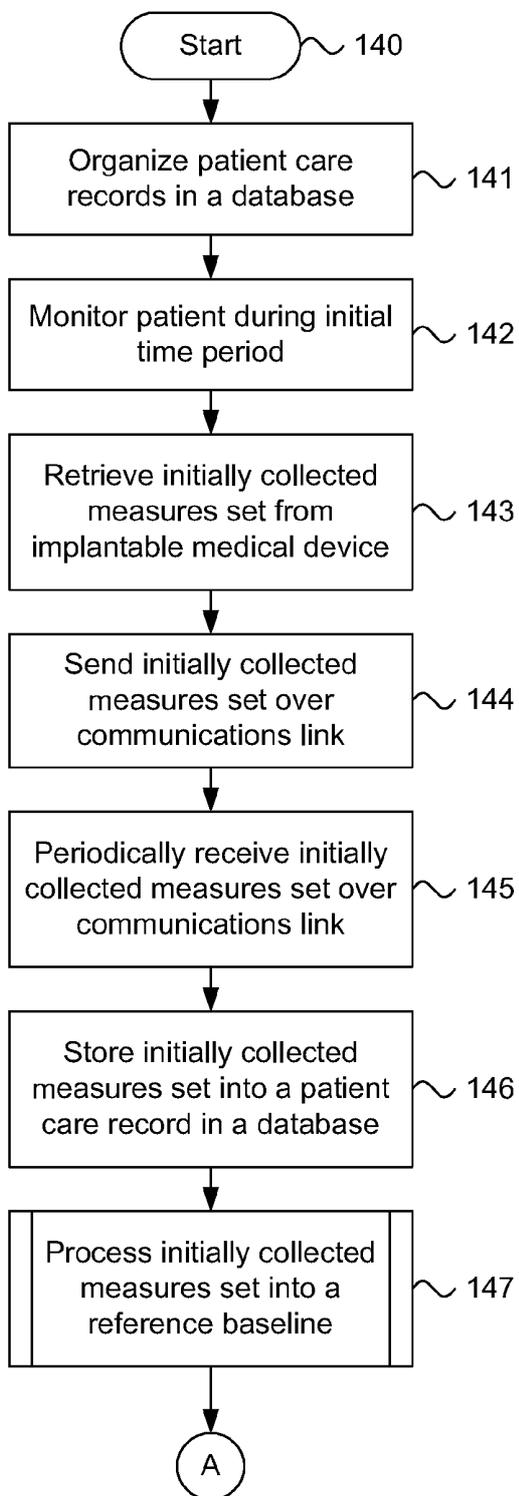


Fig. 8B.

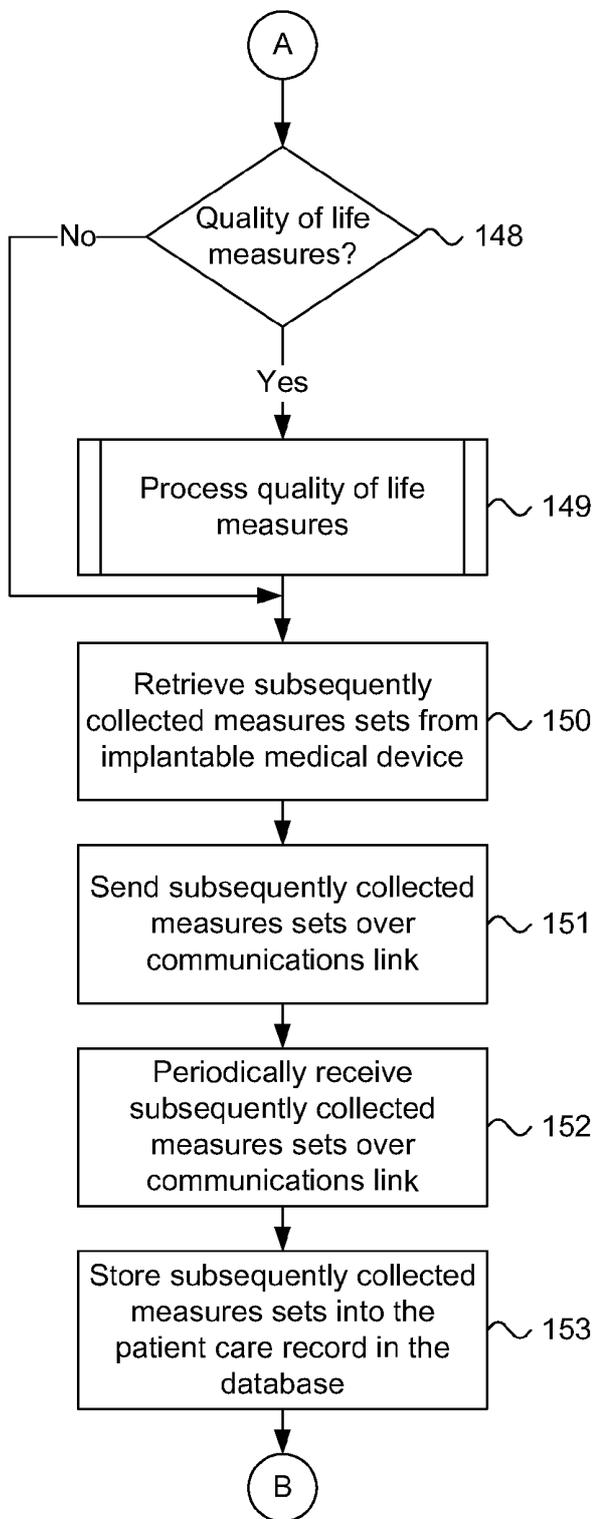


Fig. 8C.

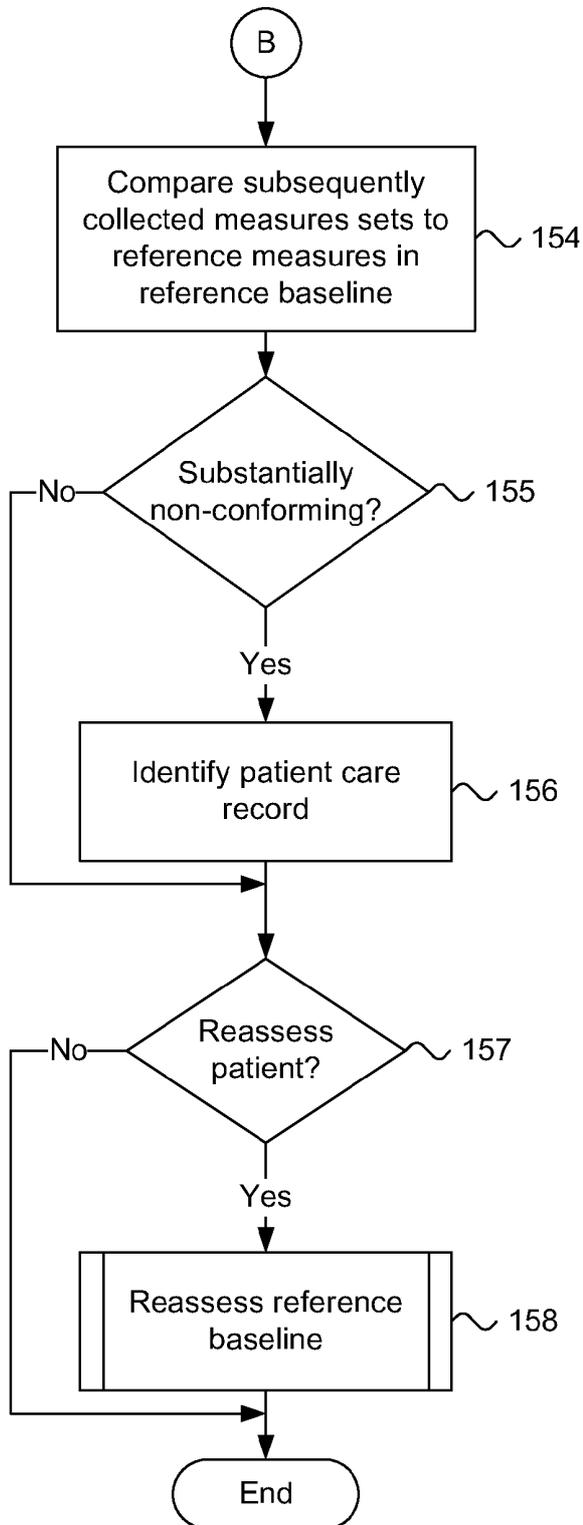


Fig. 9.

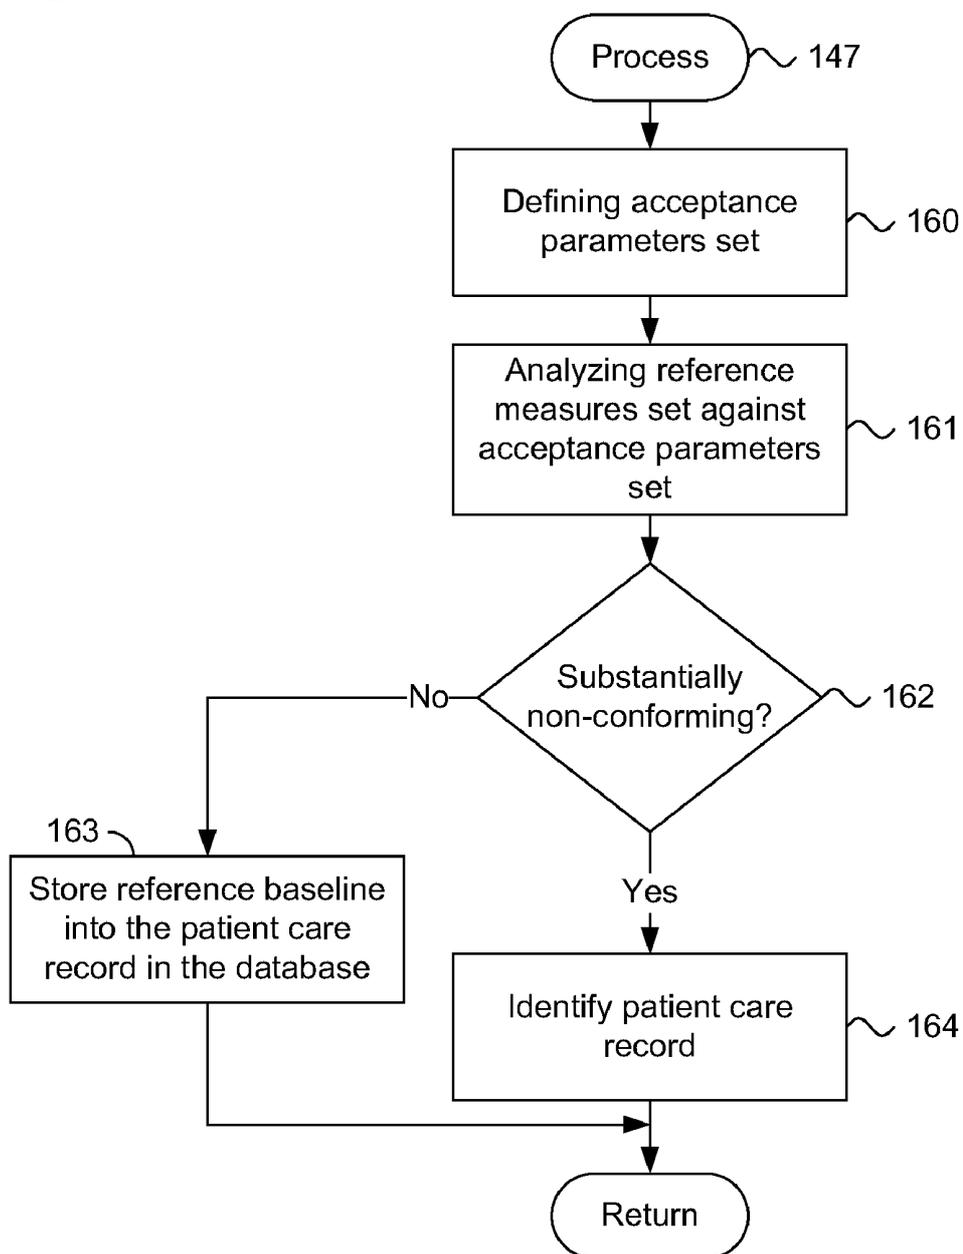


Fig. 10.


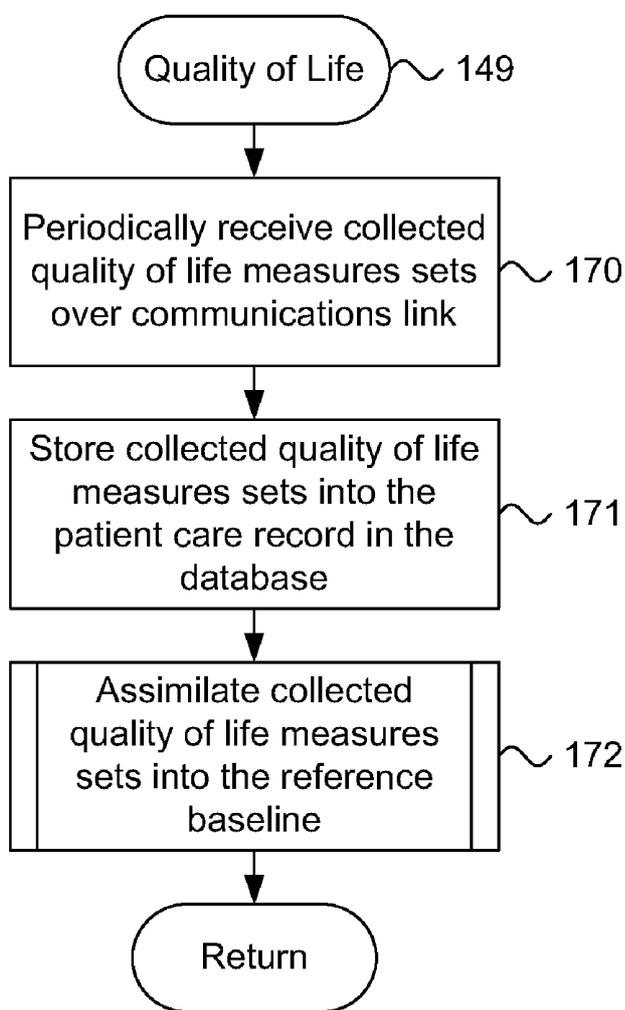


Fig. 11.

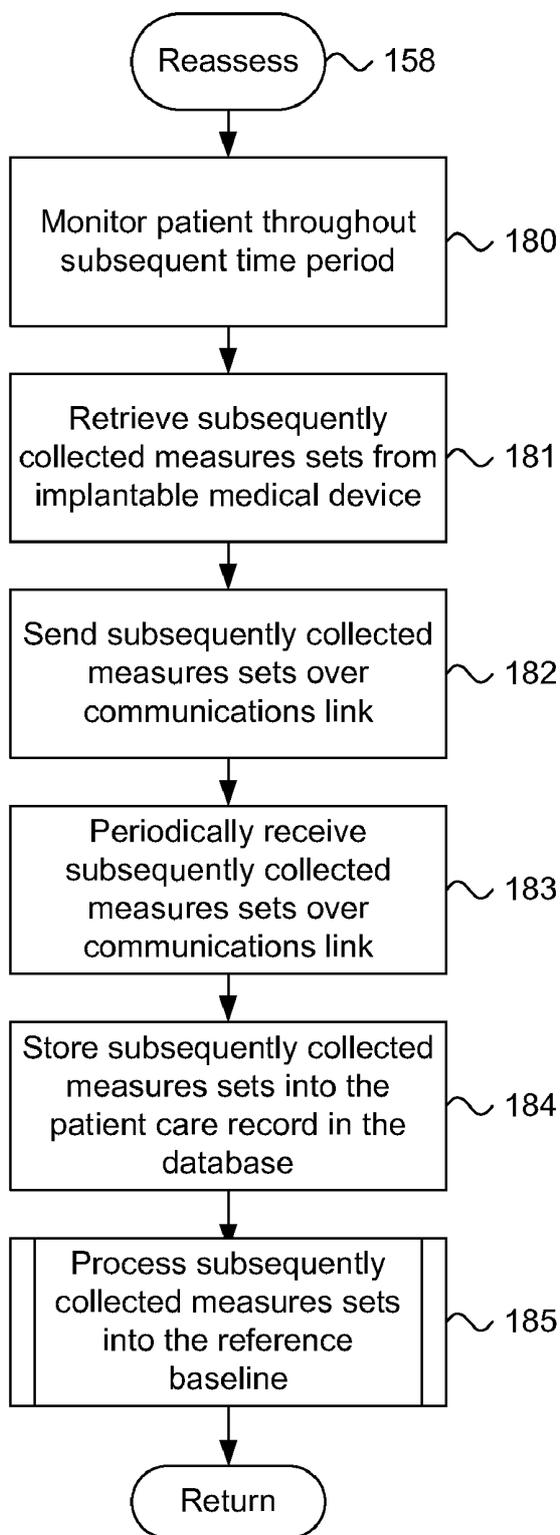

# SYSTEM AND METHOD FOR GENERATING BASELINE DATA FOR AUTOMATED MANAGEMENT OF CARDIOVASCULAR PRESSURE

## CROSS-REFERENCE TO RELATED APPLICATION

This patent application is a continuation of U.S. patent application Ser. No. 11/635,205, filed Dec. 6, 2006, now U.S. Pat. No. 7,837,629, which is a continuation of Ser. No. 09/789,416, filed Feb. 20, 2001 now U.S. Pat. No. 7,248,916, issued Jul. 24, 2007, which is a continuation of Ser. No. 09/361,332, filed Jul. 26, 1999 now U.S. Pat. No. 6,221,011, issued Apr. 24, 2001, the disclosures of which are incorporated by reference, and the priority filing dates of which are claimed.

## FIELD OF THE INVENTION

The present invention relates in general to automated data collection and analysis, and, in particular, to a system and method for determining a reference baseline of individual patient status for use in an automated collection and analysis patient care system.

## BACKGROUND OF THE INVENTION

Implantable pulse generators (IPGs) are medical devices commonly used to treat irregular heartbeats, known as arrhythmias. There are three basic types. Cardiac pacemakers are used to manage bradycardia, an abnormally slow or irregular heartbeat. Bradycardia can cause symptoms such as fatigue, dizziness, and fainting. Implantable cardioverter defibrillators (ICDs) are used to treat tachycardia, heart rhythms that are abnormally fast and life threatening. Tachycardia can result in sudden cardiac death (SCD). Implantable cardiovascular monitors and therapeutic devices are used to monitor and treat structural problems of the heart, such as congestive heart failure, as well as rhythm problems.

Pacemakers and ICDs are equipped with an on-board, volatile memory in which telemetered signals can be stored for later retrieval and analysis. In addition, a growing class of cardiac medical devices, including implantable heart failure monitors, implantable event monitors, cardiovascular monitors, and therapy devices, are being used to provide similar stored device information. These devices are able to store more than thirty minutes of per heartbeat data. Typically, the telemetered signals can provide patient device information recorded on a per heartbeat, binned average basis, or derived basis from, for example, atrial electrical activity, ventricular electrical activity, minute ventilation, patient activity score, cardiac output score, mixed venous oxygen score, cardiovascular pressure measures, time of day, and any interventions and the relative success of such interventions. Telemetered signals are also stored in a broader class of monitors and therapeutic devices for other areas of medicine, including metabolism, endocrinology, hematology, neurology, muscular disorders, gastroenterology, urology, ophthalmology, otolaryngology, orthopedics, and similar medical subspecialties.

These telemetered signals can be remotely collected and analyzed using an automated patient care system. One such system is described in a related, commonly-owned U.S. Pat. No. 6,312,378, issued Nov. 6, 2001. The telemetered signals are recorded by an implantable medical device, such as an IPG or monitor, and periodically retrieved using an interrogator, programmer, telemetered signals transceiver, or similar

device, for subsequent download. The downloaded telemetered signals are received by a network server on a regular, e.g., daily, basis as sets of collected measures which are stored along with other patient records in a database. The information is analyzed in an automated fashion and feedback, which includes a patient status indicator, is provided to the patient.

While such a system can serve as a valuable tool in automated, remote patient care, the accuracy of the patient care, particularly during the first few weeks of care, and the quality of the feedback provided to the patient would benefit from being normalized to a reference baseline of patient wellness. In particular, a starting point needs to be established for each individual patient for use in any such system in which medical device information, such as telemetered signals from implantable medical devices, is continuously monitored, collected, and analyzed. The starting point could serve as a reference baseline indicating overall patient status and wellness from the outset of remote patient care.

In addition, automated remote patient care poses a further challenge vis-à-vis evaluating quality of life issues. Unlike in a traditional clinical setting, physicians participating in providing remote patient care are not able to interact with their patients in person. Consequently, quality of life measures, such as how the patient subjectively looks and feels, whether the patient has shortness of breath, can work, can sleep, is depressed, is sexually active, can perform activities of daily life, and so on, cannot be implicitly gathered and evaluated.

Reference baseline health assessments are widely used in conventional patient health care monitoring services. Typically, a patient's vital signs, consisting of heart rate, blood pressure, weight, and blood sugar level, are measured both at the outset of care and periodically throughout the period of service. However, these measures are limited in their usefulness and do not provide the scope of detailed medical information made available through implantable medical devices. Moreover, such measures are generally obtained through manual means and do not ordinarily directly tie into quality of life assessments. Further, a significant amount of time generally passes between the collection of sets of these measures.

Thus, there is a need for an approach to determining a meaningful reference baseline of individual patient status for use in a system and method for providing automated, remote patient care through the continuous monitoring and analysis of patient information retrieved from an implantable medical device. Preferably, such an approach would establish the reference baseline through initially received measures or after a reasonable period of observation. The reference baseline could be tied to the completion of a set of prescribed physical stressors. Periodic reassessments should be obtainable as necessary. Moreover, the reference baseline should preferably be capable of correlation to quality of life assessments.

There is a further need for an approach to monitoring patient wellness based on a reference baseline for use in an automated patient care system. Preferably, such an approach would dynamically determine whether the patient is trending into an area of potential medical concern.

There is a further need for an approach to determining a situation in which remote patient care is inappropriate based on a reference baseline of patient wellness. Preferably, such an approach would include a range of acceptance parameters as part of the reference baseline, thereby enabling those potential patients whose reference baseline falls outside those acceptance parameters to be identified.

## SUMMARY OF THE INVENTION

The present invention provides a system and method for generating baseline data for automated management of car-

diovascular pressure. The patient device information relates to individual measures recorded by and retrieved from implantable medical devices, such as IPGs and monitors. The patient device information is received on a regular, e.g., daily, basis as sets of collected measures, which are stored along with other patient records in a database. The information can be analyzed in an automated fashion and feedback provided to the patient at any time and in any location.

An embodiment is a system and method for generating baseline data for automated management of cardiovascular pressure. Collected device measures are accumulated to record raw physiometry for a patient, wherein the patient is regularly monitored by an implantable medical device, beginning with an initial observation period. Derived device measures are generated to provide derivative physiometry determined at least in part from the collected device measures. A patient status indicator is determined by analyzing the collected and derived device measures to diagnose a pathophysiology indicative of an absence, onset, progression, regression, and status quo in cardiovascular pressure, wherein the collected and derived device measures and the patient status indicator originating from the initial observation period include baseline data.

The present invention provides a meaningful, quantitative measure of patient wellness for use as a reference baseline in an automated system and method for continuous, remote patient care. The reference baseline increases the accuracy of remote patient care, particularly during the first few weeks of care, by providing a grounded starting assessment of the patient's health and well-being.

A collateral benefit of the reference baseline is the removal of physician "bias" which can occur when the apparent normal outward appearance of a patient belies an underlying condition that potentially requires medical attention. The reference baseline serves to objectify a patient's self-assessment of wellness.

The present invention also provides an objective approach to humanizing the raw measures recorded by medical devices, including implantable medical devices. Using known quality of life assessment instruments, a patient can be evaluated and scored for relative quality of life at a given point in time. The reference baseline of the present invention provides a means for correlating the quality of life assessment to machine-recorded measures, thereby assisting a physician in furthering patient care.

Finally, the present invention improves the chronicling of legal responsibility in patient care. A prescribed course of treatment can be traced back to a grounded point in time memorialized by the reference baseline. Thus, a medical audit trail can be generated with a higher degree of accuracy and certainty based on having an established originating point of reference.

Still other embodiments of the present invention will become readily apparent to those skilled in the art from the following detailed description, wherein is described embodiments of the invention by way of illustrating the best mode contemplated for carrying out the invention. As will be realized, the invention is capable of other and different embodiments and its several details are capable of modifications in various obvious respects, all without departing from the spirit and the scope of the present invention. Accordingly, the drawings and detailed description are to be regarded as illustrative in nature and not as restrictive.

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1A and 1B are block diagrams showing a system for determining a reference baseline of individual patient status

for use in an automated collection and analysis patient care system in accordance with the present invention;

FIG. 2 is a block diagram showing the hardware components of the server system of the system of FIG. 1A;

FIG. 3 is a block diagram showing the software modules of the server system of the system of FIG. 1A;

FIG. 4 is a block diagram showing the processing module of the server system of FIG. 1A;

FIG. 5 is a database schema showing, by way of example, the organization of a reference baseline record for cardiac patient care stored as part of a patient care record in the database of the system of FIG. 1A;

FIG. 6 is a database schema showing, by way of example, the organization of a reference baseline quality of life record for cardiac patient care stored as part of a patient care record in the database of the system of FIG. 1A;

FIG. 7 is a database schema showing, by way of example, the organization of a monitoring record for cardiac patient care stored as part of a patient care record in the database of the system of FIG. 1A;

FIGS. 8A-8C are flow diagrams showing a method for determining a reference baseline for use in monitoring a patient status in an automated collection and analysis patient care system in accordance with the present invention; and

FIG. 9 is a flow diagram showing the routine for processing a reference baseline for use in the method of FIGS. 8A-8C;

FIG. 10 is a flow diagram showing the routine for processing quality of life measures for use in the method of FIGS. 8A-8C; and

FIG. 11 is a flow diagram showing the routine for reassessing a new reference baseline for use in the method of FIGS. 8A-8C.

#### DETAILED DESCRIPTION

FIG. 1A is a block diagram showing a system 10 for determining a reference baseline 5 of patient status for an individual patient 11 for use in an automated collection and analysis patient care system in accordance with the present invention. An automated collection and analysis patient care system suitable for use with the present invention is disclosed in the related, commonly-owned U.S. Pat. No. 6,312,378, issued Nov. 6, 2001, the disclosure of which is incorporated herein by reference. A patient 11 is a recipient of an implantable medical device 12, such as, by way of example, an IPG or a heart failure or event monitor, with a set of leads extending into his or her heart. Alternatively, subcutaneous monitors or devices inserted into other organs (not shown) without leads could also be used. The implantable medical device 12 includes circuitry for recording into a short-term, volatile memory telemetered signals, which are stored as a set of collected measures for later retrieval.

For an exemplary cardiac implantable medical device, the telemetered signals non-exclusively present patient information recorded on a per heartbeat, binned average or derived basis and relating to: atrial electrical activity, ventricular electrical activity, minute ventilation, patient activity score, cardiac output score, mixed venous oxygenation score, cardiovascular pressure measures, time of day, the number and types of interventions made, and the relative success of any interventions, plus the status of the batteries and programmed settings. Examples of pacemakers suitable for use in the present invention include the Discovery line of pacemakers, manufactured by Guidant Corporation, Indianapolis, Ind. Examples of ICDs suitable for use in the present invention include the Gem line of ICDs, manufactured by Medtronic Corporation, Minneapolis, Minn.

In the described embodiment, the patient **11** has a cardiac implantable medical device. However, a wide range of related implantable medical devices are used in other areas of medicine and a growing number of these devices are also capable of measuring and recording patient information for later retrieval. These implantable medical devices include monitoring and therapeutic devices for use in metabolism, endocrinology, hematology, neurology, muscular disorders, gastroenterology, urology, ophthalmology, otolaryngology, orthopedics, and similar medical subspecialties. One skilled in the art would readily recognize the applicability of the present invention to these related implantable medical devices.

The telemetered signals stored in the implantable medical device **12** are retrieved upon completion of an initial observation period and subsequently retrieved on a continuous, periodic basis. By way of example, a programmer **14** can be used to retrieve the telemetered signals. However, any form of programmer, interrogator, recorder, monitor, or telemetered signals transceiver suitable for communicating with an implantable medical device **12** could be used, as is known in the art. In addition, a personal computer or digital data processor could be interfaced to the implantable medical device **12**, either directly or via a telemetered signals transceiver configured to communicate with the implantable medical device **12**.

Using the programmer **14**, a magnetized reed switch (not shown) within the implantable medical device **12** closes in response to the placement of a wand **14** over the location of the implantable medical device **12**. The programmer **14** communicates with the implantable medical device **12** via RF signals exchanged through the wand **14**. Programming or interrogating instructions are sent to the implantable medical device **12** and the stored telemetered signals are downloaded into the programmer **14**. Once downloaded, the telemetered signals are sent via an internetwork **15**, such as the Internet, to a server system **16** which periodically receives and stores the telemetered signals in a database **17**, as further described below with reference to FIG. 2.

An example of a programmer **14** suitable for use in the present invention is the Model 2901 Programmer Recorder Monitor, manufactured by Guidant Corporation, Indianapolis, Ind., which includes the capability to store retrieved telemetered signals on a proprietary removable floppy diskette. The telemetered signals could later be electronically transferred using a personal computer or similar processing device to the internetwork **15**, as is known in the art.

Other alternate telemetered signals transfer means could also be employed. For instance, the stored telemetered signals could be retrieved from the implantable medical device **12** and electronically transferred to the internetwork **15** using the combination of a remote external programmer and analyzer and a remote telephonic communicator, such as described in U.S. Pat. No. 5,113,869, the disclosure of which is incorporated herein by reference. Similarly, the stored telemetered signals could be retrieved and remotely downloaded to the server system **16** using a world-wide patient location and data telemetry system, such as described in U.S. Pat. No. 5,752,976, the disclosure of which is incorporated herein by reference.

The initial set of telemetered signals recorded during the initial observation period is processed by the server system **16** into a set of reference measures and stored as a reference baseline **5** in the database **17**, as further described below with reference to FIG. 3. The purpose of the observation period is to establish a reference baseline **5** containing a set of reference measures that can include both measured and derived

patient information. The reference baseline **5** can link "hard" machine-recorded data with "soft" patient-provided self-assessment data from which can be generated a wellness status indicator. In addition, the reference baseline **5** can be used to identify patients for whom remote patient care may be inappropriate and for patient wellness comparison and analysis during subsequent, on-going remote patient care. The reference baseline **5** is maintained in the database **17** and can be reassessed as needed or on a periodic basis.

Subsequent to the initial observation period, the patient is remotely monitored by the server system **16** through the periodic receipt of telemetered signals from the implantable medical device **12** via the internetwork **15**. Feedback is then provided back to the patient **11** through a variety of means. By way of example, the feedback can be sent as an electronic mail message generated automatically by the server system **16** for transmission over the internetwork **15**. The electronic mail message is received by personal computer **18** (PC) situated for local access by the patient **11**. Alternatively, the feedback can be sent through a telephone interface device **19** as an automated voice mail message to a telephone **21** or as an automated facsimile message to a facsimile machine **22**, both also situated for local access by the patient **11**. In addition to a personal computer **18**, telephone **21**, and facsimile machine **22**, feedback could be sent to other related devices, including a network computer, wireless computer, personal data assistant, television, or digital data processor.

FIG. 1B is a block diagram showing a further embodiment of the present invention in which the patient **11** is monitored by the implantable medical device **12** while engaged in performing a prescribed set of timed physical stressors during an initial observation period or during a subsequent observation period if the patient **11** is being reassessed. The stressors are a set of normal, patient activities and cardiovascular and respiratory maneuvers that allow consistent, reproducible physiological functions to be measured by the implantable medical device **12**. These maneuvers include activities such as a change in posture, simple physical exercises, breathing state, including holding breath and hyperventilating, and oxygen challenges. By way of example, the stressors include timed physical activities such as running in place **6**, recumbency **7**, standing **8**, sitting motionless **9**, and reprogramming at least one of pacing interventions and pacing modes of the implantable medical device **12**, as further described below with reference to FIG. 5.

In a still further embodiment of the present invention, at least one of pacing interventions and pacing modes of the implantable medical device **12** is reprogrammed by the programmer **14** during the initial observation period or during a subsequent observation period if the patient **11** is being reassessed. The patient **11** is then monitored by the reprogrammed implantable medical device **12**.

FIG. 2 is a block diagram showing the hardware components of the server system **16** of the system **10** of FIG. 1A. The server system **16** consists of three individual servers: network server **31**, database server **34**, and application server **35**. These servers are interconnected via an intranetwork **33**. In the described embodiment, the functionality of the server system **16** is distributed among these three servers for efficiency and processing speed, although the functionality could also be performed by a single server or cluster of servers. The network server **31** is the primary interface of the server system **16** onto the internetwork **15**. The network server **31** periodically receives the collected telemetered signals sent by remote implantable medical devices over the internetwork **15**. The network server **31** is interfaced to the internetwork **15** through a router **32**. To ensure reliable data exchange, the

network server **31** implements a TCP/IP protocol stack, although other forms of network protocol stacks are suitable.

The database server **34** organizes the patient care records in the database **17** and provides storage of and access to information held in those records. A high volume of data in the form of collected device measures sets from individual patients is received. The database server **34** frees the network server **31** from having to categorize and store the individual collected device measures sets in the appropriate patient care record.

The application server **35** operates management applications, assimilates the reference measures into the reference baseline **5** (shown in FIG. 1A), and performs data analysis of the patient care records, as further described below with reference to FIG. 3. The application server **35** communicates feedback to the individual patients either through electronic mail sent back over the internetwork **15** via the network server **31** or as automated voice mail or facsimile messages through the telephone interface device **19**.

The server system **16** also includes a plurality of individual workstations **36** (WS) interconnected to the intranetwork **33**, some of which can include peripheral devices, such as a printer **37**. The workstations **36** are for use by the data management and programming staff, nursing staff, office staff, and other consultants and authorized personnel.

The database **17** consists of a high-capacity storage medium configured to store individual patient care records and related health care information. Preferably, the database **17** is configured as a set of high-speed, high capacity hard drives, such as organized into a Redundant Array of Inexpensive Disks (RAID) volume. However, any form of volatile storage, non-volatile storage, removable storage, fixed storage, random access storage, sequential access storage, permanent storage, erasable storage, and the like would be equally suitable. The organization of the database **17** is further described below with reference to FIGS. 5-7.

The individual servers and workstations are general purpose, programmed digital computing devices consisting of a central processing unit (CPU), random access memory (RAM), non-volatile secondary storage, such as a hard drive or CD ROM drive, network interfaces, and peripheral devices, including user interfacing means, such as a keyboard and display. Program code, including software programs, and data are loaded into the RAM for execution and processing by the CPU and results are generated for display, output, transmittal, or storage. In the described embodiment, the individual servers are Intel Pentium-based server systems, such as available from Dell Computers, Austin, Tex., or Compaq Computers, Houston, Tex. Each system is preferably equipped with 128 MB RAM, 100 GB hard drive capacity, data backup facilities, and related hardware for interconnection to the intranetwork **33** and internetwork **15**. In addition, the workstations **36** are also Intel Pentium-based personal computer or workstation systems, also available from Dell Computers, Austin, Tex., or Compaq Computers, Houston, Tex. Each workstation is preferably equipped with 64 MB RAM, 10 GB hard drive capacity, and related hardware for interconnection to the intranetwork **33**. Other types of server and workstation systems, including personal computers, minicomputers, mainframe computers, supercomputers, parallel computers, workstations, digital data processors and the like would be equally suitable, as is known in the art.

The telemetered signals are communicated over an internetwork **15**, such as the Internet. However, any type of electronic communications link could be used, including an intranetwork link, serial link, data telephone link, satellite link, radio-frequency link, infrared link, fiber optic link, coaxial

cable link, television link, and the like, as is known in the art. Also, the network server **31** is interfaced to the internetwork **15** using a T-1 network router **32**, such as manufactured by Cisco Systems, Inc., San Jose, Calif. However, any type of interfacing device suitable for interconnecting a server to a network could be used, including a data modem, cable modem, network interface, serial connection, data port, hub, frame relay, digital PBX, and the like, as is known in the art.

FIG. 3 is a block diagram showing the software modules of the server system **16** of the system **10** of FIG. 1A. Each module is a computer program written as source code in a conventional programming language, such as the C or Java programming languages, and is presented for execution by the CPU as object or byte code, as is known in the art. The various implementations of the source code and object and byte codes can be held on a computer-readable storage medium or embodied on a transmission medium in a carrier wave.

There are three basic software modules, which functionally define the primary operations performed by the server system **16**: database module **51**, analysis module **53**, and processing module **56**. In the described embodiment, these modules are executed in a distributed computing environment, although a single server or a cluster of servers could also perform the functionality of these modules. The module functions are further described below beginning with reference to FIGS. 8A-8C.

A reference baseline **5** is established at the outset of providing a patient with remote patient care. The server system **16** periodically receives an initially collected device measures set **57**. This set represents patient information, which was collected from the implantable medical device **12** (shown in FIG. 1A) during the initial observation period, as further discussed below with reference to FIG. 5. In addition, the server system **16** can also periodically receive quality of life measures sets **60** recorded by the patient **11**, as further described below with reference to FIG. 6. Both the initially collected device measures set **57** and quality of life measures set **60** are forwarded to the database module **51** for storage in the patient's patient care record in the database **52**. During subsequent, on-going monitoring for remote patient care, the server system **16** periodically receives subsequently collected device measures sets **58**, which are also forwarded to the database module **51** for storage.

The database module **51** organizes the individual patient care records stored in the database **52** and provides the facilities for efficiently storing and accessing the collected device measures sets **57**, **58** and patient data maintained in those records. Exemplary database schemes for use in storing the initially collected device measures set **57**, quality of life measures set **60**, and subsequently collected device measures sets **58** in a patient care record are described below, by way of example, with reference to FIGS. 5-7. The database server **34** (shown in FIG. 2) performs the functionality of the database module **51**. Any type of database organization could be utilized, including a flat file system, hierarchical database, relational database, or distributed database, such as provided by database vendors, such as Oracle Corporation, Redwood Shores, Calif.

The processing module **56** processes the initially collected device measures set **57** and, if available, the quality of life measures set **60**, stored in the patient care records in the database **52** into the reference baseline **5**. The reference baseline **5** includes a set of reference measures **59** which can be either directly measured or indirectly derived patient information. The reference baseline **5** can be used to identify

patients for whom remote patient care might be inappropriate and to monitor patient wellness in a continuous, on-going basis.

On a periodic basis or as needed, the processing module 56 reassesses the reference baseline 5. Subsequently collected device measures sets 58 are received from the implantable medical device 12 (shown in FIG. 1A) subsequent to the initial observation period. The processing module 56 re-simulates these additional collected device measures sets into a new reference baseline. The operations performed by the processing module 56 are further described below with reference to FIG. 4. The application server 35 (shown in FIG. 2) performs the functionality of the processing module 56.

The analysis module 53 analyzes the subsequently collected device measures sets 58 stored in the patient care records in the database 52. The analysis module 53 monitors patient wellness and makes an automated determination in the form of a patient status indicator 54. Subsequently collected device measures sets 58 are periodically received from implantable medical devices and maintained by the database module 51 in the database 52. Through the use of this collected information, the analysis module 53 can continuously follow the medical well being of a patient and can recognize any trends in the collected information that might warrant medical intervention. The analysis module 53 compares individual measures and derived measures obtained from both the care records for the individual patient and the care records for a disease specific group of patients or the patient population in general. The analytic operations performed by the analysis module 53 are further described below with reference to FIG. 4. The application server 35 (shown in FIG. 2) performs the functionality of the analysis module 53.

The feedback module 55 provides automated feedback to the individual patient based, in part, on the patient status indicator 54. As described above, the feedback could be by electronic mail or by automated voice mail or facsimile. Preferably, the feedback is provided in a tiered manner. In the described embodiment, four levels of automated feedback are provided. At a first level, an interpretation of the patient status indicator 54 is provided. At a second level, a notification of potential medical concern based on the patient status indicator 54 is provided. This feedback level could also be coupled with human contact by specially trained technicians or medical personnel. At a third level, the notification of potential medical concern is forwarded to medical practitioners located in the patient's geographic area. Finally, at a fourth level, a set of reprogramming instructions based on the patient status indicator 54 could be transmitted directly to the implantable medical device to modify the programming instructions contained therein. As is customary in the medical arts, the basic tiered feedback scheme would be modified in the event of bona fide medical emergency. The application server 35 (shown in FIG. 2) performs the functionality of the feedback module 55.

FIG. 4 is a block diagram showing the processing module 56 of the server system 16 of FIG. 1A. The processing module 53 contains two functional submodules: evaluation module 70 and acceptance module 71. The purpose of the evaluation module 70 is to process the initially collected device measures set 57 by determining any derived measures and calculating appropriate statistical values, including means and standard deviations, for the reference measures set 59 in the reference baseline 5. The purpose of the acceptance module 71 is to analyze the reference measures set 59 against the acceptance parameters set 72. A patient care record storing a reference measures set 59 substantially out of conformity with the acceptance parameters set 72 could be indicative of

a patient for whom remote patient care is inappropriate. Consequently, the acceptance module 71 identifies each patient care record storing at least one reference measure which is substantially non-conforming to a corresponding parameter in the acceptance parameters set 72.

For instance, an acceptance parameter for heart rate might be specified as a mean heart rate within a range of 40-90 beats per minute (bpm) over a 24-hour period. However, a patient care record storing a reference measure falling either substantially above or below this acceptance parameter, for example, in excess of 90 bpm, would be considered substantially non-conforming. The acceptance parameters set 72 are further described below with reference to FIG. 5.

The evaluation module 70 also determines new reference baselines 73 when necessary. For instance, the new reference baseline 73 might be reassessed on an annual or quarterly basis, as the needs of the patient 11 dictate. Similarly, the new reference baseline 73 might be reassessed for a patient whose patient care record stores a subsequently collected device measures set 58 substantially out of conformity with the reference measures set 59 in the original reference baseline 5. The new reference baseline 73 would be assessed by the processing module 56 using subsequently collected device measures sets 58 during a subsequent observation period.

FIG. 5 is a database schema showing, by way of example, the organization of a reference baseline record 75 for cardiac patient care stored as part of a patient care record in the database 17 of the system 10 of FIG. 1A. The reference baseline record 75 corresponds to the reference baseline 5, although only the information pertaining to the set of reference measures in the reference baseline 5 are shown. Each patient care record would also contain normal identifying and treatment profile information, as well as medical history and other pertinent data (not shown). For instance, during the initial observation period, the patient 11 maintains a diary of activities, including the onset of bedtime and waking time, plus the time and dosing of any medications, including non-prescription drugs. The observation period can be expanded to include additional information about the normal range of patient activities as necessary, including a range of potential anticipated activities as well as expected travel times and periods away from home. In addition, information from any set of medical records could be included in the patient care record. The diary, medication, activity, and medical record information and medical test information (e.g., electrocardiogram, echocardiogram, and/or coronary angiogram) is incorporated into the patient care record and is updated with continuing patient information, such as changes in medication, as is customary in the art.

The reference measures set 59 stored in the reference baseline record 75 are processed from the initial collected device measures set 57 (shown in FIG. 3), as further described below with reference to FIG. 9. The implantable medical device 12 (shown in FIG. 1A) records the initial collected device measures set 57 during the initial observation period. For example, for a cardiac patient, the reference baseline record 75 stores the following information as part of the reference measures set 59: patient activity score 76, posture 77 (e.g., from barometric pressure), atrial electrical activity 78 (e.g., atrial rate), ventricular electrical activity 79 (e.g., ventricular rate), cardiovascular pressures 80, cardiac output 81, oxygenation score 82 (e.g., mixed venous oxygenation), pulmonary measures 83 (e.g., transthoracic impedance, measures of lung wetness, and/or minute ventilation), body temperature 84, PR interval 85 (or AV interval), QRS measures 86 (e.g., width, amplitude, frequency content, and/or morphology), QT interval 87, ST-T wave measures 88 (e.g., T wave alternans or ST

segment depression or elevation), potassium [K+] level **89**, sodium [Na+] level **90**, glucose level **91**, blood urea nitrogen and creatinine **92**, acidity (pH) level **93**, hematocrit **94**, hormonal levels **95** (e.g., insulin, epinephrine), cardiac injury chemical tests **96** (e.g., troponin, myocardial band creatinine kinase), myocardial blood flow **97**, central nervous system injury chemical tests **98** (e.g., cerebral band creatinine kinase), central nervous system (CNS) blood flow **99**, and time of day **100**. Other types of reference measures are possible. In addition, a well-documented set of derived measures can be determined based on the reference measures, as is known in the art.

In the described embodiment, the initial and any subsequent observation periods last for about one 7-day period during which time the patient **11** might be asked to perform, if possible, repeated physical stressors representative of both relatively normal activity and/or activities designed to test the response of the body to modest activity and physiologic perturbations for use as the baseline "reference" measures that might be recorded daily for a period of one week prior to initiating fee-for-service monitoring. Reference measures taken and derived from the observation period are recorded, processed, and stored by the system **10**.

The reference measures include both measured and derived measures, including patient activity score **76**, posture **77**, atrial electrical activity **78**, ventricular electrical activity **79**, cardiovascular pressures **80**, cardiac output **81**, oxygenation score **82**, pulmonary measures **83**, body temperature **84**, PR interval **85** (or AV interval), QRS measures **86**, QT interval **87**, ST-T wave measures **88**, potassium [K+] level **89**, sodium [Na+] level **90**, glucose level **91**, blood urea nitrogen and creatinine **92**, acidity (pH) level **93**, hematocrit **94**, hormonal levels **95**, cardiac injury chemical tests **96**, myocardial blood flow **97**, central nervous system injury chemical tests **98**, central nervous system (CNS) blood flow **99**, and time of day **100**. Other combination and derivative measures can also be determined, as known in the art.

An illustrative prescribed set of timed physical stressors for a non-ambulatory patient **11** is as follows:

- (1) Running in place **6**: if possible, the patient **11** must run in place for about five minutes;
- (2) Walking (not shown): if possible, the patient **11** must walk for about six minutes and the total distance walked is measured;
- (3) Ascending stairs (not shown): if possible, the patient **11** must ascend two flights of stairs;
- (4) Recumbency **7**: if possible, the patient **11** must recline following about two minutes of motionless immobile upright posture. Upon recumbency, the patient **11** must remain as immobile as possible for about ten minutes;
- (5) Standing **8**: if possible, the patient **11** must briskly assume an upright standing posture after the ten-minute recumbency **7** and must remain standing without activity for about five minutes;
- (6) Coughing (not shown): if possible, the patient **11** must cough forcefully about three times when in an upright position to record the cardiovascular pressures **80**;
- (7) Hyperventilation (not shown): if possible, the patient **11** must hyperventilate over thirty seconds with full deep and rapid breaths to record ventilatory status;
- (8) Sitting motionless **9**: when a physician is complicit, the patient **11** must, if possible, use an approximately 2.0 liter per minute nasal cannula while transmitting data for about twenty minutes while sitting to evaluate cardiopulmonary response;

(9) Program AAI and VVI temporary pacing interventions for five minutes, at low and high rates, if applicable (e.g., 40 bpm and 120 bpm) to evaluate cardiopulmonary response; and

(10) Test dual site or biventricular pacing modes, if applicable, for approximately 20 minutes to evaluate cardiopulmonary response.

These physical and pacing stimulus stressors must be annotated with date and time of day **100** and correlated with symptoms and the quality of life measures **110**. Heart rate, temperature, and time of day are directly measured while the patient activity score and cardiac output score are derived. These physical stressors are merely illustrative in nature and the set of physical and pacing stimulus stressors actually performed by any given patient would necessarily depend upon their age and physical condition as well as device implanted. Also, during the observation period, the temperature is monitored with QT interval shortening and, if the patient is in atrial fibrillation, the patient **11** must undergo an incremental ventricular pacing protocol to assess his or her response to rate stabilization. Finally, a T-wave alternans measurement (not shown) can be integrated into the reference baseline **5** during rest and sinus rhythm activities.

In a further embodiment of the present invention, the reference measures set **59** in the reference baseline **5** are reassessed on an annual or, if necessary, quarterly, basis. In addition, if the reference measures set **59** was recorded during a period when the patient **11** was unstable or recovering from a recent illness, the reference baseline **5** is reassessed when the patient **11** is again stable, as further described below with reference to FIG. **11**.

As further described below with reference to FIG. **9**, the reference measures are analyzed against the acceptance parameters set **72**. The acceptance parameters are those indicator values consistent with the presence of some form of chronic yet stable disease which does not require immediate emergency care. In the described embodiment, the acceptance parameters set **72** for the reference measures **59** in the reference baseline record **75** are, by way of example, as follows: cardiac output **81** falling below 2.5 liters/minute/m<sup>2</sup>; heart rate below 40 bpm or above 120 bpm; body temperature **84** over 101° F. and below 97° F.; patient activity **76** score of 1.0 or below; oxygenation score **82** of less than 60% mixed venous saturation at rest; pulmonary artery diastolic pressure greater than 20 mm Hg at rest; and minute ventilation less than 10.0 liters/minute at rest.

FIG. **6** is a database schema showing, by way of example, the organization of a reference baseline quality of life record **110** for cardiac patient care stored as part of a patient care record in the database **17** of the system **10** of FIG. **1A**. A quality of life score is a semi-quantitative self-assessment of an individual patient's physical and emotional well being. Non-commercial, non-proprietary standardized automated quality of life scoring systems are readily available, such as provided by the Duke Activities Status Indicator. These scoring systems can be provided for use by the patient **11** on the personal computer **18** (shown in FIG. **1A**) and the patient **11** can then record his or her quality of life scores for periodic download to the server system **16**.

For example, for a cardiac patient, the reference baseline quality of life record **110** stores the following information as part of the reference measures set **59**: health wellness **111**, shortness of breath **112**, energy level **113**, exercise tolerance **114**, chest discomfort **115**, time of day **116**, and other quality of life measures as would be known to one skilled in the art. Using the quality of life scores **111-116** in the reference baseline quality of life record **110**, the patient **11** can be

notified automatically when variable physiological changes matches his or her symptomatology.

A quality of life indicator is a vehicle through which a patient can remotely communicate to the patient care system how he or she is subjectively feeling. When tied to machine-recorded physiological measures, a quality of life indicator can provide valuable additional information to medical practitioners and the automated collection and analysis patient care system **10** not otherwise discernible without having the patient physically present. For instance, a scoring system using a scale of 1.0 to 10.0 could be used with 10.0 indicating normal wellness and 1.0 indicating severe health problems. Upon the completion of the initial observation period, a patient might indicate a health wellness score **111** of 5.0 and a cardiac output score of 5.0. After one month of remote patient care, the patient might then indicate a health wellness score **111** of 4.0 and a cardiac output score of 4.0 and a week later indicate a health wellness score **111** of 3.5 and a cardiac output score of 3.5. Based on a comparison of the health wellness scores **111** and the cardiac output scores, the system **10** would identify a trend indicating the necessity of potential medical intervention while a comparison of the cardiac output scores alone might not lead to the same prognosis.

FIG. 7 is a database schema showing, by way of example, the organization of a monitoring record **120** for cardiac patient care stored as part of a patient care record in the database **17** of the system **10** of FIG. 1A. Each patient care record stores a multitude of subsequently collected device measures sets **58** (shown in FIG. 3) for each individual patient **11**. Each set represents a recorded snapshot of telemetered signals data which were recorded, for instance, on a per heartbeat or binned average basis by the implantable medical device **12**. For example, for a cardiac patient, the following information would be recorded as a subsequently collected device measures set **58**: atrial electrical activity **121**, ventricular electrical activity **122**, minute ventilation **123**, patient activity score **124**, cardiac output score **125**, mixed venous oxygen score **126**, pulmonary artery diastolic pressure measure **127**, time of day **128**, interventions made by the implantable medical device **129**, and the relative success of any interventions made **130**. In addition, the implantable medical device **12** would also communicate device specific information, including battery status and program settings **131**. Other types of collected or combined measures are possible as previously described. In addition, a well-documented set of derived measures can be determined based on the collected measures, as is known in the art.

FIGS. 8A-8C are flow diagrams showing a method **140** for determining a reference baseline **5** for use in monitoring a patient status in an automated collection and analysis patient care system **10** in accordance with the present invention. The method **140** operates in two phases: collection and processing of an initial reference baseline **5** (blocks **141-149**) and monitoring using the reference baseline **5** (blocks **150-158**). The method **140** is implemented as a conventional computer program for execution by the server system **16** (shown in FIG. 1A). As a preparatory step, the patient care records are organized in the database **17** with a unique patient care record assigned to each individual patient (block **141**).

The collection and processing of the initial reference baseline **5** begins with the patient **11** being monitored by the implantable medical device **12** (shown in FIG. 1A). The implantable medical device **12** records the initially collected device measures set **57** during the initial observation period (block **142**), as described above with reference to FIG. 5. Alternatively, the patient **11** could be engaged in performing the prescribed set of timed physical stressors during the initial

observation period, as described above with reference to FIG. 1B. As well, the implantable medical device **12** could be reprogrammed by the programmer **14** during the initial observation period, also as described above with reference to FIG. 1B. The initially collected device measures set **57** is retrieved from the implantable medical device **12** (block **143**) using a programmer, interrogator, telemetered signals transceiver, and the like. The retrieved initially collected device measures sets are sent over the internetwork **15** or similar communications link (block **144**) and periodically received by the server system **16** (block **145**). The initially collected device measures set **57** is stored into a patient care record in the database **17** for the individual patient **11** (block **146**). The initially collected device measures set **57** is processed into the reference baseline **5** (block **147**) which stores a reference measures set **59**, as further described below with reference to FIG. 9.

If quality of life measures are included as part of the reference baseline **5** (block **148**), the set of quality of life measures are processed (block **149**), as further described below with reference to FIG. 10. Otherwise, the processing of quality of life measures is skipped (block **148**).

Monitoring using the reference baseline **5** begins with the retrieval of the subsequently collected device measures sets **58** from the implantable medical device **12** (block **150**) using a programmer, interrogator, telemetered signals transceiver, and the like. The subsequently collected device measures sets **58** are sent, on a substantially regular basis, over the internetwork **15** or similar communications link (block **151**) and periodically received by the server system **16** (block **152**). The subsequently collected device measures sets **58** are stored into the patient care record in the database **17** for that individual patient (block **153**).

The subsequently collected device measures sets **58** are compared to the reference measures in the reference baseline **5** (block **154**). If the subsequently collected device measures sets **58** are substantially non-conforming (block **155**), the patient care record is identified (block **156**). Otherwise, monitoring continues as before.

In the described embodiment, substantial non-conformity refers to a significant departure from a set of parameters defining ranges of relative normal activity and normal exercise responses for that patient. Relative normal activity is defined as follows. Note the "test exercise period" refers to running in place, walking, and ascending stairs physical stressors described above:

- (1) Heart rate stays within a range of 40-90 bpm without upward or downward change in mean heart rate  $\pm 1.0$  standard deviation (SD) over a 24 hour period;
- (2) Wake patient activity score during awake hours stays within a range of  $\pm 1.0$  SD without change in the mean activity score over a 24 hour period with no score equal to the minimum activity score noted during sleep;
- (3) Sleep period activity score stays within a range of  $\pm 1.0$  SD of typical sleep scores for that patient for the six to ten hour period of sleep with no score less than the minimum score observed during normal awake behavior during the initial observation period or during normal sleep;
- (4) Minute ventilation **123** during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean score over a 24 hour period with no score equal to the minimum or maximum minute ventilation **123** noted during the test exercise period or the minimum or maximum minute ventilation **123** noted during the initial observation period;
- (5) Cardiac output score **125** during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the

- mean cardiac output score over a 24 hour period with no score equal to the minimum cardiac output score noted during the test exercise period or the minimum cardiac output score noted during the initial observation period;
- (6) Mixed venous oxygenation score **126** during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean mixed venous oxygenation score over a 24 hour period with no score equal to the minimum mixed venous oxygenation score noted during the test exercise period or the minimum mixed venous oxygenation score noted during the initial observation period;
- (7) Pulmonary artery diastolic pressure measure **127** during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean pulmonary artery diastolic pressure measure **127** over a 24 hour period with no score equal to the minimum or maximum pulmonary artery diastolic pressure measure **127** noted during the test exercise period or during the initial observation period;
- (8) Potassium levels [K+] score during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean K+ levels over a 24 hour period with no score less than 3.5 meq/liter or greater than 5.0 meq/liter noted during the test exercise period or during the initial observation period;
- (9) Sodium levels [Na+] score during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean Na+ levels over a 24 hour period with no score less than 135 meq/liter or greater than 145 meq/liter during the test exercise period or during the initial observation period;
- (10) Acidity (pH) score during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean pH score over a 24 hour period with no score equal to the minimum or maximum pH score noted during the test exercise period or the minimum or maximum pH scores noted during the initial observation period;
- (11) Glucose levels during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean glucose levels over a 24 hour period with no score less than 60 mg/dl or greater than 200 mg/dl during the test exercise period or during the initial observation period;
- (12) Blood urea nitrogen (BUN) or creatinine (Cr) levels during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean BUN or Cr levels score over a 24 hour period with no score equal to the maximum BUN or creatinine levels noted during the test exercise period or the maximum BUN or Cr levels noted during the initial observation period;
- (13) Hematocrit levels during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean hematocrit levels score over a 24 hour period with no score less than a hematocrit of 30 during the test exercise period or during the initial observation period;
- (14) Troponin, creatinine kinase myocardial band, or other cardiac marker of myocardial infarction or ischemia, level during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean troponin level score over a 24 hour period with no score equal to the maximum troponin level score noted during the test exercise period or the maximum troponin level scores noted during the initial observation period;
- (15) Central nervous system (CNS) creatinine kinase (CK) or equivalent markers of CNS ischemia or infarction levels during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean CNS CK levels

- over a 24 hour period with no score equal to the maximum CNS CK levels score noted during the test exercise period or the maximum CNS CK levels scores noted during the initial observation period;
- (16) Barometric pressure during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean barometric pressure score over a 24 hour period with no score equal to the minimum or maximum barometric pressure noted during the test exercise period or the minimum or maximum barometric pressure noted during the initial observation period;
- (17) PR interval (or intrinsic AV interval) of sinus rhythm during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean PR interval over a 24 hour period with no score equal to the minimum or maximum PR interval noted during the test exercise period or the minimum or maximum PR interval noted during the initial observation period;
- (18) QT interval during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean QT interval over a 24 hour period with no score equal to the minimum or maximum QT interval noted during the test exercise period or the minimum or maximum QT interval noted during the initial observation period;
- (19) QRS duration during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean QRS duration over a 24 hour period with no score equal to the maximum QRS duration noted during the test exercise period or the maximum QRS duration noted during the initial observation period;
- (20) ST segment depression or elevation during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean ST segment depression or elevation over a 24 hour period with no score equal to the maximum ST segment depression or elevation noted during the test exercise period or the maximum ST segment depression or elevation noted during the initial observation period; and
- (21) Temperature during normal awake hours stays within a range of  $\pm 1.0$  SD without change in the mean temperature over a 24 hour period with no score equal to the minimum or maximum temperature score noted during the test exercise period or the minimum or maximum temperature noted during the initial observation period.
- For an exemplary, non-ambulatory patient with no major impairments of the major limbs, reference exercise can be defined as follows:
- (1) Heart rate increases by 10 bpm for each one point increase in activity score. Note that to be considered "normal exercise," heart rate generally should not increase when the activity score does not increase at least 1.0 SD above that noted during the twenty-four hour reference period or greater than that observed during any reference exercise periods. Heart rate should decrease to the baseline value over fifteen minutes once activity stops or returns to the baseline activity level;
  - (2) Patient activity score **124** rises at least 1.0 SD over that observed in the mean activity score over a 24 hour period or greater than that observed during any reference exercise periods;
  - (3) Cardiac output score **125** rises at least 1.0 SD over that observed in the mean cardiac output score over a 24 hour period or within 0.5 SD of the two minute test exercise period. Cardiac output score should increase 0.5 liters per minute with each 10 bpm increase in heart rate period or greater than that observed during any reference exercise periods;

- (4) In conjunction with an increase in activity score and heart rate, mixed venous oxygenation score **126** falls at least 1.0 SD below observed in the mean oxygenation score over a 24 hour period or be less than any oxygenation score observed during the reference exercise periods. Oxygenation score should decrease 5.0 mm Hg with each 10 bpm increase in heart rate or 1.0 SD increase in cardiac output score during exercise;
- (5) In conjunction with an increase in activity score and heart rate, pulmonary artery diastolic pressure measure **127** rises at least 1.0 SD over that observed in the mean cardiovascular pressure score over a 24 hour period or is greater than that observed during the reference exercise periods;
- (6) In conjunction with an increase in activity score and heart rate, minute ventilation **123** rises at least 1.0 SD over that observed over a 24 hour reference period or greater than that observed during any reference exercise period. Minute ventilation should rise 1.0 liter per minute with each 10 bpm increase in heart rate; and
- (7) In conjunction with an increase in activity score and heart rate, temperature should rise at least 1.0 SD over that observed in the mean temperature over a 24 hour period or greater than that observed during the reference exercise periods. Temperature should rise 0.1° F. with each 10 bpm increase in heart rate.

Finally, if the time for a periodic reassessment has arrived or the subsequently collected device measures sets **58** are substantially non-conforming (block **157**), the reference baseline **5** is reassessed (block **158**) and a new reference baseline **73** determined, as further described below with reference to FIG. **11**. Otherwise, the routine returns.

In the described embodiment, the reference baseline **5** is preferably reassessed on an annual or, if necessary, quarterly basis. In addition, the reference baseline **5** might be reassessed if physiological findings dictate that new interventions might be indicated or if the patient **11** indicates a change in medications and general health status. Other bases for reassessing the reference baseline **5** are feasible.

FIG. **9** is a flow diagram showing the routine **147** for processing a reference baseline **5** for use in the method **140** of FIGS. **8A-8C**. The purpose of this routine is to analyze the initially collected device measures set **57** and create a reference baseline **5**, if possible. First, the acceptance parameters set **72** (shown in FIG. **3**) is defined (block **160**) and the reference measures set **59** in the reference baseline **5**, including any quality of life measures, are analyzed against the acceptance parameters set (block **161**), as described above with reference to FIG. **5**. If the reference measures in the reference baseline **5** are substantially non-conforming to the acceptance parameters set (block **162**), the patient care record is identified (block **164**). Otherwise, if conforming (block **162**), the baseline reference **72** is stored into the patient care record in the database **17** (block **163**). The routine then returns.

FIG. **10** is a flow diagram showing the routine **149** for processing quality of life measures for use in the method **140** of FIGS. **8A-8C**. The purpose of this routine is to process and store a collected quality of life measures set **60** into the reference baseline **5**. Collected quality of life measures sets **60** are periodically received by the server system **16** over the internetwork **15** or similar communications link (block **170**). The quality of life measures were previously recorded by the patient **11** using, for example, the personal computer **18** (shown in FIG. **1A**) and downloaded onto the internetwork **15** or similar communications link. The collected quality of life measures set **60** is stored into a patient care record in the

database **17** for the individual patient **11** (block **171**). The collected quality of life measures set **60** is then assimilated into the reference baseline **5** (block **172**), as further described above with reference to FIG. **9**. The routine then returns.

FIG. **11** is a flow diagram showing the routine **158** for reassessing a new reference baseline **73** for use in the method **140** of FIGS. **8A-8C**. The purpose of this routine is to reassess a new reference baseline **5** periodically or when necessary. Similar to the collection and assimilation of the initial reference baseline **5**, the routine begins with the patient **11** being monitored by the implantable medical device **12** (shown in FIG. **1A**). The implantable medical device **12** records subsequently collected device measures sets **58** throughout a subsequent observation period (block **180**), as described above with reference to FIG. **5**. Alternatively, the patient **11** could be engaged in performing the prescribed set of timed physical stressors, as described above with reference to FIG. **1B**. As well, the implantable medical device **12** could be reprogrammed by the programmer **14** during the subsequent observation period, also as described above with reference to FIG. **1B**. The subsequently collected device measures sets **58** are retrieved from the implantable medical device **12** (block **181**) using a programmer, interrogator, telemetered signals transceiver, and the like. The retrieved subsequently collected device measures sets are sent over the internetwork **15** or similar communications link (block **182**) and periodically received by the server system **16** (block **183**). The subsequently collected device measures sets **58** are stored into the patient care record in the database **17** for the individual patient **11** (block **184**). Finally, the subsequently collected device measures sets **58** are assimilated into the new reference baseline **73** (block **185**), as further described above with reference to FIG. **9**. The routine then returns.

The determination of a reference baseline consisting of reference measures makes possible improved and more accurate treatment methodologies based on an algorithmic analysis of the subsequently collected data sets. Each successive introduction of a new collected device measures set into the database server would help to continually improve the accuracy and effectiveness of the algorithms used.

While the invention has been particularly shown and described as referenced to the embodiments thereof, those skilled in the art will understand that the foregoing and other changes in form and detail may be made therein without departing from the spirit and scope of the invention.

What is claimed is:

1. A programmer for generating baseline data for automated management of cardiovascular pressure, comprising:
  - a memory to store device measures received from an implantable medical device, comprising:
    - collected device measures to record raw physiometry for a patient regularly monitored by the implantable medical device, beginning with an initial observation period; and
    - derived device measures to provide derivative physiometry determined at least in part from the collected device measures; and
  - a processor to determine a wellness indicator through analysis of the collected and derived device measures to diagnose a patient status indicative of at least one of a change and a status quo in cardiovascular pressure, wherein the collected and derived device measures and the wellness indicator originating from the initial observation period comprise baseline data.
2. A programmer according to claim 1, wherein the analysis comprises one or more of:

a monitor to accumulate collected device measures and to derive derived device measures for use in determining the wellness indicator relating to cardiovascular pressure;

a patient well being analyzer to monitor patient well being in conjunction with at least one of potassium level, sodium level, hormonal level, and blood pressure; and

a programming interface to apply programming data to effect therapy modification selected from the group comprising device parameters, drug infusion parameters, and neural stimulation parameters.

3. A programmer according to claim 1, further comprising: an evaluator to process physiometric data conjunction with monitoring of the patient, wherein the physiometric data is selected from the group comprising:

- analytic data recorded, collected, and stored for cardiovascular pressure evaluation;
- alert data generated in response to significant events, wherein the alert data is selected from the group comprising absolute measures, long term average measures, and short term average measures; and

action data executed in response to indications selected from the group comprising the significant events, ECG signals, activity level, temperature, pressure, and oxygen saturation.

4. A programmer according to claim 1, further comprising: physiometric data comprising one or more of the collected and derived device measures sensed through one or more of cardiovascular pressure, potassium level, sodium level, hormonal level, central nervous system injury, and central nervous system blood flow.

5. A programmer according to claim 1, further comprising: programming parameters, comprising at least one of: monitoring parameters to monitor the patient while asleep; and exclusion parameters to exclude physiometric data comprising one or more of the collected and derived device measures when the patient exhibits an increased respiratory rate due to exercise or activity level.

6. A programmer according to claim 1, further comprising: programmed trigger conditions with corresponding actions, wherein the actions are executed by the processor based upon the direct and derived device measures to cause activation of one or more of a therapy readout, alarm, or change in the raw physiometry measured, wherein the trigger conditions are selected from the group comprising absolute measures, pattern matching, absolute differences between averaged measures, and comparisons of a current measure to another current measure or a previous measure.

7. An analysis system for generating baseline data for automated management of cardiovascular pressure, comprising:

- a structured database, comprising:
  - collected device measures to record raw physiometry for a patient, wherein the patient is regularly monitored by an implantable medical device, beginning with an initial observation period; and
  - derived device measures to provide derivative physiometry determined at least in part from the collected device measures;
- an analyzer to determine a wellness indicator through analysis of the collected and derived device measures to diagnose a patient status indicative of at least one of a change and a status quo in cardiovascular pressure; and

a processor to designate the collected and derived device measures and the wellness indicator originating from the initial observation period as baseline data.

8. An analysis system according to claim 7, wherein the structured database organizes processed data to reflect one or more of:

- monitoring data comprising collected and derived device measures and a wellness indicator for cardiovascular pressure;
- patient well being data monitored in conjunction with at least one of potassium level, sodium level, hormonal level, and blood pressure; and
- programming data to effect therapy modification selected from the group comprising device parameters, drug infusion parameters, and neural stimulation parameters.

9. An analysis system according to claim 7, wherein the processor processes physiometric data in conjunction with monitoring of the patient, comprising at least one of:

- database management comprising physiometric data recording, collection, and storage for cardiovascular pressure evaluation;
- alert generation in response to significant events, wherein alert data is selected from the group comprising absolute measures, long term average measures, and short term average measures; and
- action execution in response to indications selected from the group comprising the significant events, ECG signals, activity level, temperature, pressure, and oxygen saturation.

10. An analysis system according to claim 7, further comprising:

- physiometric data comprising one or more of the collected and derived device measures sensed through one or more of cardiovascular pressure, potassium level, sodium level, hormonal level, central nervous system injury, and central nervous system blood flow.

11. An analysis system according to claim 7, further comprising:

- a programming interface to generate programming parameters, comprising at least one of:
  - monitoring parameters to monitor the patient while asleep; and
  - exclusion parameters to exclude physiometric data comprising one or more of the collected and derived device measures when the patient exhibits an increased respiratory rate due to exercise or activity level.

12. An analysis system according to claim 7, further comprising:

- defined trigger conditions with corresponding actions that are executed based upon the direct and derived device measures to cause activation of one or more of a therapy readout, alarm, or change in the raw physiometry measured,
- wherein the trigger conditions are selected from the group comprising absolute measures, pattern matching, absolute differences between averaged measures, and comparisons of a current measure to another current measure or a previous measure.

13. A method for generating baseline data for automated management of cardiovascular pressure, comprising:

- using an implantable medical device to accumulate collected device measures to record raw physiometry for a patient, wherein the patient is regularly monitored by the implantable medical device, beginning with an initial observation period;

generating derived device measures to provide derivative  
 physiometry determined at least in part from the col-  
 lected device measures; and  
 determining a wellness indicator by using a processor to  
 analyze the collected and derived device measures to  
 diagnose a patient status indicative of at least one of a  
 change and a status quo in cardiovascular pressure,  
 wherein the collected and derived device measures and the  
 wellness indicator originating from the initial observa-  
 tion period comprise baseline data.  
 14. A method according to claim 13, further comprising:  
 processing data, comprising one or more of:  
 monitoring data comprising collected and derived  
 device measures and a wellness indicator relating to  
 cardiovascular pressure;  
 monitoring patient well being in conjunction with at  
 least one of potassium level, sodium level, hormonal  
 level, and blood pressure; and  
 forming programming data to effect therapy modification  
 selected from the group comprising device parameters,  
 drug infusion parameters, and neural stimulation param-  
 eters.  
 15. A method according to claim 13, further comprising:  
 processing physiometric data in conjunction with monitor-  
 ing of the patient, comprising at least one of:  
 recording, collecting, and storing data for cardiovascu-  
 lar pressure evaluation;  
 generating alert data in response to significant events,  
 wherein the alert data is selected from the group com-  
 prising absolute measures, long term average mea-  
 sures, and short term average measures; and

executing actions in response to indications selected from  
 the group comprising the significant events, ECG sig-  
 nals, activity level, temperature, pressure, and oxygen  
 saturation.  
 16. A method according to claim 13, wherein physiometric  
 data comprising one or more of the collected and derived  
 device measures is sensed through one or more of cardiovas-  
 cular pressure, potassium level, sodium level, hormonal level,  
 central nervous system injury, and central nervous system  
 blood flow.  
 17. A method according to claim 13, further comprising:  
 generating programming parameters, comprising at least  
 one of:  
 defining monitoring parameters to monitor the patient  
 while asleep; and  
 defining exclusion parameters to exclude physiometric  
 data comprising one or more of the collected and derived  
 device measures when the patient exhibits an increased  
 respiratory rate due to exercise or activity level.  
 18. A method according to claim 13, further comprising:  
 executing trigger conditions with corresponding actions  
 based upon the direct and derived device measures to  
 cause activation of one or more of a therapy readout,  
 alarm, or change in the raw physiometry measured,  
 wherein the trigger conditions are selected from the group  
 comprising absolute measures, pattern matching, abso-  
 lute differences between averaged measures, and com-  
 parisons of a current measure to another current measure  
 or a previous measure.

\* \* \* \* \*

专利名称(译)	用于生成用于心血管压力的自动管理的基线数据的系统和方法		
公开(公告)号	<a href="#">US8308650</a>	公开(公告)日	2012-11-13
申请号	US12/938686	申请日	2010-11-03
[标]申请(专利权)人(译)	心脏起搏器股份公司		
申请(专利权)人(译)	心脏起搏器, INC.		
当前申请(专利权)人(译)	心脏起搏器, INC.		
[标]发明人	BARDY GUST H		
发明人	BARDY, GUST H.		
IPC分类号	A61B5/02 A61B5/00 A61N1/372 G06F19/00		
CPC分类号	A61B5/0002 A61B5/4884 G06F19/322 G06F19/324 G06F19/3418 G06F19/3431 G06Q50/24 Y10S128/92		
优先权	09/361332 2001-04-24 US		
其他公开文献	US20110046493A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

公开了一种用于生成用于心血管压力的自动管理的基线数据的系统和方法。累积收集的装置测量值以记录患者的原始生理测量值，其中从初始观察期开始，通过可植入医疗装置定期监测患者。生成导出的设备测量以提供至少部分地根据所收集的装置测量确定的导数生理测量。通过分析收集和导出的装置测量来诊断指示心血管压力的缺失，发作，进展，退化和现状的病理生理学来确定患者状态指示器，其中收集和导出的装置测量和患者状态指示器源自初始观察期包括基线数据。

