



(19) **United States**

(12) **Patent Application Publication**
Pfeiffer et al.

(10) **Pub. No.: US 2004/0249297 A1**

(43) **Pub. Date: Dec. 9, 2004**

(54) **APPARATUS FOR DETERMINING
CARDIOVASCULAR PARAMETERS**

(57) **ABSTRACT**

(76) Inventors: **Ulrich J. Pfeiffer**, Munchen (DE);
Thorsten Burger, Munchen (DE)

An apparatus that continuously monitors the arterial pressure measured by a pressure sensor in an artery, which pressure is regarded as the reading P_{ao} that approximately corresponds to the aortal pressure. In principle, the arterial pressure can be measured in the aorta, near the aorta, or in the arterial tree. To provide a second reading, the apparatus, via the input channel, continuously monitors the central venous pressure (CVP), which is regarded as the reading PIT that approximately corresponds to the intrathoracic pressure (ITP). The third reading is provided via the input channel as a reading Z which expresses the thoracic compliance. Via known algorithms of the pulse contour analysis, the apparatus calculates the stroke volume variation, using as the determining pressure the transmural pressure which is calculated according to the formula

Correspondence Address:
**WILLIAM COLLARD
COLLARD & ROE, P.C.
1077 NORTHERN BOULEVARD
ROSLYN, NY 11576 (US)**

$$P_{transmural} = P_{ao} - f(C) * PIT.$$

(21) Appl. No.: **10/743,515**

The cardiac volume responsiveness indicator (CVRI) is calculated for mechanical positive respiration according to the formula

(22) Filed: **Dec. 22, 2003**

$$CVRI = k * (SVV / \Delta CVP)$$

(30) **Foreign Application Priority Data**

or for spontaneous breathing according to the formula


Dec. 23, 2002 (DE)..... 102 60 762.1

$$CVRI = 1 - m * (\Delta CVP / SVV).$$

Publication Classification

(51) **Int. Cl.⁷ A61B 5/02**

(52) **U.S. Cl. 600/526**

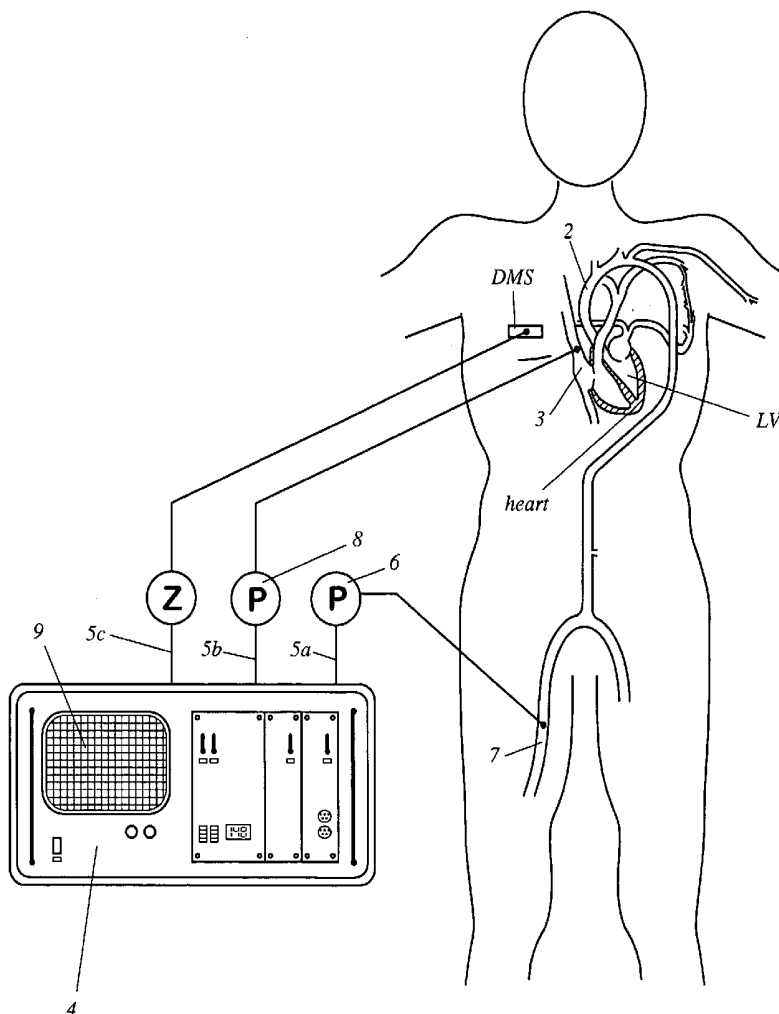

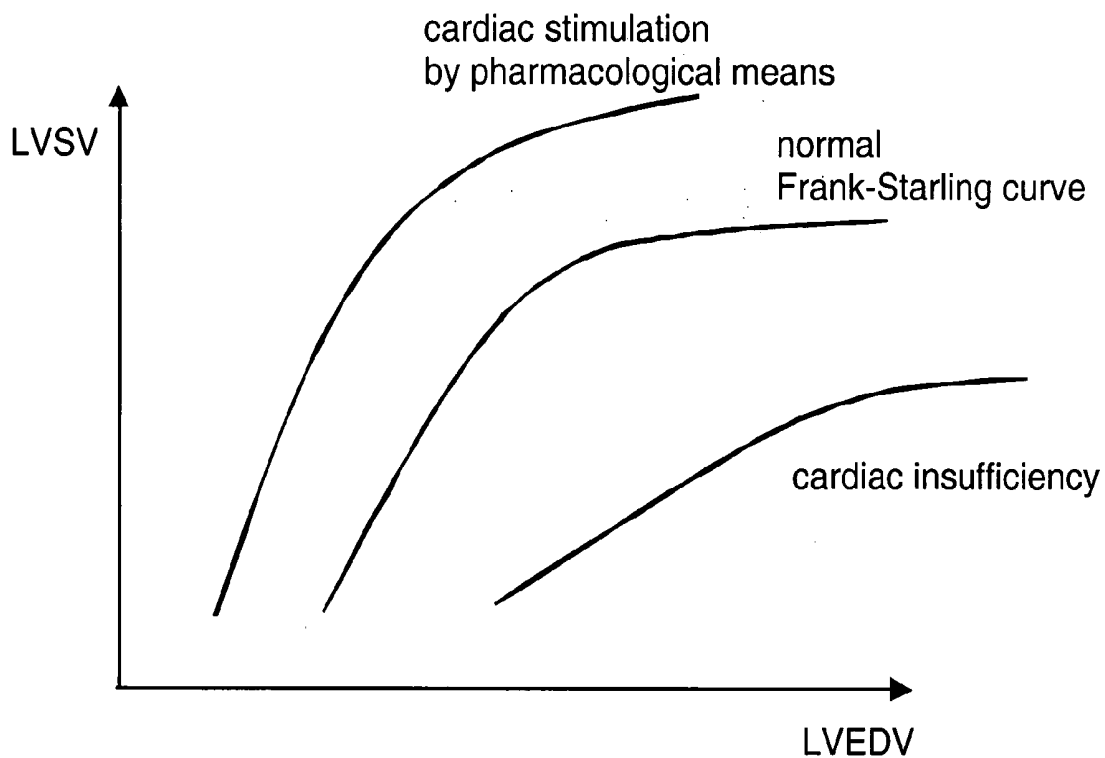


Fig. 1 (Background of the invention)

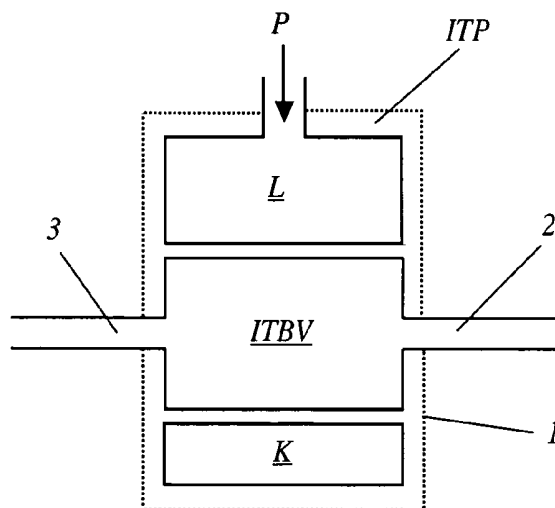


Fig. 2

Fig. 3

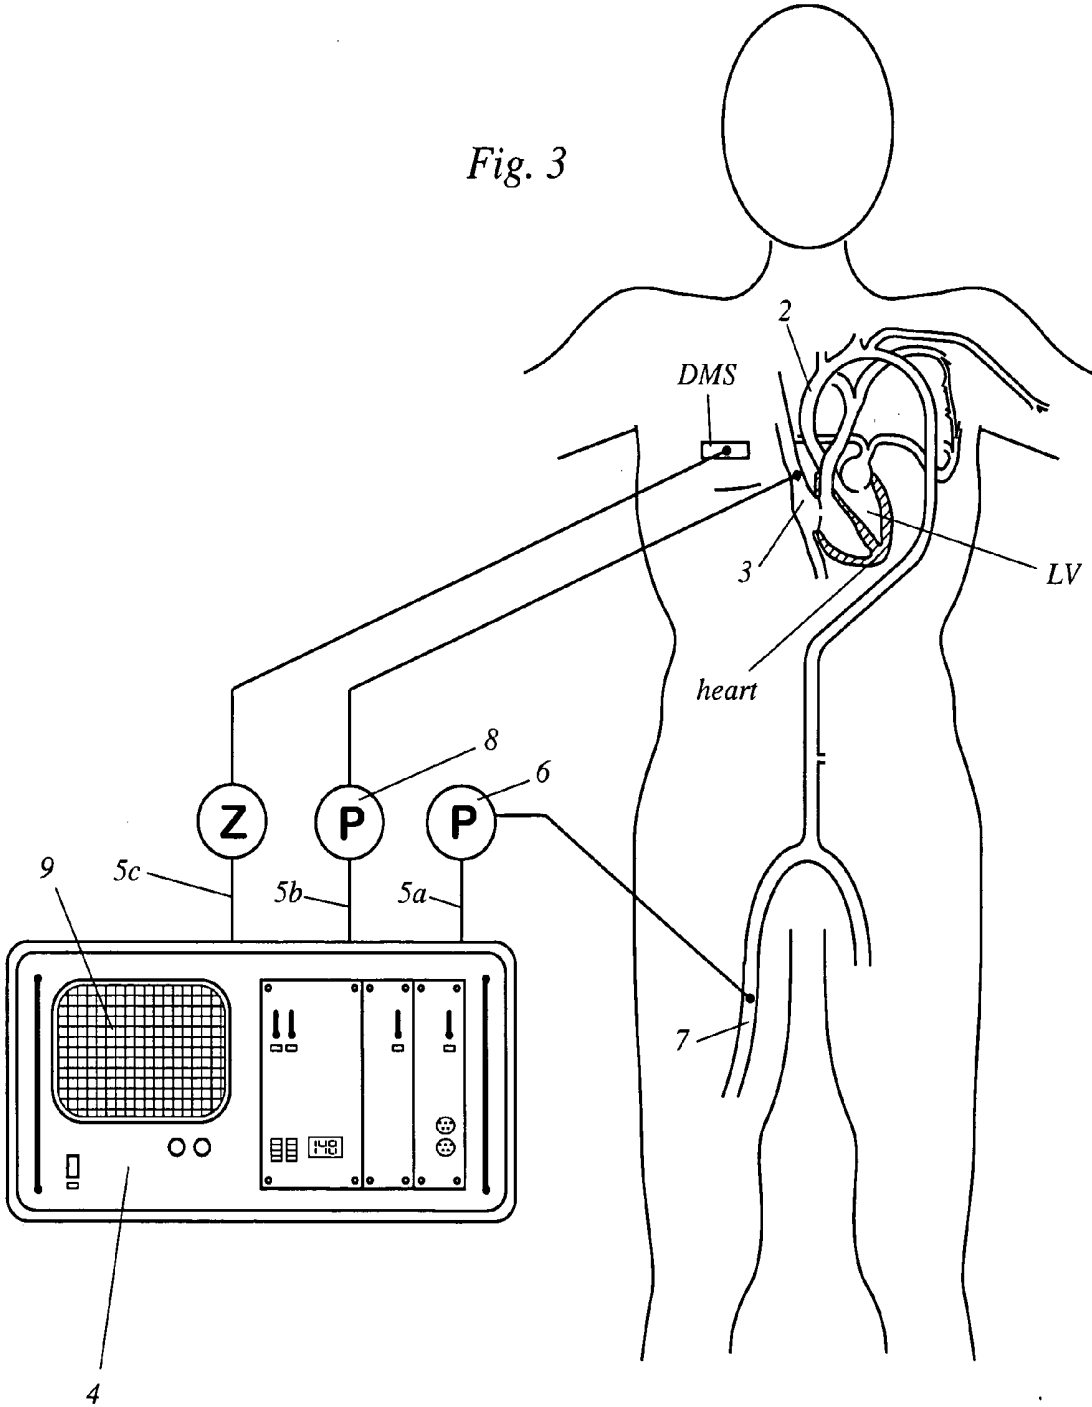


Fig. 4a

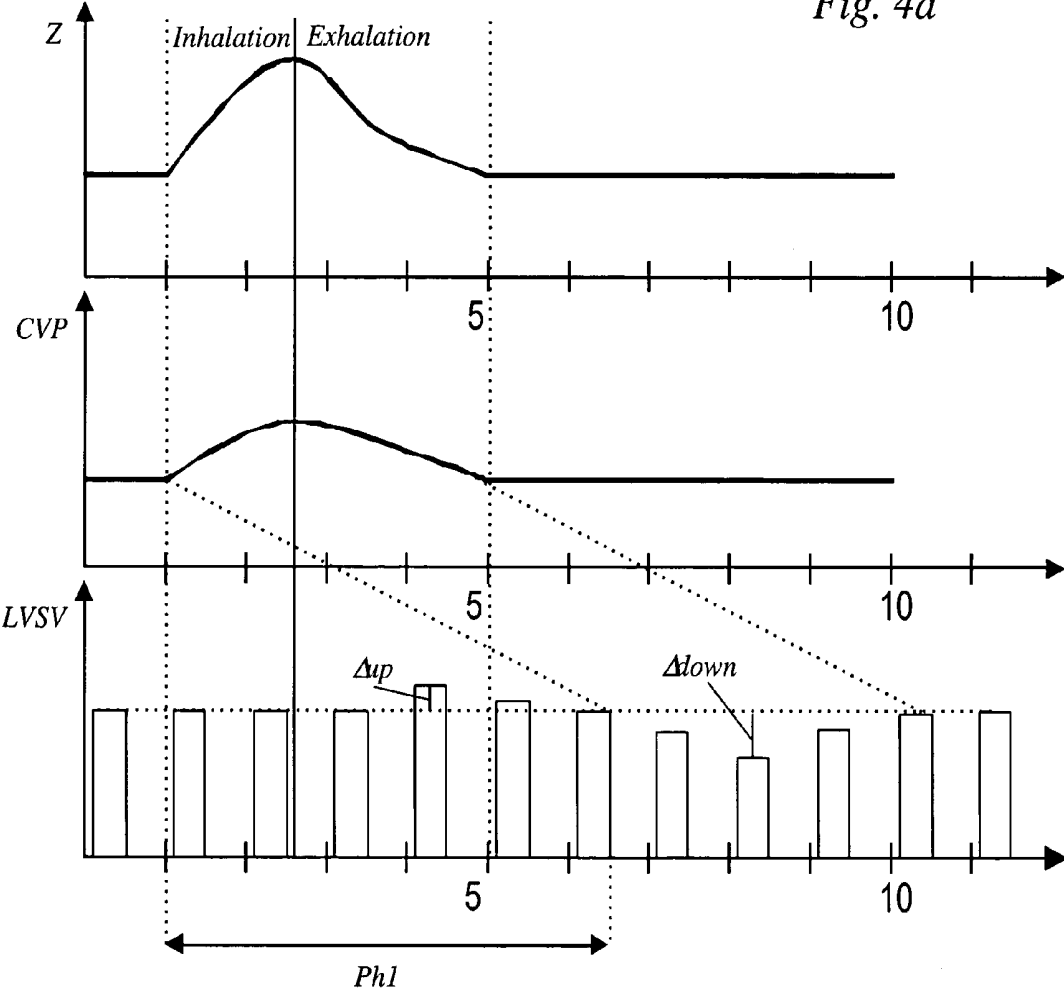
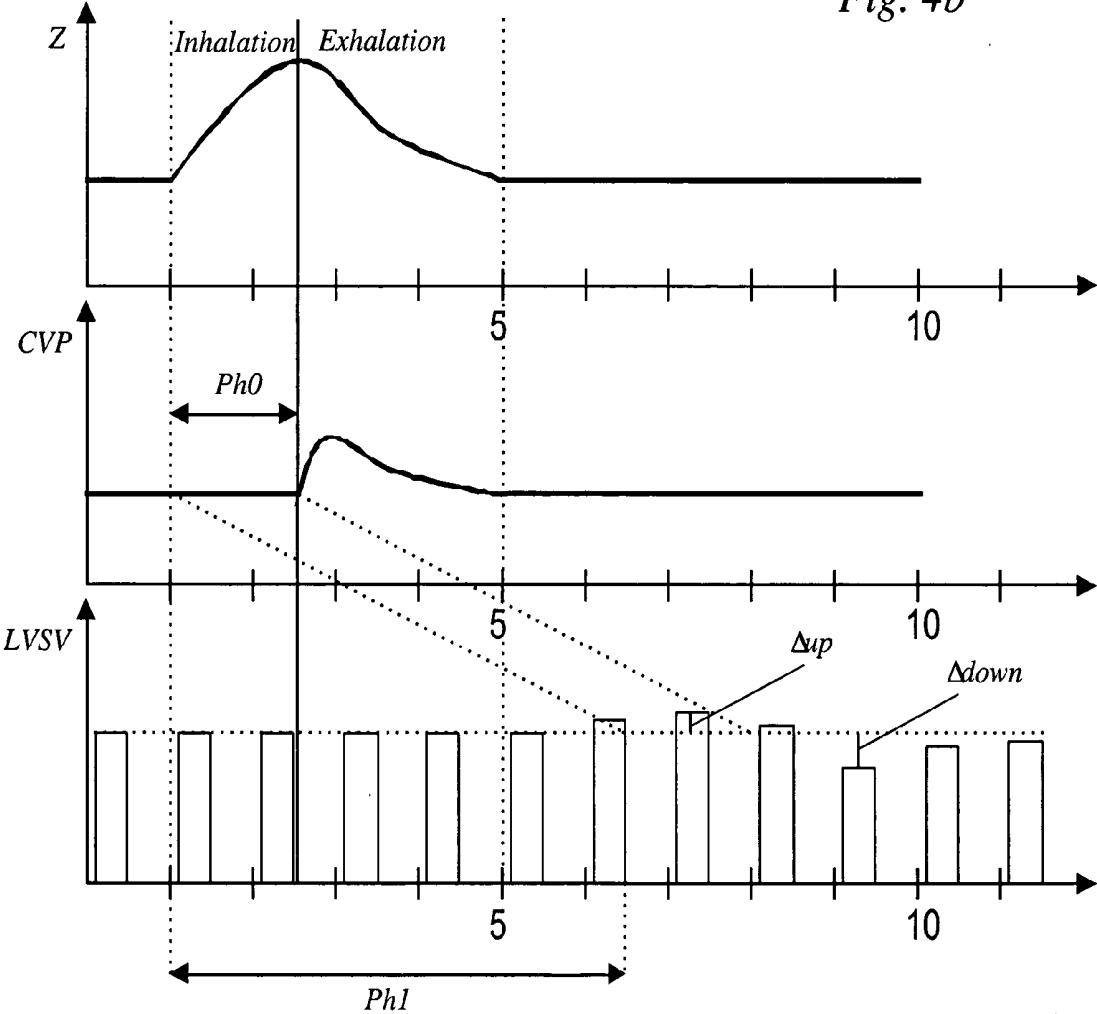


Fig. 4b



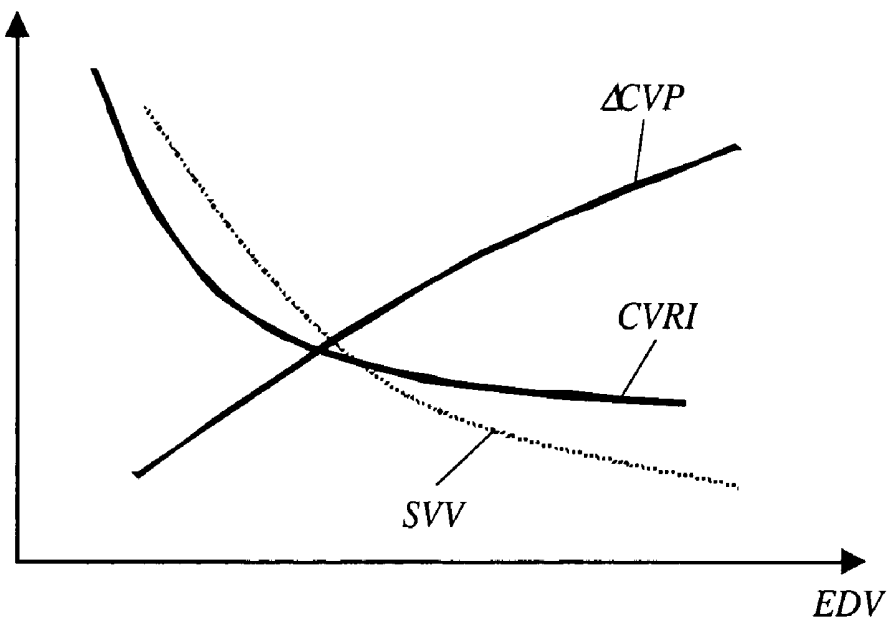


Fig. 5a

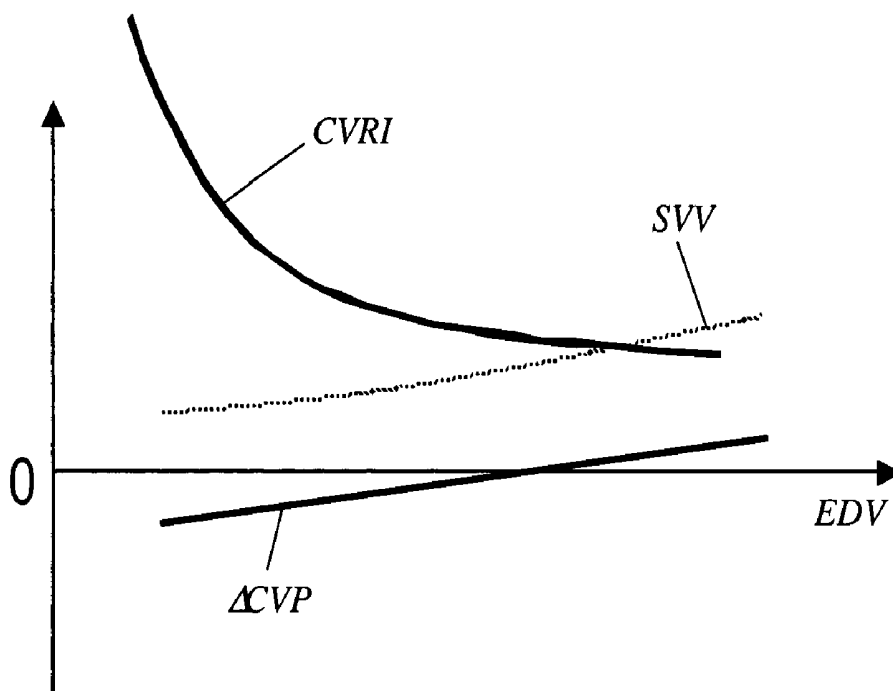


Fig. 5b

APPARATUS FOR DETERMINING CARDIOVASCULAR PARAMETERS

BACKGROUND OF THE INVENTION

[0001] 1. Field of the Invention

[0002] The present invention relates to an apparatus for determining cardiovascular parameters, in particular an apparatus for the continuous determination of the parameters that characterize a patient's left ventricular pumping action, and an apparatus for the continuous determination of the cardiac volume responsiveness indicator.

[0003] 2. The Prior Art

[0004] It is particularly important to monitor continuously cardiovascular parameters in critically ill patients, for example during surgical procedures performed under total anesthesia, or in case of a critical condition. Of special importance are the parameters that characterize the left ventricular pumping action. It is known from the prior art to determine these parameters by means of pulse contour analysis, for which technical solutions such as the commercially available PiCCO system by Pulsion Medical Systems have been known for some time. With these, the parameters to be determined are calculated from the time curve of an arterially measured pressure. In particular, a pulse contour analysis based on a non-linear wind kessel model, in which—for example as described in DE 198 14 371 A1—a non-linear function of the pressure measured close to the aorta is used for the so-called compliance (expandability) of the aorta, usually leads to very useful results. However, in patients receiving mechanical respiration, the validity of the information obtained from such an analysis could sometimes be improved.

[0005] Furthermore, in the cardiovascular monitoring of intensive-care patients, it is often of crucial importance to recognize whether a critical cardiac filling state of the patient should be treated by supplying volume or with medication. In particular with patients receiving artificial respiration, this is sometimes difficult, since the state of respiration affects the measured variables. This is briefly explained below.

[0006] The mammalian thorax can be regarded as a chamber with a variable volume. The chamber is composed of the partial volumes of the heart, the lungs, the extracardiac vessels, and fixed tissue, such as connective tissue and the esophagus. The thoracic volume changes regularly with breathing or mechanical respiration. Under pathophysiological conditions, it may vary due to increased abdominal pressure, and also due to external pressure, for example during diving, etc. Looking at a variable thoracic volume in terms of time, it contains partial volumes which change very rapidly, for example within seconds, in the course of a breathing or respiration cycle, as does the gas volume inside the lungs and the blood volume inside large vessels and inside the heart, and partial volumes which change over longer time periods, such as the functional residual volume of the lungs due to therapeutic intervention, e.g. application of constant positive end-expiratory pressure; an increase in extravasal pulmonary fluid (when a pulmonary oedema is formed), and an increase in pathological partial volumes (as in case of hemothorax, pneumothorax or pleural effusion).

[0007] It has been known for a long time that there are interactions between the heart and the lungs during breath-

ing and in particular during mechanical respiration. In the case of spontaneous breathing, the inhaled air enters the lungs due to the negative intrathoracic pressure (ITP) which is produced by the precordial musculature and the diaphragm. However, the venous blood flow into the chest region, often called venous reflux, is facilitated during inhalation as well. During exhalation in spontaneous breathing, the intrathoracic pressure becomes positive again, which causes gas to leave the lungs, since the pressure within in the lungs exceeds atmospheric pressure, while the venous reflux is slowed down. The same happens during mechanical respiration when spontaneous breathing is simulated by means of a respirator in the form of an iron lung.

[0008] During the most common form of mechanical respiration, i.e. positive-pressure respiration, inhaling is accomplished by producing a positive pressure in the airways of the breathing apparatus outside the lungs. Respiratory gas enters the lungs because the gas pressure inside the lungs is lower. Gas enters the lungs until the pressure in the external airways and the gas pressure in the lungs and internal airways reach an equilibrium. During this inhalation process, the lungs are enlarged, which increases the intrathoracic pressure, and the large blood vessels and the heart itself are compressed. Physiologically, this means that venous reflux is reduced. Exhalation occurs due to the retractive force of the thoracic wall and the lungs themselves and, to a lesser degree, due to the weight of the thoracic wall itself, whereby the intrathoracic pressure (ITP) drops again while the venous reflux increases.

[0009] The above described changes in venous reflux during spontaneous breathing as well as during mechanical positive respiration have a direct effect on the cardiac filling and—via the so-called Frank Starling mechanism—on the ventricular output, i.e. the stroke volume. In simplified terms, the Starling mechanism describes a relationship between the diastolic cardiac filling volume and the cardiac stroke volume. The more the heart is filled in the diastolic phase, the greater is the output of cardiac stroke volume. This relationship is predominantly linear in a normal heart and becomes flatter when a normally contracting heart is overfilled in the diastolic phase. This is shown in **FIG. 1**, where the left ventricular stroke volume (LVS_V) is plotted schematically against the left ventricular end-diastolic volume (LVEDV) which essentially corresponds to the filling status in the diastolic phase. The middle curve shows the normal pattern. When positively inotropic substances such as adrenalin are administered, i.e. when the cardiac contraction force is increased, the Starling curve shifts to the left, whereas conditions connected with an acutely or chronically changed cardiac contraction force reduce the rise and cause a shift of the curve to the right. The response to a volume increase can be just as varied while the measured end-diastolic volume remains the same.

[0010] In the case of spontaneous breathing or mechanical positive respiration, the effects on cardiac filling, especially on the filling of the right ventricle, cause a variable stroke volume of the right ventricle which in turn affects the filling and the output of the left ventricle after perfusion of the lungs. Finally, these changes in cardiac filling can be detected by measuring the periodic fluctuations of the aortic or arterial pressure curve which directly reflect the changes in the left ventricular volume output.

[0011] EP 0 666 056 B1 discloses an apparatus for evaluating the necessity of providing instantaneous volume or evaluating how a patient under artificial respiration responds to the intravenous administration of volume substitutes, wherein the systolic pressure variation serves as an indicator of how receptive the patient is to volume. However, with this apparatus, it is necessary to measure the tidal volume or the respiration pressure of the respirator, and to compare it to the hemodynamic pressure before any conclusions can be drawn. It is not possible to take all interactions between the state of respiration and the measured cardiovascular values into full consideration. Furthermore, the prior art apparatus does not provide any information as to what happens when the patient returns to spontaneous breathing.

SUMMARY OF THE INVENTION

[0012] Against the backdrop of the above described problems, the object of the present invention is to create an apparatus for determining parameters that characterize a patient's left ventricular pumping action without lessening the validity of measuring results through the effect of respiration and changing respiratory states. It is also an object of the present invention to create an apparatus for determining a parameter that allows a reliable evaluation of the cardiac volume responsiveness, i.e. of the readiness for a supply of volume even with variable respiration states.

[0013] According to one aspect of the invention, this object is achieved by an apparatus for the continuous determination of a parameter characterizing a patient's left ventricular pumping action comprising:

[0014] a first input channel for the continuous recording of a variable physiological first reading directly dependent on the left ventricular pumping action, and

[0015] an evaluation unit for calculating said parameter characterizing the left ventricular pumping action,

[0016] wherein the apparatus also comprises a second input channel for the continuous recording of a variable physiological second reading which at least approximately indicates the patient's intrathoracic pressure (ITP) or is dependent on same, and wherein the evaluation unit is programmed for calculating the parameter characterizing the patient's left ventricular pumping action from said first reading, using a corrective function based on said second reading.

[0017] According to another aspect of the invention, this object is achieved by an apparatus for the continuous determination of the cardiac volume responsiveness indicator comprising a first input channel for the continuous recording of a variable physiological first reading directly dependent on the patient's left ventricular pumping action, a second input channel for the continuous recording of a variable physiological second reading at least approximately representing the patient's intrathoracic pressure (ITP), a third input channel for the continuous recording of a third reading which depends directly on the patient's state of respiration, and an evaluation unit for calculating said cardiac volume responsiveness indicator. The evaluation unit is programmed to use said second and third readings to select a function that can be used for the patient's current state of

respiration and based on this function, to calculate sid volume responsiveness indicator from said first and second readings.

[0018] The periodic fluctuations of the right or left ventricular stroke volume caused by interaction between heart and lungs, or the measured periodic fluctuations of another physiological signal, which correspond to or reflect the periodic fluctuations of the right or left ventricular output of the stroke volume, such as pressure curves measured in the *Arteria pulmonalis*, the aorta or the arterial tree, or periodic fluctuations of the signal of plethysmographic pulse oximetry, are used to diagnose the heart's response to changing cardiac filling conditions, i.e. to diagnose the heart's pre-load volume. As described above, these periodic fluctuations, which depend on breathing or artificial respiration, indicate that the heart responds to changes in the cardiac pre-load volume. These fluctuations are caused by the effect of the changing ITP on the volume of the intrathoracic low pressure capacitance system (ITLPCS) consisting of the *Venae cava* superior and inferior, the right atrium, the right ventricle in the diastolic phase, the pulmonary vascular system, and the left atrium. The ITLPCS is characterized by a low mean intravascular pressure and a relatively large intravascular volume. In the ITLPCS, the connection between volume and pressure is non-linear, which means that the pressure is very low at a low volume while the mean intravascular pressure increases progressively as the volume increases. In other words, with hypovolemia, changes in ITLPCS volume have little effect on pressure, while with hypervolemia, any change in ITLPCS volume has a great effect on the mean ITLPCS pressure. Any change in the intrathoracic pressure, which is the pressure surrounding the ITLPCS, is transferred directly to the intravascular pressure inside the ITLPCS due to the very high compliance of the vascular structures contained in the ITLPCS. The transmural pressure of the ITLPCS can be estimated as the difference between intravascular pressure and the intrathoracic pressure. The effective transmural pressure in the ITLPCS determines the actual vascular dilation and thus the volume within the ITLPCS.

[0019] Hence, a constant breath, such as a mechanical breath of constant depth, causes the same change in ITP, but—depending on the volume state of the ITLPCS—it affects the cardiac pre-load and thus the stroke volume to a varying degree. The main portion of the ITLPCS consists of the *Venae cavae* superior and inferior, the right atrium and the right ventricle in the diastolic phase while it is under the lowest mean intravascular pressure. Therefore, the effects on the ITP caused by breathing or artificial respiration greatly influence the right ventricular end-diastolic volume (RVEDV) and subsequently the right ventricular stroke volume (RVSV), but they have much less direct influence on the left ventricular end-diastolic volume (LVEDV) and the left ventricular stroke volume (LVSV). Over time, however, after passage through the lungs, these effects on the right ventricular stroke volume can also be detected in the form of changes in the left ventricular end-diastolic volume and the left-ventricular stroke volume.

[0020] For that reason, the same amount of breathing will have a much greater effect on the development of the left ventricular stroke volume with hypovolemia than with hypervolemia, provided that the left ventricle responds to changes in the pre-load. With the help of the apparatus

according to the invention, the totality of these relationships can be used clinically for examining the volume responsiveness of the left ventricle. As a clinical consequence, a patient whose left heart responds to volume, which means that his heart works in a steeper section of its current Starling curve, would be supplied with volume to optimize his cardiac output (CO). On the other hand, the supply of volume would be avoided in a patient whose left heart does not respond to volume, since his heart works in the flat section of its current Starling curve. Instead, one would try to optimize his cardiac output by administering positively inotropic substances to shift his function curve into a steeper form (left shift, see FIG. 1).

[0021] This information is very valuable for anesthetists or intensive-care specialists. It can be obtained easily and fully automatically with a monitoring system designed along the principles of the apparatus according to the invention. Such a system continuously supplies the-stroke volume or any variable reflecting the stroke volume and provides the information as to which type and phase of breathing or mechanical respiration is predominant or being applied, and how the intrathoracic pressure is affected by this kind of breathing or respiration measure.

[0022] This approach has the advantage that the heart/lung interaction used for examining the cardiac volume responsiveness can be standardized for spontaneous breathing as well as for mechanical respiration by measuring the change in intrathoracic pressure it causes, while the individual breath volume does not necessarily have to be standardized and does not have to follow a certain pattern, but may be of any magnitude.

[0023] On the other hand, there would not be much sense in trying to standardize values which describe breathing itself, since the degree to which the ITLPCS is influenced depends on the compliance of the respiratory tract itself, on the compliance of the thoracic wall and on the presence of a space-occupying process with a low time constant such as a pulmonary oedema, pneumothorax, hemothorax or pleural effusion. The tidal volume (=breath volume) and all above named factors contribute to changes in ITP, which directly affects the ITPLCS. For that reason, effects caused by breathing/respiration are best standardized by taking into account the changes in ITP which accompany them. Phase-related changes in ITP can be derived directly from changes in the continuously monitored central venous pressure (CVP) if changes in the thoracic dimensions are recorded at the same time or (applicable only in the case of mechanical positive-pressure respiration) if the timing and the form of mechanical respiration can be derived from the pressure of the respiratory system measured close to the patient, thus avoiding any time lag.

BRIEF DESCRIPTION OF THE DRAWINGS

[0024] Other objects and features of the present invention will become apparent from the following detailed description considered in connection with the accompanying drawings. It is to be understood, however, that the drawings are designed as an illustration only and not as a definition of the limits of the invention.

[0025] In the drawings, wherein similar reference characters denote similar elements throughout the several views:

[0026] FIG. 1 shows as a background to the invention, a Frank Starling curve and its change due to cardiac stimulation by pharmacological means, and due to cardiac insufficiency;

[0027] FIG. 2 shows the basic interaction between different volumes and the intrathoracic pressure;

[0028] FIG. 3 shows an apparatus according to the invention being applied to a patient;

[0029] FIG. 4a is a schematic representation of the temporal variability (change vs. time) of the readings which determine the calculation of the volume responsiveness indicator in case of positive pressure respiration;

[0030] FIG. 4b is a schematic representation of the temporal variability of the readings which determine the calculation of the volume responsiveness indicator in case of spontaneous breathing;

[0031] FIG. 5a shows a schematic view of the course of the volume responsiveness indicator depending on the end-diastolic volume with positive pressure respiration; and

[0032] FIG. 5b shows a schematic view of the course of the volume responsiveness indicator depending on the end-diastolic volume with spontaneous breathing.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

[0033] FIG. 2 shows a schematic view of the volumes affected by or affecting the intrathoracic pressure (ITP) and other characteristic pressures that are of significance in connection with the invention. Inside thoracic wall 1, the ITP acts upon the intrathoracic blood volume (ITBV) which is composed of the above named intrathoracic low-pressure capacitance system (ITLPCS) and the left ventricular end-diastolic volume (LVEDV). Other volumes inside thoracic wall 1 are the gas-filled lung volume L and, if applicable, additional volumes K, such as extravascular lung fluid, pleural effusion, hemothorax, etc., which must be regarded as constant during a measuring period. Aortal pressure AP prevails in the aorta 2 while central venous pressure CVP prevails in the central vein 3. In the case of artificial respiration, the airways are subject to external pressure P.

[0034] The apparatus 4 shown in FIG. 3, via input channel 5a, continuously monitors the arterial pressure measured by the pressure sensor 6 in an artery 7. Said arterial pressure must be regarded as a reading P_{ao} which at least approximately corresponds to the aortal pressure. In principle, the arterial pressure can be measured in the aorta 2, in its vicinity, or in the arterial tree. A second reading, the central venous pressure (CVP), which is measured by pressure sensor 8 in central vein 2, is provided continuously by apparatus 4 via input channel 5b. The CVP is regarded as a pressure P_{IT} which approximately corresponds to the ITP. The third reading, which is given via input channel 5c, is a parameter Z that reflects the thoracic compliance. Measuring may be performed, for example, with a strain gauge (DMS), but it is also possible to measure another reading which directly or indirectly represents thoracic compliance in absolute or relative terms.

[0035] Typically obtained timing sequences for thoracic dimension Z (upper diagrams) and the central venous pressure (CVP) are shown in FIG. 4a for mechanical positive

pressure respiration and in **FIG. 4b** for spontaneous breathing. The abscissa is the time axis with cardiac pulse cycles as the axis unit.

[0036] By means of conventional algorithms of pulse contour analysis, the appropriately programmed apparatus 4 calculates the stroke volume (LVSV) (lower diagrams in **FIGS. 4a** and **4b**) of the left ventricle (LV), the stroke volume variation SVV, and if applicable other desired cardiovascular readings. The transmural pressure is calculated as the relevant pressure, according to the following formula:

$$P_{\text{transmural}} = P_{\text{ao}} - f(C) * PIT$$

[0037] The corrective function $f(C)$ is a function of compliance (C) of the arterial system or primarily the aorta 2, where compliance is preferably determined according to a non-linear wind kessel model, and the corrective function $f(C)$ can, for example, take the form of

$$f(C) = 1 - \exp(-a * C)$$

[0038] with (a) as the adaptation parameter, but which in any case increases monotonically as the compliance increases and may assume values between 0 and 1.

[0039] A phase shift Ph1 must be taken into consideration due to the transpulmonary and left ventricular path. As an alternative to the stroke volume variation SVV, only the upward (Δ_{up}) or downward (Δ_{down}) deviations of the stroke volume could be taken into consideration. Δ_{up} and Δ_{down} may also be required for calculating other desired cardiovascular parameters.

[0040] The phase shift Ph0 between the beginning of the rise of the thoracic dimension curve Z, i.e. beginning thoracic compliance, and the beginning of the rise of the curve of the central venous pressure CVP indicates whether mechanical respiration or spontaneous breathing is taking place. Such a phase shift Ph0 is noticeable only with spontaneous breathing (**FIG. 4b**) but not with mechanical positive pressure respiration (**FIG. 4a**). However, the less distinct phase shift of the local maximums of the curves of thoracic dimension Z and the central venous pressure can also be used as an alternative criterion.

[0041] By means of the above explained criterion, it is decided whether the cardiac volume responsiveness indicator (CVRI) should be calculated according to the formula

$$CVRI = k * (SVV / \Delta CVP)$$

[0042] for mechanical positive-pressure respiration, or according to the formula

$$CVRI = 1 - m * (\Delta CVP / SVV)$$

[0043] for spontaneous breathing, where ΔCVP is the variation of the central venous pressure during a breathing cycle. The curves obtained as a function of the end-diastolic volume EDV are shown in **FIG. 5a** for positive pressure respiration and in **FIG. 5b** for spontaneous breathing.

[0044] The k, l and m values are adaptation parameters. As a rule, these would be estimated or experimentally determined constants, but suitable adaptation functions can be used as well, for example with the goal being that both functions provide the same value in their application range when the EDV for the patient's cardiac volume responsiveness indicator has the same value.

[0045] Monitor 9 provides the calculated CVRI together with the calculated cardiac output (CO), and—if the patient's filling status is unsatisfactory—this CVRI can help the attending physician to decide whether volume must be supplied or medication is preferable.

[0046] Accordingly, while only a few embodiments of the present invention have been shown and described, it is obvious that many changes and modifications may be made thereunto without departing from the spirit and scope of the invention.

What is claimed is:

1. An apparatus for the continuous determination of a parameter characterizing a patient's left ventricular pumping action, comprising

a first input channel for continuous recording of a variable physiological first reading directly dependent on the left ventricular pumping action, and

an evaluation unit for calculating said parameter characterizing the left ventricular pumping action,

wherein said apparatus also comprises a second input channel for continuous recording of a variable physiological second reading which at least approximately indicates the patient's intrathoracic pressure (ITP) or is dependent on same,

wherein said evaluation unit is programmed for calculating the parameter characterizing the patient's left ventricular pumping action from said first reading, using a corrective function based on said second reading.

2. The apparatus according to claim 1, wherein said first input channel is configured for reading a pressure transducer signal, wherein said first reading at least approximately corresponds to the patient's aortic pressure, and wherein programming of the evaluation unit allows the calculation of said parameter characterizing the patient's left ventricular pumping action by means of a pulse contour analysis.

3. The apparatus according to claim 2, wherein said first reading which at least approximately corresponds to the aortic pressure is an arterial pressure.

4. The apparatus according to claim 3, wherein said arterial pressure is a pressure measured close to the aorta.

5. The apparatus according to claim 2, wherein said pulse contour analysis is based on a non-linear wind kessel model.

6. The apparatus according to claim 2, wherein the corrective function has the form of

$$P_{\text{transmural}} = P_{\text{ao}} - f(C) * PIT$$

wherein

P_{ao} is said first reading which at least approximately corresponds to the aortic pressure,

P_{IT} is said second reading which at least approximately expresses the intrathoracic pressure (ITP), and

$f(C)$ is a function which depends on the compliance (C) of the arterial system or the aorta and which increases monotonically as the compliance increases and may assume values between 0 and 1, and wherein the transmural pressure ($P_{\text{transmural}}$) is the determining pressure in the pulse contour analysis.

7. The apparatus according to claim 6, wherein said function $f(C)$ has the formula

$$f(C) = 1 - \exp(-a * C)$$

wherein $\exp(-a \cdot C)$ is an exponential function with argument $-a \cdot C$, wherein (C) is compliance of the arterial system or the aorta, and (a) is an estimated or experimentally determined constant.

8. The apparatus according to claim 7, wherein a dependence of the compliance (C) on the transmural pressure (P_{transmural}) is assumed and that both of these values are calculated by means of iteration.

9. The apparatus according to claim 1, wherein said second input channel is configured for reading a pressure transducer signal, and wherein said second reading at least approximately corresponds to the patient's central venous pressure (CVP).

10. The apparatus according to claim 1, wherein said parameter that characterizes the patient's left ventricular pumping action is one of a group of cardiac output, stroke volume and a parameter directly calculated from those.

11. An apparatus for the continuous determination of the cardiac volume responsiveness indicator, comprising:

a first input channel for the continuous recording of a variable physiological first reading directly dependent on a patient's left ventricular pumping action,

a second input channel for continuous recording of a variable physiological second reading at least approximately representing the patient's intrathoracic pressure (ITP),

a third input channel for continuous recording of a third reading which depends directly on the patient's state of respiration, and

an evaluation unit for calculating said cardiac volume responsiveness indicator,

wherein the evaluation unit is programmed to use said second and third readings to select a function that can be used for the patient's current state of respiration and based on this function, to calculate said volume responsiveness indicator from said first and second readings.

12. The apparatus according to claim 11, wherein said first reading is a size of the left ventricle which is determined by means selected from the group consisting of X ray densitometry, positron emission tomography, transesophageal echo cardiography, transthoracic echo cardiography and other two- or three-dimensional imaging techniques.

13. The apparatus according to claim 11, wherein said first reading which depends on the patient's left ventricular pumping function is a reading determined by a measurement selected from the group consisting of plethysmography, measuring the electric impedance, measuring the electric conductivity, ultrasound, measuring the pressure in the *Arteria pulmonalis*, and direct flow measurement.

14. The apparatus according to claim 11, wherein said first input channel (5a) is configured for reading a pressure transducer signal, and wherein said first reading at least approximately corresponds to the patient's aortic pressure.

15. The apparatus according to claim 11, wherein said evaluation unit is programmed to calculate from the temporal variability of said first reading at least one of a value selected from the group consisting of stroke volume variation (SVV), systolic pressure variation (SPV), pulse pressure variation (PPV) and a similar value.

16. The apparatus according to claim 14, wherein said evaluation unit is programmed to calculate at least one of a value selected from the group consisting of stroke volume

variation (SVV), systolic pressure variation (SPV), pulse pressure variation (PPV) and a similar value, from the first reading by means of pulse contour analysis, using a corrective function formed with the second reading.

17. The apparatus according to claim 16, wherein said corrective function has the formula:

$$P_{\text{transmural}} = P_{\text{ao}} - f(C) \cdot \text{PIT}$$

wherein P_{ao} is said first reading which at least approximately corresponds to the aortic pressure,

PIT is said second reading which at least approximately expresses the intrathoracic pressure (ITP), and

f(C) is a function which depends on compliance (C) of the arterial system or the aorta and which increases monotonically as the compliance increases and may assume values between 0 and 1,

and wherein transmural pressure (P_{transmural}) is a determining pressure in the pulse contour analysis.

18. The apparatus according to claim 17, wherein said function f(C) has the formula

$$f(C) = 1 - \exp(-a \cdot C)$$

wherein $\exp(-a \cdot C)$ is an exponential function with argument $-a \cdot C$, wherein (C) is compliance of the arterial system or of the aorta (2), and (a) is an estimated or experimentally determined constant.

19. The apparatus according to claim 18, wherein a dependence of the compliance (C) on transmural pressure (P_{transmural}) is assumed and that both of these values are calculated by means of iteration.

20. The apparatus according to claim 11, wherein selection of the function to be applied to the patient's current respiration status consists of a choice between a first function valid for the artificial respiration of the patient and a second function valid for the patient's spontaneous breathing.

21. The apparatus according to claim 20, wherein said first function valid for the artificial respiration of the patient has the formula

$$\text{CVRI} = k \cdot (\text{XXV} / \Delta \text{PIT})$$

and that said second function valid for the patient's spontaneous breathing has the formula

$$\text{CVRI} = 1 - m \cdot (\Delta \text{PIT} / \text{XXV})$$

wherein CVRI is the cardiac volume responsiveness indicator, XXV is one of the group of stroke volume variation (SVV), systolic pressure variation (SVP), pulse pressure variation (PPV) and a similar value describing the left ventricular pumping function, ΔPIT is the variation of said second reading which at least approximately expresses the intrathoracic pressure (ITP) during a breathing cycle, and wherein k, l and m are adaptation parameters.

22. The apparatus according to claim 21, wherein said adaptation parameters k, l and m are adaptation functions.

23. The apparatus according to claim 21, wherein said adaptation parameters k, l and m are estimated or experimentally calculated constants.

24. The apparatus according to claim 23, wherein said adaptation parameters k, l and m are selected such that both functions result in a same value in their application range when an end-diastolic volume for the patient's cardiac volume responsiveness indicator (CVRI) remains the same.

25. The apparatus according to claim 20, wherein the programming of the evaluation unit allows for determination of an onset of the patient's inhalation based on temporal variability of said third reading; and the determination whether said first function valid for the artificial respiration of the patient or said second function valid for the patient's spontaneous breathing should be used, depending on a phase shift between the onset of inhalation and the beginning of the rise of said second reading which at least approximately expresses the intrathoracic pressure (ITP), such that artificial respiration has to be assumed for a phase shift lying below a threshold value between the onset of inhalation and the beginning of the rise of said second reading, and spontaneous breathing has to be assumed for a phase shift lying above a threshold value between the onset of inhalation and the beginning of the rise of said second reading.

26. The apparatus according to claim 11, wherein said third reading at least approximately corresponds to the patient's thoracic compliance.

27. The apparatus according to claim 26, wherein said third input channel is configured for reading one of the group of a strain gauge (DMS) or a sensor measuring the impedance.

28. The apparatus according to claim 11, wherein said third reading at least approximately corresponds to one of the group of the respiration pressure and the volume flow of the patient's tidal air.

29. The apparatus according to claim 11, wherein said second input channel is configured for reading a pressure transducer signal, and wherein said second reading at least approximately corresponds to the patient's central venous pressure.

30. A method of continuous determination of a parameter characterizing a patient's left ventricular pumping action, comprising the steps of:

recording a variable physiological first reading directly dependent on the left ventricular pumping action;

continuously recording a variable physiological second reading which at least approximately indicates the patient's intrathoracic pressure (ITP) or is dependent on same; and

calculating said parameter characterizing the left ventricular pumping action from said first reading, using a corrective function based on said second reading.

31. The method of claim 30, wherein said first reading is taken from a pressure transducer signal which at least approximately corresponds to the patient's aortic pressure, and wherein said parameter characterizing the patient's left ventricular pumping action is calculated by means of a pulse contour analysis.

32. The method according to claim 31, wherein said first reading which at least approximately corresponds to the aortic pressure is an arterial pressure.

33. The method according to claim 32, wherein said arterial pressure is a pressure measured close to the aorta.

34. The method according to claim 31, wherein said pulse contour analysis is based on a non-linear wind kessel model.

35. The method according to claim 31, wherein the corrective function has the form of

$$P_{\text{transmural}} = P_{\text{ao}} - f(C) * P_{\text{IT}}$$

wherein

P_{ao} is said first reading which at least approximately corresponds to the aortic pressure,

P_{IT} is said second reading which at least approximately expresses the intrathoracic pressure (ITP), and

$f(C)$ is a function which depends on compliance (C) of the arterial system or the aorta and which increases monotonically as the compliance increases and may assume values between 0 and 1,

and wherein transmural pressure ($P_{\text{transmural}}$) is the determining pressure in the pulse contour analysis.

36. The method according to claim 35, wherein said function $f(C)$ has the formula

$$f(C) = 1 - \exp(-a * C)$$

wherein $\exp(-a * C)$ is the exponential function with the argument $-a * C$, wherein (C) is the compliance of the arterial system or the aorta, and (a) is an estimated or experimentally determined constant.

37. The method according to claim 36, wherein a dependence of the compliance (C) on the transmural pressure ($P_{\text{transmural}}$) is assumed, and both of these values are calculated by means of iteration.

38. The method according to claim 30, wherein said second reading is taken from a pressure transducer signal, and wherein said second reading at least approximately corresponds to the patient's central venous pressure (CVP).

39. The method according to claim 30, wherein said parameter that characterizes the patient's left ventricular pumping action is selected from the group consisting of cardiac output, stroke volume and a parameter directly calculated from those.

40. A method of continuous determination of the cardiac volume responsiveness indicator, comprising the steps of

recording a variable physiological first reading directly dependent on the patient's left ventricular pumping action,

recording a variable physiological second reading at least approximately representing the patient's intrathoracic pressure (ITP),

recording a third reading which depends directly on the patient's state of respiration,

using said second and third readings to select a function that can be used for the patient's current state of respiration, and, based on this function,

calculating said cardiac volume responsiveness indicator from said first and second readings.

41. The method according to claim 40, wherein said first reading is the size of the left ventricle which is determined by means of a method selected from the group consisting of X ray densitometry, positron emission tomography, transthoracic echo cardiography and other two- or three-dimensional imaging techniques.

42. The method according to claim 40, wherein said first reading which depends on the patient's left ventricular pumping function is a reading determined by a measurement selected from the group consisting of plethysmography, measuring electric impedance, measuring electric conduc-

tivity, ultrasound, measuring pressure in *Arteria pulmonalis*, and direct flow measurement.

43. The method according to claim 40, wherein said first reading is taken from a pressure transducer signal, and wherein said first reading at least approximately corresponds to the patient's aortic pressure.

44. The method according to claim 40, wherein from the temporal variability of said first reading at least one of the group of stroke volume variation (SVV), systolic pressure variation (SPV), pulse pressure variation (PPV) and a similar value is calculated.

45. The method according to claim 44, wherein said evaluation one of the group of stroke volume variation (SVV), systolic pressure variation (SPV), pulse pressure variation (PPV) and a similar value, is calculated from said first reading by means of pulse contour analysis, using a corrective function formed with the second reading.

46. The method according to claim 45, wherein said corrective function has the formula

$$P_{transmural} = P_{ao} - f(C) * PIT$$

wherein

P_{ao} is said first reading which at least approximately corresponds to the aortic pressure,

PIT is said second reading which at least approximately expresses the intrathoracic pressure (ITP), and

$f(C)$ is a function which depends on compliance (C) of the arterial system or the aorta and which increases monotonically as the compliance increases and may assume values between 0 and 1,

and wherein the transmural pressure ($P_{transmural}$) is the determining pressure in the pulse contour analysis.

47. The method according to claim 46, wherein said function $f(C)$ has the formula

$$f(C) = 1 - \exp(-a * C)$$

wherein $\exp(-a * C)$ is the exponential function with argument $-a * C$, wherein (C) is compliance of the arterial system or of the aorta (2), and (a) is an estimated or experimentally determined constant.

48. The method according to claim 47, wherein a dependence of the compliance (C) on the transmural pressure ($P_{transmural}$) is assumed and that both of these values are calculated by means of iteration.

49. The method according to claim 40, wherein selection of the function to be applied to the patient's current respiration status consists of a choice between a first function valid for the artificial respiration of the patient and a second function valid for the patient's spontaneous breathing.

50. The method according to claim 49, wherein said first function valid for the artificial respiration of the patient has the formula

$$CVRI = k * (XXV / \Delta PIT)$$

and that said second function valid for the patient's spontaneous breathing has the formula

$$CVRI = 1 - m * (\Delta PIT / XXV)$$

wherein CVRI is the cardiac volume responsiveness indicator, XXV is selected from the group consisting of stroke volume variation (SVV), systolic pressure variation (SVP), pulse pressure variation (PPV) and a similar value describing the left ventricular pumping function, ΔPIT is the variation of said second reading which at least approximately expresses the intrathoracic pressure (ITP) during a breathing cycle, and wherein k, l and m are adaptation parameters.

51. The method according to claim 50, wherein said adaptation parameters k, l and m are adaptation functions.

52. The method according to claim 50, wherein said adaptation parameters k, l and m are estimated or experimentally calculated constants.

53. The method according to claim 52, wherein said adaptation parameters k, l and m are selected such that both functions result in a same value in their application range when an end-diastolic volume for the patient's cardiac volume responsiveness indicator (CVRI) remains the same.

54. The method according to claim 49, wherein the onset of the patient's inhalation is determined based on the temporal variability of said third reading; and it is determined whether said first function valid for the artificial respiration of the patient or said second function valid for the patient's spontaneous breathing should be used, depending on the phase shift between the onset of inhalation and the beginning of the rise of said second reading which at least approximately expresses the intrathoracic pressure (ITP), such that artificial respiration has to be assumed for a phase shift lying below a threshold value between the onset of inhalation and the beginning of the rise of said second reading, and spontaneous breathing has to be assumed for a phase shift lying above a threshold value between the onset of inhalation and the beginning of the rise of said second reading.

55. The method according to claim 40, wherein said third reading at least approximately corresponds to the patient's thoracic compliance.

56. The method according to claim 55, wherein said third reading is taken from a signal of a strain gauge (DMS) or a sensor measuring the impedance.

57. The method according to claim 56, wherein said third reading at least approximately corresponds to one of the respiration pressure and the volume flow of the patient's tidal air.

58. The method according to claim 40, wherein said second reading is taken from a pressure transducer signal, and wherein said second reading at least approximately corresponds to the patient's central venous pressure.

* * * * *

专利名称(译)	用于确定心血管参数的装置		
公开(公告)号	US20040249297A1	公开(公告)日	2004-12-09
申请号	US10/743515	申请日	2003-12-22
[标]申请(专利权)人(译)	PFEIFFER ULRICH J BURGER托尔斯滕		
申请(专利权)人(译)	PFEIFFER ULRICH J. BURGER托尔斯滕		
当前申请(专利权)人(译)	压出性医疗系统SE		
[标]发明人	PFEIFFER ULRICH J BURGER THORSTEN		
发明人	PFEIFFER, ULRICH J. BURGER, THORSTEN		
IPC分类号	A61B5/00 A61B5/02 A61B5/0205 A61B5/0215 A61B5/113 A61B10/00 A61M16/00 G06F17/00		
CPC分类号	A61B5/02028 A61B5/0205 A61B5/02152 A61B5/1135 A61B5/02108		
优先权	10260762 2002-12-23 DE		
其他公开文献	US7314449		
外部链接	Espacenet USPTO		

摘要(译)

一种连续监测由动脉中的压力传感器测量的动脉压的装置，该压力被认为是大致对应于主动脉压的读数 P_{ao} 。原则上，动脉压可以在主动脉，主动脉附近或动脉树中测量。为了提供第二次读数，该装置通过输入通道连续监测中心静脉压（CVP），其被认为是大致对应于胸内压（ITP）的读数PIT。第三次读数通过输入通道提供，作为表示胸部顺应性的读数Z。通过脉冲轮廓分析的已知算法，该装置使用根据公式 $P_{transmural} = P_{ao} - f(C) * PIT$ 计算的透壁压力作为确定压力来计算每搏输出量变化。根据公式 $CVRI = k * (SVV / \Delta CVP)$ 或根据公式 $CVRI = 1 - m * (\Delta CVP / SVV)$ 的自发呼吸计算心脏容积响应性指标（CVRI）用于机械正呼吸。

