

US007654962B2

(12) **United States Patent**  
**Sullivan**

(10) **Patent No.:** **US 7,654,962 B2**  
(45) **Date of Patent:** **Feb. 2, 2010**

(54) **RADIATION STRESS NON-INVASIVE BLOOD PRESSURE METHOD**

(75) Inventor: **Patrick K. Sullivan**, Kailua, HI (US)  
(73) Assignee: **Hoana Medical, Inc.**, Honolulu, HI (US)  
(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 330 days.

(21) Appl. No.: **10/562,416**  
(22) PCT Filed: **Jun. 28, 2004**  
(86) PCT No.: **PCT/US2004/020767**

§ 371 (c)(1),  
(2), (4) Date: **Dec. 23, 2005**

(87) PCT Pub. No.: **WO2005/000108**  
PCT Pub. Date: **Jan. 6, 2005**

(65) **Prior Publication Data**  
US 2007/0265535 A1 Nov. 15, 2007

**Related U.S. Application Data**

(60) Provisional application No. 60/482,460, filed on Jun. 26, 2003.  
(51) **Int. Cl.**  
**A61B 5/02** (2006.01)  
**A61B 5/00** (2006.01)  
(52) **U.S. Cl.** ..... **600/481**; 600/483; 600/485; 600/300  
(58) **Field of Classification Search** ..... 600/300, 600/481, 483, 484, 485, 488, 500-503, 508-526  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,245,648 A 1/1981 Trimmer et al.  
4,320,766 A 3/1982 Alihanka et al.  
4,429,699 A 2/1984 Hatschek  
4,459,991 A 7/1984 Hatschek  
4,475,557 A 10/1984 Hatschek et al.  
4,509,527 A 4/1985 Fraden  
4,562,723 A 1/1986 Hubner  
4,695,955 A 9/1987 Faisandier  
4,827,763 A 5/1989 Bourland et al.  
4,926,866 A 5/1990 Lee  
4,961,428 A \* 10/1990 Nikias et al. .... 600/512

(Continued)

FOREIGN PATENT DOCUMENTS

WO WO 03/082111 10/2003

OTHER PUBLICATIONS


International Search Report for PCT Application No. PCT/US2004/020767.

*Primary Examiner*—Charles A Marmor, II  
*Assistant Examiner*—Navin Natnithithadha  
(74) *Attorney, Agent, or Firm*—Fulwider Patton LLP

(57) **ABSTRACT**

The invention determines the energy dispersion via acoustic, electromechanical or other related physiological signals collected from a patient that lies down or otherwise engages a discretized sensing array. Signals are monitored over a range of frequencies and collected in the time domain or frequency domain. A computing machine determines the energy from the signal measured over various elements of the array and calculates the momentum flux. Blood pressure is determined directly from the momentum flux calculation.

**26 Claims, 3 Drawing Sheets**

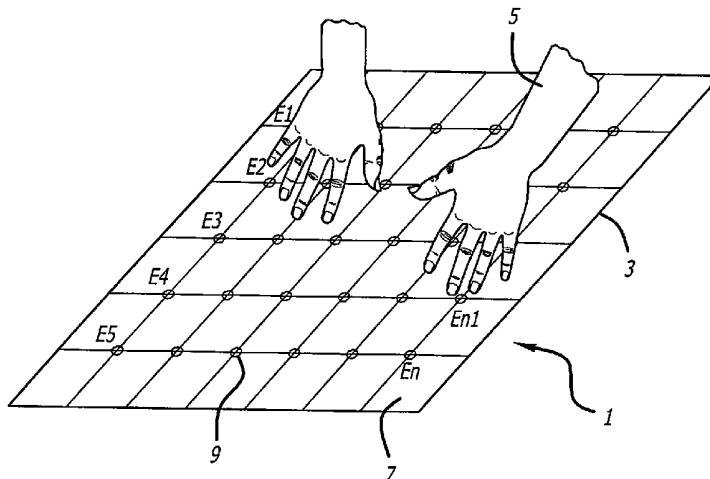


# US 7,654,962 B2

Page 2


## U.S. PATENT DOCUMENTS

4,974,598	A	*	12/1990	John .....	600/509	6,280,392	B1	8/2001	Yoshimi et al.
5,002,060	A		3/1991	Nedivi		6,315,719	B1	11/2001	Rode et al.
5,137,033	A		8/1992	Norton		6,375,621	B1	4/2002	Sullivan
5,144,284	A		9/1992	Hammett		6,402,691	B1	6/2002	Peddicord et al.
5,241,964	A		9/1993	McQuilkin		6,445,299	B1	9/2002	Rojas, Jr.
5,282,474	A		2/1994	Valdes Sosa et al.		6,450,957	B1	9/2002	Yoshimi et al.
5,292,340	A		3/1994	Crosby et al.		6,468,234	B1 *	10/2002	Van der Loos et al. .... 600/595
5,309,916	A		5/1994	Hatschek		6,475,153	B1	11/2002	Khair et al.
5,448,996	A		9/1995	Belin et al.		6,497,658	B2	12/2002	Roizen et al.
5,515,865	A		5/1996	Scanlon		6,506,153	B1	1/2003	Littek et al.
5,590,650	A		1/1997	Genova		6,540,673	B2	4/2003	Gopinathan et al.
5,808,552	A		9/1998	Wiley et al.		6,547,743	B2	4/2003	Brydon
5,846,206	A		12/1998	Bader		6,575,902	B1	6/2003	Burton
5,853,005	A		12/1998	Scanlon		6,648,828	B2	11/2003	Friedman et al.
5,942,979	A		8/1999	Luppino		6,652,466	B2	11/2003	Sugo et al.
5,964,720	A		10/1999	Pelz		6,689,069	B2	2/2004	Bratteli et al.
5,989,193	A		11/1999	Sullivan		6,746,403	B2	6/2004	Kolluri et al.
6,014,346	A		1/2000	Malone		6,826,426	B2	11/2004	Lange et al.
6,047,203	A		4/2000	Sackner et al.		6,984,207	B1	1/2006	Sullivan et al.
6,050,940	A		4/2000	Braun et al.		6,988,989	B2	1/2006	Weiner et al.
6,146,332	A		11/2000	Pinsonneault et al.		7,314,451	B2 *	1/2008	Halperin et al. .... 600/534
6,195,008	B1		2/2001	Bader		2003/0018241	A1	1/2003	Mannheimer
6,198,394	B1		3/2001	Jacobsen et al.		2004/0111045	A1	6/2004	Sullivan et al.
6,248,064	B1		6/2001	Gopinathan et al.		2005/0190062	A1	9/2005	Sullivan et al.
6,261,237	B1		7/2001	Swanson et al.		2005/0190068	A1	9/2005	Gentry et al.
						2006/0063982	A1	3/2006	Sullivan et al.

\* cited by examiner

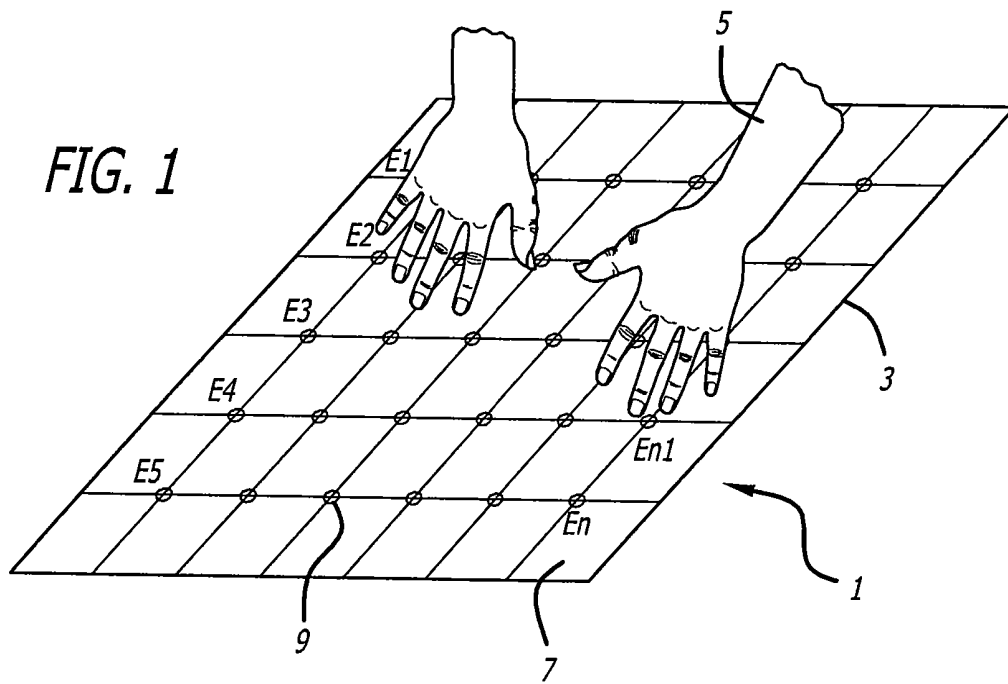

**FIG. 2**

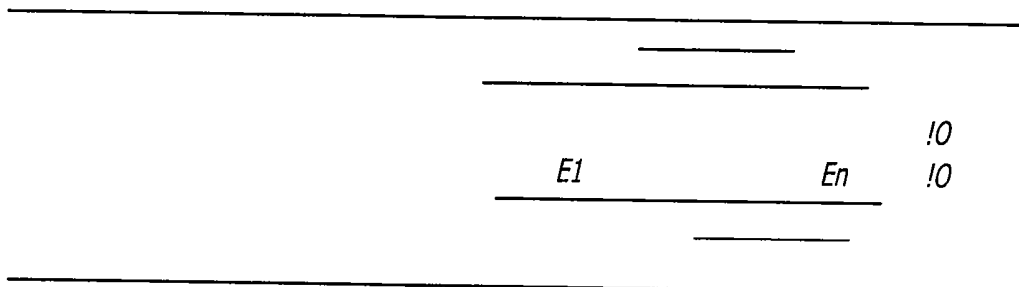

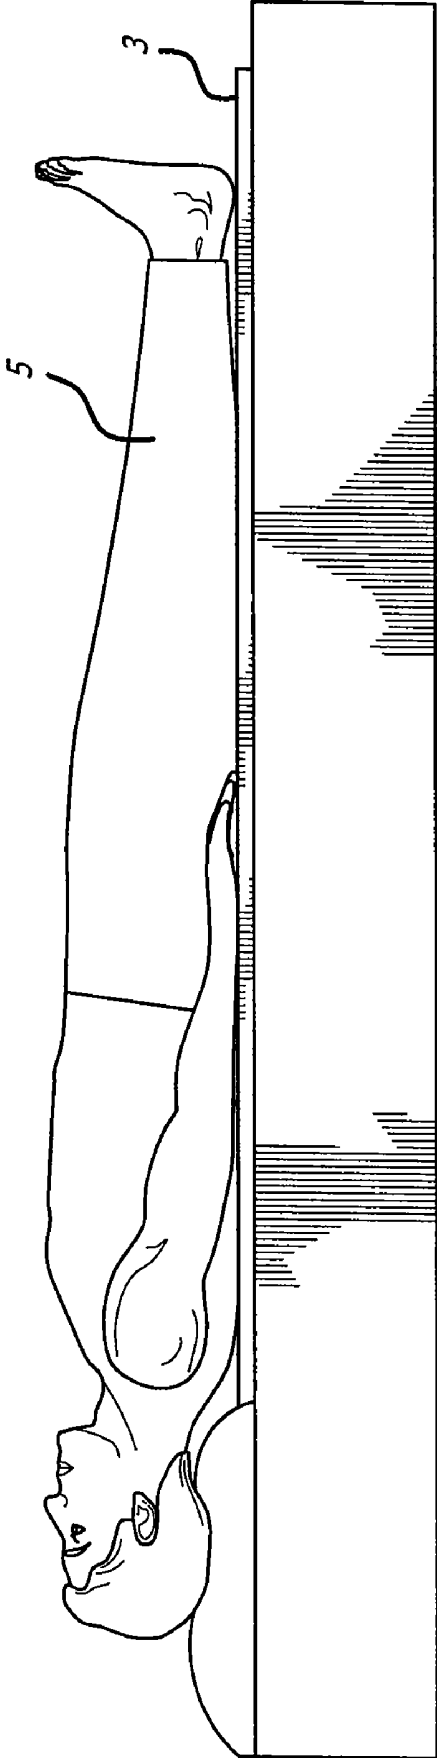


FIG. 3

FIG. 4


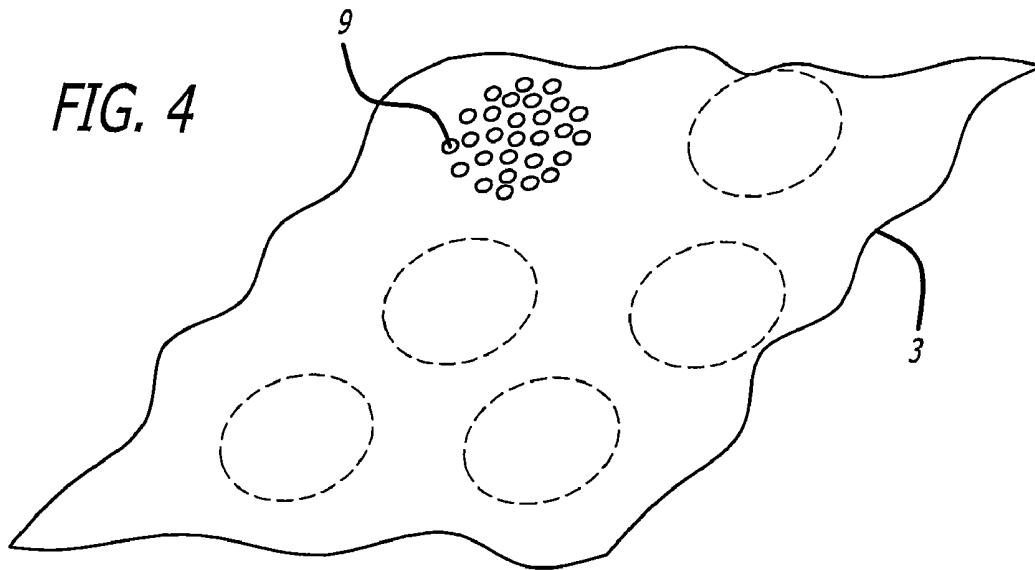


FIG. 5

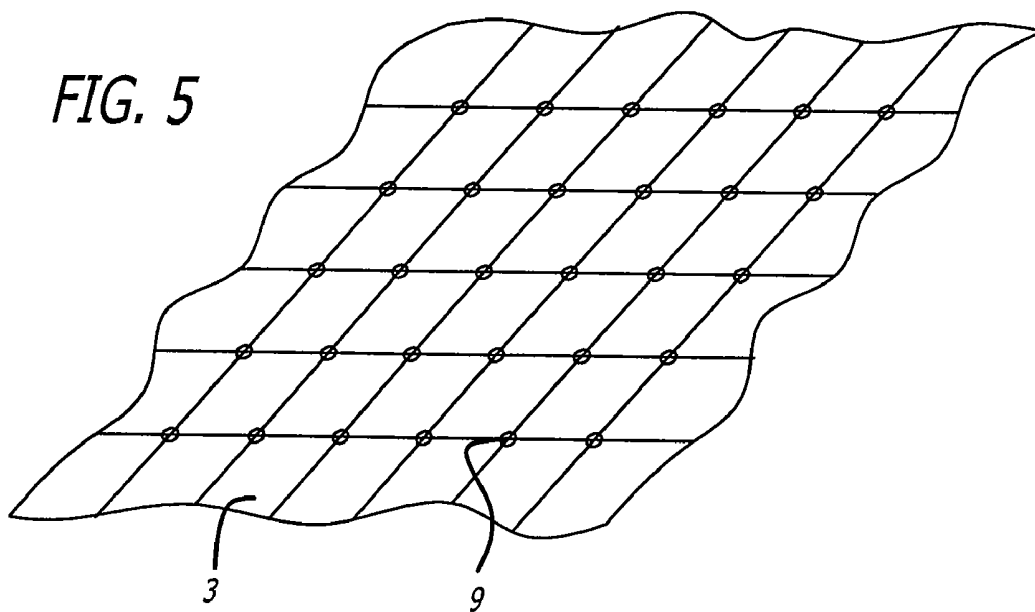

1

## RADIATION STRESS NON-INVASIVE BLOOD PRESSURE METHOD

### RELATED APPLICATIONS

This application is the National Stage of International Application No. PCT/US2004/020767, filed Jun. 28, 2004, which claims the benefit of U.S. Provisional Application No. 60/482,460, filed Jun. 26, 2003.

### BACKGROUND OF THE INVENTION

Current methods for measurement of blood pressure and other vital signs are inefficient. Many measurements of patient vital signs are invasive procedures that are uncomfortable or inconvenient for the patient. Typically, the measurement of blood pressure requires the use of a cuff around the arm of a patient and is a non-continuous "spot-check" that does not reflect the true state of patient physiology.

Needs exist for improved methods of continuous non-invasive blood pressure measurements.

### SUMMARY OF THE INVENTION

The present invention is a system that provides non-invasive, real-time, continuous collection and processing of signals from a patient to determine the current condition of the patient. The present invention relates preferably to the measurement of blood pressure. This measurement includes the average, mean, systolic and diastolic arterial blood pressure. However, the present invention is not limited to the measurement of blood pressure; other vital signs can be measured and processed as well. The present method also provides for continuous, non-invasive monitoring of hypertension and other related medical conditions.

The present invention uses acoustic, electromechanical or other related physiological signals collected from a patient. To operate the monitoring device, the patient engages discretized, discrete, separated sensors in one or more discrete sensing arrays installed in a bed, chair or any other equipment that the patient will use. The patient lies down on, sits on, stands on, or otherwise engages the discretized sensing array, and signals are monitored over a range of frequencies or at a specific frequency. Data is collected as a time series or another similar method. Data is transferred to a computing device in the form of a voltage signal via wire, fiber optics or wireless technology.

The energy spectra of each array point are determined and then are used to determine the variance of each array. Computational analysis of the data collected is used to determine energy momentum flux of blood flowing through the patient. Non-time series methods are used to determine energy at various array points or at a combination of array points. Momentum flux is determined from the data collected by the discretized separate sensors in each array. Blood pressure is related to the momentum flux through a mathematical algorithm. A computing device performs the computation of blood pressure.

These and further and other objects and features of the invention are apparent in the disclosure, which includes the above and ongoing written specification, with the claims and the drawings.

### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a diagram of the monitoring system with a discretized array.

2

FIG. 2 is a diagram of energy spectra collected from location 1 to location n.

FIG. 3 is a schematic representation of a person lying on an array of sensors.

FIGS. 4 and 5 are schematic representations of portions of sheets with sensor arrays.

### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

The present invention is a system that provides real-time, continuous collection and processing of signals from a patient to determine the condition of the patient. The present invention relates preferably to the measurement of blood pressure. The measurements include the average, mean, systolic and diastolic arterial blood pressure. The present invention is not limited to the measurement of blood pressure; other vital functions, for example, heart rate and pulses and electrical signals, can be measured and processed as well. The present method provides for continuous, non-invasive monitoring of hypertension and other related medical conditions.

FIG. 1 shows a diagram of a monitoring system 1 and a discretized array 3 of separate sensors 9. The present invention uses acoustic, electromechanical or other related physiological signals collected from a patient 5 in contact with the discretized sensors in the sensing array 3. The discretized sensing array 3 is a relatively flat device 7 with individual sensing arrays 9 dispersed throughout the surface of the discretized sensing array 3. The patient 5 lies down on, stands on, or otherwise engages the discretized sensing array 3, and signals are monitored over a range of frequencies or at a specific frequency, as shown in FIG. 3. Data is collected as a time series or another similar method. Data is collected from individual sensing arrays 9, from grid locations 1 to n, via acoustic, electromechanical or other physiological signals.

The discretized sensing array 3 can have sensors arranged in various regular or irregular configurations. FIG. 4 and FIG. 5 show different arrangements of individual sensors 9 on a portion of the large discretized sensing array.

The discretized sensing array 3 provides time series data that is analyzed to produce energy spectra at locations 1 to n, as shown in FIG. 2. The data is used to determine the variance of the time series signals. Computational analysis of data collected is used to determine momentum flux of energy through the patient.

Blood pressure is related to the momentum flux through a mathematical model. The following relationship relates the incoming data to blood pressure:

$$Pa = K * (E1 - En) = \text{Average pressure due to excess flow of momentum}$$

Pa = Average blood pressure

K = Constant

E1 = Summation of energy spectra (area under the curve - variance of time series) at location 1 x Pulse wave velocity

En = Summation of energy spectra (area under the curve - variance of time series) at location n x Pulse wave velocity

A computing device performs the computation of blood pressure. The results of computation are output to the user.

The radiation stress, non-invasive blood pressure device of the present invention uses time series analysis and computational methods to process acoustic, electromechanical or other physiological signals from the patient. An energy spectrum is created by the sensing arrays to calculate the variance.

The variance is the area under the energy spectra curve. Non-time series methods are used to determine energy at various array points.

While the invention has been described with reference to specific embodiments, modifications and variations of the invention may be constructed without departing from the scope of the invention, which is described in the following claims.

The invention claimed is:

1. A radiation stress, non-invasive vital sign monitoring method comprising:
  - providing one or more discretized sensor arrays, engaging the one or more discretized sensor arrays, measuring and collecting discretized acoustic or electro-mechanical or physiological signals with the discretized sensor arrays,
  - transmitting discretized signals to a receiving and computer device,
  - the receiving and computer device produces time series data from various discretized sensor array signals,
  - calculates energy spectrum from the time series data, determines variance of each discretized sensor array, and calculates a value for vital signs of a patient.
2. The method of claim 1, wherein the vital signs are average, mean, systolic and diastolic arterial blood pressure.
3. The method of claim 1, wherein the vital signs are hypertension.
4. The method of claim 1, further comprising lying on, standing on, or otherwise contacting the discretized sensor arrays.
5. The method of claim 1, wherein the collecting the discretized acoustic or electromechanical physiological signals is performed over a range of frequencies.
6. The method of claim 1, wherein the collecting the discretized acoustic or electromechanical physiological signals is performed over a single frequency.
7. The method of claim 1, wherein the collecting acoustic or electromechanical physiological signals further comprises collecting data in a time domain or frequency domain.
8. The method of claim 1, wherein the calculating a value for vital signs is performed with non-time series methods for determining energy at various array points or a combination of array points.
9. The method of claim 1, wherein the transmitting of discretized signals comprises transmitting discretized signals via wire, fiber optics or wirelessly.
10. The method of claim 1, further comprising providing continuous, real-time monitoring of a patient's vital signs.
11. The method of claim 1, further comprising calculating the momentum flux from data gathered from the discretized sensor arrays.
12. The method of claim 11, further comprising calculating a patient's vital signs from the momentum flux.

13. The method of claim 1, wherein the one or more discretized sensor arrays are not attached to the patient.

14. A radiation stress, non-invasive vital sign monitoring device comprising:

- one or more discretized sensor arrays for measuring and collecting discretized acoustic or electromechanical signals from a patient,
- a surface on the one or more discretized sensor arrays for engaging a patient,
- a transmission system for transmitting data collected by the one or more discretized sensor arrays,
- a receiving device for receiving the transmitted data from the one or more discretized sensor arrays, and
- a computing device connected to the receiving device for calculating values of vital signs of the patient by producing time series data from various discretized sensor array signals,
- calculating energy spectrum from the time series data, and
- determining variance of each discretized sensor array.

15. The device of claim 14, wherein the vital signs are average, mean, systolic and diastolic arterial blood pressure.

16. The device of claim 14, wherein the vital signs are hypertension.

17. The device of claim 14, wherein the patient lies on, stands on, or otherwise contacts the discretized sensor arrays.

18. The device of claim 14, wherein the discretized sensor arrays collect the discretized acoustic or electromechanical signals over a range of frequencies.

19. The device of claim 14, wherein the discretized sensor arrays collect the discretized acoustic or electromechanical signals over a single frequency.

20. The device of claim 14, wherein the discretized sensor arrays collect the discretized acoustic or electromechanical signals in a time domain or frequency domain.

21. The device of claim 14, wherein the computing device calculates a value for vital signs with non-time series methods for determining energy at various array points or a combination of array points.

22. The device of claim 14, wherein the transmission system transmits discretized signals via wire, fiber optics or wirelessly.

23. The device of claim 14, wherein the discretized sensor arrays provide continuous, real-time monitoring of a patient's vital signs.

24. The device of claim 14, wherein the computing device computes the momentum flux from data gathered from the discretized sensor arrays.

25. The device of claim 24, wherein the computing device further computes a patient's vital signs from the momentum flux.

26. The device of claim 14, wherein the one or more discretized sensor arrays are not attached to the patient.

\* \* \* \* \*

UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : 7,654,962 B2  
APPLICATION NO. : 10/562416  
DATED : February 2, 2010  
INVENTOR(S) : Patrick K. Sullivan

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:


On the Title Page:

The first or sole Notice should read --

Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 736 days.

Signed and Sealed this

Twenty-eighth Day of December, 2010

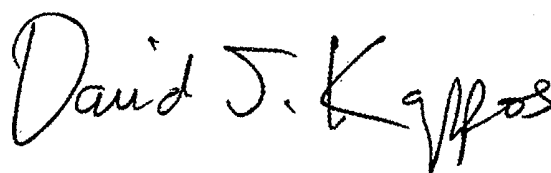A handwritten signature in black ink that reads "David J. Kappos". The signature is written in a cursive, slightly slanted style.

David J. Kappos  
*Director of the United States Patent and Trademark Office*

专利名称(译)	放射应力无创血压法		
公开(公告)号	<a href="#">US7654962</a>	公开(公告)日	2010-02-02
申请号	US10/562416	申请日	2004-06-28
[标]申请(专利权)人(译)	SULLIVAN PATRICK K		
申请(专利权)人(译)	SULLIVAN PATRICK K		
当前申请(专利权)人(译)	HOANA MEDICAL , INC.		
[标]发明人	SULLIVAN PATRICK K		
发明人	SULLIVAN, PATRICK K.		
IPC分类号	A61B5/02 A61B5/00 A61B A61B5/021 A61B5/11 A61B7/00		
CPC分类号	A61B5/021 A61B5/6892 A61B5/11 A61B7/00 A61B2562/0204 A61B2562/0247 A61B2562/046		
代理机构(译)	FULWIDER PATTON LLP		
优先权	60/482460 2003-06-26 US		
其他公开文献	US20070265535A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

#### 摘要(译)

本发明通过声学，机电或其他相关的生理信号确定能量分散，所述生理信号是从躺在或以其他方式接合于烧焦的传感阵列的患者收集的。在一定频率范围内监视信号，并在时域或频域中收集信号。计算机器根据在阵列的各种元件上测量的信号确定能量并计算动量通量。血压直接由动量通量计算确定。

