



(19) **United States**

(12) **Patent Application Publication**
Graindorge et al.

(10) **Pub. No.: US 2003/0013945 A1**

(43) **Pub. Date: Jan. 16, 2003**

(54) **MANAGING MEDICAL DATA OF AN ACTIVE IMPLANTABLE DEVICE SUCH AS PACEMAKER, DEFIBRILLATOR, CARADIOVERTOR AND/OR MULTISITE DEVICE FOR A CARDIOLOGIST**

(52) **U.S. Cl. 600/300; 707/104.1**

(57) **ABSTRACT**

(76) **Inventors: Laurence Graindorge, Chatenay-Malabry (FR); Marcel Limousin, Paris (FR)**

Correspondence Address:
ORRICK, HERRINGTON & SUTCLIFFE LLP
666 Fifth Avenue
New York, NY 10103-0001 (US)

A process for managing medical data in an active implantable medical device such as a pacemaker, defibrillator, cardiometer or multisite device for use of the medical data by a specialized follow-up practitioner such as a cardiologist. The process is characterized by reading by telemetry the memory data (12) of the device (10) in a patient by use of a programmer (14), memorizing in a database within the programmer the raw medical data thus read, the database having a memory field (24) containing an identifier of the patient (26), an address (28) of the follow-up practitioner such as a cardiologist or a regular practitioner ensuring the medical follow-up of the patient, as well as the aforementioned raw medical data (30), transmitting by a telematic way (36) to that follow-up practitioner, at the corresponding address, the medical data relating to the identified patient, and collecting, treating and presenting to the follow-up practitioner the medical data thus transmitted. A dedicated software (44) implemented on a microcomputer (40) at the disposal of the follow-up practitioner is used for the collection of the raw data and its treatment, processing and display for use by the follow-up practitioner.

(21) **Appl. No.: 10/145,573**


(22) **Filed: May 13, 2002**

(30) **Foreign Application Priority Data**

May 15, 2001 (FR)..... 01 06374

Publication Classification

(51) **Int. Cl.⁷ G06F 17/00; G06F 7/00; A61B 5/00**

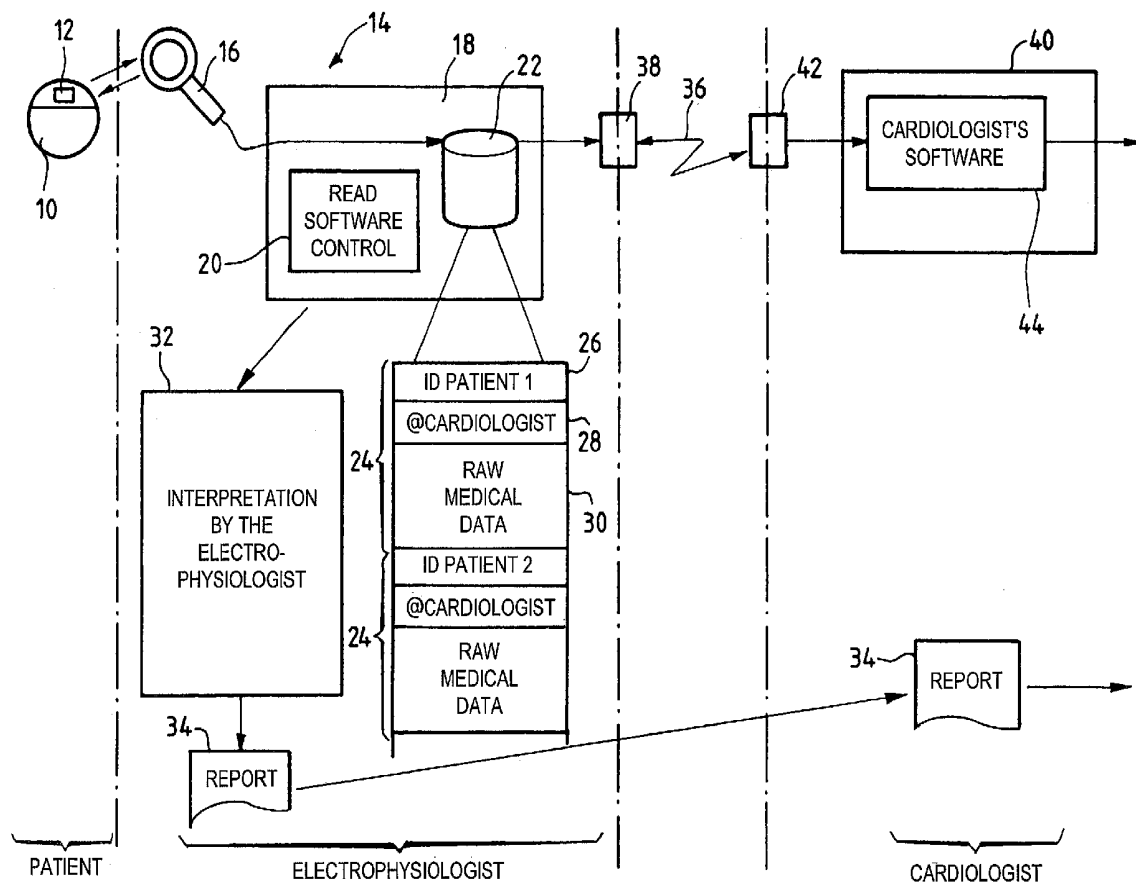

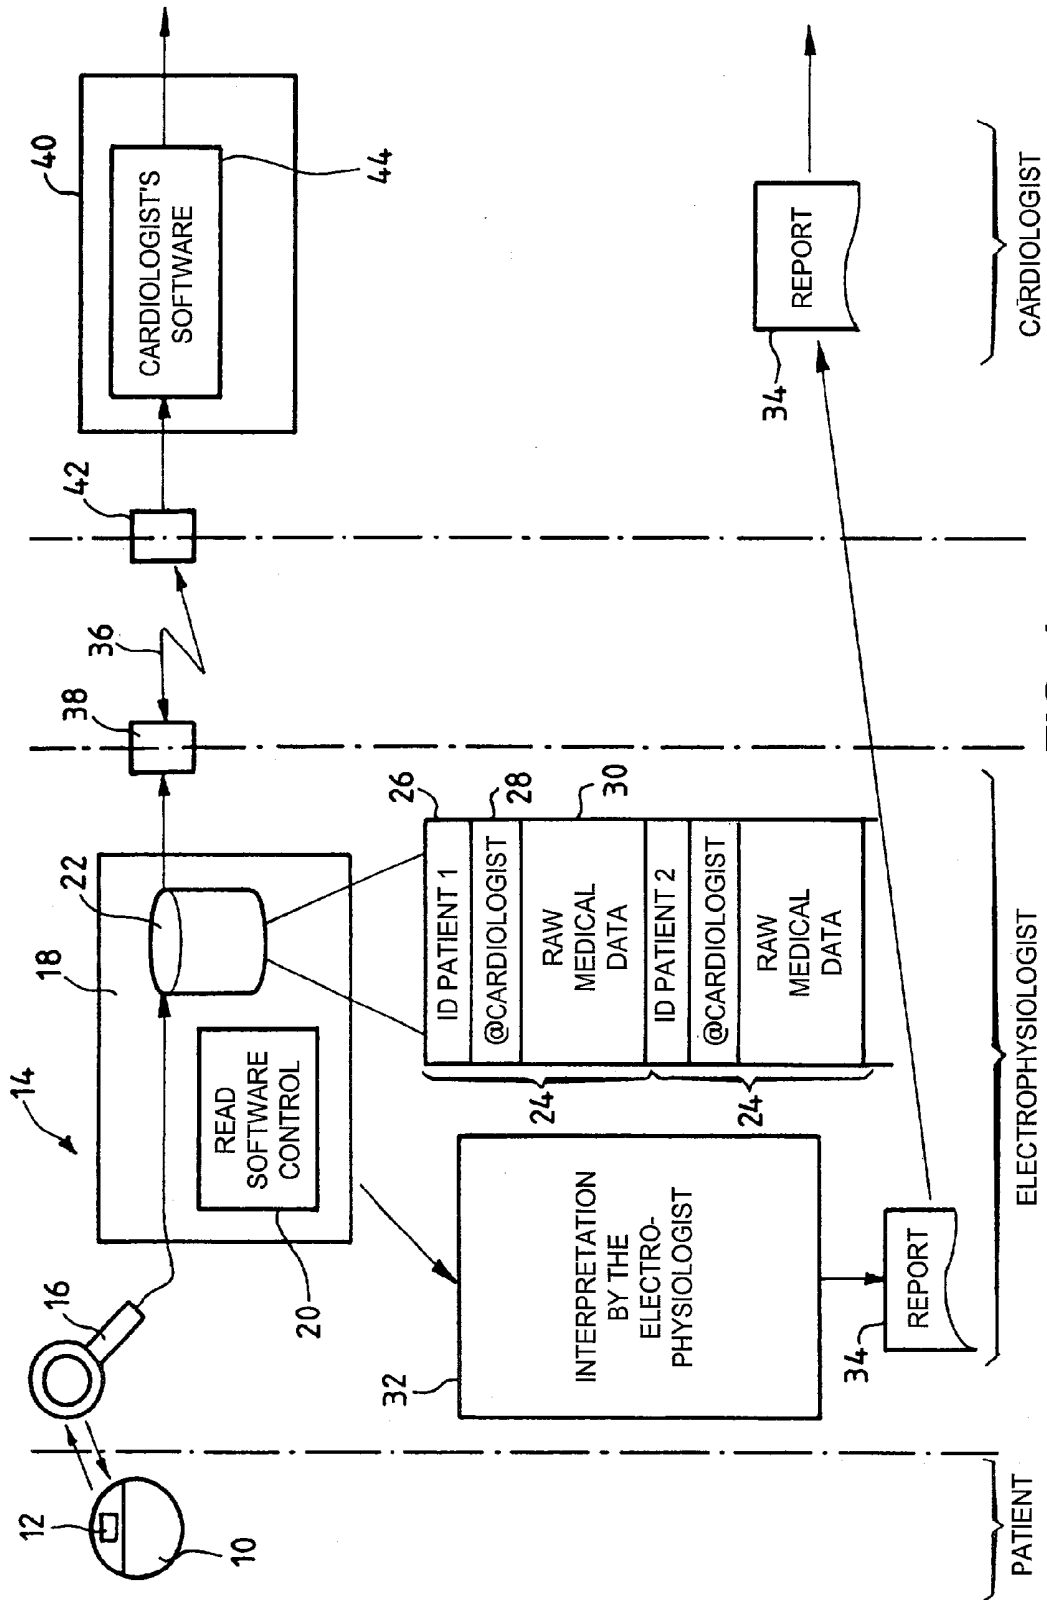


FIG. 1

**MANAGING MEDICAL DATA OF AN ACTIVE
IMPLANTABLE DEVICE SUCH AS PACEMAKER,
DEFIBRILLATOR, CARADIOVERTOR AND/OR
MULTISITE DEVICE FOR A CARDIOLOGIST**

FIELD OF THE INVENTION

[0001] The present invention is directed to "active implantable medical devices" as such devices are defined by the Jun. 20, 1990 directive 90/385/CEE of the Council of the European Communities. This definition includes pacemaker, defibrillator, cardiovertor and/or multisite devices for the treatment of the disorders of the cardiac rhythm, and neurological apparatuses, medical substance diffusion pumps, cochlear implants, implanted biological sensors, etc., as well as devices for the measurement of pH or an intra-corporeal impedance (such as the measurement of the transpulmonary impedance or the intracardiac impedance).

BACKGROUND OF THE INVENTION

[0002] Active implantable medical devices to which the present invention applies, hereinafter called "implants", comprise a data memory that can be read by means of an external programmer by telemetry techniques that are well known to persons of ordinary skill in the art. The external programmer is associated with a microcomputer, comprising a display screen, a keyboard or other input interface for the entry of control commands and data, as well as memory and associated software for data memorizing (storage) and data processing.

[0003] The practitioner who uses the programmer is generally a specialized doctor, for example, the physician who implanted the device or one who works in close co-operation with the implanting physician, oftentimes in the same hospital complex. Such a practitioner has total control over the operation of the programmer and thus direct access to the data stored in the memory of the implant, as well as the ability to read, set and modify the various "programming" controls, i.e., the commands used to modify the parameter settings and the functioning of the implant.

[0004] The starting point of the present invention is the observation that the memory of the implant contains data likely to be of interest another practitioner (referred to herein as the "follow-up practitioner"), either another medical specialist or the regular practitioner physician who ensures the current follow-up of the patient. If one takes the example of a cardiac implant, the first practitioner (i.e., the practitioner who is the implanting physician or works with that person) is a specialized doctor known as an "electrophysiologist" or "rhythmologist", and the follow-up practitioner is a specialized doctor such as a cardiologist or the regular practitioner who ensures the current follow-up of the patient following implantation.

[0005] The cardiologist typically receives a report from the electrophysiologist, who includes interpretations related to the functioning of the implant and eventually to the heartbeat rate. However, the clinical state of the patient implies a focus on employing other parameters in particular to cure pathologies, to prescribe a medication, etc.; tasks that are specific to the cardiologist and not in the area of the electrophysiologist. It will be noted that the cardiologist has the report of the electrophysiologist and the results of the clinical examinations performed by or for the cardiologist,

on which a diagnosis, such as desired changes to device operating parameters and/or prescribed medications, may be based.

[0006] However, there are certain data the knowledge of which could be interesting to help the follow-up practitioner (e.g., the cardiologist) to pose a diagnosis. This preexistent data are stored in the memory of the implant.

[0007] Generally, however the follow-up practitioner does not have a programmer that would allow him to read the memory of the implant, which would also suppose that he or she is trained to use such a programmer, apparatus that also is able to modify the programming of the implant. Moreover, the reading of the complete set of data within the memory implies a selection and analysis of that data, work that in practice makes difficult the usage of a programmer by the follow-up practitioner.

**OBJECTS AND SUMMARY OF THE
INVENTION**

[0008] It is, therefore, an object of the invention to resolve this difficulty by proposing a process for medical data management, data which are issued from the memory of the implant, to provide the follow-up practitioner with information enabling him or her to help to pose a diagnosis or to write a prescription, without requiring the acquisition of additional equipment by the follow-up practitioner.

[0009] To this end, the present invention is broadly directed to a process for managing medical data in an implant for use by more than one practitioner. One such process is characterized by the stages of: reading by telemetry the memory data of the implant device in a patient by means of a programmer; memorizing in a database of the programmer the raw medical data thus read, the database including a memory field containing an identifier of the patient, an address of a follow-up practitioner (e.g. a cardiologist or a regular practitioner) ensuring the medical follow-up of the patient, and the aforementioned raw medical data; transmitting by a telematic way to the follow-up practitioner, at the corresponding address, the medical data relating to the identified patient; collecting, treating and presenting to the follow-up practitioner the medical data thus transmitted by means of a dedicated software implemented on a microcomputer at the disposal of the follow-up practitioner.

[0010] It will be understood to those of ordinary skill in the art that the present invention is not limited to the preferential example described here that relates to the field of cardiology (with the duality electrophysiologist/cardiologist or electrophysiologist/regular practitioner), but applies mutatis-mutandis to other medical fields implying intervening practitioner parties with distinct competences in respective fields of competence, in different places and at different times, each one needing some of the particular information contained in the implant.

BRIEF DESCRIPTION OF THE DRAWING

[0011] Other features, characteristics, and advantages of the present invention will appear to a person of ordinary skill in the art in view of the following detailed description of preferred embodiments of the present invention, made with reference to the annexed drawing **FIG. 1**, which schemati-

cally represents the elements used within the framework of a process in accordance with a preferred embodiment.

DETAILED DESCRIPTION OF THE INVENTION

[0012] As indicated above, in particular in the field of the cardiology, the need exists to offer to the cardiologists, who look after pathologies of the patient (medication, cardiac insufficiency, etc.), but who do not control the pulse generator implant and thus do not have access to the data stored by the implant, a certain amount of information allowing them to help them form a diagnosis.

[0013] It will be noted that the present invention does not relate to the way in which these data are elaborated, data which preexist in the memory of the implant, nor the diagnosis itself (e.g., the significance or substance of the data or what conclusions one would draw from the data), which is posed by the follow-up practitioner using the data which are provided to him. Nor does the invention relate to other information the follow-up practitioner has on the patient and his pathology.

[0014] In the illustrated example, implant **10** is a pacemaker or a defibrillator able to store in an internal memory **12** medical data such as electrograms on the atrial or ventricular arrhythmias, the evolution of the ventilation of the patient, patient activity, a ventricular frequency, the presence of sleep apnea, the level of the stimulation capture threshold, the values of intracardiac impedance or other values, etc. This raw medical data or information is available in the memory, but until now it has been reserved to the electrophysiologist because only he has had equipment allowing one to read this data. Hence, this raw information has not been accessible to the cardiologist or the regular practitioner ensuring the current follow-up of the patient.

[0015] In order to read the data stored in memory **12** of implant **10**, the electrophysiologist has a programmer **14** with a telemetry head **16** able to establish a communication with the implant **10**, and a microcomputer **18** providing the various functions of processing and memorizing the data collected by the telemetry head **16**. Microcomputer **18** includes in particular a software **20** for reading the data and controlling (programming) the implant, and memorizing means **22**.

[0016] In a manner characteristic of the invention, when the electrophysiologist interrogates memory **12** of the implant during a control operation, the software **20** will, in addition to the usual functions, create a specific file or record comprising a plurality of zones **24** with for each one an identification field **26** of the patient, an electronic address field **28** of the cardiologist or regular practitioner ensuring the follow-up of this patient, and a field **30** storing a selection of raw medical data which could be useful within the framework of a clinical examination of the patient. These data are stored in a database in memorizing memory **22** of the programmer **14** for later use. Data for different patients will be stored in different files in the database according to the patient identifying information (e.g., an implant identification number, patient number or the like).

[0017] In addition, in a way in itself well known and traditional, the electrophysiologist carries out the work of interpretation on the disorders of the cardiac rate, the syn-

chronization of the various cardiac cavities, etc. (work schematized by block **32**). This interpretation is reduced to an establishment of a report **34**, on paper and/or in electronic media, which will be addressed and delivered to the follow-up practitioner, whether a regular practitioner, a cardiologist or both.

[0018] During the next consultation of the patient, the follow-up practitioner will interrogate the database **22** via a telematic connection **36**, for example, an Internet connection or a direct dial-up (modem to modem) connection or the like. For that purpose, computer **18** of the electrophysiologist is connected to this Internet connection by a corresponding modem **38** (or network ethernet link or the like, collectively hereinafter referred to as a "modem"). The follow-up practitioner can thus download the patient's raw medical data into a computer **40** at the disposal of the follow-up practitioner, typically an equipment of the current type, i.e., one that is not a dedicated programmer device, and similarly equipped with a compatible modem **42**.

[0019] It will be noted that the data transmission from computer **18** of the electrophysiologist to computer **40** of the cardiologist can be done as well as on the initiative of the electrophysiologist. For example, an electronic mail message with a copy of the raw data stored in database **22** attached as a file or imbedded in the message can be sent by the electrophysiologist after the raw data is acquired to each identified follow-up practitioner for each patient. In this later case, the transmission may be operated systematically during or after the consultation at the electrophysiologist's office. In an alternative embodiment a third-party service like a web host server can serve as intermediate link between those two computers. For example, a third-party service provider can be interposed between the electrophysiologist and the cardiologist in which the third-party maintains a database replicating the contents of programmer database **22**. In this embodiment, the raw data information for a given patient is uploaded by the electrophysiologist to the third-party database where it is stored and always accessible to the cardiologist. The cardiologist can then log onto the third-party server and retrieve the patient specific data. In this way, the cardiologist need not depend on the electrophysiologist's computer **18** being running and accessible remotely.

[0020] The existence in field **28** of file **24** of the address of the cardiologist makes it possible to identify the latter and to reserve only for him the transmission of the medical data **30** which are intended for him (and conversely access to the raw data **30**). The raw data thus downloaded could then be consulted and/or analyzed by the use of a dedicated software **44** loaded in computer **40**, to allow, for example, a display of the medical data in the form of a table or a page-screen (not shown).

[0021] Software **44** is preferably a dedicated software for use by the cardiologists, very simple insofar as it contains only controls for remote downloading of the raw data and presentation the raw data on the screen of the computer. From these data, as well as from the report **34** from the electrophysiologist and clinical examinations, the cardiologist will be able to benefit from having all information available on the patient in order to pose a diagnosis or write a suitable prescription.

[0022] It should be understood that the present invention is preferably implemented in software of a microprocessor

controlled implantable medical device and its cooperating programmer device. Suitable implantable devices include, but are not limited to commercial pacemaker products sold under the Talent™ brand, and its associated programmer devices available from Ela Medical, Montrouge, France. These programmers contain modems and data communication programs that are capable of, or can be easily modified to respond to appropriate password protected inquiries from remote devices to allow remote access to selected data files for teletransmission to the remote computer, and alternatively or in addition, an electronic mail messaging system or file transfer system capable of generating an electronic message including the raw data for transmission to a remote device. Similarly, the follow-up practitioner's computer also will have suitable communications and electronic mail (file transfer) capabilities. The telecommunications can be via wire or wireless telephone (modem) and broadband (ethernet, cable modem or DSL) systems or networks.

[0023] Further, it is believed to be well within the abilities of a person of ordinary skill in the art to acquire and/or develop the software to be used in the follow-up practitioner's computer and in the programmer used by the first practitioner to accomplish the raw data transmission and display as discussed herein.

[0024] Advantageously, the present invention can be implemented in software instructions that perform the aforementioned functions and the software can be delivered to the appropriate devices by CD ROM and/or an electronic file transfer such as over the Internet.

[0025] One skilled in the art will appreciate that the present invention can be practiced by other than the described embodiments, which are presented for purposes of illustration and not of limitation.

We claim:

1. A process for managing medical data contained in a memory of an active implantable medical device, comprising:

providing a programmer having a telemetry system to communicate with said active implantable medical device and a database containing at least one patient identifier and associated with each patient identifier, an address of a follow-up practitioner ensuring medical treatment of the patient, and said medical data;

establishing a telemetry link between said active implantable medical device and said programmer;

reading said medical data in said memory using said programmer;

memorizing in said programmer database said medical data thus read;

transmitting to a microcomputer associated with said follow-up practitioner, at the associated follow-up practitioner address, the medical data associated with the identified patient; and

collecting, treating and presenting to the follow-up practitioner the medical data thus transmitted.

2. The process of claim 1 further comprising providing a dedicated software routine implemented on said microcomputer for collecting, treating and presenting said medical data to said follow-up practitioner.

3. The process of claim 1 wherein the follow-up practitioner further comprises one of a cardiologist and a regular practitioner, said database comprises an address for said cardiologist and said regular practitioner, and the transmitting step further comprises transmitting to the cardiologist said medical data at the cardiologist's associated address.

4. The process of claim 1 wherein the follow-up practitioner further comprises one of a cardiologist and a regular practitioner, said database comprises an address for said cardiologist and said regular practitioner, and the transmitting step further comprises transmitting to the regular practitioner said medical data at the regular practitioner's associated address.

5. The process of claim 1 further comprising providing the follow-up practitioner with a microcomputer having a software instruction set dedicated to collecting, treating and presenting said medical data to said follow-up practitioner.

6. The process of claim 1 wherein transmitting said medical data to said follow-up practitioner's microcomputer comprises:

connecting said follow-up practitioner's computer to said programmer;

requesting access to said stored medical data; and

transmitting a copy of said stored medical data to said follow-up practitioner's microcomputer.

7. The process of claim 1 wherein transmitting said medical data to said follow-up practitioner's microcomputer further comprises:

generating at the programmer a data file containing a copy of said medical data; and

electronically transmitting said data file to said follow-up practitioner's microcomputer.

8. The process of claim 7 further comprising providing a remote database wherein transmitting said medical data further comprises transmitting said data file from the programmer to said remote database, storing said data file in the remote database, generating an inquiry at said follow-up practitioner's microcomputer, transmitting said inquiry to the remote database, and, in response to said inquiry, transmitting said data file from the remote database to said follow-up practitioner's microcomputer.

* * * * *

专利名称(译)	为心脏病专家管理有源植入设备 (如起搏器 , 除颤器 , 心脏复律器和/或多点设备) 的医疗数据		
公开(公告)号	US20030013945A1	公开(公告)日	2003-01-16
申请号	US10/145573	申请日	2002-05-13
[标]申请(专利权)人(译)	GRAINDORGE LAURENCE LIMOUSIN MARCEL		
申请(专利权)人(译)	GRAINDORGE LAURENCE LIMOUSIN MARCEL		
当前申请(专利权)人(译)	GRAINDORGE LAURENCE LIMOUSIN MARCEL		
[标]发明人	GRAINDORGE LAURENCE LIMOUSIN MARCEL		
发明人	GRAINDORGE, LAURENCE LIMOUSIN, MARCEL		
IPC分类号	A61N1/372 G06F17/00 G06F7/00 A61B5/00		
CPC分类号	A61N1/37282		
优先权	2001006374 2001-05-15 FR		
其他公开文献	US7236833		
外部链接	Espacenet USPTO		

摘要(译)

一种用于管理有源可植入医疗设备 (例如起搏器 , 除颤器 , 心率计或多点设备) 中的医疗数据的过程, 用于由诸如心脏病专家的专业后续从业者使用医疗数据。该过程的特征在于通过使用程序员 (14) 遥测读取患者中的设备 (10) 的存储器数据 (12), 在程序员内的数据库中存储由此读取的原始医疗数据, 该数据库具有包含患者 (26) 的标识符的记忆区域 (24), 后续从业者的地址 (28), 例如心脏病专家或确保患者的医疗随访的常规医生, 以及上述原始医疗数据 (30), 通过远程信息处理方式 (36) 发送给该后续从业者, 在相应的地址, 与所识别的患者相关的医疗数据, 以及收集, 治疗和向后续从业者提供医疗数据如此传播。在后续从业者处置的微计算机 (40) 上实现的专用软件 (44) 用于收集原始数据及其处理, 处理和显示以供后续从业者使用。

