



US 20070260130A1

(19) **United States**

(12) **Patent Application Publication**  
**Chin**

(10) **Pub. No.: US 2007/0260130 A1**

(43) **Pub. Date: Nov. 8, 2007**

(54) **MEDICAL SENSOR AND TECHNIQUE FOR USING THE SAME**

**Publication Classification**

(76) **Inventor: Rodney P. Chin, Carson City, NV (US)**

(51) **Int. Cl.**  
**A61B 5/00** (2006.01)

(52) **U.S. Cl.** ..... **600/323; 600/344**


Correspondence Address:  
**Nellcor Puritan Bennett LLC**  
**c/o Fletcher Yoder PC**  
**P.O. BOX 692289**  
**HOUSTON, TX 77269-2289 (US)**




(57) **ABSTRACT**




A clip-style sensor may be constructed from materials having shape memory. A clip-style sensor is provided that is able to be flattened in order to simplify transport and storing. The sensors may be held flat by shipping restraints. Such a sensor is able to recover from being flattened and resume a curved shape.




(21) **Appl. No.: 11/415,711**

(22) **Filed: May 2, 2006**

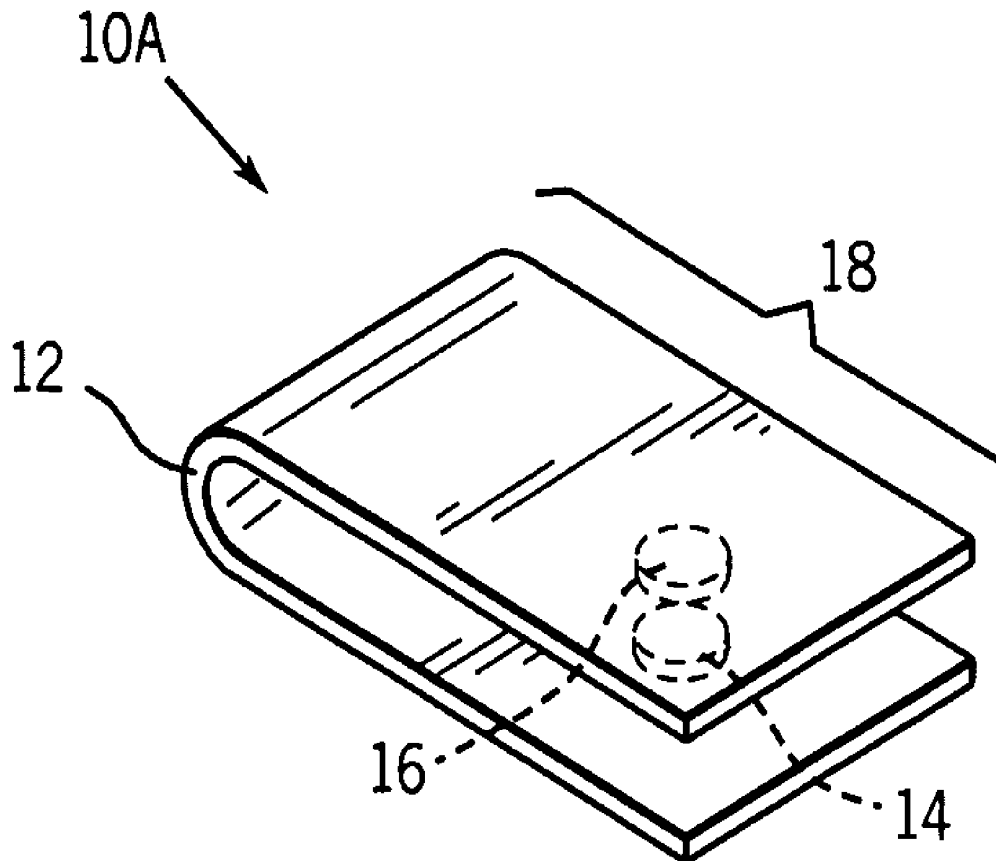

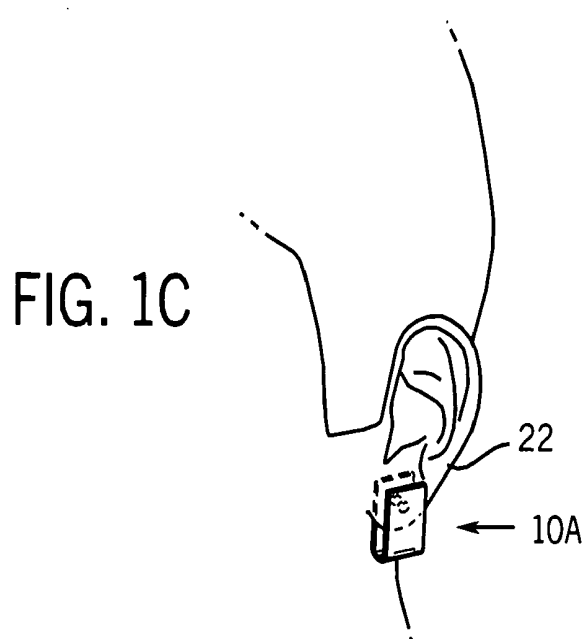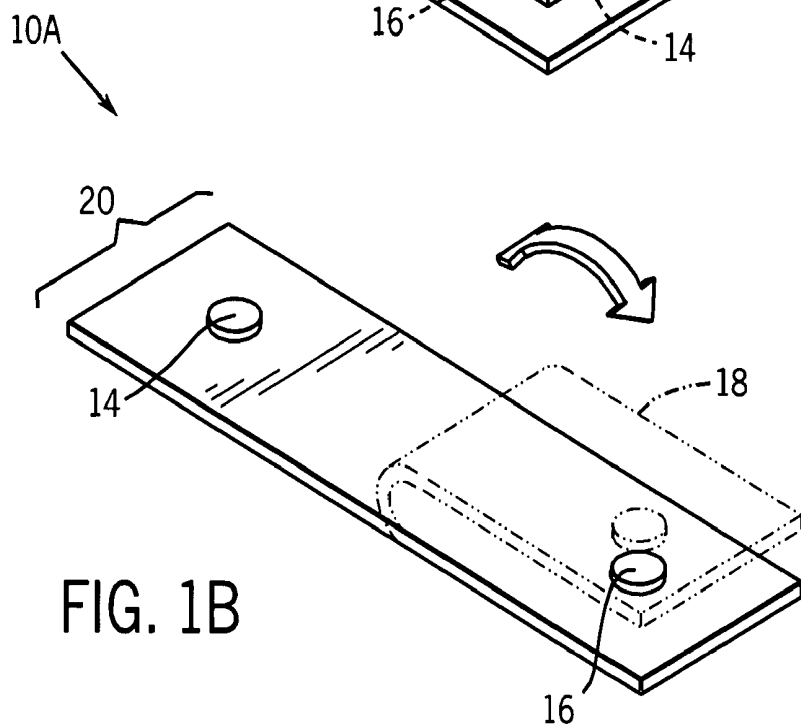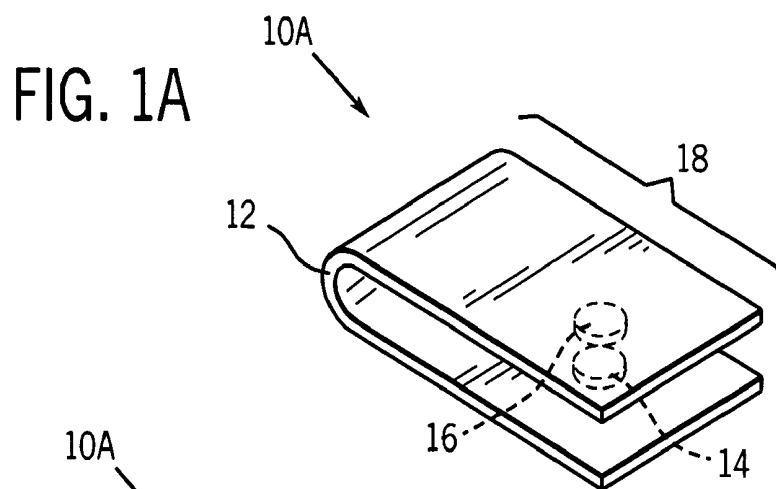

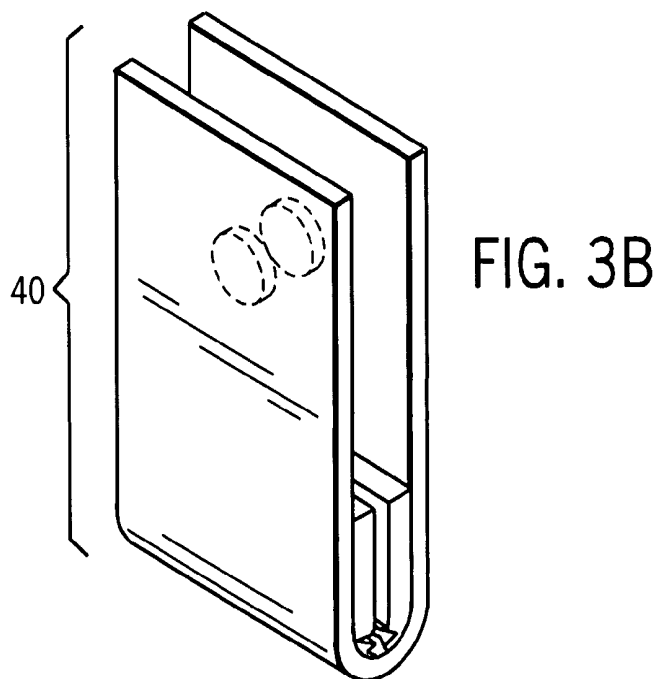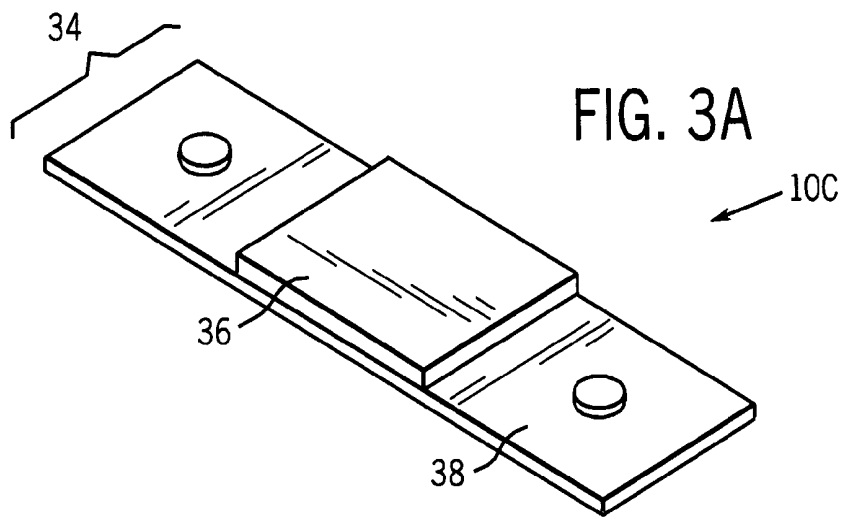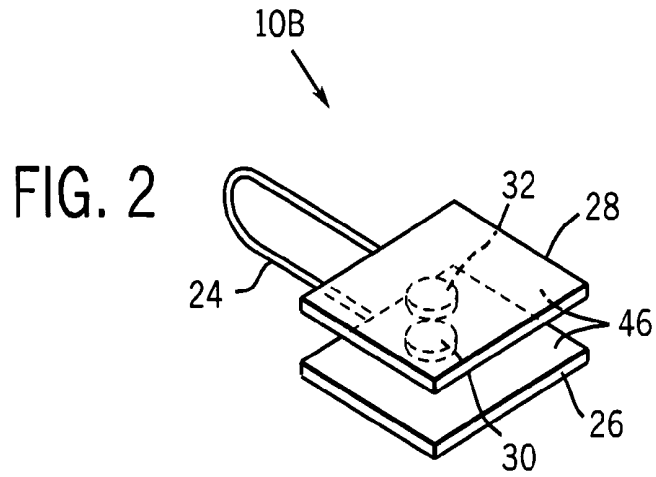

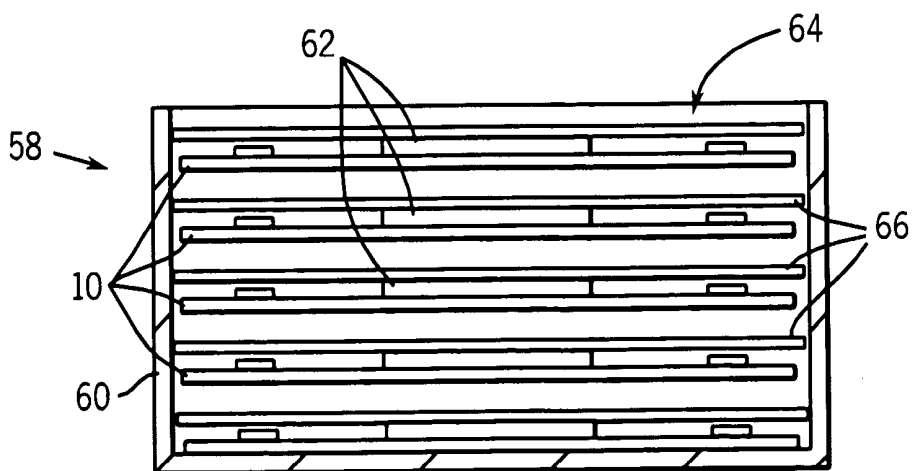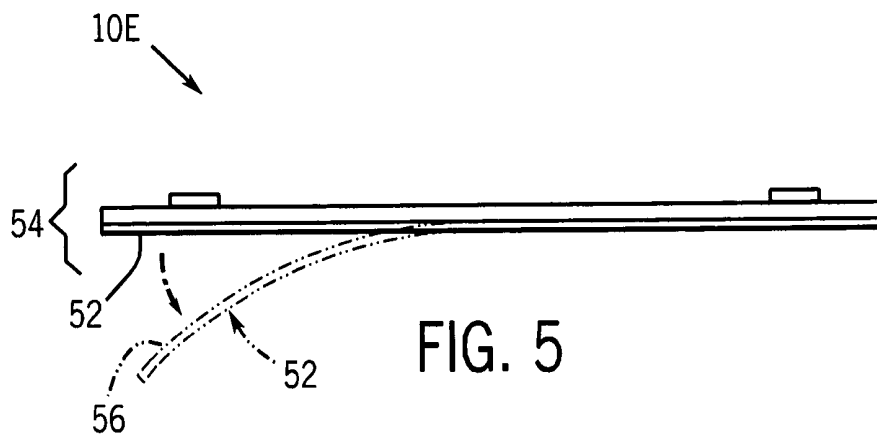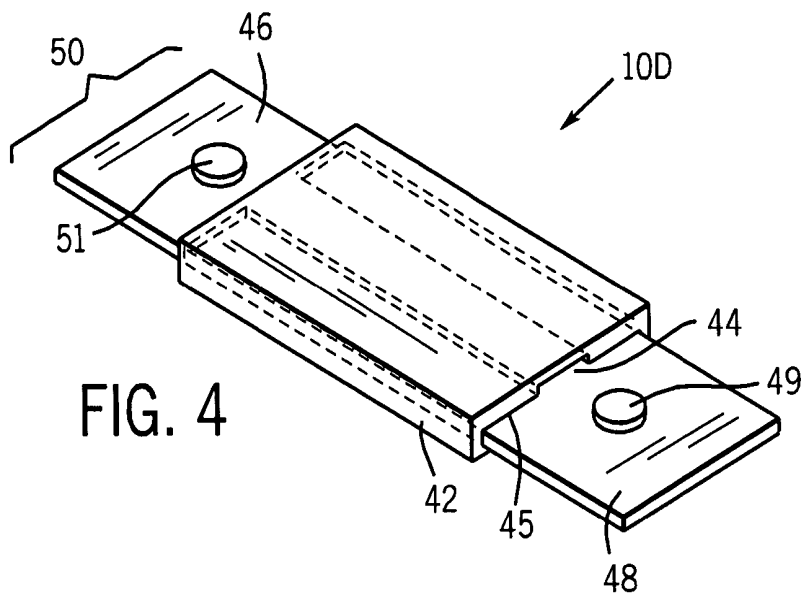

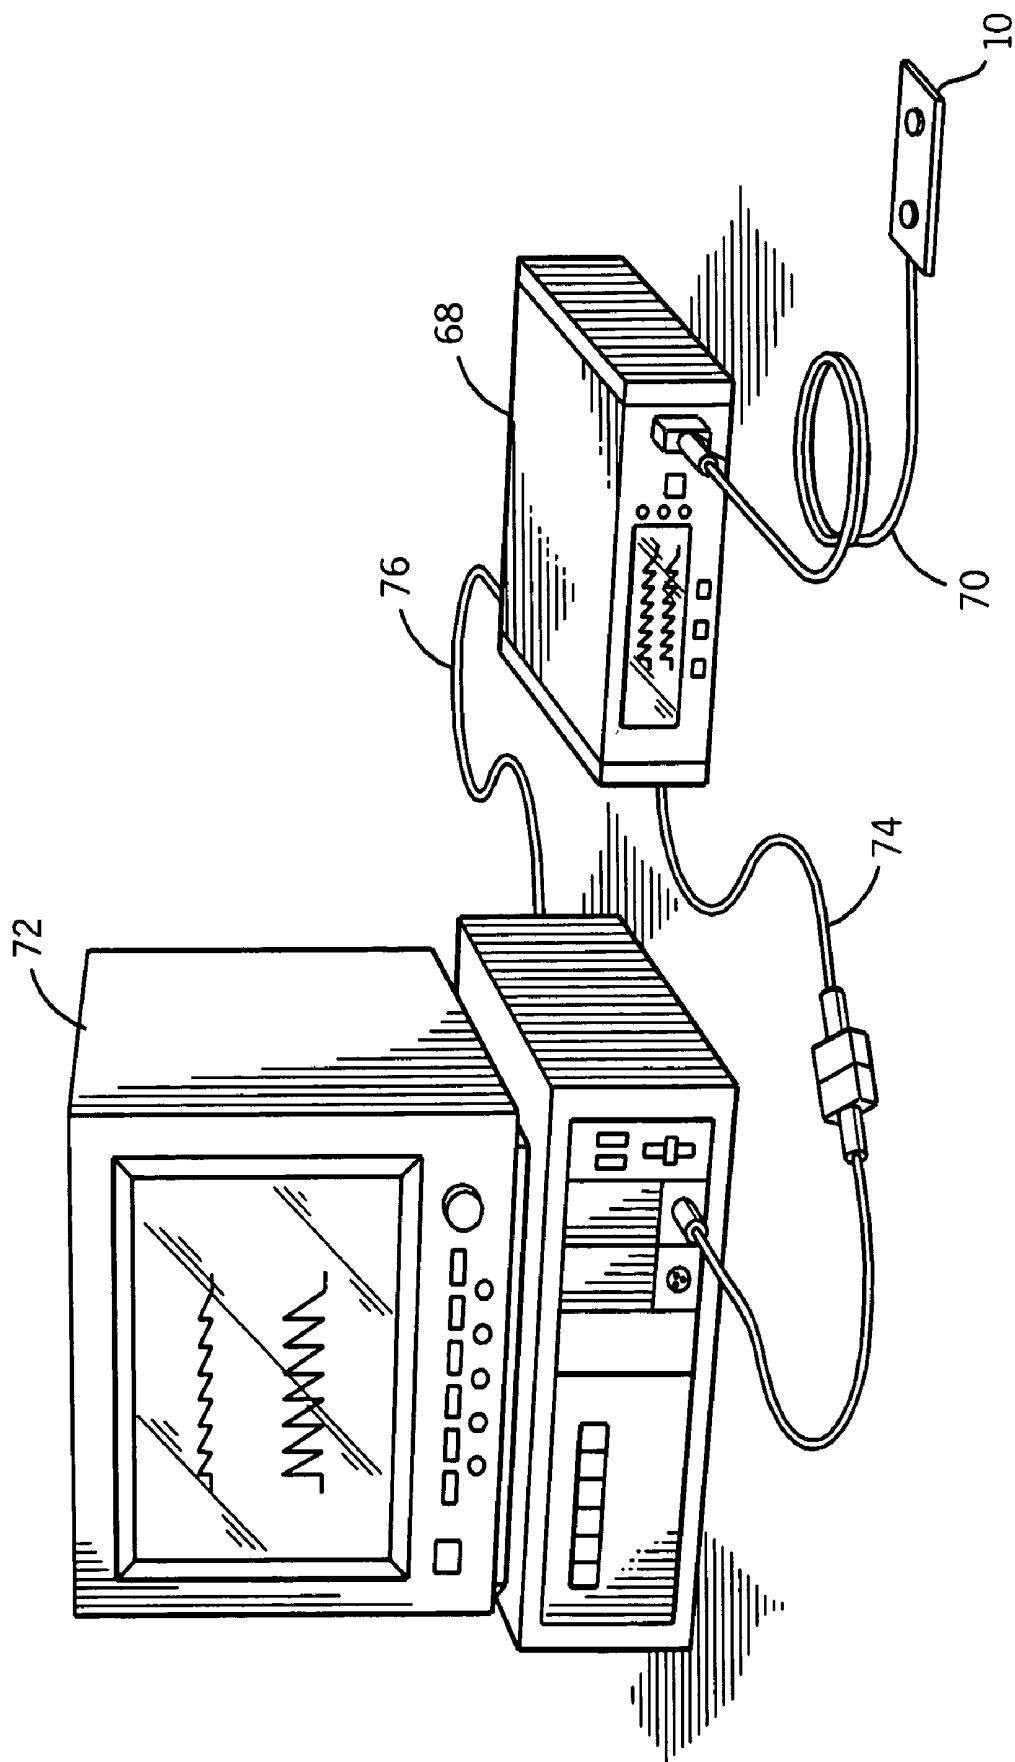


FIG. 7

## MEDICAL SENSOR AND TECHNIQUE FOR USING THE SAME

### BACKGROUND OF THE INVENTION

#### [0001] 1. Field of the Invention

[0002] The present invention relates generally to medical devices and, more particularly, to sensors used for sensing physiological parameters of a patient.

#### [0003] 2. Description of the Related Art

[0004] This section is intended to introduce the reader to various aspects of art that may be related to various aspects of the present invention, which are described and/or claimed below. This discussion is believed to be helpful in providing the reader with background information to facilitate a better understanding of the various aspects of the present invention. Accordingly, it should be understood that these statements are to be read in this light, and not as admissions of prior art.

[0005] In the field of medicine, doctors often desire to monitor certain physiological characteristics of their patients. Accordingly, a wide variety of devices have been developed for monitoring many such physiological characteristics. Such devices provide doctors and other healthcare personnel with the information they need to provide the best possible healthcare for their patients. As a result, such monitoring devices have become an indispensable part of modern medicine.

[0006] One technique for monitoring certain physiological characteristics of a patient is commonly referred to as pulse oximetry, and the devices built based upon pulse oximetry techniques are commonly referred to as pulse oximeters. Pulse oximetry may be used to measure various blood flow characteristics, such as the blood-oxygen saturation of hemoglobin in arterial blood, the volume of individual blood pulsations supplying the tissue, and/or the rate of blood pulsations corresponding to each heartbeat of a patient. In fact, the "pulse" in pulse oximetry refers to the time varying amount of arterial blood in the tissue during each cardiac cycle.

[0007] Pulse oximeters typically utilize a non-invasive sensor that transmits light through a patient's tissue and that photoelectrically detects the absorption and/or scattering of the transmitted light in such tissue. One or more of the above physiological characteristics may then be calculated based upon the amount of light absorbed or scattered. More specifically, the light passed through the tissue is typically selected to be of one or more wavelengths that may be absorbed or scattered by the blood in an amount correlative to the amount of the blood constituent present in the blood. The amount of light absorbed and/or scattered may then be used to estimate the amount of blood constituent in the tissue using various algorithms.

[0008] Conventional pulse oximetry sensors are either disposable or reusable. Disposable sensors are typically simple bandage-type structures attached to the patient with adhesive materials, providing a contact between the patient's skin and the sensor components. However, their flexible nature renders them susceptible to motion artifacts caused by mechanical deformation of the sensor. Additionally, the adhesives used to secure the bandage sensors are

generally designed for a single application, as they tend to lose adhesive strength when removed from the tissue for repositioning of the sensor. The sensor adhesives may also not adhere well to tissue that has blood or sweat on the surface.

[0009] Reusable sensors are often semi-rigid or rigid clip-type devices with three-dimensional geometry and moving parts. The clips generally affix the sensor components to a patient's tissue with spring-loaded hinges designed to hold the sensor in place after application. Clip-style pulse oximeter sensors are used repeatedly and, typically, on more than one patient. Therefore, over the life of the sensor, detritus and other bio-debris (sloughed off skin cells, dried fluids, dirt, and so forth) may accumulate on the surface of the sensor or in crevices and cavities of the sensor, after repeated uses. Thus, a thorough cleaning of a clip-style sensor may involve disassembly of the sensor and individual cleaning of the disassembled parts, or may involve careful cleaning using utensils capable of reaching into cavities or crevices of the sensor. Such cleaning is labor intensive and may be impractical in a typical hospital or clinic environment. Clip-style sensors with hinges or complex moving parts may also be more expensive to manufacture and transport. For example, a clip-style sensor with a complex structure and moving parts may require extra protection during shipping. Additionally, the complex structure of a clip-style sensor prevents easy stacking of multiple sensors in a single packaging system.

[0010] Although the clip-style sensor design provides a familiar and easy-to-use device for affixing the sensor components to a patient, the structure of the clip provides cleaning, manufacturing, and packaging challenges. It would be desirable to provide a clip-style pulse oximetry sensor that is easy to manufacture and use and that also provides suitable tissue contacting strength without complex mechanical components.

### SUMMARY

[0011] Certain aspects commensurate in scope with the originally claimed invention are set forth below. It should be understood that these aspects are presented merely to provide the reader with a brief summary of certain forms that the invention might take and that these aspects are not intended to limit the scope of the invention. Indeed, the invention may encompass a variety of aspects that may not be set forth below.

[0012] There is provided a sensor that includes: a sensor body comprising a material with shape memory, wherein the sensor body is adapted to assume a substantially curved configuration in the absence of a deforming force; and at least one sensing element disposed on the sensor body.

[0013] There is also provided a pulse oximetry system that includes: a pulse oximetry monitor; and a pulse oximetry sensor adapted to be operatively coupled to the monitor, the sensor including: a sensor body comprising a material with shape memory, wherein the sensor body is adapted to assume a substantially curved configuration in the absence of a deforming force; and at least one sensing element disposed on the sensor body.

[0014] There is also provided a sensor packaging system that includes: a protective package having an interior to hold

at least one sensor in its interior; and at least one sensor having at least one sensing element, whereby the sensor includes a material having shape memory and whereby the sensor is restrained in a substantially planar position. The sensor is adapted to be curved in the absence of a deforming force.

[0015] There is also provided a method for packaging a sensor that includes: providing a substantially curved sensor body comprising at least one sensing element and a material with shape memory; deforming the sensor body into a substantially flat position; restraining the sensor body in the substantially flat position with a removable restraining element; and packaging the sensor in a packaging container.

[0016] There is also provided a method of manufacturing a sensor that includes: providing a sensor body comprising a material with shape memory, wherein the sensor body is adapted to assume a substantially curved configuration in the absence of a deforming force; and providing at least one sensing element disposed on the sensor body.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0017] Advantages of the invention may become apparent upon reading the following detailed description and upon reference to the drawings in which:

[0018] FIG. 1A illustrates an embodiment of an exemplary clip-style pulse oximetry sensor with a flat spring in the memory configuration according to the present invention;

[0019] FIG. 1B illustrates the pulse oximetry sensor of FIG. 1A in the planar configuration due to a deforming stress;

[0020] FIG. 1C illustrates the pulse oximetry sensor of FIG. 1A applied to a patient earlobe;

[0021] FIG. 2 illustrates an embodiment of an exemplary pulse oximetry sensor in the memory configuration with a shape memory wire;

[0022] FIG. 3A illustrates a perspective view of an exemplary pulse oximetry sensor in the planar configuration with a breakable restraining element according to the present invention;

[0023] FIG. 3B illustrates the pulse oximetry sensor of FIG. 3A in the memory configuration after the restraining element has been broken;

[0024] FIG. 4 illustrates a perspective view of an exemplary pulse oximetry sensor with a sliding restraining element according to the present invention;

[0025] FIG. 5 illustrates a perspective view of an exemplary pulse oximetry sensor with an adhesive restraining element according to the present invention;

[0026] FIG. 6 illustrates a cross sectional view of an exemplary pulse oximetry sensor packaging system with multiple pulse oximetry sensors according to the present invention; and

[0027] FIG. 7 illustrates a pulse oximetry system coupled to a multi-parameter patient monitor and a sensor according to embodiments of the present invention.

#### DETAILED DESCRIPTION OF SPECIFIC EMBODIMENTS

[0028] One or more specific embodiments of the present invention will be described below. In an effort to provide a

concise description of these embodiments, not all features of an actual implementation are described in the specification. It should be appreciated that in the development of any such actual implementation, as in any engineering or design project, numerous implementation-specific decisions must be made to achieve the developers' specific goals, such as compliance with system-related and business-related constraints, which may vary from one implementation to another. Moreover, it should be appreciated that such a development effort might be complex and time consuming, but would nevertheless be a routine undertaking of design, fabrication, and manufacture for those of ordinary skill having the benefit of this disclosure.

[0029] The present techniques provide an improved medical sensor for pulse oximetry or other spectrophotometric uses. The sensor is constructed from a material with a shape memory of a curvature or a bend, such that the material will tend to return to its "memorized" shape if deformed therefrom. Thus, a sensor so constructed may have fewer parts, as the spring force of the sensor is provided by the shape memory material. Generally, such a sensor may provide certain advantages for storage or shipping. For example, when a sensor according to the present techniques is packaged for shipping, it may be flattened and restrained in a planar position that allows the sensors to be packaged efficiently for transport. Because the sensor is made of a material that has memory, when the restraints are removed from the sensor, the sensor will revert to a curved shape that provides sufficient spring force to affix the sensor to the patient.

[0030] Sensors for pulse oximetry or other spectrophotometric uses are typically placed on a patient in a location that is normally perfused with arterial blood to facilitate measurement of the desired blood characteristics, such as arterial oxygen saturation measurement (SpO<sub>2</sub>). Clip-style sensors are often used on patient digits, earlobes, or nose bridges. Such sensors rely on a spring force to hold the sensor in place.

[0031] For the exemplary sensors described below, the spring force is provided by a shape memory material. Materials which possess the characteristic of having shape memory are well known, and include certain metal alloys, plastics, and polymers. Any suitable shape-memory materials may be used, such as a nickel-titanium alloy (NiTi). One such NiTi alloy is manufactured, for example, by Shape Memory Applications, Inc., Santa Clara, Calif. A pulse oximetry sensor made of such materials can be moved between an original memory configuration to a deformed configuration, and the sensor 10 may revert to the original memory configuration under specified conditions. A sensor 10 constructed from a shape memory material may be converted from the memory configuration to a deformed configuration upon receiving a certain stimulus, such as temperature change, electrical stimulation, or mechanical force. The sensor 10 will be able to recover from the deformed configuration to resume the original memory configuration upon removal of the deforming stimulus. This tendency towards reversion to the memory configuration provides the spring force to affix the pulse oximetry sensor 10 to a patient.

[0032] In one such specific example, the sensor may be made from a shape memory material that may undergo a

phase transformation during application of a pure mechanical load. In general, metallic shape-memory alloys, such as NiTi, CuZnAl, and CuAlNi alloys, exhibit the property of solid-to-solid phase transitions. Specifically, shape-memory material is able to undergo a transformation from a solid austenite state to a solid martensite state. The austenite state generally exists at higher temperatures and is associated with more order among the atoms of the alloy, while the more atomically disordered martensite state exists at lower temperatures.

[0033] A shape memory is “fixed” in a shape memory material by holding the material in its desired memory shape while heating it to a temperature beyond the transformation temperature range that marks the phase change between the austenite state and the martensite state. For example, certain NiTi alloys are heated to approximately 500° C. to achieve a state in which a memory configuration can be fixed. In such a state, each titanium atom is surrounded by a cube of nickel atoms. When the material is cooled through a transformation temperature range after heating, the atoms adopt the more disordered martensite state. Transformation temperatures can vary widely depending on the composition of the alloy, and may range from -195° C. to 100° C.

[0034] Although shape memory materials can undergo temperature-induced shape recovery, they also may exhibit a pseudo-elastic shape recovery without a change in temperature under mechanical loads. As the transformation between austenite and martensite is an atomic rearrangement, mechanical loads may also trigger the atomic changes that lead to the solid-to-solid phase transformation. When the load is released the shape memory material in the martensite state begins to transform back to austenite. Generally, a sensor made from shape memory materials described herein experiences substantially complete shape recovery at temperatures associated with normal use, such as room temperatures in the range of 18° C.-25° C.

[0035] Clip-style pulse oximetry sensors that are constructed from materials with shape memory may take a variety of forms. For example, FIGS. 1A-C illustrate a sensor 10A adapted for use on a patient's earlobe. The sensor 10A has a flat spring 12 that is constructed at least in part from a shape memory material. The flat spring 12 is adapted to house an emitter 14 and a detector 16. One with skill in the art is aware that the emitter 14 and the detector 16 may include wires (not shown) or other electrical connections that allow the sensor 10A to communicate with a monitor, as discussed in more detail herein. The sensor 10A may be adapted to include grooves or channels for wires connected to the emitter 14 and the detector 16, such that the wires may be embedded in the sensor body. In other embodiments, wires connected to the emitter 14 and the detector 16 may run along the surface of the sensor body, either on a tissue-contacting surface or a surface that does not contact the tissue during use.

[0036] The sensor 10A shown in FIG. 1A is in its memory configuration 18 (e.g., its undeformed austenitic state). The flat spring 12 is shaped such that the radius of curvature of the flat spring 12 is sufficient to provide suitable spring force to attach the sensor 10A to a patient's earlobe. The flat spring 12 in its memory configuration 18 can be readily straightened by the application of manual force. When such force is applied to the flat spring 12, at least part of the austenitic

phase is converted to the martensitic phase so long as the force is maintained. FIG. 1B illustrates a perspective view of the planar configuration 20 of the sensor 10A after the application of a deforming force. As soon as the deforming force is removed, the sensor 10A then returns pseudoelastically to its memory configuration 18, with part of the martensitic phase converting back to the austenitic phase. As shown in FIG. 1C, the sensor recovers from the planar configuration 20 enough to provide suitable spring force to attach the sensor to the patient's earlobe 22.

[0037] It is contemplated that the radius of curvature of the sensor 10A in the memory configuration 18 may be adjusted to provide customized pressure to the patient's earlobe. In certain embodiments, the spring force that the flat spring 12 exerts on the earlobe provides sufficient pressure so that the pressure exceeds the typical venous pressure of a patient, but does not exceed the diastolic arterial pressure. As the pulse oximetry measurements are related to arterial blood oxygen saturation and pulsation, and not venous blood pulsation, reducing the effect of the venous component in the tissue may enhance the sensitivity of the sensor to variations in the arterial blood signal. Thus, the sensor 10A may apply a pressure greater than the venous pressure to squeeze excess pooled venous blood from the optically probed tissue. Yet, since the pressure applied by the sensor 10A is designed to be less than the arterial pressure, the application of pressure to the tissue does not interfere with the arterial pulse signal. Typical venous pressure, diastolic arterial pressure, and systolic arterial pressure are less than 10-35 mmHg, 80 mmHg, and 120 mmHg, respectively. Accordingly, in certain embodiments, the sensor may be adjusted to overcome an average venous pressure of 15-35 mmHg. However, venous pressures may vary because of the location of the vascular bed and the patient's condition. For example, low arterial diastolic blood pressure (about 30 mmHg) may occur in sick patients. In such embodiments, the sensor 10A removes most of the venous pooling with by applying sufficient pressure to overcome light to moderate venous pressure (about 15 mmHg).

[0038] In certain embodiments, it may be advantageous, e.g., for reasons related to expense or design, to use a limited amount of shape memory material. Hence, the shape memory material may be in a form in which it is reduced in bulk, such as the form of a strip, a mesh, a tube, a strap, or a wire. As one example, FIG. 2 illustrates a sensor 10B according to the present technique in which a shape memory strap 24 connects a first portion 26 and a second portion 28. The first portion 26 and the second portion 28 house an emitter 30 and a detector 32, which are disposed on the tissue-contacting sides 46 of the first portion 26 and the second portion 28, respectively. The first portion 26 and the second portion 28 may be constructed from any suitable rigid or semi-rigid material, such as rubber, metal, or plastic. In one embodiment (not shown) the first portion 26 and the second portion 28 may have foam pads (not shown) disposed on their tissue-contacting sides 46 to provide a more comfortable contact with the patient's skin. The sensor 10B as described above may be advantageous for application to the bridge of a patient's nose or a patient's earlobe. The shape memory strap 24 is sufficiently flexible to fit over a wide variety of sizes and shapes of nose bridges or earlobes, but has sufficient spring force due to its pseudoelastic properties to ensure a secure fit. Additionally, the shape memory strap 24 may be thin enough to fit comfortably over

the bridge of the nose without obscuring the patient's vision, particularly as the sensor 10B does not have protruding handles.

[0039] As discussed above, an advantage conferred by the present techniques is that a sensor 10 may be retained in a substantially planar configuration that allows for ease of storing and packaging. Although the package in which a sensor is placed may confer the mechanical force to retain the sensor in its deformed configuration, a sensor may include a component that performs this function instead. Turning to FIGS. 3A-B, an exemplary embodiment is depicted in which a sensor 10C includes such a restraining element. As shown in FIG. 3A, the restraining element 36 suitable to restrain the sensor 10C in a substantially flat configuration may be breakable or removable. For the former use, the restraining element 36 may be constructed from brittle ceramic or plastic. The breakable restraining element 36 may be adhesively or otherwise disposed in a region of the sensor 10C that exhibits the greatest amount of curvature when in the undeformed memory configuration. As depicted, the breakable restraining element 36 is disposed on the tissue-contacting side 38 of the sensor 10C in the interior of the curve, although it should be appreciated that the restraining element 36 may be disposed on the other side instead. The breakable restraining element 36 has sufficient strength to overcome the tendency of the sensor to revert to the undeformed memory configuration 40, as depicted in FIG. 3B. Nevertheless, the breakable restraining element 36 may also be sufficiently brittle such that it may be easily broken by hand by a healthcare worker prior to application of the sensor 10C. FIG. 3B shows the sensor 10C in the undeformed memory configuration 40 after breaking of the breakable restraining element 36. In other embodiments (not shown), the breakable restraining element 36 may be scored, which may allow it to be broken more easily by the user.

[0040] In other embodiments, it may be appropriate to employ a restraining element that does not break during the removal process and is, thus, reusable. FIG. 4 depicts a sensor 10D made from a shape memory material with a sleeve-like restraining element 42 with at least one opening 44 having a slot 45, sized to fit over a first end 46 or a second end 48 of the sensor 10D. The slot 45 is configured such that it fits the sensor 10D snugly near the edges of the sensor to prevent curvature of the memory material. The opening 44 is arranged to correspond with the emitter 49 and the detector 51, such that when the sleeve-like restraining element slides over the first end 46 or the second end 48, the opening allows the emitter 49 or the detector 51 to slide through. The sensor 10D is depicted in the planar configuration 50, and the memory configuration (not shown) is substantially U-shaped. The opening 44 is configured to allow easy removal, but is snug enough to prevent curving of the sensor 10D to partially revert to the U-shaped memory configuration. The sleeve-like restraining element 42 serves to hold the sensor 10D in the planar configuration 50 until the sleeve-like restraining element 42 is removed. The sleeve-like restraining element 42 may be removed by sliding it off the first end 46 or the second end 48 of the sensor 10D. The sleeve-like restraining element 42 may be made from any suitable material that serves to overcome the tendency of the sensor 10D to revert to the U-shaped memory configuration, such as metal or plastic. After the sensor 10D is removed from the patient, the sleeve-like

restraining element 42 can be reapplied to the sensor 10D. Thus, the sensor 10D can be returned to the planar configuration 50 for storage.

[0041] In other embodiments, it may be less costly to manufacture a sensor with a disposable adhesive restraining element. As one example, a sensor 10E with a peelable adhesive layer 52 that keeps the sensor in the substantially planar configuration 54 is illustrated in FIG. 5. The peelable adhesive layer 52 may be paper, plastic, polyester, woven fabric, or any other suitable material that serves to overcome the tendency of the sensor 10E to revert to its U-shaped memory configuration (not shown). The peelable adhesive layer 52 is coated with an adhesive on the sensor contacting side 56 and is disposed on the surface of the sensor 10E that does not contact the tissue during normal use. The peelable adhesive layer 52 may be removed by a healthcare worker prior to application of the sensor 10E to a patient.

[0042] In one embodiment (not shown), an adhesive material may be applied to the tissue-contacting side of the sensor 10E to facilitate securing the sensor to the patient. The use of an adhesive material improves the contact of the sensor to the patient and limits its susceptibility to motion artifacts. Because the sensor 10E is stored in a substantially planar configuration 54, the adhesive regions of the sensor 10E may be less likely to come into contact with one another than if the sensor 10E were in the U-shaped memory configuration.

[0043] The present techniques provide sensors that may be more efficiently packaged and shipped due to their generally planar configuration. Accordingly, FIG. 6 illustrates an exemplary packaging system 58 for storing and transporting a pulse oximetry sensor (generically identified here as a sensor 10) that includes at least one pulse oximetry sensor 10, a protective package 60, and restraining elements 62. The restraining elements 62 hold the respective sensors 10 in the planar configuration. The restraining element 62 may be attached to the sensor 10 as described above. For example, the restraining element may be any of the restraining elements described herein (e.g. breakable restraining element 36, sleeve-like restraining element 42, peelable adhesive layer 52). Alternatively, the restraining element may be incorporated into the packaging system 58. For example, the packaging system may include slots (not shown) that the sensors 10 may slide into and that restrain the sensors 10 in the planar configuration. When the sensors 10 are removed, they will revert to a U-shaped configuration. As shown, the packaging system 58 may include multiple stacked sensors 10 in the interior 64 of the protective package 60. Thin protective sheets 66 may separate the stacked sensors 10. The thin protective sheets 66 may be a relatively rigid material, such as plastic, that may provide the straightening force to the sensors 10. The planar configuration of the sensors 10 allows more convenient stacking as compared to a typical U-shaped clip-style sensor. The stacked sensors 10 in the planar configuration also occupy less space, and thus a larger number of sensors may be packaged in a packaging system relative to U-shaped sensors. Additionally, since the sensors 10 have no moving parts, the amount of protective packaging used for shipping may be minimal.

[0044] It should be understood that the sensors discussed above may be used in conjunction with a pulse oximetry monitor 68, as illustrated in FIG. 7. It should be appreciated

that the cable **70** of the sensor **10** may be coupled to the monitor **68** or it may be coupled to a transmission device (not shown) to facilitate wireless transmission between the sensor **10** and the monitor **68**. The monitor **68** may be any suitable pulse oximeter, such as those available from Nellcor Puritan Bennett Inc. Furthermore, to upgrade conventional pulse oximetry provided by the monitor **68** to provide additional functions, the monitor **68** may be coupled to a multi-parameter patient monitor **72** via a cable **74** connected to a sensor input port or via a cable **76** connected to a digital communication port.

[0045] It should also be understood that the sensors described herein include an emitter and a detector that may be of any suitable type. For example, the emitter may be one or more light emitting diodes adapted to transmit one or more wavelengths of light in the red to infrared range, and the detector may be a photodetector selected to receive light in the range or ranges emitted from the emitter. The emitter and the detector may be disposed on the sensor body, which may incorporate a shape memory material and that may be combined with any other suitable material, such as plastic, rubber, silicone, foam, woven material, or paper. Alternatively, the emitter and the detector may be remotely located and optically coupled to the sensor **10** using optical fibers. Although not shown in the embodiments discussed above, the sensors are typically coupled to a cable **70** that is responsible for transmitting electrical and/or optical signals to and from the emitter and detector of the sensor **10**. The cable **70** may be permanently coupled to the sensor **10**, or it may be removably coupled to the sensor **10**—the latter alternative being more useful and cost efficient in situations where the sensor **10** is disposable.

[0046] The sensor **10** may be a “transmission type” sensor. Transmission type sensors include an emitter and detector that are typically placed on opposing sides of the sensor site. If the sensor site is a fingertip, for example, the sensor **10** is positioned over the patient’s fingertip such that the emitter and detector lie on either side of the patient’s nail bed. In other words, the sensor **10** is positioned so that the emitter is located on the patient’s fingernail and the detector is located 180° opposite the emitter on the patient’s finger pad. During operation, the emitter shines one or more wavelengths of light through the patient’s fingertip and the light received by the detector is processed to determine various physiological characteristics of the patient. In each of the embodiments discussed herein, it should be understood that the locations of the emitter and the detector may be exchanged. For example, the detector may be located at the top of the finger and the emitter may be located underneath the finger. In either arrangement, the sensor **10** will perform in substantially the same manner.

[0047] Although the embodiments described herein generally referred to transmission type sensors, it should be understood that the sensor **10** may be a reflectance type sensor. Reflectance type sensors generally operate under the same general principles as transmittance type sensors. However, reflectance type sensors include an emitter and detector that are typically placed on the same side of the sensor site. For example, a reflectance type sensor may be placed on a patient’s fingertip, nose bridge, or earlobe such that the emitter and detector lie side-by-side. Reflectance type sensors detect light photons that are scattered back to the detector.

[0048] For pulse oximetry applications using either transmission or reflectance type sensors, the oxygen saturation of the patient’s arterial blood may be determined using two or more wavelengths of light, most commonly red and near infrared wavelengths. Similarly, in other applications a tissue water fraction (or other body fluid related metric) or a concentration of one or more biochemical components in an aqueous environment may be measured using two or more wavelengths of light, most commonly near infrared wavelengths between about 1,000 nm to about 2,500 nm. It should be understood that, as used herein, the term “light” may refer to one or more of infrared, visible, ultraviolet, or even X-ray electromagnetic radiation, and may also include any wavelength within the infrared, visible, ultraviolet, or X-ray spectra.

[0049] While the invention may be susceptible to various modifications and alternative forms, specific embodiments have been shown by way of example in the drawings and have been described in detail herein. However, it should be understood that the invention is not intended to be limited to the particular forms disclosed. Indeed, the present techniques may not only be applied to measurements of blood oxygen saturation, but these techniques may also be utilized for the measurement and/or analysis of other blood constituents using principles of pulse oximetry. Rather, the invention is to cover all modifications, equivalents, and alternatives falling within the spirit and scope of the invention as defined by the following appended claims.

What is claimed is:

1. A sensor adapted to be applied to a patient’s tissue comprising:

a sensor body comprising a material with shape memory, wherein the sensor body is adapted to assume a substantially curved configuration in the absence of a deforming force; and

at least one sensing element disposed on the sensor body.

2. The sensor, as set forth in claim 1, wherein the sensor comprises at least one of a pulse oximetry sensor or a sensor for measuring a water fraction, or a combination thereof.

3. The sensor, as set forth in claim 1, wherein the at least one sensing element comprises an emitter and a detector.

4. The sensor, as set forth in claim 3, wherein the emitter comprises at least one light emitting diode and wherein the detector comprises at least one photodetector.

5. The sensor, as set forth in claim 1, comprising a restraining element adapted to hold the sensor body in a substantially planar configuration.

6. The sensor, as set forth in claim 5, wherein the restraining element comprises a breakable component.

7. The sensor, as set forth in claim 5, wherein the restraining element comprises a peelable adhesive layer disposed on the sensor body.

8. The sensor, as set forth in claim 5, wherein the restraining element comprises a hollow sleeve adapted to slide over at least one end of the sensor.

9. The sensor, as set forth in claim 1, wherein the material with shape memory is configured to form a flat spring.

10. The sensor, as set forth in claim 1, wherein the material with shape memory is configured to form a strap.

11. The sensor, as set forth in claim 1, comprising an adhesive material disposed on a tissue-contacting surface of the sensor.

12. The sensor, as set forth in claim 1, wherein the sensor is adapted to be used on a finger, toe, ear, or nose.

13. The sensor, as set forth in claim 1, wherein the sensor is adapted to apply a spring force to a patient's tissue adapted to overcome a blood pressure of about 35 mm Hg or less.

14. The sensor, as set forth in claim 1, wherein the sensor is adapted to apply a spring force to a patient's tissue adapted to overcome a blood pressure of about 15 mm Hg or less.

15. A pulse oximetry system comprising:

a pulse oximetry monitor; and

a pulse oximetry sensor adapted to be operatively coupled to the monitor, the sensor comprising:

a sensor body comprising a material with shape memory, wherein the sensor body is adapted to assume a substantially curved configuration in the absence of a deforming force; and

at least one sensing element disposed on the sensor body.

16. The pulse oximetry system, as set forth in claim 15, wherein the sensor comprises a sensor for measuring a water fraction.

17. The pulse oximetry system, as set forth in claim 15, wherein the at least one sensing element comprises an emitter and a detector.

18. The pulse oximetry system, as set forth in claim 17, wherein the emitter comprises at least one light emitting diode and wherein the detector comprises at least one photodetector.

19. The pulse oximetry system, as set forth in claim 15, comprising a restraining element adapted to hold the sensor body in a substantially planar configuration.

20. The pulse oximetry system, as set forth in claim 19, wherein the restraining element comprises a breakable component.

21. The pulse oximetry system, as set forth in claim 19, wherein the restraining element comprises a peelable adhesive layer disposed on the sensor body.

22. The pulse oximetry system, as set forth in claim 19, wherein the restraining element comprises a hollow sleeve adapted to slide over at least one end of the sensor.

23. The pulse oximetry system, as set forth in claim 15, wherein the material with shape memory is configured to form a flat spring.

24. The pulse oximetry system, as set forth in claim 15, wherein the material with shape memory is configured to form a strap.

25. The pulse oximetry system, as set forth in claim 15, comprising an adhesive material disposed on a tissue-contacting surface of the sensor.

26. The pulse oximetry system, as set forth in claim 15, wherein the sensor is adapted to be used on a finger, toe, ear, or nose.

27. The pulse oximetry system, as set forth in claim 15, wherein the sensor is adapted to apply a spring force to a patient's tissue adapted to overcome a blood pressure of about 35 mm Hg or less.

28. The pulse oximetry system, as set forth in claim 15, wherein the sensor is adapted to apply a spring force to a patient's tissue adapted to overcome a blood pressure of about 15 mm Hg or less.

29. A sensor packaging system comprising:

a protective package having an interior to hold at least one sensor in the substantially planar position in the interior of the protective package; and

at least one sensor, the sensor comprising:

at least one sensing element; and

a material having shape memory, wherein the sensor is adapted to be curved in the absence of a deforming force, and wherein the sensor is restrained in a substantially planar position.

30. The packaging system, as set forth in claim 29, wherein the sensor comprises at least one of a pulse oximetry sensor or a sensor for measuring a water fraction.

31. The packaging system, as set forth in claim 29, wherein the sensing element comprises an emitter and a detector.

32. The packaging system, as set forth in claim 31, wherein the emitter comprises a light-emitting diode and the detector comprises at least one photodetector.

33. The packaging system, as set forth in claim 29, wherein the sensor is restrained with a breakable component disposed on the sensor body.

34. The packaging system, as set forth in claim 29, wherein the sensor is restrained with a peelable adhesive layer disposed on the sensor body.

35. The packaging system, as set forth in claim 29, wherein the sensor is restrained with a hollow sleeve adapted to slide over at least one end of the sensor.

36. The packaging system, as set forth in claim 29, wherein the sensor is restrained by a restraining element disposed on the protective package.

37. The packaging system, as set forth in claim 29, wherein the material with shape memory is configured to form a flat spring.

38. The packaging system, as set forth in claim 29, wherein the material with shape memory is configured to form a strap.

39. The packaging system, as set forth in claim 29, wherein the sensor comprises an adhesive material disposed on a tissue-contacting surface of the sensor.

40. A method for packaging a sensor comprising:

providing a substantially curved sensor body comprising a material with shape memory;

deforming the sensor body into a substantially flat position;

restraining the sensor body in the substantially flat position; and

packaging the sensor in a packaging container.

41. The method, as set forth in claim 40, wherein restraining the sensor comprises using a restraining element disposed on the sensor body.

42. The method, as set forth in claim 41, wherein the restraining element comprises a peelable adhesive layer, a hollow sleeve, or a breakable component.

43. The method, as set forth in claim 40, wherein restraining the sensor comprises using a restraining element disposed on packaging container.

44. The method, as set forth in claim 40, wherein the sensor comprises an adhesive material disposed on a tissue-contacting surface of the sensor.

- 45.** A method of manufacturing a sensor, comprising:  
providing a sensor body comprising a material with shape memory, wherein the sensor body is adapted to assume a substantially curved configuration in the absence of a deforming force; and  
providing at least one sensing element disposed on the sensor body.
- 46.** The method, as set forth in claim 45, wherein the material with shape memory is configured to form a flat spring.
- 47.** The method, as set forth in claim 45, wherein the material with shape memory is configured to form a strap.
- 48.** The method, as set forth in claim 45, wherein the sensing element comprises an emitter and a detector.
- 49.** The method, as set forth in claim 45, comprising:  
providing a restraining element adapted to hold the sensor body in a substantially planar configuration.
- 50.** The method, as set forth in claim 49, wherein the restraining element comprises a breakable component disposed on the sensor body.
- 51.** The method, as set forth in claim 49, wherein the restraining element comprises a peelable adhesive layer disposed on the sensor body.
- 52.** The method, as set forth in claim 49, wherein the restraining element comprises a hollow sleeve adapted to slide over at least one end of the sensor.
- 53.** The method, as set forth in claim 45, comprising:  
providing an adhesive material disposed on a tissue-contacting surface of sensor body.
- \* \* \* \* \*

专利名称(译)	医疗传感器及其使用技术		
公开(公告)号	<a href="#">US20070260130A1</a>	公开(公告)日	2007-11-08
申请号	US11/415711	申请日	2006-05-02
[标]申请(专利权)人(译)	CHIN RODNEY P		
申请(专利权)人(译)	CHIN RODNEY P		
当前申请(专利权)人(译)	CHIN RODNEY P		
[标]发明人	CHIN RODNEY P		
发明人	CHIN, RODNEY P.		
IPC分类号	A61B5/00		
CPC分类号	A61B5/14552 A61B5/6816 A61B5/6838 A61B5/6826 A61B5/6819		
其他公开文献	US7522948		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

夹式传感器可以由具有形状记忆的材料构成。提供了一种夹式传感器，其能够被压平以便简化运输和存储。传感器可以通过运输限制器保持平坦。这种传感器能够从平坦状态恢复并恢复弯曲形状。

