



US006999809B2

(12) **United States Patent**
Currier et al.

(10) **Patent No.:** **US 6,999,809 B2**
(45) **Date of Patent:** **Feb. 14, 2006**

(54) **CENTRAL VENOUS CATHETER HAVING A
SOFT TIP AND FIBER OPTICS**

FOREIGN PATENT DOCUMENTS

EP 0 336 984 B1 4/1988

(75) Inventors: **Clifford Currier**, Aliso Viejo, CA (US); **Michael Higgins**, Huntington Beach, CA (US); **Mark Gordon**, Corona Del Mar, CA (US); **Stacy Faught**, Aliso Viejo, CA (US); **Dean West**, Mission Viejo, CA (US)

(Continued)

Primary Examiner—Eric F. Winakur

(74) *Attorney, Agent, or Firm*—Edward Lifesciences

(73) Assignee: **Edwards Lifesciences Corporation**, Irvine, CA (US)

(57) **ABSTRACT**

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 213 days.

A multiple lumen catheter having a soft, tapered multiple lumen distal tip for insertion into a body vessel. One of the lumens is sized to pass over a guidewire such that the catheter can be inserted into the body vessel using the Seldinger technique. At least one medical implement lumen is used for placement or positioning of a biomedical sensor or other medical implement. For example, at least one optical fiber passing through the medical implement lumen may transmit and receive light at the distal tip for measuring oxygen saturation of the blood. The catheter may have a cylindrical catheter body to which the soft distal tip attaches. The soft tip reduces the possibility of vessel or tissue puncture and abrasion. The tip is constructed of a soft plastic or pliable material that yields easily when force is applied. For example, the tip may be made of a softer material than the catheter body, or if made of the same material, the tip can be configured with thinner walls or a higher air-to-material ratio cross-section. Various geometrical configurations and combinations of materials can be used to decrease the resistance of the tip to an applied load. One particular useful application for the catheter of the present invention is as a central venous catheter equipped with fibers for measuring oximetry. The fibers extend to the distal end of the tip and are preferably secured therein with minimal adhesive so as to limit the stiffness added to the tip. One particular useful construction is to secure the fibers within the medical implement lumen using adhesive only along a length of between about 0.5–3.5 mm.

(21) Appl. No.: **10/196,101**

(22) Filed: **Jul. 16, 2002**

(65) **Prior Publication Data**

US 2004/0015061 A1 Jan. 22, 2004

(51) **Int. Cl.**

A61B 5/00 (2006.01)

A61M 25/00 (2006.01)

A61N 1/04 (2006.01)

(52) **U.S. Cl.** **600/342**; 600/435; 600/361; 600/381; 604/508; 604/523; 607/122

(58) **Field of Classification Search** 600/309–310, 600/325, 327, 433–435, 466, 585, 361, 381, 600/342; 604/508, 523, 544, 528; 607/122
See application file for complete search history.


(56) **References Cited**

U.S. PATENT DOCUMENTS

3,434,775 A 3/1969 Gosselin
3,807,390 A 4/1974 Ostrowski et al.
3,847,483 A 11/1974 Shaw
4,487,475 A 12/1984 Ogawa

(Continued)

39 Claims, 11 Drawing Sheets

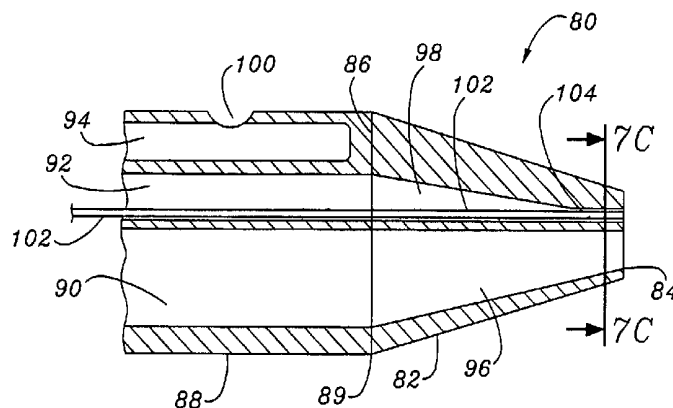

U.S. PATENT DOCUMENTS

4,647,149 A 3/1987 McCartney
 4,648,892 A 3/1987 Kittrell
 4,695,276 A * 9/1987 Shinno et al. 604/533
 4,718,423 A 1/1988 Willis et al.
 4,759,378 A 7/1988 Swendson et al.
 4,776,340 A 10/1988 Moran et al.
 4,788,967 A 12/1988 Ueda
 4,790,295 A 12/1988 Tashiro
 4,795,434 A 1/1989 Kujawski
 4,796,604 A 1/1989 Kawashima
 4,813,400 A 3/1989 Washizuka et al.
 4,830,013 A 5/1989 Maxwell
 4,871,229 A 10/1989 Tashiro
 4,911,148 A * 3/1990 Sosnowski et al. 600/136
 5,047,627 A 9/1991 Yim
 5,048,524 A 9/1991 Bailey
 5,263,928 A 11/1993 Manourchehr
 5,263,952 A 11/1993 Grace et al.
 5,280,786 A 1/1994 Wlodarczyk
 5,315,995 A 5/1994 Rivers
 5,443,057 A 8/1995 Elmore
 5,456,680 A 10/1995 Taylor et al.
 5,466,234 A * 11/1995 Loeb et al. 606/15
 5,470,330 A 11/1995 Goldenberg et al.
 5,542,924 A * 8/1996 Snoke et al. 604/264
 5,601,087 A 2/1997 Gunderson

5,665,051 A 9/1997 Quick et al.
 5,673,694 A 10/1997 Rivers
 5,702,368 A * 12/1997 Stevens et al. 604/171
 5,788,647 A 8/1998 Eggers
 5,807,261 A 9/1998 Benaron
 5,902,247 A 5/1999 Coe
 5,995,208 A 11/1999 Sarge
 6,033,398 A * 3/2000 Farley et al. 606/27
 6,196,966 B1 * 3/2001 Kerin et al. 600/114
 6,210,362 B1 * 4/2001 Ponzi 604/95.01
 6,251,128 B1 * 6/2001 Knopp et al. 607/100
 6,352,531 B1 3/2002 O'Connor et al.
 6,374,476 B1 * 4/2002 Ponzi et al. 29/527.1
 6,520,934 B1 * 2/2003 Lee et al. 604/103.1

FOREIGN PATENT DOCUMENTS

EP 0 336 985 B1 4/1988
 EP 0 311 458 A 4/1989
 EP 338149 A1 10/1989
 EP 0 514 913 A 11/1992
 EP 0 571 184 A2 5/1993
 EP 0 575 732 B1 5/1993
 GB 2210560 A 10/1987
 WO WO 97/06726 A1 2/1997
 WO WO 97/13452 A1 4/1997

* cited by examiner

Fig. 1A

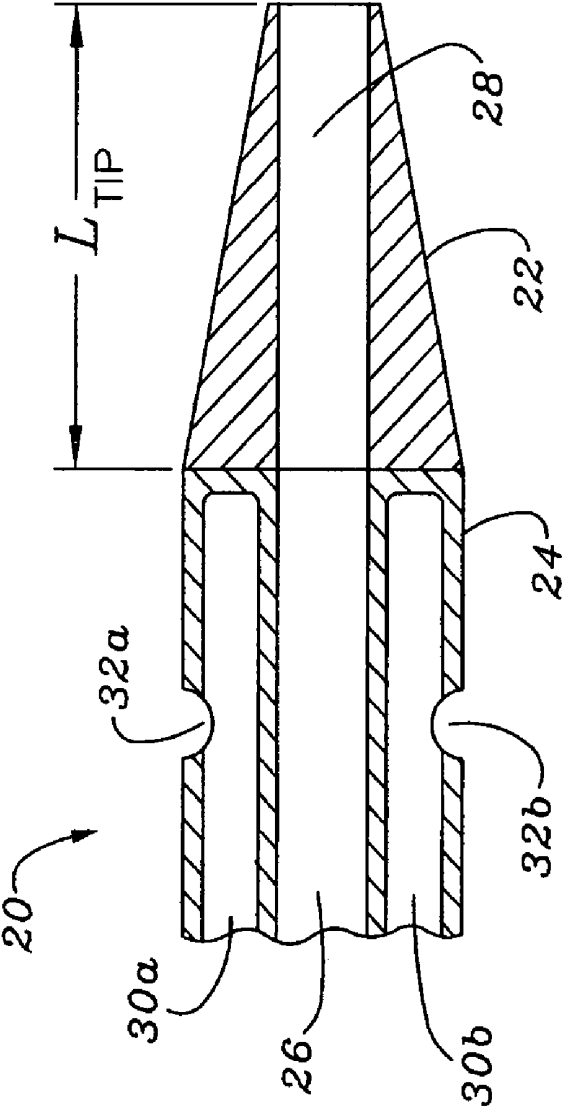
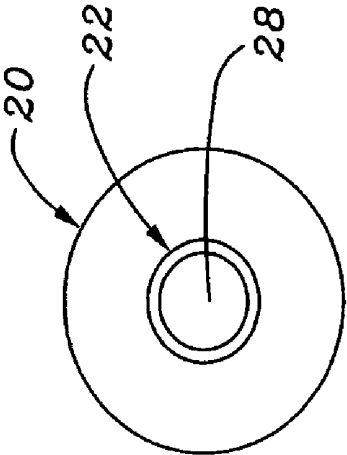


Fig. 1B



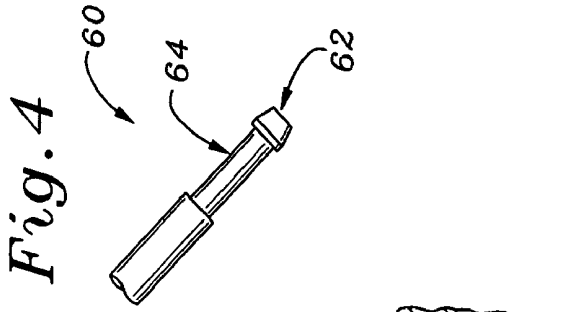


Fig. 2A

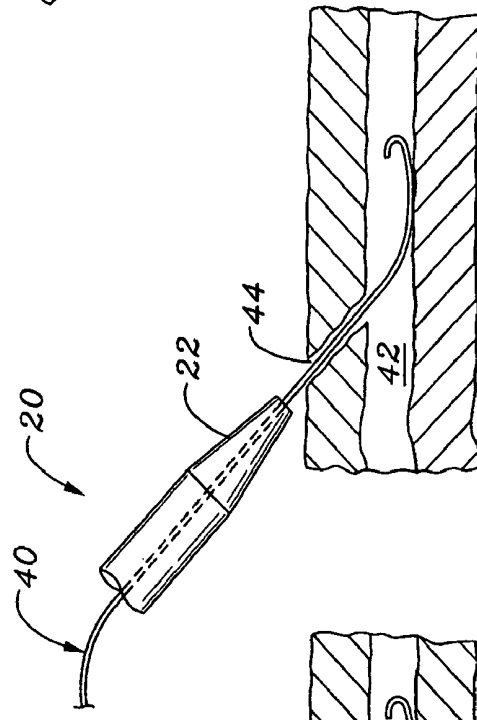


Fig. 3A

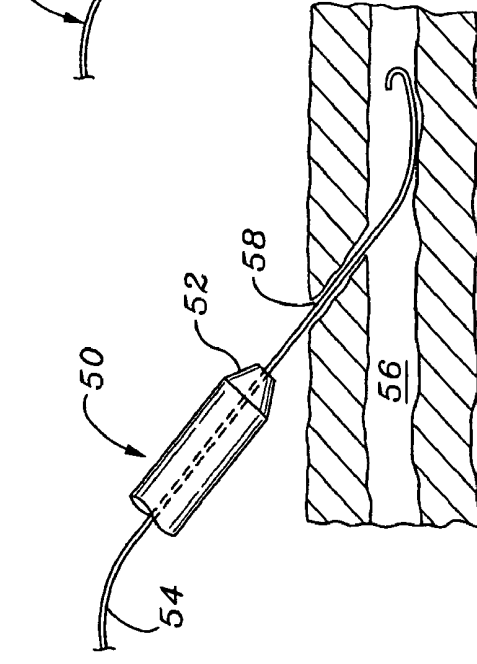


Fig. 2B

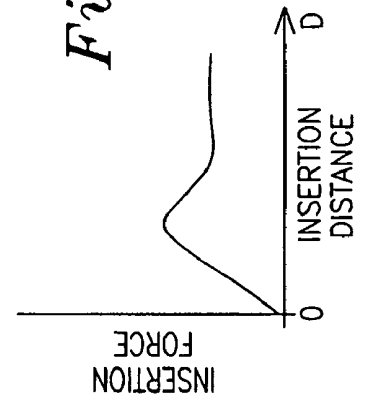


Fig. 3B

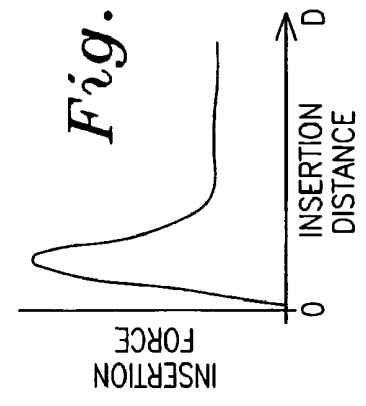


Fig. 5A

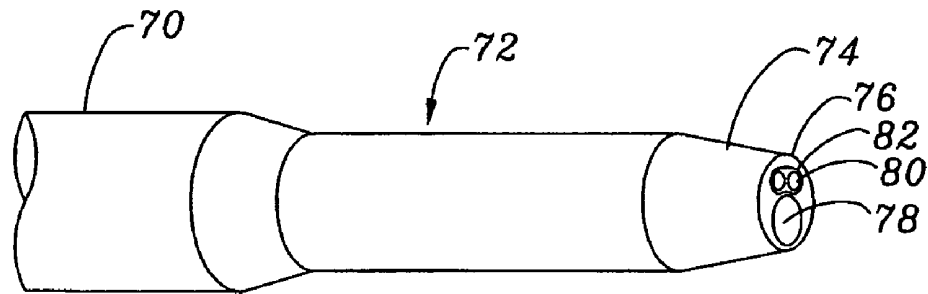


Fig. 5B

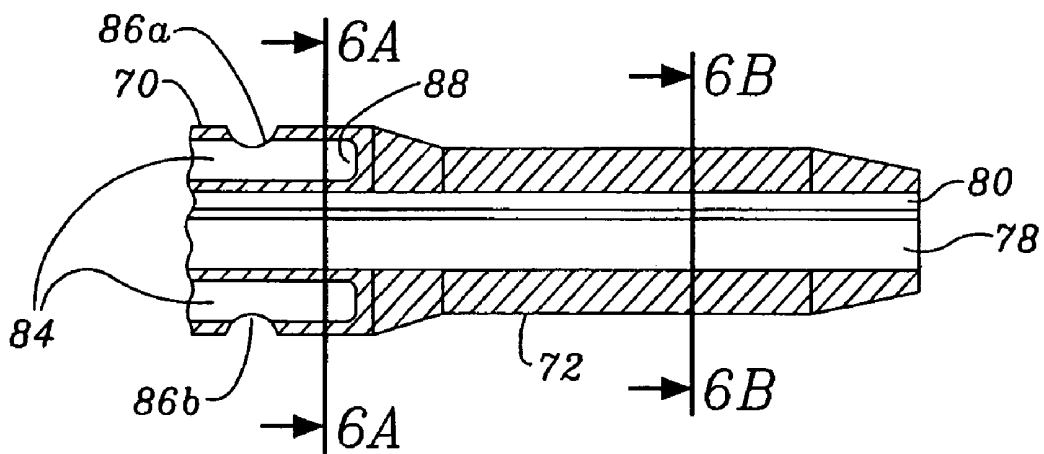


Fig. 6A

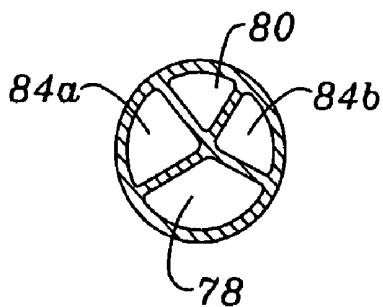


Fig. 6B




Fig. 7A

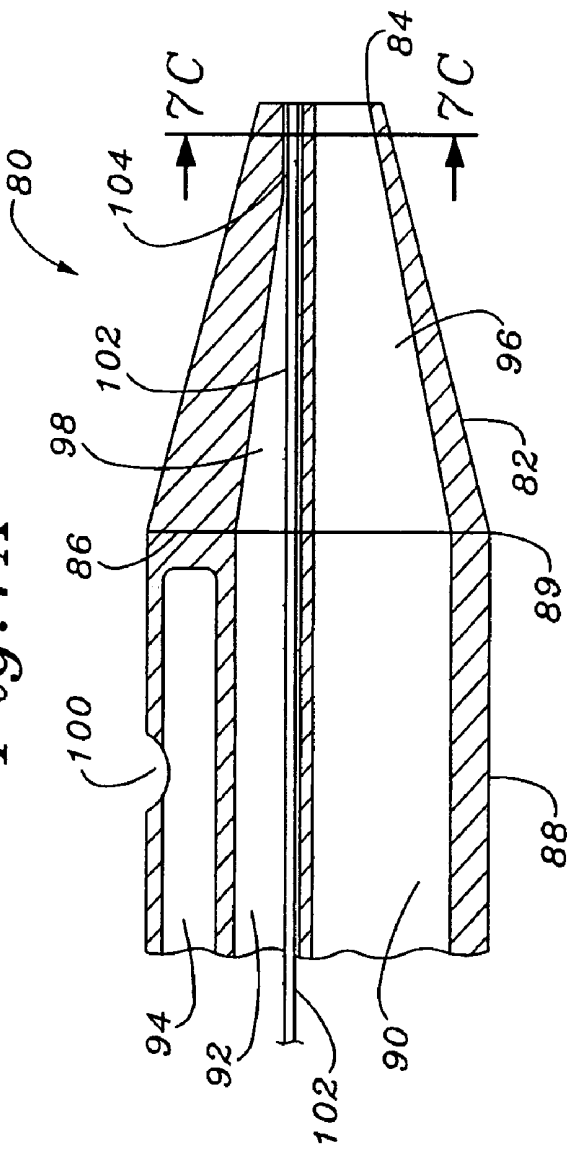


Fig. 7B

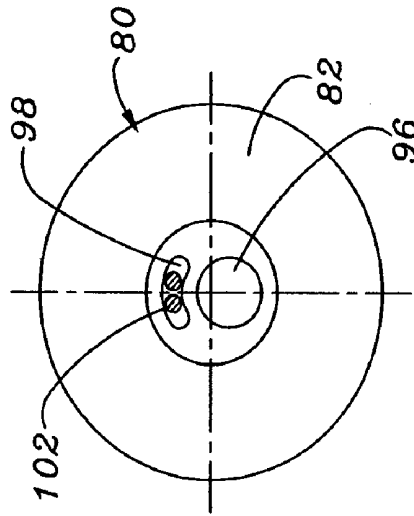


Fig. 7C

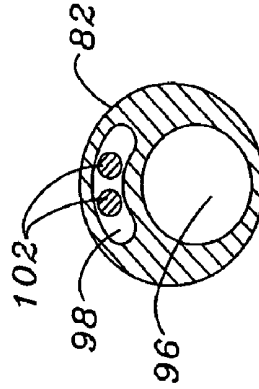


Fig. 8B

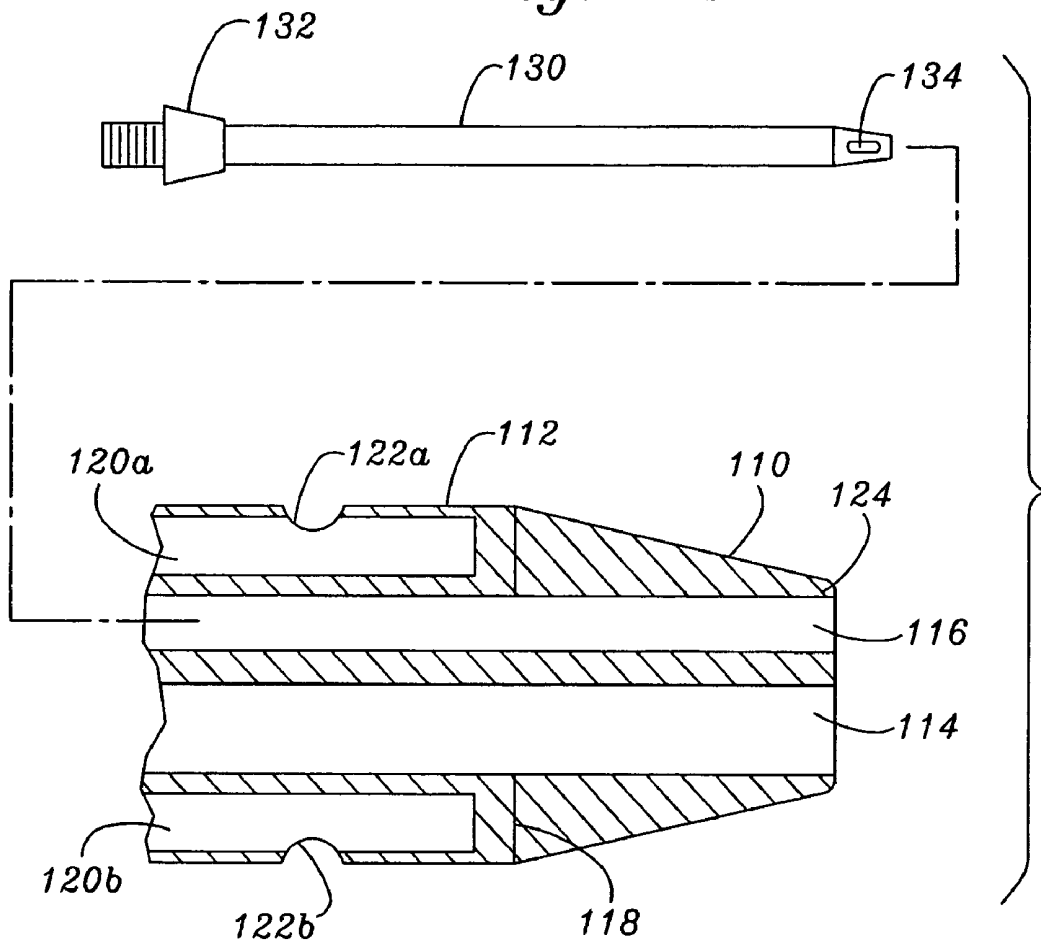
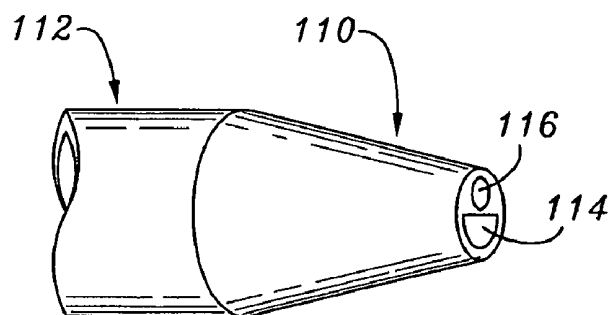


Fig. 8A



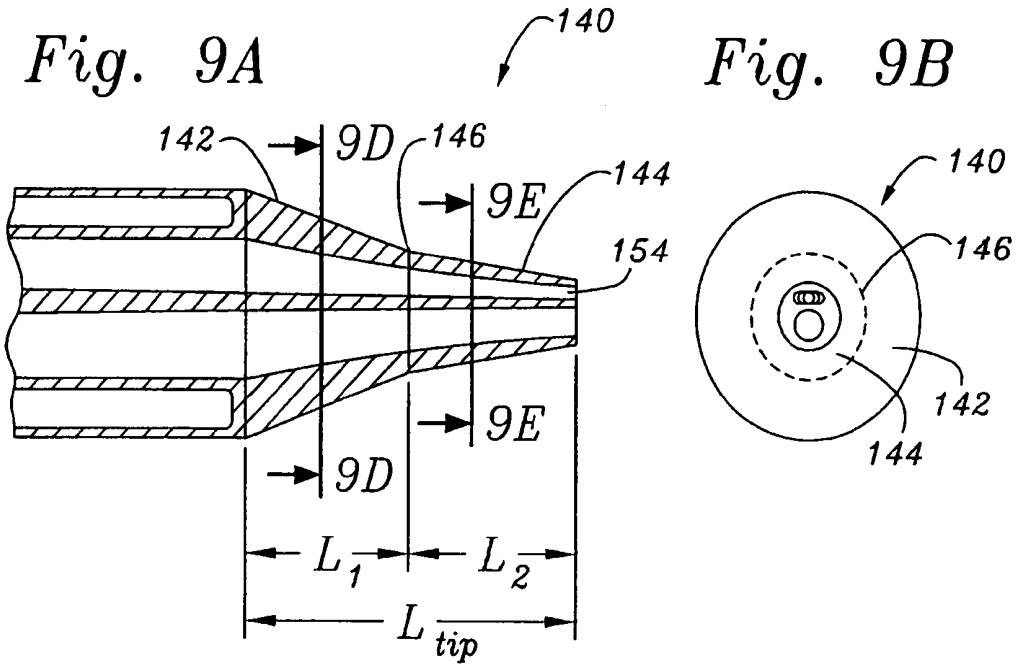


Fig. 9C

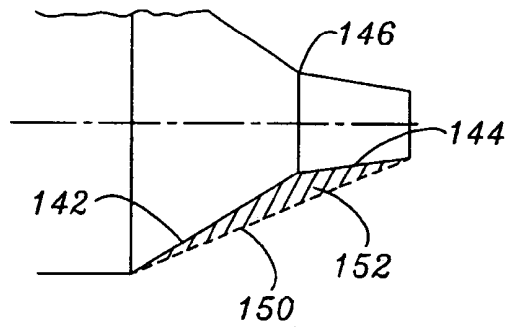


Fig. 9D


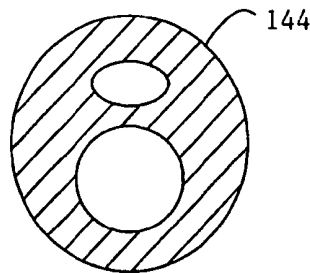


Fig. 9E



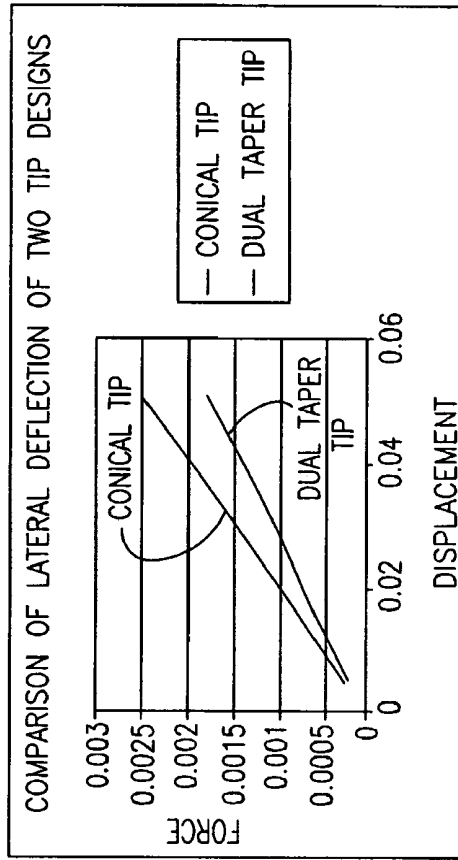
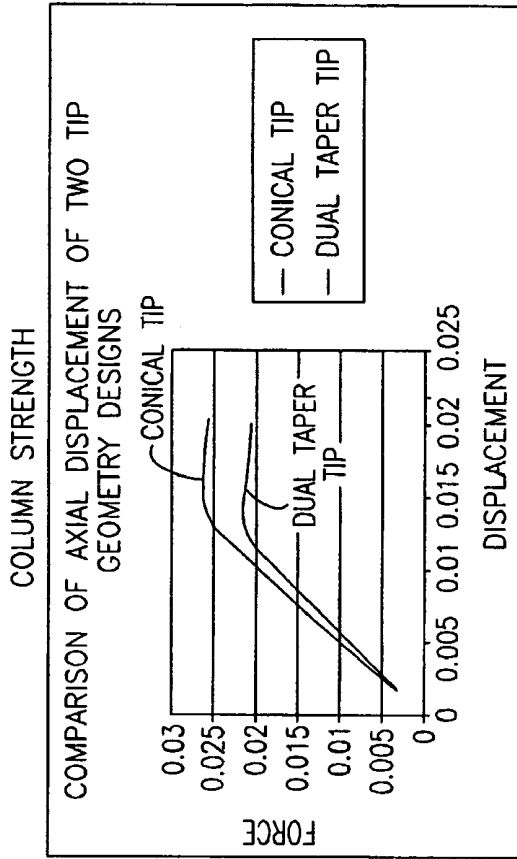


Fig. 10A

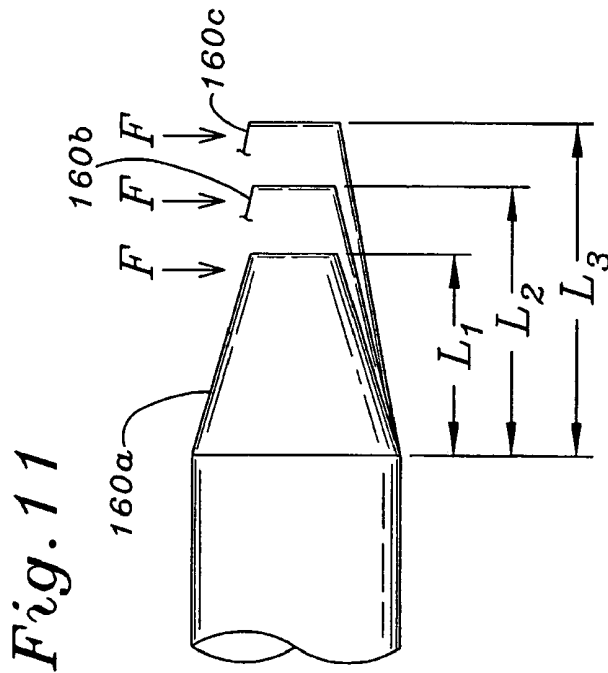


Fig. 11

Fig. 10B

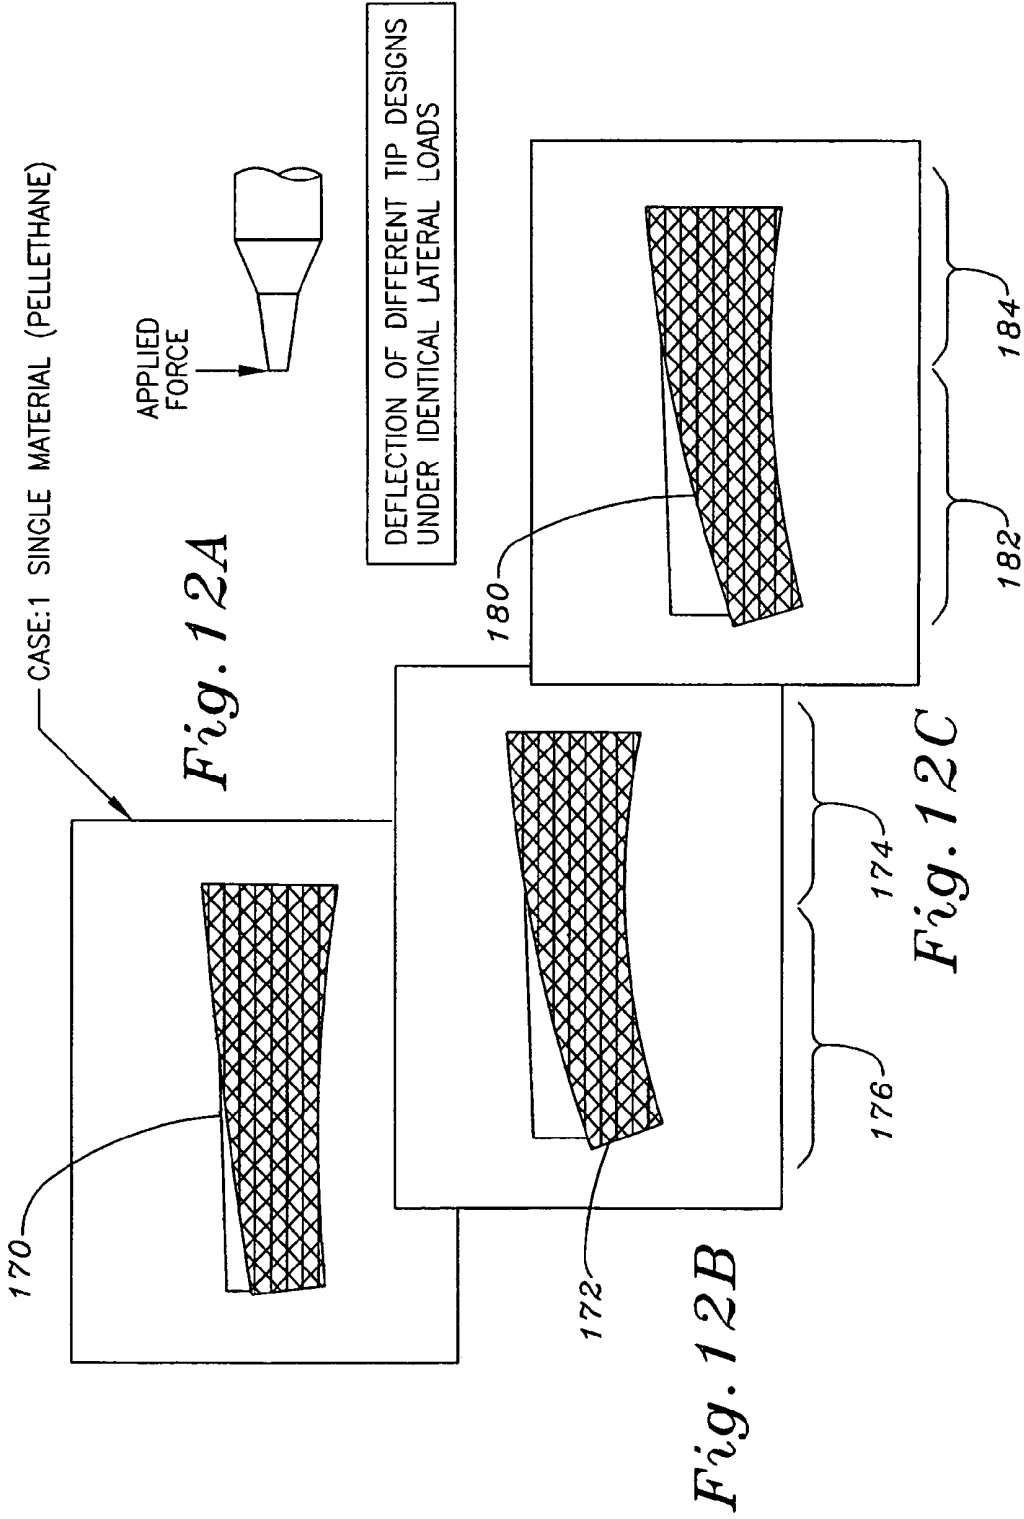


Fig. 13A

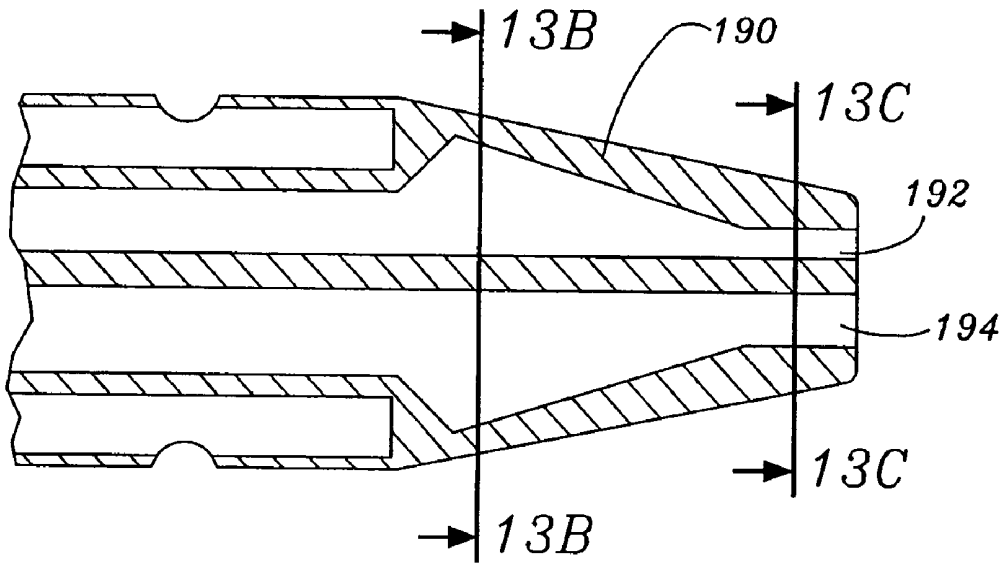


Fig. 13B

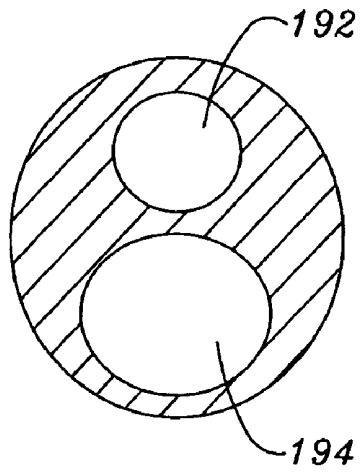


Fig. 13C

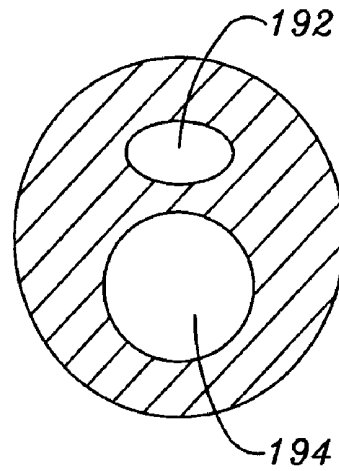


Fig. 14A


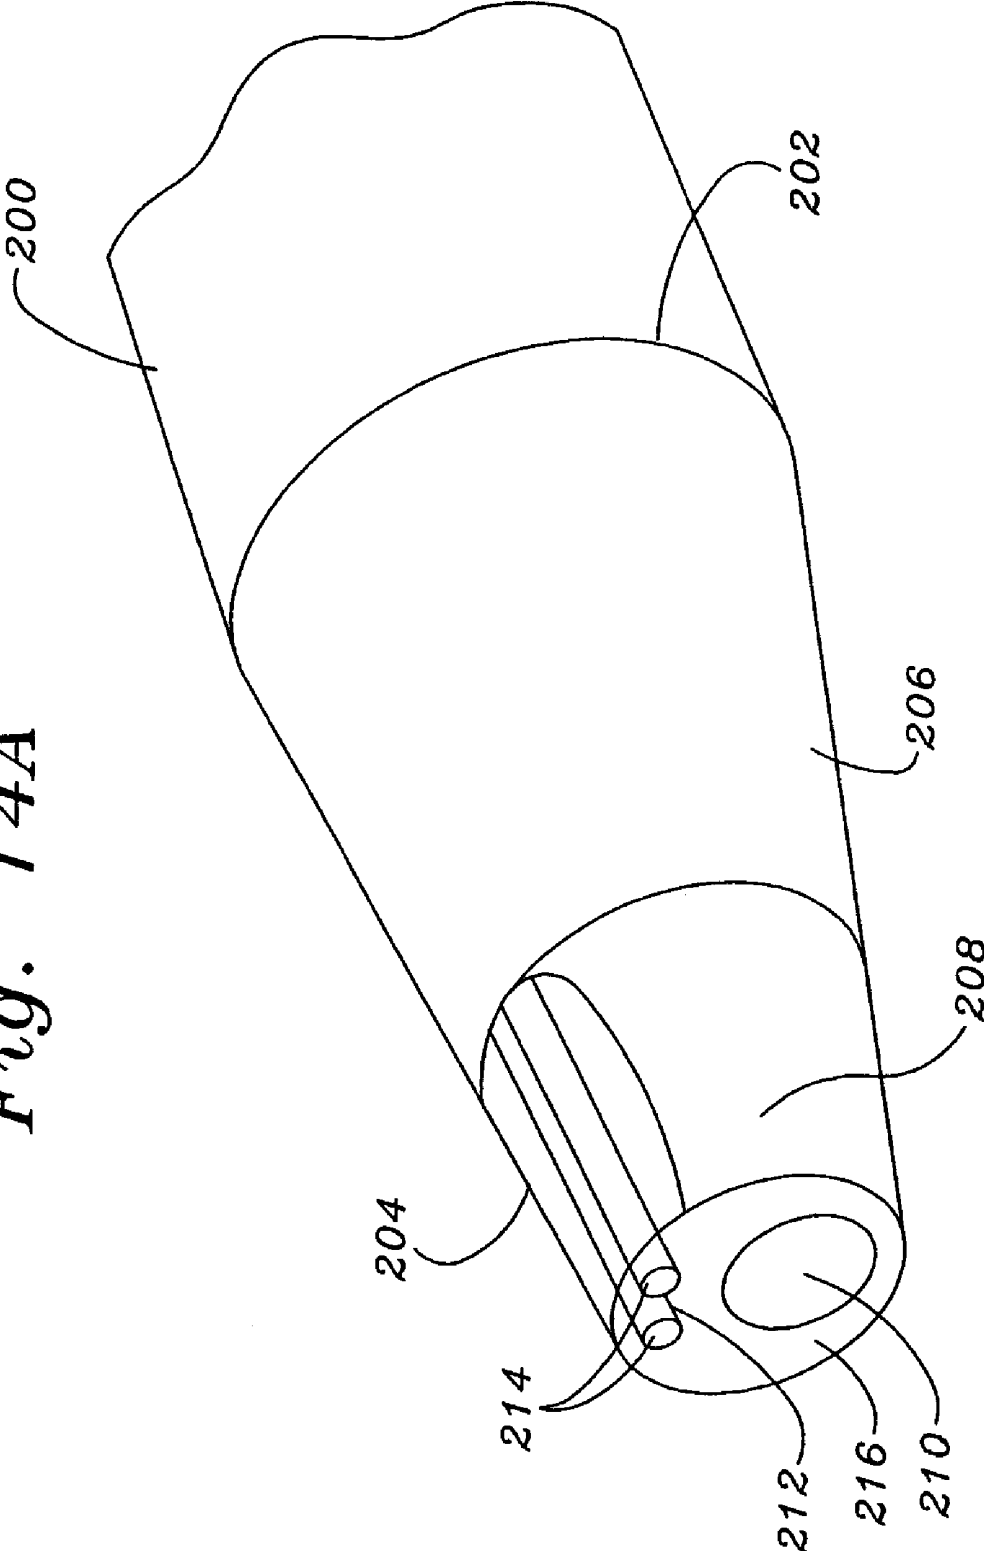


Fig. 14B

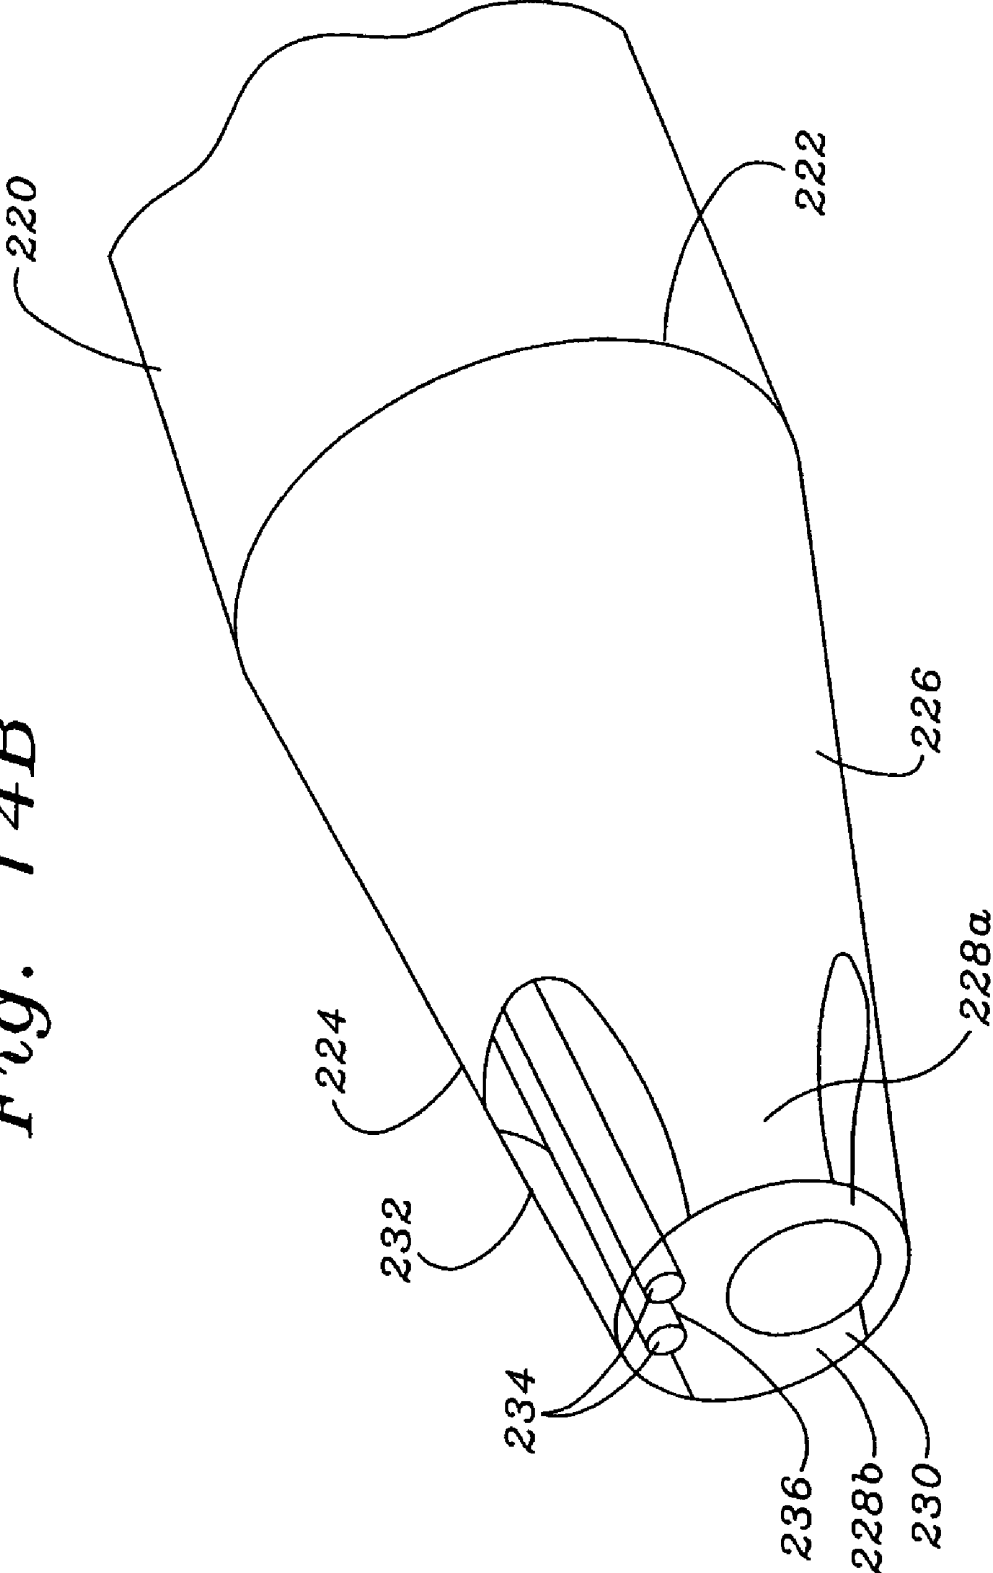

CENTRAL VENOUS CATHETER HAVING A SOFT TIP AND FIBER OPTICS

BACKGROUND OF THE INVENTION

The present invention relates generally to medical devices and, more particularly, to a central venous catheter having a multilumen soft tip whose flexibility is not compromised when a medical implement is located in one of the lumens of the soft tip during the use of the catheter. Even more specifically, the above-mentioned medical implement is fiber optics for measuring oxygen saturation of blood.

Central venous (CV) catheters are used primarily to gain access to the venous vasculature for fluid infusion, blood sampling and central venous pressure monitoring. CV catheters are inserted into the patient using the Seldinger technique. This involves identifying the target vein, puncturing the vein and inserting a guidewire. A vessel dilator is inserted over the guidewire and pushed through the vessel wall to create an opening for the CV catheter. The dilator is removed though the guidewire remains in place. The single lumen CV catheter is then threaded over the guidewire and pushed through the tissue and into the vessel. Importantly, the catheter is inserted without any stiffening members other than the guidewire. The tissue and vessel wall resist the catheter as it slides into the vessel. Therefore, to insure the catheter can easily slide into the body, the catheter body and catheter tip must be sufficiently rigid to slide over the guidewire into the blood vessel without buckling or otherwise collapsing. More than one lumen in the distal tip creates an asymmetry in the transverse cross-section and increases the chances of buckling. Therefore, CV catheters are uniformly constructed with a single lumen at the distal tip. Of course, any catheters that require such a soft tip are at present single lumen, not just CV catheters.

Once a CV catheter is placed into the blood vessel, then the stiffness that was desirable during insertion through the vessel wall becomes a disadvantage. Vessel perforation is always a concern in the design of these catheters. Another concern is that the catheter tip migrates from the central vena cava to the right atrium. The right atrium contains regions of thick and thin walls. During routine monitoring, if catheter has migrated into the right atrium, through the action of normal heart beats, and lodges into the heart wall in one of the thin walls sections, the catheter tip can punch through the atrial wall and create cardiac tamponade. If the superior vena cava above the pericardial sac is perforated, a pleural infusion is created, leaking fluid into the pleural or lung cavity. During use, a stiff catheter and tip increases the possibility of endothelial abrasion and vessel wall or right atrium wall perforation. Such perforation generally requires surgical intervention to resolve.

Because of these dangers, CV catheters typically include a soft distal tip that yields when it contacts a vessel wall, and a radiopaque marker is incorporated into the tip to monitor its location within the body. This reduces, but does not eliminate, the possibility of the catheter perforating the vessel wall during repeated contact during use. Therefore, CV catheters tips have been made with softer materials to yield more easily when contacting a vessel wall. Such tips are made of materials such as low durometer urethanes, for example Tecoflex and Pellethane, due to their high durability and ease of manufacturing. Importantly, however, all commercially available CV catheters with soft distal tips have one common feature—their distal tip has only a single

infusion. Such a lumen extending through the distal tip does not have any medical implement, for example, a sensor or a probe, located within because it would compromise the flexibility of the soft tip and would also interfere with the passing of the guidewire during insertion.

Pulmonary artery (PA) catheters, on the other hand, have blunt rigid tips because they are inserted through a vascular access introducer. Such an introducer has already been positioned within the target vessel, and includes a large bore port through which the PA catheter can be passed, and a hemostasis valve on its proximal end to prevent blood leakage around the catheter. Furthermore, many PA catheters require a stiff blunt tip to interface more efficiently with an in vitro calibrating device. Moreover, such stiff, flat tips are relatively easy to manufacture and facilitate polishing of the distal end of the optical fibers. Therefore, typically there is no need for a soft, tapered distal end on PA catheters. Consequently, rigid tipped catheters may include multiple lumens in their distal tips.

Mixed venous oxygen saturation (SvO₂) is the amount of oxygen in blood taken from a vessel coming from the right side of the heart going into the lungs. This reflects the amount of oxygen being delivered to the tissues during cardiac arrest and shock. Selective venous hypoxemia or low oxygen content, when compared to arterial blood, is characteristically seen during cardiac arrest and shock.

When oxygen delivery to the tissues is low, the SvO₂ is low. When oxygen delivery to the tissues is high, the SvO₂ is normal or high. This provides the physiological basis for using SvO₂ as an indicator of response to therapy while treating a patient in cardiac arrest or shock. Intermittent SvO₂ measurement can be predictive of outcome in cardiac patients and hemodynamically unstable trauma patients and medical patients.

Typically, SvO₂ is drawn from a pulmonary artery (PA) catheter which is between 65–110 centimeters long and is placed into a vein that accesses the right side of the heart and then into the pulmonary artery. However, placement of a PA catheter is extremely difficult and can be impractical during cardiac arrest and severe shock due to low blood pressure.

The central venous system is located much closer to the skin and can be more easily accessed during shock and cardiac arrest. Thus, a number of studies have supported the substitution of central venous (right atrial or superior vena cava) oxygen saturation (ScvO₂) for pulmonary artery blood oxygen saturation (SvO₂) during spontaneous circulation, circulatory failure, and closed chest CPR. The central venous blood can be obtained much more easily than blood from the pulmonary artery under conditions of shock and cardiac arrest. Thus, it is more feasible to use the central venous system as it provides similar information.

Fiber optic technology has previously been utilized in measuring ScvO₂. U.S. Pat. No. 5,315,995 to Rivers ('995), issued May 31, 1994, describes a fiber optic catheter and its efficacy for continuous measurement of central venous oxygen saturation. The catheter includes a catheter body having a fiber optic bundle disposed therein. In operation, this catheter is inserted into the subclavian vein or internal jugular vein with the aid of a catheter introducer or guide wire. The '995 patent, however, does not teach a soft multiple lumen tip at all and does not even address the issue of keeping the distal tip of the catheter soft and flexible during use despite the presence of a fiber optic bundle.

Currently, there is no answer to the problem of keeping a CV catheter tip flexible when multiple lumens are required at the distal tip, let alone when one or more of the lumens contains a medical implement. Accordingly, there is a need

for an improved central venous catheter having a soft tip that has multiple lumens and can measure physiologic parameters without the need for multiple catheter insertions.

SUMMARY OF THE INVENTION

The present invention provides a multiple lumen central venous catheter having a soft tip. The catheter includes a generally tubular catheter body having a proximal end and a distal end, the catheter body defining therein at least one primary lumen and at least one medical implement lumen. A soft, tapered distal catheter tip has a distal end and a proximal end abutting the distal end of the catheter body. The catheter tip defines at least one primary lumen aligned with the at least one primary lumen of the catheter body and at least one medical implement lumen aligned with the at least one medical implement lumen of the catheter body. At least one optical fiber extends through the catheter medical implement lumens of the catheter body and the catheter tip, and is secured thereto only at the distal end of the catheter tip.

Desirably, the at least one optical fiber extends to a distal face of the catheter tip and be secured thereto. The optical fiber may be secured using adhesive that is only applied along a short portion of the medical implement lumen having an axial length of between 0.5–3.5 mm. The adhesive may be cured by ultraviolet light, wherein a portion of the catheter tip permits passage of ultraviolet light therethrough into the medical implement lumen. Further, the catheter tip may be formed of two materials. For example, one material may comprise the portion that permits passage of ultraviolet light, and another material that provides a radiopaque marker.

In one embodiment, the catheter tip has at least two exterior taper angles (one in a proximal region and one in a distal region of the catheter tip), and the proximal region may have a greater taper angle than the distal region. Desirably, at least one of the proximal and distal regions of the catheter tip is more flexible than the catheter body and forms a bending portion of the catheter tip. At least one of the proximal and distal regions may be made of a material that has a durometer of less than or equal to 100 Shore A hardness. The proximal region may have a larger air-to-material ratio in transverse cross-section than the distal region. Preferably, in transverse cross-section, both the at least one primary lumen and the at least one medical implement lumen are enlarged in the proximal region relative to the surrounding material in comparison to the relative size of the lumens and material in the distal region, such that the proximal region has a larger air-to-material ratio than the distal region.

The catheter tip of the central venous catheter desirably has a length of at least 7.6 mm (0.30 inches).

Another aspect of the invention is a multiple lumen central venous catheter having a soft tip, including a generally tubular catheter body having a proximal end and a distal end, the catheter body defining therein at least one primary lumen and at least one medical implement lumen. A soft, tapered distal catheter tip has a proximal end that abuts the distal end of the catheter body and a distal end. The catheter tip defines at least one primary lumen aligned with the at least one primary lumen of the catheter body and at least one medical implement lumen aligned with the at least one medical implement lumen of the catheter body. The catheter tip comprises a proximal region and a distal region wherein at least one of the proximal and distal regions is more flexible than the catheter body.

In one exemplary embodiment, the proximal and distal regions are comprised of different materials. In another embodiment, a medical implement is extending through the medical implement lumens of the catheter body and the catheter tip and could be secured at the distal end of the catheter tip.

A still further aspect of the invention is a central venous catheter having a soft tip, comprising a generally tubular catheter body and a soft, tapered distal catheter tip. The catheter body has a proximal end and a distal end, and defines therein at least one primary lumen and at least one medical implement lumen. The catheter tip includes a proximal end abutting the distal end of the catheter body and a distal end, and further defines within at least one primary lumen aligned with the at least one primary lumen of the catheter body and at least one medical implement lumen aligned with the at least one medical implement lumen of the catheter body. The catheter tip has sufficient column strength to resist buckling during insertion using the Seldinger technique over a guidewire, but is sufficiently flexible to deform when the tip is subjected to axial or radial loads in the body in the absence of the guidewire. The catheter further incorporates a sensor extending through the medical implement lumen of the catheter body and the medical implement lumen of the catheter tip.

In one embodiment, the sensor extends to a distal face of the catheter tip and is secured thereto using adhesive. The sensor may be secured using adhesive that is only applied along a short portion of the medical implement lumen having an axial length of between 0.5–3.5 mm. The adhesive may be cured by ultraviolet light, wherein a portion of the catheter tip permits passage of ultraviolet light therethrough into the medical implement lumen. Further, the catheter tip may be formed of two materials.

The sensor is selected from the exemplary group consisting of one or more optical fibers, a pH sensor, a pressure sensor, a temperature sensor, at least one pacing lead, and a pacing electrode. The sensor could be a probe that is removable from the catheter.

In another embodiment, the catheter tip has at least two exterior taper angles, and the proximal region has a greater taper angle than the distal region. Desirably, at least one of the proximal and distal regions is more flexible than the catheter body and forms a bending portion of the catheter tip. At least one of the proximal and distal regions may be made of a material that has a durometer of less than or equal to 100 Shore A hardness. The proximal region may have a larger air-to-material ratio in transverse cross-section than the distal region.

The present invention also teaches a method of measuring oxygen saturation of the venous system, comprising the steps of:

- providing a central venous catheter having a catheter body and a soft, multiple lumen catheter tip, the catheter tip tapering down from a proximal end to a distal end;
- providing at least one optical fiber extending through the catheter body to the distal end of the catheter tip;
- inserting the central venous catheter into a venous system vessel using the Seldinger technique;
- advancing the catheter tip of the central venous catheter into a location in the venous system for measuring oxygen saturation of the venous blood; and
- measuring oxygen saturation of venous blood using the optical fiber.

BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1A and 1B are longitudinal sectional and end elevational views, respectively, of a central venous catheter of the prior art having a single lumen tip;

FIG. 2A is a partial sectional view of a taper-tipped prior art catheter similar to that shown in FIG. 1A traveling over a guidewire and just prior to insertion into a body vessel;

FIG. 2B is a graph generally illustrating the reaction force experienced by the operator when the inserting the catheter of FIG. 2A into the vessel;

FIG. 3A is a partial sectional view of a blunt-tipped prior art catheter traveling over a guidewire and just prior to insertion into a body vessel;

FIG. 3B is a graph generally illustrating the reaction force experienced by the operator when the inserting the catheter of FIG. 3A into the vessel;

FIG. 4 is a side elevational view of a typical pulmonary artery (PA) catheter of the prior art;

FIGS. 5A and 5B are perspective and longitudinal sectional views, respectively, of a central venous catheter of the prior art that includes fiber optics extending through a lumen to the rigid distal tip;

FIGS. 6A and 6B are transverse sectional views through the catheter of FIGS. 5A and 5B, taken along lines 6A—6A and 6B—6B, respectively;

FIGS. 7A and 7B are longitudinal sectional and end elevational views, respectively, of a central venous catheter of the present invention having a soft multiple lumen tip;

FIG. 7C is a transverse sectional view through the catheter of FIG. 7A, taken along lines 7C—7C and slightly enlarged;

FIG. 8A is a perspective view of a soft multiple lumen distal tip of an alternative catheter of the present invention;

FIG. 8B is an exploded, partial sectional view of the catheter distal tip of FIG. 8A and a sensor probe used therewith;

FIGS. 9A and 9B are longitudinal sectional and end elevational views, respectively, of an alternative soft multiple lumen catheter tip of the present invention having multiple tapers;

FIG. 9C is a schematic elevational view illustrating material removed from the exterior of the catheter tip of FIG. 9A so as to form the multiple tapers and create a bending focal point;

FIGS. 9D and 9E are transverse sectional views through the catheter of FIG. 9A, taken along lines 9D—9D and 9E—9E, respectively;

FIGS. 10A and 10B are graphs comparing the axial and lateral displacements, respectively, of a standard conical tip and the dual-taper tip of FIG. 9A subject to axial and radial loads;

FIG. 11 is a schematic elevational view of a catheter tip of the present invention having various lengths for increased flexibility;

FIGS. 12A—12C are Finite Element models of three catheter tips of the present invention, all being subjected to the same lateral load;

FIG. 13A is a longitudinal sectional view through a catheter distal tip of the present invention;

FIGS. 13B and 13C are transverse sectional views through the catheter of FIG. 13A, taken along lines 13B—13B and 13C—13C, respectively, illustrating the different cross-sectional areas of primary and medical implement lumens at those two locations; and

FIG. 14A is perspective view of an alternative catheter distal tip of the present invention made of two materials.

FIG. 14B is a perspective view of another alternative catheter distal tip of the present invention, that facilitates attachment of optical fibers in a medical implement lumen at a distal end of the catheter tip.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

The following detailed description, and the figures to which it refers, are provided for the purpose of describing example(s) and specific embodiment(s) of the invention only and are not intended to exhaustively describe all possible examples and embodiments of the invention.

The present invention primarily relates to an improved central venous catheter having at least one optical fiber, and preferably a plurality, for measuring oxygen saturation of venous blood. Indeed, though the examples used herein are central venous catheters, it should be understood that various aspects of the invention are generic to any catheter used in the body that requires a soft distal tip. That includes catheters that are inserted over a guidewire using the Seldinger technique, and other soft-tipped catheters that are inserted using other means. In particular, the various constructions of the soft tip of the catheters described herein may be applied to other than central venous catheters. This is not to say that all catheters can be interchanged and used for all purposes. For example, catheters that are inserted using the Seldinger technique must have a tapered tip.

Furthermore, various exemplary embodiments of the present invention maintain the soft, flexible nature of the distal tip of the catheter while also utilizing somewhat stiffer optical fibers therethrough. However, the invention is not limited to optical fibers, and any medical implement passed through the catheter to its distal tip may be substituted.

Prior to a discussion of the various advantageous aspects of the novel catheters of the present invention, various prior art catheters will be described.

FIGS. 1A and 1B schematically illustrate the distal end of a prior art central venous catheter 20. As mentioned above, central venous catheters are introduced into the venous system using the Seldinger technique, which involves advancing the catheter 20 over a previously inserted guidewire. This will be more clearly described with respect to FIGS. 2 and 3, but catheter 20 includes a tapered, soft distal tip 22 formed on the end of, or otherwise attached to, a main catheter body 24. The length of the tip 22 is shown as LTIP, which is typically around 6.35 mm (0.25 inches), and no more than 7.4 mm (0.29 inches). FIG. 1B is a view of the end of the catheter 20 which illustrates that the largest outer diameter of the tip 22 is as large as the outer diameter of catheter body 24.

The soft tip 22 is typically constructed separately from the catheter body 24 and attached thereto using adhesive or heat bonding. The catheter body 24 is relatively flexible so as to easily pass through courtesy in the venous vasculature. Exemplary materials for the catheter body 24 include Tecoflex and Pellethane. The soft tip 22 is relatively more flexible than the body 24, and is typically made of Tecoflex.

The catheter body 24 includes a generally centered through lumen 26 that is aligned with a generally centered through lumen 28 in the soft tip 22. These aligned lumens 26, 28 permit the catheter 22 to ride over the guidewire. Furthermore, once properly inserted, the guidewire can be removed and fluid can be passed through the lumens 26, 28. The catheter body 24 further includes a pair of auxiliary lumens 30a, 30b that are shown closed at their distal ends.

Each of these auxiliary lumens **30a**, **30b** communicates with the interior of the body vessel through a side port **32a**, **32b** located just proximal to the end of the catheter body **24**. Therefore, fluid may be infused through the lumens **30a**, **30b** and side port **32a**, **32b** into the target vessel. Although not shown, some type of radiopaque or otherwise imageable marker is typically provided on the tip **22** for the purpose of locating the tip within the body.

It is important to note that the central venous catheter **20** has only a single lumen (aligned lumens **26**, **28**) that extends to the soft tip **22** which is used for passing a guidewire during insertion, and later for fluid infusion. Such a lumen extending through the distal tip **22** cannot have any medical implement, for example, a sensor or a probe, located within it because such an implement would compromise the flexibility of the soft tip and would also interfere with the passing of the guidewire during insertion.

Now with reference to FIGS. 2-4, the shapes of the distal ends of various catheters are shown in conjunction with their use. FIG. 2A shows a conventional CV catheter **20** having a tapered tip **22**, such as that shown in FIGS. 1A and 1B, riding over a guidewire **40** that has previously been inserted into a body vessel **42**. The guidewire **40** passes through an insertion path **44** formed in the surrounding tissue and the wall of vessel **42**. Typically, this insertion path **44** is first formed with a needle and a guidewire inserted therethrough. Subsequently, a tubular instrument known as a dilator is inserted over the guidewire and pushed through the tissues surrounding the puncture hole and into the vessel. This creates a large enough opening for the tapered catheter **20**. FIG. 2B is a schematic graph of the force required to push the catheter **20** through the insertion path **44**. A relatively low insertion force is required to pass the catheter **20** into the vessel **42**, which is preferred by the operator.

FIG. 3A shows another exemplary catheter **50** of the prior art that has a relatively blunt and rigid tip **52**. The catheter **50** is shown riding over a guidewire **54** that has previously been inserted into a body vessel **56** through an insertion path **58**. Forcing the blunt tip **52** through the insertion path **58** results in the insertion force graph of FIG. 3B. That is, in contrast to the graph of FIG. 2B for the tapered tip **22**, the insertion force required is much larger. Disadvantageously, the higher forces are transmitted to the catheter body which may tend to buckle, and the catheter may cause trauma to the tissue surrounding the insertion path **58**. Furthermore, the operator experiences difficulty in inserting the catheter **50** into the vessel **56**, which is disconcerting and makes the task more difficult.

For comparison, FIG. 4 illustrates a typical prior art pulmonary artery (PA) catheter tip **60** that also includes a blunt or flat end face **62** that provides a terminus for the fiber optics therein. Because of this blunt end face **62**, insertion using the Seldinger technique, as with the catheter shown in FIG. 3A, results in high insertion forces and potential damage to the surrounding tissue. The PA catheter **60** further includes a recessed region **64** near its distal end for mounting an expansion balloon, which stiffens the distal tip.

Oximetry PA catheters also have a blunt or flat distal tip which provides an interface with a calibrating media for the fiber-optics therein. Specifically, the distal end of the catheter with the fiber optics is held in contact with an in vitro calibrating device which permits calibration of the catheter without drawing a blood sample from the patient. Oximetry PA catheters include an expansion balloon on their distal end for stiffening the tip. PA catheters with rigid blunt tips are acceptable in light of their use and insertion techniques, and they even have several advantages; they are easily manu-

factured, polishing of the distal end of the fibers is easy, and preparation of the expansion balloon is relatively easy. Further, the rigid tip facilitates positioning within the in vitro calibration device while maintaining intimate contact with the calibrating media. However, the rigidity of the distal tip of such catheters is undesirable in the central venous environment.

There is believed to be only one commercially available central venous (CV) catheter with oximetry, available from Edwards Lifesciences of Irvine Calif. The distal end of this catheter is illustrated in FIGS. 5A-5B and 6A-6B, and includes a multi-lumen catheter body **70**, a reduced diameter distal portion **72** for insertion into a calibration device, and a formed distal tip **74**. The distal tip includes a flat end face **76** providing a terminus for a primary lumen **78** and a smaller fiber-optic lumen **80** housing at least two optical fibers **82**. The catheter is formed of a single, homogeneous material and the reduced diameter distal portion **72** is thermo-formed on the end of the extruded catheter body **70**. The forming process renders the distal portion **72** and distal tip **74** relatively rigid.

With reference to FIG. 5B and FIGS. 6A-6B, the catheter body **70** houses four lumens; the aforementioned primary lumen **78** and fiber-optic lumen **80**, as well as a pair of infusion lumens **84a**, **84b** that open through the side wall of the catheter body **70** at a pair of side ports **86a**, **86b**. The infusion lumens **84a**, **84b** terminate at dead-end walls **88** at the distal end of the catheter body **70**. Therefore, only the primary lumen **78** and fiberoptic lumen **80** extend through the entire catheter to the distal end face **76**, which also contributes to rendering the distal portion **72** stiff because there is a smaller air-to-material ratio.

The CV oximetry catheter shown in FIGS. 5 and 6 is not an ideal design. Although the formed distal tip **74** is tapered, the distal end face **76** is flat to accommodate the fiber optics which results in a fairly rigid blunt tip similar to a PA catheter, such as shown in FIG. 4. The blunt rigid tip is difficult to insert into a vessel using the Seldinger technique and increases the risk of vessel perforation once in the vessel, compared to a soft tip CV catheter. As mentioned above, a preferred CV catheter has a soft, tapered distal tip.

More generally, there are three basic requirements of a CV catheter distal tip, with or without the presence of the medical implement. First, the column strength of the catheter tip should be maximized during insertion over the guidewire so as to prevent buckling. Secondly, the column strength of the catheter tip once the guidewire is removed should be minimized. More particularly, the tip should collapse easily if an axial load is applied, which is particularly important if the catheter migrates into the right atrium. Finally, the bend resistance of the catheter tip should be minimized so the tip will bend if it comes in contact with the vessel wall. Unfortunately, adding fiber optics or any other medical implement to a catheter distal tip normally undermines the last two flexibility requirements.

In answer to the problems of prior catheters and to present a solution meeting the above three requirements, the present invention provides a multiple lumen CV catheter which has a multiple lumen soft distal tip that stiff enough to resist buckling during insertion and flexible thereafter despite the presence of a medical implement in at least one of the lumens of the catheter that extends through the distal tip of the catheter.

FIGS. 7A-7C illustrate an exemplary a catheter **80** of the present invention which provides these features. The catheter **80** has a catheter body **88** and a catheter distal tip **82**.

The catheter tip **82** is tapered from a small diameter distal end face **84** outward to a relatively larger diameter proximal end face **86** that abuts an interface **89** of a catheter body **88**. The catheter tip **82**, or at least some portion thereof, has a softer durometer than the material of the body **88**, and may be made of the same or different material. If made of a different material, the catheter tip **82** attaches to the distal end of the catheter body **88** at the interface **89** using, for example, adhesive or other bonding means. Alternatively, the tip **82** and body **88** may be made of the same material, with the tip being more flexible by virtue of a construction of thinner walls or a higher air-to-material ratio cross-section than the catheter body. Suitable materials include, but are not limited to, polyurethane, silicone, or polyvinylchloride (PVC), KRATON, or any medical grade elastomer.

For purposes of this application, the term "soft tip" (or similar terms used herein) means a catheter tip that meets all three above described requirements. As a more specific example, it means that, for instance, at least a bending portion of the tip **82** should have a Shore A hardness of less than the catheter body **88**, and more particularly less than **100**. Stated another way, at least a bending portion of the distal tip **82** should be sufficiently soft and flexible so as to deform or collapse when it encounters the inner wall of the vessel or the heart wall.

The catheter **80** thus has the required properties mentioned above, that is, its distal tip **82** has sufficient column strength to resist buckling during insertion over a guidewire, but is sufficiently flexible to deform when subjected to axial or radial loads in the absence of the guidewire and its bend resistance should be minimized. Again, it should be noted that although the catheter **80** is particularly useful as a CV catheter with oximetry or other sensors, different catheters, such as pulmonary artery and peripheral axis catheters, could also benefit from its novel features, as disclosed in copending patent application Ser. No. 10/195,954, entitled "MULTIPLE LUMEN CATHETER HAVING A SOFT TIP," filed Jul. 16, 2002.

The catheter **80** has multiple lumens, at least one of which is normally associated with infusing fluid and withdrawing blood samples, and at least one other associated with placement or positioning of a biomedical sensor or other medical implement. In the illustrated embodiment, the catheter body **88** has a primary lumen **90**, a device or medical implement lumen **92**, and an auxiliary lumen **94**. The catheter tip **82** has a primary lumen **96** and a medical implement lumen **98**. Both the primary and medical implement lumens **90**, **92** in the catheter body **88** align with the primary and medical implement lumens **96**, **98** and extend through the catheter tip **82** and open at the distal end face **84**. The aligned medical implement lumens **92** and **98** and the aligned primary lumens **90** and **96** could be alternatively described as a single medical implement lumen extending through the catheter body and the catheter tip and as a single primary lumen extending through the catheter body and the catheter tip, respectively. In contrast, the auxiliary fluid lumen **94** terminates at the distal end of the catheter body **88** and opens at a side port **100**.

In the illustrated embodiment, a medical implement is a biomedical sensor extending through the medical implement lumens **92**, **98** which comprises, as an example, one or more optical fibers **102** used to transmit and receive light for measuring oxygen saturation. In other configurations within the scope of the present invention, the medical implement lumens **92**, **98** may be used to pass various other medical implements or sensors, for example, temperature sensors, or pressure sensors, or pH sensors, or pacing leads, or pacing

electrodes, or probes. FIGS. 7B–7C illustrate the transverse cross-section of the catheter tip **82**, and it can be seen that the primary lumen **96** intersects the central axis of the catheter **80** but is offset in one direction with respect thereto. The medical implement lumen **98** is shown elongated and arcuate, although other configurations, dimensions, shapes and relative positions of both lumens **96** and **98** are possible and within the scope of the present invention. Moreover, the central venous catheter of the present invention may have additional lumens, some of which may terminate like the lumen **94** at a side port proximally to the distal tip while others may also extend through the catheter distal tip **82**. Furthermore, the catheter body **88** of the present invention may have only a medical implement lumen **92** and a primary lumen **90** (aligned with the corresponding medical implement lumen **98** and the primary lumen **96** of the distal tip), without an auxiliary lumen **94**.

The optical fibers **102** (or other above-mentioned medical implements) are desirably fastened or secured within the distal tip **82** so as to prevent their migration. Another aspect of the present invention is that the fibers **102** are secured in a manner that does not compromise the flexibility and other required features of the soft tip **82**. For example, the medical implement lumen **98** is shown tapering down from a proximal end of the catheter tip (which is the area adjacent to and incorporating the proximal end face **86**) toward the distal end of the catheter tip (which is the area adjacent to and incorporating the distal end face **84**). A short portion **104** of the medical implement lumen **98** at a distal end of the catheter tip extending proximally from the distal end face **84** does not need to taper, but is rather sized just larger than the diameter of the fibers **102**. Only in this portion **104** are the fibers **102** secured to the catheter tip **82**, for example, by adhesive. Because the portion **104** is limited in axial length, the length along which adhesive or other means for attachment is provided is also limited. Preferably, the portion **104** extends axially along a length which is less than 3.5 mm, more preferably between 0.5–3.5 mm, and most preferably between 1–2 mm.

Typical adhesives used in this context are relatively stiff when cured, and other methods of securement contemplated, such as solvent bonding, heat forming, or ultrasonic bonding, also result in a stiff section where applied. Even a simple compression fit results in a stiff portion where the tip **82** and fibers **102** are in interfering contact. Consequently, the combination of the joined optical fibers **102**, adhesive (or other joining technique) applied in prior art along all or a substantial length of the distal tip **82**, and material of the distal tip **82** was significantly stiffer and did not fulfill the goals of the catheter of the present invention. Further, if not managed, bending of the region in which the adhesive was applied could cause the adhesive to crack or otherwise loosen. With the catheter of the present invention, however, because the optical fibers **102** are only secured in this short portion **104** of the medical implement lumen **98**, the remainder of the outer fibers remain free to slide with respect to the medical implement lumens **92** or **98**. Therefore, when an axial or radial load is imparted to distal tip **82**, the tip deforms or buckles in the region that is proximal to this short portion **104**. The very distal end of the tip **82** is relatively stiffer, but this does not compromise the performance characteristics of the catheter as mentioned above.

FIG. 8A is a perspective view of an alternative soft multiple lumen catheter tip **110** on the end of the catheter body **112** of the present invention that does not have a sensor fixed therein, such as the fiber optics **102** disclosed above.

Instead, the soft distal tip **110** includes a primary lumen **114** and a medical implement lumen **116** that receives sensors. FIG. **8B** is a longitudinal sectional view of the soft distal tip **110** and catheter body **112** that are either secured together at an interface **118**, or formed of a homogeneous material. The primary lumen **114** and the medical implement lumen **116** are aligned with or continuations of similar lumens in the catheter body **112** as shown. A pair of auxiliary lumens **120a**, **120b** that each opens at side ports **122a**, **122b** may be provided in the catheter body **112**. FIG. **8B** also shows an elongated probe **130** that has a connector **132** at its proximal end and a sensor **134** at its distal end. The probe **130** is sized to pass through the medical implement lumen **116** and may be utilized at or near the distal face **124** of the catheter tip **110**. Sensors that can be used include fiber-optics, temperature sensors, pH sensors, pressure sensors, a sensor for cardiac pacing, and the like. Once again, because the distal tip **110** is soft (i.e., softer than catheter body **112**), and because the probe **130** is not secured within the medical implement lumen **116**, the soft distal tip easily deforms upon application of axial or radial forces.

As mentioned above, the various distal tips of the catheters of the present invention are made softer than the main catheter body, and preferably soft enough to easily deform upon contact with the surrounding vessel wall or heart wall. To do this, the distal tips are made of a soft material and/or are constructed in a way that they flex easily.

For example, FIGS. **9A–9E** illustrate a soft catheter tip **140** that has a tapered proximal region **142** and distal region **144** that has a narrower taper, the two regions meeting at an elbow **146**. FIG. **9D** is a section through the proximal region **142**, and FIG. **9E** is a section through the distal region **144**. The length of the proximal region **142** is shown as L_1 , while the length of distal region **144** is shown as L_2 . The total length of the distal tip **140** is given as L_{TTP} . In an exemplary embodiment, L_{TTP} is about 7.6 mm (0.30 inches), and L_1 and L_2 are approximately equal. Alternatively, L_1 and L_2 may be unequal with the longer of the two lengths being preferably more flexible than the other. The exemplary taper angle of the proximal region **142** is about 30°, while the exemplary taper angle of the distal region **144** is about 15°. Other angles of taper are also within the scope of the present invention.

FIG. **9C** is a schematic view of the distal tip showing in phantom the line **150** of a tip having a single taper. The cross-hatched region **152** is the volume of material that is removed to result in the differing tapers of the proximal region **142** and distal region **144**. The reduction of the overall material in the center of the tip allows for a bending focal point.

FIGS. **9D** and **9E** illustrate the respective air-to-material ratios in the proximal region **142** and the distal region **144**. As seen, there is a greater volume of air to material in the proximal region **142** than in the distal region **144**. Therefore, the bending stiffness of the proximal region is less than that of the distal region. As a result, axial or radial forces imparted to the distal end face **154** of the tip **140** will cause bending in the proximal region **142** rather than in the distal region **144**. Because of this, sensors placed through, or fixed in a medical implement lumen **156**, are positioned within a relatively stiff distal region which is beneficial in some instances, such as when calibrating fiber optics.

Alternatively, rather than removing material from the exterior of the distal tip **140**, the lumens **156** and **158** may be enlarged within the tip to result in the same effect. That is, more material may be removed to enlarge the lumens in the proximal portion **142** to create a larger air-to-material

ratio therein. This is shown further in FIGS. **13A–13C**. Of course, various combinations of the two can also be utilized.

FIGS. **10A** and **10B** are graphs that illustrate the column strength and flexural strength, respectively, of the standard conical tip and a dual-tapered tip, such as that shown in FIG. **9A**. In both graphs, the applied force in pounds is indicated at the left along the vertical axis, while the corresponding displacement of the respective tips in inches is shown along the horizontal axis. As indicated, the dual-tapered tip displaces farther in either case at lower applied forces. This means that the dual-tapered tip more easily buckles upon an applied axial force and bends more easily upon an applied radial force.

FIG. **11** schematically illustrates several superimposed soft catheter distal tips **160a**, **160b**, **160c** having gradually longer lengths L_1 , L_2 , L_3 , respectively. Each of these tips **160** has a single conical taper and is otherwise cylindrical and configured much like previously described catheter distal tips. A radial force F is shown applied near the distal end of each of the tips. One way to render the tip more flexible is to increase its length. Therefore, the longest tip **160c** will bend the farthest distance from the implied force F because of the longer lever arm. For multiple lumen soft catheter tips of the present invention, the length should be at least 5.1 mm (0.20 inches), and preferably at least about 7.6 mm (0.30 inches). An additional benefit of increasing the length of the distal tip is that the taper angle is reduced, which reduces the resistance to insertion using the Seldinger technique, and consequently reduces the required column strength of the distal tip.

FIGS. **12A–12C** are Finite Element models of different catheter tips of the present invention, each under the same radial or lateral load. FIG. **12A** shows a deflected tip **170** that is made of a single homogeneous material, and the corresponding relaxed state is seen in phantom. FIG. **12B** shows a tip **172** that has a proximal region **174** made of the same material as the entire tip **170** in FIG. **12A**, and a distal region **176** made of a softer material (i.e., more flexible). Accordingly, the distal region **176** curls and deflects more than the distal portion of tip **170** in FIG. **12A**. Finally, FIG. **12C** illustrates a tip **180** that has a distal region **182** made of the same material as the entire tip **170** in FIG. **12A**, and a proximal region **184** made of a softer material (i.e., more flexible). Therefore, under load, the tip **180** bends more than tip **170** in FIG. **12A**. The behavior of tip **180** under a lateral load approximates that of the tips discussed above that have optical fibers glued to their distal ends, thus making the distal region more stiff than the proximal region. The lengths of the regions may be equal or not, and the tips may be made from the various material discussed herein, such as Pellethane and Tecothane, both urethanes. The softer of the two materials, or in other words the bending portion, preferably has a durometer of less than 100 Shore A, more particularly between about 45–100 Shore A, most desirably about 75 Shore A.

FIGS. **13A–13C** illustrate a further configuration for rendering a portion of the catheter distal tip more soft and flexible than the rest of the catheter body. Specifically, FIG. **13A** shows the distal tip **190** having a proximal region shown in cross-section in FIG. **13B** and a distal region shown in cross-section in FIG. **13C**. As can be seen, a medical implement lumen **192** and a primary lumen **194** are reduced in size in the distal region shown in FIG. **13C**. This means that the air-to-material ratio in the distal region is less than that in the proximal region, and thus the distal tip **190** bends or buckles in the proximal region. Another alternative embodiment of the present invention may combine a dual-

taper tip of the catheter with the different materials of various portions of the distal tip. One exemplary configuration of the dual-material, dual-taper is where the proximal segment consists of a high durometer material while the distal segment consists of a lower durometer material. This configuration creates a very flexible tip with low column strength.

A further example of a soft-tipped catheter of the present invention is seen in FIG. 14A. In this aspect of the present invention, a catheter body **200** attaches at an interface **202** to a distal tip **204** formed of two materials. A proximal region **206** of the catheter tip **204** is formed of a first material and a distal region **208** of the catheter tip is formed of a second material. In this embodiment, the catheter tip includes a primary lumen **210** and a medical implement lumen **212**. By way of example and not limitation, a medical implement, such as a pair of optical fibers **214**, extend through the medical implement lumen **212**. As before with reference to FIG. 7, the fibers could be secured by adhesive and the adhesive could be applied only along a short portion adjacent the distal face **216**, and preferably along a portion between 0.5–3.5 mm in length.

The two materials of the proximal and distal regions **206**, **208** may be more or less relatively flexible depending on the catheter tip design. For example, if a sensor such as fiber optics is secured in the distal end of the tip, the proximal region is desirably more flexible (softer) so that it provides a point of bending. Various combinations of materials such as polyurethane, silicone, or polyvinylchloride (PVC), KRATON, or any medical grade elastomer may be used to create a catheter tip that is either more flexible in the proximal region or more flexible in the distal region. Furthermore, various constructional differences may accentuate the difference in flexibility.

FIG. 14B illustrates a still further alternative configuration of a catheter distal tip of the present invention. As in FIG. 14A, a catheter body **220** attaches at an interface **222** to a distal tip **224** formed of two materials. In this embodiment, however, a first material **226** forms a proximal region and two generally axially-oriented segments **228a**, **228b** thereof extend on diametrically opposed sides of the distal tip all the way to a distal face **230**. Of course, more than two generally axially oriented segments, similar to **228a** and **228b**, are within the scope of the present invention. A second material **232**, which could be transparent, fills the remainder of the spaces between two or more segments **228a**, **228b**. Optical fibers **234** extend through a medical implement lumen **236** and are secured therein with adhesive. As before, the adhesive is only applied along a short portion adjacent the distal face **230**, and preferably along a portion between 0.5–3.5 mm in length.

The second material **232** may be transparent or only partly opaque such that ultraviolet light can pass therethrough. A suitable adhesive is one that is cured with ultraviolet light, and the first material **226** is desirably opaque to prevent such light passing through. In this manner, adhesive can be injected into the medical implement lumen **236**, and upon application of ultraviolet light, only a portion that is exposed by the first material **226** becomes cured. This reduces the importance of the volume of adhesive injected into medical implement lumen **236**, and thus facilitates assembly and ensures consistency.

The transparent material **232** in the distal tip provides a window through which ultraviolet light can pass and cure adhesive previously injected into the medical implement lumen **236**. The first material **226** may be radiopaque such

that the side segments **228a**, **228b** provide axially oriented markers to guide positioning of the distal tip **224** within the body.

In assembling the catheter tips of FIGS. 14A and 14B, the dual-material distal tips and catheter body may be constructed using an RF tip forming process, but techniques such as heat forming or steam forming may also work. This involves the use of three extruded tubes, one for the catheter body, and two others for the dual-material tip. Two mandrels are inserted through the three tubes and RF tip formed simultaneously. Once the catheter is constructed, the adhesive is drawn into the medical implement lumen using a vacuum pump. If the transparent materials are used in the tips, they would provide an advantage in that the depth of the adhesive can be visualized. Another alternative is to do without the transparent material but instead use an opaque or semi-opaque material that still permits some ultraviolet light through, and which may be entirely radiopaque. An adhesive that can be cured by ultraviolet light or heat could be used. Some ultraviolet passes through the tip material and partially cures the adhesive, and the remainder of the curing process is done using heat.

The present invention also teaches a method of measuring oxygen saturation of the venous system. The steps of the method are as follows:

- providing a central venous catheter having a catheter body and a soft, multiple lumen catheter tip, the catheter tip tapering down from a proximal end to a distal end;
- providing at least one optical fiber extending through the catheter body to the distal end of the catheter tip;
- inserting the central venous catheter into a venous system vessel using the Seldinger technique;
- advancing the catheter tip of the central venous catheter into a location in the venous system for measuring oxygen saturation of the venous blood; and
- measuring oxygen saturation of venous blood using the optical fiber.

The catheter body may include at least one auxiliary fluid infusion lumen and a side port opening adjacent the distal tip, wherein the method includes infusing fluids through the auxiliary fluid infusion lumen. The distal tip of the catheter preferably comprises a material that has a durometer of less than or equal to 100 Shore A hardness. Furthermore, the distal tip of the catheter preferably has a proximal region and a distal region, and wherein the proximal region has a larger taper angle than the distal region to facilitate insertion using the Seldinger technique.

It will be appreciated that the invention has been described above with reference to certain examples or preferred embodiments as shown in the drawings. Various additions, deletions, changes and alterations may be made to the above-described embodiments and examples without departing from the intended spirit and scope of this invention. Accordingly, it is intended that all such additions, deletions, changes and alterations be included within the scope of the following claims.

What is claimed is:

1. A multiple lumen central venous catheter having a soft tip, comprising:
 - a generally tubular catheter body having a proximal end and a distal end, the catheter body defining therein at least one primary lumen and at least one medical implement lumen;
 - a soft, tapered distal catheter tip having a distal end and a proximal end abutting the distal end of the catheter body, the catheter tip defining therein at least one primary lumen aligned with the at least one primary

lumen of the catheter body and at least one medical implement lumen aligned with the at least one medical implement lumen of the catheter body, wherein the catheter tip has a proximal region and a distal region, and wherein the proximal region is more flexible than the distal region and more flexible than the catheter body and forms a bending portion of the catheter tip; and

at least one optical fiber extending through the at least one medical implement lumen of the catheter body and the at least one medical implement lumen of the catheter tip, and being secured thereto only at the distal end of the catheter tip.

2. The central venous catheter of claim 1, wherein the at least one optical fiber extends to a distal face of the catheter tip and is secured thereto.

3. The central venous catheter of claim 1, wherein the optical fiber is secured using adhesive that is only applied along a short portion of the medical implement lumen of the catheter tip having an axial length of between 0.5–3.5 mm.

4. The central venous catheter of claim 3, wherein the adhesive is cured by ultraviolet light, and wherein a portion of the catheter tip permits passage of ultraviolet light there-through into the medical implement lumen.

5. The central venous catheter of claim 4, wherein the catheter tip is formed of two materials, one material comprising the portion that permits passage of ultraviolet light, and another material that provides a radiopaque marker.

6. The central venous catheter of claim 1, wherein the catheter tip is tapered to have a smaller diameter on its distal end than on its proximal end and has a proximal region and a distal region, the catheter tip having at least two exterior taper angles, and wherein the proximal region has a greater taper angle than the distal region.

7. The central venous catheter of claim 1, wherein the proximal region is made of a material that has a durometer of less than or equal to 100 Shore A hardness.

8. The central venous catheter of claim 1, wherein the proximal region has a larger air-to-material ratio in transverse cross-section than the distal region.

9. The central venous catheter of claim 8, wherein, in transverse cross-section, both the at least one primary lumen and the at least one medical implement lumen are enlarged in the proximal region relative to the surrounding material in comparison to the relative size of the lumens and material in the distal region, such that the proximal region has a larger air-to-material ratio than the distal region.

10. The central venous catheter of claim 1, wherein the catheter tip has a length of at least 7.6 mm (0.30 inches).

11. A multiple lumen central venous catheter having a soft tip, comprising:

a generally tubular catheter body having a proximal end and a distal end, the catheter body defining therein at least one primary lumen and at least one medical implement lumen;

a soft, tapered distal catheter tip having a distal end and a proximal end abutting the distal end of the catheter body, the catheter tip defining at least one primary lumen aligned with the at least one primary lumen of the catheter body and at least one medical implement lumen aligned with the at least one medical implement lumen of the catheter body, wherein the catheter tip has a proximal region and a distal region and wherein the proximal region is more flexible than the distal region and is more flexible than the catheter body, and wherein the proximal region has a larger air-to-material ratio in transverse cross-section than the distal region.

12. The central venous catheter of claim 11, wherein the catheter tip is tapered to have a smaller diameter on its distal end than on its proximal end and has at least two exterior taper angles, and wherein the proximal region has a greater taper angle than the distal region.

13. The central venous catheter of claim 11, wherein at least one of the proximal and distal regions is made of a material that has a durometer of less than or equal to 100 Shore A hardness.

14. The central venous catheter of claim 11, wherein, in transverse cross-section, both the primary lumen and the medical implement lumen are enlarged in the proximal region relative to the surrounding material in comparison to the relative size of the lumens and material in the distal region, such that the proximal region has a larger air-to-material ratio than the distal region.

15. The central venous catheter of claim 11, wherein the catheter tip is formed of two materials.

16. The central venous catheter of claim 11, further comprising a medical implement extending through the medical implement lumen of the catheter body and the medical implement lumen of the catheter tip.

17. The central venous catheter of claim 16, wherein the medical implement is a sensor for measuring physiologic parameter secured to the medical implement lumen only at the distal end of the catheter tip.

18. A multiple lumen central venous catheter having a soft tip, comprising:

generally tubular catheter body having a proximal end and a distal end, the catheter body defining therein at least one primary lumen and at least one medical implement lumen;

a soft, tapered distal catheter tip having a distal end and a proximal end abutting the distal end of the catheter body, the catheter tip defining at least one primary lumen aligned with the at least one primary lumen of the catheter body and at least one medical implement lumen aligned with the at least one medical implement lumen of the catheter body, wherein the catheter tip has a proximal region and a distal region, and wherein the proximal region has a larger air-to-material ratio in transverse cross-section than the distal region, wherein the catheter tip has sufficient column strength to resist buckling during insertion using the Seldinger technique over a guidewire, but is sufficiently flexible to deform when the tip is subjected to axial or radial loads in the body in the absence of the guidewire; and

a sensor extending through the at least one medical implement lumen of the catheter body and the at least one medical implement lumen of the catheter tip.

19. The central venous catheter of claim 18, wherein the sensor is secured only at the distal end of the catheter tip.

20. The central venous catheter of claim 19, wherein the sensor is secured using adhesive and adhesive is only applied along a short portion of the medical implement lumen having an axial length of between 0.5–3.5 mm.

21. The central venous catheter of claim 20, wherein the adhesive is cured by ultraviolet light, and wherein a portion of the catheter tip permits passage of ultraviolet light there-through into the medical implement lumen.

22. The central venous catheter of claim 18, wherein the catheter tip is formed of two materials.

23. The central venous catheter of claim 18, wherein the sensor is selected from the group consisting of:

one or more optical fibers;
a pH sensor;
a pressure sensor;

- a temperature sensor;
- at least one pacing lead;
- a pacing probe; and
- a pacing electrode.

24. The central venous catheter of claim 18, wherein the catheter tip has a proximal region and a distal region, and wherein the distal region has a different durometer than the proximal region.

25. The central venous catheter of claim 18, wherein the catheter tip has a proximal region and a distal region, and wherein at least one of the proximal and distal regions is made of a material that has a durometer of less than or equal to 100 Shore A hardness.

26. The central venous catheter of claim 18, wherein the catheter tip has a proximal region and a distal region, and wherein one of the proximal region and the distal region is more flexible than the other region.

27. The central venous catheter of claim 18, wherein the catheter tip is tapered to have a smaller diameter on its distal end than on its proximal end and has a proximal region and a distal region, and at least two exterior tapered angles, and wherein the proximal region has a greater taper angle than the distal region.

28. The central venous catheter of claim 18, wherein the sensor is a probe that fits through the medical implement lumens and is removable from the catheter.

29. A multiple lumen central venous catheter having a soft tip, comprising:

- a generally tubular catheter body having a proximal end and a distal end, the catheter body defining therein at least one primary lumen and at least one medical implement lumen;
- a soft, tapered distal catheter tip having a distal end and a proximal end abutting the distal end of the catheter body, the catheter tip defining at least one primary lumen aligned with the at least one primary lumen of the catheter body and at least one medical implement lumen aligned with the at least one medical implement lumen of the catheter body, wherein the catheter tip has sufficient column strength to resist buckling during insertion using the Seldinger technique over a guidewire, but is sufficiently flexible to deform when the tip is subjected to axial or radial loads in the body in the absence of the guidewire; and
- a sensor extending through the at least one medical implement lumen of the catheter body and the at least one medical implement lumen of the catheter tip and secured only at the distal end of the catheter tip.

30. The central venous catheter of claim 29, wherein the sensor is secured using adhesive and adhesive is only applied along a short portion of the medical implement lumen having an axial length of between 0.5–3.5 mm.

31. The central venous catheter of claim 30, wherein the adhesive is cured by ultraviolet light, and wherein a portion of the catheter tip permits passage of ultraviolet light there-through into to medical implement lumen.

32. The central venous catheter of claim 29, wherein the catheter tip is formed of two materials.

33. The central venous catheter of claim 29, wherein the catheter tip has a proximal region and a distal region, and wherein the distal region has a different durometer than the proximal region.

34. The central venous catheter of claim 29, wherein the catheter tip has a proximal region and a distal region, and wherein at least one of the proximal and distal regions is made of a material that has a durometer of less than or equal to 100 Shore A hardness.

35. The central venous catheter of claim 29, wherein the catheter tip has a proximal region and a distal region, and wherein one of the proximal region and the distal region is more flexible than the other region.

36. The central venous catheter of claim 29, wherein the catheter tip is tapered to have a smaller diameter on its distal end than on its proximal end and has a proximal region and a distal region, and at least two exterior tapered angles, and wherein the proximal region has a greater taper angle than the distal region.

37. The central venous catheter of claim 29, wherein the sensor comprises one or more optical fibers.

38. The central venous catheter of claim 29, wherein the sensor is selected from the group consisting of:

- a pH sensor;
- a pressure sensor;
- a temperature sensor;
- at least one pacing lead;
- a pacing probe; and
- a pacing electrode.

39. A multiple lumen central venous catheter having a soft tip, comprising:

- a generally tubular catheter body having a proximal end and a distal end, the catheter body defining therein at least one primary lumen and at least one medical implement lumen;
- a soft tapered distal catheter tip having a distal end and a proximal end abutting the distal end of the catheter body, the catheter tip defining therein at least one primary lumen aligned with the at least one primary lumen of the catheter body and at least one medical implement lumen aligned with the at least one medical implement lumen of the catheter body; and
- at least one optical fiber extending through the at least one medical implement lumen of the catheter body and the at least one medical implement lumen of the catheter tip, and being secured thereto only at the distal end of the catheter tip, wherein the optical fiber is secured using adhesive that is only applied along a short portion of the medical implement lumen of the catheter tip having an axial length of between 0.5–3.5 mm, wherein the adhesive is cured by ultraviolet light, and wherein the catheter tip is formed of two materials, one material comprising a portion of the catheter tip that permits passage of ultraviolet light therethrough into the medical implement lumen, and another material that provides a radiopaque marker.

* * * * *

专利名称(译)	中心静脉导管具有柔软的尖端和光纤		
公开(公告)号	US6999809	公开(公告)日	2006-02-14
申请号	US10/196101	申请日	2002-07-16
[标]申请(专利权)人(译)	CURRIER CLIFFORD 迈克尔·希金斯 GORDON MARK FAUGHT STACY WEST DEAN		
申请(专利权)人(译)	CURRIER CLIFFORD 迈克尔·希金斯 GORDON MARK FAUGHT STACY WEST DEAN		
当前申请(专利权)人(译)	爱德华生命科学公司		
[标]发明人	CURRIER CLIFFORD HIGGINS MICHAEL GORDON MARK FAUGHT STACY WEST DEAN		
发明人	CURRIER, CLIFFORD HIGGINS, MICHAEL GORDON, MARK FAUGHT, STACY WEST, DEAN		
IPC分类号	A61B5/00 A61M25/00 A61N1/04 A61B5/145 A61B5/1459		
CPC分类号	A61M25/0071 A61M25/0032 A61M2230/205 A61M2025/0081		
其他公开文献	US20040015061A1		
外部链接	Espacenet USPTO		

摘要(译)

一种多腔导管，具有柔软的锥形多腔远端尖端，用于插入身体血管。其中一个管腔的尺寸设计成可以通过导丝，使得导管可以使用Seldinger技术插入到身体血管中。至少一个医疗器械腔用于放置或定位生物学传感器或其他医疗器械。例如，穿过医疗器械腔的至少一根光纤可以在远端尖端处发射和接收光，以测量血液的氧饱和度。导管可具有圆柱形导管主体，软远侧末端附接到该导管主体。柔软的尖端减少了血管或组织穿刺和磨损的可能性。尖端由柔软的塑料或柔韧材料构成，在施加力时容易产生。例如，尖端可以由比导管主体更软的材料制成，或者如果由相同的材料制成，则尖端可以配置有更薄的壁或更高的空气-材料比横截面。可以使用各种几何构造和材料组合来降低尖端对施加载荷的抵抗力。本发明的导管的一个特别有用的应用是配备有用于测量血氧测定的纤维的中心静脉导管。纤维延伸到尖端的远端，并且优选地用最小的粘合剂固定在其中，以便限制添加到尖端的刚度。一种特别有用的结构是仅使用粘合剂沿约0.5-3.5mm的长度将纤维固定在医疗器械腔内。

