



(19) **United States**

(12) **Patent Application Publication**
Rahe-Meyer

(10) **Pub. No.: US 2005/0014999 A1**

(43) **Pub. Date: Jan. 20, 2005**

(54) **DEVICE FOR VERIFYING AND MONITORING VITAL PARAMETERS OF THE BODY**

(57) **ABSTRACT**

(76) Inventor: **Niels Rahe-Meyer, Hannover (DE)**

Correspondence Address:
Striker Striker & Stenby
103 East Neck Road
Huntington, NY 11743 (US)

(21) Appl. No.: **10/484,737**

(22) PCT Filed: **Jul. 24, 2002**

(86) PCT No.: **PCT/DE02/02718**

(30) **Foreign Application Priority Data**


Jul. 26, 2001 (DE)..... 101 36 355.9

Publication Classification

(51) **Int. Cl.⁷ A61B 5/00**

(52) **U.S. Cl. 600/323; 600/547; 600/549; 600/586**

The invention lies in the domain of medical technology and relates to a diagnosis and monitoring device for the rapid diagnosis and monitoring of vital parameters of the human or animal body, in particular of the heart and/or lungs, said device being compact, without cables and/or tubes and easy to use for the user. Devices such as a bell (1) comprising a membrane (2) and/or measuring electrodes (4, 5) for receiving and forwarding acoustic and/or electric signals of the body are arranged in a housing with a cross-section that is approximately the size of the palm of a hand and a height of approximately half a hand-width, on the side of a housing that is to be placed on the body. Said devices are connected to a device in the housing, which analyses, filters and stores the signals of the receiving device and to additional devices for visually reproducing the evaluated signals in digital or analogue form using display fields (14, 15, 16, 17) and/or for acoustically reproducing said signals using a loudspeaker (9) located in the housing. The diagnosis and monitoring device also comprises interfaces (10, 11) for connecting external devices and equipment (e.g. computer, earphones, printer). The principal characteristics of the invention are illustrated in FIGS. 1 and 3.

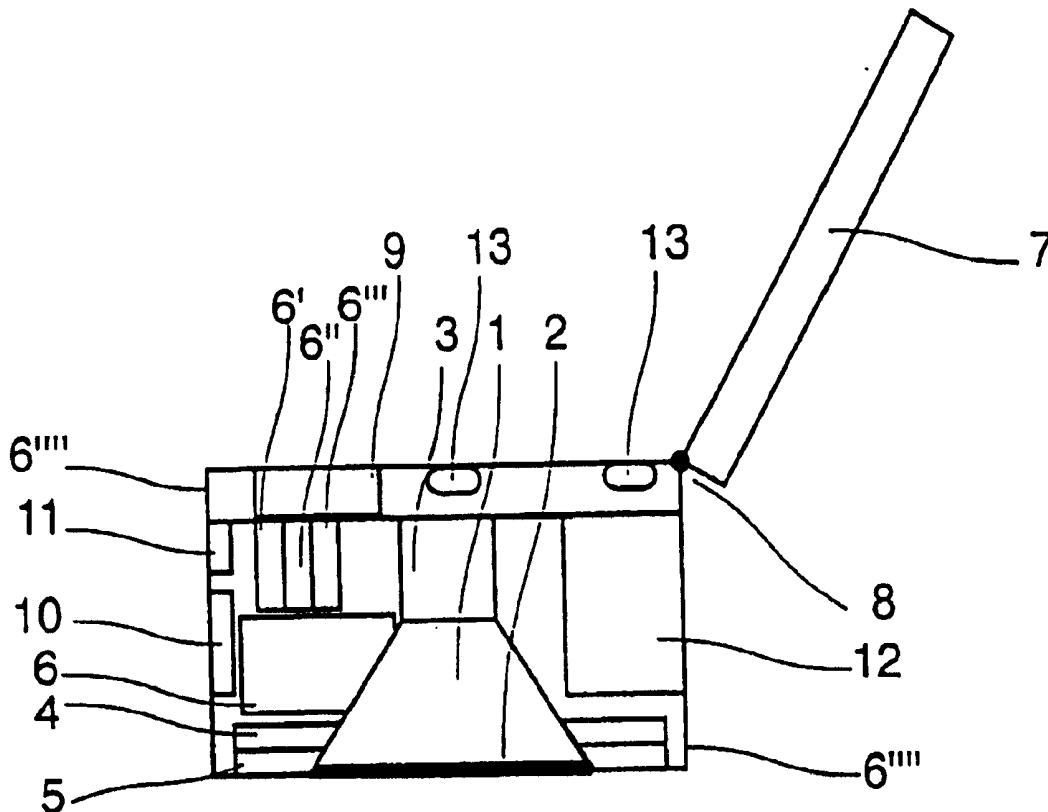

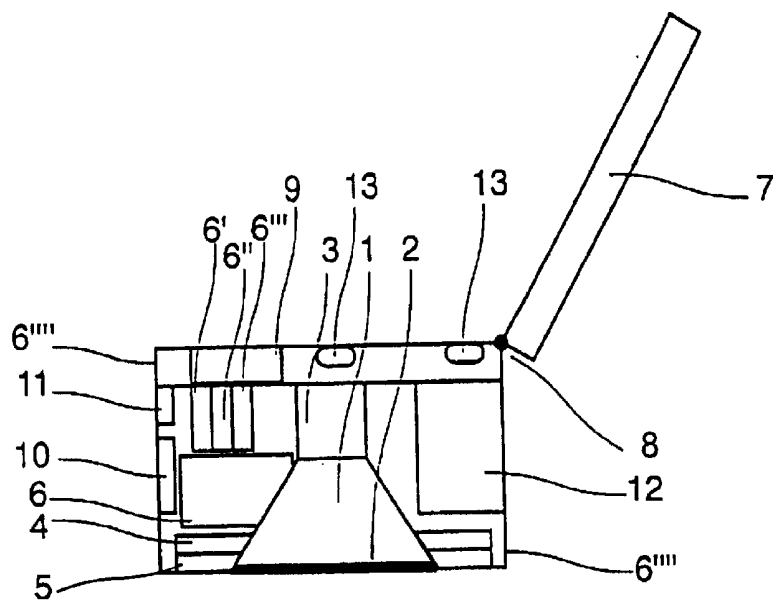


Fig.1

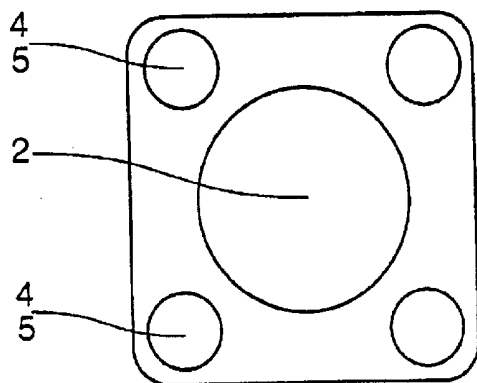


Fig.2

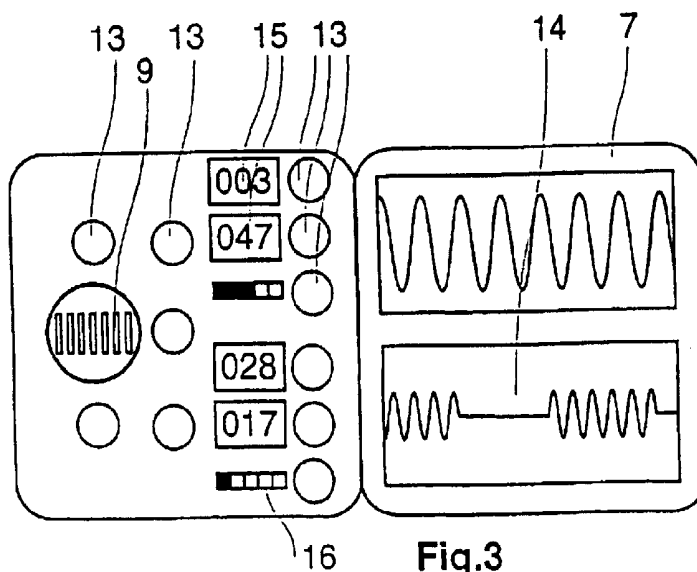


Fig.3

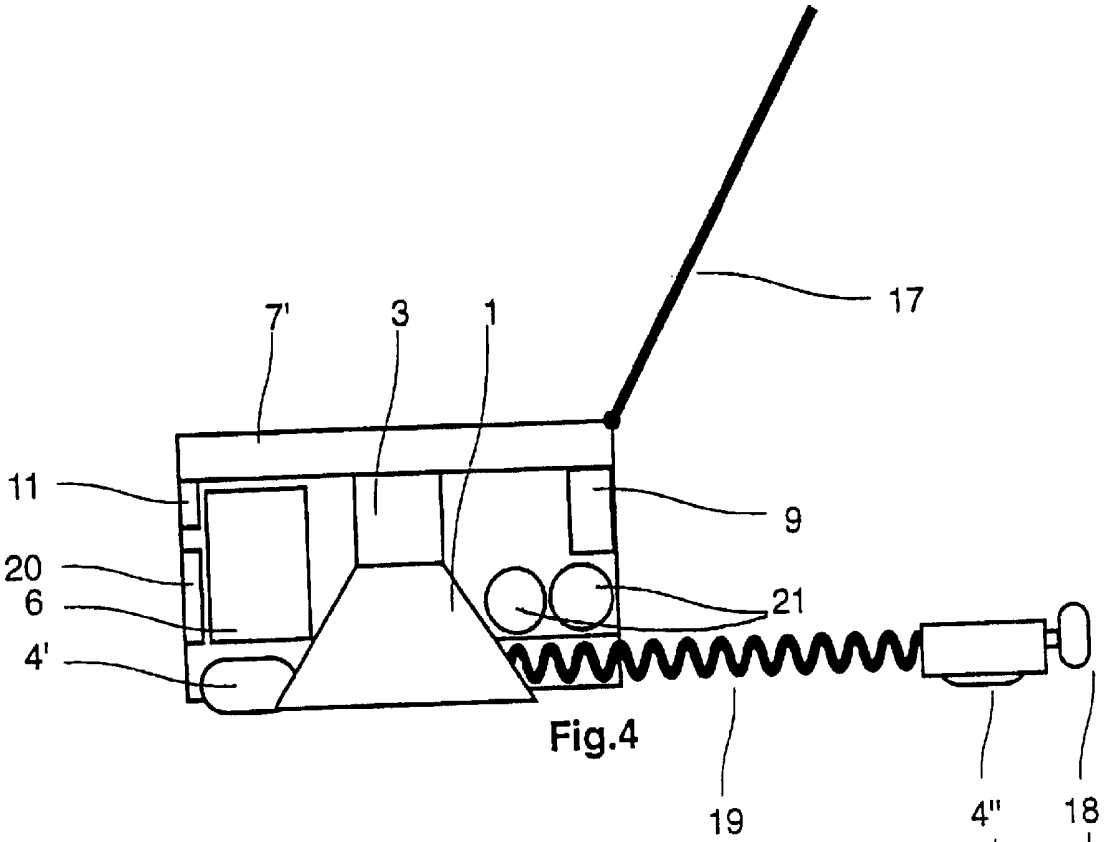


Fig.4

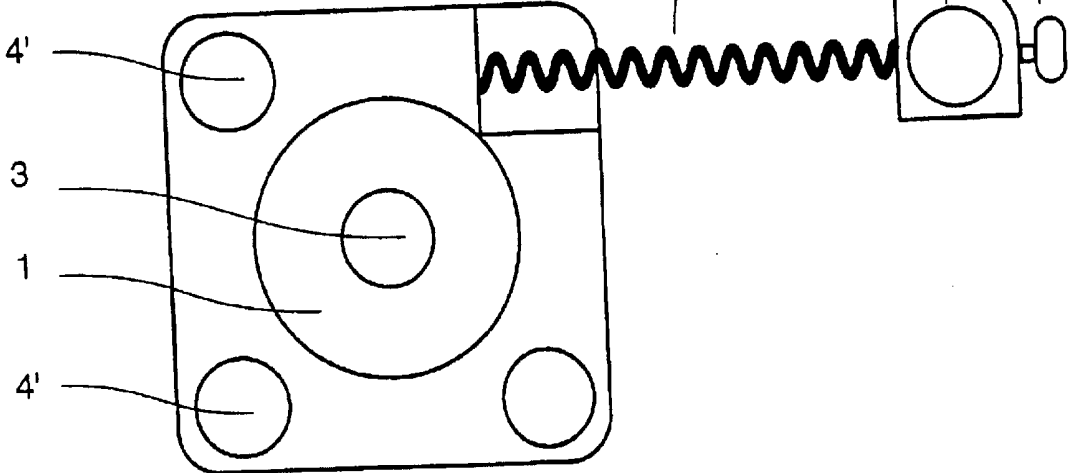


Fig.5

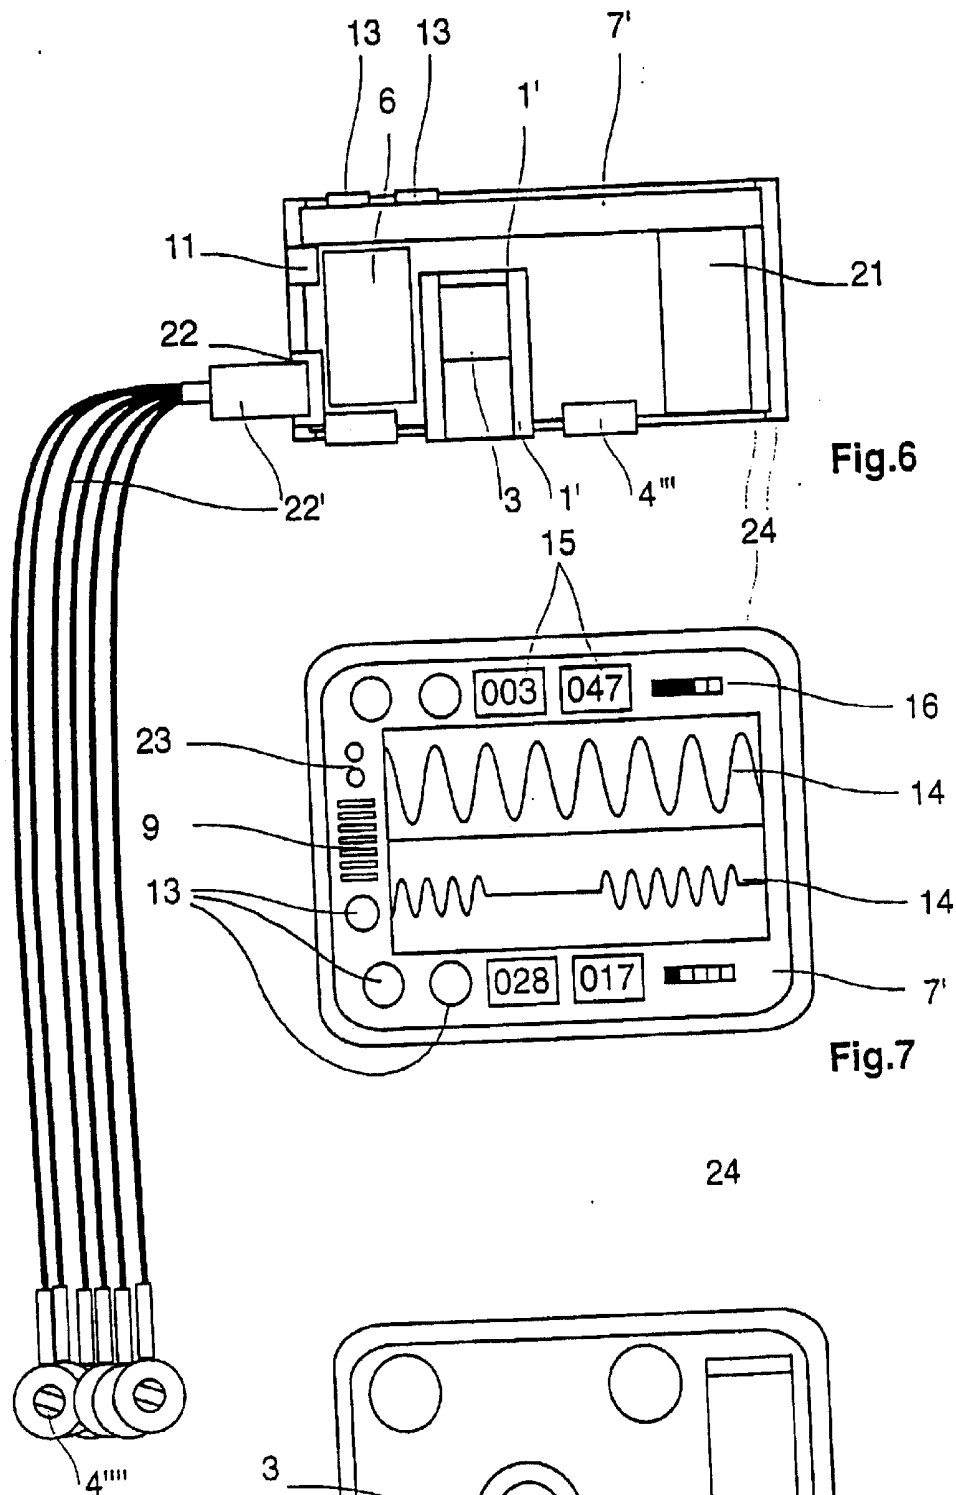


Fig.6

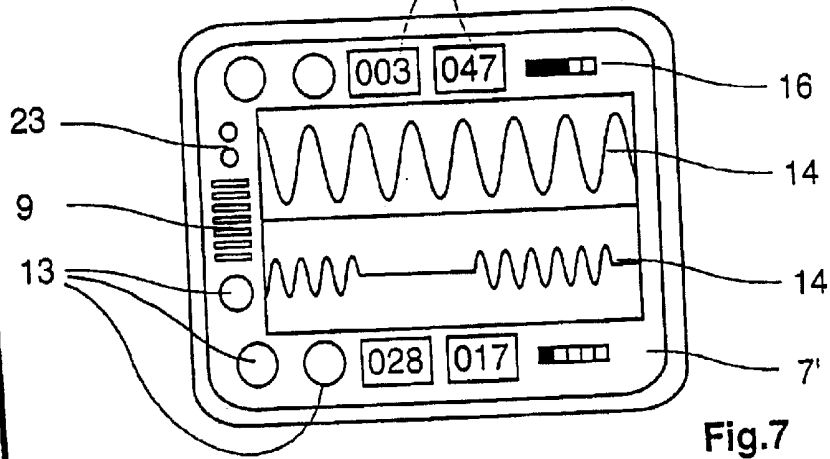


Fig.7

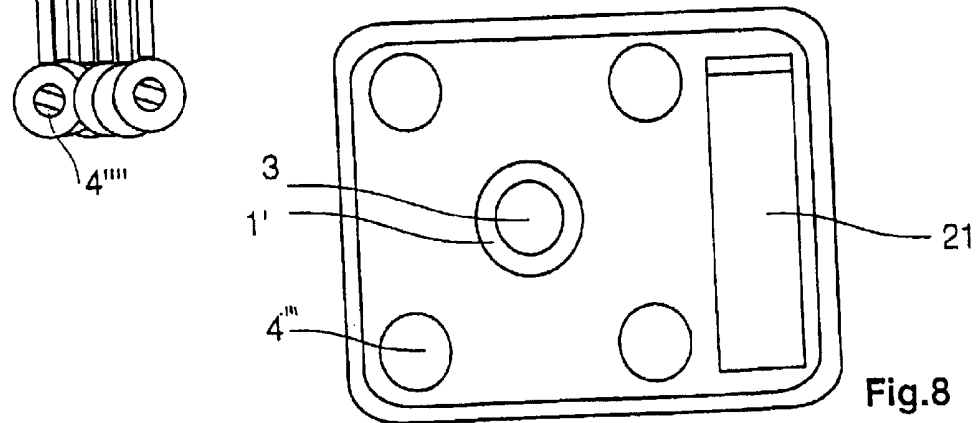


Fig.8

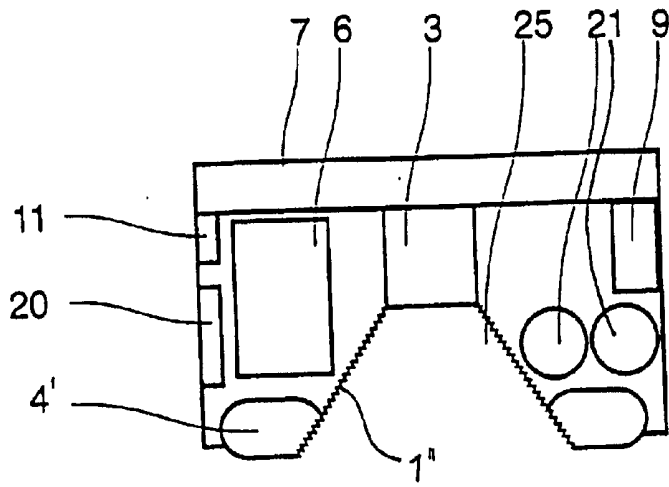


Fig.9

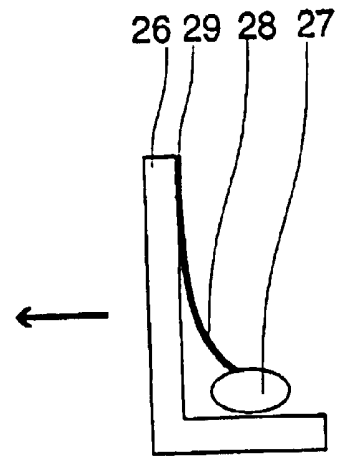


Fig.12

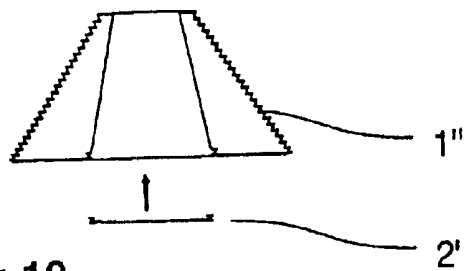


Fig.10

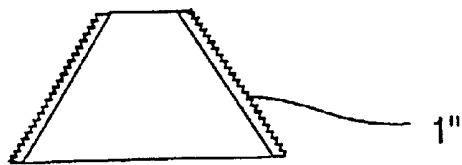


Fig.11

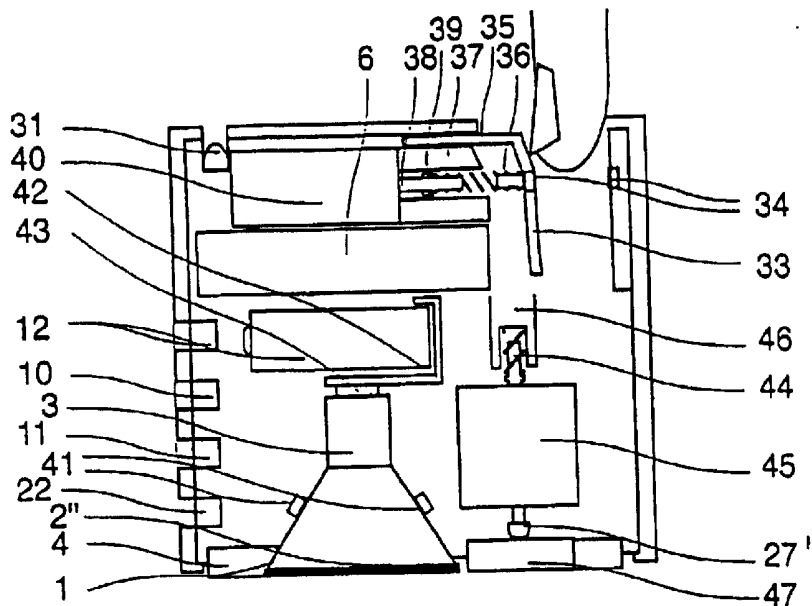


Fig.13

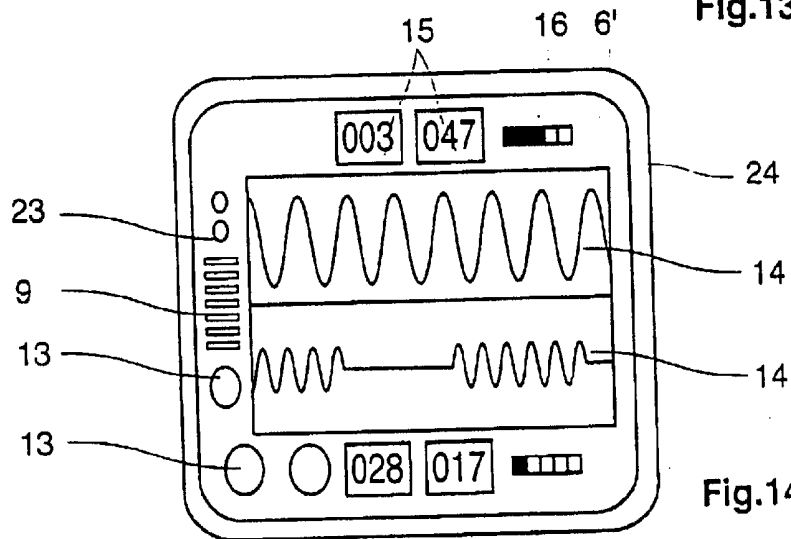


Fig.14

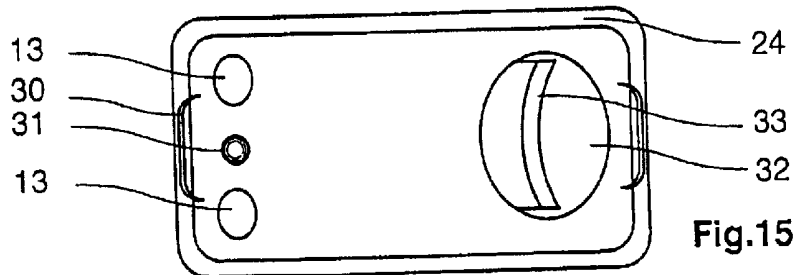


Fig.15

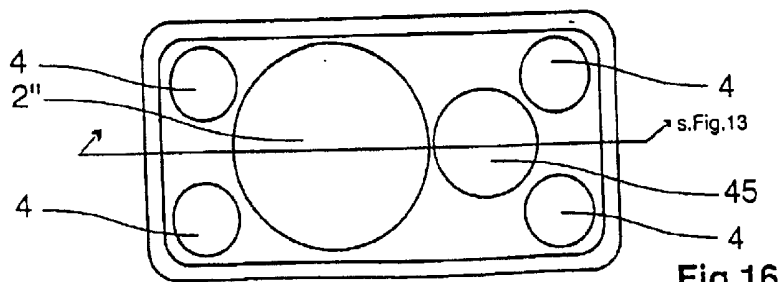


Fig.16

DEVICE FOR VERIFYING AND MONITORING VITAL PARAMETERS OF THE BODY

[0001] This invention is a device for the examination and monitoring of vital parameters of the human or animal body, in the form of a compact Diagnostic Device, which may be used single-handedly and within easy reach, without the necessity for cables or tubes.

[0002] With already known examination and monitoring equipment, several electrodes are attached to the body to be examined, to measure electrical tension fluctuations of the body. Usually, the number of electrodes is increased proportionally to the number of measuring vectors. With most of the well-known equipment, these electrodes are, connected by means of cables to the amplifier units in order to amplify the signals and connect them to separate analysis equipment. This well-known examination and monitoring equipment is, through the cable connections mentioned above and the separate amplifier units and the analysis equipment and especially through the dimensions of these components, most disadvantageous. Firstly, the cables cause obstruction the person being examined. But above all, the doctors are hindered the most, as the equipment is fixed in its location to each person being examined and can not be readily taken by the doctor and, in a short time, be used for other patients.

[0003] A cable-free diagnosis and monitoring unit is known from DE 43 29 898 A1. The electrical cable connection of the electrodes to the analysis station, can be here be omitted, as the electrodes attached to the body being examined are equipped with sender units and aerials, through which they are in wireless contact with the analysis station, which receives the recorded signals. The analysis station also has receptor units and aerials. From this publication, it is known that, positioned in one electrode casing are a number of electrode pins, for the recording of electrical potential fluctuations on various points with different vectors. This diagnosis and monitoring equipment, however still has major disadvantages. It is technically too complicated and too expensive, through the necessary transmitters, receivers, detectors, coding and encoding units and more. The relatively large electrodes, by their design, have to be removable, but permanently fixed to the body, whilst for the examination of different body areas separate electrodes, also with the necessary transmitters and receivers are required. Furthermore, the relatively large analysis station is in a separate room, which is a major disadvantage, especially as it contains the display, data storage and alarm units. It is, therefore not always accessible and viewable by the examining technician and especially by the doctor, as the unit is not transportable. A final, major disadvantage is that only a few examination functions are integrated into the device, in particular, no listening with stethoscope (Auskultation) is possible, nor any percussion, no measuring of oxygen saturation of the blood and of the time taken for recapillarisation.

[0004] Also known from DE 40 12 874 C2, is a blood pressure measuring device with long-term ECG measuring units, which can be carried on the body. The part of the equipment necessary for the automatic taking of the blood pressure, including the cuff and pump, as well as the analysis and control switches, are combined in one system. This device is especially laid out for the automatic measurement of long-term ECG and blood pressure, and its main task is

to take blood pressure measurements in connection with ECG-fluctuations. Because of the required cuff and pump necessary to operate it, the equipment has to be allocated to a single patient and be worn by him/her. In this device, the electrodes and sensors are connected by means of cables to the long-term ECG measuring equipment.

[0005] The aim of the invention is to avoid the disadvantages of known diagnostic and monitoring equipment, by creating a device for a fast diagnosis of the most important vital parameters of the human and animal body, especially the examination of the heart, and/or the lungs in their expansion, condition and ability to function, as well as the constant monitoring of the person being examined, in such a compact form and without cable and/or tube connections, so that it can be readily carried by the technician, especially the doctor, and used immediately without any connections, as well as, a procedure for measuring of oxygenation and circulation outputs of the human and animal body, using x-ray and applying pressure onto an area of the body, followed by a pressure release.

[0006] This aim will, in the main, be met through the features of the Patent Claim 1. Further useful and effective developments will be reached by adjustments listed in the further Patent Claims.

[0007] Below is a list of examples of the development of the invention, explained with the aid of drawings.

[0008] FIG. 1 shows: the device for the diagnosis and monitoring of the vital parameters, viewed in cross-section, from the side;

[0009] FIG. 2 shows: the Diagnostic Device as in FIG. 1, viewed from the underside, which will be placed on the person to be examined;

[0010] FIG. 3 shows: the Diagnostic Device as in FIG. 1, viewed from above, with monitor screen open, as well as the operational and display unit;

[0011] FIG. 4 shows: the Diagnostic Device in an altered version, with a fixed monitor/screen and foldable protective lid, as well as an extractable sensor electrode;

[0012] FIG. 5 shows: the Diagnostic Device as in FIG. 4, viewed from below, as in FIG. 2;

[0013] FIG. 6 shows: a further version of the Diagnostic Device, viewed in cross-section, from the side, as in FIG. 1, but with a sound cylinder, and an external sensor electrode positioned at the interface to the Diagnostic Device and a firmly integrated monitor/screen;

[0014] FIG. 7 shows: the Diagnostic Device as in FIG. 6, viewed from above, with the display and operational area as well as a monitor/screen;

[0015] FIG. 8 shows: the Diagnostic Device as in FIG. 6, viewed from below, as in FIG. 2;

[0016] FIG. 9 shows: the Diagnostic Device in a further version, with an exchangeable sound funnel and an exchangeable membrane, for the recording of acoustic signals;

[0017] FIG. 10 shows: a detail of FIG. 9; a sound funnel as well as a membrane, before use;

[0018] FIG. 11 shows: a detail to FIG. 9; another sound funnel without a membrane;

[0019] FIG. 12 shows: a sideways attachable percussion module, as a component for the Diagnostic Device, according to FIGS. 1, 4, 6 and 9;

[0020] FIG. 13 shows: another version of the Diagnostic Device, viewed in cross-section, with an integrated percussion element containing an electro-magnetically driven tapping device, and, on the upper side, above the operational and display area/monitor, a recording unit with a pressure device for use on inserted body part and a light transmitter/receiver;

[0021] FIG. 14 shows: the operational and display area, with a monitor/screen of the Diagnostic Device as in FIG. 13, viewed from above, after the pressure device and the recording unit have been removed;

[0022] FIG. 15 shows: the Diagnostic Device as in FIG. 13, viewed from above, looking down onto the pressure device;

[0023] FIG. 16 shows: the Diagnostic Device as in FIG. 13, viewed from below, with measuring electrodes and sound funnel.

[0024] In the described version of the Diagnostic Device in FIG. 1 to 3, are the recording units for the acoustic signals of the body (1, 2, 3) as well as the recording units for the electrical signals, in the form of tension fluctuations and/or of impedance measurements, and/or for temperature measurements, consisting of four measuring electrodes (4) with a receptacle for contact gel (5), placed in the casing; the sound funnel and the measuring electrodes with the contact gel receptacle are pointed towards the person/object being examined, when using the device. The membrane (2) of the sound funnel and the cover for the contact gel receptacle (5) of the measuring electrode (4), are positioned on a horizontal level. On the upper side of the device, is the operational and display area with the operational keys (13), the speaker (9), the digital display areas (15) and the amplitude beam display (16). On the outer rim of the casing of the Diagnostic Device, is a foldable monitor/screen (7), attached with a hinge (8) situated, which shows curve-fields' display (14) and is placed onto the operational and display area through the hinge (8) when not in use. Inserted into the casing of the Diagnostic Device are—but not individually illustrated in the drawings—analogue and digital electronics to amplify/enhance the measurements, to analyse the measurements and to display them. Furthermore, there is an element for data storage inside the casing of the Diagnostic Device. The recording unit for acoustic signals consists of the sound funnel (1), with an attached membrane (2) and the positioned microphone (3). Finally, there is a compartment in the casing for the storage of power supply elements, for example, batteries or rechargeable accumulator (12). As shown schematically in FIG. 1, the Diagnostic Device does additionally have an interface earphones/headphones (10) and for the connection to a computer (11), on an exterior wall of the casing. The microphone (3) of the sound funnel is connected to the speaker (9) in the operational and display area.

[0025] In the version in FIGS. 4 and 5 of the Diagnostic Device, instead of the attached, foldable device for the visual reproduction of the electrical signals and/or tempera-

ture measurements and the recorded and analysed by the recording unit, there is a monitor (7), with a curve-fields' display (14) integrated into the operational and display area and developed according to FIG. 7. To protect the operational and display area including the monitor, there is a protective lid (17), which is foldable on the upper side rim of the device. Incidentally, this version of the Diagnostic Device can concur with the version in FIG. 1 to 3. However, in FIG. 4, there are further developments, instead of the measuring electrodes with the contact gel receptacle (5), which are sunken in the casing, measuring electrodes (4') intended, which are on the same level as the sound funnel (1) and the membrane (2) and situated underneath the casing, slightly domed, and usefully protruding.

[0026] Further, as is shown in FIGS. 4 and 5, at least one of the electrodes is removable and placed on the bottom of the casing as a measuring electrode (4''), with a connection cable (19) to the Diagnostic Device; it can be positioned separately from the rest of the unit on an area of the body to be examined on its own or, simultaneously, when using the unit with further measuring electrodes, on a different area of the body. To make using the measuring electrode (4'') easier, it has a handle (18). In this version, the speaker (9) is also positioned on a different place on the casing of the Diagnostic Device and, instead of the compartment for the rechargeable accumulator (12), a battery slot (21) is intended. Finally, on the casing, there is, in addition to the computer interface (11) or, in its place, an interface (20) for a printer.

[0027] A further version is illustrated in FIGS. 6 and 8. They differ to the examples explained above, mainly in that, instead of the sound funnel (1) with a membrane (2), a sound cylinder (1') is used, which serves at the same time as a fixing for the microphone (3), the microphone being switched on afterwards. An interface (22) is provided by means of a connector plug (22') for the connection of external measuring electrodes (4''') via cables. Finally, instead of the measuring electrode (4'), which can be used here, domed measuring electrodes (4''') have been used. The operating and display area with the integrated monitor/screen is also set out according to FIG. 7, but can also be set out as in FIGS. 1 and 3.

[0028] FIG. 9 to 11 show the Diagnostic Device with a further development of the recording unit for acoustic signals, fitted with an exchangeable sound funnel (1'') and exchangeable membrane (2''), whereby the sound funnels used are each connected to the microphone (3) by means of a threaded fitting, a bayonet fixing or in another known way to the casing of the Diagnostic Device.

[0029] A percussion module (26 to 29) is shown in FIG. 12. as an additional component, which can be used in all versions of the Diagnostic Device. It consists of an angled elevation (26), preferably made from steel, whose sides are formed by areas facing each other in a right angle. The vertical side corresponds in its height, in the version shown—although not necessarily—to the height of the exterior walls of the Diagnostic Device; the module is firmly connected—but removable—with its outer side flush to one exterior wall of the Diagnostic Device, in such a way, that the horizontal side of the module runs on a horizontal level with the underside of the Diagnostic Device, facing the body part being examined and therefore, also rests on the object

being examined. On the vertical side of the angled steel elevation (26), on the inside of the upper area (29), a leaf spring (28) is positioned, which has a knocking mechanism (27) on its lower/bottom end. This knocking mechanism rests, held by a spring, inside the horizontal side of the angled steel elevation (26).

[0030] During the examination, by moving the spring (28) with the knocking mechanism (27) by hand, a knocking sound is produced when it springs back onto the horizontal side, which will be resonated by the body or the body part being examined and, thereby, recorded by the acoustic recording device (1, 2, 3; 1', 3'; 1", 2', 3) and passed on for processing.

[0031] A further version of the invented Diagnostic Device is shown in FIG. 13 to 16. As is apparent from FIG. 13, here is the acoustic recording device (1, 2, 3) supplemented by the electrical/electronic elements, in which the membrane (2") in front of the sound funnel (1) and facing it, is light reflective on its inside and the light transmitter (41) and the light receiver (41') are facing each other both positioned by the sound funnel (1). In accordance to the movement of the membrane (2"), when placing it on the body being examined—as for example when examining the abdominal wall of a patient with tension conditions—the light reflection, and its different results, are measured through the elements (41, 41') and passed on for analysis, in addition to the acoustic signals. Instead of the light reflecting membrane (2"), in combination with the light transmitter (41) and the light receiver (41'), the membrane (2) can also be connected with a Piezo element or an Eddy current sensor, which converts the movement or position of the membrane, during examination, into electrical/electronic signals. Instead of, or in addition to, these device elements (2", 41, 41'), surface changes can be measured on the body being examined through pressure on the sound funnel (1)—which is resting in the casing and is movable—and this exerted pressure is passed on to a pressure recorder (42, 43).

[0032] In FIG. 13, a sound-producing component (27', 44 to 47) moves into the place of the percussion module, as in FIG. 12, and is integrated in the Diagnostic Device and its casing. The knocking mechanism (27') for producing the sound is driven by an electro-magnetic drive (44, 45, 46) and, in order to produce the sound, knocks onto the striking area (47), which is on the underside of the Diagnostic Device, lying on the same level as the membrane (2, 2") for the acoustic recording unit. This percussion element can also be used in all versions of the Diagnostic Device.

[0033] In the example in FIG. 13, in addition to measuring the oxygenation and circulation levels of the human or animal body—especially the arterial oxygen saturation of the blood, the arterial capillary and venous blood pressure levels and the recapillarisation time—with the Diagnostic Device described above, there is also a recording unit for ascertaining the light conductance/penetration levels, at the section of the body being examined and the correlation of the light conductance/penetration levels (31 to 40), this unit being folded via a hinge on the side. This recording unit, has an opening for the insertion of a body part, for example a section of a finger, which rests with one side on the exterior wall of the module and on a dish (33) with the opposite side of the body part, which is connected to a pressure device (36 to 40) and is horizontally movable on the guide track (35).

The dish (33) is being pushed, by a pressure shaft (38) and the pressure shaft motor (40), against the inserted section of the finger. The force of this pressure is regulated via a regulating element (39) on the pressure shaft (38) and this element measures the amount of the pressure force. Positioned on the dish (33), in the direction of the section of the finger placed upon it, are one or more light transmitters (34), which work together with an appropriate light receiver (34'), on the opposite exterior wall. The results ascertained by the pair of sensors during the x-ray of the body section examined and correlated light conductance/penetration levels, will be passed on as signals to the analysing electronics of the Diagnostic Device. FIG. 15 shows a fastening device in the form of belt fasteners (30) for the body section being examined, situated on the upper side of the recording unit (33-40). This recording device (33-40) can be used independently of the Diagnostic Devices, as in FIG. 1 to 12, and can, as a separate Diagnostic Device, be used and equipped with a device for electronic analysis/evaluation, filtering and data storage of the supplied signals.

[0034] Finally, FIGS. 13 and 15 show a lamp (31), which can be used with all versions of the Diagnostic Device, and can be useful for checking the functioning of the pupils.

[0035] The invented device and the procedures carried out with it, make the examination and an extended, comparable overview of the vital parameters of a patient possible—amongst other things with the ECG, blood pressure or circulation levels, oxygenation levels (the oxygen saturation of the blood), the recapillarisation time, the tocography and listening with a stethoscope (Auskultation)—within a compact unit, which can be carried around by the person conducting the examination, or the doctor. It contains all the necessary recording, transmitting, analysing and data storing devices for such an extensive diagnosis and for the monitoring of the ascertained electrical and acoustic signals of the body or the body parts examined, as well as display areas for the ascertained and analysed signals. The storage and the optical and acoustic display of the data, make it possible to compare assessments of the measuring results, especially the ECG, as well as heart-beats and heart sounds heard from stethoscope (Auskultation) and percussion, and a side-by-side comparison of measurements can be made, for example by listening with a stethoscope (Auskultation) and with the percussion. The device can be used with a number of patients at any given time and makes it possible, to immediately analyse mechanical, acoustic and electrical occurrences or signals, especially the analysis of the heart and the lung and their functioning. Furthermore, the data storage function (Memory-Funktion) of the device makes it possible to compare the analyses of two occurrences at the same time or of occurrences at different times. Because of this, the device brings major advantages, in comparison to the known diagnostic and monitoring equipment, namely, in the emergency room, in the hospital admission examination departments and to doctors seeing patients in the hospital and also in their surgeries.

1. A device for the examination and monitoring of the vital parameters of the human or animal body (Vitaloskop), in the form of a compact Diagnostic Device, which may be used single-handedly and within easy reach of the user, without the necessity for cables and tubes; characteristic in that, fitted in the casing are devices (1, 1", 2, 2', 2"; 3, 4, 5; 4; 4"; 4"; 34;39;41;43;26; 47), of a size which would fit into

the pockets of a doctors coat, of approximately the size of the palm of the hand in width and a length of approximately half a hand, which record and transmit one or more signals of the body; a device for electronic analysis, filtering and data storage of the signals supplied by these recording devices; devices for visual playback in digital and analog form (7, 14, 15, 16) or for acoustic playback (9) of the analysed signals; finally that in the device on its exterior sides, are interfaces units (10, 11, 20, 22) for the connection of external devices and appliances, such as a computer, ear phones, head phones, a printer and measuring electrodes with cables (4''').

2. A device as in Patent claim 1, characteristic in that the devices for the visual playback of the analysed signals, consist of the operational and display areas with digital display areas (15), amplitude beam display (16) and the necessary operational keys (13) as well as a monitor/screen (7) with curve-fields' display (14), integrated into the operational and display area, which is positioned on the casing of the device, where a number of signals are being recorded, either at the same time or at different times, which can be displayed;

the operational and display areas (13, 15, 16) and the monitor/screen (7) are fitted to the upper side of the device, facing away from the body.

3. A device as in Patent claim 1 or 2, characteristic in that the device for the acoustic playback is a speaker (9) with an amplifier and an alarm, integrated into the casing of the entire device, positioned on the side of the entire device, which is facing away from the body.

4. A device as in Patent claim 1 or 2, characteristic in that the device has, for the recording of body signals, a recording unit for electrical signals, in the form of tension fluctuations and/or of impedance measurements and/or temperature measurements, which consists of two or more measuring electrodes (4, 5; 4'; 4''/4'''), which are positioned on one level on the underside of the casing of the entire device, for placing over or onto the body areas being examined.

5. A device as in Patent claim 1 or 3, characteristic in that the device for the recording of body signals is a recording unit for acoustic signals, consisting of a sound funnel (1, 1''), a membrane (2, 2', 2'') and a microphone (3), whereby the membrane (2, 2', 2'') is positioned on the underside of the casing of the entire device, for placing over or onto the body areas being examined.

6. A method for measuring the oxygenating levels and circulation levels of the human or animal body, especially the arterial oxygen saturation of the blood, the arterial capillary and venous blood pressure levels and the recapillarisation time, characteristic in that a section of the body is being pushed together in a defined way, by the pressure device, and then the pressure will be released again, whereby this section of the body lies between a light transmitter and a light receiver and is x-rayed, and, during this process, this light is being measured, analysed and correlated.

7. A device for the implementation of the method as in Patent claim 6, characteristic in that with a device as in Patent claim 1 or 2, the recording unit has an opening for the insertion of a body part, for example, a section of a finger, whereby the section of the finger rests with one side on the exterior wall of the module and, with the opposite side of the body part on a dish (33), which is connected to a pressure device (36 to 40) and is horizontally movable on the guide

track (35), whereby the dish (33) is being pushed by the pressure shaft (38), and the pressure shaft motor (40), against the inserted section of the finger and the pressure is being regulated and measured via a regulating element (39) on the pressure shaft (38); also, on the dish (33), in the direction of the finger section to be inserted, there is a light transmitter (34), which works together with a light receiver (34'), on the opposite exterior wall of the sensor module.

8. A device as in Patent claim 4, characteristic in that the measuring electrodes (4), on the underside of the device casing, are placed slightly inwards, and each has a receptacle (5), into which a contact substance will be filled, for example, contact gel.

9. A device as in Patent claim 1 and one or more of the Patent claims 2 to 6, characteristic in that one or more measuring electrodes (4', 4'', 4''') are used, which are positioned on one level with the membrane (2, 2', 2'') of the sound funnel (1, 1'').

10. A device as in Patent claim 1 and 8, characteristic in that the measuring electrodes (4'), on the underside of the casing, have a slightly domed surface and/or the measuring electrodes (4'') have a straight surface.

11. A device as in Patent claim 1 and one or more of the Patent claims 2 to 9, characteristic in that one or more measuring electrodes (4'') are positioned on the underside of the casing, but are movable, and are connected, through a connection cable (19) or as a wireless transmitter/receiver system, with the device and its recording unit for electrical signals.

12. A device as in Patent claim 5, characteristic in that the recording unit for acoustic signals has an exchangeable sound funnel (1''), which is placed in the device casing, by means of a threaded fitting, a bayonet fixing or in another known way, and that the exchangeable membrane (2') is positioned on the sound funnel (1'').

13. A device as in Patent claim 5, characteristic in that instead of the sound funnel (1, 1'') with the membrane (2, 2''), a sound cylinder (1') is positioned on the underside of the device, which, at the same time, serves as a fixing for the microphone (3).

14. A device as in Patent claim 1 or 2, characteristic in that the device for the recording of body signals is a recording unit for measuring the mechanical strain/elasticity of the body surface, consisting of the sound funnel (1), which is positioned vertically in the casing and can be adjusted in its height, and additionally works together with a pressure recorder (42, 43) for the recording and transmitting of sound.

15. A device as in Patent claim 1 or 2, characteristic in that the device for the recording of body signals, is a recording unit for measuring the mechanical strain/elasticity of the body surface, consisting of the sound funnel (1), with a membrane (2'), which is light reflective on its inside and is facing the sound funnel, and whereby, facing each other, are a light transmitter (41) and a light receiver (41') positioned on the sound funnel (1, 1''), which ascertain the different light reflections of the vertical doming of the membrane (2, 2') and transmit them to the electronic analysis device.

16. A device as in Patent claim 14, characteristic in that instead of the light transmitter (41) and the light receiver (41'), the membrane (2, 2') is connected to a Piezo element or a Eddy current sensor, which converts the movement or position of the membrane (2, 2') into electrical/electronic signals during the examination process.

17. A method for the diagnosis of sound transmission, reflection and the resonance properties of areas or tissues of the human or animal body, characteristic in that a percussion element produces standardised sound waves, whose reverberation through the body or the body part, is being received by a recording unit and being analysed by a electronic device.

18. A device for the implementation of the method as in Patent claim 17, characteristic in that the percussion element contains a sound-producing part (27', 44 to 47), which is inserted into the device according to Patent claim 1 or 2, with which the knocking mechanism (27') has an electromagnetic drive (44 to 46) for the production of sound, and knocks onto the striking area (47) on the underside of the Diagnostic Device, which also rests on the body part examined.

19. A device for the implementation of the method as in Patent claim 17, characteristic in that the percussion element

contains a sound-producing part (26 to 29), which is firmly connected to an exterior wall of the device casing as in Patent claim 1 or 2, but removable and consists of an angled steel elevation (26), whose side is formed by areas facing each other at a right angle, whereby the horizontal side runs on a horizontal level with the underside of the device, and, on the vertical side of the angled steel elevation (26), on its inside in the upper area (29), a leaf spring (28) is positioned, which has a knocking mechanism (27) on its lower/bottom end, and rests held by a spring, on the inside of the horizontal side of the angled steel elevation (26), which produces a knocking sound, when it is lifted and springs back.

20. A device as in Patent claim 1 or one or more of the Patent claims 2 to 17, characteristic in that the device has a usable lamp (31) with a miniaturised light.

* * * * *

专利名称(译)	用于验证和监测身体重要参数的装置		
公开(公告)号	US20050014999A1	公开(公告)日	2005-01-20
申请号	US10/484737	申请日	2002-07-24
[标]申请(专利权)人(译)	RAHE MEYER NIELS		
申请(专利权)人(译)	RAHE梅耶尔NIELS		
[标]发明人	RAHE MEYER NIELS		
发明人	RAHE-MEYER, NIELS		
IPC分类号	A61B5/00 A61B5/022 A61B5/0404 A61B5/044 A61B5/05 A61B5/053 A61B5/145 A61B5/1455 A61B7/04		
CPC分类号	A61B5/01 A61B5/0404 A61B9/00 A61B5/053 A61B7/04 A61B5/044		
优先权	10136355 2001-07-26 DE		
其他公开文献	US7955273		
外部链接	Espacenet USPTO		

摘要(译)

本发明属于医疗技术领域，涉及一种诊断和监测装置，用于快速诊断和监测人体或动物体，特别是心脏和/或肺部的生命参数，所述装置紧凑，无需电缆和/或管子，易于使用。诸如包括膜（2）的钟形件（1）和/或用于接收和传递主体的声学或/或电信号的测量电极（4,5）的装置布置在壳体中，该壳体具有近似的横截面。在要放置在主体上的壳体的侧面上，手掌的大小和大约半手宽的高度。所述设备连接到外壳中的设备，该设备分析，过滤和存储接收设备的信号以及用于使用显示字段（14,15,16,17）以数字或模拟形式可视地再现评估信号的附加设备。和/或用于使用位于壳体中的扬声器（9）声学地再现所述信号。诊断和监视设备还包括用于连接外部设备和设备（例如计算机，耳机，打印机）的接口（10,11）。本发明的主要特征如图1和图2所示。1和3。

