



US009572519B2

(12) **United States Patent**  
**Shmarak et al.**

(10) **Patent No.:** **US 9,572,519 B2**  
(45) **Date of Patent:** **Feb. 21, 2017**

(54) **METHOD AND APPARATUS FOR INVASIVE DEVICE TRACKING USING ORGAN TIMING SIGNAL GENERATED FROM MPS SENSORS**

(75) Inventors: **Itzhak Shmarak**, Haifa (IL); **Gera Strommer**, Haifa (IL); **Uzi Eichler**, Haifa (IL)

(73) Assignee: **MediGuide Ltd.**, Haifa (IL)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 2179 days.

(21) Appl. No.: **10/986,567**

(22) Filed: **Nov. 10, 2004**

(65) **Prior Publication Data**

US 2009/0182224 A1 Jul. 16, 2009

**Related U.S. Application Data**

(63) Continuation-in-part of application No. 10/938,395, filed on Sep. 9, 2004, which is a continuation-in-part (Continued)

(51) **Int. Cl.**

**A61B 5/05** (2006.01)

**A61B 5/11** (2006.01)

(Continued)

(52) **U.S. Cl.**

CPC ..... **A61B 5/1107** (2013.01); **A61B 5/06**

(2013.01); **A61B 5/7207** (2013.01);

(Continued)

(58) **Field of Classification Search**

CPC ..... **A61B 34/20**; **A61B 5/1107**; **A61B 5/7289**;

**A61B 6/527**; **A61B 6/541**; **A61B 6/547**;

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,937,066 A \* 2/1976 Green et al. .... 73/607

3,974,826 A 8/1976 Eggleton et al.

(Continued)

FOREIGN PATENT DOCUMENTS

EP 0894473 2/1999

EP 0961135 12/1999

(Continued)

OTHER PUBLICATIONS

US 5,924,990, 07/1999, Nachtomy et al. (withdrawn)

(Continued)


*Primary Examiner* — Bo J Peng

(74) *Attorney, Agent, or Firm* — Dykema Gossett PLLC

(57) **ABSTRACT**

Apparatus for generating an organ timing signal relating to an inspected organ within the body of a patient, including a medical positioning system, and a processor. The medical positioning system includes at least one reference electromagnetic transducer placed at a reference location, at least one inner electromagnetic transducer attached to a surgical tool inserted in a blood vessel in the vicinity of the inspected organ, and a medical positioning system processor coupled with the transducers. The medical positioning system processor generates medical positioning system data sets, each of which includes a collection of three-dimensional position coordinate readings demonstrating the motion trajectory of the surgical tool over time, the processor generating the organ timing signal from the data sets by detecting and identifying periodic motion frequencies in the data sets, and filtering the periodic motion frequencies from the data sets.

**63 Claims, 10 Drawing Sheets**

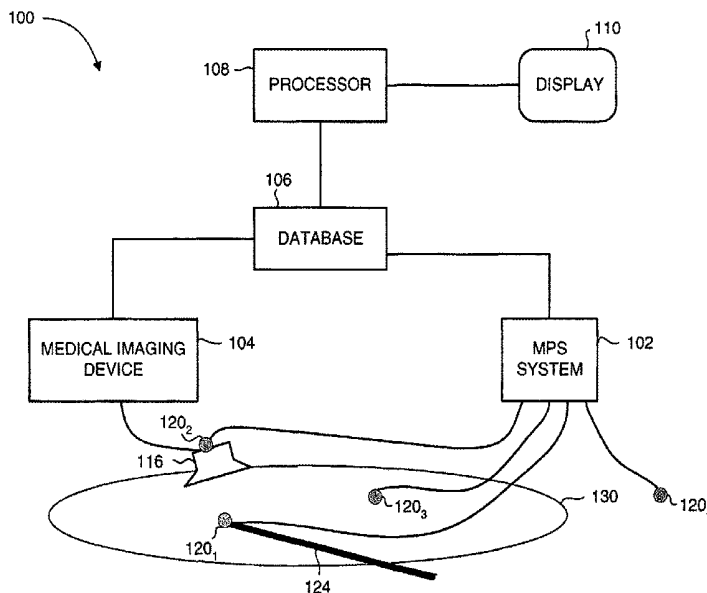

**Related U.S. Application Data**

of application No. 09/949,160, filed on Sep. 7, 2001, now Pat. No. 7,343,195, which is a continuation-in-part of application No. 09/782,528, filed on Feb. 13, 2001, now Pat. No. 7,386,339, which is a continuation-in-part of application No. 09/314,474, filed on May 18, 1999, now Pat. No. 6,233,476.

(51) **Int. Cl.**

- A61B 5/06* (2006.01)
- A61B 8/02* (2006.01)
- A61B 5/0456* (2006.01)
- A61B 5/08* (2006.01)
- A61B 5/00* (2006.01)
- A61B 6/12* (2006.01)
- A61B 6/00* (2006.01)
- A61B 8/08* (2006.01)
- A61B 8/00* (2006.01)
- A61B 17/00* (2006.01)
- A61N 5/10* (2006.01)

(52) **U.S. Cl.**

- CPC ..... *A61B 5/7289* (2013.01); *A61B 6/527* (2013.01); *A61B 6/541* (2013.01); *A61B 6/547* (2013.01); *A61B 8/02* (2013.01); *A61B 8/0841* (2013.01); *A61B 8/5276* (2013.01); *A61B 34/20* (2016.02); *A61B 90/36* (2016.02); *A61B 5/0456* (2013.01); *A61B 5/0816* (2013.01); *A61B 5/11* (2013.01); *A61B 5/721* (2013.01); *A61B 6/12* (2013.01); *A61B 6/503* (2013.01); *A61B 6/504* (2013.01); *A61B 8/0833* (2013.01); *A61B 8/0883* (2013.01); *A61B 8/0891* (2013.01); *A61B 8/4245* (2013.01); *A61B 8/4254* (2013.01); *A61B 34/10* (2016.02); *A61B 34/25* (2016.02); *A61B 90/10* (2016.02); *A61B 2017/00699* (2013.01); *A61B 2017/00703* (2013.01); *A61B 2034/105* (2016.02); *A61B 2034/107* (2016.02); *A61B 2034/2051* (2016.02); *A61B 2034/2055* (2016.02); *A61B 2034/2072* (2016.02); *A61B 2034/256* (2016.02); *A61B 2090/364* (2016.02); *A61B 2090/365* (2016.02); *A61B 2090/367* (2016.02); *A61B 2090/378* (2016.02); *A61B 2090/3958* (2016.02); *A61B 2505/05* (2013.01); *A61N 5/1067* (2013.01)

(58) **Field of Classification Search**

- CPC ..... *A61B 8/02*; *A61B 8/0841*; *A61B 8/5276*; *A61B 5/7207*; *A61B 90/36*; *A61B 5/06*; *A61B 5/0456*; *A61B 5/0816*; *A61B 5/11*; *A61B 5/721*; *A61B 6/12*; *A61B 6/503*; *A61B 6/504*; *A61B 8/00*
- USPC ..... 600/407, 424, 426, 437, 439; 128/898–899, 916
- See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 3,990,296 A 11/1976 Erikson
- 4,398,540 A \* 8/1983 Takemura et al. .... 600/441
- 4,737,794 A 4/1988 Jones
- 4,794,931 A 1/1989 Yock
- 5,016,642 A 5/1991 Dukes et al.
- 5,152,290 A 10/1992 Freeland
- 5,159,931 A 11/1992 Pini
- 5,318,025 A \* 6/1994 Dumoulin et al. .... 600/417
- 5,360,008 A \* 11/1994 Campbell, Jr. .... 600/484

- 5,398,691 A 3/1995 Martin
- 5,445,150 A 8/1995 Dumoulin et al.
- 5,453,686 A 9/1995 Anderson
- 5,529,070 A 6/1996 Augustine et al.
- 5,540,928 A 7/1996 Edelman et al.
- 5,577,502 A \* 11/1996 Darrow et al. .... 600/426
- 5,588,432 A 12/1996 Crowley et al.
- 5,622,174 A 4/1997 Yamazaki
- 5,638,819 A 6/1997 Manwaring et al.
- 5,646,525 A \* 7/1997 Gilboa ..... 324/207.17
- 5,669,385 A \* 9/1997 Pesque et al. .... 600/453
- 5,690,113 A 11/1997 Sliwa et al.
- 5,704,361 A 1/1998 Seward et al.
- 5,724,982 A 3/1998 Schnurer et al.
- 5,729,129 A 3/1998 Acker
- 5,730,129 A 3/1998 Darrow et al.
- 5,740,808 A 4/1998 Panescu et al.
- 5,744,953 A 4/1998 Hansen
- 5,752,513 A 5/1998 Acker et al.
- 5,787,889 A 8/1998 Edwards et al.
- 5,797,849 A 8/1998 Vesely et al.
- 5,806,521 A 9/1998 Morimoto et al.
- 5,810,008 A 9/1998 Dekel et al.
- 5,823,958 A 10/1998 Truppe
- 5,830,145 A 11/1998 Tenhoff
- 5,830,222 A 11/1998 Makower
- 5,833,608 A 11/1998 Acker
- 5,840,025 A 11/1998 Ben-Haim
- 5,846,200 A 12/1998 Schwartz
- 5,899,860 A \* 5/1999 Pfeiffer et al. .... 600/424
- 5,906,578 A 5/1999 Rajan et al.
- 5,913,820 A 6/1999 Bladen et al.
- 5,921,934 A 7/1999 Teo
- 5,924,989 A \* 7/1999 Polz ..... 600/443
- 5,928,248 A \* 7/1999 Acker ..... 623/1.11
- 5,935,075 A 8/1999 Casscells et al.
- 5,938,606 A \* 8/1999 Bonnefous ..... 600/437
- 5,949,491 A 9/1999 Callahan et al.
- 5,955,879 A 9/1999 Durdle et al.
- 5,957,844 A \* 9/1999 Dekel et al. .... 600/439
- 5,967,980 A \* 10/1999 Ferre et al. .... 600/424
- 5,976,088 A 11/1999 Urbano et al.
- 5,993,390 A 11/1999 Savord et al.
- 5,994,690 A 11/1999 Kulkarni et al.
- 6,006,126 A \* 12/1999 Cosman ..... 600/426
- 6,016,439 A 1/2000 Acker
- 6,030,343 A 2/2000 Chechersky et al.
- 6,035,856 A 3/2000 LaFontaine et al.
- 6,047,080 A 4/2000 Chen et al.
- 6,134,003 A 10/2000 Tearney et al.
- 6,148,095 A 11/2000 Prause et al.
- 6,152,878 A 11/2000 Nachatomy et al.
- 6,161,032 A \* 12/2000 Acker ..... 600/424
- 6,167,296 A 12/2000 Shahidi
- 6,169,917 B1 1/2001 Masotti et al.
- 6,175,669 B1 1/2001 Colston et al.
- 6,185,271 B1 \* 2/2001 Kinsinger ..... 378/19
- 6,195,450 B1 2/2001 Qian et al.
- 6,210,168 B1 4/2001 Aiger et al.
- 6,213,945 B1 4/2001 Tynan et al.
- 6,216,029 B1 4/2001 Paltieli
- 6,228,028 B1 5/2001 Klein et al.
- 6,233,476 B1 5/2001 Strommer et al.
- 6,246,898 B1 \* 6/2001 Vesely et al. .... 600/424
- 6,261,247 B1 7/2001 Ishikawa et al.
- 6,275,724 B1 8/2001 Dickinson et al.
- 6,317,621 B1 11/2001 Graumann et al.
- 6,321,109 B2 11/2001 Ben-Haim et al.
- 6,344,863 B1 2/2002 Capelli et al.
- 6,368,285 B1 4/2002 Osadchy et al.
- 6,381,350 B1 4/2002 Klingsmith et al.
- 6,385,476 B1 5/2002 Osadchy et al.
- 6,390,982 B1 5/2002 Bova et al.
- 6,405,072 B1 6/2002 Cosman et al.
- 6,416,476 B1 7/2002 Ogasawara et al.
- 6,423,009 B1 7/2002 Downey et al.
- 6,432,041 B1 8/2002 Taniguchi et al.
- 6,470,207 B1 10/2002 Simon et al.
- 6,498,944 B1 12/2002 Ben-Haim et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,501,981	B1	12/2002	Schweikard et al.	
6,546,271	B1	4/2003	Reisfeld	
6,556,695	B1	4/2003	Packer et al.	
6,587,707	B2	7/2003	Nehrke et al.	
6,589,163	B2	7/2003	Aizawa et al.	
6,626,902	B1	9/2003	Kucharczyk et al.	
6,671,538	B1	12/2003	Ehnholm et al.	
6,730,030	B2	5/2004	Palti	
6,733,458	B1	5/2004	Steins et al.	
6,773,393	B1	8/2004	Taniguchi et al.	
6,775,404	B1*	8/2004	Pagoulatos et al. ....	382/154
6,788,967	B2	9/2004	Ben-Haim et al.	
6,895,267	B2*	5/2005	Panescu et al. ....	600/424
6,917,827	B2	7/2005	Kienzle, III	
7,007,699	B2*	3/2006	Martinelli et al. ....	128/899
7,156,655	B2	1/2007	Sachdeva et al.	
7,159,592	B1	1/2007	Makower et al.	
7,195,587	B2	3/2007	Taniguchi et al.	
7,197,354	B2	3/2007	Sobe	
7,235,084	B2	6/2007	Skakoon et al.	
7,263,397	B2	8/2007	Hauck et al.	
7,343,195	B2	3/2008	Strommer et al.	
7,386,339	B2	6/2008	Strommer et al.	
7,398,116	B2*	7/2008	Edwards .....	600/424
7,527,597	B2	5/2009	Sandlen et al.	
7,739,090	B2	6/2010	Charbel et al.	
7,778,688	B2	8/2010	Strommer	
7,881,769	B2	2/2011	Sobe	
8,126,534	B2	2/2012	Maschke	
8,332,013	B2	12/2012	Strommer	
8,442,618	B2	5/2013	Strommer et al.	
2001/0031919	A1	10/2001	Strommer et al.	
2001/0044578	A1	11/2001	Ben-Haim et al.	
2002/0007124	A1*	1/2002	Woodward .....	600/481
2002/0049375	A1	4/2002	Strommer et al.	
2002/0049735	A1	4/2002	Matsumoto et al.	
2002/0193686	A1*	12/2002	Gilboa .....	600/424
2003/0074011	A1	4/2003	Gilboa et al.	
2003/0190064	A1	10/2003	Inoue	
2004/0034297	A1	2/2004	Darrow et al.	
2004/0097804	A1	5/2004	Sobe	
2004/0116775	A1	6/2004	Taniguchi et al.	
2004/0116813	A1	6/2004	Selzer et al.	
2004/0138548	A1*	7/2004	Strommer et al. ....	600/407
2004/0215071	A1	10/2004	Frank et al.	
2005/0033149	A1	2/2005	Strommer et al.	
2005/0049493	A1*	3/2005	Kerby et al. ....	600/437
2005/0107668	A1	5/2005	Smith	
2005/0107688	A1	5/2005	Strommer et al.	
2005/0129176	A1	6/2005	Kokubun et al.	
2005/0197557	A1	9/2005	Strommer et al.	
2005/0197566	A1	9/2005	Strommer et al.	
2006/0058647	A1	3/2006	Strommer et al.	
2006/0064006	A1	3/2006	Strommer et al.	
2006/0079745	A1	4/2006	Viswanathan	
2006/0089706	A1	4/2006	Plaia et al.	
2007/0287901	A1	12/2007	Strommer et al.	
2008/0175463	A1	7/2008	Strommer et al.	

2008/0221440	A1	9/2008	Iddan et al.
2008/0221442	A1	9/2008	Tolkowsky et al.
2009/0182224	A1	7/2009	Shmarak et al.
2010/0331950	A1	12/2010	Strommer
2011/0230758	A1	9/2011	Eichler

## FOREIGN PATENT DOCUMENTS

EP	1005835	6/2000
EP	1 088 515 A1	4/2001
JP	62032304	2/1987
JP	8500441	1/1996
JP	11110114	4/1999
JP	1999151246	6/1999
JP	11197159	7/1999
JP	2000023964	1/2000
JP	2000166927	6/2000
JP	2000279425	10/2000
JP	2001170027	6/2001
JP	2002200058	7/2002
JP	2003520062	7/2003
JP	2004533863	11/2004
JP	2007502187	2/2007
JP	2010507104	3/2010
JP	4701179	6/2011
WO	94/04938	3/1994
WO	WO-96/05768	2/1996
WO	96/41119	12/1996
WO	WO-96/41119	12/1996
WO	97/29682	8/1997
WO	WO-97/29685	8/1997
WO	WO-97/36143	10/1997
WO	98/11524	3/1998
WO	99/00052	1/1999
WO	99/43253	9/1999
WO	00/10456	3/2000
WO	00/16684	3/2000
WO	0069335	11/2000
WO	02-064011 A2	8/2002
WO	03059167	7/2003
WO	2004062501	7/2004
WO	WO-2004/060157	7/2004
WO	2004103174	12/2004
WO	WO-2005/039391	5/2005
WO	2008047992	4/2008

## OTHER PUBLICATIONS

Panza, Julio A. , "Real-time three-dimensional echocardiography: An overview", *The International Journal of Cardiovascular Imaging* 17:227-235, 2001.

Author: Panza, Julio A Title: Real-time three-dimensional echocardiography: An overview Citation: The International Journal of Cardiovascular Imaging 17:227-235, 2001.

Solomon, et al., "Real-time Bonchoscope Tip Localization Enables Three-dimensional CT Image Guidance for Transbronchial Needle Aspiration in Swine". *Laboratory and Animal Investigation*, vol. 114, Issue 5, Nov. 1998, pp. 105-1410.

\* cited by examiner

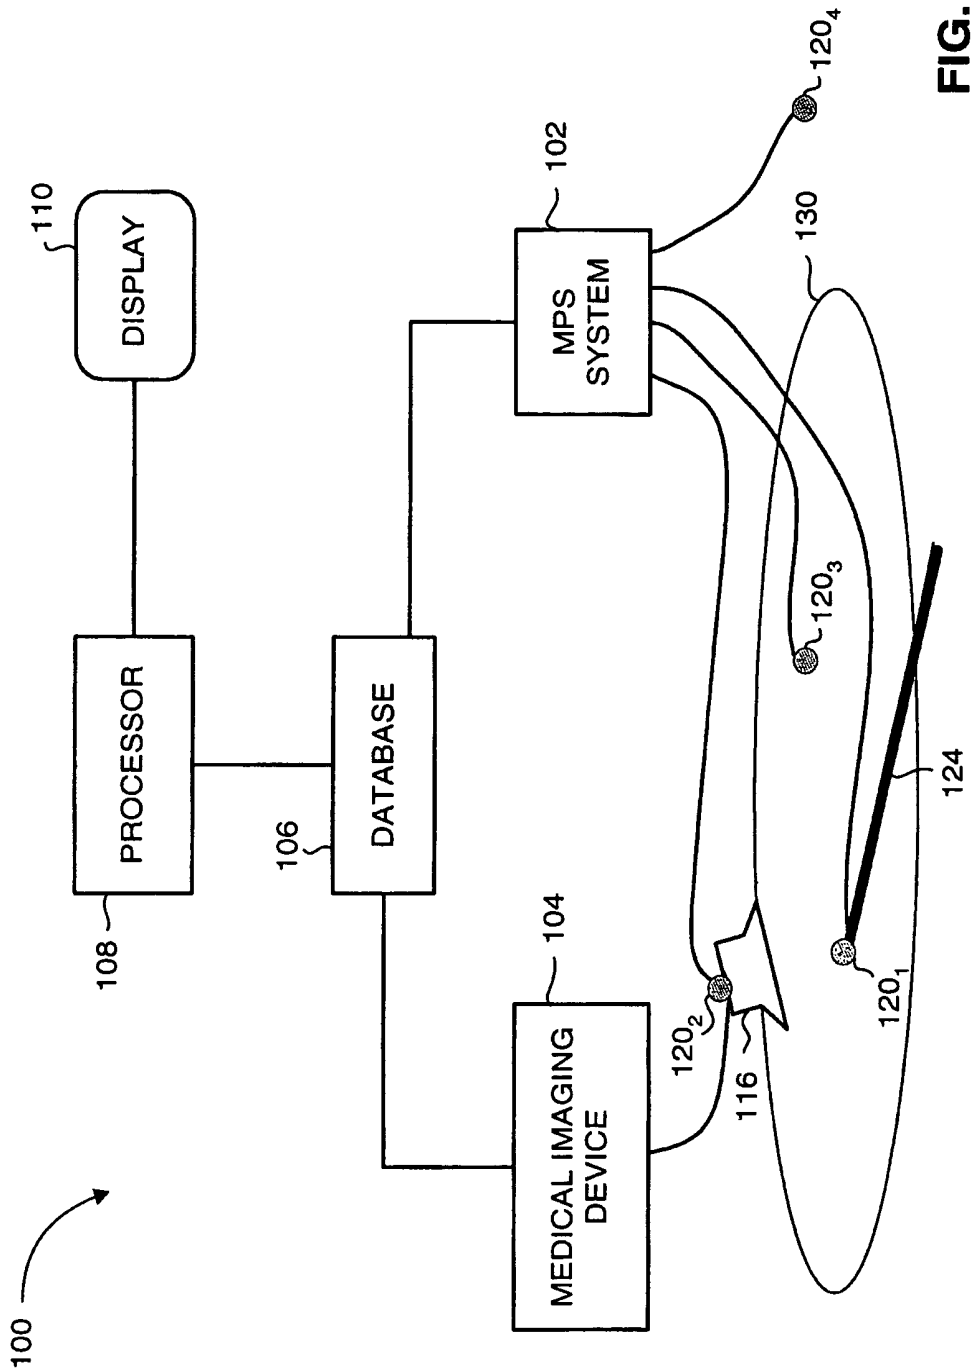


FIG. 1



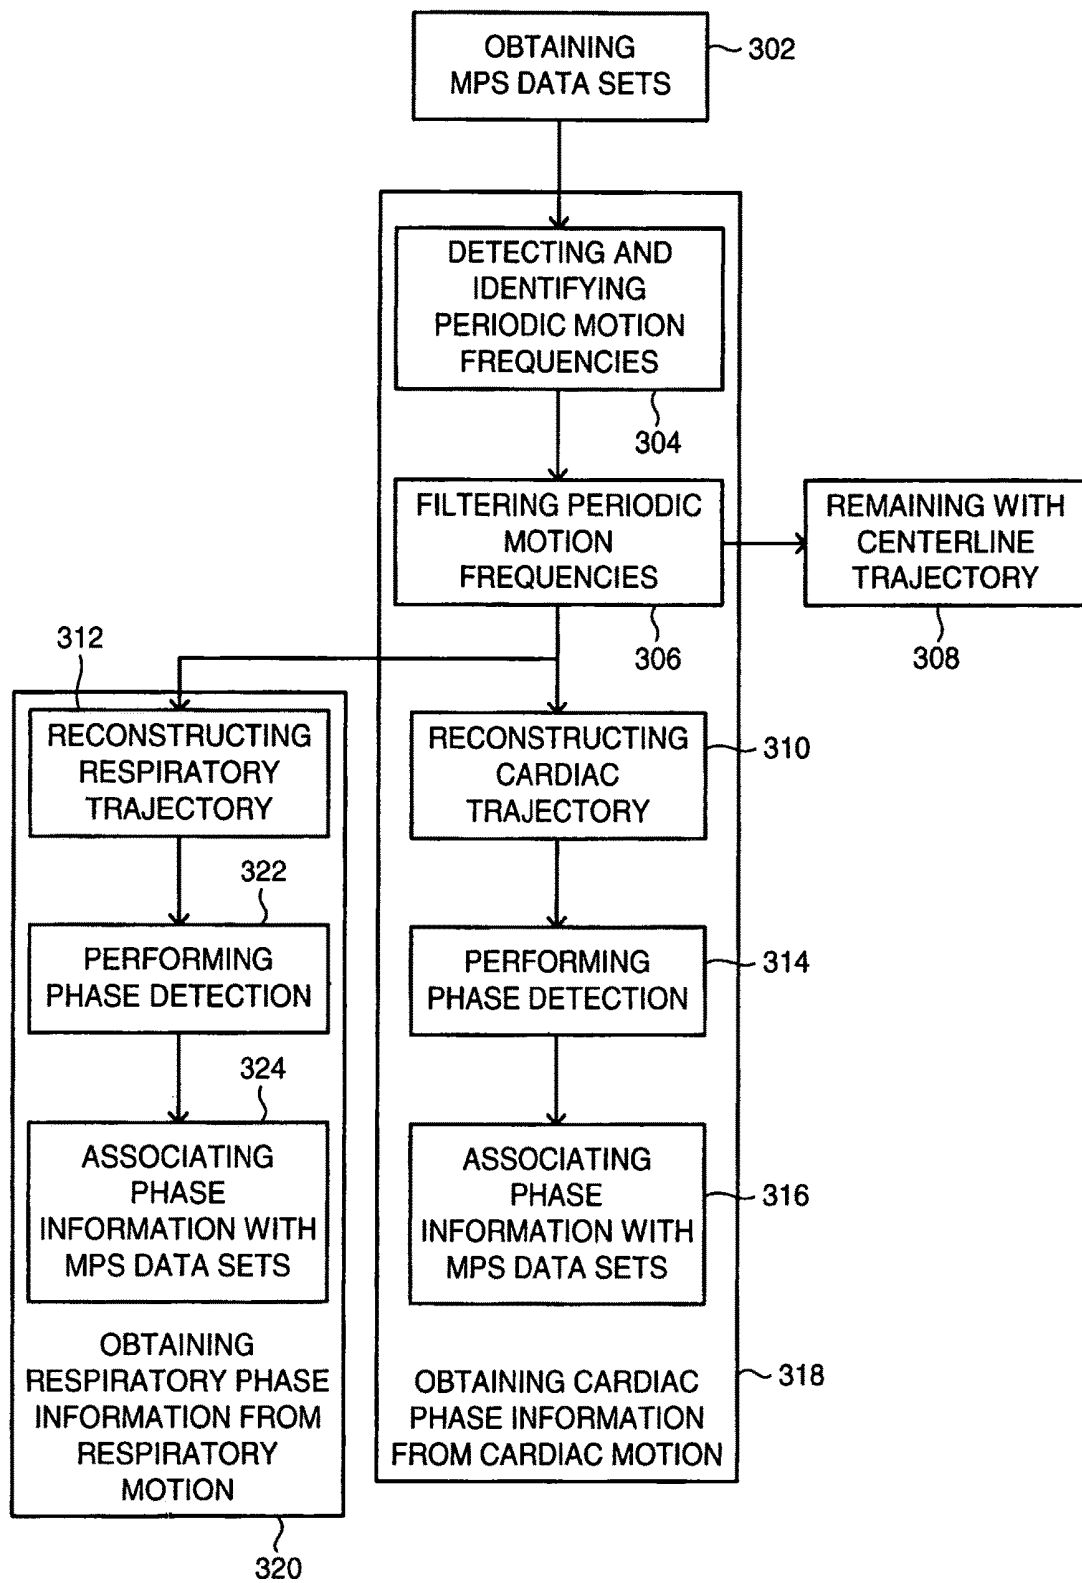


FIG. 3

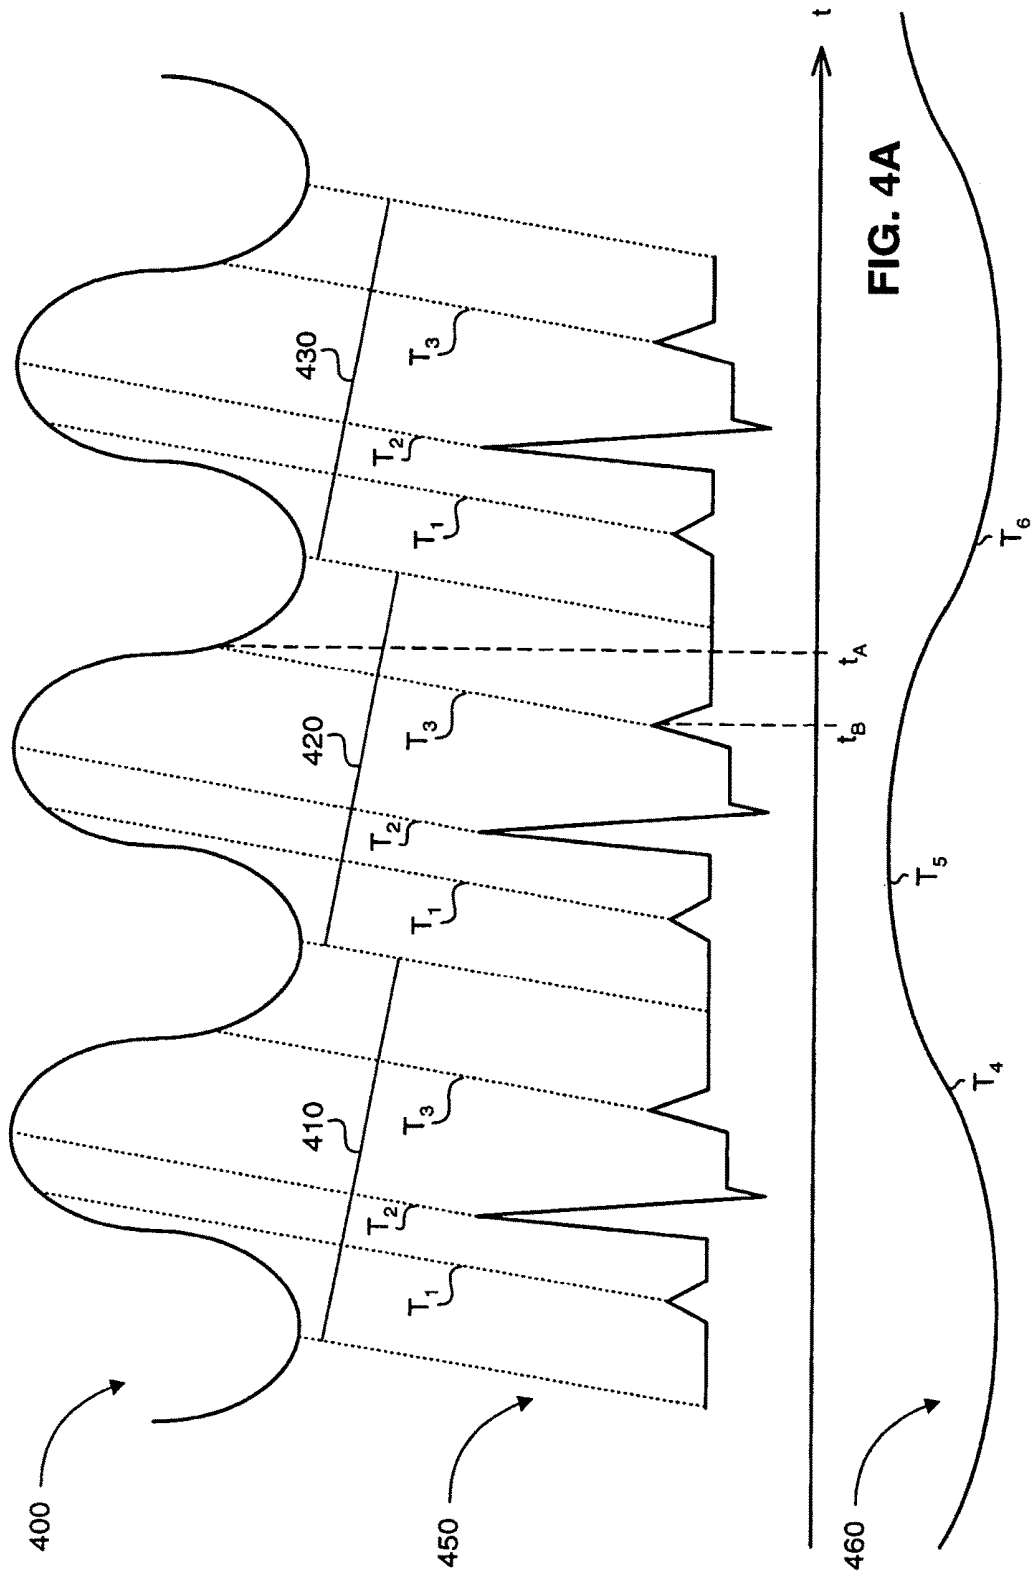


FIG. 4A

FIG. 4B

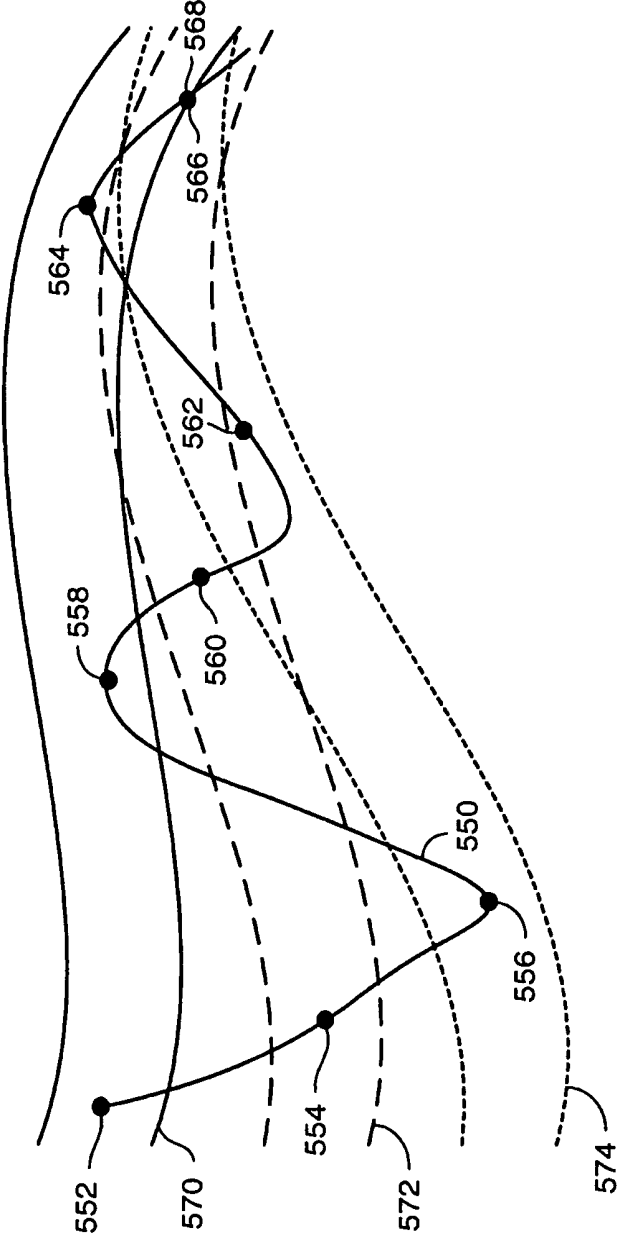


FIG. 5

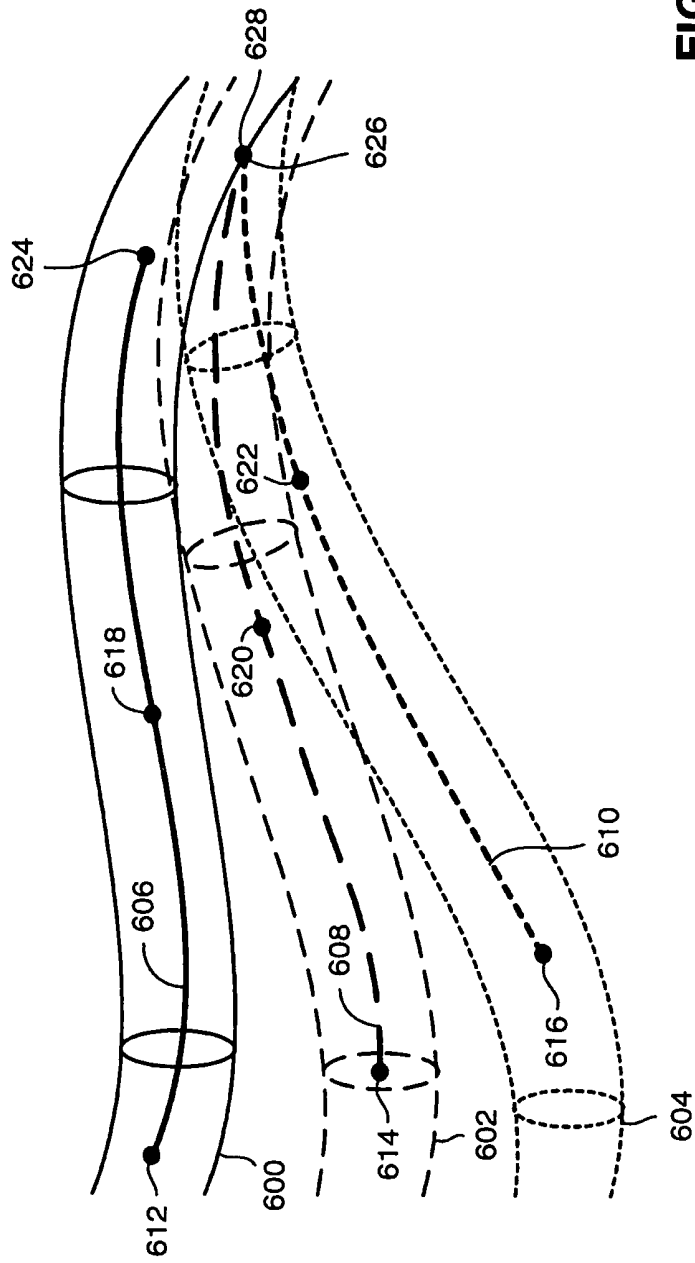


FIG. 6

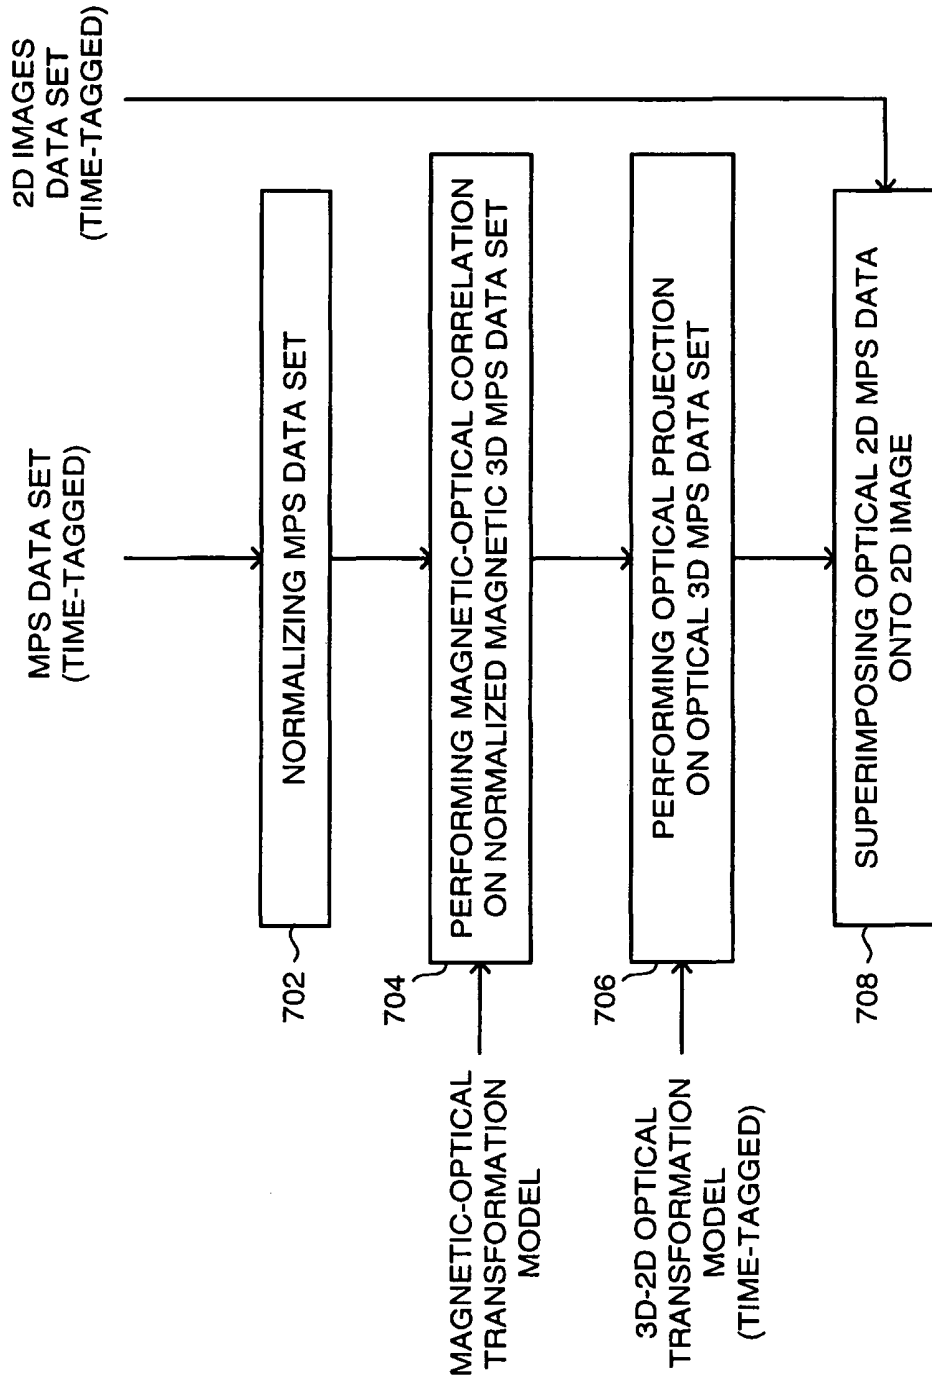


FIG. 7

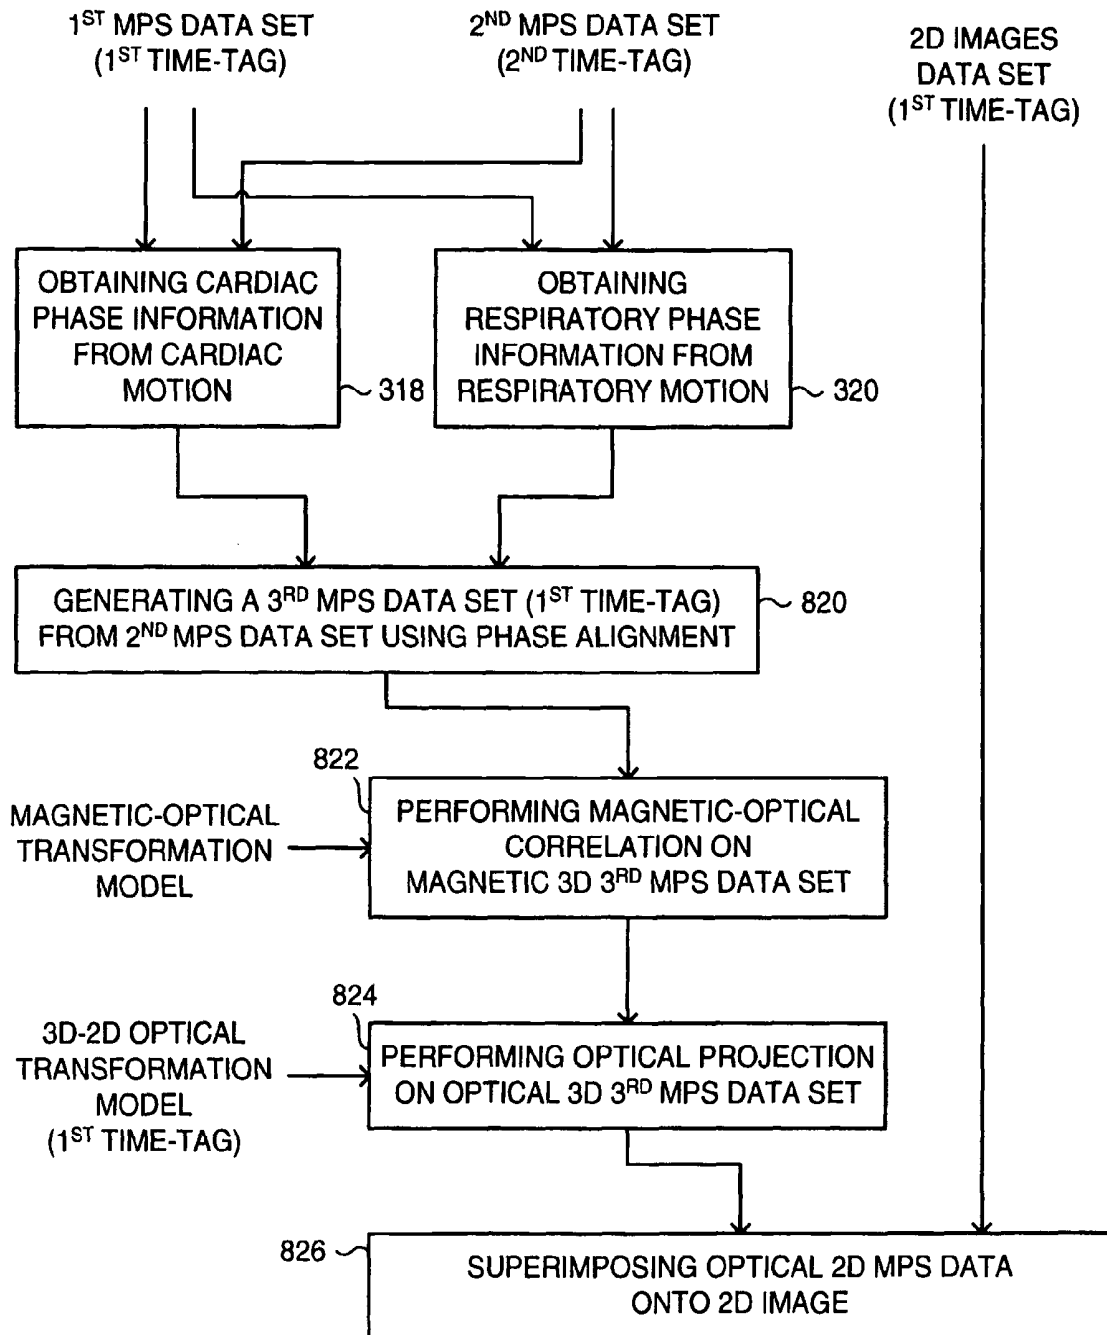


FIG. 8

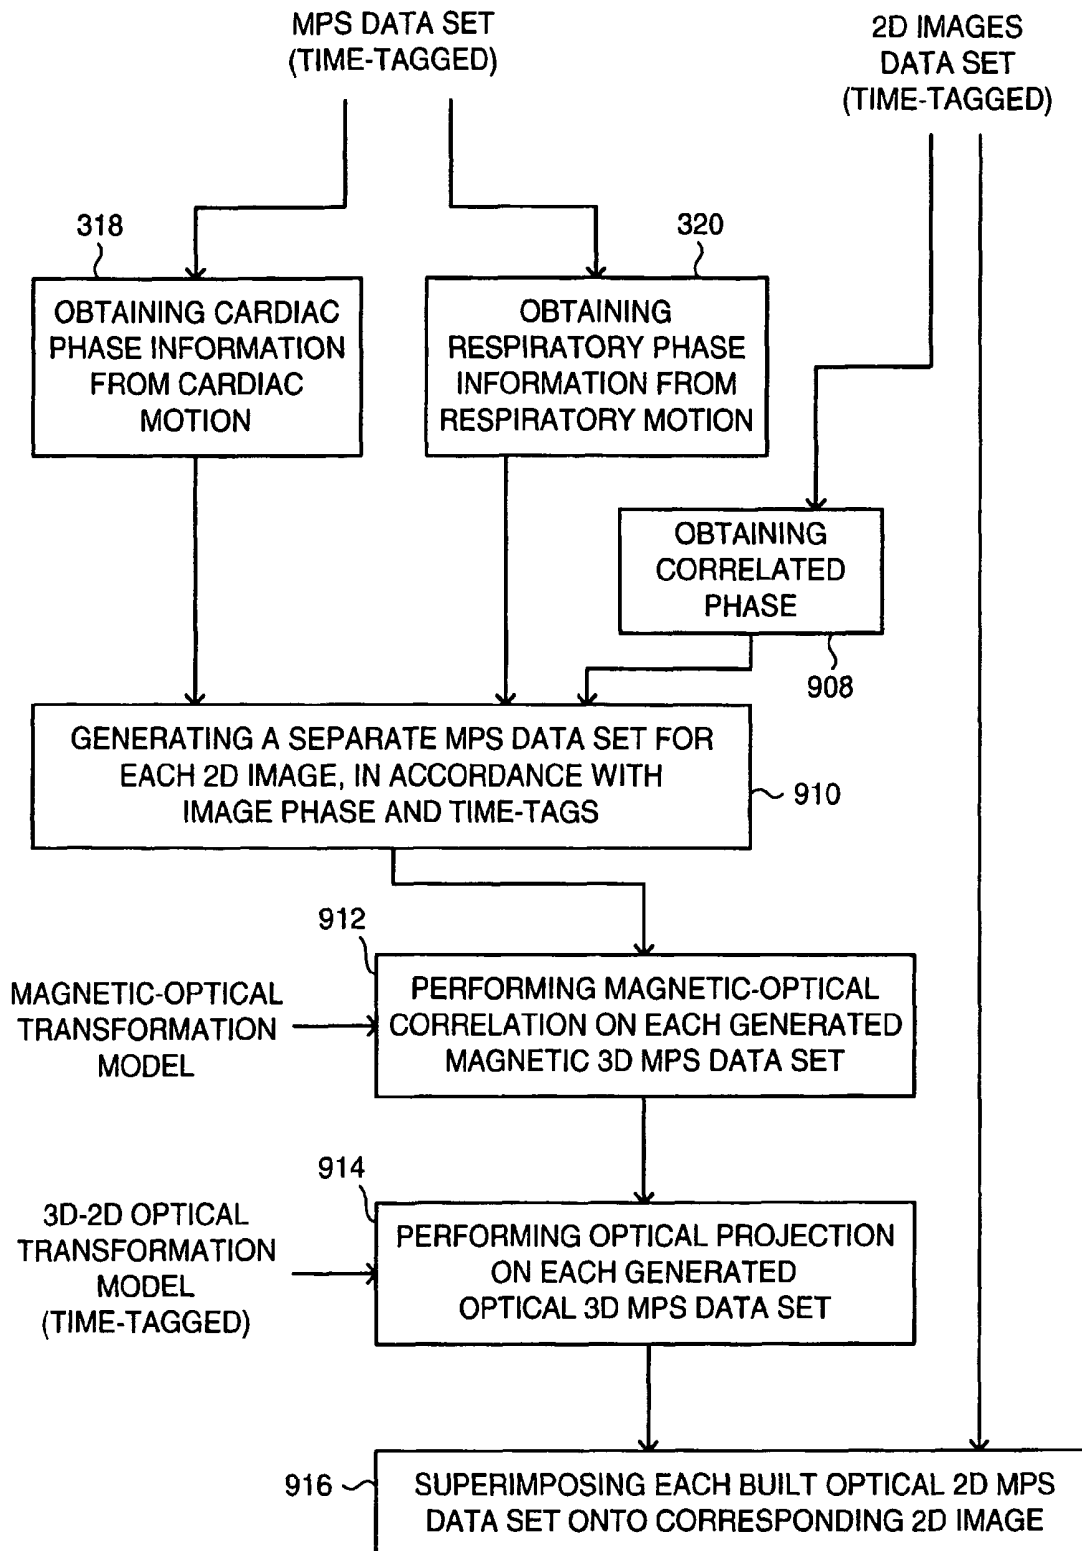


FIG. 9

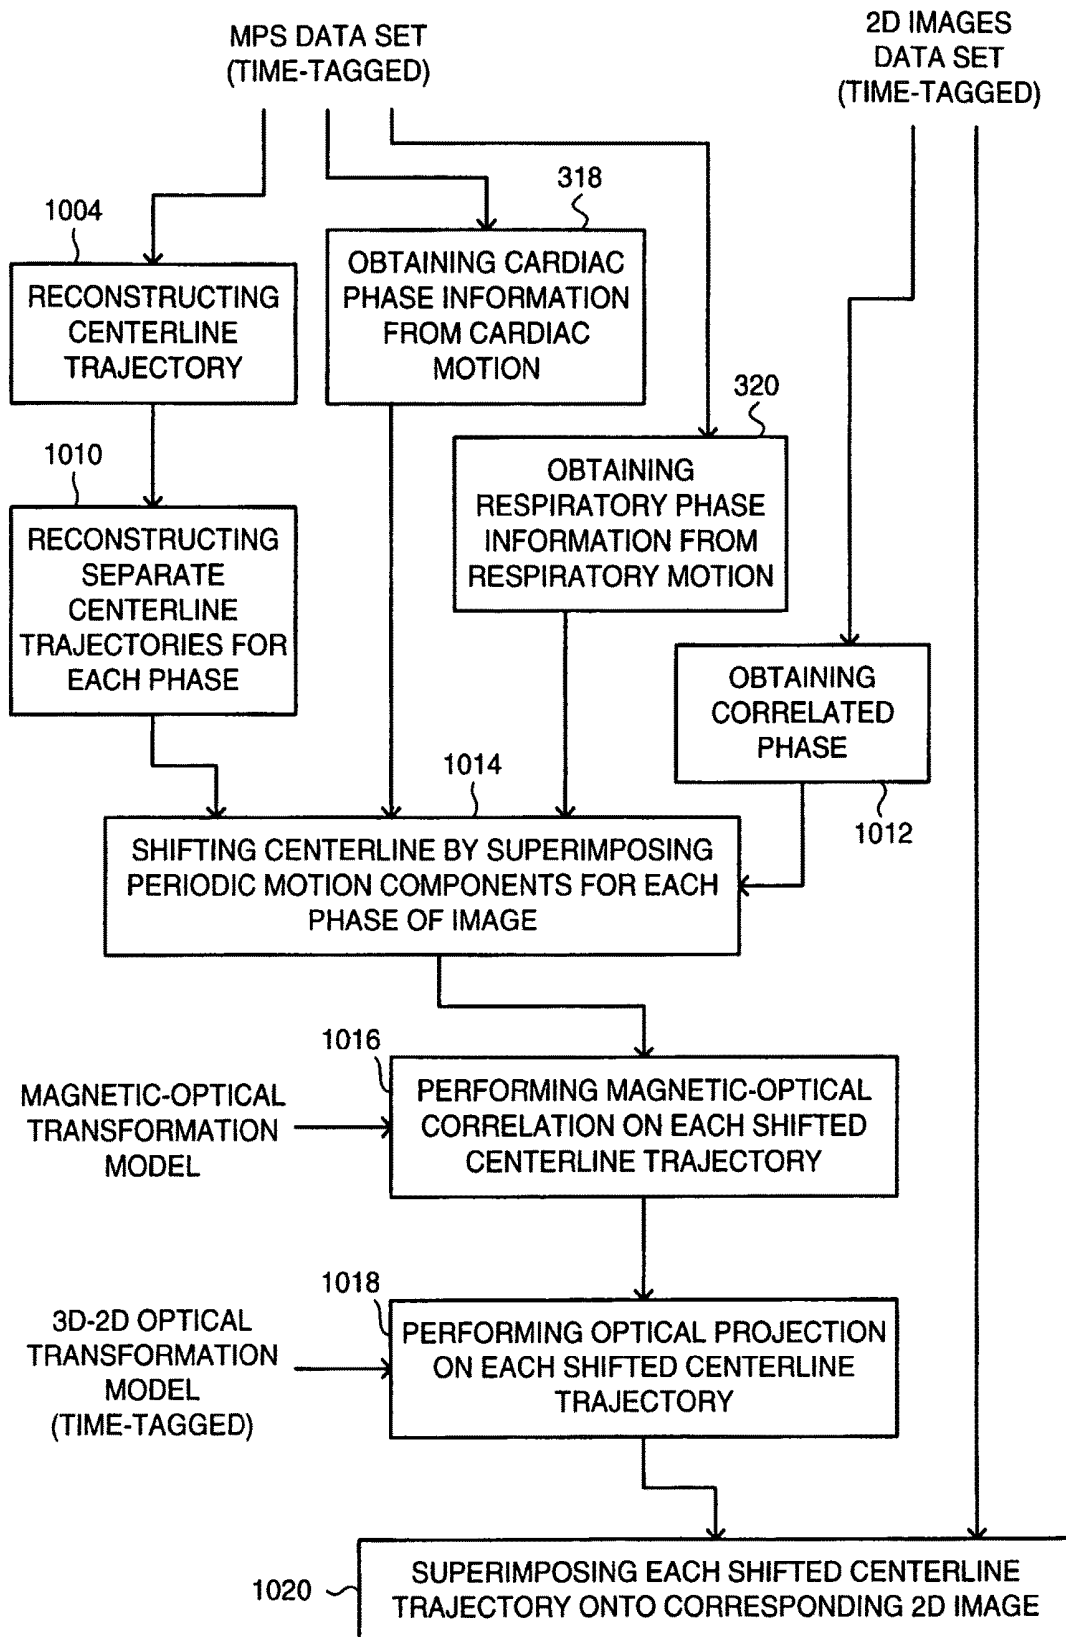


FIG. 10

**METHOD AND APPARATUS FOR INVASIVE  
DEVICE TRACKING USING ORGAN  
TIMING SIGNAL GENERATED FROM MPS  
SENSORS**

FIELD OF THE DISCLOSED TECHNIQUE

The disclosed technique relates to medical diagnostics and surgery systems and methods in general, and to a method and system for monitoring organ phases in three-dimensional medical imaging and navigation, in particular.

BACKGROUND OF THE DISCLOSED  
TECHNIQUE

Medical imaging is a powerful tool to assist in the performance of various types of medical operations, and to enhance diagnostics and other decisions concerning a medical procedure. Several systems are known in the art to produce real-time medical images via a variety of different imaging modalities. In instances of imaging of anatomical structures that involve periodic motion or cyclic phases, the imaging system may encompass a timing element to take this into account. Monitoring devices, such as an electrocardiogram (ECG) machine, are regularly incorporated into medical imaging systems to provide timing information for registering the captured images with respect to organ phase. Typically, the timing information obtained from such monitoring devices is not completely accurate. As well, the signal received from such monitoring devices involves a delay, and is not obtained in real-time with respect to the actual organ motion. Finally, an external monitoring device adds a cumbersome element to an already complex system.

U.S. Pat. No. 5,577,502 to Darrow et al entitled "Imaging of interventional devices during medical procedures", is directed to a method for compensation of subject motion during tracking of an invasive device within the body of the subject. A device tracking unit determines the location of the invasive device relative to a fixed reference point. An imaging device acquires a reference image of the subject. A position detection means placed within the imaging device measures the location over time of a reference point of the subject. Each acquired image is stored together with the corresponding location of subject reference point. A subject tracking unit receives location information over time from position detection means, and computes translation and rotation movement of the subject from time of image acquisition to time of device location measurement. A registration unit receives the reference image, the net position and orientation change of the subject, and the device location. The registration unit translates and rotates the reference image to match the position and orientation of subject at the time of device location measurement. An image of the device is superimposed upon the translated/rotated image of the subject at its absolute position and orientation. The registration unit may also adjust the displayed location of the device, rather than the display of the image.

In addition to translation and rotation motion, the registration unit accounts for expansion and contraction of the subject, occurring due to a periodic motion cycle, such as the respiratory or cardiac cycles. Position detection means measures the change in the subject due to expansion and contraction, and feeds this information to the registration unit. The registration unit distorts the reference image in accordance with the expansion and contraction, and subse-

quent translation and rotation, thereby dynamically registering the image of the subject with the current device location.

Alternatively, the imaging device may monitor subject motion by obtaining subsequent projections of the subject and then detecting offset and cross-sectional size of the subject in these images. Further alternatively, a series of reference images are each gated to the periodic motion cycle. The imaging device acquires a series of images at different times within the cardiac cycle, as measured by an ECG signal. An ECG provides a signal for each measurement of device location. At a given time, an image from the series which corresponds to the ECG signal is selected as the reference image. The registration unit translates and rotates this reference image, with respect to the information received from the subject tracking unit for that time. A representation of the measured location of the device is superimposed upon the updated image, resulting in a registered image of the subject and the invasive device.

U.S. Pat. No. 5,622,174 to Yamazaki entitled "Ultrasonic diagnostic apparatus and image displaying system", is directed to a system for determining movement velocities of a moving internal organ and providing a color display of the movement velocities over time. An ultrasonic probe transmits an ultrasound beam toward the heart. The transmitted ultrasonic beam is partially reflected by tissues of the heart as an echo signal and returned to the probe. The echo signal has a Doppler shift in frequency due to the Doppler effect. The echo signal is transduced into a voltage signal and supplied to a reception signal processor. The signal is beam-formed, detected and output to a B-mode digital scan converter (DSC). The B-mode DSC converts the image data of the signal to standard television scanning data, which is sent to an image synthesizer. The B-mode DSC also stores a plurality of image data at arbitrary cardiac timing in a B-mode frame memory.

The reception signal processor also sends the transduced echo signal to a phase detector. The phase detector performs phase detection on the Doppler shift frequency to extract the Doppler shift signal. A low pass filter filters out unnecessary Doppler signals resulting from valve motion or blood flow, leaving only the Doppler signal from the cardiac muscle. A frequency analyzer calculates physical values relating to the velocities at each sampling volume of a scan plane, using the Fast Fourier Transform (FFT) or auto-correlation method. These values include mean Doppler frequencies (corresponding to mean velocities of movement of the organ), variance (turbulence factors of Doppler spectrum), and maximum values of Doppler shift frequencies (maximum velocities of organ movement at sampling volume). These values are sent as color Doppler information to a vector-velocity calculator, which calculates the absolute movement velocities of the organ at each sampling volume point. A display presents the magnitude and/or direction of velocities, in accordance with a color scheme assignment. It is noted that detected ECG signals of the heart are used to trigger the signal generator (output reference pulses for transmission/reception of ultrasonic beams). In addition, these cardiac timing signals are used to produce a real-time image displaying changes in movement velocities of the heart in color.

U.S. Pat. No. 6,246,898 to Vesely et al entitled "Method for carrying out a medical procedure using a three-dimensional imaging and tracking system", is directed to a method for performing an in-vivo medical procedure on an associated body using three-dimensional tracking and imaging. A plurality of transceivers is used to track the three-dimensional motion of an object under investigation. At least four

transceivers are implanted within a specimen in whom distances are to be measured. Three transceivers lie in a (x,y) plane and act as a reference. The fourth transceiver determines the z-coordinates of surrounding transducers by determining if an active one of the transducers lies above or below the reference plane established by the three transceivers. Each of a plurality of transmitters attached to the specimen at various locations is sequentially fired, while the three reference transceivers record the receiver signals. Since the difference from each transmitter to the reference plane is known, the relative x,y,z coordinates of the transmitters can be determined using triangulation.

The video display is synchronized with the real-time patient heart beat using an ECG signal. An Analog-to-Digital (A/D) converter converts the ECG signal into digital data. A sync generator module produces a timing signal corresponding to the current heart activity from the digital ECG data. This is done by activating a memory location or input port, or generating an interrupt, at the precise time a QRS complex is identified. In particular, the sync generator module tests the data signal for large rates of change, zero crossings, and other information allowing the sync generator module to reveal the QRS complex of the signal

U.S. Pat. No. 6,556,695 to Packer et al entitled "Method for producing high resolution real-time images, of structure and function during medical procedures", is directed to a method for providing medical images in real-time to assist physicians in the performance of medical procedures. A Medical Resonance Imaging (MRI) system obtains a high resolution model of the heart prior to the medical procedure. Images of the heart are acquired during successive cardiac phases. A pulse generator creates a series of fast gradient echo pulse sequences. The R-R interval of the cardiac cycle is divided up into several short segments of pulse sequences, using an ECG gating signal that triggers at the peak of the R wave. A single coordinate, or view, of the heart is acquired during each fast gradient echo segment. Adjacent segments are combined into groups, and the data in each group contributes to generating an image at a different phase of the cardiac cycle. A number (e.g., fifteen) of two-dimensional slices are acquired during an entire cardiac cycle, depicting one slice through the heart at (e.g., fifteen) successive phases of the cardiac cycle. Additional slices of the heart are acquired and reconstructed into two-dimensional images. These two-dimensional slices are then combined to form (e.g., fifteen) three-dimensional image data sets.

During the medical procedure, an ultrasonic transducer acquires low-resolution image frames of the heart in real-time. An ECG signal from the patient detects the real-time cardiac phase. The stored high-resolution heart model is registered using the real-time image frames and ECG signal. The registered high-resolution model is then used to produce high-resolution, large field of view images in real-time on a display.

#### SUMMARY OF THE DISCLOSED TECHNIQUE

It is an object of the disclosed technique to provide a novel method and apparatus for intra-body navigation and invasive device tracking using an organ timing signal, which is generated without an external monitoring device.

In accordance with the disclosed technique, there is thus provided an apparatus for generating an organ timing signal relating to at least one inspected organ within the body of a patient. The apparatus includes a medical positioning system (MPS) and a processor. The processor is coupled with the MPS. The MPS includes at least one reference electromag-

netic transducer, at least one inner electromagnetic transducer, and an MPS processor. The MPS processor is coupled with the reference electromagnetic transducer and with the inner electromagnetic transducer. The inner electromagnetic transducer is attached to a surgical tool inserted in a blood vessel in the vicinity of the inspected organ. The MPS processor determines the three-dimensional position of the inner electromagnetic transducer, by processing transmitted electromagnetic signals transmitted from one of the reference electromagnetic transducer and the inner electromagnetic transducer with detected electromagnetic signals detected by the other of the reference electromagnetic transducer and the inner electromagnetic transducer. The MPS processor further generates MPS data sets. Each of the MPS data sets includes a collection of three-dimensional position coordinate readings demonstrating the motion trajectory of the surgical tool over time. The processor generates the organ timing signal from the MPS data sets by detecting and identifying periodic motion frequencies in the MPS data sets, and filtering the periodic motion frequencies from the MPS data sets.

According to the disclosed technique, there is also provided a method for generating an organ timing signal relating to an inspected organ within the body of a patient. The method includes the procedures of transmitting electromagnetic signals and detecting the electromagnetic signals, processing the transmitted electromagnetic signals with the detected electromagnetic signals, and determining the three-dimensional position of a surgical tool inserted within the body of a patient based on the processing. The method further includes the procedures of generating MPS data sets comprising a collection of three-dimensional position coordinate readings demonstrating the motion trajectory of the surgical tool over time, detecting and identifying periodic motion frequencies in the MPS data sets, and filtering the periodic motion frequencies from the MPS data sets.

#### BRIEF DESCRIPTION OF THE DRAWINGS

The disclosed technique will be understood and appreciated more fully from the following detailed description taken in conjunction with the drawings in which:

FIG. 1 is a schematic illustration of a system, constructed and operative in accordance with an embodiment of the disclosed technique;

FIG. 2 is a block diagram of a method for registering three-dimensional magnetic coordinates into two-dimensional optical coordinates, operative in accordance with another embodiment of the disclosed technique;

FIG. 3 is a block diagram of a method for obtaining phase information from MPS data sets, operative in accordance with a further embodiment of the disclosed technique;

FIG. 4A is a schematic illustration of a sample cardiac trajectory, in electrical signal representation and in mechanical signal representation;

FIG. 4B is a schematic illustration of a sample respiratory trajectory in mechanical signal representation;

FIG. 5 is a schematic illustration of a trajectory of the surgical tool of the system of FIG. 1, inside a vessel in the body of a patient, respective of different activity-states of the cardiac trajectory of FIG. 4;

FIG. 6 is a schematic illustration of trajectories of a guided surgical tool inside a vessel in the body of a patient, each trajectory processed with respect to a different activity-state;

FIG. 7 is a block diagram of a method for superimposing MPS data onto two-dimensional image data for correspond-

ing data sets, operative in accordance with another embodiment of the disclosed technique;

FIG. 8 is a block diagram of a method for superimposing MPS data onto two-dimensional image data for non-corresponding data sets, operative in accordance with a further embodiment of the disclosed technique;

FIG. 9 is a block diagram of a method for constructing trajectories of a guided surgical tool within the body of a patient, respective of different activity-states of an inspected organ, operative in accordance with another embodiment of the disclosed technique; and

FIG. 10 is a block diagram of an additional method for constructing trajectories of a guided surgical tool within the body of a patient, respective of different activity-states of an inspected organ, operative in accordance with a further embodiment of the disclosed technique.

#### DETAILED DESCRIPTION OF THE EMBODIMENTS

The disclosed technique overcomes the disadvantages of the prior art by providing methods and apparatus for intra-body navigation and invasive device tracking using an organ timing signal generated without an external monitoring device. It is noted that the terms “phase” and “activity-state” are used interchangeably herein below. According to one embodiment, phase information is generated from a sensor which concurrently provides position and orientation information. The system allows for image acquisition and playback, three-dimensional model reconstruction, intra-body navigation, and tracking an invasive device during minimally invasive surgery. These aspects are further explained in US Patent Application 2002/0049375 to Strommer et al entitled “Method and apparatus for real time quantitative three-dimensional image reconstruction of a moving organ and intra-body navigation”, which is hereby incorporated by reference. Also, the system can be used to optimally advise on the type and dimensions of surgical tool to insert, where the surgical tool should be inserted, and other decisions related to a surgical procedure.

Reference is now made to FIG. 1, which is a schematic illustration of a system, generally referenced 100, constructed and operative in accordance with an embodiment of the disclosed technique.

System 100 includes a Medical Positioning System (MPS) 102, a medical imaging device 104, a database 106, a processor 108, a display 110, an image detector 116, a plurality of MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub>, and 120<sub>4</sub>, and a surgical tool 124. MPS 102 and medical imaging device 104 are coupled with database 106. Processor 108 is coupled with database 106 and display 110. MPS 102 includes plurality of MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub>, and 120<sub>4</sub>. Medical imaging device 104 includes image detector 116.

MPS 102 receives and processes data related to the position of an area of the body of a patient. It is noted that henceforth the term “position” refers to either the location or positional coordinate of a point in space, the orientation of that point in space, or both. The data is obtained via plurality of MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub>, and 120<sub>4</sub>. MPS sensor 120<sub>1</sub> is attached to surgical tool 124. MPS sensor 120<sub>2</sub> is attached to image detector 116. MPS sensor 120<sub>3</sub> is generally attached to an inspected area of a patient body (referenced 130). MPS sensor 120<sub>4</sub> is generally attached to a known area on the surface on which the patient rests.

Each of MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub>, and 120<sub>4</sub> contain electromagnetic field detection elements, such as coils. MPS 102 produces predetermined electromagnetic fields, which

are detected by MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub>, and 120<sub>4</sub>, respectively. MPS 102 processes the detected electromagnetic fields, and obtains an indication of the three-dimensional position of MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub>, and 120<sub>4</sub>. In this manner, MPS 102 determines the three-dimensional position of image detector 116, surgical tool 124, a selected area of patient body 130, and a known area on the surface on which the patient rests. It is noted that the electromagnetic transmission may be reversed, such that the field detection elements are stationary and located in MPS 102 while predetermined electromagnetic fields are produced by MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub>, and 120<sub>4</sub>. A medical positioning system such as MPS 102 is explained further in U.S. Pat. No. 6,233,476 to Strommer et al entitled “Medical positioning system”, which is hereby incorporated by reference.

In one embodiment of the disclosed technique, each of MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub>, and 120<sub>4</sub> may be an electromagnetic transducer, capable of both transmitting an electromagnetic field and detecting an electromagnetic field. In addition, MPS 102 contains at least one reference electromagnetic transducer (not shown) which is placed at a certain reference location. The reference electromagnetic transducer may be one of MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub>, and 120<sub>4</sub>. MPS 102 further contains an MPS processor (not shown) coupled with the reference electromagnetic transducer and each of the other electromagnetic transducers. The reference transducer then transmits predetermined electromagnetic signals in the form of electromagnetic fields, which are detected by MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub>, and 120<sub>4</sub>, respectively. Alternatively, the electromagnetic transmission is reversed, such that predetermined electromagnetic signals are transmitted by MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub>, and 120<sub>4</sub>, respectively, and are detected by the reference transducer. The MPS processor processes the detected electromagnetic signals, and obtains an indication of the three-dimensional position of MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub>, and 120<sub>4</sub>. In this manner, MPS 102 determines the three-dimensional position of image detector 116, surgical tool 124, a selected area of patient body 130, and a known area on the surface on which the patient rests.

The position of image detector 116, obtained via MPS sensor 120<sub>2</sub>, is used in determining parameters (i.e., external optical parameters) relating to medical imaging device 104. It is noted that the parameters relating to medical imaging device 104 may also be obtained by other means, such as pre-known calibration target or fiducial points and the relationship of these points to their corresponding identified image.

The position of the patient body, obtained via MPS sensor 120<sub>3</sub>, is used as a reference to compensate for arbitrary patient movement. The data from MPS sensor 120<sub>3</sub> is used to determine motion of the patient with respect to a known set of coordinates, such as the origin of the magnetic coordinate system or with respect to another sensor, or a set plurality of sensors, such as MPS sensor 120<sub>4</sub>. It is noted that each of MPS sensors 120<sub>3</sub> and 120<sub>4</sub> may be used individually to determine patient movement, or they may be used both together. It is further noted that either of MPS sensors 120<sub>3</sub> or 120<sub>4</sub> may include a plurality of sensors (i.e., there may be a plurality of sensors attached to an inspected area of patient body 130, and there may be a plurality of sensors attached to a known area on the surface on which the patient rests).

The process of compensating for patient movement or movement of medical imaging device 104 is known as coordinate system normalization. Coordinate system nor-

malization, also referred herein below as “normalization”, is done using the corresponding reference sensors (i.e., MPS sensors 120<sub>3</sub> or 120<sub>4</sub>) for compensating patient movement. Compensating for movement of medical imaging device 104 may further utilize MPS sensor 120<sub>2</sub> attached to image detector 116 on medical imaging device 104, in addition to MPS sensors 120<sub>3</sub> or 120<sub>4</sub>. It is noted that normalization allows for the utilization of data sets among different sessions or medical procedures. The term “medical procedure” refers to any type of medical procedure performed on a patient, such as diagnostic, therapeutic, or preventative procedures. A medical procedure may be done in several stages. Each stage in a single medical procedure is known as a “session”. It is further noted that no nullification of MPS sensor readings are required due to coordinate system normalization. All data readings obtained from MPS sensors 120<sub>1</sub> and 120<sub>2</sub> may be used for processing, with no need to dismiss a “faulty” reading as a result of arbitrary patient motion. It is yet further noted that coordinate system normalization allows for representing MPS data in different coordinate systems. For example, data may be represented with respect to the coordinate system of the patient, whereby the body of the patient is stationary, and the inspected organ and the surgical tool move. Alternatively, data may be represented with respect to the coordinate system of the inspected organ, whereby the inspected organ is stationary, and the body of the patient and the surgical tool move. Further alternatively, data may be represented with respect to the coordinate system of the surgical tool, whereby the surgical tool is stationary, and the body of the patient and the inspected organ move.

MPS 102 may include additional MPS sensors to be used as further references, similar to MPS sensor 120<sub>3</sub> or MPS sensor 120<sub>4</sub>, thereby further assisting with coordinate system normalization. It is noted however, that other methods for assigning a reference point can be used, such as initial referencing between all MPS sensors and strapping the patient during the entire medical procedure, analyzing the acquired images and identifying a recurring visual point or section therein for each of the MPS sensors other than the sensor attached to the transducer, and the like.

MPS 102 also provides data for obtaining phase information relating to the activity state of an inspected organ. For example, if the inspected organ is a heart, phase information may be heart timing signals denoting stages within a cardiac cycle. A cardiac cycle is defined as the time between two subsequent heart contractions. The electrical activity of the heart as a function of time, such as electrical timing signals obtained by an ECG monitor, can reveal the current stage or phase of the heart within the cardiac cycle. Alternatively, if the inspected organ is a lung, phase information may relate to respiratory rate and stages of the lung within a respiratory cycle. For example, if the inspected organ is an eye, phase information may relate to movement of the eyelid and related ophthalmologic features. Processor 108 obtains phase information by processing data provided by MPS 102 via MPS sensor 120<sub>1</sub>, without the need for any external monitoring device (such as an ECG device). Other sensors may be used independently or in addition in order to generate phase information (e.g., MPS sensor 120<sub>3</sub> in conjunction with MPS sensor 120<sub>1</sub>).

Medical imaging device 104 provides a two-dimensional image of an area within the body of the patient. In the example set forth herewith, the area inspected is the heart and surrounding blood vessels. Medical image device 104 can include any type of image acquisition system known in the art, such as ultra-sound, inner-vascular ultra-sound,

X-ray, C-Arm machines (equipped with such devices), fluoroscopy, angiography, computerized tomography, nuclear magnetic resonance, positron-emission tomography, single-photon-emission tomography, and the like.

Medical imaging device 104 acquires a two-dimensional image via image detector 116. Image detector 116 detects a plurality of two-dimensional images, each representing a view of the inspected organ (e.g., the heart). MPS sensor 120<sub>2</sub> attached to image detector 116 obtains information relating to the position of image detector 116. A frame grabber (not shown) acquires the images and provides them to database 106.

Database 106 stores data required by system 100. Database 106 is typically a database unit, which allows for storage and access of data records. The data includes frames of captured two-dimensional images from medical imaging system 104, as well as MPS sensor readings from MPS 102. Data is transferred to database 106, from which the data is recalled for processing. Intermediate and final data values obtained throughout computations of processor 108 may also be stored in database 106. Database 106 may further store information from additional devices used in conjunction with system 100 (e.g., information from an external monitoring device such as an ECG, intravascular ultrasound information, and the like). In general, database 106 stores all possible information that may be needed by system 100.

Data elements that are stored in database 106 are time-tagged. The term “time-tagging” herein below refers to the process of associating a data element with the exact time at which that data element was obtained (e.g., associating an MPS coordinate reading with the exact time at which that reading was obtained). The data obtained via each of plurality of MPS sensors 120<sub>1</sub>, 120<sub>2</sub>, 120<sub>3</sub> and 120<sub>4</sub> is time-tagged. The plurality of two-dimensional images acquired by medical imaging device 104 is also time-tagged. The time-tags are taken into account when processing the data elements stored in database 106.

Latency compensation is performed on all the time-tagged data elements. In general, image frames from the set of 2D images acquired by medical imaging device 104 are shifted so that the time-tags thereof match the time-tag of the corresponding MPS data set (i.e., images acquired at the same time as an MPS coordinate reading was obtained will be matched with one another).

Processor 108 operates on data gathered in database 106. Processor 108 performs necessary calculations, correlates between the different data streams, and performs filtering, segmentation, reconstruction of three-dimensional models, and other operations. Processor 108 associates between captured two-dimensional images, position information relating to the respective images, and phase information relating to the respective images. Processor 108 constructs trajectories of surgical tool 124 guided within the body of a patient, respective of different activity-states of an inspected organ. Processor 108 may further construct a three-dimensional image from captured two-dimensional images having the same activity-state, and from three-dimensional position data associated with each of the images.

Display 110 presents a motion picture, or image sequence, of the inspected organ in real-time. The motion picture consists of the two-dimensional images captured by medical imaging device 104, with the three-dimensional position data of surgical tool 124 obtained by MPS 102 superimposed via optical projection. The motion picture may consist of a projection of a constructed three-dimensional model of the organ. The motion picture displays the trajectory of surgical tool 120 as the surgical tool is guided within the patient

body, respective of different activity-states of an inspected organ. Display **110** may present a selected image frame of the motion picture respective of the real-time detected organ activity-state. Display **110** may provide different playback effects, freeze frames, change speed, select features, and the like. For example, display **110** may present a playback of previous images in a sequence, showing the progress of surgical tool during previous activity states of the organ. Display **110** may include multiple monitors, or separate windows within a single monitor, where each monitor or window presents a different view. For example, one monitor or window presents the current real-time three-dimensional position data of surgical tool **124** superimposed on the current image frame of the inspected organ respective of the current activity-state, while another monitor or window presents the current real-time three-dimensional position data of surgical tool **124** superimposed on a previous image frame (or image sequence) of the inspected organ respective of a previous activity-state (or activity-states). Display **110** may be a two-dimensional display, an auto-stereoscopic display to be viewed with a suitable pair of spectacles, a stand alone stereoscopic display, a pair of goggles, and the like.

Reference is now made to FIG. **2**, which is a block diagram of a method for registering three-dimensional magnetic coordinates into two-dimensional optical coordinates, operative in accordance with another embodiment of the disclosed technique.

In procedure **210**, a transformation model for magnetic-optical correlation is determined. Magnetic-optical correlation involves the conversion of three-dimensional magnetic coordinates, obtained from MPS sensors, into three-dimensional optical coordinates. The correlation procedure is generally performed once, during the initialization of the entire system. Procedure **210** involves defining a transformation model between the magnetic coordinate system and the optical coordinate system. This transformation defines a global solution of the working volume and does not require any further manual calibration or correlation. In general, as long as there is no change in the magnetic configuration parameters, correlation need not be repeated. The correlation may be modified automatically during the medical procedure in order to calibrate minor changes between the magnetic and optical coordinate systems.

In procedure **220**, a transformation model for optical projection is determined. Optical projection involves the conversion of three-dimensional optical coordinates (obtained using magnetic-optical correlation) into two-dimensional optical coordinates, to be superimposed on an image displayed by display **110**. Optical projection is based on a transformation model from a three-dimensional coordinate system to a two-dimensional coordinate system. This transformation model is based on external optical parameters, internal optical parameters, and image distortion parameters of medical imaging device **104**. Procedure **220** consists of procedures **222**, **224**, **226**, and **228**.

In procedure **222**, external optical parameters are determined. External optical parameters relate to the position of the medical imaging device **104**. In particular, external optical parameters define the coordinate system of medical imaging device **104** with respect to the defined optical coordinate system. In procedure **224**, internal optical parameters are determined. Internal optical parameters of the medical imaging device **104** relate to the image acquisition mechanism. For example, internal optical parameters may include: lens center point, focal length and the like. In procedure **226**, image distortion parameters are determined.

Image distortion parameters relate to parameters which alter the original proportion of objects as they appear in the images acquired by medical imaging device **104**, as a result of physical characteristics of the image acquisition mechanism and the way that the image acquisition mechanism operates. Image distortion parameters may be computed either as a part of the internal optical parameters or as an additional set of correction parameters.

It is noted that the external optical parameters are usually calculated continuously in real-time, whereas it is generally sufficient to compute the internal optical parameters and image distortion parameters once during the beginning stages of the medical procedure. However, there may be cases when it is necessary to re-calculate the internal optical parameters and image distortion parameters at a later stage. MPS data may also be used in re-calculating the external optical parameters, internal optical parameters, and image distortion parameters of medical imaging device **104**. In procedure **228**, a transformation between the three-dimensional coordinate system and two-dimensional coordinate system is defined based on external optical parameters, internal optical parameters, and image distortion parameters of medical imaging device **104**.

Alternatively, or in addition, a direct translation between the 3D MPS coordinate system and the image plane 2D coordinate system can be determined based on known MPS coordinate readings and their relationship to their corresponding identified image coordinates. It is noted that projection procedure **220** takes into account the time-tagged data from the reference sensors of the MPS data to be projected and the images to be projected upon. In case patient movement occurred after an image was acquired, or in case movement of medical imaging device **104** occurred after MPS data was taken, the reference sensors are used in order to compensate for either movements and ensure that the MPS data is projected accurately.

The method of FIG. **2** also includes procedures for converting a set of three-dimensional magnetic coordinates to two-dimensional optical coordinates, shown with reference to the dashed lines. Three-dimensional magnetic coordinates representing position data is obtained from MPS **102**. In procedure **230**, magnetic-optical correlation is applied to three-dimensional magnetic coordinates to produce the equivalent three-dimensional optical coordinates. In procedure **240**, optical projection is applied to the three-dimensional optical coordinates to produce the equivalent two-dimensional optical coordinates. Alternatively a direct transformation from the MPS coordinate system to the image plane can be used. The two-dimensional optical coordinates may be shown on display **110**, in context of the appropriate image frame of the motion picture. The MPS data is projected onto the image plane including all the needed distortion and conversions which affect the projection coordinates only.

Reference is now made to FIG. **3**, which is a block diagram of a method for obtaining phase information from MPS data sets, operative in accordance with a further embodiment of the disclosed technique. In procedure **302**, data sets are obtained from MPS **102**. Each MPS data set comprises a series of position coordinate readings of image detector **116**, surgical tool **124**, a selected area of patient body **130**, or a known area on the surface on which the patient rests, respectively, as received from one of plurality of MPS sensors **120<sub>1</sub>**, **120<sub>2</sub>**, **120<sub>3</sub>** and **120<sub>4</sub>**. MPS **102** processes detected electromagnetic fields to obtain the respective position coordinate readings, which are subsequently stored in database **106**. It is recalled that each MPS

sensor position coordinate reading is time-tagged, or associated with the exact time at which the reading was obtained. Thus, each MPS data set received from MPS sensor 120<sub>1</sub> comprises a collection of coordinate readings demonstrating the precise motion trajectory of surgical tool 124 over time.

In procedure 318, cardiac phase information is obtained from cardiac motion. In particular, cardiac phase information is obtained from data streams originating from MPS sensor 120<sub>1</sub> located on surgical tool 124. Procedure 318 consists of procedures 304, 306, 310, 314 and 316.

In procedure 304, periodic motion frequencies are detected and identified in a time-tagged MPS data set. As surgical tool 124 is guided inside a vessel within the body of a patient, the motion of surgical tool 124 is influenced by two additional factors. The first factor relates to activity of the heart, or cardiac motion, such as systole and diastole. Cardiac motion affects the vessel in a certain way, such as contraction or expansion in varying degrees and at periodic intervals. The second factor relates to breathing activity, or respiratory motion, such as inhaling and exhaling. Respiratory motion affects the vessel in a certain way, such as contraction or expansion in varying degrees and at periodic intervals. Taken together, the overall motion of surgical tool 124 is composed of the cardiac motion and the respiratory motion superimposed onto the basic guiding movement (which corresponds to the vessel topography). The term “organ timing signal” refers herein below to the movement of the blood vessel arising from the periodic motion frequencies (i.e., the cardiac motion and the respiratory motion together).

Since the cardiac motion and respiratory motion are cyclic in nature, the periodic frequencies can be detected in the overall trajectory of surgical tool 124. The specific frequencies relating to the cardiac motion exhibit different characteristics than the specific frequencies relating to the respiratory motion. The specific frequencies relating to the cardiac motion are identified from the detected periodic frequencies. Similarly, the specific frequencies relating to the respiratory motion are identified from the detected periodic frequencies. Processor 108 performs the analysis on the MPS data set and identifies the relevant periodic motion frequencies.

In procedure 306, periodic motion frequencies are filtered from the time-tagged MPS data set. The periodic motion frequencies detected in procedure 304 are separated out from the overall trajectory of surgical tool 124. The remaining motion components correspond to the central axis of the guiding motion of surgical tool 124, which represents the vessel topography, or “centerline trajectory” (referenced procedure 308). The time-tags associated with the MPS data set are retained for each of the filtered periodic motion frequencies. Processor 108 filters out the relevant periodic motion frequencies from the MPS data set.

In procedure 310, the mechanical movement of the vessel originating from the cardiac motion, or “cardiac trajectory”, is reconstructed from the MPS data sets and the filtered periodic motion frequencies. In particular, the cardiac trajectory is reconstructed according to the previously identified specific frequencies relating to the cardiac motion. The reconstructed cardiac trajectory may be reflected, for example, by a graph that indicates the trajectory of the vessel due to cardiac motion over a period of time. Processor 108 analyzes the relevant periodic motion frequencies and creates a reconstruction of the cardiac trajectory.

In procedure 312, the mechanical movement of the vessel originating from the respiratory motion, or “respiratory trajectory”, is reconstructed from the MPS data sets and the

filtered periodic motion frequencies. In particular, the respiratory trajectory is reconstructed according to the previously identified specific frequencies relating to the respiratory motion. The reconstructed respiratory trajectory may be reflected, for example, by a graph that indicates the trajectory of the vessel due to respiratory motion over a period of time. Processor 108 analyzes the relevant periodic motion frequencies and creates a reconstruction of the respiratory trajectory.

Reconstruction of the respiratory trajectory may be based solely on coordinate readings obtained from the external reference sensors (i.e., MPS sensors 120<sub>3</sub> or 120<sub>4</sub>). It is noted that an additional reference sensor (or plurality thereof) may be attached (i.e., externally or internally) to the body of the patient, to monitor breathing patterns and the like. For example, an intravascular sensor may be used for this purpose. This sensor functions as a confirmation mechanism to provide support data regarding respiratory motion, and more accurately determine periodic motion frequencies relating to respiratory motion. It is noted that the same or additional sensor (or plurality thereof) may be used for gathering additional cardiac data either as a confirmation mechanism and/or for providing supporting data for cardiac phase detection.

In procedure 314, phase detection is performed on the reconstructed cardiac trajectory. The cardiac trajectory consists of different phases or activity-states of the heart, corresponding to different points within a cardiac cycle. The phases repeat themselves periodically with each cycle. The plurality of cardiac activity-states is identified on the reconstructed cardiac trajectory during phase detection. Processor 108 performs the analysis of the cardiac trajectory and identifies the different cardiac cycle phases.

Reference is now made to FIG. 4A, which is a schematic illustration of a sample cardiac trajectory, in electrical signal representation and in mechanical signal representation. The mechanical signal representation of the cardiac trajectory, generally referenced 400, includes a plurality of cardiac activity-states (i.e., cardiac cycle phases), such as activity-states T<sub>1</sub>, T<sub>2</sub> and T<sub>3</sub>, in each of plurality of cardiac cycles 410, 420 and 430. The mechanical representation of the cardiac trajectory is equivalent to the cardiac trajectory reconstructed from the MPS data sets and the filtered periodic motion frequencies in procedure 310. The electrical signal representation of the cardiac trajectory, generally referenced 450, depicts the same activity-states T<sub>1</sub>, T<sub>2</sub> and T<sub>3</sub>, in each of plurality of cardiac cycles 410, 420 and 430. However the precise time at which these activity-states occur may be different in the two representations, as there is a slight delay at the electrical representation with respect to the mechanical representation. For example, it is shown that activity-state T<sub>1</sub> of cardiac cycle 430 occurs at time t<sub>a</sub> in cardiac trajectory 400 and at time t<sub>b</sub> in cardiac trajectory 450. Therefore, it is necessary to perform an alignment between the activity states, when using information from the electrical representation for phase detection. The electrical representation of the cardiac trajectory is equivalent to the electrical timing signals obtained by an ECG monitor.

It is noted that the detection of cardiac phases is performed based solely on data sets originating from at least MPS sensor 120<sub>1</sub> located on surgical tool 124, and perhaps also from the reference sensors (i.e., MPS sensors 120<sub>3</sub> and 120<sub>4</sub>). These data sets provide a mechanical representation of the cardiac trajectory. No external monitoring device is required to obtain cardiac phase information. It is noted that periodic motion components relating to the respiratory motion may also be used as supporting data for cardiac

phase detection. It is further noted that phase detection may be performed on the original MPS data sets, rather than on the reconstructed cardiac trajectory, using the detected and filtered periodic motion frequencies. In this case, the different phases or activity-states of the heart are identified directly on the MPS data sets obtained in procedure 302.

In procedure 316, cardiac phase information is associated with the MPS data sets. Each data set obtained from MPS sensor 120<sub>1</sub> relating to position of surgical tool 124 is matched to one of plurality of activity-states T<sub>1</sub>, T<sub>2</sub> and T<sub>3</sub>, according to their corresponding time elements (i.e., time-tags). The position of the inspected vessel, and consequently the position of guided surgical tool 124, is different during different activity-states of the inspected organ. Processor 108 associates between a coordinate reading and the matching phase thereof, and stores the information in database 106.

Respiratory phase information may be obtained from the respiratory motion, in a similar manner as cardiac phase information is obtained from the cardiac motion. Respiration activity-states may be identified on the reconstructed respiratory trajectory using the periodic motion components relating to the respiratory motion. Periodic motion components relating to the respiratory motion may also be used in correlation of non-corresponding data sets (discussed with reference to FIG. 8).

Respiratory phase information is obtained from respiratory motion in optional procedure 320. Procedure 320 consists of procedures 304, 306, 312, 322 and 324. In procedure 312, the respiratory trajectory is reconstructed from the MPS data sets and the filtered periodic motion frequencies, as elaborated upon earlier. In procedure 322, phase detection is performed on the reconstructed respiratory trajectory. Similar to the cardiac trajectory, the respiratory trajectory consists of different phases or activity-states of the lungs, corresponding to different points within a respiratory cycle. The respiratory activity-states of the lungs may be identified from the phases of the respiratory trajectory. The phases repeat themselves periodically with each cycle. The plurality of respiratory activity-states is identified on the reconstructed respiratory trajectory during phase detection. Processor 108 performs the analysis of the respiratory trajectory and identifies the different respiratory cycle phases.

Reference is now made to FIG. 4B, which is a schematic illustration of a sample respiratory trajectory in mechanical signal representation. The mechanical signal representation of the respiratory trajectory, generally referenced 460, includes a plurality of respiratory activity-states (i.e., respiratory cycle phases), such as activity-states T<sub>4</sub>, T<sub>5</sub> and T<sub>6</sub>. The mechanical representation of the respiratory trajectory is equivalent to the respiratory trajectory reconstructed from the MPS data sets and the filtered periodic motion frequencies in procedure 310.

It is noted that the detection of respiratory phases is performed based solely on data sets originating from MPS sensor 120<sub>1</sub> located on surgical tool 124, and from MPS sensors 120<sub>3</sub> and 120<sub>4</sub>, located on a selected area of patient body 130, and a known area on the surface on which the patient rests, respectively. These data sets provide a mechanical representation of the respiratory trajectory. No external monitoring device is required to obtain respiratory phase information. It is further noted that phase detection may be performed on the original MPS data sets, rather than on the reconstructed respiratory trajectory, using the detected and filtered periodic motion frequencies. In this

case, the different phases or activity-states of the lung are identified directly on the MPS data sets obtained in procedure 302.

It is noted that the actual value of the cardiac rate or respiratory rate of the patient may be obtained without the use of an external monitoring device (such as an ECG device). The cardiac rate or respiratory rate of the patient may be obtained solely from MPS sensors 120<sub>1</sub>, 120<sub>3</sub> and 120<sub>4</sub>, either individually or jointly.

In procedure 324, respiratory phase information is associated with the MPS data sets. Each data set obtained from MPS sensor 120<sub>1</sub> relating to position of surgical tool 124 is matched to one of plurality of activity-states T<sub>4</sub>, T<sub>5</sub> and T<sub>6</sub>, according to their corresponding time tags. Procedure 324 is analogous to procedure 316 discussed above.

Reference is now made to FIG. 5, which is a schematic illustration of a trajectory 550 of the surgical tool of the system of FIG. 1, inside a vessel in the body of a patient, respective of different activity-states of the cardiac trajectory of FIG. 4. At activity-state T<sub>1</sub> of each of the cardiac cycles 410, 420 and 430, the position of the vessel is represented by a vessel image 570 (indicated in FIG. 5 with solid lines). At activity-state T<sub>2</sub> of each of the cardiac cycles 410, 420 and 430, the position of the vessel is represented by a vessel image 572 (indicated in FIG. 5 with dashed lines). At activity-state T<sub>3</sub> of each of the cardiac cycles 410, 420 and 430, the position of the vessel is represented by a vessel image 574 (indicated in FIG. 5 with dotted lines). Thus, each of the coordinates 552, 554, 556, 558, 560, 562, 564, 566 and 568 corresponds to a position of surgical tool 124, while the vessel is at a different position, in a different activity-state of a cardiac cycle.

For example, coordinate 552 corresponds to activity-state T<sub>1</sub> in cardiac cycle 410, meaning that when MPS sensor 120<sub>1</sub> on surgical tool 124 is at coordinate 552, the heart of the patient is at activity-state T<sub>1</sub>. Coordinate 554 corresponds to activity-state T<sub>2</sub> in cardiac cycle 410, meaning that when MPS sensor 120<sub>1</sub> on surgical tool 124 is at coordinate 554, the heart of the patient is at activity-state T<sub>2</sub>. Coordinate 556 corresponds to activity-state T<sub>3</sub> in cardiac cycle 410, meaning that when MPS sensor 120<sub>1</sub> on surgical tool 124 is at coordinate 556, the heart of the patient is at activity-state T<sub>3</sub>. Coordinate 558 corresponds to activity-state T<sub>1</sub> in cardiac cycle 420. Coordinate 560 corresponds to activity-state T<sub>2</sub> in cardiac cycle 420. Coordinate 562 corresponds to activity-state T<sub>3</sub> in cardiac cycle 420. Coordinate 564 corresponds to activity-state T<sub>1</sub> in cardiac cycle 430. Coordinate 566 corresponds to activity-state T<sub>2</sub> in cardiac cycle 430. Coordinate 568 corresponds to activity-state T<sub>3</sub> in cardiac cycle 430. It is noted that coordinates 552, 554, 556, 558, 560, 562, 564, 566 and 568 are related to the respiratory activity states T<sub>4</sub>, T<sub>5</sub>, T<sub>6</sub> in a similar manner.

According to another aspect of the disclosed technique, position measurements, together with acquired images, are processed with respect to the activity-state of the inspected organ at the time of acquisition or measurement. For example, with reference to FIG. 1, display 110 displays the trajectory of a surgical tool 124 superimposed on a two-dimensional image of an inspected organ, wherein the two-dimensional image corresponds to an activity-state determined by the current position of surgical tool 124 inside the inspected organ. The system records the path which surgical tool 124 follows inside the inspected organ, in either a forward or a backward direction. The system further registers this path with monitored activity-states of the inspected organ and with the instantaneous position of surgical tool 124.

Reference is now made to FIG. 6, which is a schematic illustration of trajectories of a guided surgical tool inside a vessel in the body of a patient, each trajectory processed with respect to a different activity-state. For example, processor 108 associates for a given two-dimensional image acquired during activity-state  $T_1$ , all the position coordinate readings of surgical tool 124 (i.e., coordinates 612, 618 and 624) which were detected during activity-state  $T_1$  at any cycle of cardiac trajectory 400. Similarly, processor 108 associates for a given two-dimensional image acquired during activity-state  $T_2$ , all the position coordinate readings (i.e., coordinates 614, 620 and 626) which were detected during activity-state  $T_2$  at any cycle of cardiac trajectory 400; and further associates for a given two-dimensional image acquired during activity-state  $T_3$ , all the position coordinate readings (i.e., coordinates 616, 622 and 628) which were detected during activity-state  $T_3$  at any cycle of cardiac trajectory 400.

Processor 108 calculates a trajectory 606 from points 612, 618 and 624, associated with activity state  $T_1$ . Similarly, processor 108 calculates a trajectory 608 from points 614, 620 and 626 associated with activity state  $T_2$ , and further calculates a trajectory 610 from points 616, 622 and 628 associated with activity state  $T_3$ .

Processor 108 associates between each of the calculated trajectories and a two-dimensional image, respective of a given organ activity-state. Processor 108 associates between trajectory 612 and two-dimensional image 600 (indicated with solid lines), respective of activity state  $T_1$ . Similarly, processor 108 associates between trajectory 614 and two-dimensional image 602 (indicated with dashed lines), respective of activity state  $T_2$  and further between trajectory 614 and two-dimensional image 604 (indicated with dotted lines), respective of activity state  $T_3$ .

Display 110 presents a superimposition of each of the calculated trajectories on its respective two-dimensional image. For example, display 110 presents trajectory 606 superimposed on two-dimensional image 600, trajectory 608 superimposed on two-dimensional image 602 and trajectory 610 superimposed on two-dimensional image 604. Display 110 may present these images as a single image frame shown one at a time, or a sequence of images (i.e., motion picture) shown consecutively.

It is noted that points 612, 614, 616, 618, 620, 622, 624, 626 and 628 represent a situation similar to that presented by points 552, 554, 556, 558, 560, 562, 564, 566 and 568 with respect to FIG. 5. However, according to an aspect of the disclosed technique presented in FIG. 6, processor 108 calculates a trajectory of surgical tool 124 based on the position coordinate readings detected during a given activity-state. Thus, each trajectory corresponds to a different activity-state of the inspected organ. Processor 108 further associates each calculated trajectory with a vessel image acquired during the corresponding activity-state.

Reference is now made to FIG. 7, which is a block diagram of a method for superimposing MPS data onto two-dimensional image data for corresponding data sets, operative in accordance with another embodiment of the disclosed technique. It is recalled that the position coordinate readings obtained from MPS 102 is time-tagged. Similarly, the sequence of two-dimensional images obtained from medical imaging device 104 is time-tagged. "Corresponding data sets" refer to a pair of data sets which have the same time-tags. It is noted that the time-tag of a data set refers to the set of time-tags of the elements within the data set. For example, an MPS data set is corresponding with a two-dimensional images data set if readings in the MPS data

set have the same time-tag as images in the two-dimensional images data set. Corresponding data sets represent data sets that occur during the same session in a medical procedure. "Non-corresponding data sets" refer to a pair of data sets which have different time-tags. For example, an MPS data set is non-corresponding with a two-dimensional images data set if readings in the MPS data set have a different time-tag than all the images in the two-dimensional images data set. Non-corresponding data sets represent data sets that were recorded during different sessions (within the same or different medical procedures).

In procedure 702, an MPS data set is normalized. The MPS data set, which comprises three-dimensional coordinate readings in the magnetic coordinate system, is obtained from MPS 102. Normalization compensates for patient movement or movement of medical imaging device 116, as discussed with reference to FIG. 1. Normalization is performed using MPS data with corresponding time-tags from the reference sensors (i.e., MPS sensors 120<sub>3</sub> or 120<sub>4</sub>), and perhaps also MPS sensor 120<sub>2</sub> as well.

In procedure 704, magnetic-optical correlation is performed on the normalized MPS data set. The correlation procedure transforms the three-dimensional position magnetic coordinate into a three-dimensional coordinate in the optical coordinate system. The correlation procedure is based on the magnetic-optical transformation model, determined in procedure 210 with reference to FIG. 2.

In procedure 706, optical projection is performed on the correlated MPS data set. The optical projection procedure transforms the three-dimensional position MPS coordinate reading in the optical coordinate system to a two-dimensional coordinate. The optical projection procedure is based on the three-dimensional to two-dimensional optical transformation model, determined in procedure 228 with reference to FIG. 2. It is noted that the three-dimensional to two-dimensional optical transformation model is a function of certain parameters (i.e., internal and external optical parameters and image distortion parameters of medical imaging device 104), which are computed at a given instant in time, and as such, is time-tagged. Therefore the optical projection procedure is based on a three-dimensional to two-dimensional optical transformation model which has the same time-tag as the MPS data set.

A direct transformation between 3D MPS data to 2D image coordinates can be used in case such a direct translation was computed. Compensation for optical distortions is done at a given instant in time and as such, is time-tagged.

In procedure 708, the MPS data set is superimposed onto an image from the two-dimensional images data set. The two-dimensional images data set is obtained from medical imaging device 104. The MPS data set now includes two-dimensional position coordinates in the optical coordinate system. With reference to FIG. 1, processor 108 associates between a position coordinate reading and a two-dimensional image, in accordance with their mutual time-tag. Display 110 may present a picture showing the position of surgical tool 124 respective of the inspected organ, at a given point in time, in accordance with acquired two-dimensional image data and acquired MPS data. Further, as will be elaborated upon with reference to FIGS. 9 and 10, display 110 may present a motion picture showing the trajectory of the guided surgical tool respective of the inspected organ, in accordance with acquired two-dimensional image data set and acquired MPS data set.

The MPS data and two-dimensional image data may further be associated with activity state information. With reference to FIG. 1, processor 108 associates between a

position coordinate reading and a two-dimensional image, in accordance with their mutual time-tag, respective of a given organ activity-state. Display 110 may present an image frame showing the position of surgical tool 124, respective of the inspected organ at a given activity-state, in accordance with acquired two-dimensional image data, acquired MPS data, and associated activity-state information. Further, display 110 may present a motion picture showing the trajectory of the guided surgical tool respective of the inspected organ at a given activity-state, in accordance with acquired two-dimensional image data set, acquired MPS data set, and associated activity-state information. This will be elaborated upon with reference to FIGS. 9 and 10.

Reference is now made to FIG. 8, which is a block diagram of a method for superimposing MPS data onto two-dimensional image data for non-corresponding data sets, operative in accordance with a further embodiment of the disclosed technique. A first MPS data set with a first time-tag is corresponding with a two-dimensional images data set. A second MPS data set with a second time-tag is non-corresponding with the two-dimensional images data set. The time-tagged MPS data sets are obtained from MPS 102. The time-tagged two-dimensional images data set is obtained from medical imaging device 104.

In procedure 318, cardiac phase information is obtained from cardiac motion data, for both the first MPS data set and the second MPS data set. Procedure 318 involves detecting and identifying periodic motion frequencies, filtering periodic motion components, reconstructing the cardiac trajectory from the MPS data set and filtered periodic motion frequencies, performing phase detection on the reconstructed cardiac trajectory, and associating each coordinate reading in the MPS data set with a cardiac phase, in accordance with their time-tags. Periodic motion components relating to the respiratory motion may also be used as supporting data for cardiac phase detection. Procedure 318 is described in detail with respect to FIG. 3.

In procedure 320, respiratory phase information is obtained from respiratory motion data, for both the first MPS data set and the second MPS data set. It is noted that procedure 320 is optional, and may be performed instead of procedure 318, or in conjunction with procedure 318. Procedure 320 involves detecting and identifying periodic motion frequencies, filtering periodic motion components, reconstructing the respiratory trajectory from the MPS data set and filtered periodic motion frequencies, performing phase detection on the reconstructed respiratory trajectory, and associating each coordinate reading in the MPS data set with a respiratory phase, in accordance with their time-tags. Procedure 320 is described in detail with respect to FIG. 3.

In procedure 820, a third MPS data set with the same time-tag as the first MPS data set is generated from the second MPS data set, using phase alignment between the phases of the two MPS data sets. In particular, the coordinate readings of the second MPS data set are assigned the same time-tags as the coordinate readings of the first MPS data set, by matching the phases of the coordinate readings from each data set. Each of the detected phases in the second MPS data set is mapped to the matching phase in the first MPS data set. Each of the detected phases in the second MPS data set (and thus each coordinate reading associated with that phase) is then assigned a new time-tag based on the time-tag of the matching phase in the first MPS data set. For example, if phase A occurs at time "x" in the second MPS data set, and phase A occurs at time "y" in the first MPS data set, then phase A is reassigned time-tag "y" in the third MPS data set. The phase mapping aligns the phases of the cardiac trajec-

tory of the second data set with the cardiac trajectory of the first MPS data set. After the procedures of mapping and reassigning have been completed, the resulting data set will have the same time-tag as the first MPS data set, and hence as the two-dimensional image data set. Therefore, the third MPS data set will be corresponding with the two-dimensional image data set. It is noted that periodic motion components relating to the respiratory motion may be used in addition to, or instead of, the periodic motion components relating to the cardiac motion, for performing phase alignment. It is noted that procedure 820 may generate simply an index of each element in the third data set.

In procedure 822, magnetic-optical correlation is performed on the third MPS data set. It is noted that normalization, or compensating for patient movement or movement of medical imaging device 116, is performed prior to procedure 822. Normalization is discussed in procedure 702 with reference to FIG. 7. Normalization may be performed immediately prior to procedure 820 or immediately after procedure 820. The correlation procedure transforms the three-dimensional position magnetic coordinate into a three-dimensional coordinate in the optical coordinate system. The correlation procedure is based on the magnetic-optical transformation model, determined in procedure 210 with reference to FIG. 2.

In procedure 824, optical projection is performed on the correlated third MPS data set. The optical projection procedure transforms the three-dimensional position MPS coordinate in the optical coordinate system to a two-dimensional optical coordinate. The optical projection procedure is based on the three-dimensional to two-dimensional optical transformation model, determined in procedure 228 with reference to FIG. 2. It is recalled that the three-dimensional to two-dimensional optical transformation model is time-tagged. Therefore the optical projection procedure is based on a three-dimensional to two-dimensional optical transformation model which has the same time-tag as first MPS data set.

In procedure 826, the third MPS data set is superimposed onto an image from the two-dimensional images data set. With reference to FIG. 1, processor 108 associates between a position coordinate reading in the third MPS data set and a two-dimensional image, in accordance with their mutual time-tag. Display 110 may present an image frame showing the position of surgical tool 124 respective of the inspected organ, at a given point in time, in accordance with acquired two-dimensional image data and acquired MPS data. Further, display 110 may present a motion picture showing the trajectory of the guided surgical tool respective of the inspected organ, in accordance with acquired two-dimensional image data set and acquired MPS data set. The MPS data and two-dimensional image data may further be associated with activity state information. Display 110 may further simultaneously present MPS data with a corresponding data set and with a non-corresponding data set. For example, presenting a superimposition of current real-time MPS data on current real-time images (i.e., corresponding data sets), while at the same time presenting a superimposition of the same current real-time MPS data on previously taken images (i.e., non-corresponding data sets) using associated activity state information.

Reference is now made to FIG. 9, which is a block diagram of a method for constructing trajectories of a guided surgical tool within the body of a patient, respective of different activity-states of an inspected organ (e.g., such as shown in FIG. 6), operative in accordance with another embodiment of the disclosed technique. In the following

example, an MPS data set corresponding with a two-dimensional image data set is used. It is noted that non-corresponding data sets may be used as well, after simply undergoing phase alignment, similar to procedure 820 discussed with reference to FIG. 8. The time-tagged MPS data set is obtained from MPS 102. The time-tagged two-dimensional images data set is obtained from medical imaging device 104.

In procedure 318, cardiac phase information is obtained from cardiac motion data, for the MPS data set. Procedure 318 involves detecting and identifying periodic motion frequencies, filtering periodic motion components, reconstructing the cardiac trajectory from the MPS data set and filtered periodic motion frequencies, performing phase detection on the reconstructed cardiac trajectory, and associating each coordinate reading in the MPS data set with a phase, in accordance with their time-tags. Periodic motion components relating to the respiratory motion may also be used as supporting data for cardiac phase detection. Procedure 318 is described in detail with respect to FIG. 3.

In procedure 320, respiratory phase information is obtained from respiratory motion data, for both the first MPS data set and the second MPS data set. It is noted that procedure 320 is optional, and may be performed instead of procedure 318, or in conjunction with procedure 318. Procedure 320 involves detecting and identifying periodic motion frequencies, filtering periodic motion components, reconstructing the respiratory trajectory from the MPS data set and filtered periodic motion frequencies, performing phase detection on the reconstructed respiratory trajectory, and associating each coordinate reading in the MPS data set with a respiratory phase, in accordance with their time-tags. Procedure 320 is described in detail with respect to FIG. 3.

In procedure 908, correlated phase information is obtained for the two-dimensional images data set. The phase information is correlated in the sense that the phase information is not obtained directly from the images but from correlated MPS data (occurring at the same time as a given image). The phases or activity-states of the heart, such as activity-states  $T_1$ ,  $T_2$  and  $T_3$  with reference to FIG. 4, during which each two-dimensional image was acquired, is identified. Identification of the activity-states makes use of the time-tags taken during acquisition of all the images, and the phases of an MPS data set having the same time-tags.

A monitoring device such as an ECG may be used in conjunction with MPS data to obtain phase information of the two-dimensional image data set in certain instances. For example, if there was no sensor within the body of the patient during acquisition of a given image (e.g., during the very beginning of the medical procedure when medical images are taken before the guide wire is inserted into the vessel), information from the monitoring device may be used together with non-corresponding MPS data. In such a case, phase alignment is performed between the mechanical representation based phase data obtained by the MPS data and the external phase obtained by the monitoring device (such as electrical representation based phase data obtained from an ECG device). Phase alignment between the mechanical and electrical based data is necessary in order to account for different latencies originating from the different sampled signals that represent the same cardiac trajectory. It is noted that data obtained from the monitoring device is also time-tagged.

In procedure 910, a separate MPS data set is generated for each two-dimensional image, in accordance with the image phase and time-tags. All the MPS position coordinate readings acquired during the same phase are combined into a

single data set. After procedure 910 has been completed, every image of the two-dimensional image data set has a corresponding MPS data set containing therein only those coordinate readings which were acquired in the same phase as that image.

In procedure 912, magnetic-optical correlation is performed on each MPS data set generated in procedure 910. It is noted that normalization, or compensating for patient movement or movement of medical imaging device 116, is performed prior to procedure 912. Normalization is discussed in procedure 702 with reference to FIG. 7. Normalization may be performed immediately prior to procedure 910 or immediately after procedure 910. The correlation procedure transforms the three-dimensional position magnetic coordinate into a three-dimensional coordinate in the optical coordinate system. The correlation procedure is based on the magnetic-optical transformation model, determined in procedure 210 with reference to FIG. 2.

In procedure 914, optical projection is performed on each correlated MPS data set generated in procedure 910. The optical projection procedure transforms the three-dimensional position MPS coordinate in the optical coordinate system to a two-dimensional optical coordinate. The optical projection procedure is based on the three-dimensional to two-dimensional optical transformation model, determined in procedure 228 with reference to FIG. 2. It is recalled that the three-dimensional to two-dimensional optical transformation model is time-tagged. Therefore the optical projection procedure is based on a three-dimensional to two-dimensional optical transformation which has the same time-tag as the MPS data set.

In procedure 916, each MPS data set generated in procedure 910 is superimposed onto the corresponding two-dimensional image. For each two-dimensional image, the MPS coordinate readings which were acquired during the same phase at the two-dimensional image are superimposed onto that image. The coordinate readings are then connected together by lines, thereby composing a spline representing the trajectory of surgical tool 124 respective of an activity state of the inspected organ. Display 110 may present an image frame showing the position of surgical tool 124 respective of the inspected organ, at a given point in time, in accordance with acquired two-dimensional image data and acquired MPS data. Further, display 110 may present a motion picture showing the trajectory of the guided surgical tool respective of the inspected organ, in accordance with acquired two-dimensional image data set and acquired MPS data set. The MPS data and two-dimensional image data may further be associated with activity state information. Display 110 may further simultaneously present a superimposition of current real-time MPS data on current real-time images, while presenting a superimposition of the same current real-time MPS data on previously taken images, using associated activity state information.

Reference is now made to FIG. 10, which is a block diagram of an additional method for constructing trajectories of a guided surgical tool within the body of a patient, respective of different activity-states of an inspected organ, operative in accordance with a further embodiment of the disclosed technique. In the following example, an MPS data set corresponding with a two-dimensional image data set is used. It is noted that non-corresponding data sets may be used as well, after simply undergoing phase alignment, similar to the procedure discussed with reference to FIG. 8. A time-tagged MPS data set is obtained from MPS 102. A time-tagged two-dimensional images data set is obtained from medical imaging device 104.

In procedure **318**, cardiac phase information is obtained from cardiac motion data, for the MPS data set. Procedure **318** involves detecting and identifying periodic motion frequencies, filtering periodic motion components, reconstructing the cardiac trajectory from the MPS data set and filtered periodic motion frequencies, performing phase detection on the reconstructed cardiac trajectory, and associating each coordinate reading in the MPS data set with a phase, in accordance with their time-tags. Periodic motion components relating to the respiratory motion may also be used as supporting data for cardiac phase detection. Procedure **318** is described in detail with respect to FIG. 3.

In procedure **320**, respiratory phase information is obtained from respiratory motion data, for both the first MPS data set and the second MPS data set. It is noted that procedure **320** is optional, and may be performed instead of procedure **318**, or in conjunction with procedure **318**. Procedure **320** involves detecting and identifying periodic motion frequencies, filtering periodic motion components, reconstructing the respiratory trajectory from the MPS data set and filtered periodic motion frequencies, performing phase detection on the reconstructed respiratory trajectory, and associating each coordinate reading in the MPS data set with a respiratory phase, in accordance with their time-tags. Procedure **320** is described in detail with respect to FIG. 3.

In procedure **1004**, the centerline trajectory is reconstructed. After the periodic motion components are separated out from the overall trajectory of surgical tool **124**, the remaining motion components corresponds to the central axis of the guiding motion of surgical tool **124**, or centerline trajectory. Procedure **1004** is similar to procedure **308** with reference to FIG. 3.

In procedure **1010**, separate centerline trajectories are reconstructed for each phase. Based on the time-tags and the detected phases of the cardiac trajectory, the centerline positions are matched according to phase, and a different trajectory is built for each phase.

In procedure **1012**, correlated phase information is obtained for the two-dimensional images data set. The phase is correlated in the sense that the phase information is not obtained directly from the images but from correlated MPS information (occurring at the same time as a given image). The phases or activity-states of the heart, such as activity-states  $T_1$ ,  $T_2$  and  $T_3$ , with reference to FIG. 4, during which each two-dimensional image was acquired, is identified. Identification of the activity-states makes use of the time-tags taken during acquisition of all the images, and the phases of an MPS data set having the same time-tags. A monitoring device such as an ECG may be used in conjunction with MPS data to obtain phase information of the two-dimensional image data set in certain instances, as discussed with reference to FIG. 9. In such a case, phase alignment is done between the mechanical based phase data and the electrical based phase data in order to account for different latencies originating from the different sampled signals that represent the same cardiac trajectory. Procedure **1012** is similar to procedure **908** with reference to FIG. 9.

In procedure **1014**, each centerline trajectory is shifted by superimposing the matching periodic motion components, for each phase of the images in two-dimensional images data set. The periodic motion components, relating to cardiac motion and respiratory motion, are added on to the centerline trajectories. For each separate centerline trajectory, respective of a given phase, the periodic motion components of that phase are added onto the centerline trajectory. Each centerline trajectory is then shifted, in accordance with the added periodic motion components.

In procedure **1016**, magnetic-optical correlation is performed on each cardiac trajectory shifted in procedure **1014**. It is noted that normalization, or compensating for patient movement or movement of medical imaging device **116**, is performed prior to procedure **1016**. Normalization is discussed in procedure **702** with reference to FIG. 7. Normalization may be performed immediately prior to procedure **1014** or immediately after procedure **1014**. The correlation procedure transforms the three-dimensional position magnetic coordinate into a three-dimensional coordinate in the optical coordinate system. The correlation procedure is based on the magnetic-optical transformation model, determined in procedure **210** with reference to FIG. 2.

In procedure **1018**, optical projection is performed on each correlated cardiac trajectory shifted in procedure **1014**. The optical projection procedure transforms the three-dimensional position MPS coordinate in the optical coordinate system to a two-dimensional optical coordinate. The optical projection procedure is based on the three-dimensional to two-dimensional optical transformation model, determined in procedure **228** with reference to FIG. 2. It is recalled that the three-dimensional to two-dimensional optical transformation model is time-tagged. Therefore the optical projection procedure is based on a three-dimensional to two-dimensional optical transformation which has the same time-tag as the cardiac trajectory.

In procedure **1020**, each shifted centerline trajectory is superimposed onto the corresponding two-dimensional image. For each two-dimensional image, the MPS coordinate readings of the centerline trajectory matching the same phase at the two-dimensional image are superimposed onto that image. The coordinate readings are then connected together by lines, thereby composing a spline representing the trajectory of surgical tool **124** respective of an activity state of the inspected organ. Display **110** may present an image frame showing the position of surgical tool **124** respective of the inspected organ, at a given point in time, in accordance with acquired two-dimensional image data and acquired MPS data. Further, display **110** may present a motion picture showing the trajectory of the guided surgical tool respective of the inspected organ, in accordance with acquired two-dimensional image data set and acquired MPS data set. The MPS data and two-dimensional image data may further be associated with activity state information. Display **110** may further simultaneously present a superimposition of current real-time MPS data on current real-time images, while presenting a superimposition of the same current real-time MPS data on previously taken images, using associated activity state information.

It will be appreciated by persons skilled in the art that the disclosed technique is not limited to what has been particularly shown and described hereinabove. Rather the scope of the disclosed technique is defined only by the claims, which follow.

The invention claimed is:

1. An apparatus for generating an organ timing signal relating to at least one inspected organ within a body of a patient, said apparatus comprising:

a medical positioning system (MPS) including:

- a reference electromagnetic transducer placed at a reference location;
- an inner electromagnetic transducer attached to a surgical tool inserted in a blood vessel in the vicinity of said inspected organ; and
- said medical positioning system (MPS), coupled with said reference electromagnetic transducer and with said inner electromagnetic transducer, said MPS

determining the three-dimensional position of said inner electromagnetic transducer, by processing transmitted electromagnetic signals transmitted from one of (i) the reference electromagnetic transducer and (ii) the inner electromagnetic transducer, with detected electromagnetic signals detected by the other one of said reference and inner electromagnetic transducers, said MPS further generating time-tagged MPS data sets, each of said MPS data sets comprising a collection of three-dimensional position coordinate readings wherein each of the readings is associated with a respective time at which the reading was obtained, the readings demonstrating the overall motion trajectory of said surgical tool over time; and

a processor coupled with said MPS, generating said organ timing signal from said MPS data sets by detecting and identifying periodic motion frequencies in said time-tagged MPS data sets, and filtering said periodic motion frequencies from said MPS data sets so as to separate out said periodic motion frequencies corresponding to said organ timing signal from said overall motion trajectory of said surgical tool.

2. The apparatus according to claim 1, wherein said reference electromagnetic transducer transmits electromagnetic signals and said inner electromagnetic transducer detects electromagnetic signals.

3. The apparatus according to claim 1, wherein said inner electromagnetic transducer transmits electromagnetic signals and said reference electromagnetic transducer detects electromagnetic signals.

4. The apparatus according to claim 1, wherein for at least one of said at least one reference electromagnetic transducer, said reference location is a portion of said body of a patient.

5. The apparatus according to claim 1, wherein for at least one of said at least one reference electromagnetic transducer, said reference location is stationary with respect to said body of a patient.

6. The apparatus according to claim 1, further comprising at least one additional electromagnetic transducer attached to an area of said body of a patient, said electromagnetic transducer obtaining three-dimensional position information of said area, for movement compensation.

7. The apparatus according to claim 1, further comprising at least one additional electromagnetic transducer attached to a known area on the surface on which said patient rests, said electromagnetic transducer obtaining three-dimensional position information of said area, for compensating for movement of said patient.

8. The apparatus according to claim 1, wherein said processor further reconstructs a cardiac trajectory from said MPS data sets and said filtered periodic motion frequencies, said cardiac trajectory representing a mechanical movement of said blood vessel originating from cardiac motion.

9. The apparatus according to claim 8, wherein said processor further detects phase information of said inspected organ by identifying a plurality of phases on said reconstructed cardiac trajectory.

10. The apparatus according to claim 9, further comprising:

a database coupled with said MPS and with said processor, said database storing at least said MPS data sets; and

a medical imaging device coupled with said database, said medical imaging device including an image detector, said medical imaging device acquiring a plurality of two-dimensional images of said inspected organ via

said image detector, said database further storing at least said plurality of two-dimensional images, wherein said processor further associates between said acquired two-dimensional images, said MPS data sets, and said phase information, and constructs trajectories of said surgical tool guided within said blood vessel, respective of different phases of said inspected organ.

11. The apparatus according to claim 10, wherein said processor associates between said plurality of two-dimensional images and said MPS data sets, with respect to said phase information at the time of acquisition or measurement.

12. The apparatus according to claim 10, wherein said processor associates for a given two-dimensional image acquired during a given phase of said inspected organ, position coordinate readings detected during said given phase.

13. The apparatus according to claim 10, wherein said processor constructs trajectories of said surgical tool guided within said blood vessel, based on said position coordinate readings detected during a given phase of said inspected organ.

14. The apparatus according to claim 13, wherein said processor further associates each of said constructed trajectories with a two-dimensional image acquired during the corresponding phase of said inspected organ.

15. The apparatus according to claim 13, wherein said display presents a superimposition of said constructed trajectories on a two-dimensional image.

16. The apparatus according to claim 15, wherein said display presents said images as a series of individual image frames that are shown one at a time.

17. The apparatus according to claim 15, wherein said display presents said images as a sequence of image frames that are shown consecutively.

18. The apparatus according to claim 1, wherein said processor further reconstructs a respiratory trajectory from said MPS data sets and said filtered periodic motion frequencies, said respiratory trajectory representing a mechanical movement of said blood vessel originating from respiratory motion.

19. The apparatus according to claim 18, wherein said processor further detects phase information of said inspected organ by identifying a plurality of phases on said reconstructed respiratory trajectory.

20. The apparatus according to claim 1, wherein said inspected organ is a heart.

21. The apparatus according to claim 1, wherein said inspected organ is a lung.

22. The apparatus according to claim 1, further comprising a database coupled with said MPS and with said processor, said database storing at least said MPS data sets.

23. The apparatus according to claim 22, further comprising a medical imaging device coupled with said database, said medical imaging device including an image detector, said medical imaging device acquiring a plurality of two-dimensional images of said inspected organ via said image detector, said database further storing at least said plurality of two-dimensional images.

24. The apparatus according to claim 23, wherein one of said at least one reference electromagnetic transducer is attached to said image detector, obtaining external optical parameters relating to said medical imaging device.

25. The apparatus according to claim 23, wherein said medical imaging device includes an image acquisition system selected from the list consisting of:

ultrasound;  
intra-vascular ultrasound;

X-ray;  
 C-arm machine;  
 fluoroscopy;  
 angiography;  
 computerized tomography;  
 nuclear magnetic resonance;  
 positron-emission tomography; and  
 single-photon-emission tomography.

26. The apparatus according to claim 23, further comprising a display coupled with said processor, said display presenting a motion picture of said inspected organ, said motion picture presenting the trajectory of said surgical tool guided within said blood vessel, respective of different phases of said inspected organ.

27. The apparatus according to claim 26, wherein said display presents a single image frame in said motion picture, respective of the real-time activity-state of said inspected organ.

28. The apparatus according to claim 26, wherein said display presents a playback of previous images in said motion picture, showing progress of said surgical tool during previous activity-states of said inspected organ.

29. The apparatus according to claim 26, wherein said display is selected from the list consisting of:

a two-dimensional display;  
 an auto-stereoscopic display viewed with a suitable pair of spectacles;  
 a stand alone stereoscopic display; and  
 a pair of goggles.

30. The apparatus according to claim 26, wherein said display includes multiple monitors.

31. The apparatus according to claim 30, wherein one of said monitors presents current real-time three-dimensional position data of said surgical tool superimposed on the current image frame of said inspected organ respective of the current activity-state, while another of said monitors presents the current real-time three-dimensional position data of said surgical tool superimposed on a previous image frame of said inspected organ respective of a previous activity-state.

32. The apparatus according to claim 26, wherein said display includes separate windows within a single monitor.

33. The apparatus according to claim 32, wherein one of said windows presents current real-time three-dimensional position data of said surgical tool superimposed on the current image frame of said inspected organ respective of the current activity-state, while another of said windows presents the current real-time three-dimensional position data of said surgical tool superimposed on a previous image frame of said inspected organ respective of a previous activity-state.

34. The apparatus according to claim 1, wherein one of said at least one inner electromagnetic transducer is coupled with an image sensor.

35. The apparatus according to claim 1, further comprising an additional electromagnetic transducer coupled with an image sensor.

36. The apparatus according to claim 1, wherein said reference location is associated with an image sensor.

37. An apparatus for generating an organ timing signal relating to at least one inspected organ within a body of a patient, comprising: a medical positioning system (MPS), said medical positioning system transmitting and detecting electromagnetic signals between a reference location and a surgical tool inserted in the vicinity of said inspected organ, said medical positioning system determining a three-dimensional position of said surgical tool by processing said

transmitted electromagnetic signals with said detected electromagnetic signals, said medical positioning system further generating time-tagged MPS data sets, each of said MPS data sets comprising a collection of three-dimensional position coordinate readings wherein each of the readings is associated with a respective time at which the reading was obtained, the readings demonstrating the overall motion trajectory of said surgical tool over time; and

a processor, generating said organ timing signal from said MPS data sets by detecting and identifying periodic motion frequencies in said time-tagged MPS data sets, and by filtering said periodic motion frequencies from said MPS data sets so as to separate said periodic motion frequencies corresponding to said organ timing signal from said overall motion trajectory of said surgical tool.

38. Method for generating an organ timing signal relating to an inspected organ within a body of a patient, the method comprising the steps of:

transmitting electromagnetic signals and detecting said electromagnetic signals;  
 processing said transmitted electromagnetic signals with said detected electromagnetic signals;  
 determining the three-dimensional position of a surgical tool inserted within the body of the patient based on said processing;  
 generating MPS data sets comprising a collection of time-tagged three-dimensional position coordinate readings wherein each of the readings is associated with a respective time at which the reading was obtained, the readings demonstrating the overall motion trajectory of said surgical tool over time;  
 detecting and identifying periodic motion frequencies in said time-tagged MPS data sets; and  
 filtering said periodic motion frequencies from said MPS data sets so as to separate said periodic motion frequencies corresponding to said organ timing signal from said overall motion trajectory of said surgical tool.

39. The method according to claim 38, further comprising the steps of:

reconstructing a cardiac trajectory from said MPS data sets and said filtered periodic motion frequencies, said cardiac trajectory representing a mechanical movement of a blood vessel originating from cardiac motion;  
 reconstructing a respiratory trajectory from said MPS data sets and said filtered periodic motion frequencies, said respiratory trajectory representing a mechanical movement of said blood vessel originating from respiratory motion;

detecting phases of said inspected organ by identifying a plurality of phases on either of said reconstructed cardiac trajectory or said reconstructed respiratory trajectory; and

associating said phases with said MPS data sets, thereby obtaining phase information relating to said inspected organ.

40. The method according to claim 39, further comprising the step of:

acquiring a plurality of two-dimensional images of said inspected organ.

41. The method according to claim 40, further comprising the step of:

associating between said plurality of two-dimensional images, said MPS data sets, and said phase information.

42. The method according to claim 41, wherein said plurality of two-dimensional images are associated between

said MPS data sets, with respect to said phase information at the time of acquisition or measurement.

43. The method according to claim 41, wherein a given one of said plurality of two-dimensional images acquired during a given phase is associated with position coordinate readings detected during said given phase at any cycle of said cardiac trajectory.

44. The method according to claim 40, further comprising the steps of:

normalizing one of said MPS data sets;  
performing magnetic-optical correlation on said normalized MPS data sets;

performing optical projection on said correlated MPS data set, said correlated MPS data set comprising three-dimensional coordinate readings in an optical domain; and

superimposing said projected MPS data set onto a two-dimensional image selected from said acquired plurality of two-dimensional images, said projected MPS data set comprising two-dimensional coordinate readings in the optical domain,

thereby superimposing MPS data onto two-dimensional image data for corresponding data sets.

45. The method according to claim 40, further comprising the steps of:

obtaining phase information relating to said inspected organ from said MPS data sets for a first MPS data set selected from said MPS data sets, said first MPS data set being corresponding with a two-dimensional images data set;

obtaining phase information relating to said inspected organ from said MPS data sets for a second MPS data set selected from said MPS data sets, said second MPS data set being non-corresponding with said two-dimensional images data set; and

generating a third MPS data set from said second MPS data set using phase alignment between phases of said first MPS data set and said second MPS data set, said third MPS data set having the same time-tag as said first MPS data set.

46. The method according to claim 45, further comprising the steps of:

performing magnetic-optical correlation on said third MPS data set, said third MPS data set comprising three-dimensional coordinate readings in a magnetic domain;

performing optical projection on said correlated third MPS data set, said correlated third MPS data set comprising three-dimensional coordinate readings in an optical domain; and

superimposing said projected third MPS data set onto a two-dimensional image selected from said acquired plurality of two-dimensional images, said projected third MPS data set comprising two-dimensional coordinate readings in the optical domain,  
thereby superimposing MPS data onto two-dimensional image data for non-corresponding data sets.

47. The method according to claim 45, wherein said phase information is cardiac phase information.

48. The method according to claim 45, wherein said phase information is respiratory phase information.

49. The method according to claim 45, wherein said phase information is cardiac phase information and respiratory phase information.

50. The method according to claim 40, further comprising the steps of:

obtaining phase information relating to said inspected organ from said MPS data sets for a selected one of said MPS data sets;

obtaining correlated phase information for a two-dimensional images data set selected from said acquired plurality of two-dimensional images; and

generating a separate MPS data set for each two-dimensional image in said two-dimensional images data set, in accordance with image phase and time-tags.

51. The method according to claim 50, further comprising the steps of:

performing magnetic-optical correlation on each of said generated MPS data sets, each of said generated MPS data sets comprising three-dimensional coordinate readings in a magnetic domain;

performing optical projection on each of said correlated MPS data sets, each of said correlated MPS data sets comprising three-dimensional coordinate readings in an optical domain; and

superimposing each of said projected MPS data sets onto corresponding two-dimensional image selected from said two-dimensional images data set, said projected third MPS data set comprising two-dimensional coordinate readings in the optical domain,

thereby constructing trajectories of said surgical tool guided within a blood vessel in the vicinity of said inspected organ within the body of a patient, respective of different phases of said inspected organ.

52. The method according to claim 51, wherein said constructed trajectories are presented on a display.

53. The method according to claim 50, wherein said phase information is cardiac phase information.

54. The method according to claim 50, wherein said phase information is respiratory phase information.

55. The method according to claim 50, wherein said phase information is cardiac phase information and respiratory phase information.

56. The method according to claim 40, further comprising the steps of:

obtaining phase information relating to said inspected organ from said MPS data sets for a selected one of said MPS data sets;

reconstructing the centerline trajectory from said MPS data sets and said filtered periodic motion frequencies, said centerline trajectory representing the central axis of the guiding motion of said surgical tool;

reconstructing separate centerline trajectories for each phase, in accordance with time-tags and detected phases of said reconstructed cardiac trajectory;

obtaining correlated phase information for a two-dimensional images data set selected from said acquired plurality of two-dimensional images; and

shifting each of said centerline trajectories by superimposing matching periodic motion components, for each phase of the two-dimensional images in said two-dimensional images data set.

57. The method according to claim 56, further comprising the steps of:

performing magnetic-optical correlation on each of said shifted centerline trajectories, each of said shifted centerline trajectories comprising three-dimensional coordinate readings in a magnetic domain;

performing optical projection on each of said shifted centerline trajectories, each of said shifted centerline trajectories comprising three-dimensional coordinate readings in an optical domain; and

superimposing each of said shifted centerline trajectories onto corresponding two-dimensional image selected from said two-dimensional images data set, each of said shifted centerline trajectories comprising two-dimensional coordinate readings in the optical domain, 5 thereby constructing trajectories of said surgical tool guided within a blood vessel in the vicinity of said inspected organ within the body of a patient, respective of different phases of said inspected organ.

**58.** The method according to claim **57**, wherein said 10 constructed trajectories are presented on a display.

**59.** The method according to claim **56**, wherein said phase information is cardiac phase information.

**60.** The method according to claim **56**, wherein said phase information is respiratory phase information. 15

**61.** The method according to claim **56**, wherein said phase information is cardiac phase information and respiratory phase information.

**62.** The method according to claim **38**, wherein said inspected organ is a heart. 20

**63.** The method according to claim **38**, wherein said inspected organ is a lung.

\* \* \* \* \*

专利名称(译)	使用从MPS传感器生成的器官定时信号进行侵入式设备跟踪的方法和装置		
公开(公告)号	<a href="#">US9572519</a>	公开(公告)日	2017-02-21
申请号	US10/986567	申请日	2004-11-10
[标]申请(专利权)人(译)	MEDIGUIDE		
申请(专利权)人(译)	MEDIGUIDE LTD.		
当前申请(专利权)人(译)	MEDIGUIDE LTD.		
[标]发明人	SHMARAK ITZHAK STROMMER GERA EICHLER UZI		
发明人	SHMARAK, ITZHAK STROMMER, GERA EICHLER, UZI		
IPC分类号	A61B5/05 A61B5/11 A61B5/06 A61B8/02 A61B6/12 A61B5/00 A61B5/08 A61B5/0456 A61B6/00 A61N5/10 A61B17/00 A61B8/00 A61B8/08		
CPC分类号	A61B5/1107 A61B5/06 A61B5/7207 A61B5/7289 A61B6/527 A61B6/541 A61B6/547 A61B8/02 A61B8/0841 A61B8/5276 A61B34/20 A61B90/36 A61B2090/364 A61B2090/365 A61B2090/367 A61B2090/378 A61B2090/3958 A61B2505/05 A61N5/1067 A61B5/0456 A61B5/0816 A61B5/11 A61B5/721 A61B6/12 A61B6/503 A61B6/504 A61B8/0833 A61B8/0883 A61B8/0891 A61B8/4245 A61B8/4254 A61B34/10 A61B34/25 A61B90/10 A61B2017/00699 A61B2017/00703 A61B2034/105 A61B2034/107 A61B2034/2051 A61B2034/2055 A61B2034/2072 A61B2034/256 A61B5/061 A61B5/066 A61B5/1102 A61B5/1128 A61B5/113 A61B5/7275 A61B5/742 A61B6/032 A61B6/037 A61B8/12 A61B2034/2065 A61B2090/372		
其他公开文献	US20090182224A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

用于生成与患者体内的被检查器官相关的器官定时信号的装置，包括医疗定位系统和处理器。医学定位系统包括放置在参考位置处的至少一个参考电磁换能器，至少一个内部电磁换能器附接到插入在所检查的器官附近的血管中的外科工具，以及与换能器耦合的医疗定位系统处理器。医学定位系统处理器产生医学定位系统数据集，每个数据集包括展示外科工具随时间的运动轨迹的三维位置坐标读数的集合，处理器通过检测来自数据集的器官定时信号，识别所述数据集中的周期性运动频率，以及从所述数据集中过滤所述周期性运动频率。

