



US 20060264722A1

(19) **United States**

(12) **Patent Application Publication**
Hannula et al.

(10) **Pub. No.: US 2006/0264722 A1**

(43) **Pub. Date: Nov. 23, 2006**

(54) **HAT-BASED OXIMETER SENSOR**

Publication Classification

(76) Inventors: **Don Hannula, (US); Paul Mannheim, (US)**

(51) **Int. Cl.**
A61B 5/00 (2006.01)

(52) **U.S. Cl.** **600/340; 600/344**

Correspondence Address:

Michael G. Fletcher
FLETCHER YODER
P.O. Box 692289
Houston, TX 77269-2289 (US)

(57) **ABSTRACT**


A method for use and an improved oximeter sensor substrate that is conforming to the shape of the patient's forehead. In one embodiment, the present invention is an oximeter sensor, having a substrate with a shape similar to a shape of at least a portion of a patient's forehead and including a section adapted to substantially fit over a portion of a forehead of a patient; an emitter disposed on the substrate at a position located on the section; and a detector disposed on the substrate at a distance from the emitter. In one embodiment, the substrate includes a hat that holds the emitter and the detector in a spaced-part manner against the patient's forehead.

(21) Appl. No.: **11/494,357**

(22) Filed: **Jul. 26, 2006**

Related U.S. Application Data

(60) Continuation of application No. 11/358,868, filed on Feb. 21, 2006, which is a division of application No. 10/606,668, filed on Jun. 25, 2003, now Pat. No. 7,047,056.

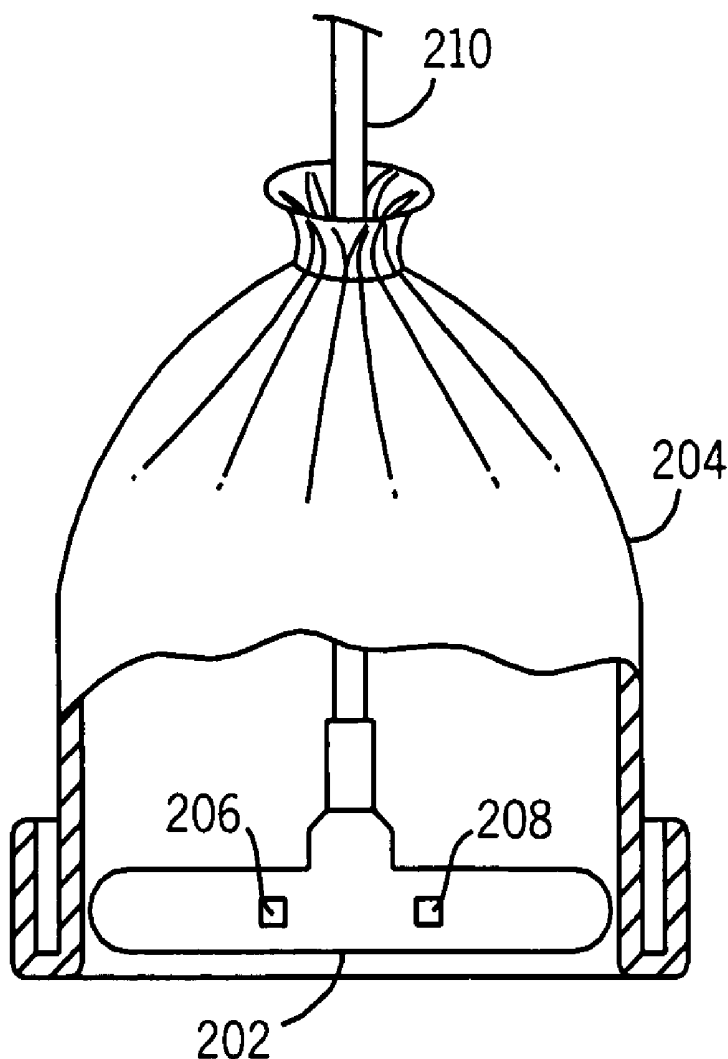

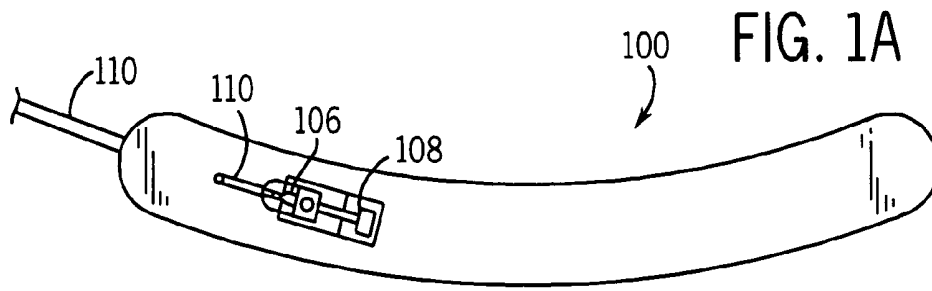


FIG. 1A

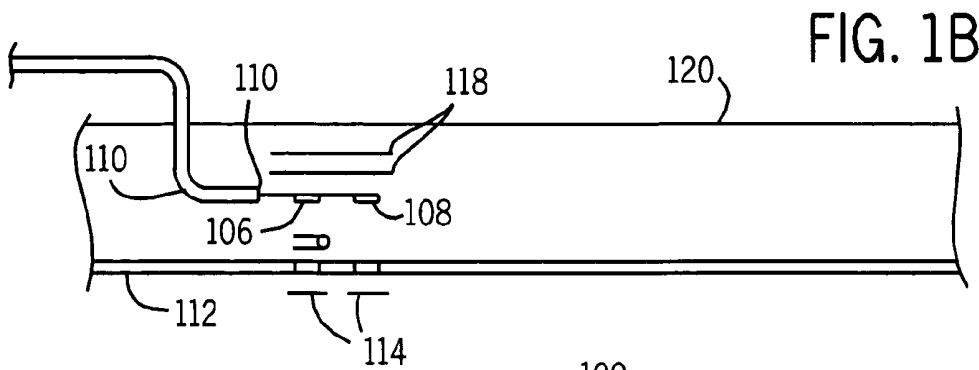


FIG. 1B

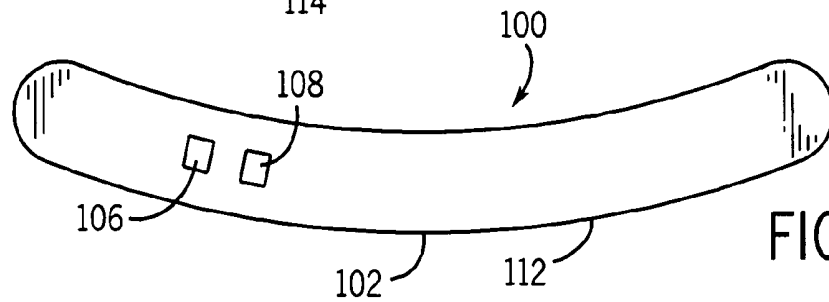


FIG. 1C

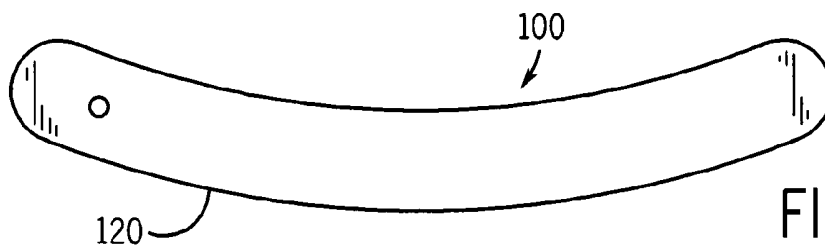


FIG. 1D

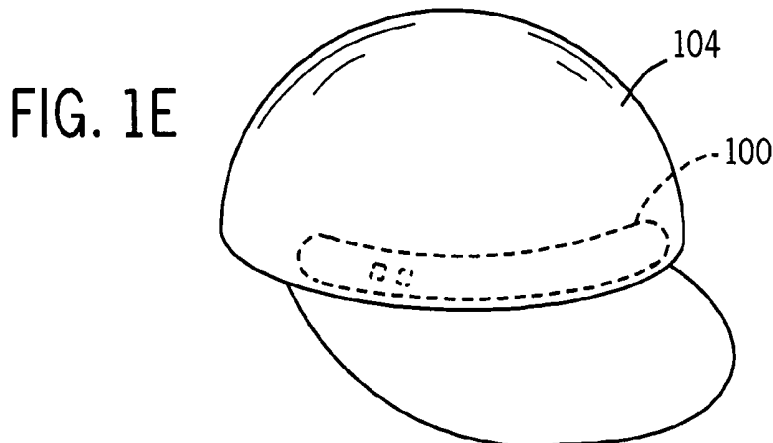


FIG. 1E

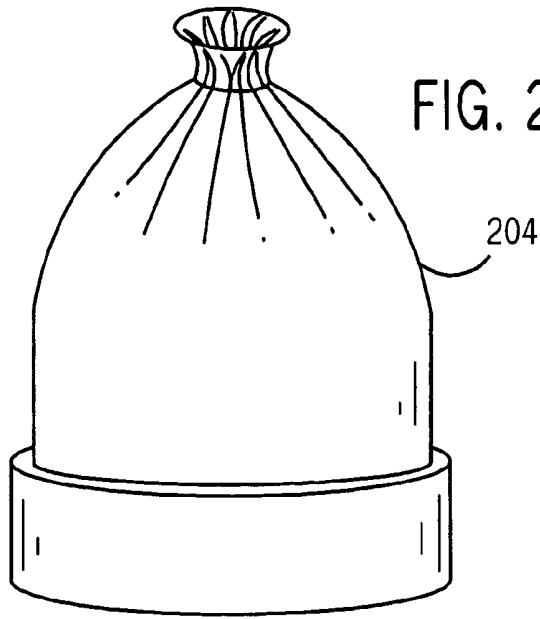


FIG. 2A

FIG. 2B

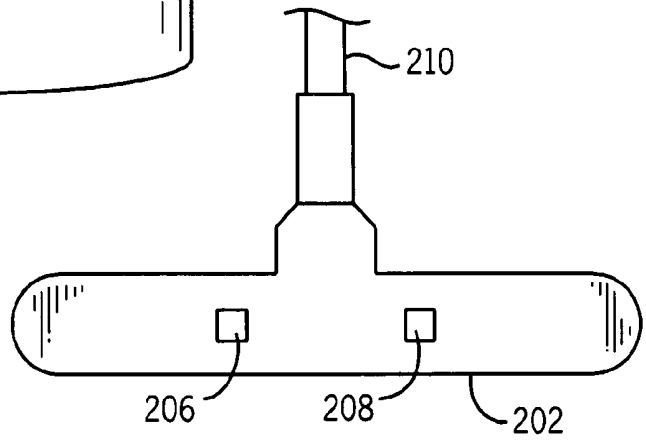
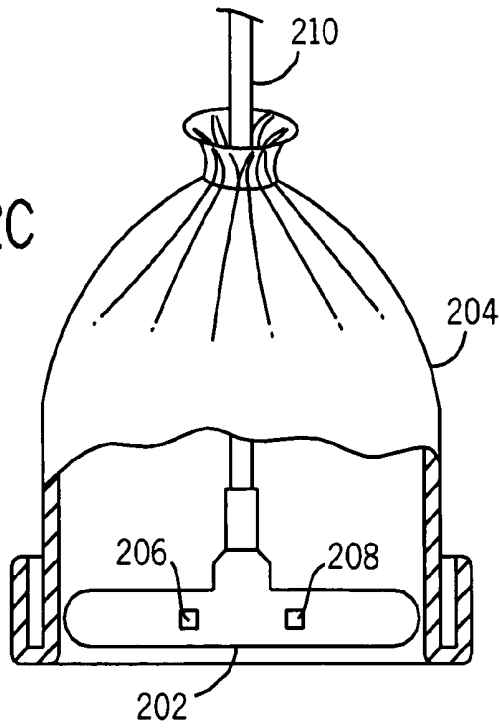


FIG. 2C



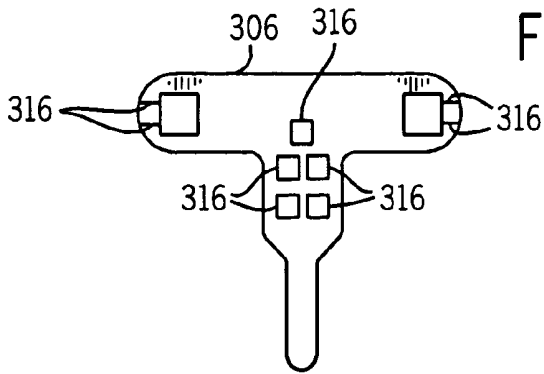


FIG. 3A

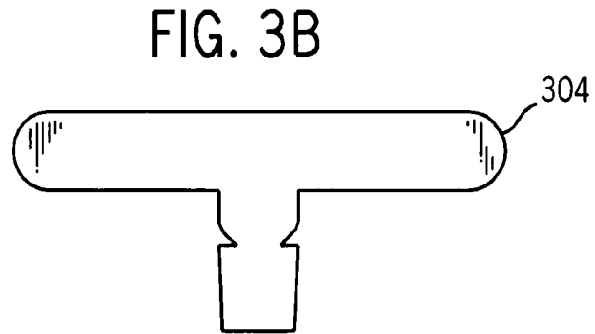


FIG. 3B

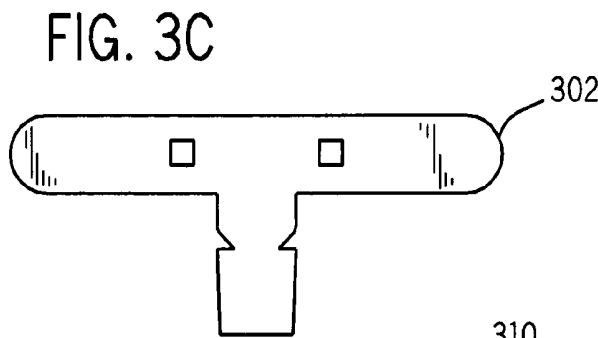


FIG. 3C

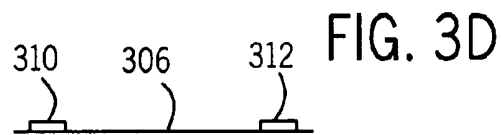


FIG. 3D

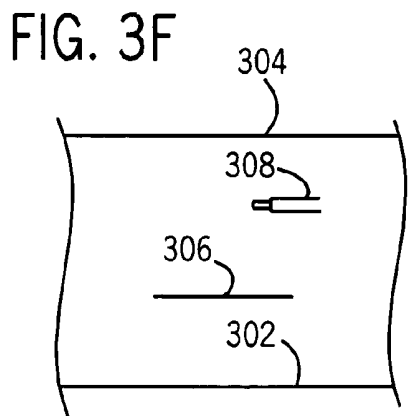


FIG. 3F

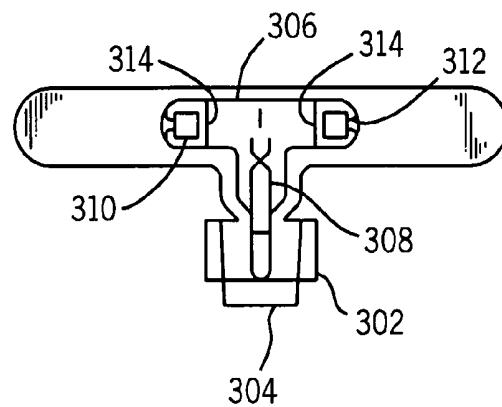


FIG. 3E

HAT-BASED OXIMETER SENSOR

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation of U.S. application Ser. No. 11/358,868 filed Feb. 21, 2006, the specification of which is hereby incorporated by reference in its entirety, which is a divisional of prior U.S. application Ser. No. 10/606,668, filed Jun. 25, 2003, now U.S. Pat. No. 7,047,056 issued May 16, 2006, the specification of which is incorporated by reference in its entirety.

BACKGROUND OF THE INVENTION

[0002] 1. Field of the Invention

[0003] The present invention relates to optical oximeter sensors, and in particular to hat-based pulse oximeter sensors.

[0004] Many types of optical sensors are used to measure physiological characteristics of a patient. Typically, an optical sensor provides emitted light which is then scattered through a portion of a patient's tissue and detected. Various characteristics of a patient can be determined from analyzing such light, such as oxygen saturation, pulse rate, tissue bilirubin, etc.

[0005] Pulse oximetry is typically used to measure various blood flow characteristics including, but not limited to, the blood-oxygen saturation of hemoglobin in arterial blood, the volume of individual blood pulsations supplying the tissue, and the rate of blood pulsations corresponding to each heartbeat of a patient. Measurement of these characteristics has been accomplished by use of a non-invasive sensor which scatters light through a portion of the patient's tissue where blood perfuses the tissue, and photoelectrically senses the absorption of light in such tissue. The amount of light absorbed is then used to calculate the amount of blood constituent being measured.

[0006] The light scattered through the tissue is selected to be of one or more wavelengths that are absorbed by the blood in an amount representative of the amount of the blood constituent present in the blood. The amount of transmitted light scattered through the tissue will vary in accordance with the changing amount of blood constituent in the tissue and the related light absorption. For measuring blood oxygen level, such sensors have typically been provided with a light source that is adapted to generate light of at least two different wavelengths, and with photodetectors sensitive to both of those wavelengths, in accordance with known techniques for measuring blood oxygen saturation.

[0007] Known non-invasive sensors include devices that are secured to a portion of the body, such as a finger, an ear or the scalp. In animals and humans, the tissue of these body portions is perfused with blood and the tissue surface is readily accessible to the sensor.

[0008] Certain types of oximeter sensors are applied to a patient's forehead. To aid in the sensor's proper placement and the proper application of pressure by the sensor to the forehead site, some forehead sensors are maintained at the forehead site by either the assistance of an adhesive layer and/or a headband. While these approaches are helpful, there

is still a need for an improved and easy way of placing, retaining, and locating the sensor on the forehead of its user.

BRIEF SUMMARY OF THE INVENTION

[0009] The present invention provides an oximeter sensor which will attach to a patient's forehead in an improved manner. In certain embodiments, the securing of the sensor to the forehead of the patient is achieved by attaching the sensor to the inside of hat which is worn by the patient when the sensor is in use.

[0010] In one embodiment, the present invention is an oximeter sensor, having: a substrate having a shape similar to a shape of at least a portion of a patient's forehead and including a section adapted to substantially fit over a portion of a forehead of a patient; an emitter disposed on the substrate at a position located on the section; and a detector disposed on the substrate at a distance from the emitter.

[0011] In one embodiment, the substrate is resilient and has a shape conformable to the forehead of a patient.

[0012] In one embodiment, the substrate includes an adhesive layer for adhering to the forehead of a patient.

[0013] In one embodiment, a hat is used for holding the sensor against the patient's forehead.

[0014] In one embodiment, the substrate is adhered to the inside of said hat.

[0015] In one embodiment, the substrate is adhesively attached to the inside of the hat. Alternately, the substrate is sewn into the hat.

[0016] In another embodiment, the present invention provides a method for determination of a blood characteristic, including: applying an emitter and a detector to spaced-apart positions on a forehead of a patient in the lower forehead region, above the eyebrow, with both the detector and the emitter placed above and predominantly lateral of the iris; securing the emitter and detector to the patient; emitting electromagnetic radiation with the emitter; detecting electromagnetic radiation scattered by the tissues of the forehead by the detector and producing a detector signal; and determining a blood characteristic in the patient from the detector signal.

[0017] In one embodiment, the securing of the emitter and the detector to the patient's forehead is achieved by attaching the emitter and the detector to an inside of a hat, and placing the hat on the head of the patient.

[0018] For a further understanding of the nature and advantages of the present invention, reference should be made to the following description in conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0019] **FIG. 1** is an assembly drawing of an embodiment of the sensor in accordance with the present invention that can be placed within a hat or cap.

[0020] **FIG. 2** is a drawing of a stocking hat, with an embodiment of the sensor in accordance with the present invention shown mounted in the hat.

[0021] **FIG. 3** is an assembly drawing of an embodiment of the sensor of **FIG. 1** or **2**.

DETAILED DESCRIPTION OF THE
INVENTION

[0022] The embodiments of the present invention are directed towards configuring a reflectance-type oximeter sensor for placement in a hat in order to provide a relatively easy means of placing, retaining, and locating the sensor on the forehead of the user. With regard to the location of the sensor on the patient's forehead, it is preferred to have the sensor be located on the lower forehead region, above the eyebrow, with the sensor optics (emitter and detector) located above and predominantly lateral to or centered over the iris. The oximeter sensor can be attached to the inside band of a hat. The precise location of the reflectance sensor in the hat allows appropriate placement of the sensor in the optimal forehead location by a user not skilled in sensor placement. It has been found that the placement of a reflectance forehead sensor is a factor in the accurate determination of a blood flow characteristic, due to the vasculature of the forehead. In addition, it has been shown that having a certain amount of pressure on the forehead sensor can reduce the incidence of venous pulsations effects on the oximeter reading. The placement of the sensor in the band of the hat would minimize these issues, as the placement of a hat is fairly repeatable and predictable. A hat-based oximeter sensor as embodied by the present invention can be used on patients in clinical settings, or by athletes, soldiers, firemen, or in any environment where information related to a physiological parameter, such as heart rate or oxygen saturation information is desired.

[0023] FIG. 1 is an assembly drawing of an embodiment of the sensor in accordance with the present invention that can be placed within a hat or cap. This figure shows an oximeter sensor placed on a substrate 102 that can be placed or adhered to the inside of a hat 104. In the hat-based embodiment, the sensor uses an emitter 106 containing two discrete wavelengths and a detector 108 placed more than 2 mm away, and ideally 10 mm-15 mm from the emitter. The surface 102 can be black in order to minimize any shunting of light between sensor and patient skin. The sensor in a hat could be used in conjunction with a small, portable oximeter to allow mobility of the user during activities. Similarly, the sensor could be incorporated into a headband. Alternately, it may be desirable to provide a sensor with adhesive backing that would allow the user to place the sensor in a hat of their choice. Also shown in FIG. 1 is a cable 110 for providing drive current to the LED and for providing the detector signal to the oximeter. The cable provides the electrical connection to the monitor; it also provides power for the emitter, signal carrying conductors from the detector, and shielding to protect the small signals from the detector against external electrical interference.

[0024] The sensor is shown in a multi-layer structure having a face portion 112. The face 112 is the surface that is placed against the patient's skin. The face material may have an adhesive layer such as an acrylic or synthetic rubber adhesive, or it may be without adhesive, and typically made from a foam PVC or foam polyurethane material. The face 112 component is preferably black so as to minimize the incidence of reflected light that does not go through the tissue. Below the face layer 112 are two windows 114. The windows 114 are generally a clear component, such as for example, a thin film or a clear molded plastic component that makes contact with the skin. The thin film window may

be a polyurethane or an acrylic adhesive on a polyester film. The intent of the window 114 is to provide an efficient optical coupling mechanism between the optical components (emitter and detector) and the skin. Located above the face 114, is a Faraday shield 116. The Faraday shield 116 is a conductive material, for example, a copper film or copper mesh, that is electrically connected to the monitor ground to help shield the detector from extraneous electrical interference while passing light to the detector. Next located are the LED 106 and the detector 108. Above the LED and the detector is a mask layer, which may include more than one mask layer. The mask layer 118 is generally a thin film that is intended to block light from entering the back side of the sensor, or from traveling directly from emitter to detector (shunt light). The purpose of the mask 118 is to ensure that all of the light reaching the detector is light from the emitter that has traveled through the capillary bed. Above the mask layer 118 is the back layer 120. The back or the top layer is the non-tissue contacting surface of the sensor. This layer may include a cosmetic finish for the sensor, which can be white with some printed artwork identifying the sensor. Typical materials may be Velcro loop, or soft PVC foam. In a case where the sensor is mounted inside a hat or cap, the top layer is sometimes referred to as the back layer. In this case, the back layer may include a double stick adhesive so that it can be mounted inside the hat.

[0025] FIG. 2 shows a stocking hat, with an embodiment of the sensor in accordance with the present invention shown mounted in the hat. This alternate embodiment of the present invention, is directed towards the placement of a small reflectance sensor 202 in a stocking cap or beanie 204. FIG. 2 shows the sensor carrier layer 202 holding an LED 206 and a detector 208 and a cable 210, similar to the ones described above in conjunction with FIG. 1. This embodiment may be used for neonates. This embodiment would allow easy placement of a sensor on the forehead of a patient while applying a predictable pressure on the sensor. The sensor in a hat also resolves a concern about the cosmetic appearance of having a sensor on the forehead of the patient. A sensor in a stocking cap is much more acceptable to a parent than having a sensor located on the forehead. Depending on the tension of the stocking cap, provided by its own stretchiness or by an adjustable integral headband strap, the sensor may have a light tack adhesive, or no adhesive at all. The lack of an adhesive layer is a desirable feature, especially on neonates as adhesives may sometimes leave visible damage to the fragile skin of a neonate.

[0026] FIG. 3 is an assembly drawing for an embodiment of the sensor of FIG. 1 or 2. FIG. 3 shows that the sensor portion generally includes a face layer 302, a top layer 304 and a flex circuit 306 that is placed between the face and top layers. Also shown in FIG. 3 is a multi-layer unassembled view showing the relative positions of the face 302, flex circuit 306, a cable 308 and the top layer 304. The flex circuit layer 306 holds the emitter (LED) 310 and the detector 312 as well as the mask layer 314 and Faraday shield as described above. The flex circuit 306 also has several holes 316 to allow for electrical connections between the leads in the cable and the LED and the detector.

[0027] As will be understood by those skilled in the art, the present invention may be embodied in other specific forms without departing from the essential characteristics thereof. For example, the sensor may include adhesive

layers for adhering to the inside of a hat or the user's skin, or that that the sensor may be sewn into the hat. These other embodiments are intended to be included within the scope of the present invention, which is set forth in the following claims.

What is claimed is:

1. A sensor comprising:
 - a stocking cap;
 - a substrate disposed on the stocking cap; and
 - at least one sensing component disposed on the substrate, wherein the sensing component is adapted to be located in a lower forehead region when the stocking cap is applied to a patient.
2. The sensor of claim 1, wherein the substrate is conformable to a forehead-contacting surface of the stocking cap.
3. The sensor of claim 1, wherein the substrate comprises an adhesive layer adapted to attach the substrate to the stocking cap.
4. The sensor of claim 1, wherein the stocking cap comprises a neonatal stocking cap.
5. The sensor of claim 1, wherein the stocking cap comprises an opening adapted to accommodate the sensor.
6. The sensor of claim 7, wherein the opening comprises a hole or a pocket.
7. The sensor of claim 1, comprising an electrical connector extending from the substrate through an open portion of the stocking cap when the stocking cap is applied to the patient.
8. The sensor of claim 1, wherein the sensing component comprises at least one of an emitter or a detector.
9. The sensor of claim 1, wherein the stocking cap comprises one or more alignment indicia for aligning the substrate to the lower forehead region.
10. The sensor of claim 1, wherein the sensing component is adapted to be centered substantially above the patient's iris when the stocking cap is applied to the patient.
11. A method of manufacturing a cap-based sensor comprising:
 - providing a stocking cap;
 - providing a substrate, and
 - providing at least one sensing component disposed on the substrate, wherein the sensing component adapted to be located in a lower forehead region when the stocking cap is applied to a patient.
12. The method of claim 11, wherein the substrate is conformable to a forehead-contacting surface of the stocking cap.
13. The method of claim 11, comprising providing an adhesive layer adapted to attach the substrate to the stocking cap.

14. The method of claim 11, wherein the stocking cap comprises a neonatal stocking cap.

15. The method of claim 11, comprising providing an opening adapted to accommodate the sensor.

16. The method of claim 15, wherein the opening comprises a hole or a pocket.

17. The method of claim 11, comprising providing an electrical connector extending from the substrate through an open portion of the stocking cap when the stocking cap is applied to the patient.

18. The method of claim 17, wherein the at least a portion of the electrical connector comprises a cable.

19. The method of claim 11, wherein the sensing component comprises at least one of an emitter or a detector.

20. The method of claim 11, wherein the sensing component is adapted to be located substantially centered above a patient's iris when the stocking cap is applied to the patient.

21. A method of applying a sensor comprising:

applying a stocking cap to a patient, wherein the stocking cap comprises a substrate and at least one sensing component disposed on the substrate;

and

aligning the sensing component to a lower forehead region when the stocking cap is applied to the patient.

22. The method of claim 21, wherein the sensing component comprises at least one of an emitter or a detector.

23. The method of claim 21, wherein the substrate is conformable to a forehead-contacting surface of the stocking cap.

24. The method of claim 21, wherein the stocking cap comprises an adhesive layer adapted to attach the substrate to the stocking cap.

25. The method of claim 21, wherein the stocking cap comprises a neonatal stocking cap.

26. The method of claim 21, wherein the stocking cap comprises an opening adapted to accommodate the sensor.

27. The method of claim 26, wherein the opening comprises a hole or a pocket.

28. The method of claim 21, wherein the stocking cap comprises an electrical connector extending from the substrate through an open portion of the stocking cap when the stocking cap is applied to the patient.

29. The method of claim 21, wherein the at least a portion of the electrical connector comprises a cable.

30. The method of claim 21, comprising aligning the sensing component to a position substantially centered above a patient's iris.

* * * * *

专利名称(译)	基于帽子的血氧计传感器		
公开(公告)号	US20060264722A1	公开(公告)日	2006-11-23
申请号	US11/494357	申请日	2006-07-26
[标]申请(专利权)人(译)	HANNULA DON MANNHEIMER PAUL		
申请(专利权)人(译)	HANNULA DON MANNHEIMER PAUL		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	HANNULA DON MANNHEIMER PAUL		
发明人	HANNULA, DON MANNHEIMER, PAUL		
IPC分类号	A61B5/00		
CPC分类号	A61B5/14552 A61B5/14553 A61B2503/06 A61B5/6814 A61B5/6833 A61B5/6804		
其他公开文献	US7809420		
外部链接	Espacenet USPTO		

摘要(译)

一种使用方法和改进的血氧计传感器基板，其符合患者前额的形状。在一个实施例中，本发明是一种血氧计传感器，其具有基板，该基板的形状类似于患者前额的至少一部分的形状，并且包括适于基本上配合在患者前额的一部分上的部分；发射器，设置在基板上位于该部分上的位置；探测器设置在距离发射器一定距离的基板上。在一个实施例中，基板包括帽子，该帽子以间隔开的方式将发射器和检测器保持在患者的前额上。

