



US 20070032711A1

(19) **United States**(12) **Patent Application Publication** (10) **Pub. No.: US 2007/0032711 A1**
(43) **Pub. Date: Feb. 8, 2007**(54) **MEDICAL SENSOR AND TECHNIQUE FOR USING THE SAME****Publication Classification**(76) Inventors: **Joseph Coakley**, Dublin, CA (US);
George L. Matlock, Pleasanton, CA (US); **William Raridan**, Pleasanton, CA (US); **Darius D. Eghbal**, Oakland, CA (US)(51) **Int. Cl.**
A61B 5/00 (2006.01)
(52) **U.S. Cl.** **600/323**(57) **ABSTRACT**Correspondence Address:
FLETCHER YODER (TYCO INTERNATIONAL, LTD.)
P.O. BOX 692289
HOUSTON, TX 77269-2289 (US)

A sensor assembly is provided that includes a frame having two or more structural supports. A coating is provided over the frame. The coating has at least one deformable region disposed between the two or more structural supports. As least one optical component is disposed within the at least one deformable region such that the at least one optical component can move relative to the two or more structural supports. A biasing component is attached to an end of the frame such that at least two different portions of the coated frame are biased closed in the absence of a sufficient opening force. The sensor may be placed on a patient's finger, toe, ear, and so forth to obtain pulse oximetry or other physiological measurements. A skeletal frame and a method for manufacturing a skeletal framework are also provided.

(21) Appl. No.: **11/494,838**(22) Filed: **Jul. 28, 2006****Related U.S. Application Data**

(63) Continuation of application No. 11/199,524, filed on Aug. 8, 2005.

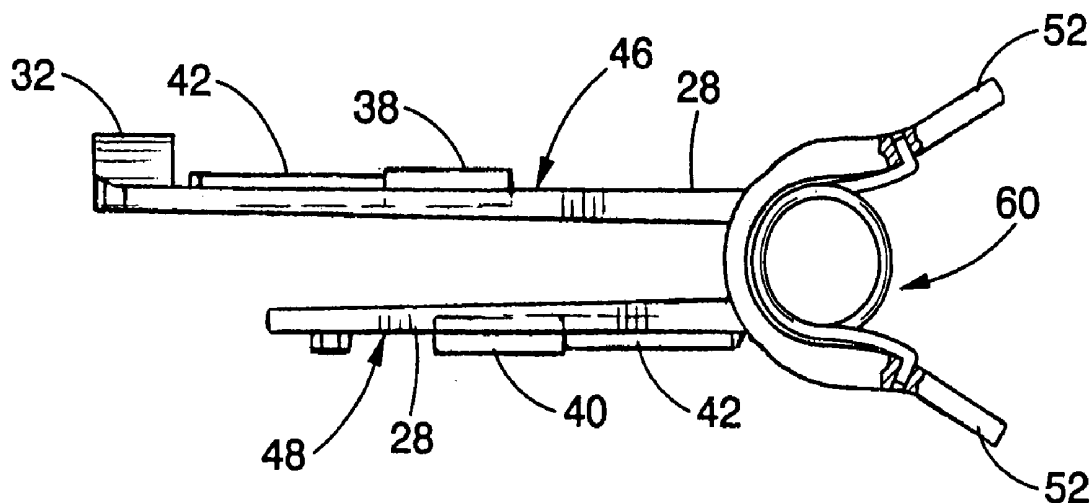
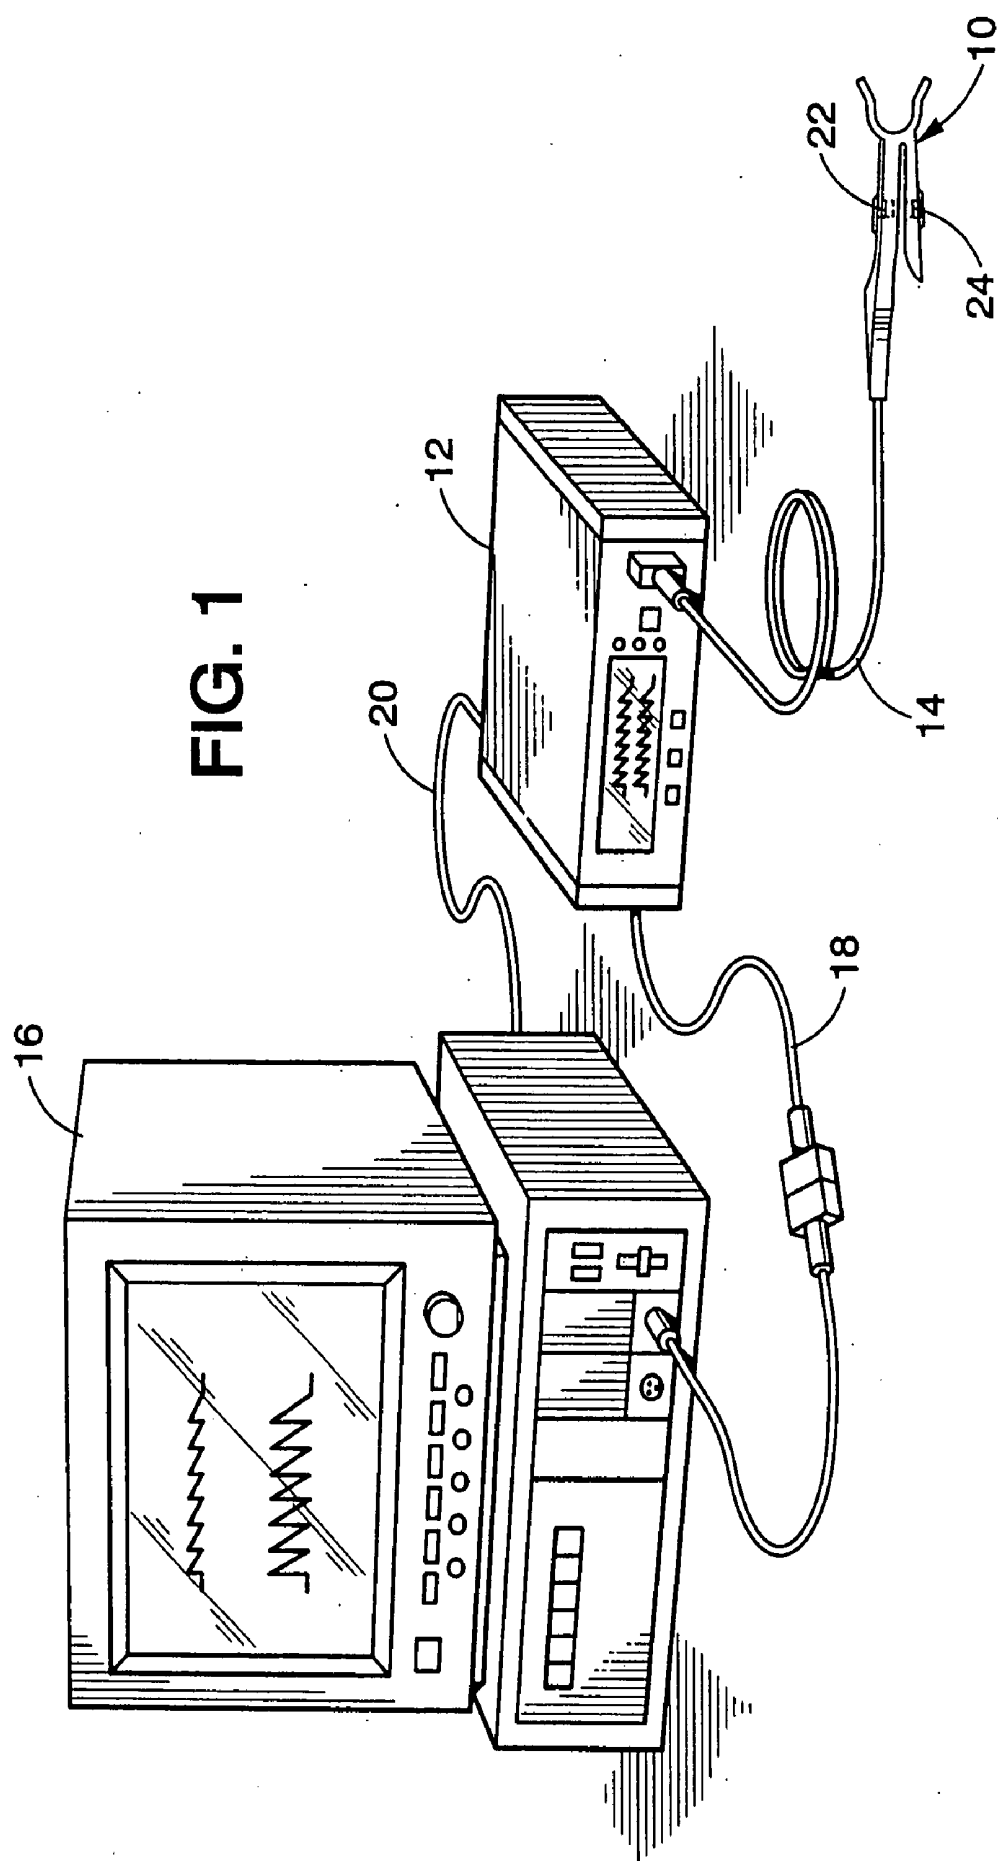
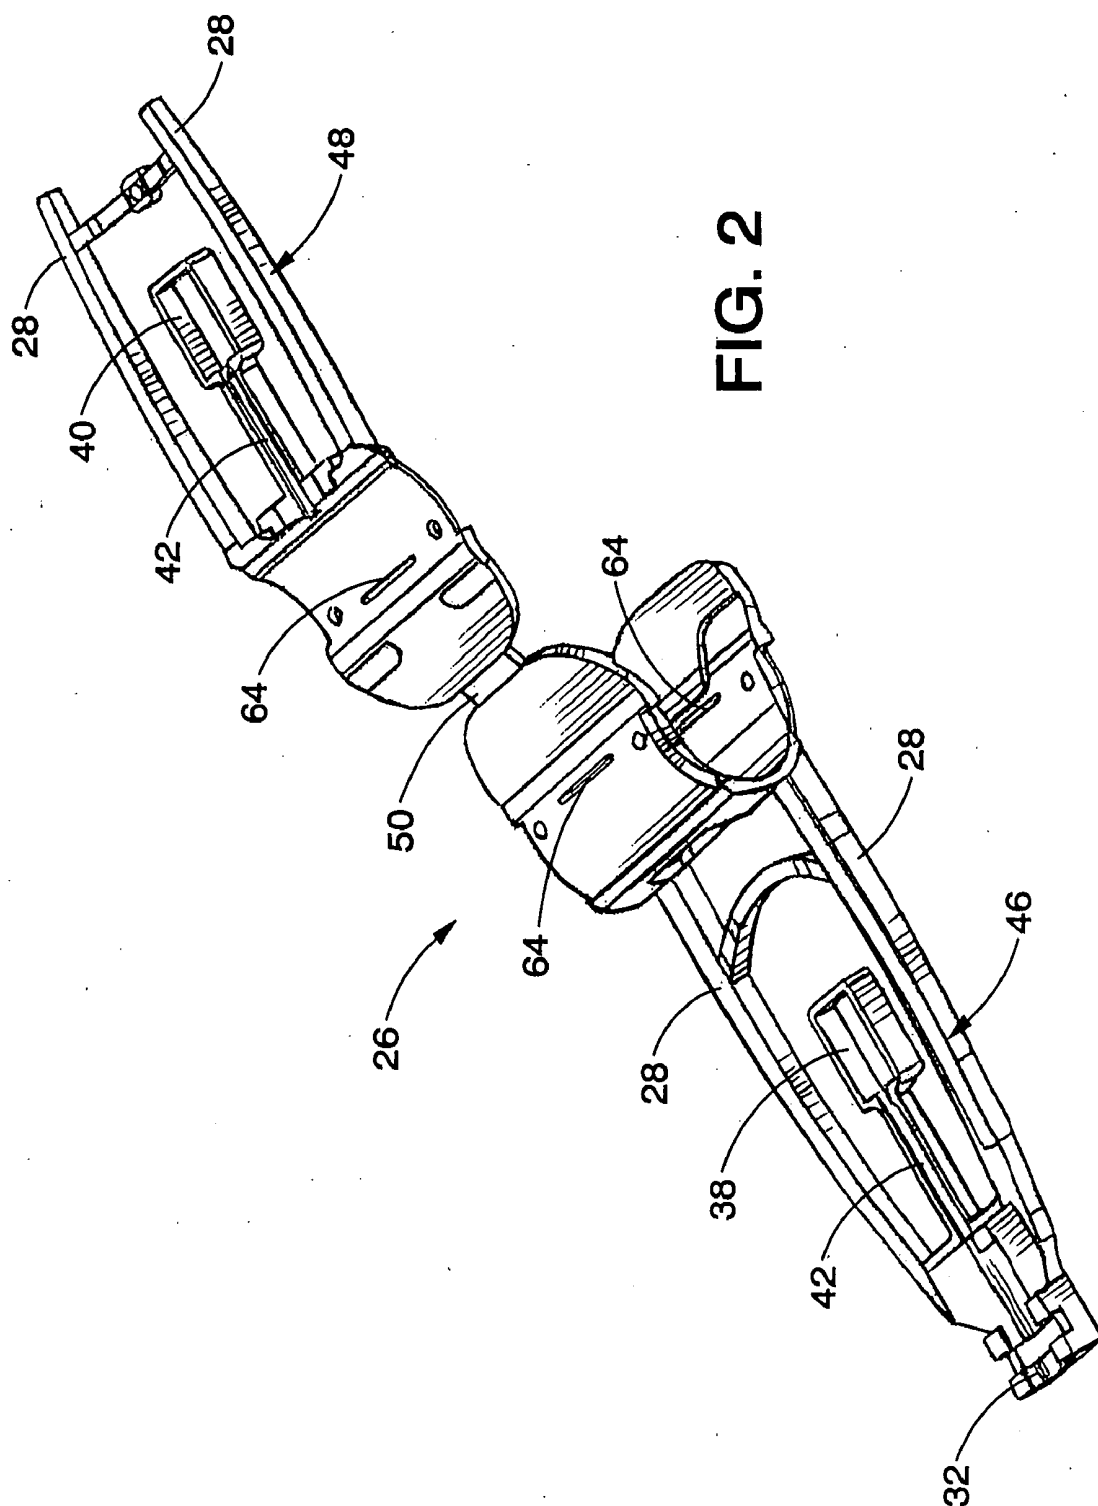
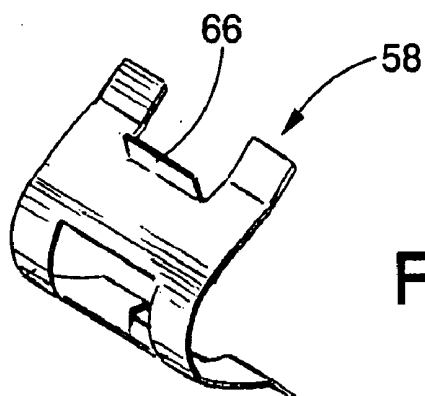
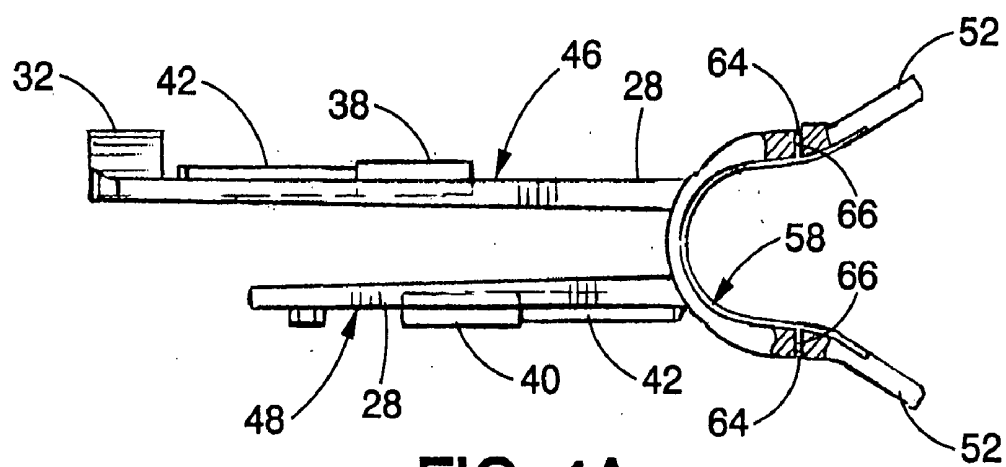
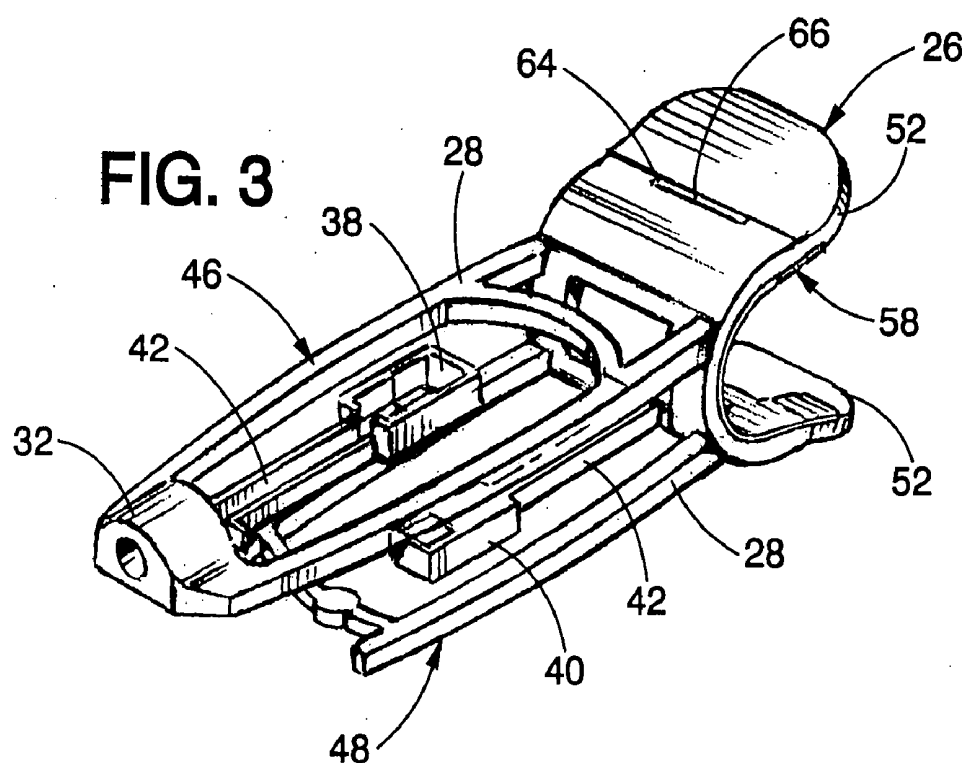


FIG. 1







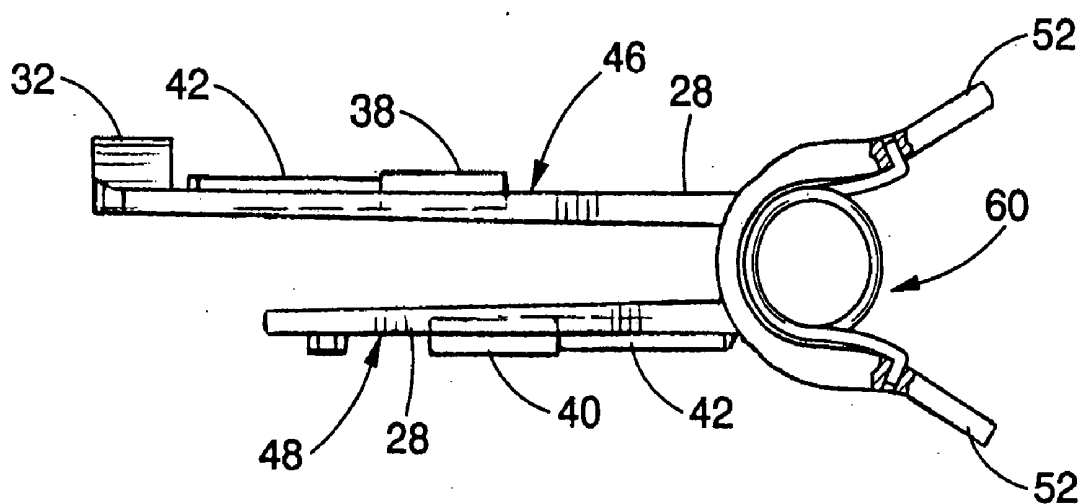


FIG. 5A

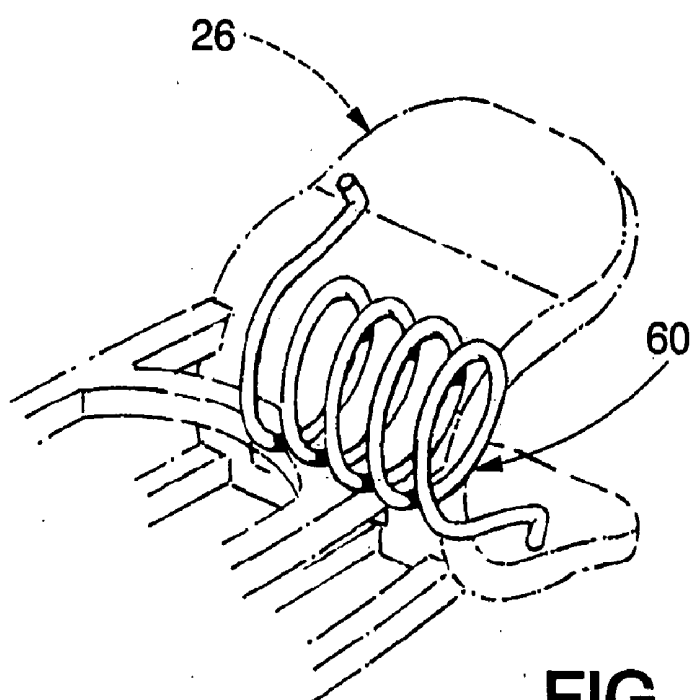


FIG. 5B

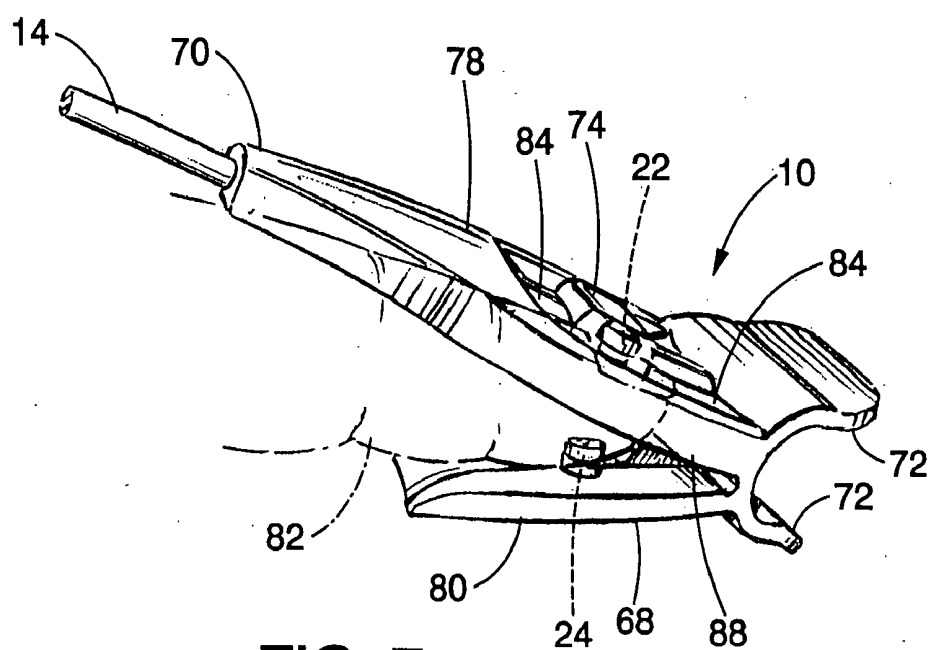
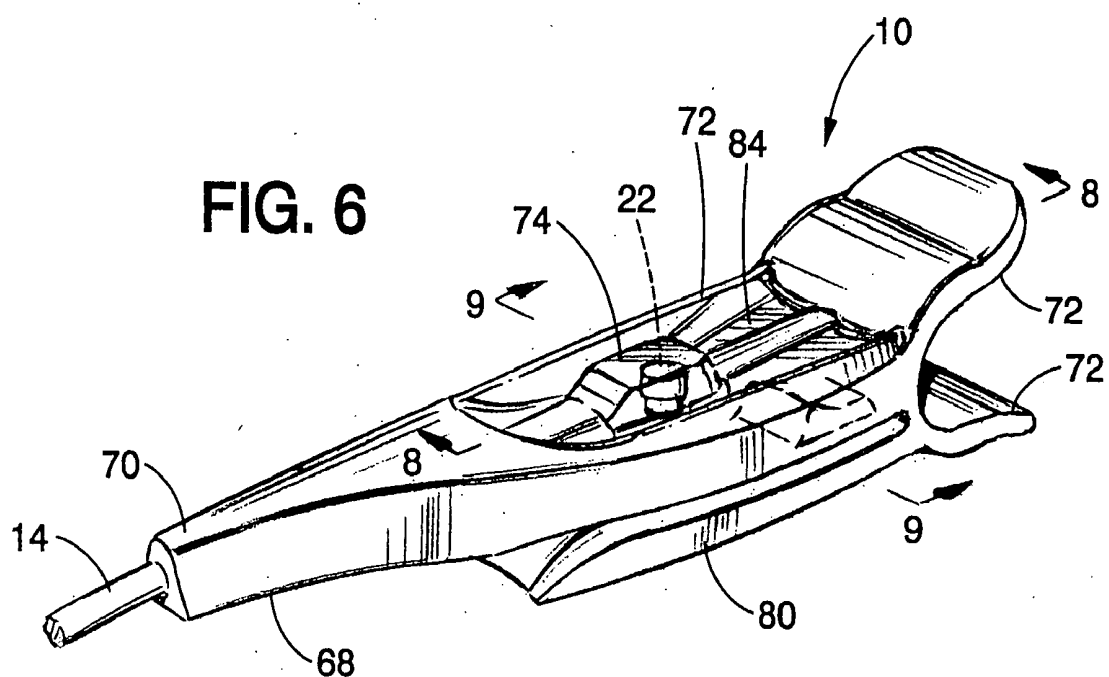


FIG. 7


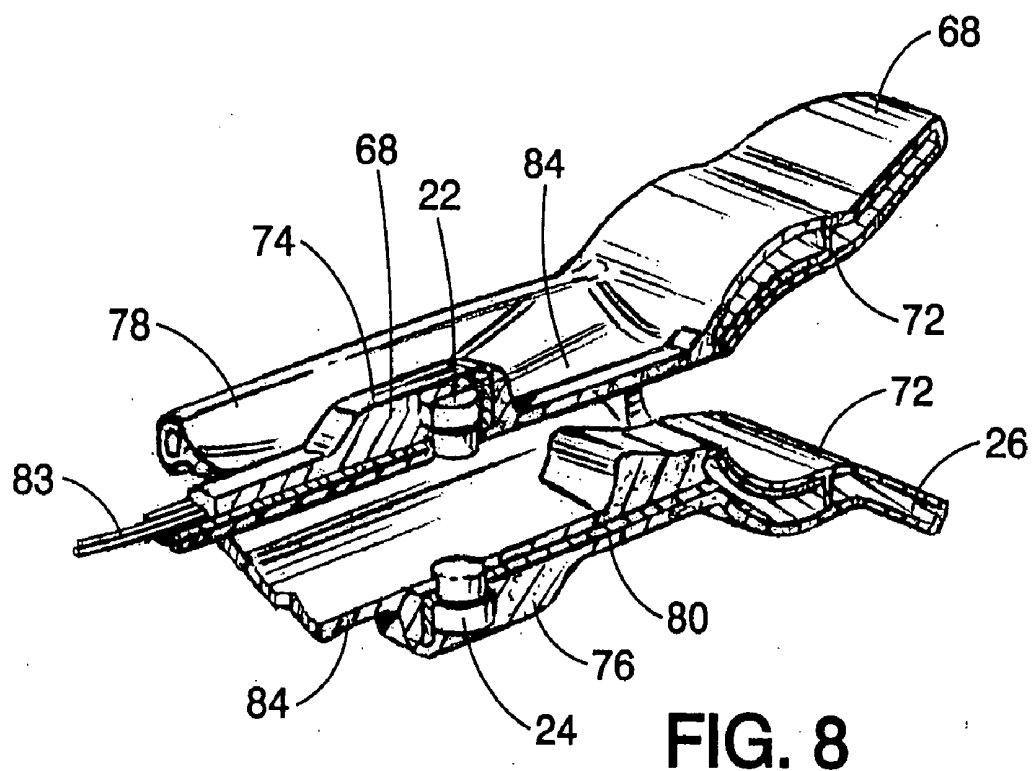


FIG. 9

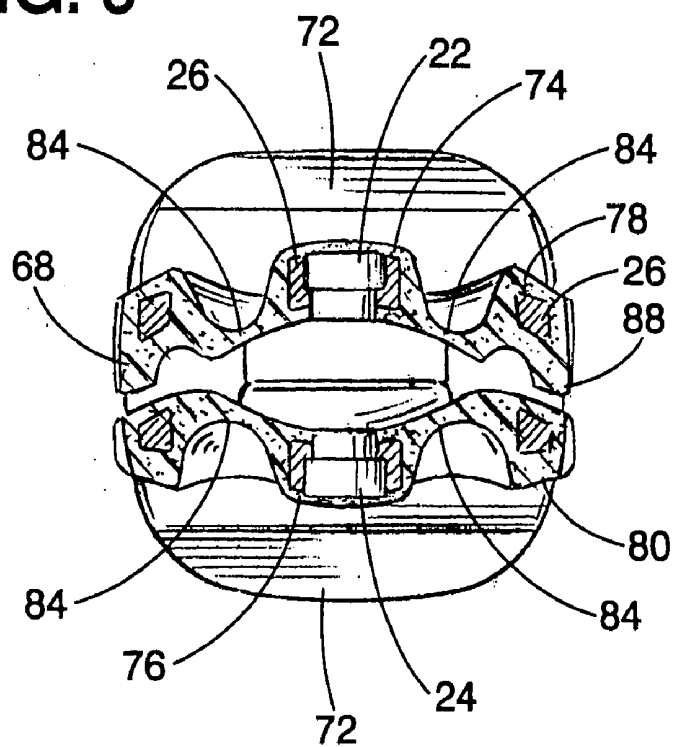

MEDICAL SENSOR AND TECHNIQUE FOR USING THE SAME

CROSS-REFERENCE TO RELATED APPLICATION

[0001] This application is a continuation of U.S. application Ser. No. 11/199,524 filed Aug. 8, 2005, the disclosure of which is hereby incorporated by reference in its entirety.

BACKGROUND OF THE INVENTION

[0002] 1. Field of the Invention

[0003] The present invention relates generally to medical devices and, more particularly, to sensors used for sensing physiological parameters of a patient.

[0004] 2. Description of the Related Art

[0005] This section is intended to introduce the reader to various aspects of art that may be related to various aspects of the present invention, which are described and/or claimed below. This discussion is believed to be helpful in providing the reader with background information to facilitate a better understanding of the various aspects of the present invention. Accordingly, it should be understood that these statements are to be read in this light, and not as admissions of prior art.

[0006] In the field of medicine, doctors often desire to monitor certain physiological characteristics of their patients. Accordingly, a wide variety of devices have been developed for monitoring physiological characteristics. Such devices provide doctors and other healthcare personnel with the information they need to provide the best possible healthcare for their patients. As a result, such monitoring devices have become an indispensable part of modern medicine.

[0007] One technique for monitoring certain physiological characteristics of a patient is commonly referred to as pulse oximetry, and the devices built based upon pulse oximetry techniques are commonly referred to as pulse oximeters. Pulse oximetry may be used to measure various blood flow characteristics, such as the blood-oxygen saturation of hemoglobin in arterial blood, the volume of individual blood pulsations supplying the tissue, and/or the rate of blood pulsations corresponding to each heartbeat of a patient.

[0008] Pulse oximeters typically utilize a non-invasive sensor that is placed on or against a patient's tissue that is well perfused with blood, such as a patient's finger, toe, forehead or earlobe. The pulse oximeter sensor emits light and photoelectrically senses the absorption and/or scattering of the light after passage through the perfused tissue. The data collected by the sensor may then be used to calculate one or more of the above physiological characteristics based upon the absorption or scattering of the light. More specifically, the emitted light is typically selected to be of one or more wavelengths that are absorbed or scattered in an amount related to the presence of oxygenated versus deoxygenated hemoglobin in the blood. The amount of light absorbed and/or scattered may then be used to estimate the amount of the oxygen in the tissue using various algorithms.

[0009] In many instances, it may be desirable to employ, for cost and/or convenience, a pulse oximeter sensor that is reusable. Such reusable sensors, however, may be uncom-

fortable for the patient for various reasons. For example, the materials used in their construction may not be adequately compliant or supple or the structural features may include angles or edges.

[0010] Furthermore, the reusable sensor should fit snugly enough that incidental patient motion will not dislodge or move the sensor, yet not so tight that it may interfere with pulse oximetry measurements. Such a conforming fit may be difficult to achieve over a range of patient physiologies without adjustment or excessive attention on the part of medical personnel. In addition, lack of a tight or secure fit may allow light from the environment to reach the photo-detecting elements of the sensor. Such environmental light is not related to a physiological characteristic of the patient and may, therefore, introduce error into the measurements derived using data obtained with the sensor.

[0011] Reusable pulse oximeter sensors are also used repeatedly and, typically, on more than one patient. Therefore, over the life of the sensor, detritus and other bio-debris (sloughed off skin cells, dried fluids, dirt, and so forth) may accumulate on the surface of the sensor or in crevices and cavities of the sensor, after repeated uses. As a result, it may be desirable to quickly and/or routinely clean the sensor in a thorough manner. However, in sensors having a multi-part construction, as is typical in reusable pulse oximeter sensors, it may be difficult to perform such a quick and/or routine cleaning. For example, such a thorough cleaning may require disassembly of the sensor and individual cleaning of the disassembled parts or may require careful cleaning using utensils capable of reaching into cavities or crevices of the sensor. Such cleaning is labor intensive and may be impractical in a typical hospital or clinic environment.

SUMMARY

[0012] Certain aspects commensurate in scope with the originally claimed invention are set forth below. It should be understood that these aspects are presented merely to provide the reader with a brief summary of certain forms the invention might take and that these aspects are not intended to limit the scope of the invention. Indeed, the invention may encompass a variety of aspects that may not be set forth below.

[0013] There is provided a sensor assembly that includes: a frame comprising two or more structural supports; a coating provided over the frame, wherein the coating comprises at least one deformable region disposed between the two or more structural supports; at least one optical component disposed within the at least one deformable region, such that the at least one optical component can move relative to the two or more structural supports; and a biasing component attached to an end of the frame such that at least two different portions of the coated frame are biased closed in the absence of a sufficient opening force.

[0014] There is also provided a skeletal frame of a sensor that includes: two or more structural support members having one or more spaces between the two or more structural support members, wherein the two or more structural support members are configured to provide support to an overlying coating when present.

[0015] There is also provided a method for manufacturing a skeletal framework of a sensor that includes: forming two

or more structural support members of a skeletal frame of a sensor having one or more spaces between the two or more structural support members, wherein the two or more structural support members are configured to provide support to an overlying coating when present.

BRIEF DESCRIPTION OF THE DRAWINGS

[0016] Advantages of the invention may become apparent upon reading the following detailed description and upon reference to the drawings in which:

[0017] FIG. 1 illustrates a patient monitoring system coupled to a multi-parameter patient monitor and a sensor, in accordance with aspects of the present technique;

[0018] FIG. 2 illustrates a perspective view of an internal frame for use in a patient sensor, in accordance with aspects of the present technique;

[0019] FIG. 3 illustrates a perspective view of the internal frame of FIG. 2 in a closed configuration, in accordance with aspects of the present technique;

[0020] FIG. 4A illustrates a side view of the internal frame of FIG. 3;

[0021] FIG. 4B illustrates a flat spring for use with the internal frame of FIGS. 2-4A, in accordance with aspects of the present technique;

[0022] FIG. 5A illustrates a side view of another internal frame for use in a patient sensor, in accordance with aspects of the present technique;

[0023] FIG. 5B illustrates a torsion spring for use with the internal frame of FIG. 5A, in accordance with aspects of the present technique;

[0024] FIG. 6 illustrates a perspective view of an overmolded patient sensor, in accordance with aspects of the present technique;

[0025] FIG. 7 illustrates the overmolded patient sensor of FIG. 6 in use on a patient's finger, in accordance with aspects of the present technique;

[0026] FIG. 8 illustrates a cross-section taken along section line 8-8 of the overmolded patient sensor depicted in FIG. 6; and

[0027] FIG. 9 illustrates a cross-section taken along section line 9-9 of the overmolded patient sensor depicted in FIG. 6.

DETAILED DESCRIPTION OF SPECIFIC EMBODIMENTS

[0028] One or more specific embodiments of the present invention will be described below. In an effort to provide a concise description of these embodiments, not all features of an actual implementation are described in the specification. It should be appreciated that in the development of any such actual implementation, as in any engineering or design project, numerous implementation-specific decisions must be made to achieve the developers' specific goals, such as compliance with system-related and business-related constraints, which may vary from one implementation to another. Moreover, it should be appreciated that such a development effort might be complex and time consuming, but would nevertheless be a routine undertaking of design,

fabrication, and manufacture for those of ordinary skill having the benefit of this disclosure.

[0029] It is desirable to provide a comfortable and conformable reusable patient sensor, such as for use in pulse oximetry or other applications utilizing spectrophotometry, that is easily cleaned and that is resistant to environmental light infiltration. In accordance with some aspects of the present technique, a reusable patient sensor is provided that is overmolded to provide patient comfort and a suitably conformable fit. The overmold material provides a seal against bodily fluids, as well as water or other cleaning fluids, that allows easy cleaning without disassembly or special tools. In accordance with some aspects of the present technique, the reusable patient sensor includes a mechanism providing a biasing force, such as a metal flat spring or a torsion spring, to facilitate the secure placement of the sensor on a patient.

[0030] Prior to discussing such exemplary sensors in detail, it should be appreciated that such sensors are typically designed for use with a patient monitoring system. For example, referring now to FIG. 1, a sensor 10 according to the present invention may be used in conjunction with a patient monitor 12. In the depicted embodiment, a cable 14 connects the sensor 10 to the patient monitor 12. As will be appreciated by those of ordinary skill in the art, the sensor 10 and/or the cable 14 may include or incorporate one or more integrated circuit devices or electrical devices, such as a memory, processor chip, or resistor, that may facilitate or enhance communication between the sensor 10 and the patient monitor 12. Likewise the cable 14 may be an adaptor cable, with or without an integrated circuit or electrical device, for facilitating communication between the sensor 10 and various types of monitors, including older or newer versions of the patient monitor 12 or other physiological monitors. In other embodiments, the sensor 10 and the patient monitor 12 may communicate via wireless means, such as using radio, infrared, or optical signals. In such embodiments, a transmission device (not shown) may be connected to the sensor 10 to facilitate wireless transmission between the sensor 10 and the patient monitor 12. As will be appreciated by those of ordinary skill in the art, the cable 14 (or corresponding wireless transmissions) are typically used to transmit control or timing signals from the monitor 12 to the sensor 10 and/or to transmit acquired data from the sensor 10 to the monitor 12. In some embodiments, however, the cable 14 may be an optical fiber that allows optical signals to be conducted between the monitor 12 and the sensor 10.

[0031] In one embodiment, the patient monitor 12 may be a suitable pulse oximeter, such as those available from Nellcor Puritan Bennett Inc. In other embodiments, the patient monitor 12 may be a monitor suitable for measuring tissue water fractions, or other body fluid related metrics, using spectrophotometric or other techniques. Furthermore, the monitor 12 may be a multi-purpose monitor suitable for performing pulse oximetry and measurement of tissue water fraction, or other combinations of physiological and/or biochemical monitoring processes, using data acquired via the sensor 10. Furthermore, to upgrade conventional monitoring functions provided by the monitor 12 to provide additional functions, the patient monitor 12 may be coupled to a multi-parameter patient monitor 16 via a cable 18

connected to a sensor input port and/or via a cable 20 connected to a digital communication port.

[0032] The sensor 10, in the example depicted in FIG. 1, is a clip-style sensor that is overmolded to provide a unitary or enclosed assembly. The sensor 10 includes an emitter 22 and a detector 24 which may be of any suitable type. For example, the emitter 22 may be one or more light emitting diodes adapted to transmit one or more wavelengths of light, such as in the red to infrared range, and the detector 24 may be a photodetector, such as a silicon photodiode package, selected to receive light in the range emitted from the emitter 22. In the depicted embodiment, the sensor 10 is coupled to a cable 14 that is responsible for transmitting electrical and/or optical signals to and from the emitter 22 and detector 24 of the sensor 10. The cable 14 may be permanently coupled to the sensor 10, or it may be removably coupled to the sensor 10—the latter alternative being more useful and cost efficient in situations where the sensor 10 is disposable.

[0033] The sensor 10 described above is generally configured for use as a “transmission type” sensor for use in spectrophotometric applications, though in some embodiments it may instead be configured for use as a “reflectance type sensor.” Transmission type sensors include an emitter and detector that are typically placed on opposing sides of the sensor site. If the sensor site is a fingertip, for example, the sensor 10 is positioned over the patient’s fingertip such that the emitter and detector lie on either side of the patient’s nail bed. For example, the sensor 10 is positioned so that the emitter is located on the patient’s fingernail and the detector is located opposite the emitter on the patient’s finger pad. During operation, the emitter shines one or more wavelengths of light through the patient’s fingertip, or other tissue, and the light received by the detector is processed to determine various physiological characteristics of the patient.

[0034] Reflectance type sensors generally operate under the same general principles as transmittance type sensors. However, reflectance type sensors include an emitter and detector that are typically placed on the same side of the sensor site. For example, a reflectance type sensor may be placed on a patient’s fingertip such that the emitter and detector are positioned side-by-side. Reflectance type sensors detect light photons that are scattered back to the detector.

[0035] For pulse oximetry applications using either transmission or reflectance type sensors the oxygen saturation of the patient’s arterial blood may be determined using two or more wavelengths of light, most commonly red and near infrared wavelengths. Similarly, in other applications a tissue water fraction (or other body fluid related metric) or a concentration of one or more biochemical components in an aqueous environment may be measured using two or more wavelengths of light, most commonly near infrared wavelengths between about 1,000 nm to about 2,500 nm. It should be understood that, as used herein, the term “light” may refer to one or more of infrared, visible, ultraviolet, or even X-ray electromagnetic radiation, and may also include any wavelength within the infrared, visible, ultraviolet, or X-ray spectra.

[0036] Pulse oximetry and other spectrophotometric sensors, whether transmission-type or reflectance-type, are typically placed on a patient in a location conducive to mea-

surement of the desired physiological parameters. For example, pulse oximetry sensors are typically placed on a patient in a location that is normally perfused with arterial blood to facilitate measurement of the desired blood characteristics, such as arterial oxygen saturation measurement (SaO_2). Common pulse oximetry sensor sites include a patient’s fingertips, toes, forehead, or earlobes. Regardless of the placement of the sensor 10, the reliability of the pulse oximetry measurement is related to the accurate detection of transmitted light that has passed through the perfused tissue and has not been inappropriately supplemented by outside light sources or modulated by subdermal anatomic structures. Such inappropriate supplementation and/or modulation of the light transmitted by the sensor can cause variability in the resulting pulse oximetry measurements.

[0037] As noted above, the overmolded sensor 10 discussed herein may be configured for either transmission or reflectance type sensing. For simplicity, the exemplary embodiment of the sensor 10 described herein is adapted for use as a transmission-type sensor. As will be appreciated by those of ordinary skill in the art, however, such discussion is merely exemplary and is not intended to limit the scope of the present technique.

[0038] Referring now to FIG. 2, an internal frame 26 for a sensor 10 is depicted. In the depicted example, the internal frame 26 is a skeletal frame for the sensor 10. Such a skeletal frame may include different structures or regions that may or may not have similar rigidities. For example, the depicted skeletal frame includes structural supports 28 that define the general shape of the sensor 10 when coated, as discussed below with regard to FIGS. 6-9. In view of their structure providing function, the structural supports 28 may be constructed to be substantially rigid or semi-rigid. In addition, the skeletal frame may include a cable guide 32 through which a cable, such as an electrical or optical cable, may pass to connect to the electrical or optical conductors attached to the emitter 22 and/or detector 24 upon assembly. Likewise, a skeletal frame, such as the depicted internal frame 26, may include component housings, such as the emitter housing 38 and detector housing 40 and struts 42 attaching such housings to the remainder of the skeletal frame. The struts 42 may be relatively flexible, allowing the emitter housing 38 and/or the detector housing 40 to move vertically (such as along an optical axis between the respective housings) relative to the structural supports 28 of the skeletal frame. Alternatively, in embodiments where the struts 42 are relatively rigid, where multiple struts 42 are employed to attach the housings 38 and 40 to the structural supports 28, or where the internal frame is substantially solid instead of skeletal, the housings 38 and/or 40 may be fixed relative to the respective structural supports 28 and, therefore, move with the structural supports 28.

[0039] In embodiments where the internal frame 26 is skeletal, the various structural supports 28, housings 38 and 40, struts 42, and other structures may define various openings and spaces between and/or around the structures of the skeletal frame. In this manner, the skeletal frame provides structural support at specific locations for a coating or overmolding. However, in regions where structural support is not provided, flexibility and freedom of motion in an overlying coating or overmolding may be possible. For example, in one implementation, the emitter housing 38 and/or the detector housing 40 may be attached to the

remainder of the skeletal frame by flexible struts **42**, as depicted in FIGS. 2-4. In such implementations, a coating provided proximate to the emitter housing **38** and/or detector housing **40** may be sufficiently flexible (such as due to the elasticity and/or the thinness of the coating material in the open areas of the skeletal frame) such that the housings **38** and **40** may move independent of the structural supports **28** of the frame **26** along an optical axis between the housings **38** and **40**.

[0040] In certain embodiments, the internal frame **26** is constructed, in whole or in part, from polymeric materials, such as thermoplastics, capable of providing a suitable rigidity or semi-rigidity for the different portions of the internal frame **26**. Examples of such suitable materials include polypropylene and nylon, though other polymeric materials may also be suitable. For example, in one embodiment, the internal frame **26** is constructed from polyurethane having a durometer of 65 Shore D. In other embodiments, the internal frame **26** is constructed, in whole or in part, from other suitably rigid or semi-rigid materials, such as stainless steel, aluminum, magnesium, graphite, fiberglass, or other metals, alloys, or compositions that are sufficiently ductile and/or strong. For example, metals, alloys, or compositions that are suitable for diecasting, sintering, lost wax casting, stamping and forming, and other metal or composition fabrication processes may be used to construct the internal frame **26**.

[0041] In addition, the internal frame **26** may be constructed as an integral structure or as a composite structure. For example, in one embodiment, the internal frame **26** may be constructed as a single piece from a single material or from different materials. Alternatively, the internal frame **26** may be constructed or assembled from two or more parts that are separately formed. In such embodiments, the different parts may be formed from the same or different materials. For example, in implementations where different parts are formed from different materials, each part may be constructed from a material having suitable mechanical and/or chemical properties for that part. The different parts may then be joined or fitted together to form the internal frame **26**.

[0042] In addition, the internal frame **26** may be molded, formed, or constructed in a different configuration than the final sensor configuration. For example, referring now to FIG. 2, the internal frame **26** for use in the sensor **10** may be initially formed in a generally open, or flat, configuration compared to the relatively closed configuration of the internal frame **26** when folded to form the sensor **10**. In such embodiments, a top portion **46** and a bottom portion **48** of the frame **26** may be formed in a generally open or planar configuration in which the two portions **46** and **48** are connected by a connective portion **50**.

[0043] For example, the top portion **46**, bottom portion **48**, and connective portion **50** may be molded or formed as a single piece in an open configuration. In such an embodiment, the connective portion **50** may be broken or deformed to bring the top portion **46** and bottom portion **48** into a closed configuration, as depicted in FIGS. 3, 4A, and 5A. In this implementation, the top portion **46** and bottom portion **48** may be secured together, such as via a snap fitting process, ultrasonic welding, or heat staking or by application of an adhesive or mechanical fastener.

[0044] Alternatively, the internal frame **26** may be formed as multiple parts that are joined together to form the internal frame **26**. For example, the top portion **46**, bottom portion **48**, tabs **52** and/or the connective portion **50** may be molded or formed separately and subsequently secured together to form the internal frame **26**. The different parts of the internal frame **26** may be joined together using one or more of the techniques noted above, such as a snap fitting process, ultrasonic welding, or heat staking or by application of an adhesive or mechanical fastener. If the internal frame **26** is secured together in an open configuration, the connective portion **50** may be broken or deformed to bring the top portion **46** and bottom portion **48** into a closed configuration, as depicted in FIGS. 3A, and 5A. Alternatively, the internal frame **26** may be constructed in a closed configuration from the separately molded or formed parts, such as the top portion **46**, bottom portion **48**, and/or tabs **52**.

[0045] In certain embodiments, the internal frame **26** is fitted with a spring or other biasing component, such as a formed flat spring **58** (as depicted in FIGS. 3, 4A, and 4B) or a torsion spring **60** (as depicted in FIGS. 5A and 5B). As will be appreciated by those of ordinary skill in the art, such biasing components may include elastic bodies or devices that may be distorted and that recover their original shape when released after being distorted. Similarly, a component or material that can store energy and release the energy to provide a gripping force, as described herein, may function as a spring or biasing component. For example, an over-molding material or composition, as discussed with regard to FIGS. 6-9, may have sufficient elasticity to function as a biasing component as discussed herein, with or without the additional gripping force provided by a component such as the flat spring **58** or the torsion spring **60**. For the purpose of this example, however, the sensor **10** is provided with and discussed as including a flat spring **58** (in FIGS. 3 and 4A) or a torsion spring **60** (in FIG. 5A).

[0046] Referring to FIGS. 3 and 4A, a flat spring **58** is fitted at or near the end of the internal frame **26** that is opposite from where the finger, toe, or other patient appendage is inserted into the assembled sensor. In alternative embodiments, the flat spring **58** connects two different portions or halves of the internal frame **26** to form the internal frame **26**. In the depicted embodiment, slots **64** are provided in the internal frame **26** that are engaged by complementary spring tabs **66** to fit the flat spring **58** to the internal frame **26**. For example, in an embodiment in which the internal frame **26** is molded or formed as a relatively open, single-piece, as depicted in FIG. 2, the internal frame **26** may be bent from the relatively open configuration to a closed configuration, as depicted in FIGS. 3 and 4A. The flat spring **58** may be fitted or attached to the internal frame **26** when in the closed configuration to provide a biasing force that maintains the internal frame **26** in the closed configuration. Referring now to FIG. 5A, the torsion spring **60** may be similarly fitted or attached to the internal frame **26** when in the closed configuration to provide a biasing force that maintains the internal frame **26** in the closed configuration.

[0047] The flat spring **58** or torsion spring **60** may be constructed from a variety of materials or combinations of materials that provide the desired resiliency and clamping force. For example, in certain embodiments, the flat spring **58** or torsion spring **60** may be constructed from a metal alloy, such as stainless steel. In one such stainless steel flat

spring embodiment, the flat spring **58** may be made from 301 high yield stainless steel that is 0.010 inch thick and that produces approximately 1.25 pounds of force at the optic plane (that is a plane through the emitter **22** and detector **24**) with a finger pad separation of approximately 15 mm. In other embodiments, the flat spring **58** or torsion spring **60** may be constructed from materials such as plastics, polymers, composites, and so forth that provide the desired resilience and elasticity.

[0048] An overmolded sensor **10** (as discussed with regard to FIGS. 6-9) incorporating a flat spring **58**, a torsion spring **60**, or other biasing component, disposed on the internal frame **26** may be opened for placement on a patient's finger, toe, ear, or other appendage by applying a force to separate the top portion **46** and bottom portion **48** of the internal frame **26**. For example, the flat spring **58** (in FIGS. 3 and 4A) or the torsion spring **60** (in FIG. 5A) provide or contribute to a closing force biasing the top portion **46** and the bottom portion **48** of the frame **26** together. An opposing force, however, may be applied to force the top portion **46** and bottom portion **48** apart. In the example depicted, an opposing force may be applied to projections, such as tabs **52**, provided at the end of the internal frame **26** to which the flat spring **58** or torsion spring **60** is fitted such that the force provided by the respective spring is overcome. In this manner, the tabs **52** are moved toward one another while the top portion **46** and bottom portion **48** are moved apart from one another.

[0049] As noted above, in certain embodiments of the present technique, the frame **26** (such as a skeletal internal frame) is coated to form a unitary or integral sensor assembly, as depicted in FIGS. 6-9. Such overmolded embodiments may result in a sensor assembly in which the internal frame **26** is completely or substantially coated. In embodiments in which the internal frame **26** is formed or molded as a relatively open or flat structure, the overmolding or coating process may be performed prior to or subsequent to bending the internal frame **26** into the closed configuration.

[0050] For example, the sensor **10** may be formed by an injection molding process. In one example of such a process the internal frame **26** may be positioned within a die or mold of the desired shape for the sensor **10**. A molten or otherwise unset overmold material may then be injected into the die or mold. For example, in one implementation, a molten thermoplastic elastomer at between about 400° F. to about 450° F. is injected into the mold. The overmold material may then be set, such as by cooling for one or more minutes or by chemical treatment, to form the sensor body **5** about the internal frame **26**. In certain embodiments, other sensor components, such as the emitter **22** and/or detector **24**, may be attached or inserted into their respective housings or positions on the overmolded sensor body.

[0051] Alternatively, the optical components (such as emitter **22** and detector **24**) and/or conductive structures (such as wires or flex circuits) may be placed on the internal frame **26** prior to overmolding. The internal frame **26** and associated components may then be positioned within a die or mold and overmolded, as previously described. To protect the emitter **22**, detector **24**, and/or other electrical components, conventional techniques for protecting such components from excessive temperatures may be employed. For example, the emitter **22** and/or the detector **24** may include

an associated clear window, such as a plastic or crystal window, in contact with the mold to prevent coating from being applied over the window. In one embodiment, the material in contact with such windows may be composed of a material, such as beryllium copper, which prevents the heat of the injection molding process from being conveyed through the window to the optical components. For example, in one embodiment, a beryllium copper material initially at about 40° F. is contacted with the windows associated with the emitter **22** and/or detector **24** to prevent coating of the windows and heat transfer to the respective optical components. As will be appreciated by those of ordinary skill in the art, the injection molding process described herein is merely one technique by which the frame **26** may be coated to form a sensor body, with or without associated sensing components. Other techniques which may be employed include, but are not limited to, dipping the frame **26** into a molten or otherwise unset coating material to coat the frame **26** or spraying the frame **26** with a molten or otherwise unset coating material to coat the frame **26**. In such implementations, the coating material may be subsequently set, such as by cooling or chemical means, to form the coating. Such alternative techniques, to the extent that they may involve high temperatures, may include thermally protecting whatever optical components are present, such as by using beryllium copper or other suitable materials to prevent heat transfer through the windows associated with the optical components, as discussed above.

[0052] By such techniques, the frame **26**, as well as the optical components and associated circuitry where desired, may be encased in a coating material **68** to form an integral or unitary assembly with no exposed or external moving parts of the internal frame **26**. For example, as depicted in FIG. 6, the sensor **10** includes features of the underlying internal frame **26** that are now completely or partially overmolded, such as the overmolded external cable guide **70**, tabs **72**, emitter housing **74**, and detector housing **76**. In addition, the overmolded sensor **10** includes an overmolded upper portion **78** and lower portion **80** that may be fitted to the finger **82** of a patient (as depicted in FIG. 7), or to the toe, ear, or other appendage of the patient, as appropriate.

[0053] In one implementation, the overmolding or coating **68** is a thermoplastic elastomer or other conformable coating or material. In such embodiments, the thermoplastic elastomer may include compositions such as thermoplastic polyolefins, thermoplastic vulcanizate alloys, silicone, thermoplastic polyurethane, and so forth. In one embodiment, the overmolding material is polyurethane having a durometer of 15 Shore A. As will be appreciated by those of ordinary skill in the art, the overmolding composition may vary, depending on the varying degrees of conformability, durability, wettability, or other physical and/or chemical traits that are desired. Furthermore, the coating material **68** may be selected to provide additional spring force to that provided by the biasing component (such as flat spring **58** or torsion spring **60**).

[0054] Furthermore, the coating material **68** may be selected based upon the desirability of a chemical bond between the internal frame **26** and the coating material **68**. Such a chemical bond may be desirable for durability of the resulting overmolded sensor **10**. For example, to prevent separation of the coating **68** from the internal frame **26**, the material used to form the coating **68** may be selected such

that the coating 68 bonds with some or all of the internal frame 26 during the overmolding process. In such embodiments, the coating 68 and the portions of the internal frame 26 to which the coating 68 is bonded are not separable, i.e., they form one continuous and generally inseparable structure.

[0055] Furthermore, in embodiments in which the coating 68 employed is liquid or fluid tight, such a sensor 10 may be easily maintained, cleaned, and/or disinfected by immersing the sensor into a disinfectant or cleaning solution or by rinsing the sensor 10 off, such as under running water. In particular, such an overmolded sensor assembly may be generally or substantially free of crevices, gaps, junctions or other surface irregularities typically associated with a multi-part construction which may normally allow the accumulation of biological detritus or residue. Such an absence of crevices and other irregularities may further facilitate the cleaning and care of the sensor 10.

[0056] Turning now to FIGS. 8 and 9, cross-sections of the coated sensor assembly 10 are depicted taken through transverse optical planes, represented by section line 8 and 9 of FIG. 6 respectively. FIGS. 8 and 9 depict, among other aspects of the sensor 10, the overmolding material 68 as well as underlying portions of the internal frame 26, such as the emitter housing 38 and detector housing 40, along with the respective emitter 22, detector 24, and signal transmission structures (such as wiring 83 or other structures for conducting electrical or optical signals). In the depicted embodiment, the emitter 22 and detector 24 are provided substantially flush with the patient facing surfaces of the sensor 10, as may be suitable for pulse oximetry applications. For other physiological monitoring applications, such as applications measuring tissue water fraction or other body fluid related metrics, other configurations may be desirable. For example, in such fluid measurement applications it may be desirable to provide one or both of the emitter 22 and detector 24 recessed relative to the patient facing surfaces of the sensor 10. Such modifications may be accomplished by proper configuration or design of a mold or die used in overmolding the internal frame 26 and/or by proper design of the emitter housing 38 or detector housing 40 of the internal frame 26.

[0057] In addition, as depicted in FIGS. 8 and 9, in certain embodiments portions 84 of the coating material 68 may be flexible, such as thin or membranous regions of coating material 68 disposed between structural supports 28 of a skeletal frame. Such flexible regions 84 allow a greater range of digit sizes to be accommodated for a given retention or clamping force of the sensor 10. For example, the flexible regions 84 may allow the emitter 22 and/or detector 24, to flex or expand apart from one another along the optical axis in embodiments in which the respective housings 38 and 40 are flexibly attached to the remainder of the frame 26. In this manner, the sensor 10 may accommodate differently sized digits. For instance, for a relatively small digit, the flexible region 84 may not be substantially deformed or vertically displaced, and therefore the emitter 22 and/or detector 24 are not substantially displaced either. For larger digits, however, the flexible regions 84 may be deformed or displaced to a greater extent to accommodate the digit, thereby displacing the emitter 22 and/or detector 24 as well. In addition, for medium to large digits, the flexible regions 84 may also increase retention of the sensor 10 on the digit by increasing the surface area to which the retaining force is applied.

[0058] Furthermore, as the flexible regions 84 deform, the force applied to the digit is spread out over a large area on the digit due to the deformation of the flexible region 84. In this way, a lower pressure on digits of all sizes may be provided for a given vertical force. Therefore, a suitable conforming fit may be obtained in which the emitter 22 and detector 24 are maintained in contact with the digit without the application of concentrated and/or undesirable amounts of force, thereby improving blood flow through the digit.

[0059] In the example depicted in FIGS. 6-9, flaps or side extensions 88 of the coating material 68 on the sides of the sensor 10 are depicted which facilitate the exclusion of environmental or ambient light from the interior of the sensor 10. Such extensions help prevent or reduce the detection of light from the outside environment, which may be inappropriately detected by the sensor 10 as correlating to the SaO_2 . Thus, a pulse oximetry sensor may detect differences in signal modulations unrelated to the underlying SaO_2 level. In turn, this may impact the detected red-to-infrared modulation ratio and, consequently, the measured blood oxygen saturation (SpO_2) value. The conformability of the fit of sensor 10 and the use of side extensions 88, therefore, may help prevent or reduce such errors.

[0060] While the exemplary medical sensors 10 discussed herein are some examples of overmolded or coated medical devices, other such devices are also contemplated and fall within the scope of the present disclosure. For example, other medical sensors and/or contacts applied externally to a patient may be advantageously applied using an overmolded sensor body as discussed herein. Examples of such sensors or contacts may include glucose monitors or other sensors or contacts that are generally held adjacent to the skin of a patient such that a conformable and comfortable fit is desired. Similarly, and as noted above, devices for measuring tissue water fraction or other body fluid related metrics may utilize a sensor as described herein. Likewise, other spectrophotometric applications where a probe is attached to a patient may utilize a sensor as described herein.

[0061] While the invention may be susceptible to various modifications and alternative forms, specific embodiments have been shown by way of example in the drawings and have been described in detail herein. However, it should be understood that the invention is not intended to be limited to the particular forms disclosed. Rather, the invention is to cover all modifications, equivalents, and alternatives falling within the spirit and scope of the invention as defined by the following appended claims. Indeed, the present techniques may not only be applied to transmission type sensors for use in pulse oximetry, but also to retroreflective and other sensor designs as well. Likewise, the present techniques are not limited to use on fingers and toes but may also be applied to placement on other body parts such as in embodiments configured for use on the ears or nose.

What is claimed is:

1. A sensor assembly, comprising:

a frame comprising two or more structural supports;

a coating provided over the frame, wherein the coating comprises at least one deformable region disposed between the two or more structural supports;

- at least one optical component disposed within the at least one deformable region, such that the at least one optical component can move relative to the two or more structural supports; and
- a biasing component attached to an end of the frame such that at least two different portions of the coated frame are biased closed in the absence of a sufficient opening force.
2. The sensor assembly of claim 1, wherein the at least one optical component comprises at least one of a light emitting diode or a photodetector.
 3. The sensor assembly of claim 1, wherein the coating comprises a first deformable region disposed between first and second structural supports and a second deformable region disposed between third and fourth structural supports.
 4. The sensor assembly of claim 3, wherein the at least one optical component comprises a light emitting diode disposed within the first deformable region and capable of moving relative to the first and second structural supports and a photodetector disposed within the second deformable region and capable of moving relative to the third and fourth structural supports.
 5. The sensor assembly of claim 1, comprising one or more signal transmission structures connected to the at least optical component.
 6. The sensor assembly of claim 1, wherein the sensor assembly comprises at least one of a pulse oximetry sensor, a sensor for measuring a water fraction, or a combination thereof.
 7. The sensor assembly of claim 1, wherein the frame comprises a single molded part.
 8. The sensor assembly of claim 1, wherein the frame comprises two or more parts joined to form the frame.
 9. The sensor assembly of claim 1, wherein the coating comprises a thermoplastic elastomer.
 10. The sensor assembly of claim 9, wherein the thermoplastic elastomer comprises at least one of a thermoplastic polyolefin, a thermoplastic vulcanizate alloy, thermoplastic polyurethane, silicone, or a combination thereof.
 11. The sensor assembly of claim 1, wherein the coating comprises a conformable material.
 12. The sensor assembly of claim 1, wherein no moving parts of the frame remain exposed from the coating.
 13. The sensor assembly of claim 1, wherein the sensor assembly is fluid tight.
 14. The sensor assembly of claim 1, wherein the coating is chemically bonded to the frame.
 15. The sensor assembly of claim 1, comprising a pulse oximeter monitor configured to receive data from the at least one optical component.
 16. The sensor assembly of claim 1, comprising a multi-parameter monitor configured to receive data from the at least one optical component.
 17. The sensor assembly of claim 1, comprising at least one integrated circuit device.
 18. The sensor assembly of claim 1, comprising a cable comprising one or more integrated circuits.
 19. The sensor assembly of claim 1, comprising an adapter cable connected to one or more signal transmission structures of the sensor assembly.
 20. The sensor assembly of claim 1, wherein the biasing component comprises at least one of a formed flat spring or a torsion spring.
 21. The sensor assembly of claim 1, wherein the biasing component comprises a metal alloy.
 22. The sensor assembly of claim 1, wherein the biasing component comprises a polymeric material.
 23. A skeletal frame of a sensor, comprising:
 - two or more structural support members having one or more spaces between the two or more structural support members, wherein the two or more structural support members are configured to provide support to an overlying coating when present.
 24. The skeletal frame of claim 23, wherein the two or more structural support members comprise at least one of an emitter housing or a detector housing.
 25. The skeletal frame of claim 23, wherein the two or more structural support members form a first portion and a second portion configured to move relative to one another.
 26. The skeletal frame of claim 23, wherein the two or more structural support members are formed as a single piece.
 27. The skeletal frame of claim 23, wherein the two or more structural support members are formed as separate pieces and joined to form the skeletal frame.
 28. The skeletal frame of claim 23, comprising a biasing component attached to the two or more structural support members.
 29. The skeletal frame of claim 23, wherein the two or more structural support members comprise a rigid material.
 30. The skeletal frame of claim 23, wherein the two or more structural support members comprise at least one of a metal, a metallic alloy, a thermoplastic material, or a composite material.
 31. A method for manufacturing a skeletal framework of a sensor, comprising:
 - forming two or more structural support members of a skeletal frame of a sensor having one or more spaces between the two or more structural support members, wherein the two or more structural support members are configured to provide support to an overlying coating when present.
 32. The method of claim 31, wherein forming the two or more structural support members comprises performing at least one of a molding operation, a diecasting operation, a sintering operation, a casting operation, or a stamping operation.
 33. The method of claim 31, wherein forming the two or more structural support members comprises forming the two or more structural support members as a single piece.
 34. The method of claim 31, wherein forming the two or more structural support members comprises forming the two or more structural support members as a plurality of pieces and joining the plurality of pieces to form the skeletal frame.
 35. The method of claim 34, wherein some or all of the plurality of pieces are formed from different materials.
 36. The method of claim 31, wherein the two or more structural support members comprises one or more of a thermoplastic material, a metal, a metallic alloy, or a composite material.

专利名称(译)	医疗传感器及其使用技术		
公开(公告)号	US20070032711A1	公开(公告)日	2007-02-08
申请号	US11/494838	申请日	2006-07-28
[标]申请(专利权)人(译)	COAKLEY JOSEPH MATLOCK GEORGE 大号 RARIDAN WILLIAM EGHBAL DARIUSD		
申请(专利权)人(译)	COAKLEY JOSEPH MATLOCK GEORGE 大号 RARIDAN WILLIAM EGHBAL DARIUSD		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	COAKLEY JOSEPH MATLOCK GEORGE L RARIDAN WILLIAM EGHBAL DARIUS D		
发明人	COAKLEY, JOSEPH MATLOCK, GEORGE L. RARIDAN, WILLIAM EGHBAL, DARIUS D.		
IPC分类号	A61B5/00		
CPC分类号	A61B5/02416 A61B5/14532 A61B5/14552 A61B2562/247 A61B5/6838 A61B2562/12 A61B5/6826		
其他公开文献	US7684843		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种传感器组件，其包括具有两个或更多个结构支撑件的框架。在框架上提供涂层。涂层具有至少一个可变形区域，该可变形区域设置在两个或更多个结构支撑件之间。至少一个光学部件设置在至少一个可变形区域内，使得至少一个光学部件可相对于两个或更多个结构支撑件移动。偏置部件附接到框架的端部，使得在没有足够的打开力的情况下，涂覆框架的至少两个不同部分被偏置闭合。传感器可以放置在患者的手指，脚趾，耳朵等上以获得脉搏血氧测量法或其他生理测量值。还提供了骨架和用于制造骨架的方法。

