



US006920345B2

(12) **United States Patent**
Al-Ali et al.

(10) **Patent No.:** **US 6,920,345 B2**
(45) **Date of Patent:** **Jul. 19, 2005**

(54) **OPTICAL SENSOR INCLUDING
DISPOSABLE AND REUSABLE ELEMENTS**

(75) Inventors: **Ammar Al-Ali**, Tustin, CA (US);
Yassir Abdul-Hafiz, Irvine, CA (US)

(73) Assignee: **Masimo Corporation**, Irvine, CA (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 225 days.

(21) Appl. No.: **10/351,645**

(22) Filed: **Jan. 24, 2003**

(65) **Prior Publication Data**

US 2004/0147822 A1 Jul. 29, 2004

5,490,505 A	2/1996	Diab et al.
5,494,043 A	2/1996	O'Sullivan et al.
5,507,286 A	4/1996	Solenberger
5,533,511 A	7/1996	Kaspari et al.
5,590,649 A	1/1997	Caro et al.
5,619,992 A	4/1997	Guthrie et al.
5,632,272 A	5/1997	Diab et al.
5,638,816 A	6/1997	Kiani-Azarbayjany et al.
5,638,818 A	6/1997	Diab et al.
5,645,440 A	7/1997	Tobler et al.
5,660,567 A	8/1997	Nierlich et al.
5,664,270 A	9/1997	Bell et al.
5,673,693 A	10/1997	Solenberger
5,678,544 A	10/1997	DeLonzor et al.
5,685,299 A	11/1997	Diab et al.
D393,830 S	4/1998	Tobler et al.
5,743,262 A	4/1998	Lepper, Jr. et al.

(Continued)

(51) **Int. Cl.⁷** **A61B 5/00**

(52) **U.S. Cl.** **600/344; 600/323**

(58) **Field of Search** 600/310, 322,
600/323, 340, 344

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,621,643 A	11/1986	New, Jr. et al.
4,685,464 A	8/1987	Goldberger et al.
4,700,708 A	10/1987	New, Jr. et al.
4,830,014 A	5/1989	Goodman et al.
4,865,038 A	9/1989	Rich et al.
4,960,128 A	10/1990	Gordon et al.
5,090,410 A	2/1992	Saper et al.
5,094,240 A	3/1992	Muz
5,158,323 A	10/1992	Yamamoto et al.
5,163,438 A	11/1992	Gordon et al.
5,170,786 A	12/1992	Thomas et al.
5,209,230 A	5/1993	Swedlow et al.
5,249,576 A	10/1993	Goldberger et al.
5,337,744 A	8/1994	Branigan
5,387,122 A	2/1995	Goldberger et al.
5,431,170 A	7/1995	Mathews
5,437,275 A *	8/1995	Amundsen et al. 600/323
5,452,717 A	9/1995	Branigan et al.
5,482,036 A	1/1996	Diab et al.

FOREIGN PATENT DOCUMENTS

AU	2000010929 B2	5/2000
CA	2 346 639	4/2000
CA	2 366 493 A1	11/2002
EP	1 222 894 A3	7/2002
EP	1 222 894 A2	7/2002
WO	WO 00/21433	4/2000
WO	WO 01/03574 A1	1/2001


Primary Examiner—Eric F. Winakur

(74) *Attorney, Agent, or Firm*—Knobbe, Martens, Olson &
Bear LLP

(57) **ABSTRACT**

A pulse oximetry sensor includes reusable and disposable elements. To assemble the sensor, the reusable element is snapped or slid within assembly mechanisms of the disposable element. In one embodiment, the reusable element includes protrusions while the disposable element includes tabs which receive the protrusions. In another embodiment, the reusable element includes neck portions and the disposable element includes straps which receive the neck portions. In any event, the assembly provides longitudinal movement between elements.

17 Claims, 10 Drawing Sheets

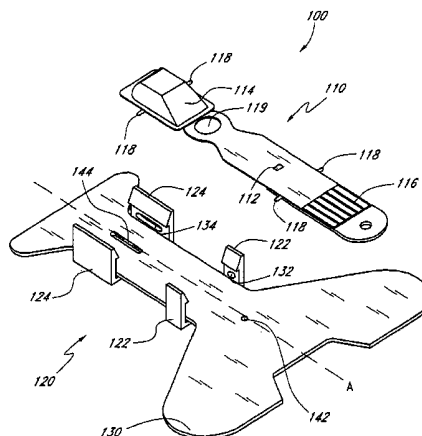

US 6,920,345 B2

Page 2

U.S. PATENT DOCUMENTS

5,758,644 A	6/1998	Diab et al.	6,343,224 B1	1/2002	Parker
5,760,910 A	6/1998	Lepper, Jr. et al.	6,349,228 B1	2/2002	Kiani et al.
5,769,785 A	6/1998	Diab et al.	6,360,114 B1	3/2002	Diab et al.
5,782,757 A	7/1998	Diab et al.	6,371,921 B1	4/2002	Caro et al.
5,785,659 A	7/1998	Caro et al.	6,377,829 B1	4/2002	Al-Ali
5,791,347 A	8/1998	Flaherty et al.	6,381,489 B1 *	4/2002	Ashibe 600/344
5,810,734 A	9/1998	Caro et al.	6,388,240 B2	5/2002	Schulz et al.
5,817,008 A	10/1998	Rafert et al.	6,397,091 B2	5/2002	Diab et al.
5,817,010 A	10/1998	Hibl	6,430,525 B1	8/2002	Weber et al.
5,823,950 A	10/1998	Diab et al.	6,463,311 B1	10/2002	Diab
5,830,131 A	11/1998	Caro et al.	6,470,199 B1	10/2002	Kopotic et al.
5,833,618 A	11/1998	Caro et al.	6,501,975 B2	12/2002	Diab et al.
RE36,000 E	12/1998	Swedlow et al.	6,515,273 B2	2/2003	Al-Ali
5,860,919 A	1/1999	Kiani-Azarbayjany et al.	6,519,487 B1 *	2/2003	Parker 600/344
5,879,373 A *	3/1999	Roper et al. 600/344	6,525,386 B1	2/2003	Mills et al.
5,890,929 A	4/1999	Mills et al.	6,526,300 B1	2/2003	Kiani et al.
5,904,654 A	5/1999	Wohlmann et al.	6,541,756 B2	4/2003	Schulz et al.
5,910,108 A	6/1999	Solenberger	6,542,764 B1	4/2003	Al-Ali et al.
5,919,133 A *	7/1999	Taylor et al. 600/344	6,580,086 B1	6/2003	Schulz et al.
5,919,134 A	7/1999	Diab	6,584,336 B1	6/2003	Ali et al.
5,934,925 A	8/1999	Tobler et al.	6,597,933 B2	7/2003	Kiani et al.
5,940,182 A	8/1999	Lepper, Jr. et al.	6,606,511 B1	8/2003	Ali et al.
5,991,648 A	11/1999	Levin	6,632,181 B2	10/2003	Flaherty et al.
5,995,855 A	11/1999	Kiani et al.	6,640,116 B2	10/2003	Diab
5,997,343 A	12/1999	Mills et al.	6,643,530 B2	11/2003	Diab et al.
5,999,834 A	12/1999	Wang et al.	6,650,917 B2	11/2003	Diab et al.
6,002,952 A	12/1999	Diab et al.	6,654,624 B2	11/2003	Diab et al.
6,011,986 A	1/2000	Diab et al.	6,658,276 B2	12/2003	Pishney et al.
6,014,576 A	1/2000	Raley	6,671,531 B2	12/2003	Al-Ali et al.
6,027,452 A	2/2000	Flaherty et al.	6,678,543 B2	1/2004	Diab et al.
6,036,642 A	3/2000	Diab et al.	6,684,090 B2	1/2004	Ali et al.
6,045,509 A	4/2000	Caro et al.	6,684,091 B2	1/2004	Parker
6,061,584 A *	5/2000	Lovejoy et al. 600/344	6,697,656 B1	2/2004	Al-Ali
6,067,462 A	5/2000	Diab et al.	6,697,658 B2	2/2004	Al-Ali
6,081,735 A	6/2000	Diab et al.	RE38,476 E	3/2004	Diab et al.
6,088,607 A	7/2000	Diab et al.	6,699,194 B1	3/2004	Diab et al.
6,110,522 A	8/2000	Lepper, Jr. et al.	6,714,804 B2	3/2004	Al-Ali et al.
6,144,868 A	11/2000	Parker	RE38,492 E	4/2004	Diab et al.
6,151,516 A	11/2000	Kiani-Azarbayjany et al.	6,721,585 B1 *	4/2004	Parker 600/344
6,152,754 A	11/2000	Gerhardt et al.	6,725,075 B2	4/2004	Al-Ali
6,157,850 A	12/2000	Diab et al.	6,735,459 B2	5/2004	Parker
6,165,005 A	12/2000	Mills et al.	6,745,060 B2	6/2004	Diab et al.
6,184,521 B1	2/2001	Coffin, IV et al.	6,760,607 B2	7/2004	Al-Ali
6,206,830 B1	3/2001	Diab et al.	6,770,028 B1	8/2004	Ali et al.
6,229,856 B1	5/2001	Diab et al.	6,771,994 B2	8/2004	Kiani et al.
6,236,872 B1	5/2001	Diab et al.	6,792,300 B1	9/2004	Diab et al.
6,256,523 B1	7/2001	Diab et al.	6,813,511 B2	11/2004	Diab et al.
6,263,222 B1	7/2001	Diab et al.	6,816,741 B2	11/2004	Diab
6,278,522 B1	8/2001	Lepper, Jr. et al.	6,822,564 B2	11/2004	Al-Ali
6,280,213 B1	8/2001	Tobler et al.	6,826,419 B2	11/2004	Diab et al.
6,285,896 B1	9/2001	Tobler et al.	6,830,711 B2	12/2004	Mills et al.
6,308,089 B1	10/2001	von der Ruhr et al.	6,850,787 B2	2/2005	Weber et al.
6,321,000 B1	11/2001	King	6,850,788 B2	2/2005	Al-Ali
6,321,100 B1	11/2001	Parker	2001/0029325 A1	10/2001	Parker
6,334,065 B1	12/2001	Al-Ali et al.	2003/0009092 A1	1/2003	Parker

* cited by examiner

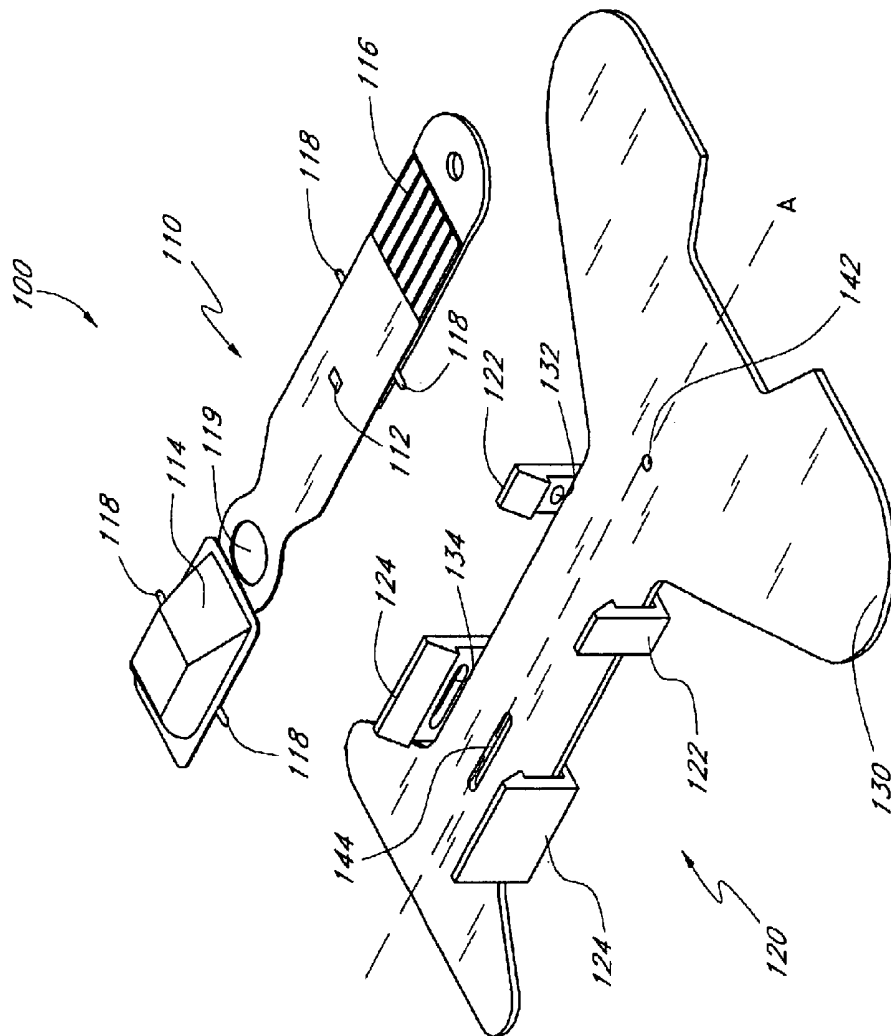
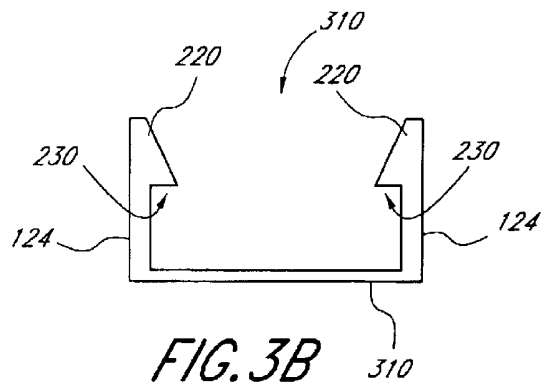
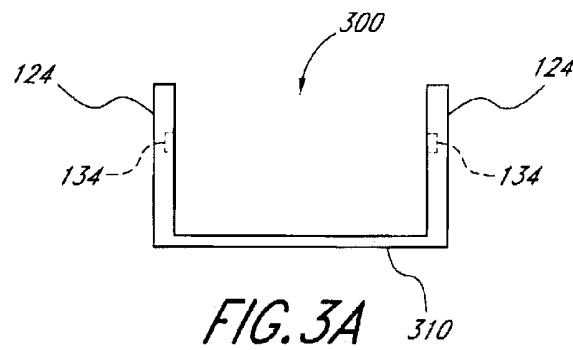
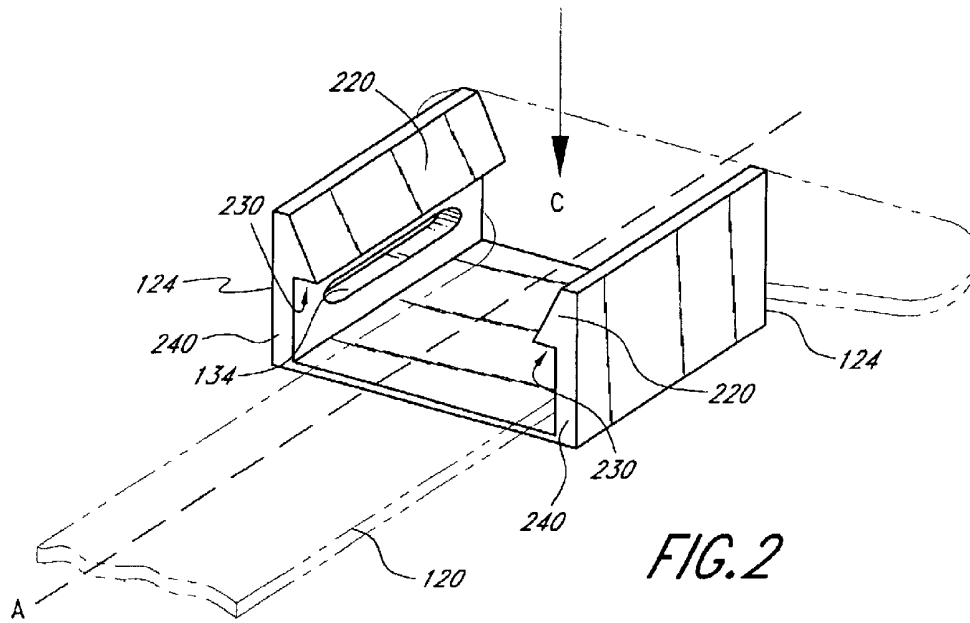
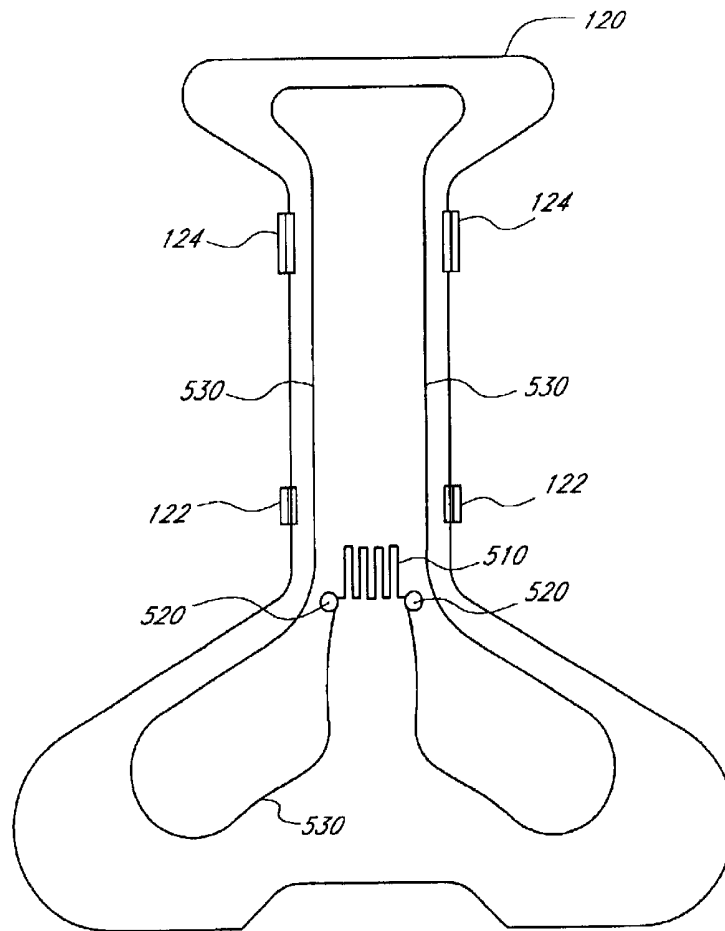
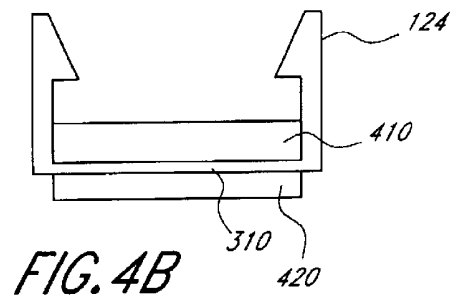
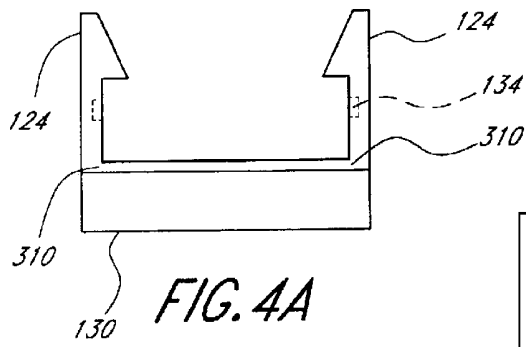
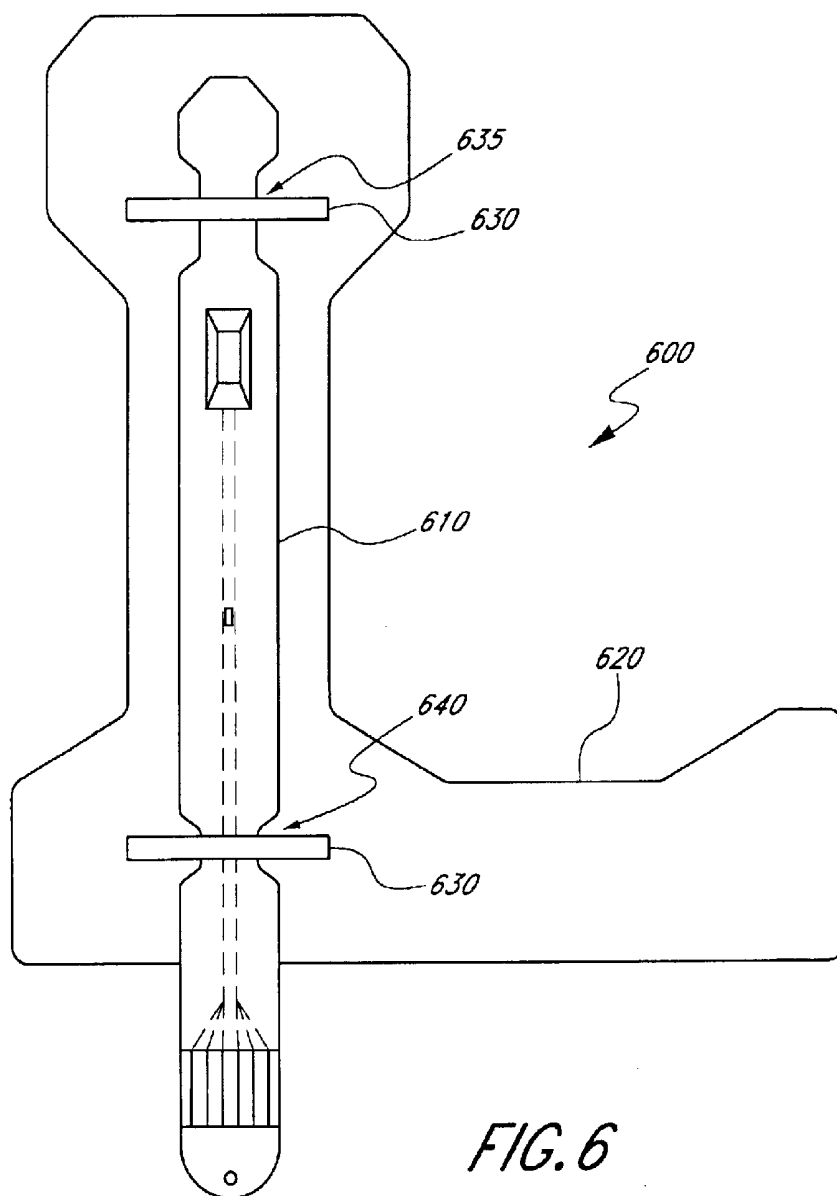


FIG. 1







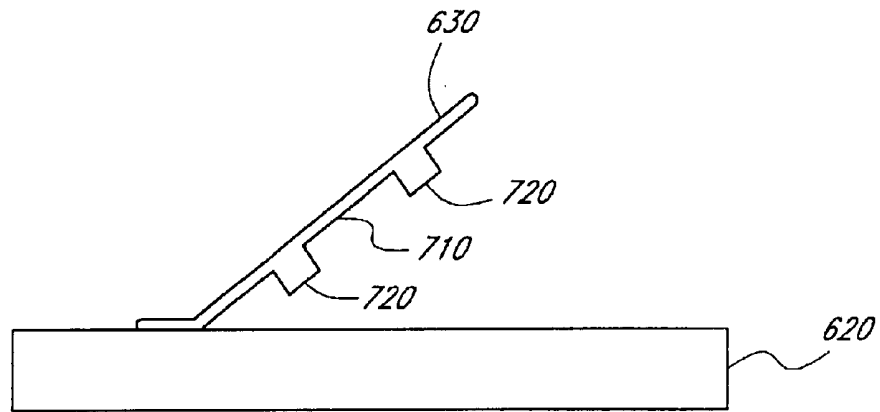


FIG. 7A





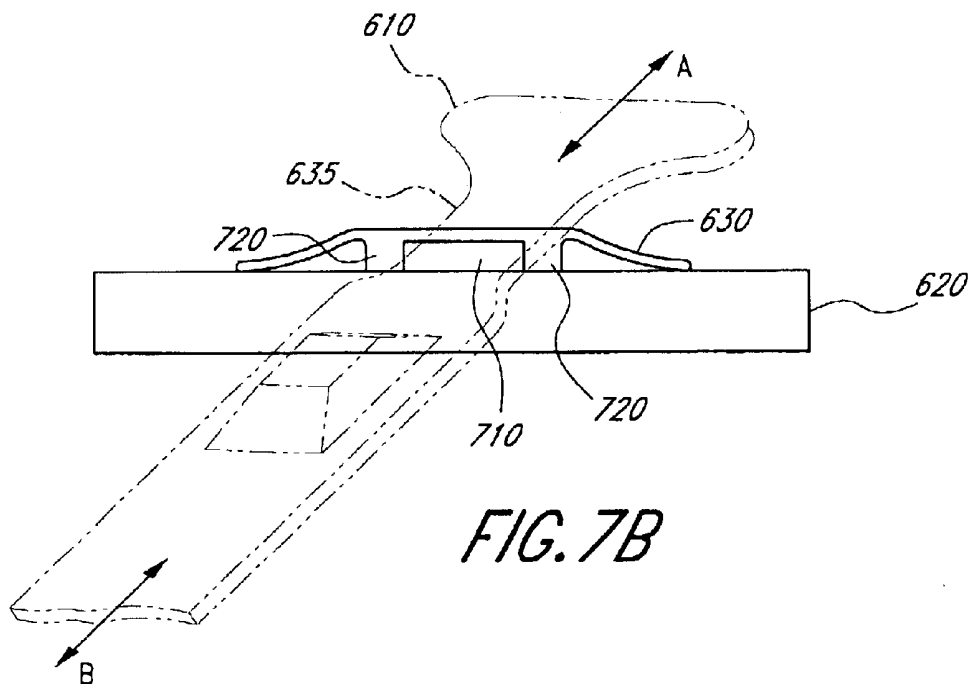



FIG. 7B

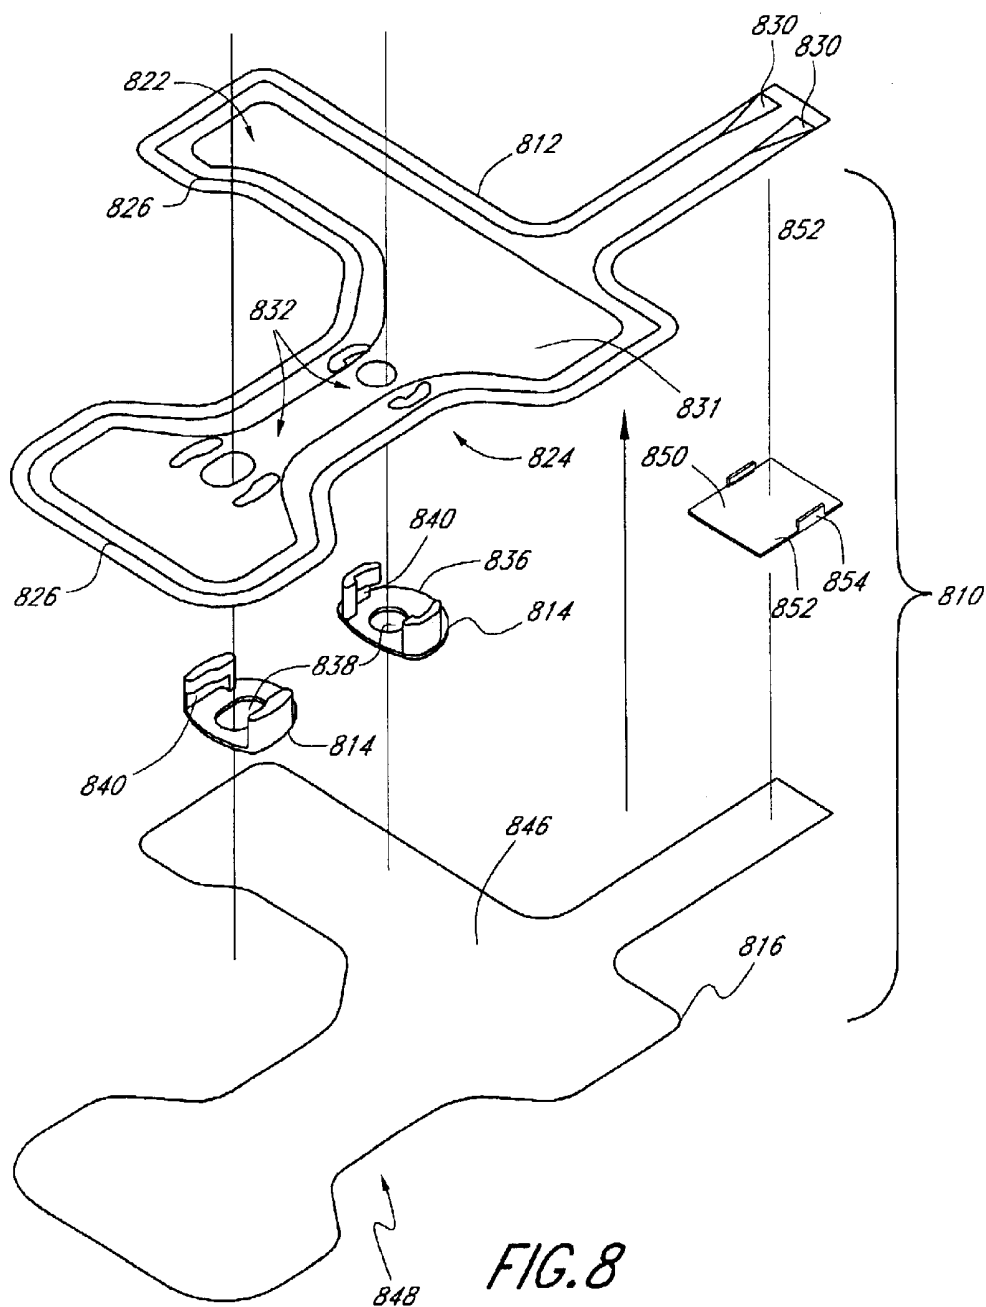

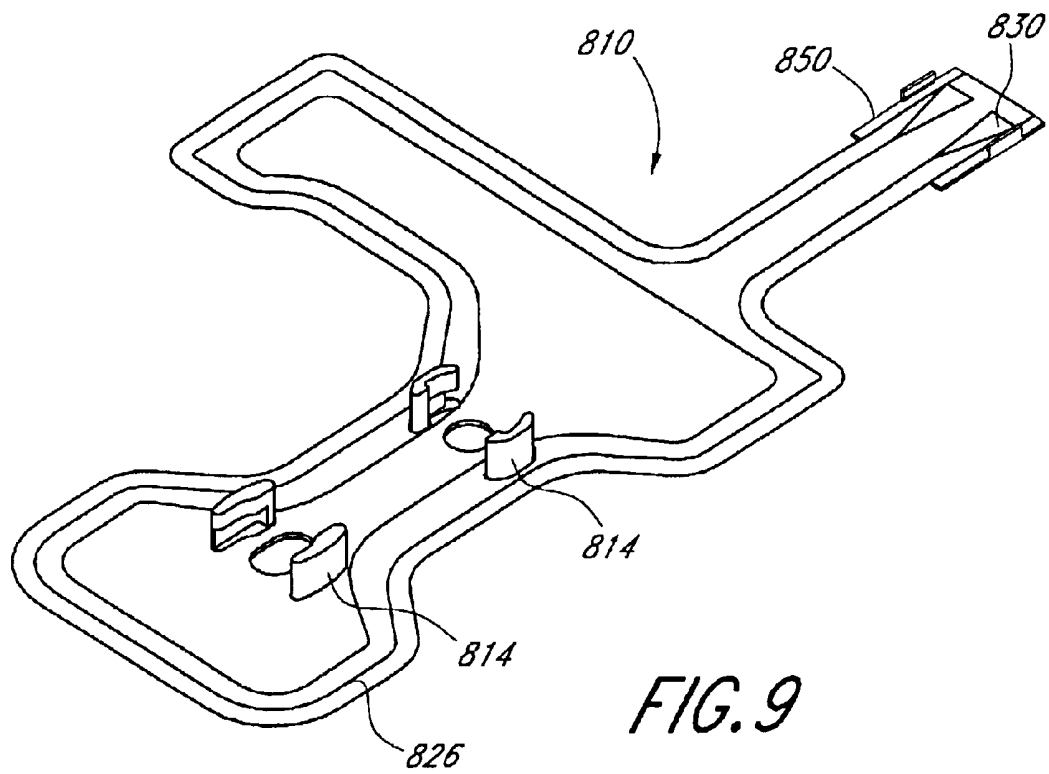

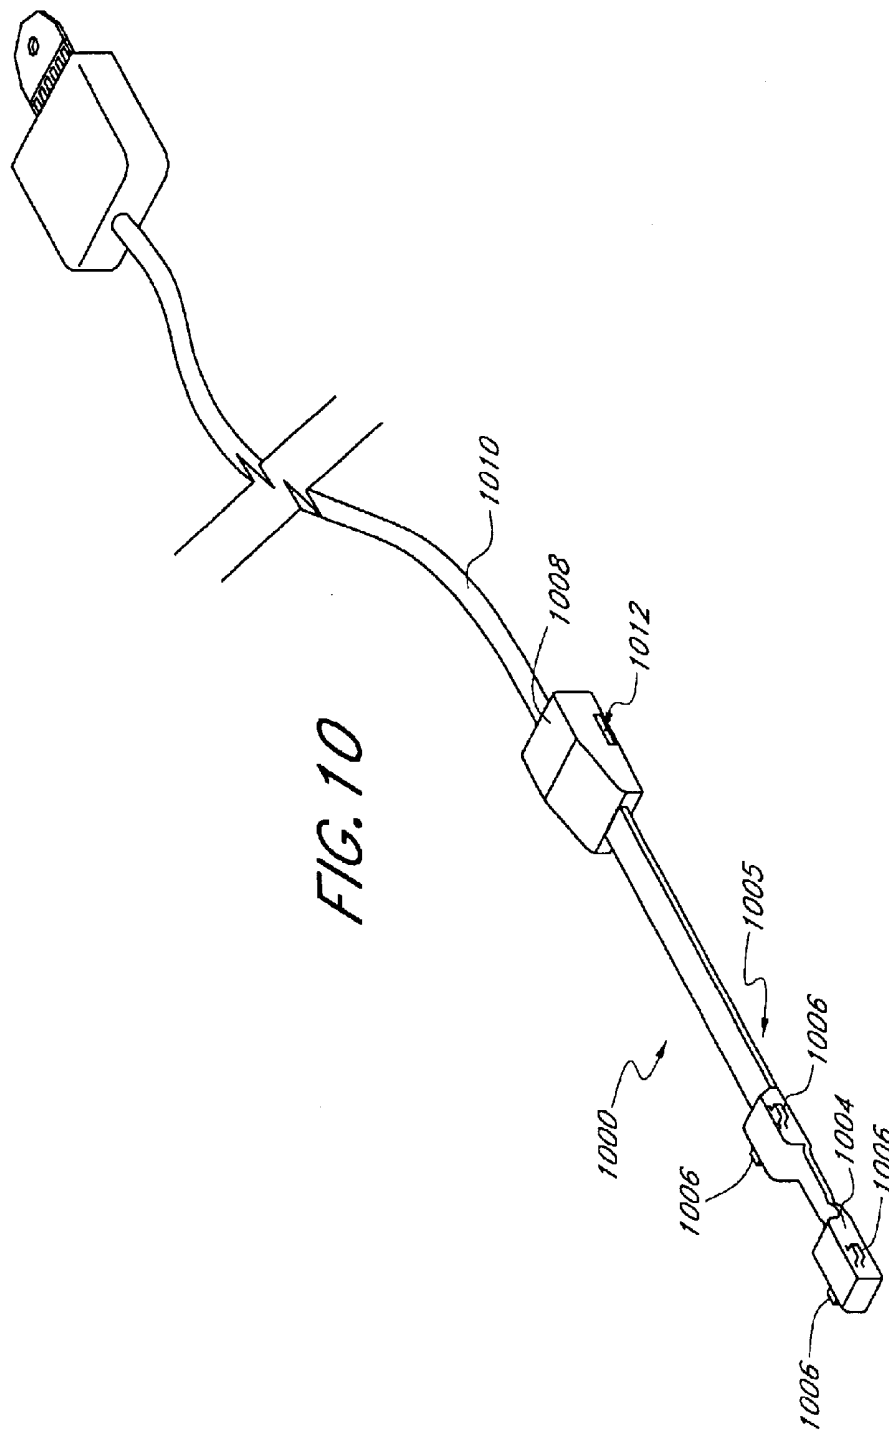

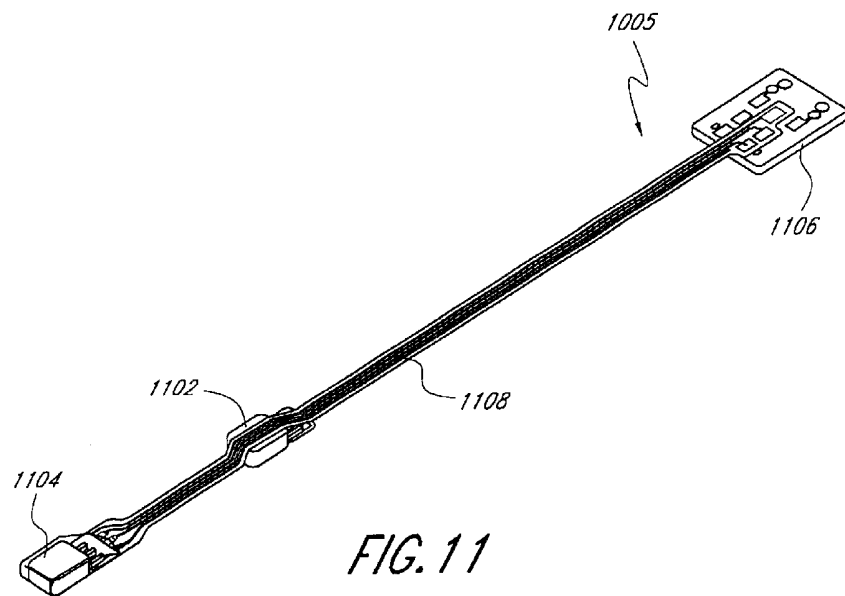

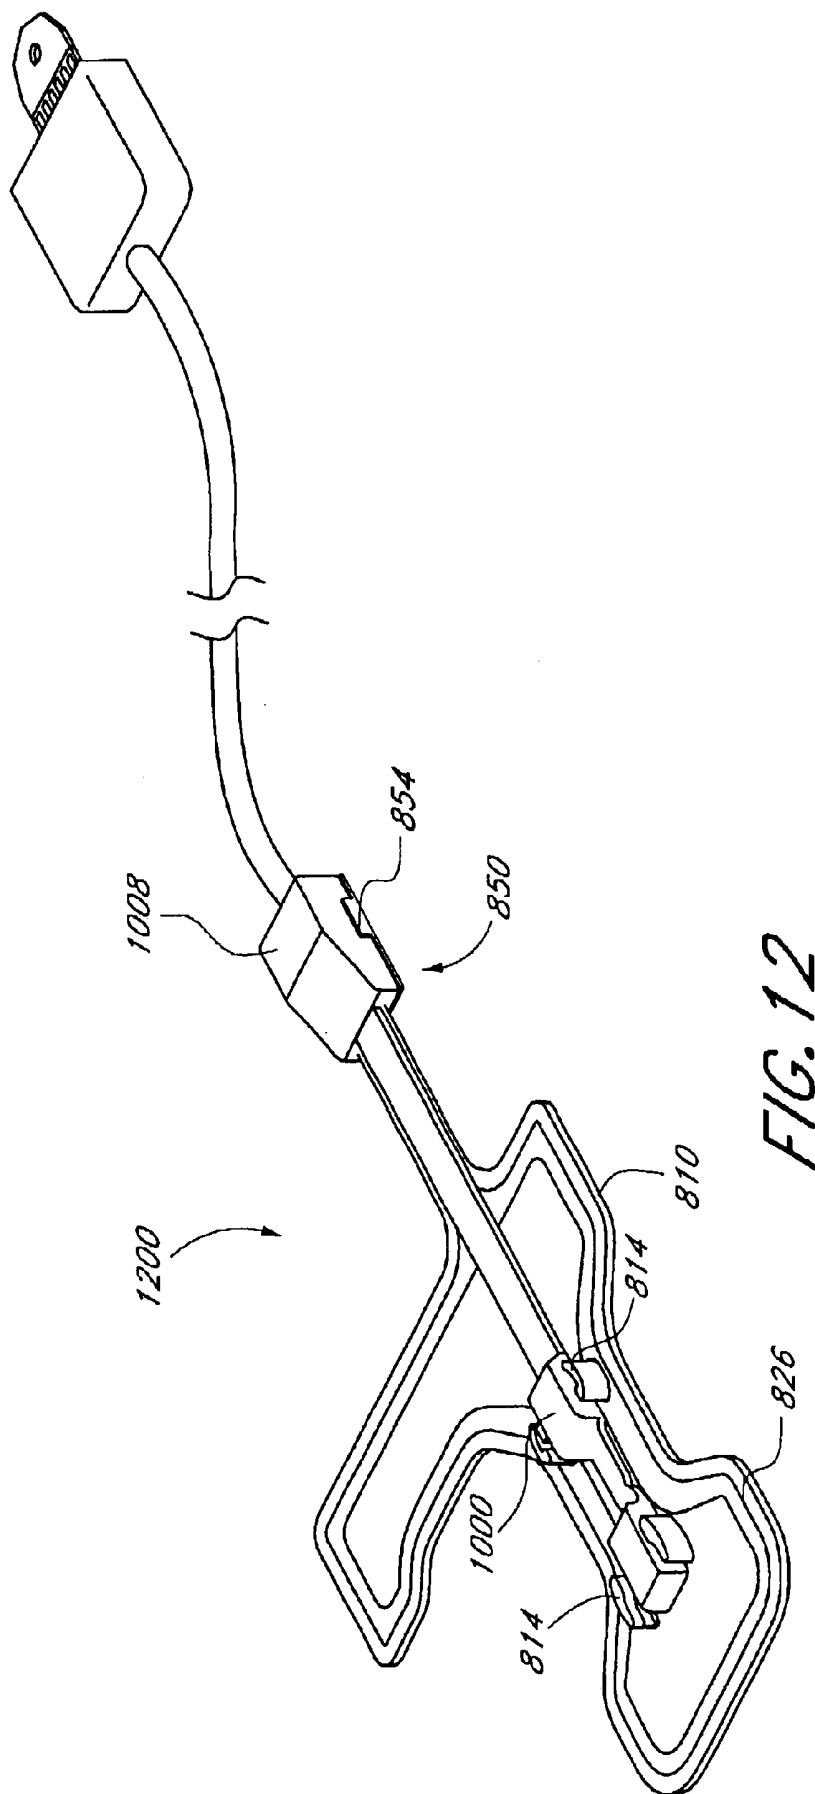

OPTICAL SENSOR INCLUDING DISPOSABLE AND REUSABLE ELEMENTS

FIELD OF THE INVENTION

The present invention relates to the field of sensors that measure oxygen content in a patient's blood. More specifically, the invention relates to a sensor that assembles reusable and disposable elements and/or allows longitudinal displacement between the reusable and disposable elements.

BACKGROUND OF THE INVENTION

Early detection of low blood oxygen is important in a wide variety of medical applications, and oximetry was developed to study and to measure, among other things, the oxygen status of blood. One type of oximetry, pulse oximetry, employs a sensor attached to a patient in order to output a signal indicative of a physiological parameter of the patient, such as, for example, the patient's blood oxygen saturation.

A pulse oximeter sensor generally uses a number of sensor components, such as one or more energy emission devices like red and infrared LED emitters, and an energy detection device like a photodiode detector. The sensor is generally attached to a measurement site such as a patient's finger, toe, ear, forehead, foot, hand, heel or the like, using an attachment mechanism such as a disposable tape, reusable housing, Velcro strap, or the like. The attachment mechanism positions the emitter and detector in proximity to the measurement site, such that the emitter projects energy into the blood vessels and capillaries of the measurement site, and the photodiode detector then detects the attenuated energy. The emitted energy can be light or other forms of energy. The detector communicates a signal indicative of the detected attenuated energy to a signal processing device such as an oximeter. The oximeter generally calculates, among other things, one or more physiological parameters of the measurement site.

In sensors where the detector detects emissions through the measurement site, it is generally desirable to position the detector opposite the emitter around the measurement site, such as, for example, above and below a finger. However, sensors are produced in a limited number of sizes and shape configurations, while patients have, for example, fingers and toes of many different sizes and shapes.

In addition, the attachment mechanism and the electronic components of a sensor are generally curved around a measurement site in a manner detrimental to one or more elements of the sensor. For example, the attachment mechanism generally wraps around the measurement site at an approximate "inner circle" having a first radius, while the electronic components such as the flexible circuits are generally fixedly attached to the attachment mechanism. Accordingly, the electronic components can form an approximate "outer circle" having a second radius unequal to the first radius. However, because the attachment mechanism generally does not move independently with respect to the electrical components, attachment of the sensor to the measurement site can exert forces on the electrical components, such as, for example, exerting forces which try to lengthen, or longitudinally stretch the electrical components to account for an increased radius thereof. The forced stretching can damage the electrical components of a flexible circuit, such as the conductive traces.

SUMMARY OF THE INVENTION

Based on the foregoing, embodiments of the present invention include a sensor comprising reusable and dispos-

able sensor elements that permit longitudinal displacement with respect to one another when the sensor is attached to a measurement site. For example, in one embodiment the sensor includes a reusable element and a disposable element configured to receive the reusable element in a releasable attachment assembly providing longitudinal displacement between the disposable and reusable elements. The longitudinal displacement advantageously allows the sensor elements to self-adjust with respect to one another during attachment to the measurement site. The self-adjustment or independent movement advantageously reduces the forces caused by longitudinal stretching, thereby reducing damage to the reusable element.

One aspect of the invention relates to an optical probe including a reusable element and a disposable element that can be attached together by placing or snapping protrusions on one element into apertures and receiving slots on the other element. For example, the reusable element can be fitted with protrusions made of plastic, and the disposable element can be fitted with detents or tabs, which include apertures or receiving slots. The reusable element attaches to the disposable element by inserting, or snapping, the protrusions into the apertures and the receiving slots of the tabs. When assembled, at least some of the protrusions are slidable within the receiving slots to independently move along a longitudinal axis of the sensor, thereby providing some longitudinal decoupling between the reusable element and the disposable element.

Another aspect of the invention relates to a sensor with a reusable element and a disposable element where the reusable element is made of a flexible or pliable material and includes one or more neck sections. The disposable element includes two straps, each of which is configured to receive a neck section. The reusable element and the disposable element are attached together by placing the neck sections within the straps. In one embodiment, the neck sections include a long neck section and a short neck section. The long neck section has a sufficient length to allow longitudinal movement of the reusable element within the strap, thus permitting movement of the reusable element with respect to the disposable element.

Another aspect of the invention relates to a sensor with a reusable element and a disposable element where the reusable element is secured by guides or tabs affixed to the disposable element. The guides allow limited longitudinal motion of the reusable element and thereby allow the reusable element to flex independently of the disposable element as the device is positioned on a patient.

Another aspect of the invention relates to a sensor with a reusable element and a disposable element where the reusable element is encased in a protective cover. In one embodiment, the protective cover is made of a pliable material and prevents any sharp edges from scratching or poking a patient or caregiver. The protective cover also advantageously prevents damage to the reusable element that could occur from dirt, dust, liquids, or other elements of the environment.

Yet another aspect of the invention relates to a sensor with a reusable element and a disposable element where the disposable element includes a breakable element. After an approximate predetermined number of safe uses, the breakable element breaks and the disposable element is rendered inoperable or otherwise indicates its over use.

For purposes of summarizing the invention, certain aspects, advantages and novel features of the invention have been described herein. Of course, it is to be understood that

not necessarily all such aspects, advantages or features will be embodied in any particular embodiment of the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

A general architecture that implements the various features of the invention will now be described with reference to the drawings. The drawings and the associated descriptions are provided to illustrate embodiments of the invention and not to limit the scope of the invention. The drawings are not necessarily drawn to scale. Throughout the drawings, reference numbers are re-used to indicate correspondence between referenced elements. In addition, the first digit of each reference number indicates the figure in which the element first appears.

FIG. 1 illustrates a perspective view of an embodiment of an unassembled sensor that includes reusable and disposable elements.

FIG. 2 illustrates a perspective view of tabs of the disposable element of FIG. 1.

FIG. 3A illustrates a cross-sectional view of another embodiment of tabs of a disposable element.

FIG. 3B illustrates a cross-sectional view of yet another embodiment of tabs of a disposable element.

FIG. 4A illustrates a cross-sectional view of the two tabs of FIG. 2, adhesively attached to the disposable element.

FIG. 4B illustrates a cross-sectional view of the two tabs of FIG. 2, attached between layers of the disposable element.

FIG. 5 illustrates a top view of the disposable element of FIG. 1, including an information element and breakable conductor.

FIG. 6 illustrates a top view of another embodiment of an assembled sensor that includes reusable and disposable elements.

FIGS. 7A and 7B illustrate simplified cross-sectional views of an embodiment of a strap of the disposable element of FIG. 6.

FIG. 8 illustrates an exploded view of a disposable element according to another embodiment of an optical sensor.

FIG. 9 illustrates a perspective view of the disposable element of FIG. 8.

FIG. 10 illustrates a perspective view of an embodiment of a reusable element according to an embodiment of the optical sensor of FIG. 8.

FIG. 11 illustrates a perspective view of a flex circuit of the reusable element of FIG. 10.

FIG. 12 illustrates a perspective view of the assembled optical sensor including the disposable element of FIG. 8 and the reusable element of FIG. 10.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

FIG. 1 illustrates an embodiment of a sensor 100. The sensor 100 includes a reusable element 110 and a disposable element 120. According to one embodiment, the reusable element 110 generally includes those components of the sensor 100 that are more expensive, such as, for example, one or more energy emitters, one or more energy detectors, one or more breakable conductors, one or more information elements, some or all of the same, or the like. In addition, the reusable element 110 includes an assembly mechanism generally shaped to mate with a corresponding component of the disposable element 120, as will be disclosed in greater detail below.

The disposable element 120 generally includes those components of the sensor 100 that are less expensive, such as, for example, face tape, bandages, or other mechanisms for removably attaching the reusable element 110 to a measurement site. Moreover, the disposable element 120 includes a mating assembly mechanism generally shaped to mate with assembly mechanism of the reusable element 110, thereby attaching the reusable element 110 to the disposable element 120 in a manner that provides for at least some self adjustment or displacement between the elements.

When the disposable element 120 attaches the reusable element 110 to tissue of a measurement site, a signal processing device, such as an oximeter, activates the energy emitters to transmit light energy into the tissue. The tissue attenuates the light energy, which is then detected by the detector. A signal indicative of the detected light energy is then generally forwarded back to the signal processing device for determination of one or more physiological parameters of the tissue, such as, for example, oxygen saturation, pulse rate, or the like.

A skilled artisan will recognize from the disclosure herein that there are many combinations of differing shapes and circuit configurations for the reusable and disposable elements, 110 and 120, respectively, such as, for example, those disclosed in U.S. Pat. No. 6,377,829, and U.S. patent application Ser. No. 10/020,664, filed on Dec. 11, 2001, both of which are hereby incorporated by reference.

As shown in the exemplary embodiment of FIG. 1, the reusable element 110 can include one or more energy emitters 112, an energy detector 114, and an electrical connector 116 electrically communicating with the emitters 112 and the detector 114 through a flexible circuit. According to one embodiment, the flexible circuit comprises material of a generally flexible or pliable construction.

The reusable element 110 also includes the foregoing assembly mechanism, such as, for example, the one or more protrusions 118. According to one embodiment, the protrusions 118 comprise approximately cylindrical-shaped or tab-shaped extensions made of plastic or other durable materials. FIG. 1, shows the reusable element 110 including four protrusions 118, two opposing protrusions proximate a front portion and extending in opposite generally horizontal directions, and two opposing protrusions proximate a back portion and extending in opposite generally horizontal directions. According to one embodiment, the protrusions 118 roughly align with one or more of the electronic components of the sensor 100. As described below, the protrusions 118 each advantageously mate with the mating assembly mechanism of the disposable element 120 in a manner providing for at least some displacement of the reusable element 110 with respect to the disposable element 120, thereby avoiding damage or harmful wear of the reusable element 110.

FIG. 1 also shows the flexible circuit including an optical barrier, such as, for example, an aperture or gap 119 to reduce light energy from travelling from the emitter 112 to the detector 114 without first passing through tissue at the measurement site (i.e., light piping). A skilled artisan will recognize from the disclosure herein that the gap 119 could be replaced with opaque materials, protrusions, pads, tabs, or other light blocking mechanisms.

Although disclosed with reference to preferred embodiments, a skilled artisan will recognize from the disclosure herein, a number of other embodiments of the reusable element 110. For example, one or more of the emitters 112 or the detector 114 can be located on the disposable element 120. Moreover, the flexible circuit may comprise plastic, electric wires, polyester substrates, or the like.

FIG. 1 also shows the disposable element **120**. According to an embodiment, the disposable element **120** generally comprises a base **130** comprising a face tapestock material similar to that of an adhesive bandage shaped to position the reusable element proximate the measurement site. The face tape can include an adhesive covered base protected by one or more conveniently shaped release liners or layers. Although illustrated in a conventional elongated surface with opposing wings style shape, an artisan will recognize from the disclosure herein that the tape may comprise virtually any shape, including those disclosed in U.S. patent application Ser. No. 10/020,664, referenced above. Moreover, the disposable element **120** may comprise a Velcro strap, a foam wrap, a reusable plastic housing or the like.

The disposable element **120** also includes the assembly mechanism, illustrated as tabs **122** and **124**. Each of the tabs **122** include an aperture **132**, while each of the tabs **124** include a receiving slot **134**. In one embodiment, the apertures **132** and the receiving slots **134** have sufficient depth to receive the protrusions **118**. In other embodiments, the apertures **132** and receiving slots **134** extend through the tabs **122** and **124**. As shown in FIG. 1, the tabs **122** and **124** are shaped to removably receive the reusable element **110**. For example, the tabs **122** and **124** can include sloped surfaces that cause the tabs **122** and **124** to displace outwardly during assembly of the sensor **100**. For example, when the reusable element **110** is properly positioned within the tabs **122** and **124**, the tabs **122** and **124** snap inwardly over the reusable element **110** such that the protrusions **118** are within the apertures **132** and the receiving slots **134**. When assembled, vertical and horizontal movement between the reusable and disposable elements, **110** and **120** respectively, is substantially prevented by the relationship between the tabs **122** and **124**, the apertures **132**, the slots **134** and the protrusions **118**. However, the slots **134** provide for displacement between elements along longitudinal axis A when the disposable portion **120** is wrapped around a measurement site by allowing the protrusions **118** to slide back and forth within the slots **134**. Thus, the assembly mechanisms of the reusable and disposable elements, **110** and **120**, provide independent movement between the elements, thereby allowing self-adjustment of the sensor **100** to the differing radiuses of each element. Such construction advantageously reduces the harmful stressing effects applied to components of the reusable element **110**.

FIG. 1 also shows that a gap **142**, slot or aperture, or otherwise transparent area can be included on the disposable element **120** to permit light from the emitter **112** to travel through the disposable element **120** to the tissue of the measurement site. Moreover, another gap **144** can be included on the disposable element **120** to permit attenuated light from the measurement site tissue to travel through the disposable element **120** to the detector **114**. In another embodiment, some or all of the base **130** of the disposable element **120** is made of a transparent material, and the gaps **142** and **144** can be omitted.

A skilled artisan will recognize from the disclosure herein that the tabs **122** and **124** of the disposable element **120** can be implemented in a wide variety of embodiments. For example, an embodiment can include each of the tabs **122** and **124** having a receiving slot **134** while another embodiment can include each of the tabs **122** and **124** having an aperture **132**.

FIG. 2 illustrates a perspective view of the tabs **124** including the receiving slots **134**. As disclosed, the tabs **124** can be shaped to include a sloped surface **220** configured to

displace a ledge or catch **230** during sensor assembly. For example, the sloped surface **220** displaces outwardly when protrusions **118** are pressed in the direction of the arrow C. Then when the reusable element **110** is properly positioned, the protrusions **118** snap into the receiving slots **134** and the catch **230** snaps over a top surface of the reusable element **110**.

The receiving slots **134** are longer than the cross sectional width of the protrusions **118** so that the protrusions **118** can move within the receiving slots **134** to different positions along the longitudinal axis A of the disposable element **120**. The apertures **132**, on the other hand, are sized to allow protrusions **118** to be located within the apertures **132** but to prevent substantial movement along the longitudinal axis A of the disposable element **120**, thus ensuring proper positioning of the sensor elements, with respect to the tissue and one another.

In an embodiment, the reusable element **110** and the disposable element **120** are assembled into the sensor **100** when the protrusions **118** are snapped into the apertures **132** and the receiving slots **134** of the tabs **122** and **124**. The assembled sensor **100** is then attached to a measurement site, through, for example, application of the adhesive covered side of the face tape to tissue at the measurement site. During application, the protrusions **118** within the receiving slots **134** move along the receiving slot **134**, while the protrusions **118** remain positioned within the aperture **132**. This type of flexibility advantageously reduces the stretching force placed on conventional reusable elements.

FIG. 2 also shows receiving slots **134** as grooves in the walls **240** of the tabs **124**, where the grooves do not extend all the way through the walls **240**. In other embodiments, the receiving slots **134** can be open slots that extend through the walls **240**. Likewise, the aperture **132** can be straightforward depressions, or punch through holes.

FIG. 3A illustrates a cross-sectional view of tabs **300** of another embodiment of a disposable element, such as disposable element **120** of FIG. 1. The tabs **300** include the receiving slot **134** for receiving the protrusions **118**, but does not include the sloped surface **220** or the catch **230** of FIG. 2. Thus, the reusable element **110** is assembled relying on the interaction described in the foregoing between the protrusions **118** and the apertures **132** and the slots **134**.

FIG. 3B illustrates a cross-sectional view of tabs **310** of another embodiment of a disposable element, such as the disposable element of FIG. 1. The tabs **310** include the sloped surface **220** and the catch **230**, but do not include the receiving slot **134** or aperture **132**. Thus, the sensor **100** is assembled relying on the interaction between the catch **230** and the surface of the reusable element **110**.

FIG. 4A illustrates a cross-sectional view of the tabs **124** of FIG. 1 adhesively attached to the disposable element **120**, according to an embodiment. In FIG. 4A, the tabs **124** are attached to the base **130** by adhesive. In a preferred arrangement, the tabs **124** share a common substrate **310**, and an adhesive is applied between the substrate **310** and the base **130** to attach the tabs **124** to the disposable element **120**.

FIG. 4B illustrates a cross-sectional view of the tabs **124** of FIG. 1 attached between layers of the disposable element **120** of FIG. 1, according to another embodiment. In FIG. 4B, the tabs **124** are attached between two layers **410** and **420** of the base **130**. In a preferred arrangement, the two tabs **124** share a common substrate **310**, and the substrate **310** is sandwiched between the layers **410** and **420**.

A skilled artisan will recognize from the disclosure herein that the embodiments disclosed with reference to FIGS. 3

and 4 can be applied to one or both sets of the tabs 122 and 124. Moreover, a skilled artisan will recognize from the disclosure herein that the protrusions 118 can be attached to the reusable element 110 in a number of ways, such as, for example, attached by adhesive to the reusable element 110, manufactured as integral parts of the reusable element 110, sandwiched between a top layer and a bottom layer of the reusable element 110, or the like.

FIG. 5 illustrates a top view of the disposable element of FIG. 1, including an information element 510, contacts 520, and a breakable conductor 530, according to yet another embodiment. The contacts 520 can electrically connect with contacts on the flexible circuit of the reusable element 120, thereby adding the information element 510 and/or the breakable conductor 530 into the electric circuit of the sensor 100. As is understood in the art, the information element 510 can provide an indication of the sensor or patient type, operating characteristics or the like, or that the sensor 100 is from an authorized supplier. In an embodiment, the information element 510 is a resistive element made by depositing a conductive ink trace having a predetermined length and width. The information element 510 is disposed between contacts 520, which can also be implemented with conductive ink. As an artisan will recognize from the disclosure herein, many type of information elements can be included, such as, for example, passive or active elements, accessible memory elements, or the like.

The breakable conductor 530 is configured to break after a predetermined number of safe uses, thus providing quality control to ensure that the disposable element 120 is not over used. Various embodiments of information element 510, contacts 520, and breakable conductor 530 can be found in U.S. Pat. No. 6,377,829.

FIG. 6 illustrates a top view of an assembled sensor 600 that includes reusable and disposable elements, according to another embodiment. As shown in FIG. 6, the sensor 600 includes a reusable element 610 and a disposable element 620. The disposable element 620 includes straps 630 which position the reusable element 610 as described below. As shown in FIG. 6, the reusable element 610 can be similar to the reusable element 110 of the foregoing embodiments, generally including, for example, the more expensive components of the sensor 600. Moreover, disposable element 620 can be similar to the disposable element 120 of the foregoing embodiments, generally including for example, a disposable tape. The disposable tape can be virtually any suitable shape, and is shown in FIG. 6 in a generally "L" shaped configuration.

FIG. 6 also shows the reusable portion 610 including an extended narrow neck or notch 635 and a neck or notch 640, each narrower in width than the general width of the reusable element 610. The straps 630 attached to the disposable element 620 extend over the necks 635 and 640 to position the reusable element 610 with respect to and proximate the disposable element 620. The straps 630 provide for longitudinal movement between the elements of the sensor 600 similar to that disclosed in the foregoing.

FIG. 7A illustrates a simplified cross-sectional view of one of the straps 630 of the disposable element 620 of FIG. 6, according to an embodiment. The strap 630 may comprise a hook-and-loop device such as Velcro. The strap 630 may alternatively be an integral part of the structure of the disposable element 620. According to an embodiment, the strap 630 includes blocks 720 forming a gap 710 therebetween. As shown in FIG. 7A, an embodiment of the strap 620 can be removed from the disposable element 620 to

permit the neck 630 of the reusable element 610 to be placed within the gap 710, as show in FIG. 7B an artisan will also recognize from the disclosure herein that the pliable material of the reusable portion 610 can alternatively or concurrently be compressed together and guided through attached straps 630.

According to one embodiment, the gap 710 is as wide or slightly wider than the necks 635 and 640, but narrower than other adjacent portions of the reusable element 610. Therefore, once placed in the gaps 710 and attached to the disposable element 620, the reusable element 610 can be moved along its longitudinal axis along the arrows A and B (FIG. 7B), but only to the extent that the necks 635 and 640 remain in the gaps 710.

In one embodiment shown in FIG. 6, the reusable element 610 includes the relatively "long" neck 635 shown near the top of the figure and a relatively "short" neck 640 shown near the bottom of the figure. Once the two necks 635 and 640 are placed within the straps 650, the long neck 635 allows the reusable element 610 to be moved along a longitudinal axis of the disposable element 120. In contrast, the short neck 640 prevents substantial movement along the longitudinal axis. Thus, similar to embodiments disclosed in the foregoing, the sensor 600 allows the neck 630 to self adjust during application to a measurement site, thereby avoiding damaging the reusable element 610.

FIG. 8 illustrates an exploded view of a disposable element 810 according to another embodiment of an optical sensor. The disposable element 810 includes a top layer 812, at least one attachment mechanism, tab, or positioning guide 814, and an adhesive, preferably transparent, tape layer 816. FIG. 8 shows tabs 814 positioned in a back-to-back or opposing manner, as will be described in greater detail below.

FIG. 8 shows the top layer 812 as a generally L shaped tape or other pliable substrate including a first side 822 and a second side 824, although an artisan will recognize from the disclosure herein that the virtually any shape can be used which provides attachment to tissue of a patient. According to an embodiment, the first side 822 includes a breakable element 826, such as the conductive trace disclosed in U.S. Pat. No. 6,377,829, discussed in the foregoing. The breakable element 826 is included into the electrical circuit of the optical sensor through electrical leads or contacts 830 configured to electrically communicate with contacts of a reusable element of the optical sensor. Moreover, the first side 822 of the top layer 812 can optionally include an optical barrier layer 831, such as a layer of material opaque or substantially opaque to light. The optical barrier layer 831 is generally designed to help prevent ambient light or light piping from interfering with the optical signals before or after they are passed through the tissue of the patient. In one embodiment, the barrier layer 831 comprises conductive trace material similar to that of the breakable element 826.

According to an embodiment, the top layer 812 also includes a plurality of apertures 832, which when the optical sensor is assembled, accept portions of the tabs 814 in a manner designed to provide proper placement, positioning, and support of the tabs 814. However, a artisan will recognize from the disclosure herein that top layer 812 may use ink outlines combined with adhesive, or the like to help an assembler properly place and support the tabs 814 on the first side 822 of the top layer 812.

Each tab 814 includes a base 836, a signal aperture 838, and grooves or slots 840. The base 836 connects and supports each of two raised side members forming a gen-

erally U shaped structure. The signal apertures **838** comprise holes through which a properly positioned sensor element can emit or detect optical signals, and the raised side members each include the slot **840**, similar to the grooves **134** of the tabs **124** of FIG. 1. However, unlike FIG. 1, an embodiment of each of the slots **840** opens from one side of the raised side member, extends along the side member, and ends before the other side of the raised side member. Thus, the slot **840** accepts a protrusion or the like from an insertion side, and allows the protrusion to slide within the slot **840** to the end thereof, proximate a blocked side. Moreover, according to one embodiment, the blocked sides of the tabs **814** approximately adjacently oppose one another, such that protrusions inserted into the insertion sides, are at one point blocked from sliding closer than a predetermined distance from one another by the blocked sides.

According to one embodiment, the tape layer **816** comprises a transparent tape or other substrate layer. The tape layer **816** has a first side **846** and a second side **848**. When assembled, the first side **846** adheres to the top layer **812** and sandwiches the tabs **814** therebetween. The second side **848** includes an adhesive, hook-and-loop, similar or combination structure configured to secure the disposable element **810** to tissue of a patient.

FIG. 8 also shows the disposable element **810** including a cable connector **850**. The cable connector **850** generally provides for connection of the disposable element **810** to the remainder of a sensor, such as, for example, the reusable elements. According to the exemplary embodiment, the cable connector **850** comprises a plastic plate **852** including mating portions **854**, such as, for example, raised pliable detents that each including a catch. However, an artisan will recognize from the disclosure herein any suitable mating mechanism can be used to connected the disposable element **810**, including virtually any mechanical-type mating mechanism, adhesives, hook-and-loop materials, combinations, or the like.

When the disposable element **810** is assembled as shown in FIG. 9, the bases **836** of the tabs **814** and the plate **852** communicate with the second side **824** of the top layer **812** and first side **846** of the tape layer **816** such that the bases **836** of the tabs **814** and the plate **852** are secured in position between the top layer **812** and the tape layer **816**. The raised side members of the tabs **814** extend through the plurality of apertures **832** in the top layer **812**, thereby aligning the signal apertures **838** with apertures in the top layer **812**. Moreover, as shown in the illustrated embodiment, the mating portions **854** of the cable connector **850** extend above the top layer **812**.

FIG. 10 shows a perspective view of an embodiment of a reusable element **1000**. The reusable element **1000** preferably includes a protective cover or coating **1004** covering a plurality of electronic sensor elements **1005** and a plurality of protrusions **1006**. The reusable element **1000** also includes a cable connection housing **1008**, and cord or cable **1010**. According to one embodiment, the protective cover **1004** comprises a soft material, such as a pliable rubber, plastic or the like, which preferably encapsulates and protects the electronic sensor elements **1005** from damage and advantageously protects caregivers and patients from sharp corners often associated with the reusable element **1000**, such as, for example, the protrusions **1006** or the sensor elements **1005**.

The protrusions **1006** extend from opposing sides of the reusable element **1000** in generally horizontal and opposing directions. To assemble the optical sensor, the protrusions

are aligned with the outside-facing insertion side of each of the slots **840** of the disposable element **810**, shown in FIG. 8, and are slid toward one another on each side. As can be seen in FIG. 12, an embodiment of the assembled sensor includes one or more of the protrusions **1006** abutting the blocked side of one pair of the slots **810**, while the other protrusions **1006** are proximate the blocked side of the other pair of slots **810**, thereby allowing the reusable element **1000** to self adjust and avoid the detrimental stretching forces caused from application to a measurement site.

FIG. 10 also shows the cable connection housing **1008** including insertion slots **1012** configured to receive and mate with the mating portions **854** of the cable connector **850** shown in FIG. 8. When mated, the cable connection housing **1008** provides electrical contact between the electrical leads **830** of the disposable element **810** and the sensor circuitry.

FIG. 11 illustrates a perspective view of portions of the electronic sensor elements **1005** of the reusable element **1100** without the protective cover or coating **1004**. The elements **1005** include one or more energy emitters **1102**, such as one or more LEDs, an energy detector **1104**, such as a photodetector, electrically connected to a connector **1106** through a flexible circuit **1108**. The connector **1106** is configured to electrically communicate with the leads **830** of the disposable element **810** when the sensor is assembled. Moreover, the connector **1106** is configured to electrically attach the conductive traces of the flexible circuit **1108** to the conductors of the cable **1010**.

FIG. 12 shows a perspective view of an assembled sensor **1200**. The sensor **1200** includes the reusable element **1000**, including the disposable element **810** connected to the connection housing **1008** through the mating portions **854** of the cable connector **850**, such that the breakable element **826** is part of the electrical circuitry of the sensor. In one embodiment, the sensor is inoperative or otherwise provides an indication of overuse or misuse when the breakable element **826** is broken or otherwise becomes an open circuit.

As disclosed, when connected to the disposable element **810**, the protrusions **1006** have a limited range of motion within the tabs **814**, thereby giving the reusable element **1000** a limited range of longitudinal motion independent of the disposable element **810**. As described with other embodiments, this longitudinal motion allows the disposable element **810** and the reusable element **1000** to flex independently as the sensor **1200** is attached to tissue of a user, such as a finger, toe, ear, or the like, thereby avoiding damage or unnecessarily harmful wear of the reusable element **1000**. Also, this limited range of motion ensures at least approximate proper alignment of various sensor components.

After use, as with embodiments described above, the disposable element **810** is removed and discarded, while the reusable element **812** can be sterilized and reused.

Although the foregoing invention has been described in terms of certain preferred embodiments, other embodiments will be apparent to those of ordinary skill in the art from the disclosure herein. For example, although the above sections describe a reusable element fitted with protrusions or necks and a disposable element fitted with apertures and receiving slots or straps, the embodiments can be reversed having, for example, the reusable element fitted with the apertures, receiving slots, or straps, and with the disposable element fitted with the protrusions or necks.

Additionally, other combinations, omissions, substitutions and modifications will be apparent to the skilled artisan in view of the disclosure herein. Accordingly, the present

11

invention is not intended to be limited by the reaction of the preferred embodiments, but is to be defined by reference to the appended claims.

What is claimed is:

1. A pulse oximetry sensor for outputting a signal indicative of one or more physiological parameters of tissue of a patient, the sensor comprising:

a reusable element comprising an energy emission device adapted to transmit energy into tissue of a patient, an energy detection device adapted to detect attenuated energy from the tissue and output a signal indicative of one or more physiological parameters of the tissue, and a plurality of protrusions extending from the reusable element; and

a disposable element comprising a tape adapted to removably attach to the tissue and a plurality of tabs each including a receiving slot, wherein each of the slots is adapted to receive one of the plurality of protrusions and adapted to permit the one protrusion to slide within a corresponding slot.

2. The sensor of claim 1, wherein at least one of the plurality of tabs includes a sloped surface that displaces the tab allowing receipt of the protrusion.

3. The sensor of claim 1, wherein the plurality of protrusions include protrusions that share a common substrate.

4. The sensor of claim 1, wherein the reusable element is encapsulated with a pliable material.

5. The sensor of claim 1, wherein the plurality of tabs include tabs that share a common substrate.

6. The sensor of claim 1, wherein the disposable element further comprises an information element adapted to provide information to a signal processor.

7. The sensor of claim 1, wherein some of the plurality of tabs each include an aperture, wherein each aperture is adapted to receive one of the plurality of protrusions and adapted to substantially prevent the one protrusion from sliding within a corresponding aperture.

8. A method of attaching a pulse oximetry sensor comprising a reusable element and a disposable element around a measurement site of a patient, the method comprising:

inserting protrusions of a reusable element respectively into tabs of a disposable element; and

attaching the disposable element proximate a measurement site, wherein the tabs permit slidable movements of at least a portion of the reusable element with respect to the disposable element.

9. The method of claim 8, wherein a plurality of the tabs each include a receiving slot respectively sized to receive a plurality of the protrusions, and wherein another plurality of the tabs each include an aperture.

10. A method of attaching a pulse oximetry sensor comprising a reusable element and a disposable element to a measurement site of a patient, the reusable element including a first neck section and a second neck section, each neck section being narrower than adjacent sections of the reusable element, the disposable element including a first strap and a second strap, wherein each of the straps includes a gap adapted to receive one of the neck sections, the method comprising:

placing a first neck section of a reusable sensor element within a gap of a first strap of a disposable sensor element;

12

placing a second neck section of the reusable sensor element within a gap of a second strap of the disposable sensor element; and

attaching the disposable element to a measurement site, wherein the gap of the first strap permits the first neck section movement along a longitudinal axis of the disposable element, and wherein the gap of the second strap substantially prevents movement along a longitudinal axis of the disposable element.

11. A method of assembling a sensor capable of outputting a signal indicative of one or more physiological parameters of measurement site, the method comprising:

providing a reusable element including a first assembly mechanism;

providing a disposable element including a second assembly mechanism mateable with the first assembly mechanism; and

attaching the first and second assembly mechanisms forming an assembled sensor, such that after assembly, at least a portion of the reusable element moves longitudinally with respect to the disposable element, thereby reducing or eliminating stretching forces exerted on the reusable element when the assembled sensor is applied to a measurement site.

12. The method of claim 11, wherein the first assembly mechanism comprises protrusions, and wherein the second assembly mechanism comprises tabs having slots for receiving the protrusions.

13. The method of claim 11, wherein the first assembly mechanism comprises narrow neck portions and the second assembly mechanism comprises straps.

14. A pulse oximetry sensor for outputting a signal indicative of one or more physiological parameters of tissue of a patient, the sensor comprising:

a reusable element comprising an energy emission device adapted to transmit energy into tissue of a patient, an energy detection device adapted to detect energy from the tissue and output a signal indicative of one or more physiological parameters of the tissue, a protective cover, and a plurality of protrusions extending from said protective cover;

a disposable element comprising a plurality of attachment members adapted to receive the protrusions of the reusable element and properly position the disposable element with respect to the reusable element; and

an adhesive layer adapted to removably attach the disposable element to the tissue, wherein the plurality of attachment members of the disposable element further comprises tabs with grooves that receive the protrusions.

15. The pulse oximetry sensor of claim 14, wherein the grooves allow limited movement of the protrusions.

16. The pulse oximetry sensor of claim 14, wherein the protective cover further comprises a pliable coating.

17. The pulse oximetry sensor of claim 14, wherein the cover substantially encapsulates the reusable element.

* * * * *

专利名称(译)	光学传感器包括一次性和可重复使用的元件		
公开(公告)号	US6920345	公开(公告)日	2005-07-19
申请号	US10/351645	申请日	2003-01-24
[标]申请(专利权)人(译)	AL ALI AMMAR ABDUL HAFIZ亚瑟尔		
申请(专利权)人(译)	AL-ALI AMMAR 阿卜杜勒·哈菲兹亚瑟尔		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	AL ALI AMMAR ABDUL HAFIZ YASSIR		
发明人	AL-ALI, AMMAR ABDUL-HAFIZ, YASSIR		
IPC分类号	A61B5/00		
CPC分类号	A61B5/14552 A61B5/6826 A61B5/6838 A61B5/6833 Y10T29/49826		
其他公开文献	US20040147822A1		
外部链接	Espacenet USPTO		

摘要(译)

脉搏血氧饱和度传感器包括可重复使用和一次性元件。为了组装传感器，可重复使用的元件在一次性元件的组装机构内被卡扣或滑动。在一个实施例中，可重复使用元件包括突起，而一次性元件包括接收突起的突片。在另一个实施例中，可重复使用的元件包括颈部，并且一次性元件包括接收颈部的带。无论如何，组件提供元件之间的纵向移动。

