



US007140766B2

(12) **United States Patent**
Glukhovsky et al.

(10) **Patent No.:** **US 7,140,766 B2**
(45) **Date of Patent:** **Nov. 28, 2006**

(54) **DEVICE, SYSTEM AND METHOD FOR TEMPERATURE SENSING IN AN IN-VIVO DEVICE**

(75) Inventors: **Arkady Glukhovsky**, Santa Clarita, CA (US); **Gavriel Meron**, Petach Tikva (IL); **Gavriel J. Iddan**, Haifa (IL)

(73) Assignee: **Given Imaging Ltd.**, Yoqneam (IL)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **10/643,086**

(22) Filed: **Aug. 19, 2003**

(65) **Prior Publication Data**

US 2004/0109488 A1 Jun. 10, 2004

Related U.S. Application Data

(63) Continuation-in-part of application No. 09/806,714, filed as application No. PCT/IL00/00470 on Aug. 3, 2000, now Pat. No. 6,607,301.

(30) **Foreign Application Priority Data**

Aug. 4, 1999 (IL) 131242

(51) **Int. Cl.**
G01K 7/00 (2006.01)

(52) **U.S. Cl.** 374/175; 374/121

(58) **Field of Classification Search** 374/175, 374/117, 121, 141; 250/339.04, 352; 348/243, 348/245, 909, 45, 65; 600/549, 474, 109, 600/117, 160; 327/512, 513

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,710,899 A * 6/1955 Marsden, Jr. et al. 374/175
2,768,266 A * 10/1956 Marsden, Jr. 374/175
3,882,384 A * 5/1975 List 327/512

3,937,086 A	2/1976	Von Thuna
3,971,362 A	7/1976	Pope et al.
4,177,800 A	12/1979	Enger
4,180,736 A	12/1979	Goodman
4,246,784 A	1/1981	Bowen
4,278,077 A	7/1981	Mizumoto
4,643,587 A	2/1987	Makabe et al.
4,646,723 A	3/1987	Arakawa
4,646,724 A *	3/1987	Sato et al. 600/109
4,689,621 A	8/1987	Kleinberg
4,744,672 A	5/1988	Tursky et al.
4,786,969 A *	11/1988	Shouji et al. 348/243
4,807,633 A	2/1989	Fry
4,844,076 A	7/1989	Lesho et al.
4,885,077 A	12/1989	Karakelle et al.

(Continued)

FOREIGN PATENT DOCUMENTS

DE 34 40 177 5/1986

(Continued)

OTHER PUBLICATIONS

Jones, B.K., "Electrical Noise Thermometer," Appl. Phys. vol. 16, No. 1, pp. 99-102 (May 1978).*


(Continued)

Primary Examiner—Diego Gutierrez
Assistant Examiner—Mirellys Jagan
(74) *Attorney, Agent, or Firm*—Pearl Cohen Zedek Latzer, LLP

(57) **ABSTRACT**

A device, method and system for sensing the temperature or temperature change of an environment. A typically in-vivo device includes an image sensor. The device may sense the dark current noise of the image sensor, and calculate the temperature or a temperature change of the image sensor.

7 Claims, 5 Drawing Sheets

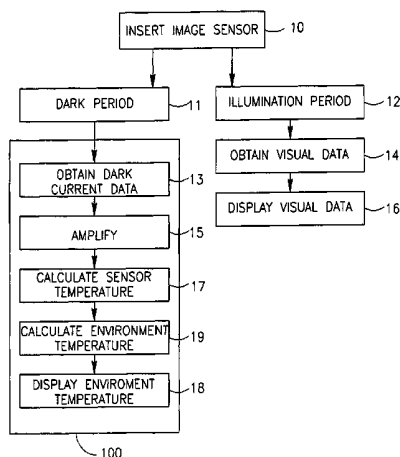

U.S. PATENT DOCUMENTS

4,891,970	A	1/1990	Remboski, Jr.	
4,936,823	A	6/1990	Colvin et al.	
5,047,863	A *	9/1991	Pape et al.	348/247
5,098,197	A	3/1992	Shepard et al.	
5,109,870	A	5/1992	Silny et al.	
5,278,656	A *	1/1994	Hynecek et al.	348/65
5,279,607	A	1/1994	Schentag et al.	
5,354,130	A	10/1994	Seppa et al.	
5,368,027	A	11/1994	Lubbers et al.	
5,508,740	A	4/1996	Myaguchi et al.	
5,604,531	A *	2/1997	Iddan et al.	600/109
5,640,235	A	6/1997	Iwasaki	
5,697,384	A	12/1997	Miyawaki et al.	
5,746,511	A	5/1998	Eryurek et al.	
5,819,736	A	10/1998	Avny et al.	
5,833,603	A	11/1998	Kovacs et al.	
5,853,005	A	12/1998	Scanlon	
5,993,378	A	11/1999	Lemelson	
6,074,349	A	6/2000	Crowley	
6,148,152	A *	11/2000	Cazier et al.	348/243
6,165,128	A	12/2000	Céspedes et al.	
6,184,511	B1	2/2001	Yamashita	
6,222,454	B1 *	4/2001	Harling et al.	250/339.04
6,240,312	B1	5/2001	Alfano et al.	
6,267,501	B1 *	7/2001	Wand et al.	348/243
6,433,333	B1 *	8/2002	Howard	250/339.04
6,584,348	B1	6/2003	Glukhovskiy	
6,607,301	B1 *	8/2003	Glukhovskiy et al.	374/175
6,614,562	B1 *	9/2003	Minemier	358/483
6,641,529	B1 *	11/2003	Kuranishi	600/109
6,927,795	B1 *	8/2005	Cazier et al.	348/243
2001/0035902	A1 *	11/2001	Iddan et al.	348/65
2002/0103417	A1	8/2002	Gazdzinski	
2002/0146368	A1	10/2002	Meron et al.	
2002/0175269	A1 *	11/2002	Krymski	250/208.1
2003/0002624	A1 *	1/2003	Rinaldi et al.	378/98.8
2003/0040685	A1	2/2003	Lewkowicz et al.	
2003/0077223	A1	4/2003	Glukhovskiy et al.	
2003/0167000	A1	9/2003	Mullick et al.	
2003/0208107	A1	11/2003	Rafael	
2004/0036776	A1 *	2/2004	Wakabayashi et al. .	348/207.99
2004/0099920	A1 *	5/2004	Rossi et al.	257/448
2004/0122315	A1 *	6/2004	Krill	600/549
2004/0170215	A1 *	9/2004	Rossi et al.	374/121

FOREIGN PATENT DOCUMENTS

EP	0 667 115	8/1995
----	-----------	--------

GB	2353166	2/2001
JP	57-45833	3/1982
JP	4-109927	4/1992
JP	4109927	4/1992
JP	5015515	1/1993
JP	6-114036	4/1994
JP	8-201170	8/1996
JP	9-45893	2/1997
WO	WO 9930610 A1 *	6/1999
WO	WO 01/50941	7/2001

OTHER PUBLICATIONS

Holst, G.C., "CCD arrays cameras and displays", Second Edition (SPIE O.E. Press and JCD Publ.), chap. 4. pp. 102-145 (1998, no month).*

Ritter, T., "Random Electrical Noise: A Literature Survey, Research Comments from Ciphers By Ritter," www.io.com, (Dec. 1999).*

Eric R. Fossum, Digital Camera System on a Chip, IEEE Micro, May-Jun. 1998, pp. 8-15.*

BBC News Online—Pill camera to 'broadcast from the gut', Feb. 21, 2000, www.news.bbc.co.uk.

Wang, et al., "Integrated Micro-Instrumentation for Dynamic Monitoring of the Gastro-Intestinal Tract", Presented at IEEE Instrumentation and Measurement Technology Conference, May 2002, Anchorage, Ak, USA. www.see.ed.ac.uk/Naa.publications.html.

The Radio Pill, Rowlands, et al., British Communications and Electronics, Aug. 1960, pp. 598-601.

Video Camera to "TAKE"—RF System lab, no date available, (1 page).

Wellesley company sends body montiors into space—Crum, Apr. 1998, Boston Business Journal, p. 7.

Wireless transmission of a color television moving image from the stomach using a miniature CCD camera, light source and micro-wave transmitter. Swain CP, Gong F, Mills TN. Gastrointest Endosc 1997;45:AB40, (Apr. 1997).

Photobit PB-159 DX Product Specification, Aug. 1998 (Version 3.0), (1 pg).

"Robots for the future"—Shin-ichi, et al., Nov. 29, 2001, (12 pages). NORIKA3, Dec. 24, 2001, (14 pages), www.rfnorika.com.

European Search Report for EP 04 01 9677 mailed on Nov. 4, 2005.

Japanese Office Action for JP Application No. 2001-514821—prior art search record, mailed on Feb. 21, 2006.

* cited by examiner

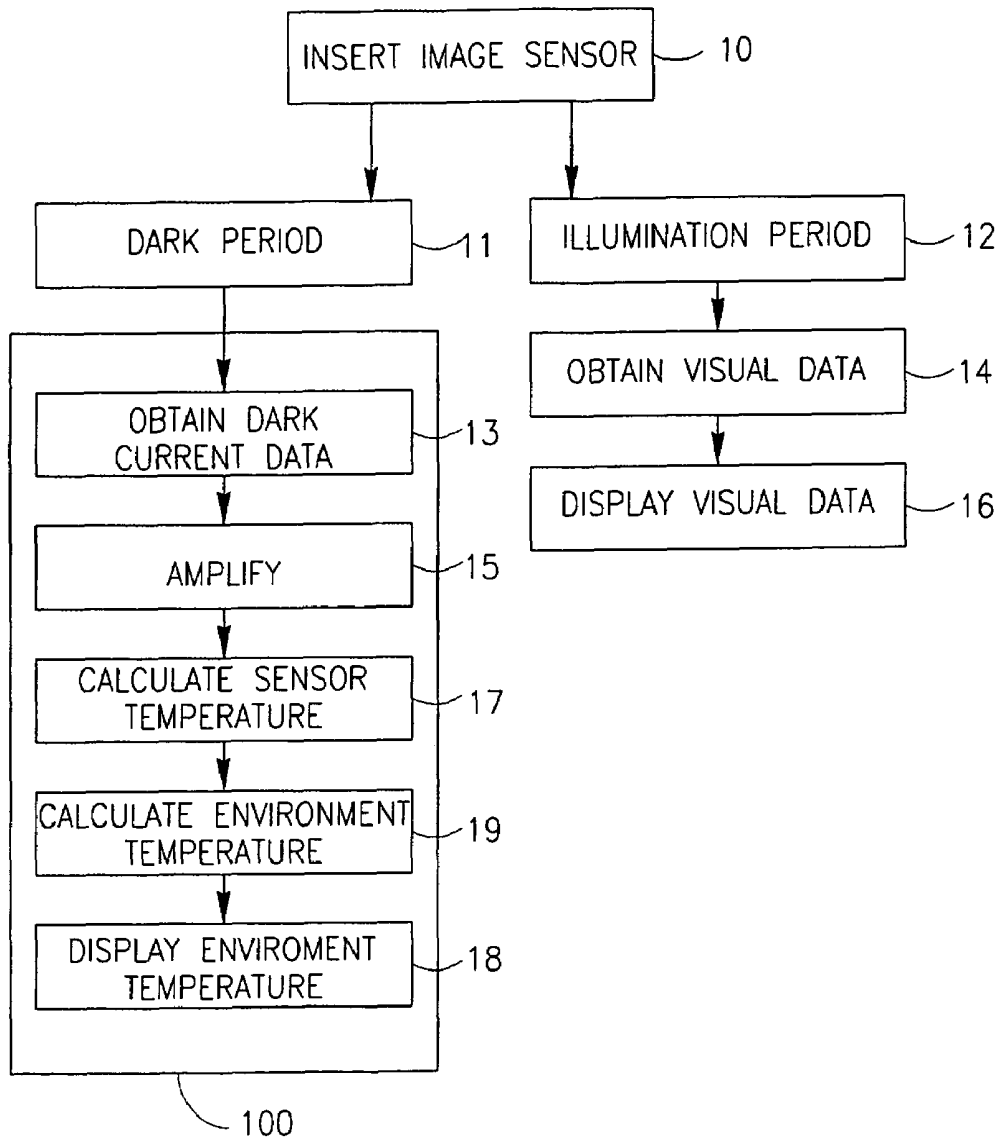


FIG. 1

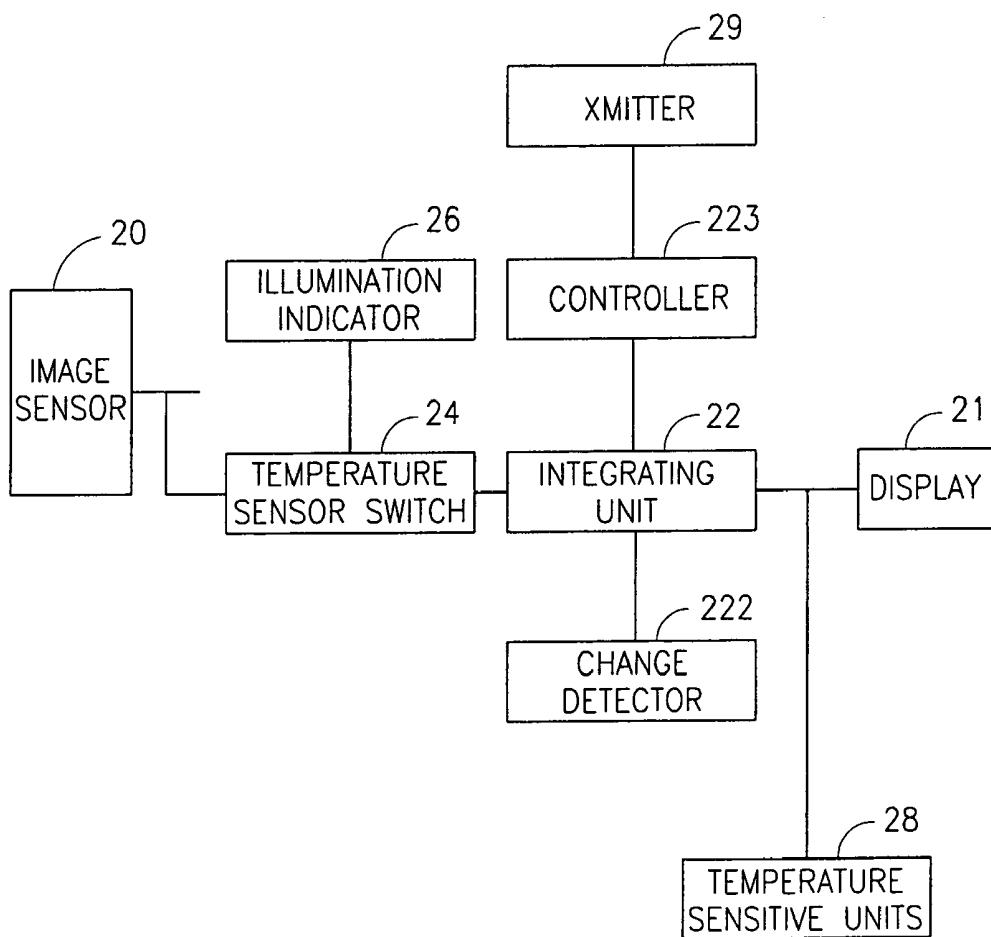


FIG. 2

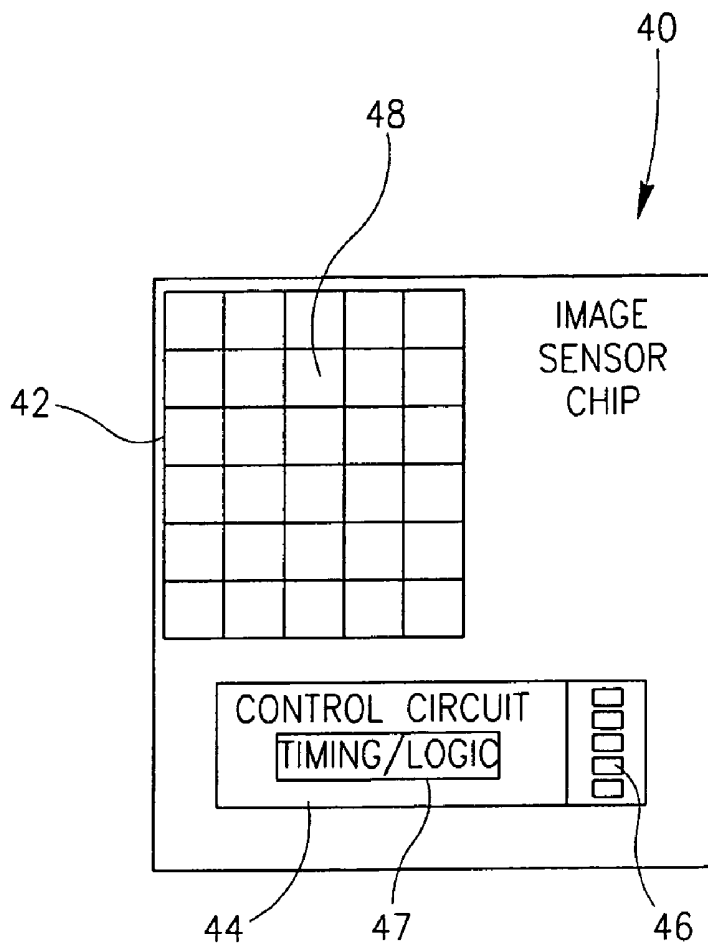


FIG. 3

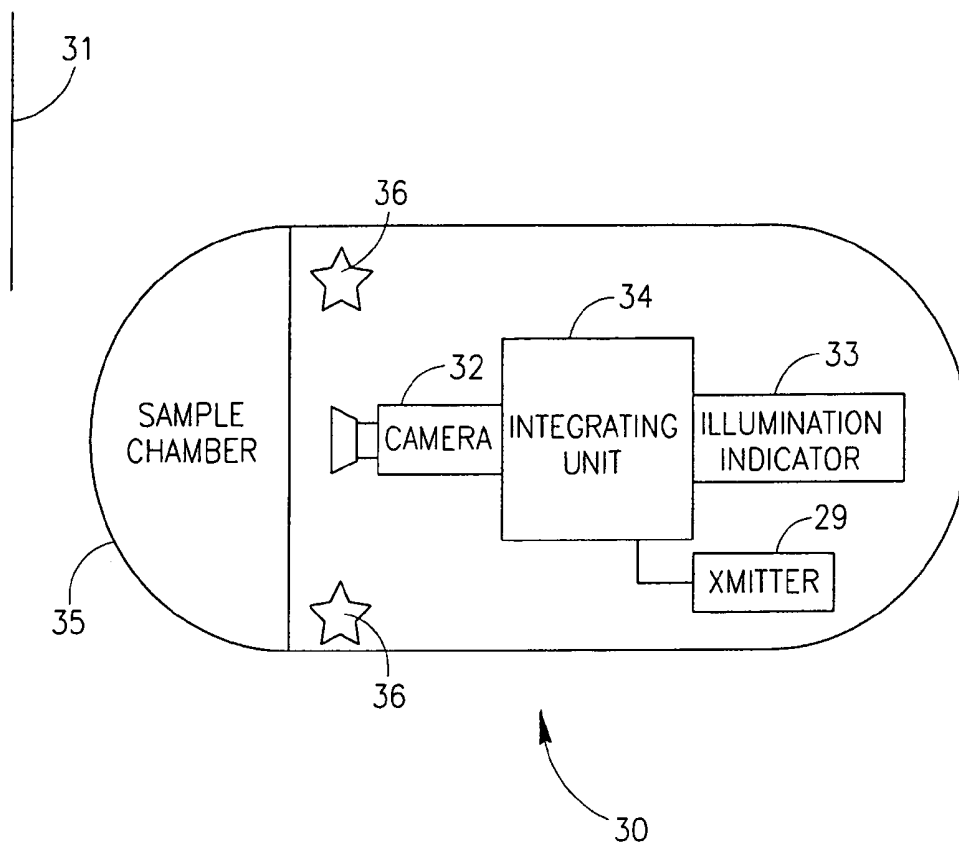


FIG. 4

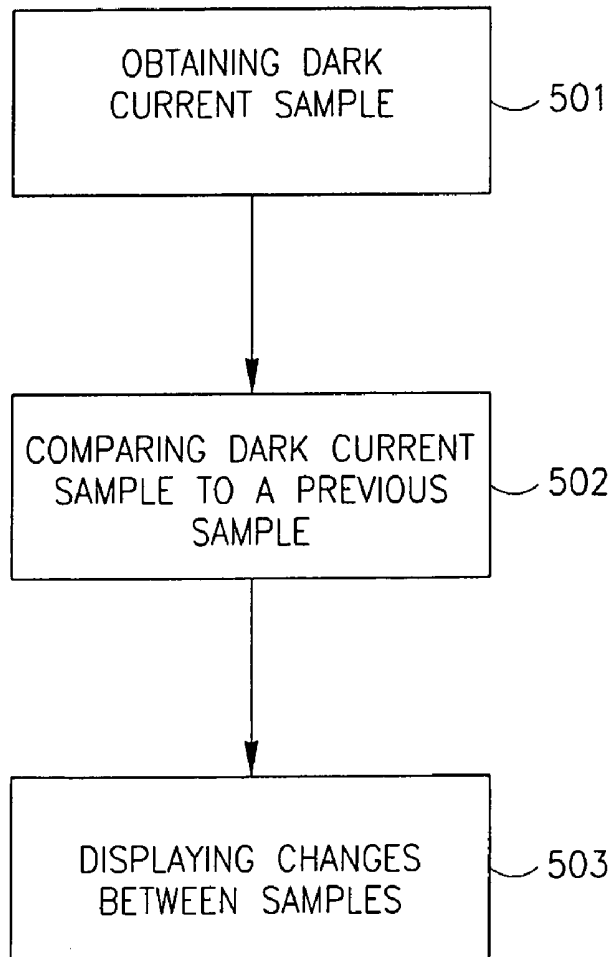


FIG. 5

DEVICE, SYSTEM AND METHOD FOR TEMPERATURE SENSING IN AN IN-VIVO DEVICE

RELATED APPLICATION DATA

The present application is a continuation-in-part of U.S. application Ser. No. 09/806,714 filed on Oct. 9, 2001 now U.S. Pat. No. 6,607,301 and entitled "DEVICE AND METHOD FOR DARK CURRENT NOISE TEMPERATURE SENSING IN AN IN-VIVO IMAGING DEVICE," which in turn claims priority from International Application number PCT/IL00/00470 filed 3 Aug. 2000 and Israeli application number 131242 filed Aug. 4, 1999.

FIELD OF THE INVENTION

The present invention relates to a method and system for measuring the temperature of an environment, such as the interior of the body.

BACKGROUND OF THE INVENTION

In many circumstances it is important to measure the temperature inside a material body. Such circumstances may occur during industrial processes or exploration and analysis processes, such as in geophysical probing or in medical diagnostics and treatment of internal parts of the body.

Conventional thermometry and absolute thermometry are known methods for measuring temperature.

Conventional thermometry is based upon the temperature coefficient of properties of materials, such as resistance or mechanical expansion.

Absolute thermometry is a method which directly measures thermal energy of a sensor resistance. This method is based upon the known physical phenomenon of spontaneous thermal noise arising from the Brownian motion of ionized molecules within a resistance.

Thermal noise, which can be discussed in terms of thermal current, provides a direct measurement of temperature on a thermodynamic scale, thus the Boltzmann constant defines the temperature. The phenomenon of thermal noise is derived, for example, in the book: *CCD arrays cameras and displays* by Holst G. C., p. 128, 2nd edition, SPIE Press, 1998. A formula that may be used to define thermal current is, for example:

$$\langle i_n^2 \rangle = k T C$$

where k is the Boltzmann constant, T is the temperature of a sensor, and C is the capacitance of the sensor. Thus the magnitude of the signals produced by the thermal current is directly proportional to the square root of the temperature of the sensor. Experiments have indicated that the signal doubles with the increase of 7° C. (degrees Centigrade), which means that a resolution better than 0.1° C. is achieved.

In image sensors, the thermal current produced in an operating photodetector device, when no optical radiation impinges on the detector, is called "dark current". In CCD cameras dark current is basically charge which accumulates in the CCD pixels due to thermal noise. The effect of dark current is to produce an additive quantity to the electron count in each pixel.

U.S. Pat. No. 3,937,086 to von Thuna, U.S. Pat. No. 5,354,130 to Seppa et al. and U.S. Pat. No. 5,098,197 to Shepard et al. all describe devices for measuring the absolute

temperature of a body material by receiving and analyzing the thermal noise of the body material.

U.S. Pat. No. 4,246,784 to Bowen describes a method for noninvasive temperature measurement of the interior of a body using the acoustic thermal noise spectrum of the measured body.

None of these temperature measurement methods utilize an image sensor to measure the thermal noise of a body material.

SUMMARY OF THE INVENTION

Embodiments of the present invention provide a method and system for sensing the temperature or temperature change of an environment, such as inside a body, by calculating the temperature of an image sensor in the environment and deducing the environment's temperature from the image sensor's calculated temperature. The temperature or temperature change of the image sensor may be calculated by measuring its generated dark current noise.

Embodiments of the present invention may use an image sensor, in which thermal noise is easily detectable, for deducing the temperature of a material body. Furthermore, according to embodiments of the invention, a single sensor is utilized for obtaining visual data and data relating to the temperature of the environment. Thus, diverse information about an environment can be obtained utilizing a single sensing device.

There is thus provided according to an embodiment of the present invention a method for sensing the temperature of an environment comprising the steps of introducing into an environment an image sensor having an image sensing module, sensing the dark current noise of the image sensor, calculating the temperature of the image sensor, calculating the temperature of the environment and optionally displaying the calculated environment temperature.

It will be appreciated that the term "environment" when used herein relates to a space enclosed within walls in which it is desired to measure the temperature of the space and/or of the walls.

The temperature of the image sensor is indicative of the temperature of its immediate surroundings and, relying on known factors such as heat distribution, distance from the image sensor, etc., the temperature of further areas can also be calculated.

The image sensors utilized in embodiments of the invention can be for example digital cameras or video cameras such as vidicon, CCD cameras or Complementary Metal Oxide Semiconductor (CMOS) cameras.

Embodiments of the present invention further provide a system for sensing the temperature of an environment. The system comprises an image sensor having an image sensing module in communication with an integrating unit for detecting the dark current of the image sensor image sensing module and for calculating the temperature of the image sensor. The integrating unit may further calculate the temperature of the environment or the temperature of the environment may be calculated, based on data from the integrating unit, by a separate unit that is in communication with the integrating unit.

The integrating unit may have an amplifying function for amplifying signals received from the image sensor.

The communication between the image sensor and integrating unit can be optionally controlled according to the illumination conditions, optionally through a switch which enables communication only during periods in which the sensor is not illuminated.

BRIEF DESCRIPTION OF THE DRAWINGS

The present invention will be understood and appreciated more fully from the following detailed description taken in conjunction with the figures in which:

FIG. 1 is a block diagram representing an embodiment of the method according to an embodiment of the invention;

FIG. 2 is a schematic illustration of an embodiment of the system according to an embodiment of the invention;

FIG. 3 is a schematic illustration of a functional block layout of the image sensor according to an embodiment of the invention;

FIG. 4 is a schematic illustration of a medical device comprising the system according to an embodiment of the invention; and

FIG. 5 is a block diagram representing an embodiment of a method according to an embodiment of the invention.

DETAILED DESCRIPTION OF THE INVENTION

In the following detailed description, numerous specific details are set forth in order to provide a thorough understanding of the invention. However, it will be understood by those of ordinary skill in the art that the invention may be practiced without these specific details. In other instances, well-known methods, procedures, components, units and/or circuits have not been described in detail so as not to obscure the invention.

Analytical and diagnostic processes which utilize image sensors to monitor environments could benefit from obtaining information relating to the temperature of the environment, as a local change of temperature can indicate an irregular event.

For example, some embodiments described in U.S. Pat. No. 5,604,531, which is assigned to the common assignees of the present application, describe a swallowable device that can pass through the entire digestive tract and operate as an autonomous video endoscope. U.S. Pat. No. 5,604,531, is hereby incorporated by reference. The swallowable device may include a) a camera system, b) an optical system for imaging an area of interest onto the camera system and c) a transmitter which transmits the video output of the camera system and/or other data. Visual data obtained by the swallowable device can indicate, inter alia, the location of pathologies in the gastrointestinal tract. Also a local change of temperature in the gastrointestinal tract can be indicative of a pathology. Thus, the information obtained by visual means can be complemented and focused by information relating to local temperature in the gastrointestinal tract. An external receiving, processing and/or display system may receive, process and or display data received from the device.

The method of an embodiment of the present invention may enable simultaneous visual monitoring and temperature sensing.

The method is schematically described by a block diagram shown in FIG. 1. An image sensor, such as in the above mentioned swallowable device, is inserted **10** into an environment, such as the gastrointestinal tract. The swallowable device **30** is typically capsule shaped, but may have other shapes and need not be swallowable.

Illumination is provided intermittently, either by elements connected to the image sensor itself or by external sources. When illumination is provided **12** only visual data is obtained **14** and displayed **16**. A process for obtaining and

displaying visual data is described, for example, in the above mentioned U.S. Pat. No. 5,604,531.

In an intermittent dark period **11** an integrating unit **100** is activated to obtain dark current data **13** from the image sensor, though it is not imperative to shut off illumination in order to obtain data relating to dark current noise, as will be discussed in more detail below.

The integrating unit **100** is a processor capable of amplifying the obtained data **15**, if necessary, and calculating the image sensor temperature **17** using the known equations derived for thermal noise. It will be appreciated that these equations are an approximation of a complex phenomenon and that calibration should be employed in order to deduce the actual calculations that will be applied. According to some embodiments, for example, as schematically illustrated in FIG. 5, the image sensor temperature and/or the environment temperature need not be calculated. Rather, a difference in dark current measurements (which are typically indicative of temperature changes) may be determined. Thus, a difference in temperature changes may be determined or calculated. In one embodiment, the amount of temperature change need not be determined, but rather that a temperature change occurred, and, possible, the direction of temperature change (hotter, cooler).

According to an embodiment of the invention a dark current data sample may be obtained (**501**), for example, according to a predetermined schedule or by any other appropriate method (for example, as discussed below). Dark current data sample may be compared, for example by using a change detector, to a previous dark current sample (**502**). A difference between two samples can indicate a temperature change. According to some embodiments a sample may be compared to an average or other manipulation of several previous samples. Thus, the actual temperature of the image sensor and/or of the body lumen environment need not be calculated.

According to some embodiments a change in dark current data may be displayed (**503**). According to other embodiments only a change which is above a predetermined threshold may be displayed. According to yet further embodiments a change which is over a predetermined threshold may be used as a trigger for changing the activity of other elements of the system. For example, a swallowable device, such as described in the above mentioned U.S. Pat. No. 5,604,531, may include an integrating unit or other calculating unit which may be capable of detecting a change in dark current data, as described above. The integrating unit may be in communication with other elements of the device, such as the power supply or the illumination system or transmitter of the device, and an ON or OFF signal may be generated, typically by the integrating unit, to any of these elements in accordance with detected dark current changes. Thus, the operational mode or settings of an in vivo sensor can be altered or activated in response to in vivo temperature. According to certain embodiments, a swallowable device may include a controller or calculating unit for activating or altering the operational mode or settings of the device in response to signals from the integrating unit. Such an embodiment may be useful in some case for example, for saving energy. According to one embodiment after a device or other in-vivo device is swallowed the patient is made to ingest a volume of cold or hot water at regular intervals. According to one embodiment the patient ingests cold or hot water over a period of a few hours, for example, a period in which the device has most probably left the stomach. While the device is in the stomach an ingested volume of cold or hot water may cause a change of temperature in the stomach

environment, Once in the small intestine, the effect of a cold or hot drink is no longer felt. According to one embodiment of the invention a change of temperature may be checked at predetermined intervals. While a temperature change (typically above a predetermined threshold) is detected the device may be kept inactive. If a temperature change is not sensed the device may be triggered to activate the device. Thus, the device begins collecting data only when it is close to the large intestine thereby saving energy and allowing effective and complete action of the device in the large intestine.

The environment temperature or a change in environment temperature is then calculated **19**, by the integrating unit **100**, by a separate unit in communication with the integrating unit **100**, or possibly by another unit. Calculations of the environment temperature may be based on the existence of thermal equilibrium between the image sensor and environment. These calculations take into account energy dissipation from the image sensor. Local temperature or the average temperature within the environment may be calculated, depending on specific requirements. The calculated temperature may then be displayed **18**.

It will be appreciated that the various calculations and/or detections may be carried out by software or software means executable on computing means such as a computer or similar data processors, microprocessors, embedded processors, microcomputers, microcontrollers etc.

The integrating unit **100** may include separate processors, which need not all be physically connected. Some of the functions carried out by integrating unit **100**, such as calculating the image sensor temperature **17** and calculating the environment temperature **19**, can be carried out in processors that are external to the environment and that are fed with data from the integrating unit **100** by communication such as by IR or radio. Indeed, if an operator is to note the temperature of the environment, at least the function of displaying the calculated temperature **18** must be performed externally to the environment.

Integrating unit **100** may be in communication with other units to further process and use the data obtained by it. For example, a device, such as described in U.S. Pat. No. 5,604,531, may include a sample chamber for collecting samples from the environment of the digestive tract. The process of collecting a sample can be controlled by integrating unit **100**, such that samples are collected only in locations along the digestive tract in which a predetermined temperature is prevalent or in which a certain temperature change has been detected.

Reference is now made to FIG. 2, which is a schematic illustration of the system according to an embodiment of the invention. The system includes an image sensor **20** having an image sensing module which includes a pixel array (as demonstrated in FIG. 3) in communication with an integrating unit **22**. Communication is enabled by temperature sense switch **24** which is controlled by illumination indicator **26**, such that communication is enabled only during dark periods.

When communication between the image sensor **20** and integrating unit **22** is established, integrating unit **22** receives dark current data from image sensor **20**.

In an alternate embodiment a switch and/or illumination indicator need not be used. According to some embodiments dark current data may be received from the image sensor **20** continuously or according to a predetermined time schedule. For example, a system in which 25 ms light flashes are followed by 475 ms dark periods, may be programmed to sample dark current data once every dark period. In an

alternate embodiment a system may include a dark frame once every so often, e.g., one frame in every 256 frames is not illuminated. According to some embodiments a system may be programmed to sample dark current data -during a dark frame. Other time periods or intervals may be used.

It is possible to calculate the image sensor's **20** temperature or temperature change based on dark current data obtained from a single pixel of the image sensor pixel array, though data obtained from a higher number of pixels may achieve more accurate results. It is therefore possible to keep a portion of the image sensor's **20** pixels of the pixel array, constantly unexposed to illumination, and obtain dark current data from the unexposed pixels, without having to shut off the illumination. Thus simultaneous image capture and and temperature sensing may be carried out.

Thus, dark current data can be obtained also during constant illumination by either covering a portion of the pixels of the pixel array or by having a portion of the pixel array pixels outside of the image field, e.g. the pixels in the periphery of the pixel array.

The integrating unit **22** may be or include a processor capable of amplifying the dark current signal and calculating the image sensor temperature from the dark current signal. It may be capable of calculating the environment temperature from the image sensor temperature and is capable of displaying the calculated environment temperature **21**. Integrating unit **22** may control different temperature sensitive units **28**, such as a sample chamber, in correspondence with predetermined temperatures or temperature changes. A transmitter **29** may transmit data such as image data, dark current data, temperature data, and/or temperature change data.

The system may also include a change detector **222** (typically in communication with the integrating unit **22**) and a controller **225** for activating or altering the operational mode or settings of the device in response to signals from the integrating unit **22** or another unit,

The various processing and detecting components described herein, and their functionalities, may be combined over different components than separately shown. For example, a single controller may perform all functionality. In one embodiment control and calculation capability may be included within transmitter **29**.

Reference is now made to FIG. 3 which is a schematic illustration of a functional block layout of the image sensor according to an embodiment of the invention. The image sensor typically includes a single chip **40** having an image sensing module **42** and a control circuits area **44**. The image sensing module **42** includes a pixel array **48** for capturing an image. The control circuits area **44** includes the timing and logic circuitry **47** and AND circuitry **46**.

Signals can be received from all the pixels of the pixel array **48**. Dark current is received from pixels that are not illuminated or from pixels during a dark period whereas current signals received from an illuminated pixel are the summation of the dark current and light current of the pixel. The accumulation of signals from all the pixels is converted to data which is communicated through a transmitter such as transmitter **29** to the integrating unit for decoding and for displaying a visual representation and/or the temperature derived from the data.

The system of an embodiment of the invention will be further described and demonstrated by FIG. 4 which is a schematic illustration of a medical device comprising a system according to an embodiment of the invention.

The medical device illustrated in FIG. 4 is a swallowable device, generally referenced **30**. Device **30** which may

include components and functionality similar to that described in the above mentioned U.S. Pat. No. 5,604,531, but alternately may be of different construction and include different functionality and components. Swallowable device **30** is typically capsule shaped, but may have other shapes and need not be swallowable. Swallowable device **30** comprises a CMOS camera **32**, that is in communication with integrating unit **34**. The swallowable device **30** further comprises illuminating elements **36** that are in communication with illumination indicator **33**. The gastrointestinal tract walls **31** are illuminated by illuminating elements **36**, in intermittent pulses, capturing consecutive images of the gastrointestinal tract walls **31** by camera **32**, enabling an operator to view the gastrointestinal tract walls. Communication between camera **32** and integrating unit **34** is enabled in between illumination pulses when illumination indicator **33**, sensing the lack of illumination, activates the temperature sense switch (not shown) to an ON position.

Alternatively, the illumination indicator **33** may be activated by the operator to simultaneously turn off the illumination elements **36** and switch the temperature sense switch to an ON position.

Once communication is established between camera **32** and integrating unit **34** dark current signals generated from camera **32** may be received and processed, as described above, by integrating unit **34**. The calculated gastrointestinal temperature, or temperature change may be displayed on a display unit external to the gastrointestinal tract. For example, a workstation or personal computer may indicate that a change in temperature occurred, the direction of temperature change, and/or the amount of temperature change. Other body lumens may have temperature or temperature change detected.

All or part of the functionality of receiving dark current data and calculating a temperature or temperature change may be carried out by parts of an external receiving, processing and/or display system, such as a remote personal computer or workstation.

Swallowable device **30** may include a sample chamber **35** for collecting samples from the gastrointestinal tract environment. The collected sample may be cells from the gastrointestinal tract walls or a liquid sample from the gastrointestinal tract environment. The mechanism for collecting samples, which can be any suitable mechanism known in the art, is controlled by integrating unit **34**, such that it is activated in accordance with the gastrointestinal tract environment calculated temperature. Alternatively, the mechanism can be controlled by the operator based on the displayed temperature.

It will be appreciated by persons skilled in the art that the present invention is not limited to what has been particularly shown and described hereinabove.

The invention claimed is:

1. A method for calculating a temperature change in vivo, the method comprising:

introducing in vivo an image sensor having an image sensing module;

sensing the dark current noise of the image sensing module;

obtaining a dark current data sample according to a predetermined time schedule during at least one dark period during which the image sensor is not illuminated;

comparing a dark current data sample of the sensed dark current noise to a previous sample; and

calculating the temperature change in vivo according to the comparison;

wherein the image sensor is contained within a capsule.

2. A method according to claim **1**, comprising displaying the in vivo temperature.

3. A system for calculating a temperature change in vivo comprising:

a capsule comprising:

an image sensor;

an integrating unit; and

a change detector;

said image sensor contained within said capsule and being introduced in vivo; and

said integrating unit receiving dark current noise samples from the image sensor according to a predetermined time schedule during at least one dark period during which the image sensor is not illuminated, and said change detector detecting changes between said dark current noise samples and calculating the temperature change in vivo according to the changes.

4. A system according to claim **3**, wherein communication between said integrating unit amplifies said dark current noise samples received from said image sensor by said integrating unit.

5. A system according to claim **3**, wherein said image sensor and said integrating unit are controlled according to an illumination condition.

6. A system according to claim **3**, wherein said image sensor senses the dark current noise during a dark period.

7. A system according to claim **3**, wherein said image sensor communicates with said controller during periods when said image sensor is not illuminated.

* * * * *

专利名称(译)	用于体内装置中的温度感测的装置，系统和方法		
公开(公告)号	US7140766	公开(公告)日	2006-11-28
申请号	US10/643086	申请日	2003-08-19
[标]申请(专利权)人(译)	GLUKHOVSKY阿尔卡季 MERON GAVRIEL IDDAN GAVRIEL J		
申请(专利权)人(译)	GLUKHOVSKY阿尔卡季 MERON GAVRIEL IDDAN GAVRIEL J.		
当前申请(专利权)人(译)	基文影像有限公司.		
[标]发明人	GLUKHOVSKY ARKADY MERON GAVRIEL IDDAN GAVRIEL J		
发明人	GLUKHOVSKY, ARKADY MERON, GAVRIEL IDDAN, GAVRIEL J.		
IPC分类号	G01K7/00 A61B5/01 A61B1/00 A61B1/04 A61B1/05 A61B5/00 A61B5/07 G01K G01K7/30		
CPC分类号	A61B1/04 A61B1/041 A61B5/0008 A61B5/01 G01K7/30		
审查员(译)	古铁雷斯DIEGO		
优先权	131242 1999-08-04 IL PCT/IL2000/000470 2000-08-03 WO		
其他公开文献	US20040109488A1		
外部链接	Espacenet USPTO		

摘要(译)

一种用于感测环境的温度或温度变化的装置，方法和系统。典型的体内装置包括图像传感器。该装置可以感测图像传感器的暗电流噪声，并计算图像传感器的温度或温度变化。

