



US008376955B2

(12) **United States Patent**
Baker, Jr.

(10) **Patent No.:** **US 8,376,955 B2**
(45) **Date of Patent:** **Feb. 19, 2013**

(54) **SPECTROSCOPIC METHOD AND SYSTEM
FOR ASSESSING TISSUE TEMPERATURE**

(75) Inventor: **Clark R. Baker, Jr.**, Newman, CA (US)

(73) Assignee: **Covidien LP**, Mansfield, MA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 588 days.

(21) Appl. No.: **12/569,721**

(22) Filed: **Sep. 29, 2009**

(65) **Prior Publication Data**

US 2011/0077547 A1 Mar. 31, 2011

(51) **Int. Cl.**

A61B 5/01 (2006.01)

A61B 5/00 (2006.01)

(52) **U.S. Cl.** **600/549**; 600/310; 600/340

(58) **Field of Classification Search** 600/310,
600/340, 549

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,638,640 A	2/1972	Shaw
3,884,219 A	5/1975	Richardson et al.
3,926,177 A	12/1975	Hardway et al.
4,028,139 A	6/1977	Smith et al.
4,714,341 A	12/1987	Hamaguri et al.
4,805,623 A	2/1989	Jöbbsis
4,807,631 A	2/1989	Hersh et al.
4,911,167 A	3/1990	Corenman et al.
4,913,150 A	4/1990	Cheung et al.
4,936,679 A	6/1990	Mersch
4,938,218 A	7/1990	Goodman et al.
4,971,062 A	11/1990	Hasebe et al.
4,972,331 A	11/1990	Chance

4,974,591 A	12/1990	Awazu et al.
5,002,060 A	3/1991	Nedivi
5,028,787 A	7/1991	Rosenthal et al.
5,065,749 A	11/1991	Hasebe et al.
5,084,327 A	1/1992	Stengel
5,119,815 A	6/1992	Chance
5,122,974 A	6/1992	Chance
5,167,230 A	12/1992	Chance
5,190,038 A	3/1993	Polson et al.
5,246,003 A	9/1993	DeLonzor
5,247,931 A	9/1993	Norwood
5,263,244 A	11/1993	Centa et al.
5,275,159 A	1/1994	Griebel
5,279,295 A	1/1994	Martens et al.
5,297,548 A	3/1994	Pologe
5,355,880 A	10/1994	Thomas et al.

(Continued)

FOREIGN PATENT DOCUMENTS

EP	0615723	9/1994
EP	0630203	12/1994

(Continued)

OTHER PUBLICATIONS

Barnum, P.T., et al.; "Novel Pulse Oximetry Technology Capable of Reliable Bradycardia Monitoring in the Neonate," *Respiratory Care*, vol. 42, No. 1, p. 1072 (Nov. 1997).


(Continued)

Primary Examiner — Sean Dougherty

(57) **ABSTRACT**

According to various embodiments, a medical system and method for determining tissue temperature may include a spectroscopic sensor. The spectroscopic sensors may be configured to provide information about changes in water absorption profiles at one or more absorption peaks. Such sensors may be incorporated into ablation systems for tissue ablation. Temperature information may be used to determine the scope, volume, and/or depth of the ablation.

16 Claims, 5 Drawing Sheets

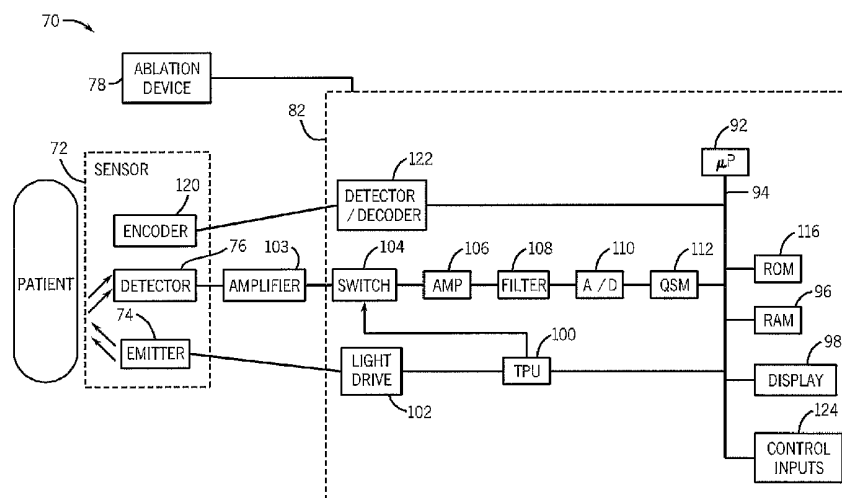

U.S. PATENT DOCUMENTS			
5,372,136 A	12/1994	Steuer et al.	
5,385,143 A	1/1995	Aoyagi	
5,390,670 A	2/1995	Centa et al.	
5,413,099 A	5/1995	Schmidt et al.	
5,469,845 A	11/1995	DeLonzor et al.	
5,482,036 A	1/1996	Diab et al.	
5,483,646 A	1/1996	Uchikoga	
5,553,614 A	9/1996	Chance	
5,564,417 A	10/1996	Chance	
5,575,285 A	11/1996	Takanashi et al.	
5,611,337 A	3/1997	Bukta	
5,630,413 A	5/1997	Thomas et al.	
5,638,816 A	6/1997	Kiani-Azarbayjany et al.	
5,645,059 A	7/1997	Fein et al.	
5,645,060 A	7/1997	Yorkey	
5,662,643 A *	9/1997	Kung et al.	606/3
5,680,857 A	10/1997	Pelikan et al.	
5,680,871 A	10/1997	Ganshorn	
5,682,898 A	11/1997	Aung et al.	
5,692,503 A	12/1997	Kuenstner	
5,730,124 A	3/1998	Yamauchi	
5,758,644 A	6/1998	Diab et al.	
5,779,631 A	7/1998	Chance	
5,782,757 A	7/1998	Diab et al.	
5,786,592 A	7/1998	Hök	
5,830,136 A	11/1998	DeLonzor et al.	
5,830,139 A	11/1998	Abreu	
5,831,598 A	11/1998	Kauffert et al.	
5,842,981 A	12/1998	Larsen et al.	
5,871,442 A	2/1999	Madarasz et al.	
5,873,821 A	2/1999	Chance et al.	
5,920,263 A	7/1999	Huttenhoff et al.	
5,995,855 A	11/1999	Kiani et al.	
5,995,856 A	11/1999	Mannheimer et al.	
5,995,859 A	11/1999	Takahashi	
6,011,986 A	1/2000	Diab et al.	
6,064,898 A	5/2000	Aldrich	
6,081,742 A	6/2000	Amano et al.	
6,088,607 A	7/2000	Diab et al.	
6,117,075 A	9/2000	Barnea	
6,120,460 A	9/2000	Abreu	
6,134,460 A	10/2000	Chance	
6,150,951 A	11/2000	Olejniczak	
6,154,667 A	11/2000	Miura et al.	
6,163,715 A	12/2000	Larsen et al.	
6,181,958 B1	1/2001	Steuer et al.	
6,181,959 B1	1/2001	Schöllermann et al.	
6,230,035 B1	5/2001	Aoyagi et al.	
6,266,546 B1	7/2001	Steuer et al.	
6,285,895 B1	9/2001	Ristolainen et al.	
6,309,352 B1	10/2001	Oraevsky et al.	
6,312,393 B1	11/2001	Abreu	
6,353,750 B1	3/2002	Kimura et al.	
6,397,091 B2	5/2002	Diab et al.	
6,405,069 B1	6/2002	Oraevsky et al.	
6,415,236 B2	7/2002	Kobayashi et al.	
6,419,671 B1	7/2002	Lemberg	
6,438,399 B1	8/2002	Kurth	
6,461,305 B1	10/2002	Schnall	
6,466,809 B1	10/2002	Riley	
6,487,428 B1	11/2002	Culver et al.	
6,487,439 B1	11/2002	Skladnev et al.	
6,501,974 B2	12/2002	Huiku	
6,501,975 B2	12/2002	Diab et al.	
6,514,278 B1 *	2/2003	Hibst et al.	607/89
6,526,298 B1 *	2/2003	Khalil et al.	600/310
6,526,301 B2	2/2003	Larsen et al.	
6,544,193 B2	4/2003	Abreu	
6,546,267 B1	4/2003	Sugiura et al.	
6,549,795 B1	4/2003	Chance	
6,580,086 B1	6/2003	Schulz et al.	
6,591,122 B2 *	7/2003	Schmitt	600/310
6,594,513 B1	7/2003	Jobsis et al.	
6,606,509 B2	8/2003	Schmitt	
6,606,511 B1	8/2003	Ali et al.	
6,615,064 B1	9/2003	Aldrich	
6,618,042 B1	9/2003	Powell	
6,622,095 B2	9/2003	Kobayashi et al.	
6,654,621 B2	11/2003	Palatnik et al.	
6,654,624 B2	11/2003	Diab et al.	
6,658,276 B2	12/2003	Kianl et al.	
6,658,277 B2	12/2003	Wasserman	
6,662,030 B2 *	12/2003	Khalil et al.	600/316
6,668,183 B2	12/2003	Hicks et al.	
6,671,526 B1	12/2003	Aoyagi et al.	
6,671,528 B2	12/2003	Steuer et al.	
6,678,543 B2	1/2004	Diab et al.	
6,679,837 B2 *	1/2004	Daikuzono	600/157
6,684,090 B2	1/2004	Ali et al.	
6,690,958 B1	2/2004	Walker et al.	
6,697,658 B2	2/2004	Al-Ali	
6,708,048 B1	3/2004	Chance	
6,711,424 B1	3/2004	Fine et al.	
6,711,425 B1	3/2004	Reuss	
6,711,426 B2	3/2004	Benaron et al.	
6,714,245 B1	3/2004	Ono	
6,723,077 B2	4/2004	Pickup et al.	
6,731,274 B2	5/2004	Powell	
6,748,259 B1	6/2004	Benaron et al.	
6,785,568 B2	8/2004	Chance	
6,793,654 B2	9/2004	Lemberg	
6,801,797 B2	10/2004	Mannheimer et al.	
6,801,798 B2	10/2004	Geddes et al.	
6,801,799 B2	10/2004	Mendelson	
6,829,496 B2	12/2004	Nagai et al.	
6,850,053 B2	2/2005	Daalmans et al.	
6,855,112 B2	2/2005	Kao et al.	
6,863,652 B2	3/2005	Huang et al.	
6,873,865 B2	3/2005	Steuer et al.	
6,889,153 B2	5/2005	Dietiker	
6,898,451 B2	5/2005	Wuori	
6,939,307 B1	9/2005	Dunlop	
6,947,780 B2	9/2005	Scharf	
6,949,081 B1	9/2005	Chance	
6,957,094 B2	10/2005	Chance et al.	
6,961,598 B2	11/2005	Diab	
6,983,178 B2	1/2006	Fine et al.	
6,993,371 B2	1/2006	Kiani et al.	
6,996,427 B2	2/2006	Ali et al.	
7,024,235 B2	4/2006	Melker et al.	
7,027,849 B2	4/2006	Al-Ali	
7,030,749 B2	4/2006	Al-Ali	
7,035,697 B1	4/2006	Brown	
7,043,287 B1 *	5/2006	Khalil et al.	600/310
7,047,056 B2	5/2006	Hannula et al.	
7,062,306 B2	6/2006	Benaron et al.	
7,083,593 B2	8/2006	Stultz	
7,127,278 B2	10/2006	Melker et al.	
7,162,306 B2	1/2007	Caby et al.	
7,184,148 B2	2/2007	Alphonse	
7,198,502 B2	4/2007	Koenig et al.	
7,209,775 B2	4/2007	Bae et al.	
7,236,811 B2	6/2007	Schmitt	
7,242,952 B2	7/2007	Shirai et al.	
7,254,425 B2 *	8/2007	Lowery et al.	600/310
7,263,395 B2	8/2007	Chan et al.	
7,272,426 B2	9/2007	Schmid	
7,316,648 B2	1/2008	Kelly et al.	
7,327,463 B2	2/2008	Alphonse	
7,366,333 B2	4/2008	Long et al.	
7,373,193 B2	5/2008	Al-Ali et al.	
7,379,769 B2	5/2008	Piron et al.	
7,393,327 B2	7/2008	Inukai et al.	
7,400,257 B2	7/2008	Rivas	
7,447,388 B2	11/2008	Bates et al.	
7,734,321 B2 *	6/2010	White	600/310
2001/0005773 A1	6/2001	Larsen et al.	
2001/0020122 A1	9/2001	Steuer et al.	
2001/0039376 A1	11/2001	Steuer et al.	
2001/0044700 A1	11/2001	Kobayashi et al.	
2002/0026106 A1	2/2002	Khalil et al.	
2002/0035318 A1	3/2002	Mannheimer et al.	
2002/0038079 A1	3/2002	Steuer et al.	
2002/0042558 A1	4/2002	Mendelson	
2002/0049389 A1	4/2002	Abreu	
2002/0062071 A1	5/2002	Diab et al.	
2002/0111748 A1	8/2002	Kobayashi et al.	

cardiac images or tumors) to determine if the scope of the ablated tissue corresponds with the size, location and/or shape of, for example, known obstructions or tumors.

Sensors as provided may be applied to a patient's skin and/or internal organs (e.g., as part of a catheter or other inserted assembly) to monitor multiple absorption peaks of water, for example in the red or near infrared spectrum. While other potential absorbers may make up some percentage of the content of a patient's tissue, many of these absorbers, such as lipid and hemoglobin, do not change their absorption profiles significantly with temperature. For this reason, the absorption of water or other constituents whose absorption, as measured spectroscopically, changes with temperature may provide more information that relates to the tissue temperature. Accordingly, by monitoring changes in the water absorption profile that occur with rising temperatures for a single area of tissue (e.g., pre and post-ablation), a change in temperature for the tissue area may be estimated. To account for the variation in light scattering, a change may be measured against a pre-ablation spectrum. In addition, such information may be combined with a measured patient baseline temperature, either local or systemic, to determine the extent of tissue temperature changes. The near-infrared peaks of water shift and narrow with increasing temperature due to increases in hydrogen bonding between water molecules. FIG. 1 is a graph 10 of successive absorption peaks 12, 14, 16, and 18 (corresponding to peaks centered near approximately 975, 1180, 1450, and 1900, respectively). Shown are the shape and position of the absorption peaks for water at 37° C., shown by data 20, and at 60° C., shown by data 22, plotted against the depth of tissue penetration. As illustrated, the water at 60° C. is shown to have a different characteristic absorption profile.

FIG. 2 is a graph 30 of estimated photon penetration depth into tissue plotted against wavelength for light emitted into tissue and detected by a detector spaced approximately 2.5 mm from the emitter. In the depicted simulation, the tissue sample is assumed to have 70% lean water concentration, which is approximately the lean water concentration of typical tissue. As shown, over a portion of the spectrum, the penetration depth varies with wavelength. Accordingly, a particular wavelength is associated with a particular penetration depth for a particular emitter-detector spacing. By using a sensor or a combination of sensors with different emitter-detector spacings as well as different wavelengths, multiple spectroscopic temperature estimates corresponding to multiple tissue depths may be combined to estimate a thermal gradient that is predictive of the total volume of tissue that has been rendered nonviable by ablation.

Simulations of the types of shifts seen at different tissue temperatures are depicted in FIGS. 3-5, with all simulations assuming a 2.5 mm separation between emitter and detector, with both facing the same direction and embedded in tissue at or near the heating source. For each exemplary simulated tissue spectrum, multi-linear regressions were performed against experimentally determined tissue component spectra of water, protein, and lipid, plus the derivative of water absorption with respect to temperature. These regressions were performed using data over the spectral ranges of 945-1035 nm, 1127-1170 nm, and 1360-1570 nm, corresponding to regions of tissue spectrum where water is the dominant absorber and where water absorption changes significantly with temperature. Mean photon penetration depths were determined to be, respectively, 0.94 mm, 0.86 mm, and 0.52 mm for these spectral ranges, and did not differ significantly between these examples. However, in certain embodiments, depending on the nature and temperature of ablation, a significant decrease in tissue water content may occur after

ablation. A decrease in water content may allow deeper penetration for a particular wavelength. Accordingly, the mean photon penetration may increase over the course of the ablation. Such effects may be accounted for in determining the temperature gradient for a particular tissue sample. Similar temperature estimates may be obtained via other methods of comparing tissue spectra to features of tissue component spectra. For example, regressions may be performed between derivatives, or other mathematical functions, of tissue and component spectra.

Table I below shows the resulting temperatures estimated from the multi-linear regressions corresponding to each example and spectral range. As shown, the temperatures increase over the course of the ablation.

Spectral Range	Temp FIG. 1	Temp FIG. 2	Temp FIG. 3
945-1035 nm	36.83° C.	49.45° C.	58.45° C.
1127-1170 nm	37.55° C.	47.33° C.	60.43° C.
1360-1570 nm	37.52° C.	60.64° C.	82.16° C.

The example shown in FIG. 3 is a graph 40 of absorption at multiple mean photon penetration depths at a plurality of near infrared water absorption peaks. The mean photon penetration depths may be estimated by using a graph similar to FIG. 2 of mean photon distribution for a particular emitter-detector spacing. Prior to heating, tissue is simulated at 37° C., assuming a tissue composition of 66% water, 24% protein, and 10% lipid. Because this corresponds to a pre-ablation tissue temperature, the temperature at different depths is generally about 37° C., corresponding to normal body temperature, before any heating through ablation occurs.

After ablation begins, the temperature of the tissue starts to rise and the water absorption profile begins to show characteristic shifting. FIG. 4 is a graph 50 of a simulation of tissue heating during the course of ablation. At a depth of 0.5 mm, the temperature was simulated to be 60° C., changing linearly to 50° C. at a distance of 1.0 mm. This corresponds with the temperature being highest closer to the ablating source and lower the farther away from the source. The tissue is assumed to have dried out during heating to a composition of 58% water, 30% protein, and 12% lipid. As shown, the center of the water absorption peak in the 1350-1600 nm range has shifted toward the shorter wavelengths as a result of temperature change.

After the ablation is completed, the temperatures have reached their highest point in the tissue and the affected region is rendered nonviable. FIG. 5 is a graph 60 of temperatures reached shortly after the completion of an ablating course of energy. At a depth of 0.5 mm, the temperature was simulated to be 80° C., changing linearly to 60° C. at a distance of 1.0 mm. The tissue is assumed to have dried out further due to continued heating, to a composition of 40% water, 42% protein, and 17% lipid. As shown, the center of the water absorption peak in the 1350-1600 nm range has shifted toward the shorter wavelengths as a result of temperature change. A shifting and narrowing of the water absorption peak in the 1350-1600 nm range may be observed.

FIG. 6 shows a system 70 that may be used for monitoring temperature in conjunction with an ablation procedure. The system 70 includes a spectroscopic sensor 72 with a light emitter 74 and detector 76 that may be of any suitable type. The emitter 74 may be a broad spectrum emitter or may be configured to emit light of a limited wavelength range or at select discrete wavelengths. In one embodiment, the emitter

72 may include a filter wheel for tuning a broad spectrum to a series of particular wavelengths. The emitter 74 may be one or more light emitting diodes adapted to transmit one or more wavelengths of light in the red to infrared range, and the detector 76 may be a photodetector configured to receive the emitted light. In specific embodiments, the emitter 74 may be a laser diode or a vertical cavity surface emitting laser (VCSEL). The laser diode may be a tunable laser, such that a single diode may be tuned to various wavelengths corresponding to a number of absorption peaks of water. Depending on the particular arrangement of the sensor 72, the emitter 74 may be associated with an optical fiber for transmitting the emitted light into the tissue. The light may be any suitable wavelength corresponding to the wavelengths absorbed by water. For example, wavelengths between about 800 nm, corresponding with far-red visible light, and about 1800 nm, in the near infrared range, may be absorbed by water.

By way of example, FIG. 6 shows an ablation device 78 that may be associated with the system 70. However, it should be understood that ablation device 78 is merely illustrative of a medical device that may be used in conjunction with a spectroscopic sensor 72 for monitoring temperature and other devices may be incorporated into the system 70 if appropriate. In certain embodiments, the ablation device may be a microwave ablation device 78. In one embodiment, the sensor 72 is structurally associated (e.g., is disposed on) the ablation device, for example the emitter 74 and the detector 76 are disposed on a catheter, such as a cardiac catheter, or other implantable portion of the device. In embodiments in which the ablation takes place on the surface of the skin, the emitter and detector may be part of a housing or other support structure for the ablation energy source.

An associated monitor 82 may receive signals, for example from the spectroscopy sensor 72 through a sensor interface (e.g., a sensor port or a wireless interface) and, in embodiments, from the ablation device 78, to determine if the ablation has generated sufficiently high tissue temperature to destroy the viability of the tissue in the area of interest. The monitor 82 may include appropriate processing circuitry for determining temperature parameters, such as a microprocessor 92, which may be coupled to an internal bus 94. Also connected to the bus may be a RAM memory 96 and a display 98. A time processing unit (TPU) 100 may provide timing control signals to light drive circuitry 102, which controls when the emitter 74 is activated, and, if multiple light sources are used, the multiplexed timing for the different light sources. TPU 100 may also control the gating-in of signals from the sensor 72 and amplifier 103 and a switching circuit 104. These signals are sampled at the proper time, depending at least in part upon which of multiple light sources is activated, if multiple light sources are used. The received signal from the sensor 72 may be passed through an amplifier 106, a low pass filter 108, and an analog-to-digital converter 110. The digital data may then be stored in a queued serial module (QSM) 112, for later downloading to RAM 96 as QSM 112 fills up.

In an embodiment, based at least in part upon the received signals corresponding to the water absorption peaks received by detector 76 of the sensor 72, microprocessor 92 may calculate the microcirculation parameters using various algorithms. In addition, the microprocessor 92 may calculate tissue temperature. These algorithms may employ certain coefficients, which may be empirically determined, and may correspond to the wavelength of light used. In addition, the algorithms may employ additional correction coefficients. The algorithms and coefficients may be stored in a ROM 116 or other suitable computer-readable storage medium and

accessed and operated according to microprocessor 92 instructions. In one embodiment, the correction coefficients may be provided as a lookup table. In addition, the sensor 72 may include certain data storage elements, such as an encoder 120, that may encode information related to the characteristics of the sensor 72, including information about the emitter 74 and the detector 76. The information may be accessed by detector/decoder 122, located on the monitor 82. Control inputs 124 may allow an operator to input patient and/or sensor characteristics.

As noted, the sensor 72 may be incorporated into the ablation device 78 or, may, in other embodiments, be a separate device. FIGS. 7-8 show examples of configurations for the sensor 72. In FIG. 7, the emitter 74 is spaced apart from the detector 76 a particular distance that may be stored into the encoder 110, so that the monitor may perform the analysis of the mean photon penetration associated with a particular emitter-detector spacing. The emitter 74 may be capable of emitting light of multiple wavelengths. Depending on the wavelength, the mean photon penetration depth may be shallower, as shown for path 130, or may be deeper, as shown for path 132. By collecting data from different depths, a temperature gradient through the tissue may be determined.

In addition to using different wavelengths to acquire data at different depths, a sensor 72 may also incorporate additional detectors 76 with varied spacing around the emitter 74. As shown in FIG. 8, a sensor 72 may incorporate detectors spaced apart different distances (shown as distances d_1 , d_2 , d_3 , and d_4) from an emitter 74. If the distances correspond with characteristic water absorption profiles and mean photon penetration depths, then any change that occurs during an ablation may be correlated to a empirically or mathematically-derived tissue temperature.

FIG. 9 is a process flow diagram illustrating a method 134 for determining tissue temperature during an ablation procedure in accordance with some embodiments. The method may be performed as an automated procedure by a system, such as system 70. In addition, certain steps of the method may be performed by a processor, or a processor-based device such as a patient monitor 82 that includes instructions for implementing certain steps of the method 134. According to an embodiment, the method 134 begins with obtaining a baseline, pre-ablation signal representative of one or more water absorption peaks from detector 76 associated with the sensor 72 (block 136). The pre-ablation signal may be associated with normal body temperatures. The ablation device 78 may be activated and the sensor 72 may collect data during the ablation (block 138). The sensor 72 may also collect post-ablation data (block 140). The monitor 82 may perform analysis of the signals from the sensor 72 and calculation of the tissue temperature (block 142) based on the signal obtained.

For example, in one embodiment, the tissue temperature may be determined by examining changes in the water absorption peaks over the course of the ablation. If the change in the temperature is indicative of ablation (i.e., nonviability of the tissue), a monitor 82 may determine that a successful ablation has occurred. For example, tissue temperatures in excess of 43° C., 50° C., 60° C., or 80° C. may be indicative of ablation. In addition, such monitoring may include any appropriate visual indication, such as a display of a temperature or temperature versus depth, displayed on the monitor 82 or any appropriate audio indication. For example, an increase of tissue temperature above a predetermined viability threshold or outside of a predetermined range may trigger an alarm or may trigger an indication of ablation. Further, additional

indications may include text or other alerts to inform that the ablation was likely successful.

While the invention may be susceptible to various modifications and alternative forms, specific embodiments have been shown by way of example in the drawings and will be described in detail herein. However, it should be understood that the invention is not intended to be limited to the particular forms disclosed. Rather, the invention is to cover all modifications, equivalents and alternatives falling within the spirit and scope of the invention as defined by the following appended claims.

What is claimed is:

1. A monitor, comprising:
a sensor interface;
a display; and
data processing circuitry configured to:
cause operation of a spectrophotometric sensor via the sensor interface, wherein the sensor comprises at least one emitter configured to emit light into a tissue of a patient and at least one detector configured to detect the light;
receive spectrophotometric data associated with a mean photon penetration depth in the tissue from the at least one detector via the sensor interface;
determine one or more temperatures of the tissue associated with the mean photon penetration depth from the spectrophotometric data; and
cause the display to display an indication related to the one or more tissue temperatures.
2. The monitor of claim 1, wherein determining the one or more tissue temperatures comprises determining a change in a magnitude of a water absorption peak.
3. The monitor of claim 2, wherein determining the one or more tissue temperatures comprises correlating the change in the magnitude of the water absorption peak to a tissue temperature associated with the change in the magnitude of the water absorption peak.
4. The monitor of claim 1, wherein the data processing circuitry is configured to activate an energy source configured to direct ablating energy into the patient's tissue.

5. The monitor of claim 4, wherein the data processing circuitry comprises instructions for determining whether the tissue temperature is associated with heat from the ablating energy.

6. The monitor of claim 4, wherein the tissue temperature associated with heat from the ablating energy is greater than about 43° C.

7. The monitor of claim 1, wherein the determining the one or more tissue temperatures comprises determining a temperature gradient in the tissue from a plurality of mean photon penetration depths.

8. The monitor of claim 2, wherein determining the one or more tissue temperatures comprises determining a change in a shape of the water absorption peak.

9. The monitor of claim 1, wherein causing operation of a spectrophotometric sensor via the sensor interface comprises driving the emitter to emit light in a range from about 945 nm to about 1035 nm.

10. The monitor of claim 1, comprising receiving information related to a tissue ablation; and
assessing the tissue ablation based on the tissue temperature.

11. The monitor of claim 10, wherein assessing the tissue ablation comprises determining a viability of the tissue.

12. The monitor of claim 10, wherein assessing the tissue ablation comprises determining a volume of ablated tissue.

13. The monitor of claim 5, wherein determining whether the tissue temperature is associated with heat from the ablating energy comprises comparing the tissue temperature to a baseline temperature.

14. The monitor of claim 13, wherein the baseline temperature comprises a local or systemic temperature of the patient.

15. The monitor of claim 13, wherein the baseline temperature comprises a temperature calculated based at least in part upon spectrophotometric data generated before ablating energy is directed into the patient's tissue.

16. The monitor of claim 1, wherein determining the one or more temperatures comprises using an estimation of lean water concentration in the tissue.

* * * * *

2002/0133068	A1	9/2002	Huiku	
2002/0156354	A1	10/2002	Larson	
2002/0161287	A1	10/2002	Schmitt	
2002/0161290	A1	10/2002	Chance	
2002/0165439	A1	11/2002	Schmitt	
2002/0183727	A1 *	12/2002	Daikuzono	606/10
2002/0198443	A1	12/2002	Ting	
2003/0023140	A1	1/2003	Chance	
2003/0055324	A1	3/2003	Wasserman	
2003/0060693	A1	3/2003	Monfre et al.	
2003/0084907	A1 *	5/2003	Pacek et al.	128/898
2003/0139687	A1	7/2003	Abreu	
2003/0144584	A1	7/2003	Mendelson	
2003/0203357	A1 *	10/2003	Huang	435/5
2003/0220548	A1	11/2003	Schmitt	
2003/0220576	A1	11/2003	Diab	
2004/0010188	A1	1/2004	Wasserman	
2004/0054270	A1	3/2004	Pewzner et al.	
2004/0087846	A1	5/2004	Wasserman	
2004/0087916	A1	5/2004	Pickup et al.	
2004/0107065	A1	6/2004	Al-Ali	
2004/0127779	A1	7/2004	Steuer et al.	
2004/0171920	A1	9/2004	Mannheimer et al.	
2004/0176670	A1	9/2004	Takamura et al.	
2004/0176671	A1	9/2004	Fine et al.	
2004/0181196	A1	9/2004	Pickup et al.	
2004/0230106	A1	11/2004	Schmitt et al.	
2005/0054907	A1	3/2005	Page et al.	
2005/0080323	A1	4/2005	Kato	
2005/0101850	A1	5/2005	Parker	
2005/01113651	A1	5/2005	Wood et al.	
2005/01113656	A1	5/2005	Chance	
2005/0154285	A1	7/2005	Neason	
2005/0154286	A1	7/2005	Neason	
2005/0165316	A1 *	7/2005	Lowery et al.	600/480
2005/0165323	A1	7/2005	Montgomery et al.	
2005/0168722	A1	8/2005	Forstner et al.	
2005/0177034	A1	8/2005	Beaumont	
2005/0192488	A1	9/2005	Bryenton et al.	
2005/0201345	A1	9/2005	Williamson	
2005/0203357	A1	9/2005	Debreczeny et al.	
2005/0228248	A1	10/2005	Dietiker	
2005/0267346	A1	12/2005	Faber et al.	
2005/0283059	A1	12/2005	Iyer et al.	
2006/0004270	A1 *	1/2006	Bedard et al.	600/316
2006/0009688	A1	1/2006	Lamego et al.	
2006/0015021	A1	1/2006	Cheng	
2006/0020181	A1	1/2006	Schmitt	
2006/0020309	A1 *	1/2006	Altshuler et al.	607/88
2006/0030763	A1	2/2006	Mannheimer et al.	
2006/0052680	A1	3/2006	Diab	
2006/0058683	A1	3/2006	Chance	
2006/0064024	A1	3/2006	Schnall	
2006/0111622	A1 *	5/2006	Merritt et al.	600/315
2006/0122475	A1	6/2006	Balberg et al.	
2006/0129204	A1	6/2006	Pless	
2006/0142808	A1	6/2006	Pearce et al.	
2006/0167367	A1	7/2006	Stanczak et al.	
2006/0178588	A1	8/2006	Brody	
2006/0195028	A1	8/2006	Hannula et al.	
2006/0206018	A1 *	9/2006	Abul-Haj et al.	600/316
2006/0217602	A1 *	9/2006	Abul-Haj et al.	600/316
2006/0224058	A1	10/2006	Mannheimer	
2006/0229515	A1 *	10/2006	Sharareh et al.	600/476
2006/0247501	A1	11/2006	Ali	
2006/0247506	A1	11/2006	Balberg et al.	
2006/0258921	A1	11/2006	Addison et al.	
2006/0265022	A1	11/2006	John et al.	
2006/0272418	A1	12/2006	Maris et al.	
2006/0272419	A1	12/2006	Maris et al.	
2007/0118045	A1	5/2007	Naghavi et al.	
2008/0060138	A1	3/2008	Price et al.	
2008/0096495	A1	4/2008	Shen	
2008/0208912	A1	8/2008	Garibaldi	
2008/0214903	A1	9/2008	Orbach	
2008/0221409	A1 *	9/2008	Hoarau	600/310
2008/0312533	A1	12/2008	Balberg et al.	
2010/0049180	A1 *	2/2010	Wells et al.	606/12
2011/0108730	A1 *	5/2011	Herrmann	250/339.04

FOREIGN PATENT DOCUMENTS

EP	1491135	12/2004
EP	1986543	11/2008
JP	63275325	11/1988
JP	3170866	7/1991
JP	3238813	10/1991
JP	4332536	11/1992
JP	7124138	5/1995
JP	7136150	5/1995
JP	2004008572	1/2004
JP	2004113353	4/2004
JP	2004194908	7/2004
JP	2004248819	9/2004
JP	2004290545	10/2004
JP	2005034472	2/2005
WO	WO9101678	2/1991
WO	WO9309711	5/1993
WO	WO9639927	12/1996
WO	WO9843071	10/1998
WO	WO9932030	7/1999
WO	WO0021438	4/2000
WO	WO0140776	6/2001
WO	WO0176461	10/2001
WO	WO0176471	10/2001
WO	WO03039326	5/2003
WO	WO2005025399	3/2005
WO	WO2006097910	9/2006

OTHER PUBLICATIONS

Nijland, Roel, et al.; "Validation of Reflectance Pulse Oximetry: An Evaluation of a new Sensor in Piglets," *Journal of Clinical Monitoring*, vol. 13, pp. 43-49 (1997).

Nogawa, Masamichi, et al.; "A New Hybrid Reflectance Optical Pulse Oximetry Sensor for Lower Oxygen Saturation Measurement and for Broader Clinical Application," *SPIE*, vol. 2976, pp. 78-87 (1997).

Mannheimer, Paul D., et al.; "Wavelength Selection for Low-Saturation Pulse Oximetry," *IEEE Transactions on Biomedical Engineering*, vol. 44, No. 3, pp. 148-158 (Mar. 1997).

Pickett, John, et al.; "Pulse Oximetry and PPG Measurements in Plastic Surgery," *Proceedings—19th International Conference—IEEE/EMBS*, Chicago, Illinois, Oct. 30-Nov. 2, 1997, pp. 2330-2332.

Leahy, Martin J., et al.; "Sensor Validation in Biomedical Applications," *IFAC Modelling and Control in Biomedical Systems*, Warwick, UK, pp. 221-226 (1997).

Barreto, Armando B., et al.; "Adaptive LMS Delay Measurement in dual Blood Volume Pulse Signals for Non-Invasive Monitoring," *IEEE*, pp. 117-120 (1997).

East, Christine E., et al.; "Fetal Oxygen Saturation and Uterine Contractions During Labor," *American Journal of Perinatology*, vol. 15, No. 6, pp. 345-349 (Jun. 1998).

Edrich, Thomas, et al.; "Can the Blood Content of the Tissues be Determined Optically During Pulse Oximetry Without Knowledge of the Oxygen Saturation?—An In-Vitro Investigation," *Proceedings of the 20th Annual International conference of the IEEE Engineering in Medicine and Biology Society*, vol. 20, No. 6, 1998.

Such, Hans Olaf; "Optoelectronic Non-invasive Vascular Diagnostics Using multiple Wavelength and Imaging Approach," *Dissertation*, (1998).

Lutter, N., et al.; "Comparison of Different Evaluation Methods for a Multi-wavelength Pulse Oximeter," *Biomedizinische Technik*, vol. 43, (1998).

Todd, Bryan, et al.; "The Identification of Peaks in Physiological Signals," *Computers and Biomedical Research*, vol. 32, pp. 322-335 (1999).

Seelbach-Göbel, Birgit, et al.; "The prediction of fetal acidosis by means of intrapartum fetal pulse oximetry," *Am J. Obstet. Gynecol.*, vol. 180, No. 1, Part 1, pp. 73-81 (1999).

Goldman, Julian M.; "Masimo Signal Extraction Pulse Oximetry," *Journal of Clinical Monitoring and Computing*, vol. 16, pp. 475-483 (2000).

Coetzee, Frans M.; "Noise-Resistant Pulse Oximetry Using a Synthetic Reference Signal," *IEEE Transactions on Biomedical Engineering*, vol. 47, No. 8, Aug. 2000, pp. 1018-1026.

- Nilsson, Lena, et al.; "Monitoring of Respiratory Rate in Postoperative Care Using a New Photoplethysmographic Technique," *Journal of Clinical Monitoring and Computing*, vol. 16, pp. 309-315 (2000).
- Kaestle, S.; "Determining Artefact Sensitivity of New Pulse Oximeters in Laboratory Using Signals Obtained from Patient," *Biomedizinische Technik*, vol. 45 (2000).
- Cysewska-Sobusaik, Anna; "Metrological Problems With noninvasive Transillumination of Living Tissues," *Proceedings of SPIE*, vol. 4515, pp. 15-24 (2001).
- Belal, Suliman Yousef, et al.; "A fuzzy system for detecting distorted plethysmogram pulses in neonates and paediatric patients," *Physiol. Meas.*, vol. 22, pp. 397-412 (2001).
- Malettras, Francois-Xavier, et al.; "Construction and calibration of a new design of Fiber Optic Respiratory Plethysmograph (FORP)," *Optomechanical Design and Engineering, Proceedings of SPIE*, vol. 4444, pp. 285-293 (2001).
- Earthrowl-Gould, T., et al.; "Chest and abdominal surface motion measurement for continuous monitoring of respiratory function," *Proc. Instn Mech Engrs*, V215, Part H; pp. 515-520 (2001).
- Relente, A.R., et al.; "Characterization and Adaptive Filtering of Motion Artifacts in Pulse Oximetry using Accelerometers," *Proceedings of the Second joint EMBS/BMES Conference*, Houston, Texas, Oct. 23-26, 2002; pp. 1769-1770.
- Chan, K.W., et al.; "17.3: Adaptive Reduction of Motion Artifact from Photoplethysmographic Recordings using a Variable Step-Size LMS Filter," *IEEE*, pp. 1343-1346 (2002).
- Yoon, Gilwon, et al.; "Multiple diagnosis based on Photoplethysmography: hematocrit, SpO₂, pulse and respiration," *Optics in Health Care and Biomedical optics: Diagnostics and Treatment; Proceedings of the SPIE*, vol. 4916; pp. 185-188 (2002).
- Lopez-Silva, Sonia Maria Lopez, et al.; "Near-infrared transmittance pulse oximetry with laser diodes," *Journal of Biomedical Optics*, vol. 8, No. 3, pp. 525-533 (Jul. 2003).
- Cyrill, D., et al.; "Adaptive Comb Filter for Quasi-Periodic Physiologic Signals," *Proceedings of the 25th Annual International Conference of the IEEE EMBS*, Cancun, Mexico, Sep. 17-21, 2003; pp. 2439-2442.
- Stetson, Paul F.; "Determining Heart Rate from Noisy Pulse Oximeter Signals Using Fuzzy Logic," *The IEEE International Conference on Fuzzy Systems*, St. Louis, Missouri, May 25-28, 2003; pp. 1053-1058.
- Lee, C.M., et al.; "Reduction of motion artifacts from photoplethysmographic recordings using wavelet denoising approach," *IEEE EMBS Asian-Pacific Conference on Biomedical Engineering*, Oct. 20-22, 2003; pp. 194-195.
- Johansson, A.; "Neural network for photoplethysmographic respiratory rate monitoring," *Medical & Biological Engineering & Computing*, vol. 41, pp. 242-248 (2003).
- Addison, Paul S., et al.; "A novel time-frequency-based 3D Lissajous figure method and its application to the determination of oxygen saturation from the photoplethysmogram," *Institute of Physics Publishing, Meas. Sci. Technol.*, vol. 15, pp. L15-L18 (2004).
- Crespi, F., et al.; "Near infrared oximeter prototype for non-invasive analysis of rat brain oxygenation," *Optical Sensing, Proceedings of SPIE*, vol. 5459, pp. 38-45 (2004).
- Johnston, W.S., et al.; "Extracting Breathing Rate Information from a Wearable Reflectance Pulse Oximeter Sensor," *Proceedings of the 26th Annual International conference of the IEEE EMBS*, San Francisco, California; Sep. 1-5, 2004; pp. 5388-5391.
- Spigulis, Janis, et al.; "Optical multi-channel sensing of skin blood pulsations," *Optical Sensing, Proceedings of SPIE*, vol. 5459, pp. 46-53 (2004).

* cited by examiner

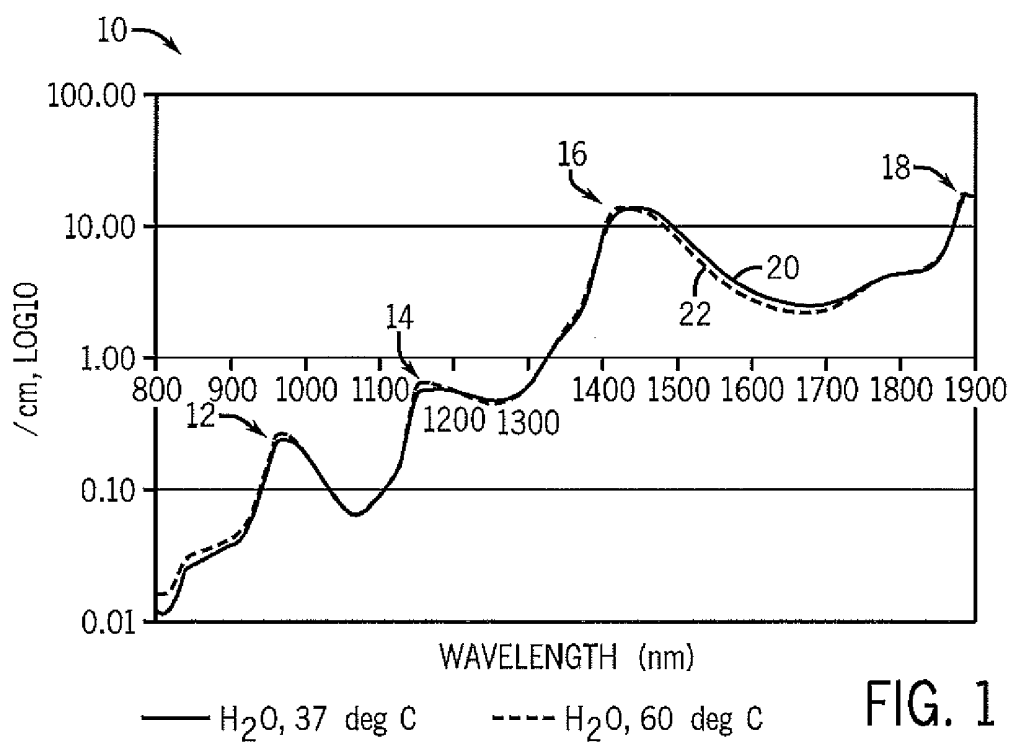


FIG. 1

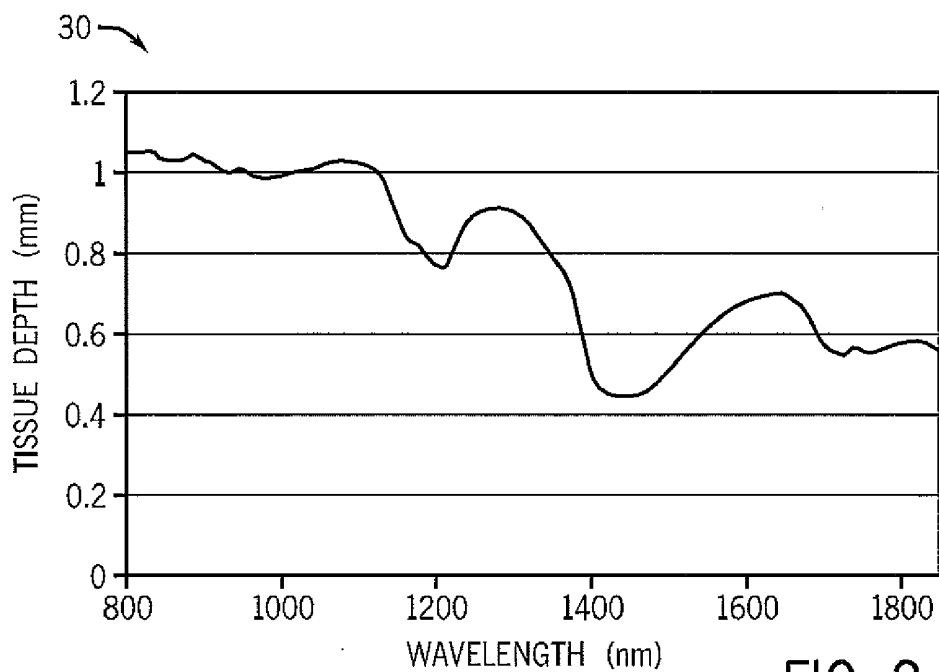


FIG. 2

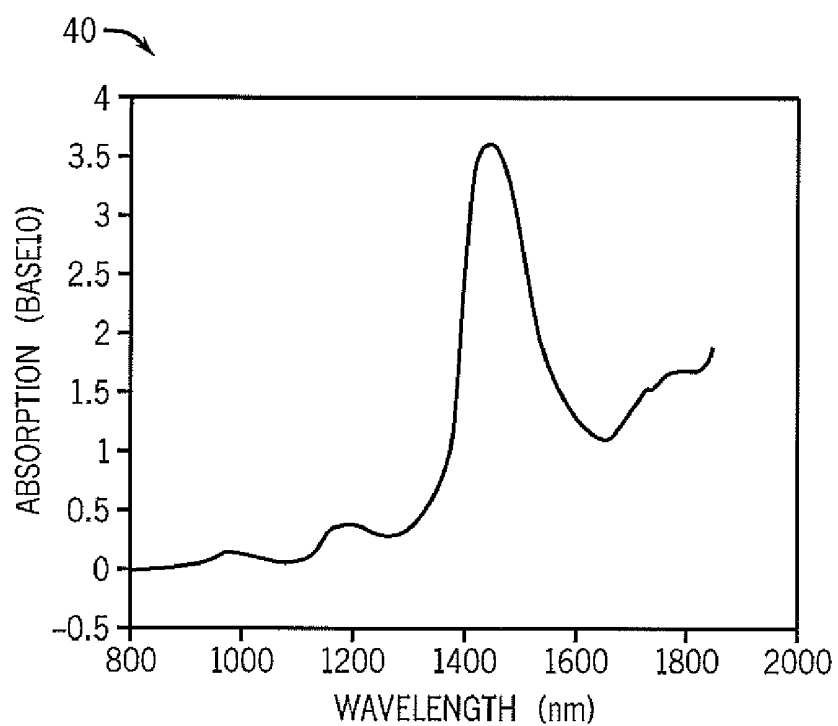


FIG. 3

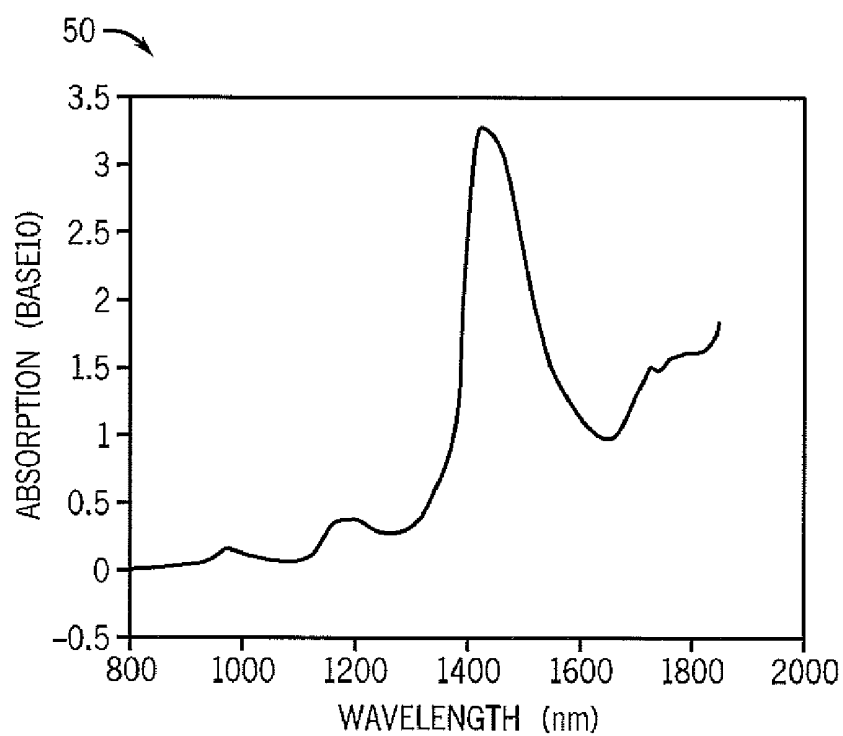


FIG. 4

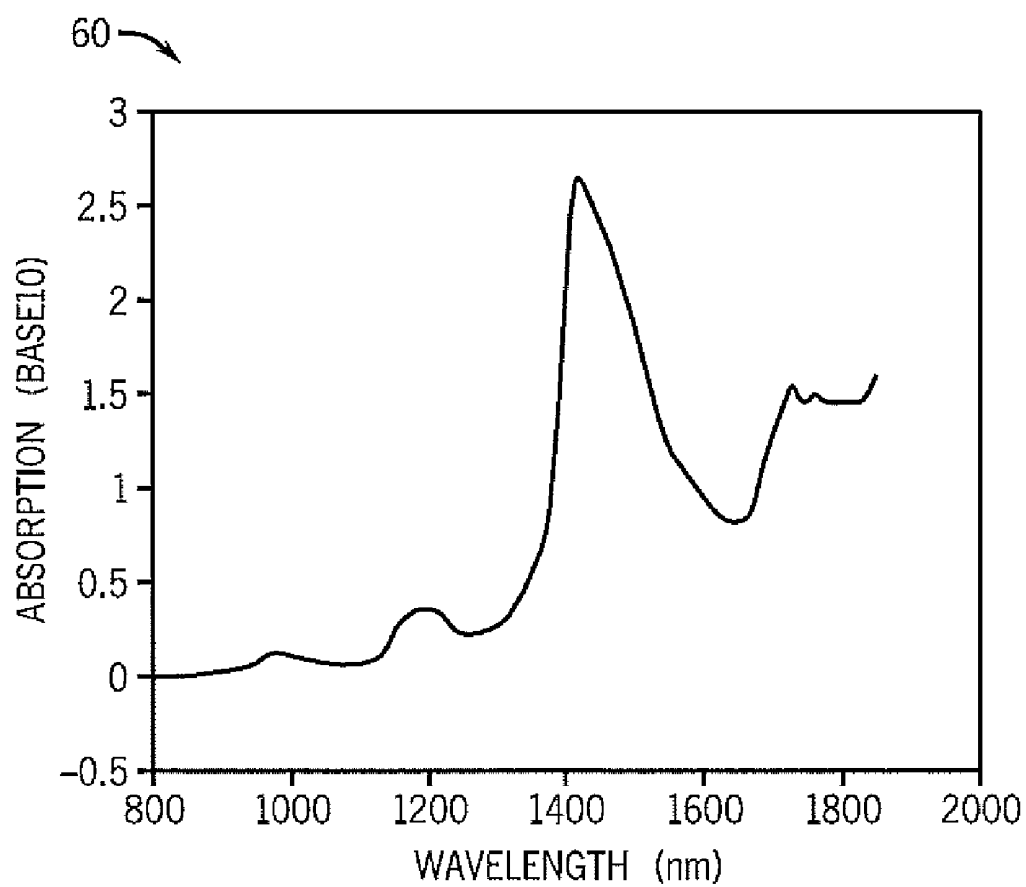


FIG. 5




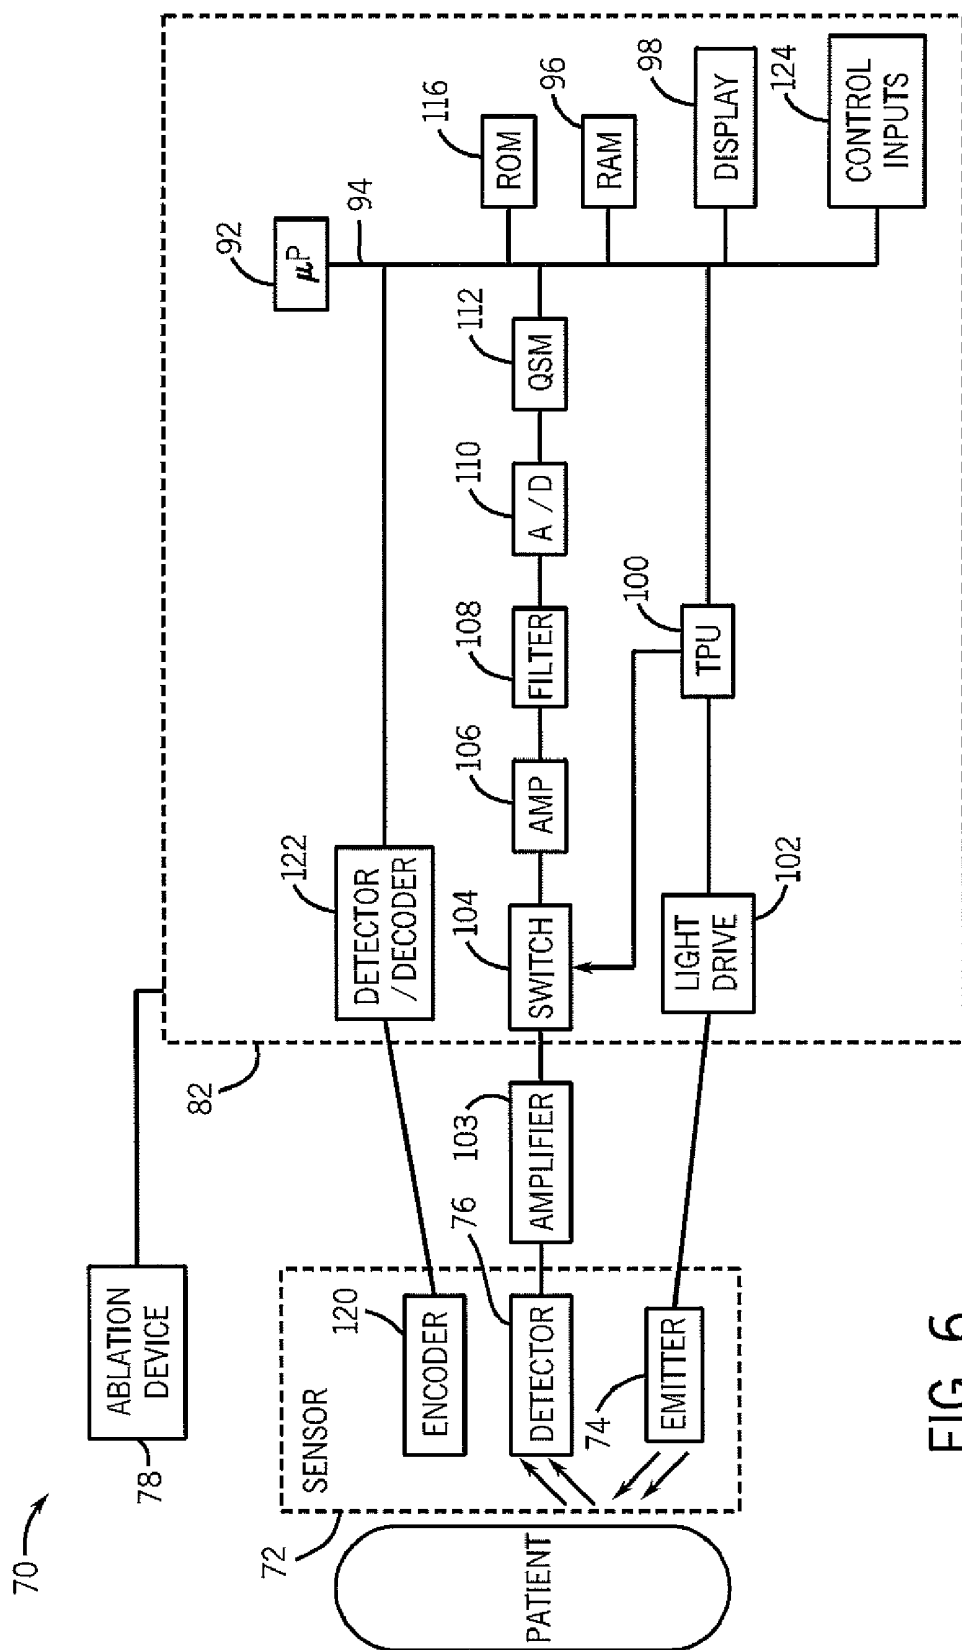


FIG. 6

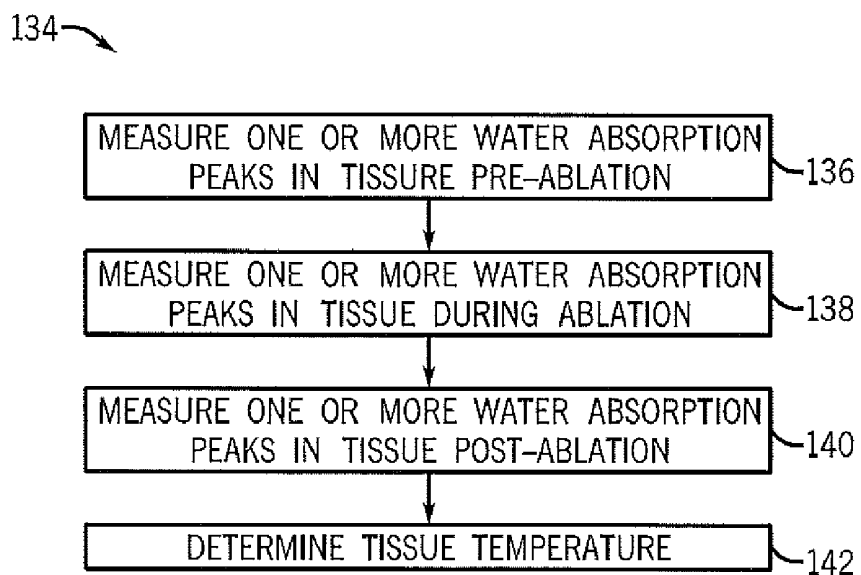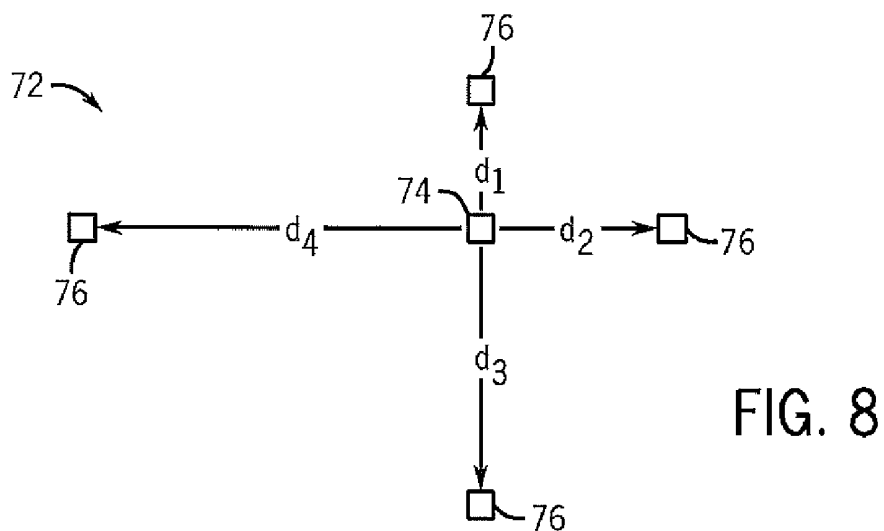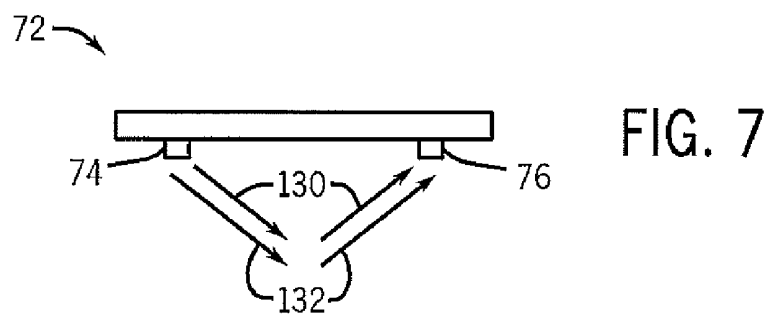

SPECTROSCOPIC METHOD AND SYSTEM FOR ASSESSING TISSUE TEMPERATURE

BACKGROUND

The present disclosure relates generally to medical devices and, more particularly, to the use of spectroscopy to monitor changes in the temperature of water-bearing tissue.

This section is intended to introduce the reader to aspects of the art that may be related to various aspects of the present disclosure, which are described and/or claimed below. This discussion is believed to be helpful in providing the reader with background information to facilitate a better understanding of the various aspects of the present disclosure. Accordingly, it should be understood that these statements are to be read in this light, and not as admissions of prior art.

Some forms of patient treatment involve removing unwanted portions of tissue from the patient, for example by surgical resection. However, for tissue areas that may be difficult to access surgically or for very small areas of tissue, tissue ablation may be more appropriate. Tissue ablation uses energy directed at the tissue site of interest to heat the tissue to temperatures that destroy the viability of the individual components of the tissue cells. During tissue ablation, an unwanted portion of a tissue, e.g., fibrous tissue, lesions, or obstructions, may be destroyed. Ablation can be achieved by various techniques, including the application of radio frequency energy, microwave energy, lasers, and ultrasound. Generally, ablation procedures involve ablating tissue that is surrounded by otherwise healthy tissue that a clinician wishes to preserve. Accordingly, better therapeutic outcomes may be achieved through precise application of the ablating energy to the tissue.

The precision of the ablation may depend in part on the type of energy applied, the skill of the clinician, and the accessibility of the tissue in question. For example, ablation may be complex if the target area is moving. During catheter ablation to correct an abnormal heartbeat, the cardiac tissue in question is typically in motion, which may affect the volume of tissue ablated. Because the ablation may take place internally, as in the case of cardiac ablation, assessment of the volume of the tissue necrosis may be difficult. In addition, depending on the type of ablating energy used, controlling the area of the ablation may be easier than controlling the depth of the ablation. Accordingly, the depth of the necrosis may vary from patient to patient.

BRIEF DESCRIPTION OF THE DRAWINGS

Advantages of the disclosure may become apparent upon reading the following detailed description and upon reference to the drawings in which:

FIG. 1 is a graph of the absorption spectra for water for two different temperature points;

FIG. 2 is a graph of estimated mean photon penetration depth plotted against wavelength for a sample of 70% lean water concentration and an emitter-detector spacing of 2.5 mm;

FIG. 3 is a graph of a simulated absorption spectrum of water for an example tissue sample at 37° C. and an emitter-detector spacing of 2.5 mm;

FIG. 4 is a graph of a simulated absorption spectrum of water for an example tissue sample at 50-60° C. and an emitter-detector spacing of 2.5 mm;

FIG. 5 is a graph of a simulated absorption spectrum of water for an example tissue sample at 60-80° C. and an emitter-detector spacing of 2.5 mm;

FIG. 6 is a block diagram of a system for monitoring tissue temperature according to an embodiment;

FIG. 7 is a side view of an example of a spectroscopic sensor for acquiring information from the tissue according to an embodiment;

FIG. 8 is a top view of an example of a spectroscopic sensor with multiple detectors spaced apart from an emitter for acquiring information from the tissue according to an embodiment; and

FIG. 9 is a block diagram of a method of monitoring tissue temperature during ablation.

DETAILED DESCRIPTION

One or more specific embodiments of the present disclosure will be described below. In an effort to provide a concise description of these embodiments, not all features of an actual implementation are described in the specification. It should be appreciated that in the development of any such actual implementation, as in any engineering or design project, numerous implementation-specific decisions must be made to achieve the developers' specific goals, such as compliance with system-related and business-related constraints, which may vary from one implementation to another. Moreover, it should be appreciated that such a development effort might be complex and time consuming, but would nevertheless be a routine undertaking of design, fabrication, and manufacture for those of ordinary skill having the benefit of this disclosure.

Provided herein are systems, sensors, and methods for spectroscopic monitoring of tissue temperature. When such systems are used in conjunction with a tissue ablation device, a medical monitor may assess changes in spectrophotometric parameters to determine the viability of a probed area of the tissue. Tissue areas with water absorption profiles characteristic of particular temperatures may be determined. Such systems may also be used to determine the viability of the probed tissue, i.e., probed tissues associated with temperatures above a certain threshold may be considered nonviable. As a result, the efficacy of the ablation may be determined. In other embodiments, the spectroscopic sensors as provided may be used in conjunction with other types of medical procedures that involve changing or monitoring tissue temperature, such as hypothermic or hyperthermic treatments.

Monitoring the necrosis of ablated tissue may be complex, particularly when using techniques that involve ablation of internal tissue. As provided herein, spectroscopic sensing may be used to noninvasively monitor tissue temperature at a number of tissue depths. The temperature information may then be used to determine the scope of the tissue ablation. Generally, ablated tissue cells will have characteristically higher temperatures as a result of the heat of ablation. During ablation, the tissue is heated until the resultant higher temperature of the tissue causes protein denaturation and other effects that lead to necrosis of the tissue. The temperature changes may be monitored by spectroscopically assessing changes in the shape, position and/or magnitude of one or more water absorption peaks of the tissue. Because wavelengths may be chosen that penetrate known depths of the patient's tissue, temperature information may be collected for relatively fine gradations of tissue depth that are otherwise difficult to obtain. Such noninvasive monitoring may provide information about the depth and/or volume of the tissue ablation and may allow clinicians to more precisely determine whether further ablating treatment may be needed. In addition, clinicians may be able to determine the borders of any ablated tissue in relation to the healthy tissue and may be able to match the borders with previously acquired data (e.g.,

专利名称(译)	用于评估组织温度的光谱方法和系统		
公开(公告)号	US8376955	公开(公告)日	2013-02-19
申请号	US12/569721	申请日	2009-09-29
[标]申请(专利权)人(译)	内尔科尔普里坦贝内特公司		
申请(专利权)人(译)	NELLCOR PURITAN BENNETT LLC		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	BAKER JR CLARK R		
发明人	BAKER, JR., CLARK R.		
IPC分类号	A61B5/01 A61B5/00		
CPC分类号	A61B5/01 A61B18/1815 A61B2017/00057 A61B2017/00084		
其他公开文献	US20110077547A1		
外部链接	Espacenet USPTO		

摘要(译)

根据各种实施例，用于确定组织温度的医疗系统和方法可包括光谱传感器。光谱传感器可以配置成提供关于一个或多个吸收峰处的吸水曲线变化的信息。这种传感器可以结合到用于组织消融的消融系统中。温度信息可用于确定消融的范围，体积和/或深度。

