



US 20050154321A1

(19) **United States**

(12) **Patent Application Publication**  
**Wolinsky et al.**

(10) **Pub. No.: US 2005/0154321 A1**

(43) **Pub. Date: Jul. 14, 2005**

(54) **DEVICES FOR FIXING A SENSOR IN A LUMEN**

**Related U.S. Application Data**

(75) Inventors: **Lone Wolinsky**, Ramat Gan (IL); **Alon Ben-Yoseph**, Amek Yisrael (IL); **Abraham Penner**, Tel Aviv (IL)

(60) Provisional application No. 60/536,580, filed on Jan. 13, 2004.

Correspondence Address:  
**Bingham McCutchen, LLP**  
**Suite 1800**  
**Three Embarcadero**  
**San Francisco, CA 94111-4067 (US)**

**Publication Classification**

(51) **Int. Cl.<sup>7</sup>** ..... **A61B 5/02**  
(52) **U.S. Cl.** ..... **600/486; 600/483**


(73) Assignee: **Remon Medical Technologies Ltd**

(57) **ABSTRACT**

(21) Appl. No.: **11/034,502**

Apparatus for positioning at least one sensor in a body lumen, the apparatus including a fixation element, a sensor, and a connecting element that connects the sensor to the fixation element, the connecting element extending at least partially into the lumen so that the sensor is located radially inward from a wall of the lumen.

(22) Filed: **Jan. 12, 2005**

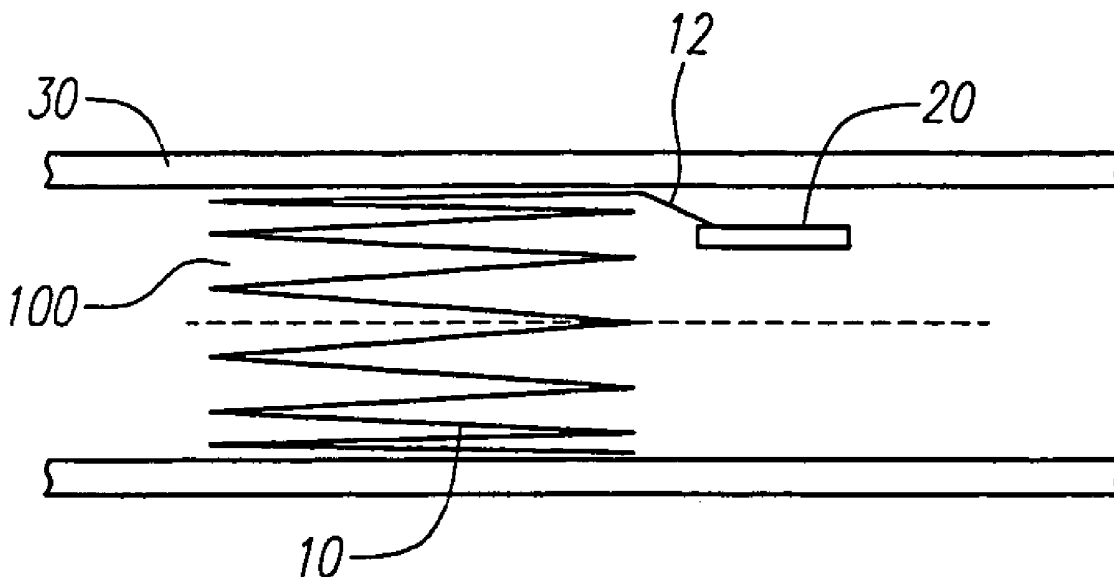

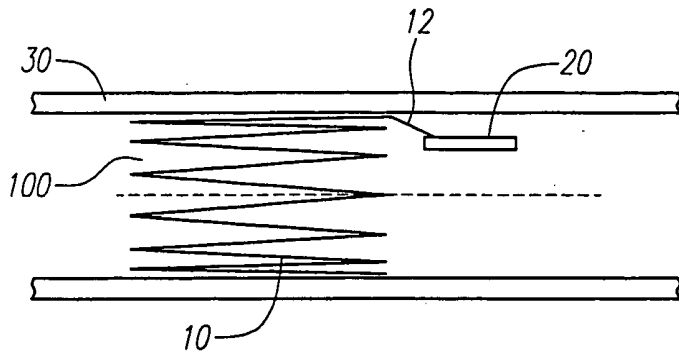


FIG. 1A

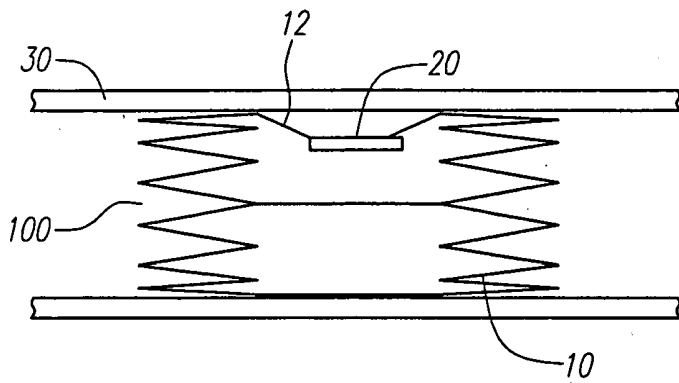


FIG. 1B

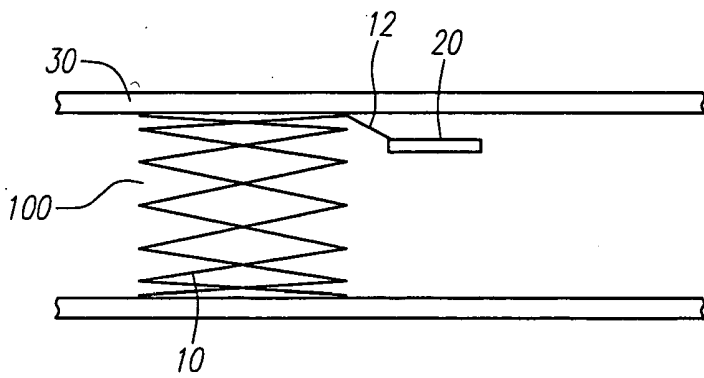


FIG. 1C

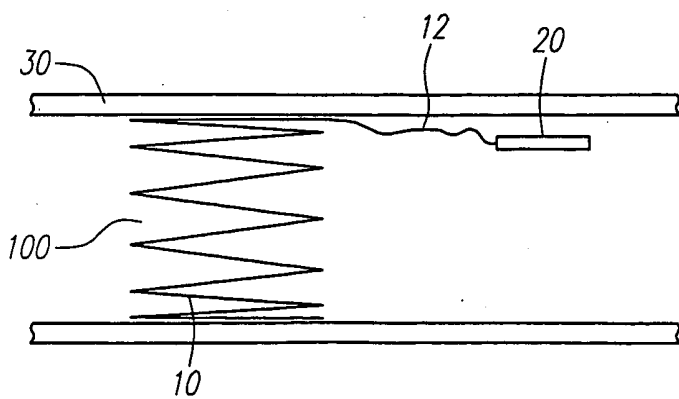


FIG. 1D

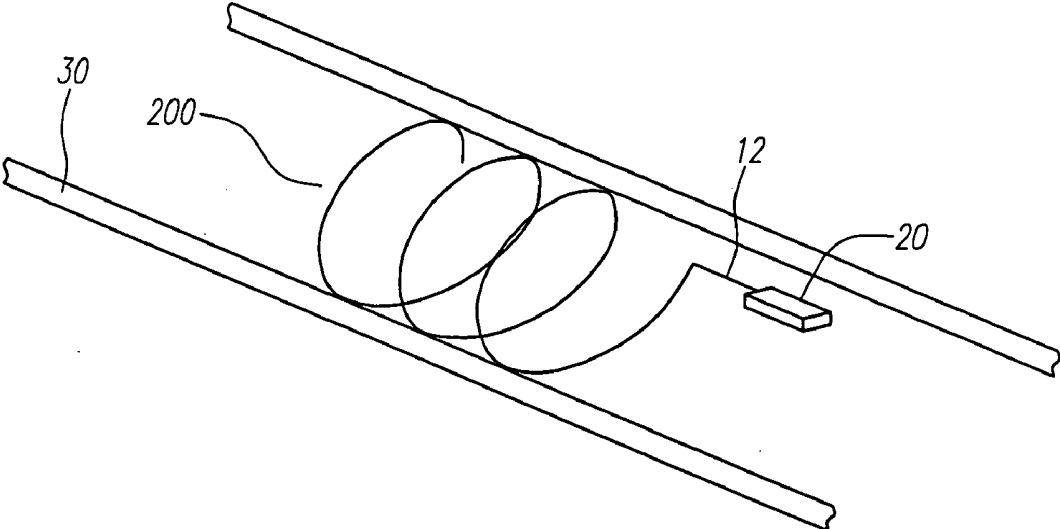


FIG. 2A

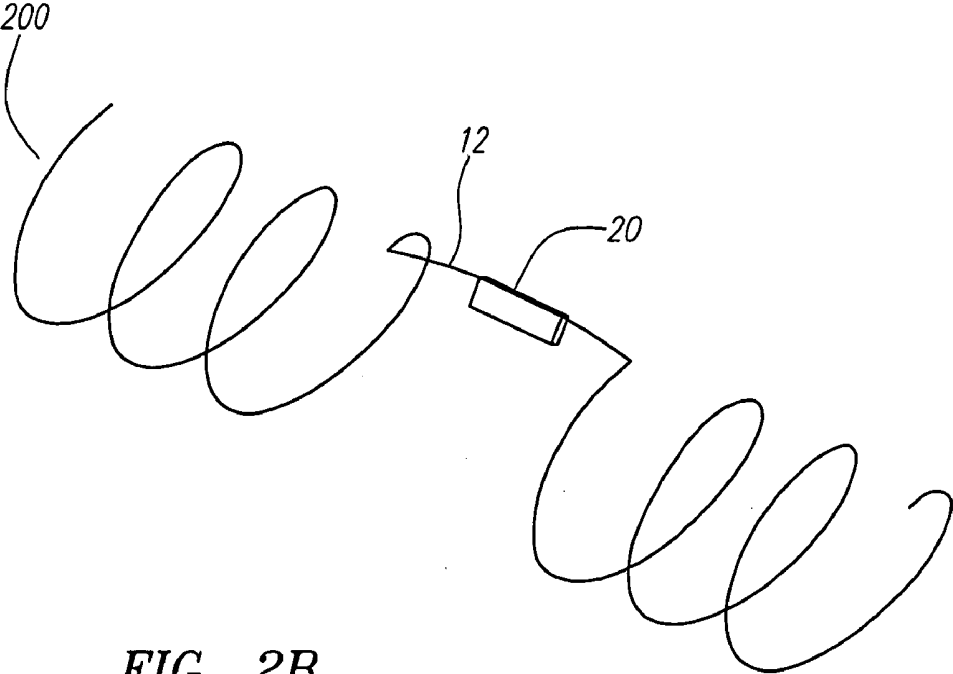


FIG. 2B

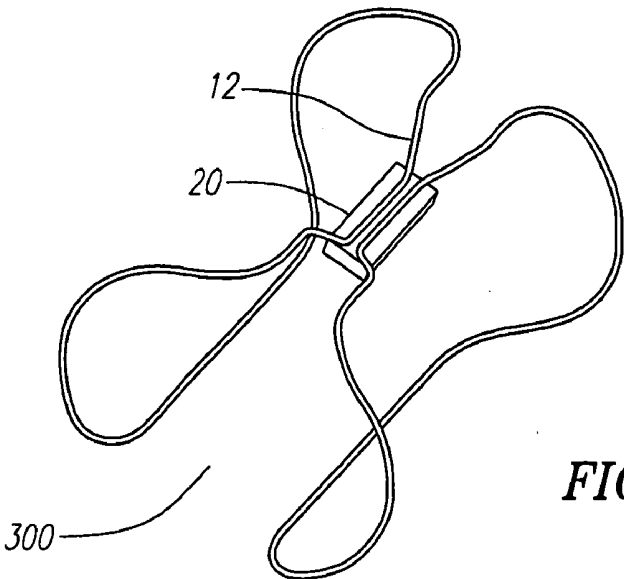


FIG. 3A

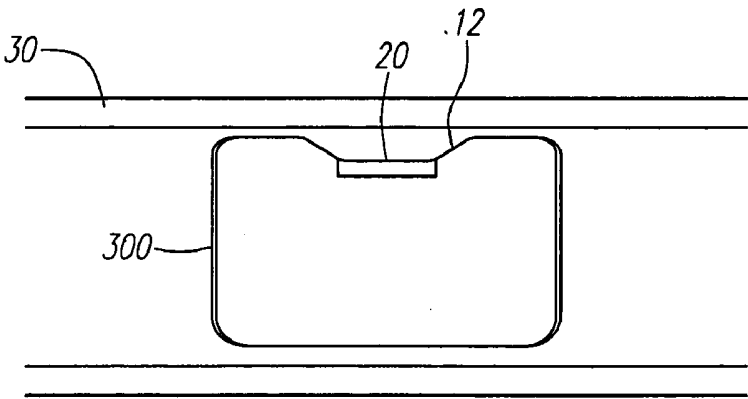


FIG. 3B

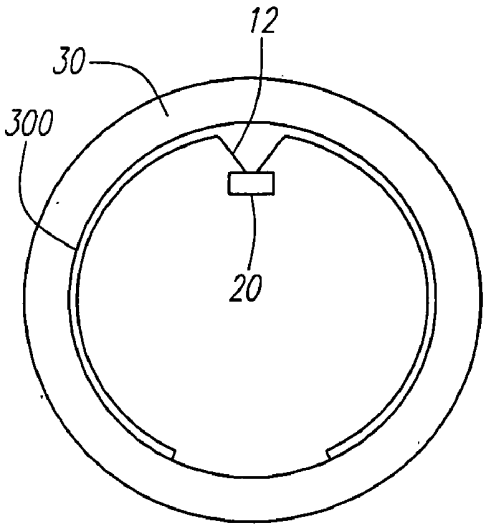


FIG. 3C

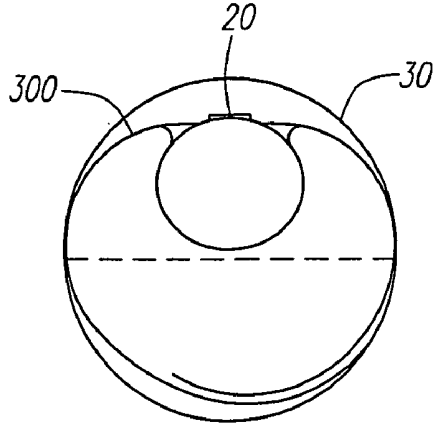


FIG. 3D

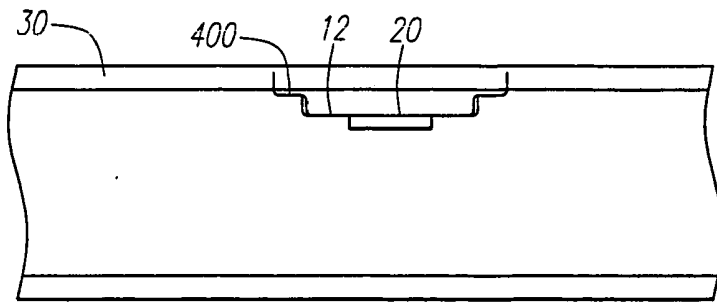


FIG. 4A

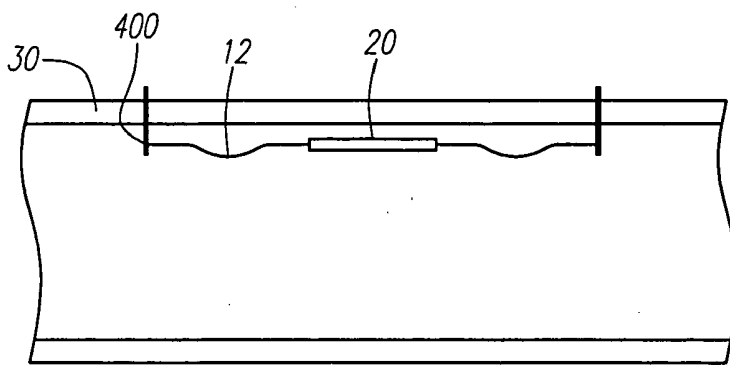


FIG. 4B

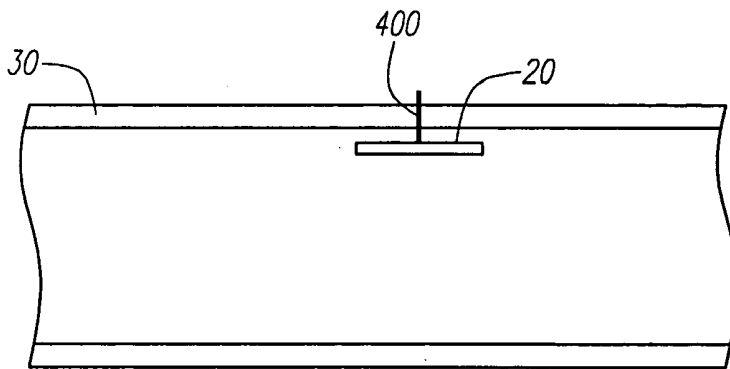


FIG. 4C

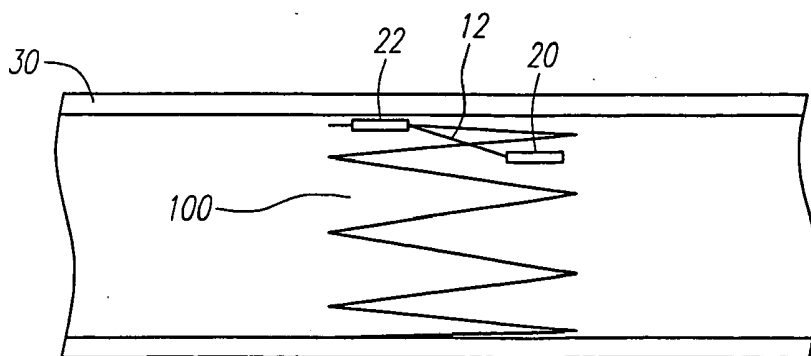


FIG. 5

## DEVICES FOR FIXING A SENSOR IN A LUMEN

### CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] The present application claims priority under 35 U.S.C. §119 to U.S. Provisional Patent Application Ser. No. 60/536,580, entitled "Device for Fixing a Sensor in a Lumen," filed Jan. 13, 2004, the complete contents of which are incorporated herein by reference.

### FIELD OF THE DISCLOSURE

[0002] The present invention relates to field of medical devices and more specifically to a device for positioning a sensor in a lumen.

### BACKGROUND

[0003] The use of sensors in body lumens is well known. For example, U.S. Pat. No. 4,485,813 describes a sensor that can be permanently implanted in a specific location within the human body in an implantable medical device such as a pacemaker. In other applications sensors are implanted alone in a body lumen. U.S. Pat. No. 6,645,143, 6,053,873, 6,442,413 and U.S. application 2002/0188207 describe medical monitoring sensors designed to be implanted in the vascular system and is capable of sensing and transmitting via a telemetry link to an external monitor.

[0004] The implanted sensors are utilized for monitoring physical, chemical or physiological parameters in the body. The aim of such sensors is to accurately monitor the desired parameter.

[0005] The position of the sensor within the lumen can influence the accuracy of the measurement. Positioning of a sensor facing a lumen wall can alter the sensing ability. Furthermore, positioning of a sensor pressing against the lumen wall in blood vessels may encourage responses, such as neo-intimal growth, which can influence and/or impact the long and short terms accuracy of measurements.

[0006] U.S. patent application publication No. 2002/0188207 discloses a device and method for anchoring a sensor at the center of the lumen. This concept addresses the issue of tissue growth. However, it is problematic to axially align multiple sensors in the same vicinity of a lumen, since a first sensor would block the further sensor(s) from blood flow through the lumen. Thus, it is desirable, and often functionally necessary, to radially and/or circumferentially off-set the sensors of a multiple sensor arrangement, so that they are not coaxially aligned. On the other hand, it is desirable, and often functionally necessary, to operably connect the individual sensors of a multiple sensor arrangement.

[0007] There are several medical procedures that require insertion of catheters or other devices through a body lumen and especially through the vascular system, for example, Swan-Ganz catheter to the pulmonary artery for monitoring hemodynamic parameters. Thus, a sensor implantation device should not prevent accessibility to a desired location within the vascular system.

### SUMMARY

[0008] One embodiment of the invention is an apparatus for positioning at least one sensor in a body lumen, the body

lumen having a wall, the apparatus including a fixation element, a sensor, and a connecting element that connects the sensor to the fixation element. The connecting element extends at least partially into the lumen so that the sensor is located radially inward from the lumen wall. Other and further embodiments and aspects of the invention are disclosed and described herein.

### BRIEF DESCRIPTION OF THE DRAWINGS

[0009] The present invention will be more fully understood and appreciated from the following detailed description taken in conjunction with the figures, in which:

[0010] **FIGS. 1A-1D** are schematic illustrations of a device having a stent-like configured fixation element according to one an embodiment of the invention.

[0011] **FIGS. 2A-2B** are schematic illustrations of a device having a coiled configured fixation element according to another embodiment of the invention.

[0012] **FIGS. 3A-3D** are schematic illustrations of a device having a wing configured fixation element according to yet another embodiment of the invention.

[0013] **FIGS. 4A-4C** are schematic illustrations of a device having a hook configured fixation element according to still another embodiment of the invention

[0014] **FIG. 5** are schematic illustrations of a device having two implants according to a still further embodiment of the invention

### DETAILED DESCRIPTION

[0015] The devices disclosed in the following detailed description enable positioning of an implant such as a sensor, a drug reservoir, or other known and/or convenient device within a lumen at a location which is between the inner lumen wall and the lumen center.

[0016] In one embodiment, the device includes a fixation part and an implant that is positioned between the lumen wall and the center of the lumen. The implant can be directly connected to the fixation part. The device can further include a connecting element for connecting between the fixation part and the implant and/or for positioning the implant at the desired location. The implant can be a sensor such as, for example, a pressure sensor that is implanted in blood vessel for monitoring blood pressure or any other known and/or convenient device. However, any known and/or convenient sensor can be used, including, but not limited to, a flow sensor, a radiation sensor, a temperature sensor, an electrical impedance sensor, other physical measurement sensor, an optical sensor for monitoring Hemoglobin concentrations and/or glucose concentrations or any other measurement, or any type of sensor for monitoring chemical species and/or composition, and/or an electrochemical sensor for monitoring various compounds within the bloods, for example, calcium, potassium, sodium and/or any other measurable compound, molecule, atom, and/or ion.

[0017] In alternate embodiments, the device can further include a second implant located either in contact with the wall or at the vicinity of the wall or in any other convenient location within a lumen. The second implant can be a second sensor such as, for example, a flow sensor for monitoring flow in the cardiovascular system or an energy source such

as a battery or any other known and/or convenient device. The second implant can be connected to the first implant. For example, a first implant which is a sensor can be electrically connected, using an isolated electric wire, to a second implant which is an energy source such as battery for enabling energy transfer from the energy source to the sensor.

[0018] In one embodiment, a first implant, which can be a sensor, can be located between the lumen wall and the center of the lumen and a second implant, which can be an energy source, can be located in contact with the lumen wall and electrically connected to the sensor. This configuration enables miniaturizing of the first implant since the energy source is not a part of the sensor.

[0019] The insertion of the device into a body lumen can be performed via a catheterization procedure. The device can be mounted on a delivery system, in a compressed configuration so as to enable navigation through the lumen, and delivered through the lumen to the desired deployment site. At the desired deployment site the expandable technique and/or any other known and/or convenient method and/or mechanism.

[0020] Other techniques for inserting a device into a lumen, such-as making an incision in the lumen and suturing the device at the desired location can be applied. Additionally, the device can be connected to other implants.

[0021] Reference is now made to FIGS. 1A-1D illustrating a device that includes a fixation element having a stent-like configuration according to an embodiment of the invention. The devices shown in the embodiments include a fixation element 100, a connecting element 12 and a sensor 20. For convenience and clarity, the lumen 30 is shown in cross-section.

[0022] In the embodiment shown in FIG. 1A, fixation element 100 can be manufactured from a wire, a laser cut tube or a chemical etched tube or sheet made of metal, for example Nickel-Titanium alloy, stainless steel titanium, cobalt-based alloy, or a polymer including a shape memory polymer with or without the addition of radio-opaque material e.g. barium sulfate or can be manufactured from any known and/or convenient material using any known and/or convenient method and having any convenient shape. In the embodiment shown in FIG. 1A, the struts 10 cross section can be round, oval, rectangular or any convenient shape. In the embodiment shown in FIG. 1A, the struts are arranged in a zigzag configuration. However in alternate embodiments, the struts can have any convenient configuration. The thickness of struts 10 is in the range of 0.05-0.5 mm. However in alternate embodiments, various other thicknesses can be used. The struts can further include ridges or hooks for preventing migration within the lumen.

[0023] FIG. 1A shows fixation element 100 having a radial zigzag configuration that is in contact with the inner side of the lumen wall. The sensor 20 can be connected to a connecting element 12 for connecting sensor 20 to fixation element 100 and for positioning sensor 20 at a desired location distanced from the lumen wall. The sensor 20 can be located between the lumen wall and the center of the lumen. In some embodiments, the sensor can be distanced from the lumen wall between 0.05 mm and 0.8 r wherein r is the lumen radius. For example, for blood vessel having

radius of  $r=10$  mm the sensor can be positioned at a distance of 0.05 to 8 mm from the vessel wall.

[0024] In some embodiments, connecting element 12 can be made of metal such as Nickel-Titanium alloy, stainless steel, titanium, cobalt-based alloy, or using tantalum, Gold, Platinum or Platinum-Iridium for enhance radio-opacity, or a polymer including a shape memory polymer with or without the addition of radio-opaque material e.g. barium sulfate, and/or composed of any known and/or convenient material and or made in any know and/or convenient shape using any known and/or convenient method.

[0025] In some embodiments, connecting element 12 can be rigid so as to maintain sensor 20 at constant position or can be flexible as illustrated in FIG. 1D, so as to enable movement of the sensor within the lumen. In alternate embodiments, sensor 20 can be connected directly to strut 10 of fixation element 100. In selected embodiments, the sensor 20, can be located in a position proximal to the fixation element 100 to reduce neo intima and cell proliferation.

[0026] In alternate embodiments, sensor 20 can be oriented parallel, perpendicular or at any other angle to the lumen wall. In still further alternate embodiments, the active face of the sensor 20 can be oriented towards the lumen center, the lumen wall or tangential and/or in any other convenient location.

[0027] Reference is now made to FIG. 1B, illustrating one configuration of the device having two fixation elements 100 at both sides, proximal and distal to the sensor 20. In the embodiment shown in FIG. 1B, proximal and distal fixation elements 100 can be connected at one or more points and sensor 20 can be connected to fixation element 100 by one connecting element. That is, sensor 20 can be connected to the distal or proximal strut or can be connected to the distal and proximal strut. Sensor 20 can be oriented parallel, perpendicular or at any other angle to the lumen wall. The active face of the sensor 20 can be oriented towards the lumen center, the lumen wall or tangential or in any convenient orientation. In some embodiments, connecting element 12 can be rigid so as to maintain sensor 20 at constant position or can be flexible so as to allow movement of sensor 20.

[0028] Reference is now made to FIG. 1C, illustrating an alternate configuration of fixation element 100 in which the struts are configured in a closed cell zigzag arrangement. However in some embodiments, any known and/or convenient strut configuration can be used. Furthermore, it will be appreciated that other configurations can be used.

[0029] Reference is now made to FIGS. 2A-2B illustrating a device having a coiled fixation element 200 according to an embodiment of the invention. The device can include coiled configured fixation element 200, connecting element 12 and sensor 20. For clarity and convenience the lumen 30 is shown in cross-sectional view.

[0030] The coiled fixation element 200 can be manufactured from a wire, a laser cut tube or a chemical etched tube or sheet made of metal, for example Nickel-Titanium alloy, stainless steel titanium, cobalt-based alloy, or a polymer including a shape memory polymer with or without the addition of radio-opaque material e.g. barium sulfate or composed of any known and/or convenient material, in any convenient shape and/or using any known and/or convenient

method. The fixation element cross-section may be round, oval, rectangular etc. The thickness of strut **10** of coiled fixation element **200** is in the range of 0.05-0.5 mm. Additionally in selected embodiments, the strut can further include ridges or hooks for preventing migration within the lumen.

[0031] The coiled fixation element **200** configuration can be radial and can be in contact with the lumen wall. The sensor **20** can be connected to a connecting element **12** for connecting sensor **20** to fixation element **200** and/or for positioning sensor **20** at a desired location distanced from the lumen wall. In alternate embodiments, sensor **20** can be connected directly to coil fixation element **200**. In various embodiments, the sensor can be located between the lumen wall and the center of the lumen. In alternate embodiments the sensor can be distanced from the lumen wall between 0.05 mm and  $0.8r$  wherein  $r$  is the lumen radius. However in alternate embodiments, the sensor can be located at any convenient distance from the lumen wall. For example, for blood vessel having radius of  $r=10$  mm the sensor can be positioned at a distance of 0.05 to 8 mm of the vessel wall. In selected embodiments, connecting element **12** can be made of metal such as Nickel-Titanium alloy, stainless steel titanium, cobalt-based alloy, or using tantalum, Gold, Platinum or Platinum-Iridium for enhance radio-opacity, or a polymer including a shape memory polymer with or without the addition of radio-opaque material e.g. barium sulfate, or any known and/or convenient material, in any convenient shape and manufactured in any known and/or convenient manner. In selected embodiments, connecting element **12** can be rigid so as to maintain sensor **20** at constant position or can be flexible so as to allow movement of sensor **20**.

[0032] The sensor **20** may be oriented parallel, perpendicular or at any other angle to the lumen wall. The active face of the sensor **20** can be oriented towards the lumen center, the lumen wall, tangential to the lumen wall or at any other convenient angle within the lumen. In selected embodiments, sensor **20** can be oriented parallel, perpendicular or at any other angle to the lumen wall.

[0033] Reference is now made to FIG. 2B, illustrating a device having coiled fixation element **200** at both sides, of sensor **20**. In the embodiment shown in FIG. 2B, proximal and distal coiled fixation element **200** can be connected at one or more points. Connecting element **12** can be rigid so as to maintain sensor **20** at constant position or can be flexible so as to allow movement of sensor **20**. Additionally, sensor **20** can be oriented parallel, perpendicular or at any other angle to the lumen wall. The active face of the sensor **20** can be oriented towards the lumen center, the lumen wall or tangential. Furthermore, sensor **20** can be oriented parallel, perpendicular or at any other angle to the lumen wall. As will be apparent to those skilled in the art, other configurations can be used.

[0034] Reference is now made to FIGS. 3A-3D, illustrating a device having a wing-configured fixation element. In the embodiments shown in FIGS. 3A-3D, the device includes wing-configured fixation element **300**, connecting element **12** and a sensor **20**. For convenience and clarity, the lumen **30** is shown in cross-sectional view.

[0035] The wing-configured fixation element **300** may be manufactured from a wire, a laser cut tube or a chemical etched tube or sheet made of metal, for example Nickel-

Titanium alloy, stainless steel titanium, cobalt-based alloy, or a polymer including a shape memory polymer with or without the addition of radio-opaque material, e.g. barium sulfate, or can be comprised of any known and/or convenient material, can be manufactured using any known and/or convenient shape and can be made using any known and/or convenient method.

[0036] The struts **10** of wing configured fixation element **300** may have a round, oval, rectangular etc. cross section. The thickness of struts **10** is in the range of 0.05-0.5 mm. The thickness of the struts may be any convenient thickness. Additionally, the struts can further include ridges or hooks for preventing migration within the lumen.

[0037] FIG. 3A is a three dimensional view of the device having wing configured fixation element **300** and FIGS. 3B and 3C illustrate longitudinal and lateral cross sections, respectively.

[0038] The sensor **20** may be connected to a connecting element **12** for connect sensor **20** to fixation element **300** and for position sensor **20** at a desired location distanced from the lumen wall. In other embodiment sensor **20** can be connected directly to fixation element **300**. The sensor can be located between the lumen wall and the center of the lumen. In one embodiment the sensor can be distanced from the lumen wall between 0.05 mm and  $0.6r$  wherein  $r$  is the lumen radius. For example, for blood vessel having radius of  $r=10$  mm the sensor can be positioned at a distance of 0.05 to 8 mm of the vessel wall. However in alternate embodiments, the sensor can be located at any convenient location within the lumen. Additionally, connecting wire **12** can be made of metal such as Nickel-Titanium alloy, stainless steel titanium, cobalt-based alloy, or using tantalum, Gold, Platinum or Platinum-Iridium for enhance radio-opacity, or a polymer including a shape memory polymer with or without the addition of radio-opaque material e.g. barium sulfate, or any known and/or convenient material, made in any convenient shape using any known and/or convenient manufacturing process.

[0039] In alternate embodiments, connecting element **12** can be made of metal such as Nickel-Titanium alloy, stainless steel titanium, a polymer or any known and/or convenient material. The connecting element **12** can be rigid so as to maintain sensor **20** at constant position or can be flexible so as to enable movement of the sensor within the lumen. In alternate embodiments, sensor **20** can be connected directly to fixation element **300**.

[0040] In the embodiments shown in FIGS. 3A-3C, sensor **20** can be oriented parallel, perpendicular or at any other angle to the lumen wall. The active face of the sensor **20** can be oriented towards the lumen center, the lumen wall, tangential to the lumen wall or at any other convenient angle.

[0041] FIG. 3D illustrates a lateral cross section of another configuration of the wing fixation element **300**. In the configuration shown in FIG. 3D, the sensor is at the same level as the strut. In those embodiments in which the struts **10** are made of superelastic Nickel-Titanium alloy, intermediate levels of expansion can be implemented such that the predetermined distances of the sensor from the vessel wall can be achieved.

[0042] Reference is now made to FIGS. 4A-4C, illustrating a device having a hook configured fixation element

according to an embodiment of the invention. The device includes hook configured fixation element **400**, connecting element **12** and a sensor **20**. Cross section of lumen **30**, for example a blood vessel, is shown.

[0043] Fixation element **400** can be manufactured from a wire, a laser cut or a chemical etched tube or sheet made of metal, for example Nickel-Titanium alloy, stainless steel titanium, cobalt-based alloy, or a polymer including a shape memory polymer with or without the addition of radio-opaque material e.g. barium sulfate or of any known and/or convenient material, can be manufactured in any convenient shape using any known and/or convenient method of manufacture. The strut of fixation element **400** cross section can be round, oval, rectangular or have any convenient shape. The thickness of struts is in the range of 0.05-1 mm. The struts can have any convenient thickness and/or dimensions. Additionally, the struts can further includes ridges or hooks for anchoring fixation element **400** within the lumen and preventing migration within the lumen.

[0044] FIG. 4A shows a device having a hook configured fixation element **400** that is hooked into the lumen wall at least at two points. Hooking can be at the longitudinal axis of the lumen as shown in FIG. 4A or at the transverse axis (not shown).

[0045] The sensor **20** can be connected to a connecting wire **12**, which is configured so as to distances the sensor from the lumen wall. The connecting wire **12** is connected to the fixation element **400**. The sensor can be located between the lumen wall and the center of the lumen. In one embodiment the sensor can be distanced from the lumen wall between 0.05 mm and 0.8 r wherein r is the lumen radius. For example, for blood vessel having radius of r=10 mm the sensor can be positioned at a distance of 0.05 to 8 mm of the vessel wall. However in alternate embodiments, the sensor can be located at any convenient location within the lumen.

[0046] Connecting element **12** can be made of metal such as Nickel-Titanium alloy, stainless steel titanium, cobalt-based alloy, or using tantalum, Gold, Platinum or Platinum-Iridium for enhance radio-opacity, or a polymer including a shape memory polymer with or without the addition of radio-opaque material e.g. barium sulfate or any known and/or convenient material, can have any convenient shape and can be manufactured using any convenient manufacturing process. Connecting element **12** can be rigid so as to maintain sensor **20** at constant position or can be flexible as illustrated in FIG. 4B, so as to enable movement of the sensor within the lumen. In other embodiment sensor **20** can be connected directly to fixation element **400**.

[0047] The sensor **20** can be oriented parallel, perpendicular or at any other angle to the lumen wall. The active face of the sensor **20** can be oriented towards the lumen center, the lumen wall, tangential to the lumen wall or at any other convenient angle.

[0048] Reference is now made to FIG. 4C, illustrating another configuration of fixation element **400** in which the fixation element **400** is inserted in the lumen similarly to the insertion of a drawing pin. The sensor **20** can be directly connected to fixation element **400** or connected via a connecting wire.

[0049] The sensor **20** can be oriented parallel, perpendicular or at any other angle to the lumen wall. The active face

of the sensor **20** can be oriented towards the lumen center, the lumen wall, tangential to the lumen wall or any other convenient angle. Additionally, it will be appreciated that other configurations can be used.

[0050] Reference is now made to FIG. 5 which is a schematic illustration of a device having two implants according to an embodiment of the invention. The device includes a fixation element **100**, a first implant **20**, a second implant **22**, and a connecting element **12**. For convenient and clarity, the lumen, which can be a blood vessel, is shown in cross-section.

[0051] It will be appreciated that fixation element **100** can have any other configuration such as, for example, coil, wing, hook and/or any other known and or convenient configuration.

[0052] A first implant **20** may be located between the lumen wall and the center of the lumen. First implant **20** can be distanced from the lumen wall between 0.05 mm and 0.8 r wherein r is the lumen radius. For example, for blood vessel having radius of r=10 mm the first implant can be positioned at a distance of 0.05 to 8 mm of the vessel wall. Second implant **22** can be in contact with the lumen wall or distances from the lumen wall. However in alternate embodiments, the first and second implants can be located at any convenient locations within the lumen and relative to each other.

[0053] The first implant **20** and second implant **22** may be connected by connecting element **12**. Second implant **22** can be directly connected to fixation element **100** or connected through an additional connecting element.

[0054] The connecting element **12** may be made of metal such as Nickel-Titanium alloy, stainless steel titanium, cobalt-based alloy, or using tantalum, Gold, Platinum or Platinum-Iridium for enhance radio-opacity, or a polymer including a shape memory polymer with or without the addition of radio-opaque material e.g. barium sulfate, or of any other know and/or convenient material.

[0055] The connecting element **12** may be rigid so as to maintain first implant **20** at constant position or can be flexible so as to enable movement of first implant **20** within the lumen. Connecting element **12** that connects first implant **20** to second implant **22** can be a metallic or a plastic tube that includes an electric wire for enabling electric communication between first and second implants. The connection between first implant **20** and second implant **22** can be achieved using mechanical means, crimp, adhesives, welding or any other convenient mechanism and/or material. In alternate embodiments, the connection between the first implant **20** and second implant **22** can be wireless, wired or made in any other known and/or convenient manner. Furthermore, in embodiments in which the second implant **22** is physically connected with the first implant and/or the fixation element **100**, the connection element can support both the first implant and the second implant. Alternately, each implant can have an separate connection element **12** to connect the implant with the fixation element.

[0056] In one embodiment first implant **20** can be a sensor such as pressure sensor and second implant **22** can be an energy source such as a battery. The sensor and the battery can be connected by electric wire for enabling energy transfer from the battery to the sensor.

[0057] While the invention is susceptible to various modifications, and alternative forms, specific examples thereof have been shown in the drawings and are herein described in detail. It should be understood, however, that the invention is not to be limited to the particular embodiments or methods disclosed, but to the contrary, the invention is to cover all modifications, equivalents and alternatives falling within the scope of the appended claims.

1. An apparatus for positioning at least one sensor in a body lumen, the lumen having a wall, the apparatus comprising:

a fixation element;  
a first sensor; and

a first connecting element connecting the first sensor to the fixation element, the first connecting element extending at least partially into the lumen so that the first sensor is located radially inward from the lumen wall.

2. The apparatus of claim 1, wherein the first sensor is located at least approximately 0.05 mm away from the lumen wall.

3. The apparatus of claim 2, wherein the first sensor is located less than approximately 0.8 r away from the lumen wall, wherein r represents the lumen radius.

4. The apparatus of claim 1, wherein the fixation element is configured as one of a stent, a coil, a wing and a hook.

5. The apparatus of claim 1, wherein the body lumen is a component of a vascular system.

6. The apparatus of claim 1, wherein the first sensor measures at least one of blood pressure, blood temperature and blood composition.

7. The apparatus of claim 1, wherein the first connecting element extends from, or is otherwise connected to, the fixation element.

8. The apparatus of claim 1, further comprising a second connecting element connecting the first sensor to the fixation element.

9. The apparatus of claim 8, the first connecting element at least partially extending in a first direction along a longitudinal axis of the lumen, and the second connecting element extending at least partially in a second direction along the longitudinal lumen axis that is substantially opposite the first direction.

10. The apparatus of claim 1, further comprising a second sensor and a second connecting element, the second connecting element connecting the second sensor to the fixation element, the second connecting element extending at least partially into the lumen so that the second sensor is located radially inward from the lumen wall, wherein the first sensor

and the second sensor are positioned such that they are other than co-axially aligned with a longitudinal axis of the lumen.

11. The apparatus of claim 10, wherein the first and second sensors each measure at least one of blood pressure, blood temperature and blood composition.

12. An apparatus for positioning at least one sensor in a body lumen, comprising:

a fixation element configured for self-anchoring within the lumen;  
a sensor; and

means for connecting the sensor to the fixation element so that the sensor is positioned radially inward from a wall of the lumen.

13. The apparatus of claim 12, wherein the sensor is positioned at least 0.05 mm away from the lumen wall and less than 0.8 r away from the lumen wall, wherein r is the radius of the lumen.

14. The apparatus of claim 12, wherein the fixation element is configured as one of a stent, a coil, a wing and a hook, and wherein the sensor measures at least one of blood pressure, blood temperature and blood composition.

15. The apparatus of claim 12, the connecting means comprising first and second struts extending from, or otherwise connected to, the fixation element.

16. The apparatus of claim 15, the first strut at least partially extending in a first direction along a longitudinal axis of the lumen, and the second strut extending at least partially in a second direction along the longitudinal lumen axis that is substantially opposite the first direction.

17. An apparatus for positioning two or more sensors within a body lumen, comprising:

a fixation element configured for self-anchoring within a lumen;

a first sensor coupled with the fixation element, wherein the first sensor is positioned at least 0.05 mm inwardly from a wall of the lumen and less than 0.8 r inwardly away from the wall of the lumen, wherein r is the radius of the lumen; and

a second sensor coupled with the fixation element and the first sensor, wherein the second sensor is positioned at least 0.05 mm inwardly from a wall of the lumen and less than 0.8 r inwardly away from the wall of the lumen;

wherein the first sensor and the second sensor are positioned such that they are other than co-axially aligned with a longitudinal axis of the lumen.

\* \* \* \* \*

专利名称(译)	用于将传感器固定在内腔中的装置		
公开(公告)号	<a href="#">US20050154321A1</a>	公开(公告)日	2005-07-14
申请号	US11/034502	申请日	2005-01-12
[标]申请(专利权)人(译)	REMON医疗TECH		
申请(专利权)人(译)	REMON MEDICAL TECHNOLOGIES LTD		
当前申请(专利权)人(译)	REMON MEDICAL TECHNOLOGIES LTD		
[标]发明人	WOLINSKY LONE BEN YOSEPH ALON PENNER ABRAHAM		
发明人	WOLINSKY, LONE BEN-YOSEPH, ALON PENNER, ABRAHAM		
IPC分类号	A61B5/00 A61B5/0215 A61F2/02 A61F2/82 A61F2/86 A61B5/02		
CPC分类号	A61B5/0031 A61B5/0215 A61B5/145 A61B5/6882 A61F2230/0091 A61F2/82 A61F2/86 A61F2250/0002 A61B5/6886		
优先权	60/536580 2004-01-13 US		
其他公开文献	US7572228		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

用于将至少一个传感器定位在体腔中的装置，该装置包括固定元件，传感器和将传感器连接到固定元件的连接元件，该连接元件至少部分地延伸到管腔中，使得传感器是从腔的壁径向向内定位。

