



US007706896B2

(12) **United States Patent**
Music et al.

(10) **Patent No.:** **US 7,706,896 B2**
(45) **Date of Patent:** **Apr. 27, 2010**

- (54) **USER INTERFACE AND IDENTIFICATION IN A MEDICAL DEVICE SYSTEM AND METHOD**
 - 4,770,179 A 9/1988 New, Jr. et al.
 - 4,805,623 A 2/1989 Jöbbsis
 - 4,869,254 A 9/1989 Stone et al.
 - 4,911,167 A 3/1990 Corenman et al.
- (75) Inventors: **Doug Music**, Livermore, CA (US);
Darius Eghbal, Oakland, CA (US);
Steve Vargas, Pleasanton, CA (US)
 - 4,936,679 A 6/1990 Mersch
 - 4,972,331 A 11/1990 Chance
 - 5,078,136 A 1/1992 Stone et al.
 - 5,119,815 A 6/1992 Chance
- (73) Assignee: **Nellcor Puritan Bennett LLC**, Boulder, CO (US)
 - 5,122,974 A 6/1992 Chance
 - 5,167,230 A 12/1992 Chance
 - 5,297,548 A 3/1994 Pologe
- (*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.
 - 5,351,685 A 10/1994 Potratz
 - 5,355,880 A 10/1994 Thomas et al.

(21) Appl. No.: **11/540,385**

(Continued)

(22) Filed: **Sep. 29, 2006**

FOREIGN PATENT DOCUMENTS

(65) **Prior Publication Data**
US 2008/0189783 A1 Aug. 7, 2008

DE 19932147 A1 1/2001

(51) **Int. Cl.**

- G06F 3/00** (2006.01)
- G05B 11/01** (2006.01)
- G05B 15/00** (2006.01)
- A61B 5/00** (2006.01)
- G06F 17/00** (2006.01)
- G06F 7/04** (2006.01)

(Continued)

OTHER PUBLICATIONS

Definition of "physiological"; 1 page.*

(Continued)

Primary Examiner—Ronald D Hartman, Jr.

(52) **U.S. Cl.** **700/17; 700/83; 715/700; 600/301; 600/323; 726/1; 726/2**

(57) **ABSTRACT**

(58) **Field of Classification Search** **705/2-3; 340/539.12, 539.13; 715/700; 700/17, 83; 600/301, 323; 726/1, 2**


See application file for complete search history.

There are provided systems and methods for user interface and identification in a medical device. More specifically, in one embodiment, there is provided a method for accessing a medical device, the method comprising detecting an identification tag, reading identification information from the identification tag, determining if a person corresponding to the identification information has been approved to access the medical device, and if the person has been approved, granting access to the medical device.

(56) **References Cited**
U.S. PATENT DOCUMENTS

- 3,638,640 A 2/1972 Shaw
- 4,621,643 A 11/1986 New, Jr. et al.
- 4,653,498 A 3/1987 New, Jr. et al.
- 4,700,708 A 10/1987 New, Jr. et al.
- 4,714,341 A 12/1987 Hamaguri et al.

17 Claims, 10 Drawing Sheets

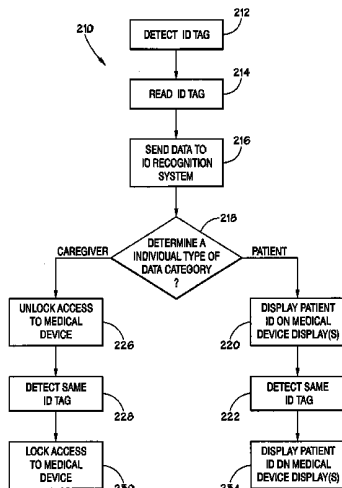

U.S. PATENT DOCUMENTS							
			7,231,263	B2 *	6/2007	Choi	700/17
			7,395,214	B2 *	7/2008	Shillingburg	705/2
			7,423,526	B2	9/2008	Despotis	
5,368,026	A	11/1994	Swedlow et al.				
5,372,136	A	12/1994	Steuer et al.				
5,385,143	A	1/1995	Aoyagi	2001/0005773	A1	6/2001	Larsen et al.
5,482,036	A	1/1996	Diab et al.	2001/0016696	A1 *	8/2001	Bystrom et al.
5,533,507	A	7/1996	Potratz	2001/0020122	A1	9/2001	Steuer et al.
5,553,614	A	9/1996	Chance	2001/0039376	A1	11/2001	Steuer et al.
5,564,417	A	10/1996	Chance	2001/0044700	A1	11/2001	Kobayashi et al.
5,575,285	A	11/1996	Takanashi et al.	2002/0026106	A1	2/2002	Khalil et al.
5,630,413	A	5/1997	Thomas et al.	2002/0035318	A1	3/2002	Mannheimer et al.
5,645,059	A	7/1997	Fein et al.	2002/0038079	A1	3/2002	Steuer et al.
5,645,060	A	7/1997	Yorkey	2002/0038081	A1	3/2002	Fein et al.
5,662,106	A	9/1997	Swedlow et al.	2002/0038392	A1 *	3/2002	De La Huerga
5,692,503	A	12/1997	Keunstner	2002/0042558	A1	4/2002	Mendelson
5,758,644	A	6/1998	Diab et al.	2002/0049389	A1	4/2002	Abreu
5,779,631	A	7/1998	Chance	2002/0062071	A1	5/2002	Diab et al.
5,830,139	A	11/1998	Abreu	2002/0111748	A1	8/2002	Kobayashi et al.
5,842,981	A	12/1998	Larsen et al.	2002/0133068	A1	9/2002	Huiku
5,873,821	A	2/1999	Chance et al.	2002/0161287	A1	10/2002	Schmitt
5,995,856	A	11/1999	Mannheimer et al.	2002/0161290	A1	10/2002	Chance
6,011,986	A	1/2000	Diab et al.	2002/0165439	A1	11/2002	Schmitt
6,035,223	A	3/2000	Baker	2002/0198443	A1	12/2002	Ting
6,064,898	A	5/2000	Aldrich	2003/0023140	A1	1/2003	Chance
6,120,460	A	9/2000	Abreu	2003/0048312	A1	3/2003	Zimmerman et al.
6,134,460	A	10/2000	Chance	2003/0055324	A1	3/2003	Wasserman
6,163,715	A	12/2000	Larsen et al.	2003/0060693	A1	3/2003	Monfre et al.
6,181,958	B1	1/2001	Steuer et al.	2003/0139687	A1	7/2003	Abreu
6,230,035	B1	5/2001	Aoyagi et al.	2003/0144584	A1	7/2003	Mendelson
6,266,546	B1	7/2001	Steuer et al.	2003/0144878	A1 *	7/2003	Wilkes et al.
6,312,393	B1	11/2001	Abreu	2003/0195402	A1	10/2003	Fein et al.
6,359,612	B1	3/2002	Fritz et al.	2003/0216974	A1 *	11/2003	Browne
6,397,091	B2	5/2002	Diab et al.	2003/0220548	A1	11/2003	Schmitt
6,398,744	B2 *	6/2002	Bystrom et al.	2003/0220576	A1	11/2003	Diab
6,415,236	B2	7/2002	Kobayashi et al.	2004/0006261	A1	1/2004	Swedlow et al.
6,438,399	B1	8/2002	Kurth	2004/0010188	A1	1/2004	Wasserman
6,445,597	B1	9/2002	Boylan et al.	2004/0054270	A1	3/2004	Pewzner et al.
6,478,800	B1	11/2002	Fraser et al.	2004/0078231	A1 *	4/2004	Wilkes et al.
6,487,439	B1	11/2002	Skladnev et al.	2004/0087846	A1	5/2004	Wasserman
6,501,974	B2	12/2002	Huiku	2004/0107065	A1	6/2004	Al-Ali
6,501,975	B2	12/2002	Diab et al.	2004/0127779	A1	7/2004	Steuer et al.
6,526,301	B2	2/2003	Larsen et al.	2004/0162472	A1	8/2004	Berson et al.
6,544,193	B2	4/2003	Abreu	2004/0167465	A1 *	8/2004	Mihai et al.
6,546,267	B1	4/2003	Sugiura et al.	2004/0171920	A1	9/2004	Mannheimer et al.
6,549,795	B1	4/2003	Chance	2004/0176670	A1	9/2004	Takamura et al.
6,591,122	B2	7/2003	Schmitt	2004/0176671	A1	9/2004	Fine et al.
6,594,513	B1	7/2003	Jobsis et al.	2004/0186357	A1 *	9/2004	Soderberg et al.
6,606,509	B2	8/2003	Schmitt	2004/0230106	A1	11/2004	Schmitt et al.
6,615,064	B1	9/2003	Aldrich	2005/0052275	A1	3/2005	Houle
6,622,095	B2	9/2003	Kobayashi et al.	2005/0062603	A1 *	3/2005	Fuerst et al.
6,658,277	B2	12/2003	Wasserman	2005/0080323	A1	4/2005	Kato
6,662,030	B2	12/2003	Khalil et al.	2005/0101850	A1	5/2005	Parker
6,671,526	B1	12/2003	Aoyagi et al.	2005/0107676	A1	5/2005	Acosta et al.
6,671,528	B2	12/2003	Steuer et al.	2005/0108057	A1 *	5/2005	Cohen et al.
6,678,543	B2	1/2004	Diab et al.	2005/0113656	A1	5/2005	Chance
6,690,958	B1	2/2004	Walker et al.	2005/0168722	A1	8/2005	Forstner et al.
6,693,812	B1	2/2004	Li et al.	2005/0192488	A1	9/2005	Bryenton et al.
6,708,048	B1	3/2004	Chance	2005/0203357	A1	9/2005	Debreczeny et al.
6,711,424	B1	3/2004	Fine et al.	2005/0234317	A1	10/2005	Chance et al.
6,711,425	B1	3/2004	Reuss	2005/0234381	A1	10/2005	Guenter et al.
6,748,254	B2	6/2004	O'Neil et al.	2005/0247319	A1 *	11/2005	Berger
6,785,568	B2	8/2004	Chance	2005/0267346	A1	12/2005	Faber et al.
6,801,797	B2	10/2004	Mannheimer et al.	2005/0280531	A1	12/2005	Fadem et al.
6,801,799	B2	10/2004	Mendelson	2006/0009688	A1	1/2006	Lamego et al.
6,873,865	B2	3/2005	Steuer et al.	2006/0015021	A1	1/2006	Cheng
6,934,571	B2	8/2005	Wiesmann et al.	2006/0020181	A1	1/2006	Schmitt
6,949,081	B1	9/2005	Chance	2006/0025660	A1	2/2006	Swedlow et al.
6,954,148	B2 *	10/2005	Pulkkinen et al.	2006/0030762	A1	2/2006	David et al.
6,961,598	B2	11/2005	Diab	2006/0030763	A1	2/2006	Mannheimer et al.
7,001,334	B2	2/2006	Reed et al.	2006/0030765	A1	2/2006	Swedlow et al.
7,027,849	B2	4/2006	Al-Ali	2006/0032918	A1 *	2/2006	Andreasson et al.
7,171,277	B2 *	1/2007	Engleson et al.	2006/0052680	A1	3/2006	Diab
7,215,991	B2	5/2007	Besson et al.	2006/0058683	A1	3/2006	Chance
				2006/0069319	A1	3/2006	Elhag et al.

2006/0079794	A1	4/2006	Liu et al.	
2006/0132283	A1	6/2006	Eberhart et al.	
2006/0155589	A1 *	7/2006	Lane et al.	705/4
2006/0185005	A1 *	8/2006	Graves et al.	726/9
2006/0211932	A1	9/2006	Al-Ali et al.	
2006/0276714	A1	12/2006	Holt et al.	
2007/0033068	A1 *	2/2007	Rao et al.	705/2
2007/0180047	A1 *	8/2007	Dong et al.	709/217
2007/0258626	A1 *	11/2007	Reiner	382/115
2008/0004513	A1	1/2008	Walker et al.	
2008/0194925	A1	8/2008	Alsafadi et al.	
2008/0208009	A1	8/2008	Shklarski	

FOREIGN PATENT DOCUMENTS

DE	102 13 692	A1	10/2003
EP	1643401		4/2006
JP	5-212016		8/1993
WO	WO 92/20273		11/1992
WO	WO 94/03102		2/1994
WO	WO 97/49330		12/1997
WO	WO 01/45553	A1	6/2001
WO	0237466		5/2002
WO	05114524		12/2005
WO	06006107		1/2006
WO	06006158		1/2006
WO	06009830		1/2006
WO	06048840		5/2006
WO	06051464		5/2006
WO	06064397		6/2006
WO	06109072		10/2006
WO	07071180		6/2007
WO	07131064		11/2007
WO	08004205		1/2008
WO	2006087689		8/2008

OTHER PUBLICATIONS

- Wikipedia—Definition of “Pulse Oximeter”; 3 pages.*
- eNewsletter—Access Control Newsletter; 3 pages.*
- Internet Archive Wayback Machine; 1 page.*
- Cardax Command Centre; “New Product Profile”; 2 pages.*
- Cardax Command Centre; “Technical Spec”; 2 pages.*

- News; Cardax FT version 4.2 released; 2 pages.*
- Lee, Jason C.S., et al., “Measurement of Percent Carboxyhemoglobin with Pulse-Oximetry Technique,” *IEEE Engineering in Medicine & Biology Society 10th Annual International Conference*, CH2566-88, vol. 88, pp. 1781-1782 (1988).
- Lee, Jason C.S., et al., “Simultaneous Measurement of Percent Carboxyhemoglobin and Functional Oxygen Saturation,” *IEEE Engineering in Medicine and Biology Society*, CH2770-6, vol. 89, pp. 1092-1093.
- Bongard, Frederic S., et al., “Continuous Dual Oximetry in Surgical critical care—Indications and Limitations,” *Annals of Surgery*, vol. 216, No. 1, pp. 60-68 (1992).
- Herman, Bruce, MD, et al., “Assessment of Dysphagia with the Use of Pulse Oximetry”, *Dysphagia* 14:152-156; Copyright Springer-Verlag New York Inc. 1999.
- Tsien, Christine L., “TrendFinder: Automated Detection of Alarmable Trends”, Massachusetts Institute of Technology, Jun. 2000 (241 pages).
- In re Application of: Doug Music, et al. Entitled: Systems and Methods for User Interface and Identification in a Medical Device U.S. Appl. No. 11/540,016; Filed: Sep. 29, 2006.
- In re Application of: Doug Music, et al. Entitled: System and Method for User Interface and Identification in a Medical Device U.S. Appl. No. 11/541,069; Filed: Sep. 29, 2006.
- In re Application of: Doug Music, et al. Entitled: User Interface and Identification in a Medical Device Systems and Methods U.S. Appl. No. 11/540,895; Filed: Sep. 29, 2006.
- In re Application of Li Li, et al. Entitled: System and Method for Secure Voice Identification in a Medical Device U.S. Appl. No. 11/540,242; Filed: Sep. 29, 2006.
- In re Application of Robin S. Boyce, et al. Entitled: System and Method for Display Control of Patient Monitor U.S. Appl. No. 11/540,379; Filed: Sep. 29, 2006.
- In re Application of: Michael P. O’Neil, et al. Entitled: Systems and Methods for Secure Voice Identification and Medical Device Interface U.S. Appl. No. 11/540,015; Filed: Sep. 29, 2006.
- In re Application of Jayesh Shah, et al. Entitled: System and Method for Integrating voice with a Medical Device U.S. Appl. No. 11/540,457; Filed Sep. 29, 2006.
- ISR, PCT/US2007/020847,6 pages, mailed Jun. 6, 2008.

* cited by examiner

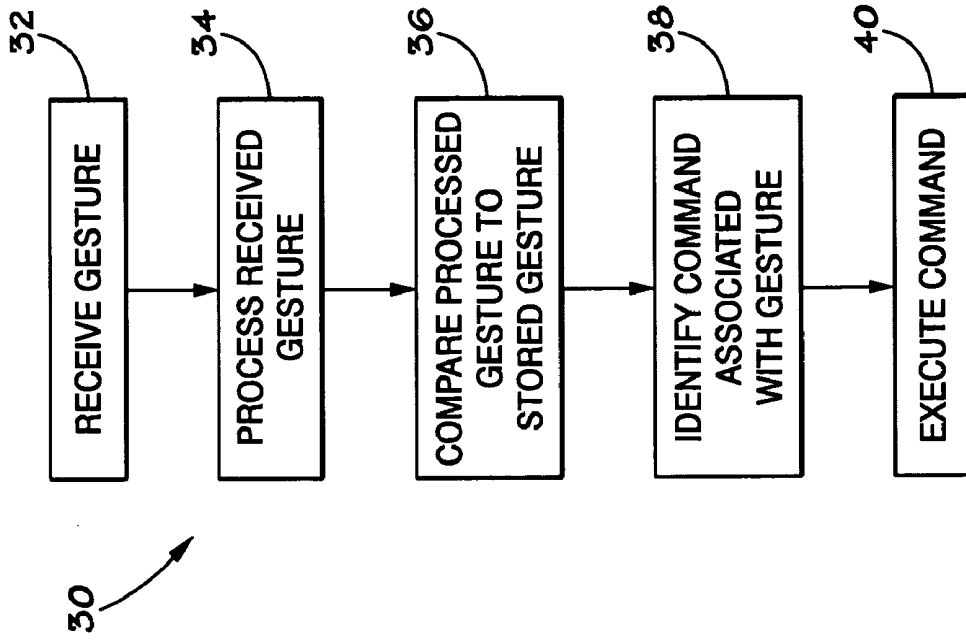


FIG. 2

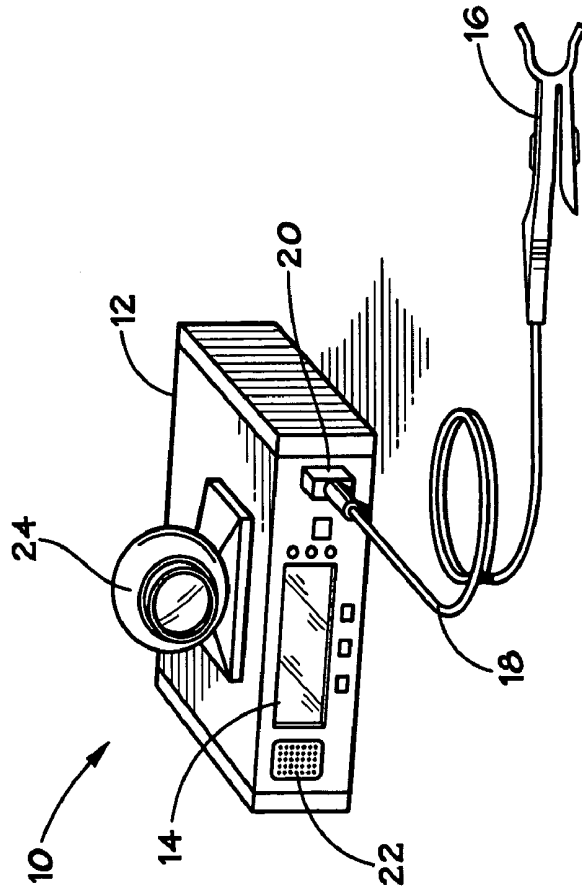


FIG. 1

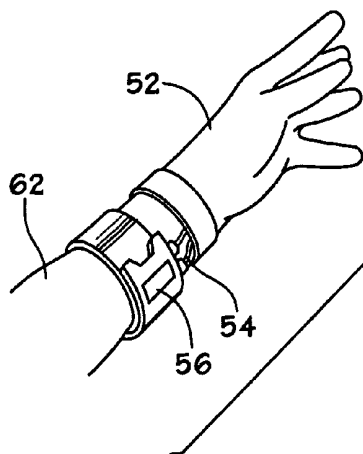
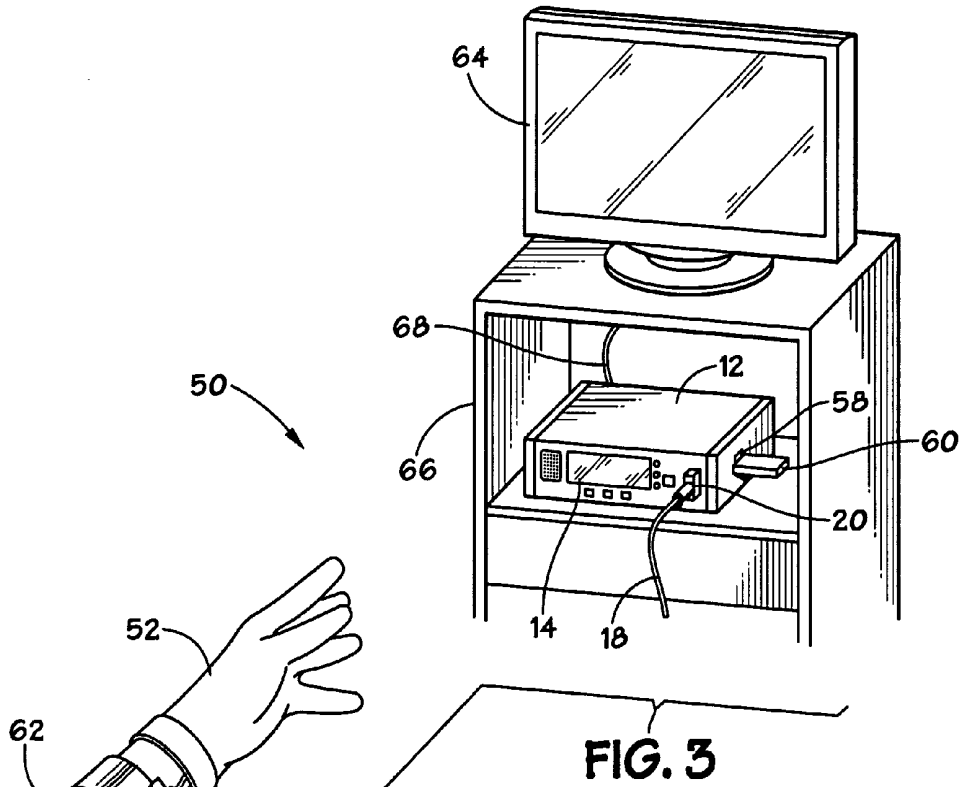


FIG. 4

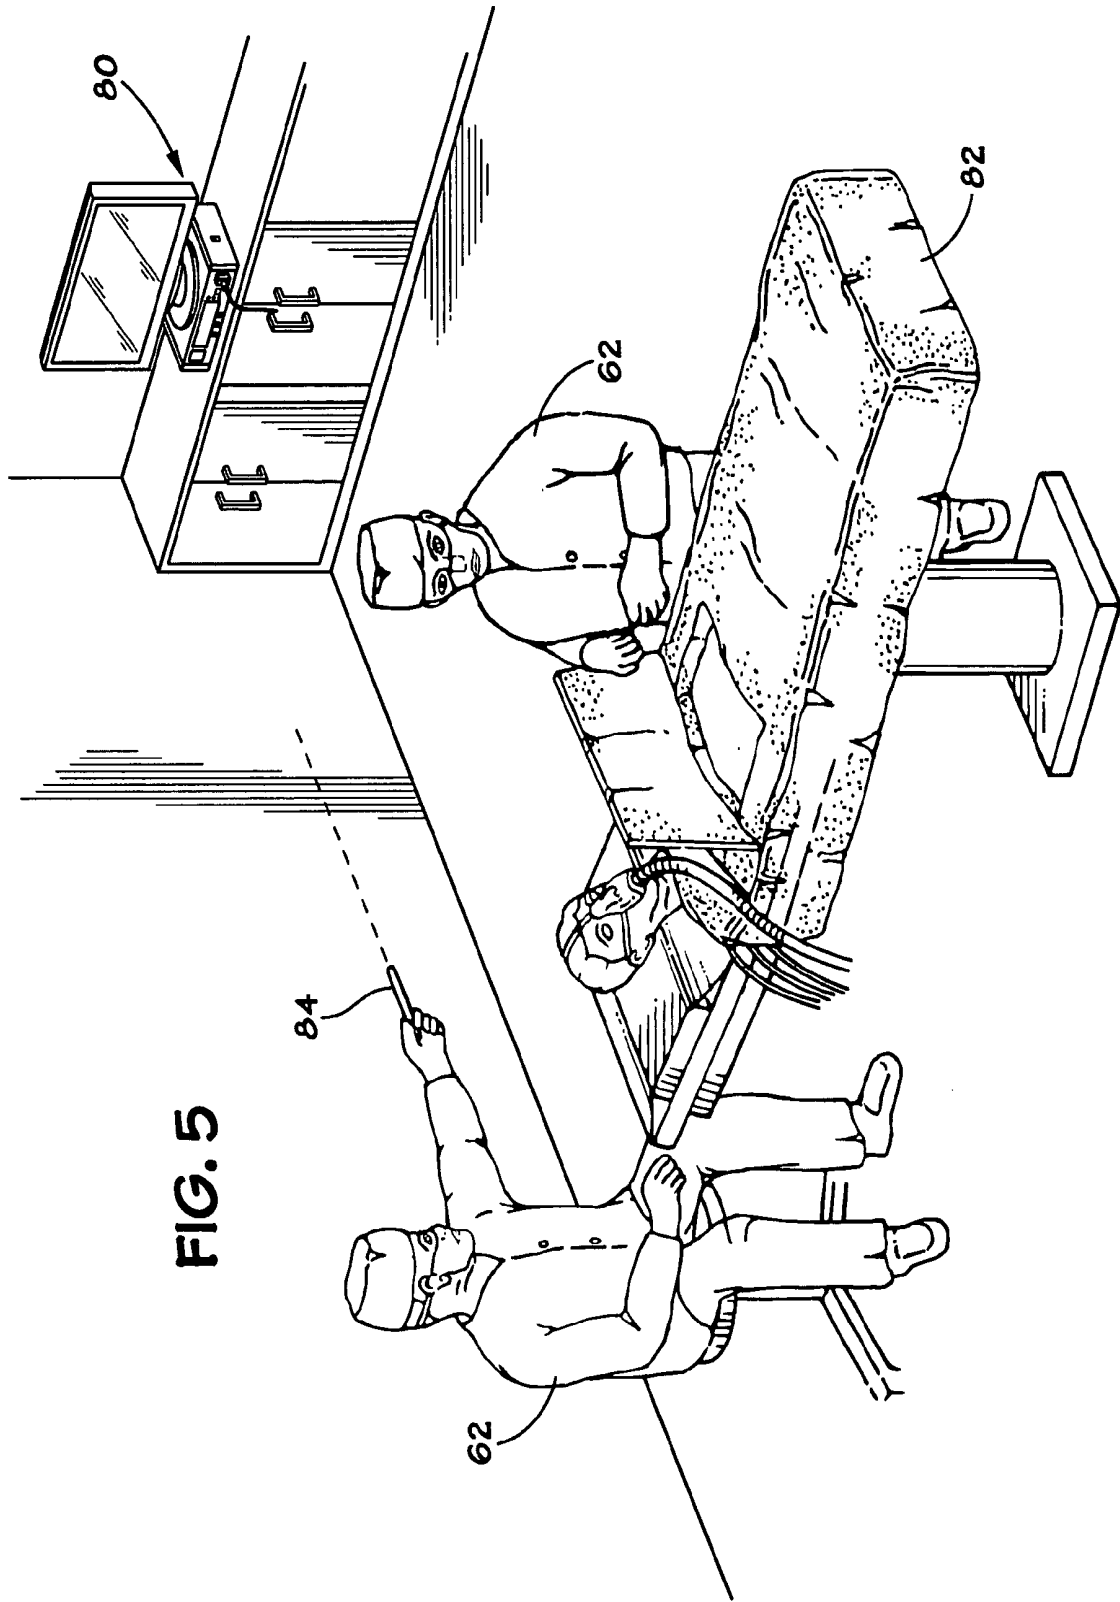


FIG. 5

FIG. 6


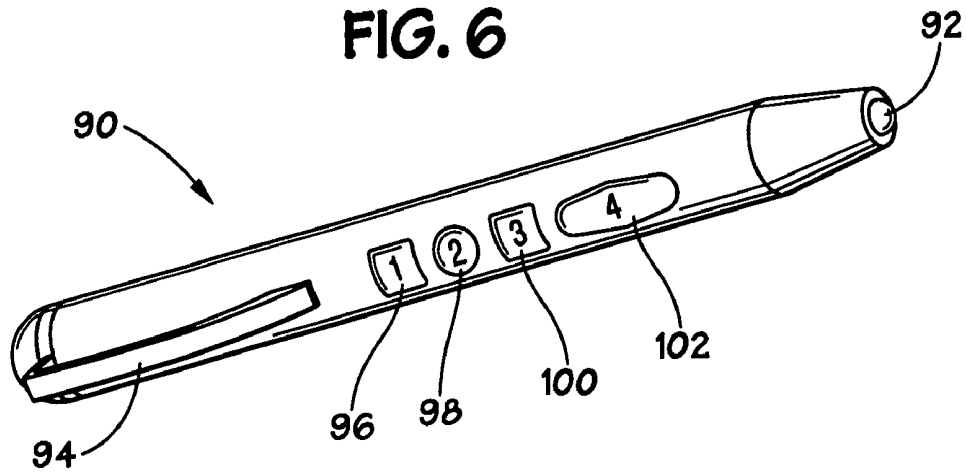


FIG. 7

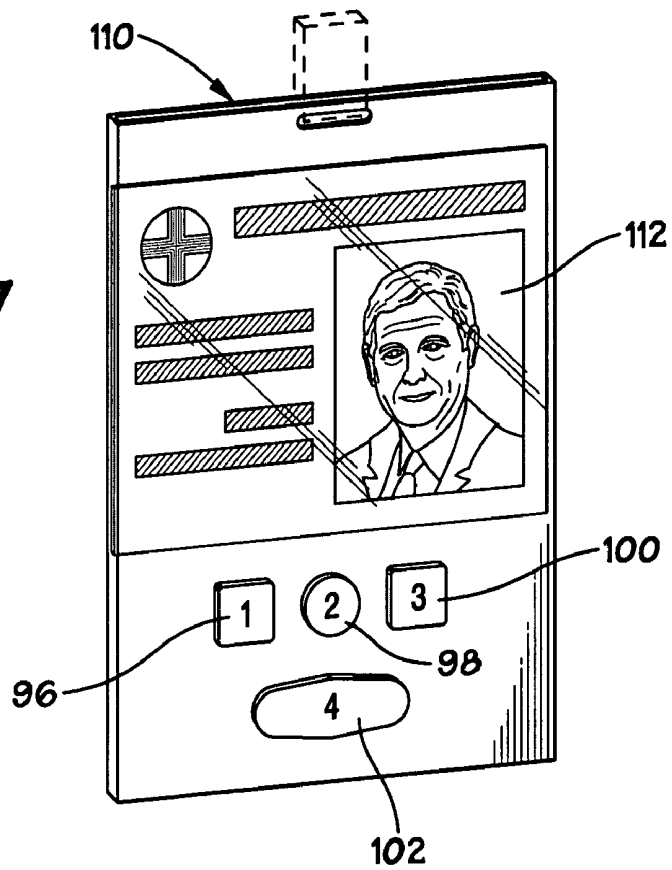

120

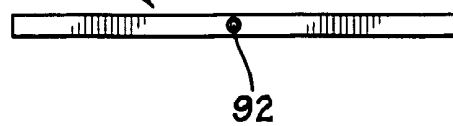
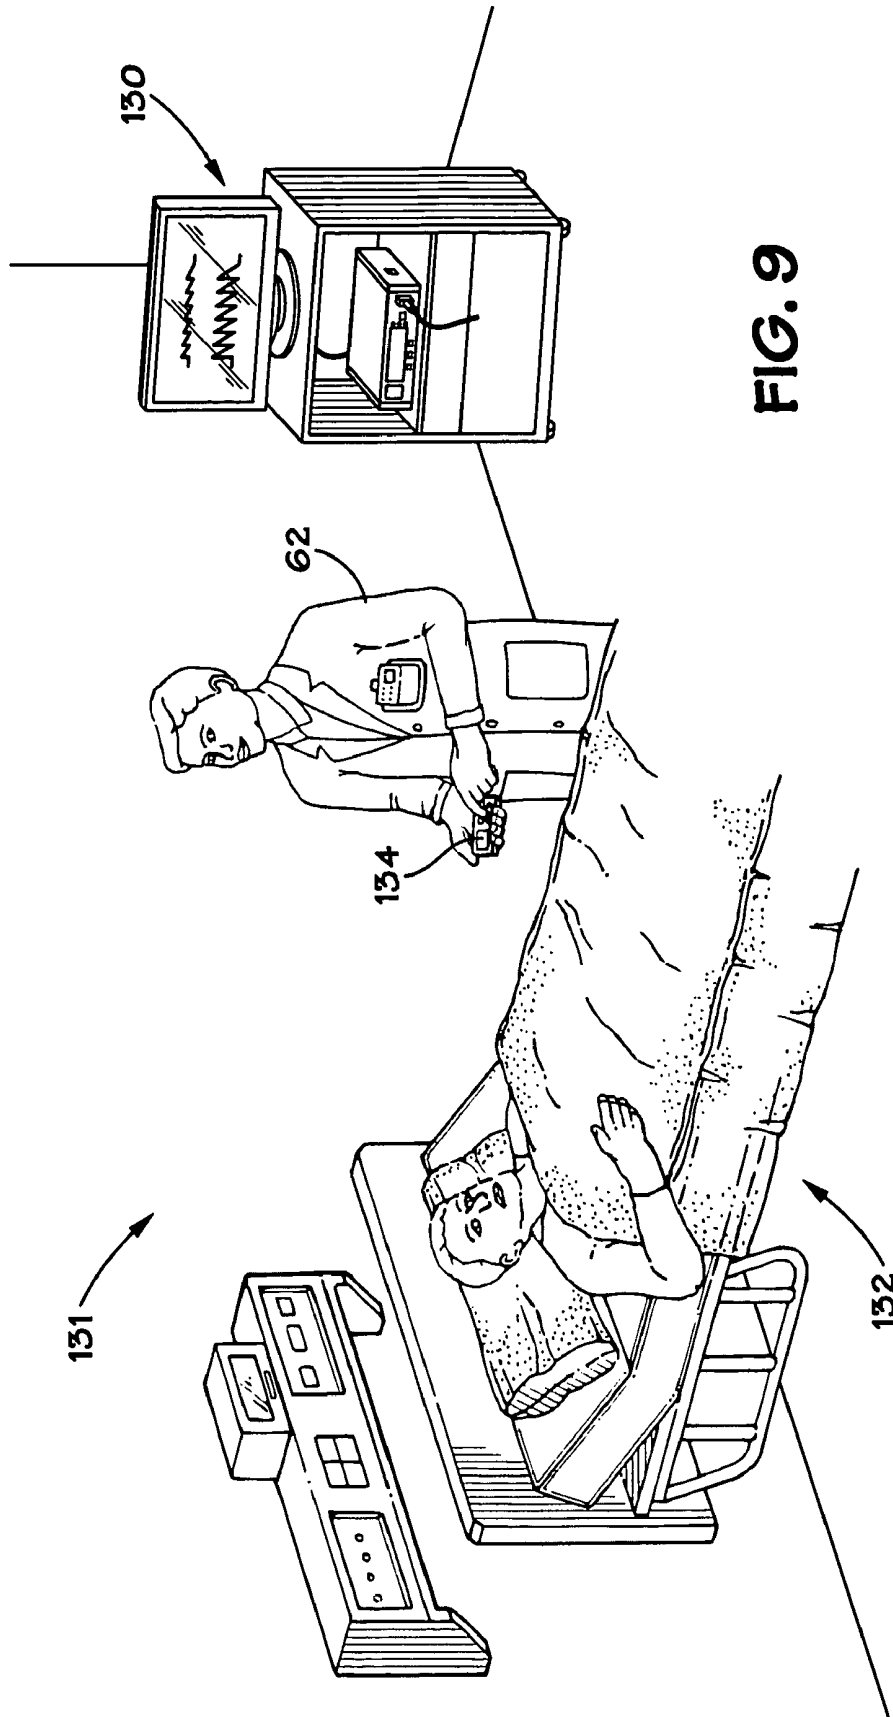


FIG. 8



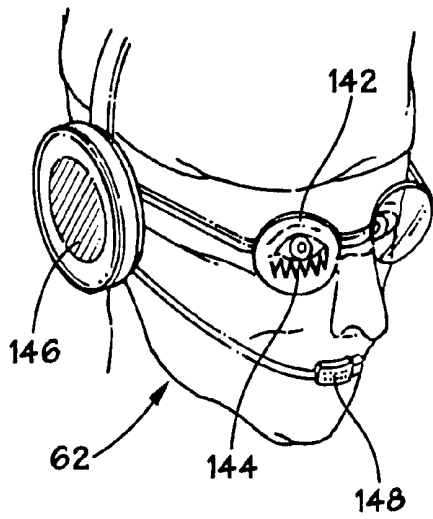


FIG. 11

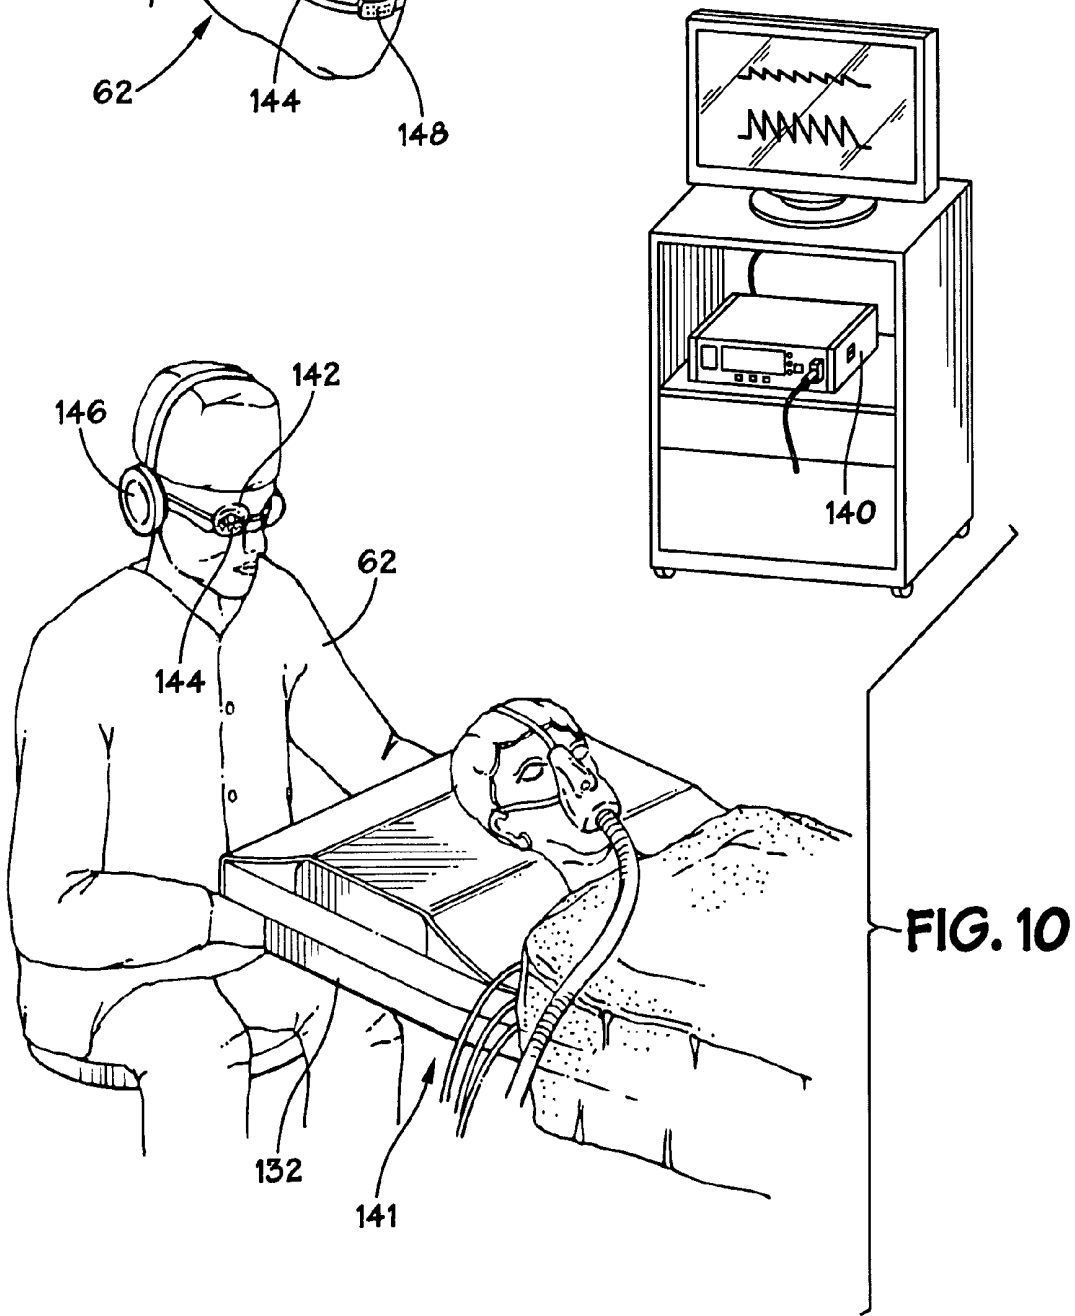
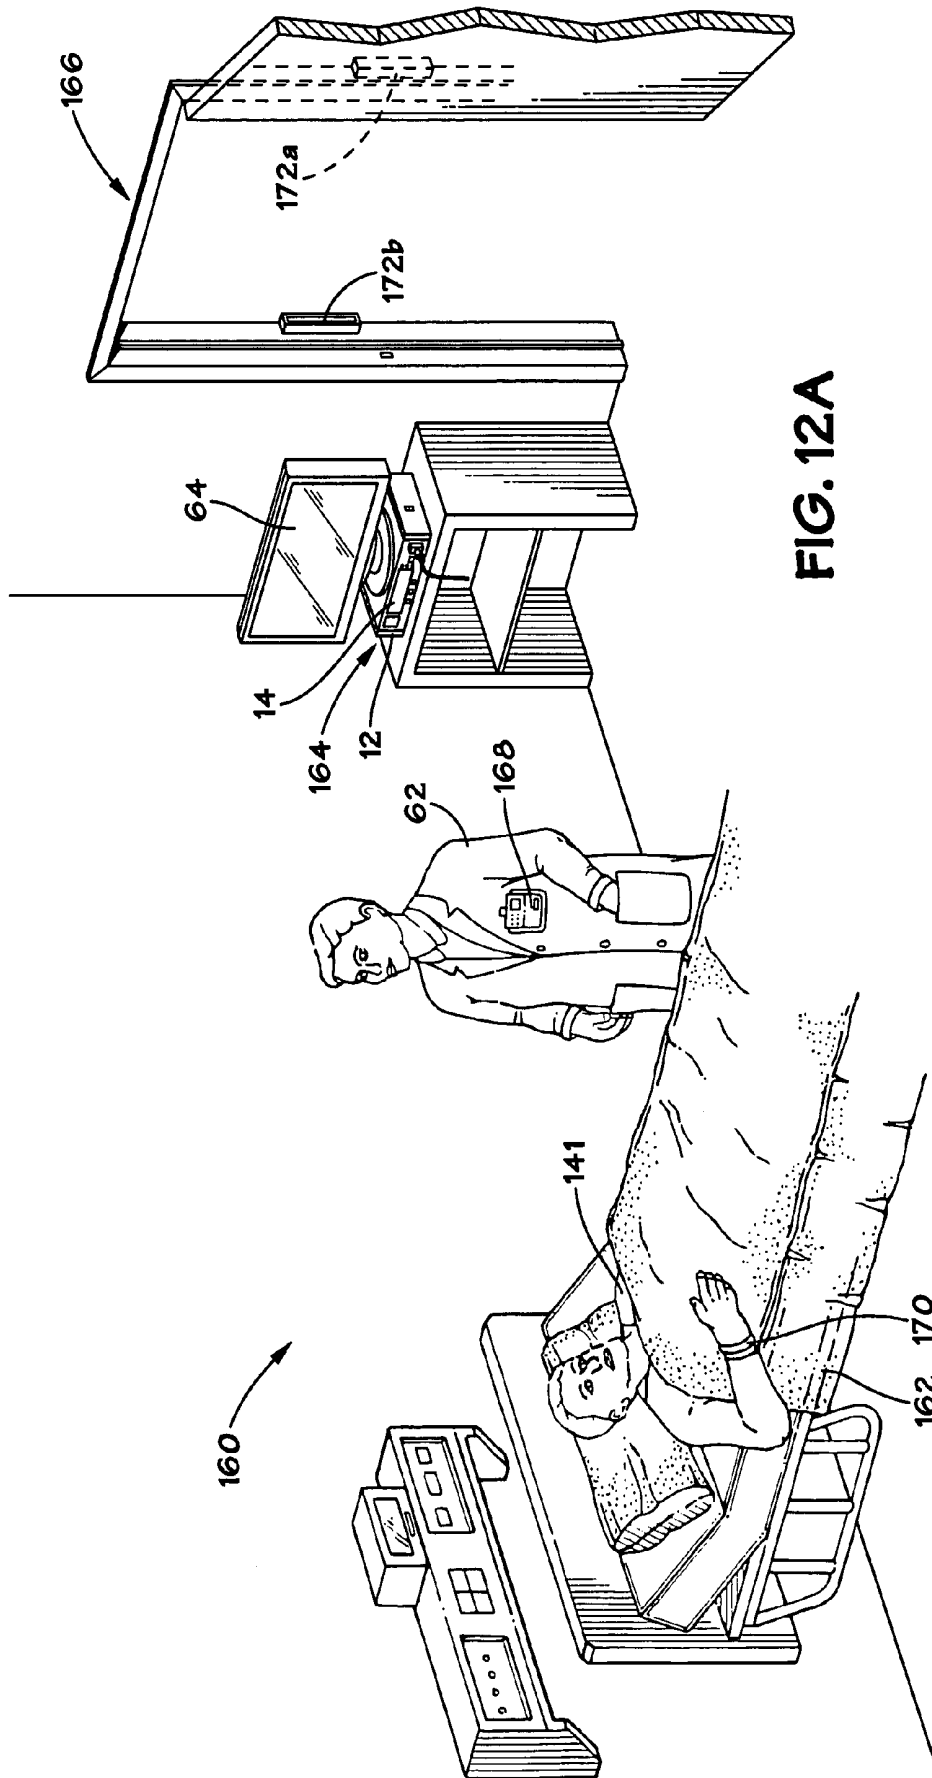


FIG. 10



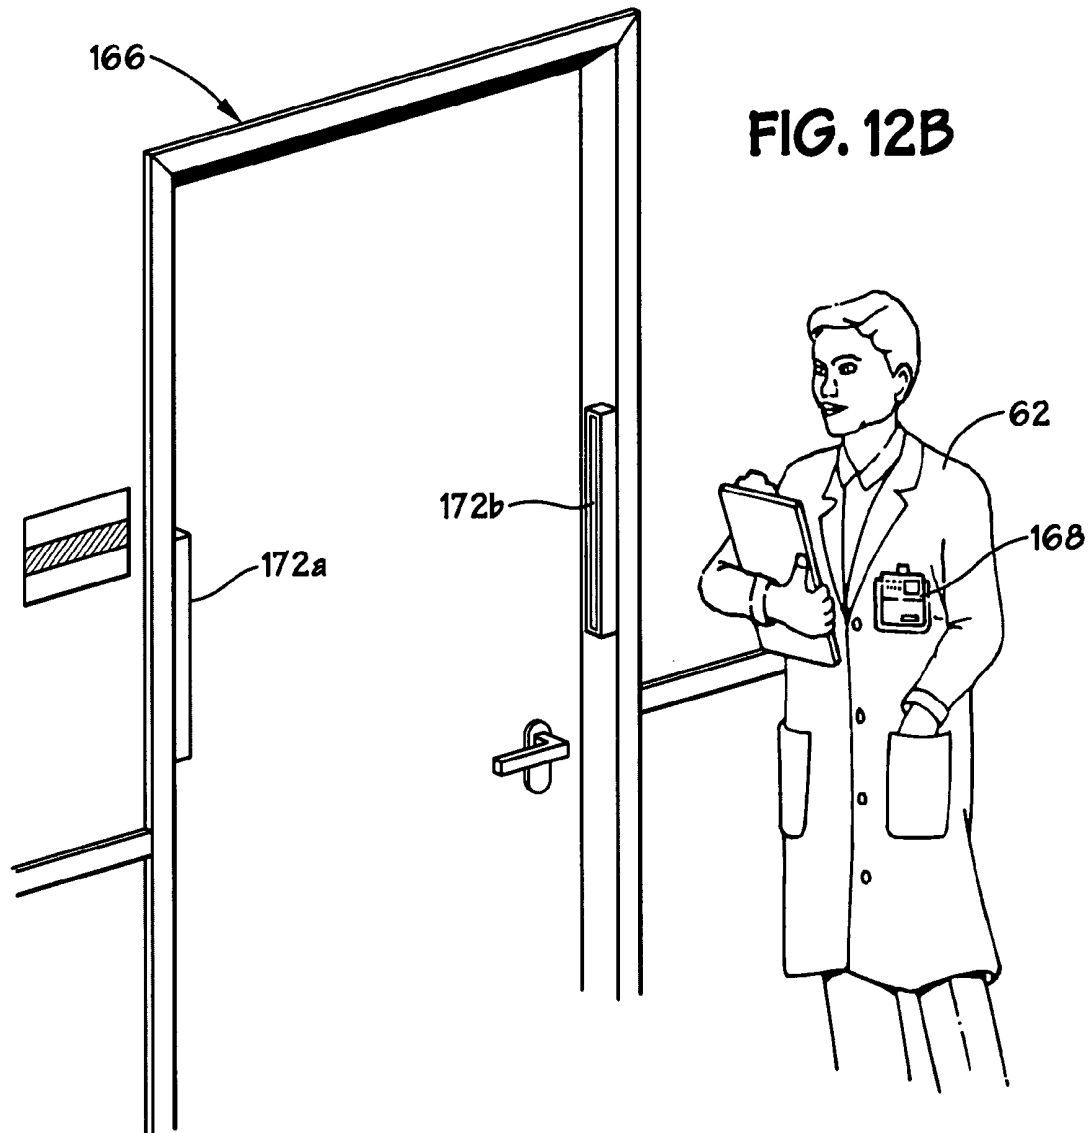


FIG. 13

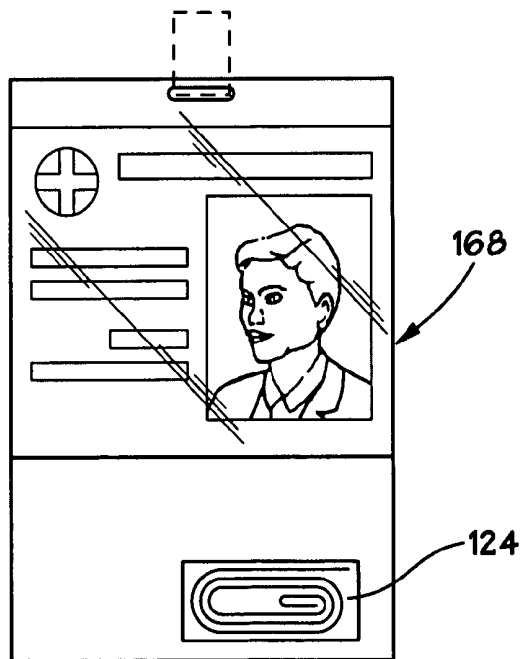
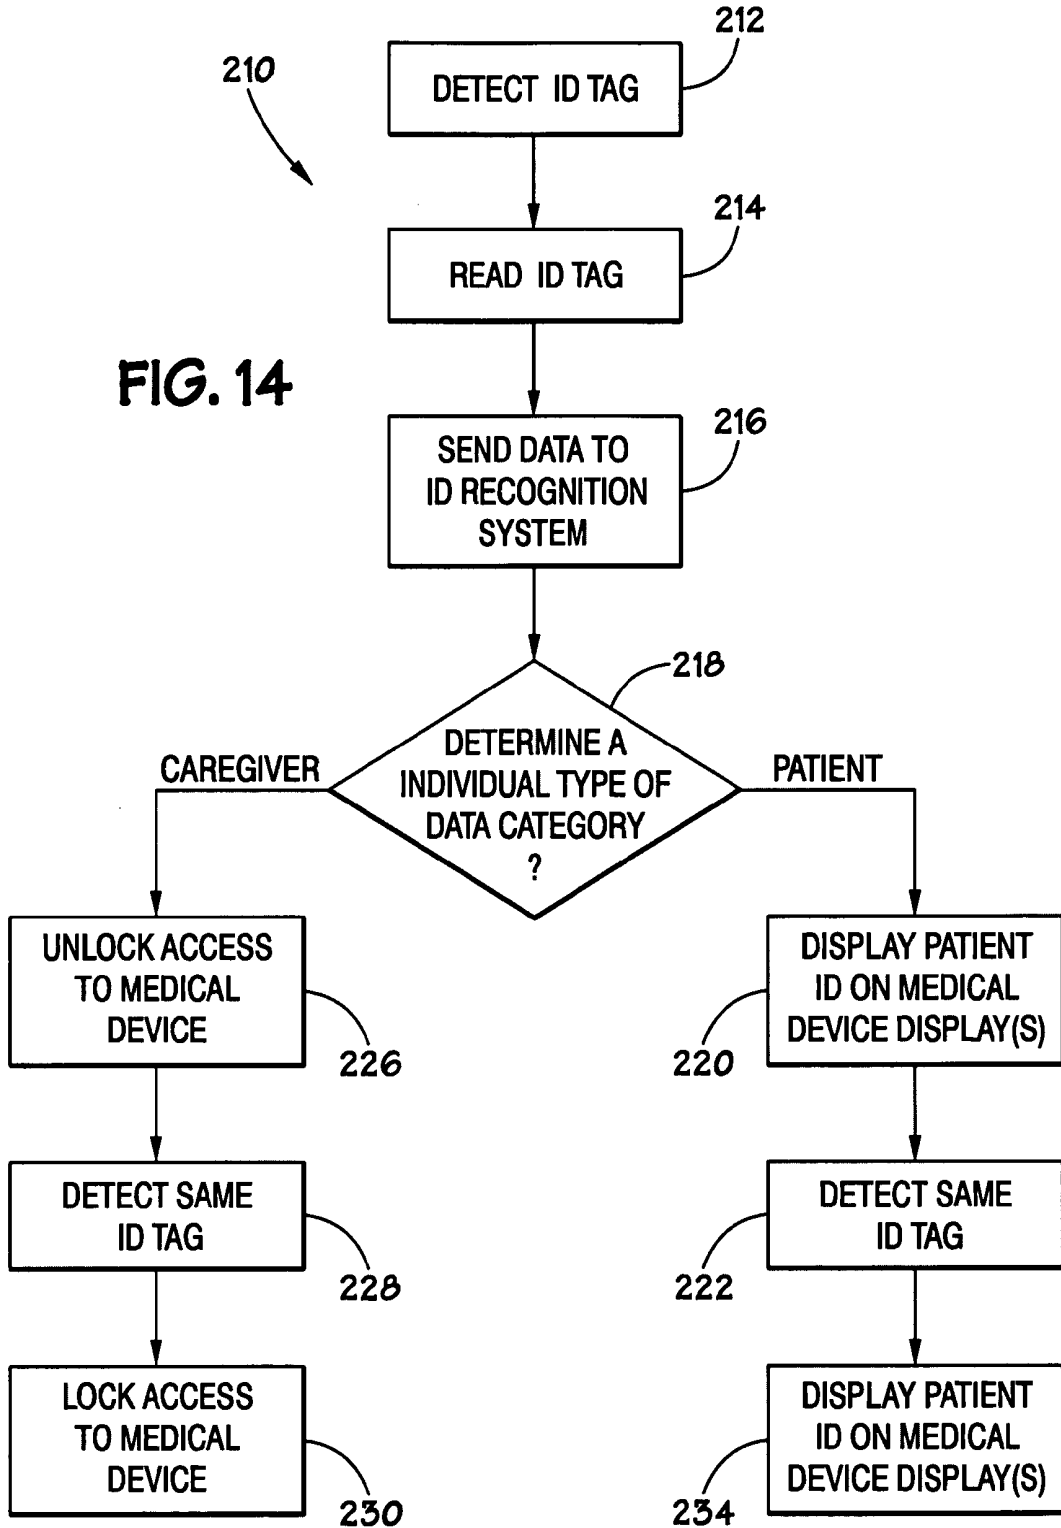


FIG. 14



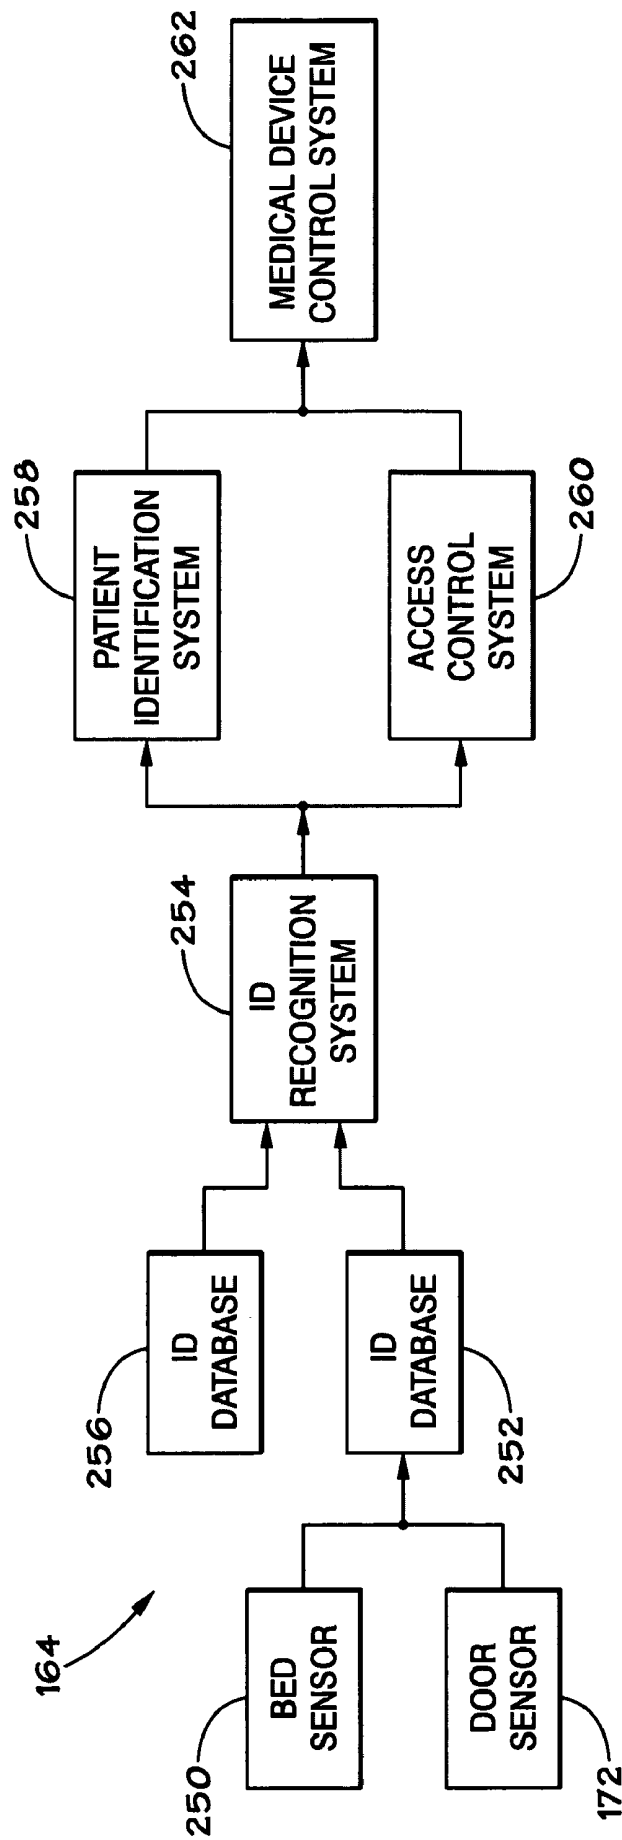


FIG. 15

USER INTERFACE AND IDENTIFICATION IN A MEDICAL DEVICE SYSTEM AND METHOD

BACKGROUND OF THE INVENTION

1. Field of the Invention

The present invention relates generally to medical devices and, more particularly, to user interfaces and identification systems integrated with medical devices.

2. Description of the Related Art

This section is intended to introduce the reader to various aspects of art that may be related to various aspects of the present invention, which are described and/or claimed below. This discussion is believed to be helpful in providing the reader with background information to facilitate a better understanding of the various aspects of the present invention. Accordingly, it should be understood that these statements are to be read in this light, and not as admissions of prior art.

In the field of medicine, doctors often desire to monitor certain physiological characteristics of their patients. Accordingly, a wide variety of devices have been developed for monitoring physiological characteristics. Such devices provide caregivers, such as doctors, nurses, and/or other health-care personnel, with the information they need to provide the best possible healthcare for their patients. As a result, such monitoring devices have become an indispensable part of modern medicine.

For example, one technique for monitoring certain physiological characteristics of a patient is commonly referred to as pulse oximetry, and the devices built based upon pulse oximetry techniques are commonly referred to as pulse oximeters. Pulse oximetry may be used to measure various blood flow characteristics, such as the blood-oxygen saturation of hemoglobin in arterial blood, the volume of individual blood pulsations supplying the tissue, and/or the rate of blood pulsations corresponding to each heartbeat of a patient.

Pulse oximeters and other medical devices are typically mounted on stands that are positioned around a patient's bed or around an operating room table. When a caregiver desires to command the medical device (e.g., program, configure, and so forth) they manipulate controls or push buttons on the monitoring device itself. The monitoring device typically provides results or responses to commands on a Liquid Crystal Diode ("LCD") screen mounted in an externally visible position within the medical device.

This conventional configuration, however, has several disadvantages. First, as described above, this conventional configuration relies upon physical contact with the monitoring device to input commands (e.g., pushing a button, turning a knob, and the like). Such physical contact, however, raises several concerns. Among these concerns are that in making contact with the medical device, the caregiver may spread illness or disease from room to room. More specifically, a caregiver may accidentally deposit germs (e.g., bacteria, viruses, and so forth) on the medical device while manipulating the device's controls. These germs may then be spread to the patient when a subsequent caregiver touches the medical device and then touches the patient. Moreover, if medical devices are moved from one patient room to another, germs transferred to the medical device via touch may be carried from one patient room to another. Even in operating rooms where medical devices are typically static, germs may be transferred onto a monitoring device during one surgery and subsequently transferred off the medical device during a later performed surgery.

Second, beyond contamination, medical devices that rely on physical contact for command input may create clutter the caregiver's workspace. For example, because the medical device must be within an arm's length of the caregiver, the medical device may crowd the caregiver-potentially even restricting free movement of the caregiver. In addition, caregivers may have difficulty manipulating controls with gloved hands. For example, it may be difficult to grasp a knob or press a small button due to the added encumbrance of a latex glove.

Third, current trends in general medical device design focus on miniaturizing overall medical device size. However, as controls which rely on physical contact must be large enough for most, if not all, caregivers to manipulate with their hands, monitoring devices that employ these types of controls are limited in their possible miniaturization. For example, even if it were possible to produce a conventional oximeter that was the size of a postage stamp, it would be difficult to control this theoretical postage stamp-sized pulse oximeter with currently available techniques.

Additionally, even as medical devices become smaller, the need for secured access remains prevalent. First, medical device alerts and alarms often require the attention of a caregiver to ensure patient health. Access to medical devices by non-caregivers could result in ineffective patient care. Second, the recently passed Health Insurance Portability and Accountability Act ("HIPPA") regulates patient privacy and security. HIPPA privacy standards require the protection of patient data from inappropriate and unauthorized disclosure or use, and HIPPA security standards require physical safeguards to protect access to equipment containing patient data. As user interfaces evolve, new methods of providing secured access will be desirable. For example, traditional entry screens can be secured using passwords. However, as device interfaces evolve to eliminate entry screens, the traditional password protection process may no longer be feasible.

In addition, conventional techniques for outputting medical data also have several potential drawbacks. For example, as described above, conventional techniques for displaying outputs rely on LCD screens mounted on the medical device itself. Besides constantly consuming power, these LCD screens must be large enough to be visually accessed by a caregiver. As such, the conventional LCD screens employed in typical medical devices also may be a barrier towards miniaturization of the medical device. Further, conventional screen-based output techniques may be impersonal to the patient and may lack configurability by the caregiver.

For at least the reasons set forth above, improved systems and methods for interfacing with and being identified by a medical device would be desirable.

BRIEF DESCRIPTION OF THE DRAWINGS

Advantages of the invention may become apparent upon reading the following detailed description and upon reference to the drawings in which:

FIG. 1 is a diagrammatical representation of a medical device including a gesture interface in accordance with one embodiment of the present invention;

FIG. 2 is a flowchart illustrating an exemplary technique for processing a gesture command in accordance with one embodiment of the present invention;

FIG. 3 is a diagrammatical representation of a medical device including another gesture interface in accordance with one embodiment of the present invention;

FIG. 4 is a diagrammatical representation of a pulse oximeter configured with a pen-based interface in accordance with one embodiment of the present invention;

FIG. 5 is a diagram of an operating room and a medical device including a laser-based interface in accordance with one embodiment of the present invention;

FIG. 6 is a diagrammatical representation of a remote control for interfacing with a medical device, in accordance with one embodiment of the present invention;

FIG. 7 is a diagrammatical representation of a remote control for interfacing with a medical device incorporated into a badge holder in accordance with one embodiment of the present invention;

FIG. 8 is a bottom view of the badge holder of FIG. 7 in accordance with one embodiment of the present invention;

FIG. 9 illustrates a patient room and a medical device configured to interface with a personal digital assistant in accordance with one embodiment of the present invention;

FIG. 10 is a diagram of a patient, a caregiver, and a medical device configured to output to a personal caregiver display in accordance with one embodiment of the present invention;

FIG. 11 is an enlarged view of the caregiver of FIG. 10 further including a microphone to interface with the medical device of FIG. 10 in accordance with one embodiment of the present invention;

FIG. 12A is a diagram of an exemplary hospital room configured to identify caregivers or patients in accordance with one embodiment of the present invention;

FIG. 12B is an enlarged view of a doorway in a hospital room configured to identify caregivers or patients in accordance with one embodiment of the present invention;

FIG. 13 is a diagram of a caregiver identifier configured to enable caregiver or patient identification in accordance with one embodiment of the present invention;

FIG. 14 is a flow chart illustrating an exemplary technique for identifying caregivers or patients in accordance with one embodiment of the present invention; and

FIG. 15 is a block diagram of an exemplary system for identifying caregivers or patients in accordance with one embodiment of the present invention.

DETAILED DESCRIPTION OF SPECIFIC EMBODIMENTS

One or more specific embodiments of the present invention will be described below. In an effort to provide a concise description of these embodiments, not all features of an actual implementation are described in the specification. It should be appreciated that in the development of any such actual implementation, as in any engineering or design project, numerous implementation-specific decisions must be made to achieve the developers' specific goals, such as compliance with system-related and business-related constraints, which may vary from one implementation to another. Moreover, it should be appreciated that such a development effort might be complex and time consuming, but would nevertheless be a routine undertaking of design, fabrication, and manufacture for those of ordinary skill having the benefit of this disclosure.

Turning initially to FIG. 1, an exemplary medical device including a gesture interface is illustrated and generally designated by a reference numeral 10. For example, in the illustrated embodiment, the medical device 10 comprises a pulse oximeter. The medical device 10 may include a main unit 12 that houses hardware and/or software configured to calculate various physiological parameters or produce various medical outputs. As illustrated, the main unit 12 may include a display 14 for displaying the calculated physiological parameters,

such as oxygen saturation or pulse rate, to a caregiver or patient. In alternate embodiments, as described in further detail below, the display 14 may be omitted from the main unit 12.

The medical device 10 may also include a sensor 16 that may be connected to a body part (e.g., finger, forehead, toe, or earlobe) of a patient or a user. The sensor 16 may be configured to emit signals or waves into the patient's or user's tissue and detect these signals or waves after dispersion and/or reflection by the tissue. For example, the sensor 16 may be configured to emit light from two or more light emitting diodes ("LEDs") into pulsatile tissue (e.g., finger, forehead, toe, or earlobe) and then detect the transmitted light with a light detector (e.g., a photodiode or photo-detector) after the light has passed through the pulsatile tissue.

As those of ordinary skill in the art will appreciate, the amount of transmitted light that passes through the tissue generally varies in accordance with a changing amount of blood constituent in the tissue and the related light absorption. On a beat-by-beat basis, the heart pumps an incremental amount of arterial blood into the pulsatile tissue, which then drains back through the venous system. The amount of light that passes through the blood-perfused tissue varies with the cardiac-induced cycling arterial blood volume. For example, when the cardiac cycle causes more light-absorbing blood to be present in the tissue, less light travels through the tissue to strike the sensor's photo-detector. These pulsatile signals allow the medical device 10 to measure signal continuation caused by the tissue's arterial blood, because light absorption from other tissues remains generally unchanged in the relevant time span.

In alternate embodiments, the sensor 16 may take other suitable forms beside the form illustrated in FIG. 1. For example, the sensor 16 may be configured to be clipped onto a finger or earlobe or may be configured to be secured with tape or another static mounting technique. The sensor 16 may be connected to the main unit 12 via a cable 18 and a connector 20. Additionally, the medical device 10 may also include a speaker 22 to broadcast alarms or alerts.

The pulse oximeter main unit 12 may also include an integral camera 24. As will be described further below, the integral camera 24 may be configured to receive gesture commands from a caregiver or user that can be processed into commands for the medical device 10. Although FIG. 1 illustrates the integral camera 24 as being located on a top surface of the main unit 12, it will be appreciated that in alternate embodiments, the integral camera 24 may be located at another suitable location on or within the main unit 12, such as the front or side facades.

In alternate embodiments, instead of an integral camera, an external camera, such as a universal serial bus ("USB") web camera, may be connected to the main unit 12 via a cable and connector. The external camera may also be wirelessly connected to the main unit 12 via radio, infrared, or optical signals. For example, wireless local area networking ("WLAN") standards, such as Wi-Fi or Bluetooth may be used. Additionally, multiple cameras may be used to reduce the effects of parallax and occlusions. The cameras may be all external cameras, all integral cameras, or a combination of external and integral cameras.

FIG. 2 illustrates a flowchart of technique 30 for processing a gesture command in accordance with one embodiment. In one embodiment, the technique 30 may be executed by the medical device 10. In other embodiments, other medical devices, such as a respirator, cardiac monitor, or multi-parameter monitoring system, may execute the technique 30.

As indicated by block 32 of FIG. 2, the technique 30 may begin by receiving a gesture. For example, the camera 24 of medical device 10 may be configured to detect hand gestures. When a caregiver performs a hand gesture in front of the camera 24 the medical device 10 first receives one or more images of the gesture (block 32) via the camera 24 and then processes the gesture (block 34). As those of ordinary skill in the art will appreciate, the camera 24 may be an analog camera that converts the gesture into an analog signal and feeds it into a digitizer board, or the camera 24 may be a digital camera that records the gesture as a digital signal. In alternate embodiments, the camera 24 may be configured to detect other gestures originating from another bodily motion or state, such as arm gestures, finger pointing, hand poses, or facial expressions.

Returning to flowchart 30, the gesture processing, as indicated by block 34, may be performed by a gesture processing system integrated into the medical device 10. For example, during processing, images captured from the gesture may be normalized, enhanced, or transformed, and then features may be extracted from the images. Next, the processed gesture may be compared to a gesture database, as indicated by block 36. The gesture database may be pre-populated or programmed with a plurality of feature combinations that are associated with commands for the medical device 10. For example, feature combinations associated with the gesture command "turn alarm off" may be associated with a command for the medical device 10 to silence an alarm. However, in alternate embodiments the feature combinations may be programmed into the gesture database using a gesture training program. Additionally, in still other embodiments, the gesture processing may be located in an external central processing unit connected to the medical device 10 via a cable or by wireless technology such as radio, infrared, or optical signals.

After the gesture is compared to a gesture database, a command associated with the gesture may be identified, as indicated by block 38. For example, a hand gesture consisting of passing a hand over the camera from right to left with the palm facing the camera may be programmed into the gesture database to correspond with the command "turn alarm off." Once the gesture is identified in the gesture database, the command may be executed, as indicated by block 40. For example, the command to turn off the alarm may be transmitted to a medical device control system which would turn off the alarm.

Turning next to FIG. 3, an exemplary medical device including another gesture interface is illustrated and generally designated by a reference numeral 50. In addition to the main unit 12, the display 14, and the cable 18 for connection to the sensor 16 (not shown), the medical device 50, which may be a pulse oximeter, may include a tracking glove 52. As will be described further below, the tracking glove 52 may be configured to receive gesture commands from a caregiver 62 or user. As with the gesture command described in regard to FIG. 2, these gesture commands can be processed into commands for the medical device 50.

The tracking glove 52 may include a battery pack 56 connected to the tracking glove 52 via a cable. Although the battery pack is worn on the forearm in this embodiment, in alternative embodiments the battery pack may be located in other locations such as around the waist of the caregiver 62. Additionally, in other embodiments, the tracking glove 52 may be replaced by another tracking device such as a finger sensor. In yet another embodiment, the tracking glove 52 may have a light emitting diode ("LED") located on the glove and a software programmable switch to permit other functions to

be directly programmed into the glove. For example, a button may be included on the glove that can be programmed so that when a caregiver presses the button an alarm on the medical device 50 is silenced.

In one embodiment, the caregiver 62 may make hand gestures while wearing the tracking glove 52. The tracking glove 52 may then record the movement (i.e., the gesture) and transmit the gesture to the medical device 50 via a wireless receiver 60 connected to the medical device 50. In alternate embodiments, the tracking glove 52 may communicate with a wireless receiver integrated into the main unit 12 or may be connected to the medical device 50 via a cable such as a fiber optic cable or a serial cable.

Similar to the medical device 10, the medical device 50 may be configured to interpret the tracking glove 52 movement and execute a command associated with the movement. For example, a hand movement, such as making a fist, may be associated with the command "turn alarm off." As such, when the caregiver 62 makes a fist while wearing the tracking glove 52, the medical device 50 may interpret the movement and sends a signal to the medical device 50 to silence an alarm.

In addition, in some embodiments, the medical device 50 may include calibration software which may allow a caregiver 62 to program movement combinations into the gesture database within the medical device. Additionally, in other embodiments, the gesture database may be located in an external central processing unit connected to the medical device 50 via a cable or by wireless technology such as radio, infrared, or optical signals.

Turning next to FIG. 4, an exemplary medical device configured with a pen-based interface is illustrated and generally designated by the reference numeral 70. In addition to the main unit 12, the display 14, and the cable 18 for connection to the sensor 16 (not shown), the medical device 70 may include a stylus 72. As will be described further below, the caregiver 62 may use the stylus 72 to control the medical device 70.

In one embodiment, the medical device 70 may have a separate display screen 74 connected to the main unit 12 via a cable or wireless means such as radio, infrared, or optical signals. The display screen 74 may be a touch screen with selection boxes corresponding to medical device commands. For example, when the caregiver 62 touches the stylus 72 to the selection box corresponding to "turn alarm off," the display screen 74 may transmit a signal to the main unit 12 which silences the alarm. In an alternate embodiment, the caregiver 62 may touch the screen directly without using the stylus. In still other embodiments, the stylus 72 may be used to touch selection boxes directly on the medical device 70, and the separate display 74 may be omitted.

In yet another embodiment, the stylus 72 may be used to draw symbols or characters representative of medical device commands on the display screen 74. In the embodiment illustrated in FIG. 4, the medical device 70 main unit 12 may include symbol recognition software which recognizes the symbols drawn on the display 74 and executes commands corresponding to the recognized symbols. For example, the letter "L" may be associated with the command "lower alarm limit." When a caregiver 62 draws an "L" on the display 74 the symbol recognition software may interpret the symbol, and the medical device 70 may lower the alarm limit by a predetermined amount. The symbol recognition software may be pre-populated or programmed with a plurality of symbols associated with medical device commands. In alternate embodiments, the symbol recognition software may include a calibration program to allow the caregiver 62 to associate symbols with medical device commands.

In still other embodiments, the stylus **72** may include an ultrasound transmitter. In this embodiment, the ultrasound transmitter may be configured to transmit movements of the stylus **72** back to the medical device **70** or another suitable receiver. For example, in one embodiment, the movements of the stylus **72** may be tracked by one or more sensors positioned around an operating room and coupled to the medical device **70**.

Turning now to FIG. **5**, an exemplary operating room and a medical device **80** including a laser-based interface in accordance with one embodiment is illustrated. In addition to the main unit **12**, the display **14**, and the cable **18** for connection to the sensor **16** (not shown), the medical device **80** may include a laser wand **84** and/or the display **64**. As will be described further below, the caregiver **62** may use the laser wand **84** to control the medical device **80**. It will be appreciated, however, that the operating room shown in FIG. **5** is merely one possible application of the medical device **80**. Accordingly, the medical device **80** may be employed in patients' rooms, doctors' offices, or other suitable locations. Moreover, it will also be appreciated that the medical devices described in regard to FIGS. **1**, **3**, and **4**, as well as those described below, may be employed in each of these locations as well.

In one embodiment, the caregiver **62** may be able to use the laser wand **84** to position a cursor on the display **64**. For example, the caregiver **62** may focus a laser pointer dot on the display **64**. As one skilled in the art will appreciate, a location of a laser pointer dot can be translated to the cursor position on a display **64**. In alternate embodiments, the laser pointer dot may alternatively be focused on the display **14**. In one embodiment, the display **64** (or the display **14**) may employ a camera, such as the camera **24** discussed above, to detect the laser pointer dot. In various embodiments, the camera may be internal to the display **64** or may be externally connected to it via a cable or wirelessly. However, it will be appreciated that in still other embodiments, other suitable laser pointer detection techniques may be employed.

In one embodiment, the display **64** may contain a plurality of selection boxes or regions corresponding to commands for medical device **80**. For example, the display **64** may contain a selection box for the command "turn alarm off." When the caregiver **62** focuses the laser pointer dot on one of the selection boxes for a minimum period of time, the software within the medical device **80** may first position the cursor at the selection box location. As the caregiver **62** continues to focus the laser pointer dot on the same selection box, the software within the medical device **80** may then select the box and execute the command associated with the selection box. In this example, the software may then silence the alarm.

In other embodiments, the laser wand **84** may have an integrated selection button. Once the caregiver **62** has positioned the cursor on the selection box, the caregiver **62** may then push the button to select the box and execute the pulse oximeter command associated with the box. The integrated selection button may employ standard remote control technology, such as transmitting an infrared signal to an infrared receiver integrated into the medical device **80**. In alternate embodiments, an external receiver connected to the medical device **80** via a cable may be used.

As shown in FIG. **5**, the laser wand **84** may allow the medical device **80** to be controlled from a distance by the caregiver **62**. Consequently, the medical device **80** may be placed at a location away from the patient **82** allowing the caregivers **62** more room to maneuver. In some embodiments, each of the caregivers **62** may have their own laser wand **84** to further reduce the risks of cross-contamination.

In another embodiment, the medical device **80** may be controlled using a remote control style wand **90**, as illustrated in FIG. **6**. The wand **90** may contain a plurality of buttons each programmed to correspond to one or more medical device commands. For example, the buttons may be programmed as follows: the button labeled "1" **96** may be programmed to correspond to the command "Raise Alarm Limit;" the button "2" **98** may be programmed to correspond to the command "Lower Alarm Limit;" the button "3" **100** may be programmed to correspond to the command "Reset Alarm Limits;" and the button "4" **102** may be programmed to correspond to the command "Turn Alarm Off." It will be appreciated that these commands are exemplary. Although the buttons **96-102** are shown in FIG. **6** as being labeled with numbers and of certain shapes and sizes, in other embodiments, the buttons may be customized with different shapes, sizes, and labels. Additionally, the number of buttons present on the wand **90** may vary. The wand **90** also may contain a pen-style clip for attaching the wand **90** to the caregiver **62**.

In the above-described embodiment, the wand **90** may contain a light emitting diode ("LED") **92** that transmits light pulses or infrared signals corresponding to a medical device command. For example, when a caregiver **62** presses button "1" **96**, an integrated circuit within the wand **90** may send a command to the LED **92**. The LED **92** may then send out a signal corresponding to this command. A receiver integrated into the medical device may receive the signal and respond by raising the alarm limit by a predetermined unit.

In other embodiments, the LED transmitter **92** may alternatively be replaced by a radio frequency ("rf") transmitter. In such an embodiment, the medical device **80** may include an integrated rf receiver. Additionally, in alternate embodiments, the rf transmitter may employ the Bluetooth radio frequency standard or other suitable standard.

The technology of the wand **90** may also be incorporated in other packages. For example, in one alternate embodiment, it may be incorporated into a badge holder, as illustrated in FIG. **7**. The badge holder **110**, in addition to holding a caregiver's badge **112**, may also contain the several command buttons **96-102**. As shown in the bottom view of FIG. **8**, the badge holder **110** may also contain the transmitter **92** on the bottom of the badge holder **110**. In alternate embodiments the transmitter **92** may be located on another facade such as the top, front, or sides of the badge holder **110**. Additionally, in still other alternate embodiments, the control buttons **96-102** may be of various shapes and sizes and be located on other facades of the badge holder **110**.

Turning now to FIG. **9**, an exemplary patient's room **131** and medical device **130** configured to interface with a personal data assistant ("PDA") **134** is illustrated. In addition to the main unit **12**, the display **14**, and the cable **18** for connection to the sensor **16** (not shown), the medical device **130** may include a PDA **134**. As will be described further below, the caregiver **62** may use the PDA **134** to control the medical device **130**. For example, the PDA **134** may be configured to present the caregiver **62** with one or more buttons or selectable locations on its screen that correspond to medical device controls or commands. Accordingly, when the caregiver **62** selects one of these controls or commands, the PDA **134** may be configured to transmit this control or command back to the medical device **130**, which may subsequently execute the control or command. For example, the PDA **134** may be configured to generate a volume control display for the medical device **130**. Upon accessing this volume display on the PDA **134**, the caregiver may adjust the volume of the medical device **130** up or down.

Advantageously, the PDA 134 enables the caregiver 62 to control medical device 130 without physically touching or manipulating it. In addition, the PDA 134 may also supplement a display on the medical device 130. In particular, the PDA 134 may be configured to mirror or reproduce some or all of the contents displayed on the medical device's 130 internal display. In this way, the medical device 130 could advantageously be located away from the patient bed 132 or the caregiver 62, possibly even out of sight, as the inputs and outputs to the medical device 130 can be supported by the PDA 134.

Furthermore, the PDA 134 may be configured to interface with a plurality of medical devices 130 in a plurality of patient rooms 131. For example, a hospital may issue each of each caregivers 62 their own PDA 134, which they may use to access and/or control medical devices within a plurality of patient rooms. More specifically, the caregiver 62 may use their PDA 134 to access one or more medical devices within a first patient's room and then use the same PDA 134 to access medical devices within a subsequent patient's room. In this way, the caregiver 62 may access and/or control medical devices within a plurality of patient rooms without ever touching the actual medical devices—substantially decreasing the chances of cross-contamination.

As described above, the PDA 134 may supplement or replace the internal screen on the medical device 130. In other words, the information that would otherwise be displayed on the medical device's 130 internal screen would be alternatively displayed on the PDA 134. Although this embodiment has several advantages (as described above) the caregiver 62 would have to periodically hold the PDA 134 in one or both of their hands. As will be appreciated, however, there may be a variety of situations where the caregiver 62 may desire free use of both of their hands while still being able to access and/or control medical devices. Accordingly, FIG. 10 is a diagram of a patient 141, the caregiver 62, and a medical device 140 configured to output to a personal caregiver display 142 in accordance with one embodiment.

As illustrated in FIG. 10 and highlighted in an enlarged view in FIG. 11, the caregiver personal display 142 may include a pair of glasses or other suitable wearable optics or eyewear (e.g., a monocular) which may be configured to display outputs from the medical device 140. In one embodiment, the caregiver personal display 142 may be configured to create a transparent or semi-transparent image that the caregiver 62 may be able to view while still being able to see the patient 141. For example, as illustrated in FIGS. 10 and 11, the caregiver personal display may include a pair of glasses with an integral liquid crystal display ("LCD") that may be configured to display a pleth signal 144 while still enabling the caregiver 62 to see the patient 141. In this case, the caregiver personal display 142 effectively creates a "heads-up" display for the caregiver 62, allowing them to see the pleth signal 144 or other suitable medical information as if it were floating in front of them.

It will be appreciated, however, that the illustrated caregiver personal display 142 is merely one potential embodiment of a suitable caregiver personal display. Accordingly, in other embodiments, other types of displays may be employed. For example, in one embodiment, the caregiver personal display may be a video display mounted on a pair of glasses or other mount, which the caregiver 62 may view by shifting his or her focus towards the display. Although medical information in this embodiment may not appear transparent to the caregiver 62, the caregiver 62 may still be able to

readily access information from the medical device 140 without having the medical device 140 within visual range of the caregiver 62.

As further illustrated in FIGS. 10 and 11, the caregiver personal display may also include a speaker 146 to enable the caregiver 62 to hear alarms or alerts from the medical device 140. Advantageously, the speaker 146 enables the caregiver 62, who is monitoring medical device 140, to hear alerts or alarms without the alarms or alerts bothering other caregiver 62, who may be focused on other activities. In addition, as illustrated in FIG. 11, the caregiver personal display 142 may also include a microphone 148 to enable voice control of the medical device 140, as further described in commonly assigned U.S. patent application Ser. No. 11/540,457 entitled SYSTEM AND METHOD FOR INTEGRATING VOICE WITH A MEDICAL DEVICE and filed on Sep. 29, 2006, which is hereby incorporated by reference.

As described above, secured access and/or patient privacy are both concerns in medical device design. In particular, as medical devices become an increasing vital component of medical treatment, it is important to ensure that only authorized caregivers are able to control these devices. For example, it could be potentially dangerous to a patient if the patient or a patient's guest were able to turn off or adjust a medical device, such as a respirator, a pulse oximeter, a heart/lung machine, and so-forth. Moreover, beyond safety concerns, modern medical devices also typically store a plurality of private personal information regarding the patient, such as social security numbers, addresses, and so-forth. In an age of increasing identity-based crimes, it is advantageous for medical devices to be able to restrict access to this information to approved individuals.

Accordingly, FIG. 12A is a diagram of an exemplary patient room 160 configured to identify caregivers or patients in accordance with one embodiment. As illustrated in FIG. 12A, the hospital room 160 may include a patient bed 162, a medical device 164, and a doorway 166. Moreover, as also illustrated in FIG. 12A, the hospital room 160 may also include the patient 141 and the caregiver 62. As illustrated, the patient 141 may be located in the bed 162 with the caregiver 62 positioned over the patient 141 and in general proximity with the medical device 164.

As illustrated in FIG. 12A, in an embodiment where the medical device 164 is a pulse oximeter, the medical device 164 may include the main unit 12, the display 14, and/or the display 64. Moreover, the medical device 164 may be configured to work in conjunction with an identification ("ID") tag, such as a caregiver ID 168 and/or a patient ID 170 to identify caregivers and/or patients within the hospital room 160. More specifically, in one embodiment, the medical device 164 may be coupled to door sensors 172A and 172B, which are located in close proximity to the door 166 and configured to detect when the caregiver ID 168 and/or the patient ID 170 pass through the doorway 166.

For example, as illustrated in FIG. 12B, which illustrates an enlarged view of the doorway 166 in accordance with one embodiment, the door sensors 172a and 172b may be configured to detect when the caregiver ID passes through the doorway 166 (e.g., when a caregiver enters or exits the patient room 160). Similarly, the door sensors 172a and 172b may be configured to detect when the patient ID 170 passes through the doorway 166 (e.g., the patient 141 walks or is pushed through the doorway 166). In one embodiment, the door sensors 172a and 172b may include radio frequency ("rf") sensors configured to detect an rf transmitter within the caregiver ID 168 and/or the patient ID 170. For example, FIG. 13 illustrates one embodiment of the caregiver ID 168 including

an rf ID tag **174**. As will be appreciated the rf ID tag **174** may be a passive rf ID configured to receive transmissions from the door sensors **172a** or **172b** and to broadcast an identifying signal in response. The door sensors **172a** or **172b** may detect this identifying signal, and, thus, identify/detect the entry or exit of the caregiver **62** and/or the patient **141**.

It will be appreciated, however, that other suitable identification technologies may be employed. For example, in one embodiment, the caregiver ID may be an active ID (e.g., a Bluetooth enabled cell phone). Furthermore, in still other embodiments, the door sensors **172a** and **172b** may be located elsewhere besides the doors. For example, the sensors **172a** and **172b** may be located in the ceiling of the patient room **160** and configured to detect when the sensors **168** and/or **170** enter are located in the patient room **160**.

Advantageously, medical device **164** may be configured to utilize this detection information to manage access to its controls and/or to identify the patient **141** for administrative or record keeping purposes. For example, FIG. **14** is a flow chart illustrating an exemplary technique **210** for identifying caregivers or patients in accordance with one embodiment. For ease of description, the technique **210** will be described in conjunction with FIG. **15** which illustrates a block diagram of the medical device **164** in accordance with one embodiment.

As illustrated by block **212** of FIG. **14**, the technique **210** may begin by detecting an ID tag. For example, in one embodiment, the door sensors **172** may detect the caregiver ID **168** or the patient ID **170**. In another embodiment, the medical device **164** may alternatively or additionally include a bed sensor **250** to detect the ID tag. More specifically, the bed sensor **250** may be mounted on the patient bed **162** and configured to detect the patient ID **170**. The bed sensor **250** may be particularly advantageous in hospital rooms including multiple patient beds **162**, as the door sensors **172** may not be able to determine which of the plurality of patient beds **162** a particular patient is occupying. Moreover, the bed sensor **250** may also be configured to detect the patient ID **170** and to communicate patient identification information to the medical device **164**, as set forth in further detail below.

Next, the technique **210** may include reading the detected ID tag, as indicated in block **214**. For example, in one embodiment, an ID reader **252** may be configured to read the identity information from the caregiver ID **168** and/or the patient ID **170**. Next, the technique **210** may include sending the identity information from the ID tag to an ID recognition system, as indicated in block **216**. For example, in one embodiment, the ID reader **252** may transmit the identity information to an ID recognition system **254**.

Next, the technique **210** may include determining an individual type of the detected ID tag, as indicated by block **218**. For example, in the illustrated embodiment of the technique **210**, the technique may include determining whether the detected ID tag corresponds to the caregiver **62** or the patient **141**. In one embodiment, the ID recognition system **254** may make this determination based on an ID database **256**, which includes information regarding a plurality of ID tags and the individual type corresponding to each of the plurality of ID tags. Alternatively, the individual type may be encoded on the caregiver ID **168** or the patient ID **170** and communicated to the ID recognition system **254** via the door sensor **172** and/or the bed sensor **250**. Although the technique **210** is illustrated in FIG. **14** as including two branches, one for caregivers and one for patients, it will be appreciated that this is merely exemplary. As such, in alternate embodiments, the technique **210** may include multiple branches for various suitable individual types. For example, the technique **210** may respond

differently to different types of caregivers, such as doctors, nurses, orderlies, and so-forth.

Returning now to FIG. **14**, if the ID tag corresponds to a caregiver, the technique **210** may next include unlocking access to the medical device at an appropriate permissions level. For example, in one embodiment, an access control system in the medical device **164** may be configured to unlock the medical device **164** and allow the medical device control system **262** to execute instructions and/or commands commensurate with the permission level of the caregiver **62**.

The technique **210** may then continue to allow the caregiver **62** to execute commands until the same ID tag is again detected by the door sensor **172** or the bed sensor **250**, as indicated by block **228** (i.e., the caregiver leaves the patient room **160**). Alternatively, the door sensors **172a** and **172b** may be configured to detect when the caregiver ID **168** leaves the proximity of the sensor. In this embodiment, rather than detecting when the caregiver ID **168** crosses their threshold, the door sensors **172a** and **172b** may be configured to detect when the caregiver ID **168** is located within a certain distance of the door sensors **172a** and **172b** (i.e., the caregiver is located in the patient room **160**).

Upon detecting the exit of the caregiver **62**, the technique **210** may include locking further access to the medical device **164** to prevent the patient **141** or other unauthorized individuals from adjusting the medical device **164** in the absence of the caregiver **162** (block **230**). In this way, the technique **210** enables the medical device **164** or other suitable medical device automatically unlock when the caregiver **62** enters the patient room **160**, to accept commands freely from the caregiver **62** while they are in the room, and then to relock automatically when the caregiver **62** leaves the patient room. Moreover, in one embodiment, the medical device **164** may be configured to record which caregiver **62** gave which commands to the medical device **164**, because each caregiver in a hospital may be assigned a unique caregiver ID **168**. In this way, it may be possible for a hospital to reconstruct patient treatment history, if desired.

Returning again to block **218** of FIG. **14**, if the individual type is determined to be a patient, the technique **210** may include displaying a patient ID on a display of the medical device **164**, as indicated by block **220**. In one embodiment, a patient identification system **258** within the medical device **164** may be configured to display the patient ID on the display **14**. Furthermore, the medical device **164** may also be configured to annotate any patient medical data subsequently stored by the medical device **164** with the patient information.

Next, if the same ID tag is detected again (or contact with the ID tag is lost, as described above), the technique **210** may include clearing the patient information from the medical device **164**, as indicated by blocks **222** and **224**. Accordingly, the medical device **164** may be able to automatically identify the identity of patients being monitored or treated without the need for caregivers to manually enter this information into the medical device **164**. Advantageously, this reduces the chances of cross-contamination and automates one additional caregiver function.

While the invention may be susceptible to various modifications and alternative forms, specific embodiments have been shown by way of example in the drawings and have been described in detail herein. However, it should be understood that the invention is not intended to be limited to the particular forms disclosed. Rather, the invention is to cover all modifications, equivalents, and alternatives falling within the spirit and scope of the invention as defined by the following appended claims. Indeed, the present techniques may not

13

only be applied to pulse oximeters, but also to other suitable medical devices, such as respirators, ventilators, EEGs, EKGs, and so-forth.

What is claimed is:

1. A method for accessing a pulse oximeter, the method comprising:

reading identification information from an identification tag;

electronically determining if a person corresponding to the identification information has been approved to access the pulse oximeter; and

if the person has been approved, granting access to the pulse oximeter, wherein granting access comprises permitting the person to execute a first command of the pulse oximeter, but denying the person to execute a second command of the pulse oximeter if the person is not a doctor.

2. The method, as set forth in claim 1, comprising determining a permission level associated with the person.

3. The method, as set forth in claim 2, wherein granting the access comprises granting access at the determined permission level.

4. The method, as set forth in claim 1, wherein the reading comprises detecting a radio frequency signal.

5. The method, as set forth in claim 1, wherein the reading comprises detecting a wireless communication protocol signal.

6. The method, as set forth in claim 1, wherein the reading comprises detecting the identification tag with a door sensor.

7. The method, as set forth in claim 1, comprising determining whether the identification tag corresponds to a caregiver or corresponds to a patient.

8. The method, as set forth in claim 7, comprising reading patient data from the identification tag if the identification tag corresponds to a patient.

14

9. The method of claim 7, wherein granting access comprises permitting the caregiver to adjust patient-specific settings of the pulse oximeter if the caregiver is a doctor.

10. A medical device comprising:

a reader configured to read identification information from an identification tag;

a recognition system configured to determine if a person corresponding to the identification information has been approved to access the medical device;

an access control system configured to grant access to the medical device if the person has been approved to access the medical device, wherein granting access comprises permitting the person to execute a first command of the medical monitoring device, but denying the person to execute a second command of the medical monitoring device if the person is not a doctor; and

a pulse oximetry sensor configured to monitor a physiological characteristic.

11. The medical device, as set forth in claim 10, wherein the reader comprises a door sensor.

12. The medical device, as set forth in claim 11, wherein the door sensor is configured to be mounted in a doorway of a hospital room.

13. The medical device, as set forth in claim 10, wherein the reader comprises a proximity sensor.

14. The medical device, as set forth in claim 10, wherein the reader is configured to read the identification information over a wireless communication protocol signal.

15. The medical device, as set forth in claim 10 comprising the identification tag.

16. The medical device, as set forth in claim 10 wherein the access control system is configured to grant access to the medical device based on a permission level associated with the identification information.

17. The medical device, as set forth in claim 10, comprising a sensor configured to detect the identification tag.

* * * * *

专利名称(译)	用户界面和医疗设备系统和方法中的识别		
公开(公告)号	US7706896	公开(公告)日	2010-04-27
申请号	US11/540385	申请日	2006-09-29
[标]申请(专利权)人(译)	内尔科尔普里坦贝内特公司		
申请(专利权)人(译)	NELLCOR PURITAN BENNETT LLC		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	MUSIC DOUG EGHBAL DARIUS VARGAS STEVE		
发明人	MUSIC, DOUG EGHBAL, DARIUS VARGAS, STEVE		
IPC分类号	G06F3/00 A61B5/00 G05B11/01 G06F7/04 G05B15/00 G06F17/00		
CPC分类号	G06F21/316 G06F21/35 G06F19/3406 G06F2221/2149 G06F2221/2113 G16H40/63		
其他公开文献	US20080189783A1		
外部链接	Espacenet USPTO		

摘要(译)

提供了用于医疗设备中的用户界面和识别的系统和方法。更具体地，在一个实施例中，提供了一种用于访问医疗设备的方法，该方法包括检测识别标签，从识别标签读取识别信息，确定对应于识别信息的人是否已被批准访问医疗设备，如果该人已被批准，则允许访问医疗设备。

