



US008286088B2

(12) **United States Patent**
Shaffer et al.

(10) **Patent No.:** **US 8,286,088 B2**
(45) **Date of Patent:** ***Oct. 9, 2012**

(54) **PATIENT MEDICAL PARAMETER TREND
INDICATIVE USER INTERFACE DISPLAY
SYSTEM**

(56) **References Cited**

(75) Inventors: **Judith Shaffer**, Orchard Park, NY (US);
Mark Penny, Salem, MA (US); **Rand J.
Monteleone**, Acton, MA (US); **Amy M.
Manetta**, North Billerica, MA (US);
Jolyn Rutledge, Amesbury, MA (US)

U.S. PATENT DOCUMENTS
4,878,175 A 10/1989 Norden-Paul et al. ... 364/413.01
(Continued)

FOREIGN PATENT DOCUMENTS
WO WO 02/32036 A2 4/2002

(73) Assignee: **Draeger Medical Systems, Inc.**,
Andover, MA (US)

OTHER PUBLICATIONS
New Flowsheet Solution From McKesson Improves Nurse Effi-
ciency, Enhances Medication Safety; Oct. 23, 2002. Horizon Expert
Documentation Sets New Standard for "Smart" Workflow Technol-
ogy Business/Medical Editors. Business Wire; New York.*
(Continued)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 2736 days.

This patent is subject to a terminal dis-
claimer.

Primary Examiner — Jordany Nunez
(74) *Attorney, Agent, or Firm* — Jack Schwartz and
Associates, PLLC

(21) Appl. No.: **10/411,950**

(57) **ABSTRACT**

(22) Filed: **Apr. 11, 2003**

(65) **Prior Publication Data**

US 2004/0002874 A1 Jan. 1, 2004

Related U.S. Application Data

(60) Provisional application No. 60/374,908, filed on Apr.
23, 2002, provisional application No. 60/413,301,
filed on Sep. 25, 2002.

A system according to invention principles advantageously
automatically displays a parameter value within the closest
Flowsheet parameter acquisition time interval column. A user
interface system provides patient medical parameter data for
trend indicative display covering a time period comprising
user selectable acquisition time intervals. The system
includes an acquisition processor for acquiring, from a patient
monitoring device, data representing a patient parameter
comprising a plurality of data values at a corresponding plu-
rality of different times within multiple user selectable patient
parameter acquisition intervals of a time period. The data
processor determines for a particular user selectable acquisi-
tion time interval a patient parameter data value closest in
time to a center time point of the particular user selected
acquisition time interval and excludes other patient parameter
data values acquired within the particular user selectable
acquisition time interval. A generator generates data repre-
senting an image showing a trend indicative display of the
patient parameter including the determined patient parameter
data value associated with the particular user selectable
acquisition time interval and omits the excluded data values.


(51) **Int. Cl.**
G06F 3/048 (2006.01)
G06F 17/21 (2006.01)
G06F 17/00 (2006.01)
G06Q 10/00 (2012.01)
G08B 23/00 (2006.01)

(52) **U.S. Cl.** **715/764; 705/2; 705/3; 340/573.1**

(58) **Field of Classification Search** **717/109;**
705/9, 3, 2; 715/764; 340/573.1

See application file for complete search history.

15 Claims, 13 Drawing Sheets

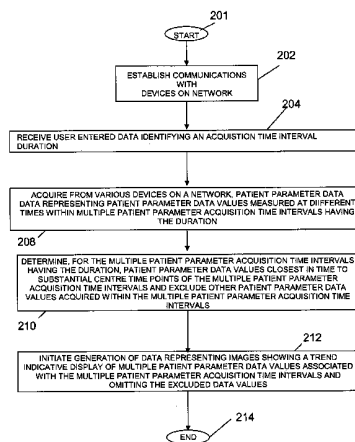

U.S. PATENT DOCUMENTS

5,072,383	A	12/1991	Brimm et al.	364/413.02
5,077,666	A	12/1991	Brimm et al.	364/413.02
5,247,611	A	9/1993	Norden-Paul et al.	395/161
5,253,362	A	10/1993	Nolan et al.	395/600
5,301,319	A	4/1994	Thurman et al.	395/600
5,325,478	A	6/1994	Shelton et al.	395/148
5,468,222	A	11/1995	Altchuler	604/49
5,546,580	A	8/1996	Seliger et al.	305/600
5,592,945	A	1/1997	Fiedler	128/710
5,682,526	A	10/1997	Smokoff et al.	395/615
5,697,959	A *	12/1997	Poore	607/32
5,715,451	A *	2/1998	Marlin	707/104.1
5,812,983	A	9/1998	Kumagai	705/3
5,942,986	A	8/1999	Shabot et al.	340/825.44
5,950,168	A *	9/1999	Simborg et al.	705/3
6,081,809	A	6/2000	Kumagai	707/104
6,179,784	B1	1/2001	Daniels et al.	600/538
6,311,162	B1	10/2001	Reichwein et al.	705/1
RE41,500	E *	8/2010	Shelton et al.	715/217

7,848,935	B2 *	12/2010	Gotlib et al.	705/2
2001/0050610	A1 *	12/2001	Gelston	340/5.53
2002/0044059	A1 *	4/2002	Reeder et al.	340/573.1
2002/0120676	A1	8/2002	Biondi et al.	709/203
2002/0138512	A1	9/2002	Buresh et al.	707/507
2003/0050794	A1	3/2003	Keck	705/2
2004/0039628	A1 *	2/2004	Thompson et al.	705/9
2004/0186746	A1 *	9/2004	Angst et al.	705/3
2006/0080140	A1 *	4/2006	Buttner et al.	705/2
2011/0202370	A1 *	8/2011	Green et al.	705/3
2011/0246226	A1 *	10/2011	Green et al.	705/2

OTHER PUBLICATIONS

Anders Kaliner "Uncertainty in measurement; Introduction and examples from laboratory medicine" The Journal of the International Federation of Clinical Chemistry, 'Online!' vol. 13, No. 1, Jan. 13, 2001, XP002296952.

* cited by examiner

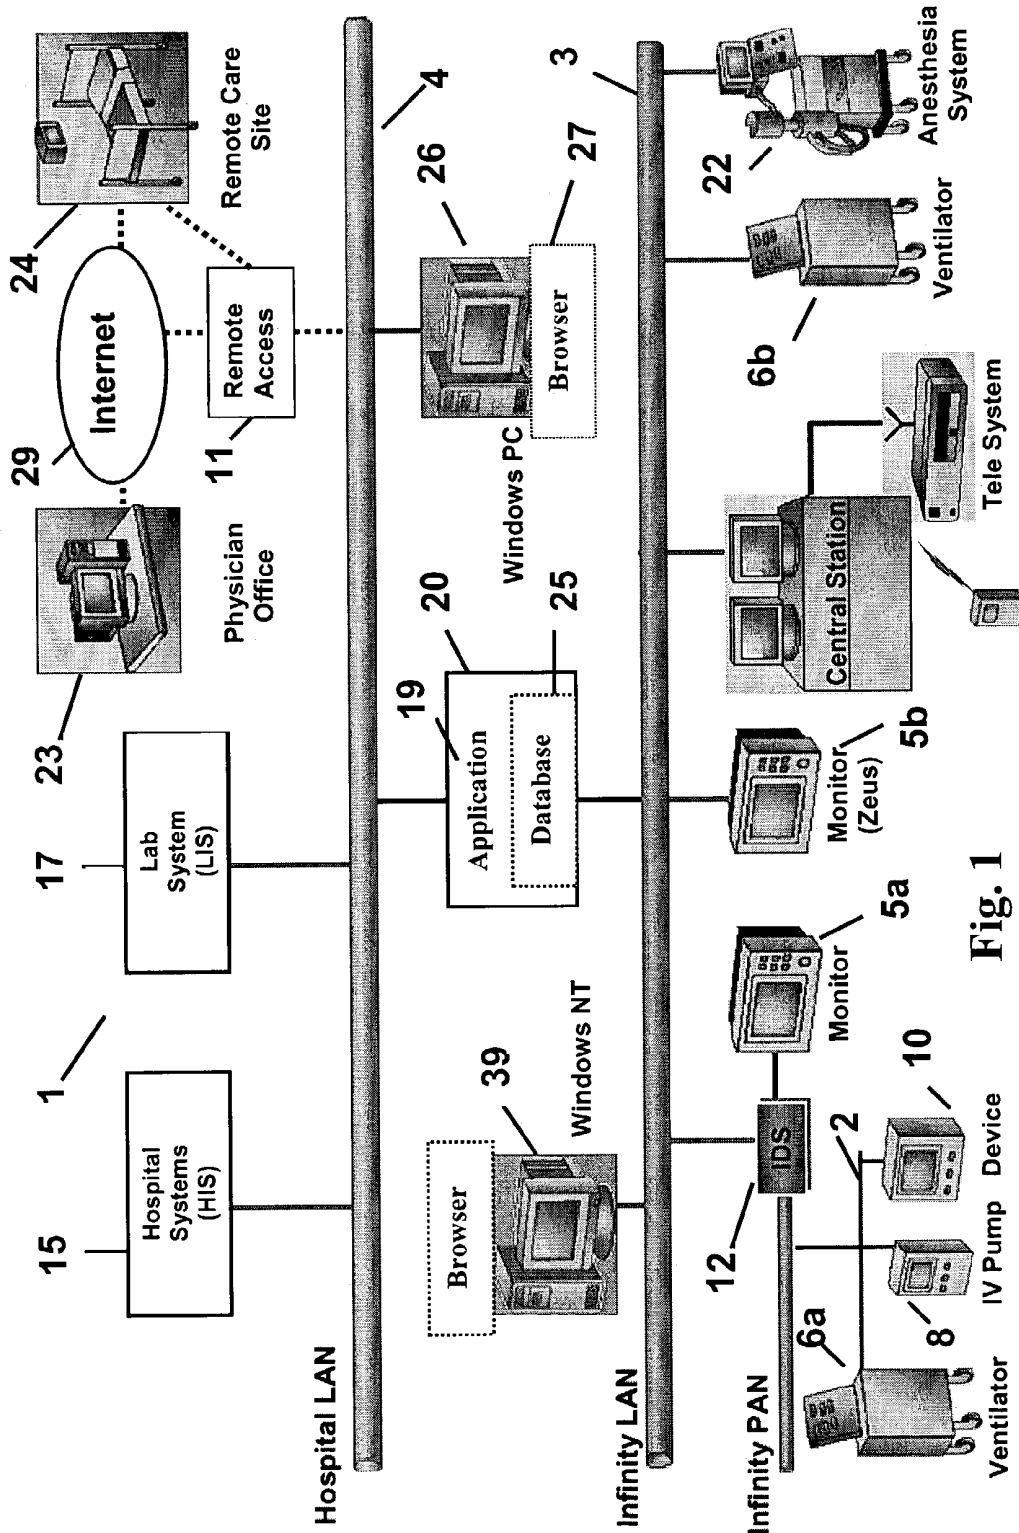


Fig. 1

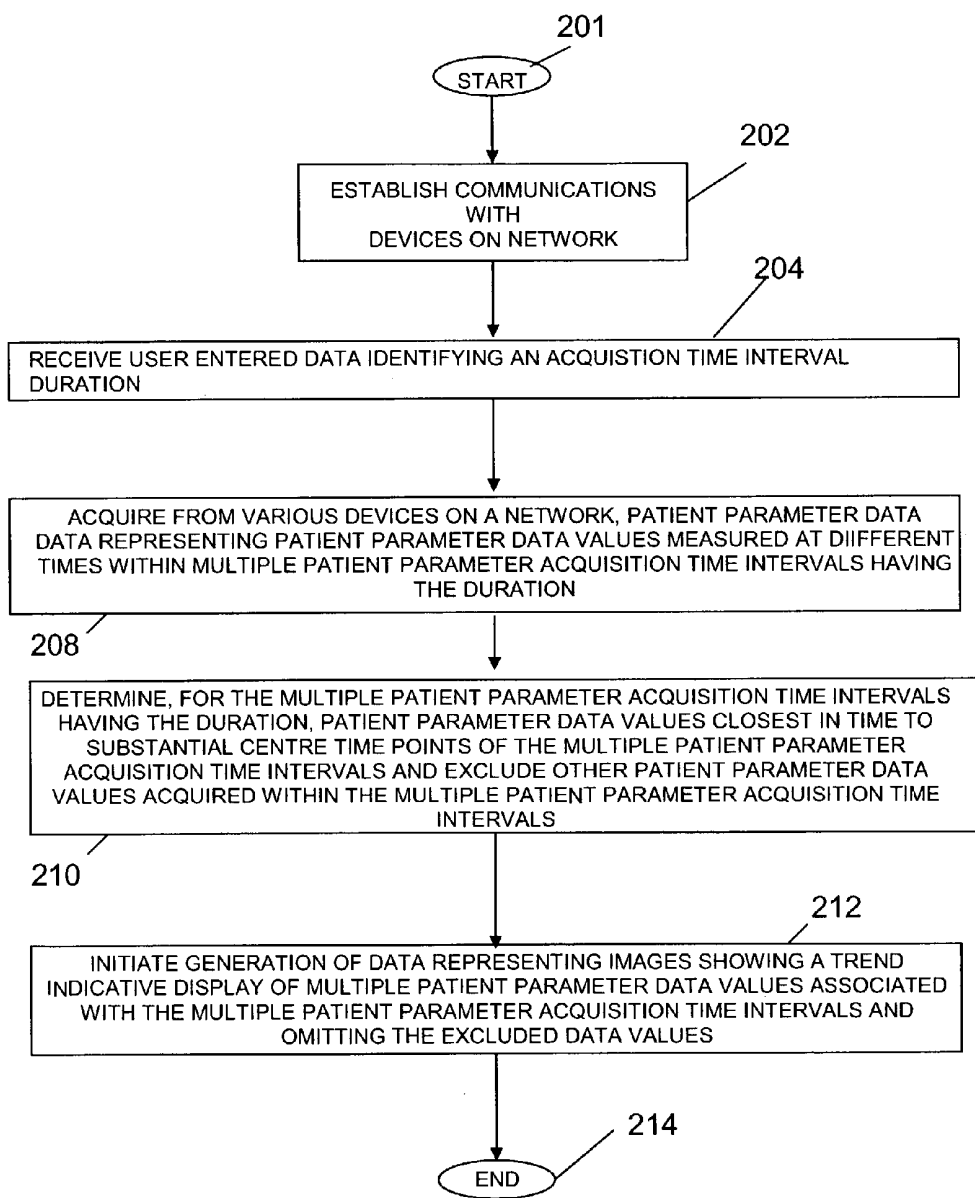


FIGURE 2

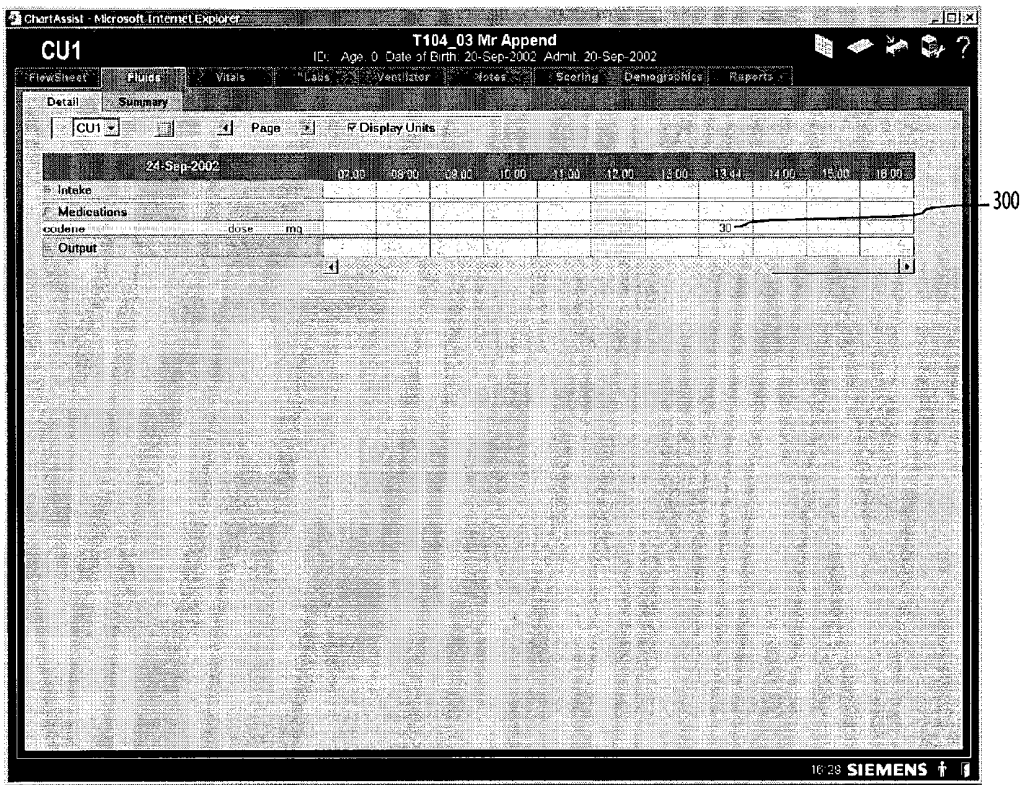


FIGURE 3

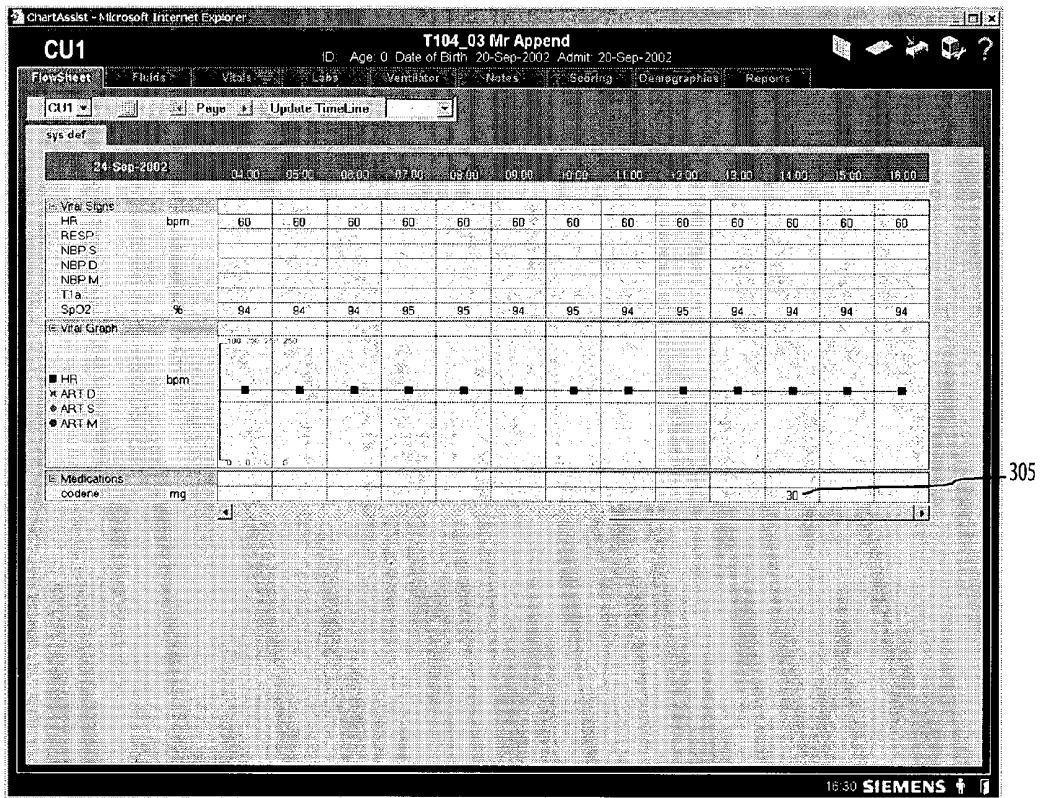


FIGURE 4

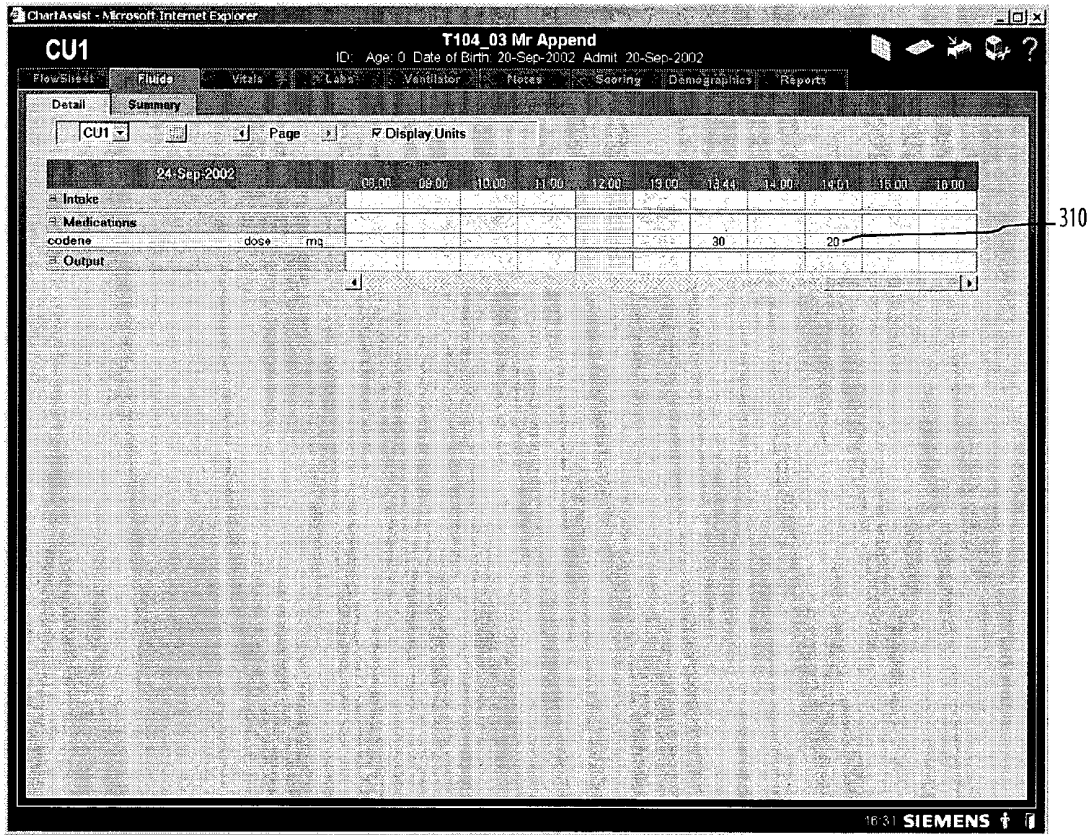


FIGURE 5

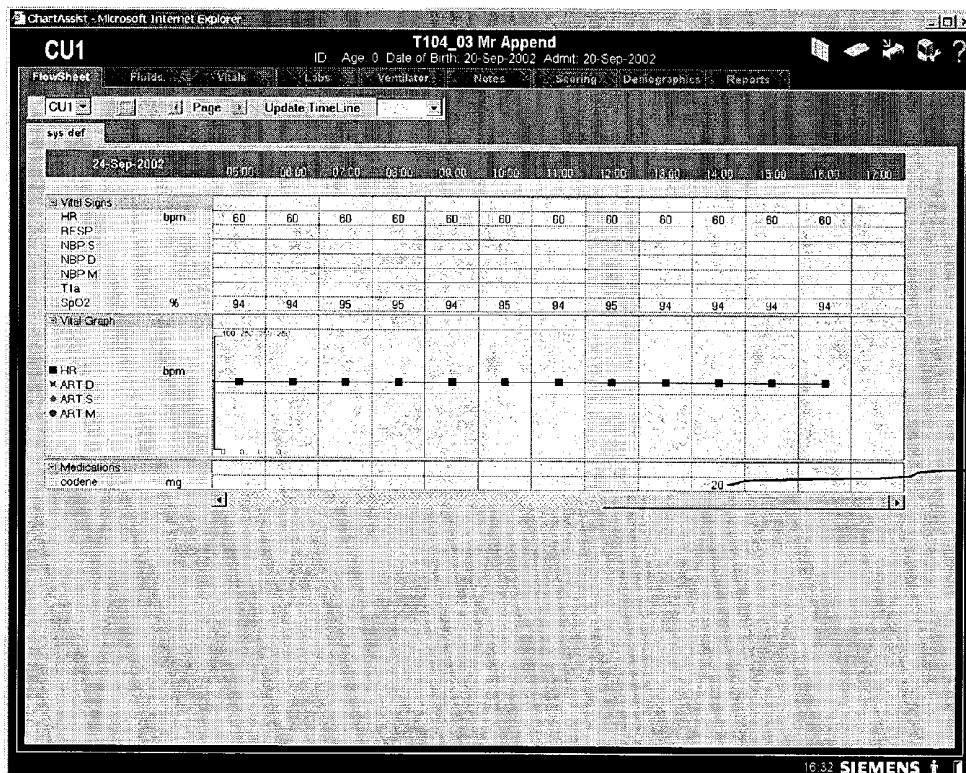


FIGURE 6

FIGURE 7

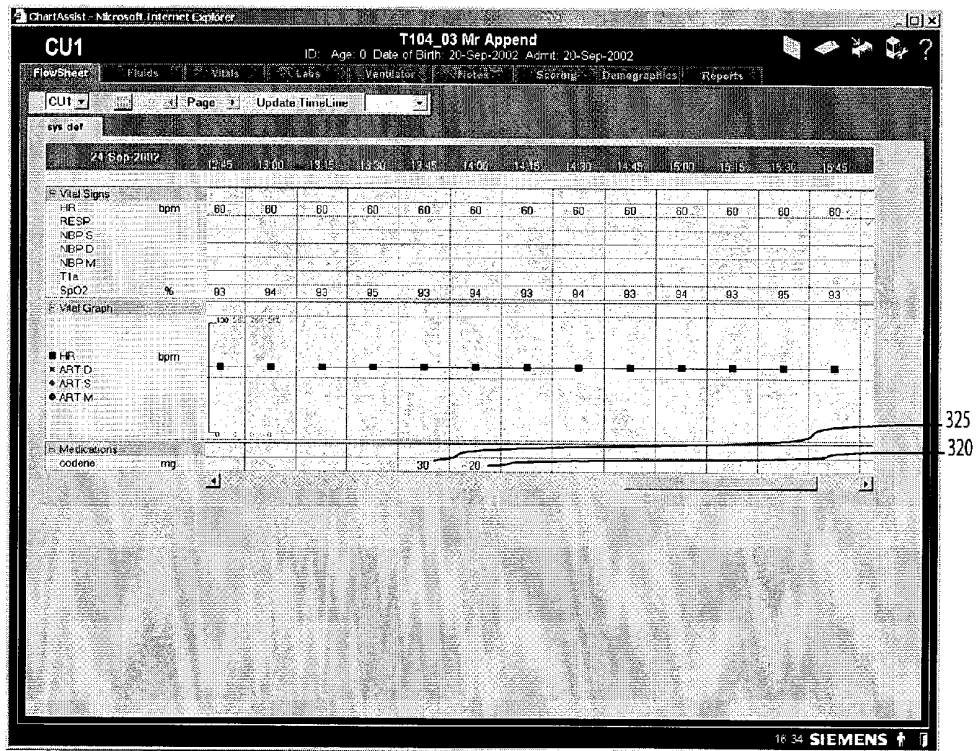


FIGURE 8

400
EXAMPLE
VALUES

CU1
sting Simulated Patient Data
ID: 023-92-8375 Age: 26 Date of Birth: 26-May-1976 Admit: 25-Mar-2002

Flow Sheet Fluids Vitals Labs Ventilator Notes Scoring Demographics Reports

Apache II Apache Risk Saps II Saps Risk TISS 28

15 Aug 2002
16 25 24 Hours
Get Values Clear

Calculate

Current Score

Date	Time	Score
15-Aug	16:17	23
15-Aug	16:14	41
15-Aug	16:02	26
15-Aug	15:59	9
15-Aug	15:52	16
15-Aug	14:41	22
15-Aug	14:32	4

Basic Activity
Standard Monitoring
Laboratory
IV Medication
Drug changes
Care of Drains

Ventilatory support
Support
Care of artificial airway
Tx for improving lung fu

Renal support
Hemofiltration techniques
Quantitative Urine output
Active diuretics

Neurologic Support
ICP monitoring

Cardiovascular Support
Vasopressive medication
IV replacement of large
Peripheral arterial cath
Left atrium monitoring
Central venous line
CPR after arrest

Metabolic support
Tx of complicated metabo
IV hyperalimentation
Enteral feeding

Specific interventions
Single specific interven
Multiple specific interrv
Specific interventions o

Clinical Investigation 16 27 SIEM

FIGURE 9

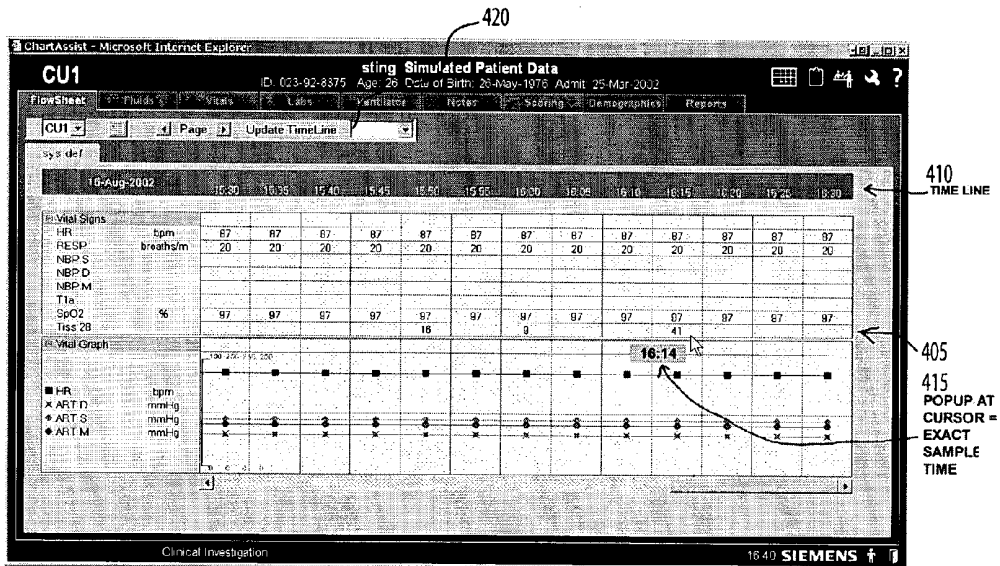


FIGURE 10

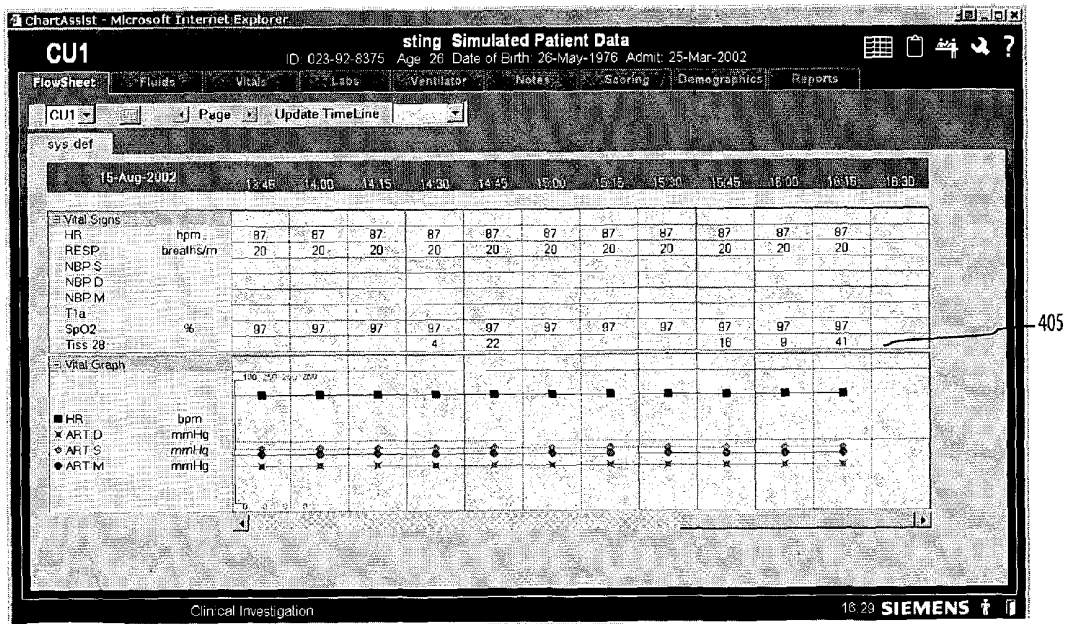


FIGURE 11

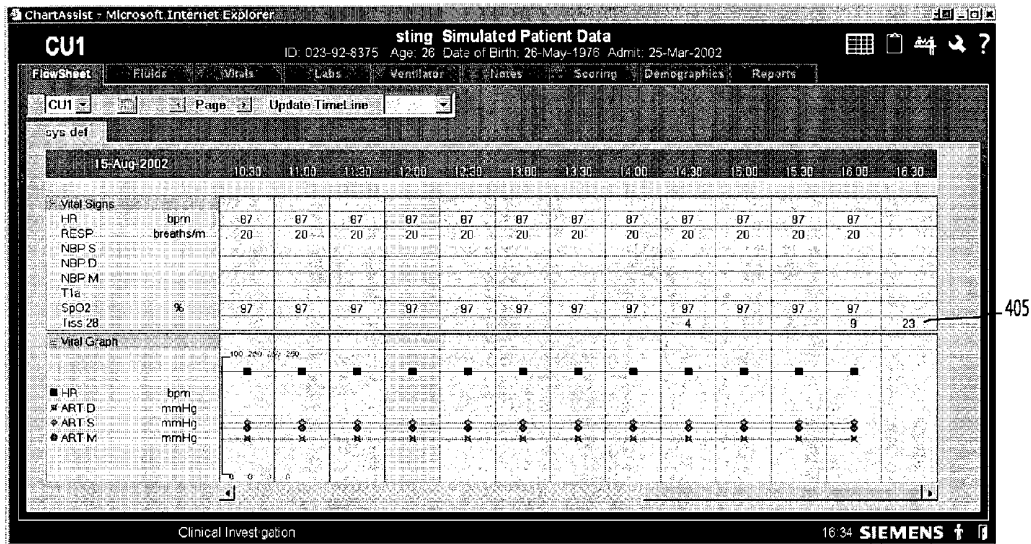
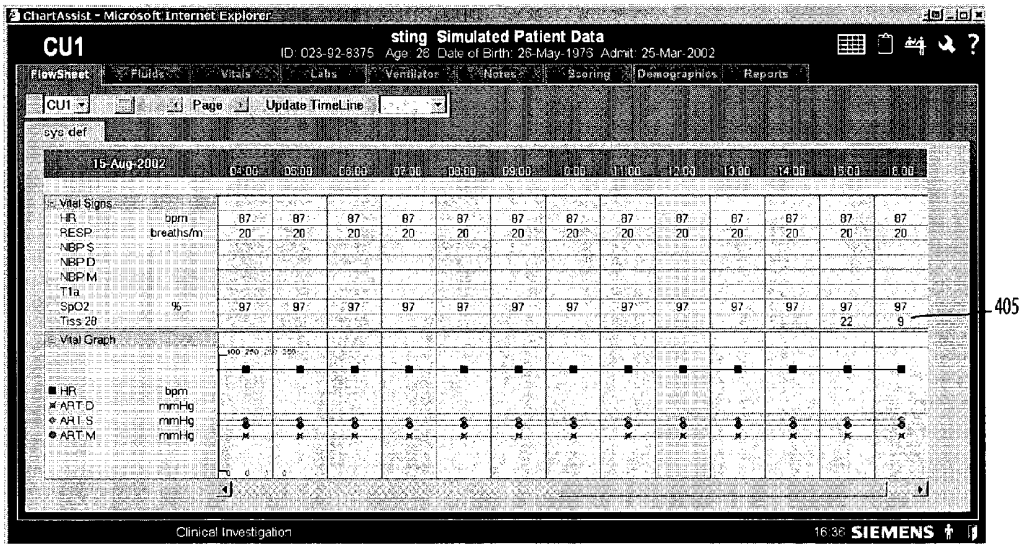


FIGURE 12



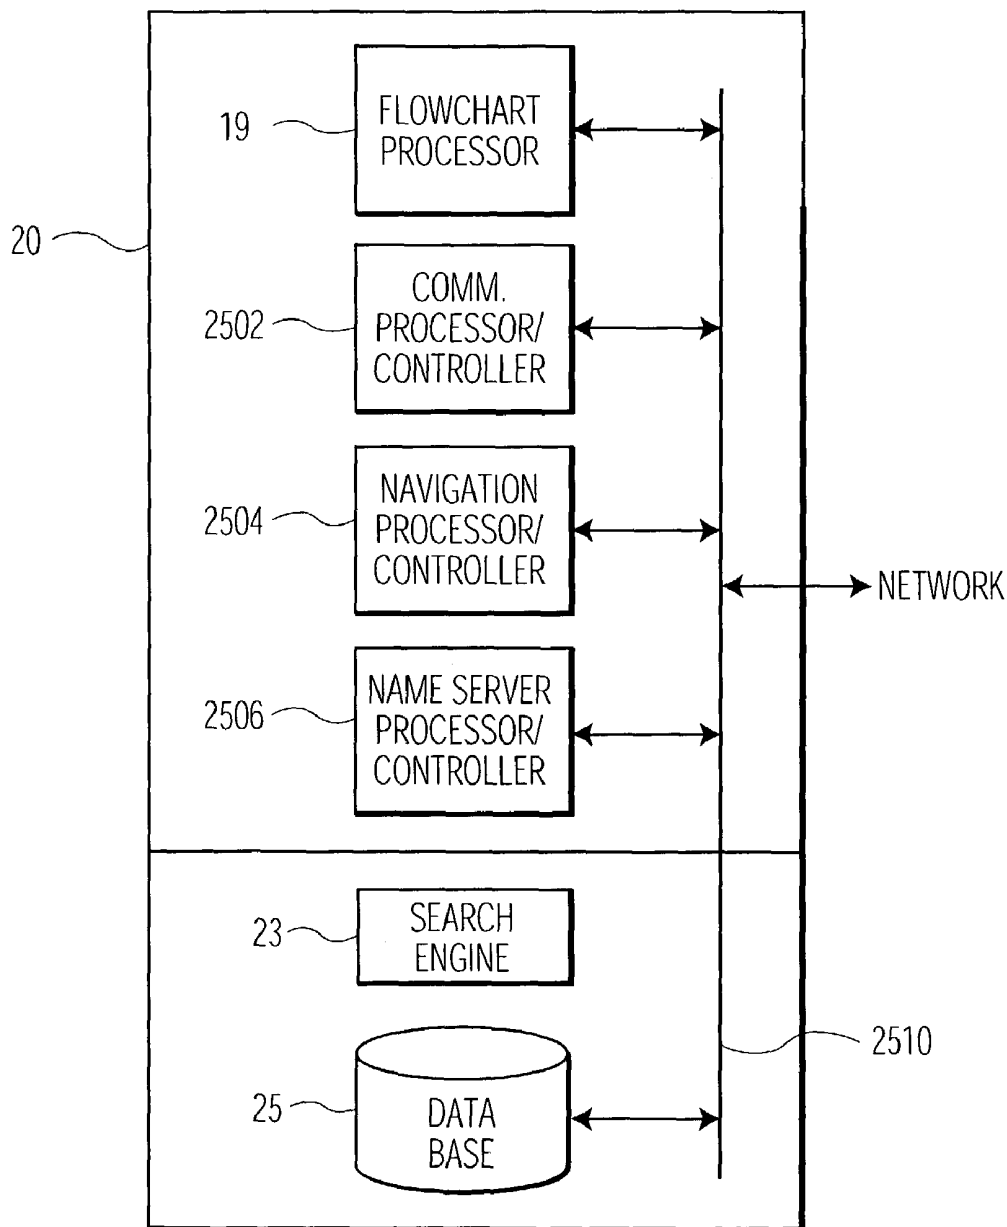


FIGURE 13

PATIENT MEDICAL PARAMETER TREND INDICATIVE USER INTERFACE DISPLAY SYSTEM

This is a non-provisional application of provisional application Ser. No. 60/374,908 by A. M. Manetta et al. filed Apr. 23, 2002 and of provisional application Ser. No. 60/413,301 by J. Rutledge et al. filed Sep. 25, 2002. This application is related to application Ser. No. 10/359,673 filed Feb. 6, 2003 entitled A System and User Interface Supporting Trend Indicative Display of Patient Medical Parameters by A. M. Manetta et al.

FIELD OF THE INVENTION

This invention is related to adaptively processing and displaying of medical information, and more particularly to processing and displaying patient medical data for user configurable display in a network environment.

BACKGROUND OF THE INVENTION

Patient medical parameter data is acquired, collated, stored and displayed for use in providing patient clinical care in hospitals, clinics, and other healthcare delivery settings. Patient medical parameter data may include vital signs ventilator information, infusion pump data associated with fluid delivery and other data. Such patient medical parameter data is typically displayed on a patient monitoring device screen in a trend indicative chart with a time axis. This type of chart is commonly termed a Flowsheet. A patient monitoring device is usually located at a patient bedside or nursing station in a hospital ward or in an intensive care, surgical or other location and may be connected to a network such as the Internet, a LAN, a WAN or an intra-net for acquiring patient parameter data from local sources (e.g., patient attached sensors) or remote sources (e.g., a remotely stored electronic patient record). The Flowsheet is an electronic chronological chart of patient information that substitutes for a paper vital sign Flowsheet. It is desirable that an electronic Flowsheet offer similar or better features and flexibility than a paper Flowsheet chart that it replaces

An electronic Flowsheet provides a trend indicative display covering a time period comprising user selectable patient parameter acquisition time intervals. A user selectable acquisition time interval is represented by a column in the Flowsheet and covers a time period (typically 3 minutes to 4 hours or another user selectable time interval) in which patient parameters are acquired. A problem occurs in known Flowsheet systems in selecting a parameter value to represent a particular parameter acquisition time interval in a trend indicative display. Specifically, in known systems a parameter value displayed in a particular acquisition time interval may not be representative of the time interval. This happens in known systems that label the acquisition time intervals with a displayed time value and automatically allocate a parameter value, received at a specific time, to a displayed labeled interval that precedes or includes the labeled time value. Similarly, it happens in known systems that automatically allocate a parameter value, received at a specific time, to a displayed labeled interval that follows or includes the labeled time value. Using these known systems, a displayed labeled interval may display a parameter value that is closer to an adjacent time interval and consequently present a misleading trend indicative display to a user. In such a known system, a manually entered parameter value or a parameter value indicated as accurate by a user may similarly be misleadingly displayed in

an incorrect labeled time interval. A system according to invention principles addresses these problems and derivative problems.

SUMMARY OF THE INVENTION

A system according to invention principles advantageously automatically displays a parameter closest in time to a centre time point of a particular Flowsheet parameter acquisition time interval column. A system provides patient medical parameter data for trend indicative display covering a time period comprising user selectable acquisition time intervals. The system includes an acquisition processor for, receiving user entered data identifying an acquisition time interval duration and acquiring data representing a patient parameter comprising a plurality of data values at a corresponding plurality of different times within multiple patient parameter acquisition time intervals individually having the duration. A data processor for determining, for the multiple patient parameter acquisition time intervals of the duration, patient parameter data values closest in time to substantial centre time points of the multiple patient parameter acquisition time intervals and for excluding other patient parameter data values acquired within the multiple patient parameter acquisition time intervals.

BRIEF DESCRIPTION OF THE DRAWINGS

In the drawing:

FIG. 1 is a block diagram of a communication network with various devices, according to the principles of the invention.

FIG. 2 represents a flowchart of a method for providing a user interface, according to the present invention.

FIGS. 3-12 show user interface display images showing a Flowsheet trend indicative display of patient parameters, according to the present invention.

FIG. 13 is a block diagram of a server having functionality in accordance with the present invention.

DETAILED DESCRIPTION

The inventors have recognized that it is desirable to provide a digital Flowsheet that automatically displays a selected parameter value in a particular Flowsheet time interval column closest in time to a centre time point of the particular Flowsheet column. For this purpose, the system advantageously stores and examines parameters acquired within half an acquisition time interval either side of the centre time point of the particular Flowsheet column. The system selects from the examined parameter values, a parameter value for display in the particular Flowsheet column that is measured at a time closest to the centre time point of the particular Flowsheet column. However, a manually entered parameter value for a particular Flowsheet acquisition time interval is taken as representative of the Flowsheet acquisition interval and is not replaced by an automatically received parameter value. This is so even if the automatically received value is closer to a Flowsheet acquisition interval centre time. A user entered parameter value, indicated as validated in response to user command via a displayed image, is not replaced by automatically acquired patient parameter data.

FIG. 1 is an exemplary block diagram of a communication network incorporating server 20 hosting executable application 19 providing a trend indicative user interface display of patient parameters (termed a Flowsheet) within identified acquisition time intervals. A Flowsheet may display different

types of parameters associated with, for example, Intra-Venous fluids, drip administered medications, blood products, blood pressure, ventilation, laboratory test data, tissue scores, vital signs, blood oxygen concentration, and infusion pump fluid delivery. In an alternative embodiment, the executable application providing the Flowsheet user interface may be resident in another processing device in any part of the network shown in FIG. 1. Communication network 1 (FIG. 1) is represented by an IP (Internet Protocol) compatible network with a hierarchy of local area and wide area networks interconnected together. It is to be noted that although the present exemplary hospital or medical network is an IP compatible network, other types of networks such as, but not limited to optical or wireless networks, using other computing protocols such as, but not limited to, for example, X.25, frame relay, IBM SNA etc., may also be used, as one skilled in the art can readily appreciate. In addition, although the exemplary network described is a hierarchical network, this is not required by the present invention. Any type of network architecture that provides communication connectivity among the devices on the network may be used.

As shown in FIG. 1, the first level of the exemplary hierarchical network 1 comprises a Medical Interface Bus (MIB) 2. A MIB is a well-known medical industry standard for locally connecting medical devices together. As shown in FIG. 1, MIB 2 is typically used to interconnect medical devices in a care unit such as a patient's room within a nursing station to administer care to a particular patient and to monitor the particular patient. Various medical devices may be connected via MIB 2; examples shown in FIG. 1 comprise a ventilator 6a, IV (Intravenous) Pump 8 or other medical equipment 10. MIB 2 is typically connected to a second level LAN network 3 through an Interface Docking Station (IDS) device 12, for interfacing to Ethernet-compatible LAN network 3. The LAN 3 may be for example, an Infinity LAN, marketed by Siemens Medical System. This higher-level LAN 3 is typically, though not necessarily, used by other care units such as a particular department within a hospital, such as an intensive care unit or surgery unit, etc., depending on the size of the organization.

Although not shown in FIG. 1, more than one MIB may be connected to the second level LAN 3, so that more than one patient may be monitored or provided with care through LAN 3. In addition, medical devices may be connected directly to higher-level LAN 3. For example, as shown in FIG. 1, a ventilator 6b and an anesthesia system 22 are connected directly to LAN 3, without use of a MIB. Furthermore, LAN 3 may be interconnected to a Hospital LAN backbone 4 which also is Ethernet compatible. This backbone network 4 provides communication connectivity between various departments within a hospital or medical organization; for example, connecting hospital administrative systems 15 together with laboratory systems 17. In addition, the Hospital LAN 4 has a remote access gateway 11 which provides remote, secured access from, for example, a remote doctor's office 23 or a remote care site 24, to the various systems and devices on network 1, through for example, Internet 29. Alternatively, a remote site may also access the remote access gateway 19 directly through, for example, a dial-up telephone port, ADSL, or other types of private connection. Remote access gateway 11 may also be part of server 20, to be described below, instead of standing alone, as well known in the art.

According to the principles of the present invention, executable application 19 (or multiple applications in another embodiment) resides on central server 20 on LAN 3 for gathering and processing data from the peripheral medical devices or facilities coupled to LAN 3 or hospital LAN 4,

including laboratory results supplied via laboratory system 17 connected through an HL7 interface, for example. Additional medical parameter data including additional laboratory results acquired from any number of medical devices such as those shown in FIG. 1 may be obtained by server 20 using ASTM messaging, for example. The acquired medical parameters associated with a given patient, including laboratory test results, are acquired from the medical devices on network 1 for display and control on monitors 5a, 5b or PCs 26 and 39 or any other display hosting device at any level of the FIG. 1 network. One skilled in the art can readily recognize that server 20 may reside at any level of the hierarchy of network 1, since all the different levels of LANs (e.g., 3, or 4), as well as remote sites in FIG. 1 are interconnected. An example of server 20, is a Prometheus server, marketed by Siemens Medical System. The server may be hosted, for example, by a computer system that is capable of running Microsoft NT operating system.

Patient parameter data acquired from patient attached equipment may be characterized as of continuous or discrete type. Continuous patient parameter data is periodically sampled and acquired at intervals typically of higher frequency than a displayed acquisition interval and discrete patient parameter data is acquired at non-periodic intervals (e.g., upon nurse measurement initiation) or at periodic intervals of relatively low frequency compared to continuous patient parameter data. Application 19 automatically advantageously filters acquired continuous patient parameter data by selecting a patient parameter value that substantially occurs at (or is reasonably near) the centre time of an individual acquisition time interval for display in a Flowsheet column representing an acquisition time interval. Specifically, the selected continuous patient parameter value is incorporated in an Internet compatible (web based) Flowsheet column representing the individual acquisition time interval. Application 19 automatically advantageously filters discrete acquired patient parameter data by selecting a patient parameter value that occurs at a time closest to the centre time of an individual acquisition time interval for display in a Flowsheet column. Further, application 19 supports generation of a Cursor Tool and user interface image windows enabling a clinician (or other user) to examine, edit, validate or annotate filtered data points or to select alternative acquired patient parameter data points to represent Flowsheet column acquisition intervals (and to override automatically filtered data).

Application 19 provides a user interface trend indicative display of patient parameters (a Flowsheet) covering a time period comprising user selectable acquisition time intervals. A user selectable acquisition time interval represented by a column in the Flowsheet covers a time period (typically 3 minutes to 4 hours or another user selectable range) in which patient parameters are acquired. Application 19 automatically filters acquired patient parameter data by selecting a patient parameter value for display in a Flowsheet column representing an individual acquisition time interval. Specifically, the selected patient parameter value is incorporated in an Internet compatible (web based) Flowsheet column representing the individual acquisition time interval.

FIG. 2 shows in flow chart form, functions that are performed by executable application 19. Application 19 establishes communication with devices on the network as shown in step 202 after the start at step 201. This is done, for example, by using IP protocol and the known IP device address for each device on the network 1 (FIG. 1), in conjunction with any higher application-layer protocols, as well known in the art. Once communication is established between

server **20** and the other devices, application **19**, in step **204**, receives user entered data identifying an acquisition time interval duration. In step **208** application **19** acquires, from various devices on the network, data representing a patient parameter comprising multiple data values at corresponding multiple different times within multiple patient parameter acquisition time intervals individually having the duration. The parameter may comprise, a blood pressure parameter, a respiratory or ventilation parameter, a vital sign parameter, a blood oxygen concentration representative parameter, an infusion pump parameter associated with fluid delivery, a drip medication related parameter and another fluid related parameter, for example. Other parameters being acquired include laboratory results and settings selected for various monitoring devices. As previously mentioned, laboratory results may be obtained through an HL7 interface with LIS **17**, or via ASTM or MIB point of care (POC) medical devices depicted in FIG. 1.

Medical data and laboratory results may be continuously, periodically or non-periodically acquired and correlated with a given patient for storage in relational data base **25** within server **20**. Data base **25** may be of the type used for storing relational data such as the Microsoft SQL server. In addition, application **19** may obtain patient parameter data and patient data comprising medical laboratory results that are first entered and stored, for example, in laboratory system **17** of FIG. 1. Also, application **19** may acquire healthcare provider entered medical notes for display. In step **210** application **19** determines, for the multiple patient parameter acquisition time intervals of the user selected duration, patient parameter data values closest in time to substantial centre time points of the multiple patient parameter acquisition time intervals. Application **19** excludes other patient parameter data values acquired within the multiple patient parameter acquisition time intervals. Flowsheet columns representing the multiple patient parameter acquisition time intervals are identified and labeled in the Flowsheet image display with the determined centre time point values.

The patient parameter data values closest in time to the centre time points of the multiple patient parameter acquisition time intervals are determined by examining patient parameters acquired within substantially half an acquisition time interval either side of a centre time point. For a one hour interval a period of 30 minutes before and after the display column centre time point is examined. An acquisition time interval data value entered (or an existing data value marked) by a user, and thereby identified as being representative of a time interval, takes precedence over a data value determined to be closest in time to a centre time point of the time interval. Such a user entered or marked data value is not replaced by a data value selected based on closeness in time to a centre time point of the time interval. In response to user selection of a different acquisition time interval duration, application **19** repeats steps **204-210**, and dynamically determines patient parameter data values closest in time to substantial centre time points of the multiple patient parameter acquisition time intervals of the new duration. Application **19** as previously described, excludes other patient parameter data values acquired within the multiple patient parameter acquisition time intervals of the new duration value.

Application **19** in step **212** generates data representing an image showing Flowsheet trend indicative display of patient parameter data values associated with multiple patient parameter acquisition time intervals and omitting excluded data values. Specifically, application **19** initiates generation of an image exemplified by the images of FIGS. 3-12. In particular, images of FIGS. 3-7 illustrate operation of the

system. The image of FIG. 3 shows a user entered Codeine medication of 30 units (item **300**) administered at 13:44 pm being displayed in the Flowsheet trend indicative display of FIG. 4 during the parameter acquisition interval labeled 14:00 pm (item **305**). This is because the Codeine medication is identified as being administered at 13:44 pm which is closest to the parameter acquisition interval labeled centre time of 14:00 pm.

In response to a user entering another Codeine dose of 20 units for that same patient at 14:01 pm, as indicated as item **310** in the image of FIG. 5, the Flowsheet image acquisition interval labeled with centre time of 14:00 pm changes to show the entered 20 units (as shown as item **315** of FIG. 6). The 30 unit dose is excluded as the 20 unit dose is entered closer in time to the 14:00 pm interval centre time. If a user places a cursor over the displayed item **315** (e.g., using a mouse, or other cursor manipulation device), the user entered time associated with the 20 unit dose (14:01 pm) is advantageously displayed. In addition, in response to a user selecting a different parameter acquisition time interval of 15 minutes instead of one hour (as in FIGS. 3-6) both the 20 unit and 30 unit values are shown, as illustrated by items **320** and **325** respectively of FIG. 7. This is because the 30 unit dose entry time (13:44 pm) is closest to the interval labeled centre time of 13:45 pm and the 20 unit dose entry time (14:00 pm) is closest to the interval labeled centre time of 14:00 pm. Also, if a user indicates (by data entry) that the 20 unit dose value of 14:01 pm is to represent the time interval, even if another Codeine dose value closer to 14:00 pm is entered, the 20 unit dose takes precedence and is displayed as representing the 14:00 pm column time interval.

Display images of FIGS. 8-12 further illustrate system operation showing Flowsheet trend indicative display of the same data values **400** (TISS28 Scoring values) of FIG. 8 within parameter acquisition time intervals of different duration. The images of FIGS. 9-12 illustrate selection of particular values of TISS28 scoring data values **400** for Flowsheet display based on data value closeness to the labeled column centre time. The images of FIGS. 9-12 also show continuously acquired data values (e.g. HR-Heart Rate) associated with a column labeled centre time. FIG. 9 shows the exemplary tissue scoring data values in row **405** displayed in 5 minute duration acquisition time intervals between 15:30 and 16:30 pm as indicated in the time line **410**. Row **405** shows three data values in columns with centre times of 15:50, 16:00 and 16:15. If a user places a cursor over the displayed value (**41**) in the 16:15 time interval column (e.g., using a mouse), the user entered time associated with value (16:14 pm, item **415**) is displayed. Further, in response to user selection of a different (15 minute) time interval duration using update time line display element **420** of FIG. 9, the exemplary data values are displayed in FIG. 10 row **405** in 15 minute duration intervals. Five values are displayed in FIG. 10 in columns with centre times of 14:30, 14:45, 15:45, 16:00 and 16:15. Similarly, FIG. 11 shows three data values displayed in row **405** in columns with centre times of 14:30, 16:00 and 16:30 (30 minute duration intervals) and FIG. 12 shows two data values displayed in row **405** in columns with centre times of 15:00 and 16:00 (one hour duration intervals).

In one aspect of the present invention, a user may use a Microsoft Windows compatible PC **26** or Windows NT compatible PC **39** as shown in FIG. 1, or any other processing devices capable of running a menu generating program such as a web browser program (e.g., Microsoft Internet Explorer or Netscape Navigator, etc.) to view a Flowsheet, medical parameters and laboratory results information associated with a given patient. That is, a user may use a web browser on

any processing device, as long as a communication connection can be made to server **20** and application **19**, to make requests and view information acquired and stored in data base **25**. This is advantageous, since a doctor may for example, gain access to a Flowsheet or laboratory test results from, for example, a remote physician's office **23**, without having to access a dedicated terminal. Of course, a user can simply use a keyboard and/or a mouse or any other user interface devices to enter a user selection or request on a user computer, as is known in the art. Application **19** is therefore capable of collating and formatting medical data to be compatible with, for example, HTML (HyperText Mark-up Language) programming language for displaying data on a web browser. Application **19** is also responsive to, for example, HTTP (HyperText Transfer Protocol) commands originated from a user's web browser for making a request. The process of FIG. **2** ends at step **214**.

FIG. **13** shows a block diagram of an exemplary embodiment of server **20** (FIG. **1**) including functions in accordance with the present invention for generating data for configuring and presenting a Flowsheet trend indicative display and for managing, collating, searching and updating data base **25** containing patient medical information. Executable applications or processors operative to carry out instructions for performing the various functions described herein include an executable application **19** for performing Flowchart related processing and communications processing module **2502** that acquires the patient data including the monitored parameters allocated to a given patient from the network and collates the information for storage in data base **25**. Navigation collation processor **2504** operates in conjunction with the web browser and display generator software to collate and prioritize parameters for display to the user while navigating through various applications selected by a user through the user interface. Name server processor **2506** associates unique identifiers (IDs) with each node connected to the system network and with each patient in the system in order to track and update patient information throughout the system. Input/output data and control signals are used to communicate between the various processors as well as to interface with the data base **25** and search engine **23** and with the network via communication line **2510**.

The Flowchart user interface display images, systems and processes presented in FIGS. **1-13** are not exclusive. Other Flowchart configuration and presentation display images, systems and processes may be derived in accordance with the principles of the invention to accomplish the same objectives. Although this invention has been described with reference to particular embodiments, it is to be understood that the embodiments and variations shown and described herein are for illustration only and that various modifications may be implemented by those skilled in the art without departing from the scope of the invention. The system advantageously enables a user to select continuous and discrete (episodic) data from a database for presentation in a user selected time period duration.

What is claimed is:

1. A system for providing patient medical parameter data for trend indicative display covering a time period comprising user selectable acquisition time intervals, comprising:
an acquisition processor for,
receiving user entered data identifying an acquisition time interval duration, and
acquiring data representing a patient parameter using a patient monitoring device having at least one patient connected sensor, the data representing the patient parameter comprising a plurality of data values at a

corresponding plurality of different times within multiple patient parameter acquisition time intervals individually having said duration; and
a data processor for determining, for said multiple patient parameter acquisition time intervals having said duration, patient parameter data values closest in time to substantial centre time points of said multiple patient parameter acquisition time intervals and for excluding other patient parameter data values acquired within said multiple patient parameter acquisition time intervals.

2. A system according to claim **1**, including
a generator for generating data representing an image showing a trend indicative display of said plurality of patient parameter data values associated with said multiple patient parameter acquisition time intervals and omitting said excluded data values.

3. A system according to claim **1**, wherein
said acquisition processor receives user entered data identifying a second acquisition time interval duration, and said data processor dynamically determines, for multiple patient parameter acquisition time intervals of said second duration, patient parameter data values closest in time to substantial centre time points of said multiple patient parameter acquisition time intervals of said second duration and excludes other patient parameter data values acquired within said multiple patient parameter acquisition time intervals of said second duration.

4. A user interface system for providing patient medical parameter data for trend indicative display covering a time period comprising user selectable acquisition time intervals, comprising:
an acquisition processor for acquiring data representing a patient parameter using a patient monitoring device having at least one patient connected sensor, the data representing the patient parameter comprising a plurality of data values at a corresponding plurality of different times within multiple user selectable patient parameter acquisition intervals comprising a time period;
a data processor for determining for a particular user selectable acquisition time interval a patient parameter data value closest in time to a substantially centre time point of said particular user selected acquisition time interval and for excluding other patient parameter data values acquired within said particular user selectable acquisition time interval; and
a generator for generating data representing an image showing a trend indicative display of said patient parameter including said determined patient parameter data value associated with said particular user selectable acquisition time interval and omitting said excluded data values.

5. A user interface system according to claim **4**, wherein in response to user selection of a plurality of second acquisition time intervals comprising said time period and said second acquisition time interval is different to said particular user selectable acquisition time interval, said data processor automatically determines another patient parameter data value closest in time to a centre time point of said second acquisition time interval and excludes other patient parameter data values acquired within said second acquisition time interval.

6. A user interface system according to claim **4**, wherein in response to user command and entry of a patient parameter data value,
said data processor uses said user entered data value as said determined patient parameter data value associated with said particular user selectable acquisition time interval

- and excludes other patient parameter data values acquired within said particular user selectable acquisition time interval.
7. A user interface-system according to claim 6, wherein said data processor excludes a non-user entered patient parameter data value acquired within said particular user selectable acquisition time interval, said non-user entered patient parameter data value being closer in time to said centre time point of said particular user selected acquisition interval.
8. A user interface system according to claim 4, wherein said patient parameter comprises at least one of, (a) a blood pressure parameter, (b) a ventilation parameter, (c) a vital sign parameter, (d) a blood oxygen concentration representative parameter, (e) an infusion pump parameter associated with fluid delivery.
9. A user interface system according to claim 4, wherein said data processor determines said patient parameter data value closest in time to a centre time point of said particular user selected acquisition time interval by examining patient parameters acquired within substantially half an acquisition time interval either side of said centre time point.
10. A user interface system according to claim 4, wherein in response to a user positioning a cursor in the proximity of said patient parameter point in said image showing said trend indicative display, a time associated with at least one of, (a) measurement and (b) acquisition, of said patient parameter point is displayed.
11. A user interface system according to claim 4, wherein said acquisition processor acquires said data representing a patient parameter comprising said plurality of data values from a patient monitoring device.
12. A method for providing patient medical parameter data for trend indicative display covering a time period comprising user selectable acquisition time intervals, comprising the activities of:
- receiving user entered data identifying an acquisition time interval duration;
 - acquiring, from a patient monitoring device using at least one patient connected sensor, data representing a patient

- parameter comprising a plurality of data values at a corresponding plurality of different times within multiple patient parameter acquisition time intervals individually having said duration;
 - determining, for said multiple patient parameter acquisition time intervals having said duration, patient parameter data values closest in time to substantial centre time points of said multiple patient parameter acquisition time intervals; and
 - excluding other patient parameter data values acquired within said multiple patient parameter acquisition time intervals.
13. A non-transitory storage medium according to claim 12, including computer readable instructions for implementing the activities of claim 12.
14. A method for providing patient medical parameter data for trend indicative display covering a time period comprising user selectable acquisition time intervals, comprising the activities of:
- acquiring, from a patient monitoring device, data representing a patient parameter comprising a plurality of data values at a corresponding plurality of different times within multiple user selectable patient parameter acquisition intervals comprising a time period;
 - determining for a particular user selectable acquisition time interval a patient parameter data value closest in time to a substantially centre time point of said particular user selected acquisition time interval;
 - excluding other patient parameter data values acquired within said particular user selectable acquisition time interval; and
 - generating data representing an image showing a trend indicative display of said patient parameter including said determined patient parameter data value associated with said particular user selectable acquisition time interval and omitting said excluded data values.
15. A non-transitory storage medium according to claim 14, including computer readable instructions for implementing the activities of claim 14.

* * * * *

专利名称(译)	患者医疗参数趋势指示用户界面显示系统		
公开(公告)号	US8286088	公开(公告)日	2012-10-09
申请号	US10/411950	申请日	2003-04-11
[标]申请(专利权)人(译)	SHAFFER JUDITH PENNY MARK 蒙特利昂娜RAND J MANETTA AMY 中号 拉特利奇JOLYN		
申请(专利权)人(译)	SHAFFER JUDITH PENNY MARK 蒙特利昂娜RAND J. MANETTA AMY M. 拉特利奇JOLYN		
当前申请(专利权)人(译)	德尔格医疗系统公司.		
[标]发明人	SHAFFER JUDITH PENNY MARK MONTELEONE RAND J MANETTA AMY M RUTLEDGE JOLYN		
发明人	SHAFFER, JUDITH PENNY, MARK MONTELEONE, RAND J. MANETTA, AMY M. RUTLEDGE, JOLYN		
IPC分类号	G06F3/048 G08B23/00 G06F17/21 G06F17/00 G06Q10/00 A61B5/00 A61G12/00 A61M5/00 A61M16/00 G06F G06F19/00 G06Q50/24 G06T11/20 G16H10/60		
CPC分类号	G06F19/3406 G06Q50/24 G06F19/00 G16H40/63 G16H40/67		
优先权	60/374908 2002-04-23 US 60/413301 2002-09-25 US		
其他公开文献	US20040002874A1		
外部链接	Espacenet USPTO		

摘要(译)

根据本发明原理的系统有利地自动地在最接近的流程图参数获取时间间隔列内显示参数值。用户界面系统提供用于趋势指示显示的患者医疗参数数据，其覆盖包括用户可选择的获取时间间隔的时间段。该系统包括获取处理器，用于从患者监测设备获取表示患者参数的数据，该数据包括在一个时间段的多个用户可选择的患者参数获取间隔内的相应的多个不同时间的多个数据值。数据处理器针对特定用户可选择的获取时间间隔确定患者参数数据值，该患者参数数据值在时间上最接近特定用户选择的获取时间间隔的中心时间点，并且排除在特定用户可选择获取时间间隔内获取的其他患者参数数据值。生成器生成表示图像的数据，该图像示出了患者参数的趋势指示显示，包括与特定用户可选择获取时间间隔相关联的所确定的患者参数数据值，并且省略了排除的数据值。

