



(19) **United States**

(12) **Patent Application Publication** (10) **Pub. No.: US 2002/0191670 A1**

Huang et al.

(43) **Pub. Date: Dec. 19, 2002**

(54) **INFRARED RADIATION EAR THERMOMETER AND OFFSET METHOD**

(52) **U.S. Cl. 374/133; 374/130; 600/549; 600/474; 702/131; 374/131**

(76) **Inventors: Yu Chien Huang, Hsinchu City (TW); Simon Taso, Hsinchu City (TW); Vincent Weng, Hsinchu City (TW); Charles Chang, Hsinchu City (TW); Kevin Lin, Hsinchu City (TW); Roger Chen, Hsinchu City (TW); Jason Liao, Hsinchu City (TW)**

(57) **ABSTRACT**

An infrared radiation ear thermometer has an optical system, an infrared detector, an ambient temperature sensor, and display unit, a signal processing section. Wherein, the infrared detector further includes an infrared sensor and a temperature reference sensor; the infrared sensor is deposition on the substrate and the temperature reference sensor is mount near the substrate of the infrared detector to convert the infrared signal into an electrical signal and sense the reference temperature separately. The ambient temperature sensor is set in the space near the optical system to detect the fast change of the ambient temperature. The signal processing section receives the signals from these temperature sensors to produce an offset by a mathematical algorithm. The offset is used to correct the temperature reading and maintain a high precision even though the ear thermometer suffers from an extreme temperature change.


Correspondence Address:
PRO-TECHTOR INTERNATIONAL SERVICES
20775 Norada Court
Saratoga, CA 95070-3018 (US)

(21) **Appl. No.: 09/877,354**

(22) **Filed: Jun. 7, 2001**

Publication Classification

(51) **Int. Cl.⁷ G01J 5/06; A61B 5/00; G01J 5/08**

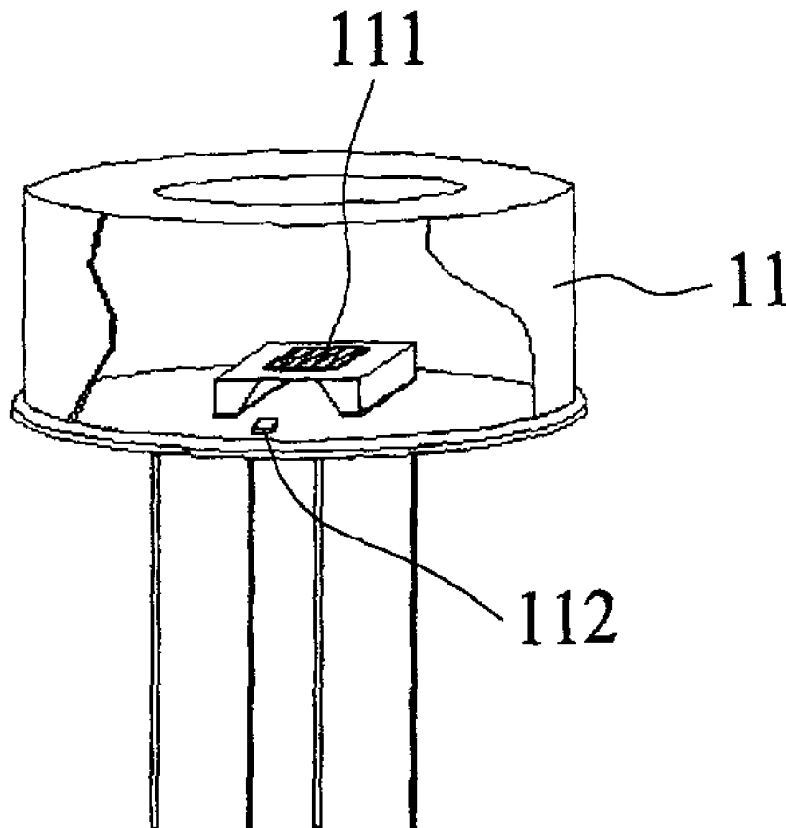

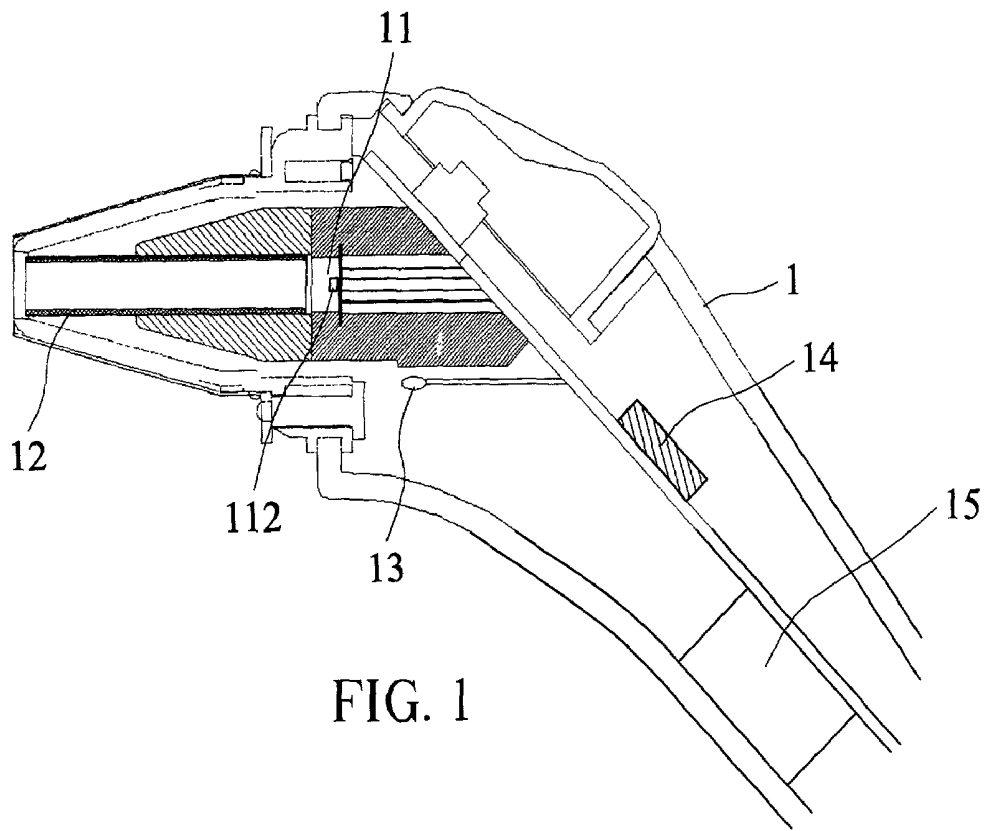


FIG. 1

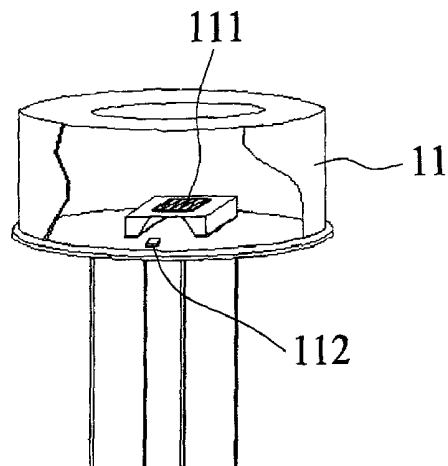


FIG. 2

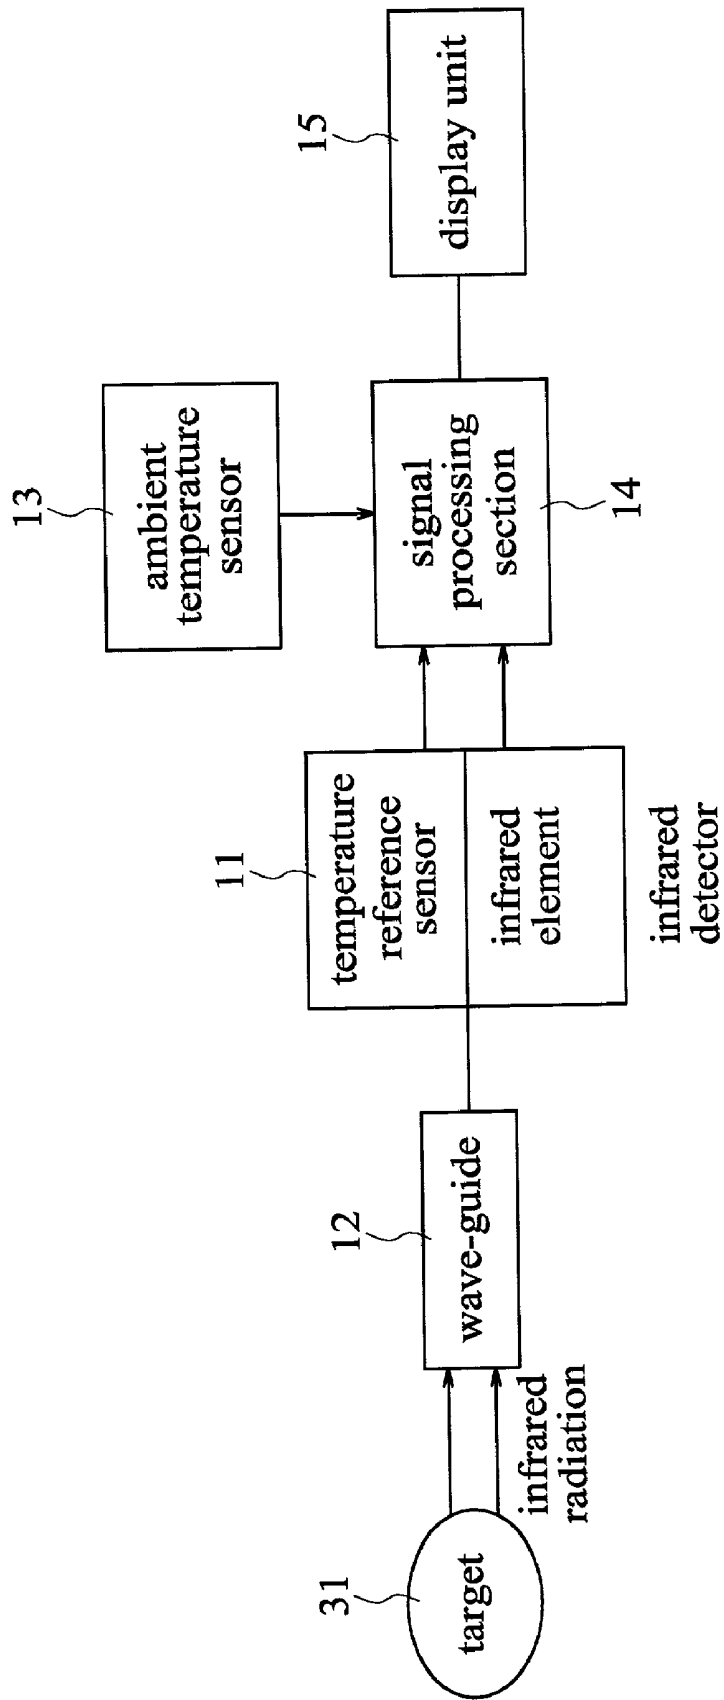


FIG. 3

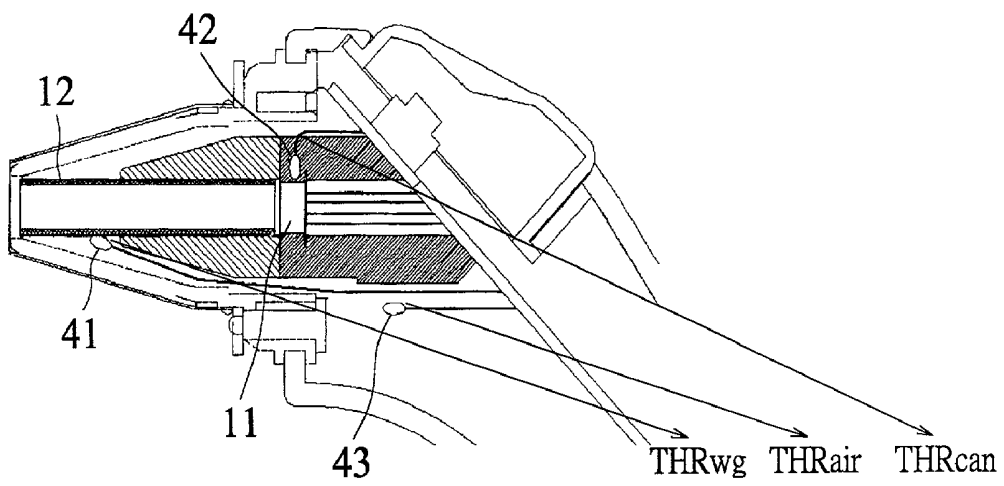


FIG. 4

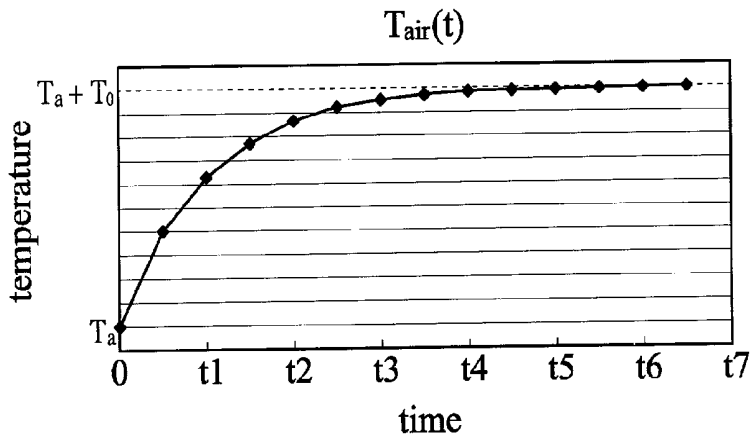


FIG. 5

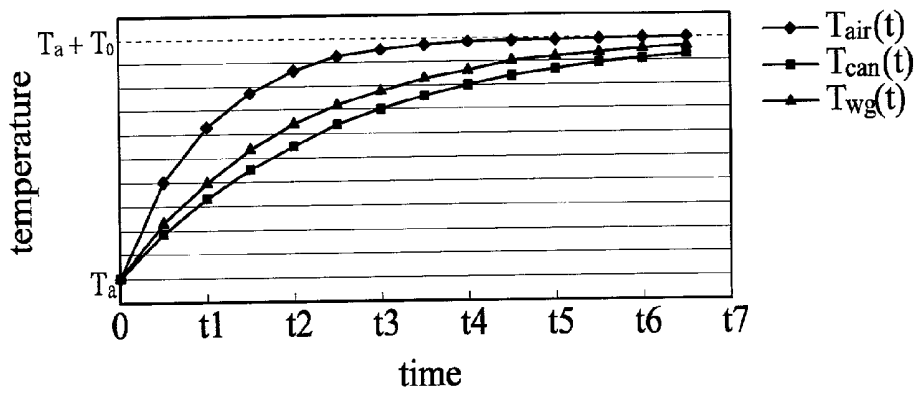


FIG. 6

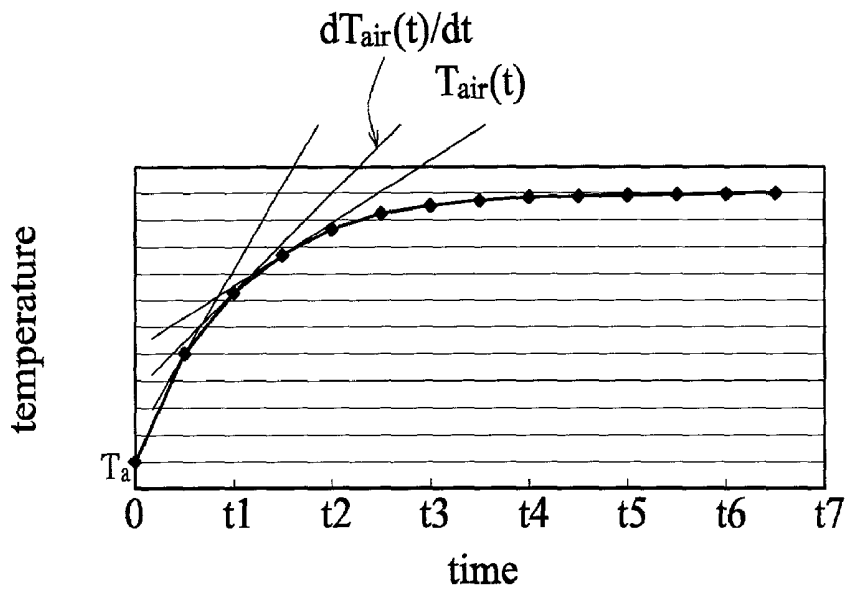


FIG. 7

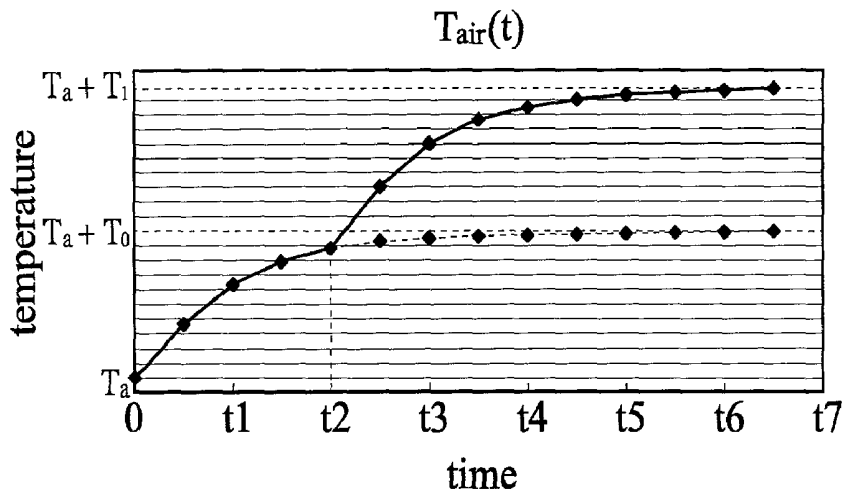


FIG. 8

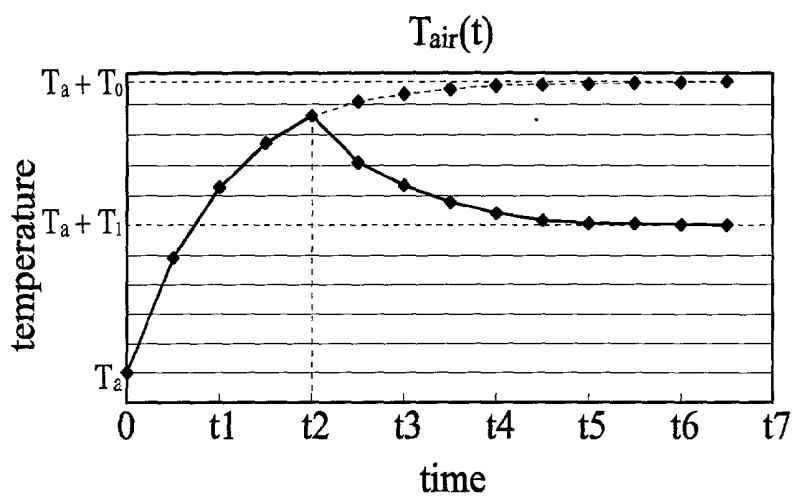


FIG. 9

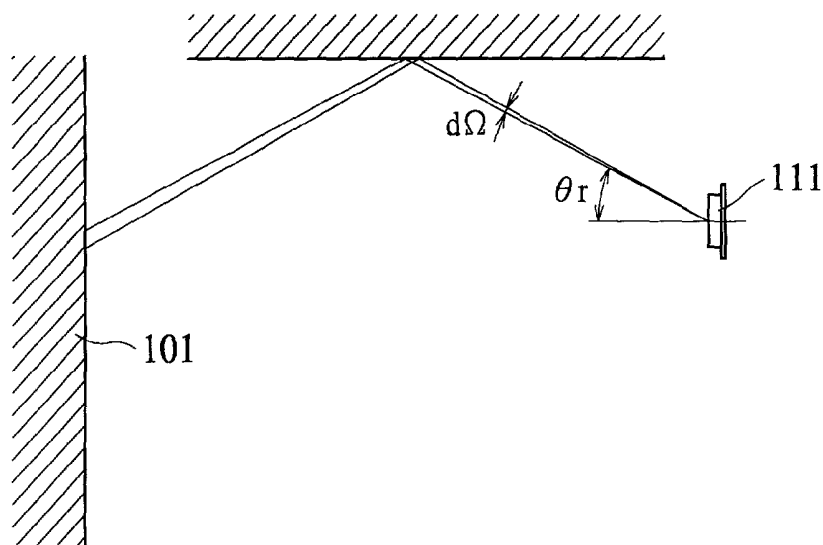


FIG. 10

INFRARED RADIATION EAR THERMOMETER AND OFFSET METHOD

BACKGROUND OF THE INVENTION

[0001] 1. Field of the Invention

[0002] The present invention relates to an ear infrared radiation ear thermometer for reading the clinical temperature of body by inserting in an external ear canal.

[0003] 2. Description of the Prior Art

[0004] All traditional infrared radiation thermometers suffer some inefficient sensitivity to the ambient temperature due to the temperature dependent detector responsibility and unexpected radiation from the optical system like optical-guide. In most infrared radiation thermometers, there is an electronic means of using a reference temperature sensor to compensate the inefficient sensitivity of temperature change. However, if the ambient temperature changes quickly, the compensation is unlikely to track the change in the detector temperature exactly.

[0005] According the disclosed infrared clinical thermometer in U.S. Pat. No. 4,895,164, its combination of a radiation detector should be operated in isothermal condition with an optical-guide. This thermometer especially has a heat conducting block that is constructed and configured so as to remain the thermometer in an isothermal state. However, the isothermal condition is not easy to maintain when the ambient temperature changes rapidly. For example, if the thermometer is taken out from a warm room (say 30° C.) to a cold room (say 15° C.), the isothermal condition is destroyed and the processing of reaching the new isothermal state of the thermometer should take up to half hour or an hour even more to ensure the whole instrument comes to equilibrium.

[0006] Another radiation clinical thermometer disclosed in U.S. Pat. 5,024,533 has a probe with an optical guide and an infrared detector, a detection signal processing section, a body temperature operating section, and a display unit. The body temperature operating section receives infrared data from infrared detector, temperature-sensitive data from two reference temperature sensors. These temperature-sensitive data is taken into account the temperature equilibrium between the optical guide and the infrared detector so as to accurately calculate body temperature. These two reference temperature sensors are separately fixed on the infrared detector and the optical guide to detect the temperature difference between the infrared detector and the optical guide. In this case, body temperature comes out basing on the temperature difference from the tow reference temperature sensors under a non-isothermal condition. Unfortunately, it is not simple for this case. First of all, the optical guide is not the only one source to cause the measure error by exchanging radiation with the infrared detector. All the optical system including the inner wall of the infrared detector package, the detector window and even the probe itself may have radiance on the detector element that must be correct in order to achieve the accuracy demand under the non-isothermal state. In addition, the ambient temperature changing may be diversely. The ambient temperature may be unsteady both on the changing directions and timing. If the thermometer is susceptible to rapid temperature changes in random position and timing, the temperature difference

between the detector and the guide may be canceled out at a transient moment. But the optical system of the thermometer is actually not stayed on the thermal equivalent condition and the compensation value may not be correct.

SUMMARY OF THE INVENTION

[0007] The primary object of the present invention is to provide an infrared radiation ear thermometer. It is used to read the clinical temperature from the external ear canal with high precision and without waiting for the isothermal condition when the thermometer suffers a rapid ambient temperature change.

[0008] The other object of the present invention is to provide a more simple and efficient method to produce an offset. The offset is used to eliminate the temperature reading error arose from the difference among the ambient temperature, the infrared detector, and the optical system; therefore, the accuracy of the infrared radiation ear thermometer is maintained.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] **FIG. 1** is a cross-sectional view of the preferred embodiment showing an internal structure of the present invention.

[0010] **FIG. 2** is a cutaway view of the infrared detector in **FIG. 1**.

[0011] **FIG. 3** is block diagram of the present invention showing signals processing.

[0012] **FIG. 4** is a cross-sectional view of the test and experiment embodiment that has three temperature reference sensors to develop the algorithm for correcting the measure error caused by instantly ambient change.

[0013] **FIG. 5** is a graph showing the rapid ambient temperature change which the test and experiment embodiment of **FIG. 4** suffers.

[0014] **FIG. 6** is a graph showing the different temperature change curves from the three sensors in the test and experiment embodiment.

[0015] **FIG. 7** is a graph showing the slope change at different time after a rapid temperature change.

[0016] **FIG. 8** is a graph showing the test and experiment embodiment suffers two different rapid ambient temperature increasing sections.

[0017] **FIG. 9** is a graph showing the test and experiment embodiment suffers a rapid ambient temperature increasing section and decreasing section.

[0018] **FIG. 10** is graph showing the infrared radiation path for the calculation of the offset when the temperature of the detector element irradiation different from that of the optical-guide.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0019] According to the one of embodiments' cross-sectional view of the present invention showing in **FIG. 1**, there are a housing **1**, an infrared detector **11**, an optical-guide **12**, an ambient temperature sensor **13**, a signal processing section **14**, and a display unit **15**. Wherein, optical-guide **12**

is mounted with one end directed to collect infrared radiation from a measured target **31** as shown in **FIG. 3**. The other end of optical-guide **12** connects with infrared detector **11**. Infrared detector **11** (as shown in **FIG. 3**) transmits the electric signal converted from infrared radiation to signal processing section **14**. Ambient temperature sensor **13** is set in the space near the optical system (optical-guide **12** and infrared detector **11**) to sense the ambient temperature change. Ambient temperature sensor **13** converts the ambient change into electric signal and transmits the signal to signal processing section **14** (as shown in **FIG. 3**). Display unit **15** is mounted on the housing to show the temperature reading after the signals from infrared detector **11** and ambient temperature sensor **13** are processed by signal processing section **14** (as shown in **FIG. 3**). In addition, infrared detector **11** comprises an infrared sensor element **111** and a temperature reference sensor **112**, wherein temperature reference sensor **112** is used to detect the substrate **114** temperature of the infrared detector **11**.

[0020] The following is the derivation of algorithm of the temperature offset method.

[0021] According **FIG. 4**, the test method with a test and experiment embodiment of the present invention that has three temperature reference sensors, THR_{wg} , THR_{can} and THR_{air} . If the infrared radiation ear thermometer suffers from an ambient temperature change from T_a to T_a+T_0 , the temperature reference sensor THR_{air} **43** in the space near the optical system (optical-guide **12** and infrared detector **11**) is assumed to have a heat capacitance C_{air} and heat conductance G_{air} from the ambient. The heat capacity is defined by

$$C_{air}=dQ/dT \quad (1)$$

[0022] Where dQ is the additional heat stored when its temperature is changed by an amount dT . The thermal conductance G_{air} is defined by the relation

$$P1=G_{air}*((T0+Ta)*u(t)-T(t)) \quad (2)$$

[0023] Where $P1$ is the heat flow from the ambient to the thermometer and $u(t)$ is the step function. The temperature of THR_{air} **43** is governed by

$$C_{air}*dT(t)/dt=P1*u(t) \quad (3)$$

[0024] Use (2) to replace $P1$

$$C_{air}*dT(t)/dt+G_{air}*T(t)=G_{air}*(T0+Ta)*u(t) \quad (4)$$

[0025] Use Laplace transform to get the solution

$$C_{air}*(s*T(s)-T0)+G_{air}*T(s)=G_{air}*(T0+Ta)/s \quad (5)$$

[0026] From (4)

$$T(s)=Ta/(s+G_{air}/C_{air})+((T0+Ta)*G_{air}/C_{air})/(s*(s+G_{air}/C_{air})) \quad (6)$$

[0027] Let $G_{air}/C_{air}=1/(\tau_{air})$, the solution of $T(t)$ is derived from the inverse Laplace transform of (6) and drew in **FIG. 5**

$$T_{air}(t)=T0*(1-\exp(-t/(\tau_{air}))) + Ta \quad (7)$$

[0028] Where τ_{air} is the thermal time constant of the space near the optical system (THR_{air} **43**) that can be derived from experiment and test.

[0029] The following is the description of the test method with a test and experiment embodiment (as shown in **FIG. 4**) that has three temperature reference sensors, THR_{wg} , THR_{can} and THR_{air} , mounted separately in three different positions: (1) the front end of the optical-guide **12** (THR_{wg}

designated as **41**); (2) the metal can wall of the infrared detector **11** (THR_{can} designated as **42**); (3) the space near the optical system (optical-guide **12** and infrared detector **11**) of the thermometer (THR_{air} designate as **43**).

[0030] First, put the thermometer into an $18^\circ C$. (T_a) constant temperature chamber for at least 1 hours to establish a thermal equilibrium condition. Second, take the thermometer out from the $18^\circ C$. chamber. Then, place it into another constant temperature chamber at $28^\circ C$. (T_a+T_0) immediately. The humidity of the chambers must be watched out to avoid the condensation. Record the changes of temperature from all temperature reference sensors, THR_{wg} **41**, THR_{can} **42** and THR_{air} **43**, for 1 hour per sampling rate of 2-20 times per sec. The changes are drawn as temperature changing curves as shown in **FIG. 6**. From the changes, the thermal time constants of temperature reference sensors, THR_{wg} **41**, THR_{can} **42** and THR_{air} **43**, are derived and represented as τ_{wg} and τ_{can} and τ_{air} respectively.

[0031] Because $T_{air}(t)$, τ_{air} and T_a are known variables, the rapid ambient temperature change T_0 can be calculated from formula (7). Apply the same theory to the positions near optical-guide **12** (Where the temperature sensor THR_{wg} **41** is positioned) and infrared detector metal can **113** (Where the temperature sensor THR_{can} **42** is positioned) where there are radiation exchanges with infrared detector element **111** when the thermometer is susceptible to the rapid ambient temperature change. We have the mathematical solution of the above temperatures.

$$T_{can}(t)=T0*(1-\exp(-t/(\tau_{can}))) + Ta \quad (8)$$

$$T_{wg}(t)=T0*(1-\exp(-t/(\tau_{wg}))) + Ta \quad (9)$$

[0032] Where $T_{can}(t)$ and $T_{wg}(t)$ are the temperatures of infrared detector metal can **113** and optical-guide **12**, while τ_{can} and τ_{wg} are their thermal time constants respectively. The τ_{can} and τ_{wg} are also derived from the same experiment and test embodiment as the τ_{air} . From formula (7), (8) and (9), the temperature of infrared detector **11** and optical-guide **12** are calculated even no real reference temperature sensor is placed on.

[0033] For real operation environment, the ambient changes are random both on direction and timing. Formula (4) must be rewritten as

$$C_{air}*dT(t)/dt+G_{air}*T(t)=G_{air}*((Ta+T0)*u(t)-(Ta+T0)*u(t-t1)+(Ta+T1)*u(t-t2)-(Ta+T1)*u(t-t2)-T2)*u(t-t2)- \quad (10)$$

$$C_{air}*dT(t)/dt+G_{air}*T(t)=G_{air}*((Ta+T0)*u(t)+\sum(n=1\sim N)((Tn-Tn-1)*u(t-tn))) \quad (11)$$

[0034] Where Tn may be positive or negative.

[0035] Use the Laplace transform and the principle of superposition, the temperature $T_{air}(t)$ can be solved as

$$T_{air}(t)=Ta+T0*(1-\exp(-t/(\tau_{air}))) + \sum(n=1\sim N)((Tn-Tn-1)*\tau_{air}*(1-\exp(-t-tn)/(\tau_{air}))) * u(t-tn) \quad (12)$$

[0036] Where $T_{air}(t)$, τ_{air} and Ta are known constant. $T_0\sim Tn$ can be calculated if tn is also a known constant. The method to get the random timing tn will be described below.

[0037] First, consider a simple condition where the thermometer of the test and experiment embodiment (as shown in **FIG. 4**) suffers only one rapid temperature changes T_0 at time $t=0$ as formula (7). Before time $t=0$, the thermometer is kept under an isothermal condition at temperature Ta . The signal processing section of the thermometer measures the

temperature $T_{air}(t)$ and its slope $dT_{air}(t)/dt$ constantly after the thermometer is powered on. The time derivative of $T_{air}(t)$ is

$$dT_{air}(t)/dt=(T_0/\tau_{air})\cdot\exp(-t/\tau_{air}) \quad (13)$$

[0038] While the thermal time constant τ_{air} is smaller than τ_{can} and τ_{wg} and τ_{sen} , (the time constant of the temperature reference sensor **112**) the speed of the response and the detectability to the rapid temperature change of THR_{air} **43** is faster and larger than THR_{can} **42**, THR_{wg} **41** or THR_{sen} **112** at $t=0$. That is why we use the time derivative of $T_{air}(t)$ as the criterion of judging whether the ambient temperature of the thermometer is changing too fast or not. When the slope of $T_{air}(t)$ is larger than a predetermined value (say $3/\tau_{air}$), the thermometer must be susceptible to a rapid ambient temperature change and the time is set to $t=0$ as shown in **FIG. 5**. As time going from $t=0$, the slope of $T_{air}(t)$ as shown in **FIG. 7** is getting smaller and finally reaching to zero from formula (13). When the time is larger than a predetermined value, say 10 times the thermal time constant τ_{air} , the slope of $T_{air}(t)$ is closing to zero and another isothermal condition is achieved at temperature, T_a+T_0 , because all the temperature $T_{air}(t)$, T_{sen} , $T_{can}(t)$ and $T_{wg}(t)$ are the same as shown in **FIG. 6**. If at time $t=t1$ the ambient changes from T_a+T_0 to T_a+T1 , $T_{air}(t)$ is governed by setting $N=1$ in formula (12).

$$T_{air}(t)=T_a+T_0\cdot(1-\exp(-t/(\tau_{air})))+(T1-T_0)\cdot(1-\exp(-\frac{t-t1}{\tau_{air}}))\cdot u(t-t1) \quad (14)$$

[0039] There are two cases should be taken into account. The first case is $T1>T0$ as shown in **FIG. 8**. The value of $dT_{air}(t)/dt$ will be increased at time $t=t1$ rather than decreasing as described above. The timer for 10 times τ_{air} will be reset and recount from zero. $T1$ is calculated mathematically because $T_{air}(t)$, T_a , T_0 and τ_{air} are known. In the other case of $T1<T0$ (including $T1<0$), the sign of the slope of $T_{air}(t)$ will change from positive to negative at $t1$ as shown in **FIG. 9**. For all the cases described above, whether and when ($t_0 \dots t_n$) the thermometer is susceptible to rapid temperature changes can be easily recognized from the time derivative of $T_{air}(t)$ (the slope of $T_{air}(t)$). The amplitudes ($T_0 \dots T_n$) of the ambient temperature interferences are also solved from the mathematical formula (12). Substitute τ_{air} by τ_{can} and τ_{wg} , the mathematical solutions of both $T_{can}(t)$ and $T_{wg}(t)$ are derived from formula (12). The effect on the accuracy of the thermometer of the temperature differences between T_{sen} , T_{can} and T_{wg} under non-isothermal condition and the calculation of the offset will be discussed below.

[0040] As described in the above paragraph, the temperature of both metal can wall of the infrared detector **11** ($T_{can}(t)$) and optical-guide **12** ($T_{wg}(t)$) can be calculated mathematically from the temperature measured by a reference sensor (ambient temperature sensor **13** as shown in **FIG. 1**) near the optical system (optical-guide **12** and infrared detector **11**) ($T_{air}(t)$), its time derivative ($dT_{air}(t)/dt$) and the known time constant τ_{can} and τ_{wg} while both are derived from the above experiment.

[0041] First, consider the temperature difference between optical-guide **12** and infrared detector element **111**.

[0042] As shown in **FIG. 10**, assume the irradiance $d\Phi$ from the target **101** with a radiance RA on the infrared detector element **111** with a small solid angle $d\Omega$ can be written as:

$$d\Phi=RA\cdot\cos(\theta r)\cdot d\Omega \quad (15)$$

[0043] From Stefan-Boltzmann law:

$$RA=(\sigma T^4/\pi)$$

[0044] We have

$$d\Phi=(\sigma T^4/\pi)\cdot\cos(\theta r)\cdot d\Omega \quad (16)$$

[0045] Where $d\Omega=2\cdot\pi\cdot\sin(\theta r)d\theta r$. Depend on the θr , the irradiance on the detector element **111** is reflected many times from the target **101** with the reflector (optical-guide **12**, in **FIG. 1**). The times of reflection Nf is a function of θr :

$$Nf(\theta r)=\text{floor}((\tan(\theta r)\cdot Ssp+Rwg)/(2\cdot Rwg)) \quad (17)$$

[0046] Where Ssp is the distance from infrared detector element **111** to tip of the optical-guide **12**, Rwg is the radius of the optical-guide **12**.

[0047] Here we introduce the emissivity, reflection and the transmission into the equation to get the net irradiance on the infrared detector **11**:

$$\Phi_{net}(\theta r, dT_{wg}, T_{tar})=\Phi_{ts}(\theta r, T_{tar})+\Phi_{ws}(\theta r, dT_{wg})-\Phi_{out}(\theta r) \quad (18)$$

[0048] Where Φ_{ts} is the irradiance from target to detector, Φ_{ws} is the irradiance from optical-guide **12**, Φ_{out} is the radiation outgoing from infrared detector **11** and T_{tar} is the temperature of the target **101**. These three items are derived from formulas (16) and (17) and written in detail:

$$\Phi_{ts}(\theta r, T_{tar})=2\cdot\pi\cdot\int_0^{\theta_{rx}}\sigma\cdot\cos(\theta r)\cdot\epsilon_s\cdot T_{tar}^4\cdot R_w^{N(\theta r,d)}\cdot\sin(\theta r)d\theta r \quad (19)$$

[0049] Where θ_{rx} is FOV of the detector, $\sigma=1-\tau_d/\pi$, τ_d is the transmission of the detector window, ϵ_s is the emissivity of the infrared detector element **111**, T_{tar} is the target temperature and $R_w=1-\epsilon_w$, the reflectivity of optical-guide **12** while ϵ_w is the emissivity of optical-guide **12**.

$$\Phi_{ws}(\theta r, dT_{wg})=2\pi\cdot\int_{\theta_0}^{\theta_{rx}}\sigma\cdot\cos(\theta r)\cdot\epsilon_w\cdot\epsilon_s\cdot(T_{sen}+dT_{wg})^4\cdot\sum_{n=1}^{Nf(\theta r,d)}R_w^{n-1}\cdot\sin(\theta r)d\theta r \quad (20)$$

[0050] Where $\theta_0=\text{atan}(Rwg/Ssp)$ is the maximum θr for zero reflection, dT_{wg} is the temperature difference between the sensor T_{sen} and optical-guide **12** T_{wg} , that is $T_{wg}=T_{sen}+dT_{wg}$.

$$\Phi_{out}(\theta r)=2\cdot\pi\cdot\int_0^{\theta_{rx}}\sigma\cdot\cos(\theta r)\cdot\epsilon_s\cdot T_{sen}^4\cdot\sin(\theta r)d\theta r \quad (21)$$

[0051] The measurement error arose from the temperature difference between infrared detector **11** and optical-guide **12** can be written as:

$$dT_{tar}/dT_{wg}=(d\Phi_{net}/dT_{wg})/(d\Phi_{net}/dT_{tar}) \quad (22)$$

[0052] From formulas (18), (19), (20), (21), and (22) and the design values of the constants (the constants are different from one thermometer to another), we have:

$$dT_{tar}/dT_{wg}=0.124 \quad (23)$$

[0053] The measurement error, i.e. the value to be compensated from the measuring result arose from dT_{wg} is 0.124°K . per 1°K . difference between infrared detector 11 and the optical-guide 12.

[0054] Apply the same theorem to the metal can, if the temperature of metal can wall of the infrared detector 11 is $T_{can}(t)$ which is different from the temperature of infrared detector element 111 $T_{sen}(t)$ under non-isothermal condition, the correcting value will be:

$$dT_{air}/d(T_{can})=0.456 \tag{24}$$

[0055] Where $dT_{can}=T_{can}-T_{sen}$, is the temperature difference between the detector temperature and the can temperature.

[0056] Therefore, from the above description, the offset can be calculated with one temperature sensor, ambient temperature sensor 13 (THR_{air}) instead of three temperature sensors, THR_{wg} , THR_{can} and THR_{air} , mounted separately in three different positions: (1) the front end of the optical-guide 12 (THR_{wg} designated as 41); (2) the metal can wall of the infrared detector 11 (THR_{can} designated as 42). Consequently, the present invention can be realized by the preferred embodiment with only an ambient temperature sensor.

[0057] Then the derived offset is used to compensate the measured temperature reading under non-isothermal condition.

[0058] While the invention has been described by way of example and in terms of a preferred embodiment, it is to be understood that the invention is not limited to the disclosed embodiment. To the contrary, it is intended to cover various modifications. Therefore, the scope of the appended claims should be accorded the broadest interpretation so as to encompass all such modifications.

What we claim is:

1. An infrared ear radiation thermometer comprising:
an optical system for receiving and collecting infrared radiation from the ear canal of patient;

an infrared detector including an infrared sensor to convert infrared radiation energy collected through said optical system into an electrical signal, and a temperature reference sensor built in the infrared detector to sense the substrate temperature of the substrate of the infrared detector;

an ambient temperature sensor for detecting the ambient temperature change;

a signal processing section collecting electric signals from the infrared sensor, the reference temperature sensor and the ambient temperature sensor for producing a offset by an algorithm to eliminate the affecting of temperature change;

a display unit for showing a temperature reading;

wherein, the offset produced by signal processing section that computes the signals from said multiple temperature reference sensors is to maintain the infrared ear radiation thermometer in high precision and make the thermometer be used without waiting isothermal condition.

2. An infrared radiation thermometer offset method comprising:

- a. Setting multiple sensors separately on the substrate of the infrared detector and in the space near the optical system to detect the difference between the ambient temperature and the infrared detector;

- b. Transferring these detected signals from said multiple sensors to a signal processing section;

- c. According these signals to produce an offset by an algorithm to compensate the thermometer reading error arose from the differences among the infrared detector, the optical system, and the ambient.

3. The infrared radiation thermometer offset method of claim 3, wherein setting using condition derives said algorithm from an experiment and test according to the real condition.

* * * * *

专利名称(译)	红外辐射耳温计和胶印法		
公开(公告)号	US20020191670A1	公开(公告)日	2002-12-19
申请号	US09/877354	申请日	2001-06-07
[标]申请(专利权)人(译)	黄玉简 TASO SIMON 翁VINCENT 常CHARLES 林一峰 陈ROGER 廖JASON		
申请(专利权)人(译)	黄玉简 TASO SIMON 翁VINCENT 常CHARLES 林凯文 陈ROGER 廖JASON		
当前申请(专利权)人(译)	黄玉简 TASO SIMON 翁VINCENT 常CHARLES 林凯文 陈ROGER 廖JASON		
[标]发明人	HUANG YU CHIEN TASO SIMON WENG VINCENT CHANG CHARLES LIN KEVIN CHEN ROGER LIAO JASON		
发明人	HUANG, YU CHIEN TASO, SIMON WENG, VINCENT CHANG, CHARLES LIN, KEVIN CHEN, ROGER LIAO, JASON		
IPC分类号	A61B5/01 G01J5/04 G01J5/06 G01J5/10 G01K13/00 A61B5/00 G01J5/08		
CPC分类号	G01J5/04 G01J5/049 G01J5/08 G01J2005/068 G01J5/10 G01J2005/0048 G01J5/0818		
外部链接	Espacenet USPTO		

摘要(译)

红外辐射耳温计具有光学系统，红外探测器，环境温度传感器和显示单元，信号处理部分。其中，红外探测器还包括红外传感器和温度参考传感器；红外传感器沉积在基板上，温度参考传感器安装在红外探测器的基板附近，以将红外信号转换成电信号并分别感测参考温度。环境温度传感器设置在光学系统附近的空间中，以检测环境温度的快速变化。信号处理部分接收来自这些温度传感器的

信号，以通过数学算法产生偏移。即使耳温计遭受极端温度变化，偏移也用于校正温度读数并保持高精度。

