



US 20080221418A1

(19) **United States**(12) **Patent Application Publication**
Al-Ali et al.(10) **Pub. No.: US 2008/0221418 A1**(43) **Pub. Date: Sep. 11, 2008**(54) **NONINVASIVE MULTI-PARAMETER
PATIENT MONITOR****Related U.S. Application Data**


(60) Provisional application No. 60/894,147, filed on Mar. 9, 2007.


Publication Classification(51) **Int. Cl.**
A61B 5/00 (2006.01)
(52) **U.S. Cl.** **600/324**
(57) **ABSTRACT**(75) Inventors: **Ammar Al-Ali**, Tustin, CA (US); **Joe E. Kiani**, Irvine, CA (US); **Ron Coverston**, Portola Hills, CA (US); **Mohamed Diab**, Ladera Ranch, CA (US); **Kristen LaRue**, Tustin, CA (US); **Russ Marable**, Rancho Santa Margarita, CA (US); **Greg Olson**, Trabuco Canyon, CA (US); **Roger Wu**, Irvine, CA (US); **Stephanie Miekko Doi Jones**, Woodinville, CA (US); **Rick Fishel**, Orange, CA (US)

Correspondence Address:

KNOBBE MARTENS OLSON & BEAR LLP
2040 MAIN STREET, FOURTEENTH FLOOR
IRVINE, CA 92614 (US)(73) Assignee: **Masimo Corporation**, Irvine, CA (US)(21) Appl. No.: **11/768,845**(22) Filed: **Jun. 26, 2007**

Embodiments of the present disclosure include a handheld multi-parameter patient monitor capable of determining multiple physiological parameters from the output of a light sensitive detector capable of detecting light attenuated by body tissue. For example, in an embodiment, the monitor is capable of advantageously and accurately displaying one or more of pulse rate, plethysmograph data, perfusion quality, signal confidence, and values of blood constituents in body tissue, including for example, arterial carbon monoxide saturation, methemoglobin saturation, total hemoglobin, arterial oxygen saturation, fractional arterial oxygen saturation, or the like. In an embodiment, the monitor advantageously includes a plurality of display modes enabling more parameter data to be displayed than the available physical display real estate. In an embodiment, the monitor advantageously includes a mode indicator to inform a user as to which parameter measurement would be displayed in one or more display areas upon actuation of a mode selector.

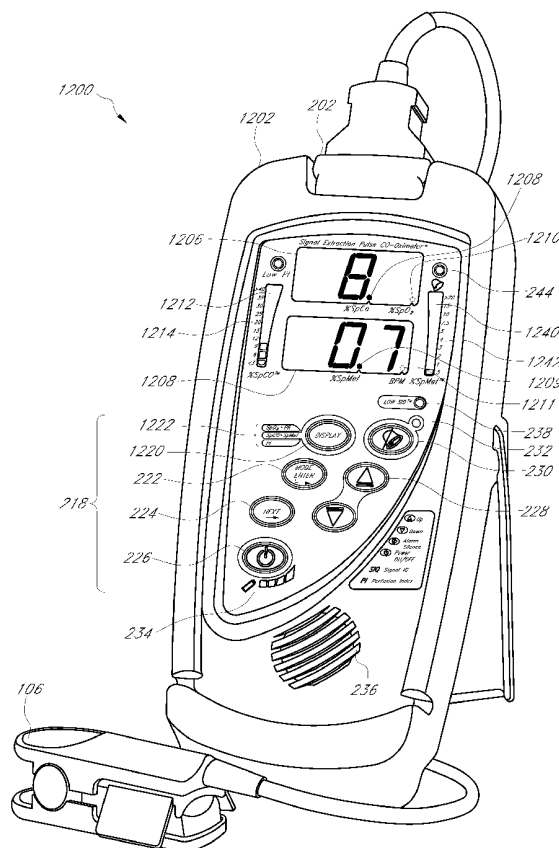

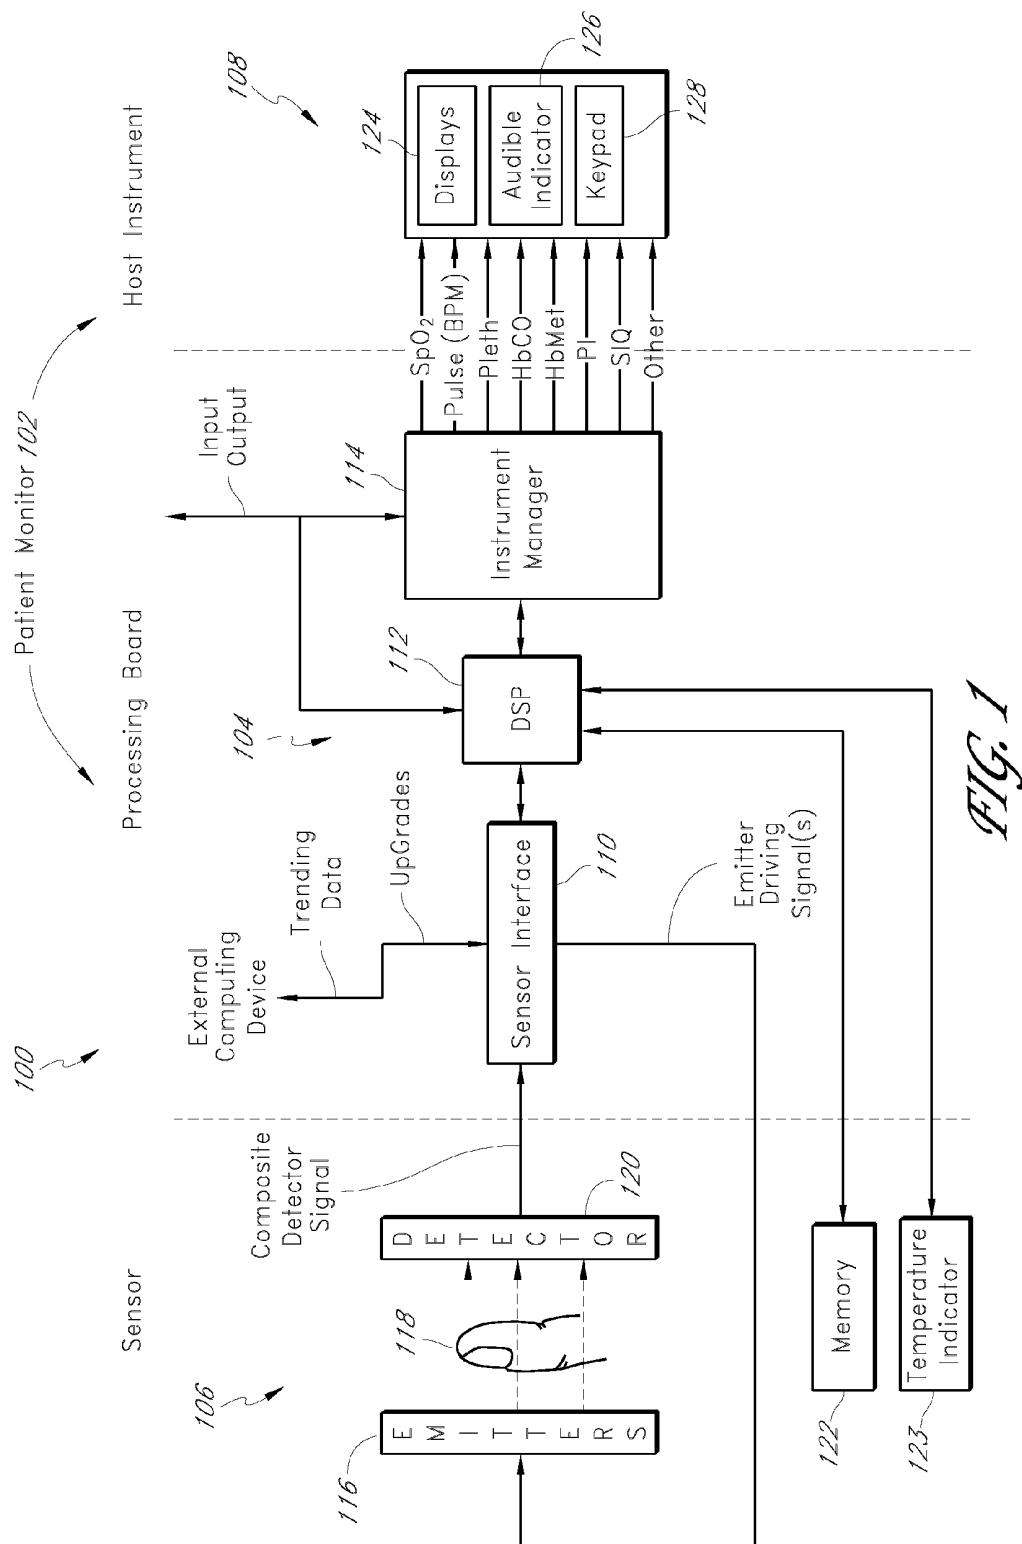

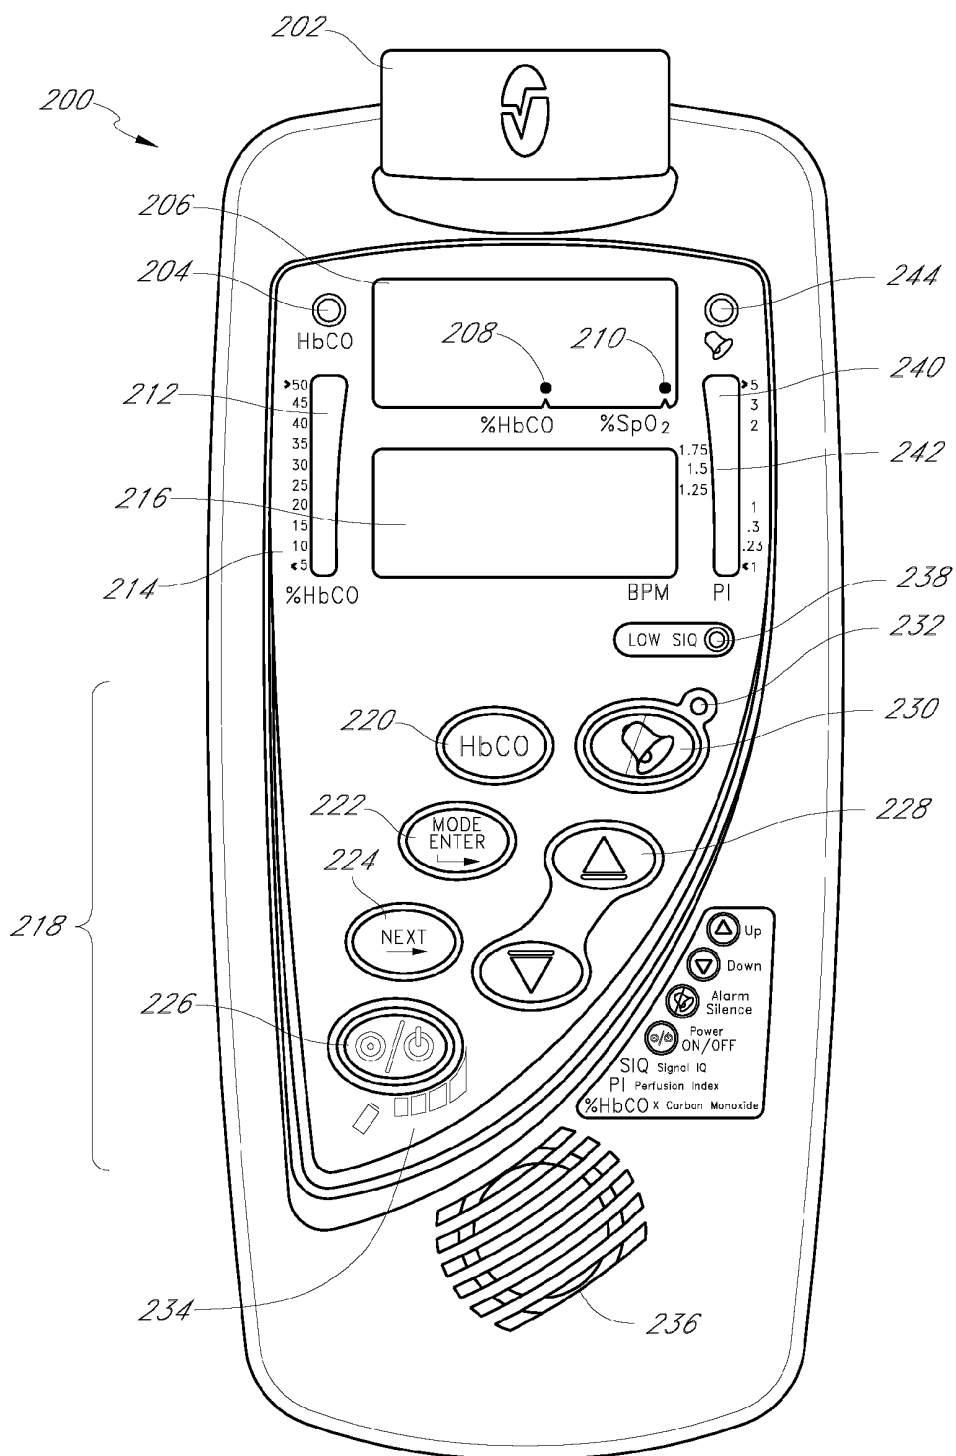


FIG. 2

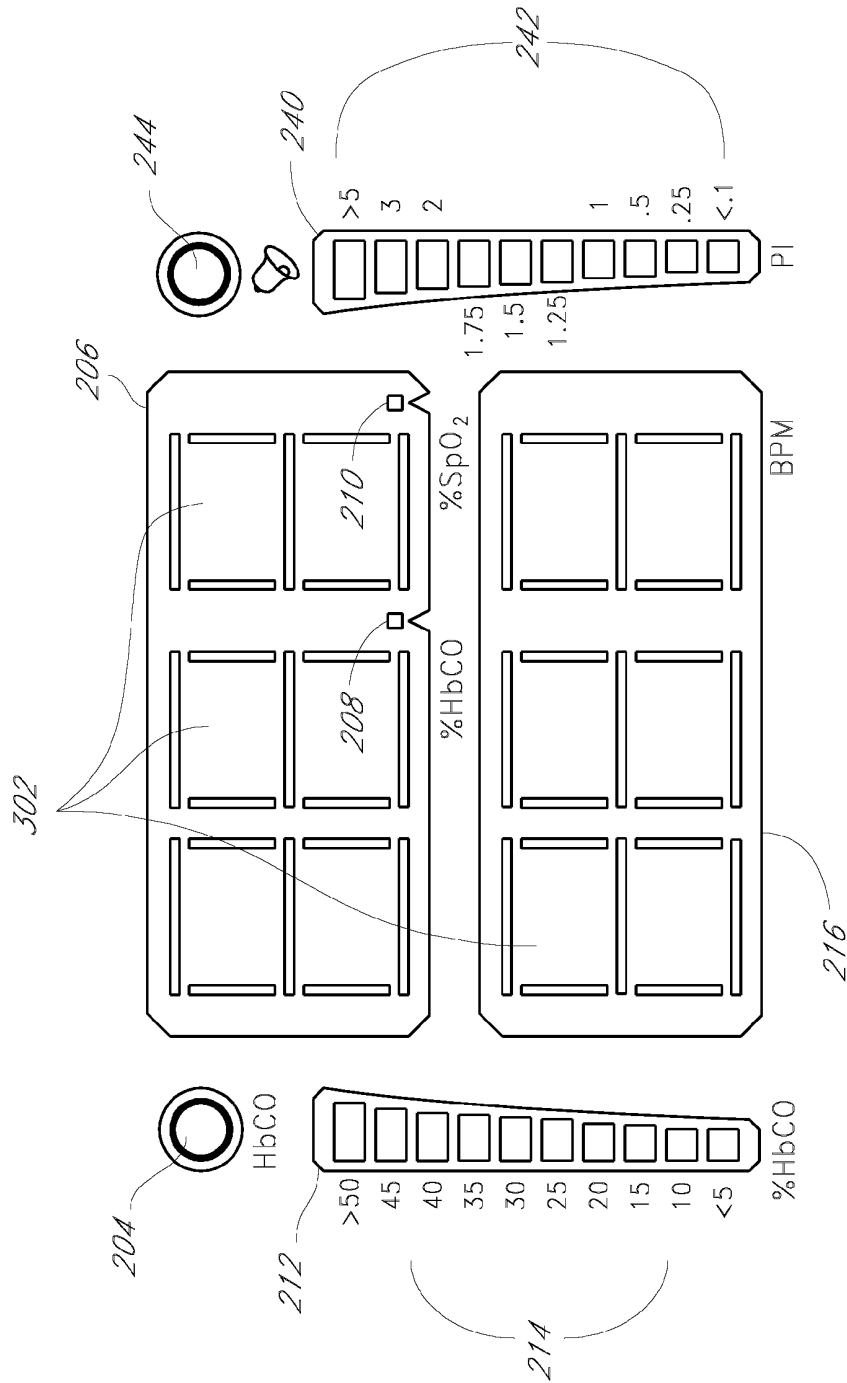


FIG. 3

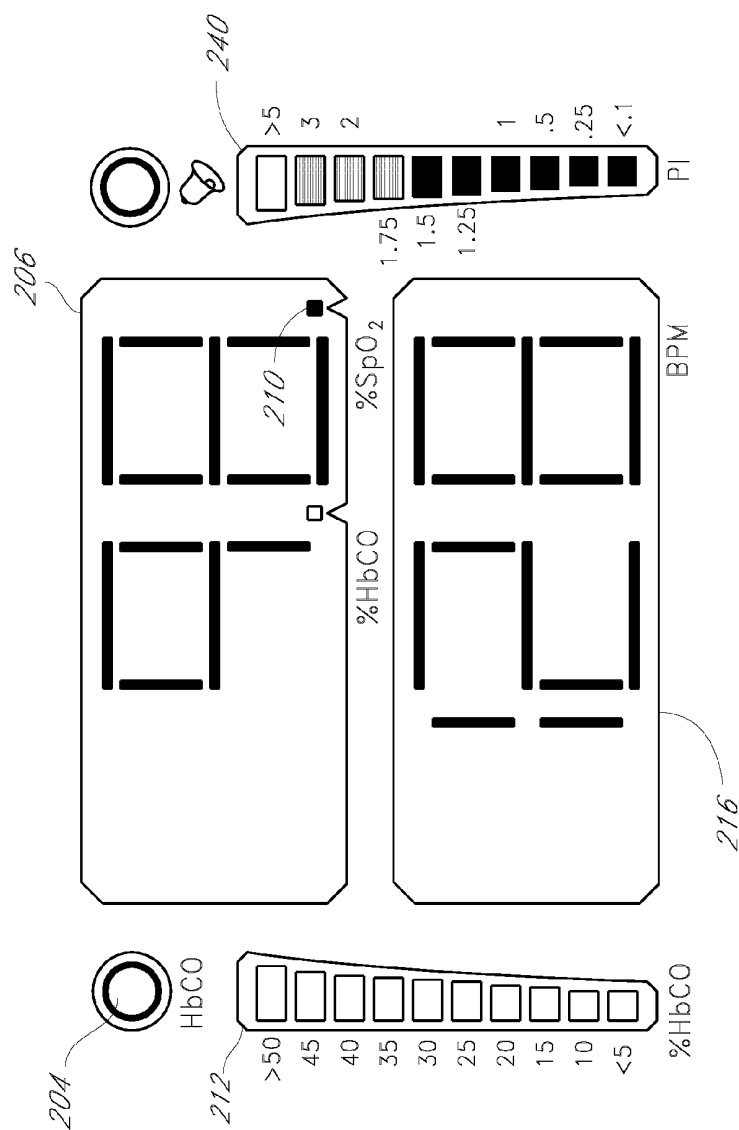


FIG. 4

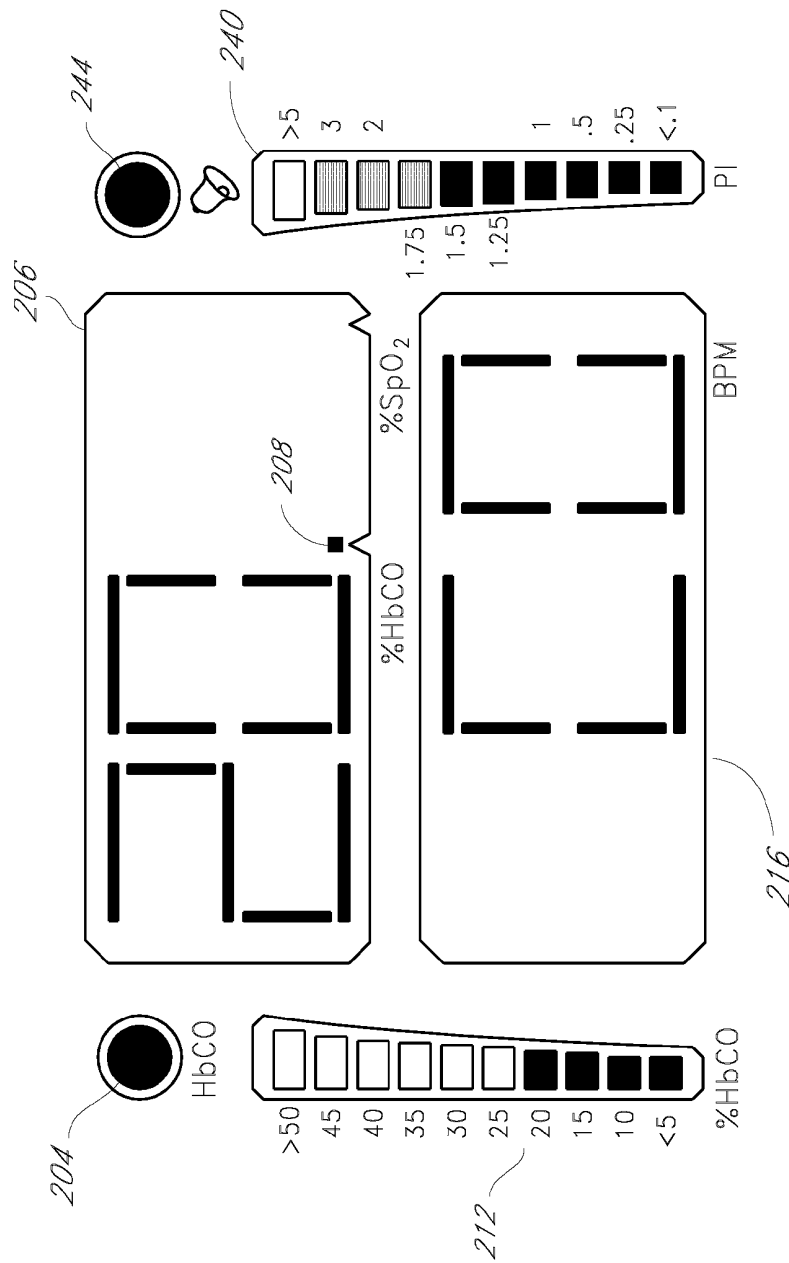


FIG. 5

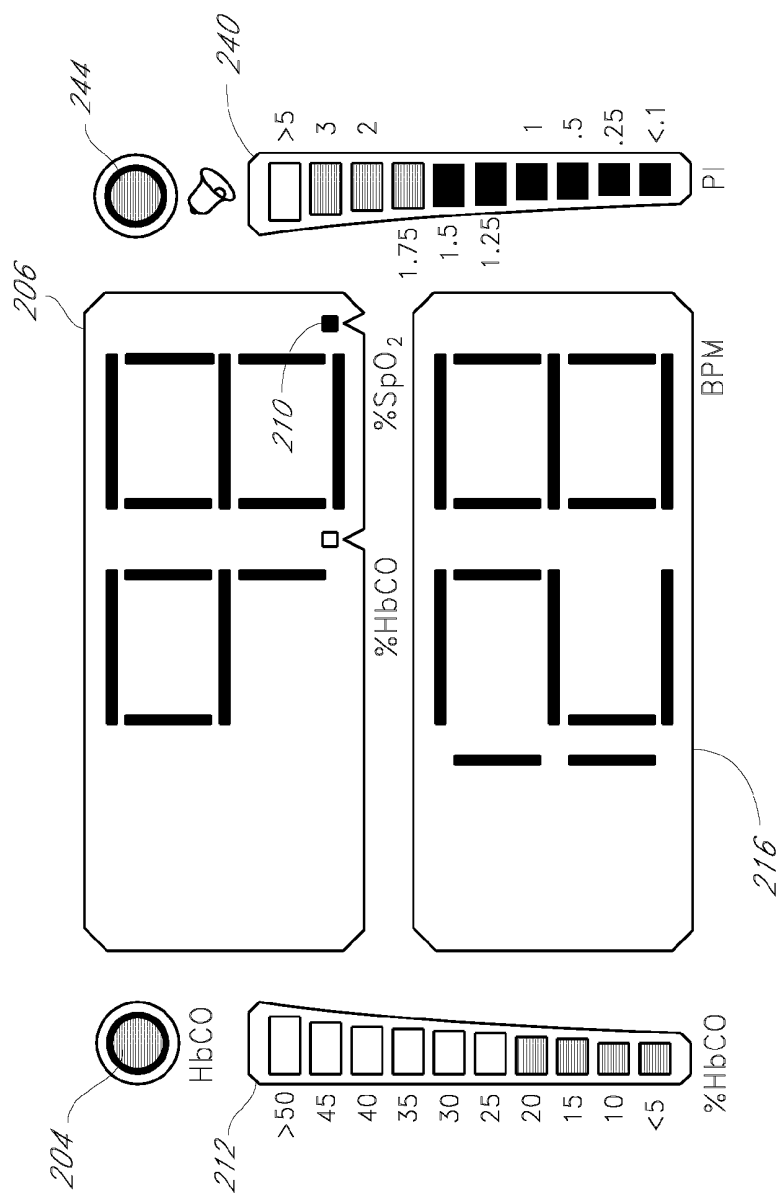


FIG. 6

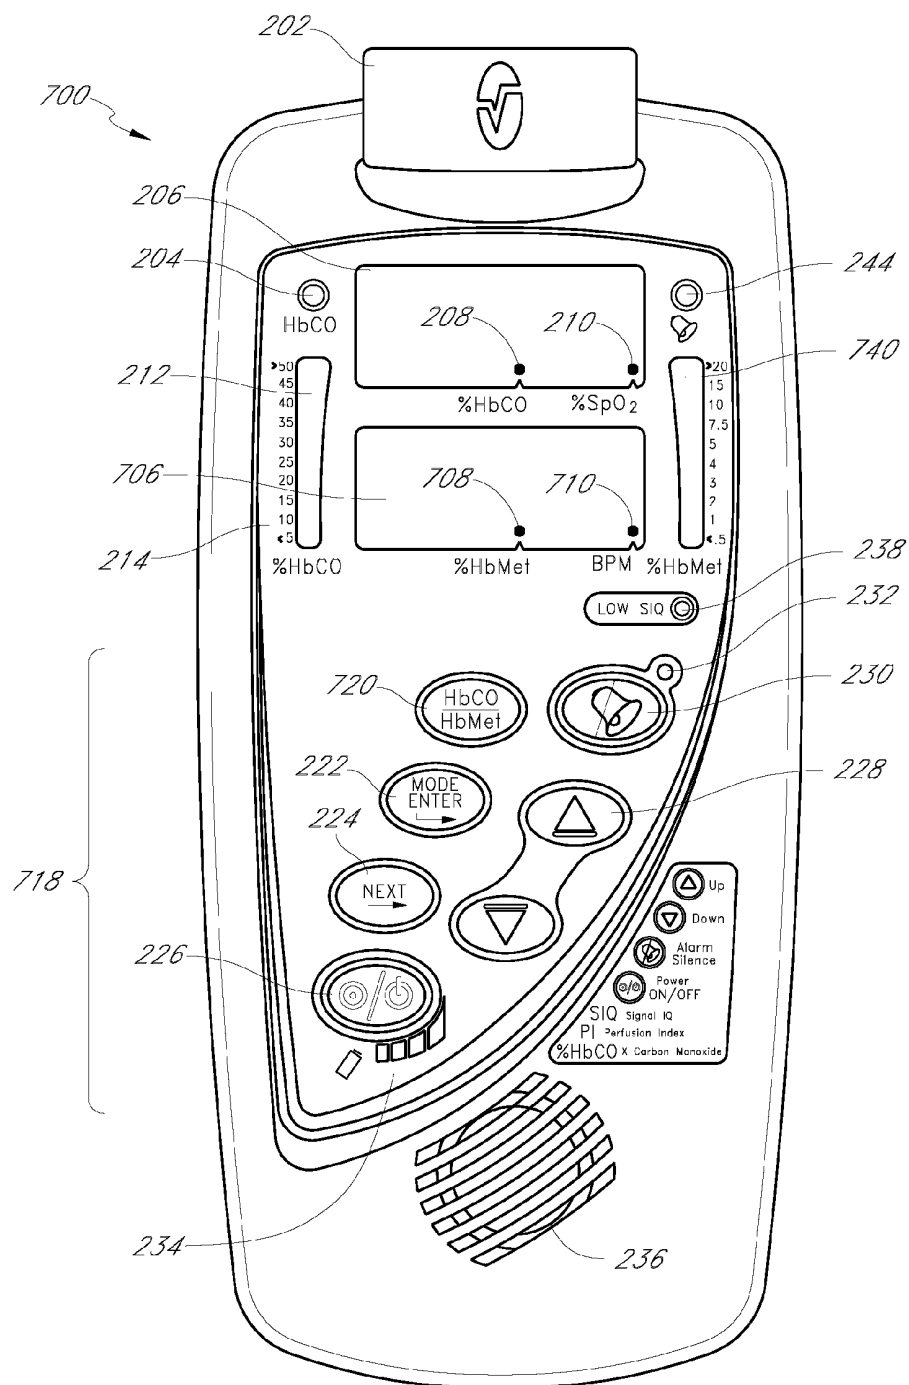


FIG. 7A

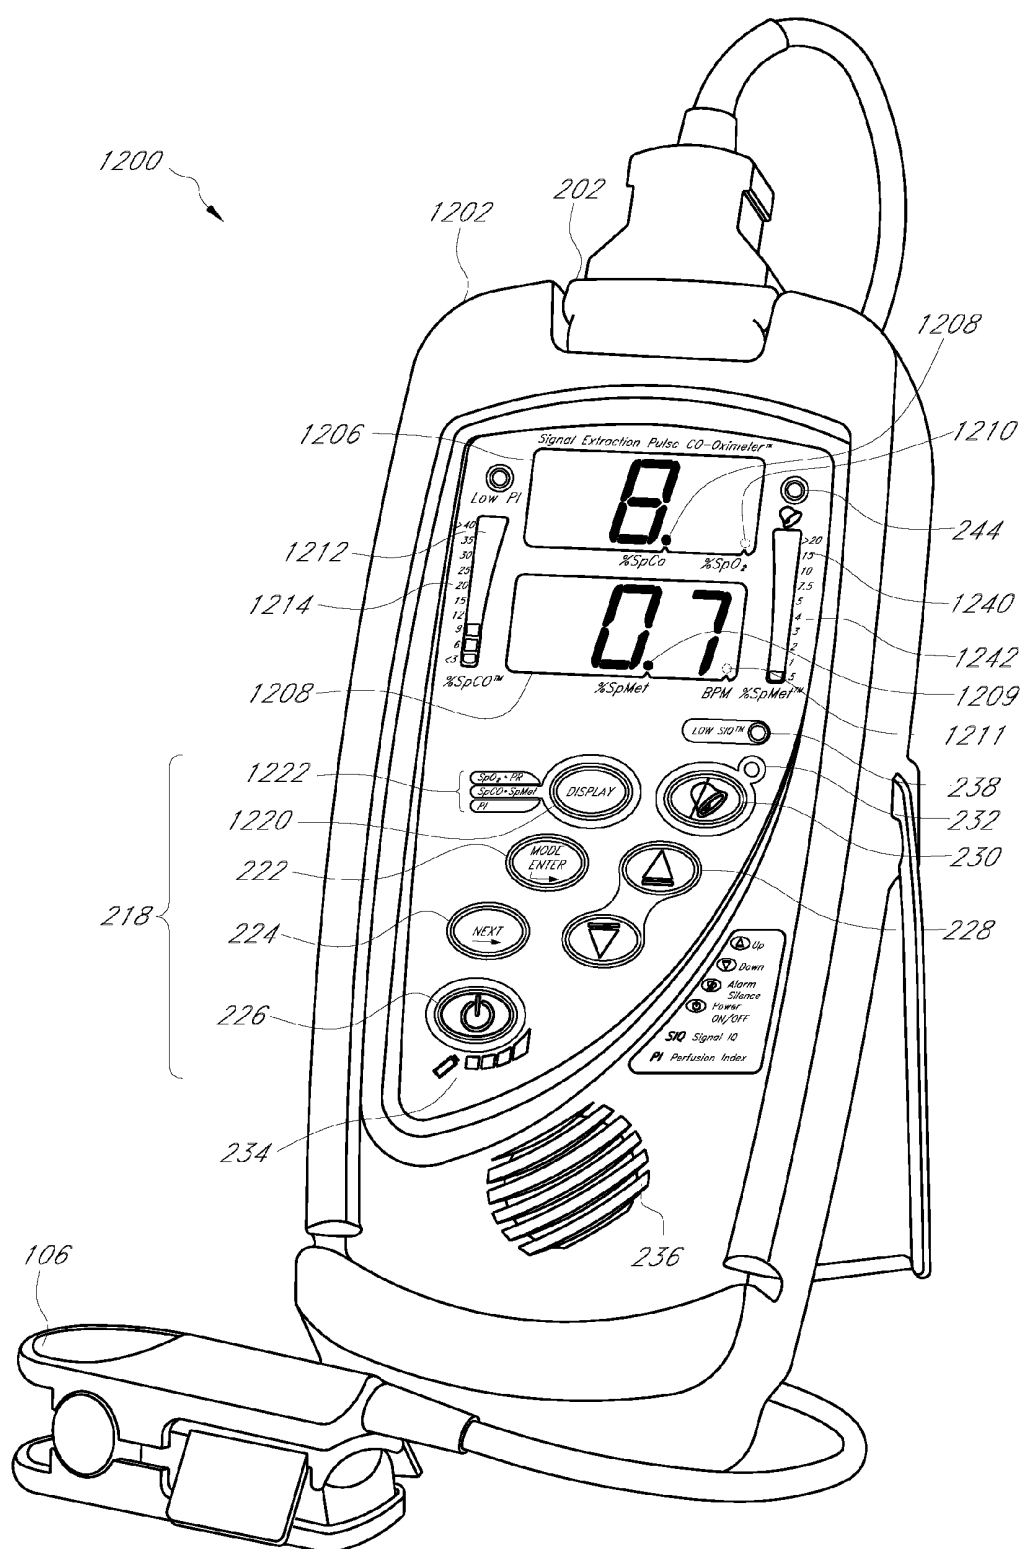


FIG. 7B

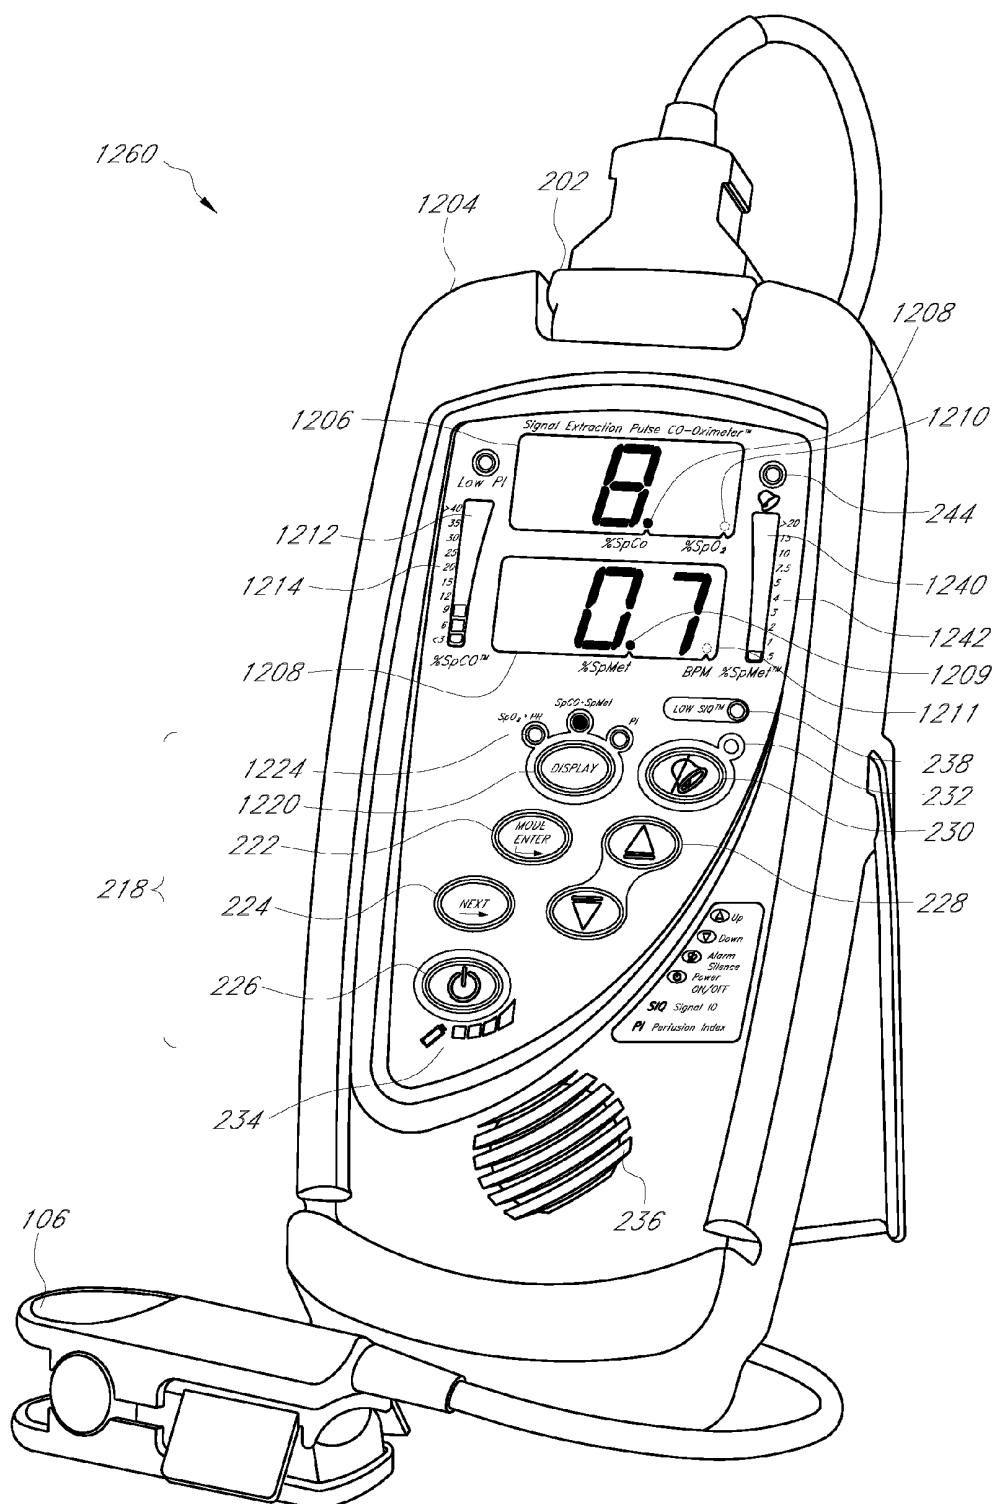


FIG. 7C

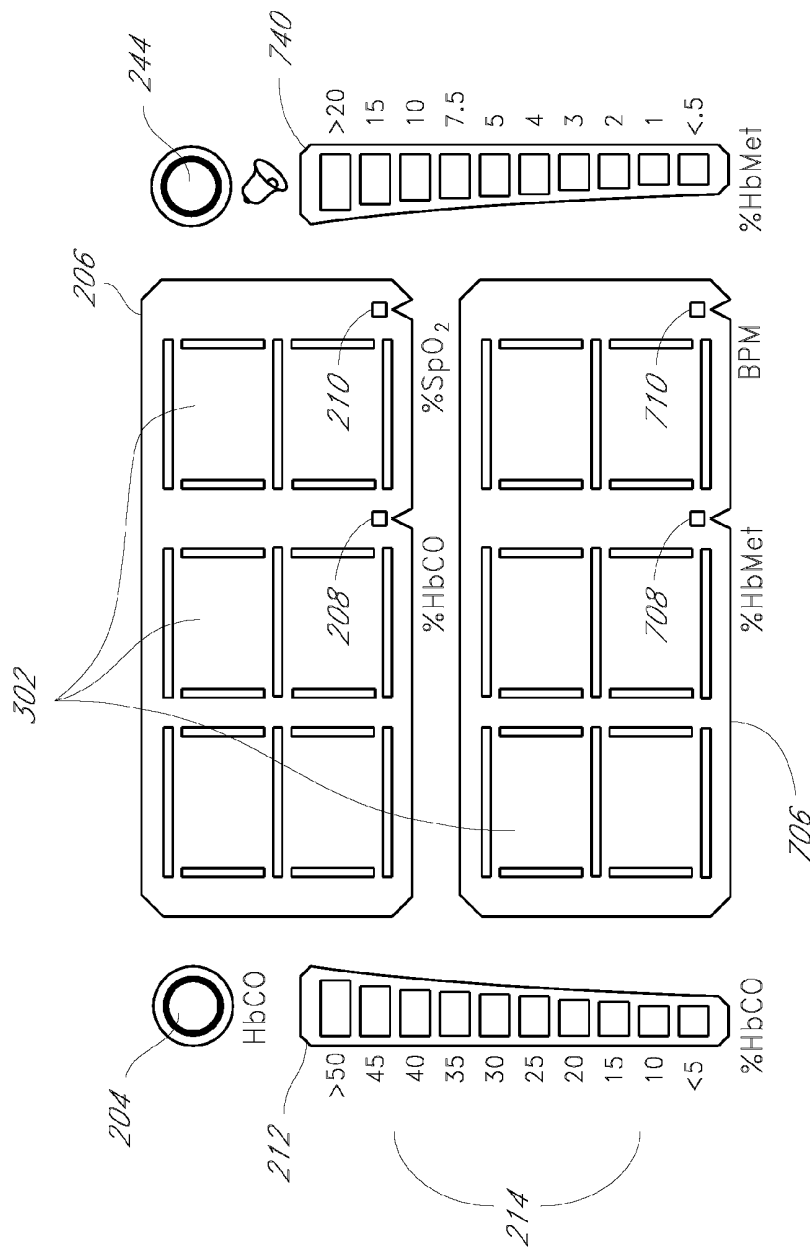


FIG. 8

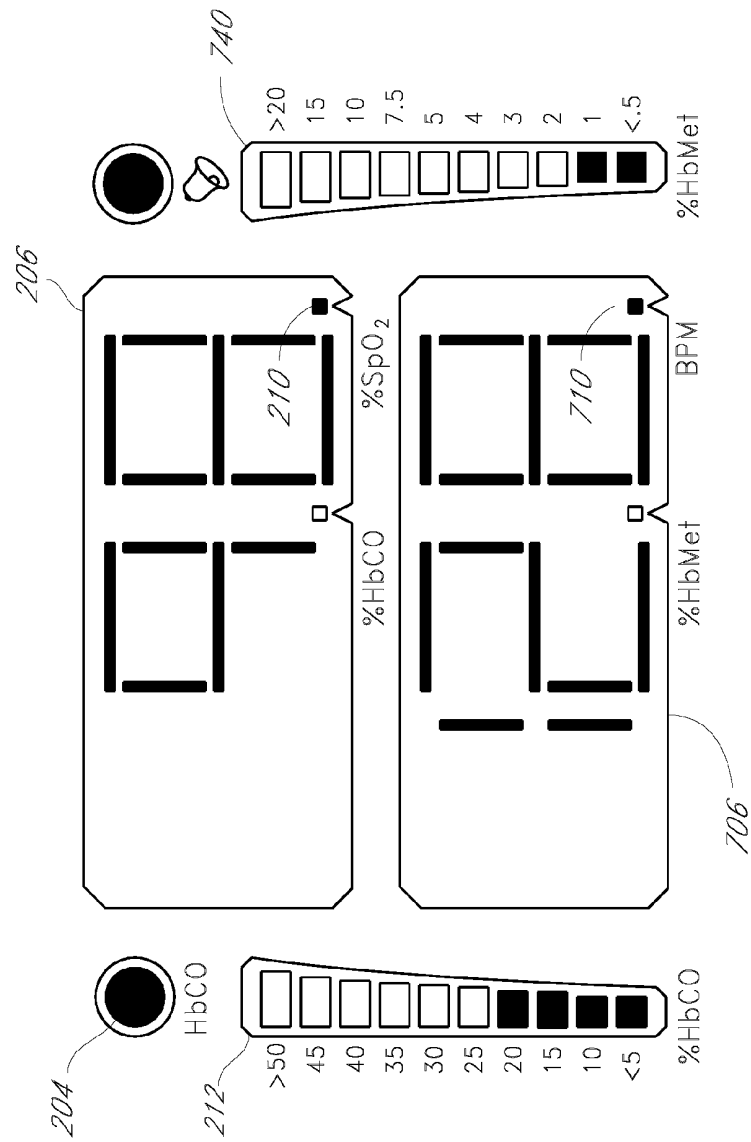


FIG. 9

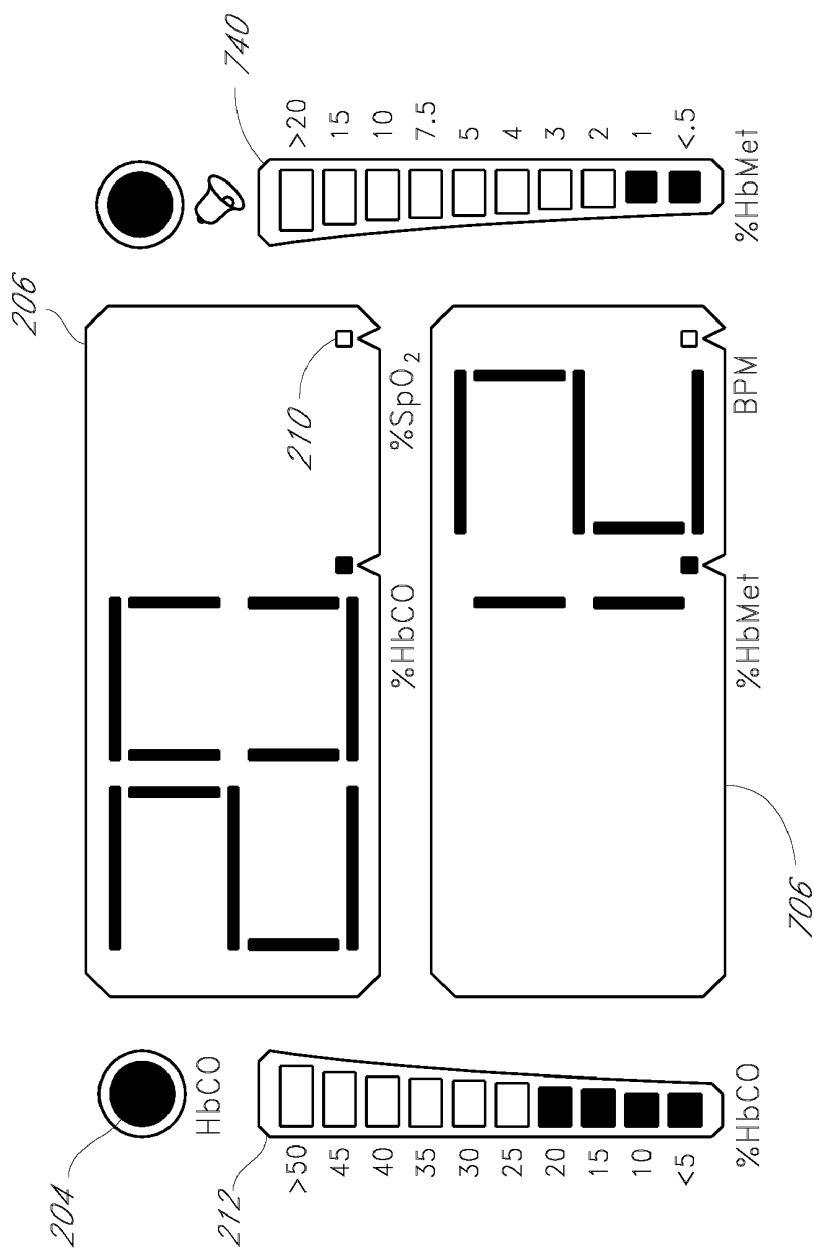


FIG. 10

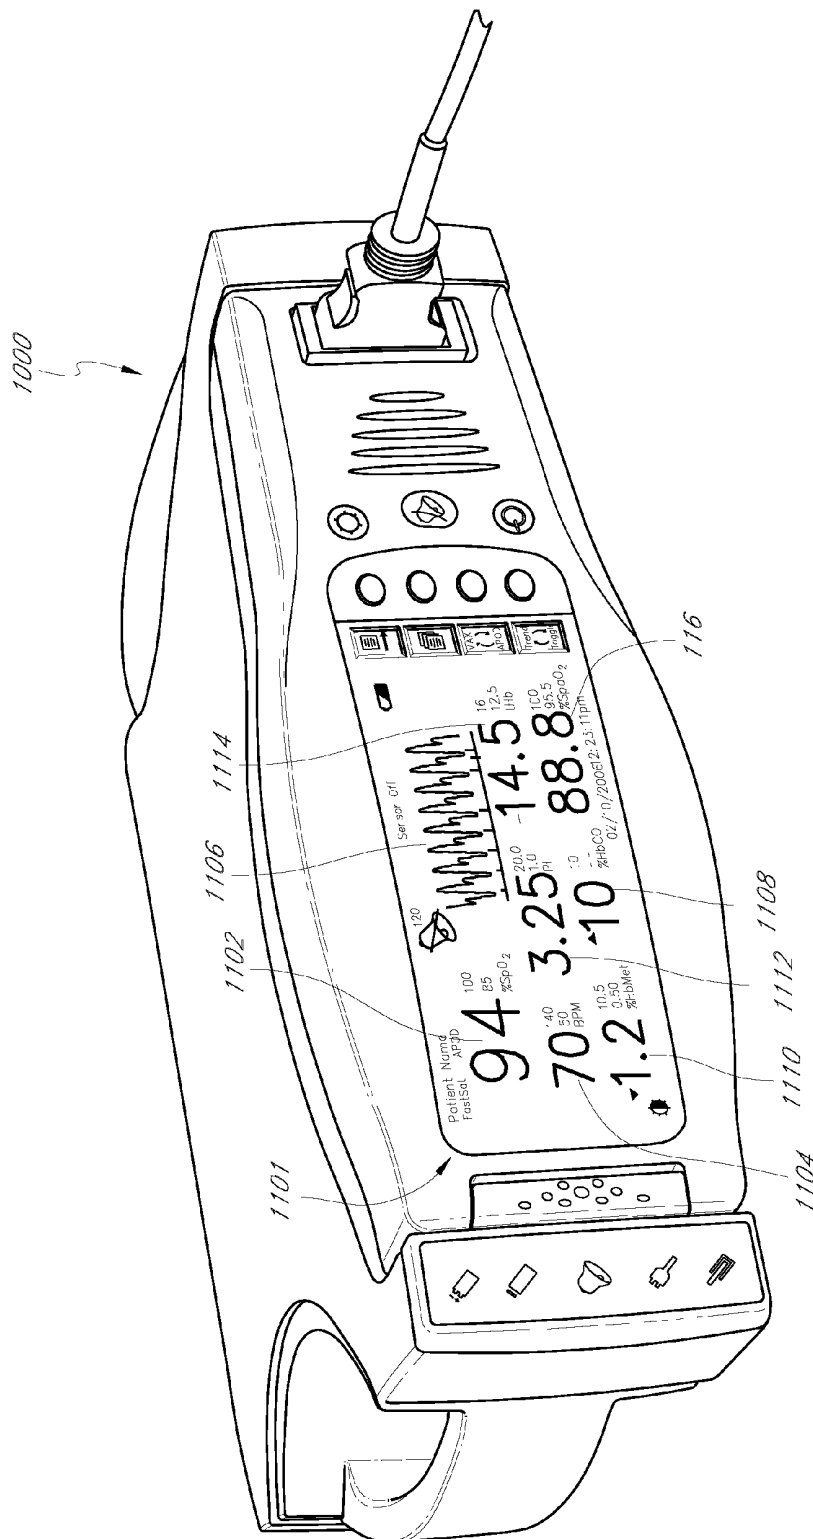


FIG. 11A

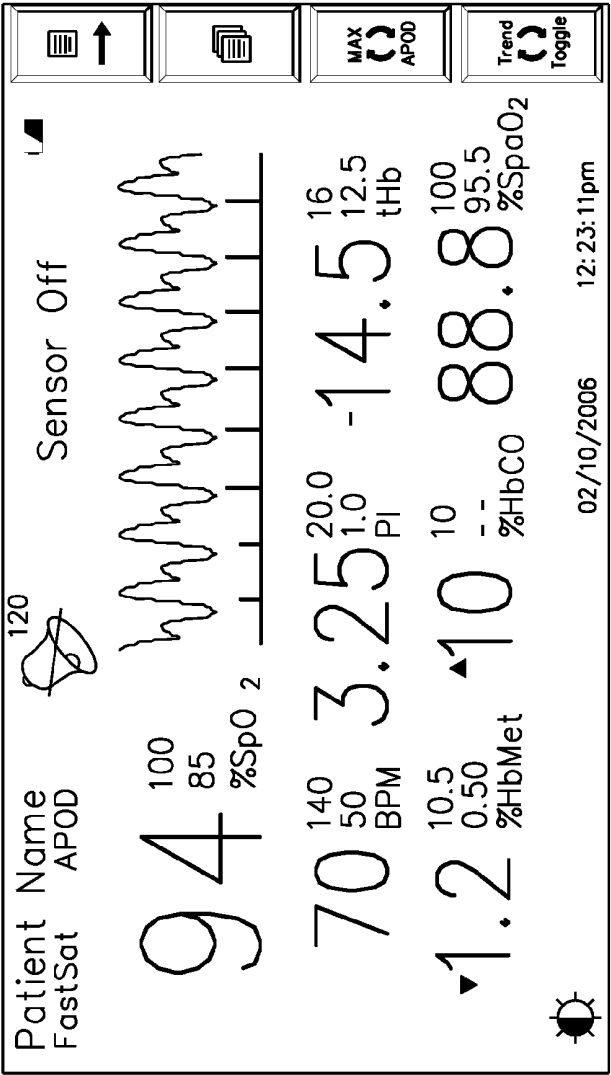


FIG. 11B

FIG. 11C

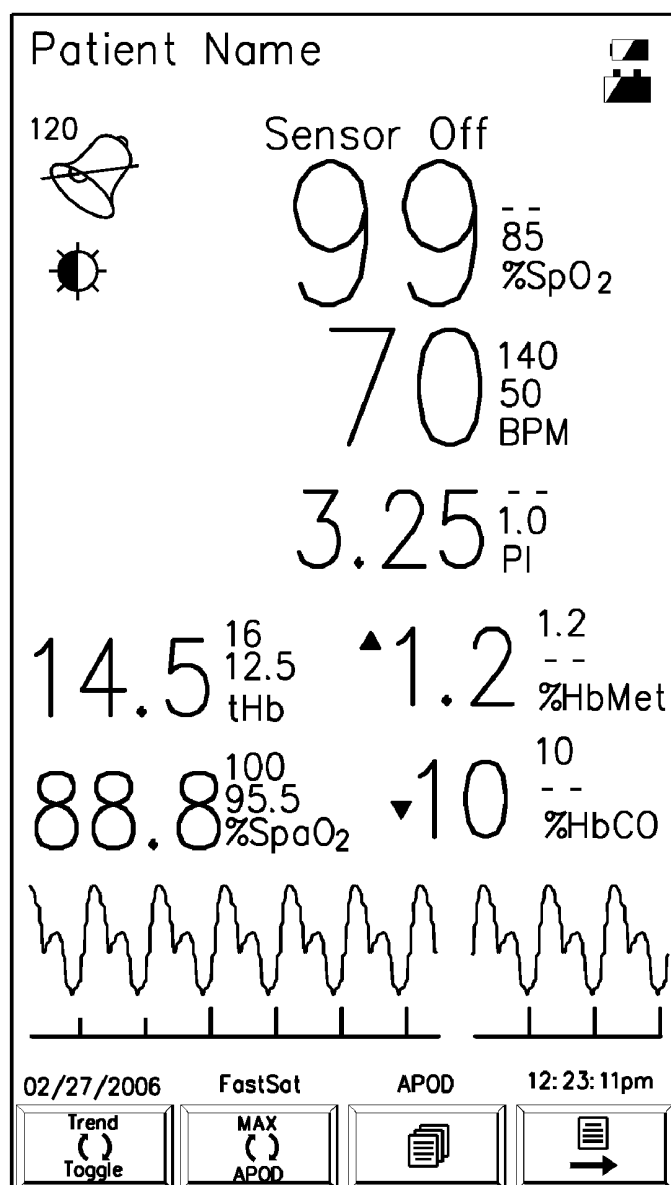


FIG. 11D

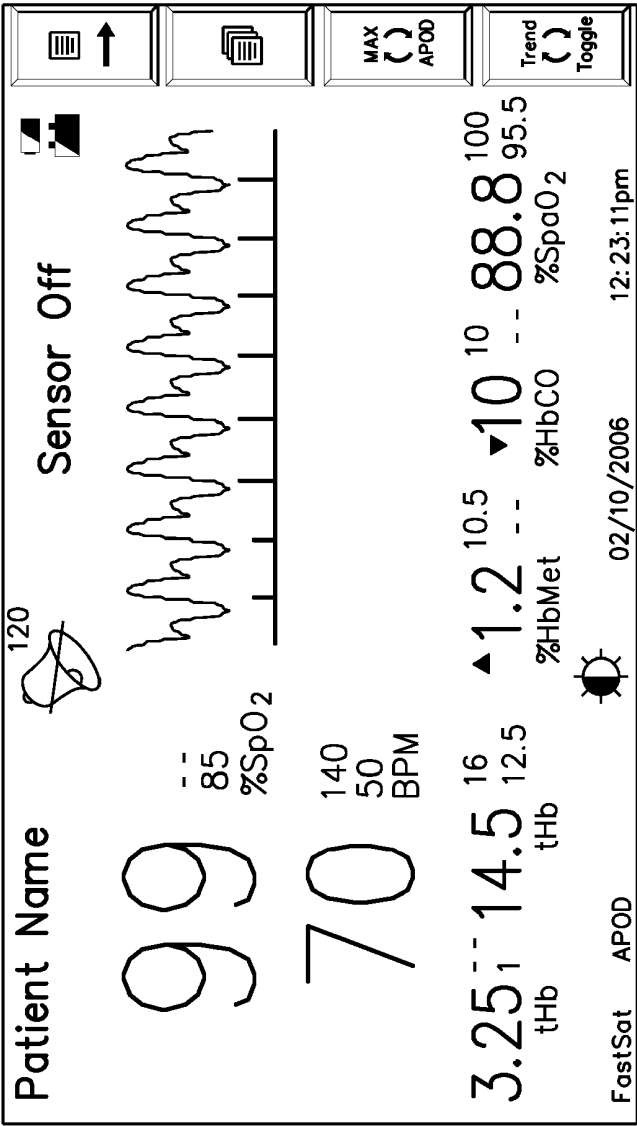


FIG. 11E

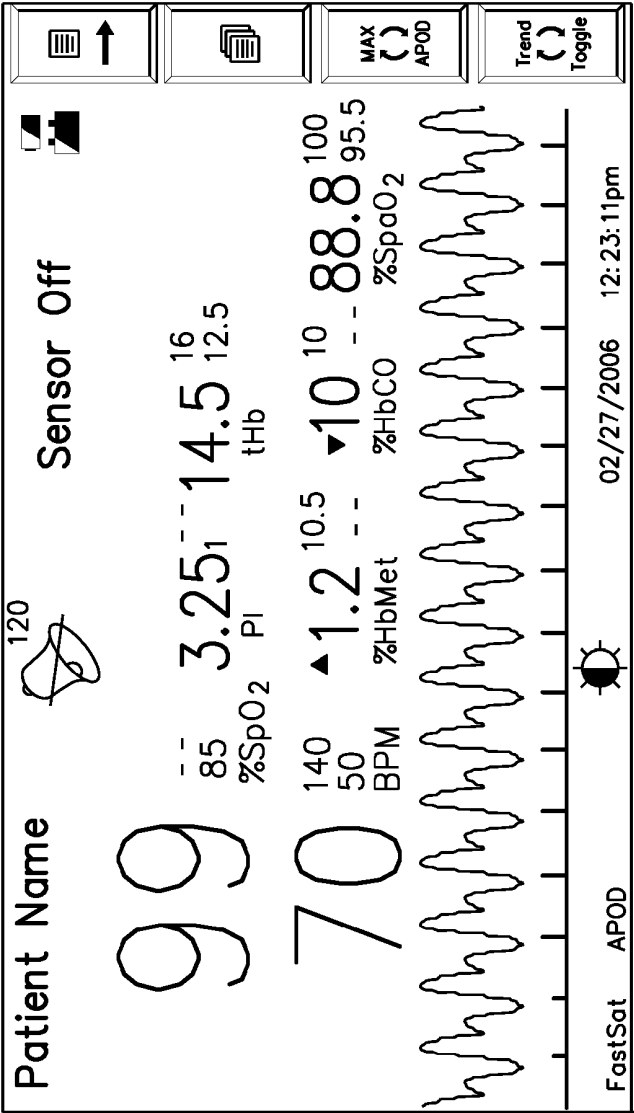


FIG. 11F

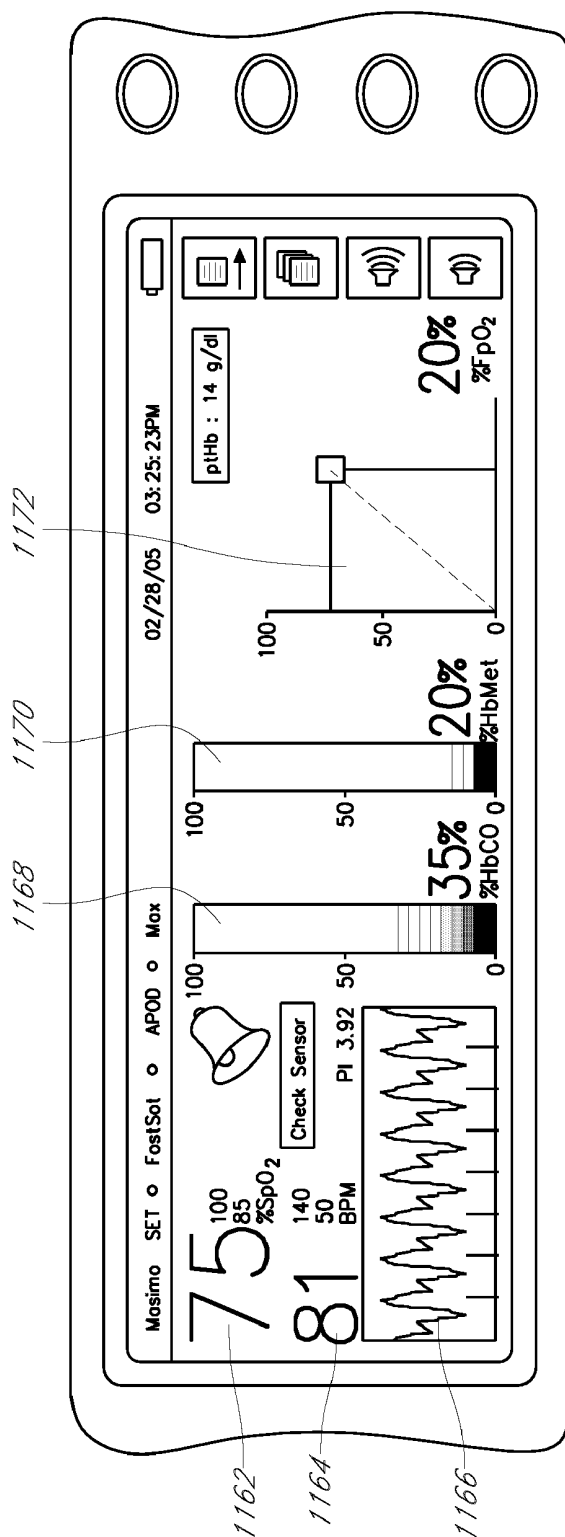


FIG. 11G

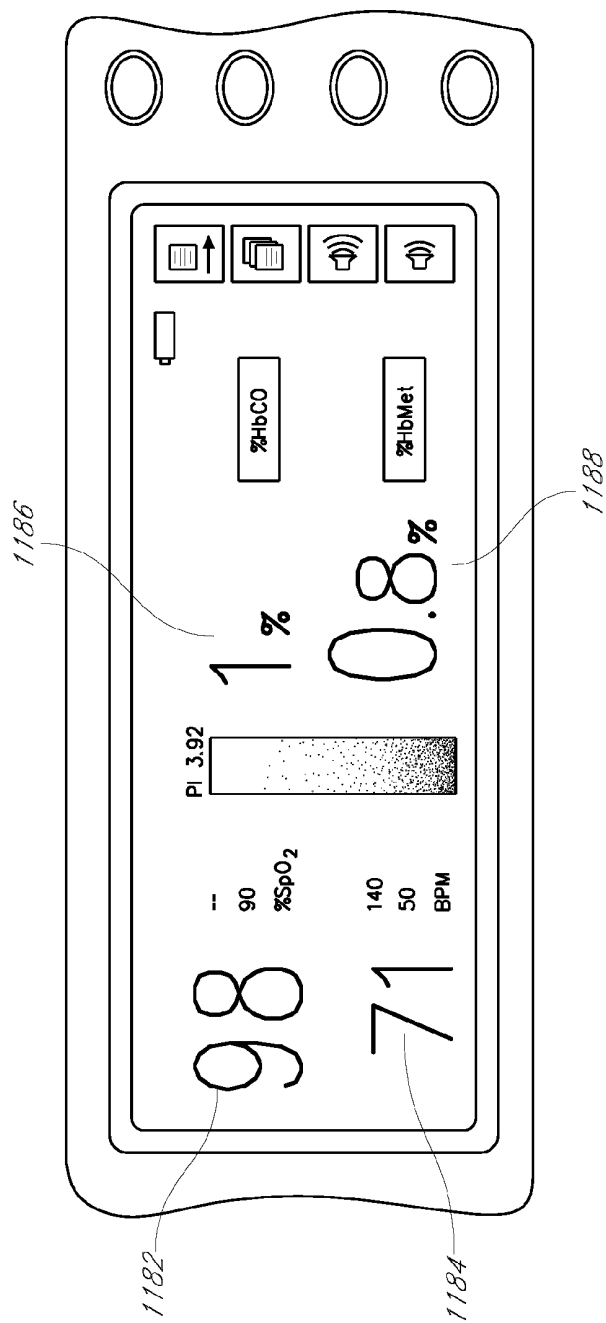


FIG. 11H

NONINVASIVE MULTI-PARAMETER PATIENT MONITOR

REFERENCE TO RELATED APPLICATIONS

[0001] This application claims priority under 35 U.S.C. § 119(e) to U.S. Provisional Patent Application Ser. No. 60/894,147, filed Mar. 9, 2007, entitled “Noninvasive Multi-Parameter Patient Monitor,” which is incorporated herein by reference in its entirety.

[0002] The present application is related to the following copending U.S. utility applications:

App. Ser. No.	Filing Date	Title	Atty. Dock.
1 11/367,013	Mar. 1, 2006	Multiple Wavelength Sensor Emitters	MLR.002A
2 11/366,995	Mar. 1, 2006	Multiple Wavelength Sensor Equalization	MLR.003A
3 11/366,209	Mar. 1, 2006	Multiple Wavelength Sensor Substrate	MLR.004A
4 11/366,210	Mar. 1, 2006	Multiple Wavelength Sensor Interconnect	MLR.005A
5 11/366,833	Mar. 1, 2006	Multiple Wavelength Sensor Attachment	MLR.006A
6 11/366,997	Mar. 1, 2006	Multiple Wavelength Sensor Drivers	MLR.009A
7 11/367,034	Mar. 1, 2006	Physiological Parameter Confidence Measure	MLR.010A
8 11/367,036	Mar. 1, 2006	Configurable Physiological Measurement System	MLR.011A
9 11/367,033	Mar. 1, 2006	Noninvasive Multi-Parameter Patient Monitor	MLR.012A
10 11/367,014	Mar. 1, 2006	Noninvasive Multi-Parameter Patient Monitor	MLR.013A
11 11/366,208	Mar. 1, 2006	Noninvasive Multi-Parameter Patient Monitor	MLR.014A

[0003] The present application incorporates the foregoing disclosures herein by reference.

FIELD OF THE DISCLOSURE

[0004] The present disclosure relates to the field of noninvasive patient monitors. More specifically, the disclosure relates to monitors displaying measurements derived using signals from optical sensors.

BACKGROUND

[0005] Spectroscopy is a common technique for measuring the concentration of organic and some inorganic constituents of a solution. The theoretical basis of this technique is the Beer-Lambert law, which states that the concentration c_i of an absorbent in solution can be determined by the intensity of light transmitted through the solution, knowing the path-length d_λ , the intensity of the incident light $I_{0,\lambda}$, and the extinction coefficient $\epsilon_{i,\lambda}$ at a particular wavelength λ . In generalized form, the Beer-Lambert law is expressed as:

$$I_\lambda = I_{0,\lambda} e^{-d_\lambda \mu_{0,\lambda}} \quad (\text{Eqn. 1})$$

$$\mu_{0,\lambda} = \sum_{i=1}^n \epsilon_{i,\lambda} \cdot c_i \quad (\text{Eqn. 2})$$

[0006] where $\mu_{0,\lambda}$ is the bulk absorption coefficient and represents the probability of absorption per unit length. The minimum number of discrete wavelengths that are required to solve Equations 1-2 are the number of significant absorbers that are present in the solution.

[0007] A practical application of this technique is pulse oximetry, which utilizes a noninvasive sensor to measure oxygen saturation (SpO_2) and pulse rate. In general, the sensor has light emitting diodes (LEDs) that transmit optical radiation of red and infrared wavelengths into a tissue site and a detector that responds to the intensity of the optical radiation after absorption (e.g., by transmission or transreflectance) by pulsatile arterial blood flowing within the tissue site. Based on this response, a processor determines measurements for SpO_2 , pulse rate, and can output representative plethysmographic waveforms. Thus, “pulse oximetry” as used herein encompasses its broad ordinary meaning known to one of skill in the art, which includes at least those noninvasive procedures for measuring parameters of circulating blood through spectroscopy. Moreover, “plethysmograph” as used herein (commonly referred to as “photoplethysmograph”), encompasses its broad ordinary meaning known to one of skill in the art, which includes at least data representative of a change in the absorption of particular wavelengths of light as a function of the changes in body tissue resulting from pulsing blood.

[0008] Pulse oximeters capable of reading through motion induced noise are available from Masimo Corporation (“Masimo”) of Irvine, Calif. Moreover, portable and other oximeters capable of reading through motion induced noise are disclosed in at least U.S. Pat. Nos. 6,770,028, 6,658,276, 6,157,850, 6,002,952, and 5,769,785, which are owned by Masimo, and which are incorporated by reference herein. Such reading through motion oximeters have gained rapid acceptance in a wide variety of medical applications, including surgical wards, intensive care and neonatal units, general wards, home care, physical training, and virtually all types of monitoring scenarios.

SUMMARY OF THE DISCLOSURE

[0009] Despite the success of read through motion oximeter systems, there is a need to provide patient monitors capable of displaying multiple physiological parameters, other than or in addition to SpO_2 , plethysmograph waveforms, or pulse rates. For example, in accessing a patient's condition, caregivers often desire knowledge of other blood constituents, including for example, a percent value for arterial carbon monoxide saturation (“HbCO”) or a percent value for methemoglobin saturation (“HbMet”) or the like. For example, in an embodiment, the display advantageously displays one or more of the following: pulse rate, plethysmograph waveform data, perfusion index, values of blood constituents in body tissue, including for example, HbCO, HbMet, total hemoglobin (“Hbt”), arterial oxygen saturation (“ SpO_2 ”), fractional arterial oxygen saturation (“ SpaO_2 ”), or the like. In other embodiments, the monitor may advantageously and accurately determine values for one or more of HbO₂, Hb, blood glucose, water, the presence or absence of therapeutic drugs (aspirin, Dapson, nitrates, or the like) or abusive/recreational drugs (methamphetamine, alcohol, steroids, or the like), concentrations of carbon dioxide (“CO₂”) or oxygen (“O”), pH levels, bilirubin, perfusion quality, signal quality or the like. Accordingly, the present disclosure includes a multi-parameter patient monitor capable of deter-

mining one or more of the foregoing parameters, other than or in addition to, SpO₂, plethysmograph waveforms, or perfusion quality index.

[0010] In an embodiment, the display of a noninvasive multi-parameter patient monitor advantageously includes a plurality of display modes enabling more parameter data to be displayed than the available physical display area or real estate. In an embodiment, a user may cycle different parameter values through an area of the display common to both parameters even when one parameter is shifted, through, for example, actuation of a user input key. The patient monitor may also display different parameters as color-coded. For example, when the following measured parameters are within "normal" ranges, SpO₂ may be displayed red, pulse rate (BPM) may be displayed green, HbCO may be displayed orange, HbMet may be displayed blue, or the like. In an embodiment, measured values of SpO₂ may be displayed in white, BPM may be displayed in yellow green or aquamarine, P_{IT} may be displayed in violet, Hbt may be displayed in grass green, HbMet may be displayed in blue or light blue, HbCO may be displayed in orange, and SpaO₂ may be displayed in electric blue.

[0011] Moreover, parameter trend data may also be displayed using the same or similar color coding, especially when multiple trends are displayed on one or more display graphs. In addition, more coarse or gross parameter indications may be displayed for quick reference to indicate to a caregiver whether any of a variety of monitored parameters, such as, for example, SpO₂, HbCO or HbMet is within acceptable ranges. The monitor may advantageously include additional display information, such as, for example, parametric displays where one parameter is displayed as a function of another, three dimensional displays (for example, extending a parametric display along time or an additional parameter), directional indicators predicting where a parameter is likely heading or reporting a general direction a parameters has been trending, or the like.

[0012] In addition to the foregoing, caregivers often desire to more closely monitor parameters that are close to, approaching, or beyond normal safe thresholds. In an embodiment, the patient monitor provides an indication that the caregiver should change display modes to view more critical monitored parameters. In alternative embodiments, the patient monitor automatically changes display modes to show parameters moving closer to or beyond normal thresholds.

[0013] In an embodiment, the patient monitor includes an audible or visual indication of a type of sensor communicating with the monitor. For example, the monitor may determine how many wavelengths a particular attached sensor will emit through communication with memory devices associated with the attached sensor or cable.

[0014] In an embodiment, a patient monitor capable of measuring at least two physiological parameters comprises a display device capable of exhibiting a first measured value of a first physiological parameter of body tissue of a monitored patient in a first display area or a second measured value of a second physiological parameter of the body tissue in the first display area, a mode selector actuable by a user to choose which of the first and second measured values is exhibited in the first display area, and a mode indicator generally associated with the mode selector and adapted to inform the user as to which of the measured values would be exhibited in the first display area upon actuation of the mode selector.

[0015] In an embodiment, a method of exhibiting at least two measurements of physiological parameters of body tissue of a monitored patient on a display device of a patient monitor, in which the display device comprising a first display area being generally capable of displaying a single physiological parameter measurement, comprises exhibiting a first measurement of a first physiological parameter of the body tissue in the first display area, informing a user with a mode indicator as to which of the at least two measurements would be exhibited in the first display area upon actuation of a mode selector, selecting a second measurement of a second physiological parameter of the body tissue to be exhibited in the first display area, associating the second measurement with the mode indicator, and actuating the mode selector at least once to stop exhibiting the first measurement in the first display area and to start exhibiting the second measurement in the first display area.

[0016] Additional embodiments include audio or visual alarms for each of multiple monitored parameters, combinations of parameters, an indication of perfusion in the tissue of the measurement site, an indication of the confidence the signal processing has in its output measurements, or the like.

[0017] For purposes of summarization, certain aspects, advantages and novel features are described herein. Of course, it is to be understood that not necessarily all such aspects, advantages or features need to be present in any particular embodiment.

BRIEF DESCRIPTION OF THE DRAWINGS

[0018] The drawings and the associated descriptions are provided to illustrate embodiments of the disclosure and not to limit the scope of the claims.

[0019] FIG. 1 illustrates a block diagram of an exemplary embodiment of a patient monitoring system including a sensor and a multi-parameter patient monitor.

[0020] FIG. 2 illustrates a top elevation view of an exemplary handheld noninvasive multi-parameter patient monitor capable of displaying at least HbCO, such as, for example, from the patient monitor of FIG. 1.

[0021] FIG. 3 illustrates an exemplary display of the patient monitor of FIG. 2A.

[0022] FIG. 4 illustrates the display of FIG. 3 showing measured values of SpO₂, BPM, perfusion, and type of sensor according to an exemplary embodiment of the patient monitor of FIG. 1.

[0023] FIG. 5 illustrates the display of FIG. 3 showing measured values of HbCO, perfusion, and type of sensor according to an exemplary embodiment of the patient monitor of FIG. 1.

[0024] FIG. 6 illustrates the display of FIG. 3 showing measured values of SpO₂, HbCO, BPM, perfusion, and type of sensor, according to an exemplary embodiment of the patient monitor of FIG. 1.

[0025] FIG. 7A illustrates a top elevation view of an exemplary handheld noninvasive multi-parameter patient monitor capable of displaying at least HbCO and HbMet, such as, for example, the patient monitor of FIG. 1.

[0026] FIG. 7B illustrates a perspective view of an example embodiment of a handheld noninvasive multi-parameter patient monitor capable of displaying a plurality of parameters, such as, for example, from the patient monitor of FIG. 1.

[0027] FIG. 7C illustrates a perspective view of another example embodiment of a handheld noninvasive multi-pa-

parameter patient monitor capable of displaying a plurality of parameters, such as, for example, from the patient monitor of FIG. 1.

[0028] FIG. 8 illustrates an exemplary display of the patient monitor of FIG. 7A.

[0029] FIG. 9 illustrates the display of FIG. 8 showing measured values of SpO₂, BPM, HbCO, HbMet, and type of sensor according to an exemplary embodiment of the patient monitor of FIG. 1.

[0030] FIG. 10 illustrates the display of FIG. 8 showing measured values of HbCO, HbMet, and type of sensor according to an exemplary embodiment of the patient monitor of FIG. 1.

[0031] FIG. 11A illustrates a perspective view of an exemplary noninvasive multi-parameter patient monitor such as, for example, the patient monitor of FIG. 1.

[0032] FIGS. 11B-11H illustrate display screens of the patient monitor of FIG. 11A.

DETAILED DESCRIPTION OF PREFERRED AND ALTERNATIVE EMBODIMENTS

[0033] Embodiments of the present disclosure include a portable or other multi-parameter patient monitor capable of determining multiple physiological parameters from one or more signals output from one or more light sensitive detectors capable of detecting light attenuated by body tissue carrying pulsing blood. For example, in an embodiment, the monitor advantageously and accurately determines a wide variety of physiological parameters or other calculations as discussed above.

[0034] In an embodiment, the display of patient monitor advantageously includes a plurality of display modes enabling more parameter data to be displayed than the available physical display real estate. For example, the patient monitor may include one or more user input keys, buttons, or switches capable of toggling through measurement data. In an embodiment, the displays include mode indicators providing caregivers easily identifiable visual queues, such as LED's, text, icons, or other indicia providing readily identifiable queues as to which parameter is being displayed. In an embodiment, the display may shift, may be parameter color-coded, or the like to further ensure quick comprehension of which measured parameter is the displayed parameter. For example, in an embodiment, the monitor displays SpO₂ in white, pulse rate (BPM) in green, HbCO in orange, and HbMet in blue when the respective measured parameter is within a "normal" range.

[0035] In an embodiment, the patient monitor provides an indication that the caregiver should change display modes to view more critical or time sensitive measured parameters, specific caregiver selected parameters, or the like. For example, the patient monitor may advantageously sound audio or visual alarms that alert the caregiver to particular one or more of worsening parameters, parameters changing in a predetermined pattern or rate, parameters stabilizing below user defined or safe thresholds, caregiver selected parameters, or the like. The monitor may also use alerts that provide audio or visual indications of the severity of the condition, severity of the change, or the like. In alternative embodiments, the patient monitor may automatically change display modes when a particular parameter crosses one or more thresholds. For example, a patient monitor may be displaying a first parameter, such as a plethysmograph, and upon determining measurements indicating that HbMet is trending toward an

alarm condition, the monitor may automatically switch from displaying the first parameter to the alarming parameter, or in this case, a trend of the alarming parameter.

[0036] In an embodiment, a switch is provided to allow a user to switch displays to view an alarming measurement. In an embodiment, during an alarm condition, a parameter display may switch to a trend graph in the same or different color, line weight, flash, flash rate, intensity, size, or the like.

[0037] The patient monitor may also include one or more displays capable of displaying trend data for any one or more of the monitored or derived patient parameters. For example, the trend data may be displayed in graph form, may include multiple trend lines, each representing a different monitored or derived patient parameter. Moreover, each trend line may be color-coded to facilitate quick comprehension of which trend line represents which measured parameter. However, an artisan will recognize from the disclosure herein a large number of identification techniques including color-coding, identifying text, or the like. Additionally, user input may toggle displayed trend data, may select which parameters to display simultaneously, or the like.

[0038] In an embodiment, the patient monitor includes an audible or visual indication of a type of sensor communicating with the monitor. For example, the patient monitor may provide a particular audio or visual indication, such as a beep, LED activation, graphic activation, text messages, voice messages, or the like, to indicate communication with or connection to an approved sensor, patient cable, combination, or the like. In an embodiment, the indication may change based on the manufacturer, type of sensor recognized or not recognized, type of patient, type of physiological parameters measurable with the attached sensor, or the like. Additional embodiments include an indication of perfusion in the tissue of the measurement site and an indication of the confidence the signal processing has in its output measurements or input signal quality.

[0039] To facilitate an understanding of the disclosure, the remainder of the description references exemplary embodiments illustrated in the drawings. Moreover, in this application, reference is made to many blood parameters. Some references that have common shorthand designations are referenced through such shorthand designations. For example, as used herein, HbCO designates carboxyhemoglobin, HbMet designates methemoglobin, and Hbt designates total hemoglobin. Other shorthand designations such as COHb, MetHb, and tHb are also common in the art for these same constituents. These constituents are generally reported herein in terms of a percentage, often referred to as saturation, relative concentration or fractional saturation. Total hemoglobin is generally reported as a concentration in g/dL. The use of the particular shorthand designators presented in this application does not restrict the term to any particular manner in which the designated constituent is reported.

[0040] FIG. 1 illustrates a block diagram of an exemplary embodiment of a patient monitoring system 100. As shown in FIG. 1, the system 100 includes a patient monitor 102 comprising a processing board 104 and a host instrument 108. The processing board 104 communicates with a sensor 106 to receive one or more intensity signal(s) indicative of one or more parameters of tissue of a patient. The processing board 104 also communicates with a host instrument 108 to display determined values calculated using the one or more intensity signals. According to an embodiment, the board 104 comprises processing circuitry arranged on one or more printed

circuit boards capable of installation into the monitor **102**, or capable of being distributed as some or all of one or more OEM components for a wide variety of host instruments monitoring a wide variety of patient information. In an embodiment, the processing board **102** comprises a sensor interface **110**, a digital signal processor and signal extractor (“DSP” or “processor”) **112**, and an instrument manager **114**. In general, the sensor interface **110** converts digital control signals into analog drive signals capable of driving sensor emitters, and converts composite analog intensity signal(s) from light sensitive detectors into digital data.

[0041] In an embodiment, the sensor interface **110** manages communication with external computing devices. For example, in an embodiment, a multipurpose sensor port (or input/output port) is capable of connecting to the sensor **106** or alternatively connecting to a computing device, such as a personal computer, a PDA, additional monitoring equipment or networks, or the like. When connected to the computing device, the processing board **104** may upload various stored data for, for example, off-line analysis and diagnosis. The stored data may comprise trend data for any one or more of the measured parameter data, plethysmograph waveform data acoustic sound waveform, or the like. Moreover, the processing board **104** may advantageously download from the computing device various upgrades or executable programs, may perform diagnosis on the hardware or software of the monitor **102**. In addition, the processing board **104** may advantageously be used to view and examine patient data, including raw data, at or away from a monitoring site, through data uploads/downloads, or network connections, combinations, or the like, such as for customer support purposes including software maintenance, customer technical support, and the like. Upgradable sensor ports are disclosed in copending U.S. application Ser. No. 10/898,680, filed on Jul. 23, 2004, titled “Multipurpose Sensor Port,” incorporated by reference herein.

[0042] As shown in FIG. 1, the digital data is output to the DSP **112**. According to an embodiment, the DSP **112** comprises a processing device based on the Super Harvard ARCHitecture (“SHARC”), such as those commercially available from Analog Devices. However, a skilled artisan will recognize from the disclosure herein that the DSP **112** can comprise a wide variety of data and/or signal processors capable of executing programs for determining physiological parameters from input data. In particular, the DSP **112** includes program instructions capable of receiving multiple channels of data related to one or more intensity signals representative of the absorption (from transmissive or reflective sensor systems) of a plurality of wavelengths of emitted light by body tissue. In an embodiment, the DSP **112** accepts data related to the absorption of eight (8) wavelengths of light, although an artisan will recognize from the disclosure herein that the data can be related to the absorption of two (2) to sixteen (16) or more wavelengths.

[0043] FIG. 1 also shows the processing board **104** including the instrument manager **114**. According to an embodiment, the instrument manager **114** may comprise one or more microcontrollers controlling system management, including, for example, communications of calculated parameter data and the like to the host instrument **108**. The instrument manager **114** may also act as a watchdog circuit by, for example, monitoring the activity of the DSP **112** and resetting it when appropriate.

[0044] The sensor **106** may comprise a reusable clip-type sensor, a disposable adhesive-type sensor, a combination sensor having reusable and disposable components, or the like. Moreover, an artisan will recognize from the disclosure herein that the sensor **106** can also comprise mechanical structures, adhesive or other tape structures, Velcro wraps or combination structures specialized for the type of patient, type of monitoring, type of monitor, or the like. In an embodiment, the sensor **106** provides data to the board **104** and vice versa through, for example, a patient cable. An artisan will also recognize from the disclosure herein that such communication can be wireless, over public or private networks or computing systems or devices, or the like.

[0045] As shown in FIG. 1, the sensor **106** includes a plurality of emitters **116** irradiating the body tissue **118** with differing wavelengths of light, and one or more detectors **120** capable of detecting the light after attenuation by the tissue **118**. In an embodiment, the emitters **116** comprise a matrix of eight (8) emission devices mounted on a flexible substrate, the emission devices being capable of emitting eight (8) differing wavelengths of light. In other embodiments, the emitters **116** may comprise twelve (12) or sixteen (16) emitters, although other numbers of emitters are contemplated, including two (2) or more emitters. As shown in FIG. 1, the sensor **106** may include other electrical components such as, for example, a memory device **122** comprising an EPROM, EEPROM, ROM, RAM, microcontroller, combinations of the same, or the like. In an embodiment, other sensor components may include a temperature determination device **123** or other mechanisms for, for example, determining real-time emission wavelengths of the emitters **116**.

[0046] The memory **122** may advantageously store some or all of a wide variety of data and information, including, for example, information on the type or operation of the sensor **106**; type or identification of sensor buyer or distributor or groups of buyer or distributors, sensor manufacturer information, sensor characteristics including the number of emitting devices, the number of emission wavelengths, data relating to emission centroids, data relating to a change in emission characteristics based on varying temperature, history of the sensor temperature, current, or voltage, emitter specifications, emitter drive requirements, demodulation data, calculation mode data, the parameters for which the sensor is capable of supplying sufficient measurement data (e.g., H_pCO, H_pMet, H_bT, or the like), calibration or parameter coefficient data, software such as scripts, executable code, or the like, sensor electronic elements, whether the sensor is a disposable, reusable, multi-site, partially reusable, partially disposable sensor, whether it is an adhesive or non-adhesive sensor, whether the sensor is a reflectance, transmittance, or transreflectance sensor, whether the sensor is a finger, hand, foot, forehead, or ear sensor, whether the sensor is a stereo sensor or a two-headed sensor, sensor life data indicating whether some or all sensor components have expired and should be replaced, encryption information, keys, indexes to keys or hash functions, or the like, monitor or algorithm upgrade instructions or data, some or all of parameter equations, information about the patient, age, sex, medications, and other information that may be useful for the accuracy or alarm settings and sensitivities, trend history, alarm history, or the like. In an embodiment, the monitor may advantageously store data on the memory device, including, for example, measured trending data for any number of param-

eters for any number of patients, or the like, sensor use or expiration calculations, sensor history, or the like.

[0047] FIG. 1 also shows the patient monitor **102** including the host instrument **108**. In an embodiment, the host instrument **108** communicates with the board **104** to receive signals indicative of the physiological parameter information calculated by the DSP **112**. The host instrument **108** preferably includes one or more display devices **124** capable of displaying indicia representative of the calculated physiological parameters of the tissue **118** at the measurement site. In an embodiment, the host instrument **108** may advantageously comprise a handheld housing capable of displaying one or more of a pulse rate ("PR"), plethysmograph data, perfusion quality such as a perfusion quality index ("PITM"), signal or measurement quality ("SQ"), values of blood constituents in body tissue, including for example, SpO₂, HbCO, HbMet, Hbt, or the like. In other embodiments, the host instrument **108** is capable of displaying values for one or more of Hbt, Hb, blood glucose, bilirubin, or the like. The host instrument **108** may be capable of storing or displaying historical or trending data related to one or more of the measured values, combinations of the measured values, plethysmograph data, or the like. The host instrument **108** also includes an audio indicator **126** and user input device **128**, such as, for example, a keypad, touch screen, pointing device, voice recognition device, or the like.

[0048] In still additional embodiments, the host instrument **108** includes audio or visual alarms that alert caregivers that one or more physiological parameters are falling below predetermined safe thresholds. The host instrument **108** may include indications of the confidence a caregiver should have in the displayed data. In a further embodiment, the host instrument **108** may advantageously include circuitry capable of determining the expiration or overuse of components of the sensor **106**, including, for example, reusable elements, disposable elements, or combinations of the same.

[0049] Although described in terms of certain embodiments, other embodiments or combination of embodiments will be apparent to those of ordinary skill in the art from the disclosure herein. For example, the monitor **102** may comprise one or more monitoring systems monitoring parameters, such as, for example, vital signs, blood pressure, ECG or EKG, respiration, glucose, bilirubin, or the like. Such systems may combine other information with intensity-derived information to influence diagnosis or device operation. Moreover, the monitor **102** may advantageously include an audio system, preferably comprising a high quality audio processor and high quality speakers to provide for voiced alarms, messaging, or the like. In an embodiment, the monitor **102** may advantageously include an audio out jack, conventional audio jacks, headphone jacks, or the like, such that any of the display information disclosed herein may be audiblized for a listener. For example, the monitor **102** may include an audible transducer input (such as a microphone, piezoelectric sensor, or the like) for collecting one or more of heart sounds, lung sounds, trachea sounds, or other body sounds and such sounds may be reproduced through the audio system and output from the monitor **102**. Also, wired or wireless communications (such as Bluetooth or WiFi, including IEEE 801.1a, b, or g), mobile communications, combinations of the same, or the like, may be used to transmit the audio output to other audio transducers separate from the monitor **102**.

[0050] For example, patterns or changes in the continuous noninvasive monitoring of intensity-derived information may

cause the activation of other vital sign measurement devices, such as, for example, blood pressure cuffs.

[0051] FIG. 2 illustrates a perspective view of an exemplary handheld noninvasive multi-parameter patient monitor **200**, such as, for example, the patient monitor **102** of FIG. 1. Patient monitors **200** exhibiting combinations of many of the features described herein are advantageously commercially available from Masimo under the brand name "Rad 57c." As shown in FIG. 2, the monitor **200** includes a patient cable connector **202** capable of mechanical mating with a patient cable to establish communication between the board **104** and the sensor **106**. In an embodiment, the connector **202** comprises a multipurpose cable connector such as that disclosed in the incorporated U.S. application Ser. No. 10/898,680, titled "Multipurpose Sensor Port," disclosing communication between the board **104** and an external computing device.

[0052] The monitor **200** also comprises a HbCO indicator **204**, advantageously providing a visual queue that a HbCO capable sensor is properly connected through the connector **202**. For example, the HbCO indicator **204** may advantageously activate when a sensor is connected that communicates sufficient information to determine HbCO, such as, for example, a sensor capable of emitting sufficient different wavelengths of light, a sensor storing sufficient data on the memory **122**, a sensor having appropriate encryption data or key, combinations of the same, or the like. For example, in an embodiment, the processor **112** may receive information from a memory **122** indicating a number of available LED wavelengths for the attached sensor. Based on the number of wavelengths, or other information stored on the memory **122**, the processor **112** may determine whether an HbCO-ready sensor has been attached to the monitor **200**. An artisan will also recognize from the disclosure herein that the HbCO indicator **204** may advantageously comprise a HbMet indicator, Hbt indicator, or the like, which activates to a predetermined color associated with a parameter, or any color, or deactivates the same, to convey a type of attached sensor. Moreover, the artisan will recognize from the disclosure herein other parameters that may use other sensor components and the monitor **200** may include indicators capable of indicating communication with those types of sensors.

[0053] In an embodiment, the monitor **200** may also audibly indicate the type of sensor connected. For example, the monitor **200** may emit predetermined number or frequency of beeps associated with recognition of a particular sensor, a particular manufacturer, failure to recognize the sensor, or the like. Moreover, the sensor type may be indicative of the componentry, such as, for example, whether the sensor produces sufficient data for the determination of HbCO, HbMet, Hbt and SpO₂, SpO₂ only, SpO₂ and HbMet, any combination of the foregoing or other parameters, or the like. Additionally, the sensor type may be indicative of specific sensors designed for a type of patient, type of patient tissue, or the like. In other embodiments, the monitor **200** may announce the type of connector through speaker **236**.

[0054] An artisan will also recognize from the disclosure herein that other mechanical (such as keys), electrical, or combination devices may inform the monitor **200** of the type of attached sensor. In an embodiment, the processor **112** also may select to drive less emitters that are currently available, such as, for example, in the presence of low noise and when power consumption is an issue.

[0055] The monitor **200** also comprises a multi-mode display **206** capable of displaying, for example, measurements

of SpO₂ and HbCO (or alternatively, HbMet). In an embodiment, the display 206 has insufficient space or display real estate to display the many parameters capable of being measured by the monitor 200. Thus, the multi-mode display 206 may advantageously cycle through two or more measured parameters in an area common to both parameters even when shifted. In such embodiments, the monitor 200 may also advantageously include parameter indicators 208, 210, providing additional visual queues as to which parameter is currently displayed. In an embodiment, the display may also cycle colors, flash rates, or other audio or visual queues providing readily identifiable information as to which measured parameter is displayed. For example, when the multi-mode display 206 displays measured values of SpO₂ that are normal, the numbers may advantageously appear in green, while normal measured values of HbCO may advantageously appear in orange, and normal measured values of HbMet may appear in blue. Moreover, in an embodiment, the display 206 flashes at a predefined rate when searching for saturation and at another predefined rate when a signal quality is below a predetermined threshold.

[0056] The monitor 200 also comprises a HbCO bar 212 where in an embodiment a plurality of LED's activate from a bottom toward a top such that the bar "fills" to a level proportional to the measured value. For example, the bar 212 is lowest when the dangers from carbon monoxide poisoning are the least, and highest when the dangers are the greatest. The bar 212 includes indicia 214 that provide an indication of the severity of carbon monoxide saturation in a patient's blood. As shown in FIG. 2, the bar 212 and the indicia 214 continuously indicate the concentration of HbCO in about 5% increments. The indicia 214 indicate a measurement of HbCO saturation percentage between about 0 and about 50% with a granularity of about 5%. However, an artisan will also recognize from the disclosure herein a wide variety of ranges and granularities could be used, the indicia 214 could be electronically displayed in order to straightforwardly increase or decrease resolution, or the like. For example, HbCO may advantageously be displayed with greater resolution than \pm about 5% in a lower portion of the scale. For example, an HbCO bar may advantageously include a scale of about <3%, about 6%, about 9%, about 12%, about 15%, about 20%, about 25%, about 30%, about 35%, and about >40%.

[0057] As is known in the art, carbon monoxide in the blood can lead to serious medical issues. For example and depending upon the particular physiology of a patient, about 10% carbon monoxide saturation can lead to headaches, about 20% can lead to throbbing headaches, or dyspnea on exertion, about 30% can lead to impaired judgment, nausea, dizziness and/or vomiting, visual disturbance, or fatigue, about 40% can lead to confusion and syncope, and about 50% and above can lead to comas, seizures, respiratory failure, and even death.

[0058] In an embodiment, the bar 212 is the same or similar color as the multi-mode display 206 when displaying HbCO. In other embodiments, the bar 212 is lowest and green when the dangers from carbon monoxide poisoning are the least, and highest and red when the dangers are the greatest. In an embodiment, as HbCO increases, the entire bar 212 may advantageously change color, such as, for example, from green to red, to provide a clear indication of deepening severity of the condition. In other embodiments, the bar 212 may advantageously blink or flash, an audio alarm may beep or provide a continuation or rise in pitch or volume, or the like to

alert a caregiver of deepening severity. Moreover, straightforward to complex alarm rules may be implemented to reduce false alarms based on, for example, knowledge of the physiological limitations on the rate of change in HbCO or the like.

[0059] Additionally, the monitor 200 may be capable of storing and outputting historical parameter data, display trend traces or data, or the like. Although the foregoing bar 212 has been described in terms of certain preferred embodiments, other embodiments will be apparent to those of ordinary skill in the art from the disclosure herein.

[0060] FIG. 2 also shows the monitor 200 including a pulse display 216 displaying measured pulse rate in beats per minute ("BPM"). In an embodiment, the display 212 flashes when searching for a pulse. The pulse display 216 advantageously displays measured pulse rates from about zero (0) to about two hundred and forty (240) BPM. Moreover, when the measured pulse rates are considered normal, the pulse display 216 is advantageously green. Similar to other displays associated with the monitor 200, the pulse display 216 may employ a variety of color changes, audio alarms, or combinations of the same to indicate measured BPM below predetermined safe thresholds. In an embodiment, the pulse rate display 216 displays the measured pulse rate during the display of SpO₂ and displays message data during the display of other parameters. For example, during the display of HbCO, the display 216 may advantageously display the term "CO." In an embodiment, the display of the message data may be in the same or similar color as the other displays. For example, in an embodiment, the multi-mode display 206, the bar 212, and the pulse display 216 may all display data or messages in orange when the multi-mode display 206 displays measured HbCO values.

[0061] FIG. 2 also illustrates the monitor 200 comprising user input keys 218, including a HbCO button 220, mode/enter button 222, next button 224, power on/off button 226, up/down button 228, and alarm silence button 230. In an embodiment, activation of the HbCO button 220 toggles the measured value displayed in the multi-mode display 206. For example, activation of the HbCO button 220 toggles the multi-mode display 206 from displaying measured values of SpO₂ to HbCO for about ten (10) seconds. Activation of the mode/enter button 222 or the next button 224 during the ten (10) second period returns the multi-mode display 206 back to SpO₂. A skilled artisan will also recognize that activation of the HbCO button 220 may advantageously toggle through a plurality of measured values, and that such values may be displayed for short segments and then return to SpO₂, may remain displayed until further activation of the button 220, or the like.

[0062] Activation of the mode/enter button 222 cycles through various setup menus allowing a caregiver to select or activate certain entries within the menu setup system, including alarm threshold customizations, or the like. Activation of the next button 224 can move through setup options within the menu setup system and in an embodiment is not active during normal patient monitoring. For example, a caregiver may activate the mode/enter button 222 and the next button 224 to specify high and low alarm thresholds for one or more of the measured parameters, to specify device sensitivity, trend settings, display customizations, color code parameters, or the like. In an embodiment, the high alarm setting for SpO₂ can range from about two percent (2%) to about one hundred percent (100%) with a granularity of about one percent (1%). The low alarm setting for SpO₂ can range from about one

percent (1%) to about one hundred percent (100%) with a granularity of about one percent (1%). Moreover, the high alarm setting for pulse rate can range from about thirty (30) BPM to about two hundred and forty (240) BPM with a granularity of about five (5) BPM. The low alarm setting for pulse rate can range from about twenty five (25) BPM to about two hundred and thirty five (235) BPM with a granularity of about five (5) BPM. Other high and low ranges for other measured parameters will be apparent to one of ordinary skill in the art from the disclosure herein.

[0063] In a further embodiment, a caregiver may activate the mode/enter button **222** and the next button **224** to specify device sensitivity, such as, for example, device averaging times, probe off detection, whether to enable fast saturation calculations, or the like. Various embodiments of fast saturation calculations are disclosed in U.S. patent application Ser. No. 10/213,270, filed Aug. 5, 2002, titled "Variable Indication Estimator," now U.S. Pat. No. 6,999,904, issued Feb. 14, 2006, and incorporated by reference herein. Using the menus, a caregiver may also advantageously enter appropriate information governing trend collection on one or more of the measured parameters, input signals, or the like.

[0064] FIG. 2 also shows the power on/off button **226**. Activation of the power on/off button **226** activates and deactivates the monitor **200**. In an embodiment, press-and-hold activation for about two (2) seconds shuts the monitor **200** off. In an additional embodiment, activation of the on/off button **226** advantageously initiates detection of a type of attached sensor. For example, activation of the on/off button **226** may advantageously cause the monitor **200** to read information from a memory on an attached sensor and determine whether sufficient wavelengths exist on the sensor to determine one or more the physiological parameters discussed in the foregoing.

[0065] An artisan will recognize from the disclosure herein that the on/off button **226** may advantageously cause an electronic determination of whether to operate in at powers consisted with the U.S. (60 Hz) or another nationality (50 Hz). In an embodiment, such automatic determination and switching is removed from the monitor **200** in order to reduce a likelihood of problematic interfering crosstalk caused by such power switching devices.

[0066] Activation of the up/down button **228** may advantageously adjust the volume of the pulse beep tone. Additionally, activation of the up/down button **228** within the menu setup system, causes the selection of values with various menu options.

[0067] Moreover, activation of the alarm silence button **230** temporarily silences audio alarms for a predetermined period, such as, for example, about one hundred and twenty (120) seconds. A second activation of the alarm silence button **230** mutes (suspends) the alarm indefinitely, while a third activation returns the monitor **200** to standard alarm monitoring. FIG. 2 also shows the alarm silence button **230** includes an alarm silenced indicator **232**. The alarm silenced indicator **232** may advantageously flash to indicate one or more alarms are temporarily silenced, may illuminate solid to indicate the alarms have been muted, or the like. Moreover, an artisan will recognize from the disclosure herein a wide variety of alarm silencing methodologies.

[0068] The monitor **200** also includes a battery level indicator **234** indicating remaining battery life. In the illustrated embodiment, four LED's indicate the status of the battery by incrementally deactivating to indicate proportionally

decreasing battery life. In an embodiment, the four LED's may also change color as the battery charge decreases, and the final LED may begin to flash to indicate that the caregiver should replace the batteries.

[0069] FIG. 2 also shows the monitor **200** including an audio transducer or speaker **236**. The speaker **236** advantageously provides audible indications of alarm conditions, pulse tone and feedback for key-presses, or the like. Moreover, the monitor **200** includes a low signal quality indicator ("SQ" or "SIQTM") **238**. The signal IQ indicator **238** activates to inform a caregiver that a measured value of the quality of the incoming signal is below predetermined threshold values. For example, in an embodiment, the measured value for signal IQ is at least partially based on an evaluation of the plethysmograph data's correspondence to predetermined models or characteristics of physiological signals. In an embodiment, the signal IQ indicator **238** output may be associated with the displayed parameter. For example, the output may be associated with one threshold for the display of SpO₂ and another for the display of other parameter data.

[0070] The monitor **200** also comprises a perfusion quality index ("PITM") bar **240** (which quantifies the measure of perfusion of the patient) where in an embodiment a plurality of LED's activate from a bottom toward a top such that the bar "fills" to a level proportional to the measured value. In one embodiment, the PITM bar **240** shows a static value of perfusion for a given time period, such as, for example, one or more pulses. In another embodiment, or functional setting, the PITM bar **240** may advantageously pulse with a pulse rate, may hold the last reading and optionally fade until the next reading, may indicate historical readings through colors or fades, or the like. Additionally, the PITM bar **240** may advantageously change colors, flash, increasingly flash, or the like to indicate worsening measured values of perfusion.

[0071] The PITM bar **240** can be used to simply indicate inappropriate occlusion due, for example, to improper attachment of the sensor **106**. The PITM bar **240** can also be used as a diagnostic tool during low perfusion for the accurate prediction of illness severity, especially in neonates. Moreover, the rate of change in the PITM bar **240** can be indicative of blood loss, sleep arousal, severe hypertension, pain management, the presence or absence of drugs, or the like. According to one embodiment, the PITM bar **240** values may comprise a measurement of the signal strength of the arterial pulse as a percentage of the total signal received. For example, in one preferred embodiment, the alternating portion of at least one intensity signal from the sensor **106** may advantageously be divided by the static portion of the signal. For example, an infrared intensity signal may advantageously be used as it is less subjective to noise.

[0072] In an embodiment, a measurement below about 1.25% may indicate medical situations in need of caregiver attention, specifically in monitored neonates. Because of the relevance of about 1.25%, the PITM bar **240** may advantageously include level indicia **242** where the indicia **242** swap sides of the PITM bar **240**, thus highlighting any readings below about that threshold. Moreover, behavior of the PITM bar **240**, as discussed above, may advantageously draw attention to monitored values below such a threshold.

[0073] As discussed above, the monitor **200** may include output functionality that outputs, for example, trend perfusion data, such that a caregiver can monitor measured values of perfusion over time. Alternatively or additionally, the monitor **200** may display historical trace data on an appropri-

ate display indicating the measured values of perfusion over time. In an embodiment, the trend data is uploaded to an external computing device through, for example, the multi-purpose sensor connector 202 or other input output systems such as USB, serial or parallel ports or the like.

[0074] The monitor 200 also includes an alarm indicator 244 capable of providing visual queues of the status of one or more of the measured parameters. For example, the alarm indicator 244 may advantageously be green when all of the measured parameters are within normal conditions, may gradually fade to red, may flash, increasing flash, or the like, as one or more of the measured values approaches or passes predetermined thresholds. In an embodiment, the alarm indicator 244 activates when any parameter falls below an associated threshold, thereby advantageously informing a caregiver that perhaps a nondisplayed parameters is at an alarm condition. In another embodiment, the alarm indicator 244 may indicate the status of the parameter displayed on the multi-mode display 206. In an embodiment, the speaker 236 may sound in conjunction with and/or in addition to the indicator 244. Moreover, in an embodiment, an alarming parameter may automatically be displayed, may be emphasized, flashed, colored, combinations of the same or the like to draw a user's attention to the alarming parameter.

[0075] Although the foregoing invention has been described in terms of certain preferred embodiments, other embodiments will be apparent to those of ordinary skill in the art from the disclosure herein.

[0076] FIG. 3 illustrates an exemplary display of the patient monitor 200. As shown in FIG. 3, the display includes the multi-mode display 206, the pulse rate display 216, parameter indicators 208, 210, the HbCO bar 212 and indicator 204, the P_{IT} bar 240, and the alarm indicator 244. In an embodiment, the multi-mode display 206 and the pulse rate display 216 each comprise a plurality of seven segment displays 302 capable of displaying alpha-numeric information. As disclosed in the foregoing, the exemplary display may advantageously include color-coded parameter displays. Moreover, the exemplary display may include color progressions, flashing, flashing progressions, audible alarms, audible progressions, or the like, indicating worsening measured values of physiological data. In addition, in an embodiment, some or all of the displays may flash at a first rate to indicate attempts to acquire data when actual measured values are unavailable. Moreover, some or all of the display may flash at a second rate to indicate low signal quality where confidence is decreasing that the measured values reflect actual physiological conditions.

[0077] FIG. 4 illustrates the display of FIG. 3 showing measured values of SpO₂, BPM, perfusion, and type of sensor, according to an exemplary embodiment of the patient monitor of FIG. 1. As shown in FIG. 4, the multi-mode display 206 is displaying a percentage value of SpO₂, and the pulse rate display 216 is displaying a pulse rate in beats per minute. Accordingly, the parameter indicator 210 is activated to confirm the display of measured values of SpO₂. As disclosed in the foregoing, in an embodiment, the multi-mode display 206 is red, indicating blood oxygen measurements while the pulse rate display 216 is green, indicating normal values of a patient's pulse.

[0078] FIG. 4 also shows the P_{IT} bar 240 almost fully activated, representing good perfusion. In addition, the HbCO indicator 204 is showing communication with a sensor producing insufficient data to determine measured values of

additional parameters, such as, HbCO. In an embodiment, such sensors may comprise sensors capable of emitting light at about two (2) different wavelengths, may comprise sensors with insufficient data stored on a memory associated therewith, or the like.

[0079] FIG. 5 illustrates the display of FIG. 3 showing measured values of HbCO, perfusion, and type of sensor, according to an exemplary embodiment of the patient monitor of FIG. 1. As shown in FIG. 5, the multi-mode display 206 is displaying a percentage value of HbCO, and the pulse rate display 216 is displaying an appropriate message indicating the HbCO measurement, such as, for example, "CO". Also, the multi-mode display 206 has shifted the data to the left to quickly and efficiently indicate that the displayed parameter is other than SpO₂. Accordingly, the parameter indicator 208 is also activated to confirm the display of measured values of HbCO. As disclosed in the foregoing, in an embodiment, the multi-mode display 206 and pulse rate display message 216 are orange.

[0080] FIG. 5 also shows the P_{IT} bar 240 almost fully activated, representing good perfusion. In addition, the activation of the HbCO indicator 204 represents communication with a sensor capable of producing sufficient data to determine measured values of HbCO. In an embodiment, such sensors may comprise sensors capable of emitting light at about eight (8) or more different wavelengths; however, such sensors may comprise about two (2) or more different wavelengths. Moreover, such sensors may have appropriate data stored on a memory associated therewith, or the like. FIG. 5 also shows the HbCO measurement being about 20% (as illustrated on the HbCO bar 212 and multi-mode display 206) thereby indicating a potentially dangerous situation that if exacerbated, will become quite problematic. Therefore, the alarm indicator 244 is also activated, and in some embodiments, the speaker 236 as well.

[0081] FIG. 6 illustrates the display of FIG. 3 showing measured values of SpO₂, HbCO, BPM, perfusion, and type of sensor, according to an exemplary embodiment of the patient monitor of FIG. 1. In contrast to FIG. 4, FIG. 6 shows that the monitor 200 is communicating with a sensor capable of producing sufficient data to determine measured values of HbCO, even though the displayed values are that of SpO₂ and BPM. Thus, FIG. 6 shows the activation of the HbCO indicator 204, and the continuous monitoring of HbCO by the HbCO bar 212. FIG. 6 also shows a high value of HbCO, and therefore, the indication of an alarm condition by activation of the alarm indicator 244. In an embodiment, upon determination of an alarm condition on a nondisplayed parameter, the monitor 200 may advantageously provide an alarm indication through speaker and alarm indicator activation, automatic toggle to the nondisplayed parameter on the multi-mode display 206 for a defined or undefined time, or the like.

[0082] FIG. 7A illustrates a top elevation view of an exemplary handheld noninvasive multi-parameter patient monitor 700 capable of displaying at least HbCO and HbMet, such as, for example, the patient monitor of FIG. 1. Patient monitors exhibiting combinations of many of the features described herein are advantageously commercially available from Masimo under the brand name "Rad 57cm." As shown in FIG. 7A, the monitor 700 comprises a monitor similar to monitor 200 disclosed with reference to FIG. 2. Moreover, monitor 700 further includes a multi-mode display 706 capable of displaying, for example, measurements of HbMet and BPM. In an embodiment, the display 706 has insufficient space or

display real estate to display the many parameters capable of being measured by the monitor **700**. Thus, the multi-mode display **706** may advantageously cycle through two or more measured parameters. In such embodiments, the monitor **700** may also advantageously include parameter indicators **708**, **710**, providing additional visual queues as to which parameter is currently displayed. In an embodiment, the display **706** may also cycle colors, flash rates, or other audio or visual queues providing readily identifiable information as to which measured parameter is displayed. For example, when the multi-mode display **706** displays measured values of BPM that are normal, the numbers may advantageously appear in green, while normal measured values of HbMet may appear in blue. Moreover, in an embodiment, the display **706** may flash at a predefined rate when searching for saturation and at another predefined rate when a signal quality is below a predetermined threshold.

[0083] FIG. 7A also illustrates the monitor **700** comprising user input keys **718**, including an HbCO/HbMet button **720**. In an embodiment, activation of the HbCO/HbMet button **720** toggles the measured value displayed in the multi-mode display **706**. For example, activation of the HbCO/HbMet button **720** toggles the multi-mode display **206** from displaying measured values of SpO₂ and BPM, to HbCO and HbMet for about ten (10) seconds. Activation of the mode/enter button **222** or the next button **224** during the ten (10) second period returns the multi-mode display **706** back to SpO₂ and BPM. A skilled artisan will also recognize that activation of the HbCO/HbMet button **720** may advantageously toggle through a plurality of measured values, and that such values may be displayed for short segments and then return to SpO₂ and BPM, may remain displayed until further activation of the button **720**, or the like.

[0084] FIG. 7B illustrates a perspective view of an exemplary handheld noninvasive multi-parameter patient monitor **1202** capable of exhibiting a plurality of parameters, such as, for example, from the patient monitor of FIG. 1. As shown in FIG. 7B, the monitoring system **1200** comprises a monitor **1202** similar to the monitors **200**, **700** disclosed with reference to FIGS. 2 and 7A. Moreover, the monitor **1202** includes a multi-mode display **1206** capable of exhibiting, for example, measurements of % SpCO, % SpO₂, and PTM and a multi-mode display **1208** capable of exhibiting, for example, % SpMet, BPM, and PTM. In an embodiment, the displays **1206**, **1208** have insufficient space or display real estate to exhibit the many parameters capable of being measured by the monitoring system **1200**. Thus, the multi-mode displays **1206**, **1208** may advantageously each cycle through two or more measured parameters. In such embodiments, the monitor **1200** may also advantageously include parameter indicators **1208**, **1209**, **1210**, **1211**, providing additional visual queues as to which parameters are being exhibited in the displays **1206**, **1208**. In an embodiment, the displays **1206**, **1208** may also cycle colors, flash rates, or other audio or visual queues providing readily identifiable information as to which measured parameters are being exhibited in the displays **1206**, **1208**. For example, when the multi-mode display **1208** exhibits measured values of BPM that are normal, the numbers may advantageously appear in green, while normal measured values of % SpMet may appear in blue. Moreover, in an embodiment, the displays **1206**, **1208** may flash at a predefined rate when searching for saturation and at another predefined rate when a signal quality is below a predetermined threshold.

[0085] FIG. 7B also illustrates the monitor **1202** comprising user input keys **218**, including a mode selector **1220**. In an embodiment, the mode selector **1220** is actuatable by a user to toggle which of the one or more of the measured values is exhibited in one or more of the multi-mode displays **1206**, **1208**. For example, actuation of the mode selector **1220** may toggle the multi-mode display **1206** from exhibiting measured values of % SpCO to % SpO₂ and/or the multi-mode display **1208** from exhibiting % SpMet to PR. A skilled artisan will also recognize that actuation of the mode selector **1220** may advantageously toggle through a plurality of measured values, and that such values may be exhibited for short durations and then return to certain preferred values such as SpO₂, may remain displayed until further actuation of the mode selector **1220**, or the like.

[0086] The monitor **1202** of FIG. 7B further comprises a mode indicator **1222** that is generally associated with the mode selector **1220** and that is adapted to inform a user as to which of the measured values of physiological parameters would be exhibited in one or more of the display areas **1206**, **1208** upon the occurrence of an event, for example if the mode selector **1220** is actuated or if a certain amount of time elapses. In the embodiment illustrated in FIG. 7B, for example, the mode indicator **1222** informs a user that, when the display **1206** exhibits % SpCO, actuation of the mode selector **1220** toggles the display **1206** such that it would exhibit % SpO₂. Such indication may be based on graphics, may include arrows, and the like. In some embodiments, the indication is based on a list that may be read from top to bottom (e.g., as indicated in FIG. 7B), left to right (e.g., as indicated in FIG. 7C), and the like. In the embodiment illustrated in FIG. 7B, the mode indicator **1222** further informs a user that, when the display **1206** exhibits % SpO₂, actuation of the mode selector **1220** toggles the display **1206** such that it would exhibit PTM, and that further even actuation of the mode selector **1220** toggles the display **1206** such that it would exhibit % SpCO again. Moreover, in the embodiment illustrated in FIG. 7B, the mode indicator **1222** informs a user that, when the display **1208** exhibits % SpMet, actuation of the mode selector **1220** toggles the display **1208** such that it would exhibit PR. The mode indicator **1222** further informs a user that, when the display **1208** exhibits PR, actuation of the mode selector **1220** toggles the display **1208** such that it would exhibit PTM, and that further even actuation of the mode selector **1220** toggles the display **1208** such that it would exhibit % SpMet again.

[0087] The monitor **1204** of FIG. 7C is similar to the monitor **1202** of FIG. 7B, although the monitor **1204** comprises a mode indicator **1224** that is generally associated with the mode selector **1220** and that is adapted to straightforwardly and directly inform a user as to which physiological parameter would be exhibited in the display areas **1206**, **1208** upon the occurrence of an event, for example if the mode selector **1220** is actuated or if a certain amount of time elapses. In the embodiment illustrated in FIG. 7C, for example, the mode indicator **1224** informs a user that, when the display **1206** exhibits % SpCO, actuation of the mode selector **1220** toggles the display **1206** such that it would exhibit % SpO₂. Such indication may be shown to a user by a plurality of LEDs associated with particular parameters that can be exhibited on the displays **1206**, **1208**. In certain embodiments, an LED indicates the parameters that would be displayed upon the occurrence of the event (e.g., actuation of the mode selector **1220**). In certain embodiments, an LED having a first color

(e.g., green) indicates the parameters being exhibited, an LED having a second color (e.g., yellow) indicates the parameters that would be displayed upon the occurrence of the event (e.g., actuation of the mode selector 1220), and an LED having a third color (e.g., orange) indicates the parameters that would be displayed upon the occurrence of a subsequent event (e.g., further actuation of the mode selector 1220). Other illuminated representations are also possible.

[0088] In the embodiment of FIG. 7C, the mode indicator 1222 further informs a user that, when the display 1206 exhibits % SpO₂, actuation of the mode selector 1220 toggles the display 1206 such that it would exhibit P_{IT}TM, and that further even actuation of the mode selector 1220 toggles the display 1206 such that it would exhibit % SpCO again. Moreover, in the embodiment illustrated in FIG. 7C, the mode indicator 1224 informs a user that, when the display 1208 exhibits % SpMet, actuation of the mode selector 1220 toggles the display 1208 such that it would exhibit PR. The mode indicator 1224 further informs a user that, when the display 1208 exhibits PR, actuation of the mode selector 1220 toggles the display 1208 such that it would exhibit P_{IT}TM, and that further even actuation of the mode selector 1220 toggles the display 1208 such that it would exhibit % SpMet again.

[0089] The mode indicators 1222, 1224 are preferably proximate (e.g., adjacent as illustrated in FIGS. 7B and 7C) to the mode selector 1220 with which they are generally associated. However, the mode indicators 1222, 1224 may be located in any suitable location on the monitors 1202, 1204, respectively.

[0090] Referring again to FIG. 7A, the monitor 700 also comprises a coarser indication of HbMet through an HbMet bar 740. In an embodiment, a plurality of LED's activate from a bottom toward a top such that the bar "fills" to a level proportional to the measured value, with increments at about 0.5%, about 1%, about 2%, about 3%, about 4%, about 5%, about 7.5%, about 10%, about 15% and greater than about 20%, although an artisan will recognize from the disclosure herein other useful delineations. Additionally, the HbMet bar 740 may advantageously change colors, flash, increasingly flash, or the like to indicate worsening measured values of perfusion.

[0091] Although disclosed with reference to the HbMet bar 740, and artisan will recognize from the disclosure herein other coarse or even gross indications of HbMet, or any measured parameter. For example, a single LED may advantageously show green, yellow, and red, to indicate worsening coarse values of HbMet. Alternatively, a single LED may simply light to indicate an alarm or approaching alarm condition.

[0092] FIG. 8 illustrates an exemplary display of the patient monitor 700 of FIG. 7A. As shown in FIG. 8, the display includes the multi-mode displays 206, 706, parameter indicators 208, 210, 708, 710, the HbCO bar 212 and indicator 204, the HbMet bar 740, and the alarm indicator 244. In an embodiment, the multi-mode display 706 is similar to multi-mode display 206, comprising a plurality of seven segment displays 302 capable of displaying alpha-numeric information, and capable of altering its display characteristics or aspects in a wide variety of configurations discussed with reference to the display 206.

[0093] FIG. 9 illustrates the display of FIG. 8 showing measured values of SpO₂, BPM, HbCO, HbMet, and type of sensor according to an exemplary embodiment of the patient monitor of FIG. 1. FIG. 9 also shows the HbMet bar 740 near

the bottom and corresponding to about 1%, representing acceptable HbMet, while the HbCO bar 212 hovers at a dangerous near 20%. In addition, the HbCO indicator 204 is showing communication with a sensor producing sufficient data to determine measured values of additional parameters, such as, HbMet, HbCO or the like. In an embodiment, such sensors may comprise sensors capable of emitting light of more than two (2) different wavelengths, preferably more than four (4) different wavelengths, and more preferably eight (8) or more different wavelengths.

[0094] FIG. 10 illustrates the display of FIG. 8 showing measured values of HbCO, HbMet, and type of sensor according to an exemplary embodiment of the patient monitor of FIG. 1. As shown in FIG. 10, the multi-mode display 706 is displaying a percentage value of HbMet that is shifted using the parameter indicator 708. The data has been advantageously shifted to the left to quickly and efficiently indicate that the displayed parameter is other than BPM. Accordingly, the parameter indicator 708 is also activated to confirm the display of measured values of HbMet. As disclosed in the foregoing, in an embodiment, the multi-mode display 706 is blue.

[0095] FIG. 10 also shows the HbMet bar 740 nearly empty, representing acceptable HbMet. In addition, the activation of the HbCO indicator 204 represents communication with a sensor capable of producing sufficient data to determine measured values of HbCO. In an embodiment, such sensors may have appropriate data stored on a memory associated therewith, or the like. FIG. 10 also shows the HbCO measurement being about 20% (as illustrated on the HbCO bar 212 and multi-mode display 206) thereby indicating a potentially dangerous situation that if exacerbated, will become quite problematic. Therefore, the alarm indicator 244 is also activated, and in some embodiments, the speaker 236 as well.

[0096] FIG. 11A illustrates a perspective view of an exemplary noninvasive multi-parameter patient monitor 1100, such as, for example, the patient monitor of FIG. 1. Moreover, FIGS. 11B-11E illustrate exemplary display screens of the patient monitor of FIG. 11A. As shown in FIGS. 11A-11B, an embodiment of the monitor 1100 includes a display 1101 showing a plurality of parameter data. For example, the display may advantageously comprise a CRT or an LCD display including circuitry similar to that available on oximeters commercially available from Masimo Corporation of Irvine, Calif. sold under the name RadicalTM, and disclosed in the U.S. patents referenced above and incorporated above. However, an artisan will recognize from the disclosure herein many commercially available display components capable of displaying multiple parameter data along with the ability to display graphical data such as plethysmographs, trend traces, and the like.

[0097] In an embodiment, the display includes a measured value of SpO₂ 1102, a measured value of pulse rate 1104 in BPM, a plethysmograph 1106, a measured value of HbCO 1108, a measured value of HbMet 1110, a measured value of a perfusion quality 1112, a measured value of HbT 1114, and a derived value of fractional saturation "SpaO₂" 1116. In an embodiment, SpaO₂ comprises HbO₂ expressed as a percentage of the four main hemoglobin species, i.e., HbO₂, Hb, HbCO, and HbMet.

[0098] In an embodiment, one or more of the foregoing parameter includes trending or prediction indicators 1118 showing the current trend or prediction for that corresponding parameter. In an embodiment, the indicators 1118 may advantageously comprise an up arrow, a down arrow, and a hyphen bar to indicate up trending/prediction, down trending/prediction, or neutral trending/prediction.

[0099] FIG. 11C illustrates an exemplary display screen showing trend graph 1140 including trend line 1142 for HbMet. In an embodiment, the trend line 1142 may be advantageously colored for quick straightforward recognition of the trending parameter, may be associated with any one or more of the foregoing alarm attributes, may include trending lines for other parameters, or the like. The display screen also shows trending directional indicators 1142, 1144 for many of the displayed physiological parameters. In an embodiment, the directional indicators 1142, 1144 may advantageously comprise arrows showing the recent trend, predicted trend, user-customizable trend, combinations thereof, or the like for the associated parameters. In an embodiment, the directional indicators 1142, 1144 comprises an up arrow indicating a rising trend/predicted trend, a middle bar indicating a somewhat stable trend/predicted trend, and a down arrow indicating a lowering trend/predicted trend. An artisan will recognize a wide variety of other directional indicators 1142, 1144 from the disclosure herein.

[0100] FIG. 11D shows an exemplary display screen in vertical format. Such vertical format could be user actuated or based on a gravity switch. FIGS. 11E-11F illustrate additional displays of various physiological parameters similar to those discussed in the foregoing. As shown in FIG. 11G, the display includes a measured value of SpO₂ 1162, a measured value of pulse rate 1164 in BPM, a plethysmograph 1166, a HbCO bar 1168, and a HbMet bar 1170. In an embodiment, the HbCO bar 1168 and HbMet bar 1170 may advantageously behave the same or similarly to the HbCO bar 212 and HbMet bar 712. Moreover, similar bars may advantageously display any of the physiological parameters discussed herein using display indicia appropriate to that parameter. For example, a SpO₂ or SpaO₂ bar may advantageously range from about 0% to about 100%, and more preferably range from about 50% to about 100%, while a Hbt bar may advantageously range from about 0 to about 30.

[0101] Moreover, similar to the disclosure above, the measured value of SpO₂ 1162 may advantageously toggle to measured values of HbCO, HbMet, Hbt, or the like based on, for example, actuation of user input keys, or the like.

[0102] In addition to the foregoing, the display may also include graphical data showing one or more color-coded or other identifying indicia for traces of trend data. Moreover, other graphical presentations may advantageously provide readily identifiable indications of monitored parameters or combinations of monitored parameters of the patient. For example, in an embodiment, the display includes a SpaO₂ graph 1172. The SpaO₂ graph 1172 plots SpO₂ as a function of other blood analytes (1-SpaO₂), where SpaO₂ comprises HbO₂ expressed as a percentage of the four main hemoglobin species, i.e., HbO₂, Hb, HbCO, and HbMet. Thus, as shown in FIG. 11C, as the slope of the displayed line or arrow increases, the caregiver can readily note that the majority of hemoglobin carriers are being used to carry oxygen, and not, for example, harmful carbon monoxide. On the other hand, as the slope decreases, the caregiver can readily and advantageously note that the number of hemoglobin species available to carry oxygen is decreasing, regardless of the current value of SpO₂. Moreover, the length of the arrow or line also provides an indication of wellness, e.g., the higher the line the more oxygen saturation, the lower the line, the more likely there may be desaturation event, or the like.

[0103] Thus, the SpaO₂ graph 1172 provides the caregiver with the ability to recognize that even though the measured value of SpO₂ may be within acceptable ranges, there are potentially an unacceptable number of hemoglobin carriers unavailable for carrying oxygen, and that other potential

problems may exist, such as, for example, harmful carbon monoxide levels, or the like. In an embodiment, various alarm conditions may cause the graph 1172 to change color, flash, or any combination of alarm indications discussed in the foregoing. Moreover, FIG. 11I illustrates yet an additional display of the foregoing parameters.

[0104] An embodiment may also include the monitor 1100 advantageously defining regions of wellness/severity of the monitored patient. For example, because the graph 1172 comprises two dimensions, the monitor 1100 may advantageously define regions where the patient's measured physiological parameters are considered acceptable, regions where the patient is considered at risk, regions where the patient is critical, and the like. For example, one region of acceptability may include a high SpO₂ and a low 1-SpaO₂, another region of risk may include a high SpO₂ and a high 1-SpaO₂, and another critical region may include a low SpO₂ and a high 1-SpaO₂. Moreover, an artisan will recognize from the disclosure herein that different parameters may also be combined to provide readily identifiable indications of patient wellness.

[0105] In addition to or as an alternative to the two dimensional SpaO₂ graph 1172, the monitor 1100 may also include a three dimensional graph, such as, for example, extending the graph 1172 along the variable of time. In this embodiment, the foregoing regions advantageously become three dimensional surfaces of wellness. Moreover, trend data may also be advantageously added to the surface to provide a history of when particular monitored parameters dipped in and out of various surfaces of wellness, risk, criticality, or the like. Such trend data could be color-coded, text identified, or the like. An artisan will also recognize that such surfaces may be dynamic. For example, measurements of HbCO > about 5 may dictate that trend data showing SpO₂ < about 90% should be considered critical; however, measurements of HbCO < about 5 may dictate only SpO₂ < about 85% would be critical. Again, an artisan will recognize from the disclosure herein other parameter combinations to create a wide variety of wellness/critical regions or surfaces that provide readily available visual or audio indications of patient well being, trigger specific alarms, or the like.

[0106] Moreover, the monitor 1100 may advantageously employ enlargement or reorganization of parameter data based on, for example, the severity of the measurement. For example, the monitor 1100 may display values for HbCO in a small portion of the screen or in the background, and when HbCO begins to approach abnormal levels, the small portion may advantageously grown as severity increases, even in some embodiments to dominate the display. Such visual alarming can be combined with audio alarms such as announcements, alarms, rising frequencies, or the like, and other visual alarms such as flashing, coloration, or the like to assist a caregiver in noticing the increasing severity of a monitored parameter. In an embodiment, a location of the display of an alarming value is changed to be displayed in a larger display area, such as 1102, so as to be readily noticeable and its display values readily ascertainable.

[0107] Although the foregoing invention has been described in terms of certain preferred embodiments, other embodiments will be apparent to those of ordinary skill in the art from the disclosure herein. For example, the monitor 100 may advantageously be adapted to monitor or be included in a monitor capable of measuring physiological parameters other than those determined through absorption spectros-

copy, such as, for example, blood pressure, ECG, EKG, respiratory rates, volumes, inputs for blood pressure sensors, acoustical sensors, and the like. Moreover, the monitor **100** may be adapted for wireless communication to and from the sensor **106**, and/or to and from other monitoring devices, such as, for example, multi-parameter or legacy monitoring devices.

[0108] Also, other combinations, omissions, substitutions and modifications will be apparent to the skilled artisan in view of the disclosure herein. Accordingly, the present invention is not intended to be limited by the recitation of the preferred embodiments, but is to be defined by reference to the appended claims.

[0109] Additionally, all publications, patents, and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication, patent, or patent application was specifically and individually indicated to be incorporated by reference.

What is claimed is:

1. A patient monitor capable of measuring at least two physiological parameters, the patient monitor comprising:

a display device capable of exhibiting a first measured value of a first physiological parameter of body tissue of a monitored patient in a first display area or a second measured value of a second physiological parameter of the body tissue in the first display area;

a mode selector actuatable by a user to choose which of the first and second measured values is exhibited in the first display area; and

a mode indicator generally associated with the mode selector and adapted to inform the user as to which of the measured values would be exhibited in the first display area upon actuation of the mode selector.

2. The patient monitor of claim **1**, wherein the mode indicator is adapted to inform the user as to which of the measured values is being exhibited in the first display area.

3. The patient monitor of claim **1**, wherein the mode indicator is proximate to the mode selector.

4. The patient monitor of claim **1**, wherein the display device is capable of exhibiting a third measured value of a third physiological parameter of body tissue of a monitored patient in a second display area or a fourth measured value of a fourth physiological parameter of the body tissue in the second display area, the mode indicator adapted to inform the user as to which of the measured values would be exhibited in the first and second display areas upon actuation of the mode selector.

5. The patient monitor of claim **3**, wherein the mode indicator is adapted to inform the user as to which of the measured values are being exhibited in the first and second display areas.

6. The patient monitor of claim **1**, wherein the mode indicator comprises a printed diagram.

7. The patient monitor of claim **1**, wherein the mode indicator comprises an illuminated representation.

8. The patient monitor of claim **7**, wherein the illuminated representation comprises a light emitting diode corresponding to each of the at least two physiological parameters.

9. The patient monitor of claim **4**, wherein the mode indicator comprises an illuminated representation.

10. The patient monitor of claim **9**, wherein the illuminated representation comprises a light emitting diode corresponding to each of the at least two physiological parameters.

11. The patient monitor of claim **9**, wherein the illuminated representation comprises a light emitting diode corresponding to pluralities of the at least two physiological parameters.

12. The patient monitor of claim **1**, wherein the first physiological parameter comprises % SpCO.

13. The patient monitor of claim **1**, wherein the second physiological parameter comprises % SpO₂.

14. The patient monitor of claim **1**, wherein the first physiological parameter comprises % SpMet.

15. The patient monitor of claim **1**, wherein the second physiological parameter comprises BPM.

16. A method of exhibiting at least two measurements of physiological parameters of body tissue of a monitored patient on a display device of a patient monitor, the display device comprising a first display area being generally capable of displaying a single physiological parameter measurement, the method comprising:

exhibiting a first measurement of a first physiological parameter of the body tissue in the first display area;

informing a user with a mode indicator as to which of the at least two measurements would be exhibited in the first display area upon actuation of a mode selector;

selecting a second measurement of a second physiological parameter of the body tissue to be exhibited in the first display area;

associating the second measurement with the mode indicator; and

actuating the mode selector at least once to stop exhibiting the first measurement in the first display area and to start exhibiting the second measurement in the first display area.

17. The method of claim **16**, further comprising informing the user as to which of the at least two physiological parameter measurements is being exhibited in the first display area.

18. The method of claim **16**, wherein the display device further comprises a second display area being generally capable of displaying a single physiological parameter measurement and wherein the method further comprises:

prior to actuating the mode selector, exhibiting a third measurement of a third physiological parameter of the body tissue in the second display area;

informing the user with the mode indicator as to which of the at least two physiological parameter measurements would be exhibited in the second display area upon actuation of the mode selector;

selecting a fourth measurement of a fourth physiological parameter of the body tissue to be exhibited on the second display area; and

associating the fourth measurement with the mode indicator, wherein actuating the mode selector stops exhibiting the third measurement in the second display area and starts exhibiting the fourth measurement in the second display area.

19. The method of claim **18**, further comprising informing the user as to which of the at least two physiological parameter measurements are being exhibited in the first and second display areas.

20. The method of claim **18**, wherein the first measurement is related to the third measurement and wherein the second measurement is related to the fourth measurement.

* * * * *

专利名称(译)	无创多参数病人监护仪		
公开(公告)号	US20080221418A1	公开(公告)日	2008-09-11
申请号	US11/768845	申请日	2007-06-26
[标]申请(专利权)人(译)	梅西莫股份有限公司		
申请(专利权)人(译)	Masimo公司		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	AL ALI AMMAR KIANI JOE E COVERSTON RON DIAB MOHAMED LARUE KRISTEN MARABLE RUSS OLSON GREG WU ROGER DOI JONES STEPHANIE MIEKO FISHEL RICK		
发明人	AL-ALI, AMMAR KIANI, JOE E. COVERSTON, RON DIAB, MOHAMED LARUE, KRISTEN MARABLE, RUSS OLSON, GREG WU, ROGER DOI JONES, STEPHANIE MIEKO FISHEL, RICK		
IPC分类号	A61B5/00		
CPC分类号	A61B5/02416 A61B5/14546 A61B2560/0406 A61B5/7475 A61B5/14551 A61B5/742		
优先权	60/894147 2007-03-09 US		
外部链接	Espacenet USPTO		

摘要(译)

本公开的实施例包括手持式多参数患者监视器，其能够从能够检测由身体组织衰减的光的光敏检测器的输出确定多个生理参数。例如，在一个实施例中，监视器能够有利且准确地显示脉搏率，体积描记器数据，灌注质量，信号置信度和身体组织中血液成分的值中的一个或多个，包括例如动脉一氧化碳饱和度，高铁血红蛋白饱和度，总血红蛋白，动脉血氧饱和度，分数动脉血氧饱和度等。在一个实施例中，监视器有利地包括多个显示模式，使得能够显示比可用物理显示器不动产更多的参数数据。在一个实施例中，监视器有利地包括模式指示器，用于在启动模式选择器时通知用户将在一个或多个显示区域中显示哪个参数测量。

