



US 20110112431A1

(19) **United States**

(12) **Patent Application Publication**
Golosarsky et al.

(10) **Pub. No.: US 2011/0112431 A1**

(43) **Pub. Date: May 12, 2011**

(54) **NEUROPATHY DIAGNOSTIC DEVICE**

Related U.S. Application Data

(75) Inventors: **Boris Golosarsky**, Nashua, NH (US); **James Bernhard**, Plainville, MA (US); **Michael Brown**, Nashua, NH (US); **John McCarthy**, Newbury, NH (US)

(60) Provisional application No. 61/081,536, filed on Jul. 17, 2008.

Publication Classification

(73) Assignee: **ELECTRONIC PRODUCTS ACCESSORIES & CHEMICALS, LLC**, Plainville, MA (US)

(51) **Int. Cl.**
A61B 5/00 (2006.01)

(52) **U.S. Cl.** **600/552; 600/555**

(57) **ABSTRACT**


A neuropathy diagnostic device includes a body having a neutral temperature surface disposed on an exterior of the body, a variable temperature surface disposed on the exterior of the body, and a vibrating surface having a variable vibration amplitude. The vibrating surface extends outwardly from the body. A touch sensor extends outwardly from the body. A processor is disposed within the body. The processor is adapted to set a temperature of the neutral temperature surface, vary a temperature of the variable temperature surface, and vary the vibration amplitude of the vibrating surface.

(21) Appl. No.: **13/054,136**

(22) PCT Filed: **Jul. 17, 2009**

(86) PCT No.: **PCT/US2009/004159**

§ 371 (c)(1),
(2), (4) Date: **Jan. 14, 2011**

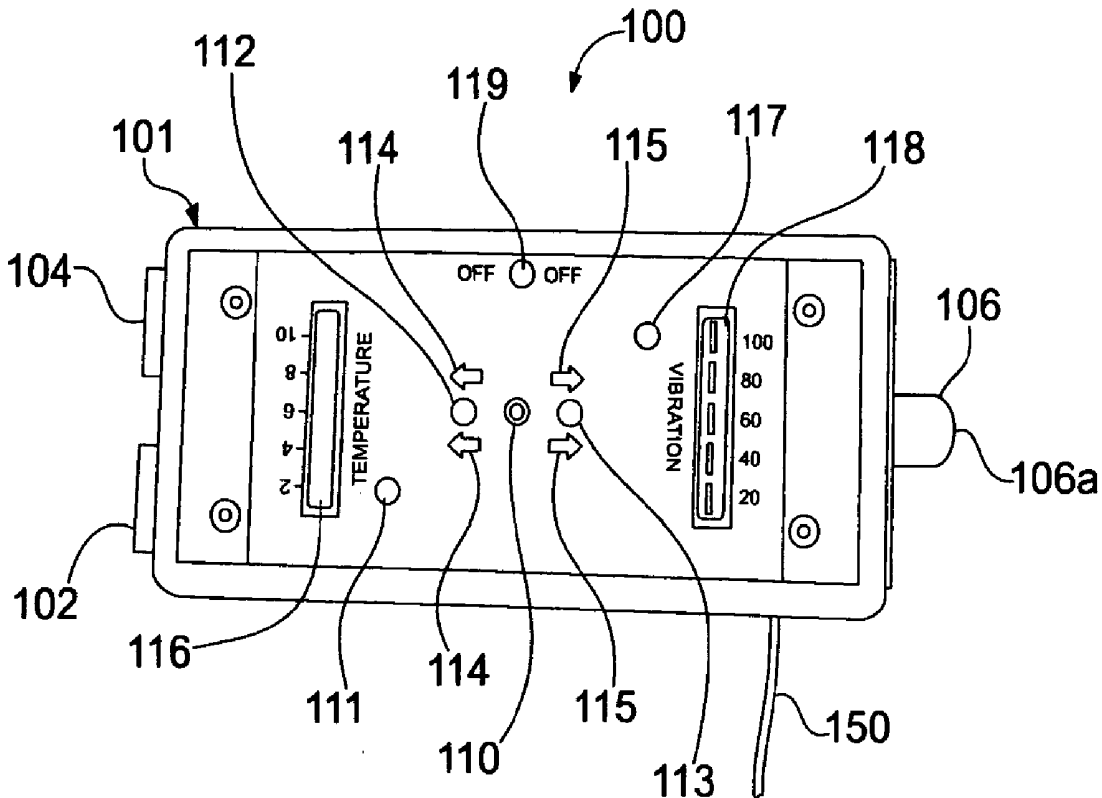

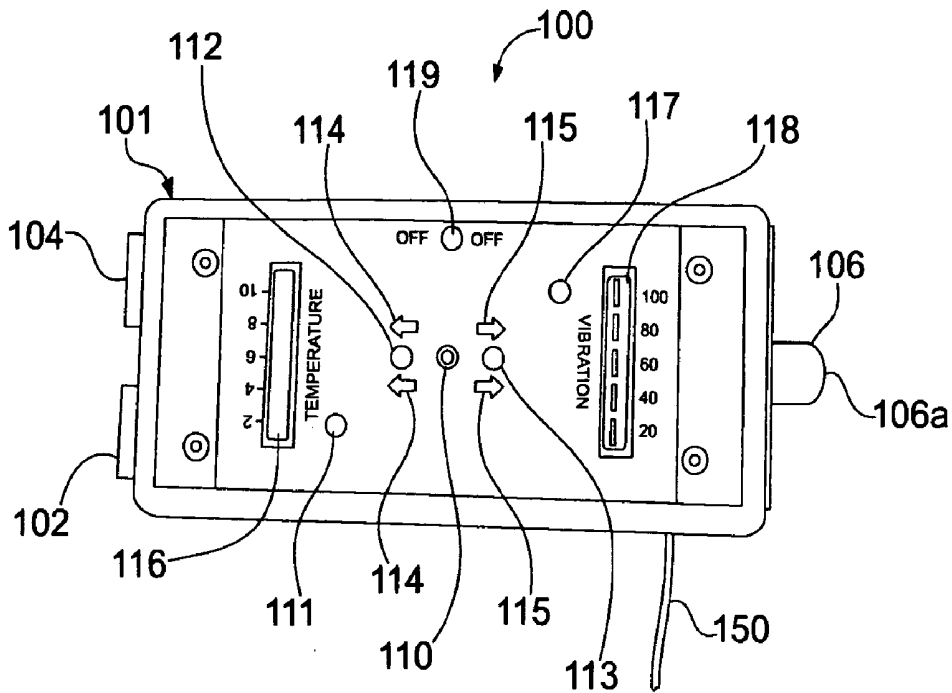


Fig. 1

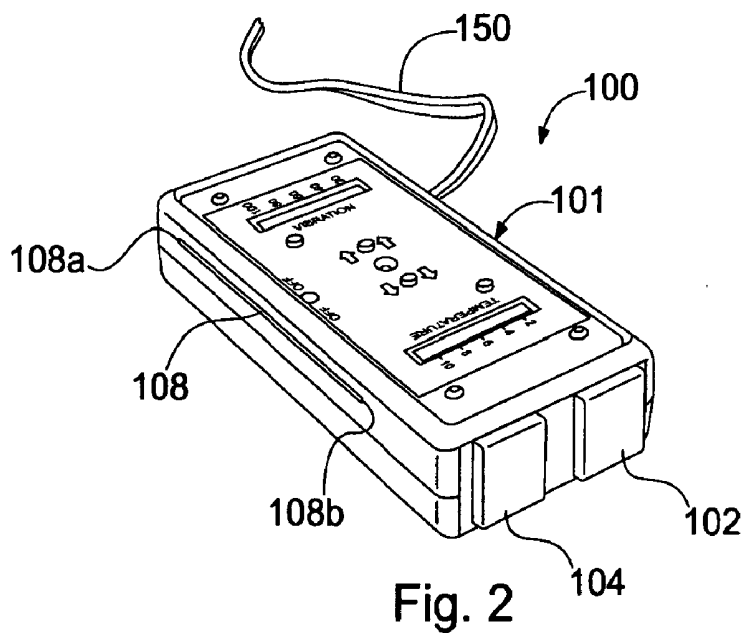


Fig. 2

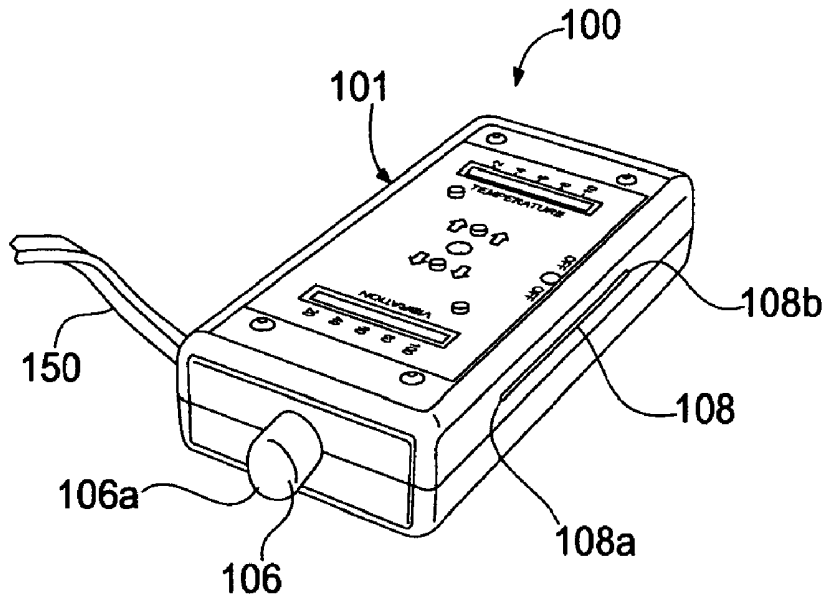


Fig. 3

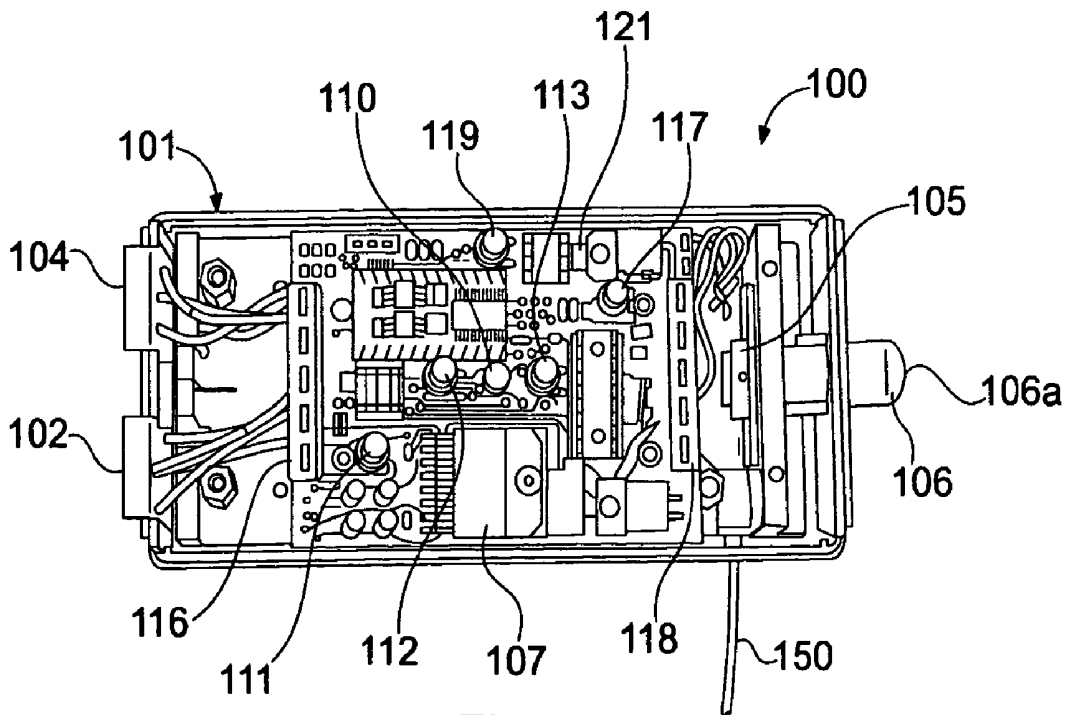
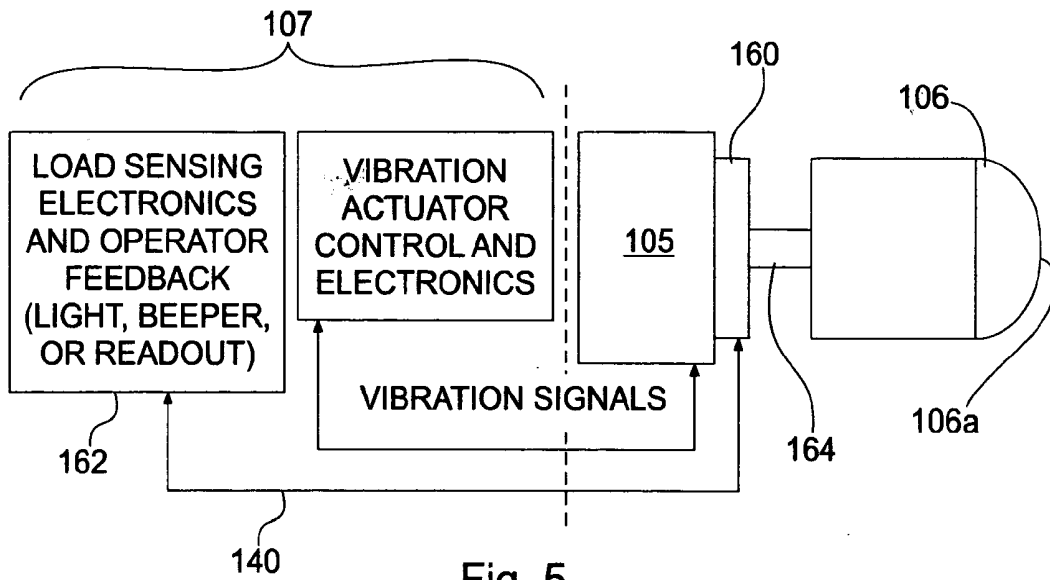


Fig. 4



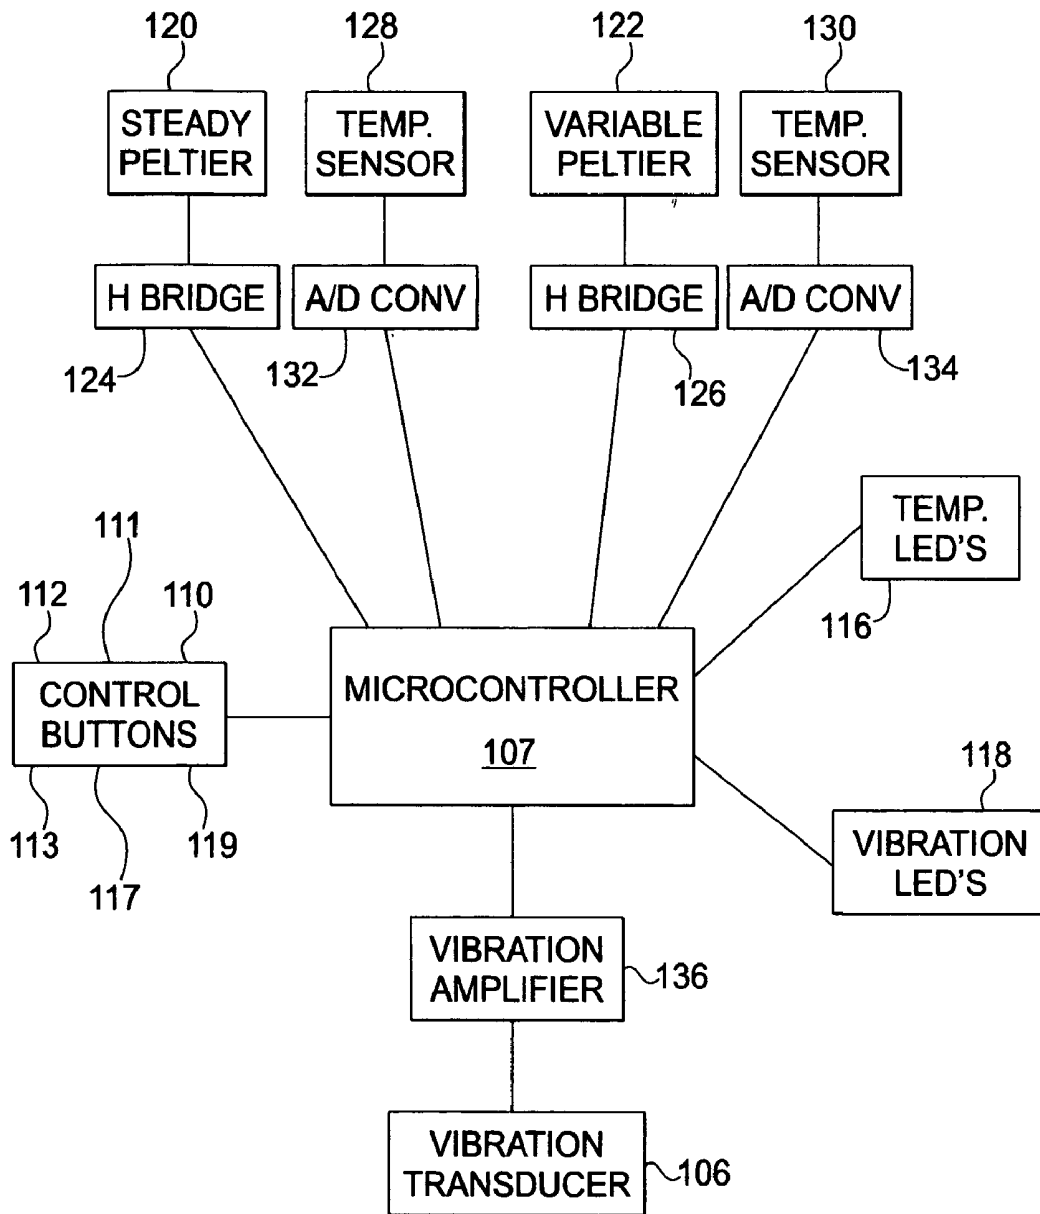


Fig. 6

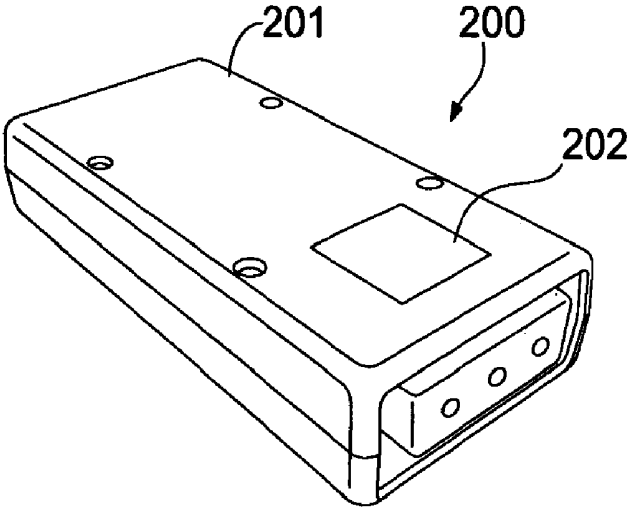


Fig. 7

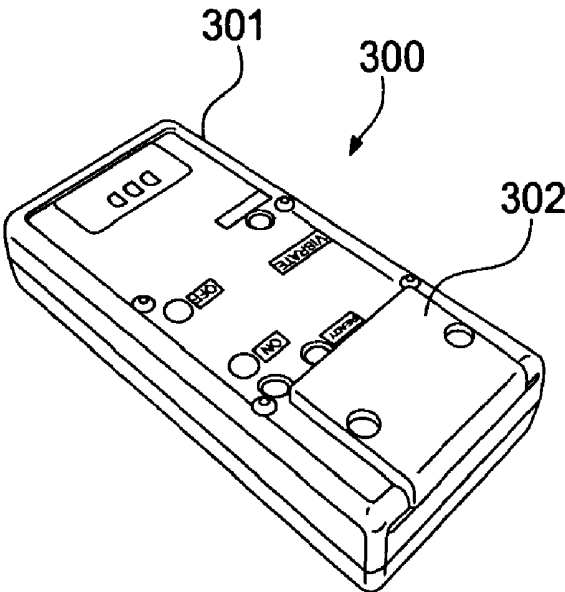


Fig. 8

NEUROPATHY DIAGNOSTIC DEVICE

CROSS-REFERENCE TO RELATED APPLICATION

[0001] The present application claims priority from U.S. Provisional Patent Application Ser. No. 61/081,536, filed on Jul. 17, 2008, which is incorporated by reference in its entirety.

BACKGROUND OF THE INVENTION

[0002] Neuropathy is a medical condition where a patient has reduced sensitivity in through-the-skin sensing of temperature variations, vibrations, and tactile stimulation. Neuropathy is common for patients with diabetes. Attention to diabetes has increased significantly as more individuals are being diagnosed with some form of the disease. Early and accurate diagnosis of neuropathies associated with diabetes or other medical issues may lead to earlier treatment to reduce the effect of these issues on the patient.

SUMMARY OF THE INVENTION

[0003] Briefly, the present invention provides a neuropathy diagnostic device that includes a body having a neutral temperature surface disposed on an exterior of the body, a variable temperature surface disposed on the exterior of the body, and a vibrating surface having a variable vibration amplitude. The vibrating surface extends outwardly from the body. A touch sensor extends outwardly from the body. A processor is disposed within the body. The processor is adapted to set a temperature of the neutral temperature surface, vary a temperature of the variable temperature surface, and vary the vibration amplitude of the vibrating surface.

BRIEF DESCRIPTION OF THE DRAWINGS

[0004] The foregoing summary, as well as the following detailed description of exemplary embodiments of the invention, will be better understood when read in conjunction with the appended drawings, which are incorporated herein and constitute part of this specification. For the purposes of illustrating the invention, there are shown in the drawings exemplary embodiments of the present invention. It should be understood, however, that the invention is not limited to the precise arrangements and instrumentalities is shown. In the drawings, the same reference numerals are employed for designating the same elements throughout the several figures. In the drawings:

[0005] FIG. 1 is a top plan view of a neuropathy detection device according to an exemplary embodiment of the present invention;

[0006] FIG. 2 is a front perspective view of the neuropathy detection device of FIG. 1;

[0007] FIG. 3 is a rear perspective view of the neuropathy detection device of FIG. 1;

[0008] FIG. 4 is a top plan view of the neuropathy detection device of FIG. 1, with the top cover removed;

[0009] FIG. 5 is a schematic drawing of an exemplary embodiment of a force sensor for a vibrating end effector in the neuropathy detection device of FIG. 1;

[0010] FIG. 6 is a block diagram illustrating a functional layout of a circuit used to operate the neuropathy detection device of FIG. 1;

[0011] FIG. 7 is a top perspective view of a neuropathy detection device according to an alternative exemplary embodiment of the present invention; and

[0012] FIG. 8 is a top perspective view of a neuropathy detection device according to another alternative exemplary embodiment of the present invention.

DETAILED DESCRIPTION OF THE INVENTION

[0013] Although the invention is illustrated and described herein with reference to specific embodiments, the invention is not intended to be limited to the details shown. Rather, various modifications may be made in the details within the scope and range of equivalents of the disclosure without departing from the invention. The invention is best understood from the following detailed description when read in connection with the accompanying drawing figures, which show exemplary embodiments of the invention selected for illustrative purposes. The invention will be illustrated with reference to the figures. Such figures are intended to be illustrative rather than limiting and are included is herewith to facilitate the explanation of the present invention.

[0014] Referring to FIGS. 1-4 in general, a neuropathy detection device 100 ("device 100") that is used to diagnose neuropathy in patients is shown. Neuropathy is common for patients with medical issues, such as diabetes or erectile dysfunction. Device 100 includes a body 101 having an exposed neutral temperature surface 102 and an exposed variable temperature surface 104 at one end of body 101, and an exposed vibration surface 106 that extends outwardly from an opposing end of body 101. A filament 108 extends outwardly from body 101. Filament 108 may be a monofilament, such as nylon wire.

[0015] A medical professional, such as, for example, a physician, may use device 100 on a patient by touching various locations on the patient's skin with surfaces 102, 104, 106 and/or filament 108. The patient's reaction to these touches may give the physician an indication of a level of neuropathy in the patient, which may in turn aid or enable the physician to diagnose the patient.

[0016] Two separate modes of operation are provided for device 100: temperature (using surfaces 102, 104) and vibration (using surface 106), as well as a tactile test (using filament 108). Each mode can be utilized at any time and the operator may switch back and forth between the two modes and/or the tactile test. Controls and indicators are included on s body 101 to allow the operator to control surfaces 102, 104, 106 and to give the operator an indication of the operating parameters of surfaces 102, 104, 106. A controller, such as a microcontroller 107, shown in FIGS. 4 and 5, is used to control operation of surfaces 102, 104, 106.

[0017] The patient's ability to discern the differences between the temperatures of neutral temperature surface 102 and variable temperature surface 104, positioned at various locations on the patient's skin, gives the physician an indication of the level of neuropathy. Referring specifically to FIGS. 1, 2, and 4, in an exemplary embodiment, neutral temperature surface 102 and variable temperature surface 104 are both generally square, flat pads with sides that are about 1-1/2 to 2 cm long.

[0018] Variable temperature surface 104 may be independently controlled by the operator such that the temperature difference between neutral temperature surface 102 and variable temperature surface 104 varies up to about 10 degrees Celsius. In an exemplary embodiment, neutral temperature

surface 102 may be set by controller 107 at about 25 degrees Celsius. Variable temperature surface 104 may be varied at 2 degree increments between a temperature of between about 15 and about 25 degrees Celsius. While in this exemplary embodiment, the temperature of variable temperature surface 104 may be set to be lower than the temperature of neutral temperature surface 102, those skilled in the art will recognize that the temperature of variable surface 104 may be set higher than the temperature of neutral temperature surface 102.

[0019] A power indicator LED 110 illuminates when power is provided to device 100. A temperature mode button 111 may be pressed to activate the temperature mode and to provide power to heat surfaces 102, 104. Neutral temperature surface 102 is powered to a fixed temperature, such as, for example, 25 degrees Celsius, and variable temperature surface 104 at a variable temperature in degree increments, such as, for example, increments of 2 degrees Celsius. The operator can control the temperature of variable temperature surface 104 by using increment buttons 112, 113. Arrows 114 on either side of increment button 112 pointing toward surfaces 102, 104 indicate that the operation of increment button 112 raises the temperature difference between neutral temperature surface 102 and variable surface 104, while arrows 115 on either side of increment button 113 pointing away from surfaces 102, 104 indicate that the operation of increment button 113 lowers the temperature difference between neutral temperature surface 102 and variable surface 104. An LED bar graph 116 displays a temperature offset between neutral temperature surface 102 and variable temperature surface 104. An "Off" button 119 turns off device 100.

[0020] Temperature variations on surfaces 102, 104 are created through standard solid state thermoelectric devices known as "Peltier Devices." As shown in FIG. 5, a Peltier Device 120 labeled "Steady Peltier" controls neutral temperature surface 102 (shown in FIG. 1), while a Peltier Device 122 labeled "Variable Peltier" controls variable temperature surface 104 (shown in FIG. 1).

[0021] A Peltier Device is essentially a solid state heat pump with no moving parts. A DC voltage is applied to the device, which causes heat to move from one side to the other. This movement of the heat causes an apparent cooling of one side and heating of the other side. Exemplary Peltier Devices used for surfaces 102, 104 may be about 1.25 cm square and about 0.25 cm thick. The direction of heat flow within a Peltier Device can be reversed by simply reversing the polarity of the DC current applied to the device. By constructively controlling the current level and polarity of the current applied to a Peltier Device, a constant temperature can be maintained.

[0022] Peltier Devices 120, 122 used in the exemplary embodiment of device 100 may be identical. Each Peltier Device 120, 122 is powered by a separate dual H Bridge 124, 126, respectively. An H bridge has two outputs that can have its output commanded to reverse polarity. An H bridge is either "on" or "off," meaning that the H bridge either delivers full power to the Peltier, or no power. Since it is necessary to set various heat pump levels (and therefore temperature as measured on surfaces 102, 104), controller 107 varies the electrical current levels to H bridges 124, 126. This may be done via pulse width modulation (PWM) which provides a repeated signal of "on" and then "off." The relative time of "off" versus "on" will set, on average, the power going to each

Peltier Device 120, 122 and therefore the temperature at surfaces 102, 104, respectively.

[0023] Each surface 102, 104 includes a respective temperature sensor 128, 130, which provides feedback to microcontroller 107 via a respective analog to digital (A/D) converter 132, 134.

[0024] The patient's ability to discern vibrations at various locations on the patient's skin also gives the physician an indication of the level of neuropathy. Referring specifically to FIGS. 1, 3, and 4, vibration surface 106 may extend outwardly from body 101 and have a generally cylindrical shape with a hemispherical end. Vibration surface 106 may be controlled to vibrate in and out at constant frequency, but with a variable amplitude. In an exemplary embodiment, vibration surface 106 vibrates at a frequency of about 120 Hz, is although other frequencies are also contemplated. The amplitude of vibration of vibration surface 106 may be varied between about 100 percent of full amplitude and about 20 percent of full amplitude. An LED bar graph 118 displays a percentage of vibration amplitude relative to a maximum available amplitude. In an exemplary embodiment, the amplitude may be adjusted in 20 percent increments (100, 80, 60, 40, or 20 percent of full amplitude), although those skilled in the art will recognize that other increments may be used.

[0025] As illustrated in FIG. 5, in an exemplary embodiment, vibration for vibrating surface 106 may be provided by a magnetic coil moving a magnet (shown collectively as magnet 105). The magnet 105 may be coupled to vibrating surface 106. A signal from microcontroller 107 to the coil is a constant frequency. A low power signal from microcontroller 107 may be amplified using a simple operational amplifier 136 (shown schematically in FIG. 6) and transistor (not shown). The amplitude of the vibration is also controlled by microcontroller 107. While an exemplary mechanism for vibrating the vibrating surface 106 is shown, those skilled in the art will recognize that other mechanisms may be used.

[0026] Referring to FIGS. 1 and 4, increment buttons 112, 113 may be used to adjust the vibration amplitude down or up as desired. Increment button 113 will increase the vibration amplitude, while increment button 112 will decrease the vibration amplitude. "Off" button 119 turns off device 100.

[0027] Optionally, as illustrated in FIG. 5, vibration surface 106 may incorporate a pressure sensor 140. Pressure sensor 140 may include a load cell 160 that is electronically coupled to a load sensing electronics component 162 in controller 107 and generates an indication when sufficient pressure is applied by device 100 on the patient's skin. The indication may be an audible indication, such as, for example, a beep, a visual indication such as, for example, a light, or some other suitable type of indication to signify to the user that device 100 is being applied to the patient's skin with sufficient force to enable the patient to sense the vibrations from vibration surface 106. The indicator would operate as is long as the pressure applied to the patient is sufficient to enable the patient to sense the vibrations.

[0028] Load cell 160 may be coupled to magnet 105 and disposed between magnet 105 and vibration surface 106. Optionally, as illustrated in FIG. 5, a mechanical extension 164 may couple load cell 160 to vibration surface 106.

[0029] Referring to the control diagram of FIG. 6, microcontroller 107 may be used to control the temperature of surfaces 102, 104 and the vibration of vibration surface 106. Microcontroller 107 is disposed within body 101 and may be an 8 bit industrial processor with 16 digital inputs and out-

puts. An associated printed circuit board **121** (shown in FIG. **4**) not only contains the circuitry, but also provides the proper layout and mounting for LED's **116**, **118** and buttons **110**, **111**, **112**, **113**, **117**, **119**.

[0030] Referring to FIGS. **2** and **3**, filament **108** provides a touch sensation test. In an exemplary embodiment, the tactile aspect of device **100** utilizes a standard monofilament nylon wire for filament **108**, having a free end **108a**, which is used to check the patient's tactile sensitivity. For protection when not in use, filament **108** may be disposed against the outside of body **101** and can be readily pivoted about a pivoting end **108b** by the operator at any time. Alternatively, although not shown, filament **108** may be housed within body **101** and pulled out from body **101** when desired. After use, filament **101** may be pushed back into body **101** for storage.

[0031] In an exemplary embodiment, device **100** may be powered by standard **110** volt alternating current, stepped down to 6 volt direct current through a transformer. Internally, a 5 volt regulator may be provided to provide voltage to digital components within device **100**.

[0032] Electrical power may be provided to device **100** through an electrical cord **150**, which is partially shown in FIGS. **1-4**. Alternatively, device **100** may be powered by batteries (rechargeable or disposable) that are contained within body **101** of device **100**.

[0033] While body **101** is illustrated in FIGS. **1-4** as a generally rectangular enclosure, those skilled in the art will recognize that body **101** may be other shapes as well, is including, but not limited to, a cylindrically shaped body.

[0034] Device **100** may optionally be used to record data obtained during testing. In a first embodiment, device **100** has no storage capacity within itself, but transmits data from microcontroller **107** via radio frequency or other suitable transmission medium to a storage device, such as, for example, a personal/laptop computer. The patient's profile may have already been called up on the storage device and the data transmitted from device **100** is automatically transmitted to the patient's file. The information transmitted from device **100** may include maximum/minimum temperatures and or vibration amplitudes generated by device **100**.

[0035] Alternatively, device **100** may have memory within microcontroller **107** or coupled to microcontroller **107** and the capability to receive/transmit information. Device **100** may receive patient information uploaded to device **100** from the personal/laptop computer. Device **100** may include an indicator, such as, for example, an LCD or LED screen that displays the patient information so that the operator knows that the correct patient information has been downloaded to device **100**. Data obtained during operation of device **100** is then associated with the patient information. This data may be transmitted back to the personal/laptop computer instantly, after all data for the particular patient is obtained, or even after uses with several different patients, such as, for example, at the end s of a work day. Those skilled in the art will recognize that known methods may be used to store and transmit data between device **100** and another device.

[0036] Further, if device **100** is battery operated with rechargeable batteries that are recharged by inserting device into a recharging station (not shown), the recharging station may include a port to engage device **100** for downloading data from device **100** into a storage device.

[0037] To operate device **100**, the operator turns on device **100** by pressing either temperature mode button **111** or vibra-

tion mode button **117**. The operator can press either mode button **111**, **117** at any time to switch between temperature and vibration modes.

[0038] To conserve energy (and battery power, if batteries are used), device **100** is times out after 30 seconds on its own if no buttons are pressed. Any adjustment using increment buttons **112**, **113** adds a new period of 30 seconds to the timeout mechanism. The operator can add another 30 seconds by simply pressing the appropriate mode button **111**, **117**. "Off" button **119** may be pressed at any time to shut down device **100** prior to device **100** timing out.

[0039] When device **100** is first powered on, device **100** will default to make variable temperature surface **104** have a 2 degree offset from neutral temperature surface **102**. At any time, the operator can use increment buttons **112**, **113** to adjust this offset. LED bar graph **116** shows the operator which offset is currently being provided by device **100**. There is a small delay in attaining the proper temperatures and LED bar graph **116** reflects this situation by blinking while surfaces **102**, **104** are brought to their desired temperatures. LED bar graph **116** remains steadily lit when surfaces **102**, **104** are at their desired temperature(s). The operator is free to adjust device **100** to any of the preprogrammed offsets based on his need for further tests as dictated by the patient's responses. Device **100** may be programmed to shut itself off if no buttons have been pushed for any desired time level, such as 60 seconds.

[0040] If the operator desires to operate the temperature mode first, the operator presses temperature mode button **111**. Device **100** will begin to appropriately heat or cool both temperature surfaces **102**, **104**. Device **100** will always attempt to make neutral temperature surface **102** stay at 25 degrees Celsius. If no other action is taken by the operator, device **100** will attempt to make variable temperature pad **104** two (2) degrees below the temperature of neutral temperature surface **102**. LED bar graph **116** will blink at "-2" while device **100** works to acquire the proper temperature, and will become steady when the proper temperatures on both surfaces **102**, **104** (i.e., a temperature difference of 2 degrees Celsius between surfaces **102**, **104**) are reached. Increment buttons **112**, **113** may be used to increase or decrease the temperature differential. With each change in desired offset, LED bar graph **116** moves to represent the new differential. The corresponding LED on LED bar graph **116** will blink while device **100** is working to achieve the new is temperature goal and will remain steady when the proper temperatures have been reached.

[0041] When LED bar graph **116** is illuminating in steady state, the operator then applies surfaces **102**, **104** simultaneously to an area on the patient's skin surface. The operator then asks for the patient's feedback depending on whether the patient could sense the temperature offset between surfaces **102**, **104**. This offset may first be set to the lowest amount (e.g., 2 degrees) and may then be incremented to larger offset values. In an exemplary embodiment, each increment makes variable surface **104** two (2) degrees cooler. Once the patient reports that he/she can feel the offset, the operator then knows the patient's temperature offset detection level for that particular part of the body.

[0042] In addition to temperature testing, the operator may also perform a vibration study. The operator presses vibration mode button **117**, activating vibration mode, causing vibration surface **106** to vibrate at 120 Hz, and at 100% of the amplitude of vibrating surface **106**. The operator may use

increment buttons **112**, **113** to adjust the vibration amplitude down or up as desired. Increment button **113** will increase the vibration amplitude, while increment button **112** will decrease the vibration amplitude. As noted earlier with respect to the temperature mode, device **100** shuts down after 30 seconds if no additional inputs are provided. Any adjustment to the amplitude via increment buttons **112**, **113** will reset the 30 second clock.

[0043] The operator touches an end **106a** of vibration surface **106** to the area of interest on the patient's body. Load cell **160** transmits a signal to load sensing electronics component **162**, which transmits a signal (e.g., light, audible, etc.) to the operator to let the operator know that vibration surface **106** is engaging the patient with sufficient force. With vibration surface **106** vibrating, the patient may react by stating whether or not he/she can feel the vibration. The operator may then decrease the amplitude of the vibration and obtain further patient feedback to discern where the patient's threshold limit of detection may be. The operator can freely move vibration amplitude up and down as desired, with the changes in amplitude happening virtually instantaneously.

[0044] The operator may also perform a tactile study. Filament **108** may be moved away from body **101** by rotating filament **108** about pivoting end **108b** to allow free end **108a** of filament **108** to extend away from body **101**. Free end **108a** may be gently pressed into the skin of the patient to determine the patient's sensation of filament **108** being pressed into the skin.

[0045] While an operating sequence of temperature, vibration, and touch using device **100** is described above, those skilled in the art will recognize that device **100** may be used in any other appropriate order, and in any combination of tests.

[0046] Alternative embodiments of devices **200**, **300** according to the present invention are illustrated in FIGS. **7** and **8**, respectively. Devices **200**, **300** incorporate temperature surfaces on opposing sides of body **201**, **301**, respectively. In FIGS. **6** and **7**, only neutral surfaces **202**, **302** are shown, with variable temperature surfaces, not shown, being located on the underside of body **201**, **301** respectively. In device **200**, neutral surface **202** is flush with body **201**, while in device **300**, neutral surface **302** extends outwardly from body **301**.

[0047] Although the invention is illustrated and described herein with reference to specific embodiments, the invention is not intended to be limited to the details shown. Rather, various modifications may be made in the details within the scope and range of equivalents of the claims and without departing from the invention. For example, device **100** may include three or more temperature surfaces. Alternatively, or in addition, device **100** may include two or more vibration surfaces, each capable of operating at different amplitudes and/or frequencies, or with different geometries to vary the amount of surface area in contact with the patient.

What is claimed:

1. A neuropathy diagnostic device comprising:
 - a body having:
 - a neutral temperature surface disposed on an exterior of the body;
 - a variable temperature surface disposed on the exterior of the body;
 - a vibration surface having a variable vibration amplitude, the vibration surface extending outwardly from the body; and
 - a touch sensor extending outwardly from the body; and
 - a processor disposed within the body, wherein the processor is adapted to set a temperature of the neutral temperature surface, vary a temperature of the variable temperature surface, and vary the vibration amplitude of the vibrating surface.
 2. The neuropathy diagnostic device according to claim 1, wherein the variable temperature surface is variable between a first temperature less than the neutral temperature surface and a second temperature greater than the neutral temperature surface.
 3. The neuropathy diagnostic device according to claim 2, wherein the variable temperature surface is incrementally variable by about two degrees below the neutral temperature surface.
 4. The neuropathy diagnostic device according to claim 2, wherein the variable temperature surface is incrementally variable by about two degrees above the neutral temperature surface.
 5. The neuropathy diagnostic device according to claim 1, wherein the body has a side and wherein the neutral temperature surface and the variable temperature surface are both disposed on the side.
 6. The neuropathy diagnostic device according to claim 1, wherein the body has a first side, the neutral temperature surface being disposed on the first side, and wherein the body has a second side, the variable temperature surface being disposed on the second side.
 7. The neuropathy diagnostic device according to claim 6, wherein the first side is opposite the second side.
 8. The neuropathy diagnostic device according to claim 1, wherein the vibration surface comprises a pressure sensor.
 9. The neuropathy diagnostic device according to claim 8, wherein the pressure sensor is coupled to an indicator for indicating sufficient pressure applied by the pressure sensor to a surface.
 10. The neuropathy diagnostic device according to claim 1, further comprising means for recording data generated by each of the neutral temperature surface, the variable temperature surface, and the vibration surface.

* * * * *

专利名称(译)	神经病变诊断装置		
公开(公告)号	US20110112431A1	公开(公告)日	2011-05-12
申请号	US13/054136	申请日	2009-07-17
[标]申请(专利权)人(译)	电子PRODS配饰 & CHEM		
申请(专利权)人(译)	电子产品配件 & CHEMICALS , LLC		
[标]发明人	GOLOSARSKY BORIS BERNHARD JAMES BROWN MICHAEL MCCARTHY JOHN		
发明人	GOLOSARSKY, BORIS BERNHARD, JAMES BROWN, MICHAEL MCCARTHY, JOHN		
IPC分类号	A61B5/00		
CPC分类号	A61B5/0051 A61B5/483 A61B5/4827 A61B5/441		
优先权	61/081536 2008-07-17 US		
其他公开文献	US8579830		
外部链接	Espacenet USPTO		

摘要(译)

一种神经病诊断装置，包括：主体，具有设置在主体外部的中性温度表面；可变温度表面，设置在主体的外部；以及振动表面，具有可变的振动幅度。振动表面从主体向外延伸。触摸传感器从主体向外延伸。处理器设置在主体内。处理器适于设定中性温度表面的温度，改变可变温度表面的温度，并改变振动表面的振动幅度。

