



US 20040133083A1

(19) **United States**

(12) **Patent Application Publication**
Comanicu et al.

(10) **Pub. No.: US 2004/0133083 A1**

(43) **Pub. Date: Jul. 8, 2004**

(54) **SYSTEM AND METHOD FOR REAL-TIME
FEATURE SENSITIVITY ANALYSIS BASED
ON CONTEXTUAL INFORMATION**

Related U.S. Application Data

(60) Provisional application No. 60/425,820, filed on Nov. 13, 2002. Provisional application No. 60/425,800, filed on Nov. 13, 2002.

(75) Inventors: **Dorin Comanicu**, Princeton, NJ (US);
Arun Krishnan, Exton, PA (US);
Xiang Sean Zhou, Somerset, NJ (US);
Bhavani Duggirala, Bellevue, WA
(US); **Diane Paine**, Redmond, WA (US)

Publication Classification

(51) **Int. Cl.⁷** **A61B 5/00**
(52) **U.S. Cl.** **600/301; 600/437; 600/509;**
128/920; 128/923

Correspondence Address:

Elsa Keller
Siemens Corporation
Intellectual Property Department
170 Wood Avenue South
Iselin, NJ 08830 (US)


(57) **ABSTRACT**

A system and method for assigning feature sensitivity values to a set of potential measurements to be taken during a medical procedure of a patient in order to provide a medical diagnosis is disclosed. Data is received from a sensor that represents a particular medical measurement. The received data and context data are analyzed with respect to one or more sets of training models. Feature sensitivity values are derived for the particular medical measurement and other potential measurements to be taken based the analysis, and the feature sensitivity values are outputted.

(73) Assignee: **Siemens Corporate Research Inc.**

(21) Appl. No.: **10/702,984**

(22) Filed: **Nov. 6, 2003**

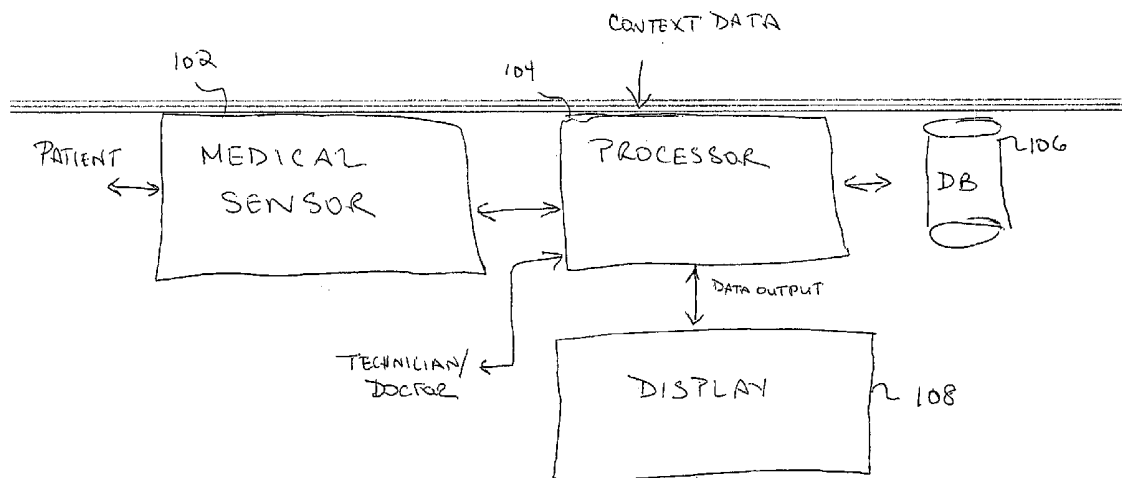

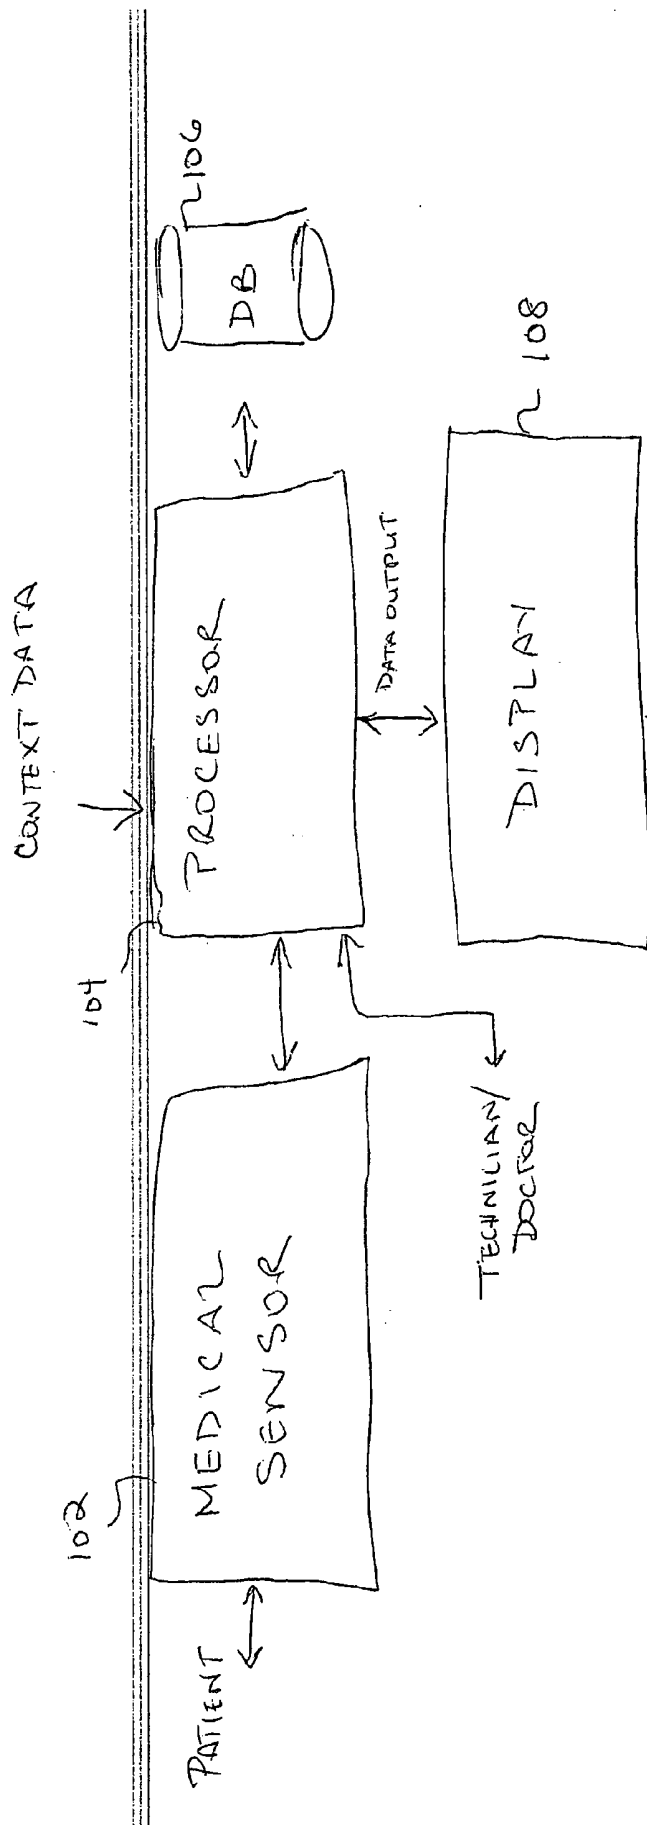


FIG. 1

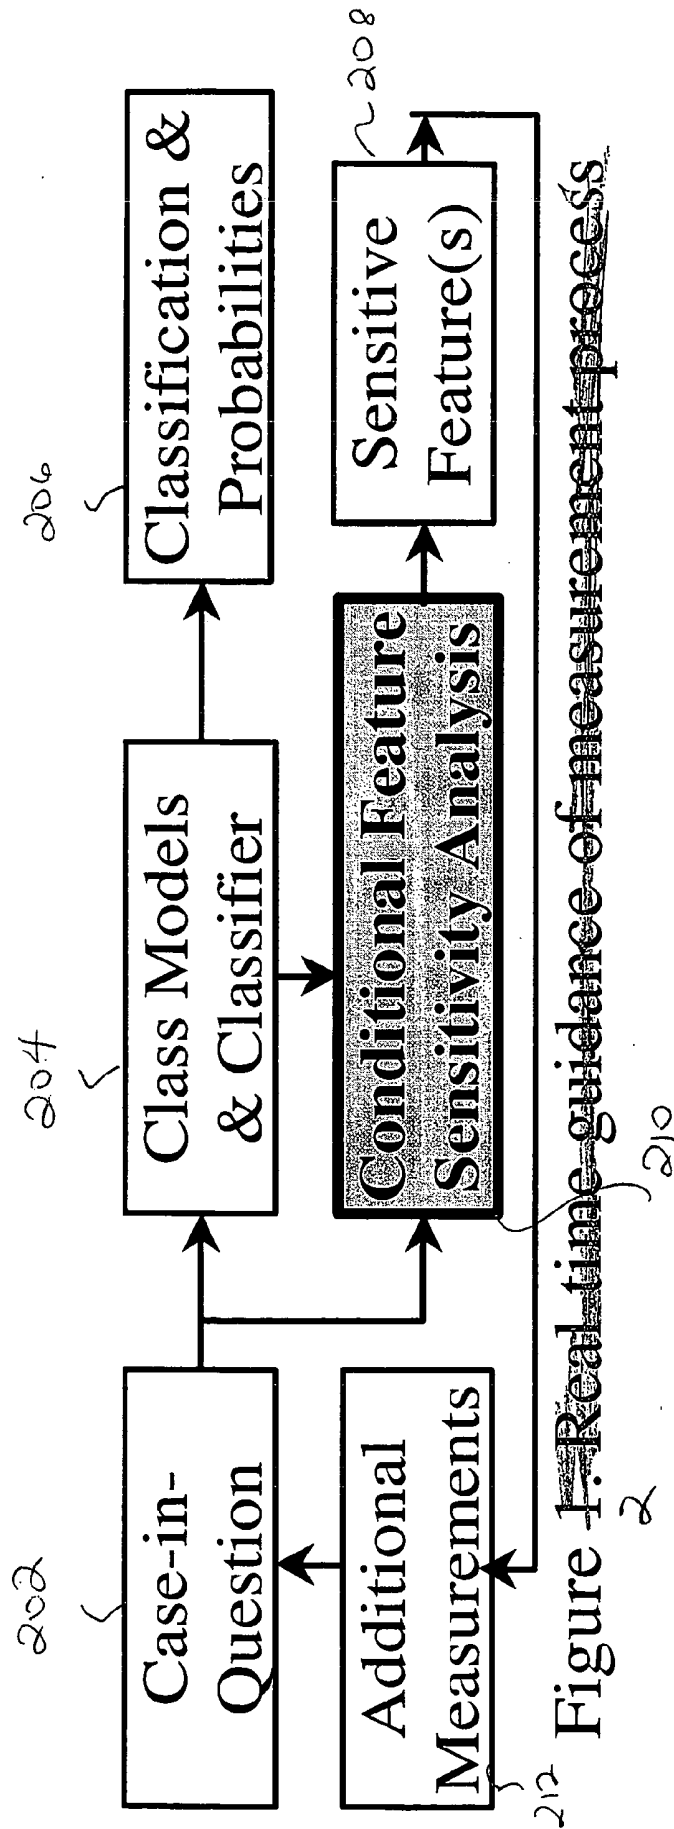
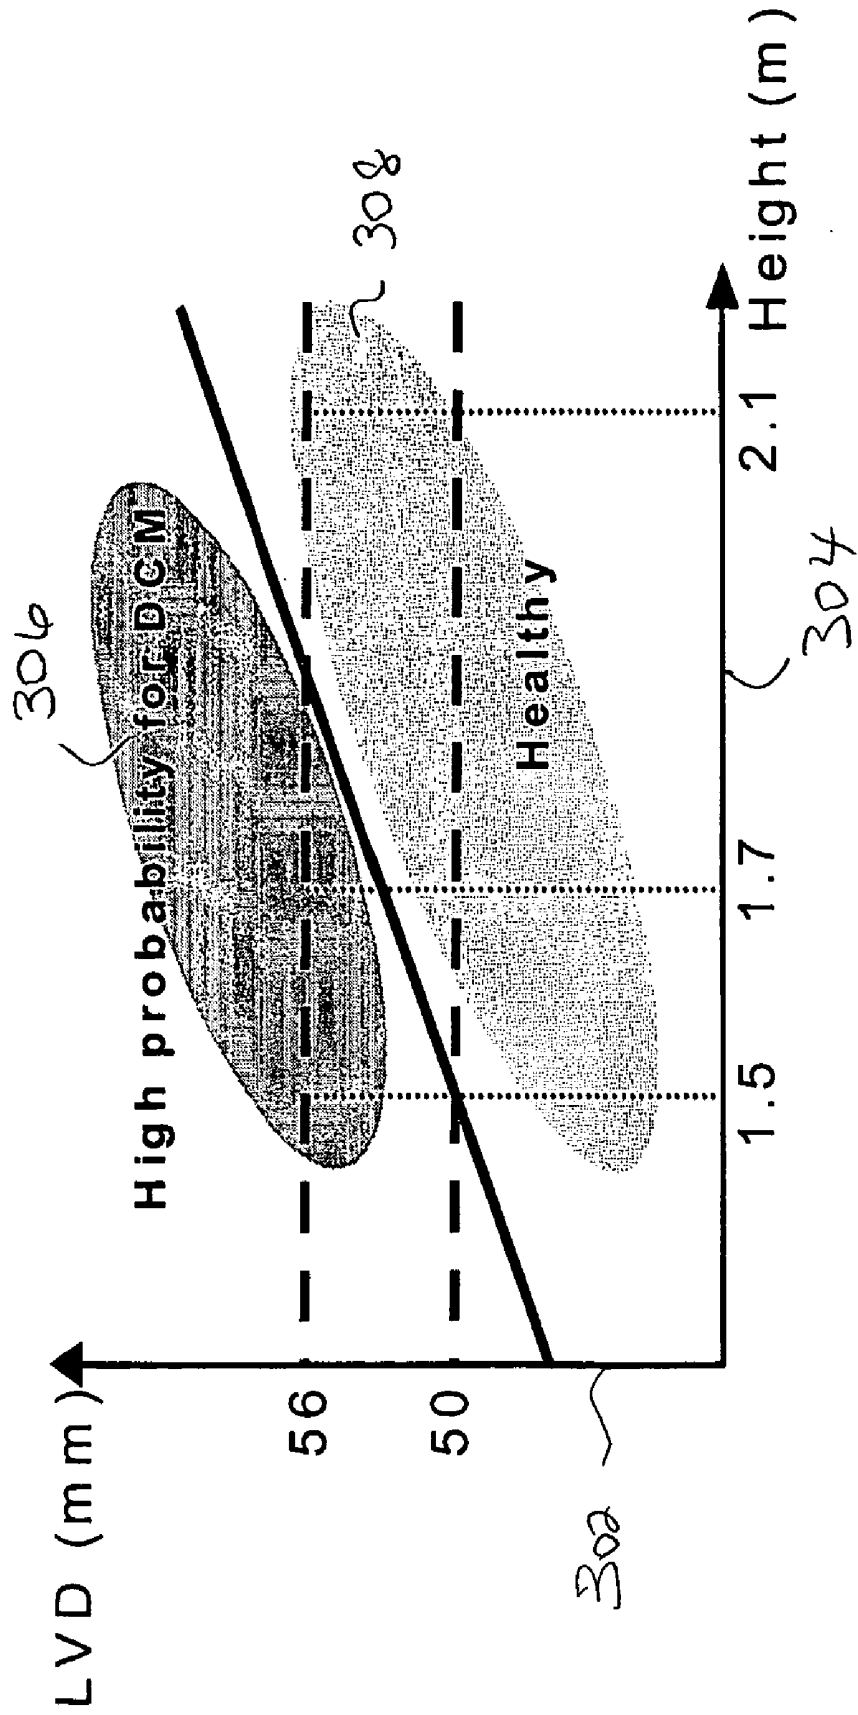


Figure 1: Real time guidance of measurement process

FIG. 3



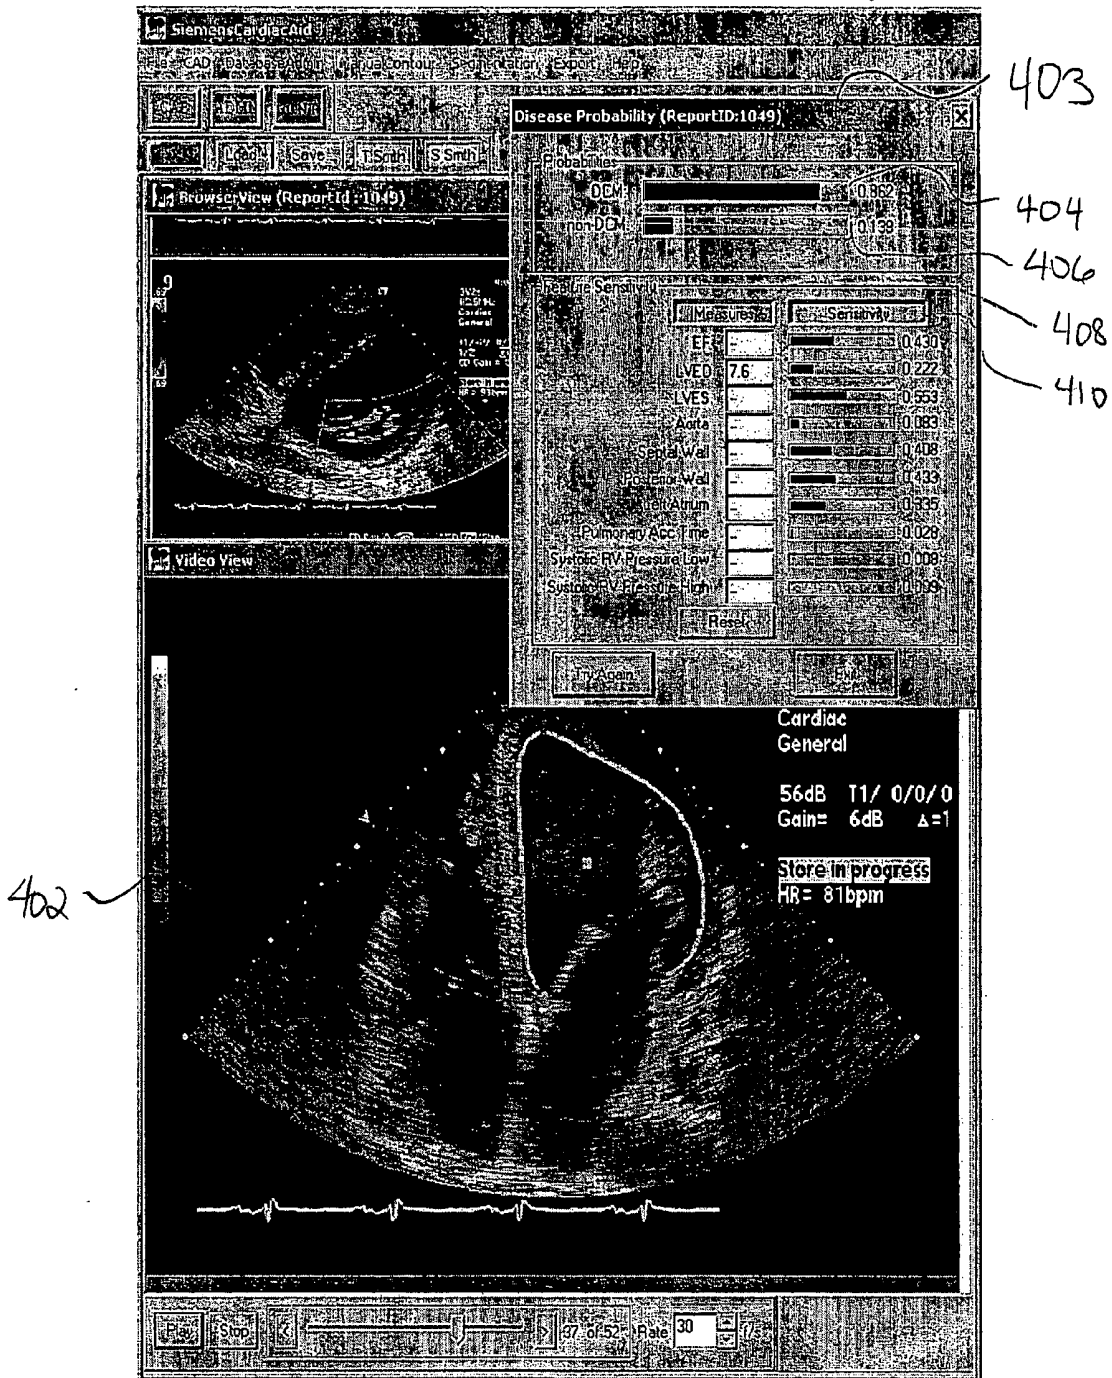


FIG. 4

SYSTEM AND METHOD FOR REAL-TIME FEATURE SENSITIVITY ANALYSIS BASED ON CONTEXTUAL INFORMATION

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application claims the benefit of U.S. Provisional Application Serial No. 60/425,800, filed on Nov. 13, 2002, which is incorporated by reference herein in its entirety.

TECHNICAL FIELD

[0002] The present invention is directed to a system and method for real-time feature sensitivity analysis based on contextual information, and more particularly, to a system and method for real-time feature selection of measurements to be taken during a medical testing procedure based in part on contextual information in order to accurately diagnose a medical condition.

BACKGROUND OF THE INVENTION

[0003] Active object recognition or active vision (or as called in robotics, active sensing/localization/navigation) deals with a specific object or scene, searching for the next action, operator, or viewpoint, to optimize some objective function. Although these topics are intimately related to feature selection in machine learning, two key issues raised in the latter field have not been consciously considered by the former, namely, the necessity of an induction algorithm, and the possibility of complex feature interactions (e.g., in-class dependencies).

[0004] As a result, an active vision system based on ad hoc heuristics may fail to fully reveal potential feature contributions. For example, most existing systems implicitly assume feature independence (which translates to viewpoint independence for object recognition using an active camera). However, in many cases two or more views are required to discriminate one class of objects from others.

[0005] Much research in active vision and robotics has used similar heuristics for active selection of best features. Some techniques include using reduction of entropy to guide the selection of viewpoints, optimal sensor parameter selection for iterative state estimation in static systems by maximizing mutual information, and information gain-based selection of "imaging operators", taking into account also operation costs. However, none of the above techniques formally addresses the role of an induction algorithm for feature analysis as well as the issue of feature interaction.

[0006] Feature selection for classification has recently also been very active. Feature selection is essentially a search for the most sensitive feature subset for the purpose of improved classification accuracy and a significantly reduced feature set. However, existing feature selection paradigm does not deal with a specific test input or case-in-question along with a context. Furthermore, many known feature selection techniques do not use an induction algorithm for feature analysis or address the issue of feature interaction.

[0007] One traditional class of feature selection techniques uses a filter model that treats feature selection solely as a preprocessing step for later induction algorithm design. Recent feature selection techniques use a wrapper model

that performs cross validation using an induction algorithm on the training set. There have also been efforts to link these two models. However, these algorithms are not directly applicable for conditional feature sensitivity analysis.

[0008] For example, the wrapper approach relies on cross validation but oftentimes sufficient training samples do not exist to cross-validate in the neighborhood defined by the context especially when more than a few features have been measured; on the other hand, most variants of the filter approach do not address the context issue, and often ignore the induction algorithm altogether. Consulting an induction algorithm is necessary during the course of feature evaluation, because the most sensitive feature is not necessarily the one that leads to the most variability in labels (which may lead to minimal empirical error on the training data but large error on test data); the best feature shall lead to the most systematic and predictable variability in labels. The present invention combines the essence of both the wrapper model and the filter model and puts an explicit emphasis on the modeling of contextual features.

[0009] For example during an echocardiograph exam, the number of possible measurements is in the hundreds, but a typical echocardiograph exam in the United States only contains about ten different measurements on average. The appropriate selection of additional measurements requires extensive training and field experience and is therefore subjective and error-prone. It would be very helpful if a machine could provide context-sensitive real-time guidance as to what additional feature(s) should be measured for the current case. A feature sensitivity analysis module also provides a way to reduce medical costs by identifying a minimal number of measurements that need to be performed to provide a proper medical diagnosis.

SUMMARY OF THE INVENTION

[0010] The present invention is directed to a method for assigning feature sensitivity values to a set of potential measurements to be taken during a medical procedure of a patient in order to provide a medical diagnosis. Data is received from a sensor that represents a particular medical measurement. The received data and context data are analyzed with respect to one or more sets of training models. Feature sensitivity values are derived for the particular medical measurement and other potential measurements to be taken based the analysis, and the feature sensitivity values are outputted.

[0011] The present invention is also directed to a system for assigning feature sensitivity values to a set of potential measurements to be taken during a medical procedure of a patient in order to provide a medical diagnosis. A medical sensor provides data pertaining to medical measurements taken of a patient. A processor connected to the medical sensor receives the data from the medical sensor and context data relating to the patient. The processor analyzes the sensor data and context data and determines feature sensitivity values for a set of potential measurements to be taken by the sensor. A display device displays the sensor data and feature sensitivity values.

BRIEF DESCRIPTION OF THE DRAWINGS

[0012] Preferred embodiments of the present invention will be described below in more detail, wherein like reference numerals indicate like elements, with reference to the accompanying drawings:

[0013] FIG. 1 is a block diagram of a system for implementing a method for conditional feature sensitivity analysis in accordance with the present invention;

[0014] FIG. 2 is a functional block diagram illustrating the overall process for conditional feature sensitivity analysis;

[0015] FIG. 3 is a graph depicting the training models used to determine if a patient has DCM; and

[0016] FIG. 4 is an exemplary display screen showing image and feature sensitivity data in accordance with the present invention.

DETAILED DESCRIPTION

[0017] The present invention is directed to a method for assigning feature sensitivity values to a set of potential measurements to be taken during a medical procedure in order to select those measurements having the highest feature sensitivity thereby achieving a proper medical diagnosis with a minimal number of measurements being taken. Feature selection is essentially a search for the most sensitive feature subset for the purpose of improved classification accuracy and a significantly reduced feature set. The present invention addresses feature selection that further includes a specific test input or case-in-question along with a context. For any given medical diagnosis, all features for a given case are presumed to be uncertain but to different degrees—a measured feature (e.g., the visible patterns from the current camera angle) contains lower uncertainty, while a missing feature (e.g., the unseen or self-occluded parts of an object) has maximal uncertainty. Then, the question is: “given an induction algorithm, a labeling on a training set, and some contextual information for the case-in-question, what is the relative sensitivity for all features?” In other words, if more measurements are taken, either on unmeasured features, or to increase the accuracy of measured features, what additional measurements should be taken? The present invention is directed to how to evaluate the importance or sensitivity of the features or measurements, as well as how to deal with uncertainty in the contextual features, which will be described in more detail hereinafter.

[0018] FIG. 1 illustrates an exemplary architecture of an echocardiograph system that uses a method for identifying conditional feature sensitivity in accordance with the present invention. A medical sensor 102, such as an ultrasound transducer is used to perform an examination on a patient. The sensor 102 is used to obtain medical measurements consistent with a particular medical examination. For example, a patient experiencing heart problems may have an echocardiogram performed to help diagnose the particular heart ailment. In such an instance, the medical sensor 102 may be an ultrasound transducer. An ultrasound system provides two- or three-dimensional images of the heart from various perspectives.

[0019] The present invention will be described in detail in the context of performing an echocardiogram examination. However, it is to be understood by those skilled in the art that the present invention can be used in conjunction with other medical examinations such as, but not limited to, breast cancer detection examinations, prenatal ultrasound examinations or another type of medical examination in which a diagnosis is being determined.

[0020] The information obtained by the sensor 102 is communicated to a processor 104 which may be a workstation or personal computer. The processor 104 converts the sensor data into an image that is communicated to display 108. The display 108 may also communicate other graphical information or tables of information relating to the image. In accordance with the present invention, the processor 104 is also provided with context data which is used in conjunction with the sensor data to determine what, if any, further measurements need to be taken by the sensor 102 in order to provide a proper medical diagnosis.

[0021] As will be described in greater detail hereinafter, context data can originate from a number of sources of information including, but not limited to, vital statistics, patient symptoms and available test data. Vital statistics can include such information as a patient's height, weight, age, blood pressure measurement, or any other personal medical data that is pertinent to the particular medical examination being performed. Patient symptoms can include, for example, indications of pain, such as chest pain, shortness of breath, detection of a foreign mass in an area of tissue, labored breathing, poor circulation, unexplained weight loss or gain or any other symptom that would be material to a particular medical examination. Available testing data can come from a baseline scan, preliminary blood work or any other test that would be material to a particular medical examination, and the data from sensor 102 during the current examination. Testing data can also include test results or medical measurements taken from a patient's prior medical examinations or procedures. Furthermore, context data may also include data pertaining to the ultrasound or other medical diagnosis system. For example, context data may include the type of exam being taken, various system settings and view settings.

[0022] Upon receipt of the data from the medical sensor 102, the processor 104 retrieves training models from a database 106 in order to perform feature sensitivity analysis as will be described in greater detail hereinafter. In addition to data from the medical sensor, the processor 104 may also receive other data inputs. For example, the processor may receive data from the technician or physician performing the medical procedure. The processor 104 may also receive other measurements or system data to be considered during the feature sensitivity analysis. The training models contain a collection of data measurements relating to one or more particular medical conditions. For example, the database may contain a plurality of distribution data points relating to the likelihood of a patient having Dilated Cardiomyopathy (DCM) or a normal heart condition (nonDCM). Such data may include measurements pertaining to the size of the heart, the thickness of the heart walls and the level of blood flow to and from the heart.

[0023] FIG. 3 illustrates a graph that represents a distribution of training models indicating the probability of DCM. The vertical axis 302 represents Left Ventricle Dimensions (LVD) in millimeters (mm) and the horizontal axis 304 represents the patient's height in meters (m). A training model distribution 306 indicates those measurements that signify a high probability of DCM and a second training model distribution 308 indicates those measurements that signify a high probability of nonDCM.

[0024] Consistent with FIG. 3, for a patient with a height of 1.5 m to 1.7 m and an LVD of 5056 mm, the patient

should definitely be re-measured more precisely for a sure diagnosis. This is because the patient has a somewhat high probability of having DCM. However, the same LVD value range is adequate and should not be a sensitive concern at all for a person taller than 2 m. Also, the LVD measurement will not be a sensitive measurement for a 1.1 m child because then it is almost certain a DCM case.

[0025] Other information may be included in the database 106 as well including image data that represents a particular medical condition (e.g., images of hearts that have various types of DCM) as well as other groupings of data that may be useful in achieving a correct medical diagnosis.

[0026] FIG. 2 illustrates a flow diagram that illustrates the real-time guidance of the measurement process during a particular medical examination. The conditional feature sensitivity analysis module 210 takes as inputs all the available information about the case in question 202 (both missing and uncertain features) together with the class models 204 (e.g., likelihood maps) provided by a given induction algorithm. The output is a list of sensitive features 208 that provides a list of additional measurements 212 that should be measured next, to maximally reduce uncertainty in classification.

[0027] Referring back to FIG. 1, once a particular measurement has been taken and the feature sensitivity analysis performed, the output is provided on display 108. An exemplary display screen is shown in FIG. 4. The screen includes an ultrasound image 402 created based on data received from the medical sensor 102 which displays views of the heart from which Left Ventricle End Diastolic (LVED) dimension measurements can be made. LVED provides an indication of the size of the heart. Also included in the screen is a graphic 403 that provides the probability of DCM vs. nonDCM as well as an indication of measurements 408 that have been taken or can be taken and the corresponding sensitivity value 410 for each measurement.

[0028] In accordance with the present invention, the sensitivity value provides an indication of the importance of a particular measurement for determining a correct medical diagnosis. For example, as illustrated in FIG. 4, the LVED measurement is 7.6 which indicates a high probability of DCM. The sensitivity values indicate that other measurements are recommended being taken that include the Left Ventricle End Systolic (LVES) dimension, as well as the wall thickness (septal wall, posterior wall) and the Ejection Fraction (EF).

[0029] A technician or doctor who is viewing this screen can then determine, depending upon the known facts regarding the patient, whether these additional measurements need to be taken. If any of these subsequent measurements are made, the graphic 403 is updated both with the DCM/nonDCM probability as well as re-calculate the feature sensitivities for the measurements. By performing these feature sensitivity analyses, the technician or doctor is able to achieve a correct medical diagnosis by performing both the "best" measurements and the fewest number of measurements.

[0030] An exemplary system for real-time diagnosis support in echocardiography with optical flow-based contour tracking for calculating heart volume, ejection fraction, and ischemia regions, etc. will now be described in conjunction

with FIG. 4. The exemplary system uses a database with about 2000 echocardiography videos, labeled by medical expert into different types and stages of cardiomyopathies. As discussed above, FIG. 4 shows the system at work for diagnosing DCM or nonDCM: after LVED (left ventricle end diastolic dimension) is measured to 7.6 cm (95% th percentile of healthy heart is <5.8 cm), the system outputs a probability of DCM at 86.2%, but recommended further measurements on LVES (LV end systolic dimension), wall thickness, EF (ejection fraction), etc., in that order.

[0031] If the doctor or technician decide to do a further measurement (e.g., LVES), the feature sensitivity analysis is recalculated and new sensitivity values are determined as well as new probability values of DCM vs. nonDCM based on the additional measurement. For each additional measurement that may be performed, the outputs are again recalculated. Based on the resulting probability results, the doctor or technician can determine if further measurements are required or if a proper medical diagnosis has been achieved.

[0032] For DCM vs. nonDCM, LVED is the most sensitive feature given no context. Subsequent feature sensitive ordering is case or context-dependent, assuming nonlinear class boundaries. In an embodiment of the present invention, once the doctor or technician has completed those measurements which he or she believes are necessary to achieve a proper medical diagnosis, the data may be added to the data base to further update the training models.

[0033] The present invention is directed to how to deal with uncertainty with respect to the contextual features. Consistent with the above, from an algorithm viewpoint, a feature with uncertainty models both a missing feature and a measured feature. In other words, all features will be treated as uncertain features, with different degrees of uncertainty. As such, a case S has a measurement vector Z with M features, each of which has a prior distribution $p_0(z)$ over the whole population, a true value z for the current case, and a posterior distribution $p(z)$ after a measurement operation. The ultimate goal is probabilistic classification, i.e., given a case S_i , to obtain probabilities of its membership in all classes: $\{P(C_i=c_1), P(C_i=c_2), \dots, P(C_i=c_K)\}$, where $c_k, k=1, 2, \dots, K$, are the class labels.

[0034] The symbol y represents the feature under current study, $\{y\} \subseteq Z$. Without loss of generality we will assume y is 1-D for simplicity unless otherwise noted. The remaining features are represented by a vector $X, X=Z \setminus \{y\}$. The current features are referred to as y , and the contextual features as X . Context—i.e., what we know about the current case—is denoted by χ and ζ , representing the distributions of X and y , respectively. The expression " $y \in \zeta$ " means " y has a distribution ζ " or " y is restricted to ζ ." A particular sample drawn from ζ is denoted by y_i ; and from χ , x_j . Note that when y is in 1-D, x_j is a $(N-1)$ -dimensional vector. The lowercase x (without a subscript) is used to represent a subset of Z .

[0035] A prerequisite for what is described hereinafter is a way to deal with missing or uncertain features for both training and testing. A principled way of treating a missing feature is to sample (for training) or integrate (for testing) over its value range (or, its conditional distribution), an idea

that parallels the EM and Bayesian treatments of missing data. A traditional formulation is as follows:

$$P(C = c_k | X \in \chi, y \in \zeta) = \frac{\int_{\chi} \int_{\zeta} P(X, y) P(C = c_k | X, y) dX dy}{P(X \in \chi, y \in \zeta)} \quad (1)$$

[0036] $P(C|X, y)$ is obtained from the classifier. An estimation of the joint distribution of the features, $P(x, y)$ is also required. It is assumed that a likelihood function is available for every class in the original feature space $P(X, y|C)$ (these can be approximated efficiently), joint distribution is implied and the following formula is used:

$$P(C = c_k | X \in \chi, y \in \zeta) = \frac{P(C = c_k) \int_{\chi} \int_{\zeta} P(X, y | C = c_k) dX dy}{\sum_k P(C = c_k) \int_{\chi} \int_{\zeta} P(X, y | C = c_k) dX dy} \quad (2)$$

[0037] Here $P(C=c_k)$ is the prior probability of the k th class.

[0038] The concept of conditional feature sensitivity is defined as follows: Given the context $\{\epsilon\chi^*, y\in\zeta\}$ for the case in question, further measurement of which feature(s) can maximally reduce uncertainty in classification? Although other criteria exist, the best gauge for uncertainty is entropy. The reduction of entropy is the mutual information or information gain. Indeed, if one only considers the class label C and the current feature y , maximizing information gain corresponds to minimizing conditional entropy and this in turn minimizes a bound on classification error according to Fano's inequality.

[0039] With contextual information coming into play, mutual information between C and y alone cannot in general reveal the potential information gain; and one shall appeal only to the information gain criterion for the right answer. Since we have uncertainty in the contextual features, it is not a trivial task to formulate an information gain strategy directly. Based on different treatments of contextual uncertainties, the present invention incorporates three models: a mean imputation model, an integral model, and a sample-expectation model; or M-model, I-model, and S-model, respectively.

[0040] The M-model provides the most straightforward treatment. It assigns the mean values to the contextual features while working on the current feature. The information gain of y , IG_{y^*} , is defined as:

$$IG_{y^*}(C, X = \bar{x}, y \in \zeta) = \quad (3)$$

$$H(C | X = \bar{x}, y \in \zeta) - \int_{\zeta} P(y | X = \bar{x}) H(C | X = \bar{x}, y) dy$$

where

$$H(C | X = \bar{x}, y \in \zeta) = - \sum_k P(C = c_k | X = \bar{x}, y \in \zeta) \log P(C = c_k | X = \bar{x}, y \in \zeta) \quad (4)$$

-continued

and

(5)

$$P(C = c_k | X = \bar{x}, y \in \zeta) = \frac{P(C = c_k) \int_{\zeta} P(X = \bar{x}, y | C = c_k) dy}{\sum_k P(C = c_k) \int_{\zeta} P(X = \bar{x}, y | C = c_k) dy}$$

[0041] The M-model is the simplest and it is very efficient. It can be practically very useful in the following scenario: when all measurements are done (with a mean value and a small variance), the doctor wants to know which feature is more sensitive than others, i.e., whether perturbations (due to, say, human or machine error) in one feature will cause more fluctuation in the final diagnosis than those of other features. However, M-model did not utilize all the statistical information available.

[0042] The Integral Model (I-Model) considers the full range of the contextual features:

$$IG_{y^*}(C, X \in \chi, y \in \zeta) = \quad (6)$$

$$H(C | X \in \chi, y \in \zeta) - \int_{\zeta} P(y | X \in \chi) H(C | X \in \chi, y) dy$$

where

(7)

$$H(C | X \in \chi, y \in \zeta) = - \sum_k P(C = c_k | X \in \chi, y \in \zeta) \log P(C = c_k | X \in \chi, y \in \zeta)$$

[0043] Here, $P(C|X\in\chi, y\in\zeta)$ is evaluated according to the likelihood sampling strategy discussed above. $H(C|X\in\chi, y)$ is defined in a similar fashion. The conditional probability can be expressed in terms of the likelihood as follows:

$$P(y | X \in \chi) = \frac{P(y, X \in \chi)}{P(X \in \chi)} \quad (8)$$

$$= \frac{\sum_k P(C = c_k) P(y, X \in \chi | C = c_k)}{\int_{\zeta} \sum_k P(C = c_k) P(y, X \in \chi | C = c_k) dy}$$

$$= \frac{\sum_k P(C = c_k) \int_{\chi} P(y, X | C = c_k) dX}{\int_{\zeta} \sum_k P(C = c_k) \int_{\chi} P(y, X | C = c_k) dX dy}$$

[0044] IG_{y^*} is now expressed in terms of $P(y, X|C)$, the prior distributions obtained through the generative classifier, and $P(C)$, the prior probability for each class. All the integrals can be estimated either analytically if closed-form models are available, or by sampling within the uncertain range. In terms of sampling, randomized sampling is preferred to a deterministic sampling for the serendipity that could be brought forth in the randomness; in other words, random sampling has the capability of capturing unexpected irregularity in distributions.

[0045] An example of an efficient sampling-based integral algorithm, CFS-I is shown below:

For every feature of interest y :
 $P_x = 0$; $\text{Sum_H}_{yt} = 0$; $L_k = 0$, $k = 1, \dots, K$;
 For every sample of y , y_i :
 $L_{yt,k} = 0$, $k = 1, \dots, K$;
 For every sample of X , X_i :
 Accumulate $L_{y_i,k} += P(X_i, y_i | C = c_k)$;
 Calculate Bayesian posterior, $P_{yt,k}$, from $L_{yt,k}$;
 Calculate Entropy H_{yt} over $P_{yt,k}$;

$$\text{Calculate } p_{yt} = \sum_k L_{yt,k} P(C = c_k);$$

Accumulate $\text{Sum_H}_{yt} += P_{yt} H_{yt}$;
 Accumulate (marginalize): $p_x += P_{yt}$;
 Accumulate $L_k += L_{yt,k}$;
 Calculate Bayesian posterior, P_k , from L_k ;
 Calculate Entropy H_y over P_k ;
 Calculate information gain: $IG_y = H_y - \text{Sum_H}_{yt} / P_x$.

[0046] For the Sample-Expectation Model (S-model), the question to answer for the current feature is: "assuming that we knew the context, on average how much information could we gain from measuring the current feature?" The formula is:

$$EIG_{y|x}(C, X \in \mathcal{X}, y \in \mathcal{Z}) = E_X[IG_y(C, X, y \in \mathcal{Z})] \quad (9)$$

$$= \int_{\mathcal{X}} P(X | y \in \mathcal{Z}) IG_y(C, X, y \in \mathcal{Z}) dX$$

$$= \int_{\mathcal{X}} P(X | y \in \mathcal{Z}) (H(C | X, y \in \mathcal{Z}) -$$

$$\int_{\mathcal{Z}} P(y | X) H(C | X, y) dy) dX$$

[0047] An exemplary sampling-based implementation, CFS-S, is shown below:

For every feature of interest y :
 $P_y = 0$; $\text{Accu_IG}_y = 0$;
 For every sample of X , X_i :
 $P_x = 0$; $\text{Sum_H}_{yt} = 0$; $L_k = 0$, $k = 1, \dots, K$;
 For every sample of y , y_i :
 Calculate $L_{y_i,k} = P(X_i, y_i | C = c_k)$;
 Calculate Bayesian posterior, $P_{yt,k}$, from $L_{yt,k}$;
 Calculate Entropy H_{yt} over $P_{yt,k}$;

$$\text{Calculate } p_{yt} = \sum_k L_{yt,k} P(C = c_k);$$

Accumulate (i.e., marginalize): $P_x += P_{yt}$;
 Accumulate $\text{Sum_H}_{yt} += P_{yt} H_{yt}$;
 Accumulate $L_k += L_{yt,k}$;

$$\text{Calculate } p_{xj} = \sum_k L_k P(C = c_k);$$

Accumulate (i.e., marginalize): $P_y += P_{xj}$;
 Calculate Bayesian posterior, P_k , from L_k ;
 Calculate Entropy H_y over P_k ;
 Accumulate the information gain:

-continued

$$\text{WeightedSum_IG}_y += P_{xj}(H_y - \text{Sum_H}_{yt} / P_x);$$

$$IG_y = \text{WeightedSum_IG}_y / P_y;$$

[0048] The sample-expectation model can also be defined more generally but in a similar fashion in the form of $EIG_{y|x}$, where x is only a subset of X .

[0049] The present invention devises a testing scheme that combines outputs from multiple models to expose complicated feature dependencies. By examining the outputs of both the I-model and the S-model different feature sensitivities or relevance scenarios are detected. The following table shows an example for two features, x and y :

TABLE 1

| An example for joint analysis of two features | | | | | | |
|---|--------|-------------|-------------|-----------|-------------------|--|
| IG_x | IG_y | $EIG_{x y}$ | $EIG_{y x}$ | IG_{xy} | Relevant features | Notes |
| 0 | 0 | 0 | 0 | 0 | — | x, y : weak or no |
| 0 | 0 | + | + | + | x, y | Both strong, e.g., $C = x \oplus y$ |
| 0 | + | 0 | + | + | y | y : Strong; x : weak or no |
| + | 0 | + | 0 | + | x | x : Strong; y : weak or no |
| + | + | 0 | 0 | + | x, y | Both weak, e.g., $x = f(y)$ |
| + | + | + | + | + | x, y | Both strong |

[0050] It is worth noting that for the first five columns in Table 1, only three columns need to be calculated. Joint analysis of two features can only expose dependency involving less than three features. In case there are dependencies between more than two features, joint analysis of more than two features must be considered.

[0051] For example, if $C = x \oplus y \oplus z$, and we have another three redundant features, $x' = x$, $y' = y$, and $z' = z$, analyzing two features at a time and we will arrive at the first row of Table 1. Only joint three-feature analysis such as $IG_{x,y,z}$ can reveal the contributions of x or x' , y or y' , and z or z' .

[0052] An easy implementation for $IG_{x,y,z}$ or $EIG_{x,y,z}$ is through nested calls to the single-feature IG function. For example,

$$IG_{x,y,z} = IG_x + EIG_{y,z|x} = IG_x + \sum_i P(x_i) IG_{y,z|x=x_i} \quad (11)$$

$$= IG_x + \sum_i P(x_i) (IG_{y|x=x_i} + EIG_{z|x=x_i,y})$$

$$= IG_x + \sum_i P(x_i) \left(IG_{y|x=x_i} + \sum_j P(y_j) IG_{z|x=x_i,y=y_j} \right)$$

$$= IG_x + \sum_i P(x_i) \left(IG_{y|x=x_i} + \sum_j P(y_j) IG_{z|x=x_i,y=y_j} \right) \quad (12)$$

[0053] The present invention uses an induction algorithm that can learn probabilistic models from the training data. We use kernel discriminant analysis combined with genera-

tive modeling for this purpose. The kernel discriminant has been shown to have comparable performance as SVM. In addition, it can provide a low dimensional, non-linearly transformed subspace, in which simple probability models can be built. We use RBF kernel with an empirically determined spread.

[0054] It is often necessary to expect missing feature values in the training data during a medical diagnosis. Data imputation is applied through sampling to fill in missing or uncertain values for feature(s) y , based on $p(y|x)$ where x represents the remaining features with known values. The term $p(y|x)$ is estimated using the training set. Robust estimates are used to reduce the influence of outliers.

[0055] Having described embodiments for method for determining feature sensitivity during a medical examination, it is noted that modifications and variations can be made by persons skilled in the art in light of the above teachings. It is therefore to be understood that changes may be made in the particular embodiments of the invention disclosed which are within the scope and spirit of the invention as defined by the appended claims. Having thus described the invention with the details and particularity required by the patent laws, what is claimed and desired protected by Letters Patent is set forth in the appended claims.

We claim:

1. A method for assigning feature sensitivity values to a set of measurements to be taken during a medical procedure of a patient in order to provide a medical diagnosis, the method comprising:

receiving data from a sensor representing a particular medical measurement;

analyzing the received data and context data with respect to one or more sets of training models;

deriving feature sensitivity values for the particular medical measurement and other measurements to be taken based on the analysis; and

outputting the feature sensitivity values.

2. The method of claim 1 wherein the medical procedure is an echocardiogram examination.

3. The method of claim 1 wherein the context data comprises vital statistics relating to the patient.

4. The method of claim 3 wherein the vital statistics include the patient's age.

5. The method of claim 3 wherein the vital statistics include the patient's height.

6. The method of claim 3 wherein the vital statistics include the patient's weight.

7. The method of claim 3 wherein the vital statistics include the patient's blood pressure measurements.

8. The method of claim 1 wherein the context data comprises the patient's symptoms.

9. The method of claim 8 wherein the symptoms include indications of pain.

10. The method of claim 8 wherein the symptoms include shortness of breath.

11. The method of claim 1 wherein context data comprises baseline test data for the patient.

12. The method of claim 1 wherein the medical sensor is an ultrasound transducer.

13. The method of claim 12 wherein the received data is image data.

14. The method of claim 1 wherein the analyzing step further comprises the step of:

analyzing the received data, context data and training models using an integral model.

15. The method of claim 1 wherein the analyzing step further comprises the step of:

analyzing the received data, context data and training models using a sample expectation model.

16. The method of claim 1 wherein the analyzing step further comprises the step of:

analyzing the received data, context data and training models using both an integral model and a sampling expectation model.

17. The method of claim 1 wherein the step of outputting the feature sensitivity values further comprises the step of:

providing an indication of a probability for one or more medical diagnosis; and

providing a listing of potential measurements wherein a feature sensitivity value is assigned to each potential measurement.

18. The method of claim 17 further comprising the steps of:

receiving input representing a selection of one or more potential measurement for which measurements are to be taken;

receiving data from the medical sensor corresponding to the selected one or more potential measurements;

analyzing the received data for the one or more potential measurements, data corresponding to any prior measurements and context data with the training models;

deriving feature sensitivity values for the set of potential measurements; and

outputting the feature sensitivity values.

19. The method of claim 1 wherein a user uses the outputted feature sensitivity values to assist in making a medical diagnosis.

20. The method of claim 1 wherein the outputted feature sensitivity values are provided in real time.

21. A system for assigning feature sensitivity values to a set of potential measurements to be taken during a medical procedure of a patient in order to provide a medical diagnosis, the system comprising:

a medical sensor that provides data pertaining to medical measurements taken of a patient;

a processor connected to the medical sensor, the processor receiving the data from the medical sensor and context data relating to the patient, the processor analyzing the sensor data and context data and determining feature sensitivity values for a set of potential measurements to be taken by the sensor; and

a display device for displaying the sensor data and feature sensitivity values.

22. The system of claim 21 further comprising a database associated with the processor, the database including a set of training models that are compared to the context data and

sensor data in order to obtain feature sensitivity values for the set of potential measurements.

23. The system of claim 21 wherein the medical sensor is an ultrasound transducer.

24. The system of claim 21 wherein the medical procedure is an echocardiogram examination.

25. The system of claim 21 wherein the context data comprises vital statistics relating to the patient.

26. The system of claim 25 wherein the vital statistics include the patient's age.

27. The system of claim 25 wherein the vital statistics include the patient's height.

28. The system of claim 25 wherein the vital statistics include the patient's weight.

29. The system of claim 25 wherein the vital statistics include the patient's blood pressure measurements.

30. The system of claim 21 wherein the context data comprises the patient's symptoms.

31. The system of claim 30 wherein the symptoms include indications of pain.

32. The system of claim 30 wherein the symptoms include shortness of breath.

33. The system of claim 21 wherein context data comprises baseline test data for the patient.

34. The system of claim 21 wherein a user uses the determined feature sensitivity values to assist in making a medical diagnosis.

35. The system of claim 21 wherein the determined feature sensitivity values are provided in real time.

36. The system of claim 21 wherein context data comprises medical measurements from a patient's prior medical examinations.

* * * * *

| | | | |
|----------------|--|---------|------------|
| 专利名称(译) | 用于基于上下文信息的实时特征灵敏度分析的系统和方法 | | |
| 公开(公告)号 | US20040133083A1 | 公开(公告)日 | 2004-07-08 |
| 申请号 | US10/702984 | 申请日 | 2003-11-06 |
| [标]申请(专利权)人(译) | 西门子公司 | | |
| 申请(专利权)人(译) | 西门子公司研究INC. | | |
| 当前申请(专利权)人(译) | 西门子公司研究INC. | | |
| [标]发明人 | COMANICIU DORIN KRISHNAN ARUN ZHOU XIANG SEAN DUGGIRALA BHAVANI PAINE DIANE | | |
| 发明人 | COMANICIU, DORIN KRISHNAN, ARUN ZHOU, XIANG SEAN DUGGIRALA, BHAVANI PAINE, DIANE | | |
| IPC分类号 | A61B5/00 A61B5/107 A61B8/02 A61B8/06 A61B8/08 G06F19/00 | | |
| CPC分类号 | A61B5/1075 A61B8/02 A61B8/065 A61B8/0858 A61B8/0883 G06K2209/051 G06F19/3406 G06K9/623 G06K9/6231 G06K9/72 A61B8/463 G16H40/63 | | |
| 优先权 | 60/425800 2002-11-13 US 60/425800 2002-11-13 US | | |
| 其他公开文献 | US7087018 | | |
| 外部链接 | Espacenet USPTO | | |

摘要(译)

公开了一种用于将特征灵敏度值分配给在患者的医疗过程期间要采取的一组潜在测量值以提供医学诊断的系统和方法。从表示特定医学测量的传感器接收数据。关于一组或多组训练模型分析所接收的数据和上下文数据。针对特定医学测量和基于分析要采取的其他潜在测量导出特征灵敏度值，并输出特征灵敏度值。

