



US009687671B2

(12) **United States Patent**  
**Weckwerth et al.**

(10) **Patent No.:** **US 9,687,671 B2**  
(45) **Date of Patent:** **Jun. 27, 2017**

- (54) **OPTICAL SENSOR AND METHOD FOR IDENTIFYING THE PRESENCE OF SKIN AND THE PIGMENTATION OF SKIN**
- (75) Inventors: **Mark V. Weckwerth**, Weckwerth, CA (US); **Tobin C. Island**, Oakland, CA (US); **Robert E. Grove**, Pleasanton, CA (US)
- (73) Assignee: **CHANNEL INVESTMENTS, LLC**, Tampa, FL (US)
- (\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 903 days.

4,449,528 A	5/1984	Auth et al.	606/31
4,551,628 A	11/1985	Grossman	250/503.1
4,573,466 A	3/1986	Simada et al.	606/11
4,592,353 A	6/1986	Daikuzono	606/16
4,608,978 A	9/1986	Rohr	606/9
4,617,926 A	10/1986	Sutton	606/9
4,690,141 A	9/1987	Castel et al.	607/90
4,733,660 A	3/1988	Itzkan	606/9
4,829,262 A	5/1989	Furumoto	359/346
4,846,184 A	7/1989	Comment et al.	600/306
4,849,211 A	7/1989	Schrauzer	424/45
4,860,744 A	8/1989	Johnson et al.	128/303.1
4,905,690 A	3/1990	Ohshiro et al.	607/89
4,930,504 A	6/1990	Diamantopoulos et al.	607/88
5,057,104 A	10/1991	Chess	606/9
5,059,013 A	10/1991	Jain	359/503
5,059,192 A	10/1991	Zaias	606/9
5,071,417 A	12/1991	Sinofsky	606/8
5,075,971 A	12/1991	Mccambridge	30/133

(21) Appl. No.: **12/430,730**

(Continued)

(22) Filed: **Apr. 27, 2009**

FOREIGN PATENT DOCUMENTS

(65) **Prior Publication Data**  
US 2009/0270848 A1 Oct. 29, 2009

CN	2442726 Y	8/2001	A63H 33/00
DE	19629978 A1	1/1998	F41A 33/02
DE	10044662 A1	3/2002	A61K 31/60
DE	10360503 A1	7/2005	A61K 8/06
DK	WO2004/010884 A1 *	2/2004	606/9
EP	0761257 A2	3/1997	A61B 18/20
EP	0933096 A2	8/1999	A61B 17/00
EP	1116476 A2	7/2001	A61B 18/20
EP	1168535 A1	1/2002	H01S 5/022
EP	1358872 A1	11/2003	A61K 31/192
FR	2665366 A1	2/1992	A61N 1/32
FR	2932679 A1	12/2009	A61K 8/36

(Continued)

**Related U.S. Application Data**

(60) Provisional application No. 61/048,154, filed on Apr. 25, 2008.

(51) **Int. Cl.**  
**A61N 5/06** (2006.01)  
**A61B 5/00** (2006.01)  
**A61B 17/00** (2006.01)  
**A61B 90/00** (2016.01)

OTHER PUBLICATIONS

Brunsting, L.A. et al., "The Color of the Skin as Analyzed by Spectrophotometric Methods: II. The Role of Pigmentation," The Journal of Clinical Investigation, vol. 7, 18 pages, Apr. 29, 1929.

(Continued)

(52) **U.S. Cl.**  
CPC ..... **A61N 5/0616** (2013.01); **A61B 5/0059** (2013.01); **A61B 5/441** (2013.01); **A61B 5/6843** (2013.01); **A61B 2017/00057** (2013.01); **A61B 2090/065** (2016.02); **A61B 2562/0238** (2013.01); **A61N 2005/0652** (2013.01); **A61N 2005/0659** (2013.01); **A61N 2005/0662** (2013.01)

Primary Examiner — Audrea Buckley

(58) **Field of Classification Search**  
CPC ..... A61B 18/203; A61B 2018/00452; A61B 2018/00476; A61B 2017/00172; A61B 2017/00057; A61B 2018/00005; A61B 2018/2261; A61B 2090/065; A61B 2017/00061; A61B 2018/00029; A61B 18/20; A61B 2017/00066  
See application file for complete search history.

(74) *Attorney, Agent, or Firm* — Slayden Grubert Beard PLLC

(57) **ABSTRACT**

Apparatus and methods are provided to control a device, such as a light emitting dermatologic or cosmetic treatment device, and ensure that the device is in contact with skin while also determining the pigmentation level of skin. One or more light sources contact the skin and one or more detectors measure spectral remission from the skin. The obtained remission measurements are compared with known skin spectral remission values, and calibration allows measurements of absolute remission to be converted to fractional remission values. Skin pigmentation levels are compared to known base-line levels to determine and control appropriate treatment parameters. A temperature sensor allows correction for temperature variations. The apparatus may or may not be incorporated into the treatment device.

(56) **References Cited**  
U.S. PATENT DOCUMENTS

3,307,533 A	3/1967	Meredith et al.	601/150
3,538,919 A	11/1970	Meyer	606/36
3,622,743 A	11/1971	Muncheryan	219/121.63
3,693,623 A	9/1972	Harte et al.	606/9
3,821,510 A	6/1974	Muncheryan	219/121.79
3,834,391 A	9/1974	Block	128/303.1
4,140,130 A	2/1979	Storm, III	607/154
4,232,678 A	11/1980	Skovajsa	607/89
4,240,738 A	12/1980	Praamsma et al.	355/1
4,354,092 A	10/1982	Manabe et al.	219/225
4,388,924 A	6/1983	Weissman et al.	606/9
4,423,736 A	1/1984	Dewitt et al.	600/306

**23 Claims, 4 Drawing Sheets**

(56)

## References Cited

## U.S. PATENT DOCUMENTS

5,107,832 A	4/1992	Guibert et al. ....	607/96	6,142,650 A	11/2000	Brown et al. ....	365/259
5,109,465 A	4/1992	Klopotek .....	385/133	6,144,536 A	11/2000	Zimmerman et al. ....	361/31
5,226,907 A	7/1993	Tankovich .....	606/133	6,160,831 A	12/2000	Kleinschmidt et al. ....	372/57
5,233,337 A	8/1993	Takahashi .....	345/82	6,168,831 B1	1/2001	Khan et al. ....	427/240
5,259,380 A	11/1993	Mendes et al. ....	607/115	6,171,301 B1	1/2001	Nelson et al. ....	606/9
5,282,797 A	2/1994	Chess .....	606/9	6,183,500 B1	2/2001	Kohler .....	607/88
5,295,052 A	3/1994	Chin et al. ....	362/580	6,183,773 B1	2/2001	Anderson .....	424/450
5,344,418 A	9/1994	Ghaffari .....	606/9	6,188,495 B1	2/2001	Inoue et al. ....	398/139
5,360,426 A	11/1994	Muller et al. ....	606/13	6,197,020 B1	3/2001	O'donnell, Jr. ....	606/9
5,401,270 A	3/1995	Muller et al. ....	606/13	6,208,749 B1	3/2001	Gutkowicz-Krusin et al. ....	382/128
5,405,368 A	4/1995	Eckhouse .....	607/88	6,214,034 B1	4/2001	Azar .....	607/89
5,425,728 A	6/1995	Tankovich .....	606/9	6,228,074 B1	5/2001	Almeida .....	606/9
5,431,647 A	7/1995	Purcell, Jr. et al. ....	606/16	6,251,127 B1	6/2001	Biel .....	607/88
5,464,434 A	11/1995	Alt .....	607/6	6,264,649 B1	7/2001	Whitcroft et al. ....	606/22
5,464,436 A	11/1995	Smith .....	607/89	6,269,818 B1	8/2001	Lui et al. ....	128/898
5,473,408 A	12/1995	Hoffman et al. ....	355/53	6,273,884 B1	8/2001	Altshuler et al. ....	606/9
5,481,385 A	1/1996	Zimmerman et al. ....	349/62	6,273,885 B1	8/2001	Koop et al. ....	606/9
5,486,172 A	1/1996	Chess .....	606/20	6,277,111 B1	8/2001	Clement et al. ....	606/9
5,519,534 A	5/1996	Smith et al. ....	359/599	6,280,438 B1	8/2001	Eckhouse et al. ....	606/9
5,549,660 A	8/1996	Mendes et al. ....	607/88	6,290,713 B1	9/2001	Russell .....	607/88
5,556,612 A	9/1996	Anderson et al. ....	424/59	6,306,130 B1	10/2001	Anderson et al. ....	606/27
5,578,022 A	11/1996	Scherson et al. ....	604/304	6,322,584 B2	11/2001	Ingle et al. ....	607/96
5,595,568 A	1/1997	Anderson et al. ....	606/9	6,379,376 B1	4/2002	Lubart .....	607/88
5,606,798 A	3/1997	Kelman .....	30/41.5	6,408,212 B1	6/2002	Neev .....	607/100
5,611,798 A	3/1997	Eggers .....	606/31	6,413,255 B1	7/2002	Stern .....	606/41
5,624,435 A	4/1997	Furumoto et al. ....	606/10	6,413,268 B1	7/2002	Hartman .....	607/94
5,628,744 A	5/1997	Coleman et al. ....	606/12	6,428,198 B1	8/2002	Saccomanno et al. ....	385/147
5,630,811 A	5/1997	Miller .....	606/9	6,436,127 B1	8/2002	Anderson et al. ....	607/89
5,632,741 A	5/1997	Zavislan et al. ....	606/9	6,440,122 B1	8/2002	Shimoji .....	606/2
5,643,252 A	7/1997	Waner et al. ....	606/9	6,441,943 B1	8/2002	Roberts et al. ....	359/267
5,647,866 A	7/1997	Zaiase et al. ....	606/9	6,451,007 B1	9/2002	Koop et al. ....	606/9
5,658,323 A	8/1997	Miller .....	607/89	6,485,484 B1	11/2002	Connors et al. ....	606/9
5,662,643 A	9/1997	Kung, V et al. ....	606/3	6,494,900 B1	12/2002	Salansky et al. ....	607/89
5,669,916 A	9/1997	Anderson .....	606/133	6,508,813 B1	1/2003	Altshuler .....	606/9
5,683,380 A	11/1997	Eckhouse et al. ....	606/9	6,511,475 B1	1/2003	Altshuler et al. ....	606/9
5,700,240 A	12/1997	Barwick, Jr. et al. ....	604/22	6,514,242 B1	2/2003	Vasily et al. ....	606/9
5,707,403 A	1/1998	Grove et al. ....	607/89	6,516,013 B1	2/2003	Patzel et al. ....	372/29.02
5,728,090 A	3/1998	Martin et al. ....	606/3	6,517,532 B1	2/2003	Altshuler et al. ....	606/9
5,735,844 A	4/1998	Anderson et al. ....	606/9	6,533,775 B1	3/2003	Rizoiu .....	606/9
5,743,901 A	4/1998	Grove et al. ....	606/9	6,536,914 B2	3/2003	Hoelen et al. ....	362/231
5,752,948 A	5/1998	Tankovich et al. ....	606/9	6,548,781 B1	4/2003	Brunwinkel .....	219/121.73
5,752,949 A	5/1998	Tankovich et al. ....	606/9	6,563,853 B2	5/2003	Heist et al. ....	372/57
5,766,214 A	6/1998	Mehl, Sr. et al. ....	606/9	6,567,696 B2	5/2003	Voznesensky et al. ....	607/3
5,769,844 A	6/1998	Ghaffari .....	606/16	6,572,637 B1	6/2003	Yamazaki et al. ....	607/89
5,792,137 A	8/1998	Carr et al. ....	606/29	6,600,951 B1	7/2003	Anderson .....	604/20
5,814,040 A	9/1998	Nelson et al. ....	606/9	6,605,080 B1	8/2003	Altshuler et al. ....	606/3
5,817,089 A	10/1998	Tankovich et al. ....	606/9	6,610,052 B2	8/2003	Furumoto .....	606/9
5,820,625 A	10/1998	Izawa et al. ....	606/9	6,621,702 B2	9/2003	Elias et al. ....	361/700
5,824,023 A	10/1998	Anderson .....	607/88	6,637,924 B2	10/2003	Pelka et al. ....	362/555
5,830,208 A	11/1998	Muller .....	606/9	6,641,044 B2	11/2003	Plesko .....	235/462.49
5,843,072 A	12/1998	Furumoto et al. ....	606/9	6,648,904 B2	11/2003	Altshuler et al. ....	607/96
5,846,252 A	12/1998	Mehl, Sr. ....	606/133	6,653,618 B2	11/2003	Zenzie .....	250/221
5,849,029 A	12/1998	Eckhouse et al. ....	607/104	6,659,999 B1	12/2003	Anderson et al. ....	606/9
5,853,407 A	12/1998	Miller .....	606/9	6,660,000 B2	12/2003	Neuberger et al. ....	606/9
5,868,732 A	2/1999	Waldman et al. ....	606/9	6,663,620 B2	12/2003	Altshuler et al. ....	606/9
5,871,479 A	2/1999	Furumoto et al. ....	606/9	6,663,659 B2	12/2003	Mcdaniel .....	607/88
5,871,480 A	2/1999	Tankovich .....	606/9	6,666,856 B2	12/2003	Connors et al. ....	606/9
5,871,521 A	2/1999	Kaneda et al. ....	607/89	6,723,090 B2	4/2004	Altshuler et al. ....	606/9
5,879,346 A	3/1999	Waldman et al. ....	606/9	6,733,493 B2	5/2004	Gruzdev et al. ....	606/9
5,885,273 A	3/1999	Eckhouse et al. ....	606/9	6,749,624 B2	6/2004	Knowlton .....	607/104
5,944,748 A	8/1999	Mager et al. ....	607/88	6,758,845 B1	7/2004	Weckwerth et al. ....	606/9
5,966,210 A	10/1999	Rosow et al. ....	356/213	6,790,205 B1	9/2004	Yamazaki et al. ....	606/9
5,968,034 A	10/1999	Fullmer et al. ....	606/9	6,808,287 B2	10/2004	Lebens et al. ....	362/184
5,989,267 A	11/1999	Anderson .....	606/133	6,817,997 B2	11/2004	Furuno et al. ....	606/9
6,015,404 A	1/2000	Altshuler et al. ....	606/9	6,872,221 B2	3/2005	Lytle .....	607/89
RE36,634 E	3/2000	Ghaffari .....	606/9	6,887,260 B1	5/2005	Mcdaniel .....	607/88
6,059,765 A	5/2000	Cole et al. ....	604/500	6,902,563 B2	6/2005	Wilkens et al. ....	606/9
6,072,551 A	6/2000	Jansson et al. ....	349/64	6,955,672 B2	10/2005	Cense et al. ....	606/9
6,080,146 A	6/2000	Altshuler et al. ....	606/9	6,957,905 B1	10/2005	Pritchard et al. ....	362/554
6,096,029 A	8/2000	O'donnell, Jr. ....	606/9	6,976,984 B2*	12/2005	Cense et al. ....	606/9
6,104,959 A	8/2000	Spertell .....	607/101	7,029,469 B2	4/2006	Vasily .....	606/9
6,106,514 A	8/2000	O'donnell, Jr. ....	606/9	7,068,910 B2	6/2006	Duine et al. ....	385/146
6,114,862 A	9/2000	Tartagni et al. ....	324/662	7,077,544 B2	7/2006	Parker .....	607/90
6,134,475 A	10/2000	Will .....	607/98	7,083,610 B1	8/2006	Murray et al. ....	606/9
6,138,041 A	10/2000	Yahia .....	455/569.2	7,115,123 B2	10/2006	Knowlton et al. ....	606/41
				7,118,563 B2	10/2006	Weckwerth et al. ....	606/9
				7,204,832 B2	4/2007	Altshuler et al. ....	606/9
				7,250,045 B2	7/2007	Island et al. ....	606/17

(56)

## References Cited

## U.S. PATENT DOCUMENTS

7,250,047 B2	7/2007	Anderson et al.	606/32
7,413,567 B2	8/2008	Weckwerth et al.	606/10
7,452,356 B2	11/2008	Grove et al.	606/9
7,762,964 B2	7/2010	Slatkine	601/7
7,981,111 B2	7/2011	Grove et al.	606/27
8,346,347 B2	1/2013	Altshuler et al.	600/476
8,551,104 B2	10/2013	Weckwerth et al.	606/89
8,709,003 B2	4/2014	Island et al.	606/9
2001/0023363 A1	9/2001	Harth et al.	607/90
2001/0046131 A1	11/2001	Hoelen et al.	362/231
2001/0048801 A1	12/2001	Saccomanno et al.	385/147
2002/0005475 A1	1/2002	Zenzie	250/221
2002/0015430 A1	2/2002	Osmanow et al.	372/55
2002/0031160 A1	3/2002	Desor	372/57
2002/0049483 A1	4/2002	Knowlton	607/101
2002/0091377 A1	7/2002	Anderson et al.	606/9
2002/0097587 A1	7/2002	Krietzman et al.	362/553
2002/0128635 A1	9/2002	Altshuler et al.	606/9
2002/0128695 A1	9/2002	Harth et al.	607/88
2002/0151887 A1	10/2002	Stern et al.	606/41
2002/0161357 A1	10/2002	Anderson et al.	606/9
2002/0161418 A1	10/2002	Wilkens et al.	607/90
2002/0173780 A1	11/2002	Altshuler et al.	606/9
2002/0173833 A1	11/2002	Korman et al.	607/88
2002/0183811 A1	12/2002	Irwin	607/94
2003/0004499 A1	1/2003	Mcdaniel	606/3
2003/0009158 A1	1/2003	Perricone	606/9
2003/0032950 A1	2/2003	Altshuler et al.	606/9
2003/0036751 A1	2/2003	Anderson et al.	606/9
2003/0046825 A1	3/2003	Slingo	34/96
2003/0050561 A1	3/2003	Bazin et al.	600/476
2003/0055413 A1	3/2003	Altshuler et al.	606/9
2003/0055414 A1	3/2003	Altshuler et al.	606/9
2003/0065314 A1	4/2003	Altshuler et al.	606/9
2003/0080755 A1	5/2003	Kobayashi	
2003/0094714 A1	5/2003	Buazza et al.	264/1.38
2003/0105069 A1	6/2003	Robinson et al.	514/185
2003/0112623 A1	6/2003	Yu et al.	362/118
2003/0133292 A1	7/2003	Mueller et al.	362/231
2003/0138249 A1	7/2003	Merola et al.	396/661
2003/0146122 A1	8/2003	Westfield et al.	206/349
2003/0169400 A1	9/2003	Buazza et al.	351/159.62
2003/0177657 A1	9/2003	Andis et al.	34/96
2003/0195494 A1	10/2003	Altshuler et al.	606/9
2003/0199859 A1	10/2003	Altshuler et al.	606/9
2003/0216795 A1	11/2003	Harth et al.	607/88
2003/0220633 A1	11/2003	Angeley et al.	606/18
2003/0232356 A1*	12/2003	Dooley et al.	435/6
2003/0233138 A1	12/2003	Spooner	607/93
2004/0006328 A1	1/2004	Anderson	604/501
2004/0010298 A1	1/2004	Altshuler et al.	607/88
2004/0010299 A1	1/2004	Tolkoff et al.	607/88
2004/0034319 A1	2/2004	Anderson et al.	604/20
2004/0034341 A1	2/2004	Altshuler et al.	606/3
2004/0036975 A1	2/2004	Slatkine	359/584
2004/0046108 A1	3/2004	Spector	250/227.13
2004/0054386 A1	3/2004	Martin et al.	607/88
2004/0073079 A1	4/2004	Altshuler et al.	600/1
2004/0093042 A1	5/2004	Altshuler et al.	607/88
2004/0116913 A1	6/2004	Pilcher et al.	606/9
2004/0120151 A1	6/2004	Ostler et al.	362/294
2004/0122492 A1	6/2004	Harth et al.	607/88
2004/0147985 A1	7/2004	Macfarland et al.	607/90
2004/0167499 A1	8/2004	Grove et al.	606/9
2004/0167500 A1	8/2004	Weckwerth et al.	606/9
2004/0167501 A1	8/2004	Island et al.	606/9
2004/0167502 A1	8/2004	Weckwerth et al.	606/9
2004/0167592 A1	8/2004	Grove et al.	607/96
2004/0176754 A1	9/2004	Island et al.	606/9
2004/0176823 A1	9/2004	Island et al.	607/88
2004/0225339 A1	11/2004	Yaroslavsky et al.	607/88
2004/0233655 A1	11/2004	Zimmerman et al.	362/19
2004/0241254 A1	12/2004	Kopas et al.	424/727
2004/0252940 A1	12/2004	Atac et al.	385/31
2005/0008049 A1	1/2005	Oomori et al.	372/36

2005/0038418 A1	2/2005	Altshuler et al.	606/9
2005/0069566 A1	3/2005	Tamarkin et al.	424/401
2005/0085878 A1	4/2005	Wilkens et al.	607/94
2005/0107849 A1	5/2005	Altshuler et al.	607/88
2005/0186168 A1	8/2005	Albin et al.	424/70.14
2005/0234527 A1	10/2005	Slatkine	607/89
2005/0276072 A1	12/2005	Hayashi et al.	362/609
2006/0142750 A1	6/2006	Da Silva et al.	606/27
2006/0149343 A1	7/2006	Altshuler et al.	607/90
2006/0206103 A1	9/2006	Altshuler et al.	606/9
2007/0025947 A1	2/2007	Hansenne et al.	424/70.22
2007/0027440 A1	2/2007	Altshuler et al.	606/9
2007/0032847 A1*	2/2007	Weckwerth et al.	607/93
2007/0038206 A1	2/2007	Altshuler et al.	606/20
2007/0042020 A1	2/2007	Howard	424/439
2007/0060819 A1*	3/2007	Altshuler et al.	600/475
2007/0129711 A1	6/2007	Altshuler et al.	
2007/0198004 A1	8/2007	Altshuler et al.	606/9
2007/0248590 A1	10/2007	Milne et al.	424/130.1
2007/0292461 A1	12/2007	Tamarkin et al.	424/401
2007/0299244 A1	12/2007	Chaki et al.	530/303
2008/0027518 A1	1/2008	Island et al.	607/88
2008/0077198 A1	3/2008	Webb et al.	607/88
2008/0125834 A1	5/2008	Hendrix et al.	607/88
2008/0147053 A1	6/2008	Kang et al.	606/9
2009/0043294 A1	2/2009	Island et al.	606/9
2009/0270848 A1	10/2009	Weckwerth et al.	606/9
2010/0069898 A1	3/2010	O'neil et al.	606/9

## FOREIGN PATENT DOCUMENTS

JP	06-273758 A	9/1994	G02F 1/1335
JP	06-334950 A	12/1994	H04N 5/74
JP	11244295 A	9/1999	A61B 18/20
JP	2000300683 A	10/2000	A61B 18/20
JP	2000515410	11/2000	A61B 18/20
JP	2001252363 A	9/2001	A61B 17/00
JP	2002253573 A	9/2002	A61B 18/20
JP	2003024458 A	1/2003	A61N 5/06
JP	2004136019 A	5/2004	A45D 26/00
JP	2004527330 A	9/2004	A61B 17/00
JP	2004533866 A	11/2004	A61B 18/18
JP	2005278724 A	10/2005	A45D 26/00
JP	2006192073 A	7/2006	A61N 5/06
JP	2006518614 A	8/2006	A61B 18/20
JP	2006525036 A	11/2006	A61B 17/00
JP	2007508243 A	4/2007	A61K 31/025
JP	2009509140 A	3/2009	A61B 5/00
JP	5146517 B2	2/2013	H01L 21/28
WO	96/14083 A1	5/1996	A23L 1/015
WO	00/02491 A1	1/2000	A61K 41/00
WO	02/094116 A1	11/2002	A61B 18/18
WO	03/001984 A2	1/2003	
WO	03/017824 A2	3/2003	A61B 18/00
WO	03/043697	5/2003	A61N 5/06
WO	03/049633 A1	6/2003	A45D 26/00
WO	2004/075731 A2	9/2004	A61B 18/20
WO	2004/080279 A2	9/2004	A61B 18/20
WO	2005/063193 A1	7/2005	A61K 8/06
WO	2007/019536 A2	2/2007	A61B 18/20
WO	2009/089177 A1	7/2009	A61N 1/00

## OTHER PUBLICATIONS

Brunsting, L.A. et al., "The Color of the Skin as Analyzed by Spectrophotometric Methods: III. The Role of Superficial Blood," The Journal of Clinical Investigation, vol. 7, 21 pages, Apr. 29, 1929.

Brown, E.B., "Modern Optics," Radiometry and Photometry, Reinhold Publishing Corporation, 3 pages, 1965.

Cornelius, C.E. et al., "Red Fluorescence of Comedones: Production of Porphyrins by Corynebacterium Acnes," The Journal of Investigative Dermatology, vol. 49(4), PMID: 4228644, [PubMed—Indexed for Medline], 3 pages, Oct. 1967.

Formanek, I. et al., "Porphyrinsynthesis by Propionibacterium Acnes (author's translation)," Archives for Dermatological

## (56) References Cited

## OTHER PUBLICATIONS

- Research, vol. 259(2), German, PMID: 334087 [PubMed—indexed for Medline], 9 pages, Aug. 22, 1977.
- Lee, W.L. et al., "Comparative Studies of Porphyrin Production in Propionibacterium Acnes and Propionibacterium Granulosum," *Journal of Bacteriology*, vol. 133(2), PMID: 637914 [PubMed—Indexed for Medline] 5 pages, Aug. 25, 1977.
- Mills, O.H. et al., "Ultraviolet Phototherapy and Photochemotherapy of Acne Vulgaris," *Archives of Dermatological Research*, vol. 114(2), PMID: 147054 [PubMed: Indexed for Medline] 3 pages, Feb. 1978.
- Fanta, D. et al., "Porphyrinsynthesis of Propionibacterium Acnes in Acne and Seborrhea (author's translation)," *Archives of Dermatological Research*, vol. 261, German, PMID: 148872 [PubMed—indexed for Medline], 5 pages, Apr. 7, 1978.
- McGinley, K.J. et al., "Facial Follicular Porphyrin Fluorescence: Correlation with Age and Density of Propionibacterium Acnes," *British Journal of Dermatology*, Vol. 102(4), PMID: 7387886 [PubMed—Indexed for Medline] 5 pages, Jul. 24, 1979.
- Sliney, D. et al., "Safety with Lasers and Other Optical Sources, a Comprehensive Handbook," Plenum Press, 9 pages, Jul. 1980.
- Fanta, D. et al., "Porphyrin Synthesis by Propionibacteria in Dependence of External Factors," *Archives of Dermatological Research*, vol. 271, 7 pages, Jul. 10, 1980.
- Melo, T.B. et al., "In Vivo Porphyrin Fluorescence for Propionibacterium Acnes. A Characterization fo the Fluorescing Pigments," *Dermatologica*, vol. 164(3), PMID: 7084539 [PubMed—Indexed for Medline] 9 pages, Mar. 1982.
- Parrish, J. et al., "Erythema and Melanogenesis Action Spectra of Normal Human Skin," *Photochemistry and Photobiology*, vol. 36, 5 pages, Mar. 15, 1982.
- Kjeldstad, B. et al., "Influence of pH on Porphyrin Production in Propionibacterium Acnes," *Archives of Dermatological Research*, vol. 276(6), PMID: 6517611 [PubMed—Indexed for Medline] 5 pages, 1984.
- Melo, T.B. et al., "Photodestruction of Propionibacterium Acnes Porphyrins," *Z. Naturforsch.*, vol. 40(C), PMID: 3993179 [PubMed—Indexed for Medline] 4 pages, Oct. 22, 1984.
- Kjeldstad, B. et al., "Porphyrin Photosensitization of Bacteria," *Adv. Exp. Med. Biol.*, PMID: 4096295 [PubMed—indexed for Medline], 5 pages, 1985.
- Kjeldstad, B. et al., "An Action Spectrum for Blue and Near Ultraviolet Inactivation of Propionibacterium Acnes; with Emphasis on a Possible Porphyrin Photosensitization," *Photochemistry and Photobiology*, vol. 43(1), PMID: 3952162 [PubMed—Indexed for Medline] 4 pages, Jul. 19, 1985.
- Guideline for Limits of Exposure to Ultraviolet Radiation of Wavelengths between 180 nm and 400 nm, *Health Physics*, vol. 49, No. 2, 10 pages, Aug. 1985.
- Meffert, H. et al., "Phototherapy of Acne Vulgaris with the "TuR" UV 10 Body Section Irradiation Unit [translation]," *Dermatol. Monatsscher.*, vol. 172, German, PMID: 2938991 [PubMed—Indexed for Medline] 6 pages, 1986.
- Meffert, H. et al., "Phototherapy of Acne Vulgaris with the UVA Irradiation Instrument TBG 400 [translation]," *Dermatol. Monatsscher.*, vol. 172, German, PMID: 2937663 [PubMed—Indexed for Medline] 2 pages, 1986.
- Johnsson, A. et al., "Fluorescence from Pilosebaceous Follicles," *Archives of Dermatological Research*, vol. 279(3), PMID: 3592747 [PubMed—Indexed for Medline] 4 pages, 1987.
- Meffert, H. et al., "Treatment of Acne Vulgaris with Visible Light [translation]," *Dermatol. Monatsscher.*, vol. 173, German, PMID: 2963772 [PubMed—Indexed for Medline] 2 pages, 1987.
- Meffert, H. et al., "Therapy of Acne with Visible Light. Decreased Irradiation Time by Using a Blue-Light High-Energy Lamp [translation]" *Dermatol. Monatsschr.*, German, PMID: 2150382 [PubMed—Indexed for Medline] 7 pages, 1990.
- Kjeldstad, B. et al., "Near-UV-Induced Radicals in Propionibacterium Acnes, Studied by Electron Spin Resonance Spectrometry at 77 K.," *Journal of Photochemistry and Photobiology*, vol. 9(2), PMID: 1650821 [PubMed—Indexed for Medline] 7 pages, Sep. 21, 1990.
- Morys et al., "The Accurate Measurements of Biologically Effective Ultraviolet Radiation," *International Symposium on High Latitude Optics*, 10 pages, Jul. 1993.
- Webster, G.F., "Inflammation in Acne Vulgaris," *Journal of the American Academy of Dermatology*, vol. 33(2 Pt. 1), Review, PMID: 7622652 [PubMed—Indexed for Medline] 7 pages, Aug. 1995.
- Leung, S., "The Porphyrin Page," website at <http://www.washburn.edu-cas-chemistry-sleung-porphyrin/page.html>, Created Apr. 16, 1996, Last Modified Nov. 11, 2002, printed Jun. 22, 2004, 7 pages, Apr. 16, 1996.
- Arakane, K. et al., "Singlet Oxygen (1 delta g) Generation from Coproporphyrin in Propionibacterium Acnes on Irradiation," *Biochemical and Biophysical Research Communication*, vol. 223, Article No. 0937, PMID: 8687438 [PubMed—Indexed for Medline], 6 pages, Jun. 25, 1996.
- Sigurdsson, V. et al., "Phototherapy of Acne Vulgaris with Visible Light," *Dermatology*, vol. 194(3), PMID: 9187844 [PubMed—Indexed for Medline] 5 pages, Nov. 15, 1996.
- Predicate Devices: LightSheer Diode Laser System by Star Medical/Coherent Star, K973324, K982940, K001746, 1997.
- Leydon, J., "Therapy for Acne Vulgaris," *The New England Journal of Medicine*, Review Article, 6 pages, Apr. 17, 1997.
- UV Index definition, Canadian Environmental Web page, See entire document, 3 pages, Jun. 1, 1998.
- Code of Federal Regulations, Class I Accessible Emmission Limits for Laser Radiation, Food and Drug Administration, HHS, 2 pages, Apr. 1, 1999.
- IEC Technical Report 60825-8, "Safety of Laser Products—Guide for the Safe Use of Medical Laser Equipment," 6 pages, Nov. 1999.
- Papageorgiou, P. et al., "Phototherapy wit Blue (415 nm) and Red (660 nm) Light in the Treatment of Acne Vulgaris," *British Journal of Dermatology*, vol. 142(5), PMID: 10809858 [PubMed—indexed for Medline] 6 pages, Dec. 7, 1999.
- Angelopoulou, E. et al., "The Reflectance Spectrum of Human Skin," Technical Report, Department of Computer and Information Science, 15 pages, Dec. 20, 1999.
- Romiti, R. et al., "High-Performance Liquid Chromatography Analysis of Porphyrins in Propionibacterium Acnes," *Archives of Dermatological Research*, vol. 292(6), PMID: 10929774 [PubMed—Indexed for Medline] 3 pages, Jan. 7, 2000.
- Shalita, A. et al., "Acne Photoclearing (APC) Using a Novel, High-Intensity, Enhanced, Narrow-Band, Blue Light Source," *Clinical Application Notes*, vol. 9(1), ESC Medical Systems Ltd., PB 558-0230, Rev. A, 4 pages, 2001.
- International Standard IEC 60825.1, Safety of Laser Products—Part 1: Equipment Classification, Requirements and User's Guide, Edtion 1.2, 121 pages, 2001.
- Kawada, A. et al., "Acne Phototherapy with a High-Intensity, Enhanced, Narrow-Band, Blue Light Source: An Open Study and In Vitro Investigation," *Journal of Dermatological Science*, vol. 30(2), PMID: 12413768 [PubMed—indexed for Medline] 7 pages, Jun. 19, 2002.
- Ashkenazi, H. et al., "Eradication of Propionibacterium Acnes by its Endogenic Porphyrins after Illumination with High Intensity Blue Light," *FEMS Immunology and Medical Microbiology*, vol. 35(1), PMID: 12589953 [PubMed: Indexed for MedLine], 8 pages, Jul. 24, 2002.
- Harnessing Light to Treat Stretch Marks and Other Hypopigmented Scars, Skin & Aging, Supplement to Nov. 2002 Skin & Aging.
- Hode, L., "Are Lasers More Dangerous than IPL Instruments?," *Lasers in Surgery and Medicine*, Supplement 15, 3 pages, 2003.
- U.S. Appl. No. 60/450,243, by Robert E. Grove, entitled "Method and Apparatus for the Treatment of Benign Pigmented Lesions", filed Feb. 25, 2003.
- U.S. Appl. No. 60/450,598, by Robert E. Grove, entitled "Personal Light Based Acne Treatment Device and Method", filed Feb. 26, 2003.

(56)

## References Cited

## OTHER PUBLICATIONS

- U.S. Appl. No. 60/451,091, by Robert E. Grove, entitled "Method and Device for Handheld and Cordless Light-Based Epilation", filed Feb. 28, 2003.
- U.S. Appl. No. 10/794,676, by Mark V. Weckworth et al. entitled "Method and Apparatus for the Repigmentation of Human Skin", filed Mar. 3, 2004.
- U.S. Appl. No. 60/452,304, by Robert E. Grove, entitled "Optical Sensor and Method for Identifying the Presence of Skin", filed Mar. 4, 2003.
- U.S. Appl. No. 60/451,981, by Robert E. Grove, entitled "Method and Apparatus for the Repigmentation of Human Skin", filed Mar. 4, 2003.
- U.S. Appl. No. 60/452,591, by Robert E. Grove, entitled "Method and Device for Sensing Skin Contact", filed Mar. 6, 2003.
- U.S. Appl. No. 60/456,379, by Robert E. Grove, entitled "Apparatus and Method for the Radiative Treatment of Skin with Increased Eye Safety", filed Mar. 20, 2003.
- U.S. Appl. No. 60/456,586, by Robert E. Grove, entitled "Handheld Dermatological Treatment Device with Power Meter", filed Mar. 21, 2003.
- U.S. Appl. No. 60/458,861, by Robert E. Grove, entitled "Method and Apparatus for Dermatologic Treatment Utilizing Battery-Powered Laser Diode Bars", filed Mar. 27, 2003.
- U.S. Appl. No. 60/472,056, by Robert E. Grove, entitled "Apparatus and Method for Dermatologic Treatment", filed May 20, 2003.
- Micro Touch Trimmer website, [www.asseenontvwork.com/vcc/ideavillage/microtouch/104917](http://www.asseenontvwork.com/vcc/ideavillage/microtouch/104917), printed Dec. 4, 2003, 21 pages.
- EP Office Action, Application No. 04 714 604.8, 5 pages, Nov. 16, 2010.
- EP Office Action, Application No. 04 714 910.1, 6 pages, Nov. 16, 2010.
- Supplemental EP Search Report, Application No. 04 712 911.9, 3 pages, Dec. 6, 2010.
- Supplemental EP Search Report, Application No. 04 712 922.6, 3 pages, Dec. 7, 2010.
- Shnitkind, E. et al., "Anti-Inflammatory Properties of Narrow Band Blue Light," Poster Presentation (Conference Unknown), 1 page.
- Predicate Devices: SLP 1000 (LC 100) Diode Laser of Palomar Medical Technologies, K010580, K011747.
- Predicate Devices: Apex 800 Pulsed Diode Laser of Iridex Corporation, K020849.
- Predicate Devices: F1 Pulsed Diode Laser of Opus Medical, Inc., K030235.
- Predicate Devices: LightSheer Diode Laser System manufactured by Lumenis, Ltd.
- Predicate Devices: Quantum Flash Lamp System Manufactured by Lumenis, Ltd.
- Predicate Devices: CoolGlide Excel YAG Laser by Altus, Inc.
- Predicate Devices: Devices by Ya-Man Ltd., of Tokyo, Japan.
- Predicate Devices: Oriel Instruments Model 48010, by Spectra-Physics, Stratford, CT.
- Predicate Devices: Panasonic part No. P-170SCW, or HHR300SCP Ni-MH Rechargeables, Panasonic P-170SCR P NiCd, by Panasonic Matsushita Electric Corporation of America, Secaucus, NJ.
- Predicate Devices: Laser Diode Bar Packages, Part No. ASM06C040W08010B80, Cutting Edge Optronics, of St. Charles, MO.
- Predicate Devices: Part No. HX8-101 or FAN-101, or CP 0.8-31-06L, from Melcor.
- Predicate Devices: PIC18LF452, manufactured by Microchip Technologies of Chandler, AZ.
- Predicate Devices: Transistors IRL3716 (International Rectifier Corp., El Segundo, CA).
- Palomar Super Long Pulse Diode Laser System, Clinical Data, Palomar Medical Technologies brochure.
- Japanese Office Action, Application No. 2011-527040, 14 pages, Feb. 21, 2014.
- Miller, Steve et al., "Isolation and Characterization of Protoporphyrin IX from Bacterial Catalase," *The Journal of Biological Chemistry*, vol. 235, No. 11, 3 pages, Mar. 7, 1960.
- Dalton, J. et al., "Reaction Between Molecular Oxygen and Photo-excited Protoporphyrin IX," *Nature*, vol. 235, 1 pages, Feb. 18, 1972.
- Hoeffler, Ulrich, "Enzymatic and Hemolytic Properties of Propionibacterium Acnes and Related Bacteria," *Journal of Clinical Microbiology*, vol. 6, No. 6, 4 pages, Jun. 10, 1977.
- Diffey, B. L. "The consistency of studies of ultraviolet erythema in normal human skin." *Physics in medicine and biology* 27.5, 6 pages, 1982.
- Meffert, H. et al., "Verkuzung der Bestrahlungszeit Verwendung eines Hochdruckstrahlers vom Blaulichttyp," *Dermatol. Mon. schr* 176, 8 pages, 1990.
- Karu, Tiina, "Primary and Secondary Mechanisms of Action of Visible to Near-IR Radiation on Cells," *Journal of Photochemistry and Photobiology*, vol. 49, 17 pages, Nov. 9, 1998.
- Saiki, Hiroyasu et al., "Diffusion of Porphyrins and Quinones in Organic Solvents," *Phys. Chem. Chem Phys.*, vol. 1, 4 pages, 1999.
- Yoo, Yeong-Min et al., "Hemoglobin Toxicity in Experimental Bacterial Peritonitis Is Due to Production of Reactive Oxygen Species," *Clinical and Diagnostic Laboratory Immunology*, vol. 6, No. 6, 2 pages, Jul. 12, 1999.
- Bagdonas, Saulius et al., "Phototransformations of 5-Aminolevulinic Acid-Induced Protoporphyrin IX in Vitro: A Spectroscopic Study," *Photochemistry and Photobiology*, vol. 72(2), 7 pages, May 6, 2000.
- Koval'skaya, N.E. et al., "The Efficiency of the Formation of Singlet Oxygen by a Sensitizer Based on Zinc Phthalocyanine," *Journal of Applied Spectroscopy*, vol. 68, No. 2, 4 pages, 2001.
- Buchczyk, Darius P. et al., "High Efficiency of 5-Aminolevulinic Acid-Induced Photodynamic Treatment Using UVA Irradiation," *Carcinogenesis*, vol. 22, No. 6, 5 pages, 2001.
- Mason, Maria G. et al., "Extracellular Heme Peroxidases in Actinomycetes: a Case of Mistaken Identity," *Applied and Environmental Microbiology*, vol. 67, No. 10, 8 pages, Jul. 18, 2001.
- Jappe, U. et al., "Propionibacterium Acnes and Inflammation in Acne; P. Acnes has T-Cell Mitogenic Activity," *British Journal of Dermatology*, vol. 146, 8 pages, Sep. 12, 2001.
- Elman et al., "The Effective Treatment of Acne Vulgaris by a High-Intensity, Narrow Band 405-420 nm Light Source," *Journal of Cosmetic & Laser Therapy*, vol. 5, 6 pages, Nov. 27, 2002.
- Wagener, Frank et al., "Different Faces of the Heme-Heme Oxygenase System in Inflammation," *Pharmaceutical Reviews*, vol. 55, No. 3, The American Society for Pharmacology and Experimental Therapeutics, 21 pages, 2003.
- Anonymous, "Akne-Guidelines Schweiz," [Online], Martin Pletscher: Dermatologie, Retrieved from Internet: <http://www.martinpletscher.ch/dermatologie/akne.html>, 5 pages, May 15, 2003.
- Burkhart, Craig N. et al., "Assessment of Etiologic Agents in Acne Pathogenesis," Review, Department of Microbiology and Immunology, and Dermatology, Medical College of Ohio at Toledo, 7 pages, Jul. 2003.
- Charakida, A. et al., "Phototherapy in the Treatment of Acne Vulgaris," *American Journal of Clinical Dermatology*, vol. 5(4), Adis. Data Information, 6 pages, 2004.
- Elman, M. et al., "Light Therapy in the Treatment of Acne Vulgaris," *Dermatological Surgery*, vol. 30(2), Dermatology and Lasers Clinic, Tel Aviv and Caesarea, Israel, American Society for Dermatology Surgery, 8 pages, Feb. 2004.
- Elman, M. et al., "The Role of Pulsed Light and Heat Energy (LHE) in Acne Clearance," *Journal of Cosmetic Laser Therapy*, vol. 6, 5 pages, Apr. 1, 2004.
- Omi, Tokuya et al., "420 nm Intense Continuous Light Therapy for Acne," *Journal of Cosmetic Laser Therapy*, vol. 6, 7 pages, Aug. 12, 2004.
- Krauthaim, A. et al., "Acne: Topical Treatment," *Clinics in Dermatology*, vol. 22, No. 5, XP004647111, 10 pages, Sep. 1, 2004.
- Ross, Victor E., "Optical Treatment for Acne," *Dermatological Therapy*, vol. 18, ISSN 1396-0296, 14 pages, 2005.
- Ross, Victor E., "Acne, Lasers, and Light," *Advances in Dermatology*, vol. 21, 29 pages, 2005.

(56)

## References Cited

## OTHER PUBLICATIONS

Ortiz, Arisa et al., "A Review of Lasers and Light Sources in the Treatment of Acne Vulgaris," *Journal of Cosmetic and Laser Therapy*, vol. 7, 7 pages, Mar. 7, 2005.

Hamblin, M. et al., "Helicobacter Phylori Accumulates Photoactive Porphyrins and Is Killed by Visible Light," *Antimicrobial Agents and Chemotherapy*, vol. 49, No. 7, American Society for Microbiology, 6 pages, Mar. 7, 2005.

Mariwalla, Kavita et al., "Use of Lasers and Light-Based Therapies for Treatment of Acne Vulgaris," *Lasers in Surgery and Medicine*, vol. 37, 10 pages, Oct. 12, 2005.

Mariwalla, Kavita et al., "Non-Traditional Acne Therapy: The Use of Lasers and Light-Based Therapies," *US Dermatology Review* 2006, 4 pages, 2006.

Tremblay, J.F. et al., "Light-Emitting Diode 415 nm in the Treatment of Inflammatory Acne: An Open-Label, Multicentric, Pilot Investigation," *Journal of Cosmetic and Laser Therapy*, vol. 8, 3 pages, Jan. 25, 2006.

Goldberg, David J. et al., "Combination Blue (415 nm) and red (633 nm) LED Phototherapy in the Treatment of Mild to Severe Acne Vulgaris," *Journal of Cosmetic and Laser Therapy*, vol. 8, 5 pages, Mar. 29, 2006.

Lee, Seung Yoon et al., "Blue and Red Light Combination LED Phototherapy for Acne Vulgaris in Patients with Skin Phototype IV," *Lasers in Surgery and Medicine*, vol. 39, 9 pages, Nov. 16, 2006.

Nestor, M., "The Use of Photodynamic Therapy for Treatment of Acne Vulgaris," *Dermatologic Clinics*, vol. 25, 11 pages, 2007.

"Light Dose Ranging Study of Photodynamic Therapy (PDT) with Levulan + Blue Light in Severe Facial Acne," DUSA Pharmaceuticals, Inc., <http://clinicaltrials.gov/ct2/show/NCT00706433>, 25 pages, Mar. 2007.

Anonymous, "BlueLight Acne Treatments," [Online], Retrieved from Internet: [http://www.topdocs.com/display\\_procedure.php?id=bluelight](http://www.topdocs.com/display_procedure.php?id=bluelight), 2 pages, Apr. 10, 2008.

"Comparison of Claro to Other Dermatological Devices for Acne Treatment," Quantitative Assessment of Light Illumination on Organism Reduction; Subculture agar: TSA + 5% Sheep's Blood (Blood agar) Organism Diluent: Butterfield's Buffer or 0.85% Saline; Propionibacterium Acnes (ATCC 11827), 16 pages, Jun. 23, 2008.

Anonymous, "Vi Derm Product Line," [Online], Kalil Medical Products, Retrieved from Internet: [http://www.kalilmedical.com/doctor/vi\\_derm\\_products.asp](http://www.kalilmedical.com/doctor/vi_derm_products.asp), 4 pages, Mar. 2, 2010.

International Search Report, Application No. PCT/US2009/056961, 7 pages, Jun. 29, 2010.

International Preliminary Report on Patentability, PCT/US2009/056961, 11 pages, Mar. 22, 2011.

International Preliminary Report on Patentability, PCT/US2009/057204, 8 pages, Mar. 22, 2011.

Supplementary European Search Report, Application No. 09815144, 9 pages, Feb. 10, 2012.

European Office Action, Application No. 09815144.2, 6 pages, Oct. 10, 2012.

European Search Report, Application No. 08797565.2, 6 pages, Oct. 29, 2012.

Japanese Office Action, Application No. 2010-520342, 6 pages, Mar. 7, 2013.

European Office Action, Application No. 09815144.2, 5 pages, Apr. 3, 2013.

Japanese Office Action, Application No. 2009-261364, 7 pages, Jun. 18, 2013.

Extended European Search Report, Application No. 13159309.7, 7 pages, May 7, 2013.

Japanese Office Action, Application No. 2011-506499, 5 pages, Nov. 26, 2013.

U.S. Non-Final Office Action, U.S. Appl. No. 14/047,998, 7 pages, Jul. 5, 2016.

Balentine, Douglas A. et al., "The Chemistry of Tea Flavonoids," *Critical Reviews in Food Science and Nutrition*, vol. 37, No. 8, pp. 693-704 (12 pages total), 1997.

Dufresne, Christiane et al., "A Review of Latest Research Findings on the Health Promotion Properties of Tea," *Journal of Nutritional Biochemistry*, vol. 12, pp. 404-421 (18 pages total), 2001.

Non-Final Office Action, U.S. Appl. No. 14/047,998, 35 pages, Feb. 11, 2016.

U.S. Non-Final Office Action, U.S. Appl. No. 14/171,592, 39 pages, Nov. 23, 2016.

U.S. Final Office Action, U.S. Appl. No. 14/047,998, 6 pages, Jan. 6, 2017.

European Office Action, Application No. 13159309.7, 4 pages, May 8, 2014.

European Search Report, Application No. 09735456.7, 10 pages, Sep. 12, 2014.

\* cited by examiner

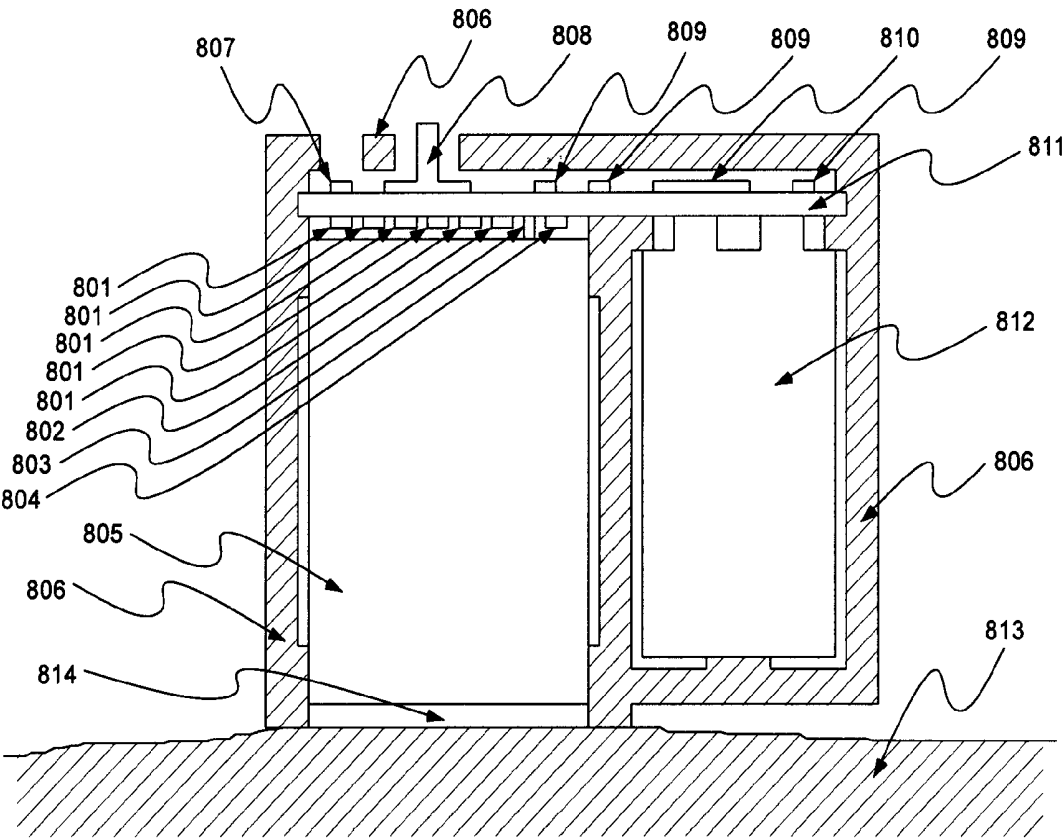
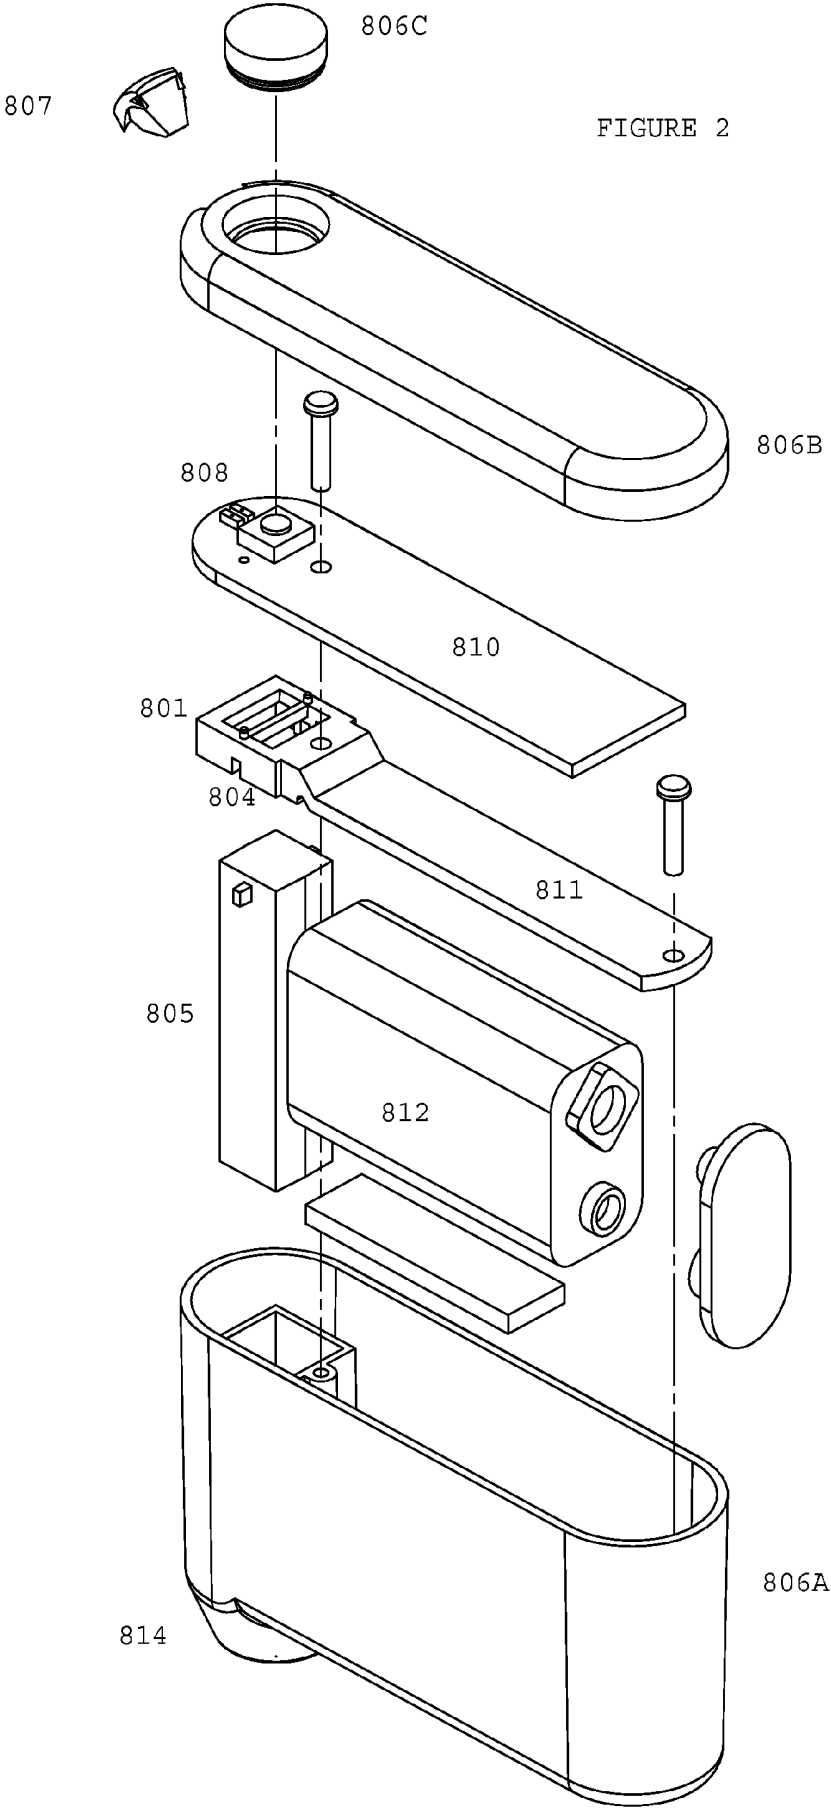


Fig. 1




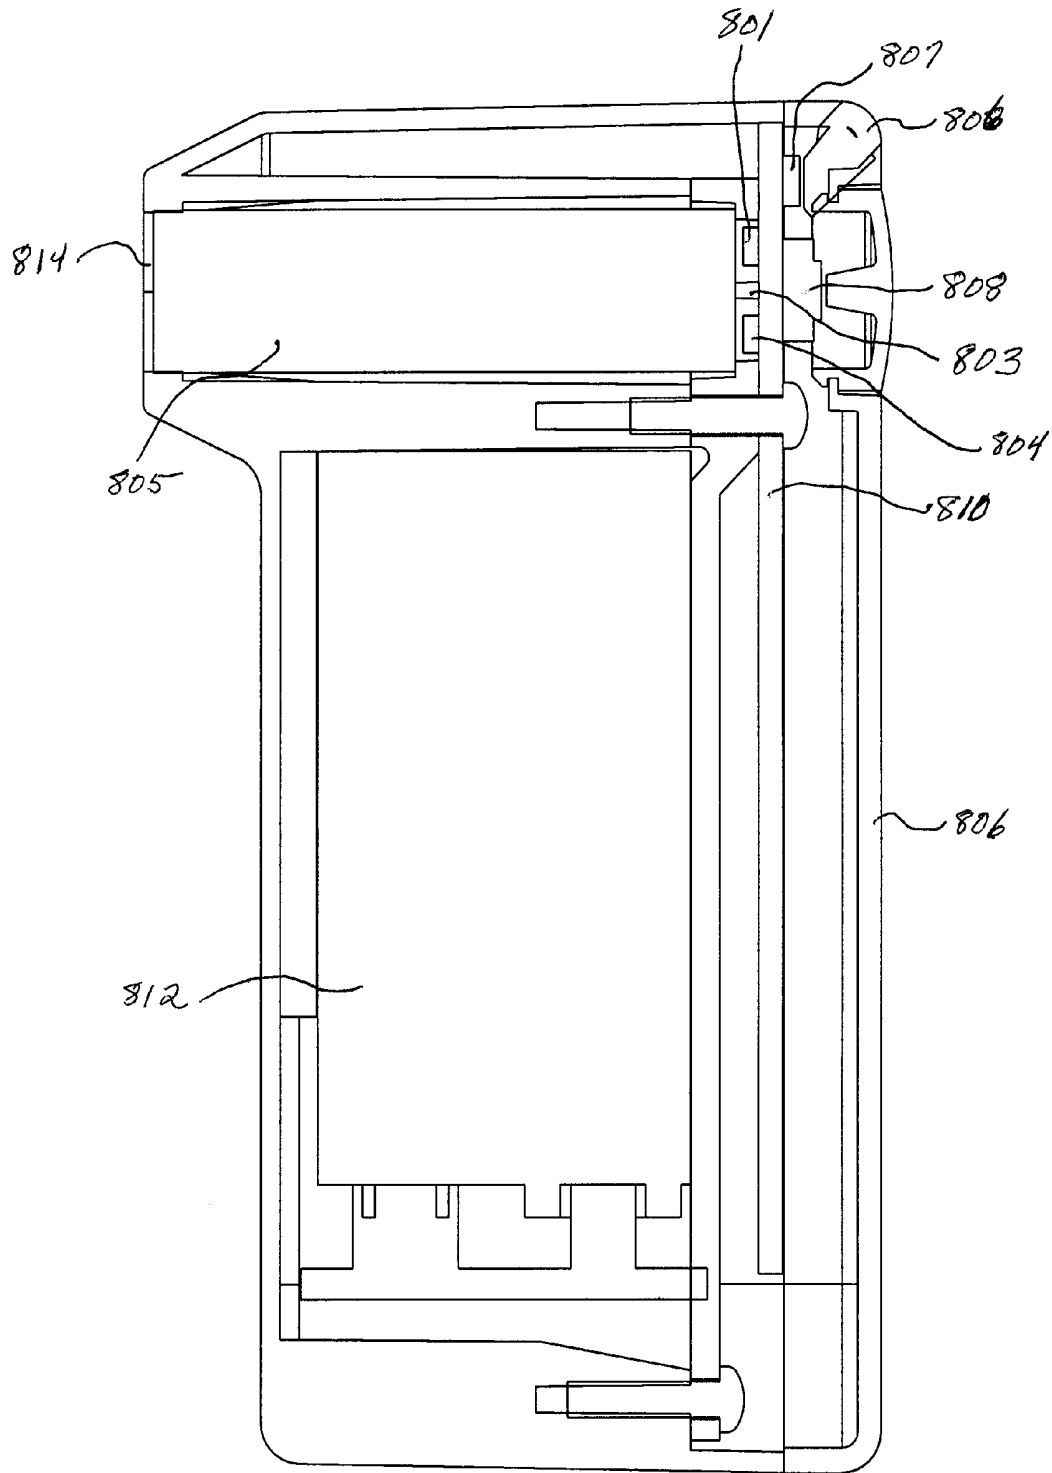


FIGURE 3

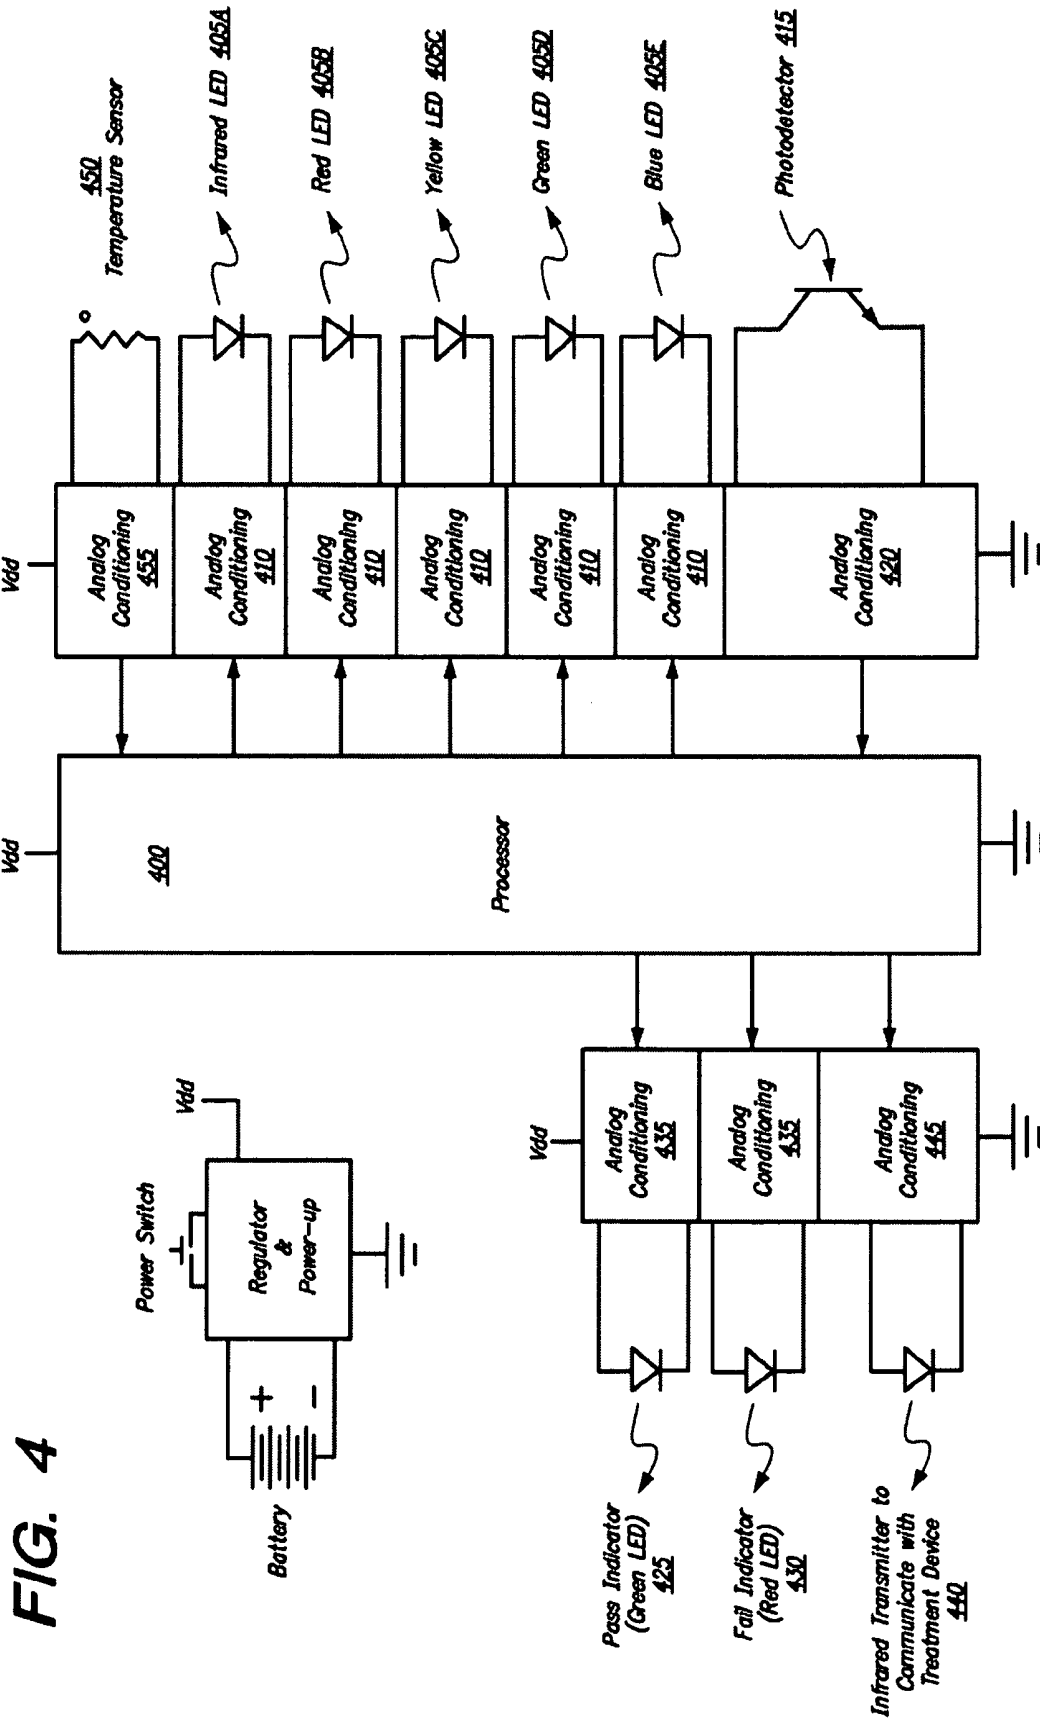

**OPTICAL SENSOR AND METHOD FOR  
IDENTIFYING THE PRESENCE OF SKIN  
AND THE PIGMENTATION OF SKIN**

RELATED APPLICATIONS

This application claims the benefit of U.S. Provisional Patent Application No. 61/048,154, filed Apr. 25, 2008, which is incorporated herein by reference. In addition, U.S. patent application Ser. No. 10/787,720, filed Feb. 25, 2004, now U.S. Pat. No. 7,413,567, issued on Aug. 19, 2008, U.S. Provisional Patent Application No. 60/450,243, filed Feb. 25, 2003; U.S. Provisional Patent Application No. 60/450,598, filed Feb. 26, 2003; U.S. Provisional Patent Application No. 60/451,091, filed Feb. 28, 2003; U.S. Provisional Patent Application No. 60/452,304, filed Mar. 4, 2003, U.S. Provisional Patent Application No. 60/451,981 filed Mar. 4, 2003; U.S. Provisional Patent Application No. 60/452,591, filed Mar. 6, 2003; U.S. Provisional Patent Applications No. 60/456,379, filed Mar. 20, 2003; U.S. Provisional Patent Application No. 60/456,586, filed Mar. 21, 2003; U.S. Provisional Patent Applications No. 60/458,861 filed Mar. 27, 2003, U.S. Provisional Patent Application No. 60/472,056, filed May 20, 2003, and U.S. Provisional Patent Application No. 61/048,154, filed Apr. 25, 2008, are also incorporated herein by reference.

FIELD OF THE INVENTION

The present application relates generally to devices and methods for differentiating human skin from other materials, and more particularly relates to devices and methods for optically differentiating human skin on a live person from other materials including other human tissue.

BACKGROUND OF THE INVENTION

Prior art devices that attempt to optically detect human skin have typically suffered from a number of limitations. Among them have been the issues of temperature sensitivity, that is, performance fluctuations caused by variations in operating or environmental temperature; variations in output power of the source, or sensitivity of the sensor.

Firstly, the device as described may be sensitive to temperature fluctuations. Since the LED's used as optical sources have an optical output power that depends on the temperature of the LED, the precise output power of each of the LED sources may vary with ambient temperature and may vary due to self-heating or by heating from the control electronics. Additionally, since the sensitivity of the phototransistor used to detect the remitted light may depend on the temperature of the phototransistor, the measurement of the remitted light may vary due to self-heating or by heating from the control electronics. Sources that vary in output power will affect the amount of light remitted. A phototransistor which has a sensitivity to temperature will give a measurement that has some error in the actual amount of remitted light.

Further, skin sensors in the prior art typically indicate only a broad indication of the presence of skin, which is less than ideal in at least some instances. None of the prior art measures the actual spectral remission at multiple wavelengths and reports that spectral remission for each wavelength as the fractional amount of light remitted at each wavelength. Thus, in the present invention, the ratio of the amount of light remitted at each wavelength is divided by

the amount of light of that wavelength incident on the skin, and this fraction is then available for further use.

In addition, the prior art is typically unable to ascertain the degree of pigmentation of the skin. This is desirable in at least some applications, especially for devices which rely upon thermolysis.

As a result, there are significant shortcomings with prior art devices, and there has been a long felt need for a device and a technique which overcomes or substantially reduces these limitations.

SUMMARY OF THE INVENTION

In accordance with the present invention, a single broadband source, or alternatively, multiple sources each of a unique emission spectra are used to illuminate a surface of interest. Multiple detectors each sensitive to a unique optical band or, alternatively, a single broad-band detector, respectively, is used to measure the amount of light remitted from said surface in each of the unique optical bands. Thus, a single broadband source can be used with multiple detectors each sensitive to a narrow wavelength band, or, alternatively, multiple narrow band sources with a single broadband detector. Still further, if increased cost and complexity is acceptable, multiple narrow band sources can be used with multiple narrow band detectors. In such a way, the spectral remission of the surface can be measured.

The spectral remission of skin, and particularly human skin in at least some embodiments, is characteristically different from most other materials. Therefore by obtaining the spectral remission from a surface of interest and by then comparing the obtained spectral remission to the spectral remission that is known to be skin one can determine whether the surface of interest is skin.

The present invention also addresses various other shortcomings of the prior art. While typical prior art optical skin-sensing devices can give variable results depending upon the operating temperature of the device, the present invention overcomes this limitation.

Therefore, the present invention provides a method for calibrating the skin sensor so that measurements of absolute remission can be converted to fractional remission.

In another embodiment of the present invention, a sensor is provided that can determine the presence of skin and also the pigmentation level of the skin.

The present invention further provides a device that is much less sensitive to ambient temperature conditions and is less sensitive to temperature variations caused by self-heating within the device.

In a preferred embodiment of the present invention a dermatological treatment device is provided which is self-contained, hand-held, and battery powered, and which has a skin sensor that compensates for temperature fluctuations and inhibits the emission of the treatment device unless the presence of skin is detected. In this preferred embodiment the sensor further detects the pigmentation level of the skin and emission of the treatment device is inhibited unless the pigmentation level of the skin is less than a predetermined level.

Alternatively, for some embodiments, the emission of the treatment device can be adjusted in accordance with the pigmentation level of the skin.

These and other attributes of the present invention may be better appreciated from the following description of the invention, together with the Figures.

## BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates in cross-sectional view an embodiment of the optical portion of a device in accordance with the invention.

FIG. 2 illustrates in exploded isometric view the major components of a device as shown in FIG. 1.

FIG. 3 illustrates in cross-sectional side a device as shown in FIG. 2.

FIG. 4 illustrates a schematic diagram of the circuit of an embodiment of the invention.

## DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

Apparatus and methods are provided to detect whether a device is in contact with skin and to determine the pigmentation level of skin. To determine skin contact, the apparatus and methods utilize light emitted onto the skin and detectors and sensors to measure spectral remission from the skin. The apparatus and methods further compare the obtained remission measurement with known skin spectral remission values. The sensors may be calibrated to allow measurements of absolute remission to be converted to fractional remission values. Measurements of skin pigmentation levels are compared to known base-line levels to determine appropriate treatment parameters.

The apparatus and methods may be used by incorporating the apparatus into the device itself, such as into a light based dermatologic or cosmetic treatment device, or the apparatus may be remote from and remotely control the treatment device.

The apparatus includes one or more light sources and one or more detectors. The one or more light sources may be a single broad band source or multiple single spectrum sources. The one or more detectors may be a single broad band detector or multiple detectors each sensitive to a unique optical band. In one embodiment, a single broad band source is utilized together with multiple detectors. In a second embodiment, multiple single spectrum sources are utilized together with a single broad band detector. In a third embodiment, multiple single spectrum sources are utilized together with multiple detectors each sensitive to a unique optical band.

The apparatus and methods of the present invention include use of measured and calculated values to control operation of the device, for instance, to allow the device to turn on or to prevent the device from turning on, or, alternatively, to adjust emission levels of the device to correspond to the treatment appropriate with the measured and calculated values.

In alternative embodiments of the present invention, the apparatus and methods include temperature sensors that compensate for temperature fluctuations.

In one embodiment of the present invention, the device is incorporated within a dermatological treatment device which is self-contained, hand-held, and battery powered. A skin sensor in this embodiment compensates for temperature fluctuations and inhibits emission of the treatment device unless the presence of skin is detected and further inhibits emission unless the pigmentation level of the skin is less than a predetermined threshold level. In an alternative embodiment, the emission level is adjustable in accordance with the determined pigmentation level of the skin.

Referring now to FIGS. 1-3, an embodiment of the present invention is shown in various views. In the illustrated embodiment, the present invention is contained within

a housing 806A-B which, depending upon the implementation, can be either a housing separate from a treatment device or the housing of the treatment device itself. When used, a measurement aperture 814 is held against the surface of skin 813 or any other material that is suitably flat over the area of the measurement aperture. The user turns on the electronics by pressing switch 808, or any other suitable arrangement, to begin the measurement. The switch 808 is actuated by pressing button 806C. Contained within housing 806A-B are light sources 801 which emit light into a lightguide, or mixer 805. Each of light sources 801 emits a distinct and unique wavelength band, such as LED's operating in, for example, blue, green, yellow, red and infrared bands, as shown in Table I, below:

LED colors used in Skin Sensor	Peak Emission Wavelength(nm)	Spectral Line Half-Width(nm)
LED GREEN	574	15
LED SUPER RED	639	20
LED YELLOW	588	15
LED BLUE	468	25
LED INFRARED(IR)	940	50

Mixer 805 is an optically transparent material made from acrylic plastic, quartz, sapphire, glass or other suitable material for transporting light having a proximal surface nearest the sources 801 and distal surface furthest from sources 801. The walls of mixer 805 are sufficiently smooth to reduce scattering of light and to ensure that substantially all the light incident on the side walls undergoes total internal reflection. In some embodiments, mixer 805 is comprised of a material whose index of refraction is greater than about 1.5. This ensures that substantially all of the light from sources 801 that is incident on the proximal surface of mixer 805 that is not reflected by the proximal surface of mixer 805 will undergo total internal reflection when incident on the side walls of mixer 805. In some alternative embodiments, a hollow light guide can be used. In an embodiment, the length and width of mixer 805 are chosen so that the light transported by mixer 805 is substantially uniform when incident on the distal surface of mixer 805. In some embodiments, a baffle 803, is incorporated into the skin sensor so that light that undergoes Fresnel reflection when incident on the proximal surface of mixer 805 is not reflected into detector 804, since the intensity of that light would not be remitted from the skin or other surface being tested.

Light entering the proximal end of mixer 805 will travel the length of the mixer 805 to the distal end where substantially all of the light leaves the mixer and exits the device through measurement aperture 814.

In some embodiments, some of the light incident on the distal end of mixer 805 can be reflected back towards detector 804 and could contribute a non-significant offset in the measurement. To overcome this, during calibration a measurement into a black surface is made so that the light reflected by this black surface can be measured and then subtracted from subsequent measurements.

In some embodiments, a significant amount of the light that is remitted by the skin may not be collected, and therefore measured, by the device of the present invention. This is because the light incident upon the skin from the device can scatter laterally in the skin, and remit outside the area covered by the aperture of the device. The extent to which such lateral scattering occurs in skin varies with

wavelength, where the scattering of blue light is small compared with the scattering of red and infrared light. In materials other than skin, the extent of such scattering can be greater or less depending upon the properties of those materials. However, such lateral scattering in skin is compensated for in at least some embodiments because the scattering adds a reproducible offset to the measurements. The lateral scattering effect can therefore be adjusted for when comparing the sample to the “known spectral remittance of skin”. This compensation can be used, depending upon the embodiment, both when determining whether the sampled material is skin and also when comparing the sampled material against threshold value(s) for determining pigmentation level.

Light exiting the measurement aperture **814** of the device is incident on the skin **813** or other surface held against the measurement aperture **814** of the device. Light incident on the skin **813** or other surface is either reflected back into the mixer or enters the skin **813** or other surface. Once inside the material being measured, the light undergoes scattering and absorption. A portion of the light entering the skin is remitted by the skin **813** or other material being measured and travels back towards the detector **804** at the proximal end of the mixer. In one embodiment, the detector **804** is a broadband detector, although detector **804** can be replaced in other embodiments by a plurality of detectors, each matched to the wavelength of one the light sources **801**.

In use, each of the sources **801** is turned on sequentially, in turn, and a measurement is made of the intensity of the light remitted by the skin for that source **801** by detector **804**.

In some embodiments, a temperature sensor **802** is located sufficiently near sources **801** and detector **804** so that the temperature of the sources **801** and detector **804** can be measured at nearly the same time as the remission measurement. The temperature sensor **802** can be a thermistor, thermocouple, or other suitable means for sensing the temperature in the vicinity of the sources **801** and detector **804**.

In one embodiment, the device comprises a printed circuit board (PCB) **811** on which the sources **801**, detector **804**, temperature sensor **802**, and a switch **808** are mounted. Also mounted on the PCB **811** are a processor **810**, battery **812**, and other electronics components **809** suitable for powering the light sources **801**, and for interfacing with the temperature sensor **802**, detector **804**, switch **808**, and indicator **807**.

Processor **810** can be a simple 8 bit microcontroller. Common microcontrollers are capable of storing calibration constants and can compute the fraction of light that is remitted, including computing the fraction of light remitted for each light source. Using appropriate programming, once the spectral remission has been calculated, the processor determines whether the spectral remission is within the range indicative of skin. Additionally the processor is programmed to determine the level of pigmentation. One suitable algorithm for determining skin pigmentation is to measure the amount of light remitted at the red wavelength and compare this to a predefined threshold. The predetermined red threshold can vary significantly depending upon the implementation, but in at least some embodiments is set in the range of 20%-40%, before adjusting for the lateral scattering effect discussed above. In some embodiments, the red threshold is set at 28% or lower, while in other embodiments the red threshold is set to 34% or higher. If a scattering loss of approximately 30% is assumed, a 28% threshold setting becomes a 40% real threshold,  $28\%/(1-0.3)=40\%$ .

Other algorithms can be used, for example algorithms considering additional wavelengths, or algorithms including adjustments for temperature or noise. The red wavelength

has been determined to offer advantages over other wavelengths because it has comparatively high remission, and is less affected by variations in temperature. Alternatively, an LED operating at the same wavelength as the treatment device, for example 810 nm, can be used.

Whichever algorithm is programmed into the processor **810**, the processor determines (1) whether the spectral remission is suitably similar to skin, and (2) whether the pigmentation is below that which would present a hazard to the user undergoing treatment. The result is displayed by indicator **807**. The display **807** can be a simple “go/no go” display or, alternatively, can display the results of both the skin test, i.e., skin or not skin, and the pigmentation level.

Depending upon the results of the various tests, the present invention can communicate with the treatment device to either permit or prevent emissions from the treatment device. Alternatively, the maximum fluence permitted to be emitted by the treatment device can be adjusted in accordance with the pigmentation level determined by the device of the present invention. If the device of the present invention is integrated into the treatment device, such adjustment can be implemented into the processor used to control emissions. If the device of the present invention is separate from the treatment device, the two can communicate by any suitable means, such as a wired or wireless link. Wireless links include infrared, RF, and so on, and can use any suitable protocol.

In some embodiments, the processor **810** is also programmed to correct for temperature variations at the sources **801** and detector **804**. In an embodiment, the correction factor for each temperature is stored in a lookup table. Alternatively, the temperature correction factor can be implemented algorithmically. In some embodiments, temperature compensation is provided both for LED power and phototransistor sensitivity, and the LED's and phototransistor can have opposite sensitivities so that the net sensitivity can be either positive or negative depending on whether the LED sensitivity dominates the detector sensitivity, or vice-versa. Depending on the wavelength, both positive and negative adjustments can be applied. In an embodiment, the correction is linear with temperatures over the temperature range that the detection device is expected to operate.

FIG. 4 illustrates in schematic diagram of the circuit of an embodiment of the invention, in which a processor **400** sequentially pulses LEDs **405A-405E**, each of which is a different wavelength band, with appropriate signal conditioning **410**. The LED's illuminate the material being testing, generally skin, and the remittance from the skin for each wavelength is detected by photodetector **415**, which sends the information to the processor after appropriate signal conditioning **420**. The processor then determines whether the material being tested is skin, using the algorithms discussed above, and also determines the level of pigmentation as discussed above. Depending upon the result, one of indicators **425** or **430** is energized by the processor through appropriate signal conditioning **435**. The indicators can, depending upon the embodiment, simply be a red or green LED, or can be an alphanumeric display. If the present invention is not integrated into the treatment device, the processor can also communicate with the treatment device using, for example, an infrared transmitter **440** after appropriate signal conditioning **445**. A temperature sensor **450** also provides an input to the processor **400** to permit the processor to compensate for temperature-induced performance variations in the LEDs and photodetector.

In the event that the device determines that the skin being tested is too heavily pigmented for safe use of the maximum

fluence available from the associated treatment device, the present invention includes inhibiting the emissions of the treatment device. Such inhibition can take the form of preventing emissions above a predetermined threshold, or can proportionately degrade the fluence of one or more output levels normally available from the treatment device. For example, if a treatment device offers three fluence levels, but the pigmentation is too high for safe operation at the two top levels, in some embodiments the top two levels are simply inhibited. In other embodiments, the top two, or even all three, levels can be proportionately diminished, or shifted, to ensure safe operation. In still other embodiments, particularly for devices where the detection device and treatment device are integrated, the pigmentation is tested before each emission, and the fluence is adjusted to be appropriate for that level of pigmentation, or at least not to exceed a safe threshold for that level of pigmentation.

As stated above, the optical sensor apparatus may be integrated into various dermatologic and cosmetic devices. For purposes of illustration only, and without limited the scope of the present invention, the device may be integrated into the dermatologic devices shown in U.S. Pat. Nos. 7,452,356, 7,250,045, and 7,118,563, which are hereby incorporated by reference into their entirety. The optical sensor apparatus is incorporated into these devices by placing the sensors/detectors around the output window of the device. Alternatively, optical fibers may be used to deliver light from the sensors to the area of the output window when the optical sensors are mounted behind the output window. In another embodiment, remission light is returned to the detectors through the mixer.

Having fully described a preferred embodiment of the invention and various alternatives, those skilled in the art will recognize, given the teachings herein, that numerous alternatives and equivalents exist which do not depart from the invention. It is therefore intended that the invention not be limited by the foregoing description, but only by the appended claims.

What is claimed is:

1. A dermatological treatment system, comprising:  
 an optical device for analyzing a target surface, the optical device comprising:  
 a housing having a surface contacting portion;  
 one or more light sources provided in the housing and configured to emit light toward a target surface proximate the surface contacting portion;  
 one or more detectors provided in the housing and configured to detect remitted light from the target surface at one or more different wavelengths;  
 control circuitry coupled to the one or more light sources and the one or more detectors, the control circuitry comprising:  
 a processor; and  
 computer instructions stored in non-transitory computer-readable media and programmed to:  
 perform a remittance analysis including analyzing the detected remittance at the one or more different wavelengths to determine at least one of (a) whether the target surface is skin or (b) a pigmentation of the target surface; and  
 a wireless transmitter coupled to the control circuitry, wherein the wireless transmitter wirelessly transmits results of the remittance analysis;  
 a treatment radiation source configured to emit treatment radiation toward a user;

a wireless receiver that receives the results of the remittance analysis transmitted by the wireless transmitter of the optical device; and

a controller configured to control radiation emission by the treatment radiation source based on the results of the remittance analysis received via the wireless receiver.

2. The dermatological treatment system of claim 1 further composing a temperature sensor coupled to the control circuitry.

3. The dermatological treatment system of claim 1 wherein the one or more light sources comprises a single broad band light source, and the one or more detectors comprises a single broad band detector.

4. The dermatological treatment system of claim 1 wherein the one or more light sources comprises multiple light sources, each of the multiple light sources emitting light at a different wavelength, and the one or more detectors comprises a single broad band detector.

5. The dermatological treatment system claim 1 wherein the one or more light sources comprises multiple light sources, each of the multiple light sources emitting light at a different wavelength, and the one or more detectors comprises multiple detectors, each of the multiple detectors detecting a different wavelength.

6. The dermatological treatment system of claim 1 wherein the one or more light sources comprises one or more LEDs selected from green, red, super red, yellow, blue and infrared LEDs.

7. The dermatological treatment system of claim 1 further comprising an indicator coupled to the control circuitry.

8. The dermatological treatment system of claim 7 wherein the indicator provides an indication to a user based on the remitted light detected by the one or more detectors.

9. A dermatologic treatment device comprising:

a housing;

a treatment radiation source within the housing capable of being activated to emit treatment radiation toward a user;

an optical control system mounted within the housing, the optical control system comprising:

one or more light sources configured to emit light toward a target surface;

a first detector configured to detect remitted light from the target surface at a first wavelength; and

control circuitry including a processor and computer instructions stored in a computer-readable medium and programmed to:

determine both (a) whether the target surface is skin and (b) the pigmentation of the target surface using the detected remittance at the first wavelength as detected by the first detector, and

control radiation emission by the treatment radiation source of the dermatologic treatment device based on (a) the determination of whether the target surface is skin and (b) the determined pigmentation of the target surface,

wherein the computer instructions are programmed with:

a first algorithm that determines whether the target surface is skin based on the detected remittance at multiple different wavelengths, including the detected remittance at the first wavelength as detected by the first detector, and

a second algorithm that determines the pigmentation of the target surface based on the detected remittance a subset of the multiple different

9

wavelengths, the subset including the detected remittance at the first wavelength as detected by the first detector,

such that detected remittance at the first wavelength as detected by the first detector is used for both the determination of whether the target surface is skin and the determination of the pigmentation of the target surface.

10. The dermatologic treatment device of claim 9 wherein the optical control system further comprises a temperature sensor coupled to the control circuitry.

11. The dermatologic treatment device of claim 9 wherein the one or more light sources comprises a single broad band light source, and the optical control system includes the first detector and at least one further detector.

12. The dermatologic treatment device of claim 9 wherein the one or more light sources comprises multiple light sources, each of the multiple light sources emitting light at a different wavelength, and the first detector comprises a single broad band detector.

13. The dermatologic treatment device of claim 9 wherein the one or more light sources comprises multiple light sources, each of the multiple light sources emitting light at a different wavelength, and the optical control system includes multiple detectors, including the first detector and at least one further detector, each of the multiple detectors detecting a different wavelength.

14. The dermatologic treatment device of claim 9 wherein the one or more light sources comprise one or more LEDs selected from green, red, super red, yellow, blue and infrared LEDs.

15. The dermatologic treatment device of claim 9 further comprising an indicator coupled to the control circuitry.

16. The dermatologic treatment device of claim 15 wherein the indicator provides an indication to a user based on the remitted light detected by the one or more detectors.

17. The optical device of claim 1 wherein the one or more light sources comprises a single broad band light source, and the one or more detectors comprises multiple detectors, each configured to detect a different optical band.

18. A method for analyzing a target surface using an optical device, the method comprising:

- operating an optical device comprising:
  - a housing having a surface contacting portion;
  - one or more light sources provided in the housing and configured to emit light toward a target surface proximate the surface contacting portion;

10

a first detector provided in the housing and configured to detect remitted light from the target surface at a first wavelength; and

control circuitry coupled to the one or more light sources and the first detector; and

determining, by the control circuitry, whether the target surface is skin based on the detected remittance at the multiple different wavelengths, including the detected remittance at the first wavelength as detected by the first detector, and

determining, by the control circuitry, a pigmentation of the target surface based on the detected remittance at a subset of the multiple different wavelengths, the subset including the detected remittance at the first wavelength as detected by the first detector,

such that such that the detected remittance at the first wavelength as detected by the first detector is used for determining both (a) whether the target surface is skin and (b) the pigmentation of the target surface, and

controlling, by the control circuitry, at least one aspect of radiation emission by a dermatologic treatment source of a dermatologic treatment device based on (a) the determination of whether the target surface is skin and (b) the determined pigmentation of the target surface.

19. The method of claim 18, wherein the subset of the multiple different wavelengths is a single wavelength.

20. The optical device of claim 1, wherein controlling radiation emission by the treatment radiation source based on the results of the remittance analysis comprises preventing radiation emission by the treatment radiation source based on the results of the remittance analysis.

21. The optical device of claim 1, wherein controlling radiation emission by the treatment radiation source based on the results of the remittance analysis comprises controlling an emission level emitted by the treatment radiation source based on the results of the remittance analysis.

22. The method of claim 18, wherein the optical control system includes multiple detectors including the first detector and at least one further detector, wherein each of the multiple detectors is configured to detect a different wavelength.

23. The method of claim 18, wherein the first detector comprises a broad band detector.

\* \* \* \* \*

专利名称(译)	光学传感器和用于识别皮肤的存在和皮肤色素沉着的方法		
公开(公告)号	<a href="#">US9687671</a>	公开(公告)日	2017-06-27
申请号	US12/430730	申请日	2009-04-27
[标]申请(专利权)人(译)	TRIA BEAUTY		
申请(专利权)人(译)	TRIA BEAUTY, INC.		
[标]发明人	WECKWERTH MARK V ISLAND TOBIN C GROVE ROBERT E		
发明人	WECKWERTH, MARK V. ISLAND, TOBIN C. GROVE, ROBERT E.		
IPC分类号	A61N5/06 A61B5/00 A61B90/00 A61B17/00		
CPC分类号	A61N5/0616 A61B5/0059 A61B5/441 A61B5/6843 A61B2017/00057 A61B2090/065 A61B2562/0238 A61N2005/0652 A61N2005/0659 A61N2005/0662		
优先权	61/048154 2008-04-25 US		
其他公开文献	US20090270848A1		
外部链接	<a href="#">Espacenet</a>	<a href="#">USPTO</a>	

摘要(译)

提供装置和方法以控制装置，例如发光皮肤病学或美容治疗装置，并确保装置与皮肤接触，同时还确定皮肤的色素沉着水平。一个或多个光源接触皮肤，并且一个或多个检测器测量来自皮肤的光谱消退。将获得的缓解测量结果与已知的皮肤光谱缓解值进行比较，并且校准允许将绝对缓解的测量结果转换为分数缓解值。将皮肤色素沉着水平与已知的基线水平进行比较，以确定和控制适当的治疗参数。温度传感器可以校正温度变化。该装置可以或可以不包含在治疗装置中。

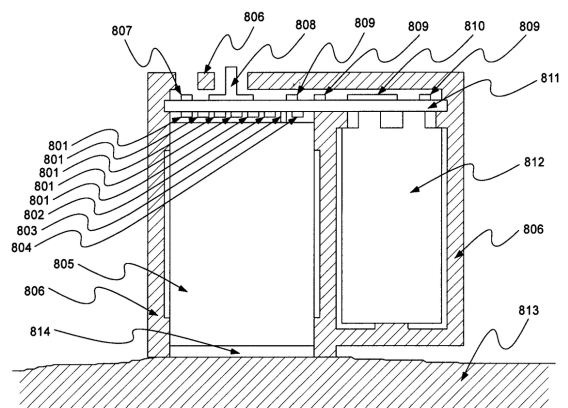


Fig. 1