

US006980112B2

(12) **United States Patent**
Nee

(10) **Patent No.:** **US 6,980,112 B2**
(45) **Date of Patent:** **Dec. 27, 2005**

- (54) **EMERGENCY CALL PATIENT LOCATING SYSTEM FOR IMPLANTED AUTOMATIC DEFIBRILLATORS**
- (75) Inventor: **Wright Jacken Nee**, Rochester, MN (US)
- (73) Assignee: **International Business Machines Corporation**, Armonk, NY (US)
- (*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 27 days.

6,045,513 A	4/2000	Stone et al.	600/508
6,112,116 A	8/2000	Fischell et al.	600/517
6,263,245 B1 *	7/2001	Snell	607/60
6,272,379 B1	8/2001	Fischell et al.	607/5
6,275,734 B1	8/2001	McClure et al.	607/27
6,280,409 B1	8/2001	Stone et al.	604/67
6,292,698 B1 *	9/2001	Duffin et al.	607/32
6,443,890 B1	9/2002	Schulze et al.	600/300
6,468,219 B1 *	10/2002	Njemanze	600/454
6,478,736 B1	11/2002	Mault	600/300
6,553,262 B1 *	4/2003	Lang et al.	607/32
6,553,263 B1 *	4/2003	Meadows et al.	607/61
6,564,104 B2 *	5/2003	Nelson et al.	607/60
6,579,231 B1	6/2003	Phipps	600/300
2002/0109600 A1	8/2002	Mault	340/573.1

(21) Appl. No.: **10/041,937**

(22) Filed: **Jan. 8, 2002**

(65) **Prior Publication Data**

US 2003/0128121 A1 Jul. 10, 2003

(51) **Int. Cl.**⁷ **G08B 23/00**

(52) **U.S. Cl.** **340/573.1; 340/539.12; 600/508**

(58) **Field of Search** **340/573.1, 539.12, 340/539.16, 539.13; 607/27, 57, 30; 128/843, 128/899; 600/508, 517, 500; 455/404.1; 379/40**

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,927,663 A	12/1975	Rusell et al.	128/2.06
4,432,375 A	2/1984	Angel et al.	128/705
4,523,595 A	6/1985	Zibell	128/419
4,830,006 A	5/1989	Haluska et al.	128/419
4,890,621 A	1/1990	Hakky	128/635
5,411,537 A *	5/1995	Munshi et al.	607/33
5,673,692 A	10/1997	Schulze et al.	128/633
5,674,249 A	10/1997	De Coriolis et al.	607/5
5,720,770 A *	2/1998	Nappholz et al.	607/30
5,772,585 A	6/1998	Lavin et al.	600/300

OTHER PUBLICATIONS

http://www.skyaid.org/LifeWatch/life_watch.htm, accessed on Sep. 19, 2001, LifeWatch: The wristwatch that can save a life, updated Sep. 6, 2001, pp. 1-5.

Implant tells your doctor how you're doing, by Lauran Neergaard, Associated Press.

http://seattlep-i.nwsourc.com/national/42402_health12.shtml, accessed on Oct. 23, 2001, FDA approves new pacemaker that can monitor patients, Oct. 12, 2001, pp. 1-3.

(Continued)



Primary Examiner—Phung T. Nguyen

(74) *Attorney, Agent, or Firm*—Patterson & Sheridan LLP

(57) **ABSTRACT**

Methods and systems for placing a distress call in response to the operation of an implanted device. The implanted device may be any of a plurality of medical devices capable of monitoring and/or regulating an organ. When threshold conditions are reached, a distress signal transmitted by the implanted device activates an external communications system. The external communications system then places a distress call, which may be responded to by the appropriate medical personnel.

22 Claims, 4 Drawing Sheets

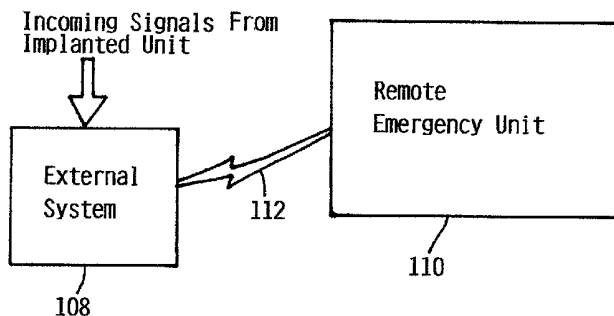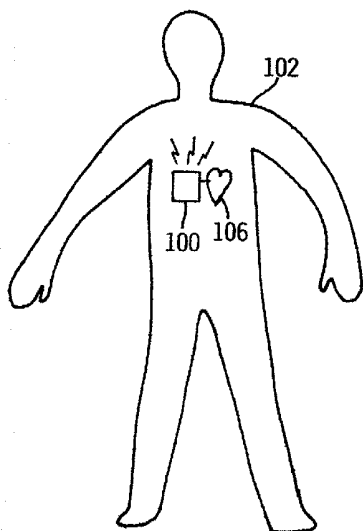

OTHER PUBLICATIONS

http://www.washingtonpost.com/wp-srv/aponline/20011012/aponine035439_000.htm, accessed on Oct. 23, 2001, FDA Approves High Tech Pacemaker, dated Oct. 12, 2001, pp. 1-3.

John Lortz and Susan Leavitt, "What is Bluetooth? We Explain the Newest Short-Range Connectivity Technology," 2002, Sandhill Publishing, Smart Computing Learning Series Wireless Computing, pp 72-74.

* cited by examiner

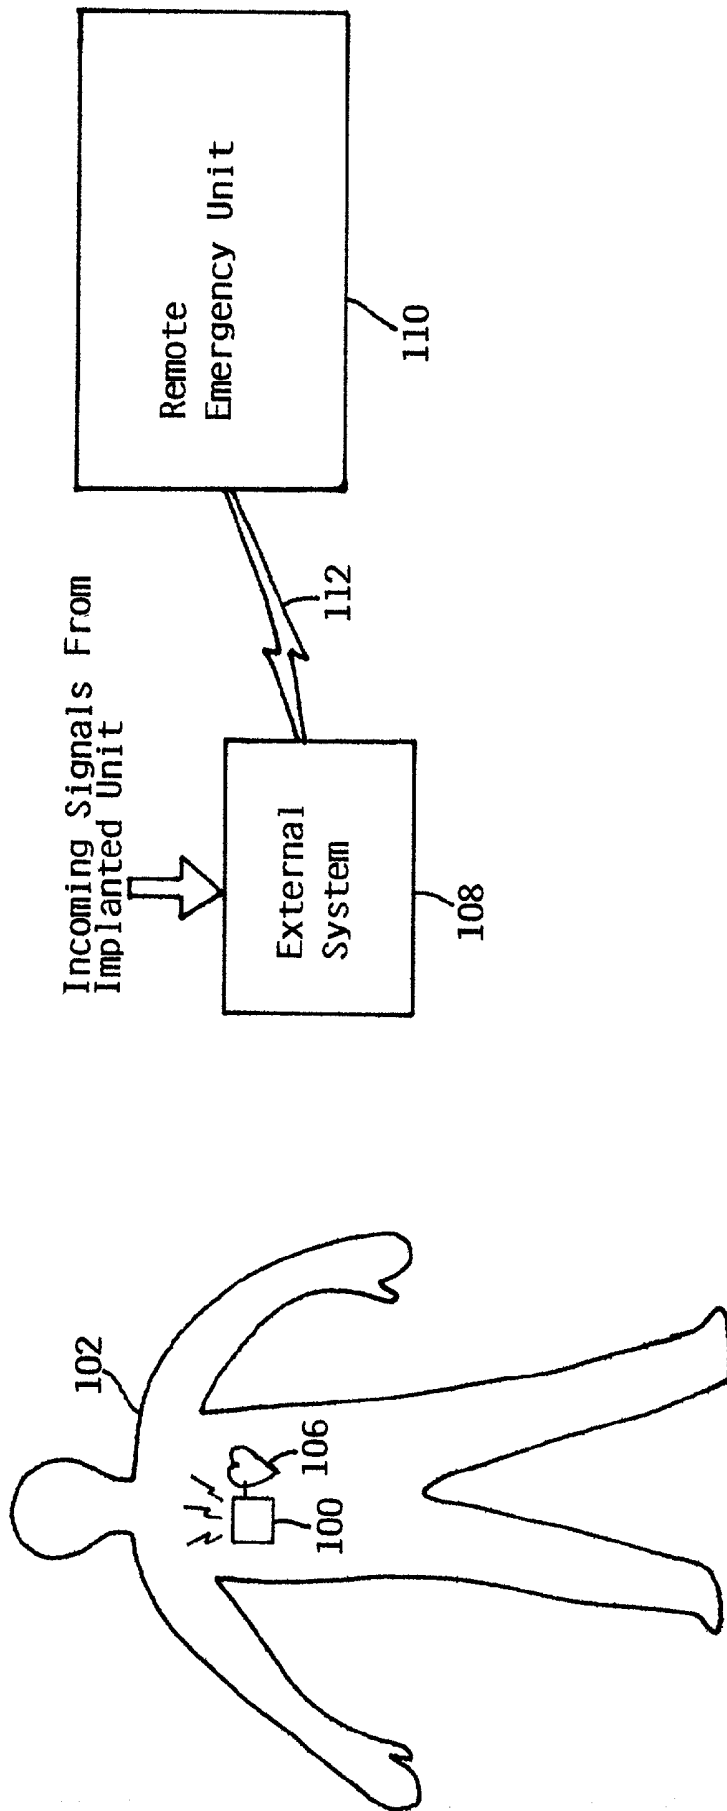


FIG. 1

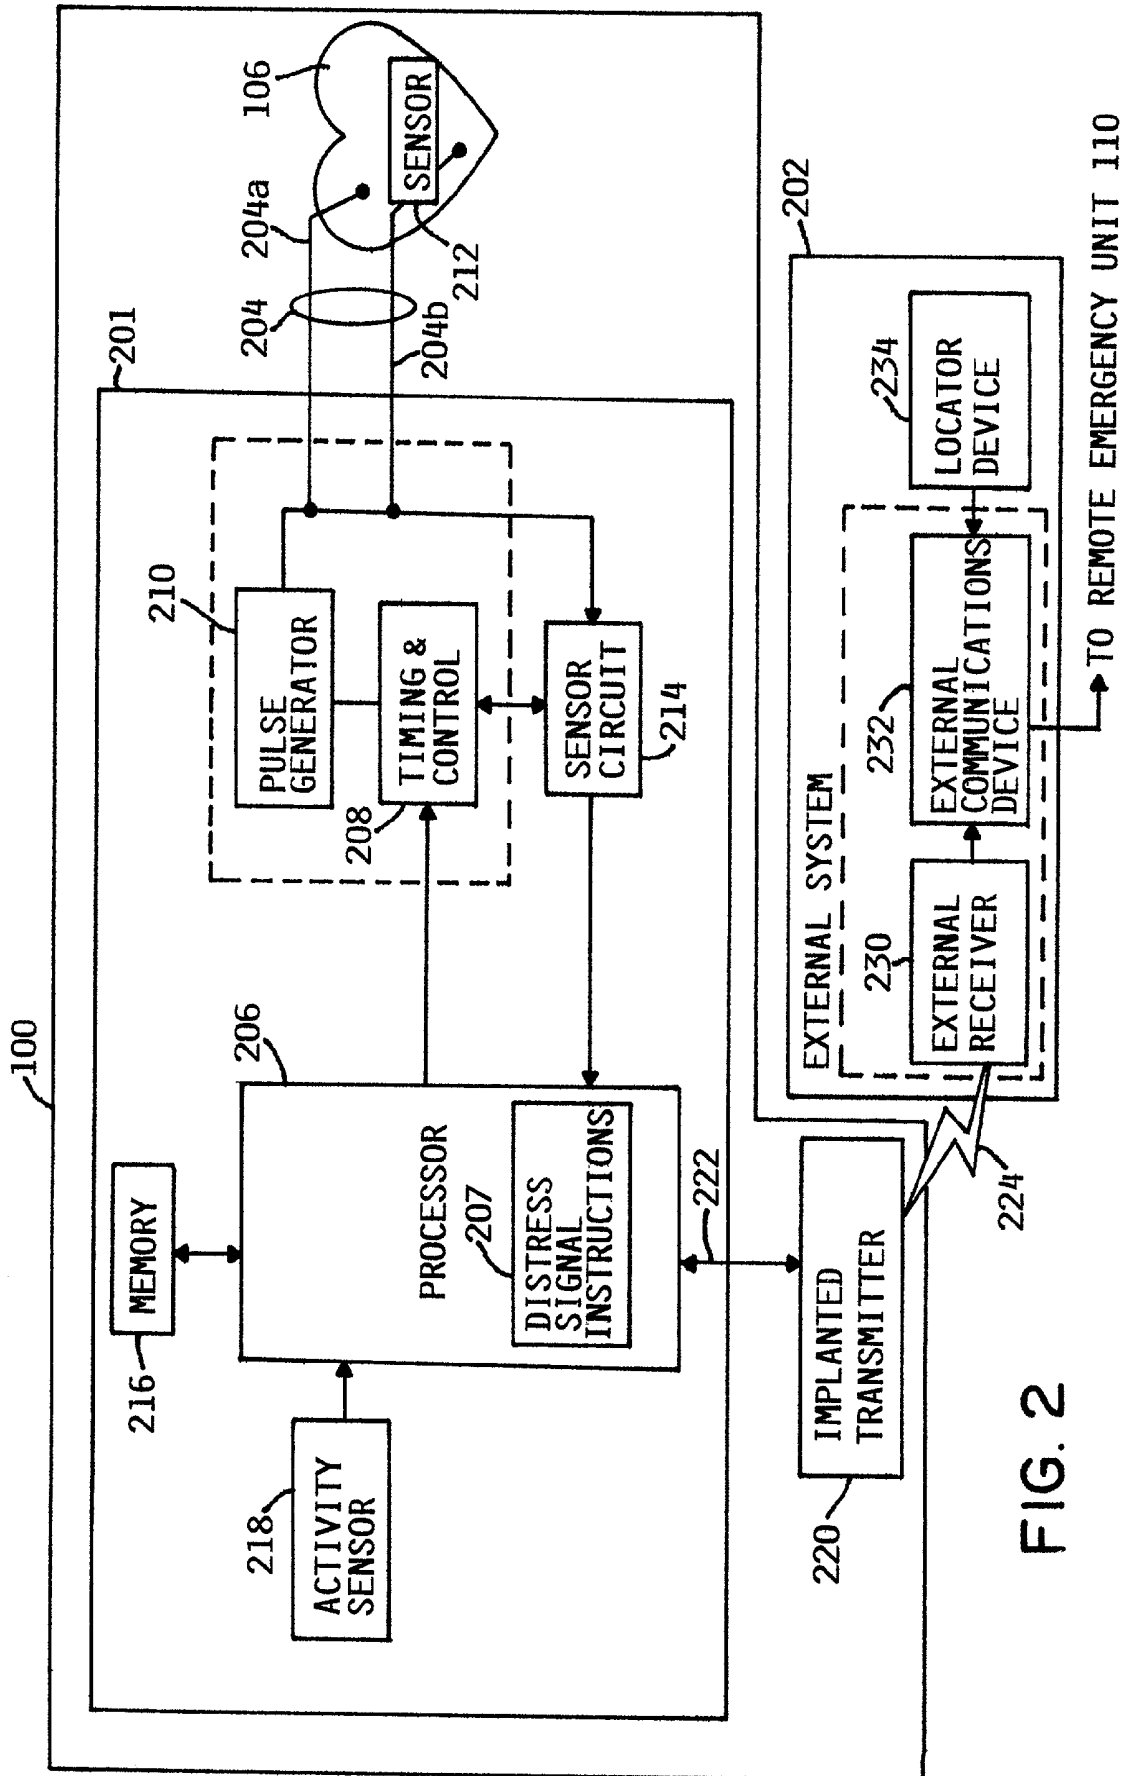


FIG. 2

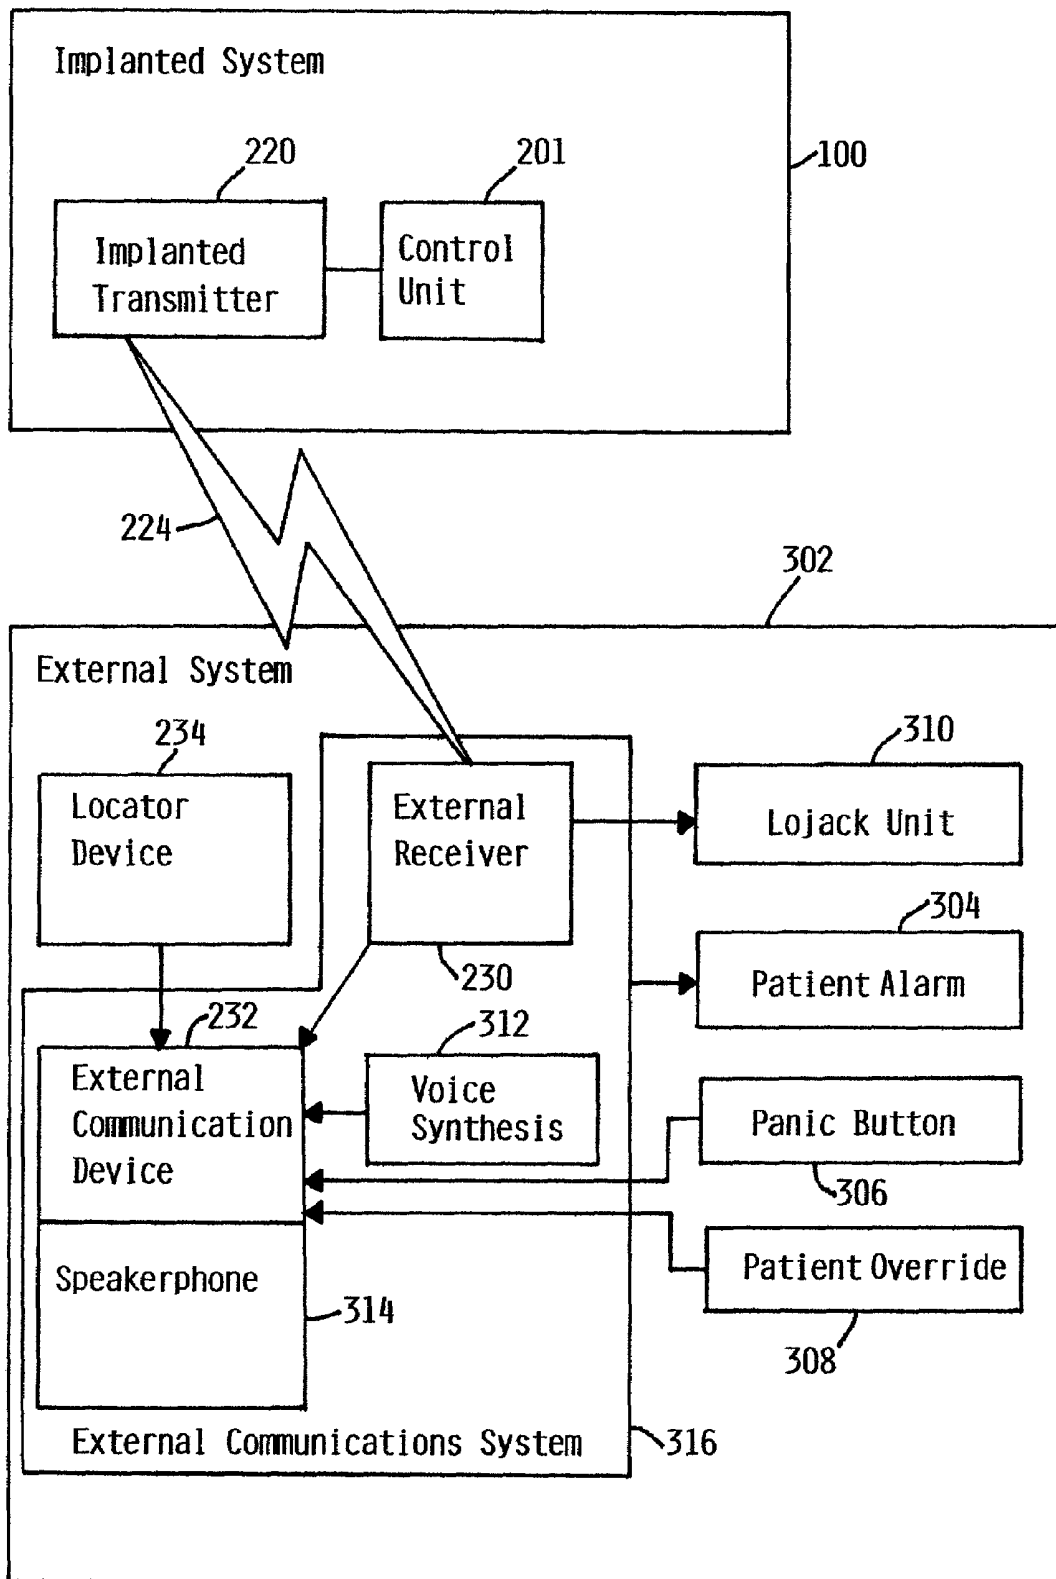


FIG. 3

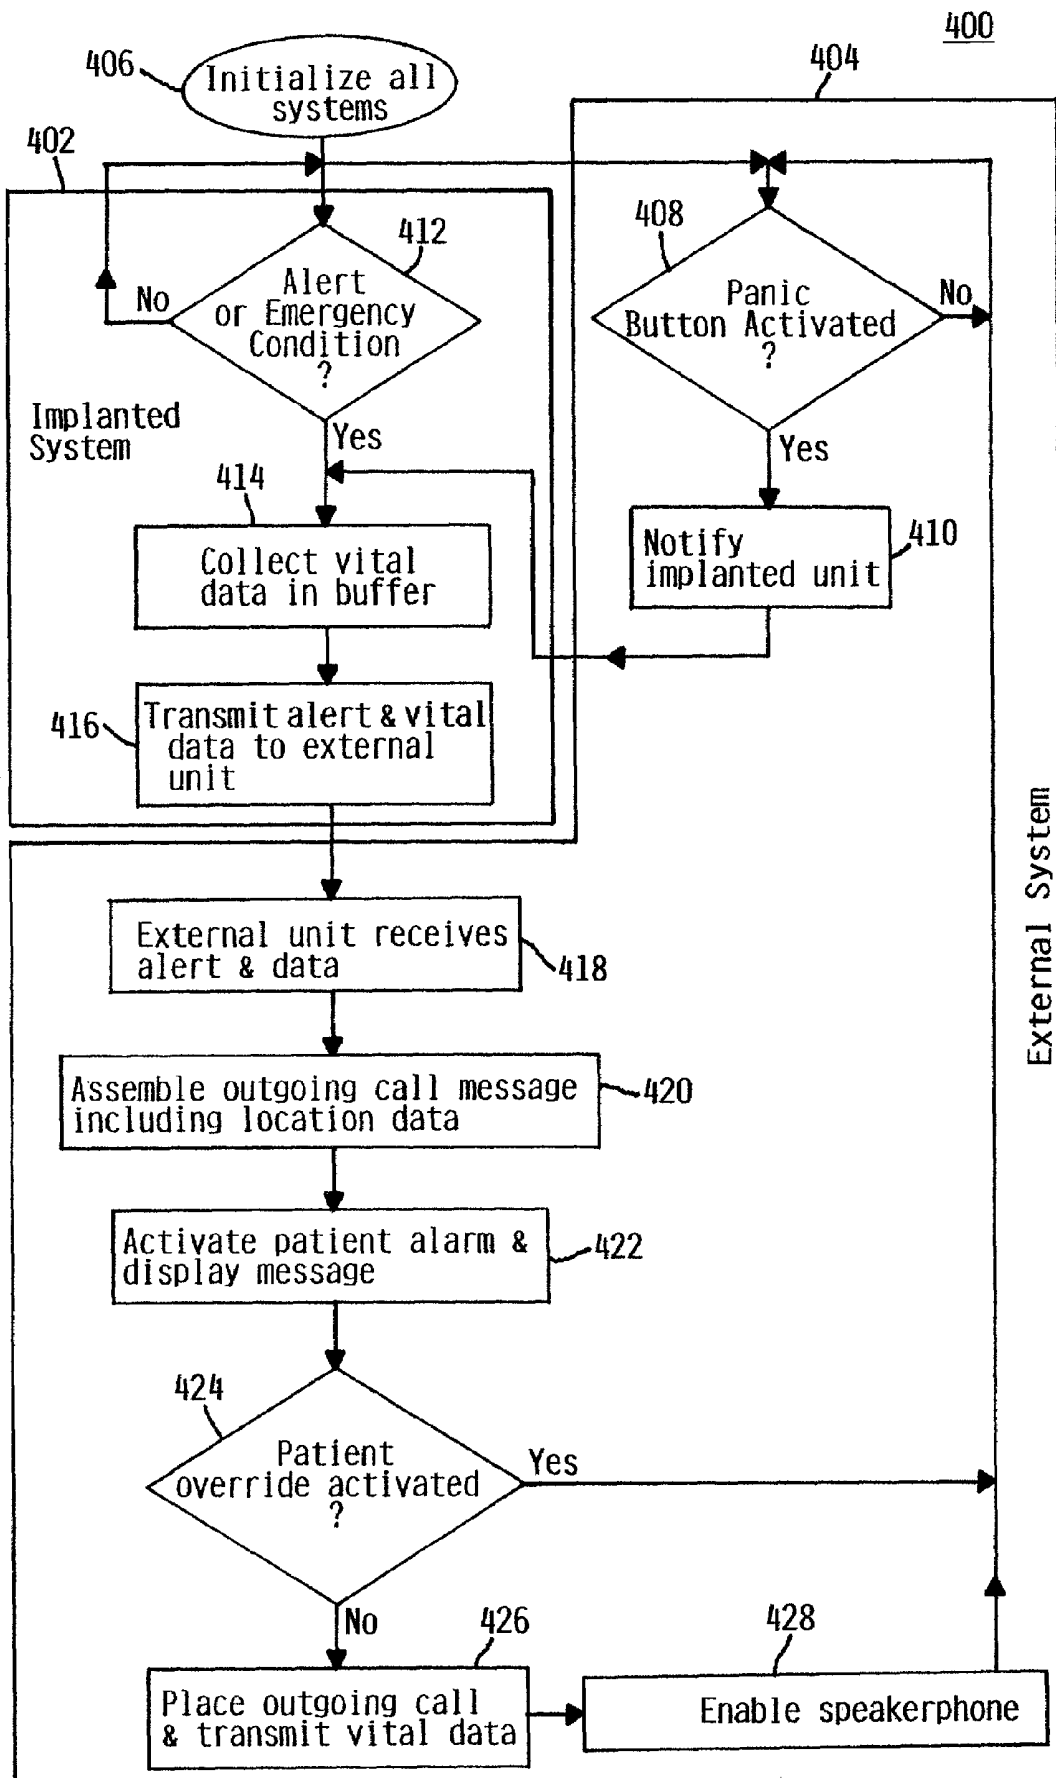


FIG. 4

1

EMERGENCY CALL PATIENT LOCATING SYSTEM FOR IMPLANTED AUTOMATIC DEFIBRILLATORS

BACKGROUND OF THE INVENTION

1. Field of the Invention

The present invention generally relates to medical devices. More particularly, the invention relates to methods and systems for transmitting a distress call in response to a signal from an implanted unit.

2. Description of the Related Art

Implantable medical devices, such as implantable cardiac devices, are devices which are implanted in the body of a patient and are capable of monitoring the function of a patient's organ, such as their heart or brain, and are further configured in some instances to be able to deliver therapeutic electrical stimulation to the patient's organ.

Implantable cardiac devices, such as pacemakers and implantable cardioverter defibrillators (ICDs), are very commonly used implantable mechanical devices and are used to treat various heart conditions. These types of implantable cardiac devices typically have one or more leads that are positioned adjacent the walls of the heart and a control unit which receives signals indicative of the functioning of the heart. The control unit induces the delivery of therapeutic electrical stimulation to the walls of the heart via the leads in response to sensed heart conditions. Generally, the control unit incorporates a processor that is capable of recognizing and discerning particular heart irregularities based upon the signals that the processor receives. The implanted leads act as a sensor that delivers an intracardial electrogram (IEGM) to the processor, which provides the processor with a signal that is indicative of the heart function. Hence, the processors of these types of implantable cardiac devices continuously receive an IEGM signal that allows the processor to determine whether therapeutic stimulation of the heart is needed to regulate the heart function.

Despite the general effectiveness of implanted devices, patients using these devices often require additional medical attention. Such a need may arise, for example, in the event that the implanted device fails or malfunctions. Often, the patient may be physically unable to call for help due to pain, confusion, loss of consciousness, etc.

Recently, systems capable of real-time monitoring have been made available. One such system is the Home Monitoring System available from Biotronik, Inc. Real-time monitoring systems download information from a pacemaker and, ultimately, transmit the downloaded information to a physician. However, the operation of such real-time monitoring systems is not dependent upon, or triggered by, the condition of the patient being monitored. Rather, the downloading and transmitting of information occurs at a preset interval. A determination that the patient requires medical attention can only be made by the doctor after receiving and reviewing the downloaded information. Because the downloaded information does not explicitly notify the physician of a possible emergency condition, the physician is not motivated to take immediate emergency action. As a result, critical time may pass between the time the information is made available for review and the time that the information is actually reviewed. Further, existing real-time monitoring systems are limited to use with pacemakers and are not used in conjunction with other implanted devices, such as implanted defibrillators.

2

Therefore, there is a need for a method and system of enhancing the utility of implanted devices where medical attention may be required.

SUMMARY OF THE INVENTION

The present invention generally provides methods and systems for placing a distress call in response to the operation of an implanted device.

One embodiment provides a method for selectively placing a distress call in response to activity of an implanted medical device. The method comprises receiving a wireless signal from the implanted medical device and transmitting the distress call to a remote location in response to receiving the wireless signal.

Another embodiment provides a system for selectively placing a distress call. The system comprises a wireless external receiver configured to receive a wireless signal from an implanted medical device; and an external communications device connected to the wireless external receiver. The external communications device is configured to transmit a distress call to a remote location in response to receiving input from the wireless external receiver.

Still another embodiment provides an implantable medical device comprising an organ monitoring device configured to monitor activity of an organ; and a wireless transmitter in communication with the organ monitoring device. The wireless transmitter is configured to selectively transmit a wireless distress signal in response to predetermined activity of the organ.

BRIEF DESCRIPTION OF THE DRAWINGS

So that the manner in which the above recited features of the present invention are attained and can be understood in detail, a more particular description of the invention, briefly summarized above, may be had by reference to the embodiments thereof which are illustrated in the appended drawings.

It is to be noted, however, that the appended drawings illustrate only typical embodiments of this invention and are therefore not to be considered limiting of its scope, for the invention may admit to other equally effective embodiments.

FIG. 1 is a diagram of an implanted system configured to cause an external system to place a distress call.

FIG. 2 is a block diagram of one embodiment of an implanted unit in communication with an external system.

FIG. 3 is a block diagram of another embodiment of an external system.

FIG. 4 is a flow diagram illustrating the operation of the implanted system and the external system.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

The present invention generally provides methods and systems for placing a distress call in response to the operation of an implanted device. The implanted device may be any of a plurality of medical devices capable of monitoring and/or regulating an organ. When threshold conditions are reached, a distress signal transmitted by the implanted device activates an external communications system. The external communications system then places a distress call, which may be responded to by the appropriate medical personnel.

Some or all aspects of the invention may be implemented as a program product for use with a computer system such as, for example, an implanted system **100** and/or external system **108**, both shown in FIG. **1**. The program(s) of the program product defines functions of the embodiments (including the methods described below) and can be contained on a variety of signal-bearing media. Illustrative signal-bearing media include, but are not limited to: (i) information permanently stored on non-writable storage media (e.g., read-only memory devices within a computer such as CD-ROM disks readable by a CD-ROM drive); (ii) alterable information stored on writable storage media (e.g., floppy disks within a diskette drive or hard-disk drive); or (iii) information conveyed to a computer by a communications medium, such as through a computer or telephone network, including wireless communications. The latter embodiment specifically includes information downloaded from the Internet and other networks. Such signal-bearing media, when carrying computer-readable instructions that direct the functions of the present invention, represent embodiments of the present invention.

In addition, various programs/instructions described hereinafter may be identified based upon the application for which they are implemented in a specific embodiment of the invention. However, it should be appreciated that any particular program/instructions nomenclature that follows is used merely for convenience, and thus the invention should not be limited to use solely in any specific application identified an/or implied by such nomenclature.

While functions of the invention may be implemented in software, the same functions may also be implemented in hardware. For example, hardwired embedded controllers and Application Specific Integrated Circuits (ASIC) may be used.

Reference will now be made the drawings wherein like numerals refer to like parts throughout. Referring to FIG. **1**, a human subject (also referred to herein as the "patient") **102** is shown with an implantable medical device system **100** (also referred to herein as the "the system **100**" and "the implantable system **100**"). The system **100** is adapted to be implanted in the human subject **102** in a well-known manner. The system **100** can be comprised of any implantable device including a pacemaker or an implantable cardioverter defibrillator (ICD) or any implantable device incorporating the functionality of both a pacemaker and an ICD. In the illustrated embodiment, the system **100** comprises an implantable cardiac device and, as such, is shown in connection with a heart **106**. While embodiments are discussed in connection with an implantable cardiac device, it will be appreciated from the following discussion that any implantable device that measures the intrinsic activity of one of the patient's organs are contemplated as embodiments of the invention. Further, the particular implanted system may or may not deliver signals to the organ being monitored for purposes of regulating a desired operation of the organ. It is further contemplated that the implanted system **100** not be limited to monitoring/regulating an organ. Accordingly, other devices within the scope of the invention may include neural devices for providing therapeutic stimulation to portions of the brain and devices that monitor organ activity such as ECG monitors, brain-wave monitors, glucose monitors and other types of monitors known in the art.

In addition to monitoring and regulating the operation of the heart **106**, the system **100** is configured to selectively transmit signals to an external system **108**. In one embodiment, the transmitted signals are distress signals indicating cardiac failure or some other emergency condition. The

signals may be transmitted, for example, at each instance the system **100** detects abnormal operation of the heart **106**. Alternatively, the distress signals may be transmitted to the external system **108** only after the system **100** has attempted to stabilize the heart **106** (such as by providing electrical signals to the heart **106** via a pulse generator) a threshold number of times within a predetermined time period. Further, the distress signals may be transmitted to the external system even in cases where the heart **106** is operating normally. For example, the power level of the system may be dangerously low. The low battery power may trigger the distress signal. In other cases, it may be desirable to anticipate an imminent low battery power situation and proactively trigger the distress signal to notify the patient **102** and/or an emergency unit **110** (described below).

In one embodiment, both the implanted system **100** and the external system **108** are configured with short range communications devices capable of communicating with one another. As such, successful communications between the implanted system **100** and external system **108** depend on their relative close proximity. As defined herein, "close proximity" means any distance at which the implanted system **100** and external system **108** are capable of communicating with one another. Persons skilled in the art will recognize that a particular effective distance is dependent upon the technical specifications (e.g., transmission power, signal strength, susceptibility to interference, etc.) of the implanted system **100** and the external system **108**. Further, the effective distance between the implanted system **100** and external system **108** may be increased by the provision of external relay devices capable of augmenting or boosting the transmission signal from the implanted device **100**.

In general, the external system **108** is any device configured to transmit a distress call to a remote emergency unit **110**, in response to the distress signal(s) received from the system **100**. In one embodiment, the external system **108** is a mobile telephone (e.g., cell phone) adapted to process the distress signal(s) received from the system **100**. A distress call may then be placed to the remote emergency unit **110** via a network **112**. The network **112** may be a telephone network, a broadband Internet network or any other type of network, according to the particular technology implemented in the external system **108**.

The remote emergency unit **110** may be a hospital, a doctor, an emergency unit dispatcher and the like. Alternatively, the remote emergency unit **110** may be an intermediary base station at which the distress call is received and then forwarded to the appropriate medical authority. It is contemplated that, in one embodiment, information provided to the remote emergency unit **110** includes at least the patient's location. In another embodiment, the patient's location may be determined by other techniques, such as by cell triangulation, or be provided by the patient himself. The information may also include the patient's name and the particular condition that caused the distress call to be made (e.g., heart failure). In one embodiment, the information may be used to initiate an automated data retrieval process, whereby the patient's medical records are retrieved (from a database) and made available for viewing by a human operator at the remote emergency unit **110**. Of course, such a data retrieval process may be manually implemented once the information is received by the human operator from the external system **108**.

Referring to FIG. **2**, a functional block diagram of one embodiment of the implantable medical device system **100** and an external system **202** is shown. The external system **202** is representative of one embodiment of the external

system **108** shown in FIG. 1. The system **100** generally comprises a control unit **201** and a plurality of leads **204a** and **204b** (collectively referred to as leads **204**) that are adapted to be positioned within, or proximate to, the chambers of a patient's heart **106**. The control unit **201** includes a processor **206** that provides output signals to a timing and control circuit **208**. Upon receipt of the output signals from the processor **206**, the timing and control circuit **208** induces a pulse generator **210** to produce therapeutic electrical stimulation, e.g., pacing pulses or cardioversion or defibrillation waveforms, that is transported via the leads **204** to stimulate the heart **106**. The exact function of the processor **206** in inducing the delivery of the therapeutic electrical stimulation to the heart is performed in any of a number of well-known manners. For example, in one embodiment, the processor **206** induces pacing pulses to be delivered to the apex of the ventricle of the heart **106**. In another embodiment, the processor **206**, upon sensing the occurrence of a particular tachycardia, induces defibrillation or cardioversion stimuli to be delivered to the heart.

Further, the processor **206** receives input signals from a sensor **212** via a sensor circuit **214**. In one embodiment, the sensor **212** is comprised of an implanted lead **204** that is positioned within one of the chambers of the heart **106** so as to provide an intracardiac electrogram (IEGM) signal to the processor **206**. The IEGM signal is provided to the sensor circuit **214** and may be further processed by the sensor circuit **214** so that the processor **206** receives a filtered IEGM signal that the processor **206** can use in determining whether to deliver therapeutic electrical stimulation to the heart via the timing and control circuit **208** and the pulse generator circuit **210**.

The processor **206** may also receive signals from an activity sensor **218** which allows the processor **206** to modify the delivery of therapeutic electrical stimulation to the heart **106**. The system **100** may provide therapy to the heart **106** according to methods known in the art of implantable cardiac devices.

In the illustrated embodiment, the processor **206** also has an associated memory **216** wherein information, such as IEGM signals, can be stored for subsequent transmission to the external system **202**. Additionally or alternatively, the memory **216** may contain programming executable by the processor **206**. In one embodiment, the memory **216** contains operational data for the implanted system **100**. Operation data may include, for example, the number of electrical charges delivered to the heart **106**, the intensity of the charges, the range of frequencies of charges, etc. The memory **216** may also contain manufacturing information such as a serial number and model number, place of manufacture, date of manufacture, etc.

In operation, one or more of the leads **204** of the sensor **212** are implanted within, or proximate to, the chambers of the heart so as to be able to provide an intracardiac electrogram (IEGM) signal to the processor **206** in a well known manner. This signal is indicative of the functioning of the heart and can be used by the processor **206** to ascertain whether certain criteria have been met that necessitate the delivery of therapeutic electrical stimulation to the heart to regulate heart function. For example, the processor **206** may review the IEGM signal and, upon detecting a ventricular tachycardia or fibrillation, may induce a cardioversion or defibrillation shock to be delivered by the leads **204** in a manner that is known in the art. Similarly, the processor **206** may also use the IEGM signal as a basis for delivering a

pacing pulse to the apex of the ventricle of the heart **106** so as to induce a paced heart activity in a demand pacing regime.

Further, the processor **206** is configured with distress signal instructions **207**. In general, the distress signal instructions **207** are executed in response to signals from the sensor circuit **214**. The distress signal instructions **207** are executed by the processor **206** in order to determine whether to activate an implanted transmitter **220**.

The implanted transmitter **220** maybe any short-range communications device capable of communicating with the external system **202**. In one embodiment, the implanted transmitter **220** is an RF telemetry device. The processor **206** and the implanted transmitter **220** are connected via a communication path **222** which may be a wireless connection or a hardwired connection (e.g., a hardwired bus, an optical connection, etc.). While shown separately from the control unit **201**, the implanted transmitter **220** may be integrated with the control unit **201**.

In general, the external system **202** is configured for receiving, transmitting and determining patient location. As such, the external system **202** comprises an external receiver **230**, an external communications device **232** and a locator device **234**. The external receiver **230** is any communication device capable of wireless communication (via connection **224**) with the implanted transmitter **220**. For example, where the implanted transmitter **220** is an RF telemetry device, the external receiver **230** is also an RF telemetry device. The external receiver **230** is connected to the external communications device **232** and provides information received from the implanted transmitter **220** thereto. The external communications device **232**, in turn, is configured to place a distress call to the remote emergency unit **110** (shown in FIG. 1). The distress call also includes a location of the external system **202**, which is provided to the external communications device **232** by the locator device **234**. Illustrative locator devices include a global positioning system (GPS), a SnapTrack GPS system, etc. As noted above, other techniques for location determination are contemplated, such as cell triangulation.

In one embodiment, the system **100** transmits information to the external system **202** only in the event of emergency condition (e.g., as determined by the distress signal instructions **207**). Alternatively, the system **100** may continuously transmit information (both emergency information and non-emergency information) to the external system **202**. Illustrative non-emergency information includes status information about the organ being monitored by the system **100**. The external system **202** may then take steps to determine whether the information indicates an emergency condition.

The external system **202** is preferably a self-contained unit configured to communicate with the implanted transmitter **220** via the wireless connection **224** and with the remote emergency unit **110** via the network connection **112**. In one embodiment, the external system **202** is a portable unit that the patient **102** may carry on their person (e.g., by means of a shoulder harness, a waist support, a wrist band, a purse, etc.). As such, it is contemplated that the wireless connection **224** is unique and that a particular system **100** is configured for communicating with a particular external system **202**. However, it is also contemplated that the external system **202** is configured to communicate with a plurality of implanted systems **100**, each of which is implanted in a different patient. In such embodiment, the implanted transmitters may be distinguished from one another by the external system **202** by transmitting a unique digital identifier (ID), operating at different frequencies, etc.

Such an implementation is particularly advantageous where a network of external systems **202** is installed, such that each external system **202** is an access point to a communications network (e.g., a telephone communication network, a wide area network (WAN), etc.). So long as the patient **102** is within a range sufficient to maintain the wireless connection **224**, the appropriate information may be exchanged between the implanted system **100** and the external system **202**. In this manner, the patient **102** is freed from the burden of having to carry, or otherwise be concerned with the proximity of, a particular external system **202**.

Referring now to FIG. **3**, another embodiment of an external system **302** is shown. Some of the components of the external system **302** are the same as those of the external system **202** described above with reference to FIG. **2**. Accordingly, like numerals identified like components which have already been described above. The additional or alternative components shown in FIG. **3** include a patient alarm **304**, a panic button **306**, a patient override button **308**, a LoJack unit **310**, a voice synthesizer **312** and a speakerphone **314**.

The patient alarm **304** is an output device configured to indicate that a condition being monitored for has been detected. Illustratively, the alarm may be an audible alarm, a vibrating alarm, a visual alarm (e.g., text or graphical display) or a combination thereof. In the case of a visual alarm, it is contemplated that information may be displayed on a display screen of the external communications device **232**, e.g., on a wireless phone display. The patient alarm **304** is particularly useful for non-emergency conditions in which a distress call is not warranted, but the patient **102** needs to be alerted about a condition (e.g., low battery power of the implanted system **100**).

The panic button **306** allows the patient **102** to manually activate the external system **302**. In one embodiment, when the panic button **306** is pressed, a signal is sent from the external system **302** to the implanted system **100** requesting vital data. Once received by the external system **302**, the vital data may be provided to the remote emergency unit **110** (shown in FIG. **1**). Alternatively or additionally, pressing the panic button **306** may simply initiate a distress call to the remote emergency unit **110** without first requesting information from the implanted system **100**. In another embodiment, the functions of the panic button **306** may be implemented by producing a magnetic field proximate the implanted system **100**. The magnetic field may be generated by a magnet held by the patient **102**. This technique is well known in the art and is used, for example, by the Biotronik Home Monitoring System.

The patient override button **308** allows the patient **102** to intercept and terminate distress calls from the external system **202** to the remote emergency unit **110**. Alternatively or additionally, the patient override button **308** may be configured to allow the patient **102** to deactivate selected portions of the implanted system **100** and/or the external system **302**.

The LoJack unit **310** is a widely known stolen vehicle recovery system. The LoJack unit **310** is equipped with a locator device that transmits a signal to a remote receiving device. The signal, once detected, can be tracked to its source. The LoJack unit **310** may be used to advantage in the present invention as an alternative to, or in conjunction with, the locator device **234**.

Illustratively, the voice synthesizer **312** and the speakerphone **314** are components of an external communications system **316**. The synthesizer **312** is configured to generate a voice message that can be transmitted to the remote emer-

gency unit **110** via the external communications device **232**. In this manner, the voice message may be output to personnel at the remote emergency unit **110** without the need for specialized decoding equipment.

Referring now to FIG. **4**, a method **400** is shown illustrating the operation of the implanted system **100** and the external system **108** (**202**, **302**). The method **400** generally includes a first routine **402** illustrating one embodiment of the operation of the implanted system **100** and a second routine **404** illustrating one embodiment of the operation of the external system **108**.

The method **400** is entered at step **406** where all systems are initialized. Processing for the implanted system **100** then proceeds to step **412** of the first routine **402** while processing for the external system **108** proceeds to step **408** of the second routine **404**. At step **408**, the external system **108** queries whether the panic button **306** has been activated. If so, a request for vital data is transmitted to the implanted system **100** at step **410**. Processing then proceeds to step **414** where the implanted system **100** collects vital data in a buffer (e.g., memory **216**). If not, processing returns to repeat step **408**.

Returning to the implanted system routine **402**, at step **412** the implanted system **100** queries whether an alert or emergency condition has been detected. If not, processing returns to repeat step **412**. If, however, an alert or emergency condition is detected, a distress signal and vital data is transmitted from the implanted system **100** to the external system **108** at step **416**.

The information transmitted at step **416** is received by the external system **108** at step **418**. At step **420**, the external system **108** assembles an outgoing distress call, including location information provided by the locator device **234**. The patient alarm **304** is then activated at step **422**. The external system **108** then queries, at step **424**, whether the patient override button **308** has been pressed. If so, the outgoing distress call is terminated and processing returns to step **408**. If the patient override button **308** has not been pressed, the distress call and vital data are transmitted at step **426**. Optionally, the speakerphone **314** is enabled at step **428** to allow for voice communication between the patient and the remote emergency unit **110**. Once the call is disconnected, the speakerphone may be disabled and the second routine **404** then returns to step **408**. The foregoing processing may continue so long as the implanted system **100** and the external system **108** are functioning.

While the foregoing is directed to embodiments of the present invention, other and further embodiments of the invention may be devised without departing from the basic scope thereof, and the scope thereof is determined by the claims that follow.

What is claimed is:

1. A method for selectively placing a distress call in response to activity of an implanted medical device worn by a human subject, comprising:

receiving a wireless signal from the implanted medical device; and

in response receiving the wireless signal:

generating, by an external voice synthesizer, a voice synthesized message providing information about a nature of the human subject's condition even in the event the human subject wearing the implanted medical device is incapable of verbal communication; and

transmitting, by an external communications device, the distress call in the form of the voice synthesized message to a remote location;

wherein the distress call includes at least one of a serial number and a model number of the implanted medical device.

2. The method of claim 1, wherein the wireless signal is indicative of a medical emergency experienced by the human subject wearing the implanted medical device.

3. The method of claim 1, prior to transmitting, determining that the wireless signal is indicative of a medical emergency being experienced by the human subject wearing the implanted medical device.

4. The method of claim 1, wherein the wireless signal and distress call contain vital data pertaining to an organ being monitored by the implanted medical device.

5. The method of claim 1, wherein the distress call contains location information indicating a location of a device initiating the distress call.

6. The method of claim 1, wherein the implanted medical device comprises one of a pacemaker, an implantable cardioverter defibrillator and a combination thereof.

7. The method of claim 1, wherein the implanted medical device comprises a transmitter configured to transmit the wireless signal and a heart regulating device.

8. A system for selectively placing and handling a distress call, comprising:

an implanted medical device worn by a human subject and comprising a wireless transmitter for issuing a wireless signal;

a wireless external receiver configured to receive the wireless signal from the implanted medical device;

a voice synthesizer configured to generate a voice synthesized message in response to the wireless signal, the voice synthesized message providing information about a nature of the human subject's condition; and an external communications device communicative with the wireless external receiver and configured to transmit a distress call in the form of the voice synthesized message to a remote location in response to receiving input from the wireless external receiver even in the event the human subject wearing the implanted medical device is incapable of verbal communication;

wherein the distress call comprises at least one of the serial number and the model number of the implanted medical device.

9. The system of claim 8, wherein the distress call contains location information indicating a location of the external communications device.

10. The system of claim 8, further comprising a locator device configured to provide location information to the external communications device, wherein the location information is included in the distress call.

11. The system of claim 8, wherein the wireless signal and distress call contain vital data pertaining to an organ being monitored by the implanted medical device.

12. The system of claim 8, wherein the implanted medical device comprises one of a pacemaker, an implantable cardioverter defibrillator and a combination thereof.

13. The system of claim 8, wherein the implanted medical device comprises a transmitter configured to transmit the wireless signal and a heart regulating device.

14. The system of claim 8, wherein the external communications device is configured to determine, prior to transmitting the distress call, that the wireless signal is indicative of a medical emergency being experienced by the human subject wearing the implanted medical device.

15. The method of claim 1, wherein the external communications device is a cell phone.

16. The method of claim 1, further comprising receiving, by the external device, a wireless power status signal from the implanted medical device indicating a low battery power of the implanted medical device.

17. The system of claim 8, wherein the external communications device is a cell phone.

18. The system of claim 8, wherein the implanted medical device is configured to transmit a wireless power status signal to the external communications device indicating a low battery power of the implanted medical device.

19. The system of claim 8, wherein the implanted medical device is configured to transmit a wireless power status signal to the external communications device indicating a low battery power of the implanted medical device.

20. A method for selectively placing and handling a distress call in response to activity of an implanted medical device worn by a human subject, comprising:

receiving, by an external communications device, a wireless signal from the implanted medical device; and

in response to receiving the wireless signal:

generating, by an external voice synthesizer, a voice synthesized message providing information about a nature of the human subject's condition even in the event the human subject is incapable of verbal communication;

transmitting the distress call, with the voice synthesized message, to a remote location in response to receiving the wireless signal;

receiving the distress call at the remote location;

in response to receiving the distress call at the remote location, automatically accessing a patient record from a database; and

displaying the patient record to an operator;

wherein the external communications device is a cell phone, and further comprising:

inputting the voice synthesized message into the cell phone from which the voice synthesized message is transmitted with the distress call.

21. The method of claim 20, wherein the wireless signal and distress call contain vital data pertaining to an organ being monitored by the implanted medical device.

22. The method of claim 20, further comprising receiving, by the external device, a wireless status signal from the implanted medical device indicating a low battery power of the implanted medical device.

专利名称(译)	用于植入式自动除颤器的紧急呼叫患者定位系统		
公开(公告)号	US6980112	公开(公告)日	2005-12-27
申请号	US10/041937	申请日	2002-01-08
[标]申请(专利权)人(译)	国际商业机器公司		
申请(专利权)人(译)	国际商业机器公司		
[标]发明人	NEE WRIGHT JACKEN		
发明人	NEE, WRIGHT JACKEN		
IPC分类号	A61B5/00 A61N1/08 A61N1/37 A61N1/372 A61N1/39 G08B21/04 G08B25/01 G08B23/00		
CPC分类号	A61N1/37282 A61N1/3956 G08B25/001 G08B21/0453 G08B25/016 G08B21/0211 A61B5/0031		
审查员(译)	阮PHUNG T.		
其他公开文献	US20030128121A1		
外部链接	Espacenet USPTO		

摘要(译)

用于响应于植入设备的操作而发出遇险呼叫的方法和系统。植入装置可以是能够监测和/或调节器官的多个医疗装置中的任何一种。当达到阈值条件时，由植入设备发送的遇险信号激活外部通信系统。然后，外部通信系统发出求救呼叫，该呼叫可由适当的医务人员响应。

