



US007813778B2

(12) **United States Patent**
Benaron et al.

(10) **Patent No.:** **US 7,813,778 B2**
(45) **Date of Patent:** **Oct. 12, 2010**

(54) **IMPLANTABLE TISSUE ISCHEMIA SENSOR**

5,357,954 A 10/1994 Shigezawa et al.
5,417,207 A 5/1995 Young et al.
5,520,190 A * 5/1996 Benedict et al. 600/513
5,645,059 A 7/1997 Fein et al.
5,672,875 A 9/1997 Block et al.
5,696,861 A 12/1997 Schimmeyer et al.

(75) Inventors: **David A. Benaron**, Portola Valley, CA (US); **Ilian H. Parachikov**, Belmont, CA (US); **Michael R. Fierro**, Los Gatos, CA (US)

(73) Assignee: **Spectros Corporation**, Portola Valley, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 764 days.

(Continued)

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **11/193,071**

EP 1111333 A1 6/2001

(22) Filed: **Jul. 29, 2005**

(65) **Prior Publication Data**

(Continued)

US 2007/0027371 A1 Feb. 1, 2007

OTHER PUBLICATIONS

(51) **Int. Cl.**
A61B 5/00 (2006.01)

Benaron, D., "Continuous, Noninvasive, and Localized Microvascular Tissue Oximetry Using Visible Light Spectroscopy," *Anesthesiology*, vol. 100, No. 6, Jun. 2004, pp. 1469-1475.

(52) **U.S. Cl.** **600/323**; 600/476

(58) **Field of Classification Search** None
See application file for complete search history.

(Continued)

(56) **References Cited**

Primary Examiner—Carl H. Layno

Assistant Examiner—Jon-Eric C. Morales

(74) *Attorney, Agent, or Firm*—Nixon Peabody LLP


U.S. PATENT DOCUMENTS

RE29,304 E 7/1977 Greenfield et al.
4,164,374 A 8/1979 Lambe et al.
4,427,889 A 1/1984 Müller
4,513,751 A 4/1985 Abe et al.
4,660,974 A 4/1987 Machler et al.
4,697,593 A 10/1987 Evans et al.
5,040,533 A * 8/1991 Fearnot 607/22
5,135,004 A 8/1992 Adams et al.
5,190,040 A 3/1993 Aoyagi
5,199,428 A 4/1993 Obel et al.
5,259,052 A 11/1993 Briggs et al.
5,280,788 A 1/1994 Janes et al.
5,318,022 A 6/1994 Taboada et al.
5,329,922 A 7/1994 Atlee, III
5,355,425 A 10/1994 Braiman et al.

(57) **ABSTRACT**

An implantable ischemia detection system in which a white LED (105) produces a continuous, visible, broadband light illuminating a target site (125). Light backscattered by the target is collected by a sensor (155), allowing for an index of ischemia to be determined, and subsequently transmitted by a sending unit (167). Power is provided by an internal power source (179). The entire implantable device is encapsulated by a biocompatible shell (102) to add long-term safety with regard to implantation.

18 Claims, 4 Drawing Sheets

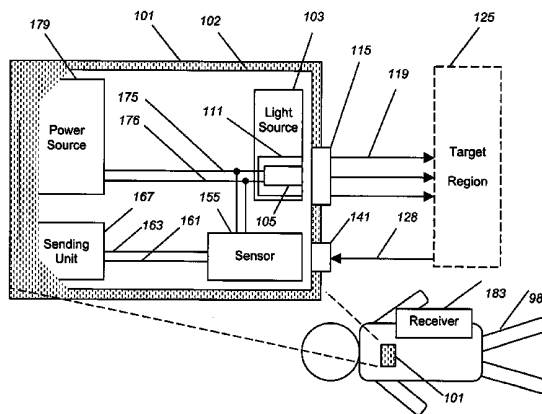

U.S. PATENT DOCUMENTS

5,733,313 A * 3/1998 Barreras et al. 607/33
 5,743,261 A 4/1998 Mainiero et al.
 5,769,791 A 6/1998 Benaron et al.
 5,830,132 A 11/1998 Robinson
 5,830,137 A 11/1998 Scharf
 5,833,603 A * 11/1998 Kovacs et al. 600/317
 5,901,261 A 5/1999 Wach
 5,902,235 A 5/1999 Lewis et al.
 5,931,779 A 8/1999 Arakaki et al.
 5,941,822 A 8/1999 Skladnev et al.
 5,974,210 A 10/1999 Alcock et al.
 5,987,346 A 11/1999 Benaron et al.
 6,043,893 A 3/2000 Treiman et al.
 6,119,031 A 9/2000 Crowley
 6,122,536 A 9/2000 Sun et al.
 6,134,460 A * 10/2000 Chance 600/342
 6,167,297 A 12/2000 Benaron
 6,226,082 B1 5/2001 Roe et al.
 6,251,068 B1 6/2001 Akiba et al.
 6,252,254 B1 6/2001 Soules
 6,256,524 B1 7/2001 Walker et al.
 6,277,078 B1 8/2001 Porat et al.
 6,278,889 B1 8/2001 Robinson
 6,353,226 B1 3/2002 Khalil
 6,381,018 B1 4/2002 Bigio et al.
 6,527,729 B1 3/2003 Turcott
 6,532,381 B2 3/2003 Bayer et al.
 6,533,466 B1 3/2003 Smith
 6,550,979 B1 4/2003 Fleenor et al.
 6,588,938 B1 7/2003 Lambert et al.
 6,599,025 B1 7/2003 Deutsch
 6,612,857 B2 9/2003 Tolmie
 6,615,065 B1 9/2003 Barrett et al.
 6,662,033 B2 12/2003 Casciani et al.

6,711,426 B2 3/2004 Benaron et al.
 6,842,635 B1 1/2005 Parker
 6,859,658 B1 2/2005 Krug
 6,921,920 B2 7/2005 Kazakevich
 6,944,488 B2 9/2005 Roberts
 7,062,306 B2 6/2006 Benaron
 2002/0082488 A1 6/2002 Ali
 2004/0122478 A1 6/2004 Stadler et al.
 2004/0218873 A1 11/2004 Nagashima et al.
 2004/0220460 A1 11/2004 Roberts
 2005/0010113 A1 1/2005 Hall
 2006/0105319 A1 5/2006 Rees et al.
 2007/0015981 A1 * 1/2007 Benaron et al. 600/323
 2007/0016080 A1 1/2007 Alfano et al.

FOREIGN PATENT DOCUMENTS

EP 1094746 B1 10/2002
 EP 0926981 B1 3/2004
 WO WO 00/01295 1/2000
 WO WO 00/64534 11/2000
 WO WO 03/003914 A1 1/2003
 WO WO 2004/058344 7/2004

OTHER PUBLICATIONS

International Search Report and Written Opinion for International Application PCT/US2006/029615, mailed Apr. 4, 2007.
 Supplemental European Search Report for EP 03718250.8 dated Jan. 30, 2008.
 International Search Report and Written Opinion for PCT/2003/10674 dated Nov. 25, 2003.
 International Search Report and Written Opinion for PCT/2008/057096 dated Jul. 31, 2008.
 International Search Report and Written Opinion for PCT/2007/013779 dated Oct. 14, 2008.

* cited by examiner

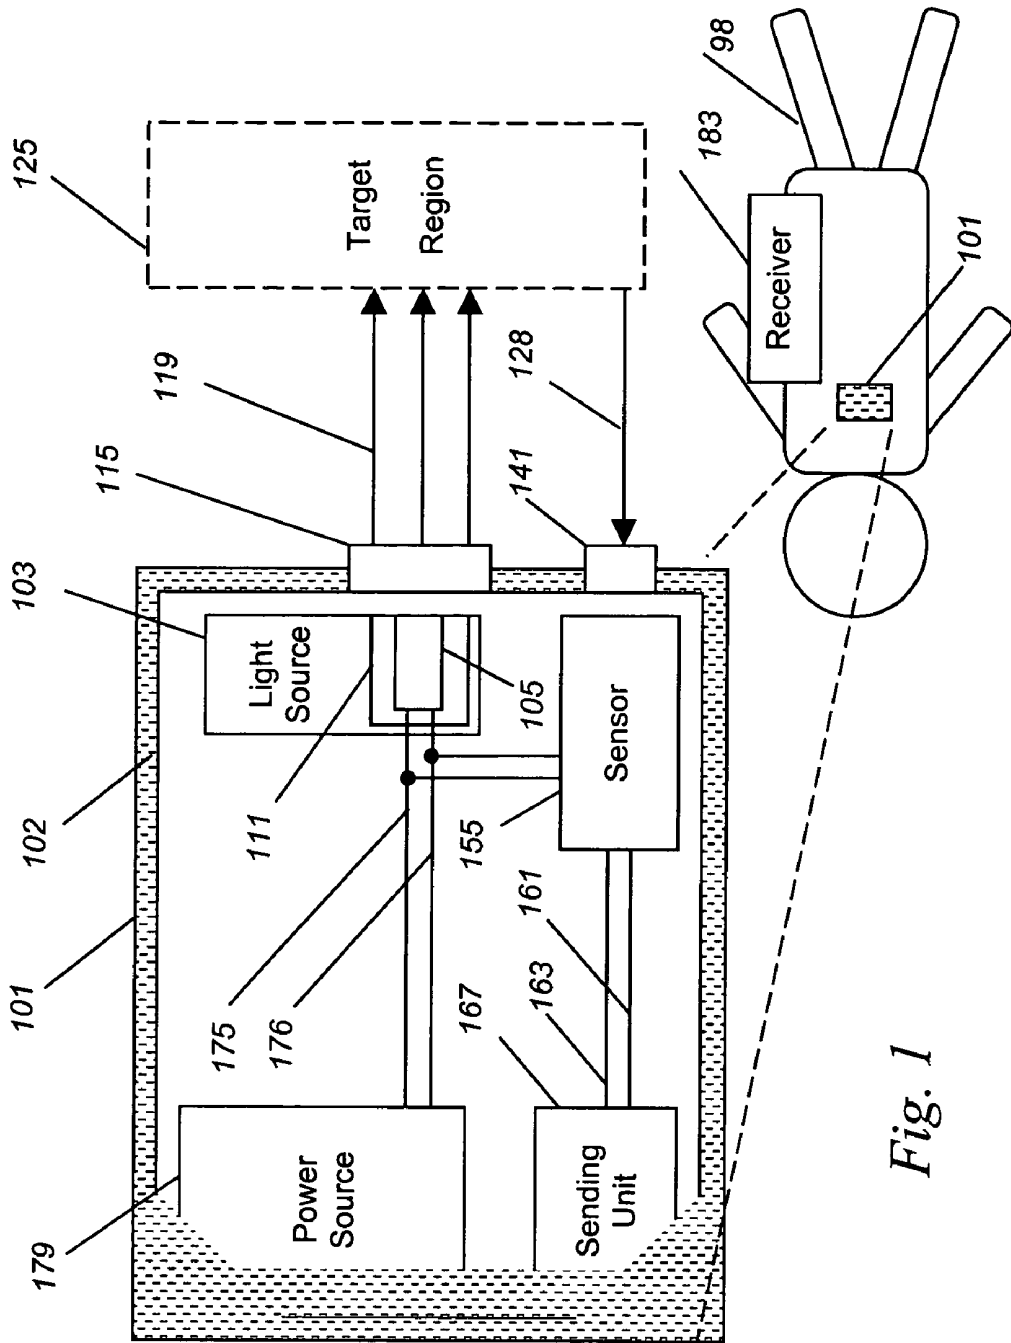


Fig. 1

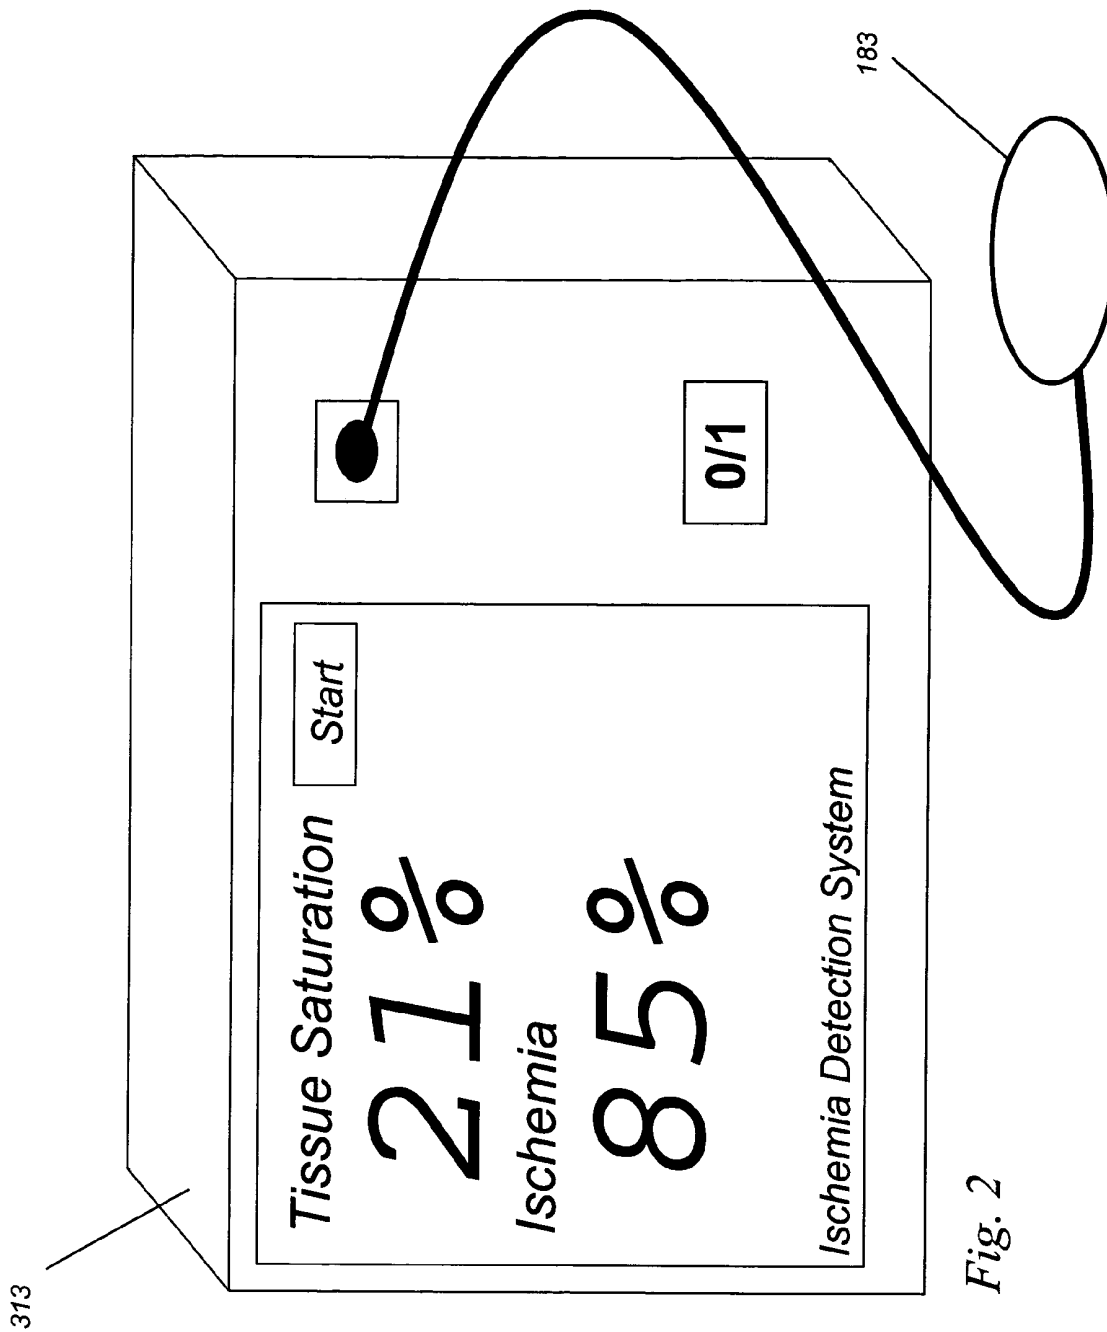


Fig. 2

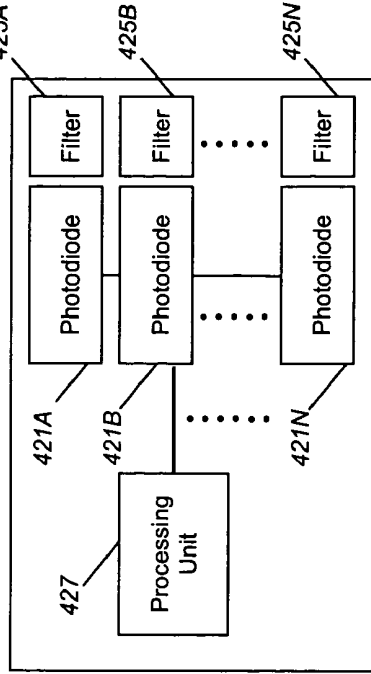


Fig. 3A

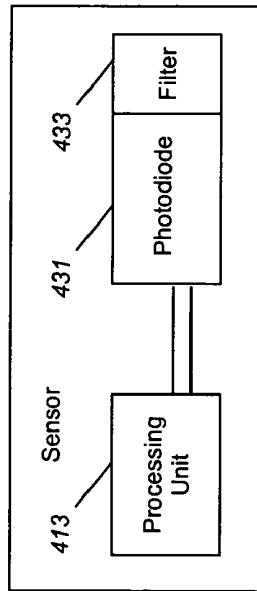


Fig. 3B

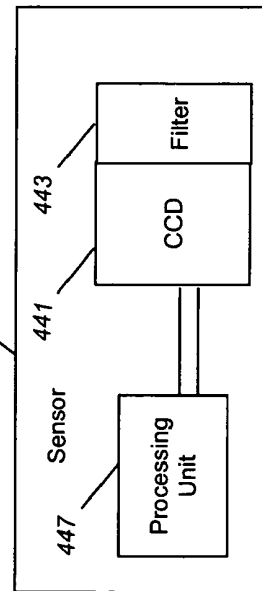


Fig. 3C

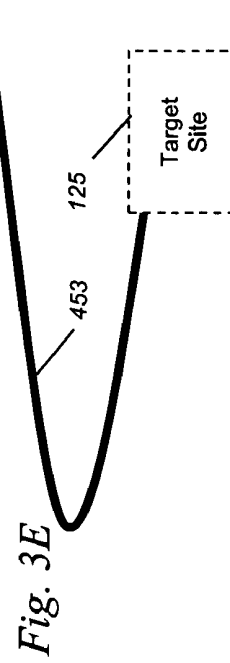


Fig. 3D

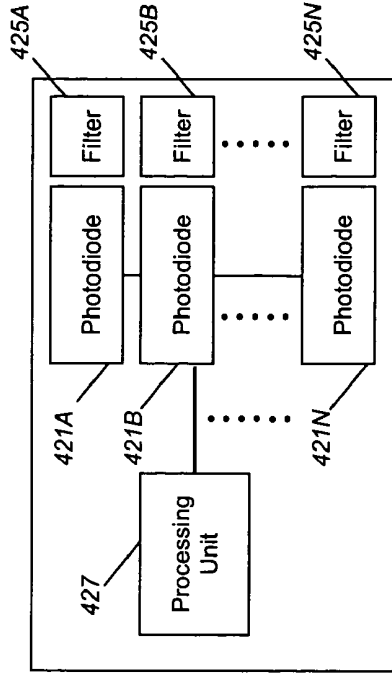


Fig. 3E

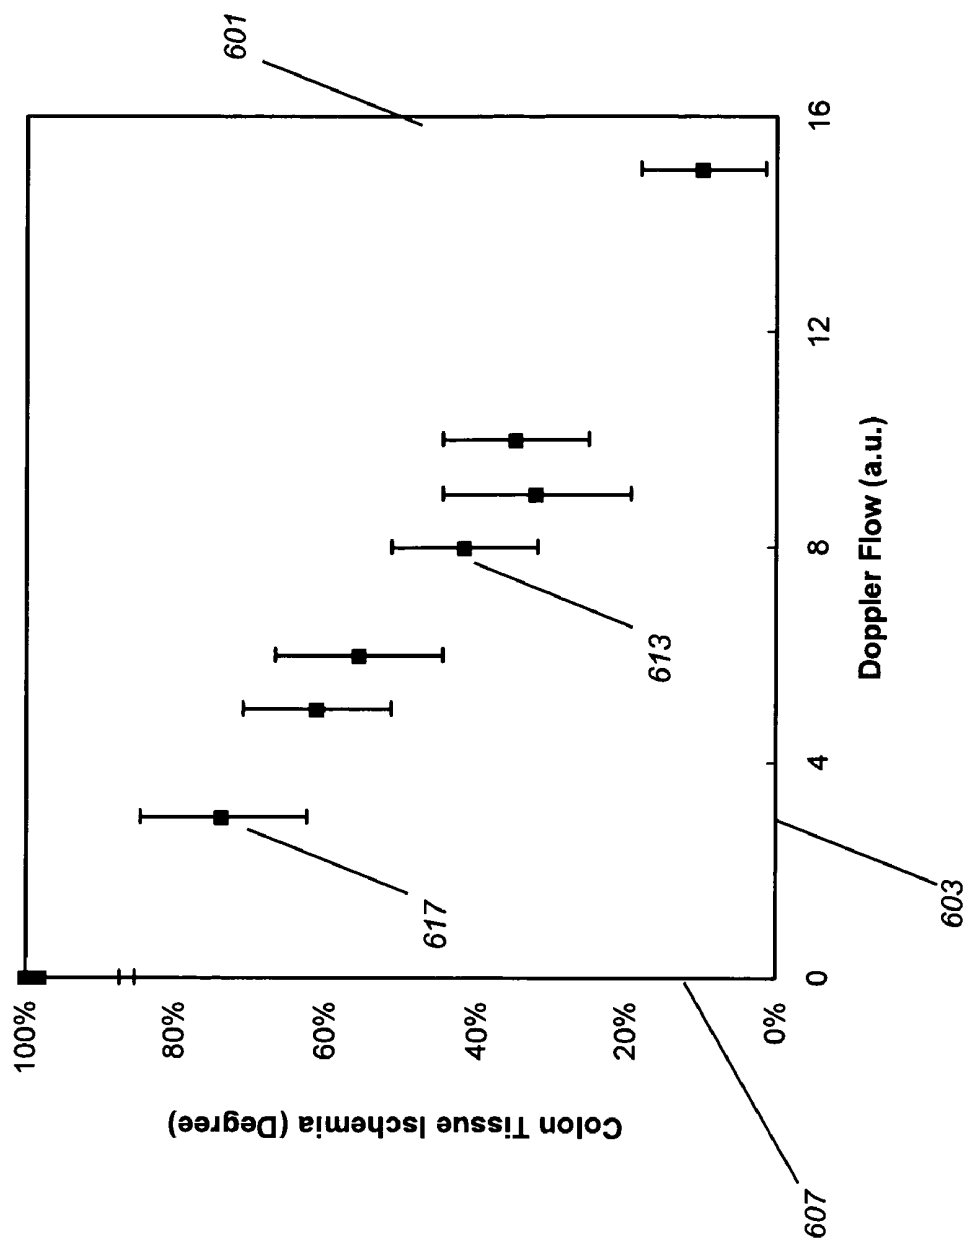


Fig. 4

IMPLANTABLE TISSUE ISCHEMIA SENSOR

FIELD OF THE INVENTION

The present invention relates to implantable devices and methods for providing localized measurements of tissue ischemia, and more particularly relates to the embedding of a visible light source, a sensor, a power source, and a transmitter into a long-term implantable shell for the purpose of performing real-time spectroscopic analysis of in vivo tissue perfusion sensitive to local tissue ischemia.

BACKGROUND OF THE INVENTION

The clinical detection of ischemia—an insufficient delivery of oxygen to meet a tissue's metabolic needs—is unreliable. Ischemia is especially difficult to detect when the ischemia is due to a localized interruption of blood flow—such as during a heart attack or stroke. Existing laboratory tests for ischemia, such as serum enzyme-leakage tests (e.g., for tests for cardiac isoenzymes after a heart attack) or EKG electrical tests, are insensitive indicators of such local tissue ischemia, especially during the early stages. Similarly, blood tests are also insensitive to local ischemia, as the ischemia is a result of low oxygenation in a local tissue, which is reflected in the local capillary oxygenation, not in the oxygenation of the arterial or venous blood when measured in the large central arteries and veins. Noninvasive imaging of ischemia lacks the immediacy that allows for early intervention or real-time feedback to other devices such as pacemakers.

Non-implantable ischemia sensors are known. For example, U.S. Pat. No. 6,532,381 teaches the detection of ischemia using externally measured electrical (EKG) monitoring and microprocessor control. However, such devices monitoring multiple external sites using wire leads placed upon the chest wall are not designed for implantability, which requires that issues of size, power consumption, biocompatibility, and robustness over time be optimized alongside sensing performance, a non-trivial task.

Implantable sensors are also well known. However, implantable sensors designed to detect ischemia are rare in the art, and none of these detect tissue ischemia directly. For example, U.S. Pat. No. 5,135,004, US Appn 2004/0122478, and WO 00/64534 predict the presence of ischemia based upon the electrical (EKG), blood pressure, local pH, and/or physical (acceleration during contraction) characteristics of the heart, while U.S. Pat. No. 6,527,729 discloses an implantable acoustic sensor that responds to heart failure by changes in the sound of the heartbeat. Further, U.S. Pat. No. 5,199,428 and US Appn 2004/0220460 teach implantable devices to monitor blood oxygenation (venous blood and arterial blood, respectively), in the latter case specifically rejecting local tissue saturation from encapsulation, thus teaching away from direct tissue monitoring. For reasons to be outlined in more detail later, such non-tissue blood oxygenation (whether arterial or venous) is insensitive to tissue ischemia, and is at best an indirect measure of tissue ischemia. For each of the devices above, then, ischemia is measured only by indirect and unreliable indicators of ischemia, such as by indicators of cardiac electrical, mechanical, and acoustic dysfunction. Another point to consider is that organs other than the heart are frequent sites of ischemia (such as in the kidney, liver, or gut), and the prior art is not directed to these other organs at all. Therefore, none of the above devices detect local tissue ischemia directly, nor can they be applied generally to any organ without regard to site.

All of the above devices are limited by being either non-implantable, by being at best an indirect measures of local tissue ischemia, or by being restricted to use in just one organ such as the heart due to the indirect measures of ischemia (such as sound or movement) which they employ.

None of the prior devices or methods allow for a direct detection of local tissue ischemia in a broad array of target sites using a long-term or short-term implantable system sensitive to local ischemia,

Such a system has not been previously described, nor successfully commercialized.

SUMMARY OF THE INVENTION

The inventors have discovered that the site at which tissue ischemia occurs is always local, and that local tissue physiology in nearly every case will attempt to compensate for this local ischemia, producing a direct depression then partial compensation on the capillary hemoglobin saturation. This local effect is often not measurable using standard blood monitoring, and capitalizing on this local capillary effect allows for the design a highly localized, fully-implantable ischemia detector.

A salient feature of the present invention is that the detection and treatment of ischemia is aided by use of an implantable ischemia sensor.

Accordingly, an object of the present invention is to provide a fully-implantable ischemia detector.

In one aspect the invention provides a direct, quantitative measure or index of local tissue ischemia.

In another aspect the invention provides a short-term implantation, such as optical fibers within the heart muscle after bypass surgery, or an implant in the lung tissue for short-term monitoring after a transplant, or even a swallowable device for detecting ischemia in the gut as it passes through the enteric system.

The improved ischemia detection system as described has many advantages one or more of which are described below. While a number of advantages are set forth for illustrative purposes only, these advantages are not intended to limit the scope of the claims in any way.

One advantage is that a physician or surgeon can obtain real-time feedback regarding local tissue ischemia in high-risk patients, and to respond accordingly, while any injury remains reversible.

Another advantage is that this system may be safely deployed within a living body.

Another advantage is that the system can be actively coupled to a therapeutic device, such as a pacemaker, to provide feedback to the pacing function, or passively coupled to a therapeutic device, such as applied to a stent to monitor stent performance over time.

Another advantage is that the system may be constructed to detect ischemia using light, which allows for simple, safe, and non-electrical transmission of the measuring photons as required.

Another advantage is that the detection can be in the tissue itself, rather than removed from the site of ischemia. Sources of local tissue signals include but are not limited to capillary hemoglobin (not in the arterial or venous circulation but locally in the capillaries in the tissue), myoglobin (which is extravascular and within muscle cells in the tissue itself) and cytochrome (which is intracellular within the mitochondria of the cells of the tissue itself).

Another advantage is that use of broadband light can allow for determination of tissue ischemia using spectroscopy, and

in particular differential spectroscopy, which allows for compensation of light scattering by tissues.

A final advantage is that ischemia sensing may be used to enable detection of many types of disease, such as tissue rejection, tissue infection, vessel leakage, vessel occlusion, and the like, many of which produce ischemia as an aspect of the disease.

There is provided an implantable device or system with broadband light source for generating light, and for delivering this light to a sample for the purpose of enabling spectroscopic ischemia detection. In some embodiments, the system uses a phosphor-coated white LED to produce continuous, broadband light from 400 nm to 700 nm, which is transmitted directly to a target site. Scattered light returning from the target is detected by a wavelength-sensitive detector, and a signal related to ischemia is generated using this wavelength-sensitive information via spectroscopic analysis. Finally, this signal is sent out from the device using radiofrequency (RF) transmission. Implantable systems incorporating the ischemia detection system and medical methods of use are described.

The breadth of uses and advantages of the present invention are best understood by example, and by a detailed explanation of the workings of a constructed apparatus, now in operation and tested in animals. These and other advantages of the invention will become apparent when viewed in light of the accompanying drawings, examples, and detailed description.

BRIEF DESCRIPTION OF THE DRAWINGS

The following drawings are provided:

FIG. 1 is a schematic diagram of an implantable tissue ischemia detector incorporating a white LED and constructed in accordance with embodiments of the invention.

FIG. 2 is a schematic of an external coil, for powering the implantable device and for receiving a signal related to the presence or degree of tissue ischemia, attached to an external monitor system.

FIGS. 3A to 3E shows five exemplary schematics of the optical sensor unit.

FIG. 4 shows data from the colon of a live subject during periods of low systemic blood flow, which led to local ischemia, as collected and analyzed in real time by a medical monitor constructed in accordance with embodiments of the invention.

DETAILED DESCRIPTION OF THE INVENTION

Definitions

For the purposes of this invention, the following definitions are provided. These definitions are intended to be illustrative and exemplary. They are not intended to restrictively limit, by the absence of any specific illustrative example, the common-sense breadth of meaning of the terms to those skilled in the art. These definitions are as follows:

Implantable: Intended for implantation internally in a living body, such as into or between internal tissues. Implantable devices typically must be biocompatible (i.e., have a biocompatible exterior), or else the host subject's immune system will attack the implanted object or the device will have a toxic effect upon the host.

Implantable does not require any fixed duration. Implantable as used herein can mean short-term implantation, such as removable fibers inserted in the heart or lung, or a swallowable device such as an gastrointestinal ischemia monitor. Implantable as used herein may also be a long-term implan-

tation, such as a pacemaker feedback system which monitors the heart or muscle, or a liver-based MEMS device that monitors for rejection.

Fully-Implantable: Complete implantation into a living body, without a physical connection to the external body. Fully-implantable devices may contain an embedded power supply, receive power from another implanted device (such as a pacemaker), or receive power from an external source such as via transcutaneous inductive coupling. Fully-implantable devices may still communicate with receivers external to the body via non-physical means, such as electromagnetic waves from RFID chips. An implantable system may be embedded long-term, such as buried deep within a body to monitor for organ rejection or cardiac ischemia. An implantable system may also be used short-term only, such as a swallowable pill that monitors for ischemic ulcers or polyps in the esophagus, stomach, intestines, and colon, and is passed via the rectum when the scanning is complete in a few hours to a few days.

Tissue: Material from a living animal, plant, viral, or bacterial subject, with an emphasis on mammals, especially humans.

Perfusion: The flow of blood to a tissue or region, which differs from tissue ischemia in that low flow does not guarantee ischemia.

Blood Oxygenation: The saturation of the hemoglobin in arterial and venous blood, which differs from tissue ischemia. Arterial blood can be 100% oxygenated, yet a blood clot in the coronary artery will produce severe ischemia despite the 100% arterial saturation. Similarly, a local occlusion may produce lethal local ischemia, while the average venous oxygenation is not lowered detectably due to the small contribution of that local tissue to the overall venous blood oxygenation.

Ischemia: A local condition of tissue in which the delivery of oxygen to the tissue is locally inadequate to meet its metabolic needs. Such conditions vary from tissue to tissue. For example, the brain has a high metabolic rate and is easily made ischemic, even during simple tasks such as deep thought and insight, unless there is a local and rapid increase in the baseline blood flow and oxygen delivery to the metabolizing cortical tissues. In contrast, the growing fetus is in a relative hibernation state, with very low oxygen needs in most tissues, and is more difficult to make ischemic. Early and mild ischemia is often evidenced by increases in the amount of oxygen extracted from the blood being delivered to the capillary bed, resulting in decreased tissue oxygenation. Later stage ischemia is evidenced by lactic acid formation and disturbed cellular metabolism that occurs when the simple compensatory mechanisms of the tissue (increase oxygen extraction, increase flow) are no longer sufficient to protect the tissue from the rising ischemia. Ischemia is therefore distinguished from perfusion (i.e., blood flow) in that low blood flow does not guarantee ischemia (such as during tissue cooling or in the fetus), nor does high flow rule out ischemia (such as during sepsis, fever, or intense work). Ischemia is a co-existing condition in many different types of illnesses, including sepsis, tissue rejection, heart attack, stroke, organ failure, diabetic disease, and other conditions.

Target: A material to be detected, imaged, or studied. In the accompanying examples, one target site is the intestine.

Target Signal: A sensed signal specific to the target. This signal may be enhanced through use of a contrast agent. This signal may be produced by scattering, absorbance, phosphorescence, fluorescence, Raman effects, or other known spectroscopy techniques.

Visible Light: Electromagnetic radiation from blue to yellow, namely with wavelengths between 400 nm and 625

microns, but especially those green to orange wavelengths between 475 and 600 nm where the absorbance by capillary hemoglobin (not in the arterial or venous circulation but locally in the capillaries in the tissue), myoglobin (which is extravascular and within muscle cells in the tissue itself) and cytochrome (which is intracellular within the mitochondria of the tissue itself) is the strongest.

Broadband Light: Light produced over a wide range of wavelengths sufficient to perform solution of multiple simultaneous spectroscopic equations. For tissue, a width of at least 40 nm is likely to be needed, while in the preferred embodiment a broadband white LED produces light from 400 nm to beyond 700 nm.

LED: A light emitting diode.

White LED: A broadband, visible wavelength LED, often comprised of a blue LED and a blue-absorbing broad-emitting phosphor that emits over a wide range of visible wavelengths. Other phosphors can be substituted. As used in the examples herein, any broadband LED could be used, even if not emitting over a full (white) spectrum. For example, a green LED emitting over a FWHM range of 100 nm would be considered to be broadband.

Light Source: A source of illuminating photons. It may be composed of a simple light bulb, a laser, a flash lamp, an LED, a white LED, or another light source or combination of sources, or it may be a complex form including but not limited to, a light emitter such as a bulb or light emitting diode, one or more filter elements, a transmission element such as an integrated optical fiber, a guidance element such as a reflective prism or internal lens, and other elements intended to enhance the optical coupling of the light from the source to the tissue or sample under study. The light may be generated using electrical input (such as with an LED), optical input (such as a fluorescent dye in a fiber responding to light), or any other source of energy, internal or external to the source. The light source may be continuously on, pulsed, or even analyzed as time-, frequency-, or spatially-resolved. The light emitter may comprise a single or multiple light emitting elements, such as a combination of different light emitting diodes to produce a spectrum of light.

Light Detector or Light Sensor: A detector that generates a measurable signal in response to the light incident on the detector.

Optical Coupling: The arrangement of two elements such that light exiting the first element interacts, at least in part, with the second element. This may be free-space (unaided) transmission through air or space, or may require use of intervening optical elements such as lenses, filters, fused fiber expanders, collimators, concentrators, collectors, optical fibers, prisms, mirrors, or mirrored surfaces and the like.

Embodiments of the device and system will now be described.

FIG. 1 shows device 101 implanted into the chest wall of patient 98. Of note, patient 98 is shown for illustrative purposes, and is not considered a part of the invention. A cut-away schematic of device 101 showing the interior of implantable device 101 is shown at the top of FIG. 1. Device 101 is surrounded by biocompatible exterior 102. Typically, exterior 102 is constructed from approved Class VI materials as recognized by the U.S. FDA or other medical device regulatory agencies, such as polyethylene or surgical steel. Portions of the sensor, power supply, light source, or transmitter may protrude as needed from this shell within the spirit of this invention, provided that the protruding parts themselves are biocompatible.

Within device 101, light source 103 is illustrated in its component parts. In some embodiments, broad spectrum

white light is emitted by a high conversion-efficiency white LED source 105 (in this case, The LED Light, model T1-3/4-20W-a, Fallon, Nev.). In the exemplary embodiments, diode source 105 is embedded into a plastic beam-shaping mount using optical clear epoxy 111 to allow light generated in LED 105 to be collimated, thus remaining at a near-constant diameter after passing through optical window 115 to leave device 101. Light then is able to pass forward as shown by light path vectors 119, with at least a portion of this light optically coupled to target region 125. Note that while target region 125 may be in some instances a living tissue, the tissue itself is not considered to be a claimed part of this invention.

A portion of the light reaching target 125 is absorbed by ischemia in the tissue and another portion is backscattered and returns as to device 101, as shown by light path vectors 128, to optical collection window 141. Collection window 141 in this embodiment is a glass, plastic, or quartz window, but can alternatively be merely an aperture, or even be a lens, as required. Light then strikes sensor 155, where it is sensed and detected.

Sensor 155 may comprise a number of discrete detectors configured to be wavelength-sensitive, or may be a continuous CCD spectrometer, with entry of light by wavelength controlled by gratings, filters, or wavelength-specific optical fibers. In any event, sensor 155 transmits an ischemia signal related to the detected light backscattered from target 125, producing an electrical signal sent via wires 161 and 163 a sending unit 167, such as a transmitter chip. The signal transmitted by the sending unit 167 is received by the receiver 183 where it can be further processed to provide a display.

In one embodiment, light source 103 also has two electrical connections 175 and 176, connecting light source 103 to power source 179. In one embodiment, power source 179 is an inductive power supply, capable of receiving an inductive field from externally powered coil and RFID receiver 183 (FIG. 2) placed outside of the body, in order to produce power for device 101 as required. Note that external powered coil 183 is shown for the purposes of example and illustration, but is not considered a required part of this invention. Alternatively, source 179 could merely be a long-lived implantable battery, in which case an external powered coil may not be required at all.

Operation of the device may now be described.

Device 101 is implanted in a patient, for example in the chest wall of a patient undergoing coronary artery repair for heart disease. The device may measure the muscle directly, or it can be placed at a distance. In the latter case, vectors 119 are fiber optics extended from device 101 and into close proximity to the target heart muscle, sufficient for optical coupling. Then the patient is allowed to heal after surgery, and the implantable device is left inside the patient's body, without a direct physical connection to the outside world.

In this example, device 101 is normally powered down and in a resting (off) state. At some point, it is desired to test the target heart muscle for the presence of ischemia. As shown in FIG. 2, external inductive coil 183 is connected to external monitor is brought into close proximity to the chest wall over the site of implantation of device 101. Referring back to FIG. 1, through inductive coupling external coil 183 induces a current in inductive power source 179 located within device 101, producing sufficient power for device 101 to power up and turn on. Light source 103 begins to illuminate the target 125, in this case heart muscle. Sensor 155, which is an embedded spectrophotometer in some embodiments, receives back-scattered light, resolves the incoming light by wavelength, a marker of ischemia. The result of this determination is sent to sending unit 167, which in the exemplary embodiment is an

RF transmitter that sends the sensed signals to external RFID receiver **184**. There, the signal received by receiver **184** may be processed for the oxygenation of the hemoglobin in the terminal capillary beds, a marker of ischemia, by external monitor **313**, as shown in the data collected and plotted under the Example section, below. An example of a system for indicating oxygenation is described in U.S. Pat. No. 5,987,346, incorporated herein by reference.

Once the measurement is completed, external coil **183** is moved away from device **101**, and device **101** powers down and returns to a resting state.

In an alternative embodiment, power source **179** may be charged during proximity to external coil, or have an internal battery source, allowing device **101** to operate when external coil **179** is not present. Sending unit **167** may then transmit without being directly queried, such as in response to a dangerous level of ischemia.

The light sensor which resolves the incoming light by wavelength and sends a signal to the sending unit has been mentioned, and will now be more fully described with reference to FIGS. 3A to 3E. In one form, FIG. 3A, the sensor **155** is merely single photodiode **411** and processing electronics **413**. Photodiode **411** is made wavelength sensitive through the design of LED **105** as a cluster of LEDs of different wavelengths, each emitting at a different time or modulation frequency to allow decoding of the illuminating wavelength by photodiode **411** and processing unit electronics **413**. Alternatively, sensor **155** may comprise a set of different photodiodes **421A** through **421N**, FIG. 3B, each with filters **425A** through **425N**, allowing each photodiode to be sensitive to only one wavelength range, again allowing decoding of the sensed light by wavelength by processing unit electronics **427**. Alternatively again, sensor **155** may be single photodiode **431** with electronically variable filter **433**, FIG. 3C, allowing the wavelength transmitted to be selected and processed by processing unit electronics **435**.

Still referring to FIGS. 3A to 3E, in other configurations, sensor **155** may be CCD chip **441** with filter window **443**, FIG. 3D, that varies over its length, allowing only certain wavelengths to reach each portion of CCD **441**, allowing decoding of the illuminating wavelength by processing unit electronics **447**. Finally, in the preferred embodiment, FIG. 3E, sensor **155** comprises CCD chip **451** with optical fibers **453** attached to CCD **451** in a linear array. Fibers **453** are manufactured such that each fiber has a different interference coating on end **454**, allowing each fiber to transmit a different narrow wavelength range, allowing decoding of the illuminating wavelength by processing unit electronics **457**. Fibers **453** are biocompatible and can extend outside of device case **102**, allowing device **101** to be placed remotely the target to be monitored, and for the free end of fibers **453** to be placed in proximity to target **125**.

EXAMPLE

The breadth of uses of the present invention is best understood by example. This example is by no means intended to be inclusive of all uses and applications of the apparatus, merely to serve as a case study by which a person, skilled in the art, can better appreciate the methods of utilizing, and the scope of, such a device.

In this example, an optical sensor, similar in basis of operation to device **101**, is implanted into abdomen of a patient undergoing colon surgery. In this case, the animal receives heart-lung bypass, such that the blood flow and oxygen content of the blood is exactly controlled by a bypass specialist rather than by the animal's own heart and lungs, affording the

ability to create and resolve ischemia at will. An aortic Doppler probe is placed, which measures the delivery of blood to tissue. In this case, when the rate of the pump is lowered to zero flow, ischemia must exist in the tissues being monitored.

Analysis of the tissue ischemia is performed by broadband, visible light, differential spectroscopy. In this technique, the first differential (for example) of the wavelength vs. intensity curve sent from the sending unit is processed to remove many of the effects caused by light scattering by the local tissue, and the resultant signal is analyzed using a least-squares minimization of the fitting error to known components of the tissue (such as myoglobin, capillary hemoglobin, or cytochromes).

The signal that is measured is a function of the presence, absence, or risk, or degree of ischemia. This can have clinical implications and applications in many different medical areas, such as impending risk of tissue death (as seen in the colon study above), impending risk of organ rejection (as inflammation results in increased total blood content, while potentially reducing oxygenation) cardiac function (as improved cardiac function is associated with a body-wide improvement in tissue ischemia as well as a likely improvement in myocardial ischemia), treatment efficacy for arterial or venous vascular disease (as the real-time effects of such interventions on tissue oxygenation adequacy can be used as a treatment signal to guide chemical and physical interventions), risk of renal damage (as kidney failure is often the result of acute or chronic reduced oxygen delivery), risk of brain injury (as stroke is often the result of acute and chronic reduced oxygen delivery), risk of colon death (as the colon does not have a large capacity to increase blood and oxygen delivery in times of stress over baseline), risk of limb amputation (as limbs with good capillary saturation are more likely to heal and not require amputation), risk of ulcer healing (as G.I. and diabetic ulcers are more likely to heal if ischemia is not the only ongoing problem), and risk of critical limb ischemia (as limb salvage is always better if possible, but delays resolution of ischemia and presents a risk to the patient if delayed when amputation is required).

As shown in FIG. 4, the creation of graded ischemia is detected by the present invention. In graph **601**, the flow detected by the Doppler probe is plotted on horizontal axis **603** versus the presence of ischemia as detected by the present invention using optical spectroscopy plotted on vertical axis **607**. Data are plotted as means with standard error bars **613**. As can be seen on graph **601**, when the blood flow to the gut is reduced to zero, the detection of the presence of ischemia rises to 100%, shown at data point **617**.

It is important to note that the measurement of flow/perfusion alone, or the measurement of blood oxygenation (not tissue oxygenation, but oxygenation of the arterial blood) alone are not sufficient to detect the condition of ischemia. Ischemia is diagnosed by low local tissue oxygenation, not blood oxygenation or flow. In some cases, arterial blood may be well oxygenated, but the delivery of this arterial blood to the tissue is insufficient (such as with a blood clot); in this case the tissue is indeed ischemia while the arterial blood oxygenation is normal. Blood flow also differs from a direct measure of ischemia. For example, in a cooled patient on heart-lung bypass, blood flow may be very, very low; however, the cooled tissues, whose oxygen need has been reduced by the low temperature, are not ischemic. Similarly, a chronically ischemic heart "hibernates" in order to reduce its own oxygen need, and may not be ischemic at reduced flow. In the above animal study example, flow was controlled sufficiently to allow for a low or zero flow to be consistent with ischemia, but such conclusions cannot be always made so clearly in the living non-experimental subject.

Also, in the example above, power was provided to the device externally. However, as noted earlier, an integrated battery or set of batteries can provide power from within the device, reducing cost of the connection tip. An added advantage of this battery-based approach is that it removes the need for electrical connection to the light source, as an added safety feature.

In this example, the signal detected from the tissue was a hemoglobin absorbance signal derived from the capillary bed. While absorbance is ideal for hemoglobin analysis, as described in the preferred embodiment, other interactions may be preferable for other measurements. The interaction with the illuminating light that provides the contrast can include absorbance, polarization, optical rotation, scattering, fluorescence, Raman effects, phosphorescence, or fluorescence decay, and measures of a contrast effect may reasonably include one or more of these effects. Other tissue components could be measured, including NADH, NADPH, cytochromes in their oxidized and reduced forms, or even ischemia or oxygen sensitive dyes. Next, when monitoring muscle such as the heart, myoglobin is another protein whose saturation is related to the presence or absence of ischemia. In such cases, a combination of hemoglobin in the capillaries as well as myoglobin in the heart, or just myoglobin in the heart myocytes, can serve as a marker of ischemia. Last, an injectable dye, sensitive to local ischemia, can be used to generate an optical signal directly related to the presence of ischemia, such as by changing color in response to mitochondrial membrane charge or in response to intracellular pH. Such use of dyes to label cells in vivo with optical dyes has been demonstrated in vivo by several groups, and the coupling of an ischemia sensitive dye to use of the present invention to detect ischemia (and conditions which are a function of ischemia) would fall within the spirit of the present invention.

We have discovered an implantable ischemia detector for detecting local tissue ischemia in a quantitative and enabling manner in a broad array of target sites. In some embodiments a device is provided comprising a phosphor-coated white LED and integrated collimating optics configured to produce continuous, broadband light from 400 nm to 700 nm in a collimated beam, which is then directly transmitted to a target site. Light backscattered by the target site is collected by a sensor, allowing for a direct measure of ischemia to be determined, and subsequently transmitted by a sending unit. Power is provided by an internal power source, which may in turn be itself powered by an external inductive coil that is brought in proximity to the implanted device in order to provide energy as needed. The entire implantable device is encapsulated by a biocompatible shell to add long-term safety while implanted. Used alone, or in combination with an estimate of arterial oxygenation, venous oxygenation, or even of blood flow, this device allows for an index of ischemia to be determined without additional invasiveness beyond the initial implantation. The present device may be interrogated using inductive technology and RF coupling. Implantable devices incorporating the ischemia system, and medical methods of use, are described. This device has immediate application to several important problems, both medical and industrial, and thus constitutes an important advance in the art.

What is claimed is:

1. An implantable device comprising:
 - a light source for illuminating a target with light;
 - a sensor configured so as to detect light backscattered substantially from local capillary and extravascular tissue within the target site onto said sensor and to provide a tissue oxygenation output signal that is a direct func-

tion of the presence or degree of internal tissue ischemia based at least on said light backscattered from said site; a power source configured to supply energy to said sensor, and said light source; and

an exterior shell enclosing said power source, light source, and sensor configured so as to be biocompatible with respect to implantation internally wherein said external shell is a swallowable capsule for passage through the gastrointestinal system.

2. The implantable device of claim 1, wherein said light source is a broadband white LED.

3. The implantable device of claim 1, wherein said sensor is a CCD configured so as to be wavelength sensitive.

4. The implantable device of claim 1, wherein said output signal is generated using differential spectroscopy.

5. The implantable device of claim 1, wherein said power source is an inductive coil for receiving power.

6. The implantable device of claim 1, wherein said measure of internal tissue ischemia is a function selected from the list of functions comprising impending risk of tissue death, impending risk of organ rejection, cardiac function, treatment efficacy for arterial or venous vascular disease, risk of renal damage, risk of brain injury, risk of colon death, risk of limb amputation, risk of ulcer healing, or risk of critical limb ischemia.

7. The device of claim 1, further comprising a sending unit for receiving the output signal and transmitting said output signal.

8. The implantable device of claim 7, wherein said output signal is a function of a measure selected from at least one of a list of measures comprising tissue capillary hemoglobin saturation, cellular myoglobin saturation, and intracellular mitochondrial cytochrome saturation.

9. The implantable device of claim 7, wherein said sending unit is comprised of any one or more of an RF transmitter, an RFID chip, or an optical fiber.

10. An implantable device comprising:

a light source for illuminating a target with light;

a sensor configured so as to detect light backscattered substantially from local capillary and extravascular tissue within the target site onto said sensor and to provide a tissue oxygenation output signal that is a direct function of the presence or degree of internal tissue ischemia based at least on said light backscattered from said site; a power source configured to supply energy to said sensor, and said light source;

an exterior shell enclosing said power source, light source, and sensor configured so as to be biocompatible with respect to implantation internally; and

a sending unit for receiving the output signal and transmitting the output signal, wherein said sending unit is coupled to an implanted pacemaker, for the purpose of real time feedback.

11. The implantable device of claim 10, wherein said external shell is a fully-sealed biocompatible shell for implantation in an organ or tissue.

12. The implantable device of claim 10, wherein said measure of tissue ischemia is a function selected from the list of functions comprising impending risk of tissue death, impending risk of organ rejections, cardiac functions, treatment efficacy for arterial or venous vascular disease, risk of renal damage, risk of brain injury, risk of colon death, risk of limb amputation, risk of ulcer healing, or risk of critical limb ischemia.

13. The implantable device of claim 10, wherein said light source is a broadband white LED.

11

14. The implantable device of claim 10, wherein said sensor is a CCD configured so as to be wavelength sensitive.

15. The implantable device of claim 10, wherein said output signal is a function of a measure selected from at least one of a list of measures comprising tissue capillary hemoglobin saturation, cellular myoglobin saturation, and intracellular mitochondrial cytochrome saturation.

16. The implantable device of claim 10, wherein said output signal is generated using differential spectroscopy.

12

17. The implantable device of claim 10, wherein said power source is an inductive coil for receiving power.

18. The implantable device of claim 10, wherein said sending unit is comprised of any one or more of an RF transmitter, an RFID chip, or an optical fiber.

* * * * *

专利名称(译)	植入式组织缺血传感器		
公开(公告)号	US7813778	公开(公告)日	2010-10-12
申请号	US11/193071	申请日	2005-07-29
[标]申请(专利权)人(译)	SPECTROS		
申请(专利权)人(译)	SPECTROS CORPORATION		
当前申请(专利权)人(译)	Alifak		
[标]发明人	BENARON DAVID A PARACHIKOV ILIAN H FIERRO MICHAEL R		
发明人	BENARON, DAVID A. PARACHIKOV, ILIAN H. FIERRO, MICHAEL R.		
IPC分类号	A61B5/00		
CPC分类号	A61B5/0031 A61B5/0261 A61B5/14542 A61B5/1459 A61B5/412		
代理机构(译)	尼克松皮博迪律师事务所		
其他公开文献	US20070027371A1		
外部链接	Espacenet USPTO		

摘要(译)

一种可植入的局部缺血检测系统，其中白色LED (105) 产生照射目标部位的连续可见宽带光 (125)。由目标反向散射的光由传感器 (155) 收集，允许确定缺血指数，并随后由发送单元 (167) 发送。电源由内部电源 (179) 提供。整个可植入装置由生物相容性壳体 (102) 封装，以增加植入的长期安全性。

