



US008781555B2

(12) **United States Patent**
Burnside et al.

(10) **Patent No.:** **US 8,781,555 B2**
(45) **Date of Patent:** ***Jul. 15, 2014**

(54) **SYSTEM FOR PLACEMENT OF A
CATHETER INCLUDING A
SIGNAL-GENERATING STYLET**

604/264, 95.01; 606/129; 128/845-849,
128/852; 607/5

See application file for complete search history.

(75) Inventors: **Eddie K. Burnside**, Bountiful, UT (US);
Shayne Messerly, Kaysville, UT (US)

(56) **References Cited**

(73) Assignee: **C. R. Bard, Inc.**, Murray Hill, NJ (US)

U.S. PATENT DOCUMENTS

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 851 days.

3,133,244 A 5/1964 Wojtulewicz
(Continued)

This patent is subject to a terminal dis-
claimer.

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **12/715,556**

AU 642647 11/1990

(22) Filed: **Mar. 2, 2010**

(Continued)

(65) **Prior Publication Data**

US 2010/0204569 A1 Aug. 12, 2010

Related U.S. Application Data

(63) Continuation-in-part of application No. 12/426,175,
filed on Apr. 17, 2009, which is a continuation-in-part
(Continued)

OTHER PUBLICATIONS

Stas, Met al, Peroperative Intravasal Electrographic Control of Cath-
eter Tip Position in Access Ports Placed by Venous Cut-Down Tech-
nique, EJSO, pp. 316-320, vol. 27, 2001.

(Continued)

(51) **Int. Cl.**

Primary Examiner — Long V. Le

Assistant Examiner — Lawrence Laryea

(74) *Attorney, Agent, or Firm* — Rutan & Tucker, LLP

A61B 5/05 (2006.01)
A61B 5/00 (2006.01)
A61B 5/06 (2006.01)
A61B 8/08 (2006.01)
A61B 19/00 (2006.01)
A61B 5/042 (2006.01)
A61B 8/00 (2006.01)
A61B 19/08 (2006.01)

(52) **U.S. Cl.**

CPC . **A61B 5/06** (2013.01); **A61B 19/38** (2013.01);
A61B 8/0833 (2013.01); **A61B 2019/5251**
(2013.01); **A61B 5/05** (2013.01); **A61B**
2019/5276 (2013.01); **A61B 5/042** (2013.01);
A61B 8/4472 (2013.01); **A61B 5/062** (2013.01);
A61B 8/0841 (2013.01); **A61B 19/08** (2013.01);
A61B 19/5244 (2013.01)

USPC **600/424**; **600/585**



(58) **Field of Classification Search**

USPC 600/407, 509, 424, 443, 528-529, 409,
600/447, 428, 587, 121; 604/523, 194, 585,

(57) **ABSTRACT**

An integrated catheter placement system for accurately plac-
ing a catheter within a patient's vasculature is disclosed. In
one embodiment, the integrated system comprises a system
console, a tip location sensor unit for temporary placement on
the patient's chest, and an ultrasound probe. The tip location
sensor senses a field produced by a stylet disposed in a lumen
of the catheter when the catheter is disposed in the vascula-
ture. The ultrasound probe ultrasonically images a portion of
the vasculature prior to introduction of the catheter. ECG
signal-based catheter tip guidance is included to enable guid-
ance of the catheter tip to a desired position with respect to a
node of the patient's heart. The stylet includes an electromag-
netic coil that can be operably connected to the sensor unit
and/or console through a sterile barrier without compromis-
ing the barrier. The stylet can also be wirelessly connected to
the sensor unit and/or console.

21 Claims, 40 Drawing Sheets

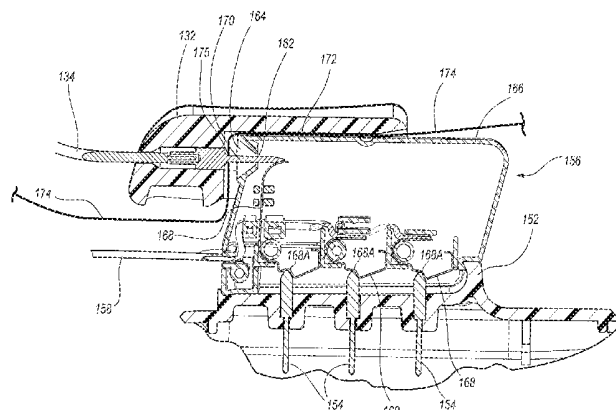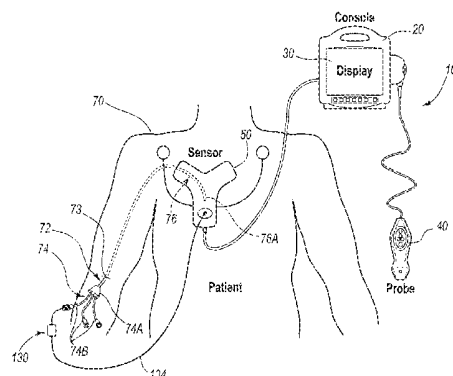

Related U.S. Application Data

of application No. 12/323,273, filed on Nov. 25, 2008, now Pat. No. 8,388,541.

- (60) Provisional application No. 61/156,842, filed on Mar. 2, 2009, provisional application No. 61/095,921, filed on Sep. 10, 2008, provisional application No. 61/095,451, filed on Sep. 9, 2008, provisional application No. 61/091,233, filed on Aug. 22, 2008, provisional application No. 61/045,944, filed on Apr. 17, 2008, provisional application No. 60/990,242, filed on Nov. 26, 2007.

(56) References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|-------------|---------|---------------------|-------------|---------|-----------------------|
| 3,297,020 A | 1/1967 | Mathiesen | 4,733,669 A | 3/1988 | Segal |
| 3,625,200 A | 12/1971 | Muller | 4,737,794 A | 4/1988 | Jones |
| 3,674,014 A | 7/1972 | Tillander et al. | 4,741,356 A | 5/1988 | Letzo et al. |
| 3,817,241 A | 6/1974 | Grausz | 4,742,356 A | 5/1988 | Kuipers |
| 3,847,157 A | 11/1974 | Caillouette et al. | 4,753,247 A | 6/1988 | Kirsner et al. |
| 3,868,565 A | 2/1975 | Kuipers | 4,770,185 A | 9/1988 | Silverstein et al. |
| 3,902,501 A | 9/1975 | Citron et al. | 4,771,788 A | 9/1988 | Millar |
| 3,995,623 A | 12/1976 | Blake et al. | 4,781,685 A | 11/1988 | Lehmann et al. |
| 4,003,369 A | 1/1977 | Heilman et al. | 4,784,646 A | 11/1988 | Feingold |
| 4,063,561 A | 12/1977 | McKenna | 4,787,070 A | 11/1988 | Suzuki et al. |
| 4,072,146 A | 2/1978 | Howes | 4,787,396 A | 11/1988 | Pidorenko |
| 4,114,601 A | 9/1978 | Abels | 4,793,361 A | 12/1988 | DuFault |
| 4,149,535 A | 4/1979 | Volder et al. | 4,794,930 A | 1/1989 | Machida et al. |
| 4,173,228 A | 11/1979 | Van Steenwyk et al. | 4,796,632 A | 1/1989 | Boyd et al. |
| 4,175,566 A | 11/1979 | Millar | 4,798,588 A | 1/1989 | Aillon |
| 4,181,120 A | 1/1980 | Kunii et al. | 4,798,598 A | 1/1989 | Bonello et al. |
| 4,224,949 A | 9/1980 | Scott et al. | 4,809,681 A | 3/1989 | Kantrowitz et al. |
| 4,244,362 A | 1/1981 | Anderson | 4,809,713 A | 3/1989 | Grayzel |
| 4,289,139 A | 9/1981 | Enjoji et al. | 4,813,729 A | 3/1989 | Speckhart |
| 4,317,078 A | 2/1982 | Weed et al. | 4,821,731 A | 4/1989 | Martinelli et al. |
| 4,327,722 A | 5/1982 | Groshong et al. | 4,836,214 A | 6/1989 | Sramek |
| 4,362,166 A | 12/1982 | Furler et al. | 4,840,622 A | 6/1989 | Hardy |
| 4,365,639 A | 12/1982 | Goldreyer | 4,849,692 A | 7/1989 | Blood |
| 4,380,237 A | 4/1983 | Newbower | 4,850,358 A | 7/1989 | Millar |
| 4,407,294 A | 10/1983 | Vilkomerson | 4,852,580 A | 8/1989 | Wood |
| 4,429,693 A | 2/1984 | Blake et al. | 4,856,317 A | 8/1989 | Pidorenko et al. |
| 4,431,005 A | 2/1984 | McCormick | 4,856,529 A | 8/1989 | Segal |
| 4,431,214 A | 2/1984 | Buffington | 4,860,757 A | 8/1989 | Lynch et al. |
| 4,445,501 A | 5/1984 | Bresler | 4,867,169 A | 9/1989 | Machida et al. |
| 4,459,854 A | 7/1984 | Richardson et al. | 4,869,263 A | 9/1989 | Segal et al. |
| 4,469,106 A | 9/1984 | Harui | 4,869,718 A | 9/1989 | Brader |
| 4,483,343 A | 11/1984 | Beyer et al. | 4,887,606 A | 12/1989 | Yock et al. |
| 4,491,137 A | 1/1985 | Jingu | 4,887,615 A | 12/1989 | Taylor |
| 4,565,201 A | 1/1986 | Lass | 4,889,128 A | 12/1989 | Millar |
| 4,572,198 A | 2/1986 | Codrington | 4,899,756 A | 2/1990 | Sonek |
| 4,577,634 A | 3/1986 | Gessman | 4,901,725 A | 2/1990 | Nappholz et al. |
| 4,582,067 A | 4/1986 | Silverstein et al. | 4,905,698 A | 3/1990 | Strohl, Jr. et al. |
| 4,588,394 A | 5/1986 | Schulte et al. | 4,911,173 A | 3/1990 | Terwilliger |
| 4,593,687 A | 6/1986 | Gray | 4,911,174 A | 3/1990 | Pederson et al. |
| 4,595,012 A | 6/1986 | Webler et al. | 4,924,870 A | 5/1990 | Wlodarczyk et al. |
| 4,601,706 A | 7/1986 | Aillon | 4,943,770 A | 7/1990 | Ashley-Rollman et al. |
| 4,608,989 A | 9/1986 | Drue | 4,945,305 A | 7/1990 | Blood |
| 4,608,992 A | 9/1986 | Hakim et al. | 4,947,852 A | 8/1990 | Nassi et al. |
| 4,619,247 A | 10/1986 | Inoue et al. | 4,957,111 A | 9/1990 | Millar |
| 4,622,644 A | 11/1986 | Hansen | 4,961,433 A | 10/1990 | Christian |
| 4,644,960 A | 2/1987 | Johans | 4,966,148 A | 10/1990 | Millar |
| 4,652,820 A | 3/1987 | Maresca | 4,967,753 A | 11/1990 | Haase et al. |
| 4,665,925 A | 5/1987 | Millar | 4,977,886 A | 12/1990 | Takehana et al. |
| 4,667,230 A | 5/1987 | Arakawa et al. | 4,989,608 A | 2/1991 | Ratner |
| 4,674,518 A | 6/1987 | Salo | 4,995,396 A | 2/1991 | Inaba et al. |
| 4,676,249 A | 6/1987 | Arenas et al. | 4,998,916 A | 3/1991 | Hammerslag et al. |
| 4,681,106 A | 7/1987 | Kensley et al. | 5,005,592 A | 4/1991 | Carmell |
| 4,681,117 A | 7/1987 | Brodman et al. | 5,016,173 A | 5/1991 | Kenet et al. |
| 4,688,578 A | 8/1987 | Takano et al. | 5,025,799 A | 6/1991 | Wilson |
| 4,692,148 A | 9/1987 | Kantrowitz et al. | 5,029,585 A | 7/1991 | Lieber et al. |
| 4,697,595 A | 10/1987 | Breyer et al. | 5,040,548 A | 8/1991 | Yock |
| 4,700,997 A | 10/1987 | Strand | 5,042,486 A | 8/1991 | Pfeiler et al. |
| 4,706,681 A | 11/1987 | Breyer et al. | 5,045,071 A | 9/1991 | McCormick et al. |
| 4,710,708 A | 12/1987 | Rorden et al. | 5,046,497 A | 9/1991 | Millar |
| | | | 5,050,607 A | 9/1991 | Bradley et al. |
| | | | 5,057,095 A | 10/1991 | Fabian |
| | | | 5,058,595 A | 10/1991 | Kern |
| | | | 5,067,489 A | 11/1991 | Lind |
| | | | 5,076,278 A | 12/1991 | Vilkomerson et al. |
| | | | 5,078,140 A | 1/1992 | Kwoh |
| | | | 5,078,148 A | 1/1992 | Nassi et al. |
| | | | 5,078,149 A | 1/1992 | Katsumata et al. |
| | | | 5,078,678 A | 1/1992 | Katims |
| | | | 5,078,714 A | 1/1992 | Katims |
| | | | 5,084,022 A | 1/1992 | Claude |
| | | | 5,092,341 A | 3/1992 | Kelen |
| | | | 5,099,845 A | 3/1992 | Besz et al. |
| | | | 5,099,850 A | 3/1992 | Matsui et al. |
| | | | 5,100,387 A | 3/1992 | Ng |
| | | | 5,105,829 A | 4/1992 | Fabian et al. |
| | | | 5,109,862 A | 5/1992 | Kelen et al. |
| | | | 5,114,401 A | 5/1992 | Stuart et al. |
| | | | 5,121,750 A | 6/1992 | Katims |
| | | | 5,134,370 A | 7/1992 | Jefferts et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|-------------|---------|--------------------|-------------|---------|--------------------|
| 5,144,955 A | 9/1992 | O'Hara | 5,429,617 A | 7/1995 | Hammersmark et al. |
| 5,158,086 A | 10/1992 | Brown et al. | 5,431,641 A | 7/1995 | Grozinger et al. |
| 5,160,342 A | 11/1992 | Reger et al. | 5,433,729 A | 7/1995 | Adams et al. |
| 5,161,536 A | 11/1992 | Vilkomerson et al. | 5,437,276 A | 8/1995 | Takada et al. |
| 5,174,295 A | 12/1992 | Christian et al. | 5,437,277 A | 8/1995 | Dumoulin et al. |
| 5,184,601 A | 2/1993 | Putman | 5,438,873 A | 8/1995 | Wlodarczyk et al. |
| 5,190,045 A | 3/1993 | Frazin | 5,443,066 A | 8/1995 | Dumoulin et al. |
| 5,202,985 A | 4/1993 | Goyal | 5,443,489 A | 8/1995 | Ben-Haim |
| 5,211,165 A | 5/1993 | Dumoulin et al. | 5,445,150 A | 8/1995 | Dumoulin et al. |
| 5,211,636 A | 5/1993 | Mische | 5,445,166 A | 8/1995 | Taylor |
| 5,212,988 A | 5/1993 | White et al. | 5,450,846 A | 9/1995 | Goldreyer |
| 5,214,615 A | 5/1993 | Bauer et al. | 5,453,575 A | 9/1995 | O'Donnell et al. |
| 5,217,026 A | 6/1993 | Stoy et al. | 5,456,256 A | 10/1995 | Schneider |
| 5,220,924 A | 6/1993 | Frazin | 5,456,718 A | 10/1995 | Szymaitis |
| 5,235,987 A | 8/1993 | Wolfe | 5,464,016 A | 11/1995 | Nicholas et al. |
| 5,239,464 A | 8/1993 | Blair et al. | 5,474,065 A | 12/1995 | Meathrel et al. |
| 5,240,004 A | 8/1993 | Walinsky et al. | 5,476,090 A | 12/1995 | Kishi |
| 5,243,995 A | 9/1993 | Maier | 5,480,422 A | 1/1996 | Ben-Haim |
| 5,246,007 A | 9/1993 | Frisbie et al. | 5,487,729 A | 1/1996 | Avellanet et al. |
| 5,247,171 A | 9/1993 | Wlodarczyk et al. | 5,490,522 A | 2/1996 | Dardel |
| 5,251,635 A | 10/1993 | Dumoulin et al. | 5,492,538 A | 2/1996 | Johlin, Jr. |
| 5,255,680 A | 10/1993 | Darrow et al. | 5,494,038 A | 2/1996 | Wang et al. |
| 5,257,636 A | 11/1993 | White | 5,500,012 A | 3/1996 | Brucker et al. |
| 5,257,979 A | 11/1993 | Jagpal | 5,505,205 A | 4/1996 | Solomon et al. |
| 5,261,409 A | 11/1993 | Dardel | 5,509,822 A | 4/1996 | Negus et al. |
| 5,265,610 A | 11/1993 | Darrow et al. | 5,513,637 A | 5/1996 | Twiss et al. |
| 5,265,614 A | 11/1993 | Hayakawa et al. | 5,515,160 A | 5/1996 | Schulz et al. |
| 5,267,569 A | 12/1993 | Lienhard | 5,515,853 A | 5/1996 | Smith et al. |
| 5,270,810 A | 12/1993 | Nishimura | 5,522,878 A | 6/1996 | Montecalvo et al. |
| 5,271,404 A | 12/1993 | Corl et al. | 5,526,812 A | 6/1996 | Dumoulin et al. |
| 5,273,025 A | 12/1993 | Sakiyama et al. | 5,531,664 A | 7/1996 | Adachi et al. |
| 5,273,042 A | 12/1993 | Lynch et al. | 5,540,230 A | 7/1996 | Vilkomerson |
| 5,274,551 A | 12/1993 | Corby, Jr. | 5,540,681 A | 7/1996 | Strul et al. |
| 5,275,053 A | 1/1994 | Wlodarczyk et al. | 5,542,938 A | 8/1996 | Avellanet et al. |
| 5,279,129 A | 1/1994 | Ito | 5,546,949 A | 8/1996 | Frazin et al. |
| 5,279,607 A | 1/1994 | Schentag et al. | 5,546,951 A | 8/1996 | Ben-Haim |
| 5,280,786 A | 1/1994 | Wlodarczyk et al. | 5,558,091 A | 9/1996 | Acker et al. |
| 5,287,331 A | 2/1994 | Schindel et al. | 5,568,809 A | 10/1996 | Ben-haim |
| 5,289,373 A | 2/1994 | Zarge et al. | D375,450 S | 11/1996 | Bidwell et al. |
| 5,292,342 A | 3/1994 | Nelson et al. | 5,570,671 A | 11/1996 | Hickey |
| 5,307,072 A | 4/1994 | Jones, Jr. | 5,575,291 A | 11/1996 | Hayakawa et al. |
| 5,311,871 A | 5/1994 | Yock | 5,588,442 A | 12/1996 | Scovil et al. |
| 5,313,949 A | 5/1994 | Yock | 5,592,939 A | 1/1997 | Martinelli |
| 5,318,025 A | 6/1994 | Dumoulin et al. | 5,598,846 A | 2/1997 | Peszynski |
| 5,325,860 A | 7/1994 | Seward et al. | 5,599,299 A | 2/1997 | Weaver et al. |
| 5,325,873 A | 7/1994 | Hirschi et al. | 5,600,330 A | 2/1997 | Blood |
| 5,330,496 A | 7/1994 | Alferness | 5,610,967 A | 3/1997 | Moorman et al. |
| 5,331,966 A | 7/1994 | Bennett et al. | 5,617,866 A | 4/1997 | Marian, Jr. |
| 5,333,614 A | 8/1994 | Feiring | 5,622,169 A | 4/1997 | Golden et al. |
| 5,337,678 A | 8/1994 | Grout et al. | 5,622,170 A | 4/1997 | Schulz |
| 5,341,807 A | 8/1994 | Nardella | 5,622,184 A | 4/1997 | Ashby et al. |
| 5,343,865 A | 9/1994 | Gardineer et al. | 5,623,931 A | 4/1997 | Wung et al. |
| 5,345,940 A | 9/1994 | Seward et al. | 5,624,430 A | 4/1997 | Eton et al. |
| 5,348,020 A | 9/1994 | Hutson | 5,626,554 A | 5/1997 | Ryaby et al. |
| 5,350,352 A | 9/1994 | Buchholtz et al. | 5,626,870 A | 5/1997 | Monshipouri et al. |
| 5,357,961 A | 10/1994 | Fields et al. | 5,630,419 A | 5/1997 | Ranalletta |
| 5,368,048 A | 11/1994 | Stoy et al. | 5,638,819 A | 6/1997 | Manwaring et al. |
| 5,375,596 A | 12/1994 | Twiss et al. | 5,644,612 A | 7/1997 | Moorman et al. |
| 5,376,083 A | 12/1994 | Mische | 5,645,065 A | 7/1997 | Shapiro et al. |
| 5,377,678 A | 1/1995 | Dumoulin et al. | 5,651,047 A | 7/1997 | Moorman et al. |
| 5,385,053 A | 1/1995 | Wlodarczyk et al. | 5,654,864 A | 8/1997 | Ritter et al. |
| 5,391,199 A | 2/1995 | Ben-Haim | D383,968 S | 9/1997 | Bidwell et al. |
| 5,394,876 A | 3/1995 | Ma | 5,662,115 A | 9/1997 | Torp et al. |
| 5,394,877 A | 3/1995 | Orr et al. | 5,665,477 A | 9/1997 | Meathrel et al. |
| 5,395,366 A | 3/1995 | D'Andrea et al. | 5,666,473 A | 9/1997 | Wallace |
| 5,398,683 A | 3/1995 | Edwards et al. | 5,666,958 A | 9/1997 | Rothenberg et al. |
| 5,398,691 A | 3/1995 | Martin et al. | 5,669,383 A | 9/1997 | Johnson |
| 5,411,485 A | 5/1995 | Tennican et al. | 5,669,388 A | 9/1997 | Vilkomerson |
| 5,413,107 A | 5/1995 | Oakley et al. | 5,676,159 A | 10/1997 | Navis |
| 5,422,478 A | 6/1995 | Wlodarczyk et al. | 5,676,673 A | 10/1997 | Ferre et al. |
| 5,425,367 A | 6/1995 | Shapiro et al. | 5,682,890 A | 11/1997 | Kormos et al. |
| 5,425,370 A | 6/1995 | Vilkomerson | 5,691,898 A | 11/1997 | Rosenberg et al. |
| 5,425,382 A | 6/1995 | Golden et al. | 5,694,945 A | 12/1997 | Ben-Haim |
| 5,427,114 A | 6/1995 | Colliver et al. | 5,695,479 A | 12/1997 | Jagpal |
| 5,429,132 A | 7/1995 | Guy et al. | 5,697,377 A | 12/1997 | Wittkampf |
| | | | 5,699,801 A | 12/1997 | Atalar et al. |
| | | | 5,700,889 A | 12/1997 | Blair |
| | | | 5,711,299 A | 1/1998 | Manwaring et al. |
| | | | 5,713,362 A | 2/1998 | Vilkomerson |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|---------------|---------|-------------------------------|-------------|---------|-----------------------|
| 5,713,363 A | 2/1998 | Seward et al. | 5,873,822 A | 2/1999 | Ferre et al. |
| 5,713,858 A | 2/1998 | Heruth et al. | 5,876,328 A | 3/1999 | Fox et al. |
| 5,713,946 A | 2/1998 | Ben-Haim | 5,879,297 A | 3/1999 | Haynor et al. |
| 5,715,817 A | 2/1998 | Stevens-Wright et al. | 5,893,363 A | 4/1999 | Little et al. |
| 5,716,389 A | 2/1998 | Walinsky et al. | 5,897,495 A | 4/1999 | Aida et al. |
| 5,718,241 A | 2/1998 | Ben-Haim et al. | 5,899,860 A | 5/1999 | Pfeiffer et al. |
| D391,838 S | 3/1998 | Bidwell et al. | 5,902,238 A | 5/1999 | Golden et al. |
| 5,722,412 A | 3/1998 | Pflugrath et al. | 5,907,487 A | 5/1999 | Rosenberg et al. |
| 5,727,550 A | 3/1998 | Montecalvo | 5,908,385 A | 6/1999 | Chechelski et al. |
| 5,727,552 A | 3/1998 | Ryan | 5,910,113 A | 6/1999 | Pruter |
| 5,727,553 A | 3/1998 | Saad | 5,910,120 A | 6/1999 | Kim et al. |
| 5,729,055 A | 3/1998 | Manning | 5,913,820 A | 6/1999 | Bladen et al. |
| 5,729,129 A | 3/1998 | Acker | 5,913,830 A | 6/1999 | Miles |
| 5,729,584 A | 3/1998 | Moorman et al. | 5,919,141 A | 7/1999 | Money et al. |
| 5,730,129 A | 3/1998 | Darrow et al. | 5,919,170 A | 7/1999 | Woessner |
| 5,731,996 A | 3/1998 | Gilbert | 5,928,145 A | 7/1999 | Ocali et al. |
| 5,733,323 A | 3/1998 | Buck et al. | 5,929,607 A | 7/1999 | Rosenberg et al. |
| 5,738,096 A | 4/1998 | Ben-Haim | 5,931,788 A | 8/1999 | Keen et al. |
| 5,740,808 A | 4/1998 | Panescu et al. | 5,931,818 A | 8/1999 | Werp et al. |
| 5,742,394 A | 4/1998 | Hansen | 5,941,858 A | 8/1999 | Johnson |
| 5,744,953 A | 4/1998 | Hansen | 5,941,889 A | 8/1999 | Cermak |
| 5,748,767 A | 5/1998 | Raab | 5,941,904 A | 8/1999 | Johnston et al. |
| 5,749,835 A | 5/1998 | Glantz | 5,944,022 A | 8/1999 | Nardella et al. |
| 5,749,938 A | 5/1998 | Coombs | 5,944,023 A | 8/1999 | Johnson et al. |
| 5,751,785 A | 5/1998 | Moorman et al. | 5,953,683 A | 9/1999 | Hansen et al. |
| 5,752,513 A | 5/1998 | Acker et al. | 5,957,857 A | 9/1999 | Hartley |
| 5,758,650 A | 6/1998 | Miller et al. | 5,961,923 A | 10/1999 | Nova et al. |
| 5,762,064 A | 6/1998 | Polvani | 5,967,978 A | 10/1999 | Littmann et al. |
| 5,767,669 A | 6/1998 | Hansen et al. | 5,967,980 A | 10/1999 | Ferre et al. |
| 5,767,960 A | 6/1998 | Orman et al. | 5,967,991 A | 10/1999 | Gardineer et al. |
| 5,769,786 A | 6/1998 | Wiegel | 5,969,722 A | 10/1999 | Palm |
| 5,769,843 A | 6/1998 | Abela et al. | 5,978,705 A | 11/1999 | KenKnight et al. |
| 5,769,881 A | 6/1998 | Schroepel et al. | 5,983,126 A | 11/1999 | Wittkamp |
| 5,771,896 A | 6/1998 | Sliwa, Jr. et al. | 5,984,908 A | 11/1999 | Davis et al. |
| 5,775,322 A | 7/1998 | Silverstein et al. | 5,991,693 A | 11/1999 | Zalewski |
| 5,775,332 A | 7/1998 | Goldman | 5,997,473 A | 12/1999 | Taniguchi et al. |
| 5,776,064 A | 7/1998 | Kalfas et al. | 5,997,481 A | 12/1999 | Adams et al. |
| 5,779,638 A | 7/1998 | Vesely et al. | 6,006,123 A | 12/1999 | Nguyen et al. |
| 5,782,767 A | 7/1998 | Pretlow, III | 6,011,988 A | 1/2000 | Lynch et al. |
| 5,785,657 A | 7/1998 | Breyer et al. | 6,014,473 A | 1/2000 | Hossack et al. |
| 5,792,055 A | 8/1998 | McKinnon et al. | 6,014,580 A | 1/2000 | Blume et al. |
| 5,795,297 A | 8/1998 | Daigle | 6,015,414 A | 1/2000 | Werp et al. |
| 5,795,298 A | 8/1998 | Vesely et al. | 6,017,496 A | 1/2000 | Nova et al. |
| 5,795,632 A | 8/1998 | Buchalter | 6,019,724 A | 2/2000 | Gronningsaeter et al. |
| 5,797,849 A | 8/1998 | Vesely et al. | 6,019,725 A | 2/2000 | Vesely et al. |
| 5,800,352 A | 9/1998 | Ferre et al. | 6,023,638 A | 2/2000 | Swanson |
| 5,800,410 A | 9/1998 | Gawreluk | 6,026,312 A | 2/2000 | Shemwell et al. |
| 5,800,497 A | 9/1998 | Bakels et al. | 6,031,765 A | 2/2000 | Lee et al. |
| 5,803,089 A | 9/1998 | Ferre et al. | 6,032,070 A | 2/2000 | Flock et al. |
| 5,810,733 A | 9/1998 | Van Creveld et al. | 6,039,694 A | 3/2000 | Larson et al. |
| 5,817,022 A | 10/1998 | Vesely | 6,050,718 A | 4/2000 | Schena et al. |
| 5,817,024 A | 10/1998 | Ogle et al. | 6,052,610 A | 4/2000 | Koch |
| 5,820,549 A | 10/1998 | Marian, Jr. | 6,052,618 A | 4/2000 | Dahlke et al. |
| 5,824,031 A | 10/1998 | Cookston et al. | D424,693 S | 5/2000 | Pruter |
| 5,829,444 A | 11/1998 | Ferre et al. | 6,059,718 A | 5/2000 | Taniguchi et al. |
| 5,830,145 A | 11/1998 | Tenhoff | 6,064,905 A | 5/2000 | Webster, Jr. et al. |
| 5,831,260 A | 11/1998 | Hansen | 6,066,094 A | 5/2000 | Ben-Haim |
| 5,833,608 A | 11/1998 | Acker | 6,068,599 A | 5/2000 | Saito et al. |
| 5,833,622 A | 11/1998 | Meathrel et al. | 6,073,043 A | 6/2000 | Schneider |
| 5,835,561 A | 11/1998 | Moorman et al. | 6,074,367 A | 6/2000 | Hubbell |
| 5,836,882 A | 11/1998 | Frazin | 6,075,442 A | 6/2000 | Welch |
| 5,836,990 A | 11/1998 | Li | 6,076,007 A | 6/2000 | England et al. |
| 5,840,024 A * | 11/1998 | Taniguchi et al. 600/424 | 6,082,366 A | 7/2000 | Andra et al. |
| 5,840,025 A | 11/1998 | Ben-Haim | 6,083,170 A | 7/2000 | Ben-Haim |
| 5,840,030 A | 11/1998 | Ferek-Petric et al. | 6,099,524 A | 8/2000 | Lipson et al. |
| 5,840,031 A | 11/1998 | Crowley | 6,100,026 A | 8/2000 | Nova et al. |
| 5,842,986 A | 12/1998 | Avrin et al. | 6,102,044 A | 8/2000 | Naidyhorski |
| 5,843,076 A | 12/1998 | Webster, Jr. et al. | 6,107,699 A | 8/2000 | Swanson |
| 5,843,153 A | 12/1998 | Johnston et al. | 6,112,111 A | 8/2000 | Glantz |
| 5,844,140 A | 12/1998 | Seale | 6,113,504 A | 9/2000 | Kuesters |
| 5,846,198 A | 12/1998 | Killmann | 6,115,624 A | 9/2000 | Lewis et al. |
| 5,855,553 A | 1/1999 | Tajima et al. | 6,120,445 A | 9/2000 | Grunwald |
| 5,859,893 A | 1/1999 | Moorman et al. | 6,128,174 A | 10/2000 | Ritter et al. |
| 5,865,748 A | 2/1999 | Co et al. | 6,129,668 A | 10/2000 | Haynor et al. |
| 5,868,673 A | 2/1999 | Vesely | 6,132,378 A | 10/2000 | Marino |
| | | | 6,132,379 A | 10/2000 | Patacsil et al. |
| | | | 6,135,961 A | 10/2000 | Pflugrath et al. |
| | | | 6,136,274 A | 10/2000 | Nova et al. |
| | | | 6,138,681 A | 10/2000 | Chen et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|--------------|---------|----------------------|--------------|---------|-----------------------|
| 6,139,496 A | 10/2000 | Chen et al. | 6,332,089 B1 | 12/2001 | Acker et al. |
| 6,139,502 A | 10/2000 | Fredriksen | 6,332,874 B1 | 12/2001 | Eliassen et al. |
| 6,144,300 A | 11/2000 | Dames et al. | 6,340,588 B1 | 1/2002 | Nova et al. |
| 6,148,823 A | 11/2000 | Hastings | 6,340,868 B1 | 1/2002 | Lys et al. |
| 6,152,933 A | 11/2000 | Werp et al. | 6,341,231 B1 | 1/2002 | Ferre et al. |
| 6,157,853 A | 12/2000 | Blume et al. | 6,346,081 B1 | 2/2002 | Vilkomerson |
| 6,165,144 A | 12/2000 | Talish et al. | 6,348,911 B1 | 2/2002 | Rosenberg et al. |
| 6,166,496 A | 12/2000 | Lys et al. | 6,350,160 B1 | 2/2002 | Feuersanger et al. |
| 6,166,806 A | 12/2000 | Tjin | 6,352,363 B1 | 3/2002 | Munger et al. |
| 6,167,765 B1 | 1/2001 | Weitzel | 6,355,026 B1 | 3/2002 | Mick |
| 6,172,499 B1 | 1/2001 | Ashe | 6,361,499 B1 | 3/2002 | Bates et al. |
| 6,173,199 B1 | 1/2001 | Gabriel | 6,364,823 B1 | 4/2002 | Garibaldi et al. |
| 6,173,715 B1 | 1/2001 | Sinanan et al. | 6,364,839 B1 | 4/2002 | Little et al. |
| 6,175,756 B1 | 1/2001 | Ferre et al. | 6,366,804 B1 | 4/2002 | Mejia |
| 6,176,829 B1 | 1/2001 | Vilkomerson | 6,368,285 B1 | 4/2002 | Osadchy et al. |
| 6,193,743 B1 | 2/2001 | Brayton et al. | 6,370,411 B1 | 4/2002 | Osadchy et al. |
| 6,200,305 B1 | 3/2001 | Berthiaume et al. | 6,373,240 B1 | 4/2002 | Govari |
| 6,203,499 B1 | 3/2001 | Imling et al. | 6,373,388 B1 | 4/2002 | Dames et al. |
| 6,208,884 B1 | 3/2001 | Kumar et al. | 6,374,134 B1 | 4/2002 | Bladen et al. |
| 6,211,626 B1 | 4/2001 | Lys et al. | 6,374,670 B1 | 4/2002 | Spelman et al. |
| 6,211,666 B1 | 4/2001 | Acker | 6,375,606 B1 | 4/2002 | Garibaldi et al. |
| 6,212,426 B1 | 4/2001 | Swanson | 6,375,639 B1 | 4/2002 | Duplessie et al. |
| 6,216,027 B1 | 4/2001 | Willis et al. | 6,377,857 B1 | 4/2002 | Brayton et al. |
| 6,216,028 B1 | 4/2001 | Haynor et al. | 6,379,302 B1 | 4/2002 | Kessman et al. |
| 6,216,029 B1 | 4/2001 | Paltiel | 6,379,303 B1 | 4/2002 | Seitz et al. |
| 6,223,087 B1 | 4/2001 | Williams | 6,379,307 B1 | 4/2002 | Filly et al. |
| 6,226,547 B1 | 5/2001 | Lockhart et al. | 6,381,485 B1 | 4/2002 | Hunter et al. |
| 6,230,042 B1 | 5/2001 | Slettenmark | 6,385,472 B1 | 5/2002 | Hall et al. |
| 6,230,046 B1 | 5/2001 | Crane et al. | 6,385,476 B1 | 5/2002 | Osadchy et al. |
| 6,233,476 B1 | 5/2001 | Strommer et al. | 6,398,736 B1 | 6/2002 | Seward |
| 6,236,883 B1 | 5/2001 | Ciaccio et al. | 6,401,723 B1 | 6/2002 | Garibaldi et al. |
| 6,238,344 B1 | 5/2001 | Gamelsky et al. | 6,406,442 B1 | 6/2002 | McFann et al. |
| 6,241,673 B1 | 6/2001 | Williams | 6,412,978 B1 | 7/2002 | Watanabe et al. |
| 6,246,231 B1 | 6/2001 | Ashe | 6,412,980 B1 | 7/2002 | Lounsberry et al. |
| 6,246,898 B1 | 6/2001 | Vesely et al. | 6,417,839 B1 | 7/2002 | Odell |
| 6,248,072 B1 | 6/2001 | Murkin | 6,418,332 B1 | 7/2002 | Mastrototaro et al. |
| 6,248,074 B1 | 6/2001 | Ohno et al. | 6,418,335 B2 | 7/2002 | Avrin et al. |
| 6,248,075 B1 | 6/2001 | McGee et al. | 6,423,002 B1 | 7/2002 | Hossack |
| 6,253,770 B1 | 7/2001 | Acker et al. | 6,423,050 B1 | 7/2002 | Twardowski |
| 6,259,941 B1 | 7/2001 | Chia et al. | 6,427,079 B1 | 7/2002 | Schneider et al. |
| 6,261,231 B1 | 7/2001 | Damphousse et al. | 6,428,551 B1 | 8/2002 | Hall et al. |
| 6,263,230 B1 | 7/2001 | Haynor et al. | 6,430,315 B1 | 8/2002 | Makram-Ebeid |
| 6,266,550 B1 | 7/2001 | Selmon et al. | 6,432,069 B1 | 8/2002 | Godo et al. |
| 6,266,551 B1 | 7/2001 | Osadchy et al. | 6,438,411 B1 | 8/2002 | Guttman et al. |
| 6,266,552 B1 | 7/2001 | Slettenmark | 6,442,416 B1 | 8/2002 | Schultz |
| 6,266,563 B1 | 7/2001 | KenKnight et al. | 6,445,943 B1 | 9/2002 | Ferre et al. |
| 6,271,833 B1 | 8/2001 | Rosenberg et al. | 6,459,919 B1 | 10/2002 | Lys et al. |
| 6,272,371 B1 | 8/2001 | Shlomo | 6,463,121 B1 | 10/2002 | Milnes |
| 6,272,374 B1 | 8/2001 | Flock et al. | 6,466,815 B1 | 10/2002 | Saito et al. |
| 6,275,258 B1 | 8/2001 | Chim | 6,473,167 B1 | 10/2002 | Odell |
| 6,275,724 B1 | 8/2001 | Dickinson et al. | 6,474,341 B1 | 11/2002 | Hunter et al. |
| 6,277,077 B1 | 8/2001 | Brisken et al. | 6,475,152 B1 | 11/2002 | Kelly, Jr. et al. |
| 6,284,459 B1 | 9/2001 | Nova et al. | 6,475,223 B1 | 11/2002 | Werp et al. |
| 6,285,898 B1 | 9/2001 | Ben-Haim | 6,477,402 B1 | 11/2002 | Lynch et al. |
| 6,288,704 B1 | 9/2001 | Flack et al. | 6,484,118 B1 | 11/2002 | Govari et al. |
| 6,292,678 B1 | 9/2001 | Hall et al. | 6,487,916 B1 | 12/2002 | Gomm et al. |
| 6,292,680 B1 | 9/2001 | Somogyi et al. | 6,491,671 B1 | 12/2002 | Larson, III et al. |
| 6,292,901 B1 | 9/2001 | Lys et al. | 6,493,573 B1 | 12/2002 | Martinelli et al. |
| 6,293,955 B1 | 9/2001 | Houser et al. | 6,496,715 B1 | 12/2002 | Lee et al. |
| 6,296,604 B1 | 10/2001 | Garibaldi et al. | 6,498,944 B1 | 12/2002 | Ben-Haim et al. |
| 6,298,261 B1 | 10/2001 | Rex | 6,500,141 B1 | 12/2002 | Irion et al. |
| 6,304,768 B1 | 10/2001 | Blume et al. | 6,505,062 B1 | 1/2003 | Ritter et al. |
| 6,306,097 B1 | 10/2001 | Park et al. | 6,507,751 B2 | 1/2003 | Blume et al. |
| 6,311,082 B1 | 10/2001 | Creighton, IV et al. | 6,508,802 B1 | 1/2003 | Rosengart et al. |
| 6,315,709 B1 | 11/2001 | Garibaldi et al. | 6,512,958 B1 | 1/2003 | Swoyer et al. |
| 6,315,727 B1 | 11/2001 | Coleman et al. | 6,514,249 B1 | 2/2003 | Maguire et al. |
| 6,319,668 B1 | 11/2001 | Nova et al. | 6,515,657 B1 | 2/2003 | Zanelli |
| 6,323,769 B1 | 11/2001 | Dames et al. | 6,516,212 B1 | 2/2003 | Bladen et al. |
| 6,323,770 B1 | 11/2001 | Dames et al. | 6,516,231 B1 | 2/2003 | Flammang |
| 6,324,416 B1 | 11/2001 | Seibert | 6,516,807 B1 | 2/2003 | Panescu et al. |
| 6,325,540 B1 | 12/2001 | Lounsberry et al. | 6,517,520 B2 | 2/2003 | Chang et al. |
| 6,325,762 B1 | 12/2001 | Tjin | 6,522,906 B1 | 2/2003 | Salisbury, Jr. et al. |
| 6,329,139 B1 | 12/2001 | Nova et al. | 6,522,907 B1 | 2/2003 | Bladen et al. |
| 6,329,916 B1 | 12/2001 | Dames et al. | 6,522,909 B1 | 2/2003 | Garibaldi et al. |
| 6,330,467 B1 | 12/2001 | Creighton, IV et al. | 6,524,303 B1 | 2/2003 | Garibaldi |
| | | | 6,528,954 B1 | 3/2003 | Lys et al. |
| | | | 6,528,991 B2 | 3/2003 | Ashe |
| | | | 6,529,761 B2 | 3/2003 | Creighton, IV et al. |
| | | | 6,529,766 B1 | 3/2003 | Guendel |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | | | |
|-----------|----|---------|-----------------------|-----------|----|---------|-----------------------|
| 6,534,982 | B1 | 3/2003 | Jakab | 6,755,789 | B2 | 6/2004 | Stringer et al. |
| 6,535,625 | B1 | 3/2003 | Chang et al. | 6,755,816 | B2 | 6/2004 | Ritter et al. |
| 6,537,192 | B1 | 3/2003 | Elliott et al. | 6,755,822 | B2 | 6/2004 | Reu et al. |
| 6,537,196 | B1 | 3/2003 | Creighton, IV et al. | 6,757,557 | B1 | 6/2004 | Bladen et al. |
| 6,538,634 | B1 | 3/2003 | Chui et al. | 6,763,261 | B2 | 7/2004 | Casscells, III et al. |
| 6,540,699 | B1 | 4/2003 | Smith et al. | 6,764,449 | B2 | 7/2004 | Lee et al. |
| 6,542,766 | B2 | 4/2003 | Hall et al. | 6,768,496 | B2 | 7/2004 | Bieger et al. |
| 6,544,251 | B1 | 4/2003 | Crawford | 6,772,001 | B2 | 8/2004 | Maschke et al. |
| 6,546,270 | B1 | 4/2003 | Goldin et al. | 6,774,624 | B2 | 8/2004 | Anderson et al. |
| 6,546,279 | B1 | 4/2003 | Bova et al. | 6,783,536 | B2 | 8/2004 | Vilsmeier et al. |
| 6,546,787 | B1 | 4/2003 | Schiller et al. | 6,784,660 | B2 | 8/2004 | Ashe |
| 6,552,841 | B1 | 4/2003 | Lasser et al. | 6,785,571 | B2 | 8/2004 | Glossop et al. |
| 6,556,858 | B1 | 4/2003 | Zeman | 6,786,219 | B2 | 9/2004 | Garibaldi et al. |
| 6,562,019 | B1 | 5/2003 | Sell | 6,788,967 | B2 | 9/2004 | Ben-Haim et al. |
| 6,564,087 | B1 | 5/2003 | Pitris et al. | 6,794,667 | B2 | 9/2004 | Noshi |
| 6,569,101 | B2 | 5/2003 | Quistgaard et al. | 6,799,066 | B2 | 9/2004 | Steines et al. |
| 6,569,160 | B1 | 5/2003 | Goldin et al. | 6,815,651 | B2 | 11/2004 | Odell |
| 6,571,004 | B1 | 5/2003 | Florent et al. | 6,816,266 | B2 | 11/2004 | Varshneya et al. |
| 6,574,518 | B1 | 6/2003 | Lounsberry et al. | 6,817,364 | B2 | 11/2004 | Garibaldi |
| 6,575,908 | B2 | 6/2003 | Barnes et al. | 6,834,201 | B2 | 12/2004 | Gillies et al. |
| 6,577,080 | B2 | 6/2003 | Lys et al. | 6,844,713 | B2 | 1/2005 | Steber et al. |
| 6,577,896 | B2 | 6/2003 | Werner et al. | 6,845,142 | B2 | 1/2005 | Ohishi |
| 6,584,343 | B1 | 6/2003 | Ransbury et al. | 6,856,823 | B2 | 2/2005 | Ashe |
| 6,593,754 | B1 | 7/2003 | Steber et al. | 6,860,422 | B2 | 3/2005 | Hull et al. |
| 6,593,884 | B1 | 7/2003 | Gilboa et al. | 6,862,467 | B2 | 3/2005 | Moore et al. |
| 6,597,943 | B2 | 7/2003 | Taha et al. | 6,869,390 | B2 | 3/2005 | Elliott et al. |
| 6,599,249 | B1 | 7/2003 | Nordgren et al. | 6,875,179 | B2 | 4/2005 | Ferguson et al. |
| 6,607,488 | B1 | 8/2003 | Jackson et al. | 6,879,160 | B2 | 4/2005 | Jakab |
| 6,610,058 | B2 | 8/2003 | Flores | 6,889,091 | B2 | 5/2005 | Hine et al. |
| 6,611,141 | B1 | 8/2003 | Schulz et al. | 6,895,268 | B1 | 5/2005 | Rahn et al. |
| 6,615,071 | B1 | 9/2003 | Casscells, III et al. | 6,902,528 | B1 | 6/2005 | Garibaldi et al. |
| 6,615,155 | B2 | 9/2003 | Gilboa | 6,908,433 | B1 | 6/2005 | Pruter |
| 6,616,610 | B2 | 9/2003 | Steininger et al. | 6,911,026 | B1 | 6/2005 | Hall et al. |
| 6,618,612 | B1 | 9/2003 | Acker et al. | 6,923,782 | B2 | 8/2005 | O'Mahony et al. |
| 6,626,832 | B1 | 9/2003 | Paltiel et al. | 6,926,673 | B2 | 8/2005 | Roberts et al. |
| 6,626,834 | B2 | 9/2003 | Dunne et al. | 6,934,575 | B2 | 8/2005 | Ferre et al. |
| 6,626,902 | B1 | 9/2003 | Kucharczyk et al. | 6,936,010 | B2 | 8/2005 | Fang et al. |
| 6,630,879 | B1 | 10/2003 | Creighton, IV et al. | 6,940,379 | B2 | 9/2005 | Creighton |
| 6,635,027 | B1 | 10/2003 | Cragg et al. | 6,941,166 | B2 | 9/2005 | MacAdam et al. |
| 6,645,148 | B2 | 11/2003 | Nguyen-Dinh et al. | 6,947,788 | B2 | 9/2005 | Gilboa et al. |
| 6,648,875 | B2 | 11/2003 | Simpson et al. | 6,950,689 | B1 | 9/2005 | Willis et al. |
| 6,649,914 | B1 | 11/2003 | Moorman et al. | 6,953,754 | B2 | 10/2005 | Machida et al. |
| 6,652,506 | B2 | 11/2003 | Bowe et al. | 6,958,677 | B1 | 10/2005 | Carter |
| 6,660,024 | B1 | 12/2003 | Flaherty et al. | 6,959,214 | B2 | 10/2005 | Pape et al. |
| 6,662,034 | B2 | 12/2003 | Segner et al. | 6,962,566 | B2 | 11/2005 | Quistgaard et al. |
| 6,672,308 | B1 | 1/2004 | Gaspari | 6,968,846 | B2 | 11/2005 | Viswanathan |
| 6,677,752 | B1 | 1/2004 | Creighton, IV et al. | 6,975,197 | B2 | 12/2005 | Creighton, IV |
| 6,679,857 | B1 | 1/2004 | Bastia et al. | 6,976,962 | B2 | 12/2005 | Bullis |
| 6,684,176 | B2 | 1/2004 | Willins et al. | 6,976,987 | B2 | 12/2005 | Flores |
| 6,685,644 | B2 | 2/2004 | Seo | 6,980,843 | B2 | 12/2005 | Eng et al. |
| 6,687,531 | B1 | 2/2004 | Ferre et al. | 6,980,852 | B2 | 12/2005 | Jersey-Willuhn et al. |
| 6,689,119 | B1 | 2/2004 | Di Caprio et al. | 6,980,921 | B2 | 12/2005 | Anderson et al. |
| 6,690,963 | B2 | 2/2004 | Ben-Haim et al. | 6,986,739 | B2 | 1/2006 | Warren et al. |
| 6,690,964 | B2 | 2/2004 | Bieger et al. | 6,999,821 | B2 | 2/2006 | Jenney et al. |
| 6,690,968 | B2 | 2/2004 | Mejia | 7,001,355 | B2 | 2/2006 | Nunomura et al. |
| 6,694,167 | B1 | 2/2004 | Ferre et al. | 7,008,418 | B2 | 3/2006 | Hall et al. |
| 6,695,786 | B2 | 2/2004 | Wang et al. | 7,010,338 | B2 | 3/2006 | Ritter et al. |
| 6,701,179 | B1 | 3/2004 | Martinelli et al. | 7,015,393 | B2 | 3/2006 | Weiner et al. |
| 6,701,918 | B2 | 3/2004 | Fariss et al. | 7,017,584 | B2 | 3/2006 | Garibaldi et al. |
| 6,702,804 | B1 | 3/2004 | Ritter et al. | 7,019,610 | B2 | 3/2006 | Creighton, IV et al. |
| 6,704,590 | B2 | 3/2004 | Haldeman | 7,020,512 | B2 | 3/2006 | Ritter et al. |
| 6,709,390 | B1 | 3/2004 | Marie Pop | D518,574 | S | 4/2006 | Chaggares |
| 6,711,429 | B1 | 3/2004 | Gilboa et al. | 7,022,075 | B2 | 4/2006 | Grunwald et al. |
| 6,711,431 | B2 | 3/2004 | Sarin et al. | 7,022,082 | B2 | 4/2006 | Sonek |
| 6,719,699 | B2 | 4/2004 | Smith | 7,026,927 | B2 | 4/2006 | Wright et al. |
| 6,719,724 | B1 | 4/2004 | Walker et al. | 7,027,634 | B2 | 4/2006 | Odell |
| 6,719,756 | B1 | 4/2004 | Muntermann | 7,028,387 | B1 | 4/2006 | Huynh et al. |
| 6,720,745 | B2 | 4/2004 | Lys et al. | 7,029,446 | B2 | 4/2006 | Wendelken et al. |
| 6,733,458 | B1 | 5/2004 | Steins et al. | 7,033,603 | B2 | 4/2006 | Nelson et al. |
| 6,733,511 | B2 | 5/2004 | Hall et al. | D520,139 | S | 5/2006 | Chaggares |
| 6,736,782 | B2 | 5/2004 | Pfeiffer et al. | D520,140 | S | 5/2006 | Chaggares |
| 6,738,656 | B1 | 5/2004 | Ferre et al. | 7,038,398 | B1 | 5/2006 | Lys et al. |
| 6,740,103 | B2 | 5/2004 | Hall et al. | 7,038,657 | B2 | 5/2006 | Rosenberg et al. |
| 6,743,177 | B2 | 6/2004 | Ito et al. | 7,043,293 | B1 | 5/2006 | Baura |
| 6,754,596 | B2 | 6/2004 | Ashe | 7,048,733 | B2 | 5/2006 | Hartley et al. |
| | | | | 7,054,228 | B1 | 5/2006 | Hickling |
| | | | | 7,066,914 | B2 | 6/2006 | Andersen |
| | | | | 7,066,924 | B1 | 6/2006 | Garibaldi et al. |
| | | | | D525,363 | S | 7/2006 | Chaggares |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|--------------|---------|-----------------------|-----------------|---------|----------------------|
| 7,070,565 B2 | 7/2006 | Vaezy et al. | 7,479,141 B2 | 1/2009 | Kleen et al. |
| 7,072,704 B2 | 7/2006 | Bucholz | 7,534,223 B2 | 5/2009 | Boutillette et al. |
| 7,082,325 B2 | 7/2006 | Hashimshony et al. | 7,538,859 B2 | 5/2009 | Tearney et al. |
| 7,090,639 B2 | 8/2006 | Govari | 7,543,239 B2 | 6/2009 | Viswanathan et al. |
| 7,096,059 B2 | 8/2006 | Geddes et al. | 7,547,282 B2 | 6/2009 | Lo et al. |
| 7,096,148 B2 | 8/2006 | Anderson et al. | 7,551,293 B2 | 6/2009 | Yelin et al. |
| 7,096,870 B2 | 8/2006 | Lamprich et al. | D603,050 S | 10/2009 | Chen |
| 7,098,907 B2 | 8/2006 | Houston et al. | 7,599,730 B2 | 10/2009 | Hunter et al. |
| 7,103,205 B2 | 9/2006 | Wang et al. | 7,606,615 B2 | 10/2009 | Makower et al. |
| 7,104,980 B1 | 9/2006 | Laherty et al. | 7,635,336 B1 | 12/2009 | Pruter |
| 7,106,043 B1 | 9/2006 | Da Silva et al. | 7,637,163 B2 | 12/2009 | Fetzer et al. |
| 7,106,431 B2 | 9/2006 | Odell | 7,640,053 B2 | 12/2009 | Verin |
| 7,106,479 B2 | 9/2006 | Roy et al. | 7,651,469 B2 | 1/2010 | Osborne et al. |
| 7,107,105 B2 | 9/2006 | Bjorklund et al. | 7,652,080 B2 | 1/2010 | Peppmoller et al. |
| 7,112,197 B2 | 9/2006 | Hartley et al. | 7,660,623 B2 | 2/2010 | Hunter et al. |
| 7,132,804 B2 | 11/2006 | Lys et al. | 7,665,893 B2 | 2/2010 | Buchalter |
| 7,137,976 B2 | 11/2006 | Ritter et al. | 7,668,583 B2 | 2/2010 | Fegert et al. |
| 7,141,812 B2 | 11/2006 | Appleby et al. | 7,699,782 B2 | 4/2010 | Angelsen et al. |
| 7,142,905 B2 | 11/2006 | Slayton et al. | 7,699,829 B2 | 4/2010 | Harris et al. |
| 7,148,970 B2 | 12/2006 | de Boer | 7,727,192 B2 | 6/2010 | Tokumoto et al. |
| 7,153,291 B2 | 12/2006 | Bierman | 7,729,743 B2 | 6/2010 | Sabczynski et al. |
| 7,161,453 B2 | 1/2007 | Creighton, IV | 7,751,865 B2 | 7/2010 | Jacob et al. |
| 7,162,291 B1 | 1/2007 | Nachaliel | 7,766,839 B2 | 8/2010 | Rogers et al. |
| 7,167,738 B2 | 1/2007 | Schweikard et al. | 7,774,051 B2 | 8/2010 | Voth |
| 7,169,107 B2 | 1/2007 | Jersey-Willuhn et al. | 7,794,407 B2 | 9/2010 | Rothenberg |
| 7,174,201 B2 | 2/2007 | Govari et al. | 7,798,970 B2 | 9/2010 | Lo et al. |
| 7,175,646 B2 | 2/2007 | Brenneman et al. | 7,819,810 B2 | 10/2010 | Stringer et al. |
| 7,180,252 B2 | 2/2007 | Lys et al. | 7,831,294 B2 | 11/2010 | Viswanathan |
| 7,184,820 B2 | 2/2007 | Jersey-Willuhn et al. | 7,833,168 B2 | 11/2010 | Taylor et al. |
| 7,189,198 B2 | 3/2007 | Harburn et al. | D629,526 S | 12/2010 | Ladwig et al. |
| 7,190,819 B2 | 3/2007 | Viswanathan | D629,527 S | 12/2010 | Crunkilton |
| 7,194,295 B2 | 3/2007 | Vilsmeier | 7,850,613 B2 | 12/2010 | Stribling |
| 7,204,798 B2 | 4/2007 | Zdeblick et al. | D630,756 S | 1/2011 | Kitayama |
| 7,206,064 B2 | 4/2007 | Rogers et al. | D630,757 S | 1/2011 | Kitayama |
| 7,207,941 B2 | 4/2007 | Sharf | 7,869,854 B2 | 1/2011 | Shachar et al. |
| 7,211,082 B2 | 5/2007 | Hall et al. | 7,873,402 B2 | 1/2011 | Shachar |
| 7,214,191 B2 | 5/2007 | Stringer et al. | 7,909,815 B2 | 3/2011 | Whitmore, III et al. |
| 7,215,326 B2 | 5/2007 | Rosenberg | 7,931,596 B2 | 4/2011 | Rachlin et al. |
| 7,221,104 B2 | 5/2007 | Lys et al. | 7,947,040 B2 | 5/2011 | Davies et al. |
| 7,223,256 B2 | 5/2007 | Bierman | 7,976,469 B2 | 7/2011 | Bonde et al. |
| 7,229,400 B2 | 6/2007 | Elliott et al. | 7,981,038 B2 | 7/2011 | Kanade et al. |
| 7,231,243 B2 | 6/2007 | Tearney et al. | 8,016,814 B2 | 9/2011 | Blakstvedt et al. |
| 7,236,157 B2 | 6/2007 | Schena et al. | 8,057,394 B2 | 11/2011 | Dala-Krishna |
| 7,236,816 B2 | 6/2007 | Kumar et al. | 8,088,072 B2 | 1/2012 | Munrow et al. |
| 7,237,313 B2 | 7/2007 | Skujins et al. | 8,090,430 B2 | 1/2012 | Makower et al. |
| 7,241,267 B2 | 7/2007 | Furia | 8,118,743 B2 | 2/2012 | Park et al. |
| 7,244,234 B2 | 7/2007 | Ridley et al. | 8,123,691 B2 | 2/2012 | Mine et al. |
| 7,248,032 B1 | 7/2007 | Hular et al. | 8,150,522 B2 | 4/2012 | Echaz et al. |
| 7,248,914 B2 | 7/2007 | Hastings et al. | 8,152,724 B2 | 4/2012 | Ridley et al. |
| 7,252,633 B2 | 8/2007 | Obata et al. | 8,214,018 B2 | 7/2012 | Markowitz et al. |
| 7,264,584 B2 | 9/2007 | Ritter et al. | 8,255,035 B2 | 8/2012 | Cao et al. |
| 7,270,662 B2 | 9/2007 | Visram et al. | 8,260,395 B2 | 9/2012 | Markowitz et al. |
| 7,276,044 B2 | 10/2007 | Ferry et al. | 8,262,577 B2 | 9/2012 | Munrow et al. |
| 7,286,034 B2 | 10/2007 | Creighton | 8,298,149 B2 | 10/2012 | Hastings et al. |
| 7,291,146 B2 | 11/2007 | Steinke et al. | 8,303,502 B2 | 11/2012 | Washburn et al. |
| 7,297,140 B2 | 11/2007 | Orlu et al. | 8,340,751 B2 | 12/2012 | Markowitz et al. |
| 7,302,288 B1 | 11/2007 | Schellenberg | 8,369,922 B2 | 2/2013 | Paul et al. |
| 7,308,296 B2 | 12/2007 | Lys et al. | 8,388,541 B2 | 3/2013 | Messerly et al. |
| 7,310,150 B2 | 12/2007 | Guillermo et al. | 8,388,546 B2 | 3/2013 | Rothenberg |
| 7,321,228 B2 | 1/2008 | Govari | 8,391,956 B2 | 3/2013 | Zellers et al. |
| 7,327,872 B2 | 2/2008 | Vaillant et al. | 8,409,103 B2 | 4/2013 | Grunwald et al. |
| 7,342,058 B2 | 3/2008 | Peppmoller et al. | 8,425,425 B2 | 4/2013 | Hagy et al. |
| 7,355,716 B2 | 4/2008 | de Boer et al. | 8,437,833 B2 | 5/2013 | Silverstein |
| 7,360,427 B2 | 4/2008 | Drinkwater et al. | 8,442,621 B2 | 5/2013 | Gorek et al. |
| 7,366,376 B2 | 4/2008 | Shishkov et al. | 8,447,384 B2 | 5/2013 | Xu et al. |
| 7,366,562 B2 | 4/2008 | Dukeshher et al. | D684,265 S | 6/2013 | Cadera |
| 7,366,563 B2 | 4/2008 | Kleen et al. | 8,456,182 B2 | 6/2013 | Bar-Tal et al. |
| 7,373,271 B1 | 5/2008 | Schneider | 8,478,382 B2 | 7/2013 | Burnside et al. |
| 7,382,949 B2 | 6/2008 | Bouma et al. | 8,485,980 B2 | 7/2013 | Sinderby et al. |
| 7,384,407 B2 | 6/2008 | Rodriguez et al. | 8,494,608 B2 | 7/2013 | Markowitz et al. |
| 7,418,169 B2 | 8/2008 | Tearney et al. | 8,496,592 B2 | 7/2013 | Ridley et al. |
| 7,447,408 B2 | 11/2008 | Bouma et al. | 8,512,256 B2 | 8/2013 | Rothenberg |
| 7,452,331 B1 | 11/2008 | Pruter | 8,527,036 B2 | 9/2013 | Jalde et al. |
| 7,452,358 B2 | 11/2008 | Stern et al. | 2002/0019447 A1 | 2/2002 | Renn et al. |
| D585,556 S | 1/2009 | Kosaku | 2002/0022777 A1 | 2/2002 | Crieghton et al. |
| | | | 2002/0032391 A1 | 3/2002 | McFann et al. |
| | | | 2002/0055680 A1 | 5/2002 | Miele et al. |
| | | | 2002/0082559 A1 | 6/2002 | Chang et al. |
| | | | 2002/0113555 A1 | 8/2002 | Lys et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | |
|-----------------|---------|-------------------|-------------------|---------|-----------------------------------|
| 2002/0123679 A1 | 9/2002 | Dominguez | 2004/0260174 A1 | 12/2004 | Keene |
| 2002/0128554 A1 | 9/2002 | Seward | 2004/0267086 A1 | 12/2004 | Anstadt et al. |
| 2002/0133079 A1 | 9/2002 | Sandhu | 2005/0004450 A1 | 1/2005 | Ben-Haim et al. |
| 2002/0156363 A1 | 10/2002 | Hunter et al. | 2005/0021019 A1 | 1/2005 | Hashimshony et al. |
| 2002/0156376 A1 | 10/2002 | Wang et al. | 2005/0033150 A1 | 2/2005 | Takahashi et al. |
| 2002/0165448 A1 | 11/2002 | Ben-Haim et al. | 2005/0038355 A1 | 2/2005 | Gellman et al. |
| 2002/0165534 A1 | 11/2002 | Hayzelden et al. | 2005/0049486 A1 | 3/2005 | Urquhart et al. |
| 2002/0198568 A1 | 12/2002 | Hafer et al. | 2005/0049510 A1 | 3/2005 | Haldeman et al. |
| 2003/0009132 A1 | 1/2003 | Schwartz et al. | 2005/0063194 A1 | 3/2005 | Lys et al. |
| 2003/0011359 A1 | 1/2003 | Ashe | 2005/0070788 A1 | 3/2005 | Wilson et al. |
| 2003/0013966 A1 | 1/2003 | Barnes et al. | 2005/0075561 A1 | 4/2005 | Golden |
| 2003/0036696 A1 | 2/2003 | Willis et al. | 2005/0085716 A1 | 4/2005 | Hamm et al. |
| 2003/0040671 A1 | 2/2003 | Somogyi et al. | 2005/0085718 A1 | 4/2005 | Shahidi |
| 2003/0072805 A1 | 4/2003 | Miyazawa et al. | 2005/0085720 A1 | 4/2005 | Jacob et al. |
| 2003/0076281 A1 | 4/2003 | Morgan et al. | 2005/0101868 A1 | 5/2005 | Ridley et al. |
| 2003/0083698 A1 | 5/2003 | Whitehurst et al. | 2005/0101869 A1 | 5/2005 | Burba et al. |
| 2003/0088195 A1 | 5/2003 | Vardi et al. | 2005/0105081 A1 | 5/2005 | Odell |
| 2003/0100849 A1 | 5/2003 | Jang | 2005/0105101 A1 | 5/2005 | Duling et al. |
| 2003/0114742 A1 | 6/2003 | Lewkowicz et al. | 2005/0112135 A1 | 5/2005 | Cormier et al. |
| 2003/0114777 A1 | 6/2003 | Griffin et al. | 2005/0113669 A1 | 5/2005 | Helfer et al. |
| 2003/0120150 A1 | 6/2003 | Govari | 2005/0113676 A1 | 5/2005 | Weiner et al. |
| 2003/0120154 A1 | 6/2003 | Sauer et al. | 2005/0113700 A1 | 5/2005 | Yanagihara et al. |
| 2003/0139661 A1 | 7/2003 | Kimchy et al. | 2005/0113873 A1 | 5/2005 | Weiner et al. |
| 2003/0149328 A1 | 8/2003 | Elliot et al. | 2005/0113874 A1 | 5/2005 | Connelly et al. |
| 2003/0152290 A1 | 8/2003 | Odell | 2005/0113876 A1 | 5/2005 | Weiner et al. |
| 2003/0160721 A1 | 8/2003 | Gilboa et al. | 2005/0149002 A1 | 7/2005 | Wang et al. |
| 2003/0163037 A1 | 8/2003 | Bladen et al. | 2005/0151489 A1 | 7/2005 | Lys et al. |
| 2003/0171691 A1 | 9/2003 | Casscells et al. | 2005/0154308 A1 | 7/2005 | Quistgaard et al. |
| 2003/0173953 A1 | 9/2003 | Ashe | 2005/0159644 A1 | 7/2005 | Takano |
| 2003/0184544 A1 | 10/2003 | Prudent | 2005/0159790 A1 | 7/2005 | Shalev |
| 2003/0191392 A1 | 10/2003 | Haldeman | 2005/0165301 A1 | 7/2005 | Smith et al. |
| 2003/0191460 A1 | 10/2003 | Hobbs et al. | 2005/0165313 A1 | 7/2005 | Byron et al. |
| 2003/0195420 A1 | 10/2003 | Mendlein et al. | 2005/0175665 A1 | 8/2005 | Hunter et al. |
| 2003/0199746 A1 | 10/2003 | Fuimaono et al. | 2005/0175703 A1 | 8/2005 | Hunter et al. |
| 2003/0208142 A1 | 11/2003 | Boudewijn et al. | 2005/0178395 A1 | 8/2005 | Hunter et al. |
| 2003/0216639 A1 | 11/2003 | Gilboa et al. | 2005/0178396 A1 | 8/2005 | Hunter et al. |
| 2003/0220557 A1 | 11/2003 | Cleary et al. | 2005/0182295 A1 | 8/2005 | Soper et al. |
| 2003/0220578 A1 | 11/2003 | Ho et al. | 2005/0203368 A1 | 9/2005 | Verin |
| 2003/0229298 A1 | 12/2003 | Iwami et al. | 2005/0203396 A1 | 9/2005 | Angelsen et al. |
| 2003/0233042 A1 | 12/2003 | Ashe | 2005/0205081 A1 | 9/2005 | Barker et al. |
| 2004/0010189 A1 | 1/2004 | van Sloun et al. | 2005/0215901 A1 | 9/2005 | Anderson et al. |
| 2004/0015070 A1 | 1/2004 | Liang et al. | 2005/0215945 A1 | 9/2005 | Harris et al. |
| 2004/0024301 A1 | 2/2004 | Hockett et al. | 2005/0222532 A1 | 10/2005 | Bertolero et al. |
| 2004/0030319 A1 | 2/2004 | Korkor et al. | 2005/0240102 A1 | 10/2005 | Rachlin et al. |
| 2004/0054278 A1 | 3/2004 | Kimchy et al. | 2005/0256398 A1 | 11/2005 | Hastings et al. |
| 2004/0082916 A1 | 4/2004 | Jenkins | 2005/0256541 A1 | 11/2005 | Stypulkowski |
| 2004/0087877 A1 | 5/2004 | Besz et al. | 2006/0015003 A1 | 1/2006 | Moaddes et al. |
| 2004/0088136 A1 | 5/2004 | Ashe | 2006/0025677 A1 * | 2/2006 | Verard et al. 600/423 |
| 2004/0097803 A1 | 5/2004 | Panescu | 2006/0058633 A1 | 3/2006 | Hoshino et al. |
| 2004/0097804 A1 | 5/2004 | Sobe | 2006/0068074 A1 | 3/2006 | Stefandl |
| 2004/0097805 A1 | 5/2004 | Verard et al. | 2006/0084867 A1 | 4/2006 | Tremblay et al. |
| 2004/0097806 A1 | 5/2004 | Hunter et al. | 2006/0116571 A1 | 6/2006 | Maschke et al. |
| 2004/0116809 A1 | 6/2004 | Chow et al. | 2006/0116578 A1 | 6/2006 | Grunwald et al. |
| 2004/0127805 A1 | 7/2004 | MacAdam et al. | 2006/0149134 A1 | 7/2006 | Soper et al. |
| 2004/0131998 A1 | 7/2004 | Marom et al. | 2006/0173329 A1 | 8/2006 | Irioka et al. |
| 2004/0133111 A1 | 7/2004 | Szczec et al. | 2006/0173407 A1 * | 8/2006 | Shaughnessy et al. 604/95.01 |
| 2004/0133130 A1 | 7/2004 | Ferry et al. | 2006/0176242 A1 | 8/2006 | Jaramaz et al. |
| 2004/0135069 A1 | 7/2004 | Odell | 2006/0184074 A1 | 8/2006 | Vaezy et al. |
| 2004/0138564 A1 | 7/2004 | Hwang et al. | 2006/0206037 A1 | 9/2006 | Braxton |
| 2004/0138570 A1 | 7/2004 | Nita et al. | 2006/0211944 A1 | 9/2006 | Mauge et al. |
| 2004/0147837 A1 | 7/2004 | Macaulay et al. | 2006/0217655 A1 | 9/2006 | Vitullo et al. |
| 2004/0150963 A1 | 8/2004 | Holmberg et al. | 2006/0224188 A1 | 10/2006 | Libbus et al. |
| 2004/0152972 A1 | 8/2004 | Hunter | 2006/0247746 A1 | 11/2006 | Danek et al. |
| 2004/0155609 A1 | 8/2004 | Lys et al. | 2006/0276867 A1 | 12/2006 | Viswanathan |
| 2004/0158140 A1 | 8/2004 | Fuimaono et al. | 2007/0010753 A1 | 1/2007 | MacAdam |
| 2004/0171924 A1 | 9/2004 | Mire et al. | 2007/0016007 A1 | 1/2007 | Govari et al. |
| 2004/0176688 A1 | 9/2004 | Haldeman | 2007/0016013 A1 | 1/2007 | Camus |
| 2004/0186461 A1 | 9/2004 | DiMatteo | 2007/0016068 A1 | 1/2007 | Grunwald et al. |
| 2004/0199069 A1 | 10/2004 | Connelly et al. | 2007/0016069 A1 | 1/2007 | Grunwald et al. |
| 2004/0210289 A1 | 10/2004 | Wang et al. | 2007/0016070 A1 | 1/2007 | Grunwald et al. |
| 2004/0230271 A1 | 11/2004 | Wang et al. | 2007/0016072 A1 | 1/2007 | Grunwald et al. |
| 2004/0234453 A1 | 11/2004 | Smith | 2007/0049822 A1 | 3/2007 | Bunce et al. |
| 2004/0243118 A1 | 12/2004 | Ayers et al. | 2007/0049846 A1 | 3/2007 | Bown et al. |
| 2004/0253365 A1 | 12/2004 | Warren et al. | 2007/0055141 A1 | 3/2007 | Kruger et al. |
| 2004/0254470 A1 | 12/2004 | Drinkwater et al. | 2007/0055142 A1 | 3/2007 | Webler |
| | | | 2007/0060992 A1 | 3/2007 | Pappone |
| | | | 2007/0062544 A1 * | 3/2007 | Rauk Bergstrom et al. .. 128/849 |
| | | | 2007/0073155 A1 | 3/2007 | Park et al. |
| | | | 2007/0087038 A1 | 4/2007 | Richardson et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

| | | | | | | | |
|--------------|------|---------|--------------------------------|--------------|----|---------|--------------------|
| 2007/0093710 | A1 | 4/2007 | Maschke | 2009/0204113 | A1 | 8/2009 | MacAdam et al. |
| 2007/0100236 | A1 | 5/2007 | McMorrow et al. | 2009/0209950 | A1 | 8/2009 | Starksen |
| 2007/0100285 | A1 | 5/2007 | Griffin et al. | 2009/0221908 | A1 | 9/2009 | Glossop |
| 2007/0112282 | A1 | 5/2007 | Skujins et al. | 2009/0227952 | A1 | 9/2009 | Blakstvedt et al. |
| 2007/0123805 | A1 | 5/2007 | Shireman et al. | 2009/0234328 | A1 | 9/2009 | Cox et al. |
| 2007/0129770 | A1 | 6/2007 | Younis | 2009/0258171 | A1 | 10/2009 | Uang |
| 2007/0135803 | A1 | 6/2007 | Belson | 2009/0259124 | A1 | 10/2009 | Rothenberg |
| 2007/0135886 | A1 | 6/2007 | Maschke | 2009/0262982 | A1 | 10/2009 | Markowitz et al. |
| 2007/0156205 | A1 | 7/2007 | Larson et al. | 2009/0275828 | A1 | 11/2009 | Shachar et al. |
| 2007/0161915 | A1 | 7/2007 | Desai | 2009/0297441 | A1 | 12/2009 | Canham et al. |
| 2007/0167738 | A1 | 7/2007 | Timinger et al. | 2010/0004543 | A1 | 1/2010 | Ahlund et al. |
| 2007/0167762 | A1 | 7/2007 | Kim et al. | 2010/0004547 | A1 | 1/2010 | Scholz et al. |
| 2007/0167769 | A1 | 7/2007 | Ikuma et al. | 2010/0016726 | A1 | 1/2010 | Meier |
| 2007/0167801 | A1 | 7/2007 | Webler et al. | 2010/0036227 | A1 | 2/2010 | Cox et al. |
| 2007/0167997 | A1 | 7/2007 | Forsberg et al. | 2010/0041973 | A1 | 2/2010 | Vu et al. |
| 2007/0197905 | A1 | 8/2007 | Timinger et al. | 2010/0049062 | A1 | 2/2010 | Ziv |
| 2007/0208255 | A1 | 9/2007 | Ridley et al. | 2010/0055153 | A1 | 3/2010 | Majmudar |
| 2007/0225589 | A1 | 9/2007 | Viswanathan | 2010/0055184 | A1 | 3/2010 | Zeitels et al. |
| 2007/0225610 | A1 | 9/2007 | Mickley et al. | 2010/0057157 | A1 | 3/2010 | Govari et al. |
| 2007/0232882 | A1 | 10/2007 | Glossop et al. | 2010/0060472 | A1 | 3/2010 | Kimura et al. |
| 2007/0238984 | A1 | 10/2007 | Maschke et al. | 2010/0076305 | A1 | 3/2010 | Maier-Hein et al. |
| 2007/0239018 | A1 | 10/2007 | Fetzer et al. | 2010/0081934 | A1 | 4/2010 | Soltani et al. |
| 2007/0244413 | A1 | 10/2007 | Biggins | 2010/0083719 | A1 | 4/2010 | Peppmoller et al. |
| 2007/0247454 | A1 | 10/2007 | Rahn et al. | 2010/0094116 | A1 | 4/2010 | Silverstein |
| 2007/0249911 | A1 | 10/2007 | Simon | 2010/0106011 | A1 | 4/2010 | Byrd et al. |
| 2007/0265526 | A1 | 11/2007 | Govari et al. | 2010/0114573 | A1 | 5/2010 | Huang et al. |
| 2007/0280974 | A1 | 12/2007 | Son et al. | 2010/0143119 | A1 | 6/2010 | Kooijman et al. |
| 2007/0282196 | A1 | 12/2007 | Birk et al. | 2010/0152596 | A1 | 6/2010 | Griffiths et al. |
| 2007/0282197 | A1 | 12/2007 | Bill et al. | 2010/0185097 | A1 | 7/2010 | Hall |
| 2007/0299352 | A1 | 12/2007 | Harlev et al. | 2010/0198048 | A1 | 8/2010 | Togawa |
| 2007/0299353 | A1 | 12/2007 | Harlev et al. | 2010/0217116 | A1 | 8/2010 | Eck et al. |
| 2008/0008745 | A1 | 1/2008 | Stinchcomb et al. | 2010/0222664 | A1 | 9/2010 | Lemon et al. |
| 2008/0009720 | A1 * | 1/2008 | Schefelker et al. 600/437 | 2010/0234733 | A1 | 9/2010 | Wahlheim |
| 2008/0015442 | A1 | 1/2008 | Watson et al. | 2010/0249598 | A1 | 9/2010 | Smith et al. |
| 2008/0027320 | A1 | 1/2008 | Bolorforosh et al. | 2010/0258033 | A1 | 10/2010 | Yang et al. |
| 2008/0045908 | A1 | 2/2008 | Gould et al. | 2010/0273895 | A1 | 10/2010 | Stinchcomb et al. |
| 2008/0051626 | A1 | 2/2008 | Sato et al. | 2010/0298702 | A1 | 11/2010 | Rogers et al. |
| 2008/0077158 | A1 | 3/2008 | Haider et al. | 2010/0298704 | A1 | 11/2010 | Pelissier et al. |
| 2008/0081958 | A1 | 4/2008 | Denison et al. | 2010/0298705 | A1 | 11/2010 | Pelissier et al. |
| 2008/0082136 | A1 | 4/2008 | Gaudiani | 2010/0298712 | A1 | 11/2010 | Pelissier et al. |
| 2008/0097232 | A1 | 4/2008 | Rothenberg | 2010/0317981 | A1 | 12/2010 | Grunwald |
| 2008/0108949 | A1 | 5/2008 | Beasley et al. | 2010/0318026 | A1 | 12/2010 | Grunwald |
| 2008/0114095 | A1 | 5/2008 | Peppmoller et al. | 2010/0331712 | A1 | 12/2010 | Rothenberg |
| 2008/0125772 | A1 | 5/2008 | Stone et al. | 2011/0015527 | A1 | 1/2011 | Heasty et al. |
| 2008/0139944 | A1 | 6/2008 | Weymer et al. | 2011/0015533 | A1 | 1/2011 | Cox et al. |
| 2008/0146939 | A1 | 6/2008 | McMorrow et al. | 2011/0034940 | A1 | 2/2011 | Payner |
| 2008/0146940 | A1 | 6/2008 | Jenkins et al. | 2011/0040212 | A1 | 2/2011 | Dietz et al. |
| 2008/0146942 | A1 | 6/2008 | Dala-Krishna | 2011/0052694 | A1 | 3/2011 | Stinchcomb et al. |
| 2008/0154100 | A1 | 6/2008 | Thalmeier et al. | 2011/0087105 | A1 | 4/2011 | Ridley et al. |
| 2008/0166453 | A1 | 7/2008 | Steele et al. | 2011/0087106 | A1 | 4/2011 | Ridley et al. |
| 2008/0171934 | A1 | 7/2008 | Greenan et al. | 2011/0087107 | A1 | 4/2011 | Lindekugel et al. |
| 2008/0183075 | A1 | 7/2008 | Govari et al. | 2011/0112396 | A1 | 5/2011 | Shachar et al. |
| 2008/0200754 | A1 | 8/2008 | Buchalter | 2011/0196248 | A1 | 8/2011 | Grunwald |
| 2008/0228082 | A1 | 9/2008 | Scheirer et al. | 2011/0245659 | A1 | 10/2011 | Ma et al. |
| 2008/0236598 | A1 * | 10/2008 | Gobel 128/849 | 2011/0282187 | A1 | 11/2011 | Harlev et al. |
| 2008/0255404 | A1 | 10/2008 | Nogawa et al. | 2011/0282188 | A1 | 11/2011 | Burnside et al. |
| 2008/0255475 | A1 | 10/2008 | Kondrosky et al. | 2011/0295108 | A1 | 12/2011 | Cox et al. |
| 2008/0275765 | A1 | 11/2008 | Kuchar | 2011/0313293 | A1 | 12/2011 | Lindekugel et al. |
| 2009/0005675 | A1 | 1/2009 | Grunwald et al. | 2012/0004564 | A1 | 1/2012 | Dobak, III |
| 2009/0018497 | A1 | 1/2009 | Birchard et al. | 2012/0046562 | A1 | 2/2012 | Powers et al. |
| 2009/0024018 | A1 | 1/2009 | Boyden et al. | 2012/0059270 | A1 | 3/2012 | Grunwald |
| 2009/0043205 | A1 | 2/2009 | Pelissier et al. | 2012/0071751 | A1 | 3/2012 | Sra et al. |
| 2009/0082661 | A1 | 3/2009 | Saladin et al. | 2012/0071759 | A1 | 3/2012 | Hagy et al. |
| 2009/0084382 | A1 | 4/2009 | Jalde et al. | 2012/0095319 | A1 | 4/2012 | Kondrosky et al. |
| 2009/0101577 | A1 | 4/2009 | Fulkerson et al. | 2012/0108950 | A1 | 5/2012 | He et al. |
| 2009/0118612 | A1 | 5/2009 | Grunwald et al. | 2012/0143029 | A1 | 6/2012 | Silverstein et al. |
| 2009/0118706 | A1 | 5/2009 | Schweikert et al. | 2012/0172727 | A1 | 7/2012 | Hastings et al. |
| 2009/0124901 | A1 | 5/2009 | Fink et al. | 2012/0220854 | A1 | 8/2012 | Messerly et al. |
| 2009/0143736 | A1 | 6/2009 | Mittermeyer et al. | 2012/0283582 | A1 | 11/2012 | Mahapatra et al. |
| 2009/0156926 | A1 | 6/2009 | Messerly et al. | 2012/0296200 | A1 | 11/2012 | Shachar et al. |
| 2009/0163810 | A1 | 6/2009 | Kanade et al. | 2012/0310052 | A1 | 12/2012 | Mahapatra et al. |
| 2009/0171217 | A1 | 7/2009 | Kim et al. | 2012/0310066 | A1 | 12/2012 | Shachar et al. |
| 2009/0177083 | A1 | 7/2009 | Matsumura | 2012/0316440 | A1 | 12/2012 | Munrow et al. |
| 2009/0177090 | A1 | 7/2009 | Grunwald et al. | 2013/0006102 | A1 | 1/2013 | Wilkes et al. |
| 2009/0203989 | A1 | 8/2009 | Burnside et al. | 2013/0018248 | A1 | 1/2013 | Hurezan |
| | | | | 2013/0035590 | A1 | 2/2013 | Ma et al. |
| | | | | 2013/0060116 | A1 | 3/2013 | Messerly et al. |

(56)

References Cited

U.S. PATENT DOCUMENTS

2013/0085416 A1 4/2013 Mest
 2013/0102890 A1 4/2013 Dib
 2013/0123597 A1 5/2013 Rothenberg

FOREIGN PATENT DOCUMENTS

AU 1860597 B2 6/1999
 AU 20009592 9/2000
 AU 20015250 6/2001
 AU 768362 B2 12/2003
 AU 2001229024 B2 9/2005
 AU 2001283703 B2 5/2006
 AU 2006202149 6/2006
 AU 2006904933 9/2006
 AU 2006283022 B2 2/2012
 CA 2420676 2/2002
 CN 1672649 A 9/2005
 CN 102209490 A 10/2011
 CN 102802514 A 11/2012
 CN 102821679 A 12/2012
 CN 103037761 A 4/2013
 CN 103037762 A 4/2013
 CN 103118591 A 5/2013
 DE 4319033 C1 6/1994
 EP 0359697 3/1990
 EP 0362821 4/1990
 EP 0399536 A1 11/1990
 EP 0823261 A2 2/1998
 EP 0928976 A2 7/1999
 EP 1311226 A1 5/2003
 EP 1504713 A1 2/2005
 EP 2313143 A1 4/2011
 EP 2440122 A1 4/2012
 EP 2464407 A2 6/2012
 EP 2482719 A1 8/2012
 EP 2575610 A1 4/2013
 EP 2575611 A1 4/2013
 EP 2603145 A2 6/2013
 EP 2605699 A2 6/2013
 EP 2618727 A1 7/2013
 FR 2545349 11/1984
 IN 9721/DELNP/2011 1/2013
 JP 01097440 4/1989
 JP 03173542 A 7/1991
 JP 4090741 8/1992
 JP 9-503054 3/1997
 JP 09-094298 A 4/1997
 JP 10043310 2/1998
 JP 10290839 A 11/1998
 JP 11128237 A 5/1999
 JP 2001161683 6/2001
 JP 2001340334 12/2001
 JP 2002-529133 A 9/2002
 JP 2003501127 A 1/2003
 JP 2003061752 A 3/2003
 JP 2003299654 10/2003
 JP 2003334191 11/2003
 JP 2002520893 2/2004
 JP 2004505748 T 2/2004
 JP 2004515298 A 5/2004
 JP 2006508744 A 3/2006
 JP 5010604 6/2012
 JP 2012-529929 11/2012
 JP 2013-518676 A 5/2013
 JP 2013-526959 A 6/2013
 JP 2013-526961 A 6/2013
 WO 9112836 A1 9/1991
 WO 9203090 3/1992
 WO 9403159 A1 2/1994
 WO 9404938 3/1994
 WO 9605768 A1 2/1996
 WO 9607352 A1 3/1996
 WO 9641119 12/1996
 WO 9729683 A1 8/1997

WO 9743989 A1 11/1997
 WO 9916495 A1 4/1999
 WO 9949407 A1 9/1999
 WO 0019906 4/2000
 WO 0027281 A1 5/2000
 WO 0040155 7/2000
 WO 0074775 A1 12/2000
 WO 0139683 A1 6/2001
 WO 0176479 A1 10/2001
 WO 0215973 A1 2/2002
 WO 0225277 A1 3/2002
 WO 03061752 7/2003
 WO 03077759 A1 9/2003
 WO 2004049970 A2 6/2004
 WO 2005033524 A1 4/2005
 WO 2005033574 A1 4/2005
 WO 2005117690 A1 12/2005
 WO 2005117733 A2 12/2005
 WO 2006031765 A2 3/2006
 WO 2006074509 A1 7/2006
 WO 2006074510 A1 7/2006
 WO 2006078677 A2 7/2006
 WO 2006103661 A2 10/2006
 WO 2006111056 A1 10/2006
 WO 2007002541 A2 1/2007
 WO 2007005976 A1 1/2007
 WO 2007014447 A1 2/2007
 WO 2007034196 A2 3/2007
 WO 2007067324 A1 6/2007
 WO 2007069168 A2 6/2007
 WO 2007109123 A2 9/2007
 WO 2007126536 A2 11/2007
 WO 2007144894 A1 12/2007
 WO 2008005480 A1 1/2008
 WO 2008024596 A2 2/2008
 WO 2008028253 3/2008
 WO 2008083111 7/2008
 WO 2008118992 A1 10/2008
 WO 2008126074 A2 10/2008
 WO 2008129326 A1 10/2008
 WO 2008131017 A2 10/2008
 WO 2008136008 A2 11/2008
 WO 2009002514 A2 12/2008
 WO 2009009064 A1 1/2009
 WO 2009057774 A1 5/2009
 WO 2009070616 A2 6/2009
 WO 2009100158 A1 8/2009
 WO 2009123819 A2 10/2009
 WO 2009126340 A1 10/2009
 WO 2009129475 A1 10/2009
 WO 2009129477 A1 10/2009
 WO 2009134605 A2 11/2009
 WO 2009137262 A2 11/2009
 WO 2010002313 A1 1/2010
 WO 2010018500 A1 2/2010
 WO 2010022370 A1 2/2010
 WO 2010027349 A1 3/2010
 WO 2010027471 A2 3/2010
 WO 2010030820 A1 3/2010
 WO 2010132857 A1 11/2010
 WO 2010132985 A1 11/2010
 WO 2010143196 A1 12/2010
 WO 2010144922 A1 12/2010
 WO 2011019760 A2 2/2011
 WO 2011041450 A1 4/2011
 WO 2011044421 A1 4/2011
 WO 2011057289 A2 5/2011
 WO 2011064209 A1 6/2011
 WO 2011084593 A2 7/2011
 WO 2011097312 A1 8/2011
 WO 2011128052 A2 10/2011
 WO 2011150358 A1 12/2011
 WO 2011150376 A1 12/2011
 WO 2012021542 A2 2/2012
 WO 2012024577 A2 2/2012
 WO 2012039866 A1 3/2012
 WO 2012040487 A1 3/2012
 WO 2012058461 A1 5/2012
 WO 2012083245 A1 6/2012

(56)

References Cited

FOREIGN PATENT DOCUMENTS

| | | | |
|----|------------|----|--------|
| WO | 2012088535 | A1 | 6/2012 |
| WO | 2013006713 | A2 | 1/2013 |
| WO | 2013006817 | A1 | 1/2013 |

OTHER PUBLICATIONS

Stereotaxis Magnetic Navigation System with Navigant™ User Interface, 2005 Brochure.

Stereotaxis, Expanding the Possibilities of Interventional Medicine: Remote Navigation and Automation, pp. 1-8.

Tepa® Health Innovation PC based ECG System Introduction and Technical Specifications, EKG Master USB, 2 pages, Nov. 2003.

The FloWire Doppler Guide Wire located <<http://www.volcanocorp.com/products/flowire-doppler-guide-wire.php>>, 2011.

Traxal Technologies, Tracking Technology website overview: www.traxal.com/rd/rd_classroom_trackingtechnology.htm.

UAB Health Systems, Arrhythmias, retrieved from <http://www.health.uab.edu/14564/> on Nov. 15, 2007, 12 pages.

U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Advisory Action dated Jun. 22, 2009.

U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Final Office Action dated Apr. 8, 2010.

U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Final Office Action dated Jan. 30, 2009.

U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Non-Final Office Action dated Sep. 25, 2009.

U.S. Appl. No. 11/552,094, filed Oct. 23, 2006 Non-Final Office Action dated Apr. 27, 2009.

U.S. Appl. No. 11/552,094, filed Oct. 23, 2006 Notice of Allowance dated May 20, 2010.

U.S. Appl. No. 12/369,625, filed Feb. 11, 2009 Non-Final Office Action dated Jul. 20, 2011.

U.S. Appl. No. 11/552,094, filed Oct. 23, 2006 Notice of Allowability dated Apr. 2, 2010.

VasoNova Inc, Vascular navigation system for accurate placement of PICCs, Start-Up Emerging Medical Ventures, pp. 44-45, vol. 14 No. 7, Jul.-Aug. 2009.

Viasys Health Care Inc. Cortrak® Fact Sheet.

Viasys Healthcare MedSystems, Navigator® Benefits, 2008.

Viasys Healthcare MedSystems, Navigator® Research in Cost Justification, 2008.

Viasys MedSystems, Cortrak™ Systems Brochure.

Volcano ComboMap Features and Benefits/Technical Specifications, 2 pages.

Watters, et al. "Use of Electrocardiogram to Position Right Atrial Catheters During Surgery." *Annals of Surgery*, vol. 225, No. 2, pp. 165-171, 1997.

Welch Allyn Cardioperfect® PC-Based Resting ECG, 2003.

Wilson, R. G. et al, Right Atrial Electrocardiography in Placement of Central Venous Catheters, *The Lancet*, pp. 462-463, Feb. 27, 1988.

Worley, Seth J. "Use of a Real-Time Three-Dimensional Magnetic Navigation System for Radiofrequency Ablation of Accessory Pathways." *PACE*, vol. 21 pp. 1636-1643, Aug. 1998.

Yilmazlar A et al, Complications of 1303 Central Venous Cannulations, *J R Soc Med*, pp. 319-321, vol. 90 No. 6, Jun. 1997 (Abstract only).

Yoon, SZ et al, Usefulness of the Carina as a Radiographic Landmark for Central Venous Catheter Placement in Paediatric Patients, *Br J Anaesth*, Jul. 2005.

Yoshida, Teruhisa et al, Detection of Concealed Left Sided Accessory Atrioventricular Pathway by P Wave Signal Averaged Electrocardiogram, *J Am Coll Cardiol*, pp. 55-62, 1999.

Zaaroor, et al. "Novel Magnetic Technology for Intraoperative Intracranial Frameless Navigation: In Vivo and in Vitro Results." *Neurosurgery*, vol. 48, No. 5, pp. 1100-1107, May 2001.

PCT/US2006/033079 filed Aug. 24, 2006 International Preliminary Report on Patentability dated Feb. 26, 2008.

PCT/US2006/033079 filed Aug. 24, 2006 Search Report dated Dec. 19, 2006.

PCT/US2006/033079 filed Aug. 24, 2006 Written Opinion dated Dec. 19, 2006.

PCT/US2008/084751 filed Nov. 25, 2008 International Preliminary Report on Patentability dated Jun. 1, 2010.

PCT/US2008/084751 filed Nov. 25, 2008 Search Report dated May 20, 2009.

PCT/US2008/084751 filed Nov. 25, 2008 Written Opinion dated May 20, 2009.

PCT/US2009/033116 filed Feb. 4, 2009 International Preliminary Report on Patentability dated Aug. 10, 2010.

PCT/US2009/033116 filed Feb. 4, 2009 Search Report dated Mar. 13, 2009.

PCT/US2009/033116 filed Feb. 4, 2009 Written Opinion dated Mar. 13, 2009.

PCT/US2009/041051 filed Apr. 17, 2009 Search Report dated Jul. 28, 2009.

PCT/US2009/041051 filed Apr. 17, 2009 Written Opinion dated Jul. 28, 2009.

PCT/US2009/054687 filed Aug. 21, 2009 International Preliminary Report on Patentability dated Feb. 22, 2011.

PCT/US2009/054687 filed Aug. 21, 2009 Search Report dated Oct. 6, 2009.

PCT/US2009/054687 filed Aug. 21, 2009 Written Opinion dated Oct. 6, 2009.

PCT/US2009/056567 filed Sep. 10, 2009 International Preliminary Report on Patentability dated Mar. 15, 2011.

PCT/US2009/056567 filed Sep. 10, 2009 Search Report dated Nov. 6, 2009.

PCT/US2009/056567 filed Sep. 10, 2009 Written Opinion dated Nov. 6, 2009.

PCT/US2010/038555 filed Jun. 14, 2010 Search Report dated Oct. 5, 2010.

PCT/US2010/038555 filed Jun. 14, 2010 Written Opinion dated Oct. 5, 2010.

PCT/US2010/045084 filed Aug. 10, 2010 Search Report dated Apr. 14, 2011.

PCT/US2010/050773 filed Sep. 29, 2010 Search Report dated Jan. 24, 2011.

PCT/US2010/050773 filed Sep. 29, 2010 Written Opinion dated Jan. 24, 2011.

PCT/US2010/051917 filed Oct. 8, 2010 Search Report dated Nov. 29, 2010.

PCT/US2010/051917 filed Oct. 8, 2010 Written Opinion dated Nov. 29, 2010.

PCT/US2011/023497 filed Feb. 2, 2011 Search Report dated Jun. 6, 2011.

PCT/US2011/023497 filed Feb. 2, 2011 Written Opinion dated Jun. 6, 2011.

Pennington, C.R., Right Atrial Thrombus: a Complication of Total Parenteral Nutrition, *British Medical Journal*, pp. 446-447, vol. 295, Aug. 15, 1987.

Perez, Valdivieso Jr et al, Evaluation of a Formula for Optimal Positioning of a Central Venous Catheter through the Right Internal Jugular Vein, *Rev Esp Anestesiol Reanim*, pp. 77-79, vol. 50 No. 2, Feb. 2003.

Petersen, J et al, Silicone Venous Access Devices Positioned with their Tip High in the Superior Vena Cava are More Likely to Malfunction, *Am J Surg*, pp. 38-41, vol. 178 No. 1, Jul. 1999.

Pittiruti, et al, Intracavitary EKG Monitoring: A reliable method for controlling tip position during and after PICC Insertion presentation in Catholic University, Rome, Italy in 2008.

Pittiruti, et al. "The EKG Method for Positioning the Tip of PICCs: Results from Two Preliminary Studies." *JAVA*, vol. 13, No. 4, pp. 179-185, 2008.

Polos, PG et al, Tips for Monitoring the Position of a Central Venous Catheter—How Placement can go awry—even when the anatomy is normal, *J Crit Illn*, pp. 660-674, vol. 8 No. 6, Jun. 1993 (Abstract only).

Randolph AG et al, Ultrasound guidance for placement of central venous catheters: a meta-analysis of the literature, *Critical Care Medicine*, pp. 2053-2058, vol. 24, Dec. 1996.

(56)

References Cited

OTHER PUBLICATIONS

- Reece, A et al, Positioning Long Lines: Contrast Versus Plain Radiography, *Arch Dis Child Fetal Neonatal Ed*, pp. 129-130, vol. 84 No. 2, Mar. 2001.
- Reynolds, N et al, Assessment of Distal Tip Position of Long Term Central Venous Feeding Catheters using Transesophageal Echocardiology, *JPEN J Parenter Enteral Nutr*, pp. 39-41, vol. 25 No. 1, Jan.-Feb. 2001.
- Ruschulte, Heiner et al, Prevention of Central Venous Catheter related infections with chlorhexidine gluconate impregnated wound dressings: A randomized controlled trial, presented as an abstract at the Annual meeting of the European Society of Anaesthesiologists (ESA) in Madrid, Spain in Jun. 2006, 12 pages, *Annals of Hematology*, Jul. 14, 2008.
- Sacolic, et al. "Electromagnetically Tracked Placement of a Peripherally Inserted Central Catheter." SPIE Medical Imaging, 2004 Proceedings.
- Salem, et al. "A New Peripherally Implanted Subcutaneous Permanent Central Venous Access Device for Patients Requiring Chemotherapy." *Journal of Clinical Oncology*, vol. 11, No. 11, pp. 2181-2185, Nov. 1993.
- Savary, D et al, Intra-atrial Monitoring to Add Insertion of a Central Venous Line in Pre-Hospital Emergency Care *Journal Europeen des Urgences*, pp. 75-78, vol. 17 No. 2, 2004.
- Schafer et al. "Incorrect placement of a vena cava catheter and its prevention by intra-atrial ECG." *Anaesthesist*. Jan. 1988;37(1):49-51.
- Schummer, et al. "Central Venous Catheters—The inability of 'intra-atrial ECG' to prove adequate positioning." *British Journal of Anaesthesia*, vol. 93, No. 2, pp. 193-198, 2004.
- Schummer, W et al, ECG-guided Central Venous Catheter Positioning: Does it detect the Pericardial Reflection rather than the Right Atrium?, *Eur J Anaesthesiol*, pp. 600-605, vol. 21 No. 8, Aug. 2004 (Abstract only).
- Schummer, W et al, Intra-Atrial ECG is not a Reliable Method for Positioning Left Internal Jugular Vein Catheters, *Br J Anaesth*, pp. 481-486, vol. 91 No. 4, Oct. 2003.
- Schummer, W, Central Venous Catheter—The Inability of "Intra-Atrial ECG" to prove Adequate Positioning, *Br J Anaesth*, pp. 193-198, vol. 93 No. 2, Aug. 2004.
- Simon, et al., "Central Venous Catheter Placement in Children: Evaluation of Electrocardiography Using J-Wire." *Paediatric Anaesthesia* vol. 9, pp. 501-504, 1999.
- Stark, DD et al, Radiographic Assessment of Venous Catheter Position in Children: Value of the Lateral View, *Pediatric Radiology*, pp. 76-80, vol. 14 No. 2, 1984.
- Starkhammar et al. "Cath-Finder Catheter Tracking System: A New Device for Positioning of Central Venous Catheters. Early Experience from Implantation of Brachial portal Systems." *Acta Anaesthesiol Scandinavia*, vol. 34, No. 4 pp. 296-300.
- Starkhammar, H et al, Central Venous Catheter Placement using Electromagnetic Position Sensing: A Clinical Evaluation, *Biomed. Instrum Technol*, vol. 30 No. 2, pp. 164-170; Mar.-Apr. 1996.
- Starr, David S et al, EKG Guided Placement of Subclavian CVP Catheters Using J-Wire, pp. 673-676, *Ann. Surg.*, Dec. 1986.
- Bankier, Alexander A., Azygos Arch Cannulation by Central Venous Catheters: Radiographic Detection of Malposition and Subsequent Complications, *Journal of Thoracic Imaging* 12:64-69 (1997).
- Cardella, John F. et al., Interventional Radiologic Placement of Peripherally Inserted Central Catheters, *Journal of Vascular and Interventional Radiology* 1993; 4:653-660.
- Chang, Thomas C. et al., Are Routine Ch Ladiographs Necessary After Image-Guided Placement of Internal Jugular Central Venous Access Devices?, *AJR* Feb. 1998;170:335-337.
- Cheung, P., et al., The Effect of a Disposable Probe Cover on Pulse Oximetry, *Anaesth Intensive Care* 2002; 30: 211-214.
- CN 200880012117.4 filed Apr. 16, 2008 First Office Action dated Dec. 23, 2011.
- Curet, Myriam J. et al., University and Practice-based Physicians' Input on the Content of a Surgical Curriculum, *The American Journal of Surgery*® vol. 178 Jul. 1999, 78-84.
- EP 09808901.4 filed Aug. 21, 2009 European Search Report dated May 23, 2012.
- EP 09813632.8 filed Apr. 5, 2011 European Search Report dated Jul. 4, 2012.
- Gjendemsjo, Anders, et al., Energy and Power, *The Connexions Project*, Version 1.2, Feb. 20, 2004.
- Joosting, Jean-Pierre, "Dual-interface RFID-compatible EEPROM enables remote access to electronic device parameters," *EE Times*, Mar. 8, 2010.
- JP 2008-528151 filed Aug. 24, 2006 Notice of Grant dated May 6, 2012.
- JP 2010-504220 filed Sep. 3, 2009 Office Action dated May 21, 2012.
- Koffler, Julia, et al., Epinephrine application via an endotracheal airway and via the Combitube in esophageal position, *Critical Care Medicine*: May 2000, vol. 28: Issue 5, pp. 1445-1449.
- Lum, Phillip, A New Formula-Based Measurement Guide for Optimal Positioning of Central Venous Catheters, *JAVA*, vol. 9, No. 2, pp. 80-85, 2004.
- Markovich, Mary B., Central Venous Catheter Tip Placement: Determination of Posterior Malposition—A Case Study, *JAVA*, vol. 11, No. 2, pp. 85-89, 2006.
- PCT/US2008/060502 filed Apr. 16, 2008 International Search Report and Written Opinion dated Oct. 16, 2008.
- PCT/US2010/045084 filed Aug. 10, 2010 International Preliminary Report on Patentability dated Feb. 23, 2012.
- PCT/US2010/045084 filed Aug. 10, 2010 Written Opinion dated Apr. 14, 2011.
- PCT/US2011/038415 filed May 27, 2011 International Search Report dated Sep. 28, 2011.
- PCT/US2011/038415 filed May 27, 2011 Written Opinion dated Sep. 28, 2011.
- PCT/US2011/047127 filed Aug. 9, 2011 International Search Report dated Feb. 29, 2012.
- PCT/US2011/047127 filed Aug. 9, 2011 Written Opinion dated Feb. 29, 2012.
- PCT/US2011/048403 filed Aug. 19, 2011 International Search Report dated Dec. 15, 2011.
- PCT/US2011/048403 filed Aug. 19, 2011 Written Opinion dated Dec. 15, 2011.
- PCT/US2011/052793 filed Sep. 22, 2011 International Search Report dated Jan. 6, 2012.
- PCT/US2011/052793 filed Sep. 22, 2011 Written Opinion dated Jan. 6, 2012.
- PCT/US2011/067268 filed Dec. 23, 2011 International Search Report and Written Opinion dated Apr. 27, 2012.
- Popp, M. B. et al., Accuracy of implanted port placement with the use of the electromagnetic CathTrack® catheter locator system, *The Journal of Vascular Access* 2005; 6: 9-12.
- Rutherford, J. S. et al., Depth of Central Venous Catheterization: An Audit of Practice in a Cardiac Surgical Unit, *Anaesth Intens Care* 1994; 22: 267-271.
- Schuster, M. et al., The carina as a landmark in central venous catheter placement, *British Journal of Anaesthesia* 85 (2): 192-4 (2000).
- Siela, Debra, Using Chest Radiography in the Intensive Care Unit, *Crit Care Nurse* Aug. 1, 2002 vol. 22 No. 4, pp. 18-27.
- Smith, Brigham, et al., Intravenous electrocardiographic guidance for placement of peripherally inserted central catheters, *Journal of Electrocardiology* 43 (2010) 274-278.
- U.S. Appl. No. 12/104,253, filed Apr. 16, 2008 Final Office Action dated Jul. 27, 2011.
- U.S. Appl. No. 12/104,253, filed Apr. 16, 2008 Non-Final Office Action dated Nov. 29, 2010.
- U.S. Appl. No. 12/323,273, filed Nov. 25, 2008 Non-Final Office Action dated Jun. 8, 2012.
- U.S. Appl. No. 12/369,625, filed Feb. 11, 2009 Final Office Action dated Feb. 23, 2012.
- U.S. Appl. No. 12/427,244, filed Apr. 21, 2009 Non-Final Office Action dated Jan. 19, 2012.

(56)

References Cited

OTHER PUBLICATIONS

- U.S. Appl. No. 12/557,401, filed Sep. 10, 2009 Non-Final Office Action dated Apr. 24, 2012.
- U.S. Appl. No. 12/878,915, filed Sep. 9, 2010 Non-Final Office Action dated Mar. 15, 2012.
- Valdivieso, J.R. Perez, et al., Evaluation of a formula for optimal positioning of a central venous catheter inserted through the right internal jugular vein, *Rev. Esp. Anesthesiol. Reanim.* 2003; 50: 77-79.
- Vesely, Thomas M. et al., Central Venous Catheter Tip Position: A Continuing Controversy, *J Vasc Interv Radiol* 2003; 14:527-534.
- Wong, Jeffrey J. et al., Azygos Tip Placement for Hemodialysis Catheters in Patients with Superior Vena Cava Occlusion, *Cardiovasc Intervent Radiol* (2006) 29:143-146.
- Zachariou, Zacharias et al., Intra-atrial ECG recording: a new and safe method for implantation of Broviac catheters in children, *Pediatr Surg Int* (1994) 9: 457-458.
- "Ascension to Launch New 3D Guidance™ Tracker at TCT 2006." Press Releases from Ascension website: www.ascension-tech.com/news/press_101106.php.
- Acuson—The Value of Vision, AcuNav Diagnostic Ultrasound Catheter, 2000.
- Advertising flyer for GAVECELT—The Italian Group for Long Term Venous Access Devices, for program on International Meeting on PICC's, Midline Catheters and Long Term Venous Access Devices in Catholic University, Rome, Italy on Dec. 3, 4, 5, 2008.
- Alexander, GD et al, The Role of Nitrous Oxide in Postoperative Nausea and Vomiting, Collection of Abstracts Presented at the International Anesthesia Research Society by various speakers, 58th Congress, Mar. 12-14, 1984, Anesthesia and Analgesia, pp. 175-284, vol. 63, 1984.
- Allan, P.L. et al, Role of Ultrasound in the Assessment of Chronic Venous Insufficiency, *Ultrasound Quarterly*, vol. 17, No. 1, pp. 3-10, 2001.
- Andropoulos, et al. "A Controlled Study of the Transesophageal Echocardiography to Guide Central Venous Catheter Placement in Congenital Heart Surgery Patients." *The International Anesthesia Research Society*, vol. 89, pp. 65-70, 1999.
- Anonymous author, Correct Catheter Placement with a low-impact, reliable and economical method, <<http://www.cvc-partner.com/index.cfm?103A955CC6844BF58ACFE3C9C1471959>>, last accessed Dec. 22, 2011.
- Arai, J et al, Detection of Peripherally Inserted Central Catheter Occlusion by in-line Pressure Monitoring, *Paediatr Anaesth*, pp. 621-624, vol. 12 No. 7, Sep. 2002.
- Arrow International, Inc., The Arrow-Johans RAECG Adapter-Making Proper Central Venous Catheter Placement More Reliable (Module No. EG-04900), Technical Report 1987, USA.
- Aslamy, et al. "MRI of Central Venous Anatomy: Implications for Central Venous Catheter Insertion." *American College of Chest Physicians*, Jun. 8, 2009.
- AU 2006283022 filed Aug. 24, 2006 Office Action dated Dec. 22, 2010.
- Aurora® System Technical Specifications 2004.
- B. Braun, Certofix Central Venous Catheter for Placement Using the Seldinger Technique with Simultaneous ECG Lead Option.
- B. Braun Website, "The Optimal Position of the Central Venous Catheter." <http://www.cvcpartner.com/index.cfm?18F1BDEA1310466194960A39F4E90968> (2009).
- Bailey, SH et al, Is Immediate Chest Radiograph Necessary after Central Venous Catheter Placement in a Surgical Intensive Care Unit?, *Am J Surg*, pp. 517-522, vol. 180 No. 6, Dec. 2000.
- Barber, JM et al, A Nurse led Peripherally Inserted Central Catheter Line Insertion Service is Effective with Radiological Support, *Clin Radiol*, pp. 352-354, vol. 57 No. 5, May 2002.
- Bard Access Systems, Sherlock Tip Location System, 5 pages, 2006.
- Bard Access Systems, Site Rite Vascular Access Ultrasound System, 4 pages, 2005.
- Benchimol, Alberto et al, Right Atrium and Superior Vena Cava Flow Velocity in Man Measured with the Doppler-Catheter Flowmeter-Telemetry System, *The Amer Journal of Medicine*, pp. 303-309, vol. 48, Mar. 1970.
- BioAdvance Lumen Vu, Greenhouse Fund Feb. 2004 Recipient, www.bioadvance.com <<http://www.bioadvance.com>>, 2005.
- Borgobello, Bridget, App allows users to view electrocardiograms on smartphones dated Oct. 15, 2010; printed from <http://www.gizmag.com/app-to-view-electrocardiograms-on-smartphones/16664/> on Feb. 4, 2011.
- Buehrle, Douglas, PICC Placement in Humans using Electromagnetic Detection, <http://www.corpakmedsystems.com/supplement_material/supplementpages/navigator/navarticle.html>, 2008.
- C.R. Bard, CathTrack™ Catheter Location System at www.bardaccess.com <<http://www.bardaccess.com>>.
- C.R. Bard, Inc., Bard Electrophysiology Product Catalogue, Bard Catheters, pp. 74-75 (2002), USA.
- Cadman, A et al, To Clot or Not to Clot? That is the question in Central Venous Catheters, *Clinical Radiology*, pp. 349-355, vol. 59 No. 4, Apr. 2004.
- Calvert, N et al, The Effectiveness and Cost-effectiveness of Ultrasound Locating Devices for Central Venous Access: A Systematic Review and Economic Evaluation, *Health Technology Assessment*, vol. 7, No. 12, 2003.
- Carlson, R et al, Secondary Migration of a Central Venous Catheter—A Case Report, *Minerva Anesthesiol*, pp. 927-931, vol. 69 No. 12, Dec. 2003.
- Caruso, LJ et al, A Better Landmark for Positioning a Central Venous Catheter, *J Clinical Monitoring and Computing*, pp. 331-334, vol. 17 No. 6, Aug. 2002.
- Cavatorta, et al., "Central Venous Catheter Placement in Hemodialysis: Evaluation of Electrocardiography Using a Guidewire." *The Journal of Vascular Access*, vol. 2, pp. 45-50, 2001.
- Chalkiadis, GA et al, Depth of Central Venous Catheter Insertion in Adults: An Audit and Assessment of a Technique to Improve Tip Position, *Anaesth Intensive Care*, pp. 61-66, vol. 26 No. 1, Feb. 1998.
- Chamsi-Pasha, Hassan et al, Cardiac Complications of Total Parenteral Nutrition: The Role of Two-Dimensional Echocardiography in Diagnosis, *Annals of the Royal College of Surgeons of England*, pp. 120-123, vol. 71, 1989.
- Chaturvedi et al., "Catheter Malplacement During Central Venous Cannulation Through Arm Veins in Pediatric Patients." *Journal of Neurosurgical Anesthesiology*, vol. 15, No. 3 pp. 170-175, Jan. 2003.
- Chen, Zhongping et al, Optical Doppler Tomography: Imaging in vivo Blood Flow Dynamics Following Pharmacological Intervention and Photodynamic Therapy, 7 pages, vol. 67, *Photochemistry and Photobiology*, 1998.
- Cheng, KI et al, A Novel Approach of Intravenous Electrocardiograph Technique in Correct Position the Long-Term Central Venous Catheter, *Kaohsiung J Med Sci*, pp. 241-247, vol. 16 No. 5, May 2000 (Abstract only).
- Chu, et al., "Accurate Central Venous Port—A Catheter Placement: Intravenous Electrocardiography and Surface Landmark Techniques Compared by Using Transesophageal Echocardiography." *The International Anesthesia Research Society*, vol. 98, pp. 910-914, 2004.
- Claasz, Antonia et al, A Study of the Relationship of the Superior Vena Cava to the Bony Landmarks of the Sternum in the Supine Adult: Implications for Magnetic Guidance Systems, *Journal*, vol. 12 No. 3, *JAVA*, Jul. 24, 2007.
- Clifford, et al. "Assessment of Hepatic Motion Secondary to Respiration for Computer Assisted Interventions." *Computer Aided Surgery*, vol. 7, pp. 291-299, 2002.
- Colley, Peter S et al, ECG-Guided Placement of Sorenson CVP Catheters via Arm Veins, *Anesthesia and Analgesia*, pp. 953-956, vol. 63, 1984.
- Collier, PE et al, Cardiac Tamponade from Central Venous Catheters, *Am J Surg*, pp. 212-214, vol. 176 No. 2, Aug. 1998.
- ComboWire® Pressure/Flow Guide Wire Ref 9500 Series, 36 pages, (information in different languages).
- Corsten, et al., "Central Placement Catheter Placement Using the ECG-Guided Cavafix-Certodyn SD Catheter." *Journal of Clinical Anesthesiology*, vol. 6, Nov./Dec. 1994.

(56)

References Cited

OTHER PUBLICATIONS

- Cucchiara, Roy et al, Time Required and Success Rate of Percutaneous Right Atrial Catheterization: Description of a Technique, *Canad. Anaesth. Soc. J.*, pp. 572-573, vol. 27, No. 6, Nov. 1980.
- Cullinane, DC et al, the Futility of Chest Roentgenograms Following Routine Central Venous Line Changes, *Am J Surg*, pp. 283-285, vol. 176 No. 3, Sep. 1998.
- David, et al., "Is ECG-Guidance a Helpful Method to Correctly Position a Central Venous Catheter During Prehospital Emergency Care?" *ACTA Anaesthesiologica Scandinavica*, vol. 49, pp. 1010-1014, 2005.
- Deltac Cath-Finder® Tracking System Operation Manual, 1994.
- Egelhof, Petra, Effects of Somatostatin on Portal Blood Flow and Portal Vein Pressure in Patients with Portal Hypertension due to Liver Cirrhosis Invasive Monitoring during TIPSS Procedures, Dissertation submitted to: Technical University of Munich, Faculty of Medicine, May 13, 2002; Date of examination: Feb. 26, 2003.
- Engelhardt, W et al, ECG-Controlled Placement of Central Venous Catheters in Patients with Atrial Fibrillation, *Anaesthesist*, pp. 476-479, vol. 38 No. 9, Sep. 1989 (Abstract only).
- Fearon, William F et al, Evaluating Intermediate Coronary Lesions in the Cardiac Catheterization Laboratory, vol. 4, No. 1, 7 pages, *Reviews in Cardiovascular Medicine*, 2003.
- Felleiter P et al, Use of Electrocardiographic Placement Control of Central Venous Catheters in Austria, *Acta Med Austriaca*, pp. 109-113, vol. 26 No. 3, 1999 (Abstract only).
- Forauer, AR et al, Change in Peripherally Inserted Central Catheter Tip Location with Abduction and Adduction of the Upper Extremity, *J Vasc Interv Radiol*, pp. 1315-1318, vol. 11 No. 10, Nov.-Dec. 2000.
- Frassinelli, P et al, Utility of Chest Radiographs after Guidewire Exchanges of Central Venous Catheters, *Crit Care Med*, pp. 611-615, vol. 26 No. 3, Mar. 1998.
- Frazin L et al, A Doppler Guided Retrograde Catheterization System, *Cathet. Cardiovasc Diagn*, pp. 41-50, May 1992.
- French, PJ et al, Sensors for Catheter Applications, *Sensors Update*, vol. 13 Issue 1 pp. 107-153, Dec. 2003.
- GB Application 0800474.9 filed Aug. 24, 2006 Office Action dated Aug. 9, 2010.
- GB Application 0800474.9 filed Aug. 24, 2006 Office Action dated Mar. 17, 2010.
- Gebauer, B et al, Ultrasound and Fluoroscopy-guided Implantation of Peripherally Inserted Central Venous Catheters (PICCs), *ROFO*, pp. 386-391, vol. 176 No. 3, Mar. 2004 (Abstract only).
- Gebhard, et al., "The accuracy of Electrocardiogram-Controlled Central Line Placement." *The International Anesthesia Research Society*, vol. 104, No. 1 Jan. 2007.
- Gladwin, MT et al, Cannulation of the Internal Jugular Vein: is postprocedural chest radiography always necessary?, *Crit Care Med*, 33 pages, Oct. 2000.
- Gonzales, et al. "Peripherally Inserted Central Catheter Placement in Swine Using Magnet Detection." *Journal of Intravenous Nursing*, vol. 22, No. 3, May/June. 1999.
- Greenall, M.J. et al, Cardiac Tamponade and Central Venous Catheters, *British Medical Journal*, pp. 595-597, Jun. 14, 1975.
- Guillory, "Basic Principles of Technologies for Catheter Localization." C.R. Bard internal paper, Oct. 20, 2004.
- Guth, AA, Routine Chest X-rays after Insertion of Implantable Long-Term Venous Catheters: Necessary or Not?, *Am Surg*, pp. 26-29, vol. 67 No. 1, Jan. 2001 (Abstract only).
- Hill, Bradley et al, Abstract of article discussing VasaNova VPS as guide for placement of PICCs.
- Hill, Bradley, Identifying the Caval-Atrial Junction Using Smart-Catheter Technology presentation, 22nd Annual Scientific Meeting of the AVA in Savannah, Georgia, Sep. 13, 2008.
- Hoffman, Thomas et al, Simultaneous Measurement of Pulmonary Venous Flow by Intravascular Catheter Doppler Velocimetry and Transesophageal Doppler Echocardiography: Relation to Left Atrial Pressure and Left Atrial and Left Ventricular Function, pp. 239-249, *J Am Coll Cardiol*, Jul. 1995.
- Hoffmann, et al. "New Procedure in Transesophageal Echocardiography: Multiplane Transesophageal Echocardiography and Transesophageal Stress Echocardiography." *Herz*, vol. 18, No. 5, pp. 269-277, Oct. 1993.
- Iacopino, Domenico Gerardo et al, Intraoperative Microvascular Doppler Monitoring of Blood Flow within a Spinal Dural Arteriovenous Fistula: A Precious Surgical Tool, vol. 10, 5 pages, *Neurosurg. Focus*, Feb. 2001.
- Kim, Ko et al, Positioning Internal Jugular Venous Catheters using the Right Third Intercostal Space in Children, *Acta Anaesthesiol Scand*, pp. 1284-1286, vol. 47 No. 10, Nov. 2003.
- Kjelstrup T et al, Positioning of Central Venous Catheters using ECG, *Tidsskr Nor Laegeforen*, pp. 599-601, vol. 111 No. 5, Feb. 1999 (Abstract only).
- Kowalski, CM et al, Migration of Central Venous Catheters: Implications for Initial Catheter Tip Positioning, *J Vasc Interv Radiol*, pp. 443-447, vol. 8 No. 3, May-June. 1997.
- Leowenthal, MR et al, the Peripherally Inserted Central Catheter (PICC): A Prospective Study of its Natural History after Fossa Insertion, *Anaesth Intensive Care*, pp. 21-24, vol. 30 No. 1, Feb. 2002.
- Lepage Ronan et al, ECG Segmentation and P-wave Feature Extraction: Application to Patients Prone to Atrial Fibrillation, *IEEE/EMBS Proceedings, 23rd Annual Conference, Istanbul, Turkey*, Oct. 25-28, 2001.
- Liu, Ji-Bin et al, Catheter-Based Intraluminal Sonography, *J Ultrasound Med*, pp. 145-160, vol. 23, 2004.
- Lucey, B et al, Routine Chest Radiographs after Central Line Insertion: Mandatory Postprocedural Evaluation or Unnecessary Waste of Resources?, *Cardiovasc Intervent Radiol*, pp. 381-384, vol. 22 No. 5, Sep.-Oct. 1999.
- Lynch, RE et al, A Procedure for Placing Pediatric Femoral Venous Catheter Tips near the Right Atrium, *Pediatr Emerg Care*, pp. 130-132, vol. 18 No. 2, Apr. 2002.
- Madan, et al. "Right Atrial Electrocardiography: A Technique for the Placement of Central Venous Catheters for Chemotherapy or Intravenous Nutrition." *British Journal of Surgery*, vol. B1, pp. 1604-1605, 1994.
- Madias, John E, Intracardiac (Superior Vena Cava/Right Atrial) ECGs using Saline Solution as the Conductive Medium for the Proper Positioning of the Shiley Hemodialysis Catheter: Is it Not Time to Forego the Postinsertion Chest Radiograph?, pp. 2363-2367, *CHEST*, 2003.
- Martin, Roy W, An Ultrasound Catheter for Intravascular Measurement of Blood Flow: Technical Details, *IEEE Transactions on Sonics and Ultrasonics*, vol. SU-27, No. 6, pp. 277-286, Nov. 1980.
- McDonnall, "Intra-Atrial Electrocardiography (ECG) for Catheter Placement." Literature review prepared for Bard Access Systems, Oct. 2007.
- McGee et al., "Accurate Placement of Central Venous Catheters: A Prospective, Randomize, Multicenter Trial." *Critical Care Medicine*, vol. 21 No. 8, Aug. 1993.
- MedGraphics, CardioPerfect® Resting/Stress ECG System, 3 pages, 2001.
- Michaels, Andrew D et al, Intravenous Electrocardiographic Guidance for Placement of Peripherally Inserted Central Catheters, pp. 274-278, vol. 43, *Journal of Electrocardiology*, 2010.
- Michenfelder, John et al, Air Embolism During Neurosurgery—An Evaluation of Right-Atrial Catheters for Diagnosis and Treatment, *JAMA*, pp. 1353-1358, vol. 208, No. 8, May 26, 1969.
- Michenfelder, John et al, Air Embolism During Neurosurgery . . . A New Method of Treatment, *Anesthesia and Analgesia . . . Current Researches*, pp. 390-395, vol. 45, No. 4, Jul.-Aug. 1966.
- Microbird™ Miniaturized DC Magnetic Sensors for Intra-body Navigation and Localization, Specifications, 2005.
- Micronix CathRite™ Cardiac Access Device Brochure.
- Micronix Pty Ltd "CathRite" Guiding Styled Core Manufacturing, Jun. 15, 2006.
- Murthy, Vrudhula et al, Analysis of Power Spectral Densities of Electrocardiograms, *Mathematical Biosciences*, pp. 41-51, vol. 12 No. 1-2, Oct. 1971.
- Nadroo, AM et al, Changes in Upper Extremity Position Cause Migration of Peripherally Inserted Central Catheters in Neonates, *Pediatrics*, pp. 131-136, vol. 110, Jul. 2002.

(56)

References Cited

OTHER PUBLICATIONS

Nakatani, K et al, Accurate Placement of Central Venous Catheters—ECG-guided method vs Patient Height Method, Masui, pp. 34-38, vol. 51 No. 1, Jan. 2002.

Nazarian, GK et al, Changes in Tunneled Catheter Tip Position when a patient is Upright, J Vasc Interv Radiol, pp. 437-441, vol. 8 No. 3, May-Jun. 1997.

Neurometer® CPT, Clinical Applications. Neurotron, Inc. website: www.neurotron.com/CLINAPS.html.

Neurometer® CPT, Frequently Asked Questions. Neurotron, Inc. website: www.neurotron.com/CPTFAQ/html.

Neurometer® CPT, Products Page. Neurotron, Inc. website: www.neurotron.com/products.html.

Neurometer® Electrodiagnostic Neuroselective Sensory Nerve Evaluation: Charts, Tables, Documents & Downloads. Neurotron, Inc. website: www.neurotron.com/downloads.html.

Odd, De et al, Does Radio-opaque Contrast Improve Radiographic localisation of Percutaneous Central Venous Lines?, Arch Dis Child Fetal Neonatal Ed, pp. 41-43, vol. 89 No. 1, Jan. 2004.

Palesty, JA et al, Routine Chest Radiographs Following Central Venous Recatheterization over a Wire are not Justified, Am J Surg, pp. 618-621, vol. 176 No. 6, Dec. 1998.

Paliotti, Roberta P. et al, Intravascular Doppler Technique for Monitoring Renal Venous Blood Flow in Man, J Nephrol, pp. 57-62, 2003.

Parker, K.H. et al, Cardiovascular Fluid Dynamics, Department of Bioengineering, National Heart and Lung Institute, Imperial College of Science, Technology and Medicine, Cardiovascular Haemodynamics, pp. 1-28, Sep. 26, 2005.

Pawlik, et al., "Central Venous Catheter Placement: Comparison of the Intravascular Guidewire and the Fluid Column Electrocardiograms." European Journal of Anaesthesiology, vol. 41, pp. 594-599, 2004.

AU 2008329807 exam requested Aug. 13, 2012 Examination Report No. 1 dated Feb. 15, 2013.

AU 2011289513 filed Jan. 21, 2013 Examiner's Report dated Jul. 5, 2013.

AU 2012202293 filed Apr. 19, 2012 Examination Report No. 1 dated Apr. 24, 2013.

AU 2013201648 filed Mar. 19, 2013 Examiner's Report dated Oct. 14, 2013.

AU 2013204243 filed Apr. 12, 2013 Examiner's Report dated Jun. 5, 2013.

CA 2,619,909 filed Aug. 24, 2006 Examiner's Report dated Oct. 26, 2012.

CN 200880012117.4 filed Apr. 16, 2008 Third Office Action dated Apr. 27, 2013.

CN 200880125528.4 filed Nov. 25, 2008 Second Office Action dated Mar. 6, 2013.

CN 200880125528.4 filed Nov. 25, 2008 Third Office Action dated Jul. 1, 2013.

CN 200980123021.X filed Dec. 17, 2010 First Office Action dated Nov. 19, 2012.

CN 200980123021.X filed Dec. 17, 2010 Second Office Action dated Aug. 13, 2013.

CN 200980144663.8 filed May 9, 2011 First Office Action dated Dec. 5, 2012.

EP 08855396.1 filed Jun. 15, 2010 Intent to Grant dated Jul. 5, 2013.

EP 09707467.8 supplemental European search report dated Jun. 18, 2013.

EP 09808901.4 filed Aug. 21, 2009 Examination Report dated May 10, 2013.

EP 09813632.8 filed Apr. 5, 2011 Office Action dated Apr. 30, 2013.

EP 12177438.4 filed Jul. 23, 2012 European Search Report dated Dec. 4, 2012.

EP 12177438.4 filed Jul. 23, 2012 extended European Search Report dated Mar. 25, 2013.

JP 2010-504220 filed Sep. 3, 2009 Final Office Action dated Apr. 18, 2013.

JP 2010-535117 filed May 26, 2011 First Office Action dated Aug. 5, 2013.

PCT/US2011/038391 filed May 27, 2011 International Preliminary Report on Patentability and Written Opinion dated Dec. 4, 2012.

PCT/US2011/038391 filed May 27, 2011 International Search Report dated Sep. 21, 2011.

PCT/US2011/038415 filed May 27, 2011 International Preliminary Report on Patentability dated Dec. 13, 2012.

PCT/US2011/047127 filed Aug. 9, 2011 International Preliminary Report on Patentability dated Apr. 18, 2013.

PCT/US2011/052793 filed Sep. 22, 2011 International Preliminary Report on Patentability dated Apr. 4, 2013.

PCT/US2011/058138 filed Oct. 27, 2011 International Preliminary Report on Patentability dated May 10, 2013.

PCT/US2011/067268 filed Dec. 23, 2011 International Preliminary Report on Patentability dated Jul. 4, 2013.

U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Final Office Action dated Oct. 28, 2013.

U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Non-Final Office Action dated Mar. 28, 2013.

U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Notice of Allowance dated Dec. 3, 2012.

U.S. Appl. No. 12/426,175, filed Apr. 17, 2009 Final Office Action dated Aug. 2, 2013.

U.S. Appl. No. 12/426,175, filed Apr. 17, 2009 Non-Final Office Action dated Dec. 3, 2012.

U.S. Appl. No. 12/545,762, filed Aug. 21, 2009 Final Office Action dated Mar. 7, 2013.

U.S. Appl. No. 12/575,456, filed Oct. 7, 2009 Non-Final Office Action dated Oct. 5, 2012.

U.S. Appl. No. 12/815,331, filed Jun. 14, 2010 Advisory Action dated Oct. 4, 2013.

U.S. Appl. No. 12/815,331, filed Jun. 14, 2010 Final Office Action dated Jul. 26, 2013.

U.S. Appl. No. 12/815,331, filed Jun. 14, 2010 Non-Final Office Action dated Jan. 22, 2013.

U.S. Appl. No. 12/854,083, filed Aug. 10, 2010 Final Office Action dated Aug. 15, 2013.

U.S. Appl. No. 12/854,083, filed Aug. 10, 2010 Non-Final Office Action dated Jan. 29, 2013.

U.S. Appl. No. 12/878,915, filed Sep. 9, 2010 Notice of Allowance dated Jan. 8, 2013.

U.S. Appl. No. 12/900,750, filed Oct. 8, 2010 Non-Final Office Action dated Jun. 3, 2013.

U.S. Appl. No. 13/019,939, filed Feb. 2, 2011 Non-Final Office Action dated Oct. 11, 2013.

U.S. Appl. No. 13/118,138, filed May 27, 2011 Final Office Action dated Apr. 3, 2013.

U.S. Appl. No. 13/118,138, filed May 27, 2011 Final Office Action dated Aug. 1, 2013.

U.S. Appl. No. 13/213,622, filed Aug. 19, 2011 Final Office Action dated Feb. 19, 2013.

U.S. Appl. No. 13/283,395, filed Oct. 27, 2011 Non-Final Office Action dated Apr. 23, 2013.

U.S. Appl. No. 13/336,919, filed Dec. 23, 2011 Advisory Action dated May 23, 2013.

U.S. Appl. No. 13/336,919, filed Dec. 23, 2011 Final Office Action dated Mar. 1, 2013.

U.S. Appl. No. 13/337,987, filed Dec. 27, 2011 Non-Final Office Action dated Mar. 15, 2013.

U.S. Appl. No. 29/428,649, filed Aug. 1, 2012 Notice of Allowance dated Jul. 5, 2013.

CN 200880012117.4 filed Apr. 16, 2008 Second Office Action dated Oct. 8, 2012.

CN 200880125528.4 filed Nov. 25, 2008 First Office Action dated Jun. 5, 2012.

EP 08855396.1 filed Jun. 15, 2010 European Search Report dated Jul. 31, 2012.

Konings, MK, et al., Development of an intravascular impedance catheter for detection of fatty lesions in arteries, IEEE Trans Med Imaging Aug. 1997; 16(4):439-46.

PCT/US2011/058138 filed Oct. 27, 2011 International Search Report dated Feb. 7, 2012.

PCT/US2011/058138 filed Oct. 27, 2011 Written Opinion dated Feb. 7, 2012.

(56)

References Cited

OTHER PUBLICATIONS

PCT/US2012/045814 filed Jul. 6, 2012 International Search Report and Written Opinion dated Oct. 1, 2012.

Pop, Gheorghe A. et al., Catheter-based impedance measurements in the right atrium for continuously monitoring hematocrit and estimating blood viscosity changes; an in vivo feasibility study in swine, Biosensors and Bioelectronics 19 (2004) 1685-1693.

U.S. Appl. No. 11/466,602, filed Aug. 23, 2006 Appeal Board Decision dated Sep. 17, 2012.

U.S. Appl. No. 12/369,625, filed Feb. 11, 2009 Notice of Allowance dated Oct. 5, 2012.

U.S. Appl. No. 12/369,625, filed Feb. 11, 2009 Notice of Panel Decision dated Aug. 1, 2012.

U.S. Appl. No. 12/545,762, filed Aug. 21, 2009 Non-Final Office Action dated Aug. 1, 2012.

U.S. Appl. No. 12/878,915, filed Sep. 9, 2010 Final Office Action dated Sep. 26, 2012.

U.S. Appl. No. 13/118,138, filed May 27, 2011 Non-Final Office Action dated Oct. 3, 2012.

U.S. Appl. No. 13/213,622, filed Aug. 19, 2011 Non-Final Office Action dated Jul. 31, 2012.

U.S. Appl. No. 13/336,919, filed Dec. 23, 2011 Non-Final Office Action dated Oct. 16, 2012.

* cited by examiner

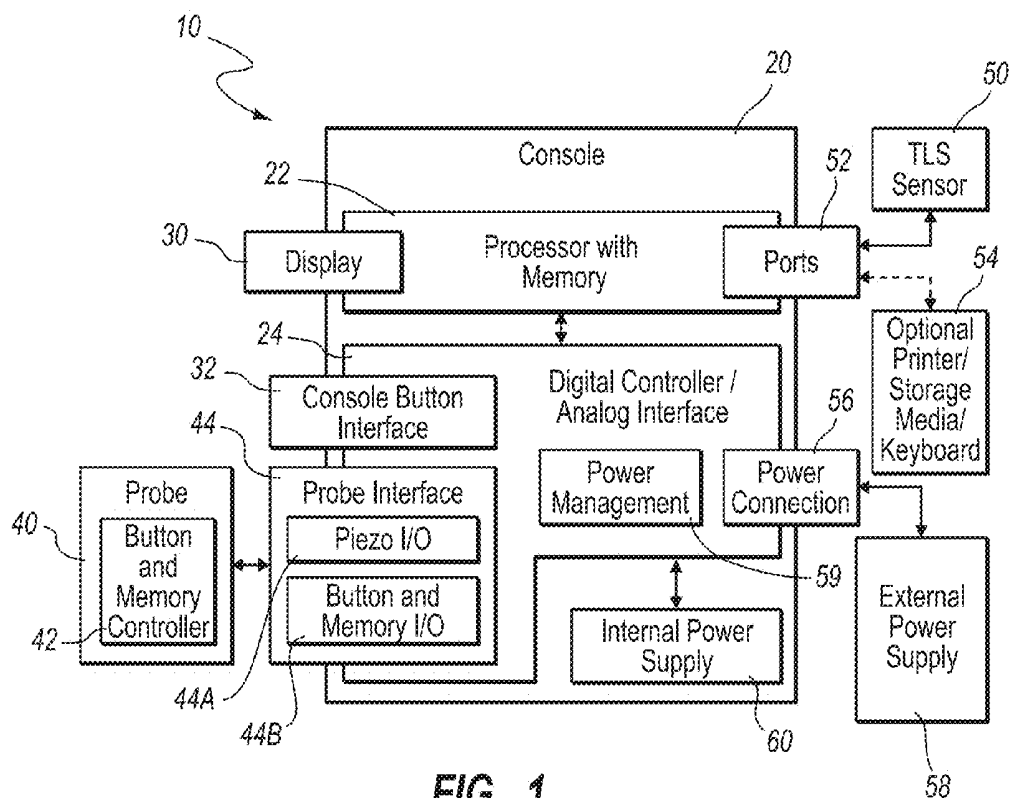


FIG. 1

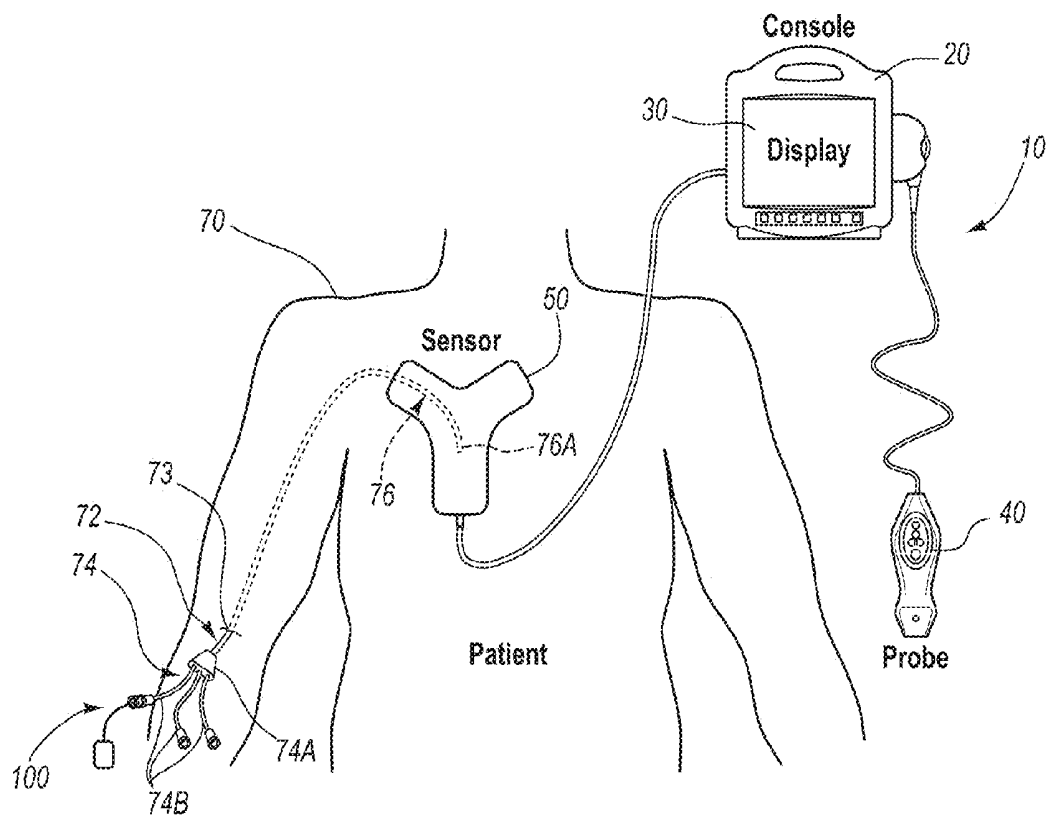


FIG. 2

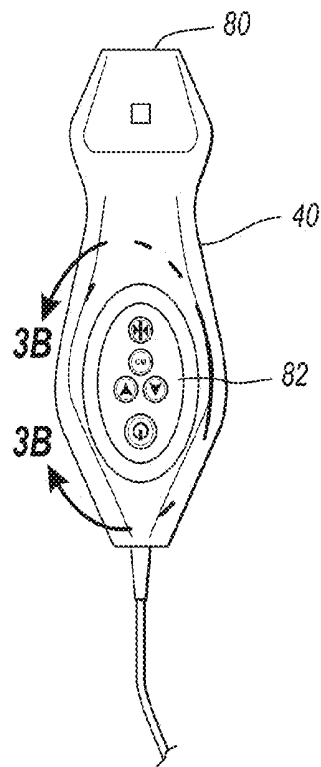


FIG. 3A

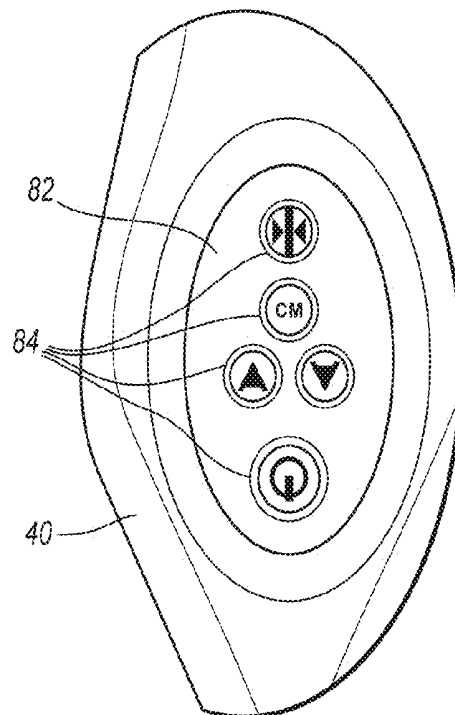


FIG. 3B

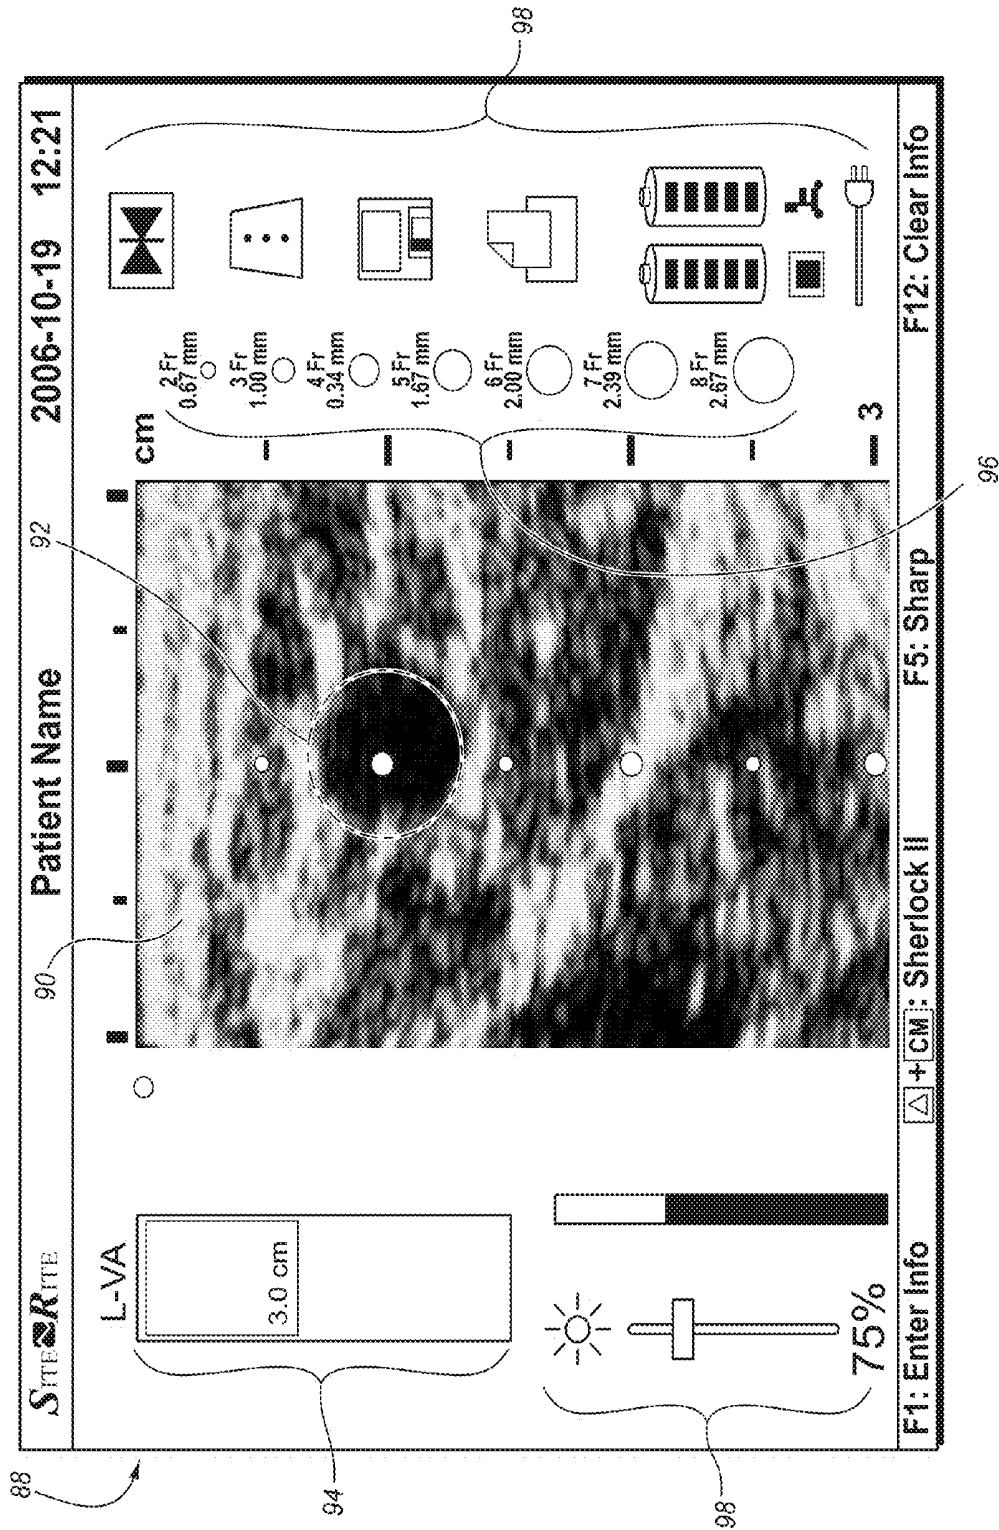


FIG. 4

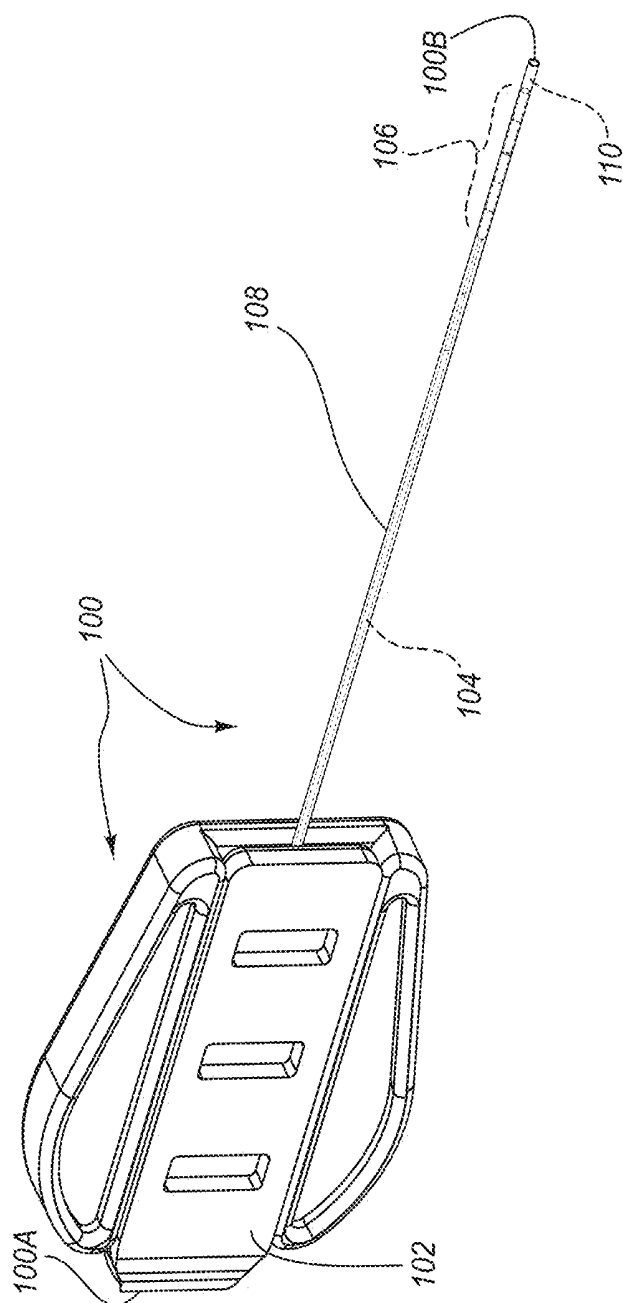


FIG. 5

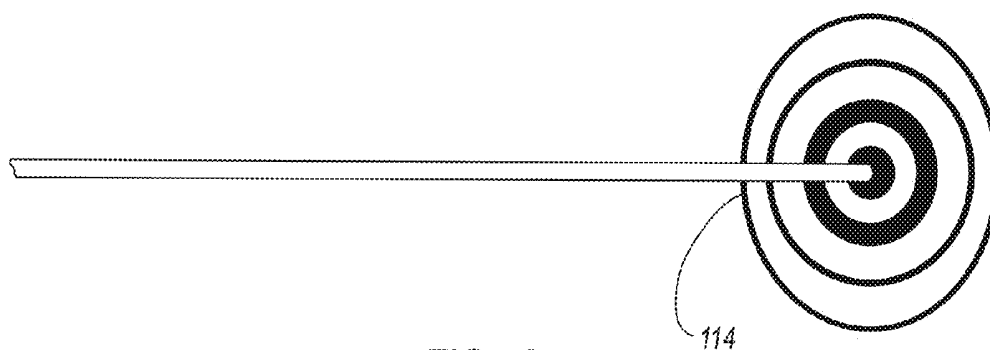


FIG. 6

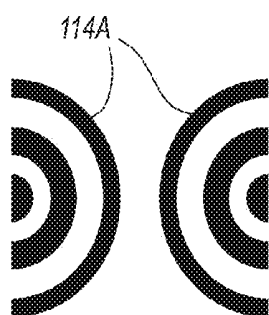


FIG. 7A




FIG. 7B



FIG. 7C




FIG. 7D




FIG. 7E

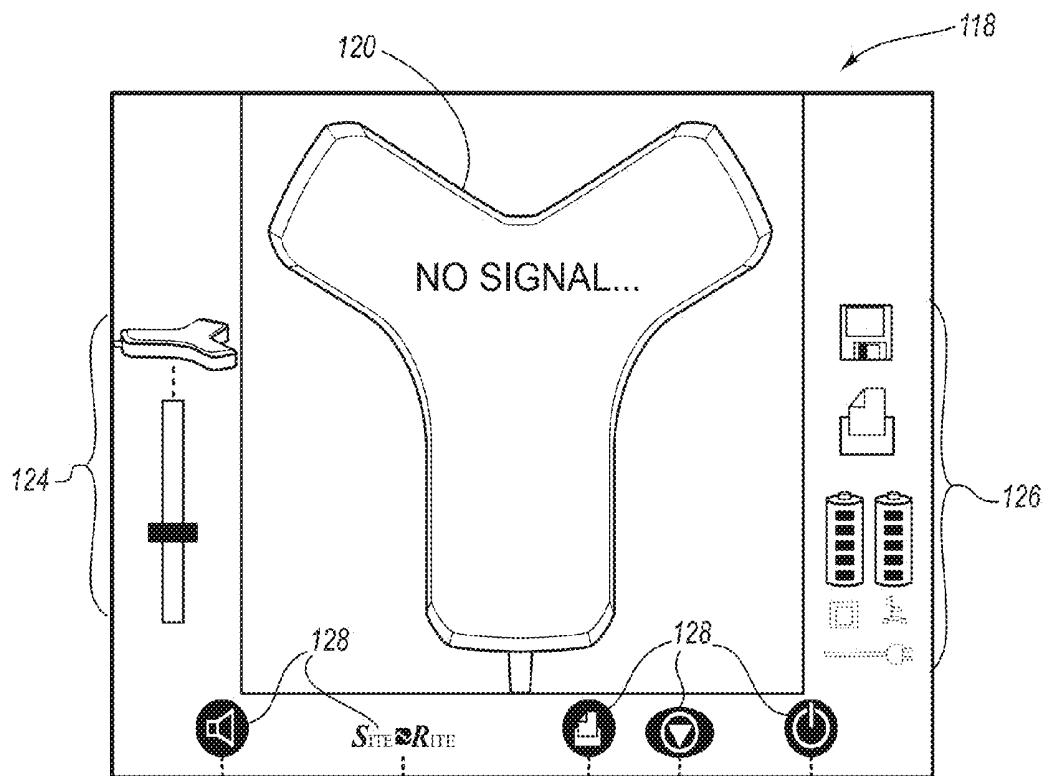


FIG. 8A

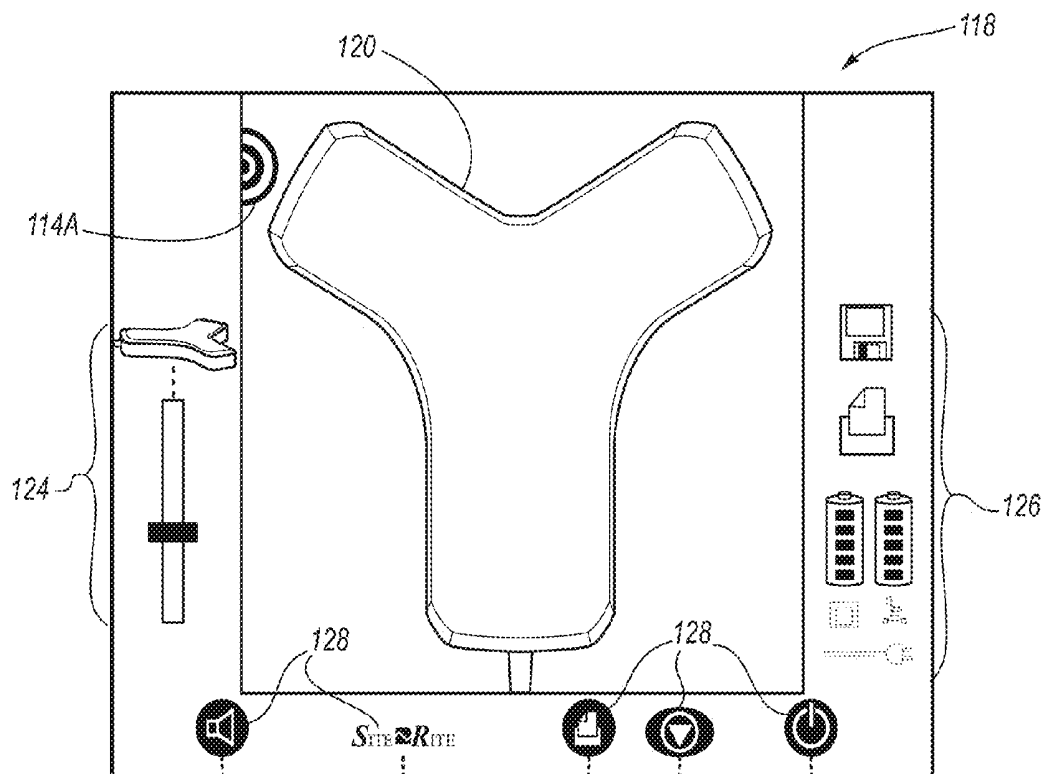


FIG. 8B

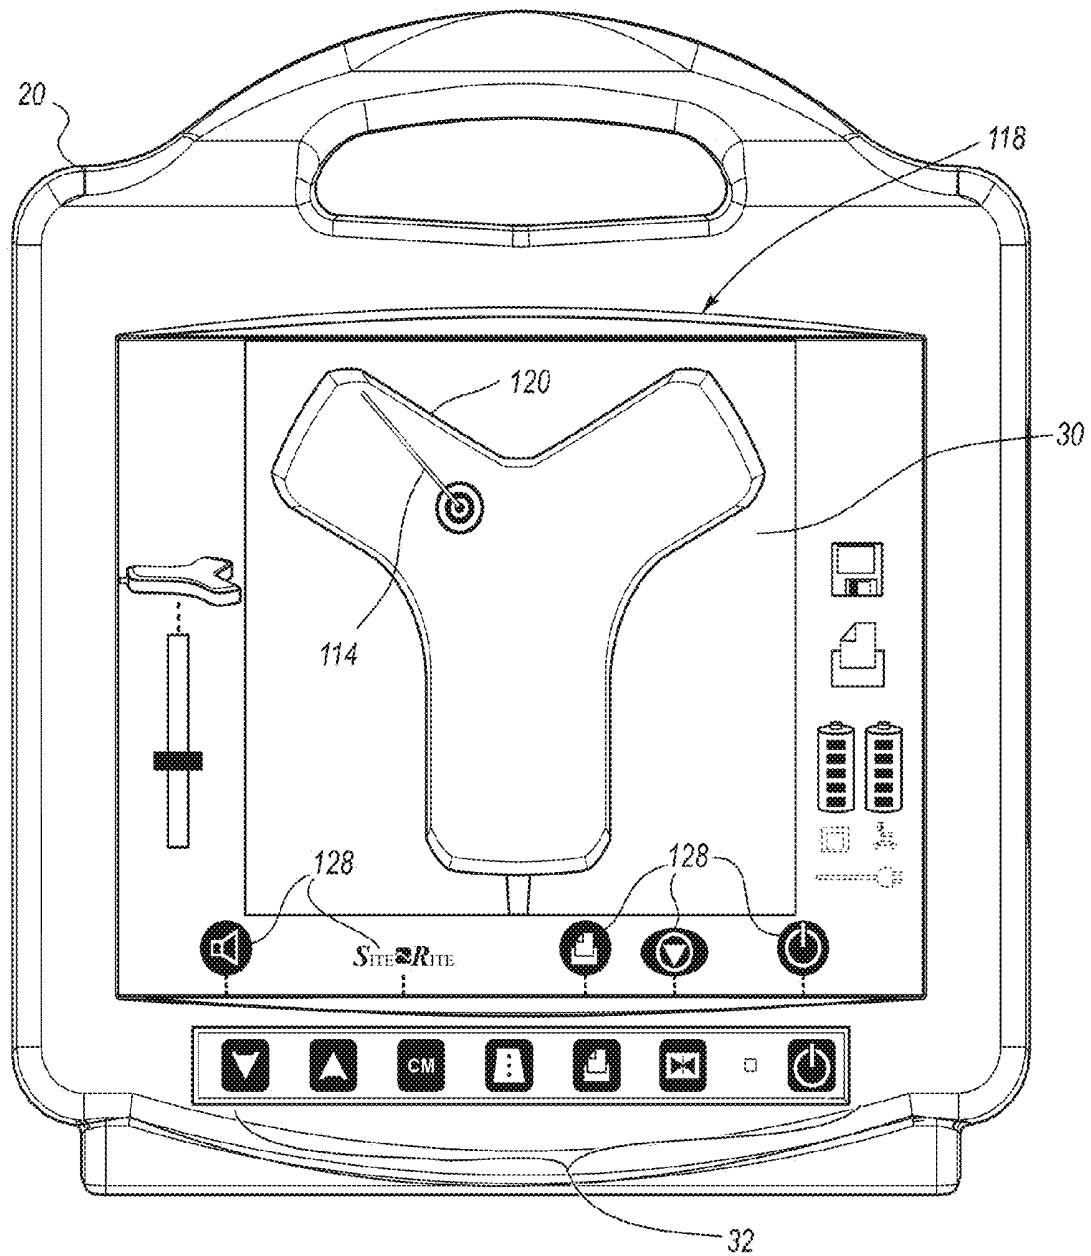


FIG. 8C

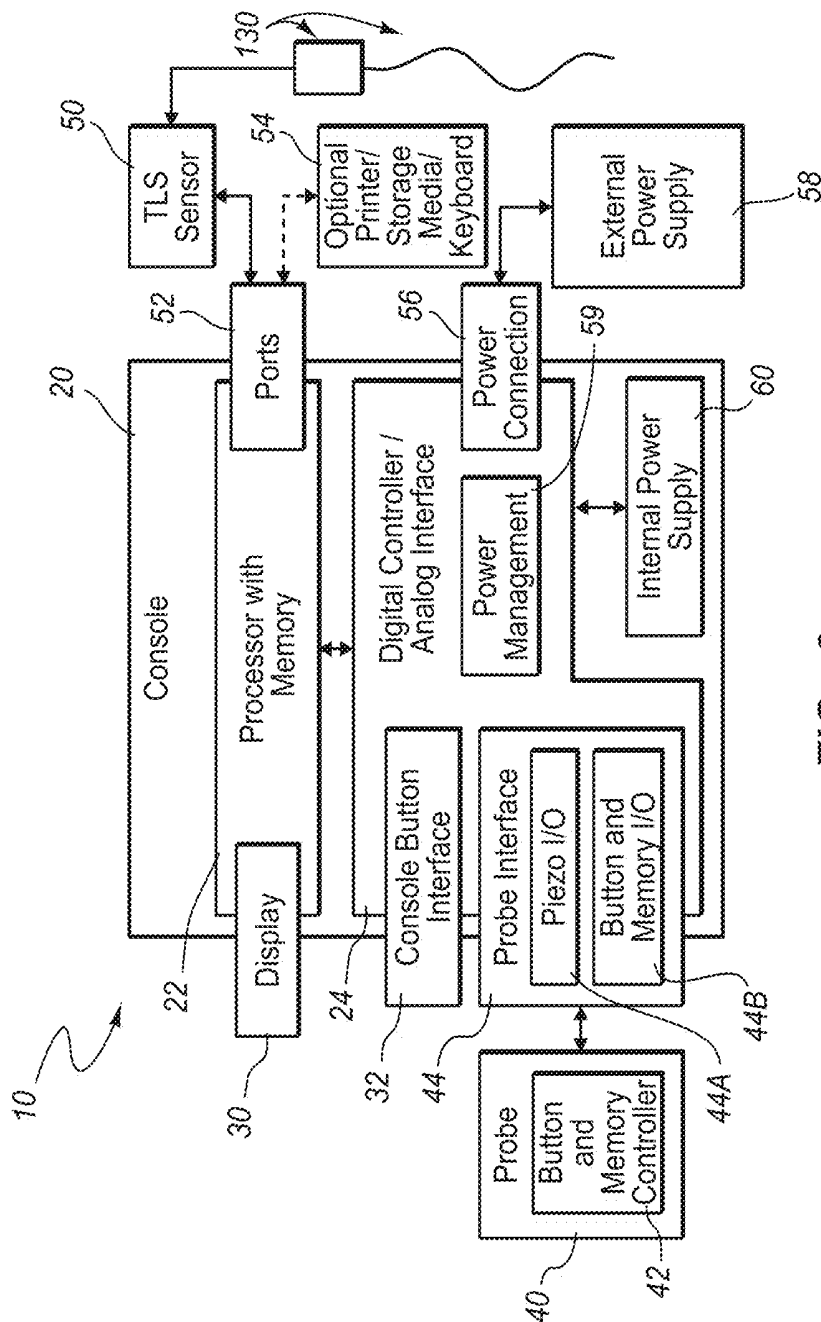


FIG. 9

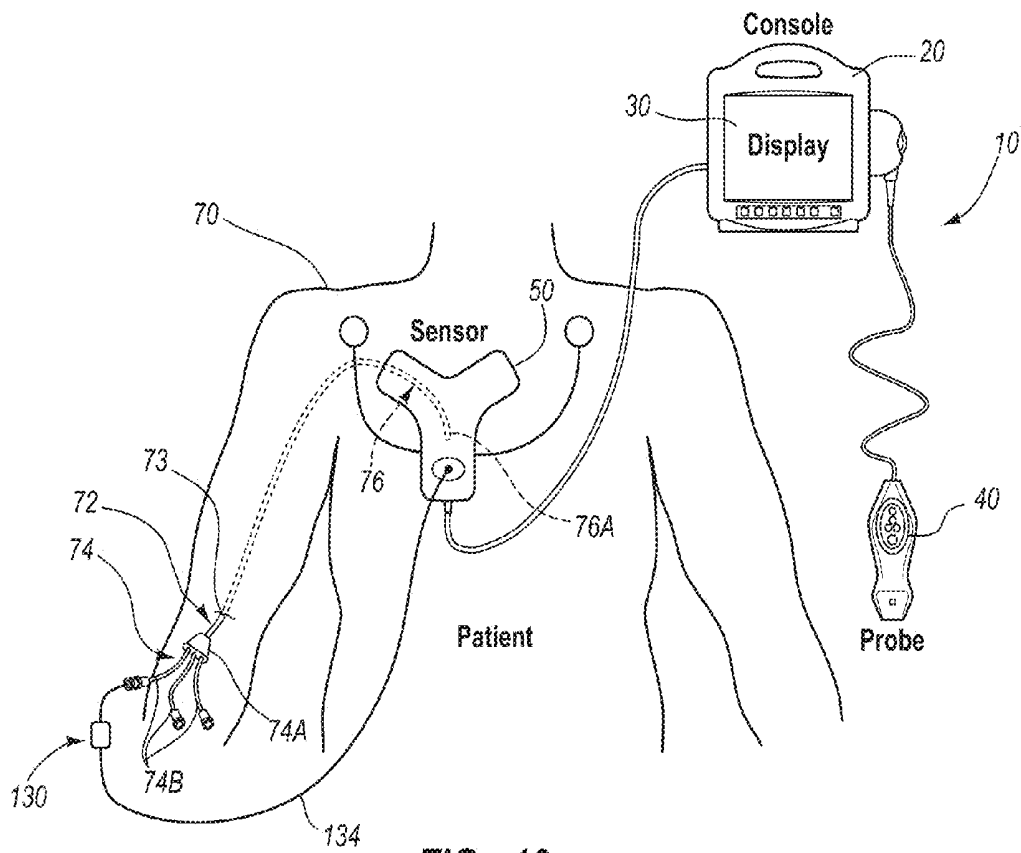


FIG. 10

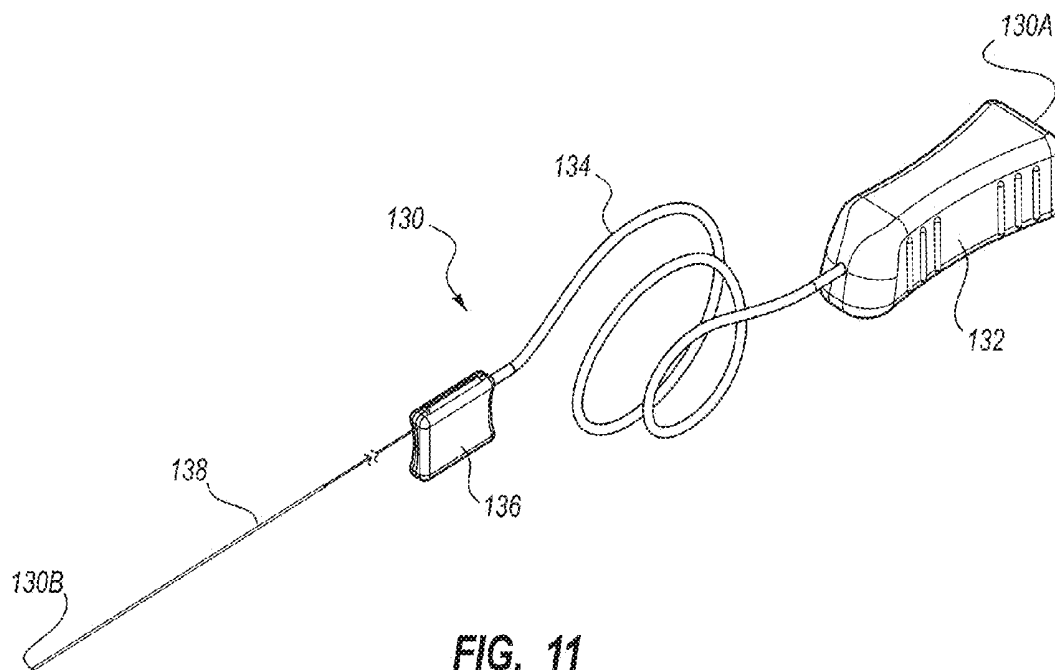


FIG. 11

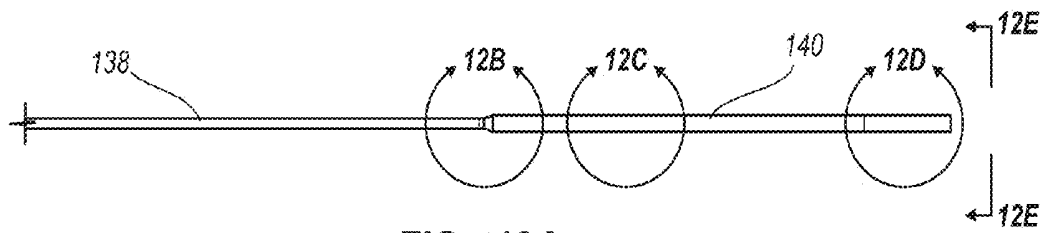


FIG. 12A

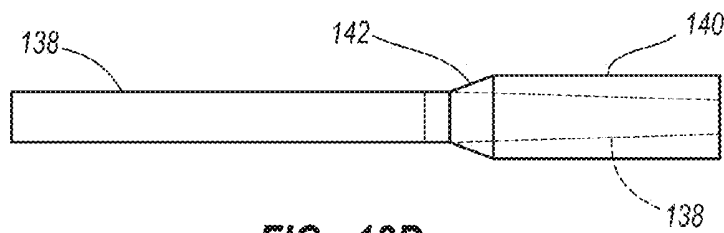


FIG. 12B

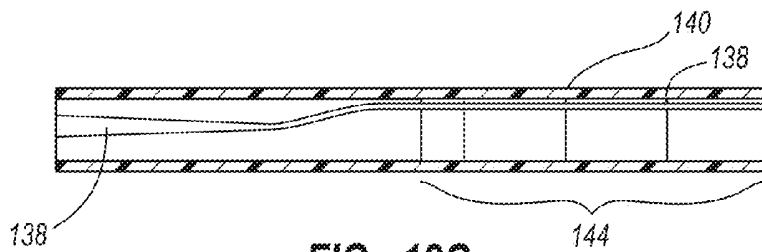


FIG. 12C

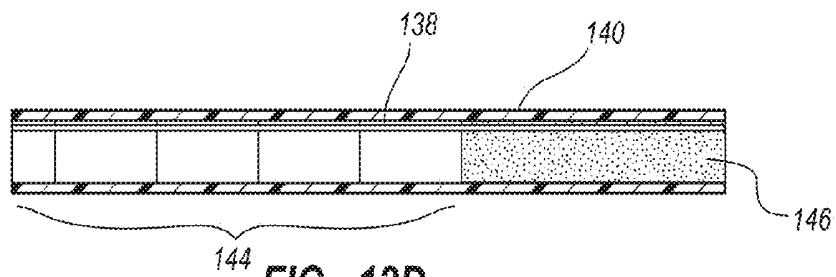


FIG. 12D

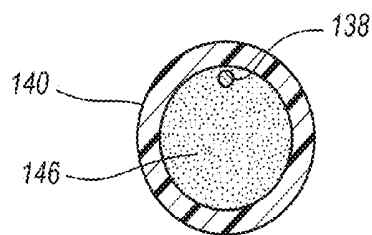


FIG. 12E

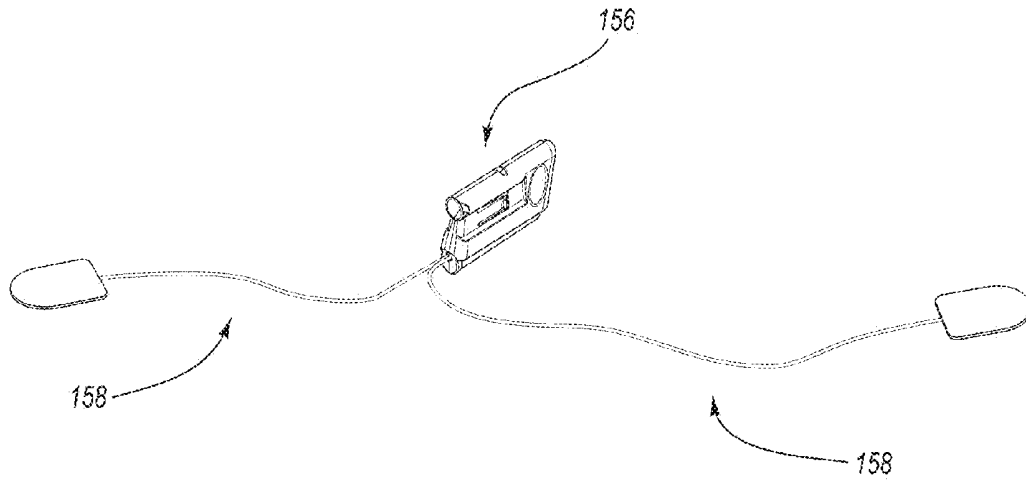


FIG. 13A

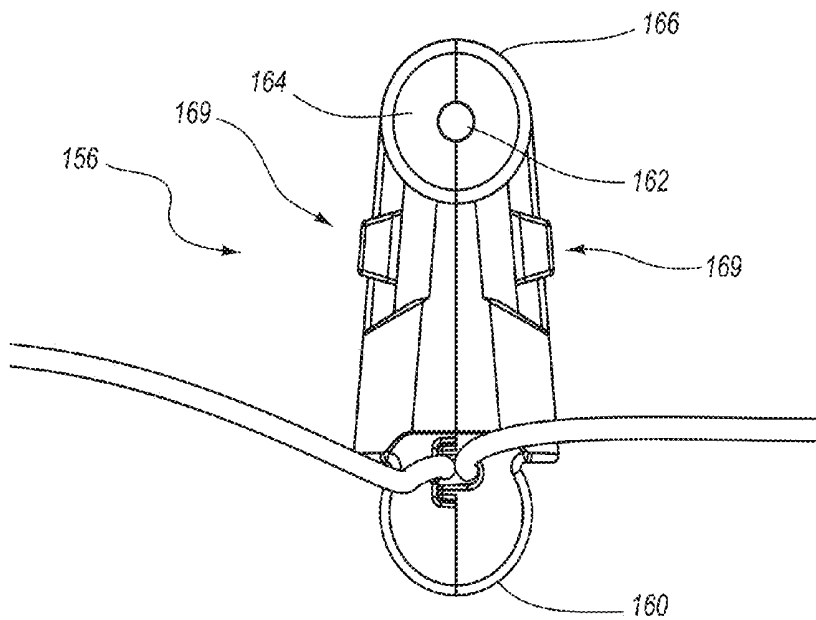


FIG. 13B

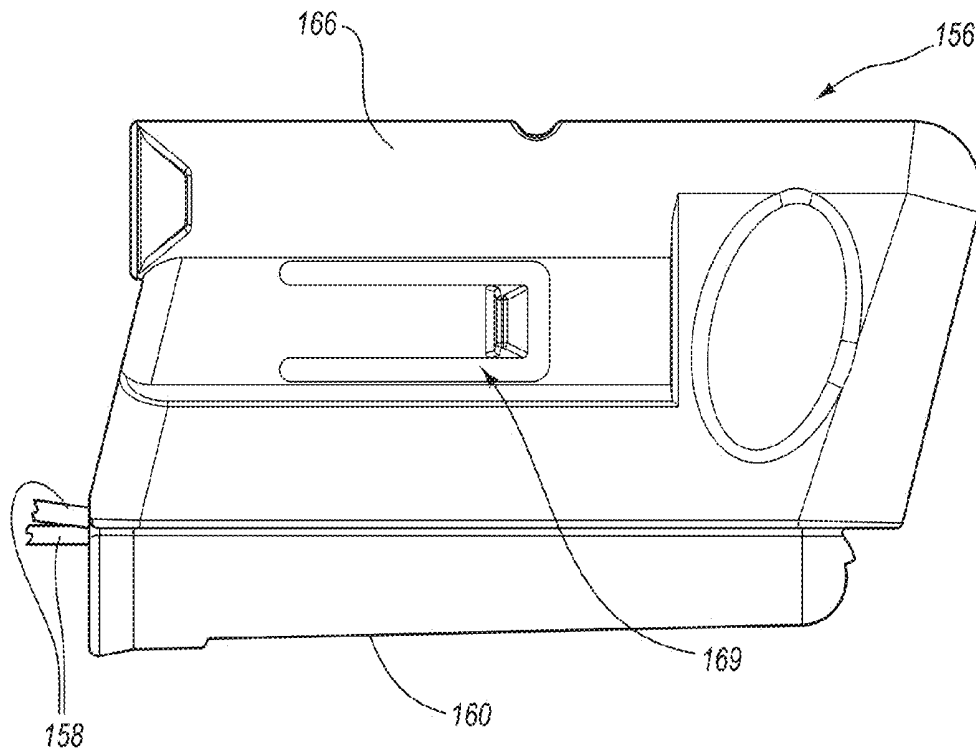


FIG. 13C

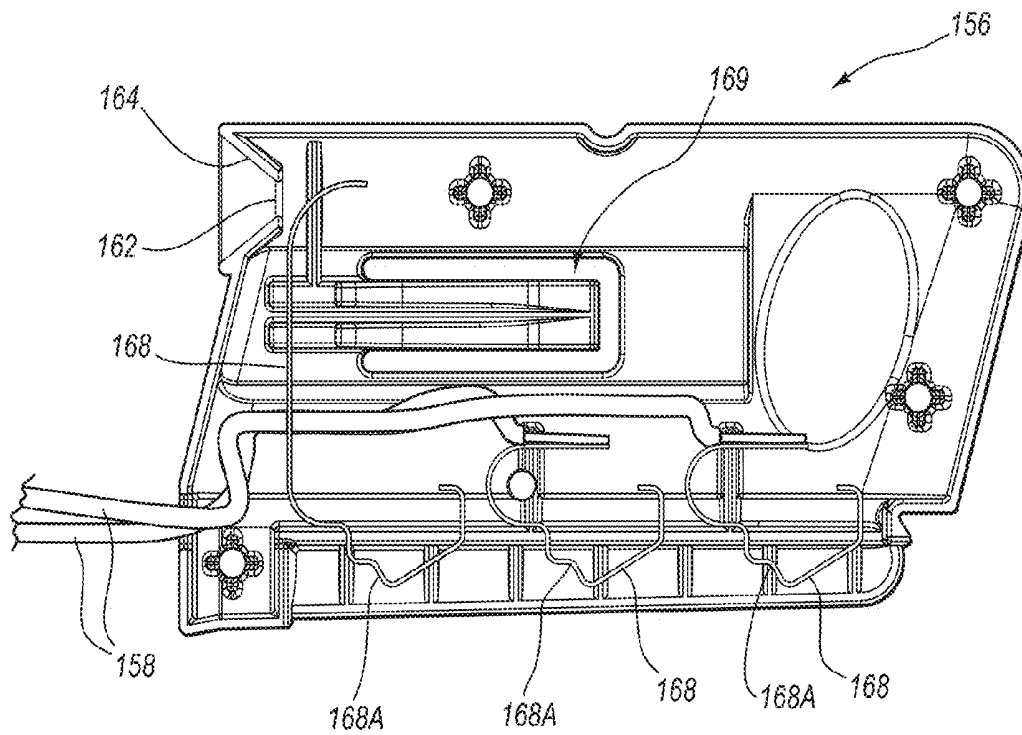


FIG. 13D

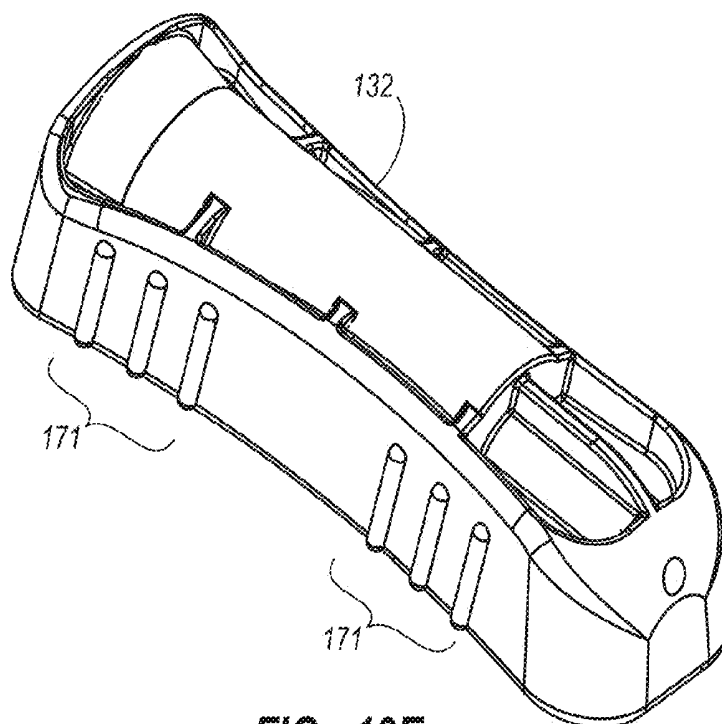


FIG. 13E

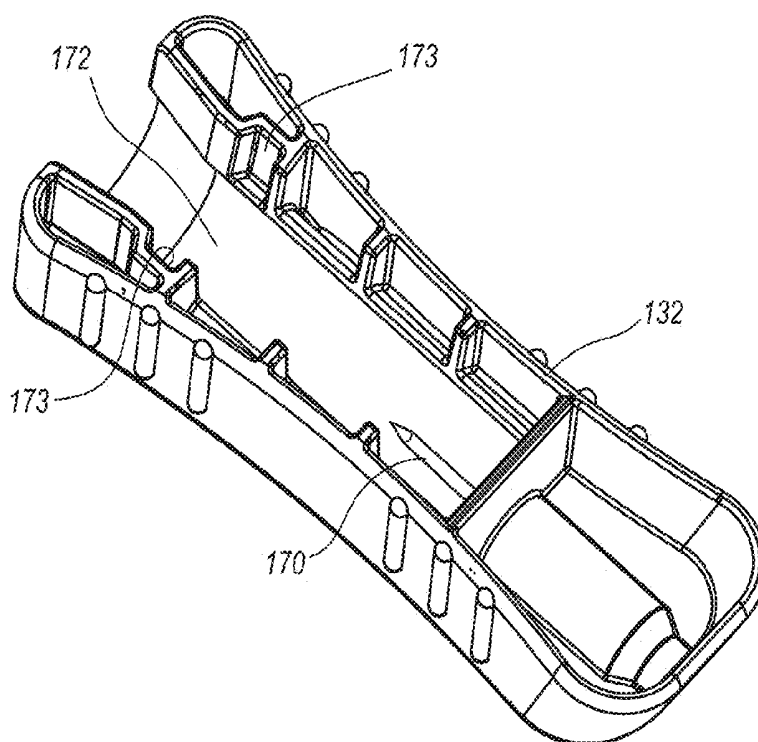


FIG. 13F

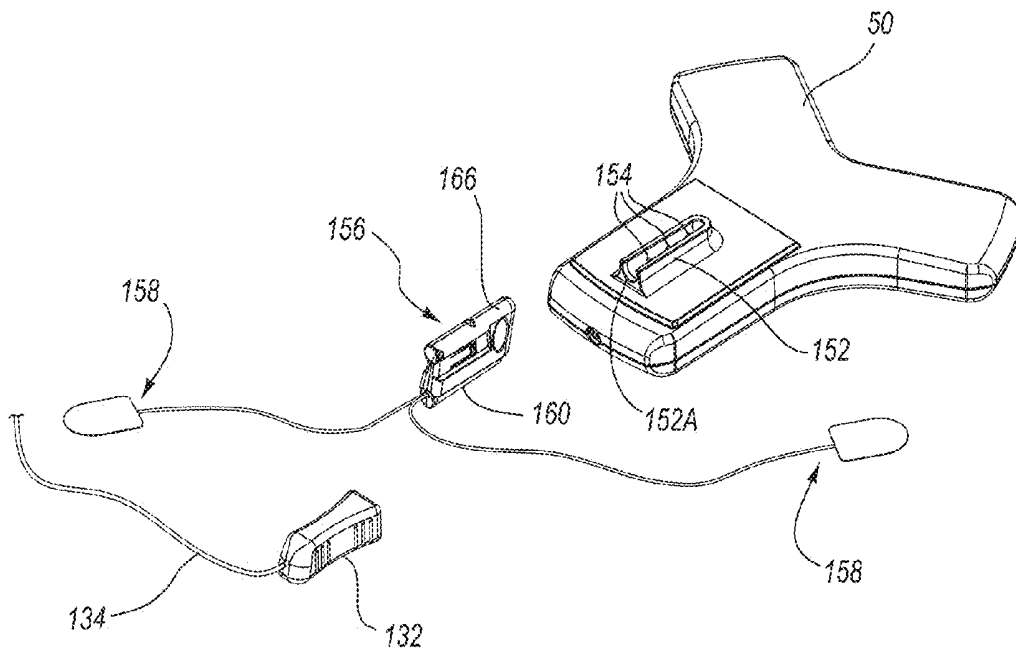


FIG. 14A

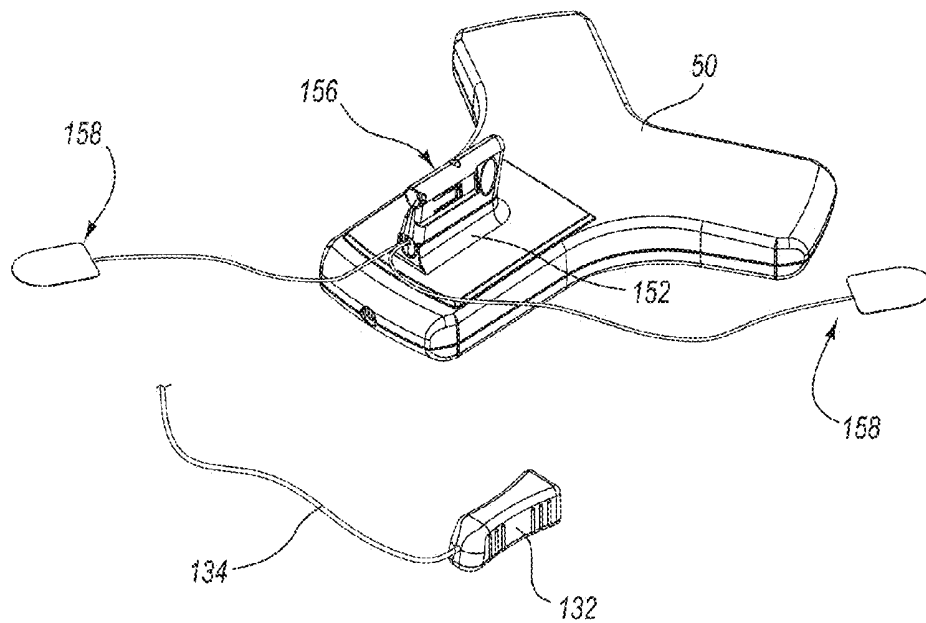


FIG. 14B



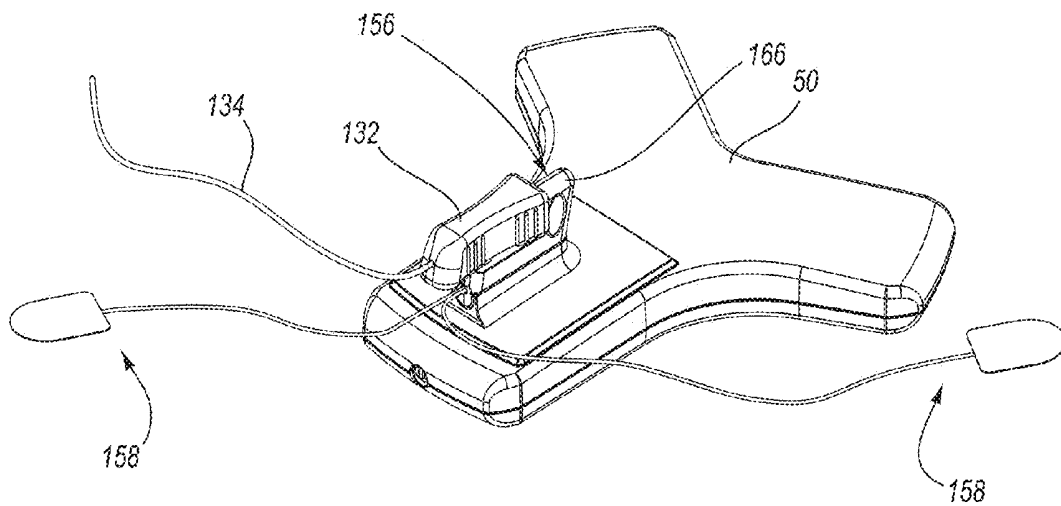


FIG. 14C

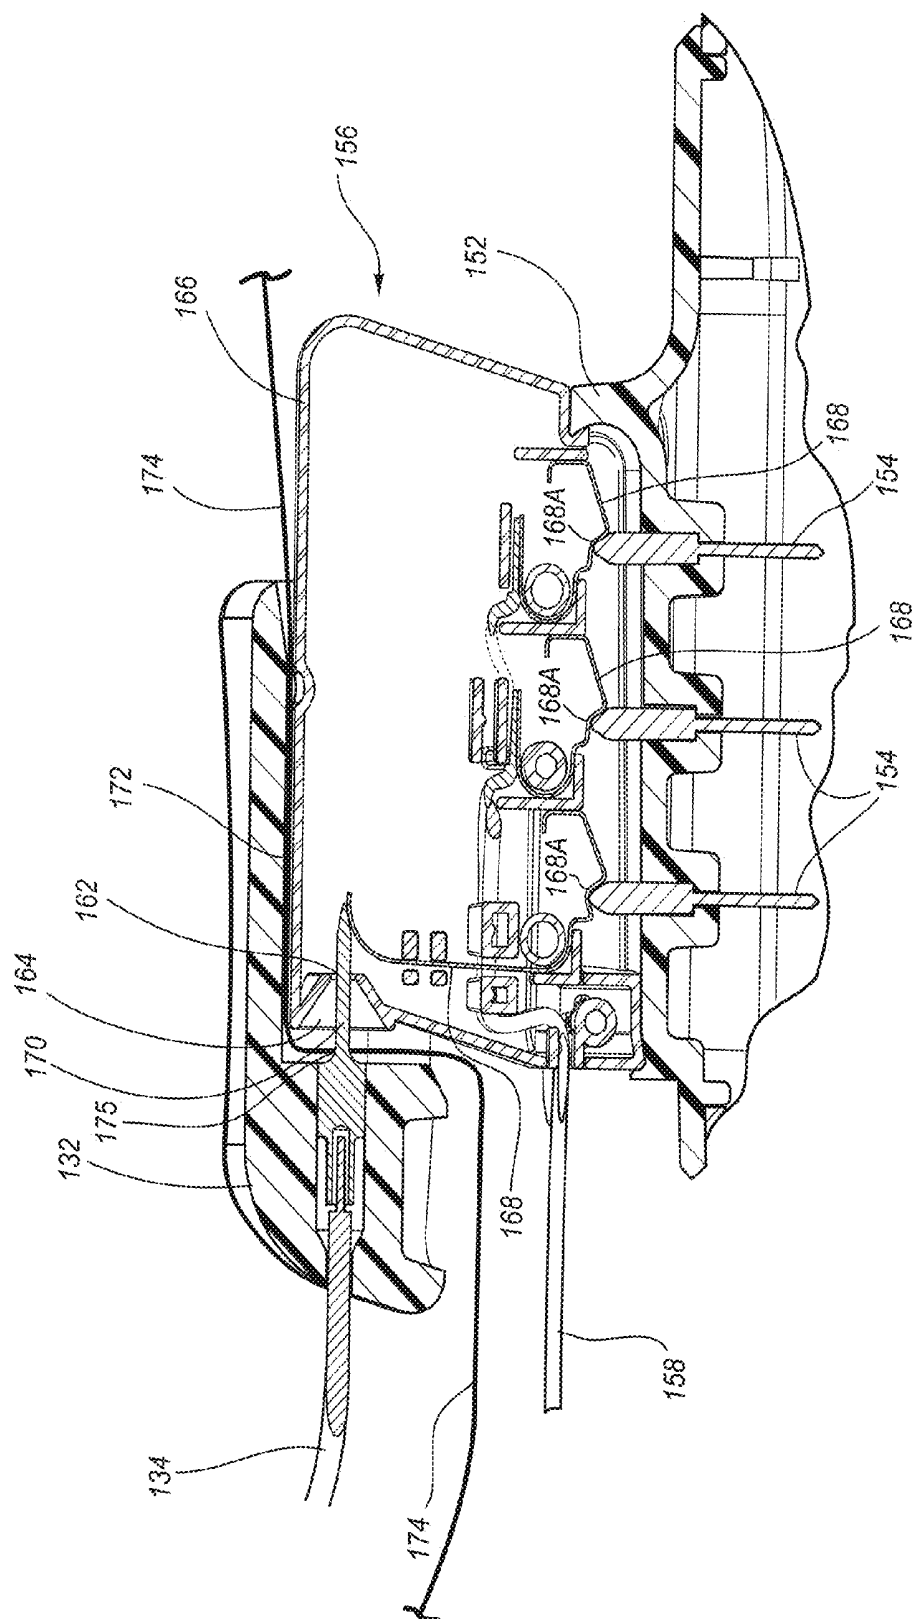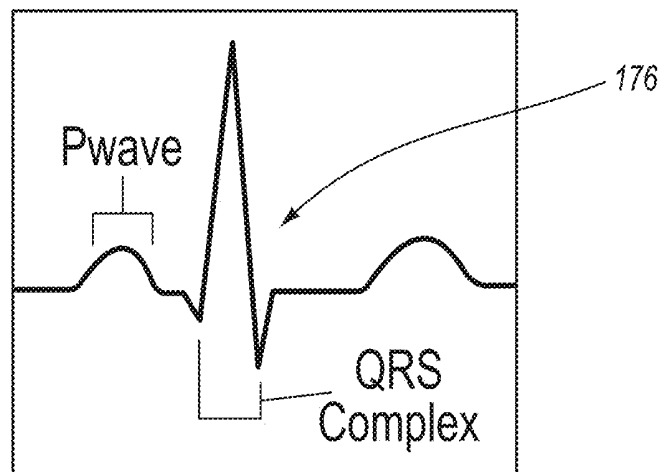

57
G^x
L

**FIG. 16**

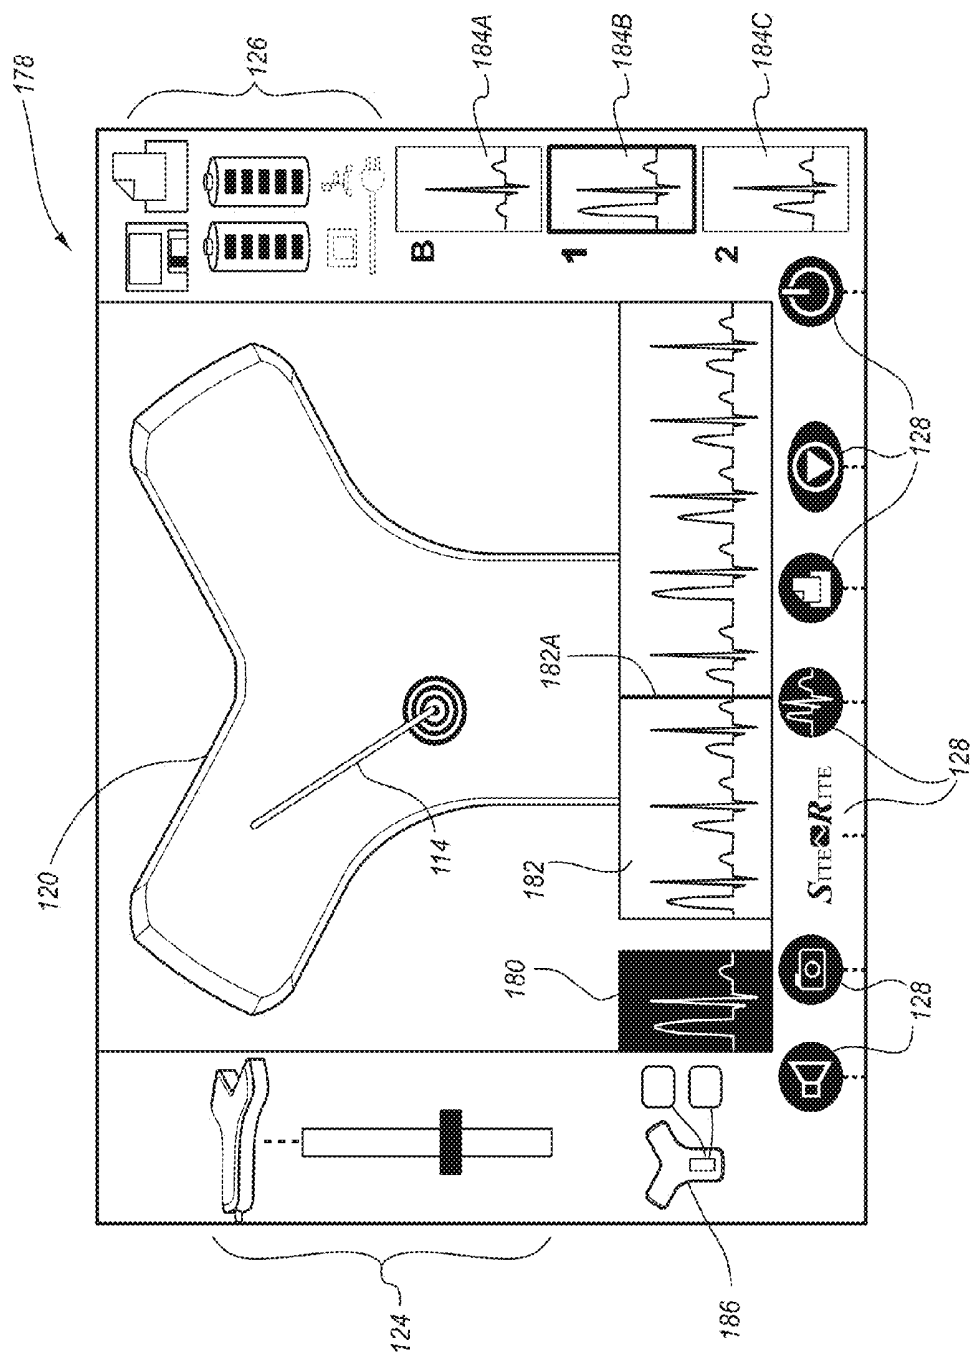


FIG. 17

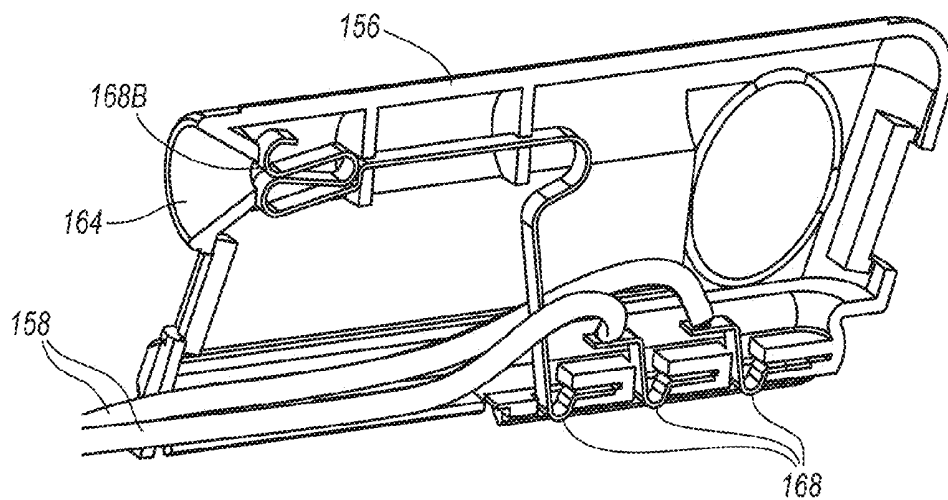


FIG. 18

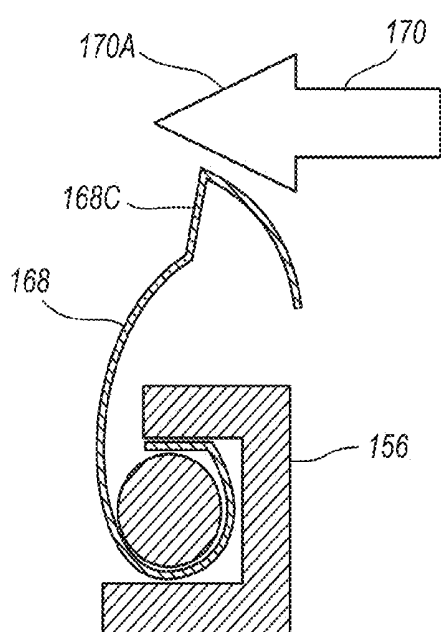


FIG. 19A

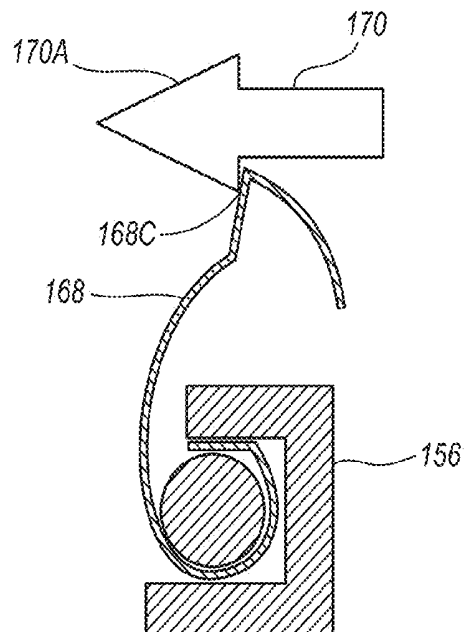
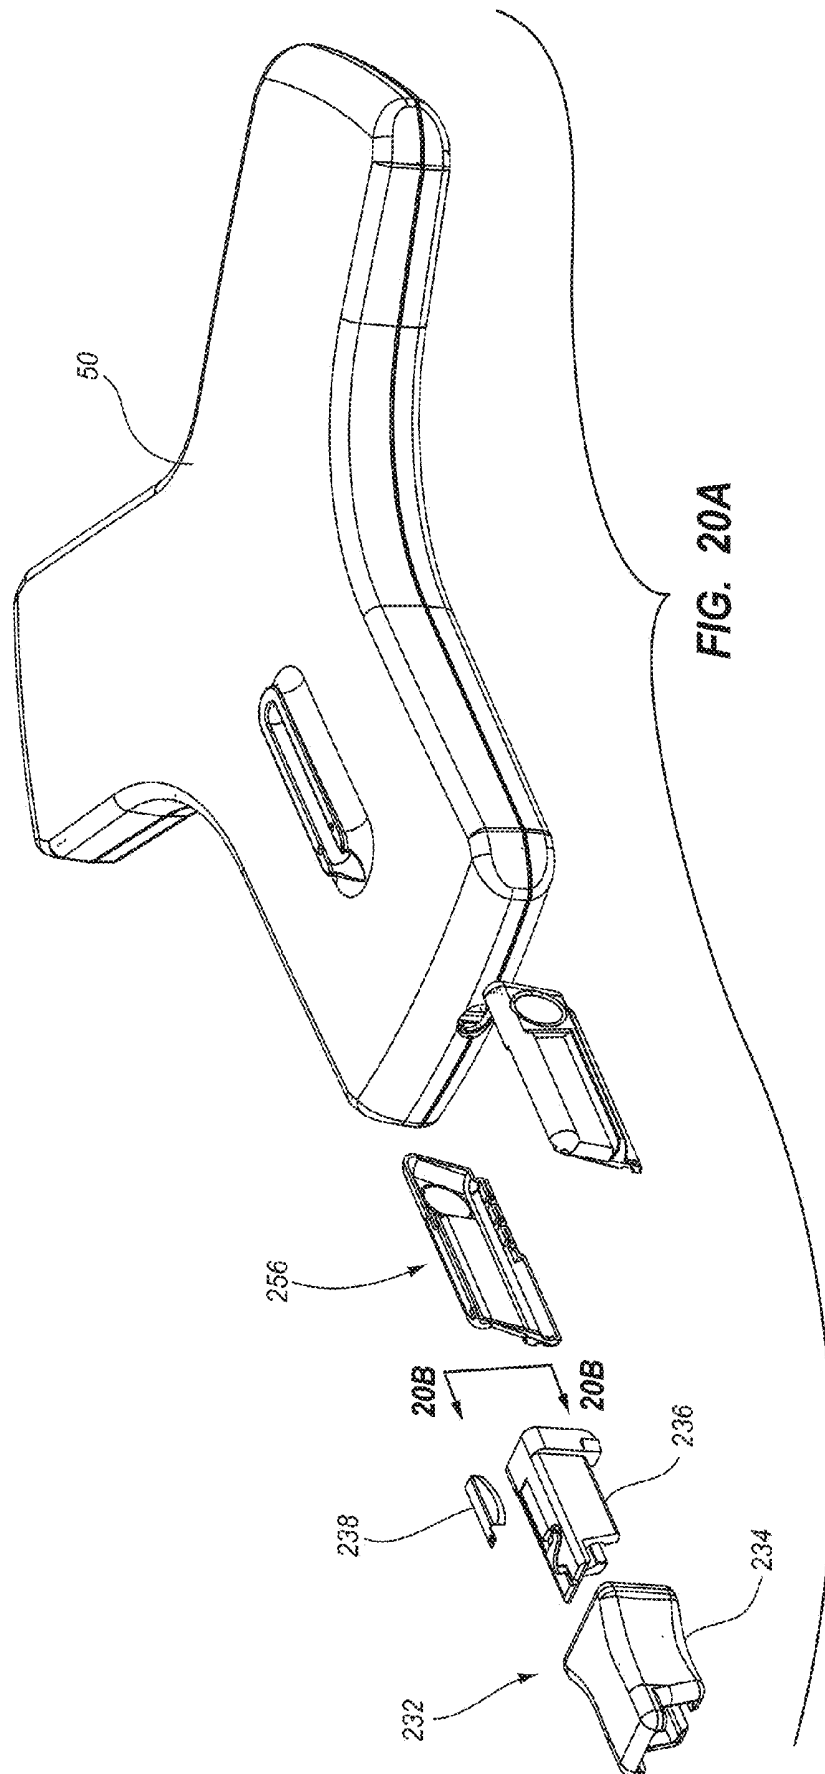


FIG. 19B



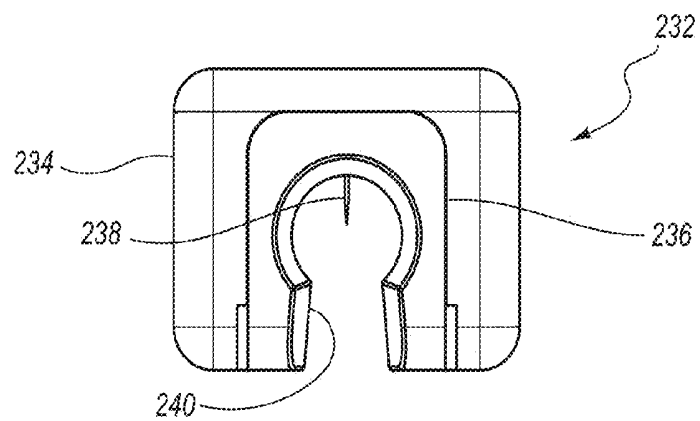


FIG. 20B

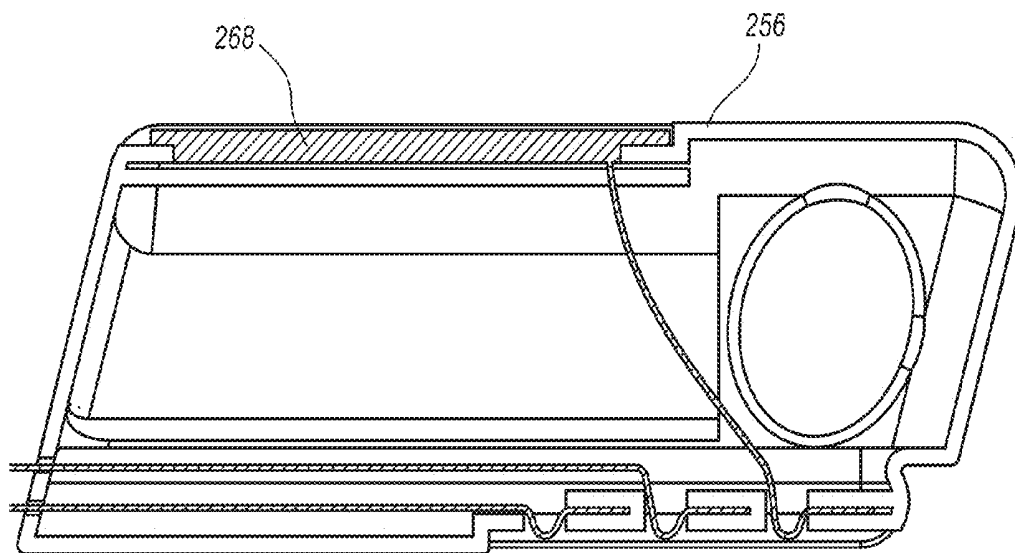


FIG. 20C

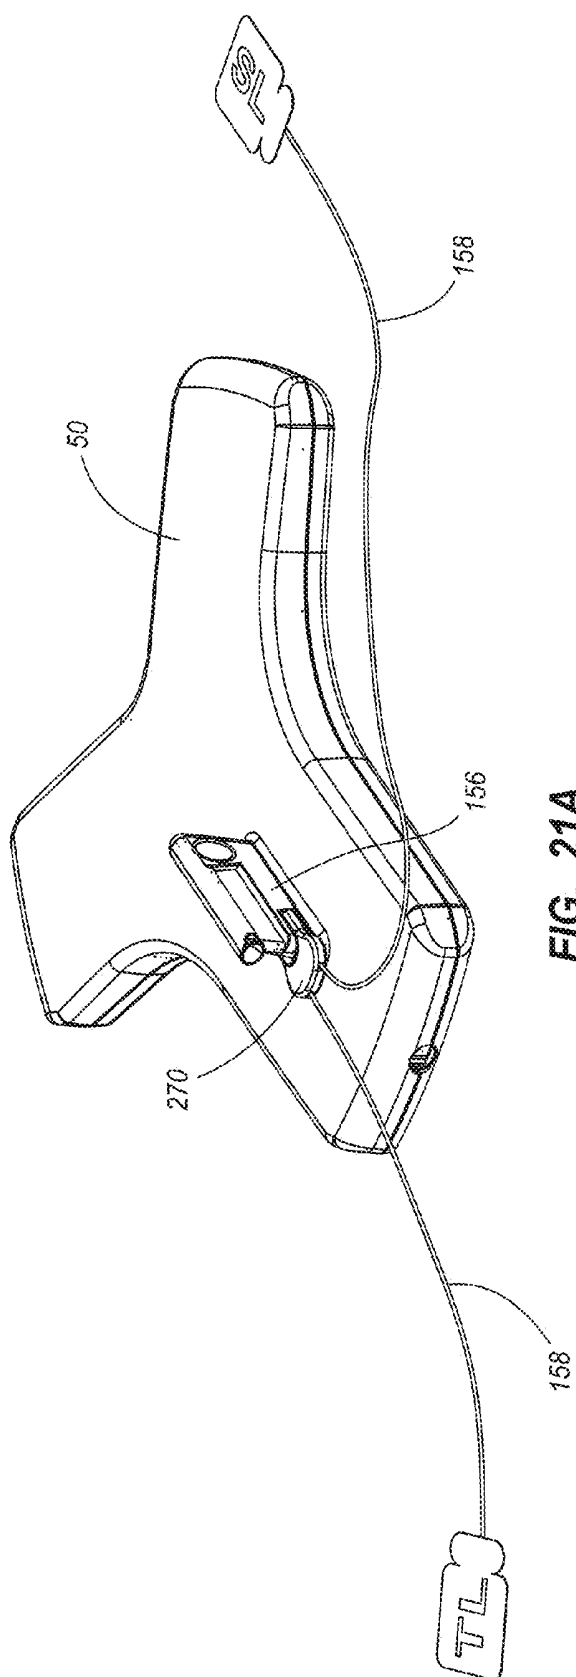


FIG. 21A

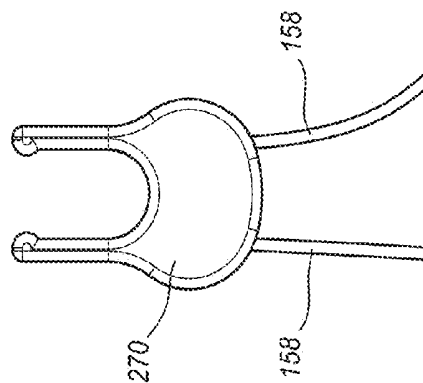


FIG. 21B

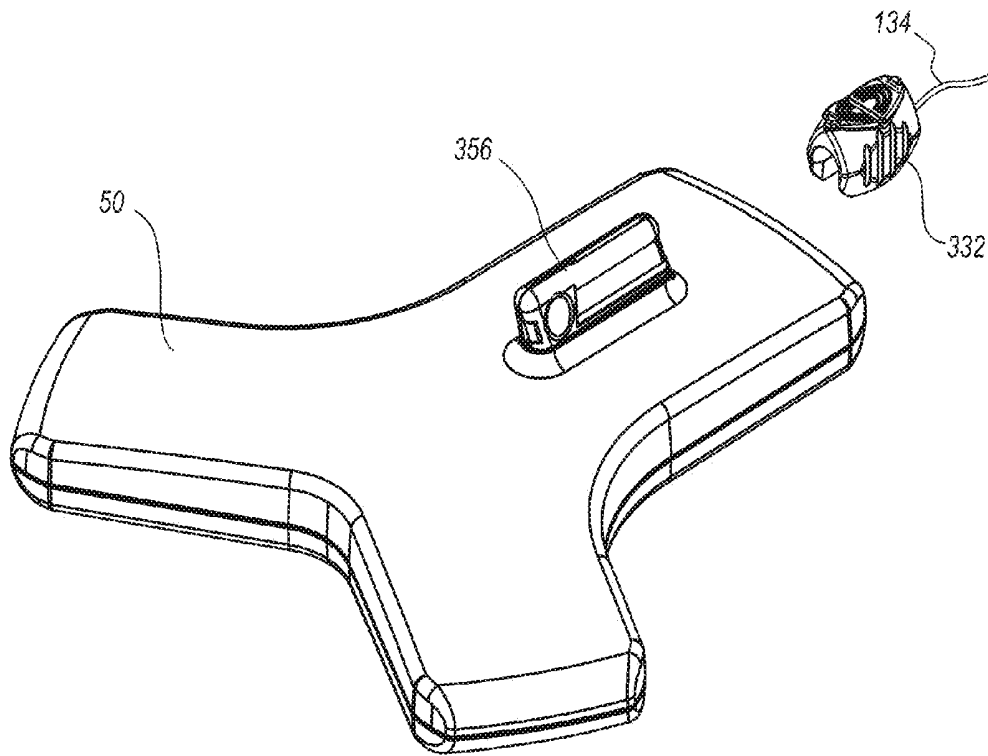


FIG. 22A

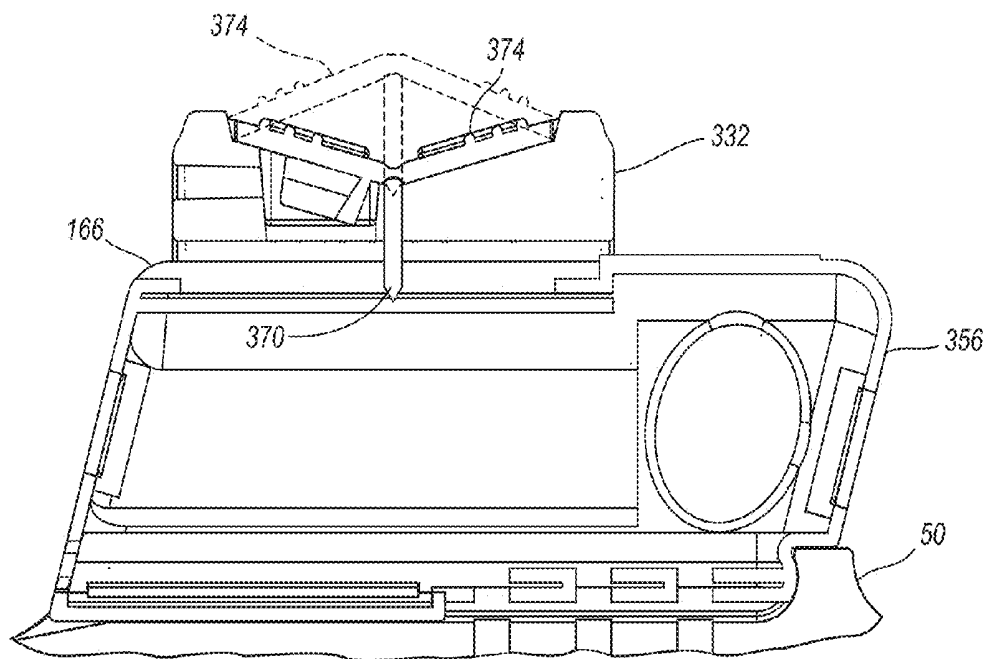


FIG. 22B

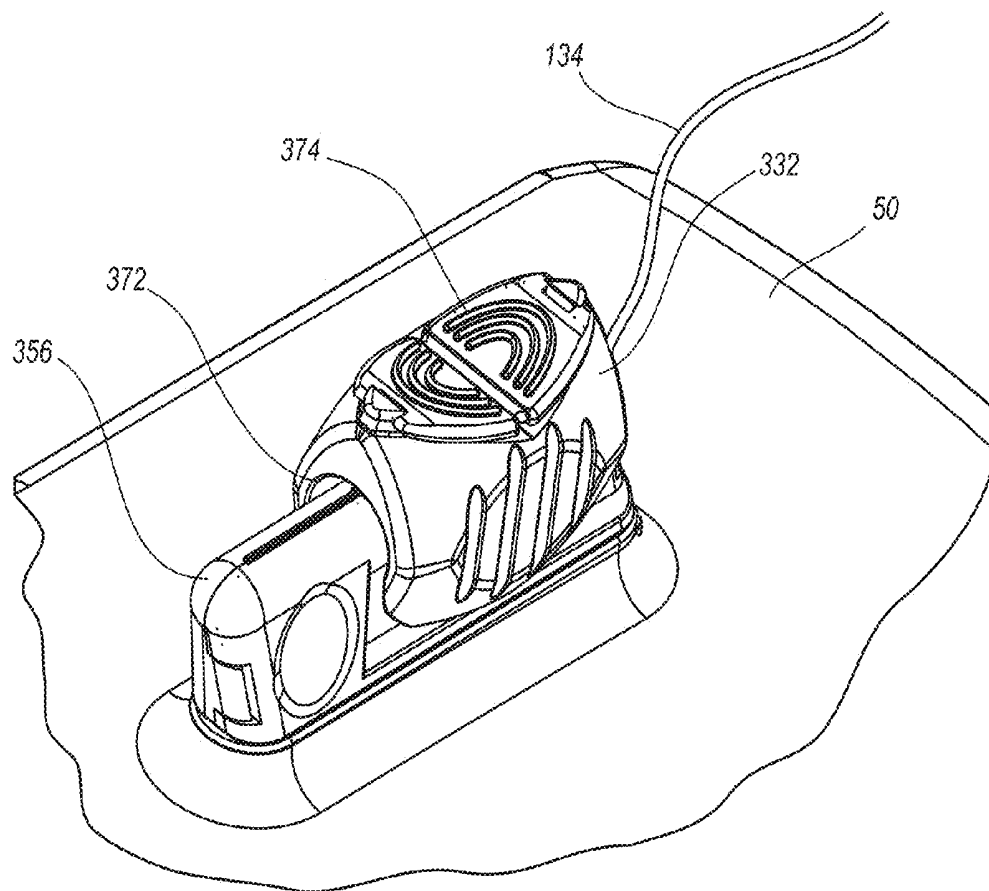


FIG. 22C

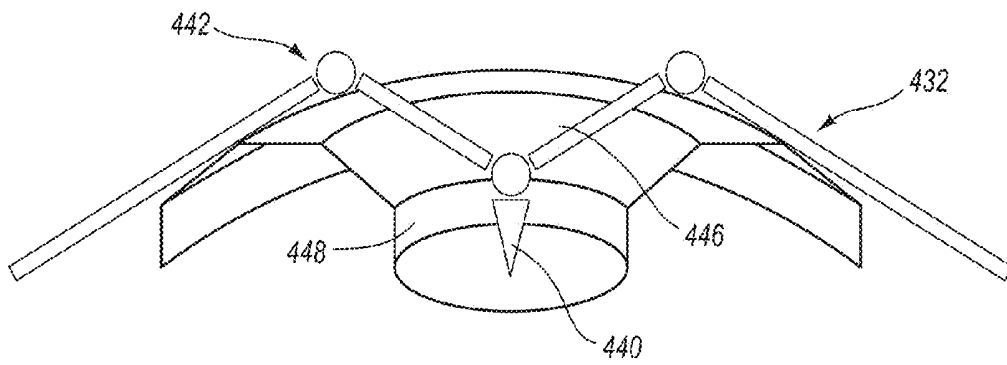


FIG. 23A

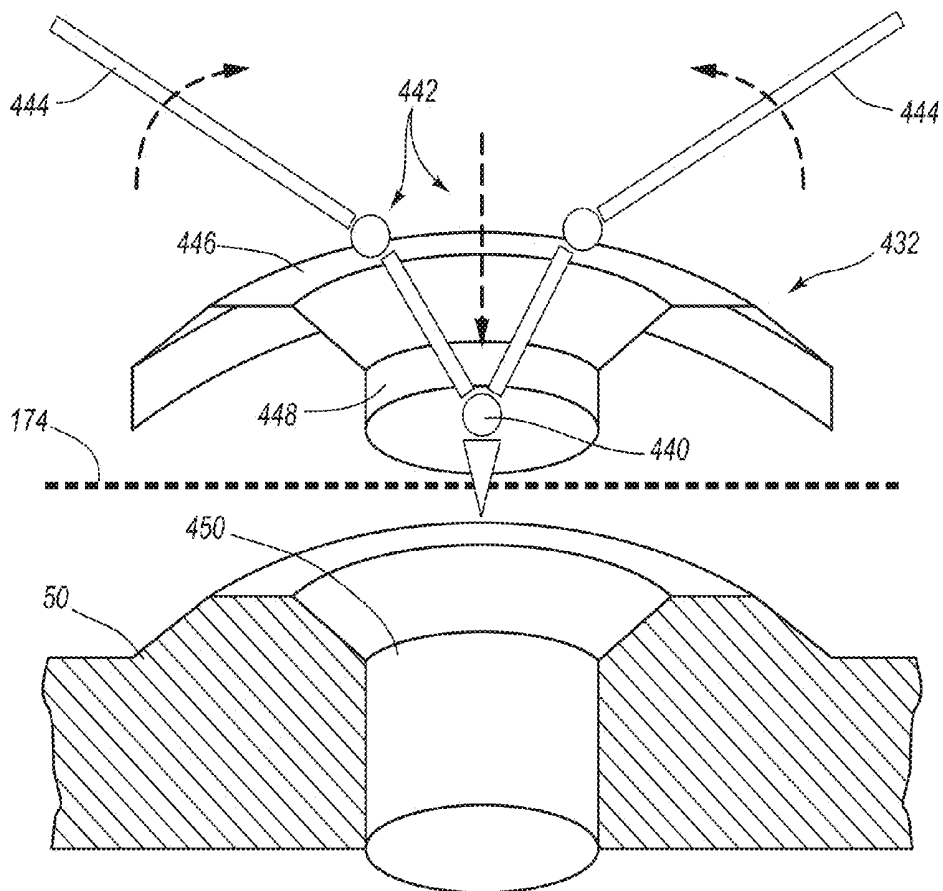
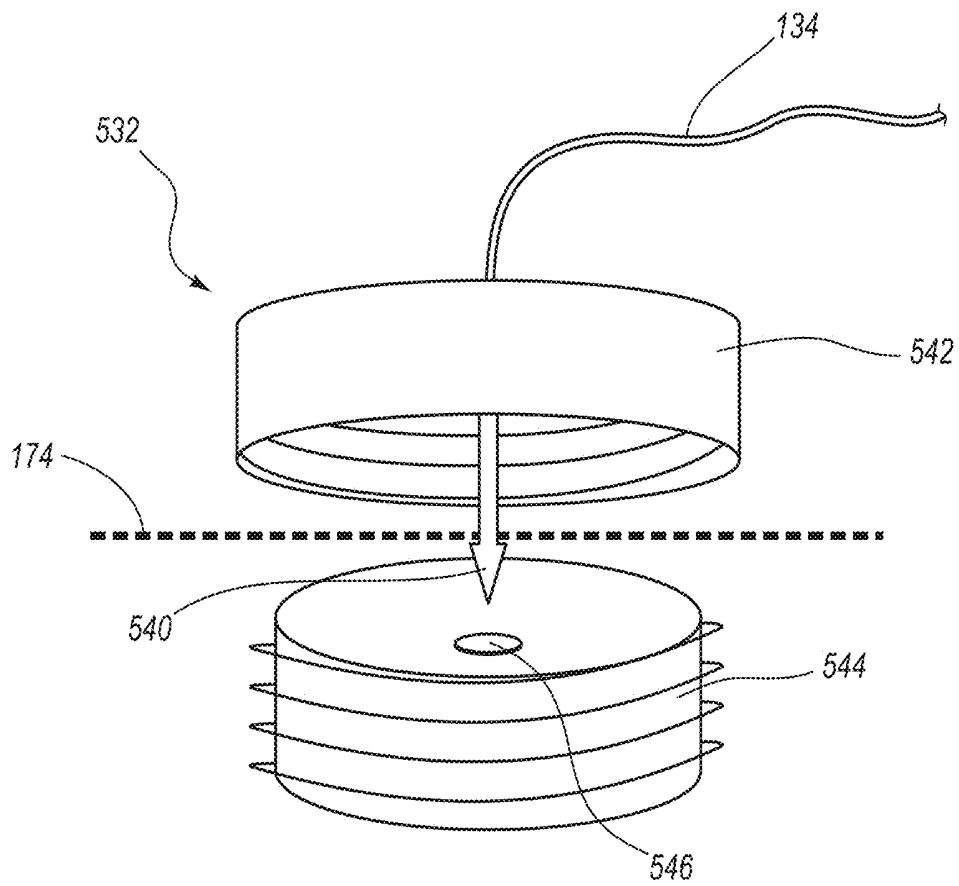


FIG. 23B

**FIG. 24**

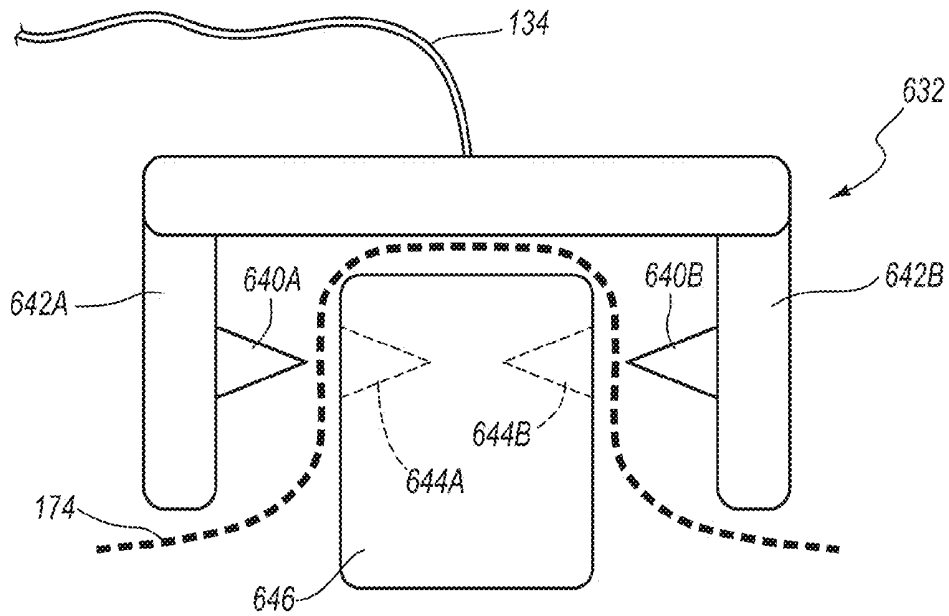


FIG. 25A

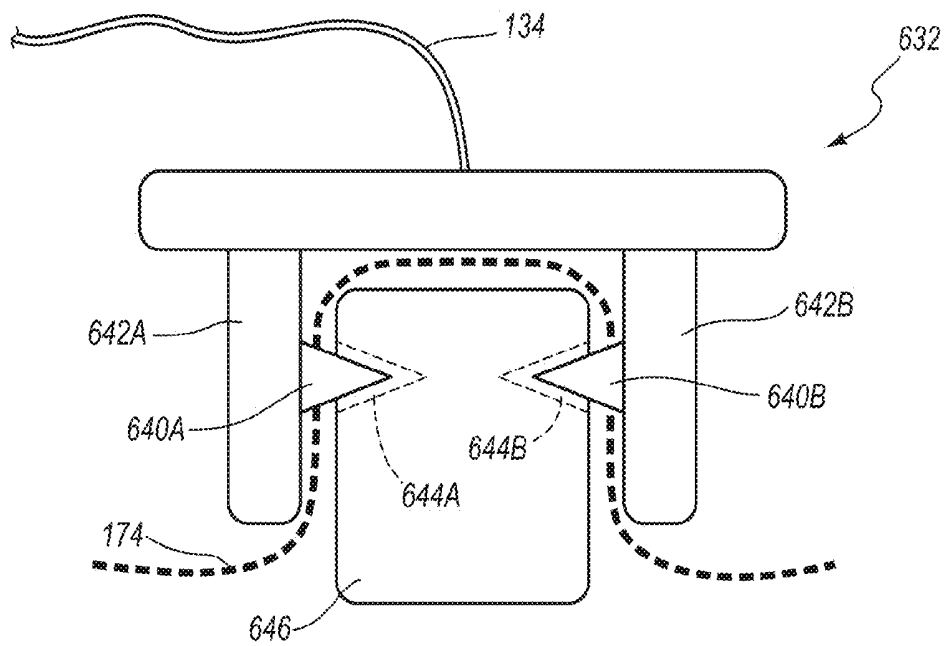


FIG. 25B

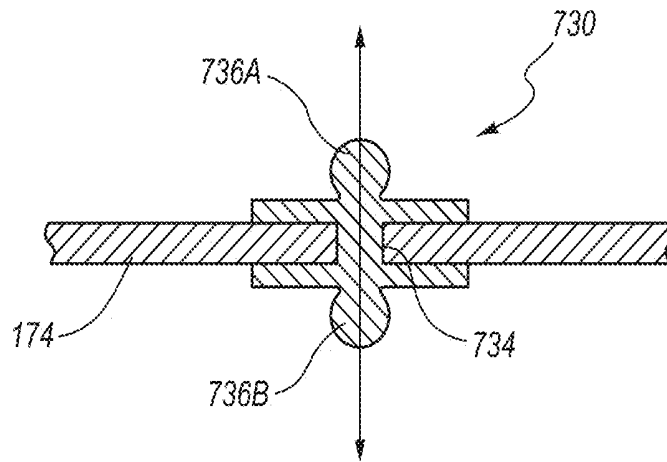


FIG. 26A

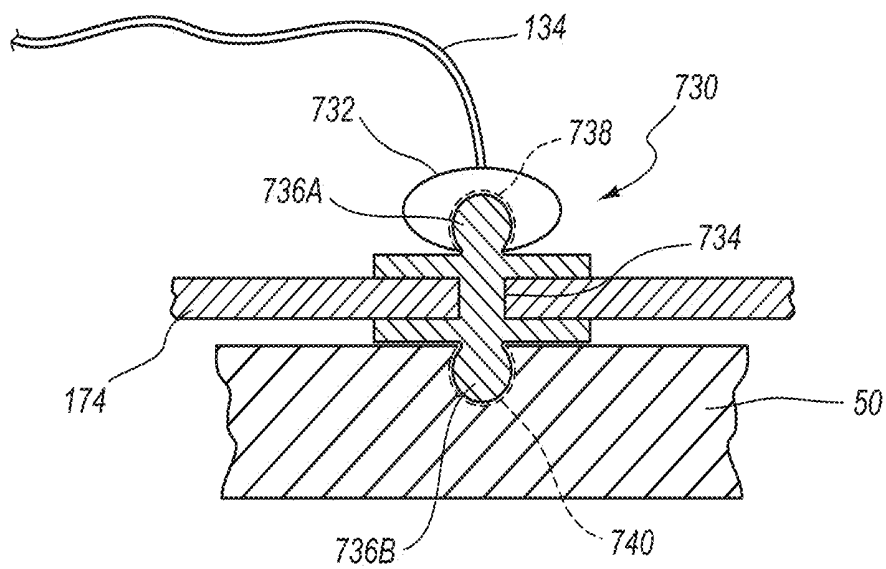


FIG. 26B

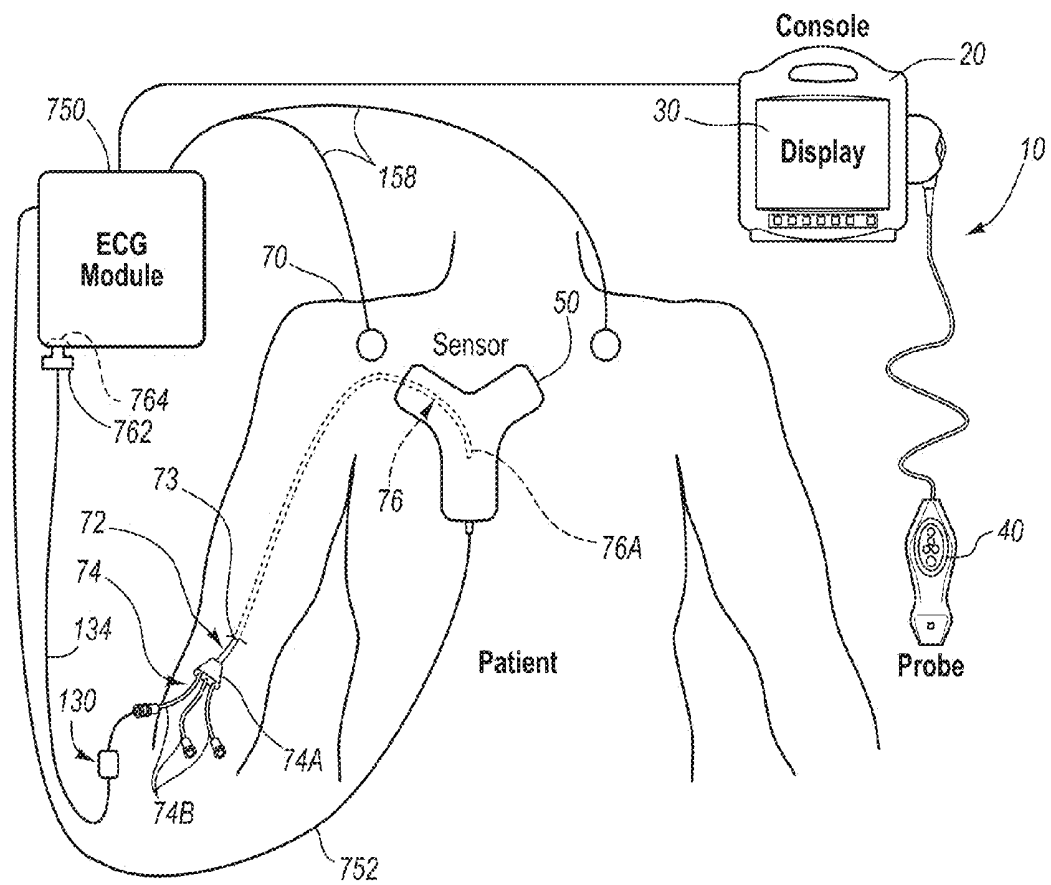


FIG. 27

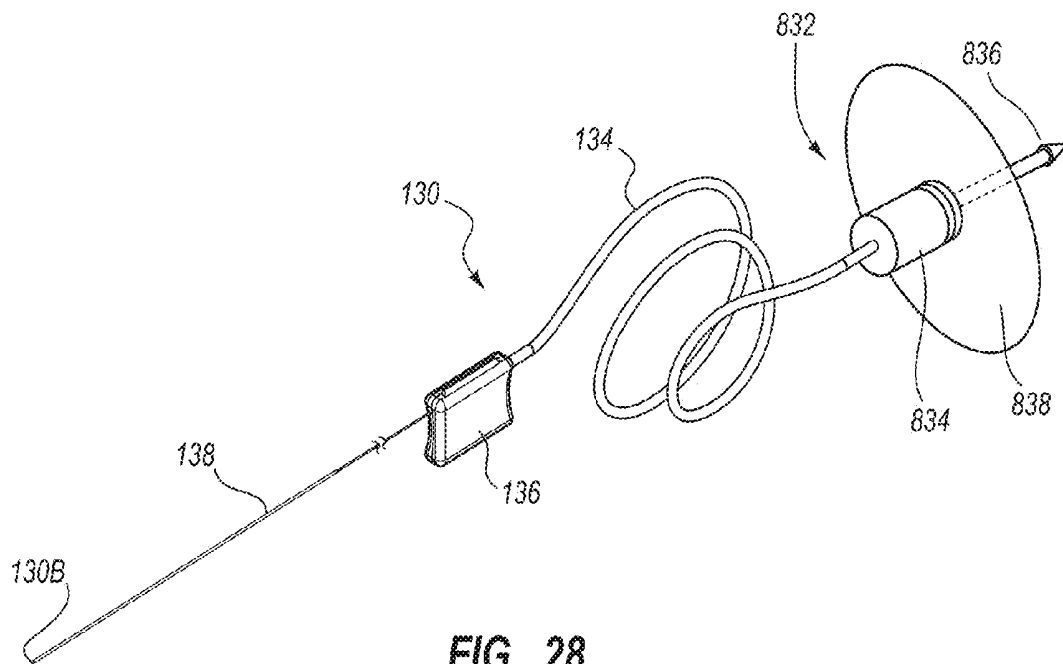
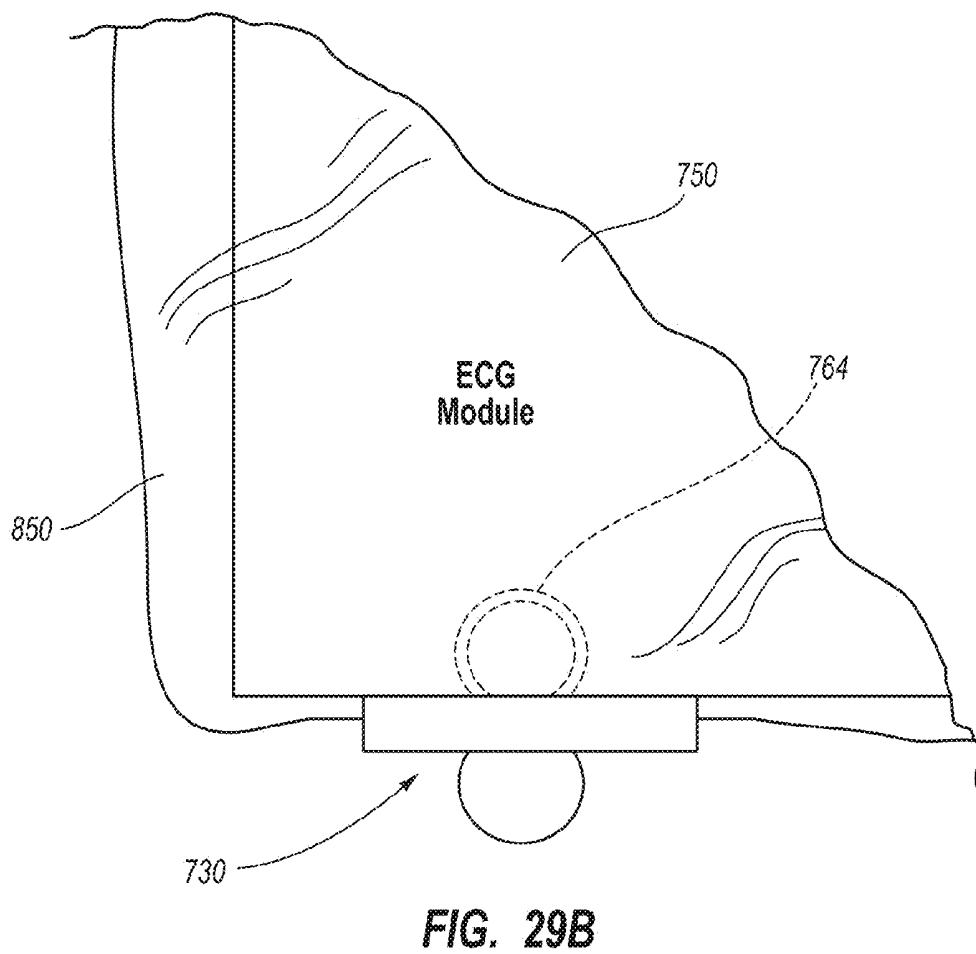
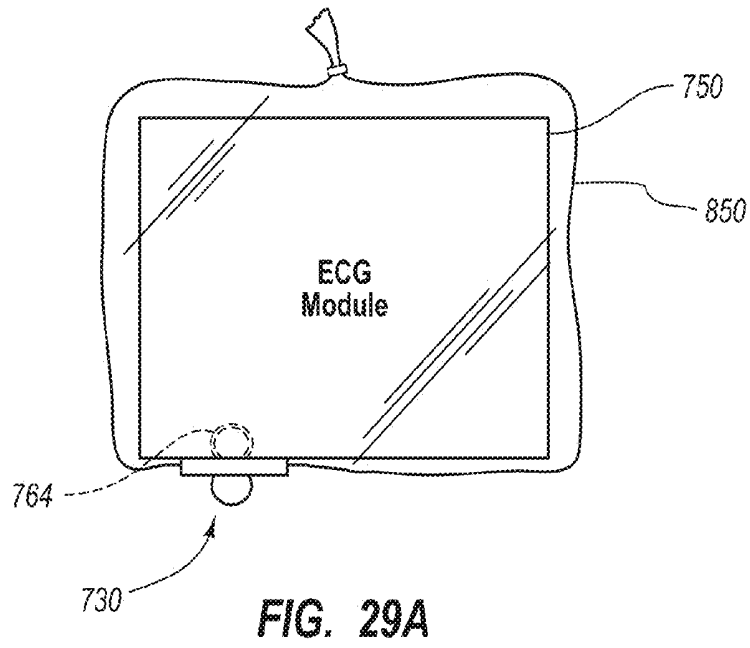
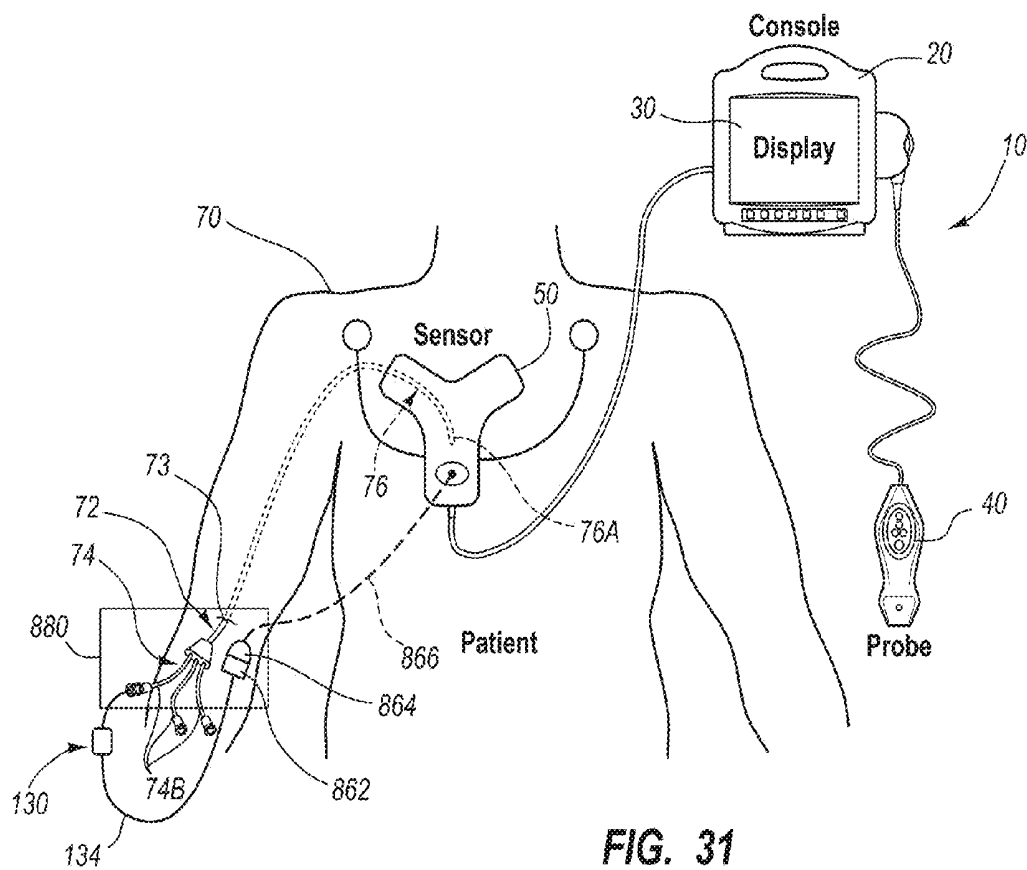
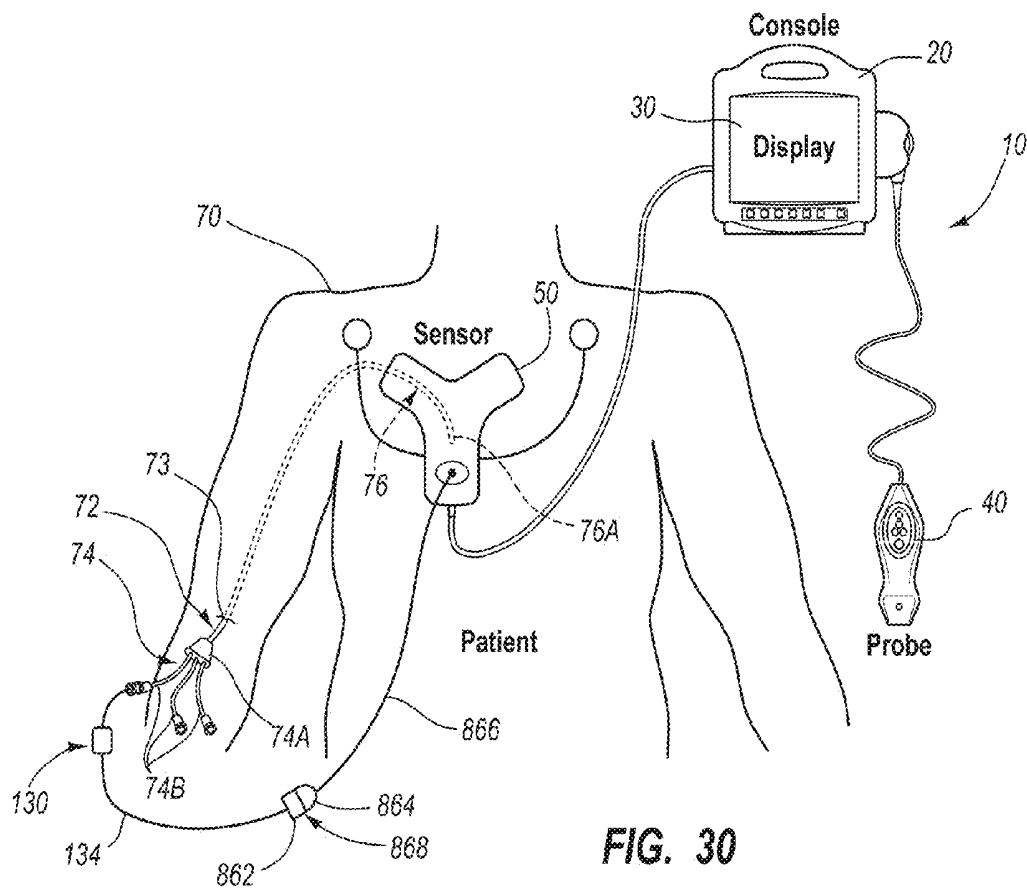


FIG. 28





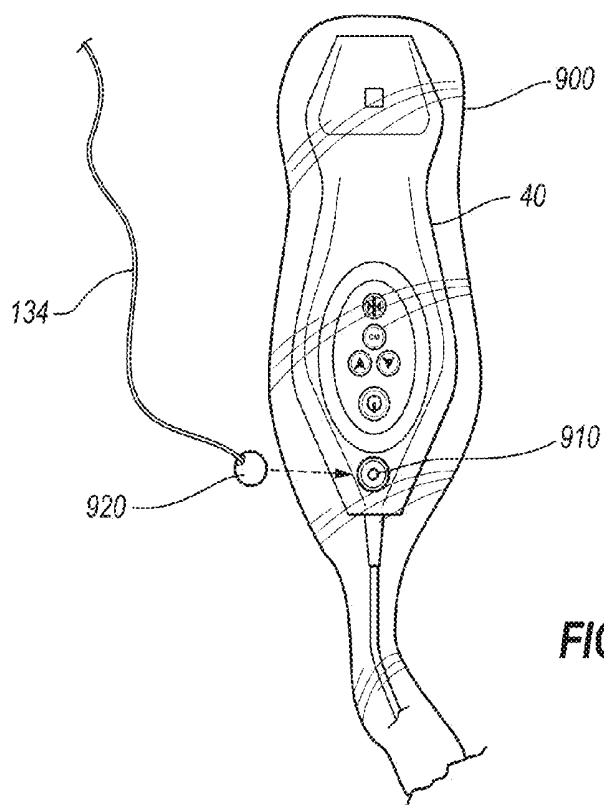


FIG. 32

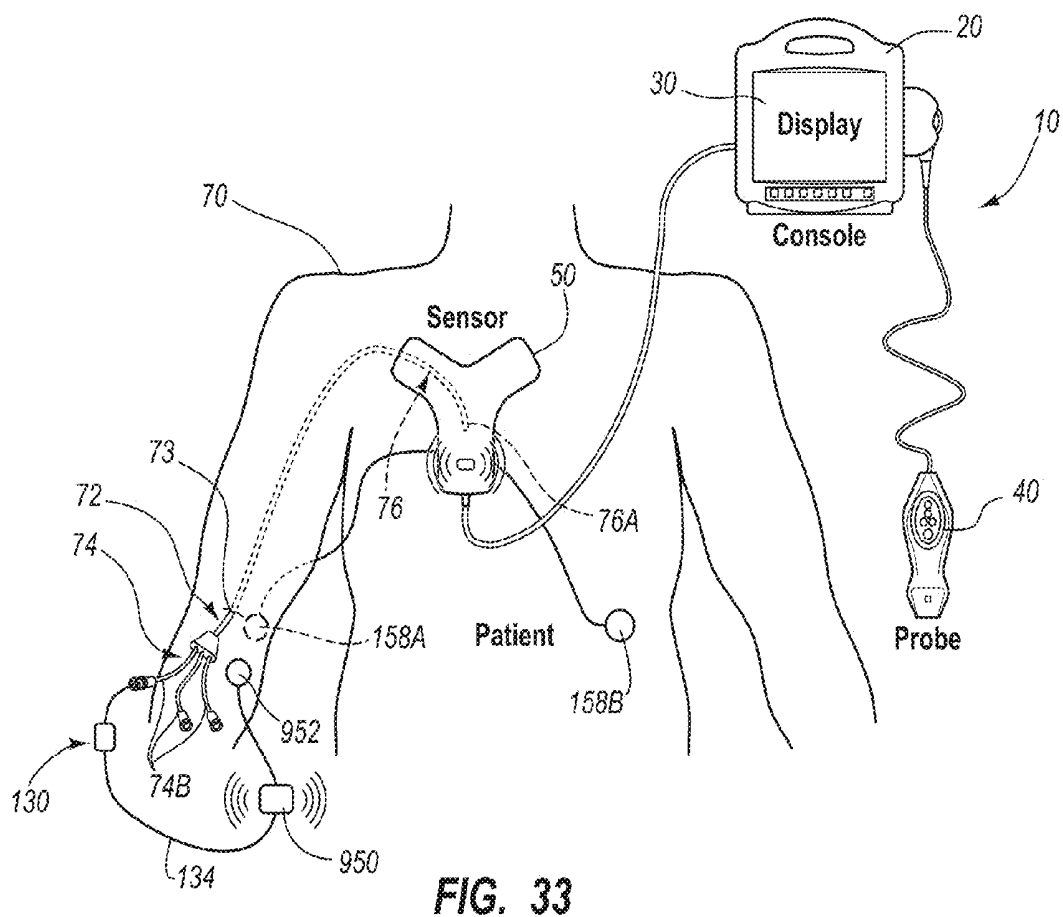


FIG. 33

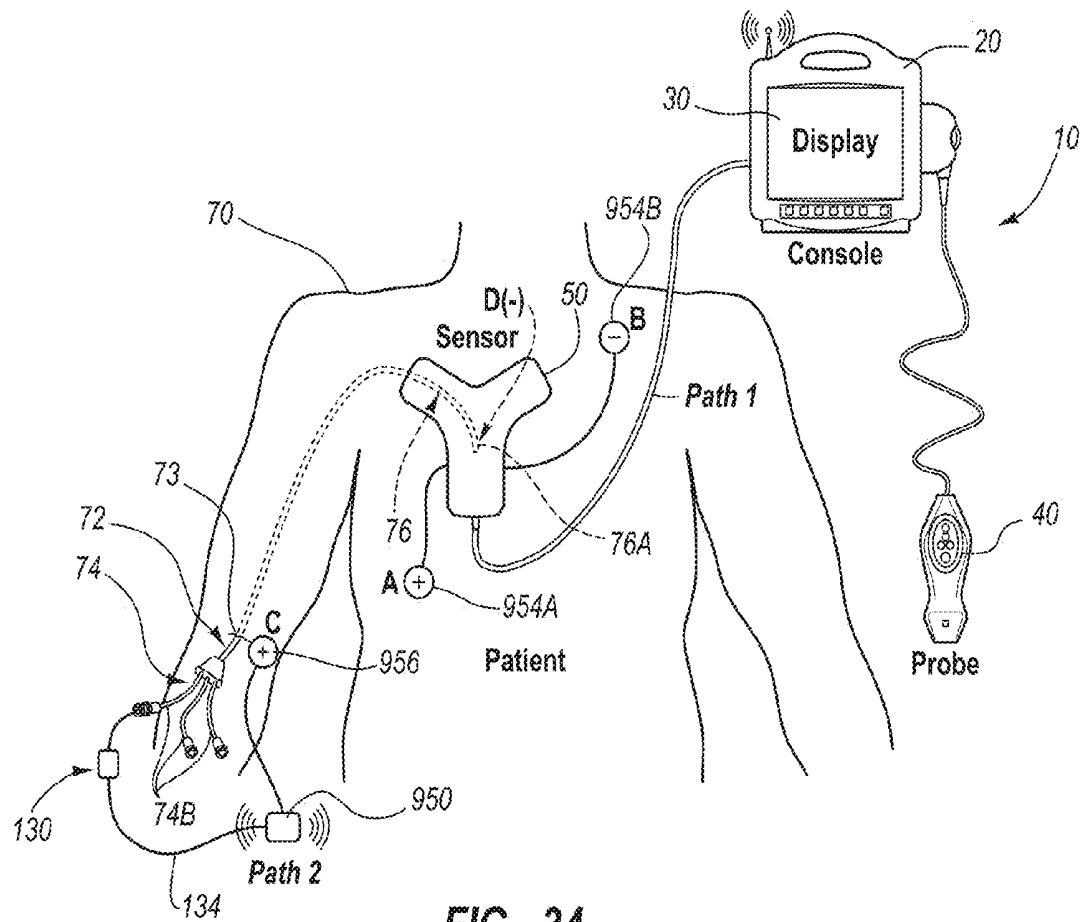


FIG. 34

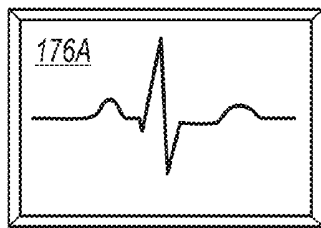


FIG. 35A

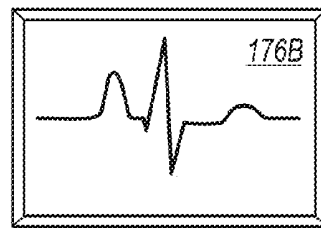


FIG. 35B

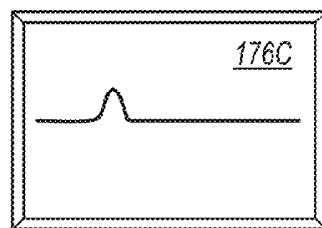


FIG. 35C

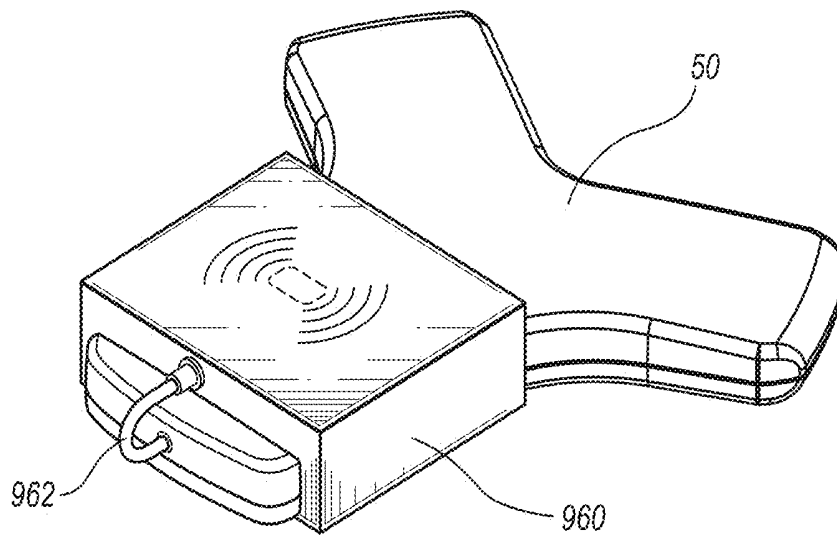


FIG. 36




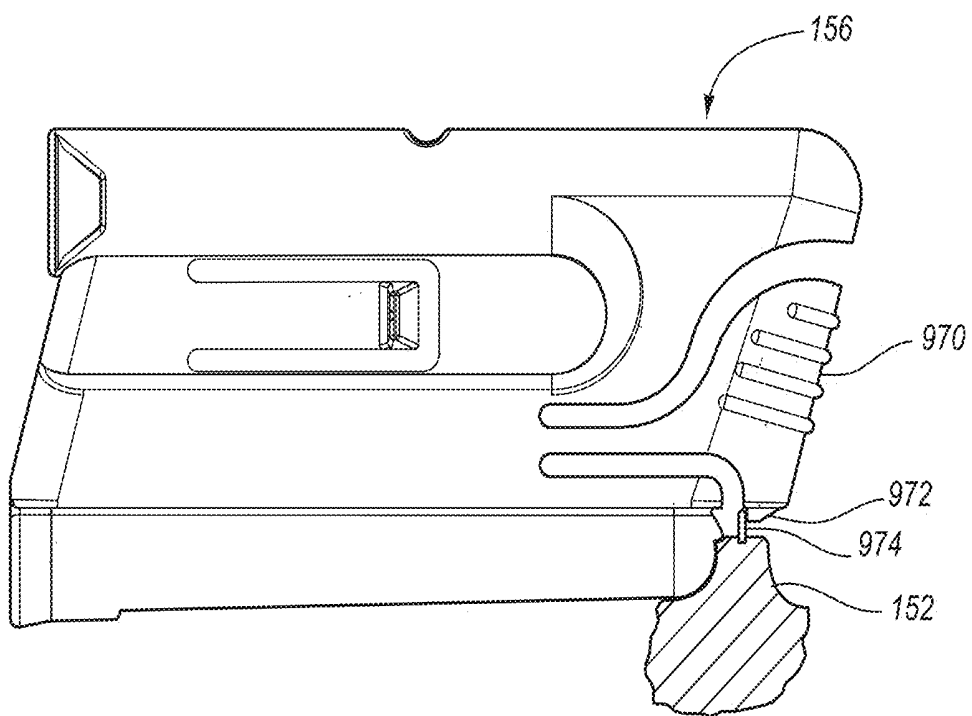


FIG. 37

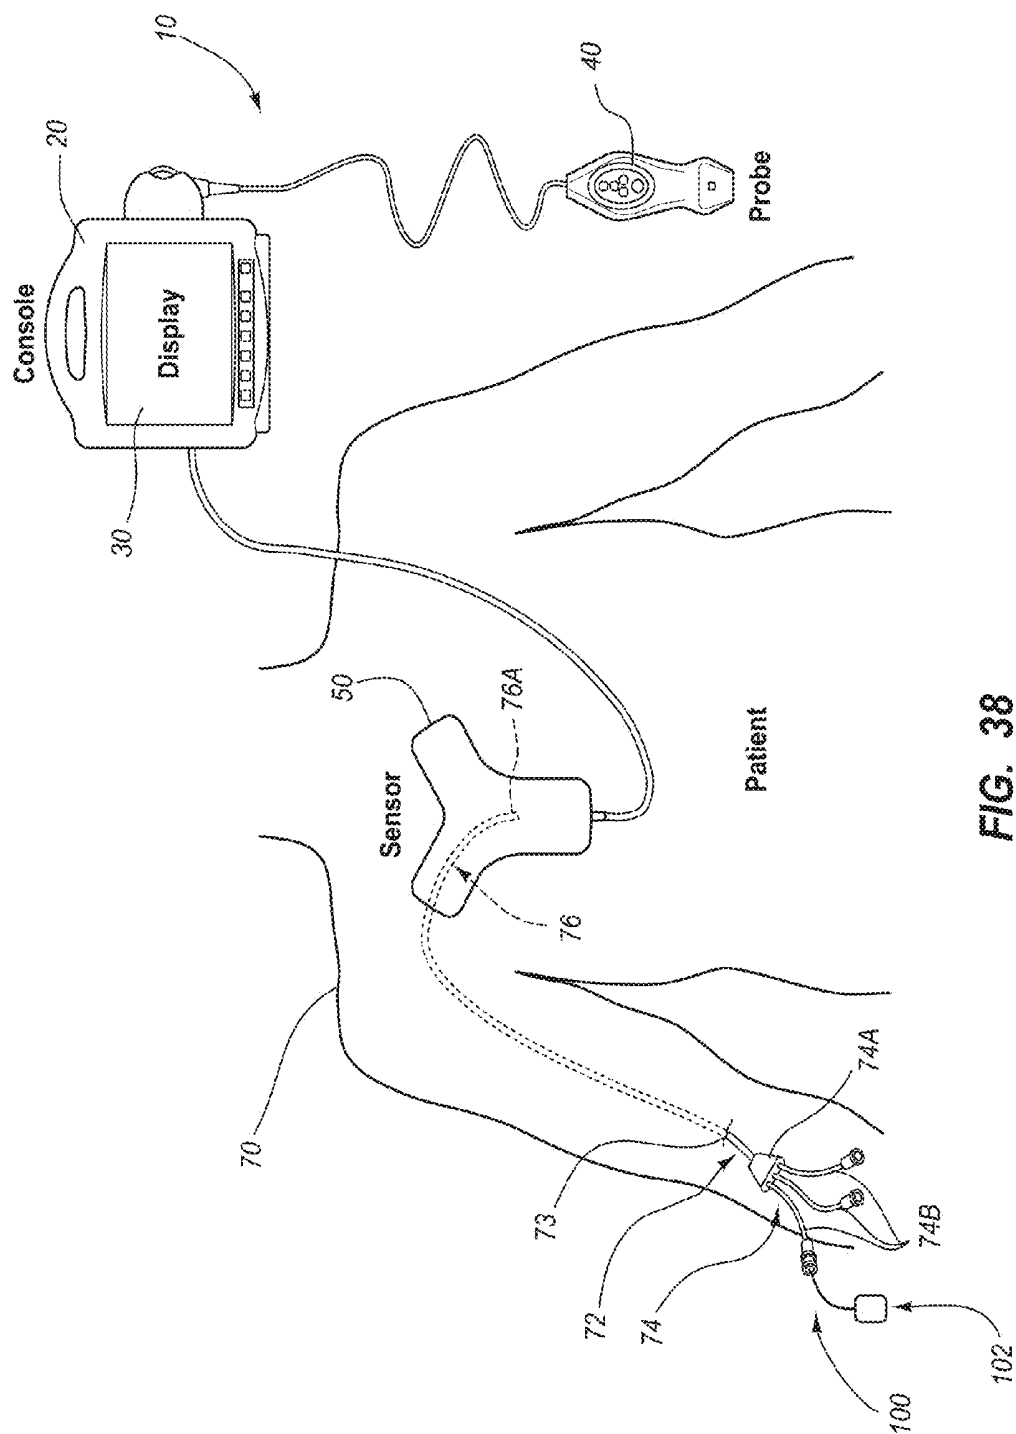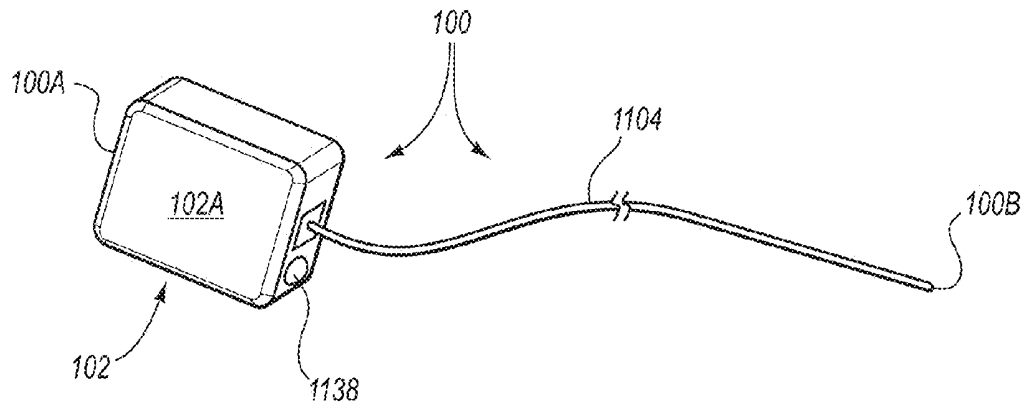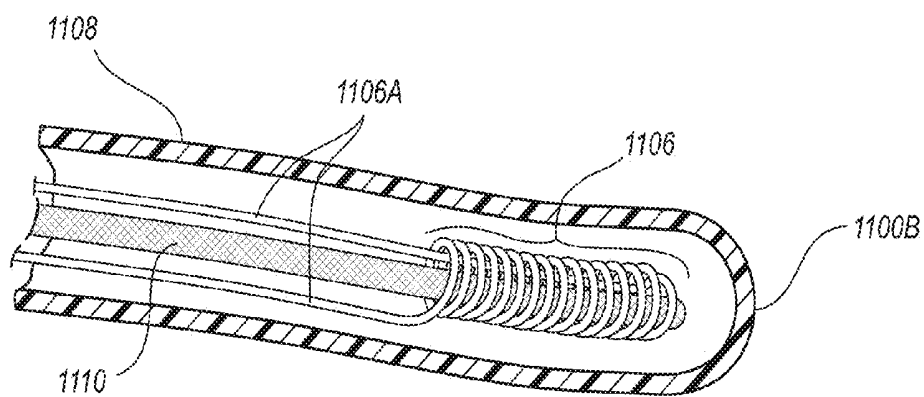

30

**FIG. 39****FIG. 40**

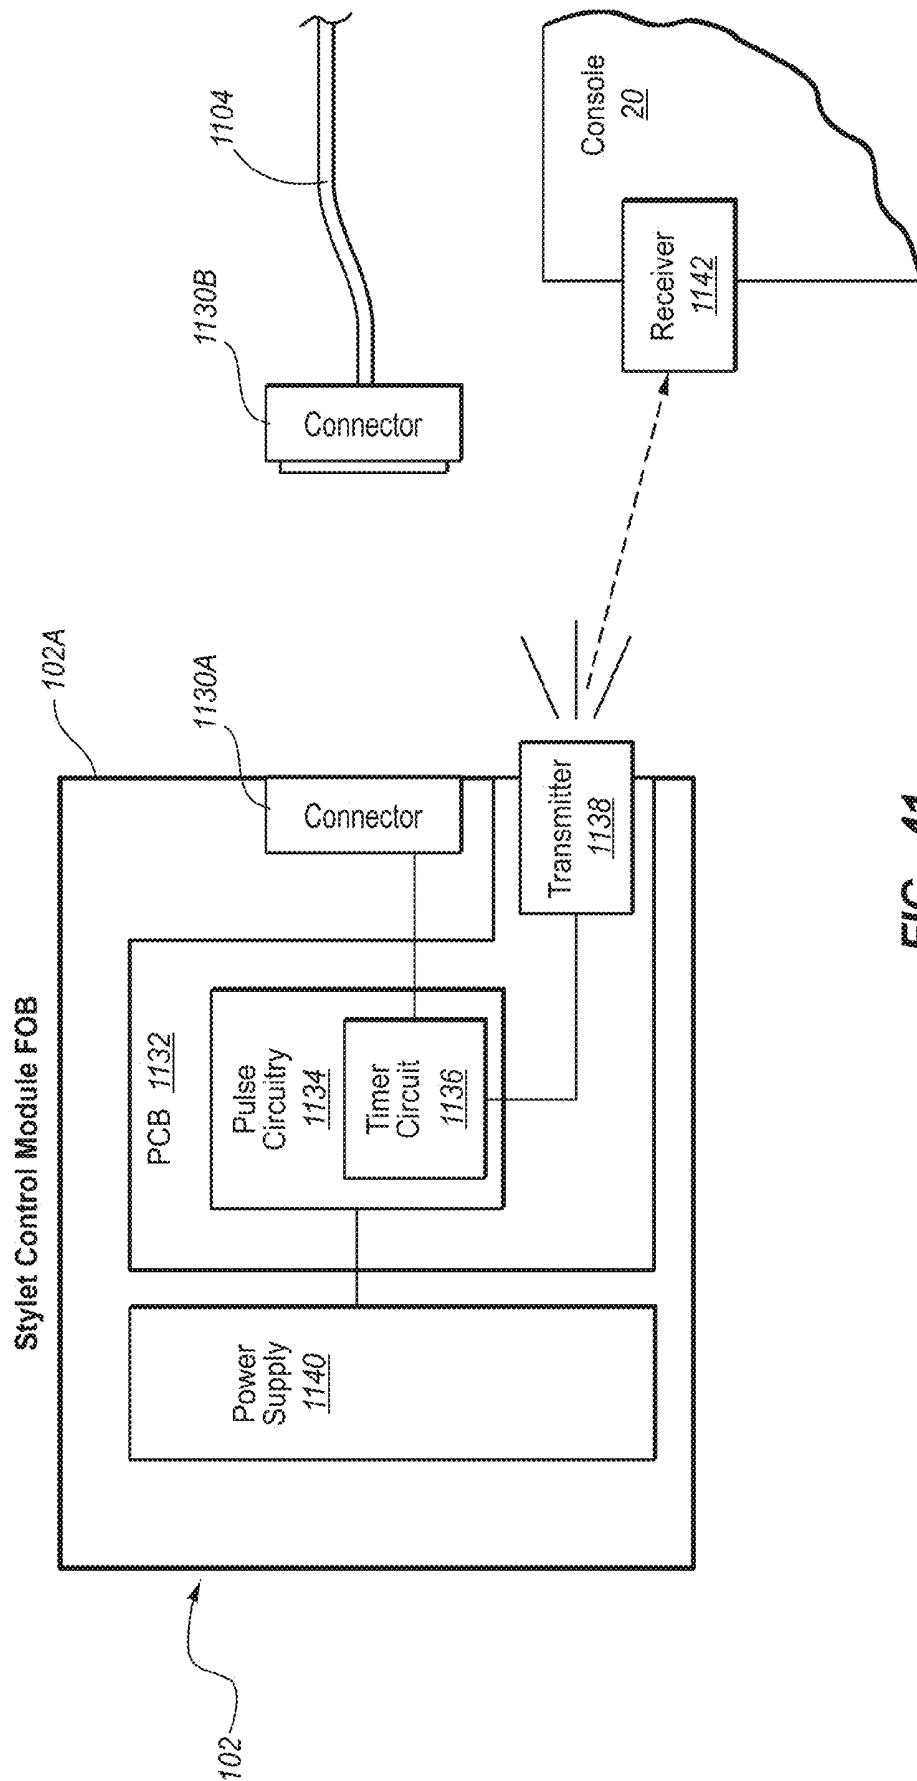


FIG. 41

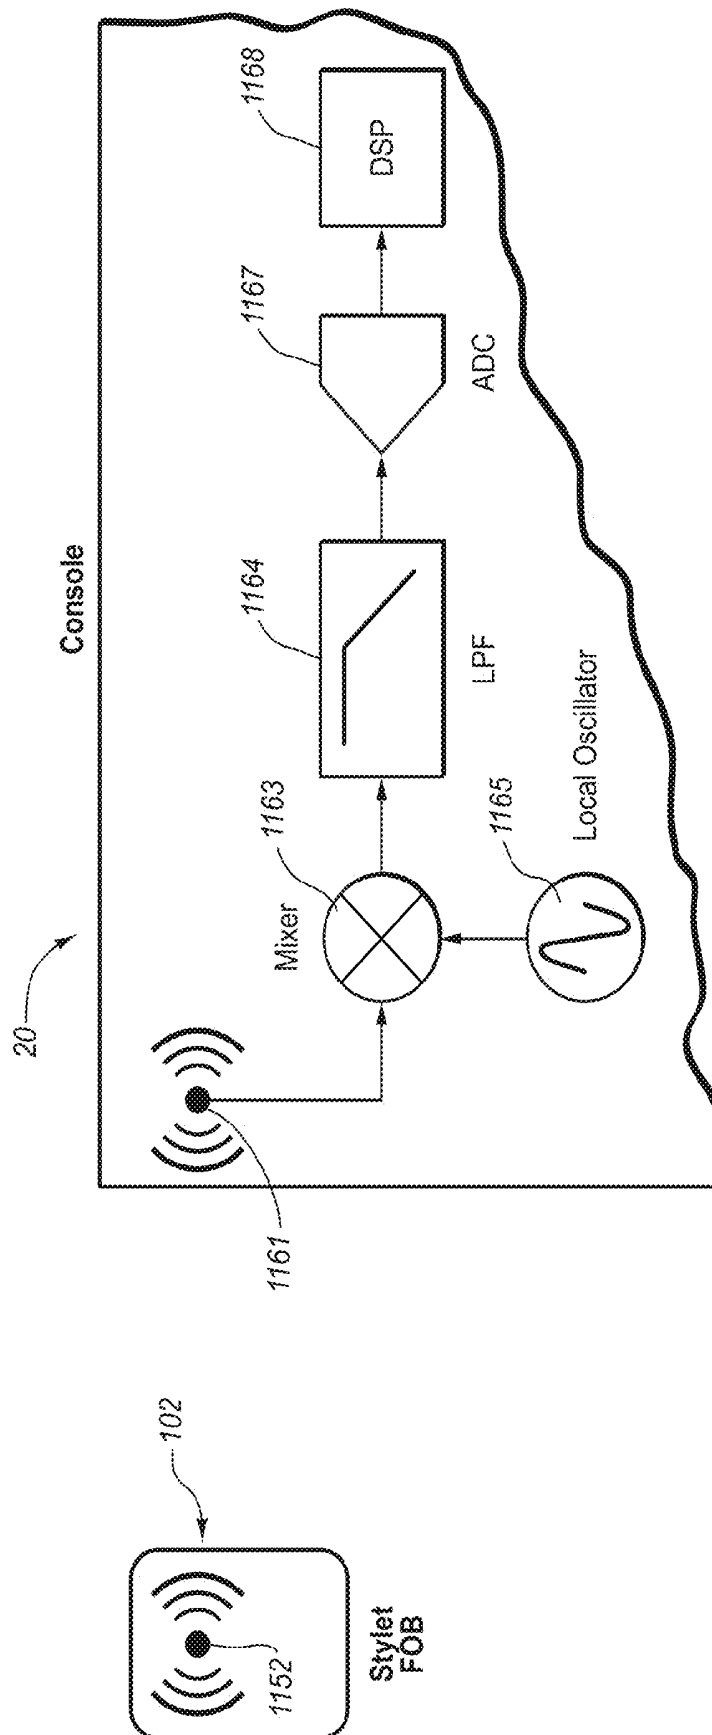


FIG. 42

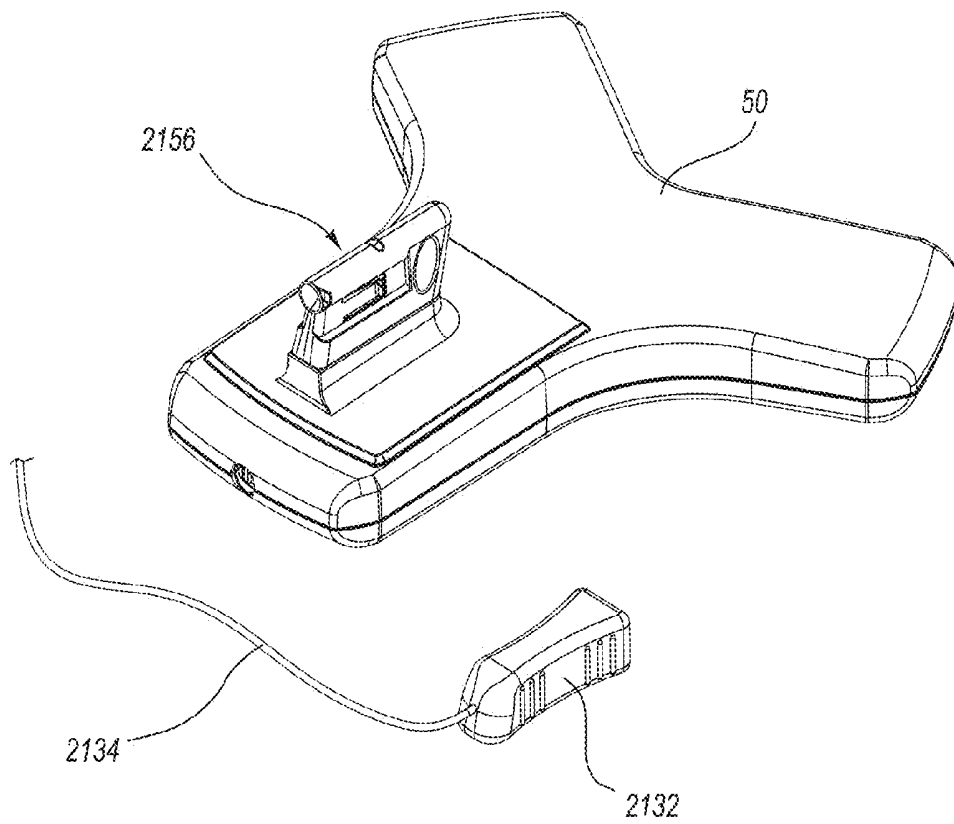


FIG. 43A

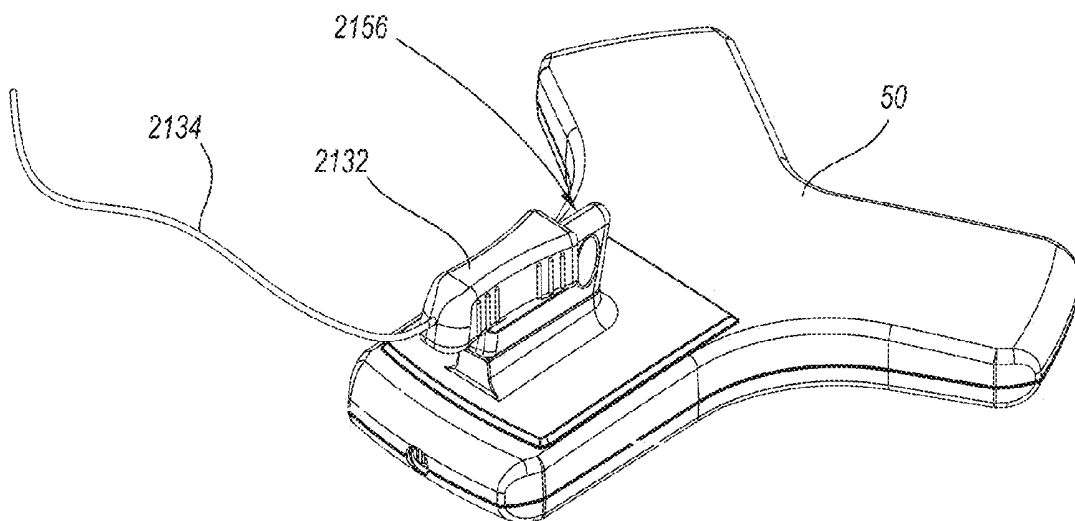


FIG. 43B

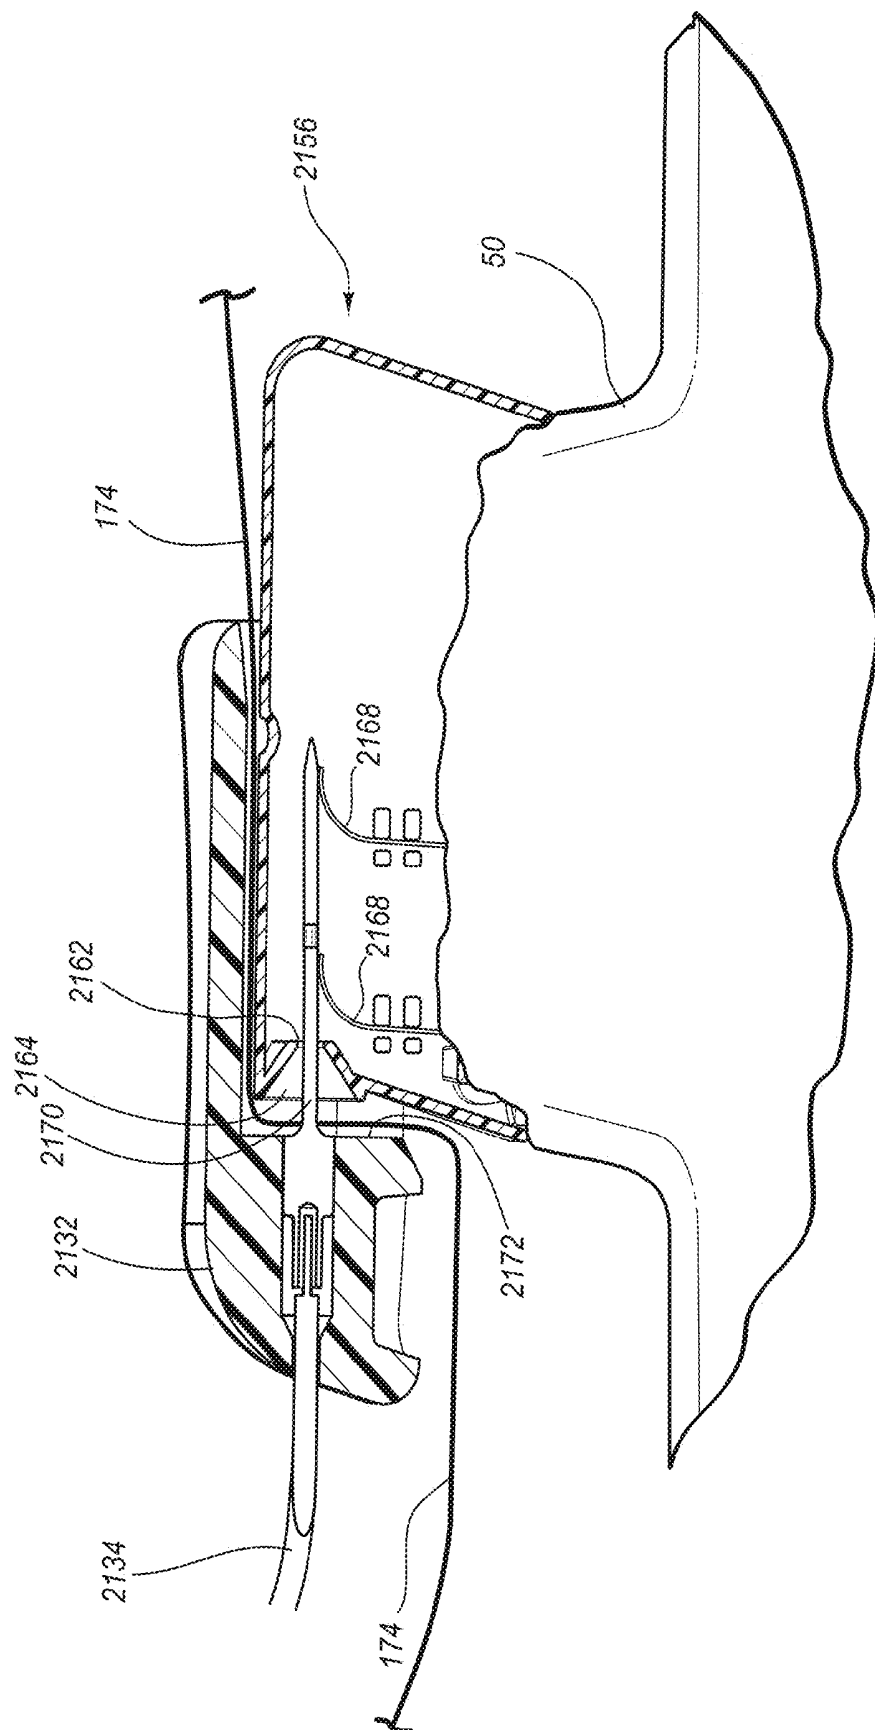


FIG. 44

1

SYSTEM FOR PLACEMENT OF A CATHETER INCLUDING A SIGNAL-GENERATING STYLET

CROSS-REFERENCE TO RELATED APPLICATIONS

This application claims the benefit of U.S. Provisional Patent Application No. 61/156,842, filed Mar. 2, 2009, and entitled "SYSTEM FOR PLACEMENT OF A CATHETER INCLUDING A SIGNAL-GENERATING STYLET." This application is also a continuation-in-part of U.S. application Ser. No. 12/426,175, filed Apr. 17, 2009, and entitled "Systems and Methods for Breaching a Sterile Field for Intravascular Placement of a Catheter," which is a continuation-in-part of U.S. application Ser. No. 12/323,273, filed Nov. 25, 2008, and entitled "Integrated System for Intravascular Placement of a Catheter," which claims the benefit of the following U.S. Provisional Patent Applications: Application No. 61/095,921, filed Sep. 10, 2008, and entitled "System and Method for Placing a Catheter Within a Vasculature of a Patient;" Application No. 61/095,451, filed Sep. 9, 2008, and entitled "Catheter Assembly Including ECG and Magnetic-Based Sensor Stylet;" Application No. 61/091,233, filed Aug. 22, 2008, and entitled "Catheter Including Preloaded Steerable Stylet;" Application No. 61/045,944, filed Apr. 17, 2008, and entitled "Drape-Breaching Electrical Connector;" and Application No. 60/990,242, filed Nov. 26, 2007, and entitled "Integrated Ultrasound and Tip Location System for Intravascular Placement of a Catheter." Each of the afore-referenced applications is incorporated herein by reference in its entirety.

BRIEF SUMMARY

Briefly summarized, embodiments of the present invention are directed to an integrated catheter placement system configured for accurately placing a catheter within the vasculature of a patient. The integrated system employs at least two modalities for improving catheter placement accuracy: 1) ultrasound-assisted guidance for introducing the catheter into the patient's vasculature; and 2) a tip location system ("TLS"), or magnetically-based (e.g., via permanent magnet(s) or electromagnet(s)) tracking of the catheter tip during its advancement through the vasculature to detect and facilitate correction of any tip malposition during such advancement.

In one embodiment, the integrated system comprises a system console including a control processor, a tip location sensor unit for temporary placement on a portion of a body of the patient, and an ultrasound probe. The tip location sensor senses a magnetic field of a stylet disposed in a lumen of the catheter when the catheter is disposed in the vasculature. The ultrasound probe ultrasonically images a portion of the vasculature prior to introduction of the catheter into the vasculature. In addition, the ultrasound probe includes user input controls for controlling use of the ultrasound probe in an ultrasound mode and use of the tip location sensor in a tip location mode.

In another embodiment, a third modality, i.e., ECG signal-based catheter tip guidance, is included in the system to enable guidance of the catheter tip to a desired position with respect to a node of the patient's heart from which the ECG signals originate. Various means for establishing a conductive pathway between a sterile field of the patient and a non-sterile field to enable passage of ECG signals from the catheter to the tip location sensor are also disclosed. Such means include, for example, connector schemes that establish the conductive

2

pathway through a perforation defined in a sterile barrier, such as a surgical drape, wherein the perforation is isolated by the connector scheme so as to prevent contamination or compromise of the sterile field of the patient.

In one embodiment, the tip location sensor stylet includes an electromagnetic coil that can be operably connected to the sensor unit and/or console through a sterile barrier without compromising the barrier and the sterile field it at least partially defines. The stylet can also be wirelessly connected to the sensor unit and/or console.

These and other features of embodiments of the present invention will become more fully apparent from the following description and appended claims, or may be learned by the practice of embodiments of the invention as set forth herein-after.

BRIEF DESCRIPTION OF THE DRAWINGS

A more particular description of the present disclosure will be rendered by reference to specific embodiments thereof that are illustrated in the appended drawings. It is appreciated that these drawings depict only typical embodiments of the invention and are therefore not to be considered limiting of its scope. Example embodiments of the invention will be described and explained with additional specificity and detail through the use of the accompanying drawings in which:

FIG. 1 is a block diagram depicting various elements of an integrated system for intravascular placement of a catheter, according to one example embodiment of the present invention;

FIG. 2 is a simplified view of a patient and a catheter being inserted therein with assistance of the integrated system of FIG. 1;

FIGS. 3A and 3B are views of a probe of the integrated system of FIG. 1;

FIG. 4 is a screenshot of an ultrasound image as depicted on a display of the integrated system of FIG. 1;

FIG. 5 is a perspective view of a stylet employed in connection with the system of FIG. 1 in placing a catheter within a patient vasculature;

FIG. 6 is an icon as depicted on a display of the integrated system of FIG. 1, indicating a position of a distal end of the stylet of FIG. 5 during catheter tip placement procedures;

FIGS. 7A-7E depict various example icons that can be depicted on the display of the integrated system of FIG. 1 during catheter tip placement procedures;

FIGS. 8A-8C are screenshots of images depicted on a display of the integrated system of FIG. 1 during catheter tip placement procedures;

FIG. 9 is a block diagram depicting various elements of an integrated system for intravascular placement of a catheter, according to another example embodiment of the present invention;

FIG. 10 is a simplified view of a patient and a catheter being inserted therein with assistance of the integrated system of FIG. 9;

FIG. 11 is a perspective view of a stylet employed in connection with the integrated system of FIG. 9 in placing a catheter within a patient vasculature;

FIGS. 12A-12E are various views of portions of the stylet of FIG. 11;

FIGS. 13A-13D are various views of a fin connector assembly for use with the integrated system of FIG. 9;

FIGS. 13E-13F are various views of a tether connector for use with the fin connector assembly shown in FIGS. 13A-13D;

FIGS. 14A-14C are views showing the connection of a stylet tether and fin connector to a sensor of the integrated system of FIG. 9;

FIG. 15 is a cross sectional view of the connection of the stylet tether, fin connector, and sensor shown in FIG. 14C;

FIG. 16 is simplified view of an ECG trace of a patient;

FIG. 17 is a screenshot of an image depicted on a display of the integrated system of FIG. 9 during catheter tip placement procedures;

FIG. 18 is a cross sectional view of a fin connector including electrical contacts configured in accordance with one embodiment;

FIGS. 19A and 19B are simplified views of an electrical contact retention system for engagement of a tether connector with a fin connector, in accordance with one embodiment;

FIGS. 20A-20C are various views of one embodiment of a fin connector and a tether connector for establishing a signal pathway through a sterile barrier in connection with use of the integrated system described herein;

FIGS. 21A and 21B are various views of a connector for electrically connecting ECG electrodes to a sensor of the integrated system, according to one embodiment;

FIGS. 22A-22C are various views of one embodiment of a fin connector and a tether connector for establishing a signal pathway through a sterile barrier;

FIGS. 23A and 23B are cross sectional views of a connector system for establishing a signal pathway through a sterile barrier, according to one embodiment;

FIG. 24 is a simplified side view of a connector system for establishing a signal pathway through a sterile barrier, according to one embodiment;

FIGS. 25A and 25B are simplified side views of a connector system for establishing a signal pathway through a sterile barrier, according to one embodiment;

FIGS. 26A and 26B are cross sectional views of a connector system for establishing a signal pathway through a sterile barrier, according to one embodiment;

FIG. 27 is a simplified view of a connector system for establishing a signal pathway through a sterile barrier, according to one embodiment;

FIG. 28 is a perspective view of stylet including a sterile shield for use with the connector system shown in FIG. 28, according to one embodiment;

FIGS. 29A and 29B are simplified views of the ECG module of FIG. 27, including a connector system for establishing a signal pathway through a sterile barrier, according to one embodiment;

FIG. 30 is a simplified view of a connector system for establishing a signal pathway through a sterile barrier, according to one embodiment;

FIG. 31 is a simplified view of a connector system for establishing a signal pathway through a sterile barrier, according to one embodiment;

FIG. 32 is a simplified view of elements of a connector system for establishing a signal pathway through a sterile barrier, according to one embodiment;

FIG. 33 is a view of a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment.

FIG. 34 is a view of another means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment.

FIGS. 35A-C depict exemplary P-wave waveforms.

FIG. 36 is a view of a sensor retro-fitted with a wireless module, according to one embodiment.

FIG. 37 is a view of a retention feature for a connector, according to one embodiment.

FIG. 38 is a simplified view of a patient and a catheter being inserted therein with the assistance of a catheter placement system, according to one embodiment;

FIG. 39 is a perspective view of an untethered stylet configured in accordance with one embodiment;

FIG. 40 is a partial cross sectional view of a distal portion of the stylet of FIG. 3;

FIG. 41 is a simplified block diagram of a module portion of the untethered stylet of FIG. 3, together with associated components of the console of FIG. 38;

FIG. 42 is a simplified diagram showing various components employed in synchronizing a pulse signal frequency between a wireless stylet and a console of the system of FIG. 38;

FIGS. 43A-43B are perspective views of the sensor unit of FIG. 10 and a tethered stylet, showing one possible connective scheme therebetween in accordance with one embodiment; and

FIG. 44 is a partial cross sectional view of the connective scheme of the sensor unit and tethered stylet, according to one embodiment.

DETAILED DESCRIPTION OF SELECTED EMBODIMENTS

Reference will now be made to figures wherein like structures will be provided with like reference designations. It is understood that the drawings are diagrammatic and schematic representations of exemplary embodiments of the present invention, and are neither limiting nor necessarily drawn to scale.

FIGS. 1-44 depict various features of embodiments of the present invention, which is generally directed to a catheter placement system configured for accurately placing a catheter within the vasculature of a patient. In one embodiment, the catheter placement system employs at least two modalities for improving catheter placement accuracy: 1) ultrasound-assisted guidance for introducing the catheter into the patient's vasculature; and 2) a tip location/navigation system ("TLS"), or magnetically-based tracking of the catheter tip during its advancement through the tortuous vasculature path to detect and facilitate correction of any tip malposition during such advancement. The ultrasound guidance and tip location features of the present system according to one embodiment are integrated into a single device for use by a clinician placing the catheter. Integration of these two modalities into a single device simplifies the catheter placement process and results in relatively faster catheter placements. For instance, the integrated catheter placement system enables ultrasound and TLS activities to be viewed from a single display of the integrated system. Also, controls located on an ultrasound probe of the integrated device, which probe is maintained within the sterile field of the patient during catheter placement, can be used to control functionality of the system, thus precluding the need for a clinician to reach out of the sterile field in order to control the system.

In another embodiment, a third modality, i.e., ECG signal-based catheter tip guidance, is included in the integrated system to enable guidance of the catheter tip to a desired position with respect to a node of the patient's heart from which the ECG signals originate. Such ECG-based positional assistance is also referred to herein as "tip confirmation."

Combination of the three modalities above according to one embodiment enables the catheter placement system to facilitate catheter placement within the patient's vasculature with a relatively high level of accuracy, i.e., placement of the distal tip of the catheter in a predetermined and desired posi-

tion. Moreover, because of the ECG-based guidance of the catheter tip, correct tip placement may be confirmed without the need for a confirmatory X-ray. This, in turn, reduces the patient's exposure to potentially harmful x-rays, the cost and time involved in transporting the patient to and from the x-ray department, costly and inconvenient catheter repositioning procedures, etc.

As the ECG signal-based modality includes a need for passing ECG signals from a catheter assembly disposed in a sterile field of a patient to a data-receiving component of the system disposed in a non-sterile field, embodiments of the present invention are further concerned with various connector systems for establishing a conductive pathway through a sterile barrier separating the sterile and non-sterile fields.

For clarity it is to be understood that the word "proximal" as used herein refers to a direction relatively closer to a clinician, while the word "distal" refers to a direction relatively further from the clinician. For example, the end of a catheter placed within the body of a patient is considered a distal end of the catheter, while the catheter end remaining outside the body is a proximal end of the catheter. Also, the words "including," "has," and "having," as used herein, including the claims, shall have the same meaning as the word "comprising."

Reference is first made to FIGS. 1 and 2 which depict various components of a catheter placement system ("system"), generally designated at 10, configured in accordance with one example embodiment of the present invention. As shown, the system 10 generally includes a console 20, display 30, probe 40, and sensor 50, each of which is described in further detail below.

FIG. 2 shows the general relation of these components to a patient 70 during a procedure to place a catheter 72 into the patient vasculature through a skin insertion site 73. FIG. 2 shows that the catheter 72 generally includes a proximal portion 74 that remains exterior to the patient and a distal portion 76 that resides within the patient vasculature after placement is complete. The system 10 is employed to ultimately position a distal tip 76A of the catheter 72 in a desired position within the patient vasculature. In one embodiment, the desired position for the catheter distal tip 76A is proximate the patient's heart, such as in the lower one-third ($\frac{1}{3}^{rd}$) portion of the Superior Vena Cava ("SVC"). Of course, the system 10 can be employed to place the catheter distal tip in other locations. The catheter proximal portion 74 further includes a hub 74A that provides fluid communication between the one or more lumens of the catheter 72 and one or more extension legs 74B extending proximally from the hub.

An example implementation of the console 20 is shown in FIG. 8C, though it is appreciated that the console can take one of a variety of forms. A processor 22, including non-volatile memory such as EEPROM for instance, is included in the console 20 for controlling system function during operation of the system 10, thus acting as a control processor. A digital controller/analog interface 24 is also included with the console 20 and is in communication with both the processor 22 and other system components to govern interfacing between the probe 40, sensor 50, and other system components.

The system 10 further includes ports 52 for connection with the sensor 50 and optional components 54 including a printer, storage media, keyboard, etc. The ports in one embodiment are USB ports, though other port types or a combination of port types can be used for this and the other interfaces connections described herein. A power connection 56 is included with the console 20 to enable operable connection to an external power supply 58. An internal battery 60 can also be employed, either with or exclusive of an external

power supply. Power management circuitry 59 is included with the digital controller/analog interface 24 of the console to regulate power use and distribution.

The display 30 in the present embodiment is integrated into the console 20 and is used to display information to the clinician during the catheter placement procedure. In another embodiment, the display may be separate from the console. As will be seen, the content depicted by the display 30 changes according to which mode the catheter placement system is in: US, TLS, or in other embodiments, ECG tip confirmation. In one embodiment, a console button interface 32 (see FIGS. 1, 8C) and buttons included on the probe 40 can be used to immediately call up a desired mode to the display 30 by the clinician to assist in the placement procedure. In one embodiment, information from multiple modes, such as TLS and ECG, may be displayed simultaneously, such as in FIG. 17. Thus, the single display 30 of the system console 20 can be employed for ultrasound guidance in accessing a patient's vasculature, TLS guidance during catheter advancement through the vasculature, and (as in later embodiments) ECG-based confirmation of catheter distal tip placement with respect to a node of the patient's heart. In one embodiment, the display 30 is an LCD device.

FIGS. 3A and 3B depict features of the probe 40 according to one embodiment. The probe 40 is employed in connection with the first modality mentioned above, i.e., ultrasound ("US")-based visualization of a vessel, such as a vein, in preparation for insertion of the catheter 72 into the vasculature. Such visualization gives real time ultrasound guidance for introducing the catheter into the vasculature of the patient and assists in reducing complications typically associated with such introduction, including inadvertent arterial puncture, hematoma, pneumothorax, etc.

The handheld probe 40 includes a head 80 that houses a piezoelectric array for producing ultrasonic pulses and for receiving echoes thereof after reflection by the patient's body when the head is placed against the patient's skin proximate the prospective insertion site 73 (FIG. 2). The probe 40 further includes a plurality of control buttons 84, which can be included on a button pad 82. In the present embodiment, the modality of the system 10 can be controlled by the control buttons 84, thus eliminating the need for the clinician to reach out of the sterile field, which is established about the patient insertion site prior to catheter placement, to change modes via use of the console button interface 32.

As such, in one embodiment a clinician employs the first (US) modality to determine a suitable insertion site and establish vascular access, such as with a needle or introducer, then with the catheter. The clinician can then seamlessly switch, via button pushes on the probe button pad 82, to the second (TLS) modality without having to reach out of the sterile field. The TLS mode can then be used to assist in advancement of the catheter 72 through the vasculature toward an intended destination.

FIG. 1 shows that the probe 40 further includes button and memory controller 42 for governing button and probe operation. The button and memory controller 42 can include non-volatile memory, such as EEPROM, in one embodiment. The button and memory controller 42 is in operable communication with a probe interface 44 of the console 20, which includes a piezo input/output component 44A for interfacing with the probe piezoelectric array and a button and memory input/output component 44B for interfacing with the button and memory controller 42.

FIG. 4 shows an example screenshot 88 as depicted on the display 30 while the system 10 is in its first ultrasound modality. An image 90 of a subcutaneous region of the patient 70 is

shown, depicting a cross section of a vein **92**. The image **90** is produced by operation of the piezoelectric array of the probe **40**. also included on the display screenshot **88** is a depth scale indicator **94**, providing information regarding the depth of the image **90** below the patient's skin, a lumen size scale **96** that provides information as to the size of the vein **92** relative to standard catheter lumen sizes, and other indicia **98** that provide information regarding status of the system **10** or possible actions to be taken, e.g., freeze frame, image templates, data save, image print, power status, image brightness, etc.

Note that while a vein is depicted in the image **90**, other body lumens or portions can be imaged in other embodiments. Note that the US mode shown in FIG. **4** can be simultaneously depicted on the display **30** with other modes, such as the TLS mode, if desired. In addition to the visual display **30**, aural information, such as beeps, tones, etc., can also be employed by the system **10** to assist the clinician during catheter placement. Moreover, the buttons included on the probe **40** and the console button interface **32** can be configured in a variety of ways, including the use of user input controls in addition to buttons, such as slide switches, toggle switches, electronic or touch-sensitive pads, etc. Additionally, both US and TLS activities can occur simultaneously or exclusively during use of the system **10**.

As just described, the handheld ultrasound probe **40** is employed as part of the integrated catheter placement system **10** to enable US visualization of the peripheral vasculature of a patient in preparation for transcutaneous introduction of the catheter. In the present example embodiment, however, the probe is also employed to control functionality of the TLS portion, or second modality, of the system **10** when navigating the catheter toward its desired destination within the vasculature as described below. Again, as the probe **40** is used within the sterile field of the patient, this feature enables TLS functionality to be controlled entirely from within the sterile field. Thus the probe **40** is a dual-purpose device, enabling convenient control of both US and TLS functionality of the system **10** from the sterile field. In one embodiment, the probe can also be employed to control some or all ECG-related functionality, or third modality, of the catheter placement system **10**, as described further below.

The catheter placement system **10** further includes the second modality mentioned above, i.e., the magnetically-based catheter TLS, or tip location system. The TLS enables the clinician to quickly locate and confirm the position and/or orientation of the catheter **72**, such as a peripherally-inserted central catheter ("PICC"), central venous catheter ("CVC"), or other suitable catheter, during initial placement into and advancement through the vasculature of the patient **70**. Specifically, the TLS modality detects a magnetic field generated by a magnetic element-equipped tip location stylet, which is pre-loaded in one embodiment into a longitudinally defined lumen of the catheter **72**, thus enabling the clinician to ascertain the general location and orientation of the catheter tip within the patient body. In one embodiment, the magnetic assembly can be tracked using the teachings of one or more of the following U.S. Pat. Nos. 5,775,322; 5,879,297; 6,129,668; 6,216,028; and 6,263,230. The contents of the aforementioned U.S. patents are incorporated herein by reference in their entireties. The TLS also displays the direction in which the catheter tip is pointing, thus further assisting accurate catheter placement. The TLS further assists the clinician in determining when a malposition of the catheter tip has occurred, such as in the case where the tip has deviated from a desired venous path into another vein.

As mentioned, the TLS utilizes a stylet to enable the distal end of the catheter **72** to be tracked during its advancement

through the vasculature. FIG. **5** gives an example of such a stylet **100**, which includes a proximal end **100A** and a distal end **100B**. A handle is included at the stylet proximal end **100A**, with a core wire **104** extending distally therefrom. A magnetic assembly is disposed distally of the core wire **104**. The magnetic assembly includes one or more magnetic elements **106** disposed adjacent one another proximate the stylet distal end **100B** and encapsulated by tubing **108**. In the present embodiment, a plurality of magnetic elements **106** is included, each element including a solid, cylindrically shaped ferromagnetic stacked end-to-end with the other magnetic elements. An adhesive tip **110** can fill the distal tip of the tubing **108**, distally to the magnetic elements **106**.

Note that in other embodiments, the magnetic elements may vary from the design in not only shape, but also composition, number, size, magnetic type, and position in the stylet distal segment. For example, in one embodiment, the plurality of ferromagnetic magnetic elements is replaced with an electromagnetic assembly, such as an electromagnetic coil, which produces a magnetic field for detection by the sensor. Another example of an assembly usable here can be found in U.S. Pat. No. 5,099,845 entitled "Medical Instrument Location Means," which is incorporated herein by reference in its entirety. Yet other examples of stylets including magnetic elements that can be employed with the TLS modality can be found in U.S. application Ser. No. 11/466,602, filed Aug. 23, 2006, and entitled "Stylet Apparatuses and Methods of Manufacture," which is incorporated herein by reference in its entirety. These and other variations are therefore contemplated by embodiments of the present invention. It should be appreciated herein that "stylet" as used herein can include any one of a variety of devices configured for removable placement within a lumen of the catheter to assist in placing a distal end of the catheter in a desired location within the patient's vasculature.

FIG. **2** shows disposal of the stylet **100** substantially within a lumen in the catheter **72** such that the proximal portion thereof extends proximally from the catheter lumen, through the hub **74A** and out through a selected one of the extension legs **74B**. So disposed within a lumen of the catheter, the distal end **100B** of the stylet **100** is substantially co-terminal with the distal catheter end **76A** such that detection by the TLS of the stylet distal end correspondingly indicates the location of the catheter distal end.

The TLS sensor **50** is employed by the system **10** during TLS operation to detect a magnetic field produced by the magnetic elements **106** of the stylet **100**. As seen in FIG. **2**, the TLS sensor **50** is placed on the chest of the patient during catheter insertion. The TLS sensor **50** is placed on the chest of the patient in a predetermined location, such as through the use of external body landmarks, to enable the magnetic field of the stylet magnetic elements **106**, disposed in the catheter **72** as described above, to be detected during catheter transit through the patient vasculature. Again, as the magnetic elements **106** of the stylet magnetic assembly are co-terminal with the distal end **76A** of the catheter **72** (FIG. **2**), detection by the TLS sensor **50** of the magnetic field of the magnetic elements provides information to the clinician as to the position and orientation of the catheter distal end during its transit.

In greater detail, the TLS sensor **50** is operably connected to the console **20** of the system **10** via one or more of the ports **52**, as shown in FIG. **1**. Note that other connection schemes between the TLS sensor and the system console can also be used without limitation. As just described, the magnetic elements **106** are employed in the stylet **100** to enable the position of the catheter distal end **76A** (FIG. **2**) to be observable relative to the TLS sensor **50** placed on the patient's chest.

Detection by the TLS sensor **50** of the stylet magnetic elements **106** is graphically displayed on the display **30** of the console **20** during TLS mode. In this way, a clinician placing the catheter is able to generally determine the location of the catheter distal end **76A** within the patient vasculature relative to the TLS sensor **50** and detect when catheter malposition, such as advancement of the catheter along an undesired vein, is occurring.

FIGS. **6** and **7A-7E** show examples of icons that can be used by the console display **30** to depict detection of the stylet magnetic elements **106** by the TLS sensor **50**. In particular, FIG. **6** shows an icon **114** that depicts the distal portion of the stylet **100**, including the magnetic elements **106** as detected by the TLS sensor **50** when the magnetic elements are positioned under the TLS sensor. As the stylet distal end **100B** is substantially co-terminal with the distal end **76A** of the catheter **72**, the icon indicates the position and orientation of the catheter distal end. FIGS. **7A-7E** show various icons that can be depicted on the console display **30** when the magnetic elements **106** of the stylet **100** are not positioned directly under a portion of the TLS sensor **50**, but are nonetheless detected nearby. The icons can include half-icons **114A** and quarter-icons **114B** that are displayed according to the position of the stylet magnetic assembly, i.e., the magnetic elements **106** in the present embodiment, relative to the TLS sensor **50**.

FIGS. **8A-8C** depict screenshots taken from the display **30** of the system **10** while in TLS mode, showing how the magnetic assembly of the stylet **100** is depicted. The screenshot **118** of FIG. **8A** shows a representative image **120** of the TLS sensor **50**. Other information is provided on the display screenshot **118**, including a depth scale indicator **124**, status/action indicia **126**, and icons **128** corresponding to the button interface **32** included on the console **20** (FIG. **8C**). Though the icons **128** in the present embodiment are simply indicators to guide the user in identifying the purpose of the corresponding buttons of the button interface **32**, in another embodiment the display can be made touch-sensitive so that the icons themselves can function as button interfaces and can change according to the mode the system is in.

During initial stages of catheter advancement through the patient's vasculature after insertion therein, the distal end **76A** of the catheter **72**, having the stylet distal end **100B** substantially co-terminal therewith, is relatively distant from the TLS sensor **50**. As such, the display screenshot will indicate "no signal," indicating that the magnetic field from the stylet magnetic assembly has not been detected. In FIG. **8B**, the magnetic assembly proximate the stylet distal end **100B** has advanced sufficiently close to the TLS sensor **50** to be detected thereby, though it is not yet under the sensor. This is indicated by the half-icon **114A** shown to the left of the sensor image **120**, representing the stylet magnetic assembly being positioned to the right of the TLS sensor **50** from the perspective of the patient.

In FIG. **8C**, the magnetic assembly proximate the stylet distal end **100B** has advanced under the TLS sensor **50** such that its position and orientation relative thereto is detected by the TLS sensor. This is indicated by the icon **114** on the sensor image **120**. Note that the button icons **128** provide indications of the actions that can be performed by pressing the corresponding buttons of the console button interface **32**. As such, the button icons **128** can change according to which modality the system **10** is in, thus providing flexibility of use for the button interface **32**. Note further that, as the button pad **82** of the probe **40** (FIG. **3A**, **3B**) includes buttons **84** that mimic several of the buttons of the button interface **32**, the button icons **128** on the display **30** provide a guide to the clinician for

controlling the system **10** with the probe buttons **84** while remaining in the sterile field. For instance, if the clinician has need to leave TLS mode and return to US (ultrasound) mode, the appropriate control button **84** on the probe button pad **82** can be depressed, and the US mode can be immediately called up, with the display **30** refreshing to accommodate the visual information needed for US functionality, such as that shown in FIG. **4**. This is accomplished without a need for the clinician to reach out of the sterile field.

Reference is now made to FIGS. **9** and **10** in describing the integrated catheter placement system **10** according to another example embodiment. As before, the integrated system **10** includes the console **20**, display **30**, probe **40** for US functionality, and the TLS sensor **50** for tip location functionality as described above. Note that the system **10** depicted in FIGS. **9** and **10** is similar in many respects to the system shown in FIGS. **1** and **2**. As such, only selected differences will be discussed below. The system **10** of FIGS. **9** and **10** includes additional functionality wherein determination of the proximity of the catheter distal tip **76A** relative to a sin θ -atrial ("SA") or other electrical impulse-emitting node of the heart of the patient **70** can be determined, thus providing enhanced ability to accurately place the catheter distal tip in a desired location proximate the node. Also referred to herein as "ECG" or "ECG-based tip confirmation," this third modality of the system **10** enables detection of ECG signals from the SA node in order to place the catheter distal tip in a desired location within the patient vasculature. Note that the US, TLS, and ECG modalities are seamlessly combined in the present system **10**, but can be employed in concert or individually to assist in catheter placement. In one embodiment, it is understood that the ECG modality as described herein can be included in a stand-alone system without the inclusion of the US and TLS modalities. Thus, the environments in which the embodiments herein are described are understood as merely example environments and are not considered limiting of the present disclosure.

FIGS. **9** and **10** show the addition to the system **10** of a stylet **130** configured in accordance with the present embodiment. As an overview, the catheter stylet **130** is removably predisposed within the lumen of the catheter **72** being inserted into the patient **70** via the insertion site **73**. The stylet **130**, in addition to including a magnetic assembly for the magnetically-based TLS modality, includes a sensing component, i.e., an ECG sensor assembly, proximate its distal end and including a portion that is co-terminal with the distal end of the catheter tip for sensing ECG signals produced by the SA node. In contrast to the previous embodiment, the stylet **130** includes a tether **134** extending from its proximal end that operably connects to the TLS sensor **50**. As will be described in further detail, the stylet tether **134** permits ECG signals detected by the ECG sensor assembly included on a distal portion of the stylet **130** to be conveyed to the TLS sensor **50** during confirmation of the catheter tip location as part of the ECG signal-based tip confirmation modality. Reference and ground ECG lead/electrode pairs **158** attach to the body of the body of the patient **70** and are operably attached to the TLS sensor **50** to enable the system to filter out high level electrical activity unrelated to the electrical activity of the SA node of the heart, thus enabling the ECG-based tip confirmation functionality. Together with the reference and ground signals received from the ECG lead/electrode pairs **158** placed on the patient's skin, the ECG signals sensed by the stylet ECG sensor assembly are received by the TLS sensor **50** positioned on the patient's chest (FIG. **10**) or other designated component of the system **10**. The TLS sensor **50** and/or console processor **22** can process the ECG signal data to produce an

electrocardiogram waveform on the display 30, as will be described. In the case where the TLS sensor 50 processes the ECG signal data, a processor is included therein to perform the intended functionality. If the console 20 processes the ECG signal data, the processor 22, controller 24, or other processor can be utilized in the console to process the data.

Thus, as it is advanced through the patient vasculature, the catheter 72 equipped with the stylet 130 as described above can advance under the TLS sensor 50, which is positioned on the chest of the patient as shown in FIG. 10. This enables the TLS sensor 50 to detect the position of the magnetic assembly of the stylet 130, which is substantially co-terminal with the distal tip 76A of the catheter as located within the patient's vasculature. The detection by the TLS sensor 50 of the stylet magnetic assembly is depicted on the display 30 during ECG mode. The display 30 further depicts during ECG mode an ECG electrocardiogram waveform produced as a result of patient heart's electrical activity as detected by the ECG sensor assembly of the stylet 130. In greater detail, the ECG electrical activity of the SA node, including the P-wave of the waveform, is detected by the ECG sensor assembly of the stylet (described below) and forwarded to the TLS sensor 50 and console 20. The ECG electrical activity is then processed for depiction on the display 30. A clinician placing the catheter can then observe the ECG data to determine optimum placement of the distal tip 76A of the catheter 72, such as proximate the SA node in one embodiment. In one embodiment, the console 20 includes the electronic components, such as the processor 22 (FIG. 9), necessary to receive and process the signals detected by the stylet ECG sensor assembly. In another embodiment, the TLS sensor 50 can include the necessary electronic components processing the ECG signals.

As already discussed, the display 30 is used to display information to the clinician during the catheter placement procedure. The content of the display 30 changes according to which mode the catheter placement system is in: US, TLS, or ECG. Any of the three modes can be immediately called up to the display 30 by the clinician, and in some cases information from multiple modes, such as TLS and ECG, may be displayed simultaneously. In one embodiment, as before, the mode the system is in may be controlled by the control buttons 84 included on the handheld probe 40, thus eliminating the need for the clinician to reach out of the sterile field (such as touching the button interface 32 of the console 20) to change modes. Thus, in the present embodiment the probe 40 is employed to also control some or all ECG-related functionality of the system 10. Note that the button interface 32 or other input configurations can also be used to control system functionality. Also, in addition to the visual display 30, aural information, such as beeps, tones, etc., can also be employed by the system to assist the clinician during catheter placement.

Reference is now made to FIGS. 11-12E in describing various details of one embodiment of the stylet 130 that is removably loaded into the catheter 72 and employed during insertion to position the distal tip 76A of the catheter in a desired location within the patient vasculature. As shown, the stylet 130 as removed from the catheter defines a proximal end 130A and a distal end 130B. A connector 132 is included at the proximal stylet end 130A, and a tether 134 extends distally from the connector and attaches to a handle 136. A core wire 138 extends distally from the handle 136. The stylet 130 is pre-loaded within a lumen of the catheter 72 in one embodiment such that the distal end 130B is substantially flush, or co-terminal, with the catheter opening at the distal end 76A thereof (FIG. 10), and such that a proximal portion of

the core wire 138, the handle 136, and the tether 134 extend proximally from a selected one of the extension tubes 74B. Note that, though described herein as a stylet, in other embodiments a guidewire or other catheter guiding apparatus could include the principles of the embodiment described herein.

The core wire 138 defines an elongate shape and is composed of a suitable stylet material including stainless steel or a memory material such as, in one embodiment, a nickel and titanium-containing alloy commonly known by the acronym "nitinol." Though not shown here, manufacture of the core wire 138 from nitinol in one embodiment enables the portion of the core wire corresponding to a distal segment of the stylet to have a pre-shaped bent configuration so as to urge the distal portion of the catheter 72 into a similar bent configuration. In other embodiments, the core wire includes no pre-shaping. Further, the nitinol construction lends torqueability to the core wire 138 to enable a distal segment of the stylet 130 to be manipulated while disposed within the lumen of the catheter 72, which in turn enables the distal portion of the catheter to be navigated through the vasculature during catheter insertion.

The handle 136 is provided to enable insertion/removal of the stylet from the catheter 72. In embodiments where the stylet core wire 138 is torqueable, the handle 136 further enables the core wire to be rotated within the lumen of the catheter 72, to assist in navigating the catheter distal portion through the vasculature of the patient 70.

The handle 136 attaches to a distal end of the tether 134. In the present embodiment, the tether 134 is a flexible, shielded cable housing one or more conductive wires electrically connected both to the core wire 138, which acts as the ECG sensor assembly referred to above, and the tether connector 132. As such, the tether 134 provides a conductive pathway from the distal portion of the core wire 138 through to the tether connector 132 at proximal end 130A of the stylet 130. As will be explained, the tether connector 132 is configured for operable connection to the TLS sensor 50 on the patient's chest for assisting in navigation of the catheter distal tip 76A to a desired location within the patient vasculature.

As seen in FIGS. 12B-12D, a distal portion of the core wire 138 is gradually tapered, or reduced in diameter, distally from a junction point 142. A sleeve 140 is slid over the reduced-diameter core wire portion. Though of relatively greater diameter here, the sleeve in another embodiment can be sized to substantially match the diameter of the proximal portion of the stylet core wire. The stylet 130 further includes a magnetic assembly disposed proximate the distal end 130B thereof for use during TLS mode. The magnetic assembly in the illustrated embodiment includes a plurality of magnetic elements 144 interposed between an outer surface of the reduced-diameter core wire 138 and an inner surface of the sleeve 140 proximate the stylet distal end 130B. In the present embodiment, the magnetic elements 144 include 20 ferromagnetic magnets of a solid cylindrical shape stacked end-to-end in a manner similar to the stylet 100 of FIG. 2. In other embodiments, however, the magnetic element(s) may vary from this design in not only shape, but also composition, number, size, magnetic type, and position in the stylet. For example, in one embodiment the plurality of magnets of the magnetic assembly is replaced with an electromagnetic coil that produces a magnetic field for detection by the TLS sensor. These and other variations are therefore contemplated by embodiments of the present invention.

The magnetic elements 144 are employed in the stylet 130 distal portion to enable the position of the stylet distal end 130B to be observable relative to the TLS sensor 50 placed on

the patient's chest. As has been mentioned, the TLS sensor **50** is configured to detect the magnetic field of the magnetic elements **144** as the stylet advances with the catheter **72** through the patient vasculature. In this way, a clinician placing the catheter **72** is able to generally determine the location of the catheter distal end **76A** within the patient vasculature and detect when catheter malposition is occurring, such as advancement of the catheter along an undesired vein, for instance.

The stylet **130** further includes the afore-mentioned ECG sensor assembly, according to one embodiment. The ECG sensor assembly enables the stylet **130**, disposed in a lumen of the catheter **72** during insertion, to be employed in detecting an intra-atrial ECG signal produced by an SA or other node of the patient's heart, thereby allowing for navigation of the distal tip **76A** of the catheter **72** to a predetermined location within the vasculature proximate the patient's heart. Thus, the ECG sensor assembly serves as an aide in confirming proper placement of the catheter distal tip **76A**.

In the embodiment illustrated in FIGS. **11-12E**, the ECG sensor assembly includes a distal portion of the core wire **138** disposed proximate the stylet distal end **130B**. The core wire **138**, being electrically conductive, enables ECG signals to be detected by the distal end thereof and transmitted proximally along the core wire. A conductive material **146**, such as a conductive epoxy, fills a distal portion of the sleeve **140** adjacent the distal termination of the core wire **138** so as to be in conductive communication with the distal end of the core wire. This in turn increases the conductive surface of the distal end **130B** of the stylet **130** so as to improve its ability to detect ECG signals.

Before catheter placement, the stylet **130** is loaded into a lumen of the catheter **72**. Note that the stylet **130** can come preloaded in the catheter lumen from the manufacturer, or loaded into the catheter by the clinician prior to catheter insertion. The stylet **130** is disposed within the catheter lumen such that the distal end **130B** of the stylet **130** is substantially co-terminal with the distal tip **76A** of the catheter **72**, thus placing the distal tips of both the stylet and the catheter in substantial alignment with one another. The co-terminality of the catheter **72** and stylet **130** enables the magnetic assembly to function with the TLS sensor **50** in TLS mode to track the position of the catheter distal tip **76A** as it advances within the patient vasculature, as has been described. Note, however, that for the tip confirmation functionality of the system **10**, the distal end **130B** of the stylet **130** need not be co-terminal with the catheter distal end **76A**. Rather, all that is required is that a conductive path between the vasculature and the ECG sensor assembly, in this case the core wire **138**, be established such that electrical impulses of the SA node or other node of the patient's heart can be detected. This conductive path in one embodiment can include various components including saline solution, blood, etc.

In one embodiment, once the catheter **72** has been introduced into the patient vasculature via the insertion site **73** (FIG. **10**) the TLS mode of the system **10** can be employed as already described to advance the catheter distal tip **76A** toward its intended destination proximate the SA node. Upon approaching the region of the heart, the system **10** can be switched to ECG mode to enable ECG signals emitted by the SA node to be detected. As the stylet-loaded catheter is advanced toward the patient's heart, the electrically conductive ECG sensor assembly, including the distal end of the core wire **138** and the conductive material **146**, begins to detect the electrical impulses produced by the SA node. As such, the ECG sensor assembly serves as an electrode for detecting the ECG signals. The elongate core wire **138** proximal to the core

wire distal end serves as a conductive pathway to convey the electrical impulses produced by the SA node and received by the ECG sensor assembly to the tether **134**.

The tether **134** conveys the ECG signals to the TLS sensor **50** temporarily placed on the patient's chest. The tether **134** is operably connected to the TLS sensor **50** via the tether connector **132** or other suitable direct or indirect connective configuration. As described, the ECG signal can then be processed and depicted on the system display **30** (FIG. **9, 10**). Monitoring of the ECG signal received by the TLS sensor **50** and displayed by the display **30** enables a clinician to observe and analyze changes in the signal as the catheter distal tip **76A** advances toward the SA node. When the received ECG signal matches a desired profile, the clinician can determine that the catheter distal tip **76A** has reached a desired position with respect to the SA node. As mentioned, in one embodiment this desired position lies within the lower one-third ($\frac{1}{3}_{rd}$) portion of the SVC.

The ECG sensor assembly and magnetic assembly can work in concert in assisting a clinician in placing a catheter within the vasculature. Generally, the magnetic assembly of the stylet **130** assists the clinician in generally navigating the vasculature from initial catheter insertion so as to place the distal end **76A** of the catheter **72** in the general region of the patient's heart. The ECG sensor assembly can then be employed to guide the catheter distal end **76A** to the desired location within the SVC by enabling the clinician to observe changes in the ECG signals produced by the heart as the stylet ECG sensor assembly approaches the SA node. Again, once a suitable ECG signal profile is observed, the clinician can determine that the distal ends of both the stylet **130** and the catheter **72** have arrived at the desired location with respect to the patient's heart. Once it has been positioned as desired, the catheter **72** may be secured in place and the stylet **130** removed from the catheter lumen. It is noted here that the stylet may include one of a variety of configurations in addition to what is explicitly described herein. In one embodiment, the stylet can attach directly to the console instead of an indirect attachment via the TLS sensor. In another embodiment, the structure of the stylet **130** that enables its TLS and ECG-related functionalities can be integrated into the catheter structure itself. For instance, the magnetic assembly and/or ECG sensor assembly can, in one embodiment, be incorporated into the wall of the catheter.

FIGS. **13A-15** describe various details relating to the passage of ECG signal data from the stylet tether **134** to the TLS sensor **50** positioned on the patient's chest, according to the present embodiment. In particular, this embodiment is concerned with passage of ECG signal data from a sterile field surrounding the catheter **72** and insertion site **73**, which includes the stylet **130** and tether **134**, and a non-sterile field, such as the patient's chest on which the TLS sensor is positioned. Such passage should not disrupt the sterile field so that the sterility thereof is compromised. A sterile drape that is positioned over the patient **70** during the catheter insertion procedure defines the majority of the sterile field: areas above the drape are sterile, while areas below (excluding the insertion site and immediately surrounding region) are non-sterile. As will be seen, the discussion below includes at least a first communication node associated with the stylet **130**, and a second communication node associated with the TLS sensor **50** that operably connect with one another to enable ECG signal data transfer therebetween.

One embodiment addressing the passage of ECG signal data from the sterile field to the non-sterile field without compromising the sterility of the former is depicted in FIGS. **13A-15**, which depict a "through-drape" implementation also

15

referred to as a “shark fin” implementation. In particular, FIG. 14A shows the TLS sensor 50 as described above for placement on the chest of the patient during a catheter insertion procedure. The TLS sensor 50 includes on a top surface thereof a connector base 152 defining a channel 152A in which are disposed three electrical base contacts 154. A fin connector 156, also shown in FIGS. 13A-13D, is sized to be slidably received by the channel 152A of the connector base 152, as shown in FIGS. 14B and 15. Two ECG lead/electrode pairs 158 extend from the fin connector 156 for placement on the shoulder and torso or other suitable external locations on the patient body. The drape-piercing tether connector 132 is configured to slidably mate with a portion of the fin connector 156, as will be described further below, to complete a conductive pathway from the stylet 120, through the sterile field to the TLS sensor 50.

FIGS. 13A-13D show further aspects of the fin connector 156. In particular, the fin connector 156 defines a lower barrel portion 160 that is sized to be received in the channel 152A of the connector base 152 (FIGS. 14B, 15). A hole 162 surrounded by a centering cone 164 is included on a back end of an upper barrel portion 166. The upper barrel portion 166 is sized to receive the tether connector 132 of the stylet 130 (FIGS. 14C, 15) such that a pin contact 170 extending into a channel 172 of the tether connector 132 (FIG. 15) is guided by the centering hole until it seats within the hole 162 of the fin connector 156, thus interconnecting the tether connector with the fin connector. An engagement feature, such as the engagement feature 169 shown in FIGS. 13C and 13D, can be included on either side of the fin connector 156 to engage with corresponding detents 173 (FIG. 13F) on the tether connector 132 to assist with maintaining a mating between the two components. If disengagement between the two components is desired, a sufficient reverse pull force is applied to the tether connector 132 while holding or securing the fin connector 156 to prevent its removal from the channel 152A of the connector base 152.

FIG. 13D shows that the fin connector 156 includes a plurality of electrical contacts 168. In the present embodiment, three contacts 168 are included: the two forward-most contact each electrically connecting with a terminal end of one of the ECG leads 158, and the rear contact extending into axial proximity of the hole 162 so as to electrically connect with the pin contact 170 of the tether connector 132 when the latter is mated with the fin connector 156 (FIG. 15). A bottom portion of each contact 168 of the fin connector 156 is positioned to electrically connect with a corresponding one of the base contacts 154 of the TLS sensor connector base 152. In one embodiment, the bottom portion of each contact 168 includes a retention feature, such as an indentation 168A. So configured, each contact 168 can resiliently engage a respective one of the base contacts 154 when the fin connector 156 is received by the TLS sensor connector base 152 such that a tip of each base contact is received in the respective indentation 168A. This configuration provides an additional securement (FIG. 15) to assist in preventing premature separation of the fin connector 156 from the connector base 152. Note that many different retention features between the base contacts 154 and the fin contacts 168 can be included in addition to what is shown and described herein.

FIGS. 13E and 13F depict various details of the tether connector 132 according to one embodiment, including the tether connector channel 172, the pin contact 170 disposed in the channel, and detents 173 for removably engaging the engagement features 169 of the fin connector 156 (FIGS. 13A-13D), as described above. FIG. 13E further shows a

16

plurality of gripping features 171 as an example of structure that can be included to assist the clinician in grasping the tether connector 132.

FIG. 14B shows a first connection stage for interconnecting the above described components, wherein the fin connector 156 is removably mated with the TLS sensor connector base 152 by the sliding engagement of the lower barrel portion 160 of the fin connector with the connector base channel 152A. This engagement electrically connects the connector base contacts 154 with the corresponding fin contacts 168 (FIG. 15).

FIG. 14C shows a second connection stage, wherein the tether connector 132 is removably mated with the fin connector 156 by the sliding engagement of the tether connector channel 172 with the upper barrel portion 166 of the fin connector. This engagement electrically connects the tether connector pin contact 170 with the back contact 168 of the fin connector 156, as best seen in FIG. 15. In the present embodiment, the horizontal sliding movement of the tether connector 132 with respect to the fin connector 156 is in the same engagement direction as when the fin connector is slidably mated to the sensor connector base channel 152A (FIG. 14B). In one embodiment, one or both of the stylet 130/tether connector 132 and the fin connector 156 are disposable. Also, the tether connector in one embodiment can be mated to the fin connector after the fin connector has been mated to the TLS sensor, while in another embodiment the tether connector can be first mated to the fin connector through the surgical drape before the fin connector is mated to the TLS sensor.

In the connection scheme shown in FIG. 14C, the stylet 130 is operably connected to the TLS sensor 50 via the tether connector 132, thus enabling the ECG sensor assembly of the stylet to communicate ECG signals to the TLS sensor. In addition, the ECG lead/electrode pairs 158 are operably connected to the TLS sensor 50. In one embodiment, therefore, the tether connector 132 is referred to as a first communication node for the stylet 130, while the fin connector 156 is referred to as a second communication node for the TLS sensor 50. As will be seen, various other first and second communication nodes can be employed to enable the establishment of a conductive pathway between the ECG sensor assembly and the TLS sensor or other system component.

Note that various other connective schemes and structures can be employed to establish operable communication between the stylet and the TLS sensor. For instance, the tether connector can use a slicing contact instead of a pin contact to pierce the drape. Or, the fin connector can be integrally formed with the TLS sensor. These and other configurations are therefore embraced within the scope of embodiments of the present disclosure.

As mentioned, a drape 174 is often placed over the patient 70 and employed as a barrier to separate a sterile field of the patient, e.g., areas and components above the drape and proximate to the insertion site 73 (including the catheter 72, the stylet 130, and tether 134 (FIG. 10)) from non-sterile areas outside of the sterile field, e.g., areas and components below the drape, including the patient's chest, the sensor 50 (FIG. 10) placed on the chest, and regions immediately surrounding the patient 70, also referred to herein as a non-sterile field. As seen in FIG. 15, the sterile drape 174 used during catheter placement to establish the sterile field is interposed between the interconnection of the tether connector 132 with the fin connector 156. As just described, the tether connector 132 includes the pin contact 170 that is configured to pierce the drape 174 when the two components are mated. This piercing forms a small hole, or perforation 175, in the sterile drape 174 that is occupied by the pin contact 170, thus minimizing the

17

size of the drape perforation by the pin contact. Moreover, the fit between the tether connector **132** and the fin connector **156** is such that the perforation in sterile drape made by piercing of the pin contact **170** is enclosed by the tether connector channel **172**, thus preserving the sterility of the drape and preventing a breach in the drape that could compromise the sterile barrier established thereby. The tether connector channel **172** is shaped and configured so as to fold the sterile drape **174** down prior to piercing by the pin contact **170** such that the pin contact does not pierce the drape until it is disposed proximate the hole **162** of the fin connector **156** and such that the drape does not bunch up within the channel. It is noted here that the tether connector **132** and fin connector **156** are configured so as to facilitate alignment therebetween blindly through the opaque sterile drape **174**, i.e., via palpation absent visualization by the clinician of both components.

As already mentioned, note further that the fin contacts **168** of the fin connector **156** as shown in FIG. **15** include the indentations **168A**, which are configured to mate with the sensor base contacts **154** in such a way as to assist in retaining the fin connector in engagement with the sensor base channel **152A**. This in turn reduces the need for additional apparatus to secure the fin connector **156** to the TLS sensor **50**. In other embodiments, retention features that are separate from the electrical contacts can be employed to assist in retaining the fin connector in engagement with the sensor base channel. In one embodiment, the base contacts **154** can be configured as pogo pins such that they are vertically displaceable to assist in retaining the fin connector **156**.

FIG. **16** shows a typical ECG waveform **176** of a patient, including a P-wave and a QRS complex. Generally, and with respect to the present system **10**, the amplitude of the P-wave varies as a function of distance of the ECG sensor assembly from the SA node, which produces the P-wave of the waveform **176**. A clinician can use this relationship in determining when the catheter tip is properly positioned proximate the heart. For instance, in one implementation the catheter tip is desirably placed within the lower one-third ($\frac{1}{3}$) of the superior vena cava, as has been discussed. The ECG data detected by the ECG sensor assembly of the stylet **130** is used to reproduce waveforms such as the waveform **176**, for depiction on the display **30** of the system **10** during ECG mode.

Reference is now made to FIG. **17** in describing display aspects of ECG signal data on the display **30** when the system **10** is in ECG mode, the third modality described further above, according to one embodiment. The screenshot **178** of the display **30** includes elements of the TLS modality, including a representative image **120** of the TLS sensor **50**, with the icon **114** corresponding to the position of the distal end of the stylet **130** during transit through the patient vasculature. The screenshot **178** further includes a window **180** in which the current ECG waveform captured by the ECG sensor assembly of the stylet **130** and processed by the system **10** is displayed. The window **180** is continually refreshed as new waveforms are detected.

Window **182** includes a successive depiction of the most recent detected ECG waveforms, and includes a refresh bar **182A**, which moves laterally to refresh the waveforms as they are detected. Window **184A** is used to display a baseline ECG waveform, captured before the ECG sensor assembly is brought into proximity with the SA node, for comparison purposes to assist the clinician in determining when the desired catheter tip location has been achieved. Windows **184B** and **184C** can be filled by user-selected detected ECG waveforms when the user pushes a predetermined button on the probe **40** or the console button interface **32**. The waveforms in the windows **184B** and **184C** remain until overwrit-

18

ten by new waveforms as a result of user selection via button pushes or other input. As in previous modes, the depth scale **124**, status/action indicia **126**, and button icons **128** are included on the display **30**. An integrity indicator **186** is also included on the display **30** to give an indication of whether the ECG lead/electrode pairs **158** are operably connected to the TLS sensor **50** and the patient **70**.

As seen above, therefore, the display **30** depicts in one embodiment elements of both the TLS and ECG modalities simultaneously on a single screen, thus offering the clinician ample data to assist in placing the catheter distal tip in a desired position. Note further that in one embodiment a print-out of the screenshot or selected ECG or TLS data can be saved, printed, or otherwise preserved by the system **10** to enable documentation of proper catheter placement.

Although the embodiments described herein relate to a particular configuration of a catheter, such as a PICC or CVC, such embodiments are merely exemplary. Accordingly, the principles of the present invention can be extended to catheters of many different configurations and designs.

FIGS. **18-19B** depict examples of contact engagement configurations for the tether connector **132** and fin connector **156**. Specifically, FIG. **18** depicts the fin contacts **168** of the fin connector **156** according to one embodiment, wherein the rear contact includes a spring clip configuration **168B** for receiving the pin contact **170** (FIG. **15**) of the tether connector **132** via the centering cone **164** or other aperture defined in the fin connector. FIGS. **19A** and **19B** depict an engagement scheme according to another embodiment, wherein the pin contact **170** of the tether connector **132** includes a barbed feature **170A** that, when inserted into the centering cone **164** or other aperture of the fin connector **156**, engages a shoulder **168C** defined on the rear fin contact **168** of the fin connector so as to help prevent premature removal of the pin contact from the fin connector. These embodiments thus serve as non-limiting examples of a variety of contact configurations that can be included with the fin connector **156**, the sensor connector base **152**, and the tether connector **132**. Note that unless referred to as otherwise, the contacts described herein are understood to include electrical contacts used in establishing a conductive pathway.

The embodiments to be described below in connection with FIGS. **20A-32** each depict an example connection scheme as a means for establishing a conductive or other communication pathway between a patient's sterile field and a non-sterile field, i.e., areas outside of the sterile field. Thus, the embodiments described herein serve as examples of structure, material, and/or compositions corresponding to the means for establishing a conductive or other communication pathway. In particular, various embodiments described herein disclose examples for breaching or otherwise circumventing a sterile barrier separating the sterile field from the non-sterile field so as to provide at least a portion of the conductive pathway for the passage of ECG signals from a sensing component such as the ECG sensor assembly of the stylet **130** to the sensor **50**, also referred to herein as a TLS sensor or chest sensor, or other suitable data-receiving component of the system **10**. Note that these embodiments are merely examples of a variety of means for establishing such a conductive or other communication pathway, and are not to be considered limiting of the scope of the present disclosure. It is therefore appreciated that the means for establishing a conductive or other communication pathway can be employed for transferring ECG signals or other information, electrical signals, optical signals, etc.

As will be seen, many of the embodiments to be described include a tether connector, also referred to herein as a first

19

communication node, which is operably connected to the stylet **130** and included in the sterile field, the tether connector is configured to operably attach to a connector included on the sensor **50** or other suitable component of the system **10**, also referred to herein as a second communications node, which is disposed outside of the sterile field. Note, however, that the first communication node and second communication node are contemplated as generally referring to various connector interfaces that provide a conductive pathway from the sterile field to the non-sterile field to enable the passage of ECG signals as described above. It is appreciated that the conductive pathway is a communication pathway and includes an electrical pathway, an optical pathway, etc. Further, the communication node connection schemes described and contemplated herein can be employed with systems involving the use of modalities exclusive of ECG signals for navigation or placement of a catheter or other medical device.

Note further that the embodiments to follow that describe configurations for breaching a drape or other non-transparent sterile barrier are configured such that location of a communication node disposed out-of-sight under the drape/barrier is facilitated by palpation of the clinician, thus easing location and connection of the first and second communication nodes. Also, many of the connector configurations described herein can be configured as one-use, disposable components so as to minimize concerns with infection.

Reference is now made to FIGS. **20A-20C**, which depict a connection scheme as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. In particular, FIGS. **20A-20C** depict a tether connector **232** that includes an outer housing **234** and a blade holder **236** that attaches to the outer housing. A blade contact **238** is secured by the blade holder **236** such that the blade contact extends into a channel **240** of the tether connector. The blade contact **238** serves to create a slice perforation in a drape that is interposed between the tether connector and the fin connector **256** when the tether connector **232** is slid on to engage the fin connector in the manner described in previous embodiments. As before, the outer housing **234** of the tether connector envelops and protects the perforation so as to prevent contamination and compromise of the sterile field.

FIG. **20C** shows that a fin connector **256** includes a fin contact **268** that is configured to physically interconnect with the blade contact **238** when the tether connector is slid on to the fin connector **256**, thus establishing a conductive pathway through the sheath so as to enable ECG signals from an ECG sensing component, i.e., the ECG sensor assembly described above for instance, to pass to the sensor **50** via the blade contact **238**/fin contact **268** engagement. Note that the particular configuration of the blade and fin contacts can be varied from what is described herein. For instance, the tether connector can include two or more blades or contacts for engagement with corresponding fin contacts to enable multiple conductive pathways to be established, if desired. The engagement surfaces of the tether connector and the fin connector can also vary from what is shown and described. In one embodiment, a light source can be included with the fin connector or other connectors as described herein so as to provide illumination through the drape **174** and provide visual assistance in locating the fin connector for interconnection with the tether connector.

As seen in FIGS. **14A** and **14B**, in one embodiment the ECG leads **158** are permanently connected to the fin connector **156**. FIG. **21A** depicts another possible embodiment, wherein the ECG leads are removably attached to the fin connector **156** via a connector, such as a horseshoe connector

20

270, best seen in FIG. **21B**. FIG. **21A** further shows that the fin connector **156** is permanently attached to the sensor **50**. These and other variations in the connective schemes of the various components of the system **10** are therefore contemplated as falling within the scope of the present disclosure. In another embodiment, the electrode of each lead is removably attachable from the lead, such as via a snap connection, for instance.

Reference is now made to FIGS. **22A-22C**, which depict a connection scheme as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. In particular, FIGS. **22A-22C** depict a tether connector **332** that includes a channel **372** for slidably engaging an upper barrel **166** of a fin connector **356** disposed on the sensor **50**, in a manner similar to previous embodiments. The tether connector **332** includes a bi-positional top cap **374** to which is attached a pin contact **370** or other piercing contact.

The top cap **374** is positioned in an un-actuated first position, shown in phantom in FIG. **22B**, when the tether connector **332** is first slid on to the fin connector **356**. The drape, removed for clarity, is interposed between the upper barrel **166** of the fin connector **356** and the tether connector channel **372**, similar to earlier embodiments. After the tether connector **332** is positioned on the fin connector **356**, the top cap **374** can then be depressed by the clinician into an actuated second position shown in FIG. **22B**, wherein the pin contact **370** is pressed downward through the drape and into operable engagement with a corresponding contact disposed in the fin connector **356**. The tether connector **332** is thus positioned as shown in FIG. **22C**. In addition to establishing a conductive path through the drape **174**, this engagement of the pin contact **370** locks the tether connector **332** on to the fin connector **356** so as to prevent premature separation of the components.

Reference is now made to FIGS. **23A** and **23B**, which depict a connection scheme as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. In particular, FIG. **23A** depicts a tether connector **432** including a pin contact **440** or other suitable contact attached to an actuation assembly **442**. The actuation assembly **442** includes lever arms for selectively lowering the pin contact **440** through an opening defined by a male end **448** of a housing **446** in which the actuation assembly is disposed. The male end **448** of the housing is configured to be received by a sensor connector receptacle **450** disposed on the sensor **50** or other suitable component of the system, such as a remote module operably connected to the sensor, for instance.

To interconnect the tether connector **432** to the sensor connector receptacle **450**, the male end **448** of the tether connector **432** is brought, above the drape **174**, into proximity with the receptacle **450**. The actuation assembly **442** is then actuated by raising the lever arms **444**, as shown in FIG. **23B**. The pin contact **440** is forced downward through the drape **174**, thus defining a perforation therein. The male end **448** can then be fully received into the sensor receptacle **450**, wherein the pin contact **440** operably connects with a suitable contact of the sensor connector receptacle. The connector scheme shown in FIGS. **23A** and **23B** is useful for imposing a minimal downward force on the body of the patient during connector interconnection. Further, the actuation assembly **442** provides a predetermined force in connecting the first communication node (the tether connector **432**) with the second communication node (the sensor connector receptacle **450**), and thus does not rely on a clinician's estimation of force to establish the node connection. In another embodiment, the housing **446** and the sensor receptacle **450** can be aligned and

mated before the actuation assembly 442 is actuated to pierce the contact 440 through the drape.

Reference is now made to FIG. 24, which depicts a connection scheme as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. As in the embodiment shown in FIGS. 23A and 23B, the present interconnection scheme minimizes downward pressure on the body of the patient during interconnection of the nodes. As shown, a tether connector 532 includes a pin contact 540 or other suitable contact included with a threaded cap 542, which defines threads on an inside surface thereof. The threaded cap 542 is configured to threadingly receive a threaded base 544 disposed on the sensor 50 or other suitable component of the system, such as a remote module operably connected to the sensor, for instance. As before, the drape 174 is interposed therebetween.

To interconnect the tether connector 532 to the sensor 50, the threaded cap 542 of the tether connector is brought, above the drape 174, into proximity with the threaded base 544 and threaded on to the base. This causes the pin contact 540 to penetrate the drape 174, thus defining a perforation therein. Further threading of the cap 542 on to the base 544 causes the pin contact 540 to engage a contact receptacle 546 included in the base 544, thus operably interconnecting the two nodes. In one embodiment, the tether 134 is rotatably attached to the threaded cap 542 so as to prevent twisting of the tether during threading. The connector scheme shown in FIG. 24 is useful for imposing a minimal downward force on the body of the patient during connector interconnection as the force to join the two connectors is directed laterally with respect to the patient via the threading operation. Note further that a variety of thread configurations and locations, as well as different cap and base configurations, are contemplated by the present disclosure.

Reference is now made to FIGS. 25A and 25B, which depict a connection scheme as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. As in the previous embodiment, the present interconnection scheme minimizes downward pressure on the body of the patient during interconnection of the nodes. As depicted in FIGS. 25A and 25B, a tether connector 632 includes one or more piercing contacts, such as pin contacts 640A and 640B that are respectively included on slide arms 642A and 642B. One or more contact receptacles, such as contact receptacles 644A and 644B, are included on a portion of the sensor 50, such as a sensor fin 646, or other suitable system component. As before, the drape 174 is interposed between the tether connector 632 and the sensor fin 646 to serve as a sterile barrier.

To interconnect the tether connector 632 to the sensor fin 646, the tether connector is brought, above the drape 174, into proximity with the sensor fin such that the slide arms 642A and 642B straddle the sensor fin and such that the pin contacts 640A and 640B are aligned with corresponding contact receptacles 644A and 644B, as shown in FIG. 25A. The slide arms 642A and 642B are then slid toward one another such that the pin contacts 640A and 640B penetrate the drape 174, each defining a perforation therein. The slide arms 642A and 642B are slid inward until the pin contacts 640A and 640B seat within and operably connect with the corresponding contact receptacles 644A and 644B, as seen in FIG. 25B, thus interconnecting the two nodes. The connector scheme shown in FIGS. 25A and 25B is useful for imposing a minimal downward force on the body of the patient during connector interconnection as the force to join the two connectors is directed laterally with respect to the patient. Note that the particular configuration of the tether connector, the sensor fin,

and the contacts can vary from what is explicitly described herein. For instance, in one embodiment the slide arms can be configured as bi-positional rocker arms that are connected in a see-saw configuration with respect to one another. Also, one, two, or more contacts can be included on the slide arms.

Reference is now made to FIGS. 26A and 26B, which depict a connection scheme as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. As shown, an integrated connector 730 is incorporated into the drape 174 so as to enable operable interconnection therethrough. In the illustrated embodiment, the integrated connector 730 includes a conductive base portion 734 from which extend mechanical connectors, such as snap balls 736A and 736B.

As shown in FIG. 26B, the integrated connector 730 is positioned in the drape 174 as to be connectable with both a suitable receptacle 738 of a tether connector 732 and a suitable receptacle 740 of the sensor 50 or other suitable component of the system 10. In particular, the tether connector 732 can be snap-attached to the integrated connector 730, after which the integrated connector can be attached to the sensor 50, thus providing a suitable pathway for signals from the ECG sensor assembly in the sterile field to be transmitted through the sterile barrier of the drape 174 to the sensor in the non-sterile field. It is appreciated that, in other embodiments, the integrated connector can include other configurations, such as different mechanical connectors, e.g., friction connectors, male/female connectors, etc., and as such the receptacles on the tether connector and sensor can likewise be modified to accommodate the different mechanical connectors. Also, the connective scheme described above can be reversed such that the receptacles are included on the integrated connector and the snap balls on the respective tether connector and sensor. Further, though presently depicted as a unitary component, the integrated connector in other embodiments can include two or more pieces that are attached to each other through a previously defined hole in the drape during manufacture thereof. These and other variations are therefore contemplated.

Reference is now made to FIG. 27, which depicts a connection scheme as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. In detail, FIG. 27 depicts an intermediate module, i.e., ECG module 750, disposed outside of the sterile field of the patient, which is operably connected to the sensor 50 of the system 10 via a sensor cable 752. The ECG module 750 is also operably connected to the ECG leads 158. In one embodiment, the ECG module 750 includes the circuitry and other components necessary for receipt and analysis of the ECG signal detected by the ECG sensor assembly of the stylet 130. As such, a conductive pathway is established between the stylet 130 and the ECG module 750 by traversing the sterile field of the patient. In the present embodiment, this is accomplished by a tether connector 762 of the tether 134.

As depicted in FIG. 27, the tether connector 762 operably attaches to a receptacle 764 of the ECG module 750. As shown, the tether connector 762 can include a sufficiently long handle that enables the clinician to attach the sterile tether connector to the receptacle 764 of the non-sterile ECG module 750 without touching the ECG module itself, thus preventing any compromise of the sterile field. In one embodiment, the handle of the tether connector 762 can include an extendable J-hook contact, for instance, that can operably connect to a suitable contact of the ECG module.

FIG. 28 shows another example of a tether connector that can be employed with the ECG module 750 of FIG. 27 or other suitable component of the system 10 as part of a con-

nection scheme as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. In particular, FIG. 28 depicts a tether connector 832, which includes a handle and a barbed contact 836 or other suitable contact at a proximal end thereof. A sterile shield 838 is interposed between the handle 834 and the contact 836. The sterile shield 838 assists in protecting the hand of the clinician while inserting the contact 836 into the receptacle 764 of the ECG module 750 in a manner similar to what is shown in FIG. 27. Thus, the sterile shield 838 serves as an additional barrier to prevent inadvertent contact by the clinician with a component outside of the sterile field, such as the ECG module 750. Note that the size, shape, and particular configuration of the sterile shield and/or tether connector can vary from what is explicitly described in the present embodiment.

FIGS. 29A and 29B show yet another example of a connection scheme that can be employed with the ECG module 750 of FIG. 27 or other suitable component of the system 10 as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. In particular, FIG. 29A shows that the ECG module 750 can be enveloped by a sterile bag 850. A connector, such as the integrated connector 730 described above in connection with FIGS. 26A and 26B, can be incorporated into the bag. As shown in FIG. 29B, an inner snap ball or other mechanical connector of the integrated connector 730 can be received by the suitably corresponding receptacle 764 of the ECG module 750. The tether connector of the system 10 can then be operably connected with the outer snap ball or other connector of the integrated connector 730, thus establishing a conductive pathway between the sterile field and the non-sterile field without compromising sterility. Note that the sterile bag 850 can include any one or more of a variety of suitable materials, including plastic. Note also that the integrated connector can include other connector configurations in addition to what is explicitly described herein. In one embodiment, the sterile bag includes no integrated connector, but rather is pierced by a pin contact of the tether connector, such as the barbed contact 836 included on the tether connector 832 of FIG. 28.

Reference is now made to FIG. 30, which depicts a connection scheme as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. Specifically, the stylet 130 includes a tether connector 862 as a first communication node, as in previous embodiments. A remote sensor connector 864 is also included as a second communications node, and is operably connected to the sensor 50 of the system 10 via a remote sensor connector cable 866. The tether connector 862 and remote sensor connector 864 operably connect to one another along a connection interface 868. The drape 174 that serves as a sterile barrier is interposed between the tether connector 862 and remote sensor connector 864 at the connection interface 868, and a suitable drape piercing configuration is included with the tether connector and the remote sensor connector to establish a conductive pathway through the drape. The present embodiment thus discloses one embodiment wherein the second communication node is located remotely with respect to the sensor 50.

Reference is now made to FIG. 31, which depicts a connection scheme as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. Specifically, the present embodiment includes the tether connector 862 and the remote sensor connector 864 that operably connect to one another along the connection interface 868, as described in connection with FIG. 30, above. The remote sensor connector 864 in the

present embodiment is placed proximate the catheter insertion site 73 in a region over which a fenestration 880 defined in the drape 174 (portions of the drape omitted for clarity) is positioned to enable clinician access to the insertion site during catheter placement. The remote sensor connector 864 is adhered to the patient's skin proximate the catheter insertion site 73 with the use of an adhesive, tape, etc., before the region surrounding the insertion site is sterilized in preparation for catheter insertion. Thus, when the insertion site is sterilized, the remote sensor connector 864 is also sterilized. Later, when connection of the tether connector 862 to the remote sensor connector 864 is made, the clinician can handle the latter component without compromising the sterile field of the patient. It is appreciated that the particular configurations of the tether connector and the remote sensor connector can vary while still residing within the scope of the present embodiment.

Reference is now made to FIG. 32, which depicts a connection scheme as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. Specifically, FIG. 32 shows the probe 40 employed by the system 10 for US functionality, as described above in connection with FIGS. 3A and 3B. A sterile sheath 900 is placed over the probe 40 so as to bring the probe into the sterile field of the patient. A connection interface, such as a receptacle 910, is included on the probe 900 and is configured so as to be operable connectable with a tether connector 920. In one embodiment, for example, the tether connector 920 includes a pin contact that penetrates the sterile sheath 900 to mate with the receptacle 910 in such a way as to prevent contamination of the sterile field. In this way, the tether connector 920, as a first communication node, operably connects with the probe 40, as a second communications node. In turn, the probe 40 is operably connected to the system console 20, as seen in FIG. 31 for example, so as to enable ECG signals received by the ECG sensor assembly of the stylet 130 via the tether connector 920 to be forwarded to the console, the sensor 50, or other system component for processing, as described above. In another embodiment, the receptacle 910 or other suitable connection interface can be included on the cable connecting the probe 40 to the system console 20. The particular contact configuration of the receptacle 910 and tether connector 920 can be varied according to the understanding of one skilled in the art. For instance, an integrated connector such as that shown in FIGS. 26A and 26B can be incorporated into the sterile sheath in one embodiment. Note further that, though including plastic in the present embodiment, the sterile sheath as described herein can include other suitable materials for providing sterility.

Reference is now made to FIG. 33 in describing means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. As shown, the tether 134 includes a wireless module 950, included within the sterile field, which serves as a first communication node for wirelessly transmitting (via RF or other suitable frequency or frequency range) ECG data received from the ECG sensor assembly of the stylet 130 to a data-receiving component as a second communication node, such as the sensor 50 or other suitable component of the system 10. A wireless module ground electrode 952 is operably connected with the wireless module 950 for placement in the sterile field proximate the catheter insertion site 73. A system ground electrode 158A extends from the sensor 50 for placement outside of the sterile field but proximate both the catheter insertion site 73 and the location of the wireless module ground electrode 952. One possible placement location for the system ground electrode 158A is beneath the patient arm, as depicted in FIG. 33.

The system reference electrode **158B** is placed on the lower torso of the patient **70** or other suitable location, as in previous embodiments. Note that the wireless module and system console as discussed herein can be configured in one or more of a variety of ways and include components for wireless signal transmission and reception not specifically detailed herein, such as patch or other antennas, signal transducers, etc.

With the system configured as shown in FIG. **33**, the system ground electrode **158A** can be electrically driven such that it produces a voltage that is sensed by the passive wireless module ground electrode **952**, given its proximate location with respect to the system ground electrode. This enables both ground electrodes to be at substantially equal electric potentials, thus enabling the wireless module **950** to utilize the wireless module ground electrode **952** and the ECG signals from the ECG sensor assembly of the stylet **130**, e.g., the core wire **138** (FIGS. **12C-12E**) in one embodiment, to detect and wirelessly transmit the ECG data to the sensor **50** for comparison with the data sensed by the system reference electrode **158B** in order to obtain the desired P-wave waveform (e.g., FIG. **16**). The data comparison in one embodiment is a differential comparison between the ECG data as obtained by the ECG sensor assembly of the stylet **130**, the wireless module ground electrode **952**, and the system reference electrode **158B**. In one embodiment, the system ground electrode **158A**, like the wireless module ground electrode **952**, can be passive and not electrically driven. Note also that the analog ECG data can be digitized or otherwise processed by the wireless module **950** before transmission to the sensor **50** or other system component, such as the console **20**.

FIG. **34** describes yet another wireless configuration as a means for establishing a conductive pathway between sterile and non-sterile fields, according to one embodiment. As shown, a positive electrode **954A** at a location A and a negative electrode **954B** at a location B are included with the sensor **50** and positioned on the torso of the patient **70**, while a positive wireless module electrode **956** is included with the wireless node **950**, as indicated at location C, positioned on or in the patient proximate the catheter insertion site **73**. The ECG sensor assembly of the stylet **130**, e.g., the core wire **138** in one embodiment, serves as a negative electrode for the wireless portion of the depicted configuration, indicated at D in FIG. **34** at its final position. Note that in one embodiment the locations A and B of the electrodes **954A** and **954B**, respectively, can be altered on the patient body to tune the system **10** for best ECG signal reception.

In the present embodiment, the electrodes **954A** and **954B** serve as a first independent source for sampling bipolar ECG signals. The ECG data from these electrodes are digitized and forwarded to the console **20** or other suitable system component via the cable interconnecting the sensor **50** and the console (path **1**) outside of the sterile field. The wireless module electrode **956** and the ECG sensor assembly serve as a second independent source for sampling bipolar ECG signals. The ECG data from these electrodes are digitized and forwarded wirelessly to the console **20** via the wireless module **950** (path **2**) within the sterile field. Thus, in the present embodiment the wireless module **950** serves as a first communication node, and a wireless receiver of the console **20** as a second communication node for the transfer of ECG signals between the two nodes. Note that the polarities of the afore-mentioned electrodes can be reversed in other embodiments.

The ECG signals received along both paths **1** and **2** are baseline corrected by appropriate circuitry of the console **20** to adjust for DC offset and drift. After such correction, a non-changing reference, or baseline, P-wave waveform **176A** from path **1** can be produced, as seen in FIG. **35A**, for

example. Similarly, a P-wave waveform **176B** as seen in FIG. **35B** is produced from path **2**, which waveform changes as the stylet **130** within the catheter **72** is advanced toward the heart of the patient. During such advancement, the waveform **176B** from path **2** is subtracted from the P-wave waveform **176A** from path **1**, employing a digital differential amplifier, for instance. This subtraction removes all common components of the waveforms represented by each of the signals, and enables the console **20** to depict via its display **30** only the differences in the two signals, as seen for example by the waveform **176C** shown in FIG. **35C**. The change in P-wave of the waveform from path **2** can then be easily observed during catheter advancement. Thus the present embodiment enables an easily observable digital display of ECG data to be represented while preventing a physical breaching of a sterile barrier, such as a surgical drape, for the passage of such data.

Note that in other embodiments the wireless module electrode **956** can include other configurations, including a conductive element imbedded into an introducer sheath, in contact with the bloodstream of the patient, which is commonly disposed through the insertion site **73** during catheter placement. The introducer can include a connector on a proximal portion thereof to enable a connection with the wireless node **950** to be made, in one embodiment.

Note further that one or more of a variety of wireless protocols can be employed in transmitting wireless signals in accordance with the embodiments described herein, including one or more of the IEEE 802.11 family of specifications, etc. Also note that in one embodiment the wireless module can be included in a sterile sheath, as described in previous embodiments, to bring the module within the sterile field, together with connectors for operably connecting the wireless module electrode through the sheath or included in the sheath itself. Of course, other methods for maintaining the wireless module within the sterile field can also be employed. In one embodiment, the wireless module can include buttons that further enable control of the system **10** from within the sterile field.

FIG. **36** shows that in one embodiment the sensor **50** can be retro-fitted with a wireless module **960** to enable signals received by the sensor to be wirelessly transmitted to the console **20** or other suitable component of the system **10**. For instance, ECG data received by the ground and reference electrodes **158A**, **158B** (FIG. **34**) can be received by the sensor **50** then wirelessly transmitted to the system console via the wireless module **960**. The wireless module **960** can include an antenna or other transmitting component and can operably connect to the sensor **50** via a sensor cable **962** or other suitable interface. Note that the wireless module **960** can be employed in connection with other embodiments described herein, including those depicted in FIGS. **10** and **33**, for instance.

FIG. **37** shows a retention feature for preventing inadvertent separation of the fin connector **156** from the sensor connector base **152** or other receptacle with which the fin connector operably connects, according to one embodiment. As shown, the fin connector **156** includes a retention arm **970** that is resiliently attached to the fin connector body. The retention arm **970** includes a tab **972** that slides over and engages a lip **974** included with the connector base **152** of the sensor **50** when the fin connector **156** is slidably received in the sensor channel **152A** (FIG. **14A**). The engagement of the tab **972** with the lip **974** prevents inadvertent removal of the fin connector **156** during use. When removal of the fin connector **156** from the sensor connector base **152** is desired, the retention arm **970** is lifted so as to disengage the tab **972** from the lip **974**, after which the fin connector can be slid out of engage-

ment with the sensor channel **152A**. This configuration can be employed either with or independent of other retention features, such as the indentations **168A** (FIG. **13D**). Note that in other embodiments a variety of modifications and configurations can be employed in assisting to maintain engagement between the fin connector and the connector. For instance, the retention arm in one embodiment can be operably attached to one or more of the fin contacts **168** (FIG. **13D**) such that displacement, e.g., lifting laterally moving, pinching, etc., of the retention arm or other suitable fin connector component disengages the fin contact(s) from the base contacts (FIG. **15**), thus reducing the overall retention force provided by the engagement of the fin contacts with the base contacts. Note further that these principles can be applied to the other connector schemes disclosed or contemplated in addition to the fin connector described here.

In addition to the above embodiments depicting various connection schemes as means for establishing a conductive pathway between sterile and non-sterile fields, other configurations can be employed, as appreciated by one skilled in the art, for performing the same functionality. Such other configurations can include, for example, wireless transmission of ECG signals from the stylet to the sensor or the system component, the inclusion of electrically conductive thread in the drape, the inclusion of an electrically conductive window (e.g., composed of an electrically conductive plastic or foil) in the sterile drape, etc. In yet another embodiment, a proximal end of the stylet/guidewire itself can be used to pierce the drape for receipt into a connector on the sensor. In this case, no tether is included on the proximal end of the stylet, and the stylet itself serves as the conductive pathway for transmitting ECG signals from the stylet sensor assembly to the sensor on the patient's chest. Such a configuration can allow for over-the-wire placement of the catheter using a stylet/guidewire as described here. As such, the above embodiments should not be construed as being limiting of the present invention in any way.

FIGS. **38-44** describe features of embodiments relating to a radiating element for use in assisting in the placement of an implantable medical device, such as a catheter, within the body of a patient. The radiating element is capable of producing a detectable electromagnetic field and in one embodiment is included in a stylet. In particular, the stylet includes functionality to generate an electrical pulse signal to a coil assembly disposed at a distal end thereof. The resulting electromagnetic field produced by the coil assembly is detectable by the sensor unit of the catheter placement system generally described above, which is placed in proximate relation to the patient during catheter advancement. The stylet including the coil assembly is positioned within the catheter such that the coil assembly is substantially co-terminal with the distal end of the catheter, thus enabling a clinician to determine an approximate location and/or orientation of the catheter distal end during advancement thereof through the patient vasculature and to determine when a possible catheter malposition has occurred. As such, the stylet described here in connection with the present embodiment replaces the stylet including a passive magnetic assembly described in previous embodiments further above in connection with the catheter placement system.

In accordance with one embodiment, the stylet including the radiating element is physically untethered to a console or other component of the catheter placement system. Thus, the stylet itself includes all necessary componentry for producing the electrical pulse signal for use by the system. The stylet in one embodiment further includes functionality to synchro-

ment system such that the system can accurately track advancement of the stylet and its corresponding catheter through the patient vasculature. In another embodiment, the stylet including the radiating element is tethered to the sensor unit of the catheter placement system in such a way as to enable the passage of driving signals from the sensor unit or system console to the radiating element through a sterile barrier interposed between the catheter/stylet and sensor unit or console without compromising the barrier itself or the sterile field it helps establish.

Reference is made to FIGS. **1** and **38** which depict the various components of the catheter placement system ("system") **10**, configured in accordance with one example embodiment, and as have already been described further above. FIG. **38** shows the general relation of these components to the patient **70** during a procedure to place the catheter **72** into the patient vasculature through the skin insertion site **73**. As before, the system **10** is employed in connection with positioning the distal tip **76A** of the catheter **72** in a desired position within the patient vasculature. In one embodiment, the desired position for the catheter distal tip **76A** is proximate the patient's heart, such as in the lower one-third portion of the SVC.

As mentioned above, the catheter placement system **10** includes a tip location system ("TLS") modality that enables the clinician to quickly locate and confirm the position and/or orientation of the catheter **72** during initial placement into and advancement through the vasculature of the patient **70**. Specifically, the TLS modality is configured to detect an electromagnetic field generated by the radiating element, such as a coil assembly included at a distal end of a stylet, which is pre-loaded in one embodiment into a longitudinally defined lumen of the catheter **72**, thus enabling the clinician to ascertain the general location and orientation of the catheter tip within the patient body. The TLS also displays the direction in which the catheter tip is pointing, further assisting accurate catheter placement. In addition, the TLS assists the clinician in determining when a malposition of the catheter tip has occurred, such as in the case where the tip has deviated from a desired venous path into another vein.

As mentioned, the TLS utilizes a stylet in one embodiment to enable the distal end of the catheter **72** to be tracked during its advancement through the vasculature. FIGS. **38** and **39** give an example of a detached configuration of such a stylet **100**, configured in accordance with one embodiment. In particular, the stylet **100** in FIGS. **38** and **39** is physically detached, or untethered, from other components of the catheter placement system **10**. The stylet **100** includes a proximal end **100A** and a distal end **100B**. A stylet control module **102**, also referred to herein as a "fob," is included at the stylet proximal end **100A**, with an elongate portion **1104** extending distally therefrom.

FIG. **40** gives further details regarding a distal portion of the stylet elongate portion **104** proximate the stylet distal end **100B**. A coil assembly **1106** is included proximate the stylet distal end **100B** and is operably connected to leads **1106A**. The leads **1106A** are in turn operably connected to corresponding circuitry located in the stylet control module **102** configured to produce an electric pulse signal so as to enable the coil assembly **1106** to be electrically pulsed during operation and produce an electromagnetic field having a predetermined frequency or pattern that is detectable by one or more sensors included in the chest sensor **50** during transit of the catheter through the vasculature when the coil assembly is within the detectable range of the sensor. Note that the coil assembly described herein is but one example of a radiating element, or a component capable of producing an electromag-

netic field for detection by the sensor. Indeed, other devices and assembly designs can be utilized here to produce the same or similar functionality. For instance, non-limiting examples of other stylet configurations can be found in U.S. patent application Ser. No. 12/545,762, filed Aug. 21, 2009, and entitled "Catheter Assembly Including ECG Sensor and Magnetic Assemblies," which is incorporated herein by reference in its entirety. In one embodiment, more than one radiating element can be included, with each radiating element oriented in a different direction or spaced apart with respect to the other(s). In another embodiment, radiating elements of different types (e.g., ultrasonic and electromagnetic) can be included together.

The coil assembly 1106 and leads 1106A are disposed within tubing 1108 that extends at least a portion of the length of the stylet elongate portion 1104. The coil assembly and leads can be protected in other ways as well. A core wire 1110 can be included within the tubing 1108 in one embodiment to offer stiffness and/or directional torqueability to the stylet elongate portion 1104. The core wire 1110 in one embodiment includes nitinol and can extend to the distal end 100B of the stylet 100 or terminate proximal thereto.

In accordance with the present embodiment, the stylet 100 is untethered, or physically unconnected, with respect to the console 20 of the system 10. As such, the electric pulsing of the coil assembly 1106 to produce the predetermined electromagnetic field is driven by suitable componentry included in the fob, or stylet control module 102, as opposed to pulse driving by the console or other system component to which the stylet would be physically connected. FIG. 41 shows such componentry according to one example embodiment. The control module 102 includes a housing 102A in which a printed circuit board ("PCB") 1132 or other suitable platform is housed. Pulse circuitry 1134 is disposed on the PCB 1132 and includes a timer circuit 1136 configured to provide electrical pulses to the coil assembly 1106 via the leads 1106A (FIG. 40). It is noted that in one embodiment the electromagnetic field can be pulsed so as to produce a predetermined pattern, if desired.

A connector 1130A is included on the control module housing 102A and configured to removably and operably connect with a corresponding connector 1130B included on a proximal end of the stylet elongate portion 1104. In this way, operable connection between the timer circuit 1136 and the coil assembly 1106 via the leads 1106A is achieved in the present embodiment. Note that other connective schemes between the pulse circuitry and the coil assembly can be used. In another embodiment, the stylet elongate portion is permanently connected to the stylet control module.

A power supply 1140 is included with the stylet control module 102 to provide power necessary for control module functions, including operation of the pulse circuitry 1134 and driving of the electric pulsing performed by the timer circuit 1136. In one embodiment, the stylet 100 is a disposable, one-time use component and as such the power supply 1140 is also disposable, such as a button-cell battery. In other embodiments, the power supply can be a rechargeable battery, a long-life power supply, or can be configured to be replaceable as may be appreciated by one skilled in the art. In one embodiment, the control module 102 includes an on/off switch for controlling operation of the control module components.

As mentioned, the timer circuit 1136 drives the coil assembly 1106 by sending electrical pulses at a predetermined frequency to the coil assembly via the leads 1106A to which the timer circuit is operably connected. Receipt of the pulses causes the coil assembly 1106 to emit an electromagnetic

field having the predetermined frequency that is detectable by the sensor unit 50 of the system 10, thus assisting guidance of the catheter 72 (FIG. 38) as has been described.

In one embodiment, the electric pulse signal of the timer circuit 1136 is synchronized with the console 20, or other system component (such as the sensor 50), to enable the system 10 to identify the frequency of the field produced by the coil assembly 1106 as a result of the pulsing. This enables the console 20 to identify the proper field relating to the stylet coil assembly 1106 and the sensor unit 50 to accurately track progress of the stylet 100 during intravascular advancement of the catheter 72. The particular frequency/frequencies employed for the pulse signal in one embodiment comply with applicable laws and regulations, including regulations promulgated by the Federal Communications Commission ("FCC"). In one implementation a frequency of 1 MHz may be used, for example.

In the present embodiment, synchronization of the pulse signal frequency produced by the timer circuit 1136 with the console 20 is achieved by a transmitter 1138 included with the stylet control module 102, as seen in FIGS. 39 and 41. The transmitter 1138 is operably connected to and receives data from the timer circuit 1136 relating to the frequency of its pulse signal being sent to the coil assembly 1106. The transmitter 1138 transmits the data to a receiver 1142 included on the console 20. Receiving the data by the receiver 1142, the console 20 can then identify the electromagnetic field produced by the coil assembly 1106 when detected by the sensor unit 50 and thus track intravascular advancement of the catheter 72.

In one implementation, the data transmitted by the transmitter 1138 are a message detailing the pulsing frequency of the pulse signal produced by the timer circuit 1136. In another implementation, the data are merely a replication of the pulse signal itself that, when received by the console 20, enable the console to determine the frequency. The console processor 22 (FIG. 1) or other suitable console circuitry can be employed to perform this determination functionality. Of course, the data can take any one of a variety of formats and configurations to enable information relating to the pulse signal to be received by the console or other suitable component of the system. In certain embodiments, the console 20, the sensor unit 50, or other suitable component of the system 10 can include the necessary circuitry to synchronize with the signal produced by the stylet 100, as described herein.

The transmitter 1138 can transmit, and the receiver 1142 receive, the above-referenced data in any number of ways, but in one implementation the transmitter transmits via infrared ("IR") or radiofrequency ("RF") wavelengths for receipt by the receiver. As such, for example, the transmitter 1138 and receiver 1142 can be configured as an IR LED/detector pair in the first case, or as an antenna pair in the second case. Note that other types of transmitter/receiver configurations can be included to perform the intended functionality described herein. Other forms of electromagnetic radiation can be employed to transmit data, including visible light in one embodiment.

In one embodiment, the timer circuit of the untethered stylet control module is configured to be adjustable such that the pulse frequency can be selected from a plurality of predetermined frequency options. Such functionality may assist in the case where interference exists on one or more of the predetermined frequencies, where different stylets are used successively by the same system, or where multiple systems are used simultaneously in close proximity to one another. In such a configuration, a selector switch may be included on the control module housing 102A, the console 20, and/or other

suitable system component. The above or other suitable synchronization scheme can be used to coordinate the selected pulse frequency to be transmitted and received between the stylet control module and the console.

In another implementation, the stylet control module/console automatically switches to one of a plurality of possible pulse frequencies for use in driving the coil assembly. In this latter implementation, the console can be configured to successively scan the plurality of possible frequencies and perform frequency identification functions, including phase locking, to identify the frequency on which the stylet control module timer circuit is producing the electrical pulse signal, thus enabling synchronization of the console therewith.

FIG. 42 shows an example of the above synchronization implementation, according to one embodiment. As shown, a transmitter such as an antenna 1152 is included with the stylet control module 102 and is configured to emit radiofrequency ("RF") or other suitable signals. A receiver such as an antenna 1161 is included with the console 20 of the system 10 to receive signals emitted by the stylet control module antenna 1152. The console further includes various components for processing signals received by the antenna 1161, including a mixer 1163, an oscillator 1165, a low pass filter 1166, an analog-to-digital converter ("ADC") 1167, and a digital signal processor ("DSP") 1168.

During operation of the system 10, the stylet antenna 102B of the stylet control module 102 emits an RF or other suitable signal (e.g., infrared ("IR")) that provides data relating to the frequency of the pulse signal. The RF signal is received by the console antenna 1161. The mixer 1163 combines the signal received by the antenna 1161 with a predetermined signal generated by the oscillator 1165, which combined signal is then filtered through the low pass filter 1166 to remove any extraneous signals. The filtered and combined signal is passed through the ADC 1167, then analyzed by the DSP 1168 to determine whether the two signals forming the combined signal match. If so, phase shifting of the signals will be performed by the DSP and/or oscillator 1165 to lock the signals in phase.

If the signals do not match, the above process is repeated with a new signal having a different frequency being produced by the oscillator 1165 until the signal. The above process is iteratively repeated until the signal from the oscillator matches in frequency the signal emitted by the stylet control module antenna 1152 and subsequently received by the console antenna 1161. Thus, the oscillator 1165 in one embodiment is capable of cycling through a plurality of pre-set signal frequencies in attempting to match the emitted signal of the stylet control module antenna 1152. In another embodiment, the oscillator can cycle through a range of frequencies in attempting to match the emitted signal. As noted before, once the proper signal frequency is determined by the console 20, phase shifting as needed can be conducted to complete synchronization between the stylet 100 and the console 20, thus enabling the console to track the distal end of the stylet 100.

It is understood that the above is merely one example of synchronizing the pulse signal produced by the stylet coil assembly with the console and that other implementations can be employed to link the frequency between the stylet coil assembly and console or other component of the system.

In another embodiment, it is appreciated that the transmitter/receiver configuration can be reversed such that the transmitter is included with the console and directs information regarding the frequency of the pulse signal to the stylet control module, which receives the information via a receiver included therein. In yet another embodiment, both the stylet and the console are manufactured to operate with a pre-set

pulse signal frequency, requiring no subsequent synchronization therebetween. These and other possible configurations are therefore contemplated. Generally, it should be understood that the pulse circuitry and timer circuit of the stylet control module, together with the processor of the console 20, can be configured in one or more of a variety of ways to achieve above-described functionality. For instance, the processor 22 of the console 20 can be included in the sensor unit 50 (FIG. 1, 38) such that synchronization operations on behalf of the system 10 are performed by the sensor. Or, in another embodiment the stylet functionality is incorporated into the catheter itself and no removable stylet is employed.

Reference is again made to FIG. 38, which shows disposal of the untethered stylet 100 substantially within a lumen in the catheter 72 such that the proximal portion thereof, including the control module 102, extends proximally beyond the catheter lumen, the hub 74A and a selected one of the extension legs 74B. So disposed within a lumen of the catheter, the coil assembly 1106 proximate the distal end 100B of the stylet 100 is substantially co-terminal with the distal catheter end 76A such that detection by the TLS of the stylet coil assembly correspondingly indicates the location of the catheter distal end.

The TLS sensor unit 50 is employed by the system 10 during TLS operation to detect the electromagnetic field produced by the coil assembly 1106 of the stylet 100. As seen in FIG. 38, the TLS sensor unit 50 is placed on the chest of the patient during catheter insertion. The TLS sensor unit 50 is placed on the chest of the patient in a predetermined location, such as through the use of external body landmarks, to enable the field of the stylet coil assembly 1106, disposed in the catheter 72 as described above, to be detected during catheter transit through the patient vasculature. Again, as the coil assembly 1106 is substantially co-terminal with the distal end 76A of the catheter 72 (FIG. 38), detection by the TLS sensor 50 of the field produced by the coil assembly provides information to the clinician as to the position and orientation of the catheter distal end 76A during its transit.

In greater detail, the TLS sensor unit 50 is operably connected to the console 20 of the system 10 via one or more of the ports 52, as shown in FIG. 1. Note that other connection schemes between the TLS sensor and the system console can also be used without limitation. As just described, the coil assembly 1106 is employed in the stylet 100 to enable the position of the catheter distal end 76A (FIG. 38) to be observable relative to the TLS sensor unit 50 placed on the patient's chest. Detection by the TLS sensor unit 50 of the stylet coil assembly 1106 is graphically displayed on the display 30 of the console 20 during TLS mode, represented in FIGS. 6-8C, for example. In this way, a clinician placing the catheter is able to generally determine the location of the catheter distal end 76A within the patient vasculature relative to the TLS sensor unit 50 and detect when catheter malposition, such as advancement of the catheter along an undesired vein, is occurring. It should be appreciated that in one embodiment the positions of the radiating element and the sensor can be reversed such that remotely powered sensor is included with the stylet for detecting a field produced by the radiating element positioned external to the body of the patient.

As mentioned further above, note that the system 10 in one embodiment can include additional functionality wherein determination of the proximity of the catheter distal tip 76A relative to a sin θ -atrial ("SA") or other electrical impulse-emitting node of the heart of the patient 70 can be determined, thus providing enhanced ability to accurately place the catheter distal tip in a desired location proximate the node. Also referred to as "ECG" or "ECG-based tip confirmation," this

third modality of the system can enable detection of ECG signals from the SA node in order to place the catheter distal tip in a desired location within the patient vasculature. Note that any functionality of an ECG sensor included with the stylet may be incorporated with the stylet control module to provide a wireless pathway for transmitting ECG sensor data from the stylet ECG sensor to the system console, the TLS sensor, or other system component in conjunction with catheter placement procedures. Such functionality can be in addition to the inclusion of a radiating element, such as the coil assembly spoken of herein. Note further that, in one embodiment, the control module housing can further serve as a handle to assist in manipulating the catheter and/or stylet during intravascular advancement.

The untethered stylet associated with the system as described immediately above herein allows for simple management of the sterile field that is established about the insertion site 73 of the patient 70 (FIG. 38) during the catheter placement procedure by eliminating wires interconnecting the stylet and the console that would have to penetrate through the sterile field. FIGS. 43A-44 provide yet another solution for operably interconnecting a radiating element included with a stylet or other suitable device through the sterile field of the patient without compromising the sterility of the field, according to one embodiment. In particular the proximal end 100A of the stylet 100, instead of including a control module 102, rather includes a tether connector 2132 configured for operably connecting to a corresponding sensor unit connector 2156 disposed on the sensor unit 50, as shown in FIG. 43A. The tether connector 2132 in the present embodiment is operably connected to the distal portion of the stylet 100 via a tether 2134. Note that, though configured similarly to the tether connector 132 and fin connector 156 shown in FIGS. 14A-14C in connection with the ECG modality of the catheter placement system 10 as described further above, the tether connector 2132 and sensor connector 2156 that enable operable connection of the radiating element with the sensor unit 50 can be configured in other ways. As such, the discussion here is understood to describe merely one possible example of operable interconnection of a radiating element of a stylet or medical device with a sensor unit or other suitable component of a catheter placement system. Many other types of operable interconnection can be employed, as appreciated by one skilled in the art.

FIG. 43B shows the slide-on manner of connection of the tether connector 2132 with the sensor connector 2156 of the sensor unit 50. FIG. 44 shows a cross sectional view of the interconnection of the tether connector 2132 with the sensor connector 2156, wherein a channel 2172 of the tether connector includes a piercing element, such as a pin contact 2170, which extends into the channel. The drape 174 that covers the sensor unit 50 when the sensor unit is placed on the chest or other portion of the body of the patient is interposed between the tether connector 2132 and the sensor connector 2156 when the tether connector is slid on the sensor connector such that the pin contact 2170 pierces the drape, extends past a centering cone 2164 and through a hole 2162 defined in the sensor connector. Once the tether connector 2132 is seated on the sensor connector 2156, the pin contact 2170, which is electrically bifurcated, physically contacts two contacts 2168 disposed in the sensor connector so as to enable a suitable closed circuit to be established therebetween. In this way, the radiating element, e.g., the coil 1106, of the stylet 100 is operably connected via the tether 2134 and connectors 2132/2156 with the necessary driving circuitry for driving the coil, which circuitry can be located in the sensor unit 50, console 20, etc.

Furthermore, the interconnection of the tether connector 2132 with the sensor connector 2156 is established through the drape 174 without compromising the barrier provided by the drape for establishing sterility about the catheter insertion site 73 (FIG. 38), similar to previous embodiments discussed further above in connection with the ECG modality of the catheter placement system 10. Indeed, the tether connector 2132 desirably covers and isolates the drape breach made by the piercing pin contact 2170. Again, other types of through-drape connective schemes can be employed for operably connecting the radiating element with the sensor unit without compromising the sterile field.

Thus, in one embodiment, a method for operably connecting a radiating element with a sensor unit includes positioning the sensor unit on the patient, placing the sterile barrier over the sensor unit, and operably connecting the radiating element to the sensor unit by penetrating the sterile barrier.

Although the embodiments described herein relate to a particular configuration of a catheter, such as a PICC or CVC, such embodiments are merely exemplary. Accordingly, the principles of the present invention can be extended to catheters of many different configurations and designs.

Embodiments of the invention may be embodied in other specific forms without departing from the spirit of the present disclosure. The described embodiments are to be considered in all respects only as illustrative, not restrictive. The scope of the embodiments is, therefore, indicated by the appended claims rather than by the foregoing description. All changes that come within the meaning and range of equivalency of the claims are to be embraced within their scope.

What is claimed is:

1. A locator for locating a portion of a stylet within a body of a patient, comprising:

a stylet that is positionable in a lumen of a catheter including a first connector disposed at a proximal end thereof; a radiating element included with the stylet, the radiating element capable of producing an electromagnetic field; and

an external sensor unit positionable on a chest portion of the patient capable of detecting the electromagnetic field of the radiating element after the stylet is adapted to be positioned at least partially within the body of the patient, the external sensor unit includes a second connector, the first and second connectors are operably connectable such that the external sensor is operably connected to the radiating element through a physical barrier that provides at least a portion of a sterile barrier interposed therebetween without compromising the sterile barrier, and one of the first and second connectors includes a piercing component that pierces the physical barrier.

2. The locator as defined in claim 1, wherein the piercing component includes a first electrical contact that physically engages a second electrical contact of the other connector to electrically interconnect the first and second connectors.

3. The locator as defined in claim 2, further comprising a control module for controlling operation of the radiating element.

4. The locator as defined in claim 3, wherein the control module is capable of wirelessly transmitting at least one characteristic of the electromagnetic field produced by the radiating element.

5. The locator as defined in claim 4, wherein the at least one characteristic is transmitted between the control module and a component of a system for assisting in placement of the stylet.

35

6. The locator as defined in claim 4, further comprising a phase locking circuit for synchronizing a frequency of the electromagnetic field produced by the radiating element.

7. The locator as defined in claim 4, wherein the characteristic that is wirelessly transmitted is transmitted using one of visible, infrared, and RF radiation.

8. The locator as defined in claim 1, wherein the radiating element includes a first connector and the sensor unit includes a second connector, and one of the first and second connectors are configured to penetrate and operably connect to the other of the first and second connector after the sterile barrier is created without compromising the sterile barrier.

9. The locator as defined in claim 8, wherein one of the first and second connectors includes a piercing component to create a passage through a physical barrier creating a portion of the sterile field when the first and second connectors are mated, and wherein the first and second connectors interconnect when mated to enclose the passage and preserve the sterility of the sterile barrier.

10. A method for establishing a connection between a radiating element included with an implantable stylet and an external sensor unit through a sterile barrier, the method comprising:

positioning a stylet in a lumen of a catheter including a first connector disposed at a proximal end thereof having a radiating element included with the stylet, the radiating element capable of producing an electromagnetic field; positioning the sensor unit on a patient capable of detecting the electromagnetic field of the radiating element after the stylet is adapted to be positioned at least partially within the body of the patient, the external sensor unit includes a second connector;

placing the sterile barrier over the sensor unit; and operably connecting the first and second connectors such that the radiating element is operably connected to the sensor unit by penetrating a physical barrier that provides at least a portion of the sterile barrier with a piercing component of one of the first and second connectors without compromising the sterile barrier.

11. The method for establishing a connection as defined in claim 10, wherein the sterile barrier is a drape.

12. The method for establishing a connection as defined in claim 11, wherein operably connecting the radiating element further comprises:

penetrating the sterile barrier with the piercing element, the piercing element being electrically connected to the radiating element.

13. The method for establishing a connection as defined in claim 10, wherein operably connecting the radiating element to the sensor unit further comprises:

operably connecting the radiating element located in a sterile field to the sensor unit located outside of the sterile field.

14. The method for establishing a connection as defined in claim 13, wherein the radiating element is removably included with the stylet, and wherein the method further comprises:

36

physically connecting a tether connector operably connected to the radiating element with a connector of the sensor unit, the sterile barrier being interposed therebetween before the physical connection.

15. The method for establishing a connection as defined in claim 10, further comprising:

inserting the stylet including the radiating element in the body of the patient; and

monitoring a field produced by the radiating element.

16. The method for establishing a connection as defined in claim 10, further comprising creating a passage through a physical barrier that creates a portion of the sterile barrier with a connector of one of the radiating element and the sensor unit after the sterile barrier is placed over the sensor unit.

17. A locator for locating a portion of a medical device within a body of a patient, comprising:

a stylet that is positionable in a lumen of a catheter including a first connector disposed at a proximal end thereof;

a radiating element included with the stylet, the radiating element capable of producing an electromagnetic field, the radiating element of the stylet includes an electromagnetic coil that is substantially co-terminal with a distal tip of the catheter when the stylet is positioned in the lumen of the catheter; and

an external sensor unit positionable on a chest portion of the patient capable of detecting the electromagnetic field of the radiating element after the stylet is adapted to be positioned at least partially within the body of the patient, the external sensor unit includes a second connector, the first and second connectors are operably connectable such that the external sensor is operably connected to the radiating element through a drape that provides at least a portion of a sterile barrier interposed therebetween without compromising the sterile barrier, the first connector includes a piercing component that pierces the drape, the piercing component including an electrical contact.

18. The locator as defined in claim 17, wherein the electrical contact physically engages a second electrical contact of the second connector to electrically interconnect the first and second connectors.

19. The locator as defined in claim 17, further comprising a control module for controlling operation of the radiating element.

20. The locator as defined in claim 19, wherein the control module is capable of wirelessly transmitting at least one characteristic of the electromagnetic field produced by the radiating element.

21. The locator as defined in claim 20, further comprising a phase locking circuit for synchronizing a frequency of the electromagnetic field produced by the radiating element.

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 8,781,555 B2
APPLICATION NO. : 12/715556
DATED : July 15, 2014
INVENTOR(S) : Eddie K. Burnside et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In the Claims

Claim 2, column 34, line 55, delete “other” and insert --second--.

Claim 5, column 34, line 65, insert before “transmitted” --wirelessly--.

Claim 7, column 35, line 4, insert before “characteristic” --at least one--.

Signed and Sealed this
Ninth Day of September, 2014

A handwritten signature in black ink, reading "Michelle K. Lee". The signature is written in a cursive, flowing style.

Michelle K. Lee
Deputy Director of the United States Patent and Trademark Office

| | | | |
|---------------|---|---------|------------|
| 专利名称(译) | 用于放置导管系统，包括产生信号的探针 | | |
| 公开(公告)号 | US8781555 | 公开(公告)日 | 2014-07-15 |
| 申请号 | US12/715556 | 申请日 | 2010-03-02 |
| 申请(专利权)人(译) | C. R. BARD , INC. | | |
| 当前申请(专利权)人(译) | C. R. BARD , INC. | | |
| [标]发明人 | BURNSIDE EDDIE K MESSERLY SHAYNE | | |
| 发明人 | BURNSIDE, EDDIE K. MESSERLY, SHAYNE | | |
| IPC分类号 | A61B5/00 A61B19/00 A61B19/08 A61B5/06 A61B5/05 A61B8/00 A61B5/042 A61B8/08 | | |
| CPC分类号 | A61B2019/5263 A61B19/5244 A61B5/05 A61B5/062 A61B8/0833 A61B5/042 A61B19/08 A61B5/06 A61B2019/5251 A61B2019/5276 A61B19/38 A61B8/0841 A61B8/4472 A61B8/4263 A61B5/0833 A61B8/12 A61B8/4422 A61B34/20 A61B46/00 A61B90/40 A61B2034/2051 A61B2090/378 | | |
| 代理机构(译) | 鲁坦和塔克LLP | | |
| 优先权 | 61/095921 2008-09-10 US 61/045944 2008-04-17 US 61/091233 2008-08-22 US 61/095451 2008-09-09 US 60/990242 2007-11-26 US 61/156842 2009-03-02 US | | |
| 其他公开文献 | US20100204569A1 | | |
| 外部链接 | Espacenet USPTO | | |

摘要(译)

公开了一种用于将导管精确地放置在患者脉管系统内的集成导管放置系统。在一个实施例中，集成系统包括系统控制台，用于临时放置在患者胸部上的尖端位置传感器单元，以及超声探头。当导管设置在脉管系统中时，尖端位置传感器感测由设置在导管内腔中的探针产生的磁场。超声探头在引入导管之前对脉管系统的一部分进行超声成像。包括基于ECG信号的导管尖端引导，以使导管尖端能够相对于患者心脏的节点引导到期望的位置。探针包括电磁线圈，该电磁线圈可通过无菌屏障可操作地连接到传感器单元和/或控制台，而不会损害屏障。探针还可以无线连接到传感器单元和/或控制台。

