

(10) **Patent No.:** US 9,968,750 B2  
(45) **Date of Patent:** May 15, 2018

- (58) **Field of Classification Search**  
CPC ..... A61M 16/042; A61M 16/0463; A61M  
16/0475; A61M 16/0477; A61M 16/0484;  
(Continued)

- (56)
- References Cited**

- U.S. PATENT DOCUMENTS

- |           |     |         |             |             |
|-----------|-----|---------|-------------|-------------|
| 4,245,633 | A * | 1/1981  | Erceg ..... | A61M 16/104 |
|           |     |         |             | 128/205.17  |
| 5,161,525 | A * | 11/1992 | Kimm .....  | A61M 16/00  |
|           |     |         |             | 128/204.21  |

- FOREIGN PATENT DOCUMENTS

- |    |            |        |
|----|------------|--------|
| CA | 2 575 939  | 6/2000 |
| CN | 1 44 0 302 | 9/2003 |

- (Continued)

- Primary Examiner* — (Jackie) Tan-Uyen T Ho

- Assistant Examiner — Joseph D Boecker

- (74) *Attorney, Agent, or Firm* — Fay Kaplun & Marcin, LLP

- (57) **ABSTRACT**


- A ventilatory assist system and method are disclosed. The system comprises a tube for connection to a patient's airway, inspiratory and expiratory tube lumens connected to the tube, an inspiratory air source connected to the inspiration tube lumen, and a controller of air pressure in the expiratory tube lumen. The pressure controller is responsive to a physiological breathing signal representative of patient's inspiratory effort to allow air flow through the expiratory tube lumen during a patient's expiration phase, partially restricting the air flow through the expiratory tube lumen to a so minimum air flow during a patient's inspiration phase. During both respiratory phases, a unidirectional air flow is produced through the inspiratory and expiratory tube lumens to prevent air expired by the patient from being breathed again. The physiological breathing signal allows synchronization of the ventilatory assist with breathing efforts of the patient.

- 22 Claims, 6 Drawing Sheets**

(60) Provisional application No. 61/359,951, filed on Jun. 30, 2010.

- (51) **Int. Cl.**  
*A61M 16/00* (2006.01)  
*A61M 16/04* (2006.01)  
 (Continued)

- (52) **U.S. Cl.**  
CPC ..... *A61M 16/0003* (2014.02); *A61B 5/0488*  
(2013.01); *A61B 5/087* (2013.01);  
(Continued)

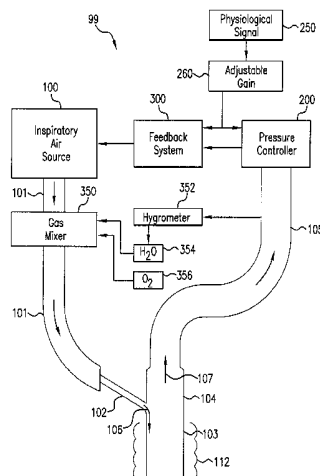

- (51) **Int. Cl.**  
*A61M 16/10* (2006.01) 5,954,051 A \* 9/1999 Heinonen ..... A61M 16/00 128/204.21  
*A61M 16/12* (2006.01) 6,588,423 B1 7/2003 Sinderby .....  
*A61M 16/16* (2006.01) 6,622,726 B1 \* 9/2003 Du ..... A61M 16/00 128/204.21  
*A61M 16/20* (2006.01) 6,901,286 B1 5/2005 Sinderby et al. ....  
*A61B 5/0488* (2006.01) 7,481,222 B2 \* 1/2009 Reissmann ..... 128/207.14  
*A61B 5/087* (2006.01) 2002/0020410 A1 \* 2/2002 Rydin ..... A61M 16/0051 128/200.24  
*A61B 5/00* (2006.01) 2002/0053345 A1 \* 5/2002 Jafari ..... A61M 16/00 128/204.23
- (52) **U.S. Cl.**  
 CPC ..... *A61B 5/4836* (2013.01); *A61M 16/00* (2013.01); *A61M 16/0012* (2014.02); *A61M 16/0051* (2013.01); *A61M 16/0069* (2014.02); *A61M 16/04* (2013.01); *A61M 16/042* (2014.02); *A61M 16/0486* (2014.02); *A61M 16/1005* (2014.02); *A61M 16/12* (2013.01); *A61M 16/125* (2014.02); *A61M 16/161* (2014.02); *A61M 16/202* (2014.02); *A61M 16/205* (2014.02); *A61M 16/024* (2017.08); *A61M 16/16* (2013.01); *A61M 2016/0018* (2013.01); *A61M 2016/0021* (2013.01); *A61M 2016/0027* (2013.01); *A61M 2016/0033* (2013.01); *A61M 2202/0208* (2013.01); *A61M 2210/1014* (2013.01); *A61M 2230/08* (2013.01); *A61M 2230/60* (2013.01)  
 2002/0129815 A1 \* 9/2002 McPhee ..... 128/200.24  
 2003/0075176 A1 \* 4/2003 Fukunaga et al. .... 128/203.12  
 2004/0069304 A1 \* 4/2004 Jam ..... 128/204.18  
 2004/0221854 A1 11/2004 Hete et al. ....  
 2004/0226559 A1 \* 11/2004 Daugherty ..... 128/203.12  
 2005/0150505 A1 \* 7/2005 Burrow et al. .... 128/911  
 2006/0249153 A1 \* 11/2006 DeVries ..... A61M 16/0057 128/204.18  
 2007/0062531 A1 \* 3/2007 Fisher ..... A61B 5/083 128/204.23  
 2007/0062534 A1 \* 3/2007 Fisher ..... A61B 5/029 128/205.14  
 2007/0144516 A1 \* 6/2007 Doyle ..... A61M 16/0883 128/204.18  
 2007/0295402 A1 \* 12/2007 Awtar et al. .... 137/119.01  
 2008/0060646 A1 \* 3/2008 Isaza ..... A61M 16/0468 128/204.21  
 2008/0121231 A1 \* 5/2008 Sinderby et al. .... 128/204.21  
 2008/0236590 A1 \* 10/2008 Reissmann ..... 128/207.14  
 2008/0264419 A1 \* 10/2008 Lomask ..... A61M 16/0051 128/204.23  
 2008/0308104 A1 \* 12/2008 Blomberg ..... A61M 16/00 128/204.23  
 2009/0159082 A1 6/2009 Eger .....  
 2009/0277448 A1 \* 11/2009 Ahlmen ..... A61M 16/0051 128/204.21  
 2010/0078024 A1 \* 4/2010 Andrieux ..... A61M 16/0051 128/204.21  
 2010/0095961 A1 \* 4/2010 Tornesel ..... A61M 16/0051 128/203.12  
 2010/0256513 A1 10/2010 Gumery et al. ....  
 2011/0126834 A1 \* 6/2011 Winter ..... A61M 16/0808 128/204.22  
 2016/0303340 A1 \* 10/2016 Sinderby ..... A61M 16/204
- (58) **Field of Classification Search**  
 CPC ..... A61M 16/0486; A61M 16/0069; A61M 16/009; A61M 16/00; A61M 16/0003; A61M 16/0012; A61M 16/0051; A61M 16/0066; A61M 16/021; A61M 16/022; A61M 16/04; A61M 16/0402; A61M 16/1005; A61M 16/12; A61M 16/125; A61M 16/202; A61M 16/205; A61M 2016/0015; A61M 2016/0018; A61M 2016/0027; A61M 2016/0033; A61B 5/087  
 USPC ..... 128/203.14, 204.18, 204.23  
 See application file for complete search history.

(56) **References Cited**

## U.S. PATENT DOCUMENTS

5,291,882 A 3/1994 Makhoul et al.  
 5,429,123 A 7/1995 Shaffer et al.  
 5,540,220 A 7/1996 Gropper et al.  
 5,671,752 A 9/1997 Sinderby et al.  
 5,797,393 A \* 8/1998 Kohl ..... A61M 16/00 128/204.18  
 5,820,560 A 10/1998 Sinderby et al.  
 5,823,184 A \* 10/1998 Gross ..... 128/204.18  
 5,823,186 A \* 10/1998 Rossen et al. .... 128/204.21

## FOREIGN PATENT DOCUMENTS

CN 1 973 766 6/2007  
 CN 101 160 148 4/2008  
 CN 101 337 101 1/2009  
 DE 10 118 605 6/2002  
 WO 2002/002169 1/2002  
 WO 2006/053446 5/2006  
 WO 2010/022513 3/2010

\* cited by examiner

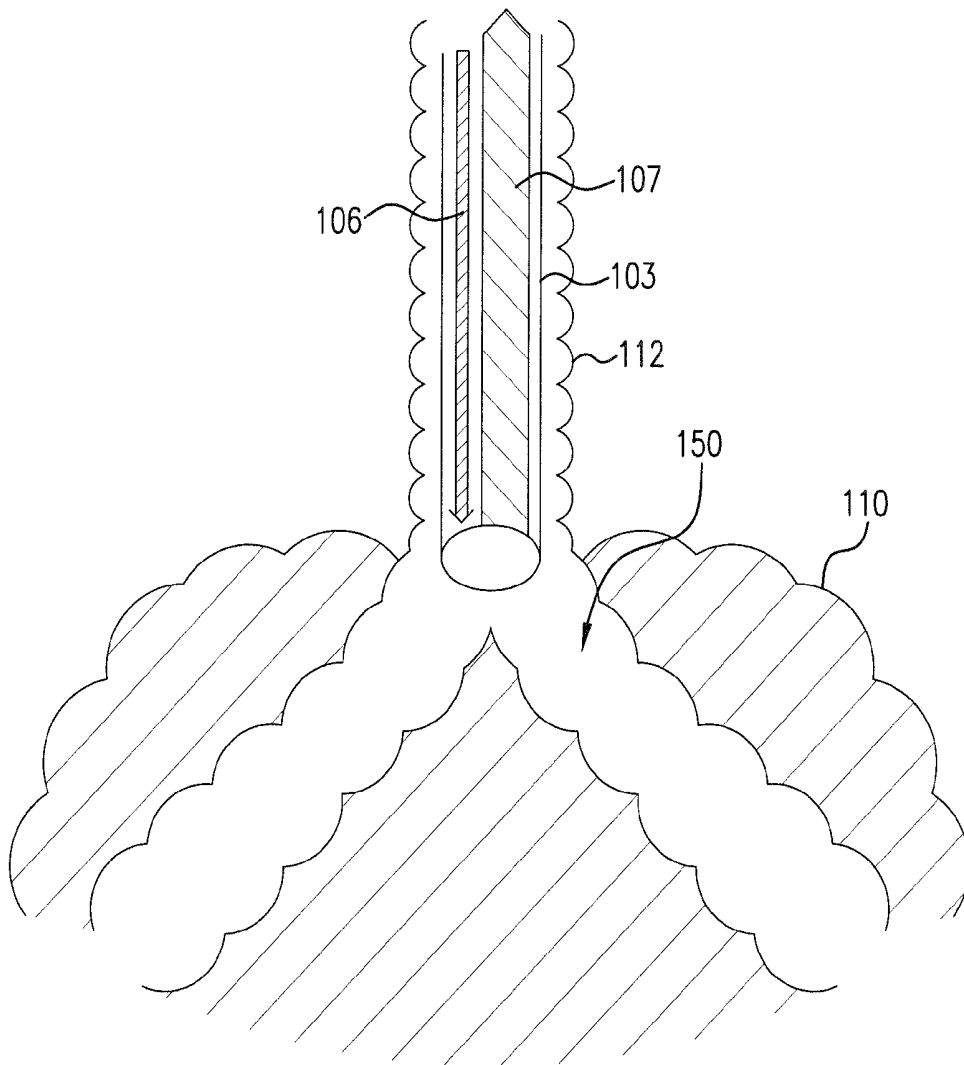


FIG. 1

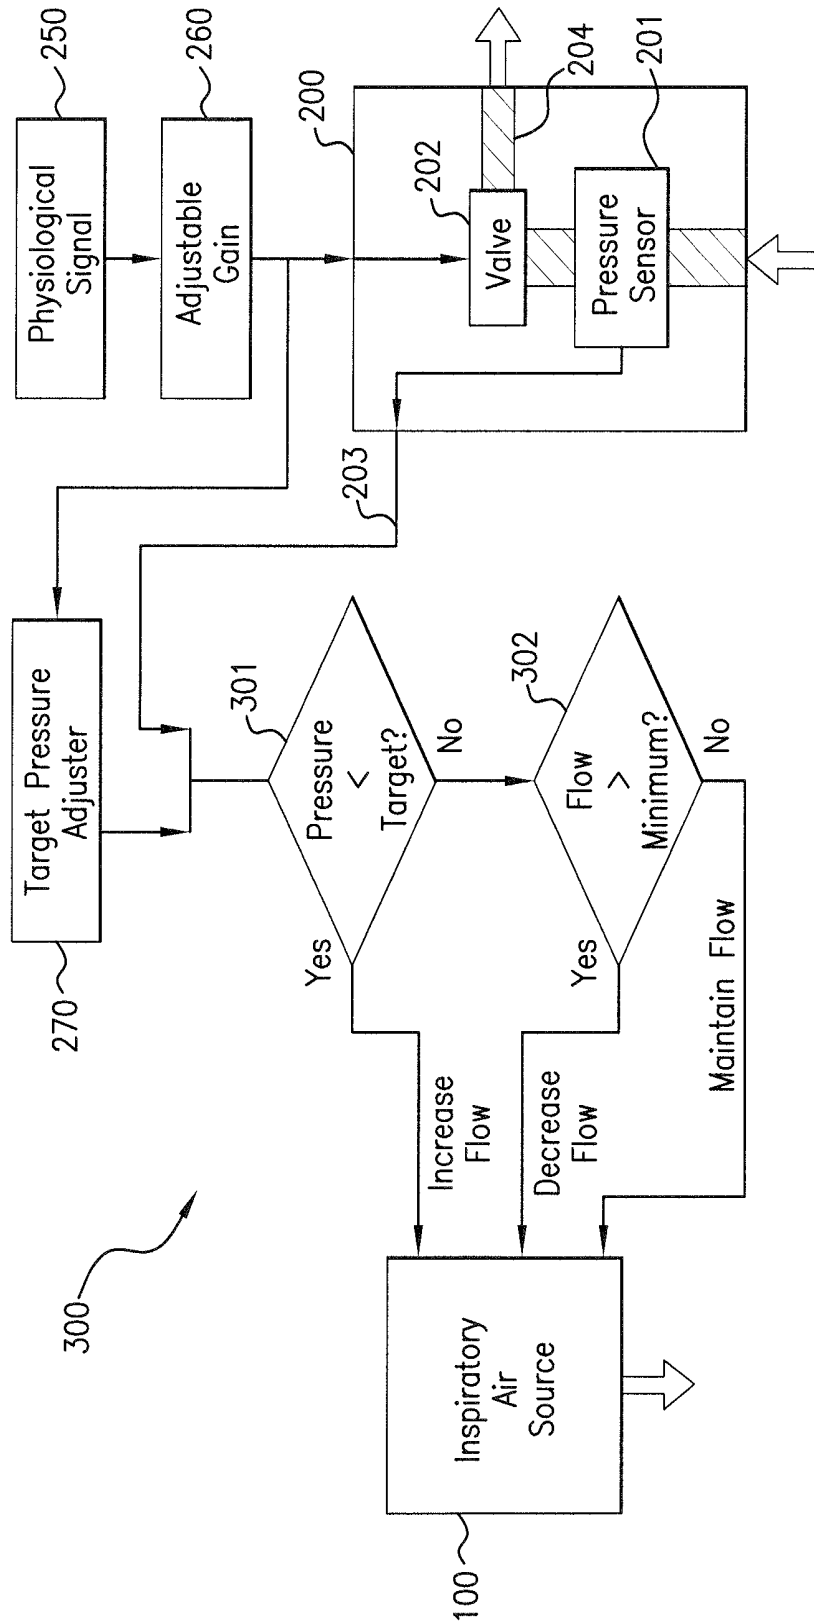


FIG.2

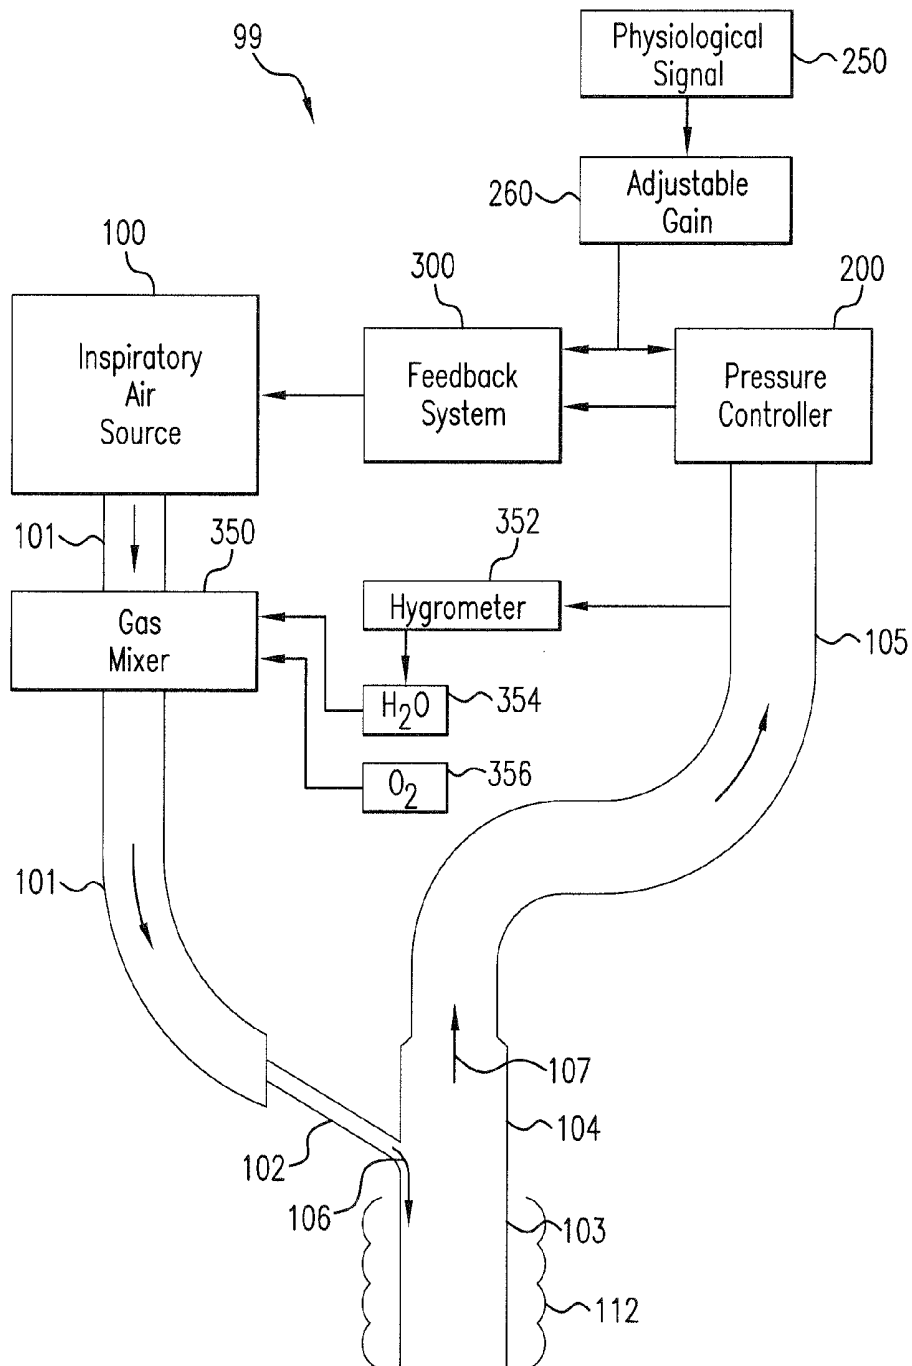


FIG. 3

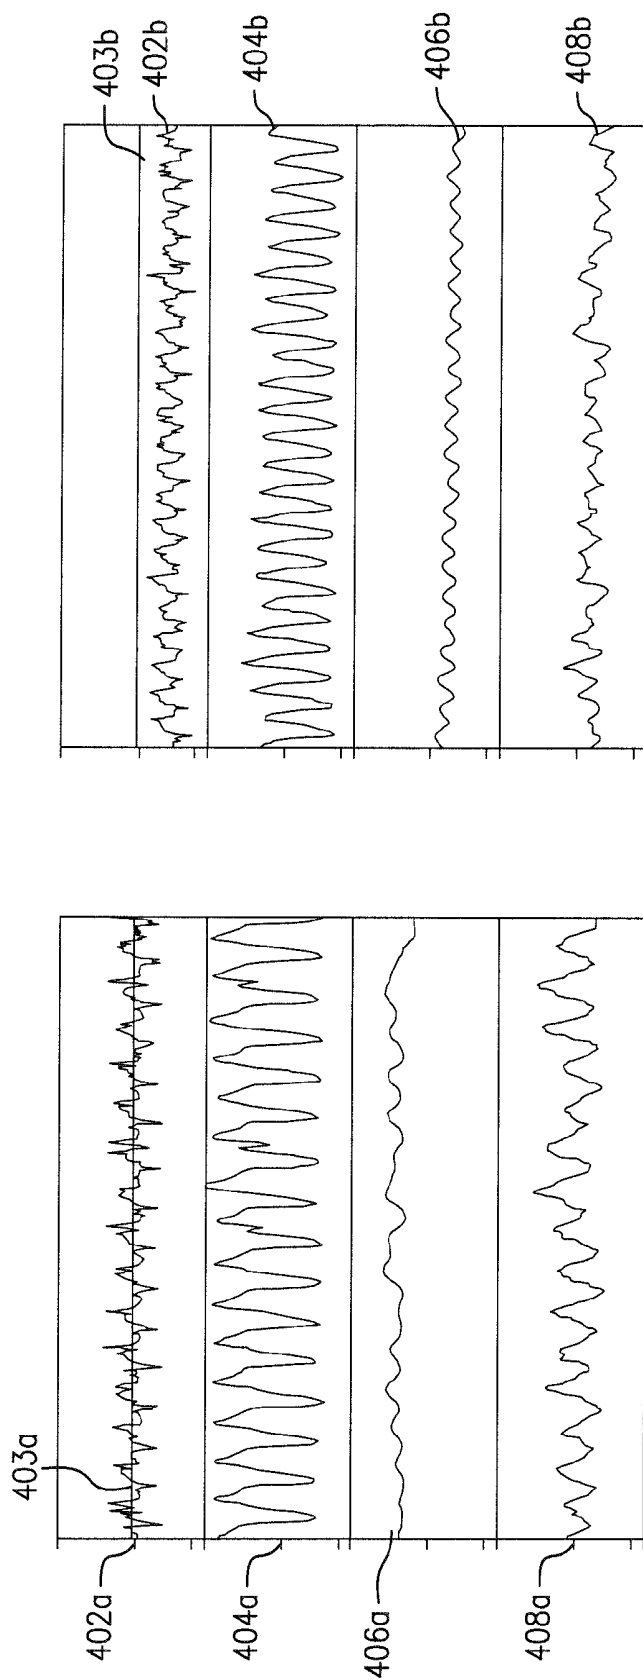


FIG. 4A

FIG. 4B

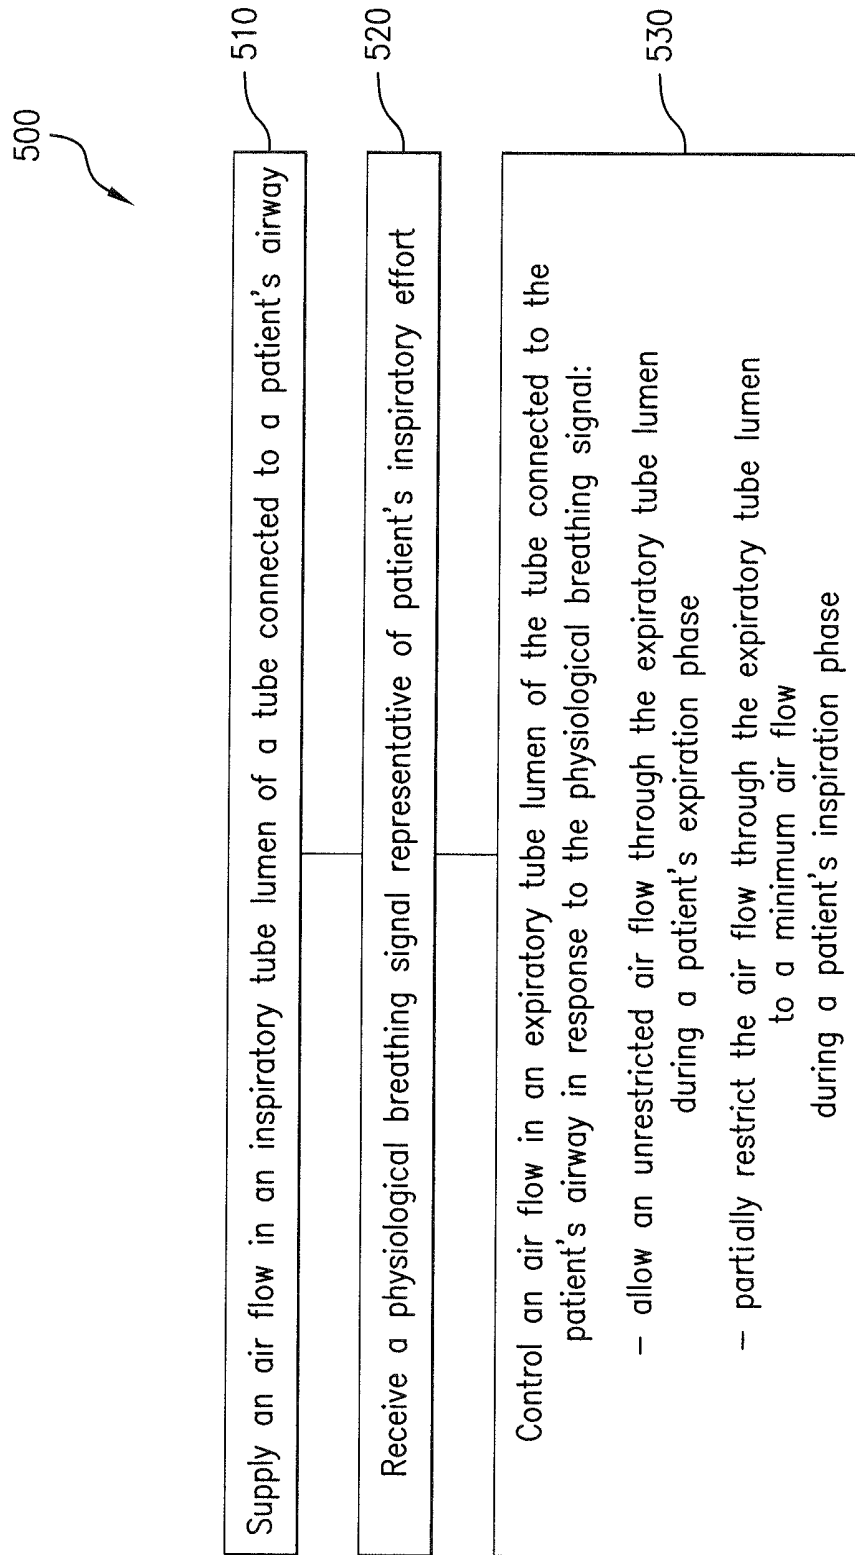


FIG. 5

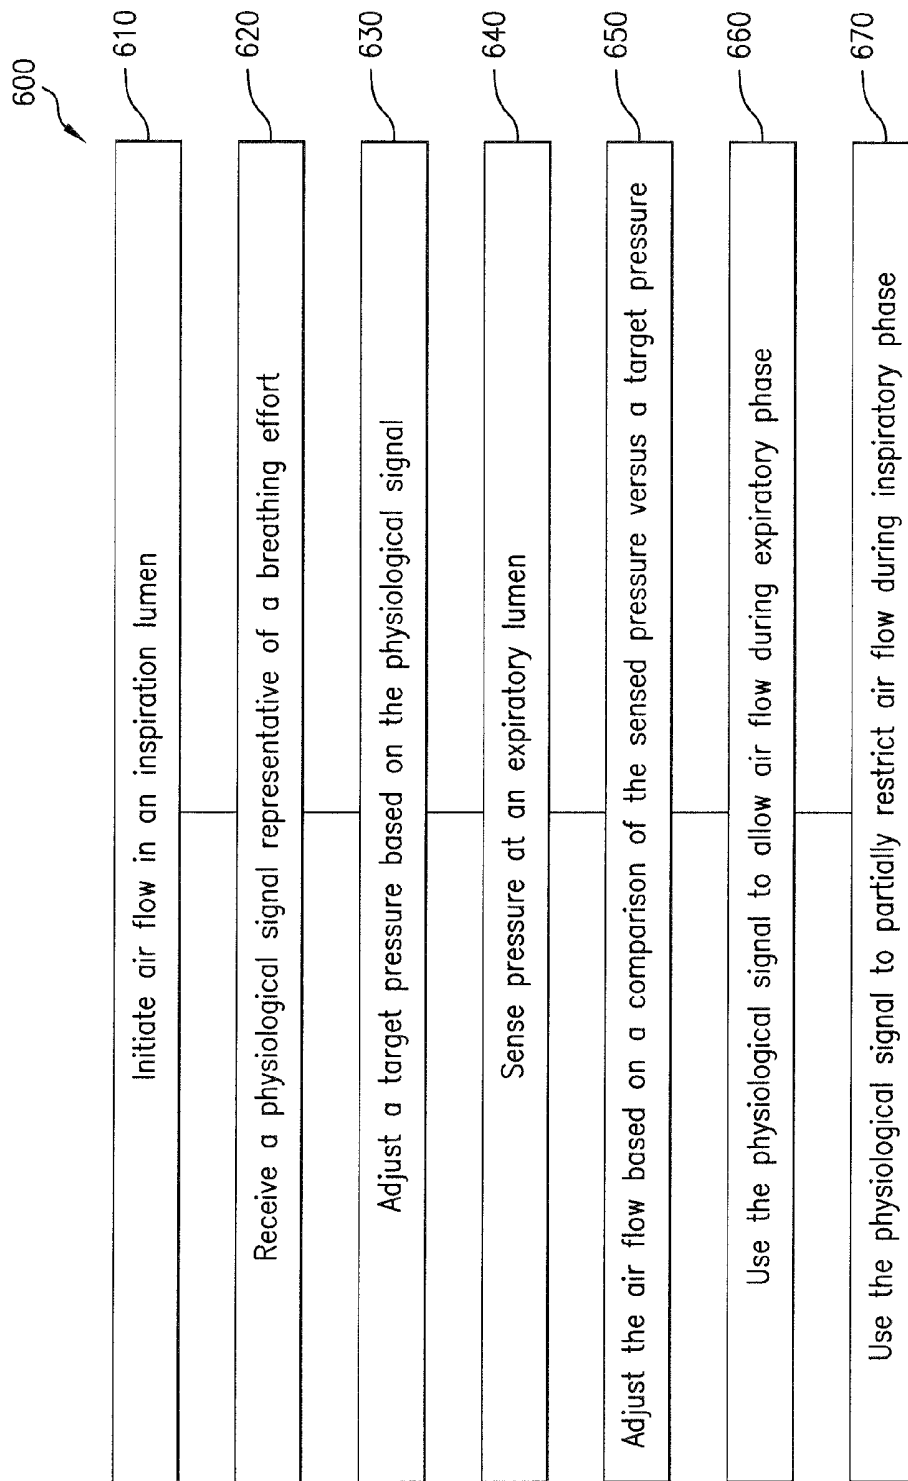


FIG. 6



1

# METHOD AND SYSTEM FOR PATIENT-SYNCHRONIZED VENTILATORY ASSIST WITH ENDOTRACHEAL THROUGH-FLOW

## TECHNICAL FIELD

The present disclosure relates to the field of ventilatory assist systems. More specifically, the present disclosure relates to a method and a system for patient-synchronized ventilatory assist with endotracheal through-flow.

## BACKGROUND

A recurring problem in patients with impaired function of the respiratory system is that the volume of air-exchanging lung parenchyma is reduced. This may be due to either edema, lung collapse and/or other factors. If a volume of air-transporting parenchyma/airways, comprising for example the main bronchi, trachea, and upper airways is maintained, the volume of air-exchanging parenchyma decreases relative to that of the air-transporting parenchyma/airways. In situations of increased need for CO<sub>2</sub> removal, a ventilatory contribution may be hampered if a dead space, or dead volume, in an air-transporting parenchyma/airways and in a respiratory circuit for a mechanical ventilator, becomes abnormally large relative to a proportion of the lungs with intact air-exchanging parenchyma. Consequently, CO<sub>2</sub> removal is hampered and arterial CO<sub>2</sub>(PaCO<sub>2</sub>) may increase. This causes the tidal volume and ventilation to increase in order to maintain a tolerable level of arterial pressure (PaCO<sub>2</sub>).

Until today, efforts have been made to minimize dead space, or dead volume, introduced in the respiratory circuit of mechanical ventilators. However actual tubes, for example endotracheal tubes, and other devices of conventional mechanical ventilators used to administer respiratory assist to a patient use single lumen designs and contribute to dead space ventilation. For that reason, CO<sub>2</sub> removal cannot be optimized.

Previous attempts to improve CO<sub>2</sub> removal from endotracheal tubes include multi-lumen designs aimed at introducing an air flow through a side lumen to eliminate CO<sub>2</sub> from a main lumen. An example of such design may be found in U.S. Pat. No. 5,291,882. The proposed approach, which uses parallel lumens, does not eliminate completely the volume of air re-breathed by the patient during inspiration. Thus the proposed approach reduces, but does not optimize the CO<sub>2</sub> removal and minimize the CO<sub>2</sub> re-breathing problem. Moreover, problems of dynamic hyperinflation due to constant inspiratory flow has also complicated this approach. Other approaches using tube lumens with valve functions may increase risk of occlusion.

Therefore, there is a need for improvements leading to further reduction or elimination of dead space induced by the respiratory circuit of a mechanical ventilator.

## SUMMARY

According to the present disclosure, there is provided a patient-synchronized ventilatory assist system. The ventilatory assist system comprises a tube for connection to a patient's airway, an inspiratory tube lumen connected to the tube, an expiratory tube lumen connected to the tube, an inspiratory air source connected to the inspiration tube lumen, and a controller of the pressure in the expiratory tube lumen. The pressure controller is responsive to a physiologi-

2

cal breathing signal representative of patient's inspiratory effort. Based on the physiological breathing signal, the pressure controller allows an unrestricted air flow through the expiratory tube lumen during a patient's expiration phase and partially restricts the air flow through the expiratory tube lumen to a minimum air flow during a patient's inspiration phase. During both the patient's inspiration and expiration phases, a unidirectional air flow is produced through the inspiratory tube lumen and the expiratory tube lumen to prevent air expired by the patient from being breathed again.

According to the present disclosure, there is also provided a patient-synchronized ventilatory assist method. The method comprises supplying an air flow in an inspiratory tube lumen of a tube connected to a patient's airway and, in response to a physiological breathing signal representative of patient's inspiratory effort, controlling an air flow in an expiratory tube lumen of the tube connected to the patient's airway. Controlling the air flow allows an unrestricted air flow through the expiratory tube lumen during a patient's expiration phase. Controlling the air flow also partially restricts the air flow through the expiratory tube lumen to a minimum air flow during a patient's inspiration phase. During both the patient's inspiration and expiration phases, a unidirectional air flow is produced through the inspiratory tube lumen and the expiratory tube lumen to prevent air expired by the patient from being breathed again.

The foregoing and other features will become more apparent upon reading of the following non-restrictive description of illustrative embodiments thereof, given by way of example only with reference to the accompanying drawings.

## BRIEF DESCRIPTION OF THE DRAWINGS

Embodiments of the disclosure will be described by way of example only with reference to the accompanying drawings, in which:

FIG. 1 is a side cross sectional, partial view of an example of double-lumen endotracheal tube showing intratracheal pulmonary ventilation;

FIG. 2 is block diagram of an exemplary pressure control system for use with the double-lumen endotracheal tube of FIG. 1;

FIG. 3 is an example of connection of the double-lumen endotracheal tube of FIG. 1 with the pressure control system of FIG. 2;

FIG. 4a is a graph of experimental recordings of physiological respiratory parameters illustrating operation of a conventional ventilator system;

FIG. 4b is a graph of experimental recordings of physiological respiratory parameters using the double-lumen endotracheal tube and pressure control system of FIGS. 1 and 2;

FIG. 5 is a flow chart of exemplary steps of a ventilatory assist method, capable of reducing neural inspiratory drive of a patient; and

FIG. 6 is a flow chart of other aspects of the ventilatory assist method of FIG. 5.

## DETAILED DESCRIPTION

Various aspects of the present disclosure generally address one or more of the problems related to the presence of dead space induced by respiratory circuits of mechanical ventilators. The present disclosure also relates to a ventilatory assist system and method including a feature of reduction of anatomical dead space in a patient's airways.

The following terminology is used throughout the present disclosure:

Ventilatory assist system: Apparatus adapted for medical use for assisting a patient in need of respiratory support.

Airway: Of a patient, lungs, bronchi, trachea, pharynx, nose and mouth, through which air is breathed.

Air: Any gas composition suitable for use in a ventilatory assist system. In the context of the present disclosure, the term "air" may refer to natural air, pure oxygen, natural air enriched with added oxygen, oxygen mixed with another gases such as water vapor, or any combination thereof. This term may also refer to air expelled from a patient's lungs, for example natural air containing additional CO<sub>2</sub> and humidity.

Lumen: A bore of a tube, for example a respiratory tube. A given tube may comprise a plurality of lumens.

Physiological signal: A measurable biometric quantity capable of being transmitted, for example as an electrical signal, such as the physiological breathing signal, generated by respiratory muscles.

Inspiratory effort: Voluntary or involuntary exertion of a breathing patient. This may be quantified as a neural measure.

Restricted/unrestricted: In the context of the present disclosure, an air flow present in a tube, lumen, or like conduit may be subject to a variable resistance, or restriction. It is well-known to those skilled in the art of fluid mechanics that any conduit will apply at least a minimum resistance to a flow. The terms "unrestricted" and "restricted" should be understood as relative terms expressing, respectively, a lower and a higher resistance to an air flow.

Minimum air flow: A partially restricted, non-zero air flow.

Endotracheal: Of a tube adapted for placement into a patient's trachea.

Synchrony: Time-wise correspondence between events.

A result of the reduction and elimination of dead space induced by the respiratory circuit of a mechanical ventilator is a reduction of respiratory drive, tidal volumes and ventilation, for example in critically ill patients. In this manner, mechanical ventilation may be used to efficiently unload the patient's respiratory system and respiratory muscles. Also, ventilatory CO<sub>2</sub> removal is optimized due to the reduction of dead space, limiting CO<sub>2</sub> rebreathing, which in turn reduces metabolic load.

The ventilatory assist system and method introduced herein supply ventilatory assist during inspiration via an endotracheal tube structured for delivering a separate, unidirectional inspiratory air flow into the patient's trachea via a first inspiratory tube lumen and a separate, unidirectional expiratory air flow from the patient's trachea through a second expiratory tube lumen. Also, a unidirectional flow of air is produced and maintained through the inspiratory tube lumen and the expiratory tube lumen; in this manner, ventilatory circuit dead space is eliminated, anatomical dead space is substantially reduced and washing out of CO<sub>2</sub> is optimized.

In an aspect, mechanical ventilation may be synchronized with patient's effort to breathe. For example, a physiological breathing signal is used to regulate the ventilatory assist in synchrony with patient's neural inspiration effort, thereby unloading and compensating for weak respiratory muscles.

Turning now to the appended drawings, FIG. 1 is a side cross sectional, partial view of an example of double-lumen endotracheal tube showing intratracheal pulmonary ventilation. A double-lumen endotracheal tube **103** shown on FIG.

**1** forms part of a mechanical ventilator system for delivering air to the lungs **110** of a patient via the trachea **112**. Schematically shown in FIG. **1** are an inspiratory flow in direction **106** toward the patient's lungs **110** and an expiratory flow in direction **107** away from the patient's lungs **110**, through the double-lumen endotracheal tube **103** inserted into the trachea **112**. Direction **106** is shown as a narrow arrow while direction **107** is shown as a thick arrow; this should be understood as a schematic manner of illustrating that the inspiratory flow in direction **106** originates from a smaller-diameter inspiratory tube lumen (also shown in FIG. **3**) while the expiratory flow in direction **107** is directed through a larger-diameter expiratory tube lumen (also shown in FIG. **3**).

FIG. **2** is block diagram of an exemplary pressure control system for use with the double-lumen endotracheal tube of FIG. **1**. FIG. **3** is an example of connection of the double-lumen endotracheal tube of FIG. **1** with the pressure control system of FIG. **2**. Therefore, the following description will refer to FIGS. **2** and **3** concurrently.

An inspiratory air source **100** is connected to an inspiratory line **101** and generates an air pressure, volume or flow to produce a target air flow through the inspiratory line **101**. The inspiratory line **101** is in turn connected to an inspiratory tube lumen **102** of the double-lumen endotracheal tube **103** that is inserted into the patient's trachea **112**. The inspiratory tube lumen **102** may be a single or multiple lumen.

A second lumen of the double-lumen endotracheal tube **103**, hereinafter referred to as an expiratory tube lumen **104**, is connected to an expiratory line **105** connected to a pressure controller **200**. The pressure controller **200** may include a pressure sensor **201** and a valve **202** connected to an exhaust **204**. A similar system for regulating air flow through the expiratory tube lumen **104** and the expiratory line **105** may be used instead of the controller **200** as shown. The pressure controller **200** may be feedback operated to produce and maintain a given pressure in the expiratory tube lumen **104** and the expiratory line **105**. As will be described in more detail in the following description, the valve **202** may be controlled by a physiological breathing signal **250** for synchronizing the air flow through the expiratory tube lumen **104** and the expiratory line **105** with this physiological breathing signal **250**. The pressure controller **200** operates in such a manner that the valve **202** restricts, but does not completely occlude the expiratory line **105** such that a minimum outward air flow remains present in the expiratory tube lumen **104** and the expiratory line **105** during the patient's inspiratory phase. Modulation of the restriction of the air flow through the expiratory tube lumen **104** allows adjustment of the pressure in the respiratory circuit of the mechanical ventilator to be proportional to the physiological breathing signal **250**. A lowest pressure limit may be manually set to ensure sufficient positive end-expiratory pressure (PEEP) to maintain lung recruitment during neural expiration.

More specifically, the inspiratory air source **100** generates a target air flow through the inspiratory line **101** and the inspiratory tube lumen **102**. In turn, the pressure controller **200** regulates a pressure for controlling air flow escaping the trachea **112** and the patient's lungs **110** through the expiratory tube lumen **104** and the expiratory line **105**; more specifically, the pressure controller uses the valve **202** to alter a resistance to air flow of the expiratory tube lumen **104** and expiratory line **105**.

The problem of limiting air flow resistance through the expiratory tube lumen **104** and the expiratory line **105** is

resolved by providing the expiratory tube lumen **104** with a diameter larger than that of the inspiratory tube lumen **102**. The larger resistance to air flow of the smaller-diameter inspiratory tube lumen **102** causes a larger pressure drop. However, the effect of this larger pressure drop is compensated for by using the inspiratory air source **100** to generate a target air flow through the inspiratory tube lumen **102**.

A feedback system **300** between the pressure controller **200** and the inspiratory air source **100** ensures that the target air flow through the inspiratory line **101** and inspiratory tube lumen **102** is adjusted to generate a preset target pressure in the trachea **112**, the expiratory tube lumen **104** and the expiratory line **105**. The feedback system **300** comprises a first comparator **301** and an optional second comparator used as a minimum flow detector **302**. The comparator **301** may receive a target pressure signal from a target pressure adjuster **270**.

The target pressure adjuster **270** is responsive to the physiological breathing signal **250** to adjust the level of a target pressure. The physiological breathing signal **250** is a physiological signal as defined hereinabove. It may be reliably obtained as a measure of the electrical activation of the patient's diaphragm (EAdi), obtained for example using a method as described in U.S. Pat. Nos. 5,671,752, 5,820, 560, 6,588,423 and 6,901,286. The physiological breathing signal **250** may alternatively take the form of an electromyogram (EMG) signal obtained at the level of the alea of the nose (EMG-AN) of the patient, or at the thorax level (EMG-THO) of the patient. Biometric signals from the phrenical nerve of the patient, surface EMG, or measures of chest wall movements of the patient may also be used. Of course any other suitable physiological breathing signal **250** indicative of inspiratory effort including onset detection of the inspiratory effort, before the generation of inspiratory flow occurs, may be used. For example, the target pressure adjuster **270** may increase the level of the target pressure when the level of the physiological breathing signal **250** increases, indicating an increase of the patient's inspiratory effort. In the same manner, the adjuster **270** may decrease the level of the target pressure when the level of the physiological breathing signal **250** decreases, indicating a decrease of the patient's inspiratory effort. In fact, the target pressure may be adjusted by the target pressure adjuster **270** in proportion to the level of patient's inspiratory activity as indicated by the level of the physiological breathing signal **250** or in any other manner beneficial to patient's inspiratory assist. In an embodiment, the target pressure may further be set to ensure sufficient positive end-expiratory pressure (PEEP). Obviously, the target pressure adjuster **270** may also be set at a single level independent of the physiological breathing signal **250**.

Operation of the feedback system **300** follows the following rules:

The target air flow through the inspiratory line **101** and inspiratory tube lumen **102** is increased when the comparator **301** detects that the pressure reading **203** from the pressure sensor **201** of the pressure controller **200**, indicative of the pressure in the trachea **112**, expiratory tube lumen **104** and expiratory line **105** during the patient's inspiration phase is lower than a target pressure, which may be set according to a target pressure signal from the target pressure adjuster **270**. The target air flow through the inspiratory line **101** and inspiratory tube lumen **102** is decreased when the comparator **301** detects that the pressure reading **203** from the pressure sensor **201** of the pressure controller **200**, indicative of the pressure in the trachea **112**,

expiratory tube lumen **104** and expiratory line **105** during the patient's inspiration phase is higher than the target pressure from the target pressure adjuster **270**, and also if it is higher than the manually set PEEP level. Before decreasing the target air flow through the inspiratory line **101** and inspiratory tube lumen **102**, the minimum flow detector **302** ensures that the inspiratory air source **100** maintains a target air flow, through the inspiratory line **101** and inspiratory tube lumen **102**, that is at least equal to or higher than a minimum value. If not, the target air flow through the inspiratory line **101** and inspiratory tube lumen **102** is maintained. The minimum value used in the minimum flow detector **302** for the target air flow is selected to be sufficient to ensure continuous washing out of CO<sub>2</sub>.

Operation of the pressure control system **300** may be synchronized using the physiological breathing signal **250**. More specifically, the valve **202** of the pressure controller **200** will partially close when the physiological breathing signal **250** indicates patient's inspiratory effort to allow the target air flow from the inspiratory line **101** and the inspiratory tube lumen **102** to build up a pressure in the endotracheal tube **103**, the expiratory tube lumen **104** and the expiratory line **105** in order to assist inspiration of the patient. The valve **202** is partially closed to maintain a minimum air flow through the expiratory tube lumen **104** and the expiratory line **105** to contribute to, if not completely eliminate, substantially reduce ventilatory circuit dead space and anatomical dead space, and ensure continuous washing out of CO<sub>2</sub>. When the physiological breathing signal **250** no longer indicates inspiratory effort of the patient, the valve **202** is opened to an extent that allows the patient to expire through the double-lumen endotracheal tube **103**, the expiratory tube lumen **104**, the expiratory line **105**, the valve **202** and the exhaust **204** while maintaining a certain level of expiratory pressure to prevent, for example, collapse of the lungs.

It should be understood that, during both the inspiration and expiration phases, a unidirectional air flow is produced through the inspiratory line **101**, the inspiratory tube lumen **102**, the expiratory tube lumen **104** and the expiratory line **105** to prevent air expired by the patient to be breathed again. In this manner, ventilatory circuit dead space and anatomical dead space are, if not completely eliminated, substantially reduced and continuous washing out of CO<sub>2</sub> is ensured.

In an embodiment, a gain adjuster **260** may alter the physiological breathing signal **250** to adjust the level of the pressure in the trachea **112**, expiratory tube lumen **104** and expiratory line **105**, and thereby adjust the level of ventilatory assistance to the patient. For example, the adjustable gain **260** may be manually set by the medical personnel. Automatic adjustment of the gain **260** may also be contemplated, for example to obtain a target level of ventilatory assistance or physiological breathing signal **250**.

Some options, amongst others, to deliver inspiratory assist to the patient are the following:

A target pressure or volume may be supplied to the patient during inspiration.

As explained in the foregoing description, the target pressure may be adjusted by the target pressure adjuster **270** in proportion to the level of patient's inspiratory activity as indicated by the level of the physiological breathing signal **250** or in any other manner beneficial to patient's inspiratory assist.

A mathematical model may be used for calculating a pressure loss within the endotracheal tube **103** based on

a known air flow resistance and the diameters of the endotracheal tube **103**, the expiratory tube lumen **104** and the expiratory line **105**, and on a measurement of the air flow through these endotracheal tube **103**, the expiratory tube lumen **104** and the expiratory line **105**. The calculated pressure loss may then serve as the target pressure used by the comparator **301**.

Another option is to directly measure a pressure at the free, proximal end of the endotracheal tube **103** inserted into the patient's trachea **112**, near the tracheal bifurcation **150** (FIG. 1), and use this pressure as the target pressure of the comparator **301**.

Oxygen from an oxygen source **356** may be injected in the inspiratory line **101** through a gas mixer **350** to enrich the target air flow through the inspiratory line **101** and inspiratory tube lumen **102**.

To ensure adequate humidification, a humidity sensor (hygrometer) **352** may be used to detect humidity in the expiratory line **105** and, in response to the detected humidity, control a humidifier **354** connected to the gas mixer **350** to humidify, whenever needed, the target air flow through the inspiratory line **101** and the inspiratory tube lumen **102**.

FIG. 4a is a graph of experimental recordings of physiological respiratory parameters illustrating operation of a conventional ventilator system. The graph of FIG. 4a may be compared with the graph of FIG. 4b, which is a graph of experimental recordings of physiological respiratory parameters using the double-lumen endotracheal tube and pressure control system of FIGS. 1 and 2. Both FIGS. 4a and 4b show recordings of air flow (**402a**, **402b**), pressure (**404a**, **404b**), and endtidal carbon dioxide (**406a**, **406b**), measured in the expiratory line **105**. FIGS. 4a and 4b also show recordings of diaphragm electrical activity (EAdi (**408a**, **408b**)).

In the case of FIG. 4a, the air flow is bidirectional (inspiration and expiration) during each breathing cycle. It may be observed that the flow (**402a**) is above a zero line (**403a**) during inspiration phases and below the zero line (**403a**) during expiration phases. This produces a dead space in a breathing tube (not shown) of the conventional ventilator system, corresponding to a volume of an expiratory line and tube lumen. Consequently, a volume of expired air from the lungs is returned to the lungs during the next inspiration.

The graph of FIG. 4b illustrates recordings obtained using the double-lumen endotracheal tube **103** and pressure control system **300** of FIGS. 1 and 2, wherein no air from the expiratory tube lumen **104** and the expiratory line **105** is returned to the patient's lungs **110**. The air flow (**402b**) is unidirectional from the patient's lungs **110** towards the atmosphere and constantly remains below a zero line (**403b**). No volume of expired air from the patient's lungs **110** is returned to the lungs during the next inspiration.

It may be observed that, in FIG. 4b, the endtidal carbon dioxide (**406b**) level is markedly reduced, compared to the corresponding level (**406a**) of FIG. 4a, during respiratory assist with the double-lumen endotracheal tube **103** and pressure control system **300** of FIGS. 1 and 2. It may also be observed that the diaphragm electrical activity (**408b**) and delivered pressure (**404b**) are reduced in FIG. 4b, compared to corresponding readings (**408a**, **404a**) of FIG. 4a, although the ventilator system settings are the same. It may further be observed that generation of the pressure (**404b**) is synchronized with the diaphragm electrical activity (**408b**).

A comparison of the graphs of FIGS. 4a and 4b shows that the double-lumen endotracheal tube **103** and pressure control system **300** of FIGS. 1 and 2 may unload the patient's respiratory muscles by delivering ventilatory assist that is synchronized to the neural inspiratory effort (EAdi (**408b**))

both in terms of timing and pressure generation. Moreover, dead space may be minimized, and the metabolic load may be reduced (lower ETCO<sub>2</sub>, **406b**) thereby further reducing respiratory drive (EAdi (**408b**)).

FIG. 5 is a flow chart of exemplary steps of a ventilatory assist method, capable of reducing neural inspiratory drive of a patient. Steps of a sequence **500** may be applied to a ventilatory assist system disclosed in the foregoing description given in relation to FIGS. 1, 2 and 3. In operation **510**, an air flow is supplied in the inspiration tube lumen **102** of the tube **103** connected to the patient's airways. In response to a physiological signal representative of the patient's inspiratory effort, received in operation **520**, control of the air flow in an expiratory tube lumen **102** of the tube **103** connected to the patient's airway is made in operation **530**. The control made in operation **530** is such that during the patient's inspiratory phase, the air flow through the expiratory tube lumen **104** connected to the patient's airways is partially restricted. In contrast, during the patient's expiratory phase, the air flow is unrestricted to allow expiratory flow from the patient's trachea **112** to evacuate through the endotracheal tube **103**, the expiratory tube lumen **104**, and thereby through the expiratory line **105**.

A result of the control made in operation **530** is that during both the patient's inspiration and expiration phases, a unidirectional air flow is produced through the inspiratory tube lumen **102** and the expiratory tube lumen **104** to prevent air expired by the patient from being breathed again.

Control of the air flow made in operation **530** may for example be made by actuating the valve **202** of FIG. 2.

FIG. 6 is a flow chart of other aspects of the ventilatory assist method of FIG. 5. It should be understood that the operations of the sequence **600** of FIG. 6 may also be applied in a ventilatory assist system as described in connection with the description of FIGS. 1, 2 and 3. More specifically, the sequence **600** comprises:

Operation **610**: A target air flow is produced by the inspiratory air source **100** through the inspiratory tube lumen **101** and the inspiratory line **102**.

Operation **620**: The physiological breathing signal **250** representative of inspiratory effort of the patient is received by the pressure control system **300**.

Operation **630**: The target pressure adjuster **270** adjusts a target pressure in response to the physiological breathing signal **250**.

Operation **640**: Pressure in the endotracheal tube **103**, the expiratory tube lumen **104** and the expiratory line **105** is sensed, or detected, through pressure sensor **201**.

Operation **650**: The target air flow produced by the inspiratory air source **100** in the inspiratory line **101** and the inspiratory tube lumen **102** is adjusted, or controlled, as a function of a comparison by the comparator **301** between the pressure detected in the endotracheal tube **103**, the expiratory tube lumen **104** and the expiratory line **105** and the target pressure from the adjuster **270**.

Operation **660**: The physiological breathing signal **250** is used to control air flow through the expiratory tube lumen **104** and the expiratory line **105** by controlling opening of the valve **202**, thereby altering a pressure in the double-lumen endotracheal tube **103**, the expiratory tube lumen **104** and the expiratory line **105** in synchrony with the patient's inspiratory effort as indicated by the physiological breathing signal **250**. In operation **660**, when the physiological breathing signal **250** indicates an expiratory phase, the valve **202** is opened to an extent to allow the patient to expire through the double-

lumen endotracheal tube 103, the expiratory tube lumen 104, the expiratory line 105, the valve 202 and the exhaust 204 while maintaining a certain level of expiratory pressure to prevent, for example, collapse of the lungs during that expiratory phase.

Operation 670: When the physiological breathing signal 250 indicates an inspiratory phase, the valve 202 will partially close to increase resistance to air flow through the expiratory tube lumen 104 and the expiratory line 105 to allow the target air flow from the inspiratory line 101 and the inspiratory tube lumen 102 to build up a pressure in the endotracheal tube 103, the expiratory tube lumen 104 and the expiratory line 105 in order to assist inspiration of the patient. The valve 202 is partially closed to maintain a minimum air flow through the endotracheal tube 103, the expiratory tube lumen 104 and the expiratory line 105 to contribute to eliminate ventilatory circuit dead space and substantially reduce anatomical dead space, and ensure continuous washing out of CO<sub>2</sub>.

Those of ordinary skill in the art will realize that the description of the devices and methods for patient-synchronized ventilatory assist are illustrative only and are not intended to be in any way limiting. Other embodiments will readily suggest themselves to such persons with ordinary skill in the art having the benefit of the present disclosure. Furthermore, the disclosed patient-synchronized ventilatory assist may be customized to offer valuable solutions to existing needs and problems of ventilatory assist systems.

In the interest of clarity, not all of the routine features of the implementations of patient-synchronized ventilatory assist systems and methods are shown and described. It will, of course, be appreciated that in the development of any such actual implementation of the patient-synchronized ventilatory assist systems and methods, numerous implementation-specific decisions may need to be made in order to achieve the developer's specific goals, such as compliance with application-, system- and business-related constraints, and that these specific goals will vary from one implementation to another and from one developer to another. Moreover, it will be appreciated that a development effort might be complex and time-consuming, but would nevertheless be a routine undertaking of engineering for those of ordinary skill in the field of ventilatory assist systems having the benefit of the present disclosure.

In accordance with the present disclosure, the components, process steps, and/or signal structures described herein may be implemented using various types of operating systems, computing platforms, network devices, computer programs, and/or general purpose machines. In addition, those of ordinary skill in the art will recognize that devices of a less general purpose nature, such as hardwired devices, field programmable gate arrays (FPGAs), application specific integrated circuits (ASICs), or the like, may also be used. Where a method comprising a series of process steps is implemented by a computer or a machine and those process steps may be stored as a series of instructions readable by the machine, they may be stored on a tangible medium.

Systems and modules described herein may comprise software, firmware, hardware, or any combination(s) of software, firmware, or hardware suitable for the purposes described herein. Software and other modules may reside on servers, workstations, personal computers, computerized tablets, personal digital assistants (PDA), and other devices suitable for the purposes described herein. Software and other modules may be accessible via local memory, via a

network, via a browser or other application or via other means suitable for the purposes described herein. Data structures described herein may comprise computer files, variables, programming arrays, programming structures, or any electronic information storage schemes or methods, or any combinations thereof, suitable for the purposes described herein.

Although the present disclosure has been described hereinabove by way of non-restrictive, illustrative embodiments thereof, these embodiments may be modified at will within the scope of the appended claims without departing from the spirit and nature of the present disclosure.

What is claimed is:

1. A ventilatory assist system, comprising:

a tube for connection to a patient's airway, the tube including (a) an inspiratory tube lumen with a proximal end in fluid communication with the patient's airway and a distal end, and (b) an expiratory tube lumen with a proximal end in fluid communication with the patient's airway and the proximal end of the inspiratory tube lumen, and a distal end in fluid communication with an exhaust;

an inspiratory air source connected to the distal end of the inspiratory tube lumen for supplying air flow to the inspiratory tube lumen; and

a pressure controller connected to the expiratory tube lumen and using a physiological breathing signal having a level indicative of an inspiratory effort of the patient to indicate expiration and inspiration phases of the patient during breathing cycles of the patient to establish, during each of the breathing cycles, (a) an expiratory pressure in the expiratory tube lumen during the patient's expiration phase to allow patient's expiration through the expiratory tube lumen while producing a first unidirectional air flow from the inspiratory air source through the inspiratory tube lumen, the expiratory tube lumen and the exhaust, and (b) an inspiratory assist pressure in the expiratory tube lumen during the patient's inspiration phase to allow the inspiratory air source to provide ventilatory assist to the patient through the inspiratory tube lumen and the patient's airway while producing a second unidirectional air flow from the inspiratory air source through the inspiratory tube lumen, the expiratory tube lumen and the exhaust;

wherein the first and second unidirectional air flows prevent air expired by a patient from being breathed again; and

wherein the pressure controller uses the physiological breathing signal to synchronize the expiratory pressure and the inspiratory assist pressure with the expiration and inspiration phases of the breathing cycles of the patient.

2. The ventilatory assist system of claim 1, wherein:

the pressure controller comprises a valve disposed between the distal end of the expiratory tube lumen and the exhaust, and controlled using the physiological breathing signal.

3. The ventilatory assist system of claim 2, wherein:

the valve is partially closed during the patient's inspiration phase to establish the inspiratory assist pressure while producing the second unidirectional air flow.

4. The ventilatory assist system of claim 1, wherein:

the physiological breathing signal is a measure of electrical activation of a patient's diaphragm (EAdi).

5. The ventilatory assist system of claim 1, further comprising:

## 11

- a pressure sensor for sensing a pressure in the expiratory tube lumen; and  
 a feedback system interposed between the pressure sensor and the inspiratory air source.
6. The ventilatory assist system of claim 5, wherein: 5  
 the feedback system comprises a comparator of the pressure sensed by the pressure sensor in the expiratory tube lumen to a target pressure.
7. The ventilatory assist system of claim 6, comprising: 10  
 a target pressure adjuster for setting the target pressure in response to the physiological breathing signal.
8. The ventilatory assist system of claim 6, wherein: 15  
 the inspiratory air source is adapted to increase an air flow through the inspiratory tube lumen in response to a detection by the comparator that the pressure sensed by the pressure sensor in the expiratory tube lumen is lower than the target pressure.
9. The ventilatory assist system of claim 5, wherein: 20  
 the feedback system comprises a minimum flow detector for maintaining at least a minimum air flow through the inspiratory tube lumen.
10. The ventilatory assist system of claim 9, wherein: 25  
 the inspiratory air source is adapted to maintain at least the minimum air flow in response to a signal from the minimum flow detector.
11. The ventilatory assist system of claim 1, wherein: 30  
 the tube is an endotracheal tube.
12. The ventilatory assist system of claim 1, wherein: 35  
 the inspiratory tube lumen is a smaller-diameter tube lumen and the expiratory tube lumen is a larger-diameter tube lumen.
13. The ventilatory assist system of claim 1, comprising: 40  
 a gas mixer connected between the inspiratory air source and the distal end of the inspiratory tube lumen.
14. The ventilatory assist system of claim 13, comprising: 45  
 an oxygen source connected to the gas mixer.
15. The ventilatory assist system of claim 13, comprising: 50  
 a hygrometer connected to the expiratory tube lumen; and a humidifier controlled by the hygrometer and connected to the gas mixer.
16. The ventilatory assist system of claim 1, comprising: 55  
 a gain adjuster interposed between a source of the physiological breathing signal and the pressure controller for adjusting a level of ventilatory assist to the patient.
17. The ventilatory assist system of claim 1, wherein the 60  
 pressure controller is responsive to the physiological breathing signal to establish the expiratory pressure in the expiratory tube lumen in proportion to the patient's inspiratory effort.
18. A ventilatory assist method, comprising: 65  
 connecting a tube to a patient's airway, the tube including (a) an inspiratory tube lumen with a proximal end in fluid communication with the patient's airway and a

## 12

- distal end, and (b) an expiratory tube lumen with a proximal end in fluid communication with the patient's airway and the proximal end of the inspiratory tube lumen, and a distal end in fluid communication with an exhaust;
- supplying an air flow to the distal end of the inspiratory tube lumen; and
- using a physiological breathing signal having a level indicative of an inspiratory effort of the patient to indicate expiration and inspiration phases of the patient during breathing cycles of the patient, establishing during of the each breathing cycles (a) an expiratory pressure in the expiratory tube lumen during the patient's expiration phase to allow patient's expiration through the expiratory tube lumen and the exhaust while producing a first unidirectional air flow through the inspiratory tube lumen, the expiratory tube lumen and the exhaust, and (b) an inspiratory assist pressure in the expiratory tube lumen during the patient's inspiration phase to provide ventilatory assist to the patient through the inspiratory tube lumen and the patient's airway while producing a second unidirectional air flow through the inspiratory tube lumen, the expiratory tube lumen and the exhaust;
- wherein the first and second unidirectional air flows prevent air expired by a patient from being breathed again; and
- wherein the expiratory pressure and the inspiratory assist pressure are synchronized with the expiration and inspiration phases of the breathing cycles of the patient.
19. The method of claim 18, comprising: 75  
 sensing a pressure in the expiratory tube lumen; and adjusting the air flow in the inspiratory tube lumen based on a comparison between the pressure sensed in the expiratory tube lumen and a target pressure.
20. The method of claim 19, wherein: 80  
 adjusting the air flow in the inspiratory tube lumen comprises increasing the air flow in the inspiratory tube lumen when the pressure sensed in the expiratory tube lumen is lower than the target pressure and decreasing the air flow in the inspiratory tube lumen when the pressure sensed in the expiratory tube lumen is higher than the target pressure.
21. The method of claim 19, comprising: 85  
 adjusting the target pressure based on the physiological breathing signal.
22. The method of claim 18, wherein the expiratory pressure in the expiratory tube lumen is established in proportion to the patient's inspiratory effort.

\* \* \* \* \*

|                |                                                                                                                                                                                                                                                                                                                                          |         |            |
|----------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------|------------|
| 专利名称(译)        | 用于患者同步通气辅助与气管内通流的方法和系统                                                                                                                                                                                                                                                                                                                   |         |            |
| 公开(公告)号        | <a href="#">US9968750</a>                                                                                                                                                                                                                                                                                                                | 公开(公告)日 | 2018-05-15 |
| 申请号            | US13/806816                                                                                                                                                                                                                                                                                                                              | 申请日     | 2011-06-29 |
| [标]申请(专利权)人(译) | BECK JENNIFER<br>SINDERBY CHRISTER                                                                                                                                                                                                                                                                                                       |         |            |
| 申请(专利权)人(译)    | BECK , JENNIFER<br>SINDERBY , CHRISTER                                                                                                                                                                                                                                                                                                   |         |            |
| 当前申请(专利权)人(译)  | ST.米高医院                                                                                                                                                                                                                                                                                                                                  |         |            |
| [标]发明人         | SINDERBY CHRISTER<br>BECK JENNIFER                                                                                                                                                                                                                                                                                                       |         |            |
| 发明人            | SINDERBY, CHRISTER<br>BECK, JENNIFER                                                                                                                                                                                                                                                                                                     |         |            |
| IPC分类号         | A61M16/00 A61M16/16 A61M16/04 A61B5/087 A61B5/0488 A61B5/00 A61M16/20 A61M16/10<br>A61M16/12                                                                                                                                                                                                                                             |         |            |
| CPC分类号         | A61M16/0003 A61B5/087 A61B5/4836 A61M16/00 A61M16/0012 A61M16/0051 A61M16/0069 A61M16/<br>/04 A61M16/042 A61M16/0486 A61M16/1005 A61M16/12 A61M16/125 A61M16/161 A61M16/202<br>A61M16/205 A61B5/0488 A61M2230/60 A61M16/024 A61M16/16 A61M2016/0018 A61M2016/0021<br>A61M2016/0027 A61M2016/0033 A61M2202/0208 A61M2210/1014 A61M2230/08 |         |            |
| 助理审查员(译)       | BOECKER , JOSEPH D                                                                                                                                                                                                                                                                                                                       |         |            |
| 优先权            | 61/359951 2010-06-30 US                                                                                                                                                                                                                                                                                                                  |         |            |
| 其他公开文献         | US20140305434A1                                                                                                                                                                                                                                                                                                                          |         |            |
| 外部链接           | <a href="#">Espacenet</a> <a href="#">USPTO</a>                                                                                                                                                                                                                                                                                          |         |            |

## 摘要(译)

公开了一种通气辅助系统和方法。该系统包括用于连接到患者气道的管，连接到管的吸气和呼气管腔，连接到吸气管腔的吸气空气源，以及呼气管腔中的气压控制器。压力控制器响应于代表患者吸气努力的生理呼吸信号，以允许空气在患者的呼气阶段期间流过呼气管腔，部分地限制通过呼气管腔的气流到患者吸气期间的最小气流。相。在两个呼吸阶段期间，通过吸气和呼气管腔产生单向气流，以防止患者呼出的空气再次呼吸。生理呼吸信号允许通气辅助与患者的呼吸努力同步。

