



US 20030125613A1

(19) **United States**(12) **Patent Application Publication**
Enegren et al.(10) **Pub. No.: US 2003/0125613 A1**(43) **Pub. Date: Jul. 3, 2003**(54) **IMPLANTABLE SENSOR FLUSH SLEEVE****Publication Classification**(75) Inventors: **Bradley J. Enegren**, Moorpark, CA
(US); **Marianne A. Kolopp**, Valencia,
CA (US)(51) **Int. Cl.⁷** **A61B 5/05**(52) **U.S. Cl.** **600/347**

Correspondence Address:

MEDTRONIC MINIMED INC.
18000 DEVONSHIRE STREET
NORTHRIDGE, CA 91325-1219 (US)(73) Assignee: **MEDTRONIC MINIMED, INC.**(21) Appl. No.: **10/034,740**(22) Filed: **Dec. 27, 2001**(57) **ABSTRACT**

A apparatus and method for cleaning a sensor tip of an implantable sensor includes a flush sleeve directed towards the sensor tip, a fluid conduit in fluid communication with the flush sleeve, where fluid injected into a first end of a flush sleeve surrounding the sensor sprays off the sensor tip through at least one orifice located at the second end of the flush sleeve. The first end of the flush sleeve contains a fluid conduit and a septum, where a needle is used to pierce the septum to inject the fluid into the fluid conduit.

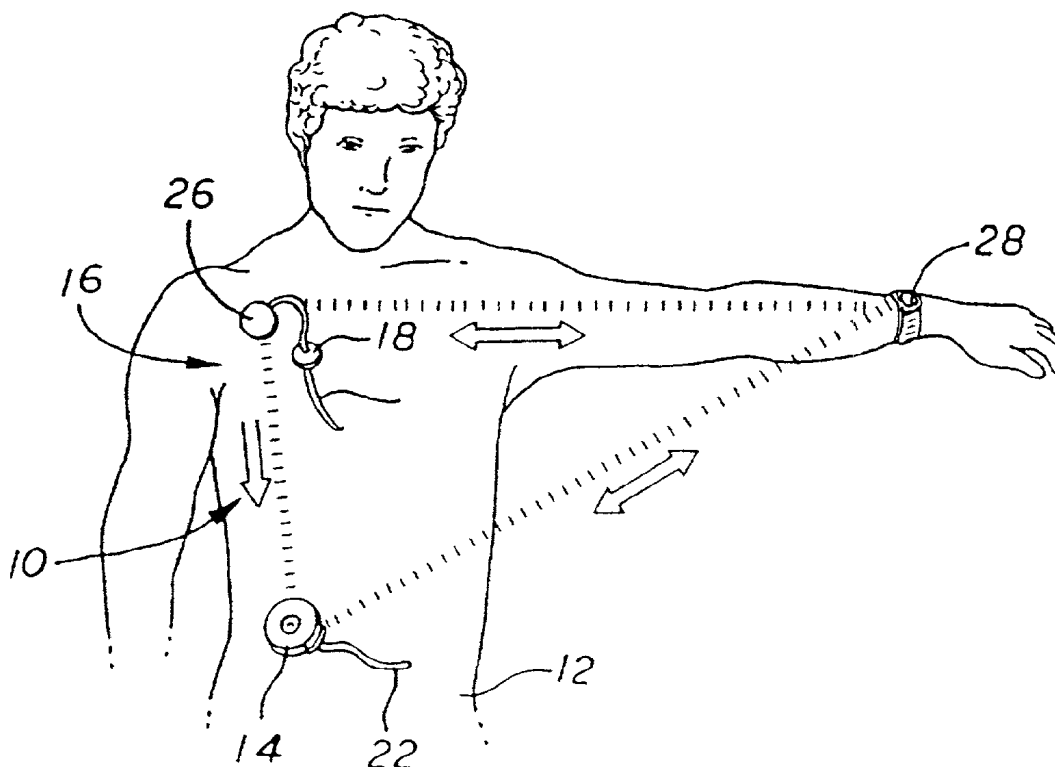


FIG 1


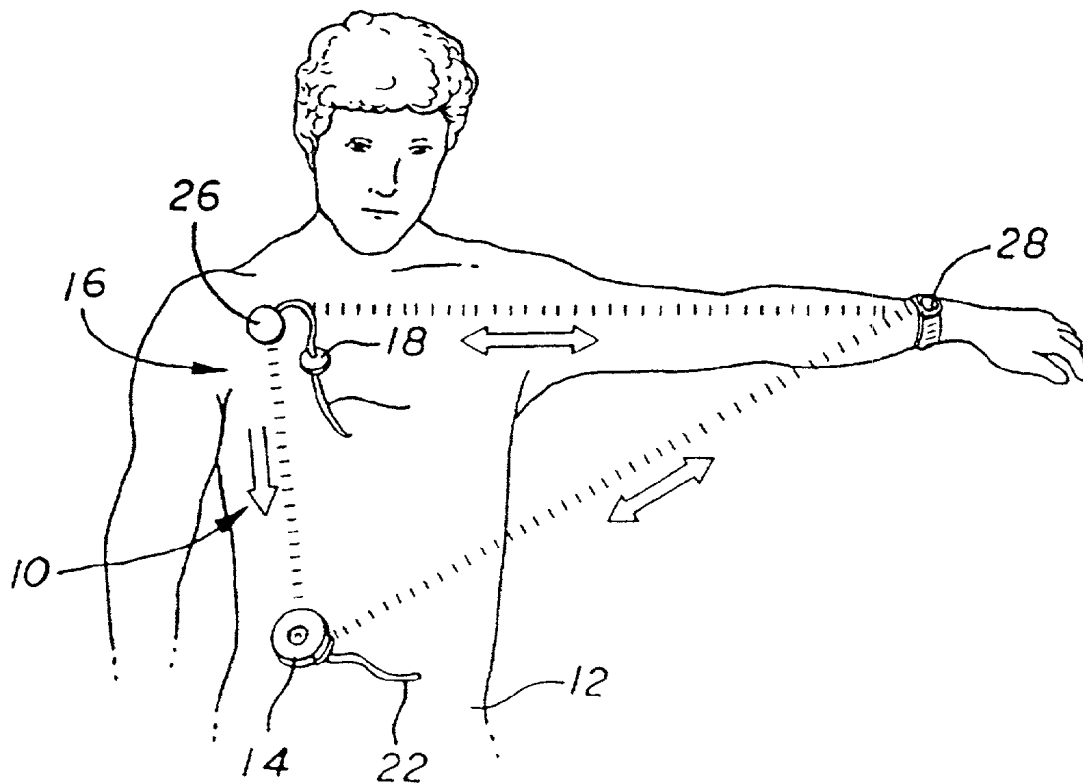


FIG. 2

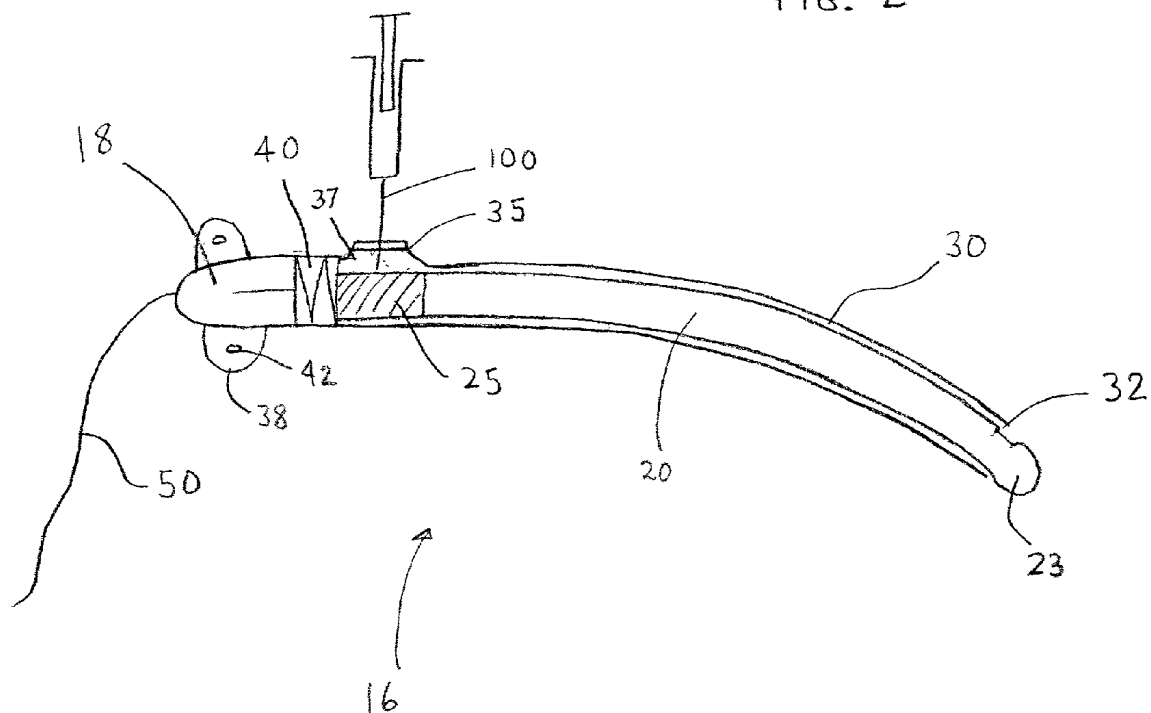

IMPLANTABLE SENSOR FLUSH SLEEVE

BACKGROUND OF THE INVENTION

[0001] 1. Field of the Invention

[0002] The present invention relates generally to implantable sensors. More specifically, the present invention relates to an implantable glucose sensor with cleaning features.

[0003] 2. Discussion of the Related Art

[0004] Recently, implantable glucose sensors for monitoring glucose concentration level in a patient fluid, such as blood, have been developed. These implantable or in vivo glucose sensors are designed to provide instantaneous reading of patient glucose concentration, where the tip of the glucose sensor is placed within a major blood vessel. Examples of some glucose sensors include U.S. Pat Nos. 4,650,547, 4,671,288, 4,781,798, 4,703,756, and 4,890,620. These implantable glucose sensors can be used in conjunction with an infusion pump system to deliver selected medication, such as insulin, to a patient in a scheduled or preprogrammed manner, including implantable infusion pumps to deliver insulin to the patient in discrete doses over an extended period of time.

[0005] However, a potential problem with implantable glucose sensors is that they can have a relatively short life span, often in the order of a few months. This stems from the fact that the implantable glucose sensors are located in a highly volatile environment, such as a large artery, and the human body tends to attack any foreign object placed in the body. Thus, clotting agents in the blood tend to cover and diminish the effectiveness of the sensor with the passage of time. In addition, the sensor can also be covered by proteins, fats, or other substances while the sensor is contact with human blood reducing the life of the sensors.

SUMMARY OF THE INVENTION

[0006] Accordingly, embodiments of the present invention are directed to a sensor apparatus and method with the added capability of a cleaning feature that substantially obviates one or more problems due to limitations and disadvantages of the related art.

[0007] Embodiments are directed to an implantable sensor apparatus for taking readings from a patient in vivo. The implantable sensor apparatus includes an implantable sensor, a flush sleeve, and a fluid conduit. The implantable sensor has a distal end with a sensor tip for direct contact with patient fluids. The flush sleeve is directed towards the sensor tip, and fluid received in the fluid conduit is used to spray the sensor tip, where the fluid conduit is in fluid communication with the flush sleeve. In additional embodiments, the implantable sensor also contains a connector fitting for supporting the implantable sensor within the patient.

[0008] In further embodiments, the fluid conduit contains a septum, where a needle is used to pierce the septum to inject the fluid into the fluid conduit. In still further embodiments, the flush sleeve surrounds the implantable sensor in a tight fit connection, and the flush sleeve contains at least one one-way valve near the sensor tip.

[0009] Further embodiments are directed to a method of cleaning a sensor tip of an implantable sensor. The method

includes the steps of injecting fluid into a first end of a flush sleeve surrounding the sensor and spraying off the sensor tip with the injected fluid through at least one orifice located at the second end of the flush sleeve. In further embodiments, the first end of the flush sleeve contains a fluid conduit and a septum, and a needle is used to pierce the septum to inject the fluid into the fluid conduit.

[0010] It is to be understood that both the foregoing general description and the following detailed description of the present invention are exemplary and explanatory and are intended to provide further explanation of the invention as claimed.

BRIEF DESCRIPTION OF THE DRAWINGS

[0011] A detailed description of embodiments of the invention will be made with reference to the accompanying drawings, wherein like numerals designate corresponding parts in the several figures.

[0012] **FIG. 1** is a schematic diagram illustrating a human environment in which preferred embodiments are implemented; and

[0013] **FIG. 2** is a cross-sectional view of the glucose sensor in accordance with the preferred embodiments of the present invention.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0014] Embodiments of the present invention are directed to implantable sensors that measure a characteristic of a patient's body. In preferred embodiments, the characteristic is the glucose level, and the implantable sensor is placed in an artery or a vein. Although embodiments of the present invention are primarily described in the context of glucose sensors used in the treatment of diabetes, the embodiments of the invention are applicable to a wide variety of patient treatment programs where a physiological characteristic is monitored. For example, embodiments of the invention can be used to determine the status and/or levels of a variety of characteristics including those associated with agents such as hormones, cholesterol, medication concentrations, pH, oxygen saturation, viral loads (e.g., HIV), or the like. Also embodiments of the present invention are not limited to implantation in an artery or vein, but can be implanted in and/or through subcutaneous, dermal, sub-dermal, interperitoneal or peritoneal tissue. Such sensors typically communicate a signal from the implantable sensor to either an internal or external monitor. The implantable sensor is primarily adapted for use with blood. However, still further embodiments of the implantable sensor may be used in other bodily fluids, such as interstitial fluid, spinal fluid, saliva, urine, tears, sweat, or the like.

[0015] **FIG. 1** is a schematic diagram illustrating a human environment in which preferred embodiments are implemented. As shown in **FIG. 1**, the preferred embodiments of the present invention are designed to be used with an infusion device system referred to generally in **FIG. 1** by the reference numeral **10** to deliver selected medication to a patient **12**. The system **10** generally includes an infusion device **14**, which responds to control signals to deliver the fluids, such as, but not limited to, saline, drugs, vitamins, medication, proteins, peptides, insulin, neural transmitters,

or the like, as needed to the patient. Embodiments of the present invention can utilize the infusion device **14** with an implantable sensor unit **16** in a closed-loop system. Alternatively, the implantable glucose sensor unit **16** may be used in an open loop system or alone to just monitor a condition of a patient.

[0016] In the preferred embodiments, the sensor unit **16** monitors patient glucose concentration level on a continuous, near-continuous or intermittent basis to provide appropriate control signals for the infusion device **14**. Selected fluid, such as insulin for a diabetic patient, may then be administered to the patient in response to actual patient requirements as represented by a glucose measurement taken by the implantable sensor unit **16**.

[0017] In accordance with an aspect of the invention, the sensor unit **16** includes a subcutaneously mounted connector fitting **18** for anchoring an in vivo glucose sensor **20** in a manner permitting convenient sensor removal and replacement. A connector fitting **18** provides a relatively simple and easily accessed structure for coupling the glucose sensor **20** with other system components, while permitting access to the glucose sensor **20** for removal and replacement. Although in the preferred embodiments, the infusion device **14** is also implanted within the patient **12** to form a closed-loop system, the sensor unit **16** can be used alternatively with external infusion device in a closed loop system and/or other open-loop systems. One example of a connector fitting **18** is disclosed in U.S. Pat. No. 5,569,186, entitled "Closed Loop Infusion Pump System With Removable Glucose Sensor," which is herein incorporated by reference. In alternative embodiments, other connection methods, such as, but not limited to, those utilized with pacemakers and/or pacemaker leads may be used.

[0018] In a preferred system arrangement, as viewed in FIG. 1, the infusion device **14** includes a small and substantially self-contained unit adapted for direct implantation into the body of the patient **12**. The infusion device **14** includes a hermetically sealed infusion device housing constructed typically from a biocompatible material, such as, but not limited to, titanium or titanium alloy, and defining an internal fluid reservoir chamber for receiving and storing a supply of the selected fluid in liquid form, such as, but not limited to, insulin for a diabetic patient. In alternative embodiments, the infusion device housing may be formed out of other materials, such as, but not limited to, metal, ceramic, composites, glass, plastics, laminates, combinations, or the like, that are suitable for implantation in a patient. Embodiments of the infusion device housing may further encase a miniature dispensing pump and associated electronic control circuitry in combination with a battery power supply for operating the pump to deliver fluid doses to the patient via an appropriate catheter **22**, or the like. In preferred embodiments, the control circuitry is suitably programmed and operated to deliver the fluid in accordance with individual patient need, including but not limited to providing insulin in a closed loop in response to glucose concentration measurement. In addition, preferred embodiments of the infusion device housing are designed to permit percutaneous refilling of the internal fluid reservoir without requiring surgical access to the implanted infusion device. For a more detailed description of the overall construction and operation of possible embodiments of implantable infu-

sion devices of this general type, see U.S. Pat. Nos. 4,373,527 and 4,573,994, which are incorporated by reference herein.

[0019] As seen in FIG. 1, the sensor unit **16** is implanted within the patient **12** at a selected position for placement of the glucose sensor **20** in contact with a patient fluid, such as in intimate contact with patient blood within a cephalic vein. In alternative embodiments, other implantation sites, as discussed above, may be used. The connector fitting **18** is located at a convenient subcutaneous site for relatively easy palpable identification, and the sensor **20** extends from the connector fitting to a distal end positioned at a selected in vivo sensor position. In the preferred embodiments, a telemetry unit **26** (FIG. 1) is coupled to the connector fitting **18** through a cable **50** and functions to transmit glucose measurement signal information by means of radio telemetry. As viewed in FIG. 1, the telemetry unit **26** can transmit the glucose measurement information to the infusion device **14** for closed loop operation, or alternately to an externally located monitor **28**. FIG. 1 illustrates the monitor **28** in the form of a wrist-worn device, although it will be understood that the monitor **28** may take other convenient forms, such as, but not limited to, an external infusion device. As is known in the art, the monitor **28** can be manipulated in response to information received and/or displayed to control infusion device operation through the use of radio telemetry signals. For instance, but not limited to, the monitor **28** may be programmed to automatically adjust infusion device operation according to glucose measurements, to recommend a treatment program to allow patient verification and manual initiation, or to simply display the glucose readings and permit manual entry of reprogramming commands.

[0020] Alternatively, instead of a telemetry unit **26**, the cable **50** can be connected directly to the control unit or circuit disposed internally within the implanted infusion device **14**. With this system, radio telemetry transfer of glucose measurement information to the infusion device **14** is unnecessary. Instead, the information is transmitted directly through the use of the cable **50**. Once again, the external monitor **28** may be used to read out or reprogram the infusion device **14** as previously described.

[0021] As shown in FIG. 1, the connector fitting **18** provides a convenient and relatively simple structure for anchoring the proximal end of the sensor **20** in electrical coupled relation with the telemetry unit **26**. More particularly, the connector fitting **18** is mounted at the proximal end of the sensor **20** through a plug-in connector **40**. In the preferred embodiments, the plug-in connector **40** is similar to a jack/plug combination, but alternatively, the plug-in connector **40** can be a Luer lock constructed at the proximal end of the sensor **20**. In this position, the proximal end of the sensor **20** is seated and retained within the connector fitting **18**. Embodiments of the connector fitting **18** may also include radially enlarged flanges **38** (or butterfly wings **38**) having suture ports **42** formed to facilitate anchored connection of the fitting by sutures, or the like, to the subcutaneous muscle fascia. Thus, the butterfly wings **38** help assure that sensor **20** will stay in the appropriate location.

[0022] FIG. 2 is a cross-sectional view of the glucose sensor **20** in accordance with the preferred embodiments of the present invention. The glucose sensor **20** generally includes, in one preferred form, an improved implantable

enzyme electrode of the general type described in U.S. Pat. Nos. 4,650,547; 4,671,288; 4,781,798; 4,703,756; and 4,890,620, which are incorporated by reference herein. Such enzyme electrodes include an elongated sensor **20** having a distal end defining a sensor tip **23** for direct contact with patient fluids, such as blood. The sensor tip **23** defines a conductivity sensor for measuring fluid conductivity changes in response to an enzymatic reaction typically involving the use of glucose oxidase to catalyze glucose in the presence of oxygen (O₂). Conductivity signals are transmitted through the sensor **20** via conductors to a proximal end of the sensor **20**.

[0023] In alternative embodiments, different sensors technology may be used, such as, but not limited to an optical sensor. Preferably, an the implantable optical sensor would include a photo-reactive substance or compound that optically changes, fluoresces, or the like, or other suitable compounds that detect changing properties in the presence of a bodily fluid analyte, such as glucose or the like. The compounds can also be used to detect the level of an analyte that has been ingested, injected or placed inside the body, such as marker substances, or the like. For example, possible compounds, including but not limited to, produce a fluorescent change in the presence of a bodily fluid analyte are disclosed in U.S. Pat. No. 5,503,770 issued Apr. 2, 1996 to James et al. and entitled "Fluorescent Compound Suitable For Use In The Detection Of Saccharides"; U.S. Pat. No. 5,512,246 issued Apr. 30, 1996 to Russell et al. and entitled "Method and Means for Detecting Polyhydroxyl Compounds"; U.S. Provisional Application Serial No. 60/007,515 to Van Antwerp et al. and entitled "Minimally Invasive Chemically Amplified Optical Glucose Sensor"; and U.S. Pat. No. 6,011,984 to Van Antwerp et al. and entitled "Detection of Biological Molecules Using Chemical Amplification", all of which are herein incorporated by reference. Other compounds using Donor Acceptor fluorescent techniques may be used, such as disclosed in U.S. Pat. No. 5,628,310 issued May 13, 1997 to Rao et al. and entitled "Method and Apparatus to Perform Trans-cutaneous Analyte Monitoring"; U.S. Pat. No. 5,342,789 issued Aug. 30, 1994 to Chick et al. and entitled "Method and Device for Detecting and Quantifying Glucose in body Fluids"; and U.S. Pat. No. 5,246,867 issued Sep. 21, 1993 to Lakowicz et al. and entitled "Determination and Quantification of Saccharides by Luminescent Lifetimes and Energy Transfer", all of which are herein incorporated by reference.

[0024] As shown in FIG. 2, in accordance with the preferred embodiments, the implantable sensor **20** includes a flush sleeve **30** in a tight fit connection surrounding the sensor **20**, which allows fluid communication along the length of the sensor **20**. Around the sensor tip **23**, the flush sleeve **30** contains a small orifice **32**, which comprises a one-way valve, to allow fluid to spray off the sensor tip **23**. More than one orifice **32** can be placed at the distal end of the flush sleeve **30** to direct fluid to different locations of the sensor tip **23**. Alternatively, the flush sleeve may be an elastomeric cover, such as, but not limited to, rubber, plastic, silicone, polyurethane, polystyrene, or the like, that fits tightly around the sensor **20**. When fluid is introduced into the flush sleeve, the flush sleeve expands under pressure so that the surrounding edge of the flush sleeve near the sensor tip separates from the sensor **20** to form at least one orifice **32** to permit the fluid to spray over the sensor tip. The edge of the sleeve may be configured and/or tailored to provide

specific spray patterns, multiple orifices, selective openings, or the like, with the configuration being dependent on the type of environment where the sensor is implanted, the type of deposits to be removed, and the type of sensor.

[0025] In preferred embodiments, the flush sleeve **30** is in fluid communication with a fluid conduit **37** formed at the proximal end of the sensor **20**. Fluid can be introduced into the fluid conduit **37** by means of a non-coring "huber" style needle **100**, where the needle **100** introduces fluid through a septum **35**. The septum **35** provides the needle **100** access to the fluid conduit **37**, while providing a seal to substantially inhibit the incursion of external contaminants, such as bacteria, debris, or the like. This reduces the likelihood of developing an infection through contact with the external environment. In further embodiments, the septum **35** and fluid conduit **37** may include an anti-bacterial agent on the interior surface of the septum **35**, or actually formed as an integral part of the septum **35** and conduit **37** material, to further minimize the chance of an infection. The combination of the septum **35** and the fluid conduit **37** acts as a syringe port, guiding the needle **100** to the flush sleeve **30**. In the fluid conduit **37**, the sensor **20** is surrounded by protector sleeve **25**, which protects the sensor **25** and acts as a backstop to the needle **100**. In preferred embodiments, the protector sleeve is made from titanium, although other material can be used to manufacture the protector sleeve. In alternative embodiments, other types of needles may be used, and the septum may be replaced or augmented with an input valve. In still other embodiments, the fluid conduit is eliminated and formed as an integral part of the flush sleeve.

[0026] In addition, certain embodiments may taper the ends of the flush sleeve **30** to improve the spraying process. The tapered ends would increase the pressure of the fluid out of the one or more orifices **32**, and better direct the ejected fluid towards the surface of the sensor tip **23**.

[0027] In use, fluid is injected into the fluid conduit **37** through the septum **35** using the needle **100**. The fluid travels through the flush sleeve **30** and ejected out of the orifice **32**. The fluid is used to clean the surface of the sensor tip **23** by knocking off any buildup of clots, encapsulation tissue, biological deposits, other debris, or the like, from the sensor tip **23**. By cleaning the surface of the sensor tip **23**, the readings by the sensor **20** can be restored, more accurate, and the life of the sensor **20** may be extended. In preferred embodiments, the fluid is a saline solution, but alternatively, the fluid can contain an anti-coagulant. A fluid that contains an anti-coagulant may assist in dissolving off the clots and/or biological deposits as well as spraying off the sensor tip **23**.

[0028] In another use, the sensor **20** may change position over time, such that the sensor tip **23** is no longer in an optimal position. In this case, the injection of the fluid into the flush sleeve can also be used to reposition the sensor tip **23**, as the fluid is injected from the orifice **32**, by thrusting the sensor tip **23** away from the non-optimal position.

[0029] In preferred embodiments, the sensor **20**, flush sleeve **30** and the connector fitting **18** are formed from a suitable medical-grade plastic, metal, glass, composites or the combination thereof that is bio-compatible. However, in alternative embodiments, the sensor **20**, flush sleeve, and the connector fitting **18** are formed out of other suitable materials.

Additional Implementation Details

[0030] This concludes the description of the preferred embodiments of the invention. The following describes some alternative embodiments for accomplishing the present invention. The preferred embodiments were described in terms of flush sleeve 30 defining a flush channel around the sensor 20. In alternative embodiments, a separate catheter can be used to direct fluid at the sensor tip to remove the biological deposits. In addition, although preferred embodiments described an enzyme oxidase sensor to detect glucose levels, the sensor may be a different type of sensor using different technology and/or detecting other biological readings. Moreover, although the preferred embodiments described the infusion device, connector fitting, and sensor as separate components, the connector fitting may be provided as part of an integrated unit including the infusion device, where the sensor is disconnectable from the pump for removal and replacement, if desired.

[0031] Thus, the foregoing description of the preferred embodiments of the invention has been presented for the purposes of illustration and description. It is not intended to be exhaustive or to limit the invention to the precise form disclosed. Many modifications and variations are possible in light of the above teaching. It is intended that the scope of the invention be limited not by this detailed description, but rather by the claims appended hereto. The above specification, examples and data provide a description of the manufacture and use of the composition of the invention. Since many embodiments of the invention can be made without departing from the spirit and scope of the invention, the invention resides in the claims hereinafter appended.

What is claimed is:

1. An implantable sensor apparatus for taking readings from a patient in vivo, the sensor apparatus comprising:

an implantable sensor having a distal end with a sensor tip for direct contact with patient fluids;

a flush sleeve directed towards the sensor tip; and

a fluid conduit in fluid communication with the flush sleeve, wherein a fluid received in the fluid conduit in fluid communication with the flush sleeve is used to spray the sensor tip.

2. The sensor apparatus of claim 1, further comprising a connector fitting for supporting the implantable sensor within the patient.

3. The sensor apparatus of claim 1, wherein the fluid conduit contains a septum, and wherein a needle is used to pierce the septum to inject the fluid into the fluid conduit.

4. The sensor apparatus of claim 1, wherein the flush sleeve surrounds the implantable sensor in a tight fit connection.

5. The sensor apparatus of claim 4, wherein the flush sleeve contains at least one one-way valve near the sensor tip.

6. The sensor apparatus of claim 1, wherein the fluid conduit is located at a proximal end of the sensor.

7. The sensor apparatus of claim 6, wherein the proximal end of the sensor is covered by a protector sleeve.

8. The sensor apparatus of claim 1, wherein the sensor is plugged into the connector fitting, and the connector fitting is affixed internally to the patient.

9. The sensor apparatus of claim 1, wherein the fluid is a saline solution.

10. The sensor apparatus of claim 1, wherein the fluid contains an anti-coagulant.

11. The sensor apparatus of claim 1, wherein the connector fitting is connected to a telemetry unit to transmit readings from the implantable sensor.

12. A method of cleaning a sensor tip of an implantable electrode sensor having the sensor tip in direct contact with patient fluid, the method comprising the steps of:

injecting fluid into a first end of a flush sleeve surrounding the sensor; and

spraying off the sensor tip with the injected fluid through at least one orifice located at a second end of the flush sleeve.

13. The method of claim 12, wherein the first end of the flush sleeve contains a fluid conduit and a septum, and wherein a needle is used to pierce the septum to inject the fluid into the fluid conduit.

14. The method of claim 12, wherein the flush sleeve surrounds the implantable sensor in a tight fit connection.

15. The method of claim 14, wherein the flush sleeve contains at least one one-way valve near the sensor tip.

16. The method of claim 14, wherein the portion of the sensor in contact with the first end of the flush sleeve is covered by a protector sleeve.

17. The method of claim 12, wherein the sensor is plugged into a connector fitting, and the connector fitting is affixed internally to the patient.

18. The method of claim 11, wherein the fluid is a saline solution.

19. The method of claim 11, wherein the fluid contains an anti-coagulant.

20. A system for cleaning a sensor tip of an implantable electrode sensor having the sensor tip in direct contact with patient fluid, the system comprising:

means for injecting fluid into a first end of a flush sleeve surrounding the sensor; and

means for spraying off the sensor tip with the injected fluid through at least one orifice located at a second end of the flush sleeve.

* * * * *

专利名称(译)	植入式传感器冲洗套管		
公开(公告)号	US20030125613A1	公开(公告)日	2003-07-03
申请号	US10/034740	申请日	2001-12-27
[标]申请(专利权)人(译)	美敦力迷你迈德公司		
申请(专利权)人(译)	MEDTRONIC MINIMED INC.		
[标]发明人	ENEGREN BRADLEY J KOLOPP MARIANNE A		
发明人	ENEGREN, BRADLEY J. KOLOPP, MARIANNE A.		
IPC分类号	A61B5/00 A61B5/05		
CPC分类号	A61B5/14532 A61B5/0031		
其他公开文献	US7018336		
外部链接	Espacenet USPTO		

摘要(译)

用于清洁可植入传感器的传感器尖端的装置和方法包括朝向传感器尖端的冲洗套管，与冲洗套管流体连通的流体导管，其中注入围绕传感器的冲洗套管的第一端的流体喷射传感器尖端穿过位于冲洗套筒第二端的至少一个孔。冲洗套管的第一端包含流体导管和隔膜，其中针用于刺穿隔膜以将流体注入流体导管。

